
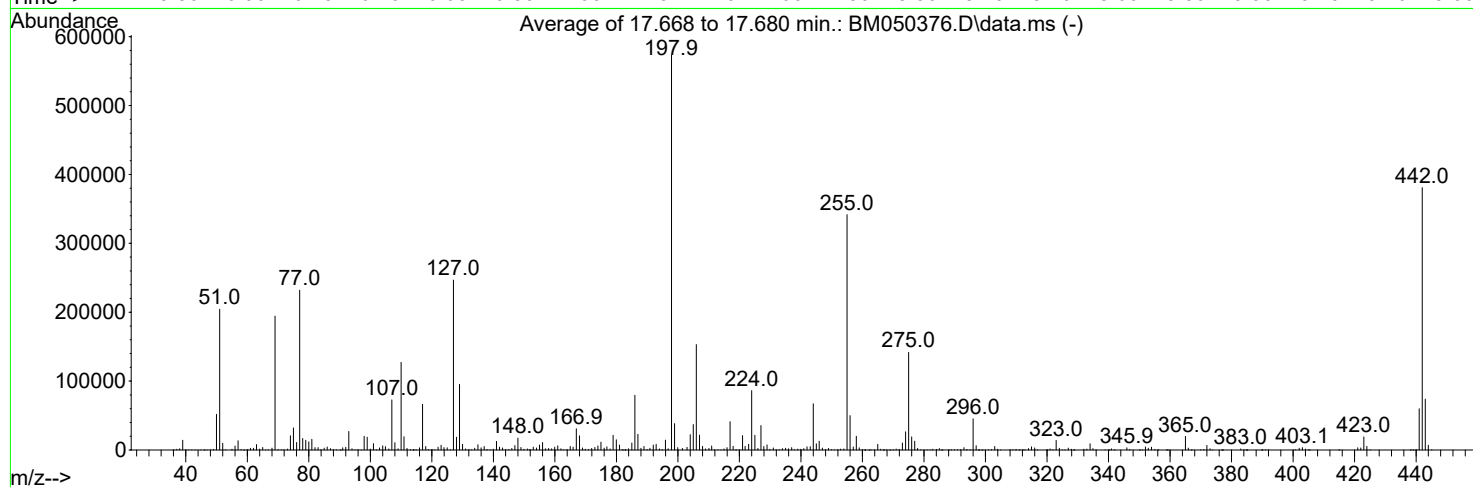


Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM070925\  
 Data File : BM050376.D  
 Acq On : 08 Jul 2025 11:59  
 Operator : RC/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_M  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM070925.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Tue Jul 08 18:32:25 2025

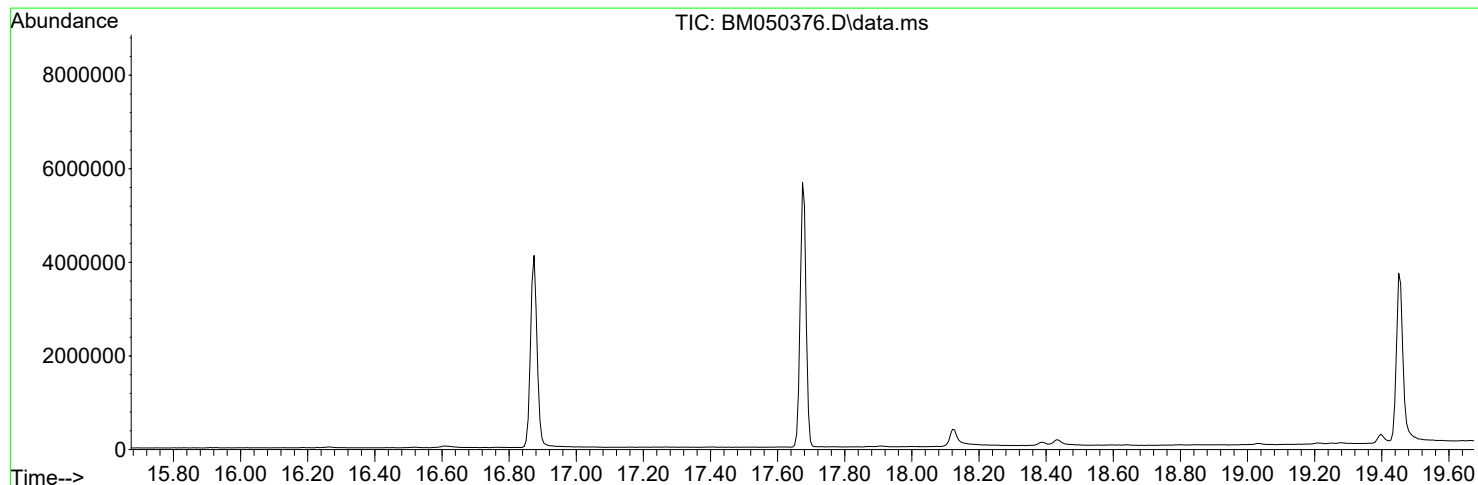

AutoFind: Scans 2496, 2497, 2498; Background Corrected with Scan 2489

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
68	69	0.00	2	1.5	2822	PASS
69	69	100	100	100.0	194463	PASS
70	69	0.00	2	0.5	943	PASS
197	198	0.00	2	0.3	1831	PASS
198	198	100	100	100.0	573141	PASS
199	198	5	9	6.7	38261	PASS
365	198	1	100	3.4	19723	PASS
441	443	0.01	150	81.4	60059	PASS
442	442	100	100	100.0	380992	PASS
443	442	15	24	19.4	73781	PASS

**DDT Breakdown**




Date	Instrument Name	DFTPP Data File
7/9/2025	BNA_M	<u>BM050376.D</u>
Compound Name	Response	Retention Time
DDT	1842274	20.692
DDD	18107	20.309
DDE	1079	19.75
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
19186	1861460	1.03

Instrument :  
 BNA\_M  
 Client:Sampled :  
 DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM070925\  
 Data File : BM050376.D  
 Acq On : 08 Jul 2025 11:59  
 Operator : RC/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_M  
 ClientSampleId :  
 DFTPP

Quant Time: Jul 08 17:14:47 2025  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM070925.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Tue Jul 08 15:59:58 2025  
 Response via : Initial Calibration

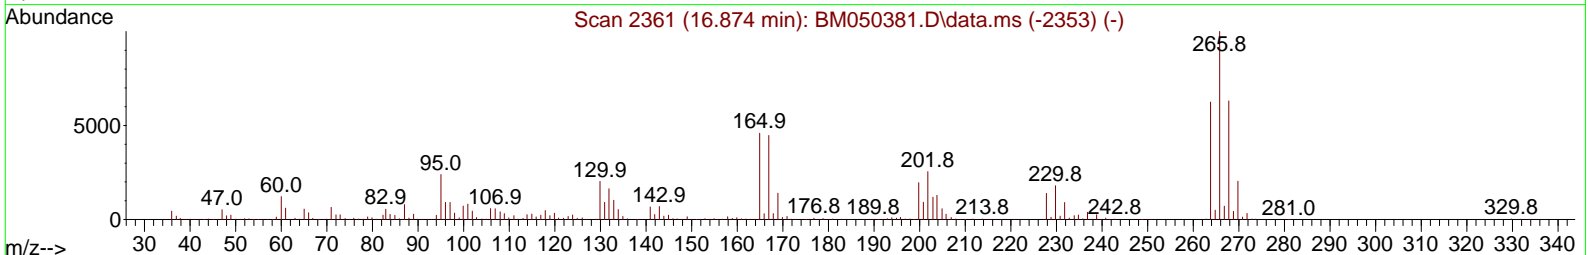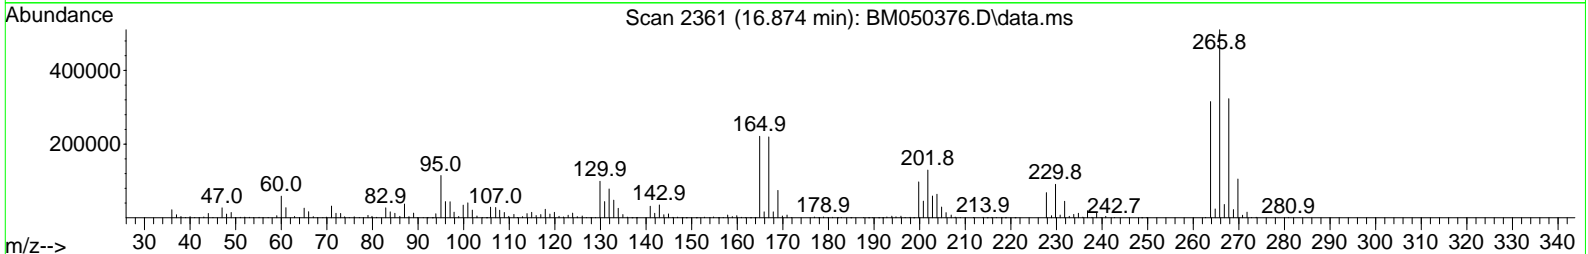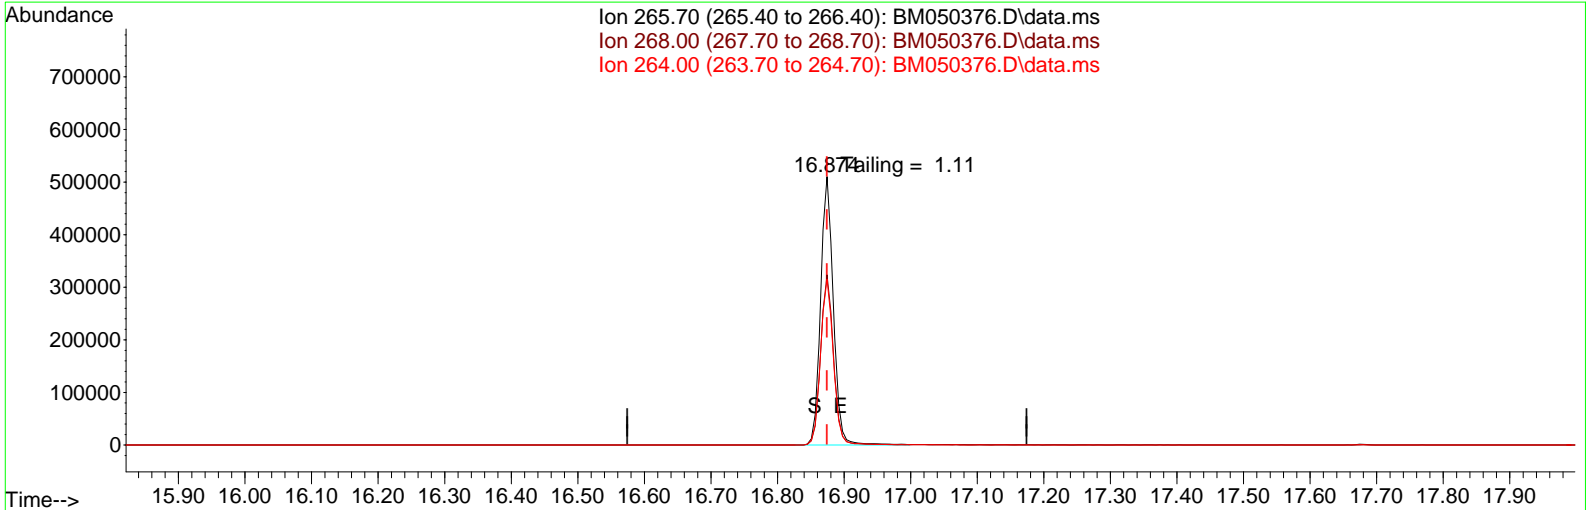

TIC: BM050376.D\data.ms




(70) Pentachlorophenol (C)

16.874min (+ 0.000)	0.00 ng
response	680595
Ion	Exp% Act%
265.70	100.00 100.00
268.00	63.10 63.37
264.00	62.40 61.79
0.00	0.00 0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM070925\  
 Data File : BM050376.D  
 Acq On : 08 Jul 2025 11:59  
 Operator : RC/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

**Instrument :**  
 BNA\_M  
**ClientSampleId :**  
 DFTPP

Quant Time: Jul 08 17:14:47 2025  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM070925.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Tue Jul 08 15:59:58 2025  
 Response via : Initial Calibration

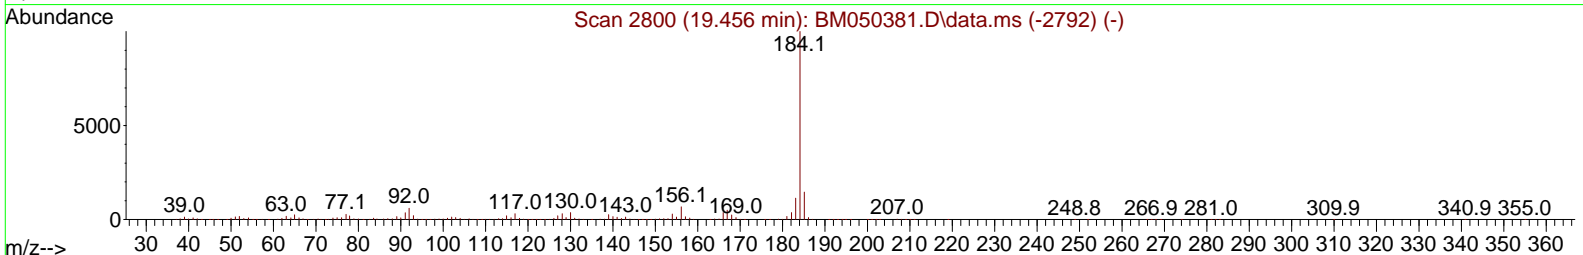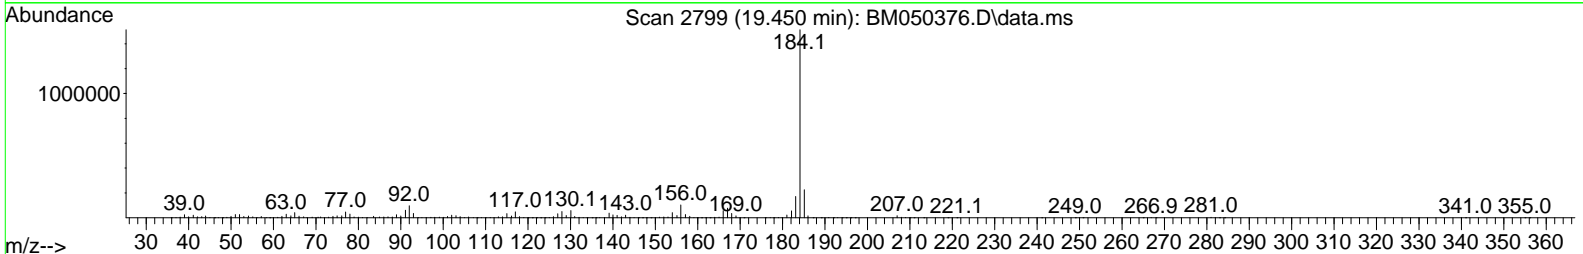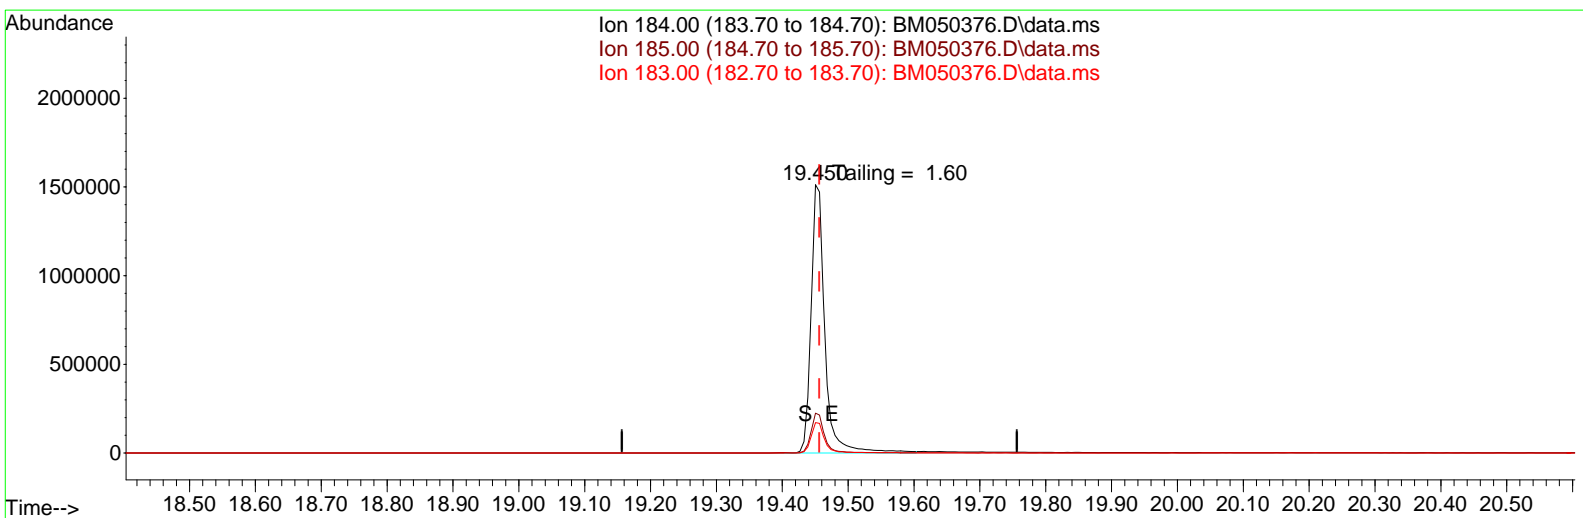

TIC: BM050376.D\data.ms

(77) Benzidine

19.450min (-0.006) 78341.13 ng

response 2201890

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.87
183.00	11.30	11.33
0.00	0.00	0.00