
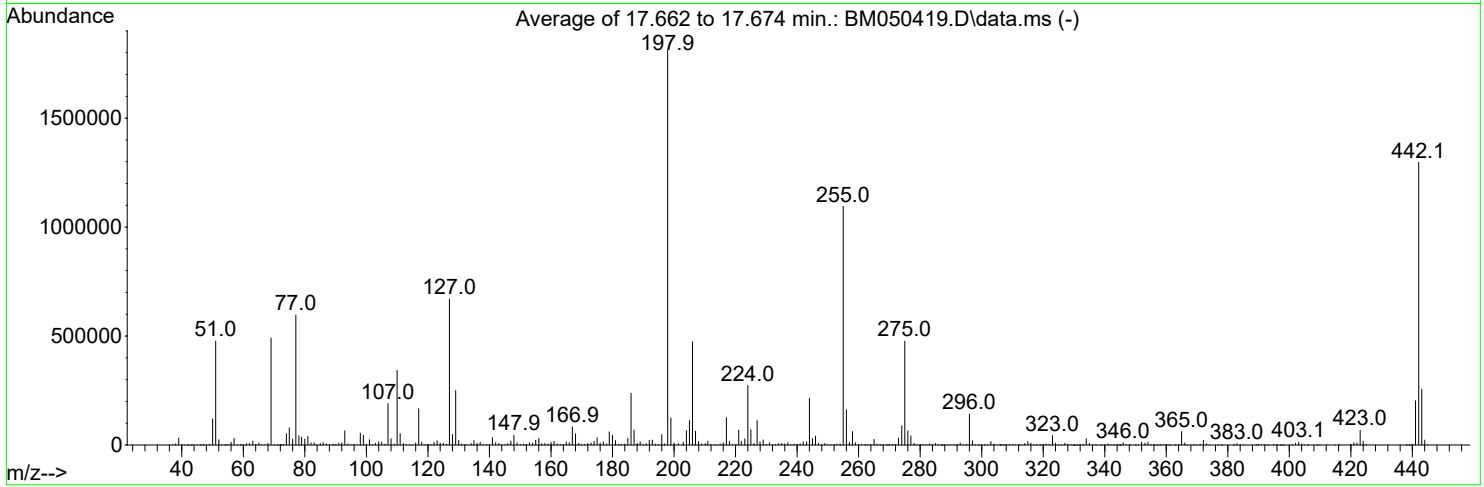


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071425\
 Data File : BM050419.D
 Acq On : 14 Jul 2025 09:30
 Operator : RC/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM070925.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jul 08 18:32:25 2025

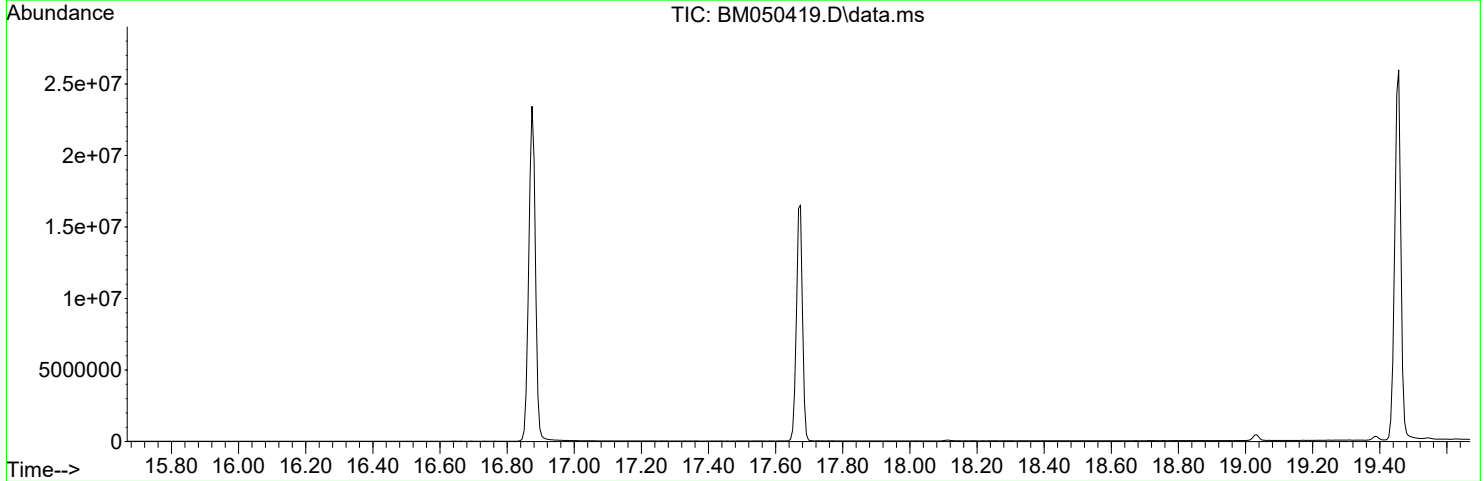

AutoFind: Scans 2495, 2496, 2497; Background Corrected with Scan 2488

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
68	69	0.00	2	1.6	7688	PASS
69	69	100	100	100.0	491019	PASS
70	69	0.00	2	0.5	2482	PASS
197	198	0.00	2	0.3	5418	PASS
198	198	100	100	100.0	1811627	PASS
199	198	5	9	6.9	124381	PASS
365	198	1	100	3.4	61507	PASS
441	443	0.01	150	79.2	203149	PASS
442	442	100	100	100.0	1296320	PASS
443	442	15	24	19.8	256488	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
7/14/2025	BNA_M	<u>BM050419.D</u>
Compound Name	Response	Retention Time
DDT	6931002	20.686
DDD	53917	20.303
DDE	7772	19.75
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
61689	6992691	0.88

Instrument :
 BNA_M
 ClientSampled :
 DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071425\
 Data File : BM050419.D
 Acq On : 14 Jul 2025 09:30
 Operator : RC/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
ClientSampleId :
 DFTPP

Quant Time: Jul 14 11:57:50 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM070925.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jul 08 18:32:25 2025
 Response via : Initial Calibration

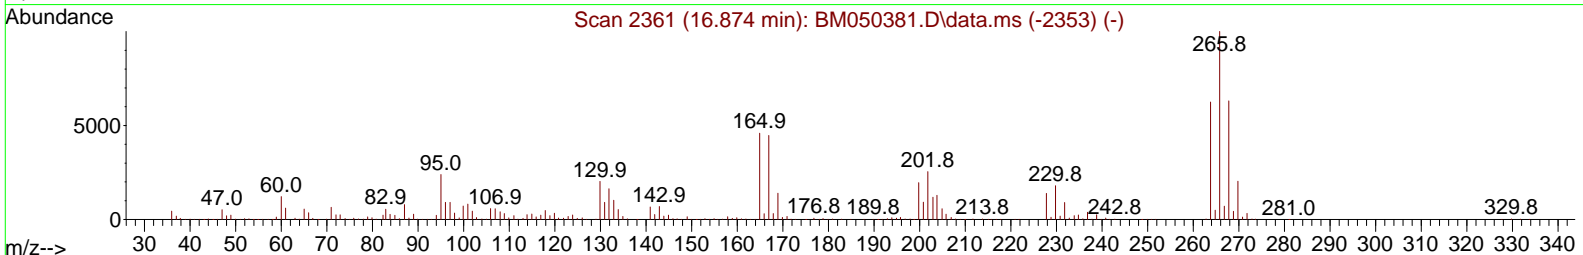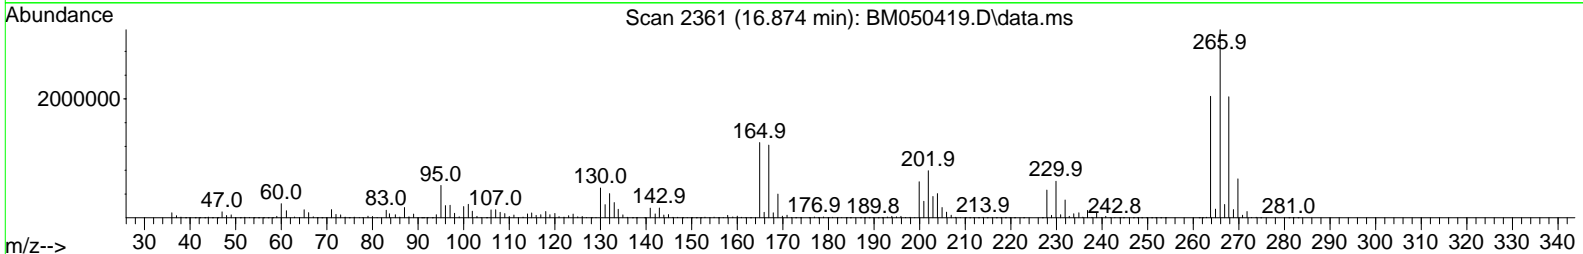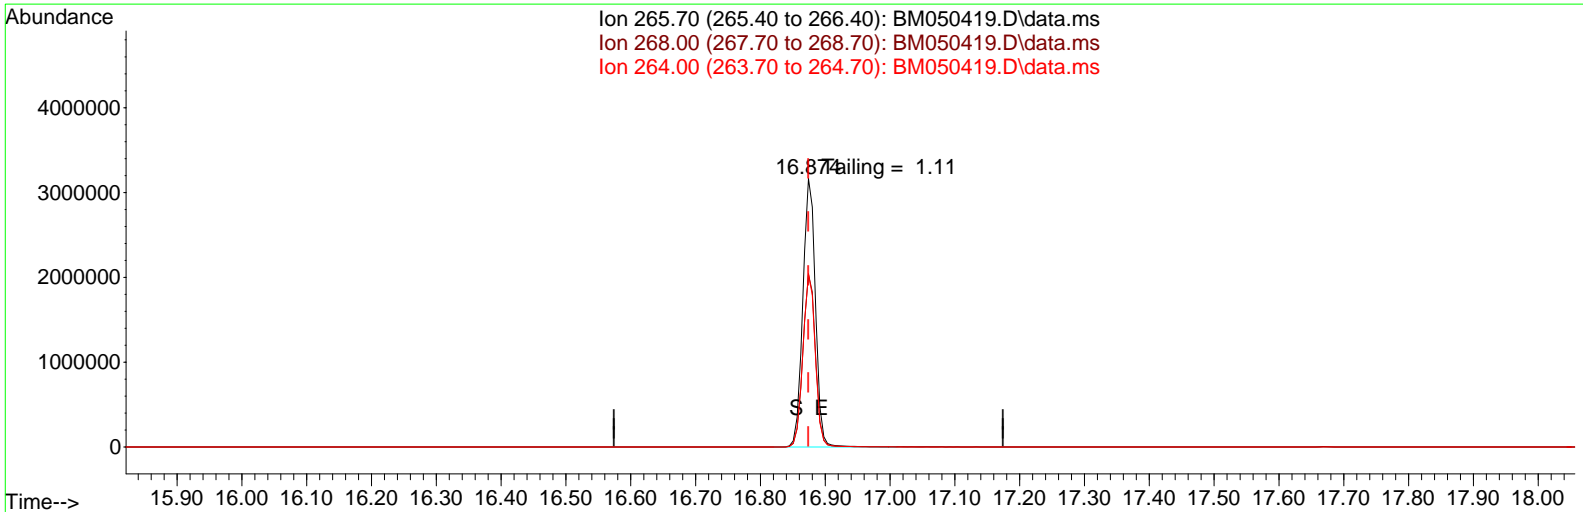

TIC: BM050419.D\data.ms

(70) Pentachlorophenol (C)

16.874min (-0.000) 1727729.72 ng




response 4282661

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	64.32
264.00	62.40	64.56
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071425\
 Data File : BM050419.D
 Acq On : 14 Jul 2025 09:30
 Operator : RC/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
ClientSampleId :
 DFTPP

Quant Time: Jul 14 11:57:50 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM070925.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jul 08 18:32:25 2025
 Response via : Initial Calibration

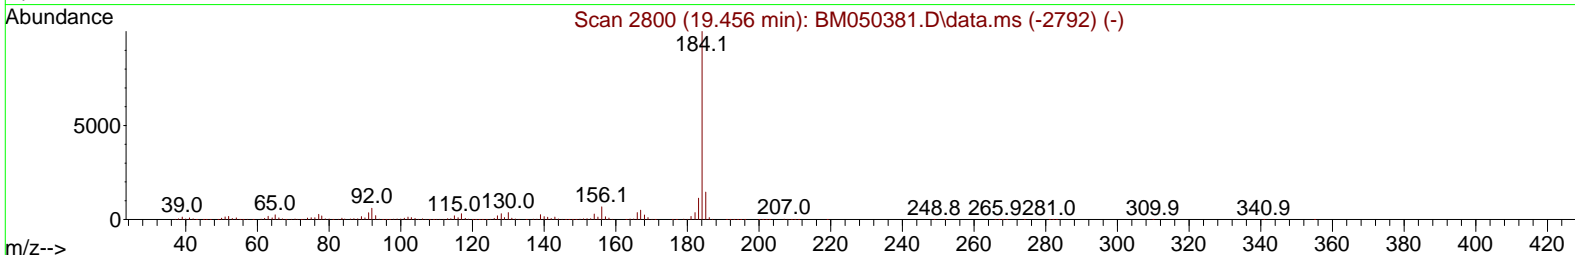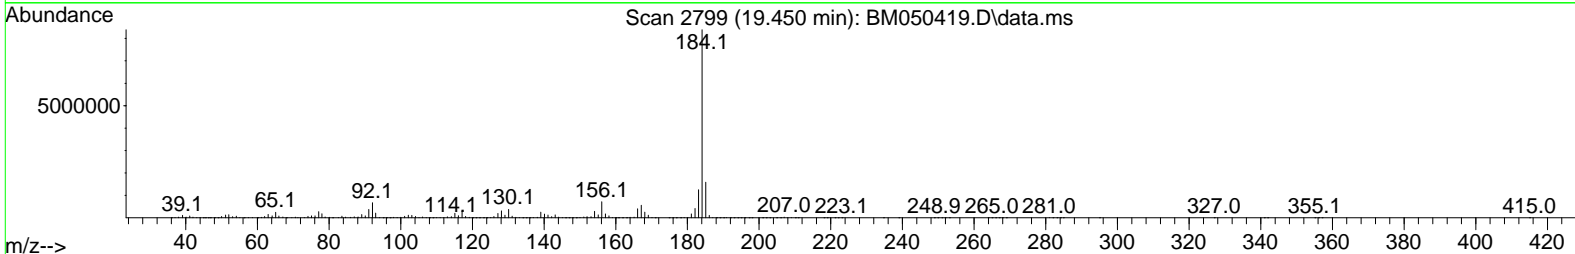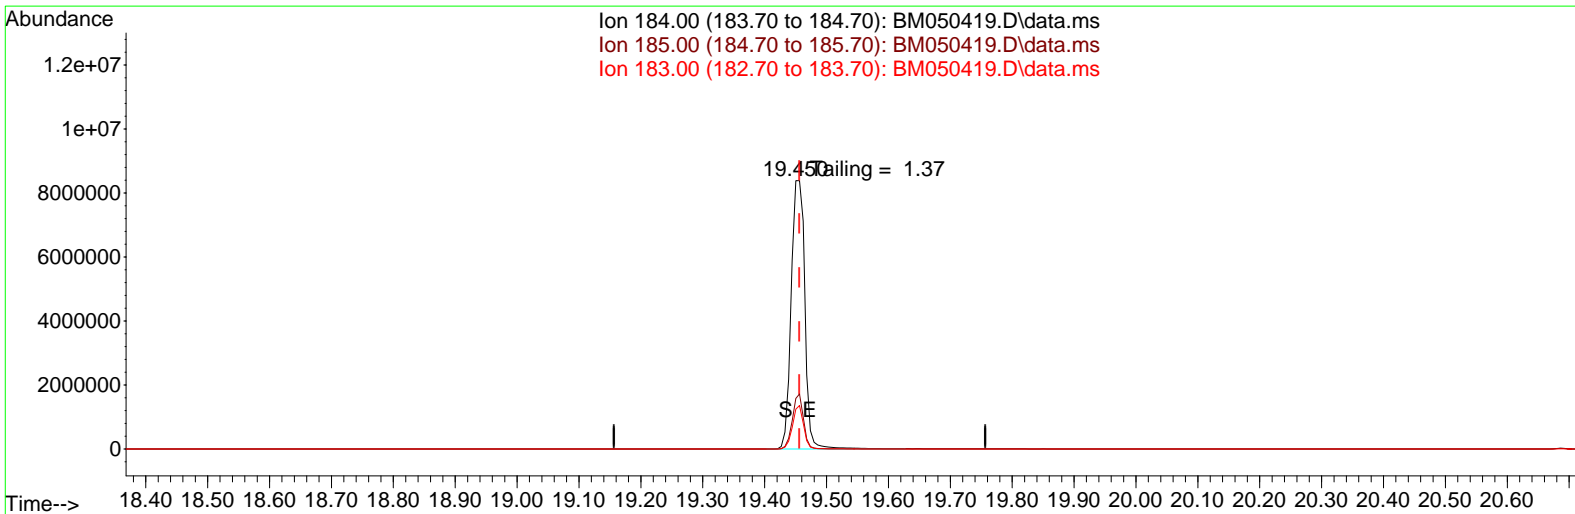

TIC: BM050419.D\data.ms

(77) Benzidine

19.450min (-0.006) 316675.61 ng

response 12931681

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	18.87#
183.00	11.30	14.88#
0.00	0.00	0.00