
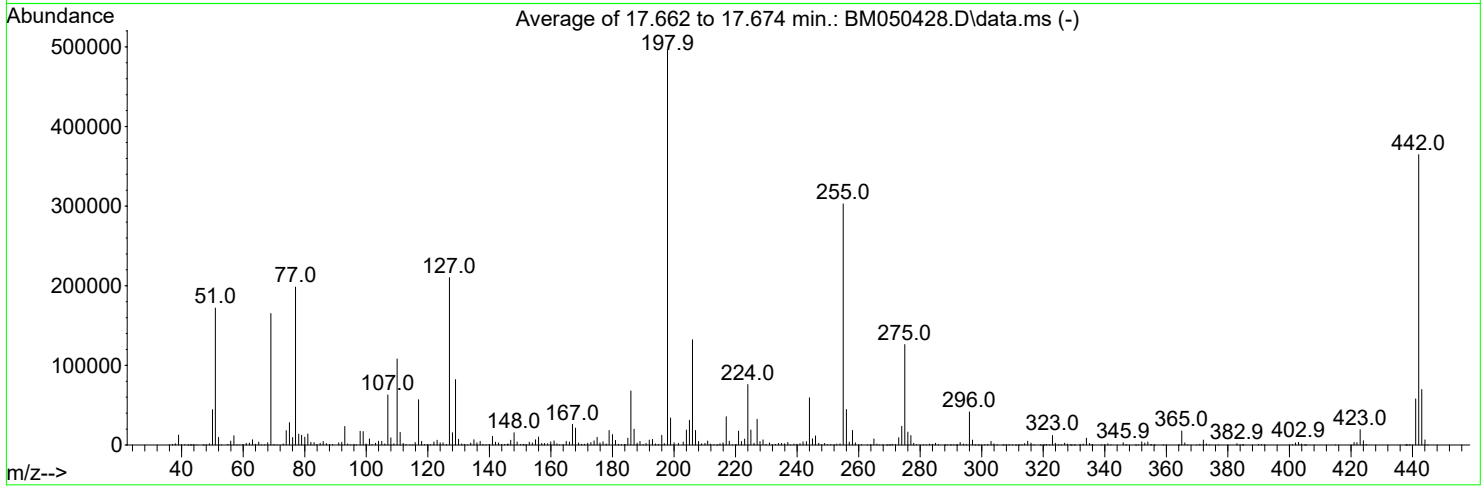


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071425\
 Data File : BM050428.D
 Acq On : 14 Jul 2025 16:13
 Operator : RC/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM070925.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jul 08 18:32:25 2025

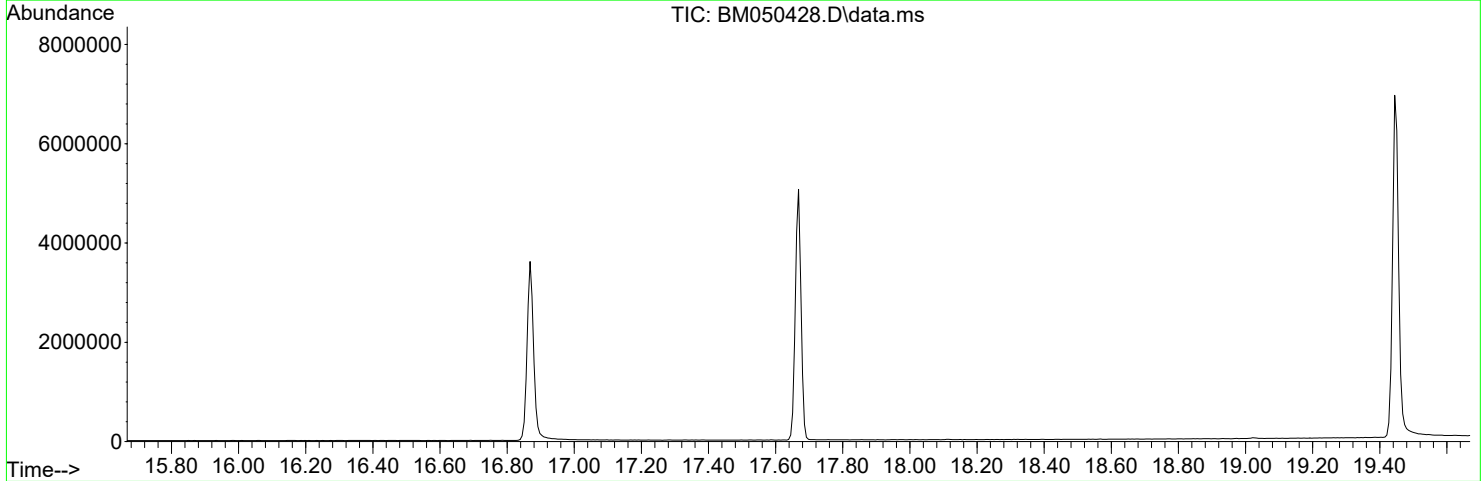

AutoFind: Scans 2495, 2496, 2497; Background Corrected with Scan 2488

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
68	69	0.00	2	1.7	2833	PASS
69	69	100	100	100.0	165195	PASS
70	69	0.00	2	0.5	890	PASS
197	198	0.00	2	0.4	1830	PASS
198	198	100	100	100.0	495893	PASS
199	198	5	9	6.8	33952	PASS
365	198	1	100	3.6	17680	PASS
441	443	0.01	150	83.0	57923	PASS
442	442	100	100	100.0	364821	PASS
443	442	15	24	19.1	69816	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
7/14/2025	BNA_M	<u>BM050428.D</u>
Compound Name	Response	Retention Time
DDT	1716788	20.686
DDD	16726	20.297
DDE	873	19.745
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
17599	1734387	1.01

Instrument :
 BNA_M
 Client:Sampled :
 DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071425\
 Data File : BM050428.D
 Acq On : 14 Jul 2025 16:13
 Operator : RC/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: Jul 14 17:12:51 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM070925.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jul 08 18:32:25 2025
 Response via : Initial Calibration

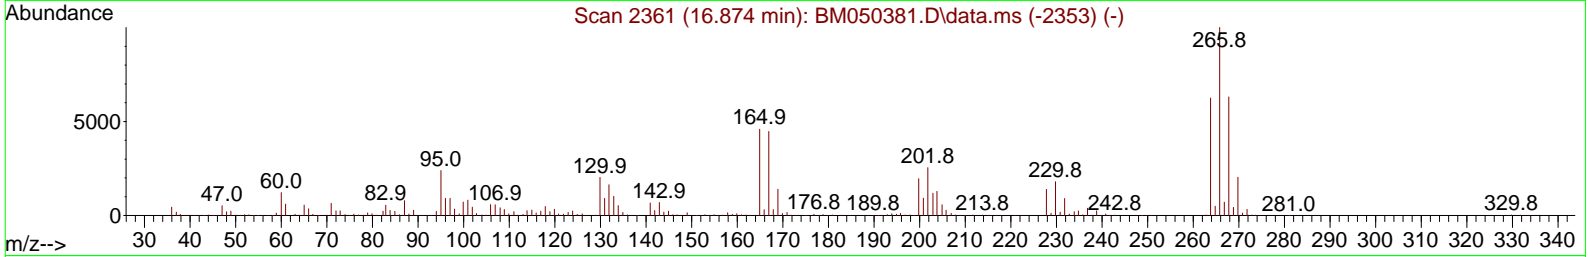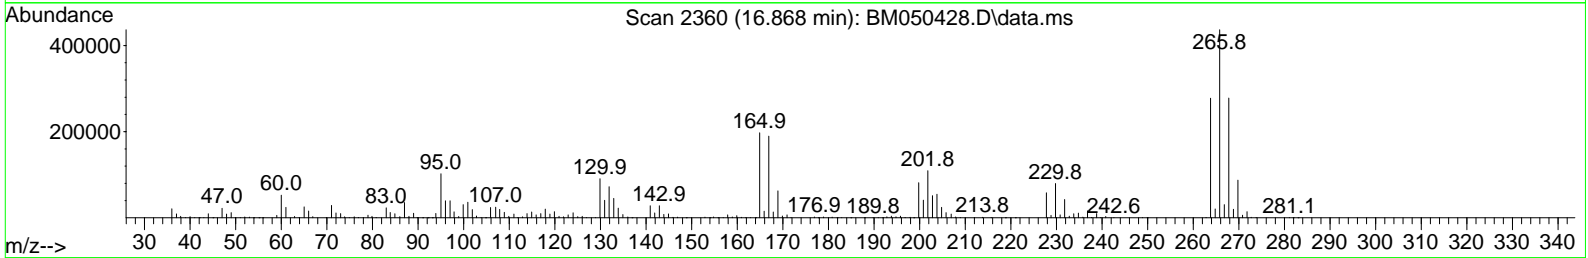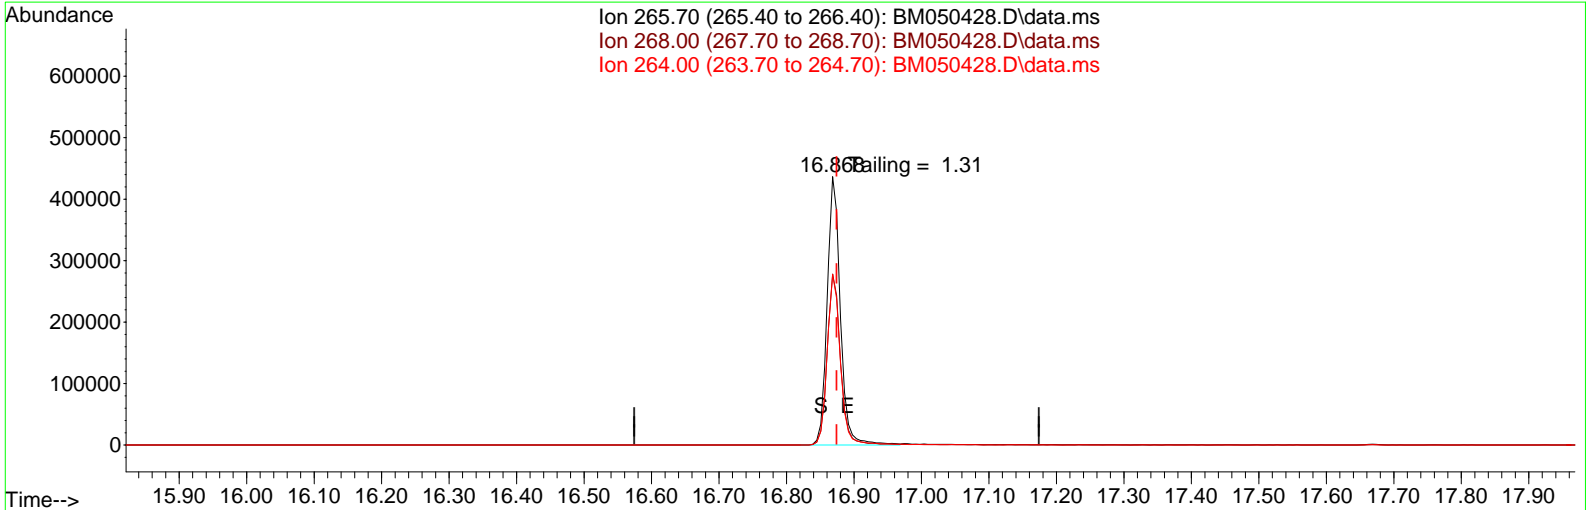

TIC: BM050428.D\data.ms

(70) Pentachlorophenol (C)

16.868min (-0.006) 260244.76 ng




response 592386

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	63.71
264.00	62.40	63.58
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071425\
 Data File : BM050428.D
 Acq On : 14 Jul 2025 16:13
 Operator : RC/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
ClientSampleId :
 DFTPP

Quant Time: Jul 14 17:12:51 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM070925.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jul 08 18:32:25 2025
 Response via : Initial Calibration

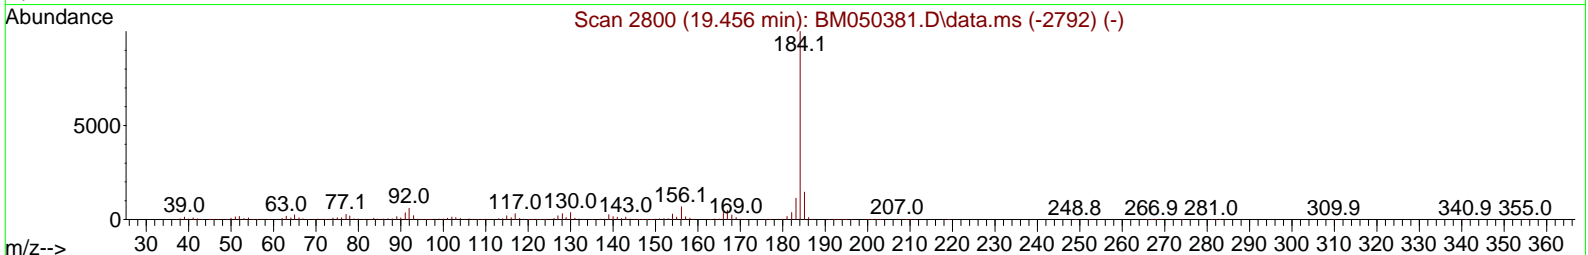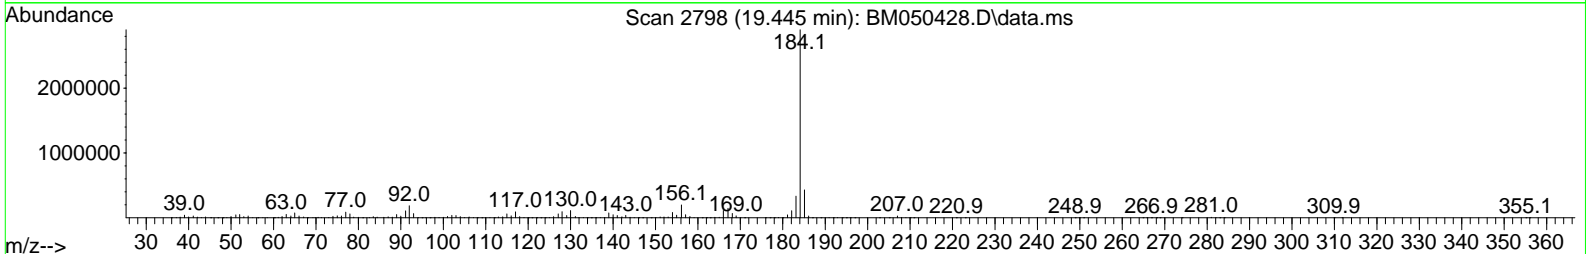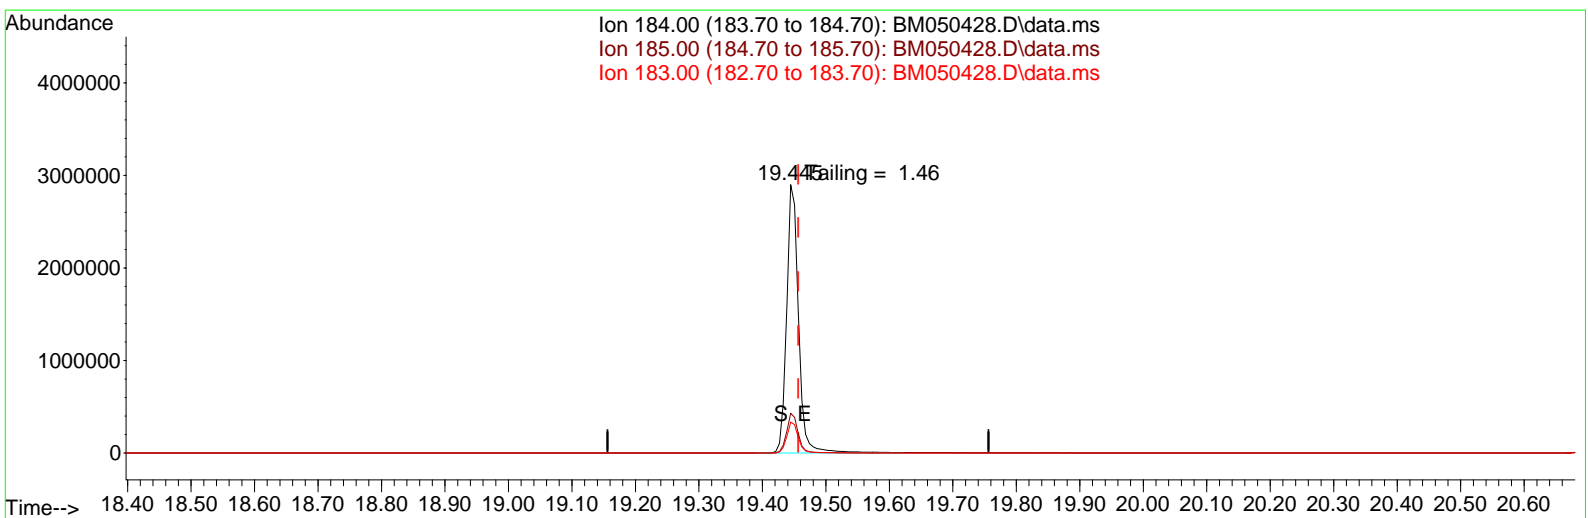

TIC: BM050428.D\data.ms

(77) Benzidine

19.445min (-0.012) 218557.17 ng

response 3796306

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.78
183.00	11.30	11.50
0.00	0.00	0.00