

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX071025\
 Data File : VX046946.D
 Acq On : 10 Jul 2025 15:47
 Operator : JC/MD
 Sample : Q2553-04
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 AOC-205

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X070225W.M
 Title : SW846 8260

Signal : TIC: VX046946.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.270	25	30	39	rBV	31146	87623	3.63%	0.646%
2	5.397	696	707	723	rBV2	252109	790164	32.77%	5.824%
3	5.562	724	734	756	rVB	421601	1285998	53.34%	9.479%
4	5.964	790	800	821	rBV	273697	785269	32.57%	5.788%
5	6.769	922	932	957	rBV	695834	1776844	73.70%	13.097%
6	8.653	1234	1241	1259	rVB	1503633	2410942	100.00%	17.771%
7	10.055	1465	1471	1489	rBV	1537474	2162792	89.71%	15.942%
8	11.079	1634	1639	1655	rBV	1344947	1692445	70.20%	12.475%
9	11.305	1670	1676	1687	rBV	26327	38238	1.59%	0.282%
10	12.018	1788	1793	1801	rBV	1808947	2182634	90.53%	16.088%
11	12.085	1801	1804	1814	rVB2	16419	27591	1.14%	0.203%
12	12.244	1824	1830	1837	rBV2	24836	36658	1.52%	0.270%
13	12.317	1837	1842	1853	rVB5	17002	36797	1.53%	0.271%
14	12.609	1886	1890	1895	rBV	33328	43580	1.81%	0.321%
15	12.695	1900	1904	1913	rVB5	11757	24187	1.00%	0.178%
16	12.920	1934	1941	1945	rBV	24103	33926	1.41%	0.250%
17	13.292	1998	2002	2012	rVB5	28623	41953	1.74%	0.309%
18	14.639	2213	2223	2235	rBV	37427	64036	2.66%	0.472%
19	14.780	2239	2246	2261	rVB2	27637	45355	1.88%	0.334%




Sum of corrected areas: 13567032

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX071025\
Data File : VX046946.D
Acq On : 10 Jul 2025 15:47
Operator : JC/MD
Sample : Q2553-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
AOC-205

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X070225W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

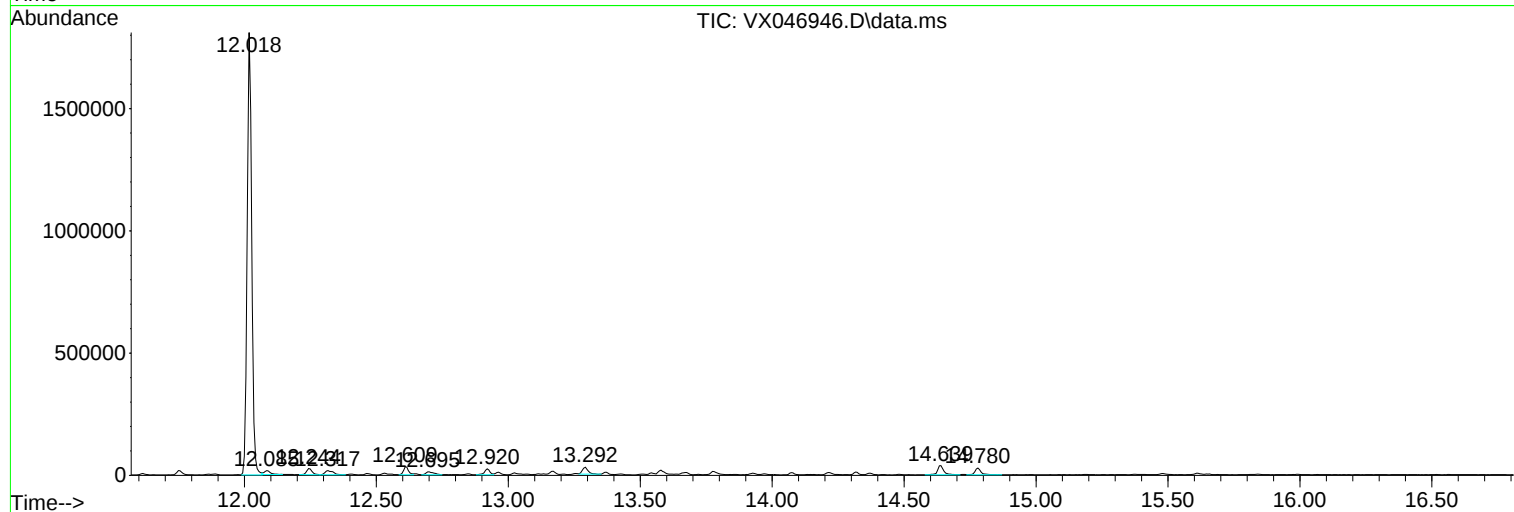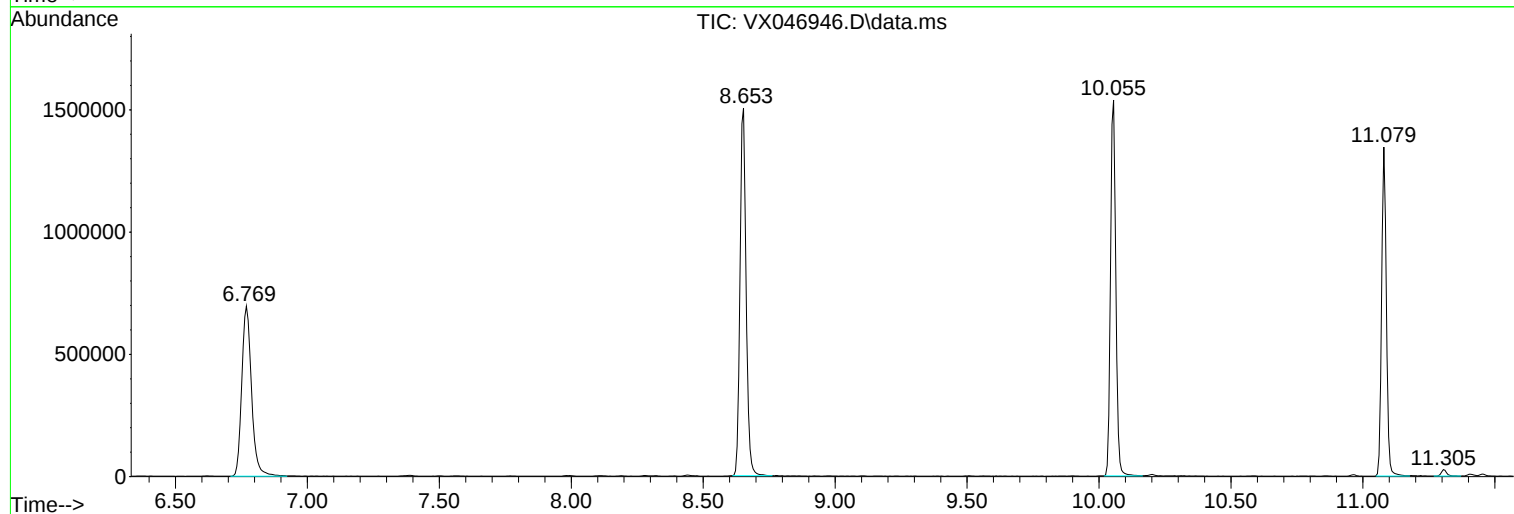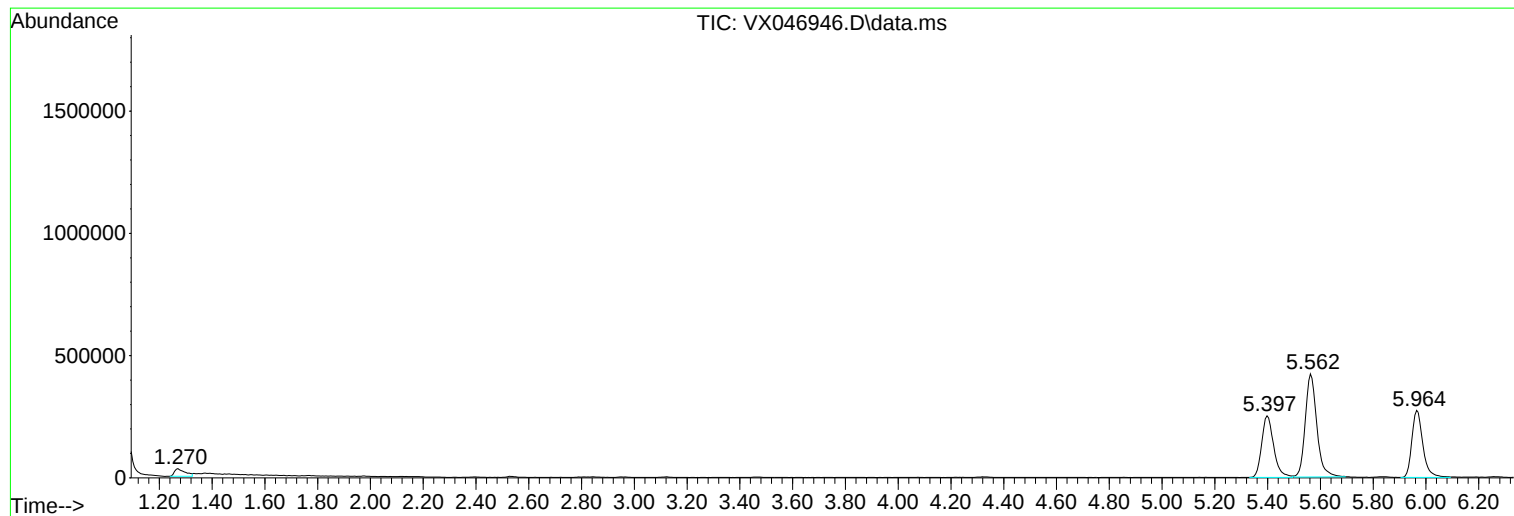

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX071025\
Data File : VX046946.D
Acq On : 10 Jul 2025 15:47
Operator : JC/MD
Sample : Q2553-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
AOC-205

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X070225W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX071025\
Data File : VX046946.D
Acq On : 10 Jul 2025 15:47
Operator : JC/MD
Sample : Q2553-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
AOC-205

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X070225W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc