


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN062525\
Data File : VN087161.D
Acq On : 25 Jun 2025 08:25
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N062525W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Wed Jun 25 10:49:56 2025

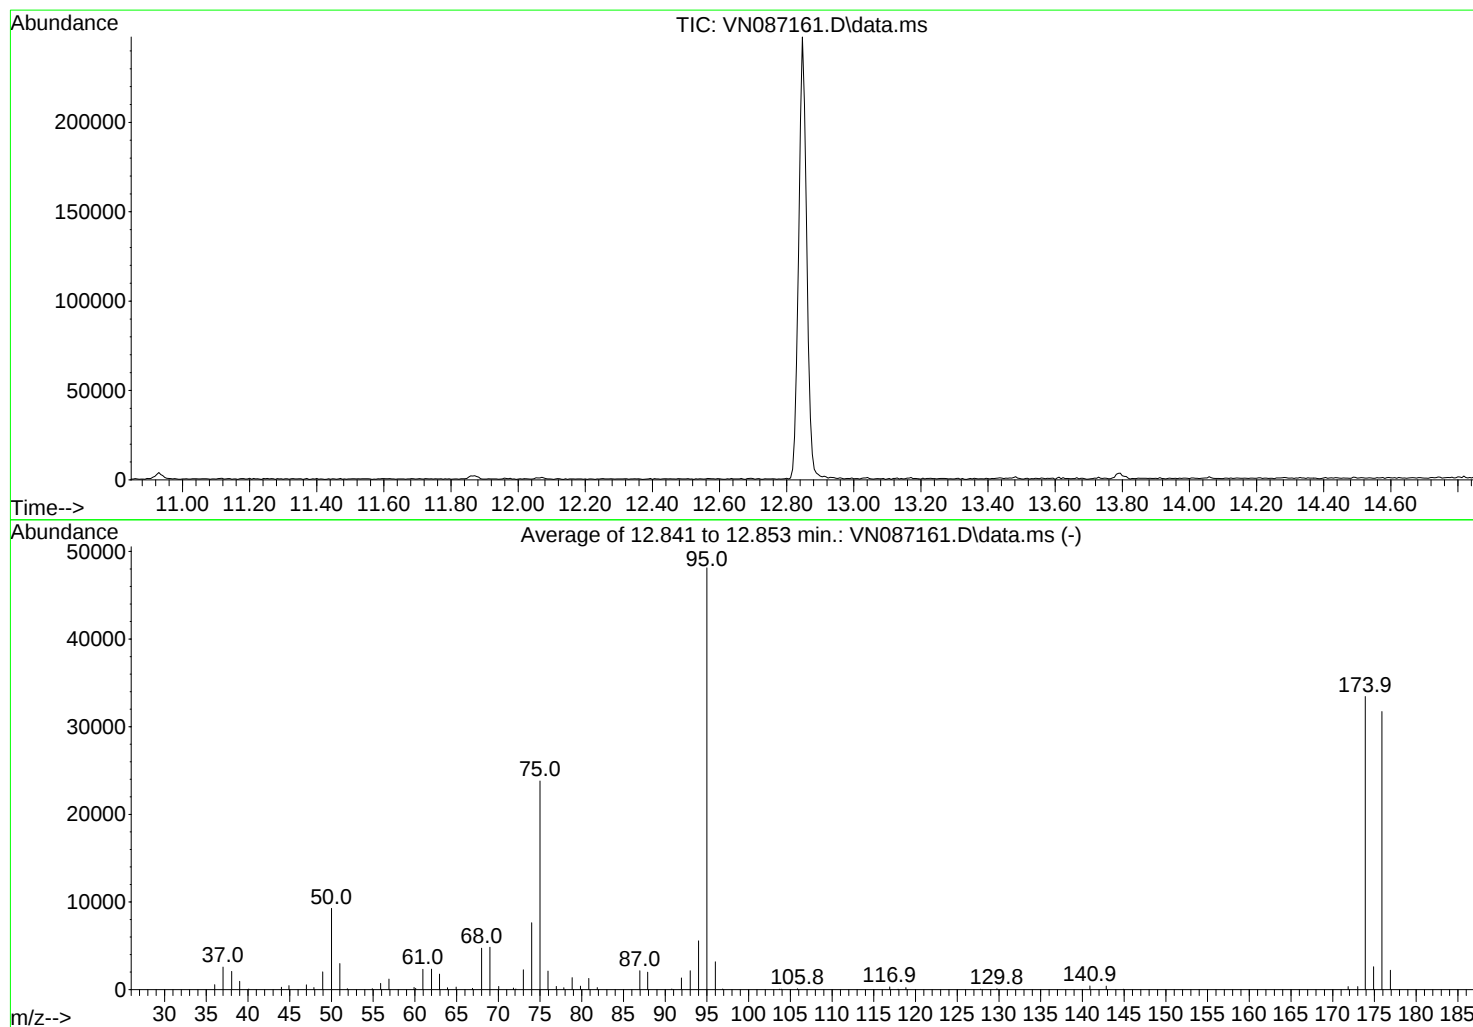

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1844

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.3	9267	PASS
75	95	30	60	49.5	23800	PASS
95	95	100	100	100.0	48128	PASS
96	95	5	9	6.6	3180	PASS
173	174	0.00	2	1.1	357	PASS
174	95	50	100	69.5	33453	PASS
175	174	5	9	7.8	2606	PASS
176	174	95	101	94.8	31725	FAIL*
177	176	5	9	7.0	2211	PASS