

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX071025\
 Data File : VX046950.D
 Acq On : 10 Jul 2025 17:12
 Operator : JC/MD
 Sample : Q2554-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 250709104-01 VOA

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X070225W.M
 Title : SW846 8260

Signal : TIC: VX046950.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.191	15	17	28	rVB	43279	61666	2.01%	0.317%
2	1.374	42	47	55	rVB2	44631	65088	2.12%	0.335%
3	2.148	168	174	186	rBV	87288	152863	4.99%	0.787%
4	2.404	209	216	233	rBV2	40984	90601	2.96%	0.466%
5	2.953	299	306	321	rBV	69758	171010	5.58%	0.880%
6	4.562	557	570	586	rBV2	113432	425278	13.87%	2.189%
7	5.013	634	644	669	rBV	215342	754881	24.63%	3.886%
8	5.398	694	707	724	rBV3	268465	854514	27.88%	4.399%
9	5.562	724	734	758	rVB	439803	1357823	44.30%	6.990%
10	5.964	790	800	809	rBV	299701	823470	26.86%	4.239%
11	6.769	922	932	953	rBV	732261	1865061	60.84%	9.601%
12	8.647	1233	1240	1249	rBV	1526348	2552664	83.28%	13.141%
13	8.720	1249	1252	1261	rVV2	30897	60003	1.96%	0.309%
14	9.379	1354	1360	1367	rBV	27460	42757	1.39%	0.220%
15	9.494	1374	1379	1385	rBV	22848	35692	1.16%	0.184%
16	10.055	1462	1471	1486	rBV2	1658375	3065320	100.00%	15.781%
17	10.195	1489	1494	1500	rBV	121665	174238	5.68%	0.897%
18	10.299	1506	1511	1520	rVB	135868	202934	6.62%	1.045%
19	10.640	1563	1567	1576	rVB	113767	151851	4.95%	0.782%
20	10.964	1614	1620	1625	rBV	67016	88529	2.89%	0.456%
21	11.079	1634	1639	1646	rBV	1387369	1768345	57.69%	9.104%
22	11.305	1668	1676	1682	rBV	45138	70999	2.32%	0.366%
23	11.366	1682	1686	1696	rVV2	27637	67040	2.19%	0.345%
24	11.610	1722	1726	1737	rVB	74951	107068	3.49%	0.551%
25	11.750	1738	1749	1754	rBV	84852	122094	3.98%	0.629%
26	11.884	1765	1771	1779	rVB	63912	88424	2.88%	0.455%
27	12.018	1787	1793	1801	rBV2	1872143	2689347	87.73%	13.845%
28	12.085	1801	1804	1809	rVB	49020	64570	2.11%	0.332%
29	12.244	1824	1830	1835	rBV2	130354	182732	5.96%	0.941%
30	12.335	1839	1845	1851	rVB5	31921	65613	2.14%	0.338%
31	12.408	1853	1857	1863	rBV7	18557	36709	1.20%	0.189%
32	12.530	1872	1877	1886	rVB4	17199	40289	1.31%	0.207%
33	12.610	1886	1890	1894	rBV	44191	53439	1.74%	0.275%
34	12.695	1901	1904	1912	rVB2	21289	35916	1.17%	0.185%
35	12.902	1934	1938	1944	rVV2	42155	92330	3.01%	0.475%
36	12.963	1944	1948	1953	rVB4	21723	32269	1.05%	0.166%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX071025\
Data File : VX046950.D
Acq On : 10 Jul 2025 17:12
Operator : JC/MD
Sample : Q2554-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
250709104-01 VOA

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X070225W.M

Title : SW846 8260

37	13.286	1996	2001	2006	rBV2	52717	74505	2.43%	0.384%
38	13.420	2018	2023	2027	rBV4	27806	38211	1.25%	0.197%
39	13.469	2027	2031	2034	rVV2	35888	48417	1.58%	0.249%
40	13.512	2034	2038	2045	rVB4	33696	55310	1.80%	0.285%
41	13.774	2075	2081	2089	rBV	396814	498105	16.25%	2.564%
42	13.926	2102	2106	2121	rVB	16226	42540	1.39%	0.219%
43	14.640	2219	2223	2225	rBV	29036	38700	1.26%	0.199%
44	14.780	2241	2246	2256	rVB	49545	72976	2.38%	0.376%
45	16.322	2492	2499	2510	rVB3	21073	42525	1.39%	0.219%




Sum of corrected areas: 19424716

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX071025\
Data File : VX046950.D
Acq On : 10 Jul 2025 17:12
Operator : JC/MD
Sample : Q2554-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
250709104-01 VOA

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X070225W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

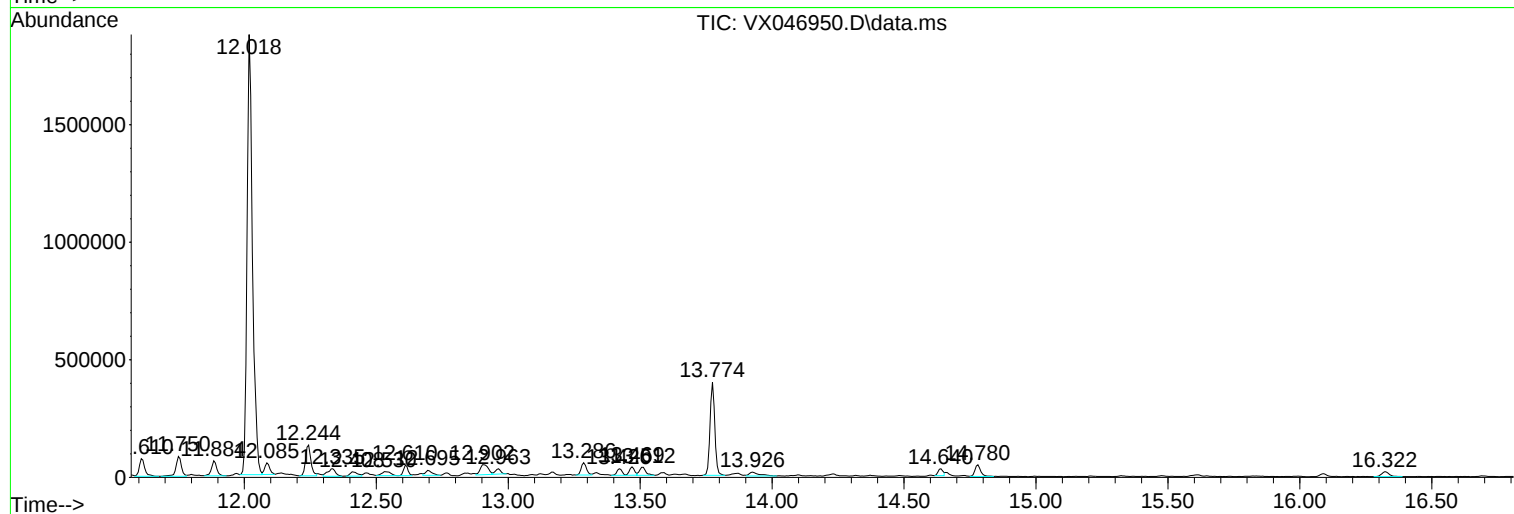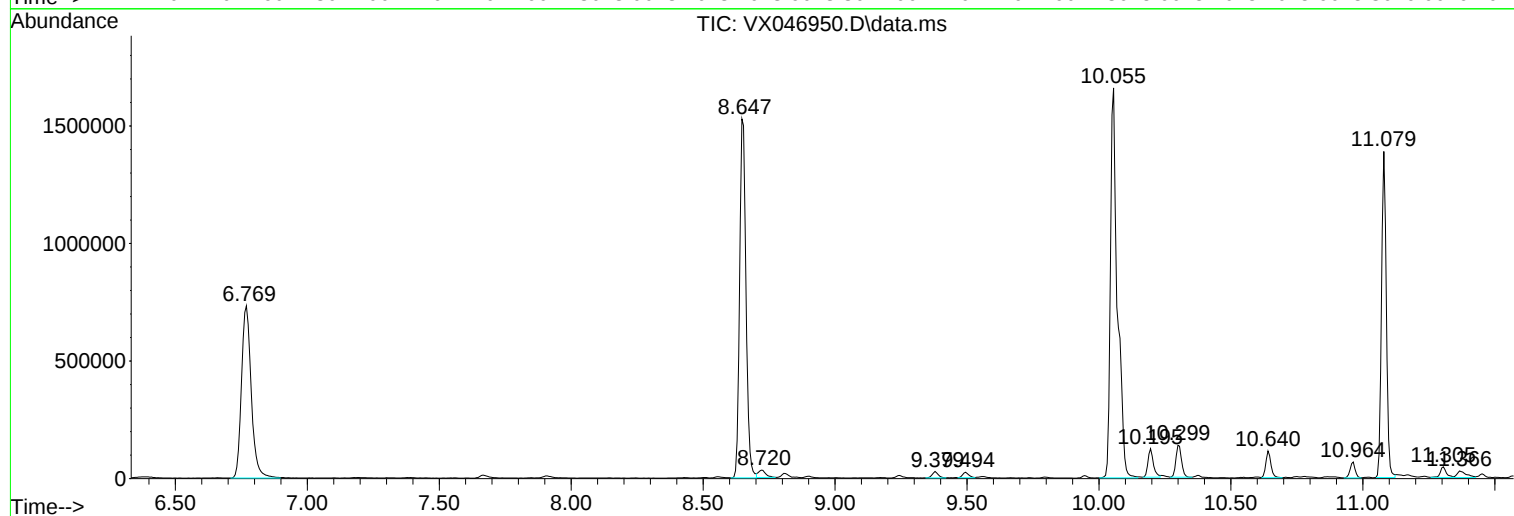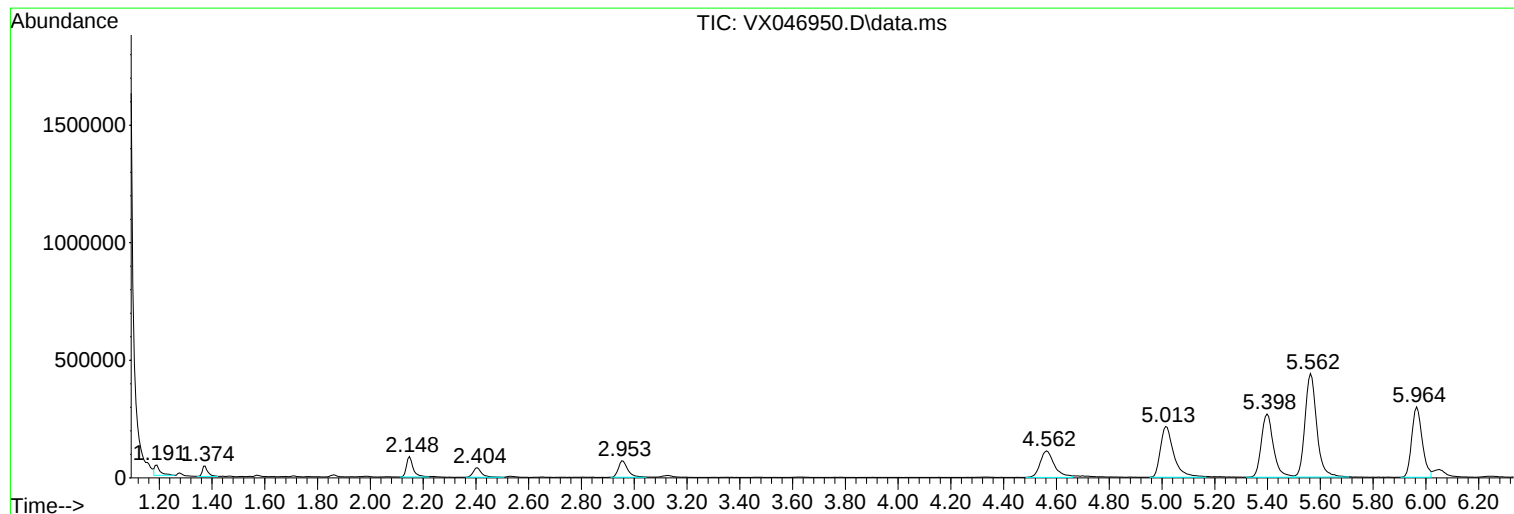

Library Search Compound Report

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX071025\
Data File : VX046950.D
Acq On : 10 Jul 2025 17:12
Operator : JC/MD
Sample : Q2554-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
250709104-01 VOA

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X070225W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX071025\
Data File : VX046950.D
Acq On : 10 Jul 2025 17:12
Operator : JC/MD
Sample : Q2554-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
250709104-01 VOA

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X070225W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc