


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071725\
Data File : BF143138.D
Acq On : 17 Jul 2025 09:58
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF071725.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Jul 17 15:14:05 2025

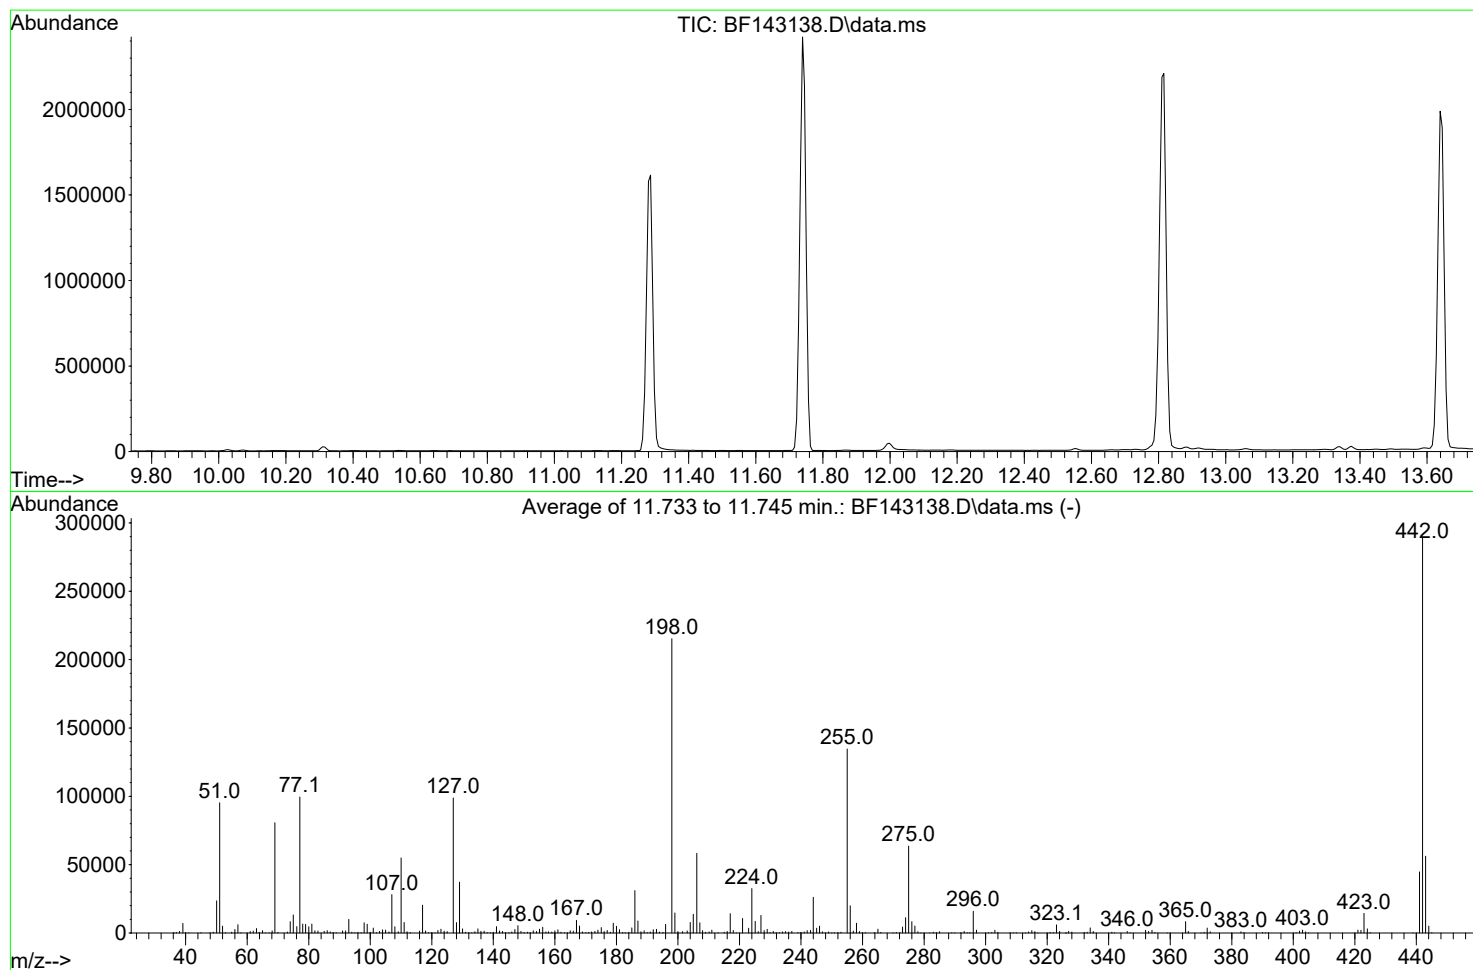

AutoFind: Scans 1622, 1623, 1624; Background Corrected with Scan 1616

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
68	69	0.00	2	1.9	1515	PASS
69	69	100	100	100.0	80680	PASS
70	69	0.00	2	0.5	430	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	215296	PASS
199	198	5	9	6.8	14617	PASS
365	198	1	100	3.8	8287	PASS
441	443	0.01	150	79.6	44723	PASS
442	442	100	100	100.0	288853	PASS
443	442	15	24	19.5	56203	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
7/17/2025	BNA_F	<u>BF143138.D</u>
Compound Name	Response	Retention Time
DDT	490244	13.639
DDD	9488	13.339
DDE	328	13.004
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
9816	500060	1.96

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071725\
Data File : BF143138.D
Acq On : 17 Jul 2025 09:58
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jul 17 16:32:18 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF071725.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 17 15:14:05 2025
Response via : Initial Calibration

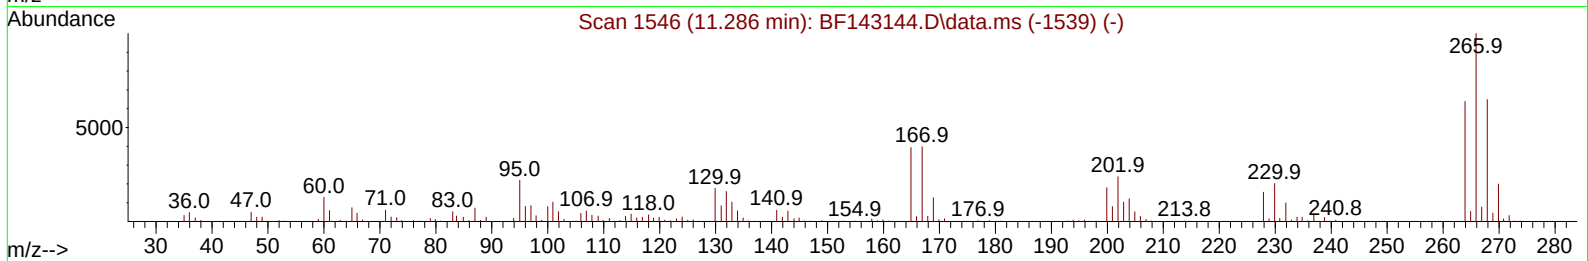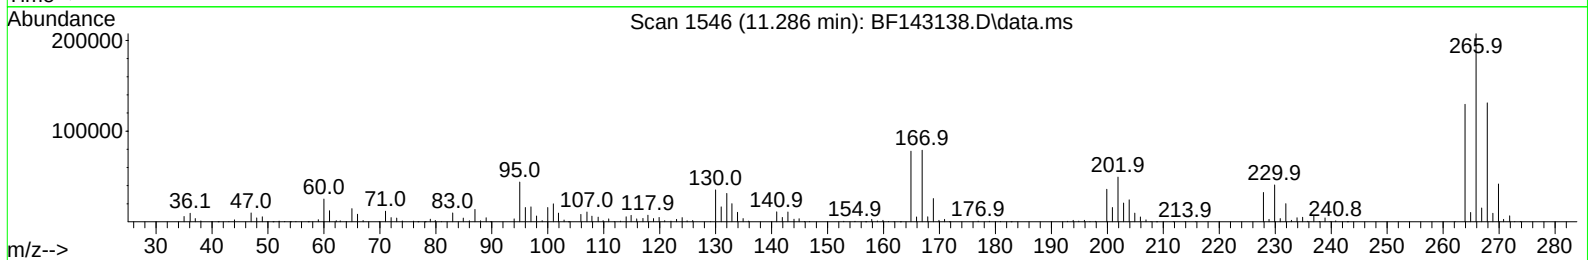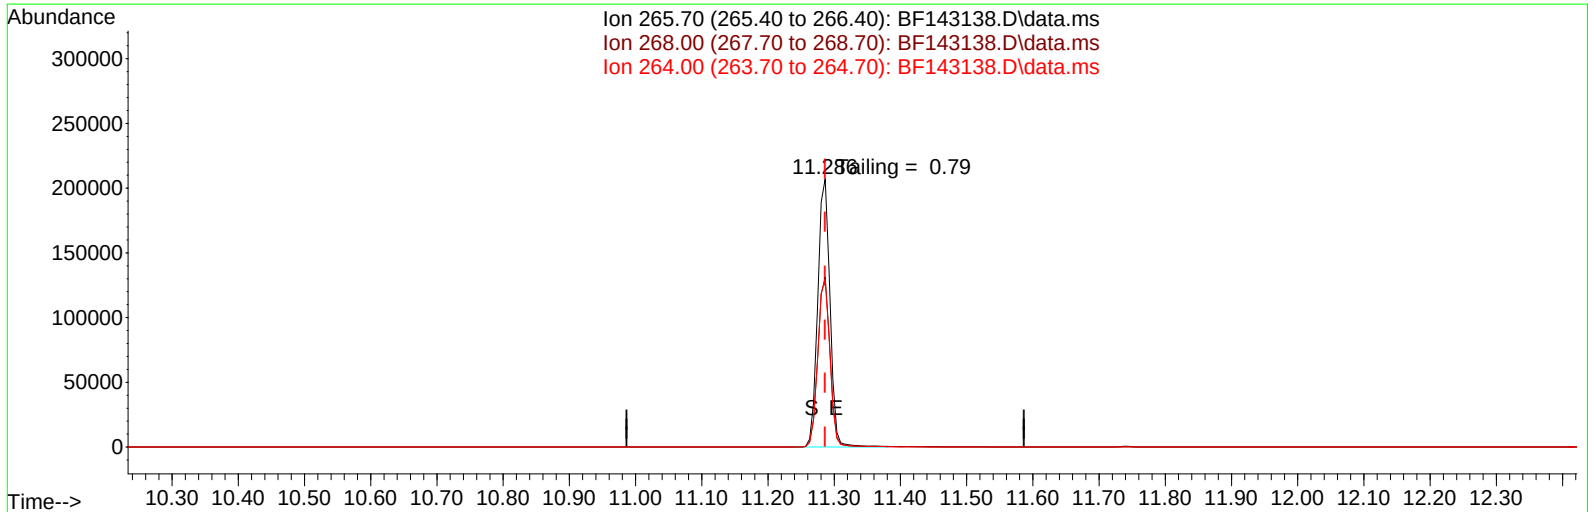

TIC: BF143138.D\data.ms

(70) Pentachlorophenol (C)

11.286min (+ 0.000) 29509.64 ng




response 268044

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.90	63.24
264.00	63.80	62.50
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071725\
Data File : BF143138.D
Acq On : 17 Jul 2025 09:58
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jul 17 16:32:18 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF071725.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 17 15:14:05 2025
Response via : Initial Calibration

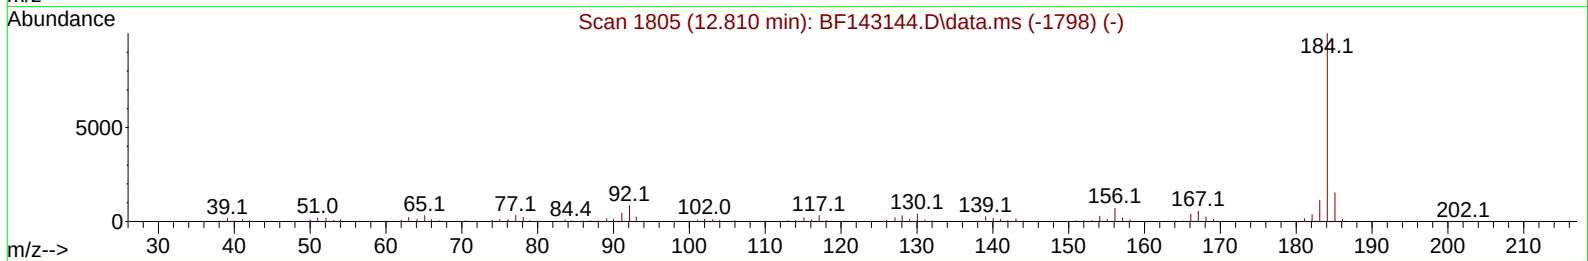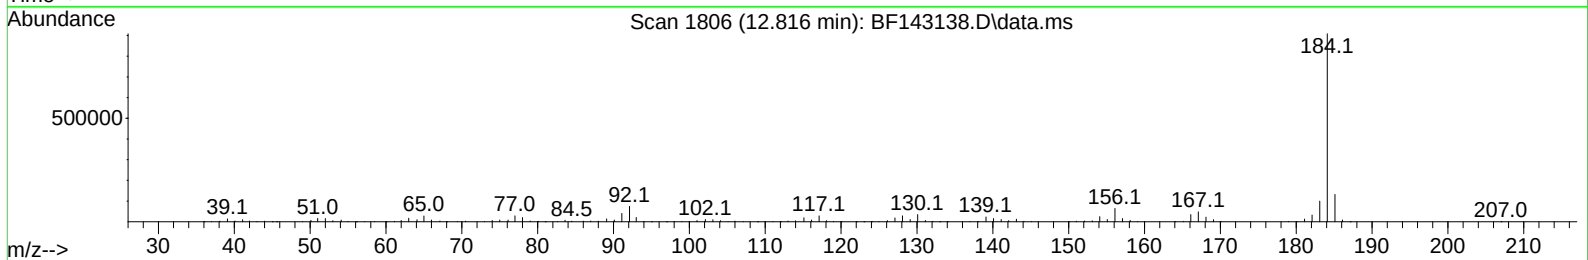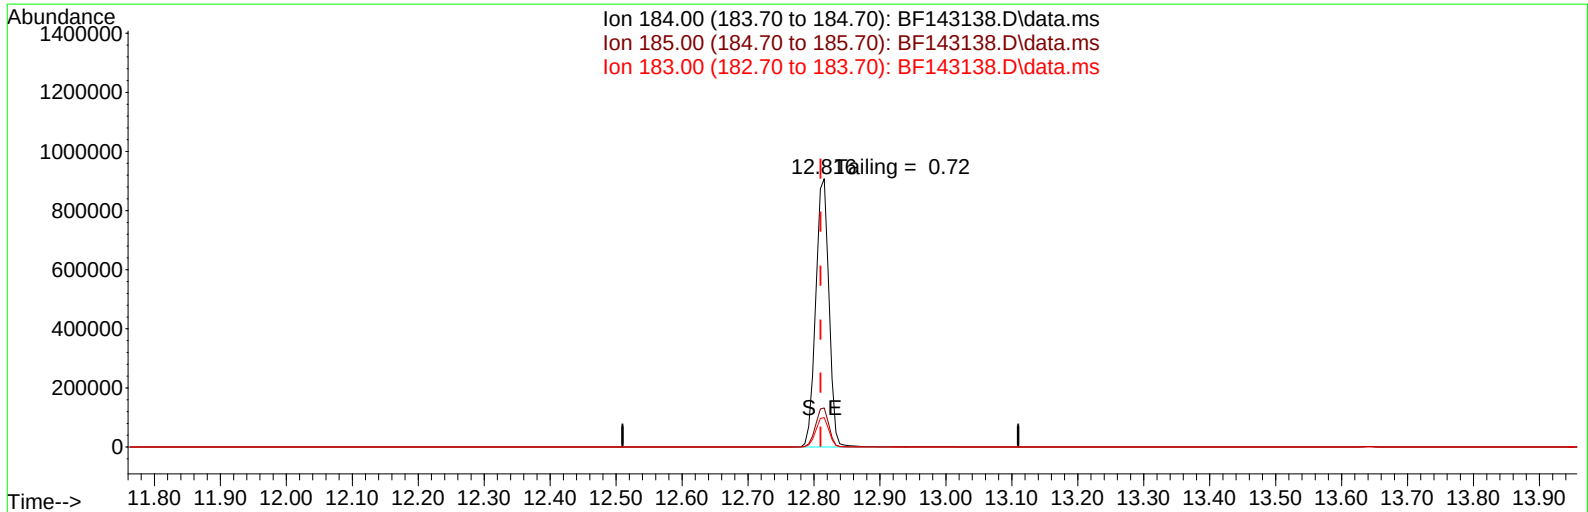

TIC: BF143138.D\data.ms

(77) Benzidine

12.816min (+ 0.006) 0.00 ng

response 1266864

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.30	14.57
183.00	11.20	10.98
0.00	0.00	0.00