

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071625\
 Data File : BF143135.D
 Acq On : 17 Jul 2025 04:31
 Operator : RC/JU
 Sample : Q2555-03
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 OU4-TS-30-070925

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF071525.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF143135.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.328	15	23	34	rVB	369168	585955	17.14%	1.553%
2	5.198	504	511	524	rVB	185715	270581	7.91%	0.717%
3	5.592	569	578	594	rBV	1764512	2292182	67.05%	6.075%
4	6.581	738	746	758	rVB	1773651	2384728	69.76%	6.320%
5	6.969	803	812	817	rBV	701966	879225	25.72%	2.330%
6	7.522	897	906	916	rBV	1160300	1521164	44.50%	4.032%
7	8.245	1022	1029	1037	rVB	861045	1060852	31.03%	2.812%
8	9.322	1201	1212	1219	rBV	1904204	2400922	70.23%	6.363%
9	10.004	1322	1328	1339	rVB	732269	955248	27.94%	2.532%
10	10.710	1440	1448	1455	rBV	274330	346028	10.12%	0.917%
11	10.786	1455	1461	1468	rBV	794501	999912	29.25%	2.650%
12	11.486	1575	1580	1587	rBV	642637	826205	24.17%	2.190%
13	12.010	1660	1669	1681	rBV3	167013	345708	10.11%	0.916%
14	12.698	1782	1786	1791	rBV	90154	131632	3.85%	0.349%
15	12.927	1820	1825	1839	rVB	88181	165238	4.83%	0.438%
16	13.068	1843	1849	1857	rBV	1418516	1857133	54.32%	4.922%
17	13.510	1920	1924	1934	rVB4	91695	196099	5.74%	0.520%
18	13.968	1997	2002	2012	rBV2	239522	398115	11.65%	1.055%
19	14.127	2023	2029	2040	rVB	677956	1053907	30.83%	2.793%
20	14.598	2104	2109	2117	rBV	391173	589113	17.23%	1.561%
21	14.998	2173	2177	2184	rVB	260458	410211	12.00%	1.087%
22	15.274	2219	2224	2234	rVB	1035213	1619407	47.37%	4.292%
23	15.633	2280	2285	2290	rBV	383196	598516	17.51%	1.586%
24	16.021	2346	2351	2363	rVB	132290	264291	7.73%	0.700%
25	16.145	2365	2372	2378	rBV	620598	1142509	33.42%	3.028%
26	16.421	2412	2419	2433	rVB4	208246	545570	15.96%	1.446%
27	17.392	2580	2584	2589	rBV7	53858	112282	3.28%	0.298%
28	17.580	2609	2616	2628	rVB5	243396	616383	18.03%	1.634%
29	17.839	2651	2660	2664	rBV	777222	2127355	62.23%	5.638%
30	17.886	2665	2668	2686	rVB2	839126	2367732	69.26%	6.275%
31	18.074	2693	2700	2708	rVB2	296396	766078	22.41%	2.030%
32	18.186	2715	2719	2724	rBV3	76593	172230	5.04%	0.456%
33	18.333	2735	2744	2757	rBV	748042	2456439	71.85%	6.510%
34	18.445	2758	2763	2774	rVB4	385564	1178850	34.48%	3.124%
35	18.703	2797	2807	2826	rBV4	755232	3418665	100.00%	9.060%
36	18.862	2827	2834	2841	rBV2	267761	675113	19.75%	1.789%

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071625\
Data File : BF143135.D
Acq On : 17 Jul 2025 04:31
Operator : RC/JU
Sample : Q2555-03
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-TS-30-070925

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF071525.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION




Sum of corrected areas: 37731578

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071625\
Data File : BF143135.D
Acq On : 17 Jul 2025 04:31
Operator : RC/JU
Sample : Q2555-03
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-TS-30-070925

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF071525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: rteint.p

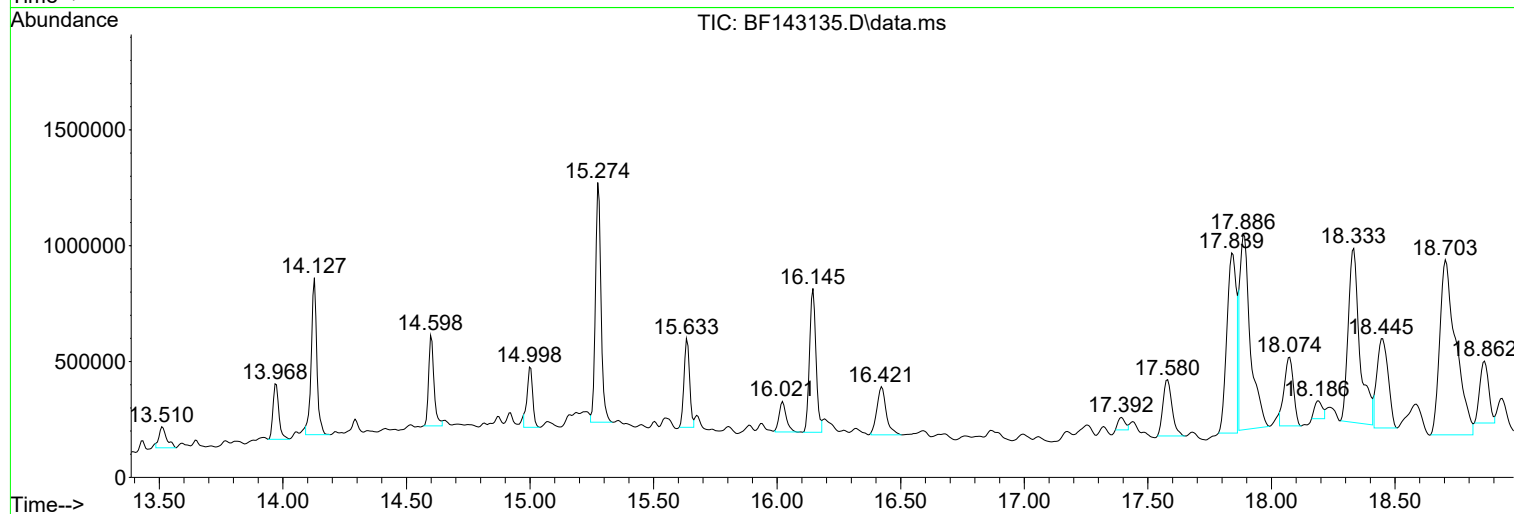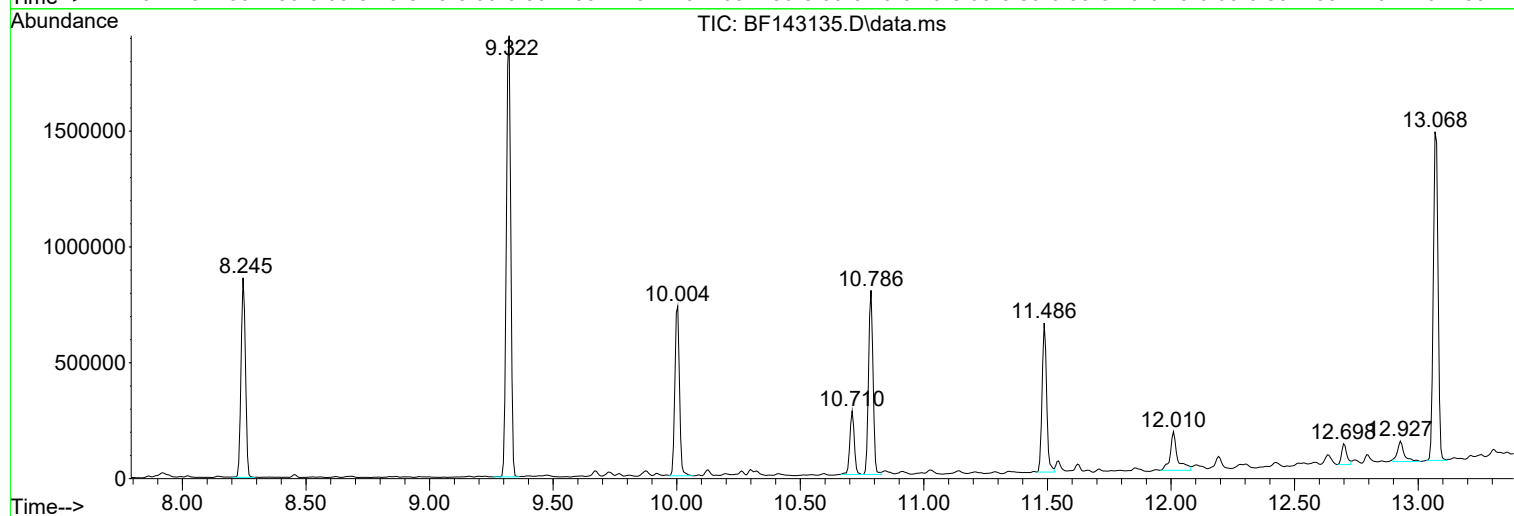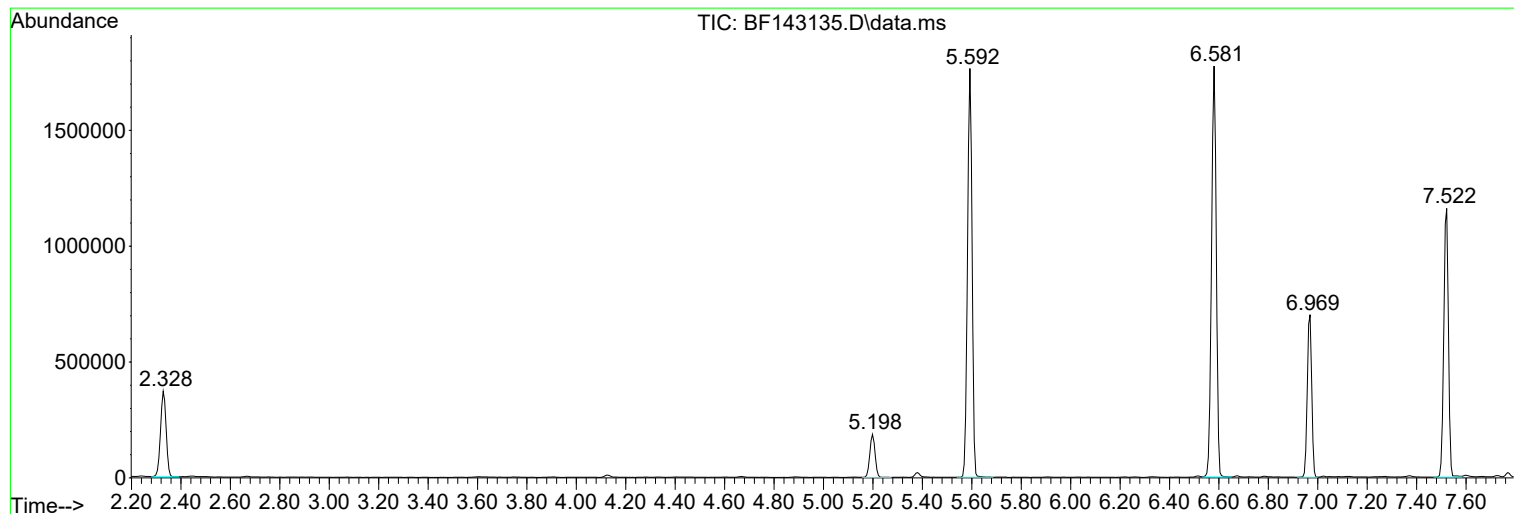

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071625\
Data File : BF143135.D
Acq On : 17 Jul 2025 04:31
Operator : RC/JU
Sample : Q2555-03
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-TS-30-070925

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF071525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071625\
Data File : BF143135.D
Acq On : 17 Jul 2025 04:31
Operator : RC/JU
Sample : Q2555-03
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-TS-30-070925

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF071525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------