

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS072425\
 Data File : PS031233.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Jul 2025 18:39
 Operator : AR\AJ
 Sample : HSTDCCC750
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HSTDCCC750

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 07/25/2025
 Supervised By :mohammad ahmed 07/25/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 25 02:14:21 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072125.M
 Quant Title : 8080.M
 QLast Update : Tue Jul 22 03:18:42 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.319	7.764	2897.4E6	704.2E6	666.345	693.771
Target Compounds							
1) T	Dalapon	2.687	2.704	3646.8E6	1685.9E6	581.355	594.302
2) T	3,5-DICHL...	6.482	6.711	3487.2E6	965.5E6	631.428	626.964
3) T	4-Nitroph...	7.119	7.298	1161.6E6	1119.3E6	704.548	618.645
5) T	DICAMBA	7.509	7.966	9918.8E6	4200.1E6	601.248	650.842
6) T	MCPD	7.690	8.065	639.6E6	128.0E6	63.900	61.597
7) T	MCPA	7.840	8.313	831.6E6	199.2E6	66.456	63.134
8) T	DICHLORPROP	8.219	8.685	2628.7E6	1015.3E6	687.792	670.244
9) T	2,4-D	8.451	9.021	2723.9E6	1183.1E6	729.306	696.612
10) T	Pentachlo...	8.755	9.545	41625.2E6	26526.7E6	762.065m	678.760
11) T	2,4,5-TP ...	9.335	9.926	15136.6E6	10005.9E6	689.481	671.801
12) T	2,4,5-T	9.629	10.352	14005.9E6	9234.0E6	717.231	649.390
13) T	2,4-DB	10.207	10.920	2059.8E6	764.1E6	688.914	652.753
14) T	DINOSEB	11.419	11.305	10002.0E6	6972.8E6	642.408m	616.949
15) T	Picloram	11.229	12.415	16290.4E6	17205.5E6	814.254m	691.121
16) T	DCPA	11.716	12.348	19417.2E6	15457.3E6	676.712	671.006m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS072425\
Data File : PS031233.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Jul 2025 18:39
Operator : AR\AJ
Sample : HSTDCCC750
Misc :
ALS Vial : 35 Sample Multiplier: 1



Instrument :
ECD_S
ClientSampleId :
HSTDCCC750


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/25/2025
Supervised By :mohammad ahmed 07/25/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 25 02:14:21 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072125.M
Quant Title : 8080.M
QLast Update : Tue Jul 22 03:18:42 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

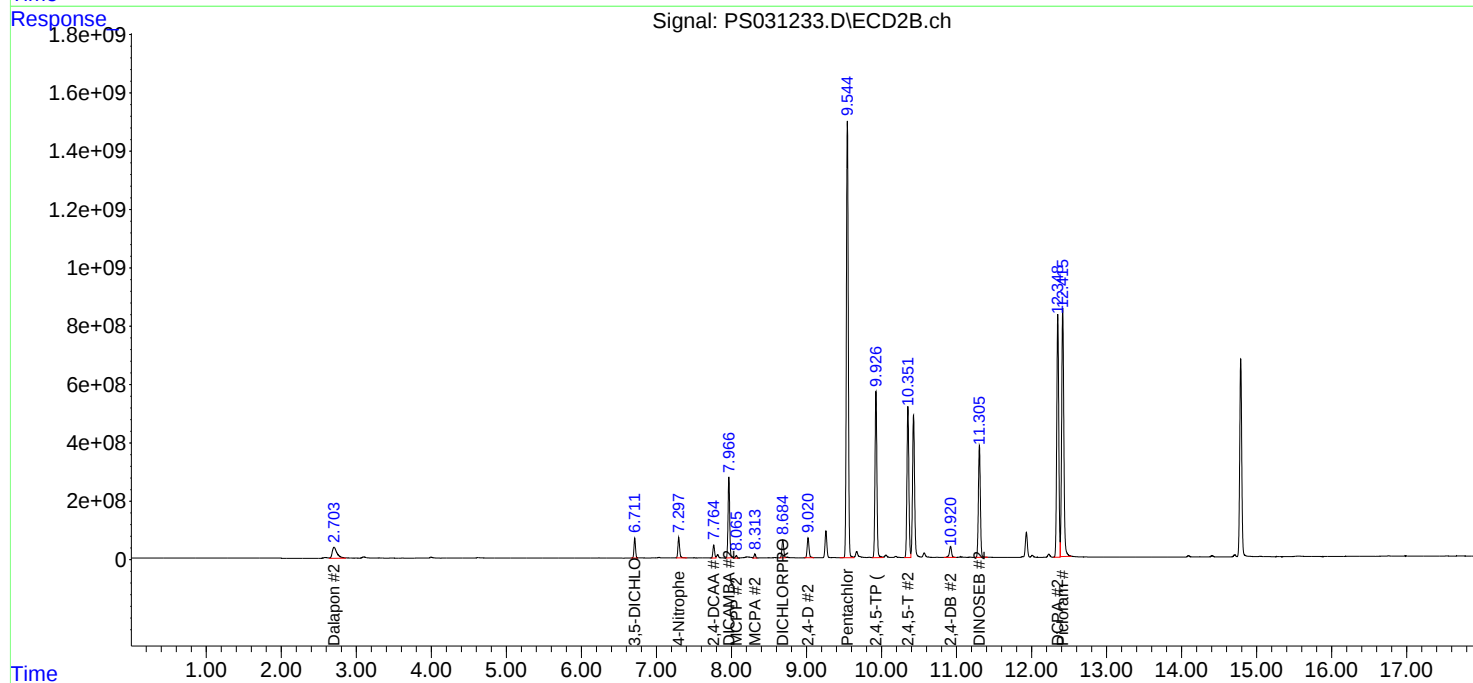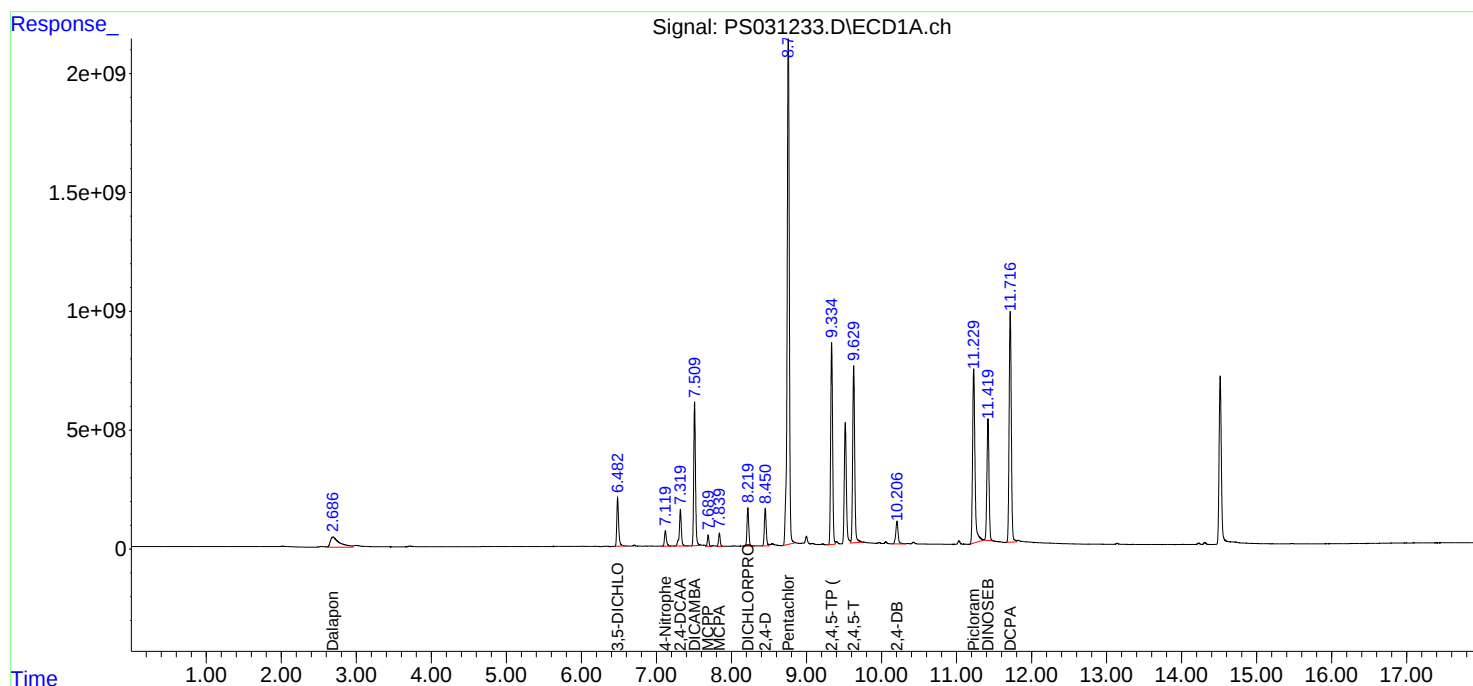

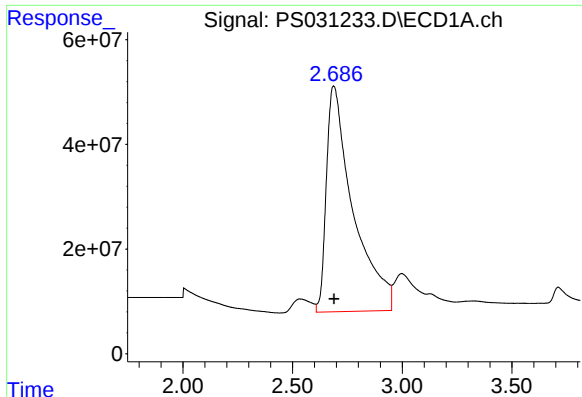


#1 Dalapon

R.T.: 2.687 min
Delta R.T.: -0.003 min
Response: 3646786474
Conc: 581.36 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/25/2025
Supervised By :mohammad ahmed 07/25/2025

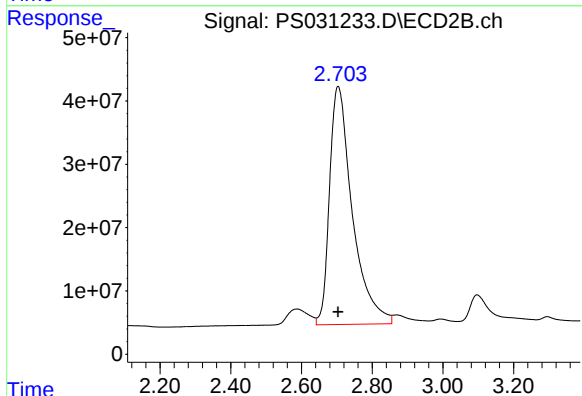


#1 Dalapon

R.T.: 2.704 min
Delta R.T.: 0.000 min
Response: 1685879056
Conc: 594.30 ng/ml

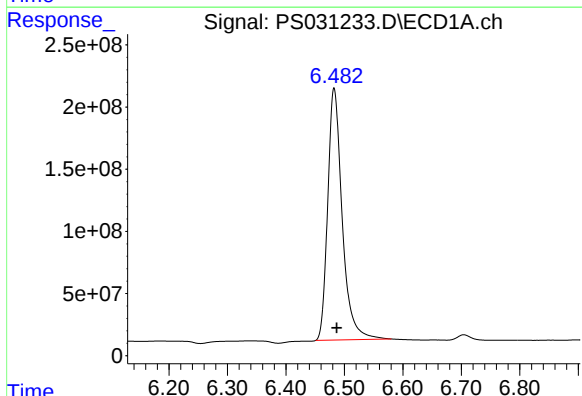


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.482 min
Delta R.T.: -0.004 min
Response: 3487217484
Conc: 631.43 ng/ml

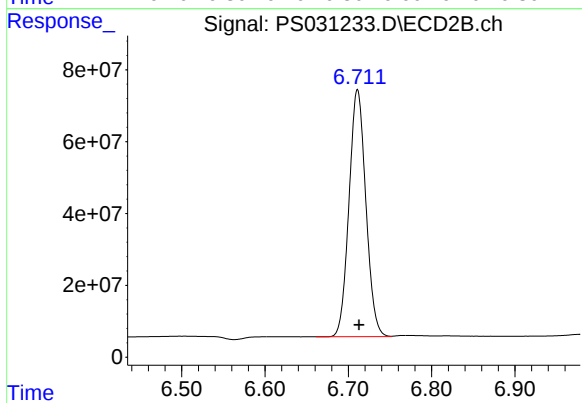

#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.711 min
Delta R.T.: -0.002 min
Response: 965457798
Conc: 626.96 ng/ml

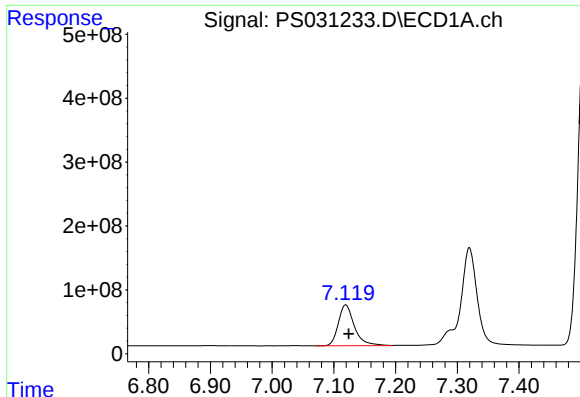

#3 4-Nitrophenol

R.T.: 7.119 min
Delta R.T.: -0.005 min
Response: 1161648350
Conc: 704.55 ng/ml

Instrument :

ECD_S

ClientSampleId :


HSTDCCC750

Manual Integrations

APPROVED


Reviewed By :Yogesh Patel 07/25/2025

Supervised By :mohammad ahmed 07/25/2025

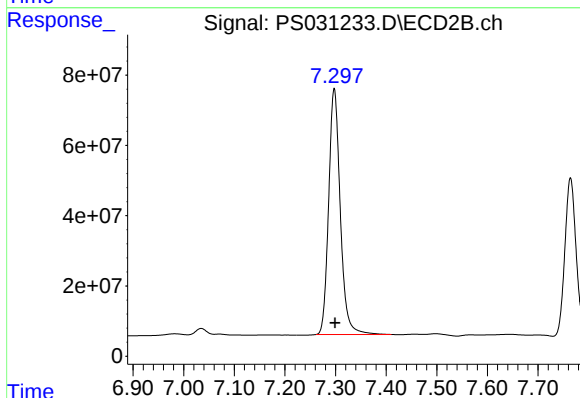


#3 4-Nitrophenol

R.T.: 7.298 min
Delta R.T.: -0.002 min
Response: 1119324899
Conc: 618.64 ng/ml

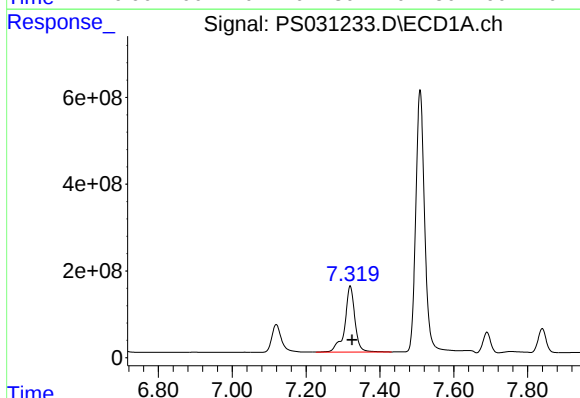


#4 2,4-DCAA

R.T.: 7.319 min
Delta R.T.: -0.005 min
Response: 2897435123
Conc: 666.34 ng/ml

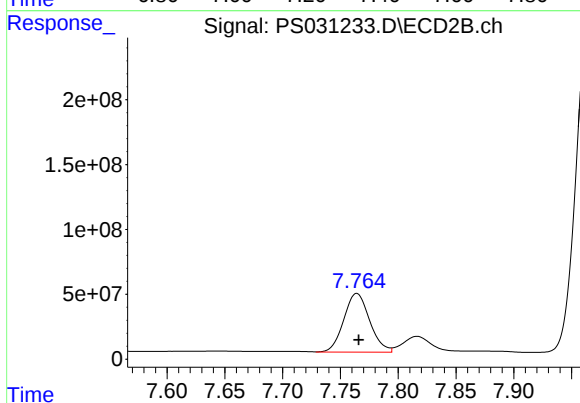

#4 2,4-DCAA

R.T.: 7.764 min
Delta R.T.: -0.002 min
Response: 704155508
Conc: 693.77 ng/ml

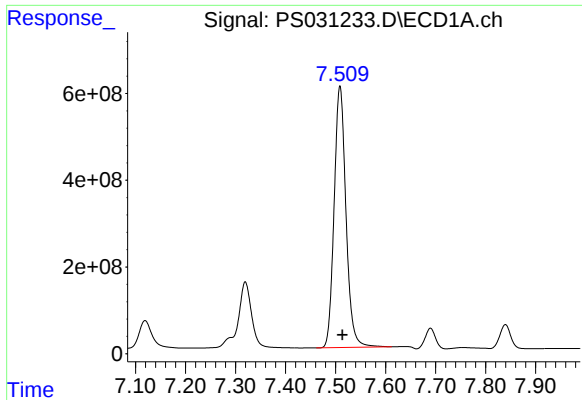


#5 DICAMBA

R.T.: 7.509 min
Delta R.T.: -0.005 min
Response: 9918771681
Conc: 601.25 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/25/2025
Supervised By :mohammad ahmed 07/25/2025

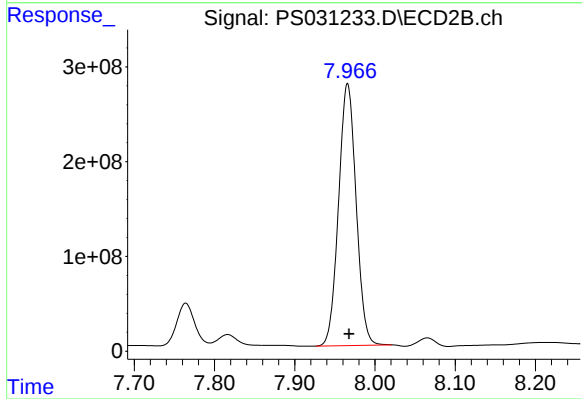


#5 DICAMBA

R.T.: 7.966 min
Delta R.T.: -0.002 min
Response: 4200124781
Conc: 650.84 ng/ml

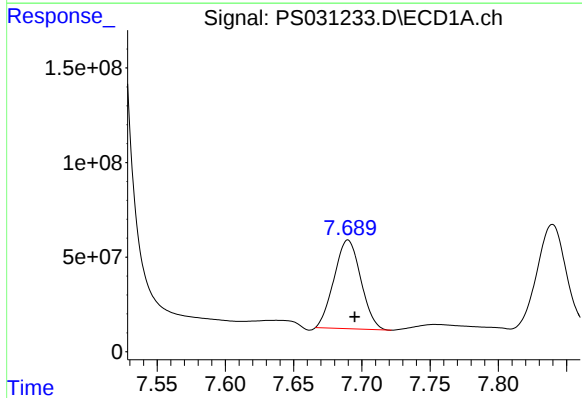


#6 MCPP

R.T.: 7.690 min
Delta R.T.: -0.005 min
Response: 639646471
Conc: 63.90 ug/ml

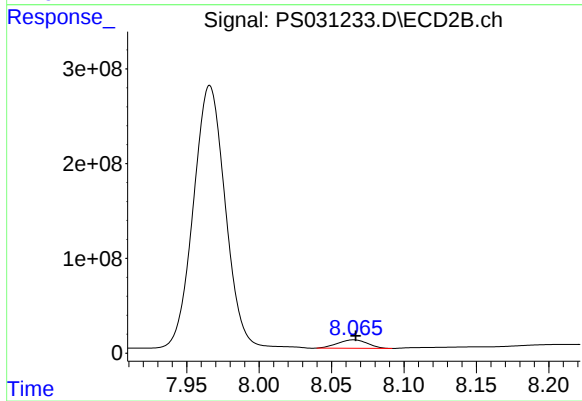

#6 MCPP

R.T.: 8.065 min
Delta R.T.: -0.001 min
Response: 127986691
Conc: 61.60 ug/ml

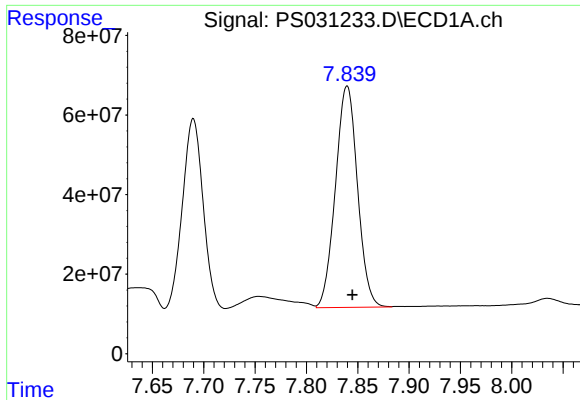


#7 MCPA

R.T.: 7.840 min
Delta R.T.: -0.005 min
Response: 831645162
Conc: 66.46 ug/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/25/2025
Supervised By :mohammad ahmed 07/25/2025

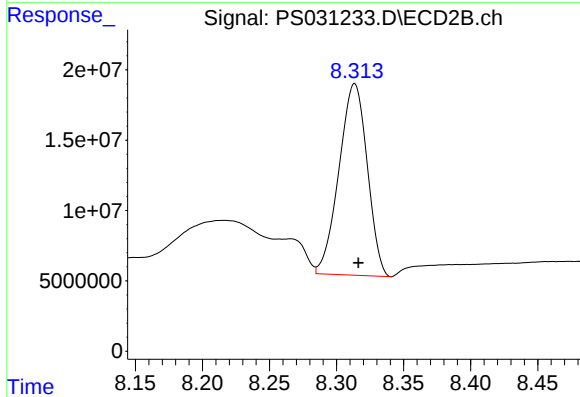


#7 MCPA

R.T.: 8.313 min
Delta R.T.: -0.003 min
Response: 199200038
Conc: 63.13 ug/ml

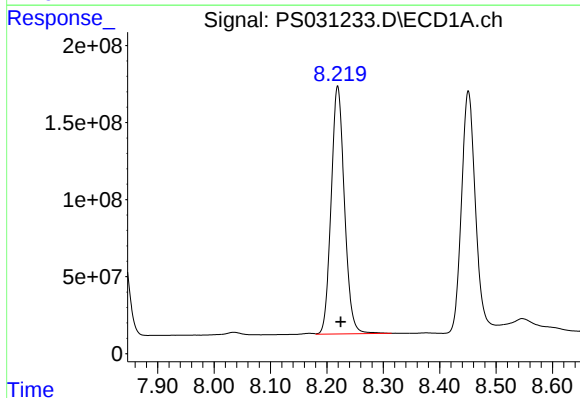


#8 DICHLORPROP

R.T.: 8.219 min
Delta R.T.: -0.005 min
Response: 2628708493
Conc: 687.79 ng/ml

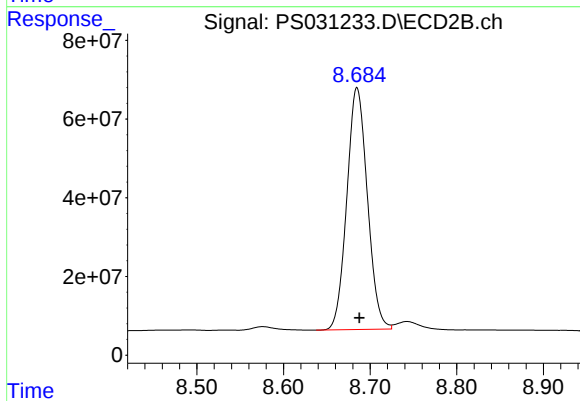

#8 DICHLORPROP

R.T.: 8.685 min
Delta R.T.: -0.003 min
Response: 1015326356
Conc: 670.24 ng/ml

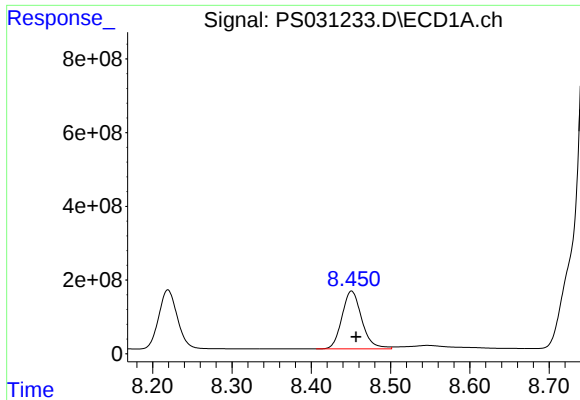


#9 2,4-D

R.T.: 8.451 min
Delta R.T.: -0.006 min
Response: 2723897944
Conc: 729.31 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/25/2025
Supervised By :mohammad ahmed 07/25/2025

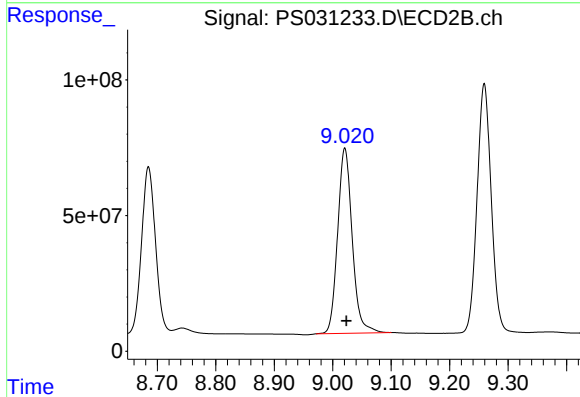


#9 2,4-D

R.T.: 9.021 min
Delta R.T.: -0.003 min
Response: 1183069685
Conc: 696.61 ng/ml

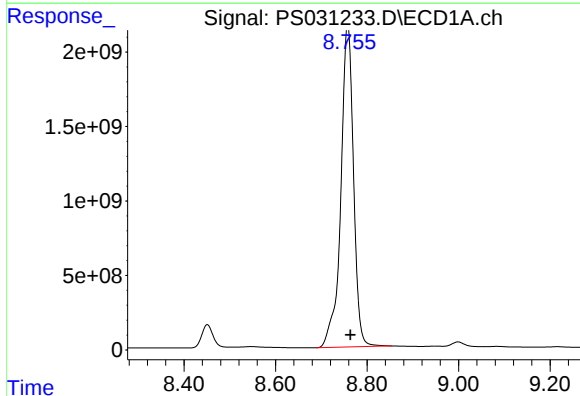


#10 Pentachlorophenol

R.T.: 8.755 min
Delta R.T.: -0.008 min
Response: 41625198173
Conc: 762.07 ng/ml m

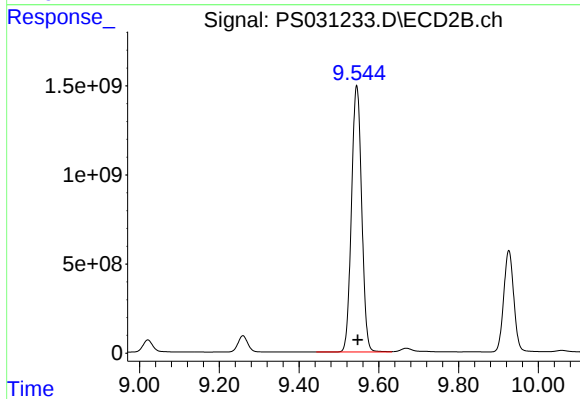

#10 Pentachlorophenol

R.T.: 9.545 min
Delta R.T.: -0.003 min
Response: 26526744051
Conc: 678.76 ng/ml

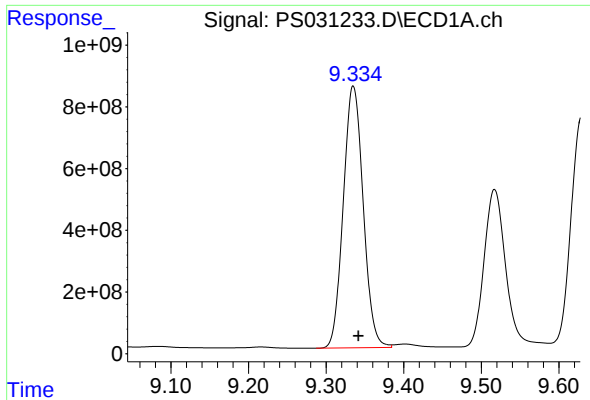


#11 2,4,5-TP (SILVEX)

R.T.: 9.335 min
Delta R.T.: -0.007 min
Response: 15136567168
Conc: 689.48 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/25/2025
Supervised By :mohammad ahmed 07/25/2025

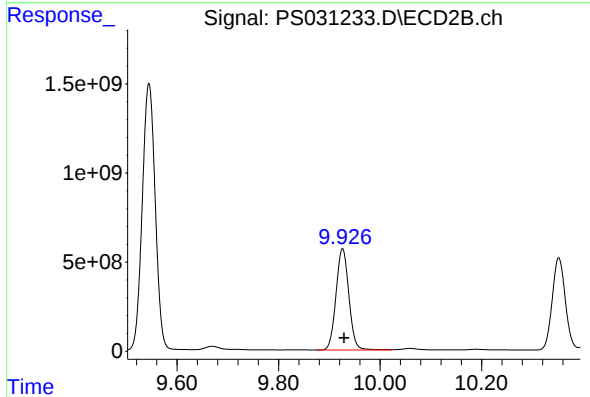


#11 2,4,5-TP (SILVEX)

R.T.: 9.926 min
Delta R.T.: -0.003 min
Response: 10005926582
Conc: 671.80 ng/ml

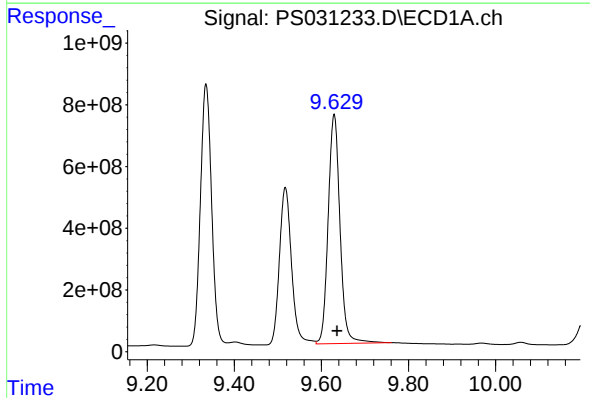


#12 2,4,5-T

R.T.: 9.629 min
Delta R.T.: -0.007 min
Response: 14005933448
Conc: 717.23 ng/ml

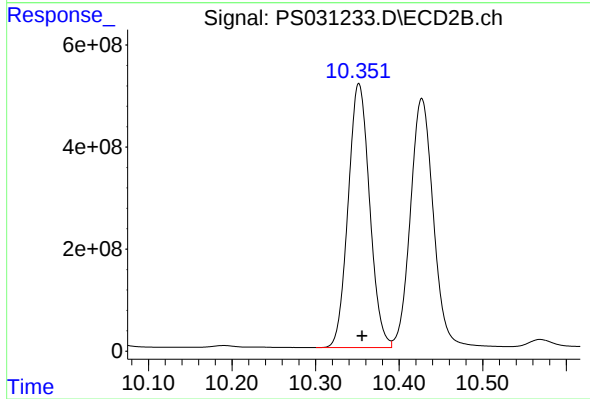

#12 2,4,5-T

R.T.: 10.352 min
Delta R.T.: -0.004 min
Response: 9233980783
Conc: 649.39 ng/ml

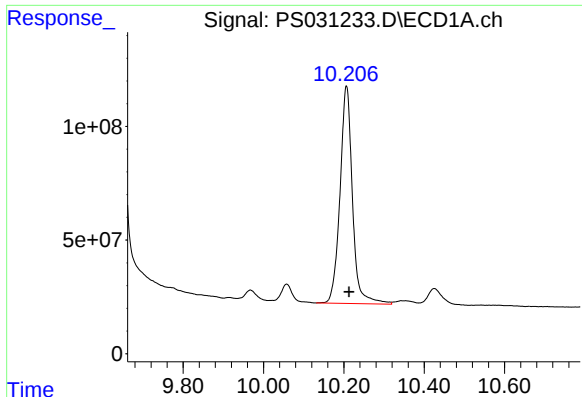


#13 2,4-DB

R.T.: 10.207 min
Delta R.T.: -0.006 min
Response: 2059772066
Conc: 688.91 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/25/2025
Supervised By :mohammad ahmed 07/25/2025

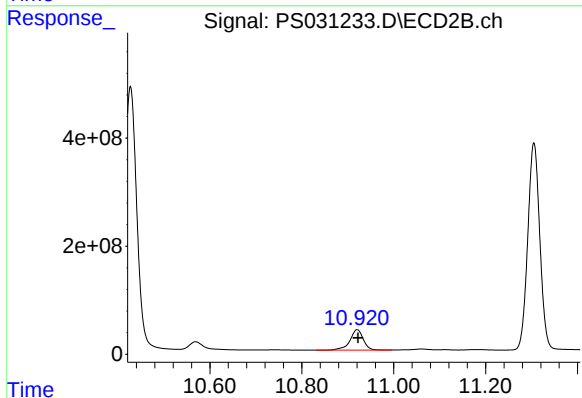


#13 2,4-DB

R.T.: 10.920 min
Delta R.T.: -0.002 min
Response: 764054036
Conc: 652.75 ng/ml

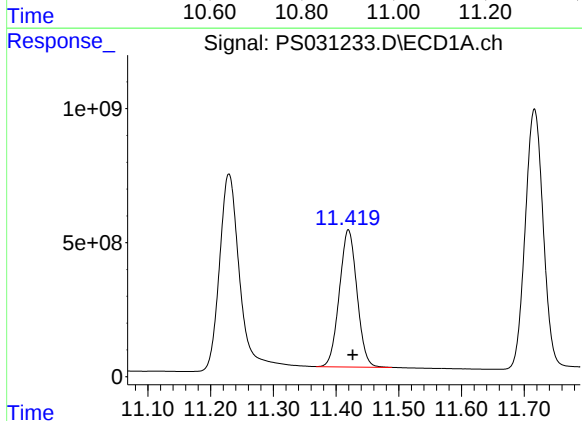


#14 DINOSEB

R.T.: 11.419 min
Delta R.T.: -0.008 min
Response: 10001961874
Conc: 642.41 ng/ml m

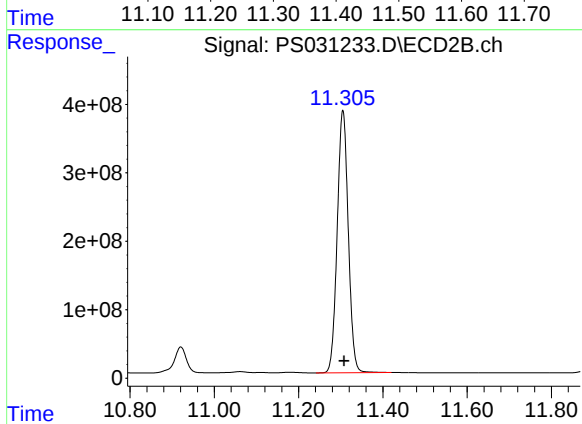

#14 DINOSEB

R.T.: 11.305 min
Delta R.T.: -0.003 min
Response: 6972808210
Conc: 616.95 ng/ml

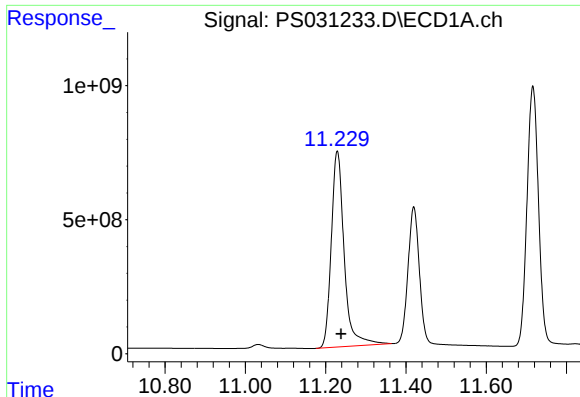


#15 Picloram

R.T.: 11.229 min
Delta R.T.: -0.010 min
Response: 16290439586
Conc: 814.25 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/25/2025
Supervised By :mohammad ahmed 07/25/2025

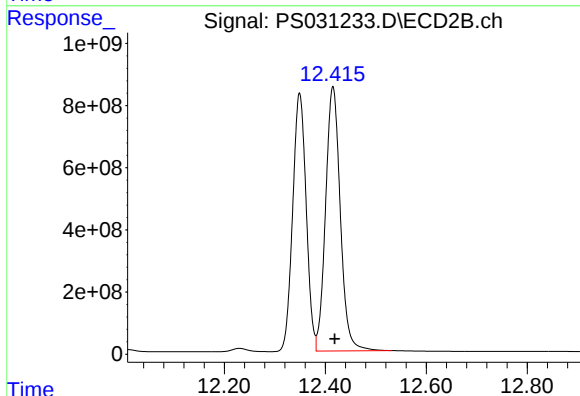


#15 Picloram

R.T.: 12.415 min
Delta R.T.: -0.004 min
Response: 17205474787
Conc: 691.12 ng/ml

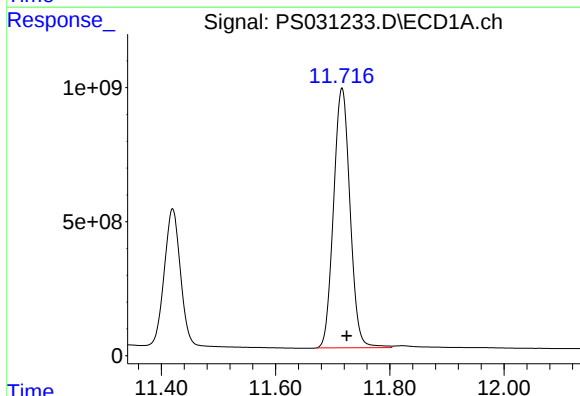

#16 DCPA

R.T.: 11.716 min
Delta R.T.: -0.008 min
Response: 19417209517
Conc: 676.71 ng/ml

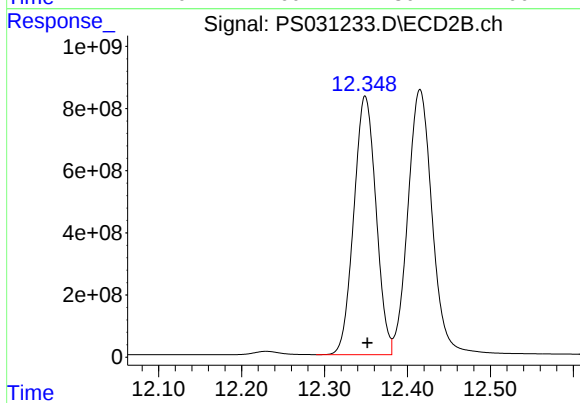

#16 DCPA

R.T.: 12.348 min
Delta R.T.: -0.003 min
Response: 15457311166
Conc: 671.01 ng/ml m