

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061825\
 Data File : PD088992.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Jun 2025 15:39
 Operator : AR\AJ
 Sample : RESCHK
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 RESCHK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 18 05:45:52 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061825.M
 Quant Title : GC Extractables
 QLast Update : Wed Jun 18 05:39:05 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.549	2.880	52680950	330.6E6	18.464	19.499
28)	SA Decachlor...	9.072	8.072	78084661	390.3E6	19.881	19.740
Target Compounds							
9)	A Endosulfan I	6.073	5.247	38990490	203.9E6	8.650	9.781
10)	B gamma-Chl...	5.945	5.126	42512564	246.4E6	8.879	10.301
12)	B 4,4'-DDE	6.194	5.375	80006399	453.6E6	18.346	19.792
13)	MA Dieldrin	6.346	5.513	85610068	448.6E6	17.845	19.331
19)	B Endosulfa...	7.149	6.482	70890098	384.7E6	18.474	19.606
20)	A Methoxychlor	7.493	6.754	177.7E6	906.9E6	87.946	84.219
21)	B Endrin ke...	7.629	6.991	74223999	422.4E6	18.223	19.555



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061825\
Data File : PD088992.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Jun 2025 15:39
Operator : AR\AJ
Sample : RESCHK
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESCHK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 18 05:45:52 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061825.M
Quant Title : GC Extractables
QLast Update : Wed Jun 18 05:39:05 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

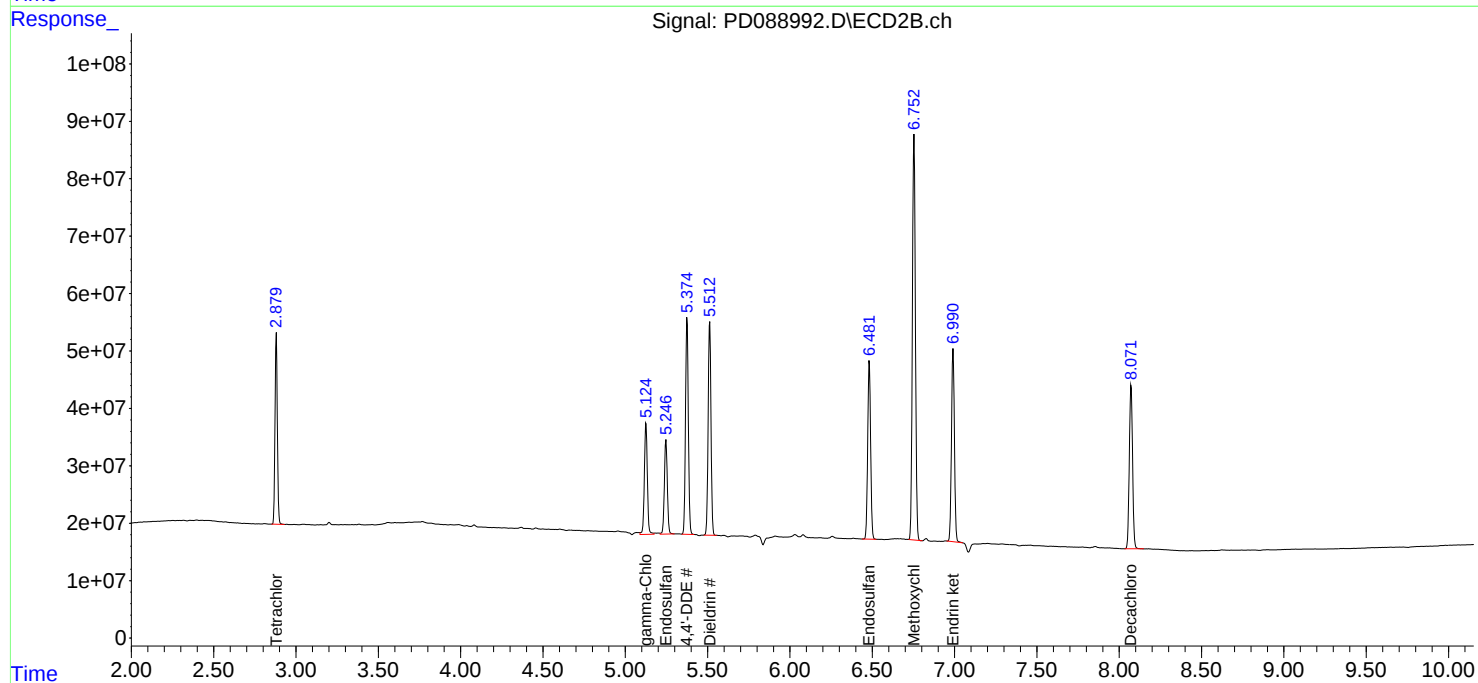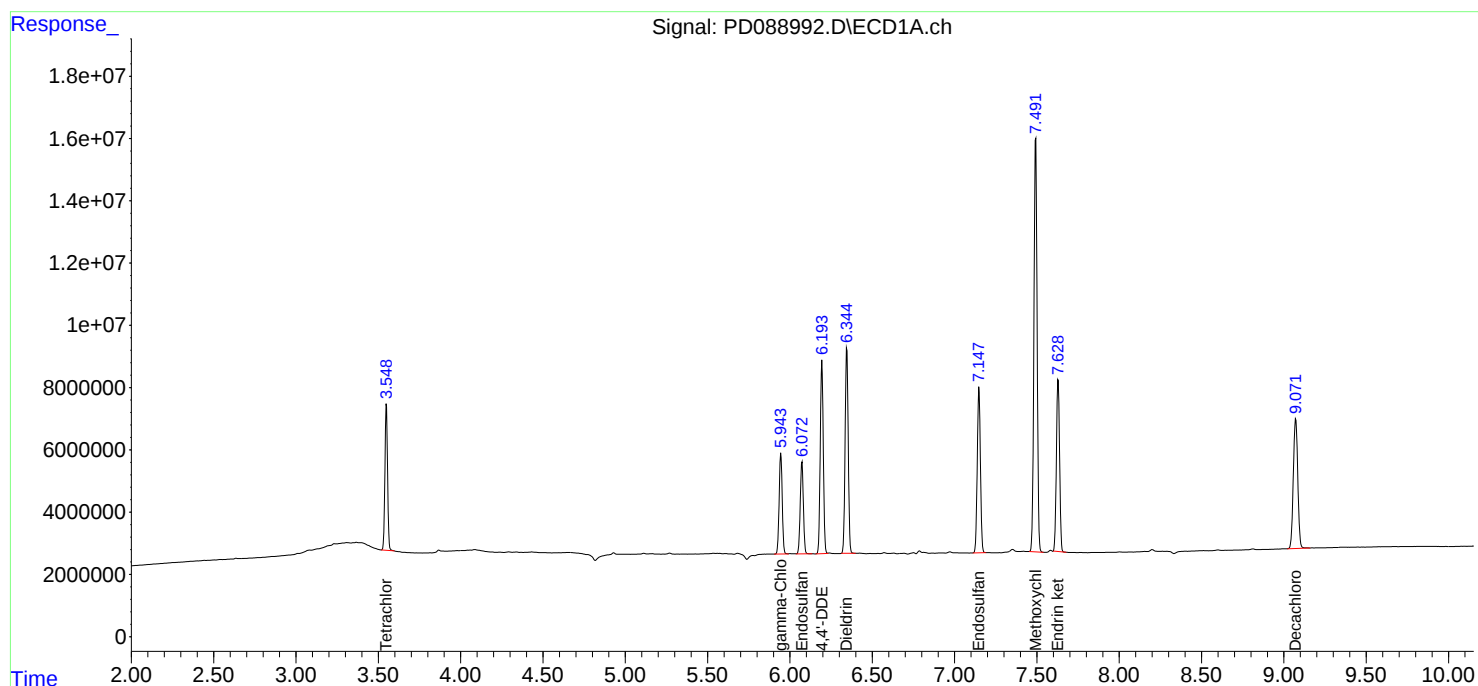


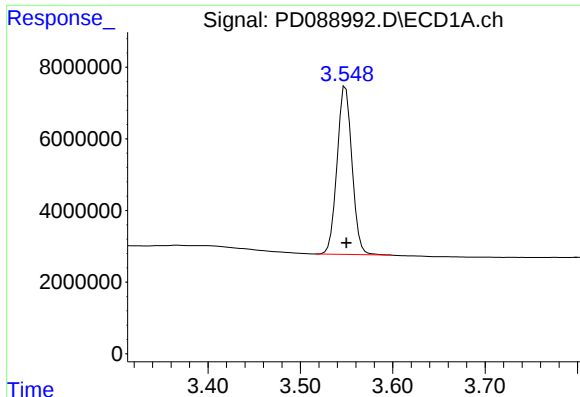

#1 Tetrachloro-m-xylene


R.T.: 3.549 min
Delta R.T.: -0.001 min
Response: 52680950
Conc: 18.46 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

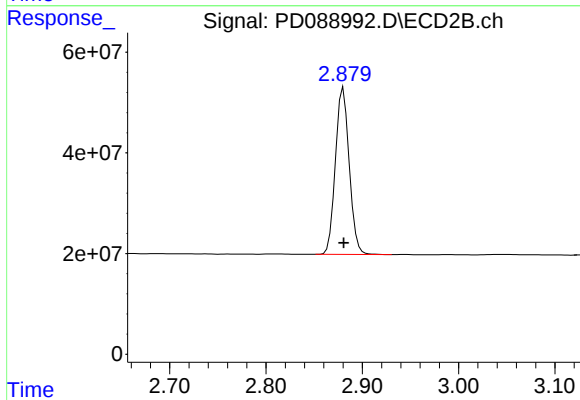


#1 Tetrachloro-m-xylene

R.T.: 2.880 min
Delta R.T.: 0.000 min
Response: 330573317
Conc: 19.50 ng/ml

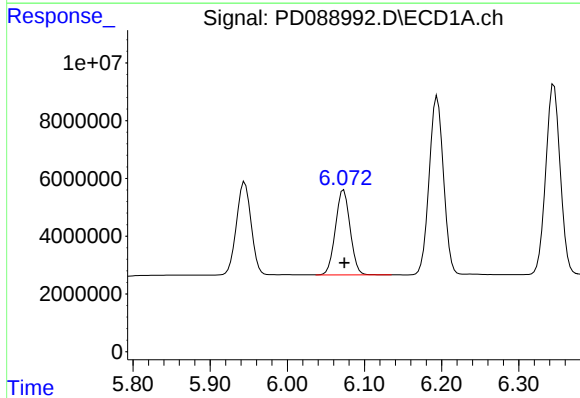


#9 Endosulfan I

R.T.: 6.073 min
Delta R.T.: 0.000 min
Response: 38990490
Conc: 8.65 ng/ml

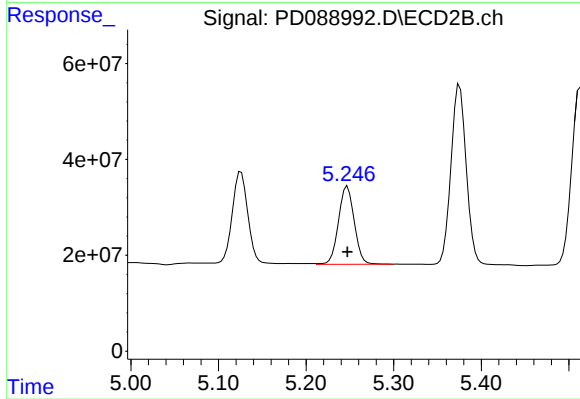

#9 Endosulfan I


R.T.: 5.247 min
Delta R.T.: 0.000 min
Response: 203864959
Conc: 9.78 ng/ml

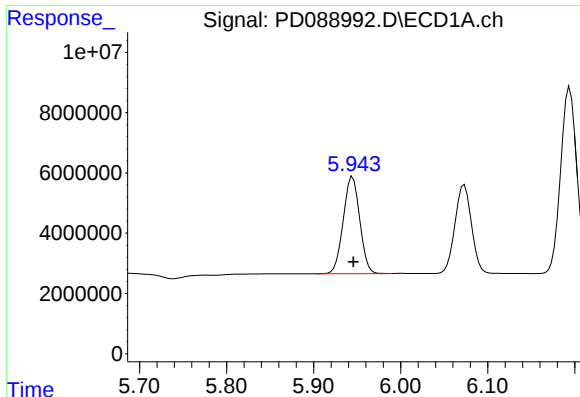

#10 gamma-Chlordane


R.T.: 5.945 min
Delta R.T.: 0.000 min
Response: 42512564
Conc: 8.88 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

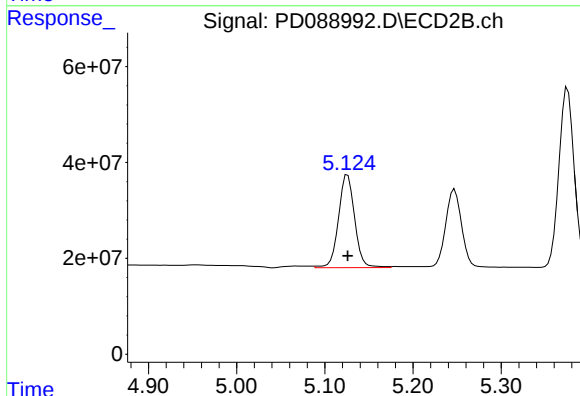


#10 gamma-Chlordane

R.T.: 5.126 min
Delta R.T.: 0.000 min
Response: 246437887
Conc: 10.30 ng/ml

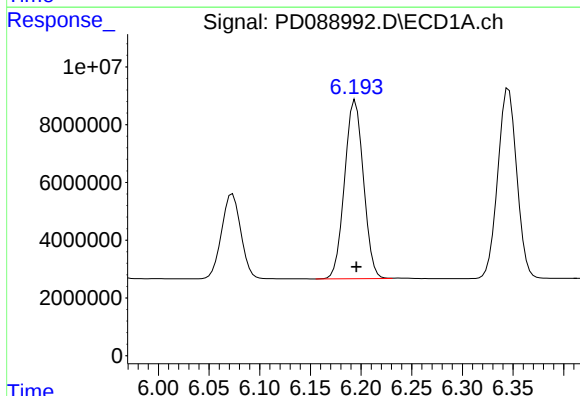


#12 4,4'-DDE

R.T.: 6.194 min
Delta R.T.: 0.000 min
Response: 80006399
Conc: 18.35 ng/ml

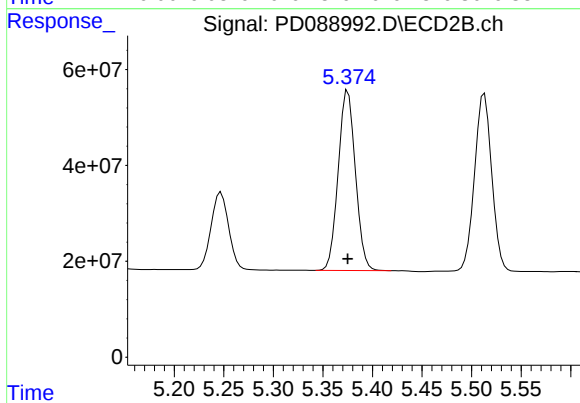

#12 4,4'-DDE


R.T.: 5.375 min
Delta R.T.: 0.000 min
Response: 453562275
Conc: 19.79 ng/ml

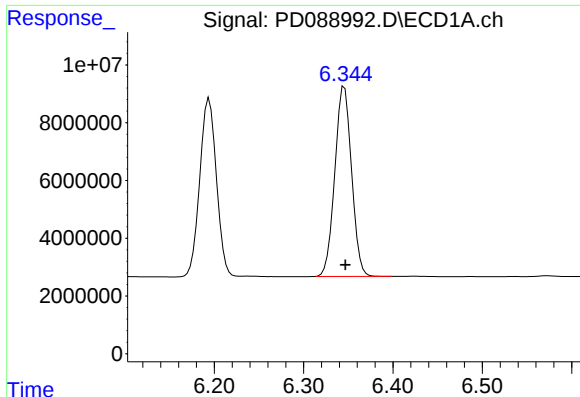

#13 Dieldrin


R.T.: 6.346 min
Delta R.T.: -0.001 min
Response: 85610068
Conc: 17.84 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

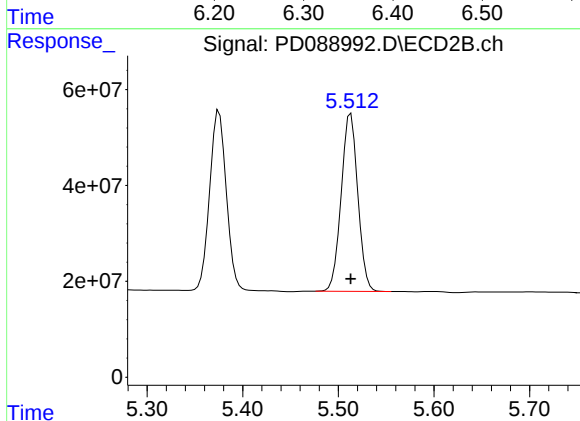


#13 Dieldrin

R.T.: 5.513 min
Delta R.T.: 0.000 min
Response: 448633404
Conc: 19.33 ng/ml

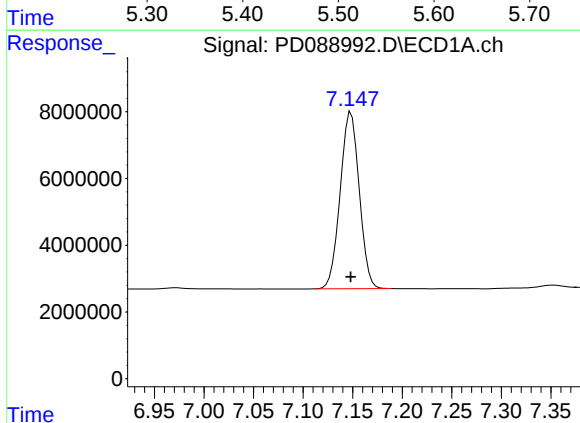


#19 Endosulfan Sulfate

R.T.: 7.149 min
Delta R.T.: 0.000 min
Response: 70890098
Conc: 18.47 ng/ml

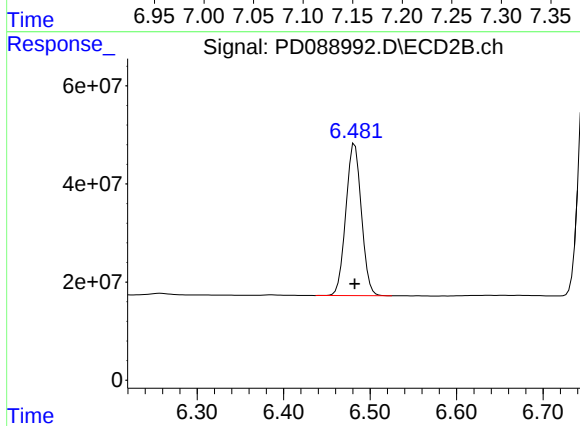

#19 Endosulfan Sulfate


R.T.: 6.482 min
Delta R.T.: 0.000 min
Response: 384695171
Conc: 19.61 ng/ml

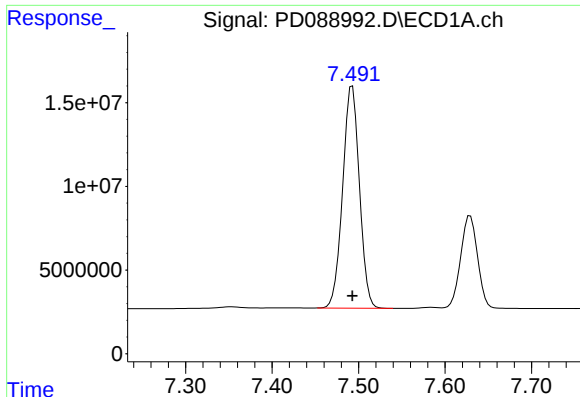

#20 Methoxychlor


R.T.: 7.493 min
Delta R.T.: 0.000 min
Response: 177705291
Conc: 87.95 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

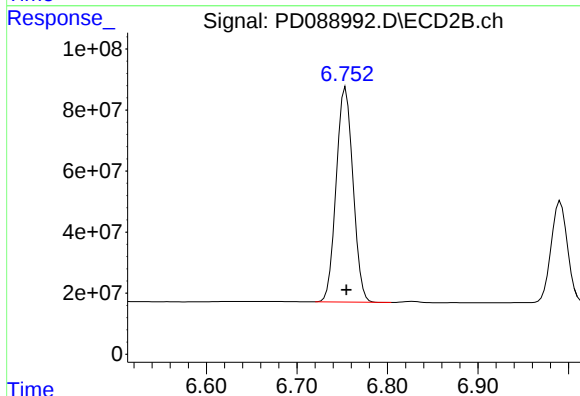


#20 Methoxychlor

R.T.: 6.754 min
Delta R.T.: 0.000 min
Response: 906875013
Conc: 84.22 ng/ml

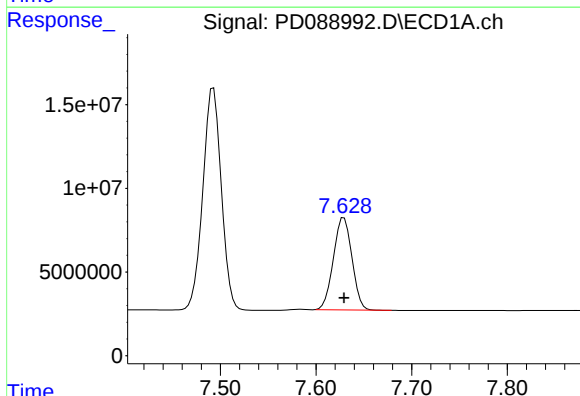


#21 Endrin ketone

R.T.: 7.629 min
Delta R.T.: 0.000 min
Response: 74223999
Conc: 18.22 ng/ml

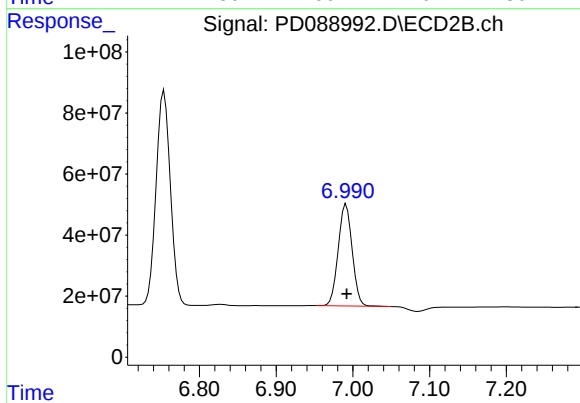

#21 Endrin ketone


R.T.: 6.991 min
Delta R.T.: -0.001 min
Response: 422419686
Conc: 19.55 ng/ml

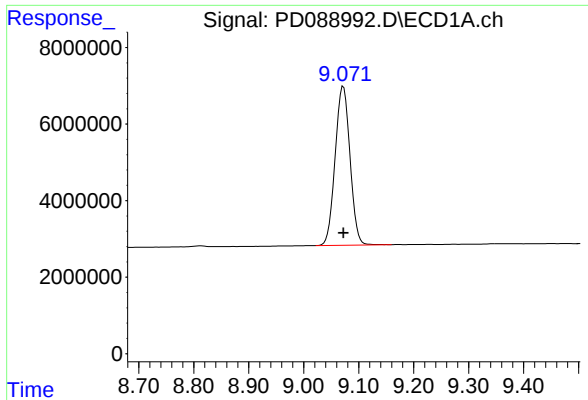

#28 Decachlorobiphenyl

R.T.: 9.072 min
Delta R.T.: 0.000 min
Response: 78084661
Conc: 19.88 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

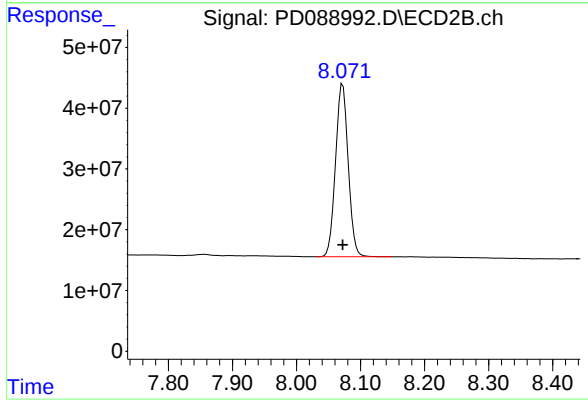

#28 Decachlorobiphenyl

R.T.: 8.072 min
Delta R.T.: 0.000 min
Response: 390253423
Conc: 19.74 ng/ml