

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071625\
 Data File : BF143134.D
 Acq On : 17 Jul 2025 04:02
 Operator : RC/JU
 Sample : Q2558-01
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 OU4-TS-Denali-070925

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF071525.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF143134.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.340	17	25	33	rVB	410120	660606	26.92%	2.985%
2	5.199	505	511	519	rBV	186031	269825	11.00%	1.219%
3	5.593	572	578	583	rBV	1786557	2323699	94.69%	10.501%
4	6.581	737	746	751	rBV	1822110	2453934	100.00%	11.090%
5	6.969	806	812	817	rVB	715131	908673	37.03%	4.106%
6	7.522	899	906	911	rBV	1170917	1560063	63.57%	7.050%
7	7.769	944	948	955	rVB	20969	24730	1.01%	0.112%
8	8.245	1023	1029	1034	rBV	920515	1137122	46.34%	5.139%
9	9.322	1206	1212	1217	rBV	1906474	2432119	99.11%	10.991%
10	9.998	1322	1327	1332	rBV	810446	1040021	42.38%	4.700%
11	10.710	1443	1448	1453	rBV	318282	384130	15.65%	1.736%
12	10.786	1455	1461	1471	rBV	611699	791684	32.26%	3.578%
13	11.486	1575	1580	1587	rBV	677070	885910	36.10%	4.004%
14	11.545	1587	1590	1596	rVB2	17692	31272	1.27%	0.141%
15	12.010	1660	1669	1673	rBV4	48413	113829	4.64%	0.514%
16	12.104	1682	1685	1692	rVB	14776	30729	1.25%	0.139%
17	12.192	1697	1700	1704	rVB5	24718	32474	1.32%	0.147%
18	12.633	1771	1775	1782	rVB5	25955	50118	2.04%	0.226%
19	12.698	1782	1786	1790	rBV	83970	102963	4.20%	0.465%
20	12.745	1790	1794	1798	rVB	30960	39402	1.61%	0.178%
21	12.792	1799	1802	1810	rBV3	13433	31012	1.26%	0.140%
22	12.927	1820	1825	1840	rVB	91807	146804	5.98%	0.663%
23	13.069	1844	1849	1856	rVB	1267147	1605709	65.43%	7.257%
24	13.810	1971	1975	1997	rVB10	89811	362196	14.76%	1.637%
25	13.969	1998	2002	2010	rBV2	119133	185057	7.54%	0.836%
26	14.127	2018	2029	2041	rVB	856610	1735236	70.71%	7.842%
27	14.598	2105	2109	2114	rBV	83925	134860	5.50%	0.609%
28	14.998	2174	2177	2185	rVB	50660	76573	3.12%	0.346%
29	15.186	2205	2209	2219	rVB	60758	138652	5.65%	0.627%
30	15.274	2219	2224	2233	rVB2	177638	292297	11.91%	1.321%
31	15.504	2260	2263	2267	rVB	33780	43969	1.79%	0.199%
32	15.563	2270	2273	2278	rVB	46142	66059	2.69%	0.299%
33	15.633	2279	2285	2301	rVB	483163	810562	33.03%	3.663%
34	16.139	2366	2371	2376	rBV	133088	241048	9.82%	1.089%
35	17.821	2650	2657	2670	rBV4	126169	443069	18.06%	2.002%
36	18.315	2735	2741	2748	rBV2	69580	182771	7.45%	0.826%

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071625\
Data File : BF143134.D
Acq On : 17 Jul 2025 04:02
Operator : RC/JU
Sample : Q2558-01
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-TS-Denali-070925

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF071525.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	18.680	2797	2803	2823	rBV5	82462	358681	14.62%	1.621%
----	--------	------	------	------	------	-------	--------	--------	--------




Sum of corrected areas: 22127858

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071625\
Data File : BF143134.D
Acq On : 17 Jul 2025 04:02
Operator : RC/JU
Sample : Q2558-01
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-TS-Denali-070925

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF071525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

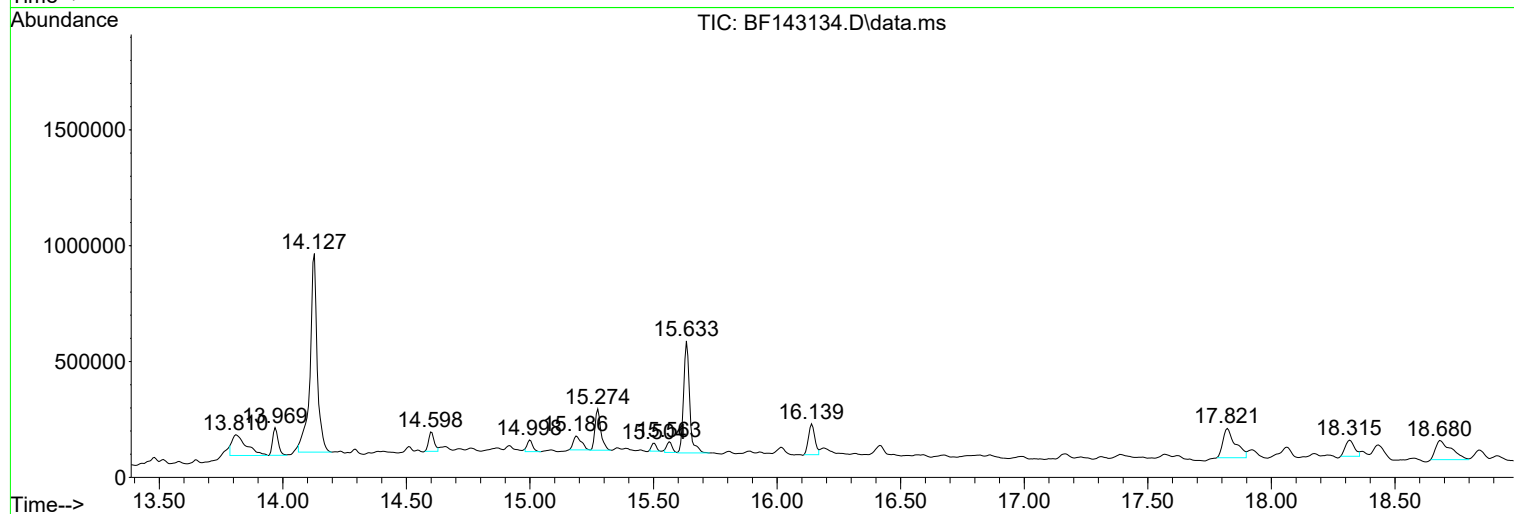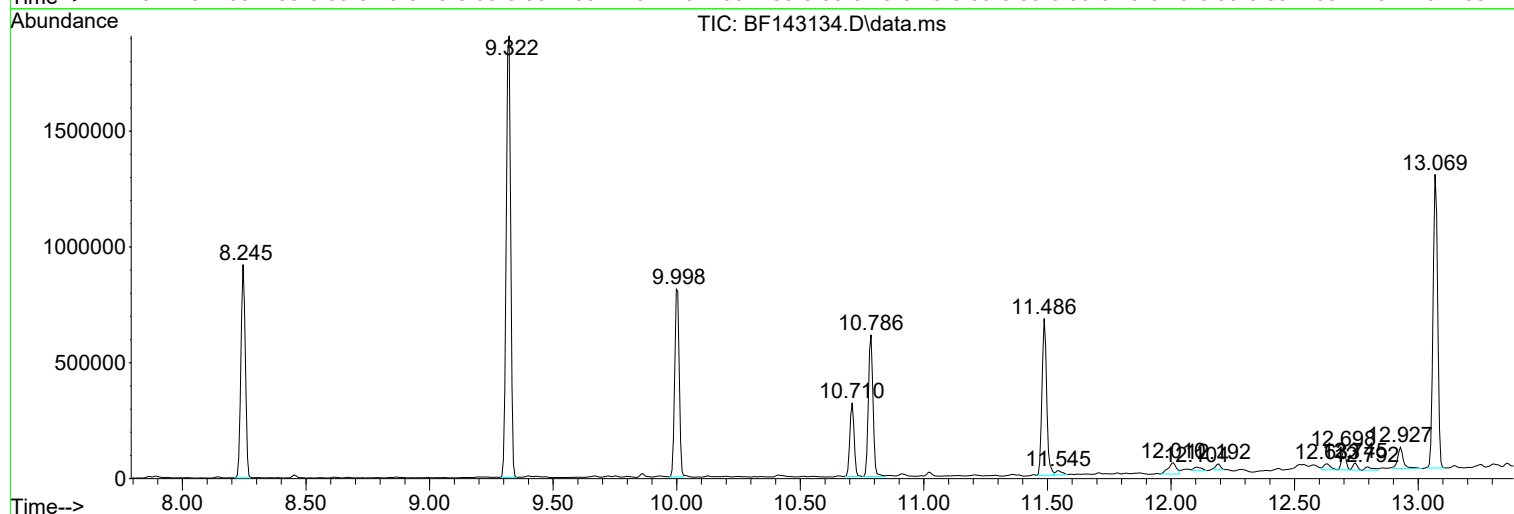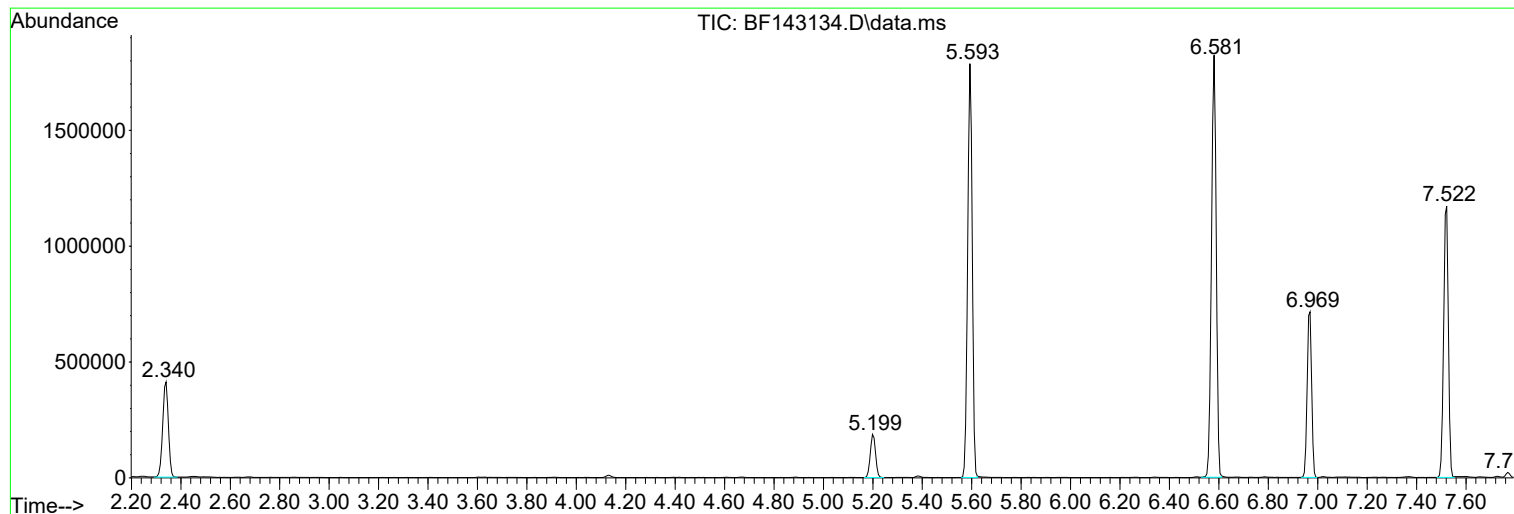

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071625\
Data File : BF143134.D
Acq On : 17 Jul 2025 04:02
Operator : RC/JU
Sample : Q2558-01
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-TS-Denali-070925

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF071525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071625\
Data File : BF143134.D
Acq On : 17 Jul 2025 04:02
Operator : RC/JU
Sample : Q2558-01
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-TS-Denali-070925

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF071525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------