

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071625\
 Data File : BF143136.D
 Acq On : 17 Jul 2025 05:00
 Operator : RC/JU
 Sample : Q2558-03
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 OU4-TS-Grillo-OG-070925

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF071525.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF143136.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.328	15	23	33	rVB	408034	661187	25.75%	2.566%
2	5.199	504	511	518	rBV	185873	271193	10.56%	1.053%
3	5.593	572	578	583	rBV	1774887	2302724	89.67%	8.938%
4	6.581	738	746	751	rBV	1784118	2376095	92.53%	9.222%
5	6.681	758	763	767	rVB	49122	62297	2.43%	0.242%
6	6.969	806	812	817	rVB	688450	874907	34.07%	3.396%
7	7.522	899	906	911	rBV	1144134	1514258	58.97%	5.877%
8	7.769	944	948	952	rVB	21717	25873	1.01%	0.100%
9	8.245	1024	1029	1034	rBV	836477	1027785	40.02%	3.989%
10	9.322	1206	1212	1217	rBV	1768832	2234127	87.00%	8.671%
11	10.004	1322	1328	1340	rBV	705877	924501	36.00%	3.588%
12	10.710	1443	1448	1455	rVB	297492	361885	14.09%	1.405%
13	10.786	1455	1461	1466	rBV	754543	960931	37.42%	3.730%
14	11.022	1498	1501	1506	rVB2	21192	30466	1.19%	0.118%
15	11.486	1575	1580	1587	rBV	643942	871104	33.92%	3.381%
16	11.545	1587	1590	1596	rVB2	26233	42811	1.67%	0.166%
17	12.010	1661	1669	1674	rBV3	172353	305857	11.91%	1.187%
18	12.104	1682	1685	1692	rVB2	26809	46788	1.82%	0.182%
19	12.192	1696	1700	1709	rVB4	69169	117522	4.58%	0.456%
20	12.698	1782	1786	1791	rBV	171883	226966	8.84%	0.881%
21	12.804	1799	1804	1809	rBV2	126243	187083	7.29%	0.726%
22	12.928	1821	1825	1838	rVB	152496	235743	9.18%	0.915%
23	13.075	1844	1850	1858	rVB	1318141	1752803	68.26%	6.803%
24	13.510	1922	1924	1929	rVB3	49336	64977	2.53%	0.252%
25	13.969	1998	2002	2012	rVB2	230755	360620	14.04%	1.400%
26	14.127	2021	2029	2042	rVB2	1106428	2567931	100.00%	9.967%
27	14.604	2106	2110	2115	rBV	215491	302496	11.78%	1.174%
28	15.004	2174	2178	2185	rVB	140462	198548	7.73%	0.771%
29	15.274	2220	2224	2234	rVB	523955	848336	33.04%	3.293%
30	15.633	2281	2285	2290	rBV	349031	538650	20.98%	2.091%
31	16.145	2366	2372	2377	rBV	311964	574592	22.38%	2.230%
32	17.833	2652	2659	2663	rBV2	356002	904818	35.24%	3.512%
33	18.327	2736	2743	2756	rBV	311298	894809	34.85%	3.473%
34	18.698	2798	2806	2810	rBV3	262290	741182	28.86%	2.877%
35	18.857	2827	2833	2840	rVB2	145896	352325	13.72%	1.367%

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071625\
Data File : BF143136.D
Acq On : 17 Jul 2025 05:00
Operator : RC/JU
Sample : Q2558-03
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-TS-Grillo-OG-070925

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF071525.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION




Sum of corrected areas: 25764190

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071625\
Data File : BF143136.D
Acq On : 17 Jul 2025 05:00
Operator : RC/JU
Sample : Q2558-03
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-TS-Grillo-OG-070925

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF071525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

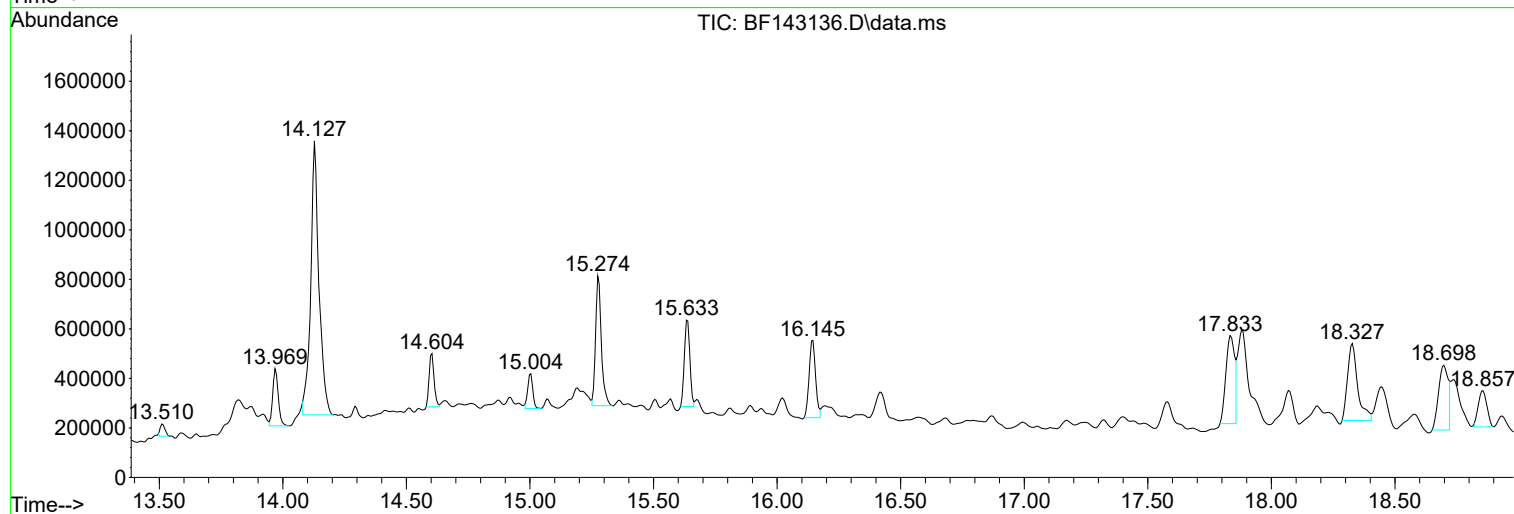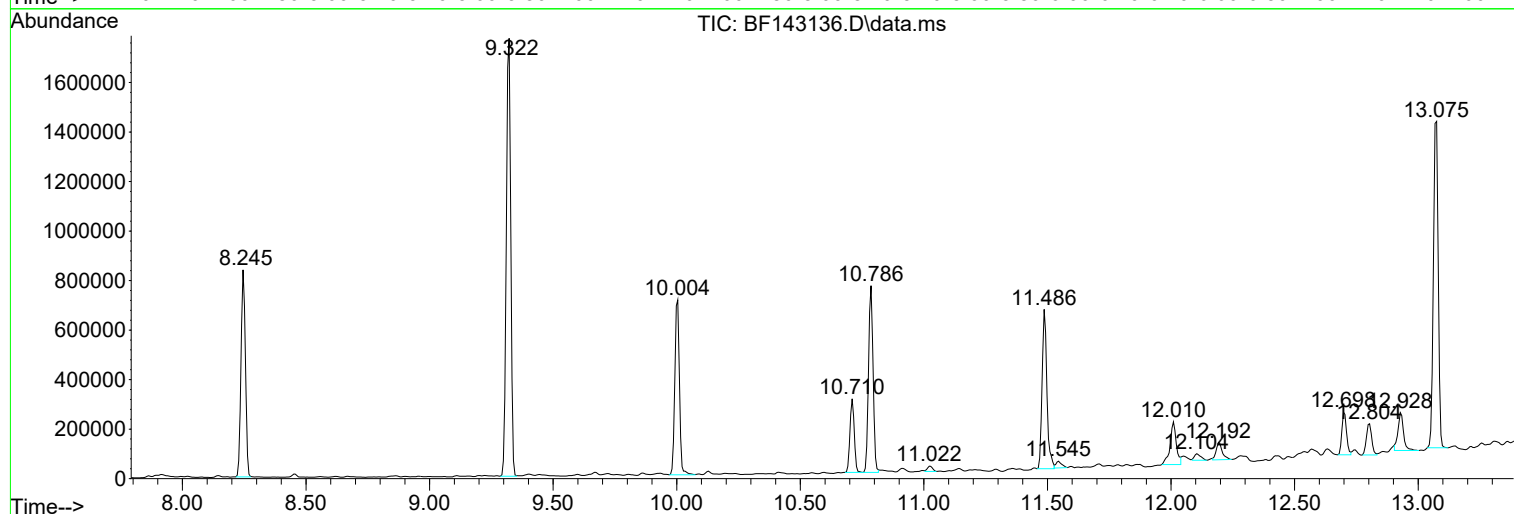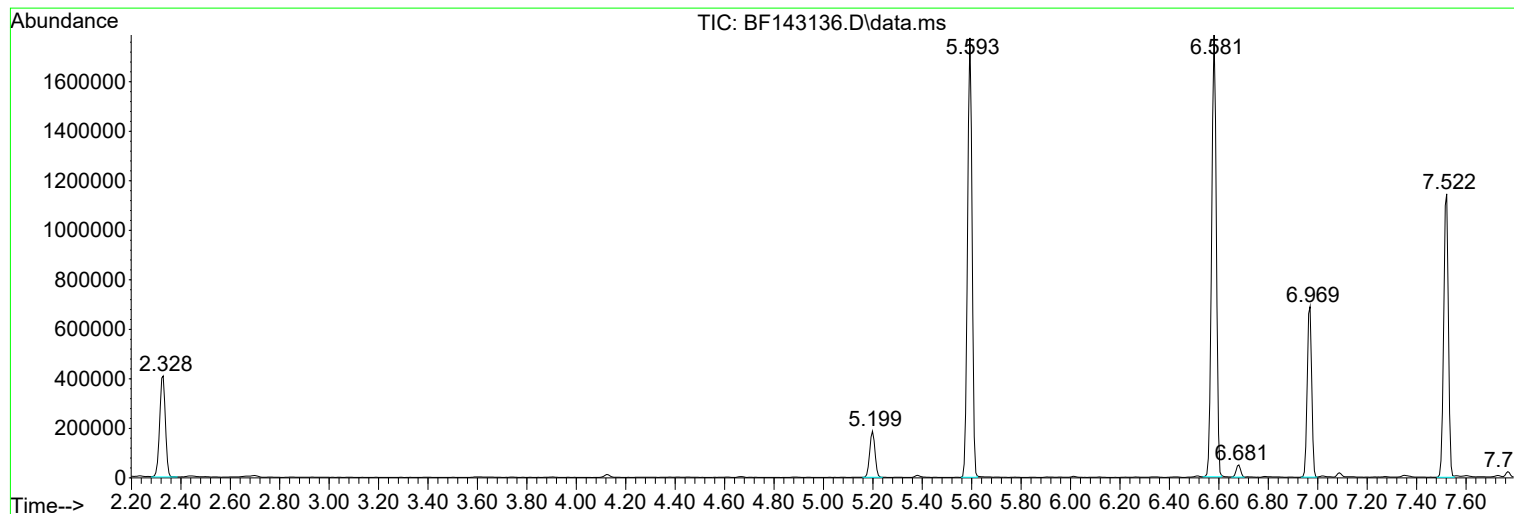

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071625\
Data File : BF143136.D
Acq On : 17 Jul 2025 05:00
Operator : RC/JU
Sample : Q2558-03
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-TS-Grillo-OG-070925

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF071525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071625\
Data File : BF143136.D
Acq On : 17 Jul 2025 05:00
Operator : RC/JU
Sample : Q2558-03
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-TS-Grillo-OG-070925

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF071525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc