


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071525\
Data File : BM050446.D
Acq On : 15 Jul 2025 08:11
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM070925.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Jul 08 18:32:25 2025

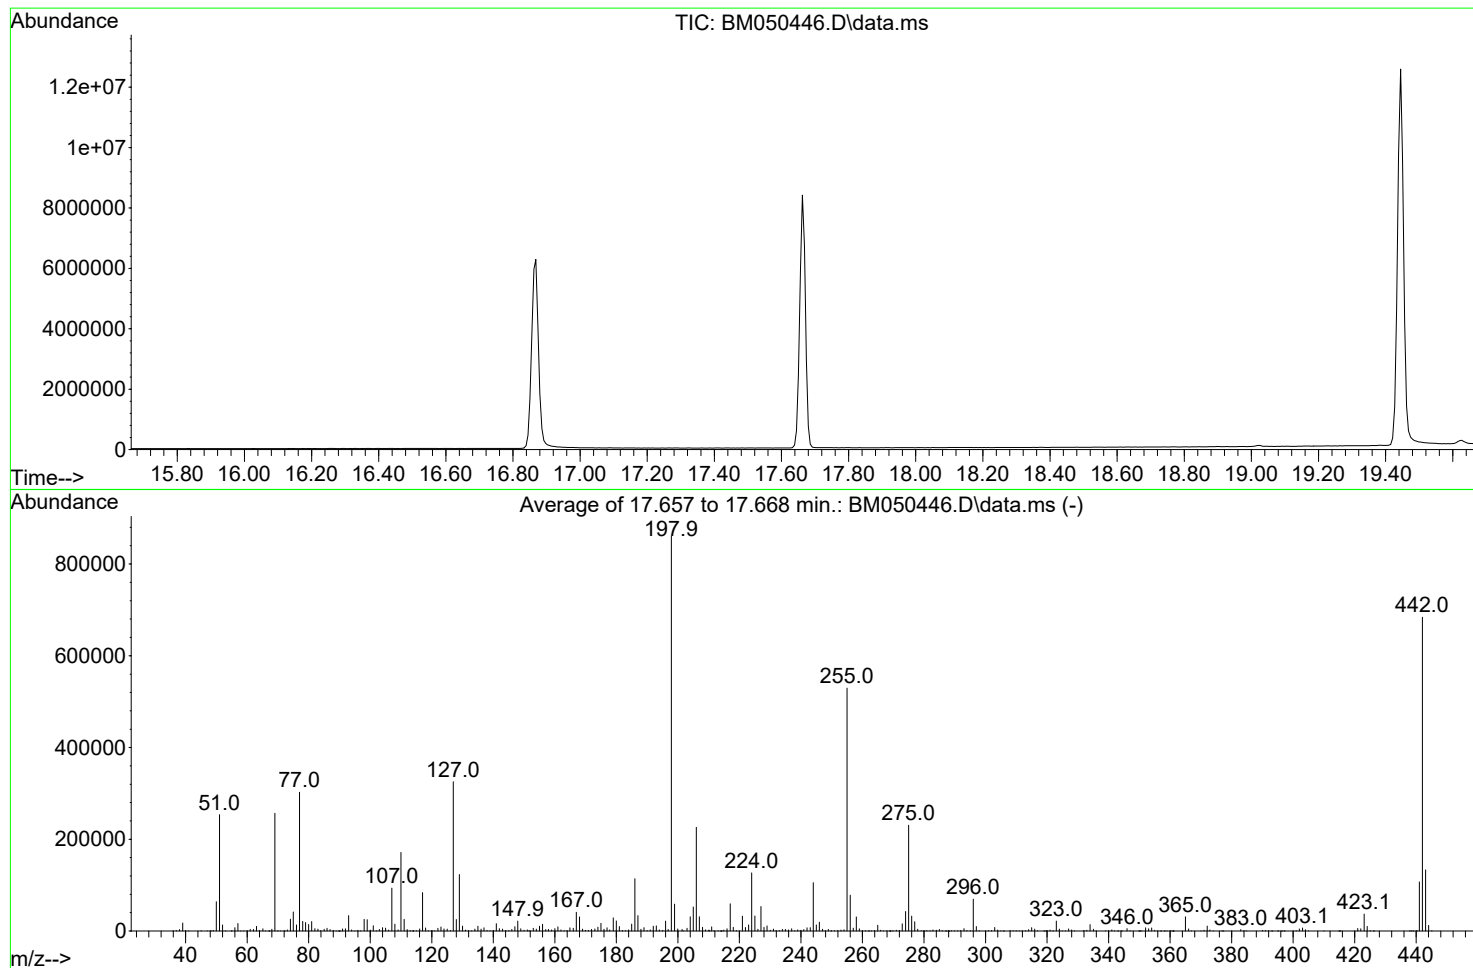

AutoFind: Scans 2494, 2495, 2496; Background Corrected with Scan 2486

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
68	69	0.00	2	1.6	3993	PASS
69	69	100	100	100.0	256824	PASS
70	69	0.00	2	0.5	1237	PASS
197	198	0.00	2	0.4	3574	PASS
198	198	100	100	100.0	860736	PASS
199	198	5	9	6.8	58565	PASS
365	198	1	100	3.6	30960	PASS
441	443	0.01	150	80.3	107000	PASS
442	442	100	100	100.0	683861	PASS
443	442	15	24	19.5	133181	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
7/15/2025	BNA_M	<u>BM050446.D</u>
Compound Name	Response	Retention Time
DDT	3019774	20.68
DDD	73691	20.239
DDE	2559	19.745
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
76250	3096024	2.46

Instrument :
BNA_M
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071525\
Data File : BM050446.D
Acq On : 15 Jul 2025 08:11
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Jul 15 10:52:38 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM070925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 08 18:32:25 2025
Response via : Initial Calibration

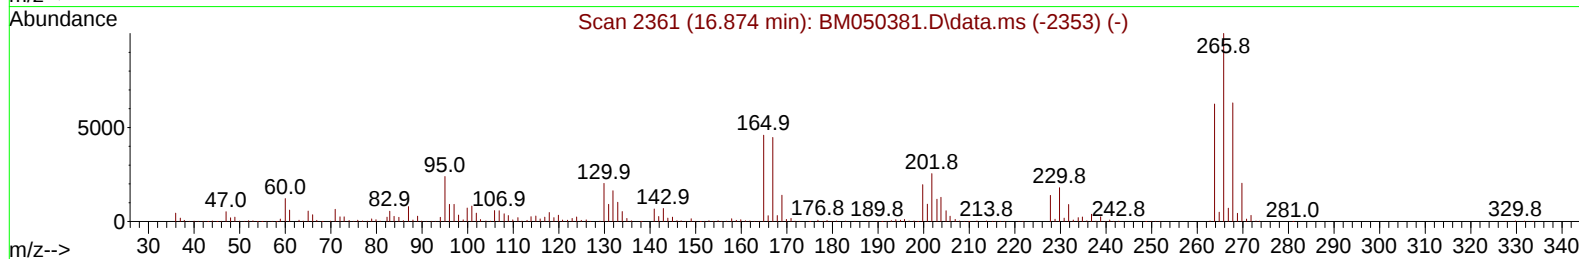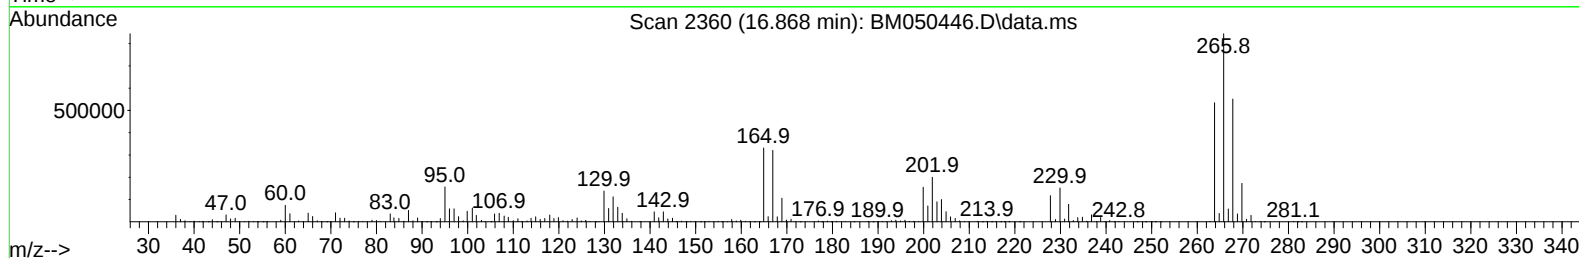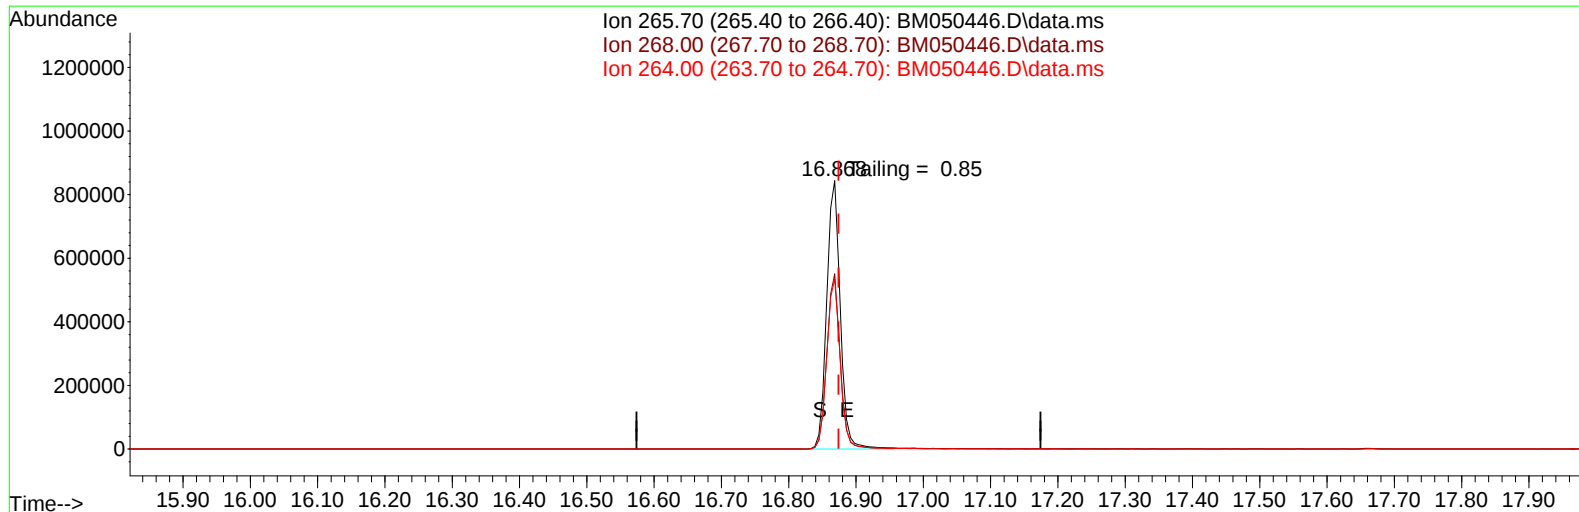

TIC: BM050446.D\data.ms

(70) Pentachlorophenol (C)

16.868min (-0.006) 502476.02 ng




response 1184472

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	65.29
264.00	62.40	63.35
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071525\
Data File : BM050446.D
Acq On : 15 Jul 2025 08:11
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Jul 15 10:52:38 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM070925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 08 18:32:25 2025
Response via : Initial Calibration

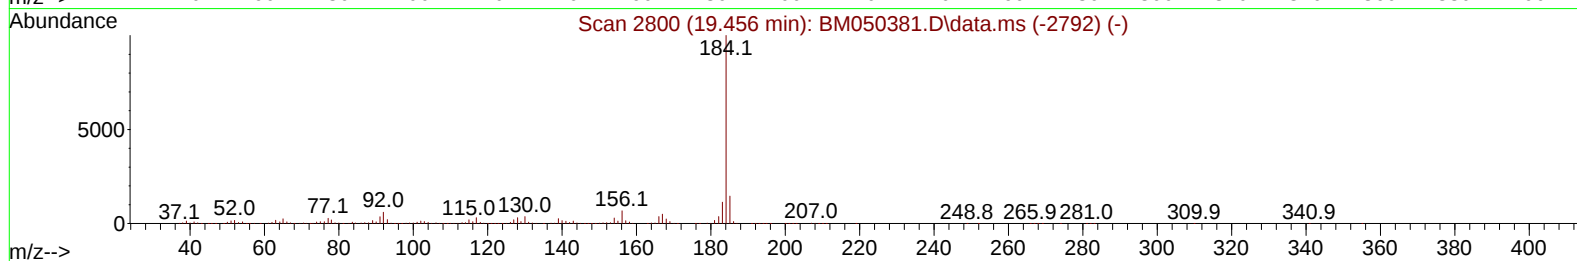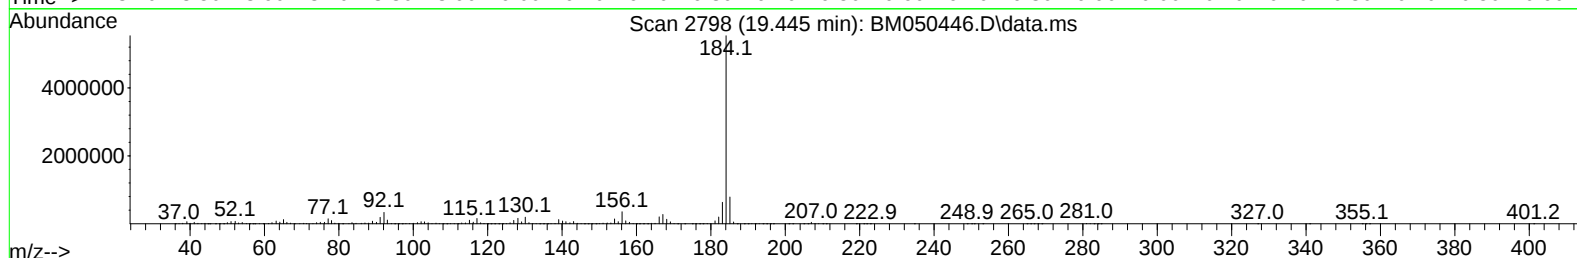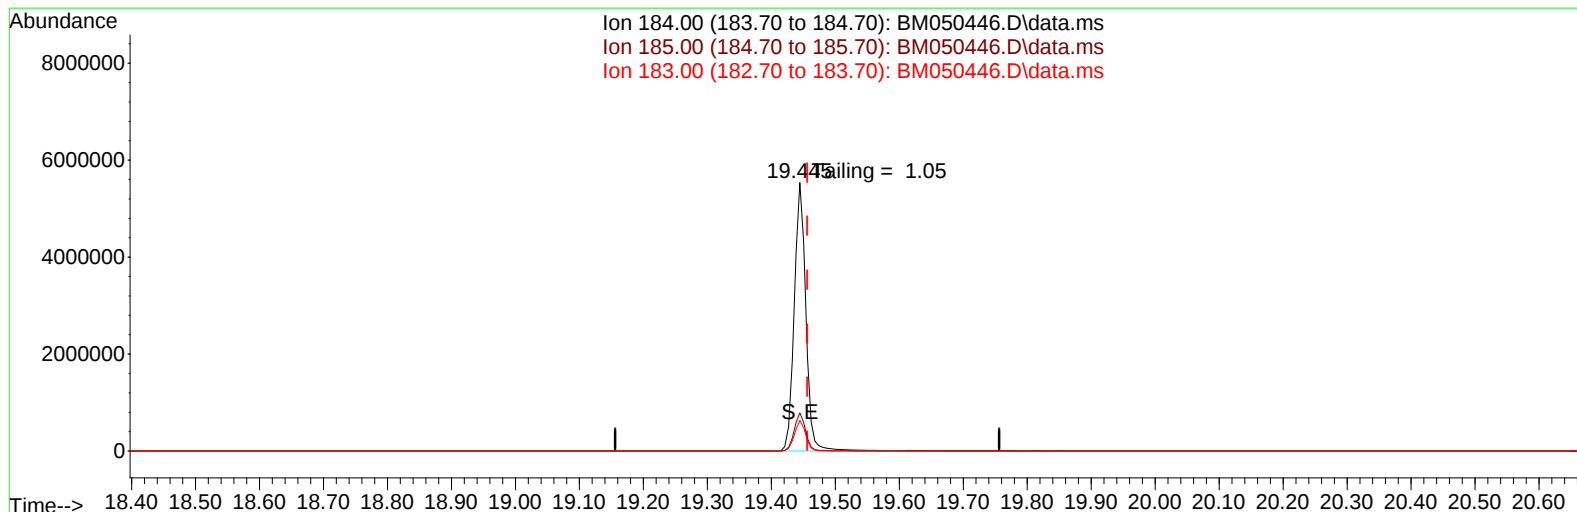

TIC: BM050446.D\data.ms

(77) Benzidine

19.445min (-0.012) 90011.87 ng

response 7016203

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.20
183.00	11.30	11.39
0.00	0.00	0.00