


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071125\
Data File : BN037465.D
Acq On : 11 Jul 2025 08:36
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN071125.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Jul 11 15:38:34 2025

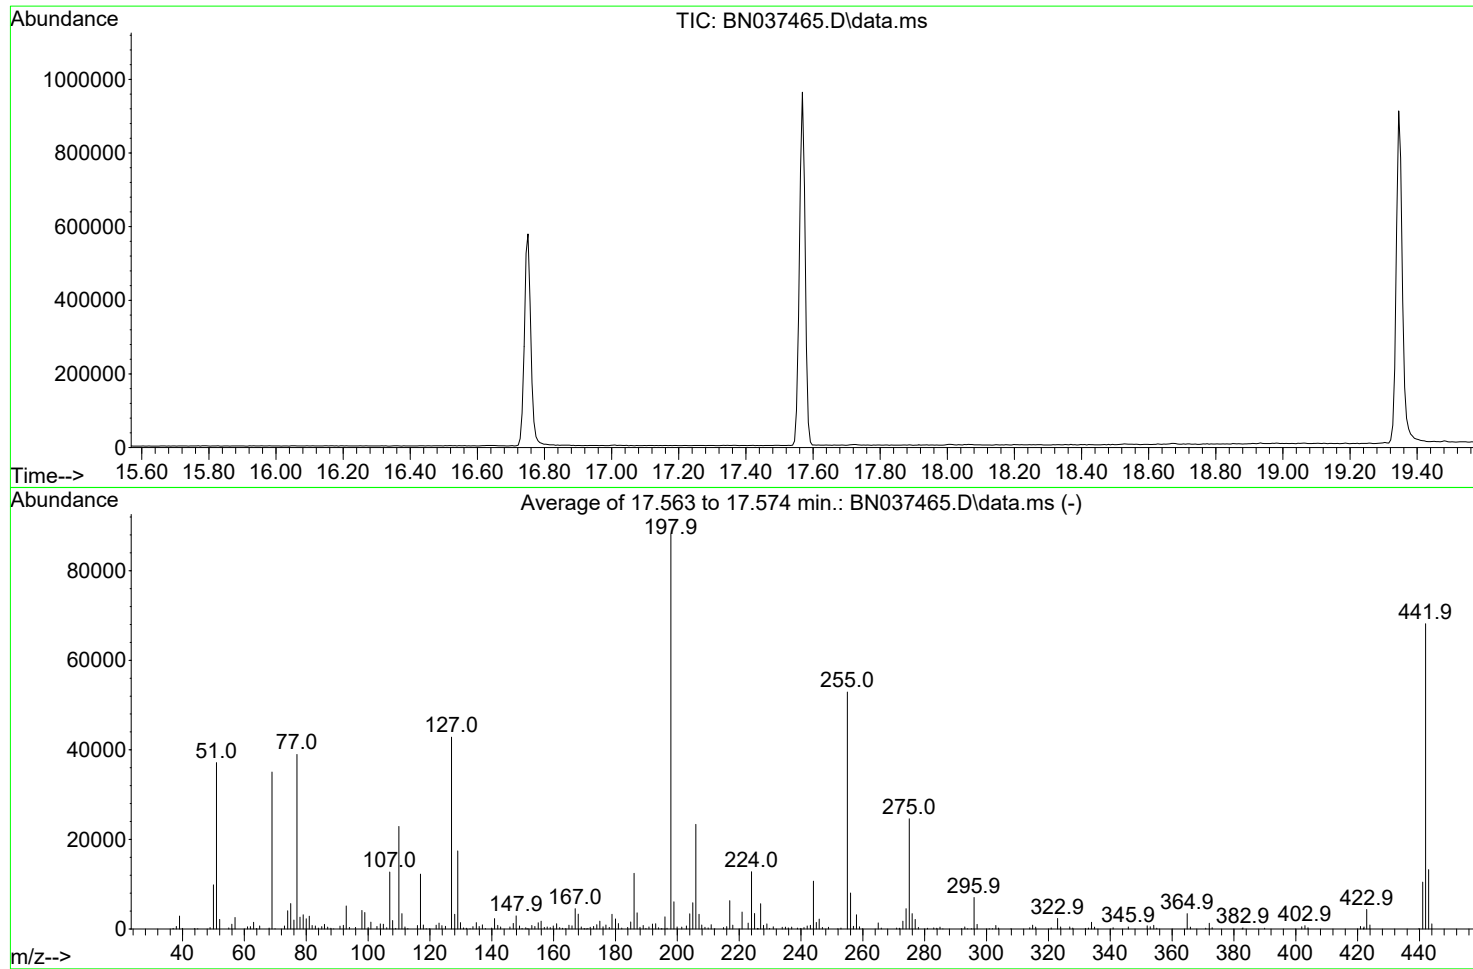

AutoFind: Scans 2461, 2462, 2463; Background Corrected with Scan 2454

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
68	69	0.00	2	0.6	212	PASS
69	69	100	100	100.0	35043	PASS
70	69	0.00	2	0.3	88	PASS
197	198	0.00	2	0.2	180	PASS
198	198	100	100	100.0	88163	PASS
199	198	5	9	6.9	6064	PASS
365	198	1	100	3.9	3416	PASS
441	443	0.01	150	78.9	10453	PASS
442	442	100	100	100.0	68157	PASS
443	442	15	24	19.4	13251	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
7/11/2025	BNA_N	<u>BN037465.D</u>
Compound Name	Response	Retention Time
DDT	193083	20.598
DDD	2276	20.21
DDE	169	19.645
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
2445	195528	1.25

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071125\
Data File : BN037465.D
Acq On : 11 Jul 2025 08:36
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jul 11 16:46:09 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 10 02:20:59 2025
Response via : Initial Calibration

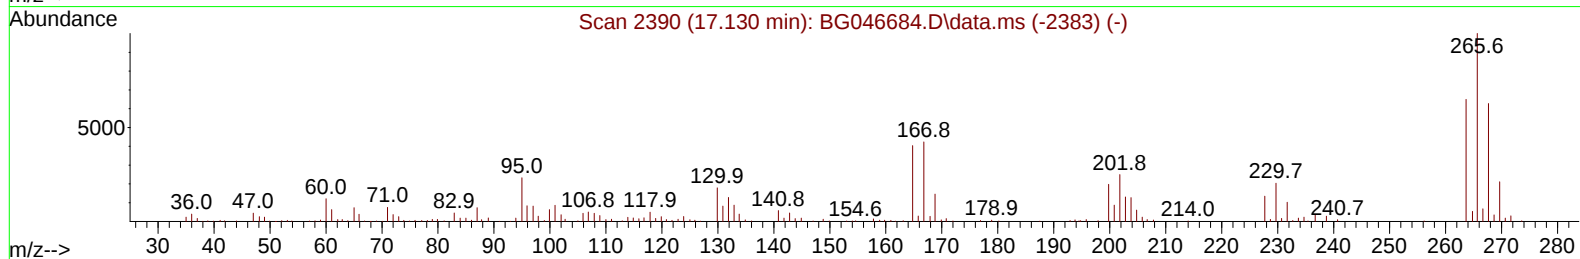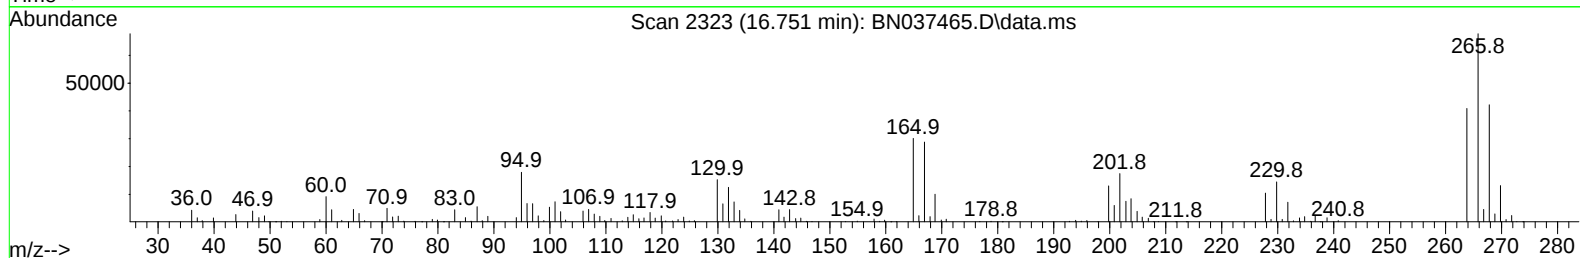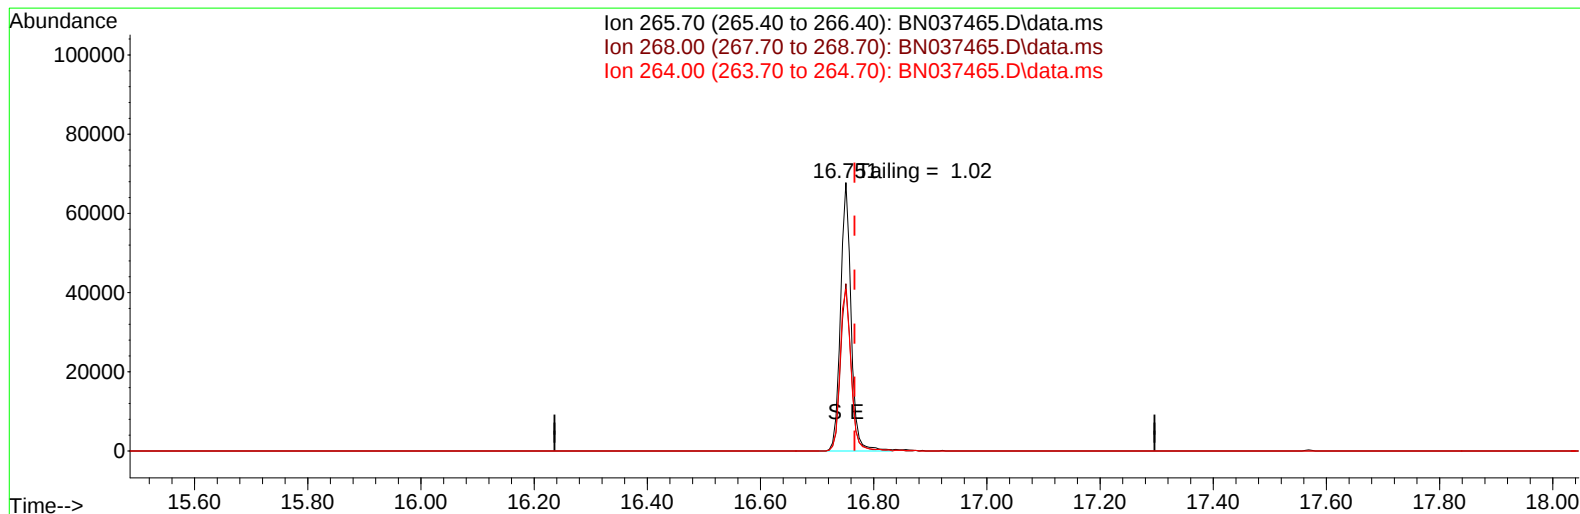

TIC: BN037465.D\data.ms

(70) Pentachlorophenol (C)

16.751min (-0.015) 19733.94 ng




response 87345

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.30
264.00	61.60	60.32
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071125\
Data File : BN037465.D
Acq On : 11 Jul 2025 08:36
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jul 11 16:46:09 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 10 02:20:59 2025
Response via : Initial Calibration

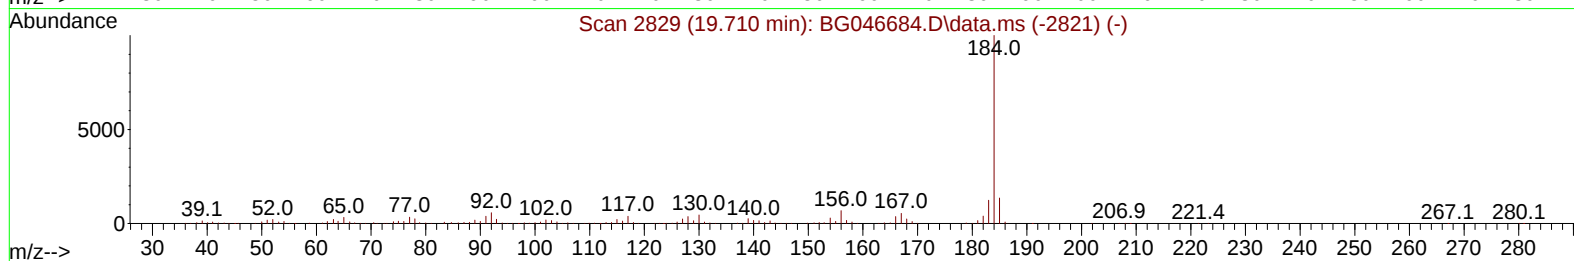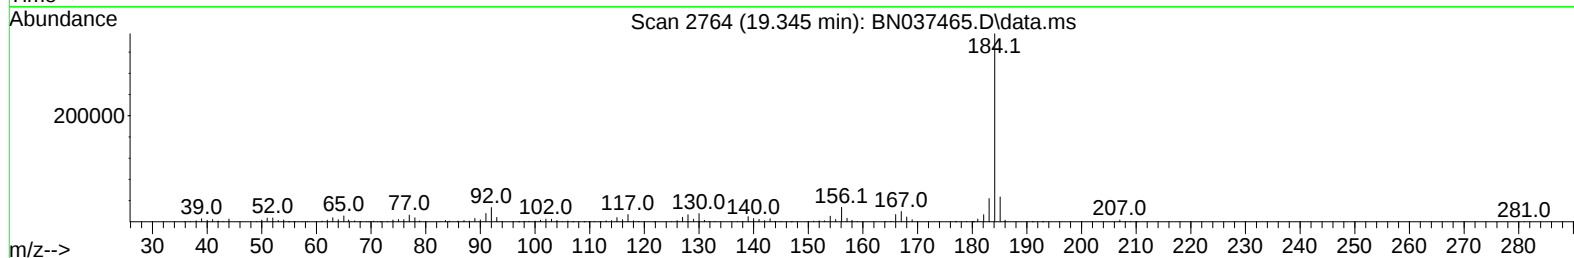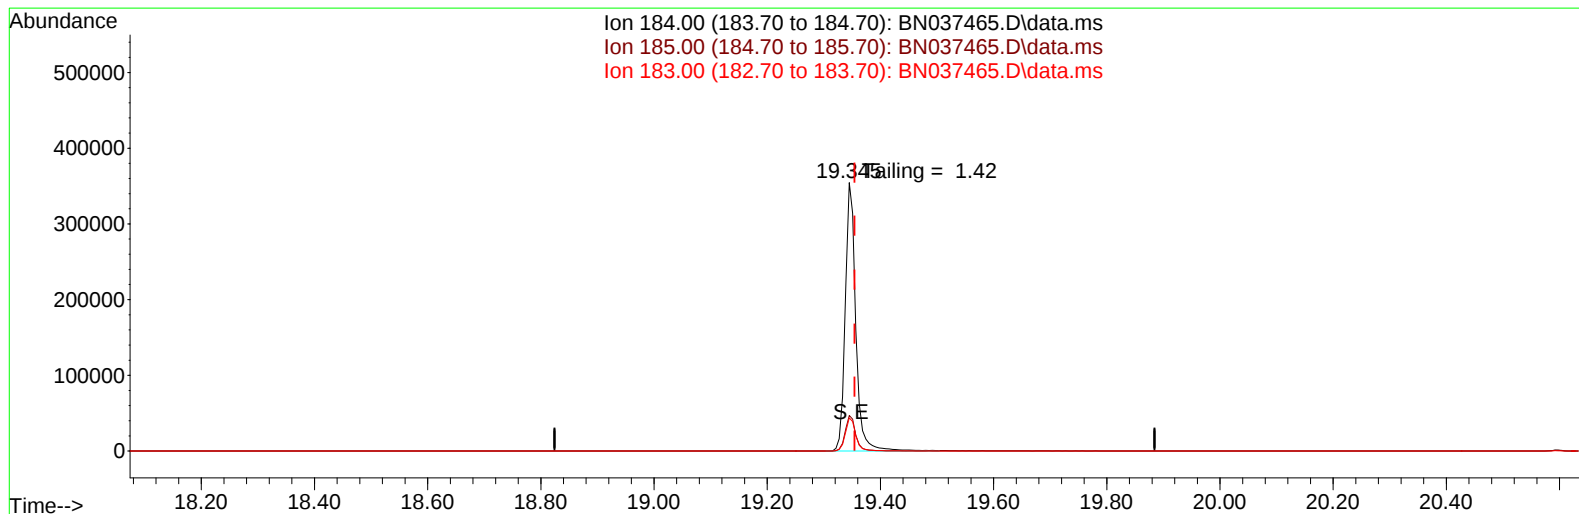

TIC: BN037465.D\data.ms

(77) Benzidine

19.345min (-0.009) 0.00 ng

response 460569

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.26
183.00	13.20	12.35
0.00	0.00	0.00