


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071425\
Data File : BN037482.D
Acq On : 14 Jul 2025 08:31
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN071125.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Jul 11 15:38:34 2025

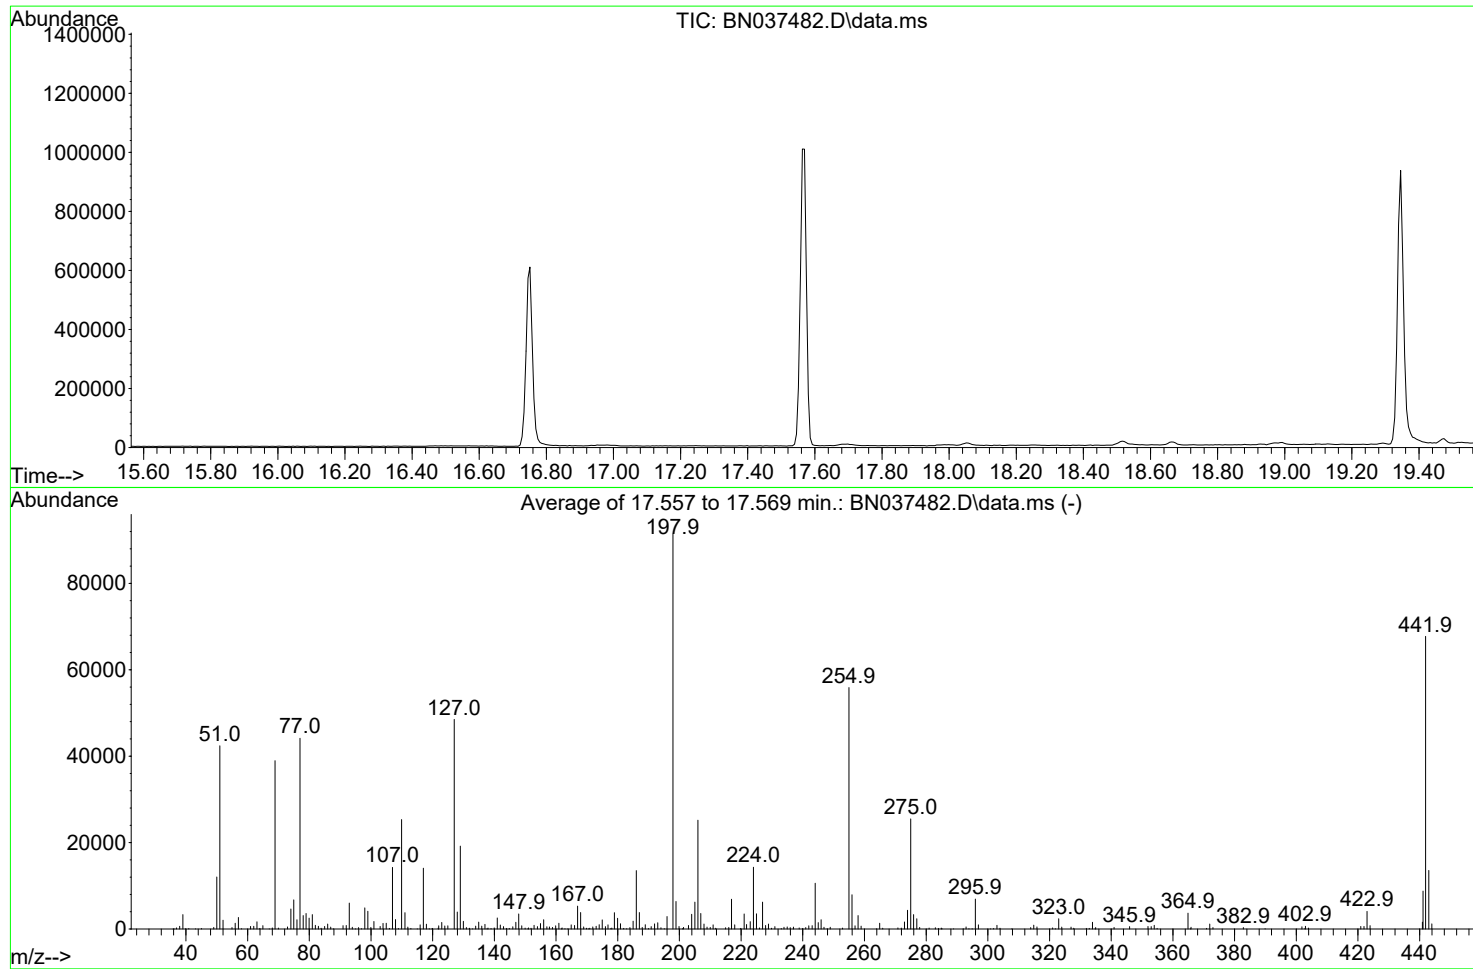

AutoFind: Scans 2460, 2461, 2462; Background Corrected with Scan 2454

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	0.7	271	PASS
69	69	100	100	100.0	38979	PASS
70	69	0.00	2	0.6	223	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	91384	PASS
199	198	5	9	7.0	6375	PASS
365	198	1	100	4.0	3663	PASS
441	443	0.01	150	64.7	8781	PASS
442	442	100	100	100.0	67717	PASS
443	442	15	24	20.0	13573	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
7/14/2025	BNA_N	<u>BN037482.D</u>
Compound Name	Response	Retention Time
DDT	217524	20.592
DDD	2566	20.204
DDE	509	19.645
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3075	220599	1.39

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071425\
Data File : BN037482.D
Acq On : 14 Jul 2025 08:31
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jul 14 15:18:31 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 10 02:20:59 2025
Response via : Initial Calibration

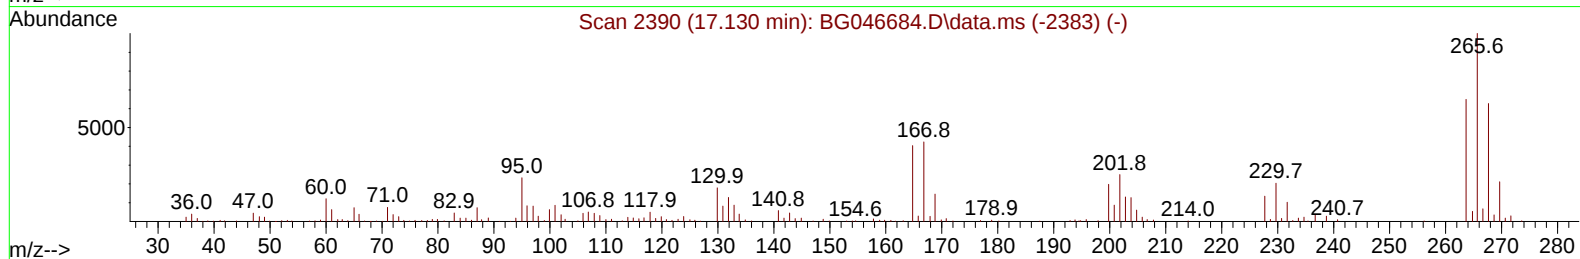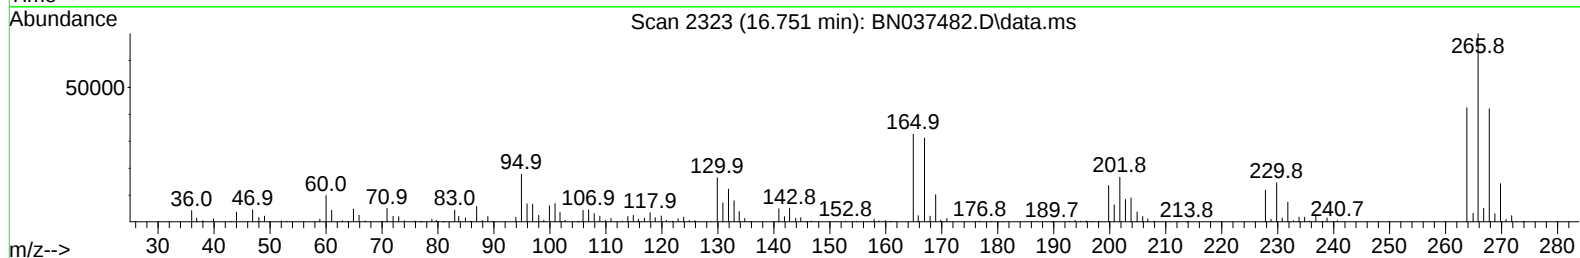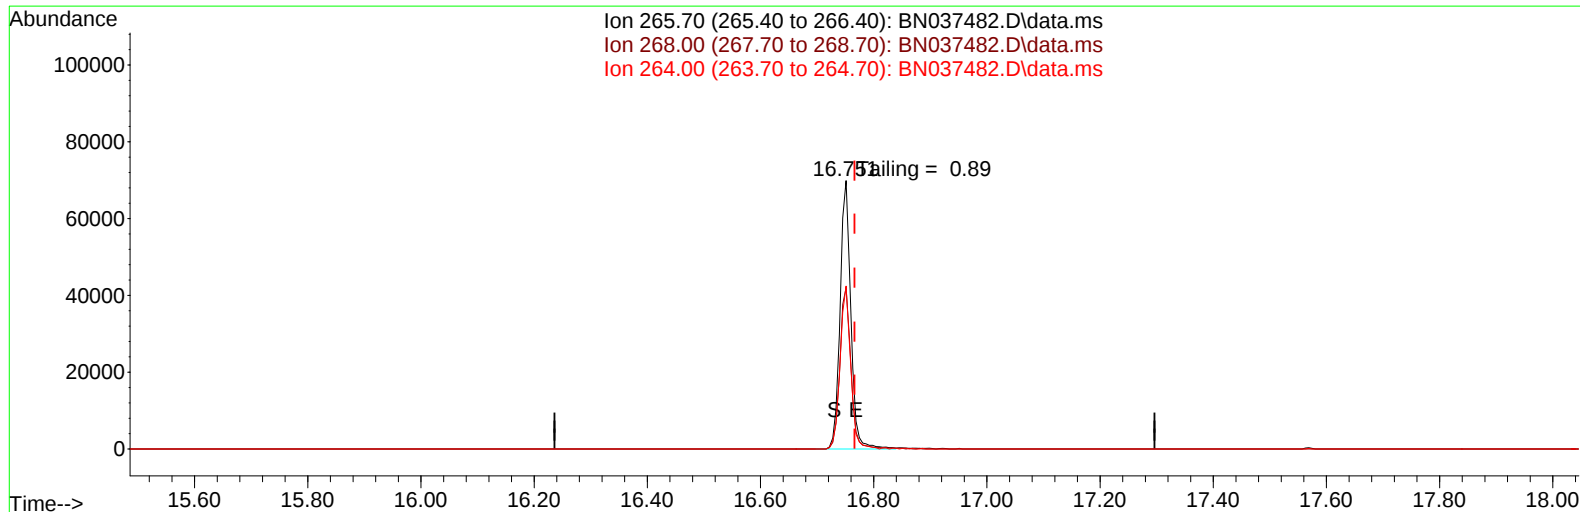

TIC: BN037482.D\data.ms

(70) Pentachlorophenol (C)

16.751min (-0.015) 23296.92 ng




response 91597

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	60.19
264.00	61.60	60.71
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071425\
Data File : BN037482.D
Acq On : 14 Jul 2025 08:31
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jul 14 15:18:31 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 10 02:20:59 2025
Response via : Initial Calibration

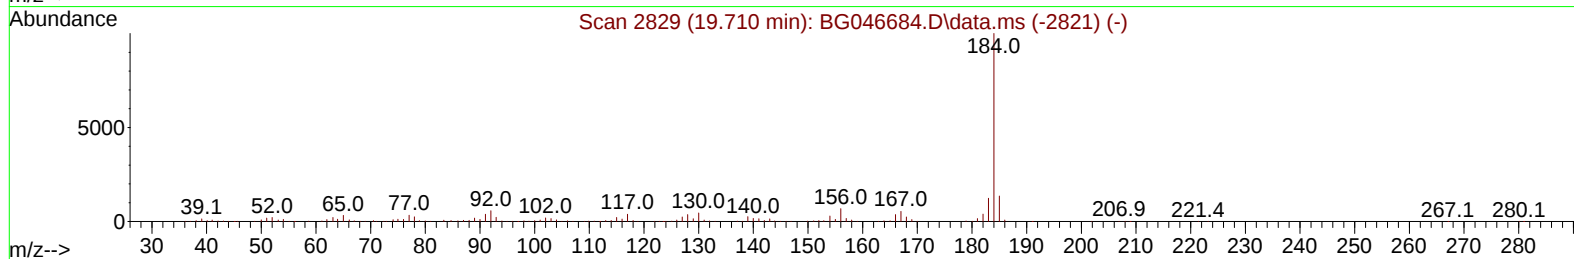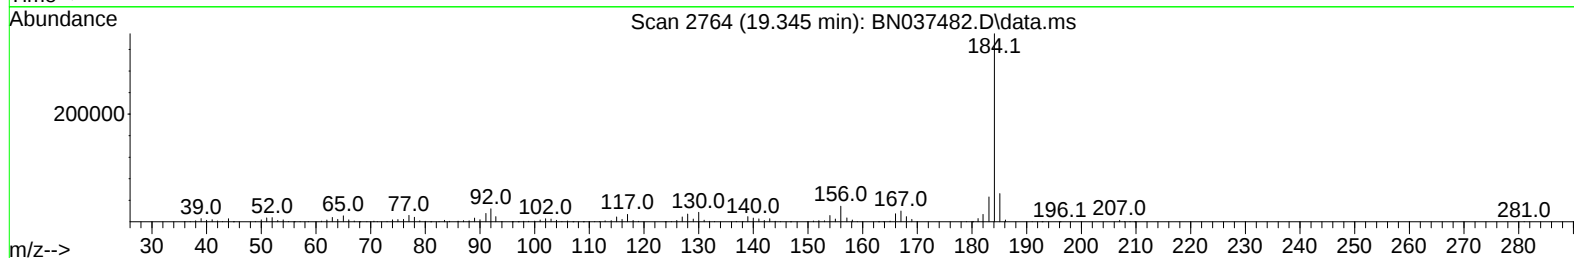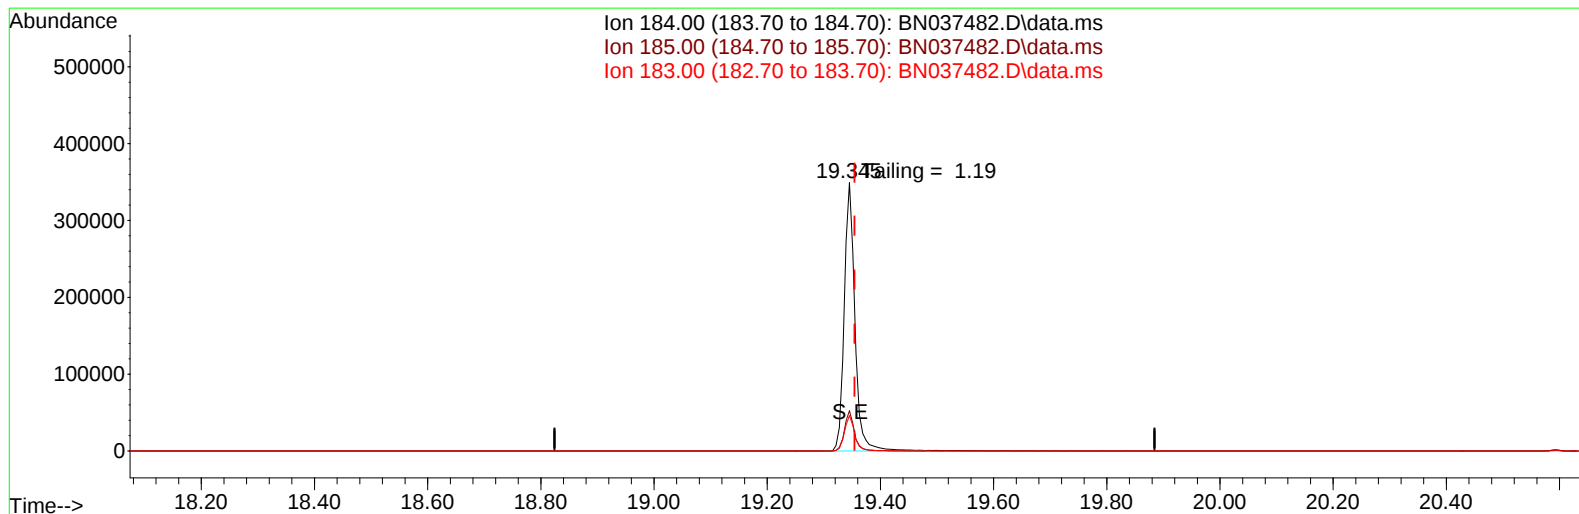

TIC: BN037482.D\data.ms

(77) Benzidine

19.345min (-0.009) 0.00 ng

response 459420

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	15.04
183.00	13.20	13.23
0.00	0.00	0.00