

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_Q\Data\PQ071625\  
Data File : PQ070545.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 16 Jul 2025 10:45  
Operator : YP\AJ  
Sample : Q2501-13  
Misc :  
ALS Vial : 5 Sample Multiplier: 1

Instrument :  
ECD\_Q  
ClientSampleId :  
PCB-GPC2-BLANK

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Jul 16 16:25:48 2025  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_Q\Method\PQ071425CLP.M  
Quant Title : GC EXTRACTABLES  
QLast Update : Mon Jul 14 15:40:06 2025  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 µl  
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2  
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

| Compound | RT#1 | RT#2 | Resp#1 | Resp#2 | ng/ml | ng/ml |
|----------|------|------|--------|--------|-------|-------|
|----------|------|------|--------|--------|-------|-------|

-----  
System Monitoring Compounds

Target Compounds  
-----



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_Q\Data\PQ071625\  
Data File : PQ070545.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 16 Jul 2025 10:45  
Operator : YP\AJ  
Sample : Q2501-13  
Misc :  
ALS Vial : 5 Sample Multiplier: 1

Instrument :  
ECD\_Q  
ClientSampleId :  
PCB-GPC2-BLANK

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Jul 16 16:25:48 2025  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_Q\Method\PQ071425CLP.M  
Quant Title : GC EXTRACTABLES  
QLast Update : Mon Jul 14 15:40:06 2025  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1  $\mu$ l  
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2  
Signal #1 Info : 30Mx0.32mmx 0.5 $\mu$ m Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

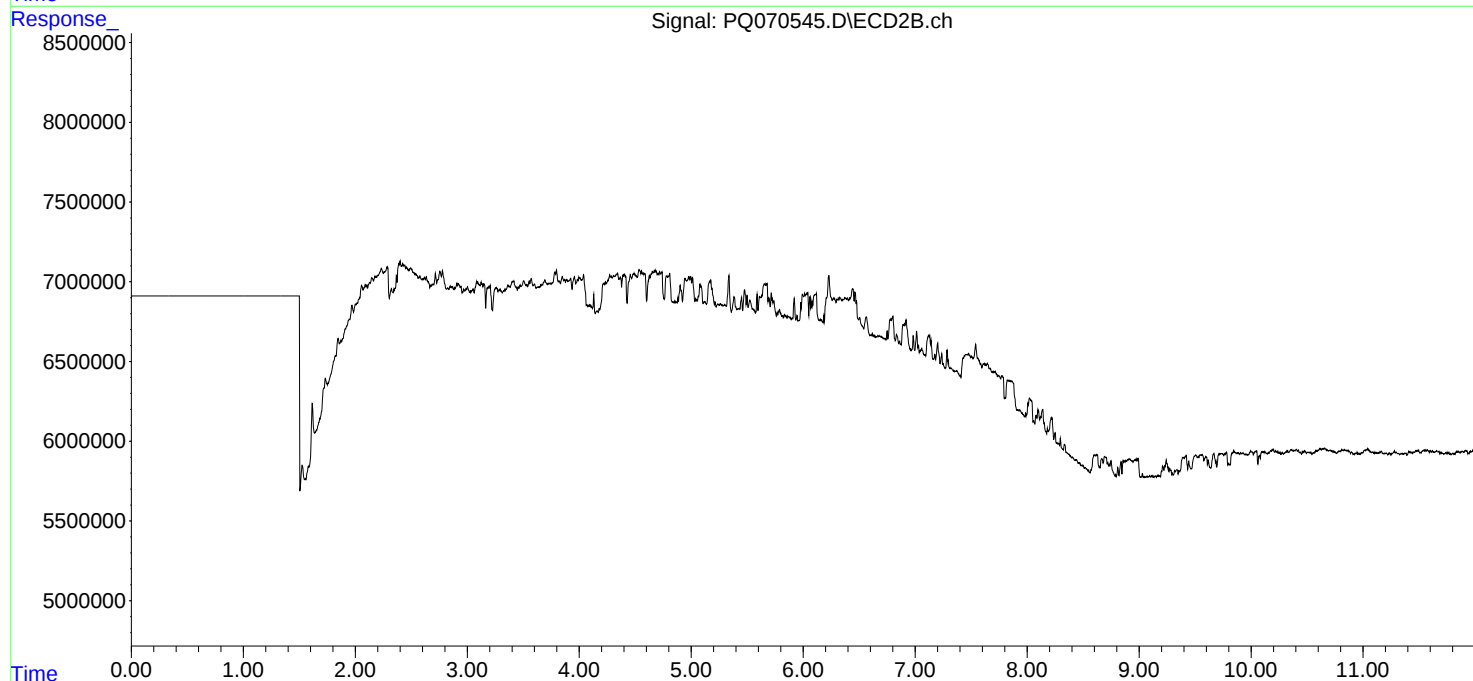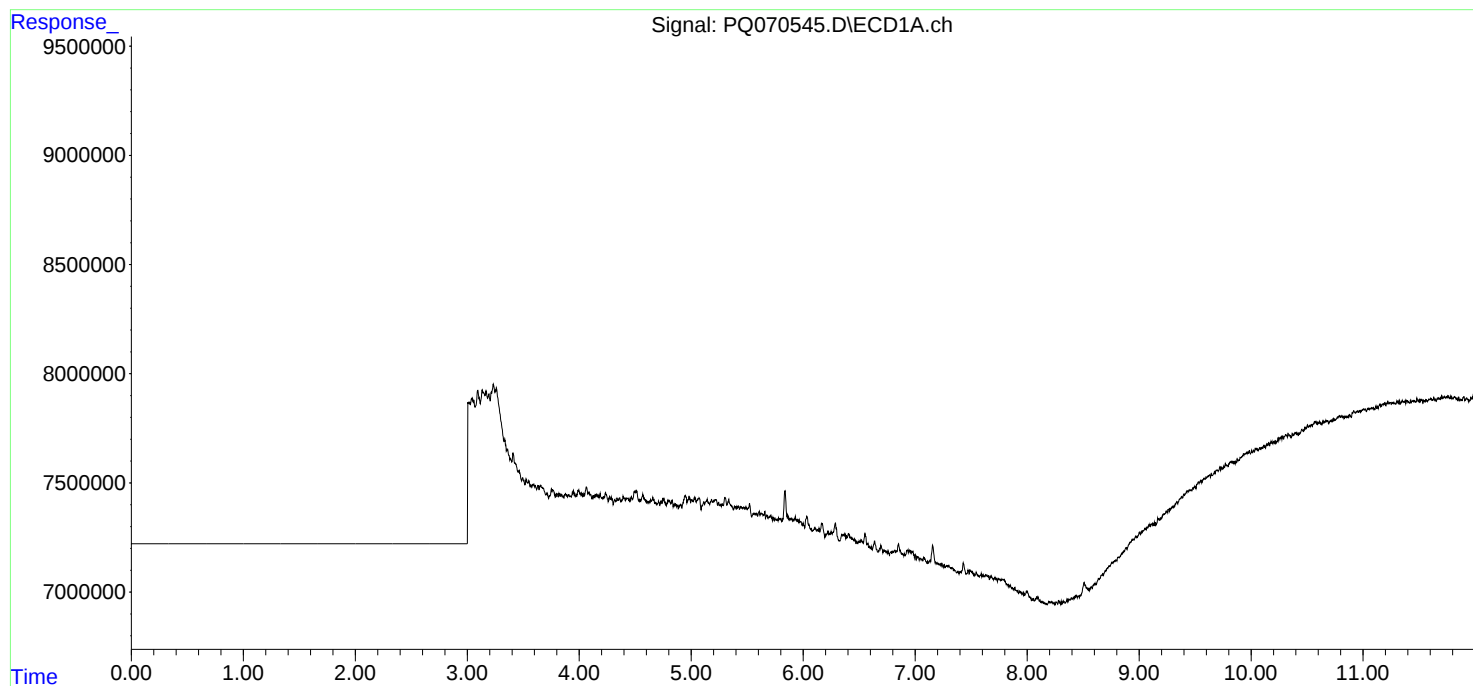


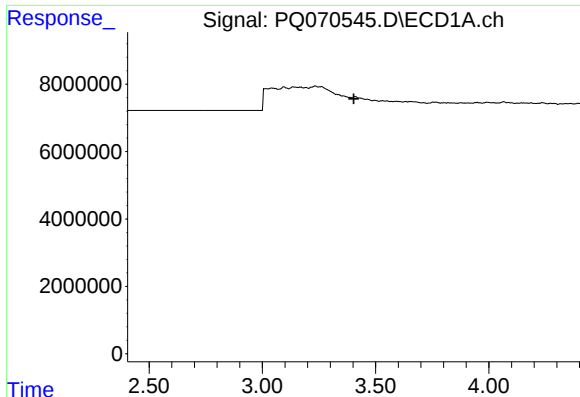

#1 Tetrachloro-m-xylene


R.T.: 0.000 min  
Exp R.T. : 3.404 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_Q  
ClientSampleId :  
PCB-GPC2-BLANK

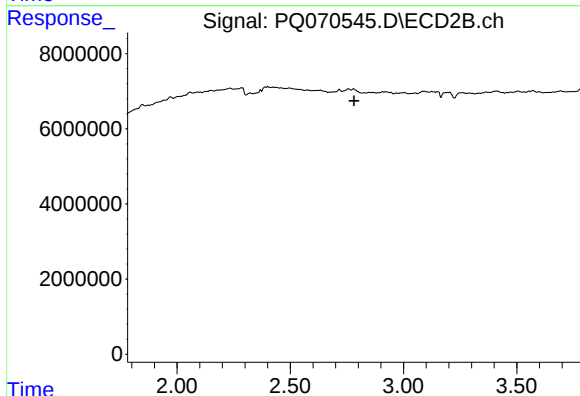


#1 Tetrachloro-m-xylene

R.T.: 0.000 min  
Exp R.T. : 2.781 min  
Response: 0  
Conc: N.D.

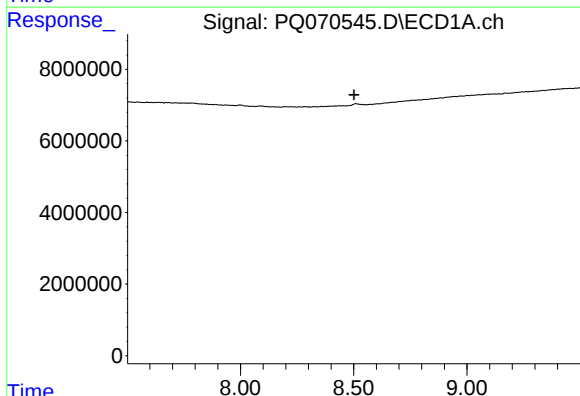

#2 Decachlorobiphenyl

R.T.: 0.000 min  
Exp R.T. : 8.502 min  
Response: 0  
Conc: N.D.

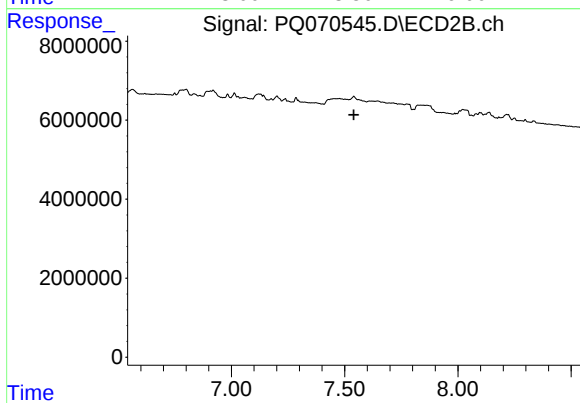

#2 Decachlorobiphenyl

R.T.: 0.000 min  
Exp R.T. : 7.540 min  
Response: 0  
Conc: N.D.