


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071825\
Data File : BN037519.D
Acq On : 18 Jul 2025 11:59
Operator : RC/JU
Sample : DFTPP380
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP380

Integration File: LSCINT.P

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN071825.MA.M
Title : SVOA CALIBRATION
Last Update : Fri Jul 18 16:22:45 2025

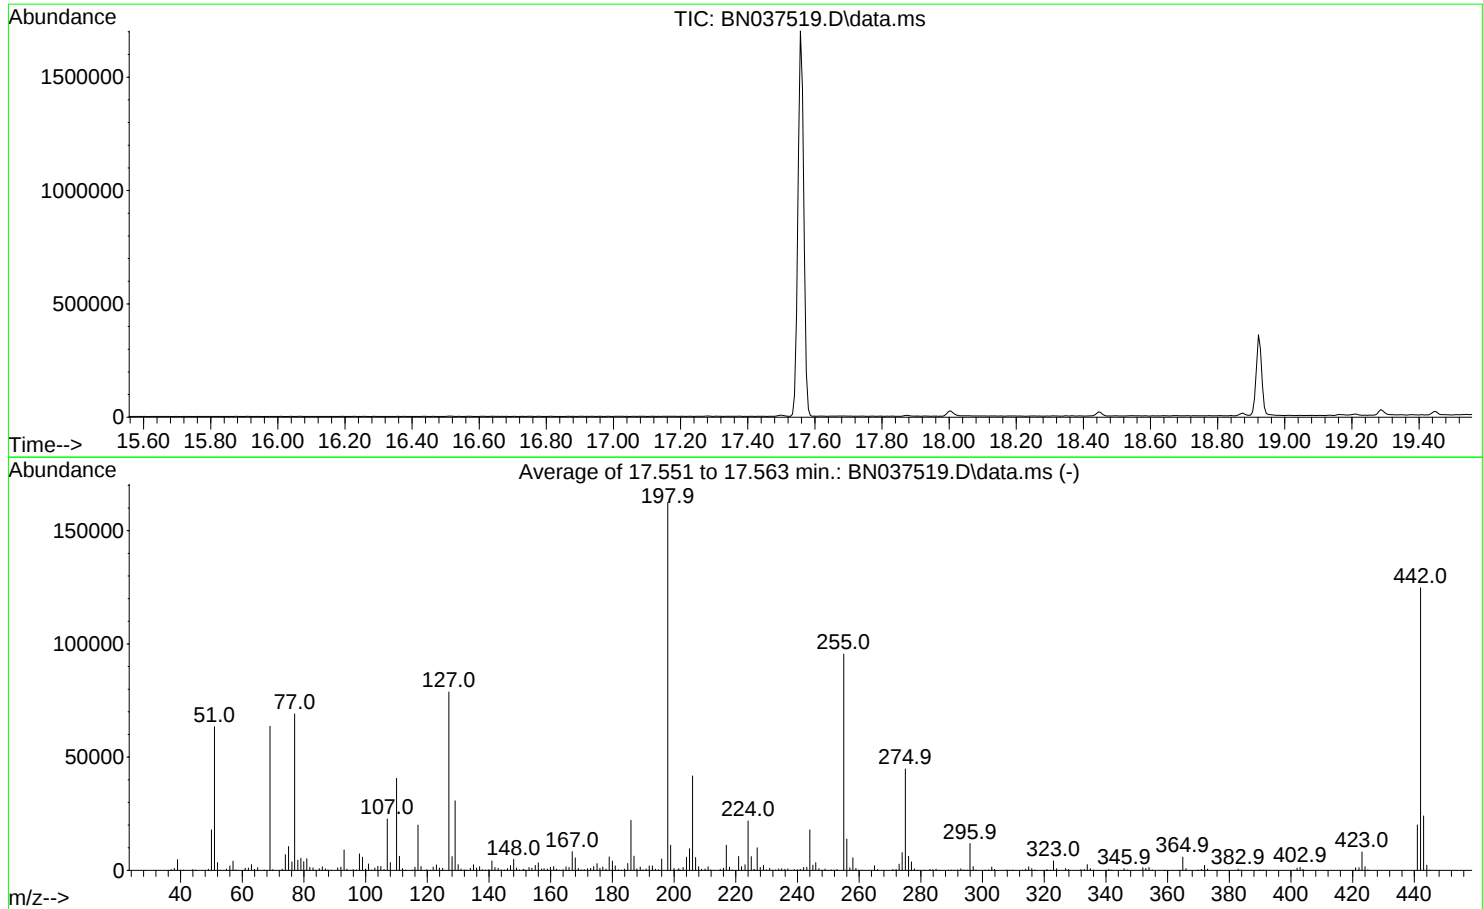

AutoFind: Scans 2459, 2460, 2461; Background Corrected with Scan 2454

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.1	63459	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	39.2	63693	PASS
70	69	0.00	2	0.6	371	PASS
127	198	10	80	48.5	78768	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	162453	PASS
199	198	5	9	6.8	11073	PASS
275	198	10	60	27.6	44805	PASS
365	198	1	100	3.6	5878	PASS
441	198	0.01	100	12.4	20076	PASS
442	198	50	100	76.8	124784	PASS
443	442	15	24	19.3	24044	PASS