


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071725\
Data File : BM050473.D
Acq On : 17 Jul 2025 13:02
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270E-Tune.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Oct 07 11:38:17 2020

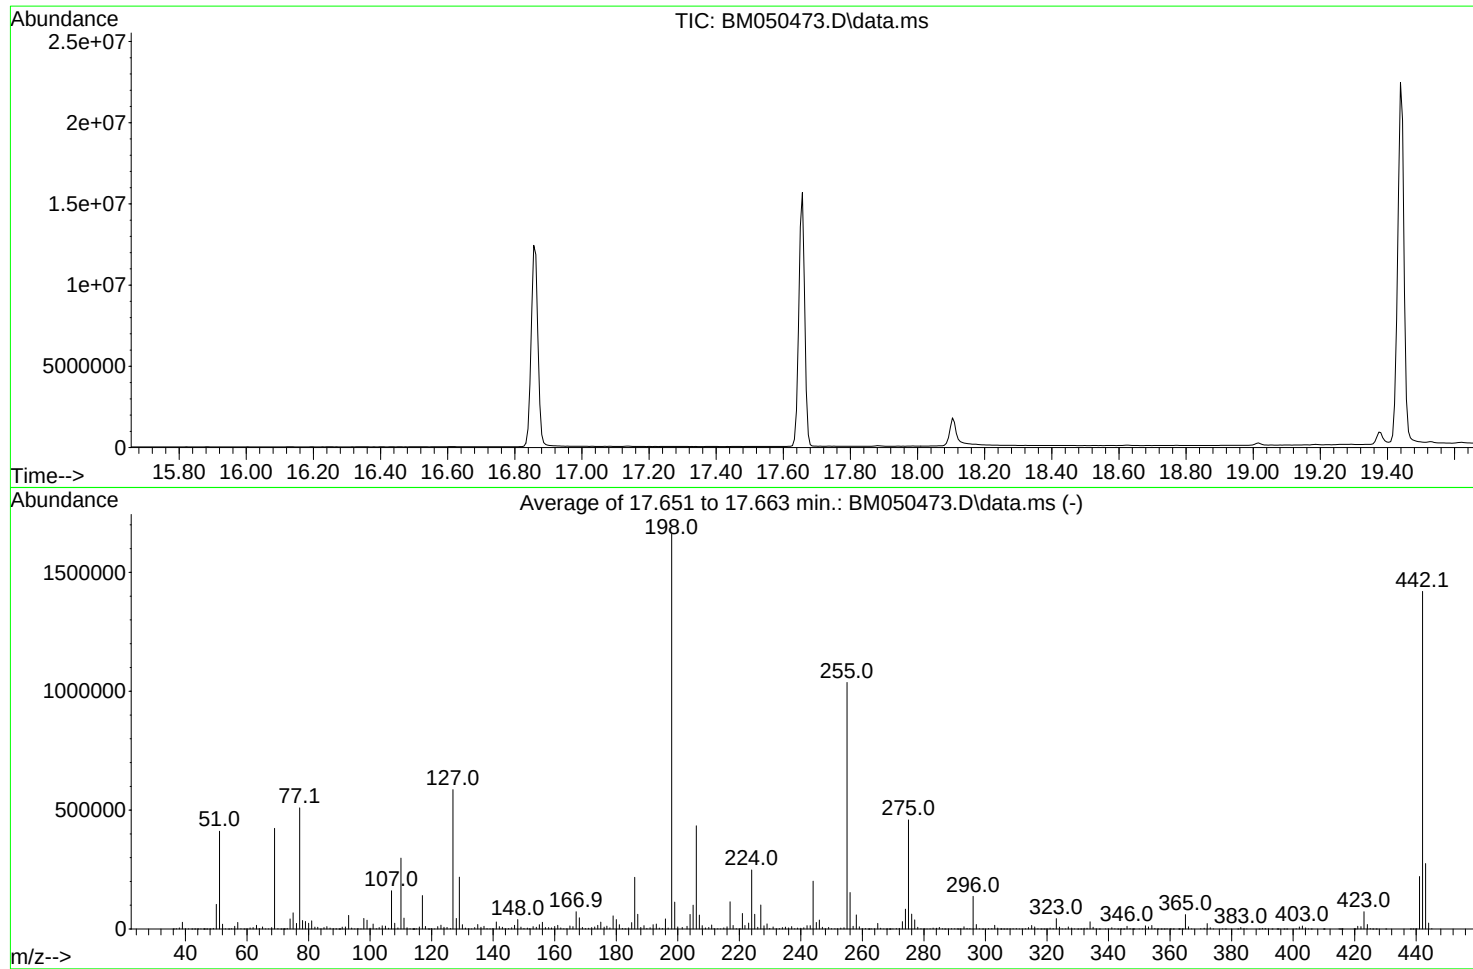




AutoFind: Scans 2493, 2494, 2495; Background Corrected with Scan 2485

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	1.5	6225	PASS
69	69	100	100	100.0	423672	PASS
70	69	0.00	2	0.5	2225	PASS
197	198	0.00	2	0.2	4012	PASS
198	198	100	100	100.0	1660757	PASS
199	198	5	9	6.8	113293	PASS
365	198	1	100	3.6	60509	PASS
441	443	0.01	150	80.2	220800	PASS
442	442	100	100	100.0	1419947	PASS
443	442	15	24	19.4	275179	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071725\
Data File : BM050473.D
Acq On : 17 Jul 2025 13:02
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Jul 17 16:24:15 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM070925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 17 16:20:15 2025
Response via : Initial Calibration

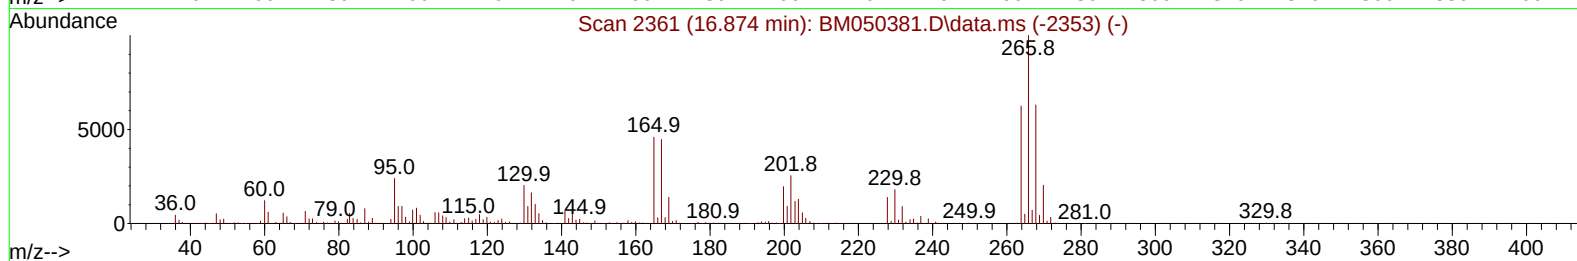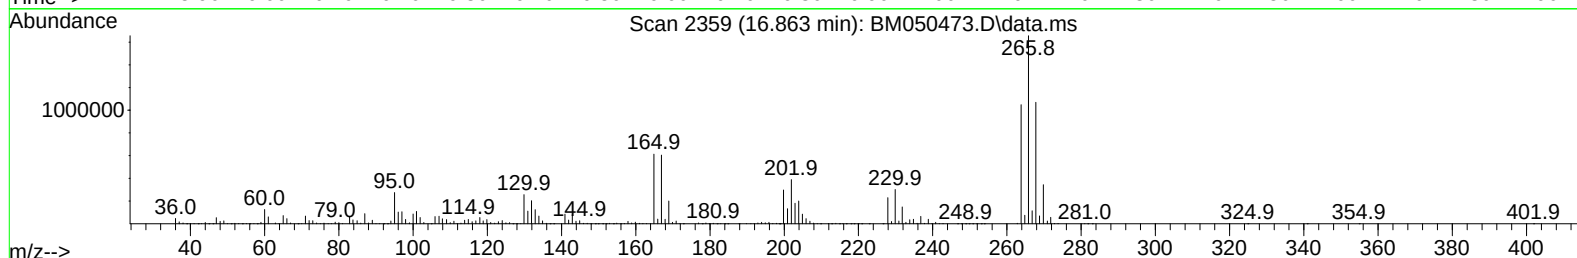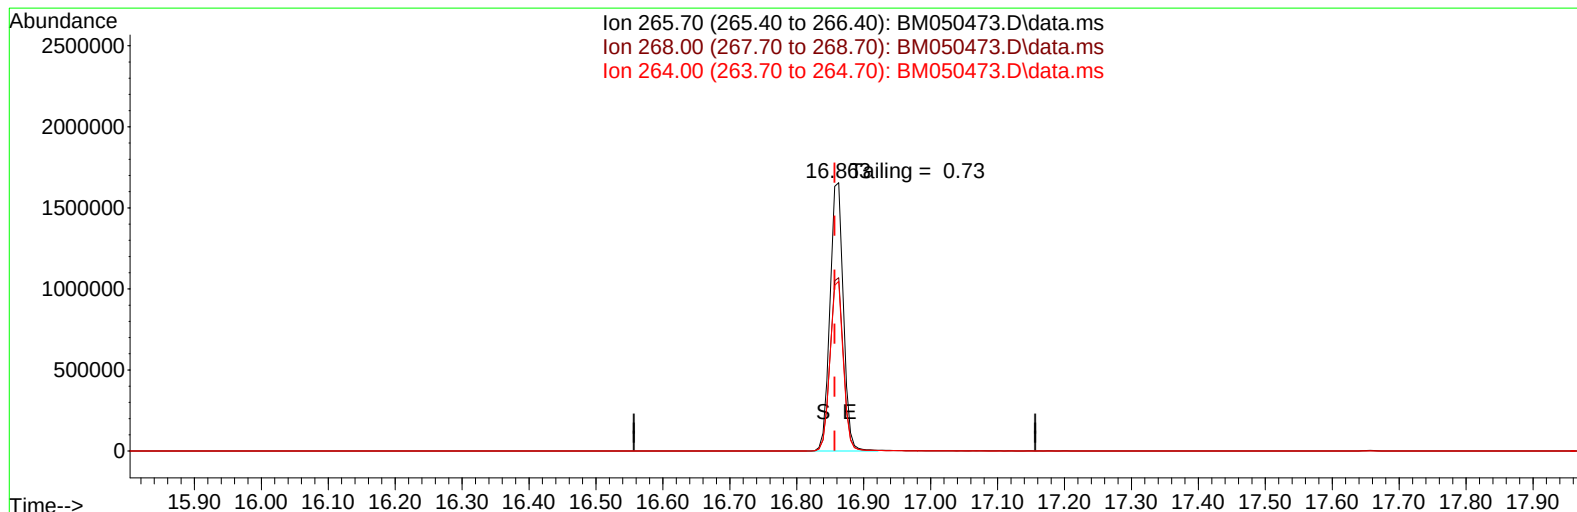

TIC: BM050473.D\data.ms

(70) Pentachlorophenol (C)

16.863min (+ 0.006) 343417.56 ng




response 2320091

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	64.56
264.00	62.40	63.28
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071725\
Data File : BM050473.D
Acq On : 17 Jul 2025 13:02
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Jul 17 16:24:15 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM070925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 17 16:20:15 2025
Response via : Initial Calibration

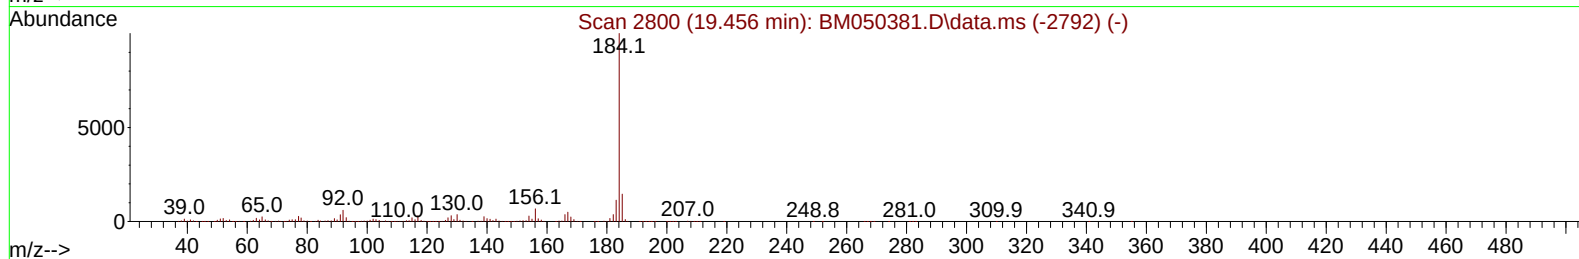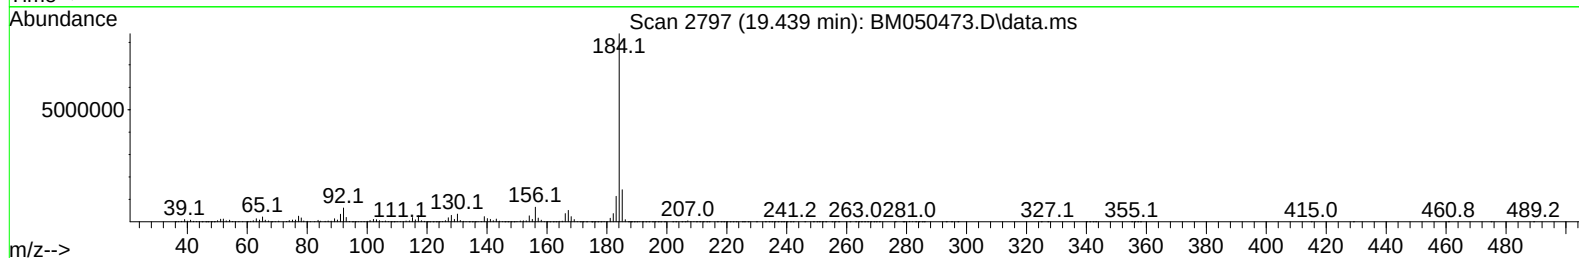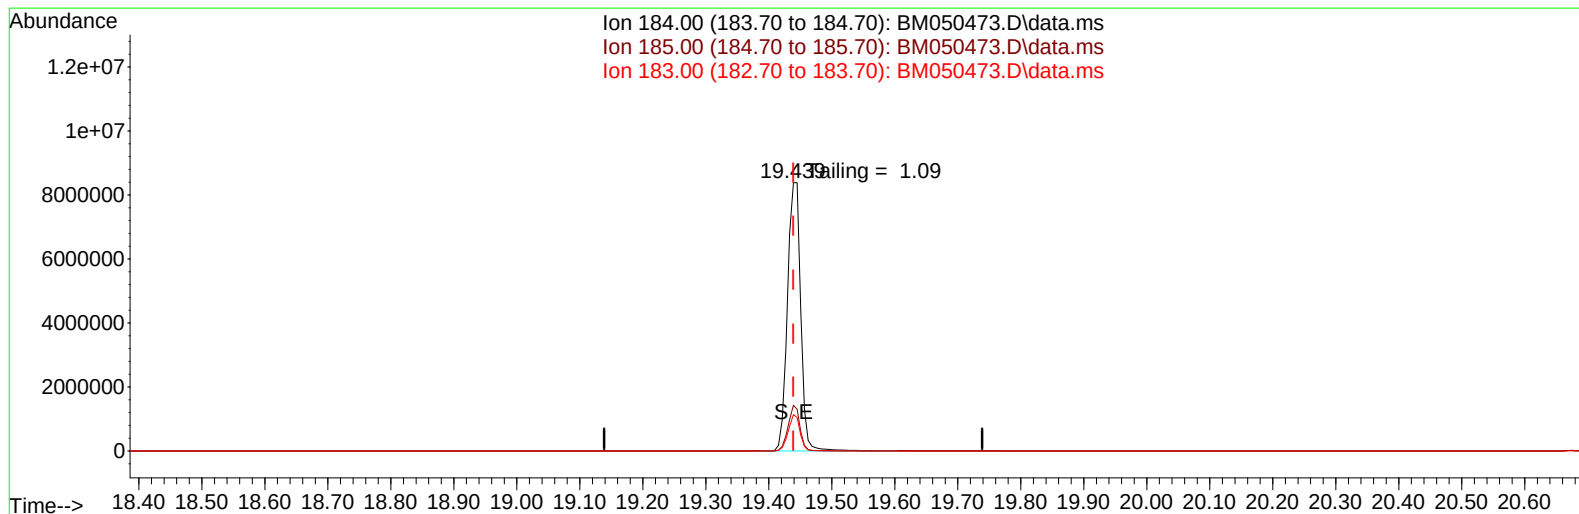

TIC: BM050473.D\data.ms

(77) Benzidine

19.439min (+ 0.000) 121383.09 ng

response 12309874

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	17.04
183.00	11.30	13.56#
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
7/17/2025	BNA_M	<u>BM050473.D</u>
Compound Name	Response	Retention Time
DDT	6172237	20.674
DDD	81432	20.292
DDE	4819	19.733
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
86251	6258488	1.38

Instrument :
BNA_M
ClientSampleId :
DFTPP