

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071425\
 Data File : VW031845.D
 Acq On : 14 Jul 2025 13:07
 Operator : SY/MD
 Sample : Q2592-01
 Misc : 6.94g/5mL/MSVOA_W/SOIL/A
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 WC-SOIL-20250711

Quant Time: Jul 15 02:44:09 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\82W063025S.M
 Quant Title : SW846 8260
 QLast Update : Tue Jul 01 03:35:17 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.965	168	205400	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.855	114	386707	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.635	117	368231	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.556	152	164076	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.319	65	145728	49.438	ug/l	0.00
Spiked Amount	50.000	Range	63 - 155	Recovery	=	98.880%
35) Dibromofluoromethane	7.904	113	122669	48.612	ug/l	0.00
Spiked Amount	50.000	Range	70 - 134	Recovery	=	97.220%
50) Toluene-d8	10.331	98	445707	47.463	ug/l	0.00
Spiked Amount	50.000	Range	74 - 123	Recovery	=	94.920%
62) 4-Bromofluorobenzene	12.617	95	178085	51.532	ug/l	0.00
Spiked Amount	50.000	Range	17 - 146	Recovery	=	103.060%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071425\
Data File : VW031845.D
Acq On : 14 Jul 2025 13:07
Operator : SY/MD
Sample : Q2592-01
Misc : 6.94g/5mL/MSVOA_W/SOIL/A
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
WC-SOIL-20250711

Quant Time: Jul 15 02:44:09 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\82W063025S.M
Quant Title : SW846 8260
QLast Update : Tue Jul 01 03:35:17 2025
Response via : Initial Calibration




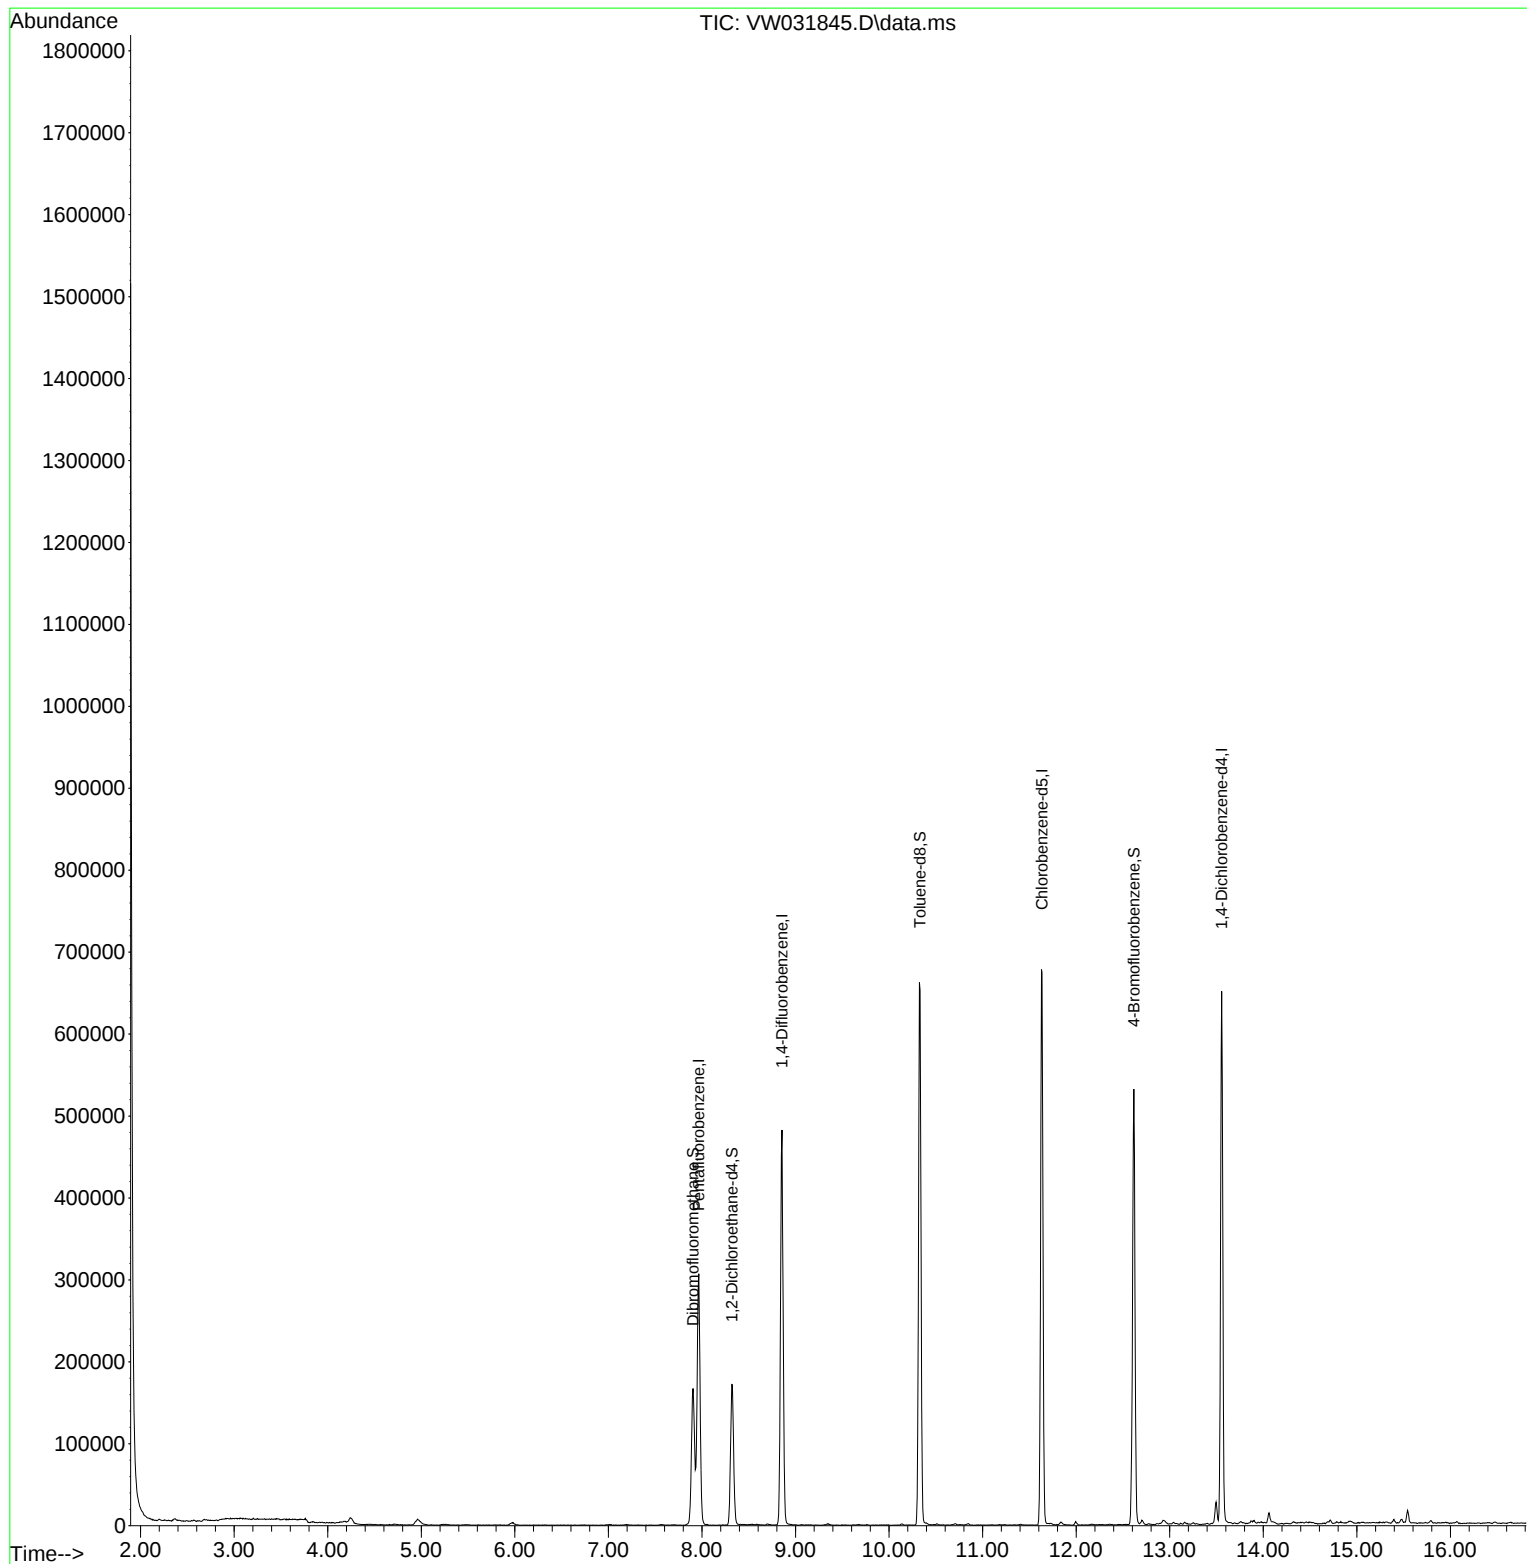


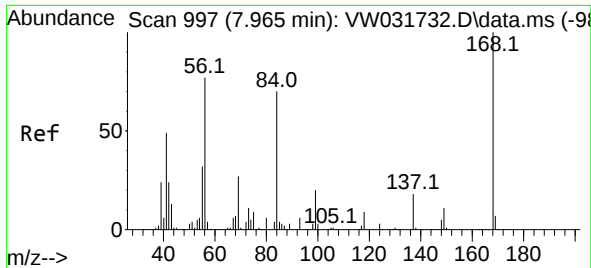

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.965 min Scan# 997
Delta R.T. 0.000 min
Lab File: VW031845.D
Acq: 14 Jul 2025 13:07




Instrument :
MSVOA_W
ClientSampleId :
WC-SOIL-20250711


Tgt Ion:168 Resp: 205400
Ion Ratio Lower Upper
168 100
99 60.4 49.4 74.2

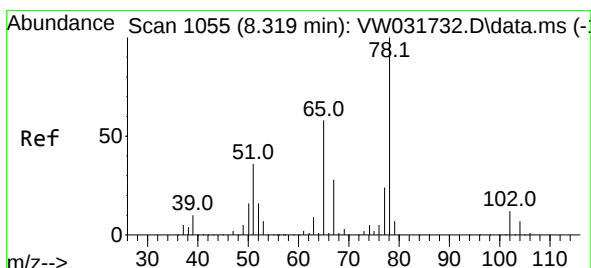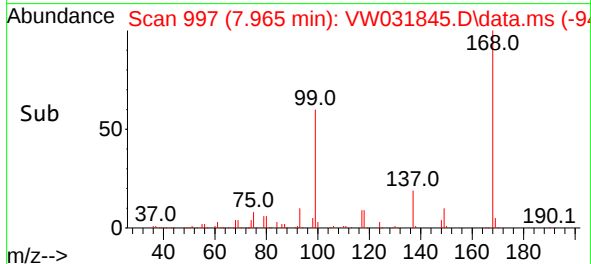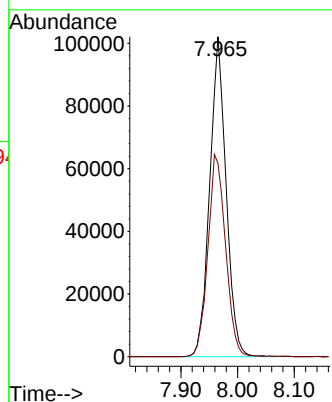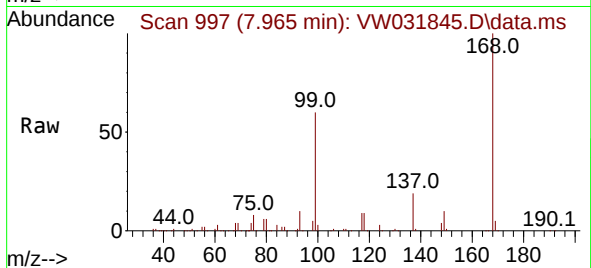

#33
1,2-Dichloroethane-d4
Concen: 49.438 ug/l
RT: 8.319 min Scan# 1055
Delta R.T. 0.000 min
Lab File: VW031845.D
Acq: 14 Jul 2025 13:07

Tgt Ion: 65 Resp: 145728
Ion Ratio Lower Upper
65 100
67 49.8 0.0 99.4


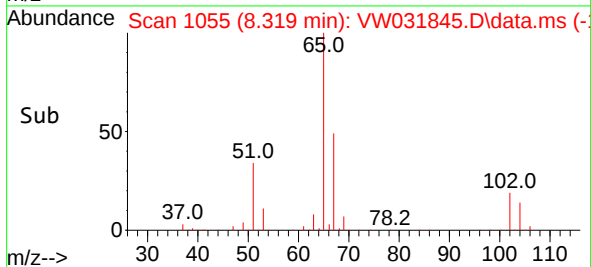
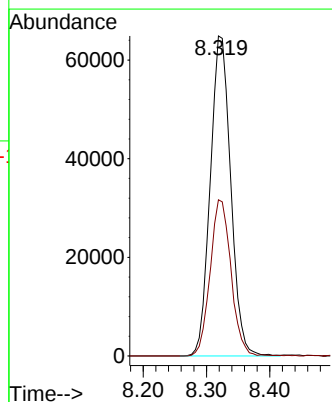
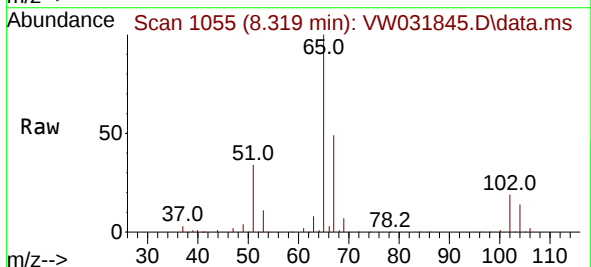


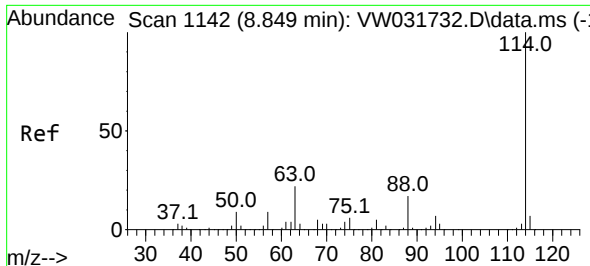

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.855 min Scan# 1142
 Delta R.T. 0.006 min
 Lab File: VW031845.D
 Acq: 14 Jul 2025 13:07




Instrument :
 MSVOA_W
 ClientSampleId :
 WC-SOIL-20250711


Tgt Ion:114 Resp: 386707
 Ion Ratio Lower Upper
 114 100
 63 21.4 0.0 43.6
 88 16.3 0.0 34.2

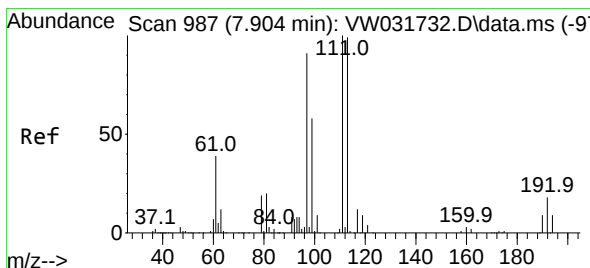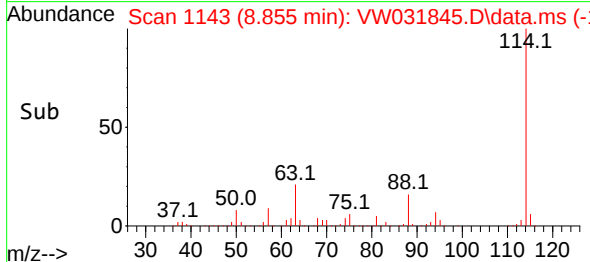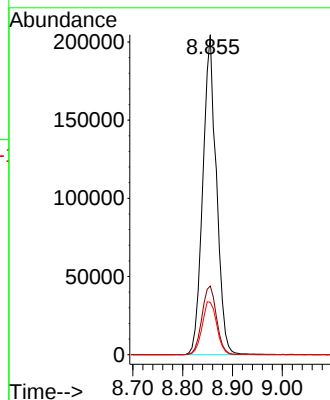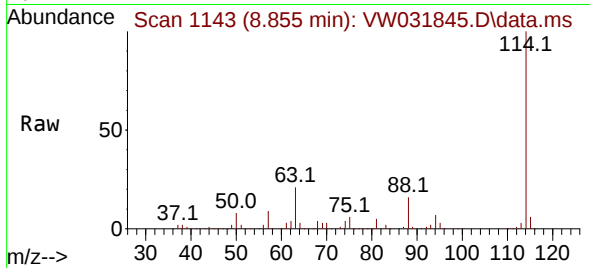

#35
 Dibromofluoromethane
 Concen: 48.612 ug/l
 RT: 7.904 min Scan# 987
 Delta R.T. 0.000 min
 Lab File: VW031845.D
 Acq: 14 Jul 2025 13:07

Tgt Ion:113 Resp: 122669
 Ion Ratio Lower Upper
 113 100
 111 103.5 82.1 123.1
 192 16.1 13.8 20.6


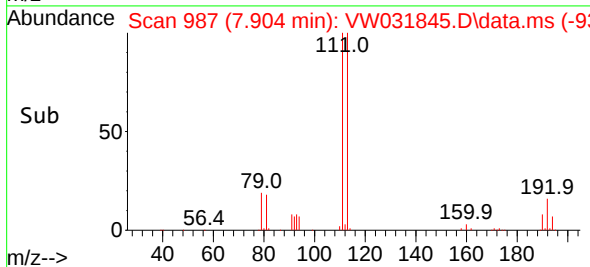
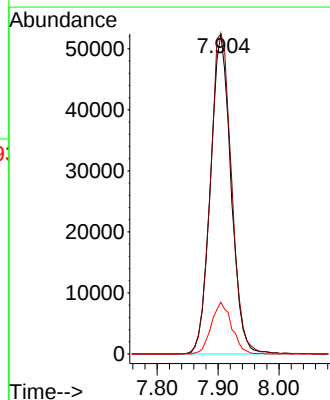
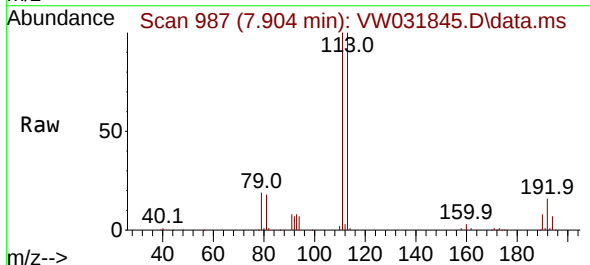


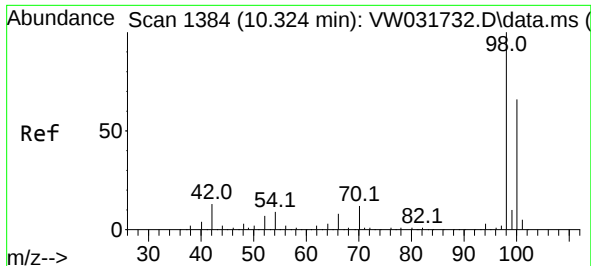

#50
Toluene-d8
Concen: 47.463 ug/l
RT: 10.331 min Scan# 11
Delta R.T. 0.006 min
Lab File: VW031845.D
Acq: 14 Jul 2025 13:07




Instrument :
MSVOA_W
ClientSampleId :
WC-SOIL-20250711


Tgt Ion: 98 Resp: 445707
Ion Ratio Lower Upper
98 100
100 65.8 53.0 79.4

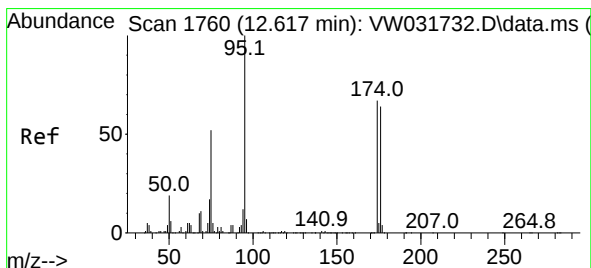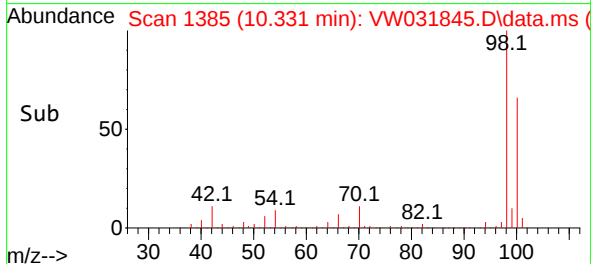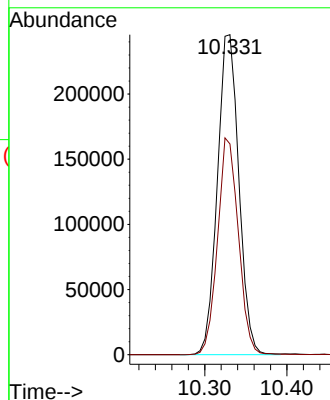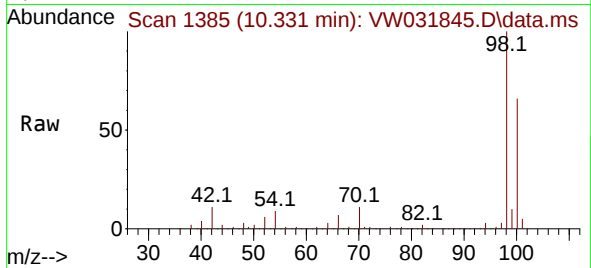

#62
4-Bromofluorobenzene
Concen: 51.532 ug/l
RT: 12.617 min Scan# 1760
Delta R.T. 0.000 min
Lab File: VW031845.D
Acq: 14 Jul 2025 13:07

Tgt Ion: 95 Resp: 178085
Ion Ratio Lower Upper
95 100
174 65.0 0.0 133.8
176 60.7 0.0 126.0


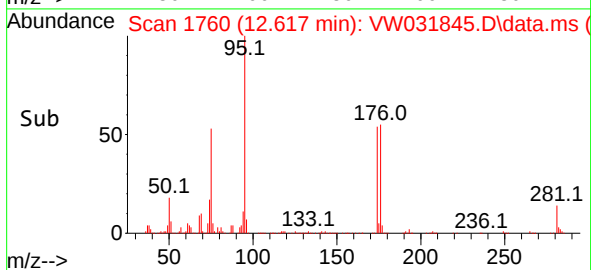
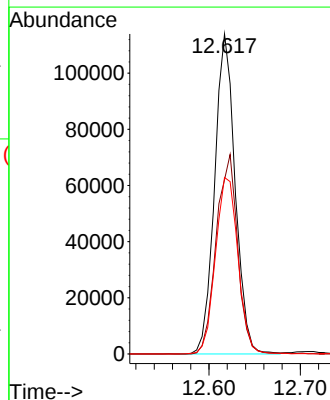
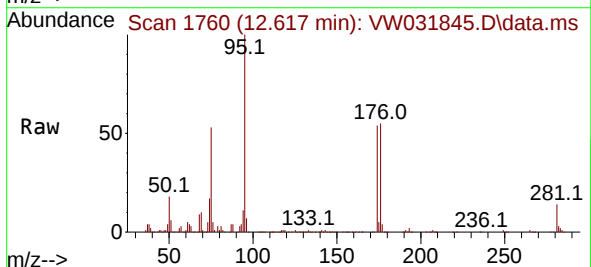


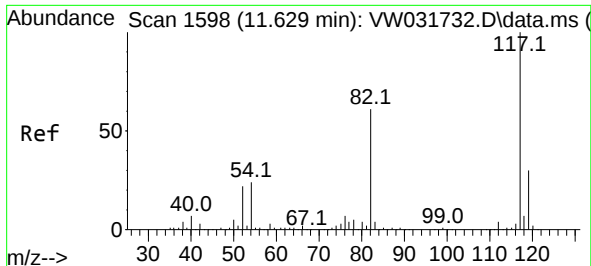

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.635 min Scan# 11
Delta R.T. 0.006 min
Lab File: VW031845.D
Acq: 14 Jul 2025 13:07

Instrument :
MSVOA_W
ClientSampleId :
WC-SOIL-20250711

Tgt Ion:117 Resp: 368231
Ion Ratio Lower Upper
117 100
82 56.8 48.6 72.8
119 32.8 23.9 35.9

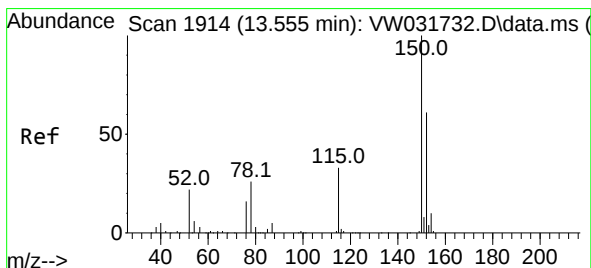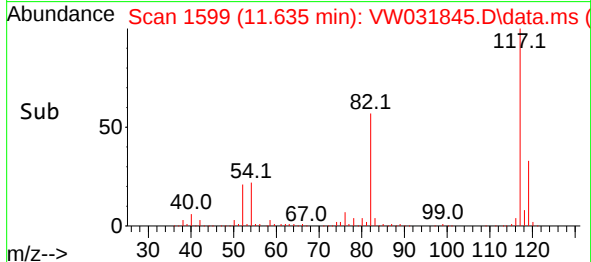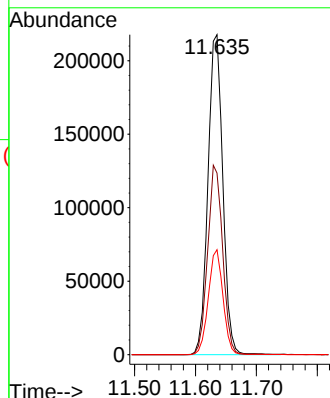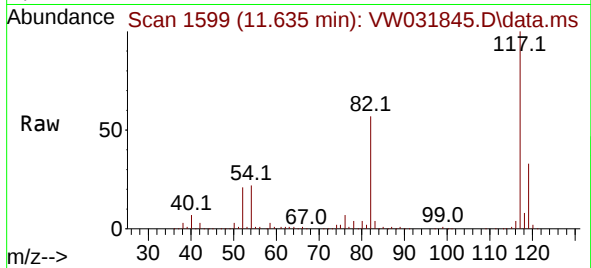

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.556 min Scan# 1914
Delta R.T. 0.000 min
Lab File: VW031845.D
Acq: 14 Jul 2025 13:07

Tgt Ion:152 Resp: 164076
Ion Ratio Lower Upper
152 100
115 65.2 31.9 95.7
150 153.9 0.0 356.4

