
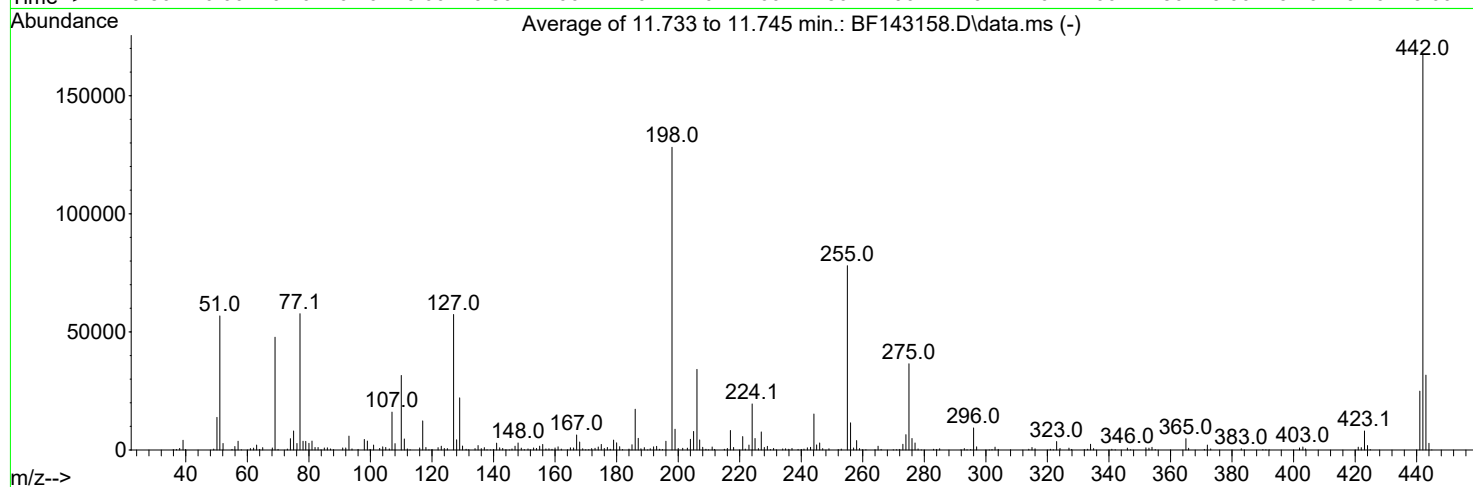


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071825\
Data File : BF143158.D
Acq On : 18 Jul 2025 10:55
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF071725.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Jul 17 15:14:05 2025

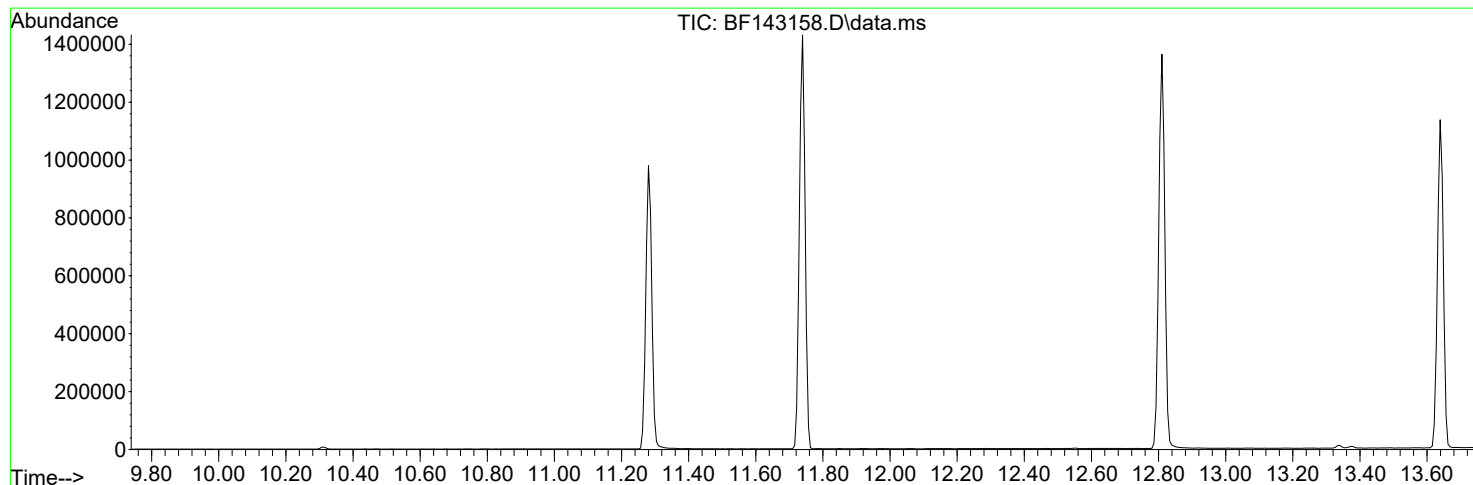

AutoFind: Scans 1622, 1623, 1624; Background Corrected with Scan 1616

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
68	69	0.00	2	1.9	919	PASS
69	69	100	100	100.0	47752	PASS
70	69	0.00	2	0.6	277	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	128128	PASS
199	198	5	9	6.9	8805	PASS
365	198	1	100	3.8	4844	PASS
441	443	0.01	150	78.8	24960	PASS
442	442	100	100	100.0	167149	PASS
443	442	15	24	19.0	31683	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
7/17/2025	BNA_F	<u>BF143138.D</u>
Compound Name	Response	Retention Time
DDT	262709	13.639
DDD	5014	13.339
DDE	214	13.004
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5228	267937	1.95

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071825\
Data File : BF143158.D
Acq On : 18 Jul 2025 10:55
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jul 18 12:10:18 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF071725.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 17 15:14:05 2025
Response via : Initial Calibration

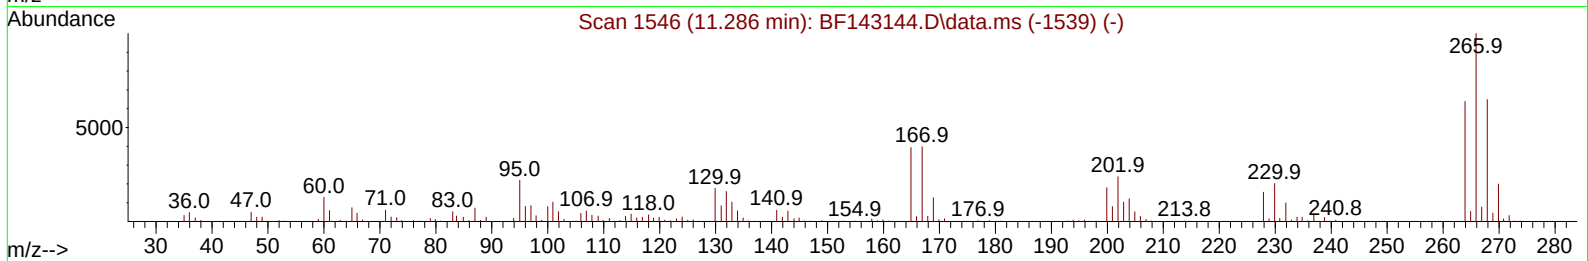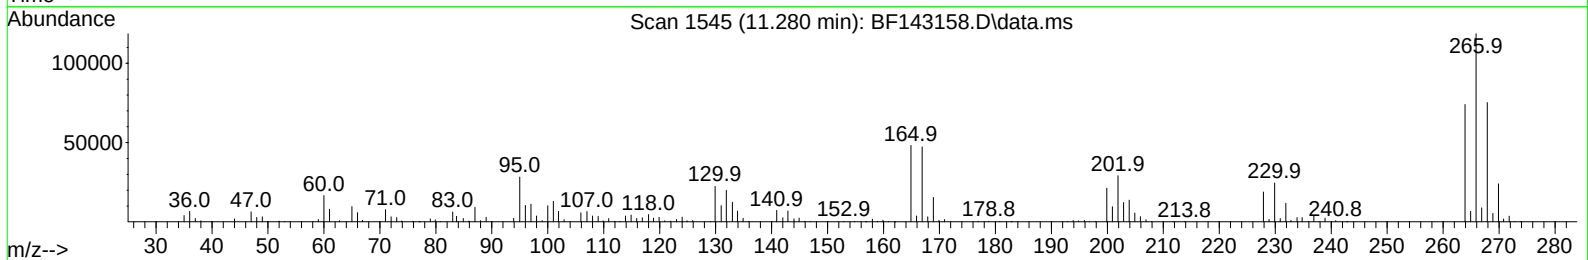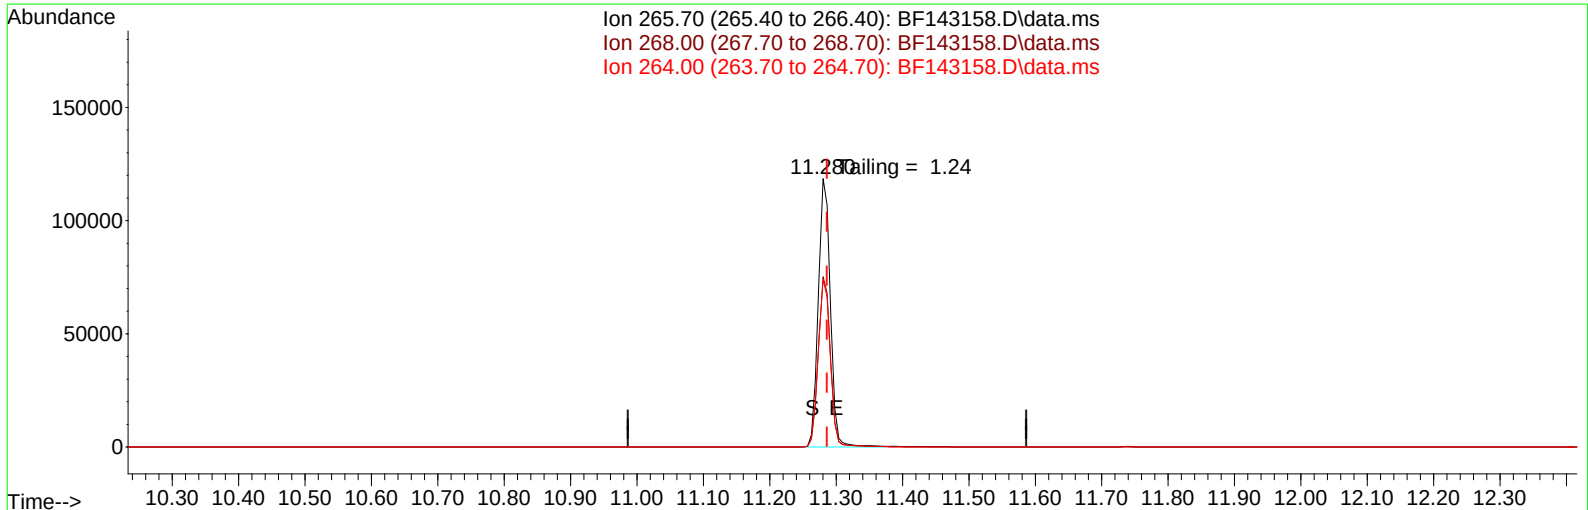

TIC: BF143158.D\data.ms

(70) Pentachlorophenol (C)

11.280min (-0.006) 27822.04 ng




response 150610

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.90	63.42
264.00	63.80	62.47
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071825\
Data File : BF143158.D
Acq On : 18 Jul 2025 10:55
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jul 18 12:10:18 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF071725.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 17 15:14:05 2025
Response via : Initial Calibration

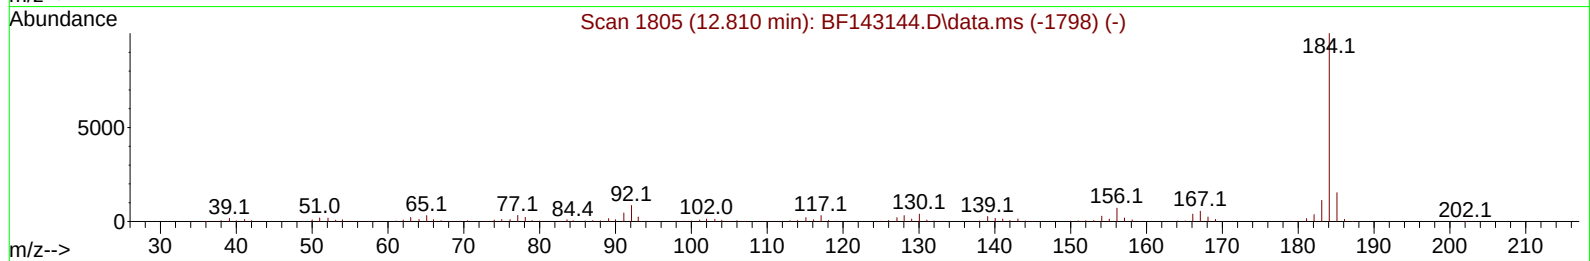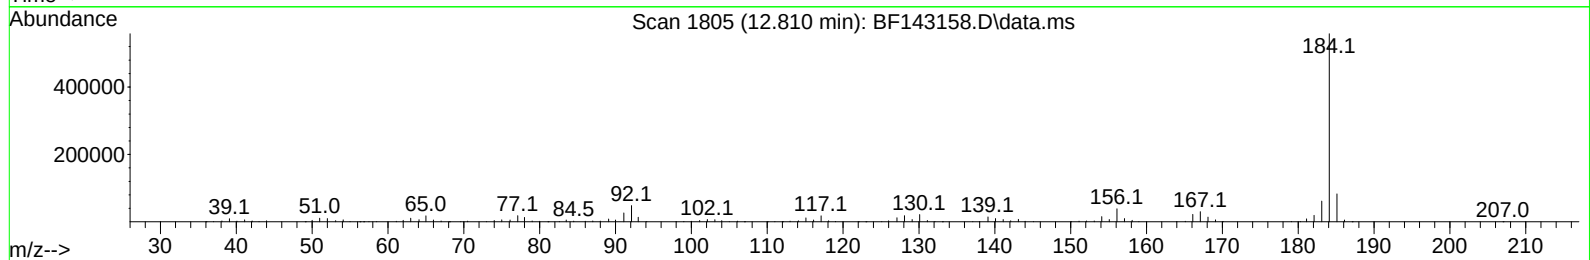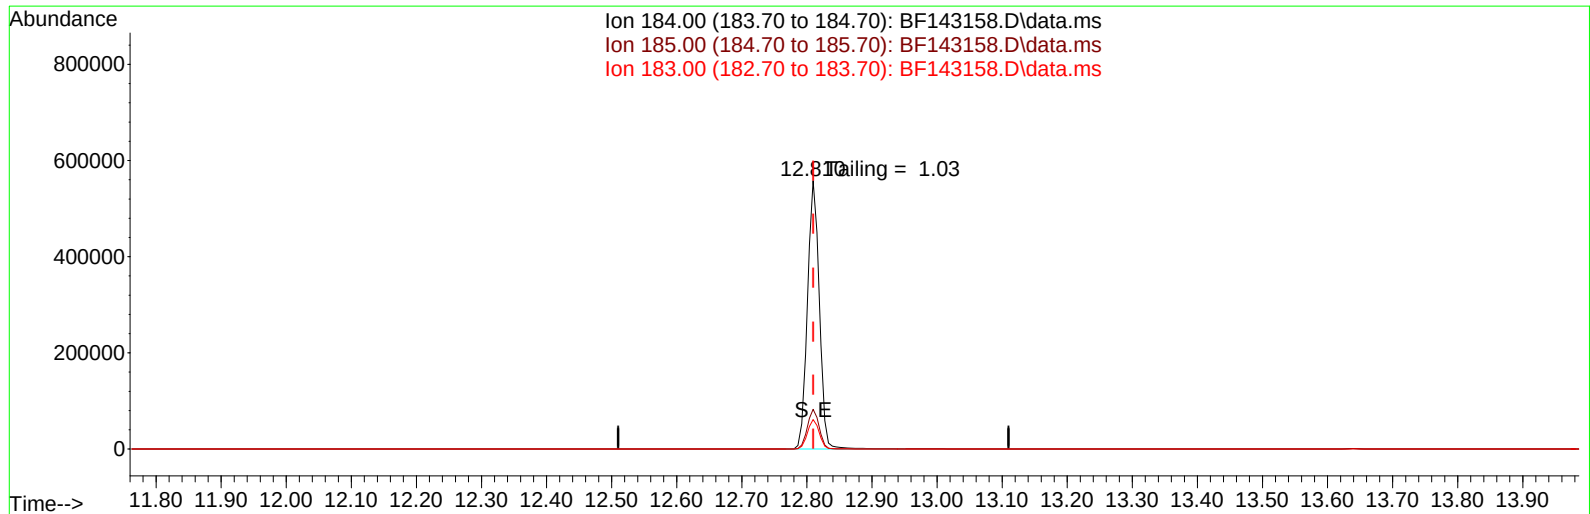

TIC: BF143158.D\data.ms

(77) Benzidine

12.810min (-0.000) 0.00 ng

response 711133

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.30	14.82
183.00	11.20	10.97
0.00	0.00	0.00