


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071825\
Data File : BP025186.D
Acq On : 18 Jul 2025 09:41
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-Tune.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Mar 29 08:52:24 2022

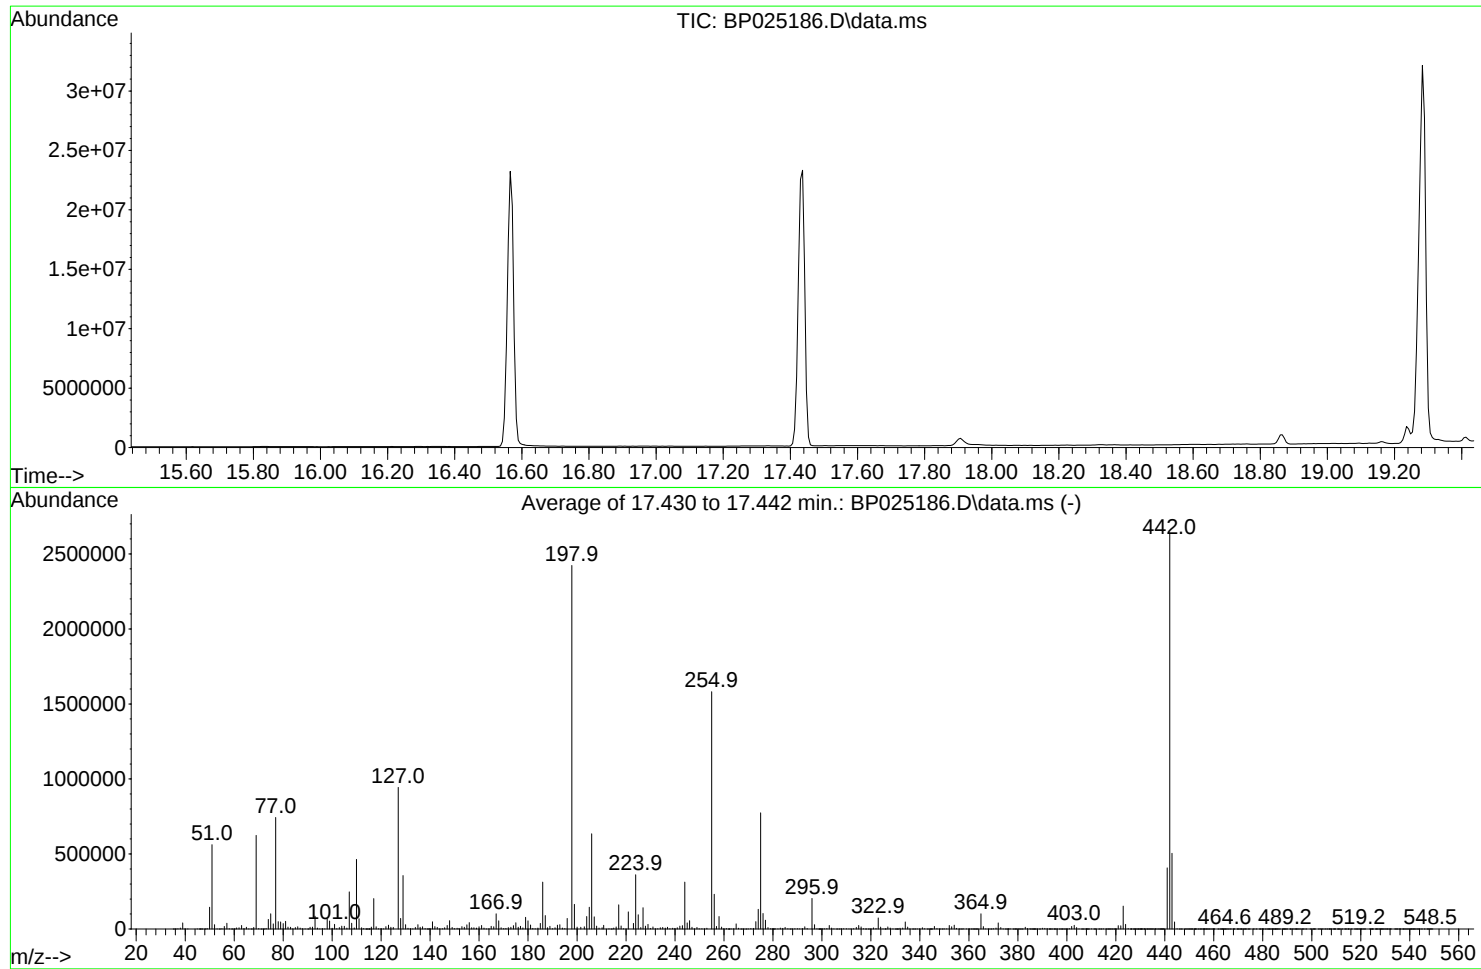




AutoFind: Scans 2464, 2465, 2466; Background Corrected with Scan 2456

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	1.8	10952	PASS
69	69	100	100	100.0	624035	PASS
70	69	0.00	2	0.5	2838	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	2422784	PASS
199	198	5	9	6.8	164253	PASS
365	198	1	100	4.2	101199	PASS
441	443	0.01	150	80.7	406912	PASS
442	442	100	100	100.0	2631503	PASS
443	442	15	24	19.2	504102	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071825\
Data File : BP025186.D
Acq On : 18 Jul 2025 09:41
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Jul 18 11:41:15 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP070325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 03 16:05:44 2025
Response via : Initial Calibration

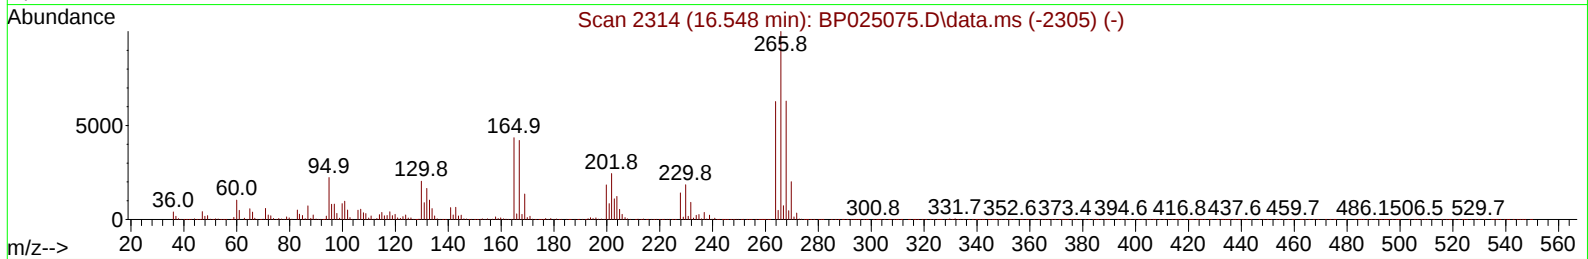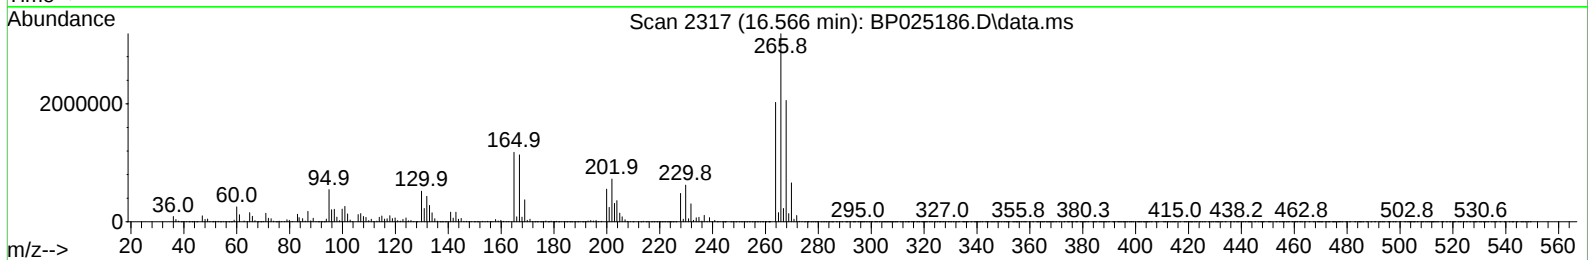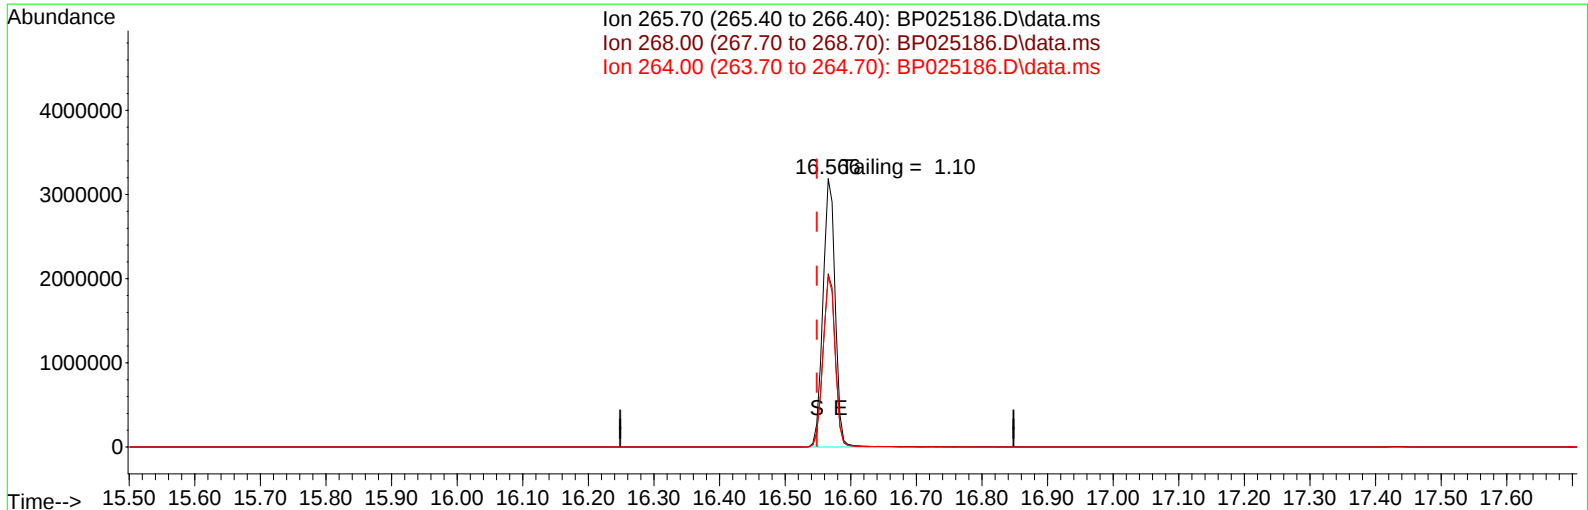

TIC: BP025186.D\data.ms

(70) Pentachlorophenol (C)

16.566min (+ 0.017) 169477.45 ng




response 4133923

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.00	64.49
264.00	62.70	63.53
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071825\
Data File : BP025186.D
Acq On : 18 Jul 2025 09:41
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Jul 18 11:41:15 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP070325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 03 16:05:44 2025
Response via : Initial Calibration

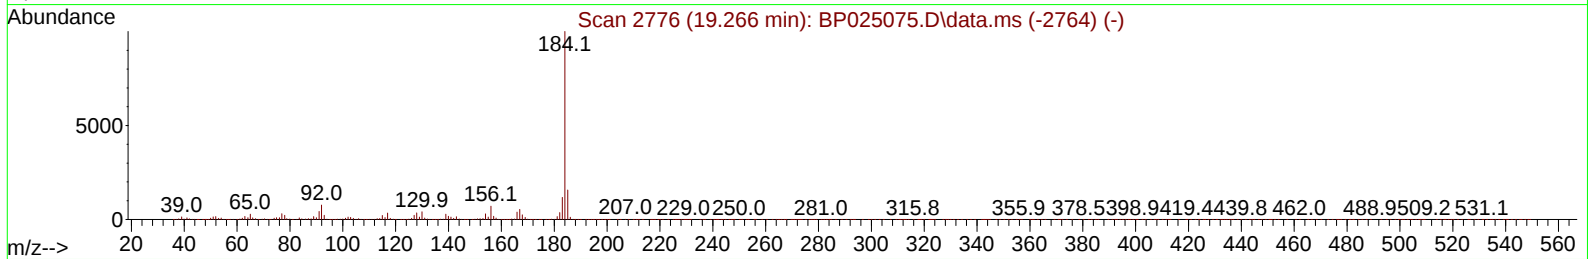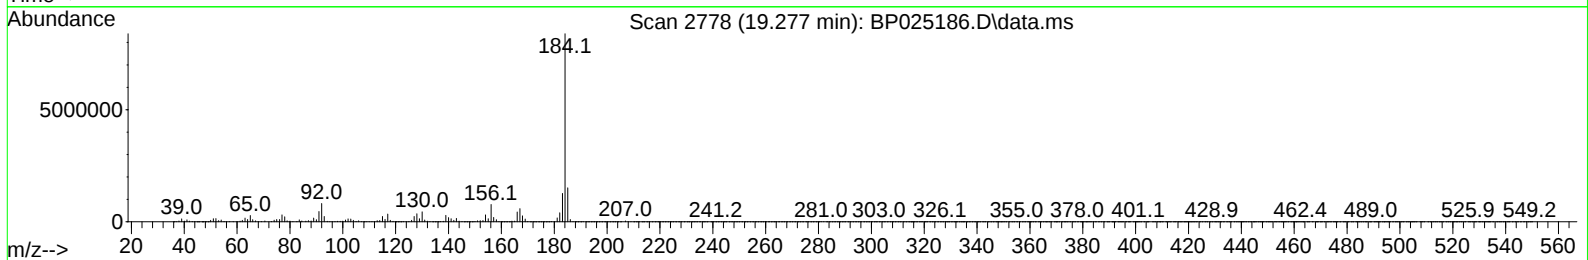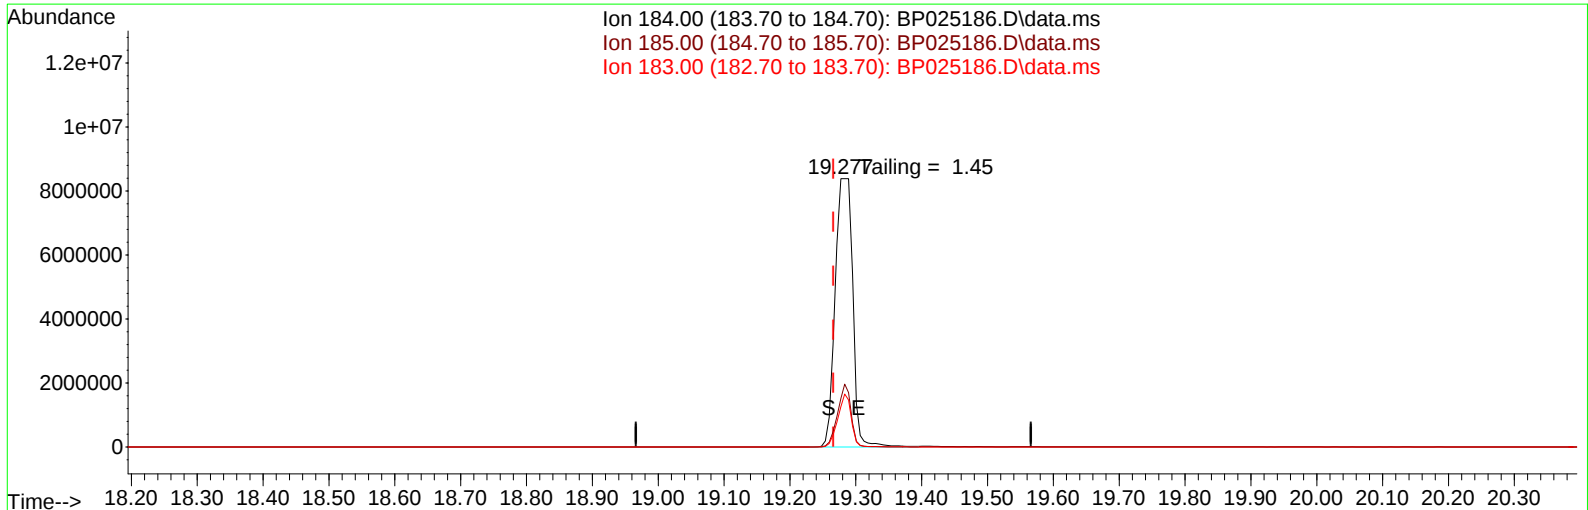

TIC: BP025186.D\data.ms

(77) Benzidine

19.277min (+ 0.011) 75417.62 ng

response 15500257

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.70	18.09
183.00	11.80	15.05#
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
7/18/2025	BNA_P	<u>BP025186.D</u>
Compound Name	Response	Retention Time
DDT	9164203	20.589
DDD	214461	20.13
DDE	11445	19.595
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
225906	9390109	2.41

Instrument :
BNA_P
ClientSampleId :
DFTPP