

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071625\
 Data File : BP025164.D
 Acq On : 16 Jul 2025 18:59
 Operator : CG/JU
 Sample : Q2600-09
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 END-OF-TRENCH

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP070325.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP025164.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.343	57	69	78	rBV3	2491589	5591276	9.43%	0.506%
2	3.708	126	131	139	rVB3	1234328	2637822	4.45%	0.239%
3	3.796	139	146	156	rVB3	1493370	3227463	5.44%	0.292%
4	3.966	168	175	178	rBV	2526874	4375923	7.38%	0.396%
5	4.231	216	220	228	rVB	1635969	2528828	4.27%	0.229%
6	4.508	258	267	278	rBV	2796806	5228900	8.82%	0.473%
7	4.602	278	283	288	rBV	2281870	3907611	6.59%	0.354%
8	4.696	296	299	304	rVB	3252611	4616306	7.79%	0.418%
9	4.749	304	308	314	rBV	4009317	6226939	10.51%	0.563%
10	4.996	344	350	353	rVV2	2727351	6041295	10.19%	0.547%
11	5.025	353	355	363	rVB2	2258577	3447514	5.82%	0.312%
12	5.108	363	369	376	rBV2	7250389	13822869	23.32%	1.251%
13	5.331	398	407	413	rVB5	1505384	3312047	5.59%	0.300%
14	5.402	413	419	426	rBV3	2046675	4205580	7.10%	0.381%
15	5.478	426	432	436	rVB	3483015	5086107	8.58%	0.460%
16	5.537	436	442	449	rVB2	1940395	3902608	6.58%	0.353%
17	5.790	476	485	492	rBV3	5424676	12869713	21.71%	1.165%
18	5.908	497	505	514	rVB2	3019861	6788346	11.45%	0.614%
19	5.996	514	520	526	rBV4	6198506	12187414	20.56%	1.103%
20	6.060	526	531	536	rBV	8487230	13786072	23.26%	1.247%
21	6.131	536	543	547	rVV4	5472280	12329799	20.80%	1.116%
22	6.172	547	550	555	rVB	6032608	9020120	15.22%	0.816%
23	6.255	555	564	568	rBV3	1681151	3828687	6.46%	0.346%
24	6.308	569	573	579	rVB3	2112384	3576309	6.03%	0.324%
25	6.390	579	587	593	rVB3	4540449	11232224	18.95%	1.016%
26	6.460	593	599	601	rBV3	7201201	12994090	21.92%	1.176%
27	6.490	601	604	609	rVB	12005156	16748108	28.26%	1.516%
28	6.543	609	613	617	rBV	4589097	5929827	10.00%	0.537%
29	6.649	622	631	638	rVB4	12847132	33576197	56.65%	3.038%
30	6.713	638	642	647	rBV2	2035895	3918818	6.61%	0.355%
31	6.819	652	660	663	rBV6	3059010	7773844	13.11%	0.703%
32	6.860	663	667	671	rVB2	4450236	6371749	10.75%	0.577%
33	6.960	676	684	689	rBV	5497657	11844724	19.98%	1.072%
34	7.002	689	691	693	rVV3	2260123	2803367	4.73%	0.254%
35	7.031	693	696	705	rVB3	5947879	12645003	21.33%	1.144%
36	7.113	705	710	714	rBV	6516207	10987956	18.54%	0.994%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071625\
 Data File : BP025164.D
 Acq On : 16 Jul 2025 18:59
 Operator : CG/JU
 Sample : Q2600-09
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 END-OF-TRENCH

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP070325.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	7.190	720	723	727	rVB3	3194946	4758444	8.03%	0.431%
38	7.284	734	739	741	rBV2	3432432	4957842	8.36%	0.449%
39	7.313	741	744	749	rVV4	3711250	7251951	12.23%	0.656%
40	7.366	749	753	755	rVV3	4179557	6075849	10.25%	0.550%
41	7.396	755	758	761	rVV2	5071892	7720209	13.02%	0.699%
42	7.460	761	769	777	rVB2	29365748	59274677	100.00%	5.364%
43	7.555	777	785	789	rBV5	4627543	15273006	25.77%	1.382%
44	7.607	789	794	798	rVV	6001691	10431638	17.60%	0.944%
45	7.660	800	803	806	rVV2	3812822	5404607	9.12%	0.489%
46	7.702	806	810	824	rVB3	16316247	48830657	82.38%	4.419%
47	7.819	824	830	835	rVB2	11871957	20242285	34.15%	1.832%
48	7.902	839	844	847	rBV5	2374483	3940509	6.65%	0.357%
49	7.943	847	851	856	rBV2	11663711	20548490	34.67%	1.859%
50	8.007	856	862	866	rVV2	23206251	40115170	67.68%	3.630%
51	8.043	866	868	873	rVB3	5810314	9161072	15.46%	0.829%
52	8.090	873	876	879	rVB2	2942149	3020439	5.10%	0.273%
53	8.137	879	884	890	rVB	20321313	39579886	66.77%	3.582%
54	8.231	890	900	902	rBV3	5711111	12148024	20.49%	1.099%
55	8.272	903	907	911	rVB3	9462067	14919504	25.17%	1.350%
56	8.337	911	918	922	rBV	11180617	22285820	37.60%	2.017%
57	8.437	931	935	940	rVB5	1318177	2805283	4.73%	0.254%
58	8.507	940	947	948	rBV3	4656800	8724975	14.72%	0.790%
59	8.554	949	955	963	rVV2	26782152	58747217	99.11%	5.316%
60	8.631	963	968	975	rVV3	9588429	23458933	39.58%	2.123%
61	8.690	975	978	985	rVB3	5241206	10124974	17.08%	0.916%
62	8.778	985	993	1002	rBV7	7316695	24612695	41.52%	2.227%
63	8.884	1002	1011	1013	rBV4	3964715	9279627	15.66%	0.840%
64	9.019	1029	1034	1036	rBV3	4241674	6443385	10.87%	0.583%
65	9.060	1036	1041	1044	rVB	10916767	15760301	26.59%	1.426%
66	9.143	1052	1055	1064	rVB5	5614689	10164061	17.15%	0.920%
67	9.219	1064	1068	1074	rVB2	1793160	2838322	4.79%	0.257%
68	9.319	1078	1085	1088	rBV3	4679719	8705956	14.69%	0.788%
69	9.354	1088	1091	1095	rVV	2859538	3528821	5.95%	0.319%
70	9.413	1095	1101	1106	rVV4	4887107	12267654	20.70%	1.110%
71	9.466	1106	1110	1113	rVB	3397748	4316203	7.28%	0.391%
72	9.507	1113	1117	1123	rVB3	4126620	8079784	13.63%	0.731%
73	9.619	1127	1136	1141	rBV3	13811175	29674710	50.06%	2.685%
74	9.766	1157	1161	1165	rBV3	1936938	3286103	5.54%	0.297%
75	9.807	1165	1168	1181	rVB5	3358865	9056851	15.28%	0.820%
76	9.919	1181	1187	1192	rBV	5024653	7676720	12.95%	0.695%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071625\
Data File : BP025164.D
Acq On : 16 Jul 2025 18:59
Operator : CG/JU
Sample : Q2600-09
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
END-OF-TRENCH

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP070325.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

77	10.125	1218	1222	1225	rVV2	2525807	3415446	5.76%	0.309%
78	10.190	1225	1233	1239	rVV2	7718405	15841984	26.73%	1.434%
79	10.260	1240	1245	1251	rVB3	3770480	6078935	10.26%	0.550%
80	10.325	1252	1256	1263	rVB3	3727361	7208833	12.16%	0.652%
81	10.396	1263	1268	1271	rBV	5868774	8733533	14.73%	0.790%
82	10.513	1284	1288	1294	rVB2	1443018	2581956	4.36%	0.234%
83	10.919	1350	1357	1362	rVB4	1514902	3489015	5.89%	0.316%
84	11.254	1408	1414	1419	rBV	3195770	5894926	9.95%	0.533%
85	11.572	1463	1468	1475	rVB	6472413	11598556	19.57%	1.050%
86	11.978	1531	1537	1546	rBV	1915889	5300835	8.94%	0.480%
87	12.095	1553	1557	1562	rVB	2743784	3947621	6.66%	0.357%
88	12.701	1654	1660	1665	rVB	9519161	14460576	24.40%	1.309%
89	14.101	1891	1898	1905	rBV	4824451	7880379	13.29%	0.713%
90	15.631	2152	2158	2168	rVB	8002304	12975239	21.89%	1.174%
91	15.948	2207	2212	2218	rVB	2180675	3506956	5.92%	0.317%
92	16.789	2351	2355	2362	rVB	3355497	5731768	9.67%	0.519%
93	16.919	2372	2377	2382	rBV2	3612852	6464683	10.91%	0.585%
94	16.972	2382	2386	2391	rVV	2497666	4028123	6.80%	0.365%
95	17.425	2459	2463	2469	rBV2	1813982	3493359	5.89%	0.316%
96	17.907	2543	2545	2553	rVB	3312214	4101293	6.92%	0.371%
97	19.072	2739	2743	2749	rBV	6713594	12076737	20.37%	1.093%
98	19.154	2753	2757	2763	rVB	14490871	18762045	31.65%	1.698%
99	19.683	2843	2847	2854	rBV	16275149	22531712	38.01%	2.039%
100	21.330	3123	3127	3129	rBV2	6968140	10135901	17.10%	0.917%




Sum of corrected areas: 1105104520

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071625\
Data File : BP025164.D
Acq On : 16 Jul 2025 18:59
Operator : CG/JU
Sample : Q2600-09
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
END-OF-TRENCH

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP070325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

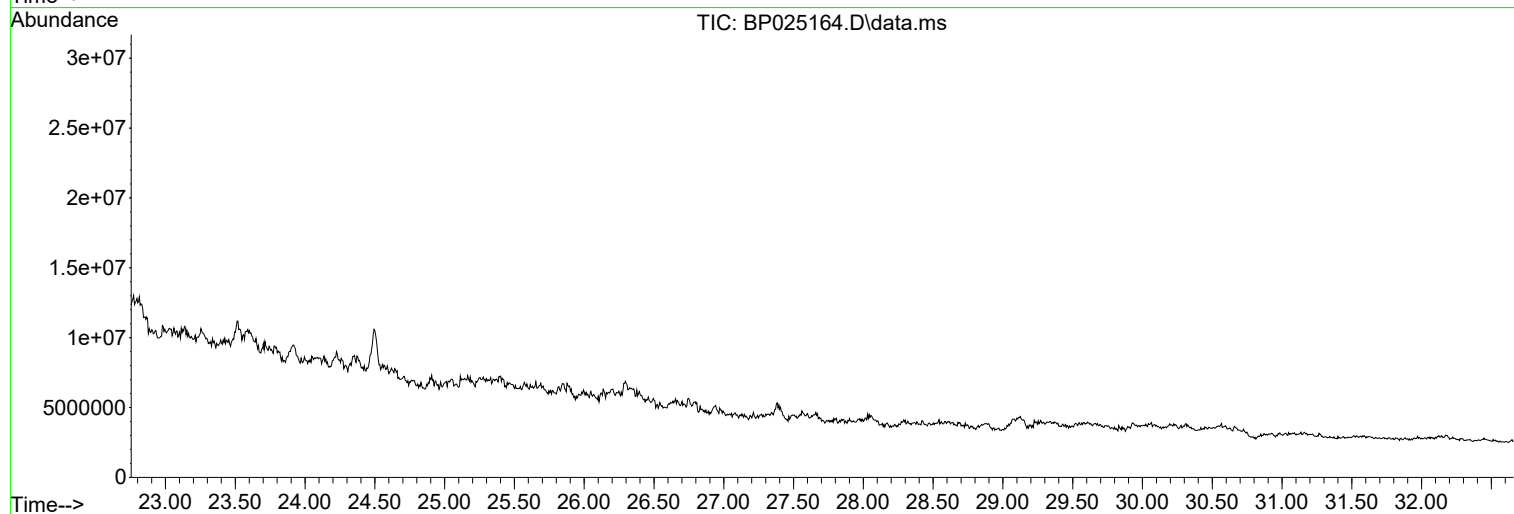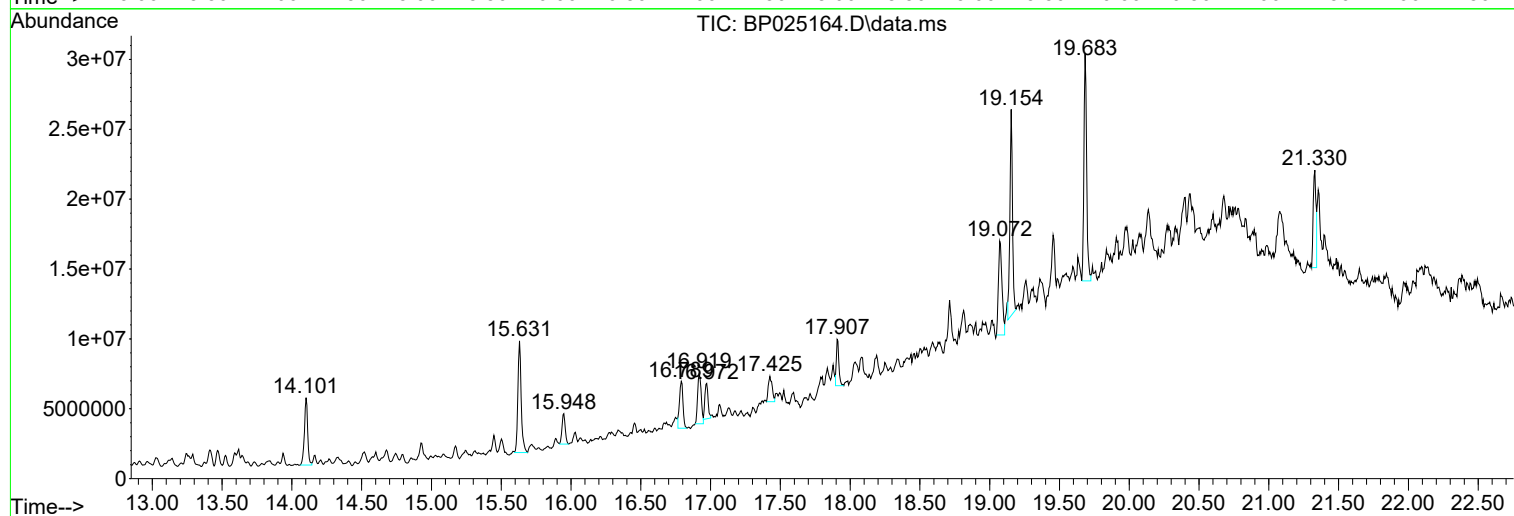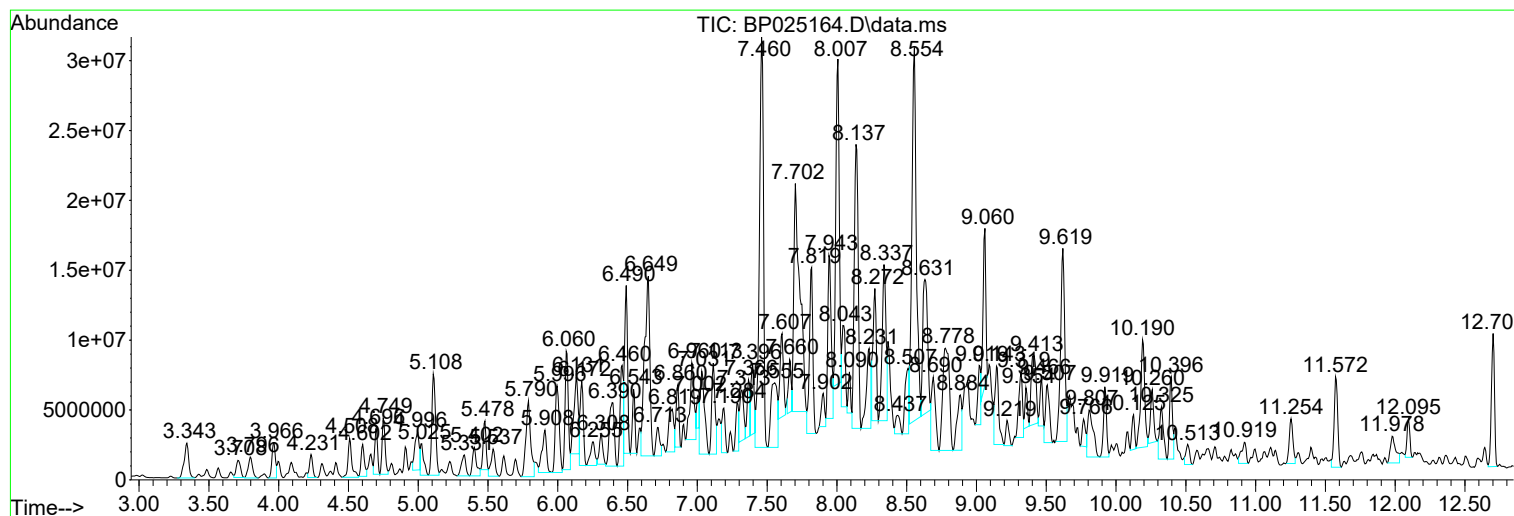

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071625\
Data File : BP025164.D
Acq On : 16 Jul 2025 18:59
Operator : CG/JU
Sample : Q2600-09
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
END-OF-TRENCH

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP070325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071625\
Data File : BP025164.D
Acq On : 16 Jul 2025 18:59
Operator : CG/JU
Sample : Q2600-09
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
END-OF-TRENCH

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP070325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------