
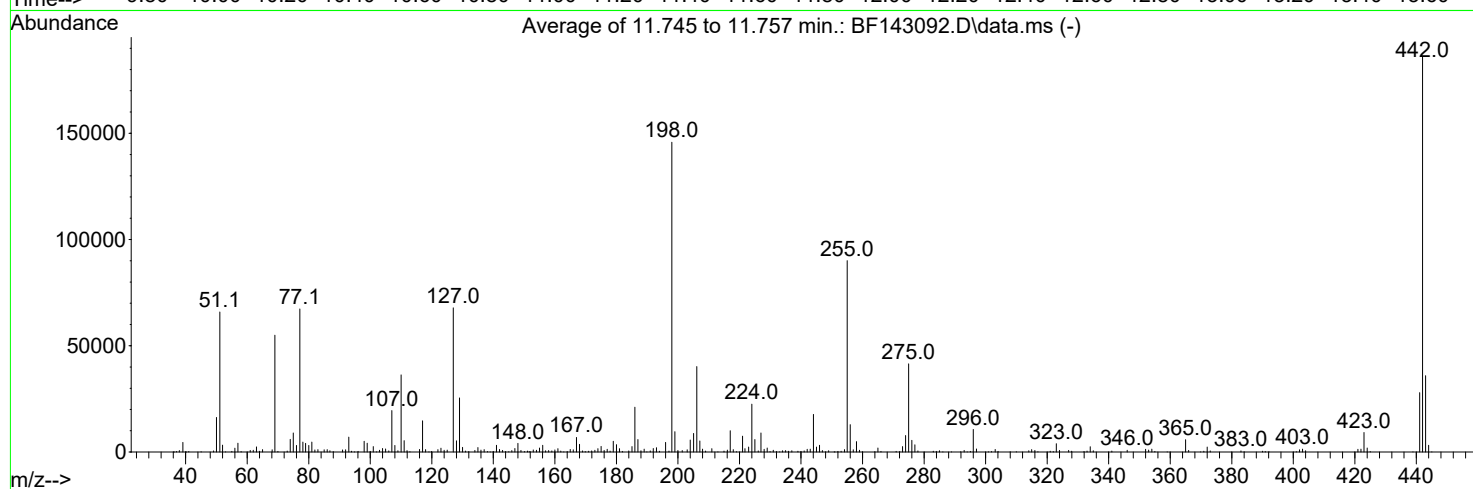


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071525\
Data File : BF143092.D
Acq On : 15 Jul 2025 12:35
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF071525.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Jul 15 17:53:25 2025

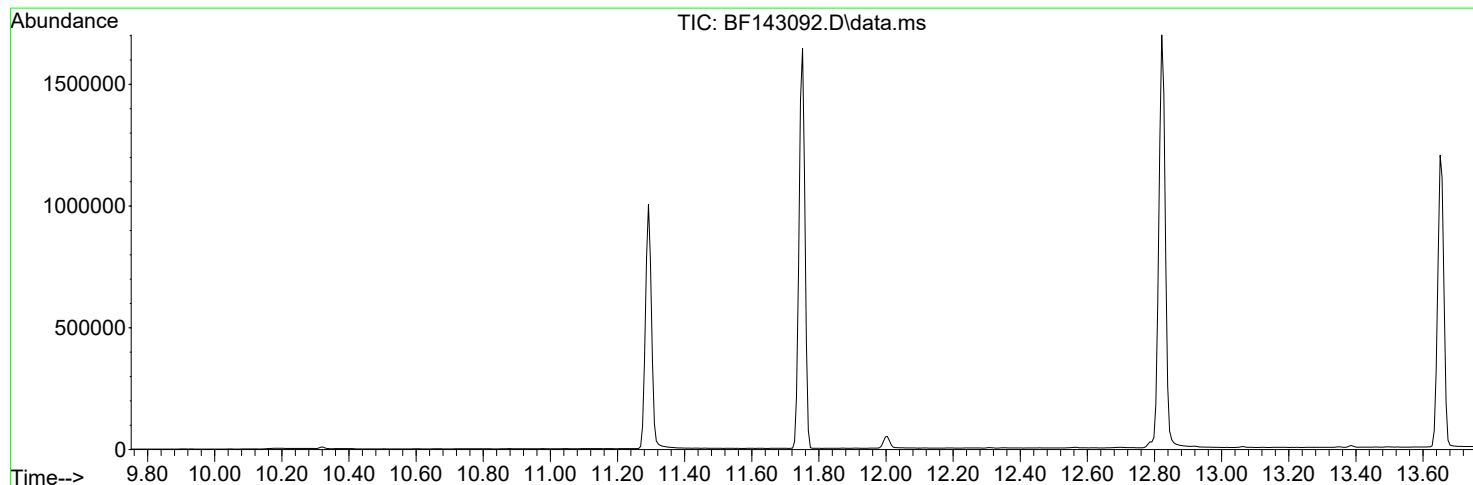

AutoFind: Scans 1624, 1625, 1626; Background Corrected with Scan 1617

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	2.0	1083	PASS
69	69	100	100	100.0	55011	PASS
70	69	0.00	2	0.5	283	PASS
197	198	0.00	2	0.3	479	PASS
198	198	100	100	100.0	145821	PASS
199	198	5	9	6.5	9539	PASS
365	198	1	100	4.0	5805	PASS
441	443	0.01	150	77.7	27936	PASS
442	442	100	100	100.0	185813	PASS
443	442	15	24	19.4	35957	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
7/15/2025	BNA_F	<u>BF143092.D</u>
Compound Name	Response	Retention Time
DDT	237029	13.651
DDD	2265	13.386
DDE	0	13.01
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
2265	239294	0.95

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071525\
Data File : BF143092.D
Acq On : 15 Jul 2025 12:35
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jul 15 18:02:12 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF071525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 15 17:53:25 2025
Response via : Initial Calibration

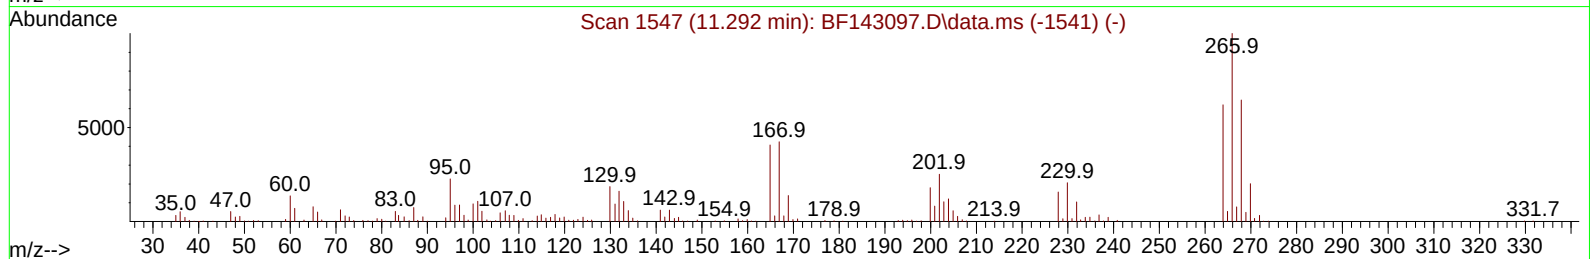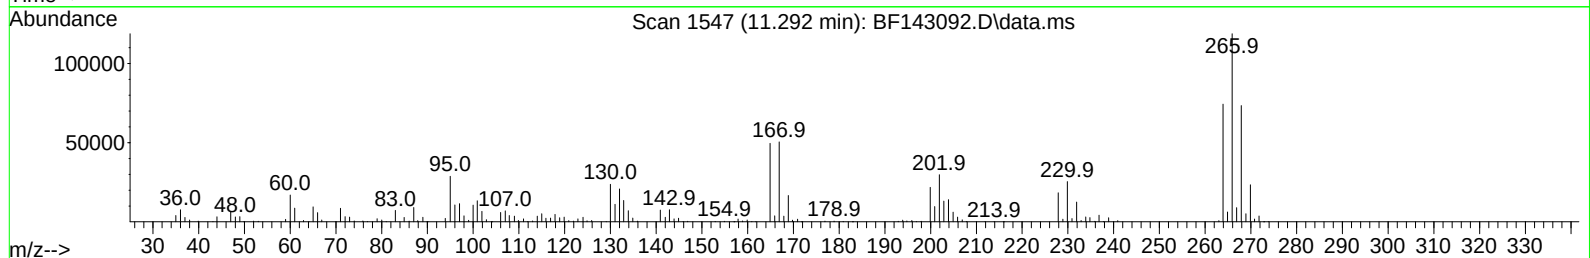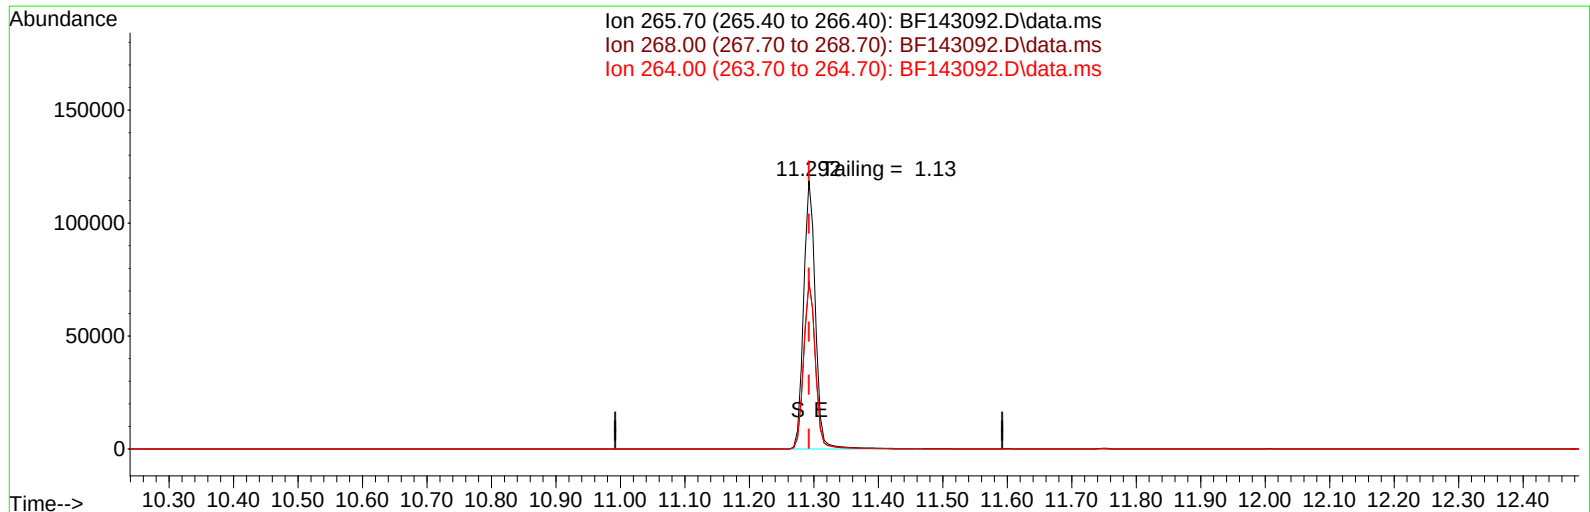

TIC: BF143092.D\data.ms

(70) Pentachlorophenol (C)

11.292min (+ 0.000) 28198.82 ng




response 151956

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.70	61.86
264.00	62.10	62.56
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071525\
Data File : BF143092.D
Acq On : 15 Jul 2025 12:35
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jul 15 18:02:12 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF071525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 15 17:53:25 2025
Response via : Initial Calibration

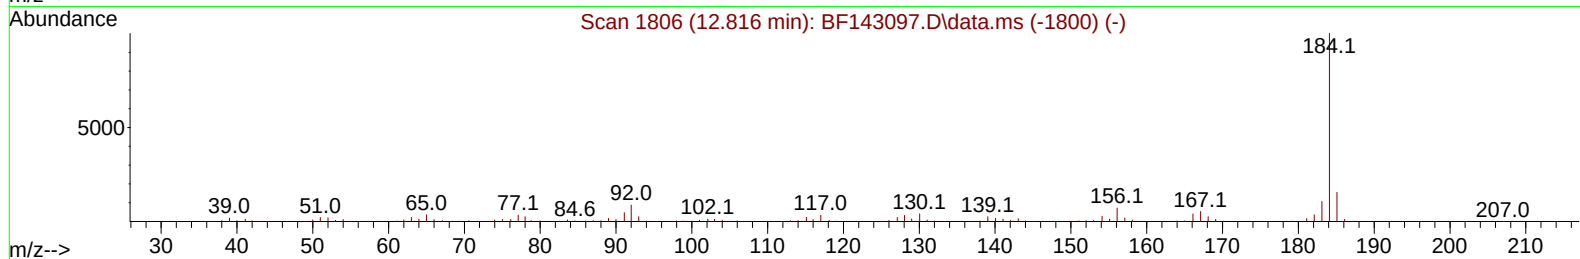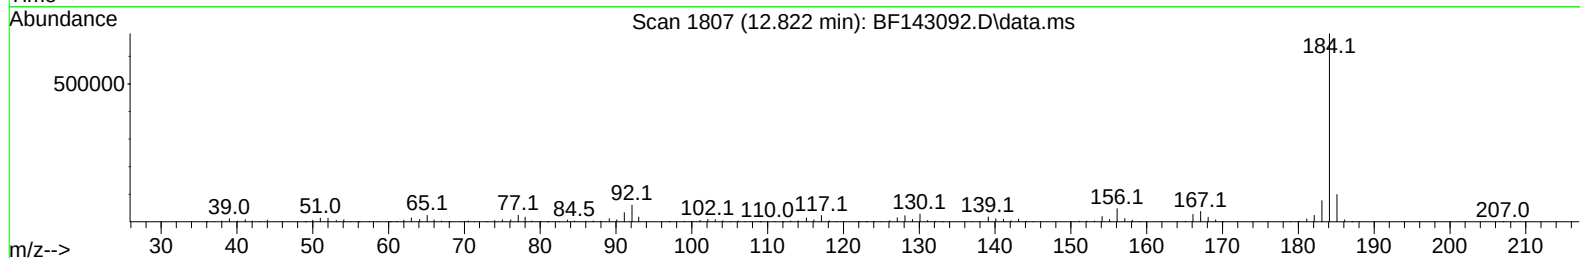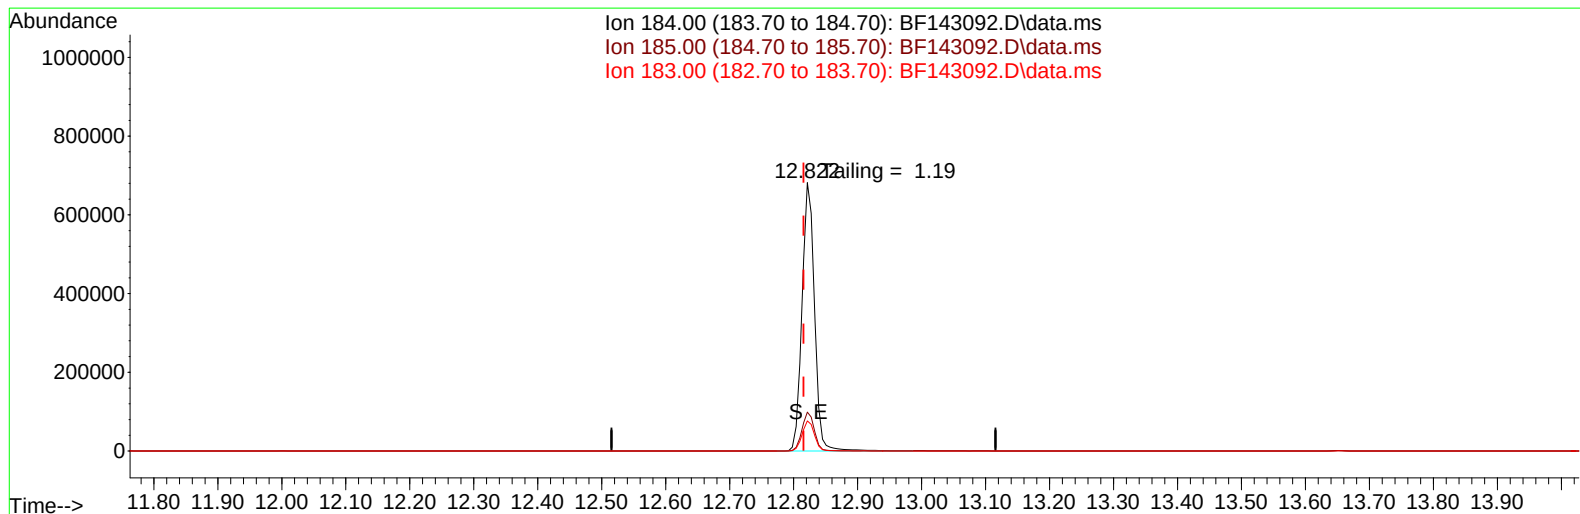

TIC: BF143092.D\data.ms

(77) Benzidine

12.822min (+ 0.006) 0.00 ng

response 925010

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.52
183.00	10.70	11.25
0.00	0.00	0.00