
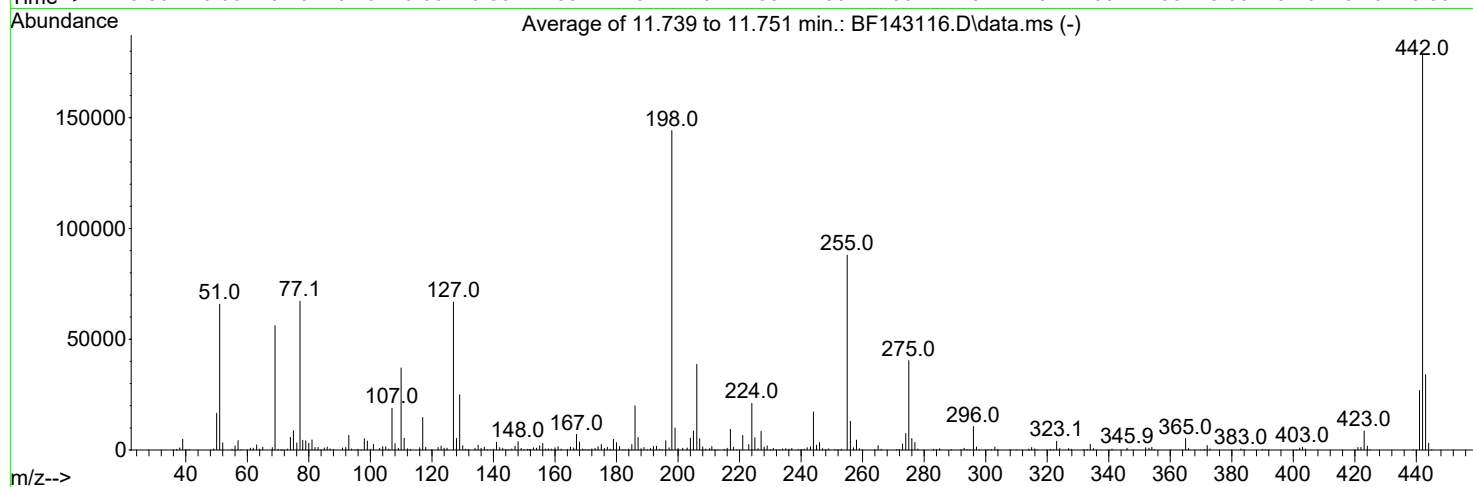


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071625\
Data File : BF143116.D
Acq On : 16 Jul 2025 19:09
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF071525.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Jul 15 17:53:25 2025

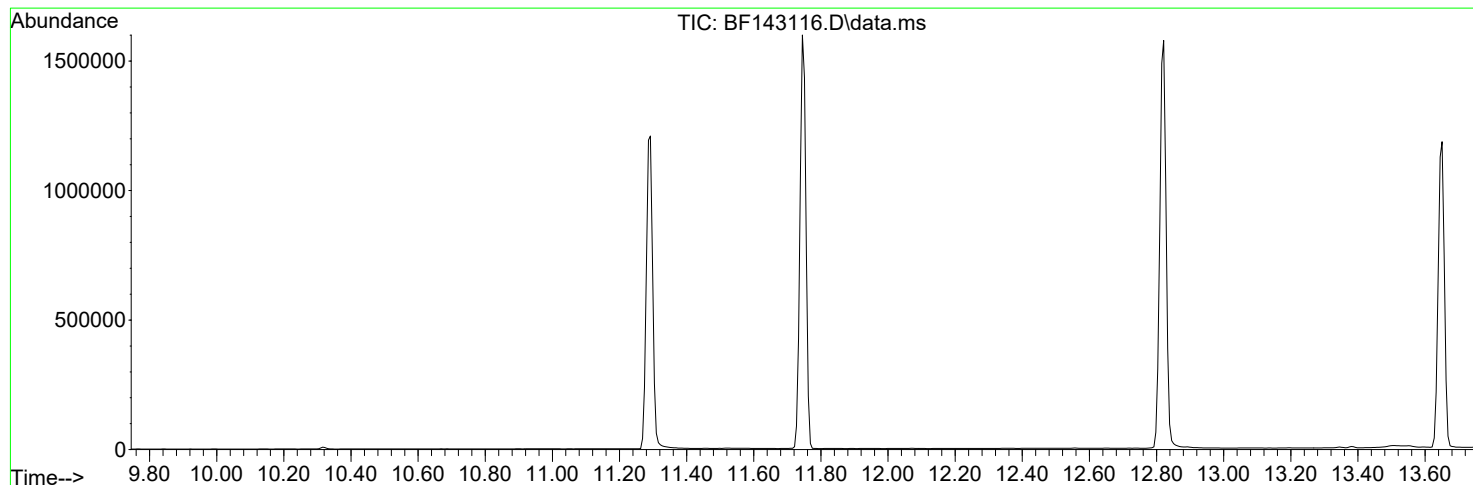

AutoFind: Scans 1623, 1624, 1625; Background Corrected with Scan 1617

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
68	69	0.00	2	1.9	1058	PASS
69	69	100	100	100.0	56128	PASS
70	69	0.00	2	0.6	318	PASS
197	198	0.00	2	0.7	1000	PASS
198	198	100	100	100.0	144192	PASS
199	198	5	9	6.8	9864	PASS
365	198	1	100	3.6	5196	PASS
441	443	0.01	150	79.1	26908	PASS
442	442	100	100	100.0	178251	PASS
443	442	15	24	19.1	34024	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
7/16/2025	BNA_F	<u>BF143116.D</u>
Compound Name	Response	Retention Time
DDT	269374	13.651
DDD	2925	13.38
DDE	0	
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
2925	272299	1.07

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071625\
Data File : BF143116.D
Acq On : 16 Jul 2025 19:09
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jul 17 03:11:34 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF071525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 15 17:53:25 2025
Response via : Initial Calibration

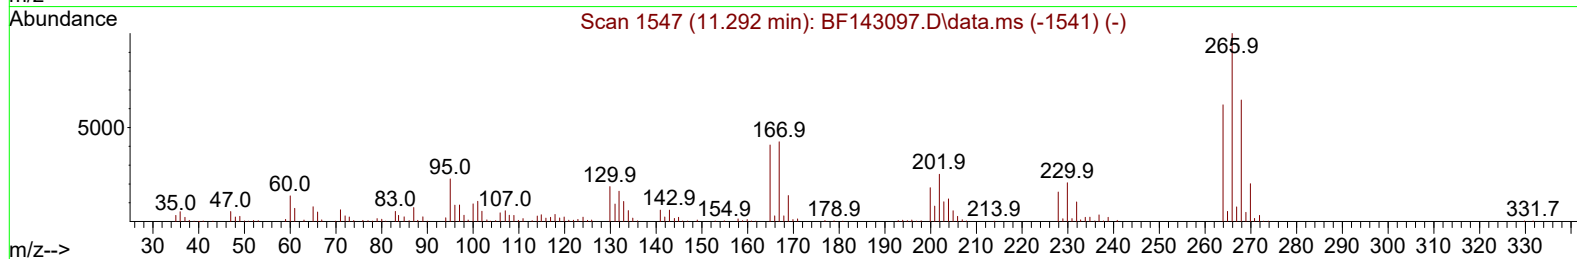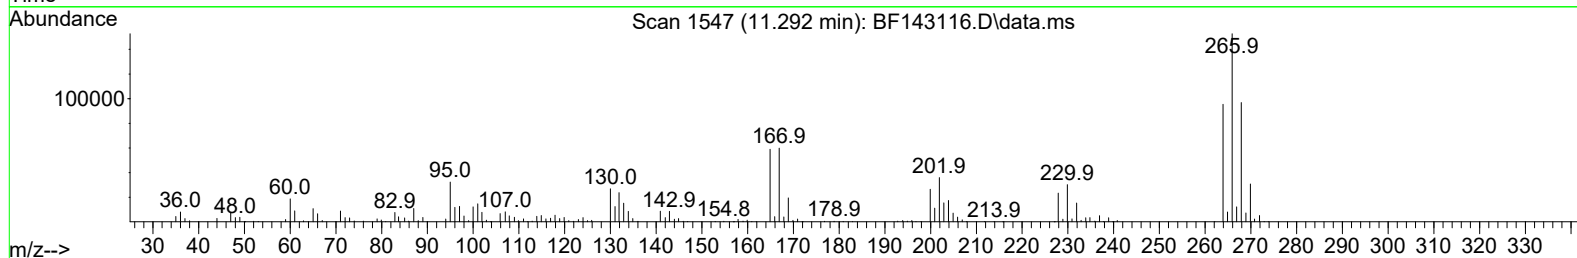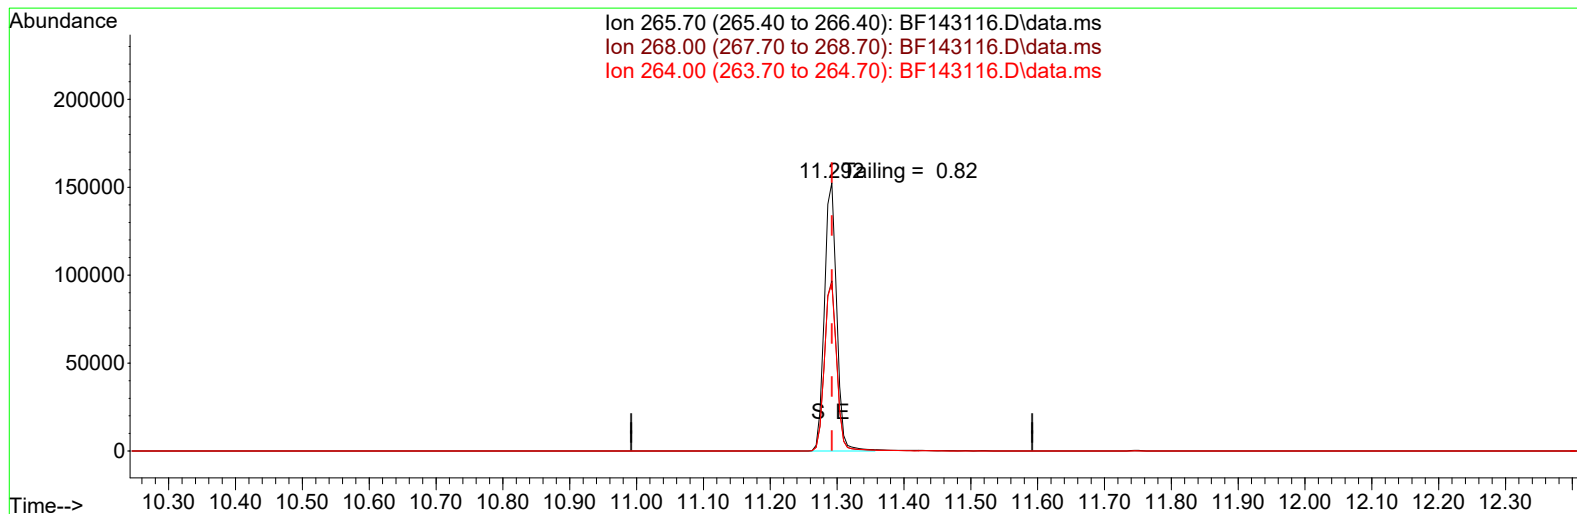

TIC: BF143116.D\data.ms

(70) Pentachlorophenol (C)

11.292min (-0.000) 32920.43 ng




response 195924

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.70	63.41
264.00	62.10	62.55
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071625\
Data File : BF143116.D
Acq On : 16 Jul 2025 19:09
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jul 17 03:11:34 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF071525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 15 17:53:25 2025
Response via : Initial Calibration

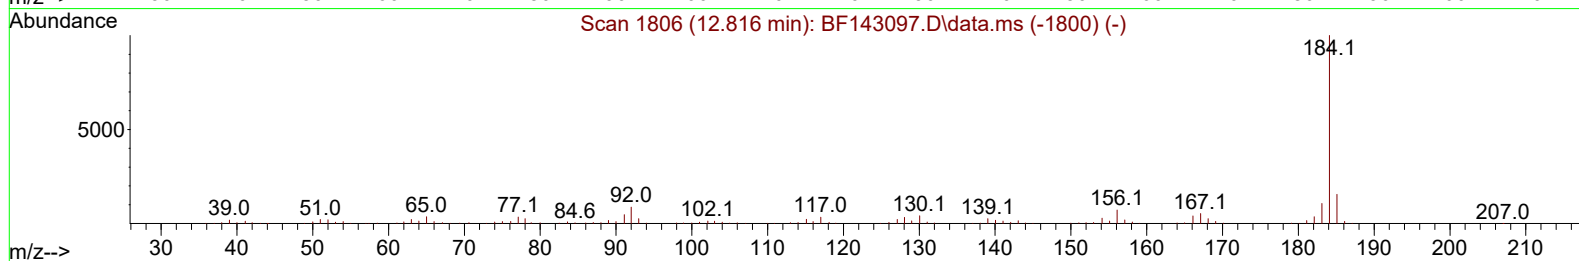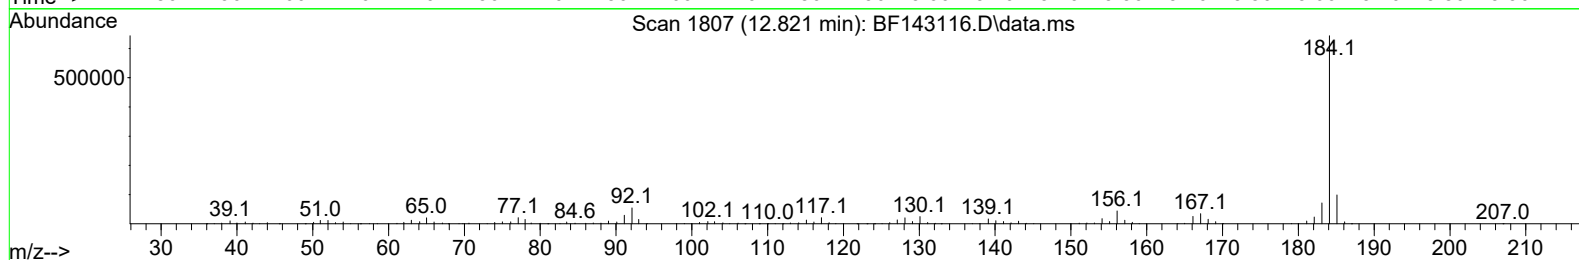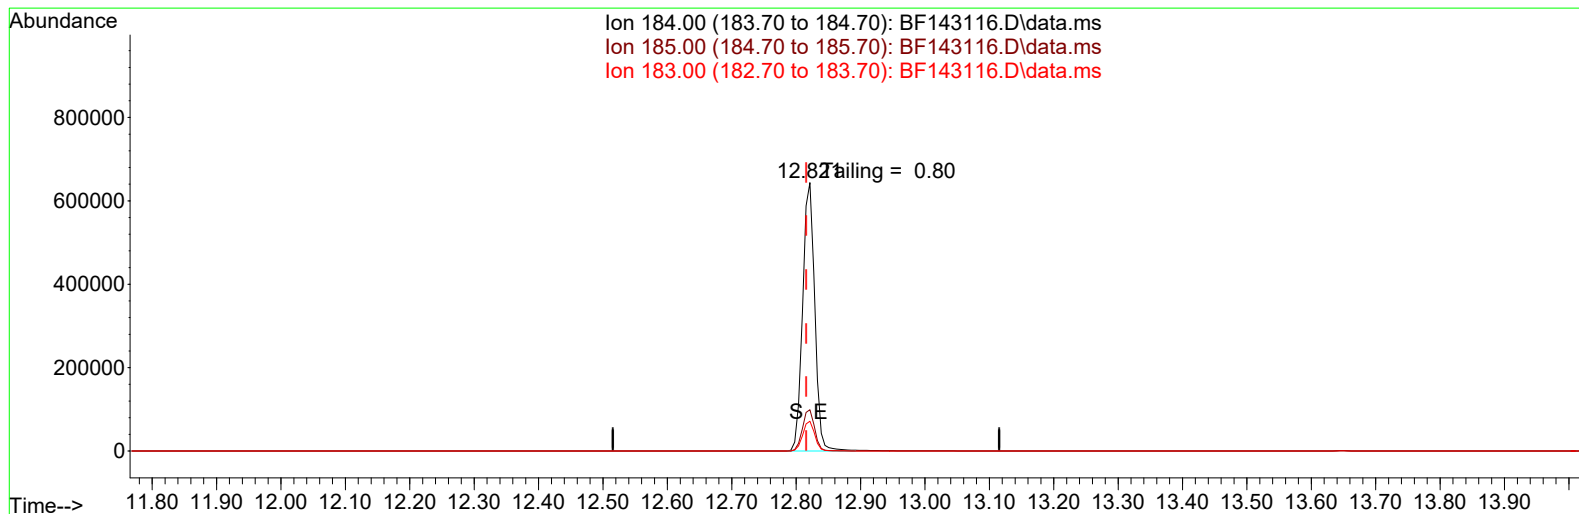

TIC: BF143116.D\data.ms

(77) Benzidine

12.821min (+ 0.006) 0.00 ng

response 848698

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	15.39
183.00	10.70	11.10
0.00	0.00	0.00