


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM070925\
Data File : BM050376.D
Acq On : 08 Jul 2025 11:59
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM070925.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Jul 08 18:32:25 2025

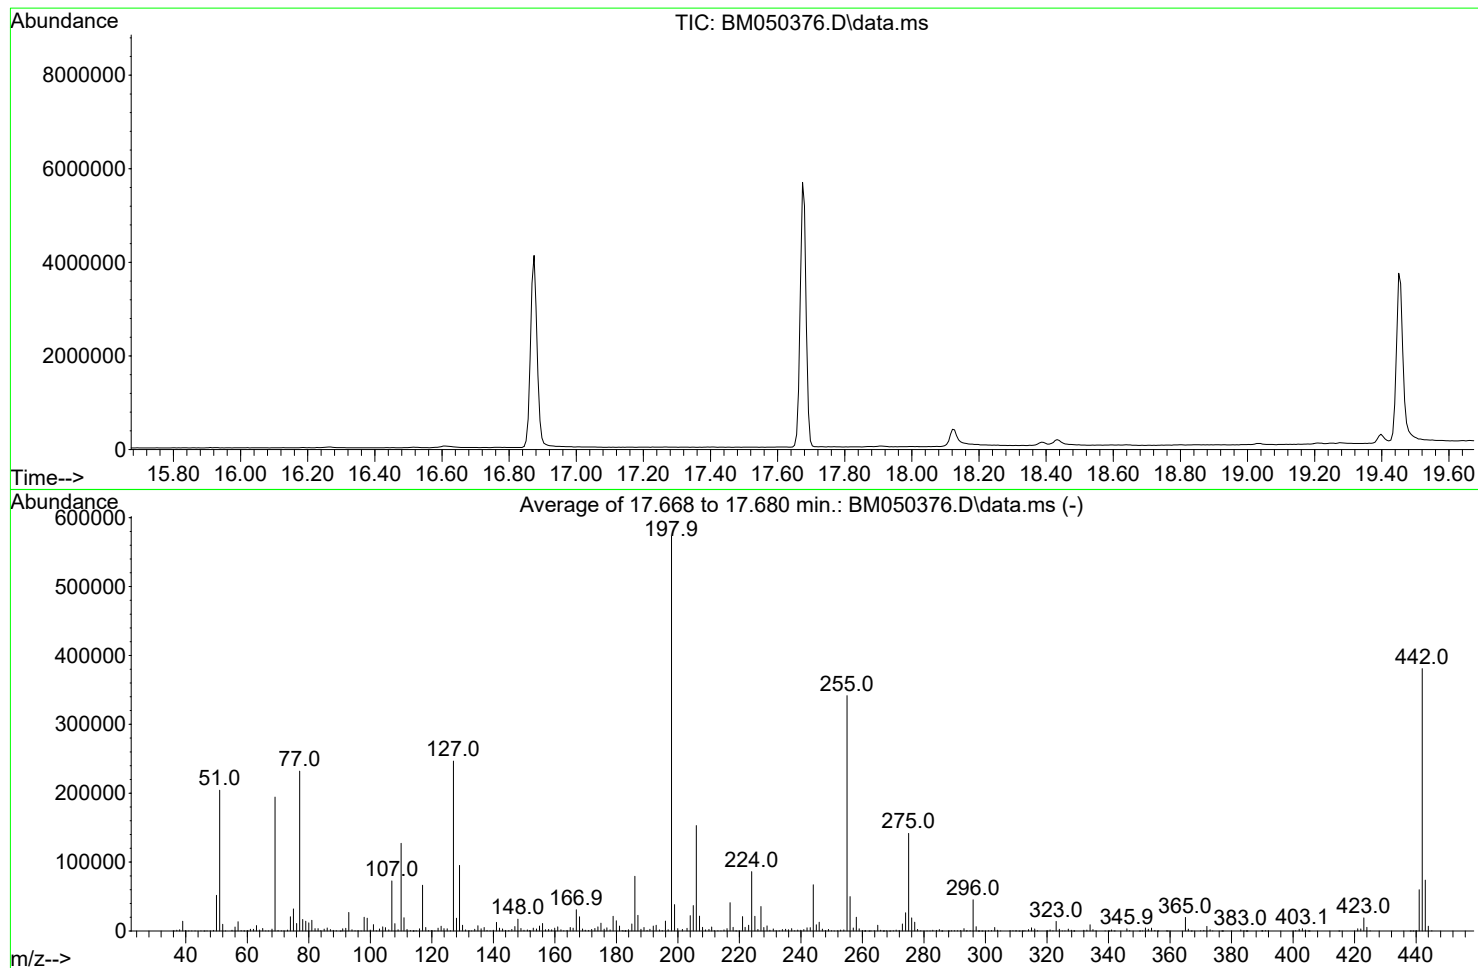

AutoFind: Scans 2496, 2497, 2498; Background Corrected with Scan 2489

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
68	69	0.00	2	1.5	2822	PASS
69	69	100	100	100.0	194463	PASS
70	69	0.00	2	0.5	943	PASS
197	198	0.00	2	0.3	1831	PASS
198	198	100	100	100.0	573141	PASS
199	198	5	9	6.7	38261	PASS
365	198	1	100	3.4	19723	PASS
441	443	0.01	150	81.4	60059	PASS
442	442	100	100	100.0	380992	PASS
443	442	15	24	19.4	73781	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
7/9/2025	BNA_M	<u>BM050376.D</u>
Compound Name	Response	Retention Time
DDT	1842274	20.692
DDD	18107	20.309
DDE	1079	19.75
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
19186	1861460	1.03

Instrument :
BNA_M
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM070925\
Data File : BM050376.D
Acq On : 08 Jul 2025 11:59
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Jul 08 17:14:47 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM070925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 08 15:59:58 2025
Response via : Initial Calibration

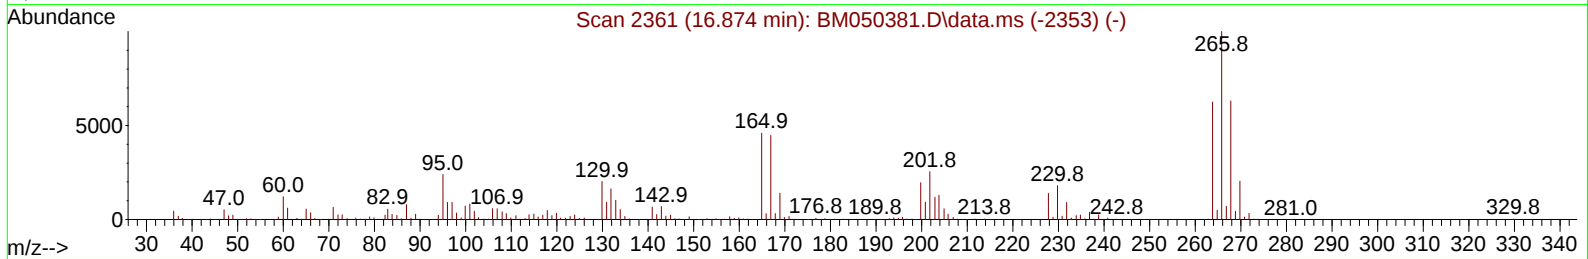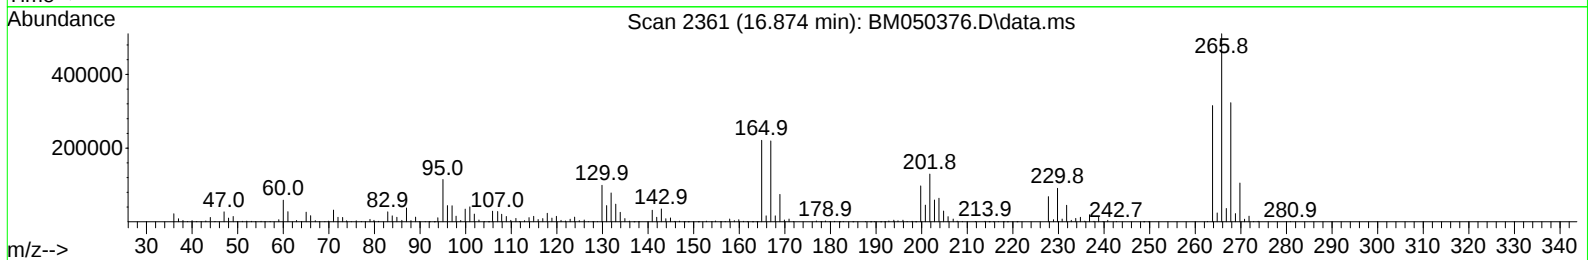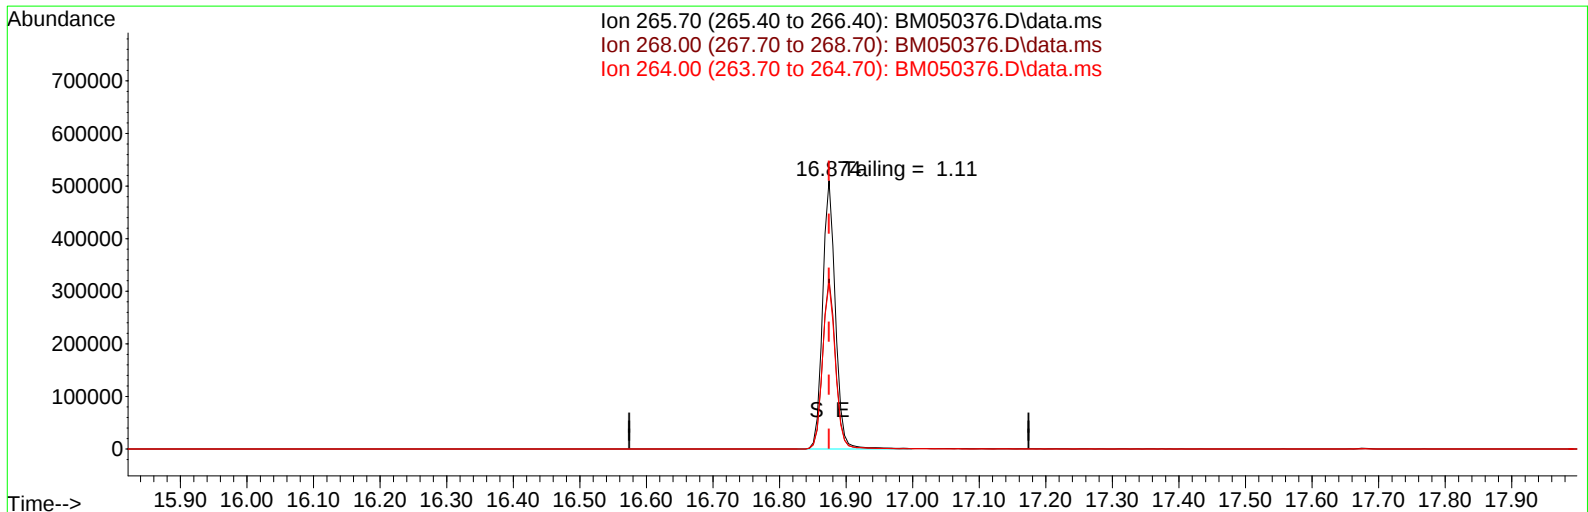

TIC: BM050376.D\data.ms

(70) Pentachlorophenol (C)

16.874min (+ 0.000) 0.00 ng




response 680595

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	63.37
264.00	62.40	61.79
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM070925\
Data File : BM050376.D
Acq On : 08 Jul 2025 11:59
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Jul 08 17:14:47 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM070925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 08 15:59:58 2025
Response via : Initial Calibration

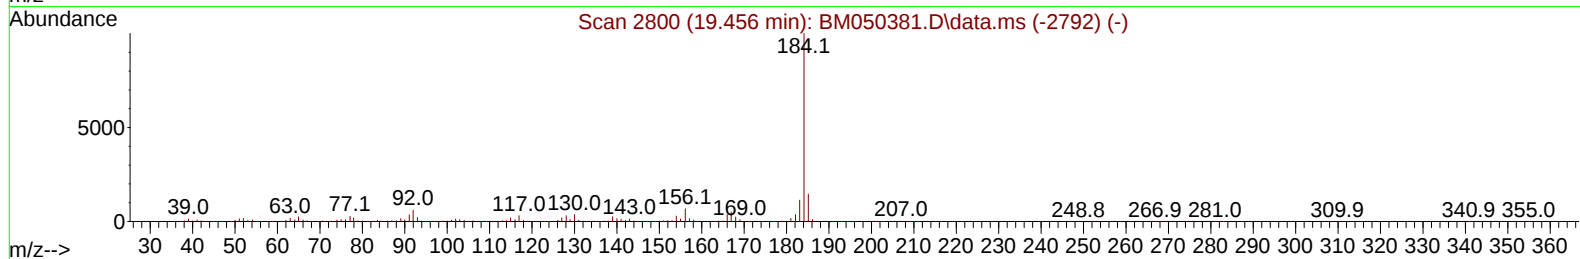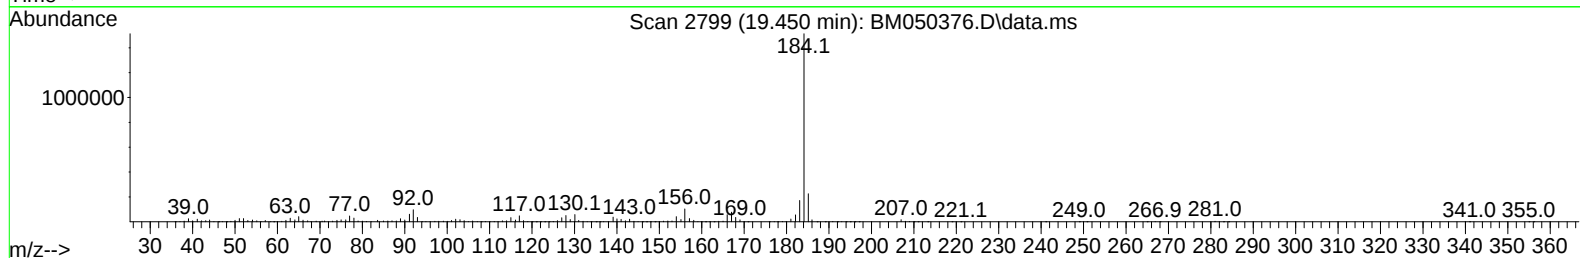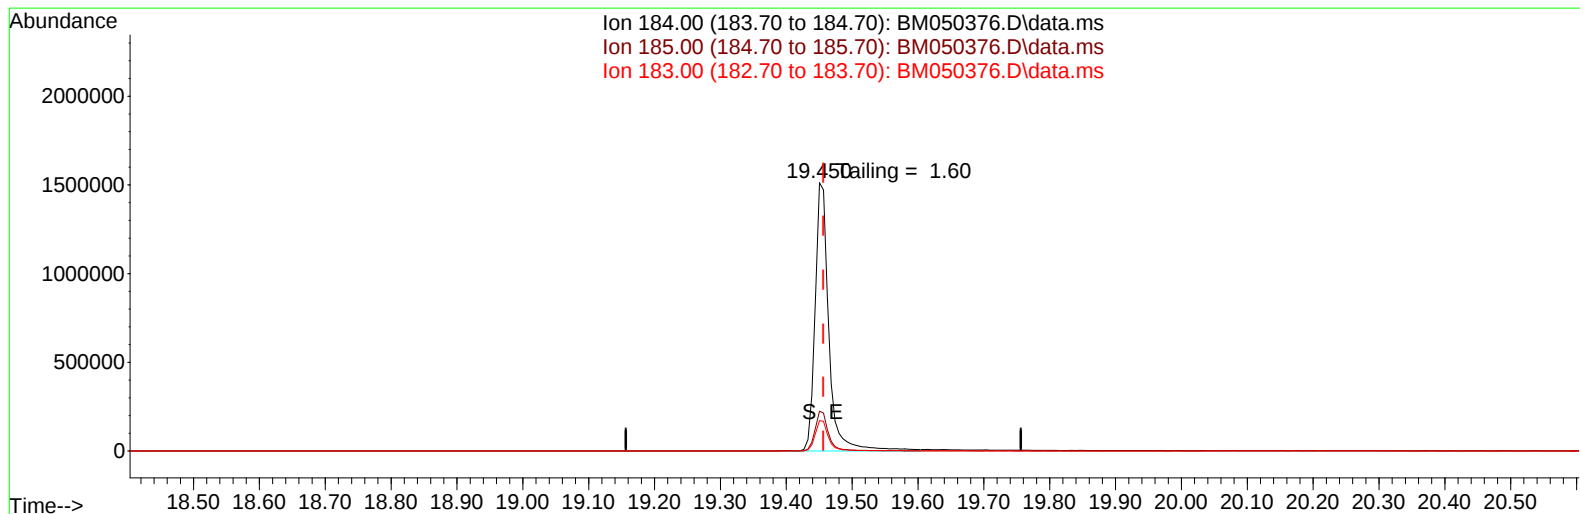

TIC: BM050376.D\data.ms

(77) Benzidine

19.450min (-0.006) 78341.13 ng

response 2201890

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.87
183.00	11.30	11.33
0.00	0.00	0.00