



BFB

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN062525\
Data File : VN087161.D
Acq On : 25 Jun 2025 08:25
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U070825W.M
Title : SW846 8260
Last Update : Wed Jul 09 04:25:34 2025

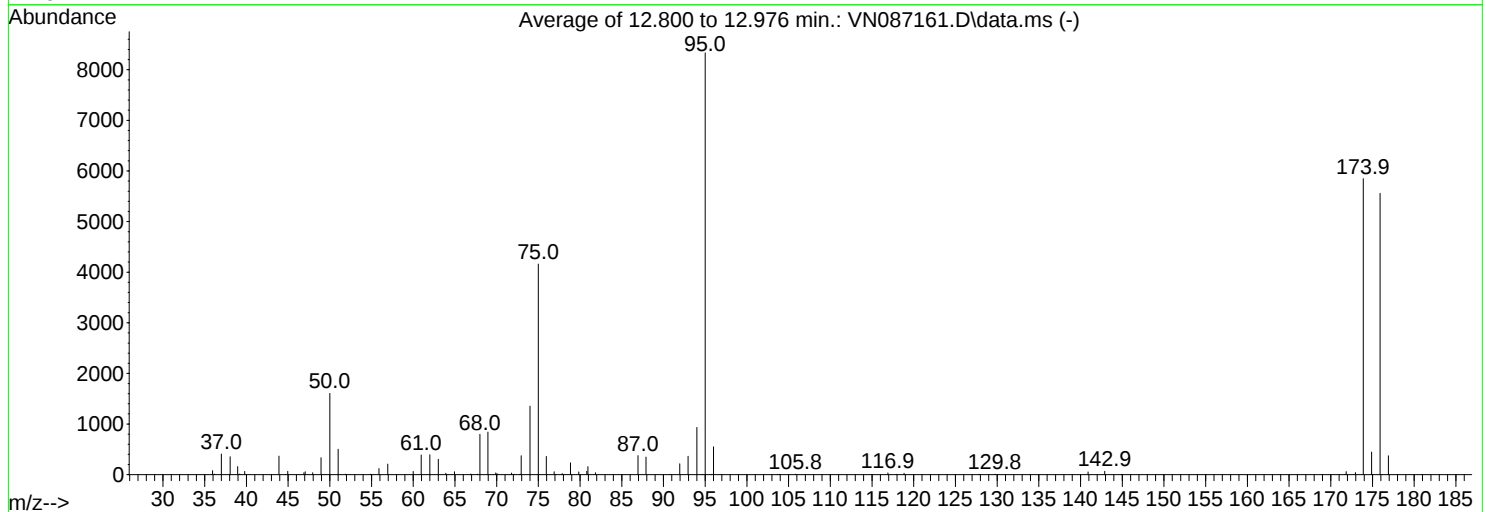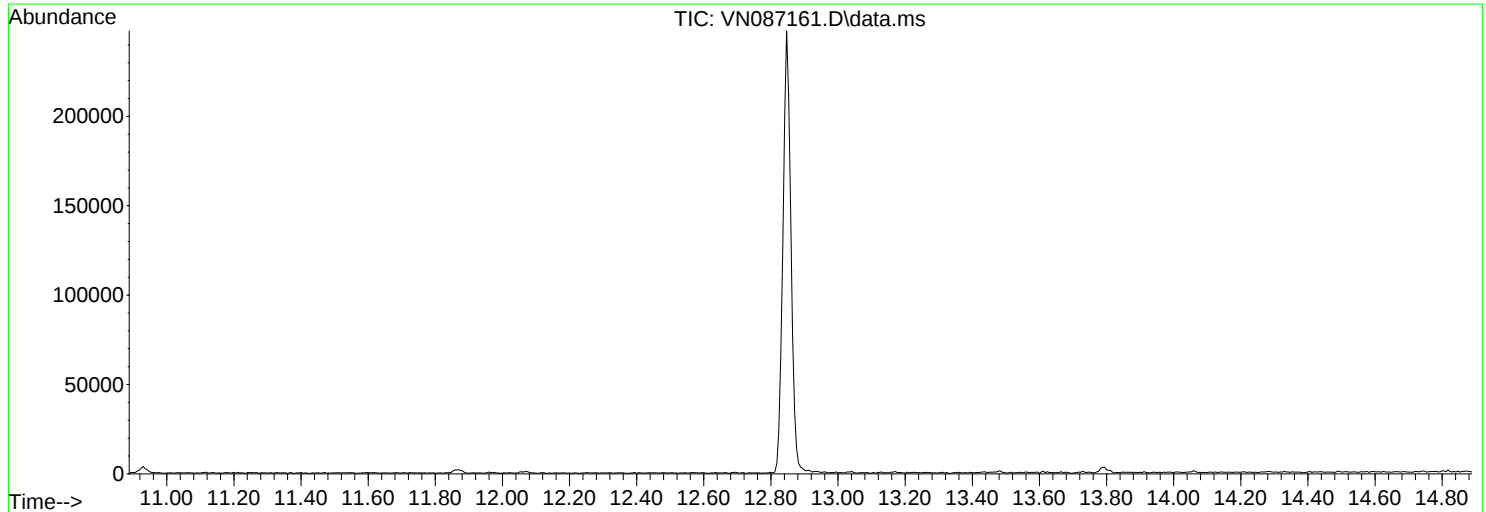

AutoFind: Averaged scan 1844 to 1874; Bkg corrected with scan 1843

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.3	1607	PASS
75	95	30	60	49.9	4160	PASS
95	95	100	100	100.0	8333	PASS
96	95	5	9	6.6	550	PASS
173	174	0.00	2	0.7	41	PASS
174	95	50	100	70.2	5847	PASS
175	174	5	9	7.6	447	PASS
176	174	95	101	95.0	5556	PASS
177	176	5	9	6.7	373	PASS