

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL070725\
 Data File : PL096247.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Jul 2025 12:30
 Operator : AR\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 07 14:08:41 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL070725.M
 Quant Title : GC Extractables
 QLast Update : Mon Jul 07 14:08:25 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.537	2.828	171.6E6	355.1E6	50.000	50.000
28)	SA Decachlor...	9.019	7.996	132.7E6	239.1E6	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.693	3.841	88704924	117.7E6	500.000	500.000
24)	Chlordane-2	5.217	4.420	95284319	136.1E6	500.000	500.000
25)	Chlordane-3	5.920	5.055	369.2E6	398.6E6	500.000	500.000
26)	Chlordane-4	6.004	5.118	448.0E6	362.9E6	500.000	500.000
27)	Chlordane-5	6.841	6.013	71924209	141.5E6	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL070725\
Data File : PL096247.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Jul 2025 12:30
Operator : AR\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 07 14:08:41 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL070725.M
Quant Title : GC Extractables
QLast Update : Mon Jul 07 14:08:25 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

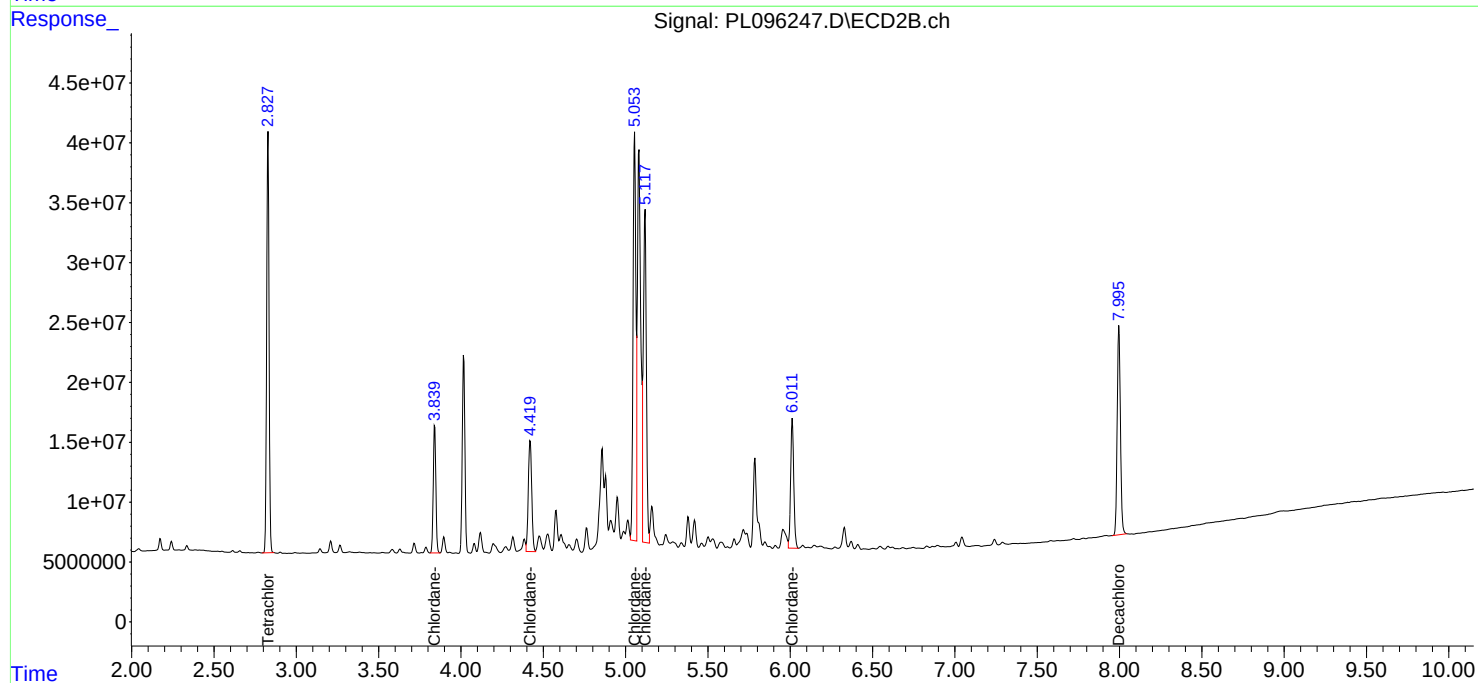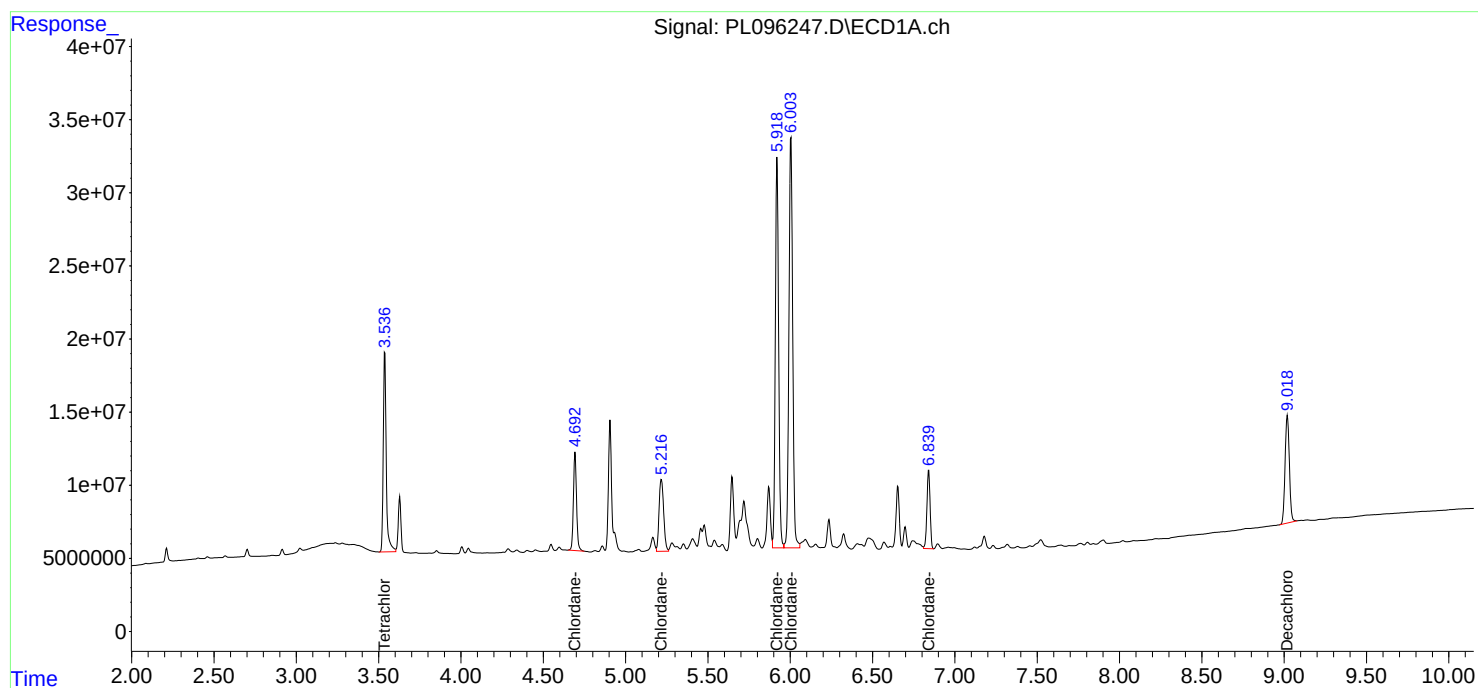


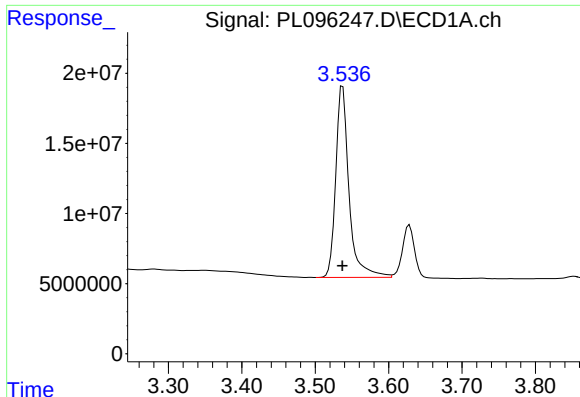

#1 Tetrachloro-m-xylene


R.T.: 3.537 min
Delta R.T.: 0.000 min
Response: 171642137
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

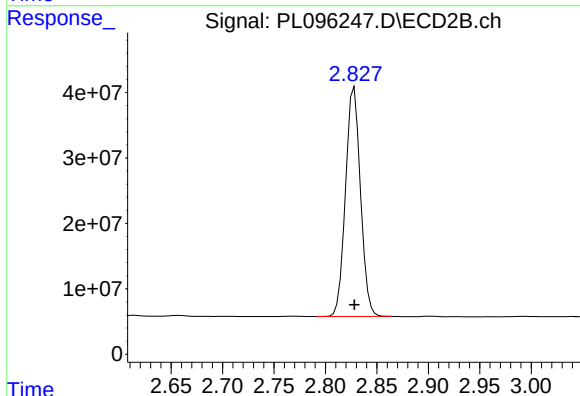


#1 Tetrachloro-m-xylene

R.T.: 2.828 min
Delta R.T.: 0.000 min
Response: 355075037
Conc: 50.00 ng/ml

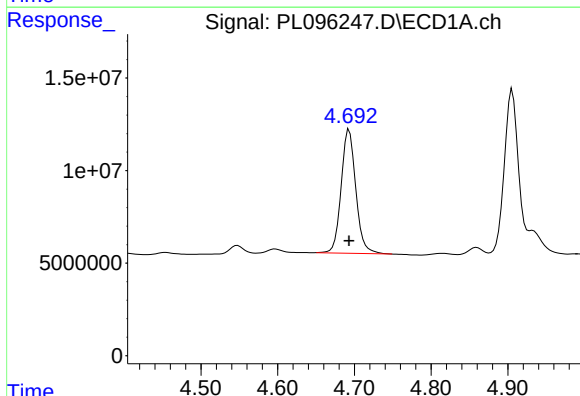


#23 Chlordane-1

R.T.: 4.693 min
Delta R.T.: 0.000 min
Response: 88704924
Conc: 500.00 ng/ml

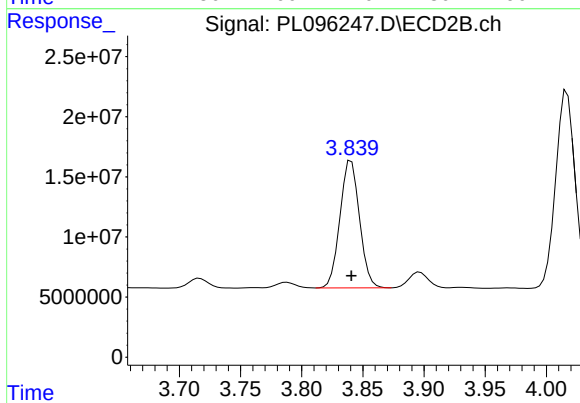

#23 Chlordane-1


R.T.: 3.841 min
Delta R.T.: 0.000 min
Response: 117738541
Conc: 500.00 ng/ml

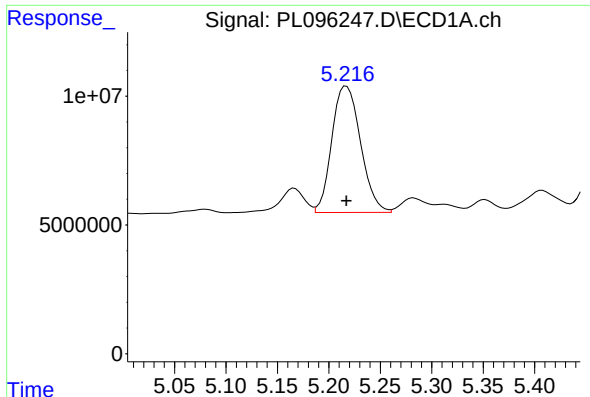

#24 Chlordane-2


R.T.: 5.217 min
Delta R.T.: 0.000 min
Response: 95284319
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

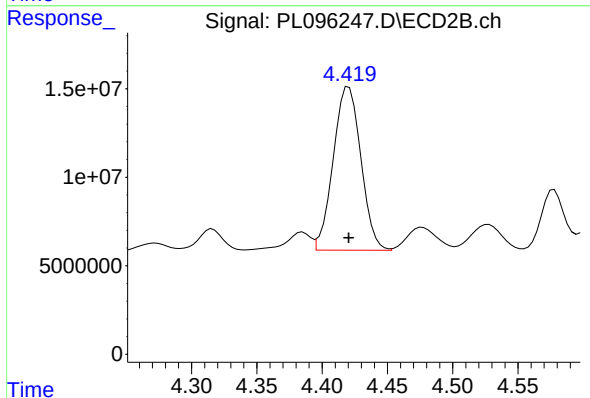


#24 Chlordane-2

R.T.: 4.420 min
Delta R.T.: 0.000 min
Response: 136085748
Conc: 500.00 ng/ml

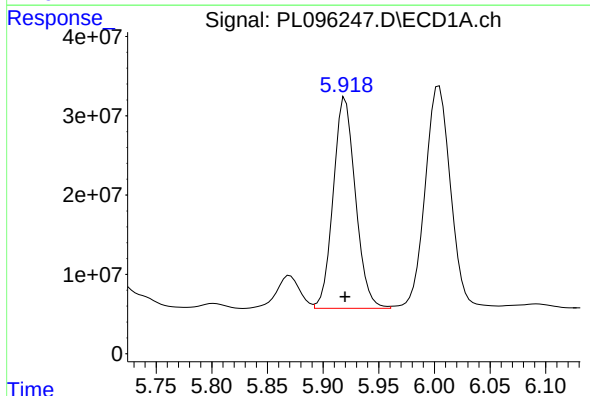


#25 Chlordane-3

R.T.: 5.920 min
Delta R.T.: 0.000 min
Response: 369220532
Conc: 500.00 ng/ml

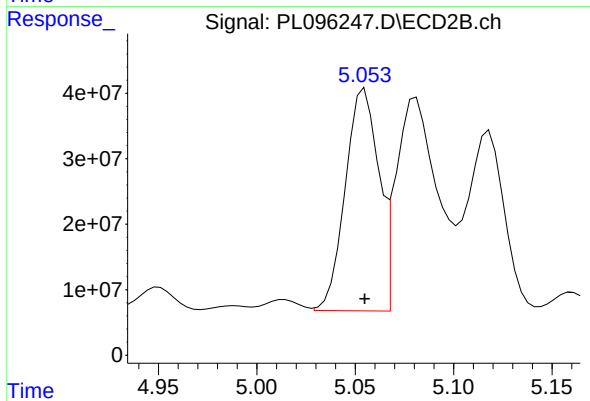

#25 Chlordane-3


R.T.: 5.055 min
Delta R.T.: 0.000 min
Response: 398637596
Conc: 500.00 ng/ml

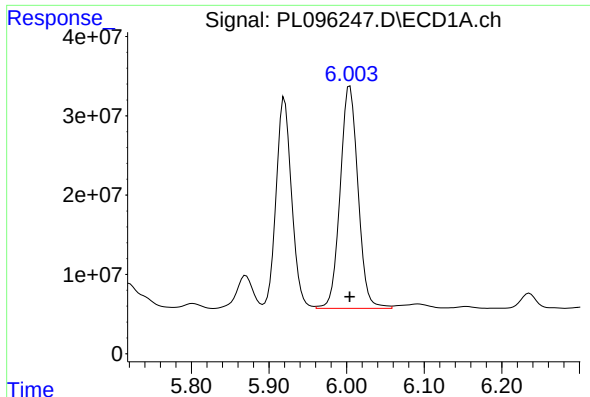

#26 Chlordane-4


R.T.: 6.004 min
Delta R.T.: 0.000 min
Response: 447993243
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

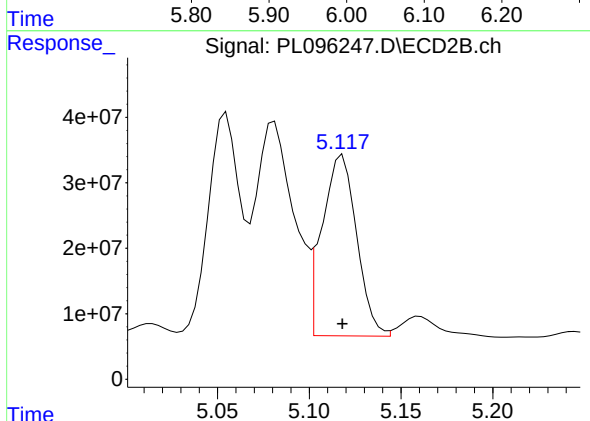


#26 Chlordane-4

R.T.: 5.118 min
Delta R.T.: 0.000 min
Response: 362887002
Conc: 500.00 ng/ml

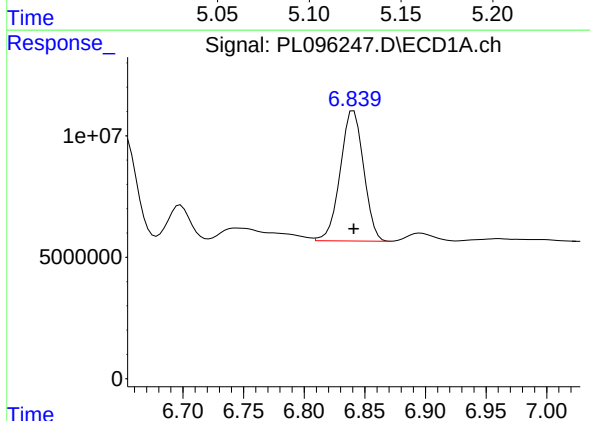


#27 Chlordane-5

R.T.: 6.841 min
Delta R.T.: 0.000 min
Response: 71924209
Conc: 500.00 ng/ml

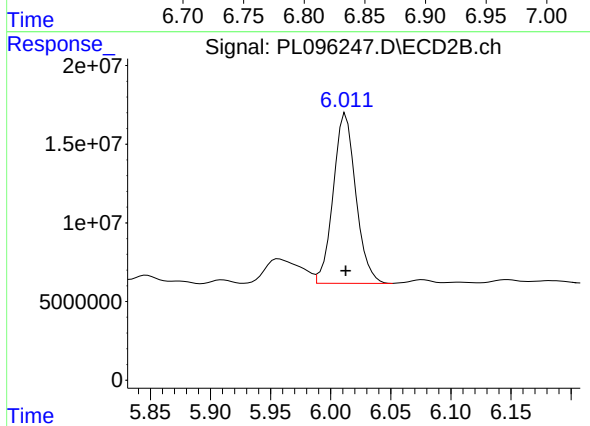

#27 Chlordane-5

R.T.: 6.013 min
Delta R.T.: 0.000 min
Response: 141479033
Conc: 500.00 ng/ml

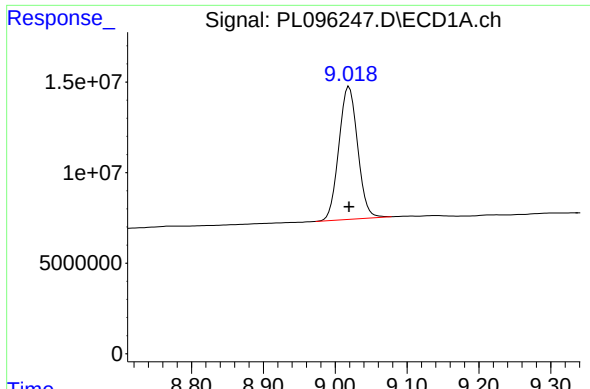

#28 Decachlorobiphenyl


R.T.: 9.019 min

Delta R.T.: 0.000 min

Response: 132747864

Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

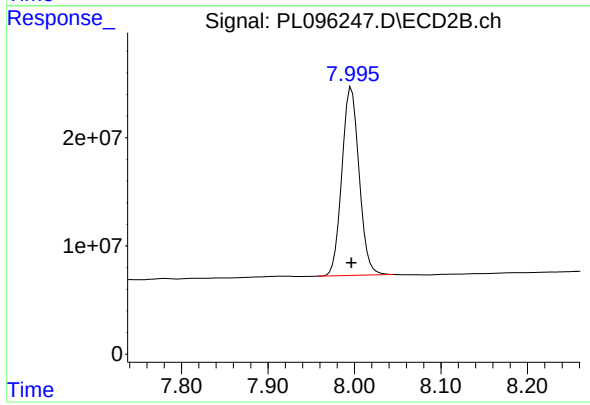

#28 Decachlorobiphenyl

R.T.: 7.996 min

Delta R.T.: 0.000 min

Response: 239141492

Conc: 50.00 ng/ml