

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072225\
 Data File : BF143183.D
 Acq On : 22 Jul 2025 11:54
 Operator : RC/JU
 Sample : Q2638-03
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 OU4-TS-32-071725

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF071725.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF143183.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.269	6	13	21	rVB	554708	895269	38.99%	3.912%
2	5.187	502	509	518	rVB	168570	238572	10.39%	1.042%
3	5.587	571	577	582	rBV	1521374	1973692	85.95%	8.624%
4	6.581	740	746	751	rBV	1585181	2073178	90.28%	9.059%
5	6.963	806	811	816	rVB	594726	719085	31.31%	3.142%
6	7.516	899	905	910	rBV	1102535	1385073	60.32%	6.052%
7	8.245	1023	1029	1034	rBV	748485	956417	41.65%	4.179%
8	8.304	1034	1039	1050	rVB	237027	339209	14.77%	1.482%
9	8.804	1119	1124	1133	rBV	25674	51918	2.26%	0.227%
10	9.316	1206	1211	1216	rBV	1881624	2296398	100.00%	10.034%
11	9.663	1263	1270	1275	rBV5	18301	34014	1.48%	0.149%
12	9.998	1322	1327	1332	rBV	815392	1002698	43.66%	4.381%
13	10.404	1392	1396	1402	rVB	27575	39451	1.72%	0.172%
14	10.704	1443	1447	1455	rVB	239995	332483	14.48%	1.453%
15	10.786	1455	1461	1466	rBV	965993	1281523	55.81%	5.599%
16	11.016	1490	1500	1505	rBV	47377	84645	3.69%	0.370%
17	11.139	1517	1521	1525	rVB2	23398	31191	1.36%	0.136%
18	11.357	1552	1558	1565	rBV7	16606	41267	1.80%	0.180%
19	11.422	1565	1569	1573	rBV	42408	65673	2.86%	0.287%
20	11.486	1575	1580	1587	rVV	651923	898359	39.12%	3.925%
21	11.704	1613	1617	1622	rBV	21177	34816	1.52%	0.152%
22	11.933	1652	1656	1659	rBV2	33009	51570	2.25%	0.225%
23	11.975	1659	1663	1664	rBV2	64042	80913	3.52%	0.354%
24	12.004	1664	1668	1673	rVV	465512	636760	27.73%	2.782%
25	12.186	1695	1699	1707	rVB4	98972	158273	6.89%	0.692%
26	12.563	1760	1763	1770	rVB5	37147	58573	2.55%	0.256%
27	12.627	1771	1774	1781	rVB4	26983	56595	2.46%	0.247%
28	12.698	1782	1786	1797	rBV	127772	296388	12.91%	1.295%
29	12.792	1798	1802	1810	rVV	119526	183089	7.97%	0.800%
30	12.927	1821	1825	1834	rVB	90111	137392	5.98%	0.600%
31	13.069	1844	1849	1855	rVB	1221376	1559674	67.92%	6.815%
32	13.963	1997	2001	2010	rVB2	302119	439645	19.14%	1.921%
33	14.121	2024	2028	2036	rVB	707537	1142637	49.76%	4.993%
34	14.592	2104	2108	2113	rBV	287141	400771	17.45%	1.751%
35	15.263	2218	2222	2233	rVB	497876	794087	34.58%	3.470%
36	15.633	2280	2285	2289	rBV	277869	439874	19.15%	1.922%

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072225\
Data File : BF143183.D
Acq On : 22 Jul 2025 11:54
Operator : RC/JU
Sample : Q2638-03
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-TS-32-071725

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF071725.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	16.127	2364	2369	2374	rBV	296798	496806	21.63%	2.171%
38	17.815	2651	2656	2660	rBV2	178381	393590	17.14%	1.720%
39	18.309	2735	2740	2752	rVB	159656	365492	15.92%	1.597%
40	18.680	2797	2803	2809	rBV2	148039	419440	18.27%	1.833%




Sum of corrected areas: 22886500

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072225\
Data File : BF143183.D
Acq On : 22 Jul 2025 11:54
Operator : RC/JU
Sample : Q2638-03
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-TS-32-071725

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF071725.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

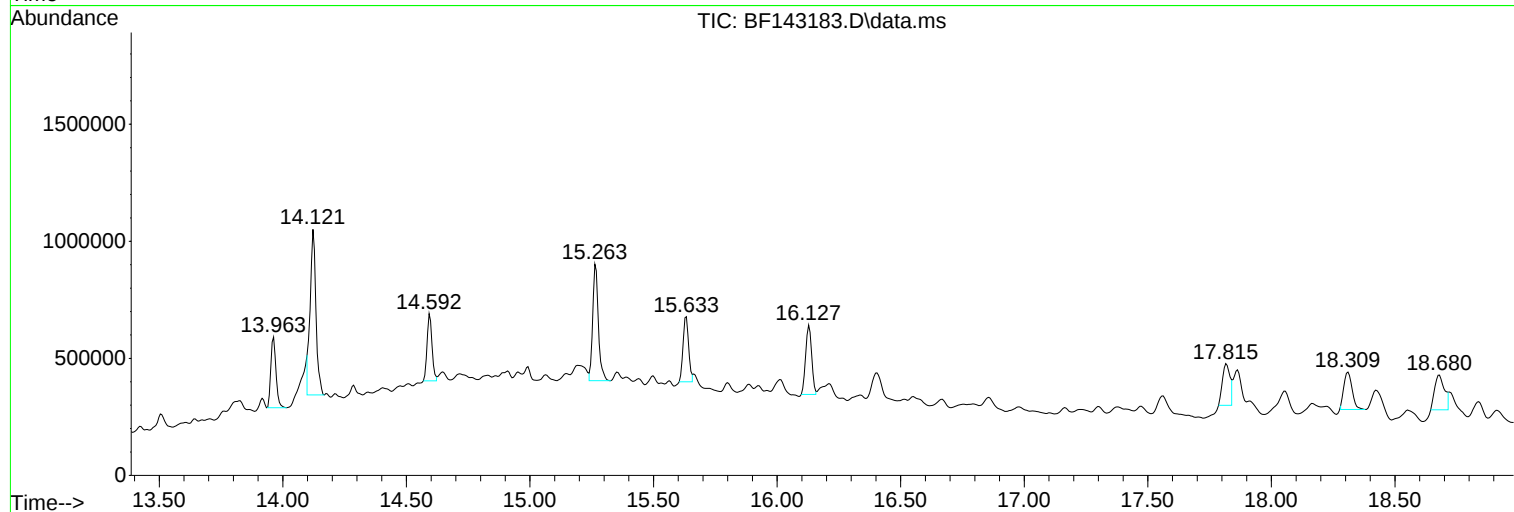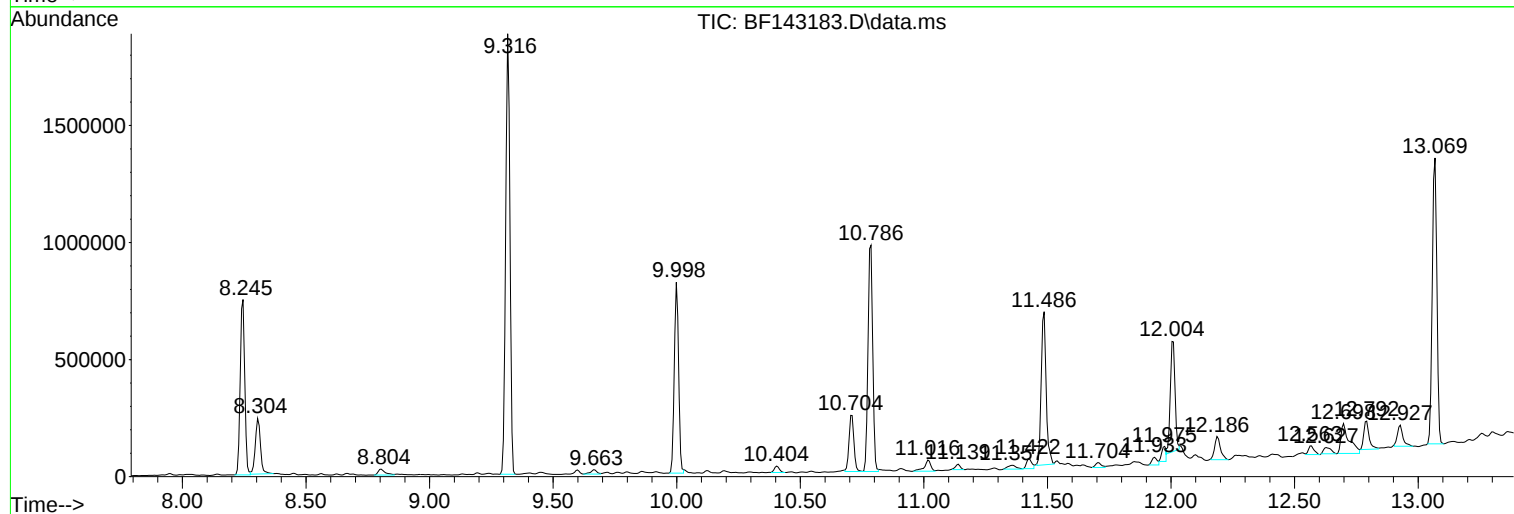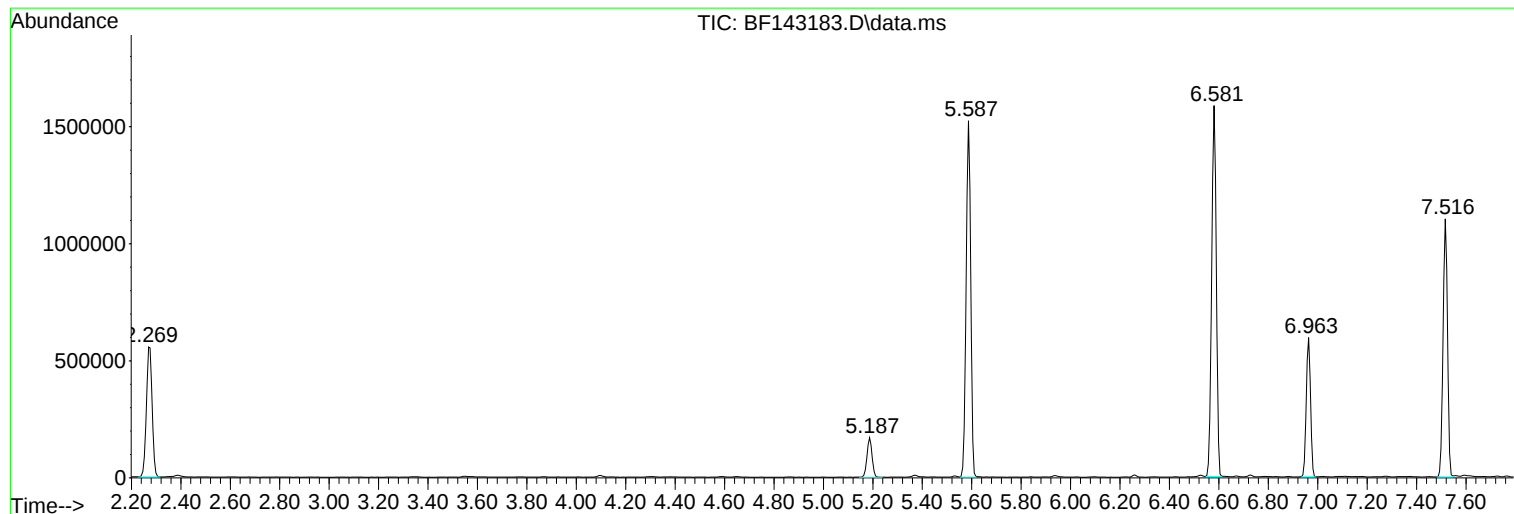

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072225\
Data File : BF143183.D
Acq On : 22 Jul 2025 11:54
Operator : RC/JU
Sample : Q2638-03
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-TS-32-071725

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF071725.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072225\
Data File : BF143183.D
Acq On : 22 Jul 2025 11:54
Operator : RC/JU
Sample : Q2638-03
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-TS-32-071725

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF071725.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------