

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY072125\
 Data File : VY023019.D
 Acq On : 21 Jul 2025 12:16
 Operator : SY/MD
 Sample : Q2638-09
 Misc : 4.55g/5.0mL/MSVOA_Y/SOIL/B
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 OU4-TS-35-071725

Quant Time: Jul 22 04:49:35 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y071825S.M
 Quant Title : SW846 8260
 QLast Update : Sat Jul 19 01:50:49 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.707	168	299685	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.610	114	560715	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.414	117	524510	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.347	152	210422	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.061	65	173755	57.273	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	114.540%
35) Dibromofluoromethane	7.628	113	177852	50.003	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	100.000%
50) Toluene-d8	10.103	98	673735	47.766	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	=	95.540%
62) 4-Bromofluorobenzene	12.402	95	217724	49.037	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	=	98.080%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY072125\
Data File : VY023019.D
Acq On : 21 Jul 2025 12:16
Operator : SY/MD
Sample : Q2638-09
Misc : 4.55g/5.0mL/MSVOA_Y/SOIL/B
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
OU4-TS-35-071725

Quant Time: Jul 22 04:49:35 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y071825S.M
Quant Title : SW846 8260
QLast Update : Sat Jul 19 01:50:49 2025
Response via : Initial Calibration




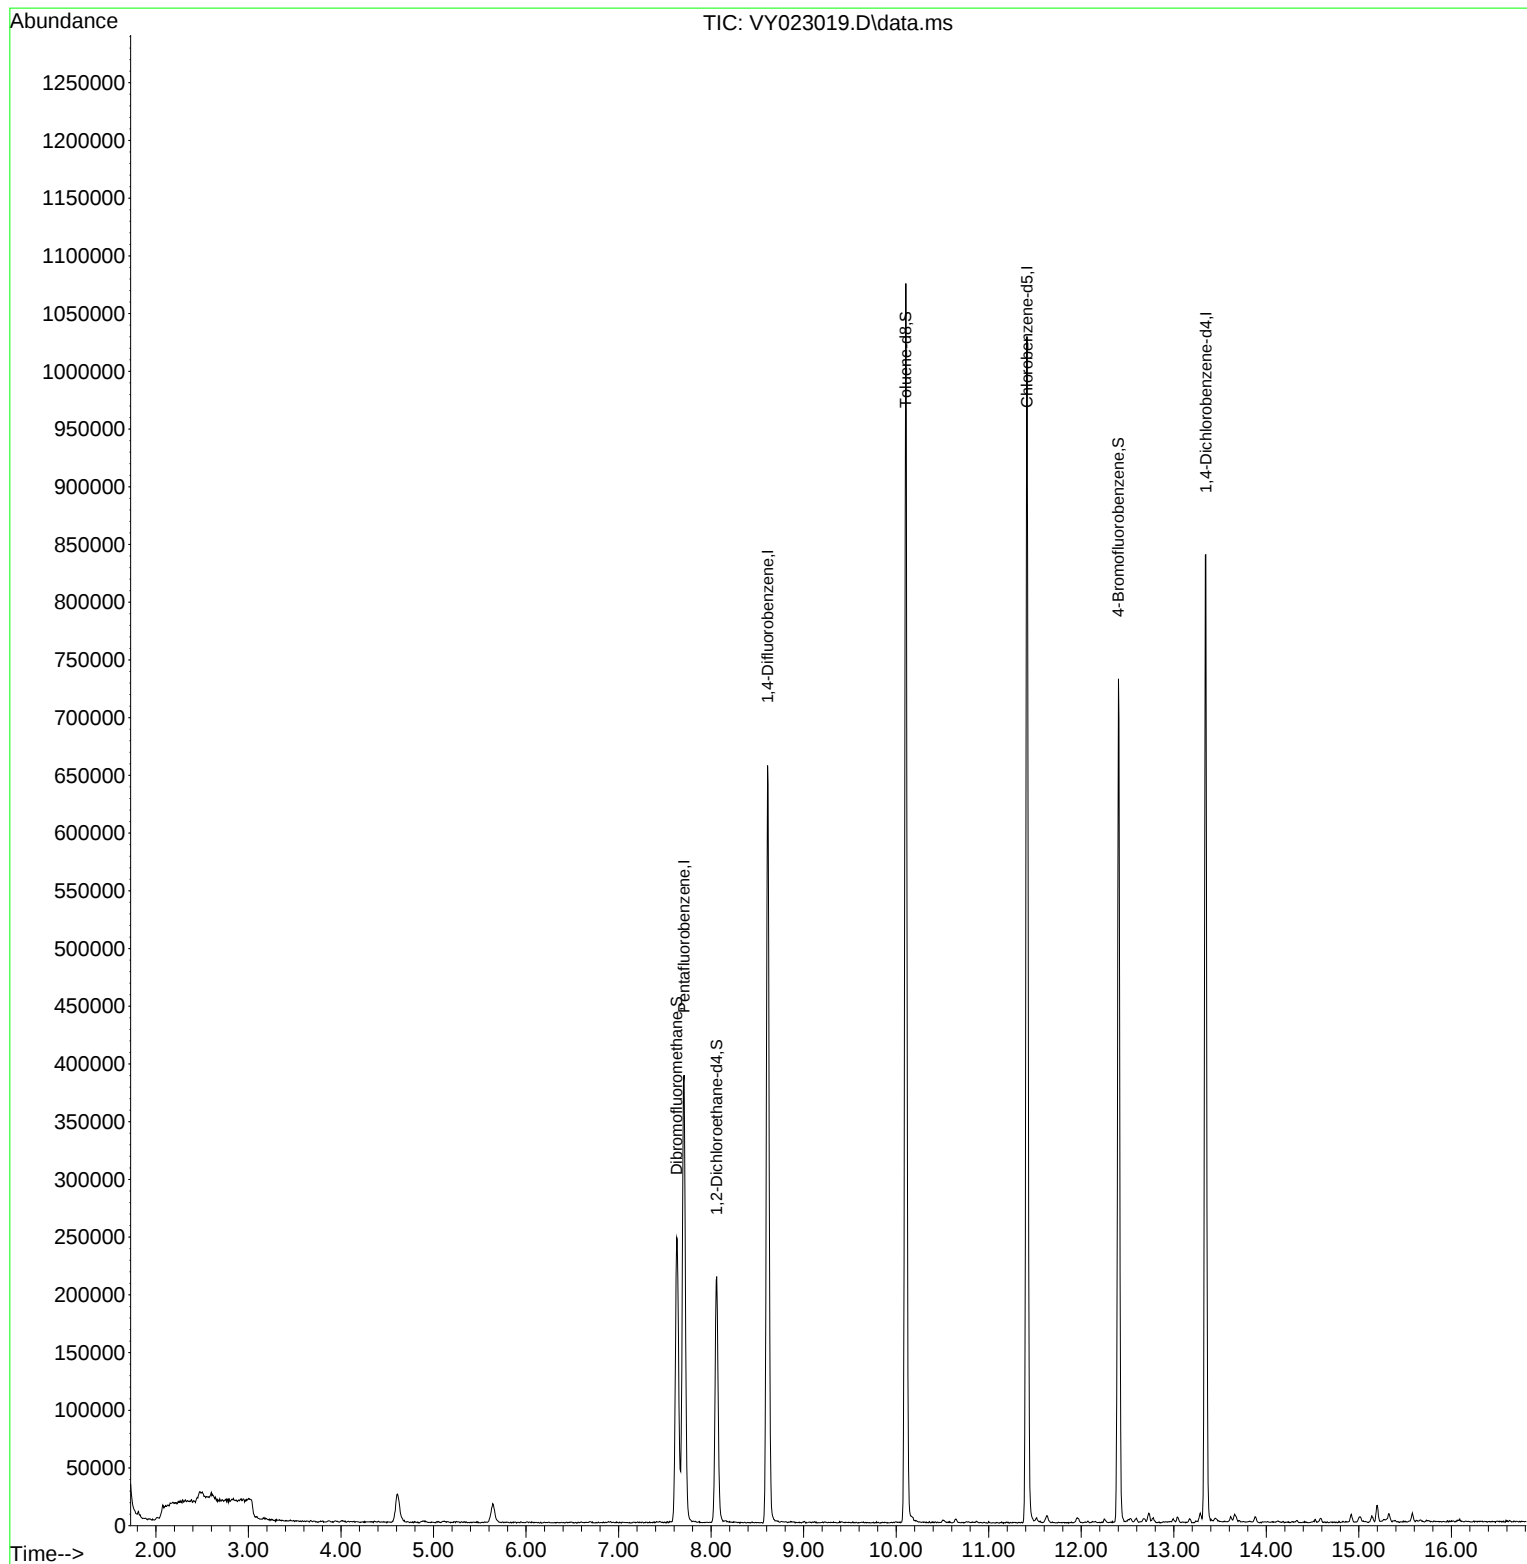


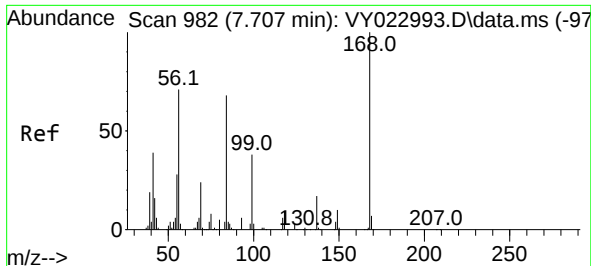

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.707 min Scan# 91
Delta R.T. 0.000 min
Lab File: VY023019.D
Acq: 21 Jul 2025 12:16




Instrument :
MSVOA_Y
ClientSampleId :
OU4-TS-35-071725


Tgt Ion:168 Resp: 299685
Ion Ratio Lower Upper
168 100
99 56.9 44.4 66.6

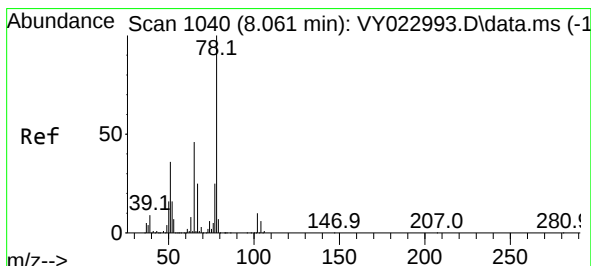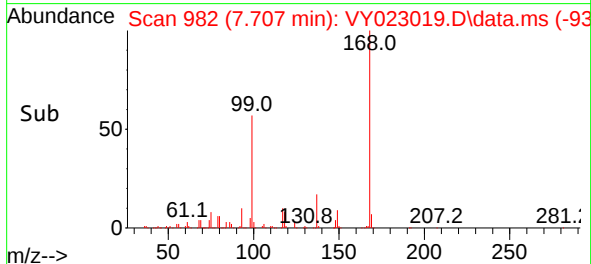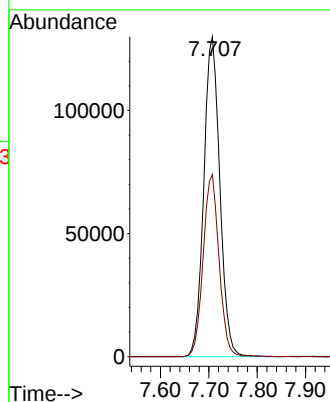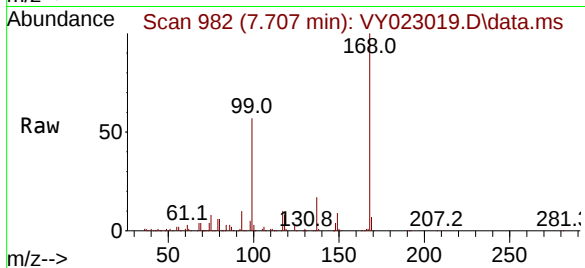

#33
1,2-Dichloroethane-d4
Concen: 57.273 ug/l
RT: 8.061 min Scan# 1040
Delta R.T. 0.000 min
Lab File: VY023019.D
Acq: 21 Jul 2025 12:16

Tgt Ion: 65 Resp: 173755
Ion Ratio Lower Upper
65 100
67 52.3 0.0 107.4

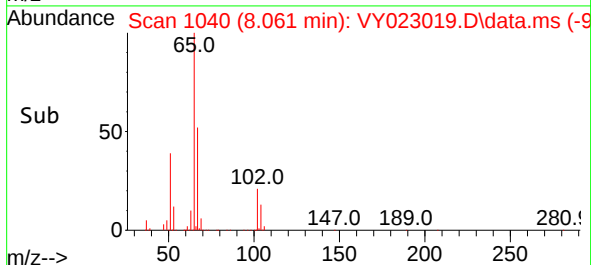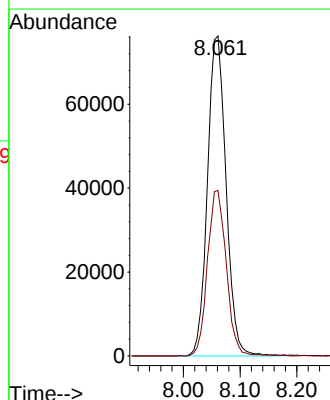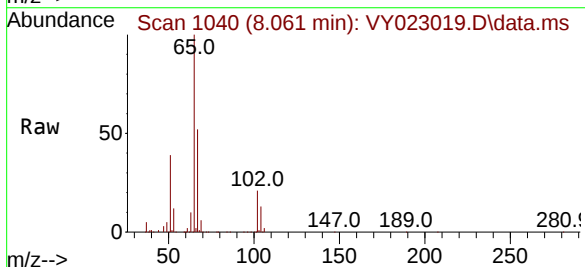

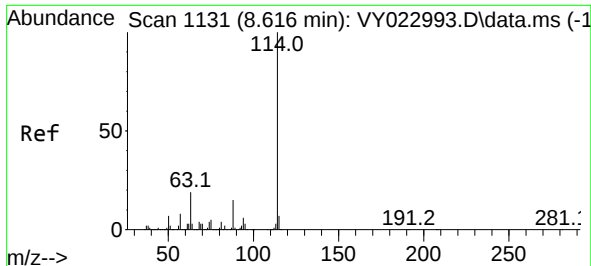

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.610 min Scan# 1131

Delta R.T. -0.006 min

Lab File: VY023019.D

Acq: 21 Jul 2025 12:16

Instrument :

MSVOA_Y

ClientSampleId :

OU4-TS-35-071725





Tgt Ion:114 Resp: 560715

Ion Ratio Lower Upper

114 100

63 19.9 0.0 38.8

88 14.8 0.0 30.2

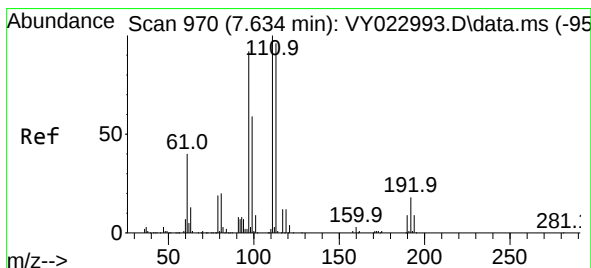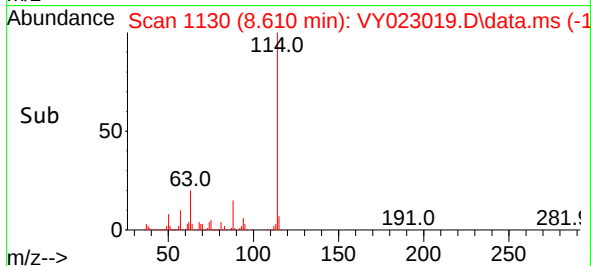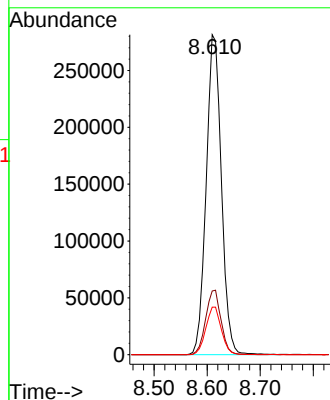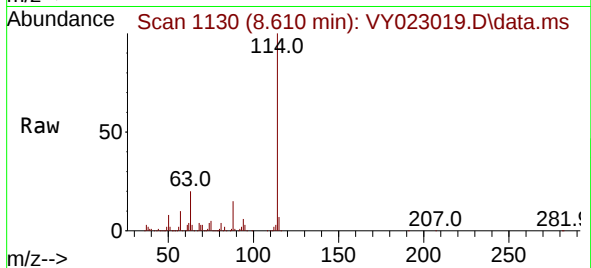

#35

Dibromofluoromethane

Concen: 50.003 ug/l

RT: 7.628 min Scan# 969

Delta R.T. -0.006 min

Lab File: VY023019.D

Acq: 21 Jul 2025 12:16




Tgt Ion:113 Resp: 177852


Ion Ratio Lower Upper

113 100

111 105.3 83.2 124.8

192 19.5 15.3 22.9


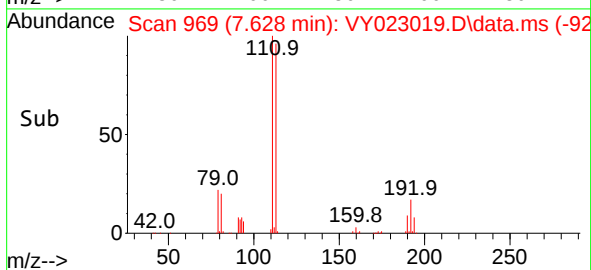
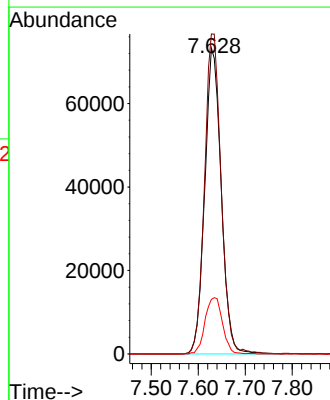
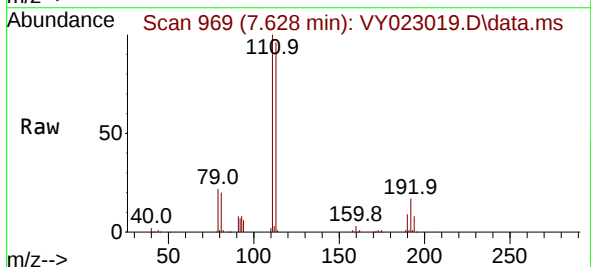


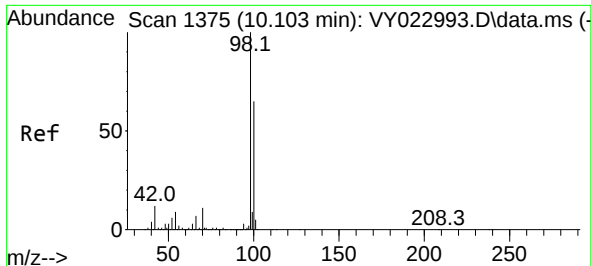

#50
Toluene-d8
Concen: 47.766 ug/l
RT: 10.103 min Scan# 1375
Delta R.T. 0.000 min
Lab File: VY023019.D
Acq: 21 Jul 2025 12:16




Instrument :
MSVOA_Y
ClientSampleId :
OU4-TS-35-071725


Tgt Ion: 98 Resp: 673735
Ion Ratio Lower Upper
98 100
100 64.8 52.2 78.2

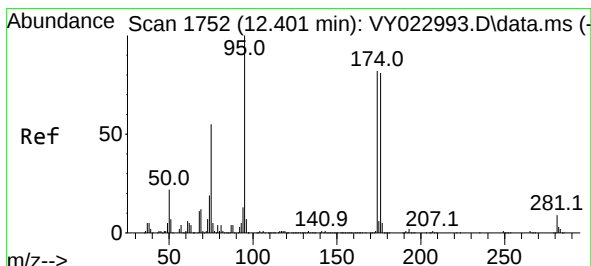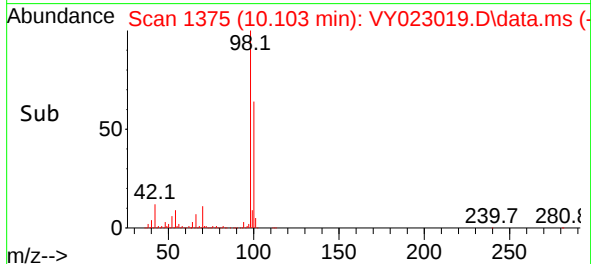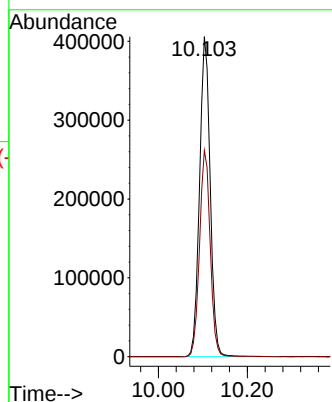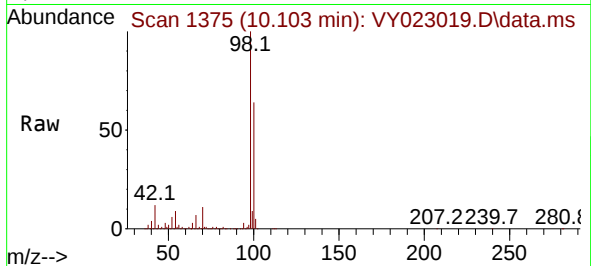

#62
4-Bromofluorobenzene
Concen: 49.037 ug/l
RT: 12.402 min Scan# 1752
Delta R.T. 0.000 min
Lab File: VY023019.D
Acq: 21 Jul 2025 12:16

Tgt Ion: 95 Resp: 217724
Ion Ratio Lower Upper
95 100
174 87.1 0.0 170.8
176 81.0 0.0 163.6

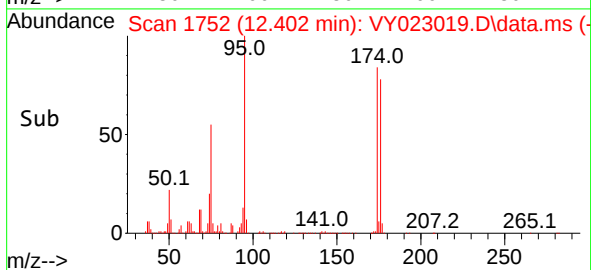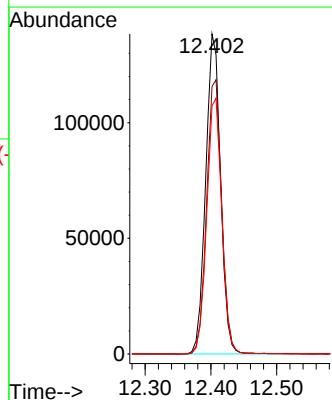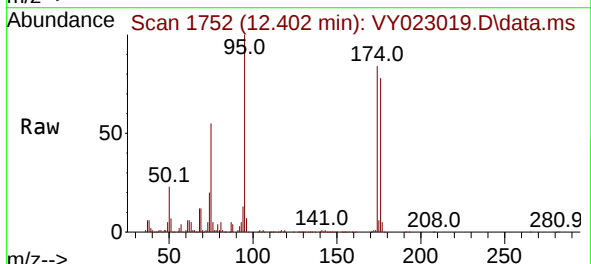

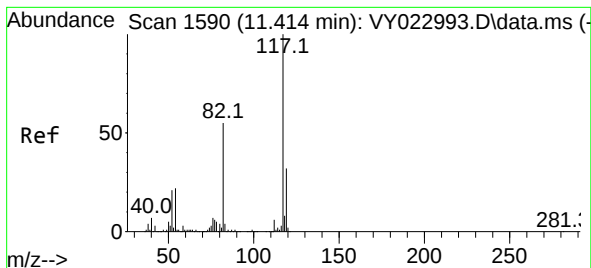

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.414 min Scan# 11

Delta R.T. 0.000 min

Lab File: VY023019.D

Acq: 21 Jul 2025 12:16

Instrument :

MSVOA_Y

ClientSampleId :

OU4-TS-35-071725





Tgt Ion:117 Resp: 524510

Ion Ratio Lower Upper

117 100

82 56.3 44.3 66.5

119 31.5 25.8 38.8

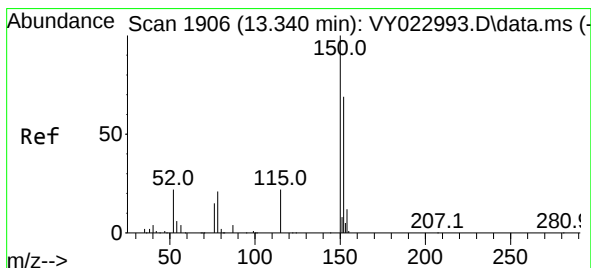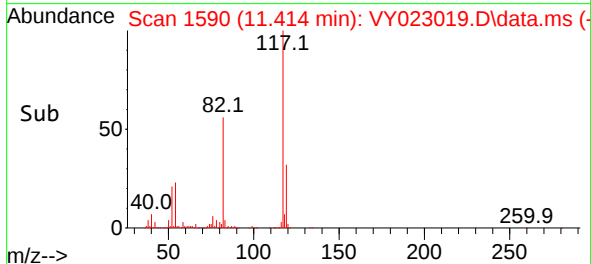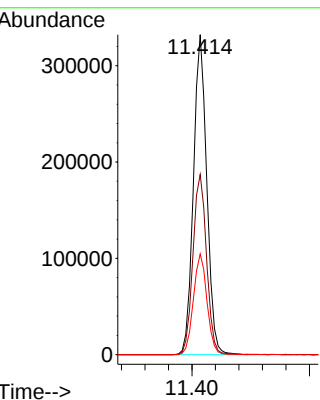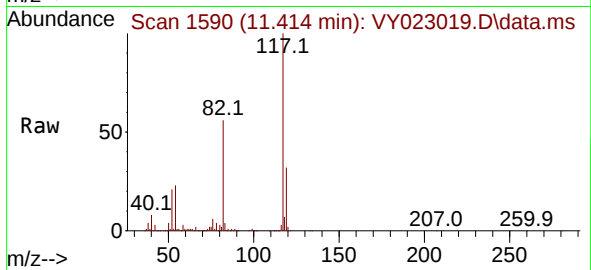

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.347 min Scan# 1907

Delta R.T. 0.006 min

Lab File: VY023019.D

Acq: 21 Jul 2025 12:16

Tgt Ion:152 Resp: 210422

Ion Ratio Lower Upper

152 100

115 58.0 29.4 88.2

150 157.3 0.0 350.0

