

**DATA PACKAGE
GC SEMI-VOLATILES**

PROJECT NAME : RAYMARK SUPERFUND SITE

NOBIS GROUP

585 Middlesex Street

Lowell, MA - 01851

Phone No: 978-683-0891

ORDER ID : Q2639

ATTENTION : Adam Roy



Laboratory Certification ID # 20012

1) PCB Data	2
2) Signature Page	4
3) Case Narrative	5
4) Qualifier Page	7
5) Conformance/Non Conformance	8
6) QA Checklist	10
7) Chronicle	11
8) Hit Summary	12
9) QC Data Summary For PCB	13
9.1) Deuterated Monitoring Compound Summary	14
9.2) MS/MSD Summary	16
9.3) LCS/LCSD Summary	18
9.4) Method Blank Summary	19
10) Sample Data	20
10.1) OU4-TS-38-071725	21
10.2) OU4-TS-39-071725	28
10.3) OU4-TS-40-071725	32
10.4) OU4-TS-41-071725	36
10.5) OU4-TS-42-071725	40
10.6) OU4-TS-43-071725	44
10.7) OU4-TS-44-071725	48
11) Calibration Data Summary	52
11.1) Initial Calibration Data	53
11.1.1) PO070825	53
11.1.2) PP070825	272
11.2) Continued Calibration Data	491
11.2.1) PO112332.D	491
11.2.2) PO112346.D	503
11.2.3) PO112366.D	515
11.2.4) PO112381.D	527
11.2.5) PP073972.D	539
11.2.6) PP073987.D	551
11.2.7) PP073990.D	563
11.2.8) PP074002.D	573
11.2.9) PP074005.D	585

Table Of Contents for Q2639

11.3) Analytical Seq	595	1
12) Compound Detection Summary	599	2
13) QC Sample Data	603	3
13.1) Method Blank Data	604	4
13.2) PIBLK Data	608	5
13.3) LCS Data	644	6
13.4) MS Data	653	7
13.5) MSD Data	662	8
14) Manual Integration	671	9
15) Analytical Runlogs	686	10
16) Percent Solid	710	11
17) Extraction Logs	714	12
17.1) PB168927.pdf	714	13
17.2) PB168927IC.pdf	716	14
18) Standard Prep Logs	717	15
19) Shipping Document	803	16
19.1) Chain Of Custody	804	17
19.2) Lab Certificate	805	18
19.3) Internal COC	806	19
20) Not Reviewed Data	808	20

Cover Page

Order ID : Q2639

Project ID : Raymark Superfund Site

Client : Nobis Group

Lab Sample Number

Q2639-01
Q2639-02
Q2639-03
Q2639-04
Q2639-05
Q2639-06
Q2639-07
Q2639-08
Q2639-09
Q2639-10
Q2639-11
Q2639-12
Q2639-13
Q2639-14

Client Sample Number

OU4-TS-38-071725
OU4-TS-38-071725
OU4-TS-39-071725
OU4-TS-39-071725
OU4-TS-40-071725
OU4-TS-40-071725
OU4-TS-41-071725
OU4-TS-41-071725
OU4-TS-42-071725
OU4-TS-42-071725
OU4-TS-43-071725
OU4-TS-43-071725
OU4-TS-44-071725
OU4-TS-44-071725

I certify that the data package is in compliance with the terms and conditions of the contract, both technically and for completeness, for other than the conditions detailed above. Release of the data contained in this hard copy data package has been authorized by the laboratory manager or his designee, as verified by the following signature.

Signature :

APPROVED

By Sohil Jodhani, QA/QC Director at 10:40 am, Aug 01, 2025

Date: 7/28/2025

NYDOH CERTIFICATION NO - 11376

NJDEP CERTIFICATION NO - 20012

CASE NARRATIVE

Nobis Group

Project Name: Raymark Superfund Site

Project # N/A

Order ID # Q2639

Test Name: PCB

A. Number of Samples and Date of Receipt:

14 Solid samples were received on 07/18/2025.

B. Parameters

According to the Chain of Custody document, the following analyses were requested: Cyanide, Herbicide Group1, Mercury, Metals Group6, Metals ICP-TAL, METALS-TAL, PCB, Pesticide-TCL, SPLP Extraction, SPLP Mercury, SPLP MetalGroup3, SVOCMS Group3 and VOCMS Group3. This data package contains results for PCB.

C. Analytical Techniques:

The analyses were performed on instrument GCECD_P. The front column is ZB-MR1 which is 30 meters, 0.32 mm ID, 0.5 um df, Catalogue # 7HM-G016-17. The rear column is ZB-MR2 which is 30 meters, 0.32 mm ID, 0.25 µm; Catalogue # 7HM-G017-11. The analyses were performed on instrument GCECD_O. The front column is ZB-MR1 which is 30 meters, 0.32 mm ID, 0.5 um df, Catalogue # 7HM-G016-17. The rear column is ZB-MR2 which is 30 meters, 0.32 mm ID, 0.25 µm; Catalogue # 7HM-G017-11. The analysis of PCBs was based on method 8082A and extraction was done based on method 3541.

D. QA/ QC Samples:

The Holding Times were met for all analysis.

The Surrogate recoveries met the acceptable criteria except for OU4-TS-38-071725 [Decachlorobiphenyl(1)56%], as per method one surrogate is allowed to failed, therefore no corrective action was taken.

The Retention Times were acceptable for all samples.

The MS recoveries met the requirements for all compounds.

The MSD recoveries met the requirements for all compounds.

The RPD met criteria. The RPD were met for all analysis.

The Blank Spike met requirements for all compounds.

The Blank analysis did not indicate the presence of lab contamination.

The Initial Calibration met the requirements.



284 Sheffield Street, Mountainside, NJ 07092
Phone: 908 789 8900 Fax: 908 789 8922

The Continuous Calibration File ID PP073987.D met the requirements except for Decachlorobiphenyl is failing in 2nd column but passing in 1st column therefore no corrective action taken.

The Continuous Calibration File ID PP074002.D met the requirements except for Aroclor-1260(Peak-02) is failing in 1st column but passing in 2nd column therefore no corrective action taken.

E. Additional Comments:

The not QT review data is reported in the Miscellaneous.

The soil samples results are based on a dry weight basis.

F. Manual Integration Comments:

Please refer to the Manual integration Report included with the Run Logs for information on the manual integrations performed.

I certify that the data package is in compliance with the terms and conditions of the contract, both technically and for completeness, for other than the conditions detailed above. The laboratory manager or his designee, as verified by the following signature has authorized release of the data contained in this hard copy data package.

Signature

APPROVED

By Sohil Jodhani, QA/QC Director at 10:40 am, Aug 01, 2025

DATA REPORTING QUALIFIERS- ORGANIC

For reporting results, the following "Results Qualifiers" are used:

- Value** If the result is a value greater than or equal to the detection limit, report the value
- U** Indicates the compound was analyzed for but was not detected. Report the minimum detection limit for the sample with the U, i.e. "10 U". This is not necessarily the instrument detection limit attainable for this particular sample based on any concentration or dilution that may have been required.
- ND** Indicates the analyte was analyzed for, but not detected
- J** Indicates an estimated value. This flag is used:
(1) When estimating a concentration for a tentatively identified compound (library search hits, where a 1:1 response is assumed.)
(2) When the mass spectral data indicated the identification, however the result was less than the specified detection limit greater than zero. If the detection limit was 10ug/L and a concentration of 3 ug/L was calculated report as 3 J. This flag is used when similar situation arise on any organic parameter i.e. Pest, PCB and others.
- B** Indicates the analyte was found in the blank as well as the sample report as "12 B".
- E** Indicates the analyte 's concentration exceeds the calibrated range of the instrument for that specific analysis.
- D** This flag identifies all compounds identified in an analysis at a secondary dilution factor.
- P** This flag is used for Pesticide/PCB target analyte when there is >25% difference for detected concentrations between the two GC columns. The lower of the two values is reported on Form 1 and flagged with a "P".
- N** This flag indicates presumptive evidence of a compound. This is only used for tentatively identified compounds (TICs), where the identification is based on a mass spectral library search. It applies to all TIC results. For generic characterization of a TIC, such as chlorinated hydrocarbon, the flag is not used.
- A** This flag indicates that a Tentatively Identified Compound is a suspected aldol-condensation product.
- Q** Indicates the LCS did not meet the control limits requirements



284 Sheffield Street, Mountainside, NJ 07092 Phone: 908 789 8900 Fax: 908 789 8922

GC ANALYSIS CONFORMANCE/NON-CONFORMANCE SUMMARY

ORDER ID: Q2639

MATRIX: Solid

METHOD: 8082A/3541

		NA	NO	YES
1.	Chromatograms Labeled/Compounds Identified.			✓
2.	Standard Summary Submitted.			✓
3.	Calibration - Initial Calibration performed within 30 days before sample analysis and continuing calibration performed within 24 hours of sample analysis, 12 HOURS IF 8000 SERIES METHOD.			✓

The Initial Calibration met the requirements.

The Continuous Calibration File ID PP073987.D met the requirements except for Decachlorobiphenyl is failing in 2nd column but passing in 1st column therefore no corrective action taken.

The Continuous Calibration File ID PP074002.D met the requirements except for Aroclor-1260(Peak-02) is failing in 1st column but passing in 2nd column therefore no corrective action taken.

4.	Blank Contamination - If yes, list compounds and concentrations in each blank:	✓
----	--	---

5.	Surrogate Recoveries Meet Criteria	✓
----	------------------------------------	---

If not met, list those compounds and their recoveries which fall outside the acceptable ranges.

The Surrogate recoveries met the acceptable criteria except for OU4-TS-38-071725 [Decachlorobiphenyl(1)56%], as per method one surrogate is allowed to failed, therefore no corrective action was taken.

6.	Matrix Spike/Matrix Spike Duplicate Recoveries Meet Criteria	✓
----	--	---

If not met, list those compounds and their recoveries which fall outside the acceptable range.

The MS recoveries met the requirements for all compounds.

The MSD recoveries met the requirements for all compounds.

The Blank Spike met requirements for all compounds.

The RPD met criteria.The RPD were met for all analysis.

7.	Retention Time Shift Meet Criteria (if applicable)	✓
----	--	---

Comments:



284 Sheffield Street, Mountainside, NJ 07092 Phone: 908 789 8900 Fax: 908 789 8922

GC ANALYSIS CONFORMANCE/NON-CONFORMANCE SUMMARY (CONTINUED)

		NA	NO	YES
8.	Extraction Holding Time Met			✓
	If not met, list number of days exceeded for each sample:			
9.	Analysis Holding Time Met			✓
	If not met, list those compounds and their recoveries which fall outside the acceptable range.			

ADDITIONAL COMMENTS:

The not QT review data is reported in the Miscellaneous.

The soil samples results are based on a dry weight basis.

APPROVED

By Sohil Jodhani, QA/QC Director at 10:40 am, Aug 01, 2025

QA REVIEW

1
2
3
4
5
6
7
8
9
10
11
12
13
14
15
16
17
18
19
20

APPENDIX A

QA REVIEW GENERAL DOCUMENTATION

Project #: Q2639

Completed

For thorough review, the report must have the following:

GENERAL:

Are all original paperwork present (chain of custody, record of communication, airbill, sample management lab chronicle, login page)

✓

Check chain-of-custody for proper relinquish/return of samples

✓

Is the chain of custody signed and complete

✓

Check internal chain-of-custody for proper relinquish/return of samples /sample extracts

✓

Collect information for each project id from server. Were all requirements followed

✓

COVER PAGE:

Do numbers of samples correspond to the number of samples in the Chain of Custody on login page

✓

Do lab numbers and client Ids on cover page agree with the Chain of Custody

✓

CHAIN OF CUSTODY:

Do requested analyses on Chain of Custody agree with form I results

✓

Do requested analyses on Chain of Custody agree with the log-in page

✓

Were the correct method log-in for analysis according to the Analytical Request and Chain of Castody

✓

Were the samples received within hold time

✓

Were any problems found with the samples at arrival recorded in the Sample Management Laboratory Chronicle

✓

ANALYTICAL:

Was method requirement followed?

✓

Was client requirement followed?

✓

Does the case narrative summarize all QC failure?

✓

All runlogs and manual integration are reviewed for requirements

✓

All manual calculations and /or hand notations verified

✓

QA Review Signature: SOHIL JODHANI

Date: 07/28/2025

LAB CHRONICLE

OrderID:	Q2639	OrderDate:	7/18/2025 10:22:00 AM
Client:	Nobis Group	Project:	Raymark Superfund Site
Contact:	Adam Roy	Location:	O13,VOA Lab

LabID	ClientID	Matrix	Test	Method	Sample Date	Prep Date	Anal Date	Received
Q2639-01	OU4-TS-38-071725	SOIL			07/17/25			07/18/25
			PCB	8082A		07/21/25	07/21/25	
Q2639-03	OU4-TS-39-071725	SOIL			07/17/25			07/18/25
			PCB	8082A		07/21/25	07/21/25	
Q2639-05	OU4-TS-40-071725	SOIL			07/17/25			07/18/25
			PCB	8082A		07/21/25	07/21/25	
Q2639-07	OU4-TS-41-071725	SOIL			07/17/25			07/18/25
			PCB	8082A		07/21/25	07/21/25	
Q2639-09	OU4-TS-42-071725	SOIL			07/17/25			07/18/25
			PCB	8082A		07/21/25	07/22/25	
Q2639-11	OU4-TS-43-071725	SOIL			07/17/25			07/18/25
			PCB	8082A		07/21/25	07/22/25	
Q2639-13	OU4-TS-44-071725	SOIL			07/17/25			07/18/25
			PCB	8082A		07/21/25	07/22/25	

Hit Summary Sheet SW-846

SDG No.: Q2639

Order ID: Q2639

Client: Nobis Group

Project ID: Raymark Superfund Site

Sample ID	Client ID	Matrix	Parameter	Concentration	C	MDL	LOD	RDL	Units
Q2639-01	OU4-TS-38-071725	SOIL	Aroclor-1254	25.5	4.00	10.3	21.1	ug/kg	
Total Concentration:									25.500



QC SUMMARY

Surrogate Summary

SDG No.: Q2639

Client: Nobis Group

Analytical Method: 8082A

Lab Sample ID	Client ID	Parameter	Column	Spike	Result	Recovery(%)	Qual	Limits(%)	
								Low	High
I.BLK-PO112087.D	PIBLK-PO112087.D	Tetrachloro-m-xyl	1	20	19.4	97		60	140
		Decachlorobiphen	1	20	18.8	94		60	140
		Tetrachloro-m-xyl	2	20	20.0	100		60	140
		Decachlorobiphen	2	20	19.3	97		60	140
I.BLK-PO112336.D	PIBLK-PO112336.D	Tetrachloro-m-xyl	1	20	22.3	112		60	140
		Decachlorobiphen	1	20	18.4	92		60	140
		Tetrachloro-m-xyl	2	20	20.7	104		60	140
		Decachlorobiphen	2	20	17.7	88		60	140
Q2639-03	OU4-TS-39-071725	Tetrachloro-m-xyl	1	20	23.9	119		44	130
		Decachlorobiphen	1	20	14.1	71		60	125
		Tetrachloro-m-xyl	2	20	22.4	112		44	130
		Decachlorobiphen	2	20	14.2	71		60	125
Q2639-05	OU4-TS-40-071725	Tetrachloro-m-xyl	1	20	22.5	113		44	130
		Decachlorobiphen	1	20	12.9	65		60	125
		Tetrachloro-m-xyl	2	20	21.0	105		44	130
		Decachlorobiphen	2	20	13.0	65		60	125
Q2639-07	OU4-TS-41-071725	Tetrachloro-m-xyl	1	20	22.8	114		44	130
		Decachlorobiphen	1	20	12.3	62		60	125
		Tetrachloro-m-xyl	2	20	20.9	104		44	130
		Decachlorobiphen	2	20	12.3	61		60	125
I.BLK-PO112350.D	PIBLK-PO112350.D	Tetrachloro-m-xyl	1	20	20.1	101		60	140
		Decachlorobiphen	1	20	17.6	88		60	140
		Tetrachloro-m-xyl	2	20	19.0	95		60	140
		Decachlorobiphen	2	20	17.4	87		60	140
I.BLK-PO112370.D	PIBLK-PO112370.D	Tetrachloro-m-xyl	1	20	20.1	100		60	140
		Decachlorobiphen	1	20	17.7	89		60	140
		Tetrachloro-m-xyl	2	20	18.3	91		60	140
		Decachlorobiphen	2	20	17.4	87		60	140
Q2639-09	OU4-TS-42-071725	Tetrachloro-m-xyl	1	20	14.8	74		44	130
		Decachlorobiphen	1	20	20.2	101		60	125
		Tetrachloro-m-xyl	2	20	13.3	67		44	130
		Decachlorobiphen	2	20	20.5	102		60	125
Q2639-11	OU4-TS-43-071725	Tetrachloro-m-xyl	1	20	16.1	80		44	130
		Decachlorobiphen	1	20	16.4	82		60	125
		Tetrachloro-m-xyl	2	20	14.7	73		44	130
		Decachlorobiphen	2	20	17.2	86		60	125
Q2639-13	OU4-TS-44-071725	Tetrachloro-m-xyl	1	20	19.6	98		44	130
		Decachlorobiphen	1	20	18.0	90		60	125
		Tetrachloro-m-xyl	2	20	17.9	89		44	130
		Decachlorobiphen	2	20	18.0	90		60	125
I.BLK-PO112385.D	PIBLK-PO112385.D	Tetrachloro-m-xyl	1	20	19.8	99		60	140

Surrogate Summary

SDG No.: Q2639

Client: Nobis Group

Analytical Method: 8082A

Lab Sample ID	Client ID	Parameter	Column	Spike	Result	Recovery(%)	Qual	Limits(%)	
								Low	High
I.BLK-PO112385.D	PIBLK-PO112385.D	Decachlorobiphen	1	20	17.6	88		60	140
		Tetrachloro-m-xyl	2	20	18.1	90		60	140
I.BLK-PP073553.D	PIBLK-PP073553.D	Decachlorobiphen	2	20	17.4	87		60	140
		Tetrachloro-m-xyl	1	20	16.2	81		60	140
I.BLK-PP073976.D	PIBLK-PP073976.D	Decachlorobiphen	1	20	17.3	87		60	140
		Tetrachloro-m-xyl	2	20	16.2	81		60	140
I.BLK-PP073976.D	PIBLK-PP073976.D	Decachlorobiphen	2	20	17.1	85		60	140
		Tetrachloro-m-xyl	1	20	16.8	84		60	140
Q2635-01MS	RT2286MS	Decachlorobiphen	1	20	17.6	88		60	140
		Tetrachloro-m-xyl	1	20	16.9	84		60	140
Q2635-01MSD	RT2286MSD	Decachlorobiphen	2	20	19.1	96		60	140
		Tetrachloro-m-xyl	1	20	16.8	84		44	130
PB168927BL	PB168927BL	Decachlorobiphen	1	20	18.0	90		60	125
		Tetrachloro-m-xyl	2	20	17.9	89		44	130
PB168927BS	PB168927BS	Decachlorobiphen	2	20	19.9	99		60	125
		Tetrachloro-m-xyl	1	20	16.8	84		44	130
Q2639-01	OU4-TS-38-071725	Decachlorobiphen	1	20	17.8	89		60	125
		Tetrachloro-m-xyl	2	20	17.9	89		44	130
I.BLK-PP074006.D	PIBLK-PP074006.D	Decachlorobiphen	2	20	19.4	97		60	125
		Tetrachloro-m-xyl	1	20	15.8	79		60	140
PB168927BL	PB168927BL	Decachlorobiphen	1	20	16.7	83		60	140
		Tetrachloro-m-xyl	2	20	17.5	87		60	140
PB168927BS	PB168927BS	Decachlorobiphen	2	20	19.7	98		60	140
		Tetrachloro-m-xyl	1	20	17.3	87		44	130
Q2639-01	OU4-TS-38-071725	Decachlorobiphen	1	20	18.7	94		60	125
		Tetrachloro-m-xyl	2	20	18.9	94		44	130
Q2639-01	OU4-TS-38-071725	Decachlorobiphen	2	20	21.9	109		60	125
		Tetrachloro-m-xyl	1	20	18.8	94		44	130
PB168927BS	PB168927BS	Decachlorobiphen	1	20	20.5	103		60	125
		Tetrachloro-m-xyl	2	20	19.3	96		44	130
Q2639-01	OU4-TS-38-071725	Decachlorobiphen	2	20	23.9	120		60	125
		Tetrachloro-m-xyl	1	20	15.3	77		44	130
I.BLK-PP074006.D	PIBLK-PP074006.D	Decachlorobiphen	1	20	11.3	56	*	60	125
		Tetrachloro-m-xyl	2	20	16.3	82		44	130
PB168927BL	PB168927BL	Decachlorobiphen	2	20	12.7	64		60	125
		Tetrachloro-m-xyl	1	20	15.8	79		60	140
PB168927BS	PB168927BS	Decachlorobiphen	1	20	17.1	85		60	140
		Tetrachloro-m-xyl	2	20	17.4	87		60	140
Q2639-01	OU4-TS-38-071725	Decachlorobiphen	2	20	19.3	97		60	140

Matrix Spike/Matrix Spike Duplicate Summary

SW-846

SDG No.: Q2639

Analytical Method: 8082A

Client: Nobis Group

DataFile : PP073984.D

	Parameter	Spike	Sample Result	Result	Units	Rec	Rec Qual	RPD	RPD Qual	Limits Low	Limits High	RPD
Lab Sample ID:	Q2635-01MS (Column 1)		Client Sample ID:	RT2286MS								
	AR1016	196.2	0	177	ug/kg	90				47	134	
	AR1260	196.2	66.9	214	ug/kg	75				53	140	
Lab Sample ID:	Q2635-01MS (Column 2)		Client Sample ID:	RT2286MS								
	AR1016	196.2	0	174	ug/kg	89				47	134	
	AR1260	196.2	67.6	212	ug/kg	108				53	140	

Matrix Spike/Matrix Spike Duplicate Summary

SW-846

SDG No.: Q2639

Analytical Method: 8082A

Client: Nobis Group

DataFile : PP073985.D

	Parameter	Spike	Sample Result	Result	Units	Rec	Rec Qual	RPD	RPD Qual	Limits Low	Limits High	RPD
Lab Sample ID:	Q2635-01MSD (Column 1)		Client Sample ID:	RT2286MSD								
	AR1016	196.4	0	177	ug/kg	90		0		47	134	20
	AR1260	196.4	66.9	210	ug/kg	73		3		53	140	20
Lab Sample ID:	Q2635-01MSD (Column 2)		Client Sample ID:	RT2286MSD								
	AR1016	196.4	0	174	ug/kg	89		0		47	134	20
	AR1260	196.4	67.6	211	ug/kg	107		1		53	140	20

Laboratory Control Sample/Laboratory Control Sample Duplicate Summary

SW-846

SDG No.: Q2639

Analytical Method: 8082A

Client: Nobis Group

Datafile : PP073993.D

Lab Sample ID	Parameter	Spike	Result	Units	Rec	RPD	RPD		Limits		
							Qual	Qual	Low	High	
PB168927BS (Column 1)	AR1016	166.6	139	ug/kg	83				47	134	
	AR1260	166.6	135	ug/kg	81				53	140	
PB168927BS (Column 2)	AR1016	166.6	153	ug/kg	92				47	134	
	AR1260	166.6	154	ug/kg	92				53	140	

4C

PESTICIDE METHOD BLANK SUMMARY

Client ID

PB168927BL

Lab Name: Alliance

Contract: NOBI03

Lab Code: ACE

SDG NO.: Q2639

Lab Sample ID: PB168927BL

Lab File ID: PP073992.D

Matrix: (soil/water) Solid

Extraction: (Type) SOXH

Sulfur Cleanup: (Y/N) N

Date Extracted: 07/21/2025

Date Analyzed (1): 07/21/2025

Date Analyzed (2): 07/21/2025

Time Analyzed (1): 16:39

Time Analyzed (2): 16:39

Instrument ID (1): ECD_P

Instrument ID (2): ECD_P

GC Column (1): ZB-MR1

ID: 0.32 (mm)

GC Column (2): ZB-MR2

ID: 0.32 (mm)

THIS METHOD BLANK APPLIES TO THE FOLLOWING SAMPLES, MS AND MSD:

EPA SAMPLE NO.	LAB SAMPLE ID	LAB FILE ID	DATE ANALYZED 1	DATE ANALYZED 2
OU4-TS-39-071725	Q2639-03	PO112338.D	07/21/2025	07/21/2025
OU4-TS-40-071725	Q2639-05	PO112339.D	07/21/2025	07/21/2025
OU4-TS-41-071725	Q2639-07	PO112340.D	07/21/2025	07/21/2025
OU4-TS-42-071725	Q2639-09	PO112372.D	07/22/2025	07/22/2025
OU4-TS-43-071725	Q2639-11	PO112373.D	07/22/2025	07/22/2025
OU4-TS-44-071725	Q2639-13	PO112374.D	07/22/2025	07/22/2025
RT2286MS	Q2635-01MS	PP073984.D	07/21/2025	07/21/2025
RT2286MSD	Q2635-01MSD	PP073985.D	07/21/2025	07/21/2025
PB168927BS	PB168927BS	PP073993.D	07/21/2025	07/21/2025
OU4-TS-38-071725	Q2639-01	PP074001.D	07/21/2025	07/21/2025

COMMENTS:



SAMPLE

DATA



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

Report of Analysis

Client:	Nobis Group			Date Collected:	07/17/25	
Project:	Raymark Superfund Site			Date Received:	07/18/25	
Client Sample ID:	OU4-TS-38-071725			SDG No.:	Q2639	
Lab Sample ID:	Q2639-01			Matrix:	SOIL	
Analytical Method:	8082A			% Solid:	80.6	Decanted:
Sample Wt/Vol:	30.01	Units:	g	Final Vol:	10000	uL
Soil Aliquot Vol:	uL			Test:	PCB	
Extraction Type:				Injection Volume :		
GPC Factor :	1.0	PH :				
Prep Method :	SW3541B					

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PP074001.D	1	07/21/25 08:30	07/21/25 19:07	PB168927

CAS Number	Parameter	Conc.	Qualifier	MDL	LOD	LOQ / CRQL	Units(Dry Weight)
TARGETS							
12674-11-2	Aroclor-1016	10.3	U	4.90	10.3	21.1	ug/kg
11104-28-2	Aroclor-1221	16.1	U	5.00	16.1	21.1	ug/kg
11141-16-5	Aroclor-1232	10.3	U	4.60	10.3	21.1	ug/kg
53469-21-9	Aroclor-1242	10.3	U	5.00	10.3	21.1	ug/kg
12672-29-6	Aroclor-1248	16.1	U	7.30	16.1	21.1	ug/kg
11097-69-1	Aroclor-1254	25.5		4.00	10.3	21.1	ug/kg
37324-23-5	Aroclor-1262	16.1	U	6.20	16.1	21.1	ug/kg
11100-14-4	Aroclor-1268	10.3	U	4.50	10.3	21.1	ug/kg
11096-82-5	Aroclor-1260	10.3	U	4.00	10.3	21.1	ug/kg
SURROGATES							
877-09-8	Tetrachloro-m-xylene	16.3		44 - 130		82%	SPK: 20
2051-24-3	Decachlorobiphenyl	12.7		60 - 125		64%	SPK: 20

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP072125\
 Data File : PP074001.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jul 2025 19:07
 Operator : YP\AJ
 Sample : Q2639-01
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
OU4-TS-38-071725

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/22/2025
 Supervised By :mohammad ahmed 07/23/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 22 02:15:21 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 08 08:35:32 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	4.482	3.773	20953277	30094893	15.300	16.336
2) SA Decachlor...	10.165	8.770	12316627	16836055	11.289	12.724

Target Compounds

26) L6 AR-1254-1	6.479	5.650	1962683	4190209	36.624m	36.113m
27) L6 AR-1254-2	6.699	5.798	3279552	2267112	39.376m	22.531m#
28) L6 AR-1254-3	7.065	6.214	5707528	11616997	64.615m	75.217m
29) L6 AR-1254-4	7.339	6.427	971267	1124015	12.347m	11.887m
30) L6 AR-1254-5	7.776	6.840	11486495	20407242	155.897	152.926

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP072125\
 Data File : PP074001.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jul 2025 19:07
 Operator : YP\AJ
 Sample : Q2639-01
 Misc :
 ALS Vial : 26 Sample Multiplier: 1



Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 22 02:15:21 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 08 08:35:32 2025
 Response via : Initial Calibration
 Integrator: ChemStation


Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Instrument :
 ECD_P
 ClientSampleId :
 OU4-TS-38-071725

Manual Integrations APPROVED

Reviewed By :Yogesh Patel 07/22/2025
 Supervised By :mohammad ahmed 07/23/2025

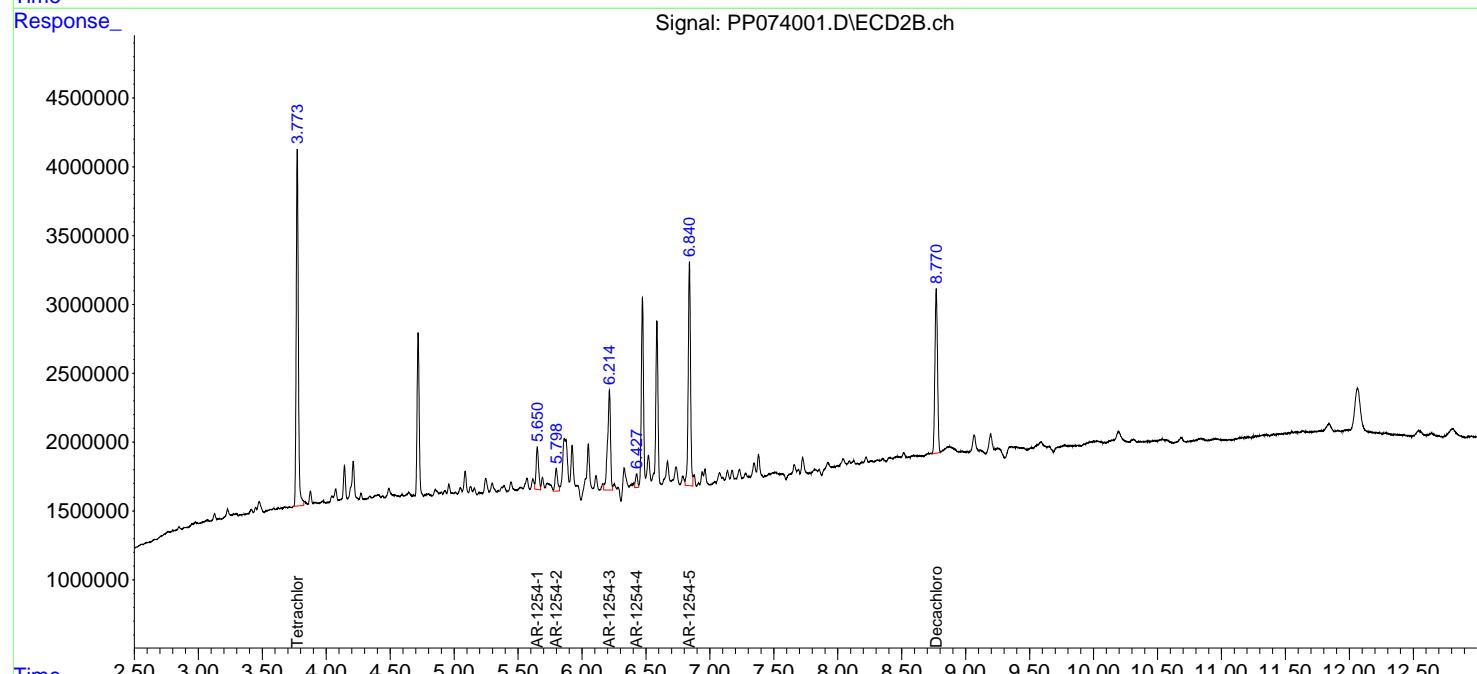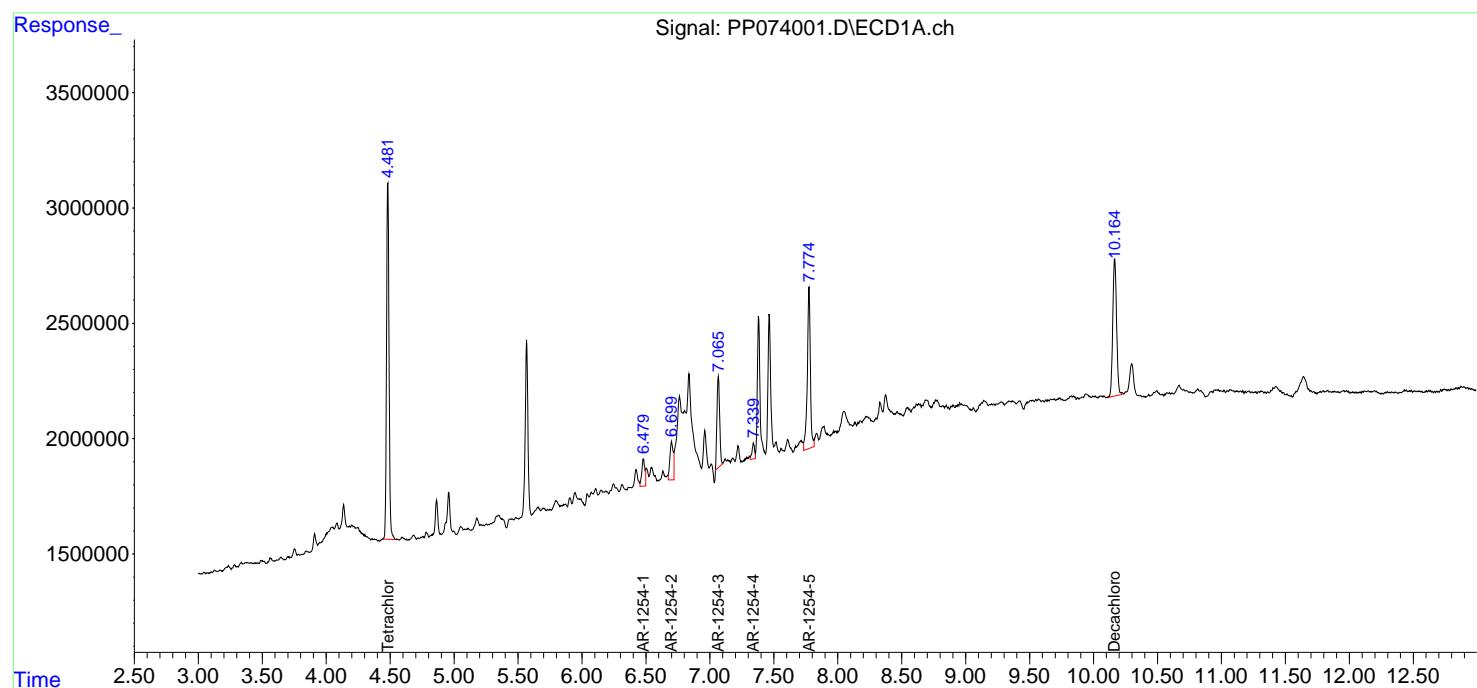

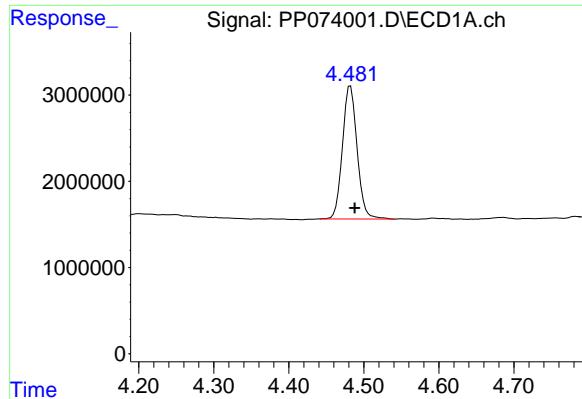


#1 Tetrachloro-m-xylene

R.T.: 4.482 min
Delta R.T.: -0.006 min
Response: 20953277
Conc: 15.30 ng/ml

Instrument: ECD_P
ClientSampleId: OU4-TS-38-071725


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/22/2025
Supervised By :mohammad ahmed 07/23/2025

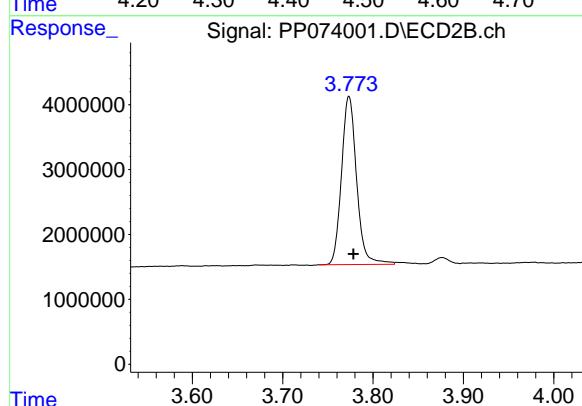


#1 Tetrachloro-m-xylene

R.T.: 3.773 min
Delta R.T.: -0.005 min
Response: 30094893
Conc: 16.34 ng/ml

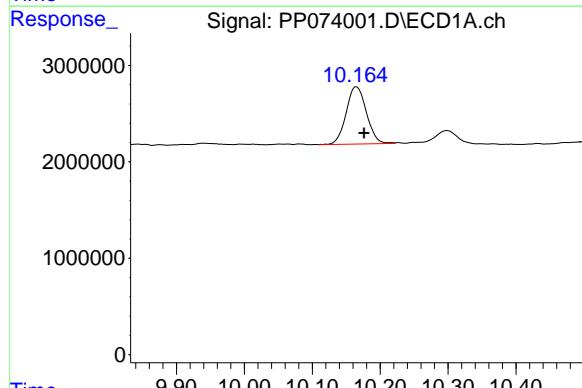


#2 Decachlorobiphenyl

R.T.: 10.165 min
Delta R.T.: -0.011 min
Response: 12316627
Conc: 11.29 ng/ml

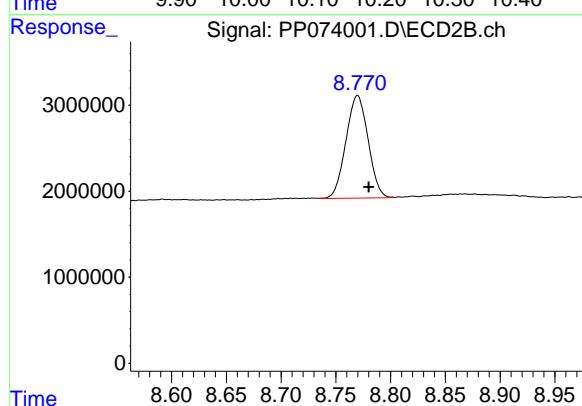

#2 Decachlorobiphenyl

R.T.: 8.770 min
Delta R.T.: -0.010 min
Response: 16836055
Conc: 12.72 ng/ml

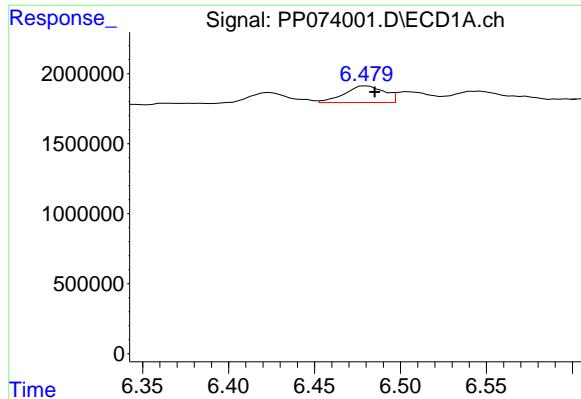


#26 AR-1254-1

R.T.: 6.479 min
 Delta R.T.: -0.006 min
 Response: 1962683
 Conc: 36.62 ng/ml

Instrument: ECD_P
 ClientSampleId: OU4-TS-38-071725


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/22/2025
 Supervised By :mohammad ahmed 07/23/2025

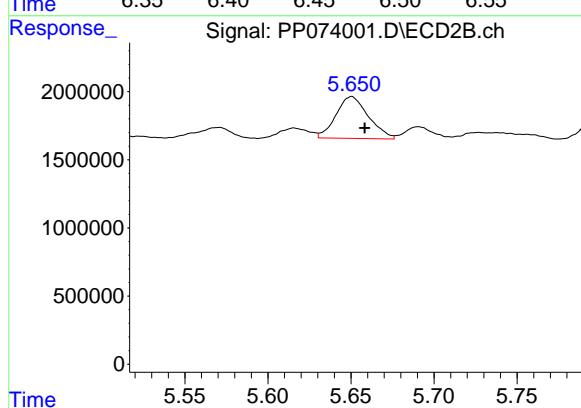


#26 AR-1254-1

R.T.: 5.650 min
 Delta R.T.: -0.008 min
 Response: 4190209
 Conc: 36.11 ng/ml




#27 AR-1254-2

R.T.: 6.699 min
 Delta R.T.: -0.002 min
 Response: 3279552
 Conc: 39.38 ng/ml

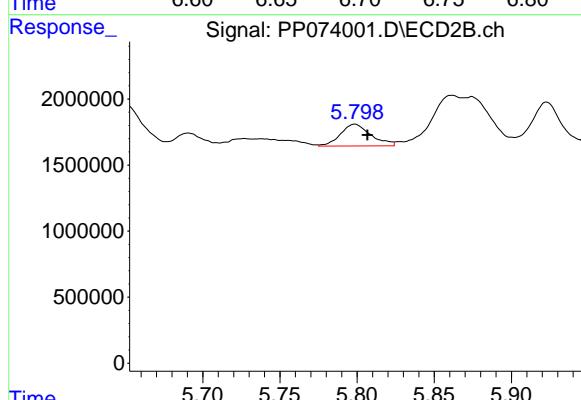

#27 AR-1254-2

R.T.: 5.798 min
 Delta R.T.: -0.008 min
 Response: 2267112
 Conc: 22.53 ng/ml

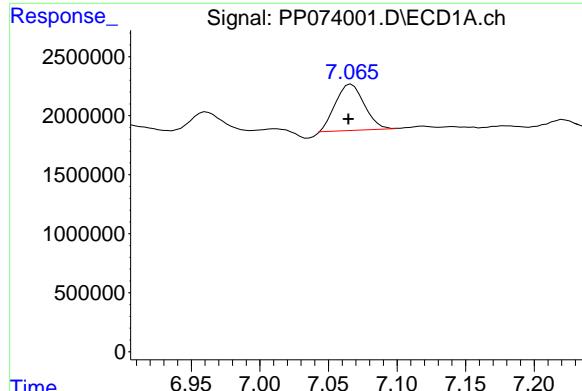


#28 AR-1254-3

R.T.: 7.065 min
 Delta R.T.: 0.000 min
 Response: 5707528
 Conc: 64.61 ng/ml

Instrument: ECD_P
 ClientSampleId: OU4-TS-38-071725


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/22/2025
 Supervised By :mohammad ahmed 07/23/2025

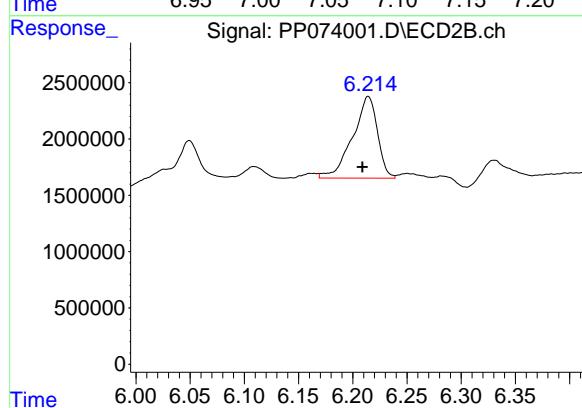


#28 AR-1254-3

R.T.: 6.214 min
 Delta R.T.: 0.005 min
 Response: 11616997
 Conc: 75.22 ng/ml

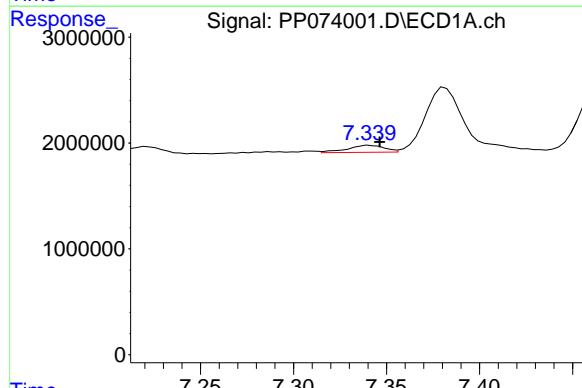


#29 AR-1254-4

R.T.: 7.339 min
 Delta R.T.: -0.007 min
 Response: 971267
 Conc: 12.35 ng/ml

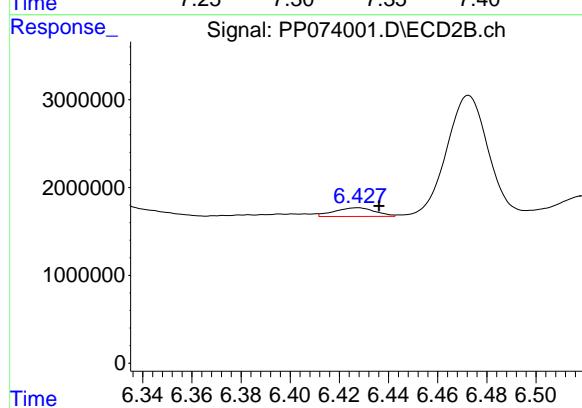

#29 AR-1254-4

R.T.: 6.427 min
 Delta R.T.: -0.009 min
 Response: 1124015
 Conc: 11.89 ng/ml

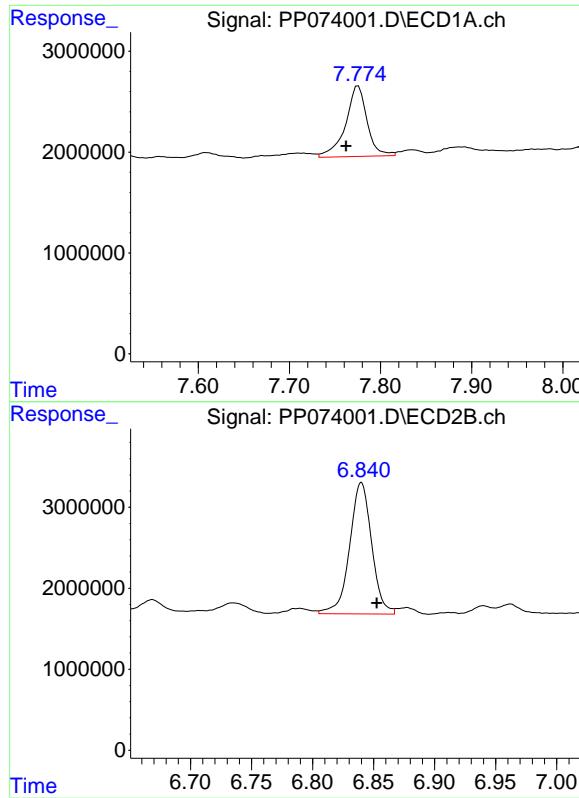

#30 AR-1254-5

R.T.: 7.776 min
 Delta R.T.: 0.013 min
 Response: 11486495
 Conc: 155.90 ng/ml

Instrument: ECD_P
 ClientSampleId: OU4-TS-38-071725

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/22/2025
 Supervised By :mohammad ahmed 07/23/2025

#30 AR-1254-5

R.T.: 6.840 min
 Delta R.T.: -0.013 min
 Response: 20407242
 Conc: 152.93 ng/ml

1
2
3
4
5
6
7
8
9
10
11
12
13
14
15
16
17
18
19
20



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

Report of Analysis

Client:	Nobis Group			Date Collected:	07/17/25	
Project:	Raymark Superfund Site			Date Received:	07/18/25	
Client Sample ID:	OU4-TS-39-071725			SDG No.:	Q2639	
Lab Sample ID:	Q2639-03			Matrix:	SOIL	
Analytical Method:	8082A			% Solid:	81	Decanted:
Sample Wt/Vol:	30.04	Units:	g	Final Vol:	10000	uL
Soil Aliquot Vol:	uL			Test:	PCB	
Extraction Type:				Injection Volume :		
GPC Factor :	1.0	PH :				
Prep Method :	SW3541B					

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PO112338.D	1	07/21/25 08:30	07/21/25 13:11	PB168927

CAS Number	Parameter	Conc.	Qualifier	MDL	LOD	LOQ / CRQL	Units(Dry Weight)
TARGETS							
12674-11-2	Aroclor-1016	10.2	U	4.90	10.2	21.0	ug/kg
11104-28-2	Aroclor-1221	16.0	U	5.00	16.0	21.0	ug/kg
11141-16-5	Aroclor-1232	10.2	U	4.60	10.2	21.0	ug/kg
53469-21-9	Aroclor-1242	10.2	U	4.90	10.2	21.0	ug/kg
12672-29-6	Aroclor-1248	16.0	U	7.30	16.0	21.0	ug/kg
11097-69-1	Aroclor-1254	10.2	U	4.00	10.2	21.0	ug/kg
37324-23-5	Aroclor-1262	16.0	U	6.20	16.0	21.0	ug/kg
11100-14-4	Aroclor-1268	10.2	U	4.40	10.2	21.0	ug/kg
11096-82-5	Aroclor-1260	10.2	U	4.00	10.2	21.0	ug/kg
SURROGATES							
877-09-8	Tetrachloro-m-xylene	23.9		44 - 130		119%	SPK: 20
2051-24-3	Decachlorobiphenyl	14.2		60 - 125		71%	SPK: 20

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0072125\
 Data File : P0112338.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jul 2025 13:11
 Operator : YP/AJ
 Sample : Q2639-03
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
OU4-TS-39-071725

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 22 01:48:29 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Jul 21 10:54:00 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	3.671	3.663	236.3E6	142.9E6	23.881	22.424
2) SA Decachlor...	8.699	8.645	96643378	24379843	14.135	14.146

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0072125\
 Data File : P0112338.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jul 2025 13:11
 Operator : YP/AJ
 Sample : Q2639-03
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 OU4-TS-39-071725

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 22 01:48:29 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Jul 21 10:54:00 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

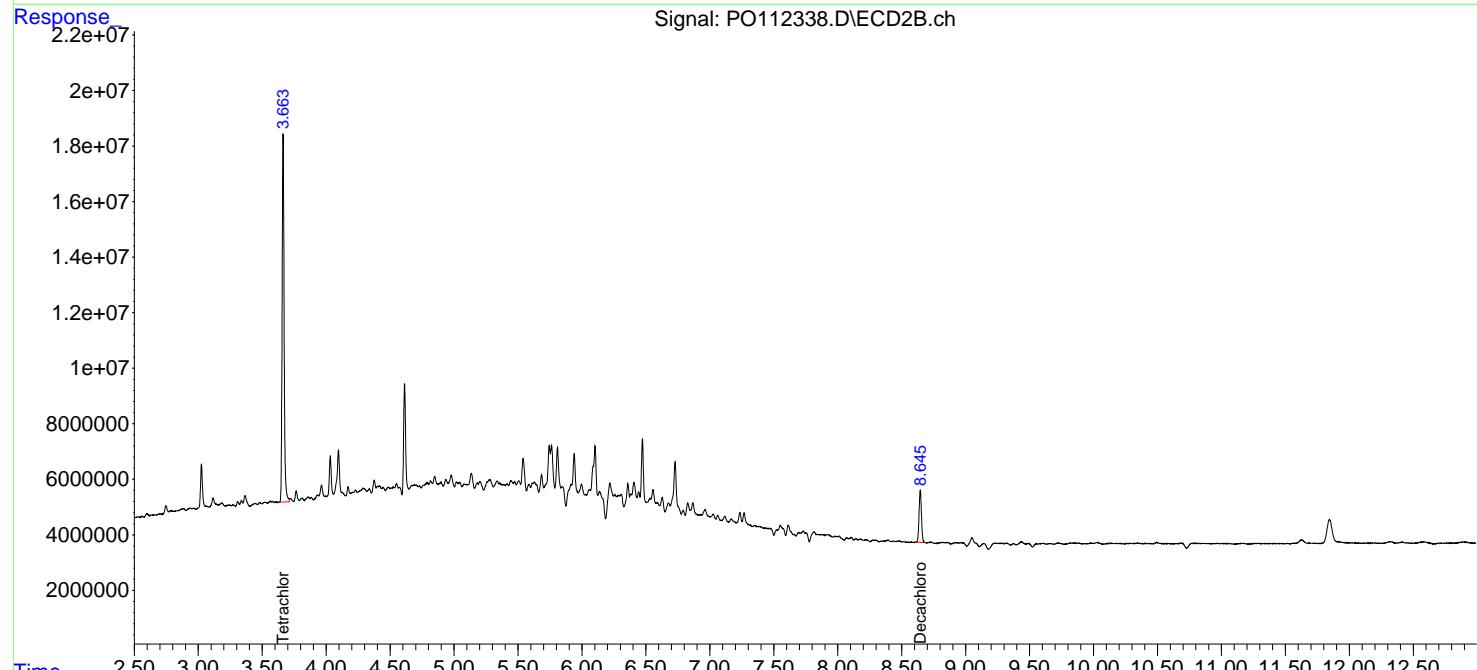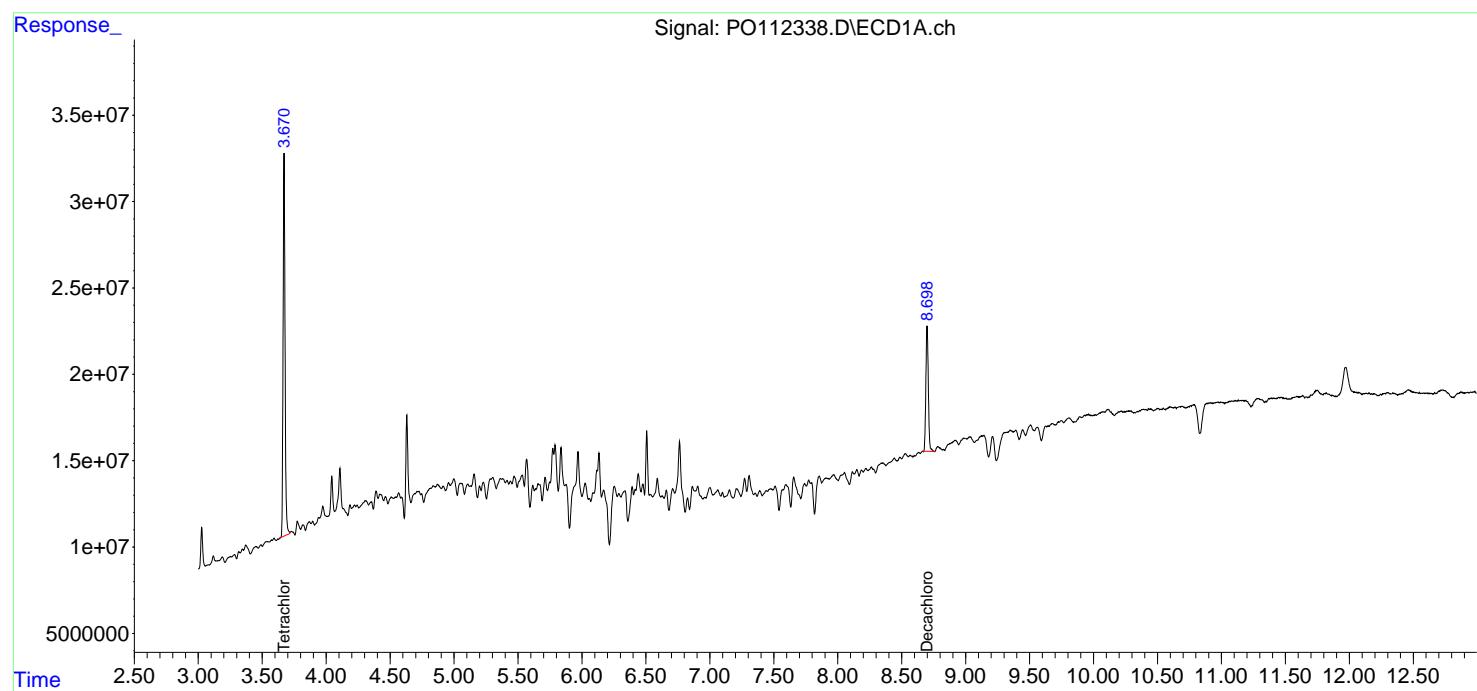

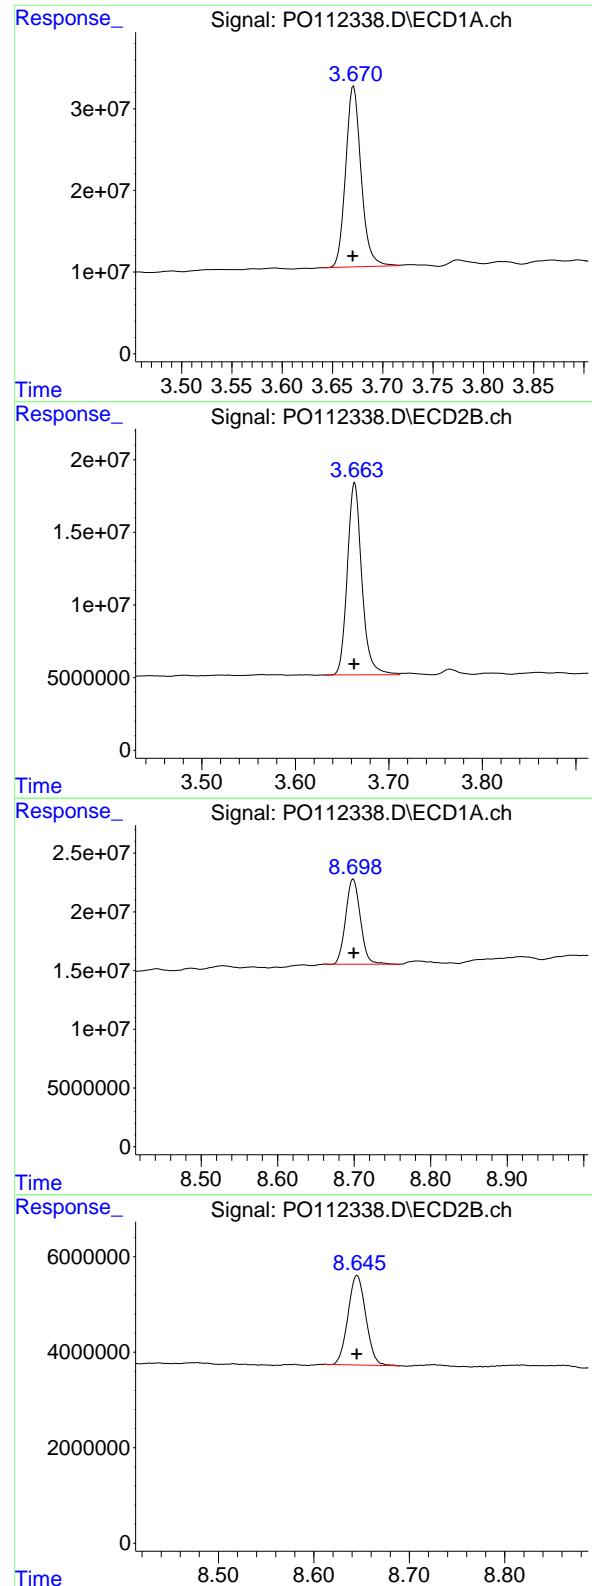

#1 Tetrachloro-m-xylene

R.T.: 3.671 min
Delta R.T.: 0.001 min
Response: 236291176
Conc: 23.88 ng/ml

Instrument:

ECD_O

ClientSampleId :

OU4-TS-39-071725

#1 Tetrachloro-m-xylene

R.T.: 3.663 min
Delta R.T.: 0.000 min
Response: 142866978
Conc: 22.42 ng/ml

#2 Decachlorobiphenyl

R.T.: 8.699 min
Delta R.T.: 0.000 min
Response: 96643378
Conc: 14.14 ng/ml

#2 Decachlorobiphenyl

R.T.: 8.645 min
Delta R.T.: 0.000 min
Response: 24379843
Conc: 14.15 ng/ml



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

Report of Analysis

Client:	Nobis Group			Date Collected:	07/17/25	
Project:	Raymark Superfund Site			Date Received:	07/18/25	
Client Sample ID:	OU4-TS-40-071725			SDG No.:	Q2639	
Lab Sample ID:	Q2639-05			Matrix:	SOIL	
Analytical Method:	8082A			% Solid:	80.7	Decanted:
Sample Wt/Vol:	30.06	Units:	g	Final Vol:	10000	uL
Soil Aliquot Vol:	uL			Test:	PCB	
Extraction Type:				Injection Volume :		
GPC Factor :	1.0	PH :				
Prep Method :	SW3541B					

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PO112339.D	1	07/21/25 08:30	07/21/25 13:30	PB168927

CAS Number	Parameter	Conc.	Qualifier	MDL	LOD	LOQ / CRQL	Units(Dry Weight)
TARGETS							
12674-11-2	Aroclor-1016	10.3	U	4.90	10.3	21.0	ug/kg
11104-28-2	Aroclor-1221	16.1	U	5.00	16.1	21.0	ug/kg
11141-16-5	Aroclor-1232	10.3	U	4.60	10.3	21.0	ug/kg
53469-21-9	Aroclor-1242	10.3	U	5.00	10.3	21.0	ug/kg
12672-29-6	Aroclor-1248	16.1	U	7.30	16.1	21.0	ug/kg
11097-69-1	Aroclor-1254	10.3	U	4.00	10.3	21.0	ug/kg
37324-23-5	Aroclor-1262	16.1	U	6.20	16.1	21.0	ug/kg
11100-14-4	Aroclor-1268	10.3	U	4.50	10.3	21.0	ug/kg
11096-82-5	Aroclor-1260	10.3	U	4.00	10.3	21.0	ug/kg
SURROGATES							
877-09-8	Tetrachloro-m-xylene	22.5		44 - 130		113%	SPK: 20
2051-24-3	Decachlorobiphenyl	13.0		60 - 125		65%	SPK: 20

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0072125\
 Data File : P0112339.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jul 2025 13:30
 Operator : YP/AJ
 Sample : Q2639-05
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
OU4-TS-40-071725

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 22 01:49:04 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Jul 21 10:54:00 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	3.671	3.663	222.7E6	133.8E6	22.511	21.004
2) SA Decachlor...	8.699	8.646	88214168	22382448	12.902	12.987

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0072125\
 Data File : P0112339.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jul 2025 13:30
 Operator : YP/AJ
 Sample : Q2639-05
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 OU4-TS-40-071725

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 22 01:49:04 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Jul 21 10:54:00 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

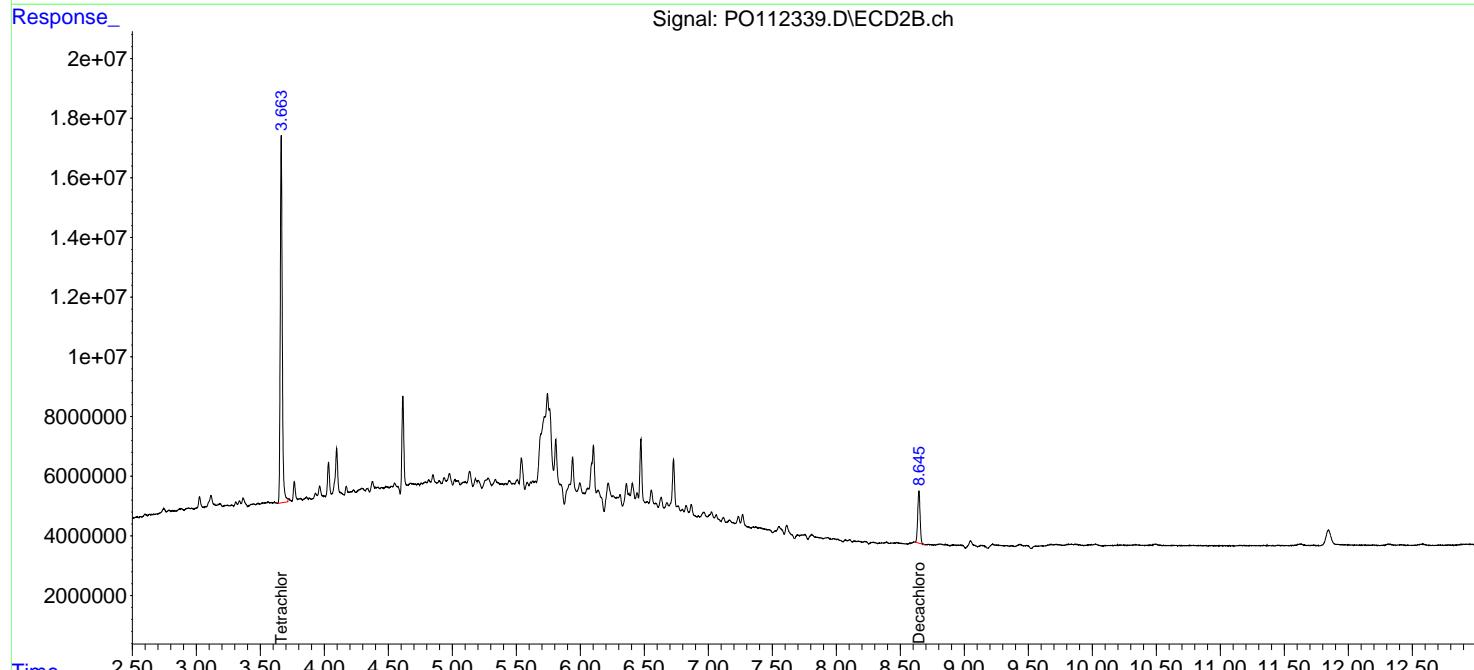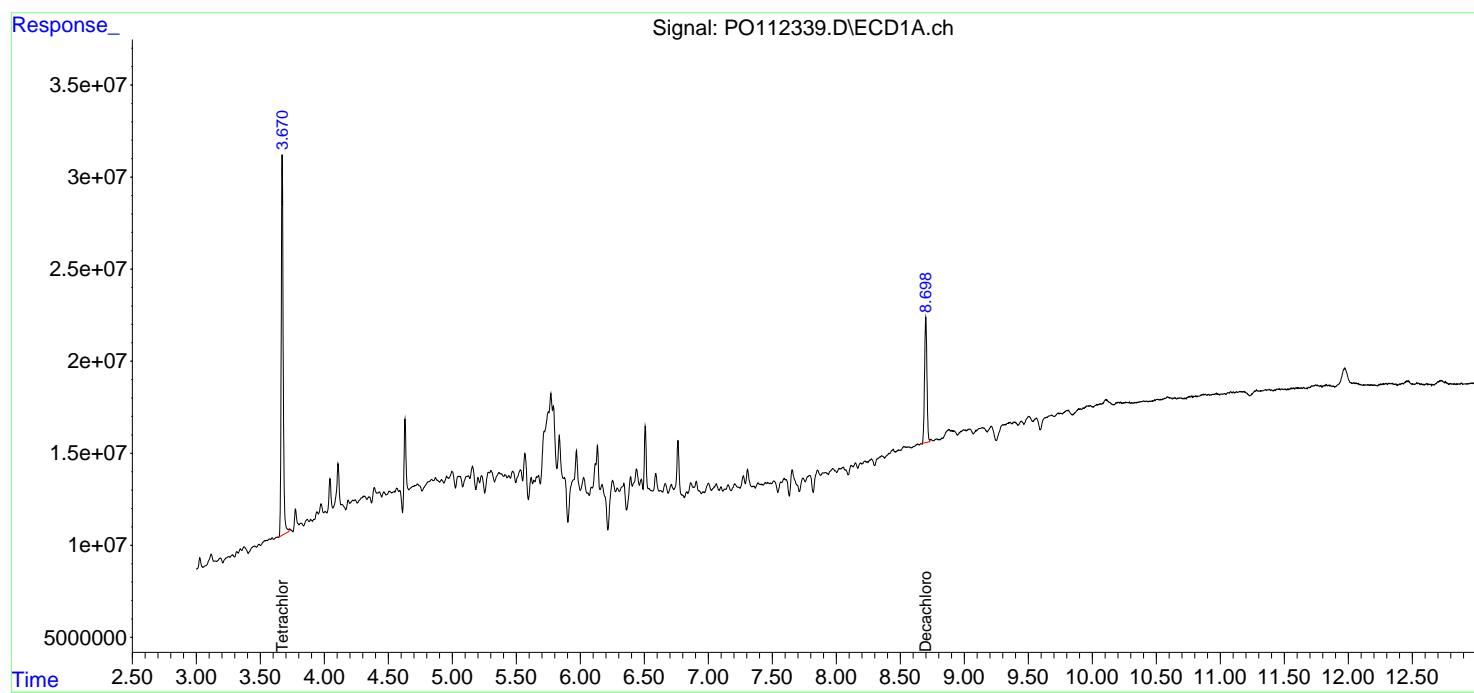

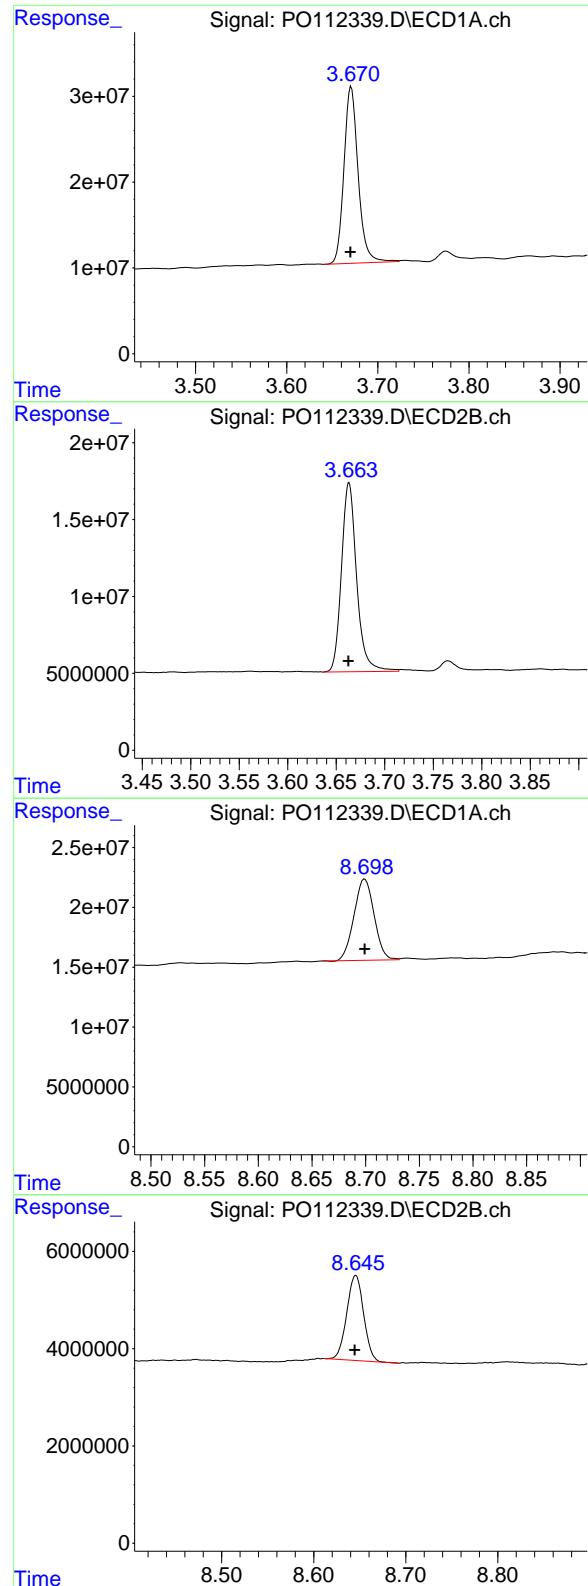

#1 Tetrachloro-m-xylene

R.T.: 3.671 min
Delta R.T.: 0.000 min
Response: 222742747
Conc: 22.51 ng/ml

Instrument:

ECD_O

ClientSampleId :

OU4-TS-40-071725

#1 Tetrachloro-m-xylene

R.T.: 3.663 min
Delta R.T.: 0.000 min
Response: 133819292
Conc: 21.00 ng/ml

#2 Decachlorobiphenyl

R.T.: 8.699 min
Delta R.T.: 0.000 min
Response: 88214168
Conc: 12.90 ng/ml

#2 Decachlorobiphenyl

R.T.: 8.646 min
Delta R.T.: 0.000 min
Response: 22382448
Conc: 12.99 ng/ml



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

Report of Analysis

Client:	Nobis Group			Date Collected:	07/17/25	
Project:	Raymark Superfund Site			Date Received:	07/18/25	
Client Sample ID:	OU4-TS-41-071725			SDG No.:	Q2639	
Lab Sample ID:	Q2639-07			Matrix:	SOIL	
Analytical Method:	8082A			% Solid:	82	Decanted:
Sample Wt/Vol:	30.09	Units:	g	Final Vol:	10000	uL
Soil Aliquot Vol:	uL			Test:	PCB	
Extraction Type:				Injection Volume :		
GPC Factor :	1.0	PH :				
Prep Method :	SW3541B					

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PO112340.D	1	07/21/25 08:30	07/21/25 13:47	PB168927

CAS Number	Parameter	Conc.	Qualifier	MDL	LOD	LOQ / CRQL	Units(Dry Weight)
TARGETS							
12674-11-2	Aroclor-1016	10.1	U	4.80	10.1	20.7	ug/kg
11104-28-2	Aroclor-1221	15.8	U	4.90	15.8	20.7	ug/kg
11141-16-5	Aroclor-1232	10.1	U	4.50	10.1	20.7	ug/kg
53469-21-9	Aroclor-1242	10.1	U	4.90	10.1	20.7	ug/kg
12672-29-6	Aroclor-1248	15.8	U	7.20	15.8	20.7	ug/kg
11097-69-1	Aroclor-1254	10.1	U	3.90	10.1	20.7	ug/kg
37324-23-5	Aroclor-1262	15.8	U	6.10	15.8	20.7	ug/kg
11100-14-4	Aroclor-1268	10.1	U	4.40	10.1	20.7	ug/kg
11096-82-5	Aroclor-1260	10.1	U	3.90	10.1	20.7	ug/kg
SURROGATES							
877-09-8	Tetrachloro-m-xylene	22.8		44 - 130		114%	SPK: 20
2051-24-3	Decachlorobiphenyl	12.3		60 - 125		62%	SPK: 20

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0072125\
 Data File : P0112340.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jul 2025 13:47
 Operator : YP/AJ
 Sample : Q2639-07
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
OU4-TS-41-071725

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 22 01:49:37 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Jul 21 10:54:00 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	3.669	3.663	225.3E6	132.9E6	22.770	20.854
2) SA Decachlor...	8.696	8.645	84361184	21108026	12.339	12.247

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0072125\
 Data File : P0112340.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jul 2025 13:47
 Operator : YP/AJ
 Sample : Q2639-07
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
OU4-TS-41-071725

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 22 01:49:37 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Jul 21 10:54:00 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

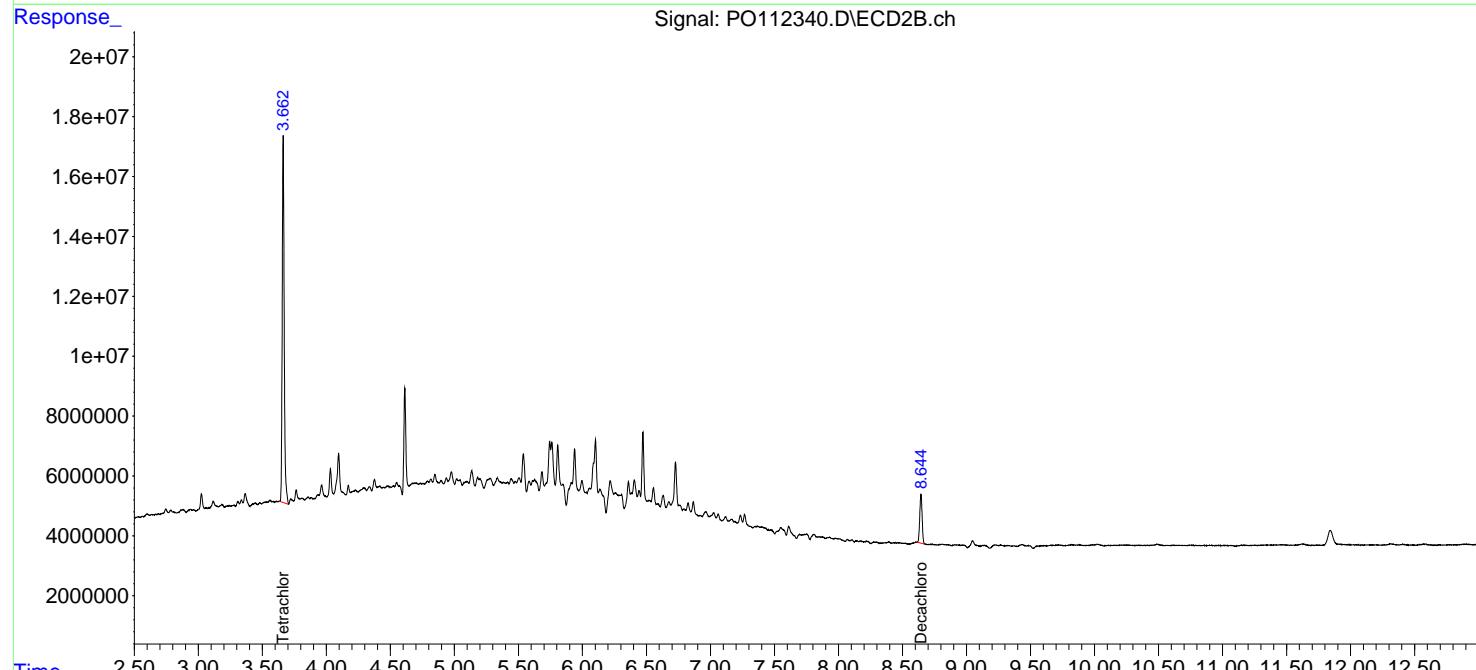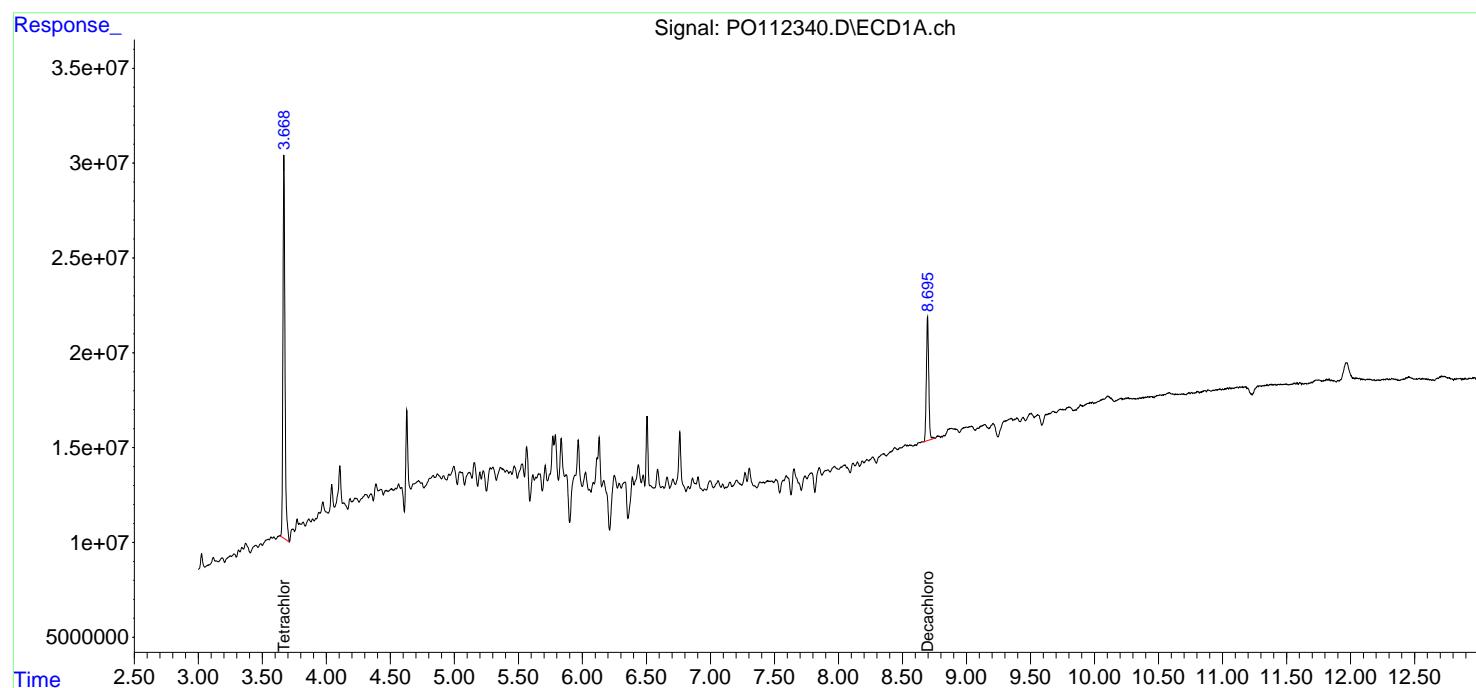

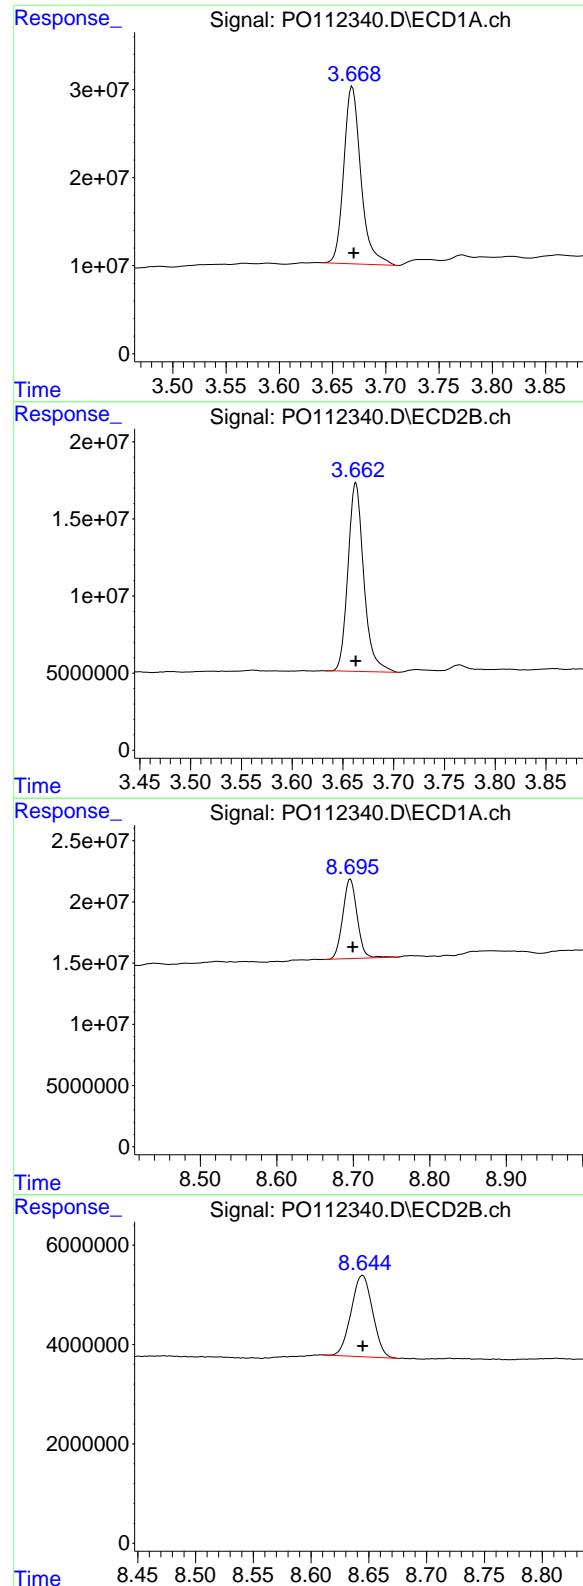

#1 Tetrachloro-m-xylene

R.T.: 3.669 min
Delta R.T.: -0.001 min
Response: 225300512
Conc: 22.77 ng/ml

Instrument: ECD_O
ClientSampleId: OU4-TS-41-071725

#1 Tetrachloro-m-xylene

R.T.: 3.663 min
Delta R.T.: 0.000 min
Response: 132860095
Conc: 20.85 ng/ml

#2 Decachlorobiphenyl

R.T.: 8.696 min
Delta R.T.: -0.003 min
Response: 84361184
Conc: 12.34 ng/ml

#2 Decachlorobiphenyl

R.T.: 8.645 min
Delta R.T.: 0.000 min
Response: 21108026
Conc: 12.25 ng/ml



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

Report of Analysis

Client:	Nobis Group			Date Collected:	07/17/25	
Project:	Raymark Superfund Site			Date Received:	07/18/25	
Client Sample ID:	OU4-TS-42-071725			SDG No.:	Q2639	
Lab Sample ID:	Q2639-09			Matrix:	SOIL	
Analytical Method:	8082A			% Solid:	60.3	Decanted:
Sample Wt/Vol:	30.05	Units:	g	Final Vol:	10000	uL
Soil Aliquot Vol:	uL			Test:	PCB	
Extraction Type:				Injection Volume :		
GPC Factor :	1.0	PH :				
Prep Method :	SW3541B					

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PO112372.D	1	07/21/25 08:30	07/22/25 11:08	PB168927

CAS Number	Parameter	Conc.	Qualifier	MDL	LOD	LOQ / CRQL	Units(Dry Weight)
TARGETS							
12674-11-2	Aroclor-1016	13.7	U	6.50	13.7	28.1	ug/kg
11104-28-2	Aroclor-1221	21.5	U	6.70	21.5	28.1	ug/kg
11141-16-5	Aroclor-1232	13.7	U	6.20	13.7	28.1	ug/kg
53469-21-9	Aroclor-1242	13.7	U	6.60	13.7	28.1	ug/kg
12672-29-6	Aroclor-1248	21.5	U	9.80	21.5	28.1	ug/kg
11097-69-1	Aroclor-1254	13.7	U	5.30	13.7	28.1	ug/kg
37324-23-5	Aroclor-1262	21.5	U	8.30	21.5	28.1	ug/kg
11100-14-4	Aroclor-1268	13.7	U	6.00	13.7	28.1	ug/kg
11096-82-5	Aroclor-1260	13.7	U	5.30	13.7	28.1	ug/kg
SURROGATES							
877-09-8	Tetrachloro-m-xylene	14.8		44 - 130		74%	SPK: 20
2051-24-3	Decachlorobiphenyl	20.5		60 - 125		102%	SPK: 20

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0072225\
 Data File : P0112372.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Jul 2025 11:08
 Operator : YP/AJ
 Sample : Q2639-09
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
OU4-TS-42-071725

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 23 01:47:37 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 22 09:14:26 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	3.674	3.662	146.2E6	85006290	14.772	13.343
2) SA Decachlor...	8.702	8.644	138.3E6	35259839	20.228	20.459

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.





Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0072225\
 Data File : P0112372.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Jul 2025 11:08
 Operator : YP/AJ
 Sample : Q2639-09
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 OU4-TS-42-071725

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 23 01:47:37 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 22 09:14:26 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ m Signal #2 Info : 30M x 0.32mm x 0.25 μ m

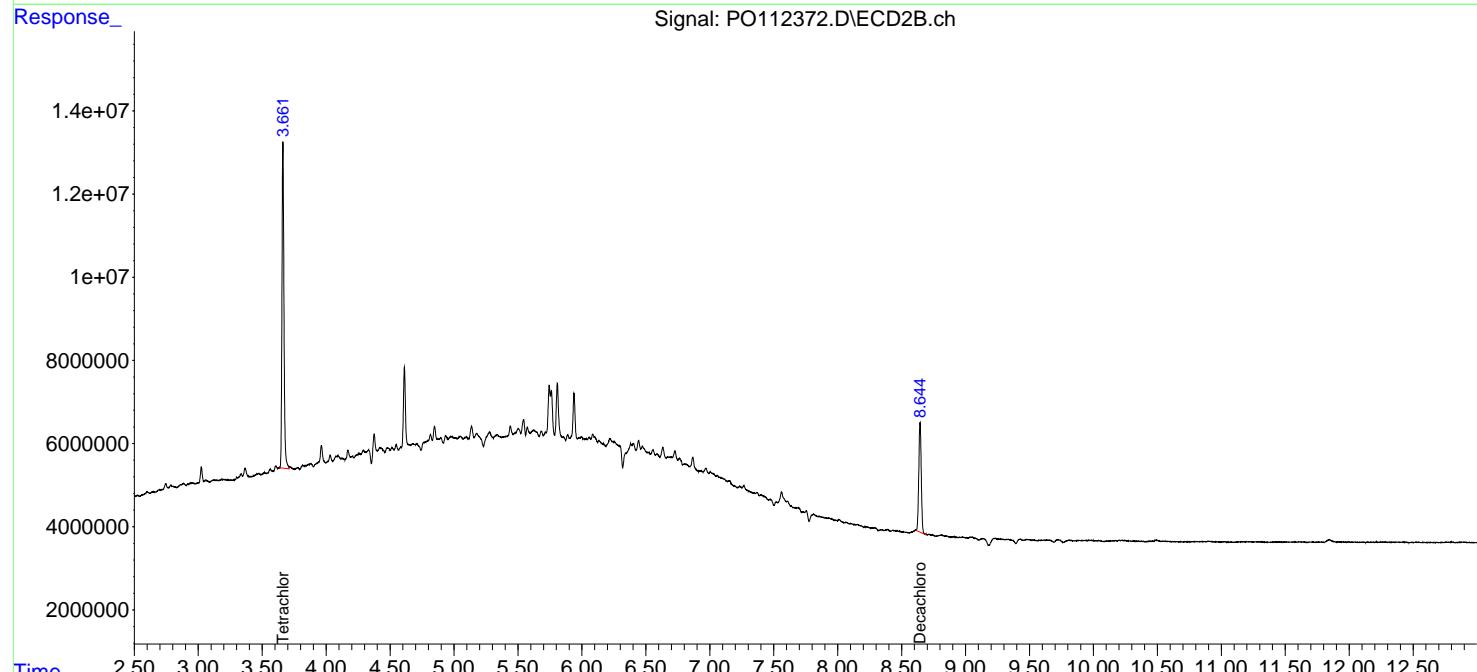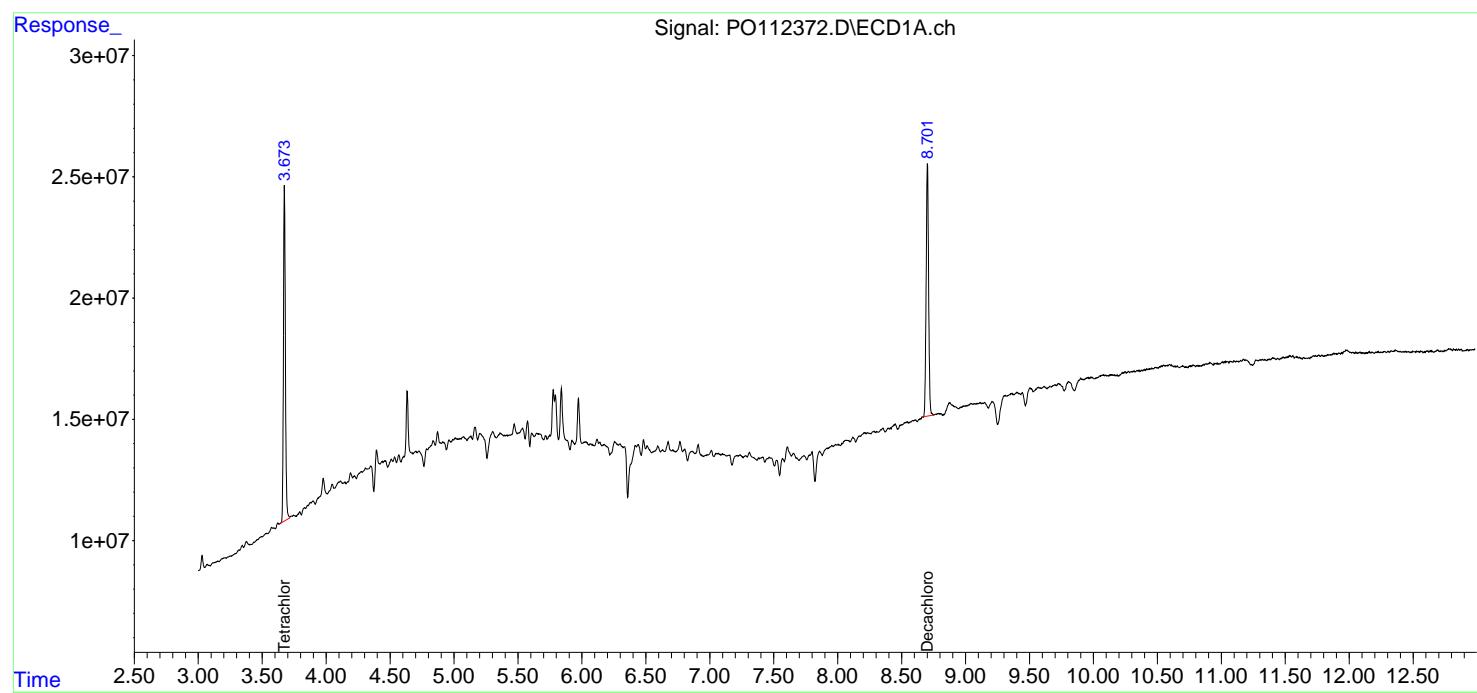

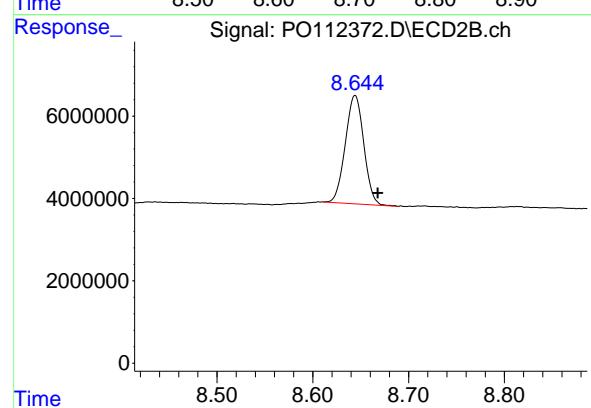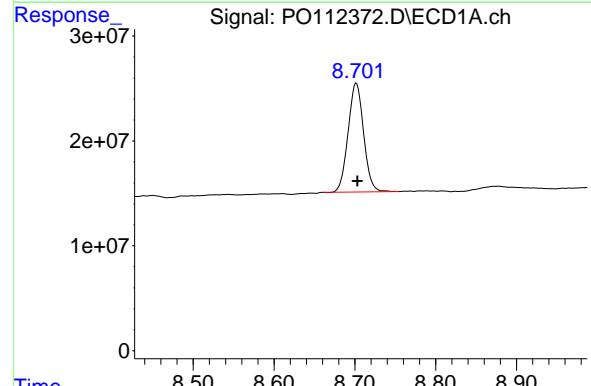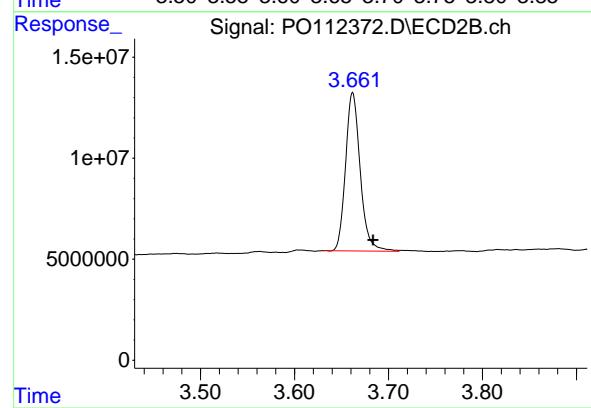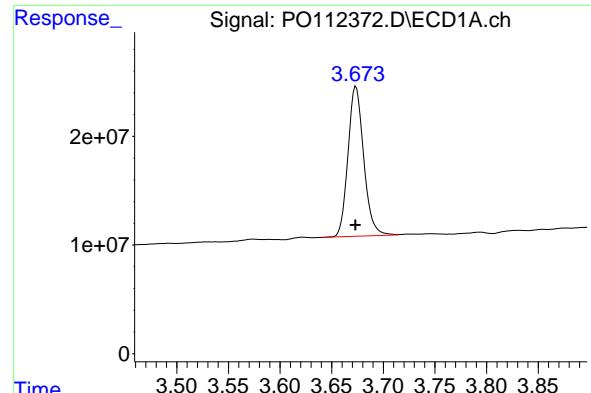

#1 Tetrachloro-m-xylene

R.T.: 3.674 min
 Delta R.T.: 0.000 min
 Response: 146161873
 Conc: 14.77 ng/ml

Instrument:

ECD_O

ClientSampleId :

OU4-TS-42-071725

#1 Tetrachloro-m-xylene

R.T.: 3.662 min
 Delta R.T.: -0.022 min
 Response: 85006290
 Conc: 13.34 ng/ml

#2 Decachlorobiphenyl

R.T.: 8.702 min
 Delta R.T.: -0.002 min
 Response: 138300931
 Conc: 20.23 ng/ml

#2 Decachlorobiphenyl

R.T.: 8.644 min
 Delta R.T.: -0.024 min
 Response: 35259839
 Conc: 20.46 ng/ml



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

Report of Analysis

Client:	Nobis Group			Date Collected:	07/17/25	
Project:	Raymark Superfund Site			Date Received:	07/18/25	
Client Sample ID:	OU4-TS-43-071725			SDG No.:	Q2639	
Lab Sample ID:	Q2639-11			Matrix:	SOIL	
Analytical Method:	8082A			% Solid:	58	Decanted:
Sample Wt/Vol:	30.06	Units:	g	Final Vol:	10000	uL
Soil Aliquot Vol:	uL			Test:	PCB	
Extraction Type:				Injection Volume :		
GPC Factor :	1.0	PH :				
Prep Method :	SW3541B					

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PO112373.D	1	07/21/25 08:30	07/22/25 11:26	PB168927

CAS Number	Parameter	Conc.	Qualifier	MDL	LOD	LOQ / CRQL	Units(Dry Weight)
TARGETS							
12674-11-2	Aroclor-1016	14.3	U	6.80	14.3	29.3	ug/kg
11104-28-2	Aroclor-1221	22.4	U	6.90	22.4	29.3	ug/kg
11141-16-5	Aroclor-1232	14.3	U	6.40	14.3	29.3	ug/kg
53469-21-9	Aroclor-1242	14.3	U	6.90	14.3	29.3	ug/kg
12672-29-6	Aroclor-1248	22.4	U	10.2	22.4	29.3	ug/kg
11097-69-1	Aroclor-1254	14.3	U	5.50	14.3	29.3	ug/kg
37324-23-5	Aroclor-1262	22.4	U	8.60	22.4	29.3	ug/kg
11100-14-4	Aroclor-1268	14.3	U	6.20	14.3	29.3	ug/kg
11096-82-5	Aroclor-1260	14.3	U	5.60	14.3	29.3	ug/kg
SURROGATES							
877-09-8	Tetrachloro-m-xylene	16.1		44 - 130		80%	SPK: 20
2051-24-3	Decachlorobiphenyl	17.2		60 - 125		86%	SPK: 20

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0072225\
 Data File : P0112373.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Jul 2025 11:26
 Operator : YP/AJ
 Sample : Q2639-11
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
OU4-TS-43-071725

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/23/2025
 Supervised By :mohammad ahmed 07/24/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 23 01:48:03 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 22 09:14:26 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	3.668	3.662	158.9E6	93373800	16.056	14.656
2) SA Decachlor...	8.695	8.640	112.4E6	29625890	16.441	17.190m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0072225\
 Data File : P0112373.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Jul 2025 11:26
 Operator : YP/AJ
 Sample : Q2639-11
 Misc :
 ALS Vial : 9 Sample Multiplier: 1



Instrument :
 ECD_O
 ClientSampleId :
 OU4-TS-43-071725


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/23/2025
 Supervised By :mohammad ahmed 07/24/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 23 01:48:03 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 22 09:14:26 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

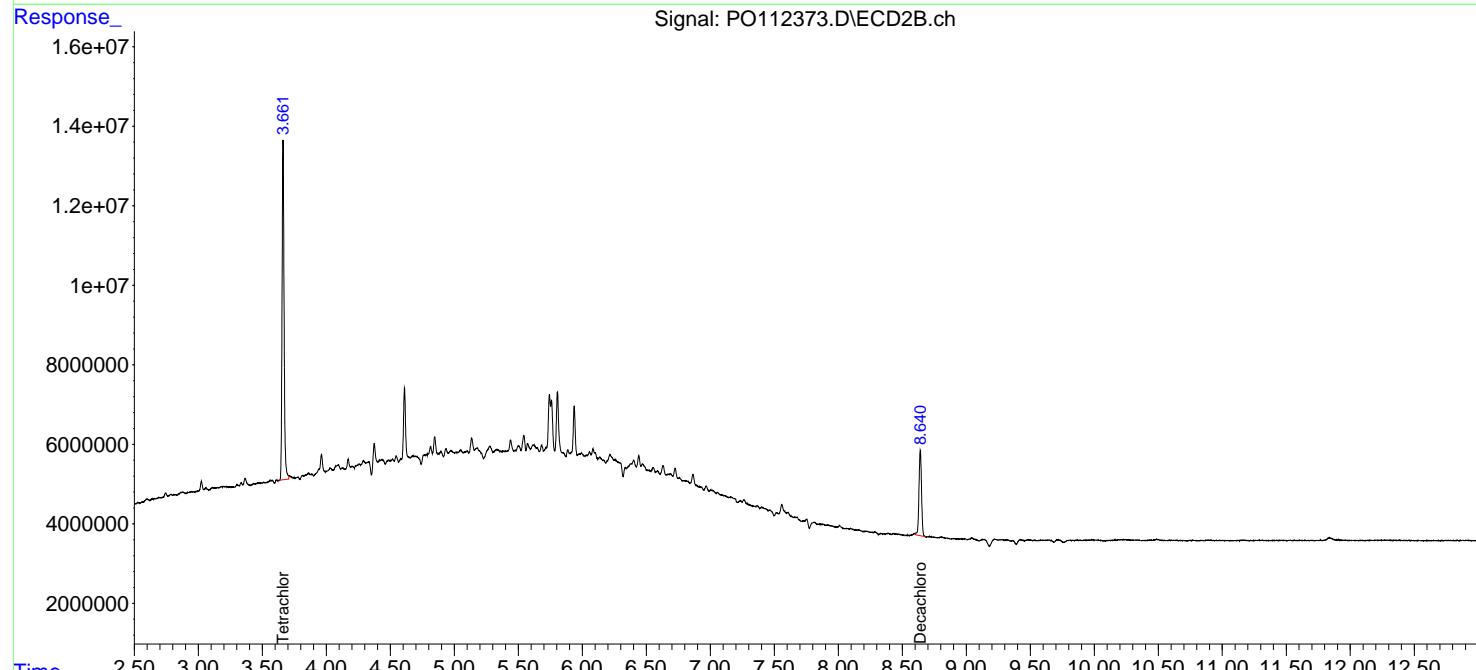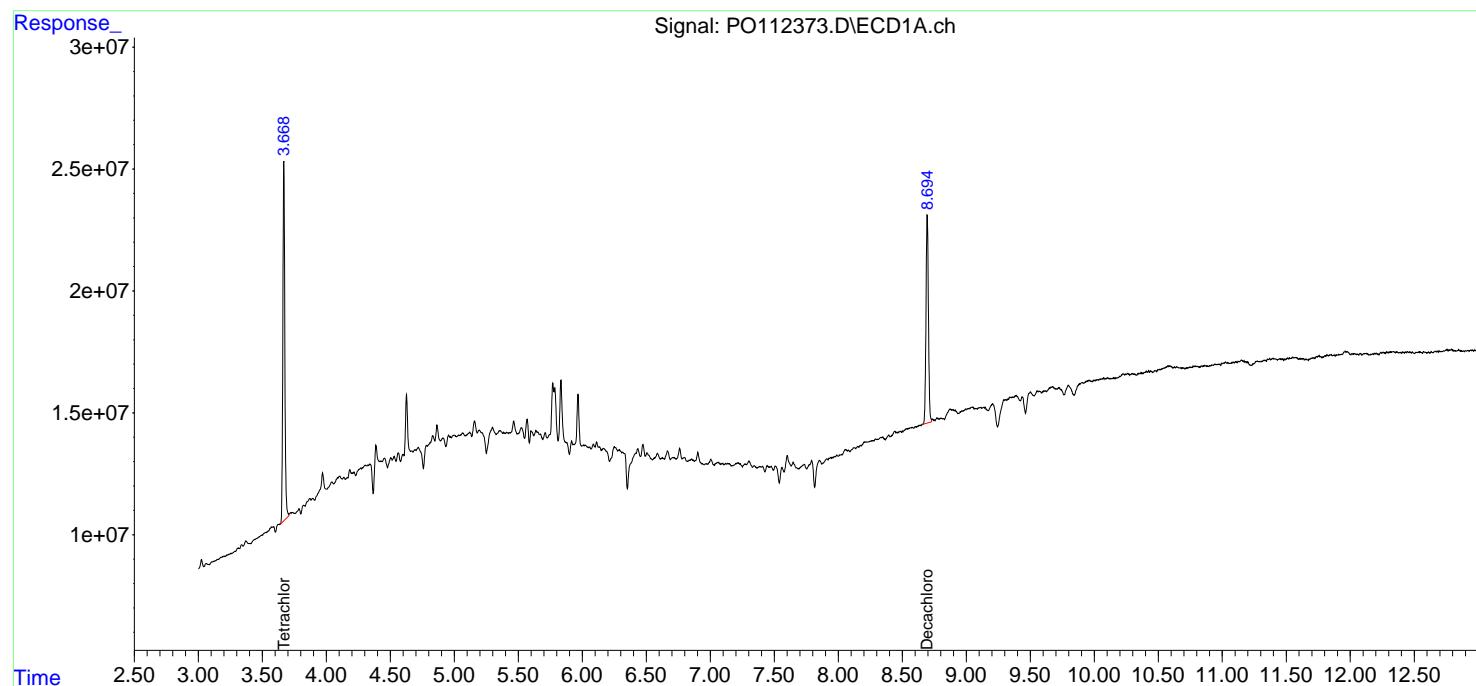

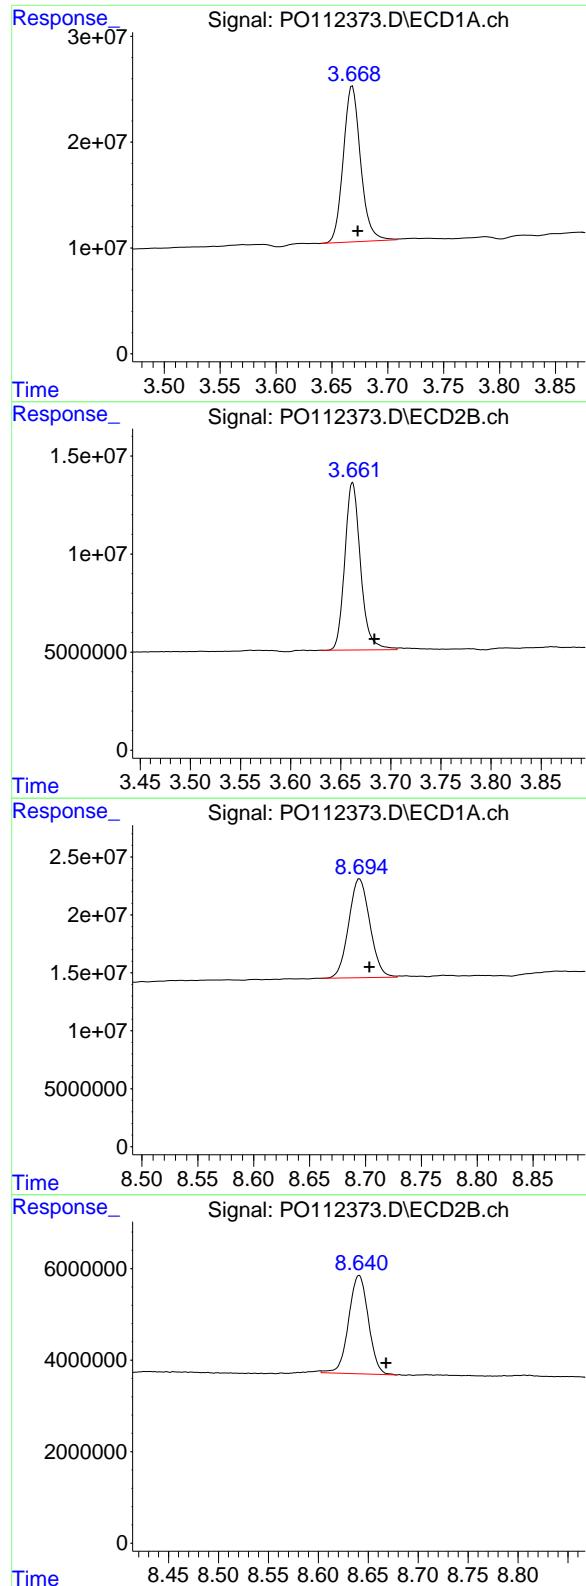

#1 Tetrachloro-m-xylene

R.T.: 3.668 min
 Delta R.T.: -0.005 min
 Response: 158871223
 Conc: 16.06 ng/ml

Instrument:
 ECD_O
 ClientSampleId :
 OU4-TS-43-071725

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/23/2025
 Supervised By :mohammad ahmed 07/24/2025

#1 Tetrachloro-m-xylene

R.T.: 3.662 min
 Delta R.T.: -0.022 min
 Response: 93373800
 Conc: 14.66 ng/ml

#2 Decachlorobiphenyl

R.T.: 8.695 min
 Delta R.T.: -0.009 min
 Response: 112410188
 Conc: 16.44 ng/ml

#2 Decachlorobiphenyl

R.T.: 8.640 min
 Delta R.T.: -0.027 min
 Response: 29625890
 Conc: 17.19 ng/ml



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

Report of Analysis

Client:	Nobis Group			Date Collected:	07/17/25	
Project:	Raymark Superfund Site			Date Received:	07/18/25	
Client Sample ID:	OU4-TS-44-071725			SDG No.:	Q2639	
Lab Sample ID:	Q2639-13			Matrix:	SOIL	
Analytical Method:	8082A			% Solid:	64.9	Decanted:
Sample Wt/Vol:	30.02	Units:	g	Final Vol:	10000	uL
Soil Aliquot Vol:	uL			Test:	PCB	
Extraction Type:				Injection Volume :		
GPC Factor :	1.0	PH :				
Prep Method :	SW3541B					

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PO112374.D	1	07/21/25 08:30	07/22/25 11:44	PB168927

CAS Number	Parameter	Conc.	Qualifier	MDL	LOD	LOQ / CRQL	Units(Dry Weight)
TARGETS							
12674-11-2	Aroclor-1016	12.8	U	6.10	12.8	26.2	ug/kg
11104-28-2	Aroclor-1221	20.0	U	6.20	20.0	26.2	ug/kg
11141-16-5	Aroclor-1232	12.8	U	5.70	12.8	26.2	ug/kg
53469-21-9	Aroclor-1242	12.8	U	6.20	12.8	26.2	ug/kg
12672-29-6	Aroclor-1248	20.0	U	9.10	20.0	26.2	ug/kg
11097-69-1	Aroclor-1254	12.8	U	4.90	12.8	26.2	ug/kg
37324-23-5	Aroclor-1262	20.0	U	7.70	20.0	26.2	ug/kg
11100-14-4	Aroclor-1268	12.8	U	5.50	12.8	26.2	ug/kg
11096-82-5	Aroclor-1260	12.8	U	5.00	12.8	26.2	ug/kg
SURROGATES							
877-09-8	Tetrachloro-m-xylene	19.6		44 - 130		98%	SPK: 20
2051-24-3	Decachlorobiphenyl	18.0		60 - 125		90%	SPK: 20

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0072225\
 Data File : P0112374.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Jul 2025 11:44
 Operator : YP/AJ
 Sample : Q2639-13
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
OU4-TS-44-071725

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 23 01:48:28 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 22 09:14:26 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	3.670	3.662	193.7E6	113.7E6	19.581	17.852
2) SA Decachlor...	8.697	8.641	123.2E6	31010440	18.013	17.993

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0072225\
 Data File : P0112374.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Jul 2025 11:44
 Operator : YP/AJ
 Sample : Q2639-13
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
OU4-TS-44-071725

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 23 01:48:28 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 22 09:14:26 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

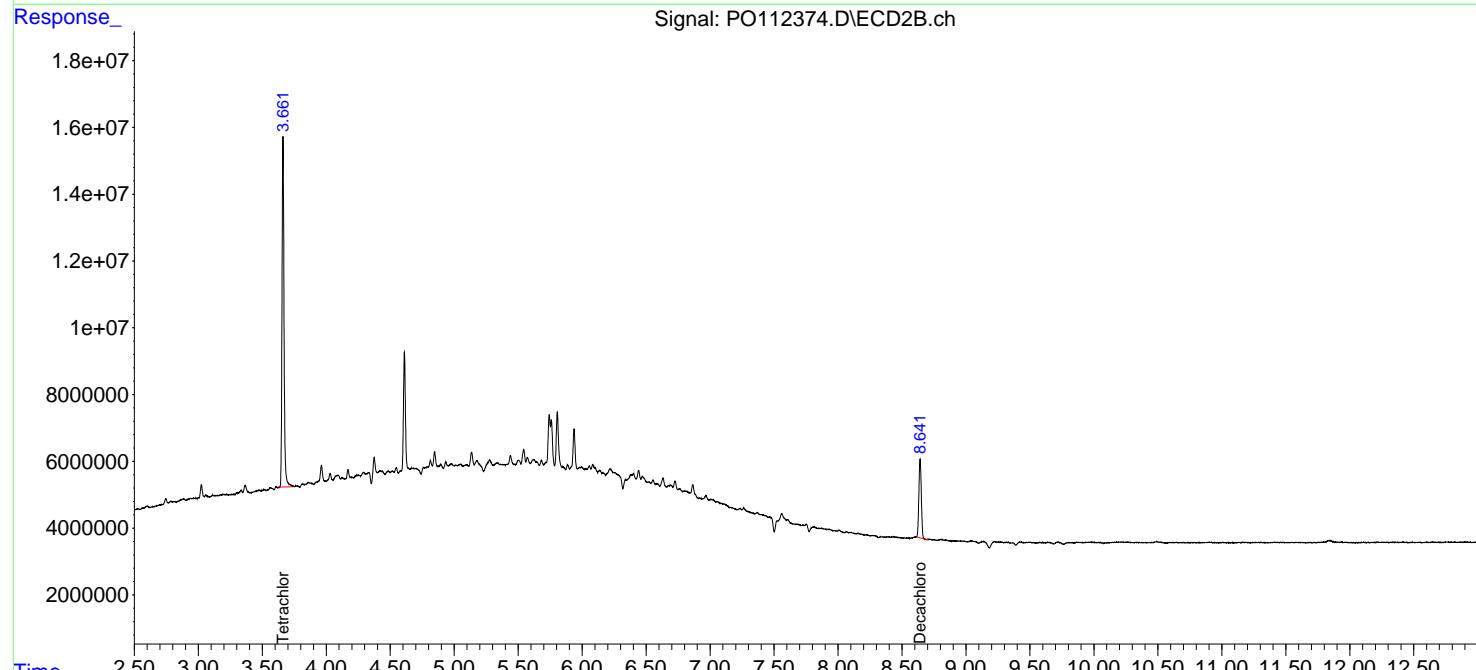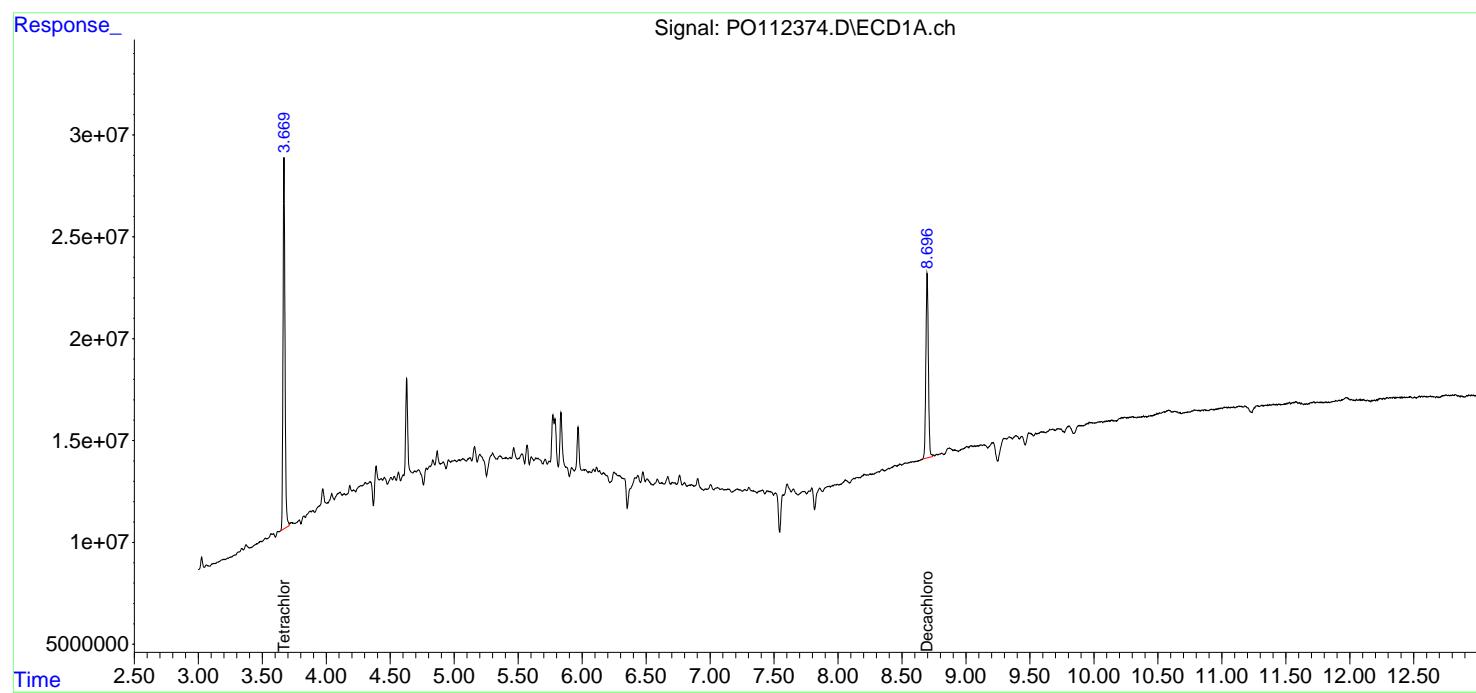

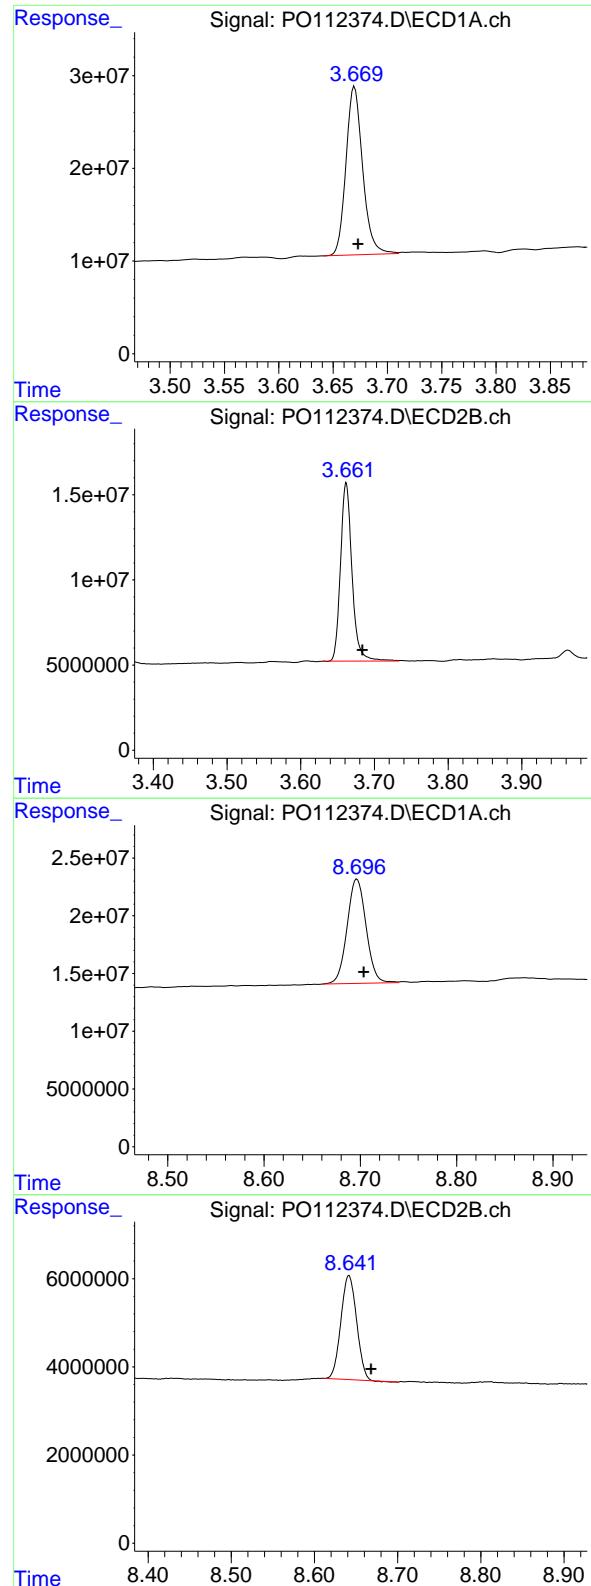

#1 Tetrachloro-m-xylene

R.T.: 3.670 min
 Delta R.T.: -0.003 min
 Response: 193743659
 Conc: 19.58 ng/ml

Instrument: ECD_O
 ClientSampleId: OU4-TS-44-071725

#1 Tetrachloro-m-xylene

R.T.: 3.662 min
 Delta R.T.: -0.022 min
 Response: 113734438
 Conc: 17.85 ng/ml

#2 Decachlorobiphenyl

R.T.: 8.697 min
 Delta R.T.: -0.007 min
 Response: 123156990
 Conc: 18.01 ng/ml

#2 Decachlorobiphenyl

R.T.: 8.641 min
 Delta R.T.: -0.027 min
 Response: 31010440
 Conc: 17.99 ng/ml



CALIBRATION

SUMMARY



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

RETENTION TIMES OF INITIAL CALIBRATION

Lab Name:	Alliance	Contract:	NOBI03
Lab Code:	ACE	SDG NO.:	Q2639
Instrument ID:	ECD_O	Calibration Date(s):	07/08/2025 07/08/2025
		Calibration Times:	14:06 22:16

GC Column: ZB-MR1 ID: 0.32 (mm)

LAB FILE ID:	RT 1000 =	PO112088.D	RT 750 =	PO112089.D
	RT 500 = PO112090.D	RT 250 = PO112091.D	RT 050 =	PO112092.D

COMPOUND	RT 1000	RT 750	RT 500	RT 250	RT 050	MEAN RT	RT WINDOW FROM	TO
Aroclor-1016-1 (1)	4.76	4.76	4.76	4.76	4.76	4.76	4.66	4.86
Aroclor-1016-2 (2)	4.78	4.78	4.78	4.78	4.78	4.78	4.68	4.88
Aroclor-1016-3 (3)	4.83	4.84	4.84	4.84	4.84	4.84	4.74	4.94
Aroclor-1016-4 (4)	4.95	4.96	4.96	4.96	4.96	4.96	4.86	5.06
Aroclor-1016-5 (5)	5.21	5.21	5.21	5.21	5.21	5.21	5.11	5.31
Aroclor-1260-1 (1)	6.25	6.25	6.25	6.25	6.25	6.25	6.15	6.35
Aroclor-1260-2 (2)	6.44	6.44	6.44	6.44	6.44	6.44	6.34	6.54
Aroclor-1260-3 (3)	6.81	6.81	6.81	6.81	6.81	6.81	6.71	6.91
Aroclor-1260-4 (4)	7.07	7.07	7.07	7.07	7.07	7.07	6.97	7.17
Aroclor-1260-5 (5)	7.31	7.31	7.31	7.31	7.31	7.31	7.21	7.41
Decachlorobiphenyl	8.70	8.70	8.70	8.70	8.70	8.70	8.60	8.80
Tetrachloro-m-xylene	3.67	3.67	3.67	3.67	3.67	3.67	3.57	3.77
Aroclor-1242-1 (1)	4.76	4.76	4.76	4.76	4.76	4.76	4.66	4.86
Aroclor-1242-2 (2)	4.78	4.78	4.78	4.78	4.78	4.78	4.68	4.88
Aroclor-1242-3 (3)	4.84	4.84	4.84	4.84	4.84	4.84	4.74	4.94
Aroclor-1242-4 (4)	4.96	4.96	4.96	4.96	4.96	4.96	4.86	5.06
Aroclor-1242-5 (5)	5.61	5.61	5.61	5.61	5.61	5.61	5.51	5.71
Decachlorobiphenyl	8.70	8.70	8.70	8.70	8.70	8.70	8.60	8.80
Tetrachloro-m-xylene	3.67	3.67	3.67	3.67	3.67	3.67	3.57	3.77
Aroclor-1248-1 (1)	4.76	4.76	4.76	4.76	4.76	4.76	4.66	4.86
Aroclor-1248-2 (2)	5.00	5.00	5.00	5.00	5.00	5.00	4.90	5.10
Aroclor-1248-3 (3)	5.21	5.21	5.21	5.21	5.21	5.21	5.11	5.31
Aroclor-1248-4 (4)	5.57	5.56	5.57	5.57	5.57	5.57	5.47	5.67
Aroclor-1248-5 (5)	5.61	5.61	5.61	5.61	5.61	5.61	5.51	5.71
Decachlorobiphenyl	8.70	8.70	8.70	8.70	8.70	8.70	8.60	8.80
Tetrachloro-m-xylene	3.67	3.67	3.67	3.67	3.67	3.67	3.57	3.77
Aroclor-1254-1 (1)	5.57	5.56	5.57	5.57	5.57	5.57	5.47	5.67
Aroclor-1254-2 (2)	5.72	5.71	5.72	5.71	5.71	5.72	5.62	5.82
Aroclor-1254-3 (3)	6.12	6.12	6.12	6.12	6.12	6.12	6.02	6.22
Aroclor-1254-4 (4)	6.35	6.35	6.35	6.35	6.35	6.35	6.25	6.45
Aroclor-1254-5 (5)	6.77	6.77	6.77	6.77	6.77	6.77	6.67	6.87
Decachlorobiphenyl	8.70	8.70	8.70	8.70	8.70	8.70	8.60	8.80
Tetrachloro-m-xylene	3.67	3.67	3.67	3.67	3.67	3.67	3.57	3.77
Aroclor-1268-1 (1)	7.59	7.59	7.59	7.59	7.59	7.59	7.49	7.69
Aroclor-1268-2 (2)	7.66	7.66	7.66	7.66	7.66	7.66	7.56	7.76
Aroclor-1268-3 (3)	7.86	7.86	7.86	7.86	7.86	7.86	7.76	7.96
Aroclor-1268-4 (4)	8.15	8.15	8.15	8.15	8.15	8.15	8.05	8.25
Aroclor-1268-5 (5)	8.45	8.44	8.45	8.45	8.45	8.45	8.35	8.55



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

RETENTION TIMES OF INITIAL CALIBRATION

Decachlorobiphenyl	8.70	8.70	8.70	8.70	8.70	8.70	8.60	8.80	1
Tetrachloro-m-xylene	3.67	3.67	3.67	3.67	3.67	3.67	3.57	3.77	2

3

4

5

6

7

8

9

10

11

12

13

14

15

16

17

18

19

20



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

RETENTION TIMES OF INITIAL CALIBRATION

Lab Name:	Alliance	Contract:	NOBI03
Lab Code:	ACE	SDG NO.:	Q2639
Instrument ID:	ECD_O	Calibration Date(s):	07/08/2025 07/08/2025
		Calibration Times:	14:06 22:16

GC Column: ZB-MR2 ID: 0.32 (mm)

LAB FILE ID:	RT 1000 =	PO112088.D	RT 750 =	PO112089.D
	RT 500 = PO112090.D	RT 250 = PO112091.D	RT 050 =	PO112092.D

COMPOUND	RT 1000	RT 750	RT 500	RT 250	RT 050	MEAN RT	RT WINDOW FROM	TO
Aroclor-1016-1 (1)	4.74	4.74	4.76	4.74	4.74	4.75	4.65	4.85
Aroclor-1016-2 (2)	4.76	4.76	4.78	4.76	4.76	4.77	4.67	4.87
Aroclor-1016-3 (3)	4.94	4.94	4.95	4.94	4.94	4.94	4.84	5.04
Aroclor-1016-4 (4)	4.98	4.98	5.00	4.98	4.98	4.98	4.88	5.08
Aroclor-1016-5 (5)	5.19	5.19	5.21	5.19	5.19	5.20	5.10	5.30
Aroclor-1260-1 (1)	6.22	6.22	6.24	6.22	6.22	6.22	6.12	6.32
Aroclor-1260-2 (2)	6.41	6.41	6.43	6.41	6.41	6.41	6.31	6.51
Aroclor-1260-3 (3)	6.56	6.56	6.58	6.56	6.56	6.56	6.46	6.66
Aroclor-1260-4 (4)	7.03	7.03	7.05	7.03	7.03	7.03	6.93	7.13
Aroclor-1260-5 (5)	7.27	7.27	7.29	7.27	7.27	7.28	7.18	7.38
Decachlorobiphenyl	8.65	8.65	8.67	8.65	8.65	8.65	8.55	8.75
Tetrachloro-m-xylene	3.67	3.67	3.68	3.67	3.67	3.67	3.57	3.77
Aroclor-1242-1 (1)	4.74	4.74	4.74	4.74	4.74	4.74	4.64	4.84
Aroclor-1242-2 (2)	4.76	4.76	4.76	4.76	4.76	4.76	4.66	4.86
Aroclor-1242-3 (3)	4.94	4.94	4.94	4.94	4.94	4.94	4.84	5.04
Aroclor-1242-4 (4)	5.02	5.02	5.02	5.02	5.02	5.02	4.92	5.12
Aroclor-1242-5 (5)	5.54	5.54	5.54	5.54	5.54	5.54	5.44	5.64
Decachlorobiphenyl	8.65	8.65	8.65	8.65	8.65	8.65	8.55	8.75
Tetrachloro-m-xylene	3.67	3.67	3.67	3.67	3.67	3.67	3.57	3.77
Aroclor-1248-1 (1)	4.74	4.74	4.74	4.74	4.74	4.74	4.64	4.84
Aroclor-1248-2 (2)	4.98	4.98	4.98	4.98	4.98	4.98	4.88	5.08
Aroclor-1248-3 (3)	5.02	5.02	5.02	5.02	5.02	5.02	4.92	5.12
Aroclor-1248-4 (4)	5.19	5.19	5.19	5.19	5.19	5.19	5.09	5.29
Aroclor-1248-5 (5)	5.58	5.58	5.58	5.58	5.58	5.58	5.48	5.68
Decachlorobiphenyl	8.65	8.65	8.65	8.65	8.65	8.65	8.55	8.75
Tetrachloro-m-xylene	3.67	3.67	3.67	3.67	3.67	3.67	3.57	3.77
Aroclor-1254-1 (1)	5.54	5.54	5.54	5.54	5.54	5.54	5.44	5.64
Aroclor-1254-2 (2)	5.69	5.69	5.69	5.69	5.69	5.69	5.59	5.79
Aroclor-1254-3 (3)	6.09	6.09	6.09	6.09	6.09	6.09	5.99	6.19
Aroclor-1254-4 (4)	6.32	6.32	6.32	6.32	6.32	6.32	6.22	6.42
Aroclor-1254-5 (5)	6.74	6.73	6.73	6.73	6.73	6.73	6.63	6.83
Decachlorobiphenyl	8.65	8.65	8.65	8.65	8.65	8.65	8.55	8.75
Tetrachloro-m-xylene	3.67	3.67	3.67	3.67	3.67	3.67	3.57	3.77
Aroclor-1268-1 (1)	7.55	7.55	7.55	7.55	7.55	7.55	7.45	7.65
Aroclor-1268-2 (2)	7.62	7.62	7.62	7.62	7.62	7.62	7.52	7.72
Aroclor-1268-3 (3)	7.82	7.82	7.82	7.82	7.82	7.82	7.72	7.92
Aroclor-1268-4 (4)	8.11	8.11	8.11	8.11	8.11	8.11	8.01	8.21
Aroclor-1268-5 (5)	8.40	8.40	8.40	8.40	8.40	8.40	8.30	8.50



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

RETENTION TIMES OF INITIAL CALIBRATION

Decachlorobiphenyl	8.65	8.65	8.65	8.65	8.65	8.65	8.55	8.75	1
Tetrachloro-m-xylene	3.67	3.67	3.67	3.67	3.67	3.67	3.57	3.77	2

3
4
5
6
7
8
9
10
11
12
13
14
15
16
17
18
19
20



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

CALIBRATION FACTOR OF INITIAL CALIBRATION

Lab Name:	Alliance	Contract:	NOBI03	
Lab Code:	ACE	SDG NO.:	Q2639	
Instrument ID:	ECD_O	Calibration Date(s):	07/08/2025	07/08/2025
		Calibration Times:	14:06	22:16
GC Column:	ZB-MR1			
ID:	0.32	(mm)		

LAB FILE ID:	CF 1000 =	PO112088.D	CF 750 =	PO112089.D			
	CF 500 =	PO112090.D	CF 250 =	PO112091.D	CF 050 =	PO112092.D	
COMPOUND	CF 1000	CF 750	CF 500	CF 250	CF 050	CF	% RSD
Aroclor-1016-1 (1)	360742355	353411084	358608078	351811628	276040300	340122689	11
Aroclor-1016-2 (2)	524757576	513734579	527286258	524874328	395805960	497291740	11
Aroclor-1016-3 (3)	332829086	325012079	334990372	341827996	283910480	323714003	7
Aroclor-1016-4 (4)	267114546	263557440	269039266	265481824	218804880	256799591	8
Aroclor-1016-5 (5)	281257689	272140703	280446704	285989380	248475020	273661899	5
Aroclor-1260-1 (1)	515263930	514045125	524528068	524922328	427435480	501238986	8
Aroclor-1260-2 (2)	755458656	751801572	763083688	740918324	679411120	738134672	5
Aroclor-1260-3 (3)	672764264	679771911	697132702	647584436	580156380	655481939	7
Aroclor-1260-4 (4)	428461498	442815881	457502760	461118372	386340060	435247714	7
Aroclor-1260-5 (5)	1355306152	1333629501	1317199750	1298892100	1007658700	1262537241	11
Decachlorobiphenyl	7091695750	7147123880	7182630500	7285420480	5478354000	6837044922	11
Tetrachloro-m-xylene	10813397260	10474815627	10513291260	10183518000	7488479400	9894700309	14
Aroclor-1242-1 (1)	285009923	305769684	302587940	302628584	252187260	289636678	8
Aroclor-1242-2 (2)	424985528	451558340	449561854	447967952	355524300	425919595	10
Aroclor-1242-3 (3)	267327438	285181779	287377204	288451804	240089600	273685565	8
Aroclor-1242-4 (4)	217524144	232173980	231748124	232379948	212764400	225318119	4
Aroclor-1242-5 (5)	218416651	232437525	224522496	231546684	151431360	211670943	16
Decachlorobiphenyl	6979969120	7147406973	7161879360	7131310800	5658336400	6815780531	10
Tetrachloro-m-xylene	10047633560	10752033107	10538404740	10524037960	8582543200	10088930513	9
Aroclor-1248-1 (1)	231871262	227298380	227625104	251373404	196330000	226899630	9
Aroclor-1248-2 (2)	312226784	305819339	307255800	349605332	266719220	308325295	10
Aroclor-1248-3 (3)	394903515	391569029	392918442	459601740	397606080	407319761	7
Aroclor-1248-4 (4)	577144829	572571723	575557162	615211088	545252760	577147512	4
Aroclor-1248-5 (5)	391149352	391468967	390698366	435680552	342525360	390304519	8
Decachlorobiphenyl	7164669710	7172590053	7258610400	7568481440	5849763800	7002823081	10
Tetrachloro-m-xylene	10966260810	10668995880	10533016680	11674212280	8664104600	10501318050	11
Aroclor-1254-1 (1)	596387386	615301855	615556214	631197528	617123200	615113237	2
Aroclor-1254-2 (2)	526620849	541456496	538329150	552782544	519240660	535685940	2
Aroclor-1254-3 (3)	832372124	848375105	844598876	861920200	810621920	839577645	2
Aroclor-1254-4 (4)	488348458	550588549	528046518	514011204	324098800	481018706	19
Aroclor-1254-5 (5)	772769124	785953607	791521408	805117428	714377600	773947833	5
Decachlorobiphenyl	7313218520	7363897040	7524909560	7619539480	6511414600	7266595840	6
Tetrachloro-m-xylene	10817495530	10970019693	10749863260	10915129200	9106609200	10511823377	8
Aroclor-1268-1 (1)	1933697823	1961714709	1933333182	1889919492	1468606580	1837454357	11



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

CALIBRATION FACTOR OF INITIAL CALIBRATION

Aroclor-1268-2	(2)	1621310763	1652283559	1624883286	1597201648	1292350600	1557605971	10
Aroclor-1268-3	(3)	1337748865	1359325231	1351894922	1337301304	1112111800	1299676424	8
Aroclor-1268-4	(4)	501678112	499381901	514040784	510400332	376538760	480407978	12
Aroclor-1268-5	(5)	3474681887	3495352783	3443761070	3349732680	2555042300	3263714144	12
Decachlorobiphenyl		13779789610	14010961973	13831208240	13686235720	10617540000	13185147109	11
Tetrachloro-m-xylene		10828416470	10960168653	10714217600	10397619080	7773509600	10134786281	13

1
2
3
4
5
6
7
8
9
10
11
12
13
14
15
16
17
18
19
20



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

CALIBRATION FACTOR OF INITIAL CALIBRATION

Lab Name:	Alliance	Contract:	NOBI03	
Lab Code:	ACE	SDG NO.:	Q2639	
Instrument ID:	ECD_O	Calibration Date(s):	07/08/2025	07/08/2025
		Calibration Times:	14:06	22:16

GC Column: ZB-MR2 ID: 0.32 (mm)

LAB FILE ID:	CF 1000 =	CF 750 =	CF 500 =	CF 250 =	CF 050 =	CF	% RSD
	<u>PO112088.D</u>	<u>PO112089.D</u>	<u>PO112090.D</u>	<u>PO112091.D</u>	<u>PO112092.D</u>		
COMPOUND	CF 1000	CF 750	CF 500	CF 250	CF 050	CF	% RSD
Aroclor-1016-1 (1)	224689947	221197589	229855740	235435032	202993580	222834378	6
Aroclor-1016-2 (2)	333676696	332964816	340716574	344871116	293258760	329097592	6
Aroclor-1016-3 (3)	173220389	172286476	177510406	175323720	150993180	169866834	6
Aroclor-1016-4 (4)	133548654	134722825	140696304	141544972	135624760	137227503	3
Aroclor-1016-5 (5)	172958737	175867975	183374190	179483264	150567480	172450329	7
Aroclor-1260-1 (1)	273966572	275587577	284396370	318959696	249900320	280562107	9
Aroclor-1260-2 (2)	339471861	339883185	345098816	366340024	309189580	339996693	6
Aroclor-1260-3 (3)	285079531	283131084	293155536	294803628	221760800	275586116	11
Aroclor-1260-4 (4)	190320237	194370733	203166394	219087436	196280140	200644988	6
Aroclor-1260-5 (5)	439428363	448516680	455912584	483251276	411533840	447728549	6
Decachlorobiphenyl	1708564380	1754251880	1790007560	1862375960	1502102800	1723460516	8
Tetrachloro-m-xylene	6849689250	6688775747	6823852720	6660365320	4832613200	6371059247	14
Aroclor-1242-1 (1)	180558203	194276476	196154442	205920884	192381760	193858353	5
Aroclor-1242-2 (2)	267145812	285888559	288791934	297310352	277625120	283352355	4
Aroclor-1242-3 (3)	139388587	149896708	150012144	154353128	134735720	145677257	6
Aroclor-1242-4 (4)	132647733	142511831	143624204	149839712	140580100	141840716	4
Aroclor-1242-5 (5)	169256952	182077477	187071418	199409696	170855060	181734121	7
Decachlorobiphenyl	1694985930	1765973813	1799728340	1866433600	1579982000	1741420737	6
Tetrachloro-m-xylene	6408694870	6872035667	6730718280	6766792760	5539281400	6463504595	8
Aroclor-1248-1 (1)	148373409	146783767	149637550	173598112	153448100	154368188	7
Aroclor-1248-2 (2)	200165378	198242231	203122858	230241332	197066700	205767700	7
Aroclor-1248-3 (3)	210851108	208337667	212783398	242780584	199239520	214798455	8
Aroclor-1248-4 (4)	249491134	246252407	253519016	297759984	246611360	258726780	9
Aroclor-1248-5 (5)	244390847	243395885	250986596	299503676	214470400	250549481	12
Decachlorobiphenyl	1741004980	1773180160	1834926600	1999524800	1593214800	1788370268	8
Tetrachloro-m-xylene	6922029440	6722968493	6653358760	7457216520	5595884000	6670291443	10
Aroclor-1254-1 (1)	358701312	372366800	376618238	404921504	393233780	381168327	5
Aroclor-1254-2 (2)	309319461	318506233	325963420	350344944	354921460	331811104	6
Aroclor-1254-3 (3)	457035033	473473401	470706516	496812748	512186320	482042804	5
Aroclor-1254-4 (4)	242702235	264458053	264466114	273730492	258116740	260694727	4
Aroclor-1254-5 (5)	340856875	348898753	356048528	374047448	361929480	356356217	4
Decachlorobiphenyl	1762037980	1801047667	1852268780	1914979680	1705564000	1807179621	4
Tetrachloro-m-xylene	6812677640	6946187027	6790686340	6873927640	5937916200	6672278969	6
Aroclor-1268-1 (1)	486556055	496283868	499490630	514433332	460511800	491455137	4



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

CALIBRATION FACTOR OF INITIAL CALIBRATION

Aroclor-1268-2	(2)	414074889	422901423	425132138	438633692	385189960	417186420	5
Aroclor-1268-3	(3)	309607188	317937561	322370012	335163612	296865480	316388771	5
Aroclor-1268-4	(4)	111375490	114260995	115590378	117536984	98796160	111512001	7
Aroclor-1268-5	(5)	736492551	750146037	748798464	755249104	641904560	726518143	7
Decachlorobiphenyl		3139191470	3230861547	3253774420	3306379000	2721463200	3130333927	8
Tetrachloro-m-xylene		6732535870	6829120120	6762174400	6573365120	5117275800	6402894262	11

1
2
3
4
5
6
7
8
9
10
11
12
13
14
15
16
17
18
19
20



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

INITIAL CALIBRATION OF MULTICOMPONENT ANALYTES

Lab Name: Alliance

Contract: NOBI03

Lab Code: ACE

SDG NO.: Q2639

Instrument ID: ECD_O

Date(s) Analyzed: 07/08/2025 07/08/2025

GC Column: ZB-MR1

ID: 0.32 (mm)

COMPOUND	AMOUNT (ng)	PEAK	RT	RT WINDOW		CALIBRATION FACTOR
				FROM	TO	
Aroclor-1221	500	1	3.88	3.78	3.98	116614000
		2	3.97	3.87	4.07	78840600
		3	4.05	3.95	4.15	269582000
		4	0.00			0
		5	0.00			0
Aroclor-1232	500	1	4.05	3.95	4.15	214668000
		2	4.54	4.44	4.64	113637000
		3	4.78	4.68	4.88	229008000
		4	4.96	4.86	5.06	114297000
		5	5.00	4.90	5.10	73400200
Aroclor-1262	500	1	6.81	6.71	6.91	1021690000
		2	7.31	7.21	7.41	1639370000
		3	7.59	7.49	7.69	641976000
		4	7.66	7.56	7.76	1071430000
		5	8.15	8.05	8.25	448140000



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

INITIAL CALIBRATION OF MULTICOMPONENT ANALYTES

Lab Name: Alliance

Contract: NOBI03

Lab Code: ACE

SDG NO.: Q2639

Instrument ID: ECD_O

Date(s) Analyzed: 07/08/2025 07/08/2025

GC Column: ZB-MR2

ID: 0.32 (mm)

COMPOUND	AMOUNT (ng)	PEAK	RT	RT WINDOW		CALIBRATION FACTOR
				FROM	TO	
Aroclor-1221	500	1	3.88	3.78	3.98	82295000
		2	3.96	3.86	4.06	59353600
		3	4.04	3.94	4.14	188777000
		4	0.00			0
		5	0.00			0
Aroclor-1232	500	1	4.04	3.94	4.14	150099000
		2	4.76	4.66	4.86	153086000
		3	4.94	4.84	5.04	75506000
		4	5.02	4.92	5.12	65988200
		5	5.19	5.09	5.29	74260000
Aroclor-1262	500	1	6.77	6.67	6.87	407320000
		2	7.27	7.17	7.37	512548000
		3	7.55	7.45	7.65	179524000
		4	7.62	7.52	7.72	290920000
		5	8.11	8.01	8.21	105784000

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0070825\
 Data File : P0112088.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jul 2025 14:06
 Operator : YP/AJ
 Sample : AR1660ICC1000
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1660ICC1000

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/09/2025
 Supervised By :mohammad ahmed 07/10/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 08 15:11:12 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 08 15:05:13 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	3.671	3.666	1081.3E6	685.0E6	101.527m	100.423m
2) SA Decachlor...	8.702	8.649	709.2E6	170.9E6	99.363	97.492m

Target Compounds

3) L1 AR-1016-1	4.759	4.743	360.7E6	224.7E6	1002.967	1009.911
4) L1 AR-1016-2	4.777	4.761	524.8E6	333.7E6	997.596	990.816
5) L1 AR-1016-3	4.834	4.936	332.8E6	173.2E6	996.764	996.808m
6) L1 AR-1016-4	4.954	4.980	267.1E6	133.5E6	996.410	973.937
7) L1 AR-1016-5	5.211	5.191	281.3E6	173.0E6	1001.444	970.770
31) L7 AR-1260-1	6.249	6.220	515.3E6	274.0E6	991.090	981.321
32) L7 AR-1260-2	6.438	6.409	755.5E6	339.5E6	994.979	991.780
33) L7 AR-1260-3	6.805	6.560	672.8E6	285.1E6	982.211	986.397m
34) L7 AR-1260-4	7.065	7.031	428.5E6	190.3E6	967.221	967.353
35) L7 AR-1260-5	7.308	7.272	1355.3E6	439.4E6	1014.259	981.589

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0070825\
 Data File : P0112088.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jul 2025 14:06
 Operator : YP/AJ
 Sample : AR1660ICC1000
 Misc :
 ALS Vial : 3 Sample Multiplier: 1



Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 08 15:11:12 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 08 15:05:13 2025
 Response via : Initial Calibration
 Integrator: ChemStation





Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Instrument :
 ECD_O
ClientSampleId :
 AR1660ICC1000

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/09/2025
 Supervised By :mohammad ahmed 07/10/2025

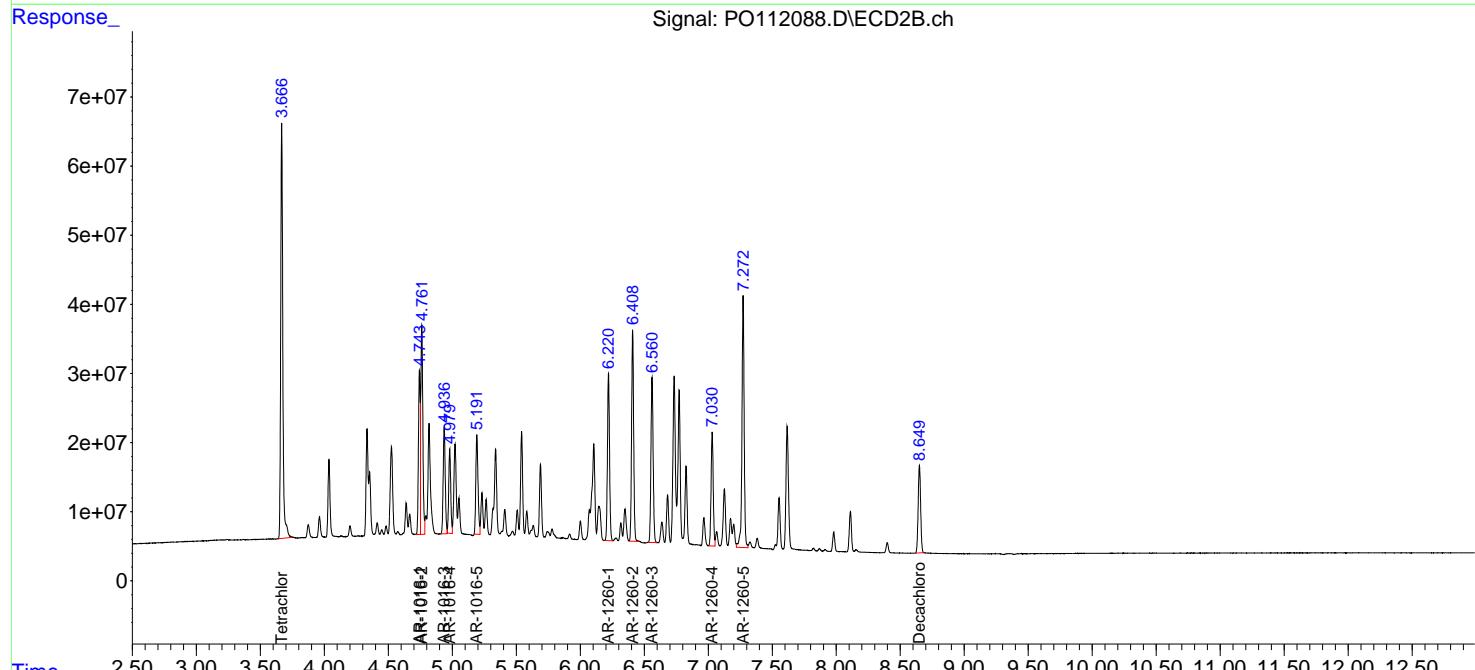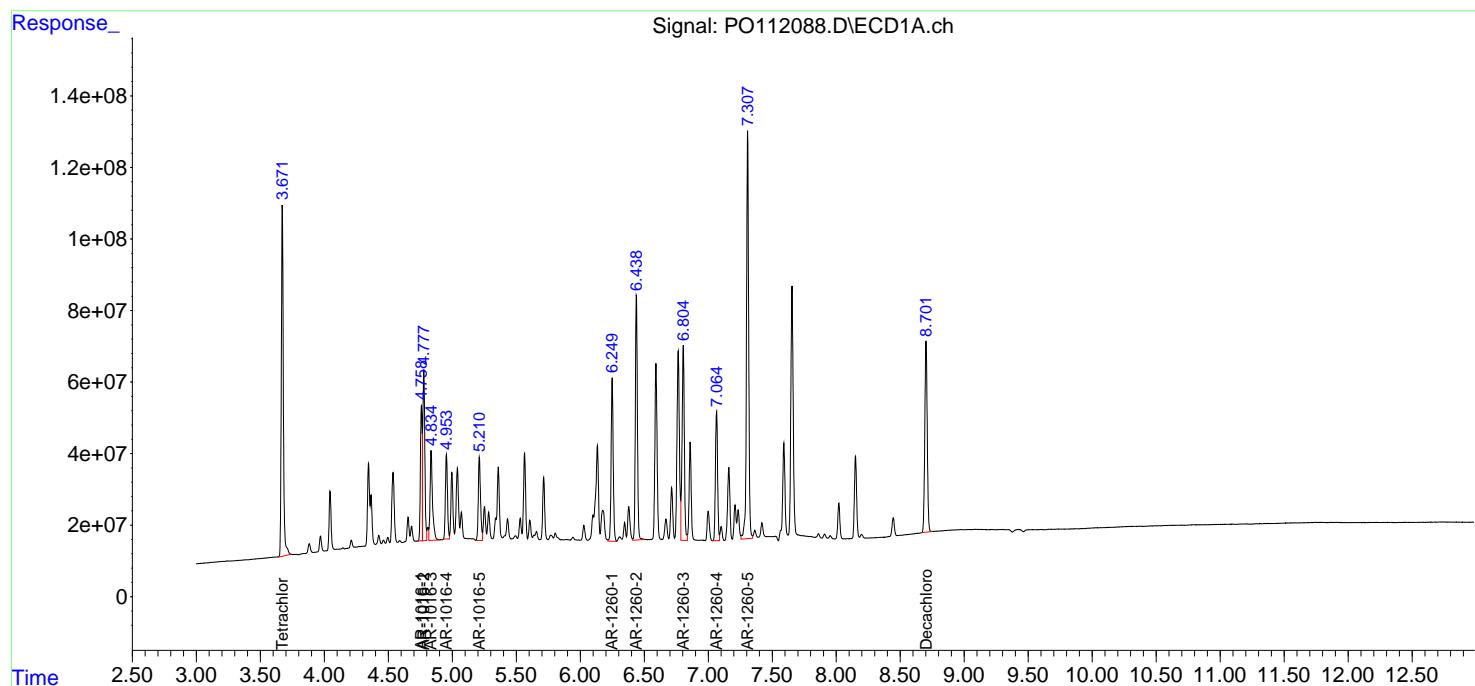

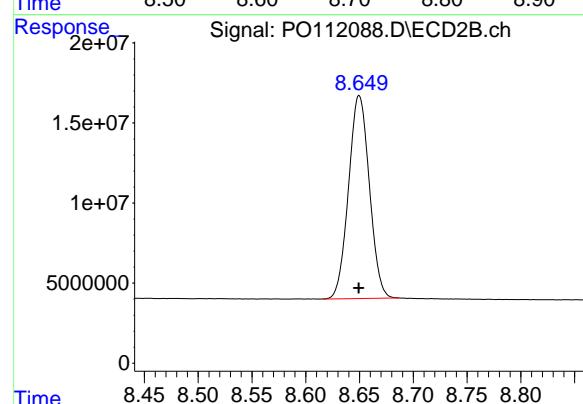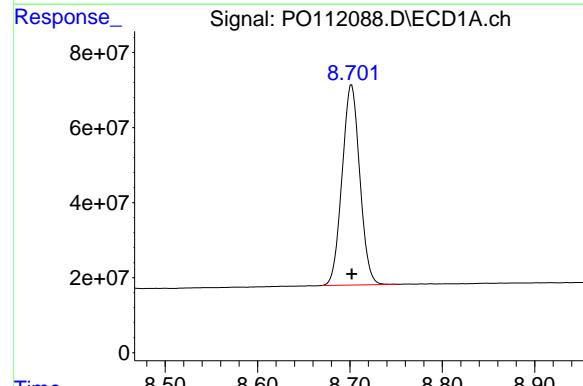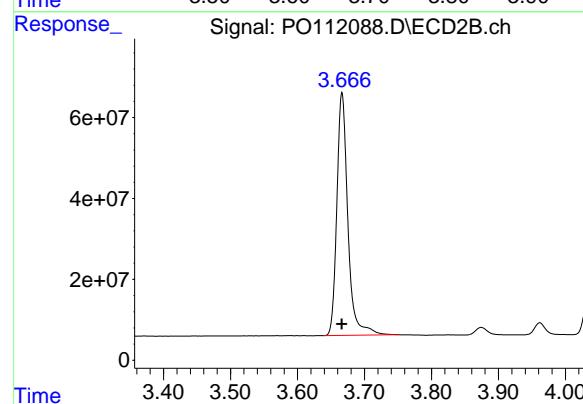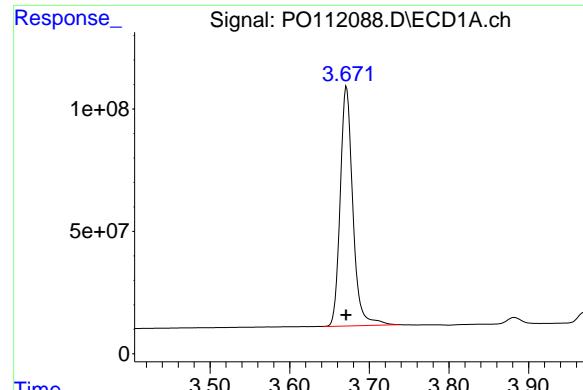

#1 Tetrachloro-m-xylene

R.T.: 3.671 min

Delta R.T.: 0.000 min

Response: 1081339726

Conc: 101.53 ng/ml

Instrument:

ECD_O

ClientSampleId :

AR1660ICC1000

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/09/2025

Supervised By :mohammad ahmed 07/10/2025

#1 Tetrachloro-m-xylene

R.T.: 3.666 min

Delta R.T.: 0.000 min

Response: 684968925

Conc: 100.42 ng/ml m

#2 Decachlorobiphenyl

R.T.: 8.702 min

Delta R.T.: 0.000 min

Response: 709169575

Conc: 99.36 ng/ml


#2 Decachlorobiphenyl

R.T.: 8.649 min

Delta R.T.: 0.000 min

Response: 170856438

Conc: 97.49 ng/ml m

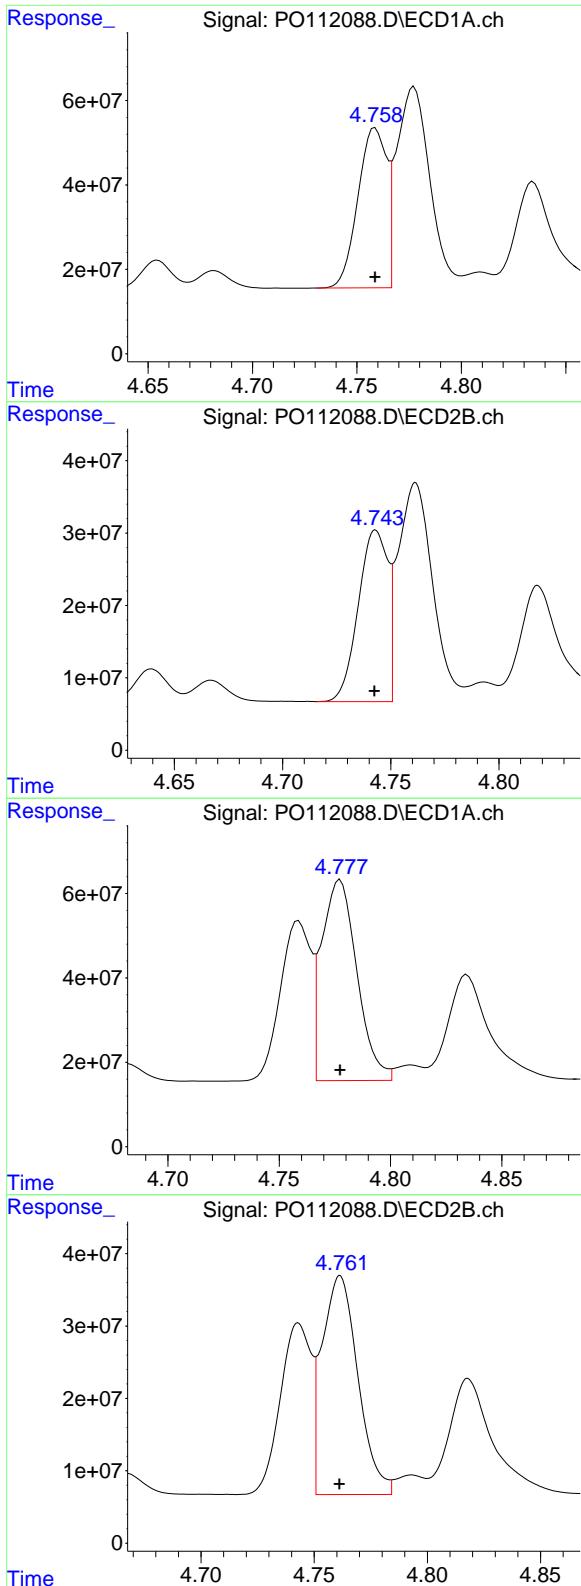

#3 AR-1016-1

R.T.: 4.759 min
Delta R.T.: 0.000 min | Instrument :
Response: 360742355 | ECD_O
Conc: 1002.97 ng/mL | ClientSampleId :
AR1660|CC1000

**Manual Integrations
APPROVED**

Reviewed By :Yogesh Patel 07/09/2025
Supervised By :mohammad ahmed 07/10/2025

#3 AR-1016-1

R.T.: 4.743 min
Delta R.T.: 0.000 min
Response: 224689947
Conc: 1009.91 ng/ml

#4 AR-1016-2

R.T.: 4.777 min
Delta R.T.: 0.000 min
Response: 524757576
Conc: 997.60 ng/ml

#4 AR-1016-2

R.T.: 4.761 min
Delta R.T.: 0.000 min
Response: 333676696
Conc: 990.82 ng/ml





#5 AR-1016-3

R.T.: 4.834 min
 Delta R.T.: 0.000 min
 Response: 332829086
 Conc: 996.76 ng/ml

Instrument: ECD_O
ClientSampleId: AR1660ICC1000

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/09/2025
 Supervised By :mohammad ahmed 07/10/2025

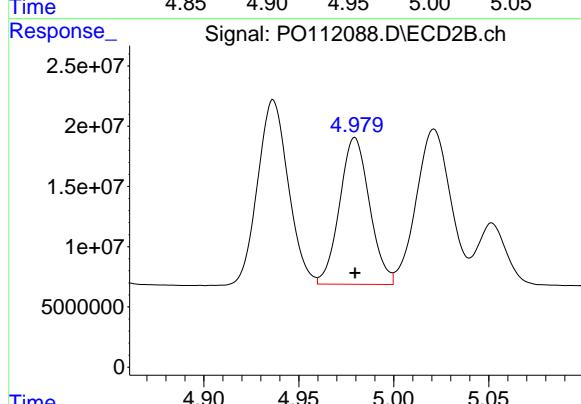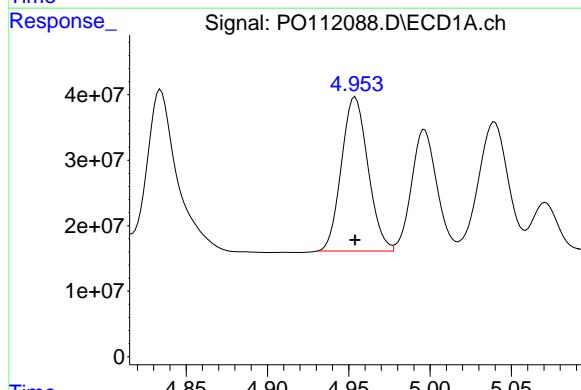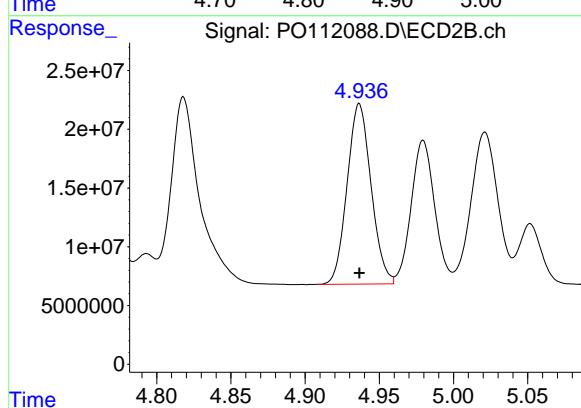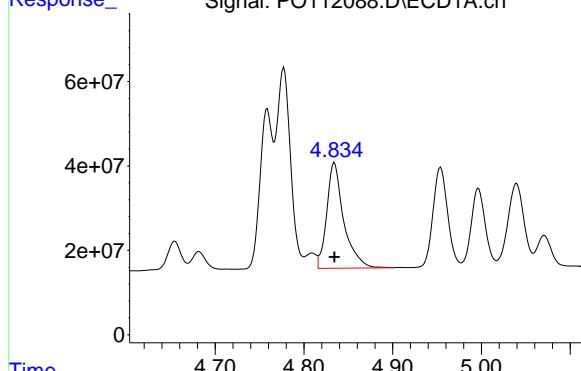

#5 AR-1016-3

R.T.: 4.936 min
 Delta R.T.: 0.000 min
 Response: 173220389
 Conc: 996.81 ng/ml

#6 AR-1016-4

R.T.: 4.954 min
 Delta R.T.: 0.000 min
 Response: 267114546
 Conc: 996.41 ng/ml

#6 AR-1016-4

R.T.: 4.980 min
 Delta R.T.: 0.000 min
 Response: 133548654
 Conc: 973.94 ng/ml





#7 AR-1016-5

R.T.: 5.211 min
 Delta R.T.: 0.000 min
 Response: 281257689
 Conc: 1001.44 ng/ml

Instrument: ECD_O
ClientSampleId: AR1660ICC1000

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/09/2025
 Supervised By :mohammad ahmed 07/10/2025

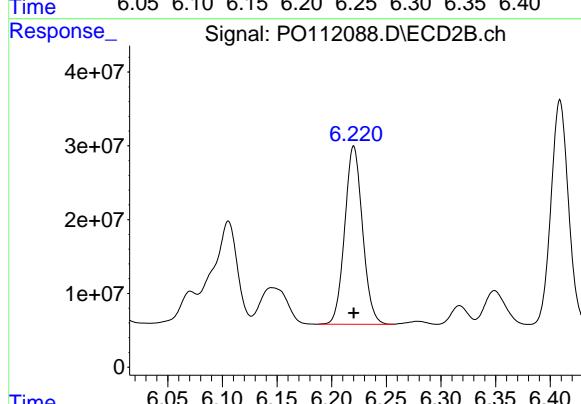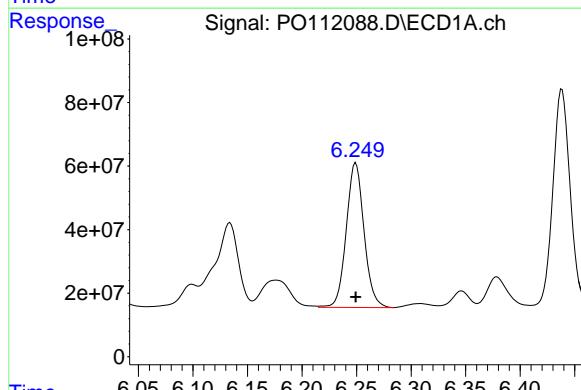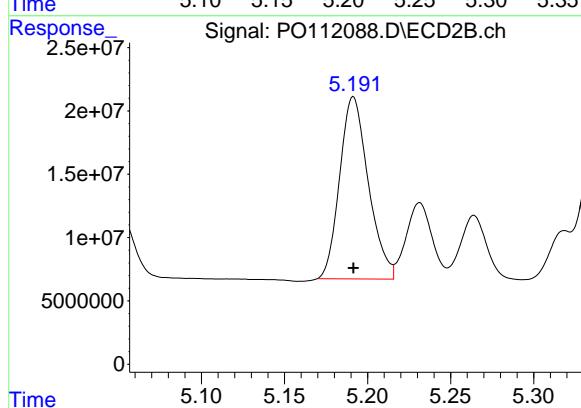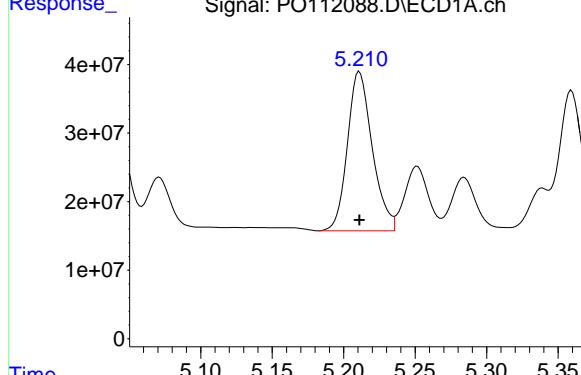

#7 AR-1016-5

R.T.: 5.191 min
 Delta R.T.: 0.000 min
 Response: 172958737
 Conc: 970.77 ng/ml

#31 AR-1260-1

R.T.: 6.249 min
 Delta R.T.: 0.000 min
 Response: 515263930
 Conc: 991.09 ng/ml

#31 AR-1260-1

R.T.: 6.220 min
 Delta R.T.: 0.000 min
 Response: 273966572
 Conc: 981.32 ng/ml

#32 AR-1260-2

R.T.: 6.438 min
 Delta R.T.: 0.000 min
 Response: 755458656
 Conc: 994.98 ng/ml

Instrument: ECD_O
ClientSampleId: AR1660ICC1000

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/09/2025
 Supervised By :mohammad ahmed 07/10/2025

#32 AR-1260-2


R.T.: 6.409 min
 Delta R.T.: 0.000 min
 Response: 339471861
 Conc: 991.78 ng/ml

#33 AR-1260-3

R.T.: 6.805 min
 Delta R.T.: 0.000 min
 Response: 672764264
 Conc: 982.21 ng/ml

#33 AR-1260-3

R.T.: 6.560 min
 Delta R.T.: 0.000 min
 Response: 285079531
 Conc: 986.40 ng/ml

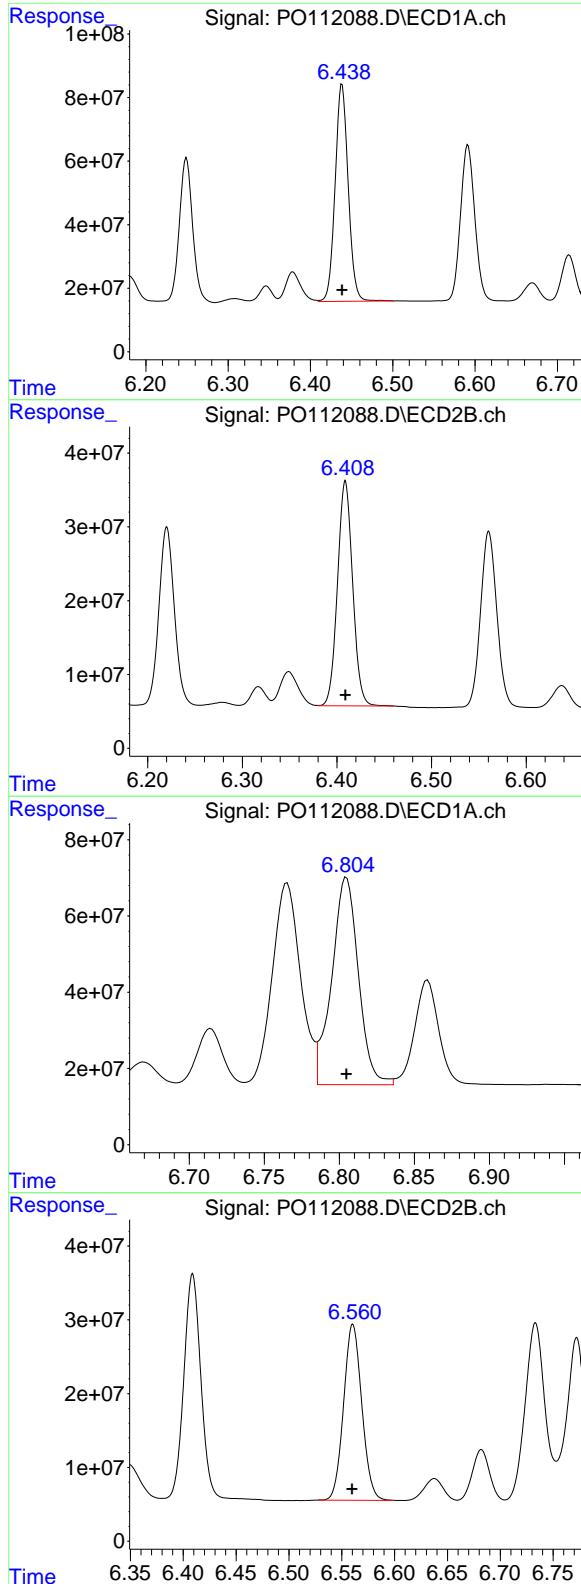

#34 AR-1260-4

R.T.: 7.065 min
 Delta R.T.: 0.000 min
 Response: 428461498
 Conc: 967.22 ng/ml

Instrument: ECD_O
ClientSampleId: AR1660ICC1000

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/09/2025
 Supervised By :mohammad ahmed 07/10/2025

#34 AR-1260-4


R.T.: 7.031 min
 Delta R.T.: 0.000 min
 Response: 190320237
 Conc: 967.35 ng/ml

#35 AR-1260-5

R.T.: 7.308 min
 Delta R.T.: 0.000 min
 Response: 1355306152
 Conc: 1014.26 ng/ml

#35 AR-1260-5

R.T.: 7.272 min
 Delta R.T.: 0.000 min
 Response: 439428363
 Conc: 981.59 ng/ml

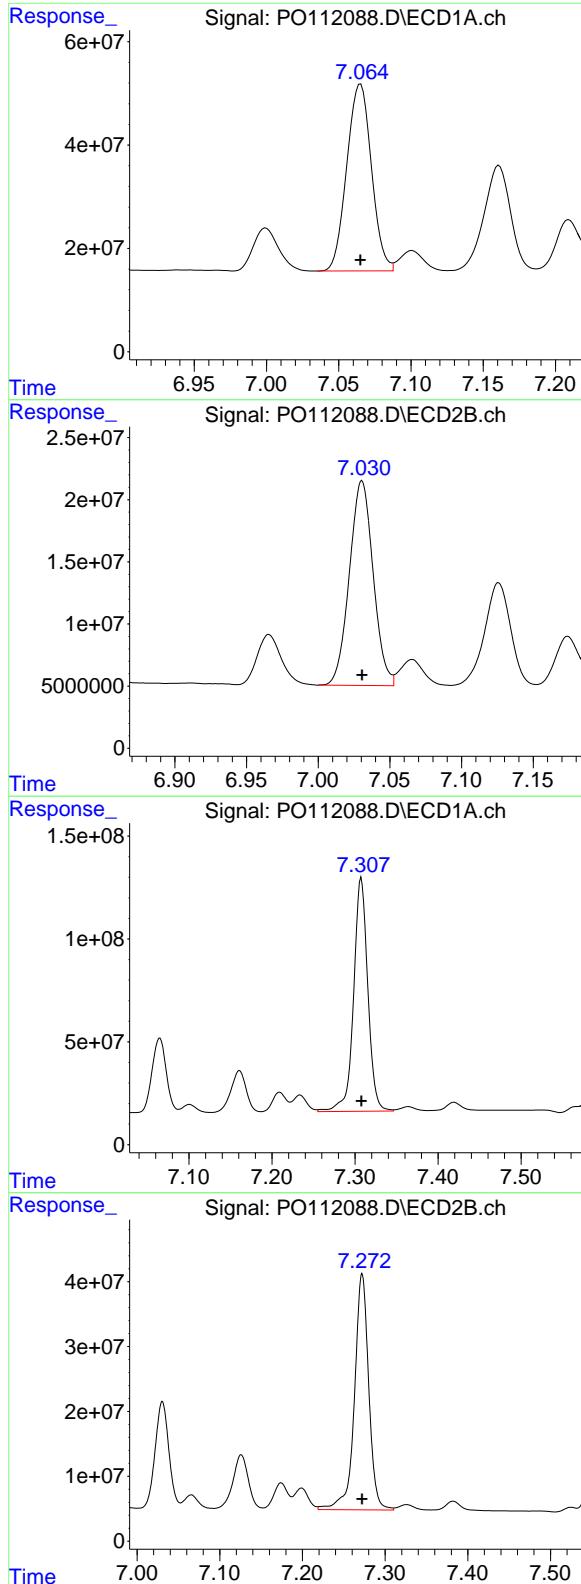

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0070825\
 Data File : P0112089.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jul 2025 14:25
 Operator : YP/AJ
 Sample : AR1660ICC750
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1660ICC750

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/09/2025
 Supervised By :mohammad ahmed 07/10/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 08 15:14:45 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 08 15:05:13 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	3.673	3.666	785.6E6	501.7E6	74.111m	73.846m
2) SA Decachlor...	8.704	8.650	536.0E6	131.6E6	75.070	75.207m

Target Compounds

3) L1 AR-1016-1	4.761	4.743	265.1E6	165.9E6	741.241	736.514
4) L1 AR-1016-2	4.780	4.762	385.3E6	249.7E6	738.229	743.699
5) L1 AR-1016-3	4.837	4.936	243.8E6	129.2E6	736.557	746.717m
6) L1 AR-1016-4	4.956	4.979	197.7E6	101.0E6	741.523	743.789m
7) L1 AR-1016-5	5.213	5.191	204.1E6	131.9E6	734.329	748.865m
31) L7 AR-1260-1	6.252	6.221	385.5E6	206.7E6	744.352	743.536
32) L7 AR-1260-2	6.441	6.409	563.9E6	254.9E6	745.065	746.483
33) L7 AR-1260-3	6.808	6.560	509.8E6	212.3E6	746.212	739.991m
34) L7 AR-1260-4	7.067	7.031	332.1E6	145.8E6	749.812	743.946
35) L7 AR-1260-5	7.309	7.273	1000.2E6	336.4E6	749.018	750.945

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0070825\
 Data File : P0112089.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jul 2025 14:25
 Operator : YP/AJ
 Sample : AR1660ICC750
 Misc :
 ALS Vial : 4 Sample Multiplier: 1



Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 08 15:14:45 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 08 15:05:13 2025
 Response via : Initial Calibration
 Integrator: ChemStation


Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Instrument :
 ECD_O
ClientSampleId :
 AR1660ICC750

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/09/2025
 Supervised By :mohammad ahmed 07/10/2025

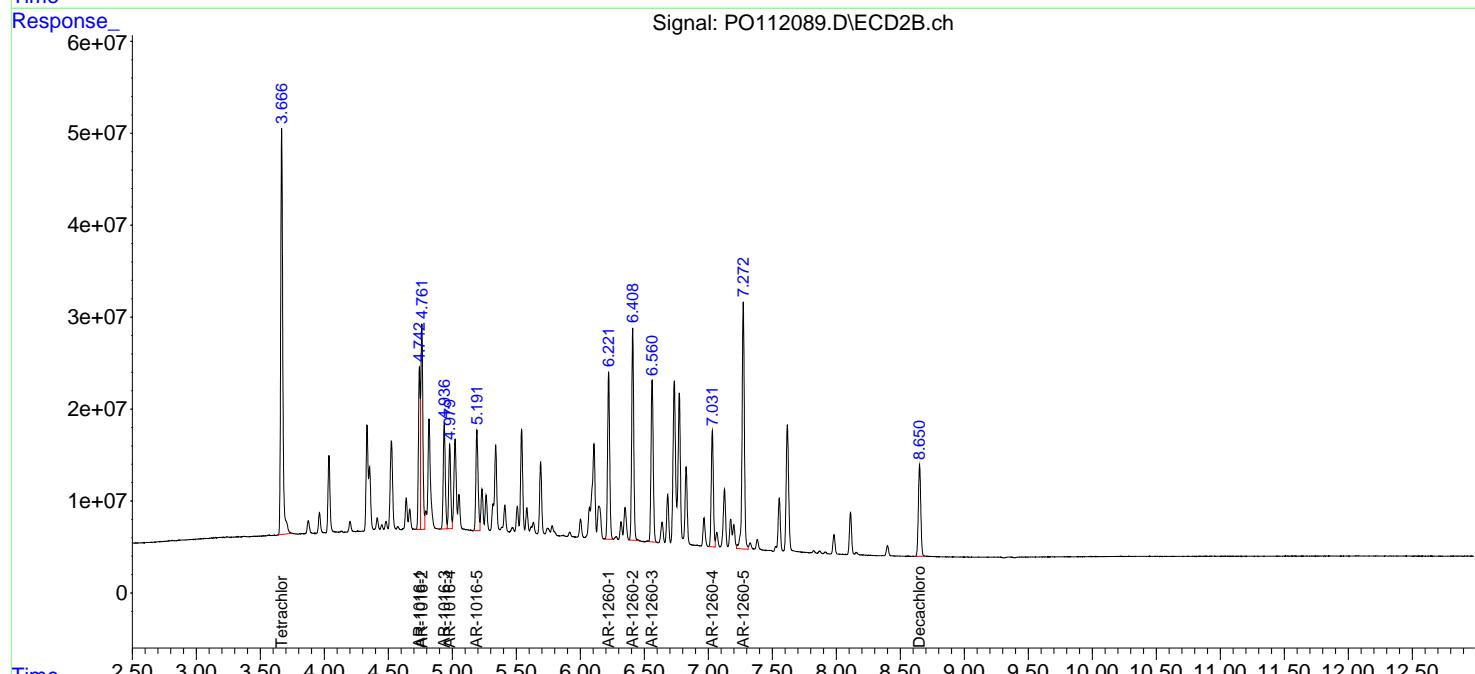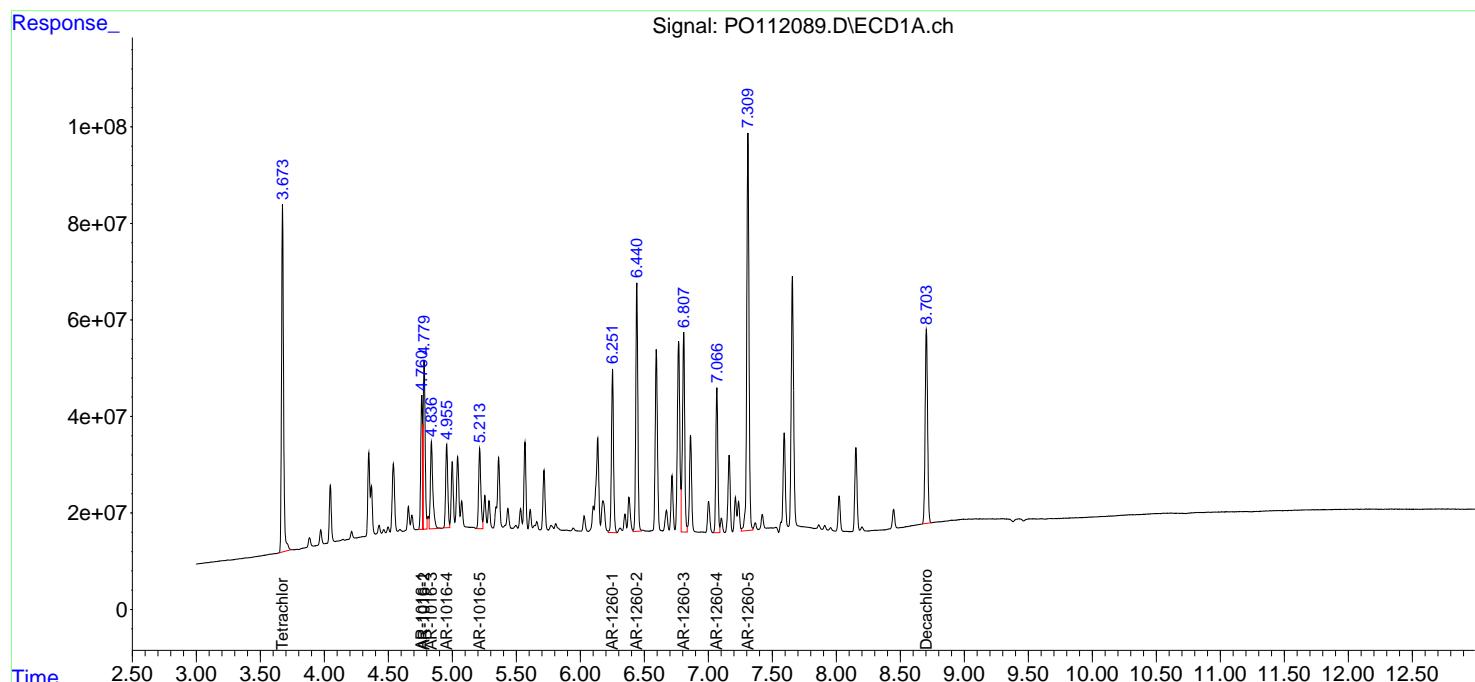

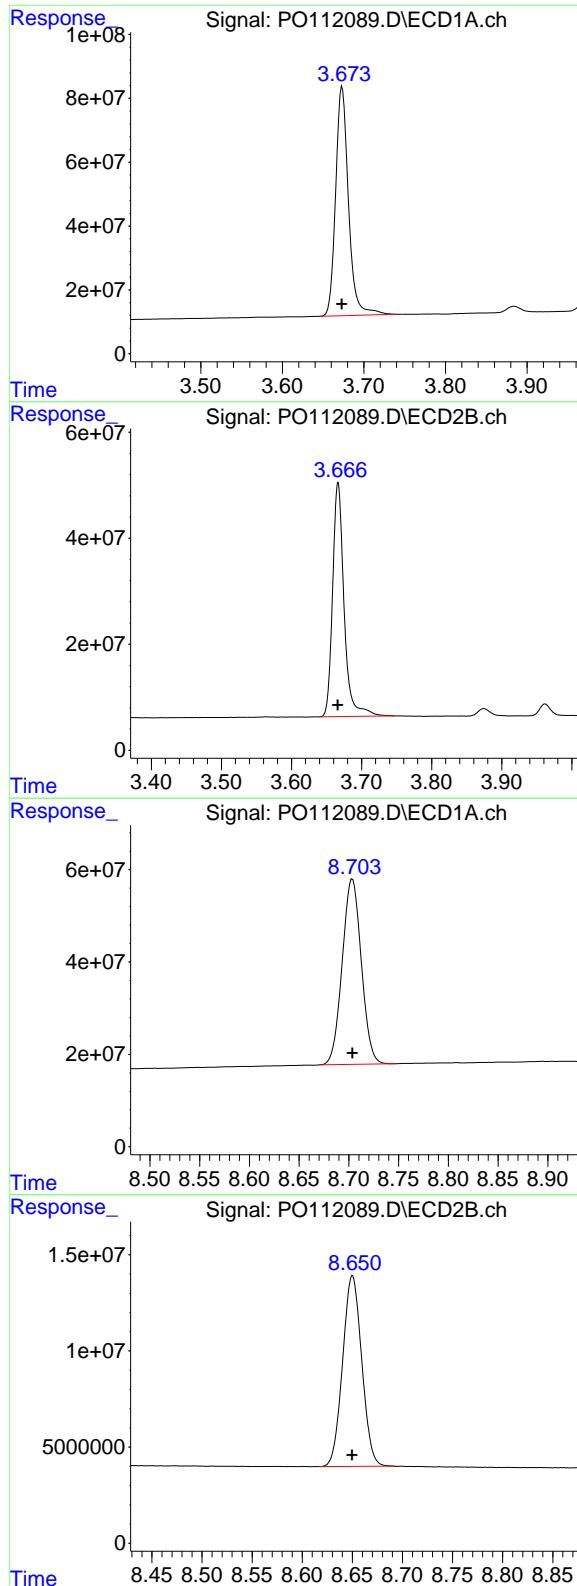

#1 Tetrachloro-m-xylene

R.T.: 3.673 min
Delta R.T.: 0.000 min
Response: 785611172
Conc: 74.11 ng/ml

Instrument:
ECD_O
ClientSampleId :
AR1660ICC750

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/09/2025
Supervised By :mohammad ahmed 07/10/2025

#1 Tetrachloro-m-xylene

R.T.: 3.666 min
Delta R.T.: 0.000 min
Response: 501658181
Conc: 73.85 ng/ml m

#2 Decachlorobiphenyl

R.T.: 8.704 min
Delta R.T.: 0.000 min
Response: 536034291
Conc: 75.07 ng/ml

#2 Decachlorobiphenyl

R.T.: 8.650 min
Delta R.T.: 0.000 min
Response: 131568891
Conc: 75.21 ng/ml m

#3 AR-1016-1

R.T.: 4.761 min
 Delta R.T.: 0.000 min
 Response: 265058313
 Conc: 741.24 ng/ml

Instrument: ECD_O
ClientSampleId: AR1660ICC750

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/09/2025
 Supervised By :mohammad ahmed 07/10/2025

#3 AR-1016-1





R.T.: 4.743 min
 Delta R.T.: 0.000 min
 Response: 165898192
 Conc: 736.51 ng/ml


#4 AR-1016-2

R.T.: 4.780 min
 Delta R.T.: 0.000 min
 Response: 385300934
 Conc: 738.23 ng/ml

#4 AR-1016-2

R.T.: 4.762 min
 Delta R.T.: 0.000 min
 Response: 249723612
 Conc: 743.70 ng/ml

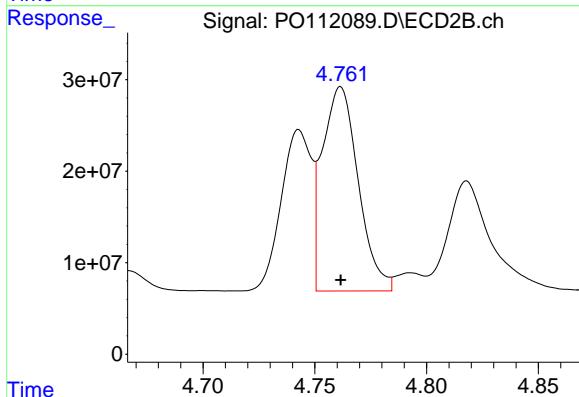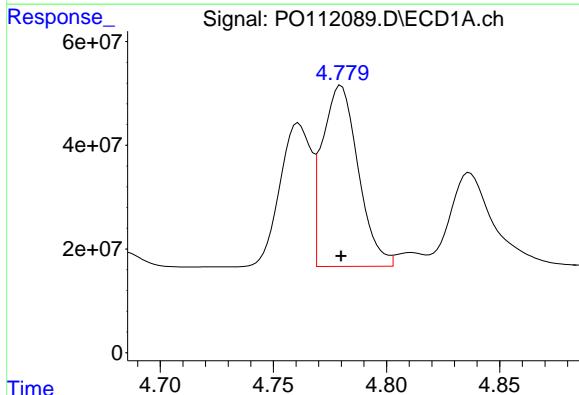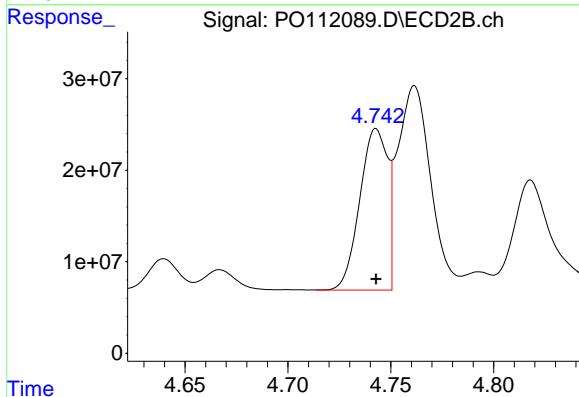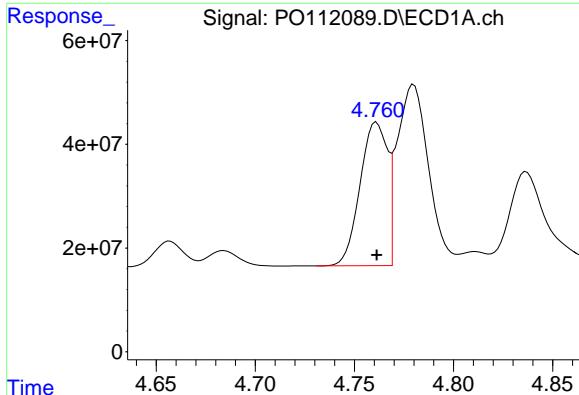

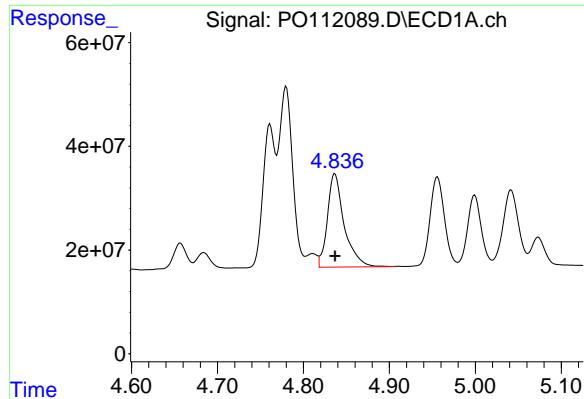


#5 AR-1016-3

R.T.: 4.837 min
Delta R.T.: 0.000 min
Response: 243759059
Conc: 736.56 ng/ml

Instrument: ECD_O
ClientSampleId: AR1660ICC750


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/09/2025
Supervised By :mohammad ahmed 07/10/2025

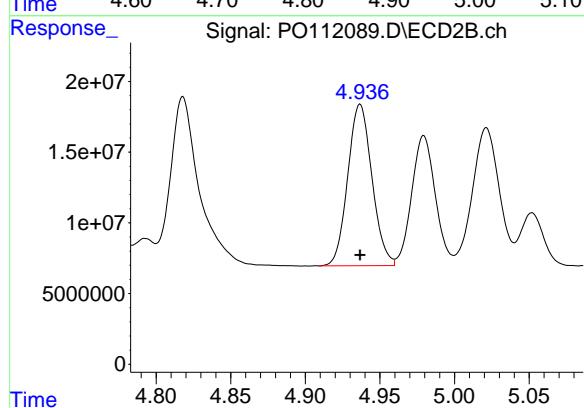


#5 AR-1016-3

R.T.: 4.936 min
Delta R.T.: 0.000 min
Response: 129214857
Conc: 746.72 ng/ml

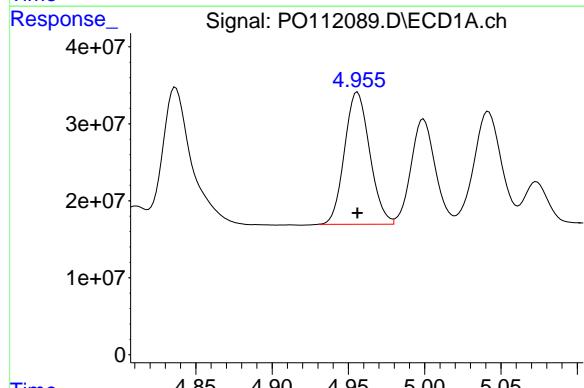


#6 AR-1016-4

R.T.: 4.956 min
Delta R.T.: 0.000 min
Response: 197668080
Conc: 741.52 ng/ml

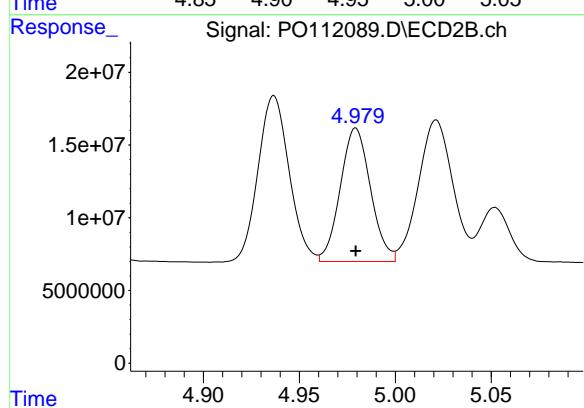

#6 AR-1016-4

R.T.: 4.979 min
Delta R.T.: 0.000 min
Response: 101042119
Conc: 743.79 ng/ml

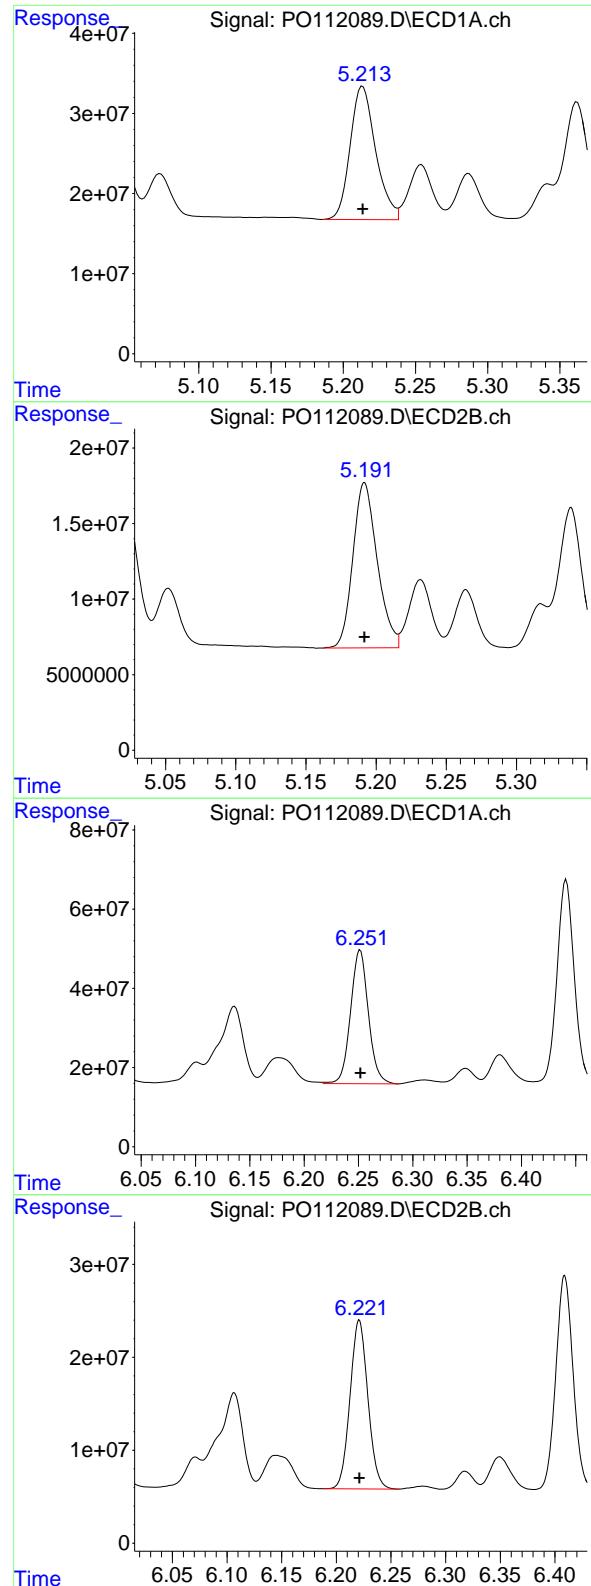

#7 AR-1016-5

R.T.: 5.213 min
 Delta R.T.: 0.000 min
 Response: 204105527
 Conc: 734.33 ng/ml

Instrument: ECD_O
ClientSampleId: AR1660ICC750

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/09/2025
 Supervised By :mohammad ahmed 07/10/2025

#7 AR-1016-5


R.T.: 5.191 min
 Delta R.T.: 0.000 min
 Response: 131900981
 Conc: 748.87 ng/ml

#31 AR-1260-1

R.T.: 6.252 min
 Delta R.T.: 0.000 min
 Response: 385533844
 Conc: 744.35 ng/ml

#31 AR-1260-1

R.T.: 6.221 min
 Delta R.T.: 0.000 min
 Response: 206690683
 Conc: 743.54 ng/ml

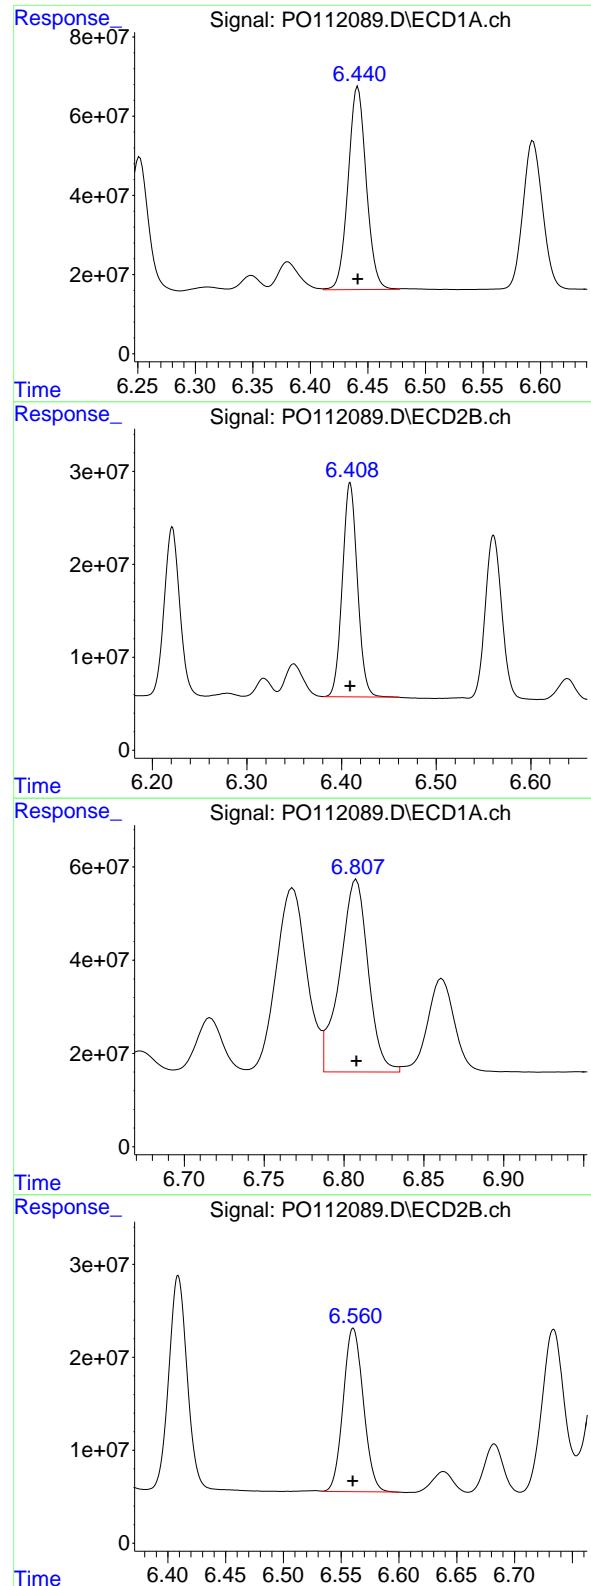

#32 AR-1260-2

R.T.: 6.441 min
 Delta R.T.: 0.000 min
 Response: 563851179
 Conc: 745.06 ng/ml

Instrument: ECD_O
ClientSampleId: AR1660ICC750

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/09/2025
 Supervised By :mohammad ahmed 07/10/2025

#32 AR-1260-2

R.T.: 6.409 min
 Delta R.T.: 0.000 min
 Response: 254912389
 Conc: 746.48 ng/ml

#33 AR-1260-3

R.T.: 6.808 min
 Delta R.T.: 0.000 min
 Response: 509828933
 Conc: 746.21 ng/ml

#33 AR-1260-3

R.T.: 6.560 min
 Delta R.T.: 0.000 min
 Response: 212348313
 Conc: 739.99 ng/ml





#34 AR-1260-4

R.T.: 7.067 min
 Delta R.T.: 0.000 min
 Response: 332111911
 Conc: 749.81 ng/ml

Instrument: ECD_O
ClientSampleId: AR1660ICC750

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/09/2025
 Supervised By :mohammad ahmed 07/10/2025

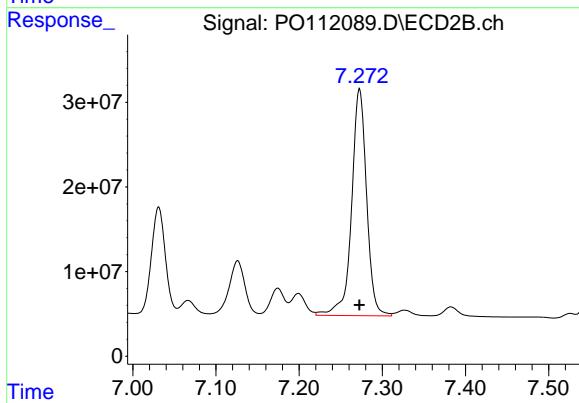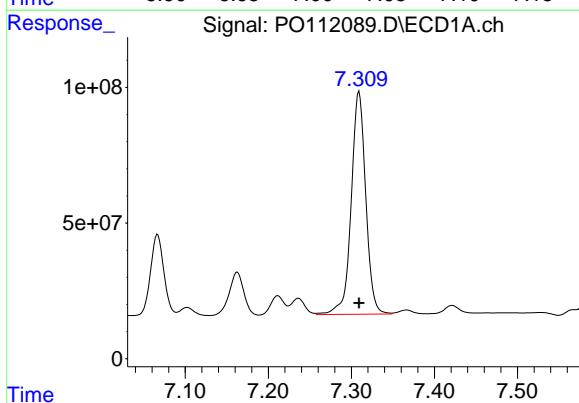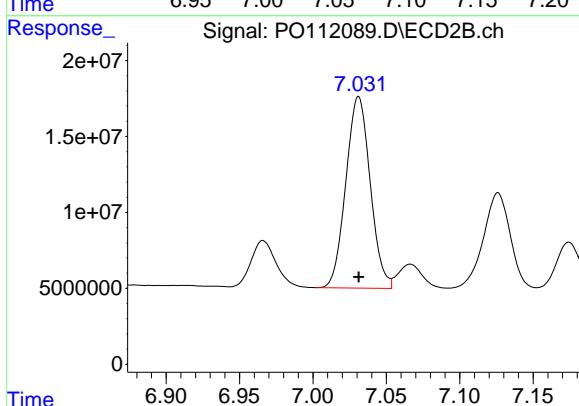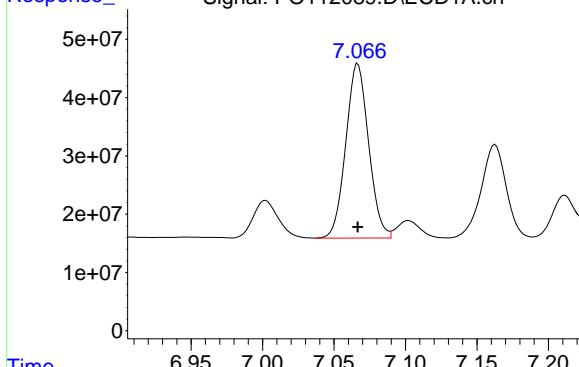

#34 AR-1260-4

R.T.: 7.031 min
 Delta R.T.: 0.000 min
 Response: 145778050
 Conc: 743.95 ng/ml

#35 AR-1260-5

R.T.: 7.309 min
 Delta R.T.: 0.000 min
 Response: 1000222126
 Conc: 749.02 ng/ml

#35 AR-1260-5

R.T.: 7.273 min
 Delta R.T.: 0.000 min
 Response: 336387510
 Conc: 750.94 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0070825\
 Data File : P0112090.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jul 2025 14:43
 Operator : YP/AJ
 Sample : AR1660ICC500
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1660ICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 08 15:07:25 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 08 15:05:13 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	3.673	3.684	525.7E6	341.2E6	50.000	50.000
2) SA Decachlor...	8.703	8.668	359.1E6	89500378	50.000	50.000

Target Compounds

3) L1 AR-1016-1	4.761	4.761	179.3E6	114.9E6	500.000	500.000
4) L1 AR-1016-2	4.780	4.779	263.6E6	170.4E6	500.000	500.000
5) L1 AR-1016-3	4.836	4.954	167.5E6	88755203	500.000	500.000
6) L1 AR-1016-4	4.956	4.997	134.5E6	70348152	500.000	500.000
7) L1 AR-1016-5	5.213	5.209	140.2E6	91687095	500.000	500.000
31) L7 AR-1260-1	6.251	6.238	262.3E6	142.2E6	500.000	500.000
32) L7 AR-1260-2	6.441	6.426	381.5E6	172.5E6	500.000	500.000
33) L7 AR-1260-3	6.807	6.578	348.6E6	146.6E6	500.000	500.000
34) L7 AR-1260-4	7.067	7.048	228.8E6	101.6E6	500.000	500.000
35) L7 AR-1260-5	7.309	7.290	658.6E6	228.0E6	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0070825\
 Data File : P0112090.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jul 2025 14:43
 Operator : YP/AJ
 Sample : AR1660ICC500
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_O
ClientSampleId :
 AR1660ICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 08 15:07:25 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 08 15:05:13 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

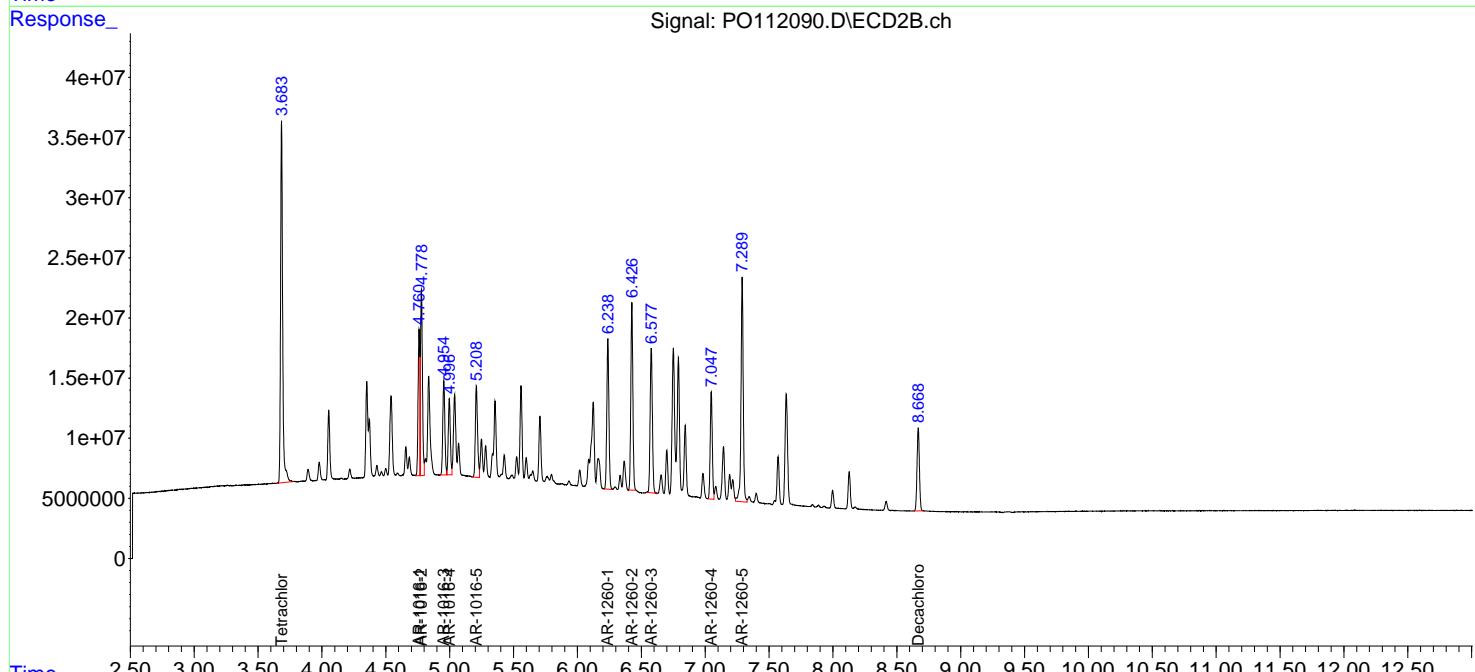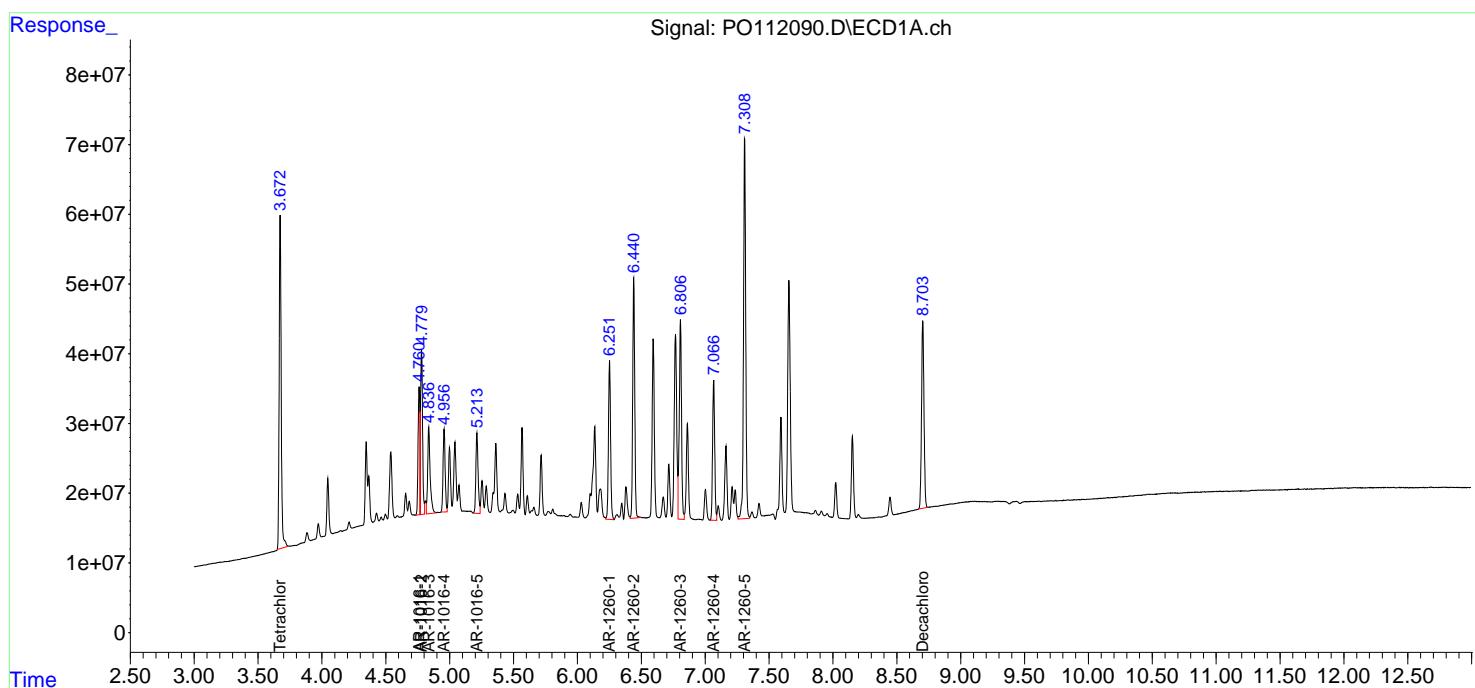

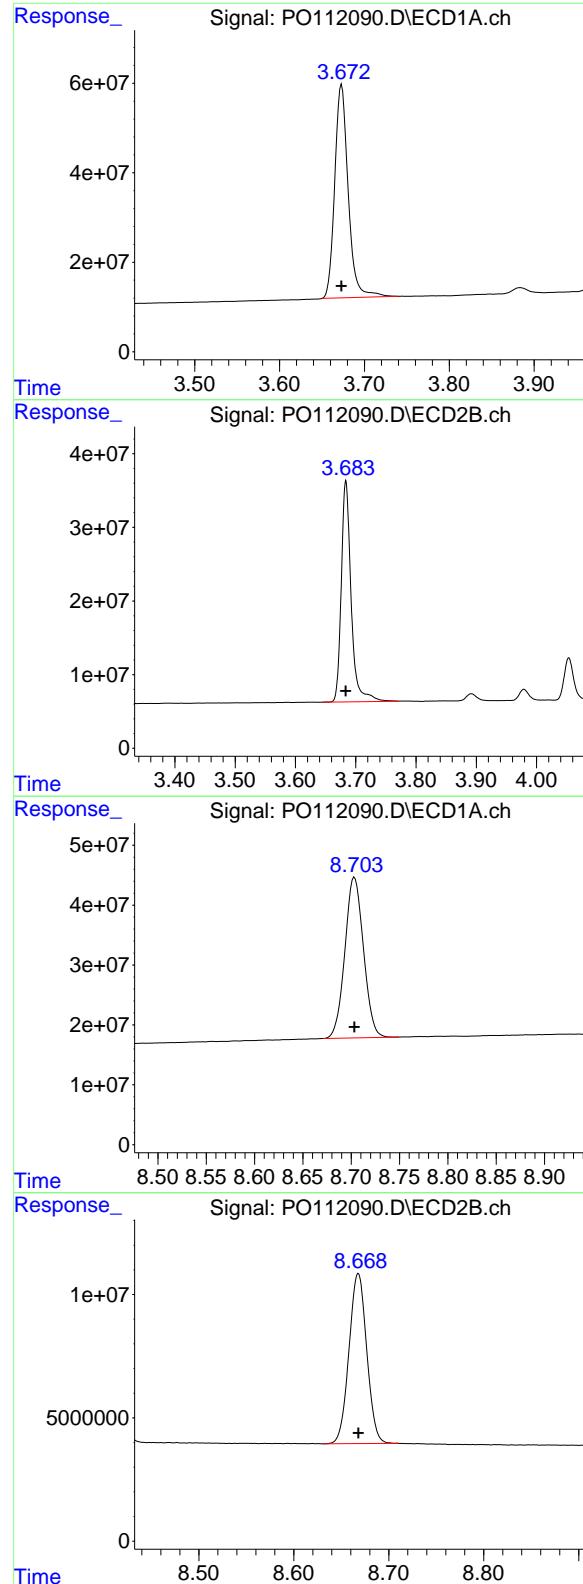

#1 Tetrachloro-m-xylene

R.T.: 3.673 min
Delta R.T.: 0.000 min
Response: 525664563
Conc: 50.00 ng/ml

Instrument:

ECD_O

ClientSampleId :

AR1660ICC500

#1 Tetrachloro-m-xylene


R.T.: 3.684 min
Delta R.T.: 0.000 min
Response: 341192636
Conc: 50.00 ng/ml

#2 Decachlorobiphenyl

R.T.: 8.703 min
Delta R.T.: 0.000 min
Response: 359131525
Conc: 50.00 ng/ml

#2 Decachlorobiphenyl

R.T.: 8.668 min
Delta R.T.: 0.000 min
Response: 89500378
Conc: 50.00 ng/ml

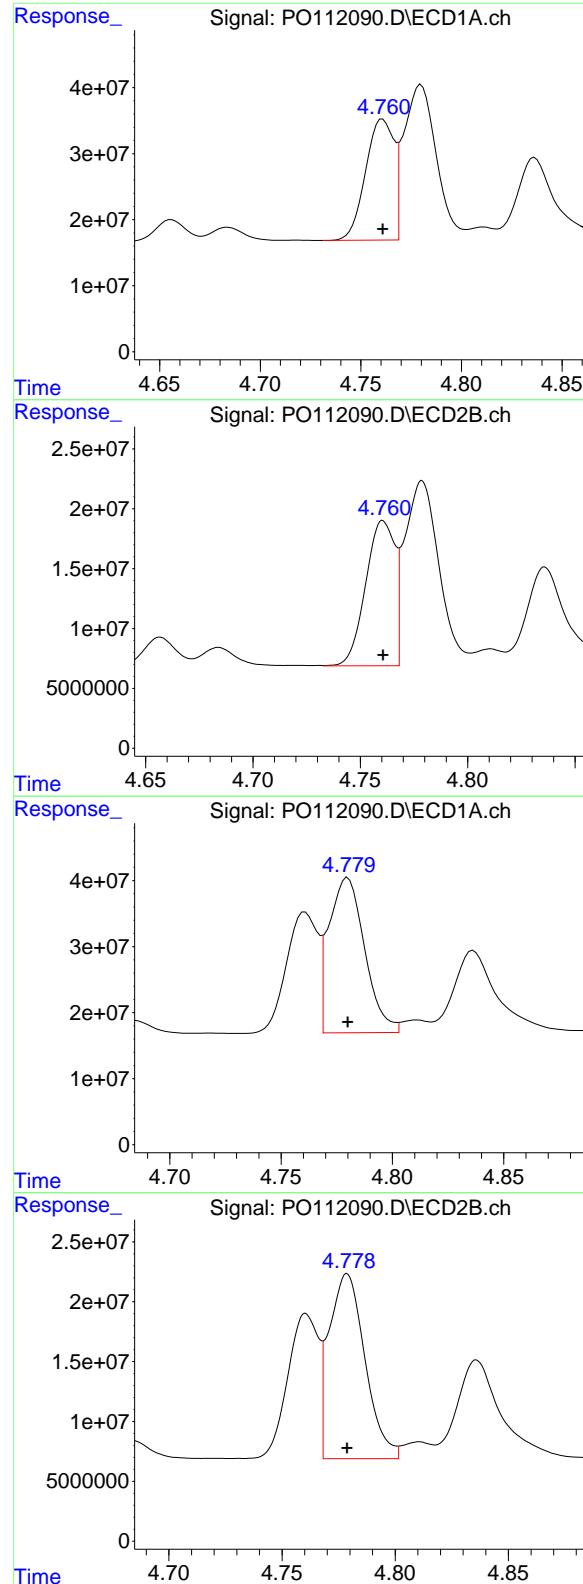

#3 AR-1016-1

R.T.: 4.761 min
 Delta R.T.: 0.000 min
 Response: 179304039
 Conc: 500.00 ng/ml

Instrument: ECD_O
ClientSampleId: AR1660ICC500

#3 AR-1016-1

R.T.: 4.761 min
 Delta R.T.: 0.000 min
 Response: 114927870
 Conc: 500.00 ng/ml

#4 AR-1016-2

R.T.: 4.780 min
 Delta R.T.: 0.000 min
 Response: 263643129
 Conc: 500.00 ng/ml





#4 AR-1016-2

R.T.: 4.779 min
 Delta R.T.: 0.000 min
 Response: 170358287
 Conc: 500.00 ng/ml

#5 AR-1016-3

R.T.: 4.836 min
 Delta R.T.: 0.000 min
 Response: 167495186
 Conc: 500.00 ng/ml

Instrument: ECD_O
ClientSampleId: AR1660ICC500

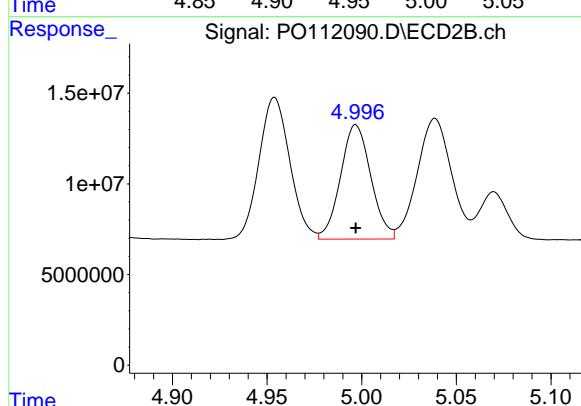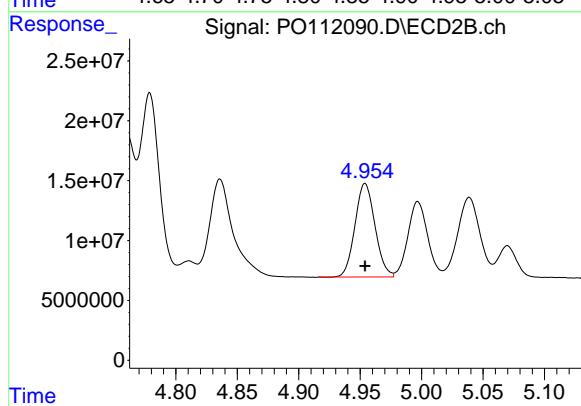

#5 AR-1016-3


R.T.: 4.954 min
 Delta R.T.: 0.000 min
 Response: 88755203
 Conc: 500.00 ng/ml

#6 AR-1016-4

R.T.: 4.956 min
 Delta R.T.: 0.000 min
 Response: 134519633
 Conc: 500.00 ng/ml

#6 AR-1016-4

R.T.: 4.997 min
 Delta R.T.: 0.000 min
 Response: 70348152
 Conc: 500.00 ng/ml

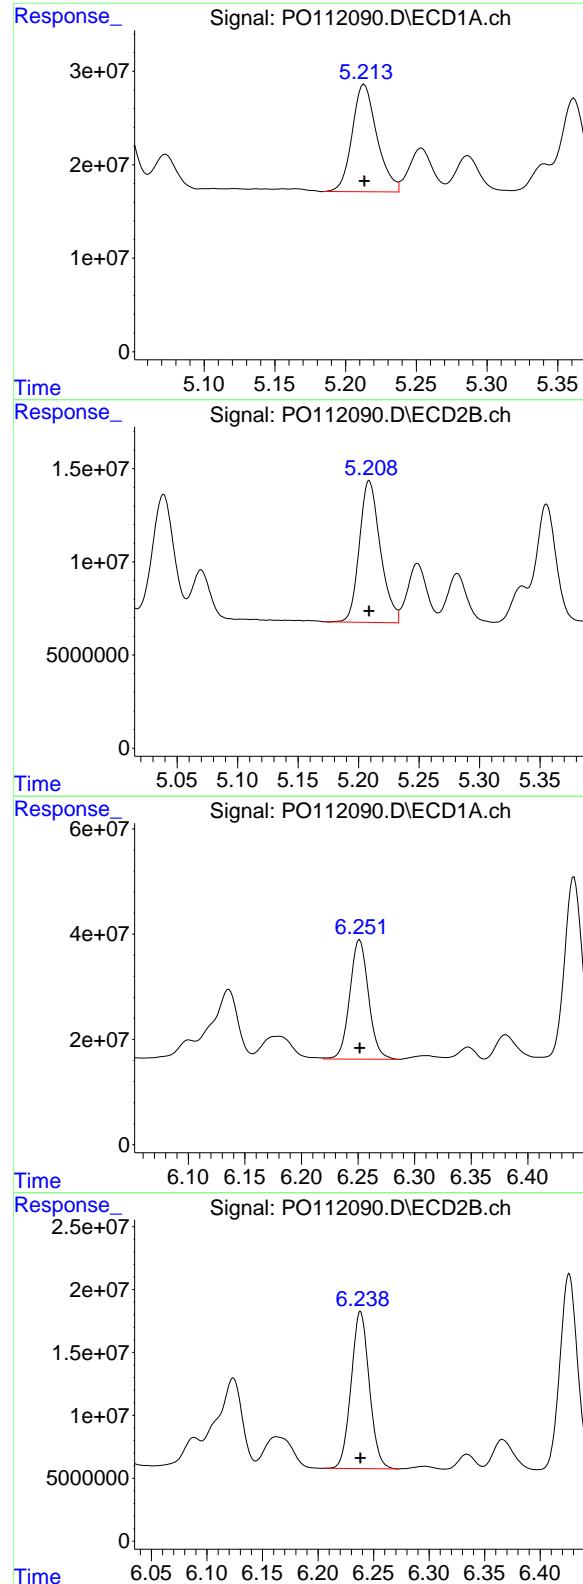

#7 AR-1016-5

R.T.: 5.213 min
 Delta R.T.: 0.000 min
 Response: 140223352
 Conc: 500.00 ng/ml

Instrument: ECD_O
ClientSampleId: AR1660ICC500

#7 AR-1016-5

R.T.: 5.209 min
 Delta R.T.: 0.000 min
 Response: 91687095
 Conc: 500.00 ng/ml

#31 AR-1260-1

R.T.: 6.251 min
 Delta R.T.: 0.000 min
 Response: 262264034
 Conc: 500.00 ng/ml





#31 AR-1260-1

R.T.: 6.238 min
 Delta R.T.: 0.000 min
 Response: 142198185
 Conc: 500.00 ng/ml

#32 AR-1260-2

R.T.: 6.441 min
 Delta R.T.: 0.000 min
 Response: 381541844
 Conc: 500.00 ng/ml

Instrument: ECD_O
ClientSampleId: AR1660ICC500

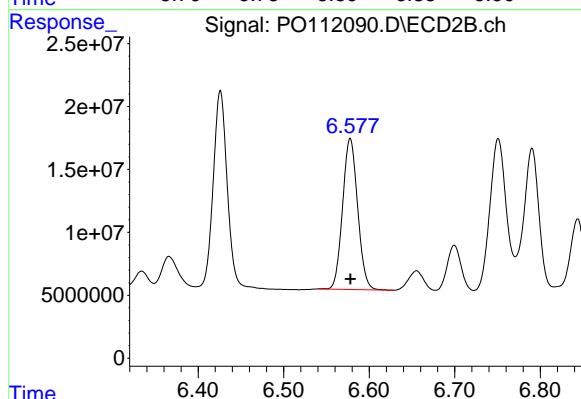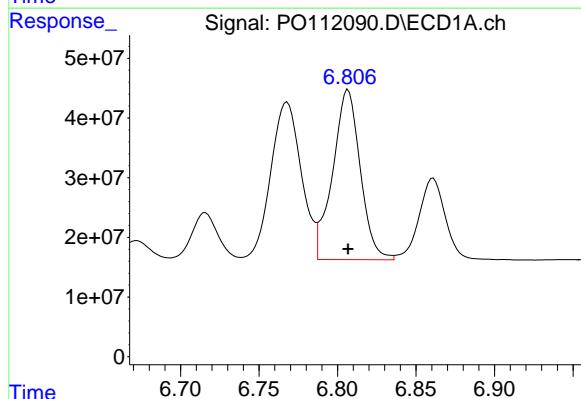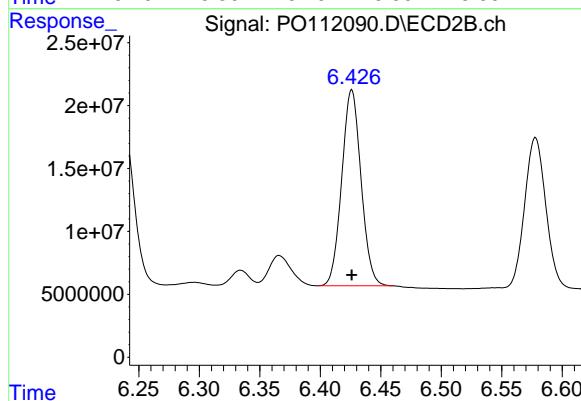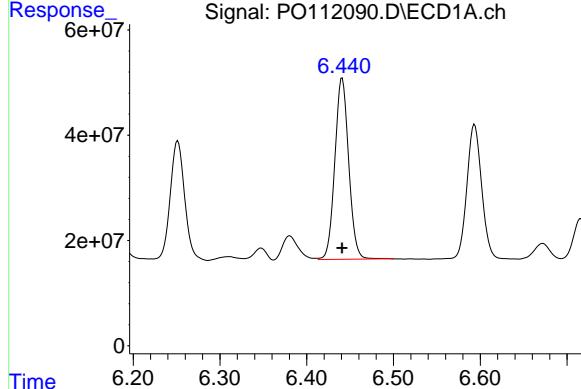

#32 AR-1260-2

R.T.: 6.426 min
 Delta R.T.: 0.000 min
 Response: 172549408
 Conc: 500.00 ng/ml

#33 AR-1260-3

R.T.: 6.807 min
 Delta R.T.: 0.000 min
 Response: 348566351
 Conc: 500.00 ng/ml


#33 AR-1260-3

R.T.: 6.578 min
 Delta R.T.: 0.000 min
 Response: 146577768
 Conc: 500.00 ng/ml

#34 AR-1260-4


R.T.: 7.067 min
 Delta R.T.: 0.000 min
 Response: 228751380
 Conc: 500.00 ng/ml

Instrument: ECD_O
ClientSampleId: AR1660ICC500

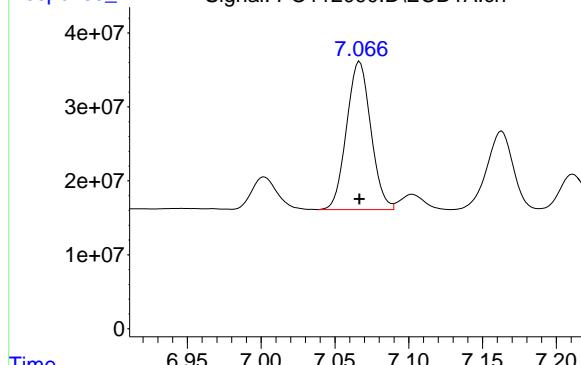


#34 AR-1260-4

R.T.: 7.048 min
 Delta R.T.: 0.000 min
 Response: 101583197
 Conc: 500.00 ng/ml

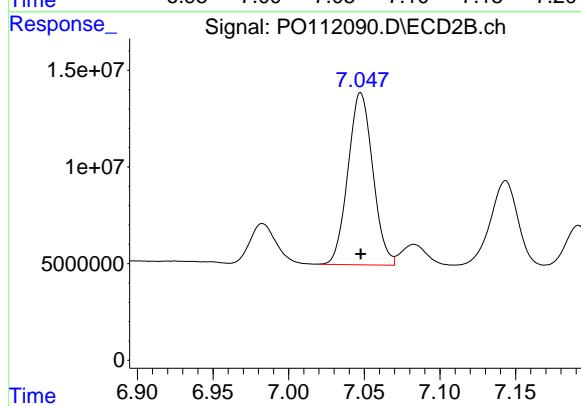


#35 AR-1260-5

R.T.: 7.309 min
 Delta R.T.: 0.000 min
 Response: 658599875
 Conc: 500.00 ng/ml



#35 AR-1260-5

R.T.: 7.290 min
 Delta R.T.: 0.000 min
 Response: 227956292
 Conc: 500.00 ng/ml

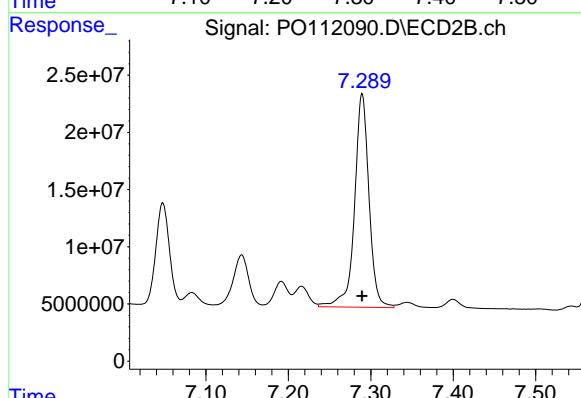

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0070825\
 Data File : P0112091.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jul 2025 15:02
 Operator : YP/AJ
 Sample : AR1660ICC250
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1660ICC250

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/09/2025
 Supervised By :mohammad ahmed 07/10/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 08 15:21:22 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 08 15:05:13 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	3.674	3.666	254.6E6	166.5E6	24.239	24.620m
2) SA Decachlor...	8.704	8.650	182.1E6	46559399	25.379	26.170m

Target Compounds

3) L1 AR-1016-1	4.762	4.743	87952907	58858758	246.959	258.385
4) L1 AR-1016-2	4.780	4.762	131.2E6	86217779	251.058	255.039
5) L1 AR-1016-3	4.838	4.937	85456999	43830930	256.116	251.057
6) L1 AR-1016-4	4.957	4.979	66370456	35386243	249.234	257.115
7) L1 AR-1016-5	5.214	5.192	71497345	44870816	255.385	251.028
31) L7 AR-1260-1	6.251	6.221	131.2E6	79739924	253.320m	276.656
32) L7 AR-1260-2	6.441	6.409	185.2E6	91585006	246.068m	263.404
33) L7 AR-1260-3	6.807	6.561	161.9E6	73700907	238.590m	254.910m
34) L7 AR-1260-4	7.066	7.031	115.3E6	54771859	256.248m	271.502
35) L7 AR-1260-5	7.309	7.272	324.7E6	120.8E6	242.889m	264.490

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0070825\
 Data File : P0112091.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jul 2025 15:02
 Operator : YP/AJ
 Sample : AR1660ICC250
 Misc :
 ALS Vial : 6 Sample Multiplier: 1



Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 08 15:21:22 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 08 15:05:13 2025
 Response via : Initial Calibration
 Integrator: ChemStation


Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Instrument :
 ECD_O
ClientSampleId :
 AR1660ICC250

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/09/2025
 Supervised By :mohammad ahmed 07/10/2025

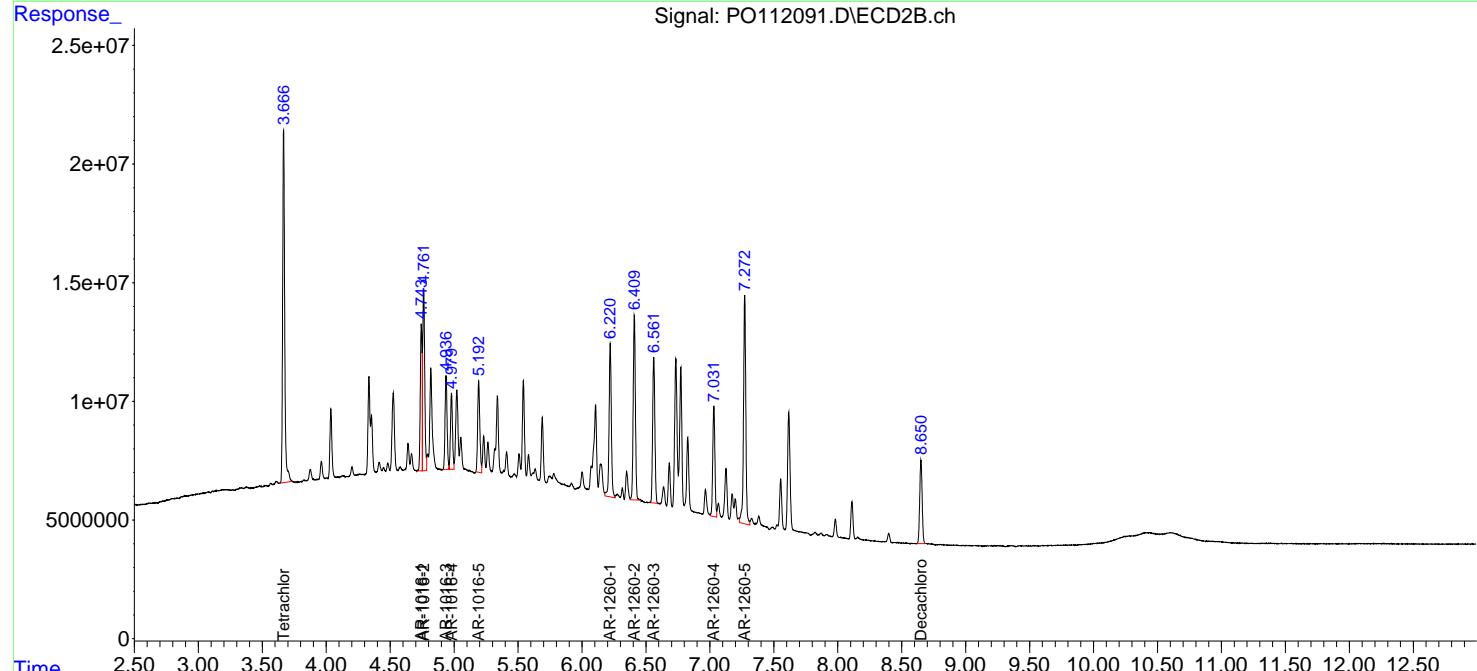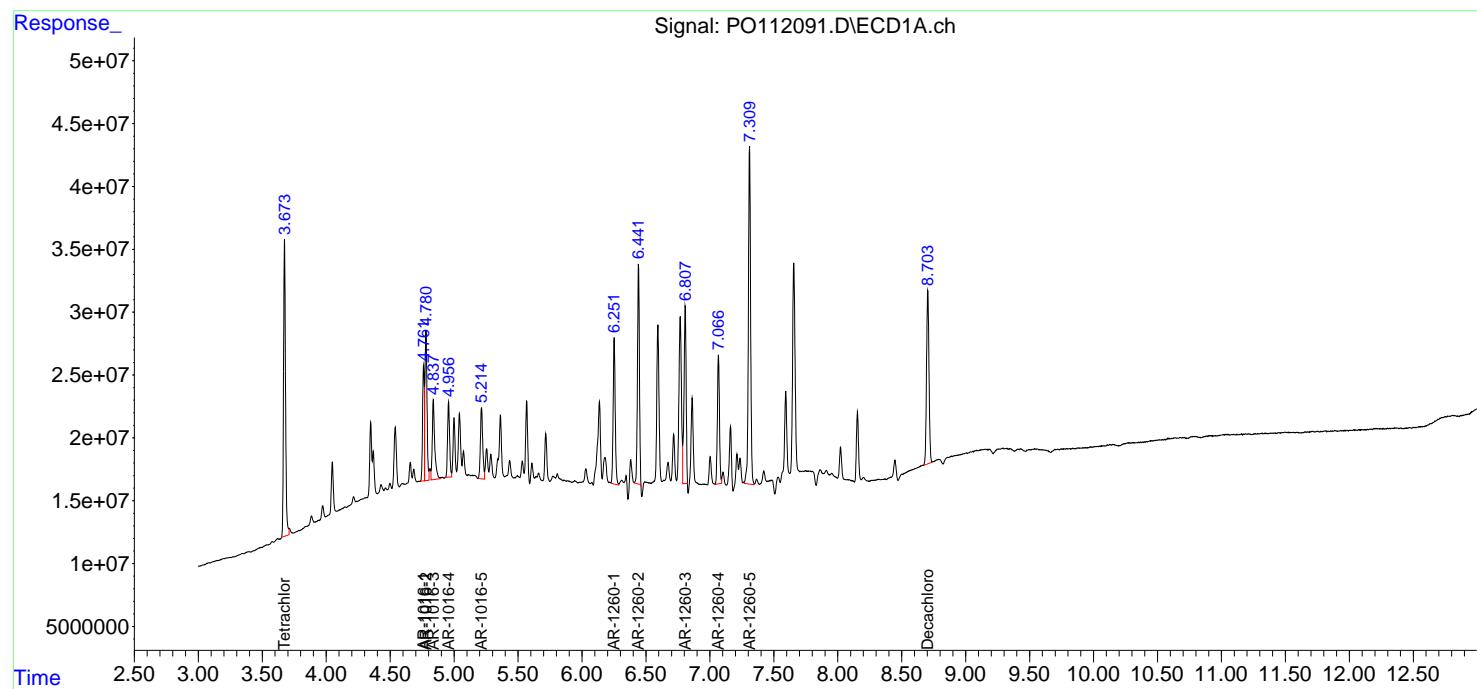

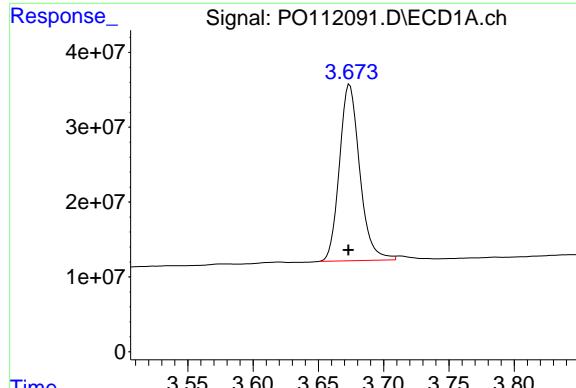

#1 Tetrachloro-m-xylene

R.T.: 3.674 min

Delta R.T.: 0.000 min

Response: 254587950

Conc: 24.24 ng/ml

Instrument:

ECD_O


ClientSampleId :

AR1660ICC250

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/09/2025

Supervised By :mohammad ahmed 07/10/2025

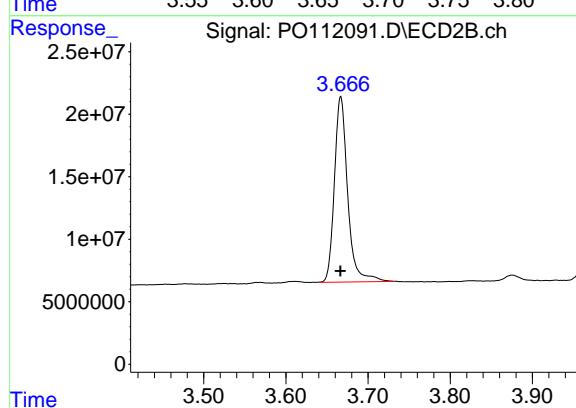


#1 Tetrachloro-m-xylene

R.T.: 3.666 min

Delta R.T.: 0.000 min

Response: 166509133

Conc: 24.62 ng/ml m

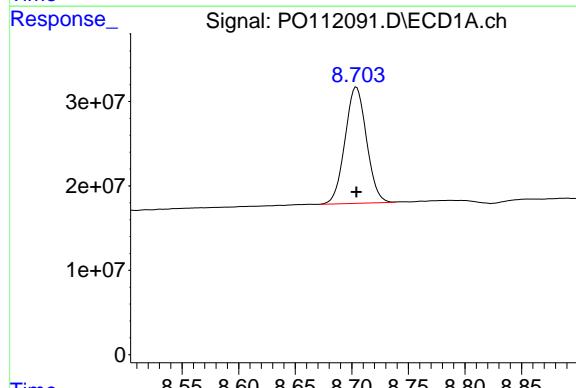


#2 Decachlorobiphenyl

R.T.: 8.704 min

Delta R.T.: 0.000 min

Response: 182135512

Conc: 25.38 ng/ml

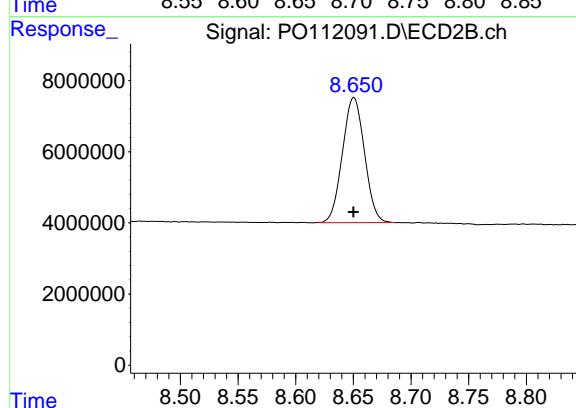

#2 Decachlorobiphenyl

R.T.: 8.650 min

Delta R.T.: 0.000 min

Response: 46559399

Conc: 26.17 ng/ml m





#3 AR-1016-1

R.T.: 4.762 min
 Delta R.T.: 0.000 min
 Response: 87952907
 Conc: 246.96 ng/ml

Instrument: ECD_O
ClientSampleId: AR1660ICC250

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/09/2025
 Supervised By :mohammad ahmed 07/10/2025

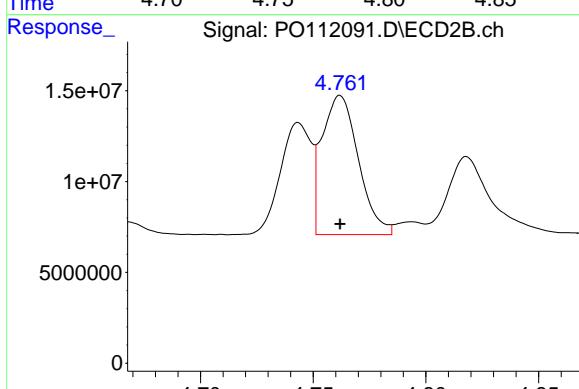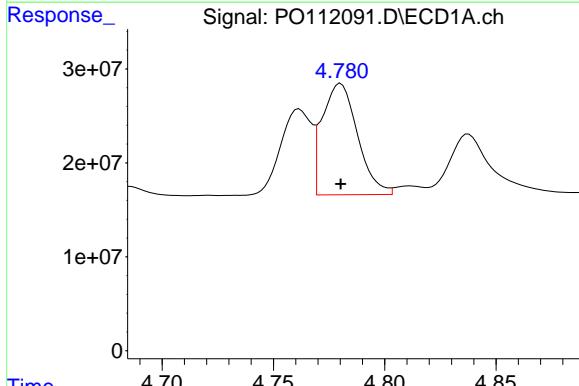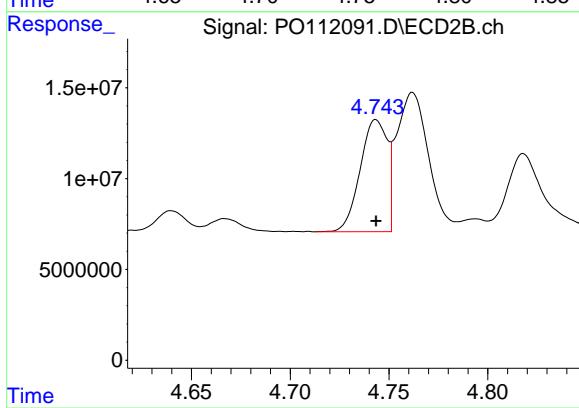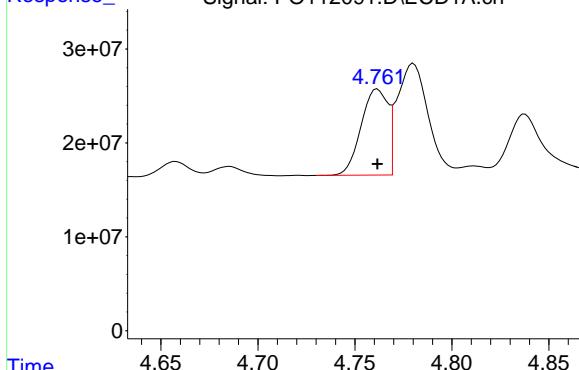

#3 AR-1016-1

R.T.: 4.743 min
 Delta R.T.: 0.000 min
 Response: 58858758
 Conc: 258.39 ng/ml

#4 AR-1016-2

R.T.: 4.780 min
 Delta R.T.: 0.000 min
 Response: 131218582
 Conc: 251.06 ng/ml

#4 AR-1016-2

R.T.: 4.762 min
 Delta R.T.: 0.000 min
 Response: 86217779
 Conc: 255.04 ng/ml





#5 AR-1016-3

R.T.: 4.838 min
 Delta R.T.: 0.000 min
 Response: 85456999
 Conc: 256.12 ng/ml

Instrument: ECD_O
ClientSampleId: AR1660ICC250

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/09/2025
 Supervised By :mohammad ahmed 07/10/2025

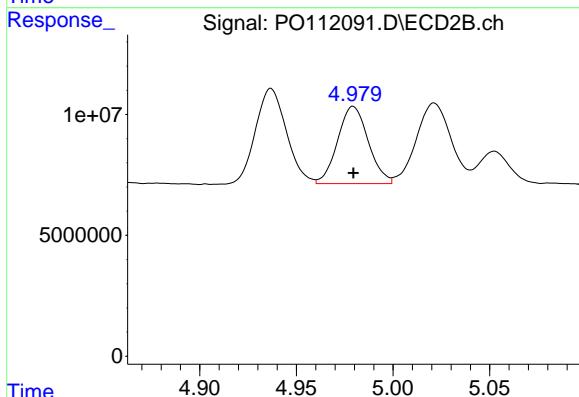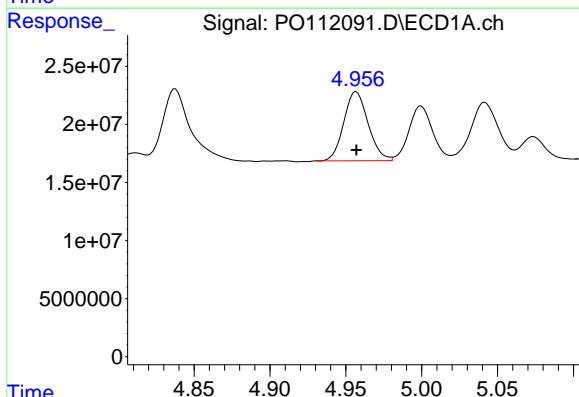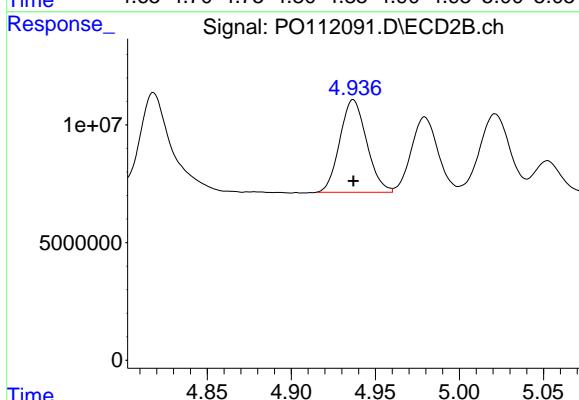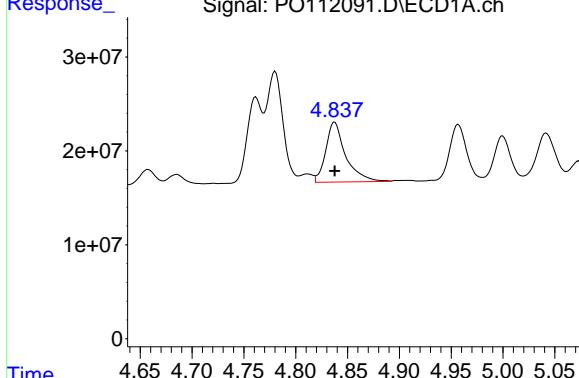

#5 AR-1016-3

R.T.: 4.937 min
 Delta R.T.: 0.000 min
 Response: 43830930
 Conc: 251.06 ng/ml

#6 AR-1016-4

R.T.: 4.957 min
 Delta R.T.: 0.000 min
 Response: 66370456
 Conc: 249.23 ng/ml

#6 AR-1016-4

R.T.: 4.979 min
 Delta R.T.: 0.000 min
 Response: 35386243
 Conc: 257.11 ng/ml

#7 AR-1016-5

R.T.: 5.214 min
 Delta R.T.: 0.000 min
 Response: 71497345
 Conc: 255.39 ng/ml

Instrument: ECD_O
ClientSampleId: AR1660ICC250

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/09/2025
 Supervised By :mohammad ahmed 07/10/2025

#7 AR-1016-5





R.T.: 5.192 min
 Delta R.T.: 0.000 min
 Response: 44870816
 Conc: 251.03 ng/ml


#31 AR-1260-1

R.T.: 6.251 min
 Delta R.T.: 0.000 min
 Response: 131230582
 Conc: 253.32 ng/ml

#31 AR-1260-1

R.T.: 6.221 min
 Delta R.T.: 0.000 min
 Response: 79739924
 Conc: 276.66 ng/ml

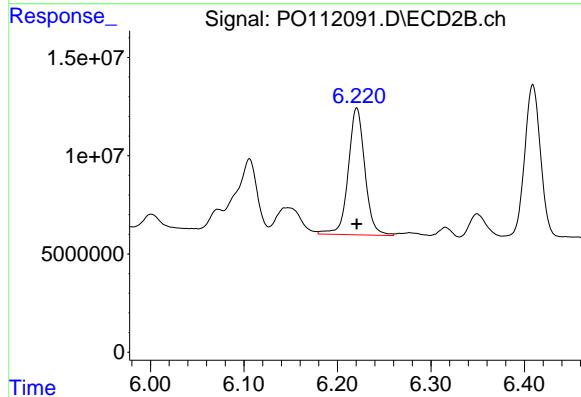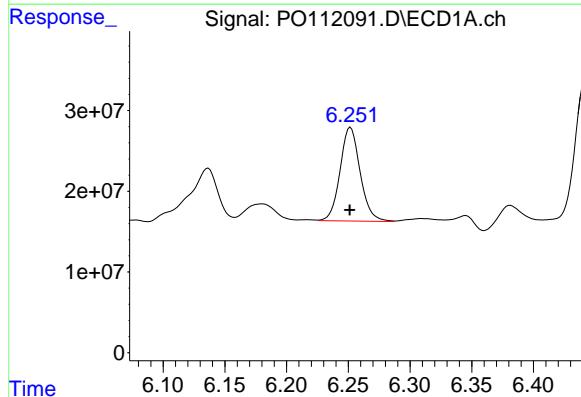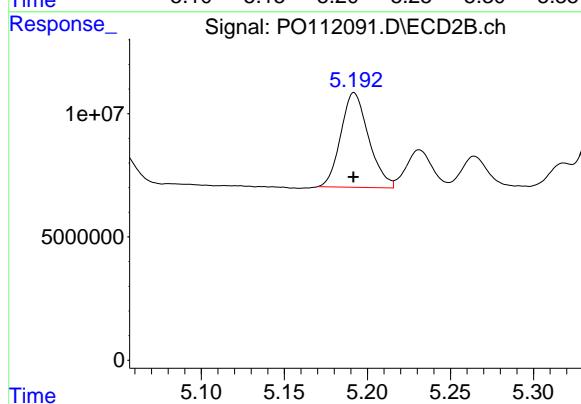

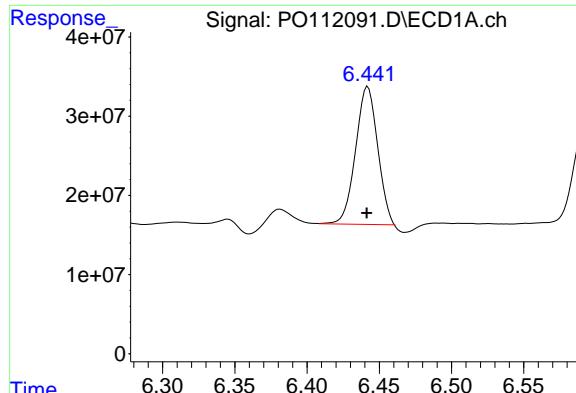


#32 AR-1260-2

R.T.: 6.441 min
Delta R.T.: 0.000 min
Response: 185229581
Conc: 246.07 ng/ml

Instrument: ECD_O
ClientSampleId: AR1660ICC250

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/09/2025
Supervised By :mohammad ahmed 07/10/2025

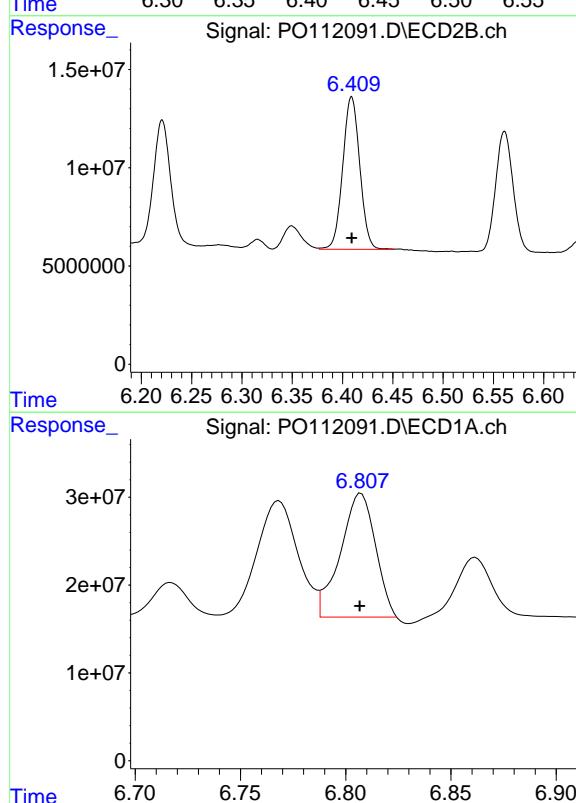

#33 AR-1260-3

R.T.: 6.807 min
Delta R.T.: 0.000 min
Response: 161896109
Conc: 238.59 ng/ml

#33 AR-1260-3

R.T.: 6.561 min
Delta R.T.: 0.000 min
Response: 73700907
Conc: 254.91 ng/ml

#34 AR-1260-4

R.T.: 7.066 min
 Delta R.T.: 0.000 min
 Response: 115279593
 Conc: 256.25 ng/ml

Instrument: ECD_O
ClientSampleId: AR1660ICC250

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/09/2025
 Supervised By :mohammad ahmed 07/10/2025

#34 AR-1260-4


R.T.: 7.031 min
 Delta R.T.: 0.000 min
 Response: 54771859
 Conc: 271.50 ng/ml

#35 AR-1260-5

R.T.: 7.309 min
 Delta R.T.: 0.000 min
 Response: 324723025
 Conc: 242.89 ng/ml

#35 AR-1260-5

R.T.: 7.272 min
 Delta R.T.: 0.000 min
 Response: 120812819
 Conc: 264.49 ng/ml

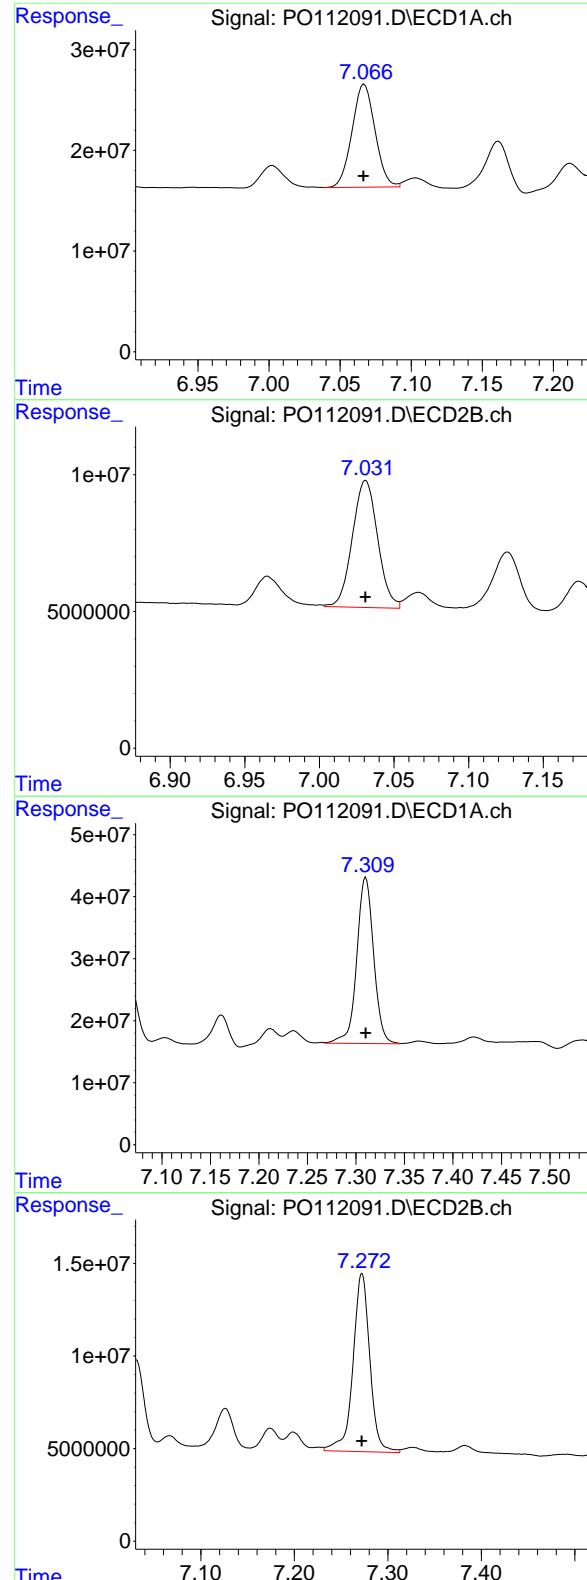

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0070825\
 Data File : P0112092.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jul 2025 15:21
 Operator : YP/AJ
 Sample : AR1660ICC050
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1660ICC050

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/09/2025
 Supervised By :mohammad ahmed 07/10/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 08 15:36:17 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 08 15:36:04 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	3.673	3.666	37442397	24163066	3.784	3.793
2) SA Decachlor...	8.703	8.650	27391770	7510514	4.006	4.354m

Target Compounds

3) L1 AR-1016-1	4.761	4.743	13802015	10149679	40.580	45.548
4) L1 AR-1016-2	4.780	4.761	19790298	14662938	39.796	44.555
5) L1 AR-1016-3	4.836	4.936	14195524	7549659	43.852	44.445
6) L1 AR-1016-4	4.956	4.979	10940244	6781238	42.602	49.416
7) L1 AR-1016-5	5.211	5.191	12423751	7528374	45.100m	43.655
31) L7 AR-1260-1	6.250	6.220	21371774	12495016	42.836m	44.579m
32) L7 AR-1260-2	6.440	6.408	33970556	15459479	46.386m	45.388m
33) L7 AR-1260-3	6.806	6.559	29007819	11088040	44.254	40.234
34) L7 AR-1260-4	7.066	7.030	19317003	9814007	44.382	48.912
35) L7 AR-1260-5	7.309	7.272	50382935	20576692	39.906	45.958

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0070825\
 Data File : P0112092.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jul 2025 15:21
 Operator : YP/AJ
 Sample : AR1660ICC050
 Misc :
 ALS Vial : 7 Sample Multiplier: 1



Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 08 15:36:17 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 08 15:36:04 2025
 Response via : Initial Calibration
 Integrator: ChemStation


Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Instrument :
 ECD_O
ClientSampleId :
 AR1660ICC050

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/09/2025
 Supervised By :mohammad ahmed 07/10/2025

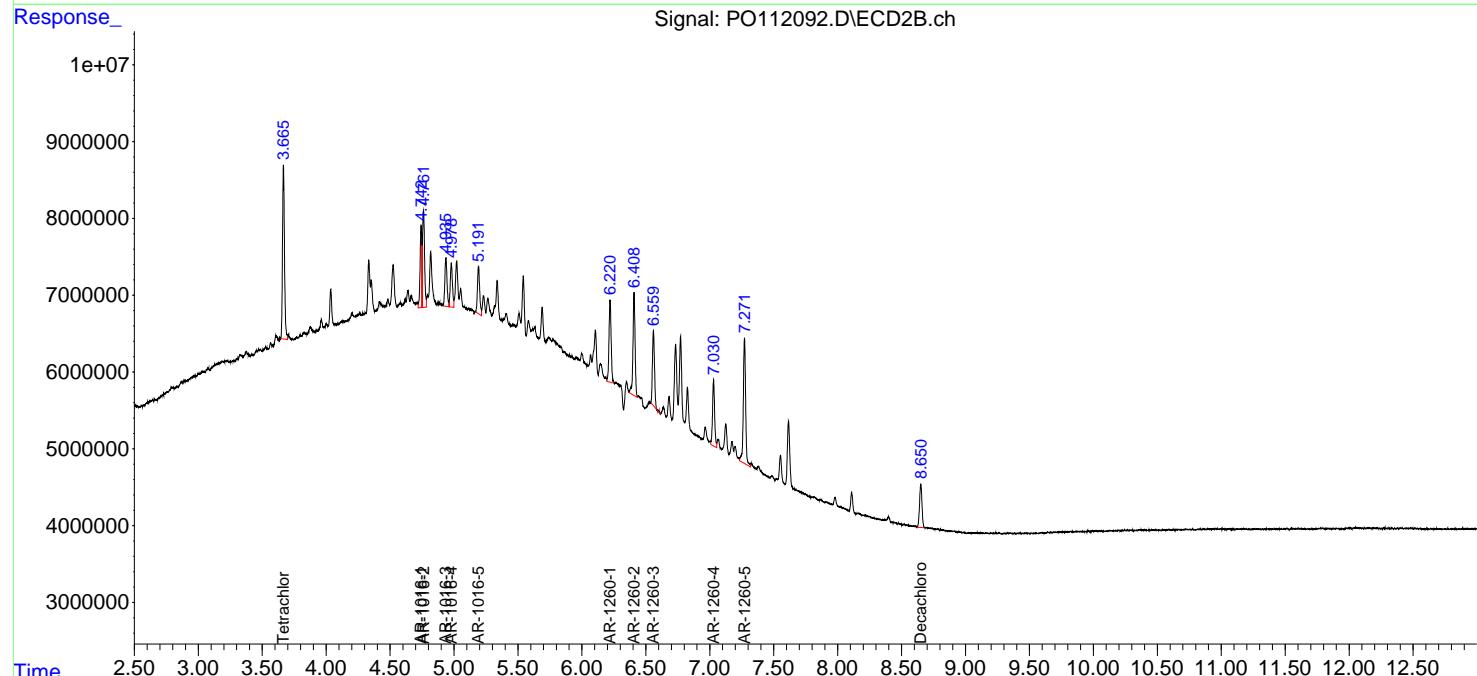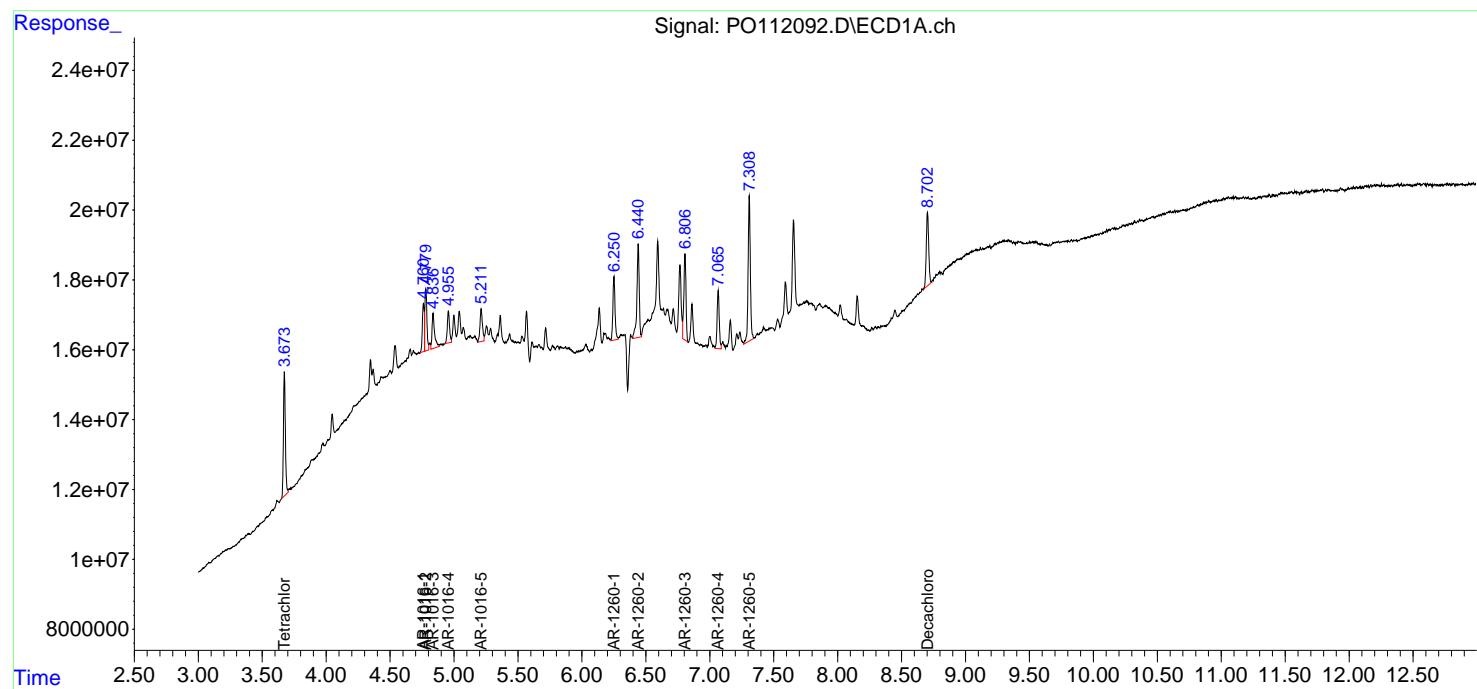

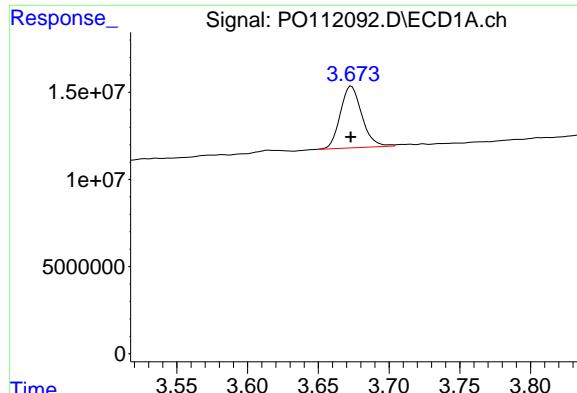


#1 Tetrachloro-m-xylene

R.T.: 3.673 min
Delta R.T.: 0.000 min
Response: 37442397
Conc: 3.78 ng/ml

Instrument: ECD_O
ClientSampleId: AR1660ICC050


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/09/2025
Supervised By :mohammad ahmed 07/10/2025

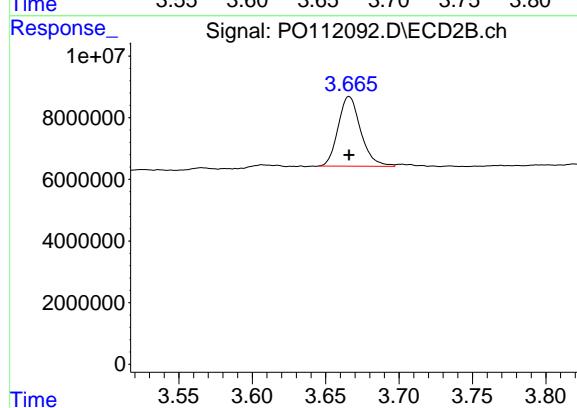


#1 Tetrachloro-m-xylene

R.T.: 3.666 min
Delta R.T.: 0.000 min
Response: 24163066
Conc: 3.79 ng/ml




#2 Decachlorobiphenyl

R.T.: 8.703 min
Delta R.T.: 0.000 min
Response: 27391770
Conc: 4.01 ng/ml

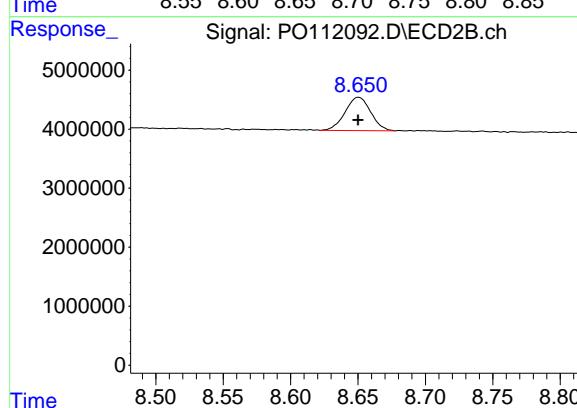

#2 Decachlorobiphenyl

R.T.: 8.650 min
Delta R.T.: 0.000 min
Response: 7510514
Conc: 4.35 ng/ml

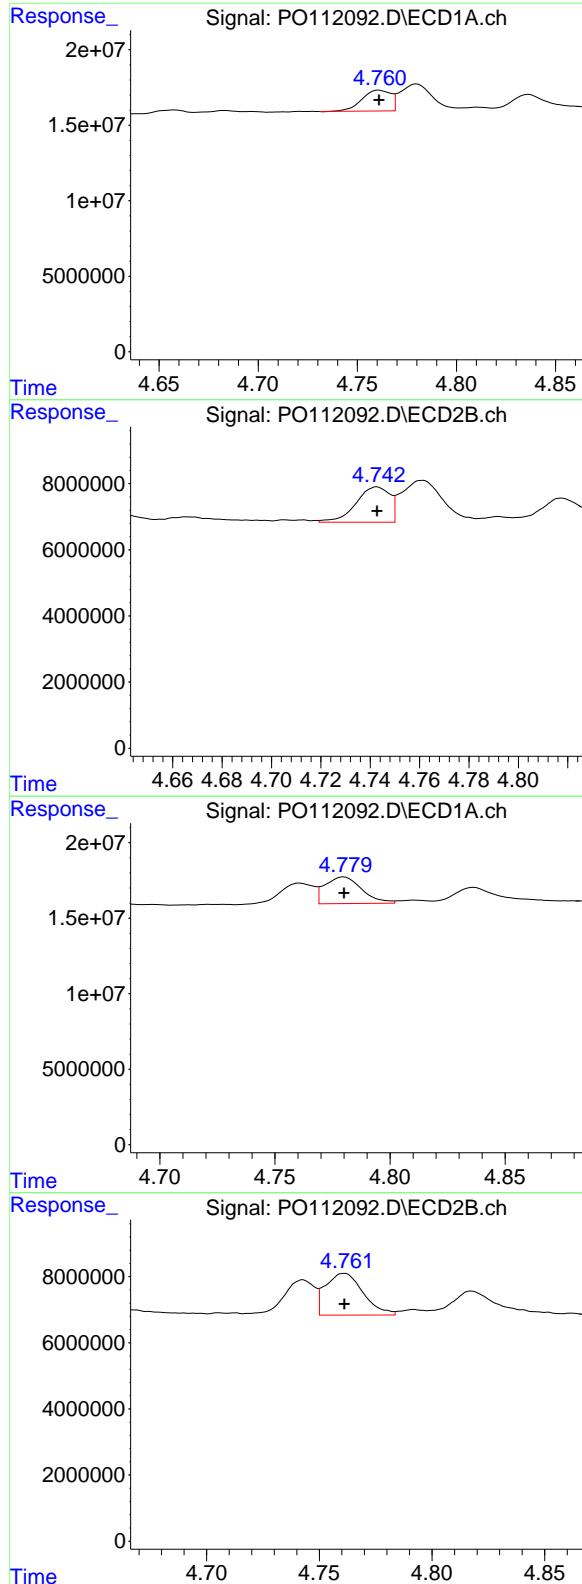

#3 AR-1016-1

R.T.: 4.761 min
 Delta R.T.: 0.000 min
 Response: 13802015
 Conc: 40.58 ng/ml

Instrument: ECD_O
ClientSampleId: AR1660ICC050

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/09/2025
 Supervised By :mohammad ahmed 07/10/2025

#3 AR-1016-1


R.T.: 4.743 min
 Delta R.T.: 0.000 min
 Response: 10149679
 Conc: 45.55 ng/ml

#4 AR-1016-2

R.T.: 4.780 min
 Delta R.T.: 0.000 min
 Response: 19790298
 Conc: 39.80 ng/ml

#4 AR-1016-2

R.T.: 4.761 min
 Delta R.T.: 0.000 min
 Response: 14662938
 Conc: 44.55 ng/ml

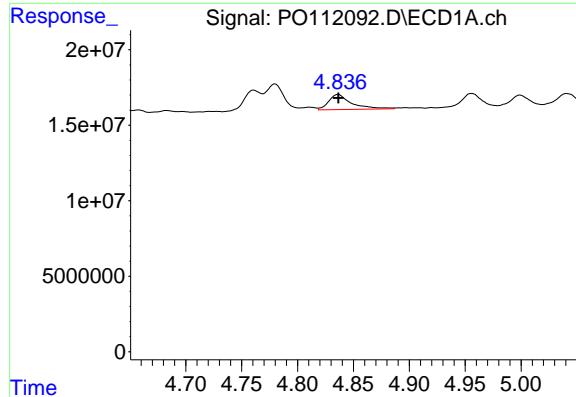


#5 AR-1016-3

R.T.: 4.836 min
Delta R.T.: 0.000 min
Response: 14195524
Conc: 43.85 ng/ml

Instrument: ECD_O
ClientSampleId: AR1660ICC050


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/09/2025
Supervised By :mohammad ahmed 07/10/2025

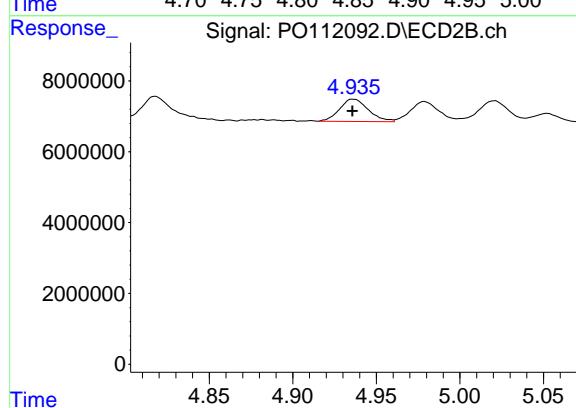


#5 AR-1016-3

R.T.: 4.936 min
Delta R.T.: 0.000 min
Response: 7549659
Conc: 44.44 ng/ml

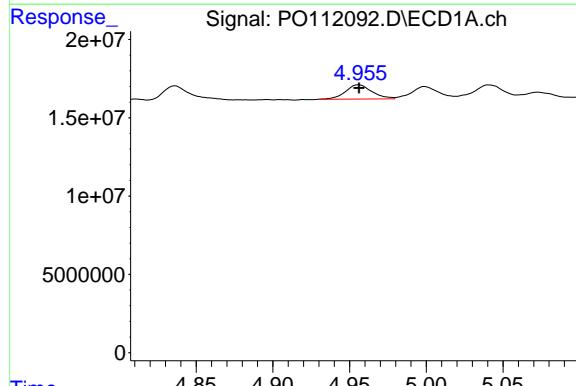


#6 AR-1016-4

R.T.: 4.956 min
Delta R.T.: 0.000 min
Response: 10940244
Conc: 42.60 ng/ml

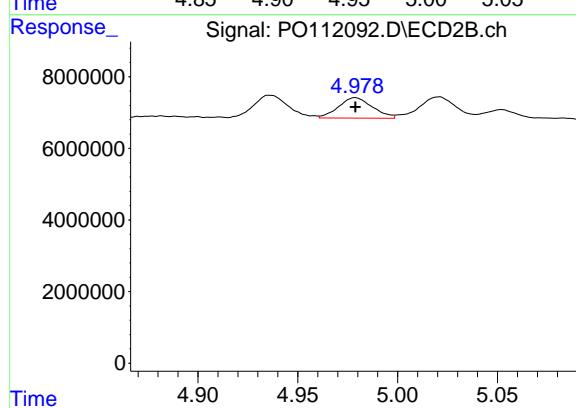

#6 AR-1016-4

R.T.: 4.979 min
Delta R.T.: 0.000 min
Response: 6781238
Conc: 49.42 ng/ml

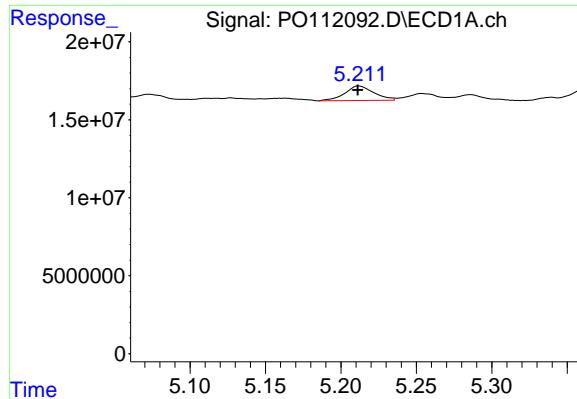


#7 AR-1016-5

R.T.: 5.211 min
Delta R.T.: 0.000 min
Response: 12423751
Conc: 45.10 ng/ml

Instrument: ECD_O
ClientSampleId: AR1660ICC050


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/09/2025
Supervised By :mohammad ahmed 07/10/2025

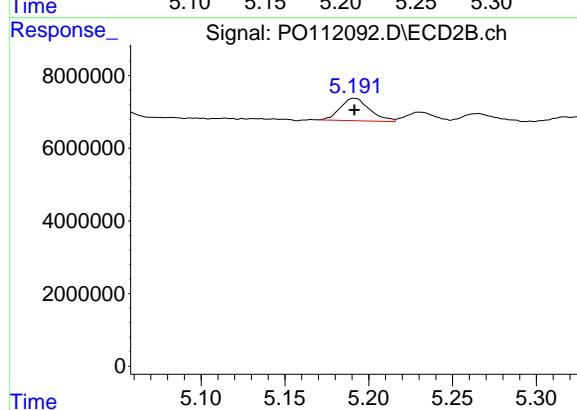


#7 AR-1016-5

R.T.: 5.191 min
Delta R.T.: 0.000 min
Response: 7528374
Conc: 43.66 ng/ml




#31 AR-1260-1

R.T.: 6.250 min
Delta R.T.: 0.000 min
Response: 21371774
Conc: 42.84 ng/ml

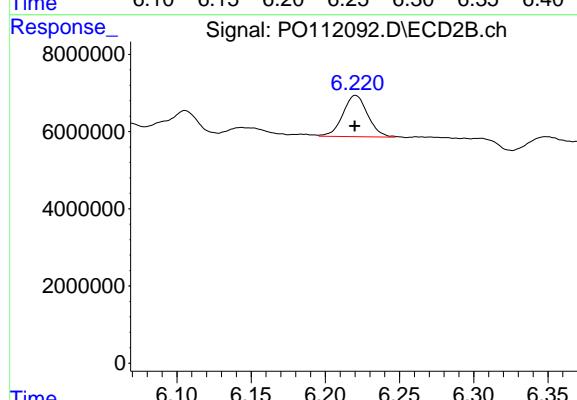

#31 AR-1260-1

R.T.: 6.220 min
Delta R.T.: 0.000 min
Response: 12495016
Conc: 44.58 ng/ml

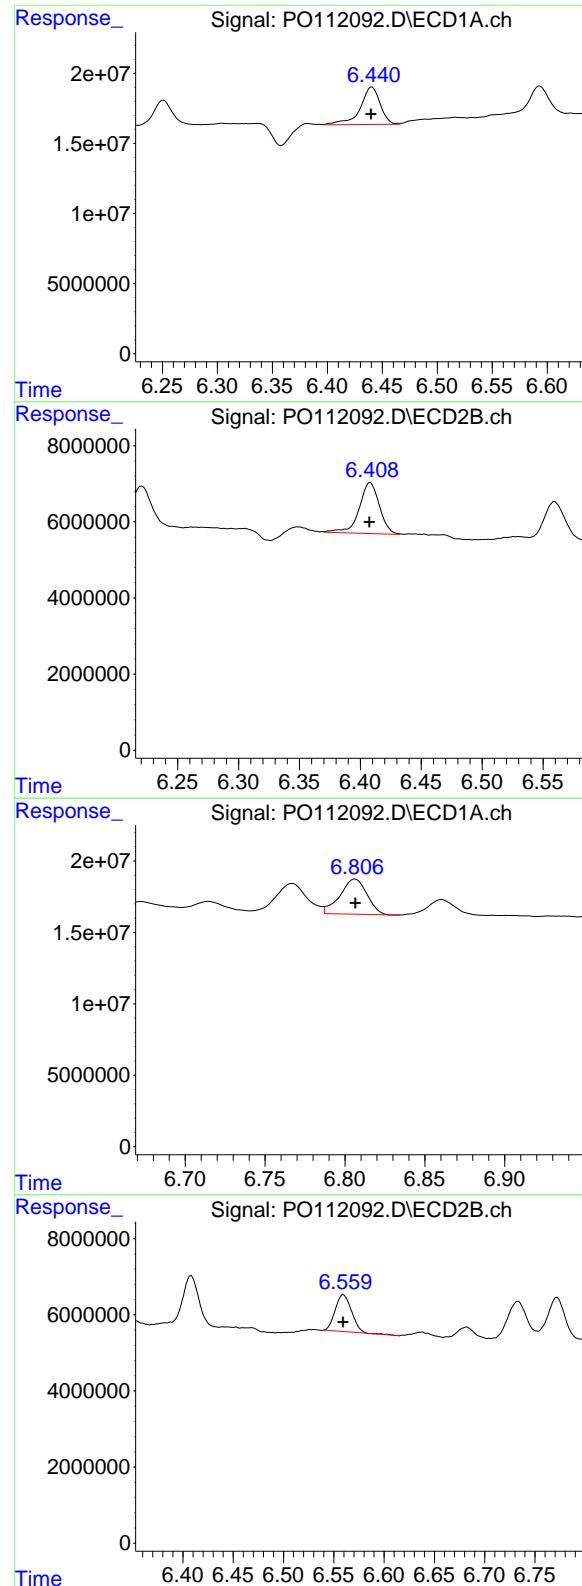

#32 AR-1260-2

R.T.: 6.440 min
 Delta R.T.: 0.000 min
 Response: 33970556
 Conc: 46.39 ng/ml

Instrument: ECD_O
ClientSampleId: AR1660ICC050

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/09/2025
 Supervised By :mohammad ahmed 07/10/2025

#32 AR-1260-2

R.T.: 6.408 min
 Delta R.T.: 0.000 min
 Response: 15459479
 Conc: 45.39 ng/ml

#33 AR-1260-3

R.T.: 6.806 min
 Delta R.T.: 0.000 min
 Response: 29007819
 Conc: 44.25 ng/ml

#33 AR-1260-3

R.T.: 6.559 min
 Delta R.T.: 0.000 min
 Response: 11088040
 Conc: 40.23 ng/ml

#34 AR-1260-4

R.T.: 7.066 min
 Delta R.T.: 0.000 min
 Response: 19317003
 Conc: 44.38 ng/ml

Instrument: ECD_O
ClientSampleId: AR1660ICC050

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/09/2025
 Supervised By :mohammad ahmed 07/10/2025

#34 AR-1260-4





R.T.: 7.030 min
 Delta R.T.: 0.000 min
 Response: 9814007
 Conc: 48.91 ng/ml

#35 AR-1260-5

R.T.: 7.309 min
 Delta R.T.: 0.000 min
 Response: 50382935
 Conc: 39.91 ng/ml

#35 AR-1260-5

R.T.: 7.272 min
 Delta R.T.: 0.000 min
 Response: 20576692
 Conc: 45.96 ng/ml

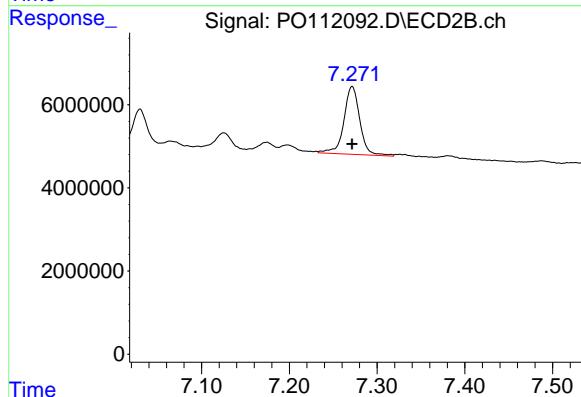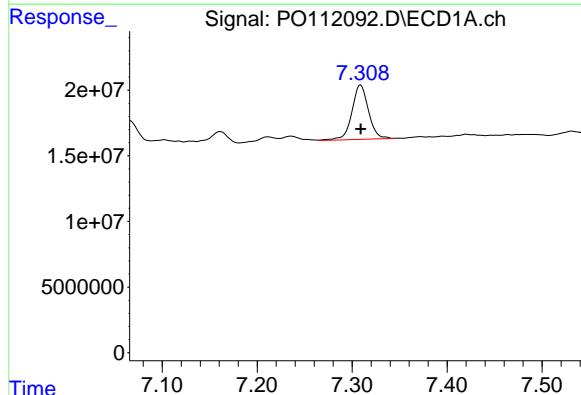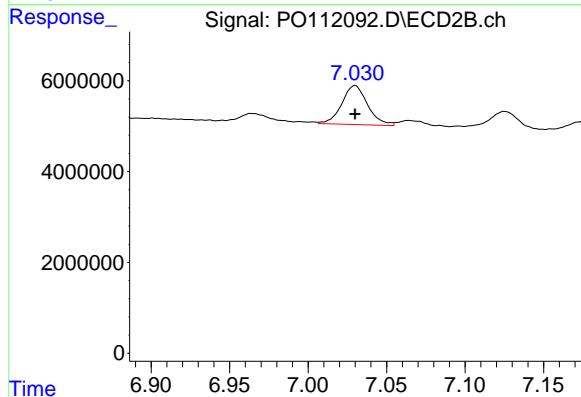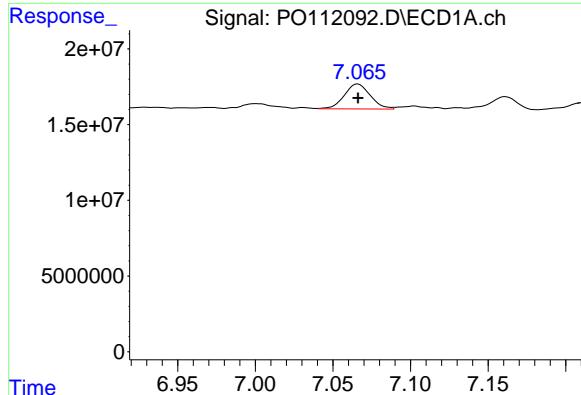

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0070825\
 Data File : P0112093.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jul 2025 15:38
 Operator : YP/AJ
 Sample : AR1221ICC500
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1221ICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 09 02:15:50 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 09 02:08:52 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	3.671	3.666	491.3E6	310.8E6	50.000	50.000
2) SA Decachlor...	8.701	8.649	354.6E6	89358669	50.000	50.000

Target Compounds

8) L2 AR-1221-1	3.883	3.875	58306973	41147512	500.000	500.000
9) L2 AR-1221-2	3.969	3.960	39420252	29676775	500.000	500.000
10) L2 AR-1221-3	4.045	4.036	134.8E6	94388324	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0070825\
 Data File : P0112093.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jul 2025 15:38
 Operator : YP/AJ
 Sample : AR1221ICC500
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1221ICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 09 02:15:50 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 09 02:08:52 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

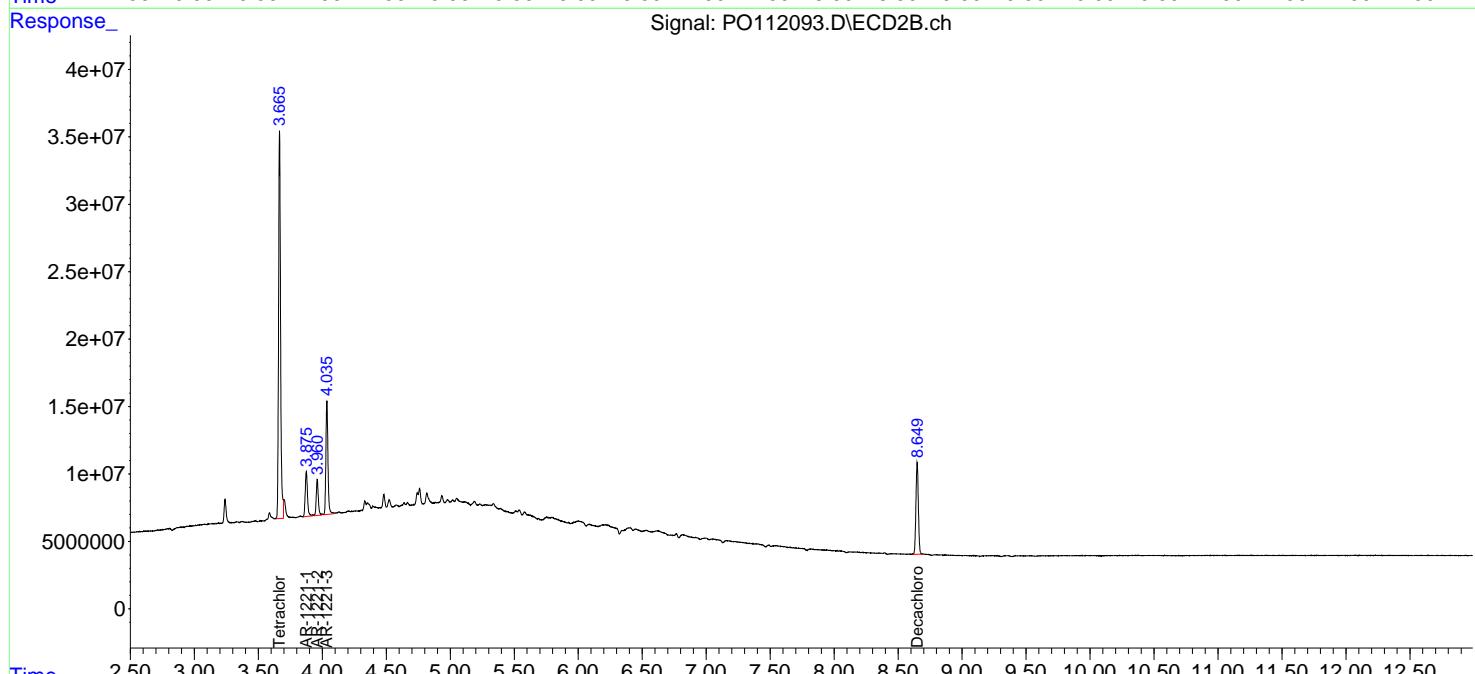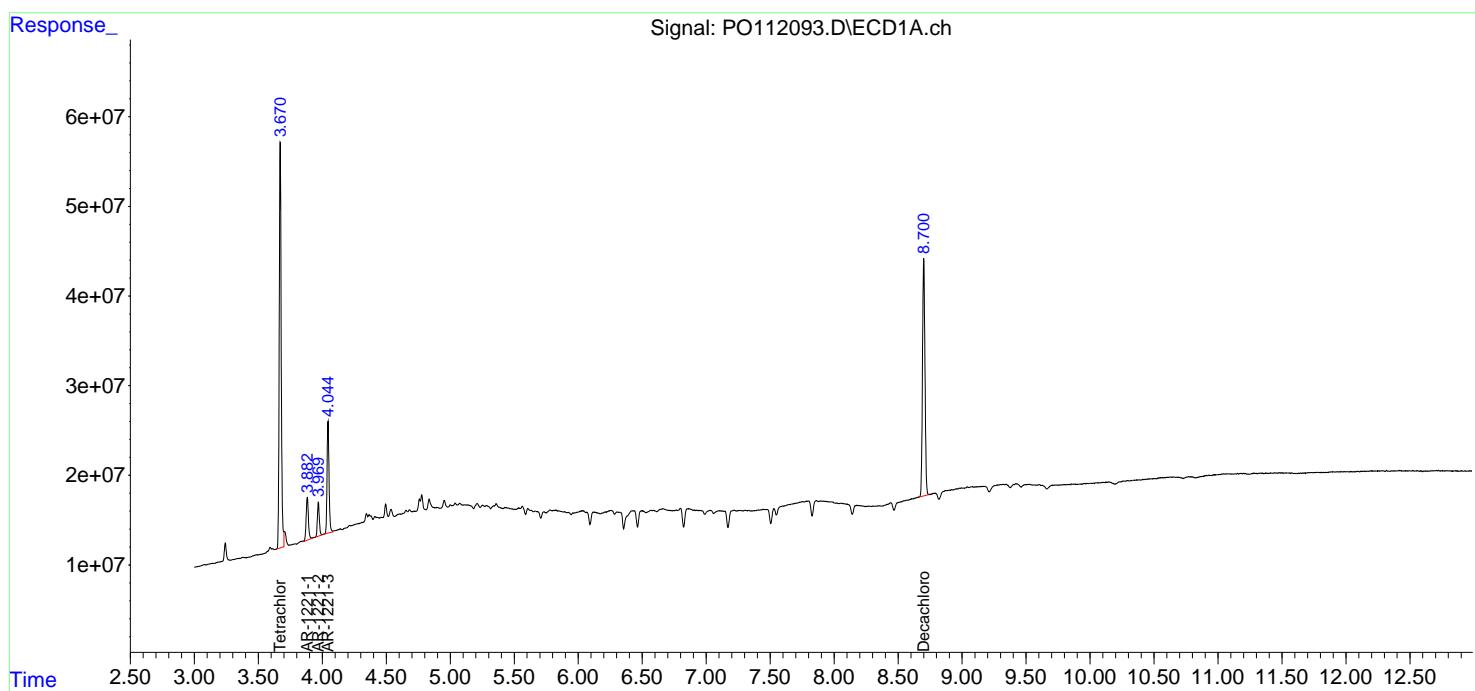

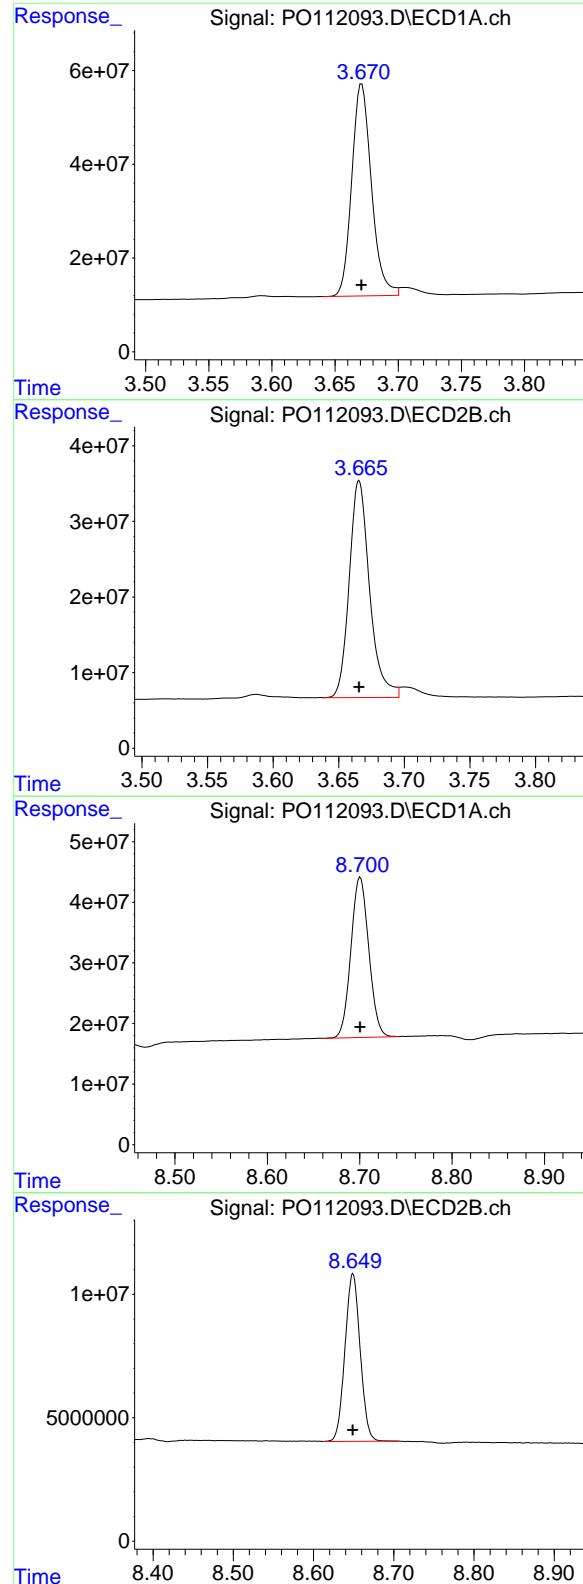

#1 Tetrachloro-m-xylene

R.T.: 3.671 min
Delta R.T.: 0.000 min
Response: 491308255
Conc: 50.00 ng/ml

Instrument:

ECD_O

ClientSampleId :

AR1221ICC500

#1 Tetrachloro-m-xylene

R.T.: 3.666 min
Delta R.T.: 0.000 min
Response: 310794942
Conc: 50.00 ng/ml

#2 Decachlorobiphenyl

R.T.: 8.701 min
Delta R.T.: 0.000 min
Response: 354582449
Conc: 50.00 ng/ml


#2 Decachlorobiphenyl

R.T.: 8.649 min
Delta R.T.: 0.000 min
Response: 89358669
Conc: 50.00 ng/ml

#8 AR-1221-1


R.T.: 3.883 min
 Delta R.T.: 0.000 min
 Response: 58306973
 Conc: 500.00 ng/ml

Instrument: ECD_O
ClientSampleId: AR1221ICC500




#8 AR-1221-1

R.T.: 3.875 min
 Delta R.T.: 0.000 min
 Response: 41147512
 Conc: 500.00 ng/ml

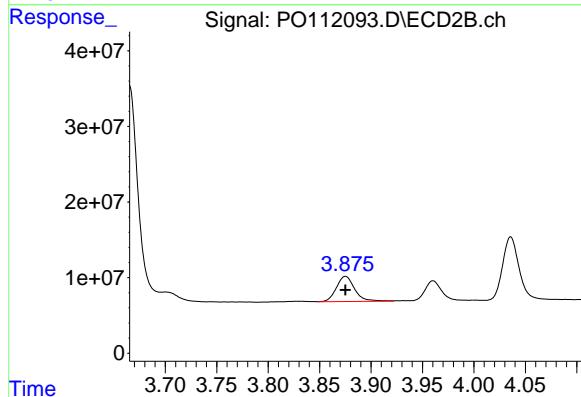


#9 AR-1221-2

R.T.: 3.969 min
 Delta R.T.: 0.000 min
 Response: 39420252
 Conc: 500.00 ng/ml

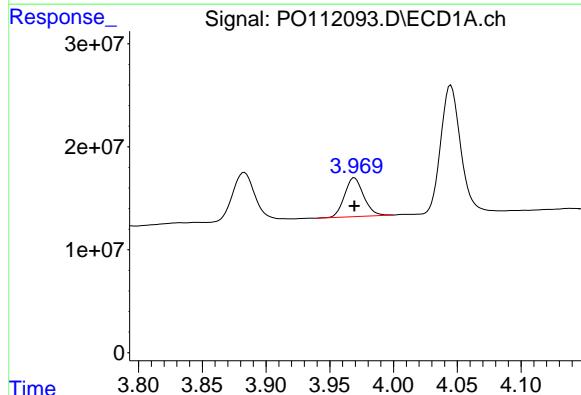

#9 AR-1221-2



R.T.: 3.960 min
 Delta R.T.: 0.000 min
 Response: 29676775
 Conc: 500.00 ng/ml

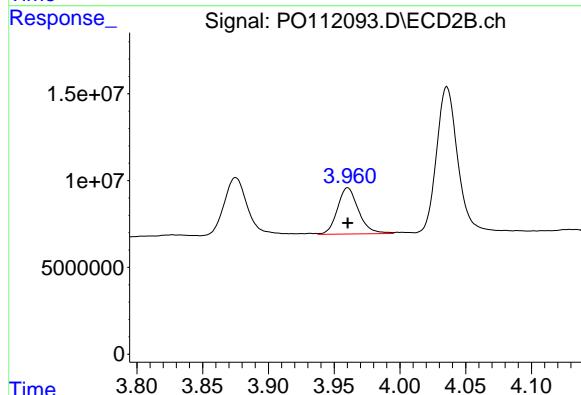

#10 AR-1221-3

R.T.: 4.045 min
Delta R.T.: 0.000 min
Response: 134790876
Conc: 500.00 ng/ml

Instrument: ECD_O
ClientSampleId: AR1221ICC500

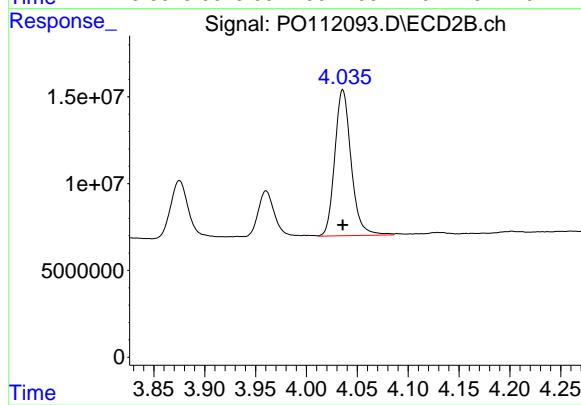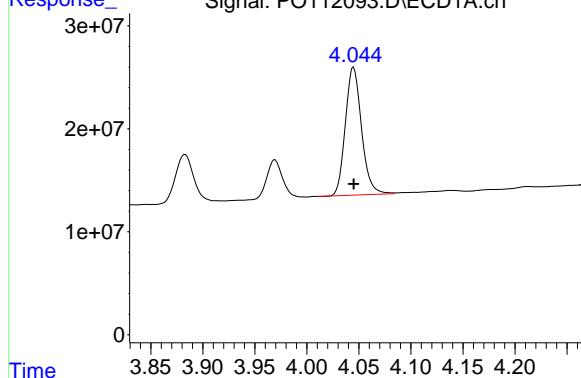

#10 AR-1221-3

R.T.: 4.036 min
Delta R.T.: 0.000 min
Response: 94388324
Conc: 500.00 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0070825\
 Data File : P0112094.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jul 2025 15:57
 Operator : YP/AJ
 Sample : AR1232ICC500
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1232ICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 09 02:23:21 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 09 02:18:55 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	3.673	3.667	508.1E6	328.2E6	50.000	50.000
2) SA Decachlor...	8.703	8.649	348.2E6	88061507	50.000	50.000

Target Compounds

11) L3 AR-1232-1	4.047	4.036	107.3E6	75049686	500.000	500.000
12) L3 AR-1232-2	4.539	4.761	56818484	76542867	500.000	500.000
13) L3 AR-1232-3	4.780	4.936	114.5E6	37753016	500.000	500.000
14) L3 AR-1232-4	4.956	5.021	57148344	32994097	500.000	500.000
15) L3 AR-1232-5	4.999	5.191	36700121	37129963	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0070825\
 Data File : P0112094.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jul 2025 15:57
 Operator : YP/AJ
 Sample : AR1232ICC500
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1232ICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 09 02:23:21 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 09 02:18:55 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ m Signal #2 Info : 30M x 0.32mm x 0.25 μ m

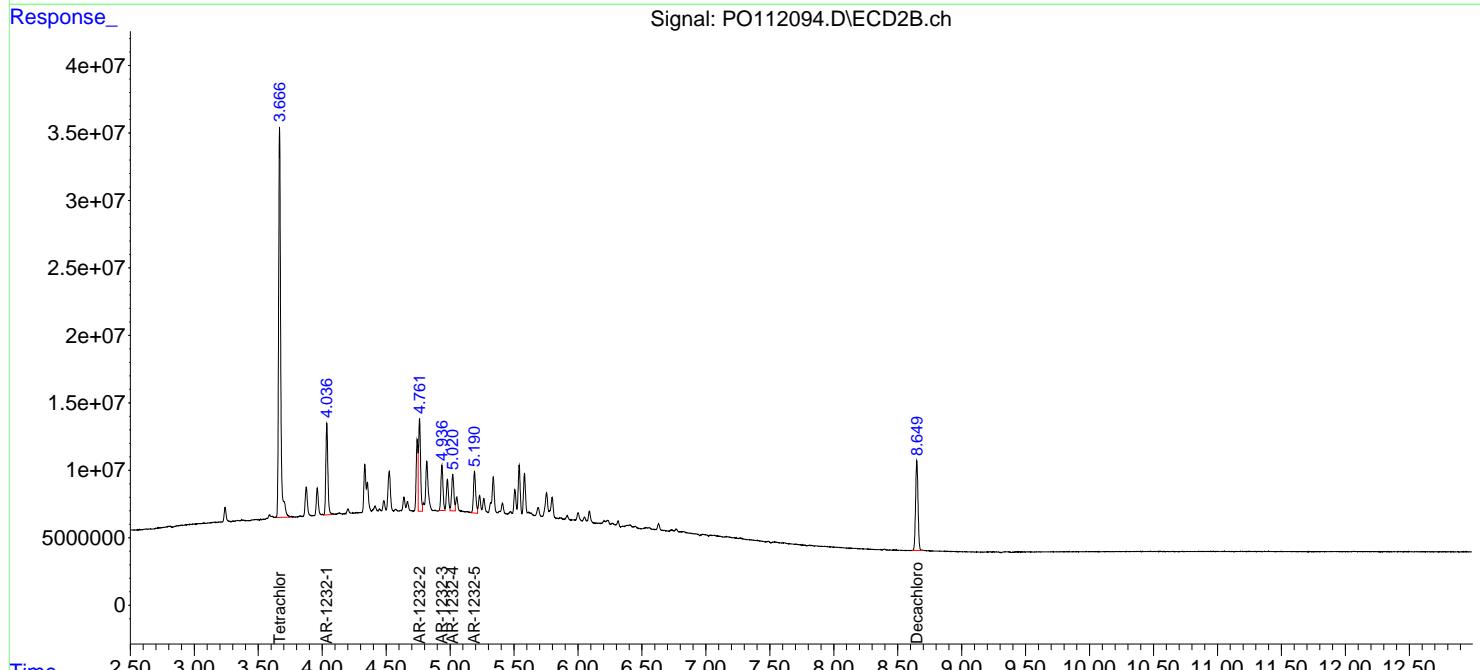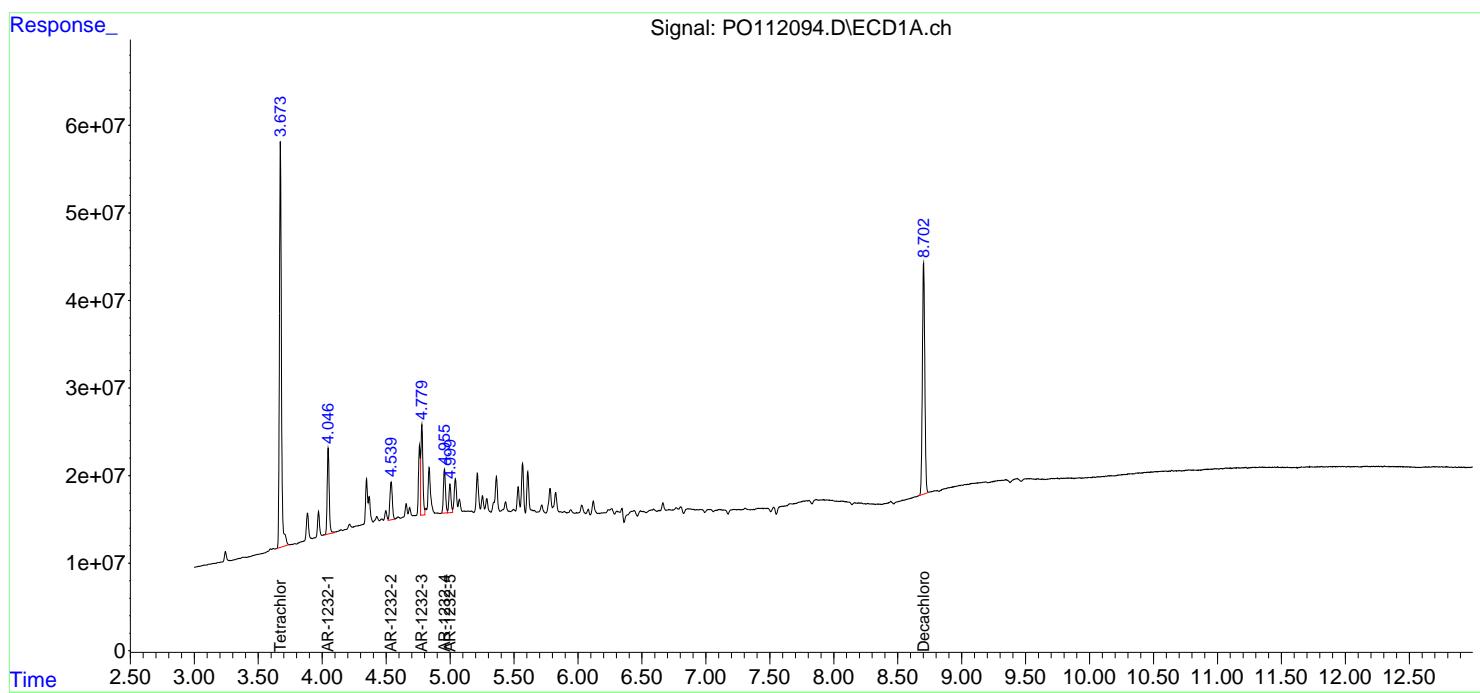

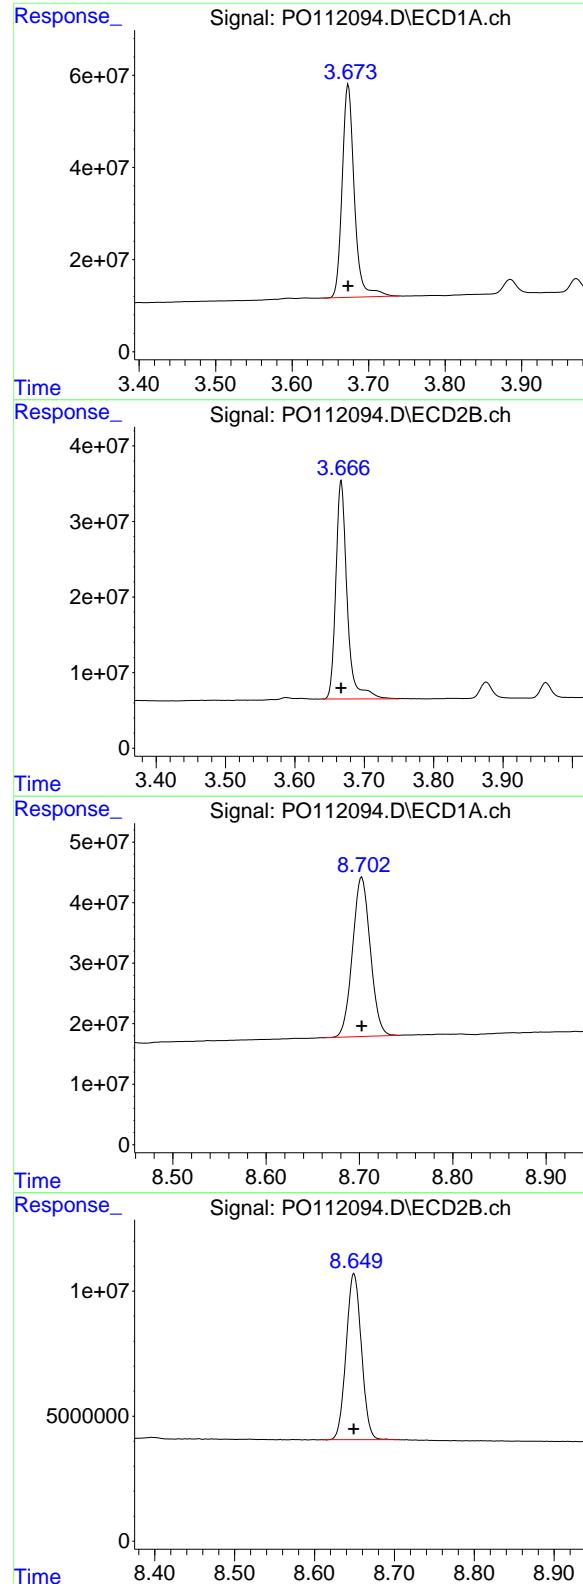

#1 Tetrachloro-m-xylene

R.T.: 3.673 min
Delta R.T.: 0.000 min
Response: 508090487
Conc: 50.00 ng/ml

Instrument: ECD_O
ClientSampleId: AR1232ICC500

#1 Tetrachloro-m-xylene


R.T.: 3.667 min
Delta R.T.: 0.000 min
Response: 328240519
Conc: 50.00 ng/ml

#2 Decachlorobiphenyl

R.T.: 8.703 min
Delta R.T.: 0.000 min
Response: 348200291
Conc: 50.00 ng/ml

#2 Decachlorobiphenyl

R.T.: 8.649 min
Delta R.T.: 0.000 min
Response: 88061507
Conc: 50.00 ng/ml

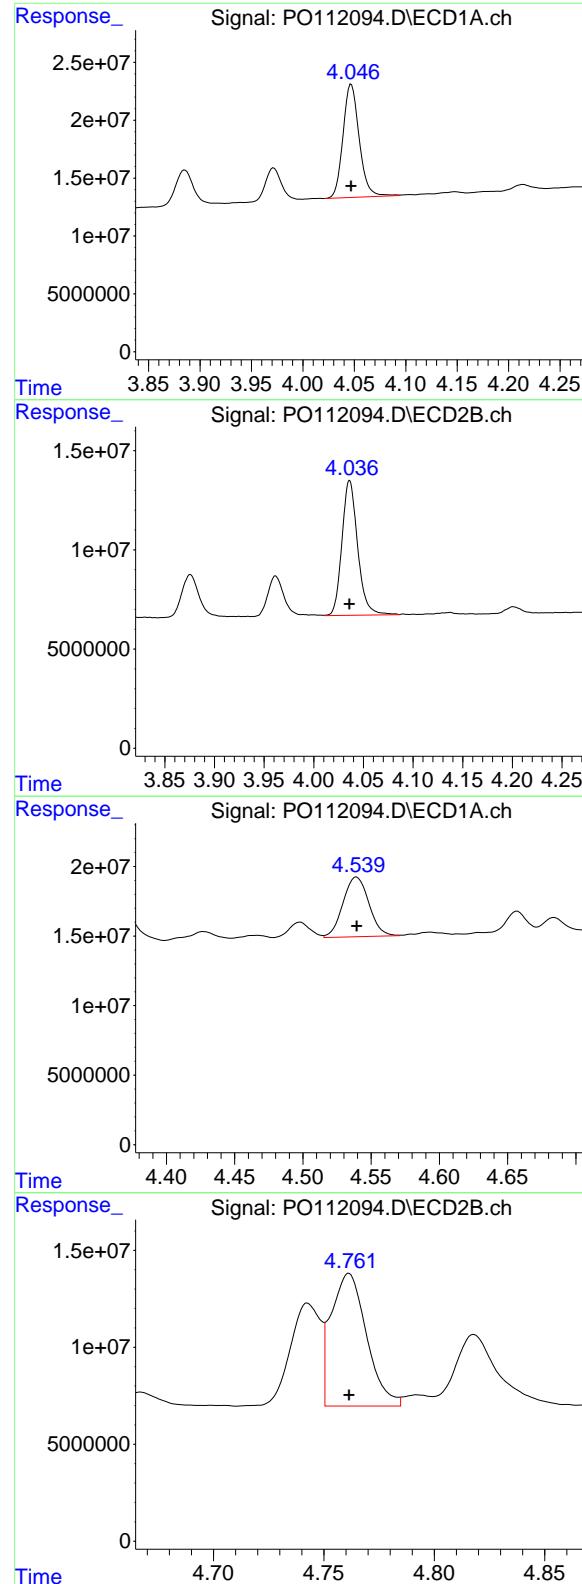

#11 AR-1232-1

R.T.: 4.047 min
 Delta R.T.: 0.000 min
 Response: 107333865
 Conc: 500.00 ng/ml

Instrument: ECD_O
ClientSampleId: AR1232ICC500

#11 AR-1232-1

R.T.: 4.036 min
 Delta R.T.: 0.000 min
 Response: 75049686
 Conc: 500.00 ng/ml


#12 AR-1232-2

R.T.: 4.539 min
 Delta R.T.: 0.000 min
 Response: 56818484
 Conc: 500.00 ng/ml

#12 AR-1232-2

R.T.: 4.761 min
 Delta R.T.: 0.000 min
 Response: 76542867
 Conc: 500.00 ng/ml

#13 AR-1232-3

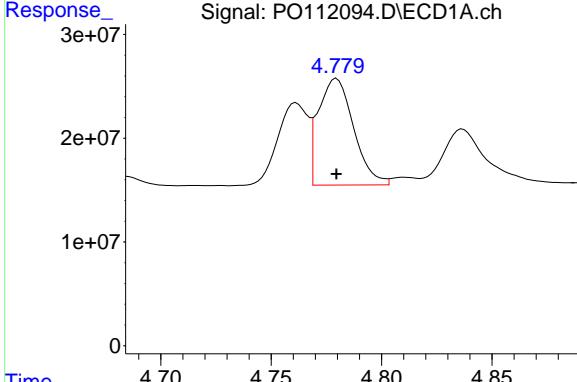


R.T.: 4.780 min
Delta R.T.: 0.000 min
Response: 114504426
Conc: 500.00 ng/ml

Instrument: ECD_O
ClientSampleId: AR1232ICC500


#13 AR-1232-3

R.T.: 4.936 min
Delta R.T.: 0.000 min
Response: 37753016
Conc: 500.00 ng/ml

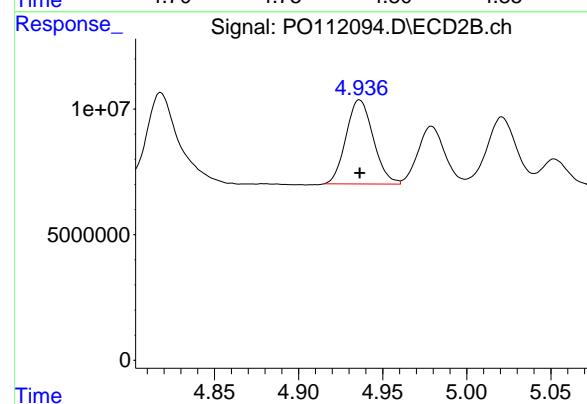


#14 AR-1232-4

R.T.: 4.956 min
Delta R.T.: 0.000 min
Response: 57148344
Conc: 500.00 ng/ml

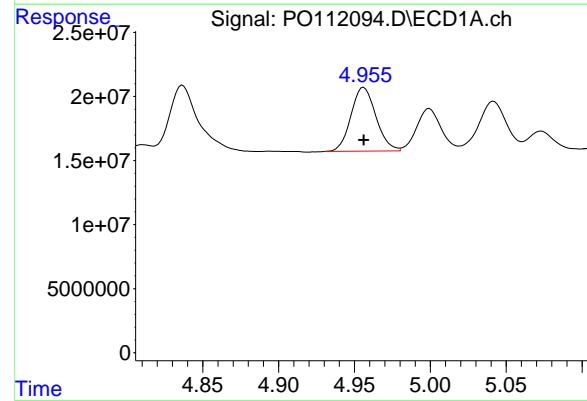



#14 AR-1232-4

R.T.: 5.021 min
Delta R.T.: 0.000 min
Response: 32994097
Conc: 500.00 ng/ml

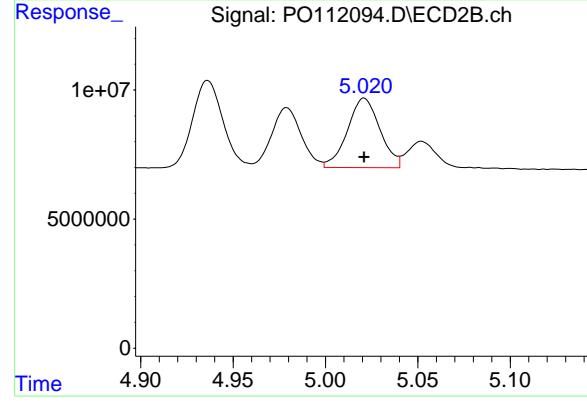

#15 AR-1232-5

R.T.: 4.999 min
Delta R.T.: 0.000 min **Instrument:**
Response: 36700121 ECD_O
Conc: 500.00 ng/ml **ClientSampleId:**
AR1232ICC500

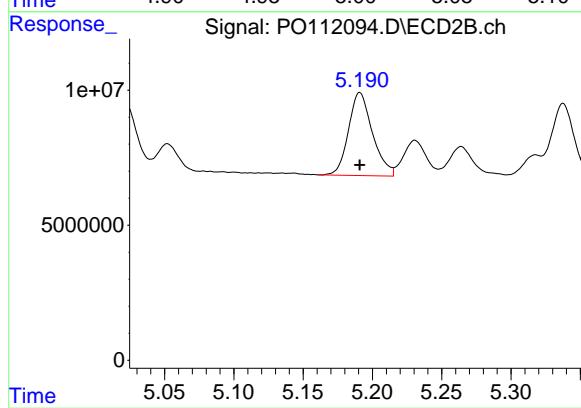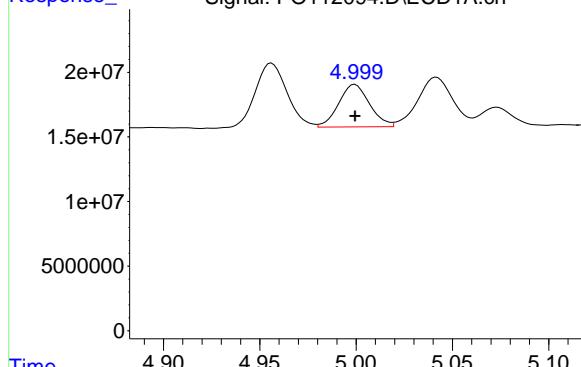

#15 AR-1232-5

R.T.: 5.191 min
Delta R.T.: 0.000 min
Response: 37129963
Conc: 500.00 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0070825\
 Data File : P0112095.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jul 2025 16:15
 Operator : YP/AJ
 Sample : AR1242ICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1242ICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 09 02:30:35 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 09 02:27:13 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	3.674	3.667	1004.8E6	640.9E6	95.343	95.216
2) SA Decachlor...	8.703	8.651	698.0E6	169.5E6	97.460	94.180

Target Compounds

16) L4 AR-1242-1	4.761	4.744	285.0E6	180.6E6	941.908	920.490
17) L4 AR-1242-2	4.780	4.762	425.0E6	267.1E6	945.333	925.046
18) L4 AR-1242-3	4.837	4.937	267.3E6	139.4E6	930.232	929.182
19) L4 AR-1242-4	4.957	5.022	217.5E6	132.6E6	938.623	923.575
20) L4 AR-1242-5	5.608	5.541	218.4E6	169.3E6	972.805	904.772



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0070825\
 Data File : P0112095.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jul 2025 16:15
 Operator : YP/AJ
 Sample : AR1242ICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1242ICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 09 02:30:35 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 09 02:27:13 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

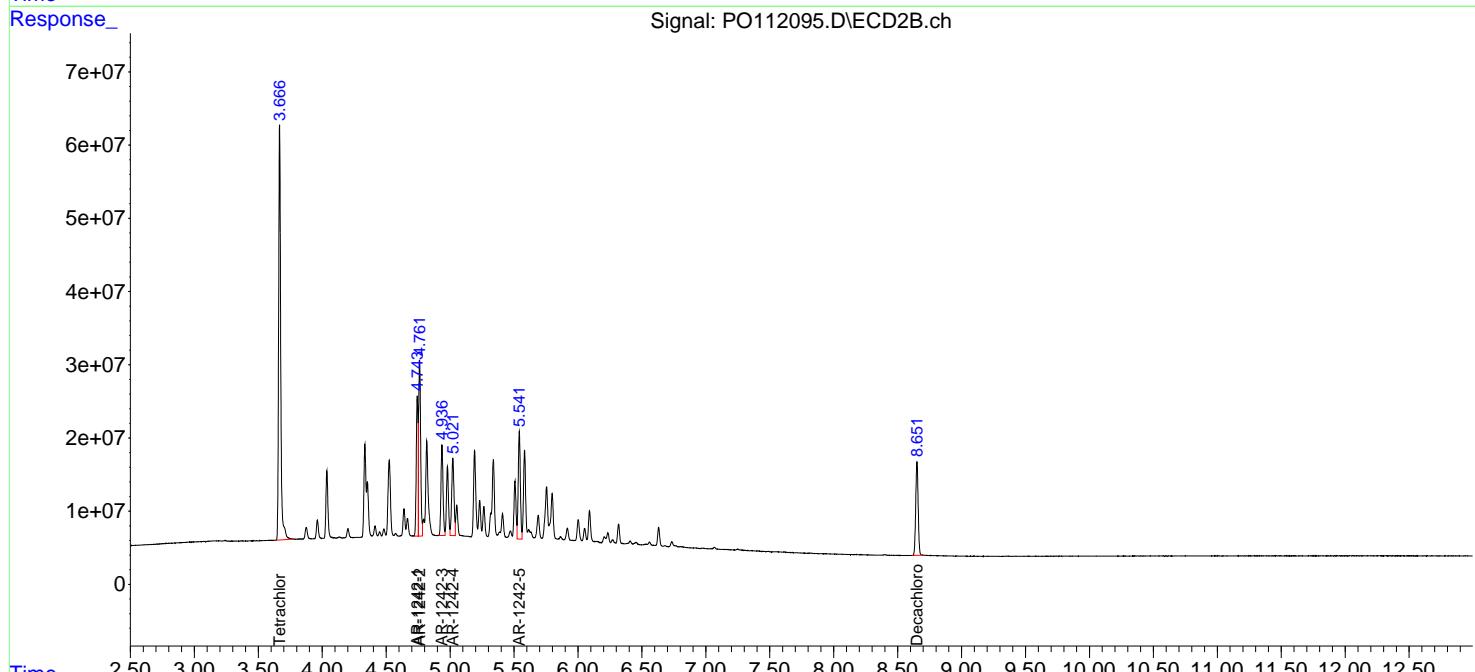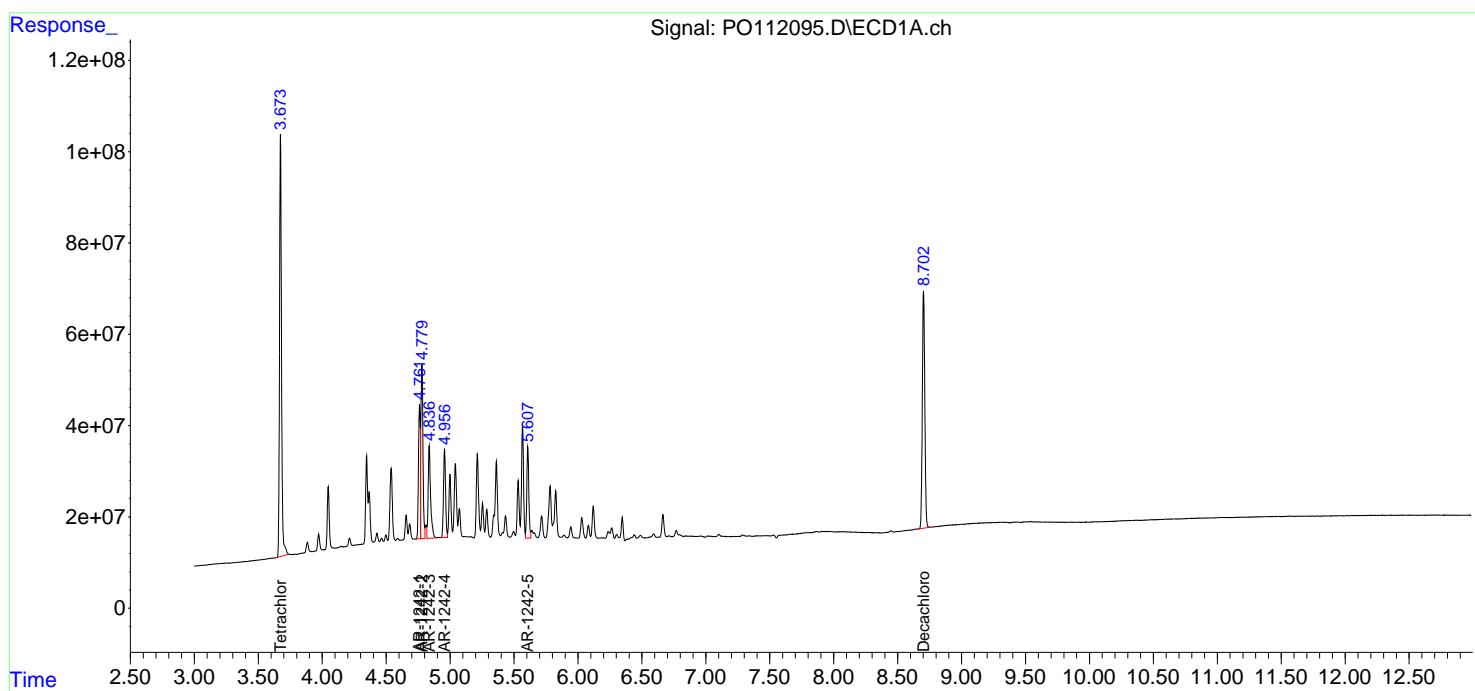

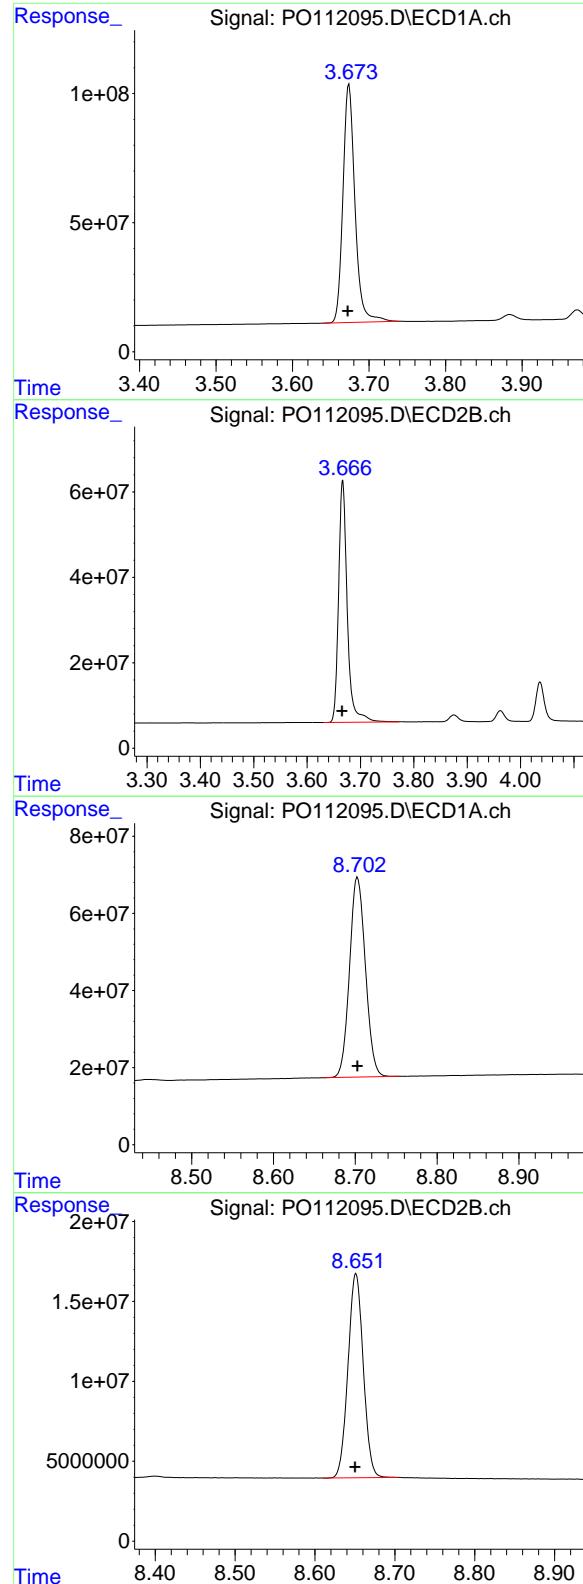

#1 Tetrachloro-m-xylene

R.T.: 3.674 min
 Delta R.T.: 0.002 min
 Response: 1004763356
 Conc: 95.34 ng/ml

Instrument: ECD_O
 ClientSampleId: AR1242ICC1000

#1 Tetrachloro-m-xylene

R.T.: 3.667 min
 Delta R.T.: 0.001 min
 Response: 640869487
 Conc: 95.22 ng/ml

#2 Decachlorobiphenyl

R.T.: 8.703 min
 Delta R.T.: 0.000 min
 Response: 697996912
 Conc: 97.46 ng/ml


#2 Decachlorobiphenyl

R.T.: 8.651 min
 Delta R.T.: 0.001 min
 Response: 169498593
 Conc: 94.18 ng/ml

#16 AR-1242-1


R.T.: 4.761 min
 Delta R.T.: 0.002 min
 Response: 285009923
 Conc: 941.91 ng/ml

Instrument: ECD_O
ClientSampleId: AR1242ICC1000

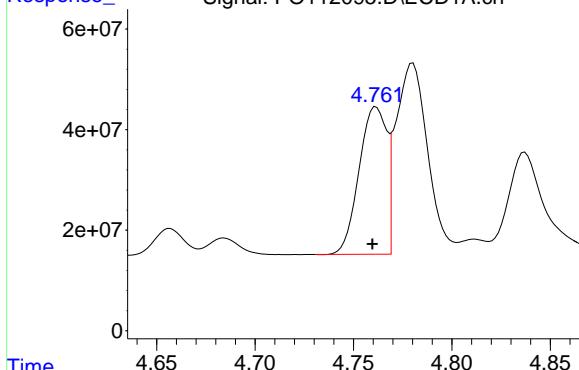


#16 AR-1242-1

R.T.: 4.744 min
 Delta R.T.: 0.002 min
 Response: 180558203
 Conc: 920.49 ng/ml

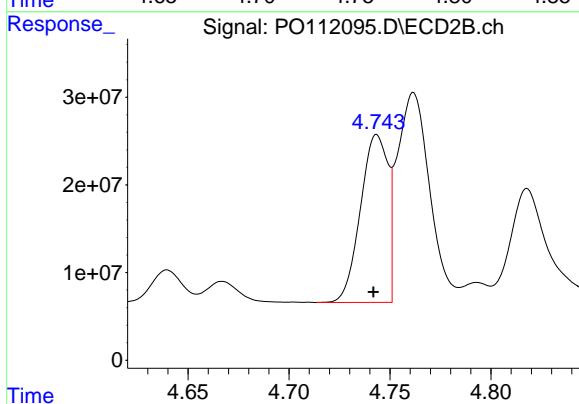


#17 AR-1242-2

R.T.: 4.780 min
 Delta R.T.: 0.002 min
 Response: 424985528
 Conc: 945.33 ng/ml

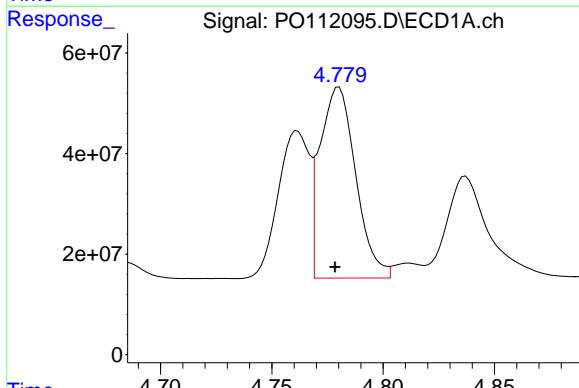

#17 AR-1242-2





R.T.: 4.762 min
 Delta R.T.: 0.001 min
 Response: 267145812
 Conc: 925.05 ng/ml

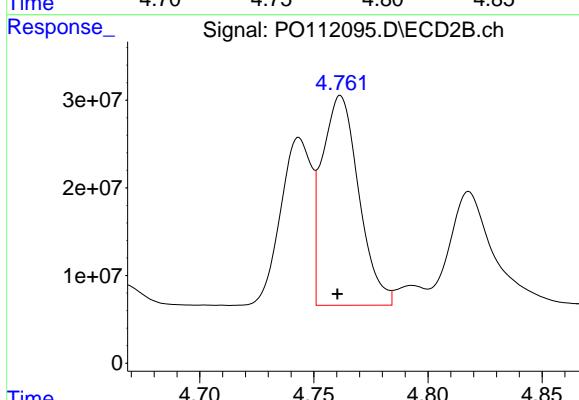

#18 AR-1242-3

R.T.: 4.837 min
 Delta R.T.: 0.002 min
 Response: 267327438
 Conc: 930.23 ng/ml

Instrument: ECD_O
 ClientSampleId: AR1242ICC1000

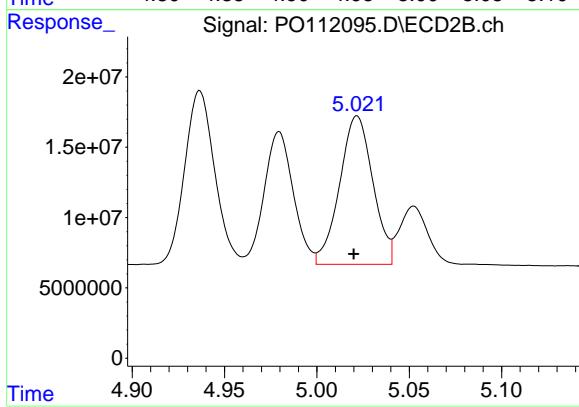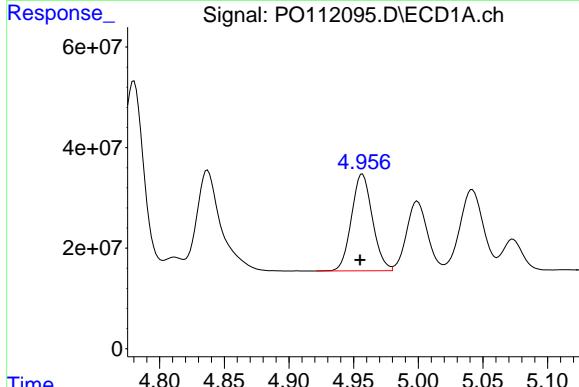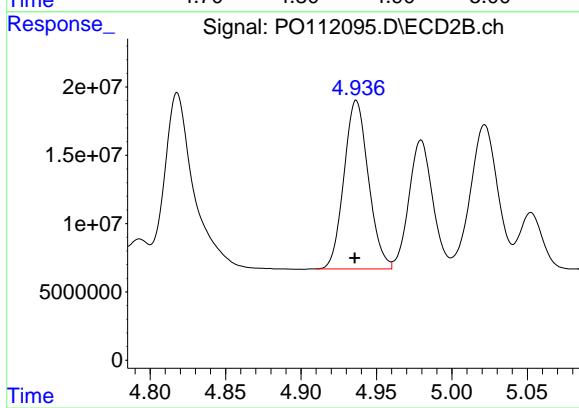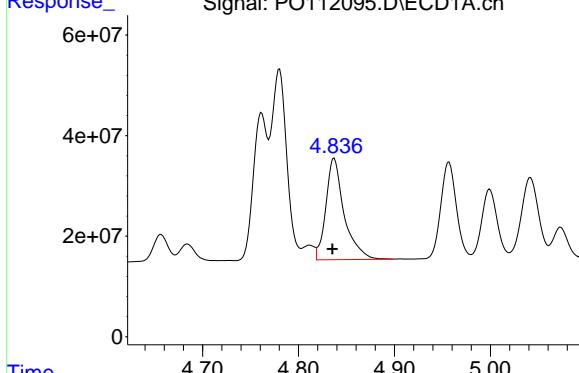

#18 AR-1242-3

R.T.: 4.937 min
 Delta R.T.: 0.000 min
 Response: 139388587
 Conc: 929.18 ng/ml

#19 AR-1242-4

R.T.: 4.957 min
 Delta R.T.: 0.002 min
 Response: 217524144
 Conc: 938.62 ng/ml


#19 AR-1242-4

R.T.: 5.022 min
 Delta R.T.: 0.002 min
 Response: 132647733
 Conc: 923.58 ng/ml

#20 AR-1242-5

R.T.: 5.608 min
Delta R.T.: 0.000 min
Response: 218416651
Conc: 972.81 ng/ml

Instrument: ECD_O
ClientSampleId: AR1242ICC1000

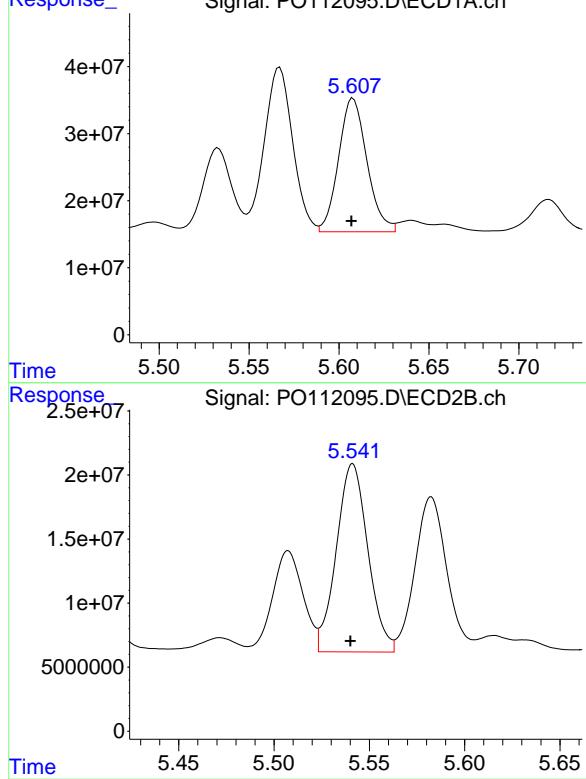

#20 AR-1242-5

R.T.: 5.541 min
Delta R.T.: 0.001 min
Response: 169256952
Conc: 904.77 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0070825\
 Data File : P0112096.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jul 2025 16:34
 Operator : YP/AJ
 Sample : AR1242ICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1242ICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 09 02:30:45 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 09 02:27:13 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	3.673	3.666	806.4E6	515.4E6	76.520	76.575
2) SA Decachlor...	8.704	8.650	536.1E6	132.4E6	74.848	73.593

Target Compounds

16) L4 AR-1242-1	4.761	4.743	229.3E6	145.7E6	757.886	742.820
17) L4 AR-1242-2	4.780	4.761	338.7E6	214.4E6	753.331	742.460
18) L4 AR-1242-3	4.837	4.936	213.9E6	112.4E6	744.270	749.423
19) L4 AR-1242-4	4.956	5.021	174.1E6	106.9E6	751.378	744.191
20) L4 AR-1242-5	5.608	5.540	174.3E6	136.6E6	776.440	729.978



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0070825\
 Data File : P0112096.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jul 2025 16:34
 Operator : YP/AJ
 Sample : AR1242ICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_O
ClientSampleId :
 AR1242ICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 09 02:30:45 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 09 02:27:13 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

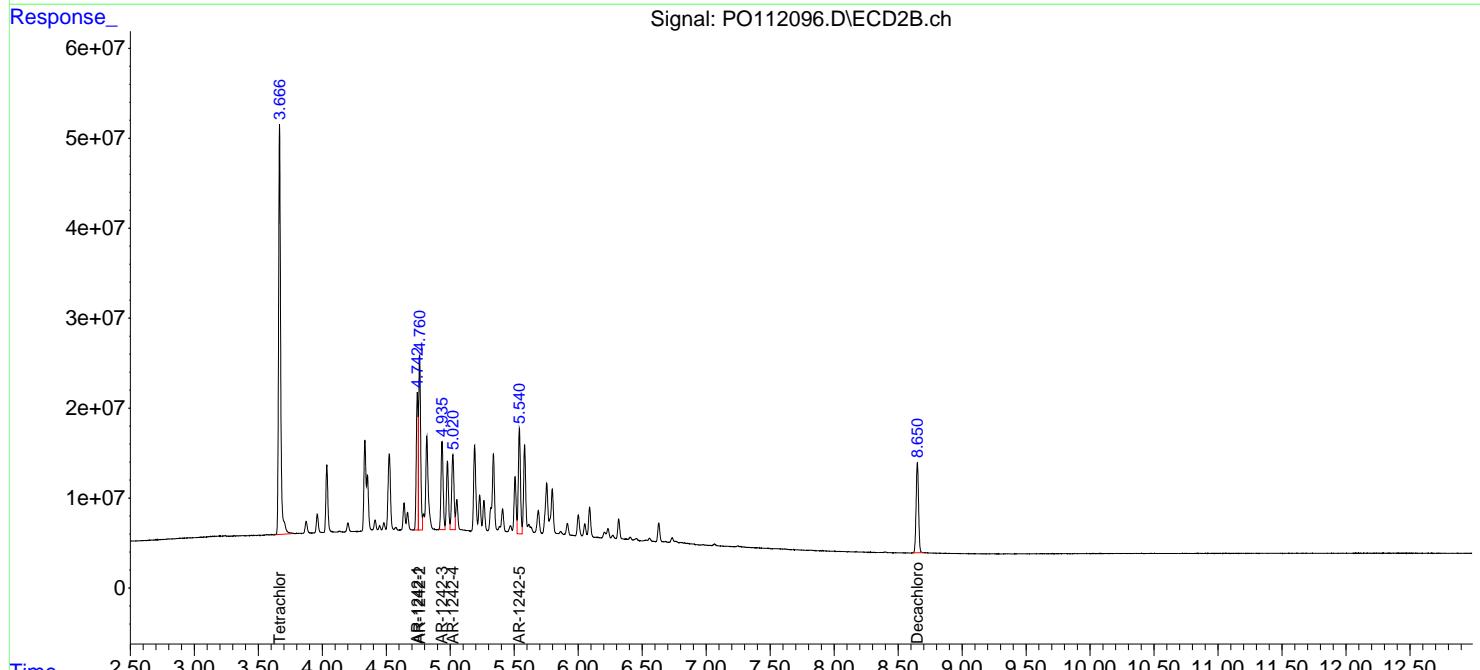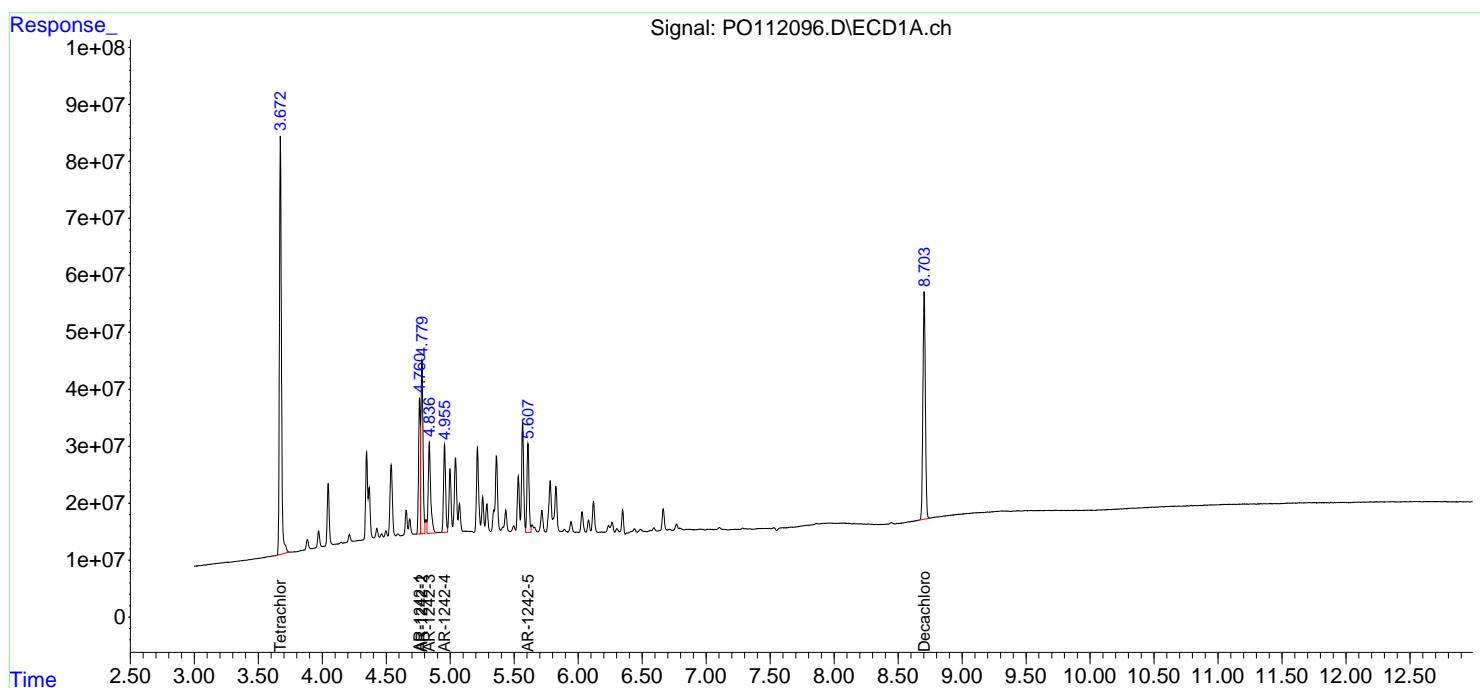

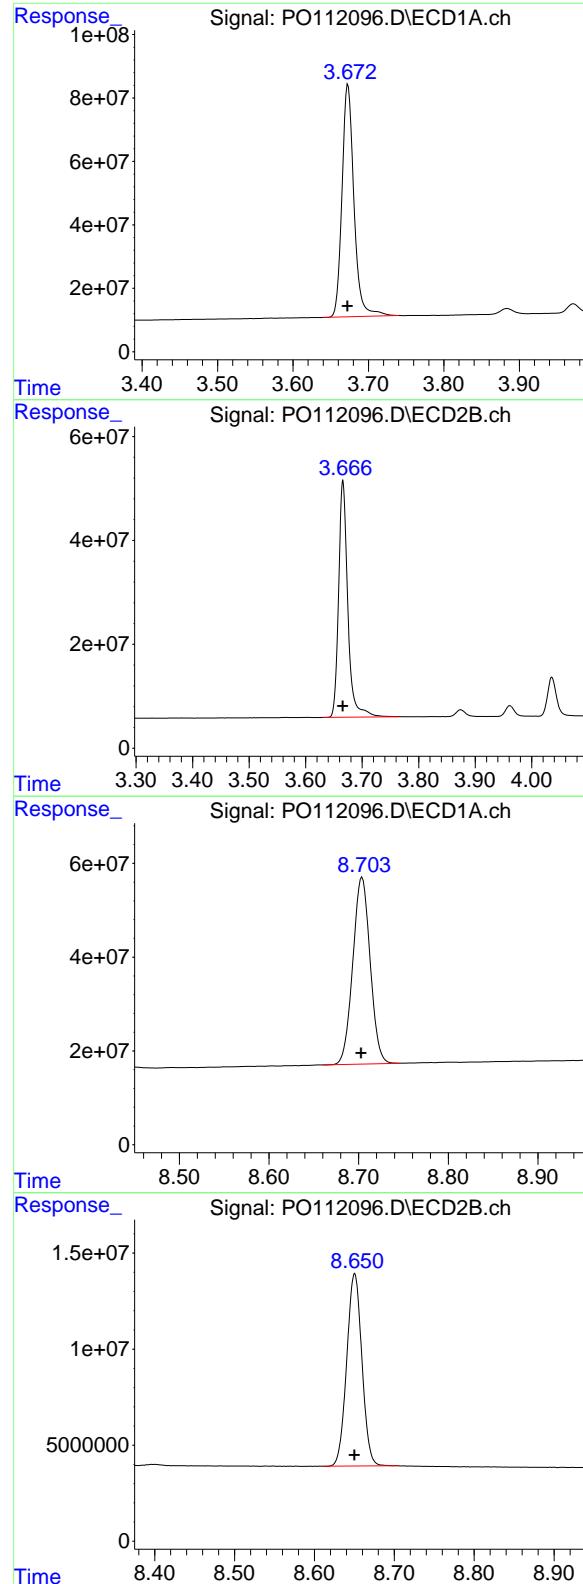

#1 Tetrachloro-m-xylene

R.T.: 3.673 min
 Delta R.T.: 0.000 min
 Response: 806402483
 Conc: 76.52 ng/ml

Instrument: ECD_O
ClientSampleId: AR1242ICC750

#1 Tetrachloro-m-xylene

R.T.: 3.666 min
 Delta R.T.: 0.000 min
 Response: 515402675
 Conc: 76.57 ng/ml


#2 Decachlorobiphenyl

R.T.: 8.704 min
 Delta R.T.: 0.001 min
 Response: 536055523
 Conc: 74.85 ng/ml

#2 Decachlorobiphenyl

R.T.: 8.650 min
 Delta R.T.: 0.000 min
 Response: 132448036
 Conc: 73.59 ng/ml

#16 AR-1242-1

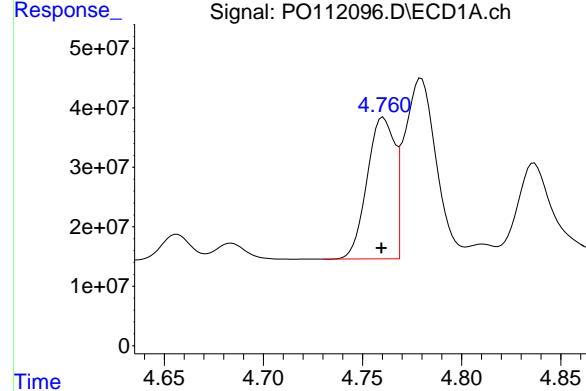

R.T.: 4.761 min
 Delta R.T.: 0.001 min
 Response: 229327263
 Conc: 757.89 ng/ml

Instrument: ECD_O
 ClientSampleId: AR1242ICC750

#16 AR-1242-1




R.T.: 4.743 min
 Delta R.T.: 0.000 min
 Response: 145707357
 Conc: 742.82 ng/ml


#17 AR-1242-2

R.T.: 4.780 min
 Delta R.T.: 0.001 min
 Response: 338668755
 Conc: 753.33 ng/ml

#17 AR-1242-2

R.T.: 4.761 min
 Delta R.T.: 0.000 min
 Response: 214416419
 Conc: 742.46 ng/ml

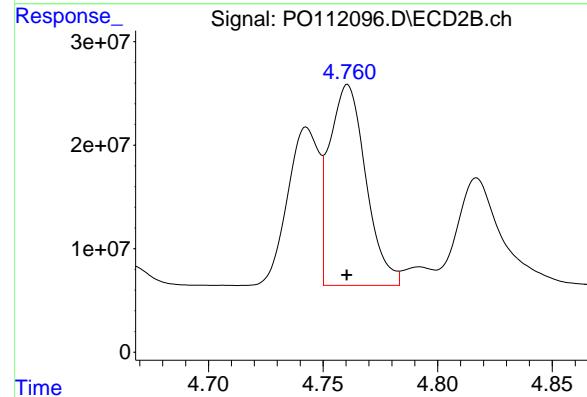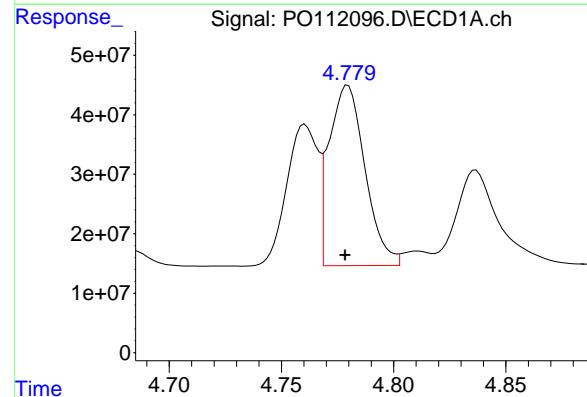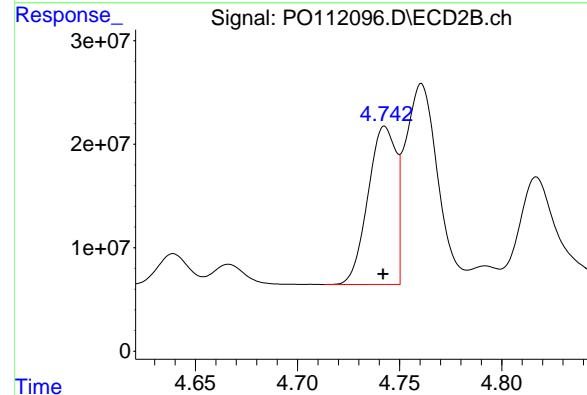

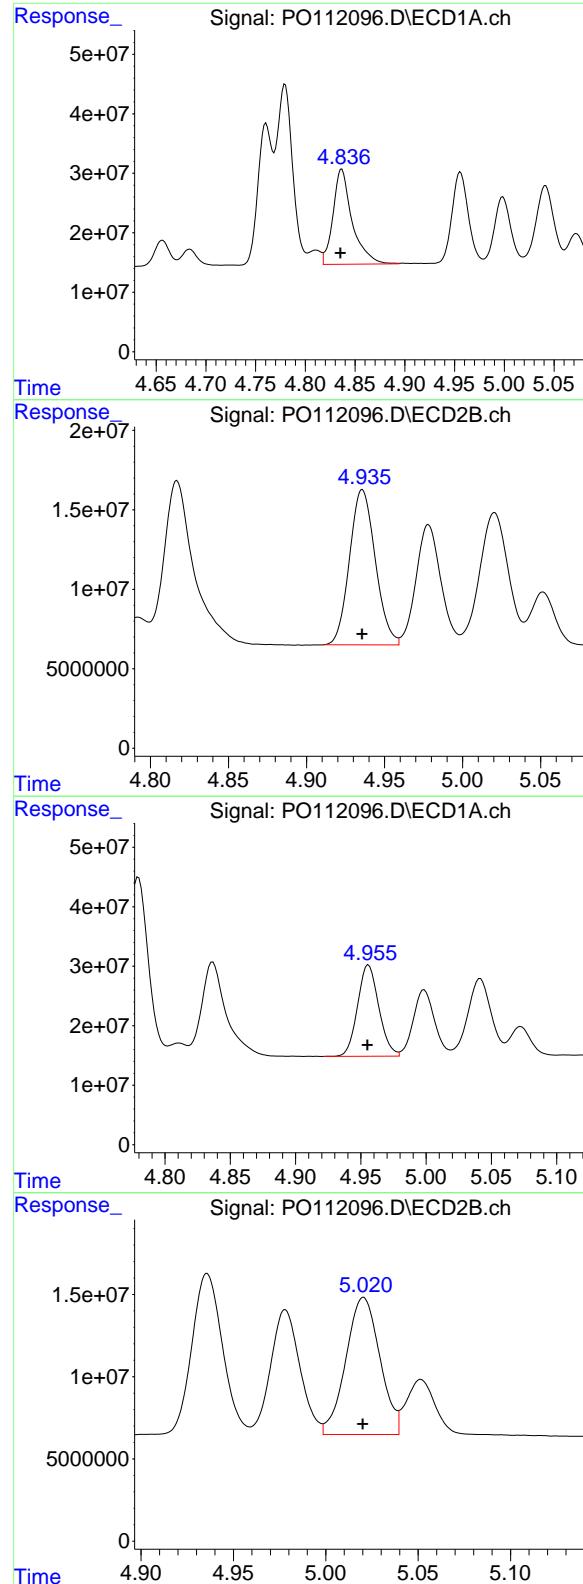

#18 AR-1242-3

R.T.: 4.837 min
 Delta R.T.: 0.001 min
 Response: 213886334
 Conc: 744.27 ng/ml

Instrument: ECD_O
 ClientSampleId: AR1242ICC750

#18 AR-1242-3


R.T.: 4.936 min
 Delta R.T.: 0.000 min
 Response: 112422531
 Conc: 749.42 ng/ml

#19 AR-1242-4

R.T.: 4.956 min
 Delta R.T.: 0.000 min
 Response: 174130485
 Conc: 751.38 ng/ml

#19 AR-1242-4

R.T.: 5.021 min
 Delta R.T.: 0.000 min
 Response: 106883873
 Conc: 744.19 ng/ml

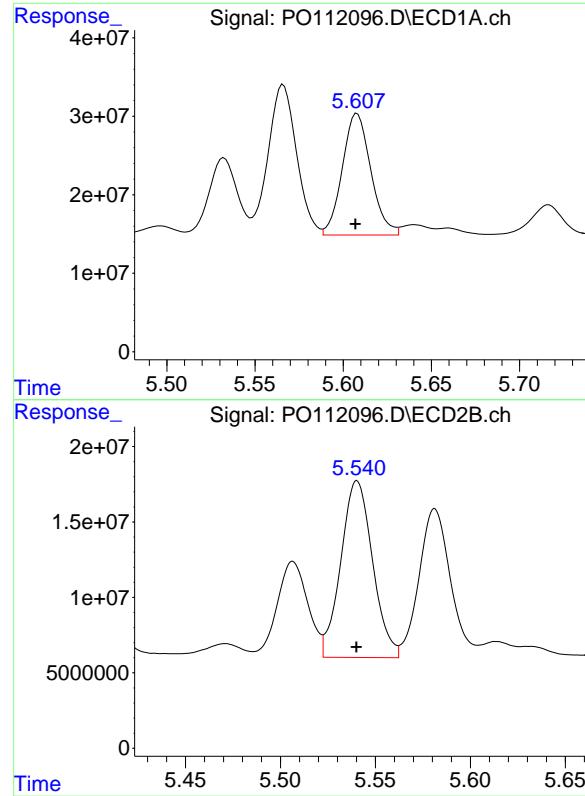

#20 AR-1242-5

R.T.: 5.608 min
Delta R.T.: 0.001 min
Response: 174328144
Conc: 776.44 ng/ml

Instrument: ECD_O
ClientSampleId: AR1242ICC750

#20 AR-1242-5

R.T.: 5.540 min
Delta R.T.: 0.000 min
Response: 136558108
Conc: 729.98 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0070825\
 Data File : P0112097.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jul 2025 16:52
 Operator : YP/AJ
 Sample : AR1242ICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1242ICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 09 02:30:55 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 09 02:27:13 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	3.672	3.666	526.9E6	336.5E6	50.000	50.000
2) SA Decachlor...	8.703	8.650	358.1E6	89986417	50.000	50.000

Target Compounds

16) L4 AR-1242-1	4.760	4.742	151.3E6	98077221	500.000	500.000
17) L4 AR-1242-2	4.778	4.760	224.8E6	144.4E6	500.000	500.000
18) L4 AR-1242-3	4.835	4.936	143.7E6	75006072	500.000	500.000
19) L4 AR-1242-4	4.955	5.020	115.9E6	71812102	500.000	500.000
20) L4 AR-1242-5	5.607	5.540	112.3E6	93535709	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0070825\
 Data File : P0112097.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jul 2025 16:52
 Operator : YP/AJ
 Sample : AR1242ICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1242ICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 09 02:30:55 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 09 02:27:13 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

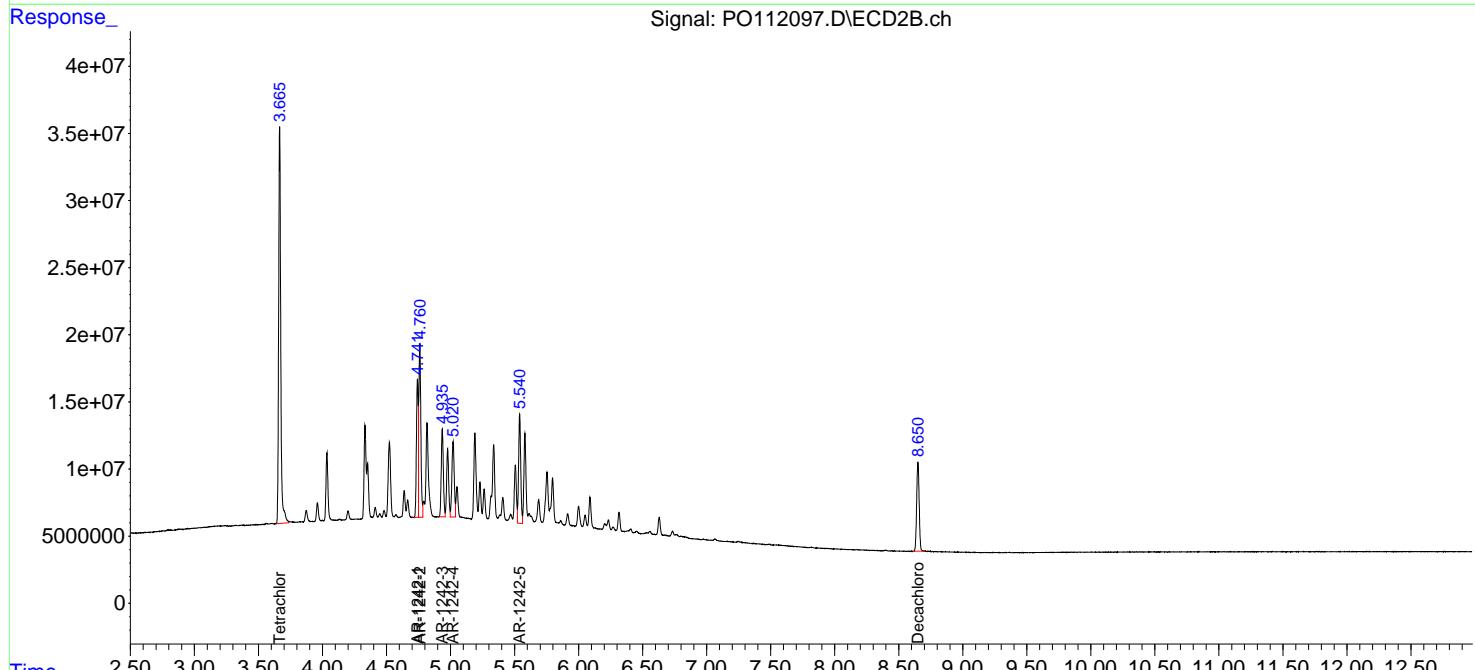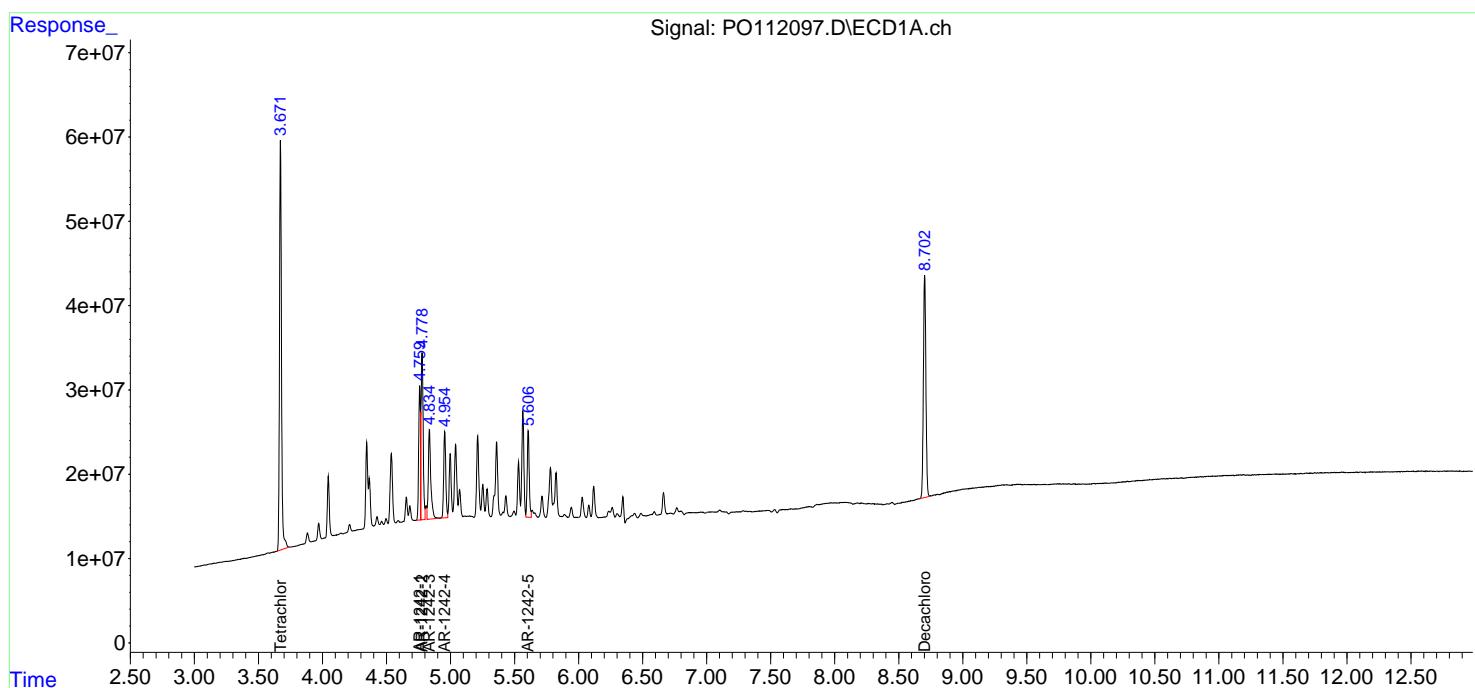

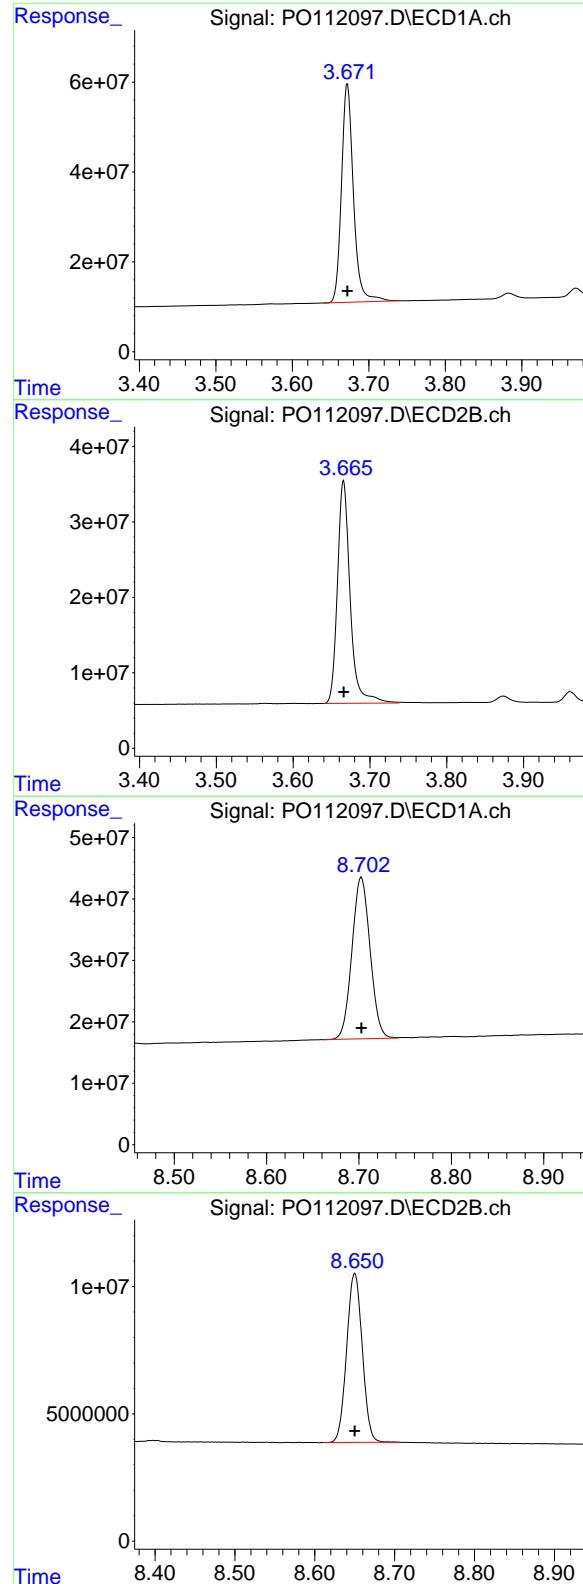

#1 Tetrachloro-m-xylene

R.T.: 3.672 min
 Delta R.T.: 0.000 min
 Response: 526920237
 Conc: 50.00 ng/ml

Instrument:

ECD_O

ClientSampleId :
AR1242ICC500

#1 Tetrachloro-m-xylene


R.T.: 3.666 min
 Delta R.T.: 0.000 min
 Response: 336535914
 Conc: 50.00 ng/ml

#2 Decachlorobiphenyl

R.T.: 8.703 min
 Delta R.T.: 0.000 min
 Response: 358093968
 Conc: 50.00 ng/ml

#2 Decachlorobiphenyl

R.T.: 8.650 min
 Delta R.T.: 0.000 min
 Response: 89986417
 Conc: 50.00 ng/ml

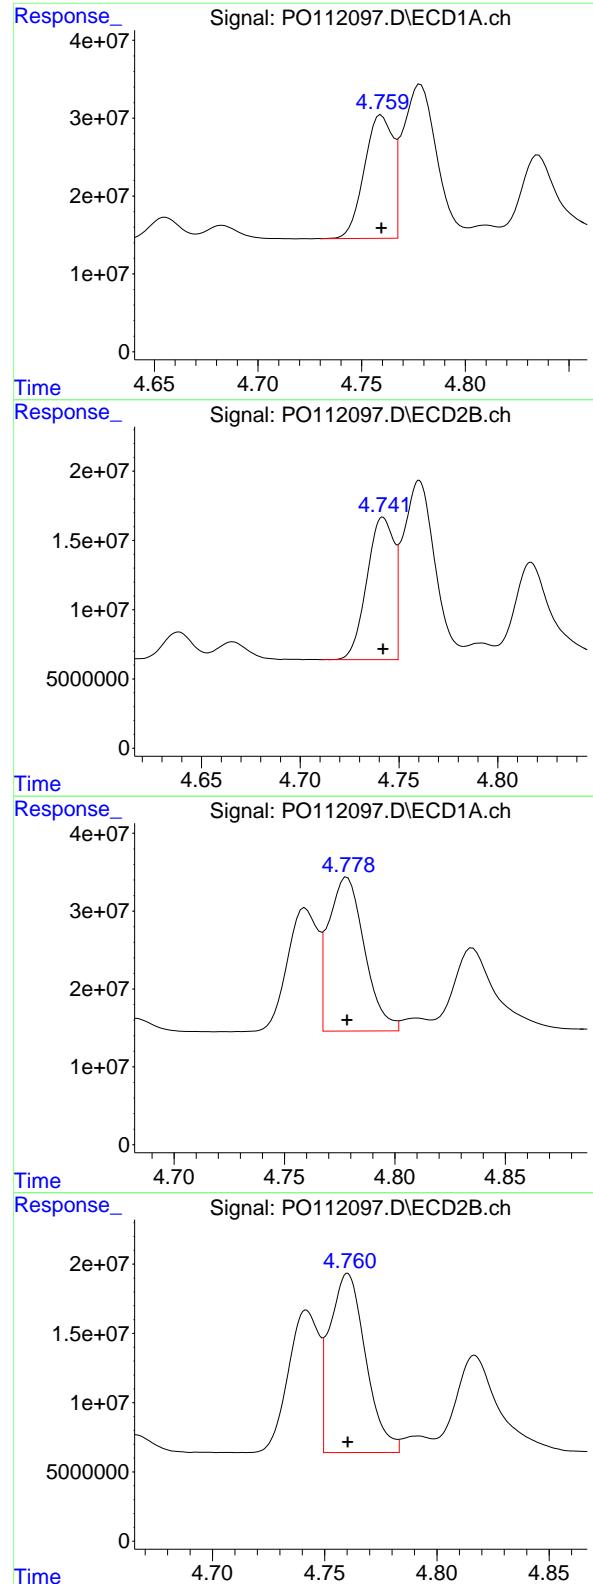

#16 AR-1242-1

R.T.: 4.760 min
 Delta R.T.: 0.000 min
 Response: 151293970
 Conc: 500.00 ng/ml

Instrument: ECD_O
 ClientSampleId: AR1242ICC500

#16 AR-1242-1

R.T.: 4.742 min
 Delta R.T.: 0.000 min
 Response: 98077221
 Conc: 500.00 ng/ml

#17 AR-1242-2

R.T.: 4.778 min
 Delta R.T.: 0.000 min
 Response: 224780927
 Conc: 500.00 ng/ml


#17 AR-1242-2

R.T.: 4.760 min
 Delta R.T.: 0.000 min
 Response: 144395967
 Conc: 500.00 ng/ml

#18 AR-1242-3


R.T.: 4.835 min
 Delta R.T.: 0.000 min
 Response: 143688602
 Conc: 500.00 ng/ml

Instrument: ECD_O
ClientSampleId: AR1242ICC500

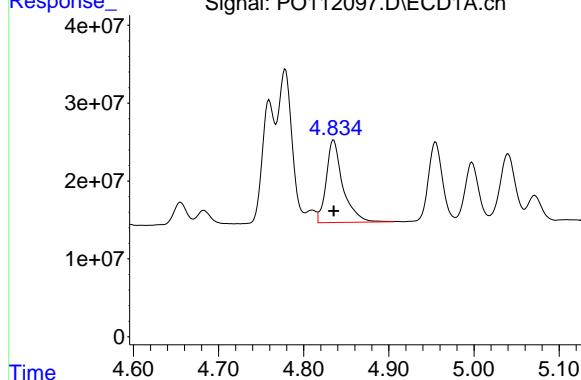


#18 AR-1242-3

R.T.: 4.936 min
 Delta R.T.: 0.000 min
 Response: 75006072
 Conc: 500.00 ng/ml

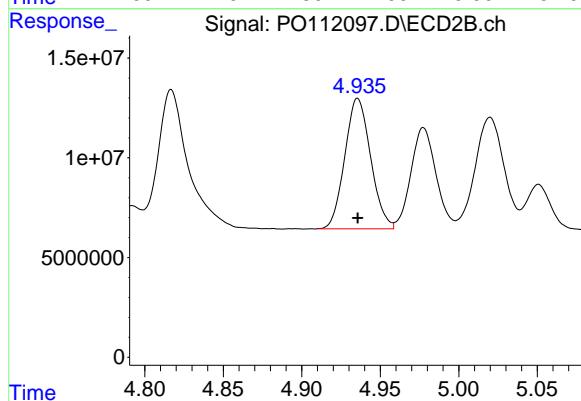


#19 AR-1242-4

R.T.: 4.955 min
 Delta R.T.: 0.000 min
 Response: 115874062
 Conc: 500.00 ng/ml

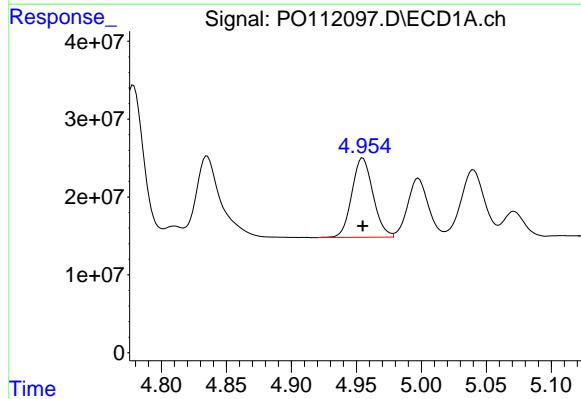

#19 AR-1242-4



R.T.: 5.020 min
 Delta R.T.: 0.000 min
 Response: 71812102
 Conc: 500.00 ng/ml

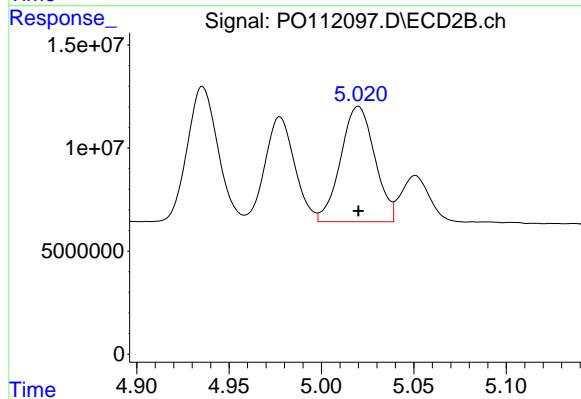

#20 AR-1242-5

R.T.: 5.607 min
Delta R.T.: 0.000 min
Response: 112261248
Conc: 500.00 ng/ml

Instrument: ECD_O
ClientSampleId: AR1242ICC500

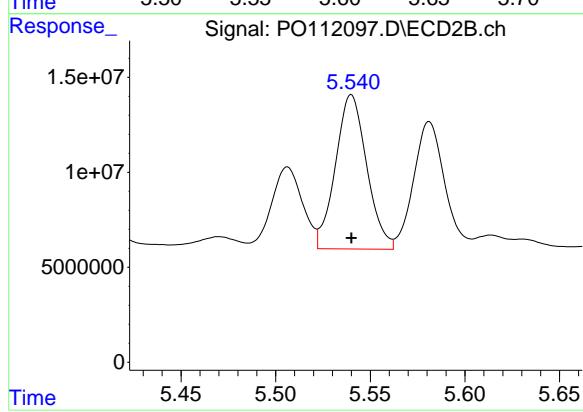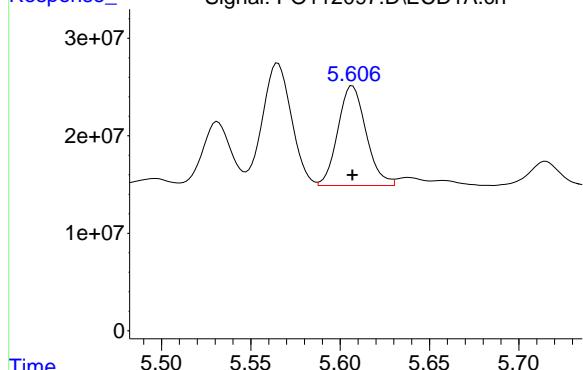

#20 AR-1242-5

R.T.: 5.540 min
Delta R.T.: 0.000 min
Response: 93535709
Conc: 500.00 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0070825\
 Data File : P0112098.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jul 2025 17:11
 Operator : YP/AJ
 Sample : AR1242ICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1242ICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 09 02:31:05 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 09 02:27:13 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	3.674	3.667	263.1E6	169.2E6	24.966	25.134
2) SA Decachlor...	8.703	8.650	178.3E6	46660840	24.893	25.927

Target Compounds

16) L4 AR-1242-1	4.761	4.744	75657146	51480221	250.034	262.447
17) L4 AR-1242-2	4.780	4.762	112.0E6	74327588	249.114	257.374
18) L4 AR-1242-3	4.837	4.937	72112951	38588282	250.935	257.234
19) L4 AR-1242-4	4.957	5.021	58094987	37459928	250.682	260.819
20) L4 AR-1242-5	5.608	5.541	57886671	49852424	257.821	266.489



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0070825\
 Data File : P0112098.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jul 2025 17:11
 Operator : YP/AJ
 Sample : AR1242ICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1242ICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 09 02:31:05 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 09 02:27:13 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ m Signal #2 Info : 30M x 0.32mm x 0.25 μ m

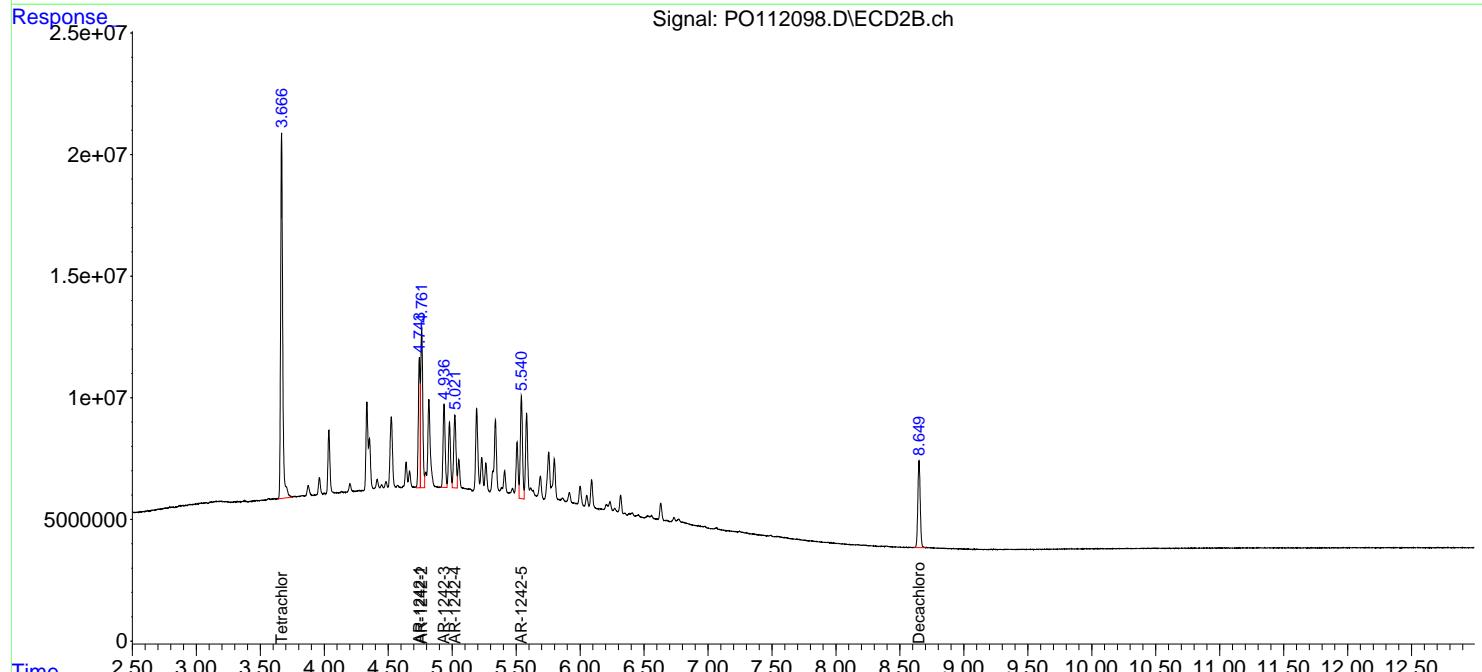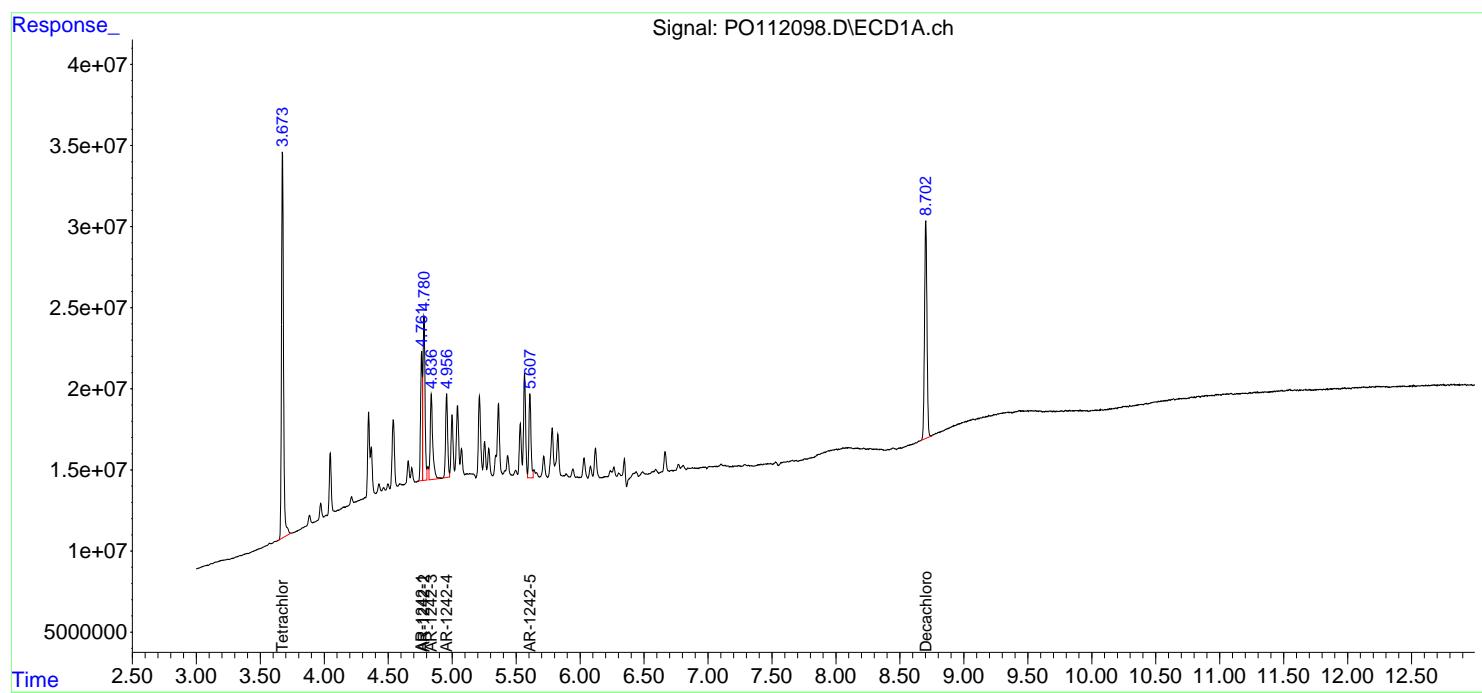

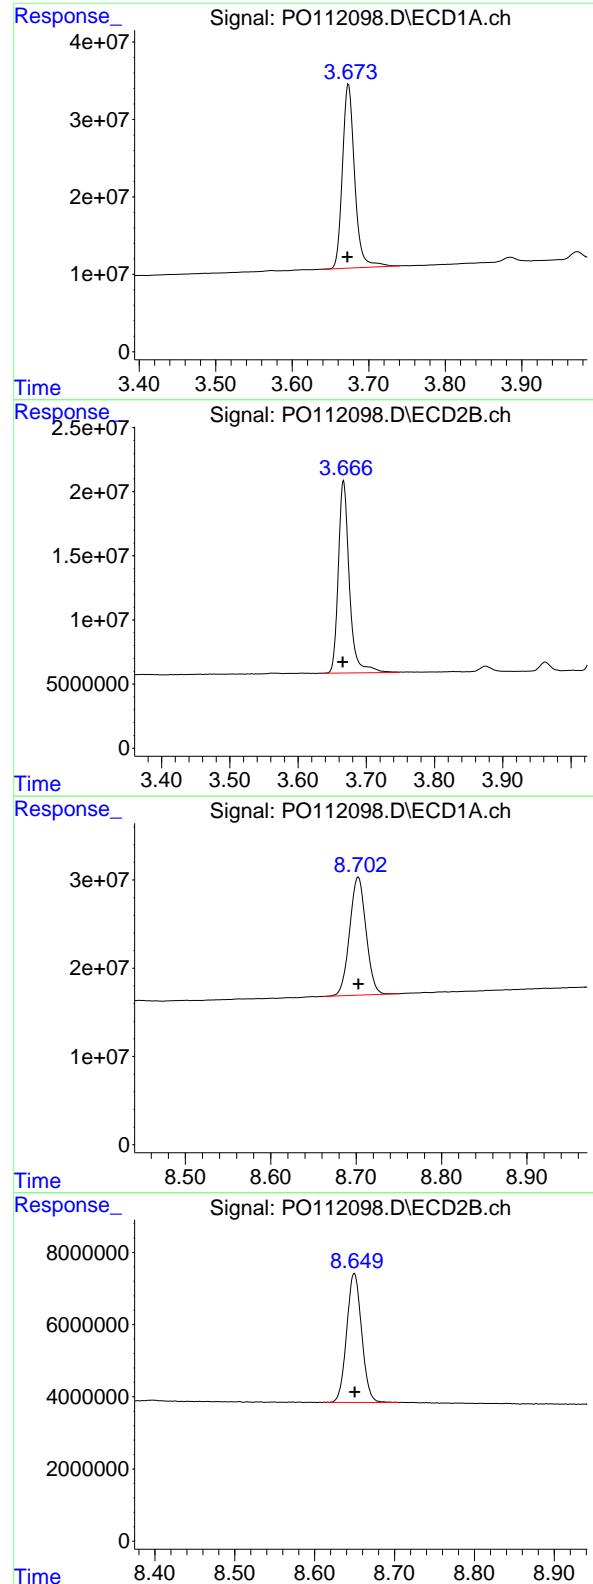

#1 Tetrachloro-m-xylene

R.T.: 3.674 min
 Delta R.T.: 0.002 min
 Response: 263100949
 Conc: 24.97 ng/ml

Instrument: ECD_O
ClientSampleId: AR1242ICC250

#1 Tetrachloro-m-xylene

R.T.: 3.667 min
 Delta R.T.: 0.000 min
 Response: 169169819
 Conc: 25.13 ng/ml

#2 Decachlorobiphenyl

R.T.: 8.703 min
 Delta R.T.: 0.000 min
 Response: 178282770
 Conc: 24.89 ng/ml


#2 Decachlorobiphenyl

R.T.: 8.650 min
 Delta R.T.: 0.000 min
 Response: 46660840
 Conc: 25.93 ng/ml

#16 AR-1242-1


R.T.: 4.761 min
 Delta R.T.: 0.002 min
 Response: 75657146
 Conc: 250.03 ng/ml

Instrument: ECD_O
ClientSampleId: AR1242ICC250




#16 AR-1242-1

R.T.: 4.744 min
 Delta R.T.: 0.002 min
 Response: 51480221
 Conc: 262.45 ng/ml

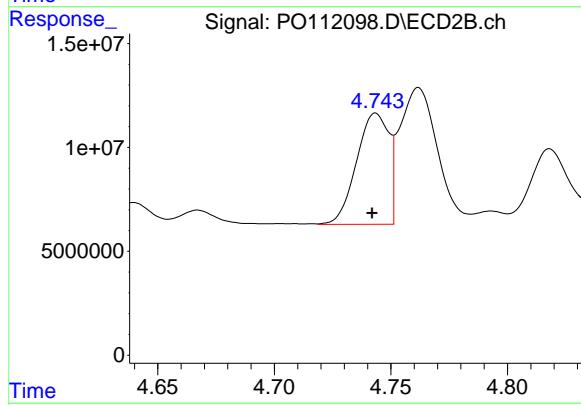


#17 AR-1242-2

R.T.: 4.780 min
 Delta R.T.: 0.002 min
 Response: 111991988
 Conc: 249.11 ng/ml

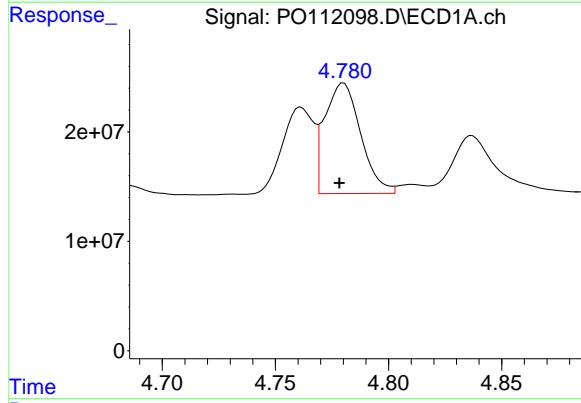

#17 AR-1242-2





R.T.: 4.762 min
 Delta R.T.: 0.002 min
 Response: 74327588
 Conc: 257.37 ng/ml

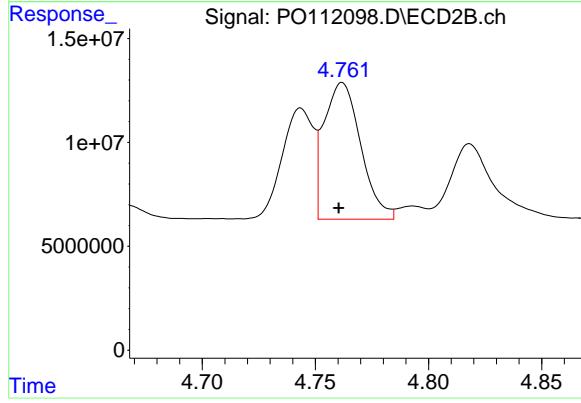

#18 AR-1242-3

R.T.: 4.837 min
 Delta R.T.: 0.002 min
 Response: 72112951
 Conc: 250.93 ng/ml

Instrument: ECD_O
 ClientSampleId: AR1242ICC250

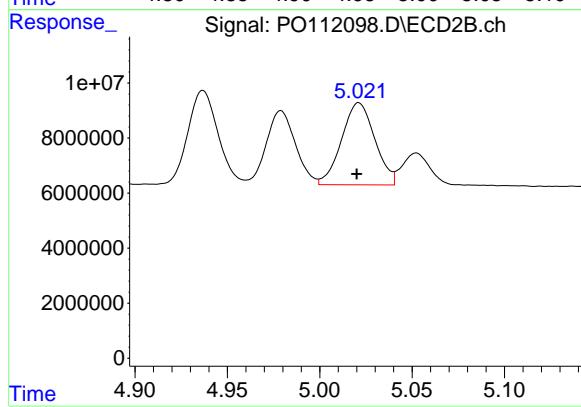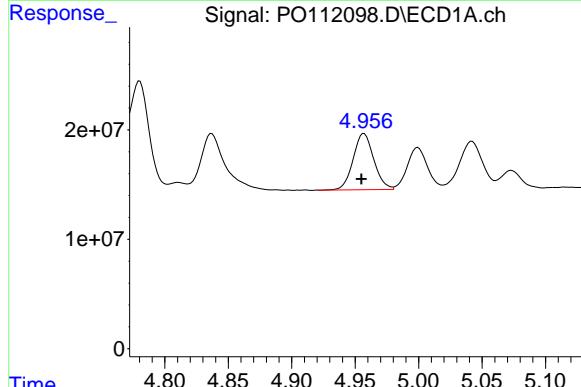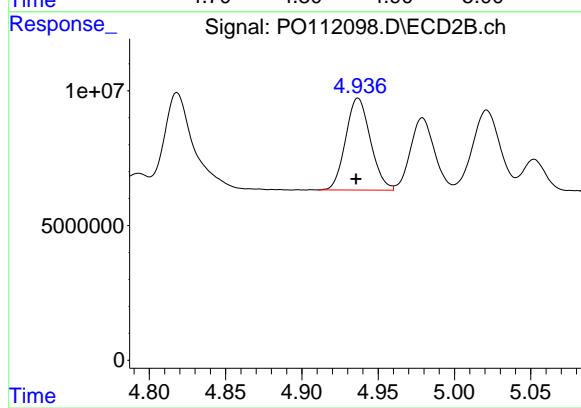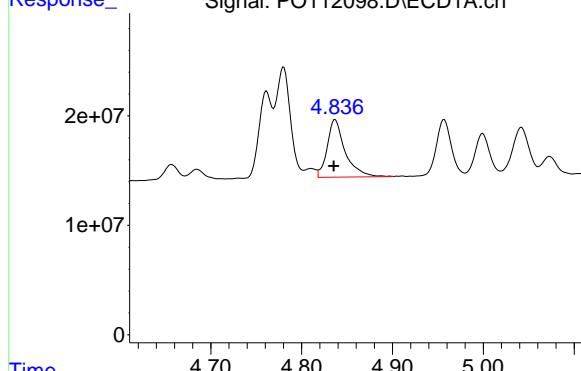

#18 AR-1242-3

R.T.: 4.937 min
 Delta R.T.: 0.001 min
 Response: 38588282
 Conc: 257.23 ng/ml

#19 AR-1242-4

R.T.: 4.957 min
 Delta R.T.: 0.002 min
 Response: 58094987
 Conc: 250.68 ng/ml



#19 AR-1242-4

R.T.: 5.021 min
 Delta R.T.: 0.001 min
 Response: 37459928
 Conc: 260.82 ng/ml

#20 AR-1242-5

R.T.: 5.608 min
Delta R.T.: 0.000 min
Response: 57886671
Conc: 257.82 ng/ml

Instrument: ECD_O
ClientSampleId: AR1242ICC250

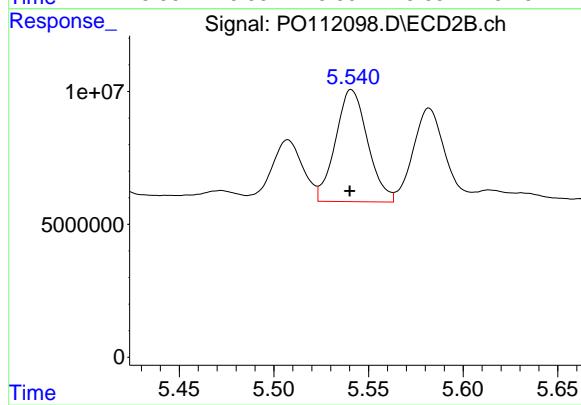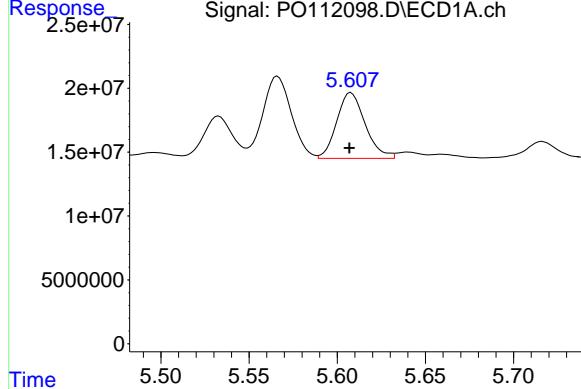

#20 AR-1242-5

R.T.: 5.541 min
Delta R.T.: 0.001 min
Response: 49852424
Conc: 266.49 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0070825\
 Data File : P0112099.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jul 2025 17:29
 Operator : YP/AJ
 Sample : AR1242ICC050
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1242ICC050

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/09/2025
 Supervised By :mohammad ahmed 07/10/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 09 02:31:15 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 09 02:27:13 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	3.673	3.666	42912716	27696407	4.072	4.115
2) SA Decachlor...	8.704	8.650	28291682	7899910	3.950	4.390

Target Compounds

16) L4 AR-1242-1	4.761	4.743	12609363	9619088	41.672	49.038
17) L4 AR-1242-2	4.780	4.761	17776215	13881256	39.541	48.067
18) L4 AR-1242-3	4.837	4.937	12004480	6736786	41.773	44.908
19) L4 AR-1242-4	4.957	5.021	10638220	7029005	45.904	48.940
20) L4 AR-1242-5	5.608	5.541	7571568	8542753	33.723m	45.666m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0070825\
 Data File : P0112099.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jul 2025 17:29
 Operator : YP/AJ
 Sample : AR1242ICC050
 Misc :
 ALS Vial : 14 Sample Multiplier: 1



Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 09 02:31:15 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 09 02:27:13 2025
 Response via : Initial Calibration
 Integrator: ChemStation





Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Instrument :
 ECD_O
ClientSampleId :
 AR1242ICC050

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/09/2025
 Supervised By :mohammad ahmed 07/10/2025

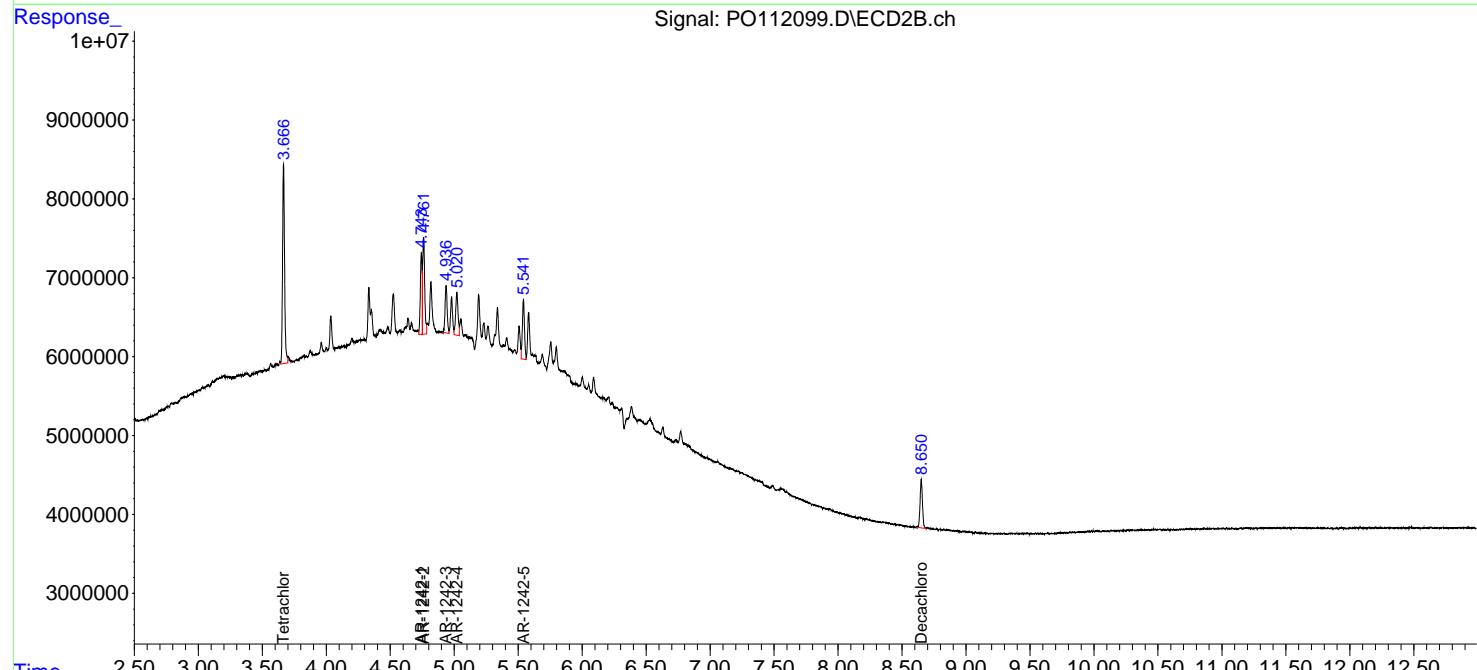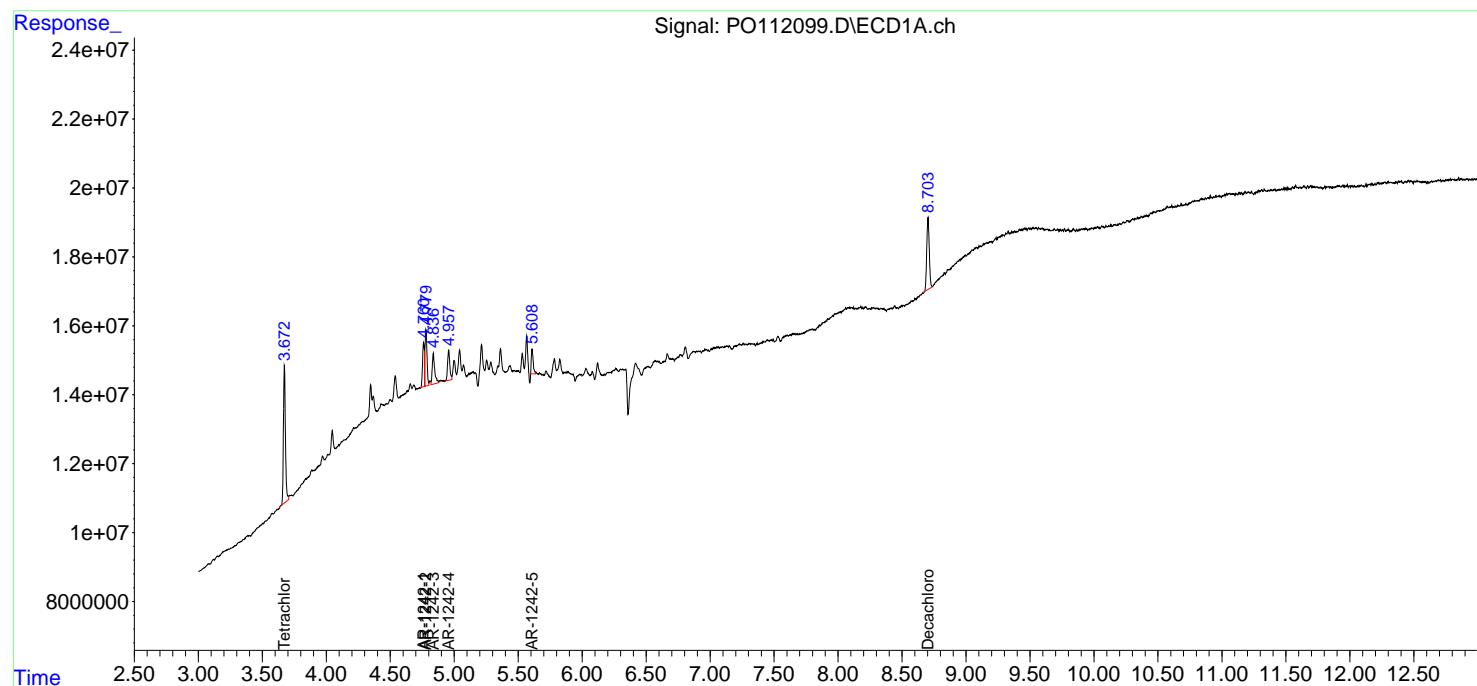

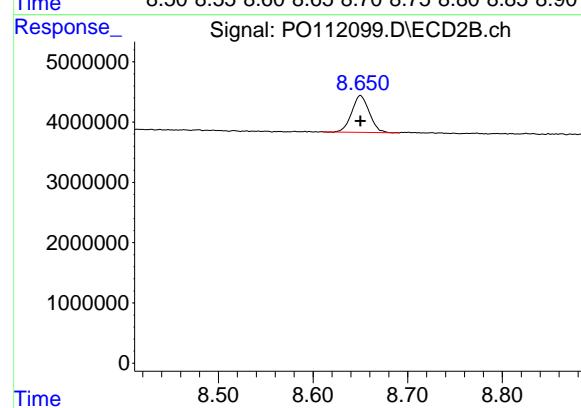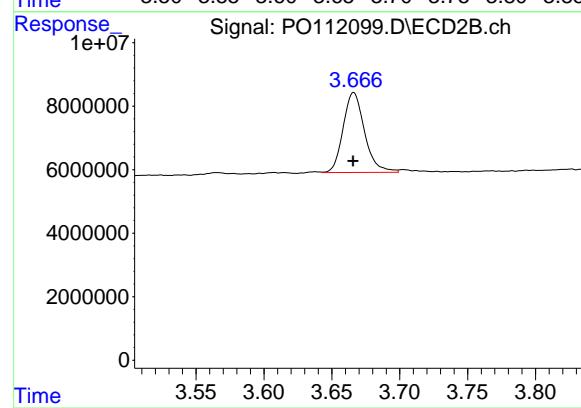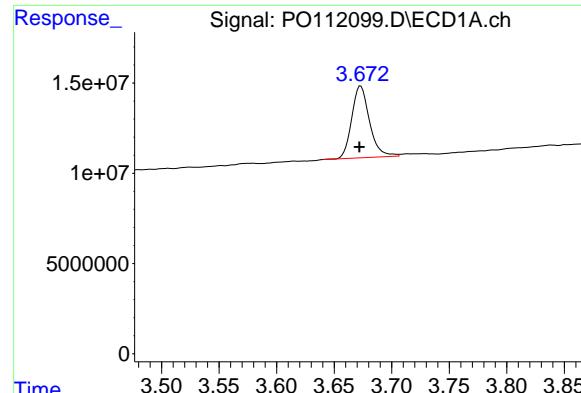

#1 Tetrachloro-m-xylene

R.T.: 3.673 min
Delta R.T.: 0.000 min
Response: 42912716
Conc: 4.07 ng/ml

Instrument:
ECD_O
ClientSampleId :
AR1242ICC050

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/09/2025
Supervised By :mohammad ahmed 07/10/2025

#1 Tetrachloro-m-xylene


R.T.: 3.666 min
Delta R.T.: 0.000 min
Response: 27696407
Conc: 4.11 ng/ml

#2 Decachlorobiphenyl

R.T.: 8.704 min
Delta R.T.: 0.000 min
Response: 28291682
Conc: 3.95 ng/ml

#2 Decachlorobiphenyl

R.T.: 8.650 min
Delta R.T.: 0.000 min
Response: 7899910
Conc: 4.39 ng/ml

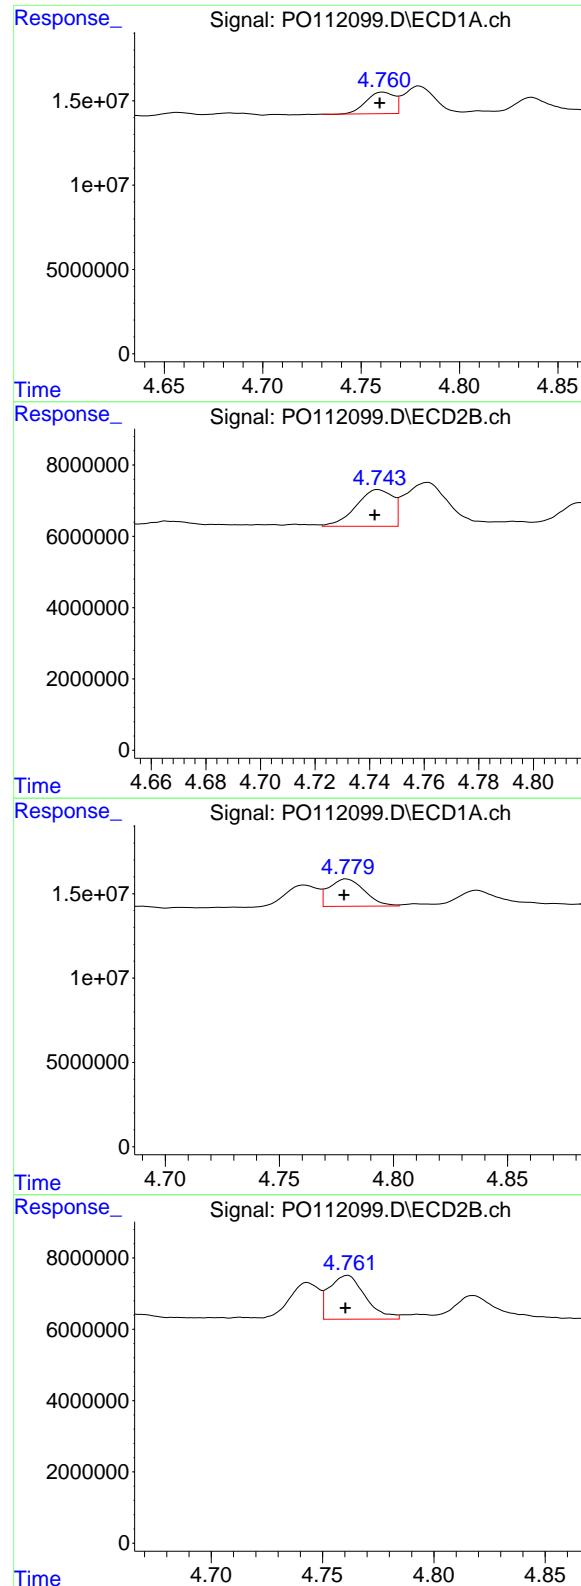

#16 AR-1242-1

R.T.: 4.761 min
 Delta R.T.: 0.002 min
 Response: 12609363
 Conc: 41.67 ng/ml

Instrument: ECD_O
ClientSampleId: AR1242ICC050

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/09/2025
 Supervised By :mohammad ahmed 07/10/2025

#16 AR-1242-1

R.T.: 4.743 min
 Delta R.T.: 0.001 min
 Response: 9619088
 Conc: 49.04 ng/ml

#17 AR-1242-2

R.T.: 4.780 min
 Delta R.T.: 0.001 min
 Response: 17776215
 Conc: 39.54 ng/ml

#17 AR-1242-2

R.T.: 4.761 min
 Delta R.T.: 0.001 min
 Response: 13881256
 Conc: 48.07 ng/ml

#18 AR-1242-3

R.T.: 4.837 min
 Delta R.T.: 0.002 min
 Response: 12004480
 Conc: 41.77 ng/ml

Instrument: ECD_O
ClientSampleId: AR1242ICC050

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/09/2025
 Supervised By :mohammad ahmed 07/10/2025

#18 AR-1242-3





R.T.: 4.937 min
 Delta R.T.: 0.000 min
 Response: 6736786
 Conc: 44.91 ng/ml

#19 AR-1242-4

R.T.: 4.957 min
 Delta R.T.: 0.002 min
 Response: 10638220
 Conc: 45.90 ng/ml

#19 AR-1242-4

R.T.: 5.021 min
 Delta R.T.: 0.000 min
 Response: 7029005
 Conc: 48.94 ng/ml

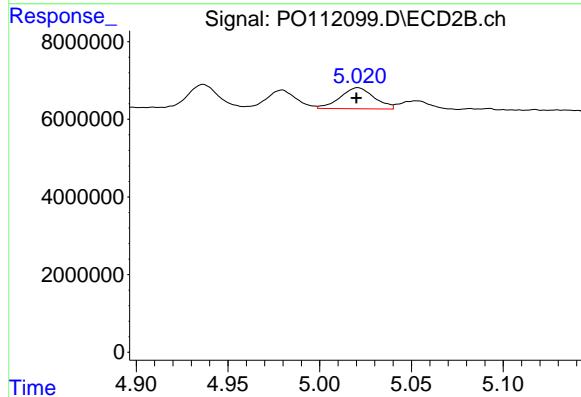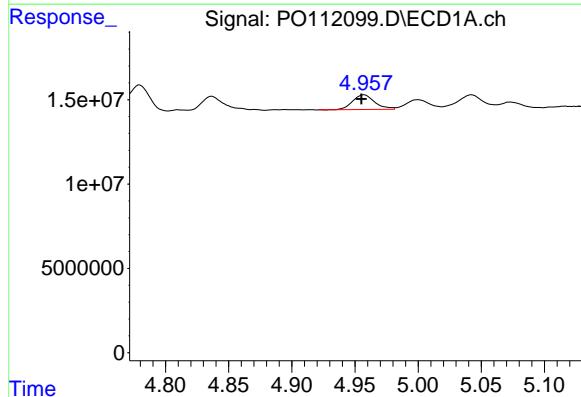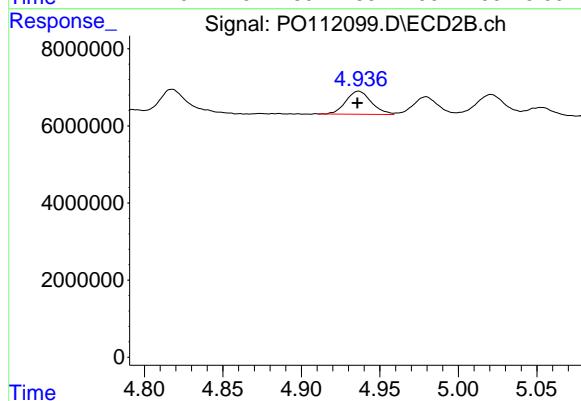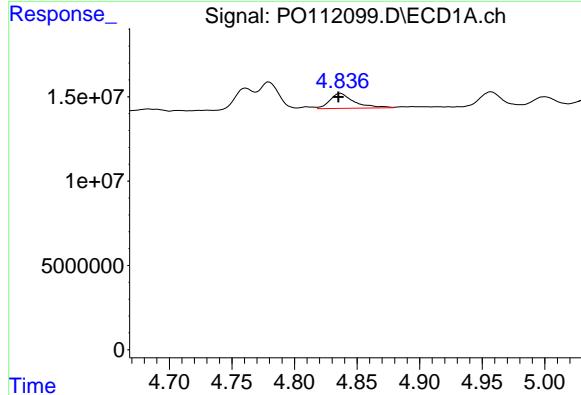


#20 AR-1242-5

R.T.: 5.608 min
 Delta R.T.: 0.000 min
 Response: 7571568
 Conc: 33.72 ng/ml

Instrument: ECD_O
ClientSampleId: AR1242ICC050

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/09/2025
 Supervised By :mohammad ahmed 07/10/2025

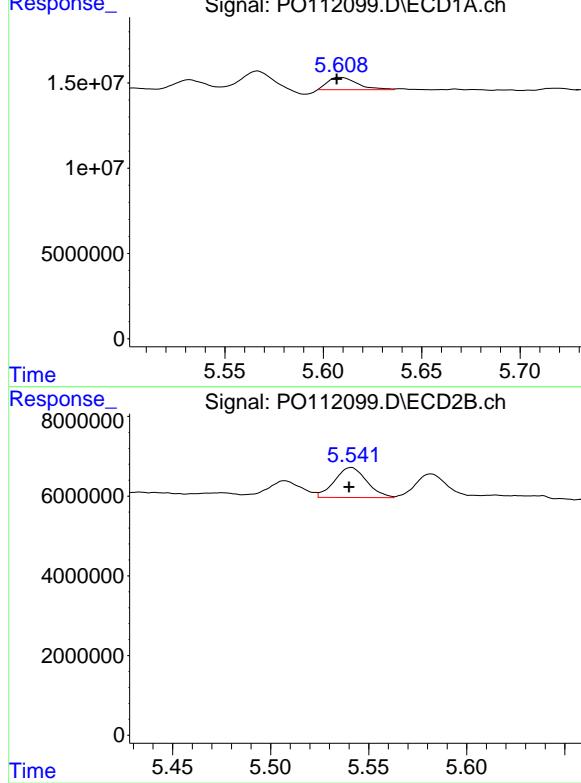

#20 AR-1242-5

R.T.: 5.541 min
 Delta R.T.: 0.001 min
 Response: 8542753
 Conc: 45.67 ng/ml

1
2
3
4
5
6
7
8
9
10
11
12
13
14
15
16
17
18
19
20

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0070825\
 Data File : P0112100.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jul 2025 17:48
 Operator : YP/AJ
 Sample : AR1248ICC1000
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1248ICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 09 02:45:01 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 09 02:41:59 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	3.672	3.666	1096.6E6	692.2E6	104.113	104.038
2) SA Decachlor...	8.704	8.650	716.5E6	174.1E6	98.706	94.881

Target Compounds

21) L5 AR-1248-1	4.760	4.743	231.9E6	148.4E6	1018.654	991.552
22) L5 AR-1248-2	4.999	4.978	312.2E6	200.2E6	1016.179	985.440
23) L5 AR-1248-3	5.213	5.020	394.9E6	210.9E6	1005.052	990.919
24) L5 AR-1248-4	5.566	5.190	577.1E6	249.5E6	1002.758	984.112
25) L5 AR-1248-5	5.607	5.581	391.1E6	244.4E6	1001.154	973.721



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0070825\
 Data File : P0112100.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jul 2025 17:48
 Operator : YP/AJ
 Sample : AR1248ICC1000
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1248ICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 09 02:45:01 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 09 02:41:59 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

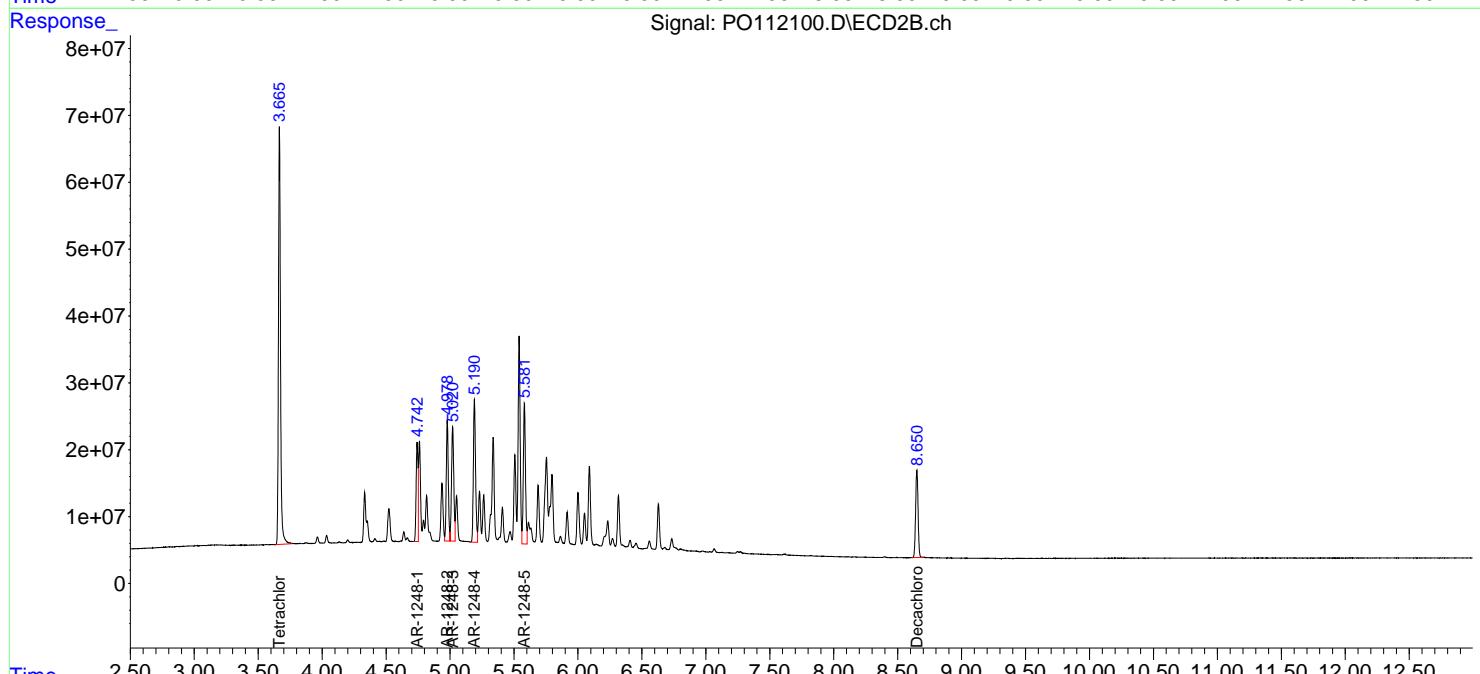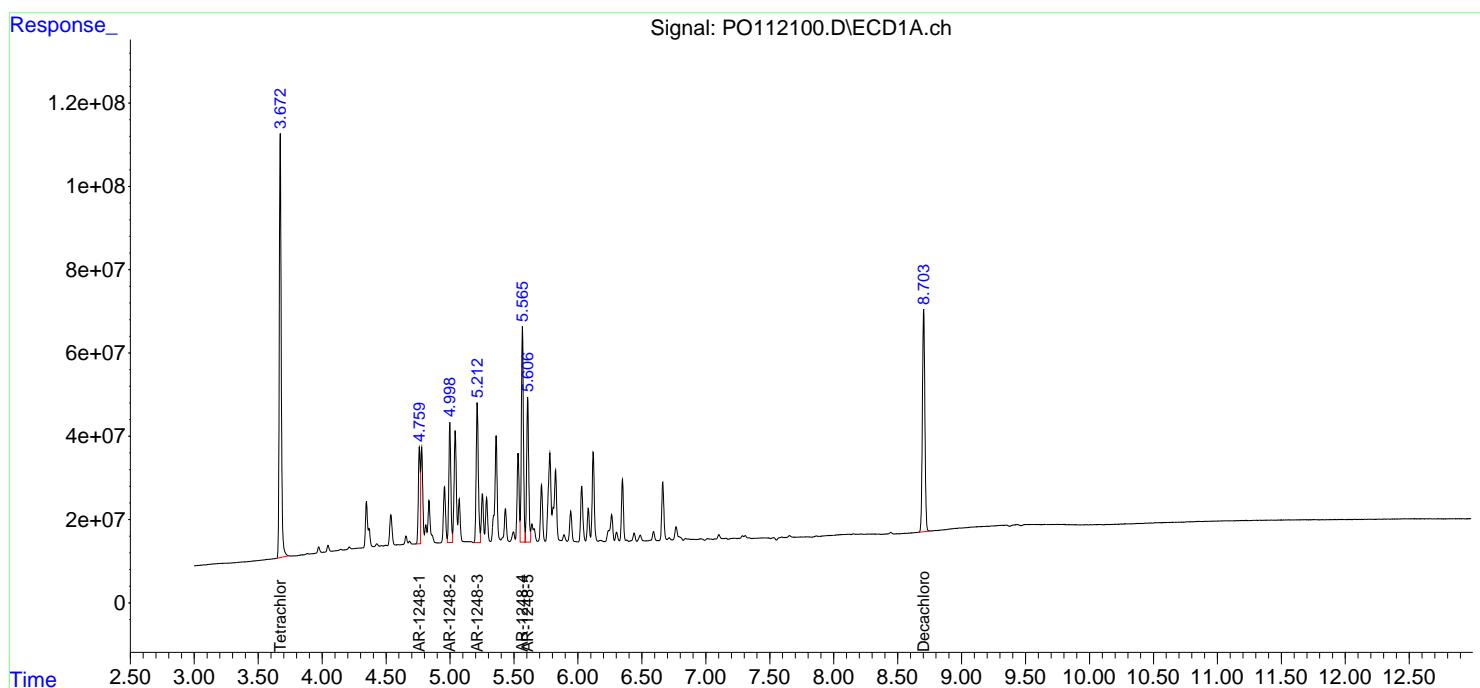

#1 Tetrachloro-m-xylene

R.T.: 3.672 min


Delta R.T.: -0.002 min

Instrument: ECD_O

Response: 1096626081

Conc: 104.11 ng/ml

ClientSampleId: AR1248ICC1000

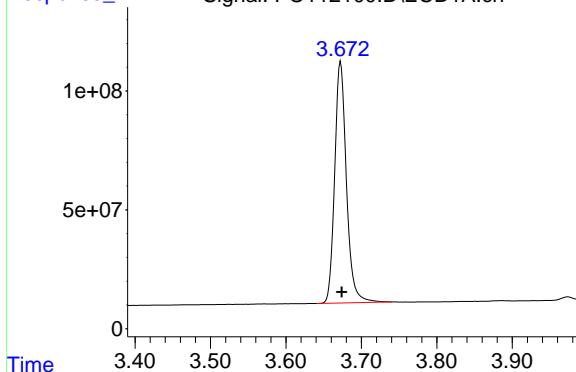


#1 Tetrachloro-m-xylene

R.T.: 3.666 min

Delta R.T.: -0.001 min

Response: 692202944

Conc: 104.04 ng/ml

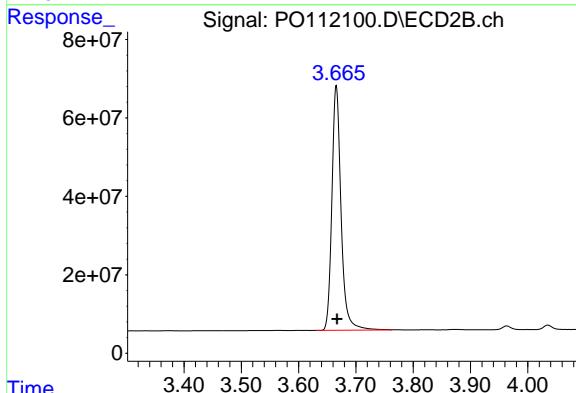


#2 Decachlorobiphenyl

R.T.: 8.704 min

Delta R.T.: 0.001 min

Response: 716466971

Conc: 98.71 ng/ml

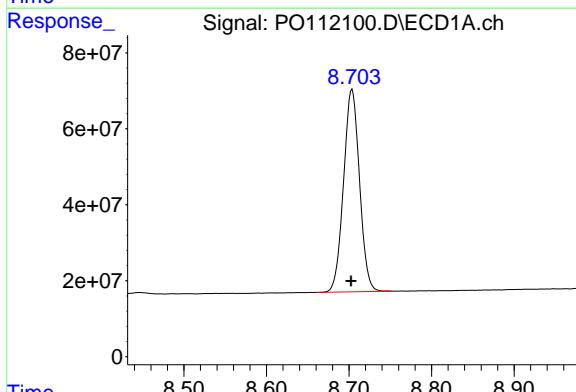


#2 Decachlorobiphenyl

R.T.: 8.650 min

Delta R.T.: 0.000 min


Response: 174100498

Conc: 94.88 ng/ml

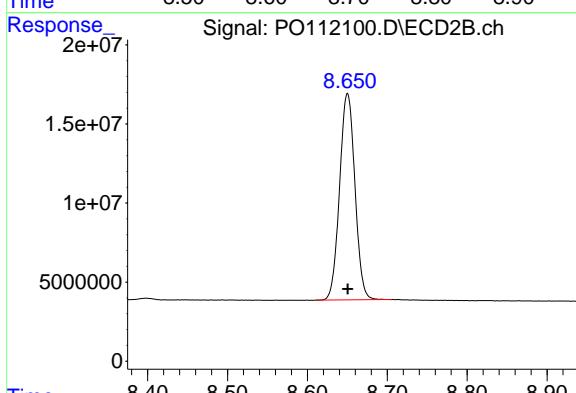


#21 AR-1248-1

R.T.: 4.760 min
 Delta R.T.: -0.001 min
 Response: 231871262
 Conc: 1018.65 ng/ml
Instrument: ECD_O
ClientSampleId: AR1248ICC1000




#21 AR-1248-1

R.T.: 4.743 min
 Delta R.T.: 0.000 min
 Response: 148373409
 Conc: 991.55 ng/ml

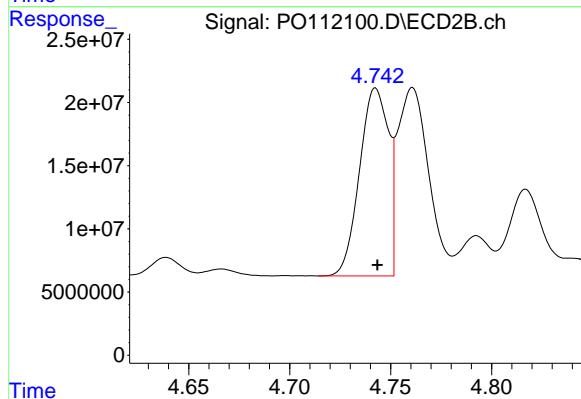


#22 AR-1248-2

R.T.: 4.999 min
 Delta R.T.: -0.001 min
 Response: 312226784
 Conc: 1016.18 ng/ml

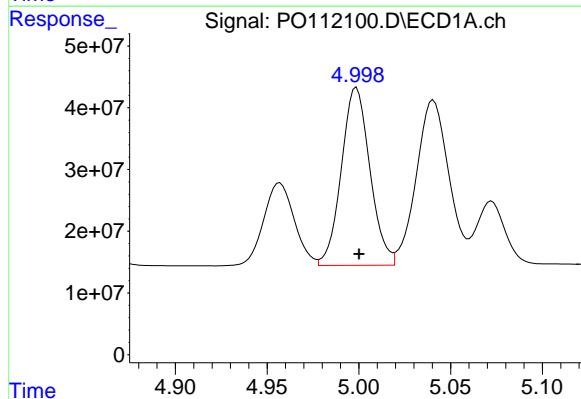

#22 AR-1248-2





R.T.: 4.978 min
 Delta R.T.: -0.001 min
 Response: 200165378
 Conc: 985.44 ng/ml

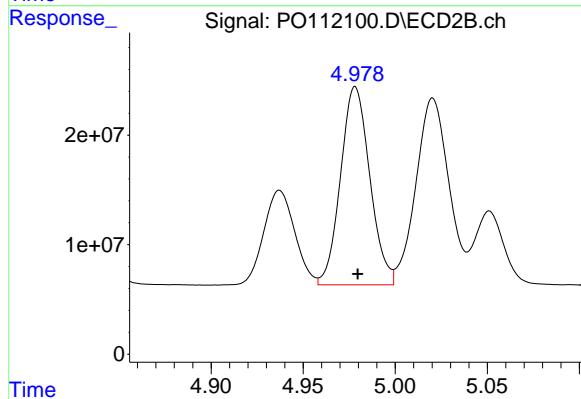

#23 AR-1248-3

R.T.: 5.213 min
 Delta R.T.: -0.002 min
 Response: 394903515
 Conc: 1005.05 ng/ml

Instrument: ECD_O
ClientSampleId: AR1248ICC1000

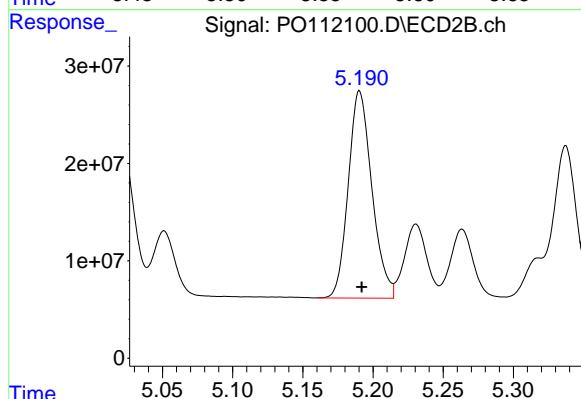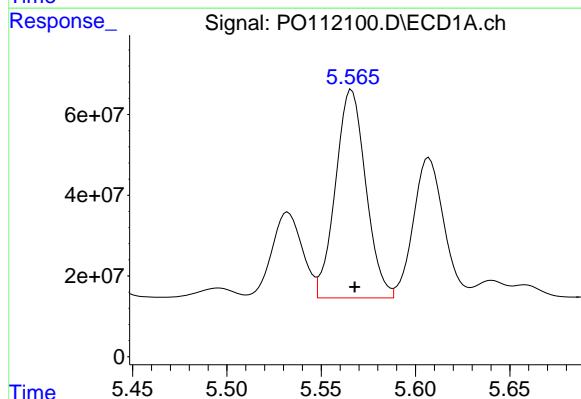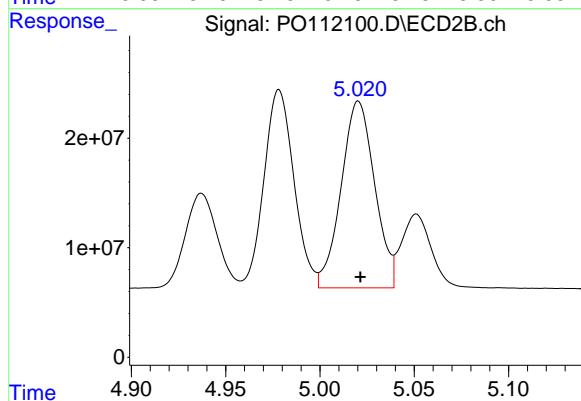

#23 AR-1248-3

R.T.: 5.020 min
 Delta R.T.: -0.001 min
 Response: 210851108
 Conc: 990.92 ng/ml

#24 AR-1248-4



R.T.: 5.566 min
 Delta R.T.: -0.002 min
 Response: 577144829
 Conc: 1002.76 ng/ml

#24 AR-1248-4

R.T.: 5.190 min
 Delta R.T.: -0.002 min
 Response: 249491134
 Conc: 984.11 ng/ml

#25 AR-1248-5

R.T.: 5.607 min
Delta R.T.: -0.002 min
Response: 391149352
Conc: 1001.15 ng/ml
Instrument: ECD_O
ClientSampleId: AR1248ICC1000

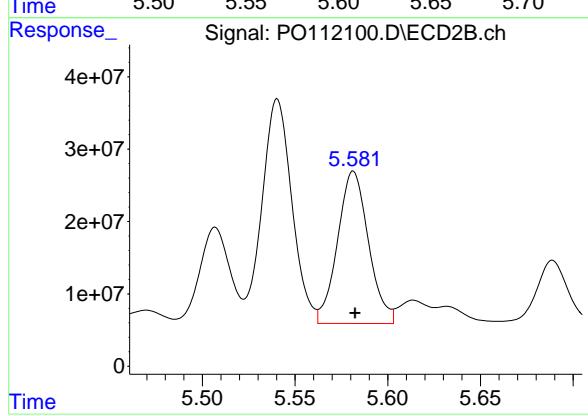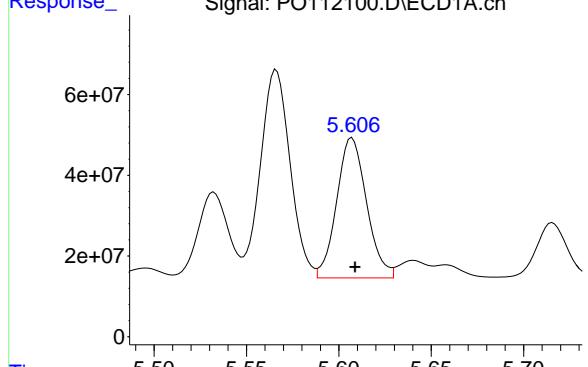

#25 AR-1248-5

R.T.: 5.581 min
Delta R.T.: 0.000 min
Response: 244390847
Conc: 973.72 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0070825\
 Data File : P0112101.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jul 2025 18:05
 Operator : YP/AJ
 Sample : AR1248ICC750
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1248ICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 09 02:45:12 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 09 02:41:59 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	3.671	3.666	800.2E6	504.2E6	75.968	75.785
2) SA Decachlor...	8.700	8.649	537.9E6	133.0E6	74.111	72.476

Target Compounds

21) L5 AR-1248-1	4.758	4.742	170.5E6	110.1E6	748.923	735.697
22) L5 AR-1248-2	4.996	4.978	229.4E6	148.7E6	746.494	731.979
23) L5 AR-1248-3	5.211	5.020	293.7E6	156.3E6	747.424	734.330
24) L5 AR-1248-4	5.564	5.190	429.4E6	184.7E6	746.110	728.503
25) L5 AR-1248-5	5.605	5.580	293.6E6	182.5E6	751.479	727.317



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0070825\
 Data File : P0112101.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jul 2025 18:05
 Operator : YP/AJ
 Sample : AR1248ICC750
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1248ICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 09 02:45:12 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 09 02:41:59 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

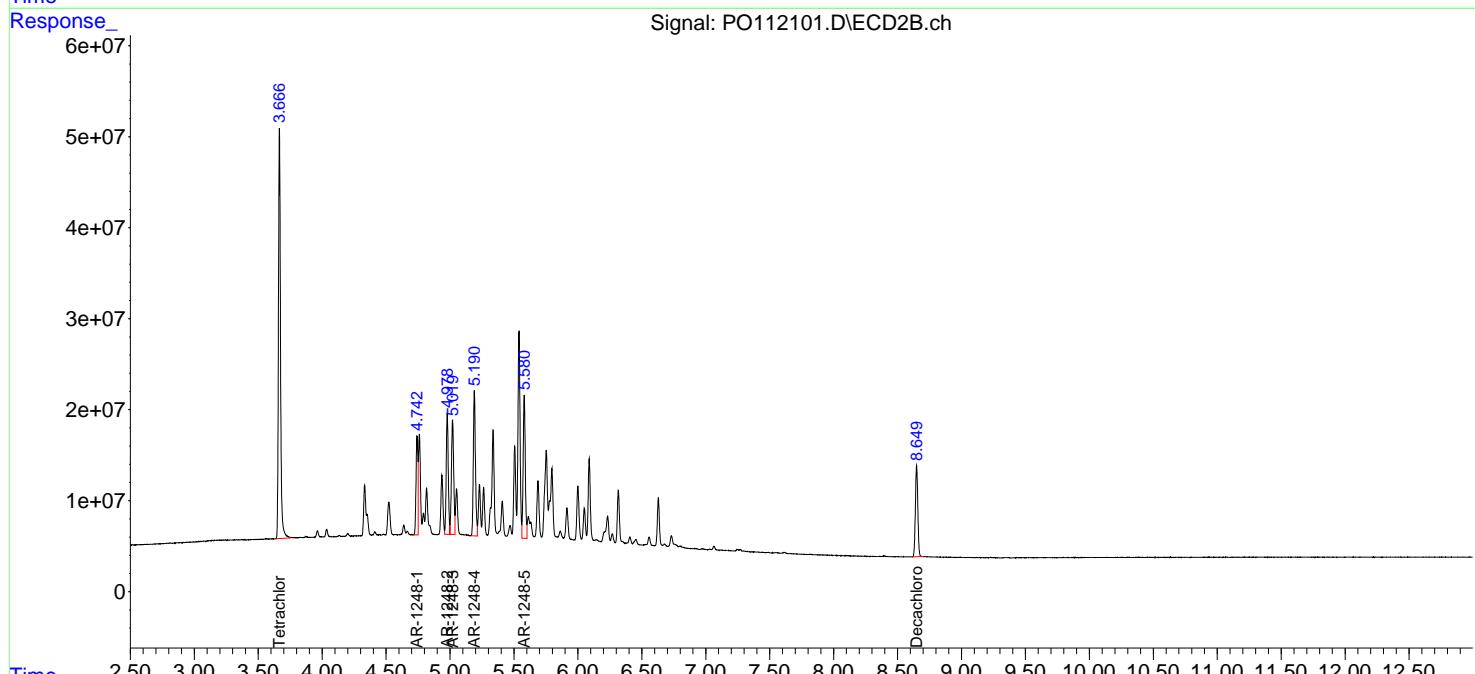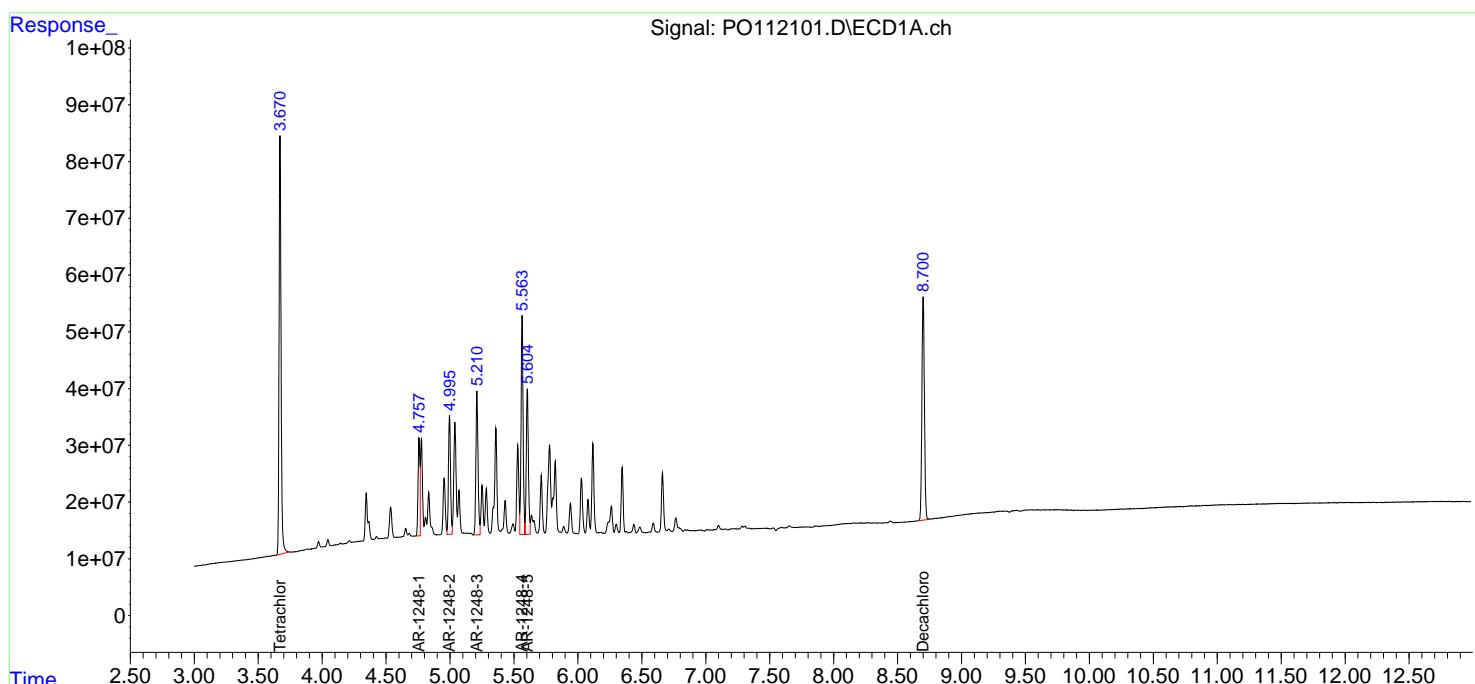

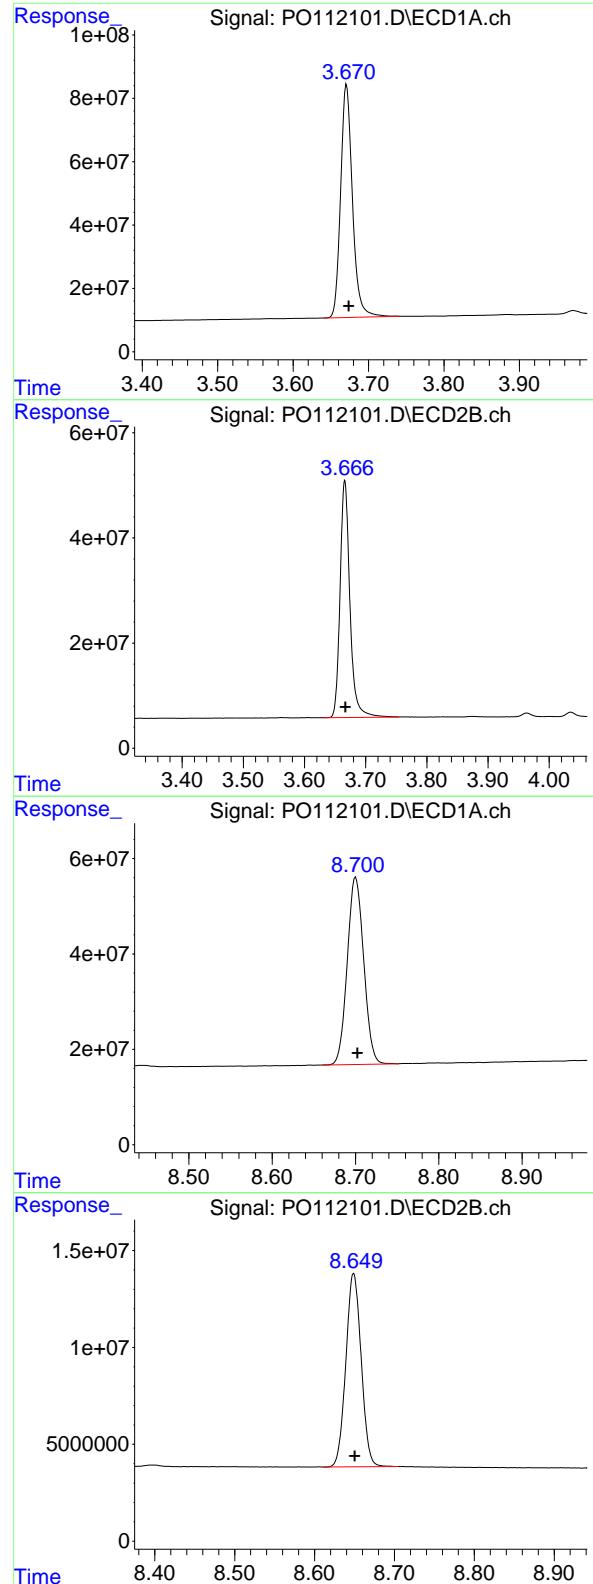

#1 Tetrachloro-m-xylene

R.T.: 3.671 min
Delta R.T.: -0.003 min
Response: 800174691
Conc: 75.97 ng/ml

Instrument: ECD_O
ClientSampleId: AR1248ICC750

#1 Tetrachloro-m-xylene

R.T.: 3.666 min
Delta R.T.: -0.001 min
Response: 504222637
Conc: 75.78 ng/ml

#2 Decachlorobiphenyl

R.T.: 8.700 min
Delta R.T.: -0.002 min
Response: 537944254
Conc: 74.11 ng/ml


#2 Decachlorobiphenyl

R.T.: 8.649 min
Delta R.T.: -0.001 min
Response: 132988512
Conc: 72.48 ng/ml

#21 AR-1248-1


R.T.: 4.758 min
 Delta R.T.: -0.003 min
 Response: 170473785
 Conc: 748.92 ng/ml

Instrument: ECD_O
ClientSampleId: AR1248ICC750




#21 AR-1248-1

R.T.: 4.742 min
 Delta R.T.: -0.001 min
 Response: 110087825
 Conc: 735.70 ng/ml

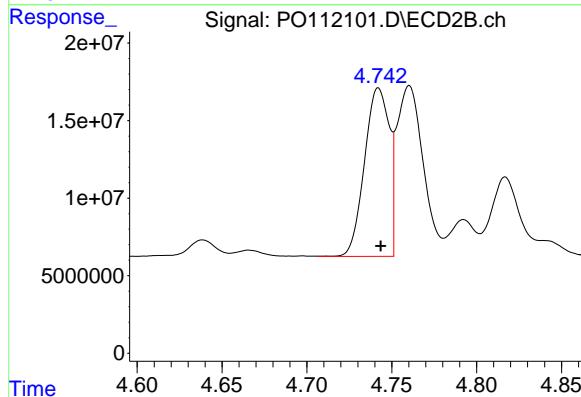


#22 AR-1248-2





R.T.: 4.996 min
 Delta R.T.: -0.004 min
 Response: 229364504
 Conc: 746.49 ng/ml

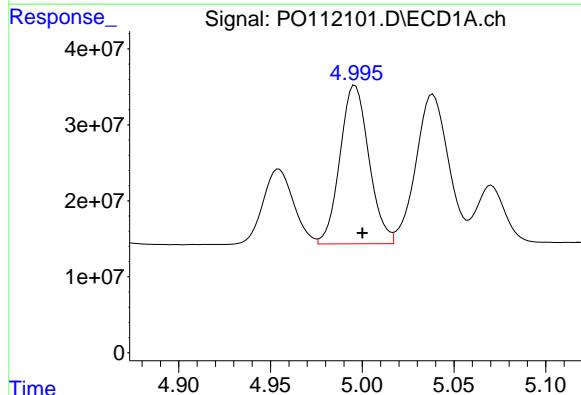

#22 AR-1248-2

R.T.: 4.978 min
 Delta R.T.: -0.001 min
 Response: 148681673
 Conc: 731.98 ng/ml

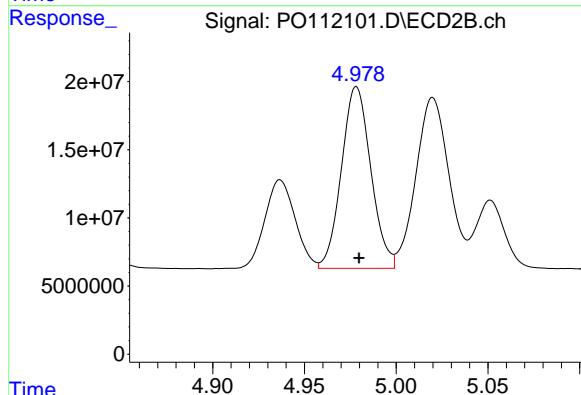

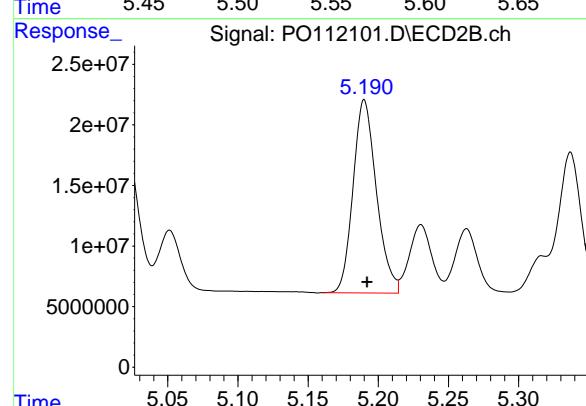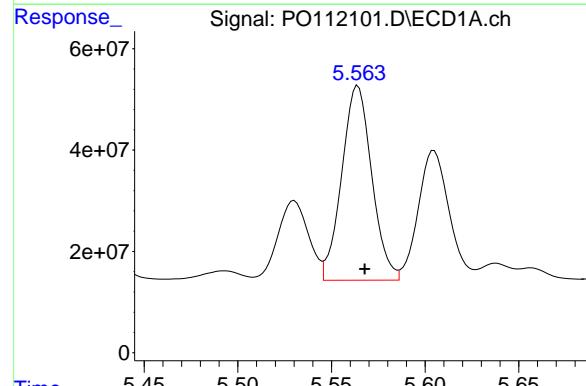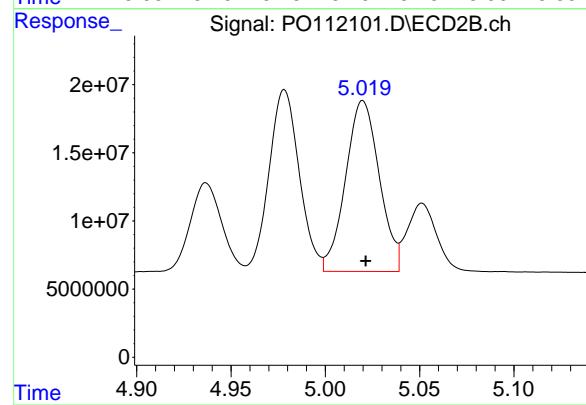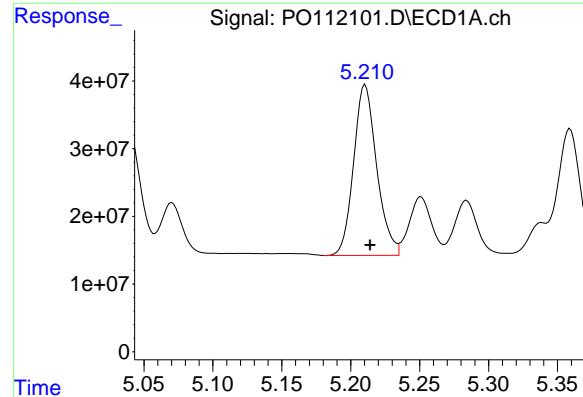

#23 AR-1248-3

R.T.: 5.211 min
 Delta R.T.: -0.004 min
 Response: 293676772
 Conc: 747.42 ng/ml

Instrument: ECD_O
ClientSampleId: AR1248ICC750

#23 AR-1248-3

R.T.: 5.020 min
 Delta R.T.: -0.002 min
 Response: 156253250
 Conc: 734.33 ng/ml

#24 AR-1248-4

R.T.: 5.564 min
 Delta R.T.: -0.004 min
 Response: 429428792
 Conc: 746.11 ng/ml



#24 AR-1248-4

R.T.: 5.190 min
 Delta R.T.: -0.002 min
 Response: 184689305
 Conc: 728.50 ng/ml

#25 AR-1248-5

R.T.: 5.605 min
Delta R.T.: -0.004 min
Response: 293601725
Conc: 751.48 ng/ml

Instrument: ECD_O
ClientSampleId: AR1248ICC750

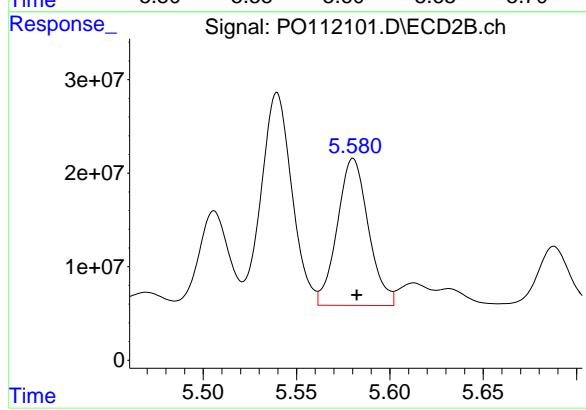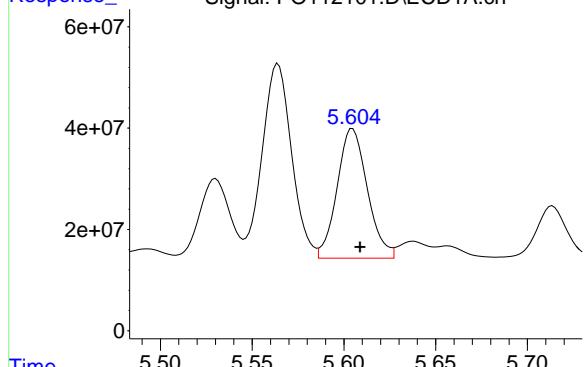

#25 AR-1248-5

R.T.: 5.580 min
Delta R.T.: -0.002 min
Response: 182546914
Conc: 727.32 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0070825\
 Data File : P0112102.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jul 2025 18:24
 Operator : YP/AJ
 Sample : AR1248ICC500
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1248ICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 09 02:45:22 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 09 02:41:59 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	3.674	3.667	526.7E6	332.7E6	50.000	50.000
2) SA Decachlor...	8.702	8.650	362.9E6	91746330	50.000	50.000

Target Compounds

21) L5 AR-1248-1	4.761	4.744	113.8E6	74818775	500.000	500.000
22) L5 AR-1248-2	5.000	4.980	153.6E6	101.6E6	500.000	500.000
23) L5 AR-1248-3	5.214	5.021	196.5E6	106.4E6	500.000	500.000
24) L5 AR-1248-4	5.568	5.192	287.8E6	126.8E6	500.000	500.000
25) L5 AR-1248-5	5.609	5.582	195.3E6	125.5E6	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0070825\
 Data File : P0112102.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jul 2025 18:24
 Operator : YP/AJ
 Sample : AR1248ICC500
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1248ICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 09 02:45:22 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 09 02:41:59 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ m Signal #2 Info : 30M x 0.32mm x 0.25 μ m

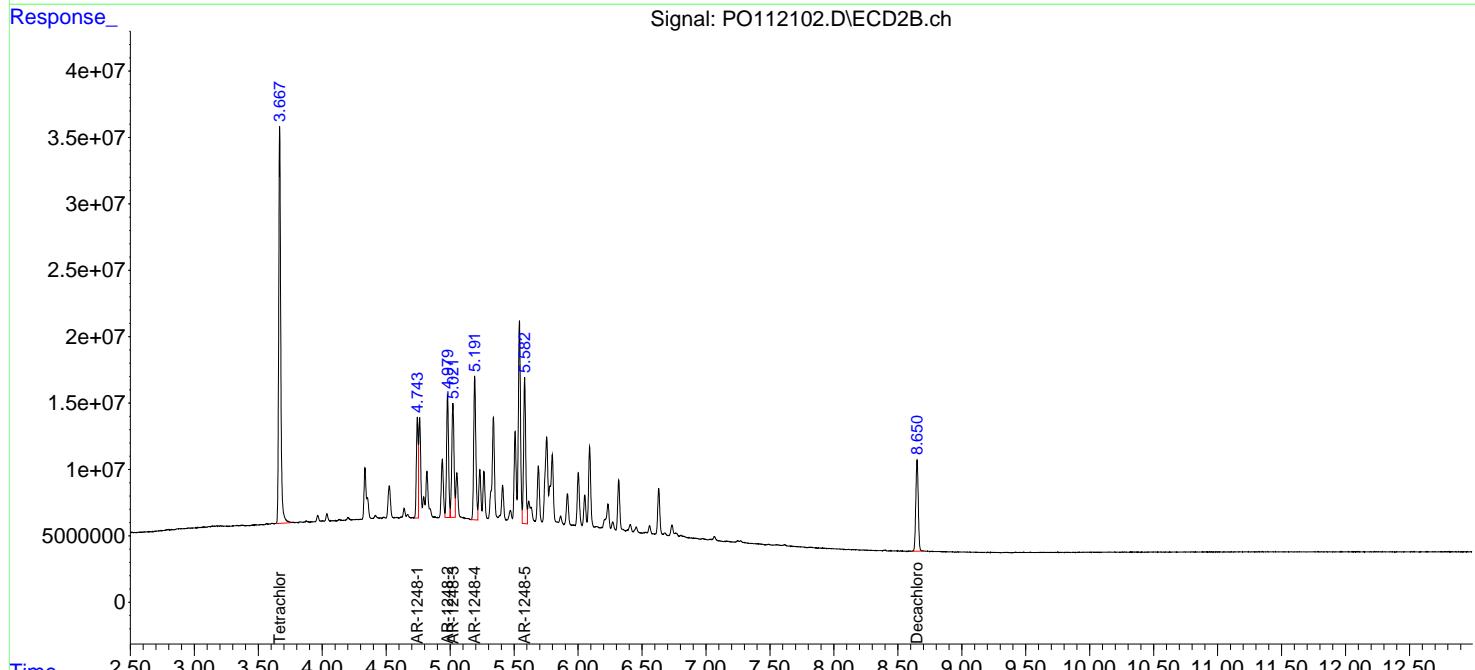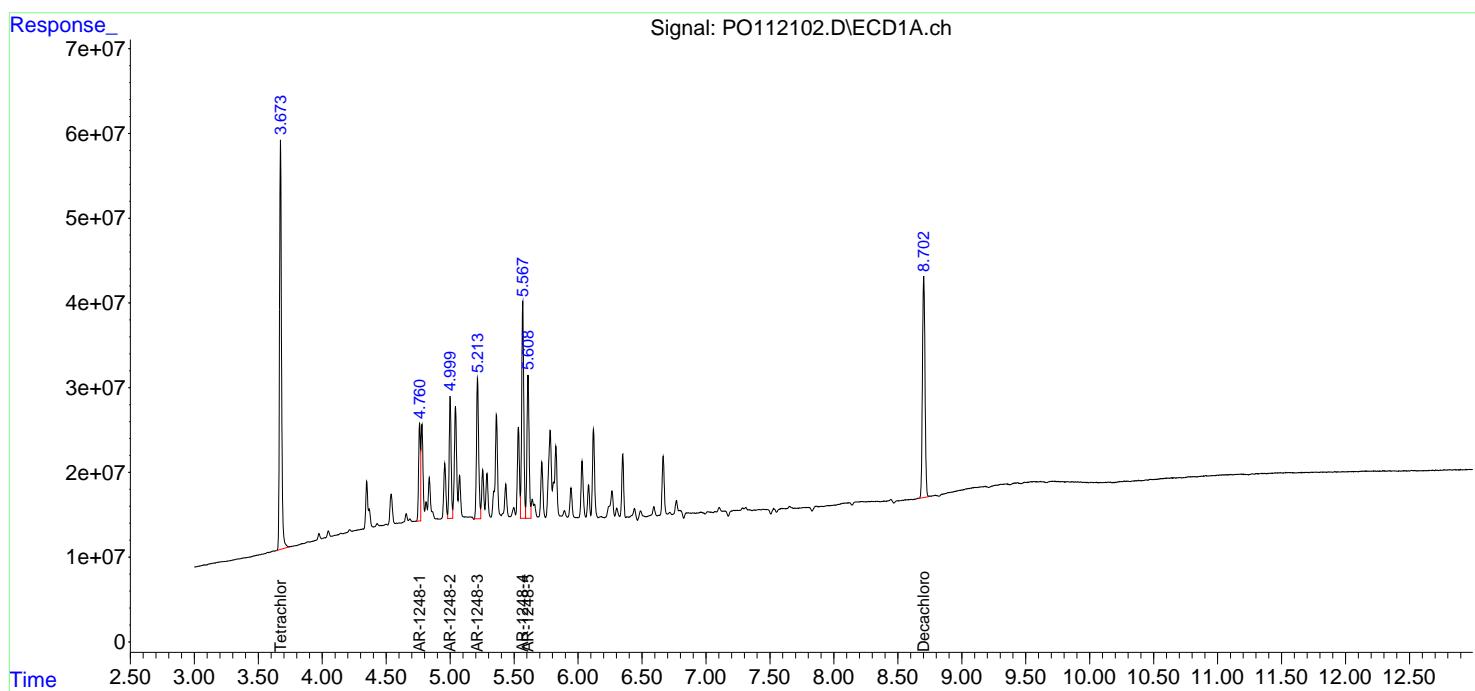

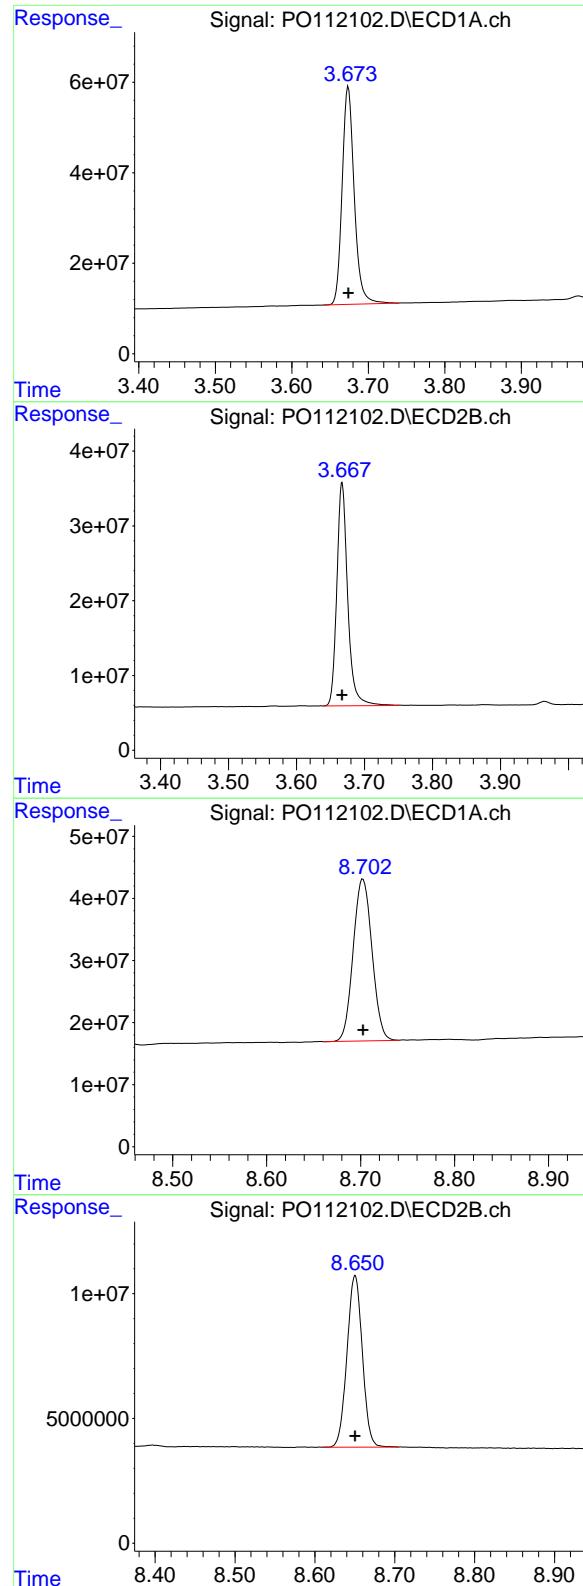

#1 Tetrachloro-m-xylene

R.T.: 3.674 min
 Delta R.T.: 0.000 min
 Response: 526650834
 Conc: 50.00 ng/ml

Instrument:

ECD_O

ClientSampleId :
AR1248ICC500

#1 Tetrachloro-m-xylene

R.T.: 3.667 min
 Delta R.T.: 0.000 min
 Response: 332667938
 Conc: 50.00 ng/ml

#2 Decachlorobiphenyl

R.T.: 8.702 min
 Delta R.T.: 0.000 min
 Response: 362930520
 Conc: 50.00 ng/ml


#2 Decachlorobiphenyl

R.T.: 8.650 min
 Delta R.T.: 0.000 min
 Response: 91746330
 Conc: 50.00 ng/ml

#21 AR-1248-1


R.T.: 4.761 min
 Delta R.T.: 0.000 min
 Response: 113812552
 Conc: 500.00 ng/ml

Instrument: ECD_O
ClientSampleId: AR1248ICC500

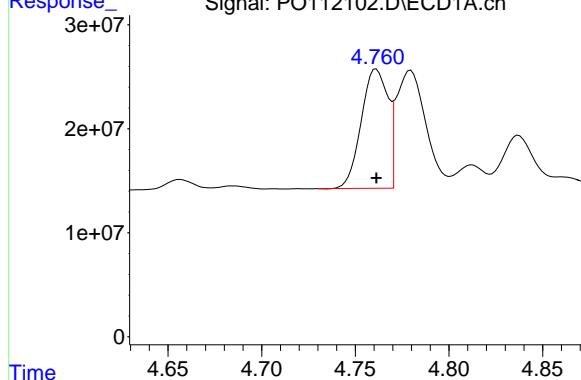


#21 AR-1248-1

R.T.: 4.744 min
 Delta R.T.: 0.000 min
 Response: 74818775
 Conc: 500.00 ng/ml

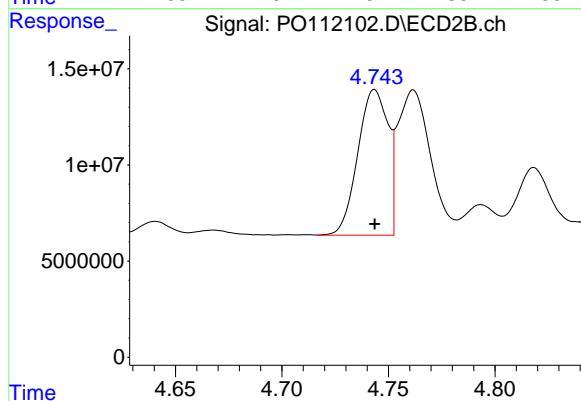


#22 AR-1248-2

R.T.: 5.000 min
 Delta R.T.: 0.000 min
 Response: 153627900
 Conc: 500.00 ng/ml

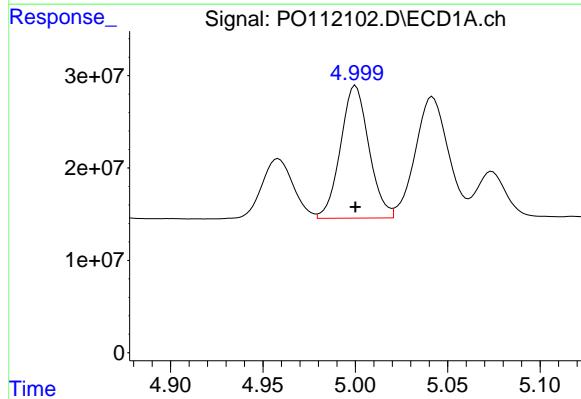

#22 AR-1248-2





R.T.: 4.980 min
 Delta R.T.: 0.000 min
 Response: 101561429
 Conc: 500.00 ng/ml

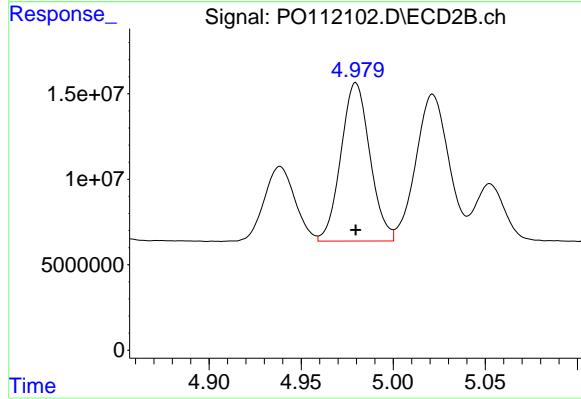

#23 AR-1248-3

R.T.: 5.214 min
 Delta R.T.: 0.000 min
 Response: 196459221
 Conc: 500.00 ng/ml

Instrument: ECD_O
ClientSampleId: AR1248ICC500

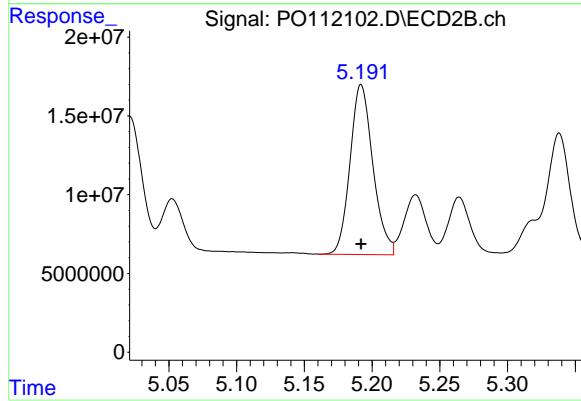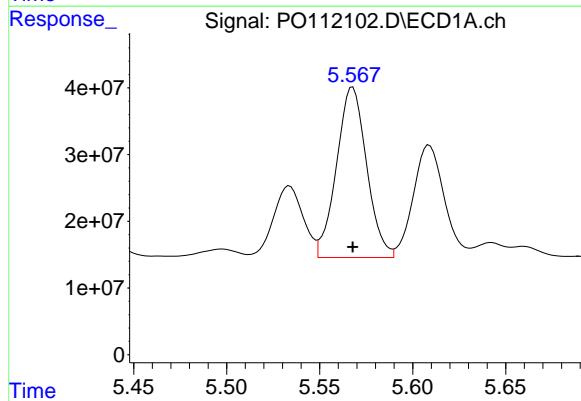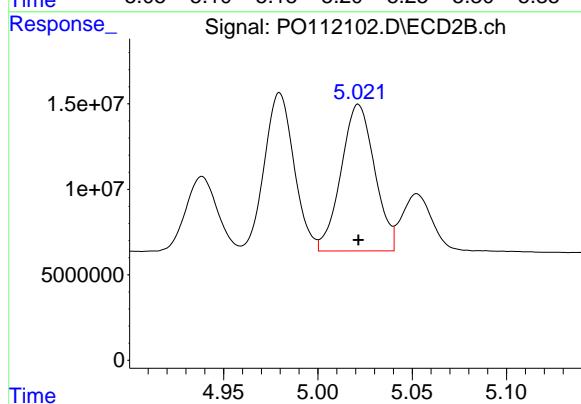

#23 AR-1248-3

R.T.: 5.021 min
 Delta R.T.: 0.000 min
 Response: 106391699
 Conc: 500.00 ng/ml

#24 AR-1248-4

R.T.: 5.568 min
 Delta R.T.: 0.000 min
 Response: 287778581
 Conc: 500.00 ng/ml



#24 AR-1248-4

R.T.: 5.192 min
 Delta R.T.: 0.000 min
 Response: 126759508
 Conc: 500.00 ng/ml

#25 AR-1248-5

R.T.: 5.609 min
Delta R.T.: 0.000 min
Response: 195349183
Conc: 500.00 ng/ml

Instrument: ECD_O
ClientSampleId: AR1248ICC500

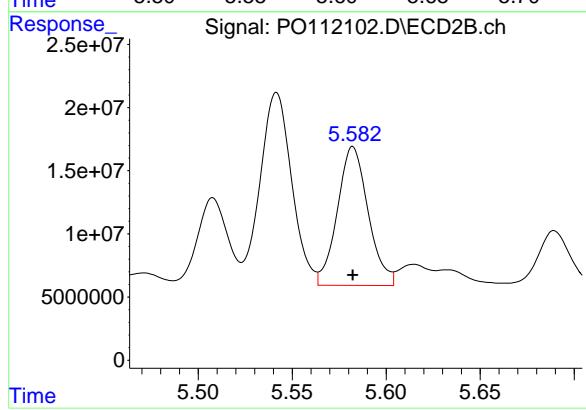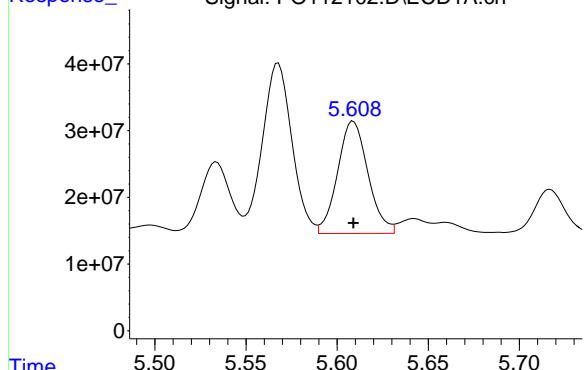

#25 AR-1248-5

R.T.: 5.582 min
Delta R.T.: 0.000 min
Response: 125493298
Conc: 500.00 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0070825\
 Data File : P0112103.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jul 2025 18:41
 Operator : YP/AJ
 Sample : AR1248ICC250
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1248ICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 09 02:45:32 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 09 02:41:59 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	3.671	3.666	291.9E6	186.4E6	27.709	28.020
2) SA Decachlor...	8.702	8.649	189.2E6	49988120	26.067	27.243

Target Compounds

21) L5 AR-1248-1	4.759	4.742	62843351	43399528	276.083	290.031
22) L5 AR-1248-2	4.997	4.978	87401333	57560333	284.458	283.377
23) L5 AR-1248-3	5.211	5.020	114.9E6	60695146	292.428	285.244
24) L5 AR-1248-4	5.565	5.190	153.8E6	74439996	267.224	293.627
25) L5 AR-1248-5	5.606	5.581	108.9E6	74875919	278.783	298.326



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.





Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0070825\
 Data File : P0112103.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jul 2025 18:41
 Operator : YP/AJ
 Sample : AR1248ICC250
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1248ICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 09 02:45:32 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 09 02:41:59 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ m Signal #2 Info : 30M x 0.32mm x 0.25 μ m

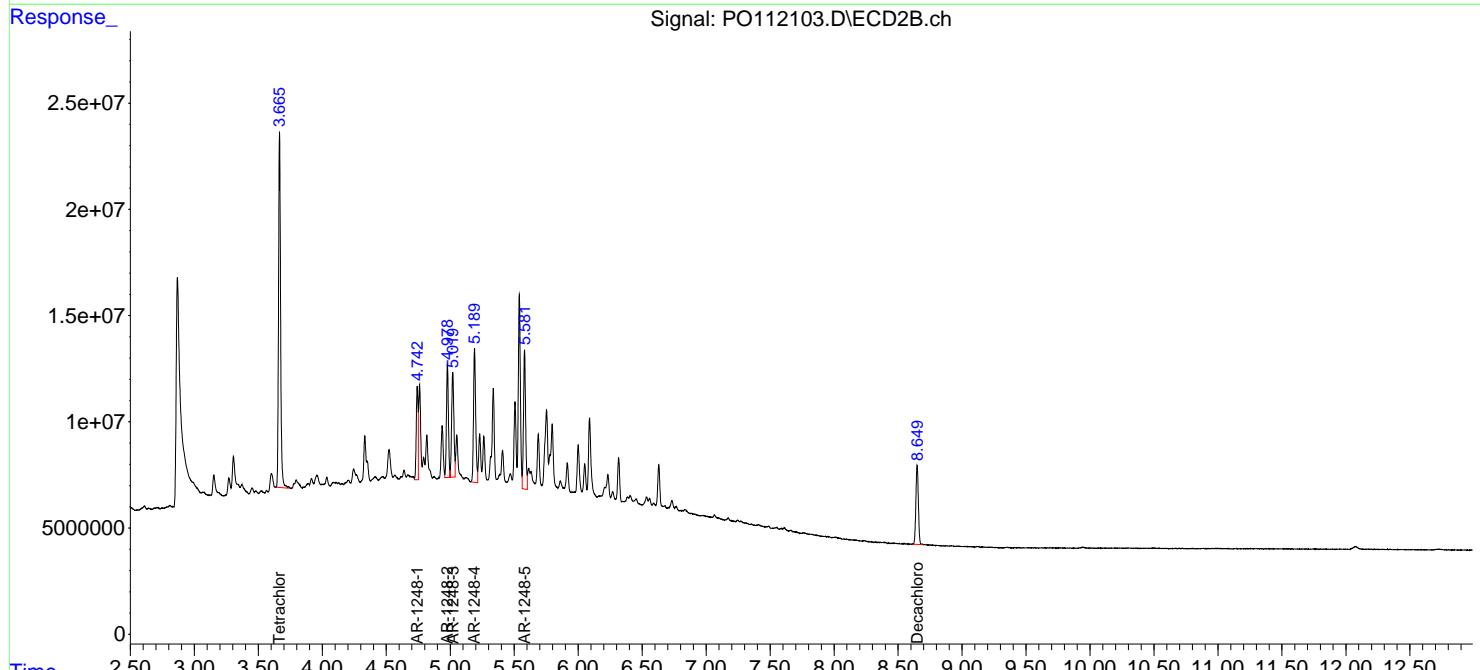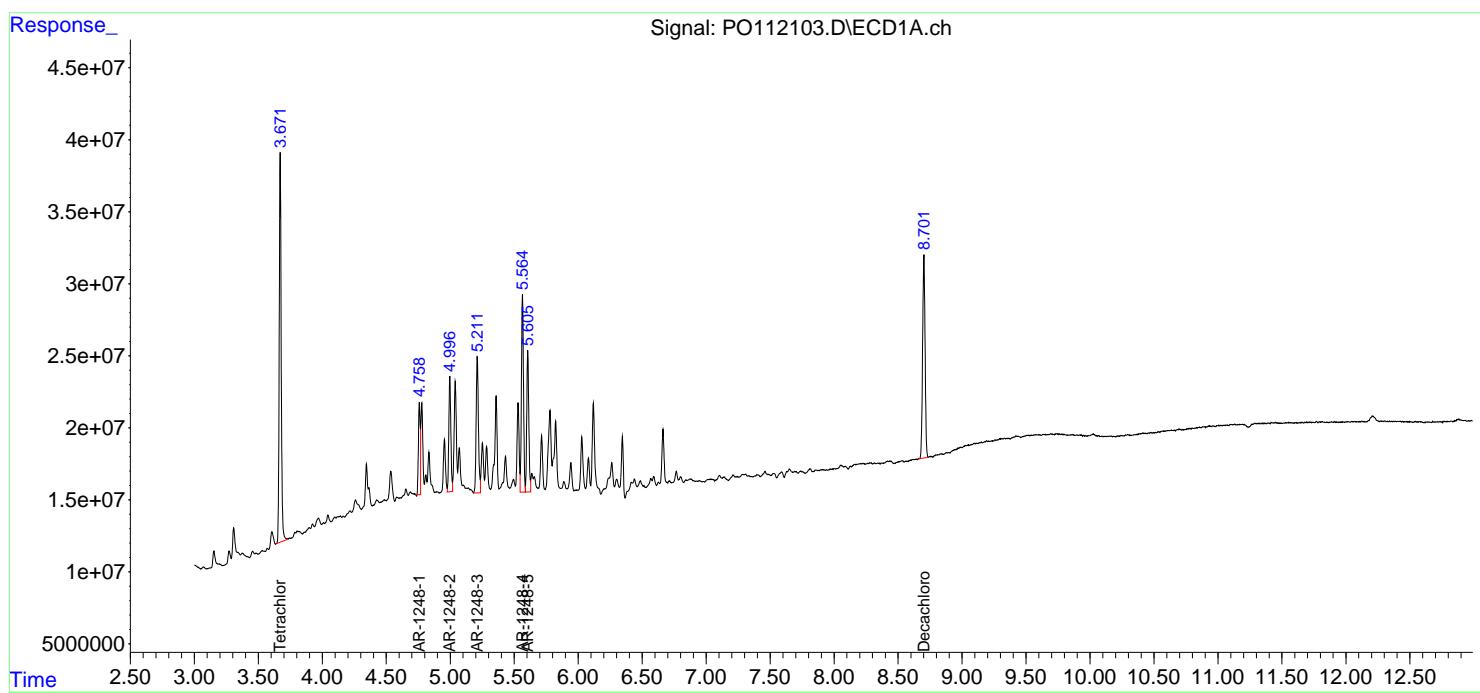

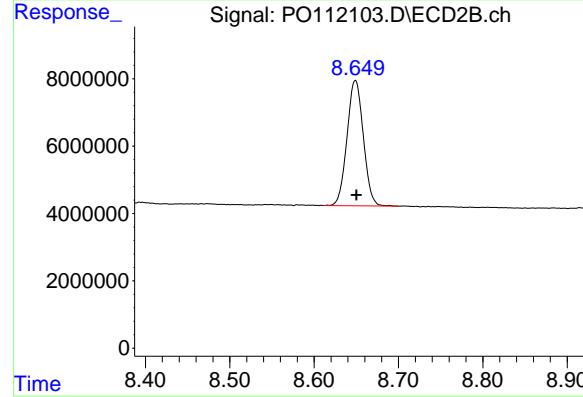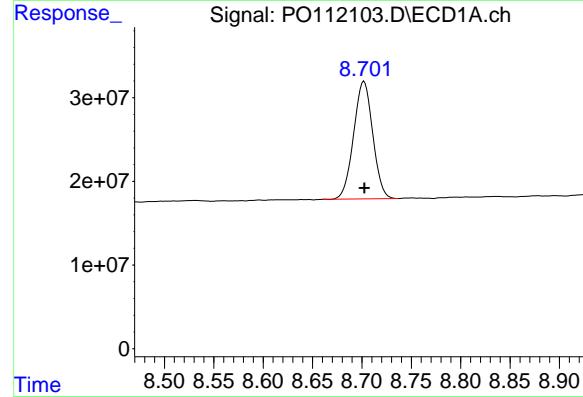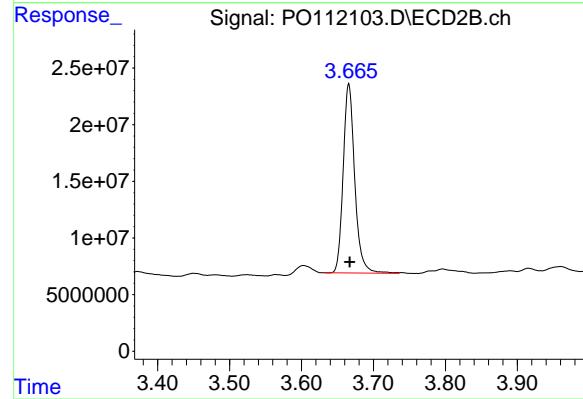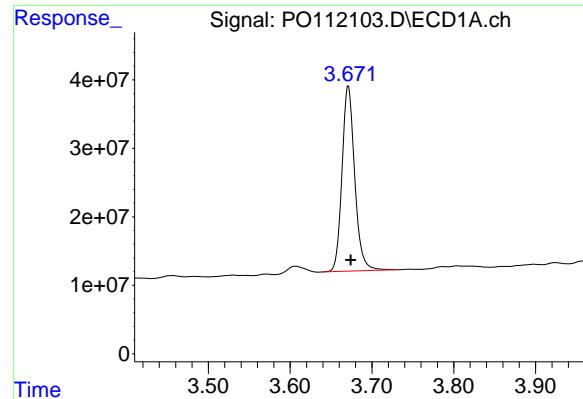

#1 Tetrachloro-m-xylene

R.T.: 3.671 min
 Delta R.T.: -0.003 min
 Response: 291855307
 Conc: 27.71 ng/ml

Instrument:
 ECD_O
 ClientSampleId :
 AR1248ICC250

#1 Tetrachloro-m-xylene

R.T.: 3.666 min
 Delta R.T.: -0.001 min
 Response: 186430413
 Conc: 28.02 ng/ml

#2 Decachlorobiphenyl

R.T.: 8.702 min
 Delta R.T.: 0.000 min
 Response: 189212036
 Conc: 26.07 ng/ml


#2 Decachlorobiphenyl

R.T.: 8.649 min
 Delta R.T.: -0.001 min
 Response: 49988120
 Conc: 27.24 ng/ml

#21 AR-1248-1


R.T.: 4.759 min
 Delta R.T.: -0.002 min
 Response: 62843351
 Conc: 276.08 ng/ml

Instrument: ECD_O
 ClientSampleId: AR1248ICC250

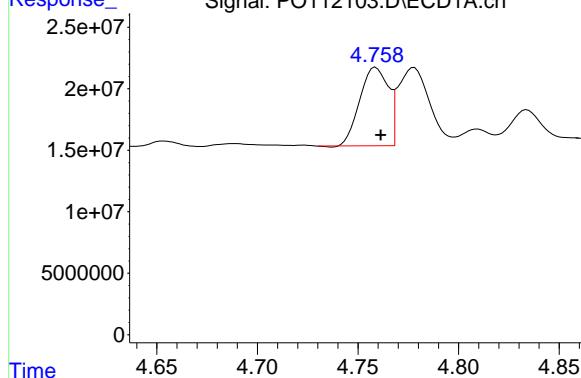


#21 AR-1248-1

R.T.: 4.742 min
 Delta R.T.: -0.001 min
 Response: 43399528
 Conc: 290.03 ng/ml

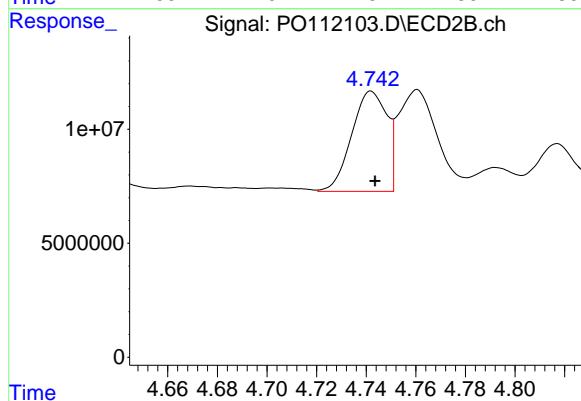


#22 AR-1248-2


R.T.: 4.997 min
 Delta R.T.: -0.003 min
 Response: 87401333
 Conc: 284.46 ng/ml

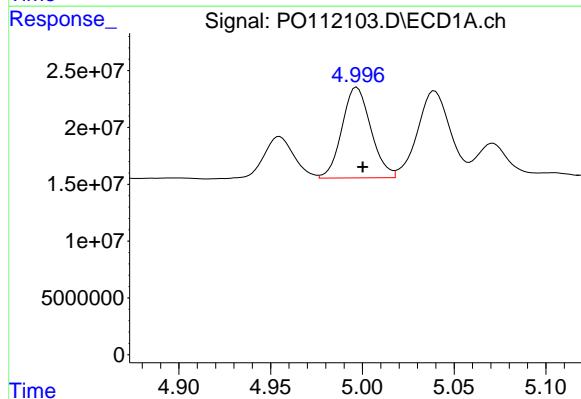

#22 AR-1248-2

R.T.: 4.978 min
 Delta R.T.: -0.002 min
 Response: 57560333
 Conc: 283.38 ng/ml

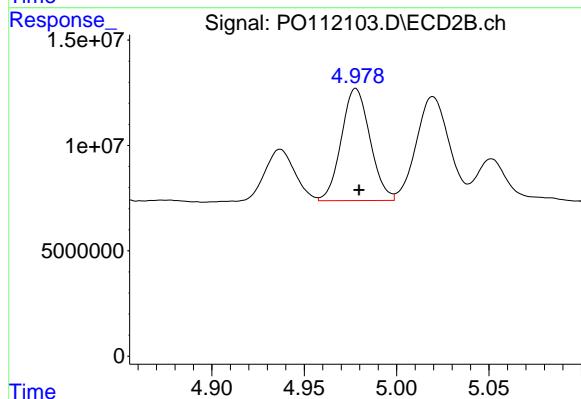

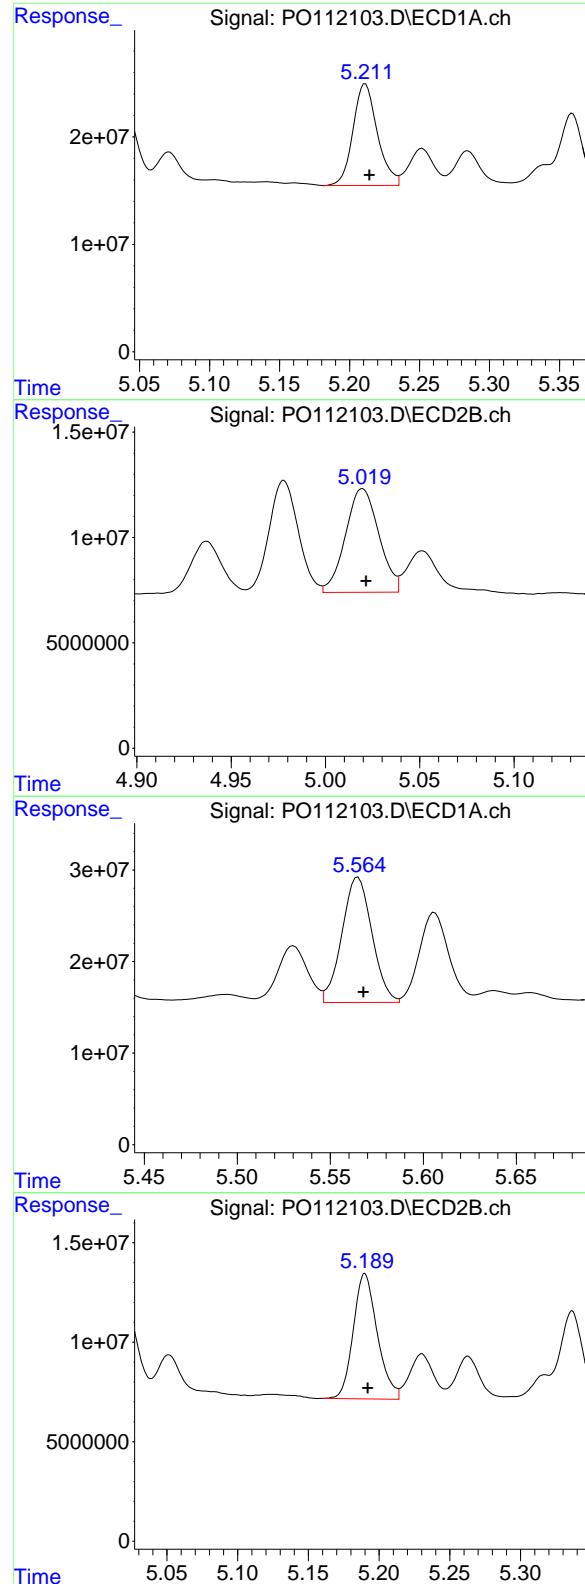

#23 AR-1248-3

R.T.: 5.211 min
 Delta R.T.: -0.003 min
 Response: 114900435
 Conc: 292.43 ng/ml

Instrument: ECD_O
 ClientSampleId: AR1248ICC250

#23 AR-1248-3

R.T.: 5.020 min
 Delta R.T.: -0.002 min
 Response: 60695146
 Conc: 285.24 ng/ml

#24 AR-1248-4

R.T.: 5.565 min
 Delta R.T.: -0.003 min
 Response: 153802772
 Conc: 267.22 ng/ml



#24 AR-1248-4

R.T.: 5.190 min
 Delta R.T.: -0.002 min
 Response: 74439996
 Conc: 293.63 ng/ml

#25 AR-1248-5

R.T.: 5.606 min
Delta R.T.: -0.003 min
Response: 108920138
Conc: 278.78 ng/ml

Instrument: ECD_O
ClientSampleId: AR1248ICC250

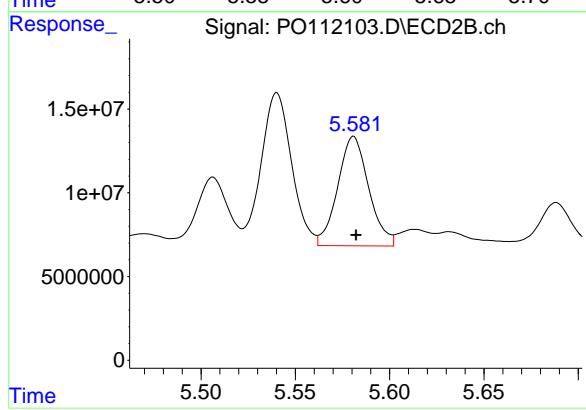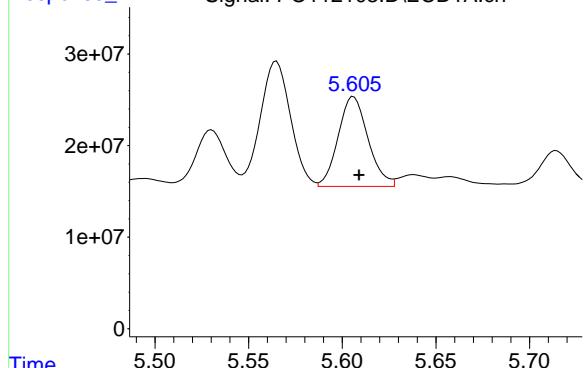

#25 AR-1248-5

R.T.: 5.581 min
Delta R.T.: -0.001 min
Response: 74875919
Conc: 298.33 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0070825\
 Data File : P0112104.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jul 2025 18:59
 Operator : YP/AJ
 Sample : AR1248ICC050
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1248ICC050

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/09/2025
 Supervised By :mohammad ahmed 07/10/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 09 02:45:42 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 09 02:41:59 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	3.673	3.666	43320523	27979420	4.113	4.205
2) SA Decachlor...	8.703	8.650	29248819	7966074	4.030	4.341

Target Compounds

21) L5 AR-1248-1	4.761	4.742	9816500	7672405	43.126	51.273
22) L5 AR-1248-2	4.999	4.979	13335961	9853335	43.403	48.509
23) L5 AR-1248-3	5.213	5.020	19880304	9961976	50.597	46.817
24) L5 AR-1248-4	5.567	5.191	27262638	12330568	47.367	48.638m
25) L5 AR-1248-5	5.608	5.581	17126268	10723520	43.835	42.725m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0070825\
 Data File : P0112104.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jul 2025 18:59
 Operator : YP/AJ
 Sample : AR1248ICC050
 Misc :
 ALS Vial : 19 Sample Multiplier: 1


Instrument :
ECD_O
ClientSampleId :
AR1248ICC050


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/09/2025
 Supervised By :mohammad ahmed 07/10/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 09 02:45:42 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 09 02:41:59 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

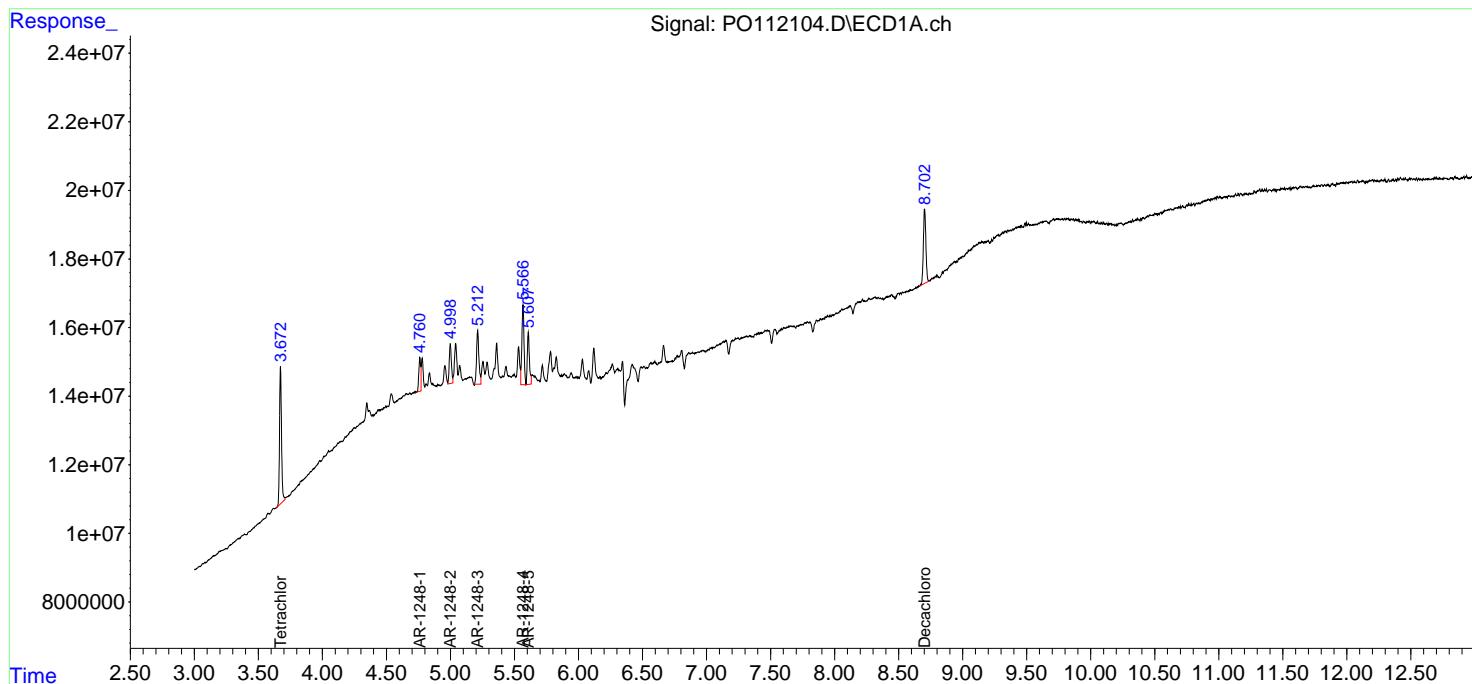

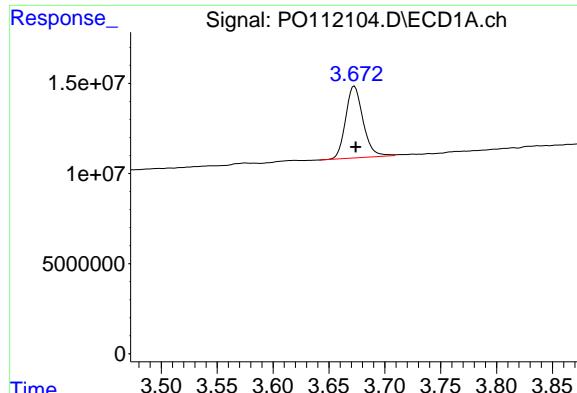


#1 Tetrachloro-m-xylene

R.T.: 3.673 min
Delta R.T.: -0.001 min
Response: 43320523
Conc: 4.11 ng/ml

Instrument: ECD_O
ClientSampleId: AR1248ICC050


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/09/2025
Supervised By :mohammad ahmed 07/10/2025

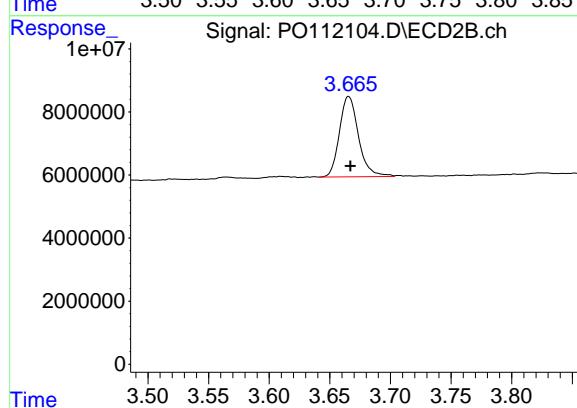


#1 Tetrachloro-m-xylene

R.T.: 3.666 min
Delta R.T.: -0.001 min
Response: 27979420
Conc: 4.21 ng/ml







#2 Decachlorobiphenyl

R.T.: 8.703 min
Delta R.T.: 0.000 min
Response: 29248819
Conc: 4.03 ng/ml

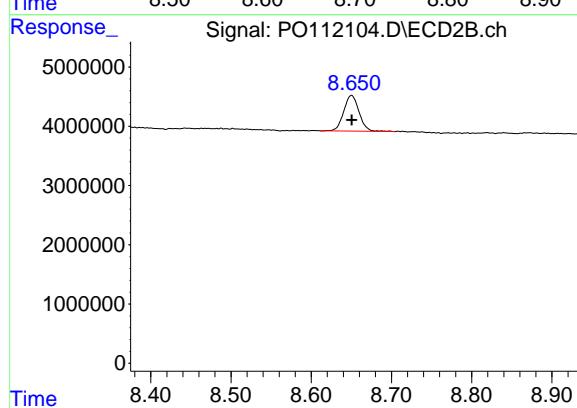

#2 Decachlorobiphenyl

R.T.: 8.650 min
Delta R.T.: 0.000 min
Response: 7966074
Conc: 4.34 ng/ml

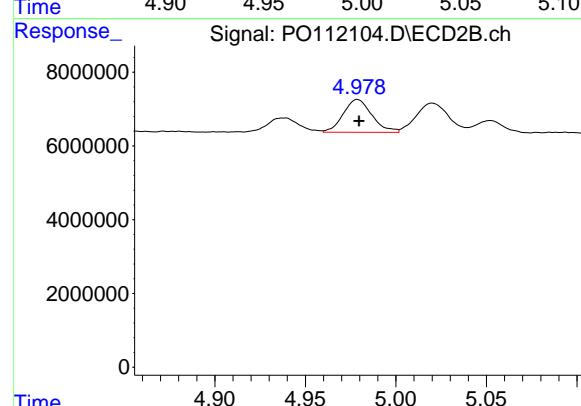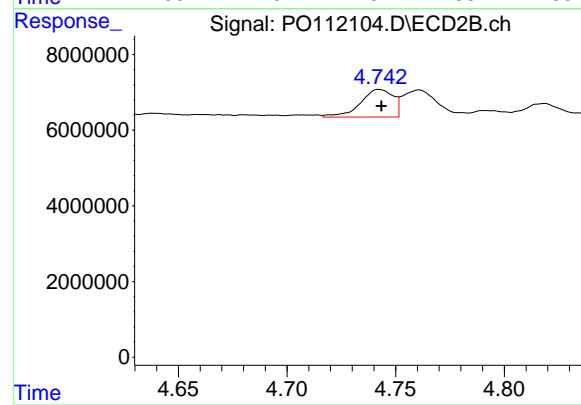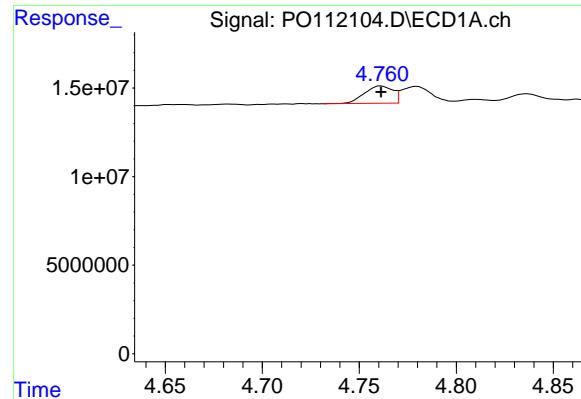




#21 AR-1248-1

R.T.: 4.761 min
Delta R.T.: 0.000 min
Response: 9816500
Conc: 43.13 ng/ml

Instrument: ECD_O
ClientSampleId: AR1248ICC050

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/09/2025
Supervised By :mohammad ahmed 07/10/2025

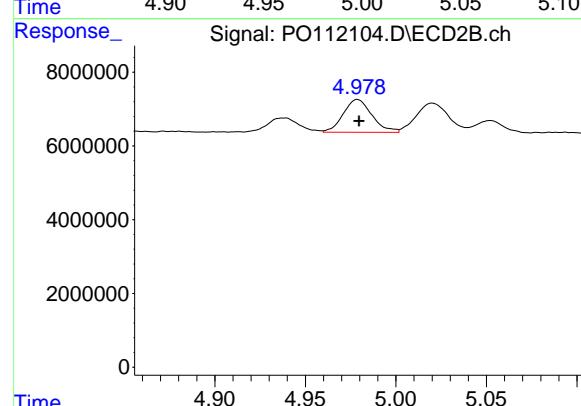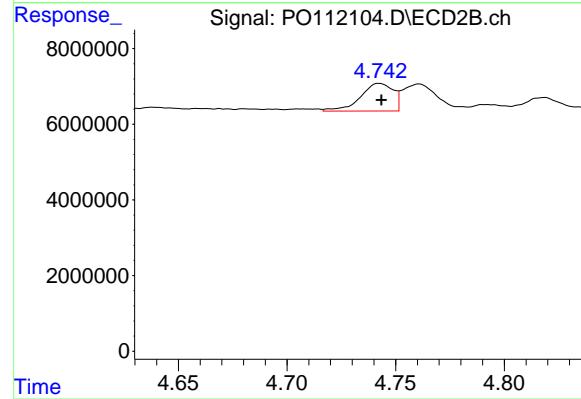

#21 AR-1248-1





R.T.: 4.742 min
Delta R.T.: -0.001 min
Response: 7672405
Conc: 51.27 ng/ml

#22 AR-1248-2

R.T.: 4.999 min
Delta R.T.: -0.001 min
Response: 13335961
Conc: 43.40 ng/ml

#22 AR-1248-2

R.T.: 4.979 min
Delta R.T.: 0.000 min
Response: 9853335
Conc: 48.51 ng/ml

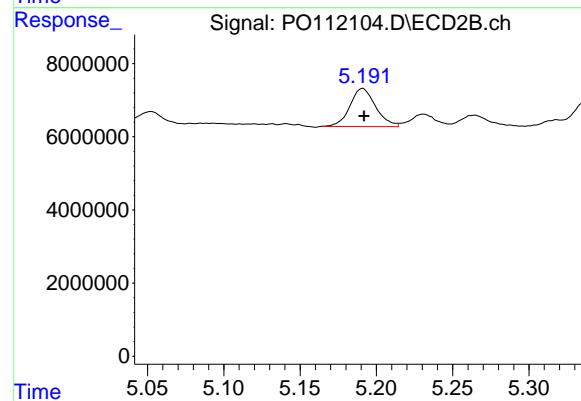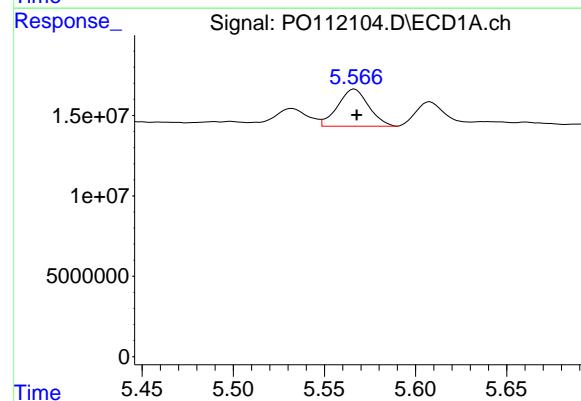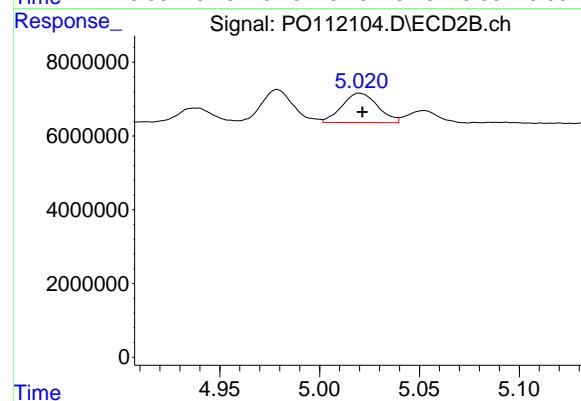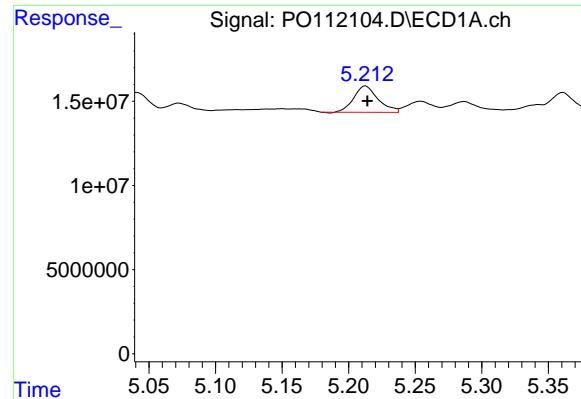




#23 AR-1248-3

R.T.: 5.213 min
Delta R.T.: -0.001 min
Response: 19880304
Conc: 50.60 ng/ml

Instrument: ECD_O
ClientSampleId: AR1248ICC050

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/09/2025
Supervised By :mohammad ahmed 07/10/2025

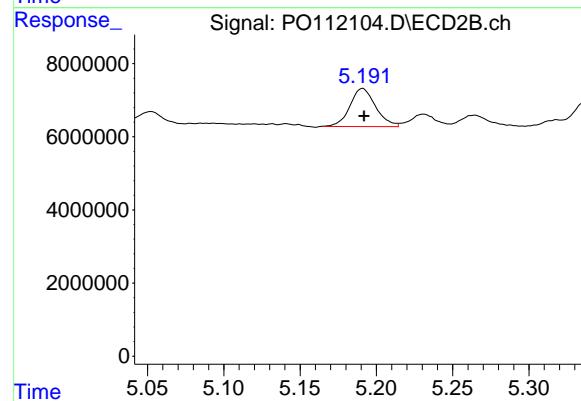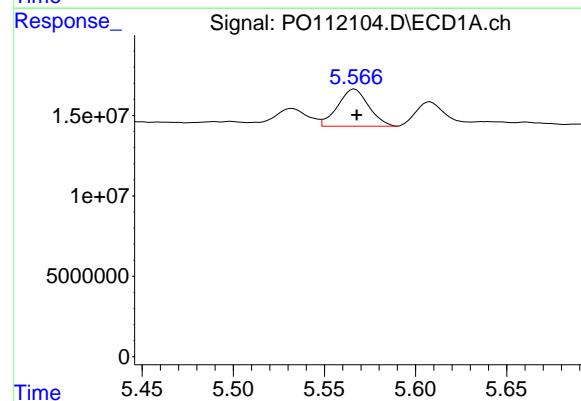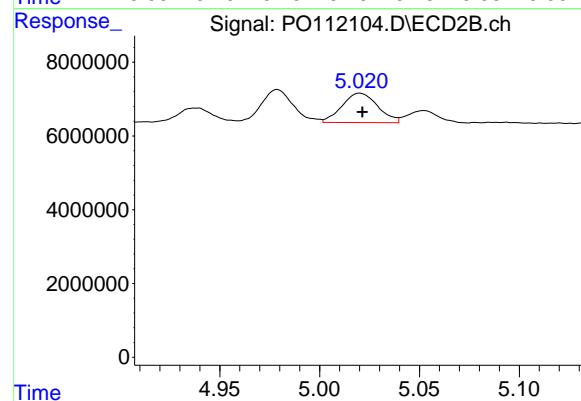

#23 AR-1248-3

R.T.: 5.020 min
Delta R.T.: -0.001 min
Response: 9961976
Conc: 46.82 ng/ml

#24 AR-1248-4

R.T.: 5.567 min
Delta R.T.: -0.001 min
Response: 27262638
Conc: 47.37 ng/ml

#24 AR-1248-4

R.T.: 5.191 min
Delta R.T.: -0.001 min
Response: 12330568
Conc: 48.64 ng/ml



#25 AR-1248-5

R.T.: 5.608 min
 Delta R.T.: -0.001 min
 Response: 17126268
 Conc: 43.84 ng/ml

Instrument: ECD_O
ClientSampleId: AR1248ICC050

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/09/2025
 Supervised By :mohammad ahmed 07/10/2025

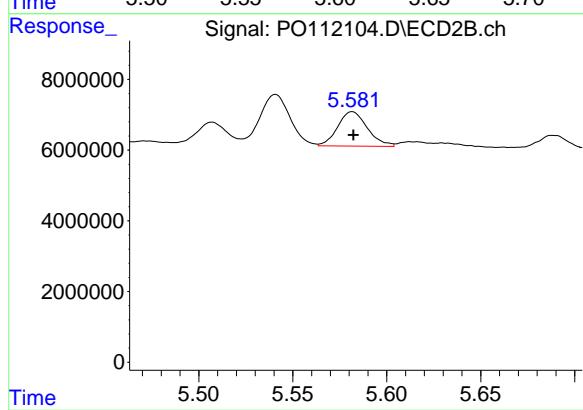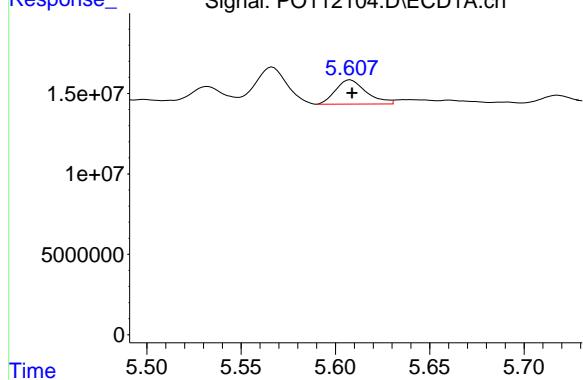

#25 AR-1248-5

R.T.: 5.581 min
 Delta R.T.: -0.001 min
 Response: 10723520
 Conc: 42.73 ng/ml

1
2
3
4
5
6
7
8
9
10
11
12
13
14
15
16
17
18
19
20

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0070825\
 Data File : P0112105.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jul 2025 19:18
 Operator : YP/AJ
 Sample : AR1254ICC1000
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1254ICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 09 03:13:13 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 09 03:10:24 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	3.674	3.666	1081.7E6	681.3E6	100.629	100.324
2) SA Decachlor...	8.704	8.651	731.3E6	176.2E6	97.187	95.129

Target Compounds

26) L6 AR-1254-1	5.567	5.542	596.4E6	358.7E6	968.859	952.427
27) L6 AR-1254-2	5.716	5.689	526.6E6	309.3E6	978.251	948.939
28) L6 AR-1254-3	6.120	6.090	832.4E6	457.0E6	985.524	970.955
29) L6 AR-1254-4	6.349	6.317	488.3E6	242.7E6	924.821	917.706
30) L6 AR-1254-5	6.769	6.735	772.8E6	340.9E6	976.309	957.333



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0070825\
 Data File : P0112105.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jul 2025 19:18
 Operator : YP/AJ
 Sample : AR1254ICC1000
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1254ICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 09 03:13:13 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 09 03:10:24 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

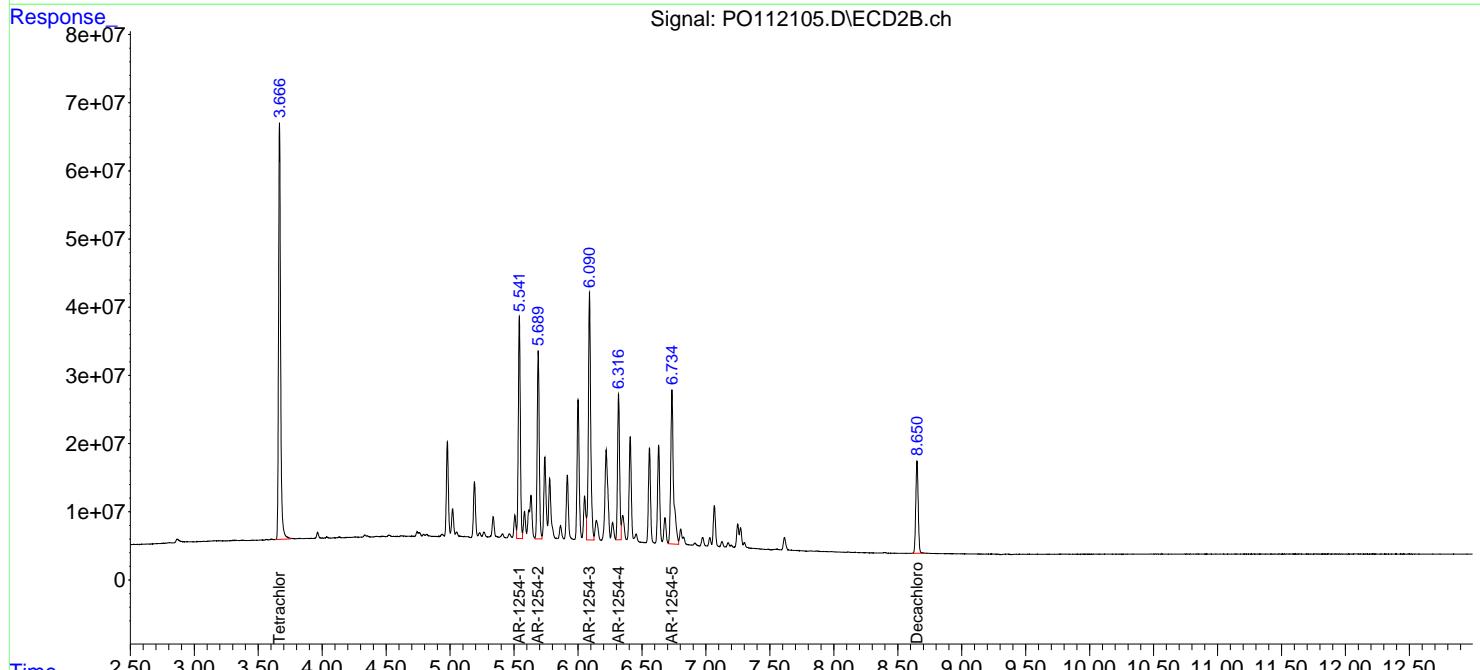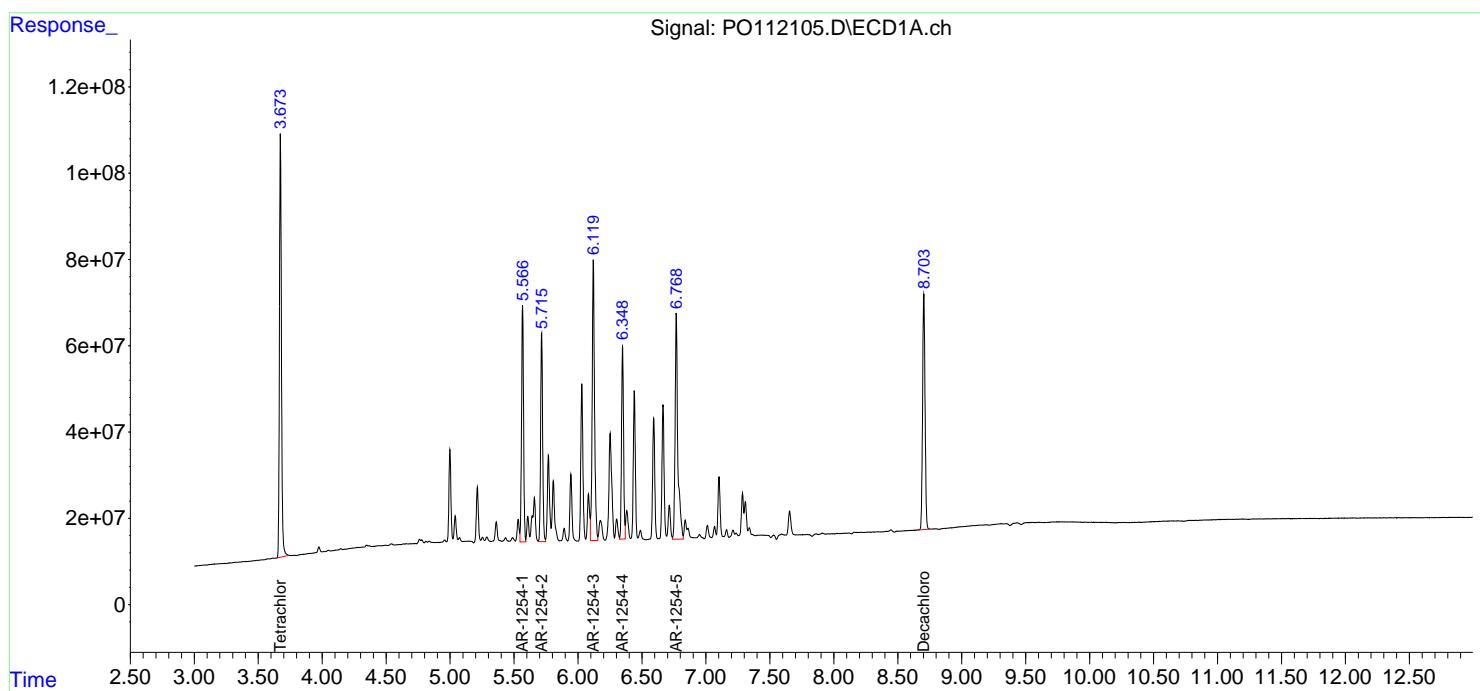

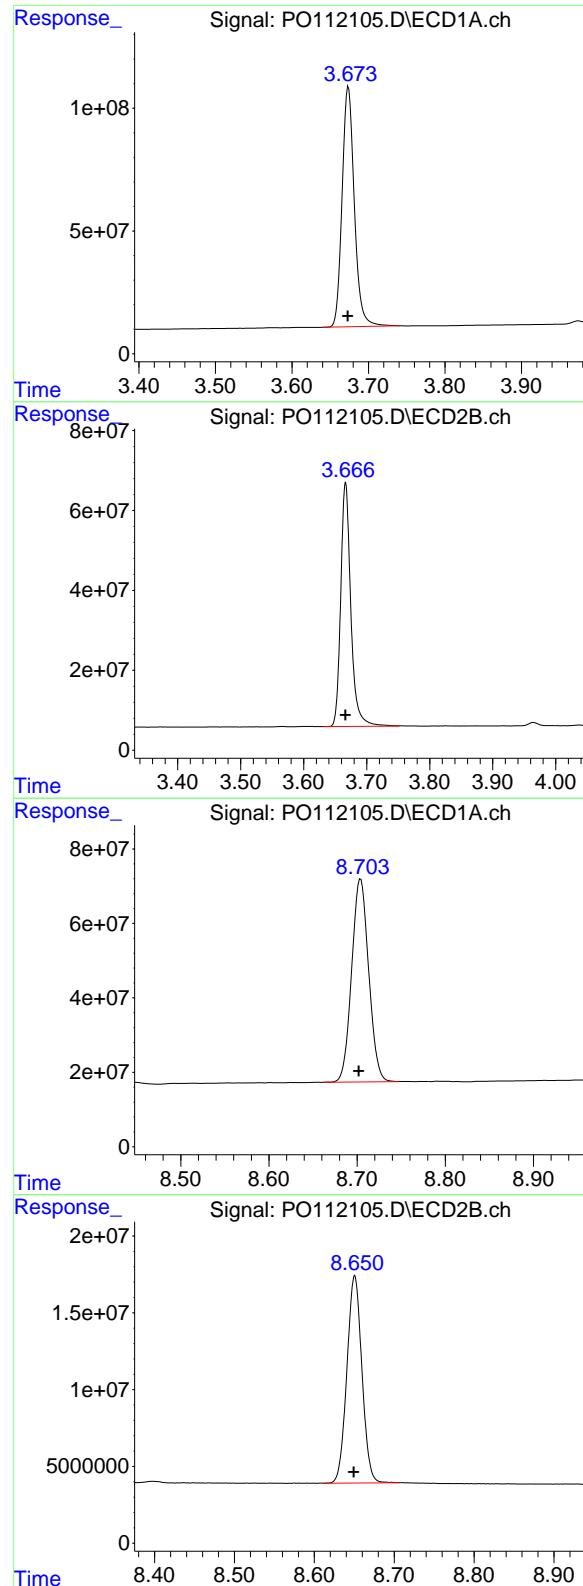

#1 Tetrachloro-m-xylene

R.T.: 3.674 min
 Delta R.T.: 0.000 min
 Response: 1081749553
 Conc: 100.63 ng/ml

Instrument: ECD_O
ClientSampleId: AR1254ICC1000

#1 Tetrachloro-m-xylene

R.T.: 3.666 min
 Delta R.T.: 0.000 min
 Response: 681267764
 Conc: 100.32 ng/ml

#2 Decachlorobiphenyl

R.T.: 8.704 min
 Delta R.T.: 0.002 min
 Response: 731321852
 Conc: 97.19 ng/ml


#2 Decachlorobiphenyl

R.T.: 8.651 min
 Delta R.T.: 0.001 min
 Response: 176203798
 Conc: 95.13 ng/ml

#26 AR-1254-1


R.T.: 5.567 min
 Delta R.T.: 0.001 min
 Response: 596387386
 Conc: 968.86 ng/ml

Instrument: ECD_O
ClientSampleId: AR1254ICC1000

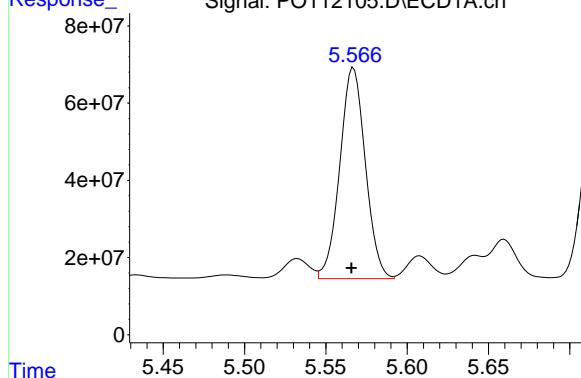


#26 AR-1254-1

R.T.: 5.542 min
 Delta R.T.: 0.000 min
 Response: 358701312
 Conc: 952.43 ng/ml

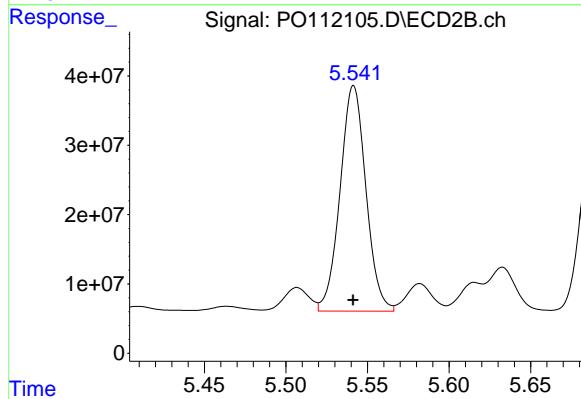


#27 AR-1254-2

R.T.: 5.716 min
 Delta R.T.: 0.001 min
 Response: 526620849
 Conc: 978.25 ng/ml

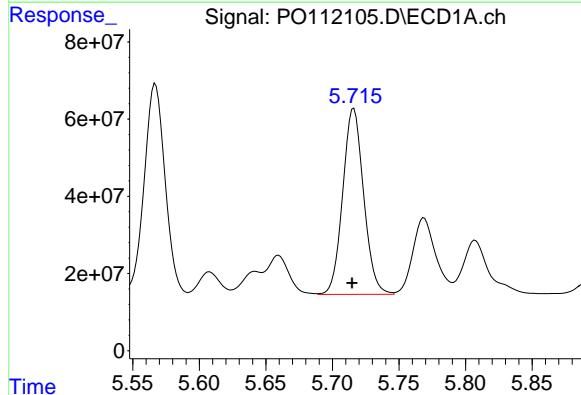

#27 AR-1254-2


R.T.: 5.689 min
 Delta R.T.: 0.000 min
 Response: 309319461
 Conc: 948.94 ng/ml

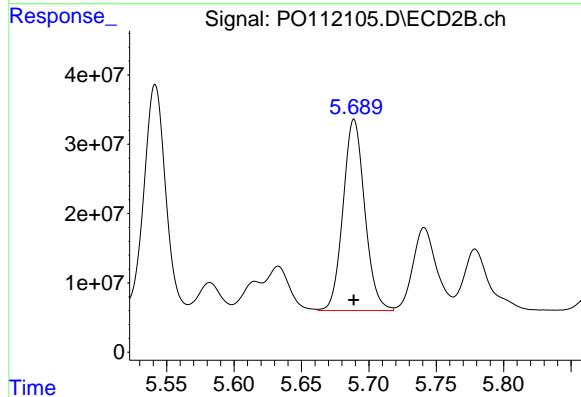

#28 AR-1254-3


R.T.: 6.120 min
 Delta R.T.: 0.000 min
 Response: 832372124
 Conc: 985.52 ng/ml

Instrument: ECD_O
ClientSampleId: AR1254ICC1000

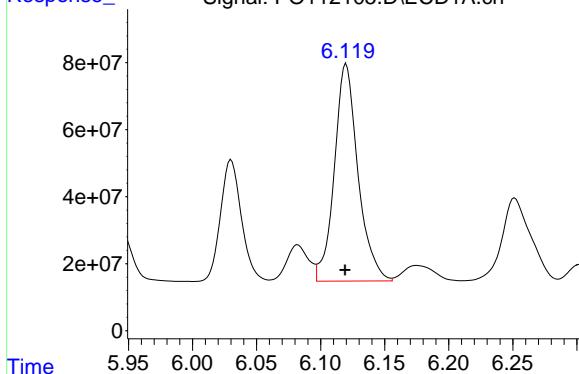


#28 AR-1254-3

R.T.: 6.090 min
 Delta R.T.: 0.000 min
 Response: 457035033
 Conc: 970.96 ng/ml

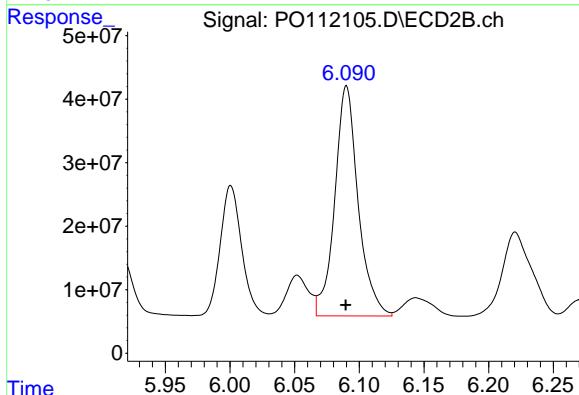


#29 AR-1254-4

R.T.: 6.349 min
 Delta R.T.: 0.000 min
 Response: 488348458
 Conc: 924.82 ng/ml

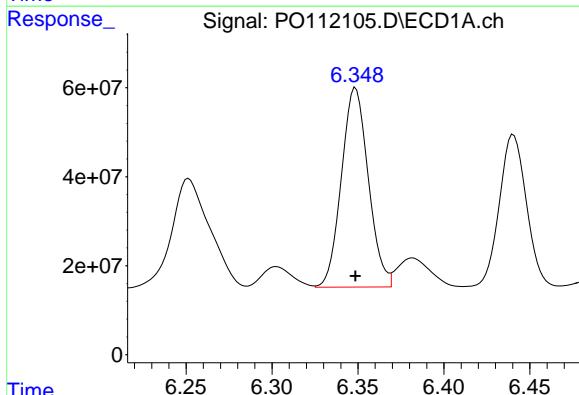

#29 AR-1254-4


R.T.: 6.317 min
 Delta R.T.: 0.000 min
 Response: 242702235
 Conc: 917.71 ng/ml

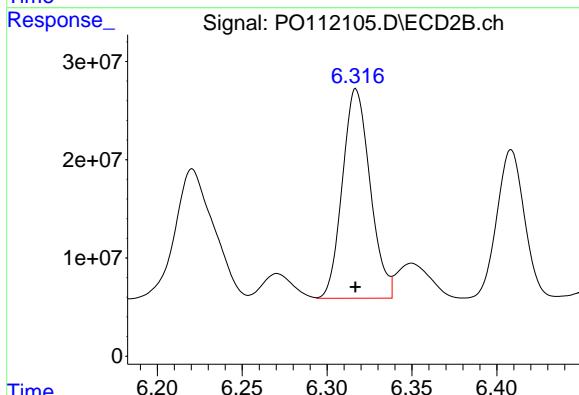

#30 AR-1254-5

R.T.: 6.769 min
Delta R.T.: 0.001 min
Response: 772769124
Conc: 976.31 ng/ml

Instrument: ECD_O
ClientSampleId: AR1254ICC1000

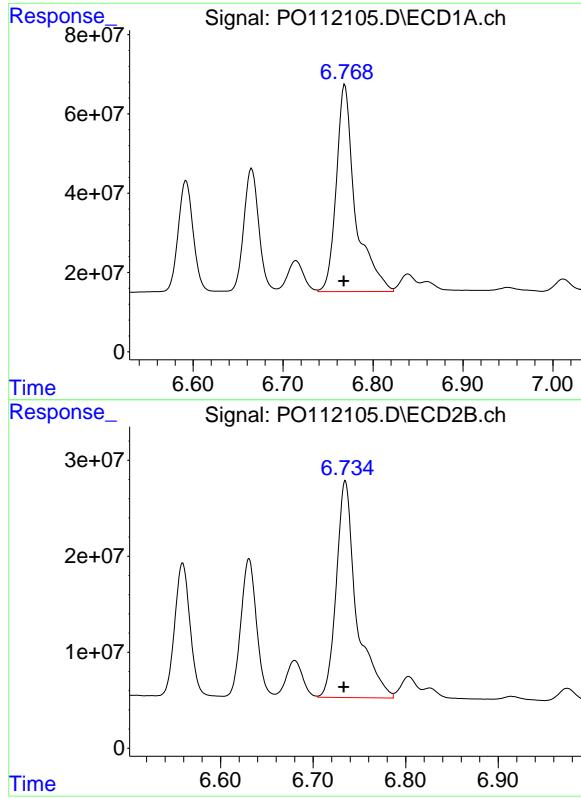

#30 AR-1254-5

R.T.: 6.735 min
Delta R.T.: 0.002 min
Response: 340856875
Conc: 957.33 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0070825\
 Data File : P0112106.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jul 2025 19:35
 Operator : YP/AJ
 Sample : AR1254ICC750
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1254ICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 09 03:13:24 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 09 03:10:24 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	3.671	3.666	822.8E6	521.0E6	76.536	76.717
2) SA Decachlor...	8.701	8.649	552.3E6	135.1E6	73.395	72.926

Target Compounds

26) L6 AR-1254-1	5.564	5.541	461.5E6	279.3E6	749.690	741.534
27) L6 AR-1254-2	5.714	5.689	406.1E6	238.9E6	754.357	732.842
28) L6 AR-1254-3	6.118	6.090	636.3E6	355.1E6	753.353	754.409
29) L6 AR-1254-4	6.347	6.317	412.9E6	198.3E6	782.017	749.977
30) L6 AR-1254-5	6.767	6.733	589.5E6	261.7E6	744.724	734.939



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0070825\
 Data File : P0112106.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jul 2025 19:35
 Operator : YP/AJ
 Sample : AR1254ICC750
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1254ICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 09 03:13:24 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 09 03:10:24 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ m Signal #2 Info : 30M x 0.32mm x 0.25 μ m

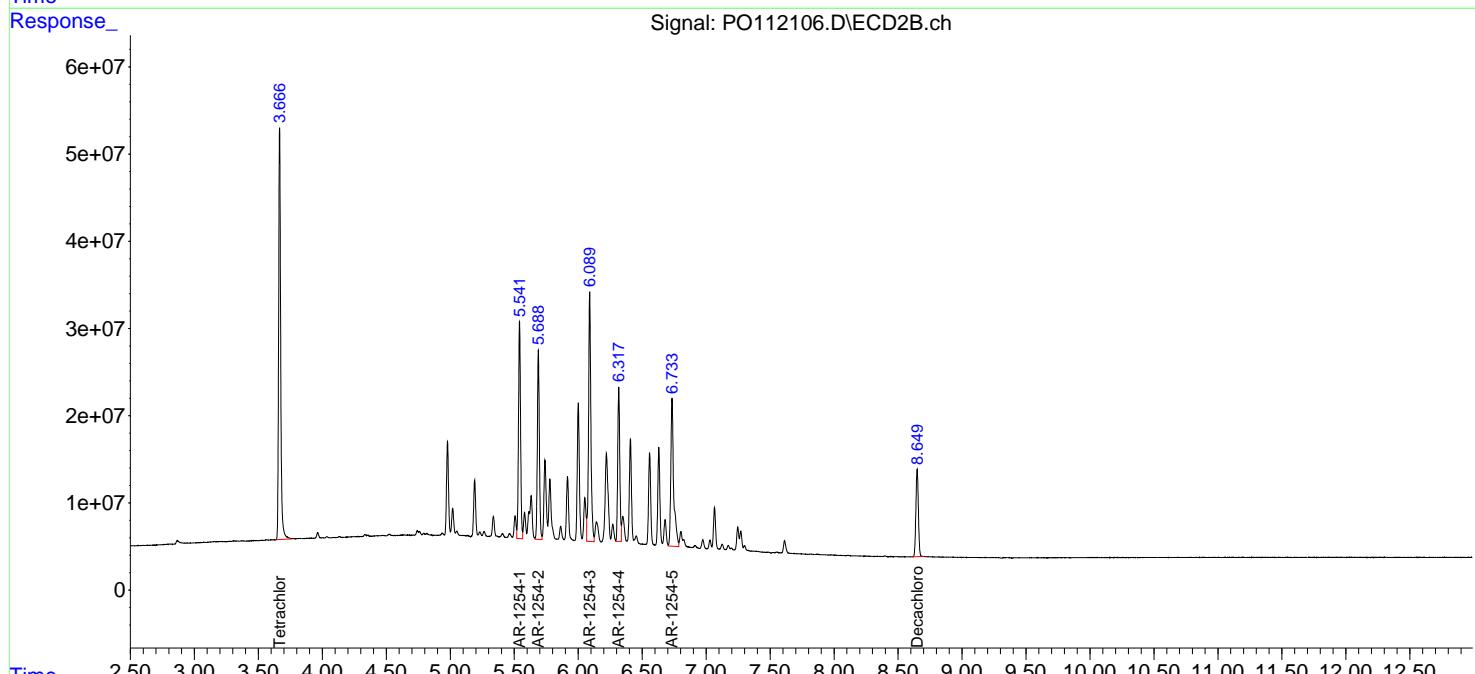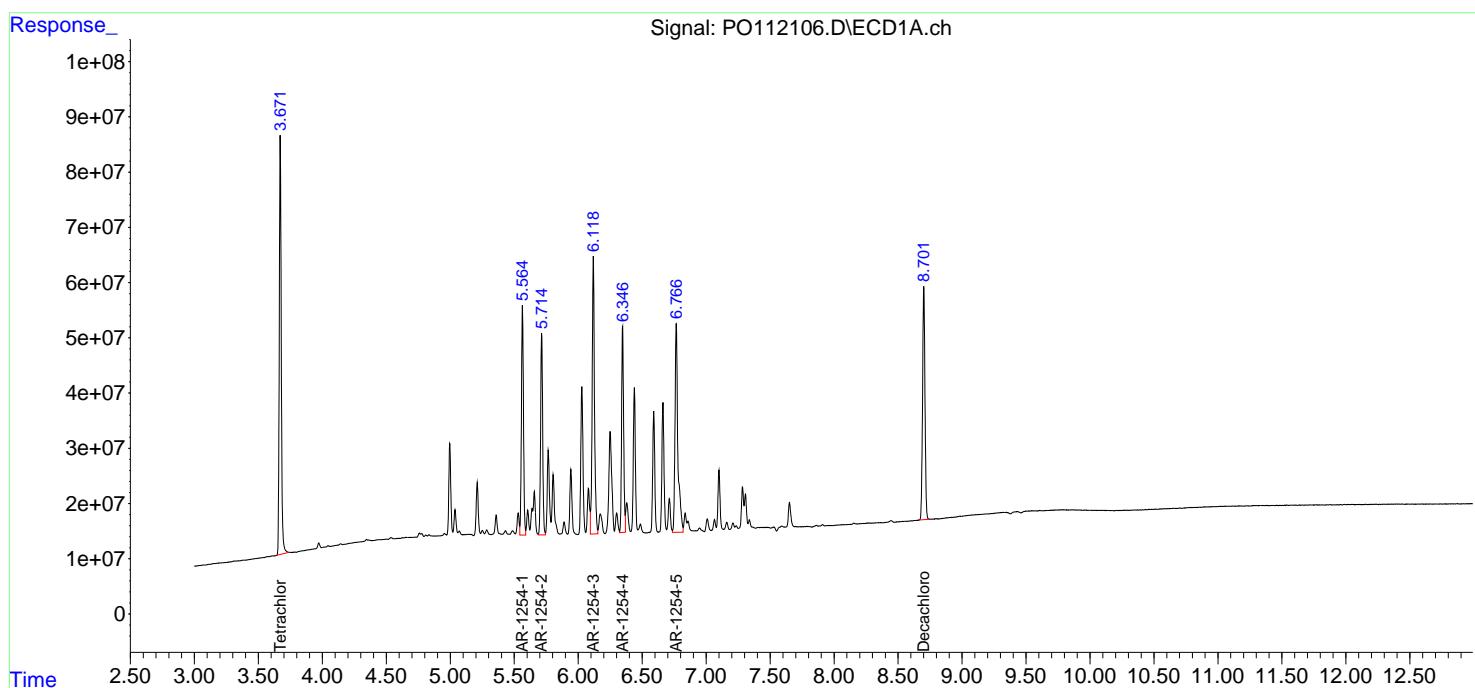

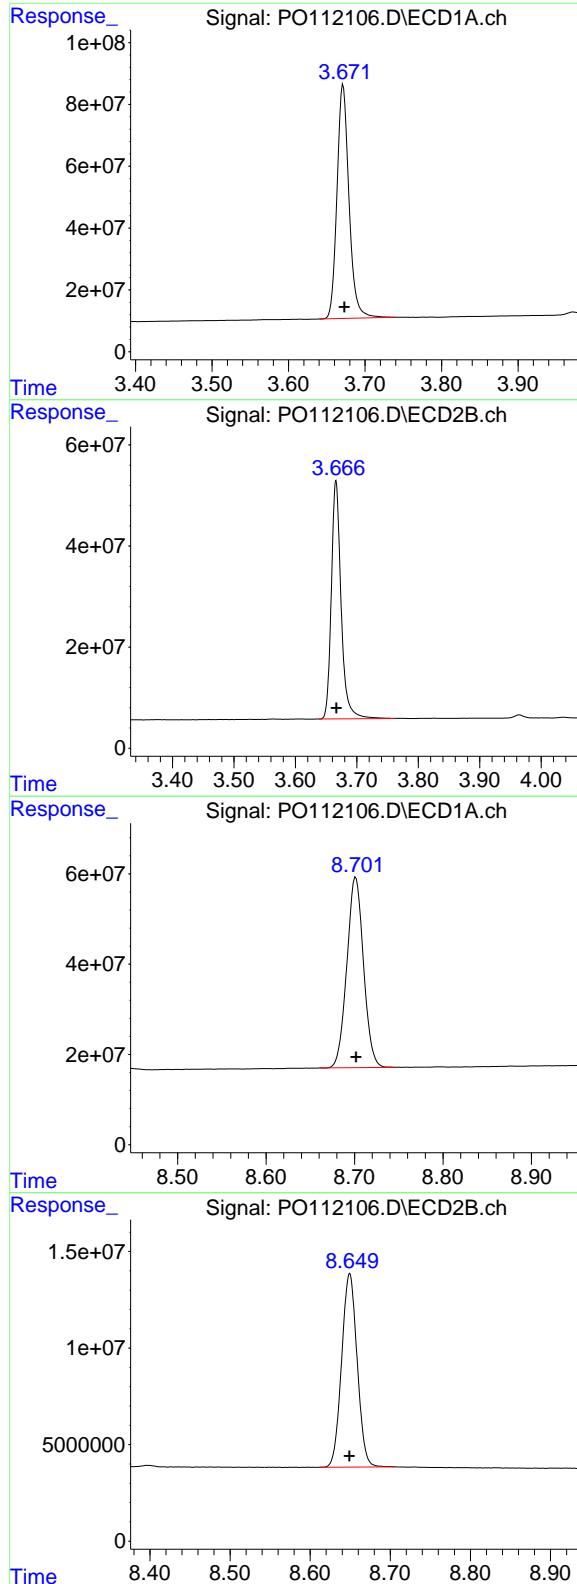

#1 Tetrachloro-m-xylene

R.T.: 3.671 min
 Delta R.T.: -0.002 min
 Response: 822751477
 Conc: 76.54 ng/ml

Instrument:
 ECD_O
 ClientSampleId :
 AR1254ICC750

#1 Tetrachloro-m-xylene





R.T.: 3.666 min
 Delta R.T.: 0.000 min
 Response: 520964027
 Conc: 76.72 ng/ml

#2 Decachlorobiphenyl

R.T.: 8.701 min
 Delta R.T.: 0.000 min
 Response: 552292278
 Conc: 73.40 ng/ml

#2 Decachlorobiphenyl

R.T.: 8.649 min
 Delta R.T.: 0.000 min
 Response: 135078575
 Conc: 72.93 ng/ml

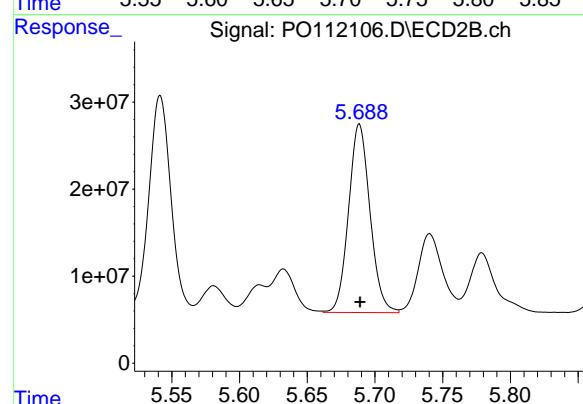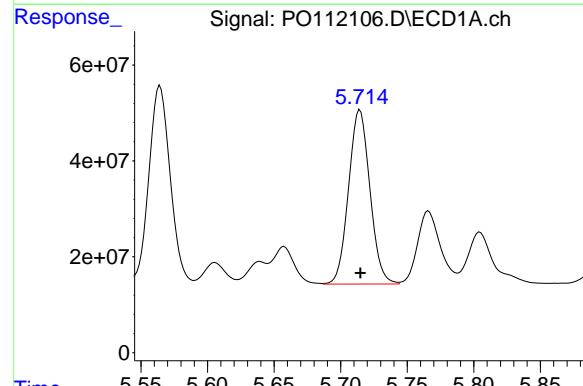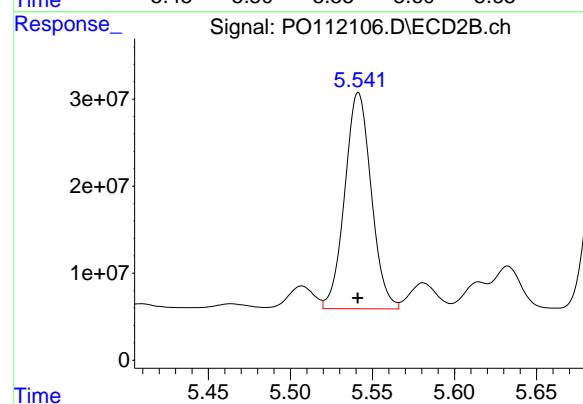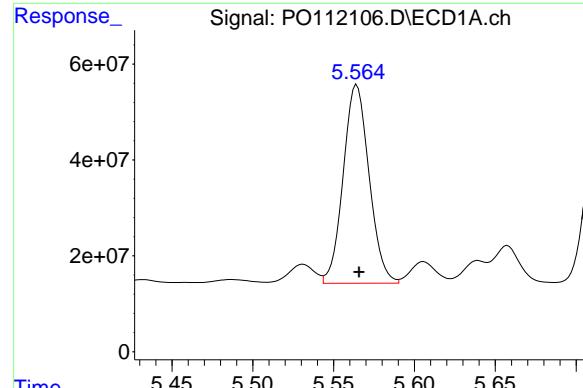

#26 AR-1254-1

R.T.: 5.564 min
 Delta R.T.: -0.001 min
 Response: 461476391
 Conc: 749.69 ng/ml

Instrument: ECD_O
ClientSampleId: AR1254ICC750

#26 AR-1254-1

R.T.: 5.541 min
 Delta R.T.: 0.000 min
 Response: 279275100
 Conc: 741.53 ng/ml

#27 AR-1254-2

R.T.: 5.714 min
 Delta R.T.: 0.000 min
 Response: 406092372
 Conc: 754.36 ng/ml


#27 AR-1254-2

R.T.: 5.689 min
 Delta R.T.: 0.000 min
 Response: 238879675
 Conc: 732.84 ng/ml

#28 AR-1254-3


R.T.: 6.118 min
 Delta R.T.: 0.000 min
 Response: 636281329
 Conc: 753.35 ng/ml

Instrument: ECD_O
ClientSampleId: AR1254ICC750




#28 AR-1254-3

R.T.: 6.090 min
 Delta R.T.: 0.000 min
 Response: 355105051
 Conc: 754.41 ng/ml

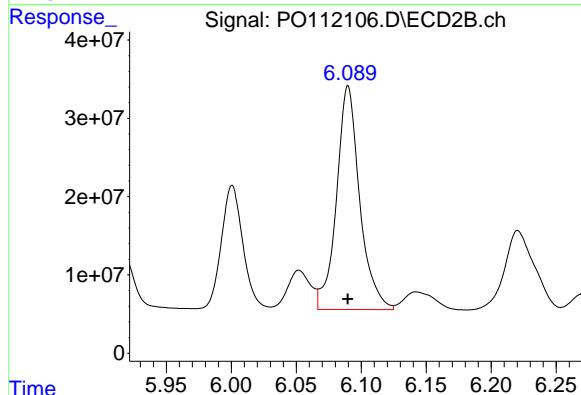


#29 AR-1254-4

R.T.: 6.347 min
 Delta R.T.: -0.001 min
 Response: 412941412
 Conc: 782.02 ng/ml

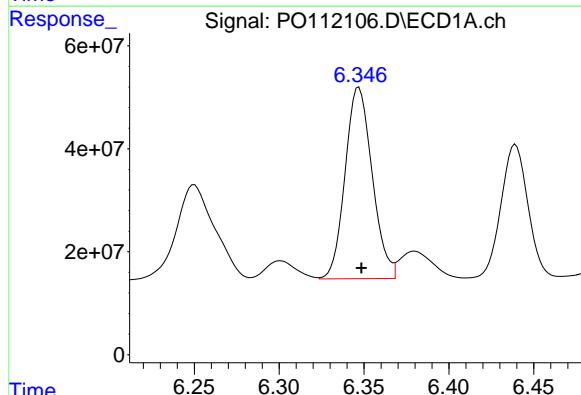

#29 AR-1254-4



R.T.: 6.317 min
 Delta R.T.: 0.000 min
 Response: 198343540
 Conc: 749.98 ng/ml

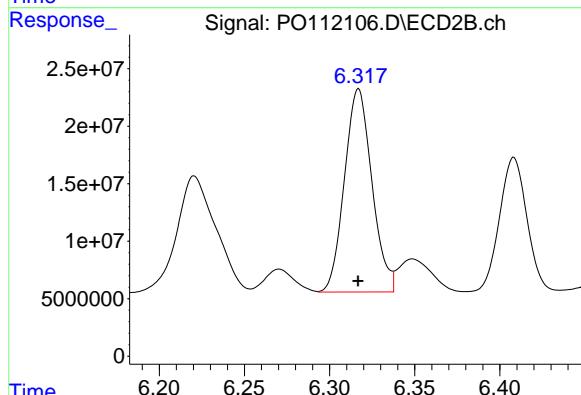

#30 AR-1254-5

R.T.: 6.767 min
Delta R.T.: 0.000 min
Response: 589465205
Conc: 744.72 ng/ml

Instrument: ECD_O
ClientSampleId: AR1254ICC750

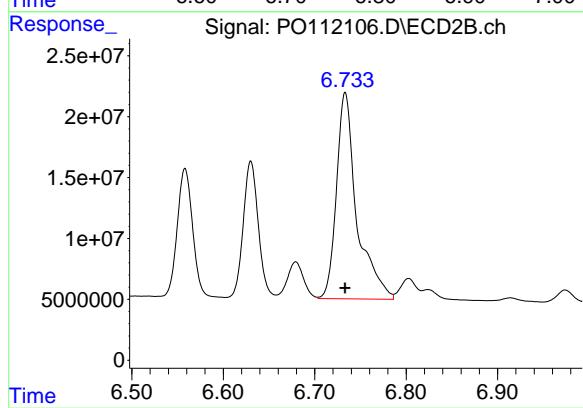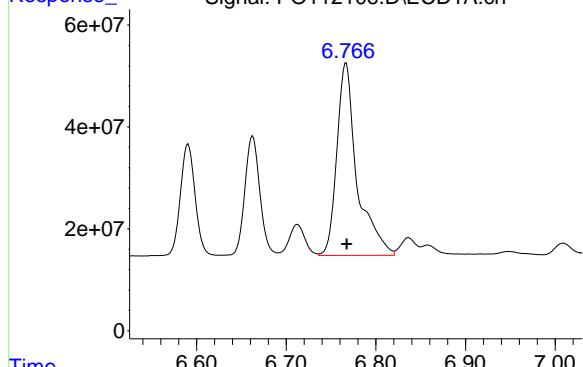

#30 AR-1254-5

R.T.: 6.733 min
Delta R.T.: 0.000 min
Response: 261674065
Conc: 734.94 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0070825\
 Data File : P0112107.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jul 2025 19:54
 Operator : YP/AJ
 Sample : AR1254ICC500
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1254ICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 09 03:13:37 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 09 03:10:24 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	3.673	3.666	537.5E6	339.5E6	50.000	50.000
2) SA Decachlor...	8.702	8.649	376.2E6	92613439	50.000	50.000

Target Compounds

26) L6 AR-1254-1	5.566	5.541	307.8E6	188.3E6	500.000	500.000
27) L6 AR-1254-2	5.715	5.689	269.2E6	163.0E6	500.000	500.000
28) L6 AR-1254-3	6.119	6.090	422.3E6	235.4E6	500.000	500.000
29) L6 AR-1254-4	6.348	6.317	264.0E6	132.2E6	500.000	500.000
30) L6 AR-1254-5	6.767	6.733	395.8E6	178.0E6	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0070825\
 Data File : P0112107.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jul 2025 19:54
 Operator : YP/AJ
 Sample : AR1254ICC500
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1254ICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 09 03:13:37 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 09 03:10:24 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ m Signal #2 Info : 30M x 0.32mm x 0.25 μ m

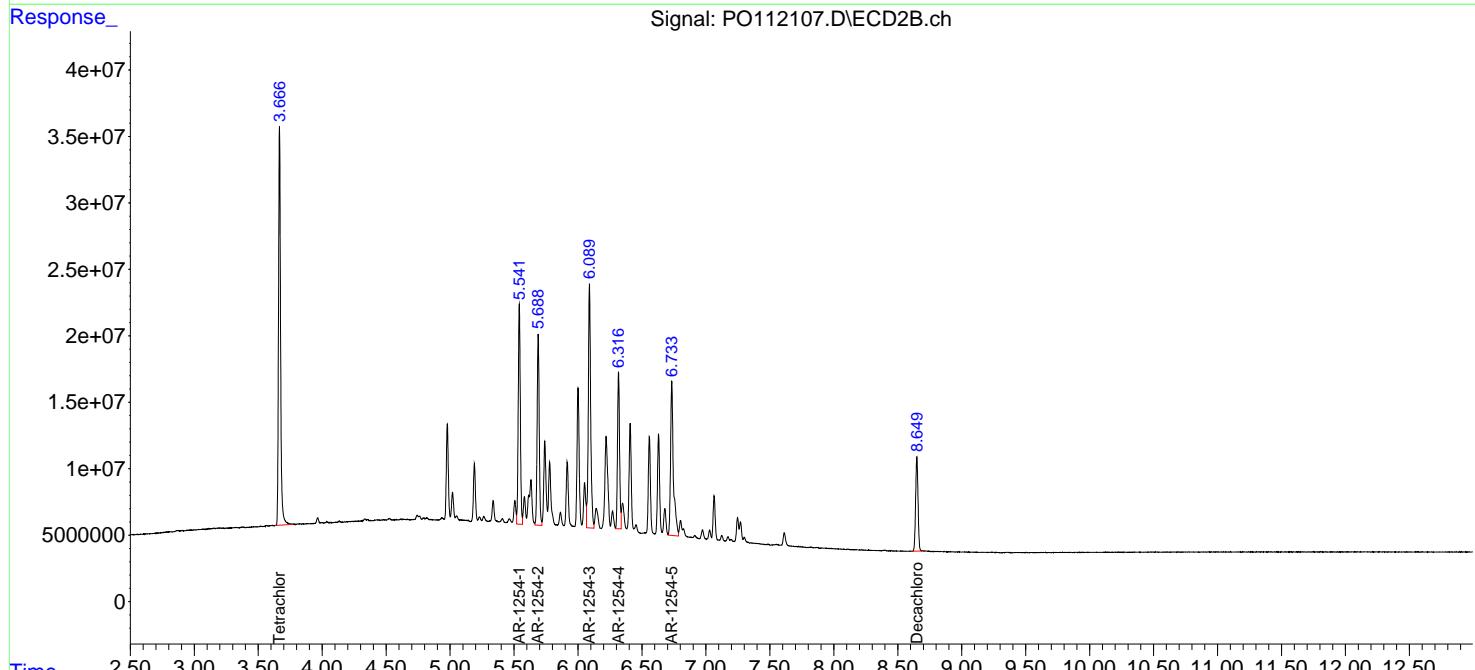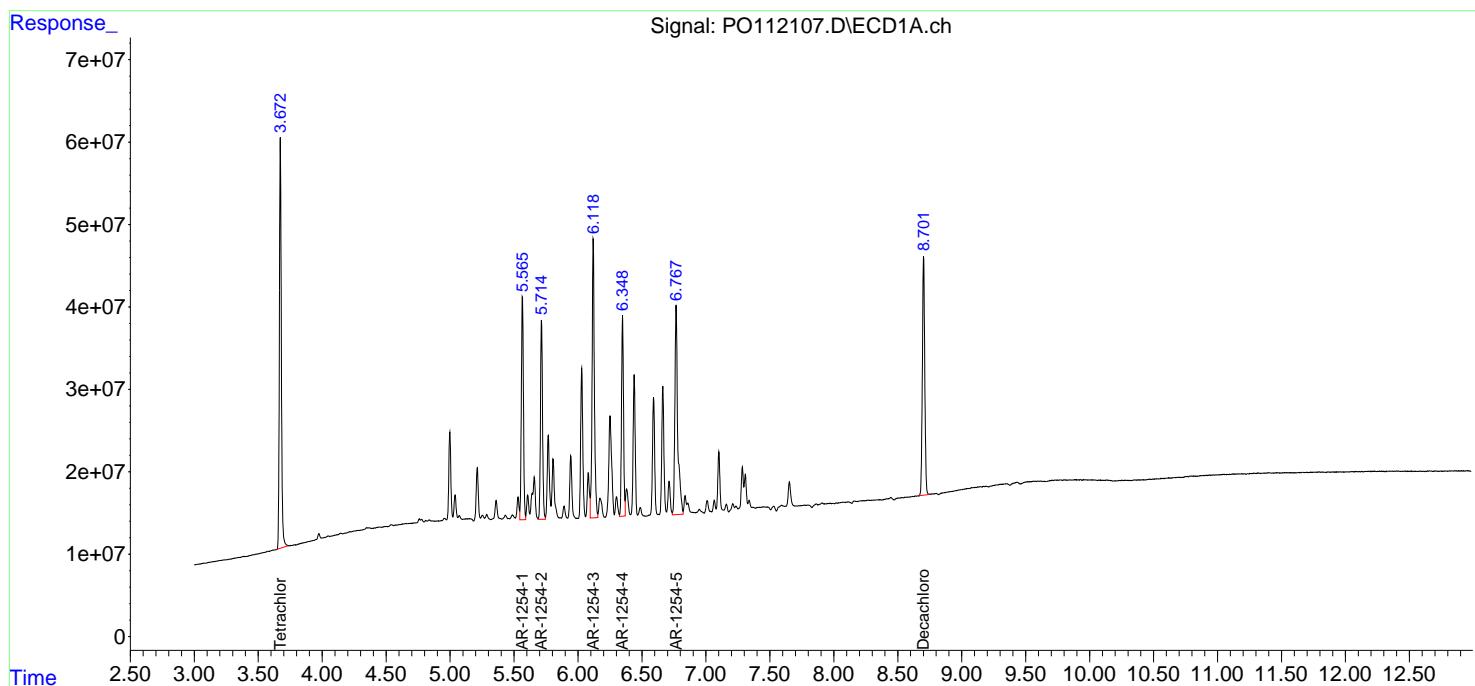

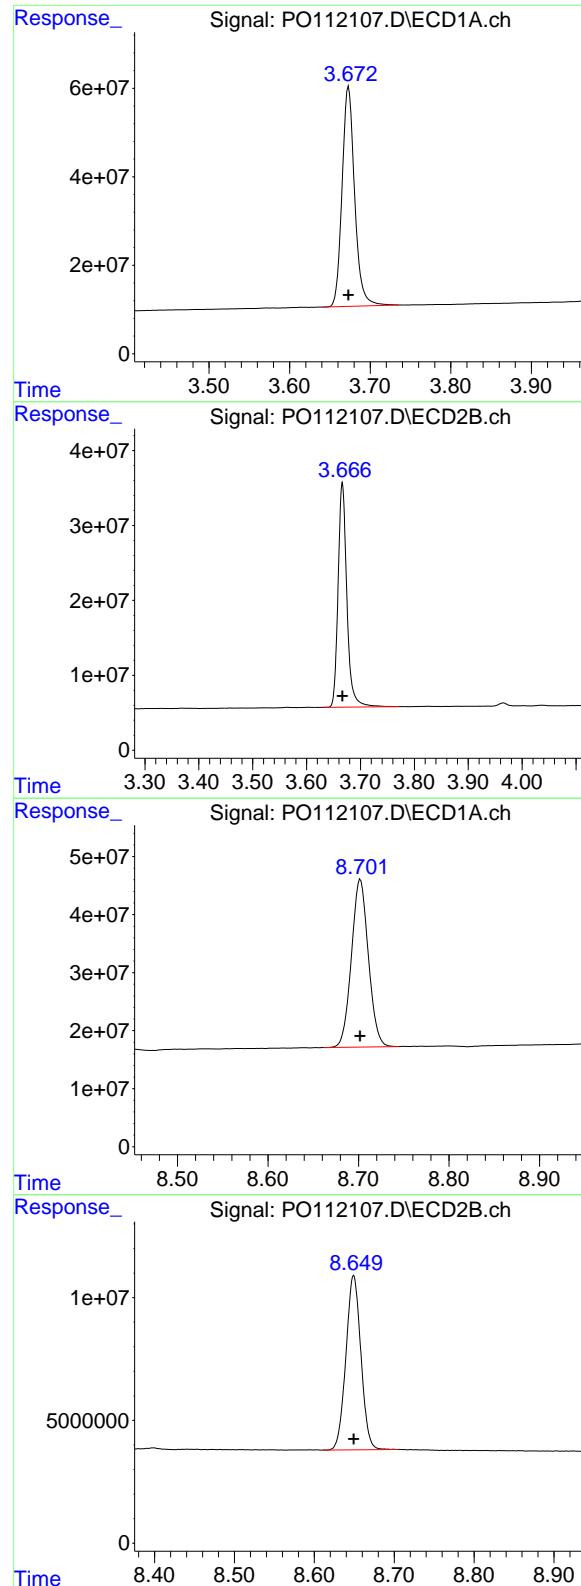

#1 Tetrachloro-m-xylene

R.T.: 3.673 min
 Delta R.T.: 0.000 min
 Response: 537493163
 Conc: 50.00 ng/ml

Instrument:

ECD_O

ClientSampleId :

AR1254ICC500

#1 Tetrachloro-m-xylene

R.T.: 3.666 min
 Delta R.T.: 0.000 min
 Response: 339534317
 Conc: 50.00 ng/ml

#2 Decachlorobiphenyl

R.T.: 8.702 min
 Delta R.T.: 0.000 min
 Response: 376245478
 Conc: 50.00 ng/ml


#2 Decachlorobiphenyl

R.T.: 8.649 min
 Delta R.T.: 0.000 min
 Response: 92613439
 Conc: 50.00 ng/ml

#26 AR-1254-1


R.T.: 5.566 min
 Delta R.T.: 0.000 min
 Response: 307778107
 Conc: 500.00 ng/ml

Instrument: ECD_O
ClientSampleId: AR1254ICC500




#26 AR-1254-1

R.T.: 5.541 min
 Delta R.T.: 0.000 min
 Response: 188309119
 Conc: 500.00 ng/ml

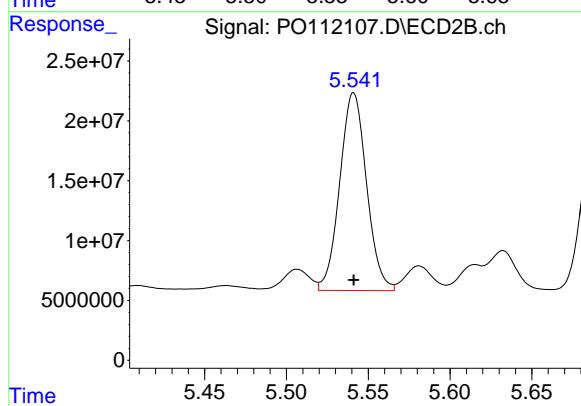


#27 AR-1254-2

R.T.: 5.715 min
 Delta R.T.: 0.000 min
 Response: 269164575
 Conc: 500.00 ng/ml



#27 AR-1254-2


R.T.: 5.689 min
 Delta R.T.: 0.000 min
 Response: 162981710
 Conc: 500.00 ng/ml

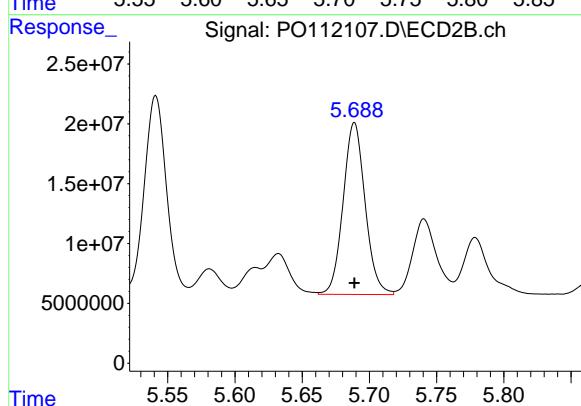

#28 AR-1254-3


R.T.: 6.119 min
 Delta R.T.: 0.000 min
 Response: 422299438
 Conc: 500.00 ng/ml

Instrument: ECD_O
ClientSampleId: AR1254ICC500




#28 AR-1254-3

R.T.: 6.090 min
 Delta R.T.: 0.000 min
 Response: 235353258
 Conc: 500.00 ng/ml

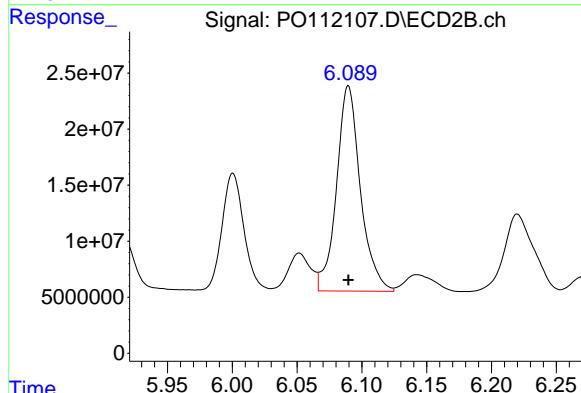


#29 AR-1254-4

R.T.: 6.348 min
 Delta R.T.: 0.000 min
 Response: 264023259
 Conc: 500.00 ng/ml

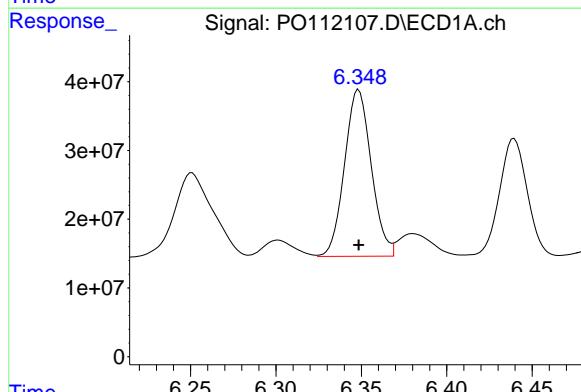


#29 AR-1254-4

R.T.: 6.317 min
 Delta R.T.: 0.000 min
 Response: 132233057
 Conc: 500.00 ng/ml

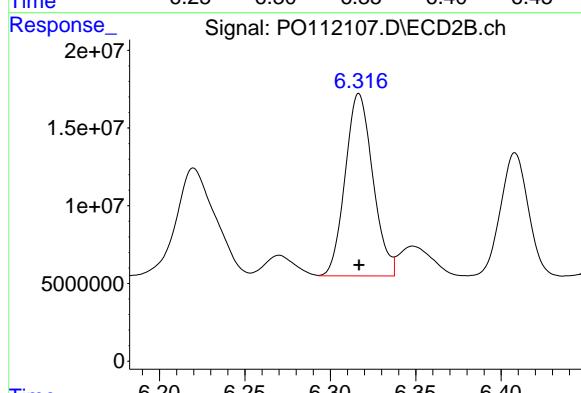


#30 AR-1254-5

R.T.: 6.767 min
Delta R.T.: 0.000 min **Instrument:**
Response: 395760704 ECD_O
Conc: 500.00 ng/ml **ClientSampleId :**
AR1254ICC500

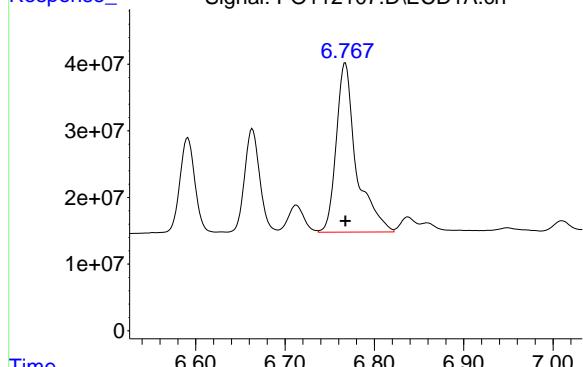

#30 AR-1254-5

R.T.: 6.733 min
Delta R.T.: 0.000 min
Response: 178024264
Conc: 500.00 ng/ml

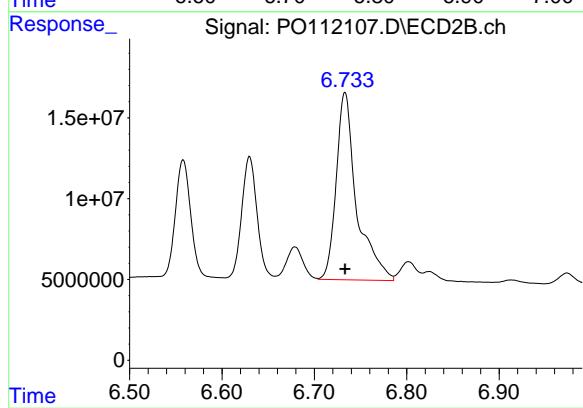

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0070825\
 Data File : P0112108.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jul 2025 20:11
 Operator : YP/AJ
 Sample : AR1254ICC250
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1254ICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 09 03:13:48 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 09 03:10:24 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	3.672	3.666	272.9E6	171.8E6	25.384	25.306
2) SA Decachlor...	8.702	8.649	190.5E6	47874492	25.314	25.846

Target Compounds

26) L6 AR-1254-1	5.565	5.541	157.8E6	101.2E6	256.353	268.788
27) L6 AR-1254-2	5.714	5.688	138.2E6	87586236	256.712	268.700
28) L6 AR-1254-3	6.117	6.089	215.5E6	124.2E6	255.127	263.865
29) L6 AR-1254-4	6.346	6.317	128.5E6	68432623	243.355	258.758
30) L6 AR-1254-5	6.766	6.733	201.3E6	93511862	254.294	262.638



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0070825\
 Data File : P0112108.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jul 2025 20:11
 Operator : YP/AJ
 Sample : AR1254ICC250
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1254ICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 09 03:13:48 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 09 03:10:24 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

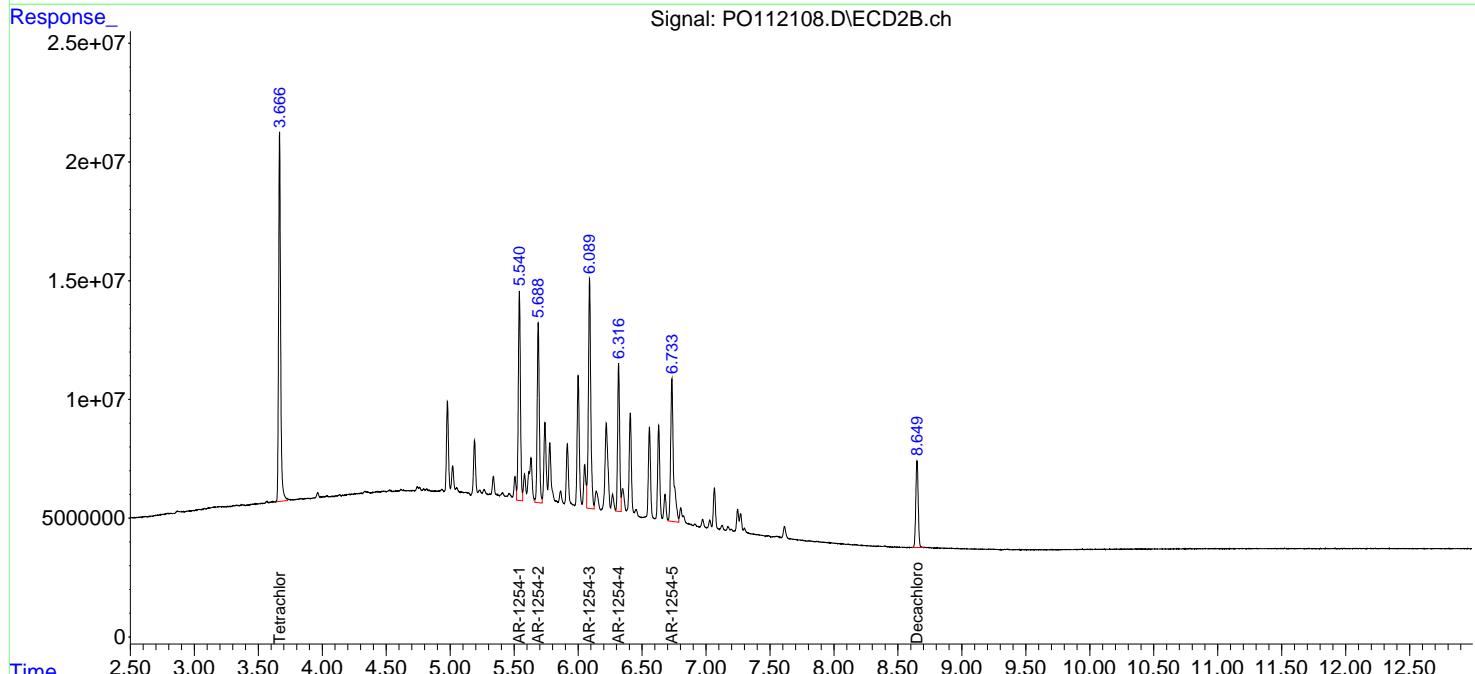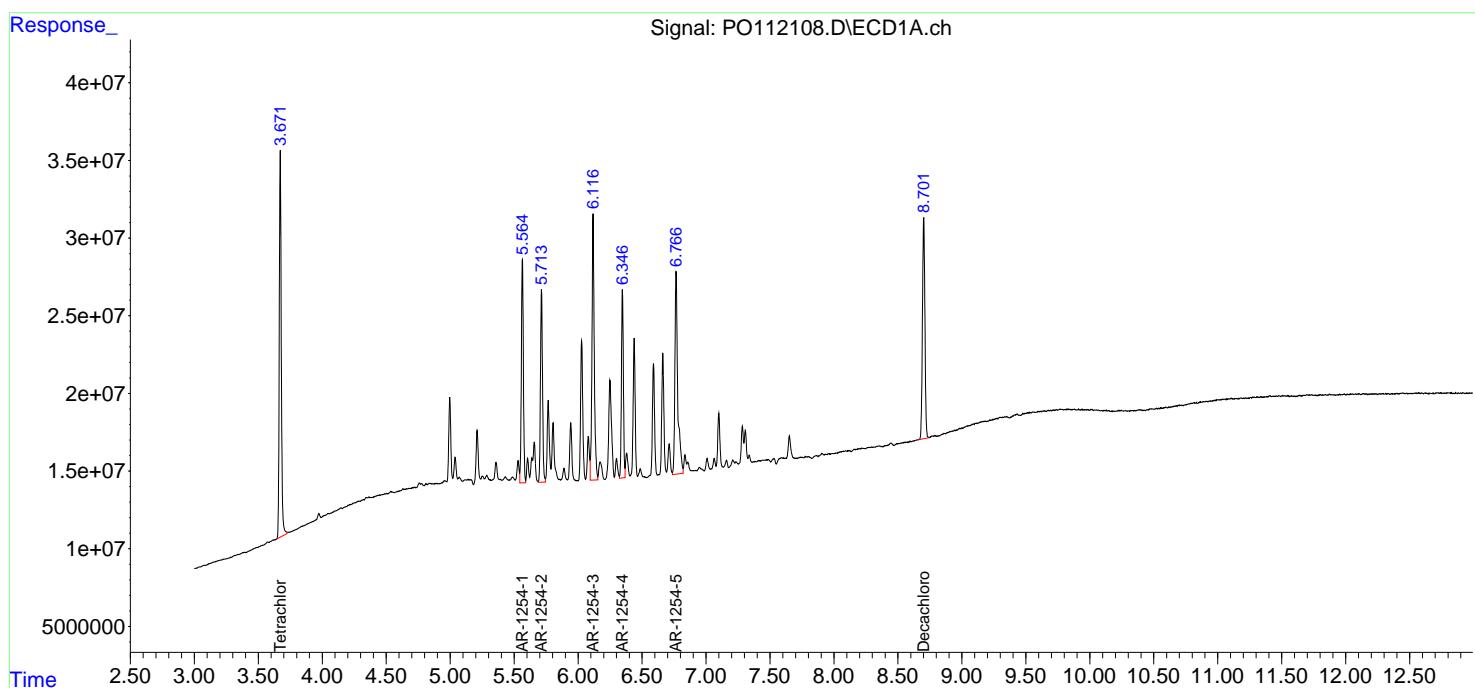

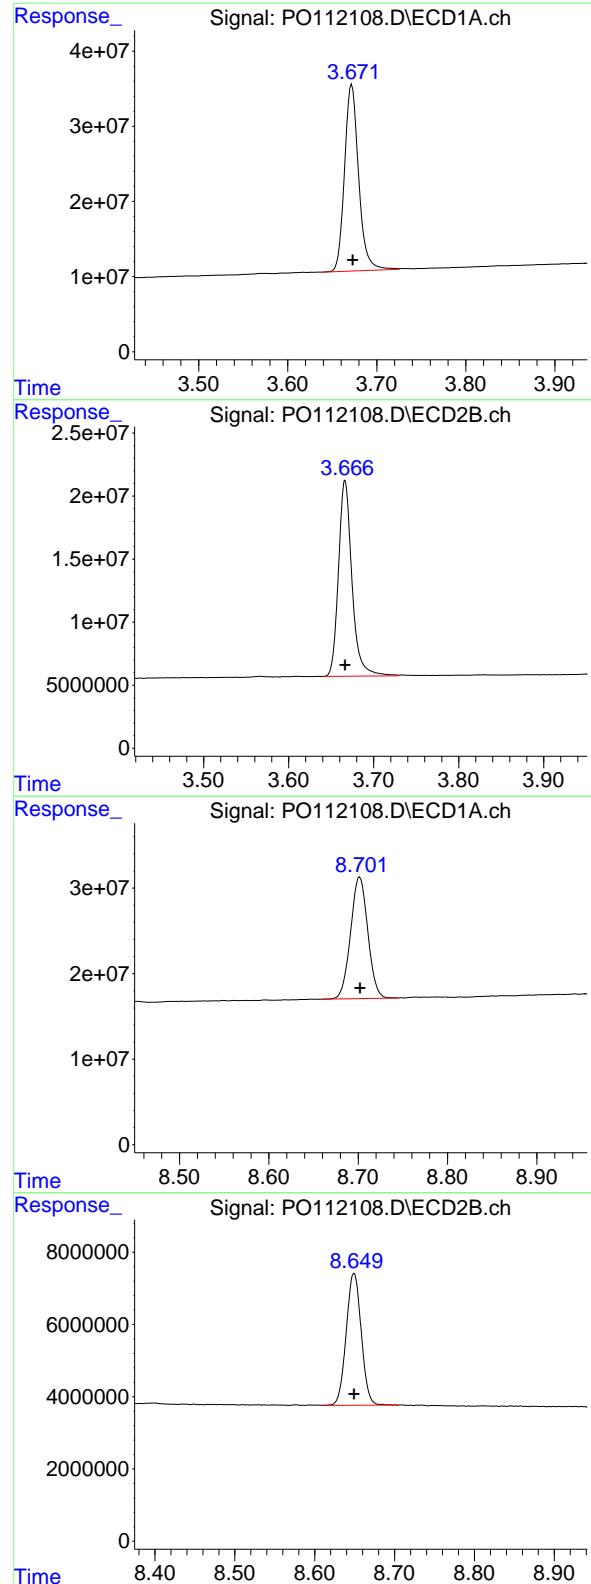

#1 Tetrachloro-m-xylene

R.T.: 3.672 min

Delta R.T.: -0.001 min

Response: 272878230

Conc: 25.38 ng/ml

Instrument:

ECD_O

ClientSampleId :

AR1254ICC250

#1 Tetrachloro-m-xylene

R.T.: 3.666 min

Delta R.T.: 0.000 min

Response: 171848191

Conc: 25.31 ng/ml

#2 Decachlorobiphenyl

R.T.: 8.702 min

Delta R.T.: 0.000 min

Response: 190488487

Conc: 25.31 ng/ml

#2 Decachlorobiphenyl

R.T.: 8.649 min

Delta R.T.: 0.000 min


Response: 47874492

Conc: 25.85 ng/ml

#26 AR-1254-1


R.T.: 5.565 min
 Delta R.T.: -0.001 min
 Response: 157799382
 Conc: 256.35 ng/ml

Instrument: ECD_O
ClientSampleId: AR1254ICC250

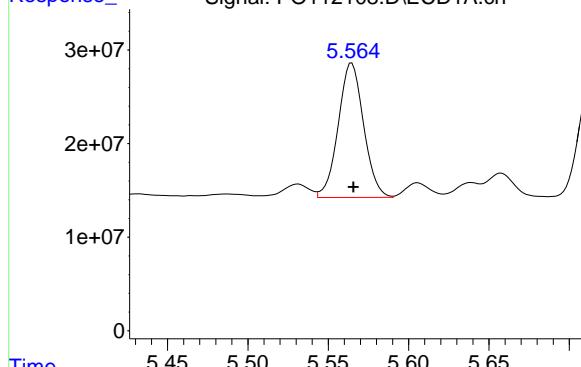


#26 AR-1254-1

R.T.: 5.541 min
 Delta R.T.: 0.000 min
 Response: 101230376
 Conc: 268.79 ng/ml

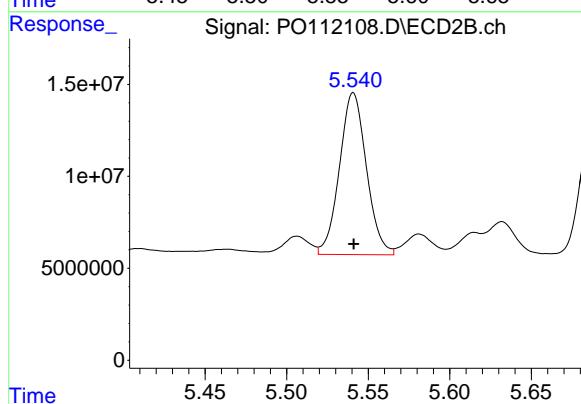


#27 AR-1254-2

R.T.: 5.714 min
 Delta R.T.: 0.000 min
 Response: 138195636
 Conc: 256.71 ng/ml



#27 AR-1254-2





R.T.: 5.688 min
 Delta R.T.: 0.000 min
 Response: 87586236
 Conc: 268.70 ng/ml

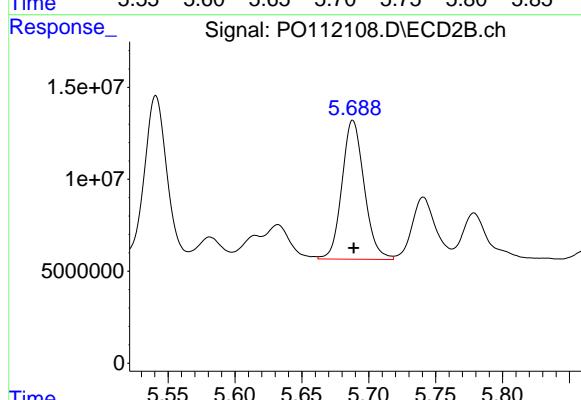

#28 AR-1254-3

R.T.: 6.117 min
 Delta R.T.: -0.002 min
 Response: 215480050
 Conc: 255.13 ng/ml

Instrument: ECD_O
ClientSampleId: AR1254ICC250

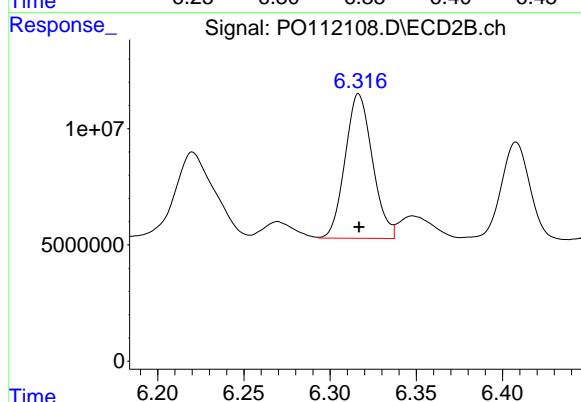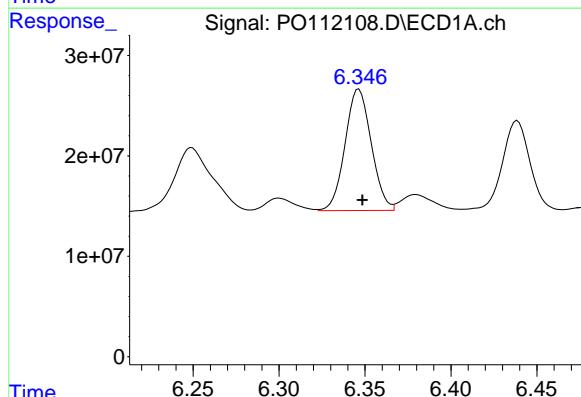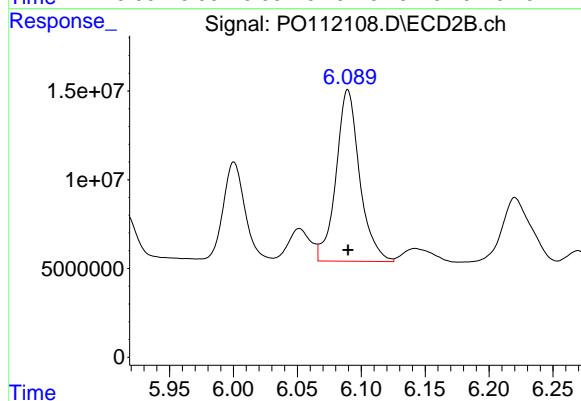

#28 AR-1254-3

R.T.: 6.089 min
 Delta R.T.: 0.000 min
 Response: 124203187
 Conc: 263.87 ng/ml

#29 AR-1254-4

R.T.: 6.346 min
 Delta R.T.: -0.002 min
 Response: 128502801
 Conc: 243.36 ng/ml



#29 AR-1254-4

R.T.: 6.317 min
 Delta R.T.: 0.000 min
 Response: 68432623
 Conc: 258.76 ng/ml

#30 AR-1254-5

R.T.: 6.766 min
Delta R.T.: -0.001 min
Response: 201279357
Conc: 254.29 ng/ml

Instrument: ECD_O
ClientSampleId: AR1254ICC250

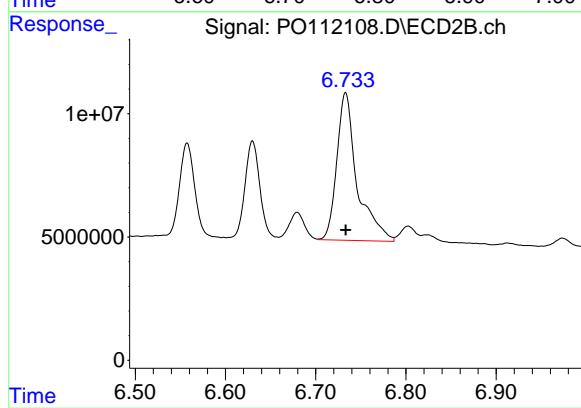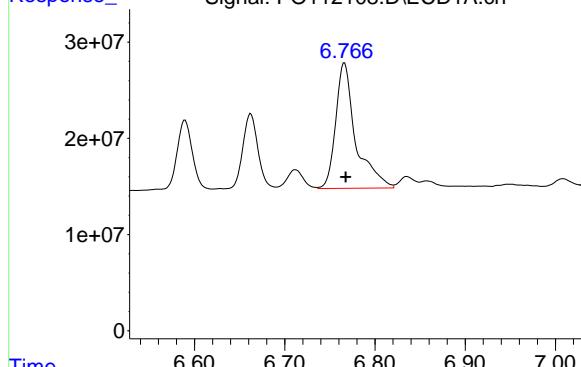

#30 AR-1254-5

R.T.: 6.733 min
Delta R.T.: 0.000 min
Response: 93511862
Conc: 262.64 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0070825\
 Data File : P0112109.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jul 2025 20:28
 Operator : YP/AJ
 Sample : AR1254ICC050
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1254ICC050

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/09/2025
 Supervised By :mohammad ahmed 07/10/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 09 03:13:58 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 09 03:10:24 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	3.672	3.666	45533046	29689581	4.236	4.372
2) SA Decachlor...	8.701	8.650	32557073	8527820	4.327	4.604

Target Compounds

26) L6 AR-1254-1	5.565	5.540	30856160	19661689	50.127	52.206m
27) L6 AR-1254-2	5.714	5.688	25962033	17746073	48.227	54.442m
28) L6 AR-1254-3	6.118	6.089	40531096	25609316	47.989	54.406
29) L6 AR-1254-4	6.345	6.316	16204940	12905837	30.688m	48.800 #
30) L6 AR-1254-5	6.765	6.733	35718880	18096474	45.127	50.826

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0070825\
 Data File : P0112109.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jul 2025 20:28
 Operator : YP/AJ
 Sample : AR1254ICC050
 Misc :
 ALS Vial : 24 Sample Multiplier: 1



Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 09 03:13:58 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 09 03:10:24 2025
 Response via : Initial Calibration
 Integrator: ChemStation


Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Instrument :
 ECD_O
ClientSampleId :
 AR1254ICC050

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/09/2025
 Supervised By :mohammad ahmed 07/10/2025

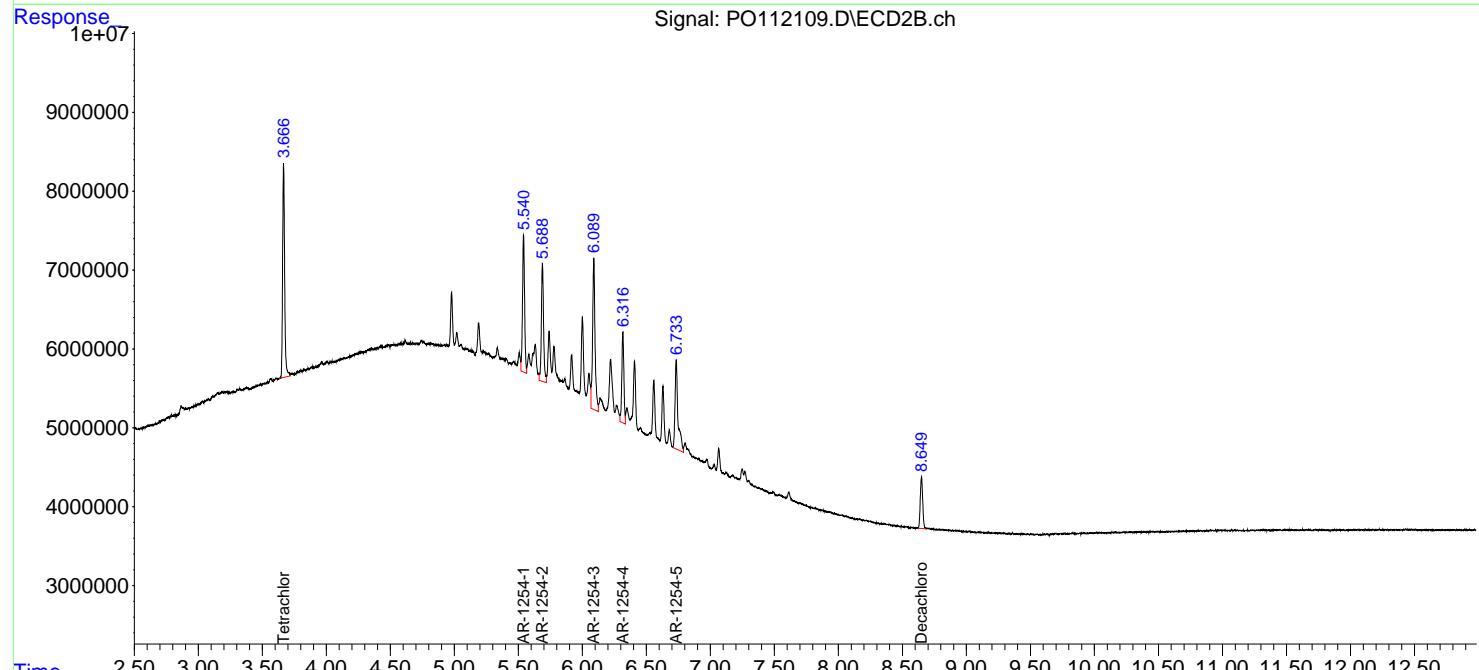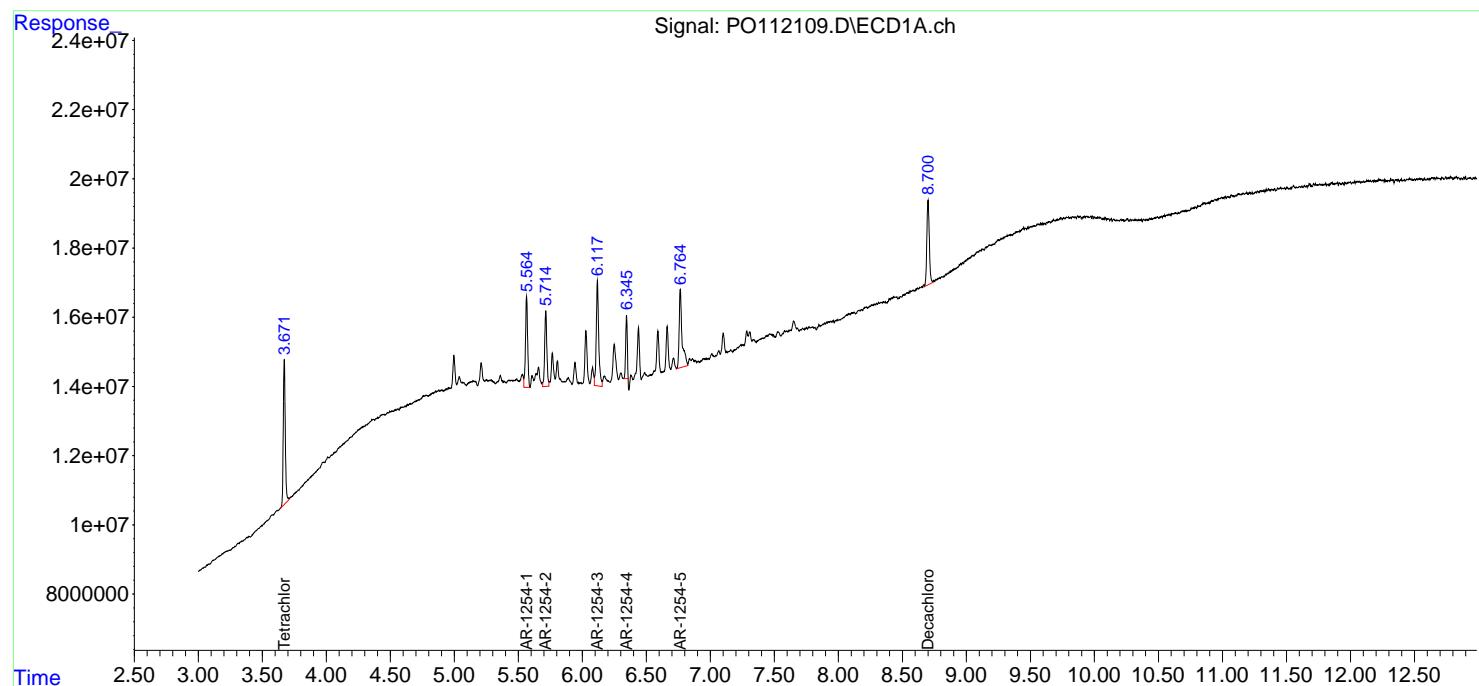

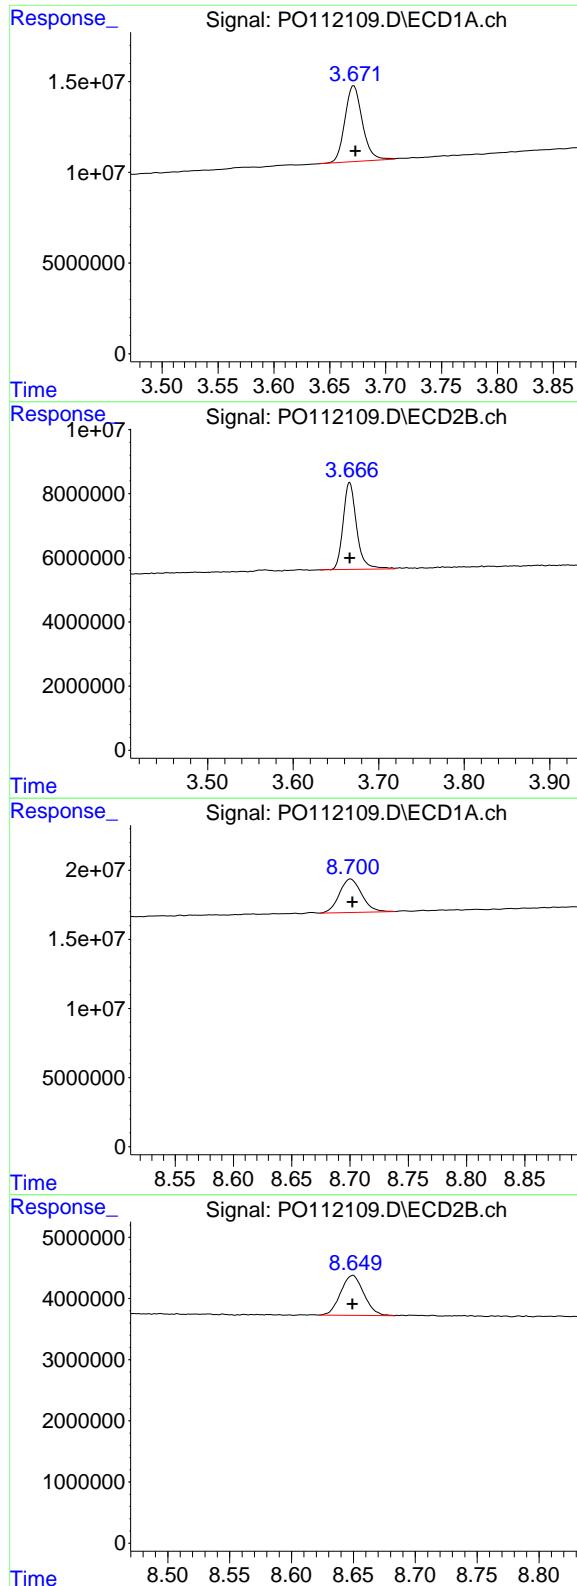

#1 Tetrachloro-m-xylene

R.T.: 3.672 min
Delta R.T.: -0.001 min
Response: 45533046
Conc: 4.24 ng/ml

Instrument: ECD_O
ClientSampleId: AR1254ICC050

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/09/2025
Supervised By :mohammad ahmed 07/10/2025

#1 Tetrachloro-m-xylene

R.T.: 3.666 min
Delta R.T.: 0.000 min
Response: 29689581
Conc: 4.37 ng/ml

#2 Decachlorobiphenyl

R.T.: 8.701 min
Delta R.T.: -0.001 min
Response: 32557073
Conc: 4.33 ng/ml

#2 Decachlorobiphenyl

R.T.: 8.650 min
Delta R.T.: 0.000 min
Response: 8527820
Conc: 4.60 ng/ml

#26 AR-1254-1

R.T.: 5.565 min
 Delta R.T.: -0.001 min
 Response: 30856160
 Conc: 50.13 ng/ml

Instrument: ECD_O
ClientSampleId: AR1254ICC050

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/09/2025
 Supervised By :mohammad ahmed 07/10/2025

#26 AR-1254-1





R.T.: 5.540 min
 Delta R.T.: -0.001 min
 Response: 19661689
 Conc: 52.21 ng/ml


#27 AR-1254-2

R.T.: 5.714 min
 Delta R.T.: 0.000 min
 Response: 25962033
 Conc: 48.23 ng/ml

#27 AR-1254-2

R.T.: 5.688 min
 Delta R.T.: -0.001 min
 Response: 17746073
 Conc: 54.44 ng/ml

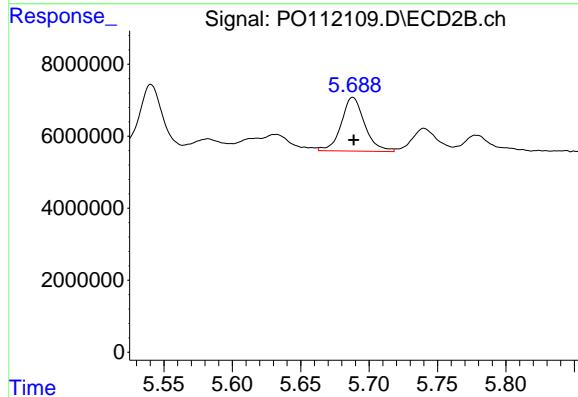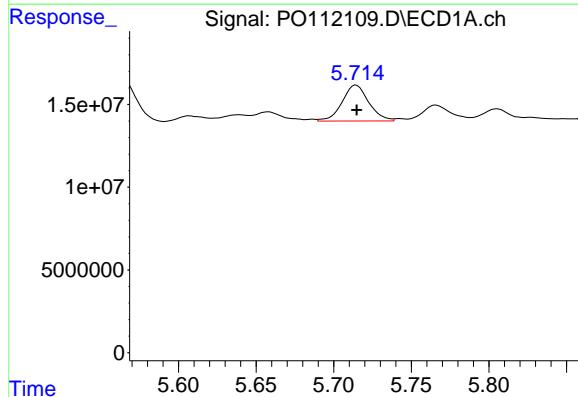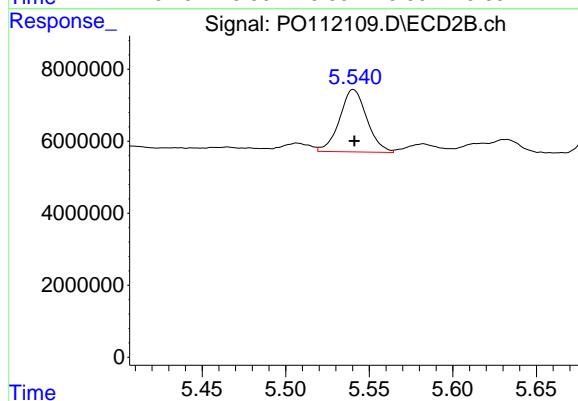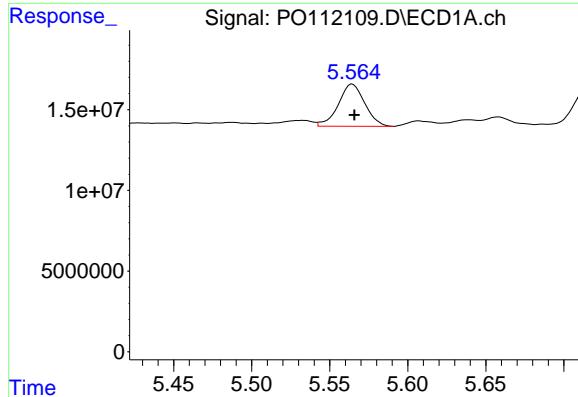

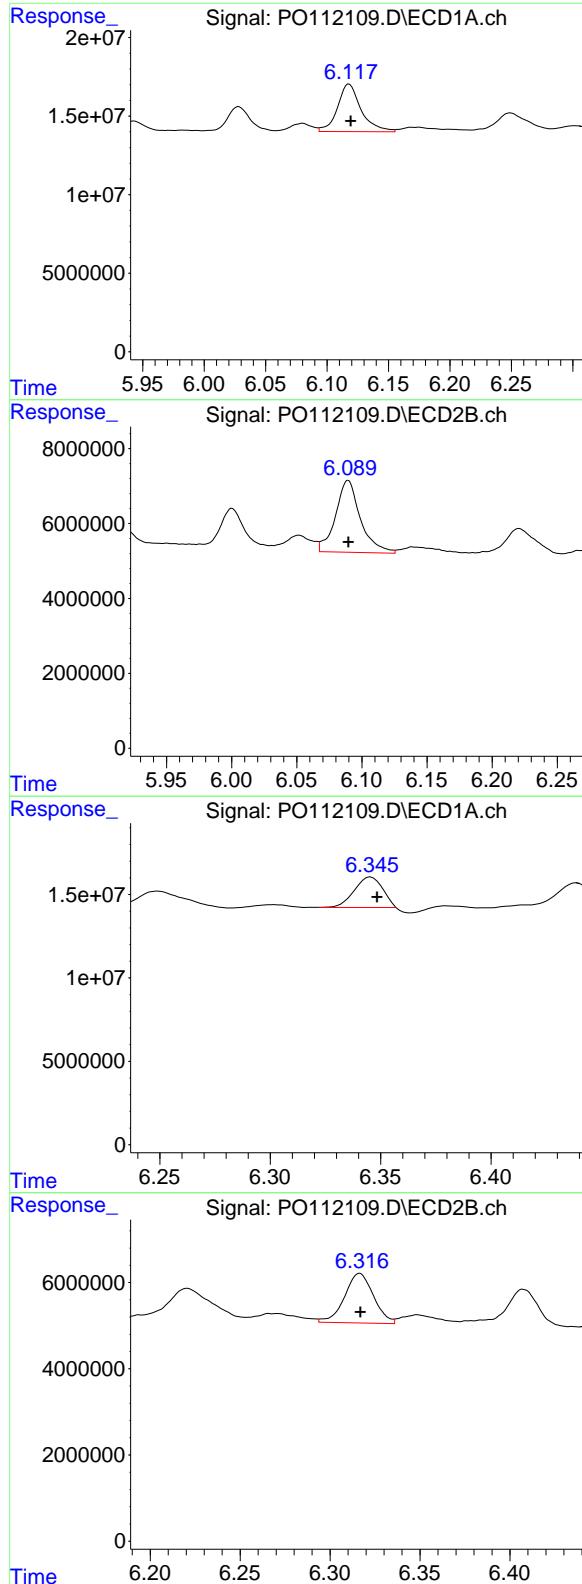

#28 AR-1254-3

R.T.: 6.118 min
 Delta R.T.: -0.001 min
 Response: 40531096
 Conc: 47.99 ng/ml

Instrument: ECD_O
ClientSampleId: AR1254ICC050

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/09/2025
 Supervised By :mohammad ahmed 07/10/2025

#28 AR-1254-3

R.T.: 6.089 min
 Delta R.T.: 0.000 min
 Response: 25609316
 Conc: 54.41 ng/ml

#29 AR-1254-4

R.T.: 6.345 min
 Delta R.T.: -0.004 min
 Response: 16204940
 Conc: 30.69 ng/ml

#29 AR-1254-4

R.T.: 6.316 min
 Delta R.T.: 0.000 min
 Response: 12905837
 Conc: 48.80 ng/ml



#30 AR-1254-5

R.T.: 6.765 min
 Delta R.T.: -0.002 min
 Response: 35718880
 Conc: 45.13 ng/ml

Instrument: ECD_O
ClientSampleId: AR1254ICC050

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/09/2025
 Supervised By :mohammad ahmed 07/10/2025

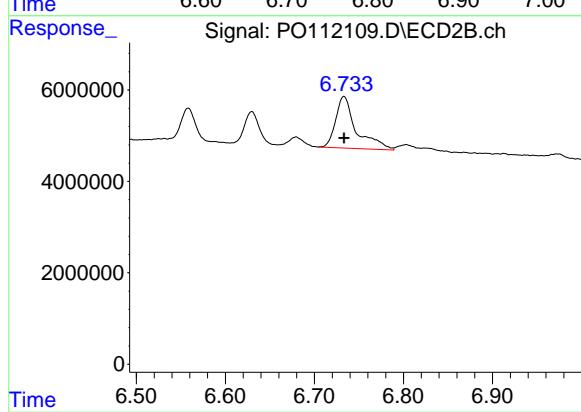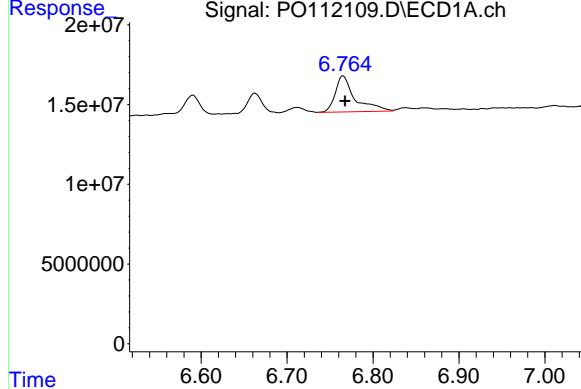

#30 AR-1254-5

R.T.: 6.733 min
 Delta R.T.: 0.000 min
 Response: 18096474
 Conc: 50.83 ng/ml

1
2
3
4
5
6
7
8
9
10
11
12
13
14
15
16
17
18
19
20

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0070825\
 Data File : P0112110.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jul 2025 20:47
 Operator : YP/AJ
 Sample : AR1262ICC500
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1262ICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 09 03:29:27 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 09 03:25:20 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	3.672	3.666	525.8E6	329.4E6	50.000	50.000
2) SA Decachlor...	8.703	8.651	370.9E6	90608483	50.000	50.000

Target Compounds

36) L8 AR-1262-1	6.807	6.772	510.8E6	203.7E6	500.000	500.000
37) L8 AR-1262-2	7.310	7.272	819.7E6	256.3E6	500.000	500.000
38) L8 AR-1262-3	7.592	7.554	321.0E6	89762034	500.000	500.000
39) L8 AR-1262-4	7.657	7.618	535.7E6	145.5E6	500.000	500.000
40) L8 AR-1262-5	8.153	8.110	224.1E6	52891763	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0070825\
 Data File : P0112110.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jul 2025 20:47
 Operator : YP/AJ
 Sample : AR1262ICC500
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1262ICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 09 03:29:27 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 09 03:25:20 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

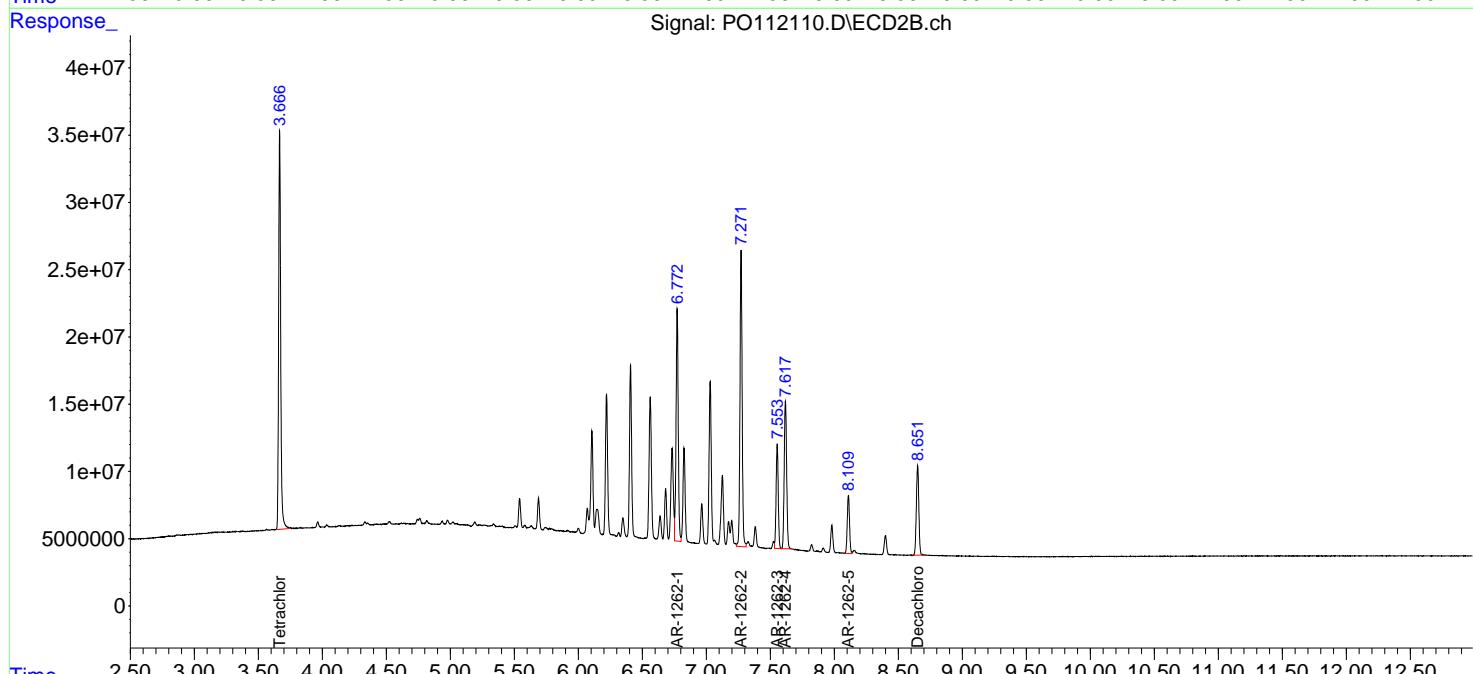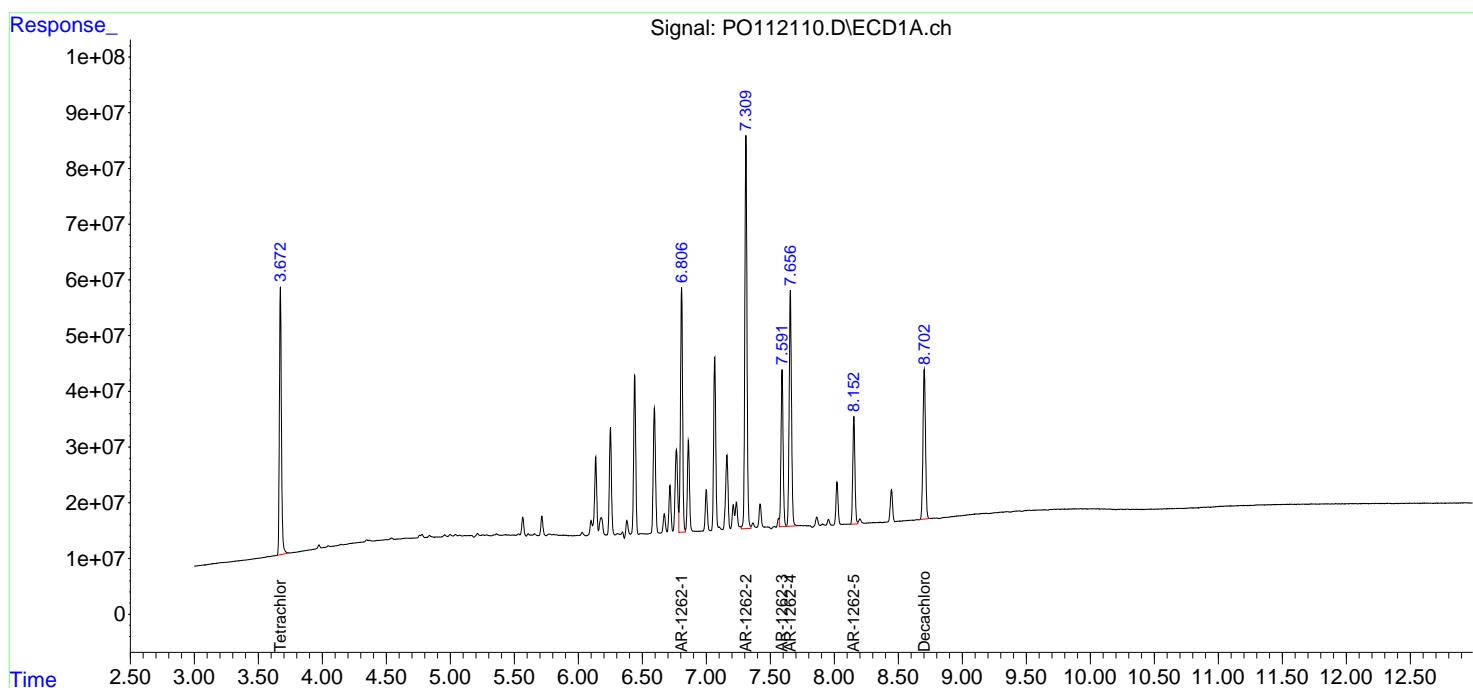

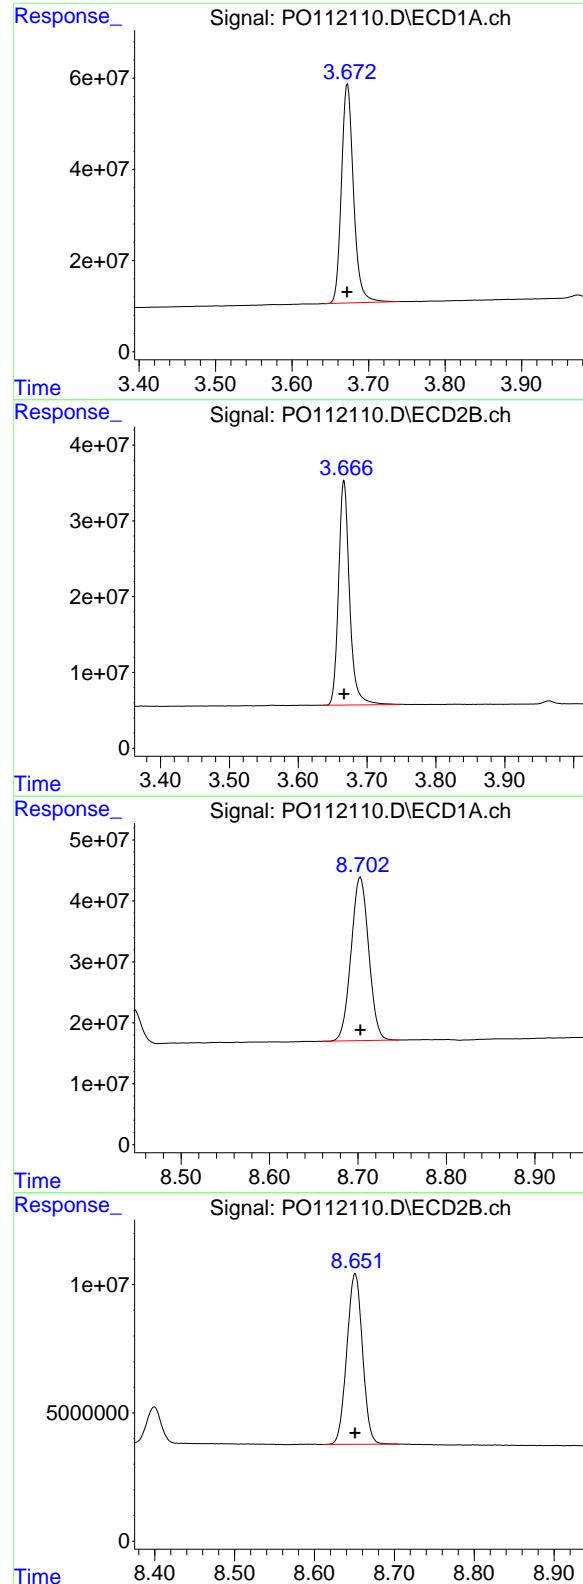

#1 Tetrachloro-m-xylene

R.T.: 3.672 min
 Delta R.T.: 0.000 min
 Response: 525756507
 Conc: 50.00 ng/ml

Instrument:

ECD_O

ClientSampleId :

AR1262ICC500

#1 Tetrachloro-m-xylene

R.T.: 3.666 min
 Delta R.T.: 0.000 min
 Response: 329387316
 Conc: 50.00 ng/ml

#2 Decachlorobiphenyl

R.T.: 8.703 min
 Delta R.T.: 0.000 min
 Response: 370896650
 Conc: 50.00 ng/ml


#2 Decachlorobiphenyl

R.T.: 8.651 min
 Delta R.T.: 0.000 min
 Response: 90608483
 Conc: 50.00 ng/ml

#36 AR-1262-1


R.T.: 6.807 min
 Delta R.T.: 0.000 min
 Response: 510843479
 Conc: 500.00 ng/ml

Instrument: ECD_O
ClientSampleId: AR1262ICC500

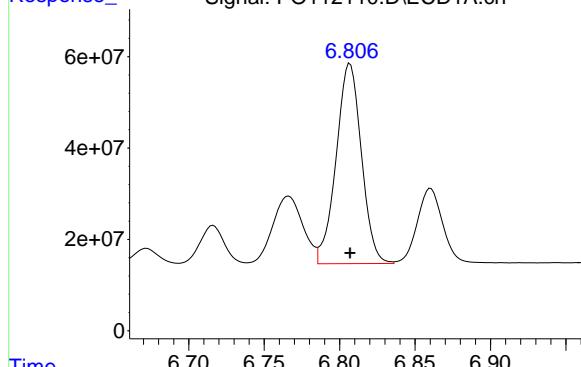


#36 AR-1262-1

R.T.: 6.772 min
 Delta R.T.: 0.000 min
 Response: 203660426
 Conc: 500.00 ng/ml

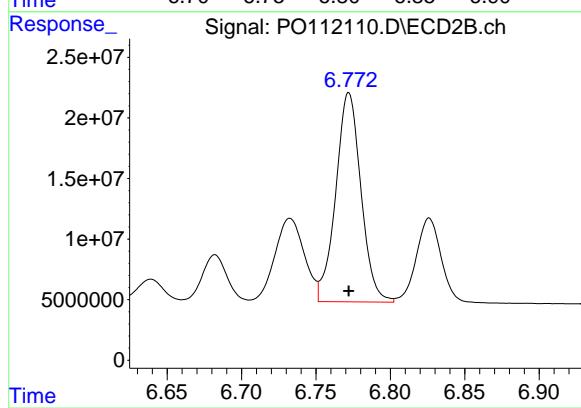


#37 AR-1262-2

R.T.: 7.310 min
 Delta R.T.: 0.000 min
 Response: 819686360
 Conc: 500.00 ng/ml

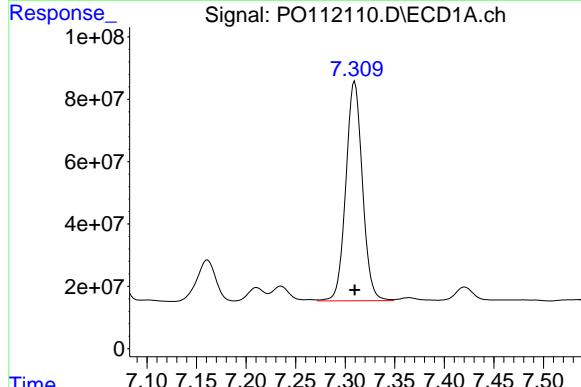

#37 AR-1262-2





R.T.: 7.272 min
 Delta R.T.: 0.000 min
 Response: 256274286
 Conc: 500.00 ng/ml

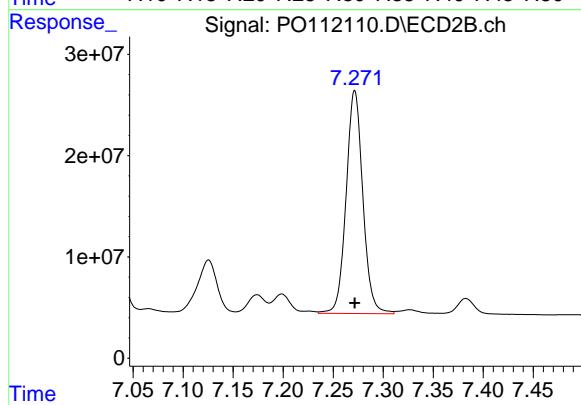

#38 AR-1262-3

R.T.: 7.592 min
 Delta R.T.: 0.000 min
 Response: 320987602
 Conc: 500.00 ng/ml

Instrument: ECD_O
ClientSampleId: AR1262ICC500

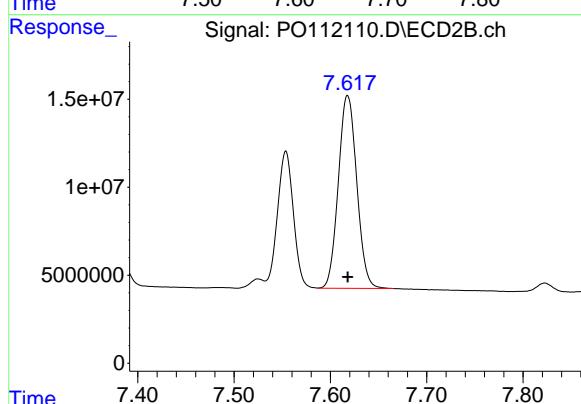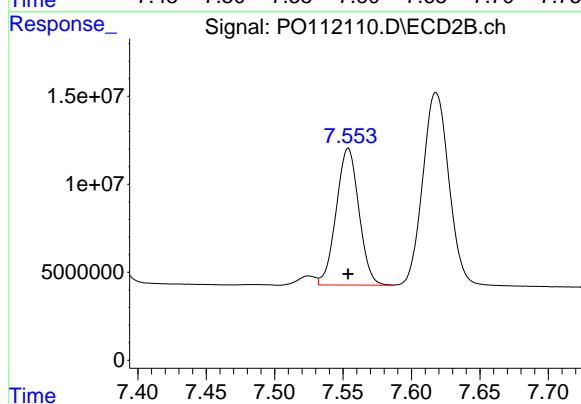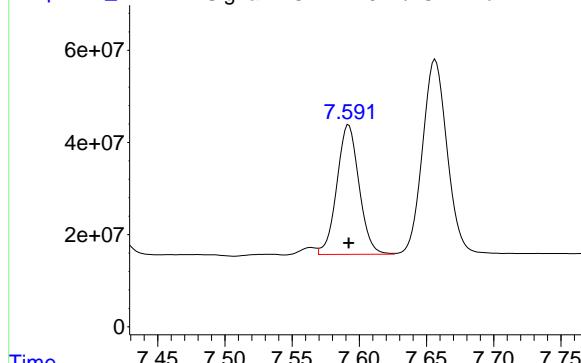

#38 AR-1262-3

R.T.: 7.554 min
 Delta R.T.: 0.000 min
 Response: 89762034
 Conc: 500.00 ng/ml

#39 AR-1262-4

R.T.: 7.657 min
 Delta R.T.: 0.000 min
 Response: 535717312
 Conc: 500.00 ng/ml



#39 AR-1262-4

R.T.: 7.618 min
 Delta R.T.: 0.000 min
 Response: 145459780
 Conc: 500.00 ng/ml

#40 AR-1262-5

R.T.: 8.153 min
Delta R.T.: 0.000 min
Response: 224070443
Conc: 500.00 ng/ml

Instrument: ECD_O
ClientSampleId: AR1262ICC500

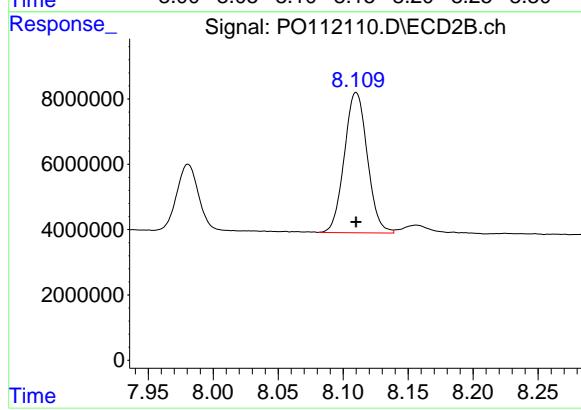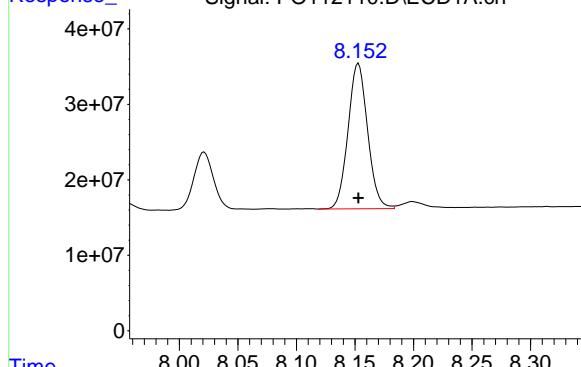

#40 AR-1262-5

R.T.: 8.110 min
Delta R.T.: 0.000 min
Response: 52891763
Conc: 500.00 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0070825\
 Data File : P0112111.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jul 2025 21:04
 Operator : YP/AJ
 Sample : AR1268ICC1000
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1268ICC1000

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/09/2025
 Supervised By :mohammad ahmed 07/10/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 09 03:41:55 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 09 03:33:24 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	3.672	3.667	1082.8E6	673.3E6	101.066	99.562
2) SA Decachlor...	8.702	8.650	1378.0E6	313.9E6	99.628	96.478

Target Compounds

41) L9 AR-1268-1	7.590	7.554	1933.7E6	486.6E6	1000.189	974.104
42) L9 AR-1268-2	7.656	7.619	1621.3E6	414.1E6	997.801	973.991
43) L9 AR-1268-3	7.862	7.823	1337.7E6	309.6E6	989.536	960.409
44) L9 AR-1268-4	8.151	8.111	501.7E6	111.4E6	975.950m	963.536
45) L9 AR-1268-5	8.445	8.399	3474.7E6	736.5E6	1008.979	983.566

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0070825\
 Data File : P0112111.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jul 2025 21:04
 Operator : YP/AJ
 Sample : AR1268ICC1000
 Misc :
 ALS Vial : 26 Sample Multiplier: 1



Instrument :
 ECD_O
 ClientSampleId :
 AR1268ICC1000





Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/09/2025
 Supervised By :mohammad ahmed 07/10/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 09 03:41:55 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 09 03:33:24 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

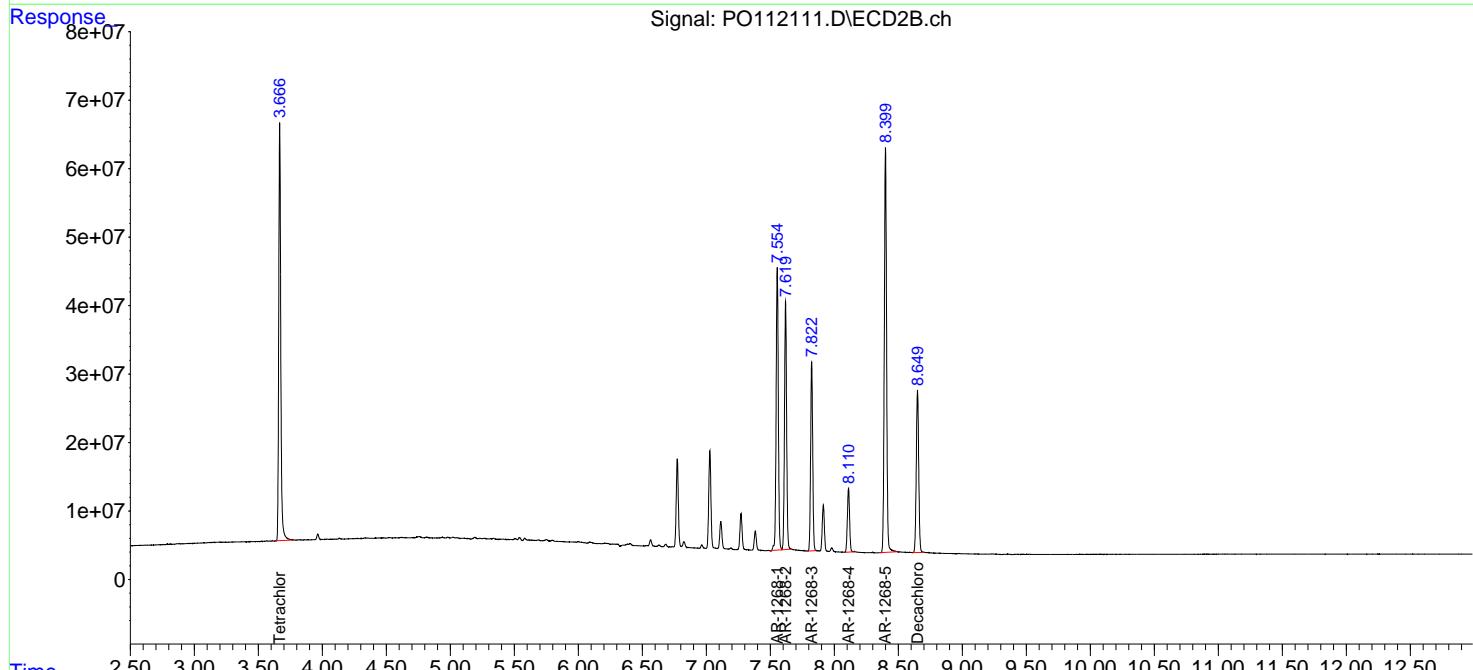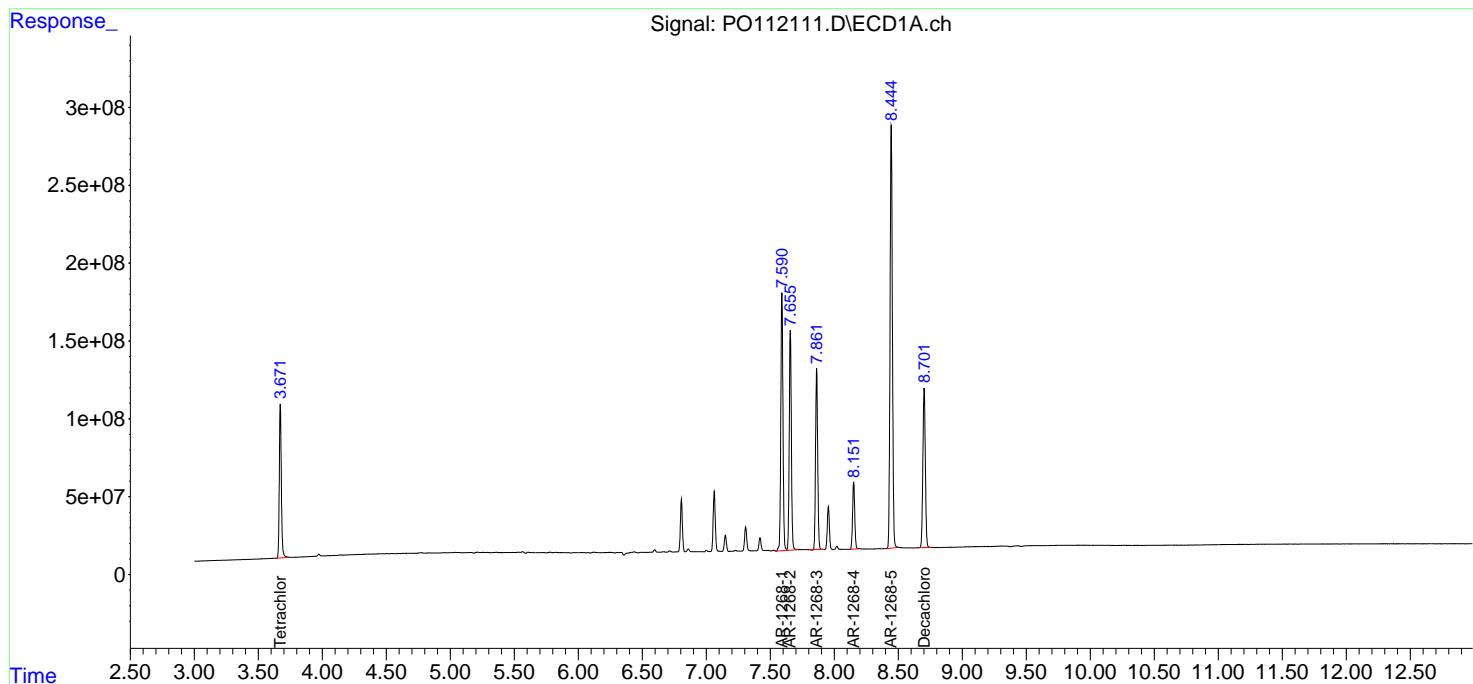

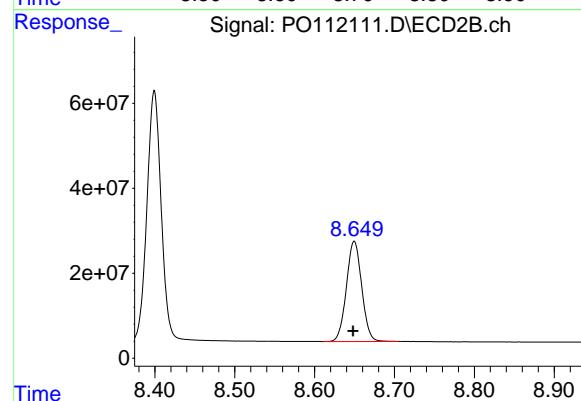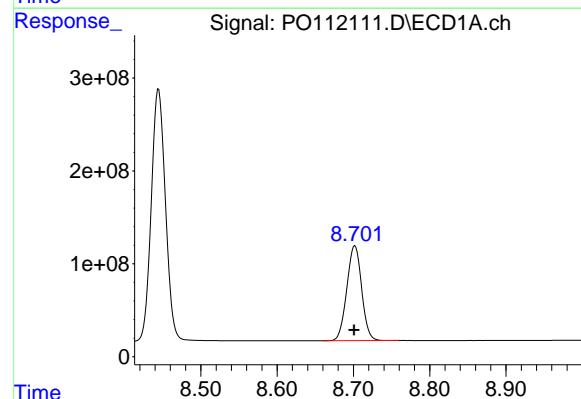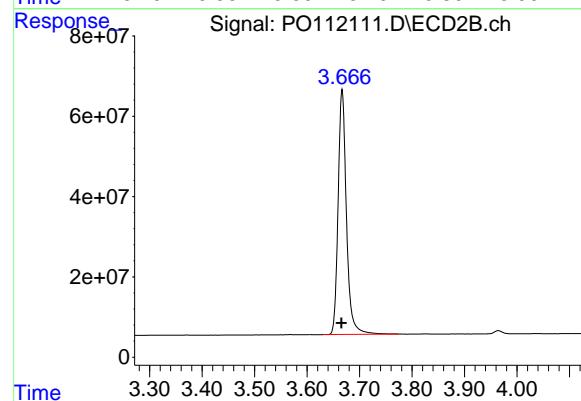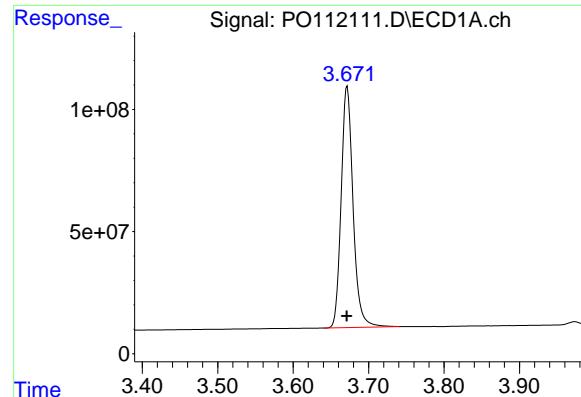




#1 Tetrachloro-m-xylene

R.T.: 3.672 min
Delta R.T.: 0.000 min
Response: 1082841647
Conc: 101.07 ng/ml

Instrument:
ECD_O
ClientSampleId :
AR1268ICC1000

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/09/2025
Supervised By :mohammad ahmed 07/10/2025

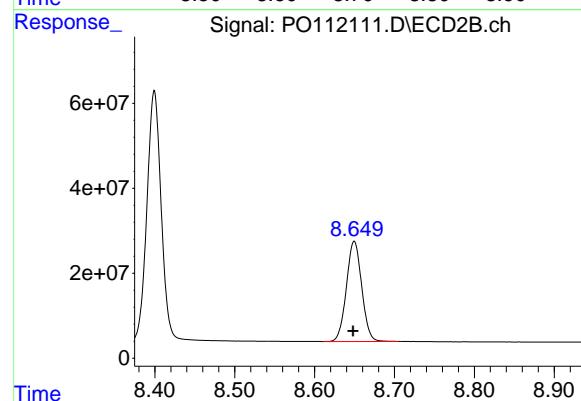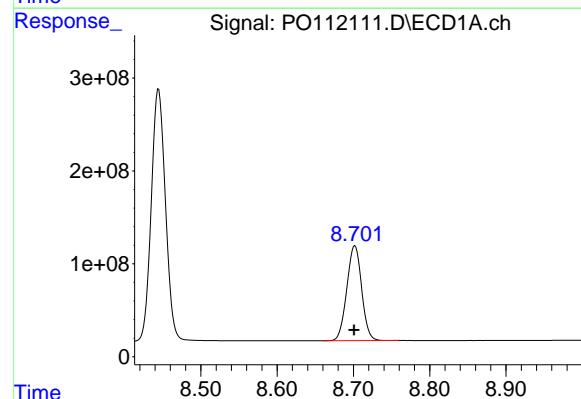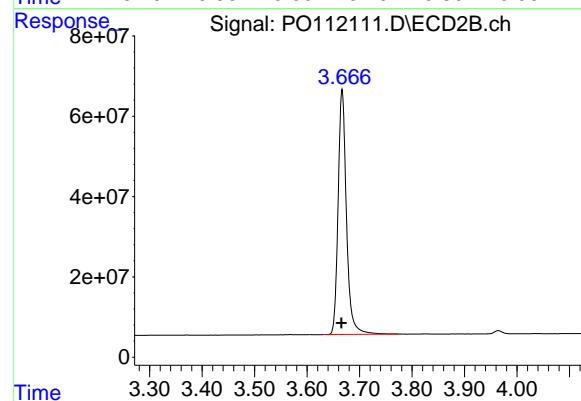

#1 Tetrachloro-m-xylene





R.T.: 3.667 min
Delta R.T.: 0.001 min
Response: 673253587
Conc: 99.56 ng/ml

#2 Decachlorobiphenyl

R.T.: 8.702 min
Delta R.T.: 0.000 min
Response: 1377978961
Conc: 99.63 ng/ml

#2 Decachlorobiphenyl

R.T.: 8.650 min
Delta R.T.: 0.002 min
Response: 313919147
Conc: 96.48 ng/ml

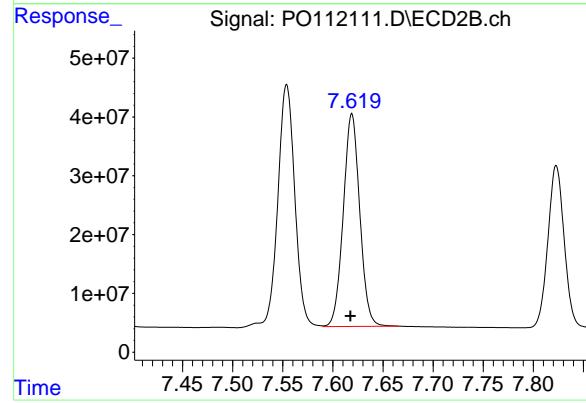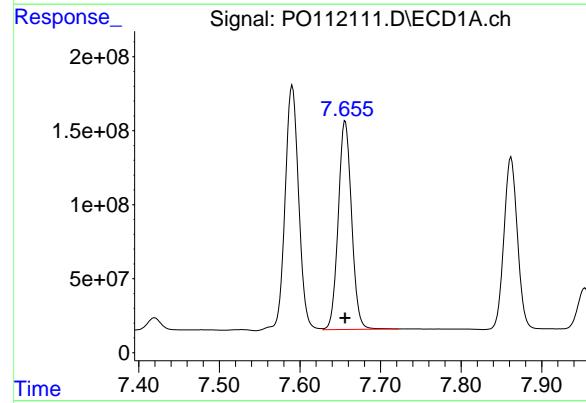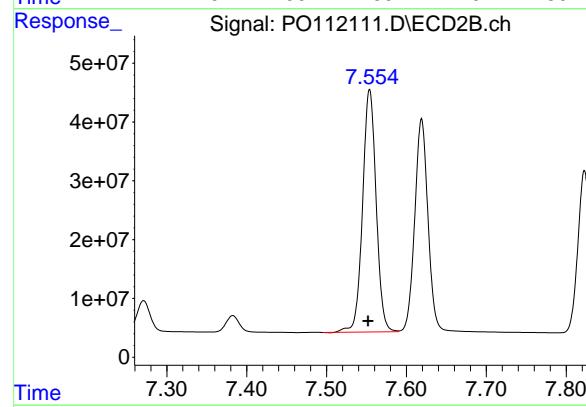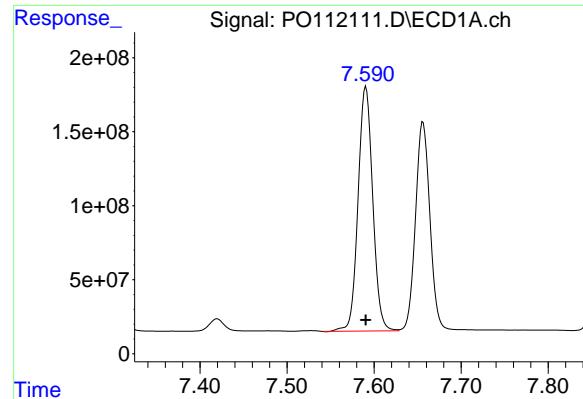




#41 AR-1268-1

R.T.: 7.590 min
Delta R.T.: 0.000 min
Response: 1933697823
Conc: 1000.19 ng/ml

Instrument: ECD_O
ClientSampleId: AR1268ICC1000

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/09/2025
Supervised By :mohammad ahmed 07/10/2025

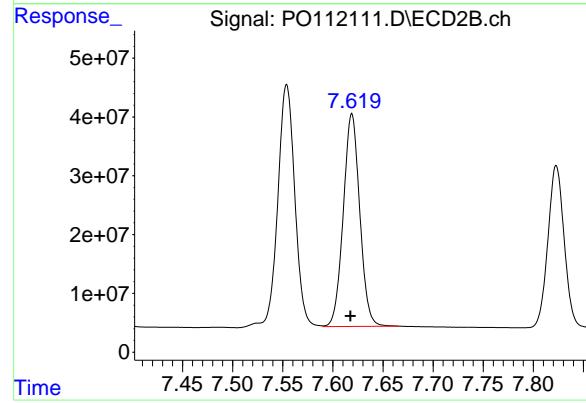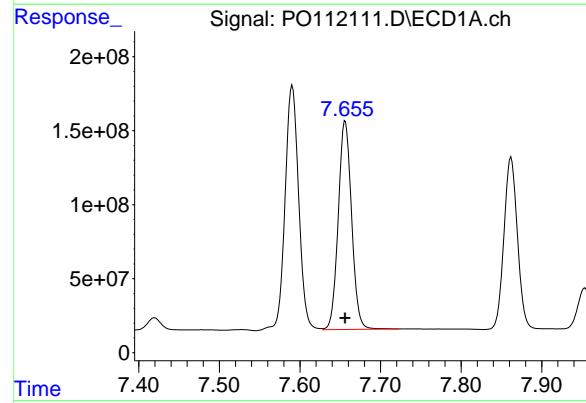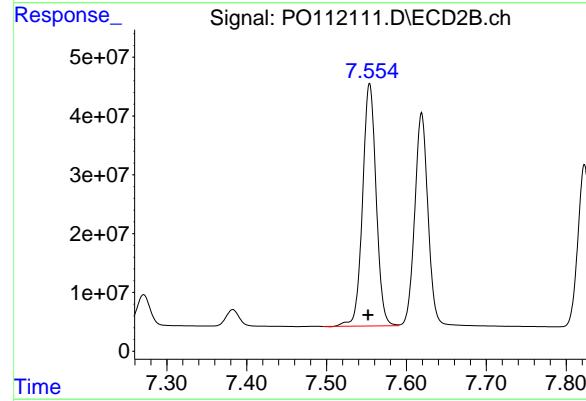

#41 AR-1268-1


R.T.: 7.554 min
Delta R.T.: 0.002 min
Response: 486556055
Conc: 974.10 ng/ml

#42 AR-1268-2

R.T.: 7.656 min
Delta R.T.: 0.000 min
Response: 1621310763
Conc: 997.80 ng/ml

#42 AR-1268-2

R.T.: 7.619 min
Delta R.T.: 0.002 min
Response: 414074889
Conc: 973.99 ng/ml

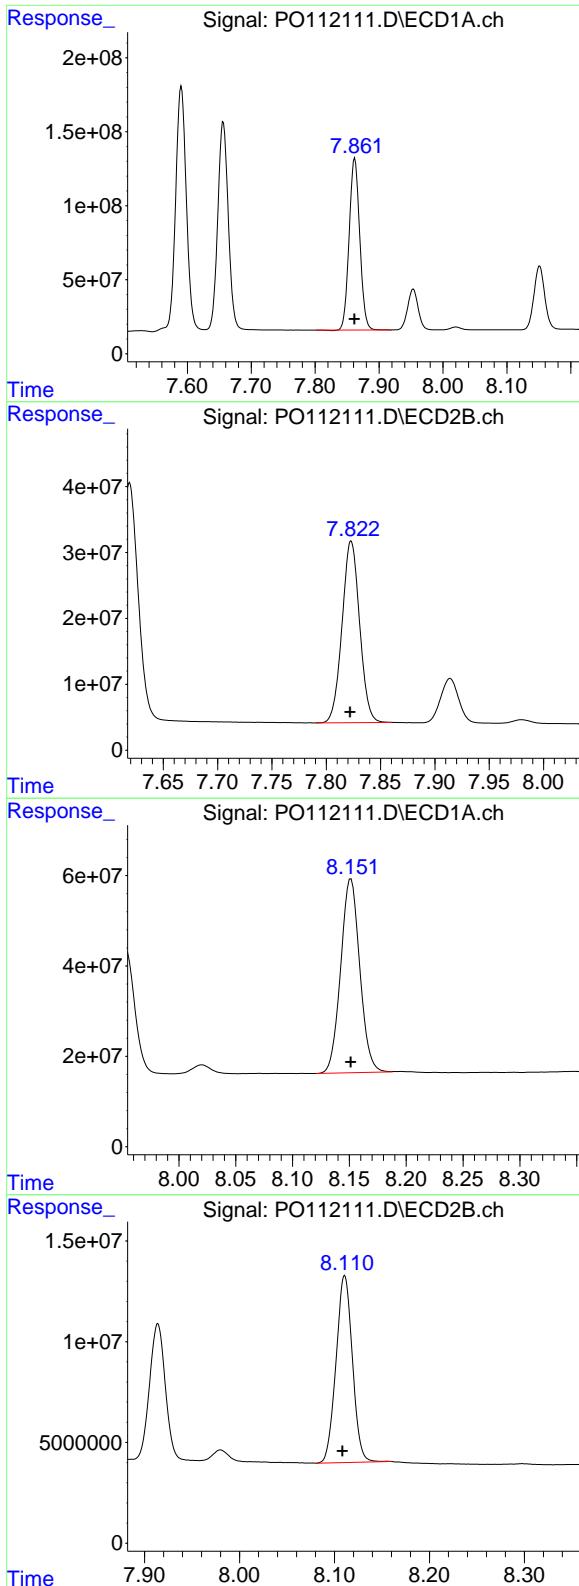

#43 AR-1268-3

R.T.: 7.862 min
Delta R.T.: 0.000 min Instrument :
Response: 1337748865 ECD_O
Conc: 989.54 ng/ml ClientSampleId :
AR12681CC1000

Manual Integrations APPROVED

Reviewed By :Yogesh Patel 07/09/2025
Supervised By :mohammad ahmed 07/10/2025

#43 AR-1268-3

R.T.: 7.823 min
Delta R.T.: 0.001 min
Response: 309607188
Conc: 960.41 ng/ml

#44 AR-1268-4

R.T.: 8.151 min
Delta R.T.: 0.000 min
Response: 501678112
Conc: 975.95 ng/ml m

#44 AR-1268-4

R.T.: 8.111 min
Delta R.T.: 0.002 min
Response: 111375490
Conc: 963.54 ng/ml



#45 AR-1268-5

R.T.: 8.445 min
 Delta R.T.: 0.000 min
 Response: 3474681887
 Conc: 1008.98 ng/ml

Instrument: ECD_O
ClientSampleId: AR1268ICC1000

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/09/2025
 Supervised By :mohammad ahmed 07/10/2025

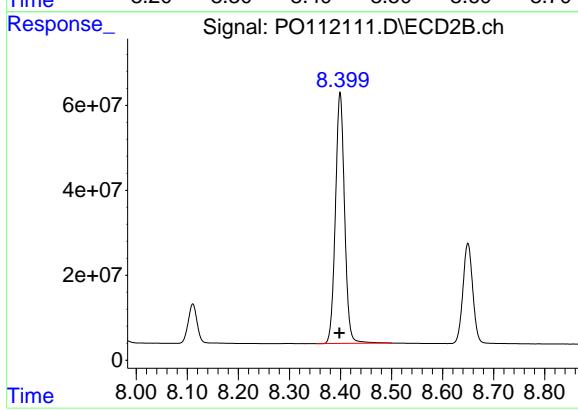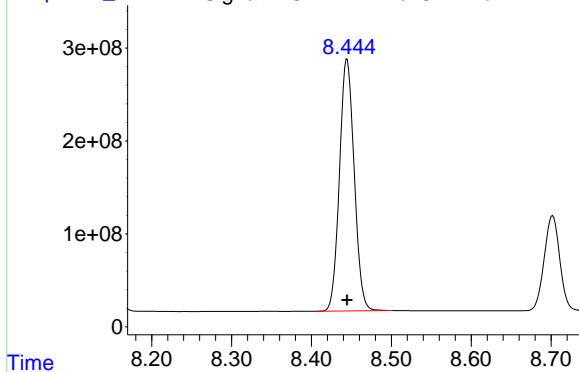

#45 AR-1268-5

R.T.: 8.399 min
 Delta R.T.: 0.002 min
 Response: 736492551
 Conc: 983.57 ng/ml

1
2
3
4
5
6
7
8
9
10
11
12
13
14
15
16
17
18
19
20

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0070825\
 Data File : P0112112.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jul 2025 21:22
 Operator : YP/AJ
 Sample : AR1268ICC750
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1268ICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 09 03:42:05 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 09 03:33:24 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	3.672	3.666	822.0E6	512.2E6	76.722	75.743
2) SA Decachlor...	8.700	8.649	1050.8E6	242.3E6	75.975	74.472

Target Compounds

41) L9 AR-1268-1	7.591	7.553	1471.3E6	372.2E6	761.010	745.185
42) L9 AR-1268-2	7.656	7.618	1239.2E6	317.2E6	762.647	746.065
43) L9 AR-1268-3	7.861	7.823	1019.5E6	238.5E6	754.122	739.688
44) L9 AR-1268-4	8.150	8.110	374.5E6	85695746	728.612	741.374
45) L9 AR-1268-5	8.444	8.399	2621.5E6	562.6E6	761.236	751.350



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0070825\
 Data File : P0112112.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jul 2025 21:22
 Operator : YP/AJ
 Sample : AR1268ICC750
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1268ICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 09 03:42:05 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 09 03:33:24 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

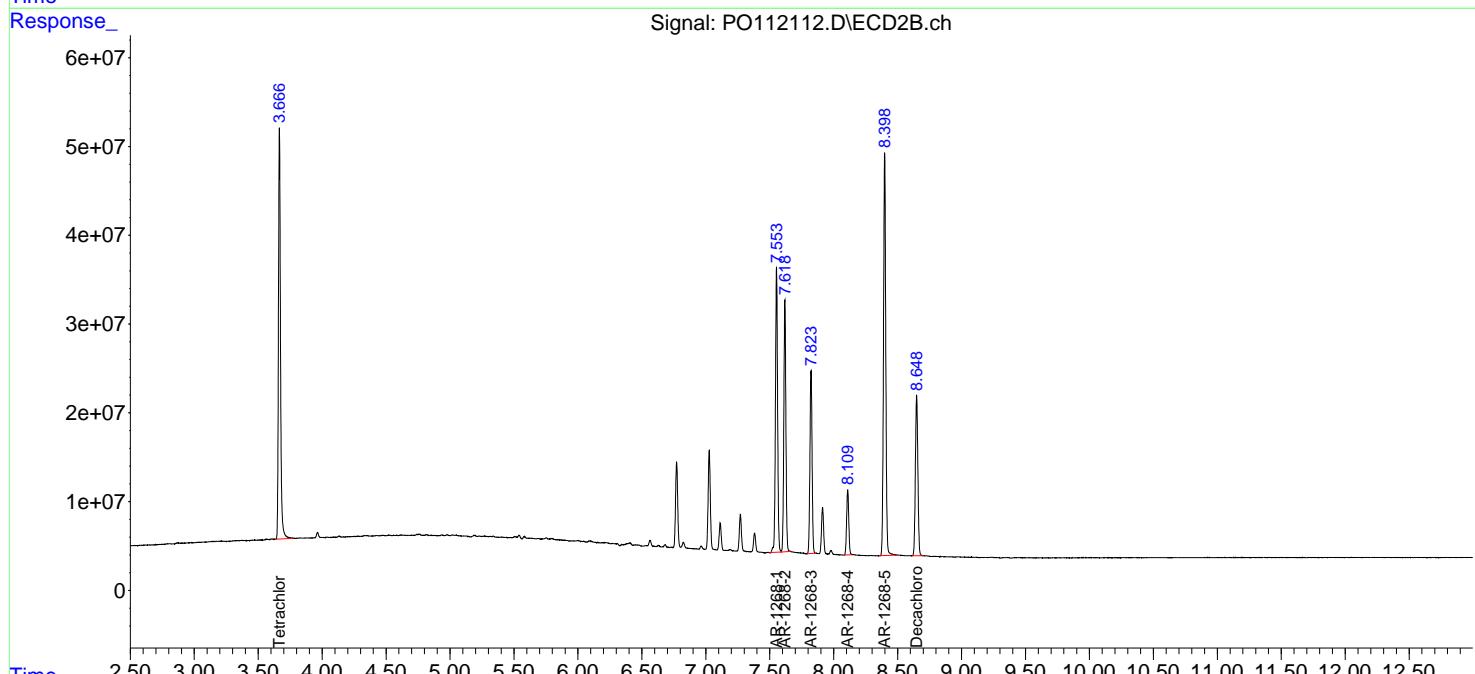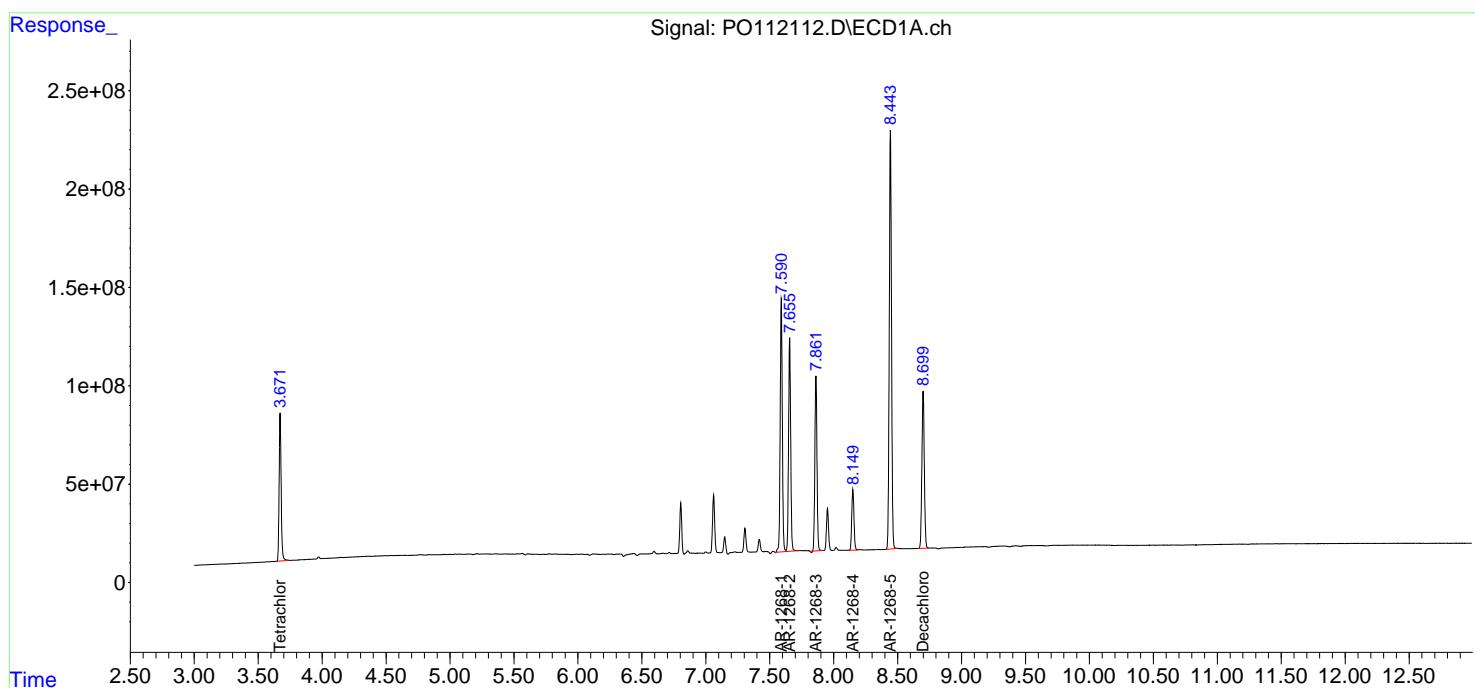

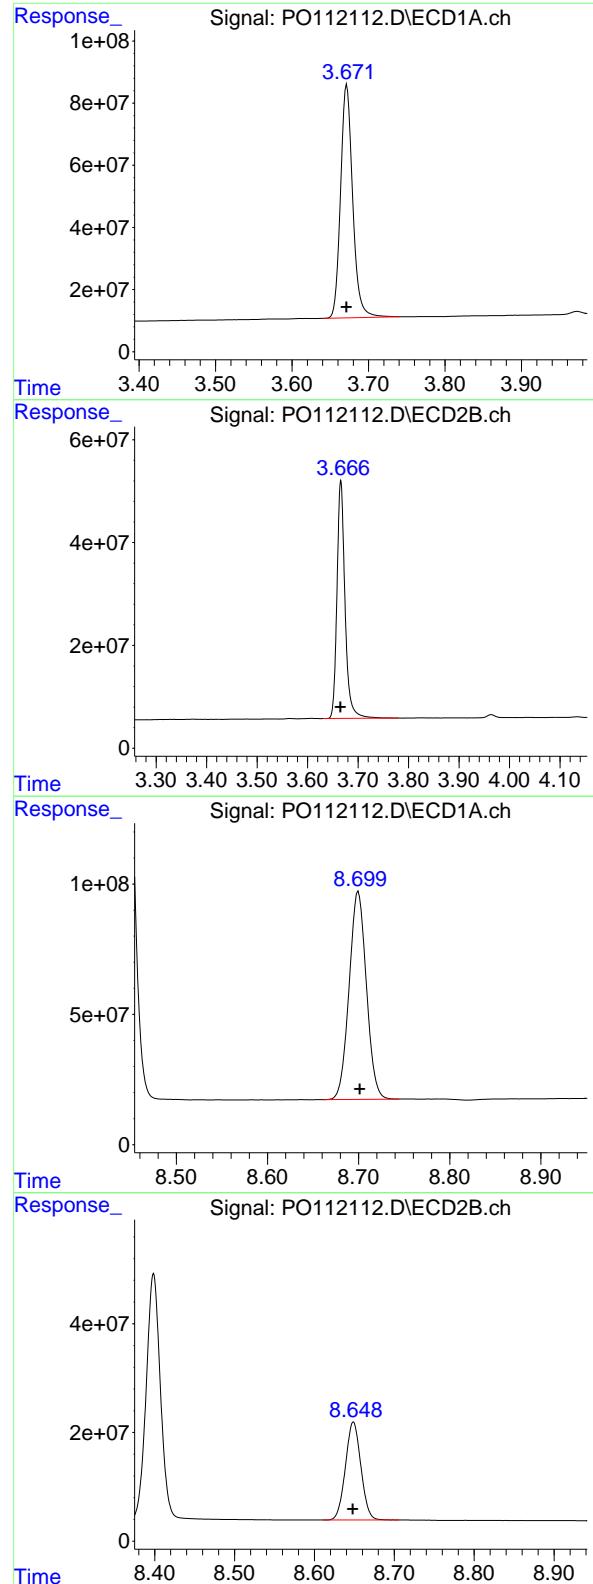

#1 Tetrachloro-m-xylene

R.T.: 3.672 min
Delta R.T.: 0.000 min
Response: 822012649
Conc: 76.72 ng/ml

Instrument: ECD_O
ClientSampleId: AR1268ICC750

#1 Tetrachloro-m-xylene


R.T.: 3.666 min
Delta R.T.: 0.000 min
Response: 512184009
Conc: 75.74 ng/ml

#2 Decachlorobiphenyl

R.T.: 8.700 min
Delta R.T.: -0.001 min
Response: 1050822148
Conc: 75.97 ng/ml

#2 Decachlorobiphenyl

R.T.: 8.649 min
Delta R.T.: 0.000 min
Response: 242314616
Conc: 74.47 ng/ml

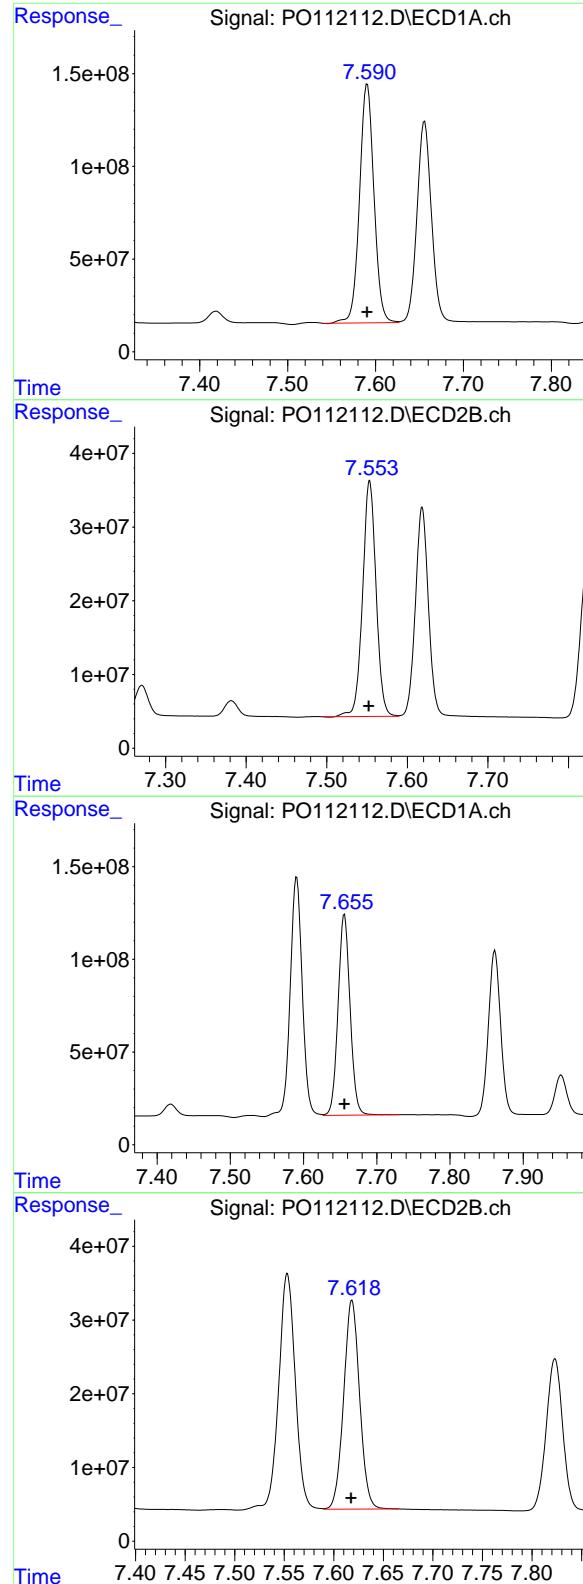

#41 AR-1268-1

R.T.: 7.591 min
 Delta R.T.: 0.000 min
 Response: 1471286032
 Conc: 761.01 ng/ml

Instrument: ECD_O
ClientSampleId: AR1268ICC750

#41 AR-1268-1

R.T.: 7.553 min
 Delta R.T.: 0.001 min
 Response: 372212901
 Conc: 745.18 ng/ml

#42 AR-1268-2





R.T.: 7.656 min
 Delta R.T.: 0.000 min
 Response: 1239212669
 Conc: 762.65 ng/ml

#42 AR-1268-2

R.T.: 7.618 min
 Delta R.T.: 0.000 min
 Response: 317176067
 Conc: 746.06 ng/ml

#43 AR-1268-3

R.T.: 7.861 min
 Delta R.T.: 0.000 min
Instrument:
 Response: 1019493923 ECD_O
 Conc: 754.12 ng/ml
ClientSampleId:
 AR1268ICC750

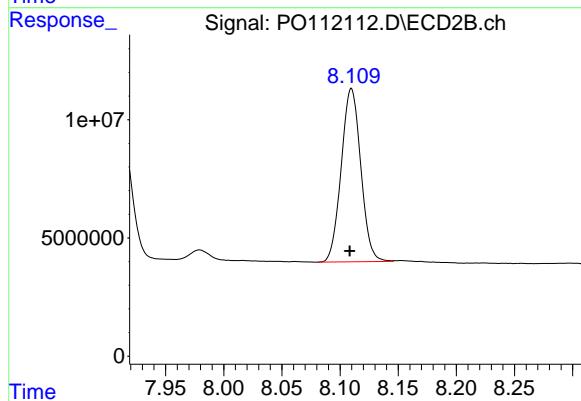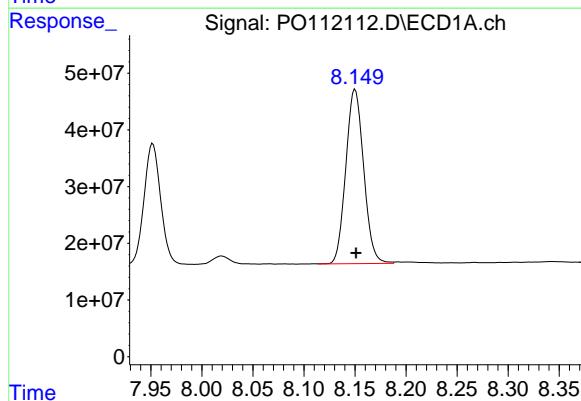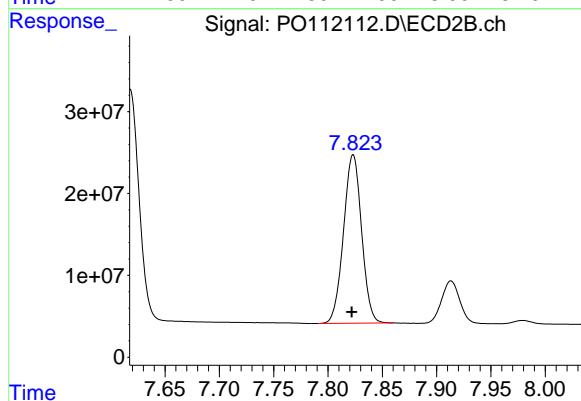

#43 AR-1268-3

R.T.: 7.823 min
 Delta R.T.: 0.001 min
 Response: 238453171
 Conc: 739.69 ng/ml

#44 AR-1268-4

R.T.: 8.150 min
 Delta R.T.: -0.001 min
 Response: 374536426
 Conc: 728.61 ng/ml



#44 AR-1268-4

R.T.: 8.110 min
 Delta R.T.: 0.002 min
 Response: 85695746
 Conc: 741.37 ng/ml

#45 AR-1268-5

R.T.: 8.444 min
Delta R.T.: 0.000 min
Response: 2621514587
Conc: 761.24 ng/ml

Instrument: ECD_O
ClientSampleId: AR1268ICC750

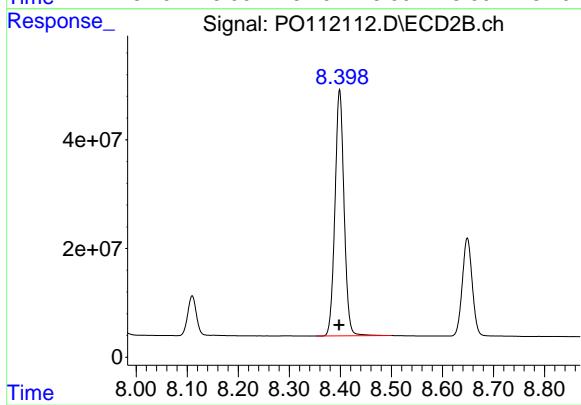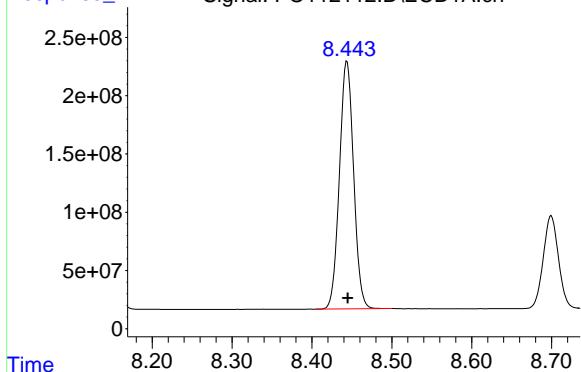

#45 AR-1268-5

R.T.: 8.399 min
Delta R.T.: 0.000 min
Response: 562609528
Conc: 751.35 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0070825\
 Data File : P0112113.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jul 2025 21:39
 Operator : YP/AJ
 Sample : AR1268ICC500
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1268ICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 09 03:42:15 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 09 03:33:24 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	3.671	3.666	535.7E6	338.1E6	50.000	50.000
2) SA Decachlor...	8.701	8.648	691.6E6	162.7E6	50.000	50.000

Target Compounds

41) L9 AR-1268-1	7.590	7.552	966.7E6	249.7E6	500.000	500.000
42) L9 AR-1268-2	7.656	7.617	812.4E6	212.6E6	500.000	500.000
43) L9 AR-1268-3	7.862	7.822	675.9E6	161.2E6	500.000	500.000
44) L9 AR-1268-4	8.151	8.108	257.0E6	57795189	500.000	500.000
45) L9 AR-1268-5	8.445	8.398	1721.9E6	374.4E6	500.000	500.000


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0070825\
 Data File : P0112113.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jul 2025 21:39
 Operator : YP/AJ
 Sample : AR1268ICC500
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1268ICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 09 03:42:15 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 09 03:33:24 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

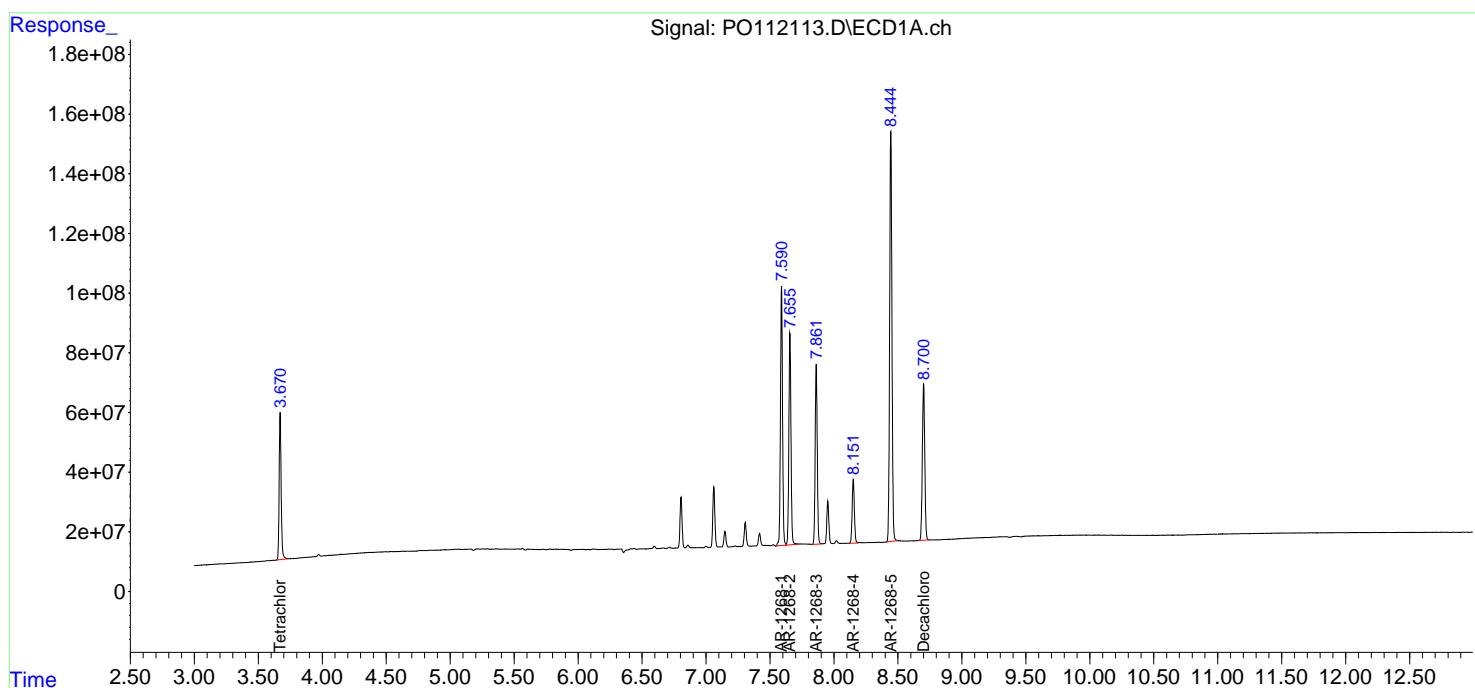

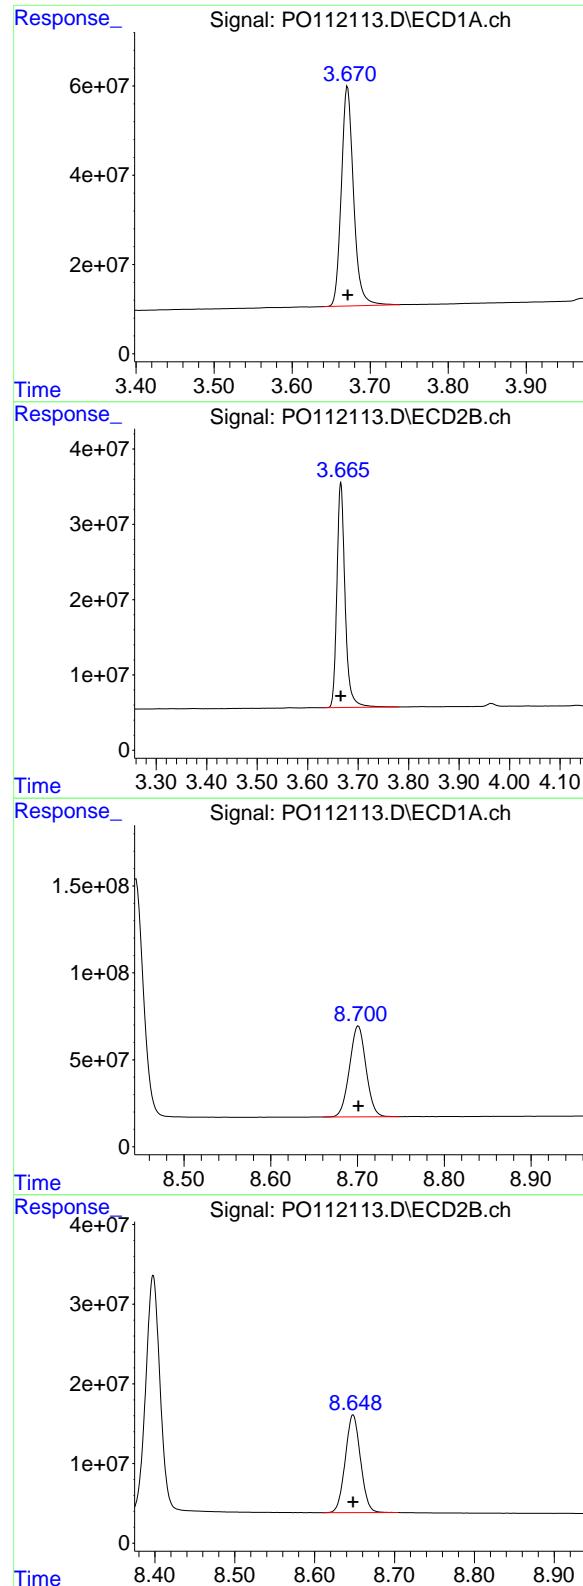

#1 Tetrachloro-m-xylene

R.T.: 3.671 min
 Delta R.T.: 0.000 min
 Response: 535710880
 Conc: 50.00 ng/ml

Instrument: ECD_O
ClientSampleId: AR1268ICC500

#1 Tetrachloro-m-xylene


R.T.: 3.666 min
 Delta R.T.: 0.000 min
 Response: 338108720
 Conc: 50.00 ng/ml

#2 Decachlorobiphenyl

R.T.: 8.701 min
 Delta R.T.: 0.000 min
 Response: 691560412
 Conc: 50.00 ng/ml

#2 Decachlorobiphenyl

R.T.: 8.648 min
 Delta R.T.: 0.000 min
 Response: 162688721
 Conc: 50.00 ng/ml

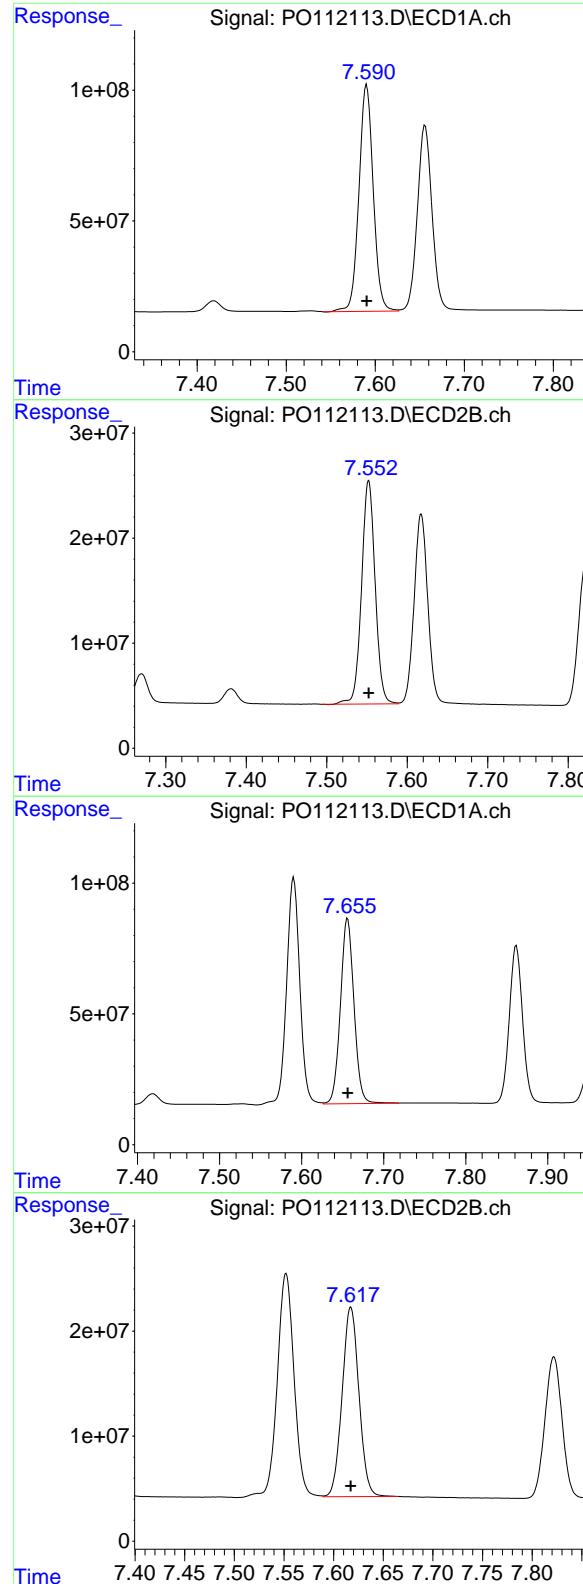

#41 AR-1268-1

R.T.: 7.590 min
 Delta R.T.: 0.000 min
 Response: 966666591
 Conc: 500.00 ng/ml

Instrument: ECD_O
ClientSampleId: AR1268ICC500

#41 AR-1268-1

R.T.: 7.552 min
 Delta R.T.: 0.000 min
 Response: 249745315
 Conc: 500.00 ng/ml

#42 AR-1268-2

R.T.: 7.656 min
 Delta R.T.: 0.000 min
 Response: 812441643
 Conc: 500.00 ng/ml





#42 AR-1268-2

R.T.: 7.617 min
 Delta R.T.: 0.000 min
 Response: 212566069
 Conc: 500.00 ng/ml

#43 AR-1268-3

R.T.: 7.862 min
 Delta R.T.: 0.000 min
 Response: 675947461
 Conc: 500.00 ng/ml

Instrument: ECD_O
ClientSampleId: AR1268ICC500

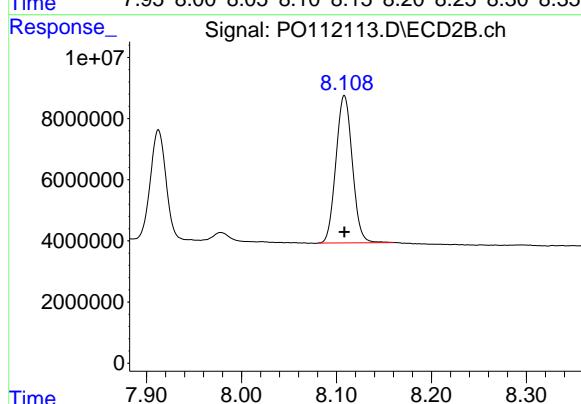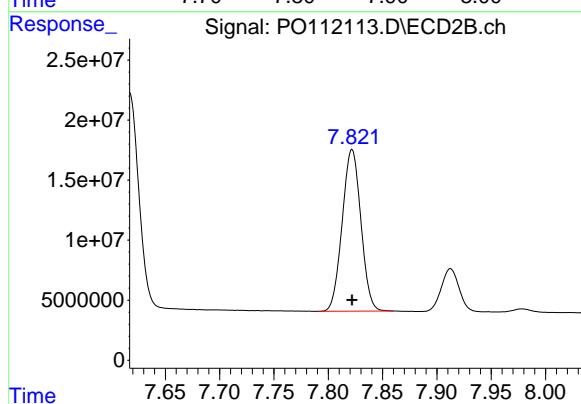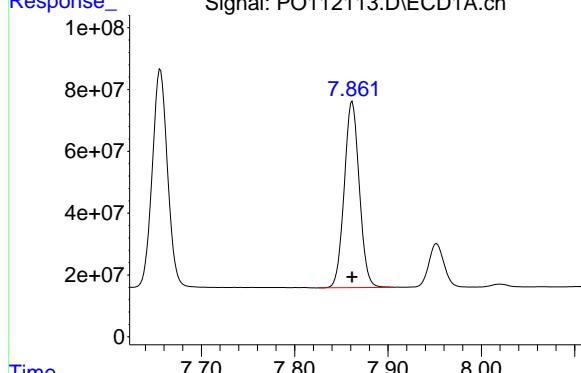

#43 AR-1268-3

R.T.: 7.822 min
 Delta R.T.: 0.000 min
 Response: 161185006
 Conc: 500.00 ng/ml

#44 AR-1268-4

R.T.: 8.151 min
 Delta R.T.: 0.000 min
 Response: 257020392
 Conc: 500.00 ng/ml



#44 AR-1268-4

R.T.: 8.108 min
 Delta R.T.: 0.000 min
 Response: 57795189
 Conc: 500.00 ng/ml

#45 AR-1268-5

R.T.: 8.445 min
Delta R.T.: 0.000 min
Response: 1721880535
Conc: 500.00 ng/ml

Instrument: ECD_O
ClientSampleId: AR1268ICC500

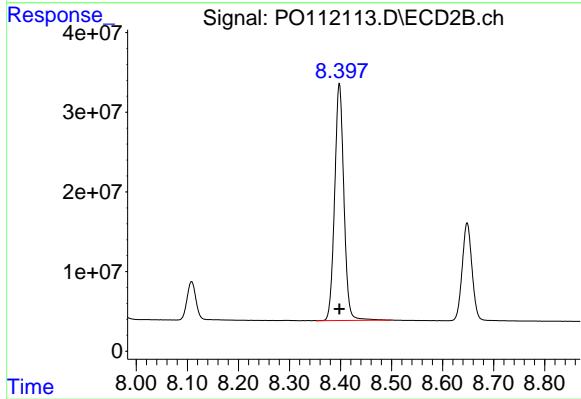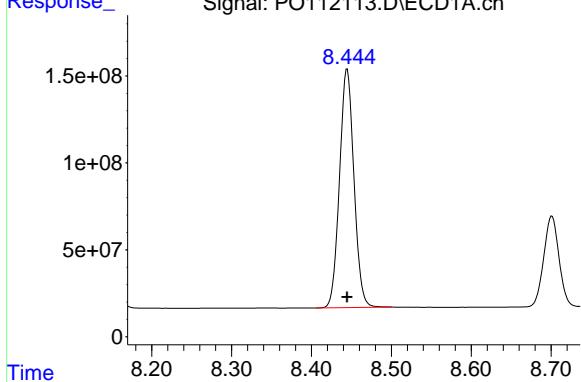

#45 AR-1268-5

R.T.: 8.398 min
Delta R.T.: 0.000 min
Response: 374399232
Conc: 500.00 ng/ml

1
2
3
4
5
6
7
8
9
10
11
12
13
14
15
16
17
18
19
20

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0070825\
 Data File : P0112114.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jul 2025 21:57
 Operator : YP/AJ
 Sample : AR1268ICC250
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1268ICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 09 03:42:25 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 09 03:33:24 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	3.673	3.667	259.9E6	164.3E6	24.261	24.302
2) SA Decachlor...	8.703	8.650	342.2E6	82659475	24.738	25.404

Target Compounds

41) L9 AR-1268-1	7.592	7.553	472.5E6	128.6E6	244.386	257.479
42) L9 AR-1268-2	7.658	7.619	399.3E6	109.7E6	245.741	257.940
43) L9 AR-1268-3	7.864	7.823	334.3E6	83790903	247.301	259.922
44) L9 AR-1268-4	8.153	8.110	127.6E6	29384246	248.229	254.210
45) L9 AR-1268-5	8.446	8.399	837.4E6	188.8E6	243.174	252.154



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0070825\
 Data File : P0112114.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jul 2025 21:57
 Operator : YP/AJ
 Sample : AR1268ICC250
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1268ICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 09 03:42:25 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 09 03:33:24 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

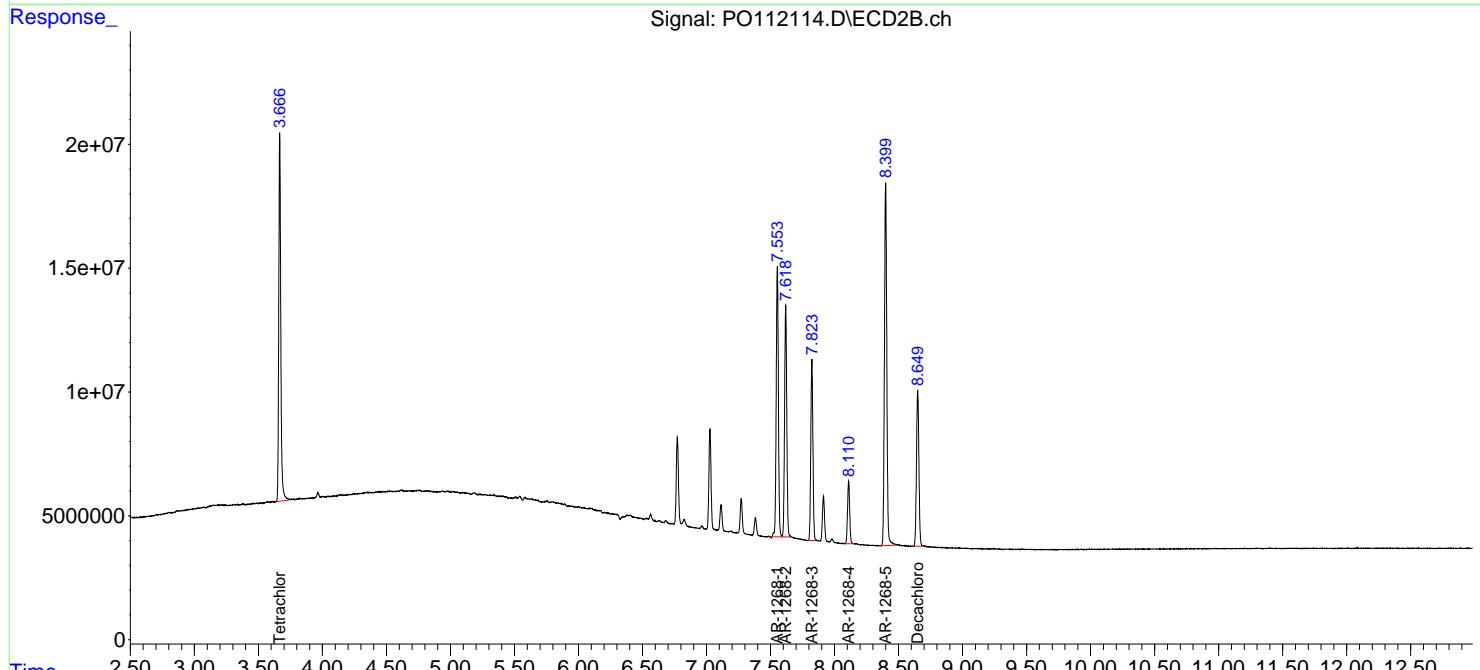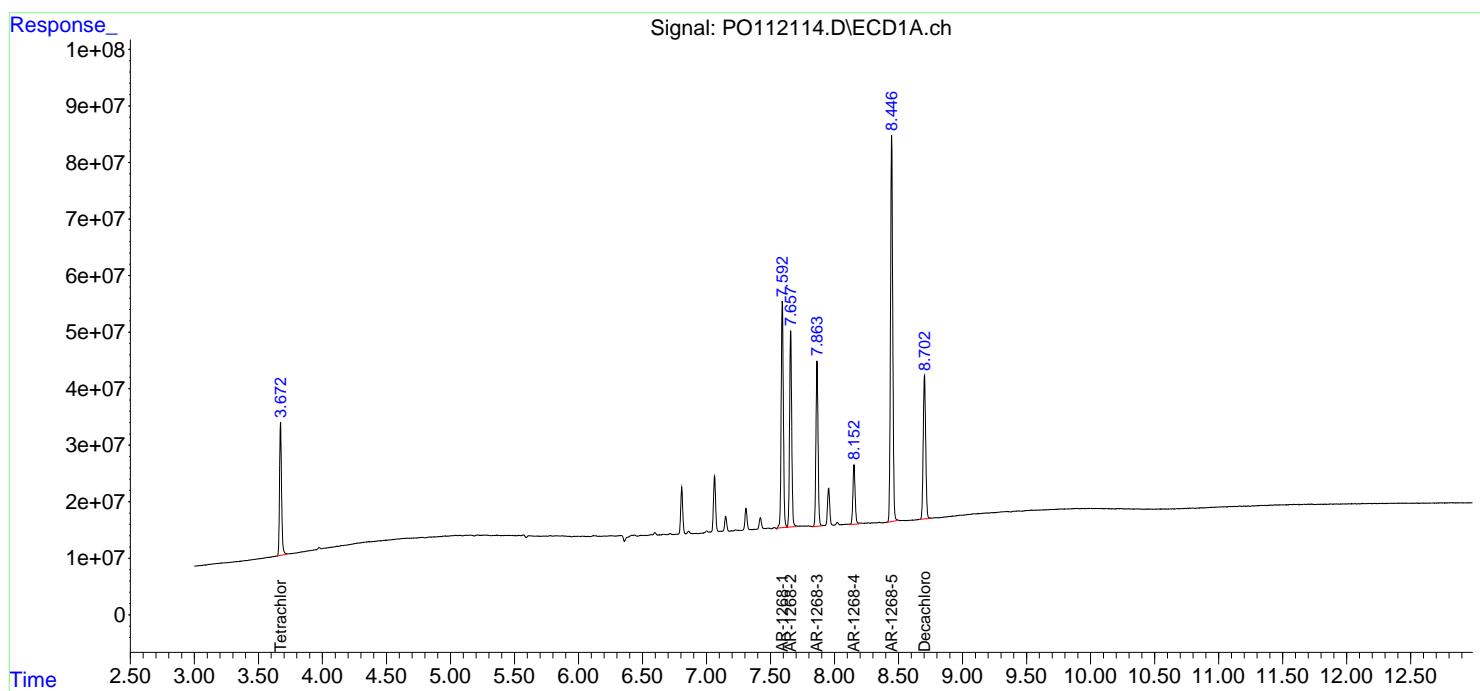

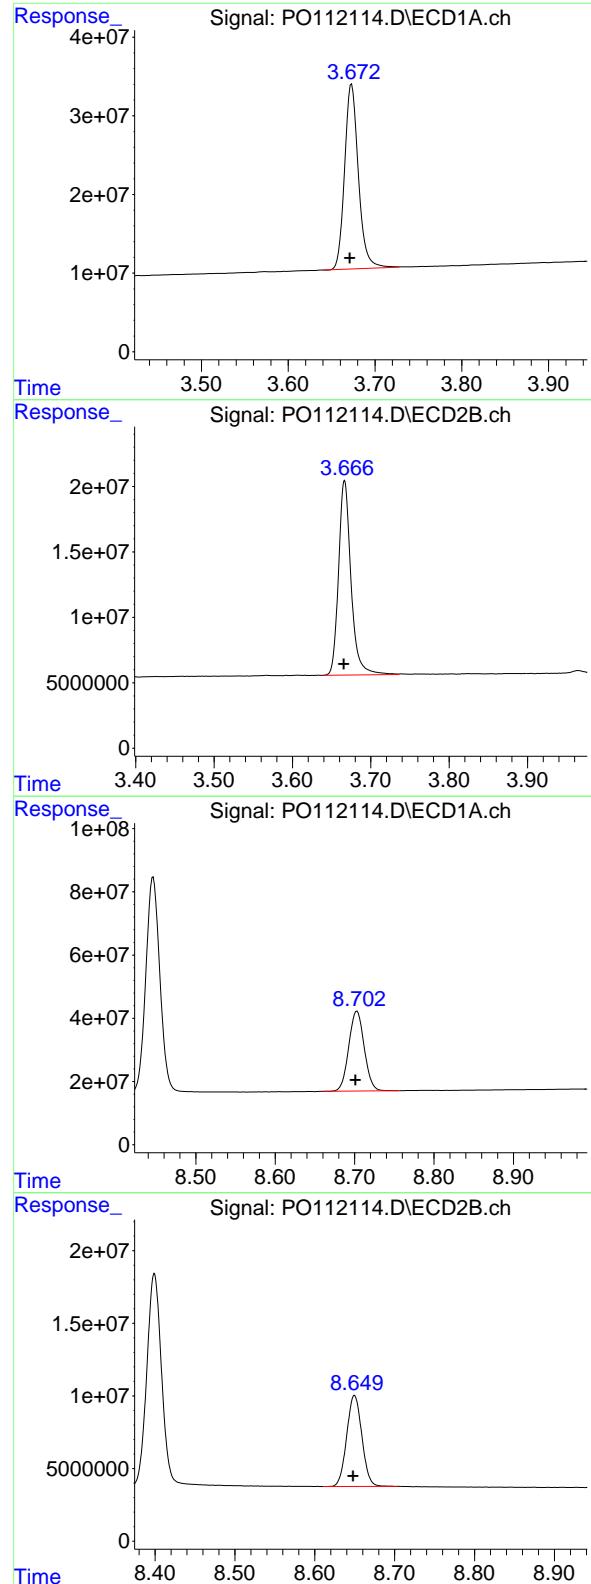

#1 Tetrachloro-m-xylene

R.T.: 3.673 min
Delta R.T.: 0.002 min
Response: 259940477
Conc: 24.26 ng/ml

Instrument:
ECD_O
ClientSampleId :
AR1268ICC250

#1 Tetrachloro-m-xylene


R.T.: 3.667 min
Delta R.T.: 0.000 min
Response: 164334128
Conc: 24.30 ng/ml

#2 Decachlorobiphenyl

R.T.: 8.703 min
Delta R.T.: 0.002 min
Response: 342155893
Conc: 24.74 ng/ml

#2 Decachlorobiphenyl

R.T.: 8.650 min
Delta R.T.: 0.002 min
Response: 82659475
Conc: 25.40 ng/ml

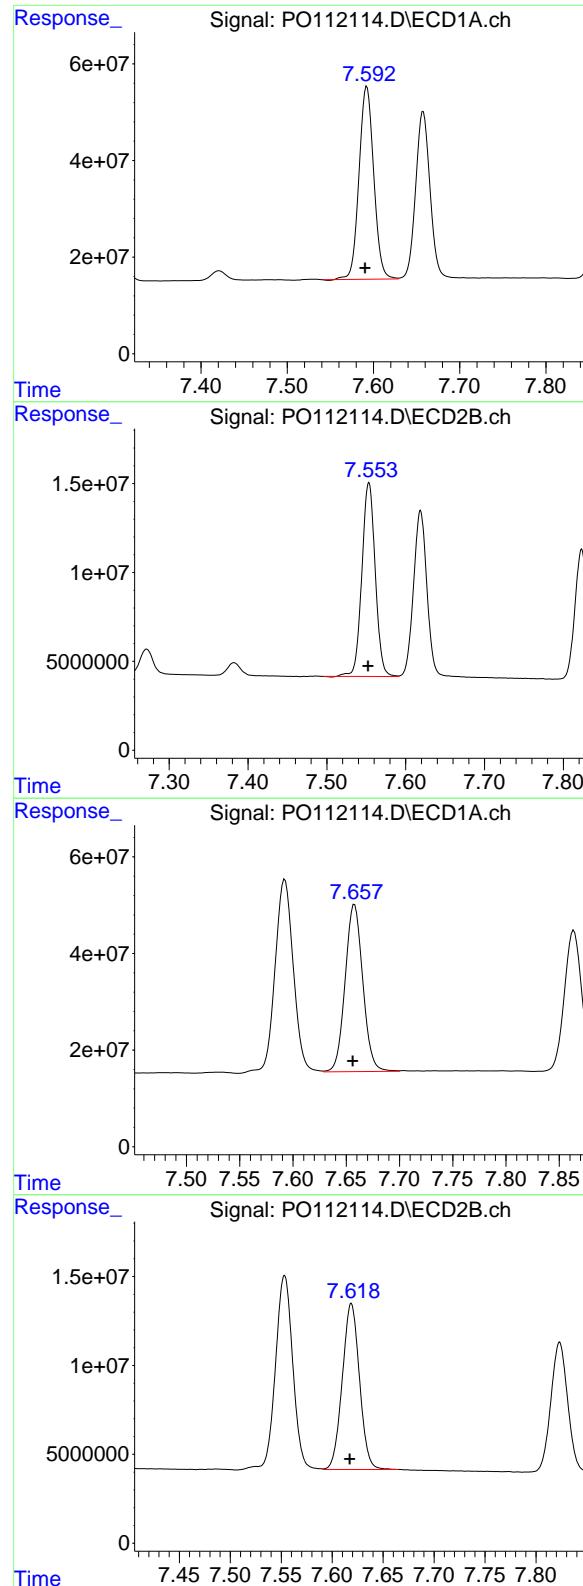

#41 AR-1268-1

R.T.: 7.592 min
 Delta R.T.: 0.002 min
 Response: 472479873
 Conc: 244.39 ng/ml

Instrument: ECD_O
ClientSampleId: AR1268ICC250

#41 AR-1268-1





R.T.: 7.553 min
 Delta R.T.: 0.001 min
 Response: 128608333
 Conc: 257.48 ng/ml

#42 AR-1268-2

R.T.: 7.658 min
 Delta R.T.: 0.002 min
 Response: 399300412
 Conc: 245.74 ng/ml

#42 AR-1268-2

R.T.: 7.619 min
 Delta R.T.: 0.001 min
 Response: 109658423
 Conc: 257.94 ng/ml

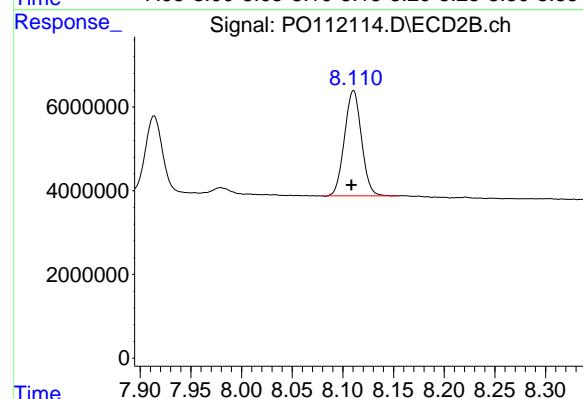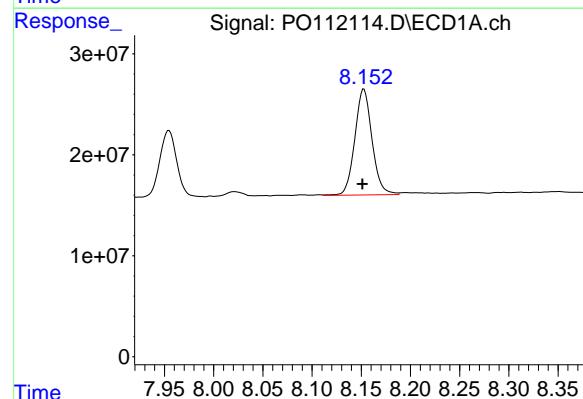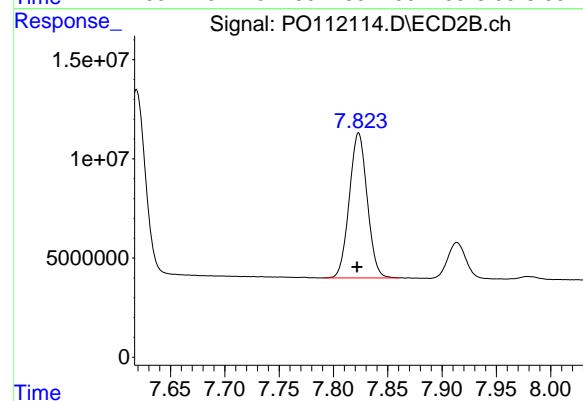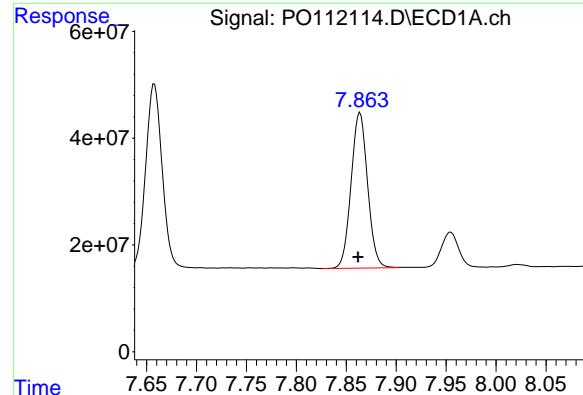

#43 AR-1268-3

R.T.: 7.864 min
Delta R.T.: 0.002 min
Response: 334325326
Conc: 247.30 ng/ml

Instrument: ECD_O
ClientSampleId: AR1268ICC250

#43 AR-1268-3

R.T.: 7.823 min
Delta R.T.: 0.001 min
Response: 83790903
Conc: 259.92 ng/ml

#44 AR-1268-4

R.T.: 8.153 min
Delta R.T.: 0.001 min
Response: 127600083
Conc: 248.23 ng/ml



#44 AR-1268-4

R.T.: 8.110 min
Delta R.T.: 0.002 min
Response: 29384246
Conc: 254.21 ng/ml

#45 AR-1268-5

R.T.: 8.446 min
Delta R.T.: 0.002 min
Response: 837433170
Conc: 243.17 ng/ml

Instrument: ECD_O
ClientSampleId: AR1268ICC250

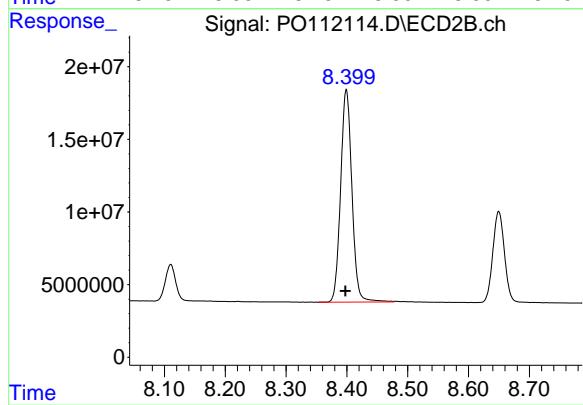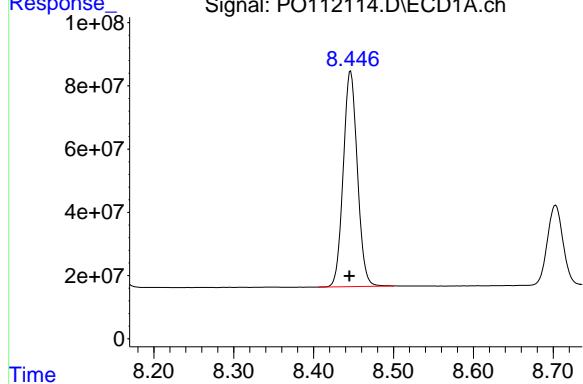

#45 AR-1268-5

R.T.: 8.399 min
Delta R.T.: 0.001 min
Response: 188812276
Conc: 252.15 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0070825\
 Data File : P0112115.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jul 2025 22:16
 Operator : YP/AJ
 Sample : AR1268ICC050
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1268ICC050

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/09/2025
 Supervised By :mohammad ahmed 07/10/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 09 03:42:35 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 09 03:33:24 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	3.674	3.666	38867548	25586379	3.628	3.784
2) SA Decachlor...	8.703	8.649	53087700	13607316	3.838	4.182

Target Compounds

41) L9 AR-1268-1	7.592	7.553	73430329	23025590	37.981m	46.098
42) L9 AR-1268-2	7.658	7.618	64617530	19259498	39.767	45.302
43) L9 AR-1268-3	7.863	7.822	55605590	14843274	41.132m	46.044
44) L9 AR-1268-4	8.154	8.109	18826938	4939808	36.625	42.735
45) L9 AR-1268-5	8.447	8.398	127.8E6	32095228	37.097	42.862

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0070825\
 Data File : P0112115.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jul 2025 22:16
 Operator : YP/AJ
 Sample : AR1268ICC050
 Misc :
 ALS Vial : 30 Sample Multiplier: 1



Instrument :
 ECD_O
ClientSampleId :
 AR1268ICC050


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/09/2025
 Supervised By :mohammad ahmed 07/10/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 09 03:42:35 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 09 03:33:24 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

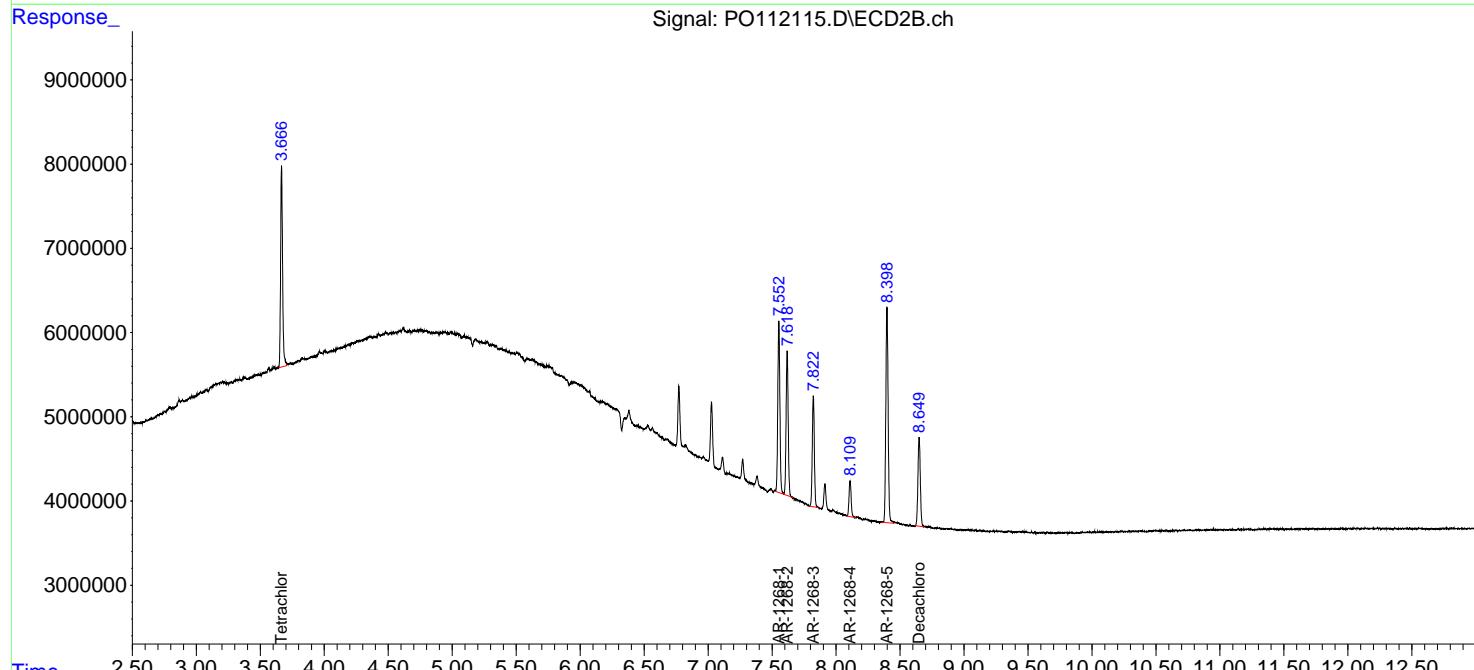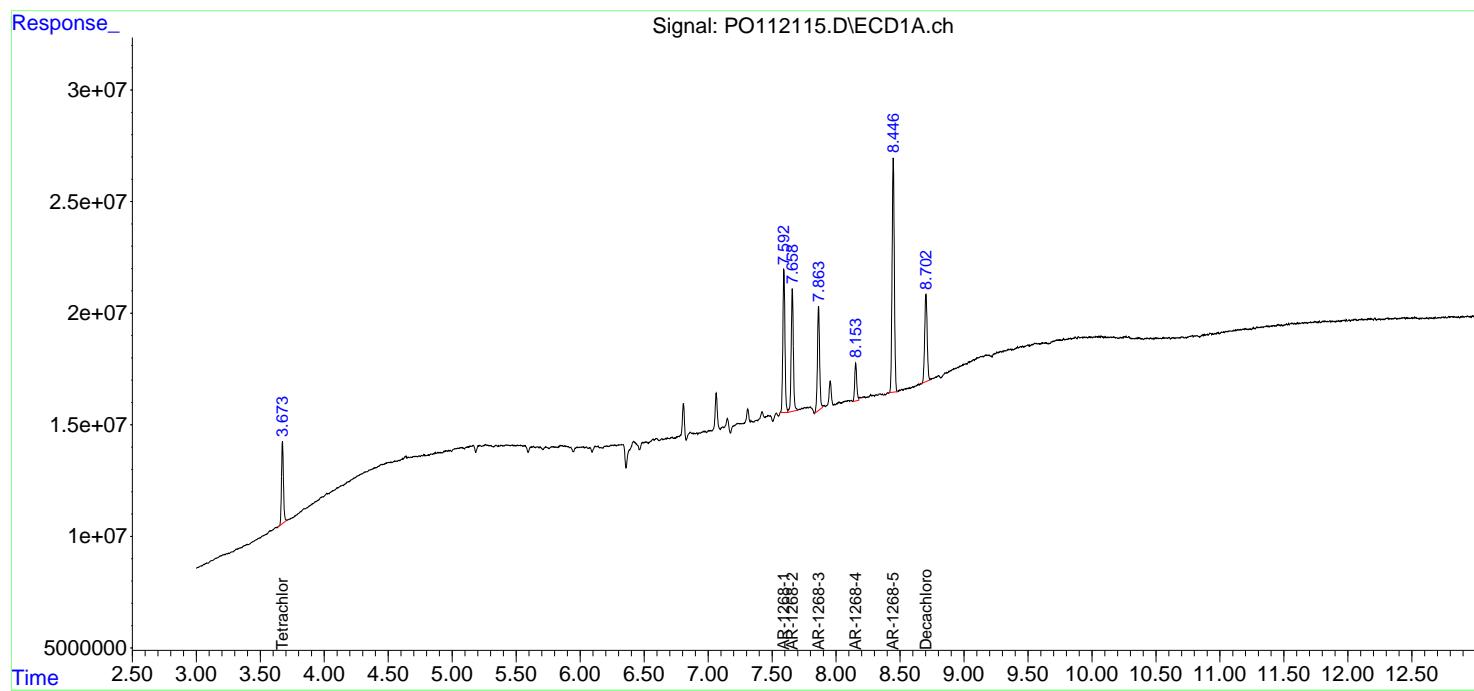

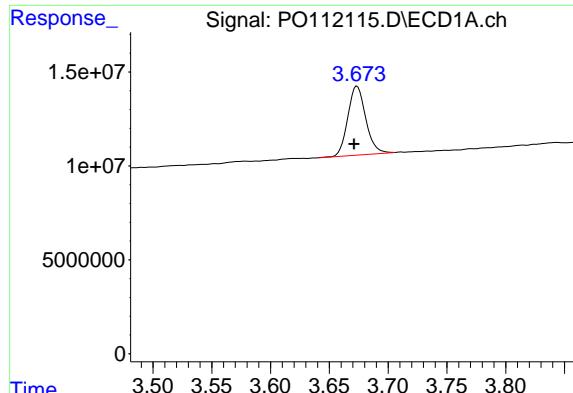


#1 Tetrachloro-m-xylene

R.T.: 3.674 min
Delta R.T.: 0.003 min
Response: 38867548
Conc: 3.63 ng/ml

Instrument: ECD_O
ClientSampleId: AR1268ICC050


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/09/2025
Supervised By :mohammad ahmed 07/10/2025

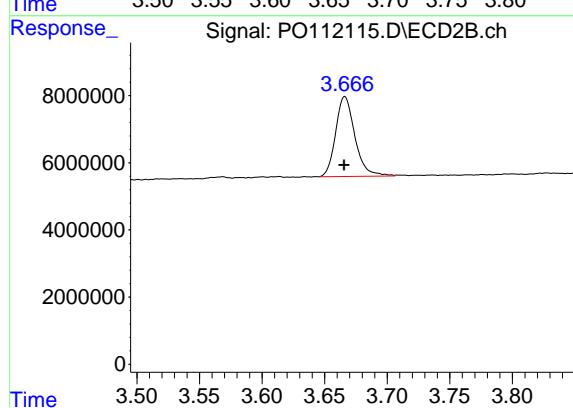


#1 Tetrachloro-m-xylene

R.T.: 3.666 min
Delta R.T.: 0.000 min
Response: 25586379
Conc: 3.78 ng/ml

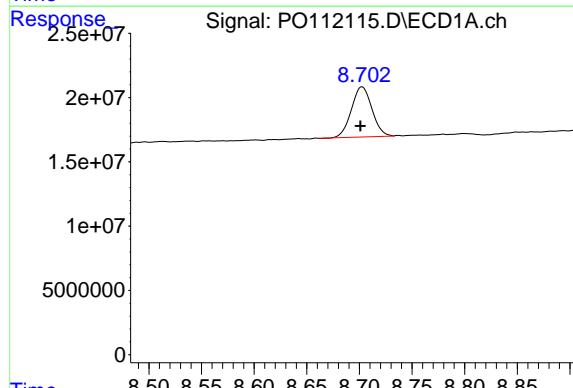


#2 Decachlorobiphenyl

R.T.: 8.703 min
Delta R.T.: 0.002 min
Response: 53087700
Conc: 3.84 ng/ml

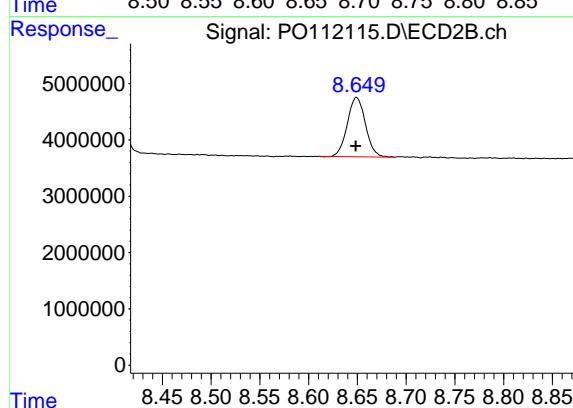

#2 Decachlorobiphenyl

R.T.: 8.649 min
Delta R.T.: 0.001 min
Response: 13607316
Conc: 4.18 ng/ml

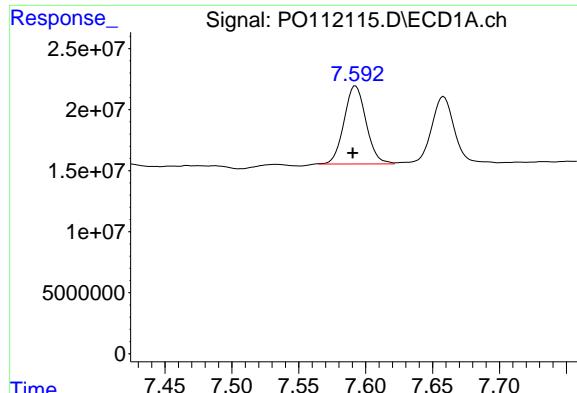


#41 AR-1268-1

R.T.: 7.592 min
Delta R.T.: 0.001 min
Response: 73430329
Conc: 37.98 ng/ml

Instrument: ECD_O
ClientSampleId: AR1268ICC050


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/09/2025
Supervised By :mohammad ahmed 07/10/2025

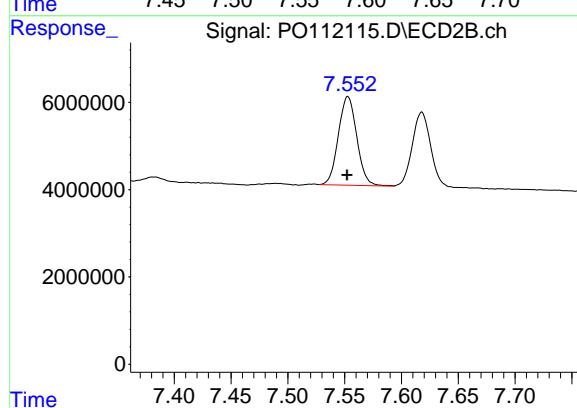


#41 AR-1268-1

R.T.: 7.553 min
Delta R.T.: 0.000 min
Response: 23025590
Conc: 46.10 ng/ml



#42 AR-1268-2

R.T.: 7.658 min
Delta R.T.: 0.002 min
Response: 64617530
Conc: 39.77 ng/ml

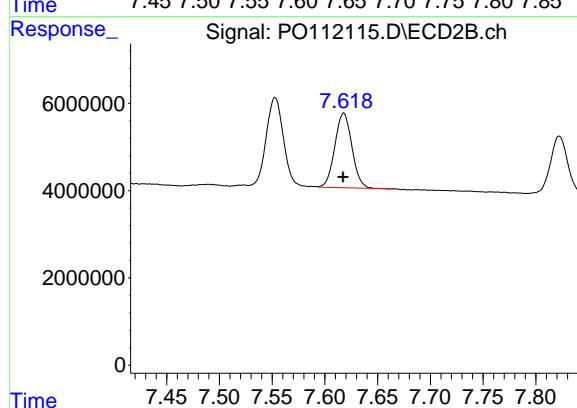

#42 AR-1268-2

R.T.: 7.618 min
Delta R.T.: 0.000 min
Response: 19259498
Conc: 45.30 ng/ml

#43 AR-1268-3

R.T.: 7.863 min
 Delta R.T.: 0.000 min
 Response: 55605590
 Conc: 41.13 ng/ml

Instrument: ECD_O
ClientSampleId: AR1268ICC050

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/09/2025
 Supervised By :mohammad ahmed 07/10/2025

#43 AR-1268-3





R.T.: 7.822 min
 Delta R.T.: 0.000 min
 Response: 14843274
 Conc: 46.04 ng/ml

#44 AR-1268-4

R.T.: 8.154 min
 Delta R.T.: 0.002 min
 Response: 18826938
 Conc: 36.63 ng/ml

#44 AR-1268-4

R.T.: 8.109 min
 Delta R.T.: 0.000 min
 Response: 4939808
 Conc: 42.74 ng/ml

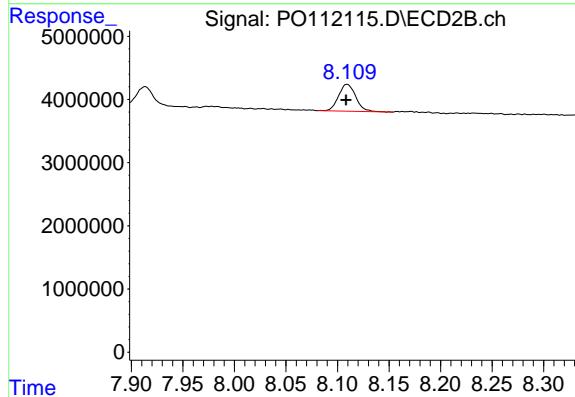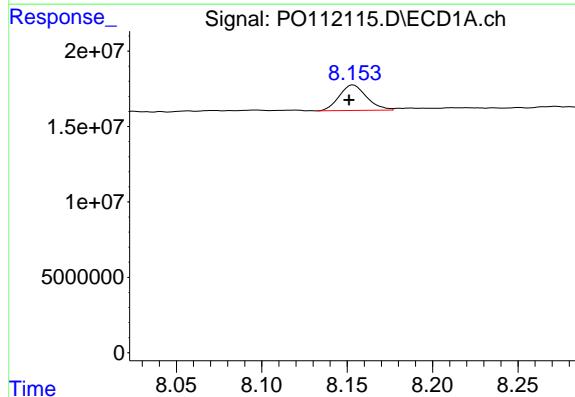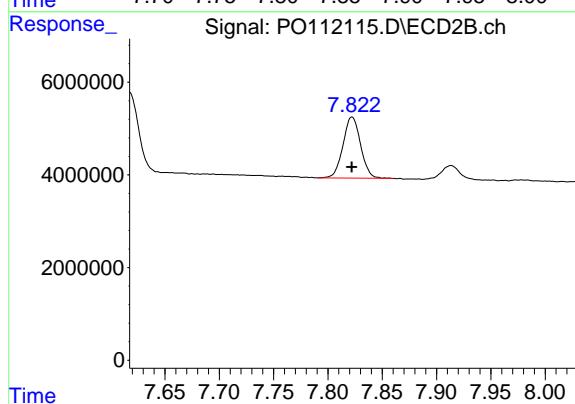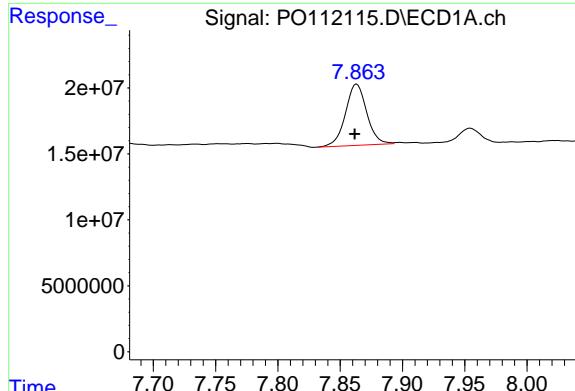



#45 AR-1268-5

R.T.: 8.447 min
 Delta R.T.: 0.002 min
 Response: 127752115
 Conc: 37.10 ng/ml

Instrument: ECD_O
ClientSampleId: AR1268ICC050

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/09/2025
 Supervised By :mohammad ahmed 07/10/2025

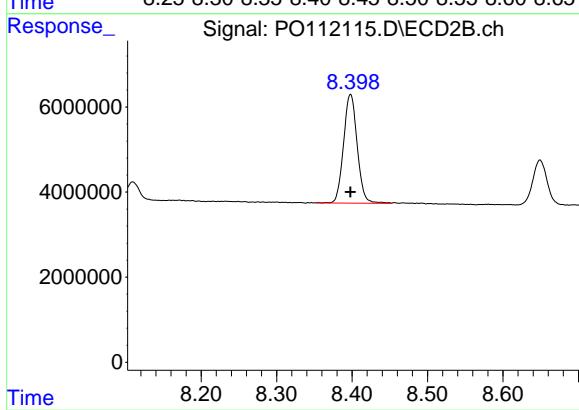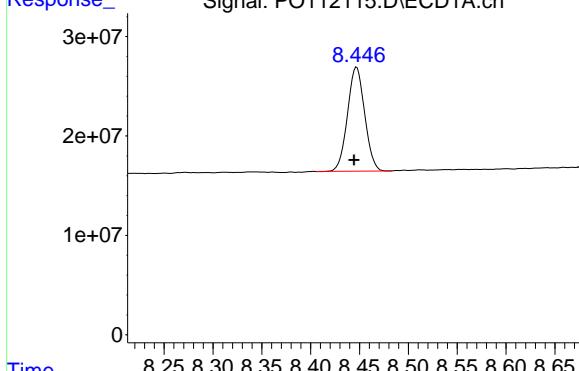

#45 AR-1268-5

R.T.: 8.398 min
 Delta R.T.: 0.000 min
 Response: 32095228
 Conc: 42.86 ng/ml

1
2
3
4
5
6
7
8
9
10
11
12
13
14
15
16
17
18
19
20

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0070825\
 Data File : P0112116.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jul 2025 22:34
 Operator : YP/AJ
 Sample : P0070825ICV500
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
ICVPO070825

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/09/2025
 Supervised By :mohammad ahmed 07/10/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 09 04:04:41 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 09 04:02:23 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	3.672	3.666	521.7E6	329.9E6	52.728	51.784
2) SA Decachlor...	8.702	8.649	362.0E6	87909411	52.944	51.007

Target Compounds

3) L1 AR-1016-1	4.760	4.742	175.3E6	107.8E6	515.284	483.610m
4) L1 AR-1016-2	4.779	4.761	259.8E6	163.6E6	522.388	497.237m
5) L1 AR-1016-3	4.836	4.936	165.0E6	85046592	509.600	500.666
6) L1 AR-1016-4	4.956	4.979	132.8E6	68299058	517.300	497.707
7) L1 AR-1016-5	5.213	5.190	137.8E6	89116759	503.683	516.768
31) L7 AR-1260-1	6.250	6.220	257.1E6	138.6E6	512.929	493.882
32) L7 AR-1260-2	6.440	6.408	380.3E6	165.9E6	515.168	487.864
33) L7 AR-1260-3	6.806	6.559	331.7E6	141.4E6	506.110	512.911m
34) L7 AR-1260-4	7.065	7.029	235.9E6	98320139	541.983	490.020m
35) L7 AR-1260-5	7.308	7.271	694.1E6	218.4E6	549.787	487.907

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0070825\
 Data File : P0112116.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jul 2025 22:34
 Operator : YP/AJ
 Sample : P0070825ICV500
 Misc :
 ALS Vial : 31 Sample Multiplier: 1



Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 09 04:04:41 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 09 04:02:23 2025
 Response via : Initial Calibration
 Integrator: ChemStation


Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Instrument :
 ECD_O
 ClientSampleId :
 ICP0070825

Manual Integrations APPROVED

Reviewed By :Yogesh Patel 07/09/2025
 Supervised By :mohammad ahmed 07/10/2025

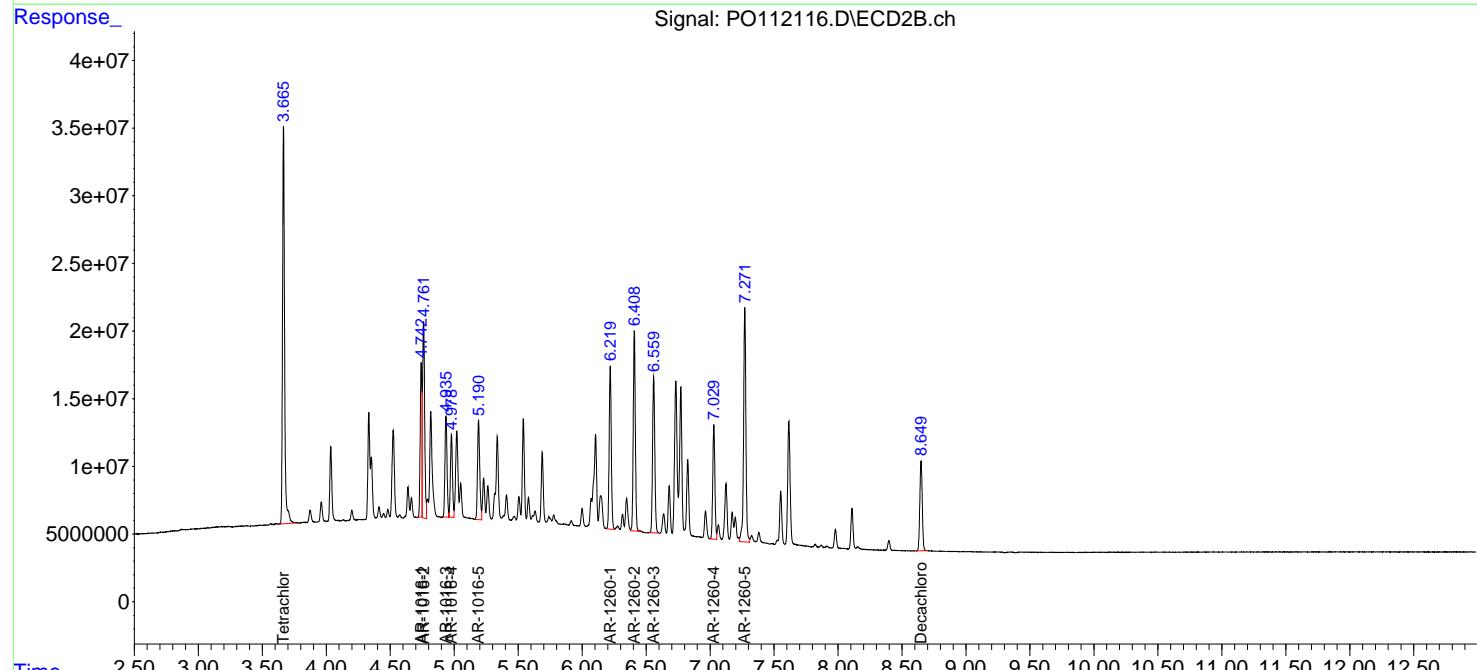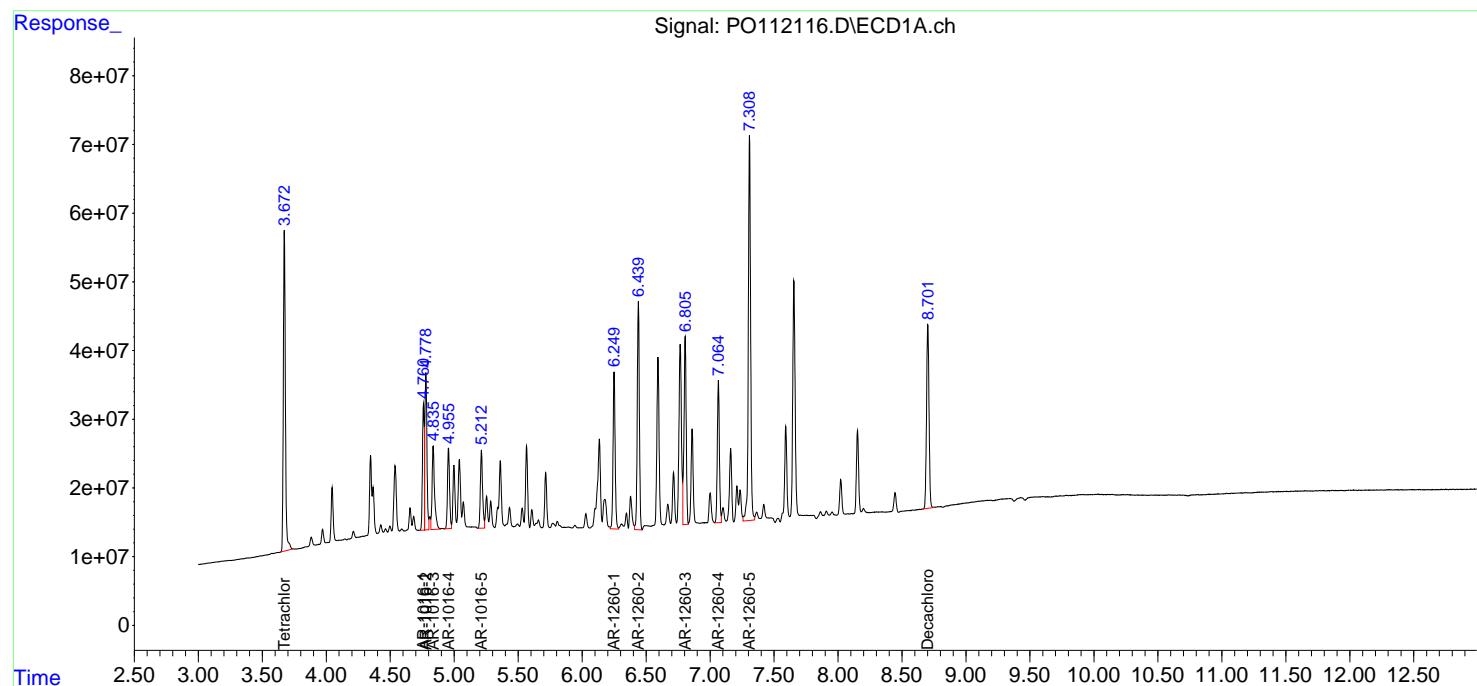

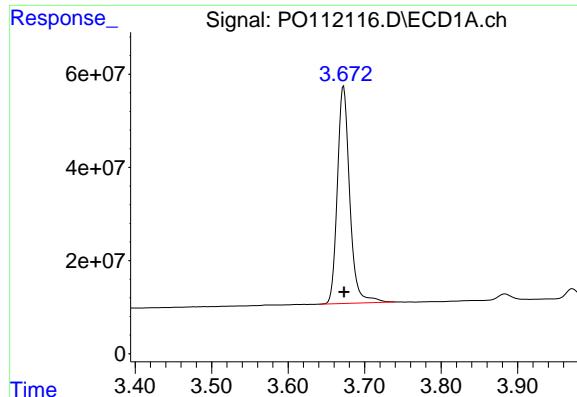


#1 Tetrachloro-m-xylene

R.T.: 3.672 min
Delta R.T.: 0.000 min
Response: 521724349
Conc: 52.73 ng/ml

Instrument: ECD_O
ClientSampleId: ICVPO070825


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/09/2025
Supervised By :mohammad ahmed 07/10/2025

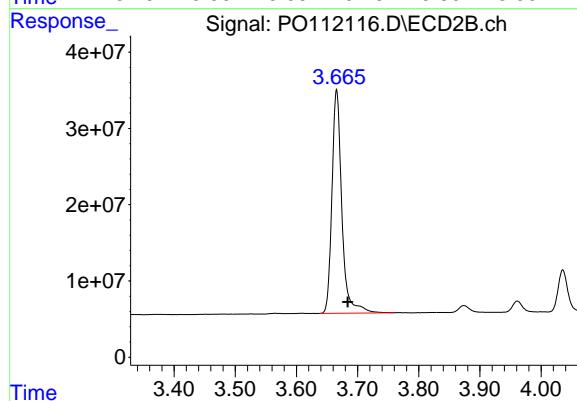


#1 Tetrachloro-m-xylene

R.T.: 3.666 min
Delta R.T.: -0.018 min
Response: 329918340
Conc: 51.78 ng/ml

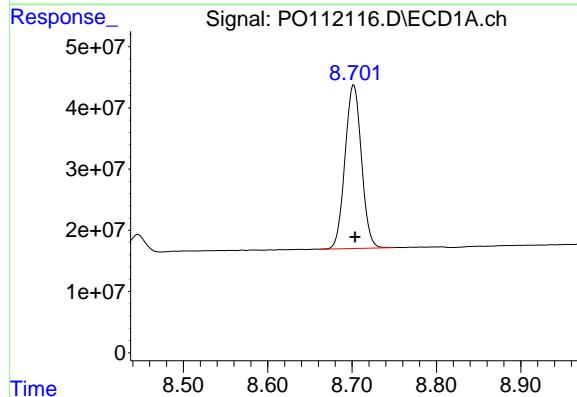


#2 Decachlorobiphenyl

R.T.: 8.702 min
Delta R.T.: -0.001 min
Response: 361977757
Conc: 52.94 ng/ml

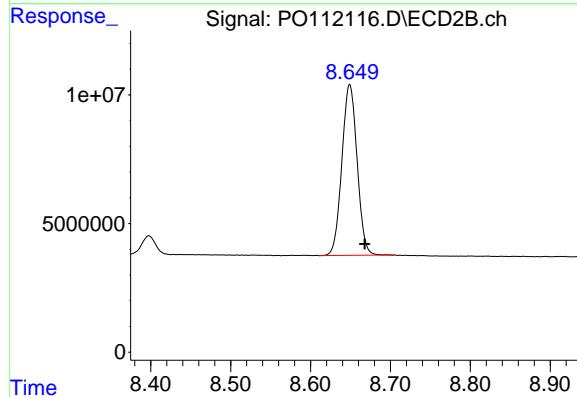

#2 Decachlorobiphenyl

R.T.: 8.649 min
Delta R.T.: -0.019 min
Response: 87909411
Conc: 51.01 ng/ml

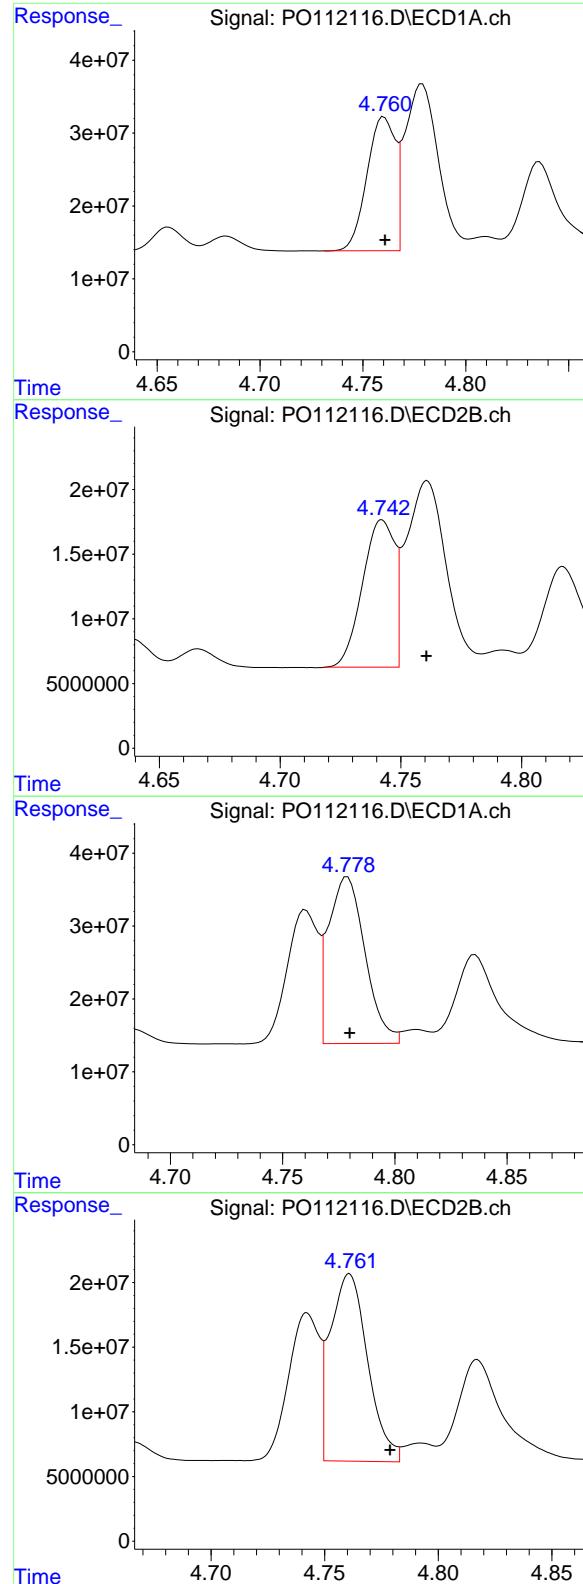

#3 AR-1016-1

R.T.: 4.760 min
 Delta R.T.: 0.000 min
 Response: 175259674
 Conc: 515.28 ng/ml

Instrument: ECD_O
 ClientSampleId: ICVPO070825

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/09/2025
 Supervised By :mohammad ahmed 07/10/2025

#3 AR-1016-1

R.T.: 4.742 min
 Delta R.T.: -0.019 min
 Response: 107764906
 Conc: 483.61 ng/ml

#4 AR-1016-2

R.T.: 4.779 min
 Delta R.T.: -0.001 min
 Response: 259779428
 Conc: 522.39 ng/ml

#4 AR-1016-2

R.T.: 4.761 min
 Delta R.T.: -0.018 min
 Response: 163639494
 Conc: 497.24 ng/ml





#5 AR-1016-3

R.T.: 4.836 min
 Delta R.T.: 0.000 min
 Response: 164964568
 Conc: 509.60 ng/ml

Instrument: ECD_O
ClientSampleId: ICVPO070825

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/09/2025
 Supervised By :mohammad ahmed 07/10/2025

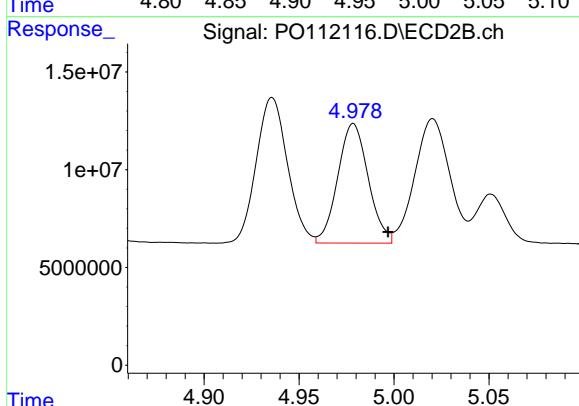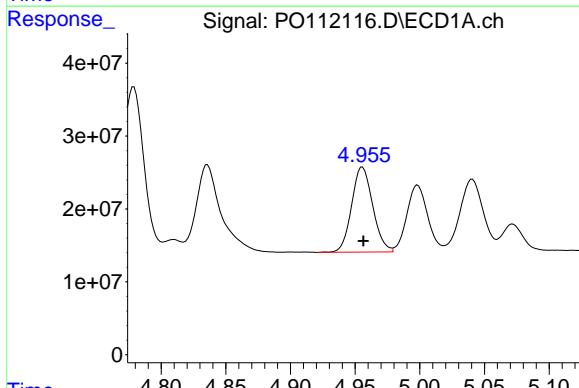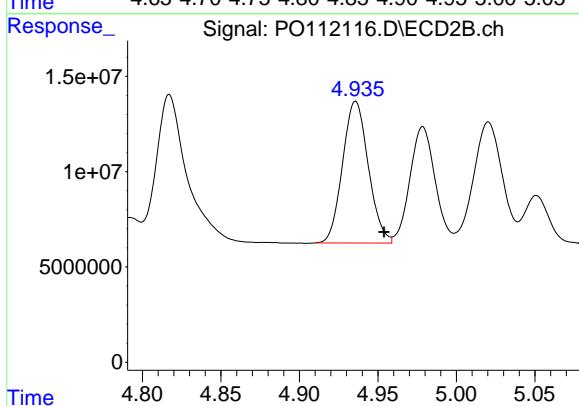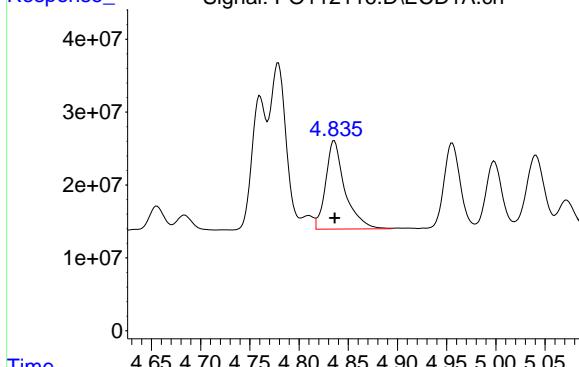

#5 AR-1016-3



R.T.: 4.936 min
 Delta R.T.: -0.018 min
 Response: 85046592
 Conc: 500.67 ng/ml

#6 AR-1016-4

R.T.: 4.956 min
 Delta R.T.: 0.000 min
 Response: 132842340
 Conc: 517.30 ng/ml

#6 AR-1016-4

R.T.: 4.979 min
 Delta R.T.: -0.018 min
 Response: 68299058
 Conc: 497.71 ng/ml

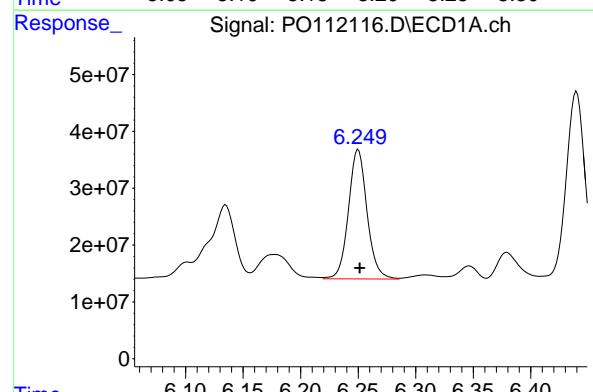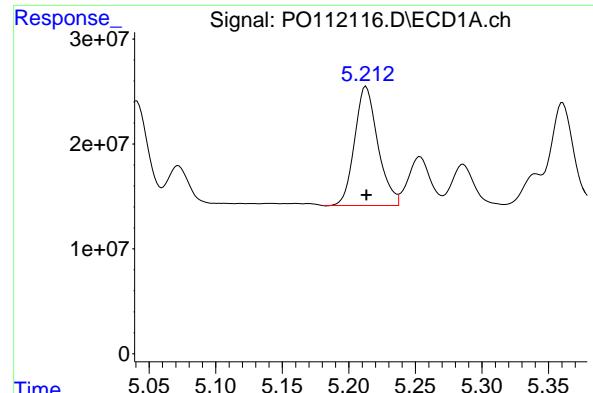

#7 AR-1016-5

R.T.: 5.213 min
Delta R.T.: 0.000 min
Response: 137838808
Conc: 503.68 ng/ml

Instrument: ECD_O
ClientSampleId: ICVPO070825

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/09/2025
Supervised By :mohammad ahmed 07/10/2025

#7 AR-1016-5

R.T.: 5.190 min
Delta R.T.: -0.018 min
Response: 89116759
Conc: 516.77 ng/ml

#31 AR-1260-1

R.T.: 6.250 min
Delta R.T.: -0.001 min
Response: 257100150
Conc: 512.93 ng/ml

#31 AR-1260-1

R.T.: 6.220 min
Delta R.T.: -0.019 min
Response: 138564703
Conc: 493.88 ng/ml

#32 AR-1260-2

R.T.: 6.440 min
 Delta R.T.: -0.001 min
 Response: 380263019
 Conc: 515.17 ng/ml

Instrument: ECD_O
ClientSampleId: ICVPO070825

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/09/2025
 Supervised By :mohammad ahmed 07/10/2025

#32 AR-1260-2


R.T.: 6.408 min
 Delta R.T.: -0.018 min
 Response: 165872316
 Conc: 487.86 ng/ml


#33 AR-1260-3

R.T.: 6.806 min
 Delta R.T.: -0.001 min
 Response: 331746197
 Conc: 506.11 ng/ml

#33 AR-1260-3

R.T.: 6.559 min
 Delta R.T.: -0.019 min
 Response: 141351043
 Conc: 512.91 ng/ml

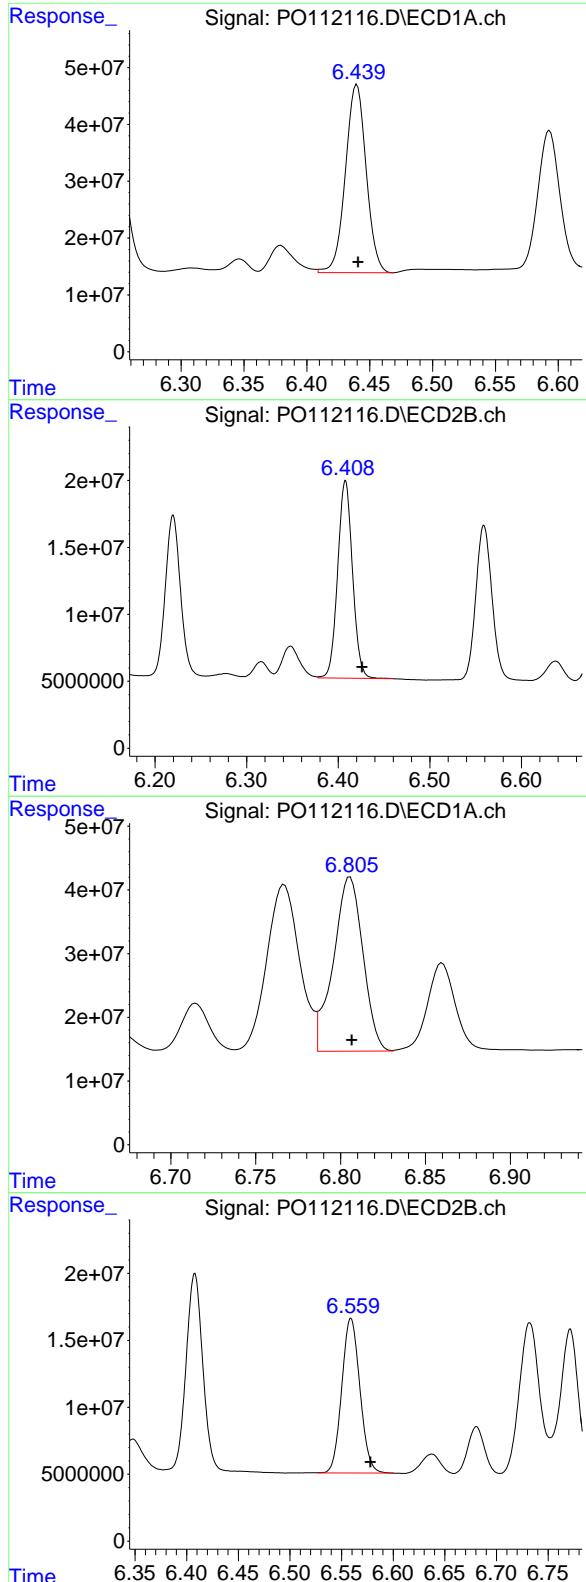

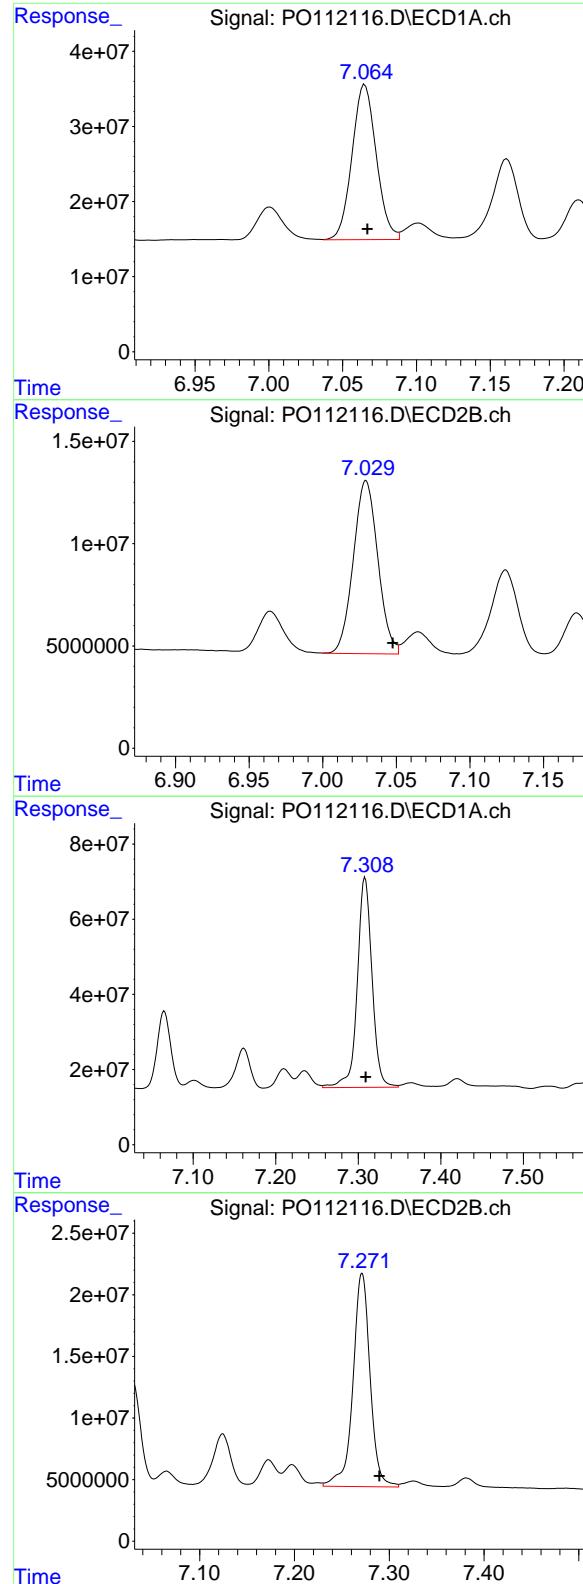

#34 AR-1260-4

R.T.: 7.065 min
Delta R.T.: -0.002 min
Response: 235897061
Conc: 541.98 ng/ml

Instrument: ECD_O
ClientSampleId: ICVPO070825

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/09/2025
Supervised By :mohammad ahmed 07/10/2025

#34 AR-1260-4

R.T.: 7.029 min
Delta R.T.: -0.019 min
Response: 98320139
Conc: 490.02 ng/ml

#35 AR-1260-5

R.T.: 7.308 min
Delta R.T.: 0.000 min
Response: 694127135
Conc: 549.79 ng/ml

#35 AR-1260-5

R.T.: 7.271 min
Delta R.T.: -0.018 min
Response: 218449847
Conc: 487.91 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0070825\
 Data File : P0112117.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jul 2025 23:11
 Operator : YP/AJ
 Sample : AR1242ICV500
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
ICVPO070825AR1242

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 09 04:05:04 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 09 04:02:23 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	3.673	3.666	512.4E6	321.3E6	51.790	50.425
2) SA Decachlor...	8.703	8.649	365.5E6	88771778	53.453	51.508

Target Compounds

16) L4 AR-1242-1	4.761	4.742	146.8E6	93302949	506.810	481.294
17) L4 AR-1242-2	4.779	4.761	220.6E6	136.9E6	518.026	483.283
18) L4 AR-1242-3	4.836	4.936	139.5E6	71189360	509.797	488.679
19) L4 AR-1242-4	4.956	5.020	112.3E6	68561477	498.302	483.370
20) L4 AR-1242-5	5.607	5.540	110.4E6	88688434	521.388	488.012



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0070825\
 Data File : P0112117.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jul 2025 23:11
 Operator : YP/AJ
 Sample : AR12421ICV500
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
ICVPO070825AR1242

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 09 04:05:04 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 09 04:02:23 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

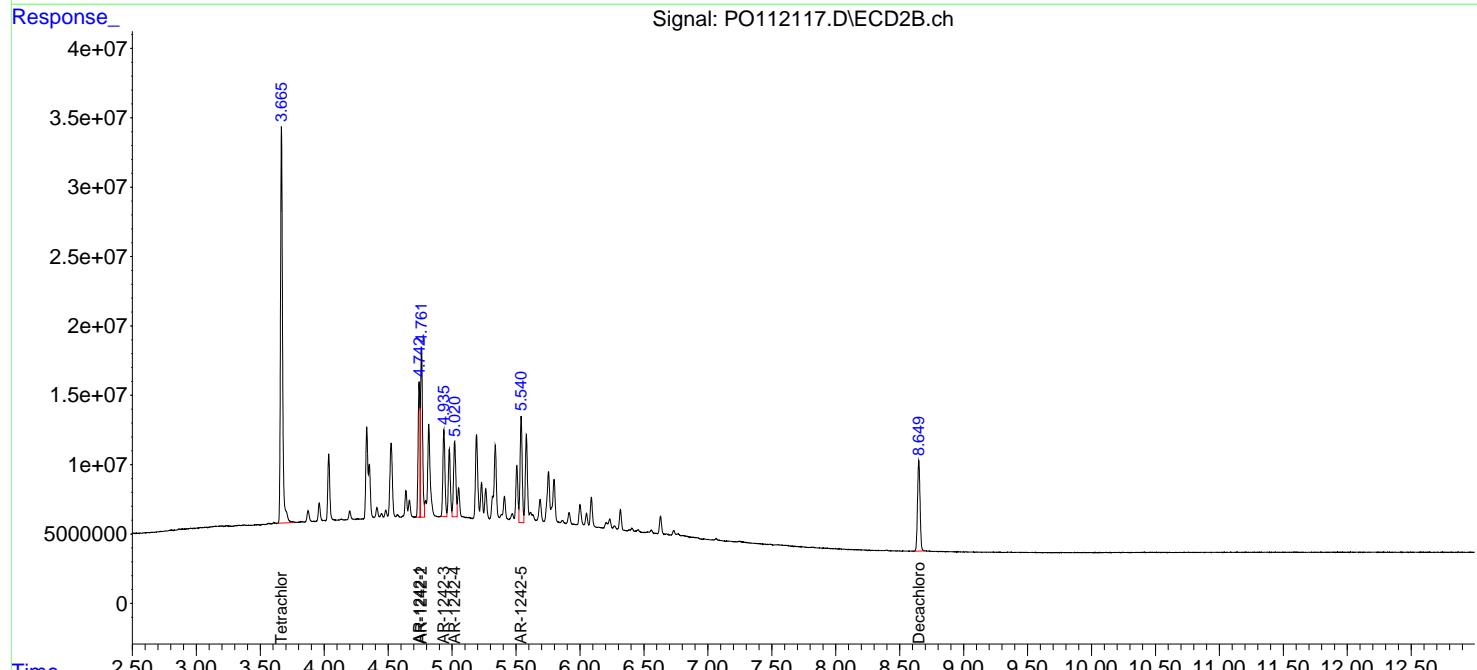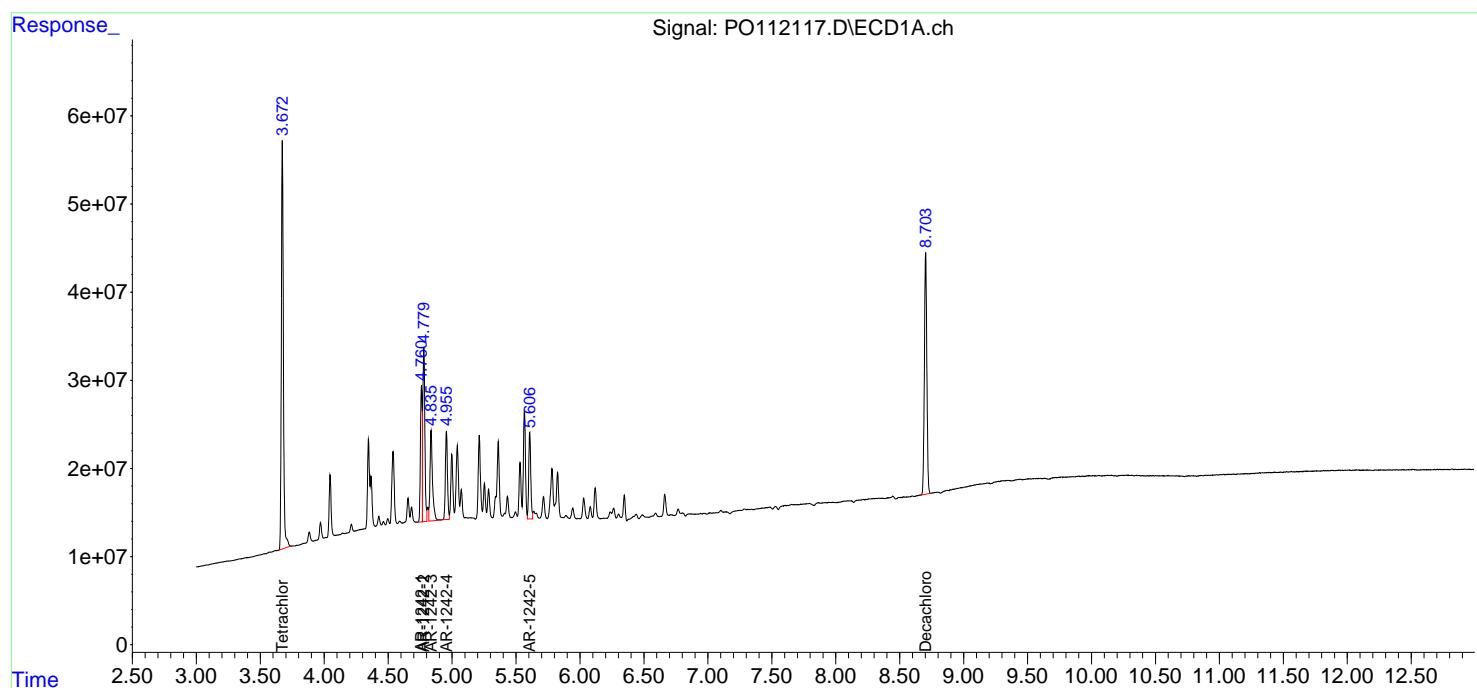

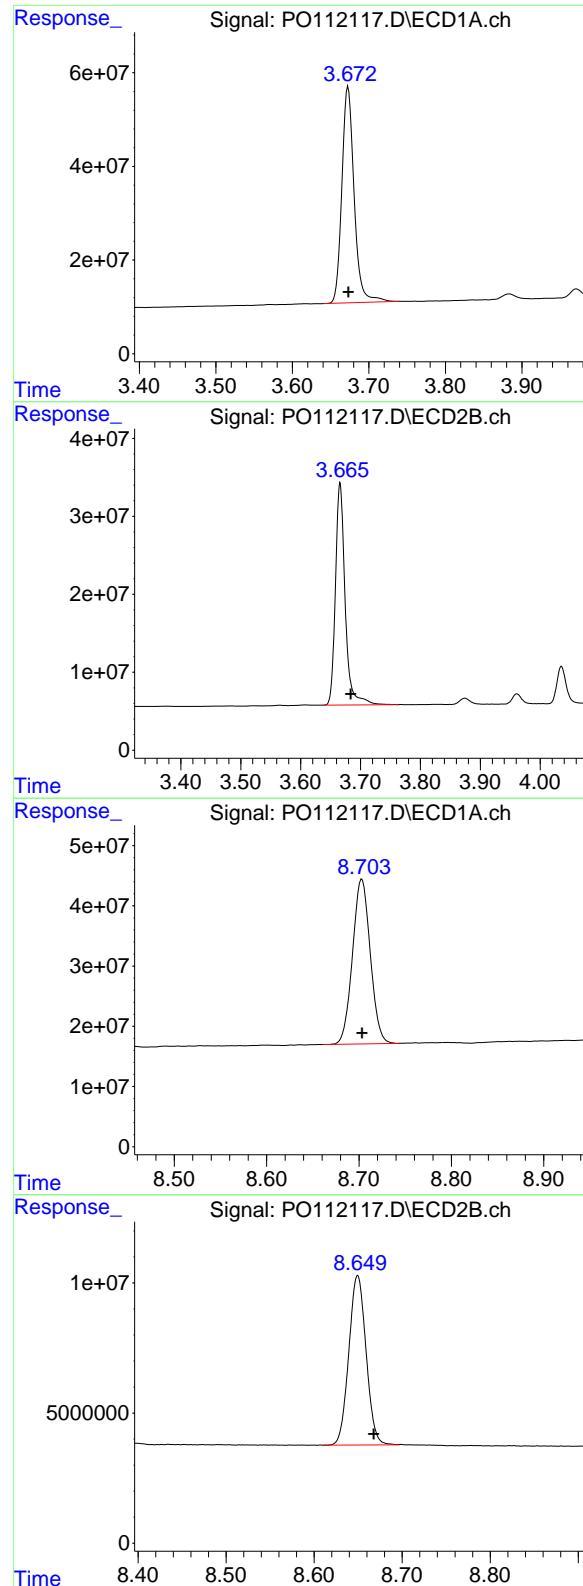

#1 Tetrachloro-m-xylene

R.T.: 3.673 min
Delta R.T.: 0.000 min
Response: 512444469
Conc: 51.79 ng/ml

Instrument: ECD_O
ClientSampleId: ICVPO070825AR1242

#1 Tetrachloro-m-xylene


R.T.: 3.666 min
Delta R.T.: -0.018 min
Response: 321262711
Conc: 50.43 ng/ml

#2 Decachlorobiphenyl

R.T.: 8.703 min
Delta R.T.: 0.000 min
Response: 365459376
Conc: 53.45 ng/ml

#2 Decachlorobiphenyl

R.T.: 8.649 min
Delta R.T.: -0.018 min
Response: 88771778
Conc: 51.51 ng/ml

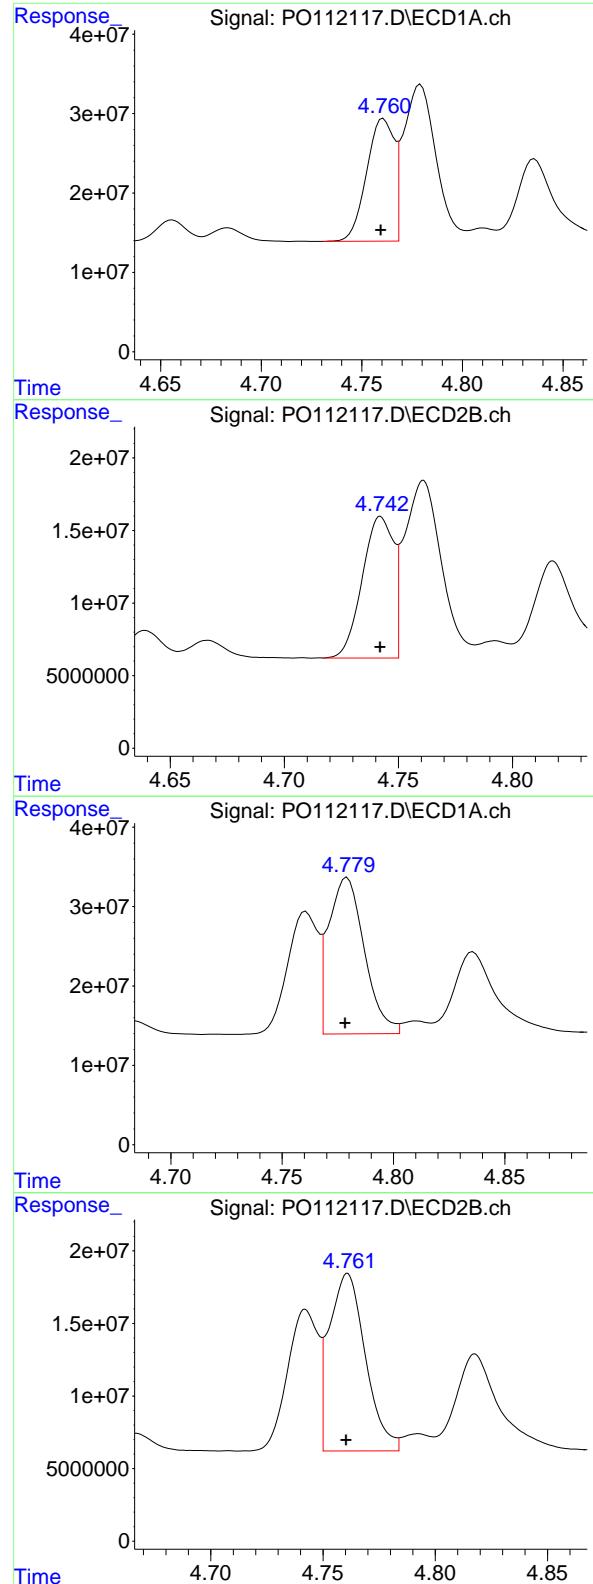

#16 AR-1242-1

R.T.: 4.761 min
 Delta R.T.: 0.001 min
 Response: 146790775
 Conc: 506.81 ng/ml

Instrument: ECD_O
 ClientSampleId: ICVPO070825AR1242

#16 AR-1242-1

R.T.: 4.742 min
 Delta R.T.: 0.000 min
 Response: 93302949
 Conc: 481.29 ng/ml

#17 AR-1242-2

R.T.: 4.779 min
 Delta R.T.: 0.000 min
 Response: 220637618
 Conc: 518.03 ng/ml


#17 AR-1242-2

R.T.: 4.761 min
 Delta R.T.: 0.000 min
 Response: 136939485
 Conc: 483.28 ng/ml

#18 AR-1242-3


R.T.: 4.836 min
 Delta R.T.: 0.000 min
 Response: 139524172
 Conc: 509.80 ng/ml

Instrument: ECD_O
ClientSampleId: ICVPO070825AR1242

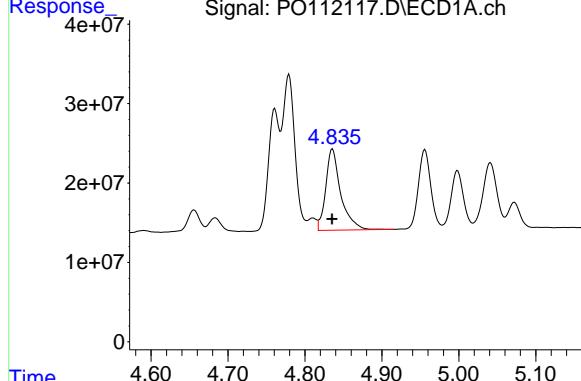


#18 AR-1242-3

R.T.: 4.936 min
 Delta R.T.: 0.000 min
 Response: 71189360
 Conc: 488.68 ng/ml

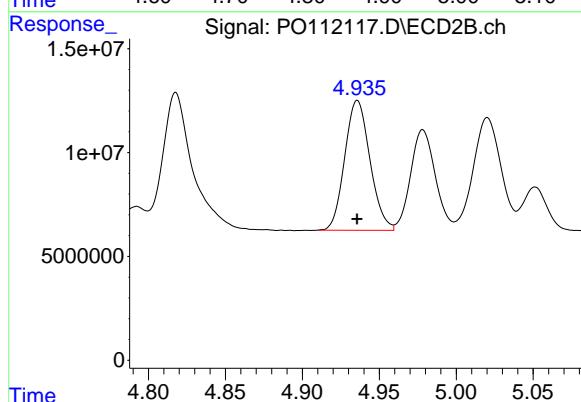


#19 AR-1242-4

R.T.: 4.956 min
 Delta R.T.: 0.001 min
 Response: 112276548
 Conc: 498.30 ng/ml

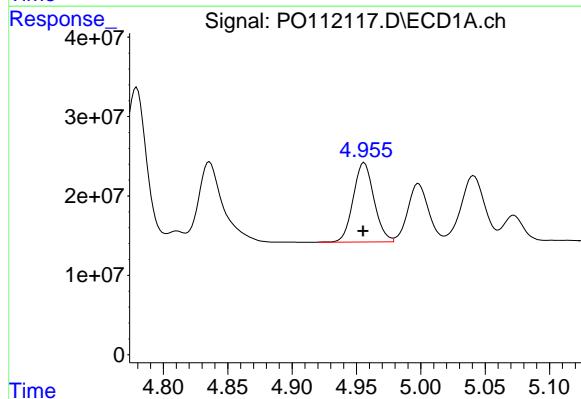

#19 AR-1242-4



R.T.: 5.020 min
 Delta R.T.: 0.000 min
 Response: 68561477
 Conc: 483.37 ng/ml

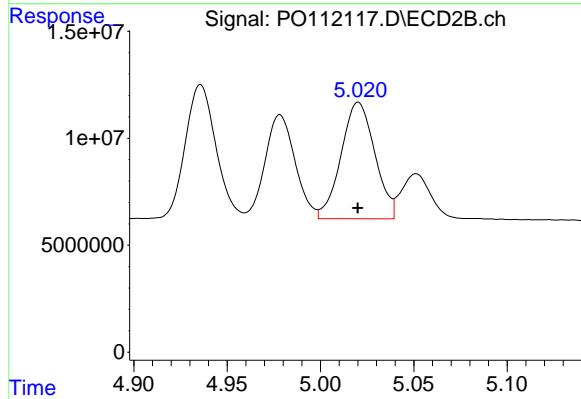

#20 AR-1242-5

R.T.: 5.607 min
Delta R.T.: 0.000 min
Response: 110362758
Conc: 521.39 ng/ml

Instrument: ECD_O
ClientSampleId: ICVPO070825AR1242

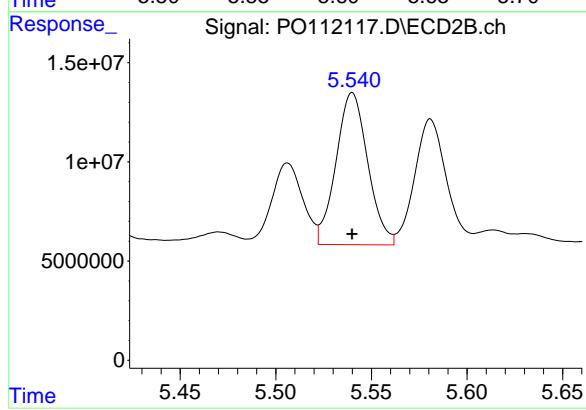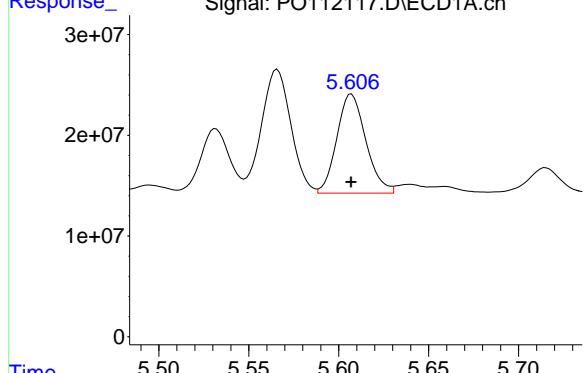

#20 AR-1242-5

R.T.: 5.540 min
Delta R.T.: 0.000 min
Response: 88688434
Conc: 488.01 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0070825\
 Data File : P0112118.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jul 2025 23:47
 Operator : YP/AJ
 Sample : AR1248ICV500
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
ICVPO070825AR1248

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 09 04:05:21 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 09 04:02:23 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	3.673	3.666	508.1E6	317.9E6	51.354	49.890
2) SA Decachlor...	8.702	8.650	362.9E6	88364492	53.072	51.272

Target Compounds

21) L5 AR-1248-1	4.761	4.742	111.3E6	71004811	490.349	459.970
22) L5 AR-1248-2	4.998	4.979	149.3E6	96786968	484.269	470.370
23) L5 AR-1248-3	5.213	5.020	189.9E6	101.5E6	466.127	472.319
24) L5 AR-1248-4	5.565	5.191	278.9E6	121.0E6	483.314	467.745
25) L5 AR-1248-5	5.607	5.581	185.2E6	118.9E6	474.463	474.612



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0070825\
 Data File : P0112118.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jul 2025 23:47
 Operator : YP/AJ
 Sample : AR1248ICV500
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
ICVPO070825AR1248

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 09 04:05:21 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 09 04:02:23 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ m Signal #2 Info : 30M x 0.32mm x 0.25 μ m

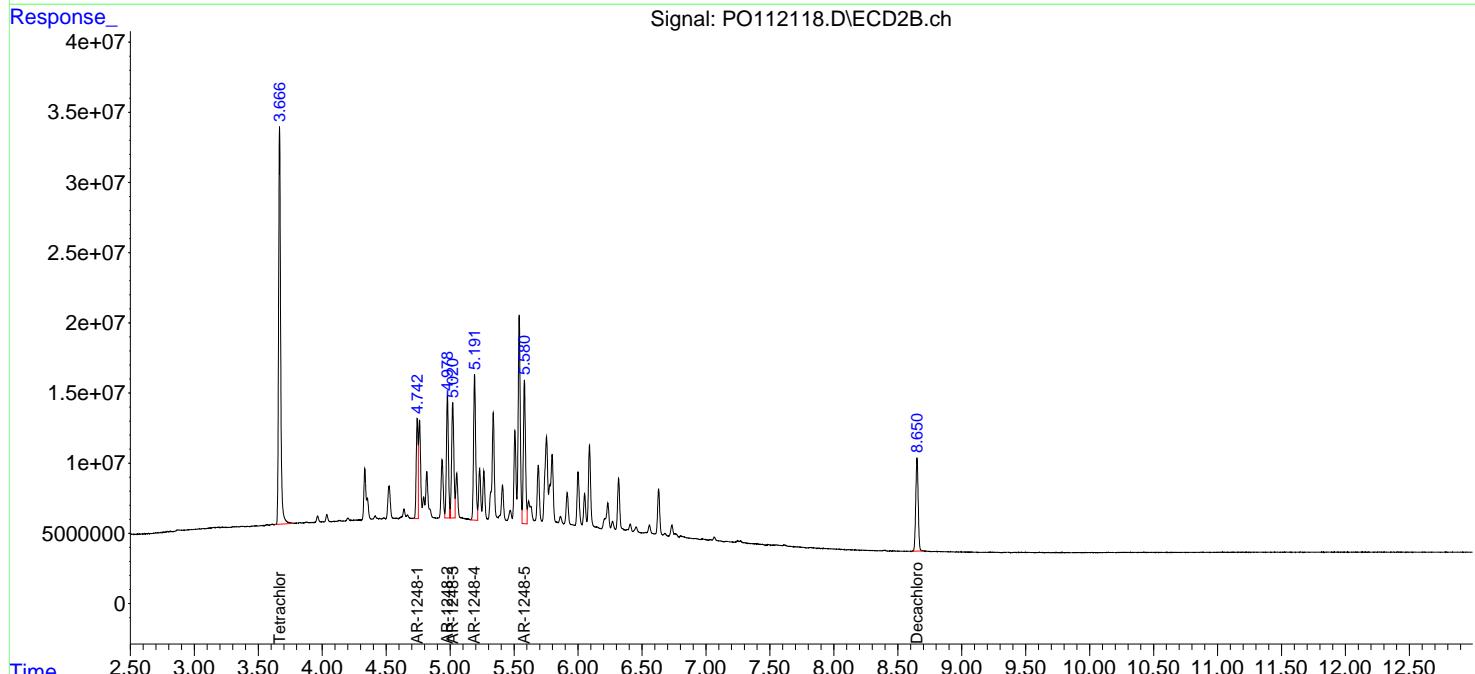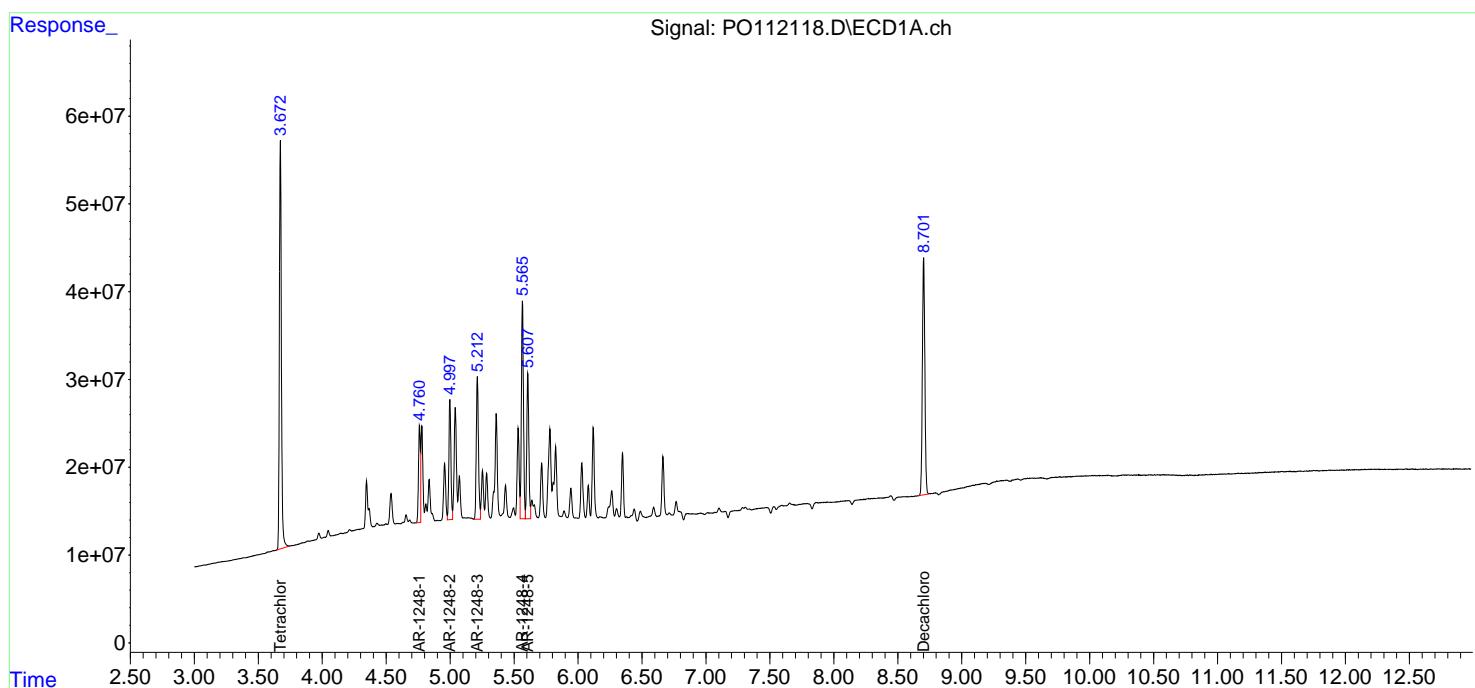

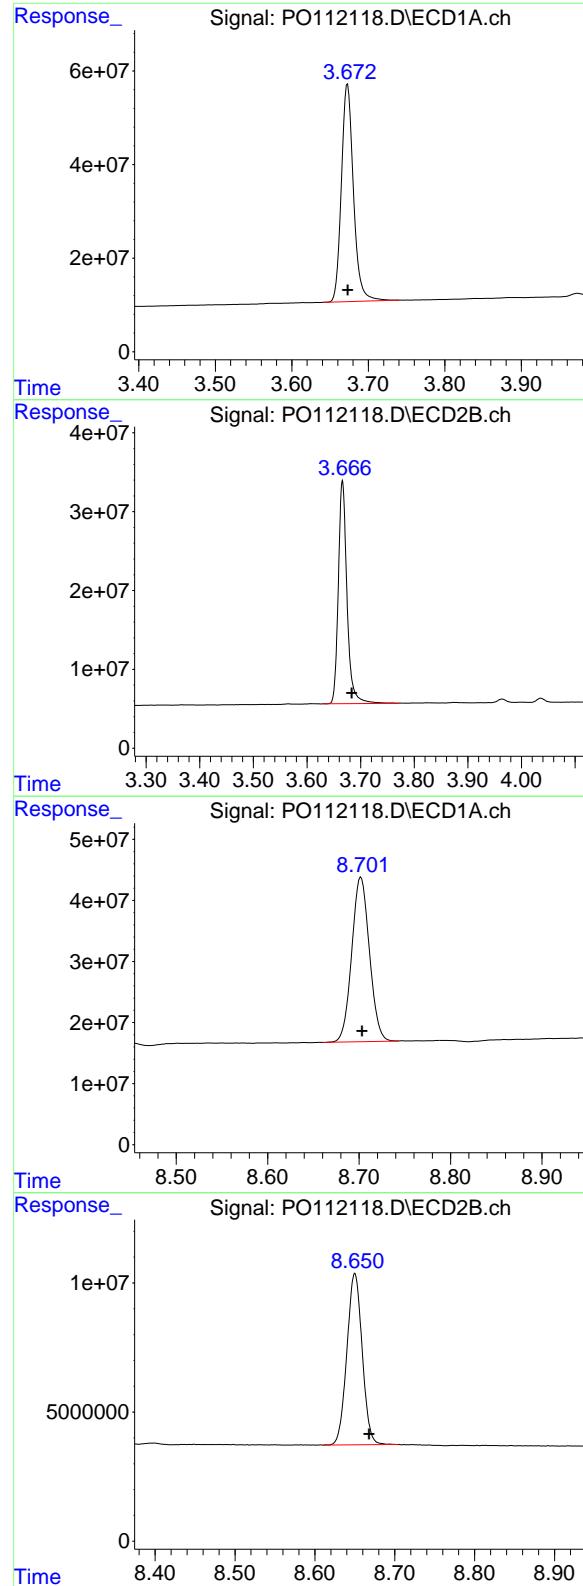

#1 Tetrachloro-m-xylene

R.T.: 3.673 min
 Delta R.T.: 0.000 min
 Response: 508134642
 Conc: 51.35 ng/ml

Instrument: ECD_O
ClientSampleId: ICVPO070825AR1248

#1 Tetrachloro-m-xylene

R.T.: 3.666 min
 Delta R.T.: -0.017 min
 Response: 317852312
 Conc: 49.89 ng/ml

#2 Decachlorobiphenyl

R.T.: 8.702 min
 Delta R.T.: -0.001 min
 Response: 362852383
 Conc: 53.07 ng/ml


#2 Decachlorobiphenyl

R.T.: 8.650 min
 Delta R.T.: -0.018 min
 Response: 88364492
 Conc: 51.27 ng/ml

#21 AR-1248-1


R.T.: 4.761 min
 Delta R.T.: 0.000 min
 Response: 111259949
 Conc: 490.35 ng/ml

Instrument: ECD_O
ClientSampleId: ICVPO070825AR1248




#21 AR-1248-1

R.T.: 4.742 min
 Delta R.T.: -0.001 min
 Response: 71004811
 Conc: 459.97 ng/ml

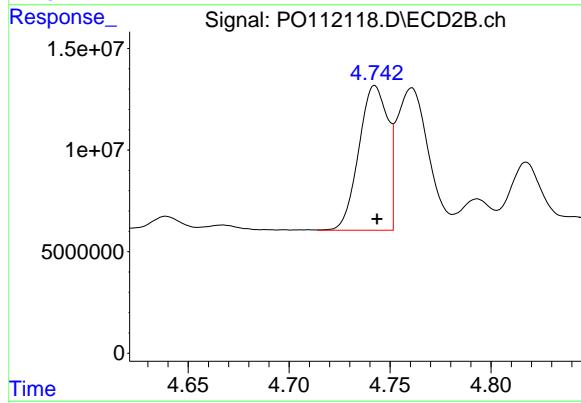


#22 AR-1248-2

R.T.: 4.998 min
 Delta R.T.: -0.002 min
 Response: 149312470
 Conc: 484.27 ng/ml

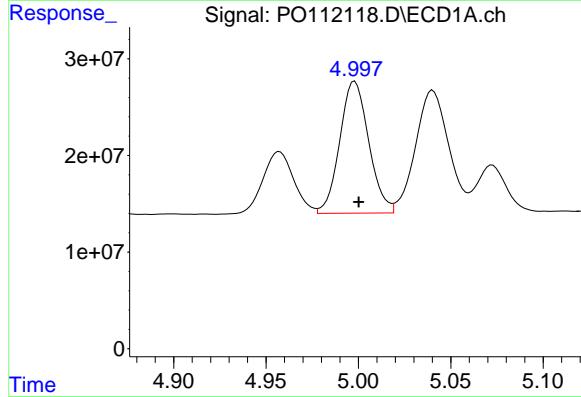

#22 AR-1248-2


R.T.: 4.979 min
 Delta R.T.: -0.001 min
 Response: 96786968
 Conc: 470.37 ng/ml

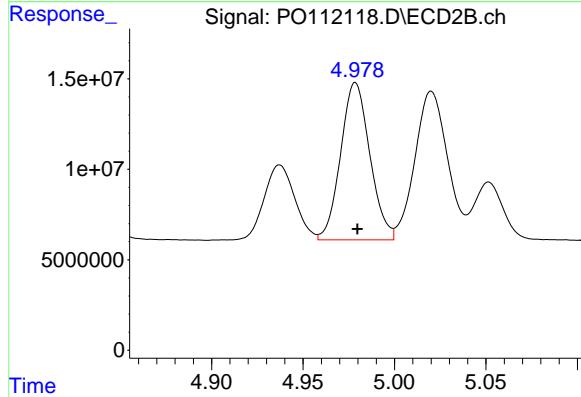

#23 AR-1248-3


R.T.: 5.213 min
 Delta R.T.: -0.001 min
 Response: 189862604
 Conc: 466.13 ng/ml

Instrument: ECD_O
ClientSampleId: ICVPO070825AR1248

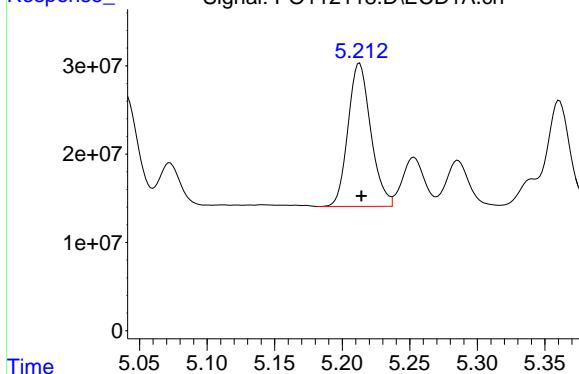


#23 AR-1248-3

R.T.: 5.020 min
 Delta R.T.: -0.001 min
 Response: 101453483
 Conc: 472.32 ng/ml

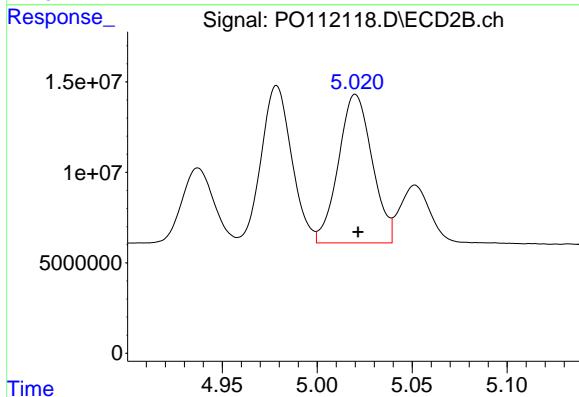


#24 AR-1248-4

R.T.: 5.565 min
 Delta R.T.: -0.002 min
 Response: 278943468
 Conc: 483.31 ng/ml

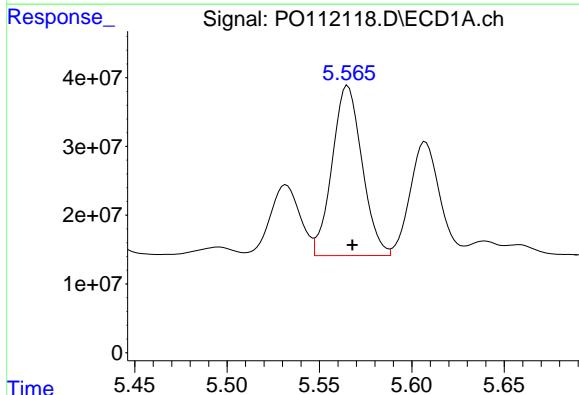

#24 AR-1248-4



R.T.: 5.191 min
 Delta R.T.: 0.000 min
 Response: 121018109
 Conc: 467.74 ng/ml

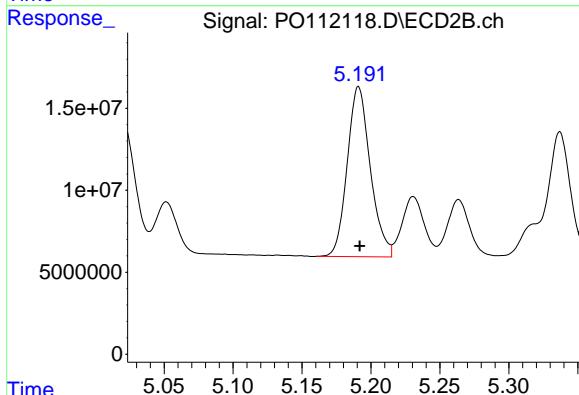

#25 AR-1248-5

R.T.: 5.607 min
Delta R.T.: -0.002 min
Response: 185185137
Conc: 474.46 ng/ml

Instrument: ECD_O
ClientSampleId: ICPPO070825AR1248

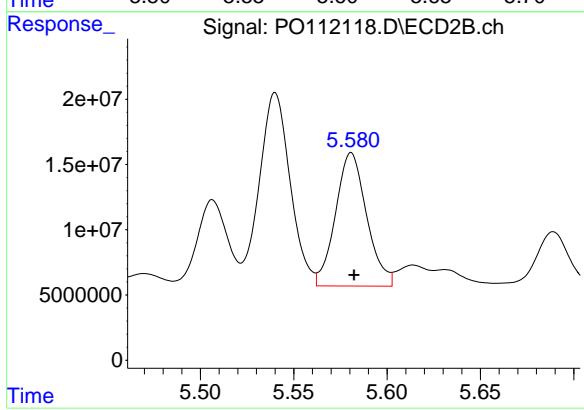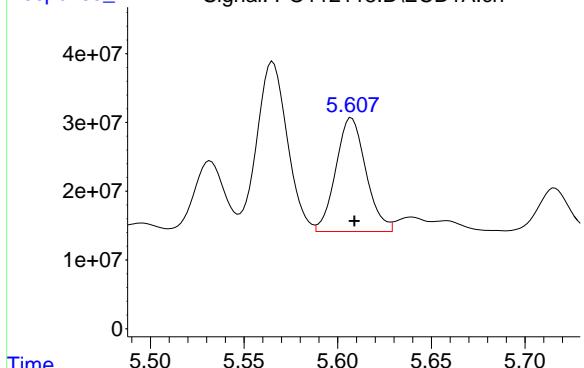

#25 AR-1248-5

R.T.: 5.581 min
Delta R.T.: -0.001 min
Response: 118913676
Conc: 474.61 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0070825\
 Data File : P0112119.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Jul 2025 00:24
 Operator : YP/AJ
 Sample : AR1254ICV500
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
ICVPO070825AR1254

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 09 04:05:39 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 09 04:02:23 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	3.673	3.666	520.2E6	322.7E6	52.569	50.649
2) SA Decachlor...	8.702	8.648	368.3E6	89811642	53.866	52.111

Target Compounds

26) L6 AR-1254-1	5.566	5.541	297.8E6	181.0E6	484.137	474.939
27) L6 AR-1254-2	5.715	5.688	261.9E6	156.8E6	488.891	472.651
28) L6 AR-1254-3	6.119	6.089	408.1E6	227.3E6	486.021	471.452
29) L6 AR-1254-4	6.348	6.317	268.6E6	129.6E6	558.360	496.987
30) L6 AR-1254-5	6.768	6.733	381.5E6	170.5E6	492.940	478.367



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.





Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0070825\
 Data File : P0112119.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Jul 2025 00:24
 Operator : YP/AJ
 Sample : AR1254ICV500
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
ICVPO070825AR1254

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 09 04:05:39 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 09 04:02:23 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

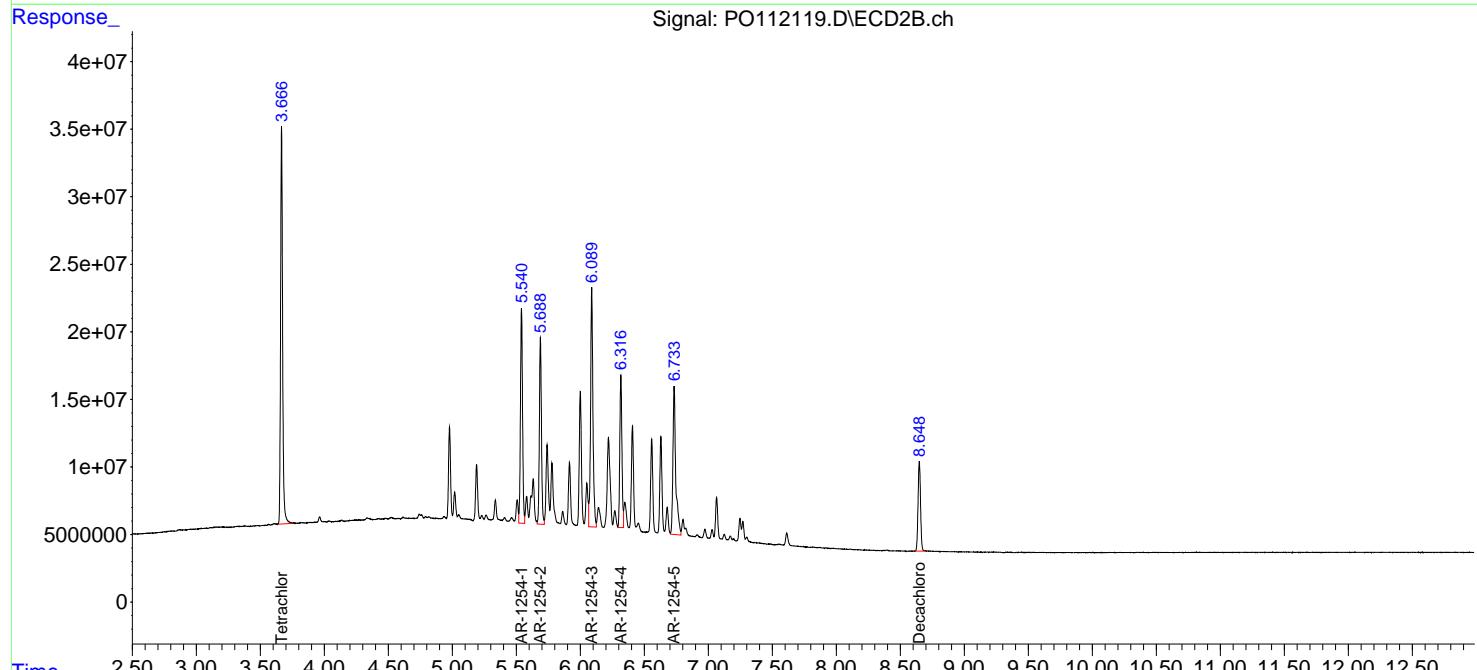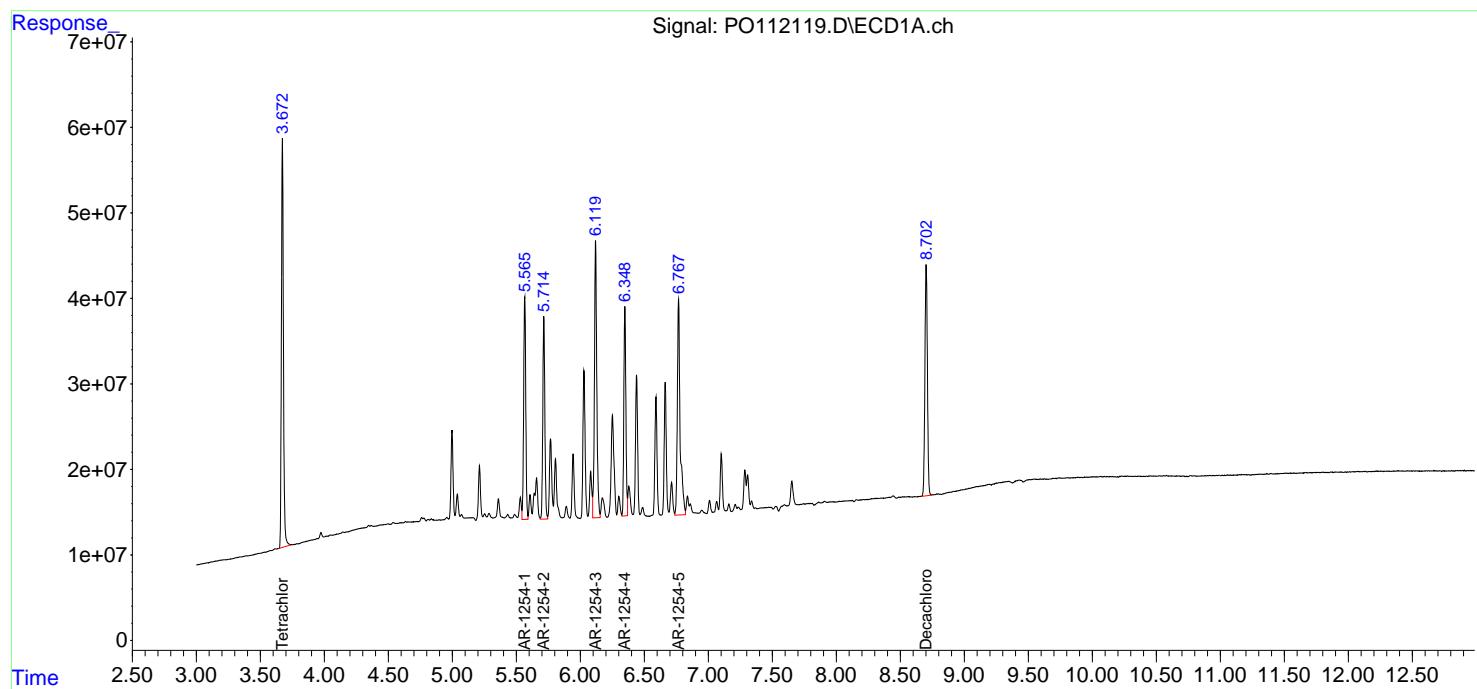

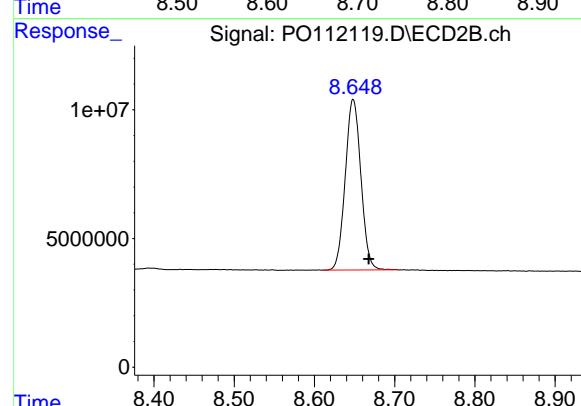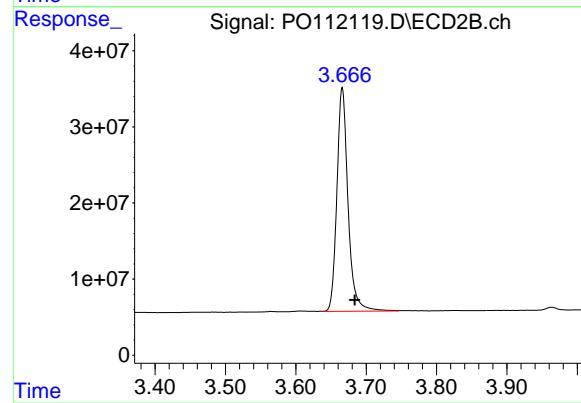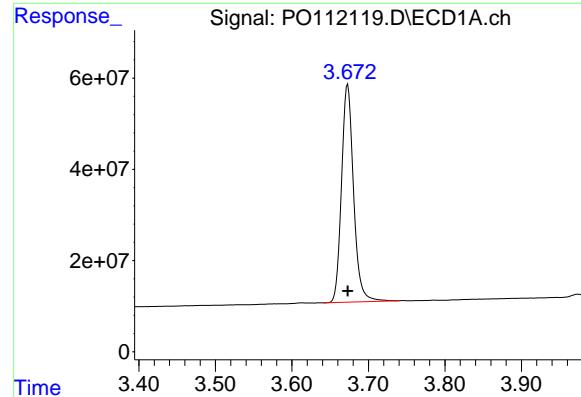

#1 Tetrachloro-m-xylene

R.T.: 3.673 min
Delta R.T.: 0.000 min
Response: 520156758
Conc: 52.57 ng/ml

Instrument: ECD_O
ClientSampleId: ICVPO070825AR1254

#1 Tetrachloro-m-xylene

R.T.: 3.666 min
Delta R.T.: -0.018 min
Response: 322690746
Conc: 50.65 ng/ml

#2 Decachlorobiphenyl

R.T.: 8.702 min
Delta R.T.: 0.000 min
Response: 368283668
Conc: 53.87 ng/ml


#2 Decachlorobiphenyl

R.T.: 8.648 min
Delta R.T.: -0.020 min
Response: 89811642
Conc: 52.11 ng/ml

#26 AR-1254-1


R.T.: 5.566 min
 Delta R.T.: 0.000 min
 Response: 297798906
 Conc: 484.14 ng/ml

Instrument: ECD_O
ClientSampleId: ICVPO070825AR1254




#26 AR-1254-1

R.T.: 5.541 min
 Delta R.T.: 0.000 min
 Response: 181031677
 Conc: 474.94 ng/ml

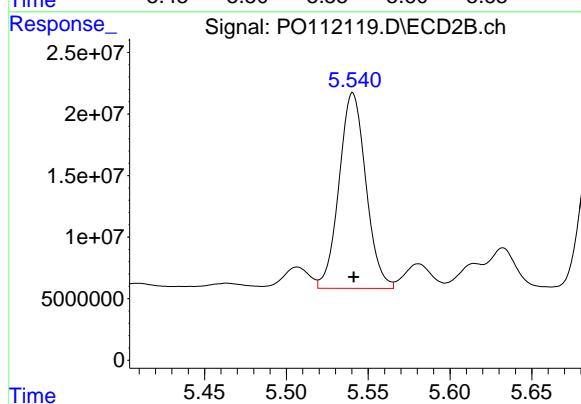


#27 AR-1254-2

R.T.: 5.715 min
 Delta R.T.: 0.000 min
 Response: 261892236
 Conc: 488.89 ng/ml

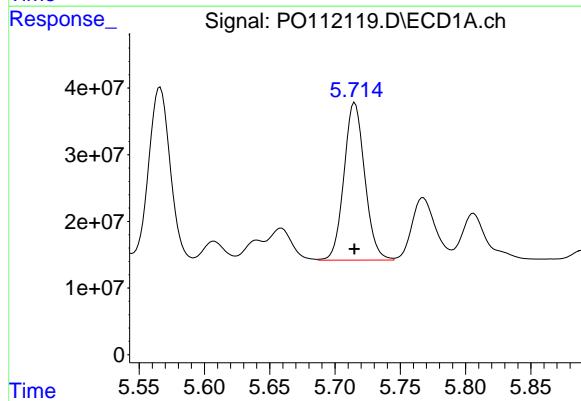

#27 AR-1254-2


R.T.: 5.688 min
 Delta R.T.: 0.000 min
 Response: 156830775
 Conc: 472.65 ng/ml

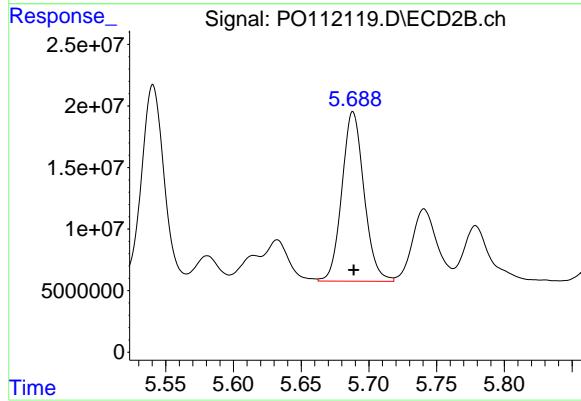

#28 AR-1254-3


R.T.: 6.119 min
 Delta R.T.: 0.000 min
 Response: 408052251
 Conc: 486.02 ng/ml

Instrument: ECD_O
ClientSampleId: ICVPO070825AR1254

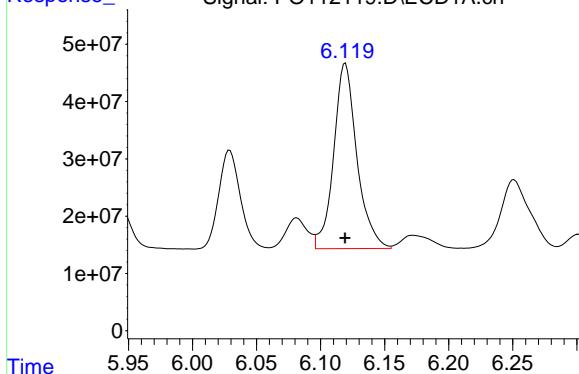


#28 AR-1254-3

R.T.: 6.089 min
 Delta R.T.: 0.000 min
 Response: 227260272
 Conc: 471.45 ng/ml

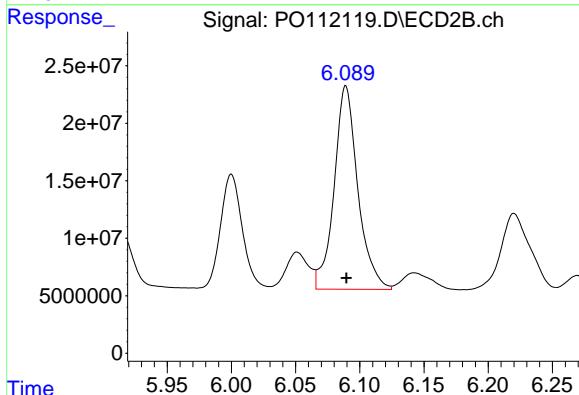


#29 AR-1254-4

R.T.: 6.348 min
 Delta R.T.: 0.000 min
 Response: 268581641
 Conc: 558.36 ng/ml

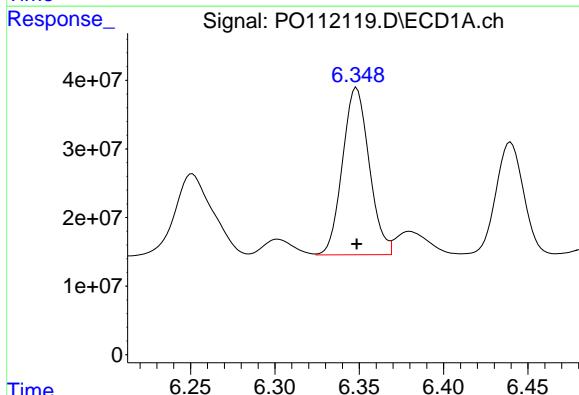

#29 AR-1254-4



R.T.: 6.317 min
 Delta R.T.: 0.000 min
 Response: 129562009
 Conc: 496.99 ng/ml

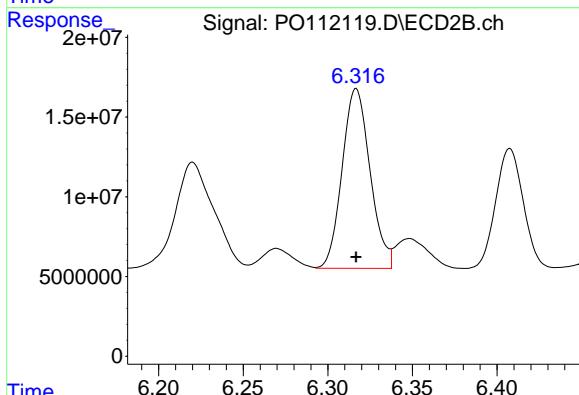

#30 AR-1254-5

R.T.: 6.768 min
Delta R.T.: 0.000 min
Response: 381510203
Conc: 492.94 ng/ml

Instrument: ECD_O
ClientSampleId: ICVPO070825AR1254

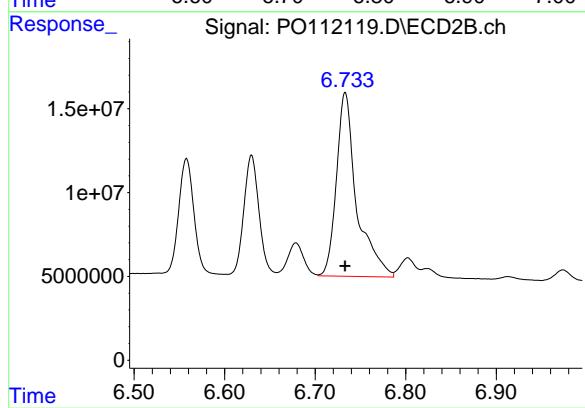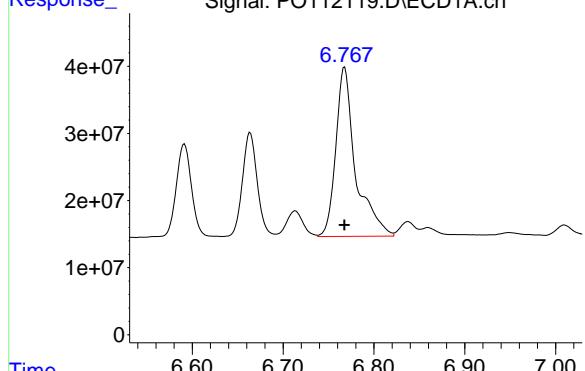

#30 AR-1254-5

R.T.: 6.733 min
Delta R.T.: 0.000 min
Response: 170469199
Conc: 478.37 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0070825\
 Data File : P0112120.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Jul 2025 01:01
 Operator : YP/AJ
 Sample : AR1268ICV500
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
ICVPO070825AR1268

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 09 03:54:46 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 09 03:33:24 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	3.672	3.666	507.9E6	314.4E6	50.119	49.097
2) SA Decachlor...	8.702	8.650	672.6E6	158.8E6	51.008	50.729

Target Compounds

41) L9 AR-1268-1	7.592	7.554	933.4E6	244.5E6	507.990	497.487
42) L9 AR-1268-2	7.658	7.619	787.7E6	208.0E6	505.709	498.485
43) L9 AR-1268-3	7.863	7.823	660.1E6	157.4E6	507.919	497.424
44) L9 AR-1268-4	8.153	8.110	233.4E6	55400600	485.897	496.813
45) L9 AR-1268-5	8.446	8.399	1686.7E6	361.3E6	516.807	497.353



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0070825\
 Data File : P0112120.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Jul 2025 01:01
 Operator : YP/AJ
 Sample : AR12681CV500
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
ICVPO070825AR1268

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 09 03:54:46 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 09 03:33:24 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

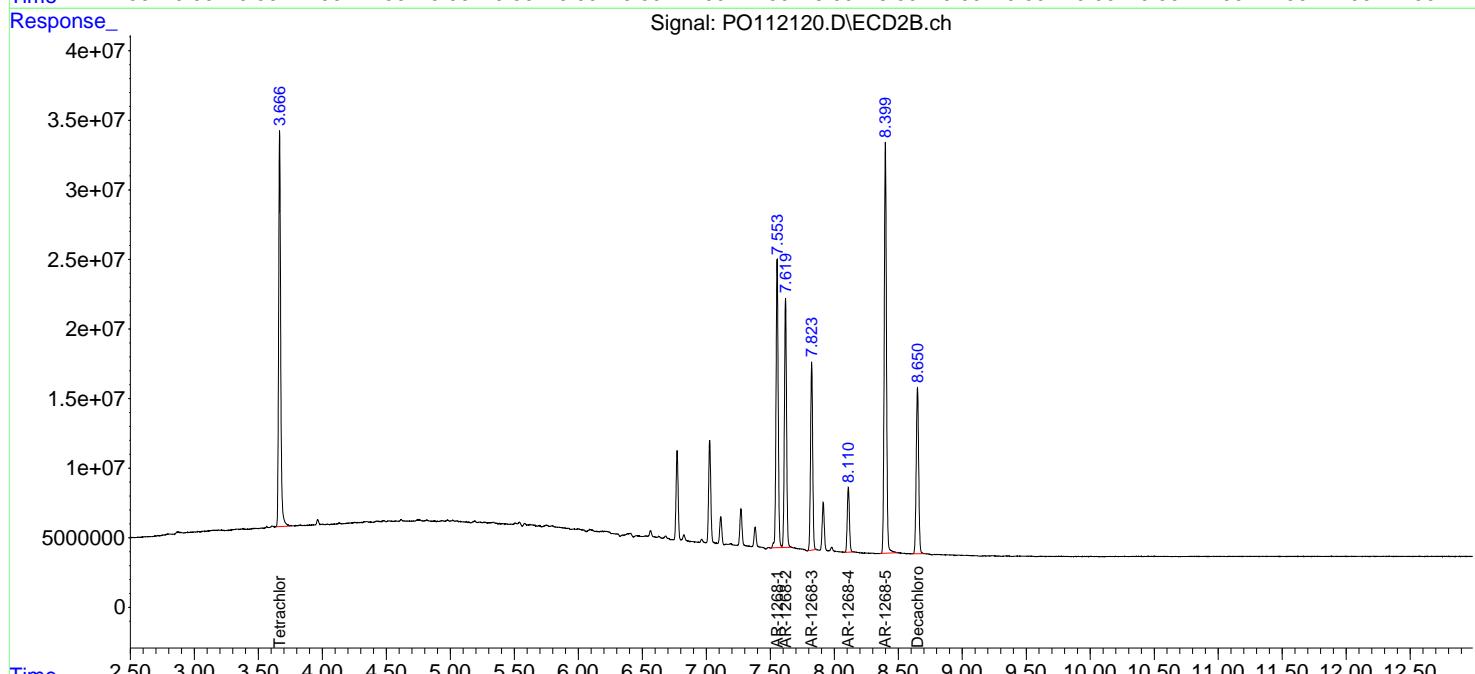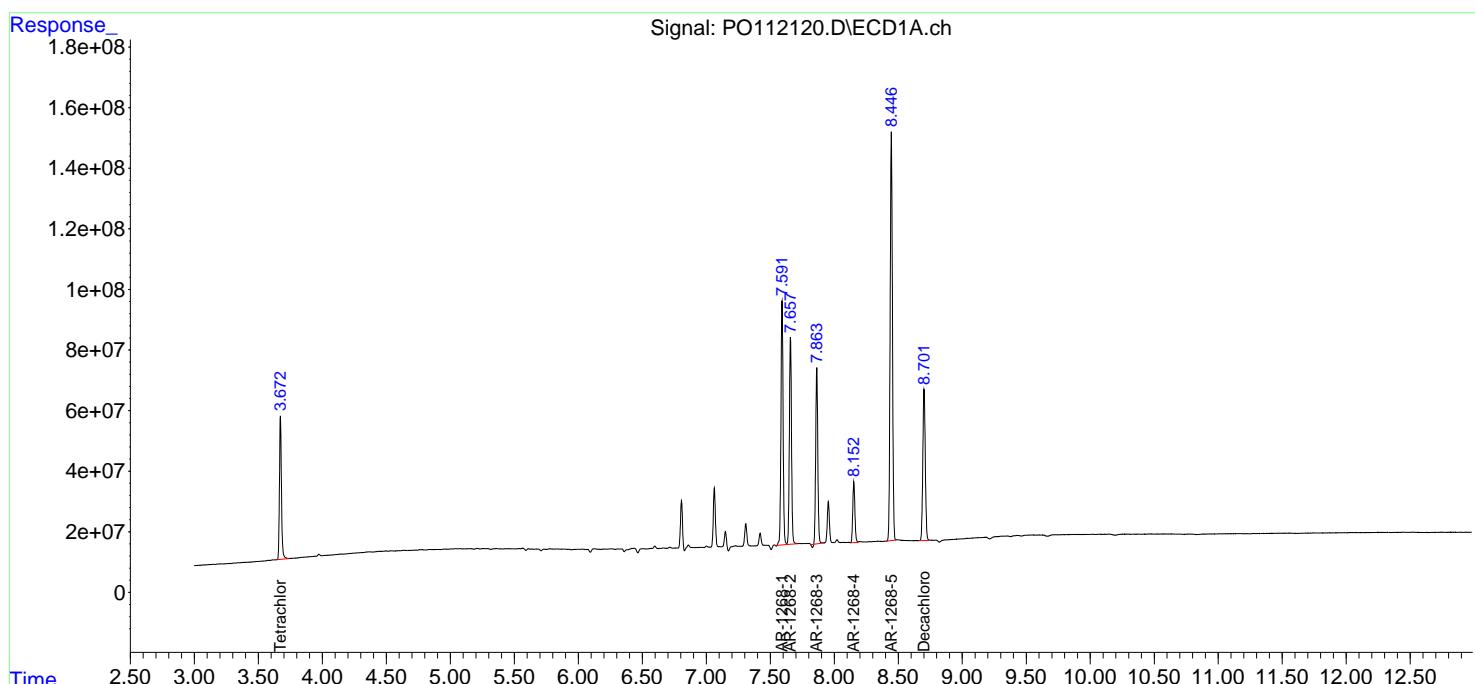

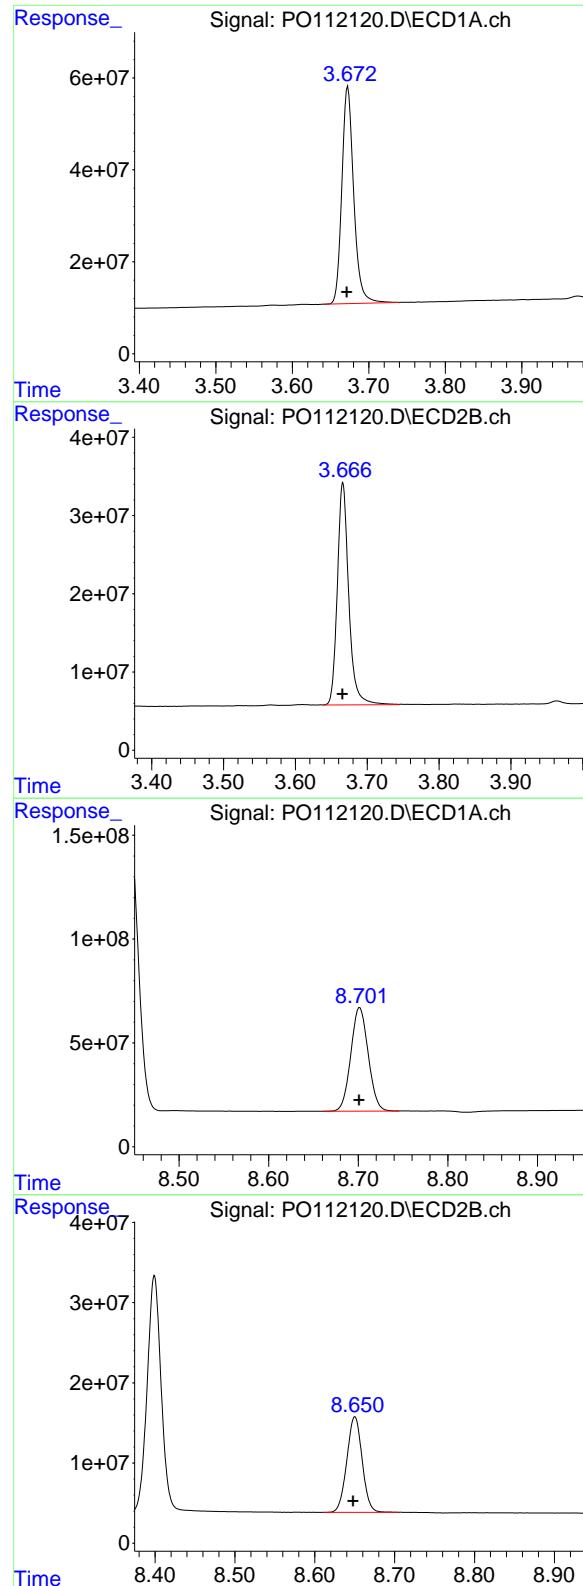

#1 Tetrachloro-m-xylene

R.T.: 3.672 min
 Delta R.T.: 0.001 min
 Response: 507948794
 Conc: 50.12 ng/ml

Instrument: ECD_O
 ClientSampleId: ICVPO070825AR1268

#1 Tetrachloro-m-xylene

R.T.: 3.666 min
 Delta R.T.: 0.000 min
 Response: 314362501
 Conc: 49.10 ng/ml

#2 Decachlorobiphenyl

R.T.: 8.702 min
 Delta R.T.: 0.000 min
 Response: 672554151
 Conc: 51.01 ng/ml


#2 Decachlorobiphenyl

R.T.: 8.650 min
 Delta R.T.: 0.002 min
 Response: 158800125
 Conc: 50.73 ng/ml

#41 AR-1268-1


R.T.: 7.592 min
 Delta R.T.: 0.002 min
 Response: 933409161
 Conc: 507.99 ng/ml

Instrument: ECD_O
ClientSampleId: ICVPO070825AR1268

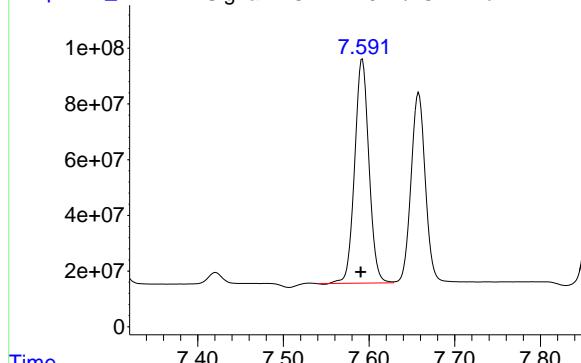


#41 AR-1268-1

R.T.: 7.554 min
 Delta R.T.: 0.001 min
 Response: 244492560
 Conc: 497.49 ng/ml

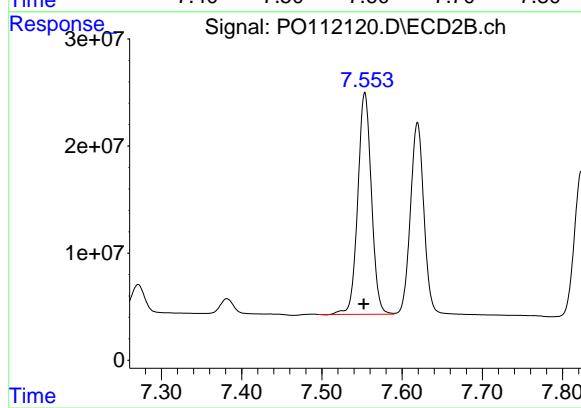


#42 AR-1268-2

R.T.: 7.658 min
 Delta R.T.: 0.002 min
 Response: 787696002
 Conc: 505.71 ng/ml



#42 AR-1268-2





R.T.: 7.619 min
 Delta R.T.: 0.002 min
 Response: 207960999
 Conc: 498.48 ng/ml

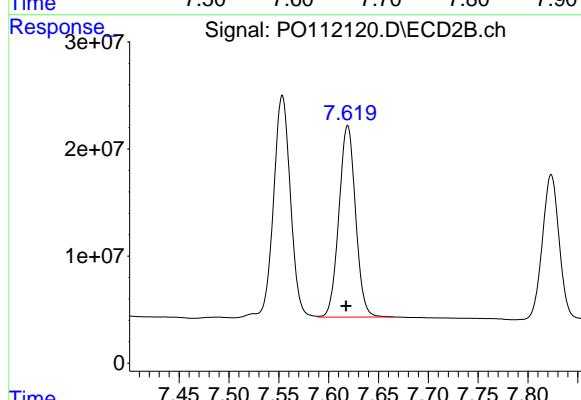

#43 AR-1268-3

R.T.: 7.863 min
 Delta R.T.: 0.002 min
 Response: 660130633
 Conc: 507.92 ng/ml

Instrument: ECD_O
ClientSampleId: ICVPO070825AR1268

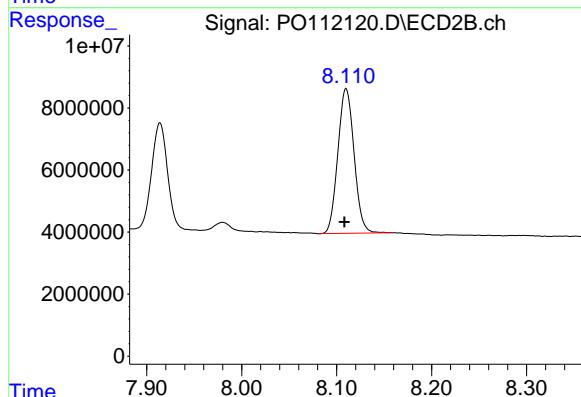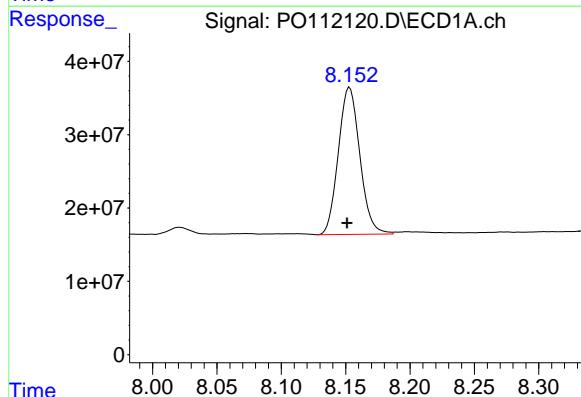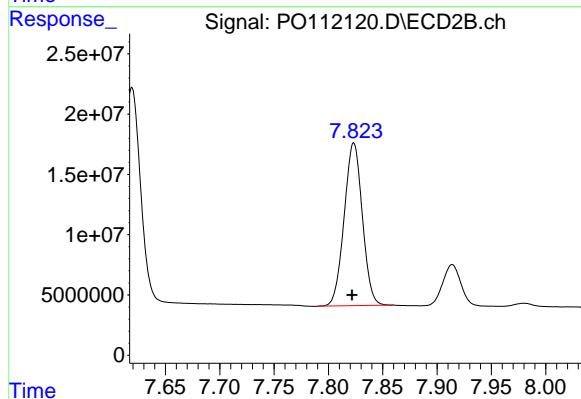

#43 AR-1268-3

R.T.: 7.823 min
 Delta R.T.: 0.002 min
 Response: 157379415
 Conc: 497.42 ng/ml

#44 AR-1268-4

R.T.: 8.153 min
 Delta R.T.: 0.002 min
 Response: 233428745
 Conc: 485.90 ng/ml



#44 AR-1268-4

R.T.: 8.110 min
 Delta R.T.: 0.002 min
 Response: 55400600
 Conc: 496.81 ng/ml

#45 AR-1268-5

R.T.: 8.446 min
Delta R.T.: 0.002 min
Response: 1686709570
Conc: 516.81 ng/ml

Instrument: ECD_O
ClientSampleId: ICVPO070825AR1268

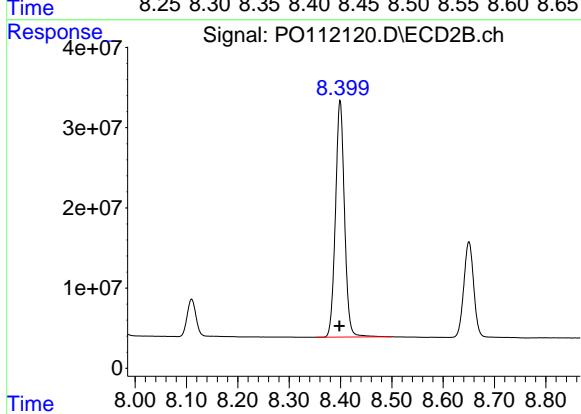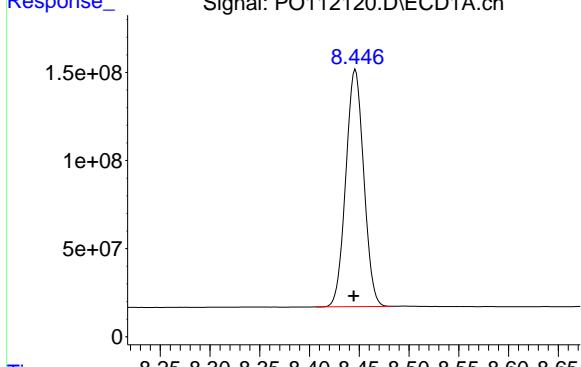

#45 AR-1268-5

R.T.: 8.399 min
Delta R.T.: 0.001 min
Response: 361335866
Conc: 497.35 ng/ml

RETENTION TIMES OF INITIAL CALIBRATION

Lab Name:	Alliance	Contract:	NOBI03
Lab Code:	ACE	SDG NO.:	Q2639
Instrument ID:	ECD_P	Calibration Date(s):	07/07/2025 07/08/2025
		Calibration Times:	21:03 04:24

GC Column: ZB-MR1 ID: 0.32 (mm)

LAB FILE ID:	RT 1000 =	PP073554.D	RT 750 =	PP073555.D
	RT 500 = PP073556.D	RT 250 = PP073557.D	RT 050 =	PP073558.D

COMPOUND	RT 1000	RT 750	RT 500	RT 250	RT 050	MEAN RT	RT WINDOW FROM	TO
Aroclor-1016-1 (1)	5.64	5.64	5.64	5.64	5.64	5.64	5.54	5.74
Aroclor-1016-2 (2)	5.66	5.66	5.66	5.66	5.66	5.66	5.56	5.76
Aroclor-1016-3 (3)	5.72	5.72	5.72	5.72	5.72	5.72	5.62	5.82
Aroclor-1016-4 (4)	5.82	5.82	5.82	5.82	5.82	5.82	5.72	5.92
Aroclor-1016-5 (5)	6.11	6.11	6.11	6.11	6.11	6.11	6.01	6.21
Aroclor-1260-1 (1)	7.23	7.23	7.23	7.23	7.23	7.23	7.13	7.33
Aroclor-1260-2 (2)	7.48	7.48	7.48	7.48	7.48	7.48	7.38	7.58
Aroclor-1260-3 (3)	7.84	7.84	7.84	7.84	7.84	7.84	7.74	7.94
Aroclor-1260-4 (4)	8.06	8.07	8.06	8.07	8.06	8.06	7.96	8.16
Aroclor-1260-5 (5)	8.38	8.38	8.38	8.39	8.38	8.38	8.28	8.48
Decachlorobiphenyl	10.18	10.18	10.18	10.18	10.17	10.18	10.08	10.28
Tetrachloro-m-xylene	4.49	4.49	4.49	4.49	4.49	4.49	4.39	4.59
Aroclor-1242-1 (1)	5.64	5.64	5.64	5.64	5.64	5.64	5.54	5.74
Aroclor-1242-2 (2)	5.66	5.66	5.66	5.66	5.66	5.66	5.56	5.76
Aroclor-1242-3 (3)	5.72	5.72	5.72	5.72	5.72	5.72	5.62	5.82
Aroclor-1242-4 (4)	5.82	5.82	5.82	5.82	5.82	5.82	5.72	5.92
Aroclor-1242-5 (5)	6.55	6.55	6.55	6.55	6.55	6.55	6.45	6.65
Decachlorobiphenyl	10.18	10.18	10.17	10.18	10.17	10.18	10.08	10.28
Tetrachloro-m-xylene	4.49	4.49	4.49	4.49	4.49	4.49	4.39	4.59
Aroclor-1248-1 (1)	5.64	5.64	5.64	5.64	5.63	5.64	5.54	5.74
Aroclor-1248-2 (2)	5.91	5.91	5.91	5.91	5.91	5.91	5.81	6.01
Aroclor-1248-3 (3)	6.11	6.11	6.11	6.11	6.11	6.11	6.01	6.21
Aroclor-1248-4 (4)	6.51	6.51	6.51	6.51	6.51	6.51	6.41	6.61
Aroclor-1248-5 (5)	6.55	6.55	6.55	6.55	6.55	6.55	6.45	6.65
Decachlorobiphenyl	10.18	10.18	10.17	10.18	10.17	10.18	10.08	10.28
Tetrachloro-m-xylene	4.49	4.49	4.49	4.49	4.49	4.49	4.39	4.59
Aroclor-1254-1 (1)	6.49	6.49	6.49	6.48	6.49	6.49	6.39	6.59
Aroclor-1254-2 (2)	6.70	6.70	6.70	6.70	6.70	6.70	6.60	6.80
Aroclor-1254-3 (3)	7.07	7.07	7.06	7.06	7.06	7.07	6.97	7.17
Aroclor-1254-4 (4)	7.35	7.35	7.35	7.35	7.35	7.35	7.25	7.45
Aroclor-1254-5 (5)	7.76	7.76	7.76	7.76	7.76	7.76	7.66	7.86
Decachlorobiphenyl	10.18	10.18	10.17	10.18	10.18	10.18	10.08	10.28
Tetrachloro-m-xylene	4.49	4.49	4.49	4.49	4.49	4.49	4.39	4.59
Aroclor-1268-1 (1)	8.69	8.69	8.69	8.69	8.69	8.69	8.59	8.79
Aroclor-1268-2 (2)	8.78	8.79	8.79	8.78	8.79	8.79	8.69	8.89
Aroclor-1268-3 (3)	9.01	9.01	9.01	9.01	9.02	9.01	8.91	9.11
Aroclor-1268-4 (4)	9.43	9.43	9.43	9.43	9.43	9.43	9.33	9.53
Aroclor-1268-5 (5)	9.84	9.84	9.84	9.84	9.84	9.84	9.74	9.94



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

RETENTION TIMES OF INITIAL CALIBRATION

Decachlorobiphenyl	10.18	10.18	10.18	10.17	10.18	10.18	10.08	10.28	1
Tetrachloro-m-xylene	4.49	4.49	4.49	4.49	4.49	4.49	4.39	4.59	2

1
2
3
4
5
6
7
8
9
10
11
12
13
14
15
16
17
18
19
20



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

RETENTION TIMES OF INITIAL CALIBRATION

Lab Name:	Alliance	Contract:	NOBI03
Lab Code:	ACE	SDG NO.:	Q2639
Instrument ID:	ECD_P	Calibration Date(s):	07/07/2025 07/08/2025
		Calibration Times:	21:03 04:24

GC Column: ZB-MR2 ID: 0.32 (mm)

LAB FILE ID:	RT 1000 =	PP073554.D	RT 750 =	PP073555.D
	RT 500 = PP073556.D	RT 250 = PP073557.D	RT 050 =	PP073558.D

COMPOUND	RT 1000	RT 750	RT 500	RT 250	RT 050	MEAN RT	RT WINDOW FROM	TO
Aroclor-1016-1 (1)	4.86	4.86	4.86	4.86	4.86	4.86	4.76	4.96
Aroclor-1016-2 (2)	4.88	4.88	4.88	4.88	4.88	4.88	4.78	4.98
Aroclor-1016-3 (3)	5.05	5.05	5.05	5.05	5.05	5.05	4.95	5.15
Aroclor-1016-4 (4)	5.10	5.10	5.09	5.10	5.09	5.09	4.99	5.19
Aroclor-1016-5 (5)	5.31	5.31	5.31	5.31	5.31	5.31	5.21	5.41
Aroclor-1260-1 (1)	6.34	6.34	6.34	6.34	6.34	6.34	6.24	6.44
Aroclor-1260-2 (2)	6.53	6.53	6.53	6.53	6.53	6.53	6.43	6.63
Aroclor-1260-3 (3)	6.68	6.68	6.68	6.68	6.68	6.68	6.58	6.78
Aroclor-1260-4 (4)	7.15	7.15	7.15	7.15	7.15	7.15	7.05	7.25
Aroclor-1260-5 (5)	7.39	7.39	7.39	7.39	7.39	7.39	7.29	7.49
Decachlorobiphenyl	8.78	8.78	8.78	8.78	8.78	8.78	8.68	8.88
Tetrachloro-m-xylene	3.78	3.78	3.78	3.78	3.78	3.78	3.68	3.88
Aroclor-1242-1 (1)	4.86	4.86	4.86	4.86	4.86	4.86	4.76	4.96
Aroclor-1242-2 (2)	4.87	4.88	4.88	4.88	4.88	4.88	4.78	4.98
Aroclor-1242-3 (3)	5.05	5.05	5.05	5.05	5.05	5.05	4.95	5.15
Aroclor-1242-4 (4)	5.14	5.14	5.14	5.14	5.14	5.14	5.04	5.24
Aroclor-1242-5 (5)	5.66	5.66	5.66	5.66	5.66	5.66	5.56	5.76
Decachlorobiphenyl	8.78	8.78	8.78	8.78	8.78	8.78	8.68	8.88
Tetrachloro-m-xylene	3.78	3.78	3.78	3.78	3.78	3.78	3.68	3.88
Aroclor-1248-1 (1)	4.86	4.86	4.86	4.86	4.86	4.86	4.76	4.96
Aroclor-1248-2 (2)	5.09	5.09	5.09	5.09	5.09	5.09	4.99	5.19
Aroclor-1248-3 (3)	5.14	5.14	5.14	5.14	5.14	5.14	5.04	5.24
Aroclor-1248-4 (4)	5.31	5.31	5.31	5.31	5.31	5.31	5.21	5.41
Aroclor-1248-5 (5)	5.70	5.70	5.70	5.70	5.70	5.70	5.60	5.80
Decachlorobiphenyl	8.78	8.78	8.78	8.78	8.78	8.78	8.68	8.88
Tetrachloro-m-xylene	3.78	3.78	3.78	3.78	3.78	3.78	3.68	3.88
Aroclor-1254-1 (1)	5.66	5.66	5.66	5.66	5.66	5.66	5.56	5.76
Aroclor-1254-2 (2)	5.81	5.81	5.81	5.81	5.81	5.81	5.71	5.91
Aroclor-1254-3 (3)	6.21	6.21	6.21	6.21	6.21	6.21	6.11	6.31
Aroclor-1254-4 (4)	6.44	6.44	6.44	6.44	6.44	6.44	6.34	6.54
Aroclor-1254-5 (5)	6.85	6.85	6.85	6.85	6.85	6.85	6.75	6.95
Decachlorobiphenyl	8.78	8.78	8.78	8.78	8.78	8.78	8.68	8.88
Tetrachloro-m-xylene	3.78	3.78	3.78	3.78	3.78	3.78	3.68	3.88
Aroclor-1268-1 (1)	7.67	7.67	7.67	7.67	7.67	7.67	7.57	7.77
Aroclor-1268-2 (2)	7.74	7.74	7.74	7.74	7.74	7.74	7.64	7.84
Aroclor-1268-3 (3)	7.94	7.94	7.94	7.94	7.94	7.94	7.84	8.04
Aroclor-1268-4 (4)	8.23	8.23	8.23	8.23	8.23	8.23	8.13	8.33
Aroclor-1268-5 (5)	8.53	8.53	8.53	8.53	8.53	8.53	8.43	8.63



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

RETENTION TIMES OF INITIAL CALIBRATION

Decachlorobiphenyl	8.78	8.78	8.78	8.78	8.78	8.78	8.68	8.88	1
Tetrachloro-m-xylene	3.78	3.78	3.78	3.78	3.78	3.78	3.68	3.88	2

3
4
5
6
7
8
9
10
11
12
13
14
15
16
17
18
19
20



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

CALIBRATION FACTOR OF INITIAL CALIBRATION

Lab Name:	Alliance	Contract:	NOBI03	
Lab Code:	ACE	SDG NO.:	Q2639	
Instrument ID:	ECD_P	Calibration Date(s):	07/07/2025	07/08/2025
		Calibration Times:	21:03	04:24

GC Column: ZB-MR1 ID: 0.32 (mm)

LAB FILE ID:	CF 1000 =	CF 750 =	CF 500 =	CF 250 =	CF 050 =	CF	% RSD
	<u>PP073554.D</u>	<u>PP073555.D</u>	<u>PP073556.D</u>	<u>PP073557.D</u>	<u>PP073558.D</u>		
COMPOUND	CF 1000	CF 750	CF 500	CF 250	CF 050	CF	% RSD
Aroclor-1016-1 (1)	42452248	45617859	47138872	50511676	51847220	47513575	8
Aroclor-1016-2 (2)	66518124	70141979	72048808	76716636	70648900	71214889	5
Aroclor-1016-3 (3)	39961628	42046196	44162638	46389840	45755080	43663076	6
Aroclor-1016-4 (4)	33606097	35475740	36592056	38460728	35593260	35945576	5
Aroclor-1016-5 (5)	30910810	31971305	32786356	34274032	26709560	31330413	9
Aroclor-1260-1 (1)	55735594	57789364	59663732	63324028	58293500	58961244	5
Aroclor-1260-2 (2)	82256765	86873544	90393892	97973444	121701660	95839861	16
Aroclor-1260-3 (3)	71122512	73727981	74691298	76804056	69007300	73070629	4
Aroclor-1260-4 (4)	63951646	66011447	66730410	69035472	60770420	65299879	5
Aroclor-1260-5 (5)	147606205	151816095	154896322	160840336	139104740	150852740	5
Decachlorobiphenyl	1075002490	1114272707	1146110620	1163852360	956024000	1091052435	8
Tetrachloro-m-xylene	1314627420	1370591720	1413189460	1469047800	1280173600	1369526000	6
Aroclor-1242-1 (1)	37824570	38531545	40764028	42347748	31473220	38188222	11
Aroclor-1242-2 (2)	59433539	58987884	63134254	65007836	52846680	59882039	8
Aroclor-1242-3 (3)	35307728	35832168	38067086	39311740	34585840	36620912	5
Aroclor-1242-4 (4)	29431539	30211543	31738592	32275500	37022940	32136023	9
Aroclor-1242-5 (5)	31742412	31628361	33353228	35089048	31871320	32736874	5
Decachlorobiphenyl	1095703140	1117596867	1144519060	1154694600	992628000	1101028333	6
Tetrachloro-m-xylene	1336424670	1349665200	1427212360	1438929280	1262569400	1362960182	5
Aroclor-1248-1 (1)	29290065	30340729	31459936	34321104	28940820	30870531	7
Aroclor-1248-2 (2)	37625323	39736876	40535254	44074952	37644360	39923353	7
Aroclor-1248-3 (3)	43927993	45846956	46075290	48569104	37628800	44409629	9
Aroclor-1248-4 (4)	53376796	55925132	57147446	59774616	49178580	55080514	7
Aroclor-1248-5 (5)	51803368	53704276	55758942	57942584	49744040	53790642	6
Decachlorobiphenyl	1098016930	1133084880	1145143920	1172914800	889666400	1087765386	10
Tetrachloro-m-xylene	1321954420	1371326347	1415433040	1456874560	1240770200	1361271713	6
Aroclor-1254-1 (1)	50900598	53159759	55209204	57116384	51561700	53589529	5
Aroclor-1254-2 (2)	77237012	80519573	82538946	86348708	89800160	83288880	6
Aroclor-1254-3 (3)	83677544	86010903	88492372	92072040	91405580	88331688	4
Aroclor-1254-4 (4)	74438148	76222969	79592040	81854844	81227180	78667036	4
Aroclor-1254-5 (5)	71888659	74572743	74620102	76347748	70969780	73679806	3
Decachlorobiphenyl	1107439250	1132832533	1145288580	1145076280	1133429800	1132813289	1
Tetrachloro-m-xylene	1351624000	1395660893	1401155480	1465561640	1387618000	1400324003	3
Aroclor-1268-1 (1)	220572869	225132533	228083942	237689468	204639620	223223686	5



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

CALIBRATION FACTOR OF INITIAL CALIBRATION

Aroclor-1268-2	(2)	188785361	192061012	194228718	202923360	174527620	190505214	5
Aroclor-1268-3	(3)	161320167	164379476	166708106	175220108	160250740	165575719	4
Aroclor-1268-4	(4)	68937885	69804631	69558114	75087068	64331720	69543884	5
Aroclor-1268-5	(5)	477643268	472782711	485154758	497337016	371889540	460961459	11
Decachlorobiphenyl		1977874930	2021254947	2057047680	2189262080	1794844800	2008056887	7
Tetrachloro-m-xylene		1351774000	1390310400	1415817780	1495349000	1314096000	1393469436	5

1
2
3
4
5
6
7
8
9
10
11
12
13
14
15
16
17
18
19
20



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

CALIBRATION FACTOR OF INITIAL CALIBRATION

Lab Name:	Alliance	Contract:	NOBI03	
Lab Code:	ACE	SDG NO.:	Q2639	
Instrument ID:	ECD_P	Calibration Date(s):	07/07/2025	07/08/2025
		Calibration Times:	21:03	04:24

GC Column: ZB-MR2 ID: 0.32 (mm)

LAB FILE ID:	CF 1000 =	CF 750 =	CF 500 =	CF 250 =	CF 050 =	CF	% RSD
	<u>PP073554.D</u>	<u>PP073555.D</u>	<u>PP073556.D</u>	<u>PP073557.D</u>	<u>PP073558.D</u>		
COMPOUND	CF 1000	CF 750	CF 500	CF 250	CF 050	CF	% RSD
Aroclor-1016-1 (1)	63548895	66956692	68520980	73175628	68671440	68174727	5
Aroclor-1016-2 (2)	95987811	99810097	102589296	109872788	101161940	101884386	5
Aroclor-1016-3 (3)	50406684	53112144	54849034	57930668	54233060	54106318	5
Aroclor-1016-4 (4)	39688708	42104989	43896956	47040184	46673360	43880839	7
Aroclor-1016-5 (5)	50298801	53487816	55660288	59272232	54193420	54582511	6
Aroclor-1260-1 (1)	89335231	94510516	99471332	104207304	100277120	97560301	6
Aroclor-1260-2 (2)	113000947	118559808	124003550	129850992	128772620	122837583	6
Aroclor-1260-3 (3)	102918015	108414332	112293296	117668340	106025080	109463813	5
Aroclor-1260-4 (4)	82942909	90440599	92349274	96325208	84984160	89408430	6
Aroclor-1260-5 (5)	218347404	234684793	232225124	233707816	204717920	224736611	6
Decachlorobiphenyl	1288482360	1338938240	1324505420	1466524480	1197294400	1323148980	7
Tetrachloro-m-xylene	1774031450	1893159427	1873404460	1944042160	1726825000	1842292499	5
Aroclor-1242-1 (1)	53636877	56644489	60339480	62120840	56082120	57764761	6
Aroclor-1242-2 (2)	81745742	82323689	88927402	91756504	87517600	86454187	5
Aroclor-1242-3 (3)	43191003	44194741	47579930	48843488	45924140	45946660	5
Aroclor-1242-4 (4)	40719317	41867060	45117014	46860680	46752460	44263306	6
Aroclor-1242-5 (5)	53173633	53609452	57067394	58584716	53777140	55242467	4
Decachlorobiphenyl	1306642480	1369985587	1353011840	1407476720	1194819200	1326387165	6
Tetrachloro-m-xylene	1787240920	1786937067	1893455580	1997751320	1666197200	1826316417	7
Aroclor-1248-1 (1)	41993150	43590469	45185544	49843992	43861300	44894891	7
Aroclor-1248-2 (2)	55737799	58586344	61889020	66706936	64762540	61536528	7
Aroclor-1248-3 (3)	58429721	61323012	64407590	69469512	66692820	64064531	7
Aroclor-1248-4 (4)	68661033	72026459	75308372	81734520	79156680	75377413	7
Aroclor-1248-5 (5)	69725277	73210425	76423314	81696724	71898780	74590904	6
Decachlorobiphenyl	1298382400	1392805453	1360355620	1440840840	1158845800	1330246023	8
Tetrachloro-m-xylene	1855486030	1865559853	1910416600	1967065360	1674658000	1854637169	6
Aroclor-1254-1 (1)	105364555	111697468	112323806	121711620	129052960	116030082	8
Aroclor-1254-2 (2)	90612135	96205700	96079760	105129084	115091100	100623556	10
Aroclor-1254-3 (3)	142515413	152219476	152099148	162118636	163279600	154446455	6
Aroclor-1254-4 (4)	86996505	93901768	94351020	100389560	97157080	94559187	5
Aroclor-1254-5 (5)	123596587	131044949	130737444	141046724	140798600	133444861	6
Decachlorobiphenyl	1348192280	1398430560	1372338640	1507697520	1377457800	1400823360	4
Tetrachloro-m-xylene	1809940380	1949806187	1892015400	1932532480	1944382600	1905735409	3
Aroclor-1268-1 (1)	290584667	307587391	307795276	323603296	307313580	307376842	4



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

CALIBRATION FACTOR OF INITIAL CALIBRATION

Aroclor-1268-2	(2)	254148086	267727805	267575410	282961968	256026000	265687854	4
Aroclor-1268-3	(3)	211648098	225837245	227309934	242217372	220889640	225580458	5
Aroclor-1268-4	(4)	89640321	95098047	95218176	99881904	85000720	92967834	6
Aroclor-1268-5	(5)	595257746	637650785	622434144	650778188	576631820	616550537	5
Decachlorobiphenyl		2396229270	2556860227	2535017940	2683507840	2355689000	2505460855	5
Tetrachloro-m-xylene		1866286350	1953909840	1937791560	2021719520	1790813600	1914104174	5

1
2
3
4
5
6
7
8
9
10
11
12
13
14
15
16
17
18
19
20



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

INITIAL CALIBRATION OF MULTICOMPONENT ANALYTES

Lab Name:	<u>Alliance</u>	Contract:	<u>NOBI03</u>
Lab Code:	<u>ACE</u>	SDG NO.:	<u>Q2639</u>
Instrument ID:	<u>ECD_P</u>	Date(s) Analyzed:	<u>07/07/2025</u> <u>07/08/2025</u>
GC Column:	<u>ZB-MR1</u>	ID:	<u>0.32</u> (mm)

COMPOUND	AMOUNT (ng)	PEAK	RT	RT WINDOW		CALIBRATION FACTOR
				FROM	TO	
Aroclor-1221	500	1	4.69	4.59	4.79	17866400
		2	4.78	4.68	4.88	13504500
		3	4.85	4.75	4.95	41604800
		4	0.00			0
		5	0.00			0
Aroclor-1232	500	1	4.85	4.75	4.95	32650800
		2	5.37	5.27	5.47	16254700
		3	5.66	5.56	5.76	32993400
		4	5.82	5.72	5.92	16445200
		5	5.91	5.81	6.01	10570400
Aroclor-1262	500	1	8.07	7.97	8.17	87027200
		2	8.38	8.28	8.48	198028000
		3	8.70	8.60	8.80	125725000
		4	8.78	8.68	8.88	93262800
		5	9.43	9.33	9.53	63389400



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

INITIAL CALIBRATION OF MULTICOMPONENT ANALYTES

Lab Name:	<u>Alliance</u>	Contract:	<u>NOBI03</u>
Lab Code:	<u>ACE</u>	SDG NO.:	<u>Q2639</u>
Instrument ID:	<u>ECD_P</u>	Date(s) Analyzed:	<u>07/07/2025</u> <u>07/08/2025</u>
GC Column:	<u>ZB-MR2</u>	ID:	<u>0.32</u> (mm)

COMPOUND	AMOUNT (ng)	PEAK	RT	RT WINDOW		CALIBRATION FACTOR
				FROM	TO	
Aroclor-1221	500	1	3.99	3.89	4.09	27045000
		2	4.08	3.98	4.18	20360400
		3	4.15	4.05	4.25	61448600
		4	0.00			0
		5	0.00			0
Aroclor-1232	500	1	4.15	4.05	4.25	46614400
		2	4.88	4.78	4.98	47659800
		3	5.05	4.95	5.15	25029000
		4	5.14	5.04	5.24	21656200
		5	5.31	5.21	5.41	22563400
Aroclor-1262	500	1	6.89	6.79	6.99	147692000
		2	7.15	7.05	7.25	127829000
		3	7.67	7.57	7.77	114019000
		4	7.74	7.64	7.84	184049000
		5	8.23	8.13	8.33	84435600

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP070825\
 Data File : PP073554.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Jul 2025 21:03
 Operator : YP\AJ
 Sample : AR1660ICC1000
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
AR1660ICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 08 01:39:10 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 08 01:37:59 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	4.486	3.781	131.5E6	177.4E6	93.026	94.696
2) SA Decachlor...	10.176	8.782	107.5E6	128.8E6	93.796	97.280

Target Compounds

3) L1 AR-1016-1	5.637	4.858	42452248	63548895	900.578	927.437
4) L1 AR-1016-2	5.658	4.876	66518124	95987811	923.237	935.651
5) L1 AR-1016-3	5.720	5.053	39961628	50406684	904.874	919.008
6) L1 AR-1016-4	5.818	5.095	33606097	39688708	918.399	904.134
7) L1 AR-1016-5	6.111	5.308	30910810	50298801	942.795	903.675
31) L7 AR-1260-1	7.227	6.338	55735594	89335231	934.162	898.100
32) L7 AR-1260-2	7.481	6.527	82256765	113.0E6	909.981	911.272
33) L7 AR-1260-3	7.838	6.679	71122512	102.9E6	952.220	916.511
34) L7 AR-1260-4	8.063	7.148	63951646	82942909	958.358	898.144
35) L7 AR-1260-5	8.381	7.390	147.6E6	218.3E6	952.936	940.240



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP070825\
 Data File : PP073554.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Jul 2025 21:03
 Operator : YP\AJ
 Sample : AR1660ICC1000
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
AR1660ICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 08 01:39:10 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 08 01:37:59 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

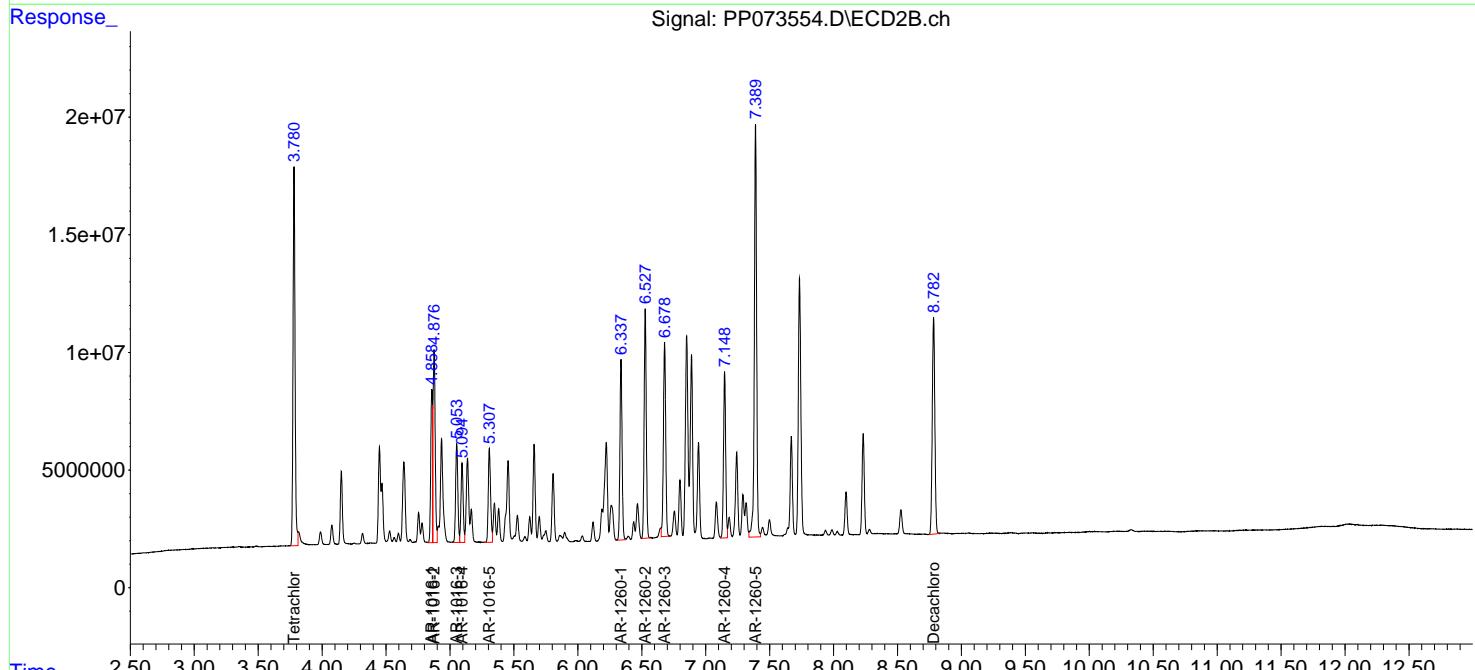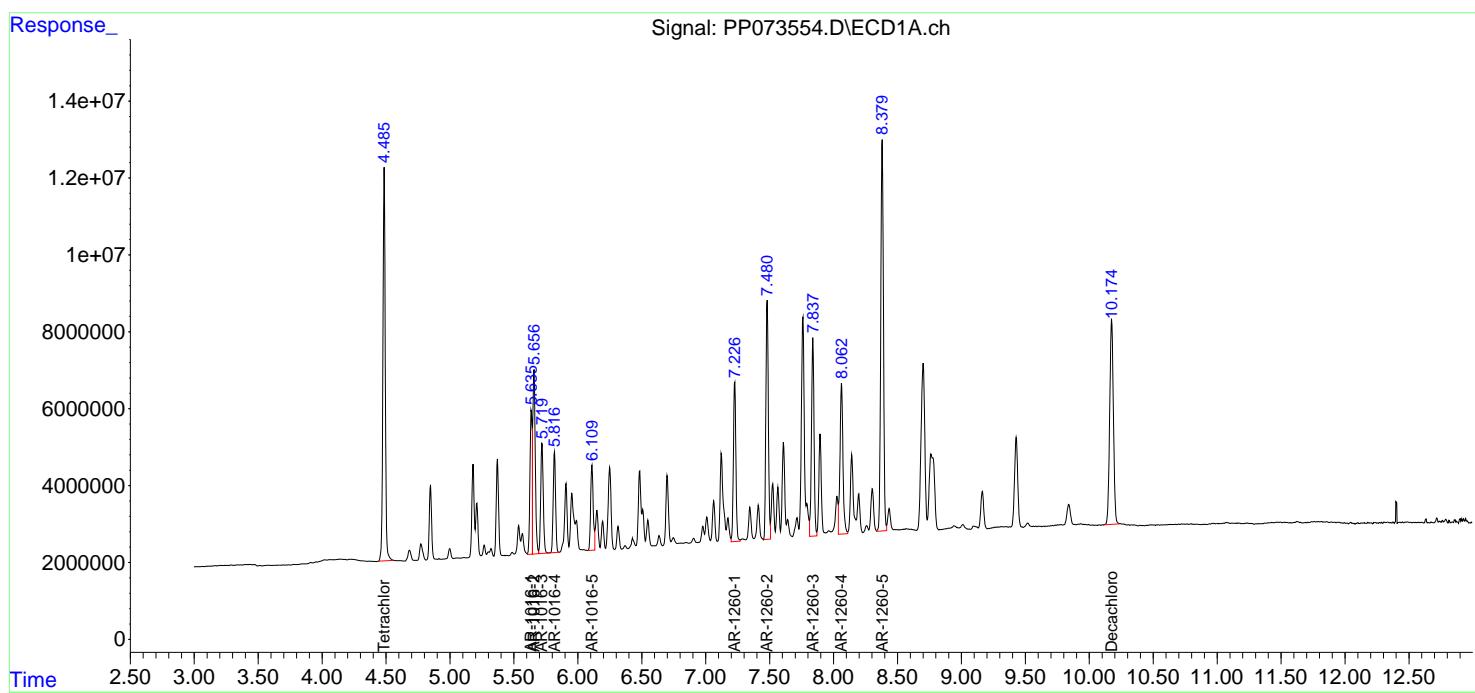

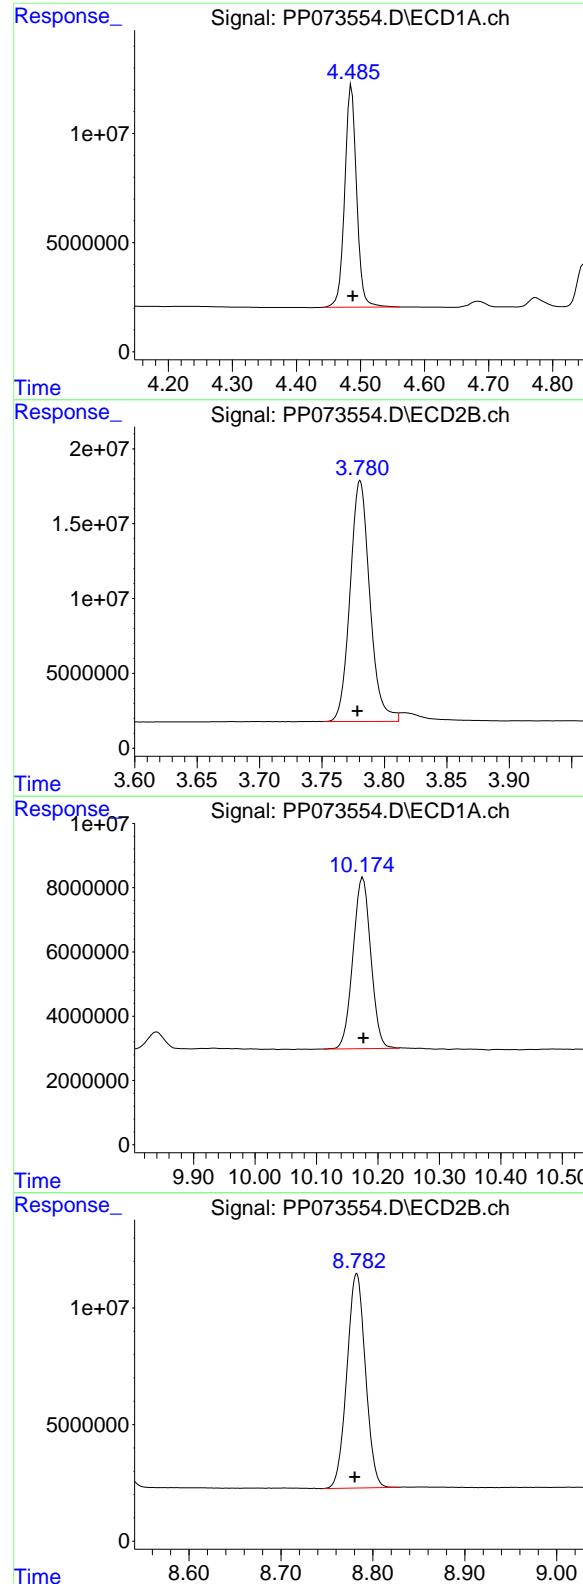

#1 Tetrachloro-m-xylene

R.T.: 4.486 min
 Delta R.T.: -0.002 min
 Response: 131462742
 Conc: 93.03 ng/ml

Instrument: ECD_P
 ClientSampleId: AR1660ICC1000

#1 Tetrachloro-m-xylene

R.T.: 3.781 min
 Delta R.T.: 0.002 min
 Response: 177403145
 Conc: 94.70 ng/ml

#2 Decachlorobiphenyl

R.T.: 10.176 min
 Delta R.T.: 0.000 min
 Response: 107500249
 Conc: 93.80 ng/ml


#2 Decachlorobiphenyl

R.T.: 8.782 min
 Delta R.T.: 0.002 min
 Response: 128848236
 Conc: 97.28 ng/ml

#3 AR-1016-1


R.T.: 5.637 min
 Delta R.T.: -0.002 min
 Response: 42452248
 Conc: 900.58 ng/ml

Instrument: ECD_P
ClientSampleId: AR1660ICC1000

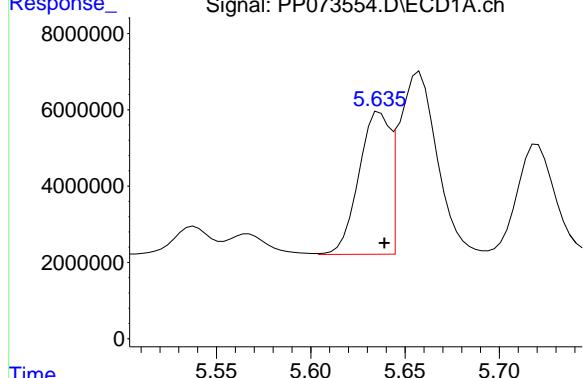


#3 AR-1016-1

R.T.: 4.858 min
 Delta R.T.: 0.000 min
 Response: 63548895
 Conc: 927.44 ng/ml

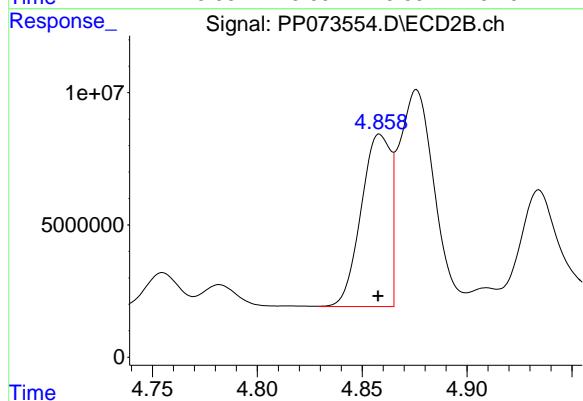


#4 AR-1016-2

R.T.: 5.658 min
 Delta R.T.: -0.003 min
 Response: 66518124
 Conc: 923.24 ng/ml

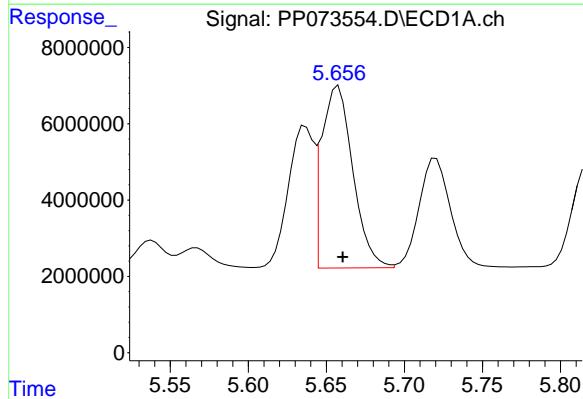

#4 AR-1016-2


R.T.: 4.876 min
 Delta R.T.: 0.000 min
 Response: 95987811
 Conc: 935.65 ng/ml

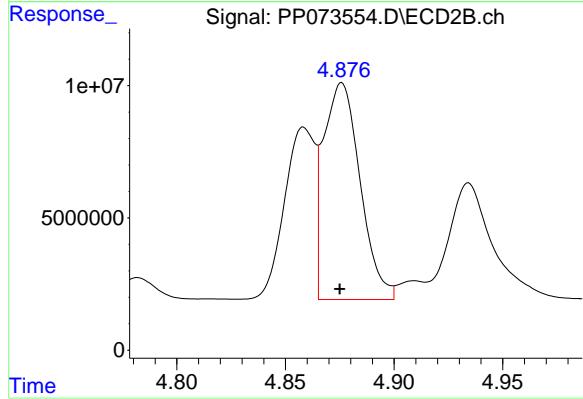

#5 AR-1016-3


R.T.: 5.720 min
 Delta R.T.: -0.002 min
 Response: 39961628
 Conc: 904.87 ng/ml

Instrument: ECD_P
 ClientSampleId: AR1660ICC1000

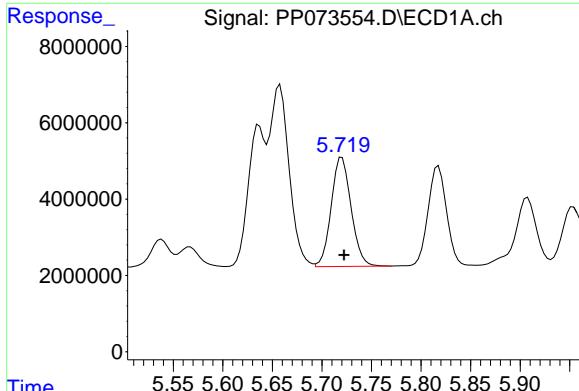


#5 AR-1016-3

R.T.: 5.053 min
 Delta R.T.: 0.001 min
 Response: 50406684
 Conc: 919.01 ng/ml

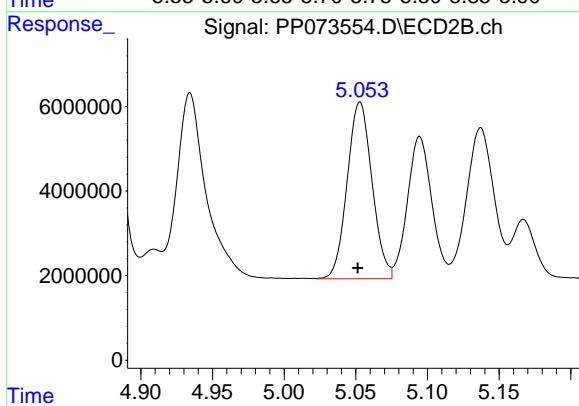


#6 AR-1016-4


R.T.: 5.818 min
 Delta R.T.: -0.003 min
 Response: 33606097
 Conc: 918.40 ng/ml

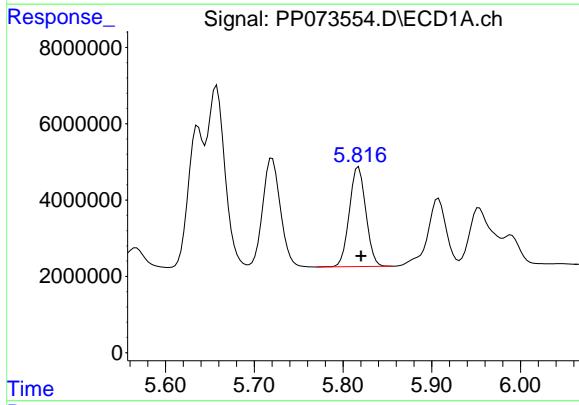

#6 AR-1016-4

R.T.: 5.095 min
 Delta R.T.: 0.001 min
 Response: 39688708
 Conc: 904.13 ng/ml

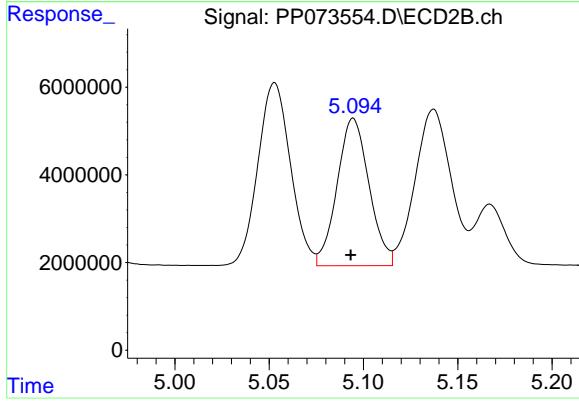

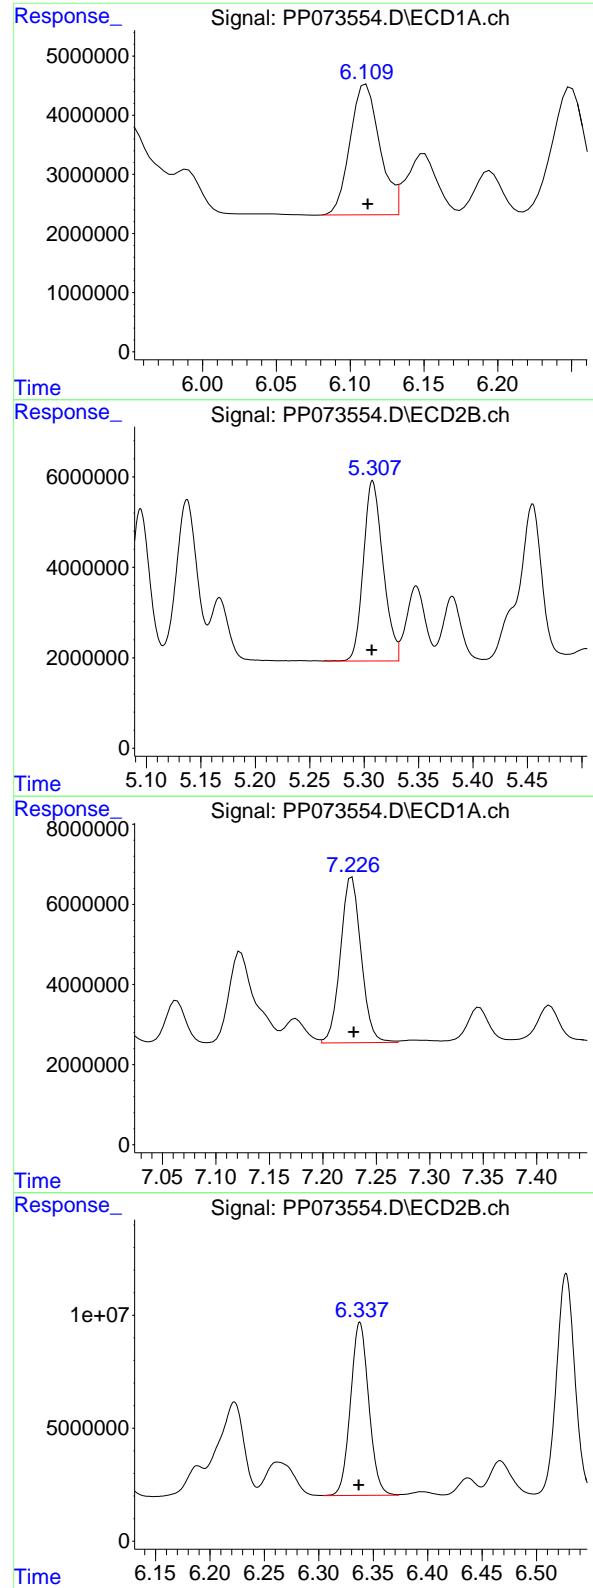

#7 AR-1016-5

R.T.: 6.111 min
 Delta R.T.: -0.001 min
 Response: 30910810
 Conc: 942.79 ng/ml

Instrument: ECD_P
 ClientSampleId: AR1660ICC1000

#7 AR-1016-5

R.T.: 5.308 min
 Delta R.T.: 0.000 min
 Response: 50298801
 Conc: 903.67 ng/ml

#31 AR-1260-1

R.T.: 7.227 min
 Delta R.T.: -0.002 min
 Response: 55735594
 Conc: 934.16 ng/ml





#31 AR-1260-1

R.T.: 6.338 min
 Delta R.T.: 0.001 min
 Response: 89335231
 Conc: 898.10 ng/ml

#32 AR-1260-2

R.T.: 7.481 min
 Delta R.T.: -0.002 min
 Response: 82256765
 Conc: 909.98 ng/ml

Instrument: ECD_P
ClientSampleId: AR1660ICC1000

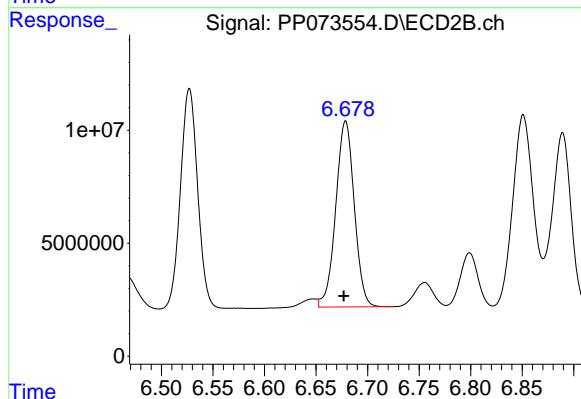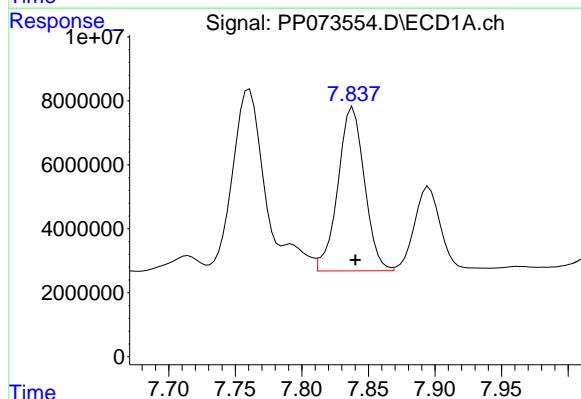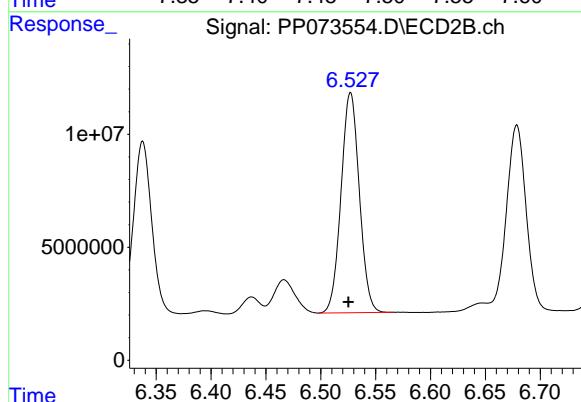

#32 AR-1260-2

R.T.: 6.527 min
 Delta R.T.: 0.002 min
 Response: 113000947
 Conc: 911.27 ng/ml

#33 AR-1260-3

R.T.: 7.838 min
 Delta R.T.: -0.002 min
 Response: 71122512
 Conc: 952.22 ng/ml





#33 AR-1260-3

R.T.: 6.679 min
 Delta R.T.: 0.002 min
 Response: 102918015
 Conc: 916.51 ng/ml

#34 AR-1260-4

R.T.: 8.063 min
 Delta R.T.: -0.001 min
 Response: 63951646
 Conc: 958.36 ng/ml

Instrument: ECD_P
ClientSampleId: AR1660ICC1000

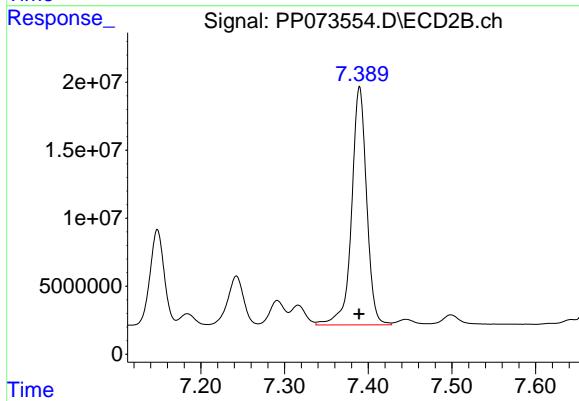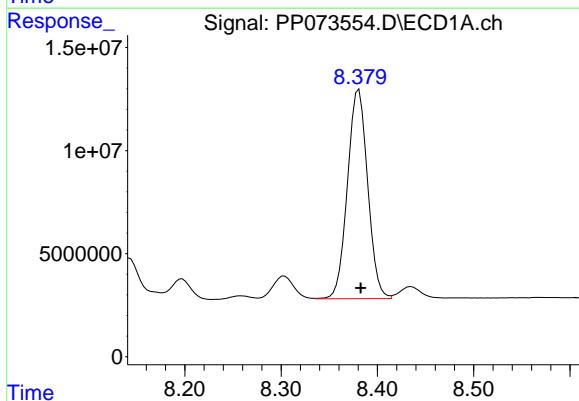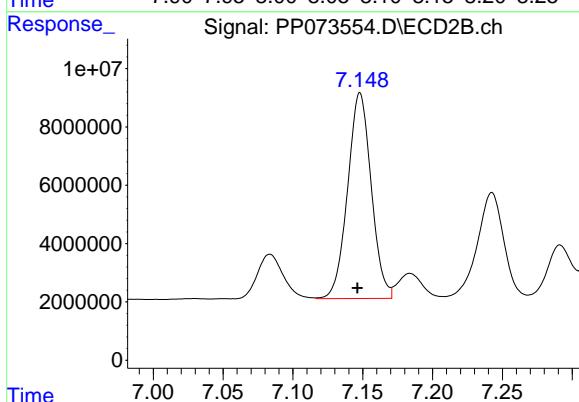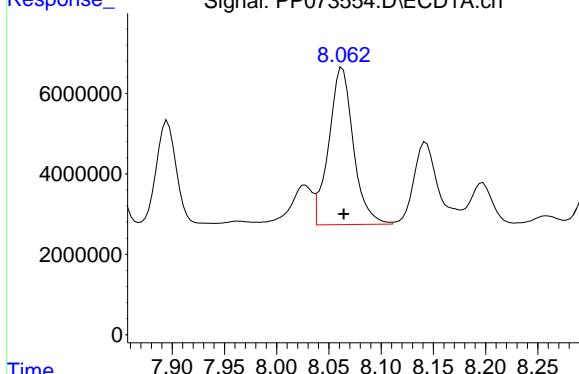

#34 AR-1260-4

R.T.: 7.148 min
 Delta R.T.: 0.002 min
 Response: 82942909
 Conc: 898.14 ng/ml

#35 AR-1260-5

R.T.: 8.381 min
 Delta R.T.: -0.002 min
 Response: 147606205
 Conc: 952.94 ng/ml

#35 AR-1260-5

R.T.: 7.390 min
 Delta R.T.: 0.000 min
 Response: 218347404
 Conc: 940.24 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP070825\
 Data File : PP073555.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Jul 2025 21:19
 Operator : YP\AJ
 Sample : AR1660ICC750
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
AR1660ICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 08 01:39:38 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 08 01:37:59 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	4.488	3.780	102.8E6	142.0E6	72.739	75.791
2) SA Decachlor...	10.177	8.781	83570453	100.4E6	72.917	75.817

Target Compounds

3) L1 AR-1016-1	5.639	4.859	34213394	50217519	725.800	732.878
4) L1 AR-1016-2	5.661	4.876	52606484	74857573	730.151	729.682
5) L1 AR-1016-3	5.722	5.052	31534647	39834108	714.057	726.250
6) L1 AR-1016-4	5.820	5.095	26606805	31578742	727.120	719.383
7) L1 AR-1016-5	6.112	5.308	23978479	40115862	731.355	720.727
31) L7 AR-1260-1	7.230	6.338	43342023	70882887	726.438	712.596
32) L7 AR-1260-2	7.483	6.527	65155158	88919856	720.792	717.075
33) L7 AR-1260-3	7.841	6.678	55295986	81310749	740.327	724.093
34) L7 AR-1260-4	8.065	7.148	49508585	67830449	741.919	734.499
35) L7 AR-1260-5	8.383	7.390	113.9E6	176.0E6	735.086	757.944



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.





Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP070825\
 Data File : PP073555.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Jul 2025 21:19
 Operator : YP\AJ
 Sample : AR1660ICC750
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
AR1660ICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 08 01:39:38 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 08 01:37:59 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

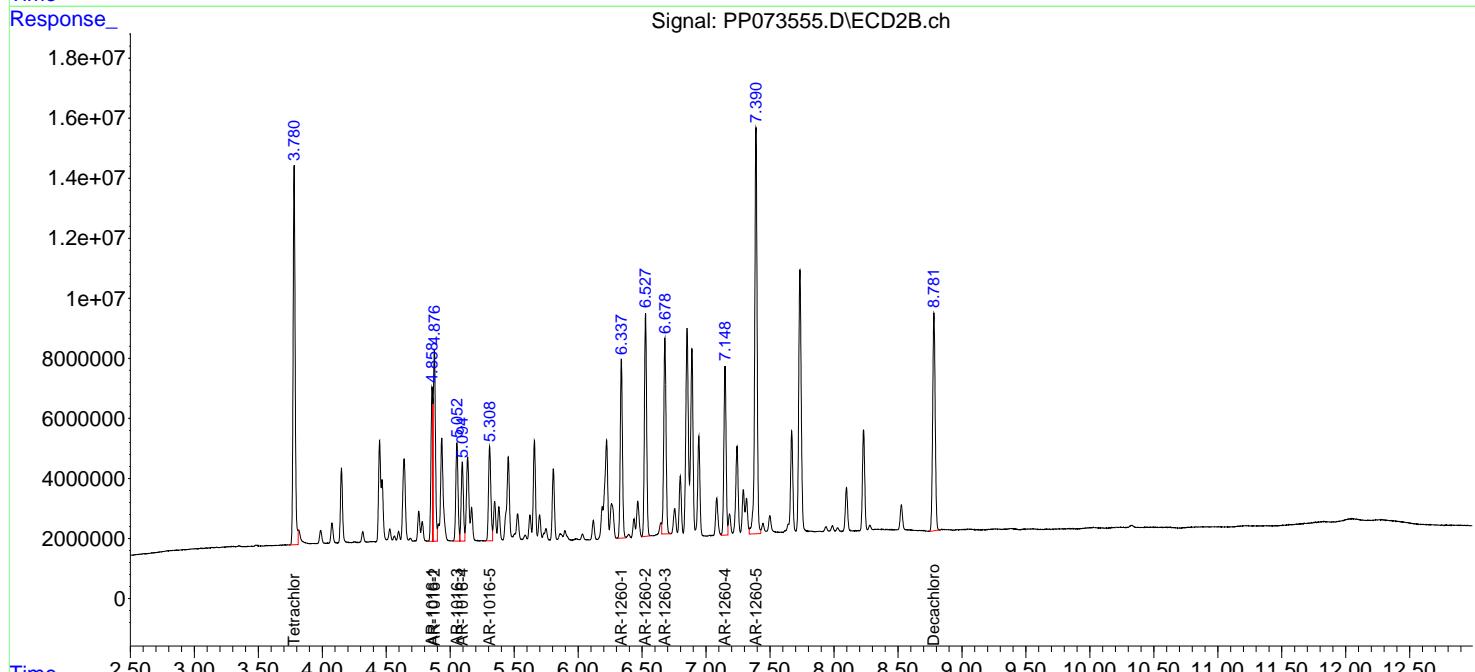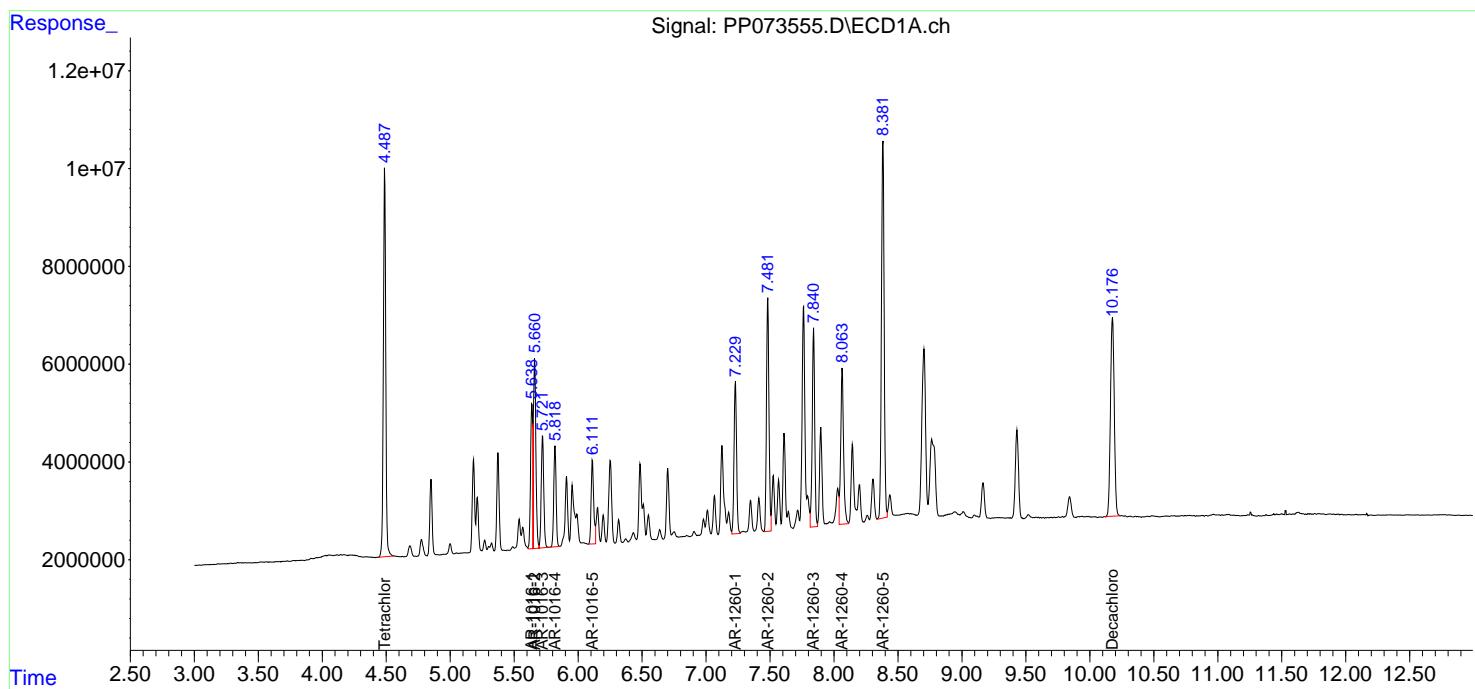

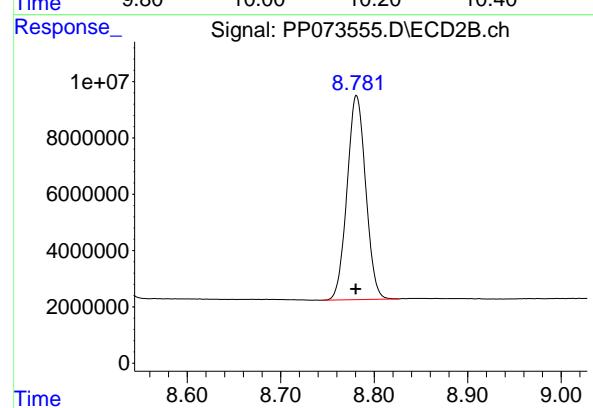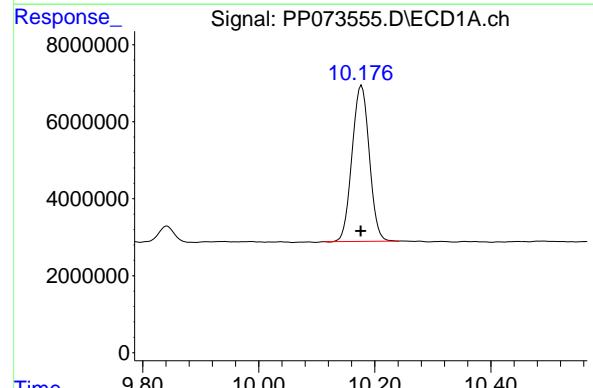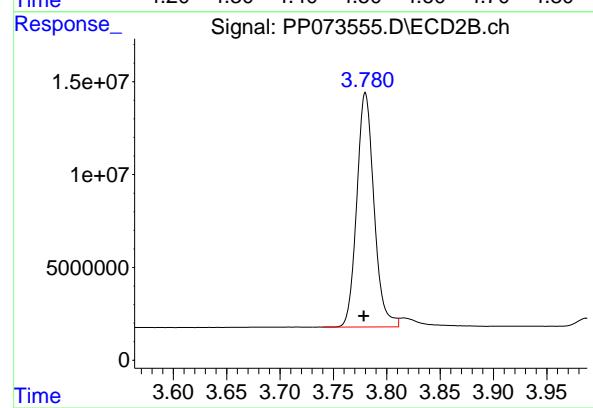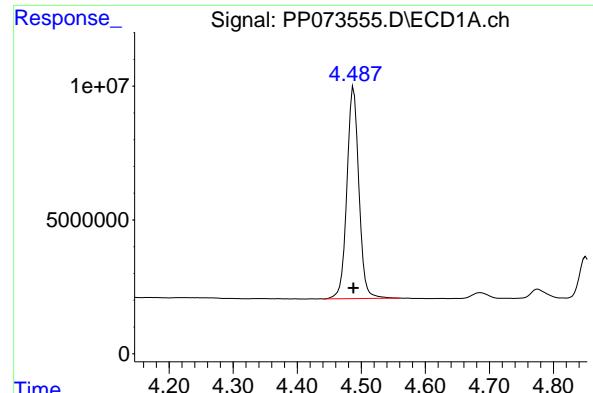

#1 Tetrachloro-m-xylene

R.T.: 4.488 min
Delta R.T.: 0.000 min
Response: 102794379
Conc: 72.74 ng/ml

Instrument: ECD_P
ClientSampleId: AR1660ICC750

#1 Tetrachloro-m-xylene





R.T.: 3.780 min
Delta R.T.: 0.002 min
Response: 141986957
Conc: 75.79 ng/ml

#2 Decachlorobiphenyl

R.T.: 10.177 min
Delta R.T.: 0.001 min
Response: 83570453
Conc: 72.92 ng/ml

#2 Decachlorobiphenyl

R.T.: 8.781 min
Delta R.T.: 0.000 min
Response: 100420368
Conc: 75.82 ng/ml

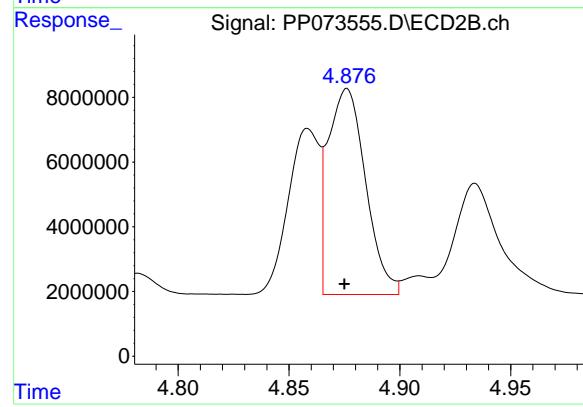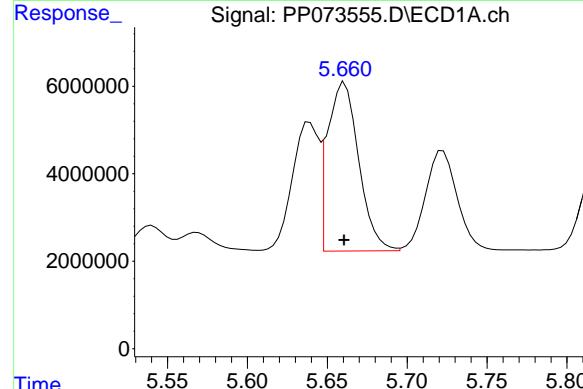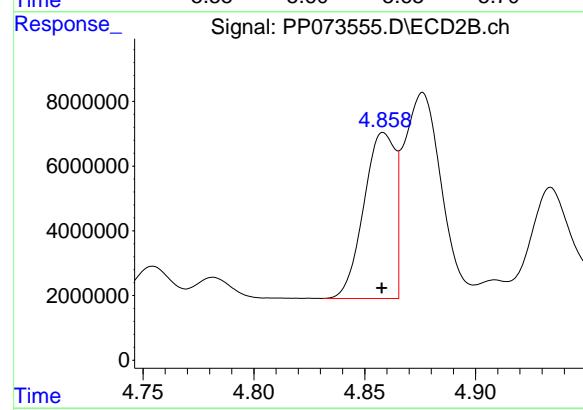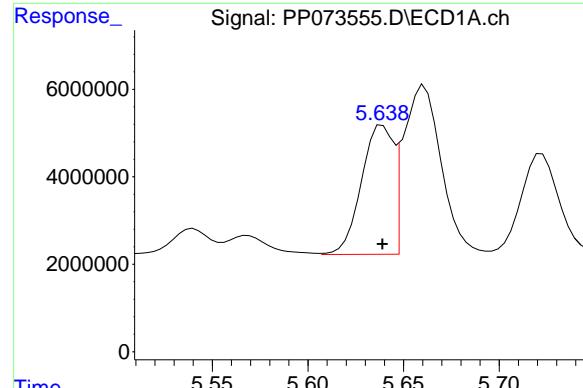

#3 AR-1016-1

R.T.: 5.639 min
 Delta R.T.: 0.000 min
 Response: 34213394
 Conc: 725.80 ng/ml

Instrument: ECD_P
 ClientSampleId: AR1660ICC750

#3 AR-1016-1

R.T.: 4.859 min
 Delta R.T.: 0.000 min
 Response: 50217519
 Conc: 732.88 ng/ml

#4 AR-1016-2

R.T.: 5.661 min
 Delta R.T.: 0.000 min
 Response: 52606484
 Conc: 730.15 ng/ml





#4 AR-1016-2

R.T.: 4.876 min
 Delta R.T.: 0.001 min
 Response: 74857573
 Conc: 729.68 ng/ml

#5 AR-1016-3

R.T.: 5.722 min
 Delta R.T.: 0.000 min
 Response: 31534647
 Conc: 714.06 ng/ml

Instrument: ECD_P
ClientSampleId: AR1660ICC750

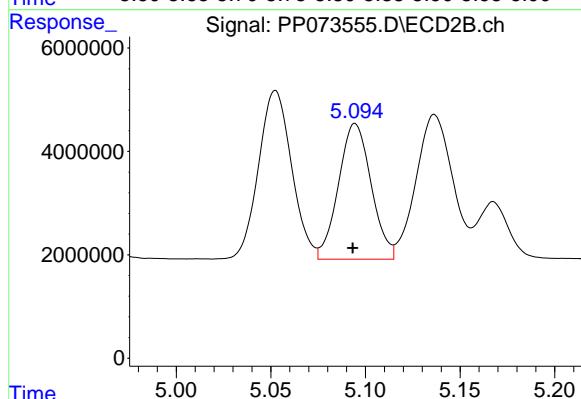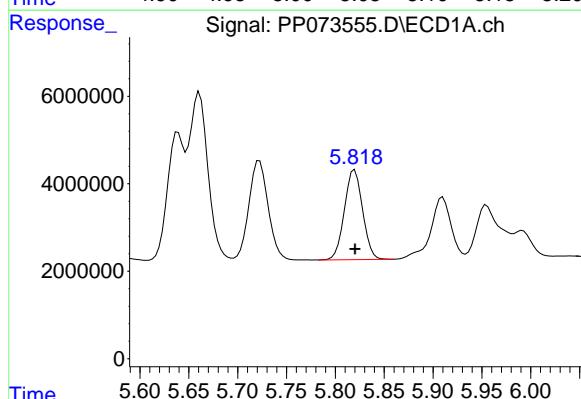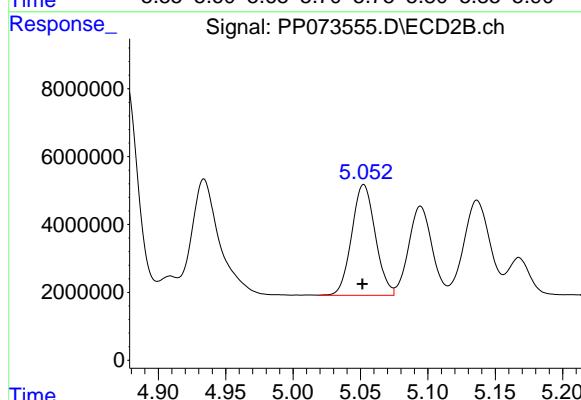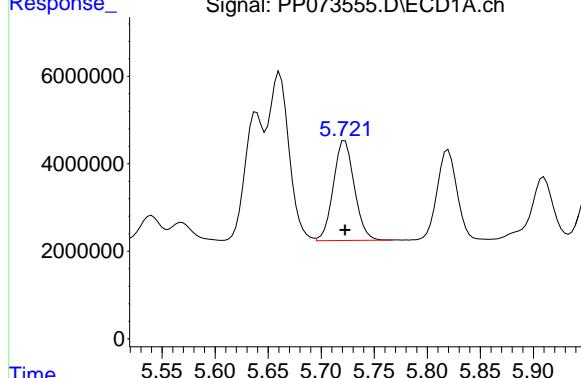

#5 AR-1016-3


R.T.: 5.052 min
 Delta R.T.: 0.000 min
 Response: 39834108
 Conc: 726.25 ng/ml

#6 AR-1016-4

R.T.: 5.820 min
 Delta R.T.: 0.000 min
 Response: 26606805
 Conc: 727.12 ng/ml

#6 AR-1016-4

R.T.: 5.095 min
 Delta R.T.: 0.001 min
 Response: 31578742
 Conc: 719.38 ng/ml

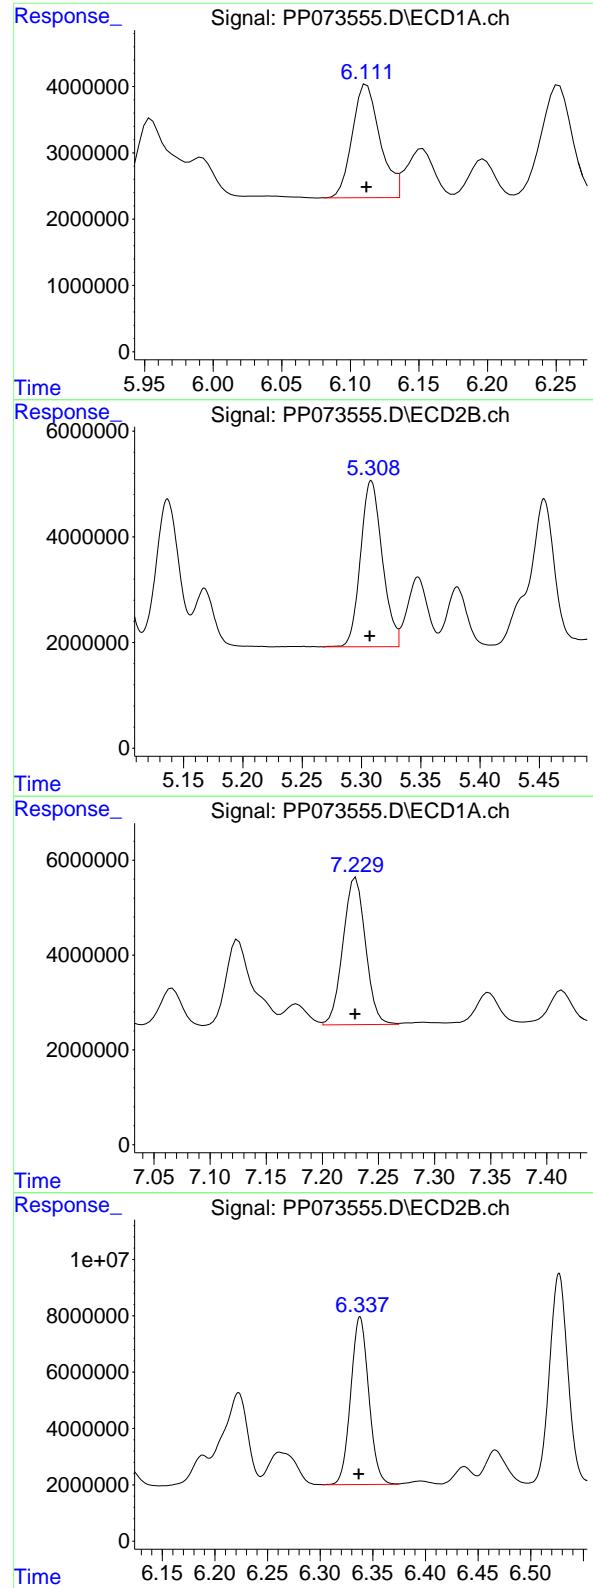

#7 AR-1016-5

R.T.: 6.112 min
 Delta R.T.: 0.000 min
 Response: 23978479
 Conc: 731.36 ng/ml

Instrument: ECD_P
 ClientSampleId: AR1660ICC750

#7 AR-1016-5

R.T.: 5.308 min
 Delta R.T.: 0.001 min
 Response: 40115862
 Conc: 720.73 ng/ml

#31 AR-1260-1

R.T.: 7.230 min
 Delta R.T.: 0.000 min
 Response: 43342023
 Conc: 726.44 ng/ml





#31 AR-1260-1

R.T.: 6.338 min
 Delta R.T.: 0.001 min
 Response: 70882887
 Conc: 712.60 ng/ml

#32 AR-1260-2

R.T.: 7.483 min
 Delta R.T.: 0.000 min
 Response: 65155158
 Conc: 720.79 ng/ml

Instrument: ECD_P
ClientSampleId: AR1660ICC750

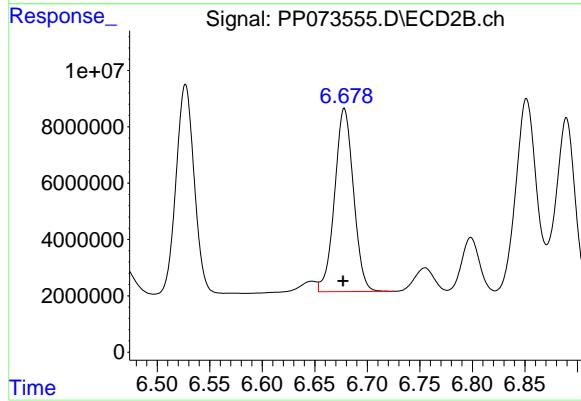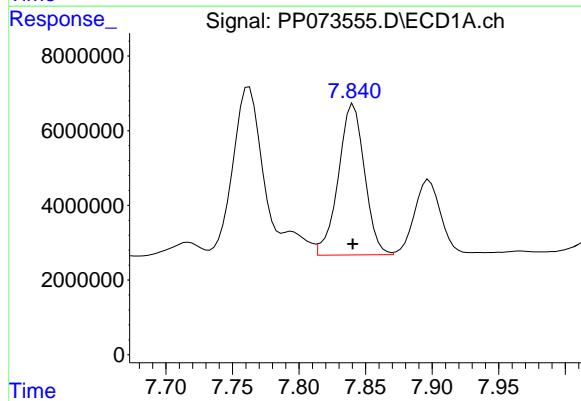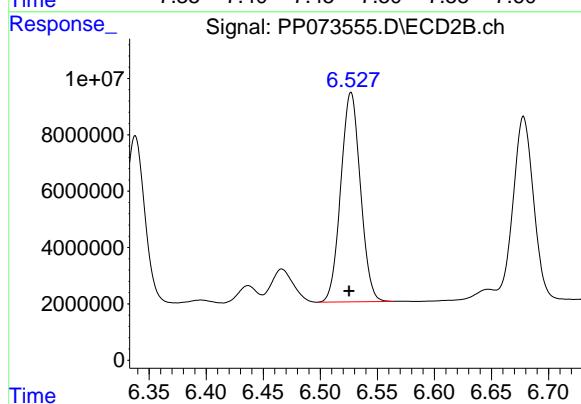

#32 AR-1260-2

R.T.: 6.527 min
 Delta R.T.: 0.002 min
 Response: 88919856
 Conc: 717.08 ng/ml

#33 AR-1260-3

R.T.: 7.841 min
 Delta R.T.: 0.000 min
 Response: 55295986
 Conc: 740.33 ng/ml





#33 AR-1260-3

R.T.: 6.678 min
 Delta R.T.: 0.001 min
 Response: 81310749
 Conc: 724.09 ng/ml

#34 AR-1260-4

R.T.: 8.065 min
 Delta R.T.: 0.000 min
 Response: 49508585
 Conc: 741.92 ng/ml

Instrument: ECD_P
ClientSampleId: AR1660ICC750

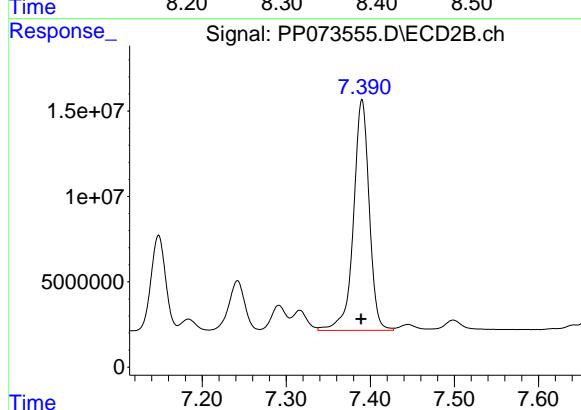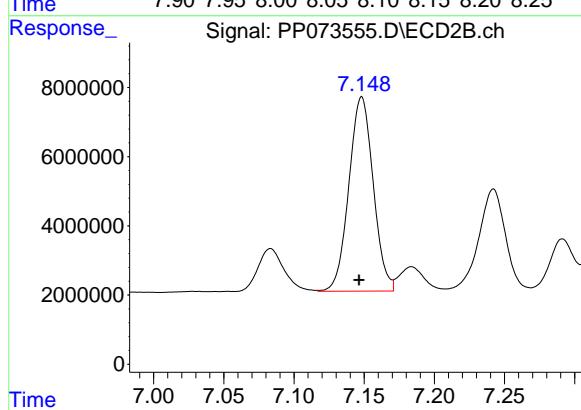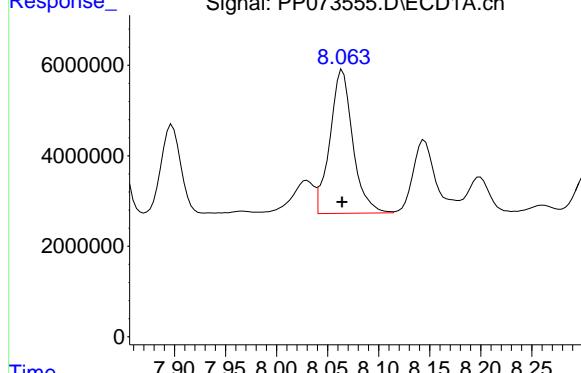

#34 AR-1260-4

R.T.: 7.148 min
 Delta R.T.: 0.002 min
 Response: 67830449
 Conc: 734.50 ng/ml

#35 AR-1260-5

R.T.: 8.383 min
 Delta R.T.: 0.000 min
 Response: 113862071
 Conc: 735.09 ng/ml

#35 AR-1260-5

R.T.: 7.390 min
 Delta R.T.: 0.001 min
 Response: 176013595
 Conc: 757.94 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP070825\
 Data File : PP073556.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Jul 2025 21:35
 Operator : YP\AJ
 Sample : AR1660ICC500
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
AR1660ICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 08 01:40:01 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 08 01:37:59 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	4.488	3.778	70659473	93670223	50.000	50.000
2) SA Decachlor...	10.176	8.780	57305531	66225271	50.000	50.000

Target Compounds

3) L1 AR-1016-1	5.639	4.858	23569436	34260490	500.000	500.000
4) L1 AR-1016-2	5.660	4.875	36024404	51294648	500.000	500.000
5) L1 AR-1016-3	5.722	5.051	22081319	27424517	500.000	500.000
6) L1 AR-1016-4	5.820	5.093	18296028	21948478	500.000	500.000
7) L1 AR-1016-5	6.112	5.307	16393178	27830144	500.000	500.000
31) L7 AR-1260-1	7.229	6.337	29831866	49735666	500.000	500.000
32) L7 AR-1260-2	7.483	6.525	45196946	62001775	500.000	500.000
33) L7 AR-1260-3	7.840	6.677	37345649	56146648	500.000	500.000
34) L7 AR-1260-4	8.064	7.146	33365205	46174637	500.000	500.000
35) L7 AR-1260-5	8.383	7.389	77448161	116.1E6	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.





Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP070825\
Data File : PP073556.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Jul 2025 21:35
Operator : YP\AJ
Sample : AR1660ICC500
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
AR1660ICC500

```
Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 08 01:40:01 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070825.M
Quant Title  : GC EXTRACTABLES
QLast Update : Tue Jul 08 01:37:59 2025
Response via : Initial Calibration
Integrator: ChemStation
```

Volume Inj. : 2 μ l
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

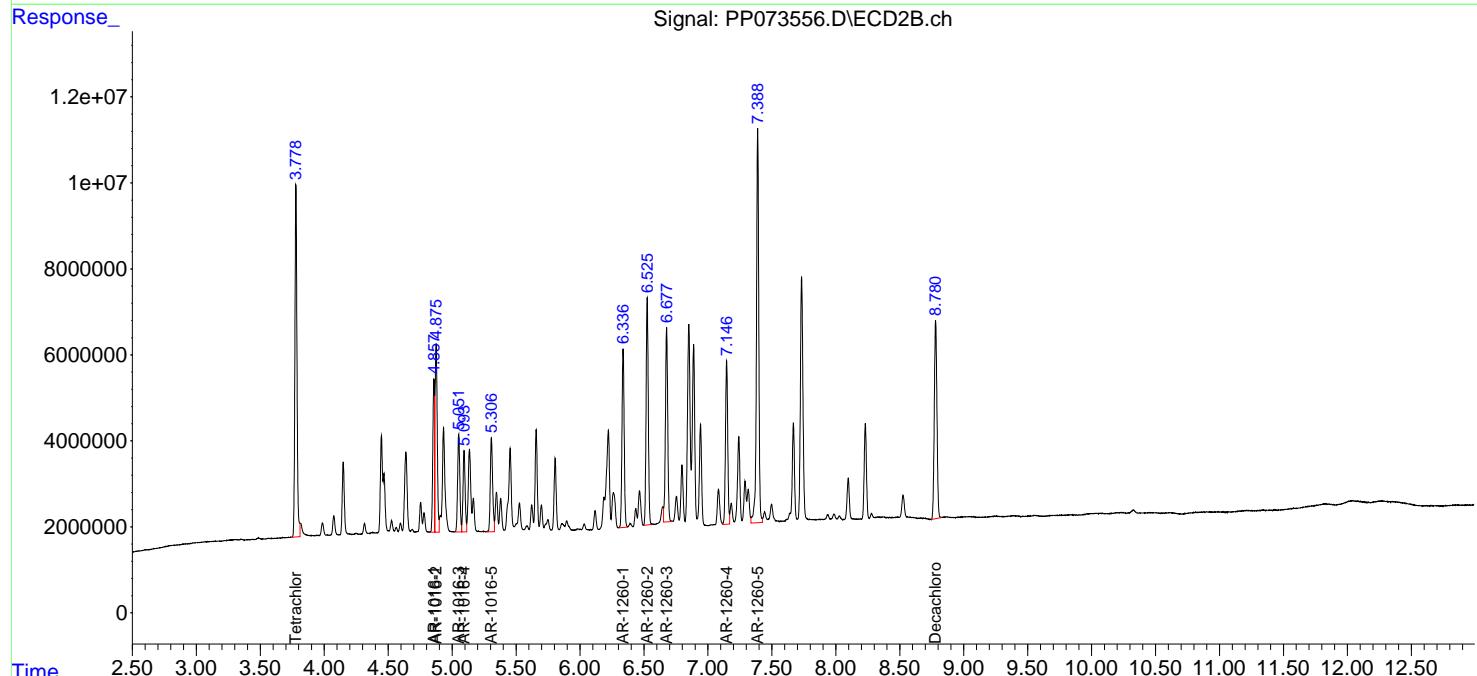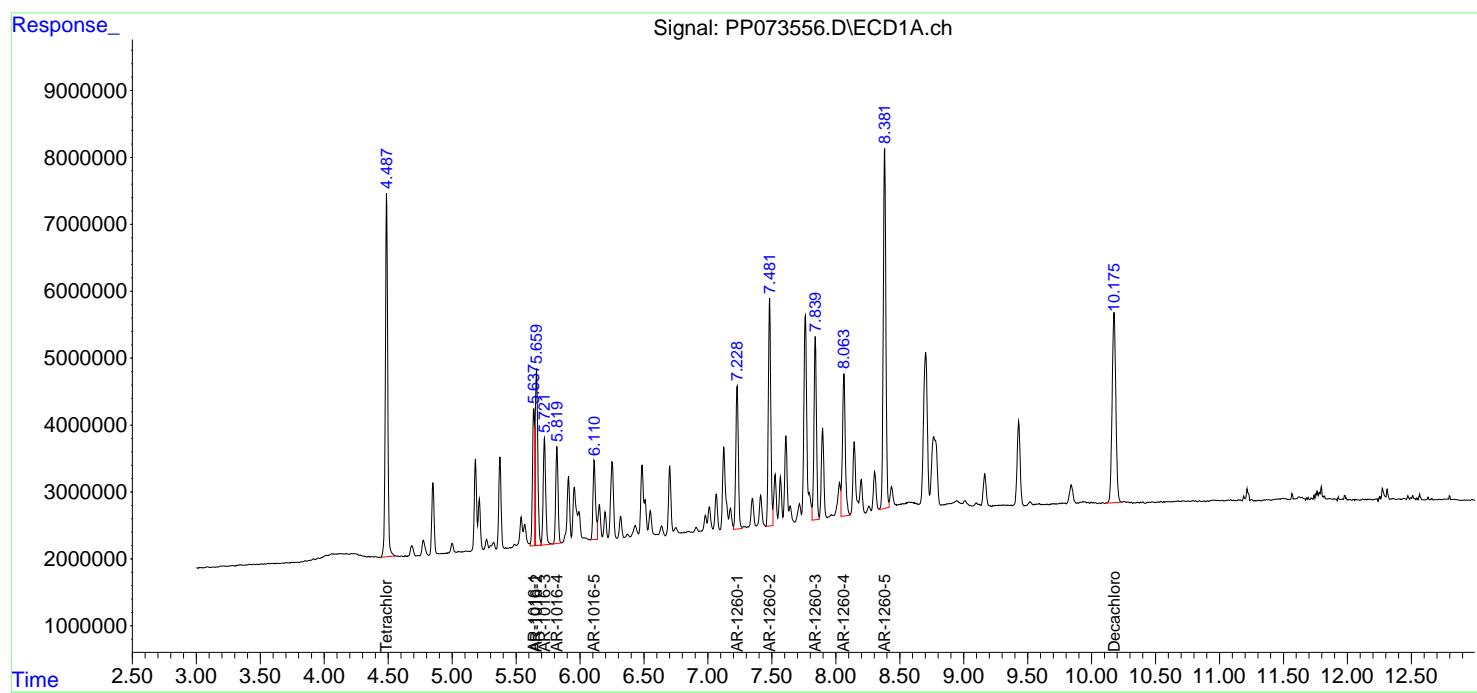

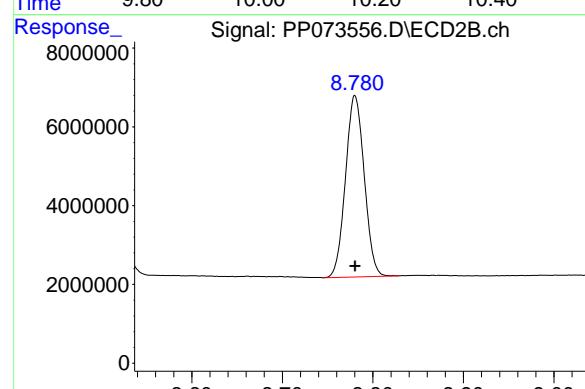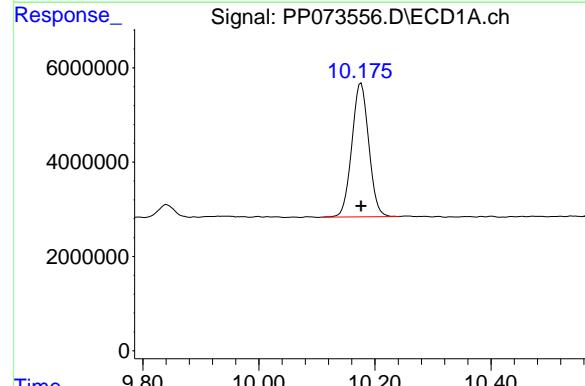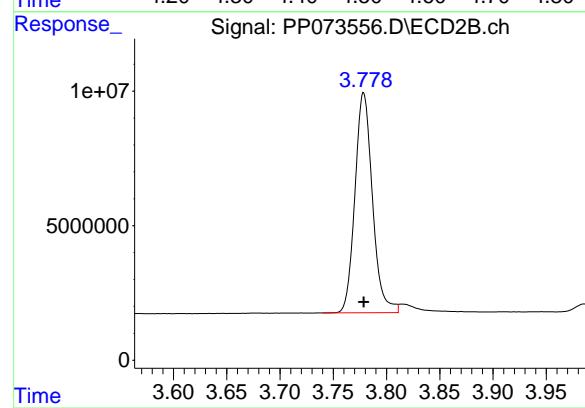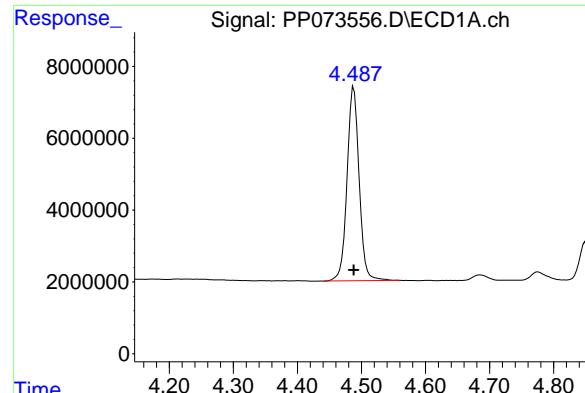

#1 Tetrachloro-m-xylene

R.T.: 4.488 min
 Delta R.T.: 0.000 min
 Response: 70659473
 Conc: 50.00 ng/ml

Instrument: ECD_P
ClientSampleId: AR1660ICC500

#1 Tetrachloro-m-xylene

R.T.: 3.778 min
 Delta R.T.: 0.000 min
 Response: 93670223
 Conc: 50.00 ng/ml

#2 Decachlorobiphenyl

R.T.: 10.176 min
 Delta R.T.: 0.000 min
 Response: 57305531
 Conc: 50.00 ng/ml


#2 Decachlorobiphenyl

R.T.: 8.780 min
 Delta R.T.: 0.000 min
 Response: 66225271
 Conc: 50.00 ng/ml

#3 AR-1016-1


R.T.: 5.639 min
 Delta R.T.: 0.000 min
 Response: 23569436
 Conc: 500.00 ng/ml

Instrument: ECD_P
ClientSampleId: AR1660ICC500




#3 AR-1016-1

R.T.: 4.858 min
 Delta R.T.: 0.000 min
 Response: 34260490
 Conc: 500.00 ng/ml

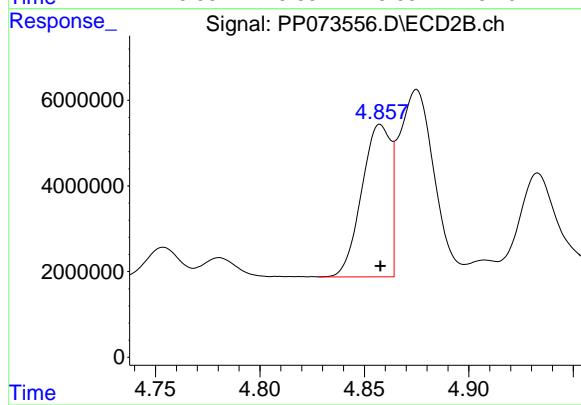


#4 AR-1016-2

R.T.: 5.660 min
 Delta R.T.: 0.000 min
 Response: 36024404
 Conc: 500.00 ng/ml

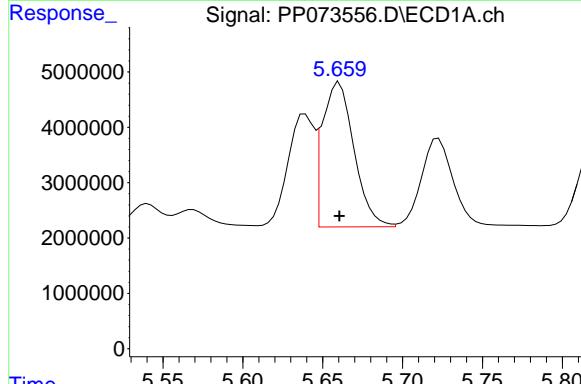

#4 AR-1016-2


R.T.: 4.875 min
 Delta R.T.: 0.000 min
 Response: 51294648
 Conc: 500.00 ng/ml

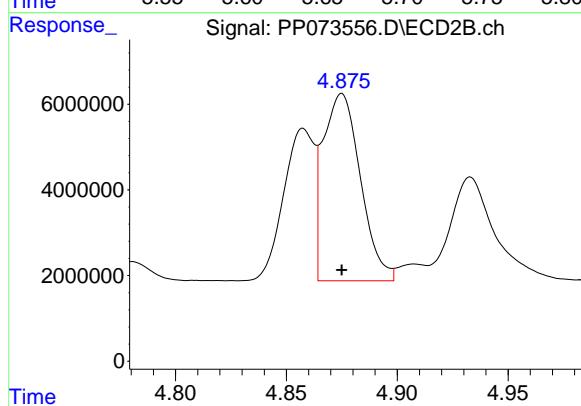

#5 AR-1016-3


R.T.: 5.722 min
 Delta R.T.: 0.000 min
 Response: 22081319
 Conc: 500.00 ng/ml

Instrument: ECD_P
ClientSampleId: AR1660ICC500

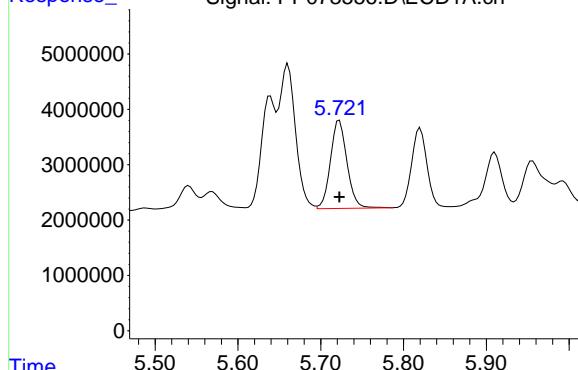


#5 AR-1016-3

R.T.: 5.051 min
 Delta R.T.: 0.000 min
 Response: 27424517
 Conc: 500.00 ng/ml

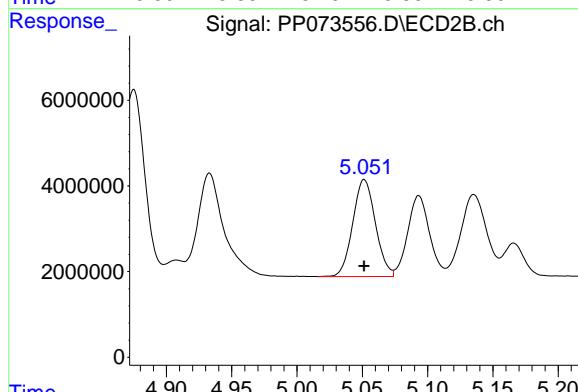


#6 AR-1016-4


R.T.: 5.820 min
 Delta R.T.: 0.000 min
 Response: 18296028
 Conc: 500.00 ng/ml

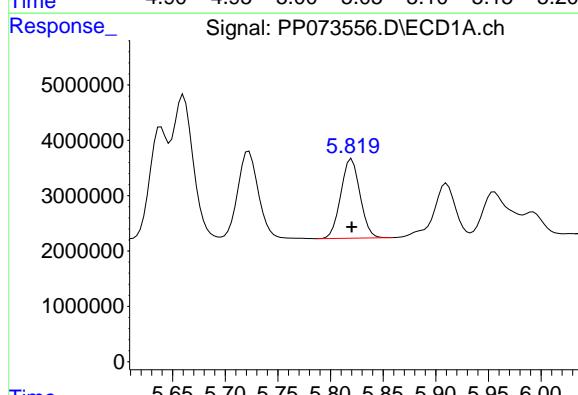

#6 AR-1016-4

R.T.: 5.093 min
 Delta R.T.: 0.000 min
 Response: 21948478
 Conc: 500.00 ng/ml

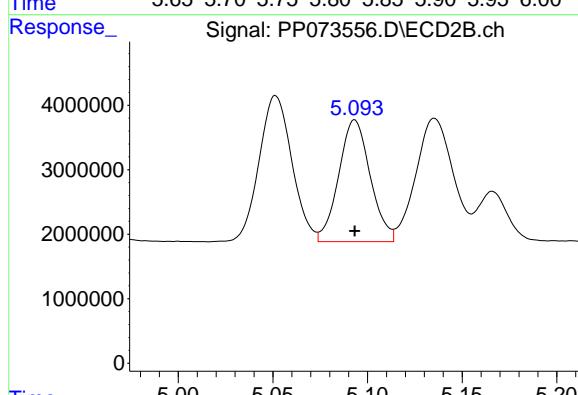

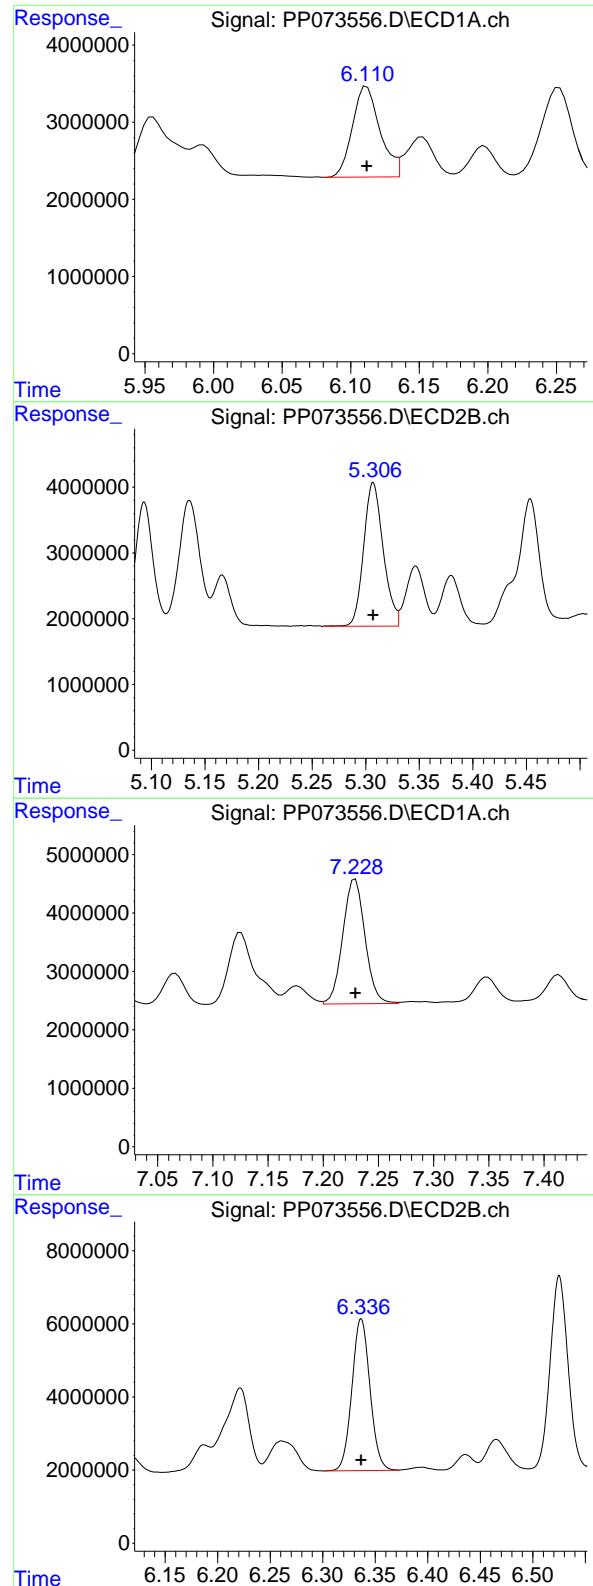

#7 AR-1016-5

R.T.: 6.112 min
 Delta R.T.: 0.000 min
 Response: 16393178
 Conc: 500.00 ng/ml

Instrument: ECD_P
 ClientSampleId: AR1660ICC500

#7 AR-1016-5

R.T.: 5.307 min
 Delta R.T.: 0.000 min
 Response: 27830144
 Conc: 500.00 ng/ml

#31 AR-1260-1

R.T.: 7.229 min
 Delta R.T.: 0.000 min
 Response: 29831866
 Conc: 500.00 ng/ml





#31 AR-1260-1

R.T.: 6.337 min
 Delta R.T.: 0.000 min
 Response: 49735666
 Conc: 500.00 ng/ml

#32 AR-1260-2

R.T.: 7.483 min
 Delta R.T.: 0.000 min
 Response: 45196946
 Conc: 500.00 ng/ml

Instrument: ECD_P
ClientSampleId: AR1660ICC500

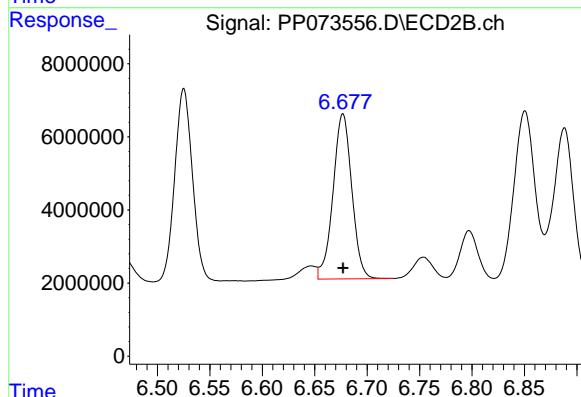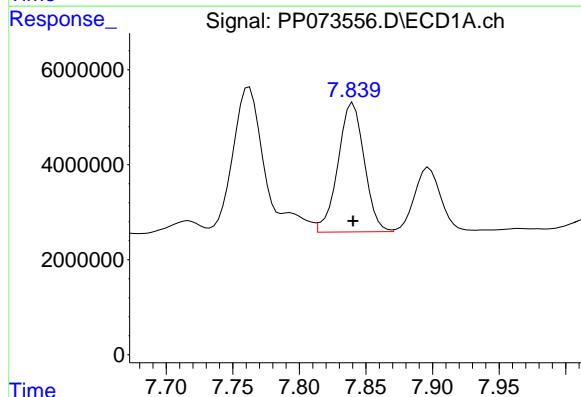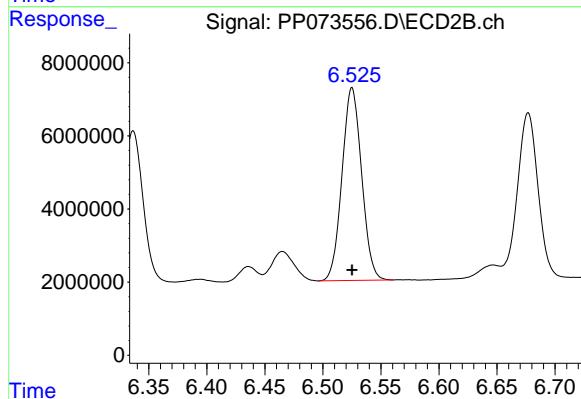

#32 AR-1260-2

R.T.: 6.525 min
 Delta R.T.: 0.000 min
 Response: 62001775
 Conc: 500.00 ng/ml

#33 AR-1260-3

R.T.: 7.840 min
 Delta R.T.: 0.000 min
 Response: 37345649
 Conc: 500.00 ng/ml





#33 AR-1260-3

R.T.: 6.677 min
 Delta R.T.: 0.000 min
 Response: 56146648
 Conc: 500.00 ng/ml

#34 AR-1260-4

R.T.: 8.064 min
 Delta R.T.: 0.000 min
 Response: 33365205
 Conc: 500.00 ng/ml

Instrument: ECD_P
ClientSampleId: AR1660ICC500

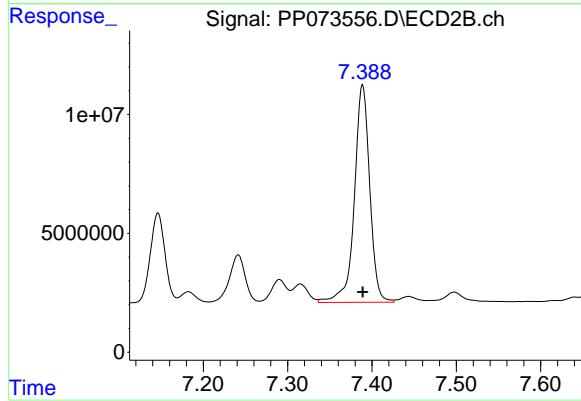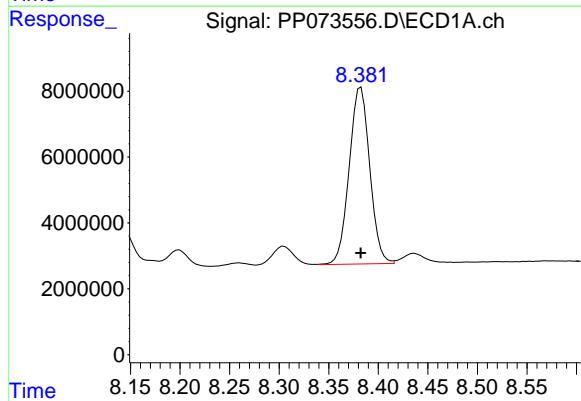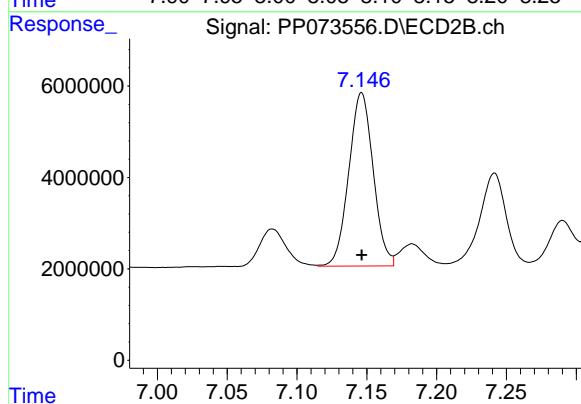

#34 AR-1260-4

R.T.: 7.146 min
 Delta R.T.: 0.000 min
 Response: 46174637
 Conc: 500.00 ng/ml

#35 AR-1260-5

R.T.: 8.383 min
 Delta R.T.: 0.000 min
 Response: 77448161
 Conc: 500.00 ng/ml

#35 AR-1260-5

R.T.: 7.389 min
 Delta R.T.: 0.000 min
 Response: 116112562
 Conc: 500.00 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP070825\
 Data File : PP073557.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Jul 2025 21:52
 Operator : YP\AJ
 Sample : AR1660ICC250
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
AR1660ICC250

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/08/2025
 Supervised By :mohammad ahmed 07/09/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 08 01:40:26 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 08 01:37:59 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	4.489	3.780	36726195	48601054	25.988	25.943
2) SA Decachlor...	10.180	8.781	29096309	36663112	25.387	27.681

Target Compounds

3) L1 AR-1016-1	5.640	4.858	12627919	18293907	267.888	266.983
4) L1 AR-1016-2	5.662	4.876	19179159	27468197	266.197	267.749
5) L1 AR-1016-3	5.723	5.053	11597460	14482667	262.608	264.046
6) L1 AR-1016-4	5.821	5.095	9615182	11760046	262.767	267.901
7) L1 AR-1016-5	6.113	5.308	8568508	14818058	261.344	266.223
31) L7 AR-1260-1	7.231	6.339	15831007	26051826	265.337	261.903
32) L7 AR-1260-2	7.484	6.527	24493361	32462748	270.963	261.789
33) L7 AR-1260-3	7.843	6.679	19201014	29417085	257.072	261.967
34) L7 AR-1260-4	8.066	7.147	17258868	24081302	258.636	260.763m
35) L7 AR-1260-5	8.385	7.391	40210084	58426954	259.594	251.596m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP070825\
 Data File : PP073557.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Jul 2025 21:52
 Operator : YP\AJ
 Sample : AR1660ICC250
 Misc :
 ALS Vial : 6 Sample Multiplier: 1



Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 08 01:40:26 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 08 01:37:59 2025
 Response via : Initial Calibration
 Integrator: ChemStation


Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Instrument :
 ECD_P
 ClientSampleId :
 AR1660ICC250

Manual Integrations APPROVED

Reviewed By :Yogesh Patel 07/08/2025
 Supervised By :mohammad ahmed 07/09/2025

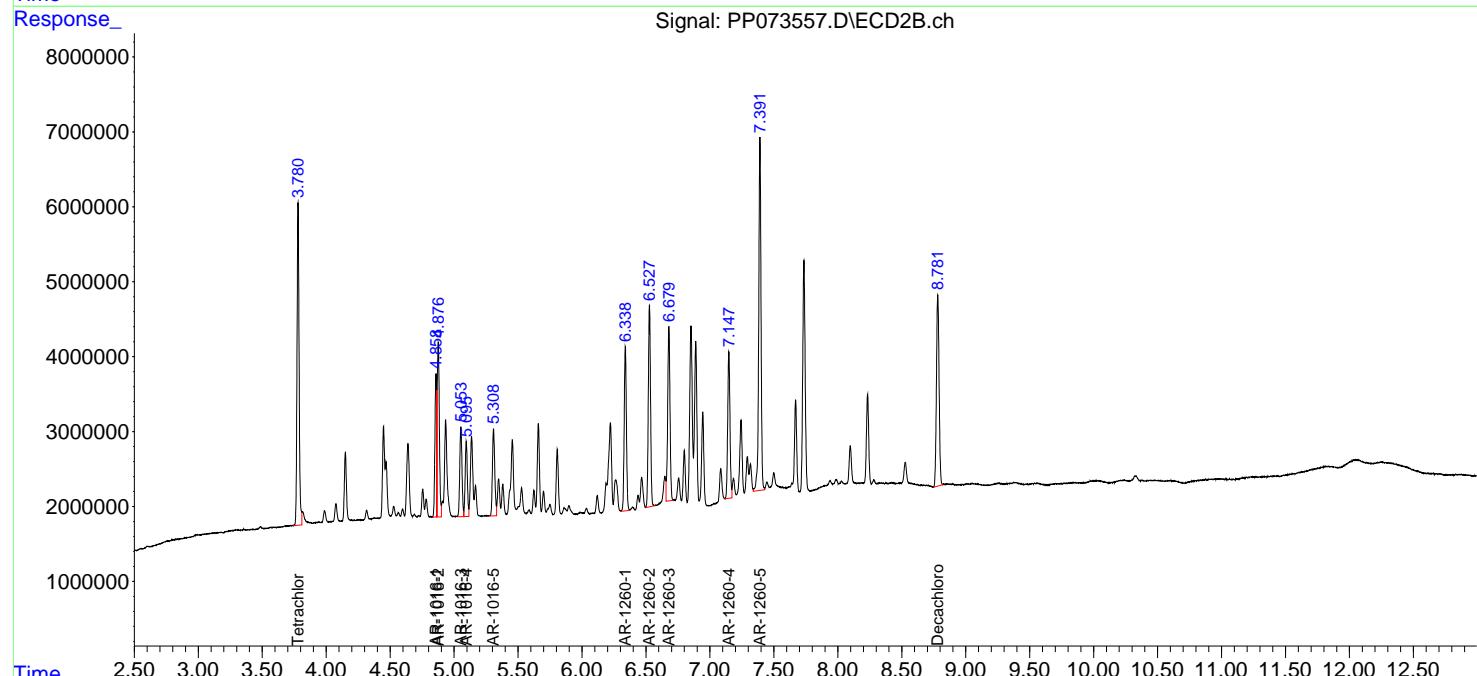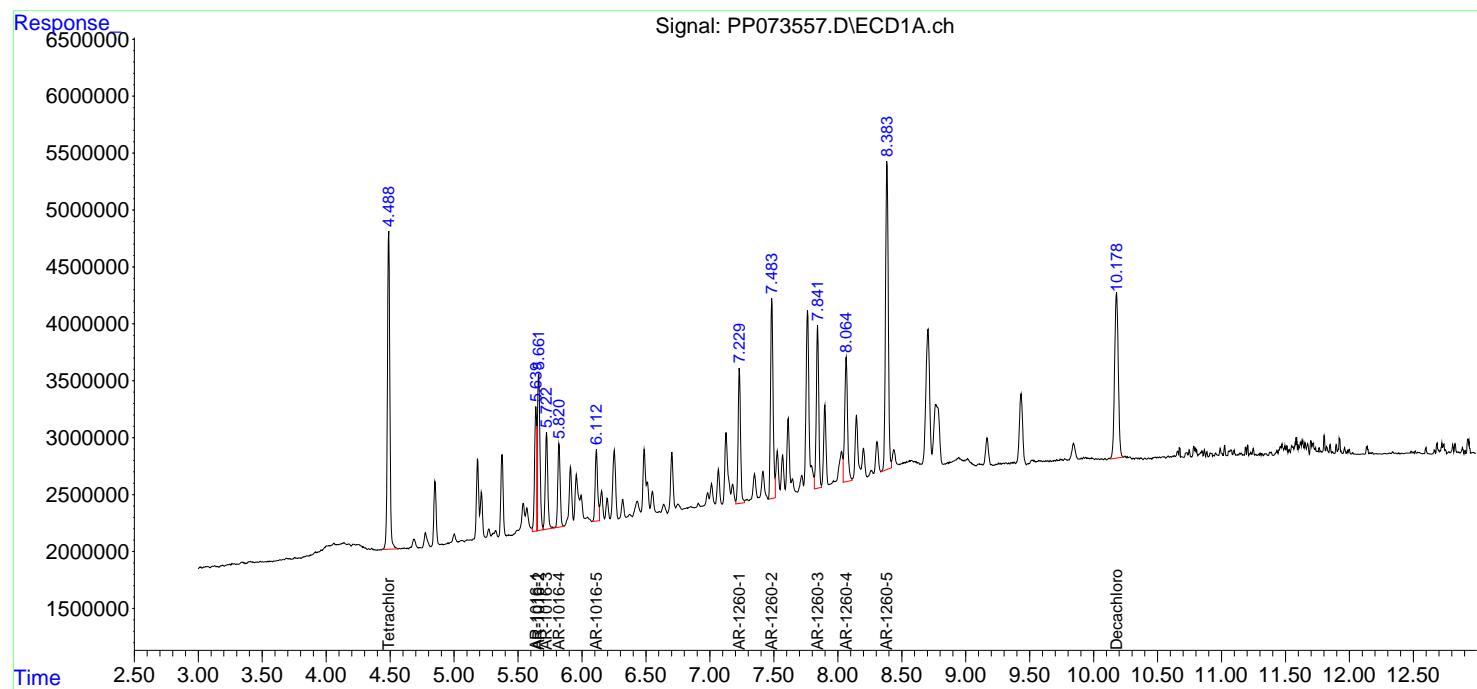

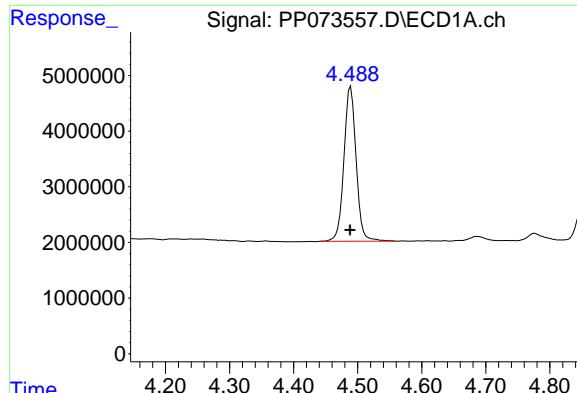


#1 Tetrachloro-m-xylene

R.T.: 4.489 min
Delta R.T.: 0.001 min
Response: 36726195
Conc: 25.99 ng/ml

Instrument: ECD_P
ClientSampleId: AR1660ICC250


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/08/2025
Supervised By :mohammad ahmed 07/09/2025

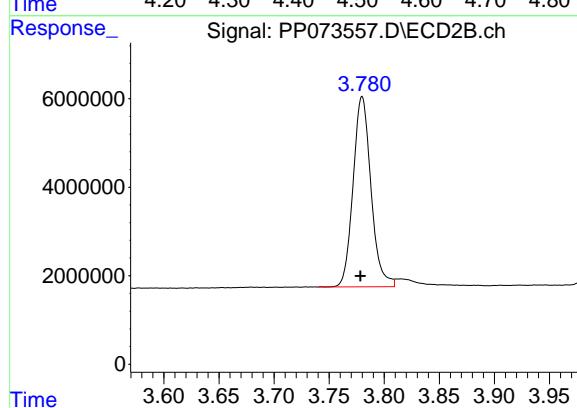


#1 Tetrachloro-m-xylene

R.T.: 3.780 min
Delta R.T.: 0.002 min
Response: 48601054
Conc: 25.94 ng/ml




#2 Decachlorobiphenyl

R.T.: 10.180 min
Delta R.T.: 0.003 min
Response: 29096309
Conc: 25.39 ng/ml

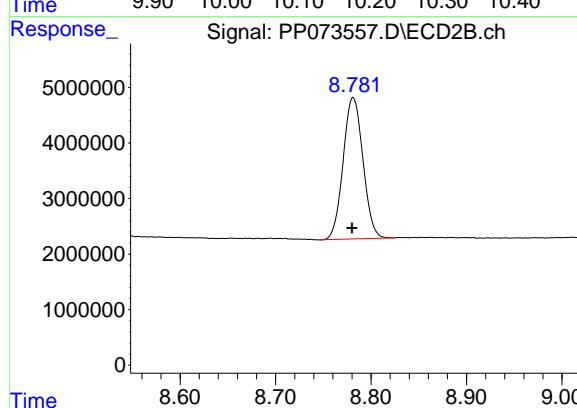

#2 Decachlorobiphenyl

R.T.: 8.781 min
Delta R.T.: 0.001 min
Response: 36663112
Conc: 27.68 ng/ml

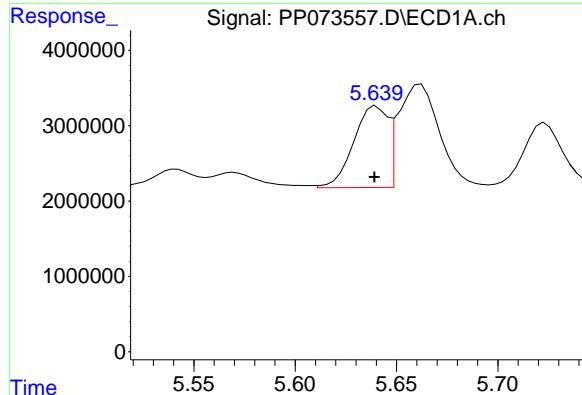


#3 AR-1016-1

R.T.: 5.640 min
Delta R.T.: 0.001 min
Response: 12627919
Conc: 267.89 ng/ml

Instrument: ECD_P
ClientSampleId: AR1660ICC250


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/08/2025
Supervised By :mohammad ahmed 07/09/2025

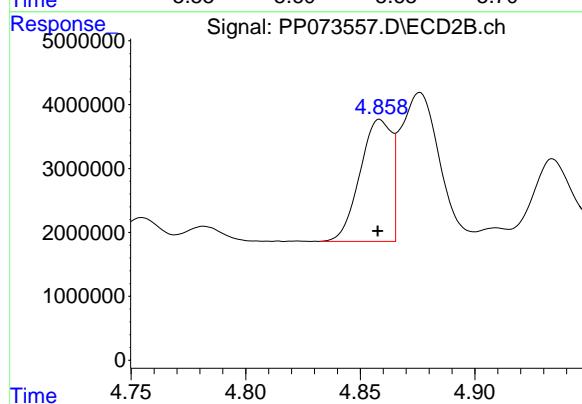


#3 AR-1016-1

R.T.: 4.858 min
Delta R.T.: 0.000 min
Response: 18293907
Conc: 266.98 ng/ml

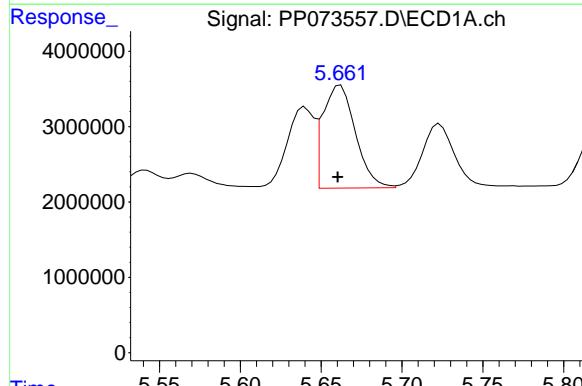

#4 AR-1016-2

R.T.: 5.662 min
Delta R.T.: 0.002 min
Response: 19179159
Conc: 266.20 ng/ml

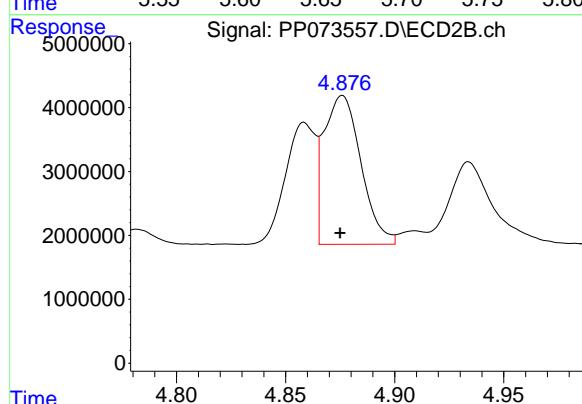

#4 AR-1016-2

R.T.: 4.876 min
Delta R.T.: 0.001 min
Response: 27468197
Conc: 267.75 ng/ml


#5 AR-1016-3

R.T.: 5.723 min
 Delta R.T.: 0.000 min
 Response: 11597460
 Conc: 262.61 ng/ml

Instrument :
 ECD_P
 ClientSampleId :
 AR1660ICC250


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/08/2025
 Supervised By :mohammad ahmed 07/09/2025

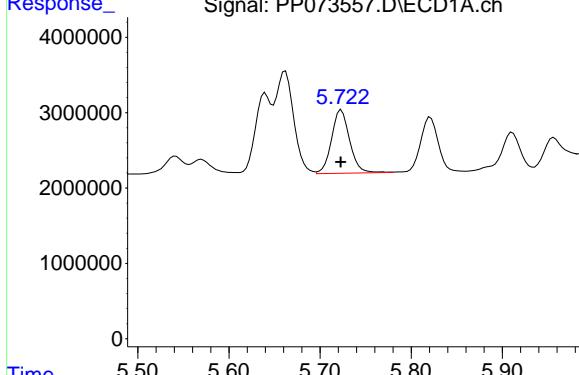

#5 AR-1016-3

R.T.: 5.053 min
 Delta R.T.: 0.002 min
 Response: 14482667
 Conc: 264.05 ng/ml

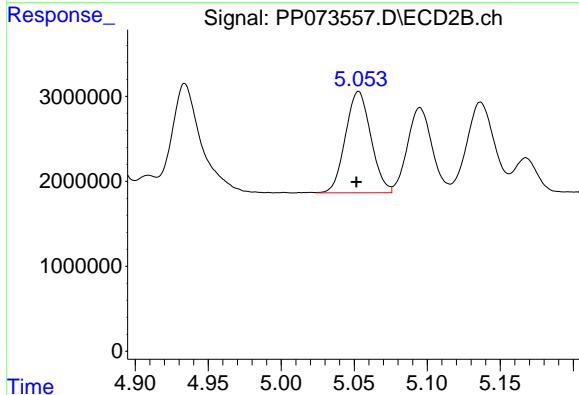


#6 AR-1016-4

R.T.: 5.821 min
 Delta R.T.: 0.000 min
 Response: 9615182
 Conc: 262.77 ng/ml

#6 AR-1016-4

R.T.: 5.095 min
 Delta R.T.: 0.002 min
 Response: 11760046
 Conc: 267.90 ng/ml

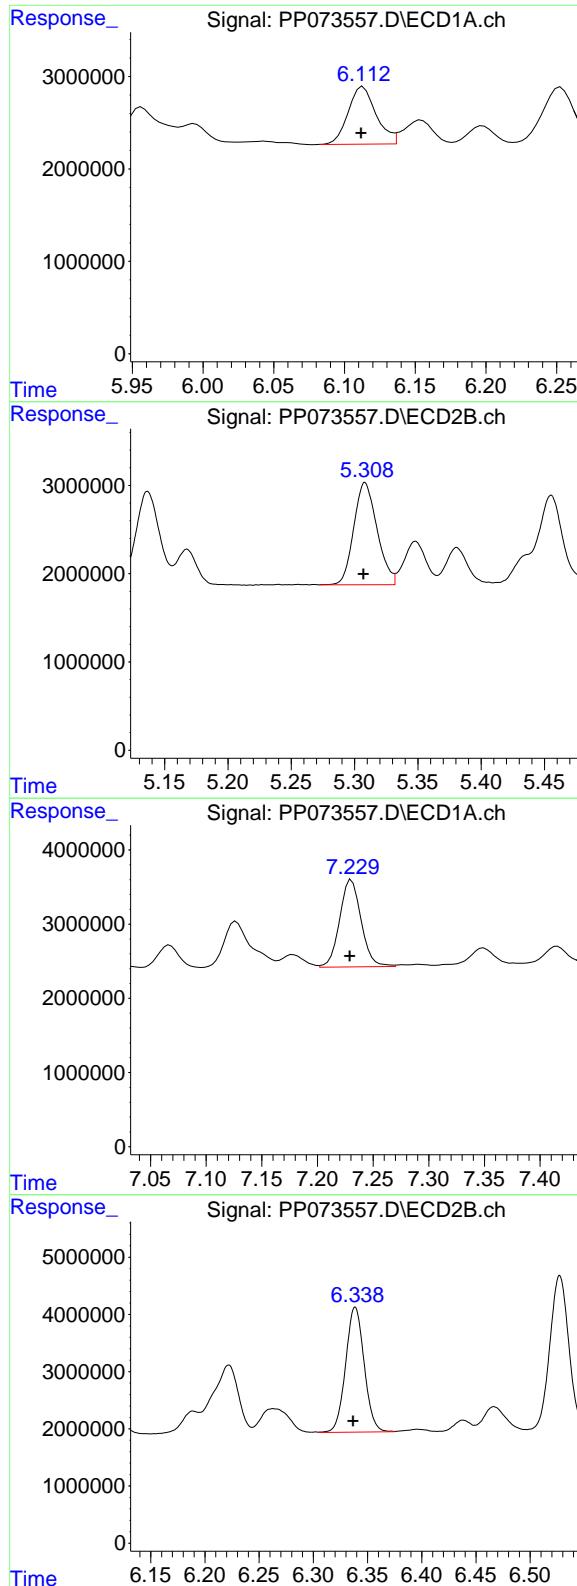

#7 AR-1016-5

R.T.: 6.113 min
 Delta R.T.: 0.001 min
 Response: 8568508
 Conc: 261.34 ng/ml

Instrument: ECD_P
ClientSampleId: AR1660ICC250

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/08/2025
 Supervised By :mohammad ahmed 07/09/2025

#7 AR-1016-5


R.T.: 5.308 min
 Delta R.T.: 0.001 min
 Response: 14818058
 Conc: 266.22 ng/ml

#31 AR-1260-1

R.T.: 7.231 min
 Delta R.T.: 0.002 min
 Response: 15831007
 Conc: 265.34 ng/ml

#31 AR-1260-1

R.T.: 6.339 min
 Delta R.T.: 0.002 min
 Response: 26051826
 Conc: 261.90 ng/ml

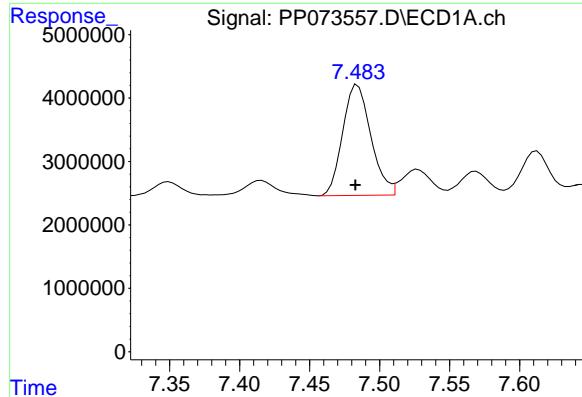


#32 AR-1260-2

R.T.: 7.484 min
 Delta R.T.: 0.002 min
 Response: 24493361
 Conc: 270.96 ng/ml

Instrument: ECD_P
ClientSampleId: AR1660ICC250


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/08/2025
 Supervised By :mohammad ahmed 07/09/2025

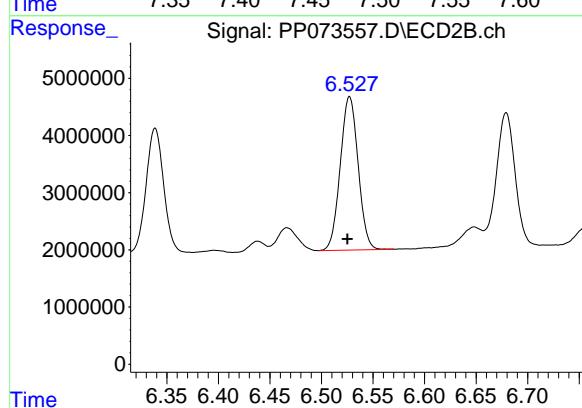


#32 AR-1260-2

R.T.: 6.527 min
 Delta R.T.: 0.002 min
 Response: 32462748
 Conc: 261.79 ng/ml

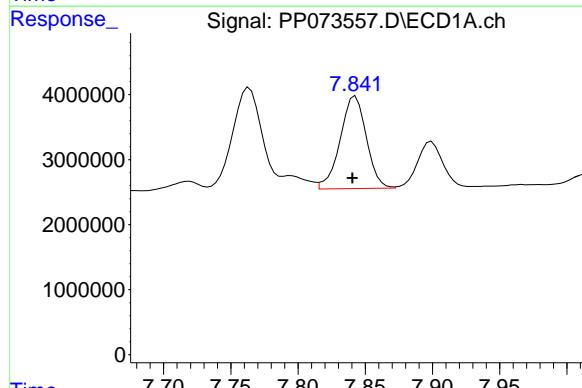

#33 AR-1260-3

R.T.: 7.843 min
 Delta R.T.: 0.002 min
 Response: 19201014
 Conc: 257.07 ng/ml

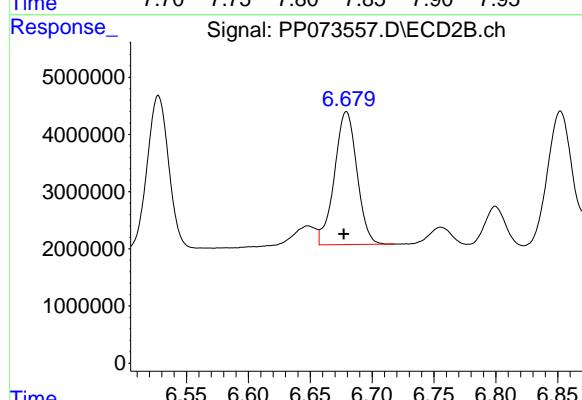

#33 AR-1260-3

R.T.: 6.679 min
 Delta R.T.: 0.002 min
 Response: 29417085
 Conc: 261.97 ng/ml





#34 AR-1260-4

R.T.: 8.066 min
 Delta R.T.: 0.001 min
 Response: 17258868
 Conc: 258.64 ng/ml

Instrument: ECD_P
ClientSampleId: AR1660ICC250

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/08/2025
 Supervised By :mohammad ahmed 07/09/2025

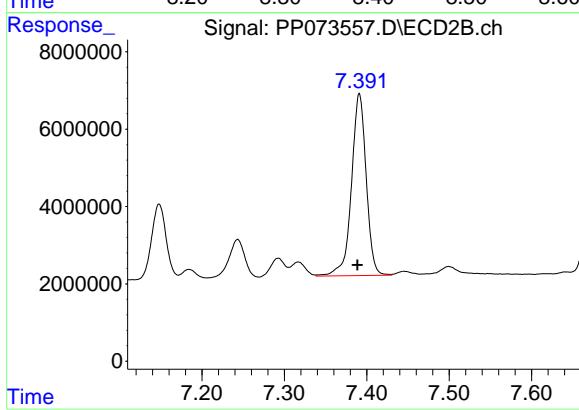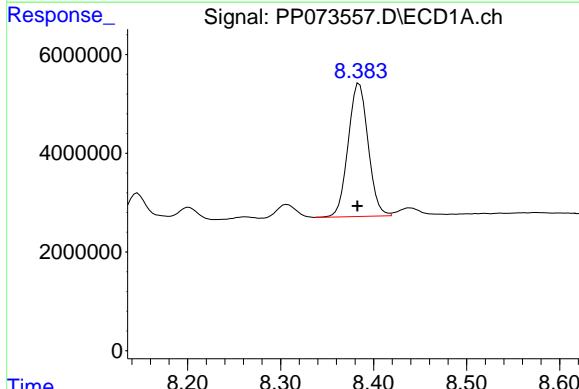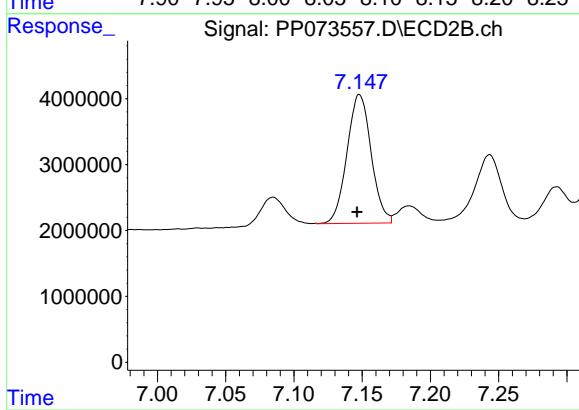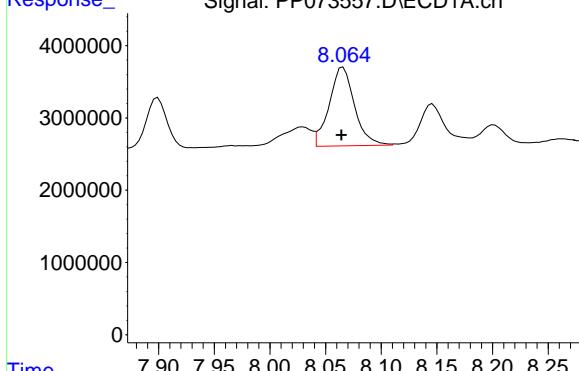

#34 AR-1260-4

R.T.: 7.147 min
 Delta R.T.: 0.001 min
 Response: 24081302
 Conc: 260.76 ng/ml

#35 AR-1260-5

R.T.: 8.385 min
 Delta R.T.: 0.002 min
 Response: 40210084
 Conc: 259.59 ng/ml

#35 AR-1260-5

R.T.: 7.391 min
 Delta R.T.: 0.002 min
 Response: 58426954
 Conc: 251.60 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP070825\
 Data File : PP073558.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Jul 2025 22:08
 Operator : YP\AJ
 Sample : AR1660ICC050
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
AR1660ICC050

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/08/2025
 Supervised By :mohammad ahmed 07/09/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 08 01:40:50 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 08 01:37:59 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	4.485	3.779	6400868	8634125	4.529	4.609
2) SA Decachlor...	10.173	8.780	4780120	5986472	4.171	4.520

Target Compounds

3) L1 AR-1016-1	5.635	4.857	2592361	3433572	54.994m	50.110
4) L1 AR-1016-2	5.658	4.875	3532445	5058097	49.029	49.304
5) L1 AR-1016-3	5.719	5.052	2287754	2711653	51.803	49.438
6) L1 AR-1016-4	5.817	5.094	1779663	2333668	48.635	53.162
7) L1 AR-1016-5	6.109	5.307	1335478	2709671	40.733	48.682
31) L7 AR-1260-1	7.226	6.336	2914675	5013856	48.852	50.405m
32) L7 AR-1260-2	7.482	6.525	6085083	6438631	67.317	51.923
33) L7 AR-1260-3	7.838	6.677	3450365	5301254	46.195	47.209
34) L7 AR-1260-4	8.061	7.146	3038521	4249208	45.534	46.012m
35) L7 AR-1260-5	8.379	7.388	6955237	10235896	44.903	44.077m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP070825\
 Data File : PP073558.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Jul 2025 22:08
 Operator : YP\AJ
 Sample : AR1660ICC050
 Misc :
 ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
AR1660ICC050


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/08/2025
 Supervised By :mohammad ahmed 07/09/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 08 01:40:50 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 08 01:37:59 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

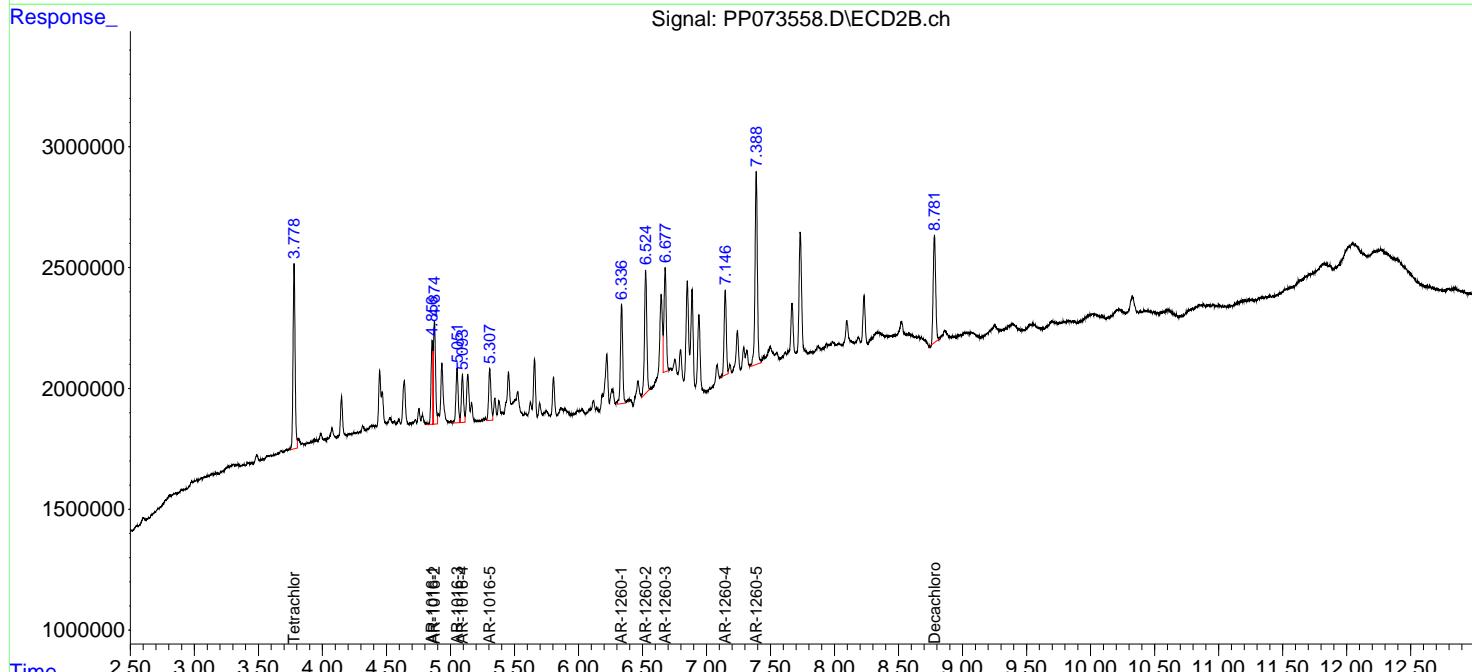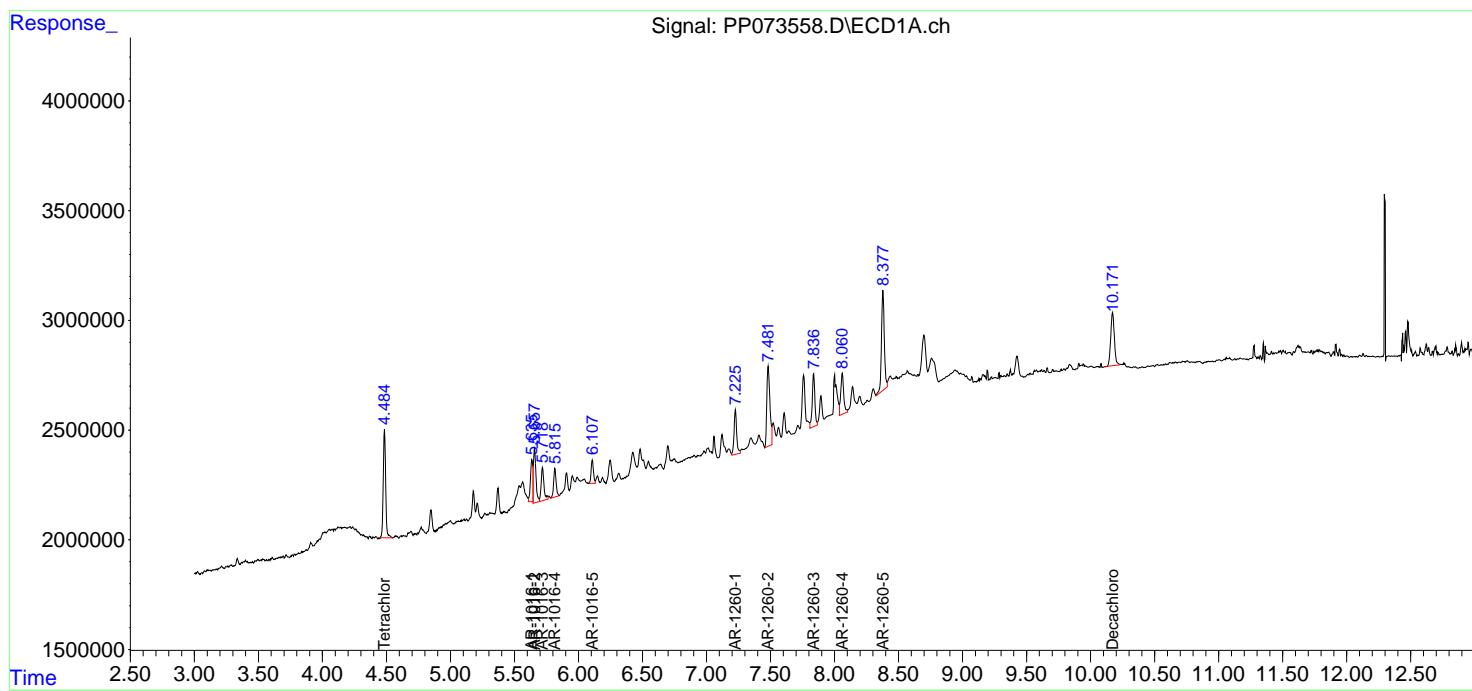

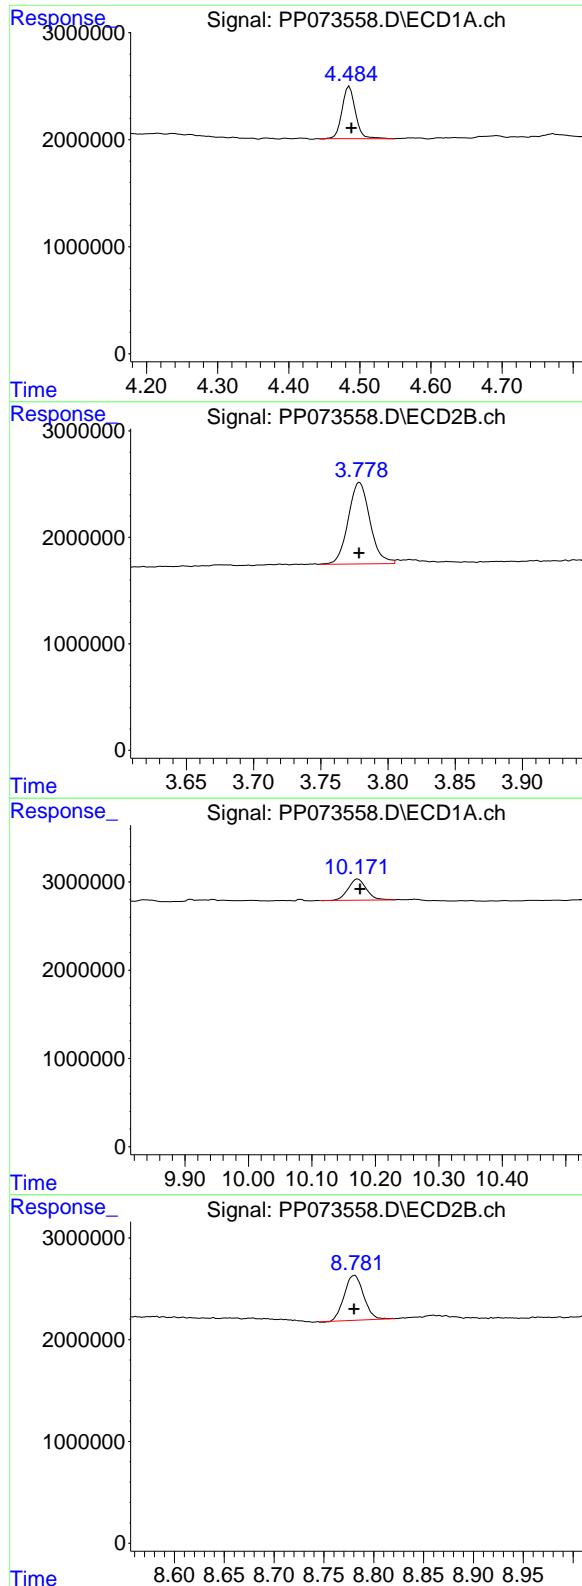

#1 Tetrachloro-m-xylene

R.T.: 4.485 min
Delta R.T.: -0.003 min
Response: 6400868
Conc: 4.53 ng/ml

Instrument: ECD_P
ClientSampleId : AR1660ICC050

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/08/2025
Supervised By :mohammad ahmed 07/09/2025

#1 Tetrachloro-m-xylene

R.T.: 3.779 min
Delta R.T.: 0.000 min
Response: 8634125
Conc: 4.61 ng/ml

#2 Decachlorobiphenyl

R.T.: 10.173 min
Delta R.T.: -0.004 min
Response: 4780120
Conc: 4.17 ng/ml

#2 Decachlorobiphenyl

R.T.: 8.780 min
Delta R.T.: 0.000 min
Response: 5986472
Conc: 4.52 ng/ml





#3 AR-1016-1

R.T.: 5.635 min
 Delta R.T.: -0.004 min
 Response: 2592361
 Conc: 54.99 ng/ml

Instrument: ECD_P
ClientSampleId: AR1660ICC050

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/08/2025
 Supervised By :mohammad ahmed 07/09/2025

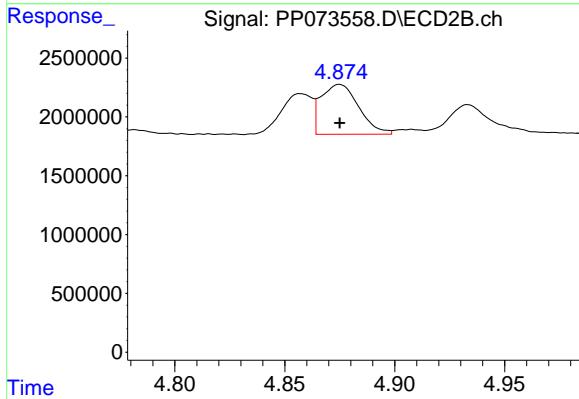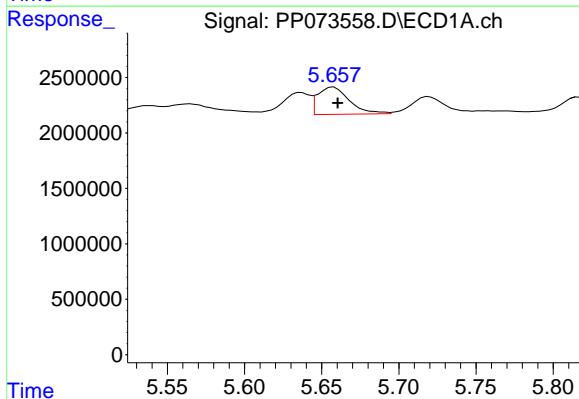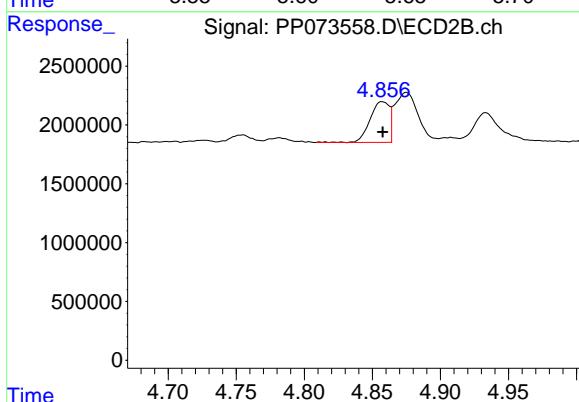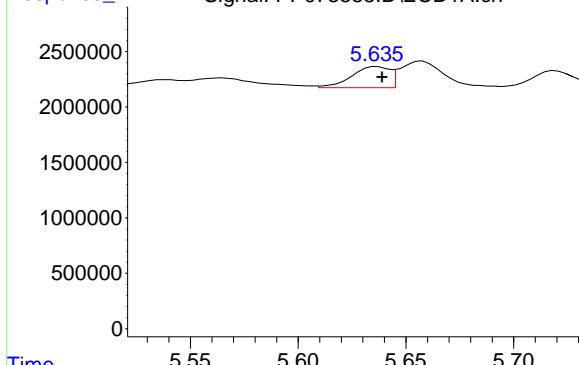

#3 AR-1016-1

R.T.: 4.857 min
 Delta R.T.: 0.000 min
 Response: 3433572
 Conc: 50.11 ng/ml

#4 AR-1016-2

R.T.: 5.658 min
 Delta R.T.: -0.003 min
 Response: 3532445
 Conc: 49.03 ng/ml

#4 AR-1016-2

R.T.: 4.875 min
 Delta R.T.: 0.000 min
 Response: 5058097
 Conc: 49.30 ng/ml





#5 AR-1016-3

R.T.: 5.719 min
 Delta R.T.: -0.003 min
 Response: 2287754
 Conc: 51.80 ng/ml

Instrument: ECD_P
ClientSampleId: AR1660ICC050

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/08/2025
 Supervised By :mohammad ahmed 07/09/2025

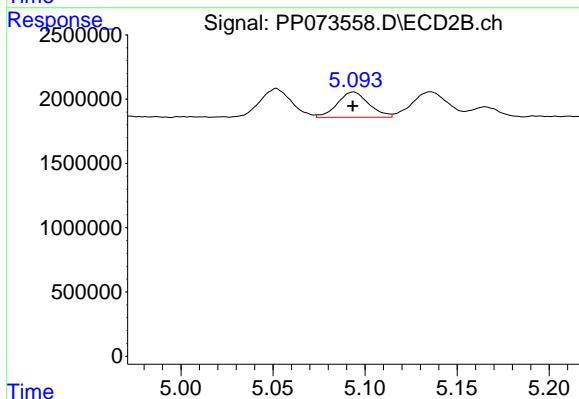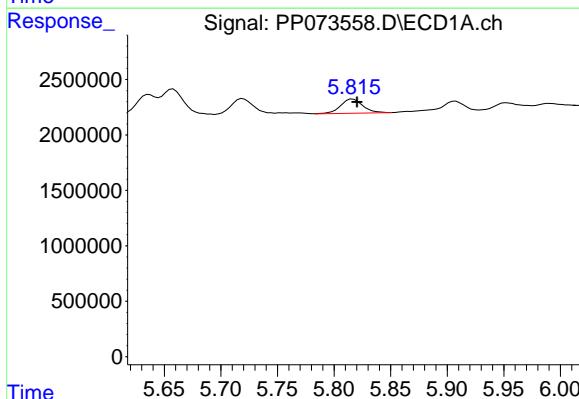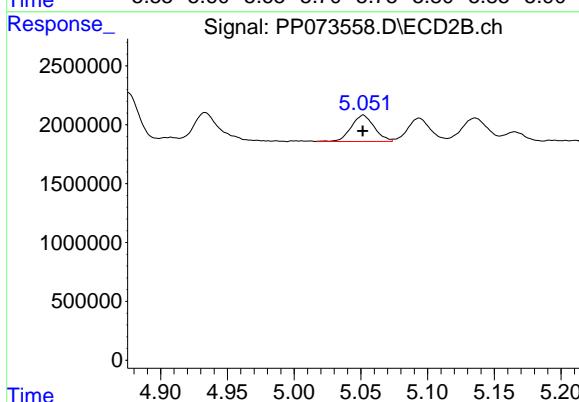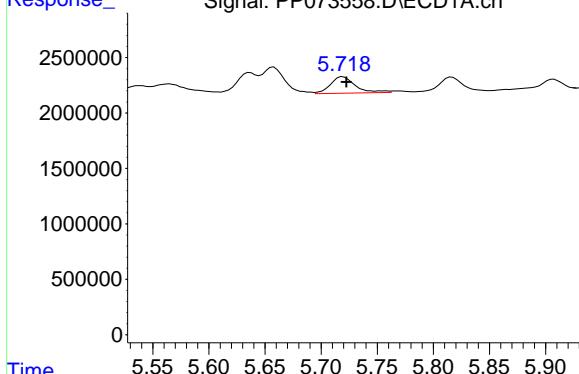

#5 AR-1016-3





R.T.: 5.052 min
 Delta R.T.: 0.000 min
 Response: 2711653
 Conc: 49.44 ng/ml

#6 AR-1016-4

R.T.: 5.817 min
 Delta R.T.: -0.004 min
 Response: 1779663
 Conc: 48.64 ng/ml

#6 AR-1016-4

R.T.: 5.094 min
 Delta R.T.: 0.000 min
 Response: 2333668
 Conc: 53.16 ng/ml

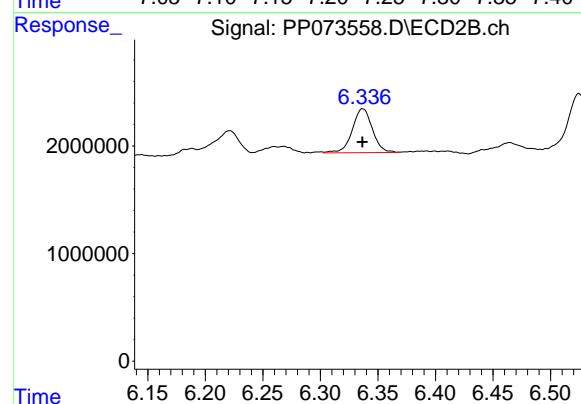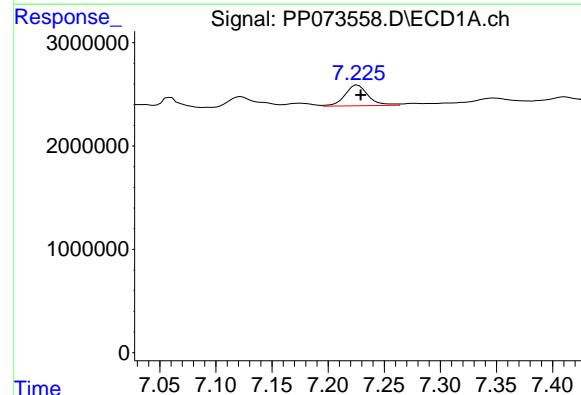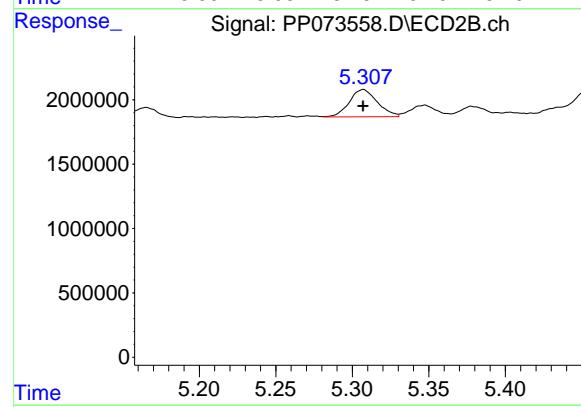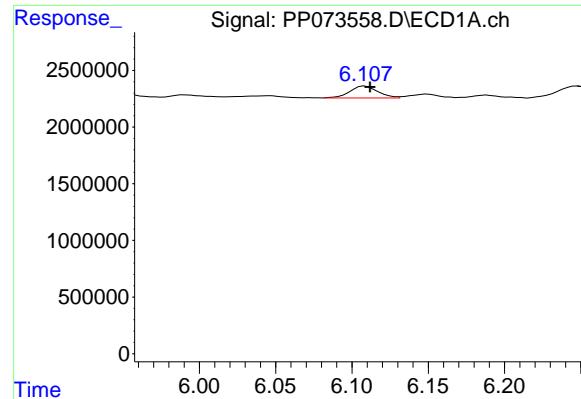




#7 AR-1016-5

R.T.: 6.109 min
 Delta R.T.: -0.003 min
 Response: 1335478
 Conc: 40.73 ng/ml

Instrument: ECD_P
ClientSampleId: AR1660ICC050

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/08/2025
 Supervised By :mohammad ahmed 07/09/2025

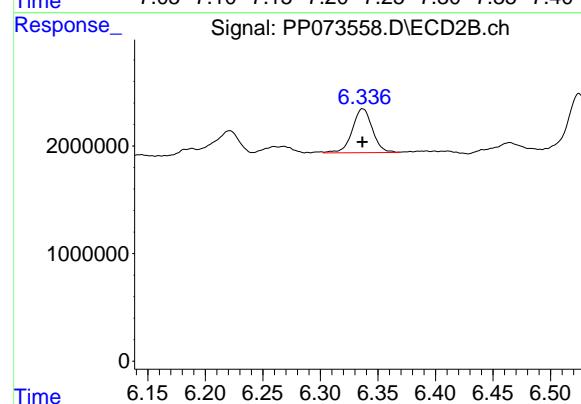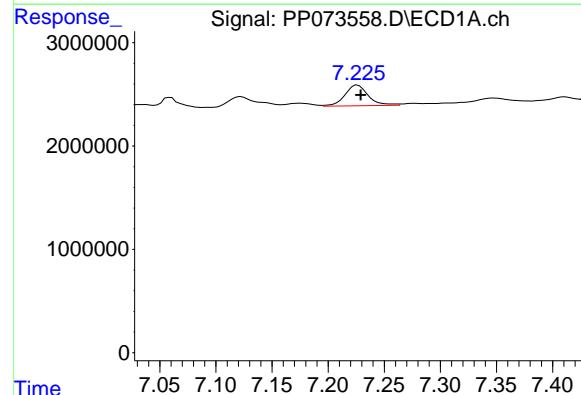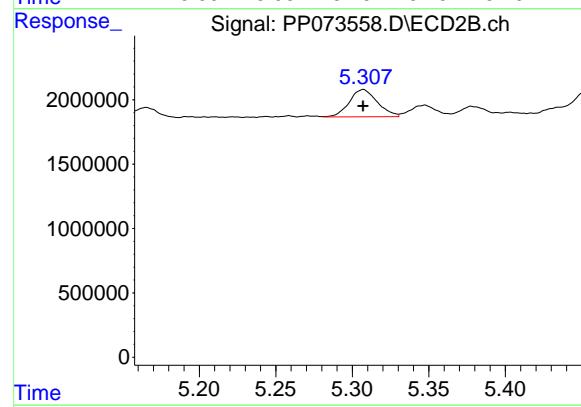

#7 AR-1016-5


R.T.: 5.307 min
 Delta R.T.: 0.000 min
 Response: 2709671
 Conc: 48.68 ng/ml

#31 AR-1260-1

R.T.: 7.226 min
 Delta R.T.: -0.003 min
 Response: 2914675
 Conc: 48.85 ng/ml

#31 AR-1260-1

R.T.: 6.336 min
 Delta R.T.: 0.000 min
 Response: 5013856
 Conc: 50.41 ng/ml

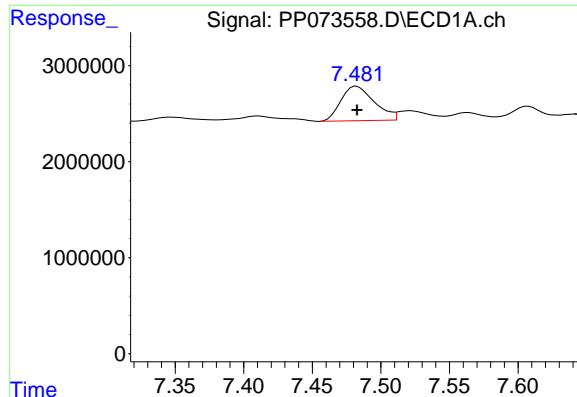


#32 AR-1260-2

R.T.: 7.482 min
 Delta R.T.: 0.000 min
 Response: 6085083
 Conc: 67.32 ng/ml

Instrument: ECD_P
ClientSampleId: AR1660ICC050


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/08/2025
 Supervised By :mohammad ahmed 07/09/2025

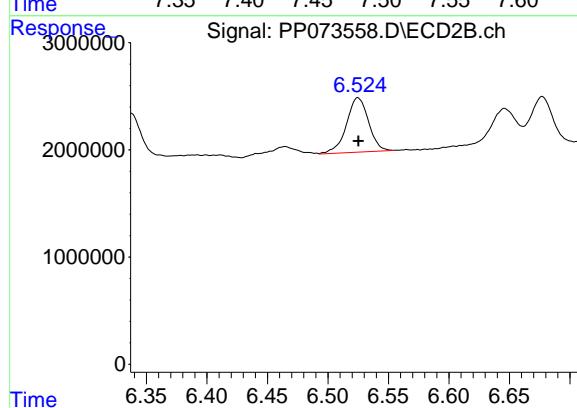


#32 AR-1260-2

R.T.: 6.525 min
 Delta R.T.: 0.000 min
 Response: 6438631
 Conc: 51.92 ng/ml

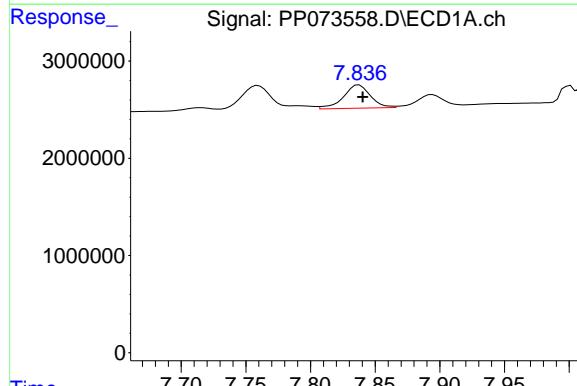

#33 AR-1260-3

R.T.: 7.838 min
 Delta R.T.: -0.003 min
 Response: 3450365
 Conc: 46.20 ng/ml

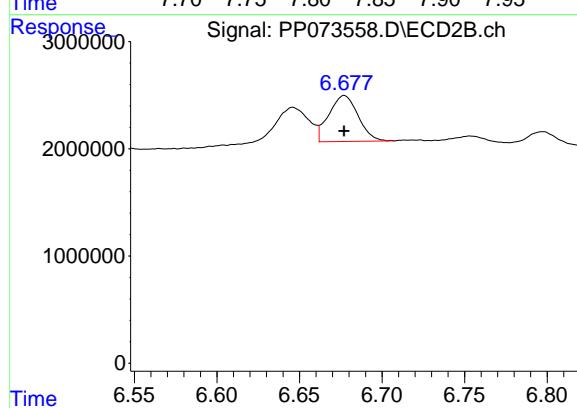

#33 AR-1260-3

R.T.: 6.677 min
 Delta R.T.: 0.000 min
 Response: 5301254
 Conc: 47.21 ng/ml

#34 AR-1260-4

R.T.: 8.061 min
 Delta R.T.: -0.003 min
 Response: 3038521
 Conc: 45.53 ng/ml

Instrument: ECD_P
ClientSampleId: AR1660ICC050

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/08/2025
 Supervised By :mohammad ahmed 07/09/2025

#34 AR-1260-4





R.T.: 7.146 min
 Delta R.T.: 0.000 min
 Response: 4249208
 Conc: 46.01 ng/ml

#35 AR-1260-5

R.T.: 8.379 min
 Delta R.T.: -0.004 min
 Response: 6955237
 Conc: 44.90 ng/ml

#35 AR-1260-5

R.T.: 7.388 min
 Delta R.T.: -0.001 min
 Response: 10235896
 Conc: 44.08 ng/ml

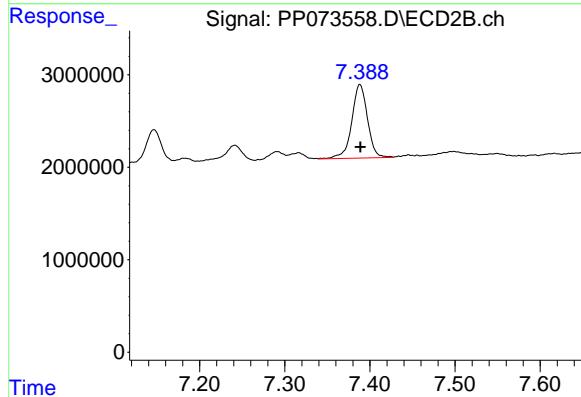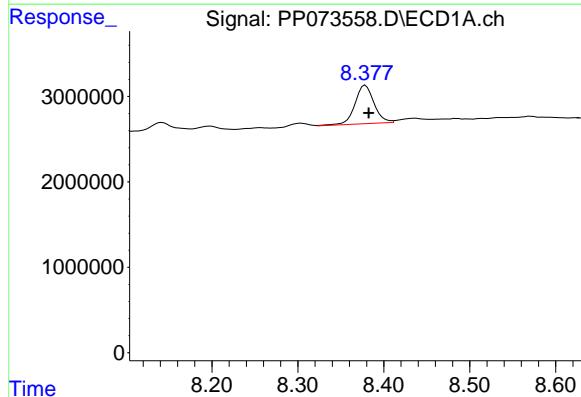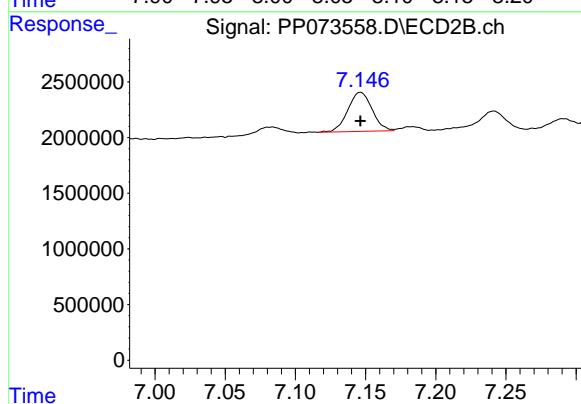

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP070825\
 Data File : PP073559.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Jul 2025 22:24
 Operator : YP\AJ
 Sample : AR1221ICC500
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
AR1221ICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 08 01:53:45 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 08 01:53:24 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	4.489	3.779	71300233	92532894	50.000	50.000
2) SA Decachlor...	10.176	8.782	56752030	68180160	50.000	50.000

Target Compounds

8) L2 AR-1221-1	4.690	3.988	8933218	13522466	500.000	500.000
9) L2 AR-1221-2	4.776	4.075	6752235	10180159	500.000	500.000
10) L2 AR-1221-3	4.851	4.150	20802411	30724321	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP070825\
 Data File : PP073559.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Jul 2025 22:24
 Operator : YP\AJ
 Sample : AR1221ICC500
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
AR1221ICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 08 01:53:45 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 08 01:53:24 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

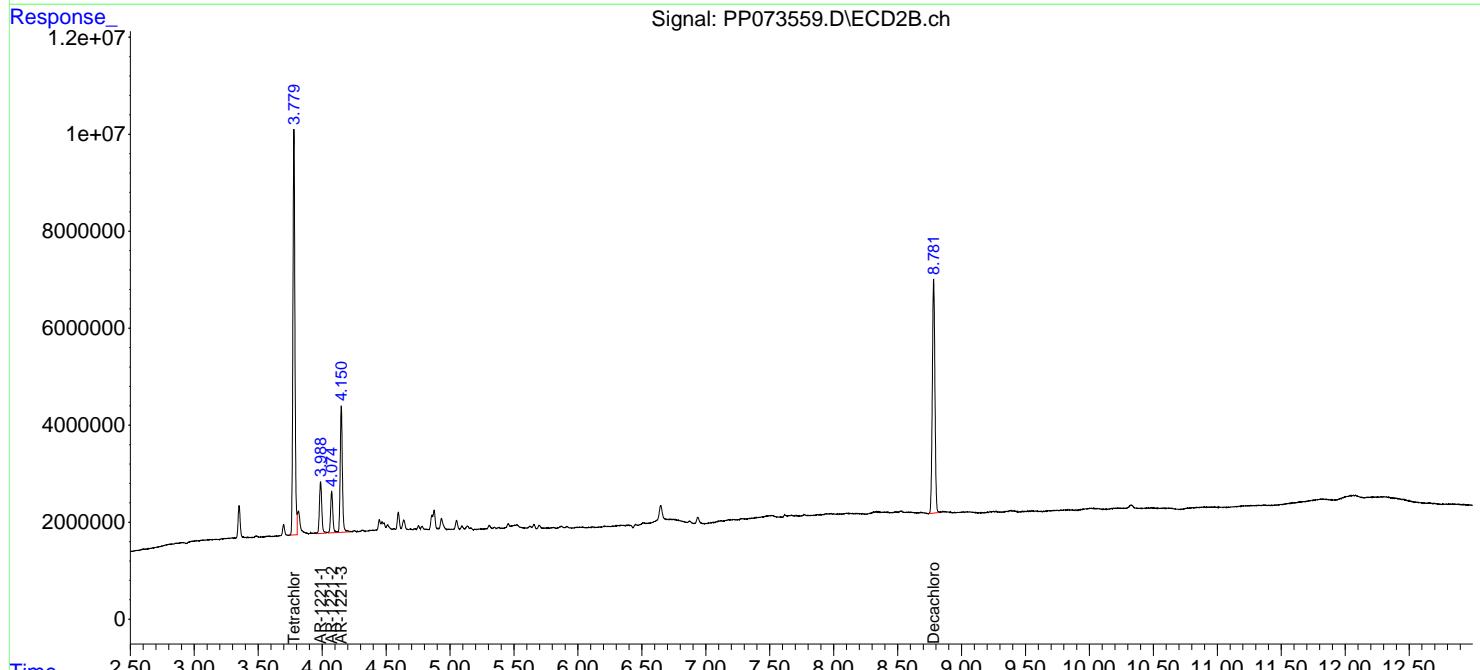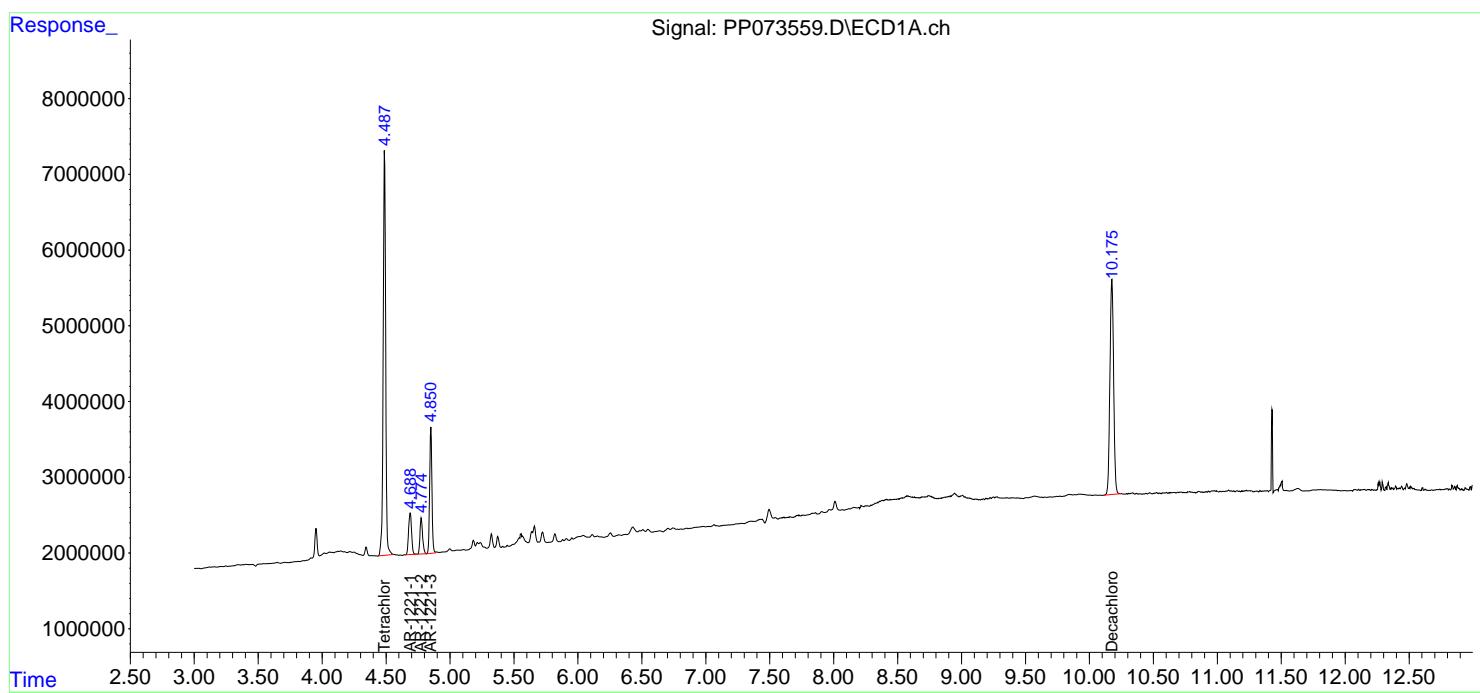


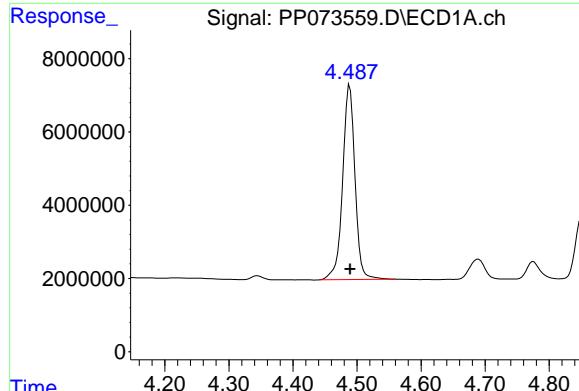

#1 Tetrachloro-m-xylene

R.T.: 4.489 min
Delta R.T.: 0.000 min
Response: 71300233
Conc: 50.00 ng/ml

Instrument: ECD_P
ClientSampleId: AR1221ICC500

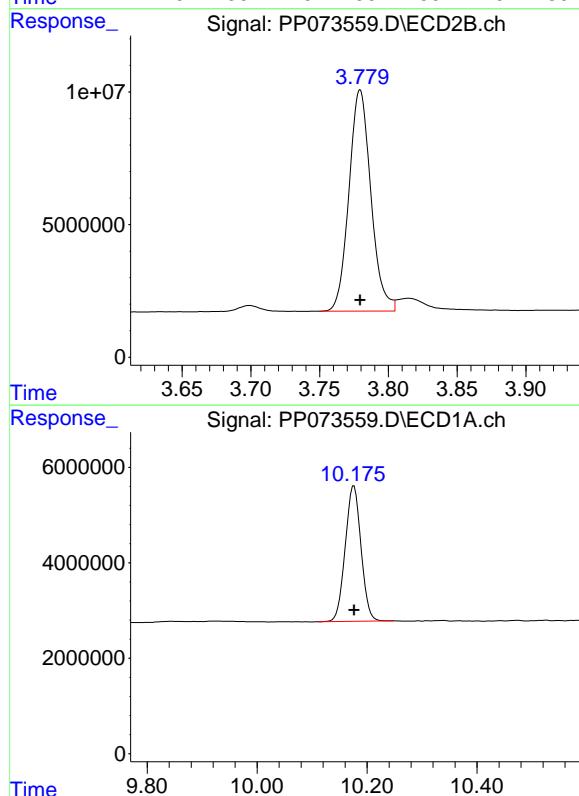

#1 Tetrachloro-m-xylene

R.T.: 3.779 min
Delta R.T.: 0.000 min
Response: 92532894
Conc: 50.00 ng/ml

#2 Decachlorobiphenyl

R.T.: 10.176 min
Delta R.T.: 0.000 min
Response: 56752030
Conc: 50.00 ng/ml





#2 Decachlorobiphenyl

R.T.: 8.782 min
Delta R.T.: 0.000 min
Response: 68180160
Conc: 50.00 ng/ml

#8 AR-1221-1

R.T.: 4.690 min
 Delta R.T.: 0.000 min
 Response: 8933218
 Conc: 500.00 ng/ml

Instrument: ECD_P
ClientSampleId: AR1221ICC500

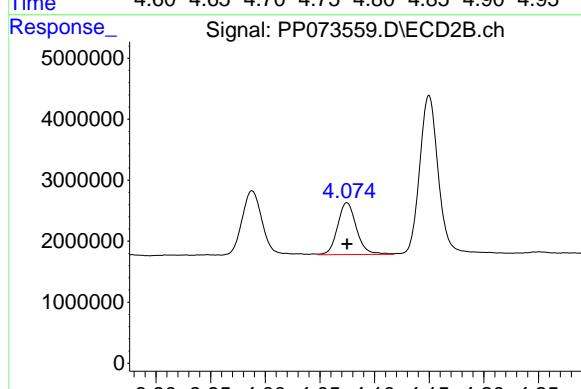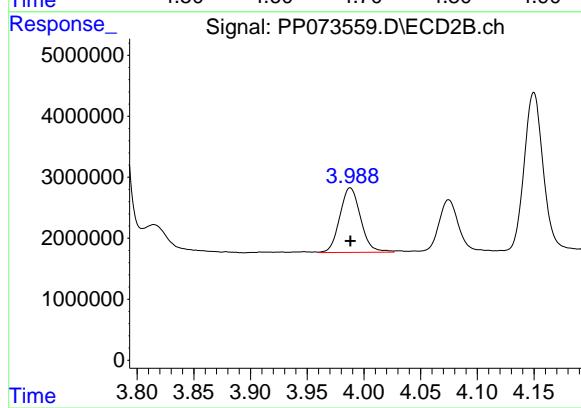

#8 AR-1221-1

R.T.: 3.988 min
 Delta R.T.: 0.000 min
 Response: 13522466
 Conc: 500.00 ng/ml

#9 AR-1221-2

R.T.: 4.776 min
 Delta R.T.: 0.000 min
 Response: 6752235
 Conc: 500.00 ng/ml



#9 AR-1221-2

R.T.: 4.075 min
 Delta R.T.: 0.000 min
 Response: 10180159
 Conc: 500.00 ng/ml

#10 AR-1221-3

R.T.: 4.851 min
Delta R.T.: 0.000 min
Response: 20802411
Conc: 500.00 ng/ml

Instrument: ECD_P
ClientSampleId: AR1221ICC500

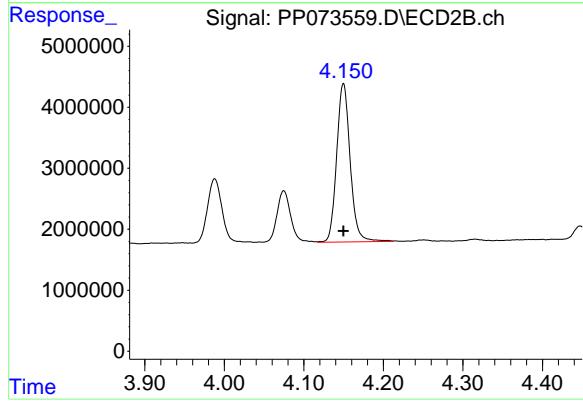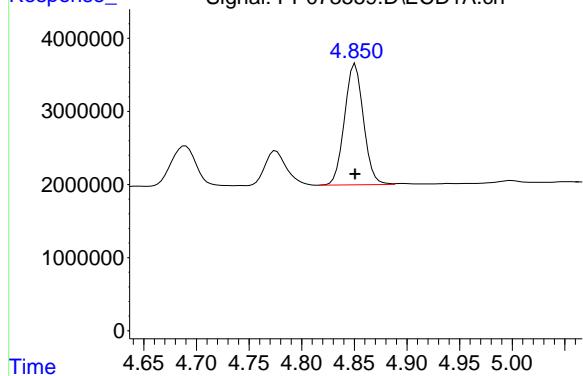

#10 AR-1221-3

R.T.: 4.150 min
Delta R.T.: 0.000 min
Response: 30724321
Conc: 500.00 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP070825\
 Data File : PP073560.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Jul 2025 22:41
 Operator : YP\AJ
 Sample : AR1232ICC500
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
AR1232ICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 08 01:58:44 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 08 01:58:13 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	4.488	3.779	69747801	89329746	50.000	50.000
2) SA Decachlor...	10.175	8.781	55031795	64481917	50.000	50.000

Target Compounds

11) L3 AR-1232-1	4.850	4.149	16325352	23307175	500.000	500.000
12) L3 AR-1232-2	5.374	4.875	8127340	23829904	500.000	500.000
13) L3 AR-1232-3	5.660	5.052	16496729	12514513	500.000	500.000
14) L3 AR-1232-4	5.820	5.137	8222579	10828145	500.000	500.000
15) L3 AR-1232-5	5.909	5.308	5285179	11281724	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP070825\
 Data File : PP073560.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Jul 2025 22:41
 Operator : YP\AJ
 Sample : AR1232ICC500
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
AR1232ICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 08 01:58:44 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 08 01:58:13 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ m Signal #2 Info : 30M x 0.32mm x 0.25 μ m

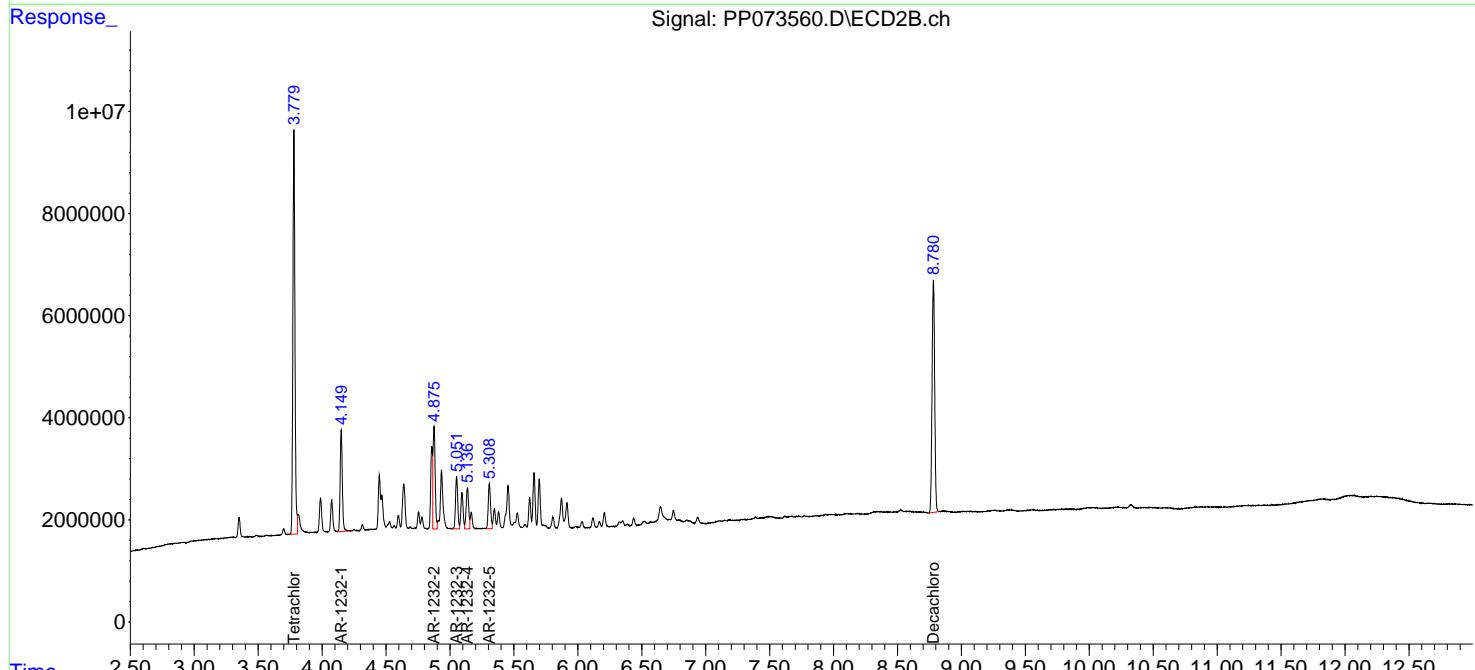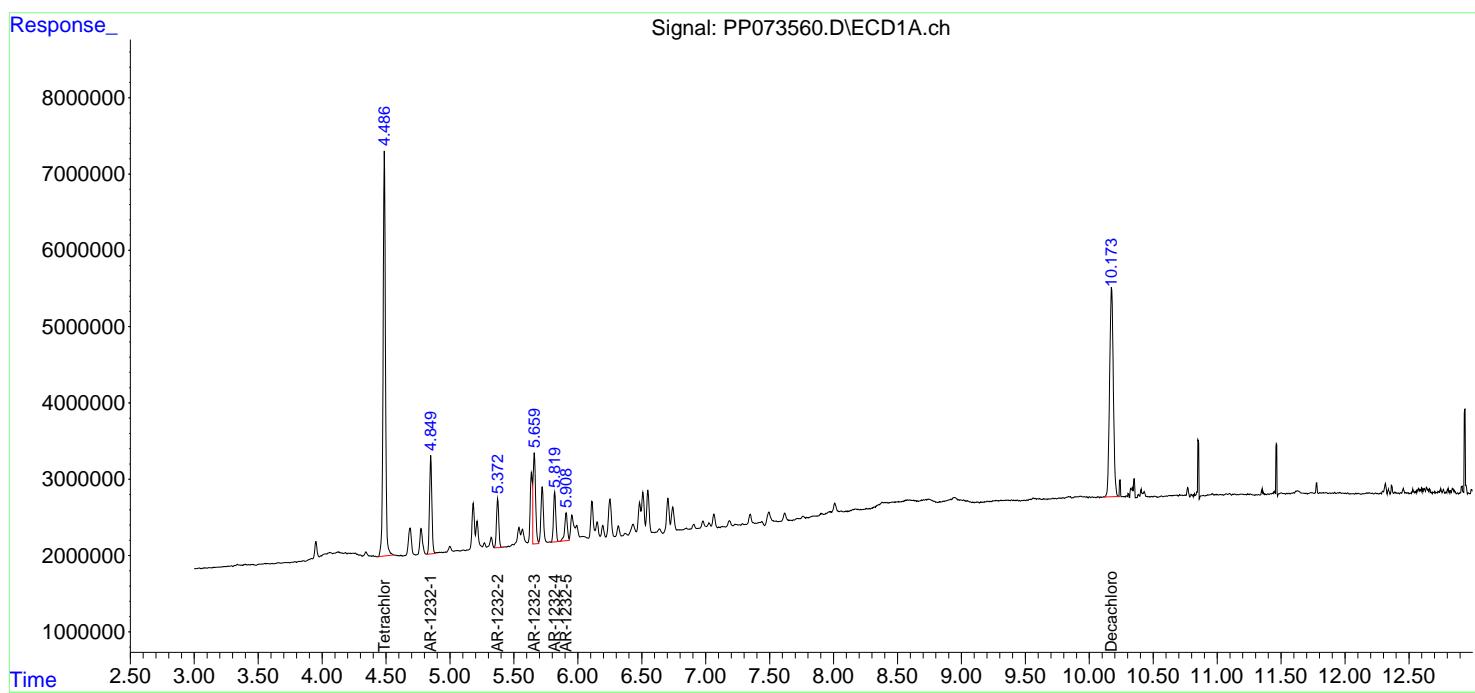

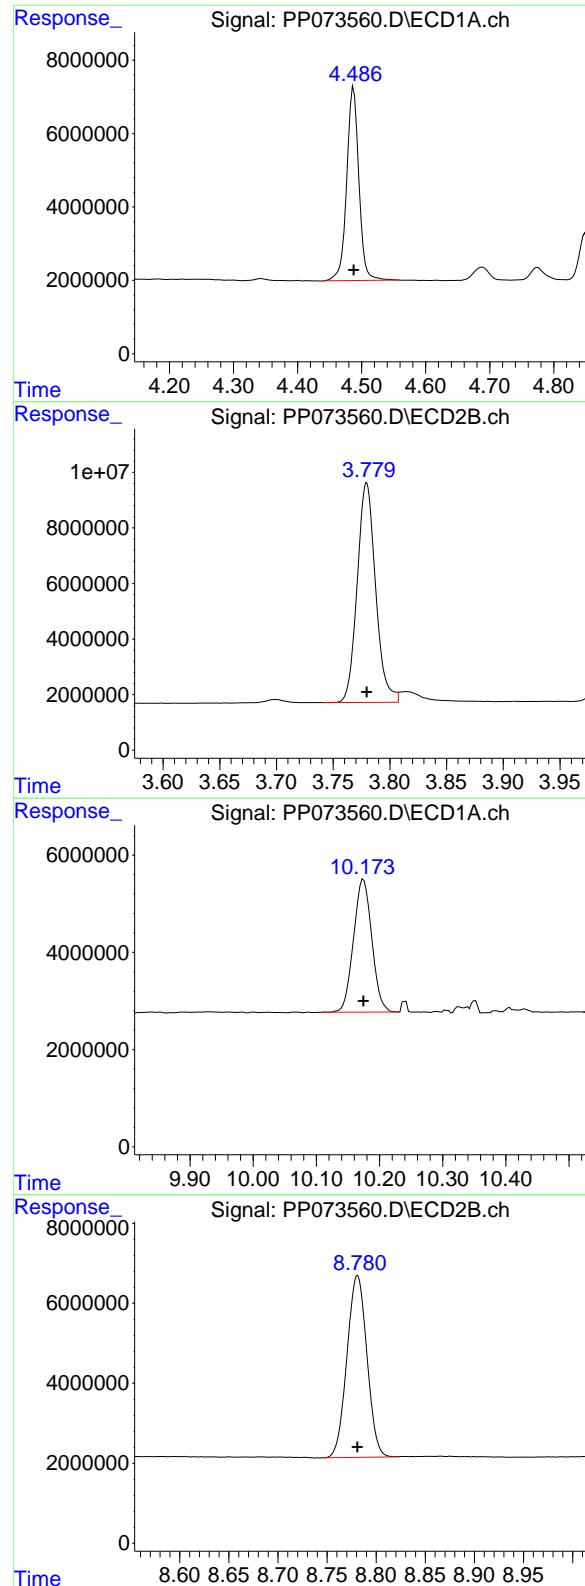

#1 Tetrachloro-m-xylene

R.T.: 4.488 min
 Delta R.T.: 0.000 min
 Response: 69747801
 Conc: 50.00 ng/ml

Instrument: ECD_P
ClientSampleId: AR1232ICC500

#1 Tetrachloro-m-xylene





R.T.: 3.779 min
 Delta R.T.: 0.000 min
 Response: 89329746
 Conc: 50.00 ng/ml

#2 Decachlorobiphenyl

R.T.: 10.175 min
 Delta R.T.: 0.000 min
 Response: 55031795
 Conc: 50.00 ng/ml

#2 Decachlorobiphenyl

R.T.: 8.781 min
 Delta R.T.: 0.000 min
 Response: 64481917
 Conc: 50.00 ng/ml

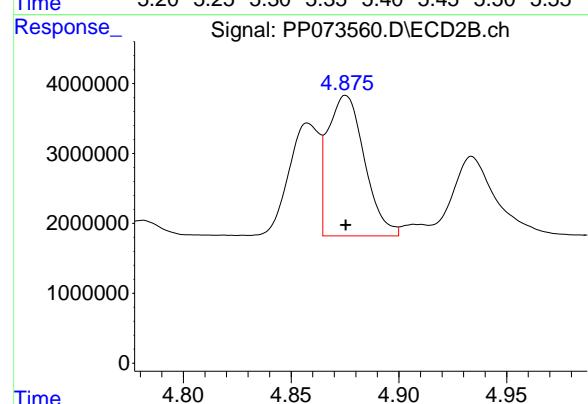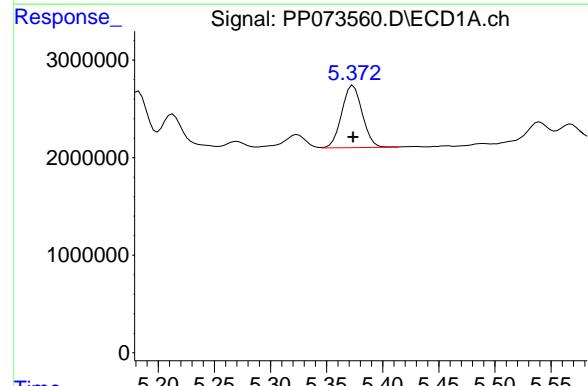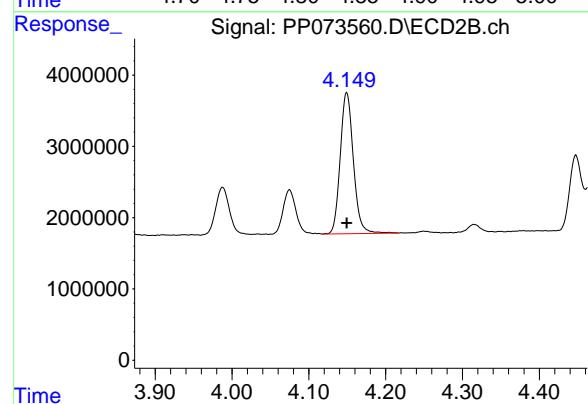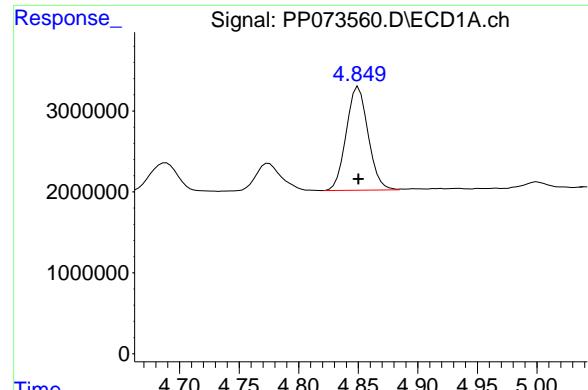

#11 AR-1232-1

R.T.: 4.850 min
Delta R.T.: 0.000 min
Response: 16325352
Conc: 500.00 ng/ml

Instrument: ECD_P
ClientSampleId: AR1232ICC500

#11 AR-1232-1





R.T.: 4.149 min
Delta R.T.: 0.000 min
Response: 23307175
Conc: 500.00 ng/ml

#12 AR-1232-2

R.T.: 5.374 min
Delta R.T.: 0.000 min
Response: 8127340
Conc: 500.00 ng/ml

#12 AR-1232-2

R.T.: 4.875 min
Delta R.T.: 0.000 min
Response: 23829904
Conc: 500.00 ng/ml

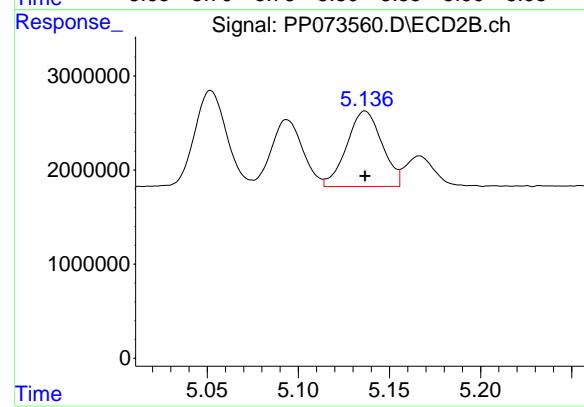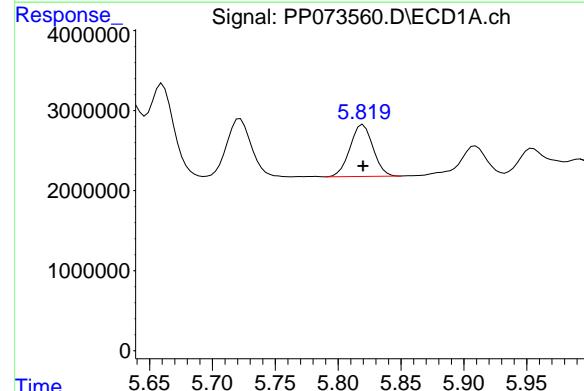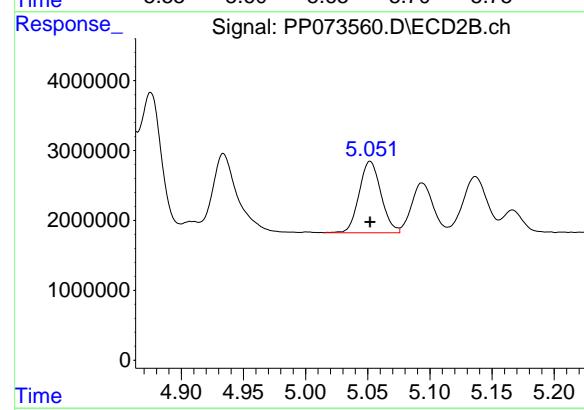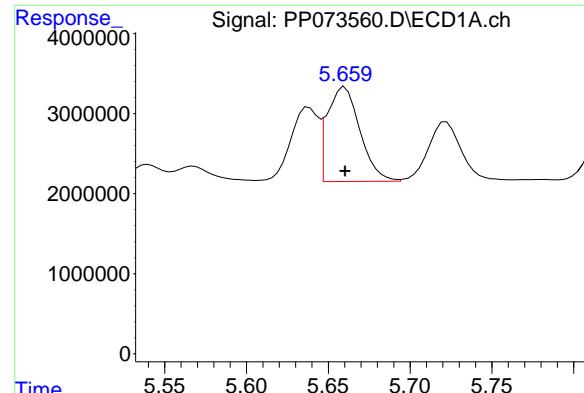

#13 AR-1232-3

R.T.: 5.660 min
 Delta R.T.: 0.000 min
 Response: 16496729
 Conc: 500.00 ng/ml

Instrument: ECD_P
ClientSampleId: AR1232ICC500

#13 AR-1232-3

R.T.: 5.052 min
 Delta R.T.: 0.000 min
 Response: 12514513
 Conc: 500.00 ng/ml

#14 AR-1232-4

R.T.: 5.820 min
 Delta R.T.: 0.000 min
 Response: 8222579
 Conc: 500.00 ng/ml



#14 AR-1232-4

R.T.: 5.137 min
 Delta R.T.: 0.000 min
 Response: 10828145
 Conc: 500.00 ng/ml

#15 AR-1232-5

R.T.: 5.909 min
Delta R.T.: 0.000 min
Response: 5285179
Conc: 500.00 ng/ml

Instrument: ECD_P
ClientSampleId: AR1232ICC500

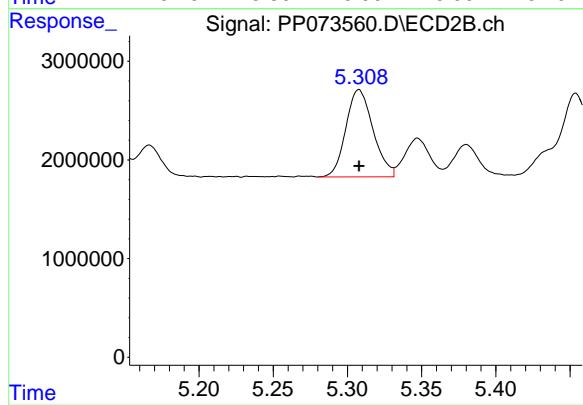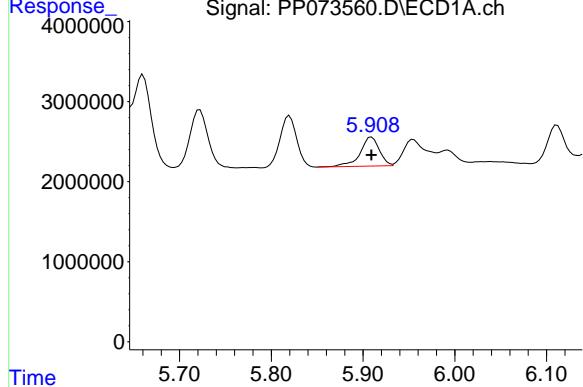

#15 AR-1232-5

R.T.: 5.308 min
Delta R.T.: 0.000 min
Response: 11281724
Conc: 500.00 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP070825\
 Data File : PP073561.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Jul 2025 22:57
 Operator : YP\AJ
 Sample : AR1242ICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
AR1242ICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 08 02:03:57 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 08 02:03:06 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	4.489	3.779	133.6E6	178.7E6	93.639	94.390
2) SA Decachlor...	10.177	8.779	109.6E6	130.7E6	95.735	96.573

Target Compounds

16) L4 AR-1242-1	5.639	4.857	37824570	53636877	927.891	888.918
17) L4 AR-1242-2	5.661	4.874	59433539	81745742	941.383	919.241
18) L4 AR-1242-3	5.723	5.051	35307728	43191003	927.513	907.757
19) L4 AR-1242-4	5.820	5.135	29431539	40719317	927.311	902.527
20) L4 AR-1242-5	6.549	5.656	31742412	53173633	951.704	931.769



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP070825\
 Data File : PP073561.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Jul 2025 22:57
 Operator : YP\AJ
 Sample : AR1242ICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
AR1242ICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 08 02:03:57 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 08 02:03:06 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ m Signal #2 Info : 30M x 0.32mm x 0.25 μ m

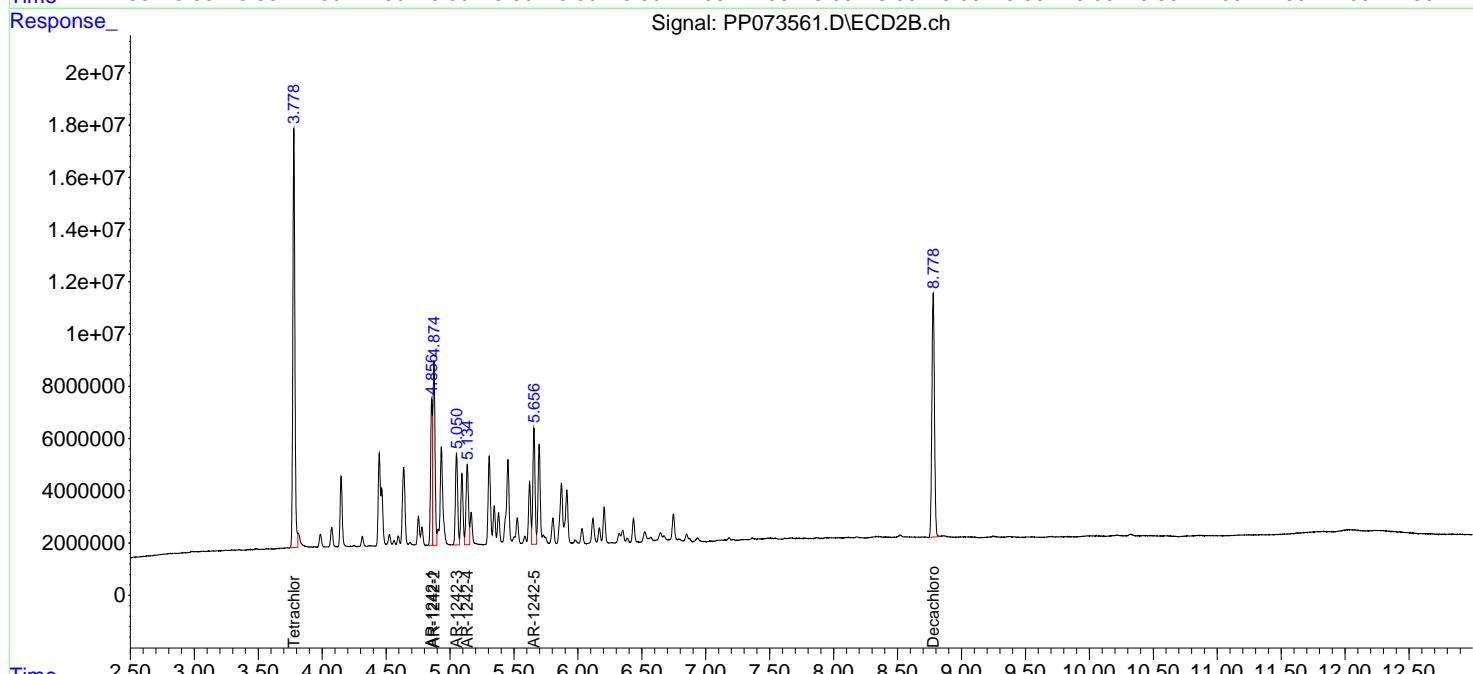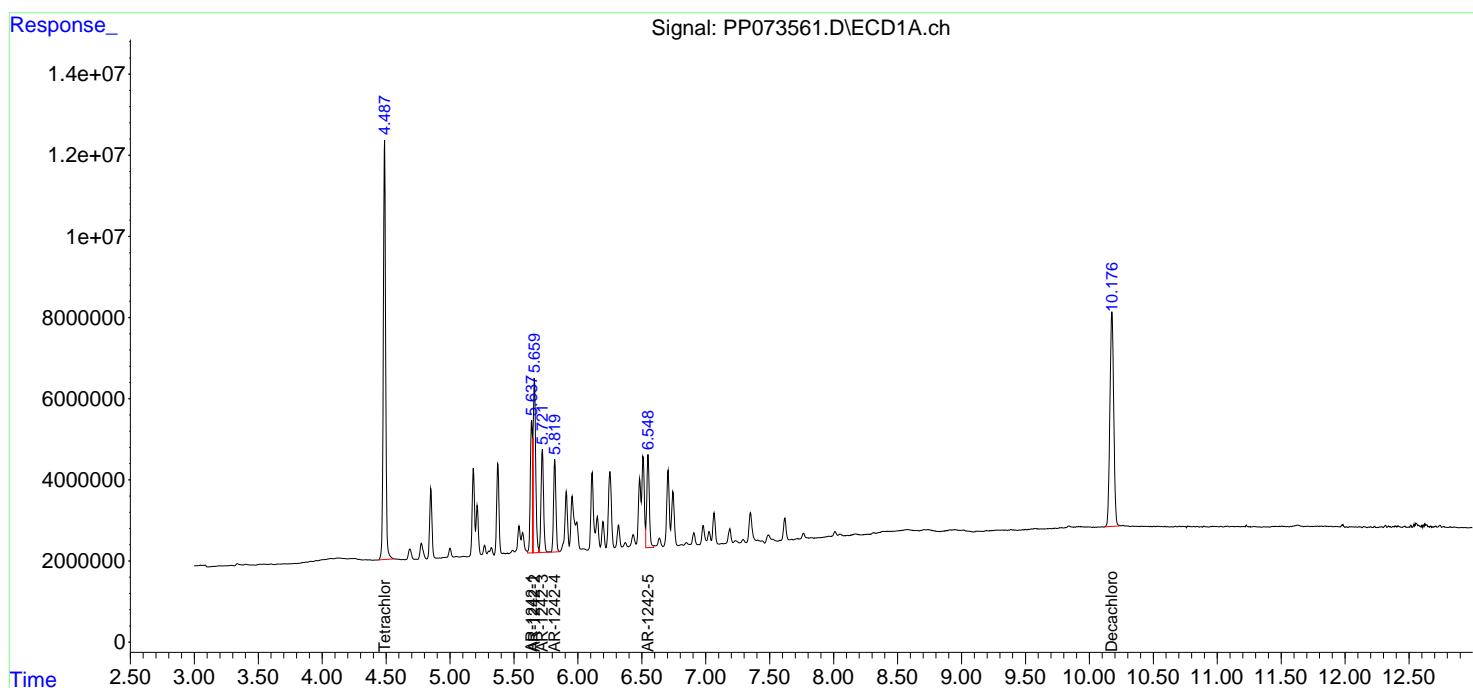

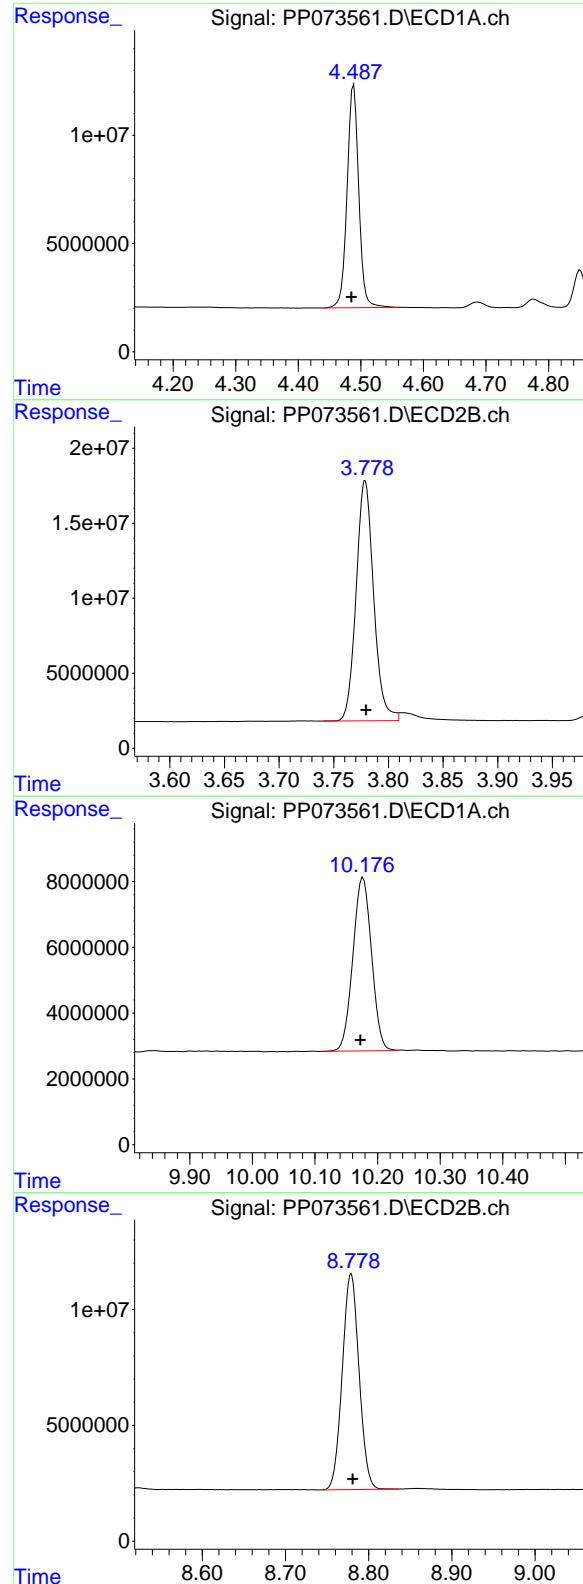

#1 Tetrachloro-m-xylene

R.T.: 4.489 min
 Delta R.T.: 0.004 min
 Response: 133642467
 Conc: 93.64 ng/ml

Instrument : ECD_P

ClientSampleId : AR1242ICC1000

#1 Tetrachloro-m-xylene

R.T.: 3.779 min
 Delta R.T.: 0.000 min
 Response: 178724092
 Conc: 94.39 ng/ml

#2 Decachlorobiphenyl

R.T.: 10.177 min
 Delta R.T.: 0.004 min
 Response: 109570314
 Conc: 95.73 ng/ml


#2 Decachlorobiphenyl

R.T.: 8.779 min
 Delta R.T.: -0.002 min
 Response: 130664248
 Conc: 96.57 ng/ml

#16 AR-1242-1


R.T.: 5.639 min
 Delta R.T.: 0.003 min
 Response: 37824570
 Conc: 927.89 ng/ml

Instrument: ECD_P
ClientSampleId: AR1242ICC1000

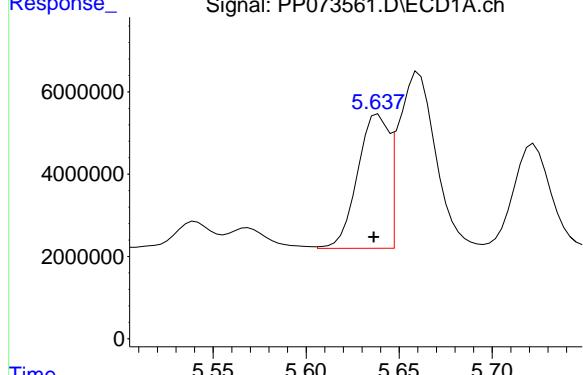


#16 AR-1242-1

R.T.: 4.857 min
 Delta R.T.: -0.001 min
 Response: 53636877
 Conc: 888.92 ng/ml

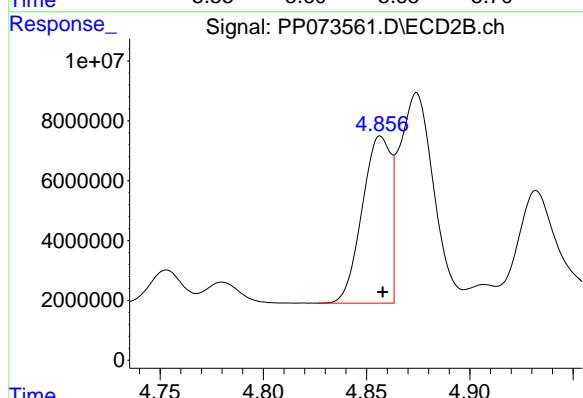


#17 AR-1242-2

R.T.: 5.661 min
 Delta R.T.: 0.003 min
 Response: 59433539
 Conc: 941.38 ng/ml

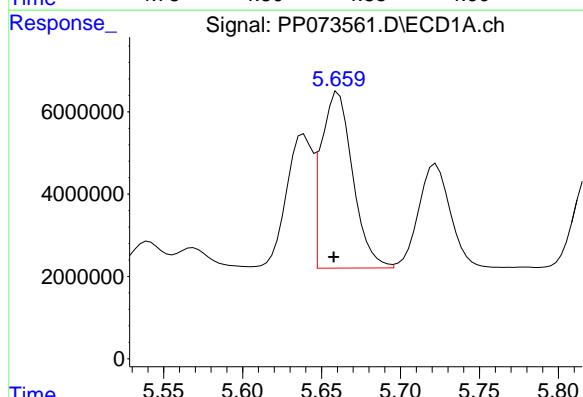

#17 AR-1242-2





R.T.: 4.874 min
 Delta R.T.: -0.001 min
 Response: 81745742
 Conc: 919.24 ng/ml

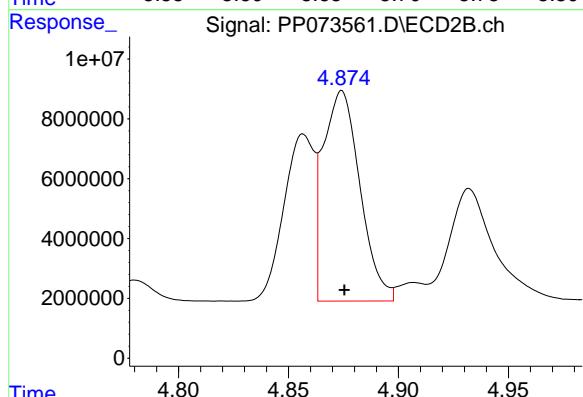

#18 AR-1242-3

R.T.: 5.723 min
 Delta R.T.: 0.003 min
 Response: 35307728
 Conc: 927.51 ng/ml

Instrument: ECD_P
ClientSampleId: AR1242ICC1000

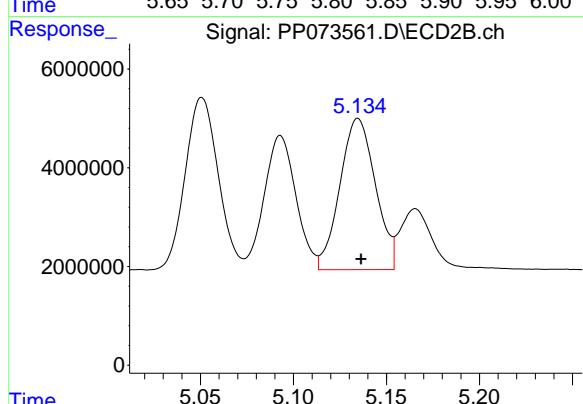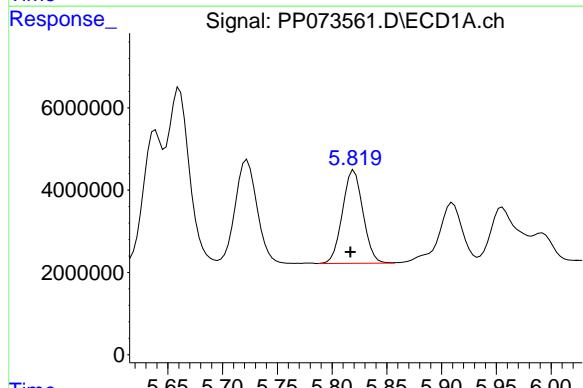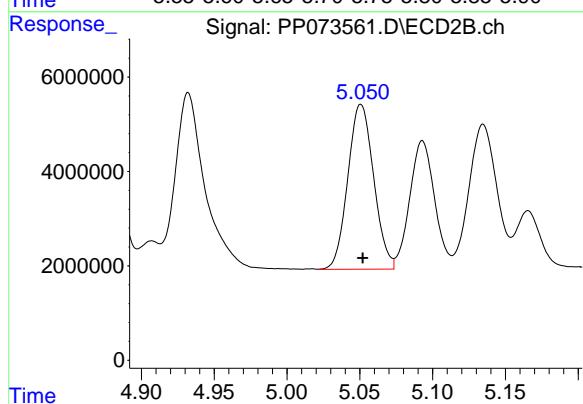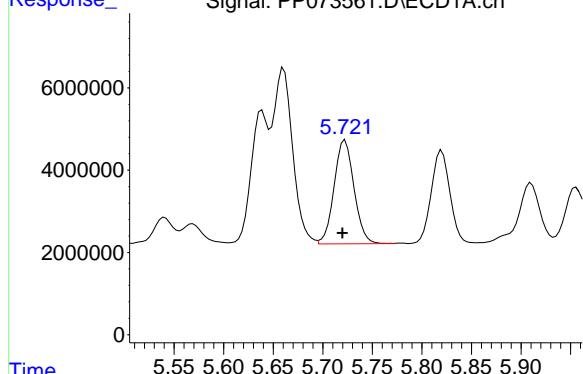

#18 AR-1242-3

R.T.: 5.051 min
 Delta R.T.: -0.001 min
 Response: 43191003
 Conc: 907.76 ng/ml

#19 AR-1242-4

R.T.: 5.820 min
 Delta R.T.: 0.003 min
 Response: 29431539
 Conc: 927.31 ng/ml



#19 AR-1242-4

R.T.: 5.135 min
 Delta R.T.: -0.002 min
 Response: 40719317
 Conc: 902.53 ng/ml

#20 AR-1242-5

R.T.: 6.549 min
Delta R.T.: 0.003 min
Response: 31742412
Conc: 951.70 ng/ml

Instrument: ECD_P
ClientSampleId: AR1242ICC1000

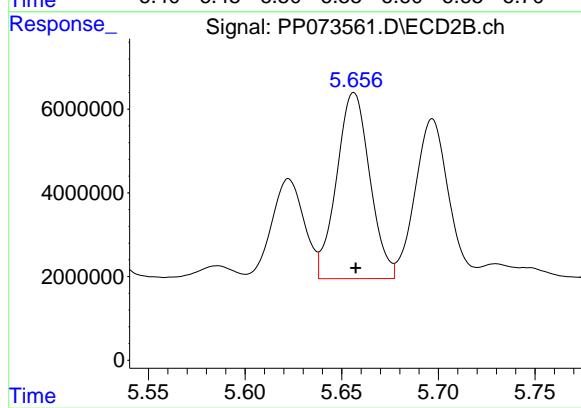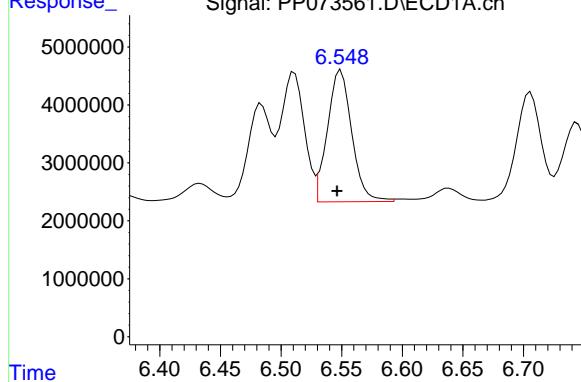

#20 AR-1242-5

R.T.: 5.656 min
Delta R.T.: 0.000 min
Response: 53173633
Conc: 931.77 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP070825\
 Data File : PP073562.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Jul 2025 23:14
 Operator : YP\AJ
 Sample : AR1242ICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
AR1242ICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 08 02:04:21 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 08 02:03:06 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	4.487	3.779	101.2E6	134.0E6	70.925	70.781
2) SA Decachlor...	10.176	8.781	83819765	102.7E6	73.236	75.941

Target Compounds

16) L4 AR-1242-1	5.637	4.858	28898659	42483367	708.926	704.072
17) L4 AR-1242-2	5.660	4.875	44240913	61742767	700.743	694.305
18) L4 AR-1242-3	5.721	5.051	26874126	33146056	705.967	696.639
19) L4 AR-1242-4	5.819	5.135	22658657	31400295	713.915	695.975
20) L4 AR-1242-5	6.548	5.657	23721271	40207089	711.214	704.555


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.





Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP070825\
 Data File : PP073562.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Jul 2025 23:14
 Operator : YP\AJ
 Sample : AR1242ICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
AR1242ICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 08 02:04:21 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 08 02:03:06 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ m Signal #2 Info : 30M x 0.32mm x 0.25 μ m

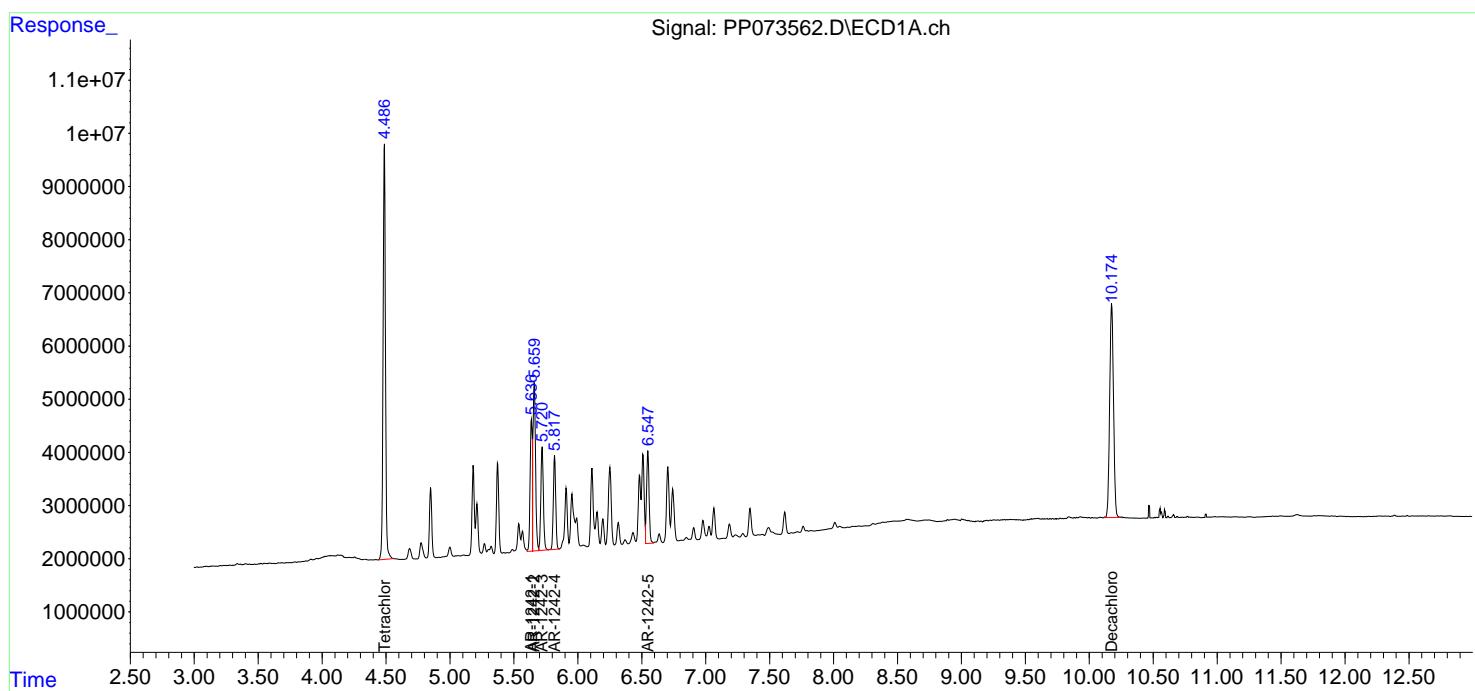

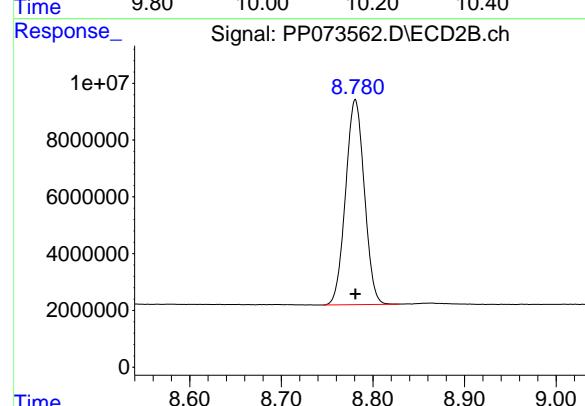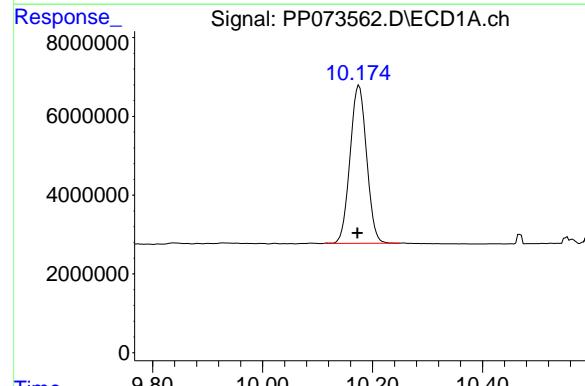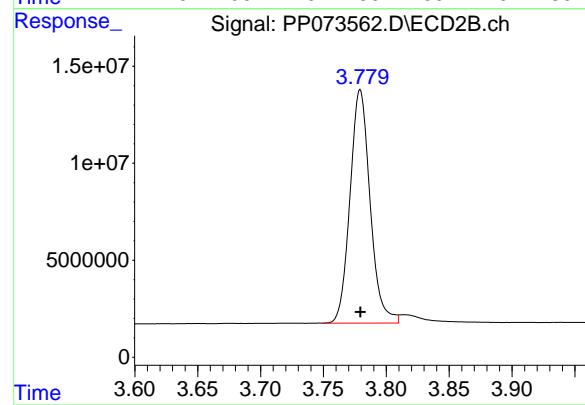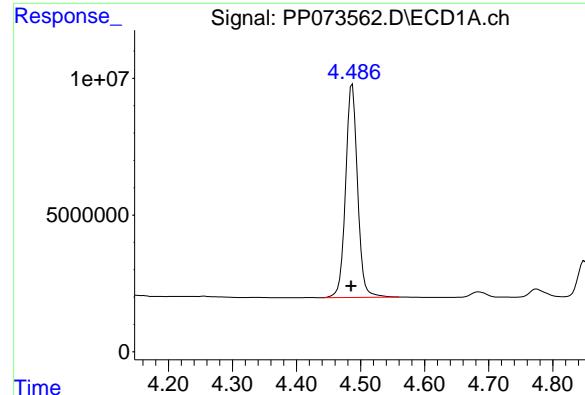

#1 Tetrachloro-m-xylene

R.T.: 4.487 min
Delta R.T.: 0.002 min
Response: 101224890
Conc: 70.92 ng/ml

Instrument: ECD_P
ClientSampleId: AR1242ICC750

#1 Tetrachloro-m-xylene

R.T.: 3.779 min
Delta R.T.: 0.000 min
Response: 134020280
Conc: 70.78 ng/ml

#2 Decachlorobiphenyl

R.T.: 10.176 min
Delta R.T.: 0.003 min
Response: 83819765
Conc: 73.24 ng/ml


#2 Decachlorobiphenyl

R.T.: 8.781 min
Delta R.T.: 0.000 min
Response: 102748919
Conc: 75.94 ng/ml

#16 AR-1242-1


R.T.: 5.637 min
 Delta R.T.: 0.001 min
 Response: 28898659
 Conc: 708.93 ng/ml

Instrument: ECD_P
 ClientSampleId: AR1242ICC750

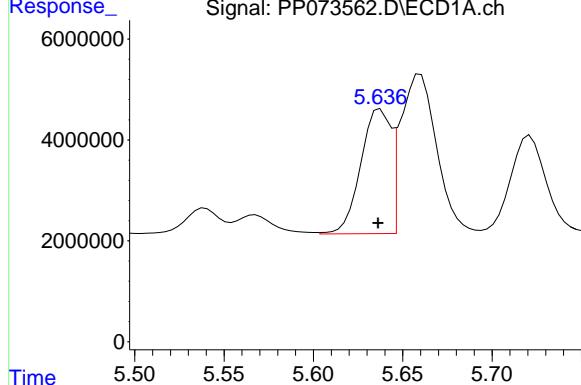


#16 AR-1242-1

R.T.: 4.858 min
 Delta R.T.: 0.000 min
 Response: 42483367
 Conc: 704.07 ng/ml

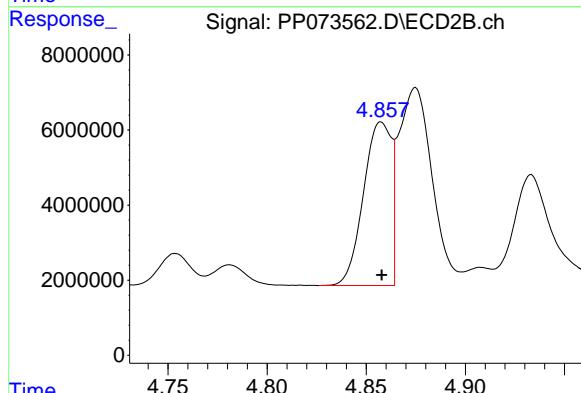


#17 AR-1242-2

R.T.: 5.660 min
 Delta R.T.: 0.002 min
 Response: 44240913
 Conc: 700.74 ng/ml

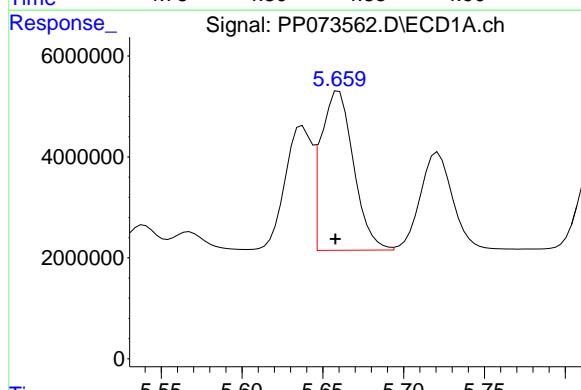

#17 AR-1242-2





R.T.: 4.875 min
 Delta R.T.: 0.000 min
 Response: 61742767
 Conc: 694.31 ng/ml

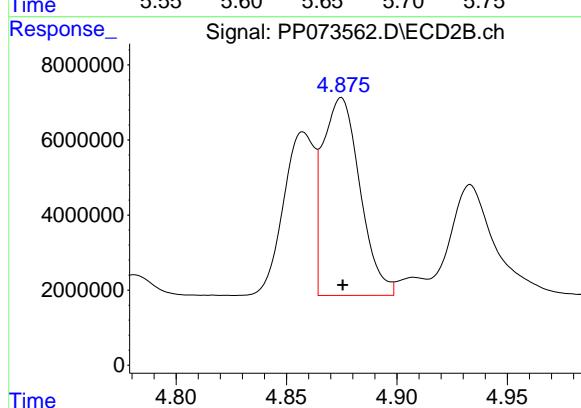

#18 AR-1242-3

R.T.: 5.721 min
 Delta R.T.: 0.002 min
 Response: 26874126
 Conc: 705.97 ng/ml

Instrument: ECD_P
ClientSampleId: AR1242ICC750

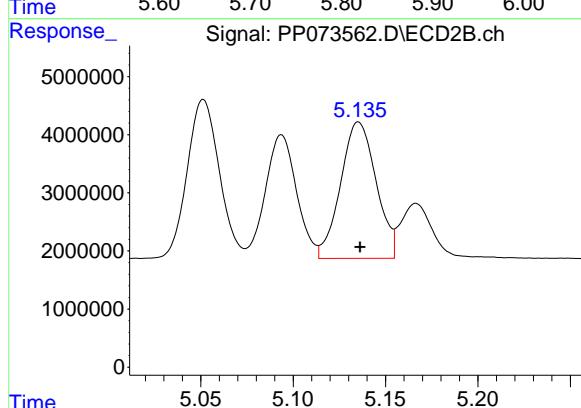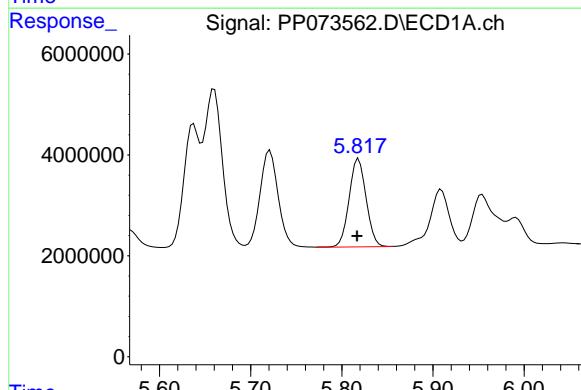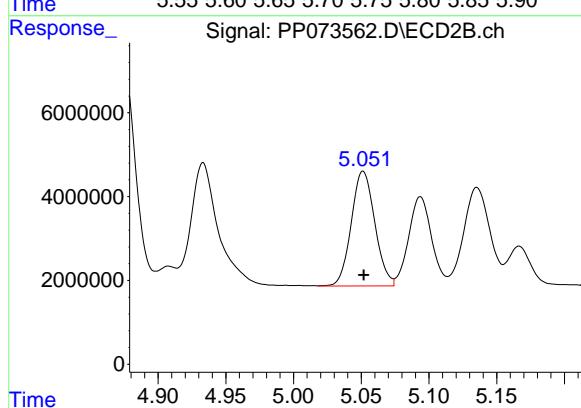

#18 AR-1242-3


R.T.: 5.051 min
 Delta R.T.: 0.000 min
 Response: 33146056
 Conc: 696.64 ng/ml

#19 AR-1242-4

R.T.: 5.819 min
 Delta R.T.: 0.002 min
 Response: 22658657
 Conc: 713.91 ng/ml

#19 AR-1242-4

R.T.: 5.135 min
 Delta R.T.: 0.000 min
 Response: 31400295
 Conc: 695.97 ng/ml

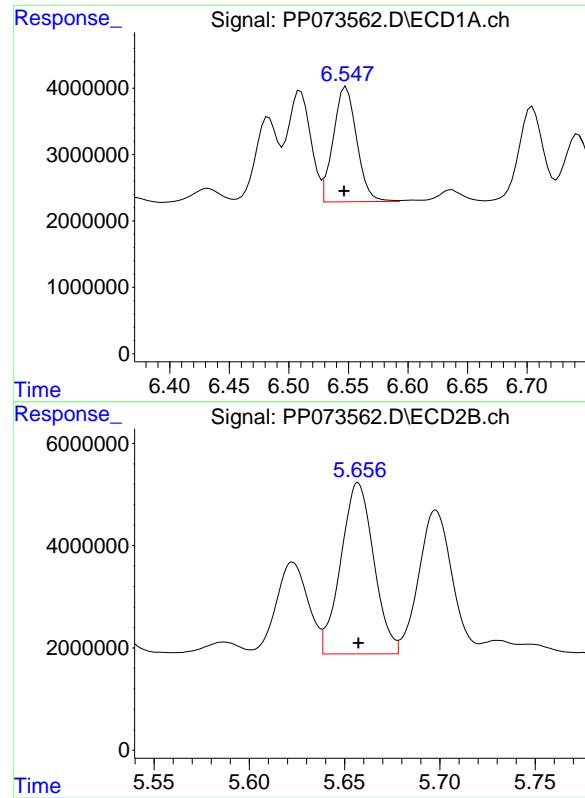

#20 AR-1242-5

R.T.: 6.548 min
Delta R.T.: 0.002 min
Response: 23721271
Conc: 711.21 ng/ml

Instrument: ECD_P
ClientSampleId: AR1242ICC750

#20 AR-1242-5

R.T.: 5.657 min
Delta R.T.: 0.000 min
Response: 40207089
Conc: 704.55 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP070825\
 Data File : PP073563.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Jul 2025 23:30
 Operator : YP\AJ
 Sample : AR1242ICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
AR1242ICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 08 02:04:41 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 08 02:03:06 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	4.485	3.779	71360618	94672779	50.000	50.000
2) SA Decachlor...	10.173	8.781	57225953	67650592	50.000	50.000

Target Compounds

16) L4 AR-1242-1	5.636	4.858	20382014	30169740	500.000	500.000
17) L4 AR-1242-2	5.658	4.875	31567127	44463701	500.000	500.000
18) L4 AR-1242-3	5.720	5.052	19033543	23789965	500.000	500.000
19) L4 AR-1242-4	5.817	5.136	15869296	22558507	500.000	500.000
20) L4 AR-1242-5	6.546	5.657	16676614	28533697	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.





Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP070825\
 Data File : PP073563.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Jul 2025 23:30
 Operator : YP\AJ
 Sample : AR1242ICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
AR1242ICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 08 02:04:41 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 08 02:03:06 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ m Signal #2 Info : 30M x 0.32mm x 0.25 μ m

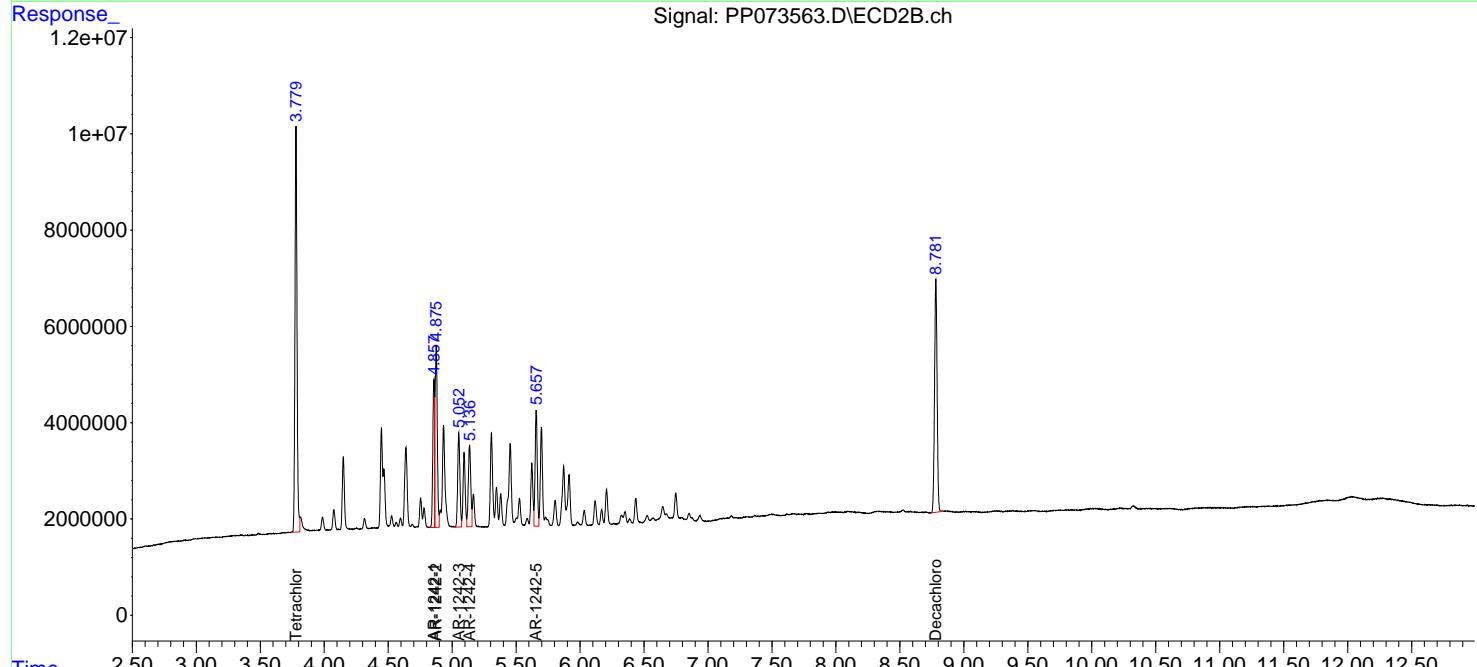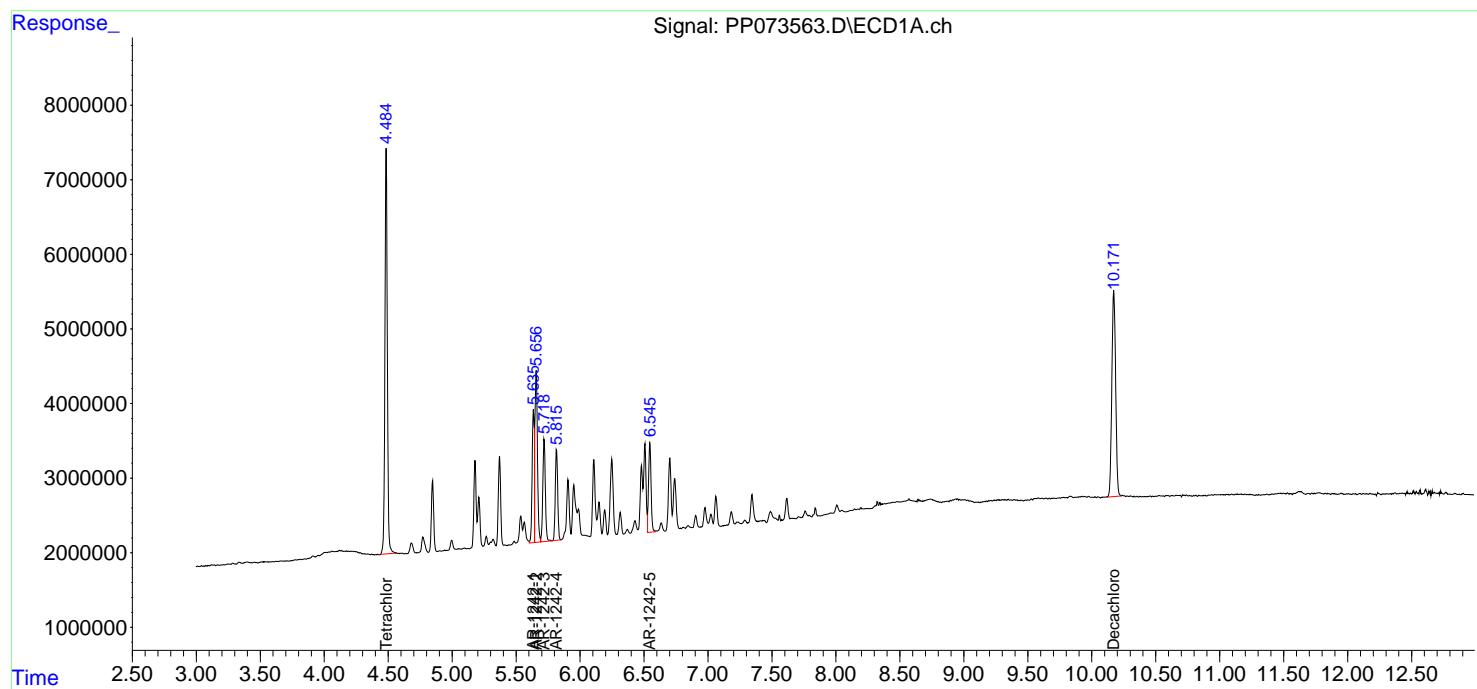

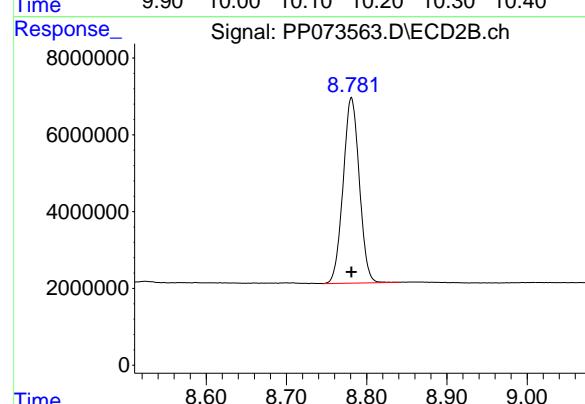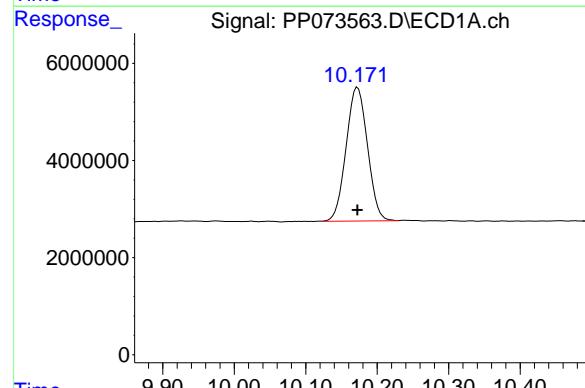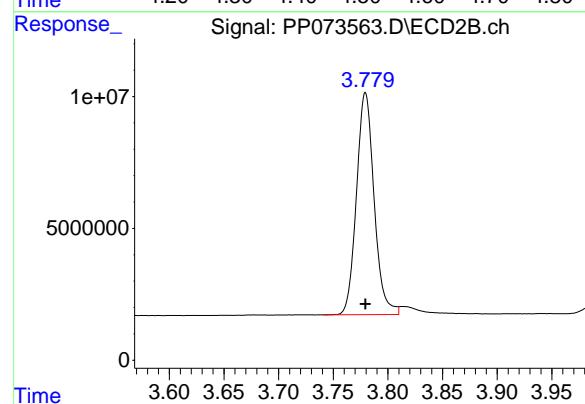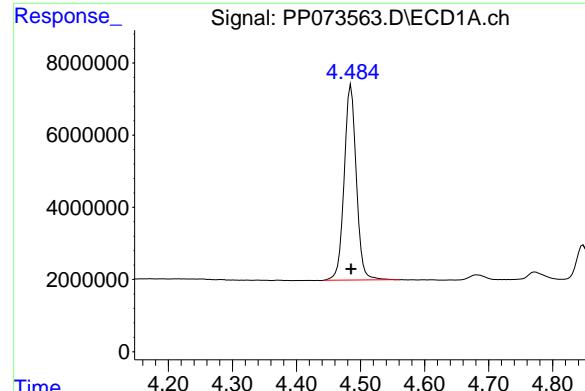

#1 Tetrachloro-m-xylene

R.T.: 4.485 min
 Delta R.T.: 0.000 min
 Response: 71360618
 Conc: 50.00 ng/ml

Instrument: ECD_P
ClientSampleId: AR1242ICC500

#1 Tetrachloro-m-xylene

R.T.: 3.779 min
 Delta R.T.: 0.000 min
 Response: 94672779
 Conc: 50.00 ng/ml


#2 Decachlorobiphenyl

R.T.: 10.173 min
 Delta R.T.: 0.000 min
 Response: 57225953
 Conc: 50.00 ng/ml

#2 Decachlorobiphenyl

R.T.: 8.781 min
 Delta R.T.: 0.000 min
 Response: 67650592
 Conc: 50.00 ng/ml

#16 AR-1242-1

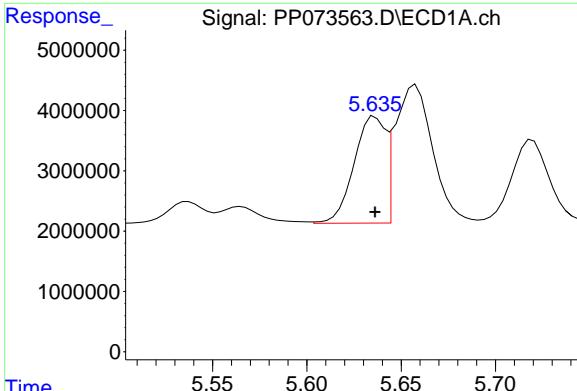


R.T.: 5.636 min
Delta R.T.: 0.000 min
Response: 20382014
Conc: 500.00 ng/ml

Instrument: ECD_P
ClientSampleId: AR1242ICC500


#16 AR-1242-1

R.T.: 4.858 min
Delta R.T.: 0.000 min
Response: 30169740
Conc: 500.00 ng/ml

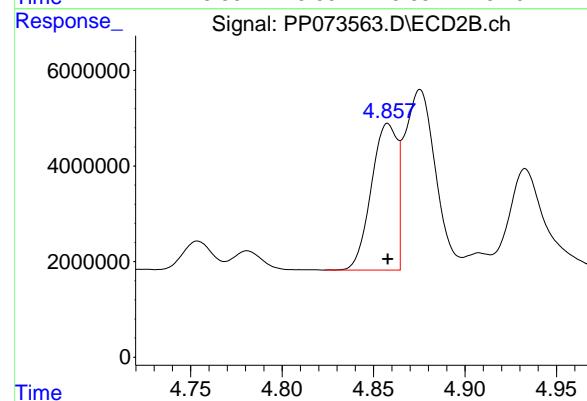


#17 AR-1242-2

R.T.: 5.658 min
Delta R.T.: 0.000 min
Response: 31567127
Conc: 500.00 ng/ml

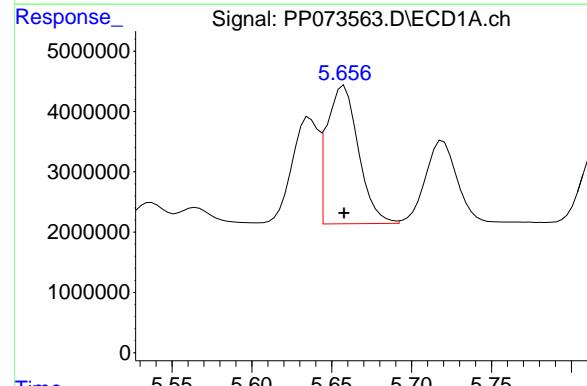

#17 AR-1242-2


R.T.: 4.875 min
Delta R.T.: 0.000 min
Response: 44463701
Conc: 500.00 ng/ml

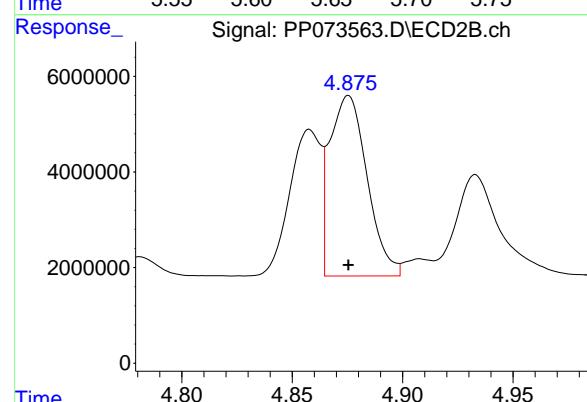

#18 AR-1242-3


R.T.: 5.720 min
 Delta R.T.: 0.000 min
 Response: 19033543
 Conc: 500.00 ng/ml

Instrument: ECD_P
ClientSampleId: AR1242ICC500

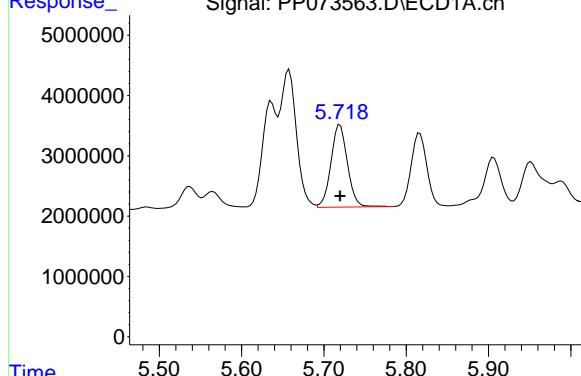


#18 AR-1242-3

R.T.: 5.052 min
 Delta R.T.: 0.000 min
 Response: 23789965
 Conc: 500.00 ng/ml

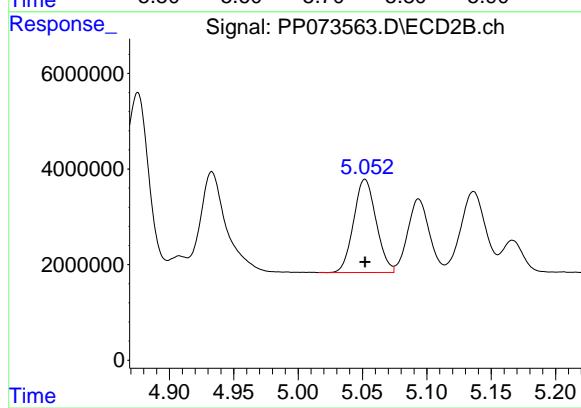


#19 AR-1242-4


R.T.: 5.817 min
 Delta R.T.: 0.000 min
 Response: 15869296
 Conc: 500.00 ng/ml

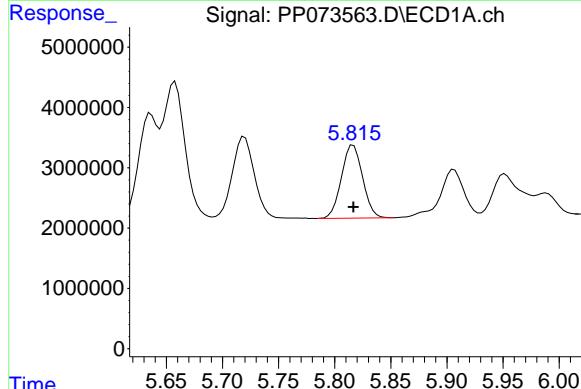

#19 AR-1242-4

R.T.: 5.136 min
 Delta R.T.: 0.000 min
 Response: 22558507
 Conc: 500.00 ng/ml

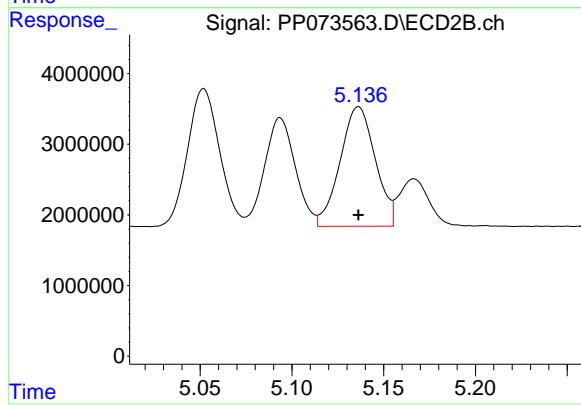

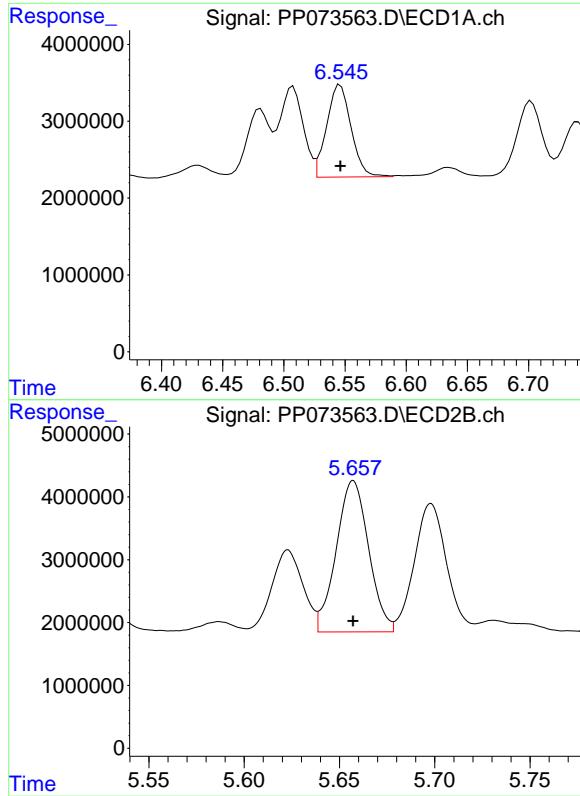

#20 AR-1242-5

R.T.: 6.546 min
Delta R.T.: 0.000 min
Response: 16676614
Conc: 500.00 ng/ml

Instrument: ECD_P
ClientSampleId: AR1242ICC500

#20 AR-1242-5

R.T.: 5.657 min
Delta R.T.: 0.000 min
Response: 28533697
Conc: 500.00 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP070825\
 Data File : PP073564.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Jul 2025 23:46
 Operator : YP\AJ
 Sample : AR1242ICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
AR1242ICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 08 02:05:02 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 08 02:03:06 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	4.488	3.779	35973232	49943783	25.205	26.377
2) SA Decachlor...	10.176	8.781	28867365	35186918	25.222	26.006

Target Compounds

16) L4 AR-1242-1	5.638	4.857	10586937	15530210	259.713	257.381
17) L4 AR-1242-2	5.660	4.875	16251959	22939126	257.419	257.953
18) L4 AR-1242-3	5.722	5.051	9827935	12210872	258.174	256.639
19) L4 AR-1242-4	5.819	5.135	8068875	11715170	254.229	259.662
20) L4 AR-1242-5	6.550	5.656	8772262	14646179	263.011	256.647


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.





Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP070825\
 Data File : PP073564.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Jul 2025 23:46
 Operator : YP\AJ
 Sample : AR1242ICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
AR1242ICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 08 02:05:02 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 08 02:03:06 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ m Signal #2 Info : 30M x 0.32mm x 0.25 μ m

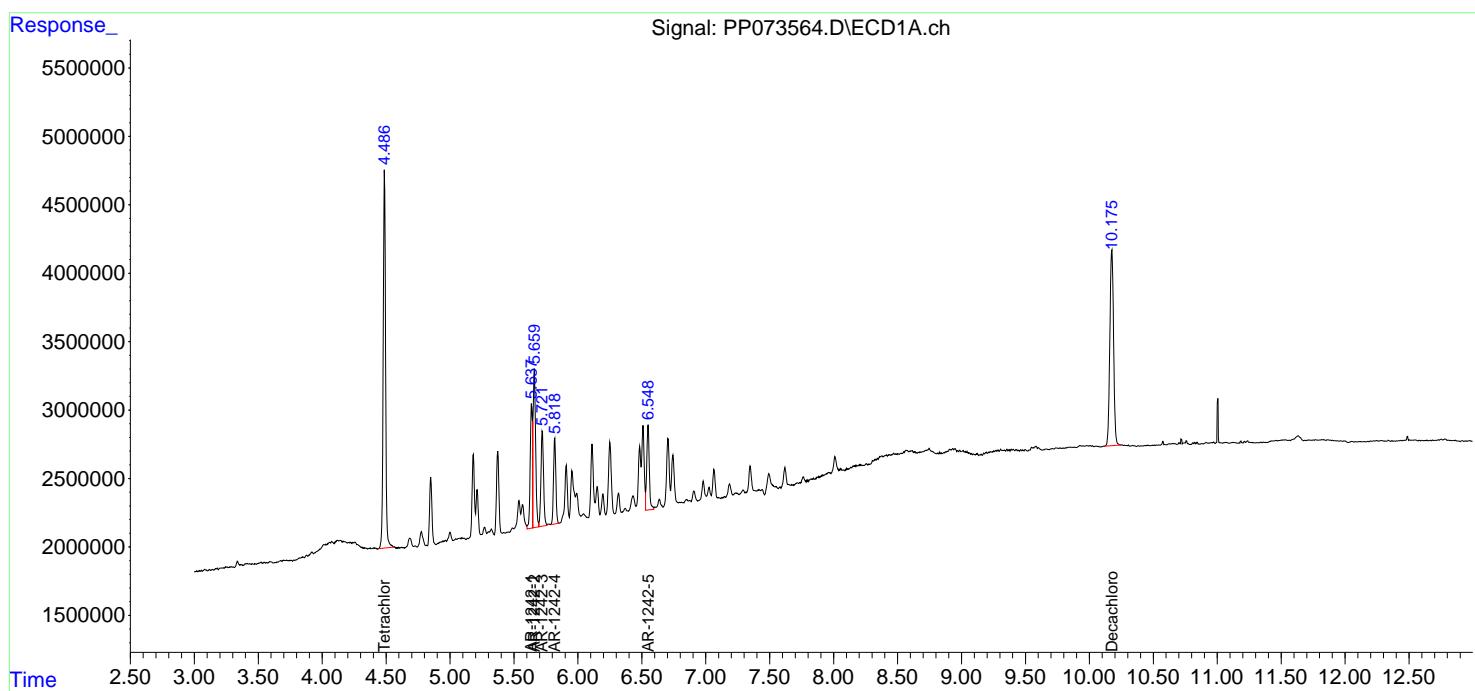

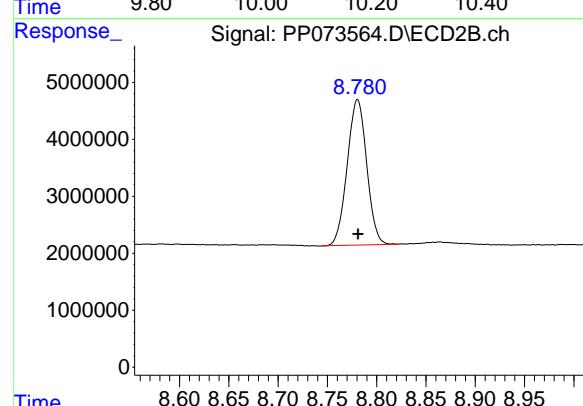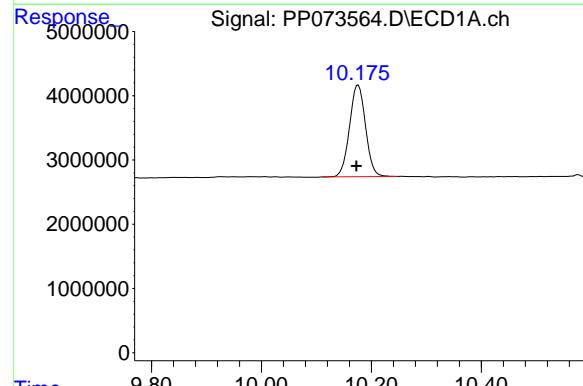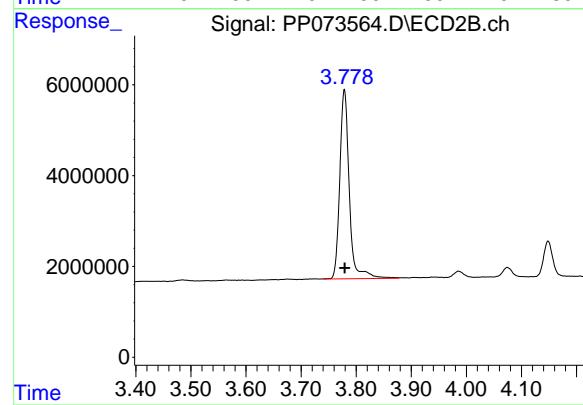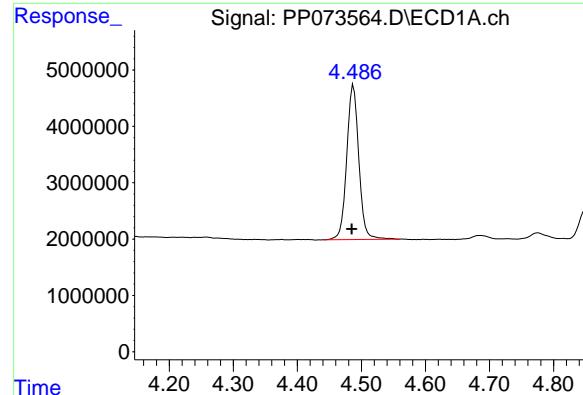

#1 Tetrachloro-m-xylene

R.T.: 4.488 min
 Delta R.T.: 0.003 min
 Response: 35973232
 Conc: 25.21 ng/ml

Instrument: ECD_P
ClientSampleId: AR1242ICC250

#1 Tetrachloro-m-xylene

R.T.: 3.779 min
 Delta R.T.: 0.000 min
 Response: 49943783
 Conc: 26.38 ng/ml

#2 Decachlorobiphenyl

R.T.: 10.176 min
 Delta R.T.: 0.003 min
 Response: 28867365
 Conc: 25.22 ng/ml


#2 Decachlorobiphenyl

R.T.: 8.781 min
 Delta R.T.: 0.000 min
 Response: 35186918
 Conc: 26.01 ng/ml

#16 AR-1242-1


R.T.: 5.638 min
 Delta R.T.: 0.002 min
 Response: 10586937
 Conc: 259.71 ng/ml

Instrument: ECD_P
ClientSampleId: AR1242ICC250

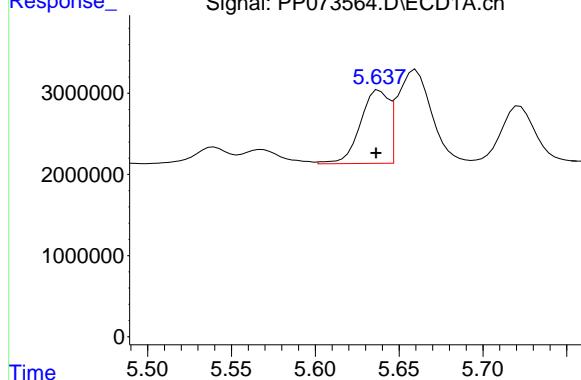


#16 AR-1242-1

R.T.: 4.857 min
 Delta R.T.: 0.000 min
 Response: 15530210
 Conc: 257.38 ng/ml

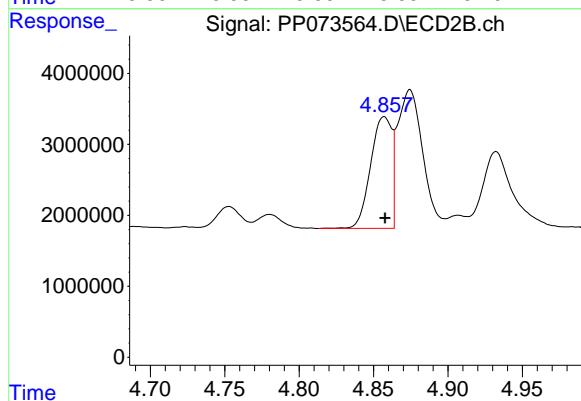


#17 AR-1242-2

R.T.: 5.660 min
 Delta R.T.: 0.002 min
 Response: 16251959
 Conc: 257.42 ng/ml

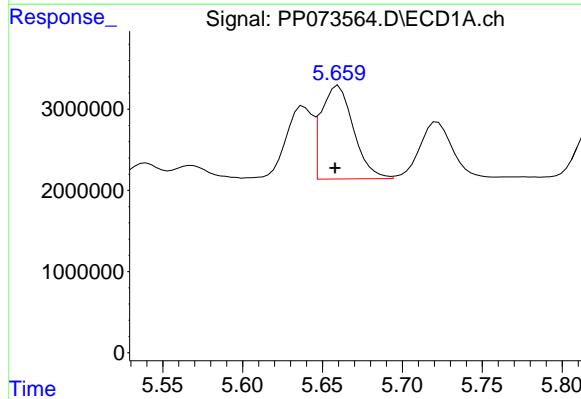

#17 AR-1242-2





R.T.: 4.875 min
 Delta R.T.: 0.000 min
 Response: 22939126
 Conc: 257.95 ng/ml

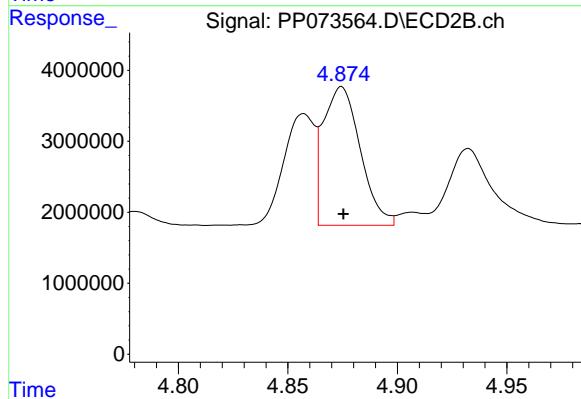

#18 AR-1242-3

R.T.: 5.722 min
 Delta R.T.: 0.002 min
 Response: 9827935
 Conc: 258.17 ng/ml

Instrument: ECD_P
ClientSampleId: AR1242ICC250

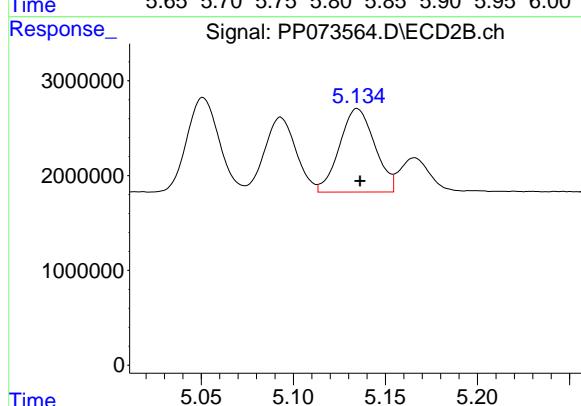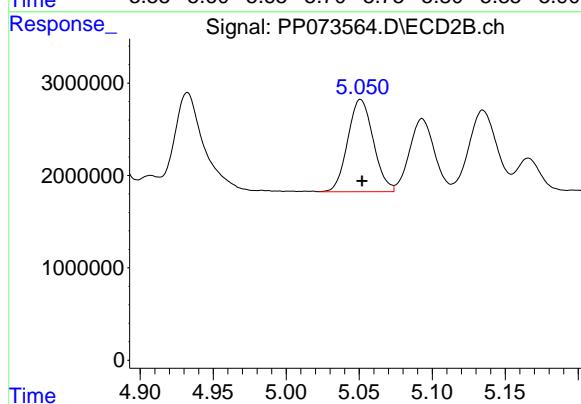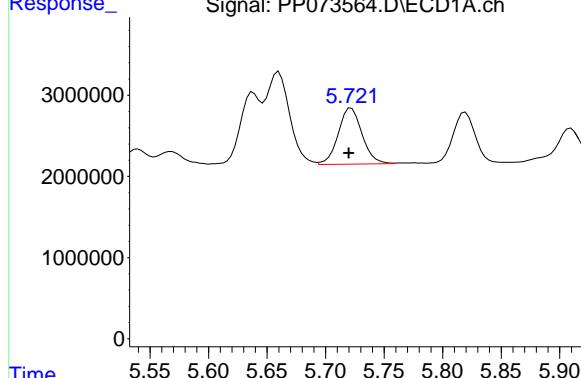

#18 AR-1242-3

R.T.: 5.051 min
 Delta R.T.: -0.001 min
 Response: 12210872
 Conc: 256.64 ng/ml

#19 AR-1242-4

R.T.: 5.819 min
 Delta R.T.: 0.003 min
 Response: 8068875
 Conc: 254.23 ng/ml



#19 AR-1242-4

R.T.: 5.135 min
 Delta R.T.: -0.002 min
 Response: 11715170
 Conc: 259.66 ng/ml

#20 AR-1242-5

R.T.: 6.550 min
Delta R.T.: 0.003 min
Response: 8772262
Conc: 263.01 ng/ml

Instrument: ECD_P
ClientSampleId: AR1242ICC250

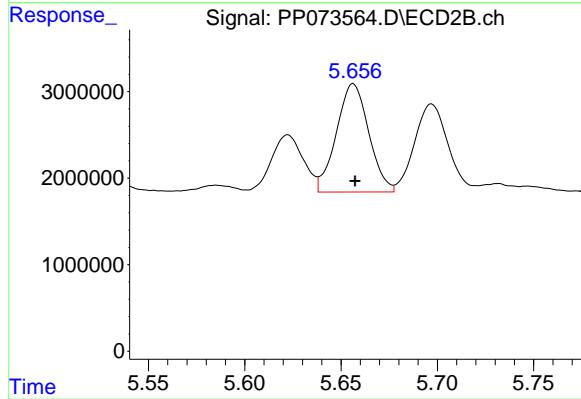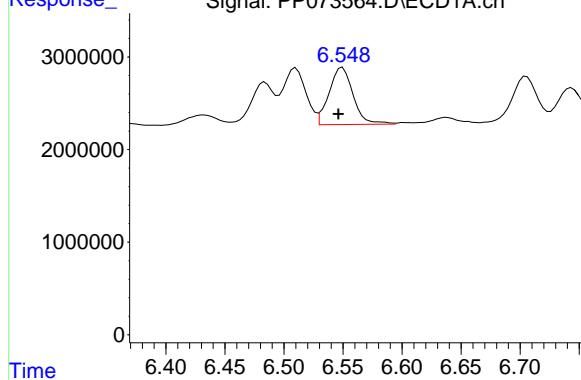

#20 AR-1242-5

R.T.: 5.656 min
Delta R.T.: 0.000 min
Response: 14646179
Conc: 256.65 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP070825\
 Data File : PP073565.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jul 2025 00:03
 Operator : YP\AJ
 Sample : AR1242ICC050
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
AR1242ICC050

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/08/2025
 Supervised By :mohammad ahmed 07/09/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 08 02:05:27 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 08 02:03:06 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	4.487	3.779	6312847	8330986	4.423	4.400
2) SA Decachlor...	10.173	8.780	4963140	5974096	4.336	4.415

Target Compounds

16) L4 AR-1242-1	5.636	4.857	1573661	2804106	38.604m	46.472
17) L4 AR-1242-2	5.657	4.875	2642334	4375880	41.853m	49.207
18) L4 AR-1242-3	5.720	5.052	1729292	2296207	45.427m	48.260
19) L4 AR-1242-4	5.818	5.136	1851147	2337623	58.325	51.812
20) L4 AR-1242-5	6.546	5.657	1593566	2688857	47.778m	47.117

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP070825\
 Data File : PP073565.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jul 2025 00:03
 Operator : YP\AJ
 Sample : AR1242ICC050
 Misc :
 ALS Vial : 14 Sample Multiplier: 1


Instrument :
 ECD_P
 ClientSampleId :
 AR1242ICC050


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/08/2025
 Supervised By :mohammad ahmed 07/09/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 08 02:05:27 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 08 02:03:06 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

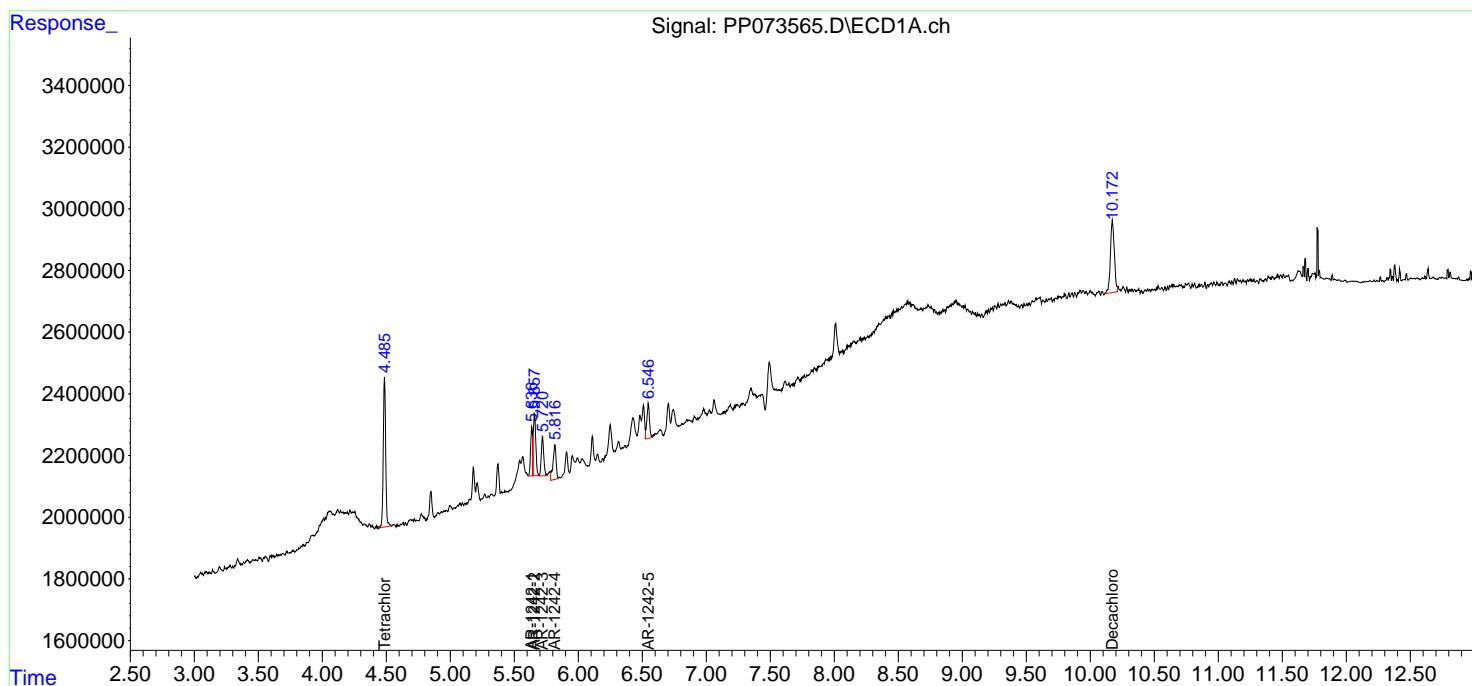

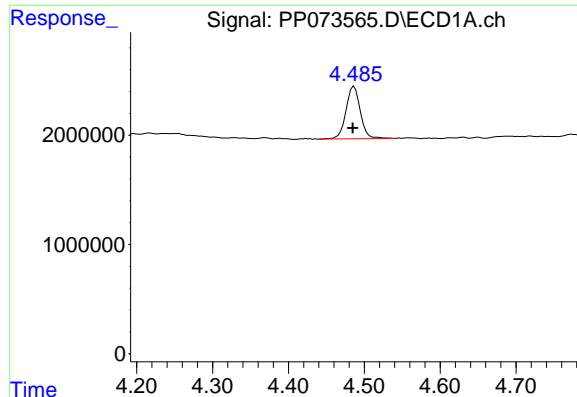


#1 Tetrachloro-m-xylene

R.T.: 4.487 min
Delta R.T.: 0.002 min
Response: 6312847
Conc: 4.42 ng/ml

Instrument: ECD_P
ClientSampleId: AR1242ICC050


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/08/2025
Supervised By :mohammad ahmed 07/09/2025

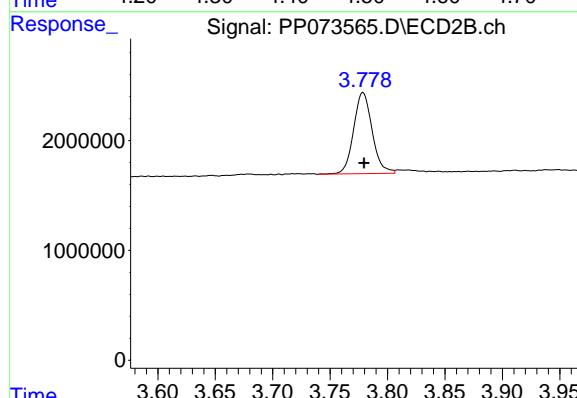


#1 Tetrachloro-m-xylene

R.T.: 3.779 min
Delta R.T.: 0.000 min
Response: 8330986
Conc: 4.40 ng/ml

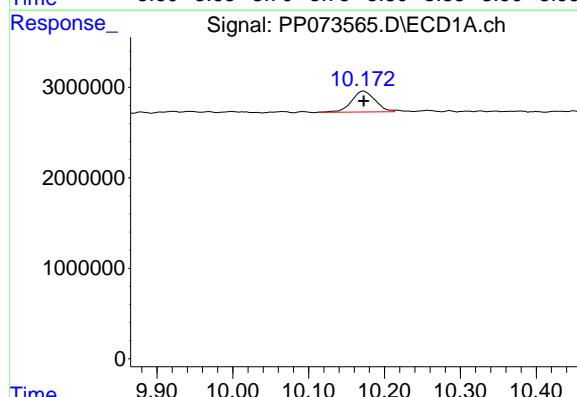


#2 Decachlorobiphenyl

R.T.: 10.173 min
Delta R.T.: 0.000 min
Response: 4963140
Conc: 4.34 ng/ml

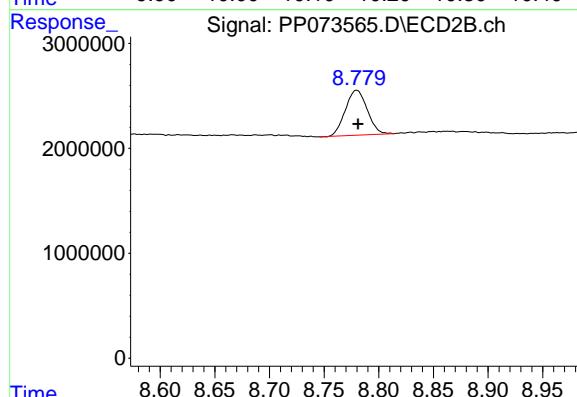

#2 Decachlorobiphenyl

R.T.: 8.780 min
Delta R.T.: -0.001 min
Response: 5974096
Conc: 4.42 ng/ml

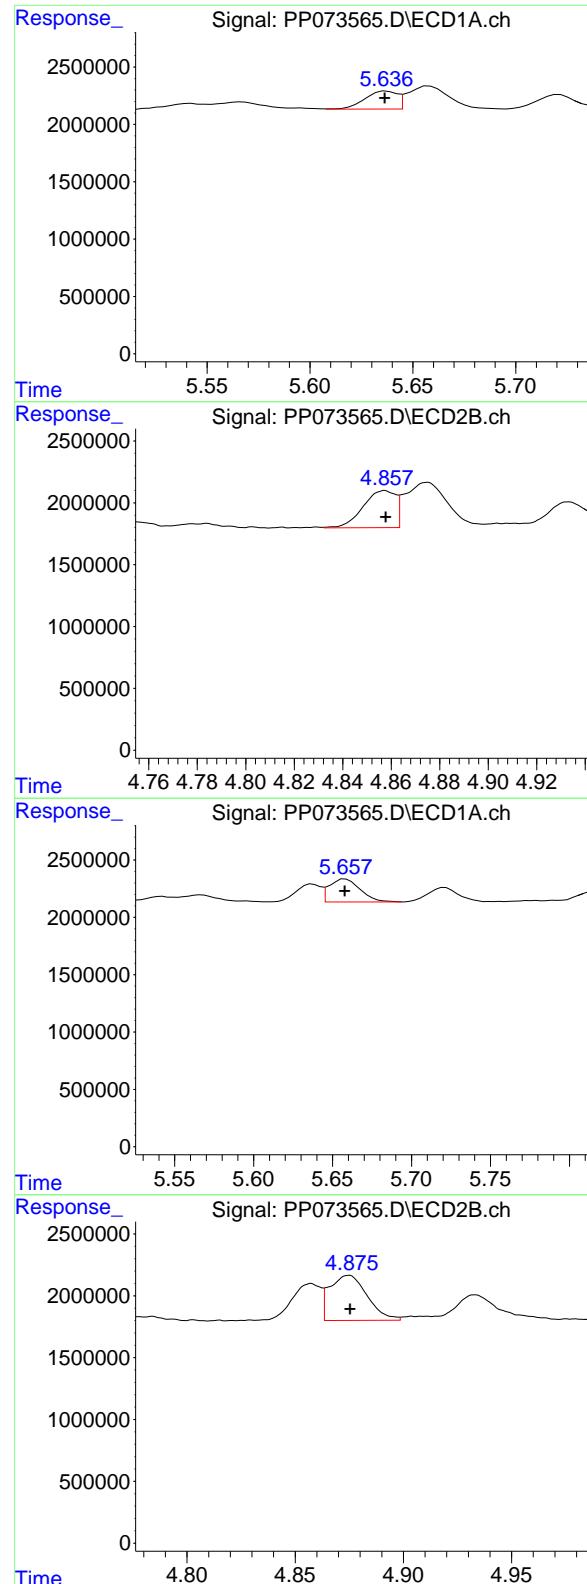

#16 AR-1242-1

R.T.: 5.636 min
 Delta R.T.: 0.000 min
 Response: 1573661
 Conc: 38.60 ng/ml

Instrument: ECD_P
ClientSampleId: AR1242ICC050

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/08/2025
 Supervised By :mohammad ahmed 07/09/2025

#16 AR-1242-1


R.T.: 4.857 min
 Delta R.T.: 0.000 min
 Response: 2804106
 Conc: 46.47 ng/ml

#17 AR-1242-2

R.T.: 5.657 min
 Delta R.T.: -0.001 min
 Response: 2642334
 Conc: 41.85 ng/ml

#17 AR-1242-2

R.T.: 4.875 min
 Delta R.T.: 0.000 min
 Response: 4375880
 Conc: 49.21 ng/ml

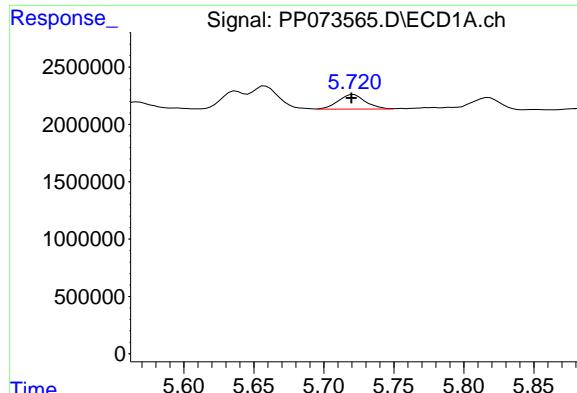


#18 AR-1242-3

R.T.: 5.720 min
 Delta R.T.: 0.000 min
 Response: 1729292
 Conc: 45.43 ng/ml

Instrument: ECD_P
 ClientSampleId: AR1242ICC050

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/08/2025
 Supervised By :mohammad ahmed 07/09/2025

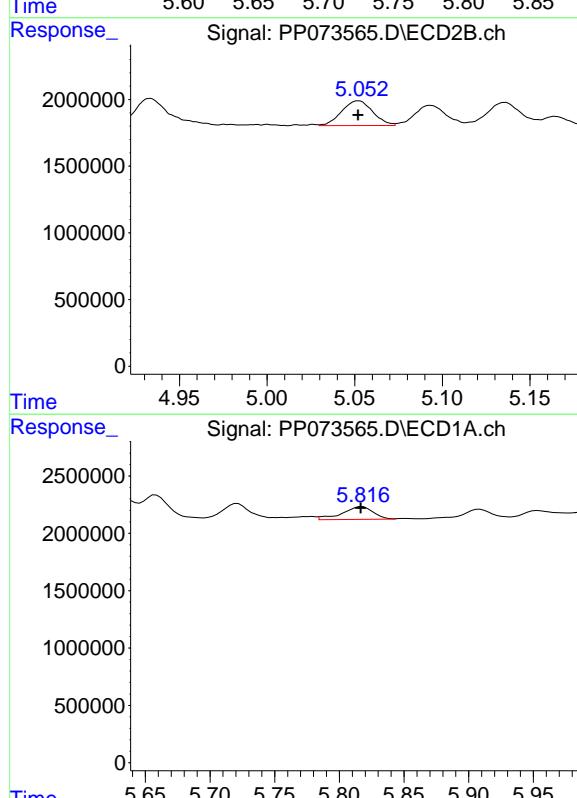

#18 AR-1242-3

R.T.: 5.052 min
 Delta R.T.: 0.000 min
 Response: 2296207
 Conc: 48.26 ng/ml

#19 AR-1242-4

R.T.: 5.818 min
 Delta R.T.: 0.001 min
 Response: 1851147
 Conc: 58.32 ng/ml

#19 AR-1242-4

R.T.: 5.136 min
 Delta R.T.: 0.000 min
 Response: 2337623
 Conc: 51.81 ng/ml



#20 AR-1242-5

R.T.: 6.546 min
 Delta R.T.: 0.000 min
 Response: 1593566
 Conc: 47.78 ng/ml

Instrument: ECD_P
ClientSampleId: AR1242ICC050

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/08/2025
 Supervised By :mohammad ahmed 07/09/2025

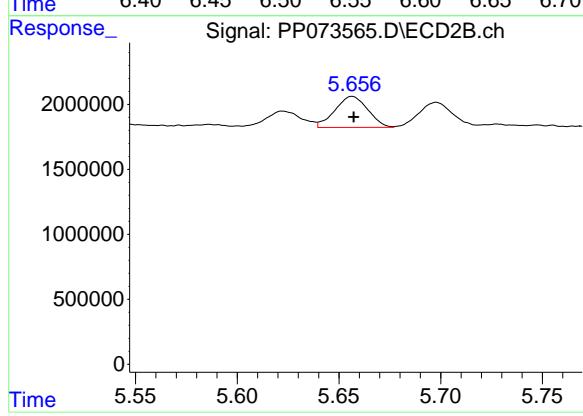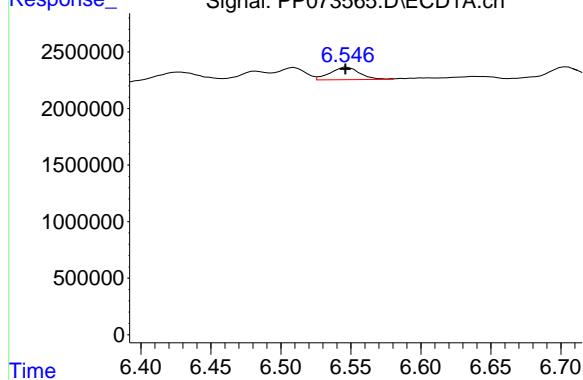

#20 AR-1242-5

R.T.: 5.657 min
 Delta R.T.: 0.000 min
 Response: 2688857
 Conc: 47.12 ng/ml

1
2
3
4
5
6
7
8
9
10
11
12
13
14
15
16
17
18
19
20

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP070825\
 Data File : PP073566.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jul 2025 00:19
 Operator : YP\AJ
 Sample : AR1248ICC1000
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
AR1248ICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 08 02:20:56 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 08 02:20:17 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	4.488	3.779	132.2E6	185.5E6	93.396	97.125
2) SA Decachlor...	10.176	8.781	109.8E6	129.8E6	95.885	95.444

Target Compounds

21) L5 AR-1248-1	5.639	4.857	29290065	41993150	931.027	929.349
22) L5 AR-1248-2	5.910	5.093	37625323	55737799	928.212	900.609
23) L5 AR-1248-3	6.112	5.136	43927993	58429721	953.396	907.187
24) L5 AR-1248-4	6.510	5.307	53376796	68661033	934.019	911.732
25) L5 AR-1248-5	6.549	5.698	51803368	69725277	929.059	912.356



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.





Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP070825\
 Data File : PP073566.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jul 2025 00:19
 Operator : YP\AJ
 Sample : AR1248ICC1000
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
AR1248ICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 08 02:20:56 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 08 02:20:17 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ m Signal #2 Info : 30M x 0.32mm x 0.25 μ m

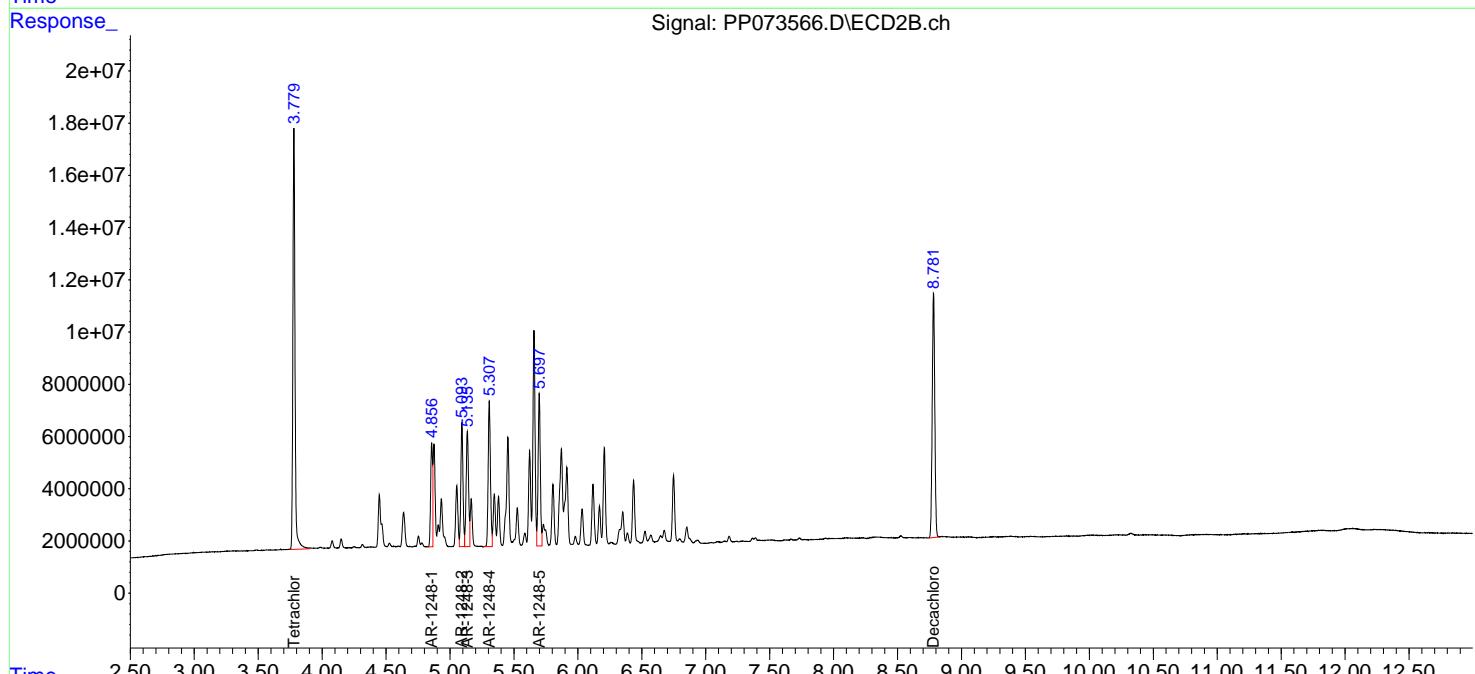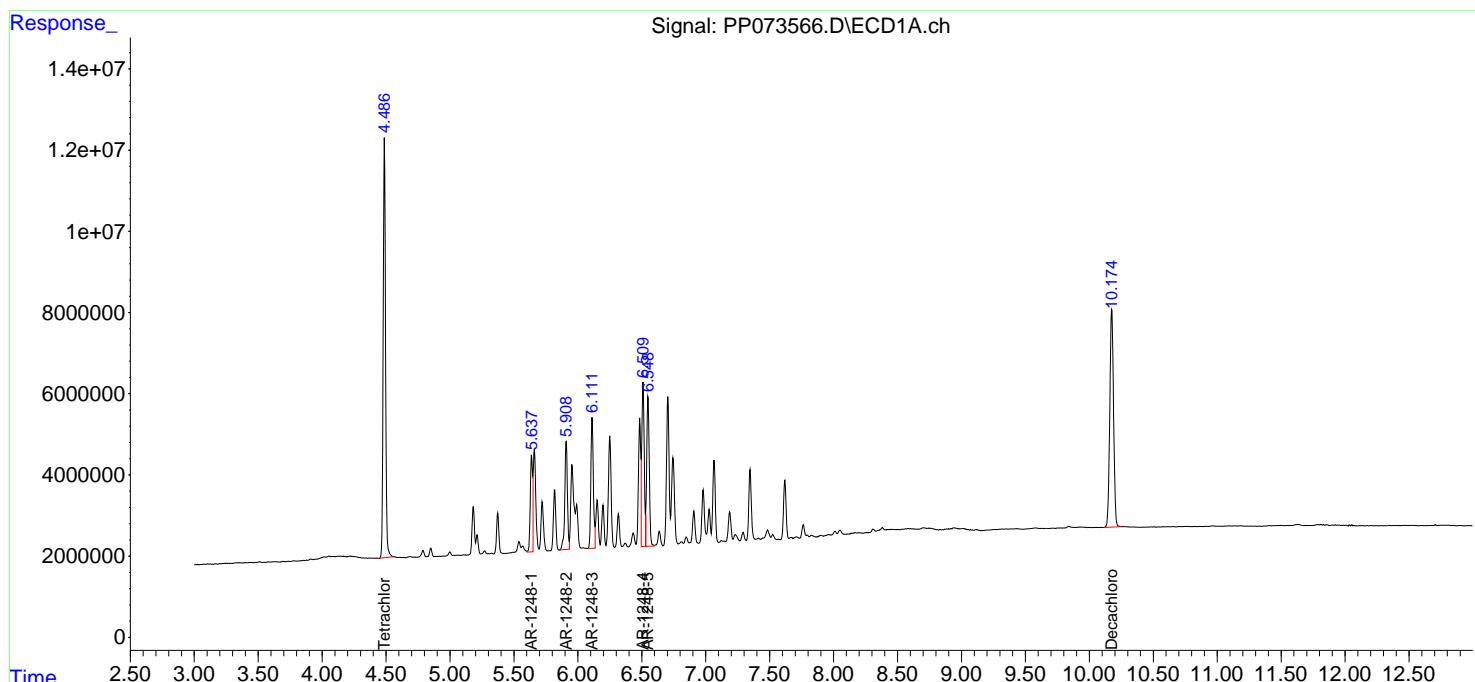

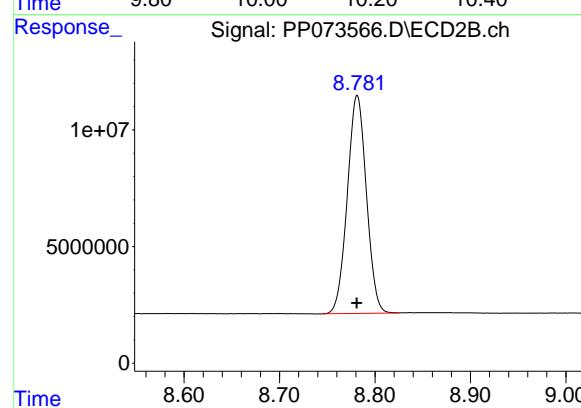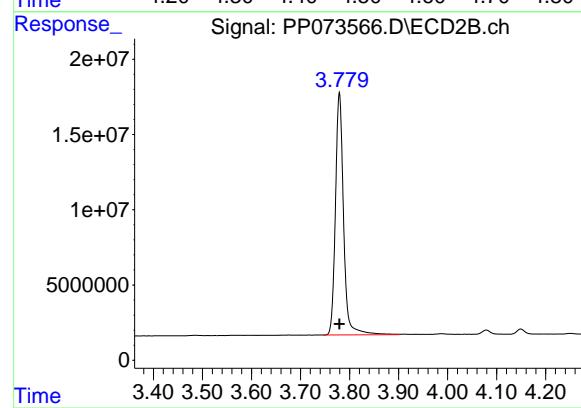

#1 Tetrachloro-m-xylene

R.T.: 4.488 min
 Delta R.T.: 0.002 min
 Response: 132195442
 Conc: 93.40 ng/ml

Instrument: ECD_P
 ClientSampleId: AR1248ICC1000

#1 Tetrachloro-m-xylene



R.T.: 3.779 min
 Delta R.T.: 0.000 min
 Response: 185548603
 Conc: 97.12 ng/ml

#2 Decachlorobiphenyl

R.T.: 10.176 min
 Delta R.T.: 0.002 min
 Response: 109801693
 Conc: 95.88 ng/ml

#2 Decachlorobiphenyl

R.T.: 8.781 min
 Delta R.T.: 0.000 min
 Response: 129838240
 Conc: 95.44 ng/ml

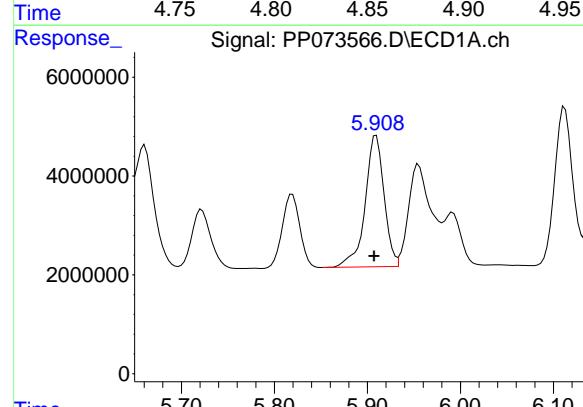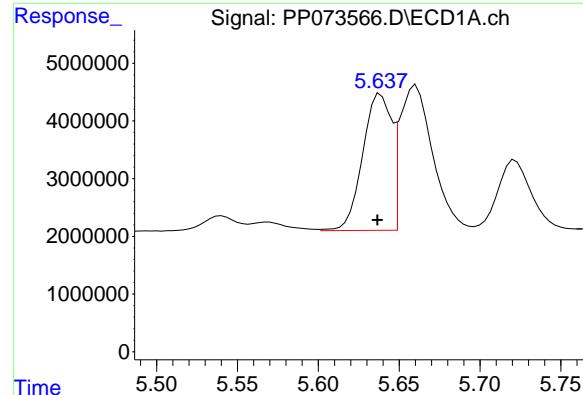

#21 AR-1248-1

R.T.: 5.639 min
 Delta R.T.: 0.002 min
 Response: 29290065
 Conc: 931.03 ng/ml

Instrument: ECD_P
 ClientSampleId: AR1248ICC1000

#21 AR-1248-1

R.T.: 4.857 min
 Delta R.T.: 0.000 min
 Response: 41993150
 Conc: 929.35 ng/ml

#22 AR-1248-2

R.T.: 5.910 min
 Delta R.T.: 0.002 min
 Response: 37625323
 Conc: 928.21 ng/ml


#22 AR-1248-2

R.T.: 5.093 min
 Delta R.T.: 0.000 min
 Response: 55737799
 Conc: 900.61 ng/ml

#23 AR-1248-3


R.T.: 6.112 min
 Delta R.T.: 0.002 min
 Response: 43927993
 Conc: 953.40 ng/ml

Instrument: ECD_P
ClientSampleId: AR1248ICC1000




#23 AR-1248-3

R.T.: 5.136 min
 Delta R.T.: 0.000 min
 Response: 58429721
 Conc: 907.19 ng/ml




#24 AR-1248-4

R.T.: 6.510 min
 Delta R.T.: 0.002 min
 Response: 53376796
 Conc: 934.02 ng/ml



#24 AR-1248-4



R.T.: 5.307 min
 Delta R.T.: 0.000 min
 Response: 68661033
 Conc: 911.73 ng/ml

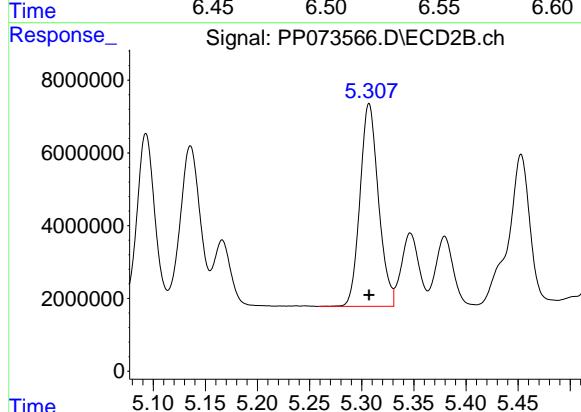

#25 AR-1248-5

R.T.: 6.549 min
Delta R.T.: 0.002 min
Response: 51803368
Conc: 929.06 ng/ml

Instrument: ECD_P
ClientSampleId: AR1248ICC1000

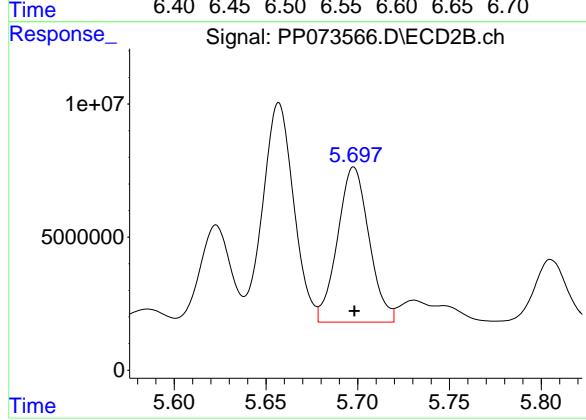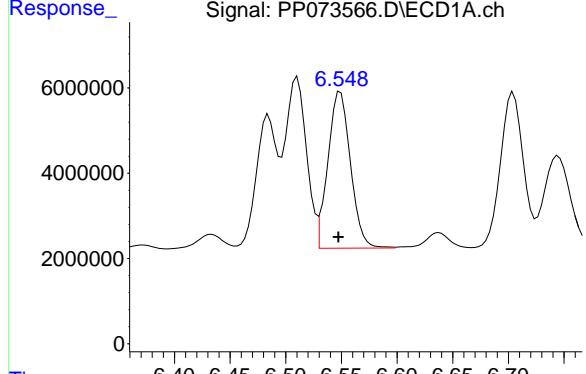

#25 AR-1248-5

R.T.: 5.698 min
Delta R.T.: 0.000 min
Response: 69725277
Conc: 912.36 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP070825\
 Data File : PP073567.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jul 2025 00:35
 Operator : YP\AJ
 Sample : AR1248ICC750
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
AR1248ICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 08 02:21:34 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 08 02:20:17 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	4.489	3.779	102.8E6	139.9E6	72.663	73.239
2) SA Decachlor...	10.178	8.781	84981366	104.5E6	74.210	76.789

Target Compounds

21) L5 AR-1248-1	5.639	4.858	22755547	32692852	723.318	723.525
22) L5 AR-1248-2	5.911	5.094	29802657	43939758	735.228	709.977
23) L5 AR-1248-3	6.113	5.135	34385217	45992259	746.283	714.081
24) L5 AR-1248-4	6.511	5.307	41943849	54019844	733.958	717.315
25) L5 AR-1248-5	6.551	5.698	40278207	54907819	722.363	718.469



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.





Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP070825\
 Data File : PP073567.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jul 2025 00:35
 Operator : YP\AJ
 Sample : AR1248ICC750
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
AR1248ICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 08 02:21:34 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 08 02:20:17 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

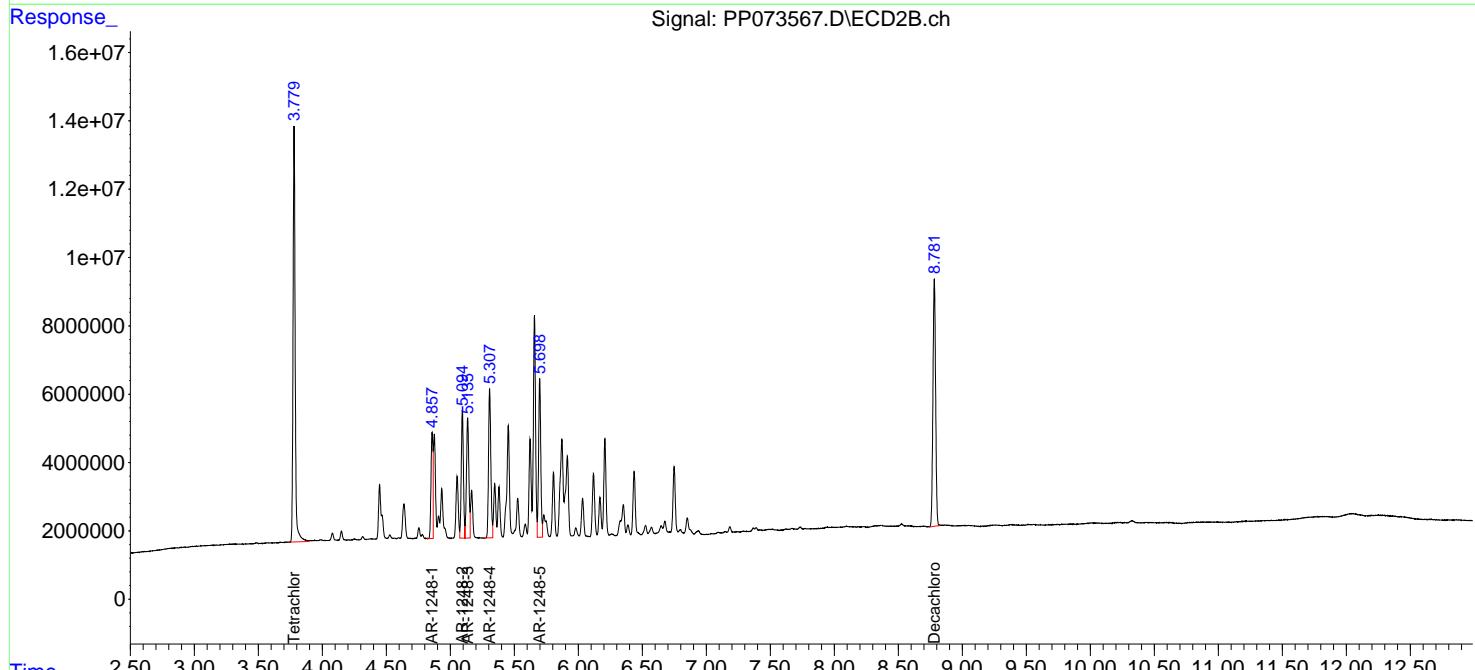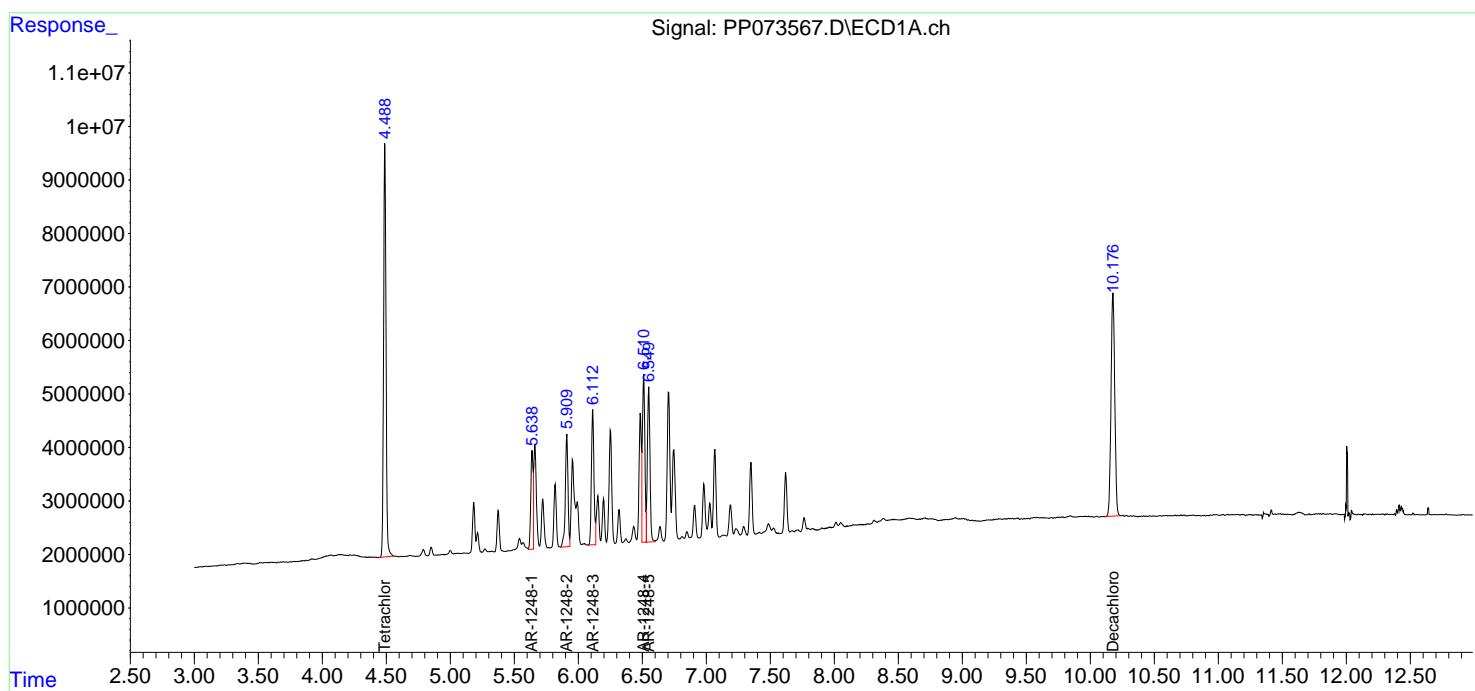

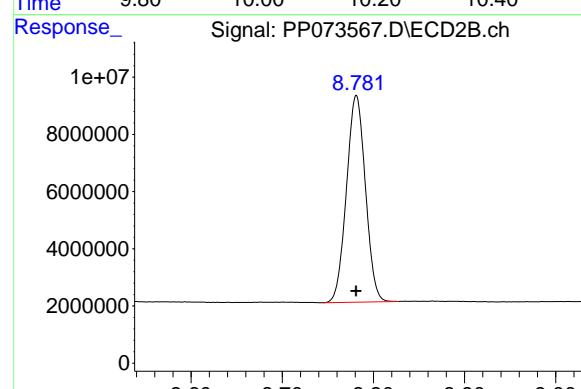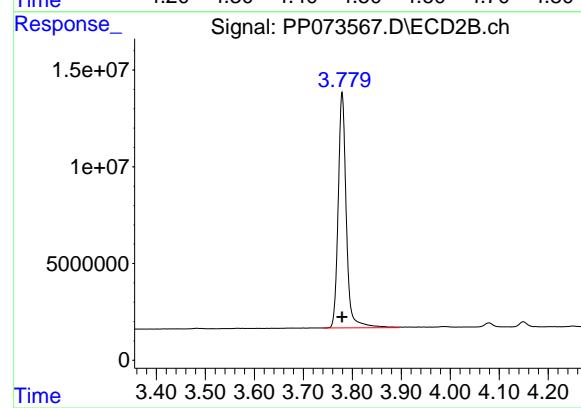

#1 Tetrachloro-m-xylene

R.T.: 4.489 min
Delta R.T.: 0.003 min
Response: 102849476
Conc: 72.66 ng/ml

Instrument:

ECD_P

ClientSampleId :

AR1248ICC750

#1 Tetrachloro-m-xylene





R.T.: 3.779 min
Delta R.T.: 0.000 min
Response: 139916989
Conc: 73.24 ng/ml

#2 Decachlorobiphenyl

R.T.: 10.178 min
Delta R.T.: 0.004 min
Response: 84981366
Conc: 74.21 ng/ml

#2 Decachlorobiphenyl

R.T.: 8.781 min
Delta R.T.: 0.000 min
Response: 104460409
Conc: 76.79 ng/ml

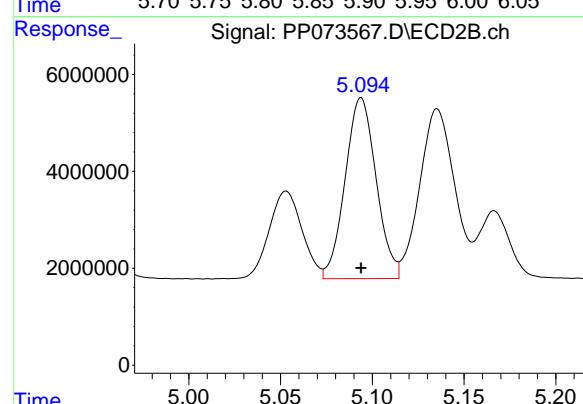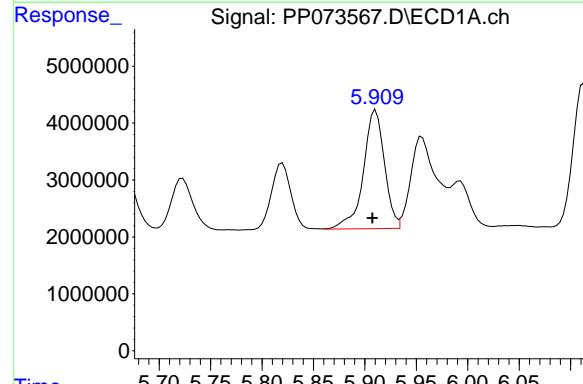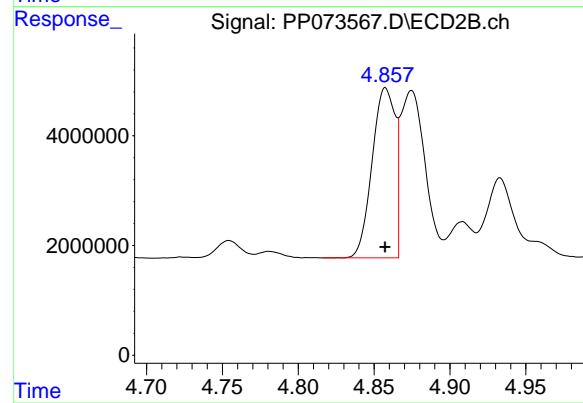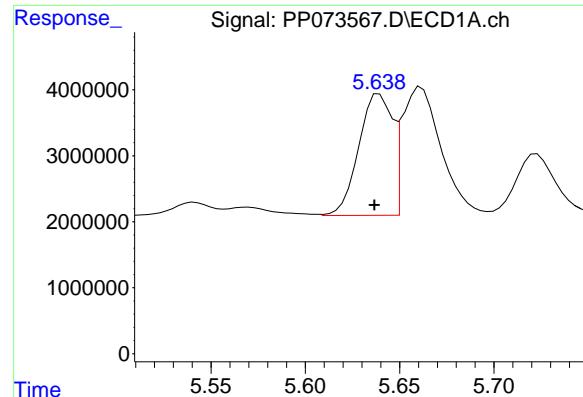

#21 AR-1248-1

R.T.: 5.639 min
 Delta R.T.: 0.003 min
 Response: 22755547
 Conc: 723.32 ng/ml

Instrument: ECD_P
ClientSampleId: AR1248ICC750

#21 AR-1248-1

R.T.: 4.858 min
 Delta R.T.: 0.000 min
 Response: 32692852
 Conc: 723.52 ng/ml

#22 AR-1248-2

R.T.: 5.911 min
 Delta R.T.: 0.003 min
 Response: 29802657
 Conc: 735.23 ng/ml


#22 AR-1248-2

R.T.: 5.094 min
 Delta R.T.: 0.000 min
 Response: 43939758
 Conc: 709.98 ng/ml

#23 AR-1248-3


R.T.: 6.113 min
 Delta R.T.: 0.003 min
 Response: 34385217
 Conc: 746.28 ng/ml

Instrument: ECD_P
ClientSampleId: AR1248ICC750




#23 AR-1248-3

R.T.: 5.135 min
 Delta R.T.: 0.000 min
 Response: 45992259
 Conc: 714.08 ng/ml

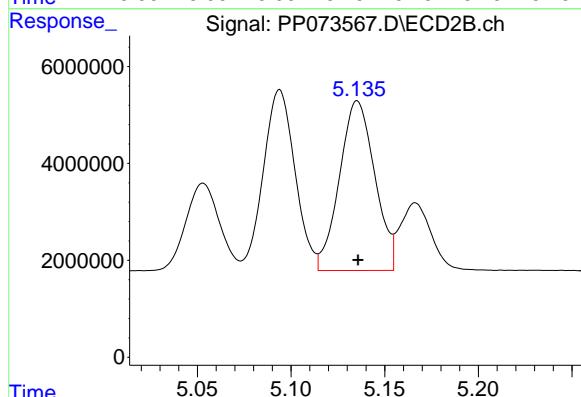


#24 AR-1248-4

R.T.: 6.511 min
 Delta R.T.: 0.003 min
 Response: 41943849
 Conc: 733.96 ng/ml

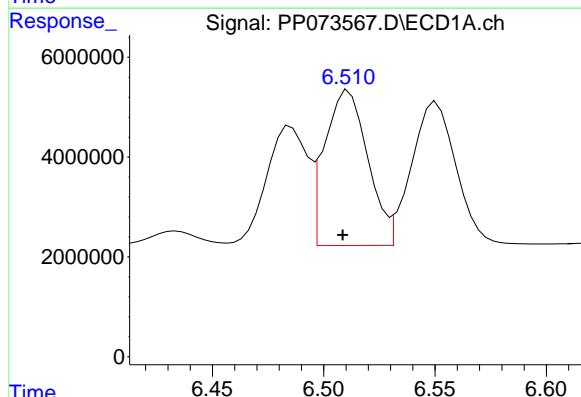


#24 AR-1248-4

R.T.: 5.307 min
 Delta R.T.: 0.000 min
 Response: 54019844
 Conc: 717.32 ng/ml

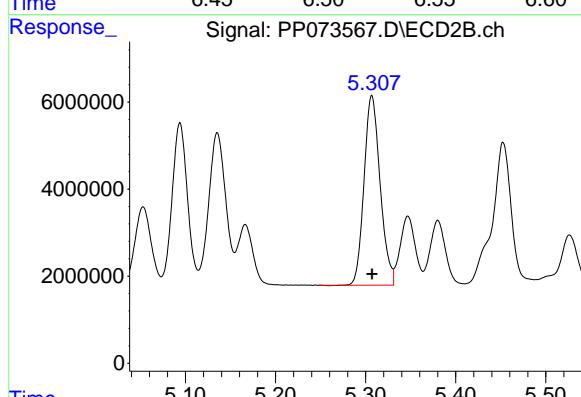

#25 AR-1248-5

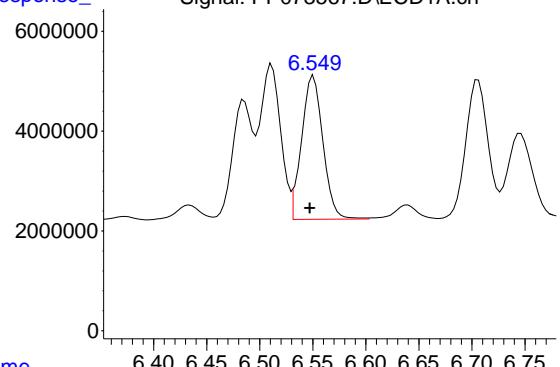


R.T.: 6.551 min
Delta R.T.: 0.003 min
Response: 40278207
Conc: 722.36 ng/ml

Instrument: ECD_P
ClientSampleId: AR1248ICC750

#25 AR-1248-5

R.T.: 5.698 min
Delta R.T.: 0.000 min
Response: 54907819
Conc: 718.47 ng/ml

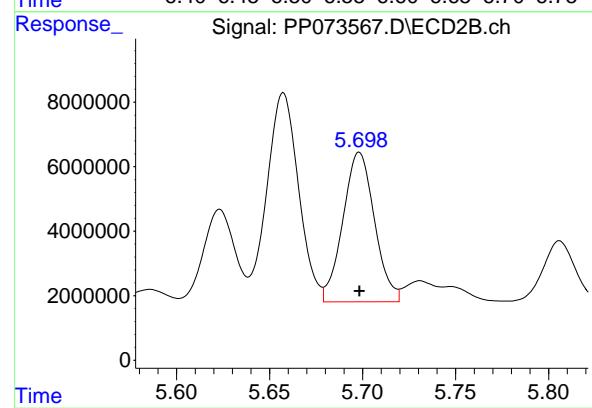

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP070825\
 Data File : PP073568.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jul 2025 00:52
 Operator : YP\AJ
 Sample : AR1248ICC500
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
AR1248ICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 08 02:21:57 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 08 02:20:17 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	4.486	3.779	70771652	95520830	50.000	50.000
2) SA Decachlor...	10.174	8.781	57257196	68017781	50.000	50.000

Target Compounds

21) L5 AR-1248-1	5.637	4.857	15729968	22592772	500.000	500.000
22) L5 AR-1248-2	5.907	5.094	20267627	30944510	500.000	500.000
23) L5 AR-1248-3	6.110	5.136	23037645	32203795	500.000	500.000
24) L5 AR-1248-4	6.509	5.307	28573723	37654186	500.000	500.000
25) L5 AR-1248-5	6.547	5.698	27879471	38211657	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.





Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP070825\
 Data File : PP073568.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jul 2025 00:52
 Operator : YP\AJ
 Sample : AR1248ICC500
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
AR1248ICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 08 02:21:57 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 08 02:20:17 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

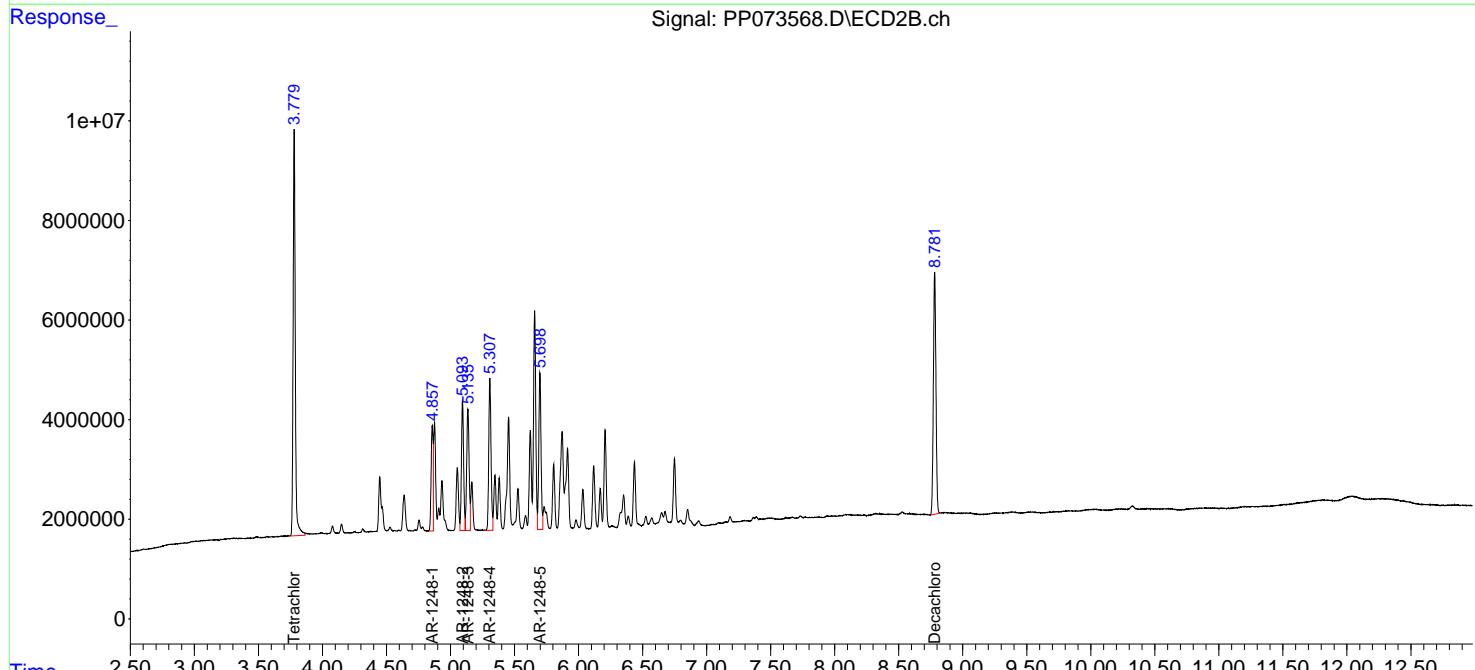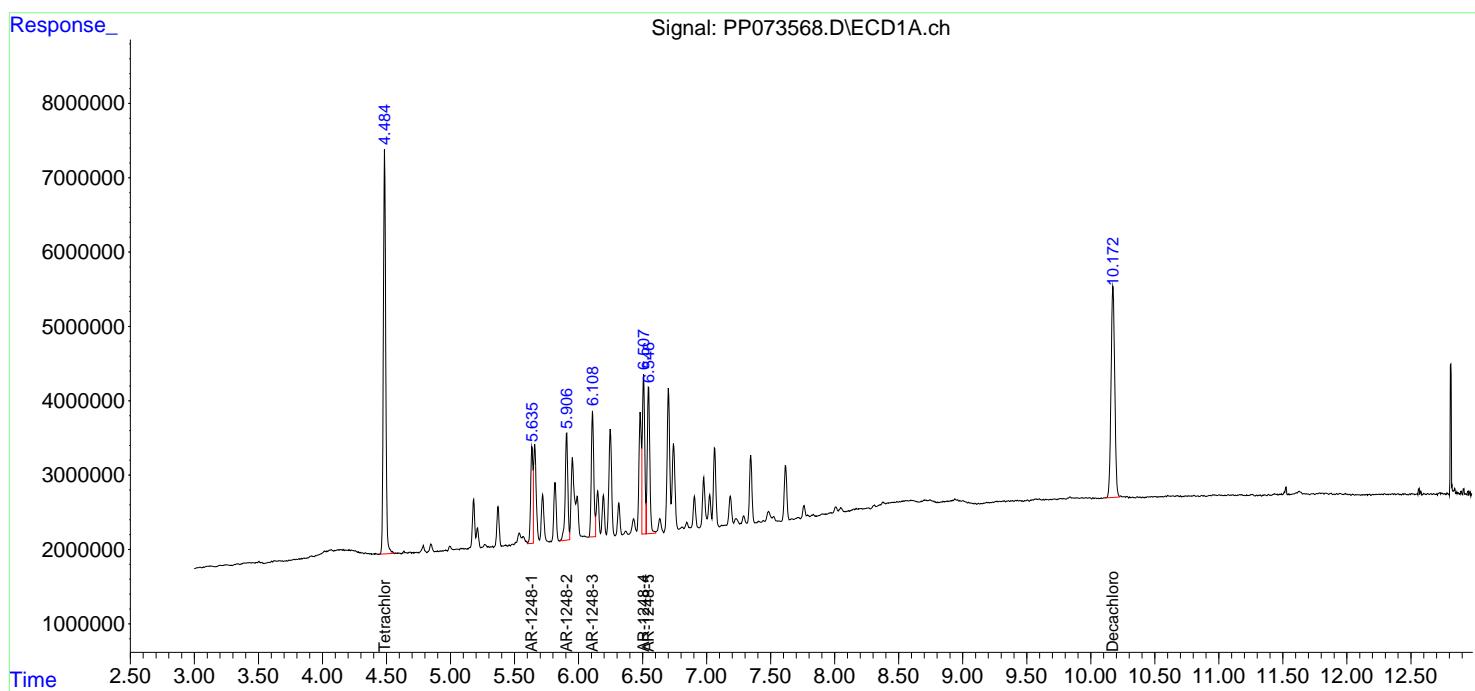

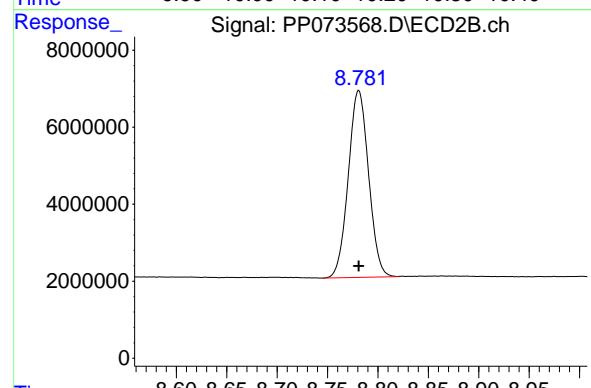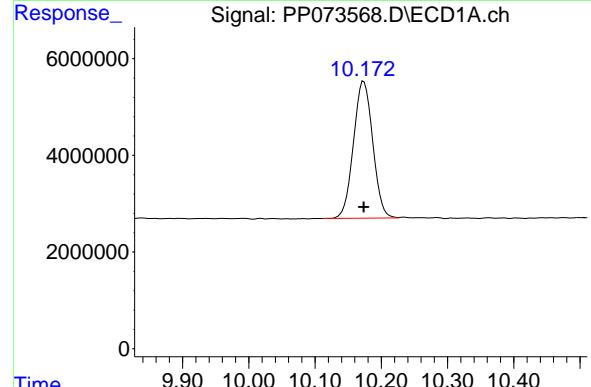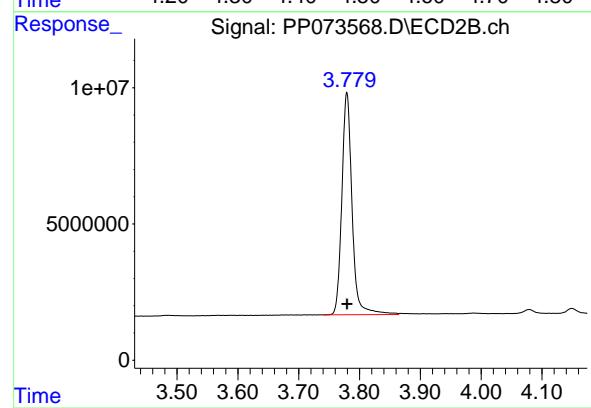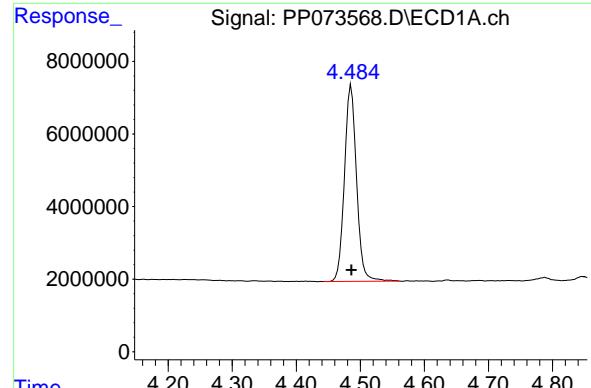

#1 Tetrachloro-m-xylene

R.T.: 4.486 min
 Delta R.T.: 0.000 min
 Response: 70771652
 Conc: 50.00 ng/ml

Instrument: ECD_P
ClientSampleId: AR1248ICC500

#1 Tetrachloro-m-xylene


R.T.: 3.779 min
 Delta R.T.: 0.000 min
 Response: 95520830
 Conc: 50.00 ng/ml

#2 Decachlorobiphenyl

R.T.: 10.174 min
 Delta R.T.: 0.000 min
 Response: 57257196
 Conc: 50.00 ng/ml

#2 Decachlorobiphenyl

R.T.: 8.781 min
 Delta R.T.: 0.000 min
 Response: 68017781
 Conc: 50.00 ng/ml

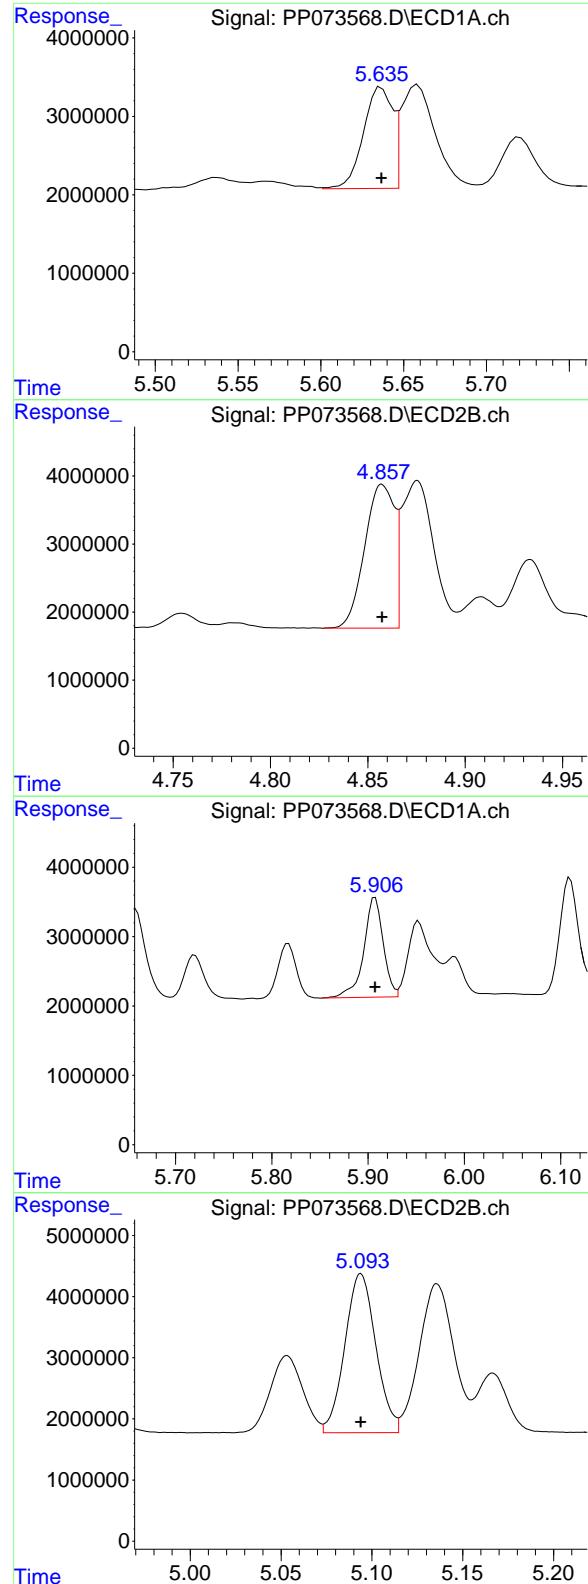

#21 AR-1248-1

R.T.: 5.637 min
 Delta R.T.: 0.000 min
 Response: 15729968
 Conc: 500.00 ng/ml

Instrument: ECD_P
 ClientSampleId: AR1248ICC500

#21 AR-1248-1

R.T.: 4.857 min
 Delta R.T.: 0.000 min
 Response: 22592772
 Conc: 500.00 ng/ml

#22 AR-1248-2

R.T.: 5.907 min
 Delta R.T.: 0.000 min
 Response: 20267627
 Conc: 500.00 ng/ml


#22 AR-1248-2

R.T.: 5.094 min
 Delta R.T.: 0.000 min
 Response: 30944510
 Conc: 500.00 ng/ml

#23 AR-1248-3


R.T.: 6.110 min
 Delta R.T.: 0.000 min
 Response: 23037645
 Conc: 500.00 ng/ml

Instrument: ECD_P
ClientSampleId: AR1248ICC500

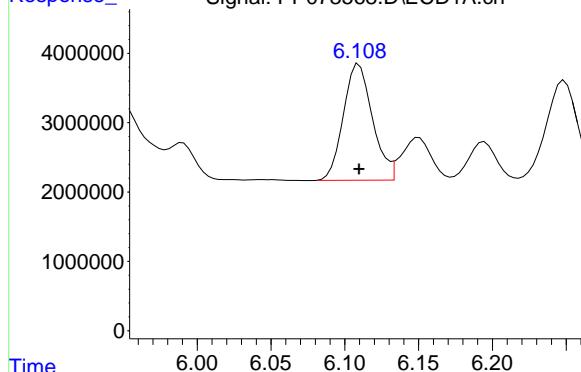


#23 AR-1248-3

R.T.: 5.136 min
 Delta R.T.: 0.000 min
 Response: 32203795
 Conc: 500.00 ng/ml

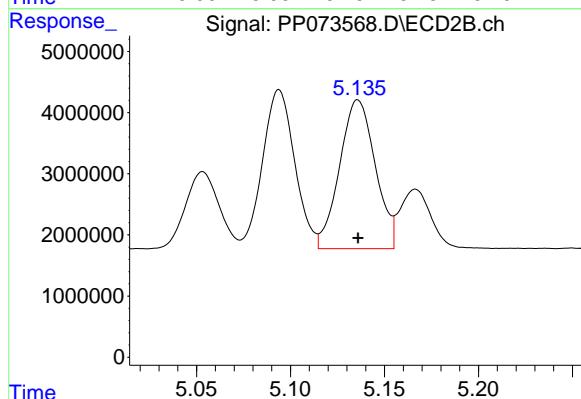


#24 AR-1248-4

R.T.: 6.509 min
 Delta R.T.: 0.000 min
 Response: 28573723
 Conc: 500.00 ng/ml

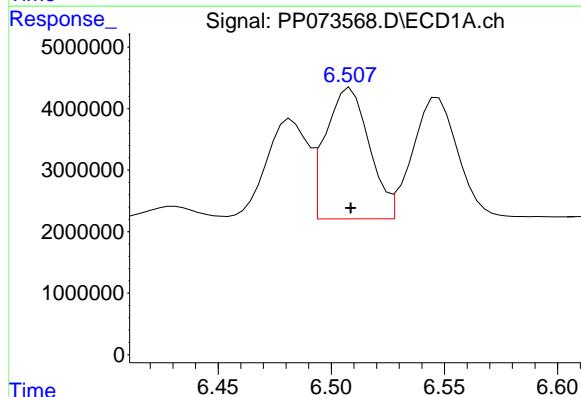

#24 AR-1248-4



R.T.: 5.307 min
 Delta R.T.: 0.000 min
 Response: 37654186
 Conc: 500.00 ng/ml

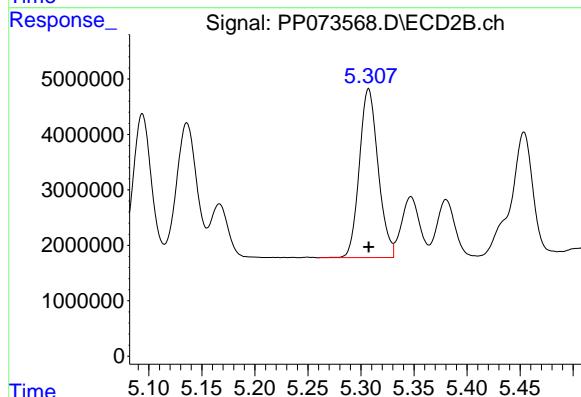

#25 AR-1248-5

R.T.: 6.547 min
Delta R.T.: 0.000 min
Response: 27879471
Conc: 500.00 ng/ml

Instrument: ECD_P
ClientSampleId: AR1248ICC500

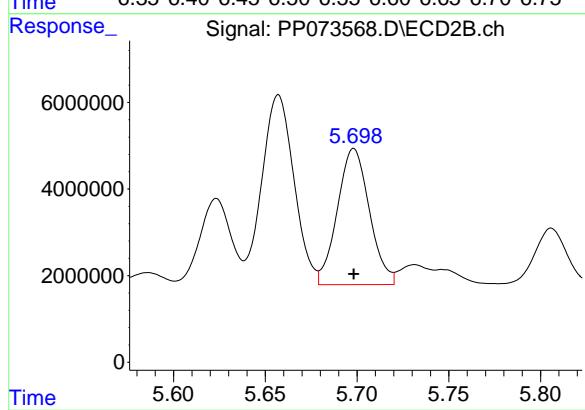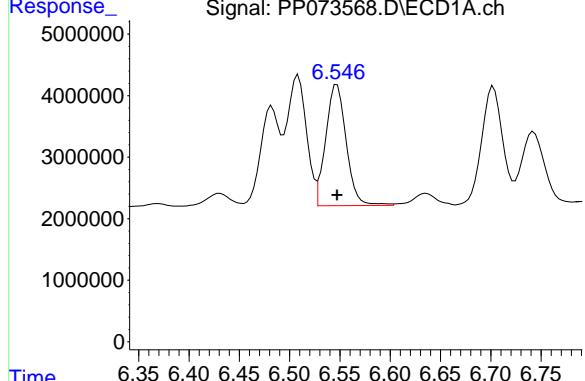

#25 AR-1248-5

R.T.: 5.698 min
Delta R.T.: 0.000 min
Response: 38211657
Conc: 500.00 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP070825\
 Data File : PP073569.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jul 2025 01:08
 Operator : YP\AJ
 Sample : AR1248ICC250
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
AR1248ICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 08 02:22:22 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 08 02:20:17 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	4.490	3.779	36421864	49176634	25.732	25.741
2) SA Decachlor...	10.178	8.780	29322870	36021021	25.606	26.479

Target Compounds

21) L5 AR-1248-1	5.640	4.857	8580276	12460998	272.737	275.774
22) L5 AR-1248-2	5.912	5.093	11018738	16676734	271.831	269.462
23) L5 AR-1248-3	6.114	5.136	12142276	17367378	263.531	269.648
24) L5 AR-1248-4	6.513	5.307	14943654	20433630	261.493	271.333
25) L5 AR-1248-5	6.552	5.698	14485646	20424181	259.791	267.251



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP070825\
 Data File : PP073569.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jul 2025 01:08
 Operator : YP\AJ
 Sample : AR1248ICC250
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
AR1248ICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 08 02:22:22 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 08 02:20:17 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ m Signal #2 Info : 30M x 0.32mm x 0.25 μ m

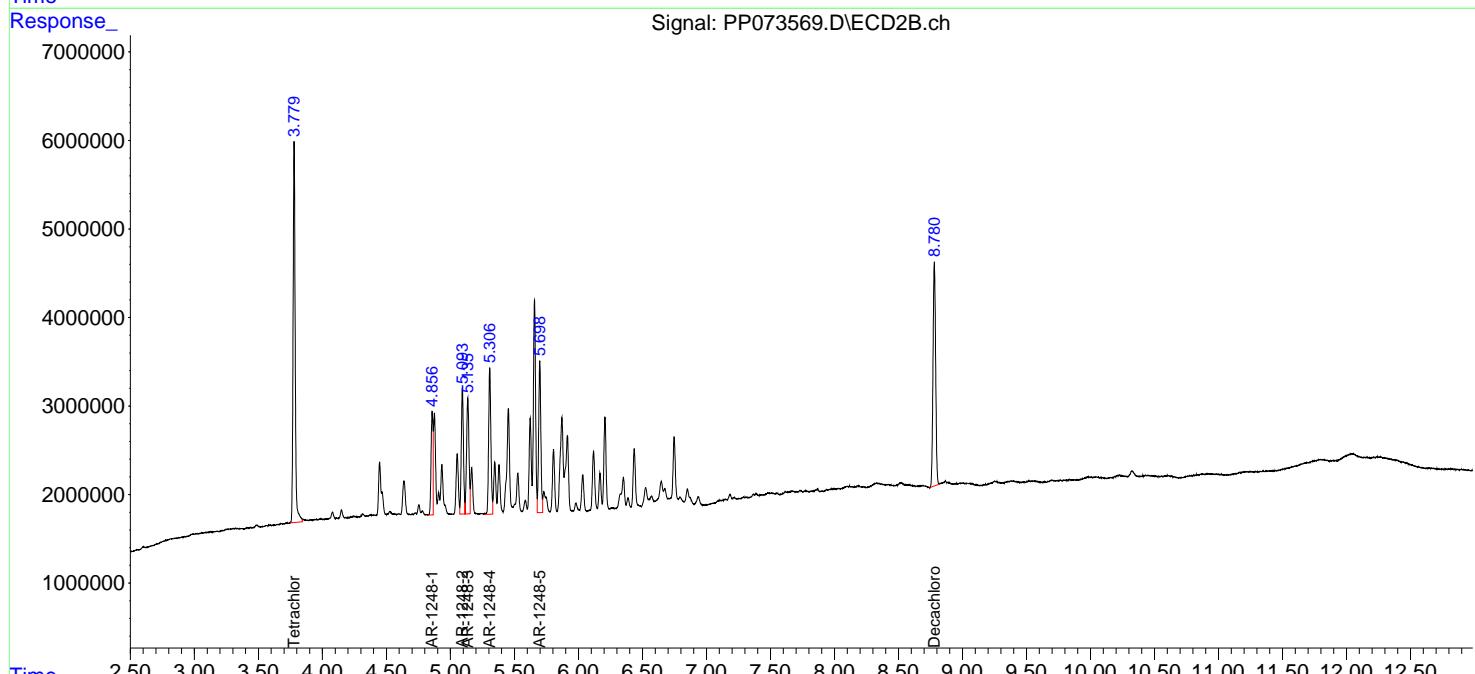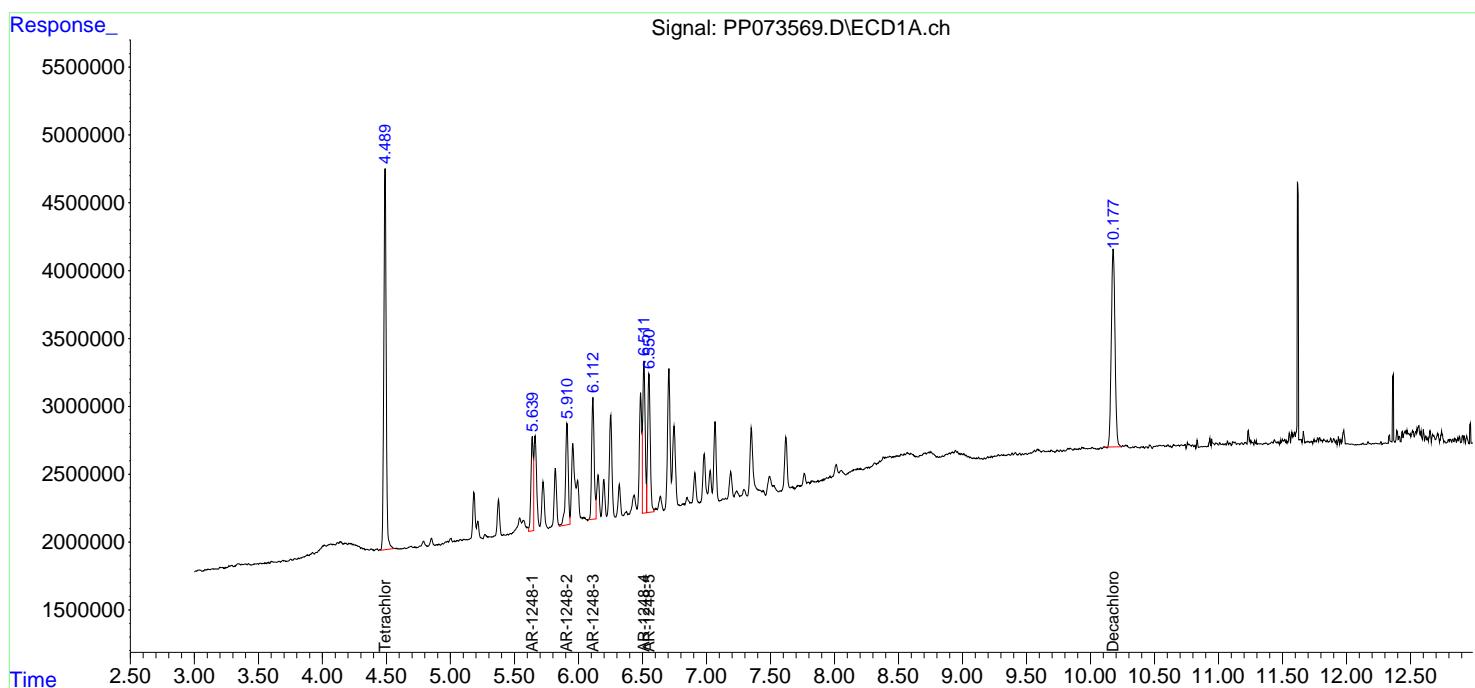

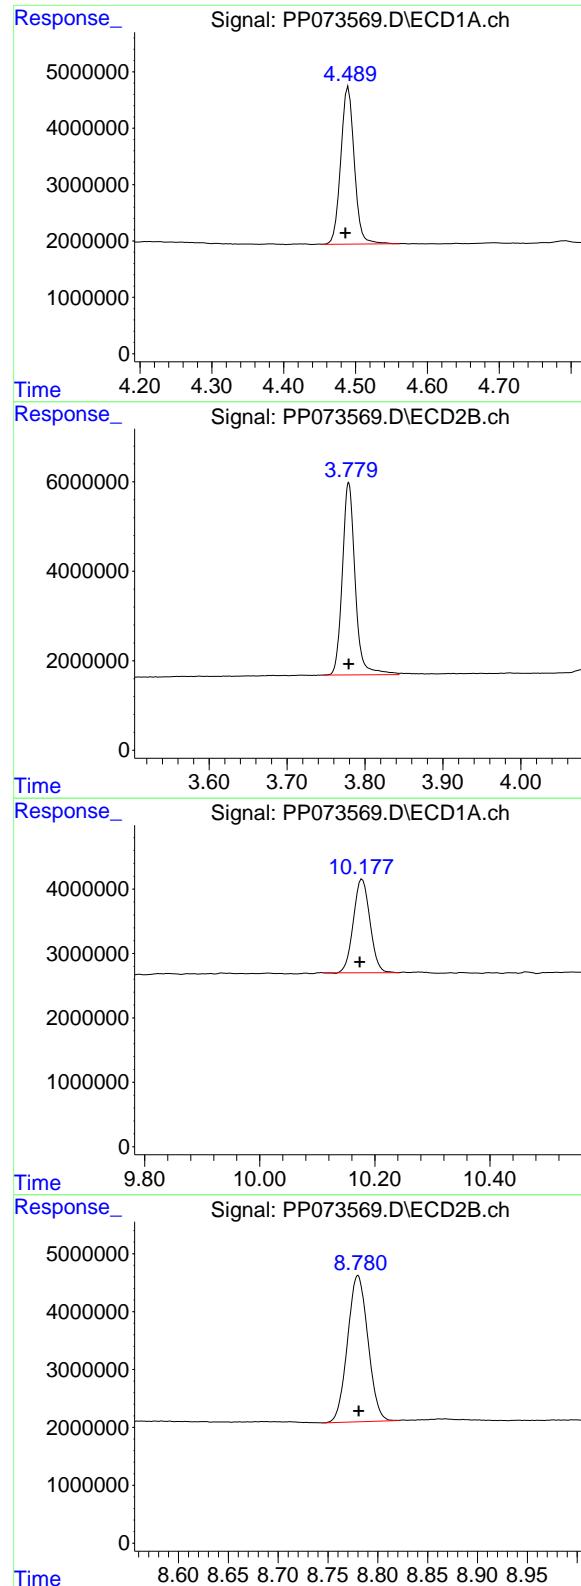

#1 Tetrachloro-m-xylene

R.T.: 4.490 min
 Delta R.T.: 0.004 min
 Response: 36421864
 Conc: 25.73 ng/ml

Instrument:

ECD_P

ClientSampleId :
AR1248ICC250

#1 Tetrachloro-m-xylene

R.T.: 3.779 min
 Delta R.T.: 0.000 min
 Response: 49176634
 Conc: 25.74 ng/ml

#2 Decachlorobiphenyl

R.T.: 10.178 min
 Delta R.T.: 0.004 min
 Response: 29322870
 Conc: 25.61 ng/ml


#2 Decachlorobiphenyl

R.T.: 8.780 min
 Delta R.T.: 0.000 min
 Response: 36021021
 Conc: 26.48 ng/ml

#21 AR-1248-1


R.T.: 5.640 min
 Delta R.T.: 0.003 min
 Response: 8580276
 Conc: 272.74 ng/ml

Instrument: ECD_P
 ClientSampleId: AR1248ICC250

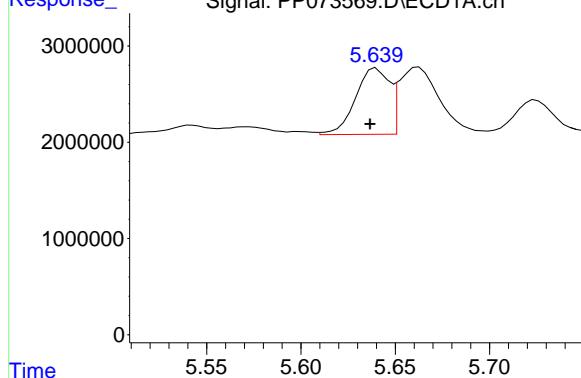


#21 AR-1248-1

R.T.: 4.857 min
 Delta R.T.: 0.000 min
 Response: 12460998
 Conc: 275.77 ng/ml

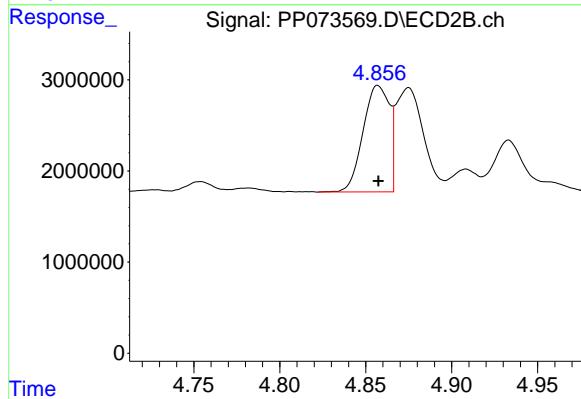


#22 AR-1248-2


R.T.: 5.912 min
 Delta R.T.: 0.004 min
 Response: 11018738
 Conc: 271.83 ng/ml

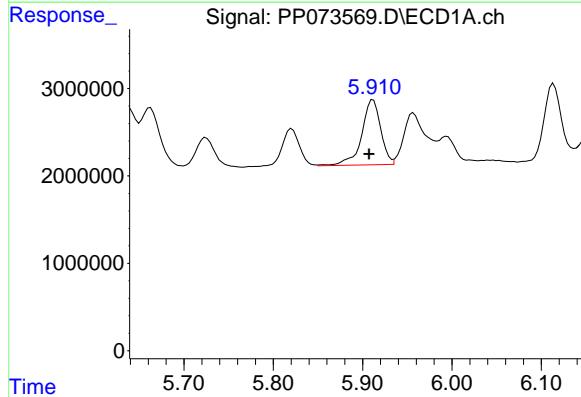

#22 AR-1248-2

R.T.: 5.093 min
 Delta R.T.: 0.000 min
 Response: 16676734
 Conc: 269.46 ng/ml

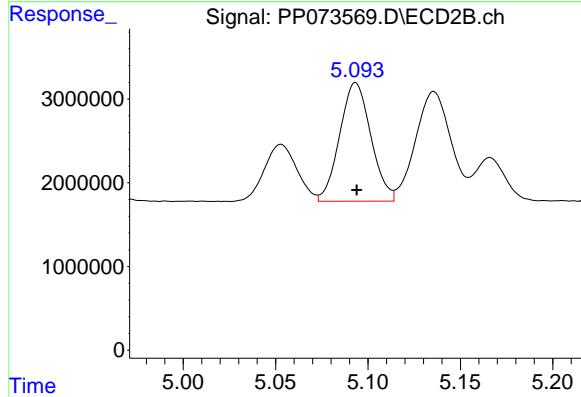

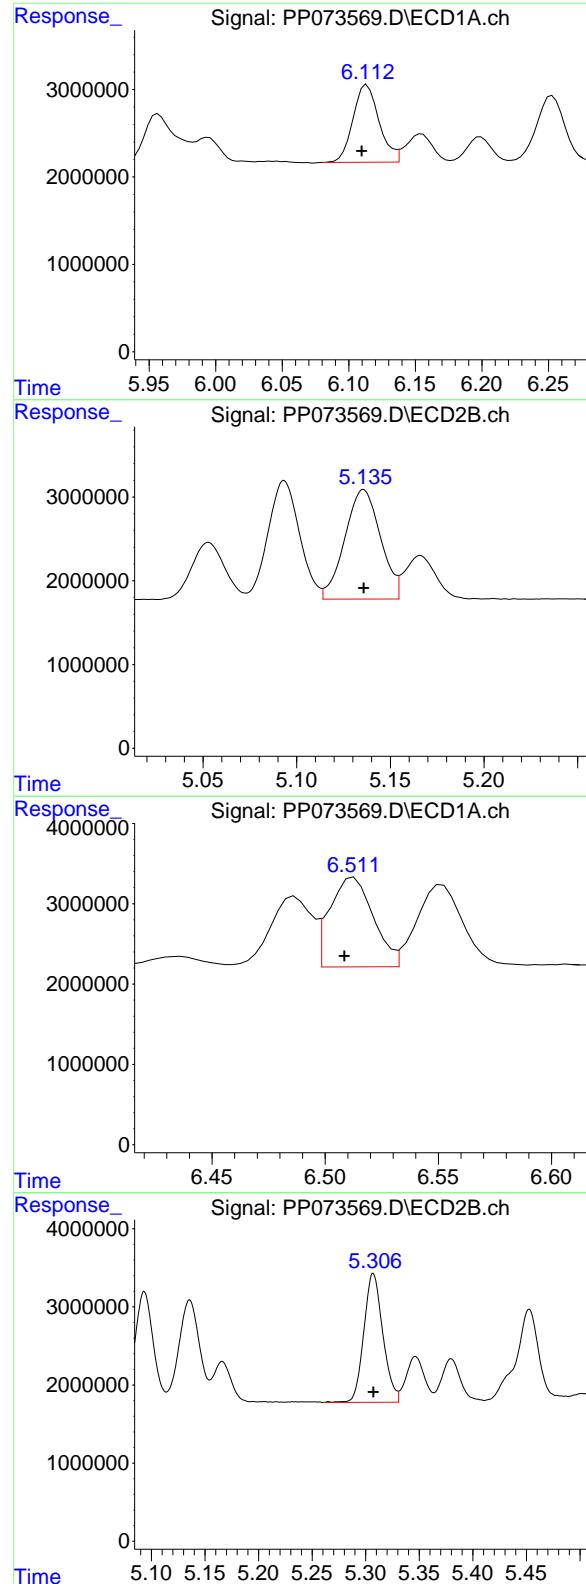

#23 AR-1248-3

R.T.: 6.114 min
 Delta R.T.: 0.004 min
 Response: 12142276
 Conc: 263.53 ng/ml

Instrument: ECD_P
 ClientSampleId: AR1248ICC250

#23 AR-1248-3


R.T.: 5.136 min
 Delta R.T.: 0.000 min
 Response: 17367378
 Conc: 269.65 ng/ml

#24 AR-1248-4

R.T.: 6.513 min
 Delta R.T.: 0.004 min
 Response: 14943654
 Conc: 261.49 ng/ml

#24 AR-1248-4

R.T.: 5.307 min
 Delta R.T.: 0.000 min
 Response: 20433630
 Conc: 271.33 ng/ml

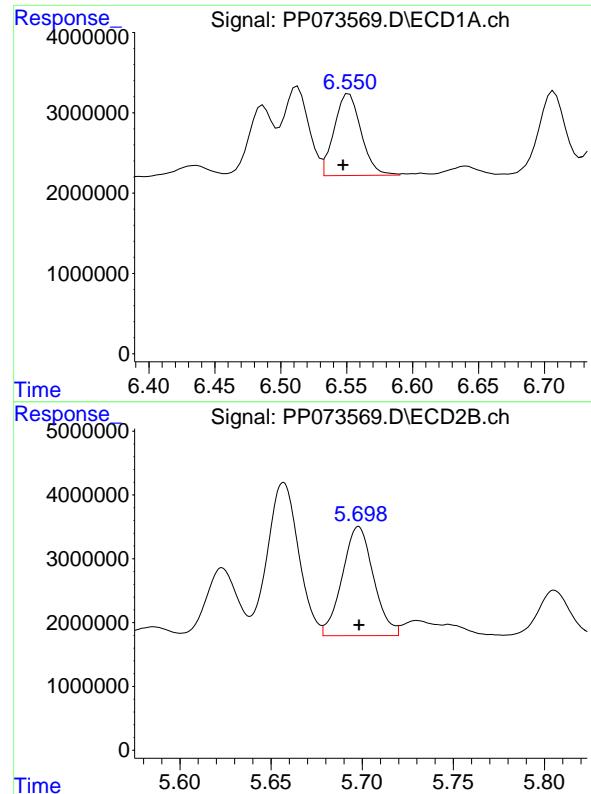

#25 AR-1248-5

R.T.: 6.552 min
Delta R.T.: 0.005 min
Response: 14485646
Conc: 259.79 ng/ml

Instrument: ECD_P
ClientSampleId: AR1248ICC250

#25 AR-1248-5

R.T.: 5.698 min
Delta R.T.: 0.000 min
Response: 20424181
Conc: 267.25 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP070825\
 Data File : PP073570.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jul 2025 01:25
 Operator : YP\AJ
 Sample : AR1248ICC050
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
AR1248ICC050

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/08/2025
 Supervised By :mohammad ahmed 07/09/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 08 02:22:43 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 08 02:20:17 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	4.485	3.779	6203851	8373290	4.383	4.383
2) SA Decachlor...	10.173	8.780	4448332	5794229	3.885	4.259

Target Compounds

21) L5 AR-1248-1	5.634	4.857	1447041	2193065	45.996m	48.535
22) L5 AR-1248-2	5.906	5.093	1882218	3238127	46.434	52.322
23) L5 AR-1248-3	6.108	5.135	1881440	3334641	40.834	51.774 #
24) L5 AR-1248-4	6.506	5.307	2458929	3957834	43.028m	52.555
25) L5 AR-1248-5	6.545	5.698	2487202	3594939	44.606m	47.040

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP070825\
 Data File : PP073570.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jul 2025 01:25
 Operator : YP\AJ
 Sample : AR1248ICC050
 Misc :
 ALS Vial : 19 Sample Multiplier: 1



Instrument :
 ECD_P
 ClientSampleId :
 AR1248ICC050

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/08/2025
 Supervised By :mohammad ahmed 07/09/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 08 02:22:43 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 08 02:20:17 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

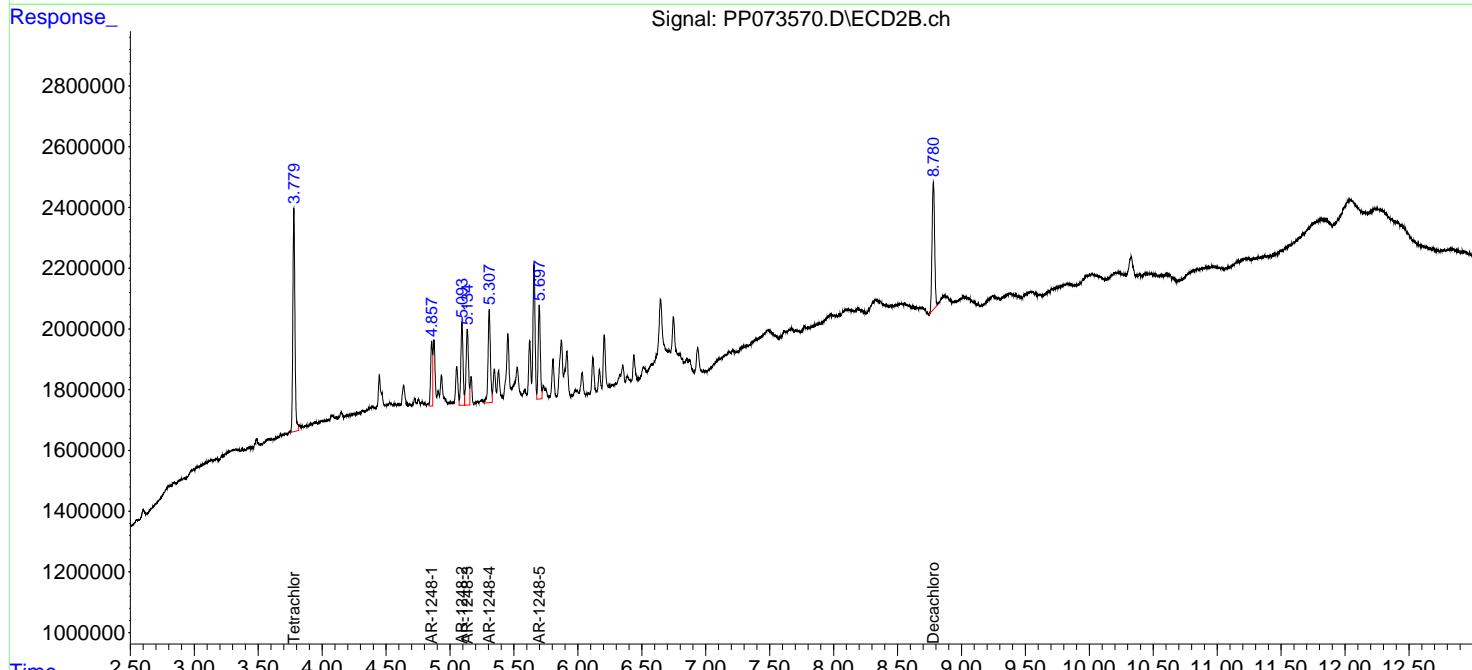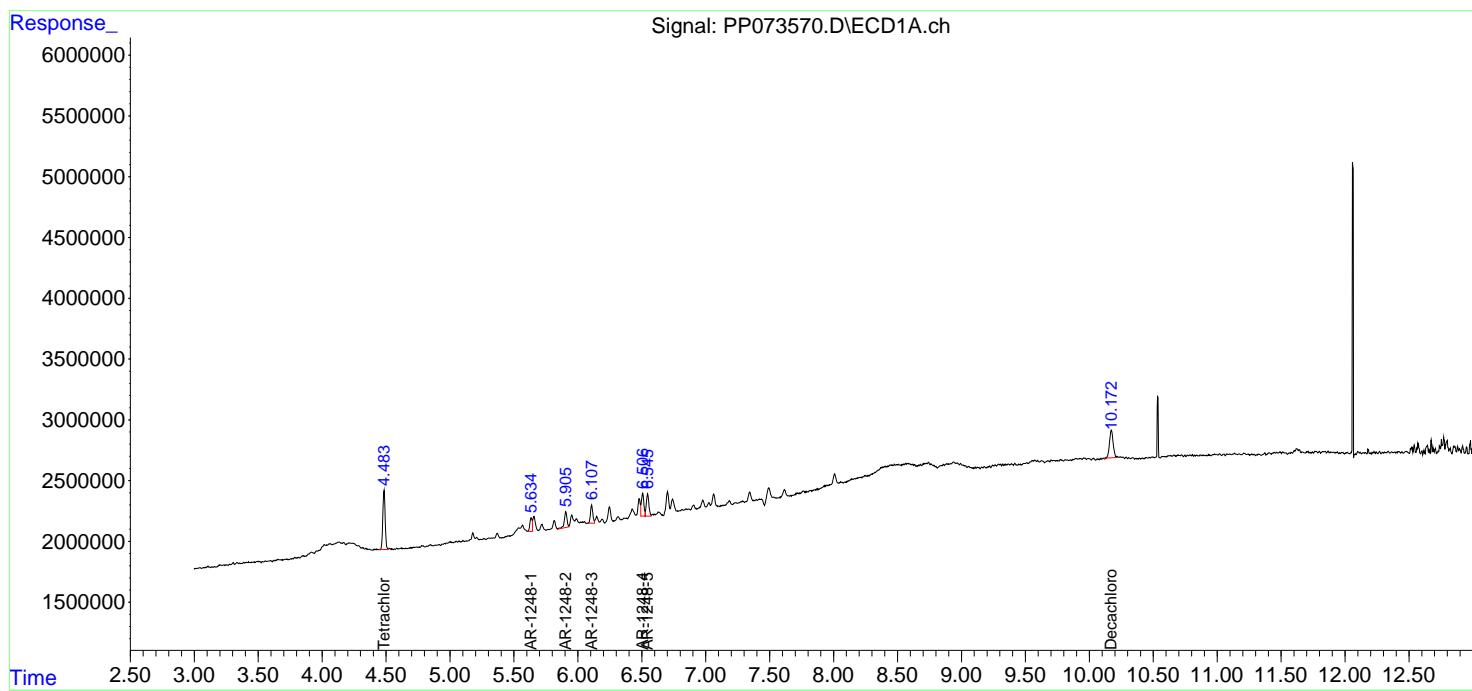


#1 Tetrachloro-m-xylene

R.T.: 4.485 min
 Delta R.T.: -0.001 min
 Response: 6203851
 Conc: 4.38 ng/ml

Instrument : ECD_P
 ClientSampleId : AR1248ICC050


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/08/2025
 Supervised By :mohammad ahmed 07/09/2025

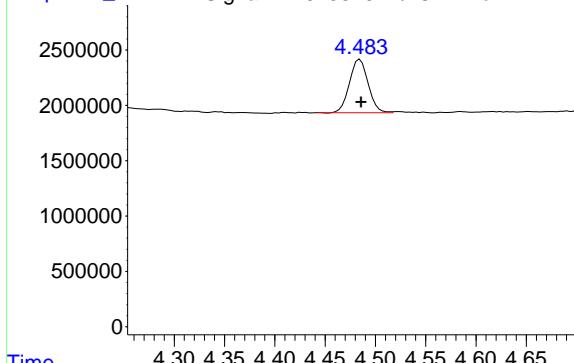


#1 Tetrachloro-m-xylene

R.T.: 3.779 min
 Delta R.T.: 0.000 min
 Response: 8373290
 Conc: 4.38 ng/ml

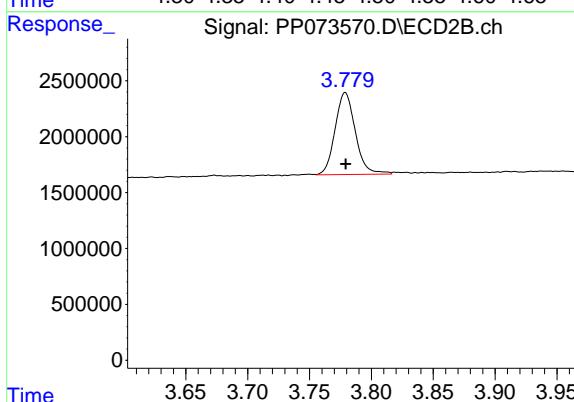


#2 Decachlorobiphenyl


R.T.: 10.173 min
 Delta R.T.: 0.000 min
 Response: 4448332
 Conc: 3.88 ng/ml

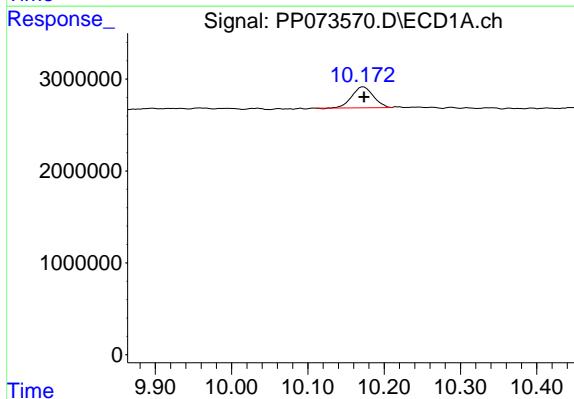

#2 Decachlorobiphenyl

R.T.: 8.780 min
 Delta R.T.: 0.000 min
 Response: 5794229
 Conc: 4.26 ng/ml

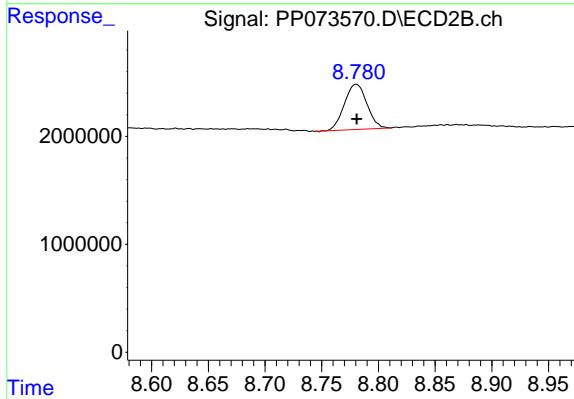

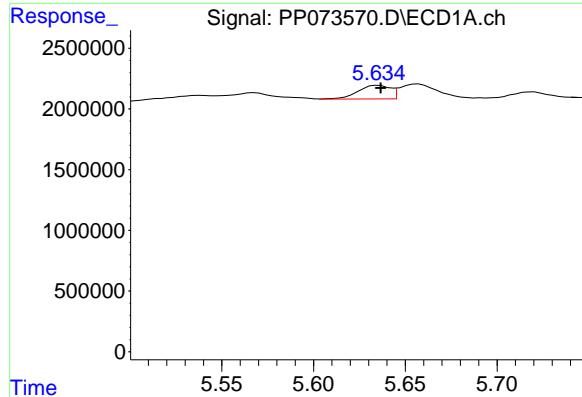


#21 AR-1248-1

R.T.: 5.634 min
 Delta R.T.: -0.003 min
 Response: 1447041
 Conc: 46.00 ng/ml

Instrument: ECD_P
 ClientSampleId: AR1248ICC050


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/08/2025
 Supervised By :mohammad ahmed 07/09/2025

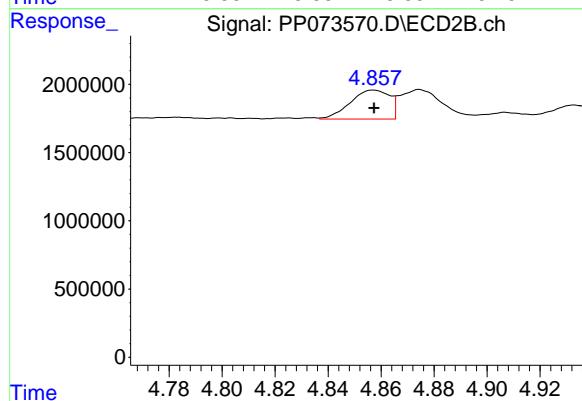


#21 AR-1248-1

R.T.: 4.857 min
 Delta R.T.: 0.000 min
 Response: 2193065
 Conc: 48.53 ng/ml

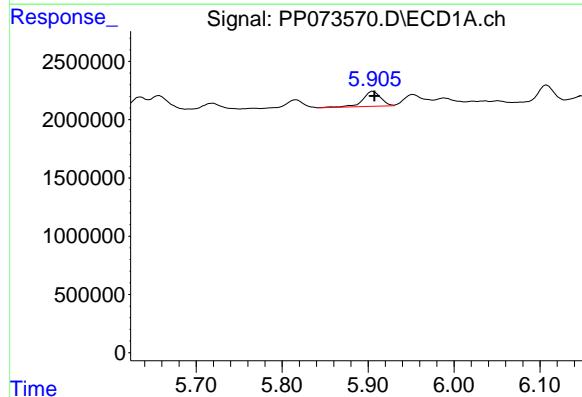

#22 AR-1248-2

R.T.: 5.906 min
 Delta R.T.: -0.001 min
 Response: 1882218
 Conc: 46.43 ng/ml

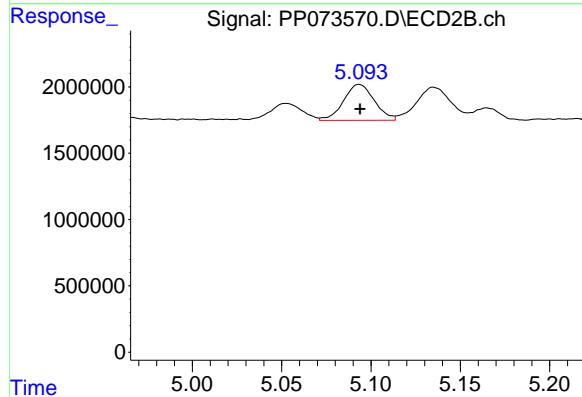

#22 AR-1248-2

R.T.: 5.093 min
 Delta R.T.: 0.000 min
 Response: 3238127
 Conc: 52.32 ng/ml

#23 AR-1248-3

R.T.: 6.108 min
 Delta R.T.: -0.001 min
 Response: 1881440
 Conc: 40.83 ng/ml

Instrument: ECD_P
ClientSampleId: AR1248ICC050

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/08/2025
 Supervised By :mohammad ahmed 07/09/2025

#23 AR-1248-3





R.T.: 5.135 min
 Delta R.T.: 0.000 min
 Response: 3334641
 Conc: 51.77 ng/ml

#24 AR-1248-4

R.T.: 6.506 min
 Delta R.T.: -0.002 min
 Response: 2458929
 Conc: 43.03 ng/ml

#24 AR-1248-4

R.T.: 5.307 min
 Delta R.T.: 0.000 min
 Response: 3957834
 Conc: 52.56 ng/ml

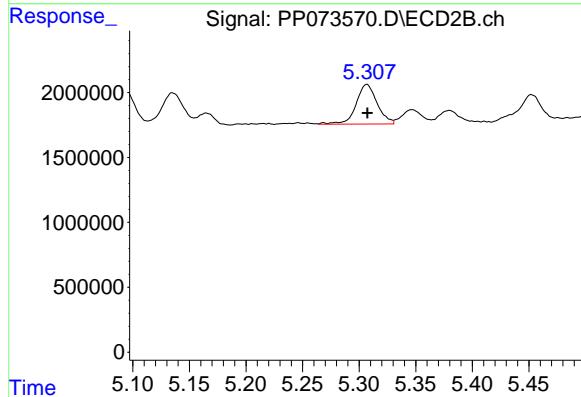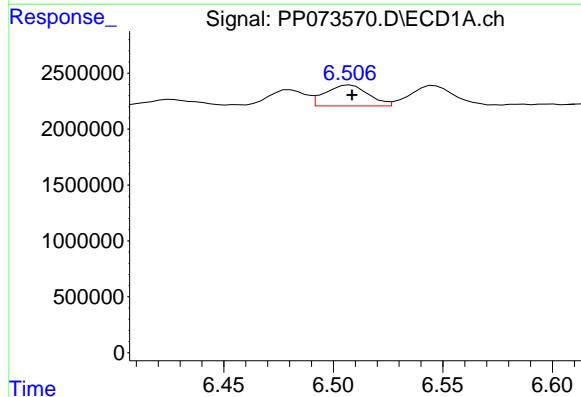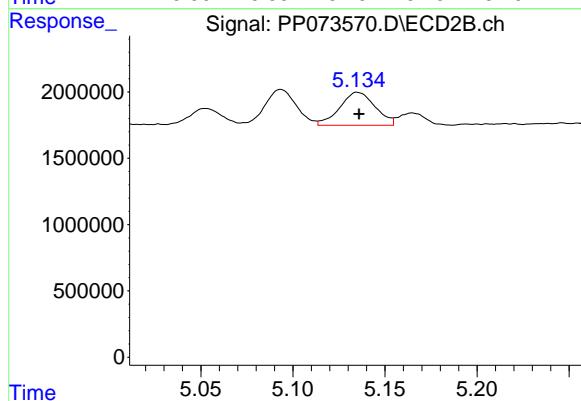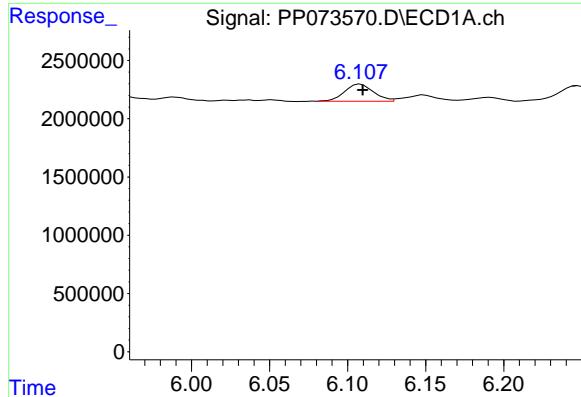



#25 AR-1248-5

R.T.: 6.545 min
 Delta R.T.: -0.003 min
 Response: 2487202
 Conc: 44.61 ng/ml

Instrument: ECD_P
ClientSampleId: AR1248ICC050

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/08/2025
 Supervised By :mohammad ahmed 07/09/2025

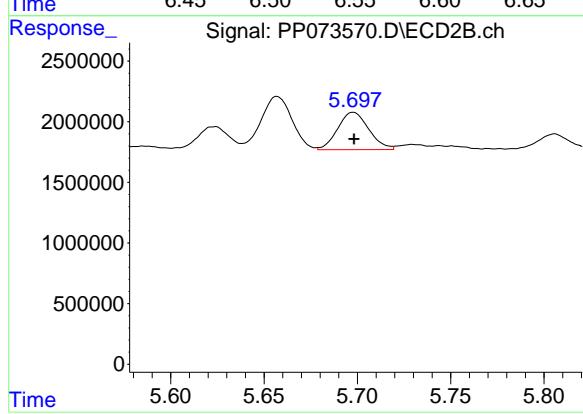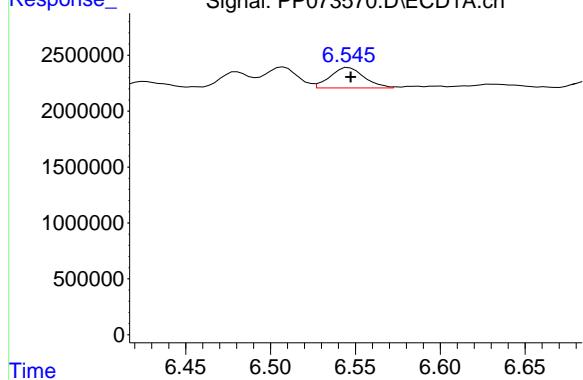

#25 AR-1248-5

R.T.: 5.698 min
 Delta R.T.: 0.000 min
 Response: 3594939
 Conc: 47.04 ng/ml

1
2
3
4
5
6
7
8
9
10
11
12
13
14
15
16
17
18
19
20

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP070825\
 Data File : PP073571.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jul 2025 01:41
 Operator : YP\AJ
 Sample : AR1254ICC1000
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
AR1254ICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 08 02:43:42 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 08 02:41:54 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	4.489	3.780	135.2E6	181.0E6	96.465	95.662
2) SA Decachlor...	10.177	8.782	110.7E6	134.8E6	96.695	98.240

Target Compounds

26) L6 AR-1254-1	6.487	5.658	50900598	105.4E6	921.959	938.043
27) L6 AR-1254-2	6.703	5.806	77237012	90612135	935.764	943.093
28) L6 AR-1254-3	7.066	6.207	83677544	142.5E6	945.590	936.990
29) L6 AR-1254-4	7.348	6.436	74438148	86996505	935.246	922.052
30) L6 AR-1254-5	7.764	6.851	71888659	123.6E6	963.395	945.380



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.





Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP070825\
 Data File : PP073571.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jul 2025 01:41
 Operator : YP\AJ
 Sample : AR1254ICC1000
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
AR1254ICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 08 02:43:42 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 08 02:41:54 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ m Signal #2 Info : 30M x 0.32mm x 0.25 μ m

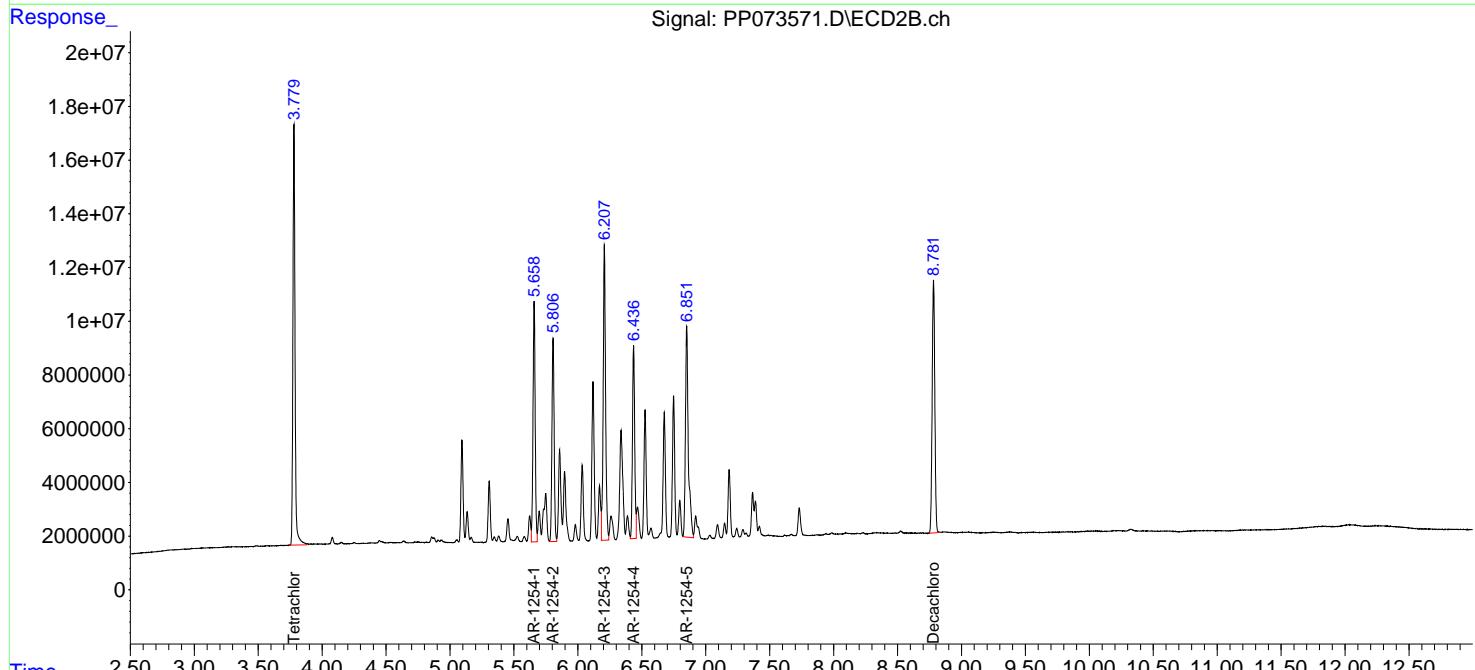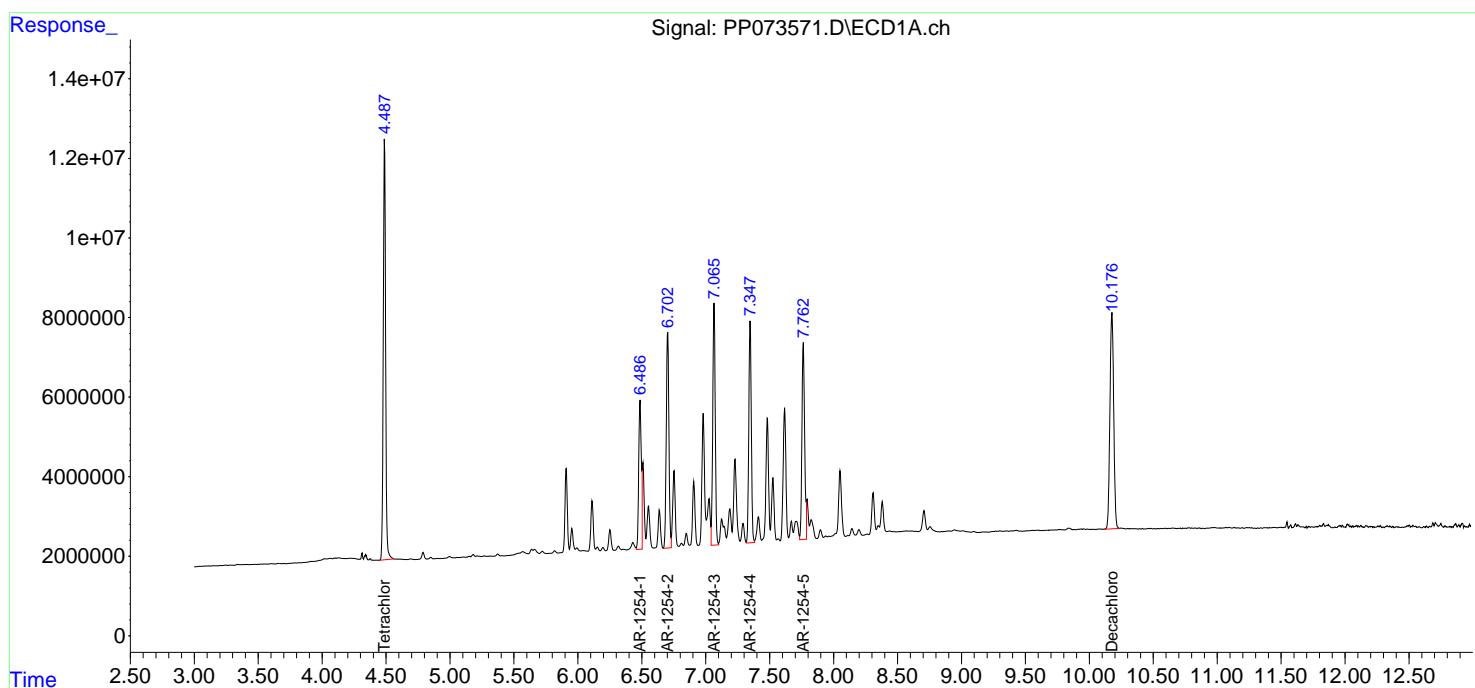

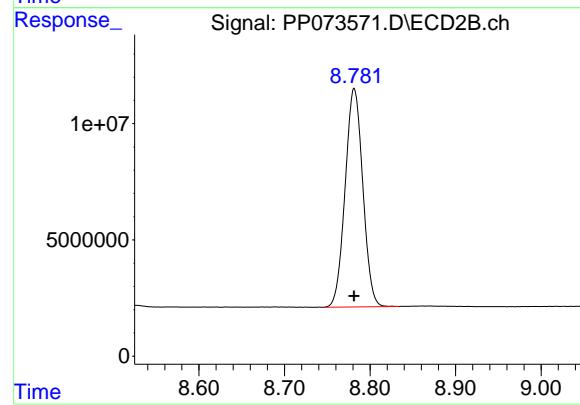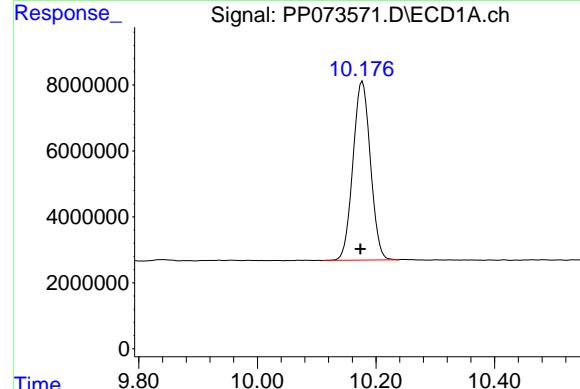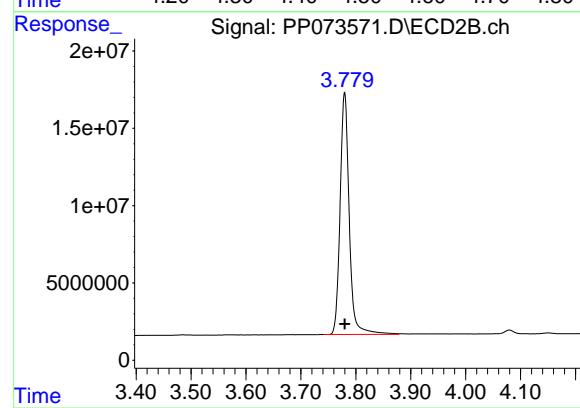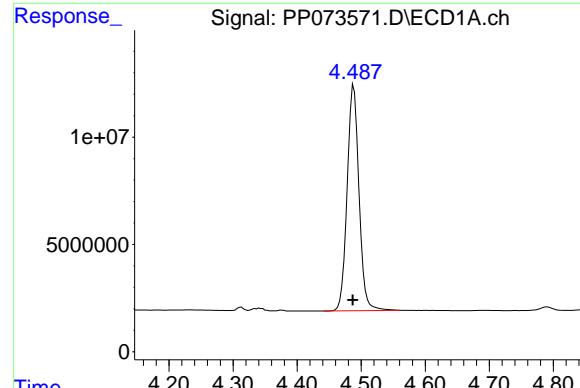

#1 Tetrachloro-m-xylene

R.T.: 4.489 min
 Delta R.T.: 0.002 min
 Response: 135162400
 Conc: 96.46 ng/ml

Instrument: ECD_P
 ClientSampleId : AR1254ICC1000

#1 Tetrachloro-m-xylene

R.T.: 3.780 min
 Delta R.T.: 0.000 min
 Response: 180994038
 Conc: 95.66 ng/ml

#2 Decachlorobiphenyl

R.T.: 10.177 min
 Delta R.T.: 0.003 min
 Response: 110743925
 Conc: 96.70 ng/ml





#2 Decachlorobiphenyl

R.T.: 8.782 min
 Delta R.T.: 0.000 min
 Response: 134819228
 Conc: 98.24 ng/ml

#26 AR-1254-1

R.T.: 6.487 min
 Delta R.T.: 0.002 min
 Response: 50900598
 Conc: 921.96 ng/ml

Instrument: ECD_P
ClientSampleId: AR1254ICC1000

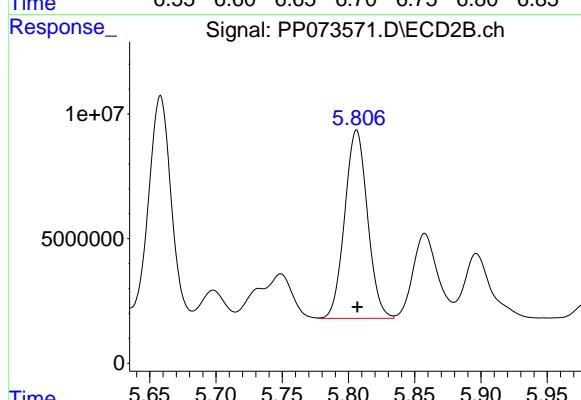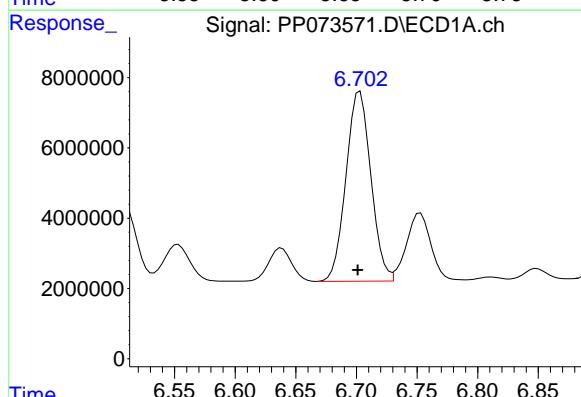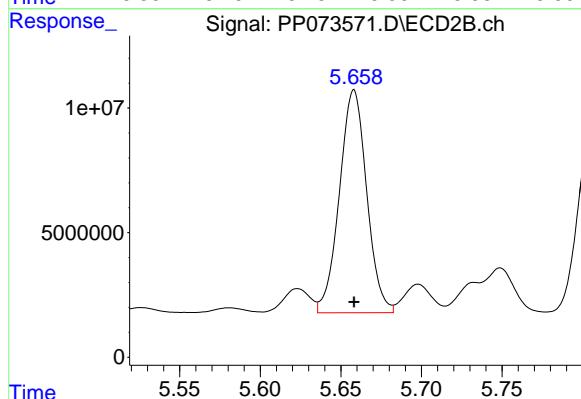

#26 AR-1254-1


R.T.: 5.658 min
 Delta R.T.: 0.000 min
 Response: 105364555
 Conc: 938.04 ng/ml

#27 AR-1254-2

R.T.: 6.703 min
 Delta R.T.: 0.002 min
 Response: 77237012
 Conc: 935.76 ng/ml

#27 AR-1254-2

R.T.: 5.806 min
 Delta R.T.: 0.000 min
 Response: 90612135
 Conc: 943.09 ng/ml

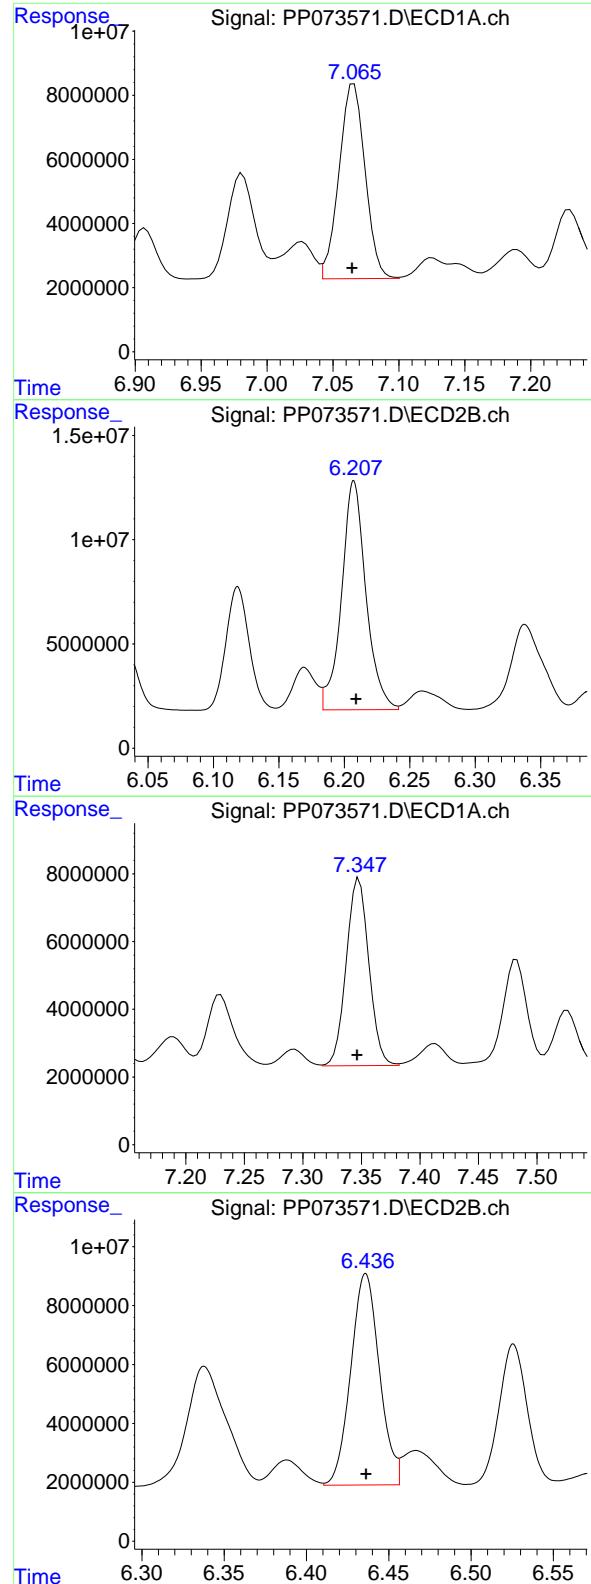

#28 AR-1254-3

R.T.: 7.066 min
 Delta R.T.: 0.002 min
 Response: 83677544
 Conc: 945.59 ng/ml

Instrument: ECD_P
 ClientSampleId: AR1254ICC1000

#28 AR-1254-3

R.T.: 6.207 min
 Delta R.T.: -0.002 min
 Response: 142515413
 Conc: 936.99 ng/ml

#29 AR-1254-4

R.T.: 7.348 min
 Delta R.T.: 0.002 min
 Response: 74438148
 Conc: 935.25 ng/ml



#29 AR-1254-4

R.T.: 6.436 min
 Delta R.T.: 0.000 min
 Response: 86996505
 Conc: 922.05 ng/ml

#30 AR-1254-5

R.T.: 7.764 min
Delta R.T.: 0.002 min
Response: 71888659
Conc: 963.40 ng/ml

Instrument: ECD_P
ClientSampleId: AR1254ICC1000

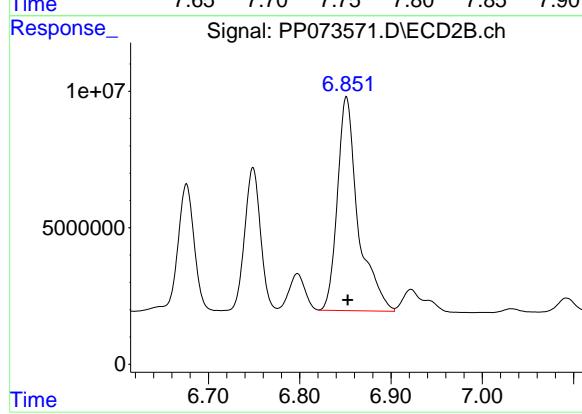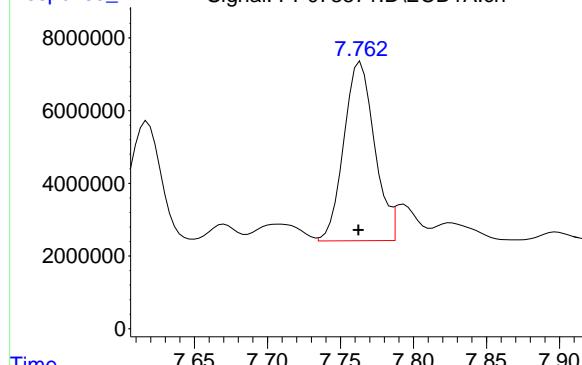

#30 AR-1254-5

R.T.: 6.851 min
Delta R.T.: -0.001 min
Response: 123596587
Conc: 945.38 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP070825\
 Data File : PP073572.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jul 2025 01:57
 Operator : YP\AJ
 Sample : AR1254ICC750
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
AR1254ICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 08 02:44:03 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 08 02:41:54 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	4.488	3.779	104.7E6	146.2E6	74.706	77.291
2) SA Decachlor...	10.175	8.780	84962440	104.9E6	74.184	76.426

Target Compounds

26) L6 AR-1254-1	6.486	5.657	39869819	83773101	722.159	745.818
27) L6 AR-1254-2	6.702	5.805	60389680	72154275	731.651	750.983
28) L6 AR-1254-3	7.066	6.207	64508177	114.2E6	728.969	750.593
29) L6 AR-1254-4	7.348	6.435	57167227	70426326	718.253	746.429
30) L6 AR-1254-5	7.764	6.851	55929557	98283712	749.524	751.764



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP070825\
 Data File : PP073572.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jul 2025 01:57
 Operator : YP\AJ
 Sample : AR1254ICC750
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
AR1254ICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 08 02:44:03 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 08 02:41:54 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ m Signal #2 Info : 30M x 0.32mm x 0.25 μ m

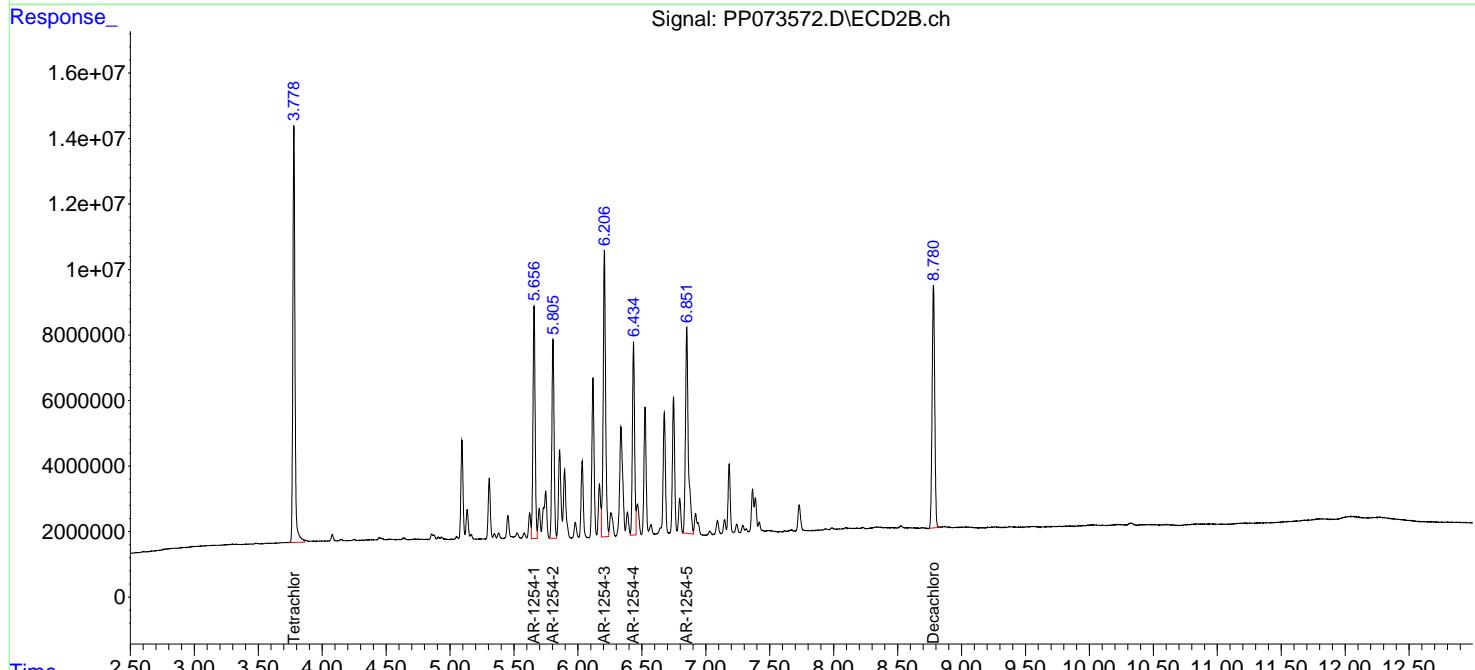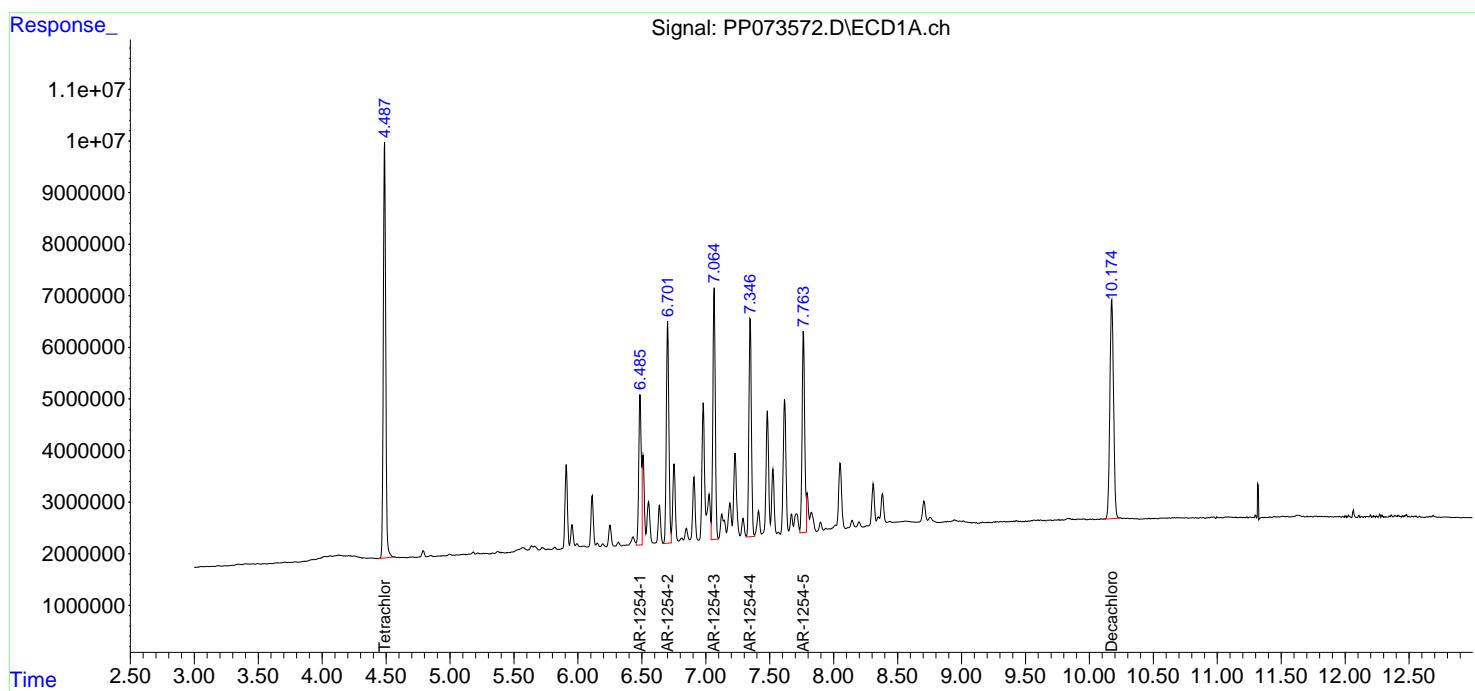

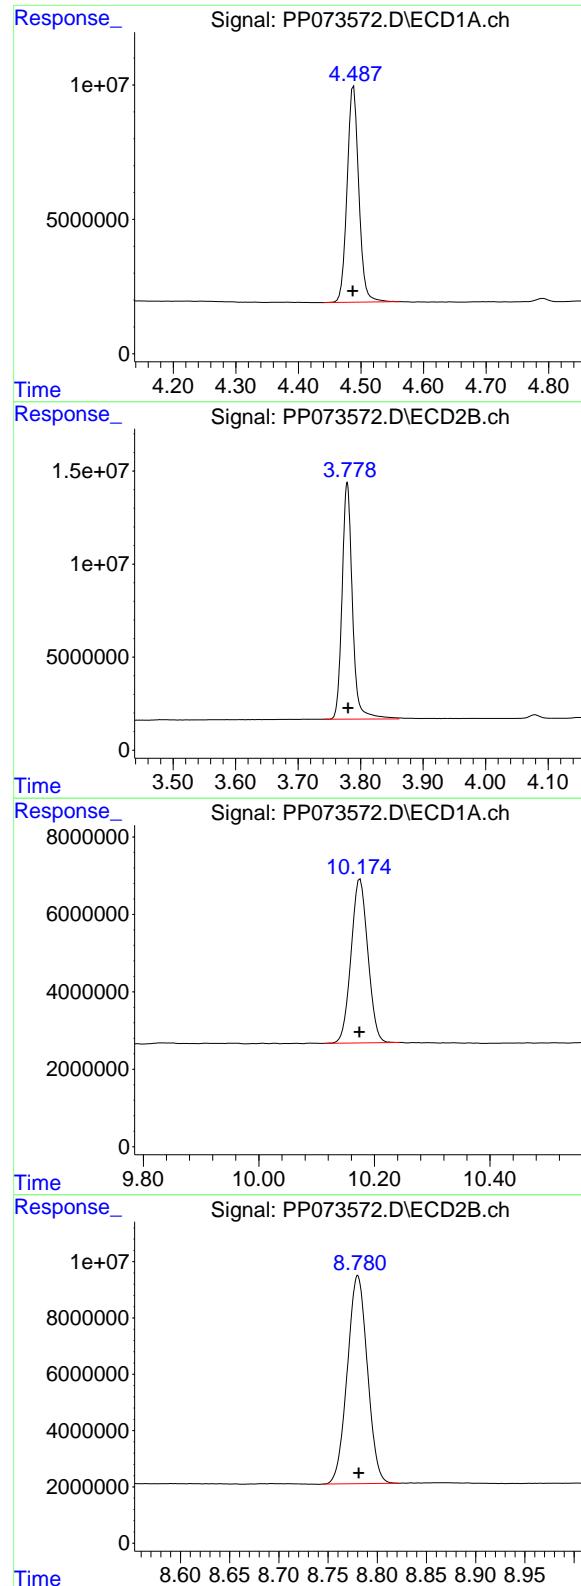

#1 Tetrachloro-m-xylene

R.T.: 4.488 min
 Delta R.T.: 0.001 min
 Response: 104674567
 Conc: 74.71 ng/ml

Instrument: ECD_P
 ClientSampleId: AR1254ICC750

#1 Tetrachloro-m-xylene

R.T.: 3.779 min
 Delta R.T.: -0.001 min
 Response: 146235464
 Conc: 77.29 ng/ml

#2 Decachlorobiphenyl

R.T.: 10.175 min
 Delta R.T.: 0.001 min
 Response: 84962440
 Conc: 74.18 ng/ml


#2 Decachlorobiphenyl

R.T.: 8.780 min
 Delta R.T.: -0.001 min
 Response: 104882292
 Conc: 76.43 ng/ml

#26 AR-1254-1


R.T.: 6.486 min
 Delta R.T.: 0.001 min
 Response: 39869819
 Conc: 722.16 ng/ml

Instrument: ECD_P
ClientSampleId: AR1254ICC750

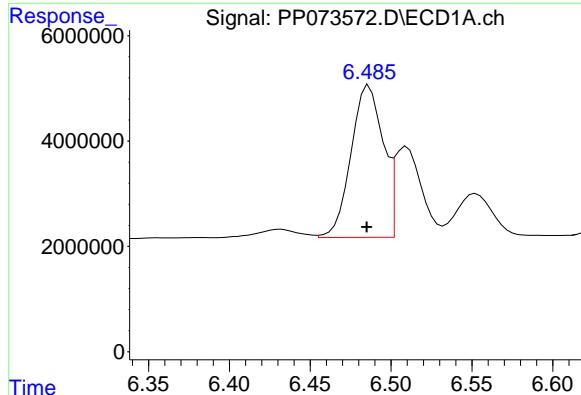


#26 AR-1254-1

R.T.: 5.657 min
 Delta R.T.: -0.001 min
 Response: 83773101
 Conc: 745.82 ng/ml

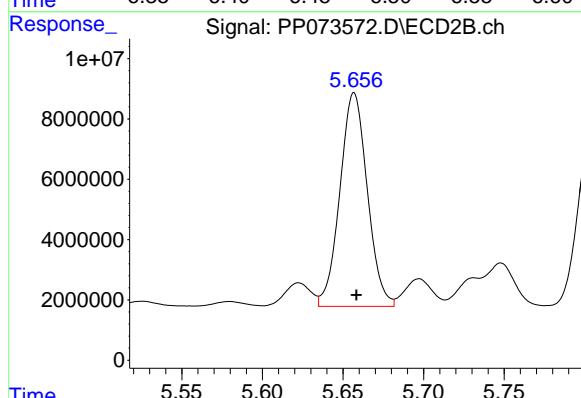


#27 AR-1254-2

R.T.: 6.702 min
 Delta R.T.: 0.000 min
 Response: 60389680
 Conc: 731.65 ng/ml

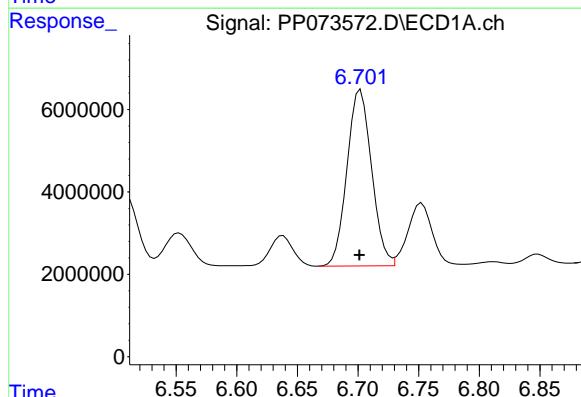

#27 AR-1254-2


R.T.: 5.805 min
 Delta R.T.: -0.002 min
 Response: 72154275
 Conc: 750.98 ng/ml

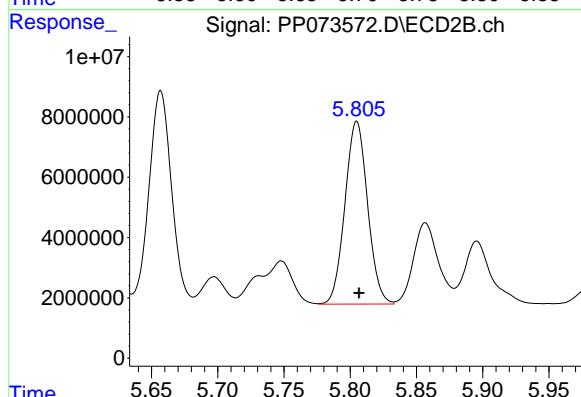

#28 AR-1254-3


R.T.: 7.066 min
 Delta R.T.: 0.001 min
 Response: 64508177
 Conc: 728.97 ng/ml

Instrument: ECD_P
ClientSampleId: AR1254ICC750

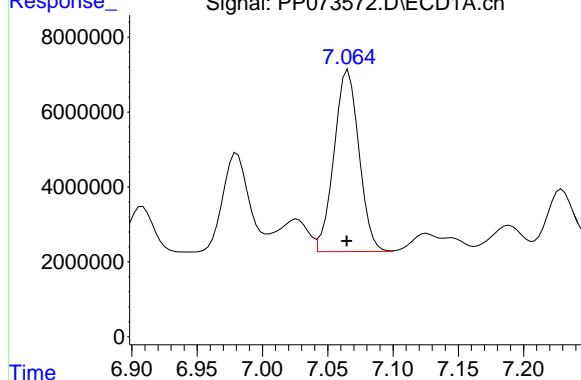


#28 AR-1254-3

R.T.: 6.207 min
 Delta R.T.: -0.002 min
 Response: 114164607
 Conc: 750.59 ng/ml

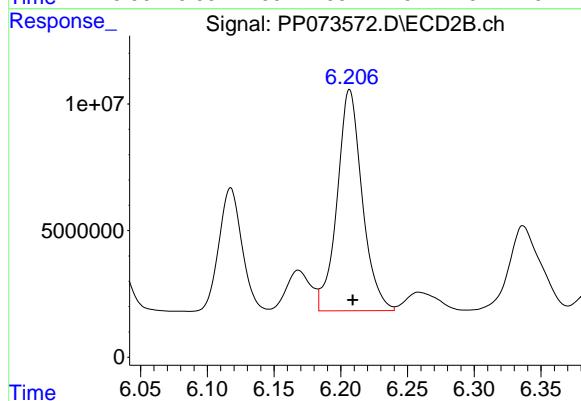


#29 AR-1254-4

R.T.: 7.348 min
 Delta R.T.: 0.002 min
 Response: 57167227
 Conc: 718.25 ng/ml




#29 AR-1254-4

R.T.: 6.435 min
 Delta R.T.: -0.001 min
 Response: 70426326
 Conc: 746.43 ng/ml

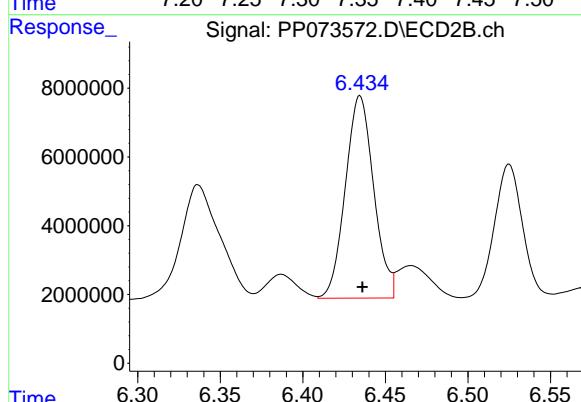

#30 AR-1254-5

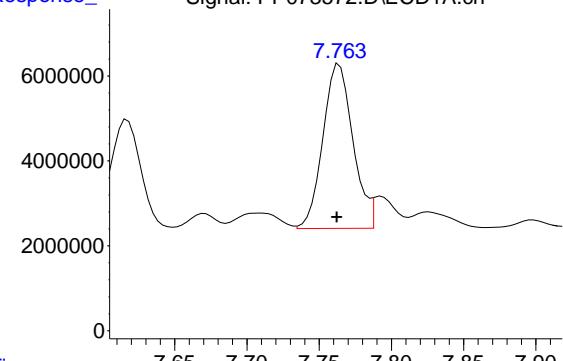


R.T.: 7.764 min
Delta R.T.: 0.002 min
Response: 55929557
Conc: 749.52 ng/ml

Instrument: ECD_P
ClientSampleId: AR1254ICC750

#30 AR-1254-5

R.T.: 6.851 min
Delta R.T.: -0.002 min
Response: 98283712
Conc: 751.76 ng/ml

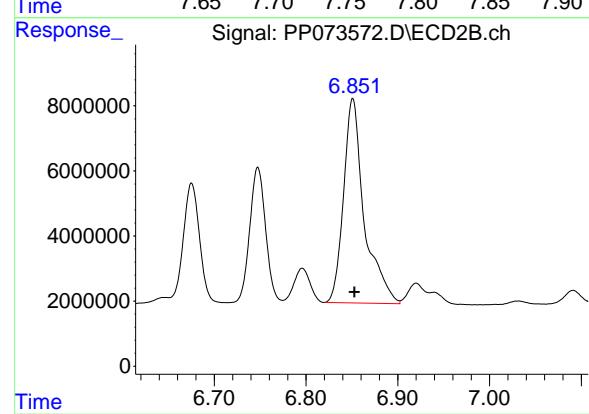

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP070825\
 Data File : PP073573.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jul 2025 02:14
 Operator : YP\AJ
 Sample : AR1254ICC500
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
AR1254ICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 08 02:44:25 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 08 02:41:54 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	4.487	3.780	70057774	94600770	50.000	50.000
2) SA Decachlor...	10.174	8.781	57264429	68616932	50.000	50.000

Target Compounds

26) L6 AR-1254-1	6.485	5.658	27604602	56161903	500.000	500.000
27) L6 AR-1254-2	6.701	5.807	41269473	48039880	500.000	500.000
28) L6 AR-1254-3	7.064	6.209	44246186	76049574	500.000	500.000
29) L6 AR-1254-4	7.346	6.436	39796020	47175510	500.000	500.000
30) L6 AR-1254-5	7.762	6.853	37310051	65368722	500.000	500.000


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.





Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP070825\
 Data File : PP073573.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jul 2025 02:14
 Operator : YP\AJ
 Sample : AR1254ICC500
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
AR1254ICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 08 02:44:25 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 08 02:41:54 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ m Signal #2 Info : 30M x 0.32mm x 0.25 μ m

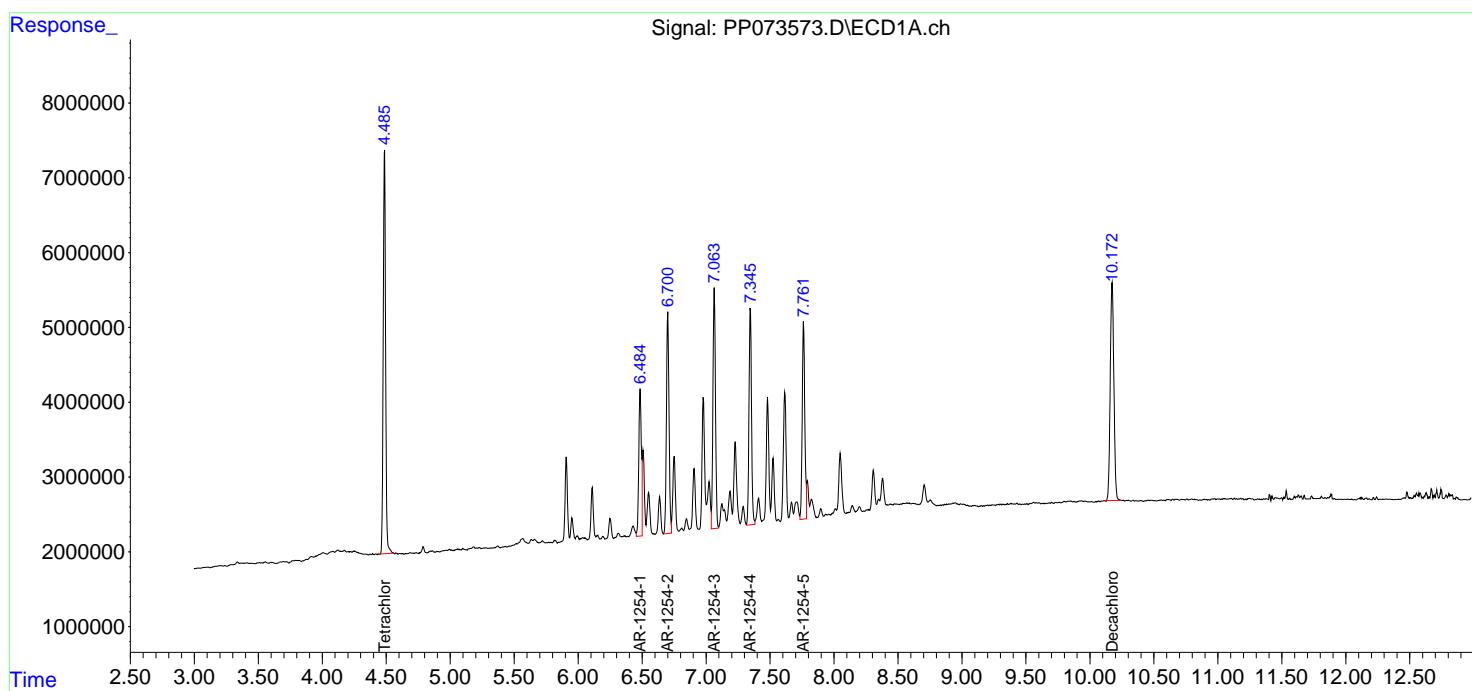

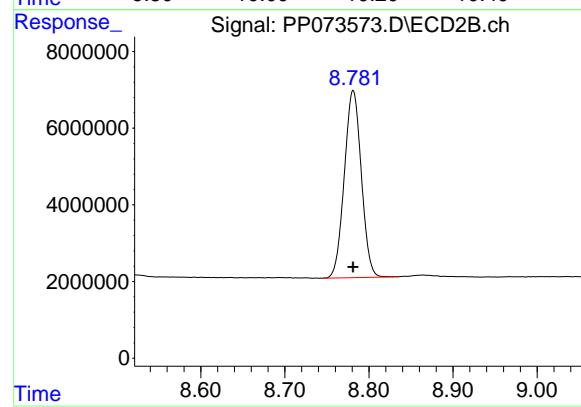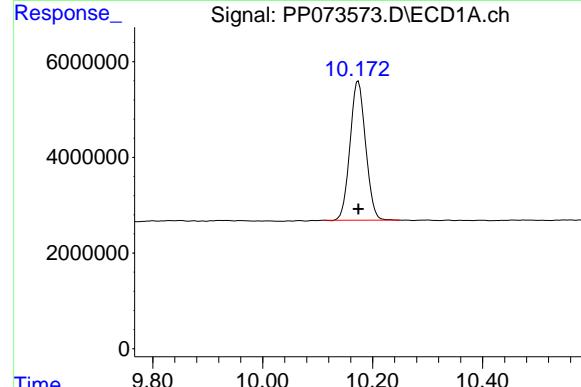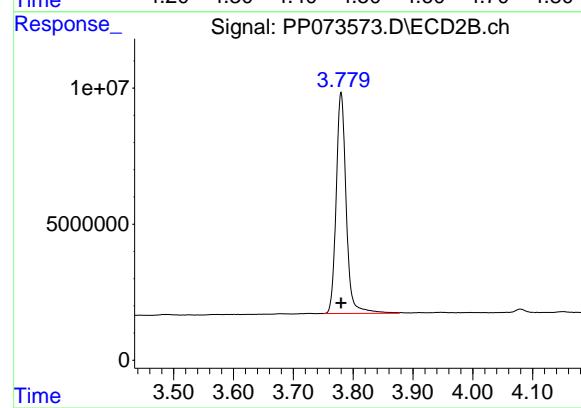

#1 Tetrachloro-m-xylene

R.T.: 4.487 min
 Delta R.T.: 0.000 min
 Response: 70057774
 Conc: 50.00 ng/ml

Instrument:

ECD_P

ClientSampleId :

AR1254ICC500

#1 Tetrachloro-m-xylene


R.T.: 3.780 min
 Delta R.T.: 0.000 min
 Response: 94600770
 Conc: 50.00 ng/ml

#2 Decachlorobiphenyl

R.T.: 10.174 min
 Delta R.T.: 0.000 min
 Response: 57264429
 Conc: 50.00 ng/ml

#2 Decachlorobiphenyl

R.T.: 8.781 min
 Delta R.T.: 0.000 min
 Response: 68616932
 Conc: 50.00 ng/ml

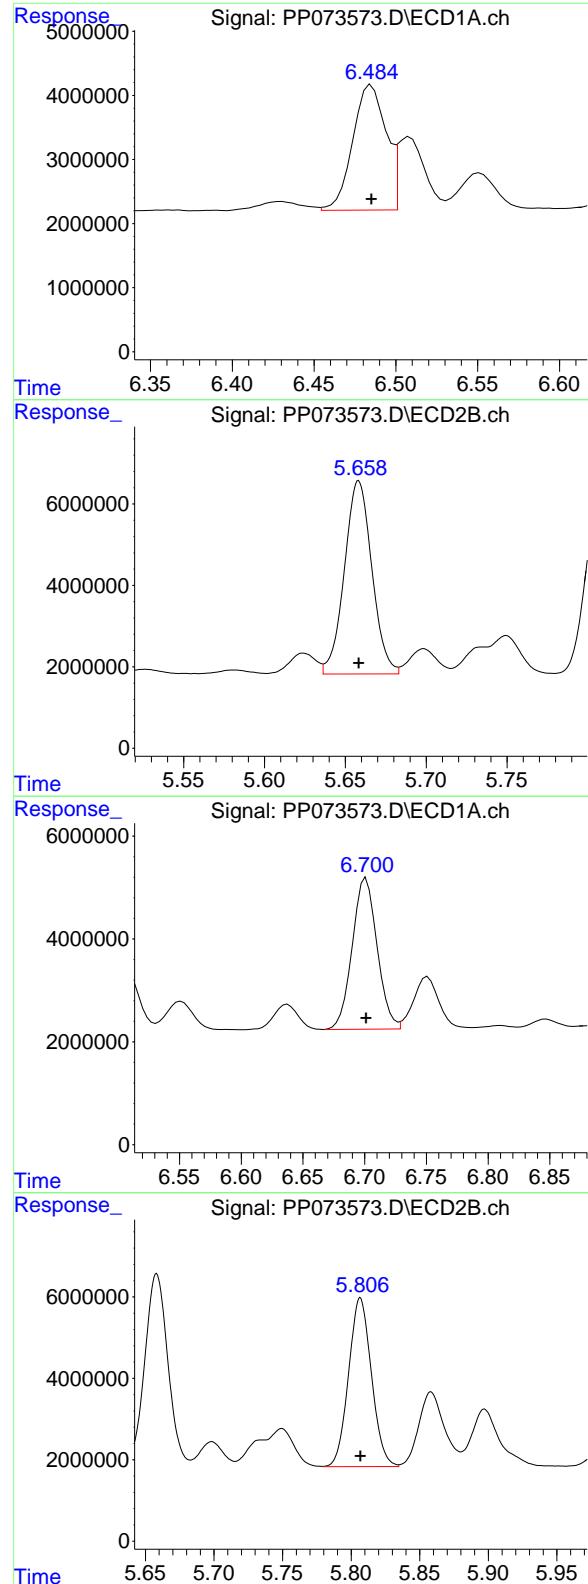

#26 AR-1254-1

R.T.: 6.485 min
 Delta R.T.: 0.000 min
 Response: 27604602
 Conc: 500.00 ng/ml

Instrument: ECD_P
 ClientSampleId: AR1254ICC500

#26 AR-1254-1

R.T.: 5.658 min
 Delta R.T.: 0.000 min
 Response: 56161903
 Conc: 500.00 ng/ml

#27 AR-1254-2

R.T.: 6.701 min
 Delta R.T.: 0.000 min
 Response: 41269473
 Conc: 500.00 ng/ml


#27 AR-1254-2

R.T.: 5.807 min
 Delta R.T.: 0.000 min
 Response: 48039880
 Conc: 500.00 ng/ml

#28 AR-1254-3


R.T.: 7.064 min
 Delta R.T.: 0.000 min
 Response: 44246186
 Conc: 500.00 ng/ml

Instrument: ECD_P
ClientSampleId: AR1254ICC500




#28 AR-1254-3

R.T.: 6.209 min
 Delta R.T.: 0.000 min
 Response: 76049574
 Conc: 500.00 ng/ml

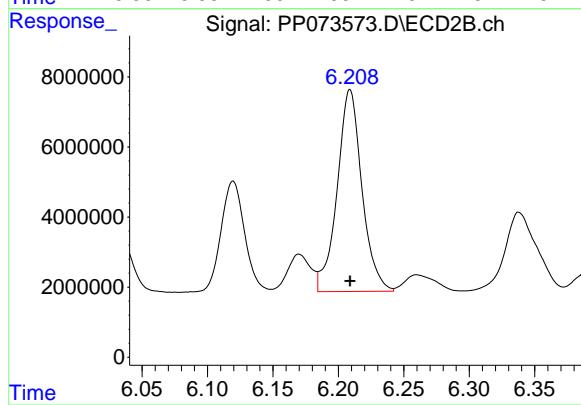


#29 AR-1254-4

R.T.: 7.346 min
 Delta R.T.: 0.000 min
 Response: 39796020
 Conc: 500.00 ng/ml



#29 AR-1254-4



R.T.: 6.436 min
 Delta R.T.: 0.000 min
 Response: 47175510
 Conc: 500.00 ng/ml

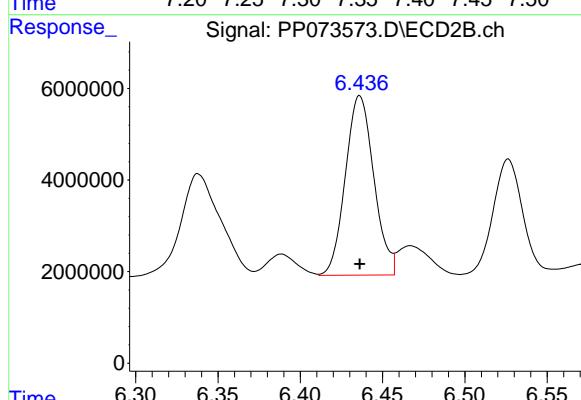

#30 AR-1254-5

R.T.: 7.762 min
Delta R.T.: 0.000 min
Response: 37310051
Conc: 500.00 ng/ml

Instrument: ECD_P
ClientSampleId: AR1254ICC500

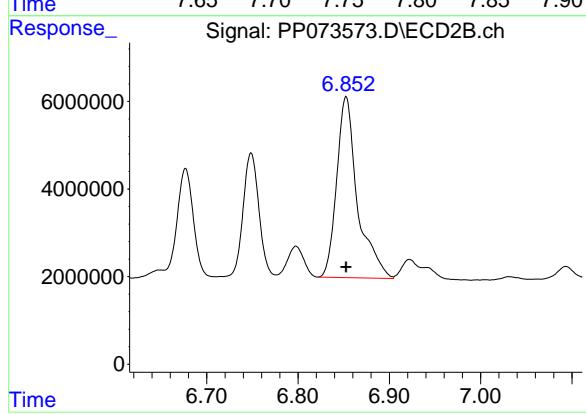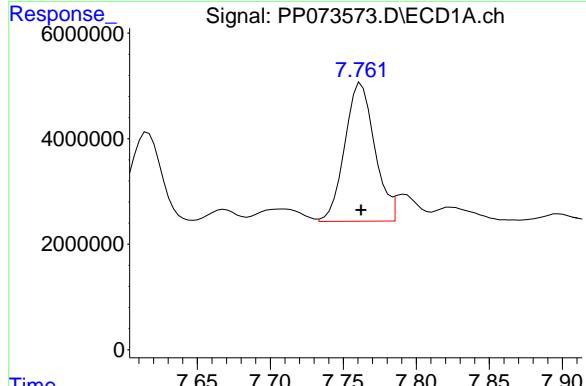

#30 AR-1254-5

R.T.: 6.853 min
Delta R.T.: 0.000 min
Response: 65368722
Conc: 500.00 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP070825\
 Data File : PP073574.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jul 2025 02:30
 Operator : YP\AJ
 Sample : AR1254ICC250
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
AR1254ICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 08 02:44:44 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 08 02:41:54 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	4.487	3.779	36639041	48313312	26.149	25.535
2) SA Decachlor...	10.176	8.780	28626907	37692438	24.995	27.466

Target Compounds

26) L6 AR-1254-1	6.484	5.657	14279096	30427905	258.636	270.895
27) L6 AR-1254-2	6.701	5.805	21587177	26282271	261.539	273.546
28) L6 AR-1254-3	7.064	6.207	23018010	40529659	260.113	266.469
29) L6 AR-1254-4	7.346	6.435	20463711	25097390	257.108	266.000
30) L6 AR-1254-5	7.762	6.851	19086937	35261681	255.788	269.714



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP070825\
 Data File : PP073574.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jul 2025 02:30
 Operator : YP\AJ
 Sample : AR1254ICC250
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
AR1254ICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 08 02:44:44 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 08 02:41:54 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

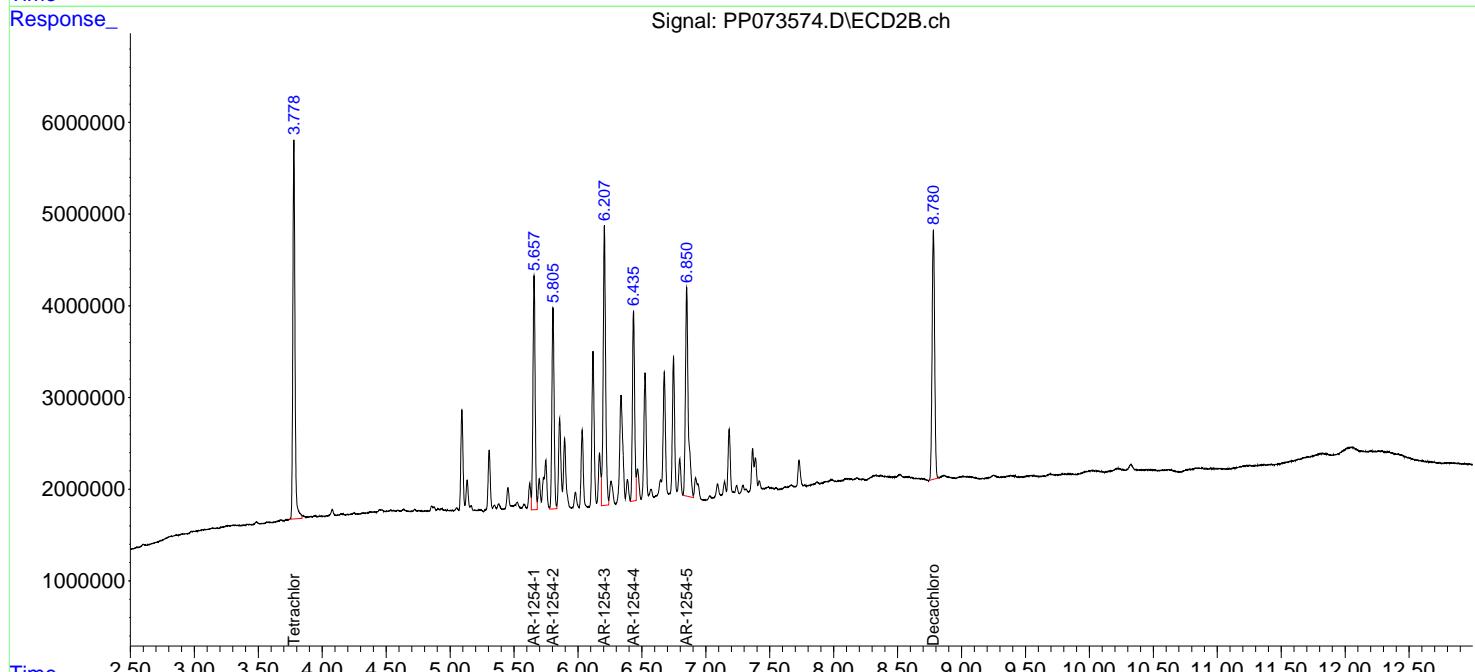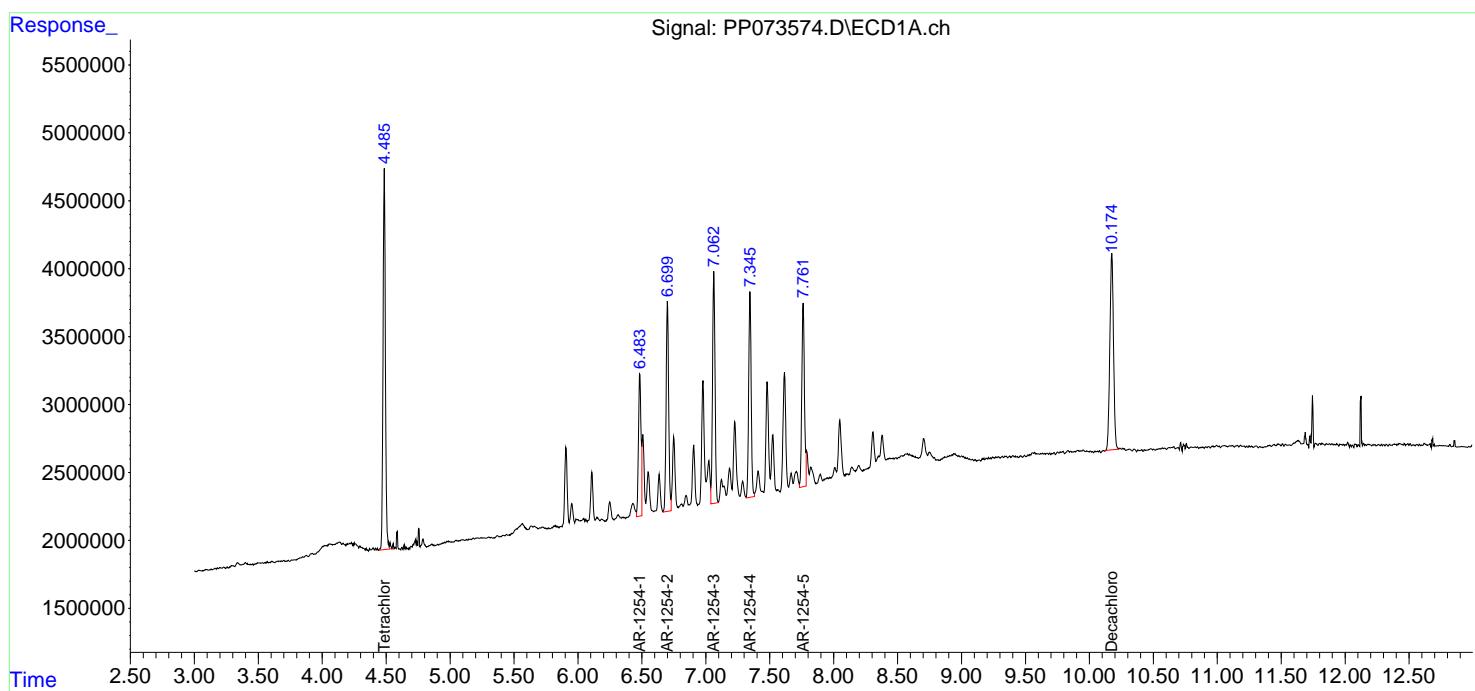

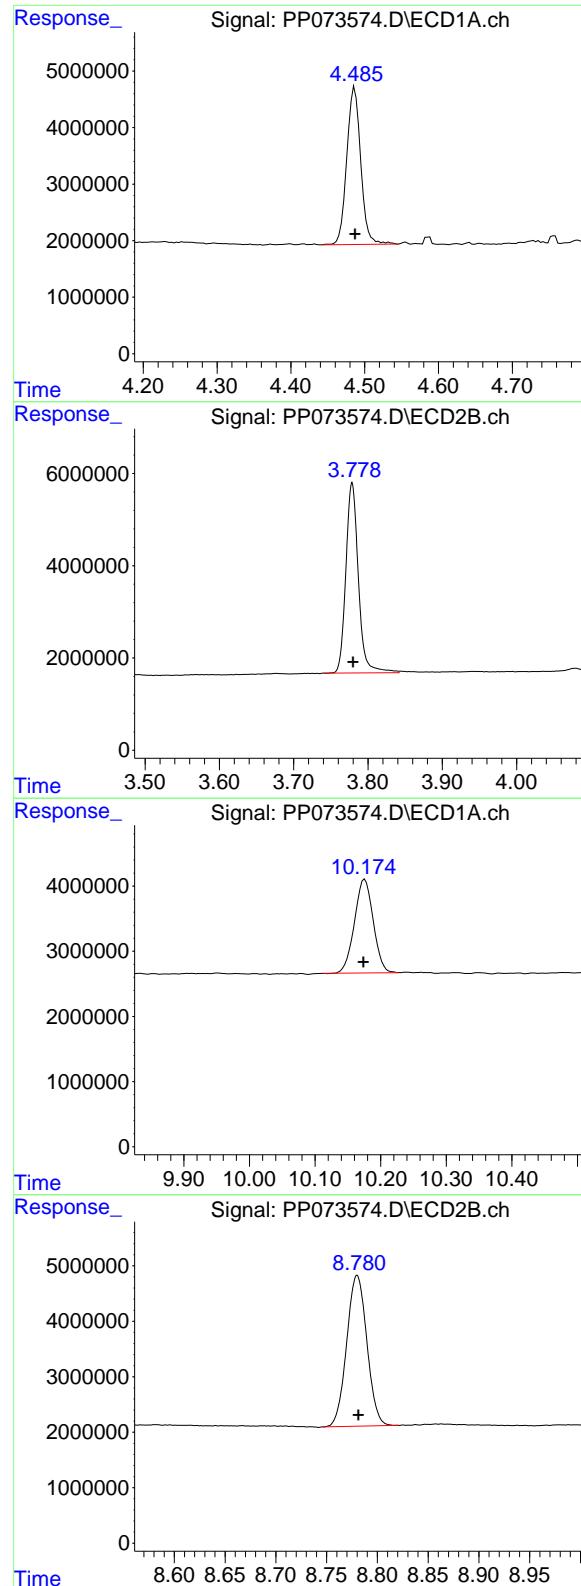

#1 Tetrachloro-m-xylene

R.T.: 4.487 min
 Delta R.T.: 0.000 min
 Response: 36639041
 Conc: 26.15 ng/ml

Instrument : ECD_P

ClientSampleId : AR1254ICC250

#1 Tetrachloro-m-xylene

R.T.: 3.779 min
 Delta R.T.: -0.001 min
 Response: 48313312
 Conc: 25.54 ng/ml

#2 Decachlorobiphenyl

R.T.: 10.176 min
 Delta R.T.: 0.002 min
 Response: 28626907
 Conc: 25.00 ng/ml


#2 Decachlorobiphenyl

R.T.: 8.780 min
 Delta R.T.: -0.001 min
 Response: 37692438
 Conc: 27.47 ng/ml

#26 AR-1254-1


R.T.: 6.484 min
 Delta R.T.: 0.000 min
 Response: 14279096
 Conc: 258.64 ng/ml

Instrument: ECD_P
 ClientSampleId: AR1254ICC250

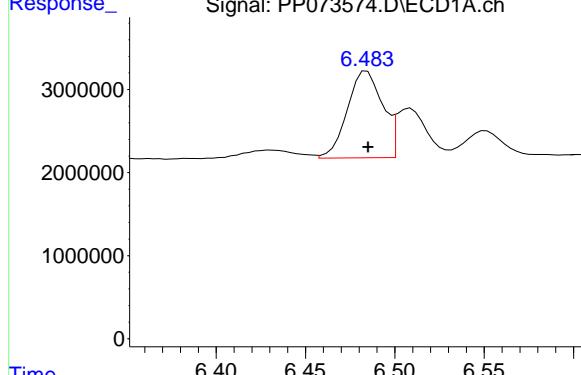


#26 AR-1254-1

R.T.: 5.657 min
 Delta R.T.: -0.001 min
 Response: 30427905
 Conc: 270.89 ng/ml

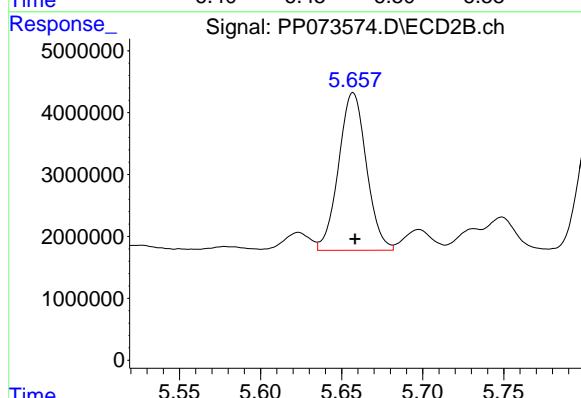


#27 AR-1254-2

R.T.: 6.701 min
 Delta R.T.: 0.000 min
 Response: 21587177
 Conc: 261.54 ng/ml

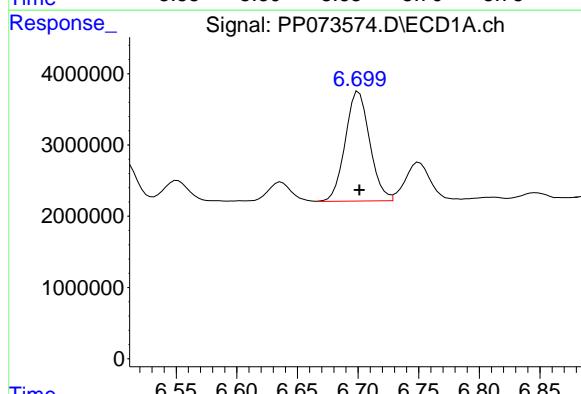

#27 AR-1254-2


R.T.: 5.805 min
 Delta R.T.: -0.002 min
 Response: 26282271
 Conc: 273.55 ng/ml

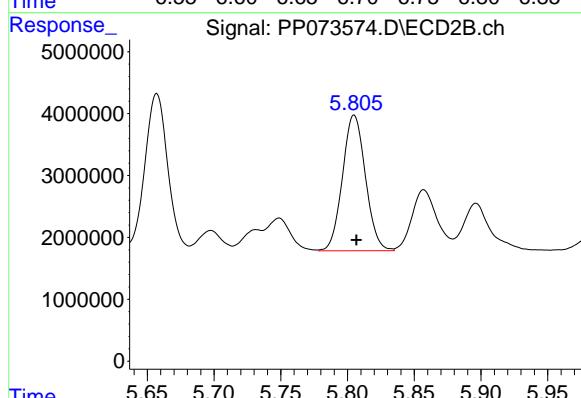

#28 AR-1254-3


R.T.: 7.064 min
 Delta R.T.: 0.000 min
 Response: 23018010
 Conc: 260.11 ng/ml

Instrument: ECD_P
ClientSampleId: AR1254ICC250

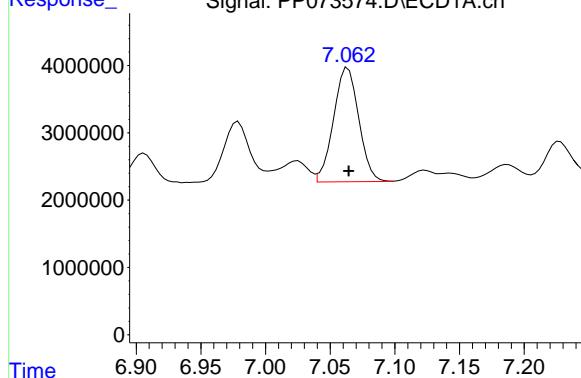


#28 AR-1254-3

R.T.: 6.207 min
 Delta R.T.: -0.002 min
 Response: 40529659
 Conc: 266.47 ng/ml

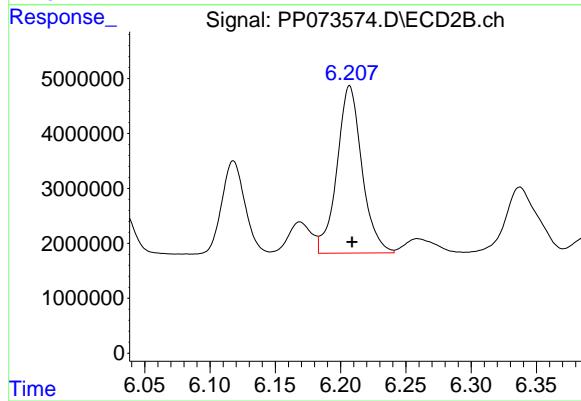


#29 AR-1254-4

R.T.: 7.346 min
 Delta R.T.: 0.000 min
 Response: 20463711
 Conc: 257.11 ng/ml

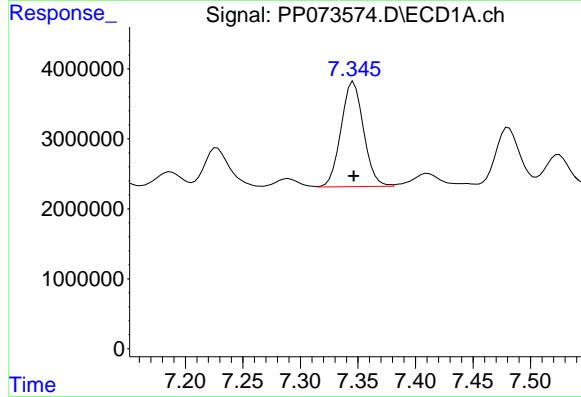

#29 AR-1254-4



R.T.: 6.435 min
 Delta R.T.: -0.001 min
 Response: 25097390
 Conc: 266.00 ng/ml

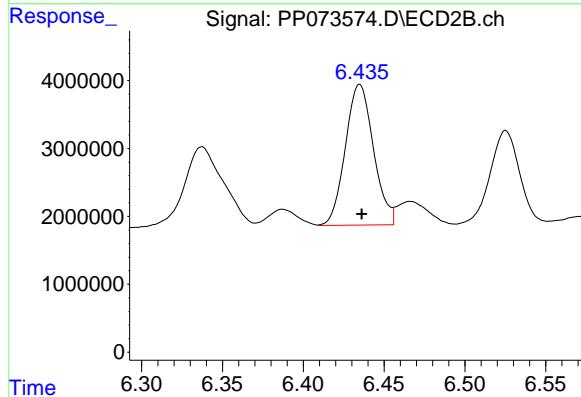

#30 AR-1254-5

R.T.: 7.762 min
Delta R.T.: 0.000 min
Response: 19086937
Conc: 255.79 ng/ml

Instrument: ECD_P
ClientSampleId: AR1254ICC250

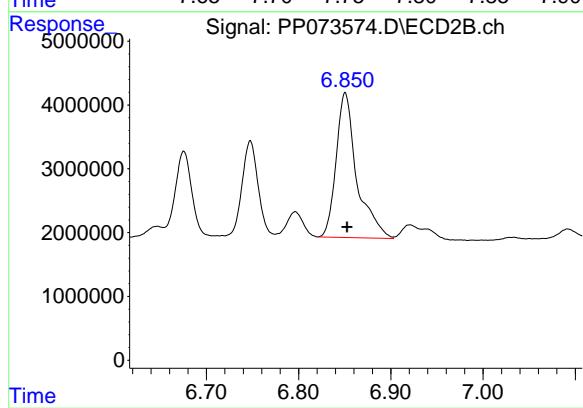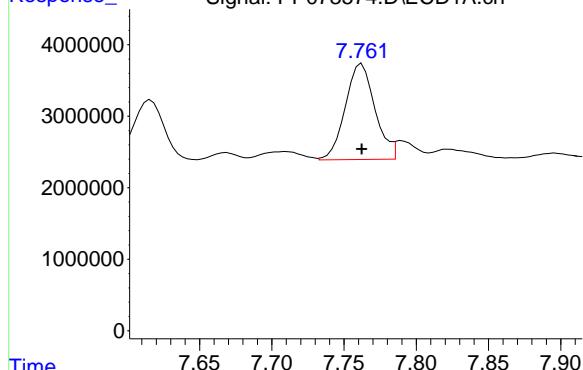

#30 AR-1254-5

R.T.: 6.851 min
Delta R.T.: -0.002 min
Response: 35261681
Conc: 269.71 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP070825\
 Data File : PP073575.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jul 2025 02:46
 Operator : YP\AJ
 Sample : AR1254ICC050
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
AR1254ICC050

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/08/2025
 Supervised By :mohammad ahmed 07/09/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 08 03:42:13 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 08 02:41:54 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	4.488	3.779	6938090	9721913	4.952	5.138
2) SA Decachlor...	10.178	8.780	5667149	6887289	4.948	5.019

Target Compounds

26) L6 AR-1254-1	6.485	5.657	2578085	6452648	46.697m	57.447
27) L6 AR-1254-2	6.701	5.806	4490008	5754555	54.399m	59.894
28) L6 AR-1254-3	7.064	6.207	4570279	8163980	51.646m	53.675
29) L6 AR-1254-4	7.347	6.436	4061359	4857854	51.027m	51.487
30) L6 AR-1254-5	7.764	6.851	3548489	7039930	47.554	53.848

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP070825\
 Data File : PP073575.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jul 2025 02:46
 Operator : YP\AJ
 Sample : AR1254ICC050
 Misc :
 ALS Vial : 24 Sample Multiplier: 1



Instrument :
 ECD_P
 ClientSampleId :
 AR1254ICC050


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/08/2025
 Supervised By :mohammad ahmed 07/09/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 08 03:42:13 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 08 02:41:54 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

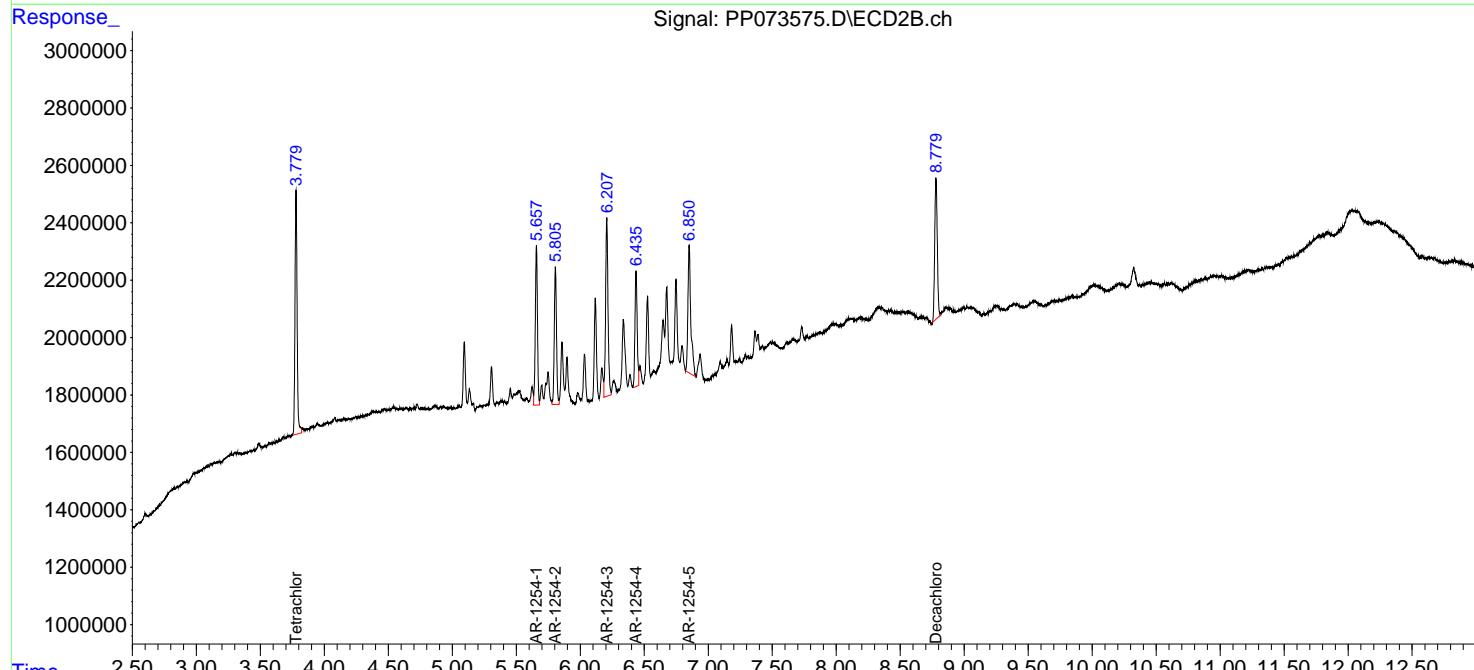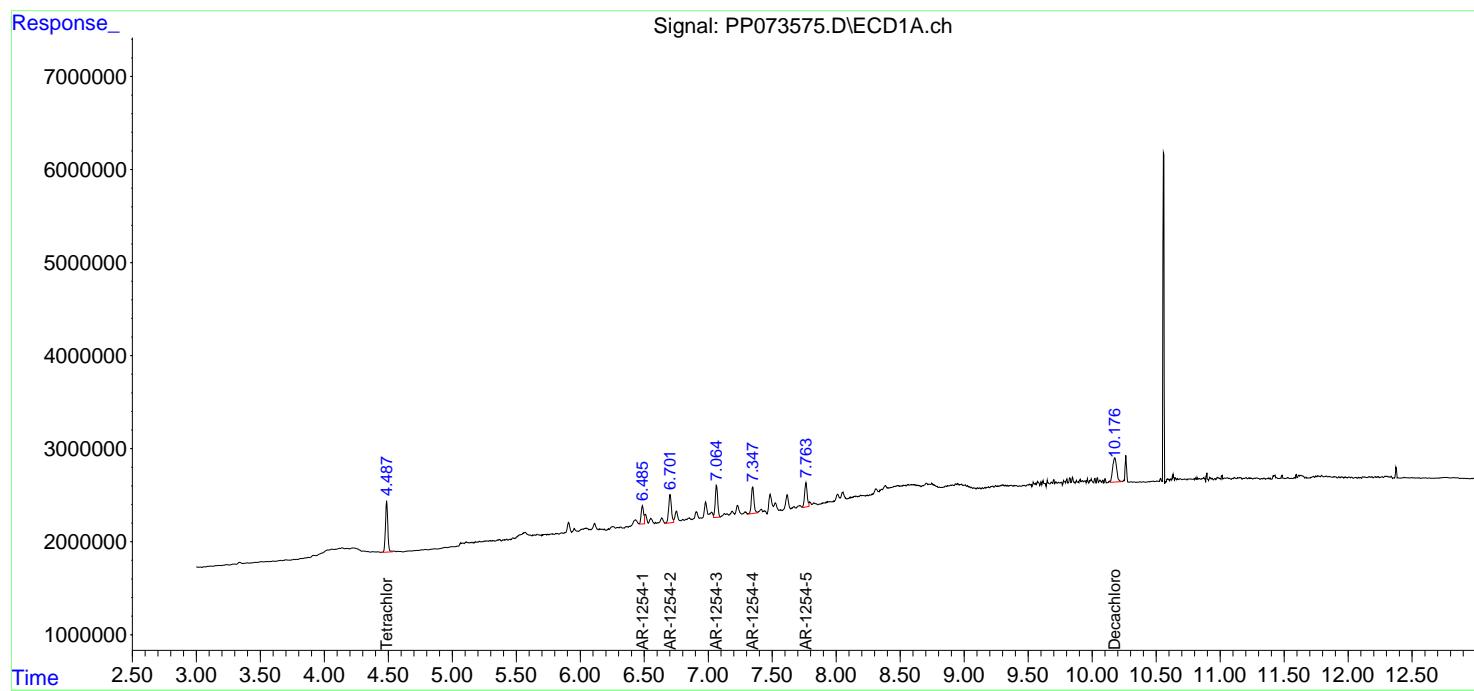

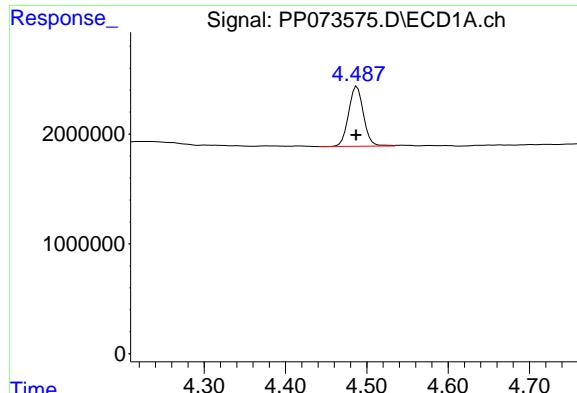


#1 Tetrachloro-m-xylene

R.T.: 4.488 min
Delta R.T.: 0.001 min
Response: 6938090
Conc: 4.95 ng/ml

Instrument: ECD_P
ClientSampleId: AR1254ICC050


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/08/2025
Supervised By :mohammad ahmed 07/09/2025

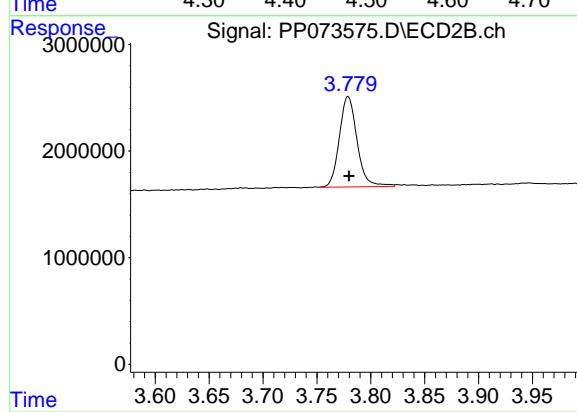


#1 Tetrachloro-m-xylene

R.T.: 3.779 min
Delta R.T.: 0.000 min
Response: 9721913
Conc: 5.14 ng/ml



#2 Decachlorobiphenyl

R.T.: 10.178 min
Delta R.T.: 0.004 min
Response: 5667149
Conc: 4.95 ng/ml

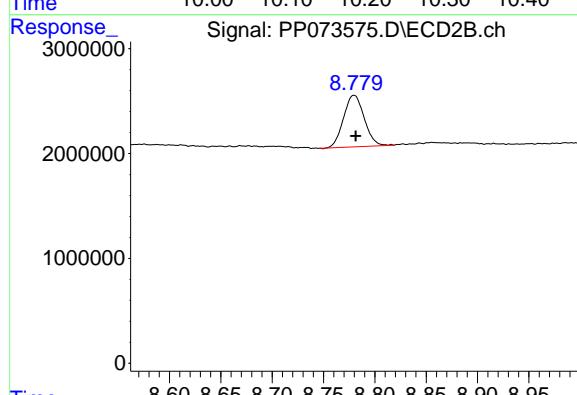

#2 Decachlorobiphenyl

R.T.: 8.780 min
Delta R.T.: -0.002 min
Response: 6887289
Conc: 5.02 ng/ml

#26 AR-1254-1

R.T.: 6.485 min
 Delta R.T.: 0.000 min
 Response: 2578085
 Conc: 46.70 ng/ml

Instrument: ECD_P
ClientSampleId: AR1254ICC050

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/08/2025
 Supervised By :mohammad ahmed 07/09/2025

#26 AR-1254-1





R.T.: 5.657 min
 Delta R.T.: 0.000 min
 Response: 6452648
 Conc: 57.45 ng/ml





#27 AR-1254-2

R.T.: 6.701 min
 Delta R.T.: 0.000 min
 Response: 4490008
 Conc: 54.40 ng/ml

#27 AR-1254-2

R.T.: 5.806 min
 Delta R.T.: 0.000 min
 Response: 5754555
 Conc: 59.89 ng/ml

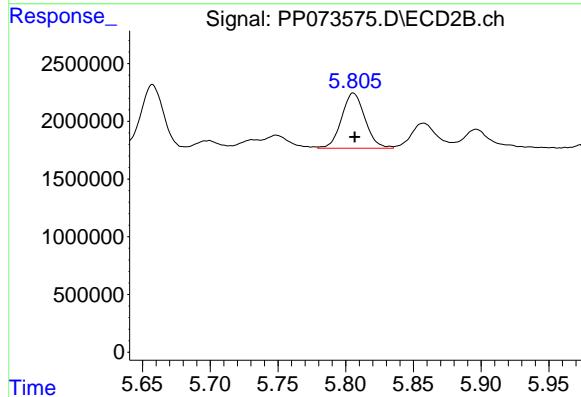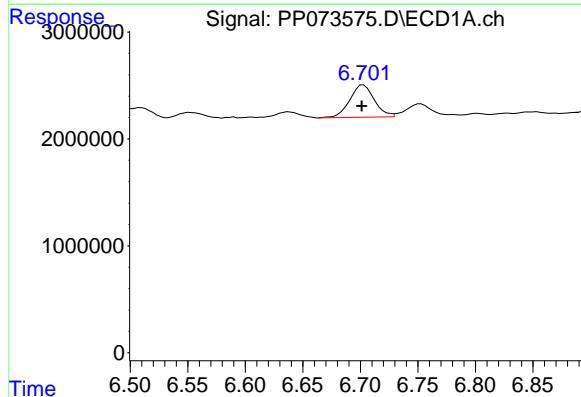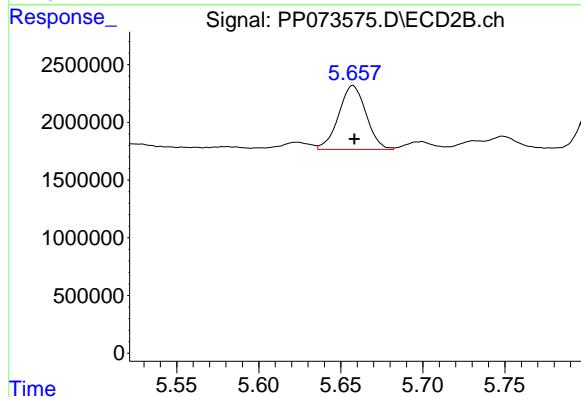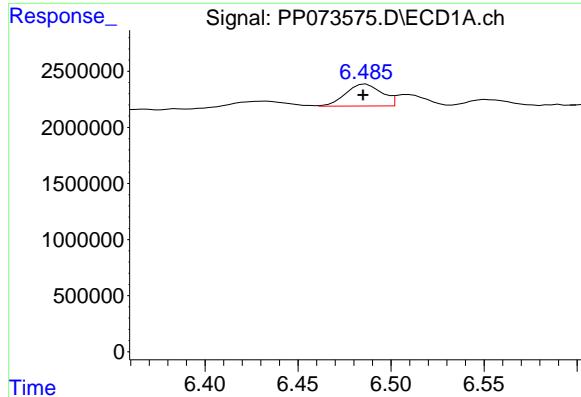

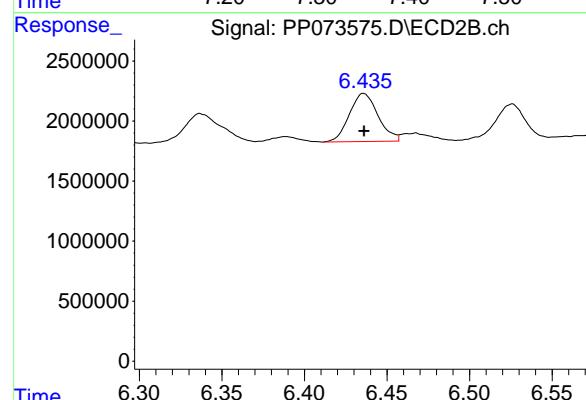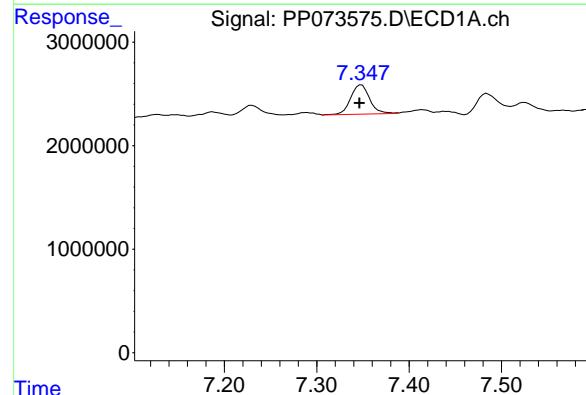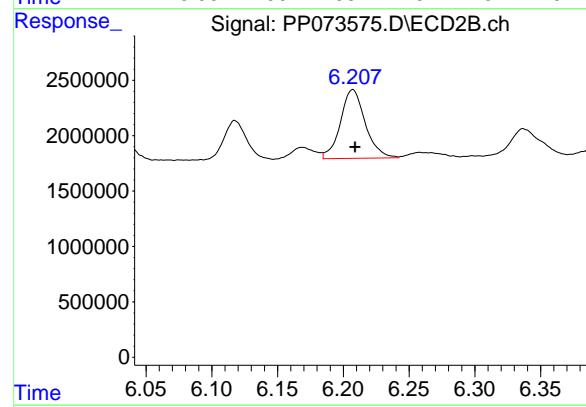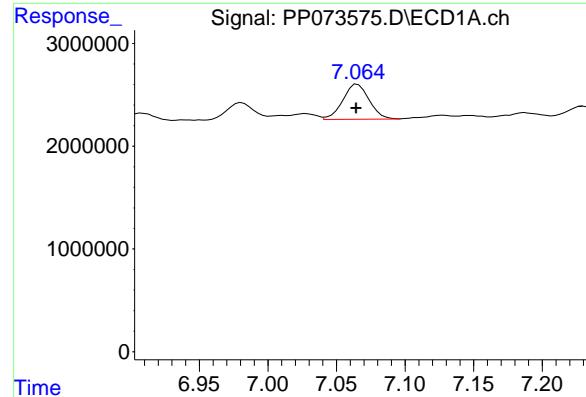




#28 AR-1254-3

R.T.: 7.064 min
 Delta R.T.: 0.000 min
 Response: 4570279
 Conc: 51.65 ng/ml

Instrument: ECD_P
ClientSampleId: AR1254ICC050

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/08/2025
 Supervised By :mohammad ahmed 07/09/2025

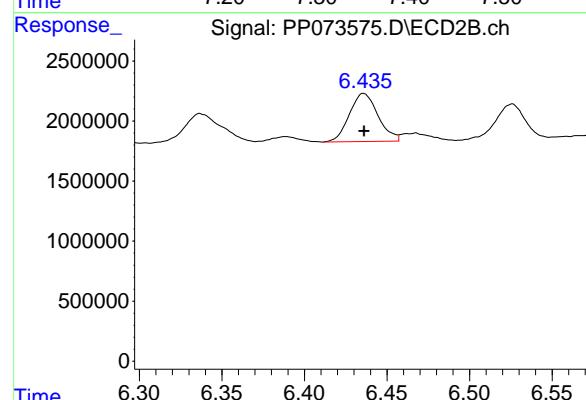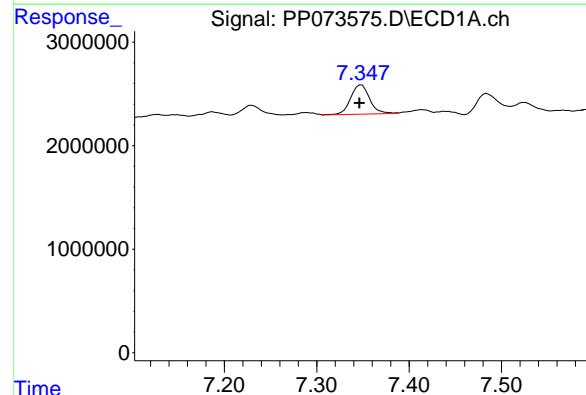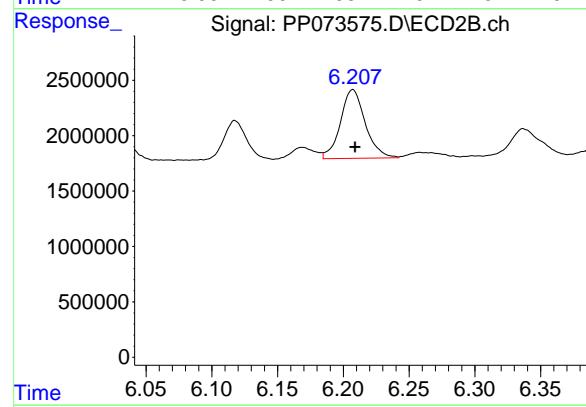

#28 AR-1254-3


R.T.: 6.207 min
 Delta R.T.: -0.002 min
 Response: 8163980
 Conc: 53.68 ng/ml

#29 AR-1254-4

R.T.: 7.347 min
 Delta R.T.: 0.001 min
 Response: 4061359
 Conc: 51.03 ng/ml

#29 AR-1254-4

R.T.: 6.436 min
 Delta R.T.: 0.000 min
 Response: 4857854
 Conc: 51.49 ng/ml

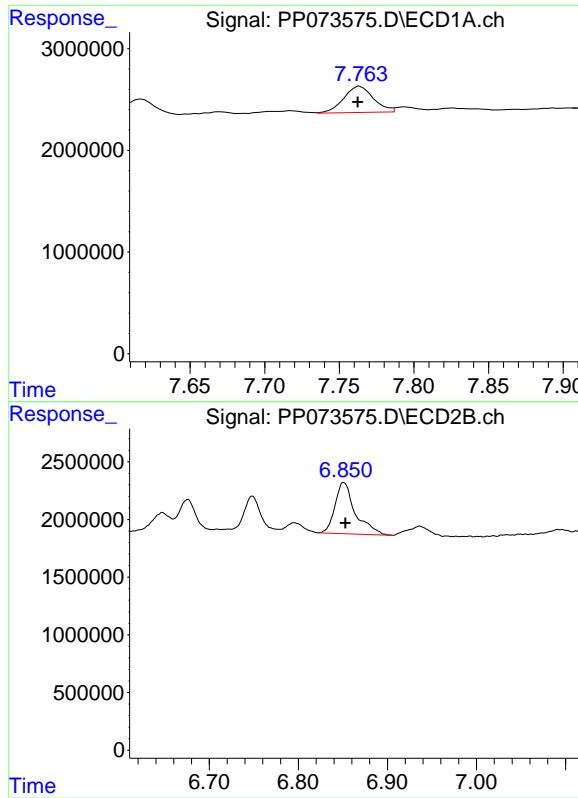

#30 AR-1254-5

R.T.: 7.764 min
 Delta R.T.: 0.002 min
 Response: 3548489
 Conc: 47.55 ng/ml

Instrument: ECD_P
 ClientSampleId: AR1254ICC050

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/08/2025
 Supervised By :mohammad ahmed 07/09/2025

1
2
3
4
5
6
7
8
9
10
11
12
13
14
15
16
17
18
19
20

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP070825\
 Data File : PP073576.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jul 2025 03:03
 Operator : YP\AJ
 Sample : AR1262ICC500
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
AR1262ICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 08 03:49:46 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 08 03:49:15 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	4.488	3.779	69434570	94417779	50.000	50.000
2) SA Decachlor...	10.177	8.781	57470872	69838496	50.000	50.000

Target Compounds

36) L8 AR-1262-1	8.065	6.889	43513643	73845842	500.000	500.000
37) L8 AR-1262-2	8.383	7.147	99013762	63914528	500.000	500.000
38) L8 AR-1262-3	8.697	7.669	62862521	57009497	500.000	500.000
39) L8 AR-1262-4	8.782	7.735	46631386	92024537	500.000	500.000
40) L8 AR-1262-5	9.432	8.231	31694688	42217822	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.



Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP070825\
 Data File : PP073576.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jul 2025 03:03
 Operator : YP\AJ
 Sample : AR1262ICC500
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
AR1262ICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 08 03:49:46 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 08 03:49:15 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ m Signal #2 Info : 30M x 0.32mm x 0.25 μ m

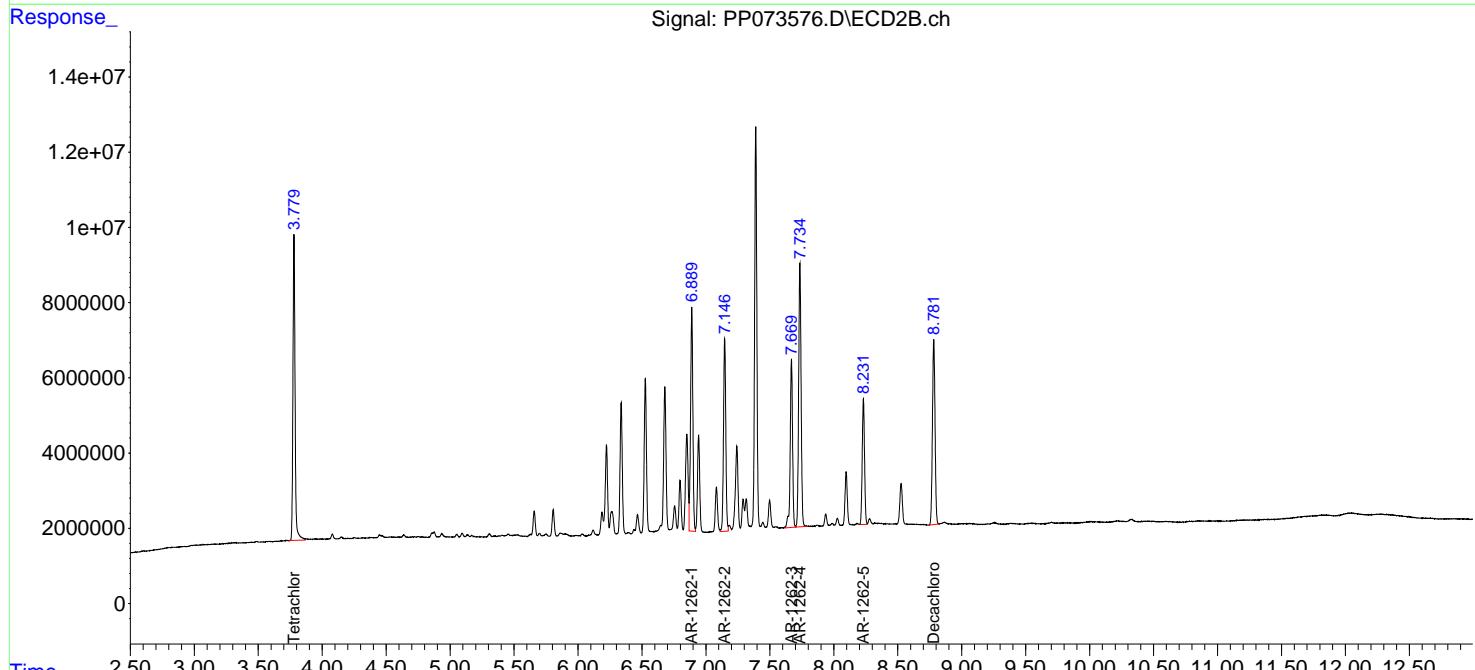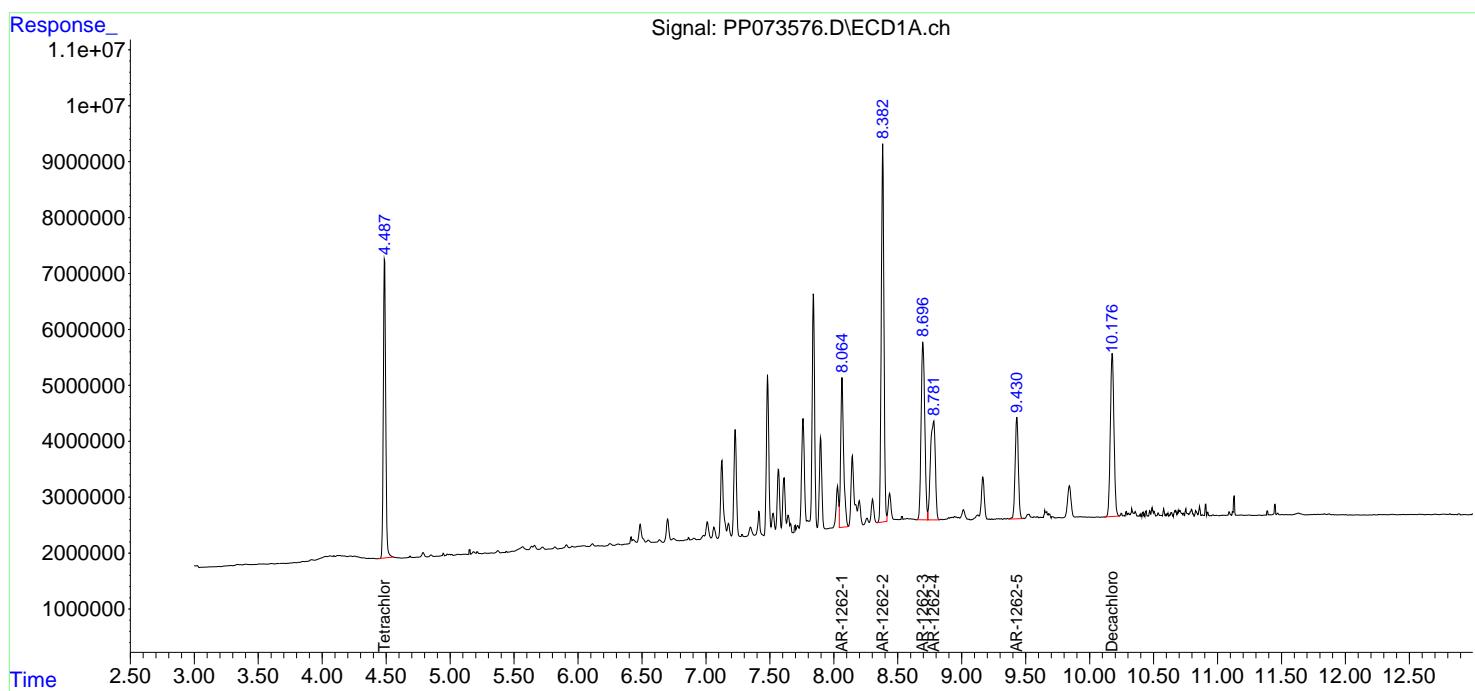

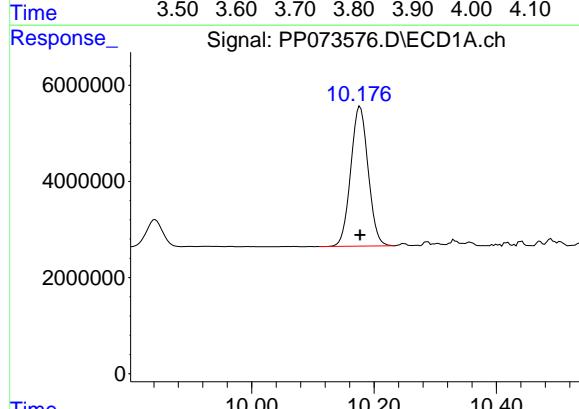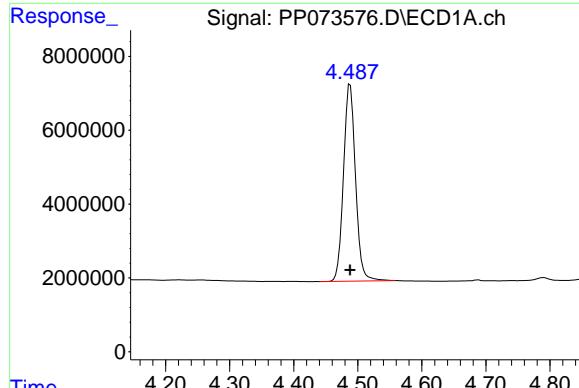

#1 Tetrachloro-m-xylene

R.T.: 4.488 min
Delta R.T.: 0.000 min
Response: 69434570
Conc: 50.00 ng/ml

Instrument:

ECD_P

ClientSampleId :
AR1262ICC500

#1 Tetrachloro-m-xylene

R.T.: 3.779 min
Delta R.T.: 0.000 min
Response: 94417779
Conc: 50.00 ng/ml

#2 Decachlorobiphenyl

R.T.: 10.177 min
Delta R.T.: 0.000 min
Response: 57470872
Conc: 50.00 ng/ml





#2 Decachlorobiphenyl

R.T.: 8.781 min
Delta R.T.: 0.000 min
Response: 69838496
Conc: 50.00 ng/ml

#36 AR-1262-1

R.T.: 8.065 min
 Delta R.T.: 0.000 min
 Response: 43513643
 Conc: 500.00 ng/ml

Instrument: ECD_P
ClientSampleId: AR1262ICC500

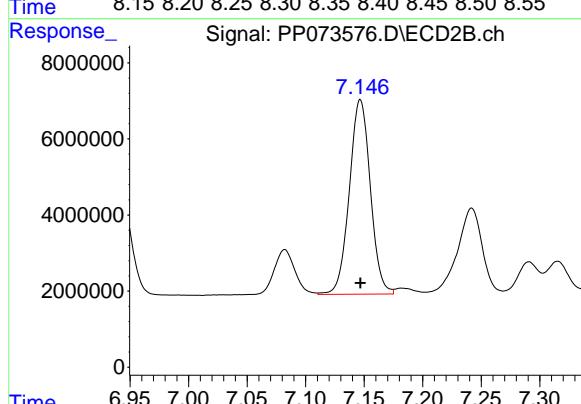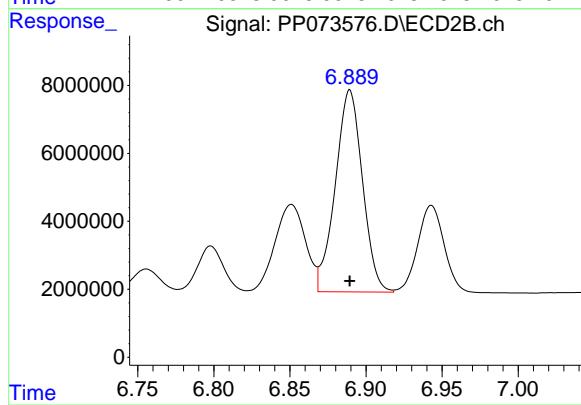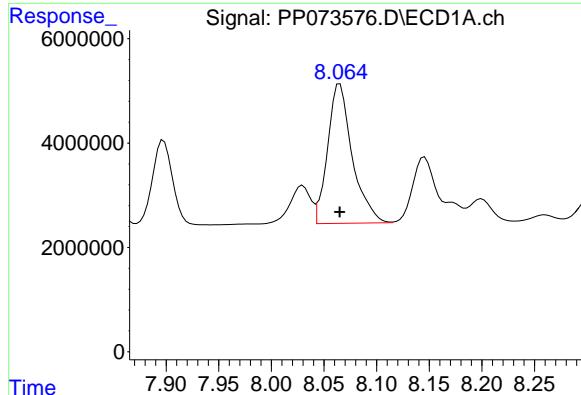

#36 AR-1262-1

R.T.: 6.889 min
 Delta R.T.: 0.000 min
 Response: 73845842
 Conc: 500.00 ng/ml

#37 AR-1262-2

R.T.: 8.383 min
 Delta R.T.: 0.000 min
 Response: 99013762
 Conc: 500.00 ng/ml





#37 AR-1262-2

R.T.: 7.147 min
 Delta R.T.: 0.000 min
 Response: 63914528
 Conc: 500.00 ng/ml

#38 AR-1262-3

R.T.: 8.697 min
 Delta R.T.: 0.000 min
 Response: 62862521
 Conc: 500.00 ng/ml

Instrument: ECD_P
ClientSampleId: AR1262ICC500

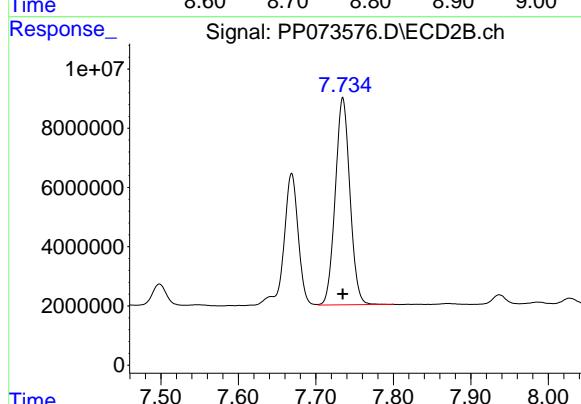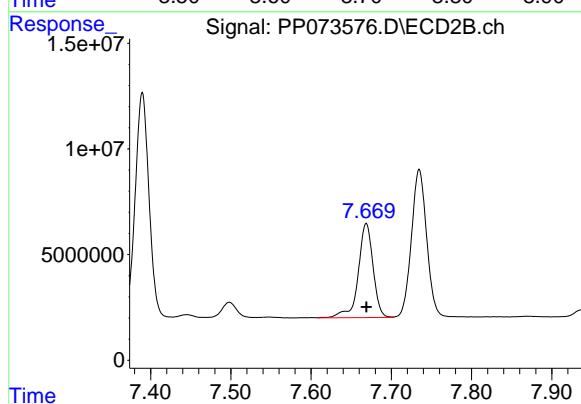

#38 AR-1262-3

R.T.: 7.669 min
 Delta R.T.: 0.000 min
 Response: 57009497
 Conc: 500.00 ng/ml

#39 AR-1262-4

R.T.: 8.782 min
 Delta R.T.: 0.000 min
 Response: 46631386
 Conc: 500.00 ng/ml



#39 AR-1262-4

R.T.: 7.735 min
 Delta R.T.: 0.000 min
 Response: 92024537
 Conc: 500.00 ng/ml

#40 AR-1262-5

R.T.: 9.432 min
Delta R.T.: 0.000 min
Response: 31694688
Conc: 500.00 ng/ml

Instrument: ECD_P
ClientSampleId: AR1262ICC500

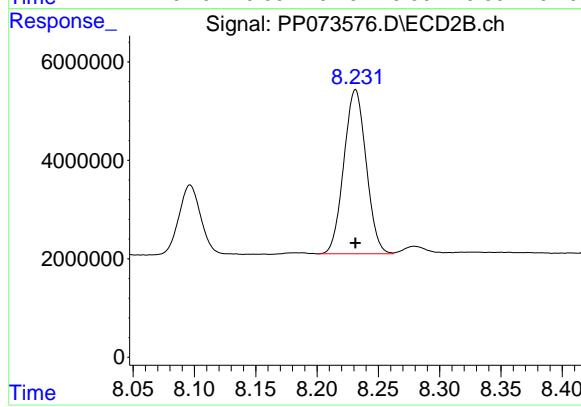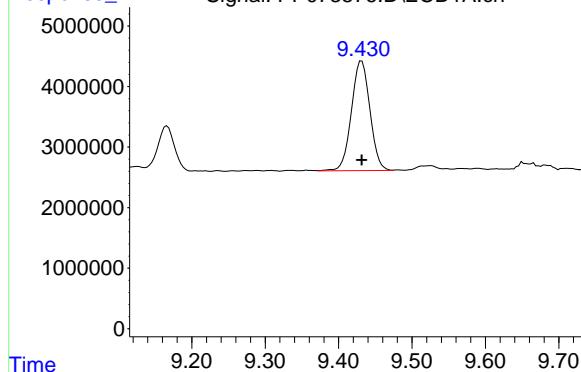

#40 AR-1262-5

R.T.: 8.231 min
Delta R.T.: 0.000 min
Response: 42217822
Conc: 500.00 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP070825\
 Data File : PP073577.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jul 2025 03:19
 Operator : YP\AJ
 Sample : AR1268ICC1000
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
AR1268ICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 08 04:41:25 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 08 04:40:39 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	4.487	3.780	135.2E6	186.6E6	95.477	96.310
2) SA Decachlor...	10.175	8.780	197.8E6	239.6E6	96.151	94.525

Target Compounds

41) L9 AR-1268-1	8.691	7.669	220.6E6	290.6E6	967.069	944.084
42) L9 AR-1268-2	8.784	7.736	188.8E6	254.1E6	971.974	949.819
43) L9 AR-1268-3	9.012	7.937	161.3E6	211.6E6	967.680	931.099
44) L9 AR-1268-4	9.428	8.231	68937885	89640321	991.083	941.420
45) L9 AR-1268-5	9.841	8.527	477.6E6	595.3E6	984.517	956.339



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP070825\
 Data File : PP073577.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jul 2025 03:19
 Operator : YP\AJ
 Sample : AR1268ICC1000
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
AR1268ICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 08 04:41:25 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 08 04:40:39 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ m Signal #2 Info : 30M x 0.32mm x 0.25 μ m

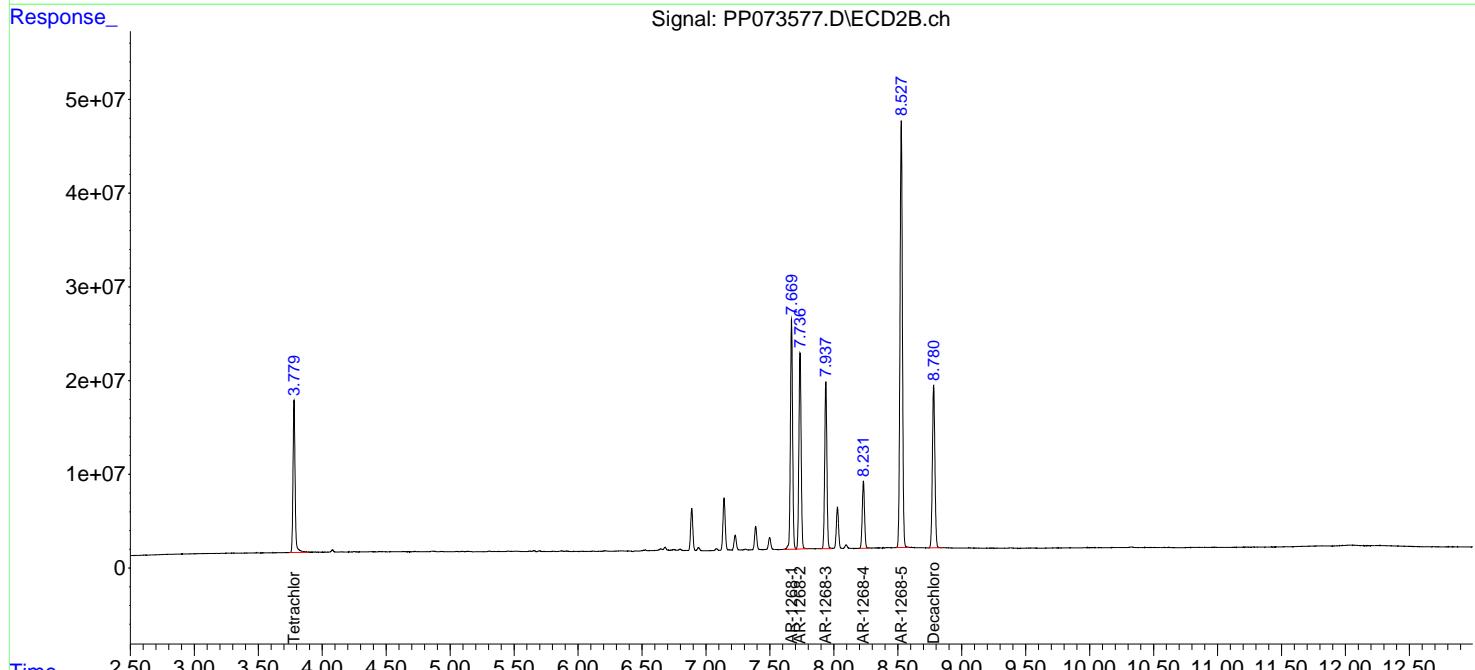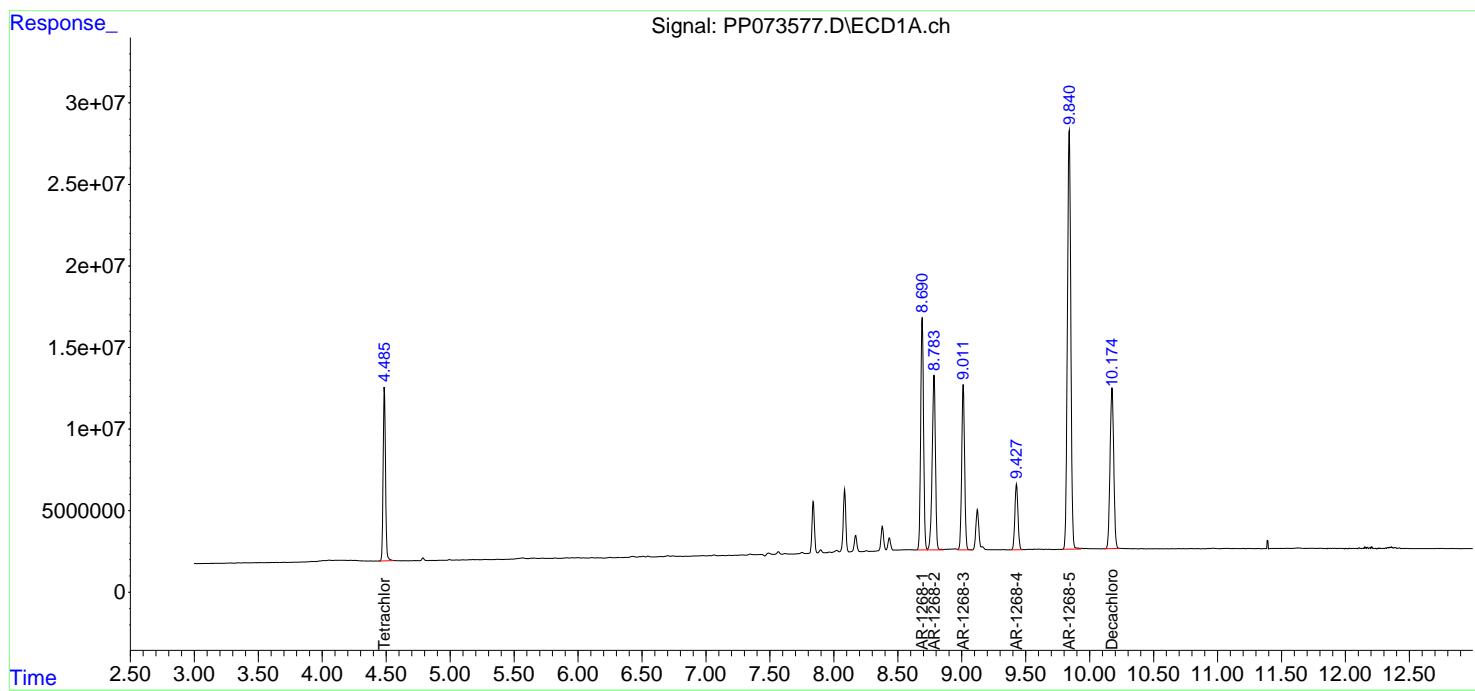

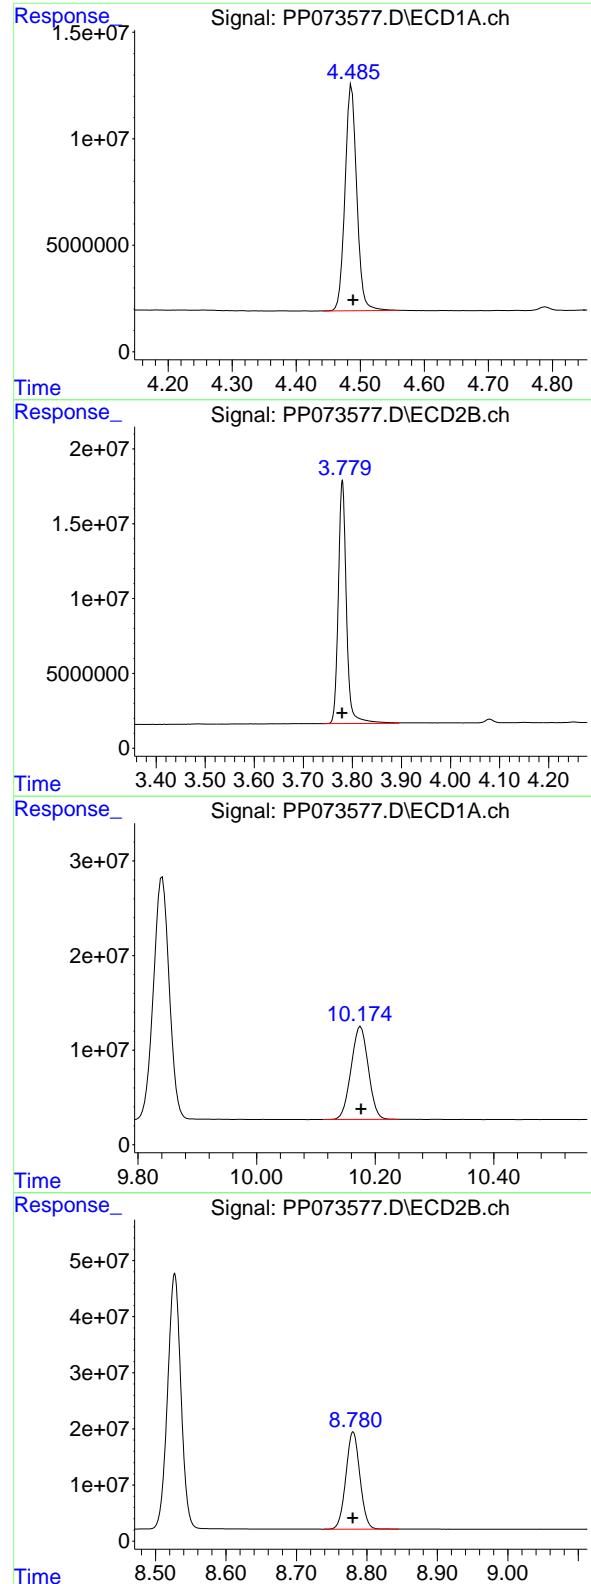

#1 Tetrachloro-m-xylene

R.T.: 4.487 min
 Delta R.T.: -0.002 min
 Response: 135177400
 Conc: 95.48 ng/ml

Instrument: ECD_P
ClientSampleId: AR1268ICC1000

#1 Tetrachloro-m-xylene

R.T.: 3.780 min
 Delta R.T.: 0.000 min
 Response: 186628635
 Conc: 96.31 ng/ml

#2 Decachlorobiphenyl

R.T.: 10.175 min
 Delta R.T.: -0.001 min
 Response: 197787493
 Conc: 96.15 ng/ml


#2 Decachlorobiphenyl

R.T.: 8.780 min
 Delta R.T.: 0.000 min
 Response: 239622927
 Conc: 94.53 ng/ml

#41 AR-1268-1


R.T.: 8.691 min
 Delta R.T.: -0.001 min
 Response: 220572869
 Conc: 967.07 ng/ml

Instrument: ECD_P
ClientSampleId: AR1268ICC1000




#41 AR-1268-1

R.T.: 7.669 min
 Delta R.T.: 0.000 min
 Response: 290584667
 Conc: 944.08 ng/ml

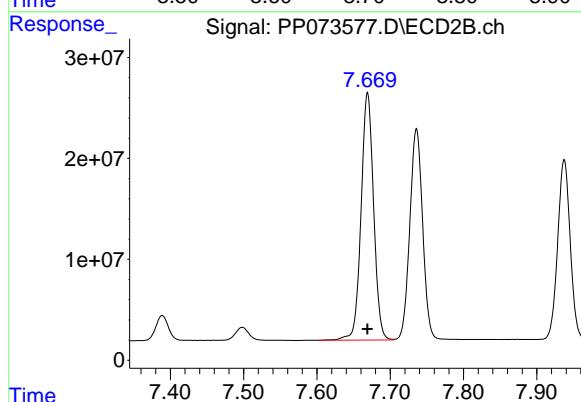


#42 AR-1268-2

R.T.: 8.784 min
 Delta R.T.: -0.002 min
 Response: 188785361
 Conc: 971.97 ng/ml

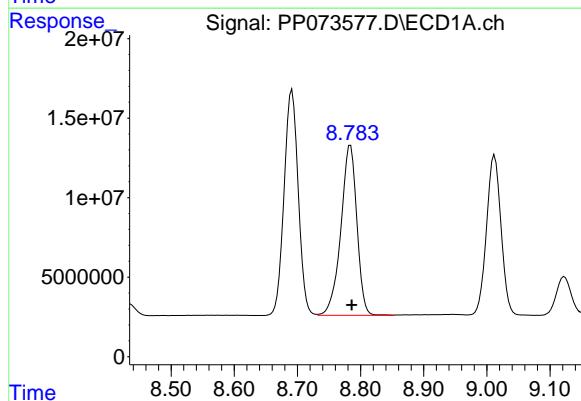

#42 AR-1268-2





R.T.: 7.736 min
 Delta R.T.: 0.000 min
 Response: 254148086
 Conc: 949.82 ng/ml

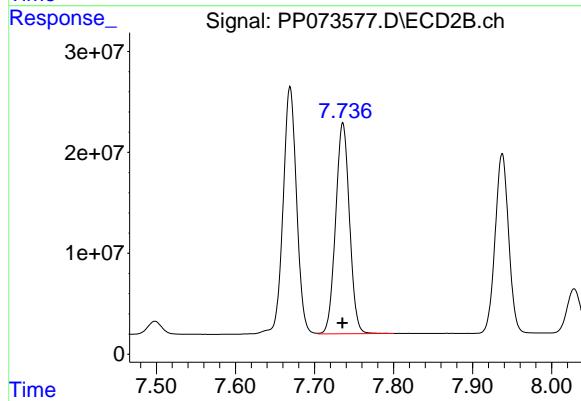

#43 AR-1268-3

R.T.: 9.012 min
 Delta R.T.: -0.002 min
 Response: 161320167
 Conc: 967.68 ng/ml

Instrument: ECD_P
ClientSampleId: AR1268ICC1000

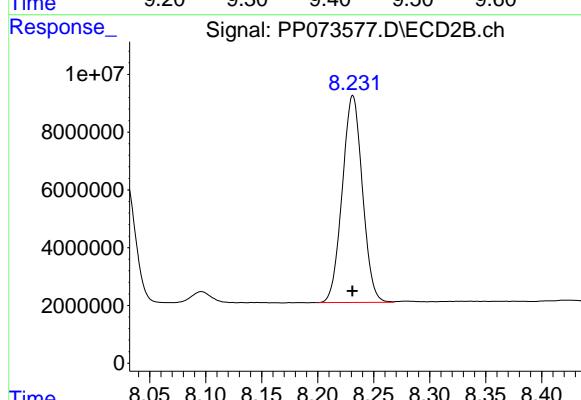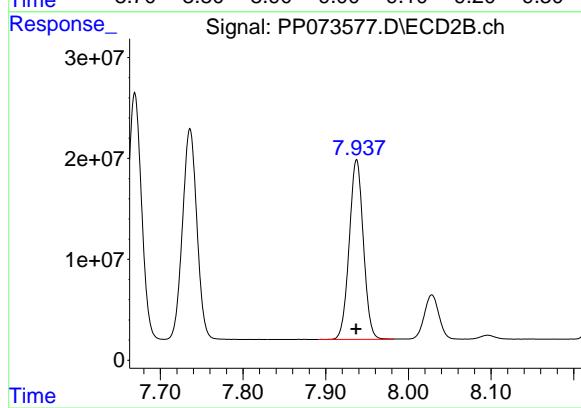

#43 AR-1268-3

R.T.: 7.937 min
 Delta R.T.: 0.000 min
 Response: 211648098
 Conc: 931.10 ng/ml

#44 AR-1268-4

R.T.: 9.428 min
 Delta R.T.: -0.002 min
 Response: 68937885
 Conc: 991.08 ng/ml



#44 AR-1268-4

R.T.: 8.231 min
 Delta R.T.: 0.000 min
 Response: 89640321
 Conc: 941.42 ng/ml

#45 AR-1268-5

R.T.: 9.841 min
Delta R.T.: 0.000 min
Response: 477643268
Conc: 984.52 ng/ml

Instrument: ECD_P
ClientSampleId: AR1268ICC1000

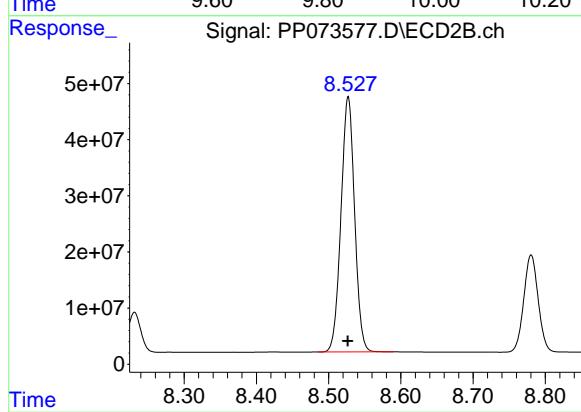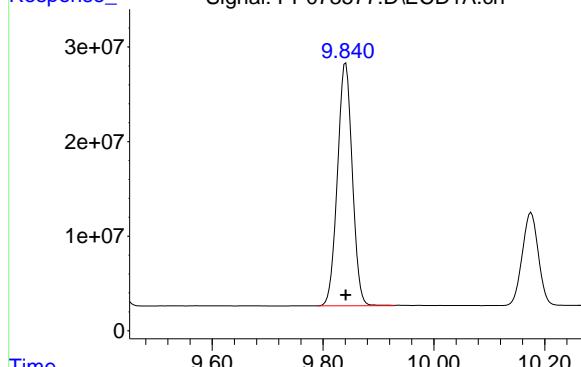

#45 AR-1268-5

R.T.: 8.527 min
Delta R.T.: 0.000 min
Response: 595257746
Conc: 956.34 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP070825\
 Data File : PP073578.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jul 2025 03:35
 Operator : YP\AJ
 Sample : AR1268ICC750
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
AR1268ICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 08 04:41:34 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 08 04:40:39 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	4.486	3.779	104.3E6	146.5E6	73.649	75.624
2) SA Decachlor...	10.176	8.780	151.6E6	191.8E6	73.695	75.646

Target Compounds

41) L9 AR-1268-1	8.691	7.668	168.8E6	230.7E6	740.295	749.493
42) L9 AR-1268-2	8.785	7.735	144.0E6	200.8E6	741.630	750.427
43) L9 AR-1268-3	9.013	7.936	123.3E6	169.4E6	739.524	745.141
44) L9 AR-1268-4	9.430	8.230	52353473	71323535	752.658	749.054
45) L9 AR-1268-5	9.841	8.526	354.6E6	478.2E6	730.874	768.335


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP070825\
 Data File : PP073578.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jul 2025 03:35
 Operator : YP\AJ
 Sample : AR1268ICC750
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
AR1268ICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 08 04:41:34 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 08 04:40:39 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

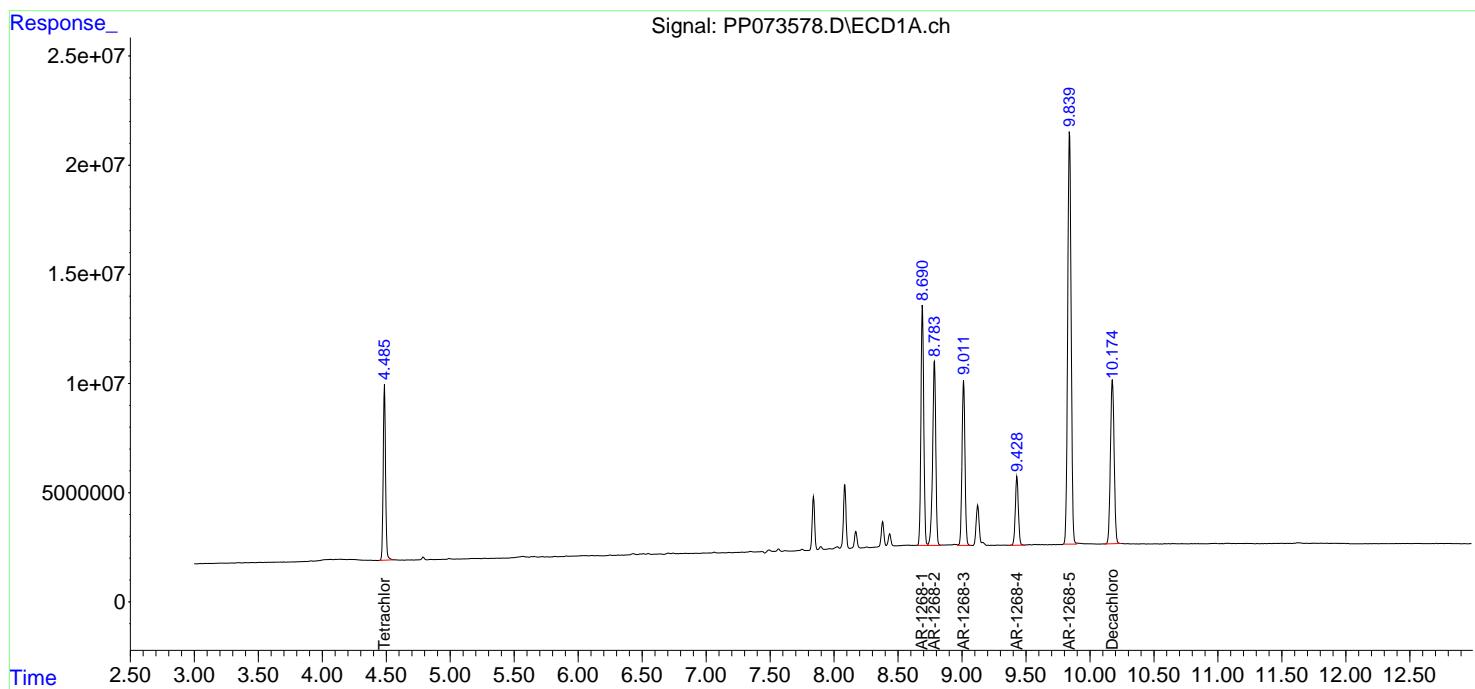

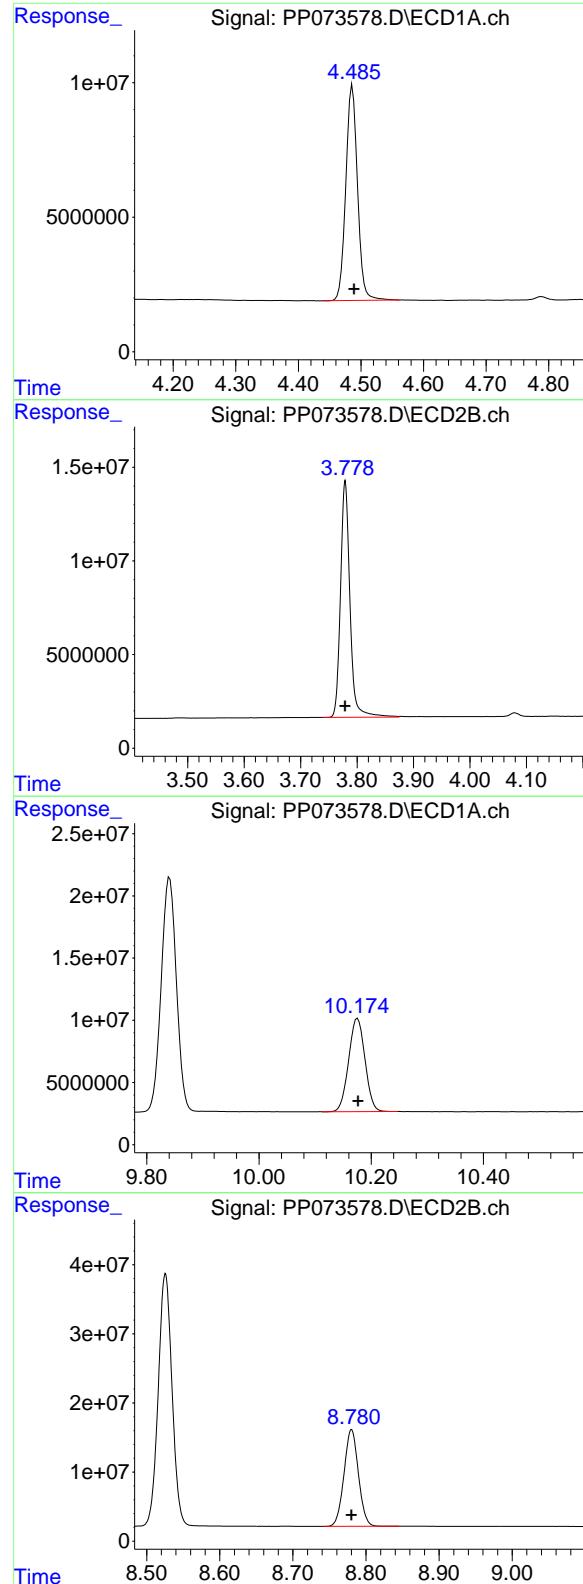

#1 Tetrachloro-m-xylene

R.T.: 4.486 min
 Delta R.T.: -0.003 min
 Response: 104273280
 Conc: 73.65 ng/ml

Instrument: ECD_P
ClientSampleId: AR1268ICC750

#1 Tetrachloro-m-xylene

R.T.: 3.779 min
 Delta R.T.: 0.000 min
 Response: 146543238
 Conc: 75.62 ng/ml

#2 Decachlorobiphenyl

R.T.: 10.176 min
 Delta R.T.: 0.000 min
 Response: 151594121
 Conc: 73.69 ng/ml


#2 Decachlorobiphenyl

R.T.: 8.780 min
 Delta R.T.: 0.000 min
 Response: 191764517
 Conc: 75.65 ng/ml

#41 AR-1268-1


R.T.: 8.691 min
 Delta R.T.: -0.002 min
 Response: 168849400
 Conc: 740.29 ng/ml

Instrument: ECD_P
ClientSampleId: AR1268ICC750




#41 AR-1268-1

R.T.: 7.668 min
 Delta R.T.: 0.000 min
 Response: 230690543
 Conc: 749.49 ng/ml

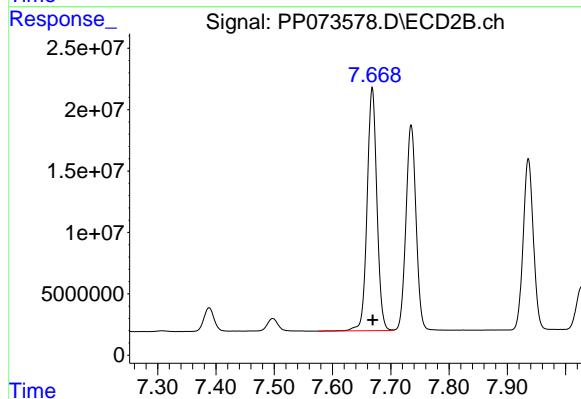


#42 AR-1268-2

R.T.: 8.785 min
 Delta R.T.: -0.001 min
 Response: 144045759
 Conc: 741.63 ng/ml

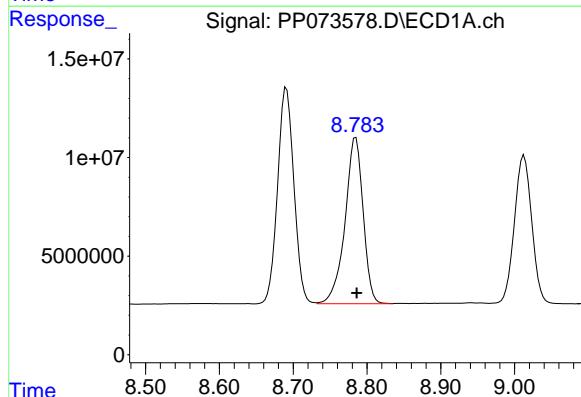

#42 AR-1268-2





R.T.: 7.735 min
 Delta R.T.: 0.000 min
 Response: 200795854
 Conc: 750.43 ng/ml

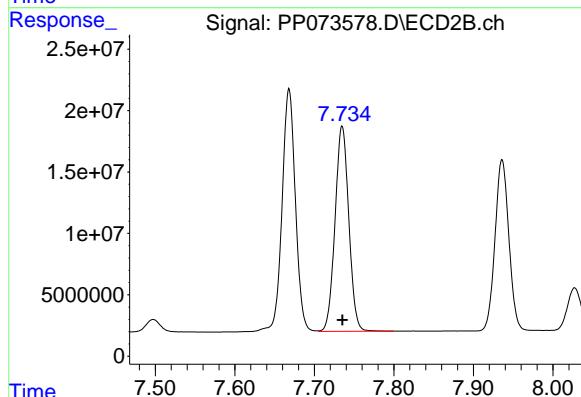

#43 AR-1268-3

R.T.: 9.013 min
 Delta R.T.: 0.000 min
 Response: 123284607
 Conc: 739.52 ng/ml

Instrument: ECD_P
ClientSampleId: AR1268ICC750

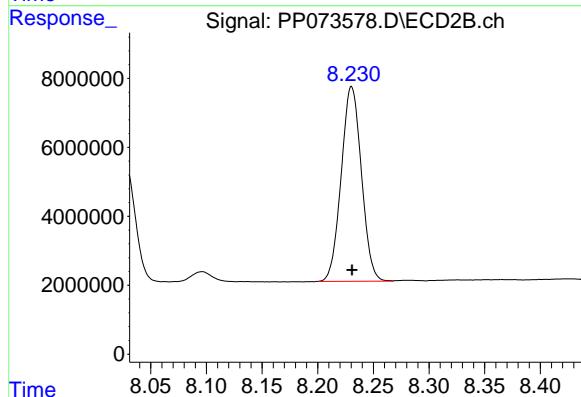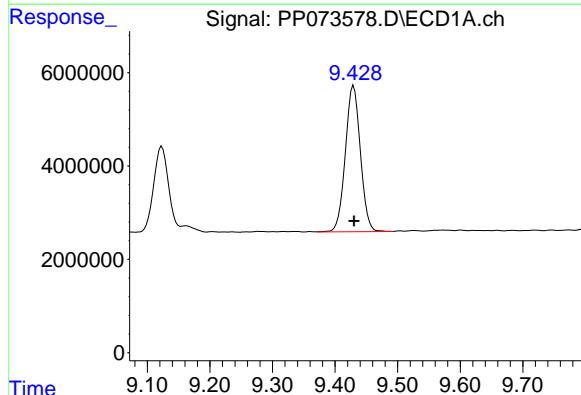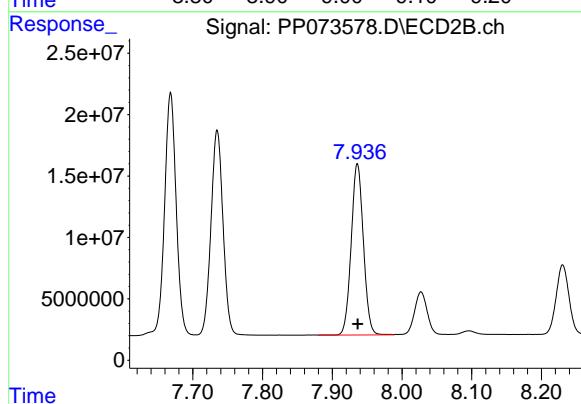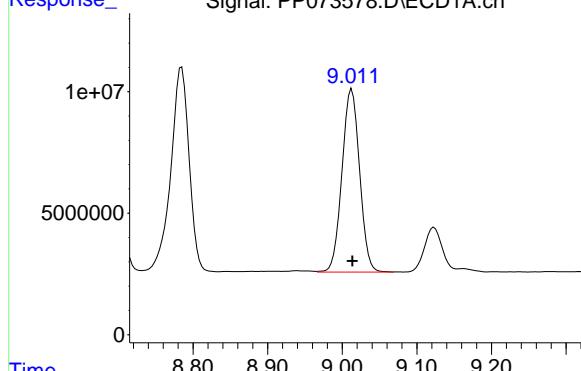

#43 AR-1268-3

R.T.: 7.936 min
 Delta R.T.: 0.000 min
 Response: 169377934
 Conc: 745.14 ng/ml

#44 AR-1268-4

R.T.: 9.430 min
 Delta R.T.: 0.000 min
 Response: 52353473
 Conc: 752.66 ng/ml



#44 AR-1268-4

R.T.: 8.230 min
 Delta R.T.: 0.000 min
 Response: 71323535
 Conc: 749.05 ng/ml

#45 AR-1268-5

R.T.: 9.841 min
Delta R.T.: 0.000 min
Response: 354587033
Conc: 730.87 ng/ml

Instrument: ECD_P
ClientSampleId: AR1268ICC750

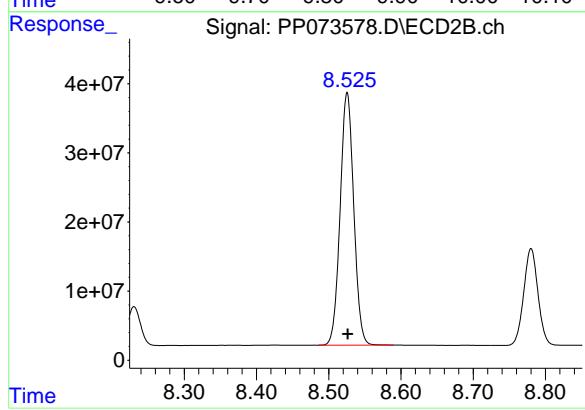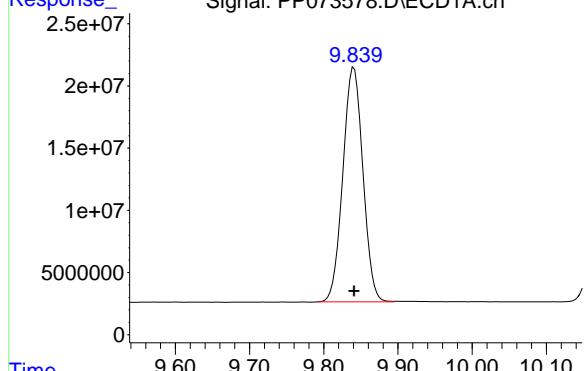

#45 AR-1268-5

R.T.: 8.526 min
Delta R.T.: 0.000 min
Response: 478238089
Conc: 768.34 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP070825\
 Data File : PP073579.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jul 2025 03:52
 Operator : YP\AJ
 Sample : AR1268ICC500
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
AR1268ICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 08 04:41:46 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 08 04:40:39 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	4.489	3.779	70790889	96889578	50.000	50.000
2) SA Decachlor...	10.177	8.780	102.9E6	126.8E6	50.000	50.000

Target Compounds

41) L9 AR-1268-1	8.693	7.669	114.0E6	153.9E6	500.000	500.000
42) L9 AR-1268-2	8.786	7.735	97114359	133.8E6	500.000	500.000
43) L9 AR-1268-3	9.014	7.937	83354053	113.7E6	500.000	500.000
44) L9 AR-1268-4	9.430	8.231	34779057	47609088	500.000	500.000
45) L9 AR-1268-5	9.841	8.527	242.6E6	311.2E6	500.000	500.000


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP070825\
 Data File : PP073579.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jul 2025 03:52
 Operator : YP\AJ
 Sample : AR1268ICC500
 Misc :
 ALS Vial : 28 Sample Multiplier: 1


Instrument :
ECD_P
ClientSampleId :
AR1268ICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 08 04:41:46 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 08 04:40:39 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

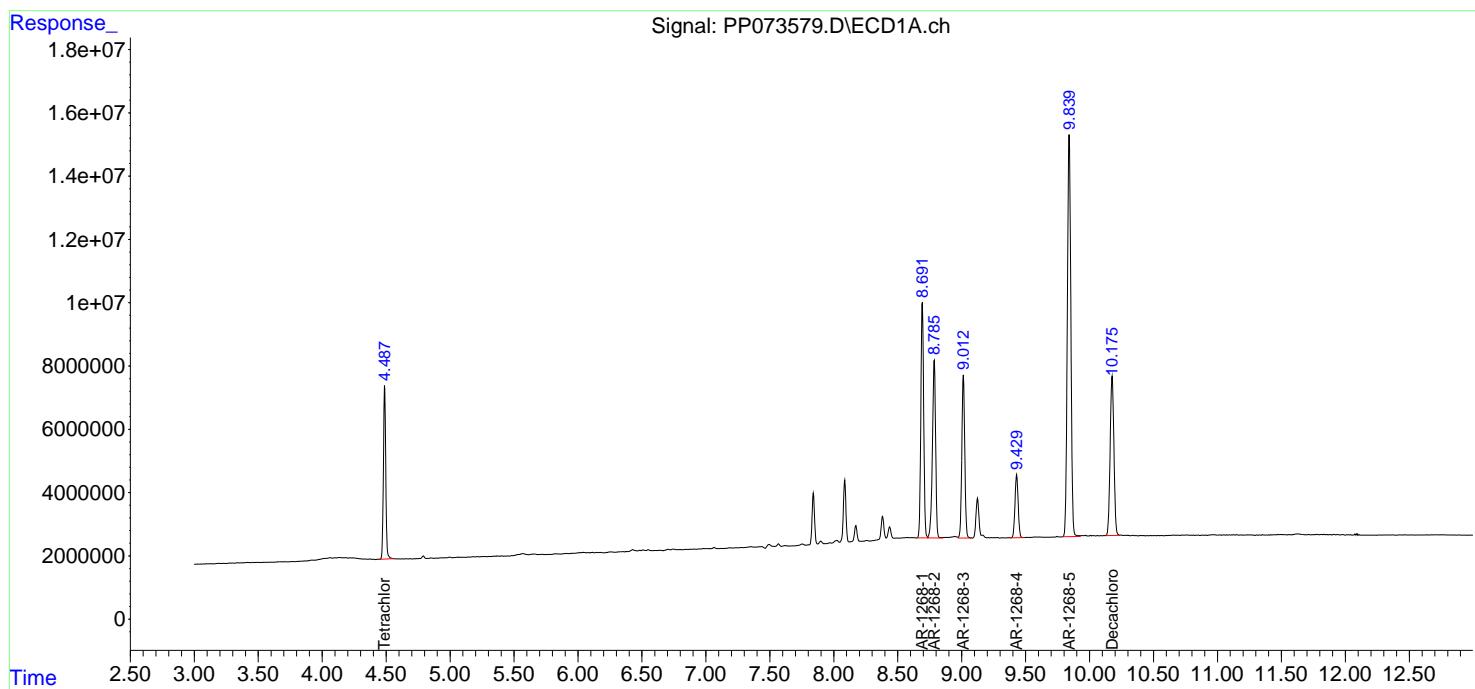

#1 Tetrachloro-m-xylene

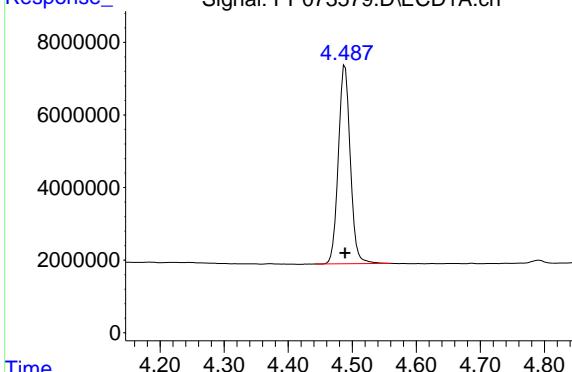

R.T.: 4.489 min
Delta R.T.: 0.000 min
Response: 70790889
Conc: 50.00 ng/ml

Instrument: ECD_P
ClientSampleId: AR1268ICC500

#1 Tetrachloro-m-xylene





R.T.: 3.779 min
Delta R.T.: 0.000 min
Response: 96889578
Conc: 50.00 ng/ml

#2 Decachlorobiphenyl

R.T.: 10.177 min
Delta R.T.: 0.000 min
Response: 102852384
Conc: 50.00 ng/ml

#2 Decachlorobiphenyl

R.T.: 8.780 min
Delta R.T.: 0.000 min
Response: 126750897
Conc: 50.00 ng/ml

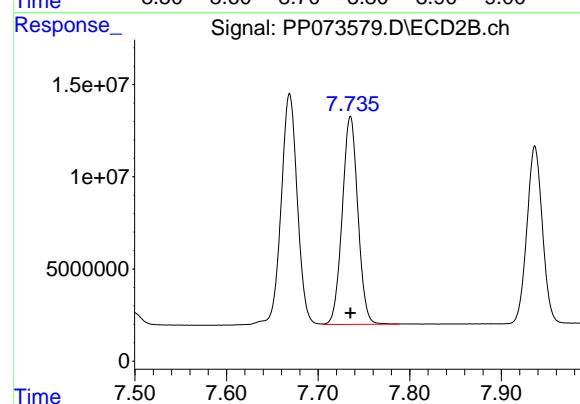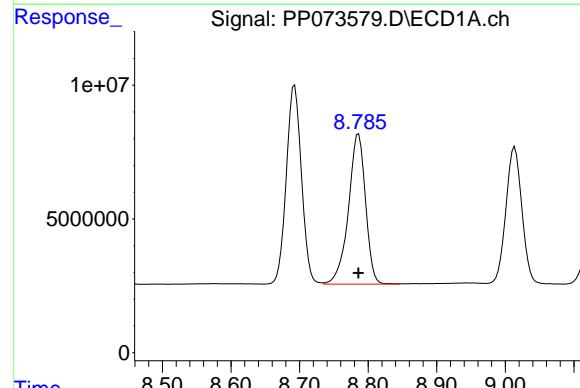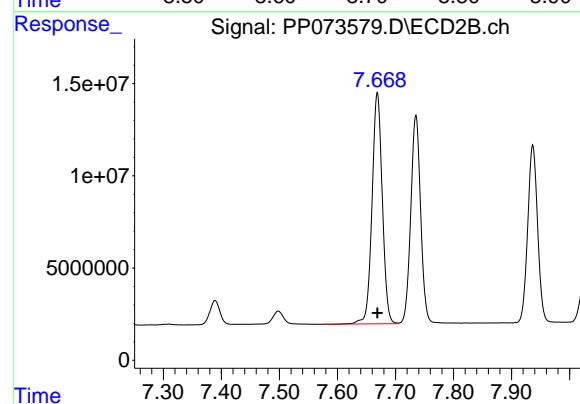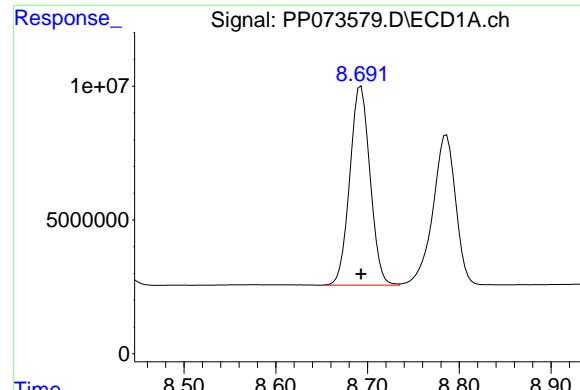

#41 AR-1268-1

R.T.: 8.693 min
Delta R.T.: 0.000 min
Response: 114041971
Conc: 500.00 ng/ml

Instrument: ECD_P
ClientSampleId: AR1268ICC500

#41 AR-1268-1

R.T.: 7.669 min
Delta R.T.: 0.000 min
Response: 153897638
Conc: 500.00 ng/ml

#42 AR-1268-2

R.T.: 8.786 min
Delta R.T.: 0.000 min
Response: 97114359
Conc: 500.00 ng/ml





#42 AR-1268-2

R.T.: 7.735 min
Delta R.T.: 0.000 min
Response: 133787705
Conc: 500.00 ng/ml

#43 AR-1268-3

R.T.: 9.014 min
 Delta R.T.: 0.000 min
 Response: 83354053
 Conc: 500.00 ng/ml

Instrument: ECD_P
ClientSampleId: AR1268ICC500

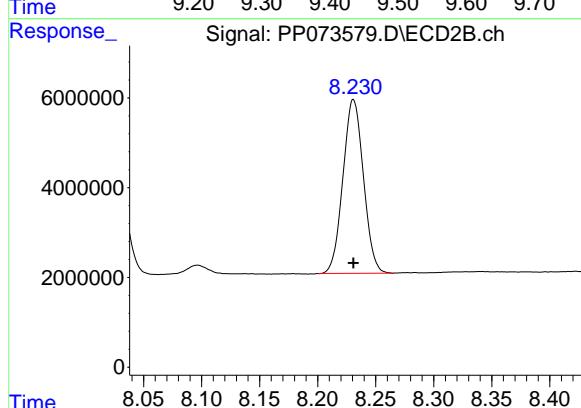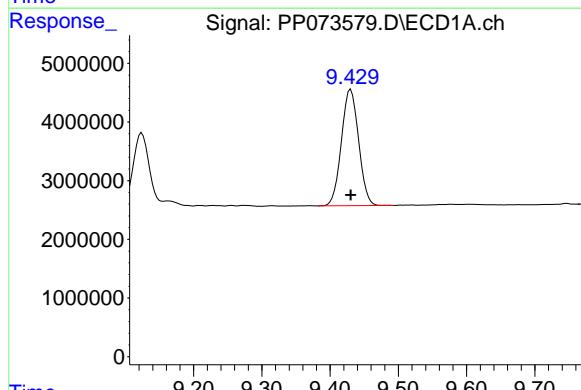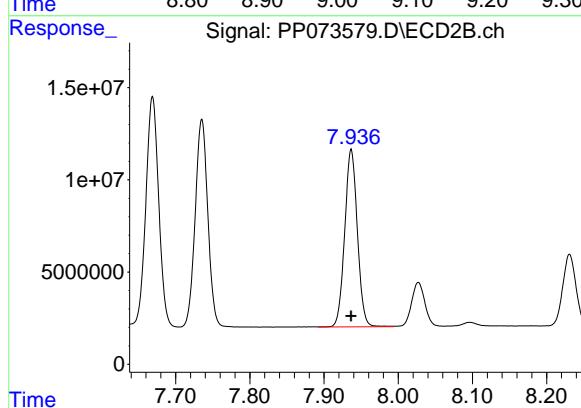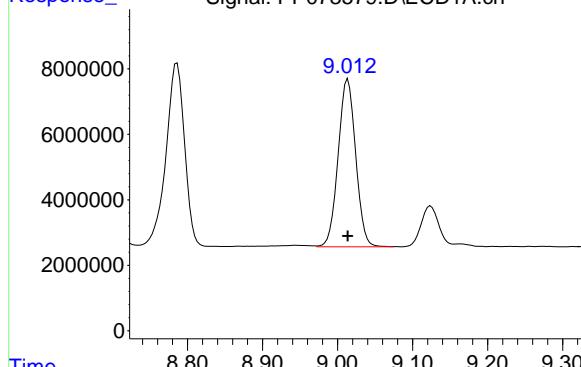

#43 AR-1268-3

R.T.: 7.937 min
 Delta R.T.: 0.000 min
 Response: 113654967
 Conc: 500.00 ng/ml

#44 AR-1268-4

R.T.: 9.430 min
 Delta R.T.: 0.000 min
 Response: 34779057
 Conc: 500.00 ng/ml



#44 AR-1268-4

R.T.: 8.231 min
 Delta R.T.: 0.000 min
 Response: 47609088
 Conc: 500.00 ng/ml

#45 AR-1268-5

R.T.: 9.841 min
Delta R.T.: 0.000 min
Response: 242577379
Conc: 500.00 ng/ml

Instrument: ECD_P
ClientSampleId: AR1268ICC500

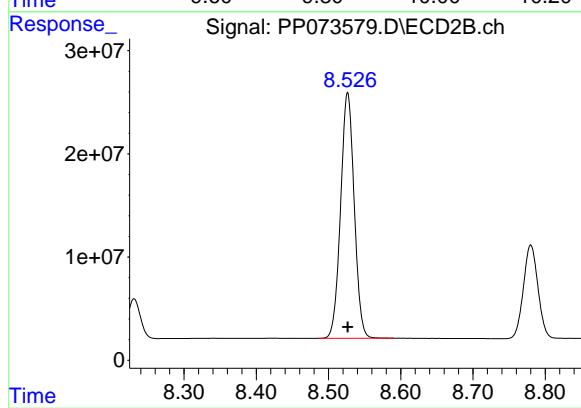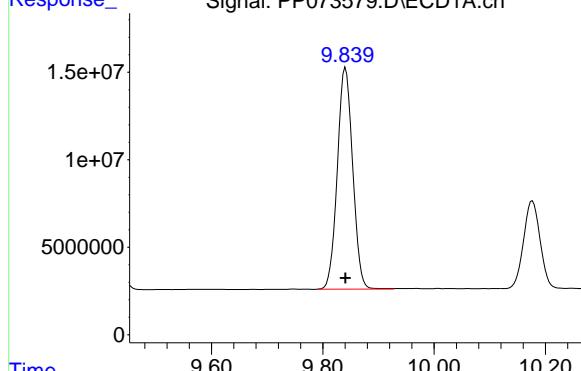

#45 AR-1268-5

R.T.: 8.527 min
Delta R.T.: 0.000 min
Response: 311217072
Conc: 500.00 ng/ml

1
2
3
4
5
6
7
8
9
10
11
12
13
14
15
16
17
18
19
20

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP070825\
 Data File : PP073580.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jul 2025 04:08
 Operator : YP\AJ
 Sample : AR1268ICC250
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
AR1268ICC250

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/08/2025
 Supervised By :mohammad ahmed 07/09/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 08 04:41:57 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 08 04:40:39 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	4.485	3.779	37383725	50542988	26.404	26.083
2) SA Decachlor...	10.171	8.781	54731552	67087696	26.607	26.464

Target Compounds

41) L9 AR-1268-1	8.690	7.668	59422367	80900824	260.528	262.840m
42) L9 AR-1268-2	8.783	7.735	50730840	70740492	261.191	264.376
43) L9 AR-1268-3	9.010	7.936	43805027	60554343	262.765	266.395
44) L9 AR-1268-4	9.428	8.231	18771767	24970476	269.872	262.245
45) L9 AR-1268-5	9.839	8.525	124.3E6	162.7E6	256.278	261.384

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP070825\
 Data File : PP073580.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jul 2025 04:08
 Operator : YP\AJ
 Sample : AR1268ICC250
 Misc :
 ALS Vial : 29 Sample Multiplier: 1



Instrument :
 ECD_P
 ClientSampleId :
 AR1268ICC250


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/08/2025
 Supervised By :mohammad ahmed 07/09/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 08 04:41:57 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 08 04:40:39 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

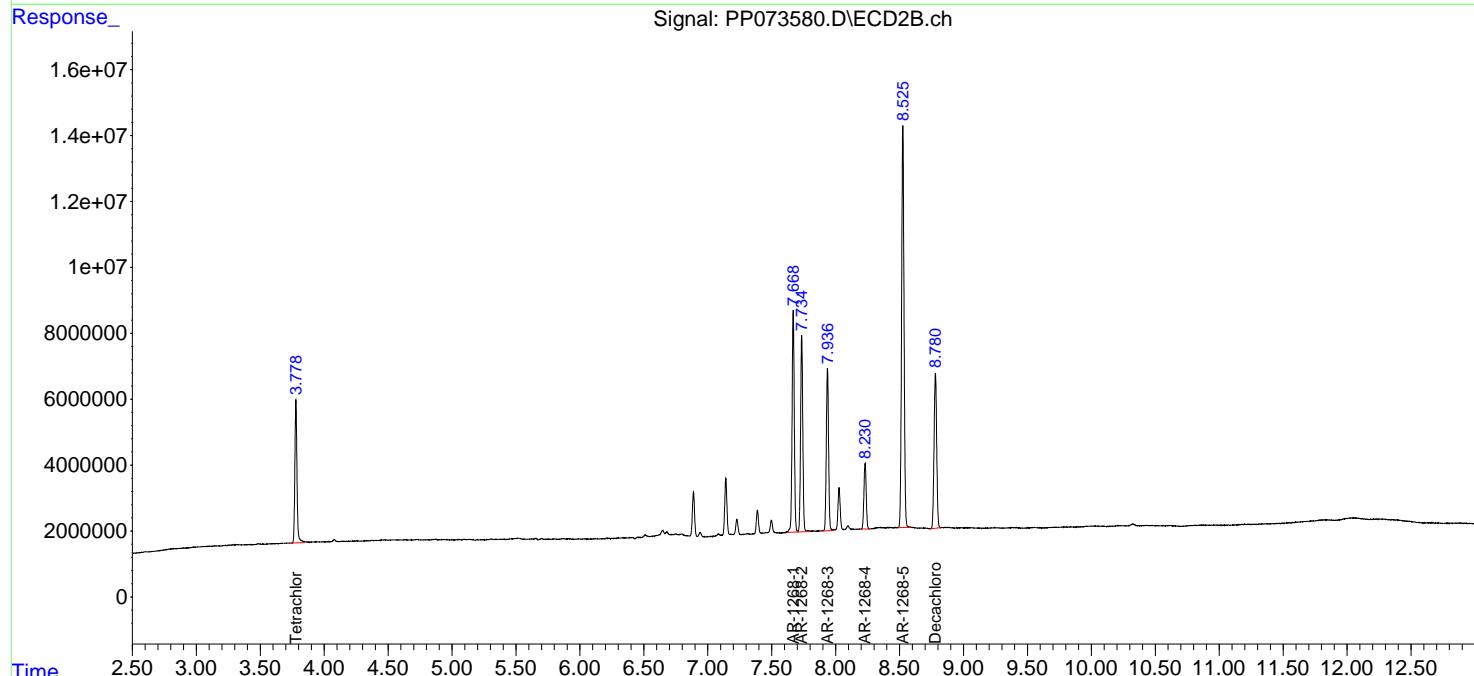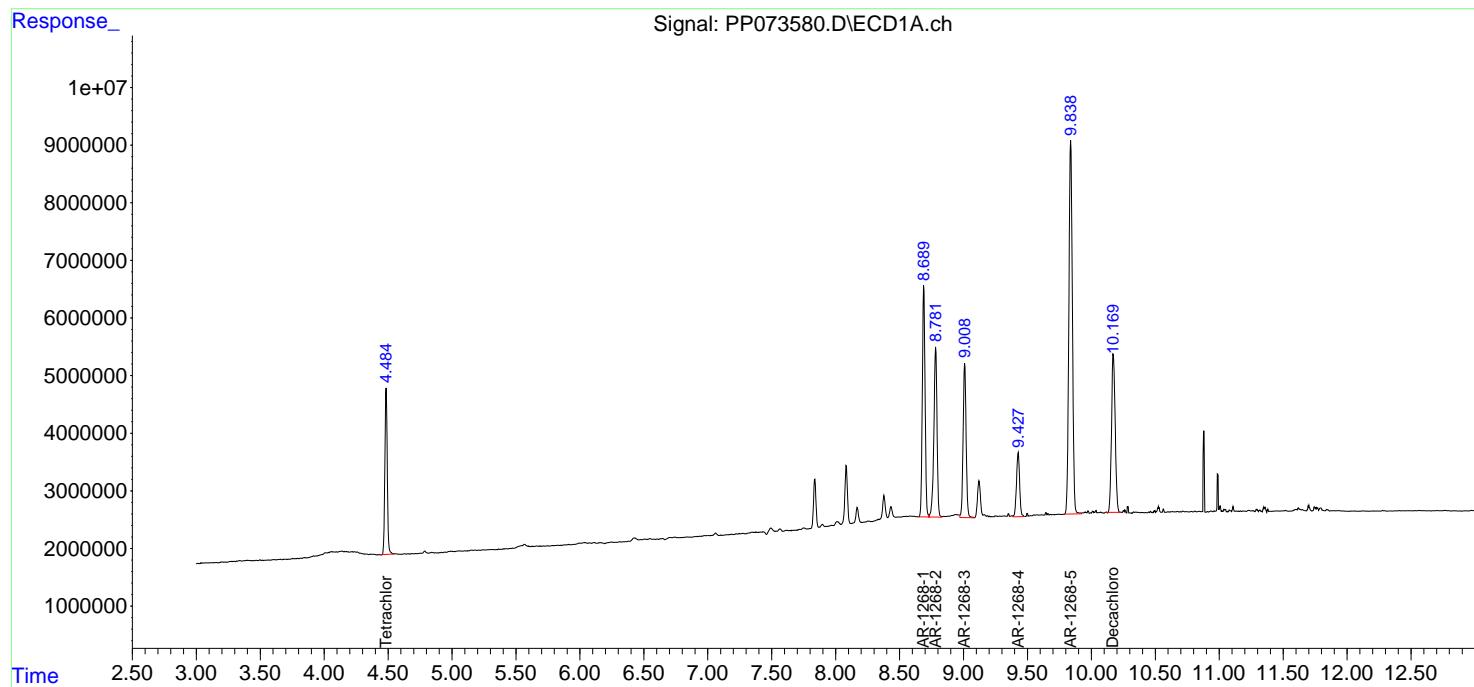

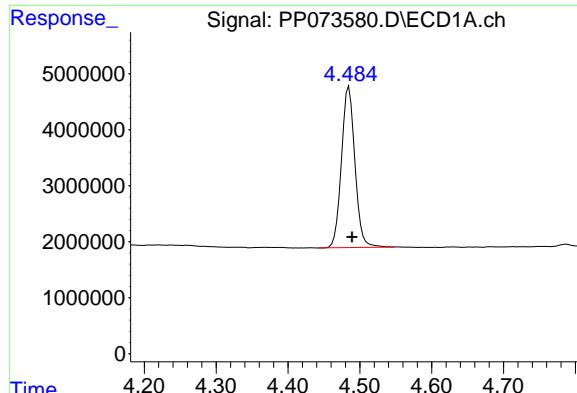


#1 Tetrachloro-m-xylene

R.T.: 4.485 min
Delta R.T.: -0.004 min
Response: 37383725
Conc: 26.40 ng/ml

Instrument: ECD_P
ClientSampleId: AR1268ICC250


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/08/2025
Supervised By :mohammad ahmed 07/09/2025

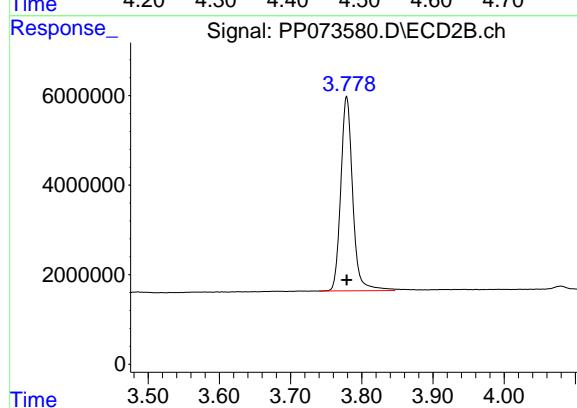


#1 Tetrachloro-m-xylene

R.T.: 3.779 min
Delta R.T.: 0.000 min
Response: 50542988
Conc: 26.08 ng/ml







#2 Decachlorobiphenyl

R.T.: 10.171 min
Delta R.T.: -0.005 min
Response: 54731552
Conc: 26.61 ng/ml

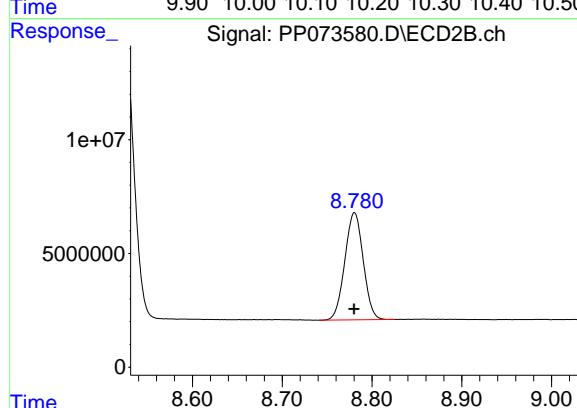

#2 Decachlorobiphenyl

R.T.: 8.781 min
Delta R.T.: 0.000 min
Response: 67087696
Conc: 26.46 ng/ml

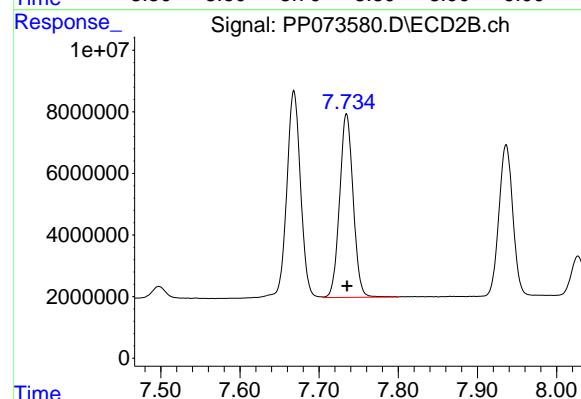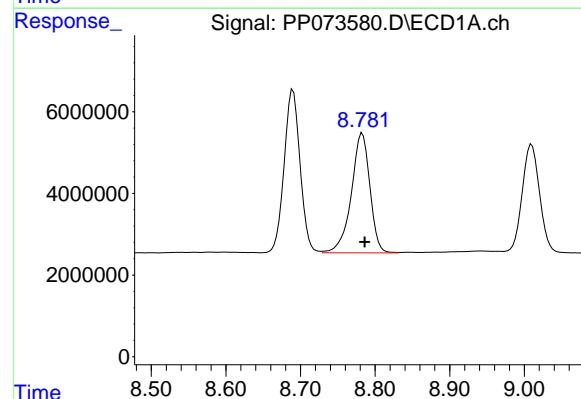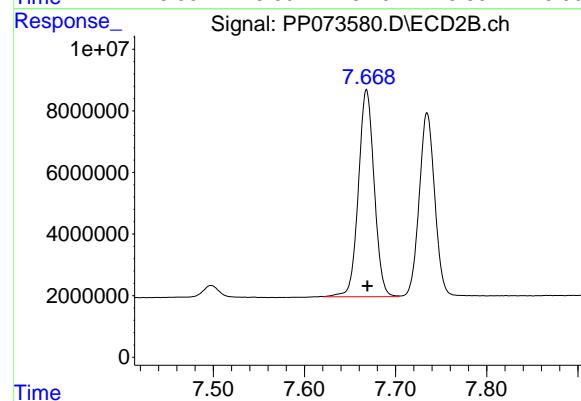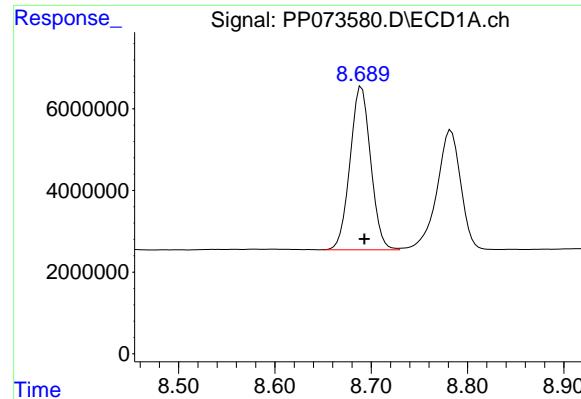

#41 AR-1268-1

R.T.: 8.690 min
 Delta R.T.: -0.003 min
 Response: 59422367
 Conc: 260.53 ng/ml

Instrument: ECD_P
ClientSampleId: AR1268ICC250

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/08/2025
 Supervised By :mohammad ahmed 07/09/2025

#41 AR-1268-1

R.T.: 7.668 min
 Delta R.T.: -0.001 min
 Response: 80900824
 Conc: 262.84 ng/ml

#42 AR-1268-2

R.T.: 8.783 min
 Delta R.T.: -0.003 min
 Response: 50730840
 Conc: 261.19 ng/ml

#42 AR-1268-2

R.T.: 7.735 min
 Delta R.T.: 0.000 min
 Response: 70740492
 Conc: 264.38 ng/ml

#43 AR-1268-3

R.T.: 9.010 min
 Delta R.T.: -0.004 min
 Response: 43805027
 Conc: 262.76 ng/ml

Instrument: ECD_P
ClientSampleId: AR1268ICC250

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/08/2025
 Supervised By :mohammad ahmed 07/09/2025

#43 AR-1268-3





R.T.: 7.936 min
 Delta R.T.: 0.000 min
 Response: 60554343
 Conc: 266.40 ng/ml

#44 AR-1268-4


R.T.: 9.428 min
 Delta R.T.: -0.002 min
 Response: 18771767
 Conc: 269.87 ng/ml

#44 AR-1268-4

R.T.: 8.231 min
 Delta R.T.: 0.000 min
 Response: 24970476
 Conc: 262.24 ng/ml

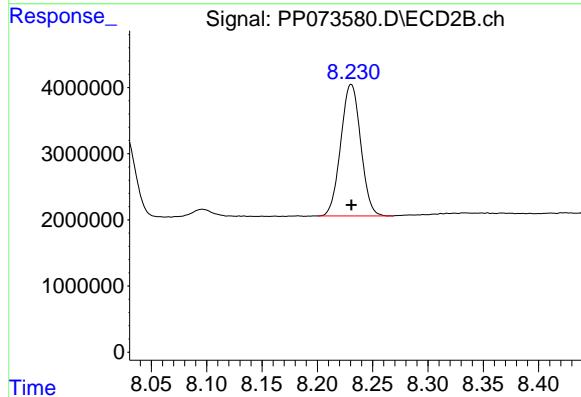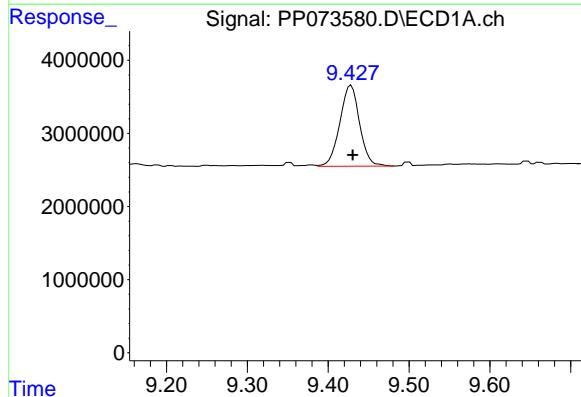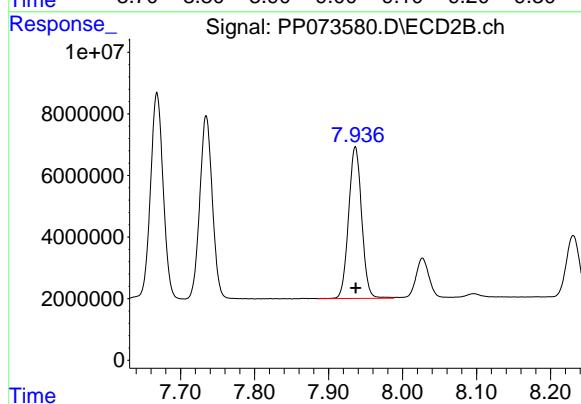

#45 AR-1268-5

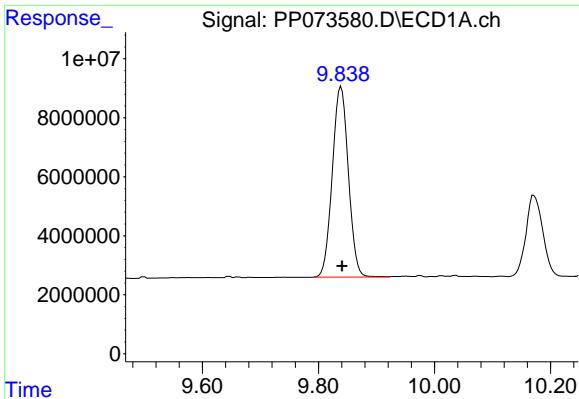

R.T.: 9.839 min
Delta R.T.: -0.002 min
Response: 124334254
Conc: 256.28 ng/ml

Instrument: ECD_P
ClientSampleId: AR1268ICC250

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/08/2025
Supervised By :mohammad ahmed 07/09/2025

#45 AR-1268-5

R.T.: 8.525 min
Delta R.T.: -0.001 min
Response: 162694547
Conc: 261.38 ng/ml

5

6

7

8

9

10

11

12

13

14

15

16

17

18

19

20

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP070825\
 Data File : PP073581.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jul 2025 04:24
 Operator : YP\AJ
 Sample : AR1268ICC050
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
AR1268ICC050

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/08/2025
 Supervised By :mohammad ahmed 07/09/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 08 04:52:34 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 08 04:46:40 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	4.489	3.778	6570480	8954068	4.649	4.604
2) SA Decachlor...	10.178	8.780	8974224	11778445	4.354	4.632

Target Compounds

41) L9 AR-1268-1	8.694	7.668	10231981	15365679	44.903	49.987
42) L9 AR-1268-2	8.787	7.735	8726381	12801300	44.866	47.748
43) L9 AR-1268-3	9.015	7.936	8012537	11044482	48.006	48.707
44) L9 AR-1268-4	9.433	8.231	3216586	4250036	45.402	44.756
45) L9 AR-1268-5	9.839	8.526	18594477	28831591	38.480m	46.018

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP070825\
 Data File : PP073581.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jul 2025 04:24
 Operator : YP\AJ
 Sample : AR1268ICC050
 Misc :
 ALS Vial : 30 Sample Multiplier: 1



Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 08 04:52:34 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 08 04:46:40 2025
 Response via : Initial Calibration
 Integrator: ChemStation





Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Instrument :
 ECD_P
ClientSampleId :
 AR1268ICC050

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/08/2025
 Supervised By :mohammad ahmed 07/09/2025

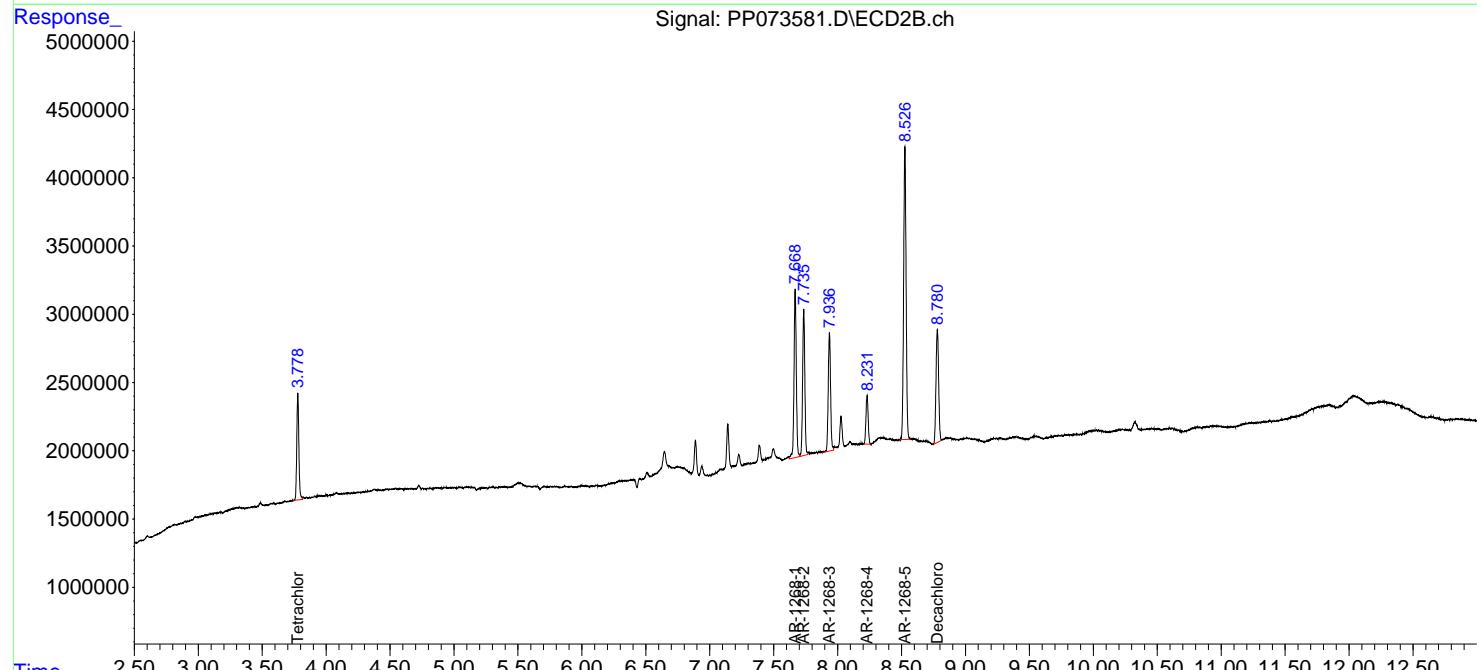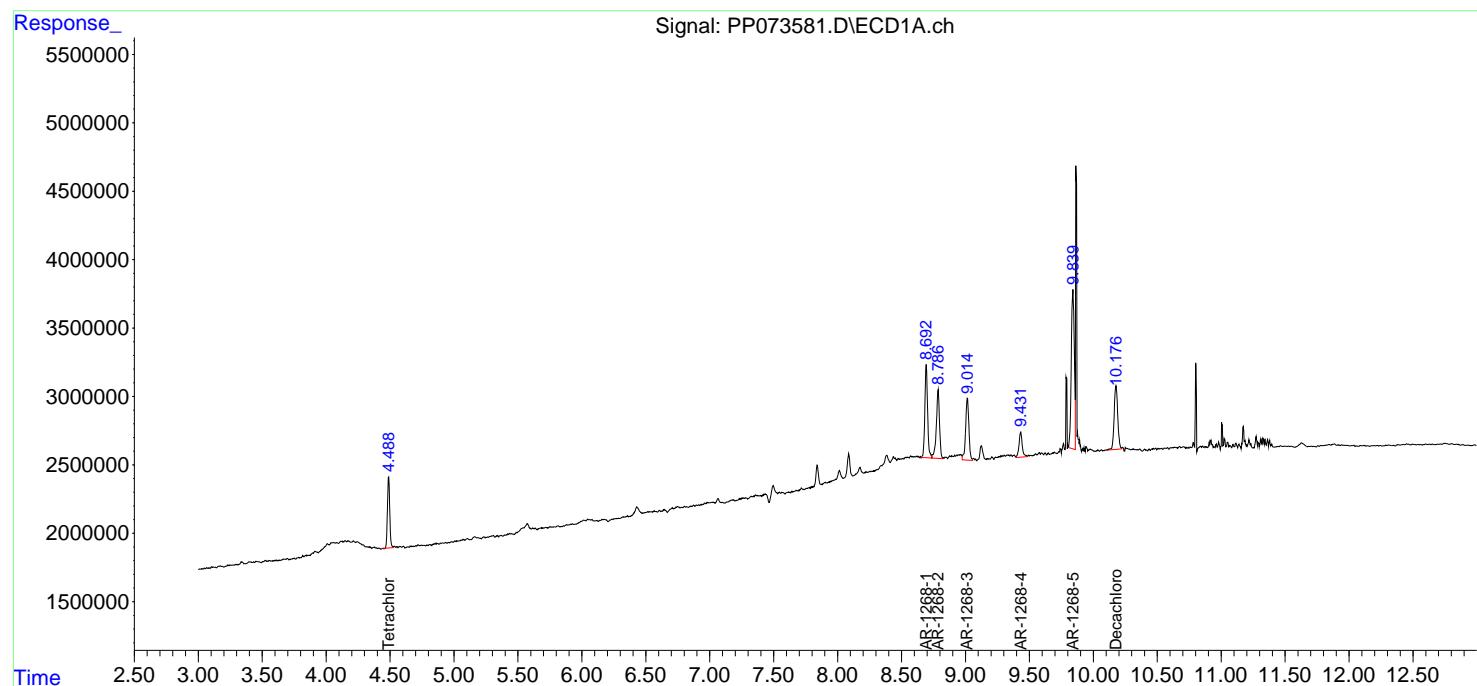

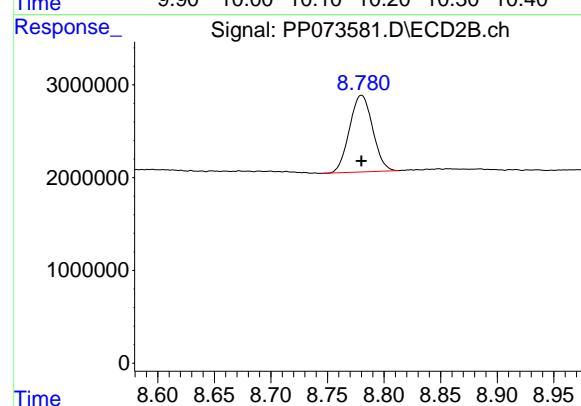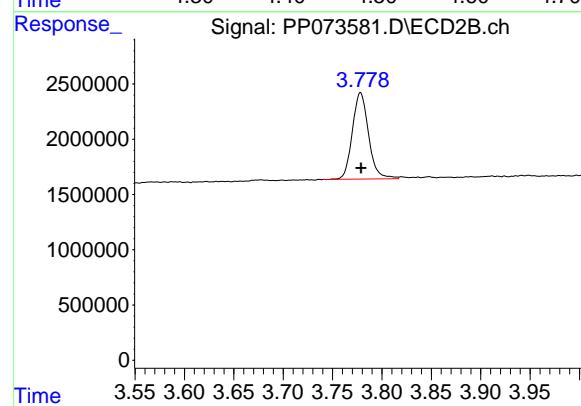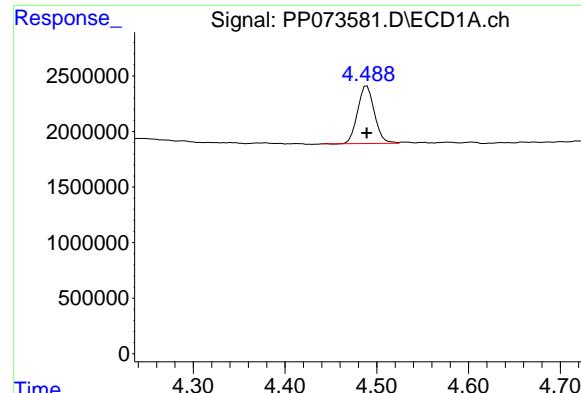

#1 Tetrachloro-m-xylene

R.T.: 4.489 min
 Delta R.T.: 0.000 min
 Response: 6570480
 Conc: 4.65 ng/ml

Instrument: ECD_P
 ClientSampleId : AR1268ICC050

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/08/2025
 Supervised By :mohammad ahmed 07/09/2025

#1 Tetrachloro-m-xylene

R.T.: 3.778 min
 Delta R.T.: 0.000 min
 Response: 8954068
 Conc: 4.60 ng/ml

#2 Decachlorobiphenyl

R.T.: 10.178 min
 Delta R.T.: 0.001 min
 Response: 8974224
 Conc: 4.35 ng/ml

#2 Decachlorobiphenyl

R.T.: 8.780 min
 Delta R.T.: 0.000 min
 Response: 11778445
 Conc: 4.63 ng/ml





#41 AR-1268-1

R.T.: 8.694 min
 Delta R.T.: 0.000 min
 Response: 10231981
 Conc: 44.90 ng/ml

Instrument: ECD_P
ClientSampleId: AR1268ICC050

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/08/2025
 Supervised By :mohammad ahmed 07/09/2025

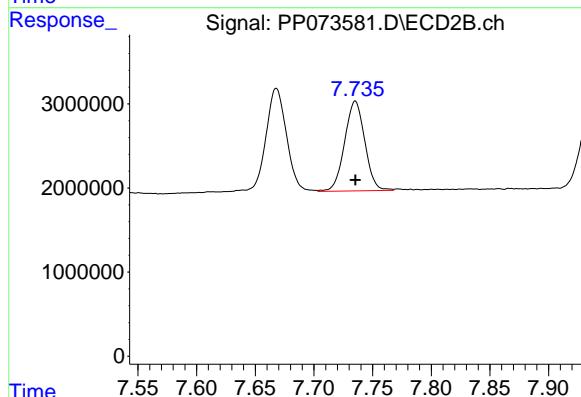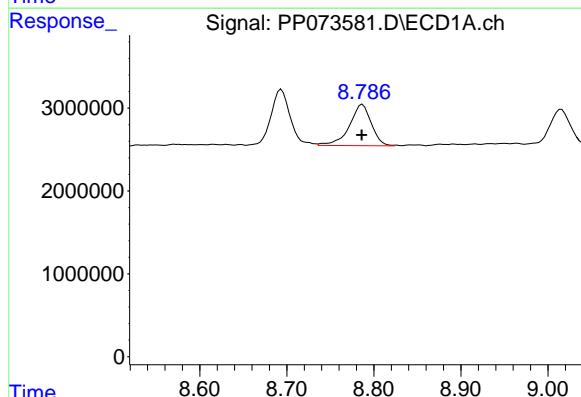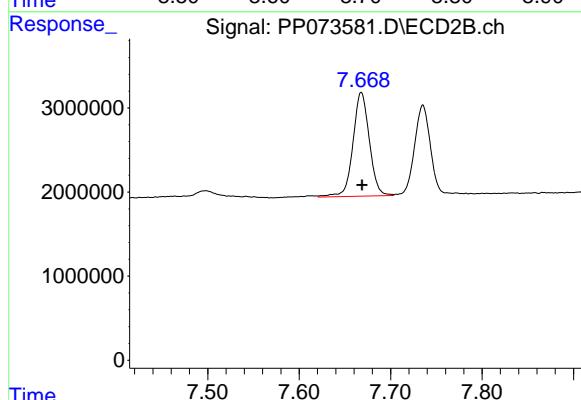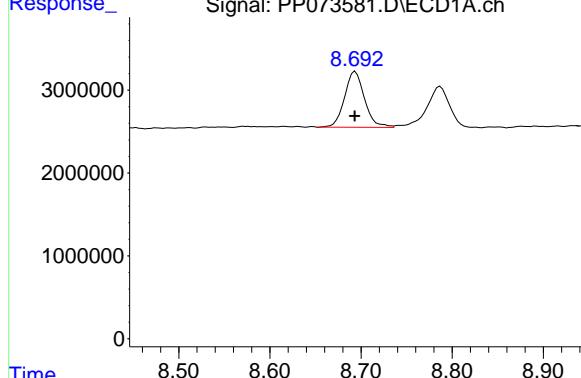

#41 AR-1268-1


R.T.: 7.668 min
 Delta R.T.: 0.000 min
 Response: 15365679
 Conc: 49.99 ng/ml

#42 AR-1268-2

R.T.: 8.787 min
 Delta R.T.: 0.000 min
 Response: 8726381
 Conc: 44.87 ng/ml

#42 AR-1268-2

R.T.: 7.735 min
 Delta R.T.: 0.000 min
 Response: 12801300
 Conc: 47.75 ng/ml

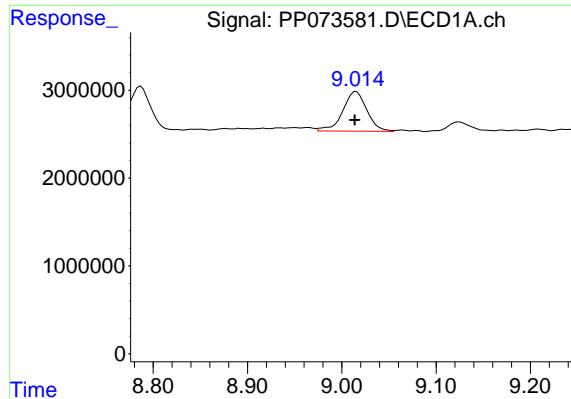


#43 AR-1268-3

R.T.: 9.015 min
 Delta R.T.: 0.002 min
 Response: 8012537
 Conc: 48.01 ng/ml

Instrument: ECD_P
ClientSampleId: AR1268ICC050


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/08/2025
 Supervised By :mohammad ahmed 07/09/2025

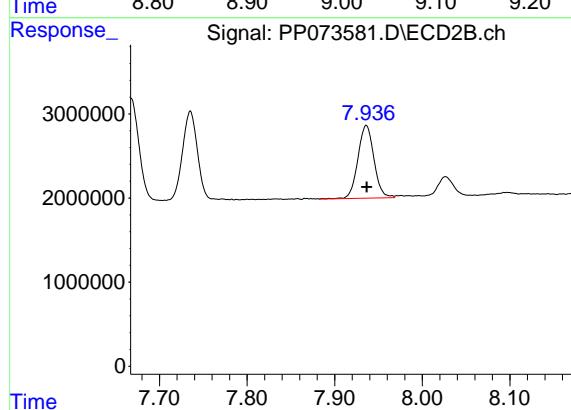


#43 AR-1268-3

R.T.: 7.936 min
 Delta R.T.: 0.000 min
 Response: 11044482
 Conc: 48.71 ng/ml

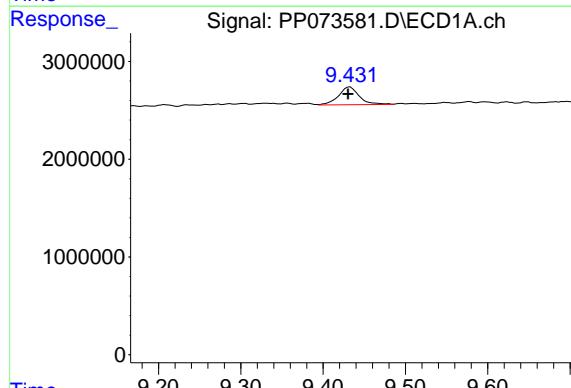

#44 AR-1268-4

R.T.: 9.433 min
 Delta R.T.: 0.003 min
 Response: 3216586
 Conc: 45.40 ng/ml

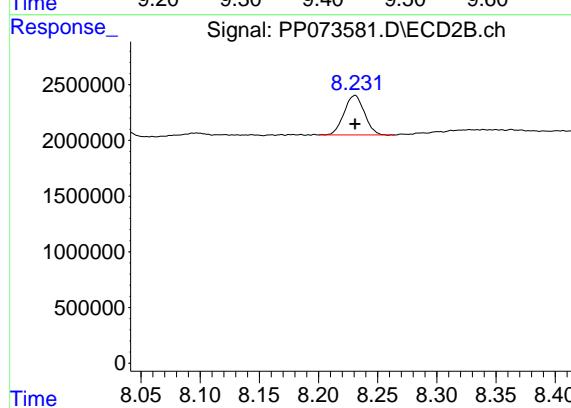

#44 AR-1268-4

R.T.: 8.231 min
 Delta R.T.: 0.000 min
 Response: 4250036
 Conc: 44.76 ng/ml



#45 AR-1268-5

R.T.: 9.839 min
 Delta R.T.: -0.002 min
 Response: 18594477
 Conc: 38.48 ng/ml

Instrument: ECD_P
ClientSampleId: AR1268ICC050

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/08/2025
 Supervised By :mohammad ahmed 07/09/2025

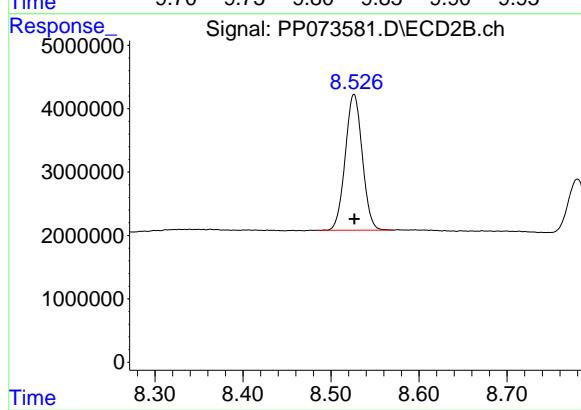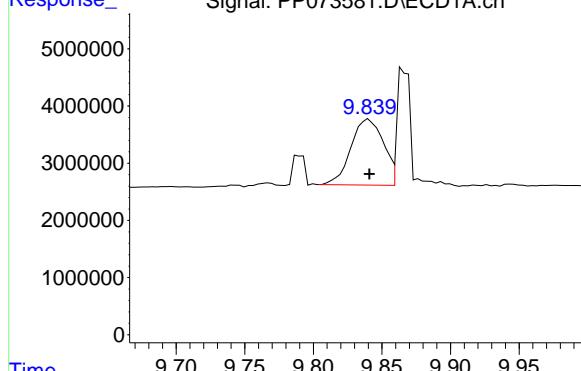

#45 AR-1268-5

R.T.: 8.526 min
 Delta R.T.: 0.000 min
 Response: 28831591
 Conc: 46.02 ng/ml

1
2
3
4
5
6
7
8
9
10
11
12
13
14
15
16
17
18
19
20

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP070825\
 Data File : PP073582.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jul 2025 04:41
 Operator : YP\AJ
 Sample : PP070825ICV500
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
ICVPP070825

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 08 05:27:43 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 08 05:27:19 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	4.485	3.779	72260983	95891777	52.763	52.050
2) SA Decachlor...	10.173	8.780	57429181	73824211	52.636	55.794

Target Compounds

3) L1 AR-1016-1	5.636	4.857	23819344	35187796	501.317	516.141
4) L1 AR-1016-2	5.657	4.875	36673403	52182388	514.968	512.173
5) L1 AR-1016-3	5.719	5.051	22168045	28112093	507.707	519.571
6) L1 AR-1016-4	5.817	5.093	18666023	22689979	519.286	517.082
7) L1 AR-1016-5	6.109	5.307	16712865	28698340	533.439	525.779
31) L7 AR-1260-1	7.226	6.337	30361600	49427132	514.942	506.632
32) L7 AR-1260-2	7.479	6.525	43933298	61439670	458.403	500.170
33) L7 AR-1260-3	7.837	6.677	37495485	56331160	513.140	514.610
34) L7 AR-1260-4	8.061	7.146	33945827	47047060	519.845	526.204
35) L7 AR-1260-5	8.379	7.389	79838825	118.4E6	529.250	526.873



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.





Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP070825\
 Data File : PP073582.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jul 2025 04:41
 Operator : YP\AJ
 Sample : PP070825ICV500
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
ICVPP070825

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 08 05:27:43 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 08 05:27:19 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

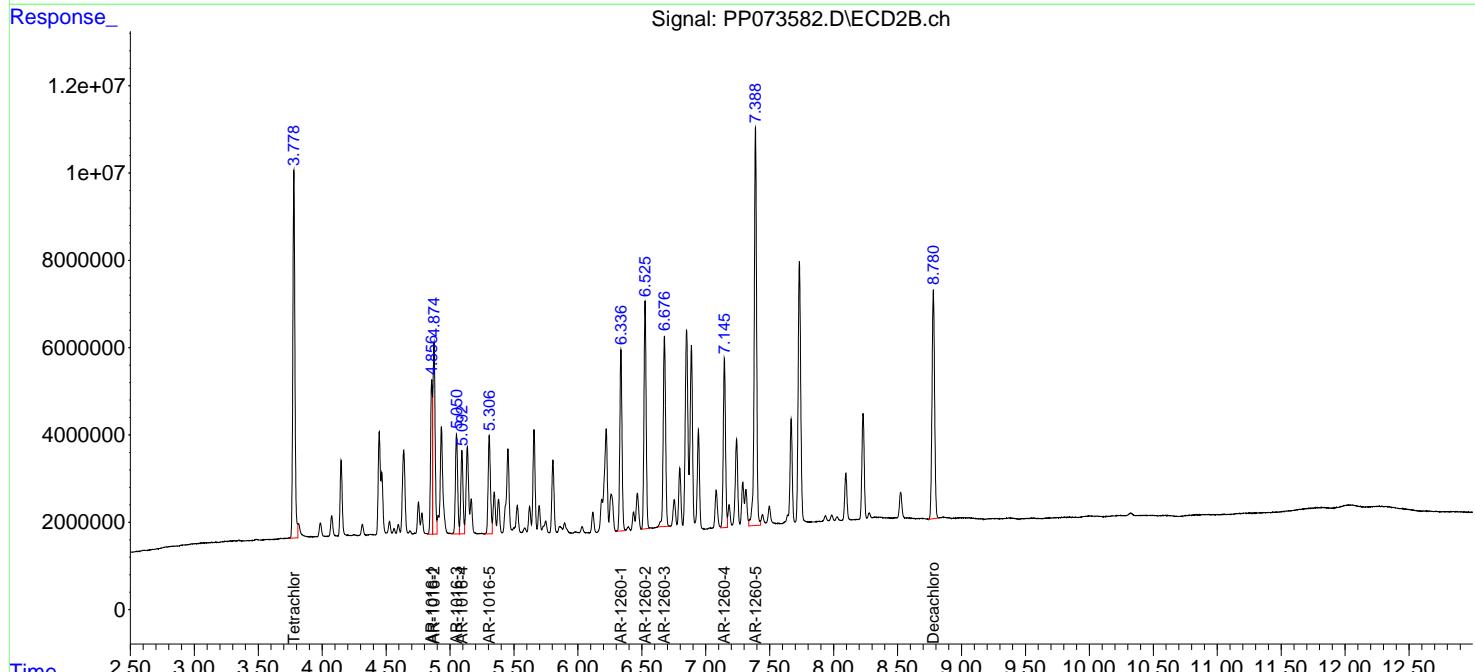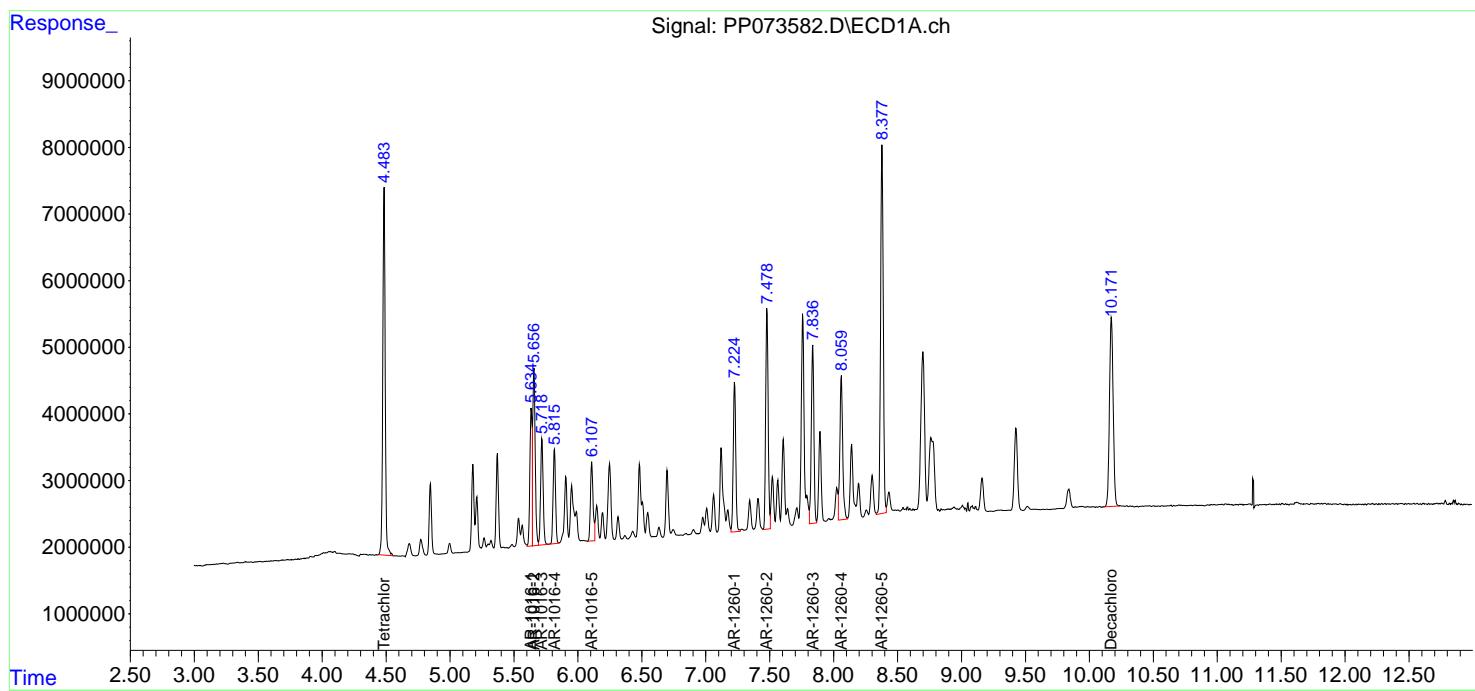

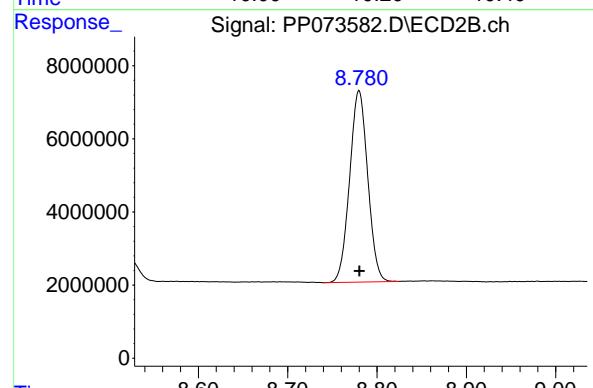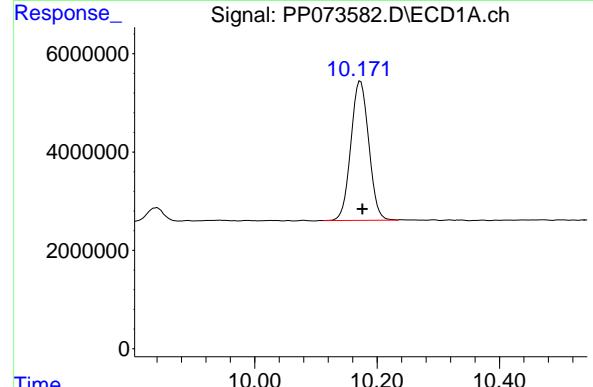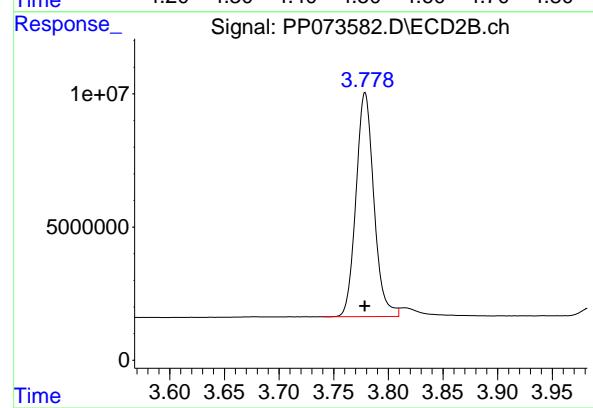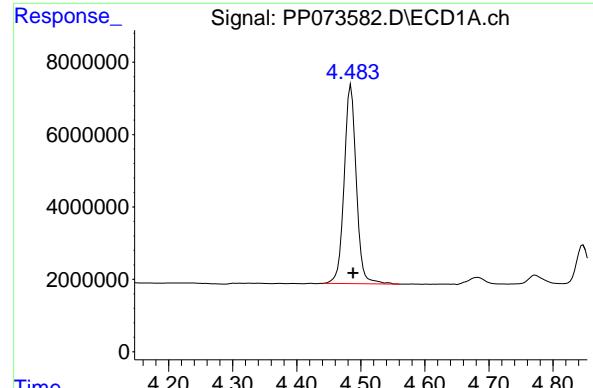

#1 Tetrachloro-m-xylene

R.T.: 4.485 min
 Delta R.T.: -0.003 min
 Response: 72260983
 Conc: 52.76 ng/ml

Instrument: ECD_P
ClientSampleId: ICVPP070825

#1 Tetrachloro-m-xylene

R.T.: 3.779 min
 Delta R.T.: 0.000 min
 Response: 95891777
 Conc: 52.05 ng/ml

#2 Decachlorobiphenyl

R.T.: 10.173 min
 Delta R.T.: -0.003 min
 Response: 57429181
 Conc: 52.64 ng/ml


#2 Decachlorobiphenyl

R.T.: 8.780 min
 Delta R.T.: 0.000 min
 Response: 73824211
 Conc: 55.79 ng/ml

#3 AR-1016-1


R.T.: 5.636 min
 Delta R.T.: -0.003 min
 Response: 23819344
 Conc: 501.32 ng/ml

Instrument: ECD_P
 ClientSampleId: ICVPP070825




#3 AR-1016-1

R.T.: 4.857 min
 Delta R.T.: 0.000 min
 Response: 35187796
 Conc: 516.14 ng/ml

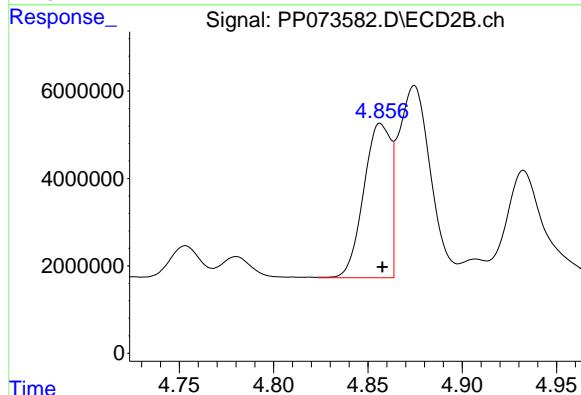


#4 AR-1016-2

R.T.: 5.657 min
 Delta R.T.: -0.003 min
 Response: 36673403
 Conc: 514.97 ng/ml

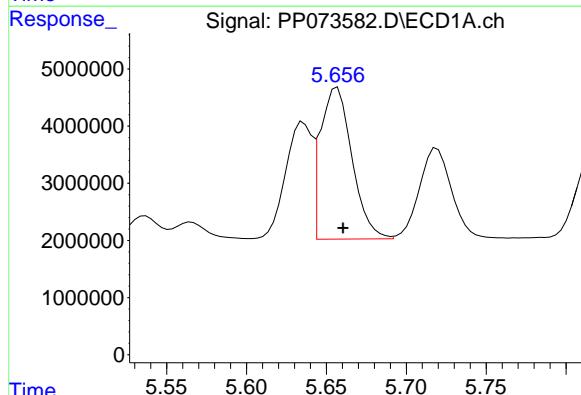

#4 AR-1016-2


R.T.: 4.875 min
 Delta R.T.: 0.000 min
 Response: 52182388
 Conc: 512.17 ng/ml

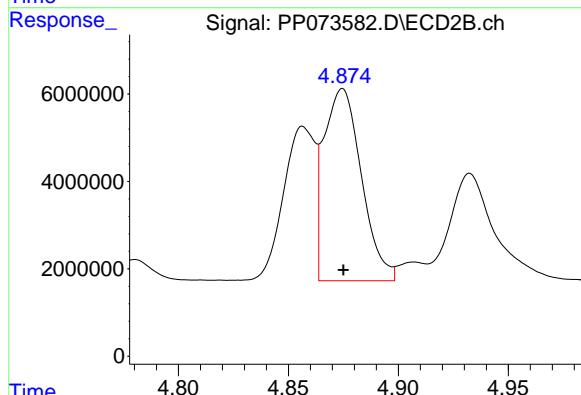

#5 AR-1016-3


R.T.: 5.719 min
 Delta R.T.: -0.003 min
 Response: 22168045
 Conc: 507.71 ng/ml

Instrument: ECD_P
 ClientSampleId: ICVPP070825

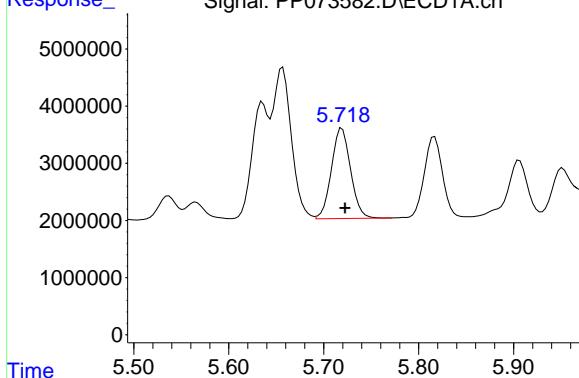


#5 AR-1016-3

R.T.: 5.051 min
 Delta R.T.: 0.000 min
 Response: 28112093
 Conc: 519.57 ng/ml

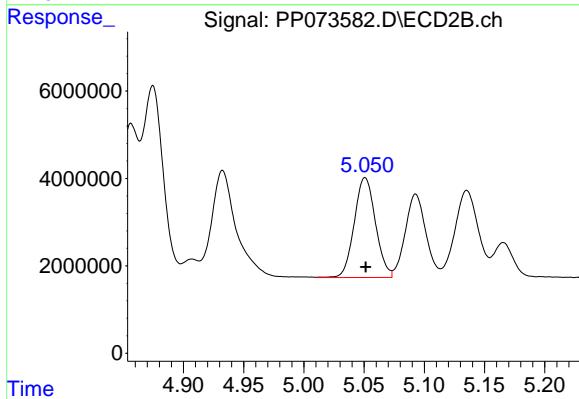


#6 AR-1016-4


R.T.: 5.817 min
 Delta R.T.: -0.003 min
 Response: 18666023
 Conc: 519.29 ng/ml

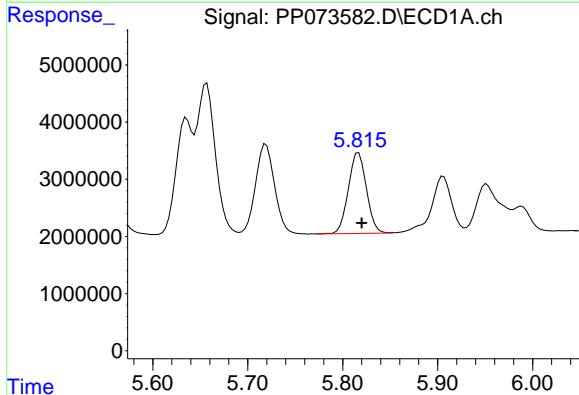

#6 AR-1016-4

R.T.: 5.093 min
 Delta R.T.: 0.000 min
 Response: 22689979
 Conc: 517.08 ng/ml

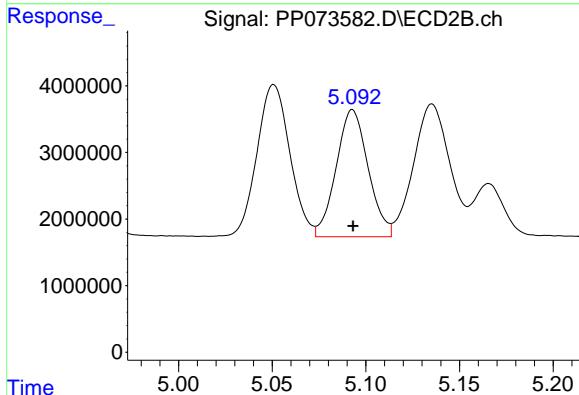

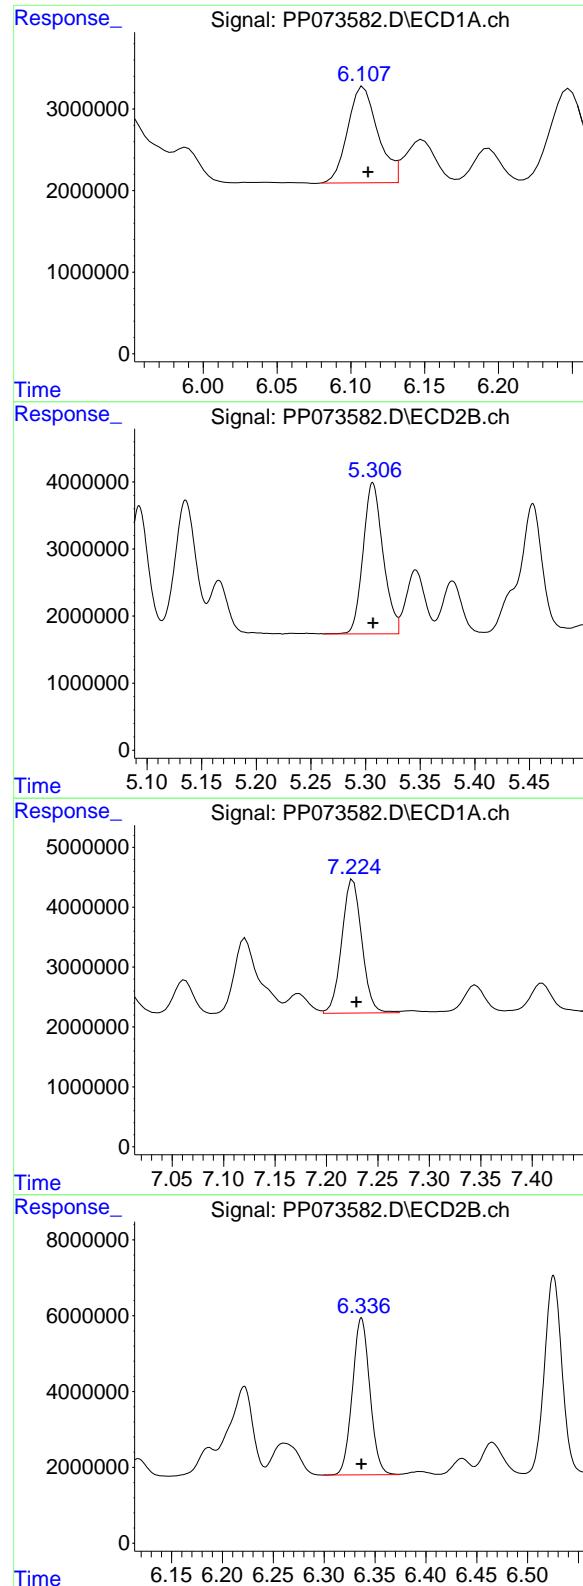

#7 AR-1016-5

R.T.: 6.109 min
 Delta R.T.: -0.003 min
 Response: 16712865
 Conc: 533.44 ng/ml

Instrument: ECD_P
 ClientSampleId: ICVPP070825

#7 AR-1016-5

R.T.: 5.307 min
 Delta R.T.: 0.000 min
 Response: 28698340
 Conc: 525.78 ng/ml

#31 AR-1260-1

R.T.: 7.226 min
 Delta R.T.: -0.003 min
 Response: 30361600
 Conc: 514.94 ng/ml





#31 AR-1260-1

R.T.: 6.337 min
 Delta R.T.: 0.000 min
 Response: 49427132
 Conc: 506.63 ng/ml

#32 AR-1260-2

R.T.: 7.479 min
 Delta R.T.: -0.004 min
 Response: 43933298
 Conc: 458.40 ng/ml

Instrument: ECD_P
ClientSampleId: ICVPP070825

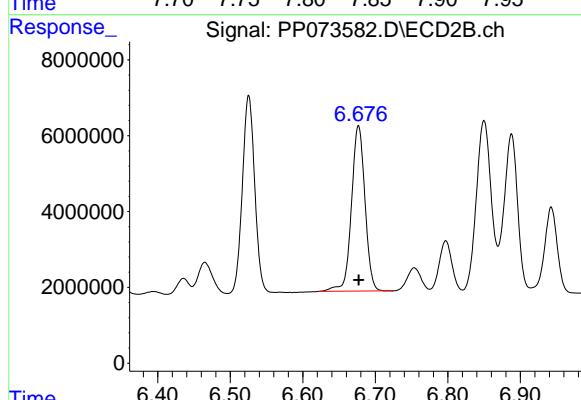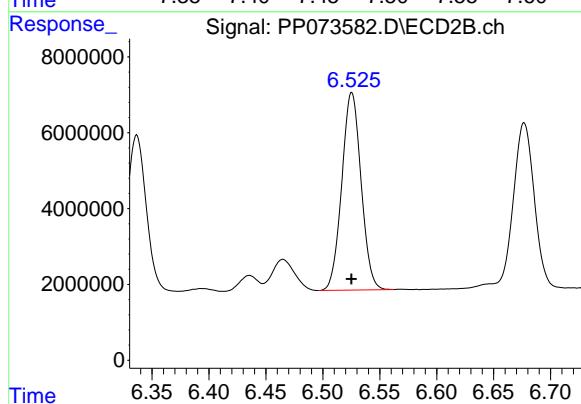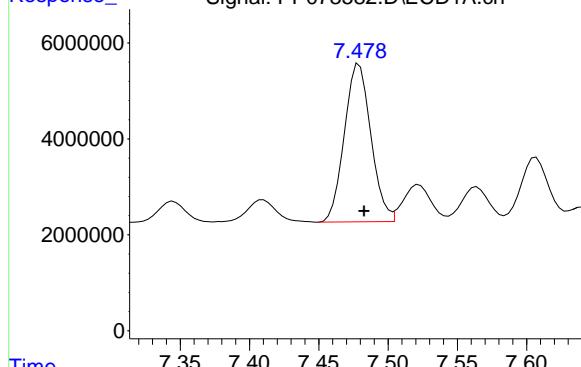

#32 AR-1260-2

R.T.: 6.525 min
 Delta R.T.: 0.000 min
 Response: 61439670
 Conc: 500.17 ng/ml

#33 AR-1260-3

R.T.: 7.837 min
 Delta R.T.: -0.003 min
 Response: 37495485
 Conc: 513.14 ng/ml


#33 AR-1260-3

R.T.: 6.677 min
 Delta R.T.: 0.000 min
 Response: 56331160
 Conc: 514.61 ng/ml

#34 AR-1260-4


R.T.: 8.061 min
 Delta R.T.: -0.004 min
 Response: 33945827
 Conc: 519.85 ng/ml

Instrument: ECD_P
ClientSampleId: ICVPP070825




#34 AR-1260-4

R.T.: 7.146 min
 Delta R.T.: 0.000 min
 Response: 47047060
 Conc: 526.20 ng/ml

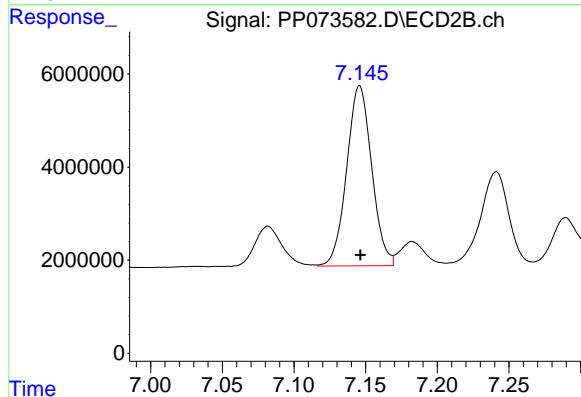


#35 AR-1260-5

R.T.: 8.379 min
 Delta R.T.: -0.004 min
 Response: 79838825
 Conc: 529.25 ng/ml

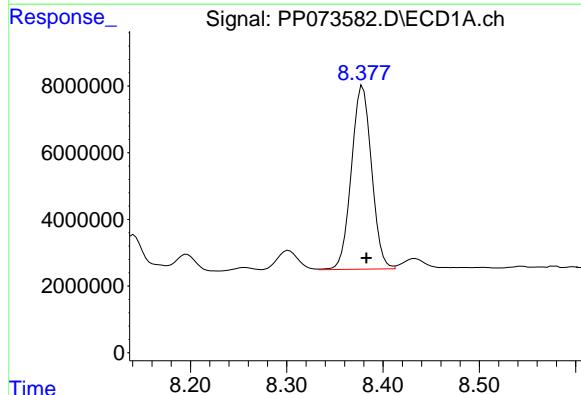

#35 AR-1260-5

R.T.: 7.389 min
 Delta R.T.: 0.000 min
 Response: 118407698
 Conc: 526.87 ng/ml

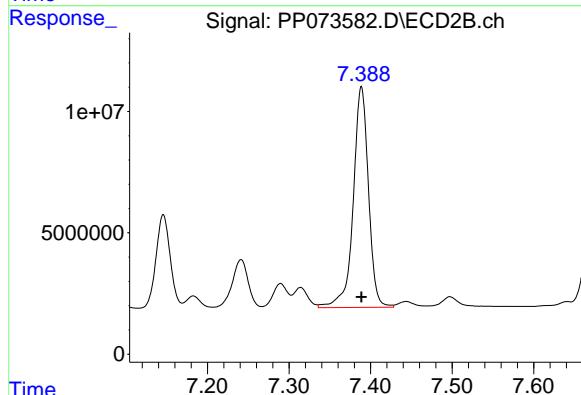

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP070825\
 Data File : PP073583.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jul 2025 05:30
 Operator : YP\AJ
 Sample : AR1242ICV500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
ICVPP070825AR1242

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 08 05:53:38 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 08 05:39:05 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	4.486	3.780	72993940	98810271	53.555	54.104
2) SA Decachlor...	10.175	8.781	59178077	71524197	53.748	53.924

Target Compounds

16) L4 AR-1242-1	5.637	4.858	20775175	30801945	544.021	533.231
17) L4 AR-1242-2	5.658	4.875	31979969	45687015	534.049	528.453
18) L4 AR-1242-3	5.720	5.052	19490860	24488942	532.233	532.986
19) L4 AR-1242-4	5.817	5.136	16125476	23556759	501.788	532.196
20) L4 AR-1242-5	6.547	5.657	17188141	29930341	525.039	541.800



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.



Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP070825\
 Data File : PP073583.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jul 2025 05:30
 Operator : YP\AJ
 Sample : AR12421ICV500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
ICVPP070825AR1242

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 08 05:53:38 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 08 05:39:05 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ m Signal #2 Info : 30M x 0.32mm x 0.25 μ m

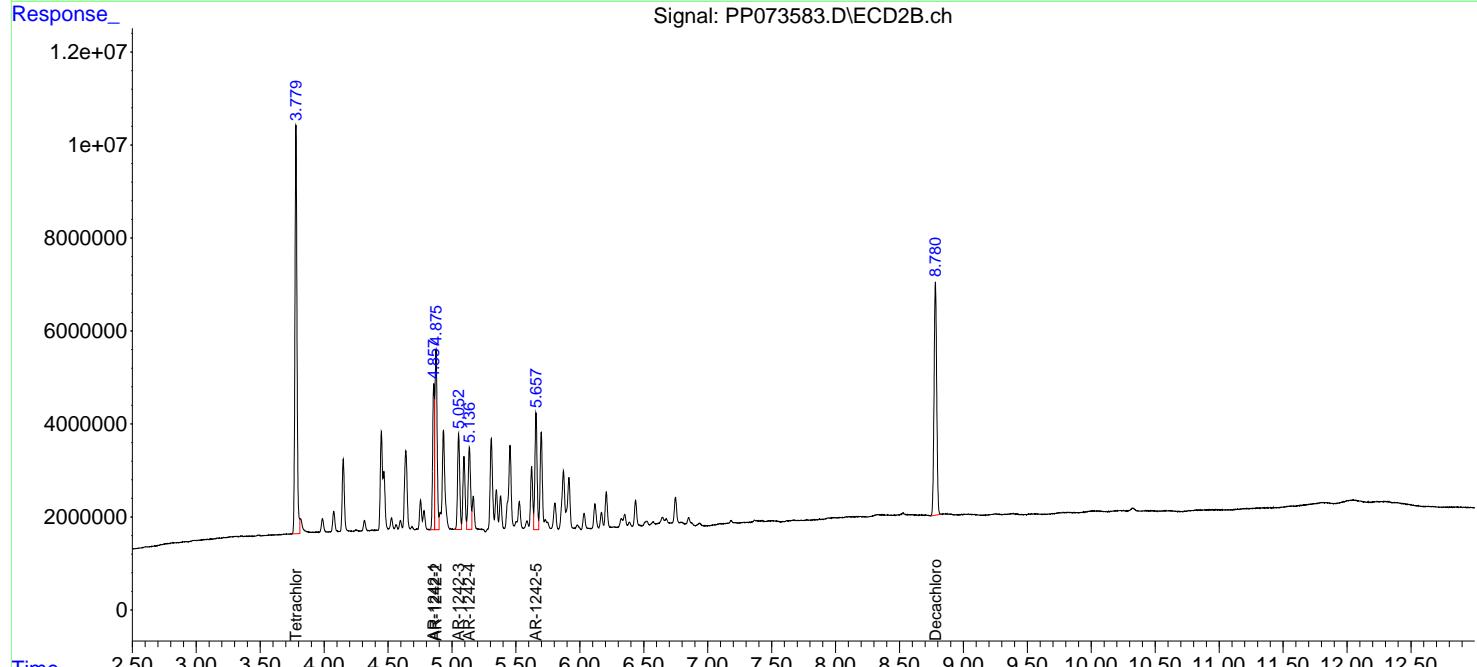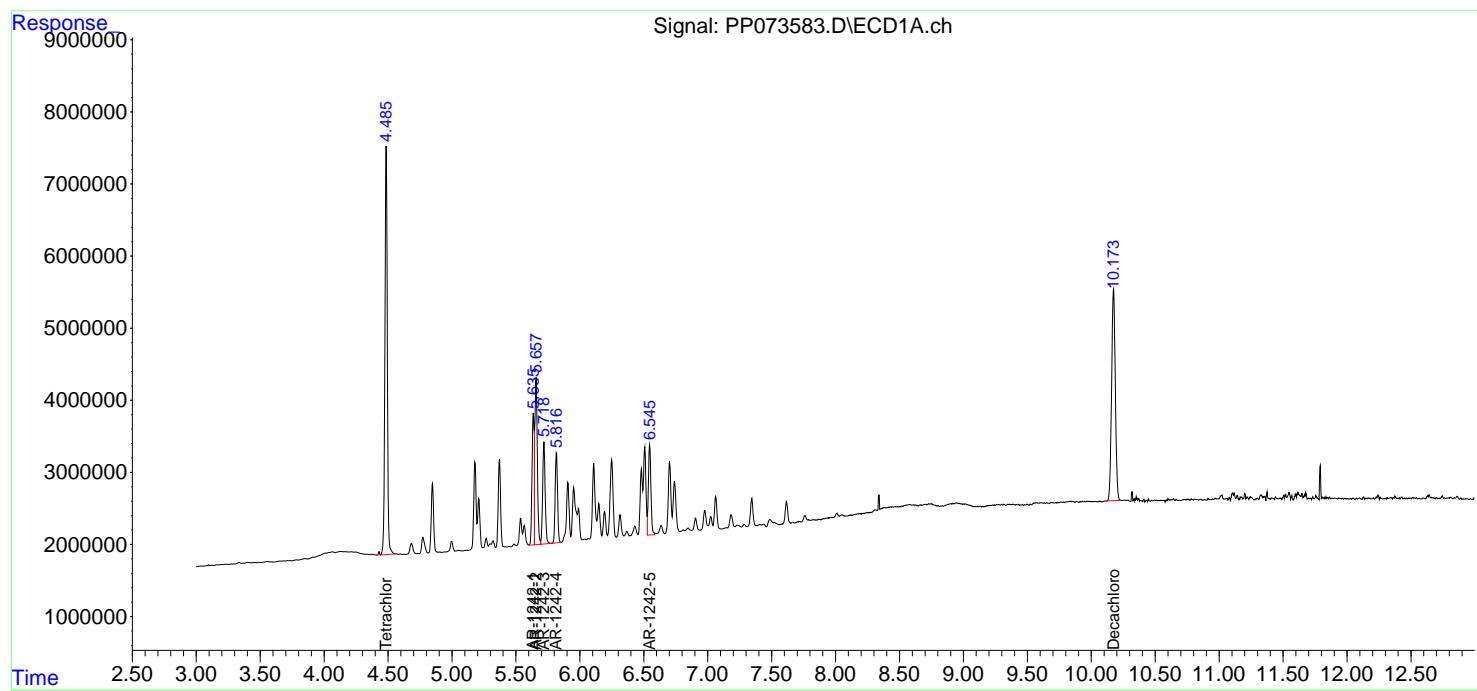

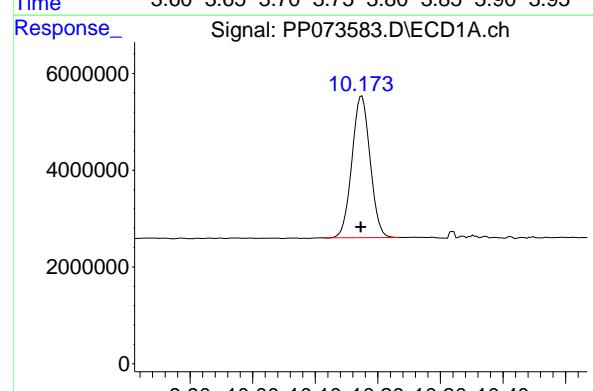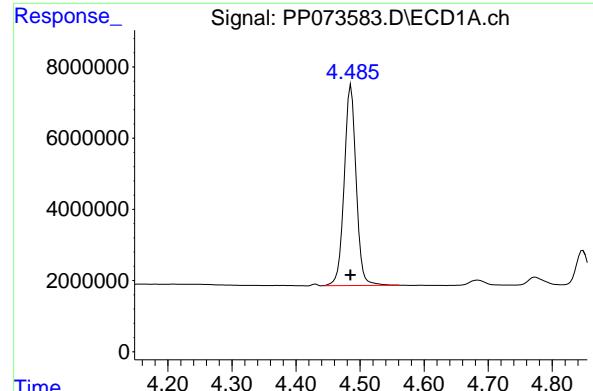

#1 Tetrachloro-m-xylene

R.T.: 4.486 min
Delta R.T.: 0.000 min
Response: 72993940
Conc: 53.56 ng/ml

Instrument: ECD_P
ClientSampleId: ICVPP070825AR1242

#1 Tetrachloro-m-xylene

R.T.: 3.780 min
Delta R.T.: 0.000 min
Response: 98810271
Conc: 54.10 ng/ml

#2 Decachlorobiphenyl

R.T.: 10.175 min
Delta R.T.: 0.002 min
Response: 59178077
Conc: 53.75 ng/ml


#2 Decachlorobiphenyl

R.T.: 8.781 min
Delta R.T.: 0.000 min
Response: 71524197
Conc: 53.92 ng/ml

#16 AR-1242-1


R.T.: 5.637 min
 Delta R.T.: 0.000 min
 Response: 20775175
 Conc: 544.02 ng/ml

Instrument: ECD_P
 ClientSampleId: ICVPP070825AR1242

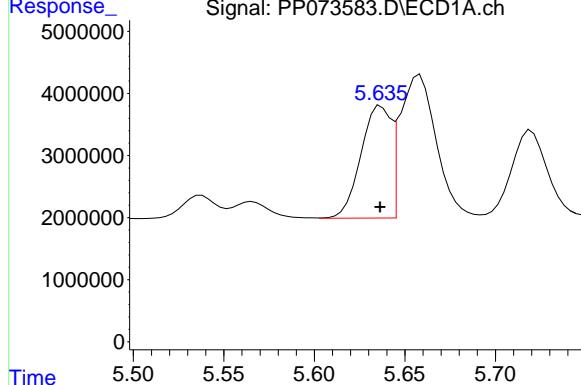


#16 AR-1242-1

R.T.: 4.858 min
 Delta R.T.: 0.000 min
 Response: 30801945
 Conc: 533.23 ng/ml

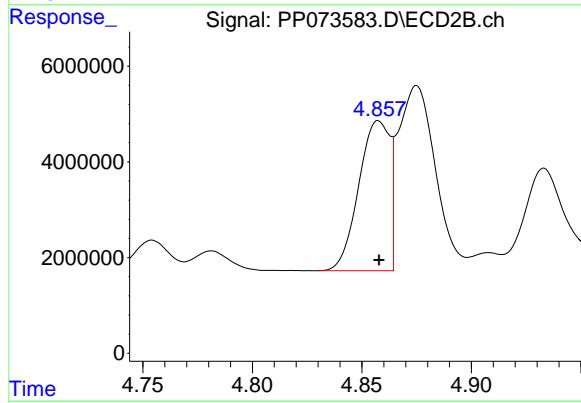


#17 AR-1242-2

R.T.: 5.658 min
 Delta R.T.: 0.000 min
 Response: 31979969
 Conc: 534.05 ng/ml

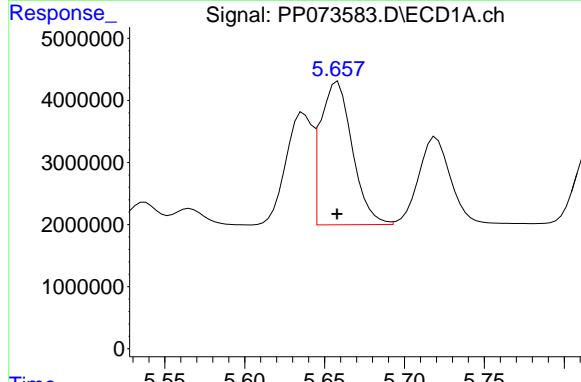

#17 AR-1242-2


R.T.: 4.875 min
 Delta R.T.: 0.000 min
 Response: 45687015
 Conc: 528.45 ng/ml

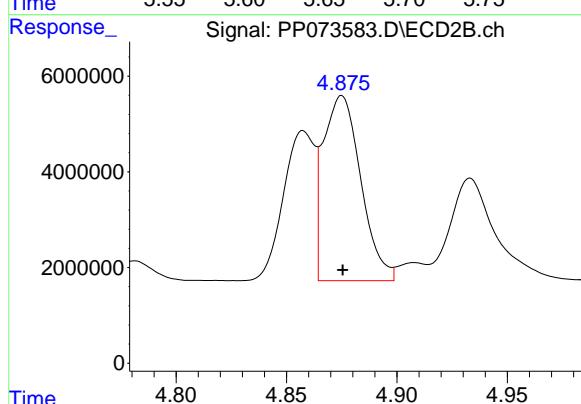

#18 AR-1242-3


R.T.: 5.720 min
 Delta R.T.: 0.000 min
 Response: 19490860
 Conc: 532.23 ng/ml

Instrument: ECD_P
 ClientSampleId: ICVPP070825AR1242

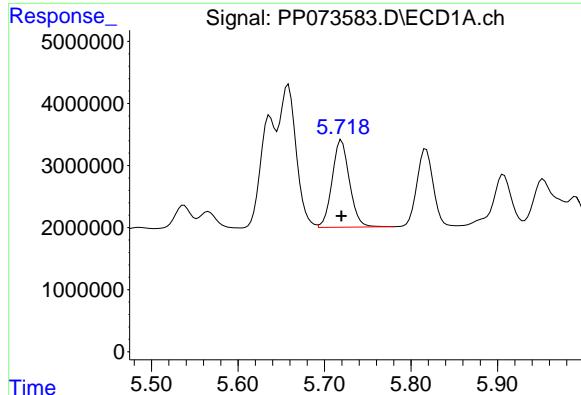


#18 AR-1242-3

R.T.: 5.052 min
 Delta R.T.: 0.000 min
 Response: 24488942
 Conc: 532.99 ng/ml

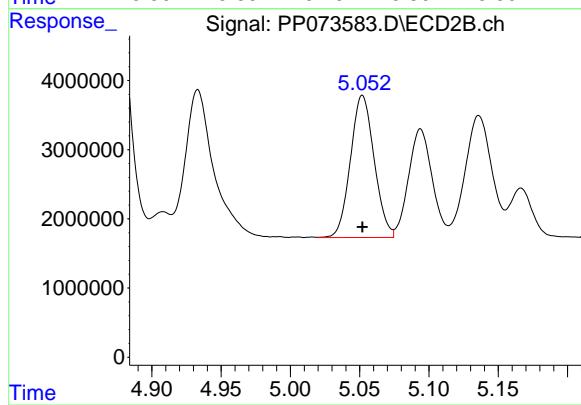


#19 AR-1242-4

R.T.: 5.817 min
 Delta R.T.: 0.000 min
 Response: 16125476
 Conc: 501.79 ng/ml



#19 AR-1242-4



R.T.: 5.136 min
 Delta R.T.: 0.000 min
 Response: 23556759
 Conc: 532.20 ng/ml



#20 AR-1242-5

R.T.: 6.547 min
Delta R.T.: 0.000 min
Response: 17188141
Conc: 525.04 ng/ml

Instrument: ECD_P
ClientSampleId: ICVPP070825AR1242

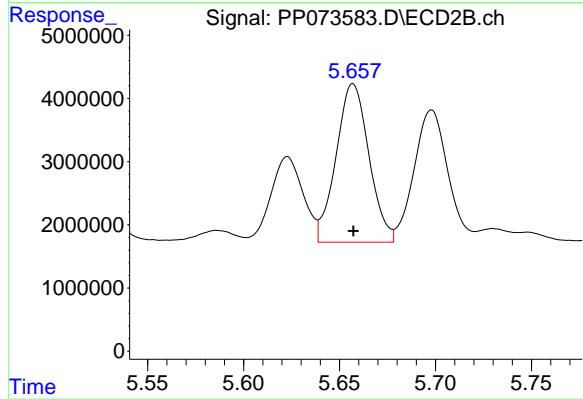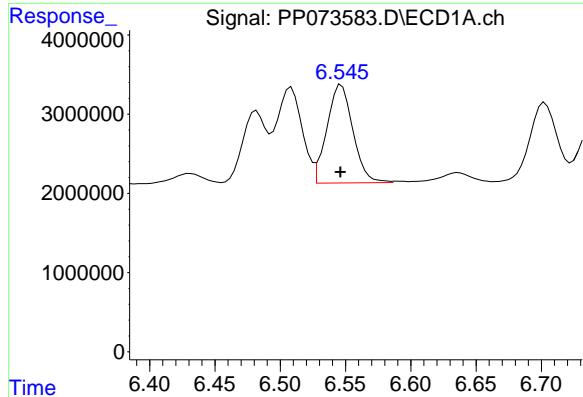

#20 AR-1242-5

R.T.: 5.657 min
Delta R.T.: 0.000 min
Response: 29930341
Conc: 541.80 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP070825\
 Data File : PP073584.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jul 2025 05:46
 Operator : YP\AJ
 Sample : AR1248ICV500
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
ICVPP070825AR1248

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 08 06:11:45 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 08 06:01:49 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	4.489	3.778	71424974	97266201	52.153	52.796
2) SA Decachlor...	10.176	8.779	58027297	74824812	53.185	56.551

Target Compounds

21) L5 AR-1248-1	5.639	4.857	15762091	23607850	510.587	525.847
22) L5 AR-1248-2	5.910	5.092	20492312	31849894	513.291	517.577
23) L5 AR-1248-3	6.112	5.134	23677594	33328191	533.164	520.228
24) L5 AR-1248-4	6.511	5.306	28997723	39129254	526.461	519.111
25) L5 AR-1248-5	6.550	5.697	28371365	39383540	527.441	527.994



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.





Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP070825\
 Data File : PP073584.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jul 2025 05:46
 Operator : YP\AJ
 Sample : AR1248ICV500
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
ICVPP070825AR1248

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 08 06:11:45 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 08 06:01:49 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

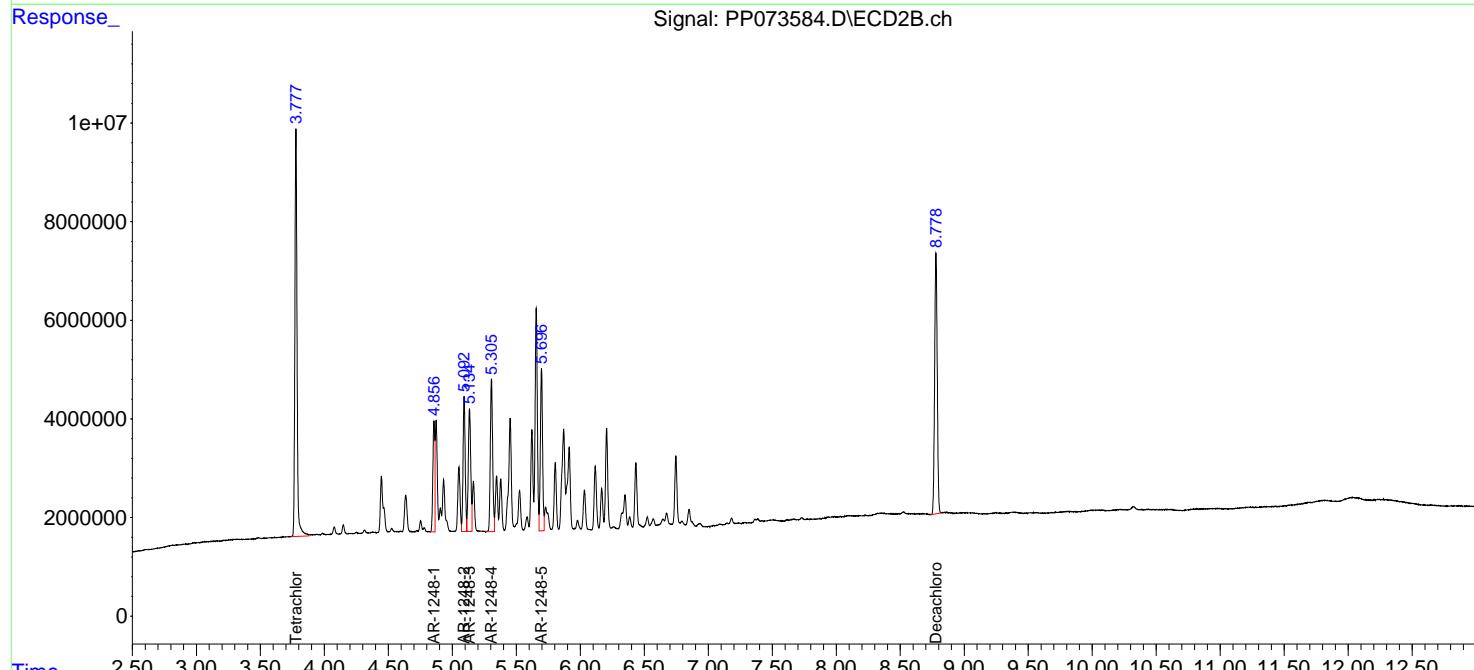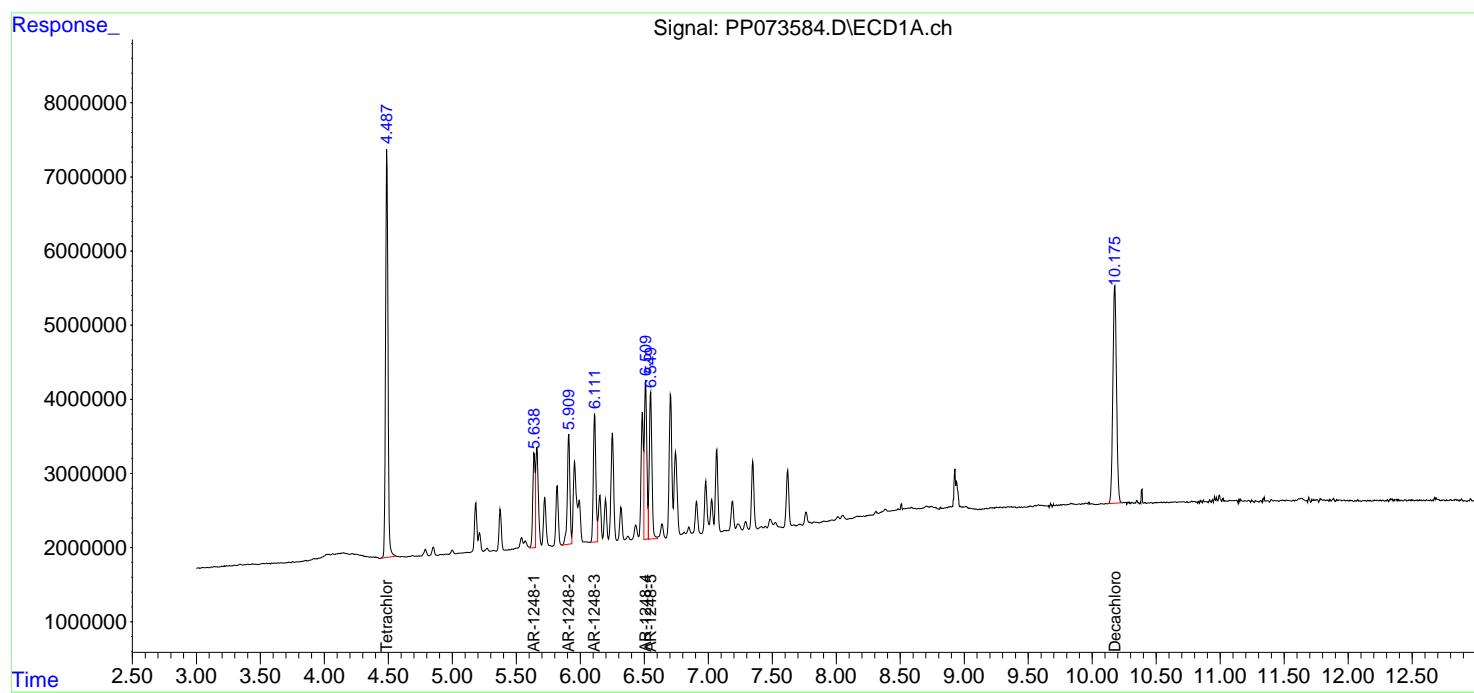

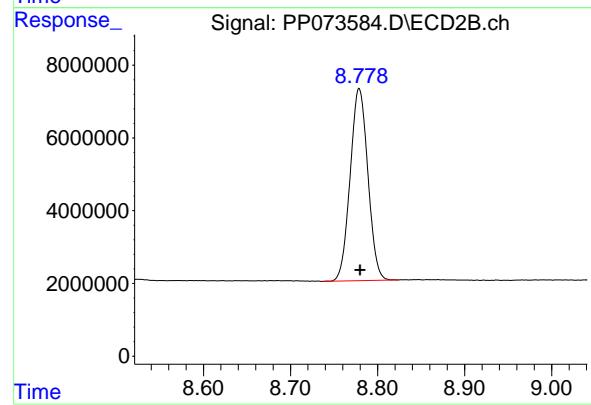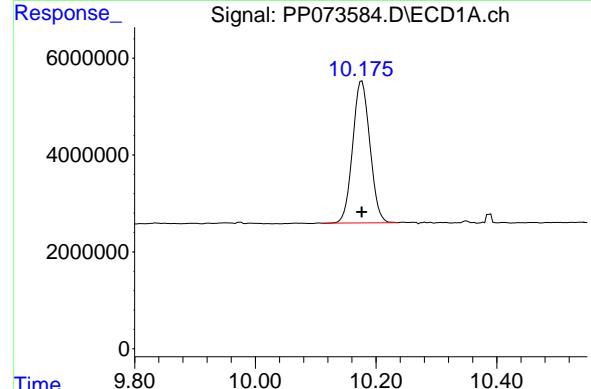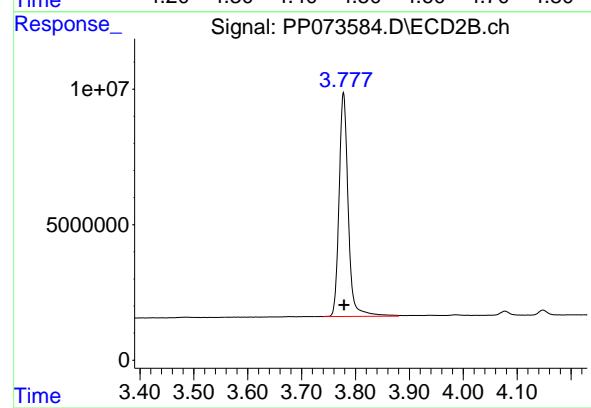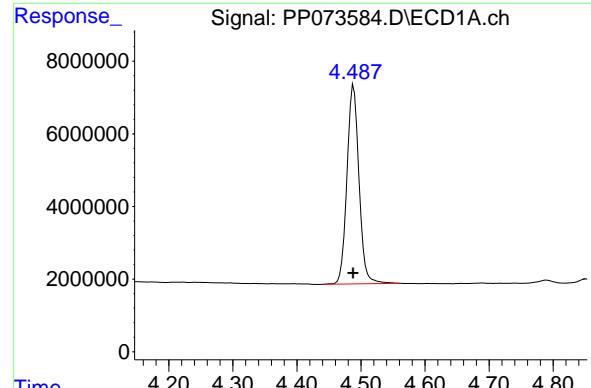

#1 Tetrachloro-m-xylene

R.T.: 4.489 min
 Delta R.T.: 0.000 min
 Response: 71424974
 Conc: 52.15 ng/ml

Instrument: ECD_P
 ClientSampleId: ICVPP070825AR1248

#1 Tetrachloro-m-xylene


R.T.: 3.778 min
 Delta R.T.: 0.000 min
 Response: 97266201
 Conc: 52.80 ng/ml

#2 Decachlorobiphenyl

R.T.: 10.176 min
 Delta R.T.: 0.000 min
 Response: 58027297
 Conc: 53.18 ng/ml

#2 Decachlorobiphenyl

R.T.: 8.779 min
 Delta R.T.: -0.001 min
 Response: 74824812
 Conc: 56.55 ng/ml

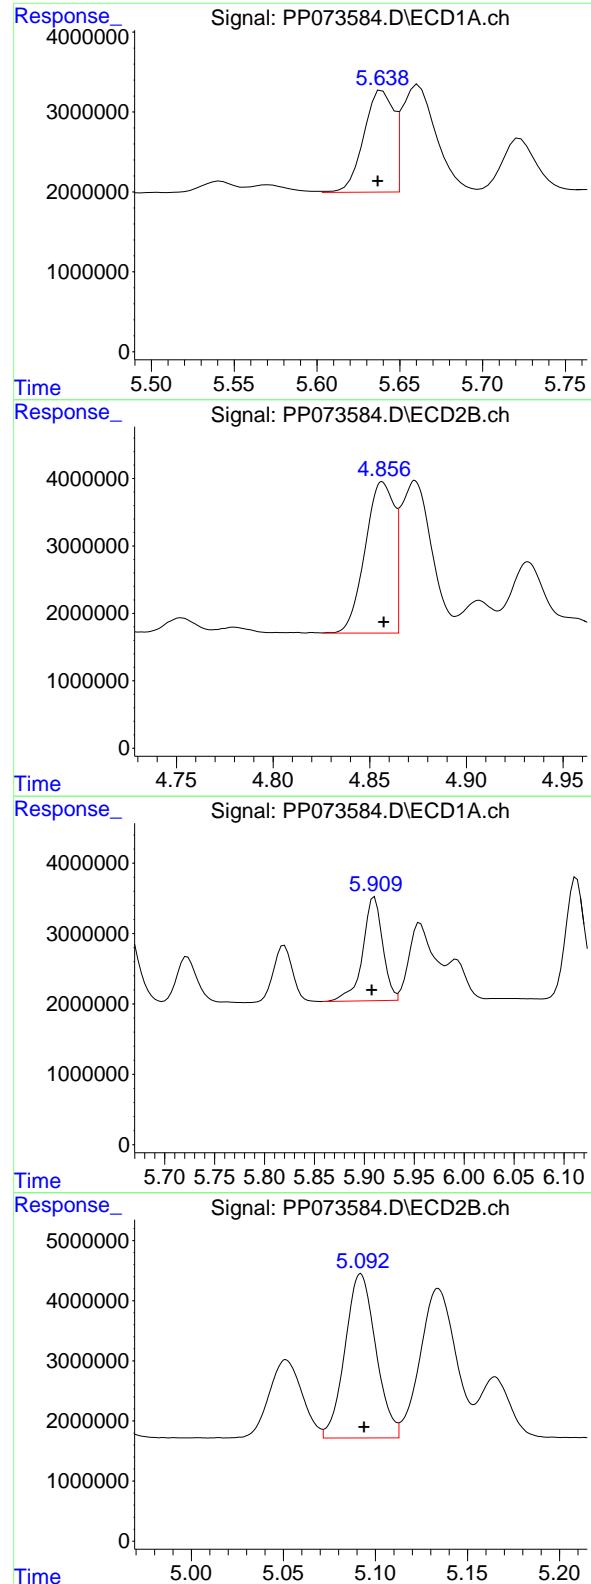

#21 AR-1248-1

R.T.: 5.639 min
 Delta R.T.: 0.003 min
 Response: 15762091
 Conc: 510.59 ng/ml

Instrument: ECD_P
 ClientSampleId: ICVPP070825AR1248

#21 AR-1248-1

R.T.: 4.857 min
 Delta R.T.: 0.000 min
 Response: 23607850
 Conc: 525.85 ng/ml

#22 AR-1248-2

R.T.: 5.910 min
 Delta R.T.: 0.003 min
 Response: 20492312
 Conc: 513.29 ng/ml


#22 AR-1248-2

R.T.: 5.092 min
 Delta R.T.: -0.002 min
 Response: 31849894
 Conc: 517.58 ng/ml

#23 AR-1248-3


R.T.: 6.112 min
 Delta R.T.: 0.003 min
 Response: 23677594
 Conc: 533.16 ng/ml

Instrument: ECD_P
ClientSampleId: ICVPP070825AR1248




#23 AR-1248-3

R.T.: 5.134 min
 Delta R.T.: -0.002 min
 Response: 33328191
 Conc: 520.23 ng/ml

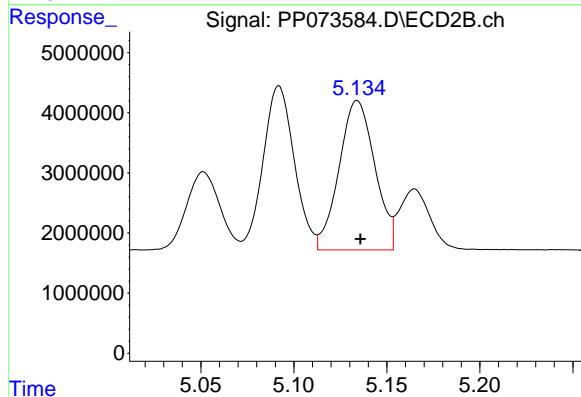


#24 AR-1248-4

R.T.: 6.511 min
 Delta R.T.: 0.002 min
 Response: 28997723
 Conc: 526.46 ng/ml

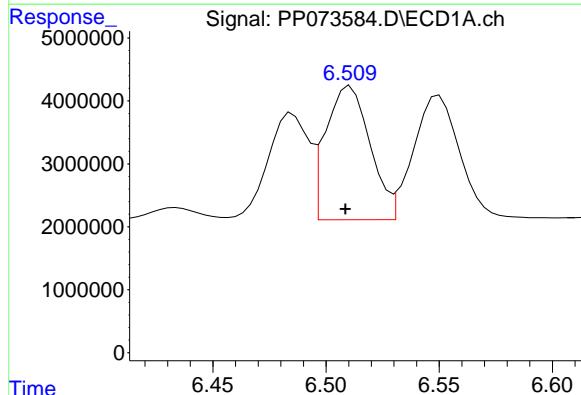

#24 AR-1248-4



R.T.: 5.306 min
 Delta R.T.: -0.002 min
 Response: 39129254
 Conc: 519.11 ng/ml

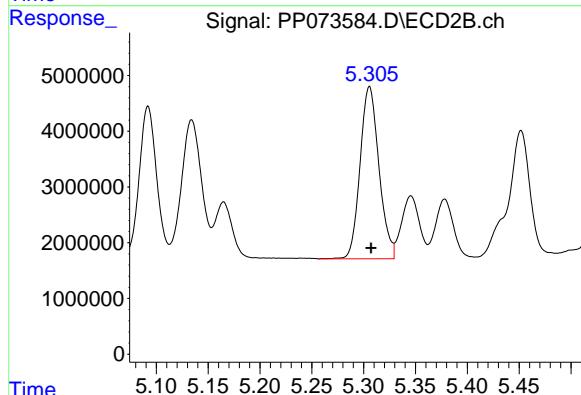

#25 AR-1248-5

R.T.: 6.550 min
Delta R.T.: 0.003 min
Response: 28371365
Conc: 527.44 ng/ml

Instrument: ECD_P
ClientSampleId: ICVPP070825AR1248

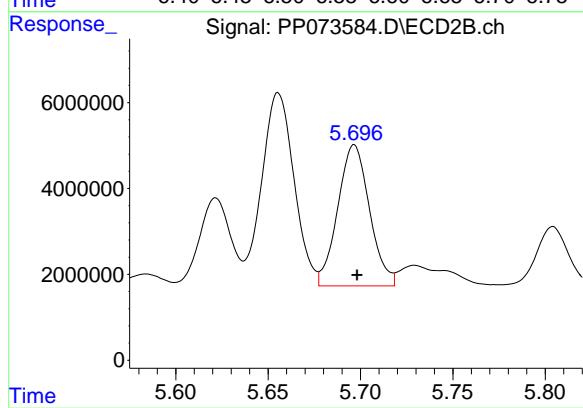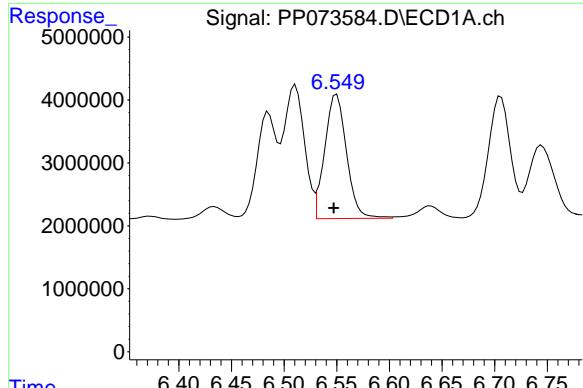

#25 AR-1248-5

R.T.: 5.697 min
Delta R.T.: -0.002 min
Response: 39383540
Conc: 527.99 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP070825\
 Data File : PP073585.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jul 2025 06:19
 Operator : YP\AJ
 Sample : AR1254ICV500
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
ICVPP070825AR1254

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 08 06:42:24 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 08 06:01:49 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	4.488	3.779	72137939	98177371	52.674	53.291
2) SA Decachlor...	10.176	8.780	58669520	75798661	53.773	57.287

Target Compounds

26) L6 AR-1254-1	6.486	5.657	27751618	57179282	517.855	492.797
27) L6 AR-1254-2	6.702	5.805	42039125	49615142	504.739	493.077
28) L6 AR-1254-3	7.065	6.207	45059626	78048221	510.118	505.342
29) L6 AR-1254-4	7.348	6.435	39772060	48017763	505.575	507.806
30) L6 AR-1254-5	7.764	6.851	38107518	68206603	517.204	511.122


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.





Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP070825\
 Data File : PP073585.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jul 2025 06:19
 Operator : YP\AJ
 Sample : AR1254ICV500
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
ICVPP070825AR1254

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 08 06:42:24 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 08 06:01:49 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ m Signal #2 Info : 30M x 0.32mm x 0.25 μ m

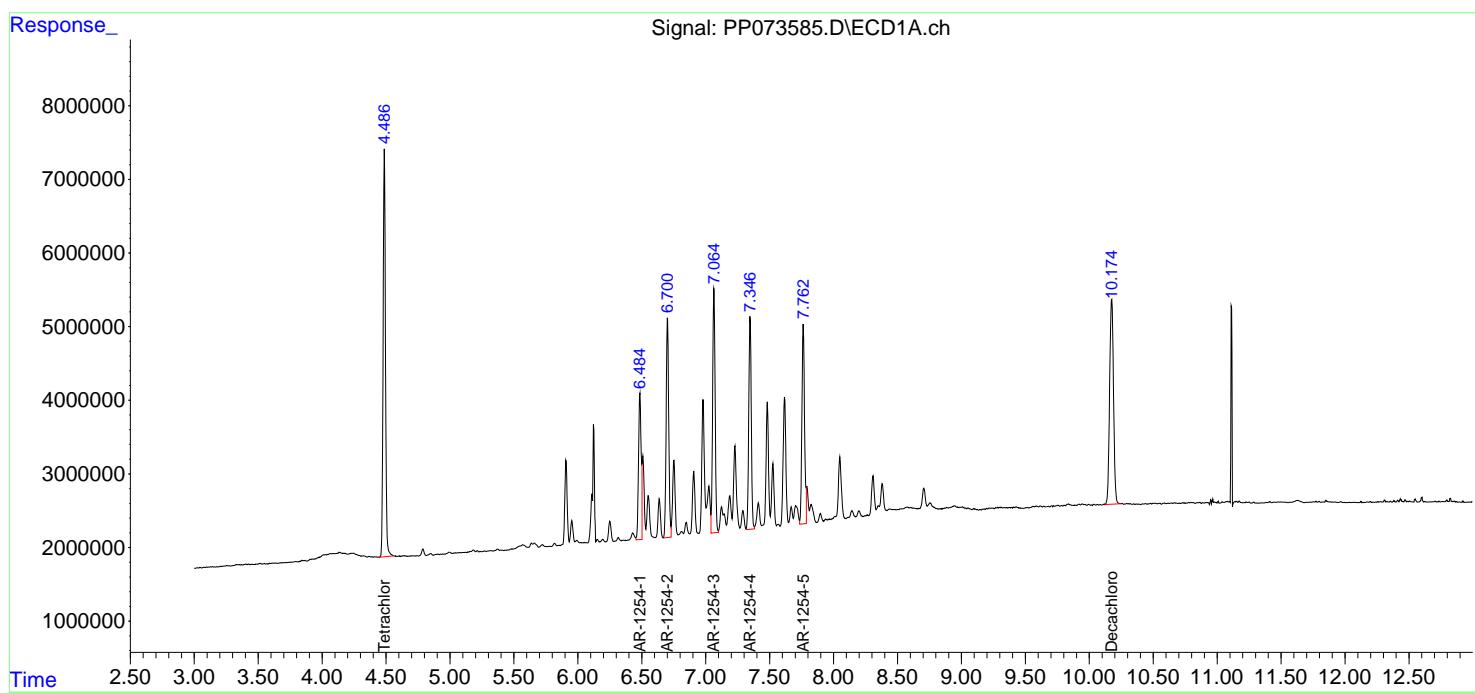

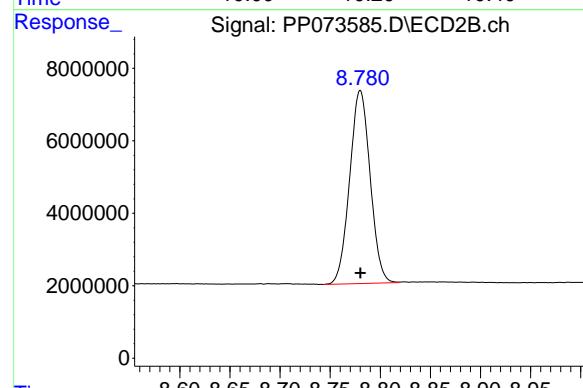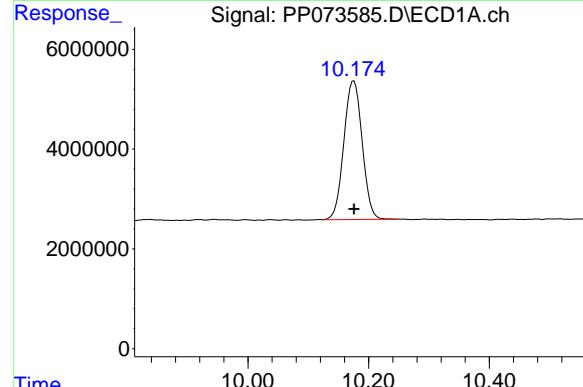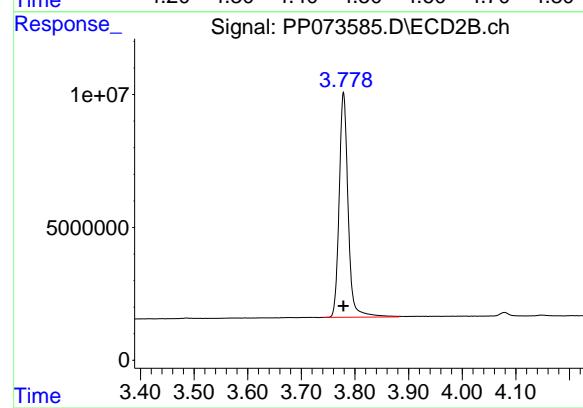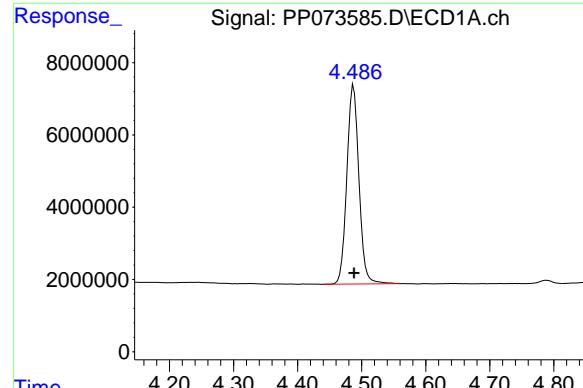

#1 Tetrachloro-m-xylene

R.T.: 4.488 min
Delta R.T.: 0.000 min
Response: 72137939
Conc: 52.67 ng/ml

Instrument: ECD_P
ClientSampleId: ICVPP070825AR1254

#1 Tetrachloro-m-xylene

R.T.: 3.779 min
Delta R.T.: 0.000 min
Response: 98177371
Conc: 53.29 ng/ml

#2 Decachlorobiphenyl

R.T.: 10.176 min
Delta R.T.: 0.000 min
Response: 58669520
Conc: 53.77 ng/ml


#2 Decachlorobiphenyl

R.T.: 8.780 min
Delta R.T.: 0.000 min
Response: 75798661
Conc: 57.29 ng/ml

#26 AR-1254-1


R.T.: 6.486 min
 Delta R.T.: 0.000 min
 Response: 27751618
 Conc: 517.86 ng/ml

Instrument: ECD_P
ClientSampleId: ICVPP070825AR1254




#26 AR-1254-1

R.T.: 5.657 min
 Delta R.T.: -0.001 min
 Response: 57179282
 Conc: 492.80 ng/ml

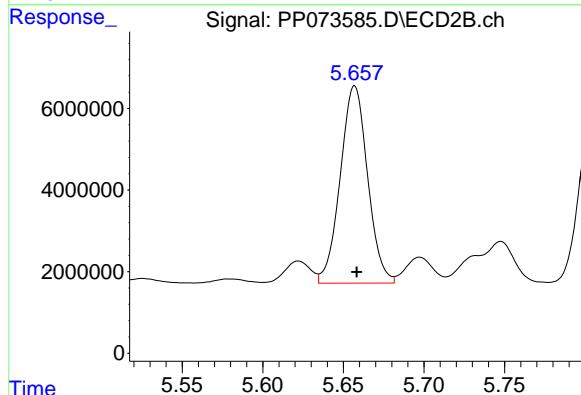


#27 AR-1254-2


R.T.: 6.702 min
 Delta R.T.: 0.000 min
 Response: 42039125
 Conc: 504.74 ng/ml

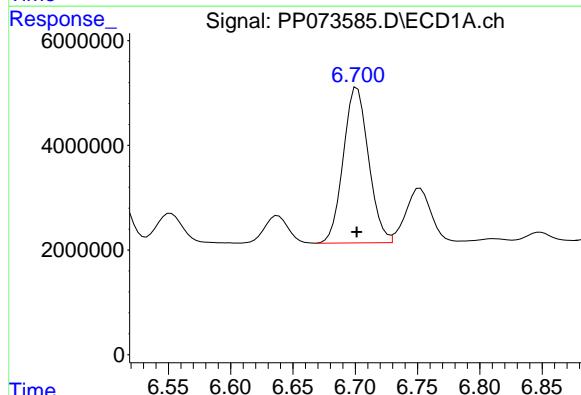

#27 AR-1254-2

R.T.: 5.805 min
 Delta R.T.: -0.002 min
 Response: 49615142
 Conc: 493.08 ng/ml

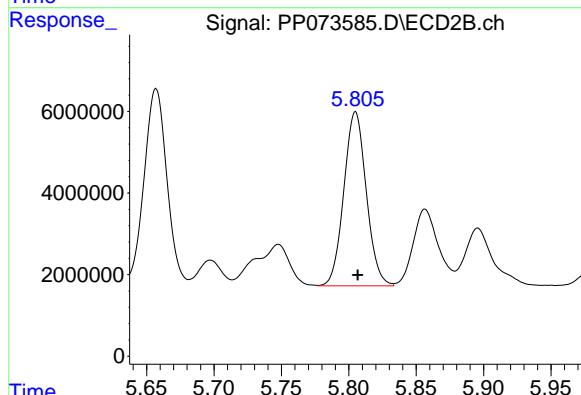

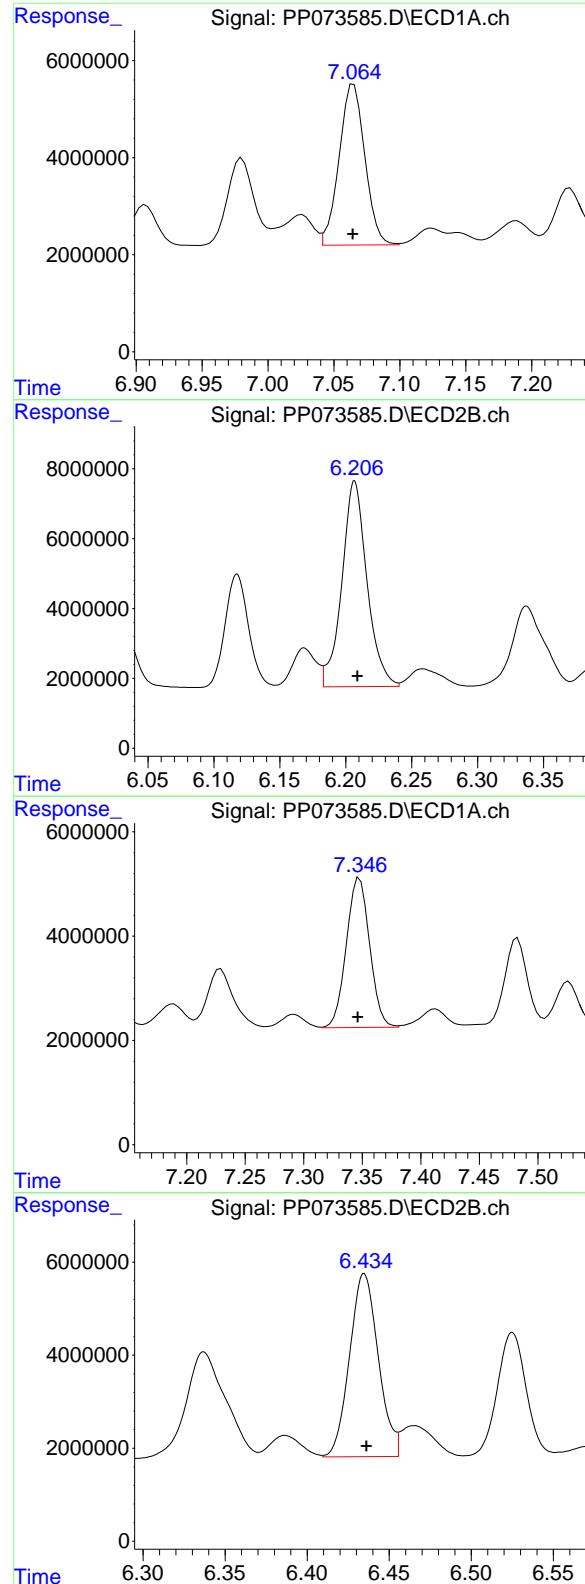

#28 AR-1254-3

R.T.: 7.065 min
 Delta R.T.: 0.000 min
 Response: 45059626
 Conc: 510.12 ng/ml

Instrument: ECD_P
 ClientSampleId: ICVPP070825AR1254

#28 AR-1254-3

R.T.: 6.207 min
 Delta R.T.: -0.002 min
 Response: 78048221
 Conc: 505.34 ng/ml


#29 AR-1254-4

R.T.: 7.348 min
 Delta R.T.: 0.001 min
 Response: 39772060
 Conc: 505.57 ng/ml

#29 AR-1254-4

R.T.: 6.435 min
 Delta R.T.: -0.001 min
 Response: 48017763
 Conc: 507.81 ng/ml

#30 AR-1254-5

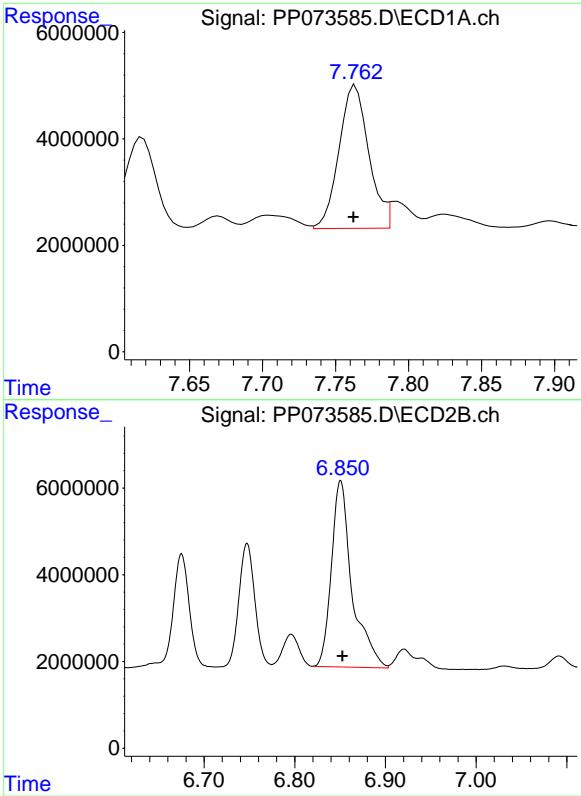


R.T.: 7.764 min
Delta R.T.: 0.001 min
Response: 38107518
Conc: 517.20 ng/ml

Instrument: ECD_P
ClientSampleId: ICVPP070825AR1254

#30 AR-1254-5

R.T.: 6.851 min
Delta R.T.: -0.002 min
Response: 68206603
Conc: 511.12 ng/ml

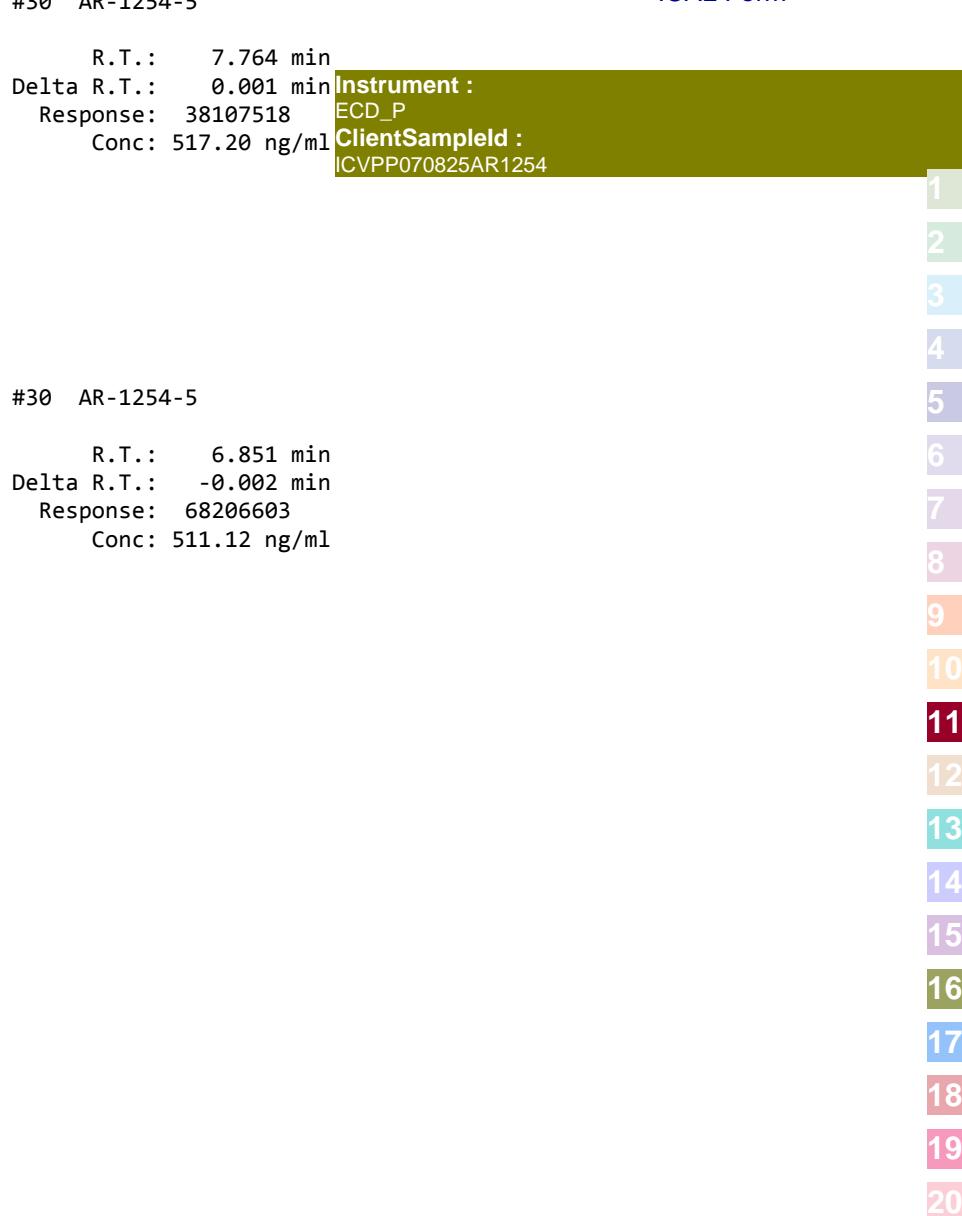

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP070825\
 Data File : PP073586.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jul 2025 06:52
 Operator : YP\AJ
 Sample : AR1268ICV500
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
ICVPP070825AR1268

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 08 08:27:27 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 08 08:22:37 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	4.484	3.778	70596120	97414683	50.662	50.893
2) SA Decachlor...	10.172	8.779	103.0E6	129.1E6	51.291	51.524

Target Compounds

41) L9 AR-1268-1	8.689	7.667	113.4E6	151.6E6	508.169	493.340
42) L9 AR-1268-2	8.781	7.734	97840395	131.8E6	513.584	495.942
43) L9 AR-1268-3	9.010	7.935	83760936	112.1E6	505.877	496.950
44) L9 AR-1268-4	9.426	8.229	34884334	47107861	501.616	506.711
45) L9 AR-1268-5	9.837	8.525	236.8E6	312.0E6	513.720	506.004


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.





Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP070825\
 Data File : PP073586.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jul 2025 06:52
 Operator : YP\AJ
 Sample : AR1268ICV500
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
ICVPP070825AR1268

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 08 08:27:27 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 08 08:22:37 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

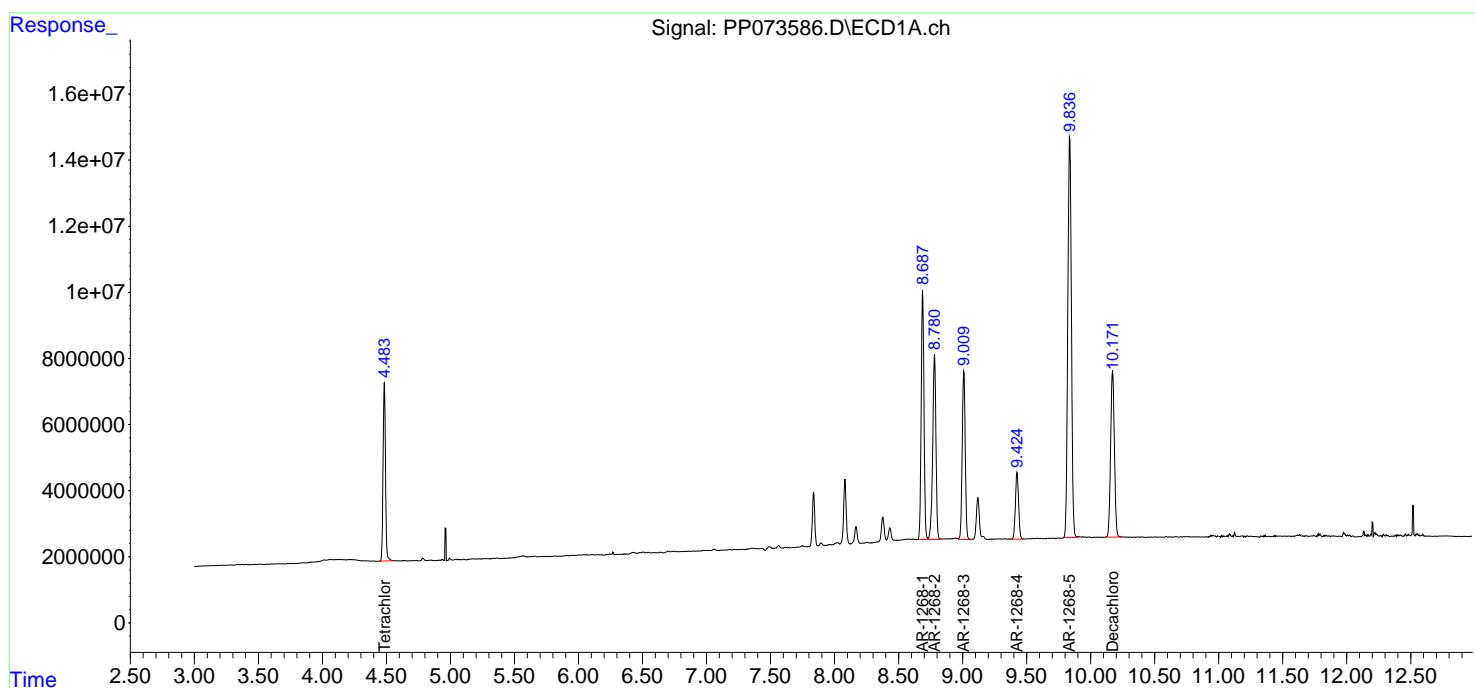

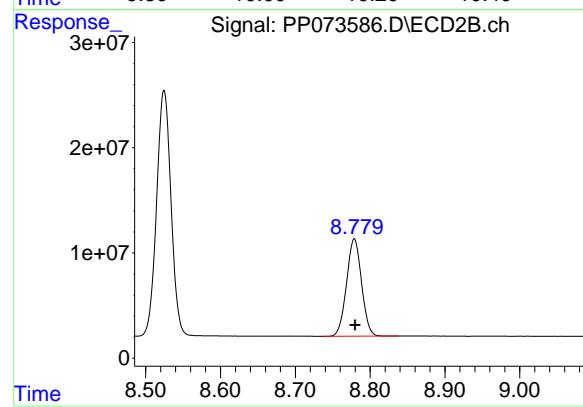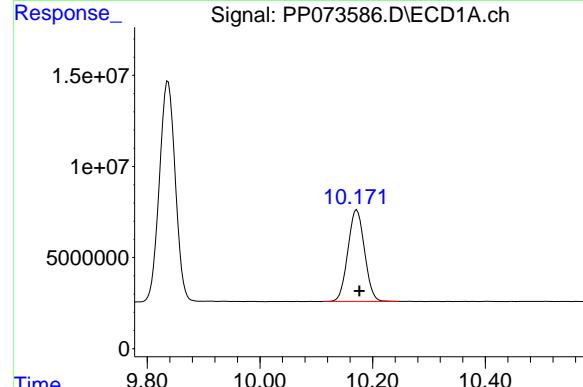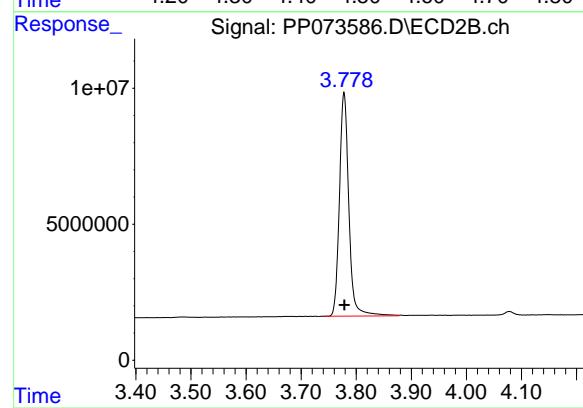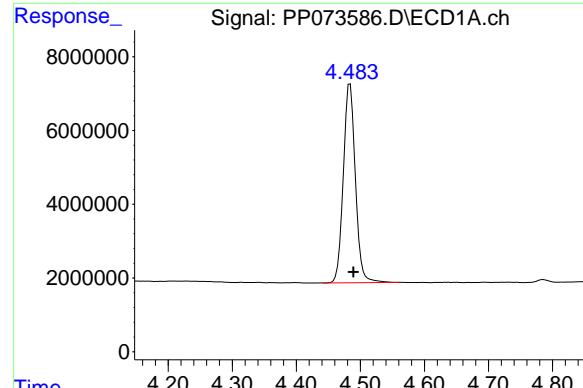

#1 Tetrachloro-m-xylene

R.T.: 4.484 min
 Delta R.T.: -0.005 min
 Response: 70596120
 Conc: 50.66 ng/ml

Instrument: ECD_P
ClientSampleId: ICVPP070825AR1268

#1 Tetrachloro-m-xylene





R.T.: 3.778 min
 Delta R.T.: 0.000 min
 Response: 97414683
 Conc: 50.89 ng/ml

#2 Decachlorobiphenyl

R.T.: 10.172 min
 Delta R.T.: -0.005 min
 Response: 102995358
 Conc: 51.29 ng/ml

#2 Decachlorobiphenyl

R.T.: 8.779 min
 Delta R.T.: -0.001 min
 Response: 129091204
 Conc: 51.52 ng/ml

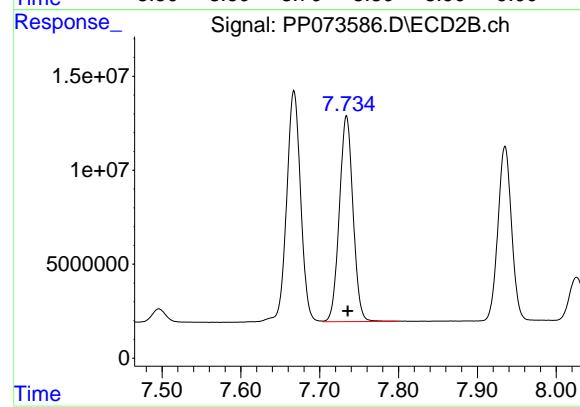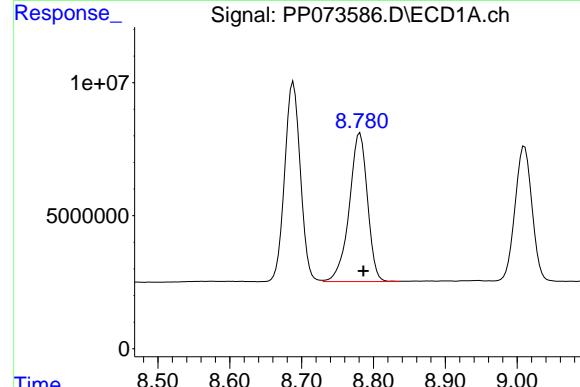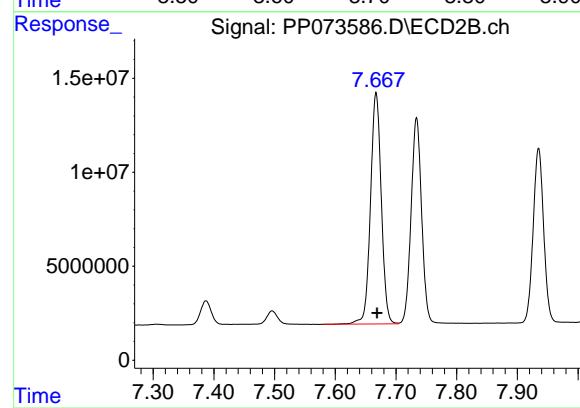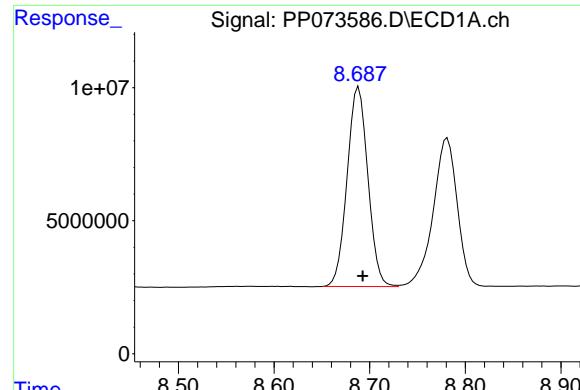

#41 AR-1268-1

R.T.: 8.689 min
 Delta R.T.: -0.004 min
 Response: 113435388
 Conc: 508.17 ng/ml

Instrument: ECD_P
ClientSampleId: ICVPP070825AR1268

#41 AR-1268-1

R.T.: 7.667 min
 Delta R.T.: -0.002 min
 Response: 151641353
 Conc: 493.34 ng/ml

#42 AR-1268-2

R.T.: 8.781 min
 Delta R.T.: -0.005 min
 Response: 97840395
 Conc: 513.58 ng/ml





#42 AR-1268-2

R.T.: 7.734 min
 Delta R.T.: -0.001 min
 Response: 131765701
 Conc: 495.94 ng/ml

#43 AR-1268-3

R.T.: 9.010 min
 Delta R.T.: -0.004 min
 Response: 83760936
 Conc: 505.88 ng/ml

Instrument: ECD_P
ClientSampleId: ICVPP070825AR1268

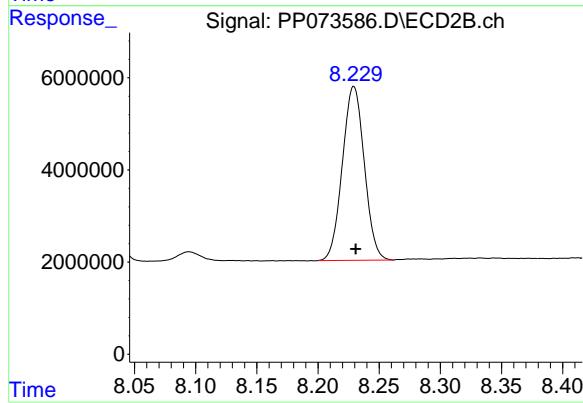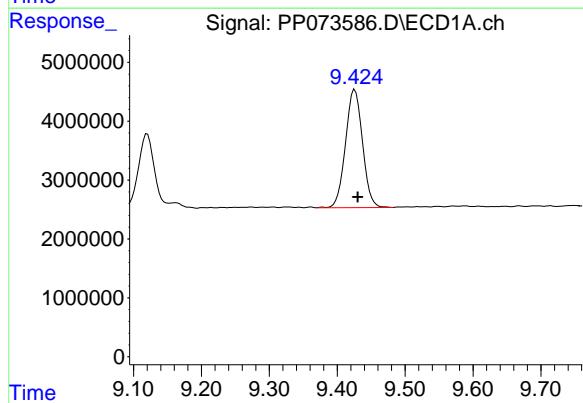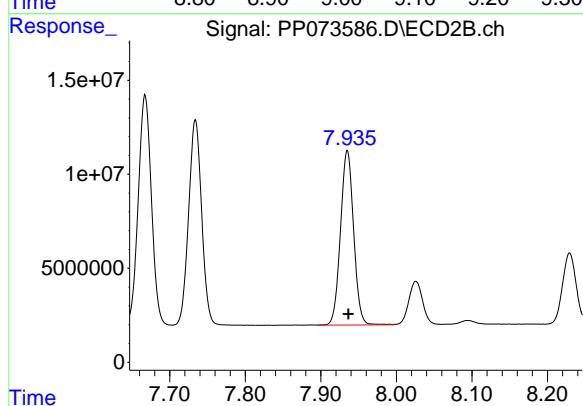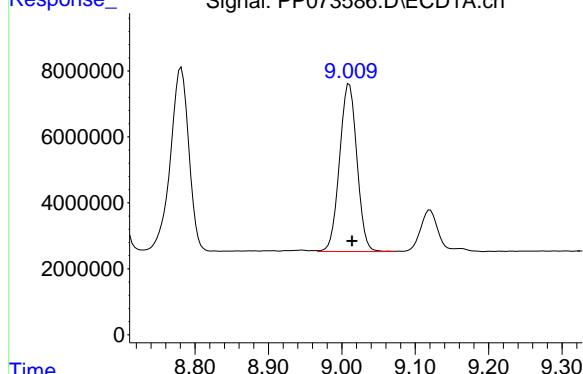

#43 AR-1268-3

R.T.: 7.935 min
 Delta R.T.: -0.002 min
 Response: 112102210
 Conc: 496.95 ng/ml

#44 AR-1268-4

R.T.: 9.426 min
 Delta R.T.: -0.004 min
 Response: 34884334
 Conc: 501.62 ng/ml



#44 AR-1268-4

R.T.: 8.229 min
 Delta R.T.: -0.002 min
 Response: 47107861
 Conc: 506.71 ng/ml

#45 AR-1268-5

R.T.: 9.837 min
Delta R.T.: -0.004 min
Response: 236804938
Conc: 513.72 ng/ml

Instrument: ECD_P
ClientSampleId: ICVPP070825AR1268

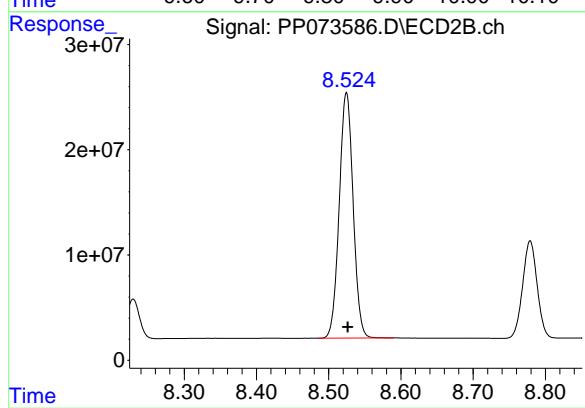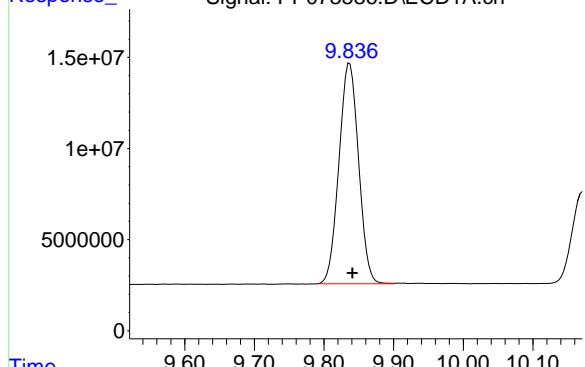

#45 AR-1268-5

R.T.: 8.525 min
Delta R.T.: -0.002 min
Response: 311977174
Conc: 506.00 ng/ml



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Lab Name: Alliance

Contract: NOBI03

Lab Code: ACE

SDG NO.: Q2639

Continuing Calib Date: 07/21/2025

Initial Calibration Date(s): 07/08/2025

07/08/2025

Continuing Calib Time: 10:15

Initial Calibration Time(s): 14:06

22:16

GC Column: ZB-MR1

ID: 0.32 (mm)

COMPOUND	CCAL RT	Avg RT	RT Window From	TO	Diff RT
Aroclor-1016-1 (1)	4.76	4.76	4.66	4.86	0.00
Aroclor-1016-2 (2)	4.78	4.78	4.68	4.88	0.00
Aroclor-1016-3 (3)	4.83	4.84	4.74	4.94	0.01
Aroclor-1016-4 (4)	4.95	4.96	4.86	5.06	0.01
Aroclor-1016-5 (5)	5.21	5.21	5.11	5.31	0.00
Aroclor-1260-1 (1)	6.25	6.25	6.15	6.35	0.00
Aroclor-1260-2 (2)	6.44	6.44	6.34	6.54	0.00
Aroclor-1260-3 (3)	6.80	6.81	6.71	6.91	0.01
Aroclor-1260-4 (4)	7.06	7.07	6.97	7.17	0.01
Aroclor-1260-5 (5)	7.31	7.31	7.21	7.41	0.00
Tetrachloro-m-xylene	3.67	3.67	3.57	3.77	0.00
Decachlorobiphenyl	8.70	8.70	8.60	8.80	0.00



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Lab Name: Alliance

Contract: NOBI03

Lab Code: ACE

SDG NO.: Q2639

Continuing Calib Date: 07/21/2025

Initial Calibration Date(s): 07/08/2025

07/08/2025

Continuing Calib Time: 10:15

Initial Calibration Time(s): 14:06

22:16

GC Column: ZB-MR2

ID: 0.32 (mm)

COMPOUND	CCAL RT	Avg RT	RT Window From	TO	Diff RT
Aroclor-1016-1 (1)	4.74	4.76	4.66	4.86	0.02
Aroclor-1016-2 (2)	4.76	4.78	4.68	4.88	0.02
Aroclor-1016-3 (3)	4.93	4.95	4.85	5.05	0.02
Aroclor-1016-4 (4)	4.98	5.00	4.90	5.10	0.03
Aroclor-1016-5 (5)	5.19	5.21	5.11	5.31	0.02
Aroclor-1260-1 (1)	6.22	6.24	6.14	6.34	0.02
Aroclor-1260-2 (2)	6.40	6.43	6.33	6.53	0.03
Aroclor-1260-3 (3)	6.56	6.58	6.48	6.68	0.02
Aroclor-1260-4 (4)	7.03	7.05	6.95	7.15	0.02
Aroclor-1260-5 (5)	7.27	7.29	7.19	7.39	0.02
Tetrachloro-m-xylene	3.66	3.68	3.58	3.78	0.02
Decachlorobiphenyl	8.65	8.67	8.57	8.77	0.02



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900, Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Lab Name:	<u>Alliance</u>	Contract:	<u>NOBI03</u>
Lab Code:	<u>ACE</u>	SDG NO.:	<u>Q2639</u>
GC Column:	<u>ZB-MR1</u>	ID: <u>0.32</u> (mm)	Initi. Calib. Date(s): <u>07/08/2025</u> <u>07/08/2025</u>

Client Sample No.:	<u>CCAL01</u>	Date Analyzed:	<u>07/21/2025</u>
Lab Sample No.:	<u>AR1660CCC500</u>	Data File :	<u>PO112332.D</u>
		Time Analyzed:	<u>10:15</u>

COMPOUND	RT	RT WINDOW FROM	TO	CALC AMOUNT(ng)	NOM AMOUNT(ng)	%D
Aroclor-1016-1	4.757	4.661	4.861	557.420	500.000	11.5
Aroclor-1016-2	4.776	4.680	4.880	558.820	500.000	11.8
Aroclor-1016-3	4.833	4.736	4.936	540.410	500.000	8.1
Aroclor-1016-4	4.953	4.856	5.056	557.830	500.000	11.6
Aroclor-1016-5	5.210	5.113	5.313	536.030	500.000	7.2
Aroclor-1260-1	6.247	6.151	6.351	512.290	500.000	2.5
Aroclor-1260-2	6.437	6.341	6.541	503.430	500.000	0.7
Aroclor-1260-3	6.804	6.707	6.907	494.730	500.000	-1.1
Aroclor-1260-4	7.063	6.967	7.167	504.090	500.000	0.8
Aroclor-1260-5	7.307	7.209	7.409	490.290	500.000	-1.9
Decachlorobiphenyl	8.699	8.603	8.803	47.230	50.000	-5.5
Tetrachloro-m-xylene	3.670	3.573	3.773	59.910	50.000	19.8



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900, Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Lab Name:	<u>Alliance</u>	Contract:	<u>NOBI03</u>
Lab Code:	<u>ACE</u>	SDG NO.:	<u>Q2639</u>
GC Column:	<u>ZB-MR2</u>	ID: <u>0.32</u> (mm)	Initi. Calib. Date(s): <u>07/08/2025</u> <u>07/08/2025</u>

Client Sample No.:	<u>CCAL01</u>	Date Analyzed:	<u>07/21/2025</u>
Lab Sample No.:	<u>AR1660CCC500</u>	Data File :	<u>PO112332.D</u>
		Time Analyzed:	<u>10:15</u>

COMPOUND	RT	RT WINDOW FROM	TO	CALC AMOUNT(ng)	NOM AMOUNT(ng)	%D
Aroclor-1016-1	4.738	4.661	4.861	497.080	500.000	-0.6
Aroclor-1016-2	4.757	4.679	4.879	506.560	500.000	1.3
Aroclor-1016-3	4.932	4.854	5.054	517.340	500.000	3.5
Aroclor-1016-4	4.975	4.897	5.097	523.900	500.000	4.8
Aroclor-1016-5	5.187	5.109	5.309	527.390	500.000	5.5
Aroclor-1260-1	6.216	6.138	6.338	494.430	500.000	-1.1
Aroclor-1260-2	6.404	6.326	6.526	498.700	500.000	-0.3
Aroclor-1260-3	6.556	6.478	6.678	493.670	500.000	-1.3
Aroclor-1260-4	7.026	6.948	7.148	448.420	500.000	-10.3
Aroclor-1260-5	7.268	7.190	7.390	436.750	500.000	-12.7
Decachlorobiphenyl	8.645	8.568	8.768	44.140	50.000	-11.7
Tetrachloro-m-xylene	3.663	3.584	3.784	54.830	50.000	9.7

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0072125\
 Data File : P0112332.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jul 2025 10:15
 Operator : YP/AJ
 Sample : AR1660CCC500
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1660CCC500

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/22/2025
 Supervised By :mohammad ahmed 07/23/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 22 09:15:16 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 22 09:14:26 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	3.670	3.663	592.8E6	349.3E6	59.914	54.828
2) SA Decachlor...	8.699	8.645	322.9E6	76065272	47.232	44.135

Target Compounds

3) L1 AR-1016-1	4.757	4.738	189.6E6	110.8E6	557.415	497.080m
4) L1 AR-1016-2	4.776	4.757	277.9E6	166.7E6	558.822	506.563m
5) L1 AR-1016-3	4.833	4.932	174.9E6	87879007	540.411	517.341m
6) L1 AR-1016-4	4.953	4.975	143.2E6	71893820	557.827	523.902m
7) L1 AR-1016-5	5.210	5.187	146.7E6	90948860	536.029	527.392m
31) L7 AR-1260-1	6.247	6.216	256.8E6	138.7E6	512.292	494.432
32) L7 AR-1260-2	6.437	6.404	371.6E6	169.6E6	503.427	498.705
33) L7 AR-1260-3	6.804	6.556	324.3E6	136.0E6	494.727	493.674m
34) L7 AR-1260-4	7.063	7.026	219.4E6	89972946	504.087	448.419m
35) L7 AR-1260-5	7.307	7.268	619.0E6	195.5E6	490.290	436.745

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0072125\
 Data File : P0112332.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jul 2025 10:15
 Operator : YP/AJ
 Sample : AR1660CCC500
 Misc :
 ALS Vial : 3 Sample Multiplier: 1



Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 22 09:15:16 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 22 09:14:26 2025
 Response via : Initial Calibration
 Integrator: ChemStation


Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Instrument :
 ECD_O
 ClientSampleId :
 AR1660CCC500

Manual Integrations APPROVED

Reviewed By :Yogesh Patel 07/22/2025
 Supervised By :mohammad ahmed 07/23/2025

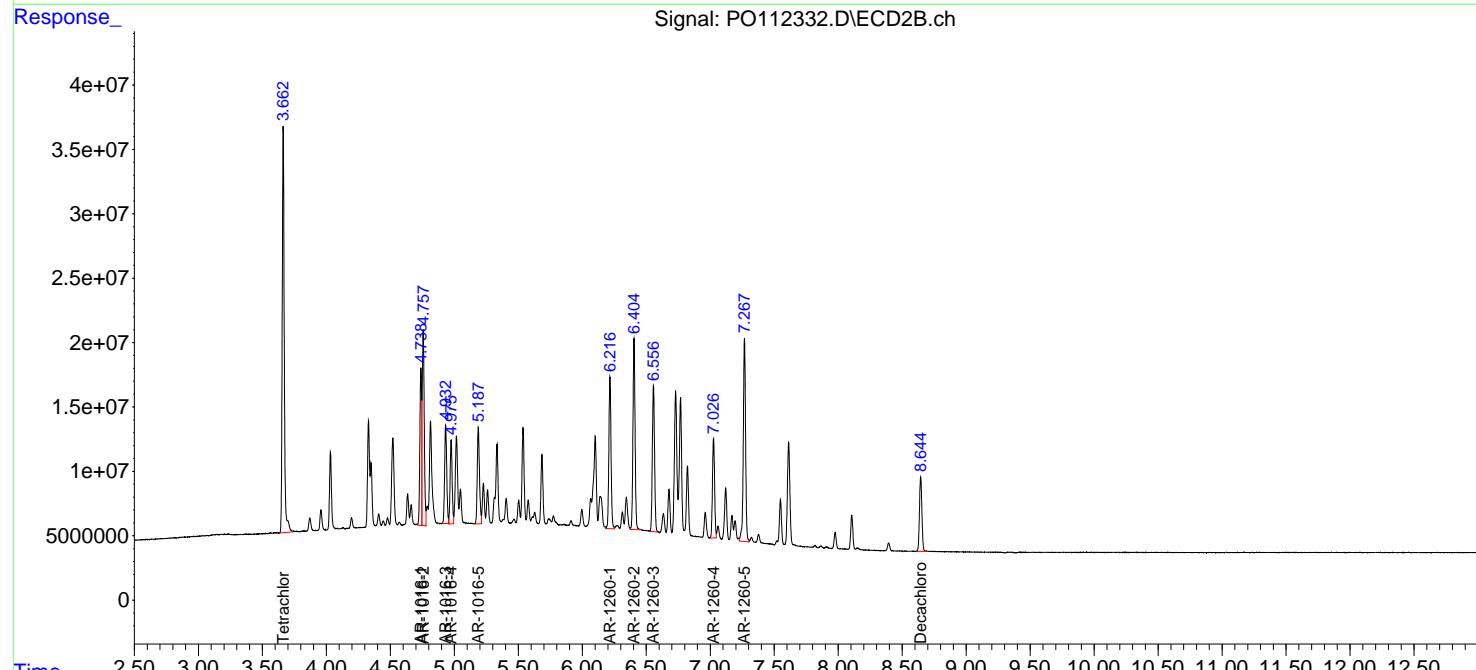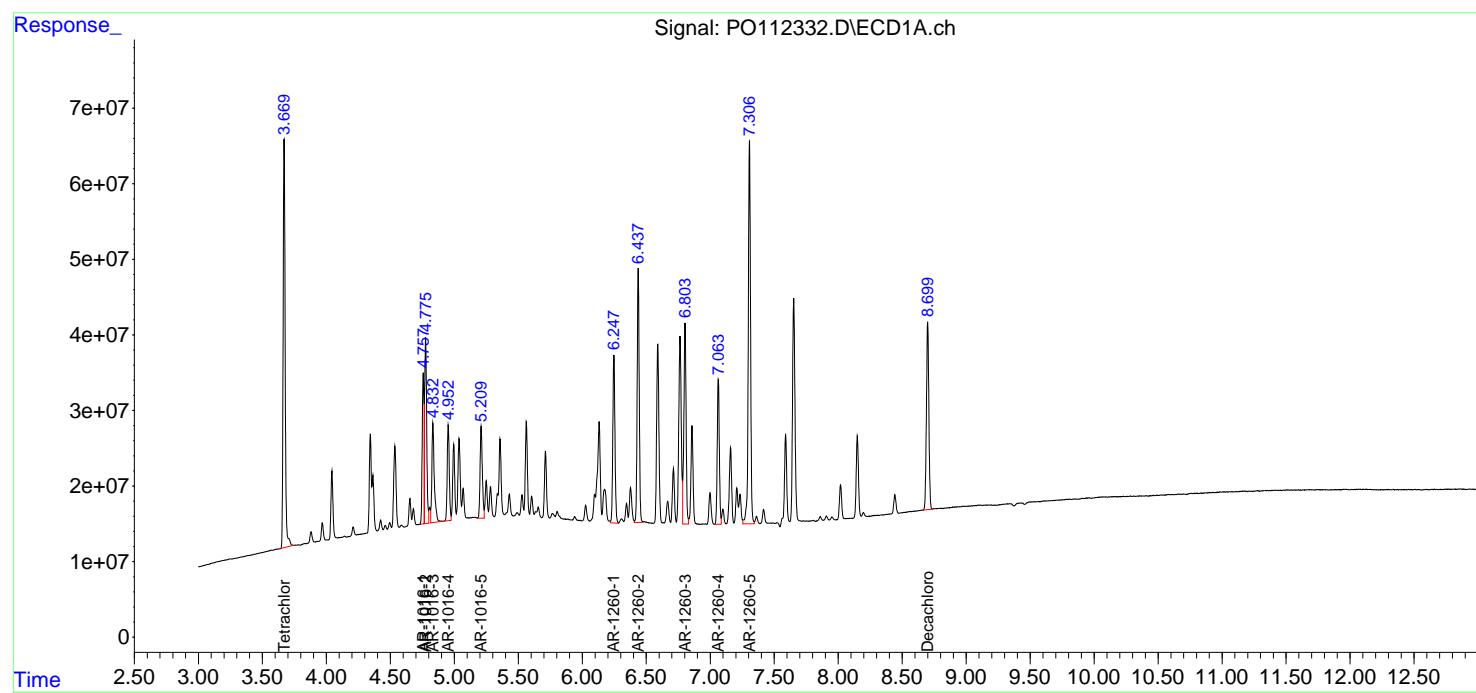

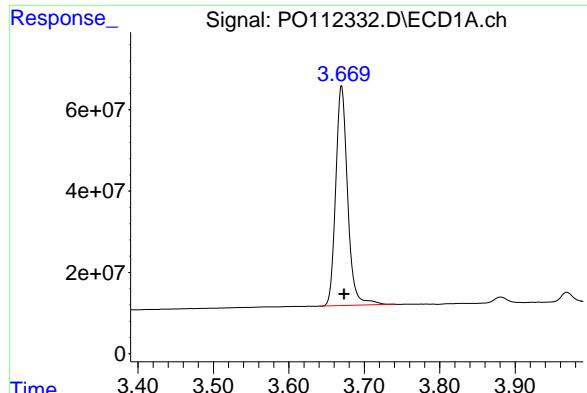


#1 Tetrachloro-m-xylene

R.T.: 3.670 min
Delta R.T.: -0.003 min
Response: 592831825
Conc: 59.91 ng/ml

Instrument: ECD_O
ClientSampleId: AR1660CCC500


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/22/2025
Supervised By :mohammad ahmed 07/23/2025

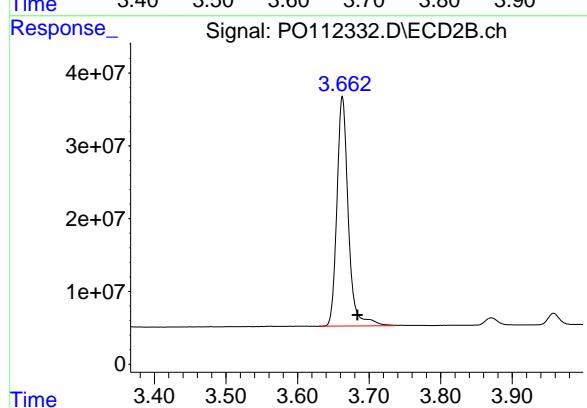


#1 Tetrachloro-m-xylene

R.T.: 3.663 min
Delta R.T.: -0.021 min
Response: 349312435
Conc: 54.83 ng/ml

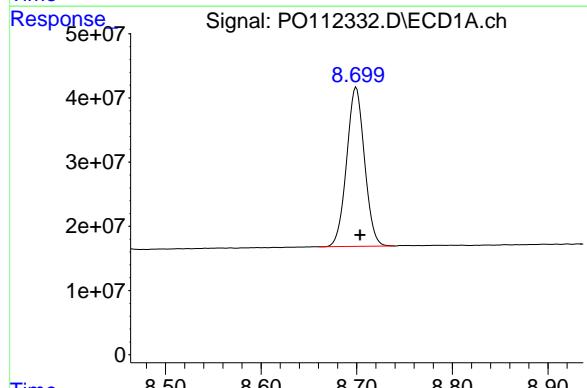


#2 Decachlorobiphenyl

R.T.: 8.699 min
Delta R.T.: -0.004 min
Response: 322926705
Conc: 47.23 ng/ml

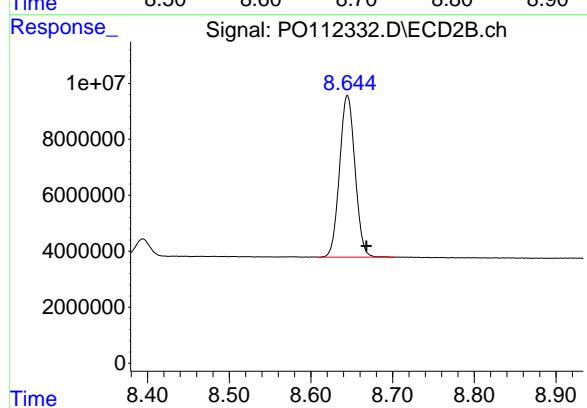

#2 Decachlorobiphenyl

R.T.: 8.645 min
Delta R.T.: -0.023 min
Response: 76065272
Conc: 44.14 ng/ml

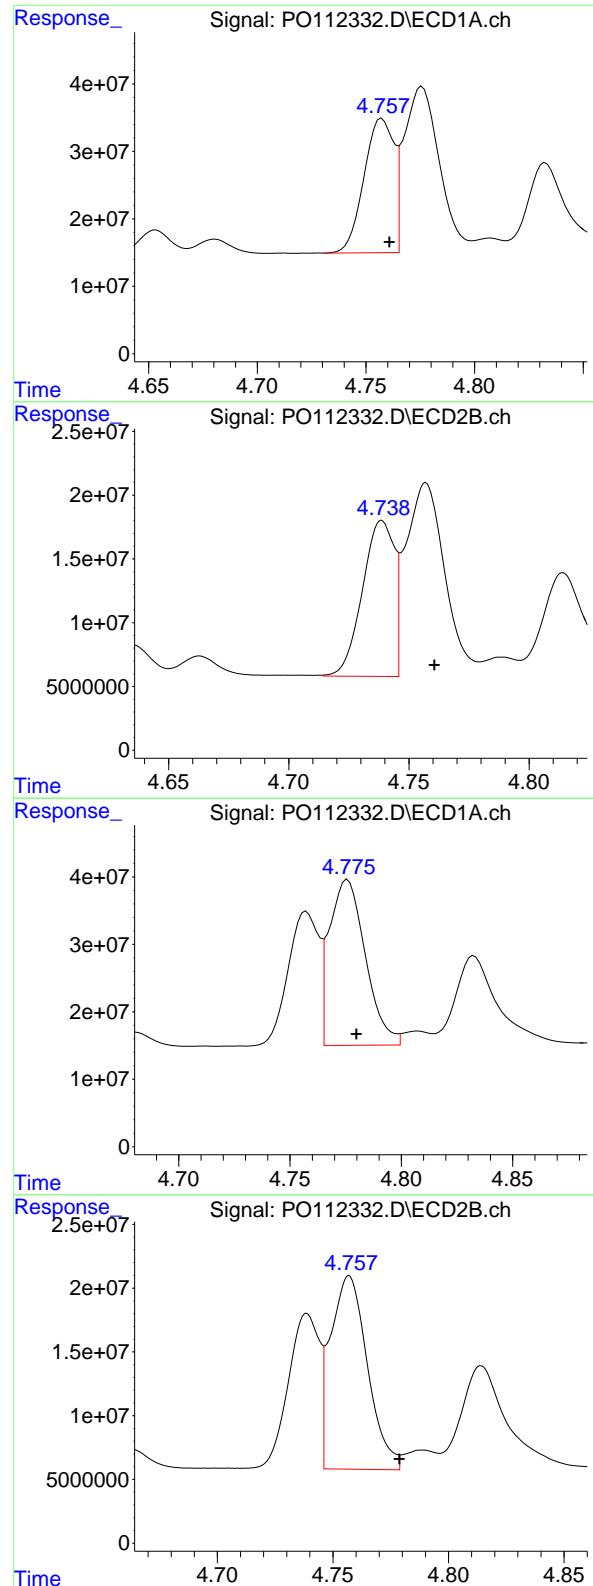

#3 AR-1016-1

R.T.: 4.757 min
 Delta R.T.: -0.003 min
 Response: 189589630
 Conc: 557.42 ng/ml

Instrument: ECD_O
 ClientSampleId: AR1660CCC500

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/22/2025
 Supervised By :mohammad ahmed 07/23/2025

#3 AR-1016-1


R.T.: 4.738 min
 Delta R.T.: -0.022 min
 Response: 110766571
 Conc: 497.08 ng/ml

#4 AR-1016-2

R.T.: 4.776 min
 Delta R.T.: -0.004 min
 Response: 277897665
 Conc: 558.82 ng/ml

#4 AR-1016-2

R.T.: 4.757 min
 Delta R.T.: -0.022 min
 Response: 166708517
 Conc: 506.56 ng/ml

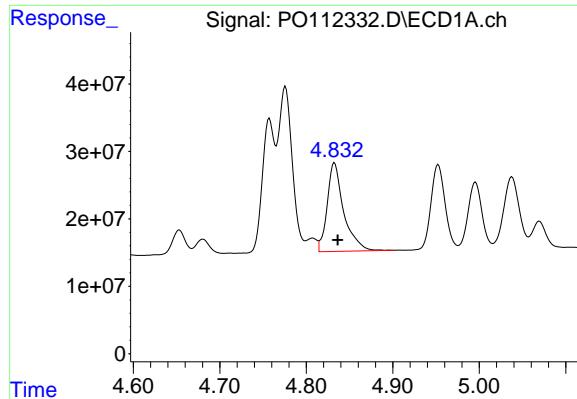


#5 AR-1016-3

R.T.: 4.833 min
Delta R.T.: -0.004 min
Response: 174938598
Conc: 540.41 ng/ml

Instrument: ECD_O
ClientSampleId: AR1660CCC500


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/22/2025
Supervised By :mohammad ahmed 07/23/2025

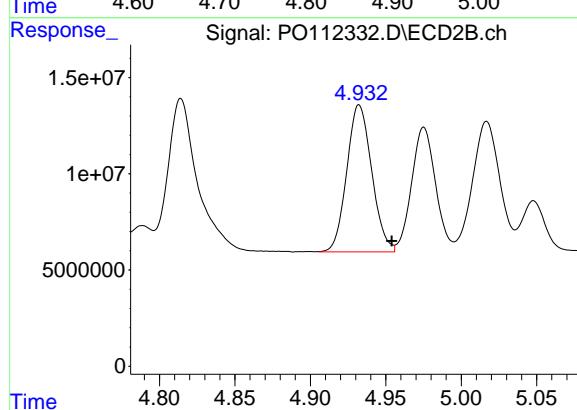


#5 AR-1016-3

R.T.: 4.932 min
Delta R.T.: -0.022 min
Response: 87879007
Conc: 517.34 ng/ml

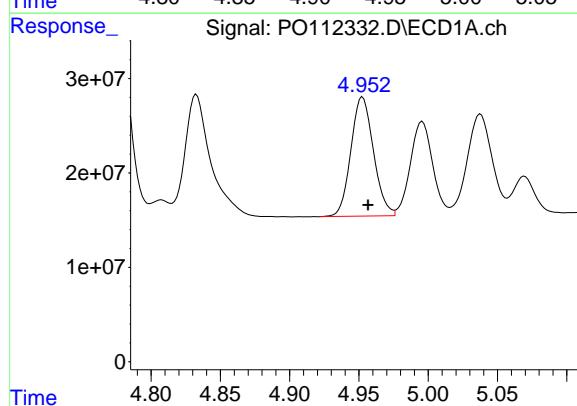





#6 AR-1016-4

R.T.: 4.953 min
Delta R.T.: -0.004 min
Response: 143249651
Conc: 557.83 ng/ml

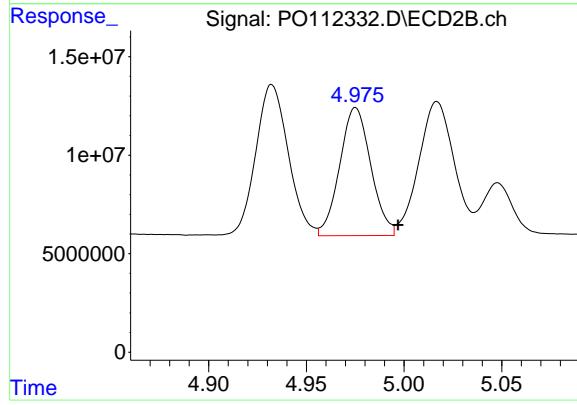

#6 AR-1016-4

R.T.: 4.975 min
Delta R.T.: -0.022 min
Response: 71893820
Conc: 523.90 ng/ml

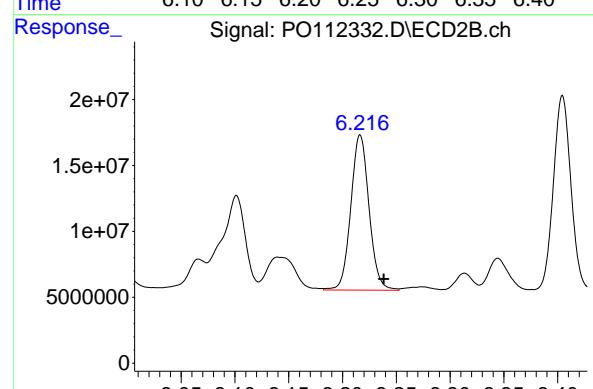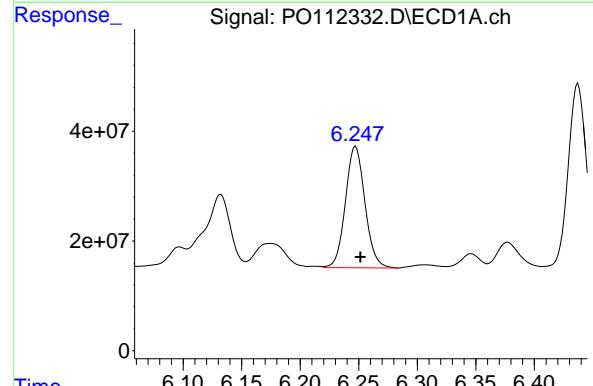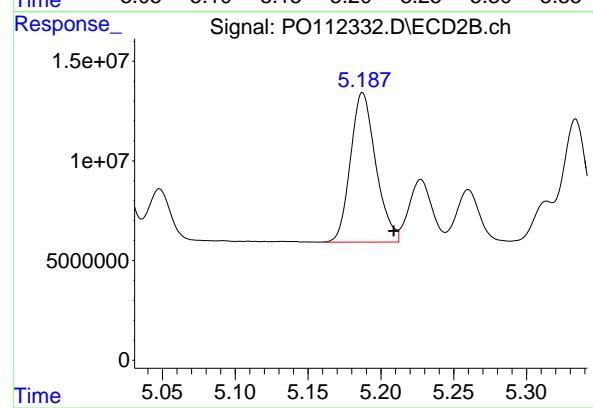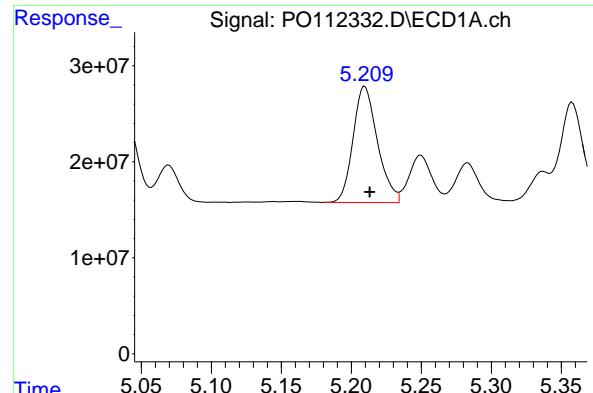





#7 AR-1016-5

R.T.: 5.210 min
 Delta R.T.: -0.004 min
 Response: 146690723
 Conc: 536.03 ng/ml

Instrument: ECD_O
 ClientSampleId: AR1660CCC500

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/22/2025
 Supervised By :mohammad ahmed 07/23/2025

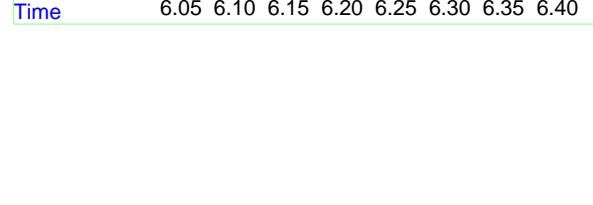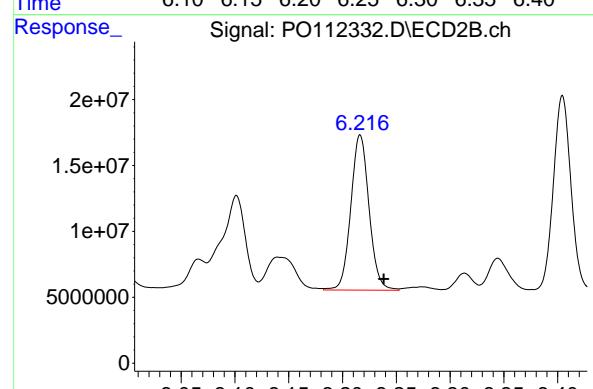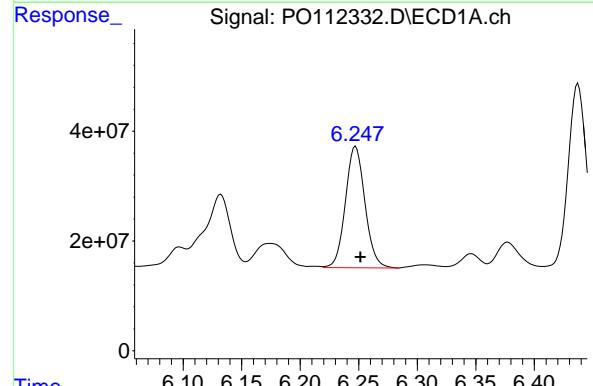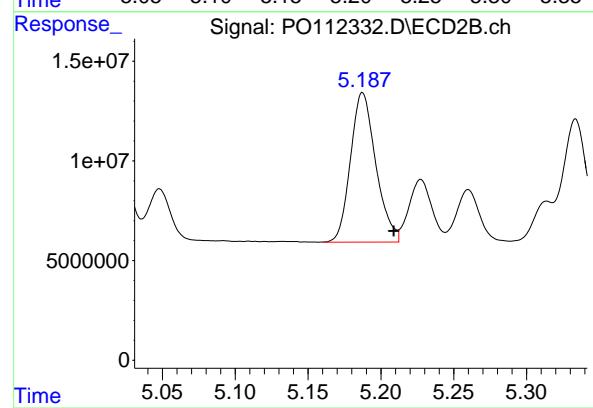

#32 AR-1260-2

R.T.: 6.437 min
 Delta R.T.: -0.003 min
 Response: 371597084
 Conc: 503.43 ng/ml

Instrument: ECD_O
ClientSampleId: AR1660CCC500

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/22/2025
 Supervised By :mohammad ahmed 07/23/2025

#32 AR-1260-2





R.T.: 6.404 min
 Delta R.T.: -0.022 min
 Response: 169558040
 Conc: 498.70 ng/ml





#33 AR-1260-3

R.T.: 6.804 min
 Delta R.T.: -0.003 min
 Response: 324284745
 Conc: 494.73 ng/ml

#33 AR-1260-3

R.T.: 6.556 min
 Delta R.T.: -0.022 min
 Response: 136049690
 Conc: 493.67 ng/ml

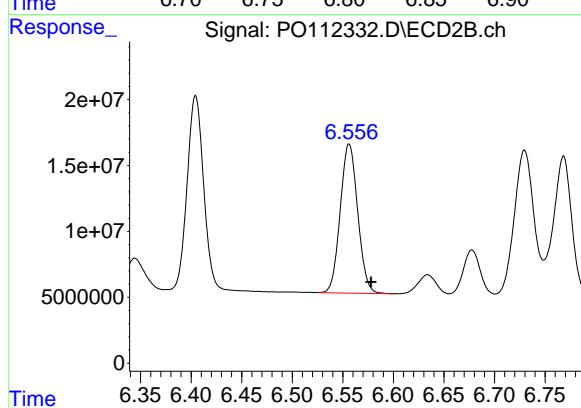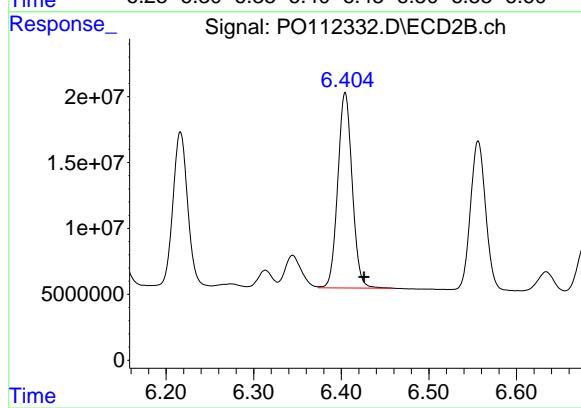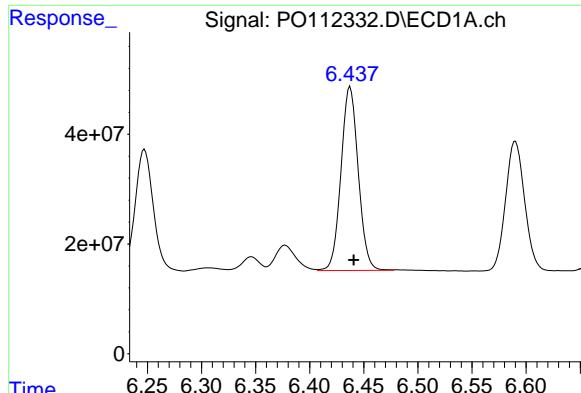

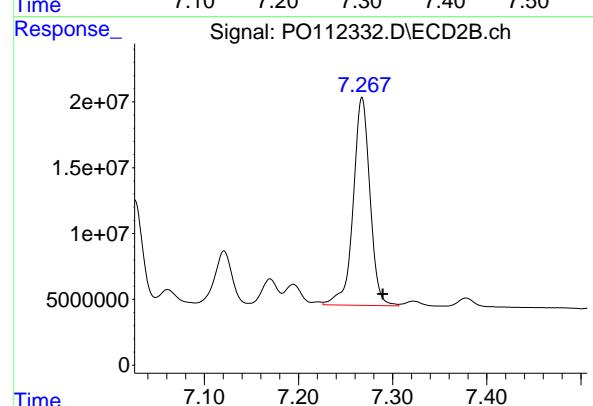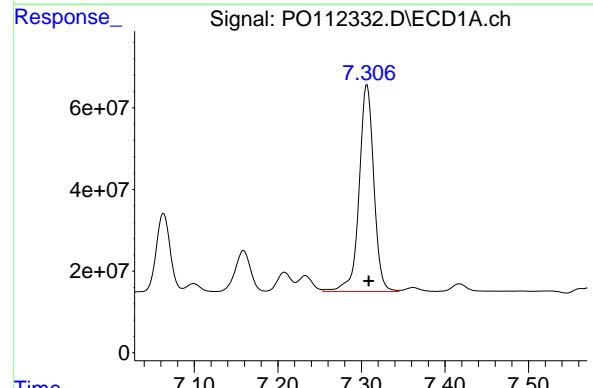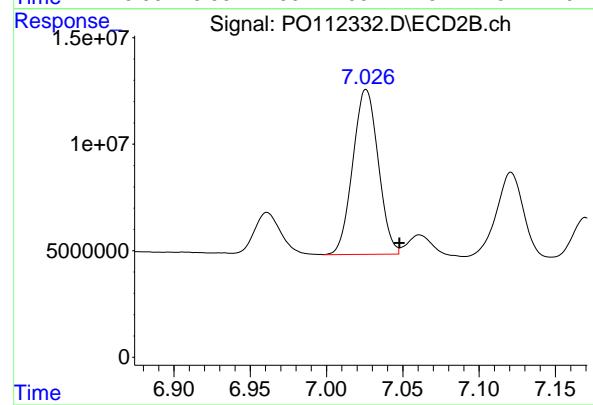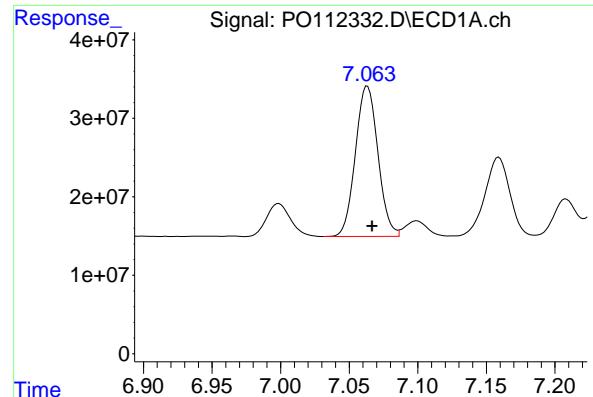

#34 AR-1260-4

R.T.: 7.063 min
Delta R.T.: -0.003 min
Response: 219402703
Conc: 504.09 ng/ml

Instrument: ECD_O
ClientSampleId: AR1660CCC500

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/22/2025
Supervised By :mohammad ahmed 07/23/2025

#34 AR-1260-4

R.T.: 7.026 min
Delta R.T.: -0.022 min
Response: 89972946
Conc: 448.42 ng/ml

#35 AR-1260-5

R.T.: 7.307 min
Delta R.T.: -0.002 min
Response: 619009807
Conc: 490.29 ng/ml

#35 AR-1260-5

R.T.: 7.268 min
Delta R.T.: -0.022 min
Response: 195543329
Conc: 436.75 ng/ml



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Lab Name: Alliance

Contract: NOBI03

Lab Code: ACE

SDG NO.: Q2639

Continuing Calib Date: 07/21/2025

Initial Calibration Date(s): 07/08/2025

07/08/2025

Continuing Calib Time: 16:10

Initial Calibration Time(s): 14:06

22:16

GC Column: ZB-MR1

ID: 0.32 (mm)

COMPOUND	CCAL RT	Avg RT	RT Window From	TO	Diff RT
Aroclor-1016-1 (1)	4.76	4.76	4.66	4.86	0.00
Aroclor-1016-2 (2)	4.77	4.78	4.68	4.88	0.01
Aroclor-1016-3 (3)	4.83	4.84	4.74	4.94	0.01
Aroclor-1016-4 (4)	4.95	4.96	4.86	5.06	0.01
Aroclor-1016-5 (5)	5.21	5.21	5.11	5.31	0.00
Aroclor-1260-1 (1)	6.25	6.25	6.15	6.35	0.01
Aroclor-1260-2 (2)	6.44	6.44	6.34	6.54	0.01
Aroclor-1260-3 (3)	6.80	6.81	6.71	6.91	0.01
Aroclor-1260-4 (4)	7.06	7.07	6.97	7.17	0.01
Aroclor-1260-5 (5)	7.30	7.31	7.21	7.41	0.01
Tetrachloro-m-xylene	3.67	3.67	3.57	3.77	0.00
Decachlorobiphenyl	8.70	8.70	8.60	8.80	0.00



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Lab Name: Alliance

Contract: NOBI03

Lab Code: ACE

SDG NO.: Q2639

Continuing Calib Date: 07/21/2025

Initial Calibration Date(s): 07/08/2025

07/08/2025

Continuing Calib Time: 16:10

Initial Calibration Time(s): 14:06

22:16

GC Column: ZB-MR2

ID: 0.32 (mm)

COMPOUND	CCAL RT	Avg RT	RT Window From	TO	Diff RT
Aroclor-1016-1 (1)	4.74	4.76	4.66	4.86	0.02
Aroclor-1016-2 (2)	4.76	4.78	4.68	4.88	0.02
Aroclor-1016-3 (3)	4.93	4.95	4.85	5.05	0.02
Aroclor-1016-4 (4)	4.97	5.00	4.90	5.10	0.03
Aroclor-1016-5 (5)	5.19	5.21	5.11	5.31	0.02
Aroclor-1260-1 (1)	6.22	6.24	6.14	6.34	0.02
Aroclor-1260-2 (2)	6.40	6.43	6.33	6.53	0.03
Aroclor-1260-3 (3)	6.56	6.58	6.48	6.68	0.03
Aroclor-1260-4 (4)	7.03	7.05	6.95	7.15	0.02
Aroclor-1260-5 (5)	7.27	7.29	7.19	7.39	0.02
Tetrachloro-m-xylene	3.66	3.68	3.58	3.78	0.02
Decachlorobiphenyl	8.65	8.67	8.57	8.77	0.02



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900, Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Lab Name:	Alliance	Contract:	NOBI03
Lab Code:	ACE	SDG NO.:	Q2639
GC Column:	ZB-MR1	ID: 0.32 (mm)	Initi. Calib. Date(s): 07/08/2025 07/08/2025

Client Sample No.:	CCAL02	Date Analyzed:	07/21/2025
Lab Sample No.:	AR1660CCC500	Data File :	PO112346.D
		Time Analyzed:	16:10

COMPOUND	RT	RT WINDOW FROM TO		CALC AMOUNT(ng)	NOM AMOUNT(ng)	%D
Aroclor-1016-1	4.755	4.661	4.861	493.200	500.000	-1.4
Aroclor-1016-2	4.774	4.680	4.880	504.490	500.000	0.9
Aroclor-1016-3	4.831	4.736	4.936	485.600	500.000	-2.9
Aroclor-1016-4	4.950	4.856	5.056	494.510	500.000	-1.1
Aroclor-1016-5	5.208	5.113	5.313	517.120	500.000	3.4
Aroclor-1260-1	6.245	6.151	6.351	450.880	500.000	-9.8
Aroclor-1260-2	6.435	6.341	6.541	453.990	500.000	-9.2
Aroclor-1260-3	6.801	6.707	6.907	449.210	500.000	-10.2
Aroclor-1260-4	7.061	6.967	7.167	455.120	500.000	-9.0
Aroclor-1260-5	7.304	7.209	7.409	444.970	500.000	-11.0
Decachlorobiphenyl	8.697	8.603	8.803	44.760	50.000	-10.5
Tetrachloro-m-xylene	3.669	3.573	3.773	53.590	50.000	7.2



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900, Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Lab Name:	Alliance	Contract:	NOBI03
Lab Code:	ACE	SDG NO.:	Q2639
GC Column:	ZB-MR2	ID: 0.32 (mm)	Initi. Calib. Date(s): 07/08/2025 07/08/2025

Client Sample No.:	CCAL02	Date Analyzed:	07/21/2025
Lab Sample No.:	AR1660CCC500	Data File :	PO112346.D
		Time Analyzed:	16:10

COMPOUND	RT	RT WINDOW FROM TO		CALC AMOUNT(ng)	NOM AMOUNT(ng)	%D
Aroclor-1016-1	4.738	4.661	4.861	440.050	500.000	-12.0
Aroclor-1016-2	4.757	4.679	4.879	439.280	500.000	-12.1
Aroclor-1016-3	4.931	4.854	5.054	457.420	500.000	-8.5
Aroclor-1016-4	4.974	4.897	5.097	450.520	500.000	-9.9
Aroclor-1016-5	5.186	5.109	5.309	472.360	500.000	-5.5
Aroclor-1260-1	6.215	6.138	6.338	447.760	500.000	-10.4
Aroclor-1260-2	6.404	6.326	6.526	468.060	500.000	-6.4
Aroclor-1260-3	6.555	6.478	6.678	465.510	500.000	-6.9
Aroclor-1260-4	7.025	6.948	7.148	436.340	500.000	-12.7
Aroclor-1260-5	7.268	7.190	7.390	459.070	500.000	-8.2
Decachlorobiphenyl	8.645	8.568	8.768	43.200	50.000	-13.6
Tetrachloro-m-xylene	3.663	3.584	3.784	49.080	50.000	-1.8

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0072125\
 Data File : P0112346.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jul 2025 16:10
 Operator : YP/AJ
 Sample : AR1660CCC500
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1660CCC500

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/22/2025
 Supervised By :mohammad ahmed 07/23/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 22 09:16:01 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 22 09:14:26 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	3.669	3.663	530.3E6	312.7E6	53.594	49.077
2) SA Decachlor...	8.697	8.645	306.0E6	74451617	44.762	43.199

Target Compounds

3) L1 AR-1016-1	4.755	4.738	167.7E6	98059177	493.201	440.054m
4) L1 AR-1016-2	4.774	4.757	250.9E6	144.6E6	504.494	439.278m
5) L1 AR-1016-3	4.831	4.931	157.2E6	77700801	485.598	457.422m
6) L1 AR-1016-4	4.950	4.974	127.0E6	61824314	494.505	450.524m
7) L1 AR-1016-5	5.208	5.186	141.5E6	81459246	517.122	472.364m
31) L7 AR-1260-1	6.245	6.215	226.0E6	125.6E6	450.876	447.762
32) L7 AR-1260-2	6.435	6.404	335.1E6	159.1E6	453.990	468.063
33) L7 AR-1260-3	6.801	6.555	294.4E6	128.3E6	449.209	465.505m
34) L7 AR-1260-4	7.061	7.025	198.1E6	87550066	455.117	436.343m
35) L7 AR-1260-5	7.304	7.268	561.8E6	205.5E6	444.971	459.066

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0072125\
 Data File : P0112346.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jul 2025 16:10
 Operator : YP/AJ
 Sample : AR1660CCC500
 Misc :
 ALS Vial : 3 Sample Multiplier: 1



Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 22 09:16:01 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 22 09:14:26 2025
 Response via : Initial Calibration
 Integrator: ChemStation


Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Instrument :
 ECD_O
 ClientSampleId :
 AR1660CCC500

Manual Integrations APPROVED

Reviewed By :Yogesh Patel 07/22/2025
 Supervised By :mohammad ahmed 07/23/2025

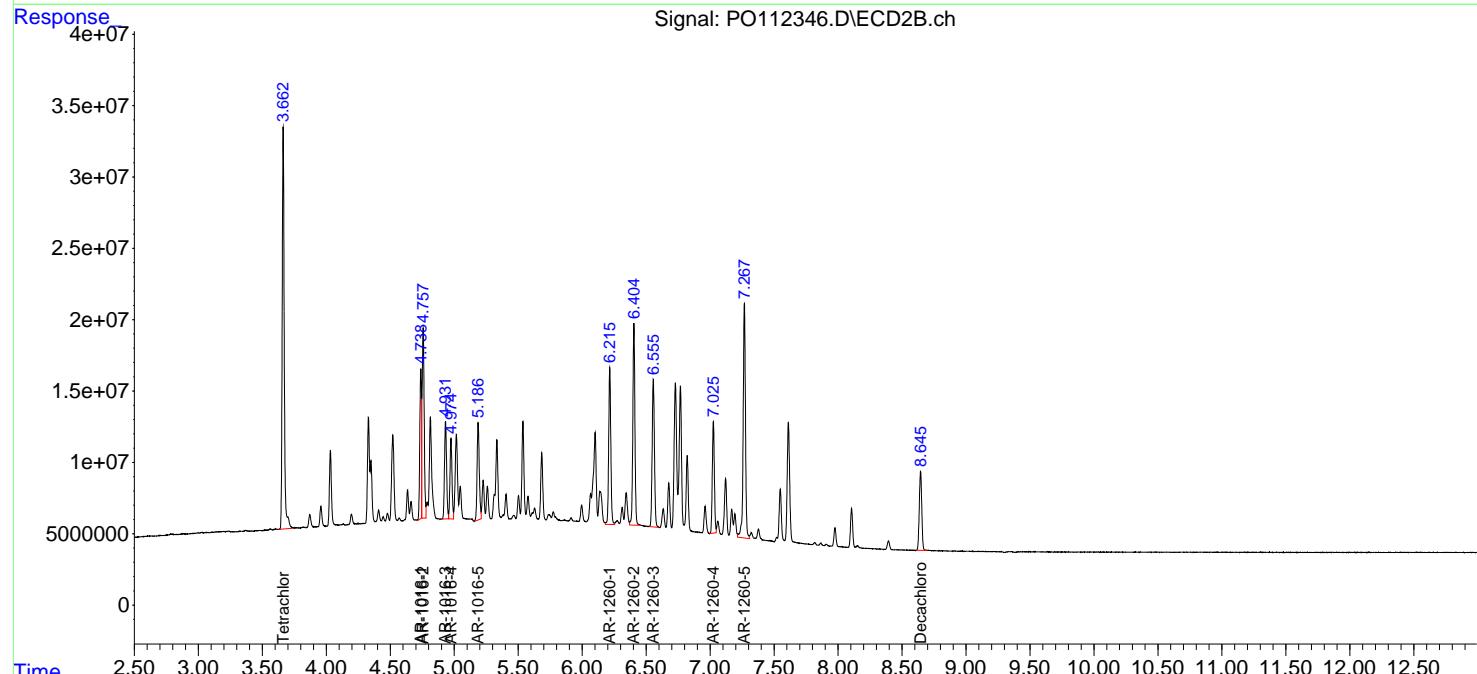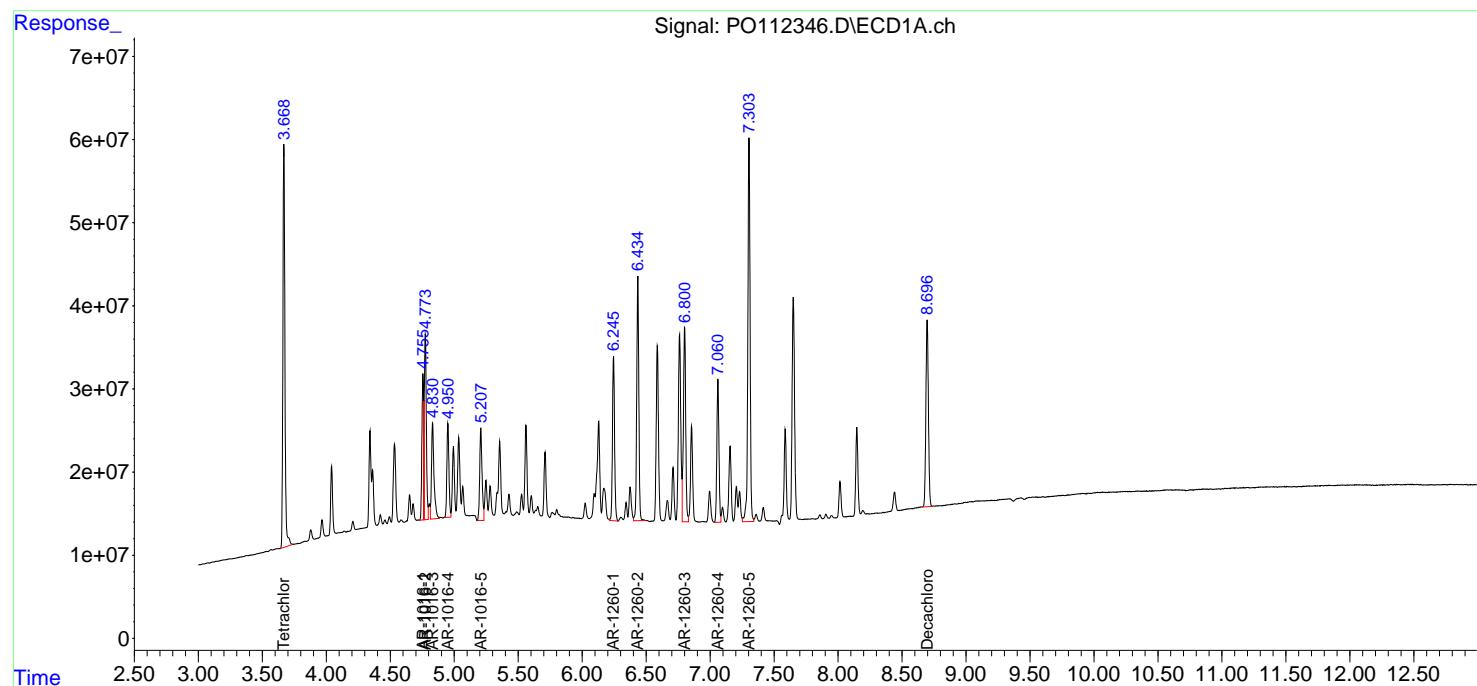

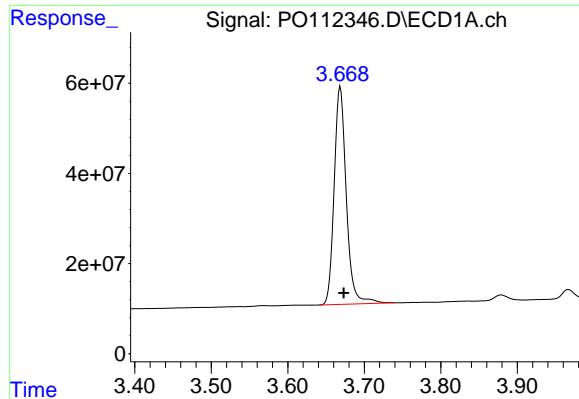


#1 Tetrachloro-m-xylene

R.T.: 3.669 min
Delta R.T.: -0.004 min
Response: 530299098
Conc: 53.59 ng/ml

Instrument: ECD_O
ClientSampleId: AR1660CCC500


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/22/2025
Supervised By :mohammad ahmed 07/23/2025

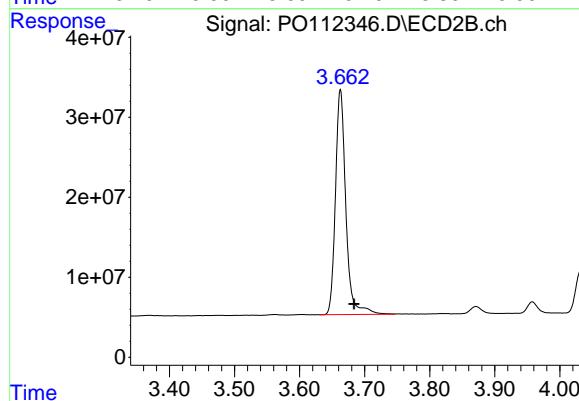


#1 Tetrachloro-m-xylene

R.T.: 3.663 min
Delta R.T.: -0.021 min
Response: 312671778
Conc: 49.08 ng/ml

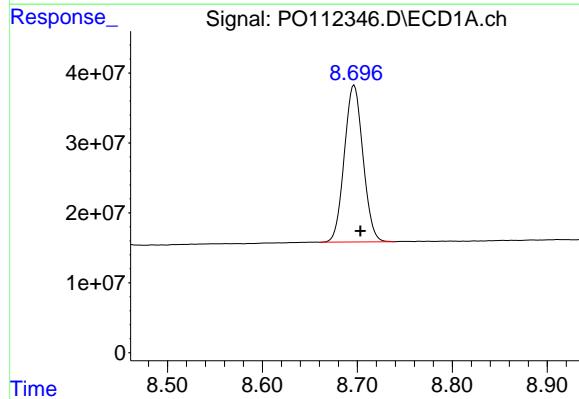


#2 Decachlorobiphenyl

R.T.: 8.697 min
Delta R.T.: -0.007 min
Response: 306036817
Conc: 44.76 ng/ml

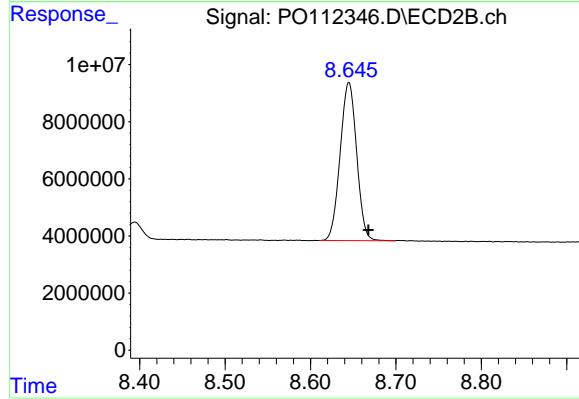

#2 Decachlorobiphenyl

R.T.: 8.645 min
Delta R.T.: -0.023 min
Response: 74451617
Conc: 43.20 ng/ml

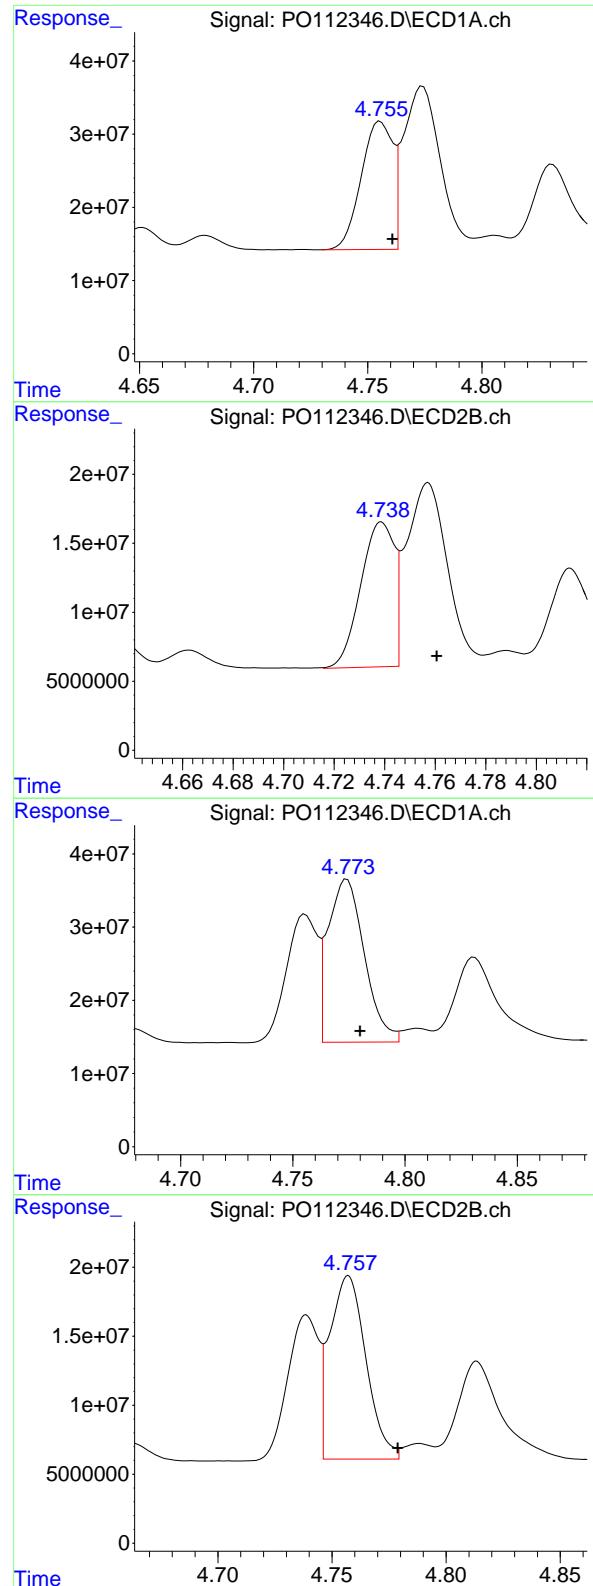

#3 AR-1016-1

R.T.: 4.755 min
 Delta R.T.: -0.005 min
 Response: 167749009
 Conc: 493.20 ng/ml

Instrument: ECD_O
 ClientSampleId: AR1660CCC500

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/22/2025
 Supervised By :mohammad ahmed 07/23/2025

#3 AR-1016-1


R.T.: 4.738 min
 Delta R.T.: -0.022 min
 Response: 98059177
 Conc: 440.05 ng/ml

#4 AR-1016-2

R.T.: 4.774 min
 Delta R.T.: -0.006 min
 Response: 250880622
 Conc: 504.49 ng/ml

#4 AR-1016-2

R.T.: 4.757 min
 Delta R.T.: -0.022 min
 Response: 144565183
 Conc: 439.28 ng/ml

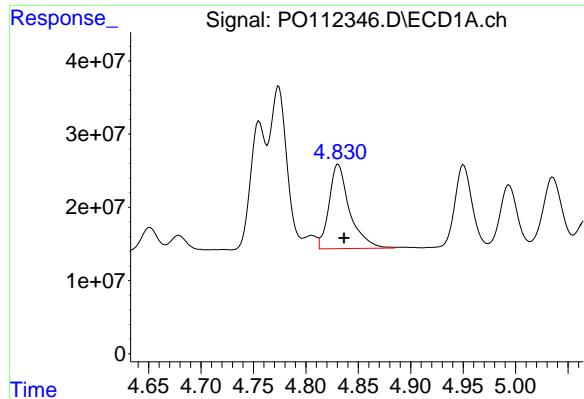


#5 AR-1016-3

R.T.: 4.831 min
Delta R.T.: -0.005 min
Response: 157194927
Conc: 485.60 ng/ml

Instrument: ECD_O
ClientSampleId: AR1660CCC500


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/22/2025
Supervised By :mohammad ahmed 07/23/2025

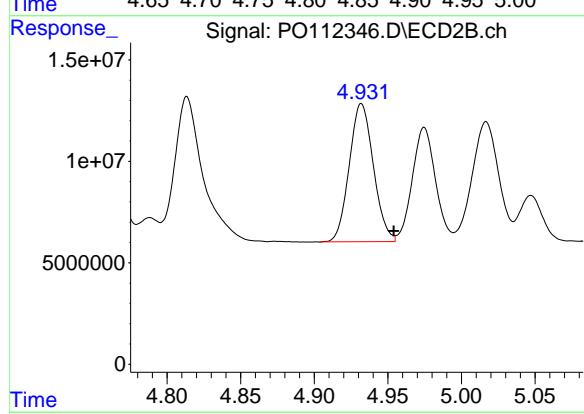


#5 AR-1016-3

R.T.: 4.931 min
Delta R.T.: -0.023 min
Response: 77700801
Conc: 457.42 ng/ml

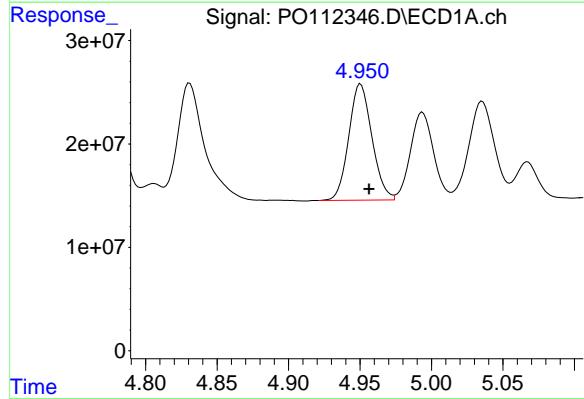


#6 AR-1016-4

R.T.: 4.950 min
Delta R.T.: -0.006 min
Response: 126988725
Conc: 494.51 ng/ml

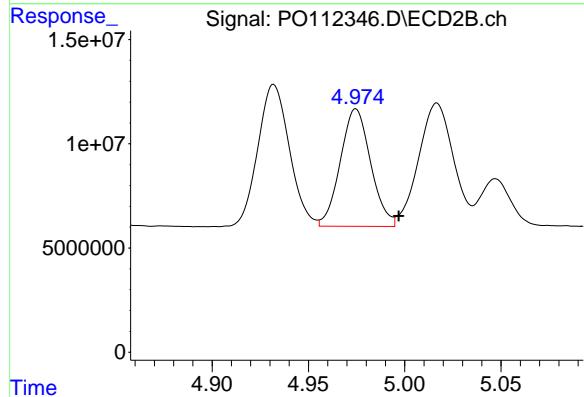

#6 AR-1016-4

R.T.: 4.974 min
Delta R.T.: -0.023 min
Response: 61824314
Conc: 450.52 ng/ml

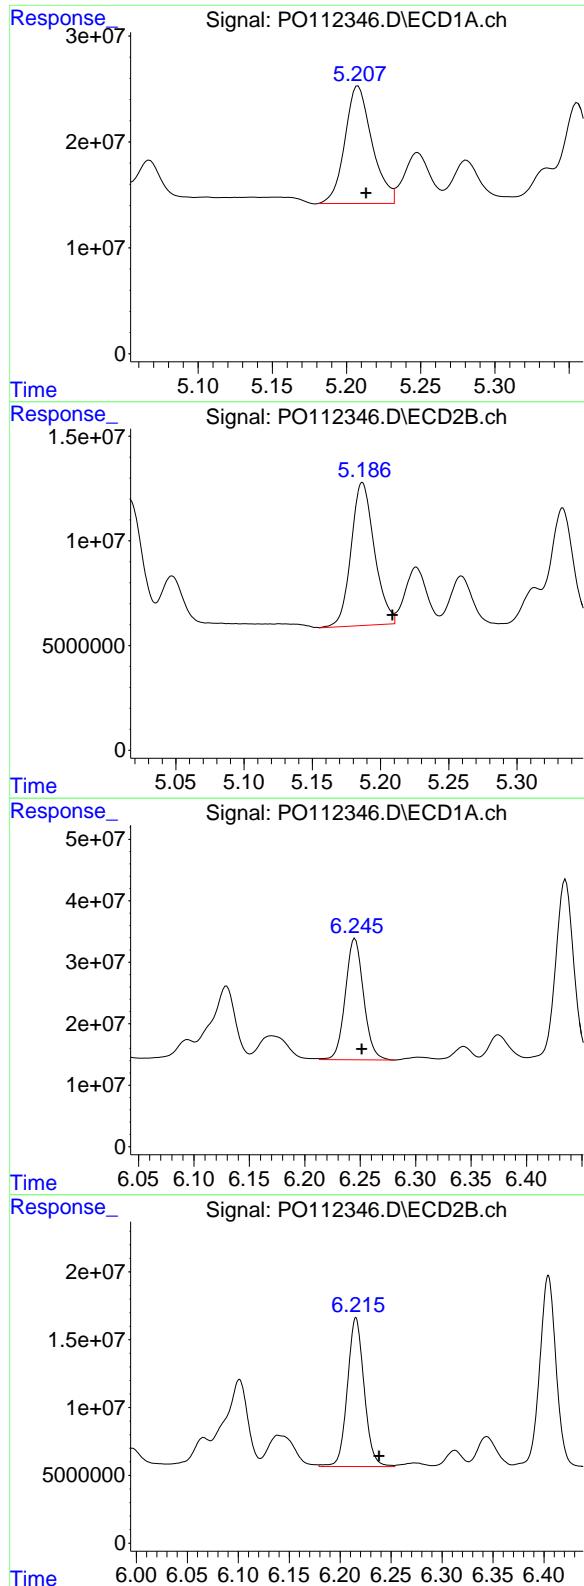

#7 AR-1016-5

R.T.: 5.208 min
 Delta R.T.: -0.005 min
 Response: 141516499
 Conc: 517.12 ng/ml

Instrument: ECD_O
 ClientSampleId: AR1660CCC500

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/22/2025
 Supervised By :mohammad ahmed 07/23/2025

#7 AR-1016-5


R.T.: 5.186 min
 Delta R.T.: -0.023 min
 Response: 81459246
 Conc: 472.36 ng/ml

#31 AR-1260-1

R.T.: 6.245 min
 Delta R.T.: -0.006 min
 Response: 225996595
 Conc: 450.88 ng/ml

#31 AR-1260-1

R.T.: 6.215 min
 Delta R.T.: -0.023 min
 Response: 125625189
 Conc: 447.76 ng/ml

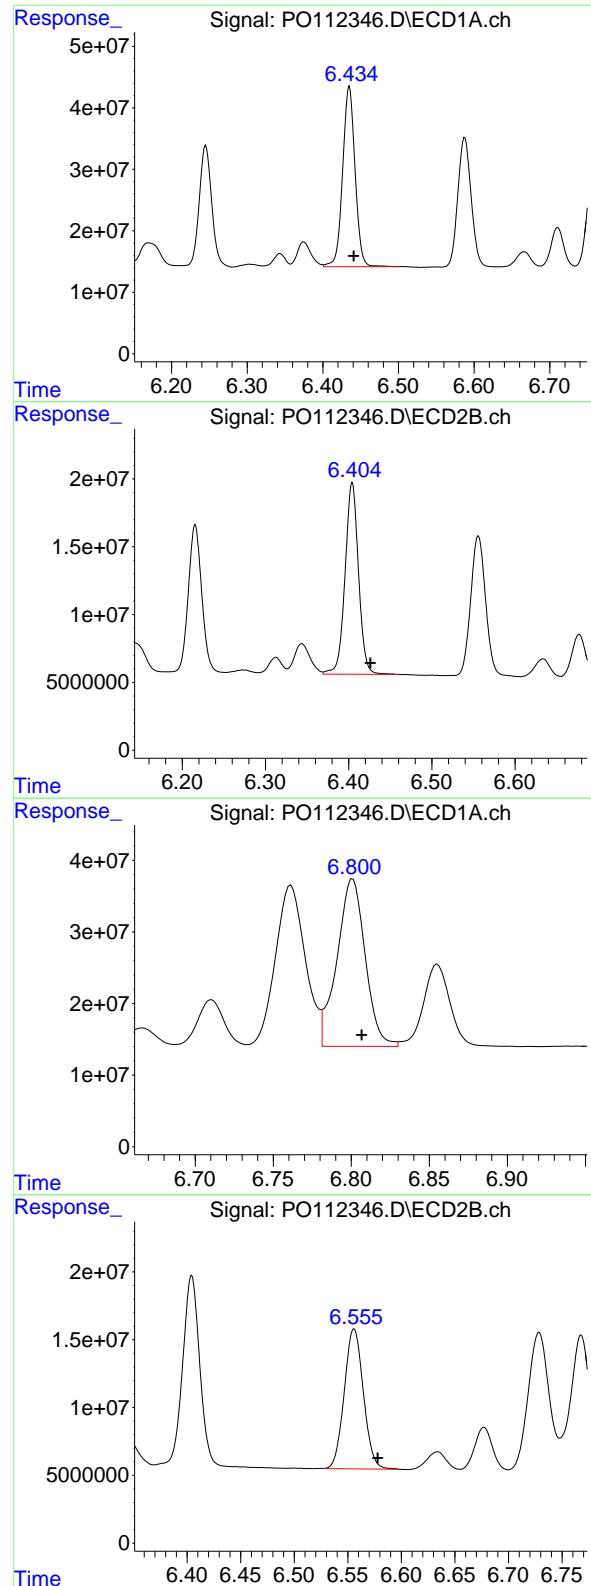

#32 AR-1260-2

R.T.: 6.435 min
 Delta R.T.: -0.006 min
 Response: 335105953
 Conc: 453.99 ng/ml

Instrument: ECD_O
 ClientSampleId: AR1660CCC500

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/22/2025
 Supervised By :mohammad ahmed 07/23/2025

#32 AR-1260-2


R.T.: 6.404 min
 Delta R.T.: -0.022 min
 Response: 159139752
 Conc: 468.06 ng/ml

#33 AR-1260-3

R.T.: 6.801 min
 Delta R.T.: -0.006 min
 Response: 294448405
 Conc: 449.21 ng/ml

#33 AR-1260-3

R.T.: 6.555 min
 Delta R.T.: -0.022 min
 Response: 128286726
 Conc: 465.51 ng/ml

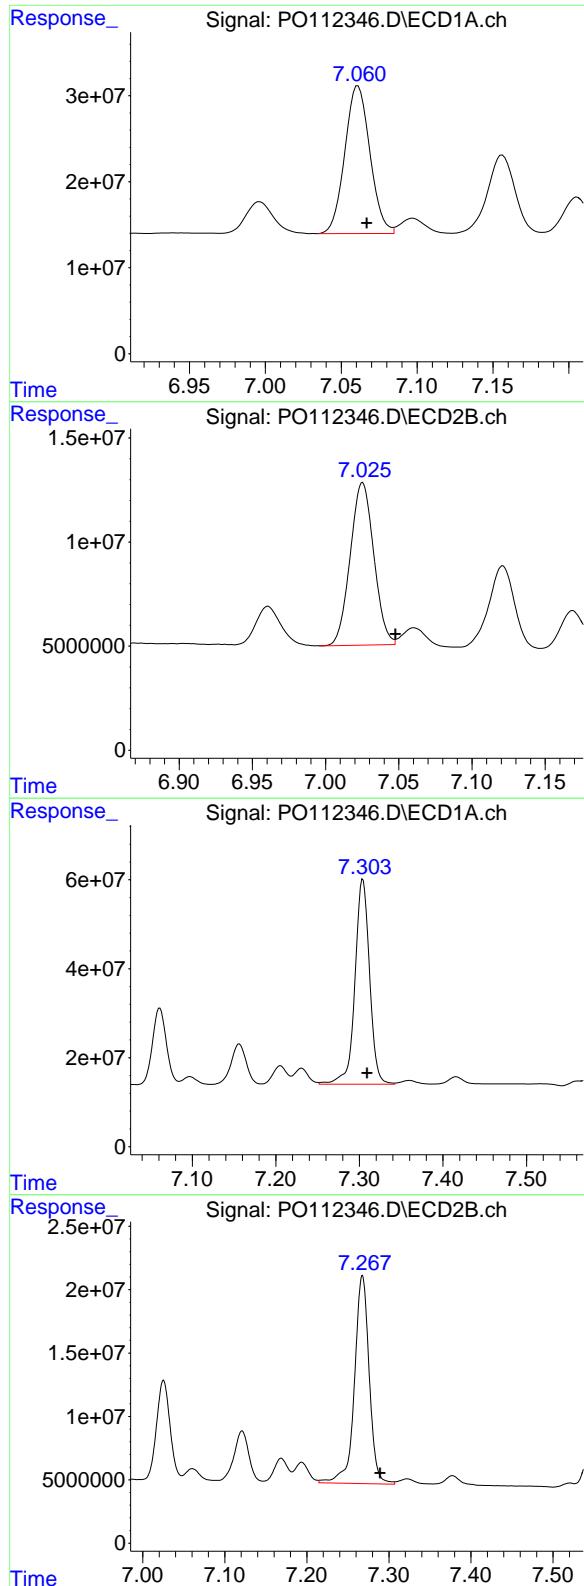

#34 AR-1260-4

R.T.: 7.061 min
 Delta R.T.: -0.006 min
 Response: 198088517
 Conc: 455.12 ng/ml

Instrument: ECD_O
ClientSampleId: AR1660CCC500

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/22/2025
 Supervised By :mohammad ahmed 07/23/2025

#34 AR-1260-4

R.T.: 7.025 min
 Delta R.T.: -0.023 min
 Response: 87550066
 Conc: 436.34 ng/ml

#35 AR-1260-5

R.T.: 7.304 min
 Delta R.T.: -0.005 min
 Response: 561793030
 Conc: 444.97 ng/ml

#35 AR-1260-5

R.T.: 7.268 min
 Delta R.T.: -0.022 min
 Response: 205537159
 Conc: 459.07 ng/ml



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Lab Name: Alliance

Contract: NOBI03

Lab Code: ACE

SDG NO.: Q2639

Continuing Calib Date: 07/22/2025

Initial Calibration Date(s): 07/08/2025

07/08/2025

Continuing Calib Time: 08:57

Initial Calibration Time(s): 14:06

22:16

GC Column: ZB-MR1

ID: 0.32 (mm)

COMPOUND	CCAL RT	AVG RT	RT WINDOW FROM	TO	DIFF RT
Aroclor-1016-1 (1)	4.76	4.76	4.66	4.86	0.00
Aroclor-1016-2 (2)	4.78	4.78	4.68	4.88	0.00
Aroclor-1016-3 (3)	4.84	4.84	4.74	4.94	0.00
Aroclor-1016-4 (4)	4.95	4.96	4.86	5.06	0.01
Aroclor-1016-5 (5)	5.21	5.21	5.11	5.31	0.00
Aroclor-1260-1 (1)	6.25	6.25	6.15	6.35	0.00
Aroclor-1260-2 (2)	6.44	6.44	6.34	6.54	0.00
Aroclor-1260-3 (3)	6.81	6.81	6.71	6.91	0.01
Aroclor-1260-4 (4)	7.06	7.07	6.97	7.17	0.01
Aroclor-1260-5 (5)	7.31	7.31	7.21	7.41	0.00
Tetrachloro-m-xylene	3.67	3.67	3.57	3.77	0.00
Decachlorobiphenyl	8.70	8.70	8.60	8.80	0.00



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Lab Name: Alliance

Contract: NOBI03

Lab Code: ACE

SDG NO.: Q2639

Continuing Calib Date: 07/22/2025

Initial Calibration Date(s): 07/08/2025

07/08/2025

Continuing Calib Time: 08:57

Initial Calibration Time(s): 14:06

22:16

GC Column: ZB-MR2

ID: 0.32 (mm)

COMPOUND	CCAL RT	AVG RT	RT WINDOW FROM	TO	DIFF RT
Aroclor-1016-1 (1)	4.74	4.76	4.66	4.86	0.02
Aroclor-1016-2 (2)	4.76	4.78	4.68	4.88	0.02
Aroclor-1016-3 (3)	4.93	4.95	4.85	5.05	0.02
Aroclor-1016-4 (4)	4.97	5.00	4.90	5.10	0.03
Aroclor-1016-5 (5)	5.19	5.21	5.11	5.31	0.03
Aroclor-1260-1 (1)	6.21	6.24	6.14	6.34	0.03
Aroclor-1260-2 (2)	6.40	6.43	6.33	6.53	0.03
Aroclor-1260-3 (3)	6.55	6.58	6.48	6.68	0.03
Aroclor-1260-4 (4)	7.02	7.05	6.95	7.15	0.03
Aroclor-1260-5 (5)	7.27	7.29	7.19	7.39	0.02
Tetrachloro-m-xylene	3.66	3.68	3.58	3.78	0.02
Decachlorobiphenyl	8.64	8.67	8.57	8.77	0.03



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900, Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Lab Name:	Alliance	Contract:	NOBI03
Lab Code:	ACE	SDG NO.:	Q2639
GC Column:	ZB-MR1	ID: 0.32 (mm)	Initi. Calib. Date(s): 07/08/2025 07/08/2025

Client Sample No.:	CCAL03	Date Analyzed:	07/22/2025
Lab Sample No.:	AR1660CCC500	Data File :	PO112366.D
		Time Analyzed:	08:57

COMPOUND	RT	RT WINDOW FROM TO		CALC AMOUNT(ng)	NOM AMOUNT(ng)	%D
Aroclor-1016-1	4.759	4.661	4.861	518.970	500.000	3.8
Aroclor-1016-2	4.778	4.680	4.880	532.520	500.000	6.5
Aroclor-1016-3	4.835	4.736	4.936	514.470	500.000	2.9
Aroclor-1016-4	4.954	4.856	5.056	522.410	500.000	4.5
Aroclor-1016-5	5.211	5.113	5.313	511.450	500.000	2.3
Aroclor-1260-1	6.249	6.151	6.351	493.780	500.000	-1.2
Aroclor-1260-2	6.439	6.341	6.541	495.000	500.000	-1.0
Aroclor-1260-3	6.805	6.707	6.907	500.210	500.000	0.0
Aroclor-1260-4	7.064	6.967	7.167	503.510	500.000	0.7
Aroclor-1260-5	7.307	7.209	7.409	486.250	500.000	-2.8
Decachlorobiphenyl	8.700	8.603	8.803	49.980	50.000	0.0
Tetrachloro-m-xylene	3.672	3.573	3.773	57.200	50.000	14.4



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900, Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Lab Name:	<u>Alliance</u>	Contract:	<u>NOBI03</u>
Lab Code:	<u>ACE</u>	SDG NO.:	<u>Q2639</u>
GC Column:	<u>ZB-MR2</u>	ID: <u>0.32</u> (mm)	Initi. Calib. Date(s): <u>07/08/2025</u> <u>07/08/2025</u>

Client Sample No.:	<u>CCAL03</u>	Date Analyzed:	<u>07/22/2025</u>
Lab Sample No.:	<u>AR1660CCC500</u>	Data File :	<u>PO112366.D</u>
		Time Analyzed:	<u>08:57</u>

COMPOUND	RT	RT WINDOW FROM	TO	CALC AMOUNT(ng)	NOM AMOUNT(ng)	%D
Aroclor-1016-1	4.737	4.661	4.861	471.470	500.000	-5.7
Aroclor-1016-2	4.756	4.679	4.879	469.570	500.000	-6.1
Aroclor-1016-3	4.930	4.854	5.054	484.320	500.000	-3.1
Aroclor-1016-4	4.973	4.897	5.097	496.800	500.000	-0.6
Aroclor-1016-5	5.185	5.109	5.309	472.560	500.000	-5.5
Aroclor-1260-1	6.214	6.138	6.338	482.800	500.000	-3.4
Aroclor-1260-2	6.403	6.326	6.526	514.630	500.000	2.9
Aroclor-1260-3	6.554	6.478	6.678	517.520	500.000	3.5
Aroclor-1260-4	7.024	6.948	7.148	501.240	500.000	0.2
Aroclor-1260-5	7.267	7.190	7.390	519.750	500.000	4.0
Decachlorobiphenyl	8.643	8.568	8.768	47.160	50.000	-5.7
Tetrachloro-m-xylene	3.662	3.584	3.784	51.060	50.000	2.1

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0072225\
 Data File : P0112366.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Jul 2025 08:57
 Operator : YP/AJ
 Sample : AR1660CCC500
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1660CCC500

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/23/2025
 Supervised By :mohammad ahmed 07/24/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 22 10:29:49 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 22 09:14:26 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	3.672	3.662	565.9E6	325.3E6	57.195	51.055
2) SA Decachlor...	8.700	8.643	341.7E6	81274339	49.977	47.158m

Target Compounds

3) L1 AR-1016-1	4.759	4.737	176.5E6	105.1E6	518.970	471.475m
4) L1 AR-1016-2	4.778	4.756	264.8E6	154.5E6	532.518	469.570m
5) L1 AR-1016-3	4.835	4.930	166.5E6	82269412	514.472	484.317m
6) L1 AR-1016-4	4.954	4.973	134.2E6	68174317	522.411	496.798m
7) L1 AR-1016-5	5.211	5.185	140.0E6	81492370	511.454	472.556m
31) L7 AR-1260-1	6.249	6.214	247.5E6	135.5E6	493.782	482.798
32) L7 AR-1260-2	6.439	6.403	365.4E6	175.0E6	495.002	514.627
33) L7 AR-1260-3	6.805	6.554	327.9E6	142.6E6	500.210	517.520m
34) L7 AR-1260-4	7.064	7.024	219.2E6	100.6E6	503.511	501.240m
35) L7 AR-1260-5	7.307	7.267	613.9E6	232.7E6	486.246	519.751

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0072225\
 Data File : P0112366.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Jul 2025 08:57
 Operator : YP/AJ
 Sample : AR1660CCC500
 Misc :
 ALS Vial : 3 Sample Multiplier: 1



Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 22 10:29:49 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 22 09:14:26 2025
 Response via : Initial Calibration
 Integrator: ChemStation


Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Instrument :
 ECD_O
 ClientSampleId :
 AR1660CCC500

Manual Integrations APPROVED

Reviewed By :Yogesh Patel 07/23/2025
 Supervised By :mohammad ahmed 07/24/2025

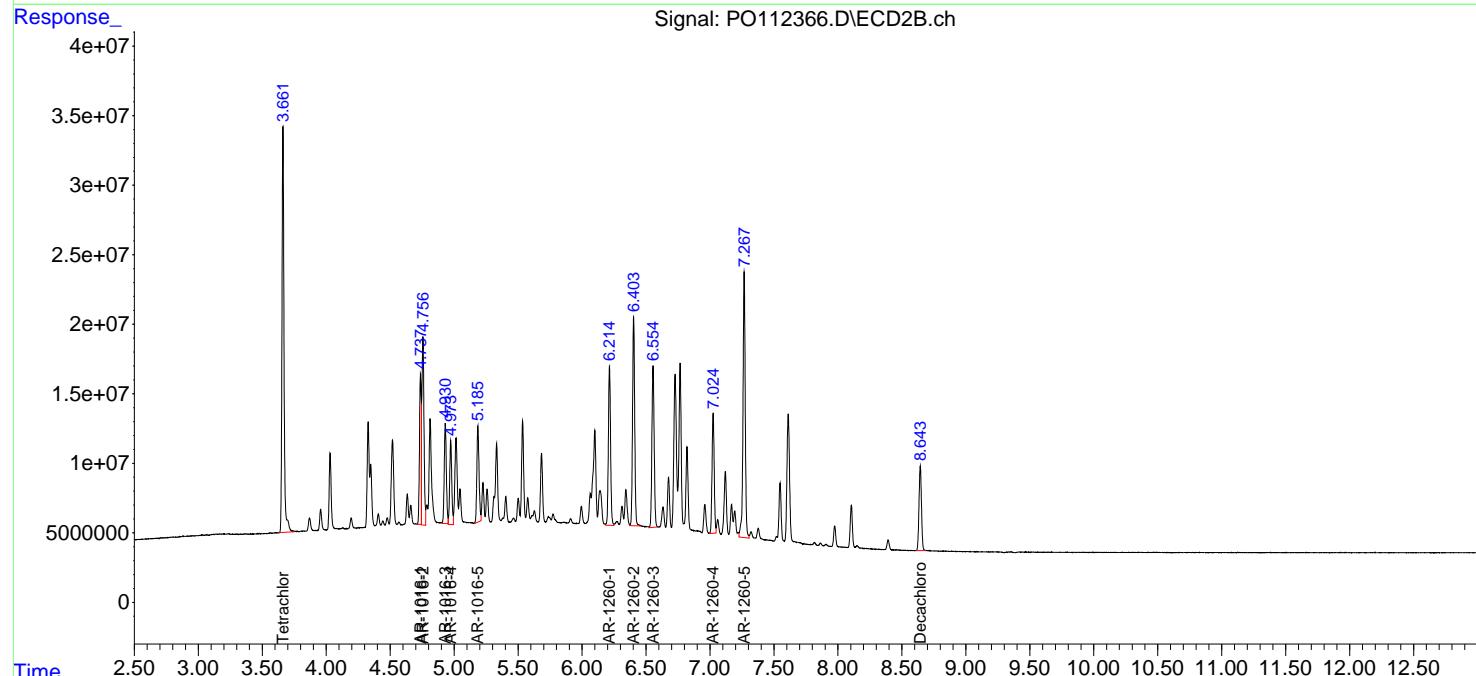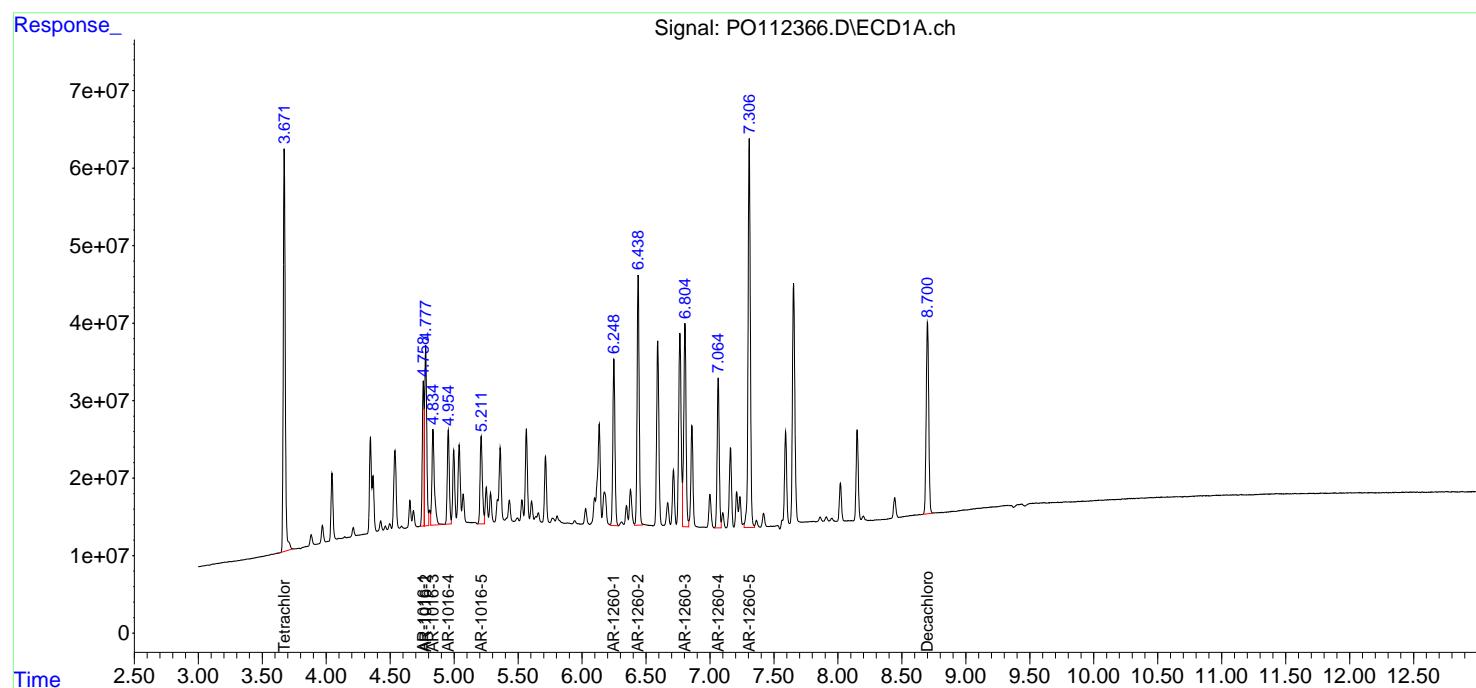

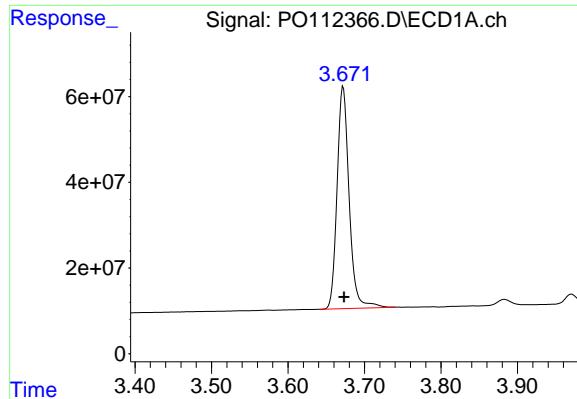


#1 Tetrachloro-m-xylene

R.T.: 3.672 min
Delta R.T.: 0.000 min
Response: 565932233
Conc: 57.20 ng/ml

Instrument: ECD_O
ClientSampleId: AR1660CCC500


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/23/2025
Supervised By :mohammad ahmed 07/24/2025

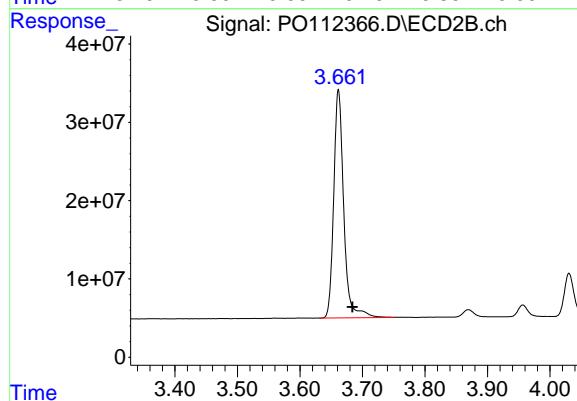


#1 Tetrachloro-m-xylene

R.T.: 3.662 min
Delta R.T.: -0.022 min
Response: 325275039
Conc: 51.06 ng/ml

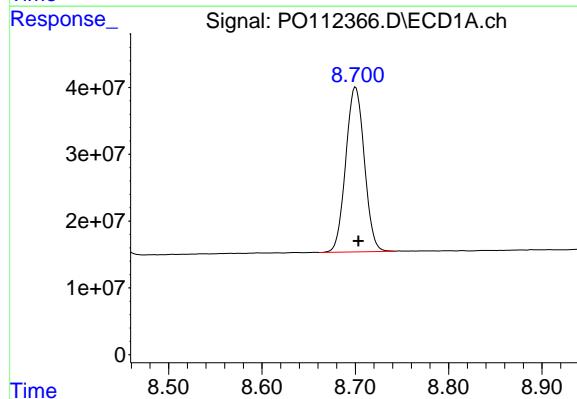


#2 Decachlorobiphenyl

R.T.: 8.700 min
Delta R.T.: -0.003 min
Response: 341696880
Conc: 49.98 ng/ml

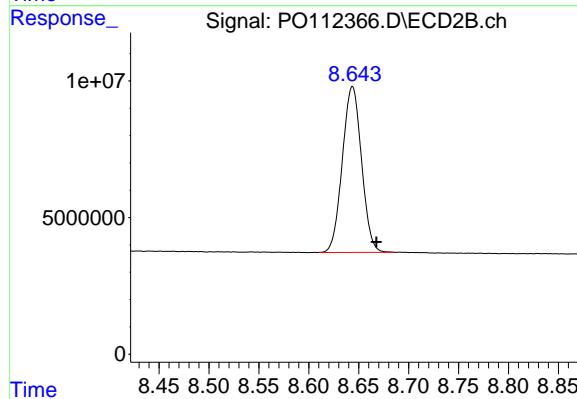

#2 Decachlorobiphenyl

R.T.: 8.643 min
Delta R.T.: -0.025 min
Response: 81274339
Conc: 47.16 ng/ml

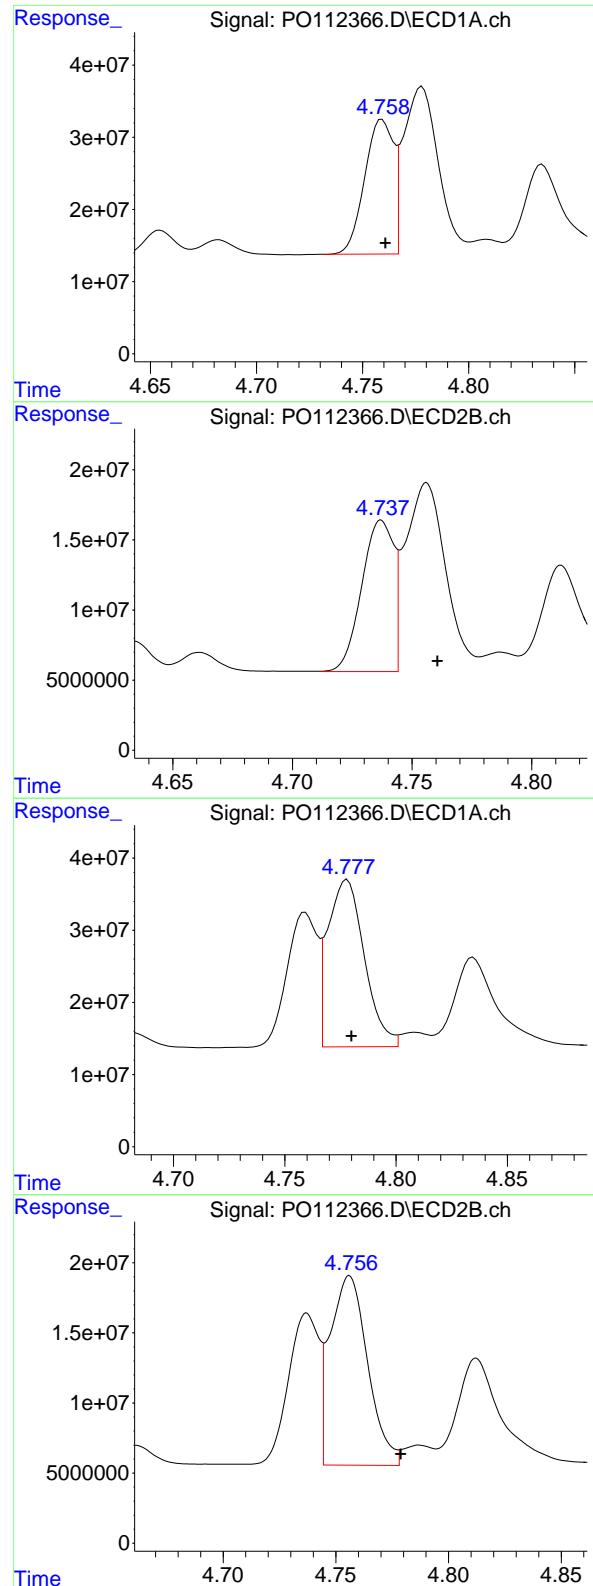

#3 AR-1016-1

R.T.: 4.759 min
 Delta R.T.: -0.002 min
 Response: 176513620
 Conc: 518.97 ng/ml

Instrument: ECD_O
 ClientSampleId: AR1660CCC500

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/23/2025
 Supervised By :mohammad ahmed 07/24/2025

#3 AR-1016-1


R.T.: 4.737 min
 Delta R.T.: -0.024 min
 Response: 105060816
 Conc: 471.47 ng/ml

#4 AR-1016-2

R.T.: 4.778 min
 Delta R.T.: -0.002 min
 Response: 264817007
 Conc: 532.52 ng/ml

#4 AR-1016-2

R.T.: 4.756 min
 Delta R.T.: -0.023 min
 Response: 154534389
 Conc: 469.57 ng/ml

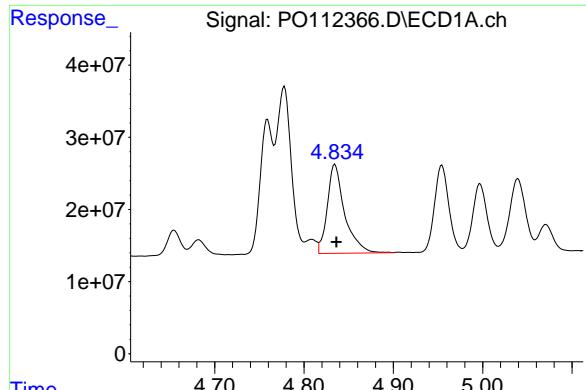


#5 AR-1016-3

R.T.: 4.835 min
Delta R.T.: -0.002 min
Response: 166541661
Conc: 514.47 ng/ml

Instrument: ECD_O
ClientSampleId: AR1660CCC500


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/23/2025
Supervised By :mohammad ahmed 07/24/2025

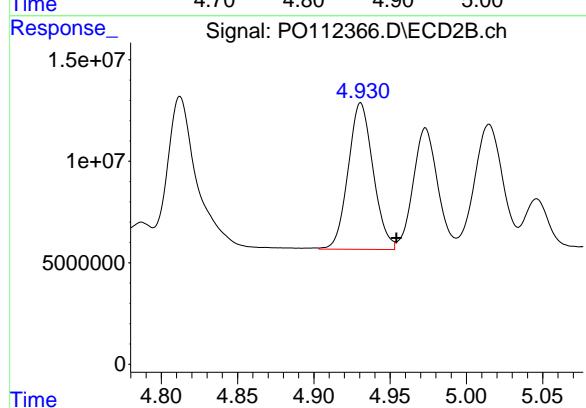


#5 AR-1016-3

R.T.: 4.930 min
Delta R.T.: -0.024 min
Response: 82269412
Conc: 484.32 ng/ml

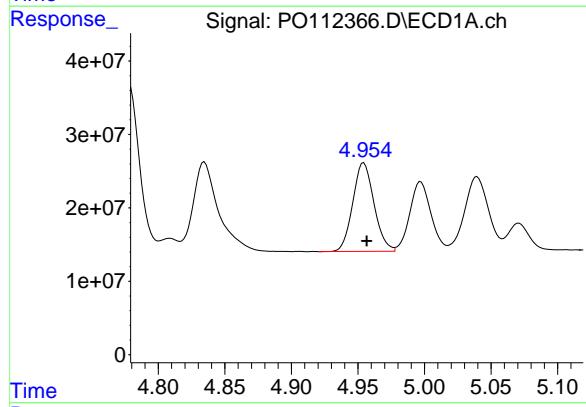


#6 AR-1016-4

R.T.: 4.954 min
Delta R.T.: -0.002 min
Response: 134155056
Conc: 522.41 ng/ml

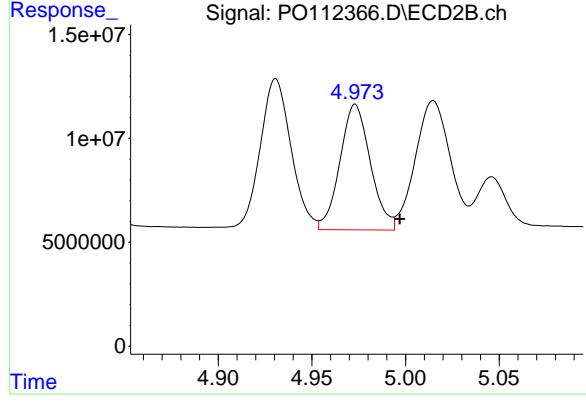

#6 AR-1016-4

R.T.: 4.973 min
Delta R.T.: -0.024 min
Response: 68174317
Conc: 496.80 ng/ml

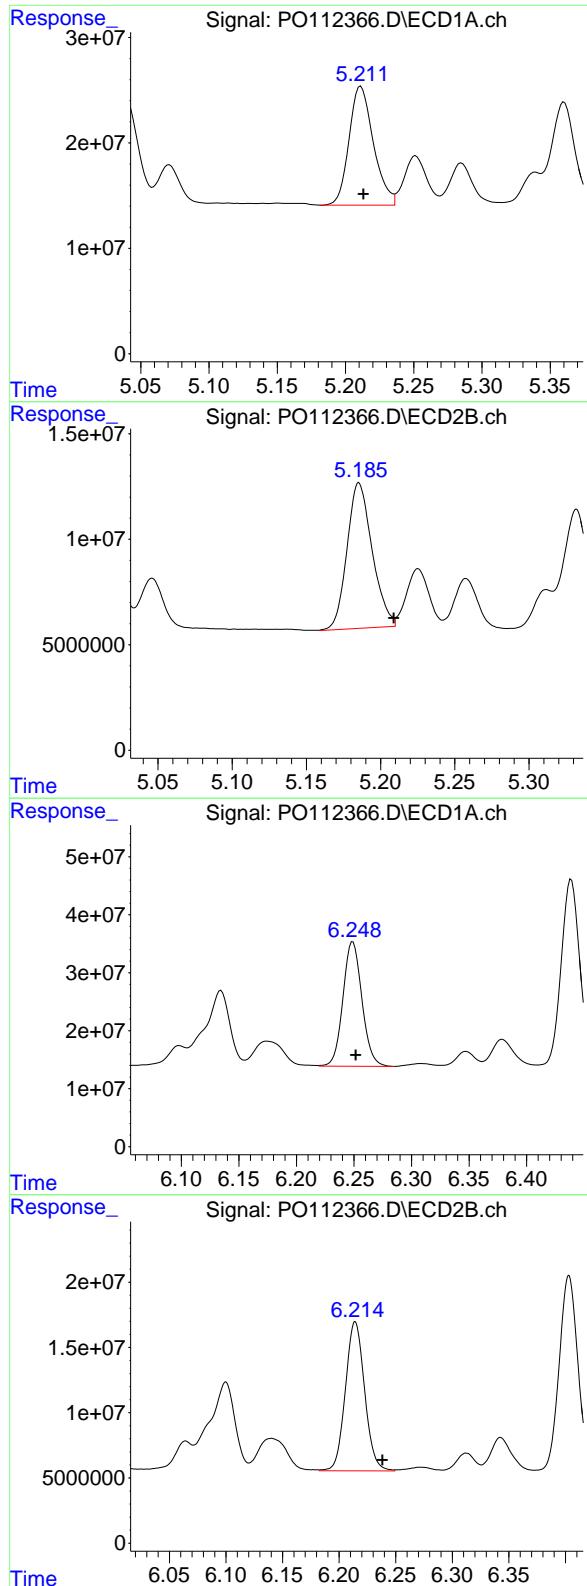

#7 AR-1016-5

R.T.: 5.211 min
 Delta R.T.: -0.002 min
 Response: 139965370
 Conc: 511.45 ng/ml

Instrument: ECD_O
 ClientSampleId: AR1660CCC500

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/23/2025
 Supervised By :mohammad ahmed 07/24/2025

#7 AR-1016-5


R.T.: 5.185 min
 Delta R.T.: -0.024 min
 Response: 81492370
 Conc: 472.56 ng/ml

#31 AR-1260-1

R.T.: 6.249 min
 Delta R.T.: -0.003 min
 Response: 247502934
 Conc: 493.78 ng/ml

#31 AR-1260-1

R.T.: 6.214 min
 Delta R.T.: -0.024 min
 Response: 135454857
 Conc: 482.80 ng/ml

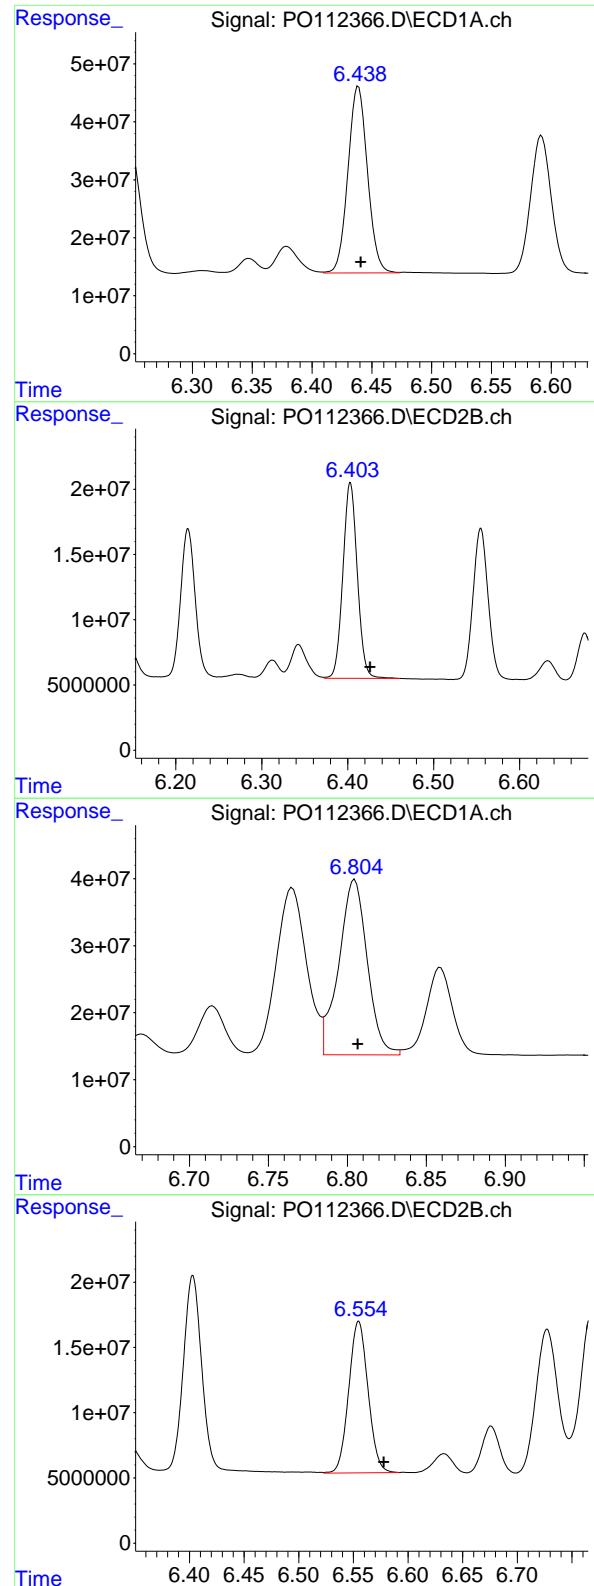

#32 AR-1260-2

R.T.: 6.439 min
Delta R.T.: -0.002 min
Response: 365378129
Conc: 495.00 ng/ml

Instrument: ECD_O
ClientSampleId: AR1660CCC500

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/23/2025
Supervised By :mohammad ahmed 07/24/2025

#32 AR-1260-2





R.T.: 6.403 min
Delta R.T.: -0.023 min
Response: 174971478
Conc: 514.63 ng/ml

#33 AR-1260-3

R.T.: 6.805 min
Delta R.T.: -0.002 min
Response: 327878936
Conc: 500.21 ng/ml

#33 AR-1260-3

R.T.: 6.554 min
Delta R.T.: -0.023 min
Response: 142621388
Conc: 517.52 ng/ml

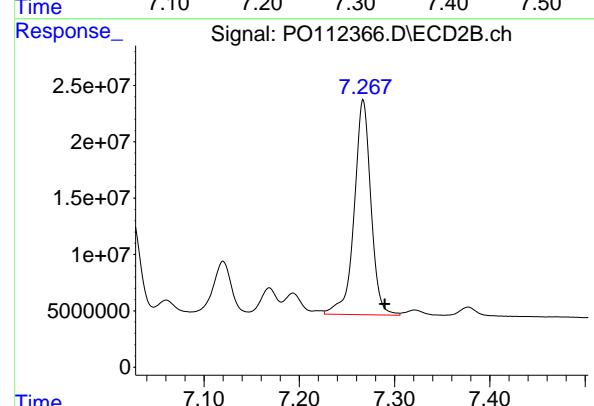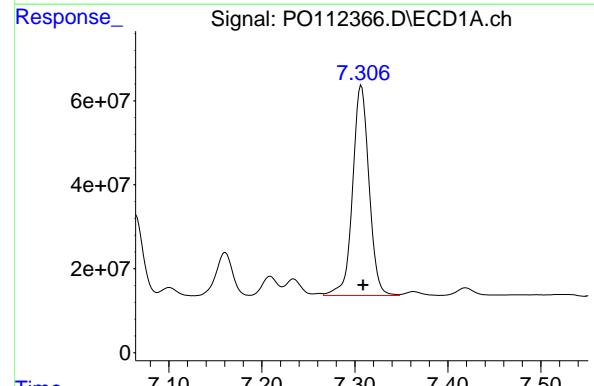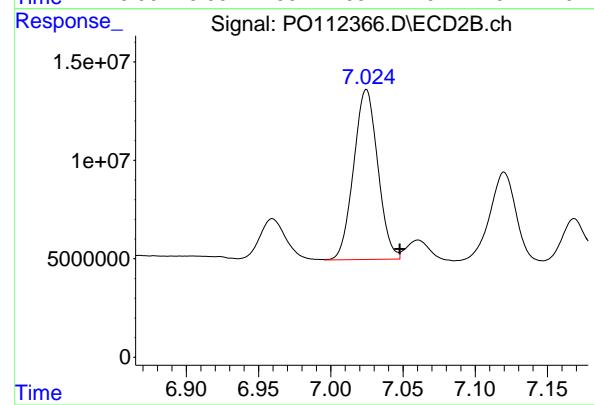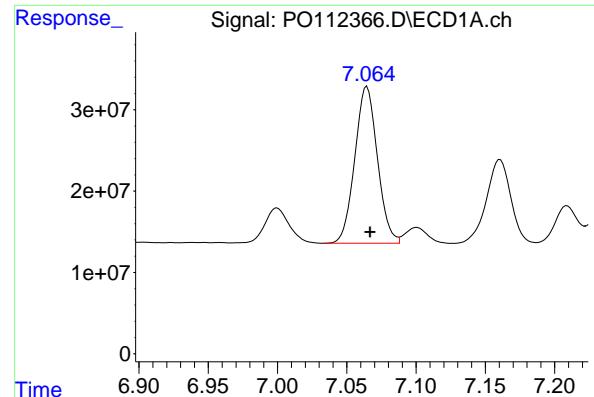

#34 AR-1260-4

R.T.: 7.064 min
Delta R.T.: -0.002 min
Response: 219151907
Conc: 503.51 ng/ml

Instrument: ECD_O
ClientSampleId: AR1660CCC500

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/23/2025
Supervised By :mohammad ahmed 07/24/2025

#34 AR-1260-4

R.T.: 7.024 min
Delta R.T.: -0.023 min
Response: 100571277
Conc: 501.24 ng/ml

#35 AR-1260-5

R.T.: 7.307 min
Delta R.T.: -0.002 min
Response: 613903993
Conc: 486.25 ng/ml

#35 AR-1260-5

R.T.: 7.267 min
Delta R.T.: -0.022 min
Response: 232707276
Conc: 519.75 ng/ml



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Lab Name: Alliance

Contract: NOBI03

Lab Code: ACE

SDG NO.: Q2639

Continuing Calib Date: 07/22/2025

Initial Calibration Date(s): 07/08/2025

07/08/2025

Continuing Calib Time: 16:21

Initial Calibration Time(s): 14:06

22:16

GC Column: ZB-MR1

ID: 0.32 (mm)

COMPOUND	CCAL RT	Avg RT	RT Window From	TO	Diff RT
Aroclor-1016-1 (1)	4.76	4.76	4.66	4.86	0.00
Aroclor-1016-2 (2)	4.78	4.78	4.68	4.88	0.00
Aroclor-1016-3 (3)	4.83	4.84	4.74	4.94	0.01
Aroclor-1016-4 (4)	4.95	4.96	4.86	5.06	0.01
Aroclor-1016-5 (5)	5.21	5.21	5.11	5.31	0.00
Aroclor-1260-1 (1)	6.25	6.25	6.15	6.35	0.00
Aroclor-1260-2 (2)	6.44	6.44	6.34	6.54	0.00
Aroclor-1260-3 (3)	6.80	6.81	6.71	6.91	0.01
Aroclor-1260-4 (4)	7.06	7.07	6.97	7.17	0.01
Aroclor-1260-5 (5)	7.30	7.31	7.21	7.41	0.01
Tetrachloro-m-xylene	3.67	3.67	3.57	3.77	0.00
Decachlorobiphenyl	8.70	8.70	8.60	8.80	0.01



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Lab Name: Alliance

Contract: NOBI03

Lab Code: ACE

SDG NO.: Q2639

Continuing Calib Date: 07/22/2025

Initial Calibration Date(s): 07/08/2025

07/08/2025

Continuing Calib Time: 16:21

Initial Calibration Time(s): 14:06

22:16

GC Column: ZB-MR2

ID: 0.32 (mm)

COMPOUND	CCAL RT	AVG RT	RT WINDOW FROM	TO	DIFF RT
Aroclor-1016-1 (1)	4.74	4.76	4.66	4.86	0.02
Aroclor-1016-2 (2)	4.76	4.78	4.68	4.88	0.02
Aroclor-1016-3 (3)	4.93	4.95	4.85	5.05	0.02
Aroclor-1016-4 (4)	4.97	5.00	4.90	5.10	0.03
Aroclor-1016-5 (5)	5.19	5.21	5.11	5.31	0.02
Aroclor-1260-1 (1)	6.22	6.24	6.14	6.34	0.02
Aroclor-1260-2 (2)	6.40	6.43	6.33	6.53	0.03
Aroclor-1260-3 (3)	6.55	6.58	6.48	6.68	0.03
Aroclor-1260-4 (4)	7.02	7.05	6.95	7.15	0.03
Aroclor-1260-5 (5)	7.27	7.29	7.19	7.39	0.02
Tetrachloro-m-xylene	3.66	3.68	3.58	3.78	0.02
Decachlorobiphenyl	8.64	8.67	8.57	8.77	0.03



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900, Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Lab Name:	Alliance	Contract:	NOBI03
Lab Code:	ACE	SDG NO.:	Q2639
GC Column:	ZB-MR1	ID: 0.32 (mm)	Initi. Calib. Date(s): 07/08/2025 07/08/2025

Client Sample No.:	CCAL04	Date Analyzed:	07/22/2025
Lab Sample No.:	AR1660CCC500	Data File :	PO112381.D
		Time Analyzed:	16:21

COMPOUND	RT	RT WINDOW FROM	TO	CALC AMOUNT(ng)	NOM AMOUNT(ng)	%D
Aroclor-1016-1	4.756	4.661	4.861	531.760	500.000	6.4
Aroclor-1016-2	4.775	4.680	4.880	537.930	500.000	7.6
Aroclor-1016-3	4.832	4.736	4.936	518.230	500.000	3.6
Aroclor-1016-4	4.951	4.856	5.056	526.680	500.000	5.3
Aroclor-1016-5	5.209	5.113	5.313	549.170	500.000	9.8
Aroclor-1260-1	6.246	6.151	6.351	488.230	500.000	-2.4
Aroclor-1260-2	6.436	6.341	6.541	488.260	500.000	-2.3
Aroclor-1260-3	6.801	6.707	6.907	477.960	500.000	-4.4
Aroclor-1260-4	7.061	6.967	7.167	504.140	500.000	0.8
Aroclor-1260-5	7.304	7.209	7.409	501.750	500.000	0.4
Decachlorobiphenyl	8.695	8.603	8.803	49.550	50.000	-0.9
Tetrachloro-m-xylene	3.670	3.573	3.773	58.470	50.000	16.9



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900, Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Lab Name:	<u>Alliance</u>	Contract:	<u>NOBI03</u>
Lab Code:	<u>ACE</u>	SDG NO.:	<u>Q2639</u>
GC Column:	<u>ZB-MR2</u>	ID: <u>0.32</u> (mm)	Initi. Calib. Date(s): <u>07/08/2025</u> <u>07/08/2025</u>

Client Sample No.:	<u>CCAL04</u>	Date Analyzed:	<u>07/22/2025</u>
Lab Sample No.:	<u>AR1660CCC500</u>	Data File :	<u>PO112381.D</u>
		Time Analyzed:	<u>16:21</u>

COMPOUND	RT	RT WINDOW FROM	TO	CALC AMOUNT(ng)	NOM AMOUNT(ng)	%D
Aroclor-1016-1	4.738	4.661	4.861	492.160	500.000	-1.6
Aroclor-1016-2	4.756	4.679	4.879	479.070	500.000	-4.2
Aroclor-1016-3	4.931	4.854	5.054	496.440	500.000	-0.7
Aroclor-1016-4	4.974	4.897	5.097	492.160	500.000	-1.6
Aroclor-1016-5	5.186	5.109	5.309	516.450	500.000	3.3
Aroclor-1260-1	6.215	6.138	6.338	481.700	500.000	-3.7
Aroclor-1260-2	6.404	6.326	6.526	499.280	500.000	-0.1
Aroclor-1260-3	6.554	6.478	6.678	492.460	500.000	-1.5
Aroclor-1260-4	7.024	6.948	7.148	455.250	500.000	-9.0
Aroclor-1260-5	7.266	7.190	7.390	459.270	500.000	-8.1
Decachlorobiphenyl	8.642	8.568	8.768	46.920	50.000	-6.2
Tetrachloro-m-xylene	3.662	3.584	3.784	53.080	50.000	6.2

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0072225\
 Data File : P0112381.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Jul 2025 16:21
 Operator : YP/AJ
 Sample : AR1660CCC500
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1660CCC500

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/23/2025
 Supervised By :mohammad ahmed 07/24/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 23 01:52:11 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 22 09:14:26 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	3.670	3.662	578.5E6	338.2E6	58.470	53.081
2) SA Decachlor...	8.695	8.642	338.8E6	80859360	49.551	46.917

Target Compounds

3) L1 AR-1016-1	4.756	4.738	180.9E6	109.7E6	531.757	492.161m
4) L1 AR-1016-2	4.775	4.756	267.5E6	157.7E6	537.929	479.071m
5) L1 AR-1016-3	4.832	4.931	167.8E6	84329493	518.228	496.445m
6) L1 AR-1016-4	4.951	4.974	135.3E6	67538407	526.679	492.164m
7) L1 AR-1016-5	5.209	5.186	150.3E6	89062171	549.172	516.451m
31) L7 AR-1260-1	6.246	6.215	244.7E6	135.1E6	488.228	481.696
32) L7 AR-1260-2	6.436	6.404	360.4E6	169.8E6	488.264	499.283
33) L7 AR-1260-3	6.801	6.554	313.3E6	135.7E6	477.962	492.462m
34) L7 AR-1260-4	7.061	7.024	219.4E6	91343921	504.145	455.251m
35) L7 AR-1260-5	7.304	7.266	633.5E6	205.6E6	501.754	459.271

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0072225\
 Data File : P0112381.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Jul 2025 16:21
 Operator : YP/AJ
 Sample : AR1660CCC500
 Misc :
 ALS Vial : 3 Sample Multiplier: 1



Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 23 01:52:11 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 22 09:14:26 2025
 Response via : Initial Calibration
 Integrator: ChemStation


Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Instrument :
 ECD_O
 ClientSampleId :
 AR1660CCC500

Manual Integrations APPROVED

Reviewed By :Yogesh Patel 07/23/2025
 Supervised By :mohammad ahmed 07/24/2025

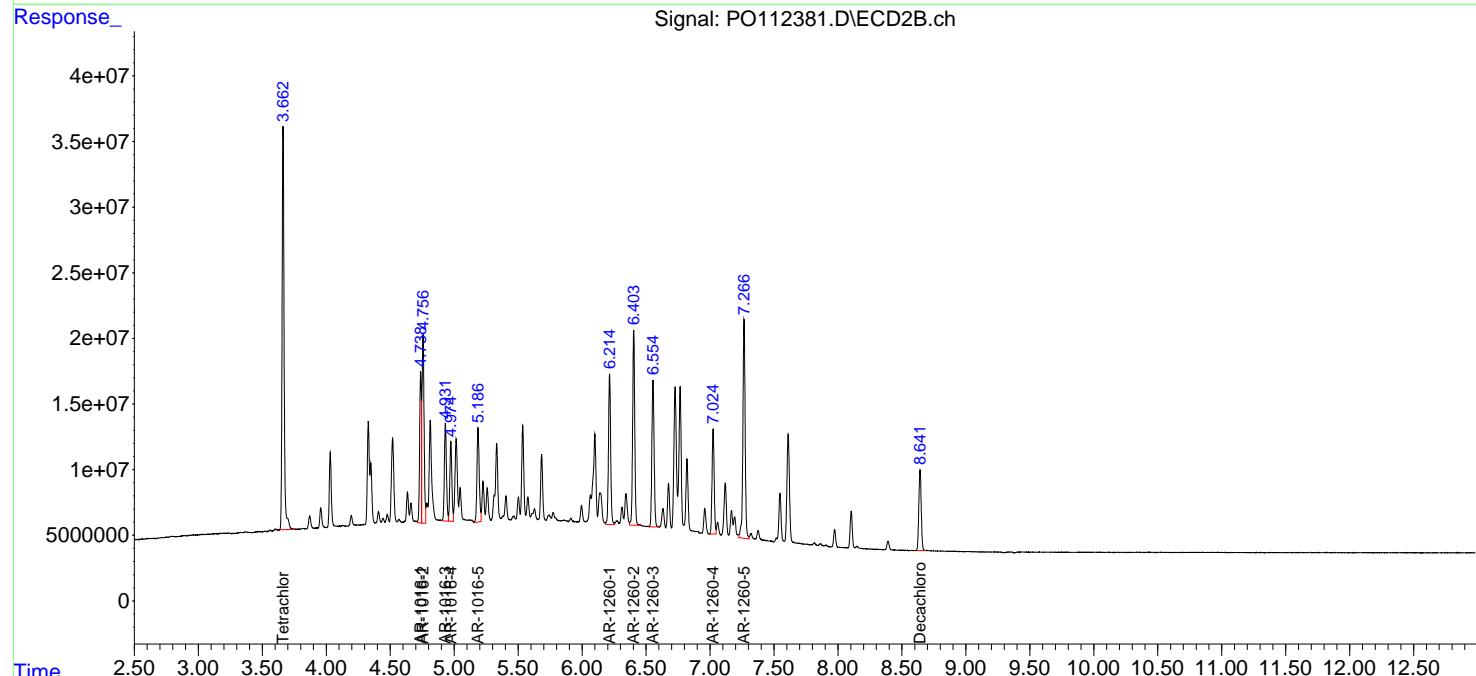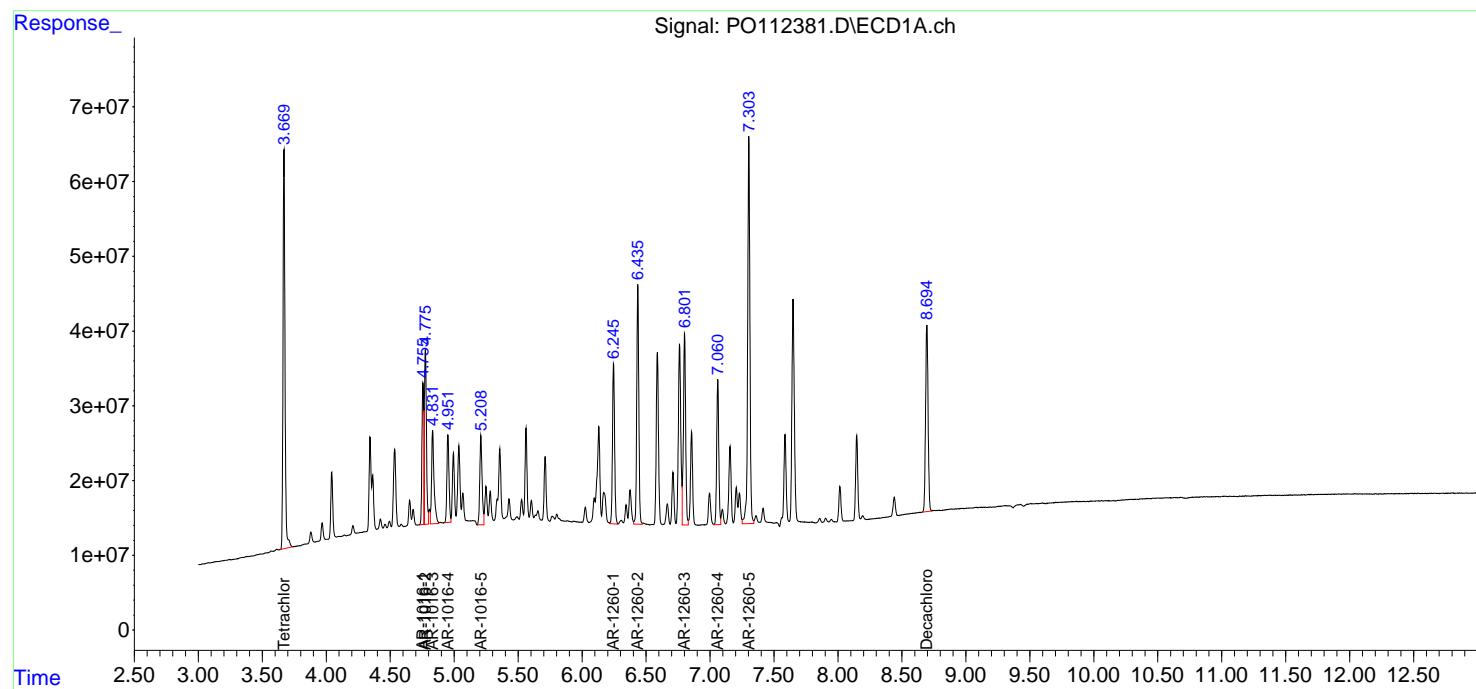

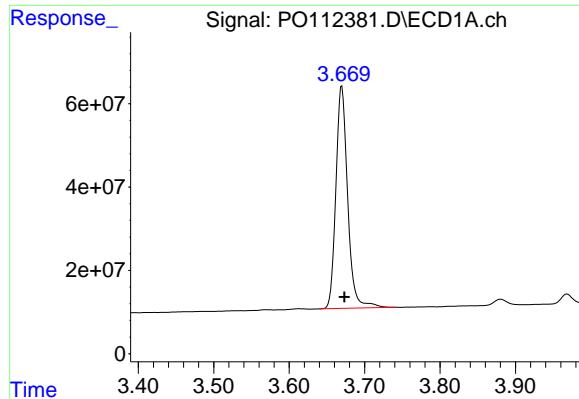


#1 Tetrachloro-m-xylene

R.T.: 3.670 min
Delta R.T.: -0.003 min
Response: 578547123
Conc: 58.47 ng/ml

Instrument: ECD_O
ClientSampleId: AR1660CCC500


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/23/2025
Supervised By :mohammad ahmed 07/24/2025

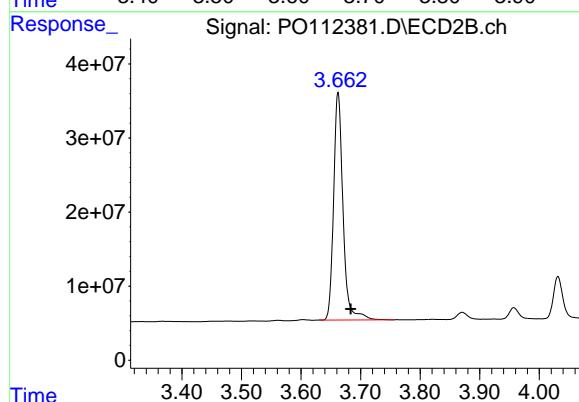


#1 Tetrachloro-m-xylene

R.T.: 3.662 min
Delta R.T.: -0.021 min
Response: 338183063
Conc: 53.08 ng/ml

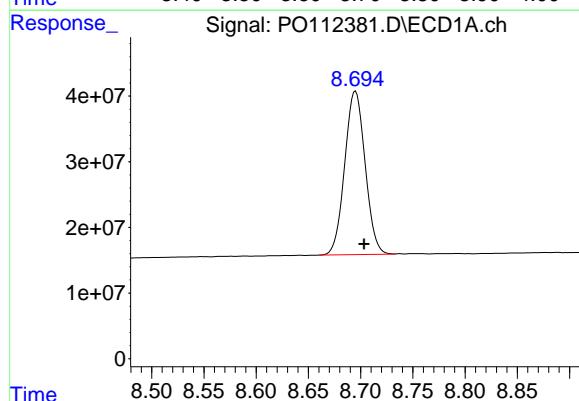





#2 Decachlorobiphenyl

R.T.: 8.695 min
Delta R.T.: -0.008 min
Response: 338782695
Conc: 49.55 ng/ml

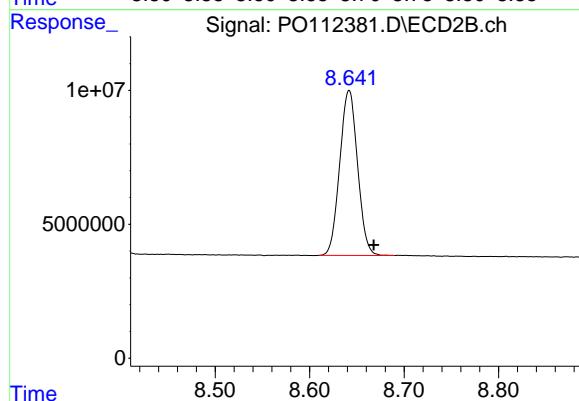

#2 Decachlorobiphenyl

R.T.: 8.642 min
Delta R.T.: -0.026 min
Response: 80859360
Conc: 46.92 ng/ml

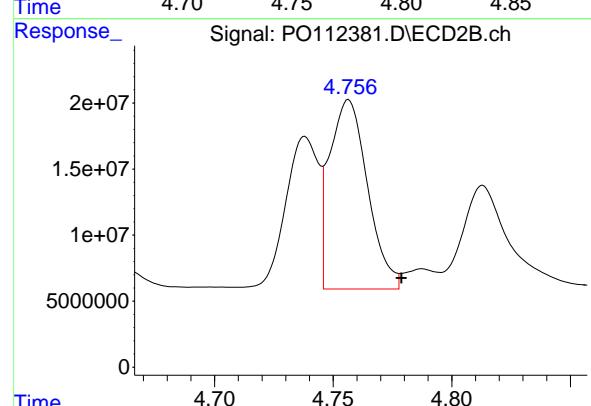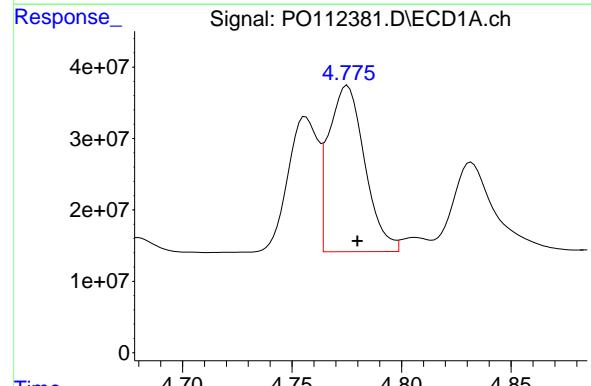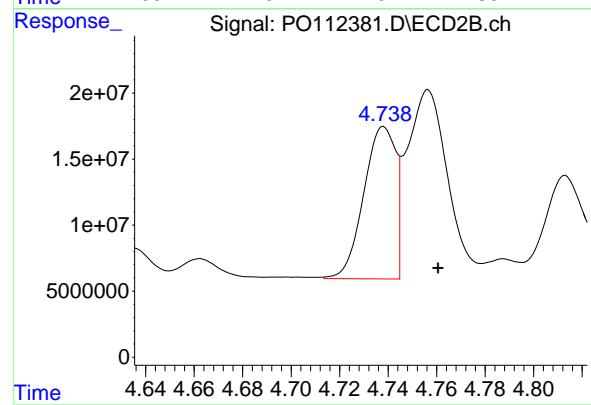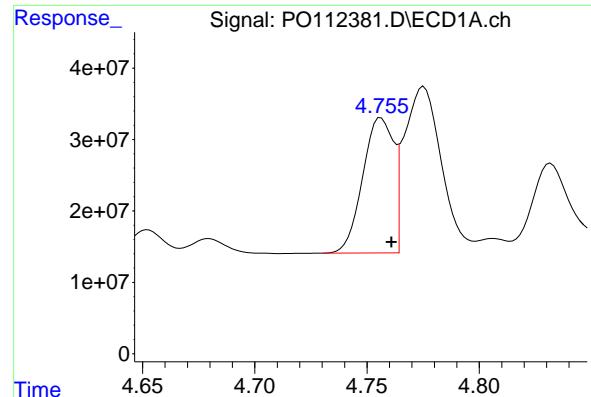




#3 AR-1016-1

R.T.: 4.756 min
 Delta R.T.: -0.005 min
 Response: 180862710
 Conc: 531.76 ng/ml

Instrument: ECD_O
 ClientSampleId: AR1660CCC500




Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/23/2025
 Supervised By :mohammad ahmed 07/24/2025

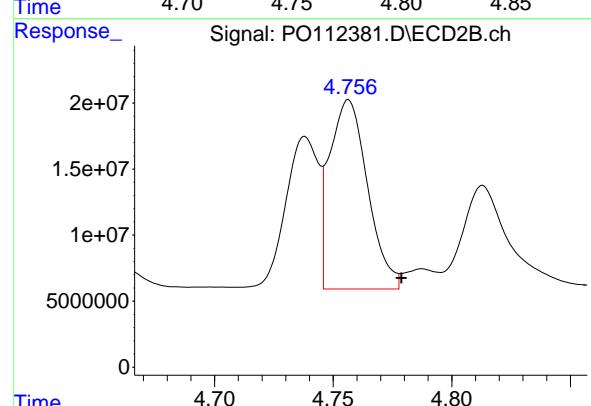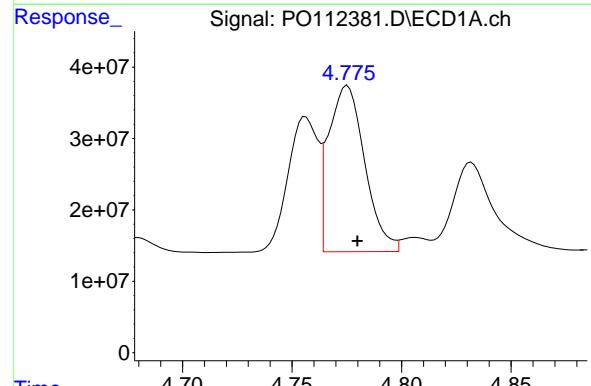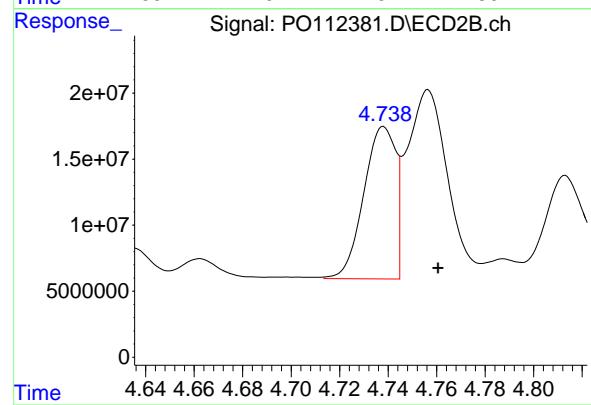




#3 AR-1016-1

R.T.: 4.738 min
 Delta R.T.: -0.023 min
 Response: 109670488
 Conc: 492.16 ng/ml

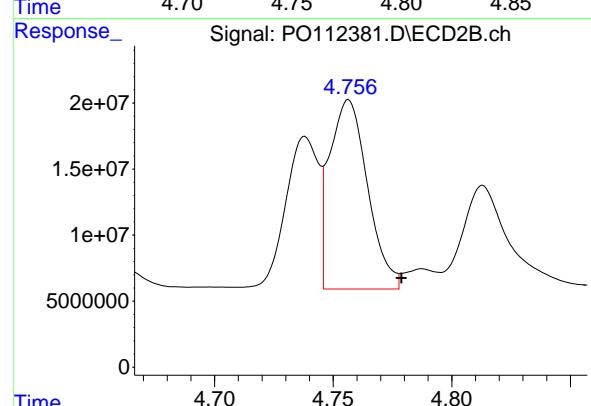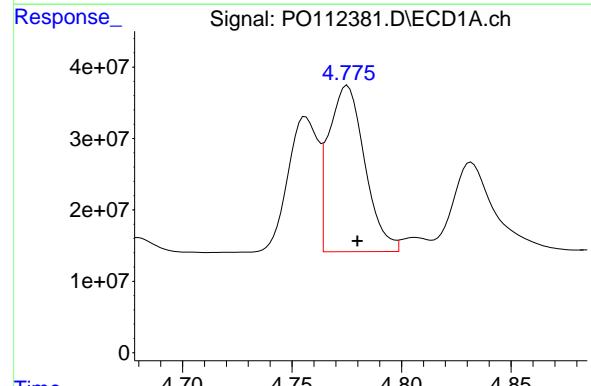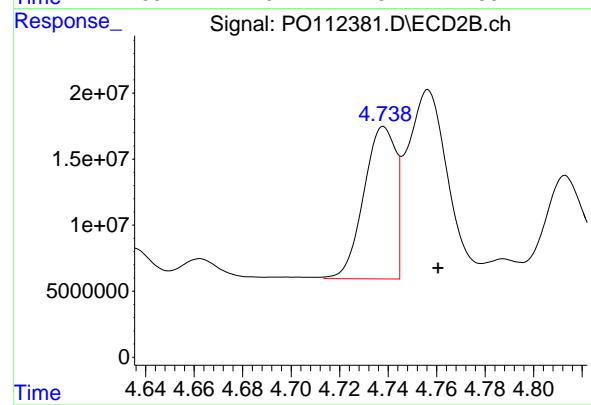


#4 AR-1016-2

R.T.: 4.775 min
 Delta R.T.: -0.005 min
 Response: 267507791
 Conc: 537.93 ng/ml

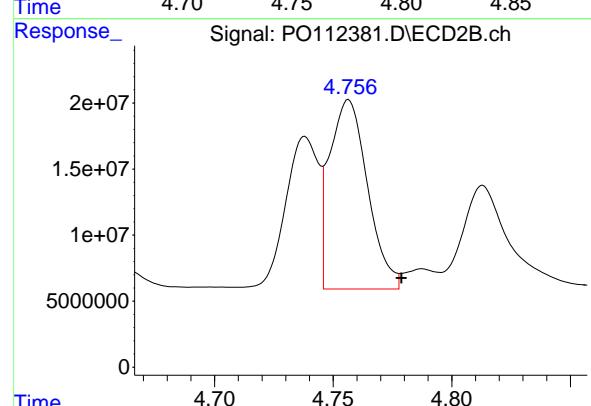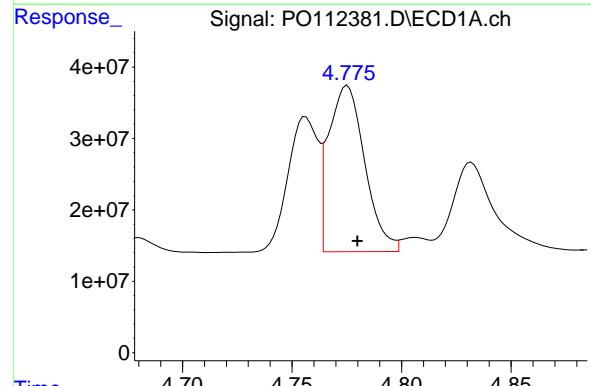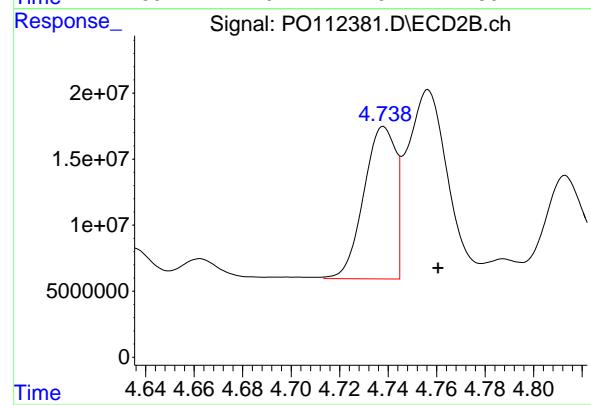

#4 AR-1016-2

R.T.: 4.756 min
 Delta R.T.: -0.023 min
 Response: 157661241
 Conc: 479.07 ng/ml

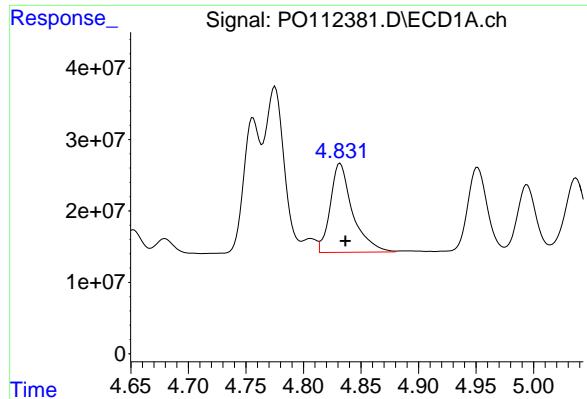


#5 AR-1016-3

R.T.: 4.832 min
Delta R.T.: -0.004 min
Response: 167757685
Conc: 518.23 ng/ml

Instrument: ECD_O
ClientSampleId: AR1660CCC500


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/23/2025
Supervised By :mohammad ahmed 07/24/2025

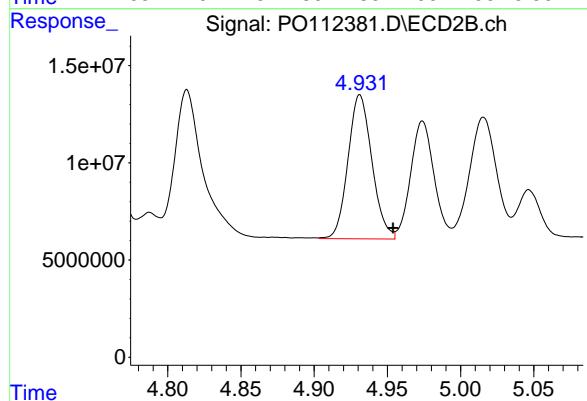


#5 AR-1016-3

R.T.: 4.931 min
Delta R.T.: -0.023 min
Response: 84329493
Conc: 496.44 ng/ml

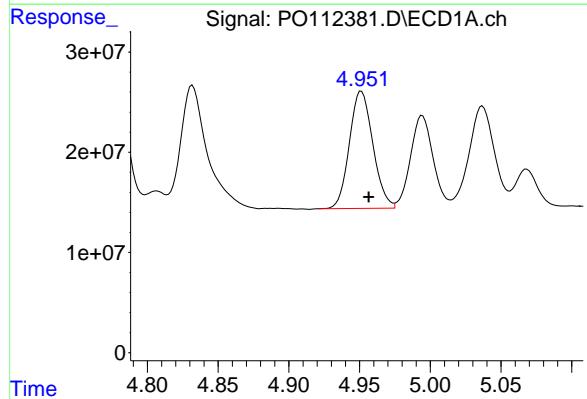


#6 AR-1016-4

R.T.: 4.951 min
Delta R.T.: -0.005 min
Response: 135250965
Conc: 526.68 ng/ml

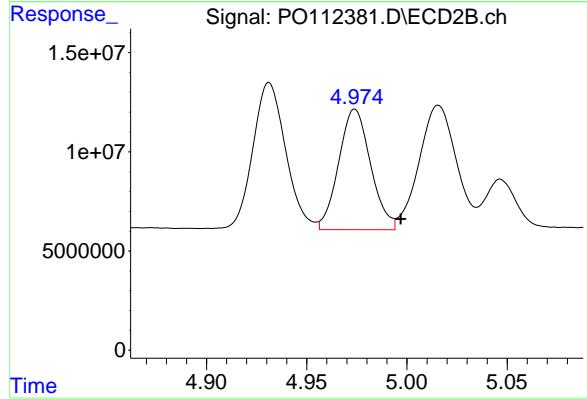

#6 AR-1016-4

R.T.: 4.974 min
Delta R.T.: -0.023 min
Response: 67538407
Conc: 492.16 ng/ml

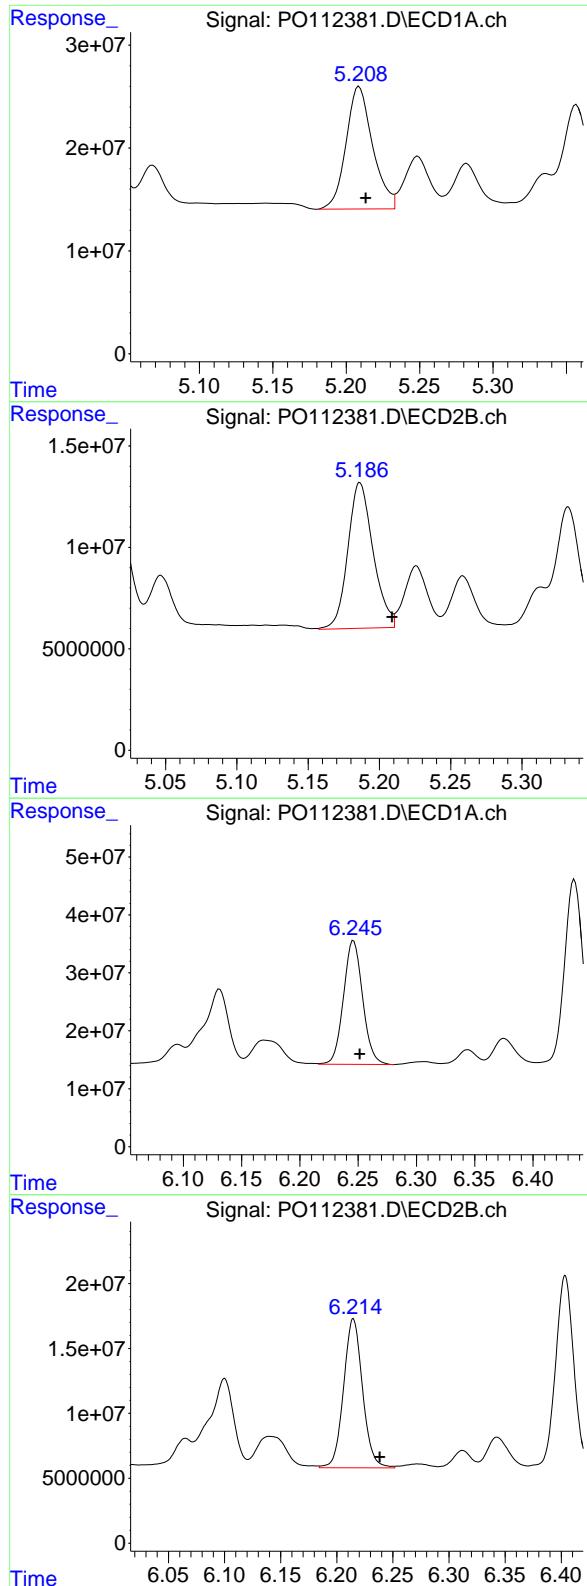

#7 AR-1016-5

R.T.: 5.209 min
 Delta R.T.: -0.004 min
 Response: 150287384
 Conc: 549.17 ng/ml

Instrument:
 ECD_O
 ClientSampleId :
 AR1660CCC500

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/23/2025
 Supervised By :mohammad ahmed 07/24/2025

#7 AR-1016-5


R.T.: 5.186 min
 Delta R.T.: -0.023 min
 Response: 89062171
 Conc: 516.45 ng/ml

#31 AR-1260-1

R.T.: 6.246 min
 Delta R.T.: -0.005 min
 Response: 244719104
 Conc: 488.23 ng/ml

#31 AR-1260-1

R.T.: 6.215 min
 Delta R.T.: -0.023 min
 Response: 135145555
 Conc: 481.70 ng/ml

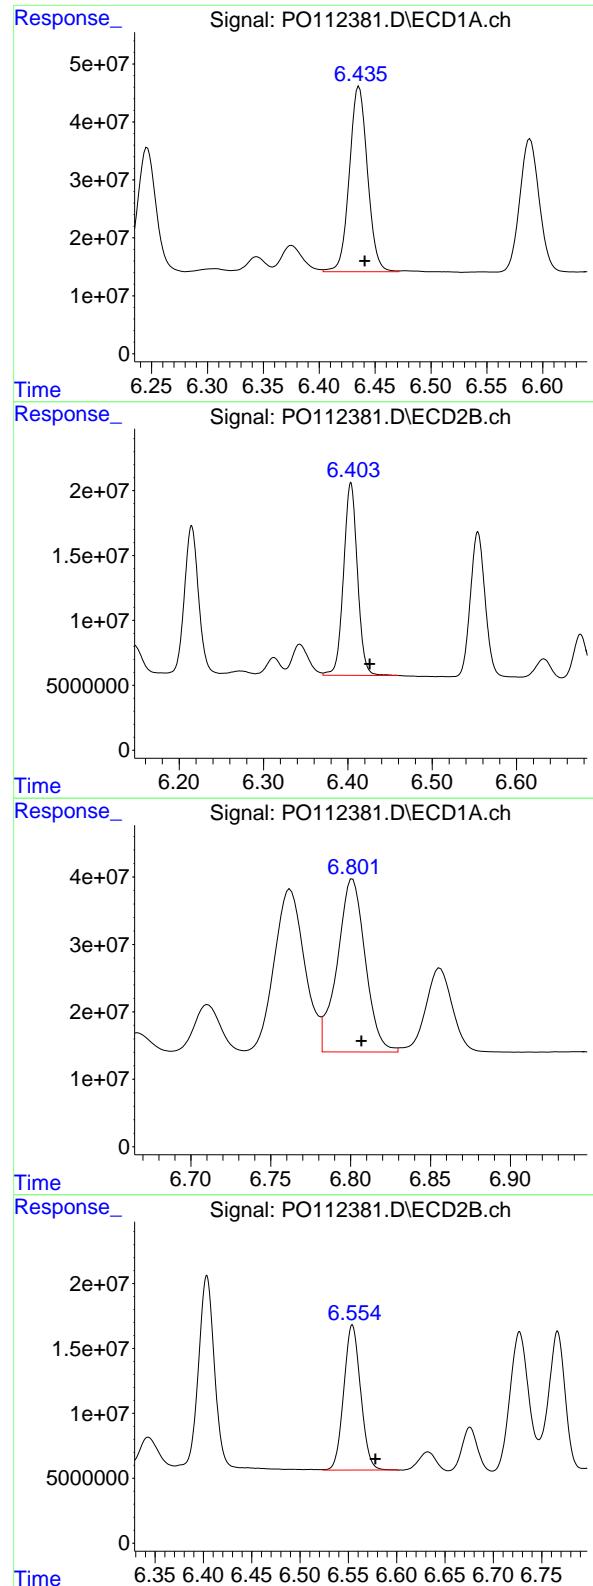

#32 AR-1260-2

R.T.: 6.436 min
 Delta R.T.: -0.005 min
 Response: 360404699
 Conc: 488.26 ng/ml

Instrument: ECD_O
 ClientSampleId: AR1660CCC500

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/23/2025
 Supervised By :mohammad ahmed 07/24/2025

#32 AR-1260-2


R.T.: 6.404 min
 Delta R.T.: -0.022 min
 Response: 169754475
 Conc: 499.28 ng/ml

#33 AR-1260-3

R.T.: 6.801 min
 Delta R.T.: -0.005 min
 Response: 313295711
 Conc: 477.96 ng/ml

#33 AR-1260-3

R.T.: 6.554 min
 Delta R.T.: -0.024 min
 Response: 135715722
 Conc: 492.46 ng/ml

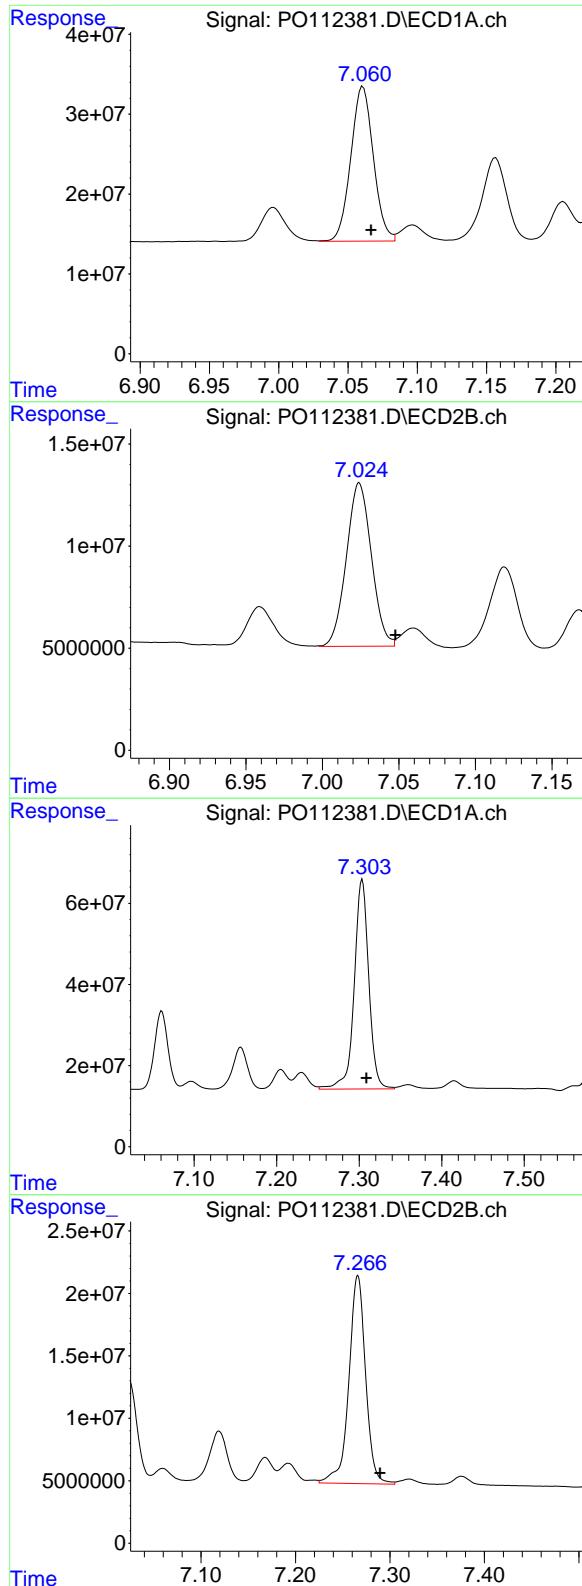

#34 AR-1260-4

R.T.: 7.061 min
 Delta R.T.: -0.006 min
 Response: 219427950
 Conc: 504.14 ng/ml

Instrument: ECD_O
 ClientSampleId: AR1660CCC500

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/23/2025
 Supervised By :mohammad ahmed 07/24/2025

#34 AR-1260-4

R.T.: 7.024 min
 Delta R.T.: -0.024 min
 Response: 91343921
 Conc: 455.25 ng/ml

#35 AR-1260-5

R.T.: 7.304 min
 Delta R.T.: -0.005 min
 Response: 633483438
 Conc: 501.75 ng/ml

#35 AR-1260-5

R.T.: 7.266 min
 Delta R.T.: -0.024 min
 Response: 205628634
 Conc: 459.27 ng/ml



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Lab Name: Alliance

Contract: NOBI03

Lab Code: ACE

SDG NO.: Q2639

Continuing Calib Date: 07/21/2025

Initial Calibration Date(s): 07/07/2025

07/08/2025

Continuing Calib Time: 08:51

Initial Calibration Time(s): 21:03

04:24

GC Column: ZB-MR1

ID: 0.32 (mm)

COMPOUND	CCAL RT	AVG RT	RT WINDOW FROM	TO	DIFF RT
Aroclor-1016-1 (1)	5.63	5.64	5.54	5.74	0.01
Aroclor-1016-2 (2)	5.65	5.66	5.56	5.76	0.01
Aroclor-1016-3 (3)	5.72	5.72	5.62	5.82	0.00
Aroclor-1016-4 (4)	5.81	5.82	5.72	5.92	0.01
Aroclor-1016-5 (5)	6.11	6.11	6.01	6.21	0.00
Aroclor-1260-1 (1)	7.22	7.23	7.13	7.33	0.01
Aroclor-1260-2 (2)	7.48	7.48	7.38	7.58	0.00
Aroclor-1260-3 (3)	7.83	7.84	7.74	7.94	0.01
Aroclor-1260-4 (4)	8.06	8.06	7.96	8.16	0.00
Aroclor-1260-5 (5)	8.38	8.38	8.28	8.48	0.00
Tetrachloro-m-xylene	4.48	4.49	4.39	4.59	0.01
Decachlorobiphenyl	10.17	10.18	10.08	10.28	0.01



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Lab Name: Alliance

Contract: NOBI03

Lab Code: ACE

SDG NO.: Q2639

Continuing Calib Date: 07/21/2025

Initial Calibration Date(s): 07/07/2025

07/08/2025

Continuing Calib Time: 08:51

Initial Calibration Time(s): 21:03

04:24

GC Column: ZB-MR2

ID: 0.32 (mm)

COMPOUND	CCAL RT	Avg RT	RT Window From	TO	Diff RT
Aroclor-1016-1 (1)	4.85	4.86	4.76	4.96	0.01
Aroclor-1016-2 (2)	4.87	4.88	4.78	4.98	0.01
Aroclor-1016-3 (3)	5.04	5.05	4.95	5.15	0.01
Aroclor-1016-4 (4)	5.09	5.09	4.99	5.19	0.00
Aroclor-1016-5 (5)	5.30	5.31	5.21	5.41	0.01
Aroclor-1260-1 (1)	6.33	6.34	6.24	6.44	0.01
Aroclor-1260-2 (2)	6.52	6.53	6.43	6.63	0.01
Aroclor-1260-3 (3)	6.67	6.68	6.58	6.78	0.01
Aroclor-1260-4 (4)	7.14	7.15	7.05	7.25	0.01
Aroclor-1260-5 (5)	7.38	7.39	7.29	7.49	0.01
Tetrachloro-m-xylene	3.77	3.78	3.68	3.88	0.01
Decachlorobiphenyl	8.77	8.78	8.68	8.88	0.01



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900, Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Lab Name:	Alliance	Contract:	NOBI03
Lab Code:	ACE	SDG NO.:	Q2639
GC Column:	ZB-MR1	ID: 0.32 (mm)	Initi. Calib. Date(s): 07/07/2025 07/07/2025

Client Sample No.:	CCAL05	Date Analyzed:	07/21/2025
Lab Sample No.:	AR1660CCC500	Data File :	PP073972.D
		Time Analyzed:	08:51

COMPOUND	RT	RT WINDOW FROM TO		CALC AMOUNT(ng)	NOM AMOUNT(ng)	%D
Aroclor-1016-1	5.633	5.539	5.739	451.720	500.000	-9.7
Aroclor-1016-2	5.654	5.560	5.760	488.530	500.000	-2.3
Aroclor-1016-3	5.716	5.622	5.822	479.600	500.000	-4.1
Aroclor-1016-4	5.814	5.720	5.920	483.450	500.000	-3.3
Aroclor-1016-5	6.106	6.012	6.212	488.110	500.000	-2.4
Aroclor-1260-1	7.223	7.129	7.329	470.410	500.000	-5.9
Aroclor-1260-2	7.476	7.383	7.583	429.810	500.000	-14.0
Aroclor-1260-3	7.834	7.740	7.940	494.290	500.000	-1.1
Aroclor-1260-4	8.057	7.964	8.164	508.080	500.000	1.6
Aroclor-1260-5	8.375	8.283	8.483	513.090	500.000	2.6
Decachlorobiphenyl	10.166	10.076	10.276	53.820	50.000	7.6
Tetrachloro-m-xylene	4.482	4.388	4.588	51.200	50.000	2.4



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900, Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Lab Name:	<u>Alliance</u>	Contract:	<u>NOBI03</u>
Lab Code:	<u>ACE</u>	SDG NO.:	<u>Q2639</u>
GC Column:	<u>ZB-MR2</u>	ID: <u>0.32</u> (mm)	Initi. Calib. Date(s): <u>07/07/2025</u> <u>07/07/2025</u>

Client Sample No.:	<u>CCAL05</u>	Date Analyzed:	<u>07/21/2025</u>
Lab Sample No.:	<u>AR1660CCC500</u>	Data File :	<u>PP073972.D</u>
		Time Analyzed:	<u>08:51</u>

COMPOUND	RT	RT WINDOW FROM	TO	CALC AMOUNT(ng)	NOM AMOUNT(ng)	%D
Aroclor-1016-1	4.849	4.758	4.958	471.860	500.000	-5.6
Aroclor-1016-2	4.867	4.775	4.975	478.870	500.000	-4.2
Aroclor-1016-3	5.043	4.951	5.151	489.440	500.000	-2.1
Aroclor-1016-4	5.085	4.993	5.193	487.850	500.000	-2.4
Aroclor-1016-5	5.298	5.207	5.407	494.440	500.000	-1.1
Aroclor-1260-1	6.328	6.237	6.437	472.030	500.000	-5.6
Aroclor-1260-2	6.516	6.425	6.625	470.640	500.000	-5.9
Aroclor-1260-3	6.668	6.577	6.777	469.520	500.000	-6.1
Aroclor-1260-4	7.137	7.046	7.246	489.920	500.000	-2.0
Aroclor-1260-5	7.379	7.289	7.489	491.630	500.000	-1.7
Decachlorobiphenyl	8.769	8.680	8.880	55.590	50.000	11.2
Tetrachloro-m-xylene	3.772	3.678	3.878	48.690	50.000	-2.6

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP072125\
 Data File : PP073972.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jul 2025 08:51
 Operator : YP\AJ
 Sample : AR1660CCC500
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
AR1660CCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 22 01:44:10 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 08 08:35:32 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	4.482	3.772	70122852	89704759	51.202	48.692
2) SA Decachlor...	10.166	8.769	58718229	73552446	53.818	55.589

Target Compounds

3) L1 AR-1016-1	5.633	4.849	21462747	32168950	451.718	471.860
4) L1 AR-1016-2	5.654	4.867	34790309	48789605	488.526	478.872
5) L1 AR-1016-3	5.716	5.043	20940600	26481602	479.595	489.436
6) L1 AR-1016-4	5.814	5.085	17377876	21407444	483.450	487.854
7) L1 AR-1016-5	6.106	5.298	15292750	26987830	488.112	494.441
31) L7 AR-1260-1	7.223	6.328	27735757	46051101	470.407	472.027
32) L7 AR-1260-2	7.476	6.516	41192512	57811705	429.806	470.635
33) L7 AR-1260-3	7.834	6.668	36118391	51395792	494.294	469.523
34) L7 AR-1260-4	8.057	7.137	33177678	43803186	508.082	489.922
35) L7 AR-1260-5	8.375	7.379	77401624	110.5E6	513.094	491.630



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP072125\
 Data File : PP073972.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jul 2025 08:51
 Operator : YP\AJ
 Sample : AR1660CCC500
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 AR1660CCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 22 01:44:10 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 08 08:35:32 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

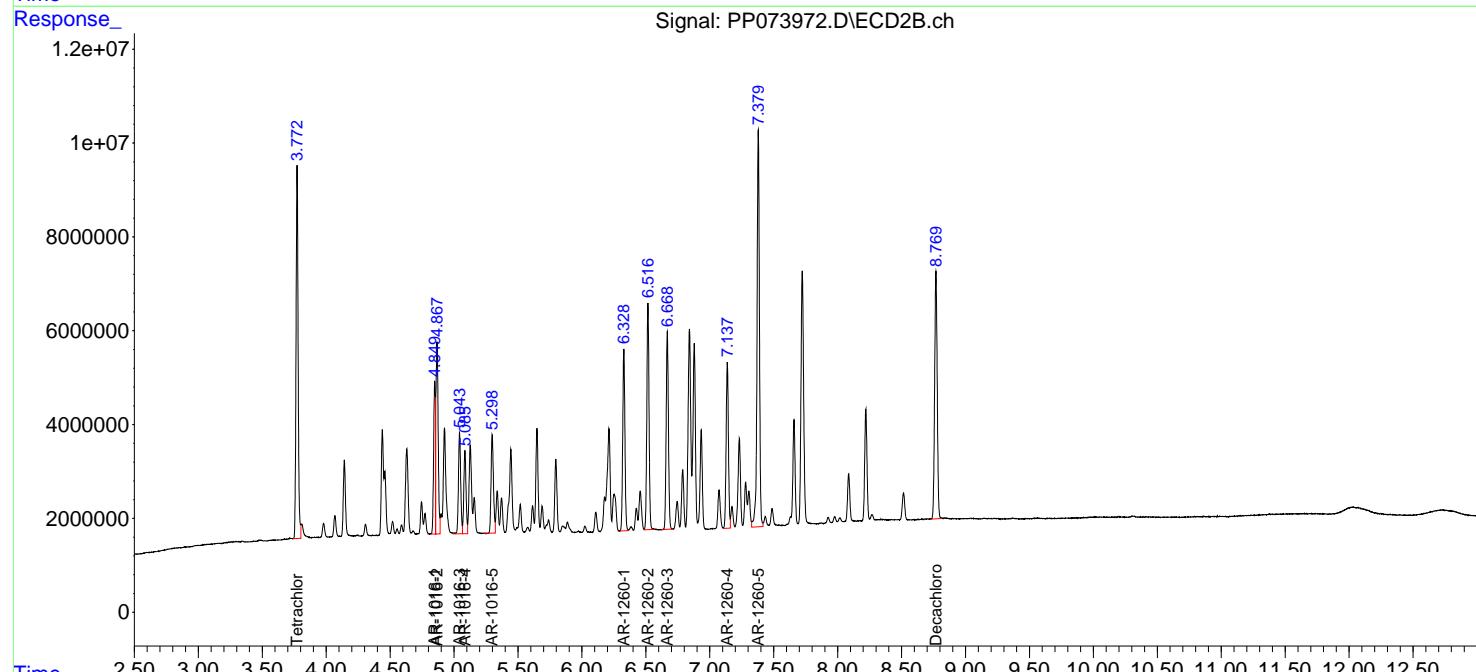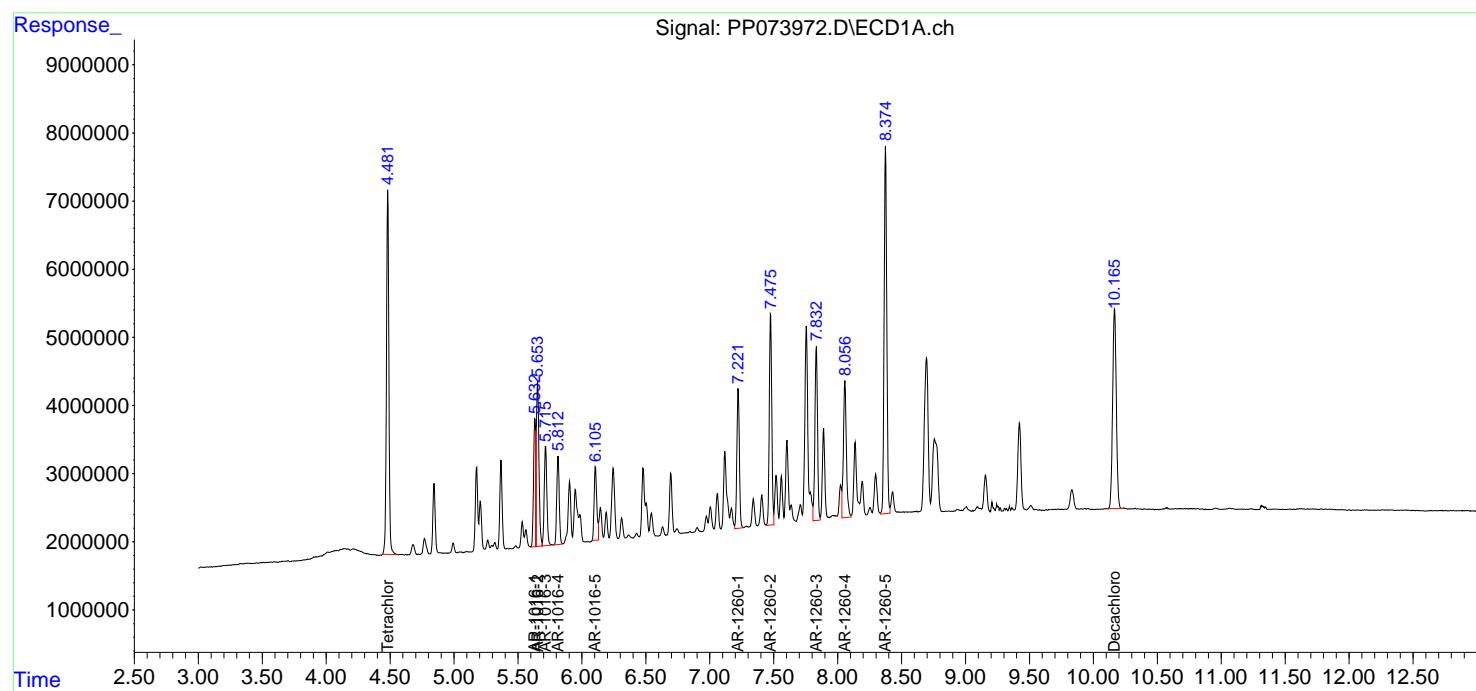


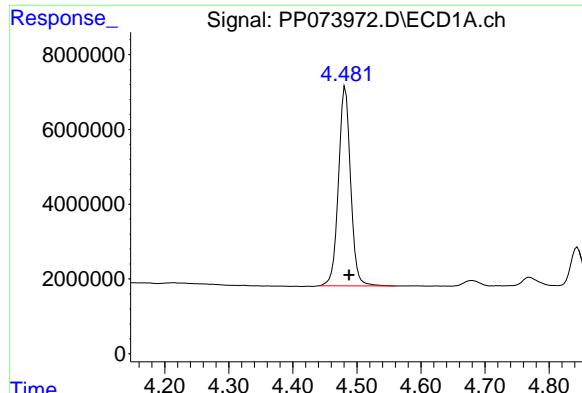

#1 Tetrachloro-m-xylene


R.T.: 4.482 min
 Delta R.T.: -0.006 min
 Response: 70122852
 Conc: 51.20 ng/ml

Instrument: ECD_P
 ClientSampleId: AR1660CCC500

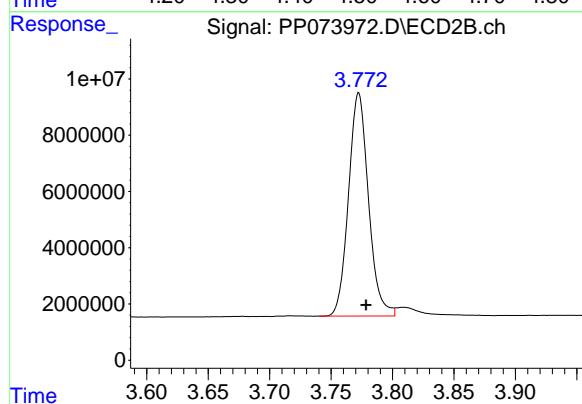


#1 Tetrachloro-m-xylene

R.T.: 3.772 min
 Delta R.T.: -0.006 min
 Response: 89704759
 Conc: 48.69 ng/ml

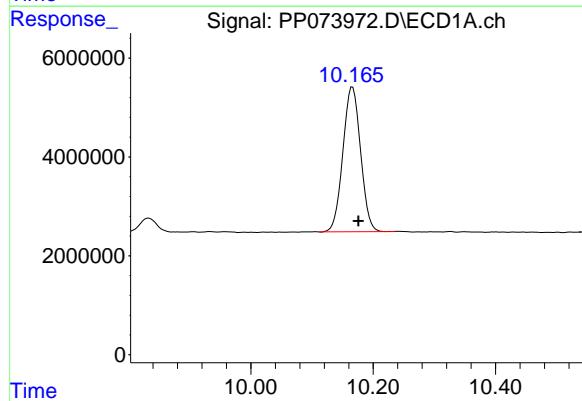


#2 Decachlorobiphenyl

R.T.: 10.166 min
 Delta R.T.: -0.010 min
 Response: 58718229
 Conc: 53.82 ng/ml

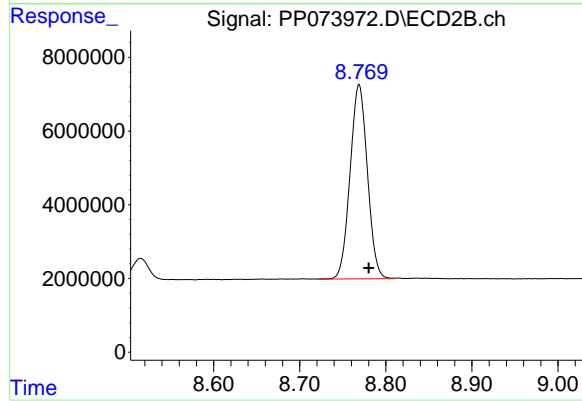

#2 Decachlorobiphenyl

R.T.: 8.769 min
 Delta R.T.: -0.011 min
 Response: 73552446
 Conc: 55.59 ng/ml

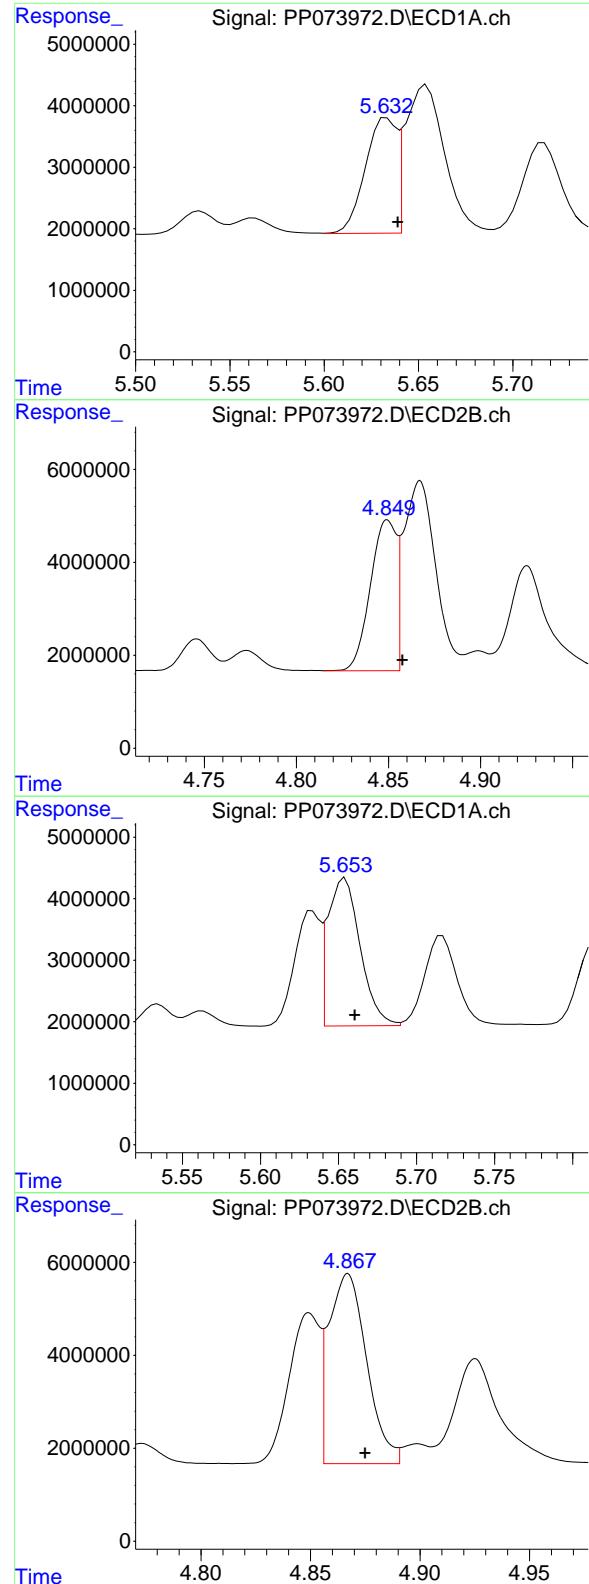

#3 AR-1016-1

R.T.: 5.633 min
 Delta R.T.: -0.006 min
 Response: 21462747
 Conc: 451.72 ng/ml

Instrument: ECD_P
 ClientSampleId: AR1660CCC500

#3 AR-1016-1


R.T.: 4.849 min
 Delta R.T.: -0.008 min
 Response: 32168950
 Conc: 471.86 ng/ml

#4 AR-1016-2

R.T.: 5.654 min
 Delta R.T.: -0.006 min
 Response: 34790309
 Conc: 488.53 ng/ml

#4 AR-1016-2

R.T.: 4.867 min
 Delta R.T.: -0.008 min
 Response: 48789605
 Conc: 478.87 ng/ml

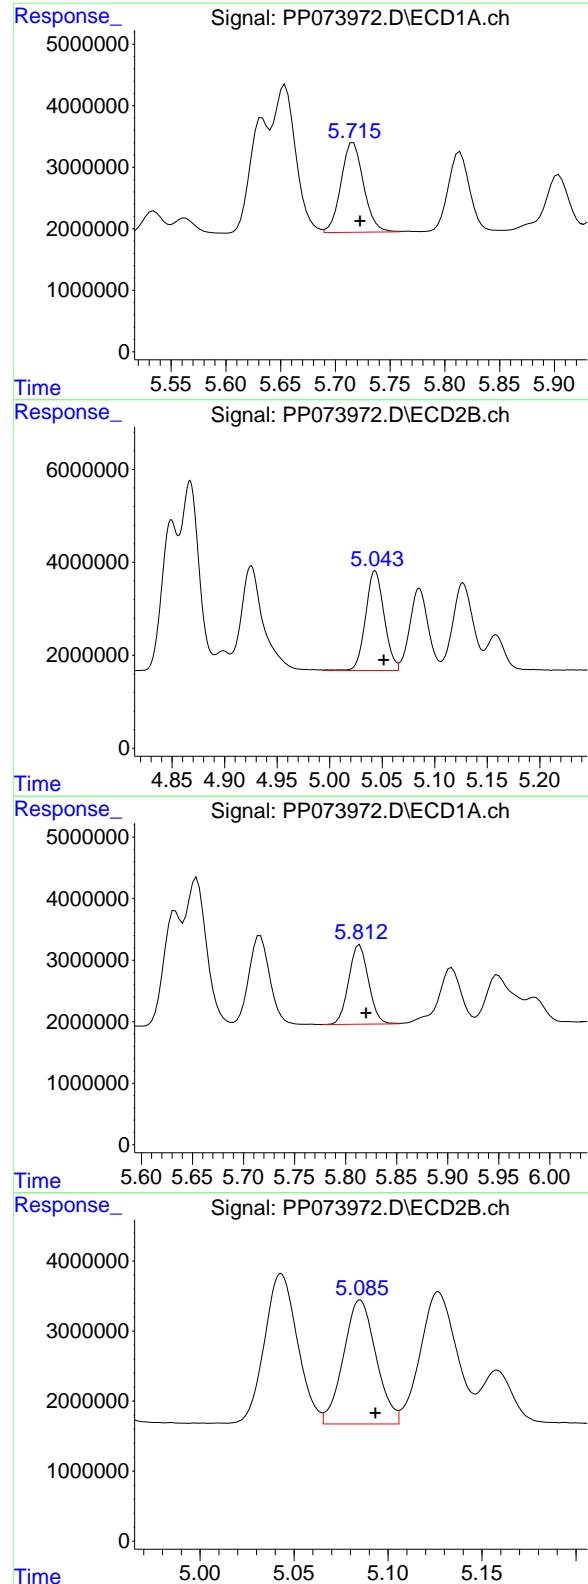

#5 AR-1016-3

R.T.: 5.716 min
 Delta R.T.: -0.006 min
 Response: 20940600
 Conc: 479.60 ng/ml

Instrument: ECD_P
 ClientSampleId: AR1660CCC500

#5 AR-1016-3


R.T.: 5.043 min
 Delta R.T.: -0.008 min
 Response: 26481602
 Conc: 489.44 ng/ml

#6 AR-1016-4

R.T.: 5.814 min
 Delta R.T.: -0.006 min
 Response: 17377876
 Conc: 483.45 ng/ml

#6 AR-1016-4

R.T.: 5.085 min
 Delta R.T.: -0.008 min
 Response: 21407444
 Conc: 487.85 ng/ml

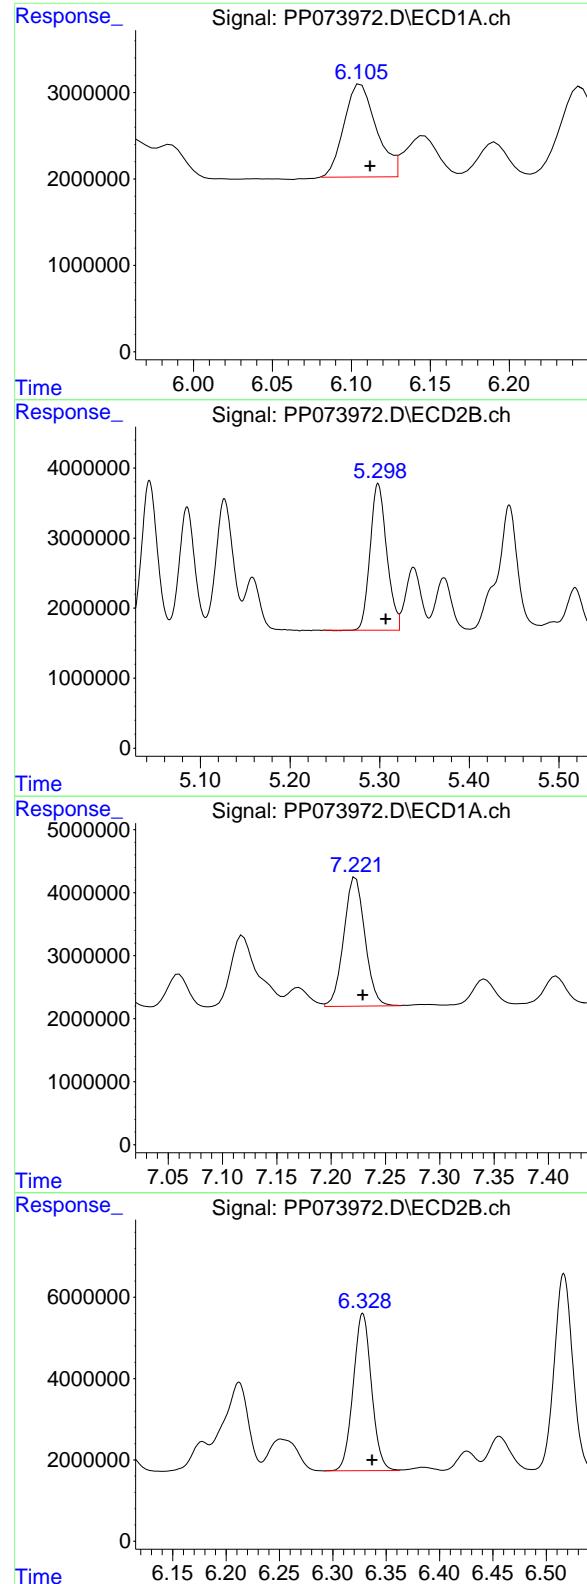

#7 AR-1016-5

R.T.: 6.106 min
 Delta R.T.: -0.006 min
 Response: 15292750
 Conc: 488.11 ng/ml

Instrument: ECD_P
 ClientSampleId: AR1660CCC500

#7 AR-1016-5



R.T.: 5.298 min
 Delta R.T.: -0.009 min
 Response: 26987830
 Conc: 494.44 ng/ml

#31 AR-1260-1

R.T.: 7.223 min
 Delta R.T.: -0.006 min
 Response: 27735757
 Conc: 470.41 ng/ml

#31 AR-1260-1

R.T.: 6.328 min
 Delta R.T.: -0.009 min
 Response: 46051101
 Conc: 472.03 ng/ml

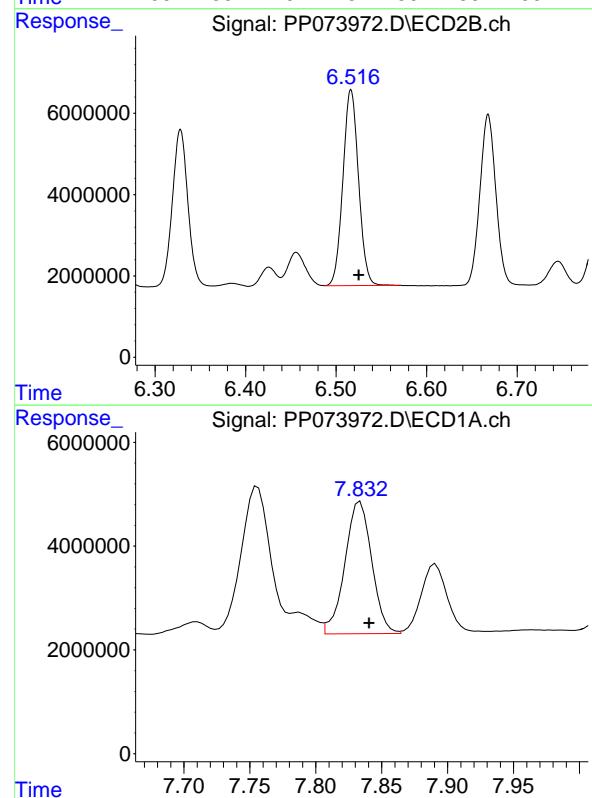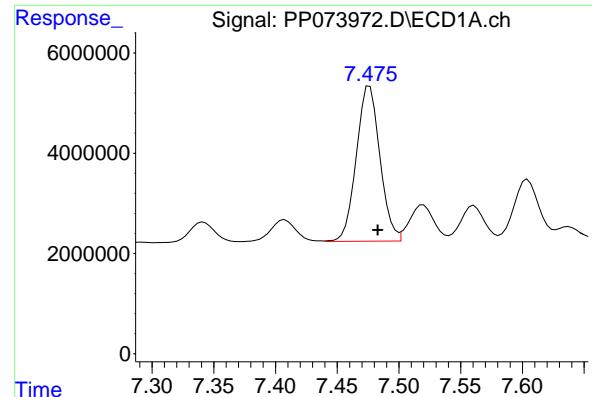

#32 AR-1260-2

R.T.: 7.476 min
 Delta R.T.: -0.006 min
 Response: 41192512
 Conc: 429.81 ng/ml

Instrument: ECD_P
 ClientSampleId: AR1660CCC500

#32 AR-1260-2


R.T.: 6.516 min
 Delta R.T.: -0.009 min
 Response: 57811705
 Conc: 470.64 ng/ml

#33 AR-1260-3

R.T.: 7.834 min
 Delta R.T.: -0.007 min
 Response: 36118391
 Conc: 494.29 ng/ml

#33 AR-1260-3

R.T.: 6.668 min
 Delta R.T.: -0.009 min
 Response: 51395792
 Conc: 469.52 ng/ml

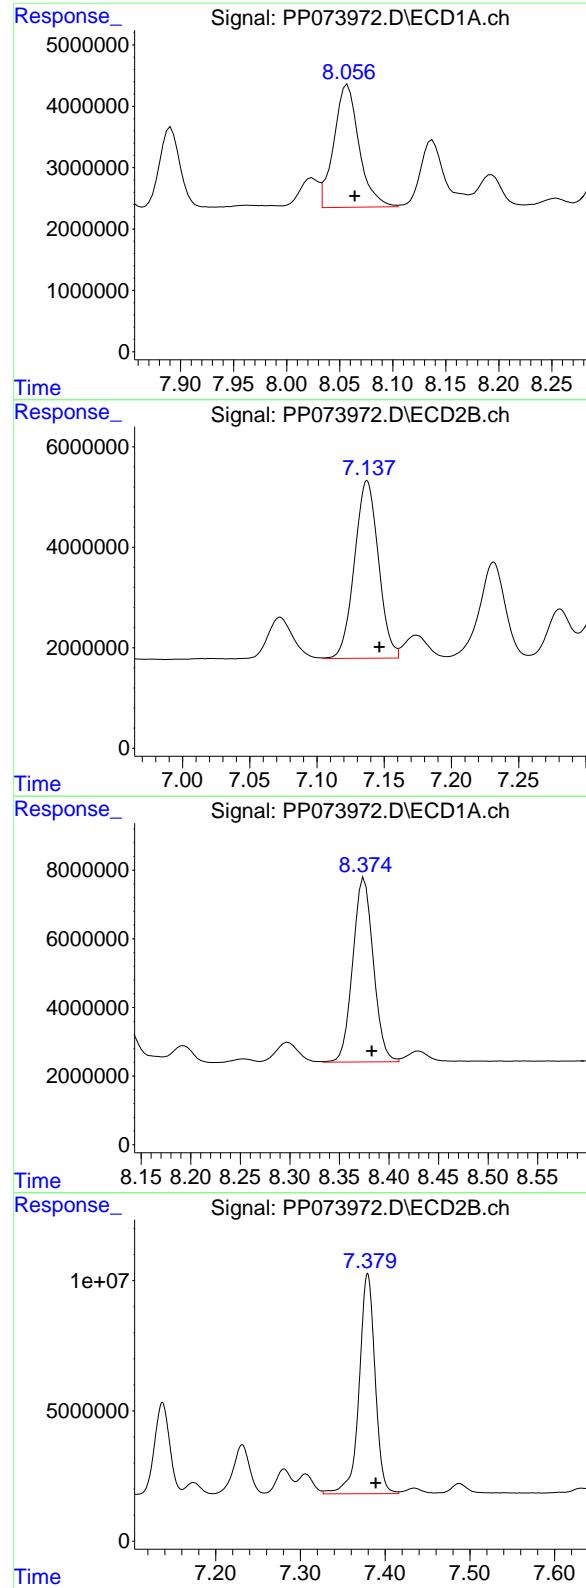

#34 AR-1260-4

R.T.: 8.057 min
 Delta R.T.: -0.007 min
 Response: 33177678
 Conc: 508.08 ng/ml

Instrument: ECD_P
 ClientSampleId: AR1660CCC500

#34 AR-1260-4

R.T.: 7.137 min
 Delta R.T.: -0.009 min
 Response: 43803186
 Conc: 489.92 ng/ml

#35 AR-1260-5

R.T.: 8.375 min
 Delta R.T.: -0.008 min
 Response: 77401624
 Conc: 513.09 ng/ml

#35 AR-1260-5

R.T.: 7.379 min
 Delta R.T.: -0.009 min
 Response: 110487282
 Conc: 491.63 ng/ml



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Lab Name: Alliance

Contract: NOBI03

Lab Code: ACE

SDG NO.: Q2639

Continuing Calib Date: 07/21/2025

Initial Calibration Date(s): 07/07/2025

07/08/2025

Continuing Calib Time: 15:18

Initial Calibration Time(s): 21:03

04:24

GC Column: ZB-MR1

ID: 0.32 (mm)

COMPOUND	CCAL RT	AVG RT	RT WINDOW FROM	TO	DIFF RT
Aroclor-1016-1 (1)	5.63	5.64	5.54	5.74	0.01
Aroclor-1016-2 (2)	5.66	5.66	5.56	5.76	0.00
Aroclor-1016-3 (3)	5.72	5.72	5.62	5.82	0.00
Aroclor-1016-4 (4)	5.82	5.82	5.72	5.92	0.00
Aroclor-1016-5 (5)	6.11	6.11	6.01	6.21	0.00
Aroclor-1260-1 (1)	7.22	7.23	7.13	7.33	0.01
Aroclor-1260-2 (2)	7.48	7.48	7.38	7.58	0.00
Aroclor-1260-3 (3)	7.84	7.84	7.74	7.94	0.00
Aroclor-1260-4 (4)	8.06	8.06	7.96	8.16	0.00
Aroclor-1260-5 (5)	8.38	8.38	8.28	8.48	0.00
Tetrachloro-m-xylene	4.48	4.49	4.39	4.59	0.01
Decachlorobiphenyl	10.17	10.18	10.08	10.28	0.01



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Lab Name: Alliance

Contract: NOBI03

Lab Code: ACE

SDG NO.: Q2639

Continuing Calib Date: 07/21/2025

Initial Calibration Date(s): 07/07/2025

07/08/2025

Continuing Calib Time: 15:18

Initial Calibration Time(s): 21:03

04:24

GC Column: ZB-MR2

ID: 0.32 (mm)

COMPOUND	CCAL RT	AVG RT	RT WINDOW FROM	TO	DIFF RT
Aroclor-1016-1 (1)	4.85	4.86	4.76	4.96	0.01
Aroclor-1016-2 (2)	4.87	4.88	4.78	4.98	0.01
Aroclor-1016-3 (3)	5.05	5.05	4.95	5.15	0.00
Aroclor-1016-4 (4)	5.09	5.09	4.99	5.19	0.00
Aroclor-1016-5 (5)	5.30	5.31	5.21	5.41	0.01
Aroclor-1260-1 (1)	6.33	6.34	6.24	6.44	0.01
Aroclor-1260-2 (2)	6.52	6.53	6.43	6.63	0.01
Aroclor-1260-3 (3)	6.67	6.68	6.58	6.78	0.01
Aroclor-1260-4 (4)	7.14	7.15	7.05	7.25	0.01
Aroclor-1260-5 (5)	7.38	7.39	7.29	7.49	0.01
Tetrachloro-m-xylene	3.77	3.78	3.68	3.88	0.01
Decachlorobiphenyl	8.77	8.78	8.68	8.88	0.01



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900, Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Lab Name:	<u>Alliance</u>	Contract:	<u>NOBI03</u>
Lab Code:	<u>ACE</u>	SDG NO.:	<u>Q2639</u>
GC Column:	<u>ZB-MR1</u>	ID: <u>0.32</u> (mm)	Initi. Calib. Date(s): <u>07/07/2025</u> <u>07/07/2025</u>

Client Sample No.:	<u>CCAL06</u>	Date Analyzed:	<u>07/21/2025</u>
Lab Sample No.:	<u>AR1660CCC500</u>	Data File :	<u>PP073987.D</u>
		Time Analyzed:	<u>15:18</u>

COMPOUND	RT	RT WINDOW FROM	TO	CALC AMOUNT(ng)	NOM AMOUNT(ng)	%D
Aroclor-1016-1	5.634	5.539	5.739	447.980	500.000	-10.4
Aroclor-1016-2	5.655	5.560	5.760	488.950	500.000	-2.2
Aroclor-1016-3	5.717	5.622	5.822	483.620	500.000	-3.3
Aroclor-1016-4	5.815	5.720	5.920	487.720	500.000	-2.5
Aroclor-1016-5	6.107	6.012	6.212	490.820	500.000	-1.8
Aroclor-1260-1	7.223	7.129	7.329	477.040	500.000	-4.6
Aroclor-1260-2	7.477	7.383	7.583	431.310	500.000	-13.7
Aroclor-1260-3	7.835	7.740	7.940	484.320	500.000	-3.1
Aroclor-1260-4	8.058	7.964	8.164	499.440	500.000	-0.1
Aroclor-1260-5	8.376	8.283	8.483	502.480	500.000	0.5
Decachlorobiphenyl	10.168	10.076	10.276	53.680	50.000	7.4
Tetrachloro-m-xylene	4.482	4.388	4.588	50.840	50.000	1.7



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900, Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Lab Name:	<u>Alliance</u>	Contract:	<u>NOBI03</u>
Lab Code:	<u>ACE</u>	SDG NO.:	<u>Q2639</u>
GC Column:	<u>ZB-MR2</u>	ID: <u>0.32</u> (mm)	Initi. Calib. Date(s): <u>07/07/2025</u> <u>07/07/2025</u>

Client Sample No.:	<u>CCAL06</u>	Date Analyzed:	<u>07/21/2025</u>
Lab Sample No.:	<u>AR1660CCC500</u>	Data File :	<u>PP073987.D</u>
		Time Analyzed:	<u>15:18</u>

COMPOUND	RT	RT WINDOW FROM	TO	CALC AMOUNT(ng)	NOM AMOUNT(ng)	%D
Aroclor-1016-1	4.851	4.758	4.958	523.290	500.000	4.7
Aroclor-1016-2	4.869	4.775	4.975	525.770	500.000	5.2
Aroclor-1016-3	5.045	4.951	5.151	530.150	500.000	6.0
Aroclor-1016-4	5.086	4.993	5.193	529.020	500.000	5.8
Aroclor-1016-5	5.301	5.207	5.407	537.530	500.000	7.5
Aroclor-1260-1	6.330	6.237	6.437	529.710	500.000	5.9
Aroclor-1260-2	6.519	6.425	6.625	534.970	500.000	7.0
Aroclor-1260-3	6.670	6.577	6.777	517.150	500.000	3.4
Aroclor-1260-4	7.139	7.046	7.246	539.350	500.000	7.9
Aroclor-1260-5	7.382	7.289	7.489	536.370	500.000	7.3
Decachlorobiphenyl	8.772	8.680	8.880	60.720	50.000	21.4
Tetrachloro-m-xylene	3.774	3.678	3.878	53.660	50.000	7.3

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP072125\
 Data File : PP073987.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jul 2025 15:18
 Operator : YP\AJ
 Sample : AR1660CCC500
 Misc :
 ALS Vial : 97 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
AR1660CCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 22 01:52:27 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 08 08:35:32 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	4.482	3.774	69631726	98851408	50.844	53.657
2) SA Decachlor...	10.168	8.772	58562821	80339742	53.676	60.719

Target Compounds

3) L1 AR-1016-1	5.634	4.851	21285031	35674841	447.978	523.285
4) L1 AR-1016-2	5.655	4.869	34820583	53567329	488.951	525.766
5) L1 AR-1016-3	5.717	5.045	21116147	28684318	483.616	530.147
6) L1 AR-1016-4	5.815	5.086	17531206	23214036	487.715	529.024
7) L1 AR-1016-5	6.107	5.301	15377637	29339780	490.821	537.531
31) L7 AR-1260-1	7.223	6.330	28126866	51678611	477.040	529.709
32) L7 AR-1260-2	7.477	6.519	41336288	65714064	431.306	534.967
33) L7 AR-1260-3	7.835	6.670	35389503	56609708	484.319	517.155
34) L7 AR-1260-4	8.058	7.139	32613157	48222670	499.437	539.353
35) L7 AR-1260-5	8.376	7.382	75800503	120.5E6	502.480	536.367



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.



Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP072125\
 Data File : PP073987.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jul 2025 15:18
 Operator : YP\AJ
 Sample : AR1660CCC500
 Misc :
 ALS Vial : 97 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 AR1660CCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 22 01:52:27 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 08 08:35:32 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

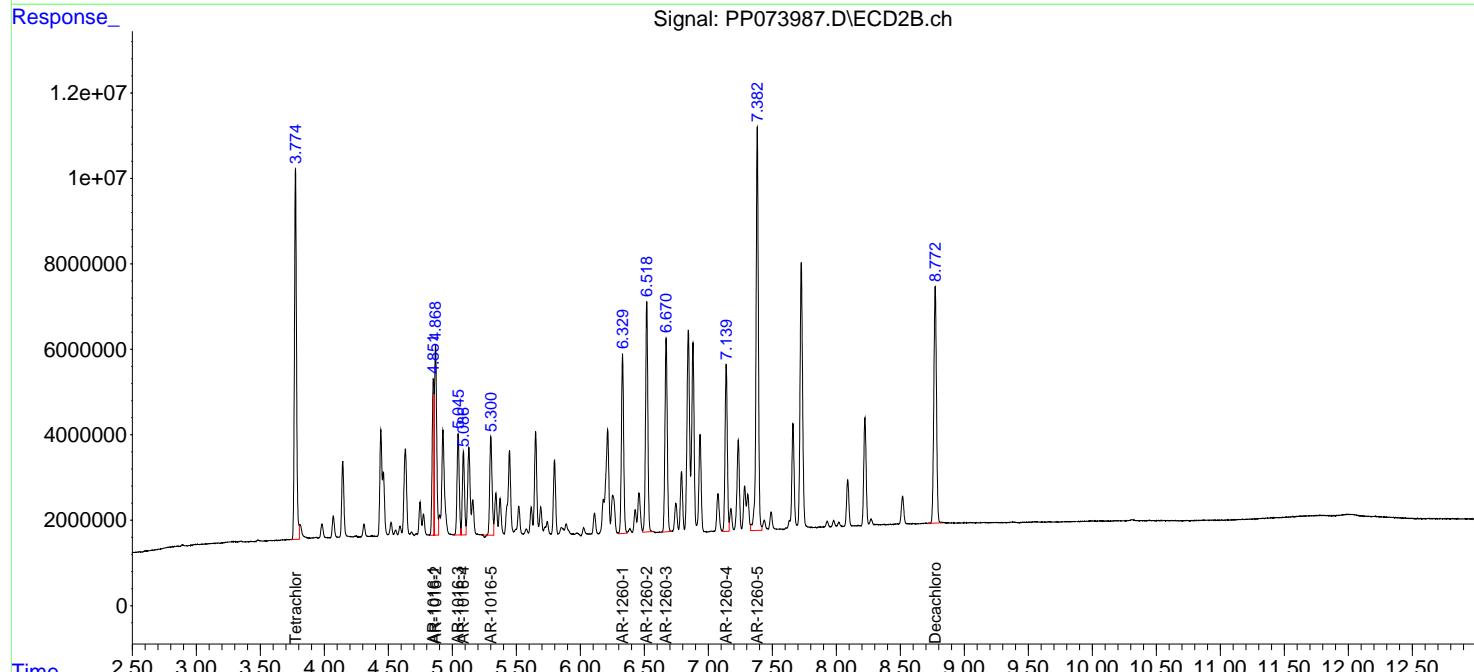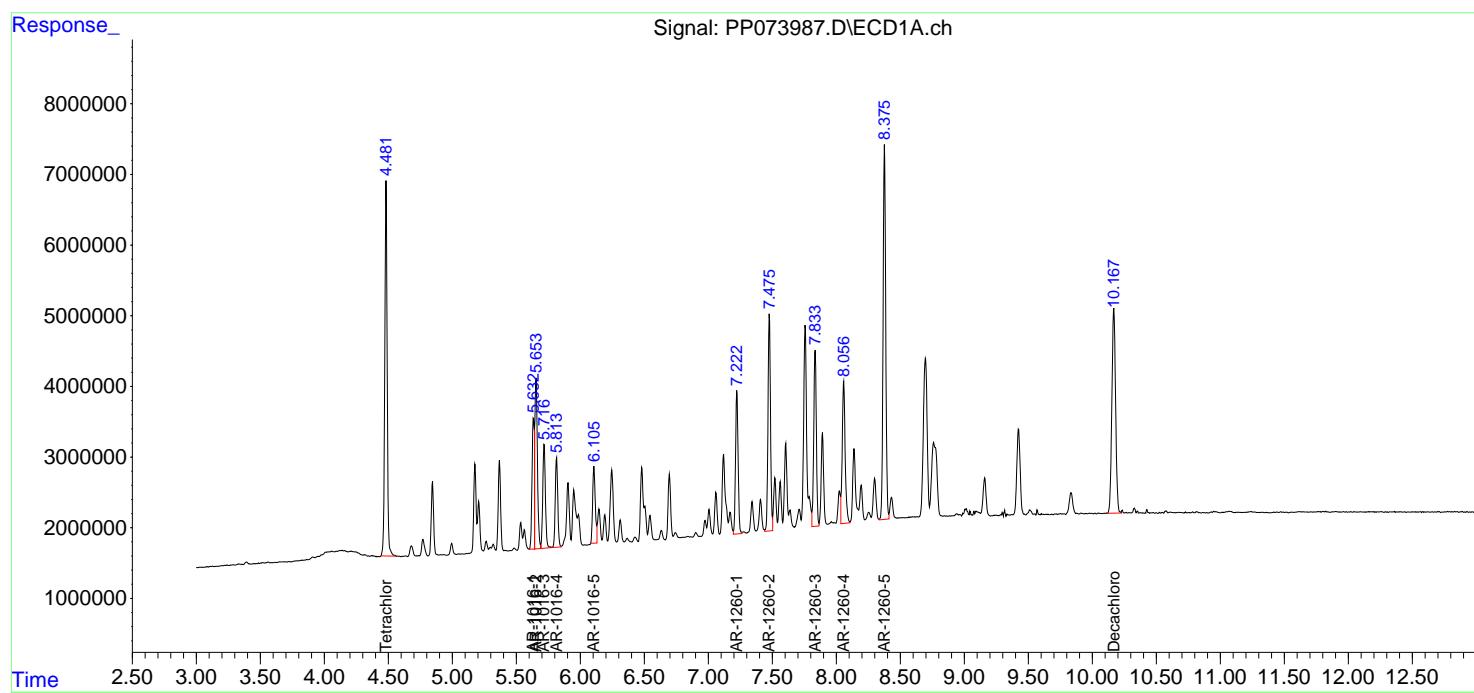

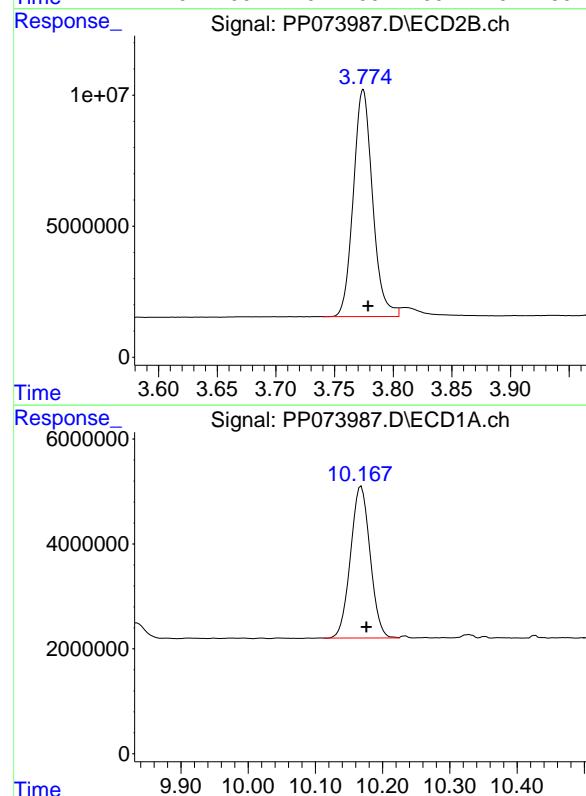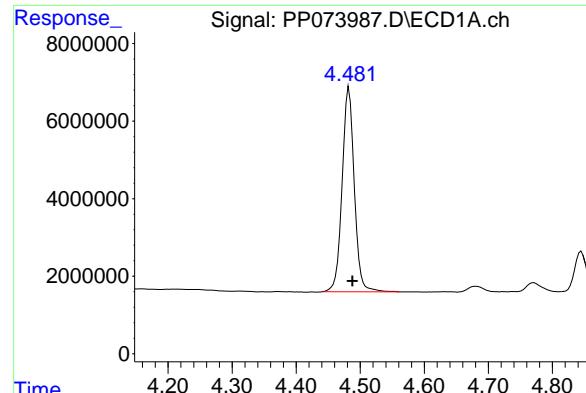

#1 Tetrachloro-m-xylene

R.T.: 4.482 min
Delta R.T.: -0.006 min
Response: 69631726
Conc: 50.84 ng/ml

Instrument: ECD_P
ClientSampleId: AR1660CCC500

#1 Tetrachloro-m-xylene





R.T.: 3.774 min
Delta R.T.: -0.004 min
Response: 98851408
Conc: 53.66 ng/ml

#2 Decachlorobiphenyl

R.T.: 10.168 min
Delta R.T.: -0.008 min
Response: 58562821
Conc: 53.68 ng/ml

#2 Decachlorobiphenyl

R.T.: 8.772 min
Delta R.T.: -0.008 min
Response: 80339742
Conc: 60.72 ng/ml

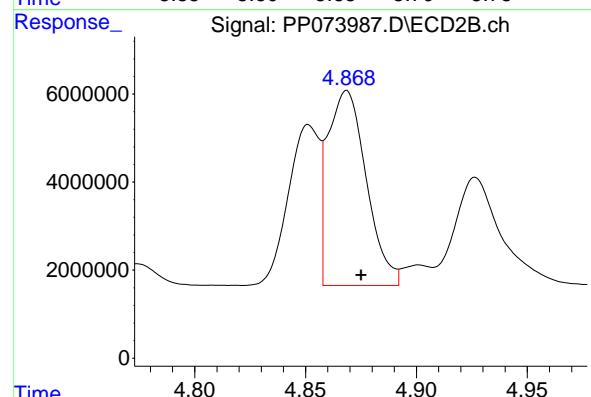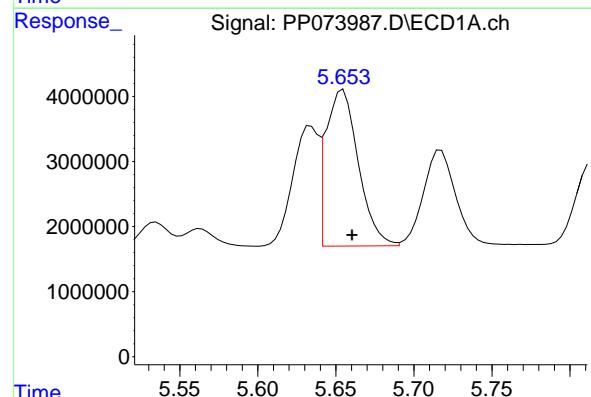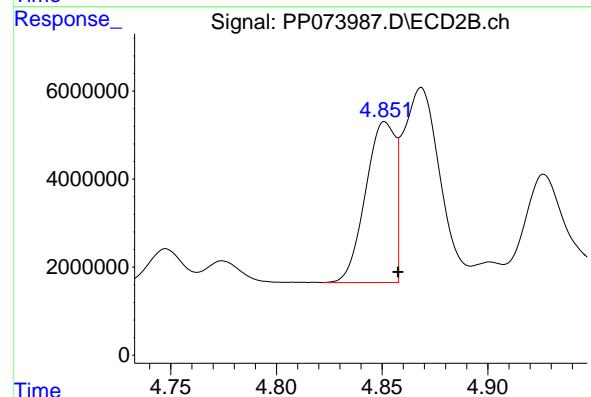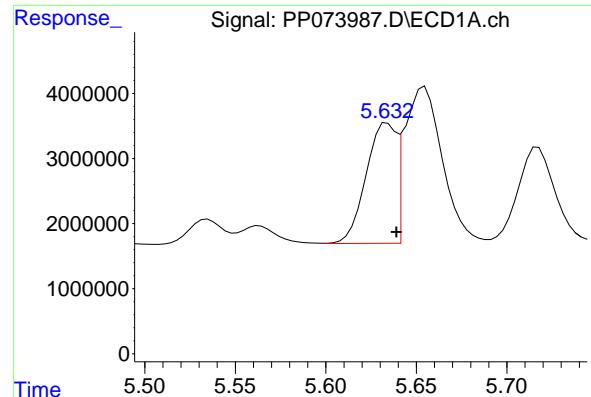

#3 AR-1016-1

R.T.: 5.634 min
 Delta R.T.: -0.005 min
 Response: 21285031
 Conc: 447.98 ng/ml

Instrument: ECD_P
 ClientSampleId: AR1660CCC500

#3 AR-1016-1


R.T.: 4.851 min
 Delta R.T.: -0.006 min
 Response: 35674841
 Conc: 523.29 ng/ml

#4 AR-1016-2

R.T.: 5.655 min
 Delta R.T.: -0.006 min
 Response: 34820583
 Conc: 488.95 ng/ml

#4 AR-1016-2

R.T.: 4.869 min
 Delta R.T.: -0.006 min
 Response: 53567329
 Conc: 525.77 ng/ml

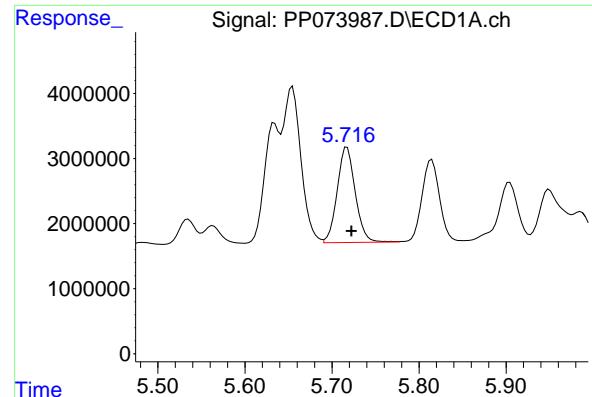

#5 AR-1016-3

R.T.: 5.717 min
 Delta R.T.: -0.005 min
 Response: 21116147
 Conc: 483.62 ng/ml

Instrument: ECD_P
 ClientSampleId: AR1660CCC500

#5 AR-1016-3


R.T.: 5.045 min
 Delta R.T.: -0.006 min
 Response: 28684318
 Conc: 530.15 ng/ml


#6 AR-1016-4

R.T.: 5.815 min
 Delta R.T.: -0.006 min
 Response: 17531206
 Conc: 487.72 ng/ml

#6 AR-1016-4

R.T.: 5.086 min
 Delta R.T.: -0.007 min
 Response: 23214036
 Conc: 529.02 ng/ml

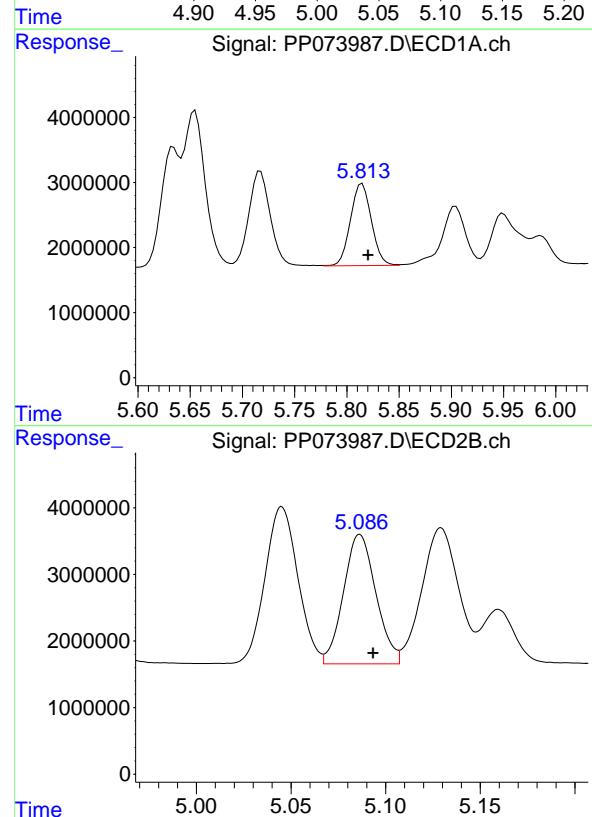

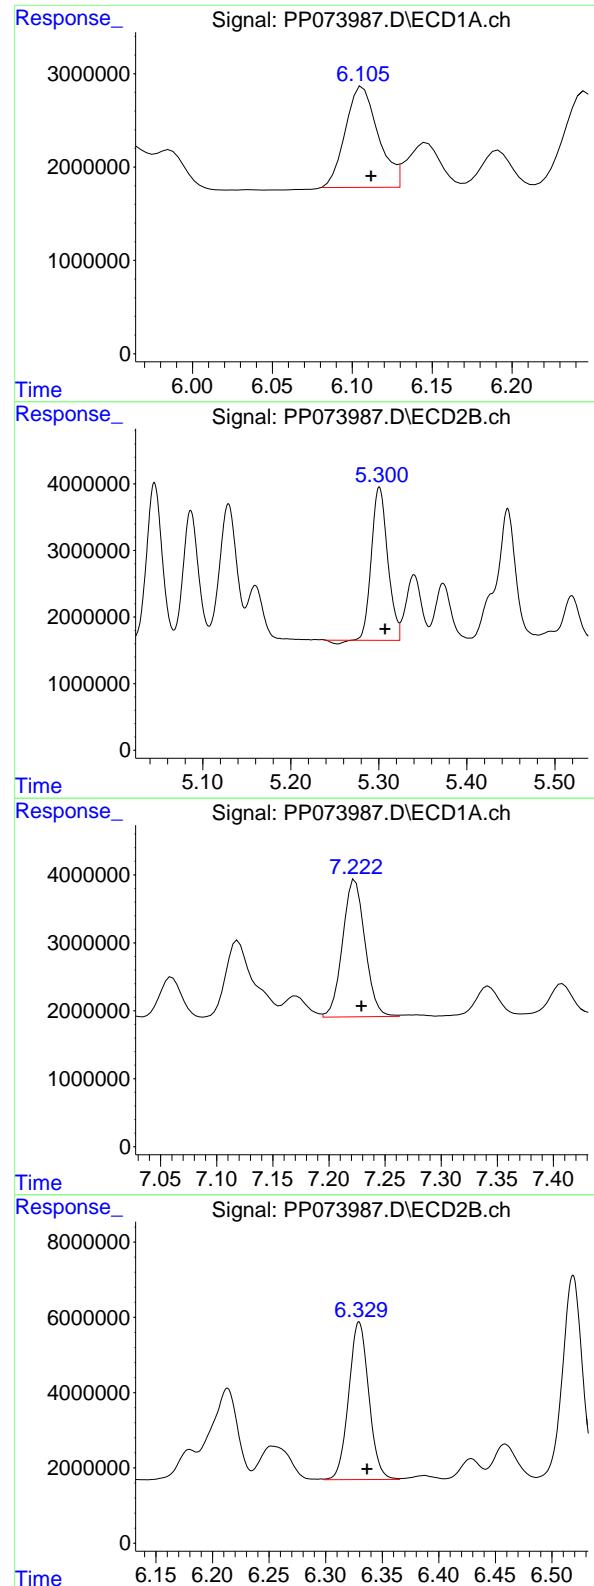

#7 AR-1016-5

R.T.: 6.107 min
 Delta R.T.: -0.005 min
 Response: 15377637
 Conc: 490.82 ng/ml

Instrument: ECD_P
 ClientSampleId: AR1660CCC500

#7 AR-1016-5


R.T.: 5.301 min
 Delta R.T.: -0.006 min
 Response: 29339780
 Conc: 537.53 ng/ml

#31 AR-1260-1

R.T.: 7.223 min
 Delta R.T.: -0.006 min
 Response: 28126866
 Conc: 477.04 ng/ml

#31 AR-1260-1

R.T.: 6.330 min
 Delta R.T.: -0.007 min
 Response: 51678611
 Conc: 529.71 ng/ml

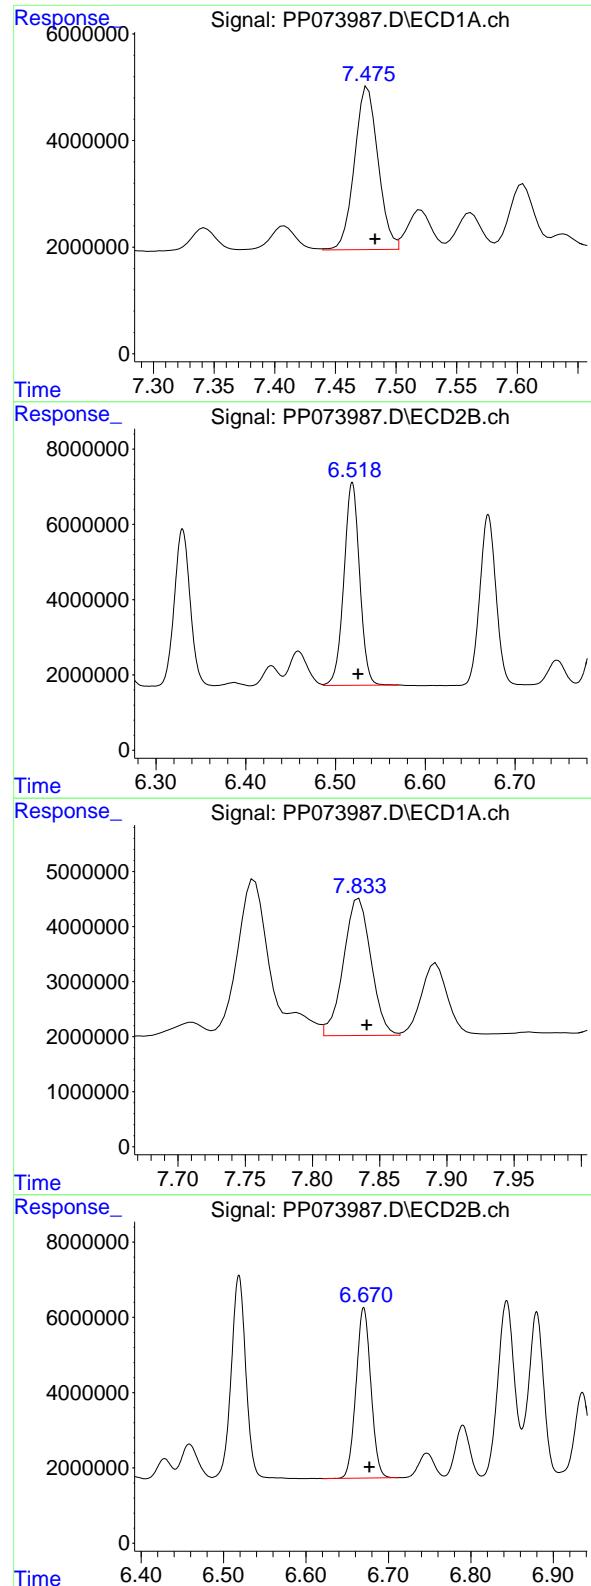

#32 AR-1260-2

R.T.: 7.477 min
 Delta R.T.: -0.006 min
 Response: 41336288
 Conc: 431.31 ng/ml

Instrument: ECD_P
 ClientSampleId: AR1660CCC500

#32 AR-1260-2


R.T.: 6.519 min
 Delta R.T.: -0.006 min
 Response: 65714064
 Conc: 534.97 ng/ml

#33 AR-1260-3

R.T.: 7.835 min
 Delta R.T.: -0.006 min
 Response: 35389503
 Conc: 484.32 ng/ml

#33 AR-1260-3

R.T.: 6.670 min
 Delta R.T.: -0.007 min
 Response: 56609708
 Conc: 517.15 ng/ml

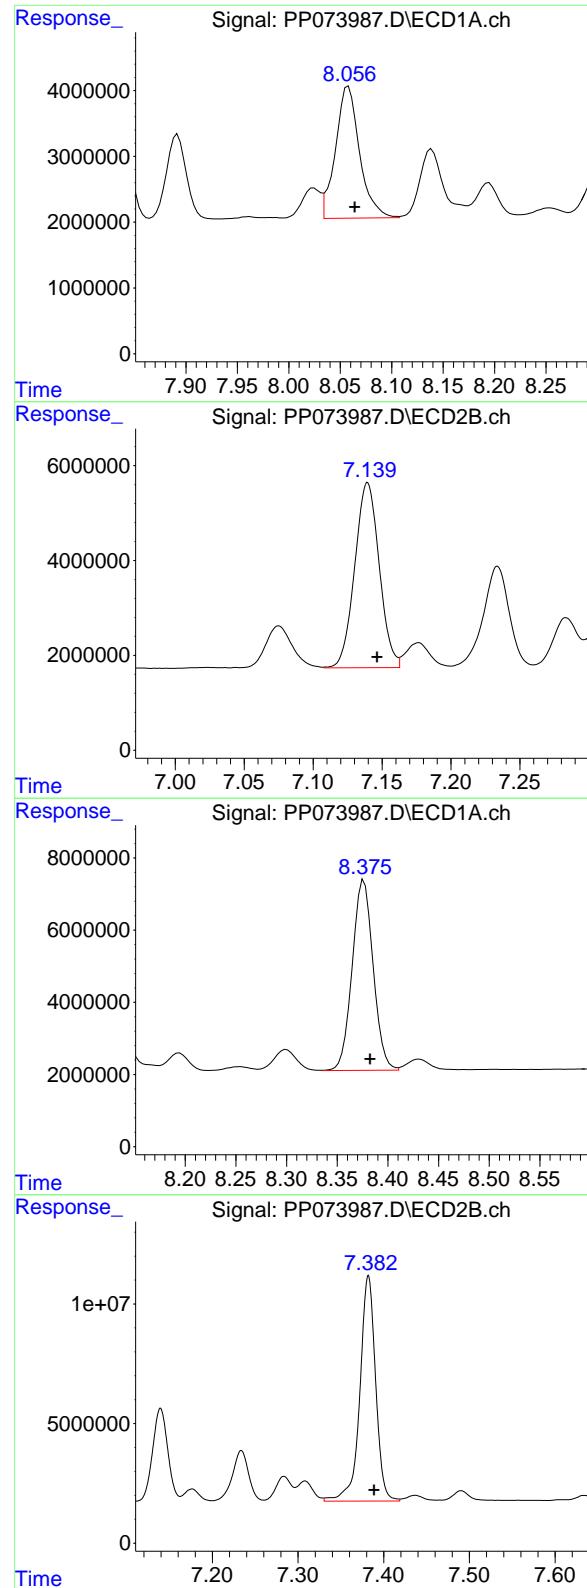

#34 AR-1260-4

R.T.: 8.058 min
 Delta R.T.: -0.006 min
 Response: 32613157
 Conc: 499.44 ng/ml

Instrument: ECD_P
 ClientSampleId: AR1660CCC500

#34 AR-1260-4

R.T.: 7.139 min
 Delta R.T.: -0.007 min
 Response: 48222670
 Conc: 539.35 ng/ml

#35 AR-1260-5

R.T.: 8.376 min
 Delta R.T.: -0.006 min
 Response: 75800503
 Conc: 502.48 ng/ml

#35 AR-1260-5

R.T.: 7.382 min
 Delta R.T.: -0.007 min
 Response: 120541218
 Conc: 536.37 ng/ml



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Lab Name: Alliance

Contract: NOBI03

Lab Code: ACE

SDG NO.: Q2639

Continuing Calib Date: 07/21/2025

Initial Calibration Date(s): 07/07/2025

07/08/2025

Continuing Calib Time: 16:07

Initial Calibration Time(s): 21:03

04:24

GC Column: ZB-MR1

ID: 0.32 (mm)

COMPOUND	CCAL RT	AVG RT	RT WINDOW FROM	TO	DIFF RT
Aroclor-1254-1 (1)	6.48	6.49	6.39	6.59	0.01
Aroclor-1254-2 (2)	6.70	6.70	6.60	6.80	0.00
Aroclor-1254-3 (3)	7.06	7.06	6.96	7.16	0.00
Aroclor-1254-4 (4)	7.34	7.35	7.25	7.45	0.01
Aroclor-1254-5 (5)	7.76	7.76	7.66	7.86	0.00
Tetrachloro-m-xylene	4.48	4.49	4.39	4.59	0.01
Decachlorobiphenyl	10.17	10.17	10.07	10.27	0.00



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Lab Name: Alliance

Contract: NOBI03

Lab Code: ACE

SDG NO.: Q2639

Continuing Calib Date: 07/21/2025

Initial Calibration Date(s): 07/07/2025

07/08/2025

Continuing Calib Time: 16:07

Initial Calibration Time(s): 21:03

04:24

GC Column: ZB-MR2

ID: 0.32 (mm)

COMPOUND	CCAL RT	AVG RT	RT WINDOW FROM	TO	DIFF RT
Aroclor-1254-1 (1)	5.65	5.66	5.56	5.76	0.01
Aroclor-1254-2 (2)	5.80	5.81	5.71	5.91	0.01
Aroclor-1254-3 (3)	6.20	6.21	6.11	6.31	0.01
Aroclor-1254-4 (4)	6.43	6.44	6.34	6.54	0.01
Aroclor-1254-5 (5)	6.85	6.85	6.75	6.95	0.01
Tetrachloro-m-xylene	3.78	3.78	3.68	3.88	0.00
Decachlorobiphenyl	8.77	8.78	8.68	8.88	0.01



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900, Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Lab Name:	<u>Alliance</u>	Contract:	<u>NOBI03</u>
Lab Code:	<u>ACE</u>	SDG NO.:	<u>Q2639</u>
GC Column:	<u>ZB-MR1</u>	ID: <u>0.32</u> (mm)	Initi. Calib. Date(s): <u>07/08/2025</u> <u>07/08/2025</u>

Client Sample No.:	<u>CCAL07</u>	Date Analyzed:	<u>07/21/2025</u>
Lab Sample No.:	<u>AR1254CCC500</u>	Data File :	<u>PP073990.D</u>
		Time Analyzed:	<u>16:07</u>

COMPOUND	RT	RT WINDOW FROM	TO	CALC AMOUNT(ng)	NOM AMOUNT(ng)	%D
Aroclor-1254-1	6.481	6.385	6.585	455.410	500.000	-8.9
Aroclor-1254-2	6.697	6.601	6.801	434.420	500.000	-13.1
Aroclor-1254-3	7.061	6.964	7.164	441.660	500.000	-11.7
Aroclor-1254-4	7.343	7.246	7.446	436.050	500.000	-12.8
Aroclor-1254-5	7.758	7.662	7.862	446.410	500.000	-10.7
Decachlorobiphenyl	10.169	10.074	10.274	50.640	50.000	1.3
Tetrachloro-m-xylene	4.483	4.387	4.587	46.520	50.000	-7.0



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900, Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Lab Name:	<u>Alliance</u>	Contract:	<u>NOBI03</u>
Lab Code:	<u>ACE</u>	SDG NO.:	<u>Q2639</u>
GC Column:	<u>ZB-MR2</u>	ID: <u>0.32</u> (mm)	Initi. Calib. Date(s): <u>07/08/2025</u> <u>07/08/2025</u>

Client Sample No.:	<u>CCAL07</u>	Date Analyzed:	<u>07/21/2025</u>
Lab Sample No.:	<u>AR1254CCC500</u>	Data File :	<u>PP073990.D</u>
		Time Analyzed:	<u>16:07</u>

COMPOUND	RT	RT WINDOW		CALC AMOUNT(ng)	NOM AMOUNT(ng)	%D
		FROM	TO			
Aroclor-1254-1	5.651	5.558	5.758	500.870	500.000	0.2
Aroclor-1254-2	5.799	5.707	5.907	495.710	500.000	-0.9
Aroclor-1254-3	6.201	6.109	6.309	499.720	500.000	-0.1
Aroclor-1254-4	6.428	6.336	6.536	530.210	500.000	6.0
Aroclor-1254-5	6.845	6.753	6.953	504.520	500.000	0.9
Decachlorobiphenyl	8.772	8.681	8.881	56.160	50.000	12.3
Tetrachloro-m-xylene	3.775	3.680	3.880	52.730	50.000	5.5

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP072125\
 Data File : PP073990.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jul 2025 16:07
 Operator : YP\AJ
 Sample : AR1254CCC500
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
AR1254CCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 22 01:54:08 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 08 08:35:32 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	4.483	3.775	63706895	97146661	46.517	52.731
2) SA Decachlor...	10.169	8.772	55251157	74304235	50.640	56.157

Target Compounds

26) L6 AR-1254-1	6.481	5.651	24404962	58115408	455.405	500.865
27) L6 AR-1254-2	6.697	5.799	36182084	49880408	434.417	495.713
28) L6 AR-1254-3	7.061	6.201	39012462	77180535	441.659	499.724
29) L6 AR-1254-4	7.343	6.428	34302541	50136100	436.047	530.209
30) L6 AR-1254-5	7.758	6.845	32891291	67325498	446.408	504.519



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.





Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP072125\
 Data File : PP073990.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jul 2025 16:07
 Operator : YP\AJ
 Sample : AR1254CCC500
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 AR1254CCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 22 01:54:08 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 08 08:35:32 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

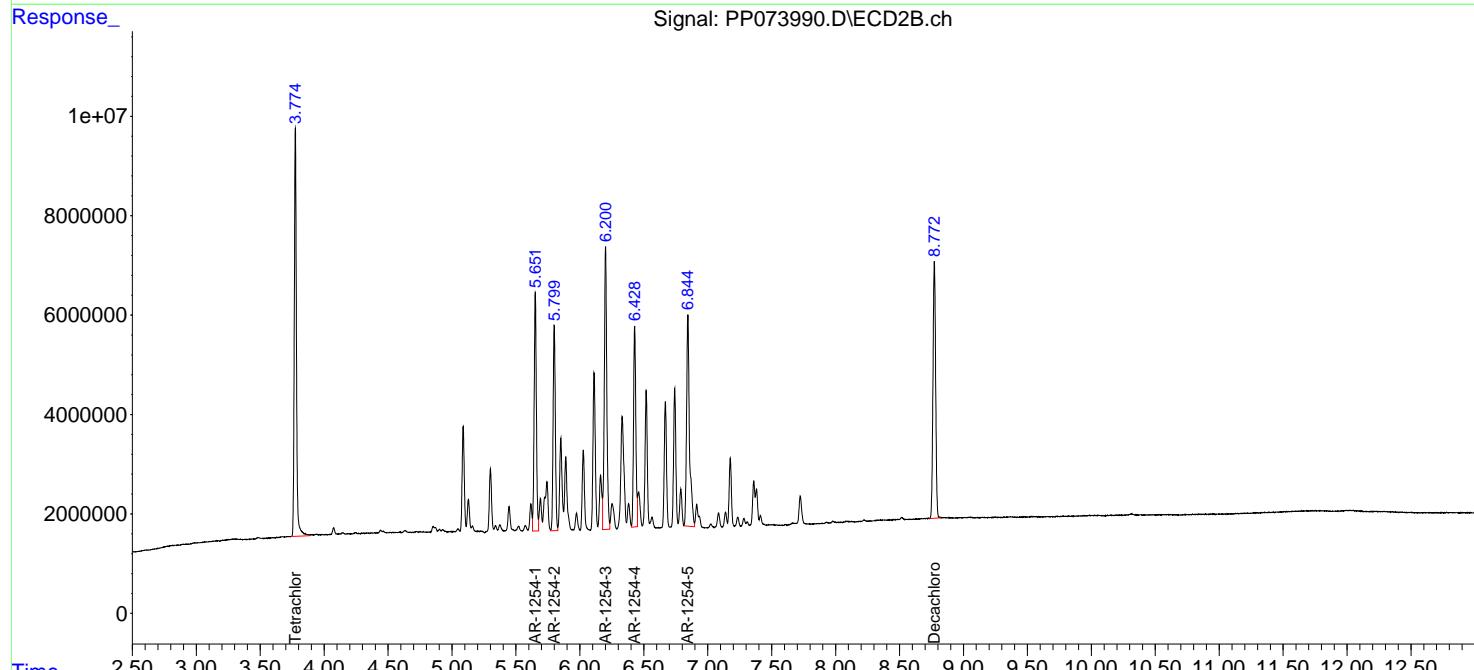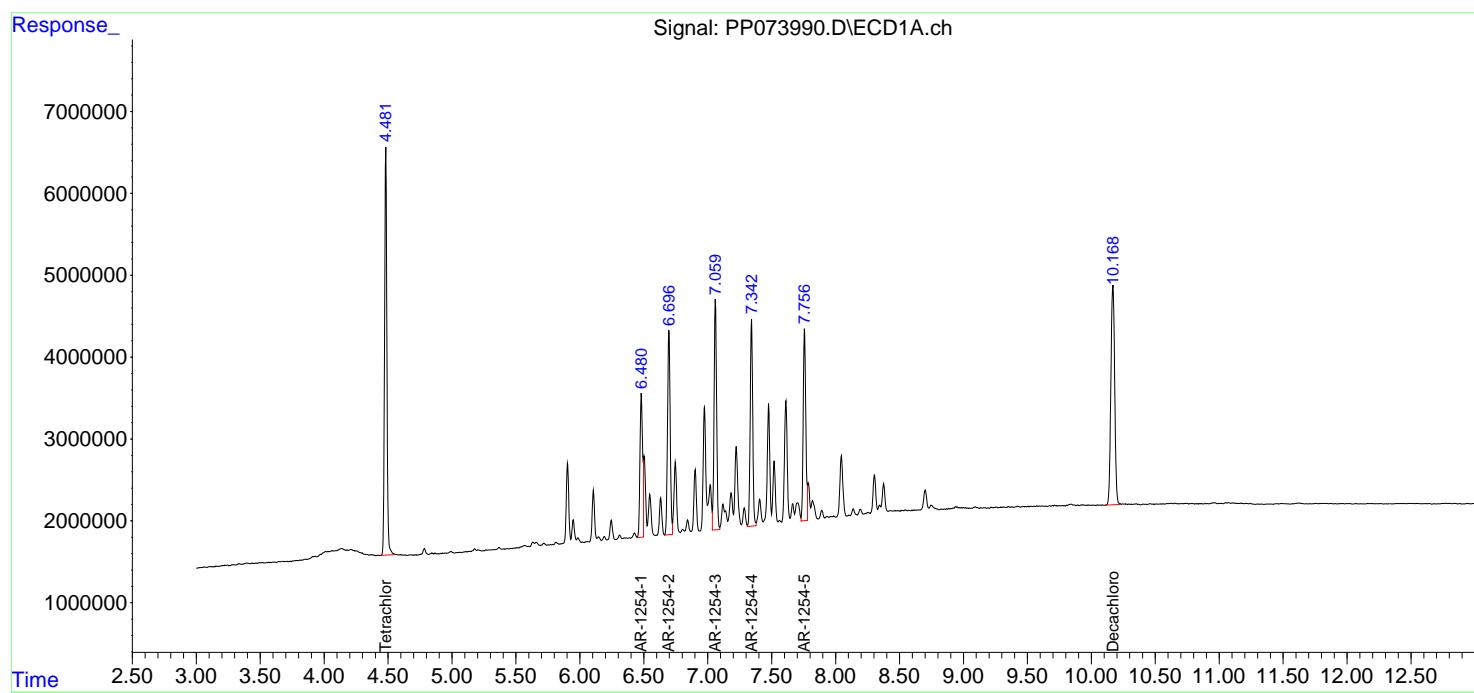

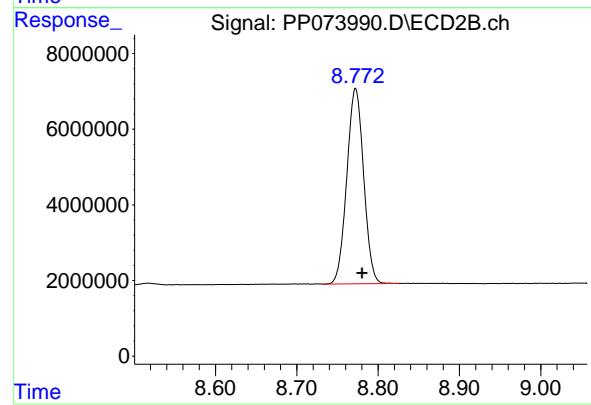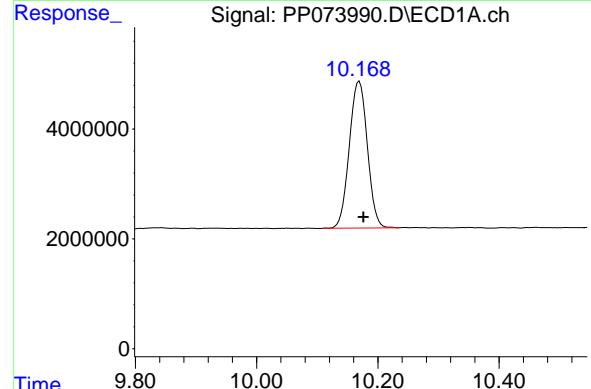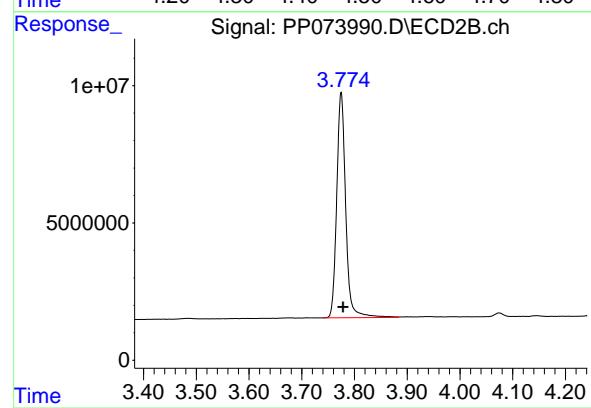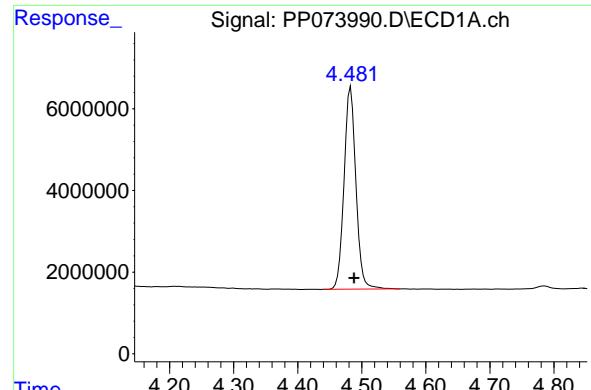

#1 Tetrachloro-m-xylene

R.T.: 4.483 min
Delta R.T.: -0.005 min
Response: 63706895
Conc: 46.52 ng/ml

Instrument:

ECD_P

ClientSampleId :

AR1254CCC500

#1 Tetrachloro-m-xylene


R.T.: 3.775 min
Delta R.T.: -0.004 min
Response: 97146661
Conc: 52.73 ng/ml

#2 Decachlorobiphenyl

R.T.: 10.169 min
Delta R.T.: -0.007 min
Response: 55251157
Conc: 50.64 ng/ml

#2 Decachlorobiphenyl


R.T.: 8.772 min
Delta R.T.: -0.008 min
Response: 74304235
Conc: 56.16 ng/ml

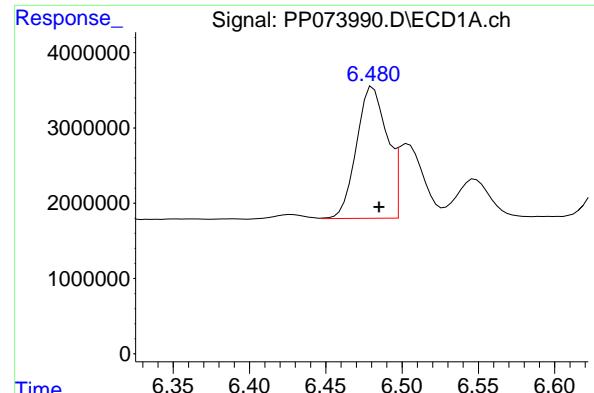

#26 AR-1254-1


R.T.: 6.481 min
 Delta R.T.: -0.004 min
 Response: 24404962
 Conc: 455.41 ng/ml

Instrument: ECD_P
 ClientSampleId: AR1254CCC500

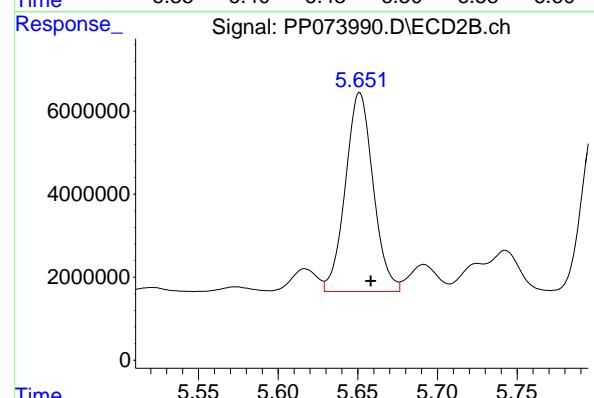


#26 AR-1254-1

R.T.: 5.651 min
 Delta R.T.: -0.007 min
 Response: 58115408
 Conc: 500.87 ng/ml

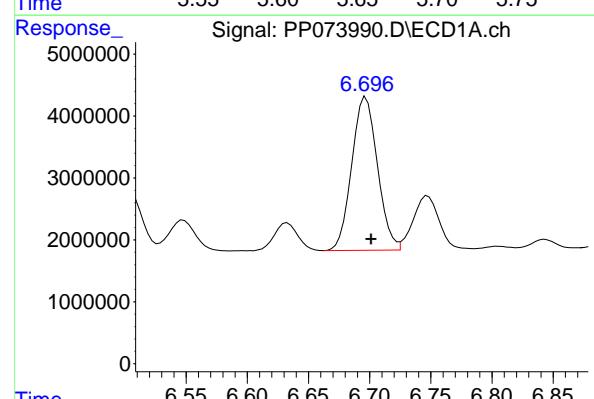





#27 AR-1254-2

R.T.: 6.697 min
 Delta R.T.: -0.004 min
 Response: 36182084
 Conc: 434.42 ng/ml

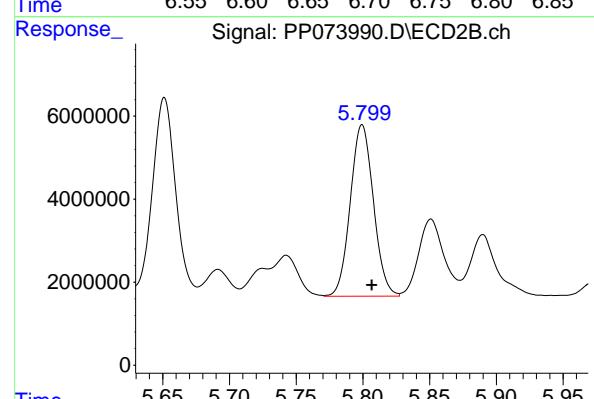

#27 AR-1254-2

R.T.: 5.799 min
 Delta R.T.: -0.007 min
 Response: 49880408
 Conc: 495.71 ng/ml

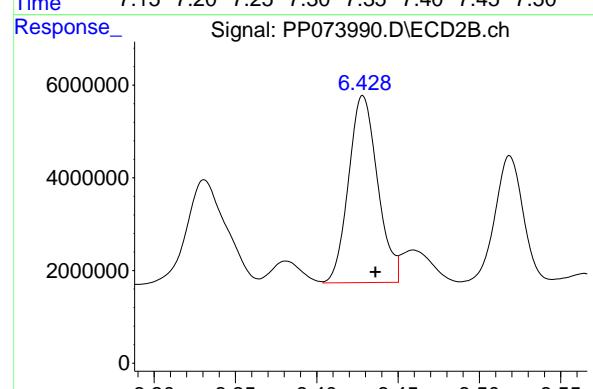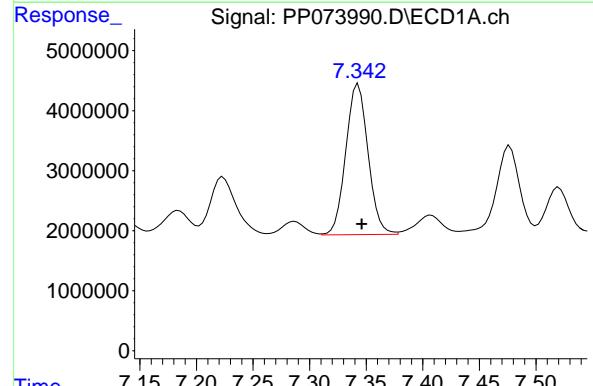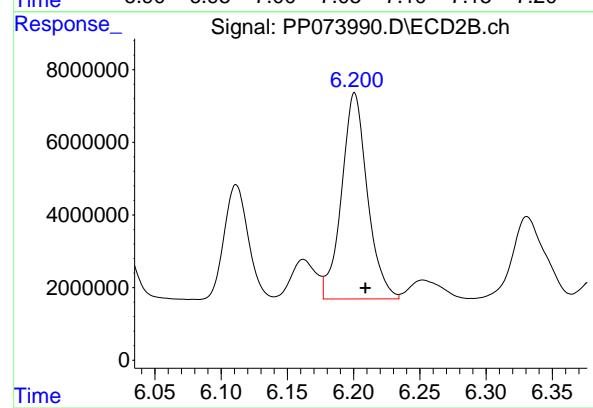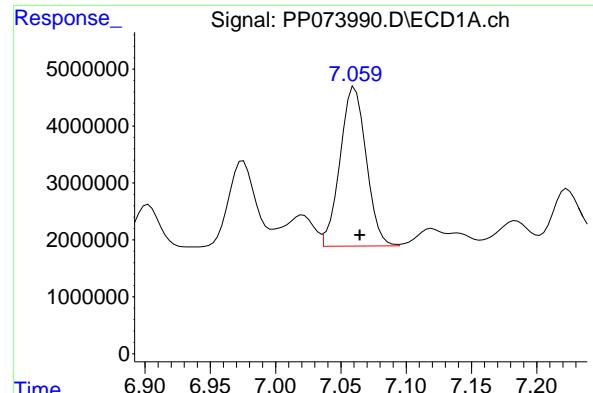

#28 AR-1254-3

R.T.: 7.061 min
 Delta R.T.: -0.004 min
 Response: 39012462
 Conc: 441.66 ng/ml

Instrument: ECD_P
 ClientSampleId: AR1254CCC500

#28 AR-1254-3


R.T.: 6.201 min
 Delta R.T.: -0.008 min
 Response: 77180535
 Conc: 499.72 ng/ml

#29 AR-1254-4

R.T.: 7.343 min
 Delta R.T.: -0.003 min
 Response: 34302541
 Conc: 436.05 ng/ml

#29 AR-1254-4

R.T.: 6.428 min
 Delta R.T.: -0.008 min
 Response: 50136100
 Conc: 530.21 ng/ml

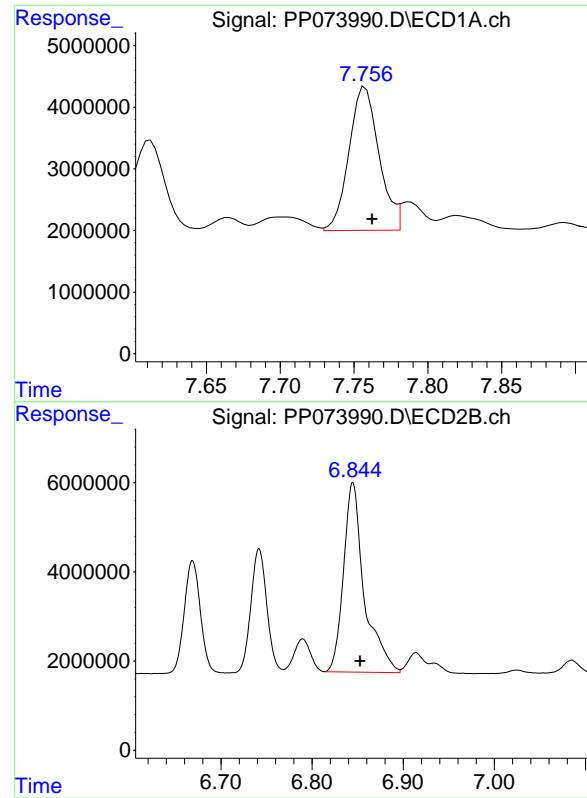

#30 AR-1254-5

R.T.: 7.758 min
Delta R.T.: -0.005 min
Response: 32891291
Conc: 446.41 ng/ml

Instrument: ECD_P
ClientSampleId: AR1254CCC500

#30 AR-1254-5

R.T.: 6.845 min
Delta R.T.: -0.008 min
Response: 67325498
Conc: 504.52 ng/ml



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Lab Name: Alliance

Contract: NOBI03

Lab Code: ACE

SDG NO.: Q2639

Continuing Calib Date: 07/21/2025

Initial Calibration Date(s): 07/07/2025

07/08/2025

Continuing Calib Time: 20:12

Initial Calibration Time(s): 21:03

04:24

GC Column: ZB-MR1

ID: 0.32 (mm)

COMPOUND	CCAL RT	Avg RT	RT Window From	TO	Diff RT
Aroclor-1016-1 (1)	5.63	5.64	5.54	5.74	0.01
Aroclor-1016-2 (2)	5.66	5.66	5.56	5.76	0.00
Aroclor-1016-3 (3)	5.72	5.72	5.62	5.82	0.00
Aroclor-1016-4 (4)	5.81	5.82	5.72	5.92	0.01
Aroclor-1016-5 (5)	6.11	6.11	6.01	6.21	0.00
Aroclor-1260-1 (1)	7.22	7.23	7.13	7.33	0.01
Aroclor-1260-2 (2)	7.48	7.48	7.38	7.58	0.00
Aroclor-1260-3 (3)	7.84	7.84	7.74	7.94	0.00
Aroclor-1260-4 (4)	8.06	8.06	7.96	8.16	0.00
Aroclor-1260-5 (5)	8.38	8.38	8.28	8.48	0.00
Tetrachloro-m-xylene	4.48	4.49	4.39	4.59	0.01
Decachlorobiphenyl	10.17	10.18	10.08	10.28	0.01



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Lab Name: Alliance

Contract: NOBI03

Lab Code: ACE

SDG NO.: Q2639

Continuing Calib Date: 07/21/2025

Initial Calibration Date(s): 07/07/2025

07/08/2025

Continuing Calib Time: 20:12

Initial Calibration Time(s): 21:03

04:24

GC Column: ZB-MR2

ID: 0.32 (mm)

COMPOUND	CCAL RT	Avg RT	RT Window From	TO	Diff RT
Aroclor-1016-1 (1)	4.85	4.86	4.76	4.96	0.01
Aroclor-1016-2 (2)	4.87	4.88	4.78	4.98	0.01
Aroclor-1016-3 (3)	5.05	5.05	4.95	5.15	0.00
Aroclor-1016-4 (4)	5.09	5.09	4.99	5.19	0.00
Aroclor-1016-5 (5)	5.30	5.31	5.21	5.41	0.01
Aroclor-1260-1 (1)	6.33	6.34	6.24	6.44	0.01
Aroclor-1260-2 (2)	6.52	6.53	6.43	6.63	0.01
Aroclor-1260-3 (3)	6.67	6.68	6.58	6.78	0.01
Aroclor-1260-4 (4)	7.14	7.15	7.05	7.25	0.01
Aroclor-1260-5 (5)	7.38	7.39	7.29	7.49	0.01
Tetrachloro-m-xylene	3.77	3.78	3.68	3.88	0.01
Decachlorobiphenyl	8.77	8.78	8.68	8.88	0.01



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900, Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Lab Name:	<u>Alliance</u>	Contract:	<u>NOBI03</u>
Lab Code:	<u>ACE</u>	SDG NO.:	<u>Q2639</u>
GC Column:	<u>ZB-MR1</u>	ID: <u>0.32</u> (mm)	Initi. Calib. Date(s): <u>07/07/2025</u> <u>07/07/2025</u>

Client Sample No.:	<u>CCAL08</u>	Date Analyzed:	<u>07/21/2025</u>
Lab Sample No.:	<u>AR1660CCC500</u>	Data File :	<u>PP074002.D</u>
		Time Analyzed:	<u>20:12</u>

COMPOUND	RT	RT WINDOW FROM	TO	CALC AMOUNT(ng)	NOM AMOUNT(ng)	%D
Aroclor-1016-1	5.633	5.539	5.739	417.670	500.000	-16.5
Aroclor-1016-2	5.655	5.560	5.760	441.230	500.000	-11.8
Aroclor-1016-3	5.717	5.622	5.822	440.930	500.000	-11.8
Aroclor-1016-4	5.814	5.720	5.920	447.640	500.000	-10.5
Aroclor-1016-5	6.106	6.012	6.212	447.640	500.000	-10.5
Aroclor-1260-1	7.223	7.129	7.329	436.450	500.000	-12.7
Aroclor-1260-2	7.476	7.383	7.583	388.210	500.000	-22.4
Aroclor-1260-3	7.835	7.740	7.940	446.560	500.000	-10.7
Aroclor-1260-4	8.058	7.964	8.164	457.200	500.000	-8.6
Aroclor-1260-5	8.375	8.283	8.483	463.250	500.000	-7.4
Decachlorobiphenyl	10.167	10.076	10.276	49.370	50.000	-1.3
Tetrachloro-m-xylene	4.482	4.388	4.588	46.140	50.000	-7.7



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900, Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Lab Name:	<u>Alliance</u>	Contract:	<u>NOBI03</u>
Lab Code:	<u>ACE</u>	SDG NO.:	<u>Q2639</u>
GC Column:	<u>ZB-MR2</u>	ID: <u>0.32</u> (mm)	Initi. Calib. Date(s): <u>07/07/2025</u> <u>07/07/2025</u>

Client Sample No.:	<u>CCAL08</u>	Date Analyzed:	<u>07/21/2025</u>
Lab Sample No.:	<u>AR1660CCC500</u>	Data File :	<u>PP074002.D</u>
		Time Analyzed:	<u>20:12</u>

COMPOUND	RT	RT WINDOW FROM	TO	CALC AMOUNT(ng)	NOM AMOUNT(ng)	%D
Aroclor-1016-1	4.851	4.758	4.958	493.890	500.000	-1.2
Aroclor-1016-2	4.868	4.775	4.975	499.810	500.000	0.0
Aroclor-1016-3	5.045	4.951	5.151	503.470	500.000	0.7
Aroclor-1016-4	5.086	4.993	5.193	504.400	500.000	0.9
Aroclor-1016-5	5.300	5.207	5.407	538.420	500.000	7.7
Aroclor-1260-1	6.328	6.237	6.437	491.430	500.000	-1.7
Aroclor-1260-2	6.518	6.425	6.625	498.630	500.000	-0.3
Aroclor-1260-3	6.669	6.577	6.777	486.440	500.000	-2.7
Aroclor-1260-4	7.138	7.046	7.246	498.710	500.000	-0.3
Aroclor-1260-5	7.381	7.289	7.489	492.290	500.000	-1.5
Decachlorobiphenyl	8.770	8.680	8.880	55.670	50.000	11.3
Tetrachloro-m-xylene	3.774	3.678	3.878	49.390	50.000	-1.2

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP072125\
 Data File : PP074002.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jul 2025 20:12
 Operator : YP\AJ
 Sample : AR1660CCC500
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
AR1660CCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 22 02:15:43 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 08 08:35:32 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	4.482	3.774	63193426	90988816	46.143	49.389
2) SA Decachlor...	10.167	8.770	53862595	73653605	49.368	55.665

Target Compounds

3) L1 AR-1016-1	5.633	4.851	19845079	33671086	417.672	493.894
4) L1 AR-1016-2	5.655	4.868	31421872	50923060	441.226	499.812
5) L1 AR-1016-3	5.717	5.045	19252218	27240841	440.927	503.469
6) L1 AR-1016-4	5.814	5.086	16090510	22133580	447.635	504.402
7) L1 AR-1016-5	6.106	5.300	14024771	29388405	447.641	538.422
31) L7 AR-1260-1	7.223	6.328	25733643	47943599	436.450	491.425
32) L7 AR-1260-2	7.476	6.518	37205677	61251085	388.207	498.635 #
33) L7 AR-1260-3	7.835	6.669	32630488	53247386	446.561	486.438
34) L7 AR-1260-4	8.058	7.138	29855389	44588741	457.204	498.708
35) L7 AR-1260-5	8.375	7.381	69882878	110.6E6	463.252	492.291



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.





Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP072125\
 Data File : PP074002.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jul 2025 20:12
 Operator : YP\AJ
 Sample : AR1660CCC500
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 AR1660CCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 22 02:15:43 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 08 08:35:32 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

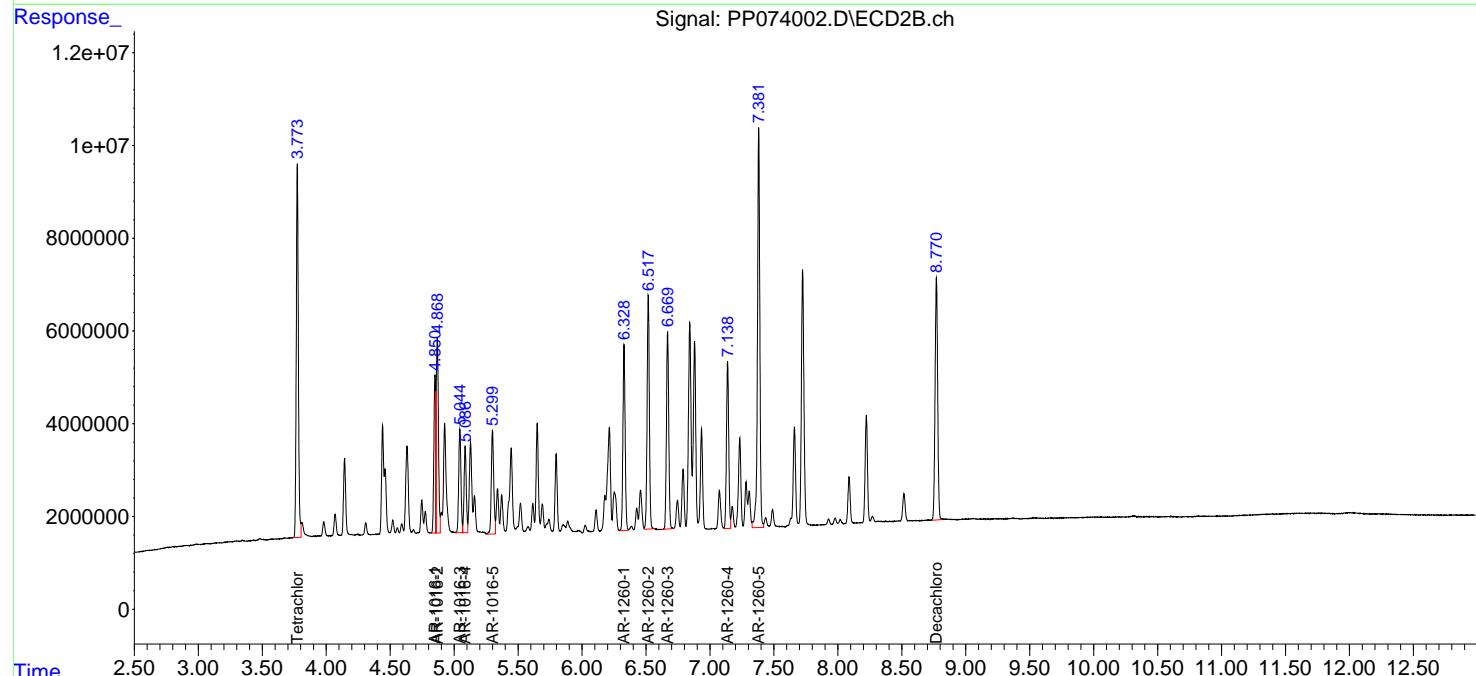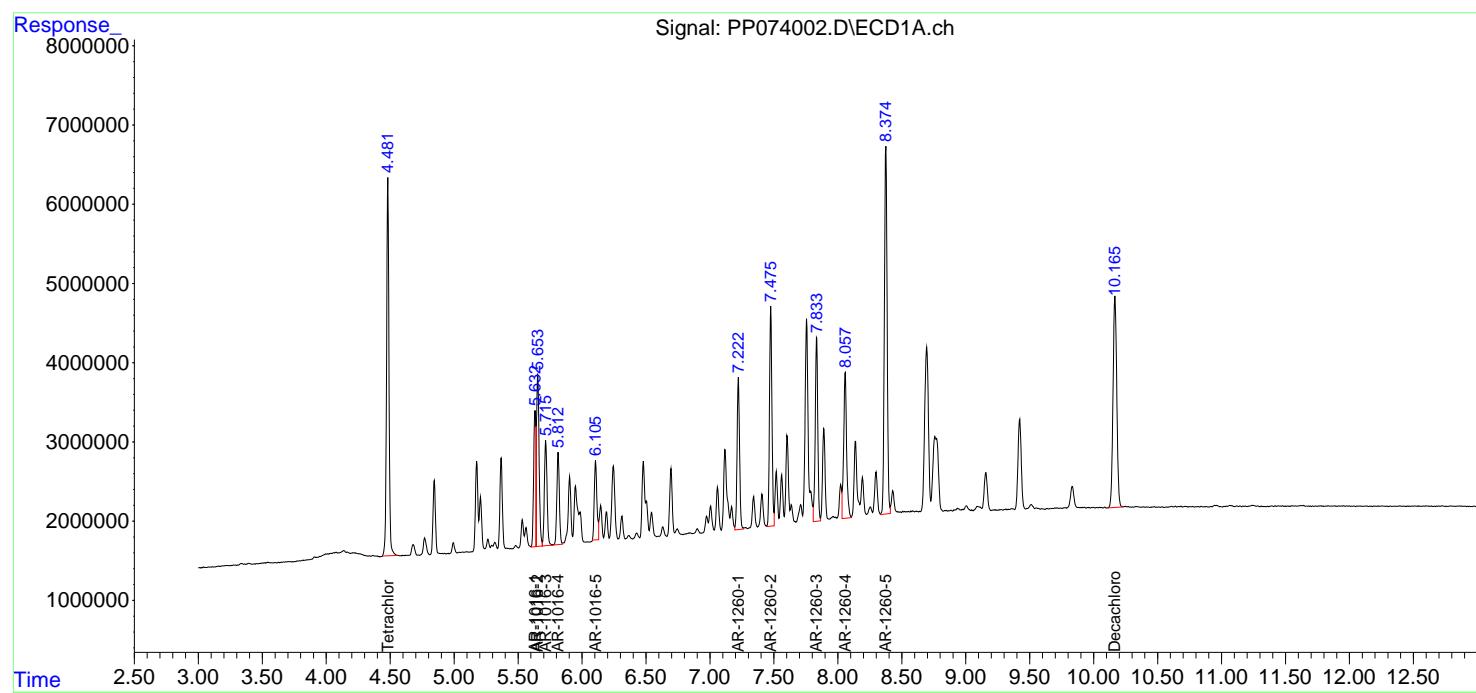

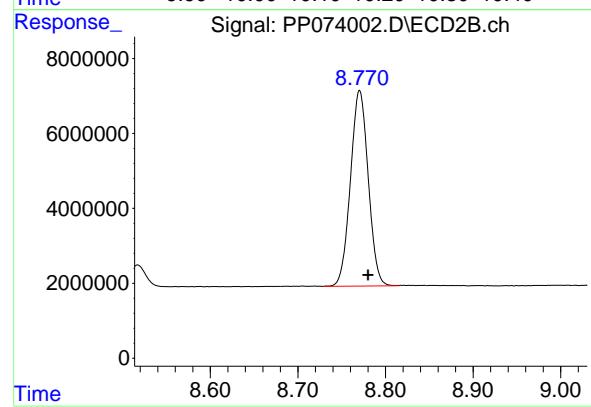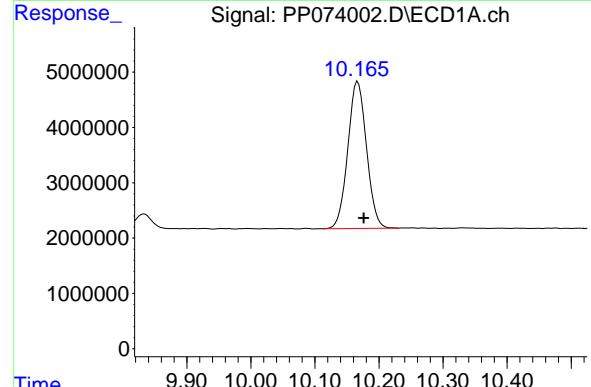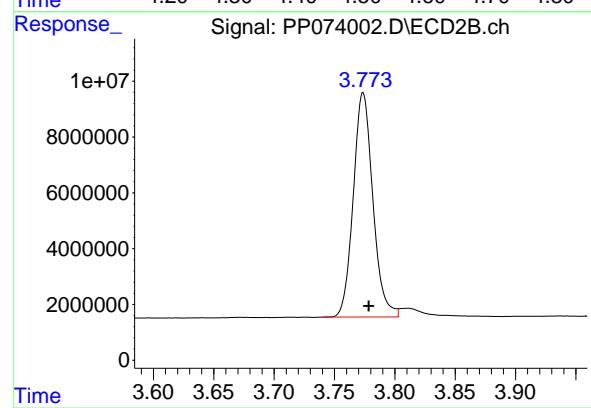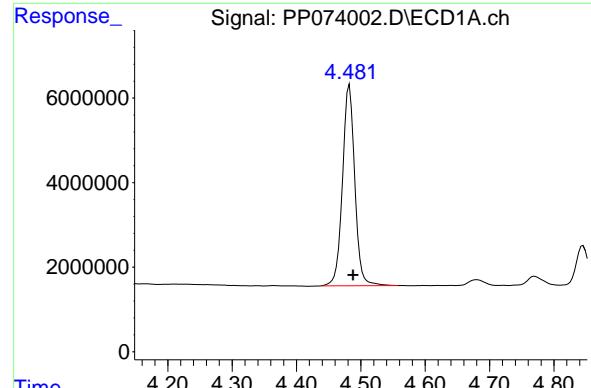

#1 Tetrachloro-m-xylene

R.T.: 4.482 min
 Delta R.T.: -0.006 min
 Response: 63193426
 Conc: 46.14 ng/ml

Instrument : ECD_P

ClientSampleId : AR1660CCC500

#1 Tetrachloro-m-xylene





R.T.: 3.774 min
 Delta R.T.: -0.005 min
 Response: 90988816
 Conc: 49.39 ng/ml

#2 Decachlorobiphenyl

R.T.: 10.167 min
 Delta R.T.: -0.009 min
 Response: 53862595
 Conc: 49.37 ng/ml

#2 Decachlorobiphenyl

R.T.: 8.770 min
 Delta R.T.: -0.010 min
 Response: 73653605
 Conc: 55.67 ng/ml

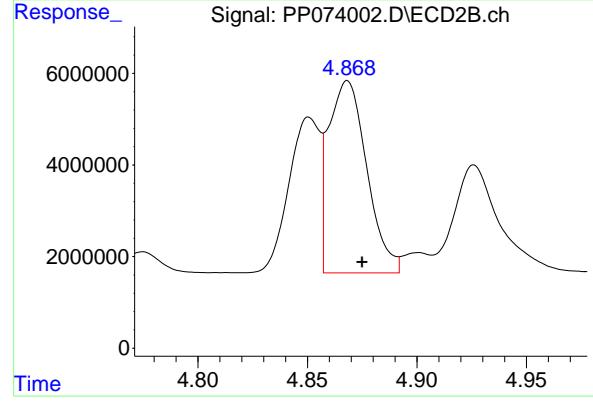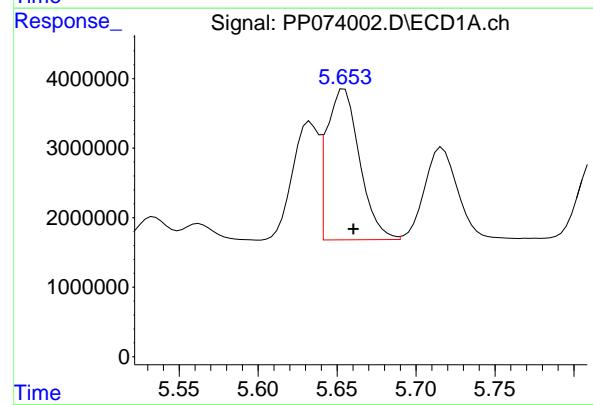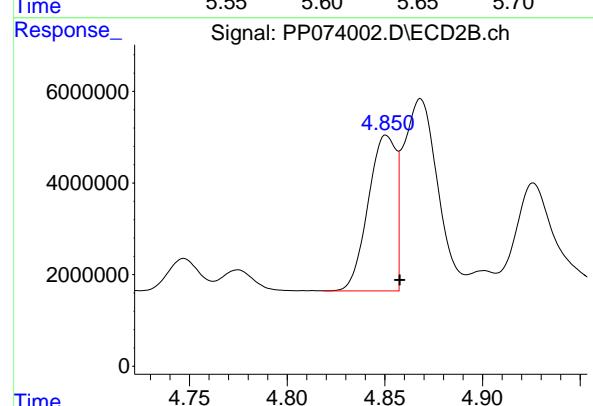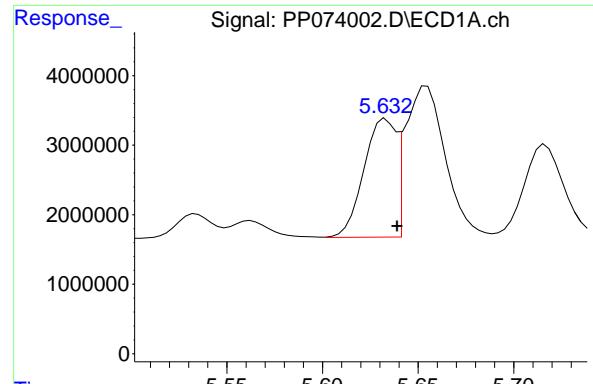

#3 AR-1016-1

R.T.: 5.633 min
 Delta R.T.: -0.006 min
 Response: 19845079
 Conc: 417.67 ng/ml

Instrument: ECD_P
 ClientSampleId: AR1660CCC500

#3 AR-1016-1


R.T.: 4.851 min
 Delta R.T.: -0.007 min
 Response: 33671086
 Conc: 493.89 ng/ml

#4 AR-1016-2

R.T.: 5.655 min
 Delta R.T.: -0.006 min
 Response: 31421872
 Conc: 441.23 ng/ml

#4 AR-1016-2


R.T.: 4.868 min
 Delta R.T.: -0.007 min
 Response: 50923060
 Conc: 499.81 ng/ml

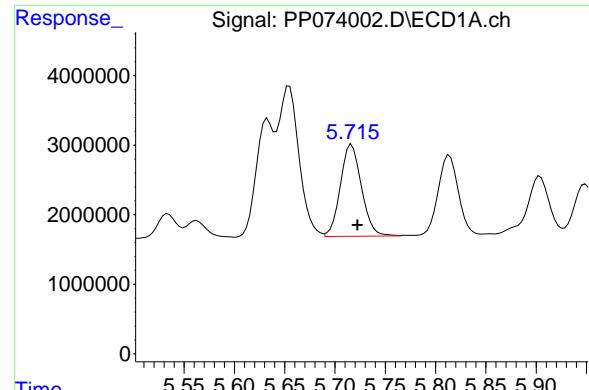

#5 AR-1016-3


R.T.: 5.717 min
 Delta R.T.: -0.006 min
 Response: 19252218
 Conc: 440.93 ng/ml

Instrument: ECD_P
 ClientSampleId: AR1660CCC500

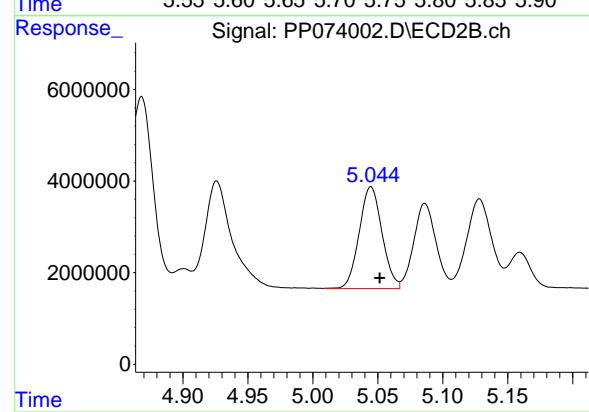


#5 AR-1016-3

R.T.: 5.045 min
 Delta R.T.: -0.007 min
 Response: 27240841
 Conc: 503.47 ng/ml

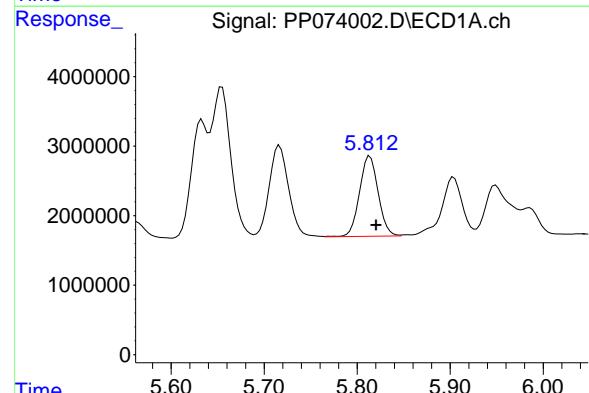


#6 AR-1016-4

R.T.: 5.814 min
 Delta R.T.: -0.006 min
 Response: 16090510
 Conc: 447.64 ng/ml

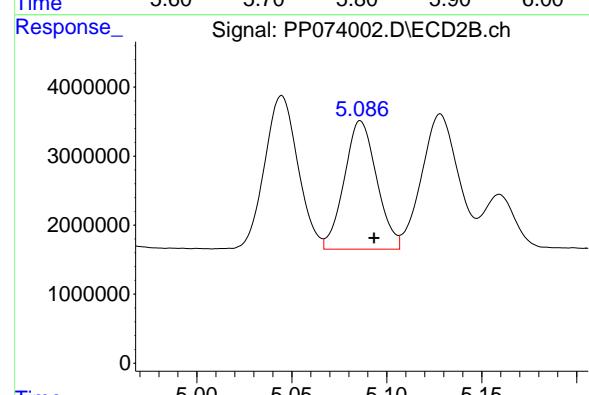

#6 AR-1016-4

R.T.: 5.086 min
 Delta R.T.: -0.007 min
 Response: 22133580
 Conc: 504.40 ng/ml

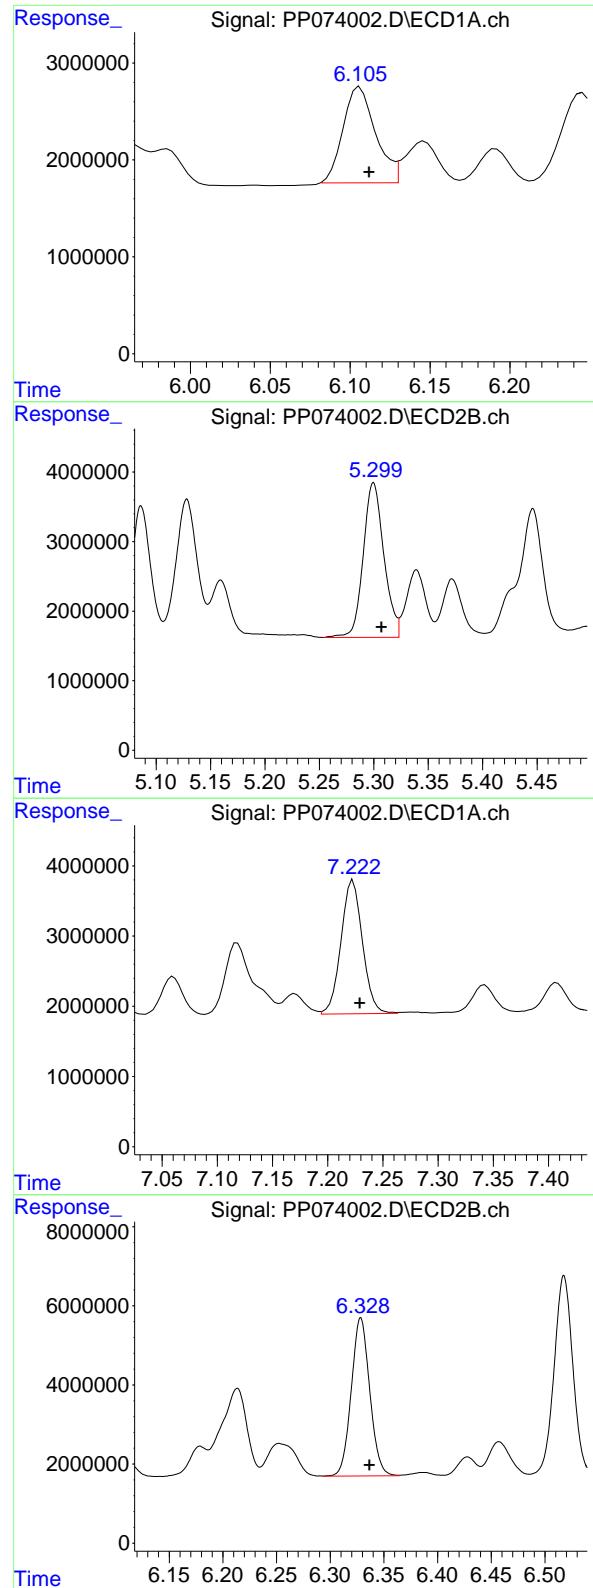

#7 AR-1016-5

R.T.: 6.106 min
 Delta R.T.: -0.006 min
 Response: 14024771
 Conc: 447.64 ng/ml

Instrument: ECD_P
 ClientSampleId: AR1660CCC500

#7 AR-1016-5

R.T.: 5.300 min
 Delta R.T.: -0.007 min
 Response: 29388405
 Conc: 538.42 ng/ml

#31 AR-1260-1

R.T.: 7.223 min
 Delta R.T.: -0.006 min
 Response: 25733643
 Conc: 436.45 ng/ml


#31 AR-1260-1

R.T.: 6.328 min
 Delta R.T.: -0.008 min
 Response: 47943599
 Conc: 491.43 ng/ml

#32 AR-1260-2


R.T.: 7.476 min
 Delta R.T.: -0.006 min
 Response: 37205677
 Conc: 388.21 ng/ml

Instrument: ECD_P
 ClientSampleId: AR1660CCC500

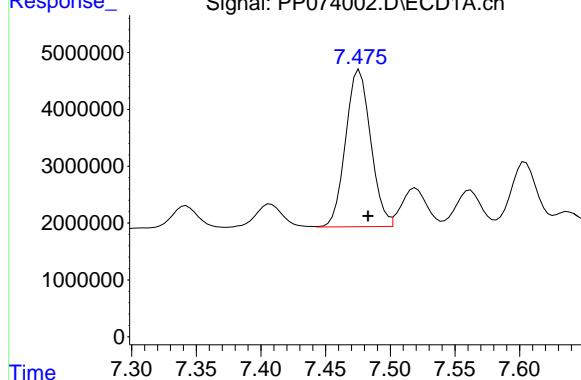


#32 AR-1260-2

R.T.: 6.518 min
 Delta R.T.: -0.007 min
 Response: 61251085
 Conc: 498.63 ng/ml

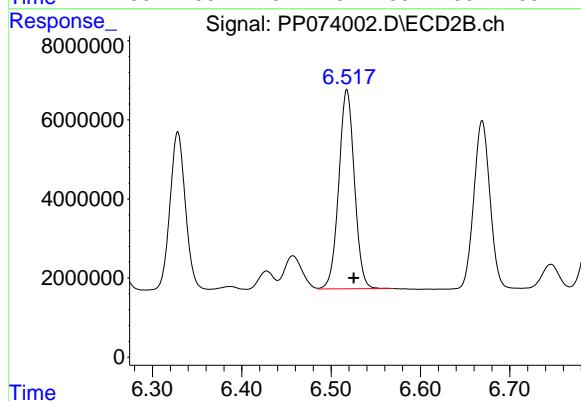


#33 AR-1260-3


R.T.: 7.835 min
 Delta R.T.: -0.006 min
 Response: 32630488
 Conc: 446.56 ng/ml

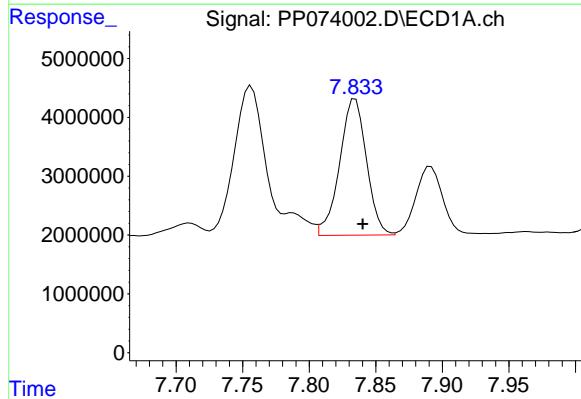

#33 AR-1260-3

R.T.: 6.669 min
 Delta R.T.: -0.008 min
 Response: 53247386
 Conc: 486.44 ng/ml

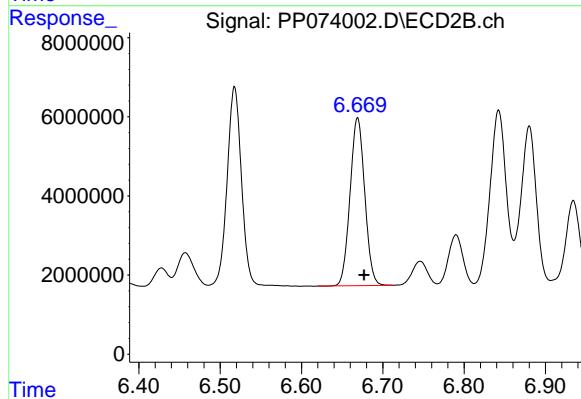

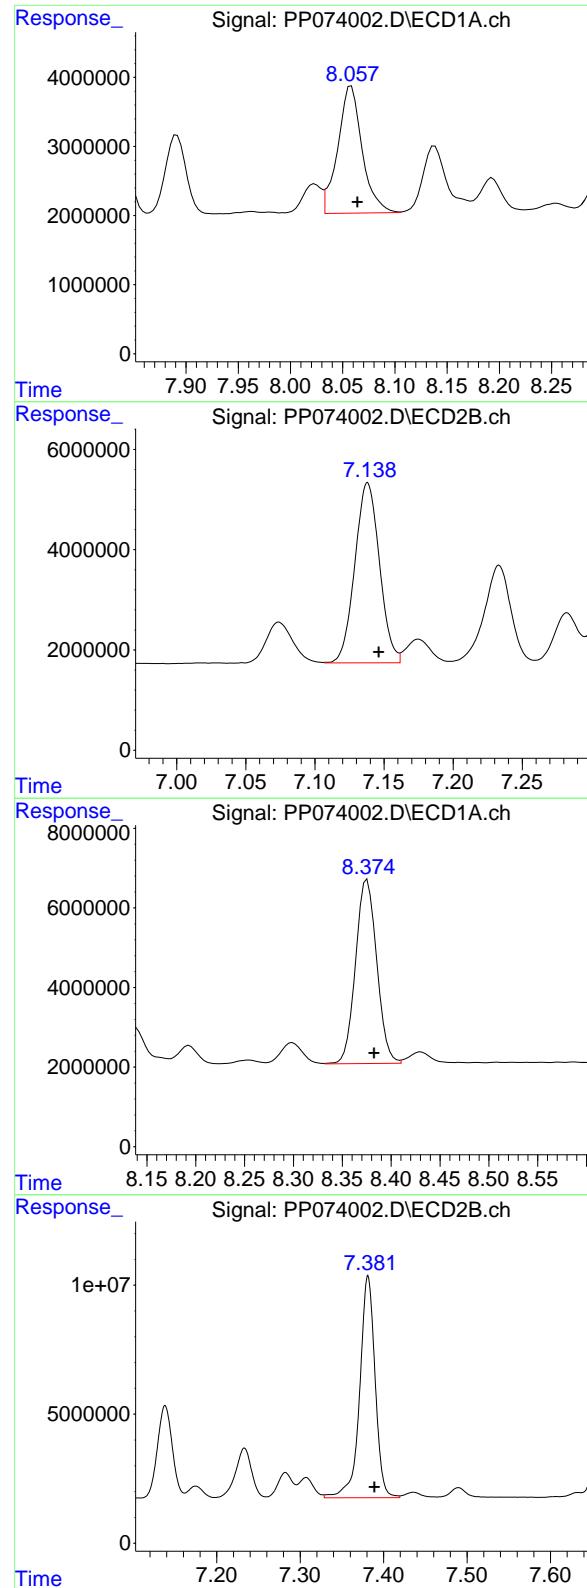

#34 AR-1260-4

R.T.: 8.058 min
 Delta R.T.: -0.006 min
 Response: 29855389
 Conc: 457.20 ng/ml

Instrument: ECD_P
 ClientSampleId: AR1660CCC500

#34 AR-1260-4

R.T.: 7.138 min
 Delta R.T.: -0.008 min
 Response: 44588741
 Conc: 498.71 ng/ml

#35 AR-1260-5

R.T.: 8.375 min
 Delta R.T.: -0.007 min
 Response: 69882878
 Conc: 463.25 ng/ml

#35 AR-1260-5

R.T.: 7.381 min
 Delta R.T.: -0.008 min
 Response: 110635763
 Conc: 492.29 ng/ml



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Lab Name: Alliance

Contract: NOBI03

Lab Code: ACE

SDG NO.: Q2639

Continuing Calib Date: 07/21/2025

Initial Calibration Date(s): 07/07/2025

07/08/2025

Continuing Calib Time: 21:17

Initial Calibration Time(s): 21:03

04:24

GC Column: ZB-MR1

ID: 0.32 (mm)

COMPOUND	CCAL RT	AVG RT	RT WINDOW FROM	TO	DIFF RT
Aroclor-1254-1 (1)	6.48	6.49	6.39	6.59	0.01
Aroclor-1254-2 (2)	6.70	6.70	6.60	6.80	0.00
Aroclor-1254-3 (3)	7.06	7.06	6.96	7.16	0.00
Aroclor-1254-4 (4)	7.35	7.35	7.25	7.45	0.01
Aroclor-1254-5 (5)	7.76	7.76	7.66	7.86	0.00
Tetrachloro-m-xylene	4.48	4.49	4.39	4.59	0.01
Decachlorobiphenyl	10.17	10.17	10.07	10.27	0.00



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Lab Name: Alliance

Contract: NOBI03

Lab Code: ACE

SDG NO.: Q2639

Continuing Calib Date: 07/21/2025

Initial Calibration Date(s): 07/07/2025

07/08/2025

Continuing Calib Time: 21:17

Initial Calibration Time(s): 21:03

04:24

GC Column: ZB-MR2

ID: 0.32 (mm)

COMPOUND	CCAL RT	AVG RT	RT WINDOW FROM	TO	DIFF RT
Aroclor-1254-1 (1)	5.65	5.66	5.56	5.76	0.01
Aroclor-1254-2 (2)	5.80	5.81	5.71	5.91	0.01
Aroclor-1254-3 (3)	6.20	6.21	6.11	6.31	0.01
Aroclor-1254-4 (4)	6.43	6.44	6.34	6.54	0.01
Aroclor-1254-5 (5)	6.84	6.85	6.75	6.95	0.01
Tetrachloro-m-xylene	3.77	3.78	3.68	3.88	0.01
Decachlorobiphenyl	8.77	8.78	8.68	8.88	0.01



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900, Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Lab Name:	<u>Alliance</u>	Contract:	<u>NOBI03</u>
Lab Code:	<u>ACE</u>	SDG NO.:	<u>Q2639</u>
GC Column:	<u>ZB-MR1</u>	ID: <u>0.32</u> (mm)	Initi. Calib. Date(s): <u>07/08/2025</u> <u>07/08/2025</u>

Client Sample No.:	<u>CCAL09</u>	Date Analyzed:	<u>07/21/2025</u>
Lab Sample No.:	<u>AR1254CCC500</u>	Data File :	<u>PP074005.D</u>
		Time Analyzed:	<u>21:17</u>

COMPOUND	RT	RT WINDOW FROM		CALC AMOUNT(ng)	NOM AMOUNT(ng)	%D
		FROM	TO			
Aroclor-1254-1	6.483	6.385	6.585	449.490	500.000	-10.1
Aroclor-1254-2	6.699	6.601	6.801	431.330	500.000	-13.7
Aroclor-1254-3	7.062	6.964	7.164	442.240	500.000	-11.6
Aroclor-1254-4	7.345	7.246	7.446	435.450	500.000	-12.9
Aroclor-1254-5	7.760	7.662	7.862	446.680	500.000	-10.7
Decachlorobiphenyl	10.169	10.074	10.274	50.920	50.000	1.8
Tetrachloro-m-xylene	4.484	4.387	4.587	45.940	50.000	-8.1



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900, Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Lab Name:	<u>Alliance</u>	Contract:	<u>NOBI03</u>
Lab Code:	<u>ACE</u>	SDG NO.:	<u>Q2639</u>
GC Column:	<u>ZB-MR2</u>	ID: <u>0.32</u> (mm)	Initi. Calib. Date(s): <u>07/08/2025</u> <u>07/08/2025</u>

Client Sample No.:	<u>CCAL09</u>	Date Analyzed:	<u>07/21/2025</u>
Lab Sample No.:	<u>AR1254CCC500</u>	Data File :	<u>PP074005.D</u>
		Time Analyzed:	<u>21:17</u>

COMPOUND	RT	RT WINDOW FROM	TO	CALC AMOUNT(ng)	NOM AMOUNT(ng)	%D
Aroclor-1254-1	5.649	5.558	5.758	515.380	500.000	3.1
Aroclor-1254-2	5.797	5.707	5.907	504.980	500.000	1.0
Aroclor-1254-3	6.197	6.109	6.309	506.890	500.000	1.4
Aroclor-1254-4	6.426	6.336	6.536	529.650	500.000	5.9
Aroclor-1254-5	6.842	6.753	6.953	504.770	500.000	1.0
Decachlorobiphenyl	8.769	8.681	8.881	56.490	50.000	13.0
Tetrachloro-m-xylene	3.772	3.680	3.880	52.550	50.000	5.1

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP072125\
 Data File : PP074005.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jul 2025 21:17
 Operator : YP\AJ
 Sample : AR1254CCC500
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
AR1254CCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 22 02:16:45 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 08 08:35:32 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	4.484	3.772	62918811	96808458	45.942	52.548
2) SA Decachlor...	10.169	8.769	55557066	74740902	50.921	56.487

Target Compounds

26) L6 AR-1254-1	6.483	5.649	24087897	59799936	449.489	515.383
27) L6 AR-1254-2	6.699	5.797	35924728	50812946	431.327	504.981
28) L6 AR-1254-3	7.062	6.197	39063469	78287085	442.236	506.888
29) L6 AR-1254-4	7.345	6.426	34255719	50083505	435.452	529.652
30) L6 AR-1254-5	7.760	6.842	32911104	67358728	446.677	504.768



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP072125\
 Data File : PP074005.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jul 2025 21:17
 Operator : YP\AJ
 Sample : AR1254CCC500
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 AR1254CCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 22 02:16:45 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 08 08:35:32 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

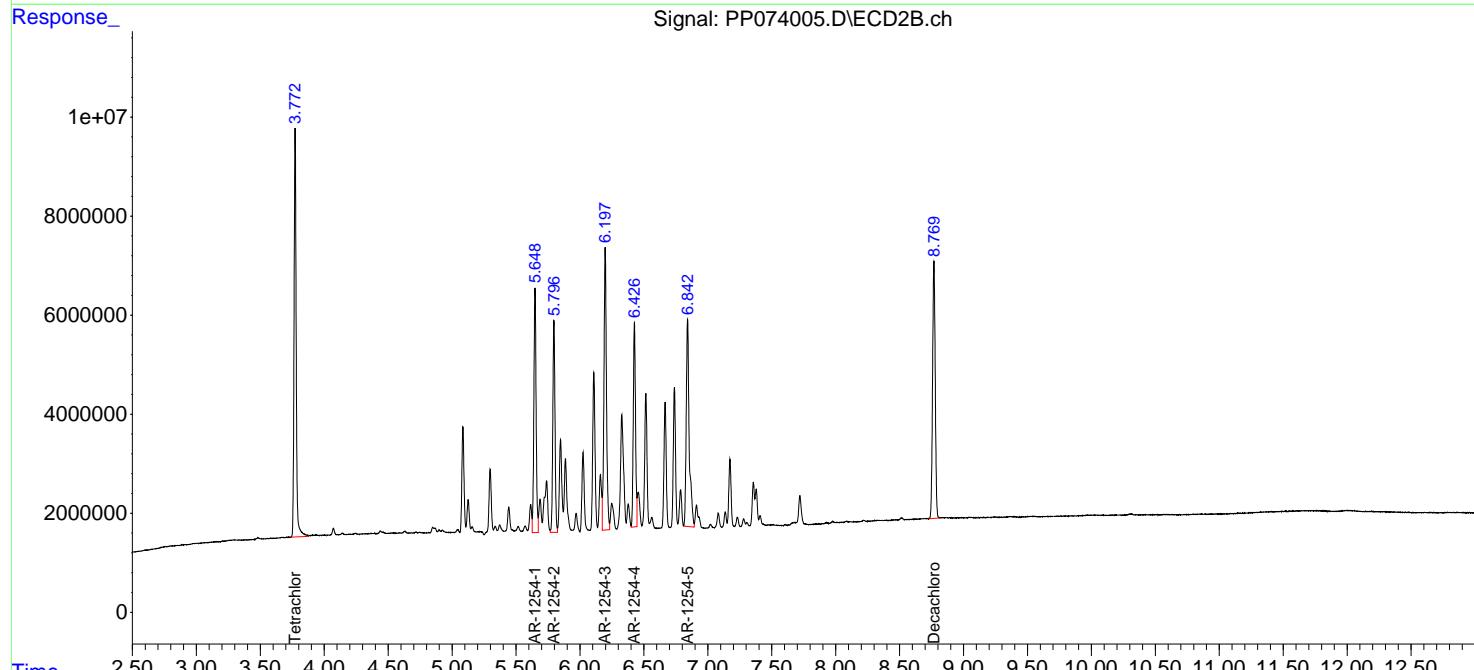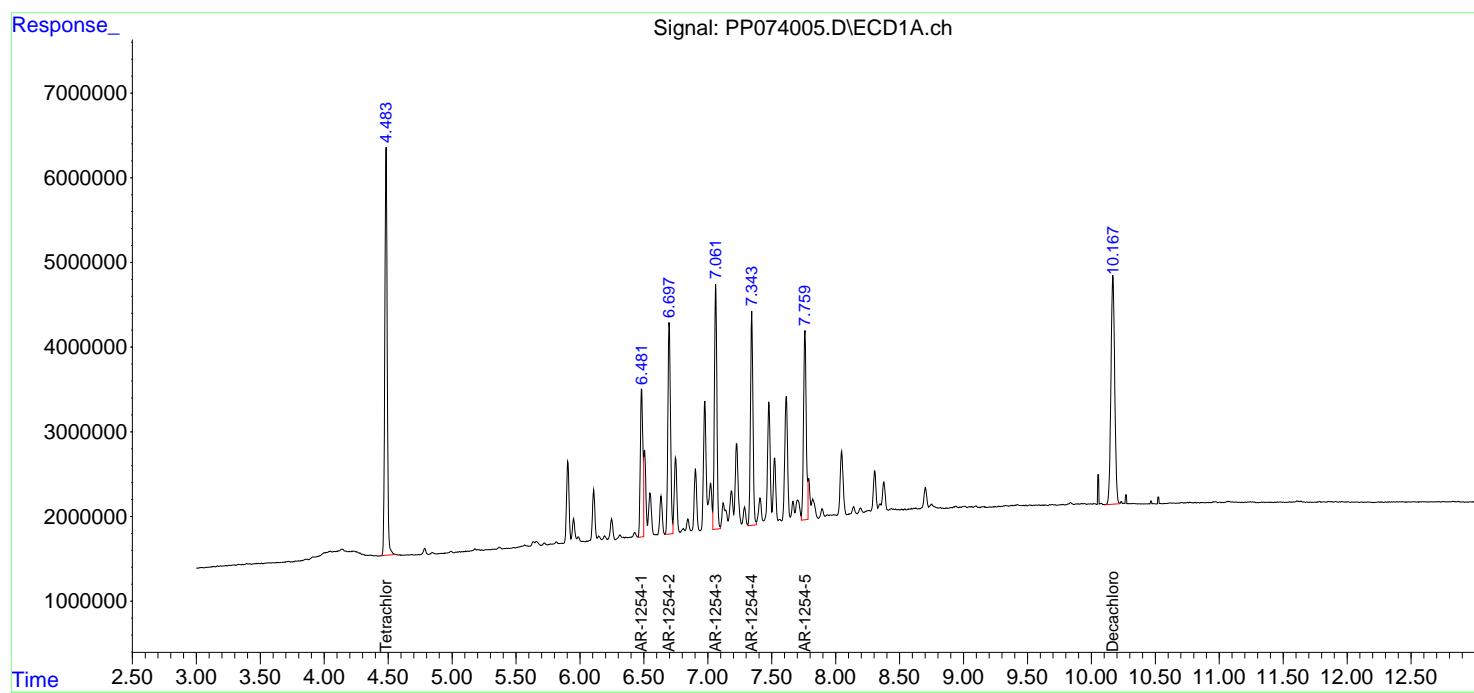


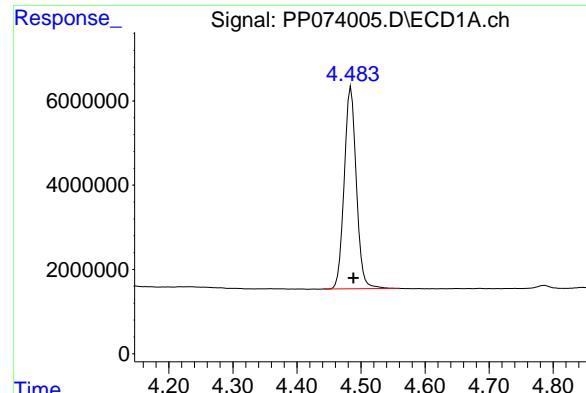

#1 Tetrachloro-m-xylene


R.T.: 4.484 min
Delta R.T.: -0.004 min
Response: 62918811
Conc: 45.94 ng/ml

Instrument: ECD_P
ClientSampleId: AR1254CCC500

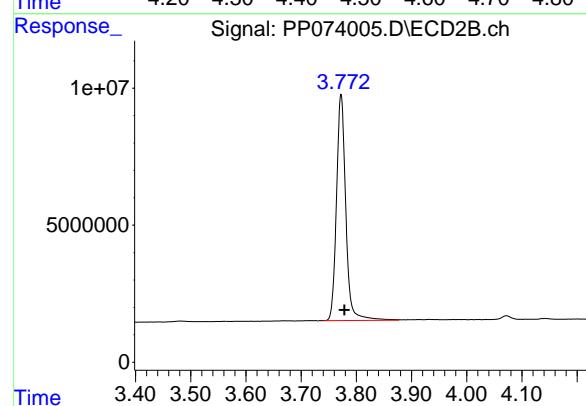


#1 Tetrachloro-m-xylene

R.T.: 3.772 min
Delta R.T.: -0.006 min
Response: 96808458
Conc: 52.55 ng/ml

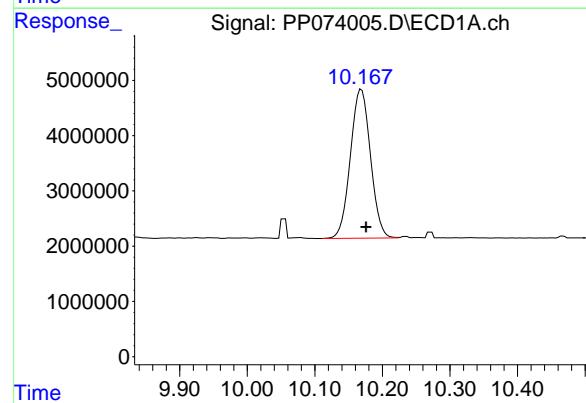

#2 Decachlorobiphenyl

R.T.: 10.169 min
Delta R.T.: -0.007 min
Response: 55557066
Conc: 50.92 ng/ml

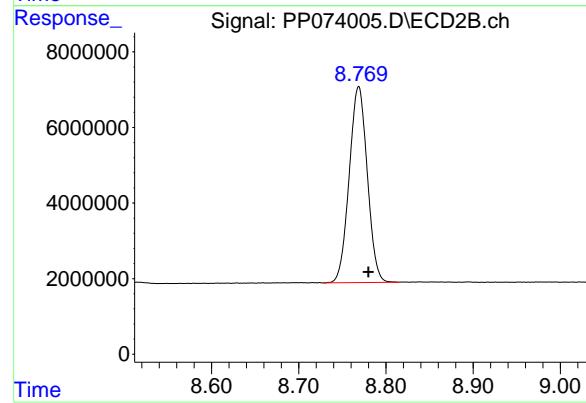


#2 Decachlorobiphenyl

R.T.: 8.769 min
Delta R.T.: -0.011 min
Response: 74740902
Conc: 56.49 ng/ml

#26 AR-1254-1


R.T.: 6.483 min
 Delta R.T.: -0.002 min
 Response: 24087897
 Conc: 449.49 ng/ml

Instrument: ECD_P
 ClientSampleId: AR1254CCC500




#26 AR-1254-1

R.T.: 5.649 min
 Delta R.T.: -0.010 min
 Response: 59799936
 Conc: 515.38 ng/ml




#27 AR-1254-2



R.T.: 6.699 min
 Delta R.T.: -0.002 min
 Response: 35924728
 Conc: 431.33 ng/ml

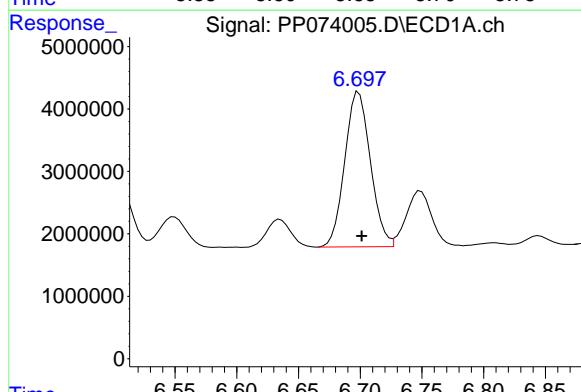

#27 AR-1254-2

R.T.: 5.797 min
 Delta R.T.: -0.010 min
 Response: 50812946
 Conc: 504.98 ng/ml

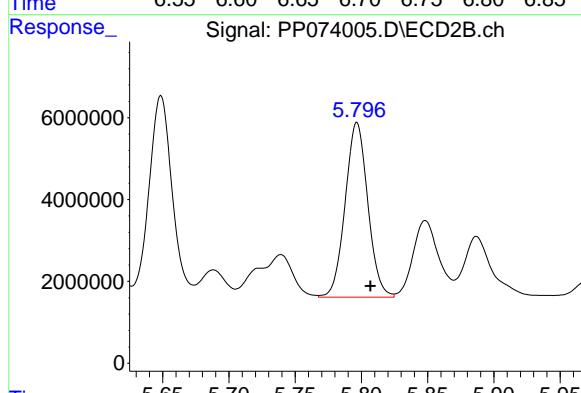

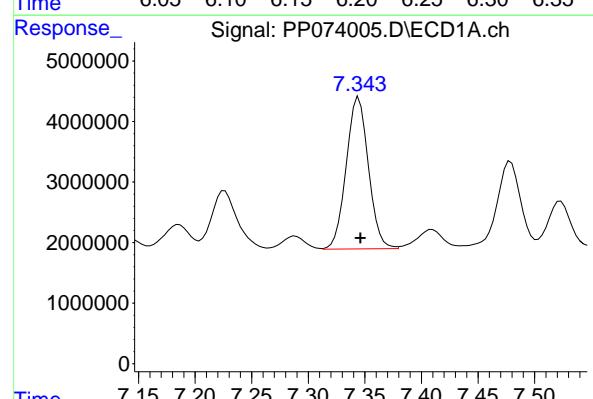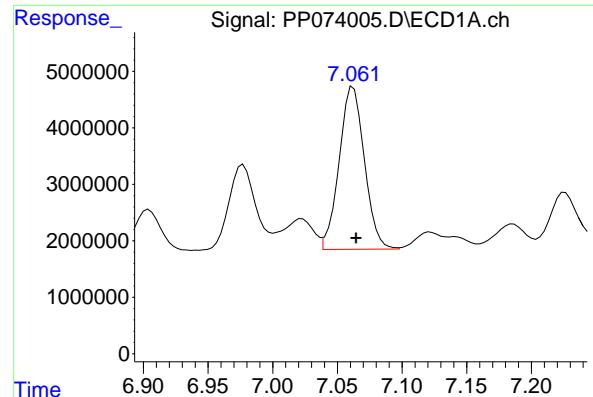

#28 AR-1254-3

R.T.: 7.062 min
 Delta R.T.: -0.002 min
 Response: 39063469
 Conc: 442.24 ng/ml

Instrument: ECD_P
 ClientSampleId: AR1254CCC500

#28 AR-1254-3


R.T.: 6.197 min
 Delta R.T.: -0.012 min
 Response: 78287085
 Conc: 506.89 ng/ml

#29 AR-1254-4

R.T.: 7.345 min
 Delta R.T.: -0.002 min
 Response: 34255719
 Conc: 435.45 ng/ml

#29 AR-1254-4

R.T.: 6.426 min
 Delta R.T.: -0.010 min
 Response: 50083505
 Conc: 529.65 ng/ml

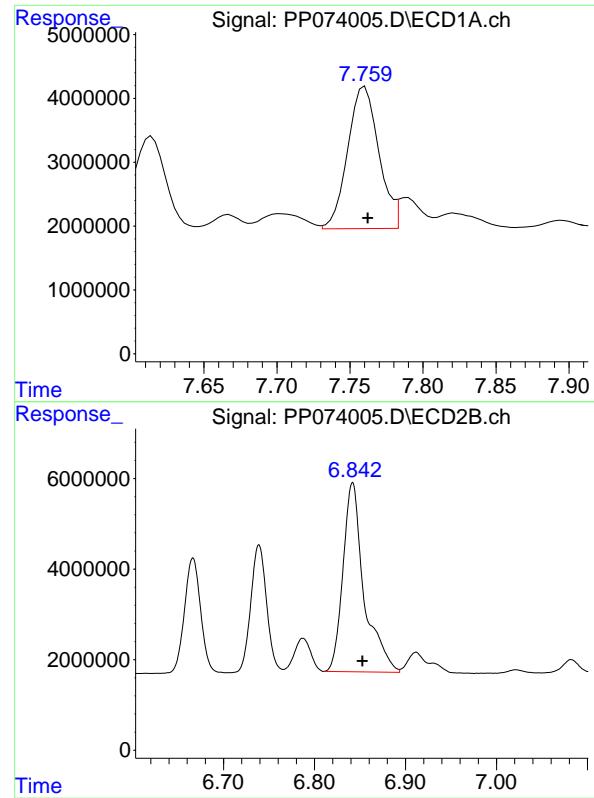

#30 AR-1254-5

R.T.: 7.760 min
Delta R.T.: -0.002 min
Response: 32911104
Conc: 446.68 ng/ml

Instrument: ECD_P
ClientSampleId: AR1254CCC500

#30 AR-1254-5

R.T.: 6.842 min
Delta R.T.: -0.011 min
Response: 67358728
Conc: 504.77 ng/ml

Analytical Sequence

Client: Nobis Group	SDG No.: Q2639		
Project: Raymark Superfund Site	Instrument ID: ECD_O		
GC Column: ZB-MR1	ID: 0.32 (mm)	Inst. Calib. Date(s): 07/08/2025	07/08/2025

THE ANALYTICAL SEQUENCE OF PERFORMANCE EVALUATION MIXTURES, BLANKS, SAMPLES, AND STANDARDS IS GIVEN BELOW:

CLIENT ID	LAB SAMPLE ID	DATE ANALYZED	TIME ANALYZED	DATAFILE	DCB RT #	TCX RT #
I.BLK	I.BLK	07/08/2025	13:49	PO112087.D	8.70	3.67
AR1660ICC1000	AR1660ICC1000	07/08/2025	14:06	PO112088.D	8.70	3.67
AR1660ICC750	AR1660ICC750	07/08/2025	14:25	PO112089.D	8.70	3.67
AR1660ICC500	AR1660ICC500	07/08/2025	14:43	PO112090.D	8.70	3.67
AR1660ICC250	AR1660ICC250	07/08/2025	15:02	PO112091.D	8.70	3.67
AR1660ICC050	AR1660ICC050	07/08/2025	15:21	PO112092.D	8.70	3.67
AR1221ICC500	AR1221ICC500	07/08/2025	15:38	PO112093.D	8.70	3.67
AR1232ICC500	AR1232ICC500	07/08/2025	15:57	PO112094.D	8.70	3.67
AR1242ICC1000	AR1242ICC1000	07/08/2025	16:15	PO112095.D	8.70	3.67
AR1242ICC750	AR1242ICC750	07/08/2025	16:34	PO112096.D	8.70	3.67
AR1242ICC500	AR1242ICC500	07/08/2025	16:52	PO112097.D	8.70	3.67
AR1242ICC250	AR1242ICC250	07/08/2025	17:11	PO112098.D	8.70	3.67
AR1242ICC050	AR1242ICC050	07/08/2025	17:29	PO112099.D	8.70	3.67
AR1248ICC1000	AR1248ICC1000	07/08/2025	17:48	PO112100.D	8.70	3.67
AR1248ICC750	AR1248ICC750	07/08/2025	18:05	PO112101.D	8.70	3.67
AR1248ICC500	AR1248ICC500	07/08/2025	18:24	PO112102.D	8.70	3.67
AR1248ICC250	AR1248ICC250	07/08/2025	18:41	PO112103.D	8.70	3.67
AR1248ICC050	AR1248ICC050	07/08/2025	18:59	PO112104.D	8.70	3.67
AR1254ICC1000	AR1254ICC1000	07/08/2025	19:18	PO112105.D	8.70	3.67
AR1254ICC750	AR1254ICC750	07/08/2025	19:35	PO112106.D	8.70	3.67
AR1254ICC500	AR1254ICC500	07/08/2025	19:54	PO112107.D	8.70	3.67
AR1254ICC250	AR1254ICC250	07/08/2025	20:11	PO112108.D	8.70	3.67
AR1254ICC050	AR1254ICC050	07/08/2025	20:28	PO112109.D	8.70	3.67
AR1262ICC500	AR1262ICC500	07/08/2025	20:47	PO112110.D	8.70	3.67
AR1268ICC1000	AR1268ICC1000	07/08/2025	21:04	PO112111.D	8.70	3.67
AR1268ICC750	AR1268ICC750	07/08/2025	21:22	PO112112.D	8.70	3.67
AR1268ICC500	AR1268ICC500	07/08/2025	21:39	PO112113.D	8.70	3.67
AR1268ICC250	AR1268ICC250	07/08/2025	21:57	PO112114.D	8.70	3.67
AR1268ICC050	AR1268ICC050	07/08/2025	22:16	PO112115.D	8.70	3.67
AR1660CCC500	AR1660CCC500	07/21/2025	10:15	PO112332.D	8.70	3.67
I.BLK	I.BLK	07/21/2025	12:34	PO112336.D	8.70	3.67
OU4-TS-39-071725	Q2639-03	07/21/2025	13:11	PO112338.D	8.70	3.67
OU4-TS-40-071725	Q2639-05	07/21/2025	13:30	PO112339.D	8.70	3.67
OU4-TS-41-071725	Q2639-07	07/21/2025	13:47	PO112340.D	8.70	3.67
AR1660CCC500	AR1660CCC500	07/21/2025	16:10	PO112346.D	8.70	3.67
I.BLK	I.BLK	07/21/2025	17:38	PO112350.D	8.70	3.67
AR1660CCC500	AR1660CCC500	07/22/2025	08:57	PO112366.D	8.70	3.67
I.BLK	I.BLK	07/22/2025	10:08	PO112370.D	8.70	3.67
OU4-TS-42-071725	Q2639-09	07/22/2025	11:08	PO112372.D	8.70	3.67
OU4-TS-43-071725	Q2639-11	07/22/2025	11:26	PO112373.D	8.70	3.67
OU4-TS-44-071725	Q2639-13	07/22/2025	11:44	PO112374.D	8.70	3.67
AR1660CCC500	AR1660CCC500	07/22/2025	16:21	PO112381.D	8.70	3.67

Analytical Sequence

I.BLK	L.BLK	07/22/2025	17:32	PO112385.D	8.70	3.67
L.BLK	L.BLK	07/07/2025	20:30	PP073553.D	10.18	4.49
AR1660ICC1000	AR1660ICC1000	07/07/2025	21:03	PP073554.D	10.18	4.49
AR1660ICC750	AR1660ICC750	07/07/2025	21:19	PP073555.D	10.18	4.49
AR1660ICC500	AR1660ICC500	07/07/2025	21:35	PP073556.D	10.18	4.49
AR1660ICC250	AR1660ICC250	07/07/2025	21:52	PP073557.D	10.18	4.49
AR1660ICC050	AR1660ICC050	07/07/2025	22:08	PP073558.D	10.17	4.49
AR1221ICC500	AR1221ICC500	07/07/2025	22:24	PP073559.D	10.18	4.49
AR1232ICC500	AR1232ICC500	07/07/2025	22:41	PP073560.D	10.18	4.49
AR1242ICC1000	AR1242ICC1000	07/07/2025	22:57	PP073561.D	10.18	4.49
AR1242ICC750	AR1242ICC750	07/07/2025	23:14	PP073562.D	10.18	4.49
AR1242ICC500	AR1242ICC500	07/07/2025	23:30	PP073563.D	10.17	4.49
AR1242ICC250	AR1242ICC250	07/07/2025	23:46	PP073564.D	10.18	4.49
AR1242ICC050	AR1242ICC050	07/08/2025	00:03	PP073565.D	10.17	4.49
AR1248ICC1000	AR1248ICC1000	07/08/2025	00:19	PP073566.D	10.18	4.49
AR1248ICC750	AR1248ICC750	07/08/2025	00:35	PP073567.D	10.18	4.49
AR1248ICC500	AR1248ICC500	07/08/2025	00:52	PP073568.D	10.17	4.49
AR1248ICC250	AR1248ICC250	07/08/2025	01:08	PP073569.D	10.18	4.49
AR1248ICC050	AR1248ICC050	07/08/2025	01:25	PP073570.D	10.17	4.49
AR1254ICC1000	AR1254ICC1000	07/08/2025	01:41	PP073571.D	10.18	4.49
AR1254ICC750	AR1254ICC750	07/08/2025	01:57	PP073572.D	10.18	4.49
AR1254ICC500	AR1254ICC500	07/08/2025	02:14	PP073573.D	10.17	4.49
AR1254ICC250	AR1254ICC250	07/08/2025	02:30	PP073574.D	10.18	4.49
AR1254ICC050	AR1254ICC050	07/08/2025	02:46	PP073575.D	10.18	4.49
AR1262ICC500	AR1262ICC500	07/08/2025	03:03	PP073576.D	10.18	4.49
AR1268ICC1000	AR1268ICC1000	07/08/2025	03:19	PP073577.D	10.18	4.49
AR1268ICC750	AR1268ICC750	07/08/2025	03:35	PP073578.D	10.18	4.49
AR1268ICC500	AR1268ICC500	07/08/2025	03:52	PP073579.D	10.18	4.49
AR1268ICC250	AR1268ICC250	07/08/2025	04:08	PP073580.D	10.17	4.49
AR1268ICC050	AR1268ICC050	07/08/2025	04:24	PP073581.D	10.18	4.49
AR1660CCC500	AR1660CCC500	07/21/2025	08:51	PP073972.D	10.17	4.48
I.BLK	L.BLK	07/21/2025	09:56	PP073976.D	10.17	4.48
RT2286MS	Q2635-01MS	07/21/2025	13:40	PP073984.D	10.17	4.48
RT2286MSD	Q2635-01MSD	07/21/2025	13:56	PP073985.D	10.17	4.49
AR1660CCC500	AR1660CCC500	07/21/2025	15:18	PP073987.D	10.17	4.48
AR1254CCC500	AR1254CCC500	07/21/2025	16:07	PP073990.D	10.17	4.48
I.BLK	L.BLK	07/21/2025	16:23	PP073991.D	10.17	4.48
PB168927BL	PB168927BL	07/21/2025	16:39	PP073992.D	10.17	4.48
PB168927BS	PB168927BS	07/21/2025	16:56	PP073993.D	10.17	4.49
OU4-TS-38-071725	Q2639-01	07/21/2025	19:07	PP074001.D	10.17	4.48
AR1660CCC500	AR1660CCC500	07/21/2025	20:12	PP074002.D	10.17	4.48
AR1254CCC500	AR1254CCC500	07/21/2025	21:17	PP074005.D	10.17	4.48
I.BLK	L.BLK	07/21/2025	21:34	PP074006.D	10.16	4.48

Analytical Sequence

Client: Nobis Group	SDG No.: Q2639		
Project: Raymark Superfund Site	Instrument ID: ECD_O		
GC Column: ZB-MR2	ID: 0.32 (mm)	Inst. Calib. Date(s): 07/08/2025	07/08/2025

THE ANALYTICAL SEQUENCE OF PERFORMANCE EVALUATION MIXTURES, BLANKS, SAMPLES, AND STANDARDS IS GIVEN BELOW:

CLIENT ID	LAB SAMPLE ID	DATE ANALYZED	TIME ANALYZED	DATAFILE	DCB RT #	TCX RT #
I.BLK	I.BLK	07/08/2025	13:49	PO112087.D	8.65	3.67
AR1660ICC1000	AR1660ICC1000	07/08/2025	14:06	PO112088.D	8.65	3.67
AR1660ICC750	AR1660ICC750	07/08/2025	14:25	PO112089.D	8.65	3.67
AR1660ICC500	AR1660ICC500	07/08/2025	14:43	PO112090.D	8.67	3.68
AR1660ICC250	AR1660ICC250	07/08/2025	15:02	PO112091.D	8.65	3.67
AR1660ICC050	AR1660ICC050	07/08/2025	15:21	PO112092.D	8.65	3.67
AR1221ICC500	AR1221ICC500	07/08/2025	15:38	PO112093.D	8.65	3.67
AR1232ICC500	AR1232ICC500	07/08/2025	15:57	PO112094.D	8.65	3.67
AR1242ICC1000	AR1242ICC1000	07/08/2025	16:15	PO112095.D	8.65	3.67
AR1242ICC750	AR1242ICC750	07/08/2025	16:34	PO112096.D	8.65	3.67
AR1242ICC500	AR1242ICC500	07/08/2025	16:52	PO112097.D	8.65	3.67
AR1242ICC250	AR1242ICC250	07/08/2025	17:11	PO112098.D	8.65	3.67
AR1242ICC050	AR1242ICC050	07/08/2025	17:29	PO112099.D	8.65	3.67
AR1248ICC1000	AR1248ICC1000	07/08/2025	17:48	PO112100.D	8.65	3.67
AR1248ICC750	AR1248ICC750	07/08/2025	18:05	PO112101.D	8.65	3.67
AR1248ICC500	AR1248ICC500	07/08/2025	18:24	PO112102.D	8.65	3.67
AR1248ICC250	AR1248ICC250	07/08/2025	18:41	PO112103.D	8.65	3.67
AR1248ICC050	AR1248ICC050	07/08/2025	18:59	PO112104.D	8.65	3.67
AR1254ICC1000	AR1254ICC1000	07/08/2025	19:18	PO112105.D	8.65	3.67
AR1254ICC750	AR1254ICC750	07/08/2025	19:35	PO112106.D	8.65	3.67
AR1254ICC500	AR1254ICC500	07/08/2025	19:54	PO112107.D	8.65	3.67
AR1254ICC250	AR1254ICC250	07/08/2025	20:11	PO112108.D	8.65	3.67
AR1254ICC050	AR1254ICC050	07/08/2025	20:28	PO112109.D	8.65	3.67
AR1262ICC500	AR1262ICC500	07/08/2025	20:47	PO112110.D	8.65	3.67
AR1268ICC1000	AR1268ICC1000	07/08/2025	21:04	PO112111.D	8.65	3.67
AR1268ICC750	AR1268ICC750	07/08/2025	21:22	PO112112.D	8.65	3.67
AR1268ICC500	AR1268ICC500	07/08/2025	21:39	PO112113.D	8.65	3.67
AR1268ICC250	AR1268ICC250	07/08/2025	21:57	PO112114.D	8.65	3.67
AR1268ICC050	AR1268ICC050	07/08/2025	22:16	PO112115.D	8.65	3.67
AR1660CCC500	AR1660CCC500	07/21/2025	10:15	PO112332.D	8.65	3.66
I.BLK	I.BLK	07/21/2025	12:34	PO112336.D	8.65	3.66
OU4-TS-39-071725	Q2639-03	07/21/2025	13:11	PO112338.D	8.65	3.66
OU4-TS-40-071725	Q2639-05	07/21/2025	13:30	PO112339.D	8.65	3.66
OU4-TS-41-071725	Q2639-07	07/21/2025	13:47	PO112340.D	8.65	3.66
AR1660CCC500	AR1660CCC500	07/21/2025	16:10	PO112346.D	8.65	3.66
I.BLK	I.BLK	07/21/2025	17:38	PO112350.D	8.65	3.66
AR1660CCC500	AR1660CCC500	07/22/2025	08:57	PO112366.D	8.64	3.66
I.BLK	I.BLK	07/22/2025	10:08	PO112370.D	8.64	3.66
OU4-TS-42-071725	Q2639-09	07/22/2025	11:08	PO112372.D	8.64	3.66
OU4-TS-43-071725	Q2639-11	07/22/2025	11:26	PO112373.D	8.64	3.66
OU4-TS-44-071725	Q2639-13	07/22/2025	11:44	PO112374.D	8.64	3.66
AR1660CCC500	AR1660CCC500	07/22/2025	16:21	PO112381.D	8.64	3.66

Analytical Sequence

I.BLK	L.BLK	07/22/2025	17:32	PO112385.D	8.64	3.66
L.BLK	L.BLK	07/07/2025	20:30	PP073553.D	8.78	3.78
AR1660ICC1000	AR1660ICC1000	07/07/2025	21:03	PP073554.D	8.78	3.78
AR1660ICC750	AR1660ICC750	07/07/2025	21:19	PP073555.D	8.78	3.78
AR1660ICC500	AR1660ICC500	07/07/2025	21:35	PP073556.D	8.78	3.78
AR1660ICC250	AR1660ICC250	07/07/2025	21:52	PP073557.D	8.78	3.78
AR1660ICC050	AR1660ICC050	07/07/2025	22:08	PP073558.D	8.78	3.78
AR1221ICC500	AR1221ICC500	07/07/2025	22:24	PP073559.D	8.78	3.78
AR1232ICC500	AR1232ICC500	07/07/2025	22:41	PP073560.D	8.78	3.78
AR1242ICC1000	AR1242ICC1000	07/07/2025	22:57	PP073561.D	8.78	3.78
AR1242ICC750	AR1242ICC750	07/07/2025	23:14	PP073562.D	8.78	3.78
AR1242ICC500	AR1242ICC500	07/07/2025	23:30	PP073563.D	8.78	3.78
AR1242ICC250	AR1242ICC250	07/07/2025	23:46	PP073564.D	8.78	3.78
AR1242ICC050	AR1242ICC050	07/08/2025	00:03	PP073565.D	8.78	3.78
AR1248ICC1000	AR1248ICC1000	07/08/2025	00:19	PP073566.D	8.78	3.78
AR1248ICC750	AR1248ICC750	07/08/2025	00:35	PP073567.D	8.78	3.78
AR1248ICC500	AR1248ICC500	07/08/2025	00:52	PP073568.D	8.78	3.78
AR1248ICC250	AR1248ICC250	07/08/2025	01:08	PP073569.D	8.78	3.78
AR1248ICC050	AR1248ICC050	07/08/2025	01:25	PP073570.D	8.78	3.78
AR1254ICC1000	AR1254ICC1000	07/08/2025	01:41	PP073571.D	8.78	3.78
AR1254ICC750	AR1254ICC750	07/08/2025	01:57	PP073572.D	8.78	3.78
AR1254ICC500	AR1254ICC500	07/08/2025	02:14	PP073573.D	8.78	3.78
AR1254ICC250	AR1254ICC250	07/08/2025	02:30	PP073574.D	8.78	3.78
AR1254ICC050	AR1254ICC050	07/08/2025	02:46	PP073575.D	8.78	3.78
AR1262ICC500	AR1262ICC500	07/08/2025	03:03	PP073576.D	8.78	3.78
AR1268ICC1000	AR1268ICC1000	07/08/2025	03:19	PP073577.D	8.78	3.78
AR1268ICC750	AR1268ICC750	07/08/2025	03:35	PP073578.D	8.78	3.78
AR1268ICC500	AR1268ICC500	07/08/2025	03:52	PP073579.D	8.78	3.78
AR1268ICC250	AR1268ICC250	07/08/2025	04:08	PP073580.D	8.78	3.78
AR1268ICC050	AR1268ICC050	07/08/2025	04:24	PP073581.D	8.78	3.78
AR1660CCC500	AR1660CCC500	07/21/2025	08:51	PP073972.D	8.77	3.77
I.BLK	L.BLK	07/21/2025	09:56	PP073976.D	8.77	3.77
RT2286MS	Q2635-01MS	07/21/2025	13:40	PP073984.D	8.77	3.77
RT2286MSD	Q2635-01MSD	07/21/2025	13:56	PP073985.D	8.77	3.77
AR1660CCC500	AR1660CCC500	07/21/2025	15:18	PP073987.D	8.77	3.77
AR1254CCC500	AR1254CCC500	07/21/2025	16:07	PP073990.D	8.77	3.78
I.BLK	L.BLK	07/21/2025	16:23	PP073991.D	8.77	3.77
PB168927BL	PB168927BL	07/21/2025	16:39	PP073992.D	8.77	3.78
PB168927BS	PB168927BS	07/21/2025	16:56	PP073993.D	8.77	3.78
OU4-TS-38-071725	Q2639-01	07/21/2025	19:07	PP074001.D	8.77	3.77
AR1660CCC500	AR1660CCC500	07/21/2025	20:12	PP074002.D	8.77	3.77
AR1254CCC500	AR1254CCC500	07/21/2025	21:17	PP074005.D	8.77	3.77
I.BLK	L.BLK	07/21/2025	21:34	PP074006.D	8.77	3.77



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

IDENTIFICATION SUMMARY
FOR MULTICOMPONENT ANALYTES

SAMPLE NO.

RT2286MS

Lab Name: Alliance Contract: NOBI03
Lab Code: ACE SDG NO.: Q2639
Lab Sample ID: Q2635-01MS Date(s) Analyzed: 07/21/2025 07/21/2025
Instrument ID (1): ECD_P Instrument ID (2): ECD_P
GC Column: (1): ZB-MR1 ID: 0.32 (mm) GC Column: (2): ZB-MR2 ID: 0.32 (mm)
Data file PP073984.D

ANALYTE	COL	RT	RT WINDOW FROM	TO	CONCENTRATION	MEAN CONCENTRATION	%RPD	
Aroclor-1016	1	5.633	5.583	5.683	156	177	1.71	
	2	5.654	5.604	5.704	164			
	3	5.716	5.666	5.766	164			
	4	5.813	5.763	5.863	177			
	5	6.107	6.057	6.157	222			
	1	4.849	4.799	4.899	170	174		
	2	4.867	4.817	4.917	168			
	3	5.043	4.993	5.093	176			
	4	5.085	5.035	5.135	176			
	5	5.298	5.248	5.348	179			
Aroclor-1260	1	7.222	7.172	7.272	231	214	0.94	
	2	7.476	7.426	7.526	204			
	3	7.834	7.784	7.884	203			
	4	8.058	8.008	8.108	222			
	5	8.375	8.325	8.425	209			
	1	6.328	6.278	6.378	222	212		
	2	6.517	6.467	6.567	213			
	3	6.668	6.618	6.718	216			
	4	7.137	7.087	7.187	207			
	5	7.38	7.33	7.43	205			

**IDENTIFICATION SUMMARY
FOR MULTICOMPONENT ANALYTES**

SAMPLE NO.

RT2286MSD

Lab Name:	Alliance	Contract:	NOBI03				
Lab Code:	ACE	SDG NO.:	Q2639				
Lab Sample ID:	Q2635-01MSD	Date(s) Analyzed:	07/21/2025 07/21/2025				
Instrument ID (1):	ECD_P	Instrument ID (2):	ECD_P				
GC Column: (1):	ZB-MR1	ID:	0.32 (mm)	GC Column: (2):	ZB-MR2	ID:	0.32 (mm)
Data file	PP073985.D						

ANALYTE	COL	RT	RT WINDOW		CONCENTRATION	MEAN CONCENTRATION	%RPD
			FROM	TO			
Aroclor-1016	1	5.636	5.586	5.686	155	177	1.71
	2	5.657	5.607	5.707	166		
	3	5.719	5.669	5.769	164		
	4	5.816	5.766	5.866	176		
	5	6.11	6.06	6.16	223		
	1	4.851	4.801	4.901	170		
	2	4.869	4.819	4.919	169		
	3	5.045	4.995	5.095	176		
	4	5.087	5.037	5.137	177		
	5	5.3	5.25	5.35	177	174	
Aroclor-1260	1	7.224	7.174	7.274	211	210	0.48
	2	7.478	7.428	7.528	194		
	3	7.837	7.787	7.887	203		
	4	8.059	8.009	8.109	233		
	5	8.378	8.328	8.428	211		
	1	6.33	6.28	6.38	221		
	2	6.518	6.468	6.568	210		
	3	6.67	6.62	6.72	213		
	4	7.139	7.089	7.189	203		
	5	7.383	7.333	7.433	204	211	

**IDENTIFICATION SUMMARY
FOR MULTICOMPONENT ANALYTES**

SAMPLE NO.

PB168927BS

Lab Name:	Alliance	Contract:	NOBI03				
Lab Code:	ACE	SDG NO.:	Q2639				
Lab Sample ID:	PB168927BS	Date(s) Analyzed:	07/21/2025 07/21/2025				
Instrument ID (1):	ECD_P	Instrument ID (2):	ECD_P				
GC Column: (1):	ZB-MR1	ID:	0.32 (mm)	GC Column: (2):	ZB-MR2	ID:	0.32 (mm)
Data file	PP073993.D						

ANALYTE	COL	RT	RT WINDOW		CONCENTRATION	MEAN CONCENTRATION	%RPD	
			FROM	TO				
Aroclor-1016	1	5.637	5.587	5.687	131	139	9.59	
	2	5.658	5.608	5.708	142			
	3	5.72	5.67	5.77	140			
	4	5.817	5.767	5.867	141			
	5	6.109	6.059	6.159	142			
	1	4.852	4.802	4.902	151	153		
	2	4.87	4.82	4.92	153			
	3	5.047	4.997	5.097	155			
	4	5.089	5.039	5.139	153			
	5	5.301	5.251	5.351	154			
Aroclor-1260	1	7.226	7.176	7.276	147	135	13.15	
	2	7.479	7.429	7.529	131			
	3	7.837	7.787	7.887	124			
	4	8.06	8.01	8.11	138			
	5	8.378	8.328	8.428	134			
	1	6.33	6.28	6.38	159	154		
	2	6.519	6.469	6.569	158			
	3	6.671	6.621	6.721	160			
	4	7.139	7.089	7.189	147			
	5	7.383	7.333	7.433	145			

**IDENTIFICATION SUMMARY
FOR MULTICOMPONENT ANALYTES**

SAMPLE NO.

OU4-TS-38-071725

Lab Name:	Alliance	Contract:	NOBI03				
Lab Code:	ACE	SDG NO.:	Q2639				
Lab Sample ID:	Q2639-01	Date(s) Analyzed:	07/21/2025 07/21/2025				
Instrument ID (1):	ECD_P	Instrument ID (2):	ECD_P				
GC Column: (1):	ZB-MR1	ID:	0.32 (mm)	GC Column: (2):	ZB-MR2	ID:	0.32 (mm)
Data file	PP074001.D						

ANALYTE	COL	RT	RT WINDOW		CONCENTRATION	MEAN CONCENTRATION	%RPD
			FROM	TO			
Aroclor-1254	1	6.479	6.429	6.529	15.1	25.5	3.19
	2	6.699	6.649	6.749	16.3		
	3	7.065	7.015	7.115	26.7		
	4	7.339	7.289	7.389	5.11		
	5	7.776	7.726	7.826	64.5		
	1	5.65	5.6	5.7	14.9		
	2	5.798	5.748	5.848	9.31		
	3	6.214	6.164	6.264	31.1		
	4	6.427	6.377	6.477	4.92		
	5	6.84	6.79	6.89	63.2		



QC SAMPLE

DATA



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

Report of Analysis

Client:	Nobis Group			Date Collected:	
Project:	Raymark Superfund Site			Date Received:	
Client Sample ID:	PB168927BL			SDG No.:	Q2639
Lab Sample ID:	PB168927BL			Matrix:	SOIL
Analytical Method:	8082A			% Solid:	100 Decanted:
Sample Wt/Vol:	30.02	Units:	g	Final Vol:	10000 uL
Soil Aliquot Vol:			uL	Test:	PCB
Extraction Type:				Injection Volume :	
GPC Factor :	1.0	PH :			
Prep Method :	SW3541B				

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PP073992.D	1	07/21/25 08:30	07/21/25 16:39	PB168927

CAS Number	Parameter	Conc.	Qualifier	MDL	LOD	LOQ / CRQL	Units(Dry Weight)
TARGETS							
12674-11-2	Aroclor-1016	8.30	U	3.90	8.30	17.0	ug/kg
11104-28-2	Aroclor-1221	13.0	U	4.00	13.0	17.0	ug/kg
11141-16-5	Aroclor-1232	8.30	U	3.70	8.30	17.0	ug/kg
53469-21-9	Aroclor-1242	8.30	U	4.00	8.30	17.0	ug/kg
12672-29-6	Aroclor-1248	13.0	U	5.90	13.0	17.0	ug/kg
11097-69-1	Aroclor-1254	8.30	U	3.20	8.30	17.0	ug/kg
37324-23-5	Aroclor-1262	13.0	U	5.00	13.0	17.0	ug/kg
11100-14-4	Aroclor-1268	8.30	U	3.60	8.30	17.0	ug/kg
11096-82-5	Aroclor-1260	8.30	U	3.20	8.30	17.0	ug/kg
SURROGATES							
877-09-8	Tetrachloro-m-xylene	18.9		44 - 130		94%	SPK: 20
2051-24-3	Decachlorobiphenyl	21.9		60 - 125		109%	SPK: 20

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP072125\
Data File : PP073992.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Jul 2025 16:39
Operator : YP\AJ
Sample : PB168927BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
PB168927BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 22 02:12:23 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070825.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jul 08 08:35:32 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 μ l
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	4.482	3.775	23731935	34783449	17.329	18.881
2) SA Decachlor...	10.168	8.771	20402079	28960366	18.699	21.887

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP072125\
 Data File : PP073992.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jul 2025 16:39
 Operator : YP\AJ
 Sample : PB168927BL
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 PB168927BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 22 02:12:23 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 08 08:35:32 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

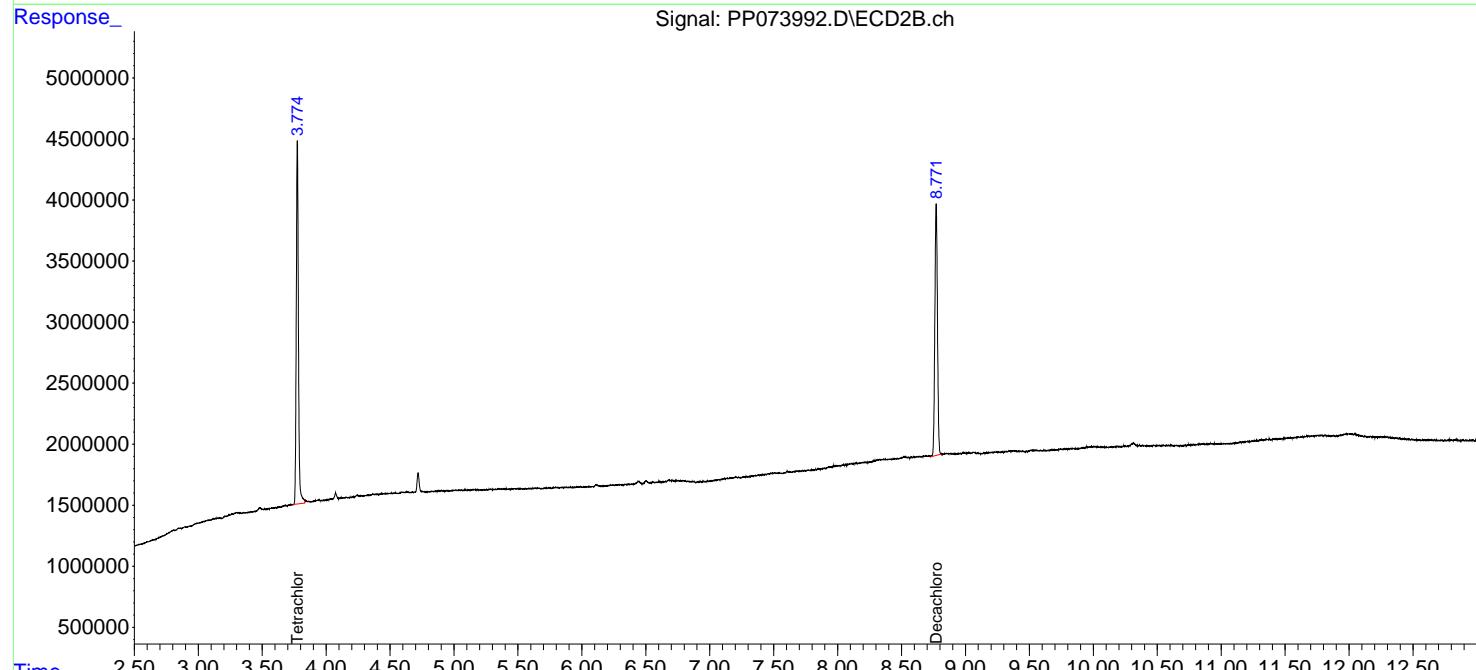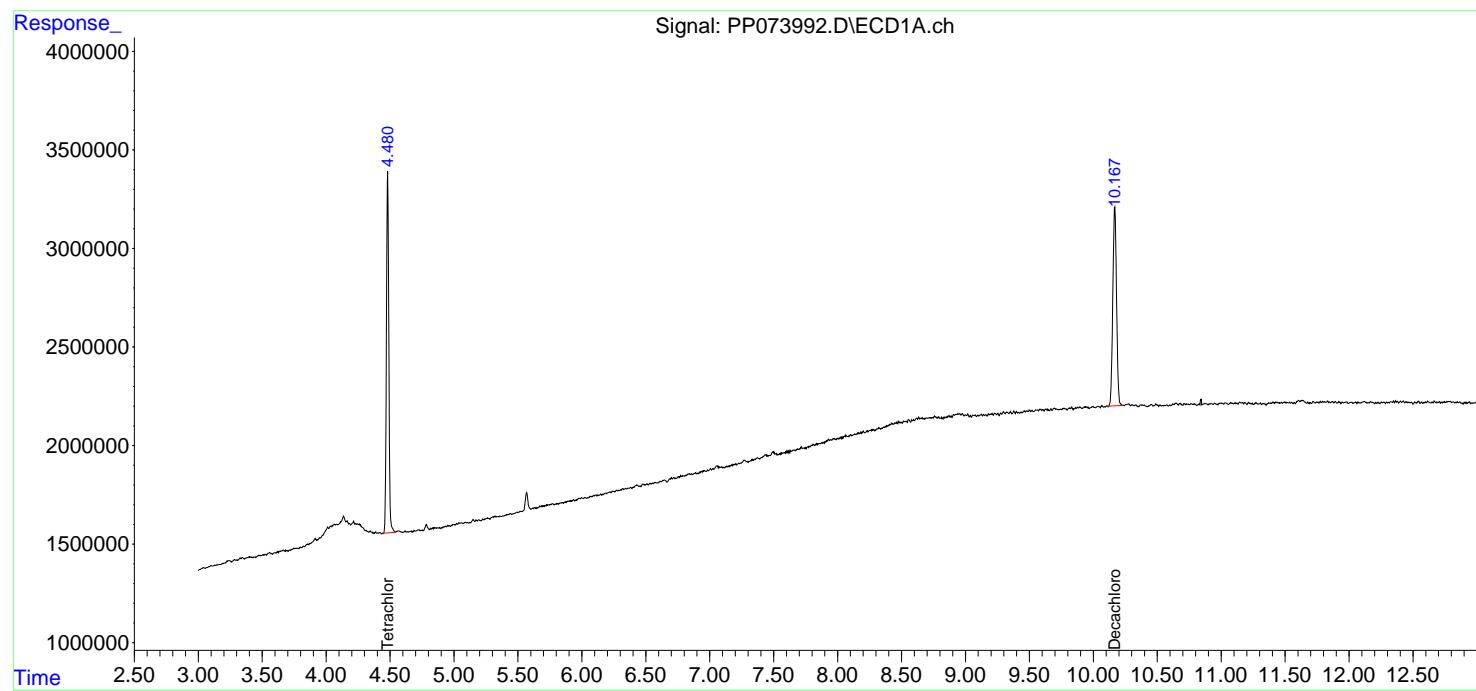


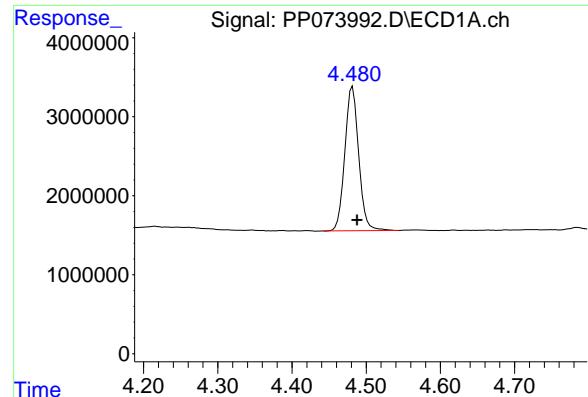

#1 Tetrachloro-m-xylene


R.T.: 4.482 min
Delta R.T.: -0.006 min
Response: 23731935
Conc: 17.33 ng/ml

Instrument: ECD_P
ClientSampleId: PB168927BL

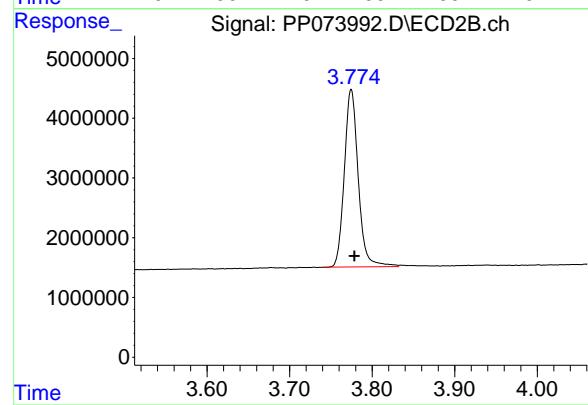


#1 Tetrachloro-m-xylene

R.T.: 3.775 min
Delta R.T.: -0.004 min
Response: 34783449
Conc: 18.88 ng/ml

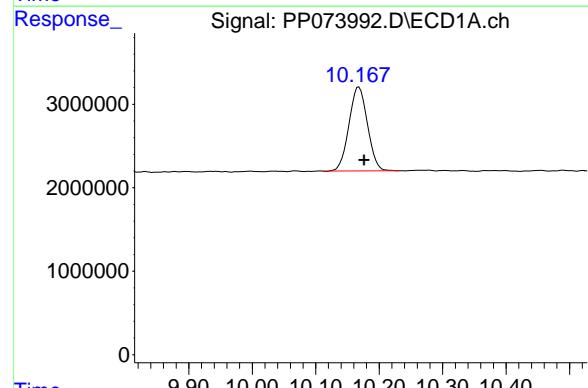

#2 Decachlorobiphenyl

R.T.: 10.168 min
Delta R.T.: -0.008 min
Response: 20402079
Conc: 18.70 ng/ml

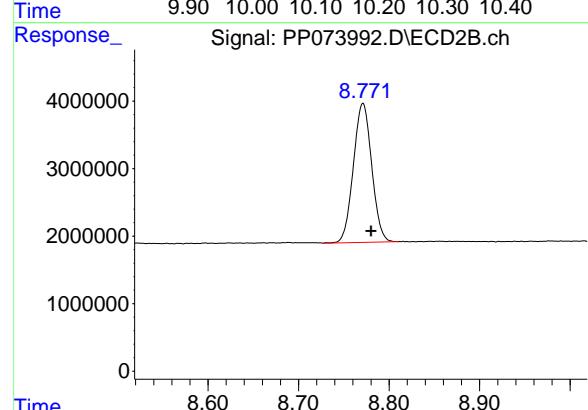

#2 Decachlorobiphenyl

R.T.: 8.771 min
Delta R.T.: -0.009 min
Response: 28960366
Conc: 21.89 ng/ml



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

Report of Analysis

Client:	Nobis Group			Date Collected:	07/08/25			
Project:	Raymark Superfund Site			Date Received:	07/08/25			
Client Sample ID:	PIBLK-PO112087.D			SDG No.:	Q2639			
Lab Sample ID:	I.BLK-PO112087.D			Matrix:	WATER			
Analytical Method:	8082A			% Solid:	0	Decanted:		
Sample Wt/Vol:	1000	Units:	mL	Final Vol:	10000	uL		
Soil Aliquot Vol:	uL			Test:	PCB			
Extraction Type:				Injection Volume :				
GPC Factor :	1.0	PH :						
Prep Method :	5030							

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PO112087.D	1		07/08/25	po070825

CAS Number	Parameter	Conc.	Qualifier	MDL	LOD	LOQ / CRQL	Units
TARGETS							
12674-11-2	Aroclor-1016	0.25	U	0.097	0.25	0.50	ug/L
11104-28-2	Aroclor-1221	0.40	U	0.13	0.40	0.50	ug/L
11141-16-5	Aroclor-1232	0.25	U	0.096	0.25	0.50	ug/L
53469-21-9	Aroclor-1242	0.25	U	0.12	0.25	0.50	ug/L
12672-29-6	Aroclor-1248	0.25	U	0.071	0.25	0.50	ug/L
11097-69-1	Aroclor-1254	0.25	U	0.094	0.25	0.50	ug/L
11096-82-5	Aroclor-1260	0.25	U	0.081	0.25	0.50	ug/L
37324-23-5	Aroclor-1262	0.40	U	0.14	0.40	0.50	ug/L
11100-14-4	Aroclor-1268	0.25	U	0.11	0.25	0.50	ug/L
SURROGATES							
877-09-8	Tetrachloro-m-xylene	19.4		60 - 140		97%	SPK: 20
2051-24-3	Decachlorobiphenyl	18.8		60 - 140		94%	SPK: 20

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0070825\
Data File : P0112087.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Jul 2025 13:49
Operator : YP/AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 09 04:04:19 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070825.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jul 09 04:02:23 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 μ l
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	3.672	3.667	192.2E6	127.1E6	19.421	19.956
2) SA Decachlor...	8.701	8.649	128.3E6	33314140	18.760	19.330

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.





Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0070825\
 Data File : P0112087.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jul 2025 13:49
 Operator : YP/AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 09 04:04:19 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 09 04:02:23 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

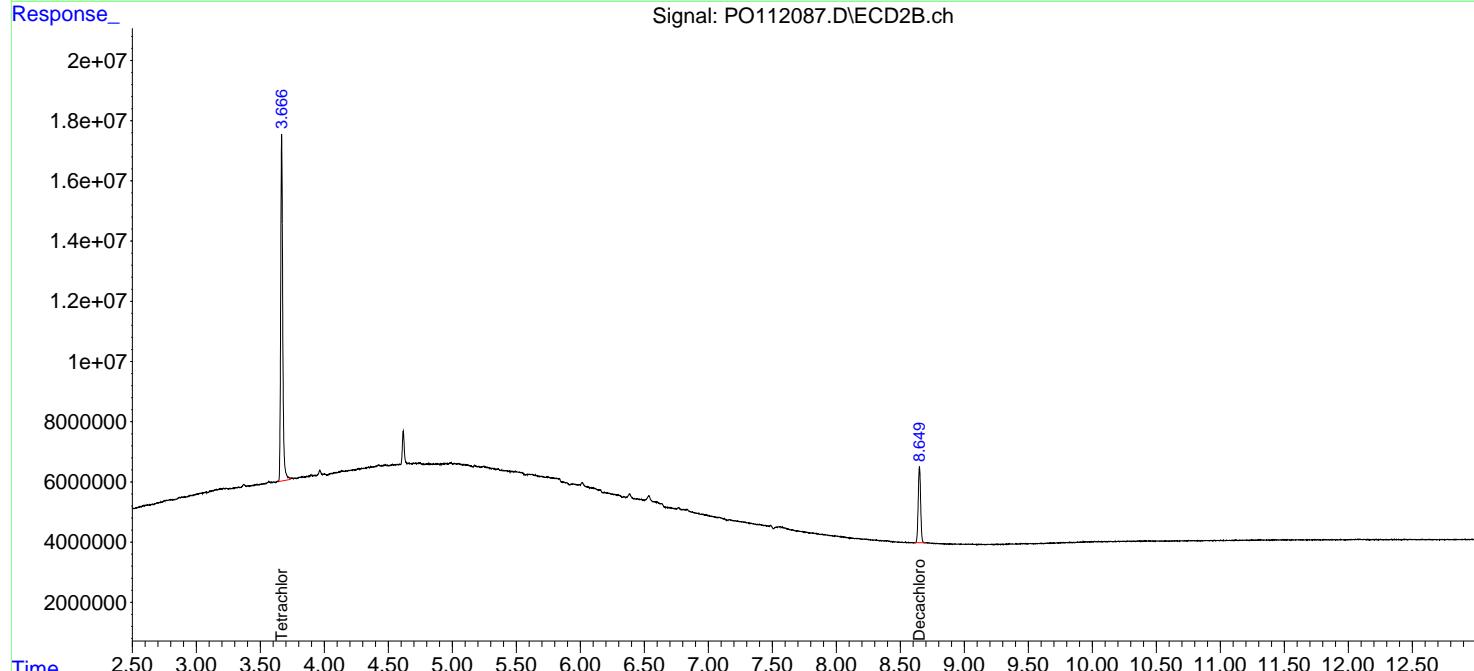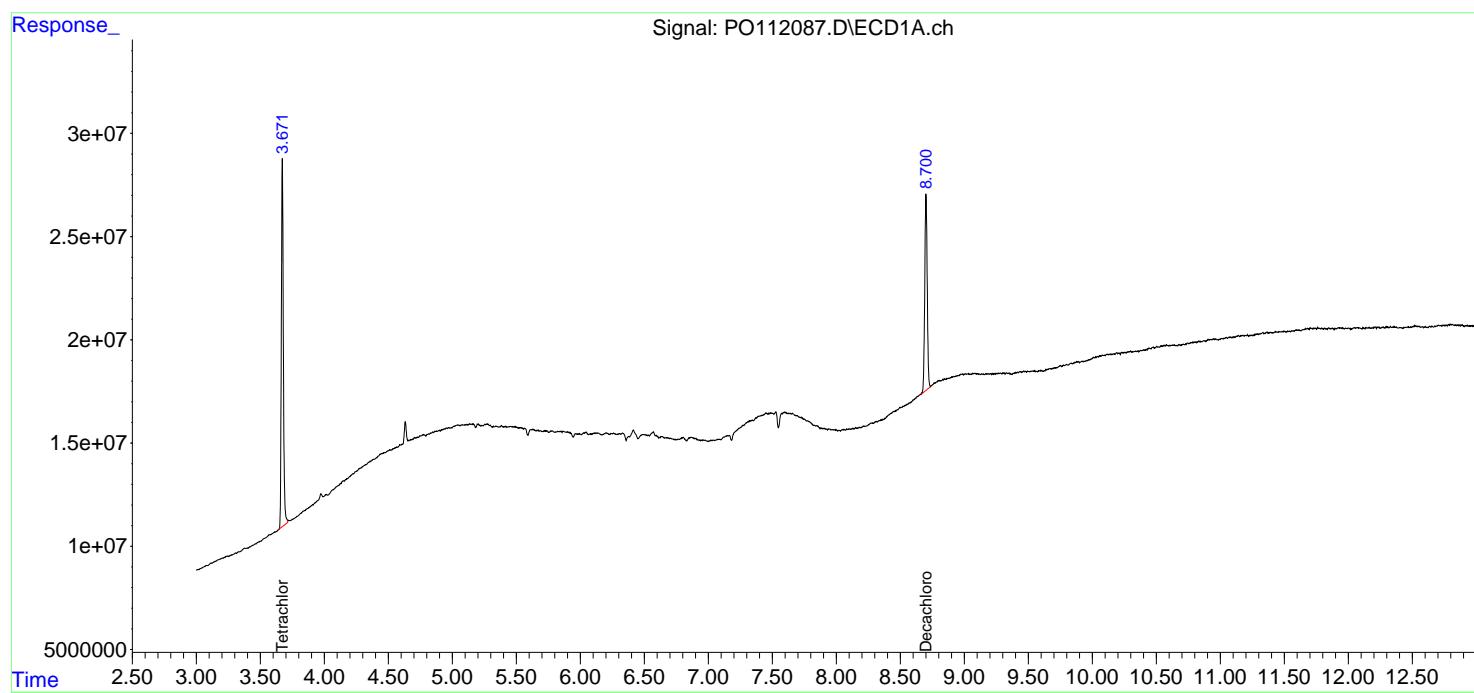

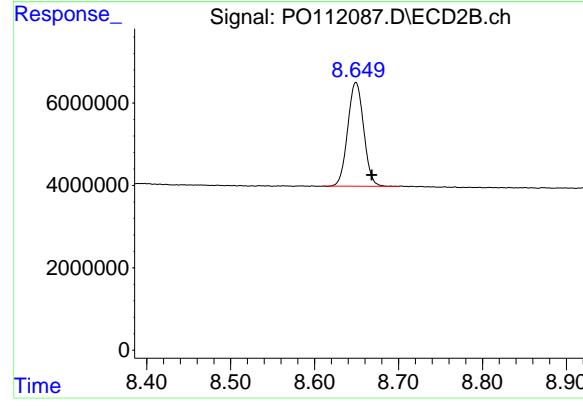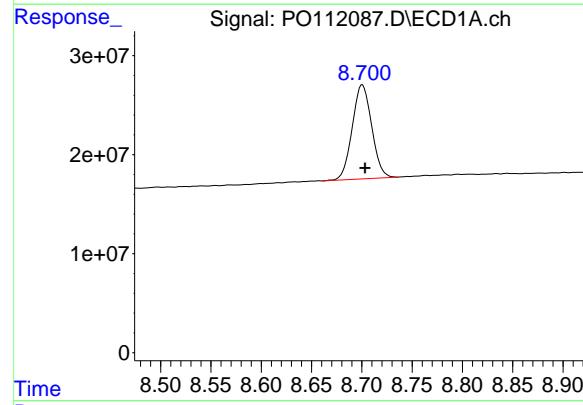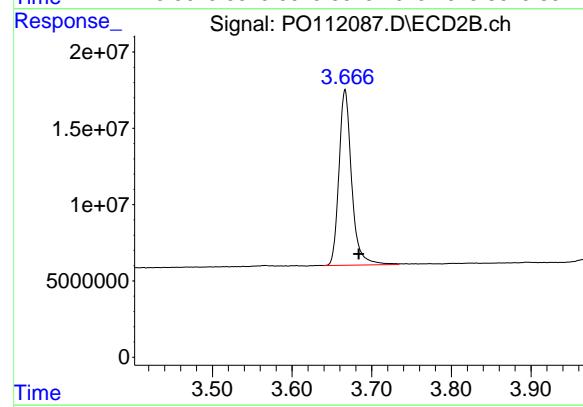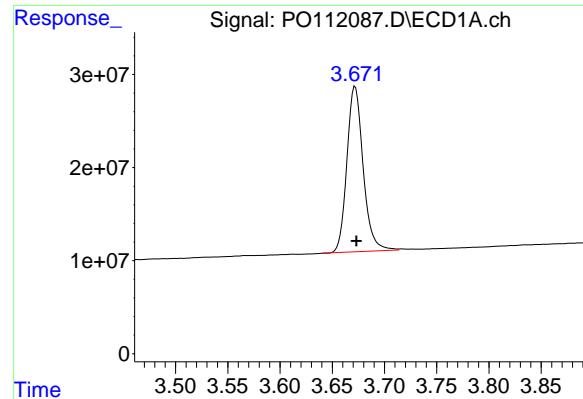

#1 Tetrachloro-m-xylene

R.T.: 3.672 min
Delta R.T.: -0.001 min
Response: 192161483
Conc: 19.42 ng/ml

Instrument: ECD_O
ClientSampleId: I.BLK

#1 Tetrachloro-m-xylene

R.T.: 3.667 min
Delta R.T.: -0.017 min
Response: 127143413
Conc: 19.96 ng/ml

#2 Decachlorobiphenyl

R.T.: 8.701 min
Delta R.T.: -0.003 min
Response: 128266236
Conc: 18.76 ng/ml

#2 Decachlorobiphenyl

R.T.: 8.649 min
Delta R.T.: -0.019 min
Response: 33314140
Conc: 19.33 ng/ml



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

Report of Analysis

Client:	Nobis Group			Date Collected:	07/21/25	
Project:	Raymark Superfund Site			Date Received:	07/21/25	
Client Sample ID:	PIBLK-PO112336.D			SDG No.:	Q2639	
Lab Sample ID:	I.BLK-PO112336.D			Matrix:	WATER	
Analytical Method:	8082A			% Solid:	0	Decanted:
Sample Wt/Vol:	1000	Units:	mL	Final Vol:	10000	uL
Soil Aliquot Vol:	uL			Test:	PCB	
Extraction Type:				Injection Volume :		
GPC Factor :	1.0	PH :				
Prep Method :	5030					

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PO112336.D	1		07/21/25	po072125

CAS Number	Parameter	Conc.	Qualifier	MDL	LOD	LOQ / CRQL	Units
TARGETS							
12674-11-2	Aroclor-1016	0.25	U	0.097	0.25	0.50	ug/L
11104-28-2	Aroclor-1221	0.40	U	0.13	0.40	0.50	ug/L
11141-16-5	Aroclor-1232	0.25	U	0.096	0.25	0.50	ug/L
53469-21-9	Aroclor-1242	0.25	U	0.12	0.25	0.50	ug/L
12672-29-6	Aroclor-1248	0.25	U	0.071	0.25	0.50	ug/L
11097-69-1	Aroclor-1254	0.25	U	0.094	0.25	0.50	ug/L
11096-82-5	Aroclor-1260	0.25	U	0.081	0.25	0.50	ug/L
37324-23-5	Aroclor-1262	0.40	U	0.14	0.40	0.50	ug/L
11100-14-4	Aroclor-1268	0.25	U	0.11	0.25	0.50	ug/L
SURROGATES							
877-09-8	Tetrachloro-m-xylene	20.7		60 - 140		104%	SPK: 20
2051-24-3	Decachlorobiphenyl	17.7		60 - 140		88%	SPK: 20

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0072125\
 Data File : P0112336.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jul 2025 12:34
 Operator : YP/AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 22 01:47:10 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Jul 21 10:54:00 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	3.673	3.664	220.6E6	131.9E6	22.296	20.698
2) SA Decachlor...	8.701	8.646	126.1E6	30465533	18.438	17.677

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0072125\
 Data File : P0112336.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jul 2025 12:34
 Operator : YP/AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 22 01:47:10 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Jul 21 10:54:00 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

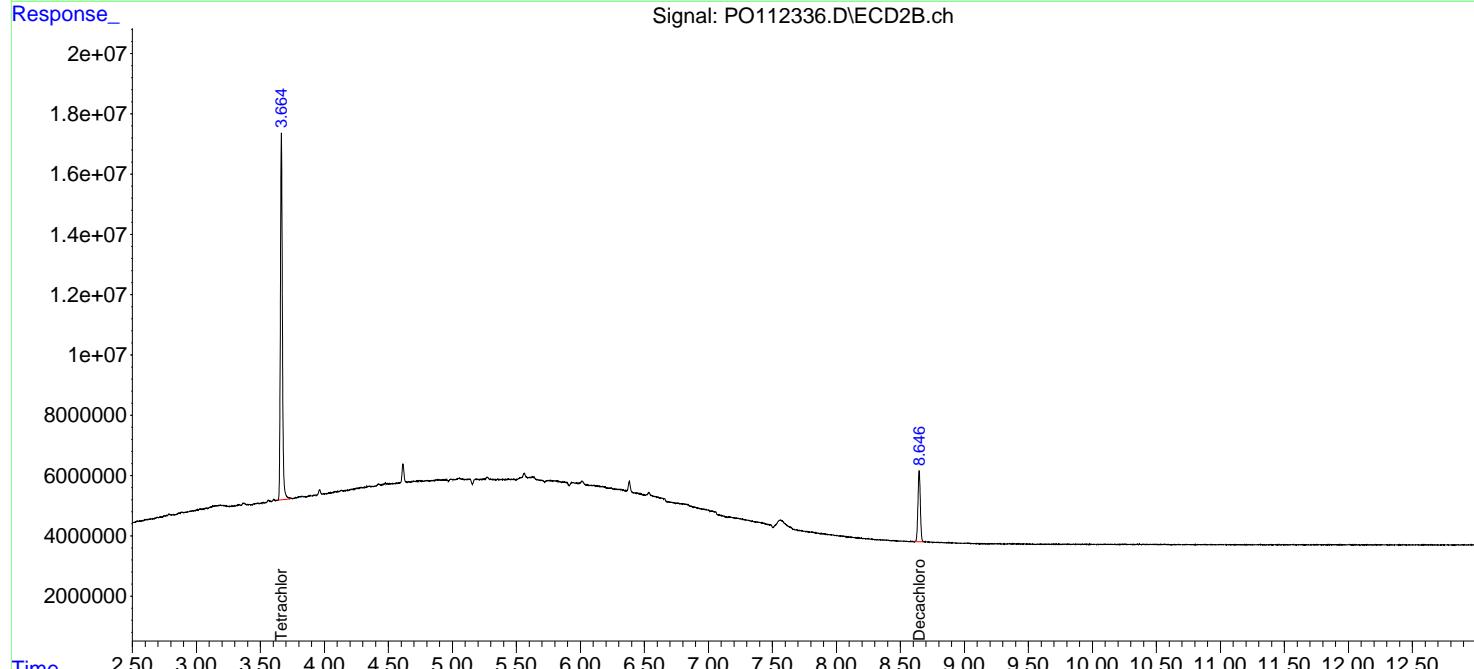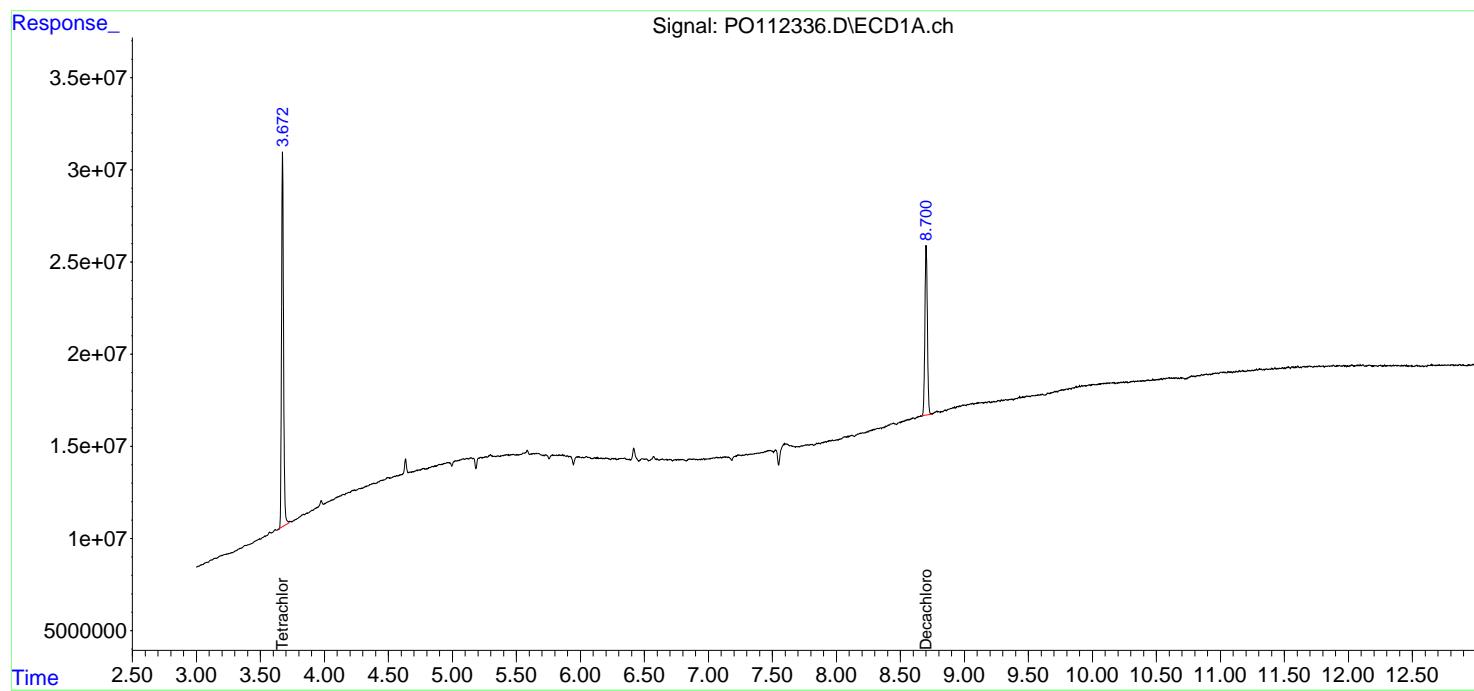




#1 Tetrachloro-m-xylene


R.T.: 3.673 min
Delta R.T.: 0.003 min
Response: 220611369
Conc: 22.30 ng/ml

Instrument: ECD_O
ClientSampleId: I.BLK

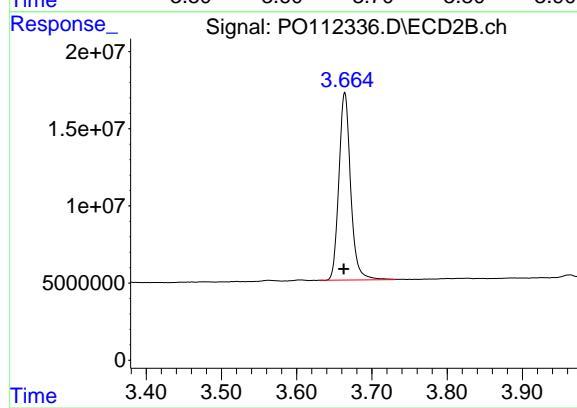


#1 Tetrachloro-m-xylene

R.T.: 3.664 min
Delta R.T.: 0.001 min
Response: 131866827
Conc: 20.70 ng/ml



#2 Decachlorobiphenyl

R.T.: 8.701 min
Delta R.T.: 0.002 min
Response: 126058150
Conc: 18.44 ng/ml

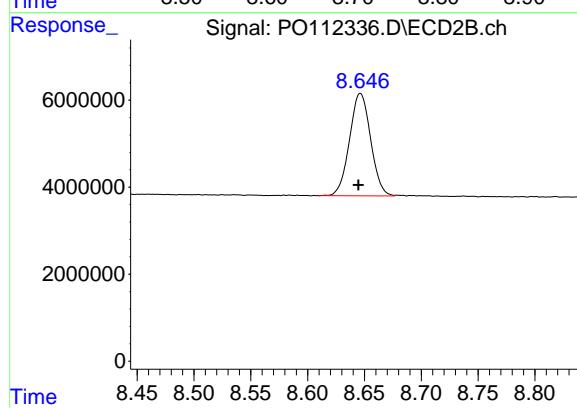

#2 Decachlorobiphenyl

R.T.: 8.646 min
Delta R.T.: 0.002 min
Response: 30465533
Conc: 17.68 ng/ml



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

Report of Analysis

Client:	Nobis Group			Date Collected:	07/21/25	
Project:	Raymark Superfund Site			Date Received:	07/21/25	
Client Sample ID:	PIBLK-PO112350.D			SDG No.:	Q2639	
Lab Sample ID:	I.BLK-PO112350.D			Matrix:	WATER	
Analytical Method:	8082A			% Solid:	0	Decanted:
Sample Wt/Vol:	1000	Units:	mL	Final Vol:	10000	uL
Soil Aliquot Vol:	uL			Test:	PCB	
Extraction Type:				Injection Volume :		
GPC Factor :	1.0	PH :				
Prep Method :	5030					

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PO112350.D	1		07/21/25	po072125

CAS Number	Parameter	Conc.	Qualifier	MDL	LOD	LOQ / CRQL	Units
TARGETS							
12674-11-2	Aroclor-1016	0.25	U	0.097	0.25	0.50	ug/L
11104-28-2	Aroclor-1221	0.40	U	0.13	0.40	0.50	ug/L
11141-16-5	Aroclor-1232	0.25	U	0.096	0.25	0.50	ug/L
53469-21-9	Aroclor-1242	0.25	U	0.12	0.25	0.50	ug/L
12672-29-6	Aroclor-1248	0.25	U	0.071	0.25	0.50	ug/L
11097-69-1	Aroclor-1254	0.25	U	0.094	0.25	0.50	ug/L
11096-82-5	Aroclor-1260	0.25	U	0.081	0.25	0.50	ug/L
37324-23-5	Aroclor-1262	0.40	U	0.14	0.40	0.50	ug/L
11100-14-4	Aroclor-1268	0.25	U	0.11	0.25	0.50	ug/L
SURROGATES							
877-09-8	Tetrachloro-m-xylene	19.0		60 - 140		95%	SPK: 20
2051-24-3	Decachlorobiphenyl	17.4		60 - 140		87%	SPK: 20

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0072125\
 Data File : P0112350.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jul 2025 17:38
 Operator : YP/AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 22 01:53:54 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Jul 21 10:54:00 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	3.669	3.664	199.3E6	121.2E6	20.144	19.021
2) SA Decachlor...	8.698	8.645	120.2E6	29976071	17.574	17.393

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0072125\
 Data File : P0112350.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jul 2025 17:38
 Operator : YP/AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 22 01:53:54 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Jul 21 10:54:00 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

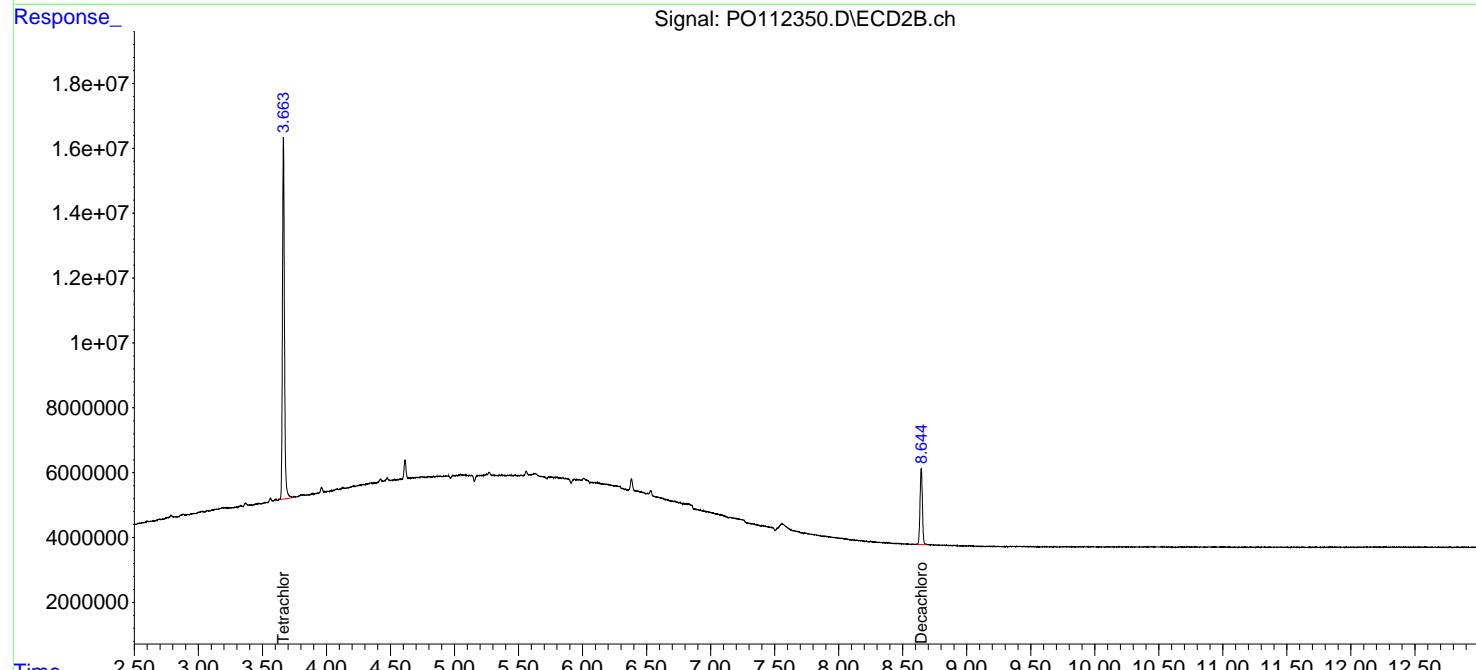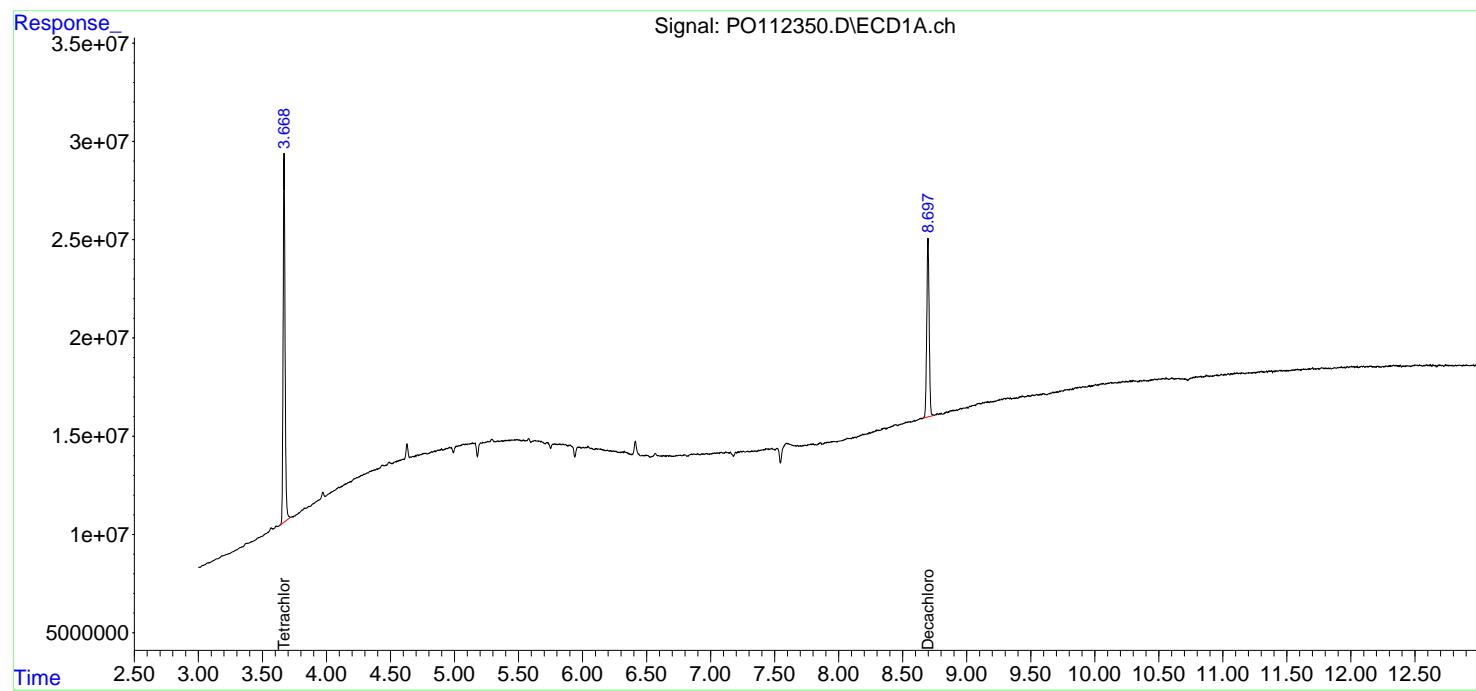

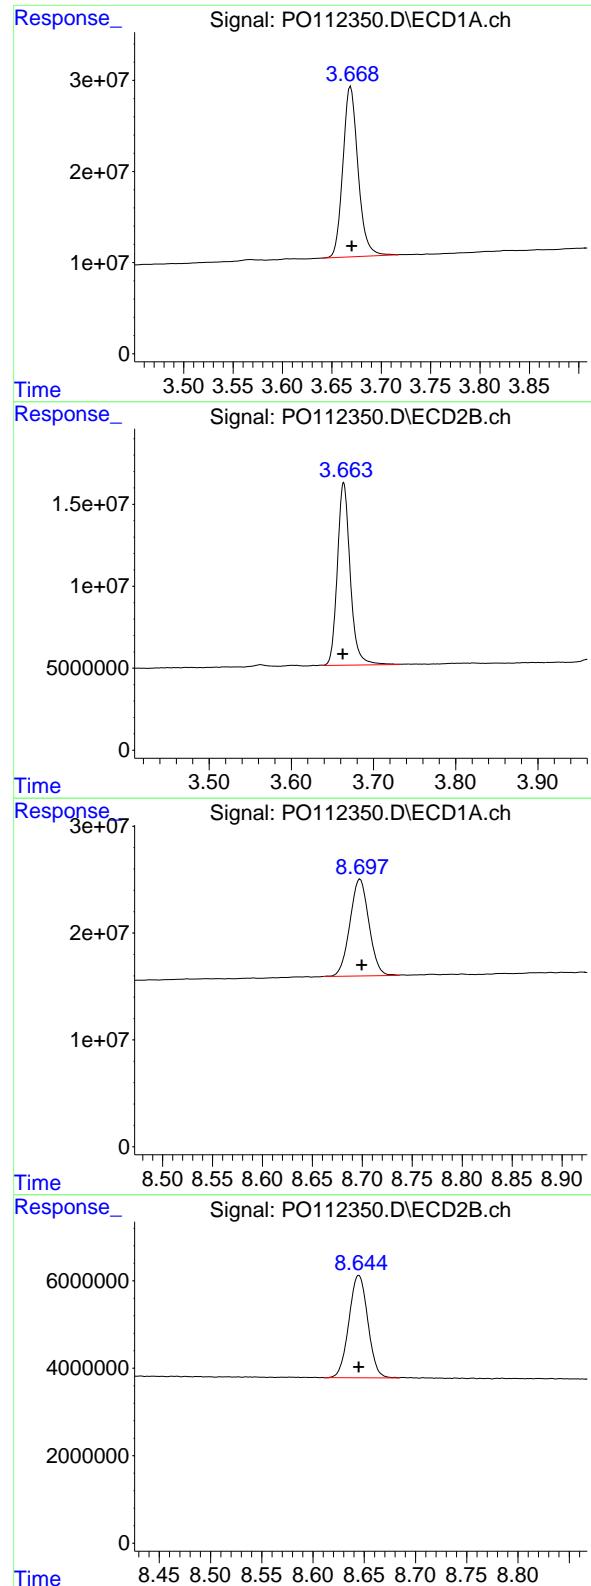

#1 Tetrachloro-m-xylene

R.T.: 3.669 min
Delta R.T.: 0.000 min
Response: 199318998
Conc: 20.14 ng/ml

Instrument: ECD_O
ClientSampleId: I.BLK

#1 Tetrachloro-m-xylene

R.T.: 3.664 min
Delta R.T.: 0.000 min
Response: 121183959
Conc: 19.02 ng/ml

#2 Decachlorobiphenyl

R.T.: 8.698 min
Delta R.T.: -0.002 min
Response: 120156793
Conc: 17.57 ng/ml

#2 Decachlorobiphenyl

R.T.: 8.645 min
Delta R.T.: 0.000 min
Response: 29976071
Conc: 17.39 ng/ml



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

Report of Analysis

Client:	Nobis Group			Date Collected:	07/22/25	
Project:	Raymark Superfund Site			Date Received:	07/22/25	
Client Sample ID:	PIBLK-PO112370.D			SDG No.:	Q2639	
Lab Sample ID:	I.BLK-PO112370.D			Matrix:	WATER	
Analytical Method:	8082A			% Solid:	0	Decanted:
Sample Wt/Vol:	1000	Units:	mL	Final Vol:	10000	uL
Soil Aliquot Vol:	uL			Test:	PCB	
Extraction Type:				Injection Volume :		
GPC Factor :	1.0	PH :				
Prep Method :	5030					

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PO112370.D	1		07/22/25	po072225

CAS Number	Parameter	Conc.	Qualifier	MDL	LOD	LOQ / CRQL	Units
TARGETS							
12674-11-2	Aroclor-1016	0.25	U	0.097	0.25	0.50	ug/L
11104-28-2	Aroclor-1221	0.40	U	0.13	0.40	0.50	ug/L
11141-16-5	Aroclor-1232	0.25	U	0.096	0.25	0.50	ug/L
53469-21-9	Aroclor-1242	0.25	U	0.12	0.25	0.50	ug/L
12672-29-6	Aroclor-1248	0.25	U	0.071	0.25	0.50	ug/L
11097-69-1	Aroclor-1254	0.25	U	0.094	0.25	0.50	ug/L
11096-82-5	Aroclor-1260	0.25	U	0.081	0.25	0.50	ug/L
37324-23-5	Aroclor-1262	0.40	U	0.14	0.40	0.50	ug/L
11100-14-4	Aroclor-1268	0.25	U	0.11	0.25	0.50	ug/L
SURROGATES							
877-09-8	Tetrachloro-m-xylene	18.3		60 - 140		91%	SPK: 20
2051-24-3	Decachlorobiphenyl	17.4		60 - 140		87%	SPK: 20

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0072225\
 Data File : P0112370.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Jul 2025 10:08
 Operator : YP/AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 22 10:37:30 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 22 09:14:26 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	3.670	3.662	198.4E6	116.3E6	20.046	18.256
2) SA Decachlor...	8.698	8.642	121.1E6	29977061	17.713	17.394

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0072225\
 Data File : P0112370.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Jul 2025 10:08
 Operator : YP/AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 22 10:37:30 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 22 09:14:26 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

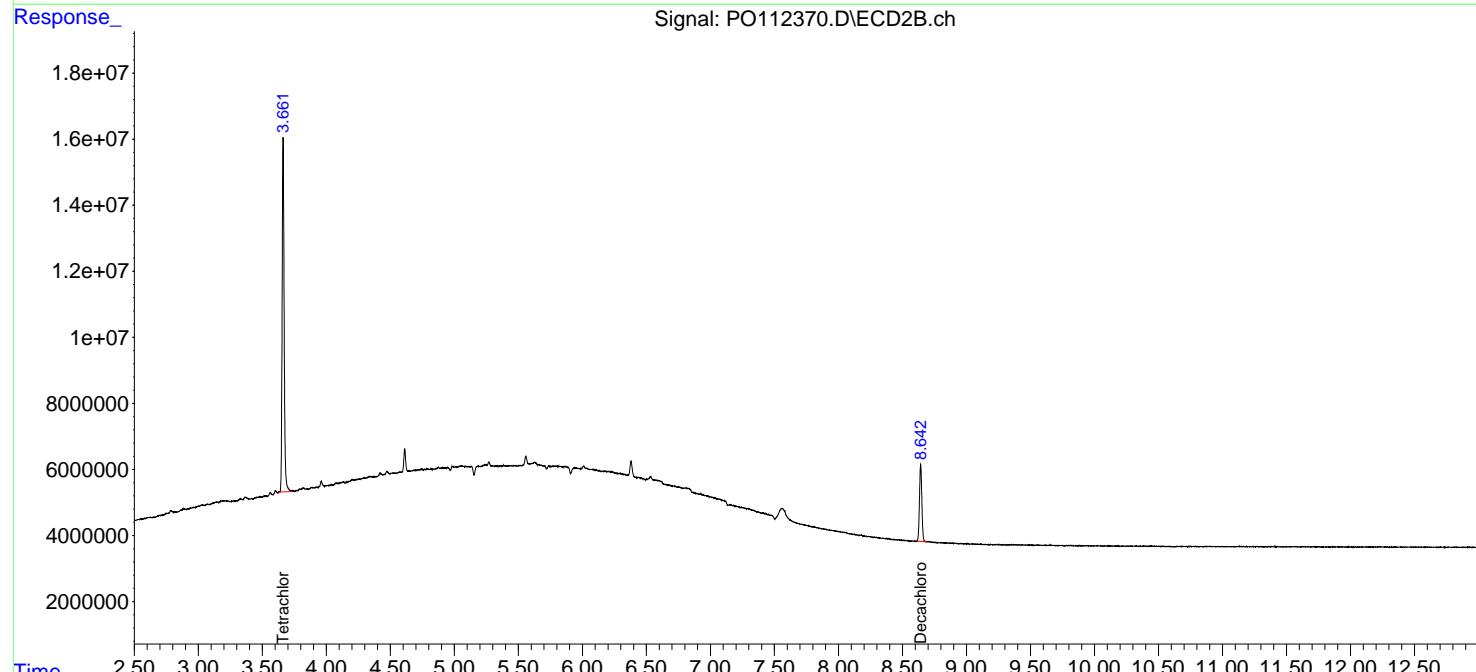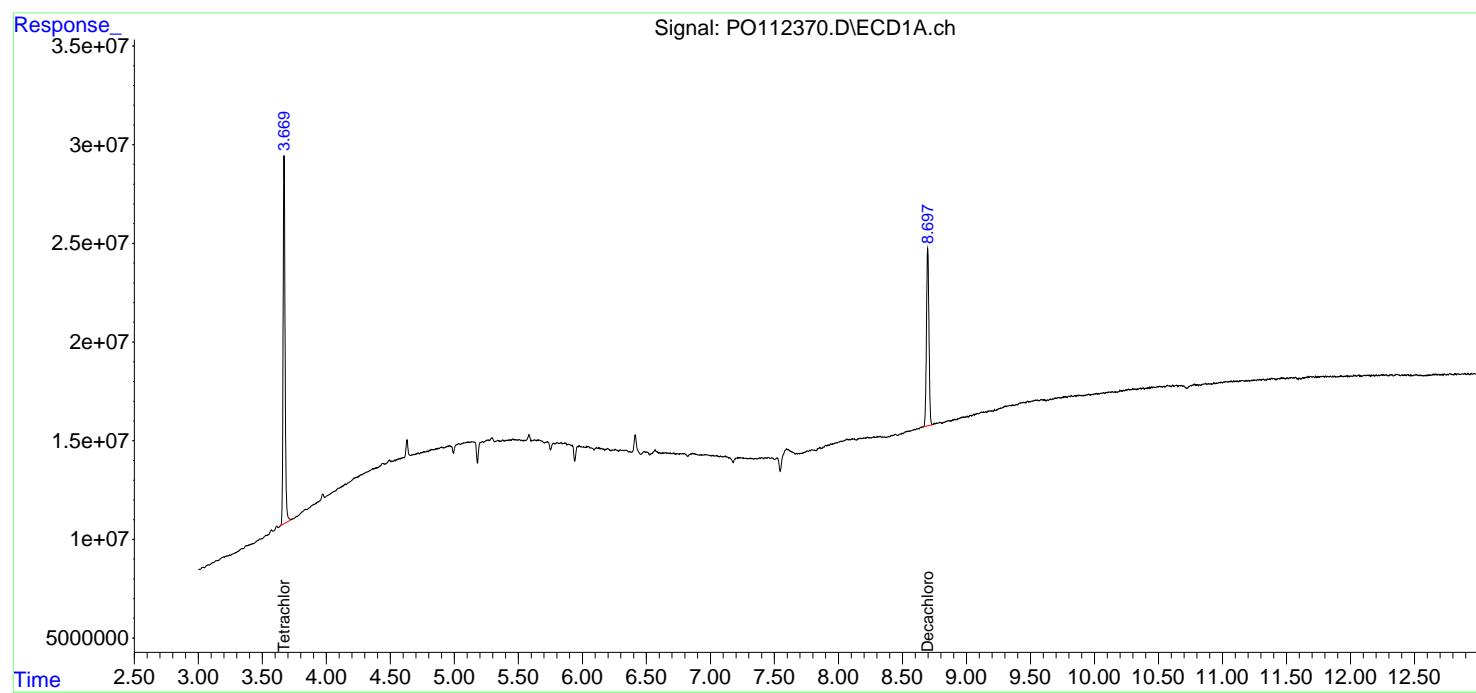


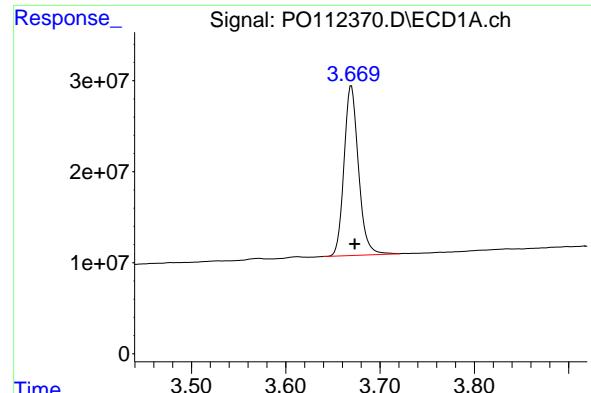

#1 Tetrachloro-m-xylene


R.T.: 3.670 min
Delta R.T.: -0.003 min
Response: 198352825
Conc: 20.05 ng/ml

Instrument: ECD_O
ClientSampleId: I.BLK

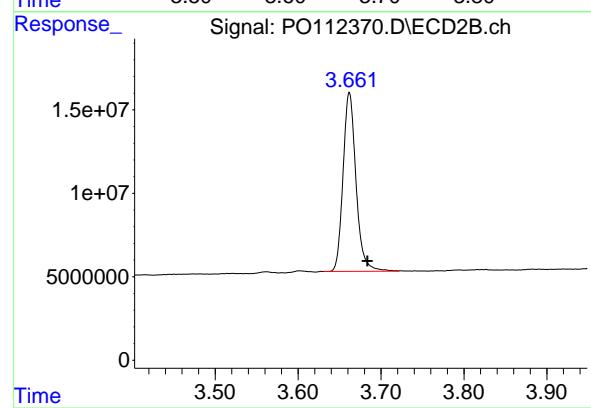


#1 Tetrachloro-m-xylene

R.T.: 3.662 min
Delta R.T.: -0.022 min
Response: 116310058
Conc: 18.26 ng/ml

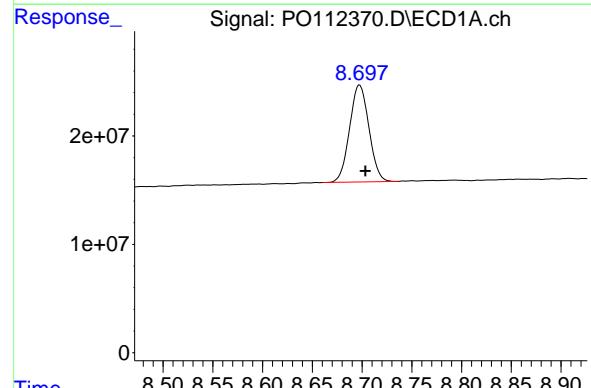

#2 Decachlorobiphenyl

R.T.: 8.698 min
Delta R.T.: -0.006 min
Response: 121107515
Conc: 17.71 ng/ml

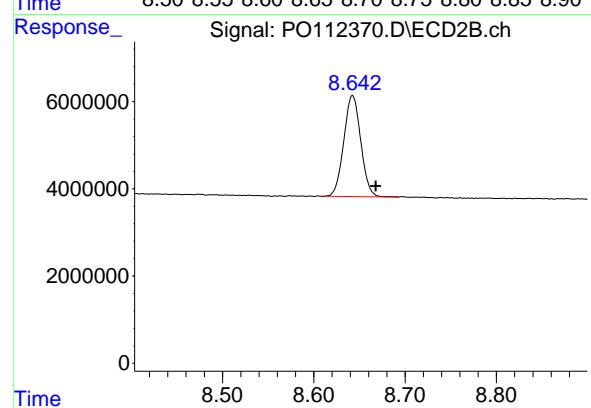

#2 Decachlorobiphenyl

R.T.: 8.642 min
Delta R.T.: -0.026 min
Response: 29977061
Conc: 17.39 ng/ml



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

Report of Analysis

Client:	Nobis Group			Date Collected:	07/22/25	
Project:	Raymark Superfund Site			Date Received:	07/22/25	
Client Sample ID:	PIBLK-PO112385.D			SDG No.:	Q2639	
Lab Sample ID:	I.BLK-PO112385.D			Matrix:	WATER	
Analytical Method:	8082A			% Solid:	0	Decanted:
Sample Wt/Vol:	1000	Units:	mL	Final Vol:	10000	uL
Soil Aliquot Vol:	uL			Test:	PCB	
Extraction Type:				Injection Volume :		
GPC Factor :	1.0	PH :				
Prep Method :	5030					

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PO112385.D	1		07/22/25	po072225

CAS Number	Parameter	Conc.	Qualifier	MDL	LOD	LOQ / CRQL	Units
TARGETS							
12674-11-2	Aroclor-1016	0.25	U	0.097	0.25	0.50	ug/L
11104-28-2	Aroclor-1221	0.40	U	0.13	0.40	0.50	ug/L
11141-16-5	Aroclor-1232	0.25	U	0.096	0.25	0.50	ug/L
53469-21-9	Aroclor-1242	0.25	U	0.12	0.25	0.50	ug/L
12672-29-6	Aroclor-1248	0.25	U	0.071	0.25	0.50	ug/L
11097-69-1	Aroclor-1254	0.25	U	0.094	0.25	0.50	ug/L
11096-82-5	Aroclor-1260	0.25	U	0.081	0.25	0.50	ug/L
37324-23-5	Aroclor-1262	0.40	U	0.14	0.40	0.50	ug/L
11100-14-4	Aroclor-1268	0.25	U	0.11	0.25	0.50	ug/L
SURROGATES							
877-09-8	Tetrachloro-m-xylene	18.1		60 - 140		90%	SPK: 20
2051-24-3	Decachlorobiphenyl	17.4		60 - 140		87%	SPK: 20

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0072225\
 Data File : P0112385.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Jul 2025 17:32
 Operator : YP/AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 23 01:54:29 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 22 09:14:26 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	3.670	3.662	195.5E6	115.0E6	19.763	18.050
2) SA Decachlor...	8.695	8.641	120.4E6	30026588	17.607	17.422

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0072225\
 Data File : P0112385.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Jul 2025 17:32
 Operator : YP/AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 23 01:54:29 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 22 09:14:26 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

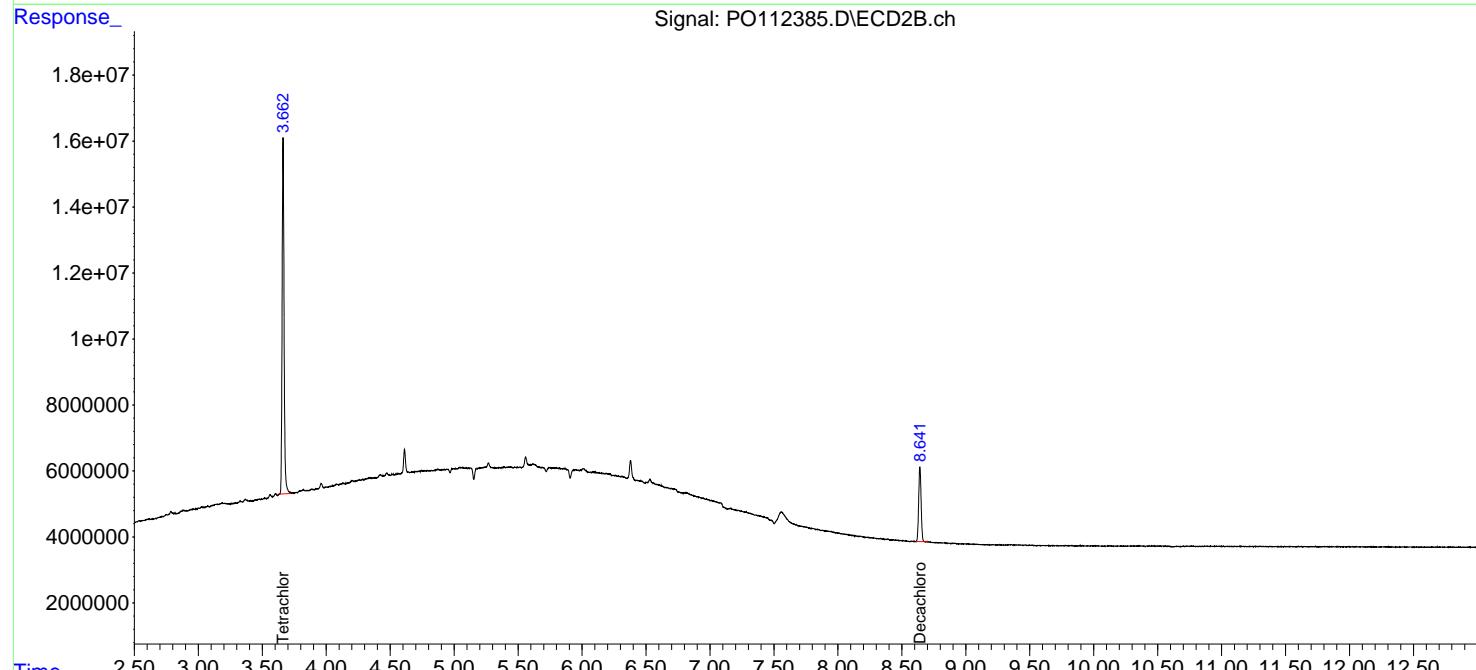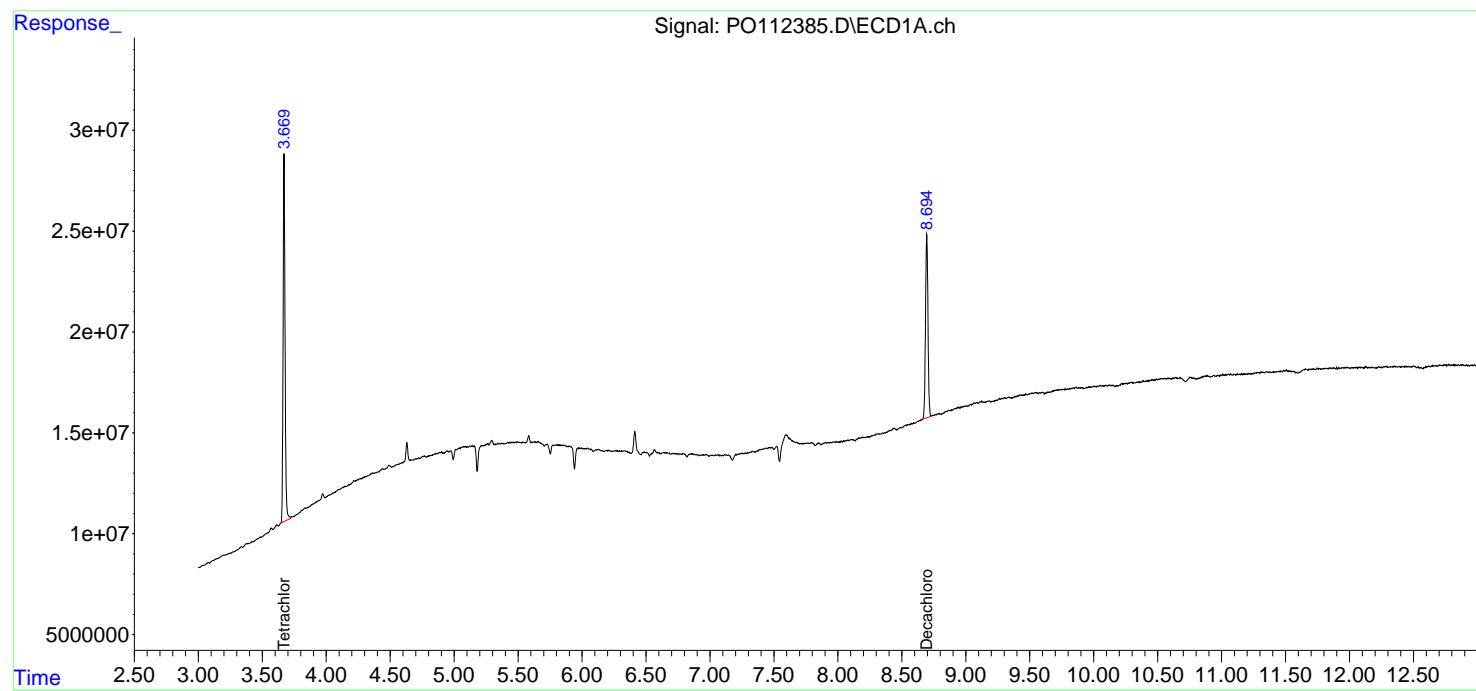

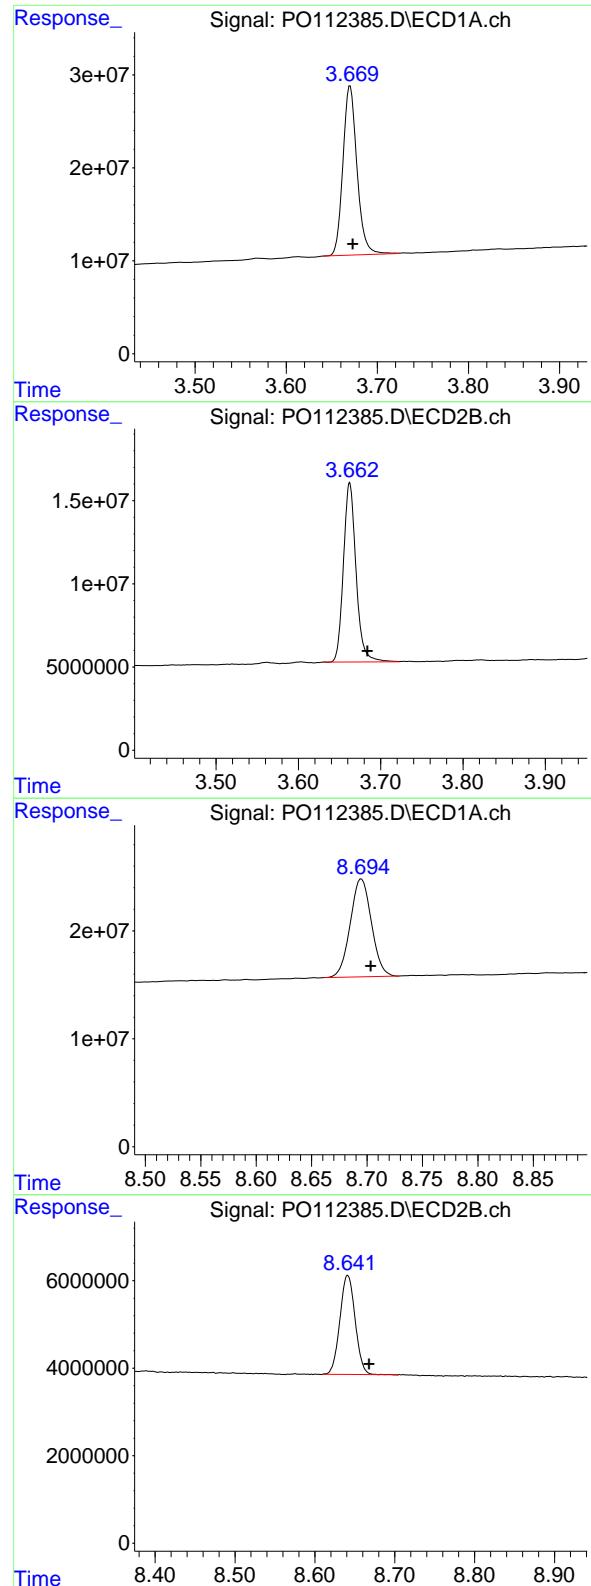

#1 Tetrachloro-m-xylene

R.T.: 3.670 min
 Delta R.T.: -0.003 min
 Response: 195544841
 Conc: 19.76 ng/ml

Instrument: ECD_O
 ClientSampleId: I.BLK

#1 Tetrachloro-m-xylene

R.T.: 3.662 min
 Delta R.T.: -0.021 min
 Response: 115000490
 Conc: 18.05 ng/ml

#2 Decachlorobiphenyl

R.T.: 8.695 min
 Delta R.T.: -0.008 min
 Response: 120379192
 Conc: 17.61 ng/ml

#2 Decachlorobiphenyl

R.T.: 8.641 min
 Delta R.T.: -0.027 min
 Response: 30026588
 Conc: 17.42 ng/ml



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

Report of Analysis

Client:	Nobis Group			Date Collected:	07/07/25			
Project:	Raymark Superfund Site			Date Received:	07/07/25			
Client Sample ID:	PIBLK-PP073553.D			SDG No.:	Q2639			
Lab Sample ID:	I.BLK-PP073553.D			Matrix:	WATER			
Analytical Method:	8082A			% Solid:	0	Decanted:		
Sample Wt/Vol:	1000	Units:	mL	Final Vol:	10000	uL		
Soil Aliquot Vol:	uL			Test:	PCB			
Extraction Type:				Injection Volume :				
GPC Factor :	1.0	PH :						
Prep Method :	5030							

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PP073553.D	1		07/07/25	pp070825

CAS Number	Parameter	Conc.	Qualifier	MDL	LOD	LOQ / CRQL	Units
TARGETS							
12674-11-2	Aroclor-1016	0.25	U	0.097	0.25	0.50	ug/L
11104-28-2	Aroclor-1221	0.40	U	0.13	0.40	0.50	ug/L
11141-16-5	Aroclor-1232	0.25	U	0.096	0.25	0.50	ug/L
53469-21-9	Aroclor-1242	0.25	U	0.12	0.25	0.50	ug/L
12672-29-6	Aroclor-1248	0.25	U	0.071	0.25	0.50	ug/L
11097-69-1	Aroclor-1254	0.25	U	0.094	0.25	0.50	ug/L
11096-82-5	Aroclor-1260	0.25	U	0.081	0.25	0.50	ug/L
37324-23-5	Aroclor-1262	0.40	U	0.14	0.40	0.50	ug/L
11100-14-4	Aroclor-1268	0.25	U	0.11	0.25	0.50	ug/L
SURROGATES							
877-09-8	Tetrachloro-m-xylene	16.2		60 - 140		81%	SPK: 20
2051-24-3	Decachlorobiphenyl	17.1		60 - 140		85%	SPK: 20

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP070825\
Data File : PP073553.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Jul 2025 20:30
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 08 08:36:05 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070825.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jul 08 08:22:37 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 μ l
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	4.489	3.780	22153163	29828480	16.176	16.191
2) SA Decachlor...	10.178	8.781	18922819	22582394	17.344	17.067

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.





Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP070825\
 Data File : PP073553.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Jul 2025 20:30
 Operator : YP\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 08 08:36:05 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 08 08:22:37 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

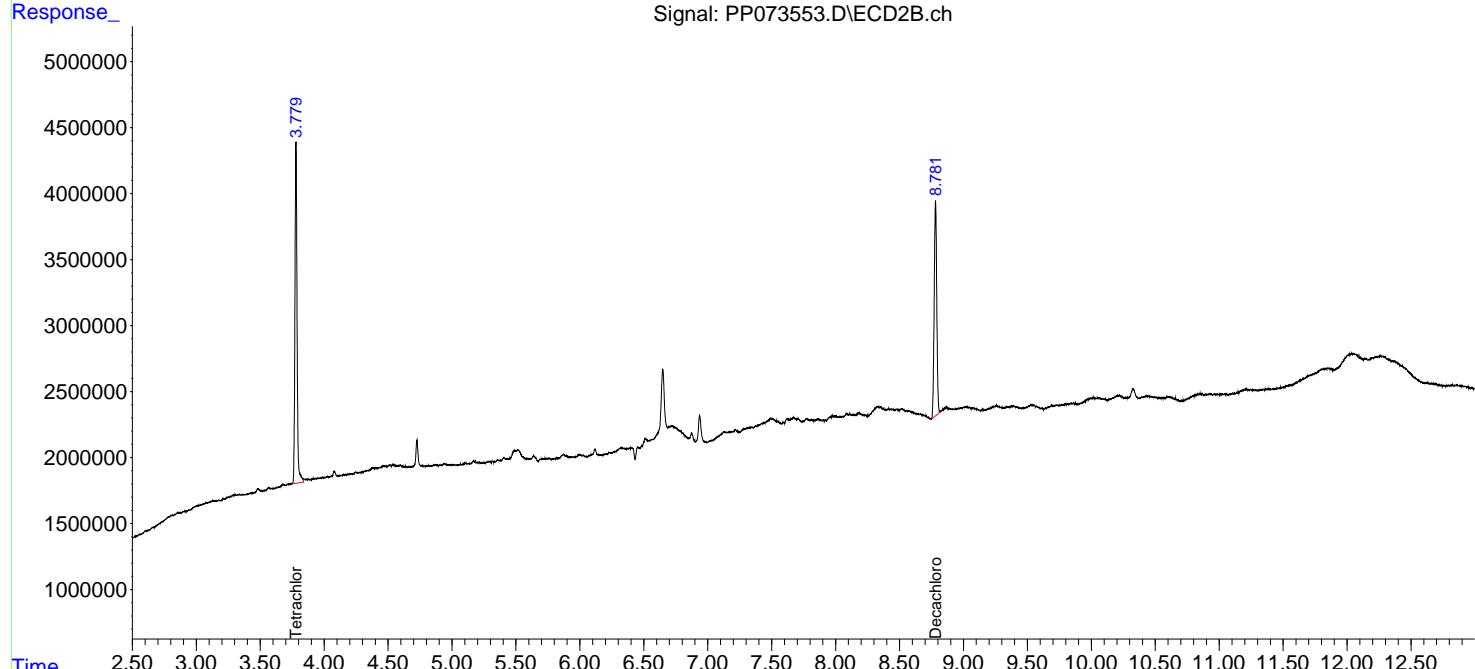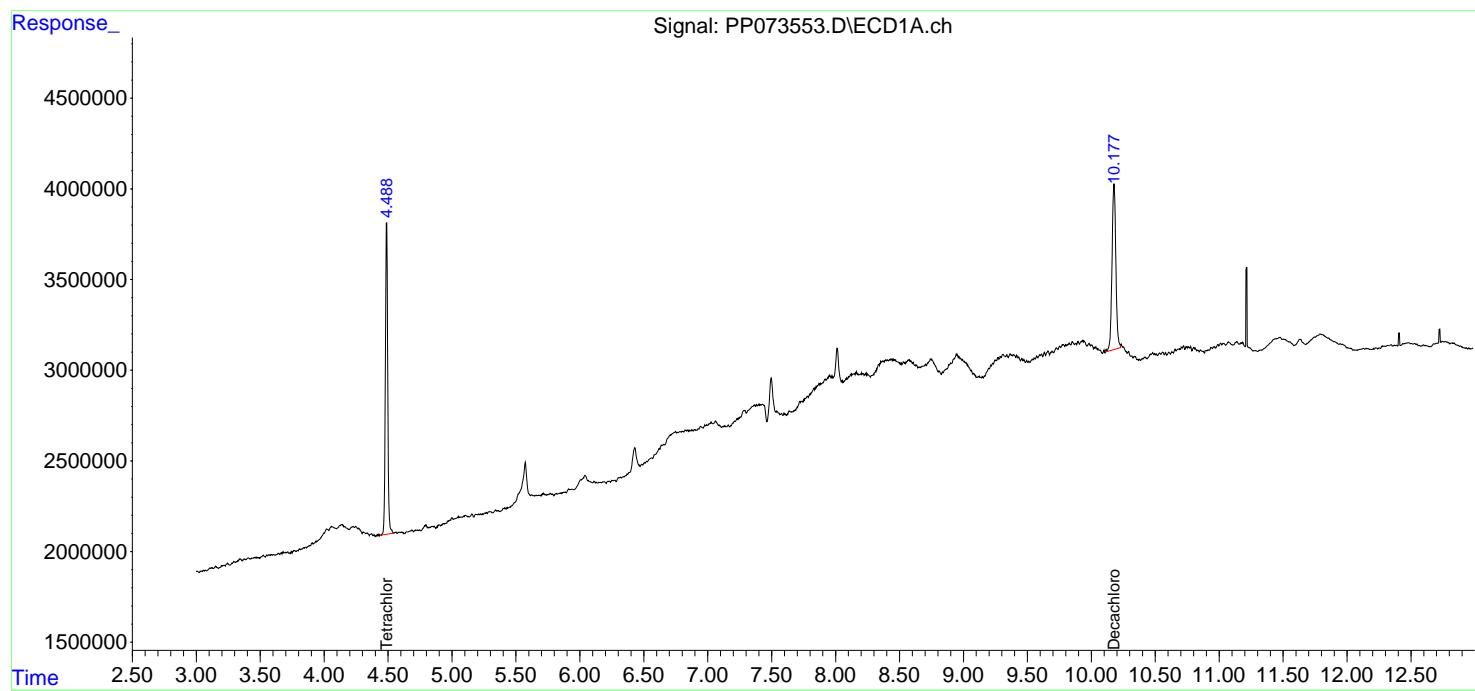

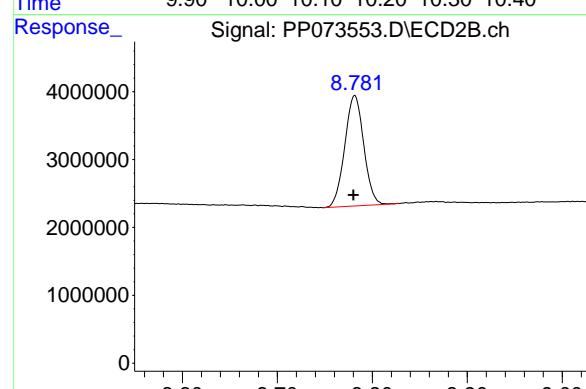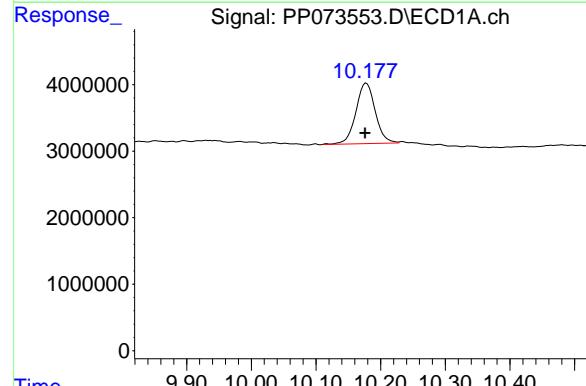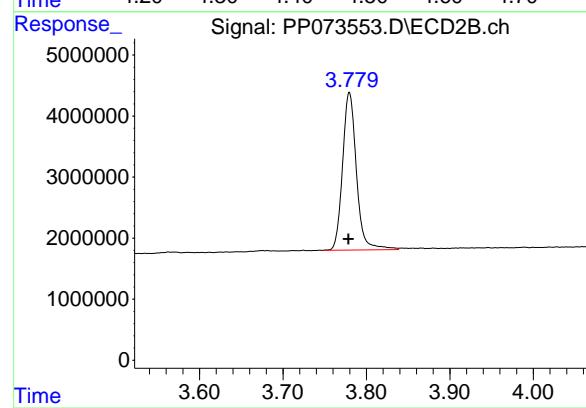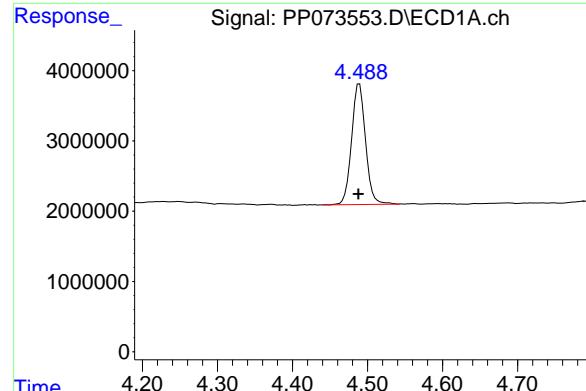

#1 Tetrachloro-m-xylene

R.T.: 4.489 min
 Delta R.T.: 0.001 min
 Response: 22153163
 Conc: 16.18 ng/ml

Instrument:

ECD_P

ClientSampleId :

I.BLK

#1 Tetrachloro-m-xylene

R.T.: 3.780 min
 Delta R.T.: 0.001 min
 Response: 29828480
 Conc: 16.19 ng/ml

#2 Decachlorobiphenyl

R.T.: 10.178 min
 Delta R.T.: 0.002 min
 Response: 18922819
 Conc: 17.34 ng/ml

#2 Decachlorobiphenyl

R.T.: 8.781 min
 Delta R.T.: 0.001 min
 Response: 22582394
 Conc: 17.07 ng/ml



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

Report of Analysis

Client:	Nobis Group			Date Collected:	07/21/25			
Project:	Raymark Superfund Site			Date Received:	07/21/25			
Client Sample ID:	PIBLK-PP073976.D			SDG No.:	Q2639			
Lab Sample ID:	I.BLK-PP073976.D			Matrix:	WATER			
Analytical Method:	8082A			% Solid:	0	Decanted:		
Sample Wt/Vol:	1000	Units:	mL	Final Vol:	10000	uL		
Soil Aliquot Vol:	uL			Test:	PCB			
Extraction Type:				Injection Volume :				
GPC Factor :	1.0	PH :						
Prep Method :	5030							

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PP073976.D	1		07/21/25	pp072125

CAS Number	Parameter	Conc.	Qualifier	MDL	LOD	LOQ / CRQL	Units
TARGETS							
12674-11-2	Aroclor-1016	0.25	U	0.097	0.25	0.50	ug/L
11104-28-2	Aroclor-1221	0.40	U	0.13	0.40	0.50	ug/L
11141-16-5	Aroclor-1232	0.25	U	0.096	0.25	0.50	ug/L
53469-21-9	Aroclor-1242	0.25	U	0.12	0.25	0.50	ug/L
12672-29-6	Aroclor-1248	0.25	U	0.071	0.25	0.50	ug/L
11097-69-1	Aroclor-1254	0.25	U	0.094	0.25	0.50	ug/L
11096-82-5	Aroclor-1260	0.25	U	0.081	0.25	0.50	ug/L
37324-23-5	Aroclor-1262	0.40	U	0.14	0.40	0.50	ug/L
11100-14-4	Aroclor-1268	0.25	U	0.11	0.25	0.50	ug/L
SURROGATES							
877-09-8	Tetrachloro-m-xylene	16.8		60 - 140		84%	SPK: 20
2051-24-3	Decachlorobiphenyl	17.6		60 - 140		88%	SPK: 20

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP072125\
Data File : PP073976.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Jul 2025 09:56
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 22 01:46:14 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070825.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jul 08 08:35:32 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 μ l
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	4.482	3.774	23034074	31045310	16.819	16.851
2) SA Decachlor...	10.167	8.770	19247044	25335367	17.641	19.148

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP072125\
 Data File : PP073976.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jul 2025 09:56
 Operator : YP\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 22 01:46:14 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 08 08:35:32 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ m Signal #2 Info : 30M x 0.32mm x 0.25 μ m

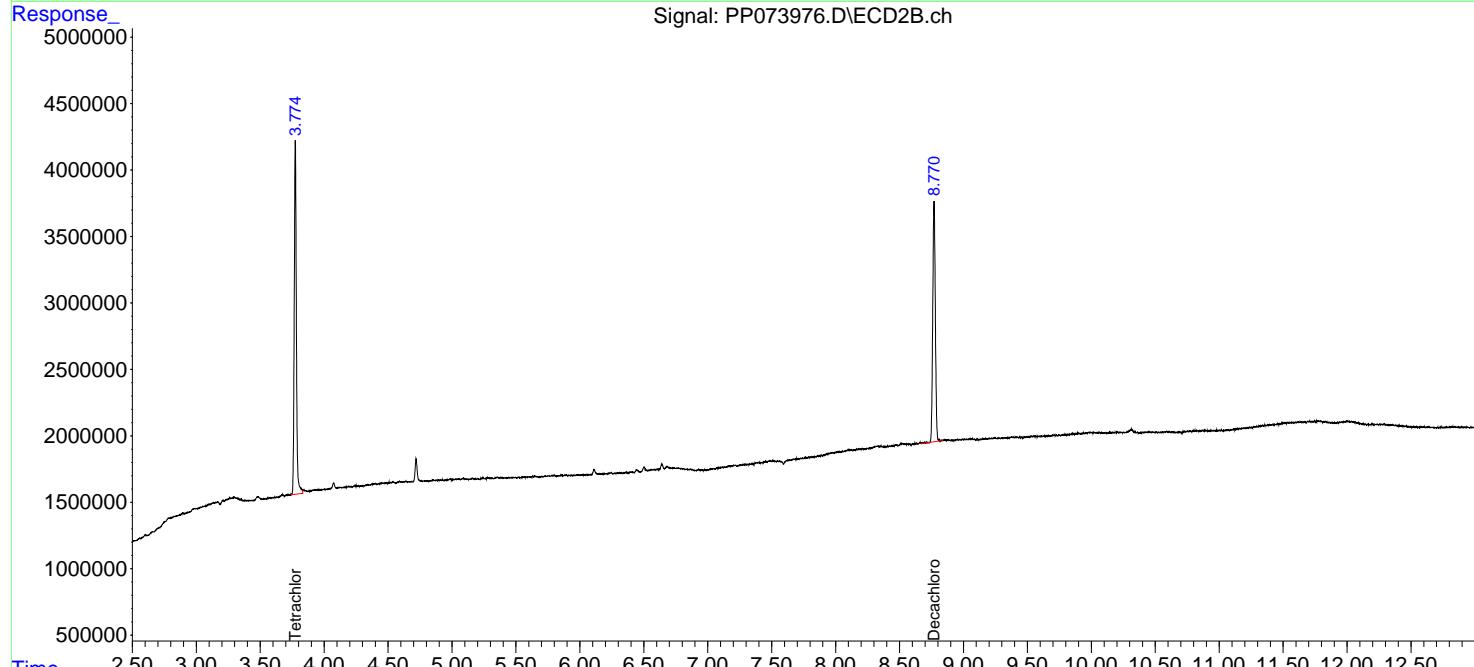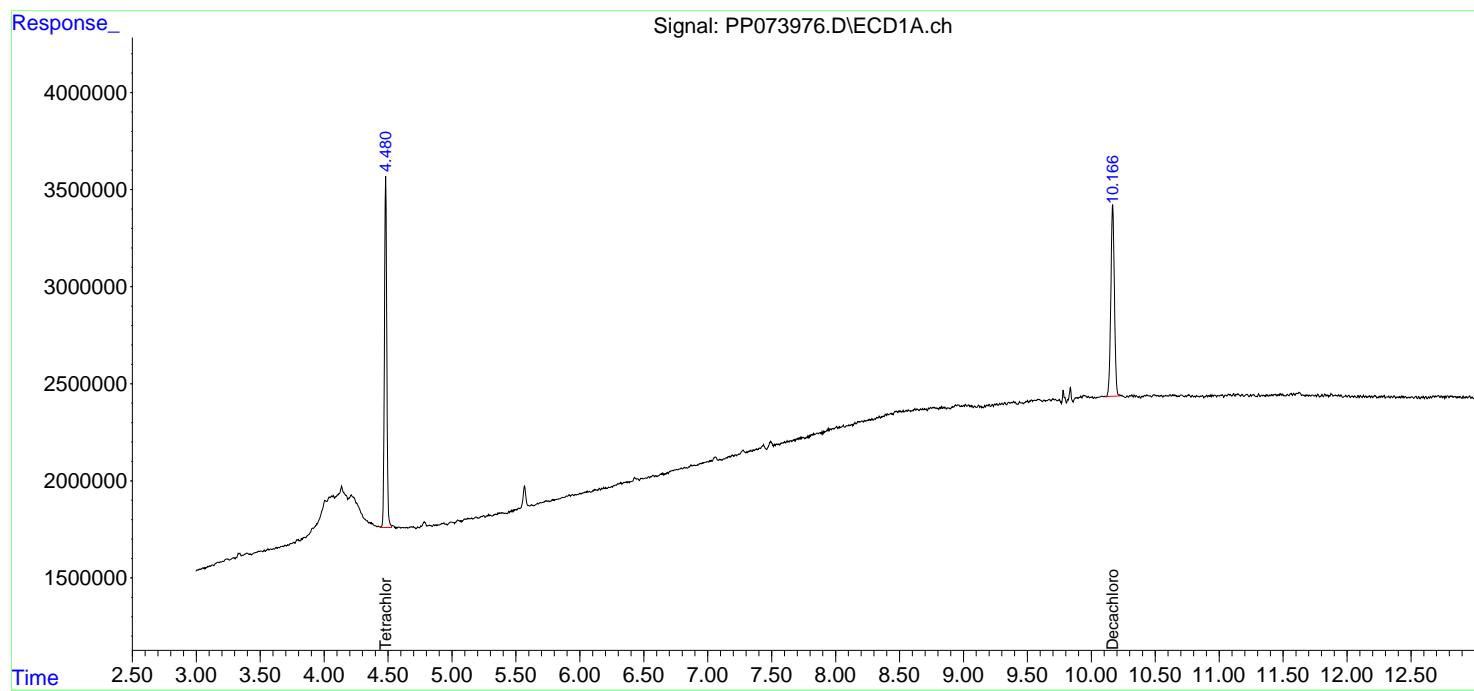

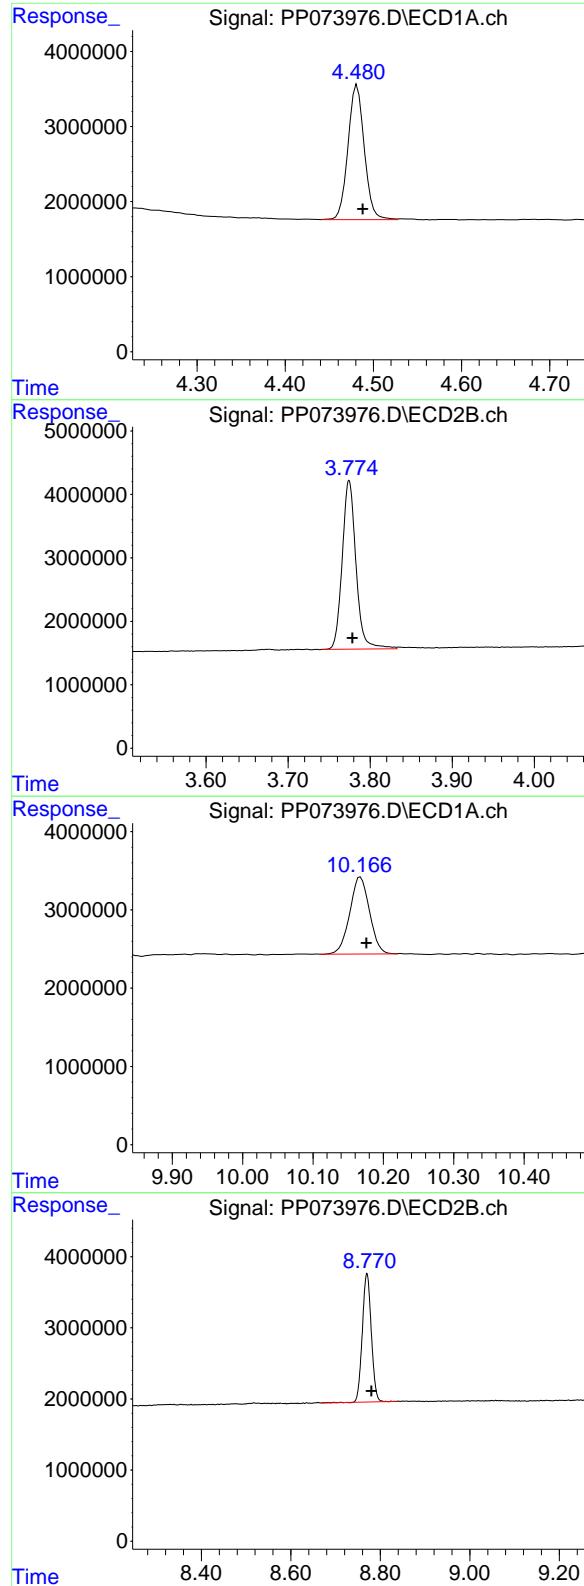

#1 Tetrachloro-m-xylene

R.T.: 4.482 min
Delta R.T.: -0.006 min
Response: 23034074
Conc: 16.82 ng/ml

Instrument : ECD_P

ClientSampleId : I.BLK

#1 Tetrachloro-m-xylene

R.T.: 3.774 min
Delta R.T.: -0.004 min
Response: 31045310
Conc: 16.85 ng/ml

#2 Decachlorobiphenyl

R.T.: 10.167 min
Delta R.T.: -0.009 min
Response: 19247044
Conc: 17.64 ng/ml

#2 Decachlorobiphenyl

R.T.: 8.770 min
Delta R.T.: -0.010 min
Response: 25335367
Conc: 19.15 ng/ml



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

Report of Analysis

Client:	Nobis Group			Date Collected:	07/21/25			
Project:	Raymark Superfund Site			Date Received:	07/21/25			
Client Sample ID:	PIBLK-PP073991.D			SDG No.:	Q2639			
Lab Sample ID:	I.BLK-PP073991.D			Matrix:	WATER			
Analytical Method:	8082A			% Solid:	0	Decanted:		
Sample Wt/Vol:	1000	Units:	mL	Final Vol:	10000	uL		
Soil Aliquot Vol:	uL			Test:	PCB			
Extraction Type:				Injection Volume :				
GPC Factor :	1.0	PH :						
Prep Method :	5030							

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PP073991.D	1		07/21/25	pp072125

CAS Number	Parameter	Conc.	Qualifier	MDL	LOD	LOQ / CRQL	Units
TARGETS							
12674-11-2	Aroclor-1016	0.25	U	0.097	0.25	0.50	ug/L
11104-28-2	Aroclor-1221	0.40	U	0.13	0.40	0.50	ug/L
11141-16-5	Aroclor-1232	0.25	U	0.096	0.25	0.50	ug/L
53469-21-9	Aroclor-1242	0.25	U	0.12	0.25	0.50	ug/L
12672-29-6	Aroclor-1248	0.25	U	0.071	0.25	0.50	ug/L
11097-69-1	Aroclor-1254	0.25	U	0.094	0.25	0.50	ug/L
11096-82-5	Aroclor-1260	0.25	U	0.081	0.25	0.50	ug/L
37324-23-5	Aroclor-1262	0.40	U	0.14	0.40	0.50	ug/L
11100-14-4	Aroclor-1268	0.25	U	0.11	0.25	0.50	ug/L
SURROGATES							
877-09-8	Tetrachloro-m-xylene	15.8		60 - 140		79%	SPK: 20
2051-24-3	Decachlorobiphenyl	16.7		60 - 140		83%	SPK: 20

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP072125\
Data File : PP073991.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Jul 2025 16:23
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 22 01:54:33 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070825.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jul 08 08:35:32 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 μ l
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	4.484	3.774	21712730	32171043	15.854	17.463
2) SA Decachlor...	10.170	8.771	18173509	26037964	16.657	19.679

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP072125\
 Data File : PP073991.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jul 2025 16:23
 Operator : YP\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 22 01:54:33 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 08 08:35:32 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

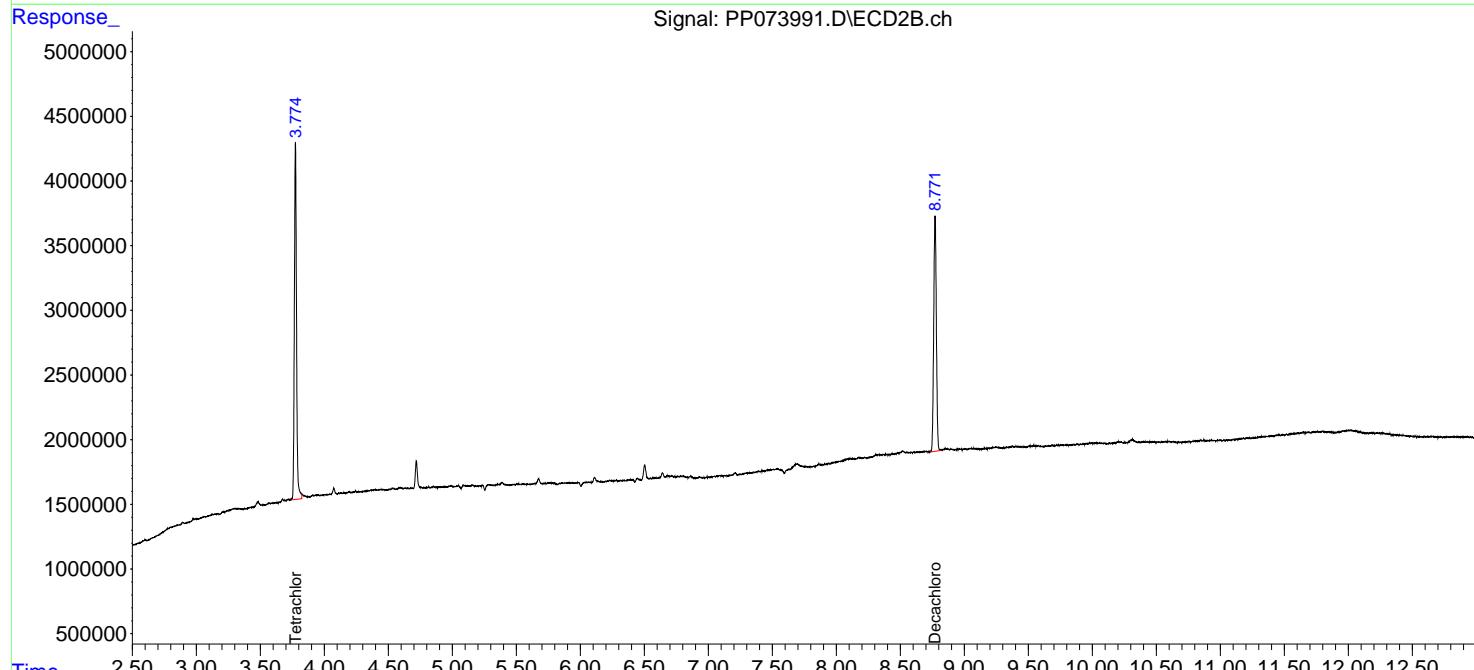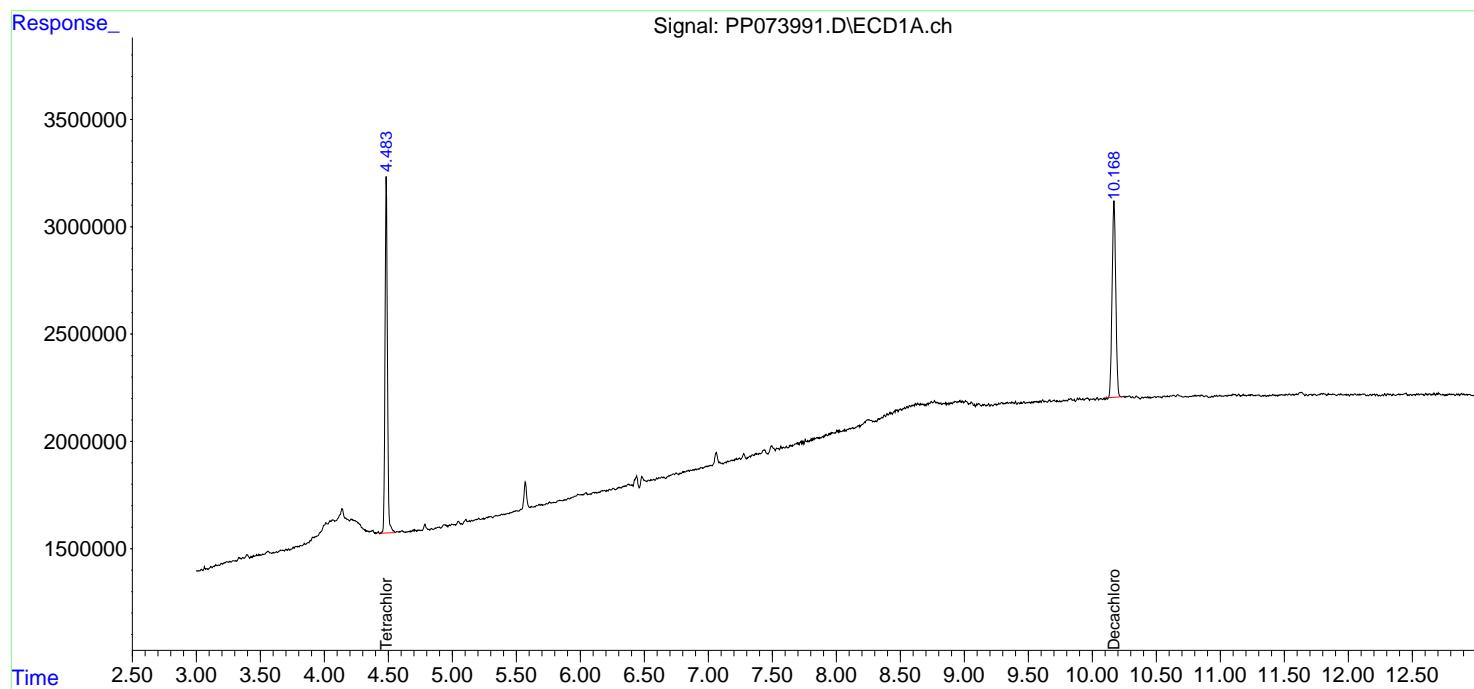

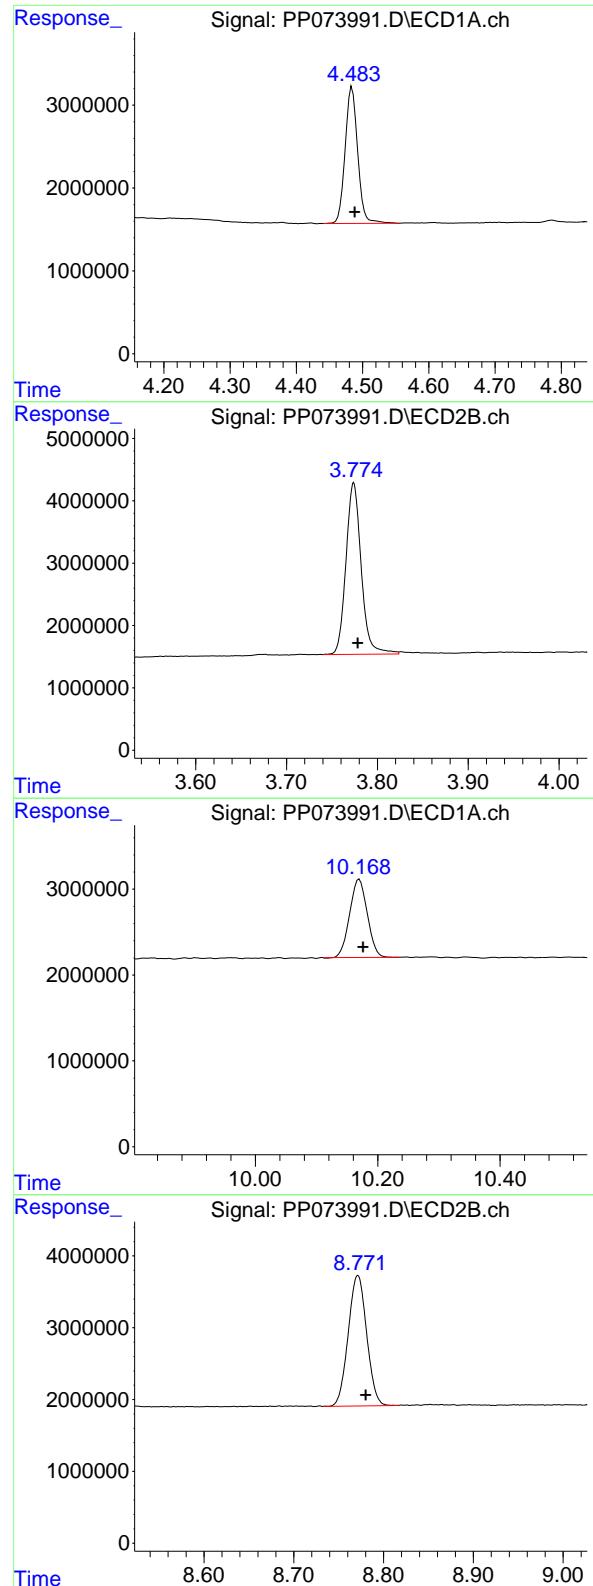

#1 Tetrachloro-m-xylene

R.T.: 4.484 min
 Delta R.T.: -0.004 min
 Response: 21712730
 Conc: 15.85 ng/ml

Instrument:

ECD_P

ClientSampleId:
I.BLK

#1 Tetrachloro-m-xylene

R.T.: 3.774 min
 Delta R.T.: -0.005 min
 Response: 32171043
 Conc: 17.46 ng/ml

#2 Decachlorobiphenyl

R.T.: 10.170 min
 Delta R.T.: -0.006 min
 Response: 18173509
 Conc: 16.66 ng/ml

#2 Decachlorobiphenyl

R.T.: 8.771 min
 Delta R.T.: -0.009 min
 Response: 26037964
 Conc: 19.68 ng/ml



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

Report of Analysis

Client:	Nobis Group			Date Collected:	07/21/25			
Project:	Raymark Superfund Site			Date Received:	07/21/25			
Client Sample ID:	PIBLK-PP074006.D			SDG No.:	Q2639			
Lab Sample ID:	I.BLK-PP074006.D			Matrix:	WATER			
Analytical Method:	8082A			% Solid:	0	Decanted:		
Sample Wt/Vol:	1000	Units:	mL	Final Vol:	10000	uL		
Soil Aliquot Vol:	uL			Test:	PCB			
Extraction Type:				Injection Volume :				
GPC Factor :	1.0	PH :						
Prep Method :	5030							

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PP074006.D	1		07/21/25	pp072125

CAS Number	Parameter	Conc.	Qualifier	MDL	LOD	LOQ / CRQL	Units
TARGETS							
12674-11-2	Aroclor-1016	0.25	U	0.097	0.25	0.50	ug/L
11104-28-2	Aroclor-1221	0.40	U	0.13	0.40	0.50	ug/L
11141-16-5	Aroclor-1232	0.25	U	0.096	0.25	0.50	ug/L
53469-21-9	Aroclor-1242	0.25	U	0.12	0.25	0.50	ug/L
12672-29-6	Aroclor-1248	0.25	U	0.071	0.25	0.50	ug/L
11097-69-1	Aroclor-1254	0.25	U	0.094	0.25	0.50	ug/L
11096-82-5	Aroclor-1260	0.25	U	0.081	0.25	0.50	ug/L
37324-23-5	Aroclor-1262	0.40	U	0.14	0.40	0.50	ug/L
11100-14-4	Aroclor-1268	0.25	U	0.11	0.25	0.50	ug/L
SURROGATES							
877-09-8	Tetrachloro-m-xylene	15.8		60 - 140		79%	SPK: 20
2051-24-3	Decachlorobiphenyl	17.1		60 - 140		85%	SPK: 20

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP072125\
 Data File : PP074006.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jul 2025 21:34
 Operator : YP\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 22 02:17:05 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 08 08:35:32 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	4.479	3.773	21664756	32074283	15.819	17.410
2) SA Decachlor...	10.164	8.769	18614863	25580988	17.061	19.333

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP072125\
 Data File : PP074006.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jul 2025 21:34
 Operator : YP\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 22 02:17:05 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 08 08:35:32 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ m Signal #2 Info : 30M x 0.32mm x 0.25 μ m

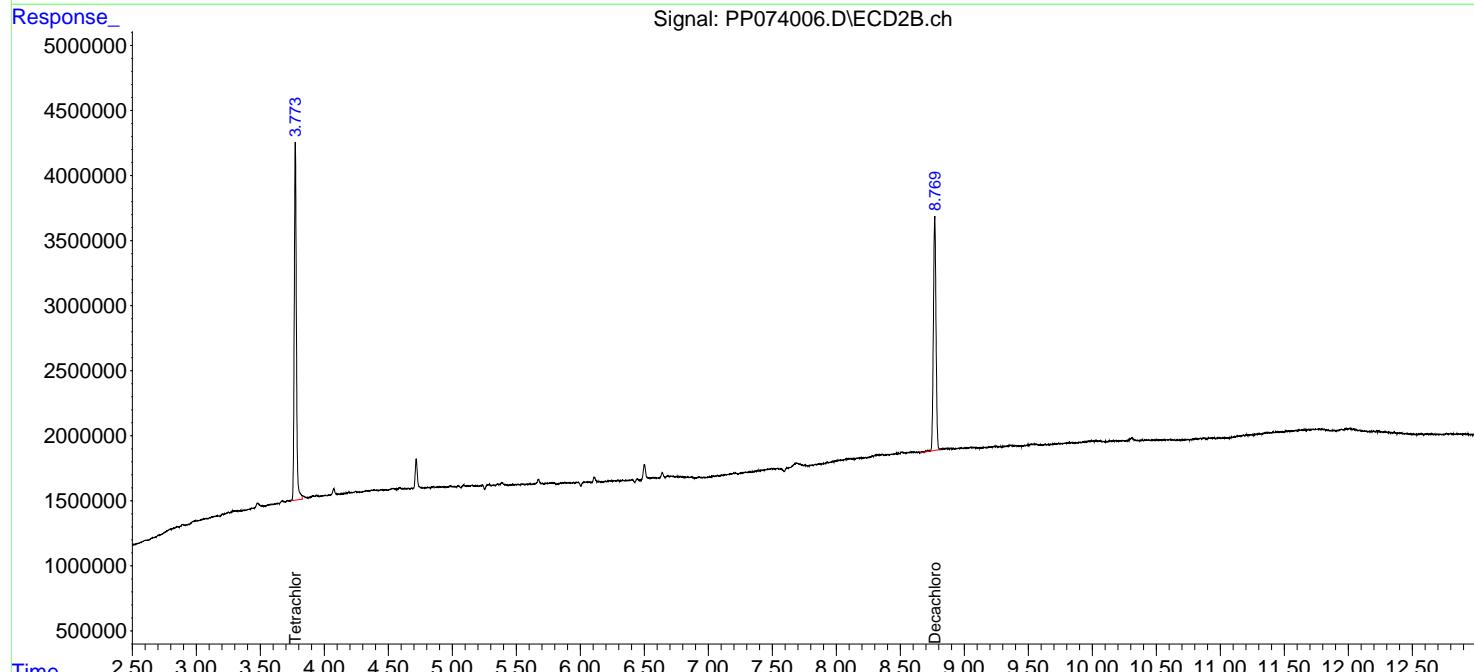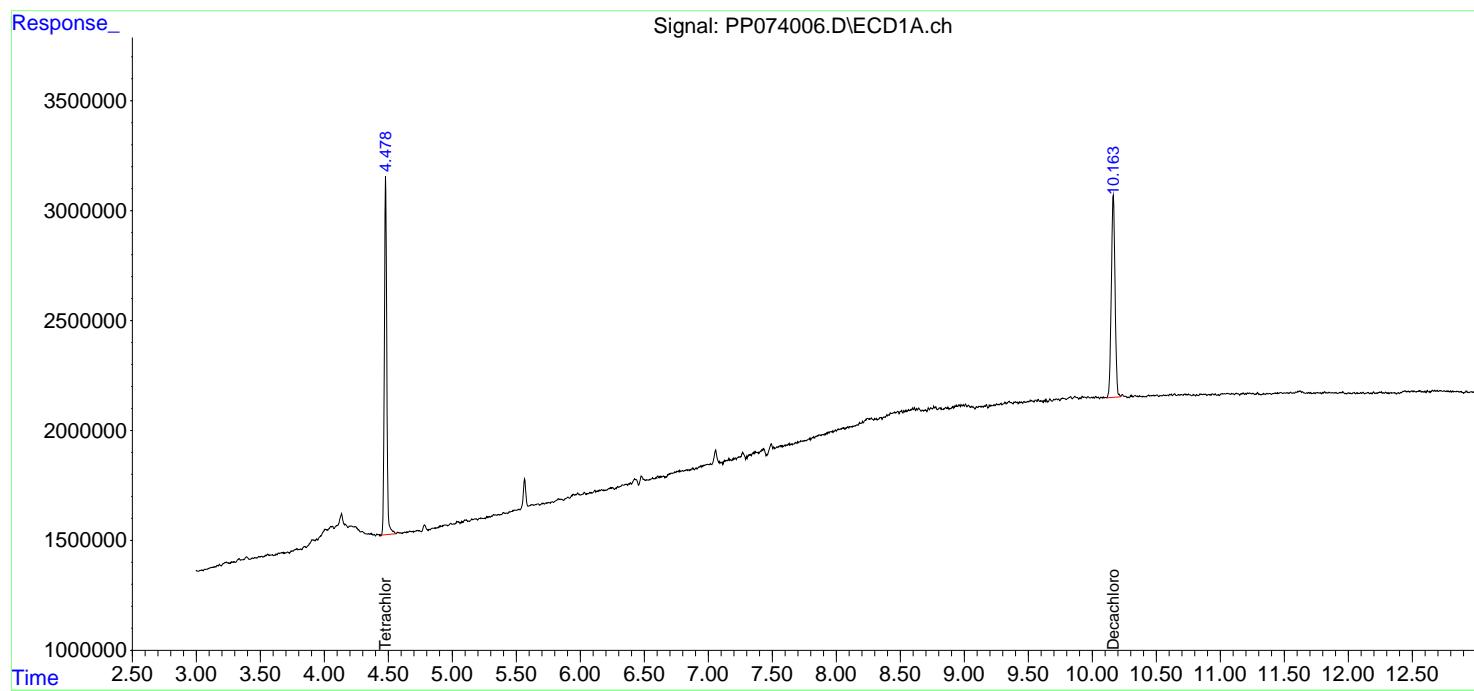


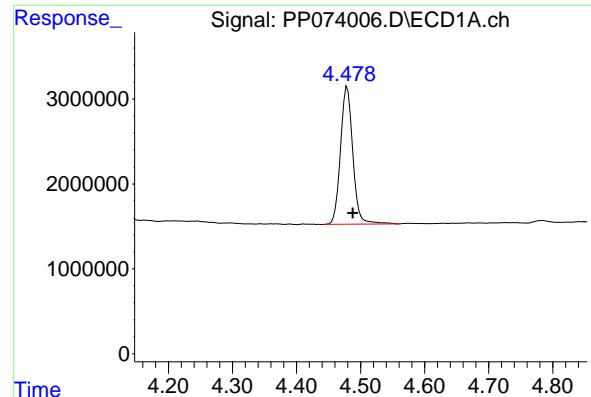

#1 Tetrachloro-m-xylene


R.T.: 4.479 min
Delta R.T.: -0.009 min
Response: 21664756
Conc: 15.82 ng/ml

Instrument: ECD_P
ClientSampleId: I.BLK

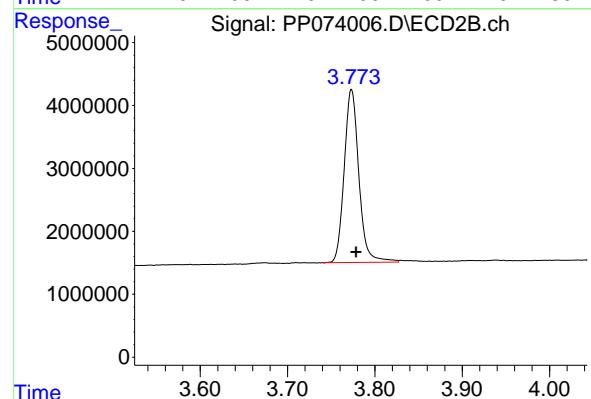


#1 Tetrachloro-m-xylene

R.T.: 3.773 min
Delta R.T.: -0.005 min
Response: 32074283
Conc: 17.41 ng/ml

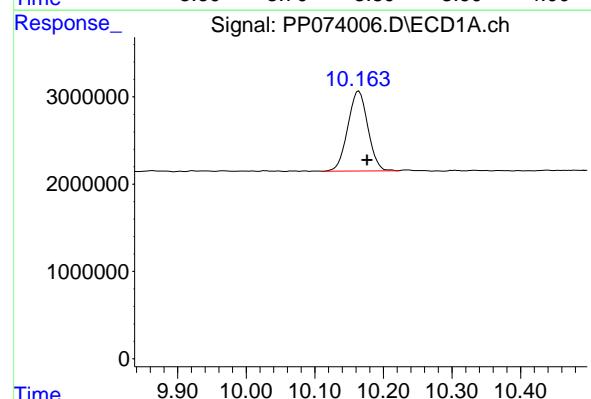

#2 Decachlorobiphenyl

R.T.: 10.164 min
Delta R.T.: -0.012 min
Response: 18614863
Conc: 17.06 ng/ml

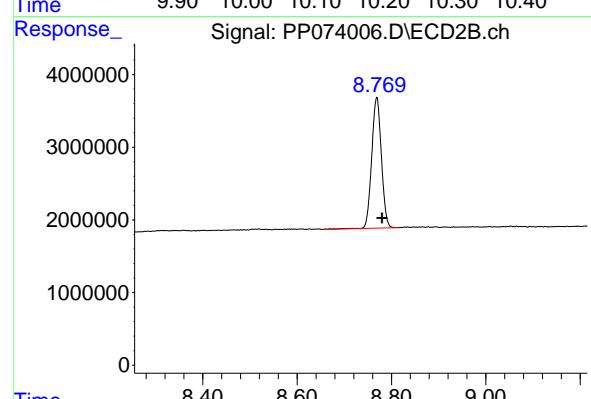

#2 Decachlorobiphenyl

R.T.: 8.769 min
Delta R.T.: -0.011 min
Response: 25580988
Conc: 19.33 ng/ml



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

Report of Analysis

Client:	Nobis Group			Date Collected:	
Project:	Raymark Superfund Site			Date Received:	
Client Sample ID:	PB168927BS			SDG No.:	Q2639
Lab Sample ID:	PB168927BS			Matrix:	SOIL
Analytical Method:	8082A			% Solid:	100 Decanted:
Sample Wt/Vol:	30.01	Units:	g	Final Vol:	10000 uL
Soil Aliquot Vol:			uL	Test:	PCB
Extraction Type:				Injection Volume :	
GPC Factor :	1.0	PH :			
Prep Method :	SW3541B				

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PP073993.D	1	07/21/25 08:30	07/21/25 16:56	PB168927

CAS Number	Parameter	Conc.	Qualifier	MDL	LOD	LOQ / CRQL	Units(Dry Weight)
TARGETS							
12674-11-2	Aroclor-1016	153		3.90	8.30	17.0	ug/kg
11104-28-2	Aroclor-1221	13.0	U	4.00	13.0	17.0	ug/kg
11141-16-5	Aroclor-1232	8.30	U	3.70	8.30	17.0	ug/kg
53469-21-9	Aroclor-1242	8.30	U	4.00	8.30	17.0	ug/kg
12672-29-6	Aroclor-1248	13.0	U	5.90	13.0	17.0	ug/kg
11097-69-1	Aroclor-1254	8.30	U	3.20	8.30	17.0	ug/kg
37324-23-5	Aroclor-1262	13.0	U	5.00	13.0	17.0	ug/kg
11100-14-4	Aroclor-1268	8.30	U	3.60	8.30	17.0	ug/kg
11096-82-5	Aroclor-1260	154		3.20	8.30	17.0	ug/kg
SURROGATES							
877-09-8	Tetrachloro-m-xylene	19.3		44 - 130		96%	SPK: 20
2051-24-3	Decachlorobiphenyl	23.9		60 - 125		120%	SPK: 20

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP072125\
 Data File : PP073993.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jul 2025 16:56
 Operator : YP\AJ
 Sample : PB168927BS
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
PB168927BS

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 22 02:12:41 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 08 08:35:32 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	4.485	3.775	25710118	35503610	18.773	19.271
2) SA Decachlor...	10.170	8.772	22397635	31653782	20.528	23.923

Target Compounds

3) L1 AR-1016-1	5.637	4.852	18648947	30859437	392.497	452.652
4) L1 AR-1016-2	5.658	4.870	30337806	46806903	426.004	459.412
5) L1 AR-1016-3	5.720	5.047	18341794	25209696	420.076	465.929
6) L1 AR-1016-4	5.817	5.089	15197443	20133996	422.790	458.833
7) L1 AR-1016-5	6.109	5.301	13328312	25250923	425.411	462.619
31) L7 AR-1260-1	7.226	6.330	25980515	46681069	440.637	478.484
32) L7 AR-1260-2	7.479	6.519	37795564	58282520	394.362	474.468
33) L7 AR-1260-3	7.837	6.671	27297740	52505882	373.580	479.664 #
34) L7 AR-1260-4	8.060	7.139	26969847	39497845	413.015	441.769
35) L7 AR-1260-5	8.378	7.383	60726734	97958387	402.556	435.881



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.





Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP072125\
 Data File : PP073993.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jul 2025 16:56
 Operator : YP\AJ
 Sample : PB168927BS
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 PB168927BS

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 22 02:12:41 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 08 08:35:32 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

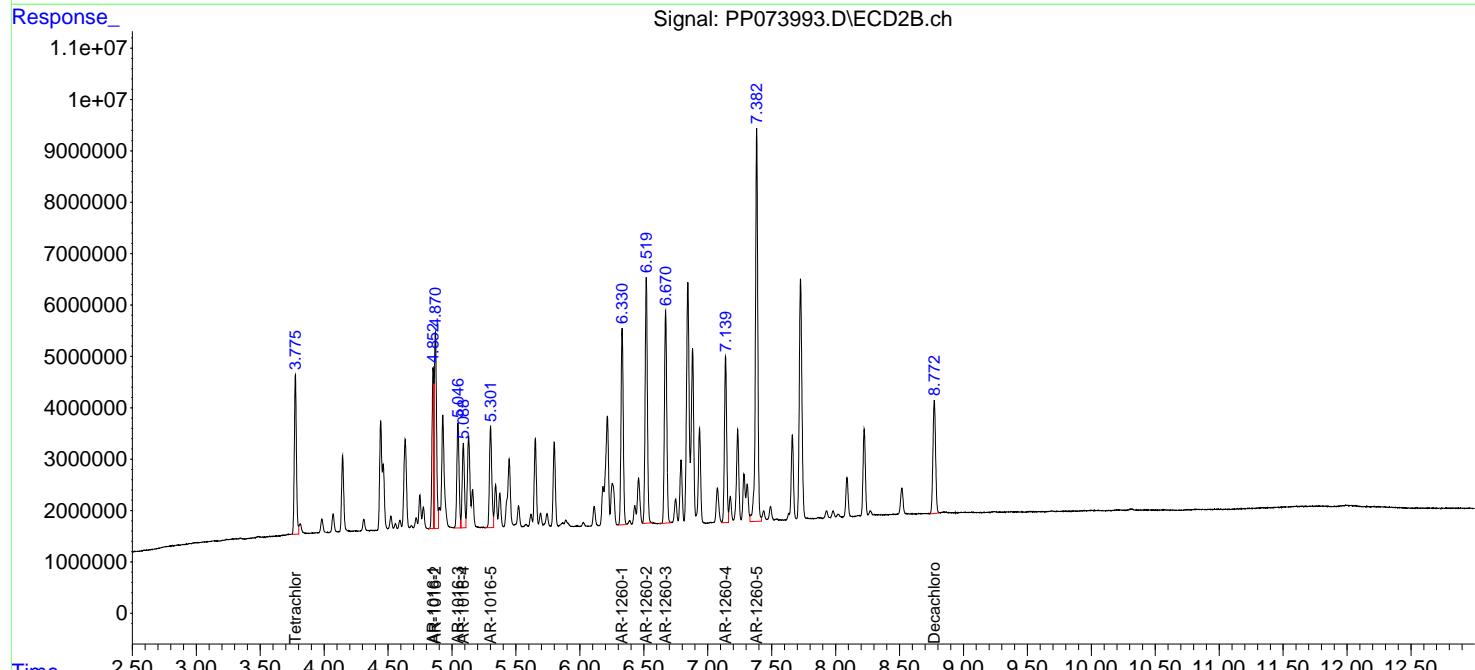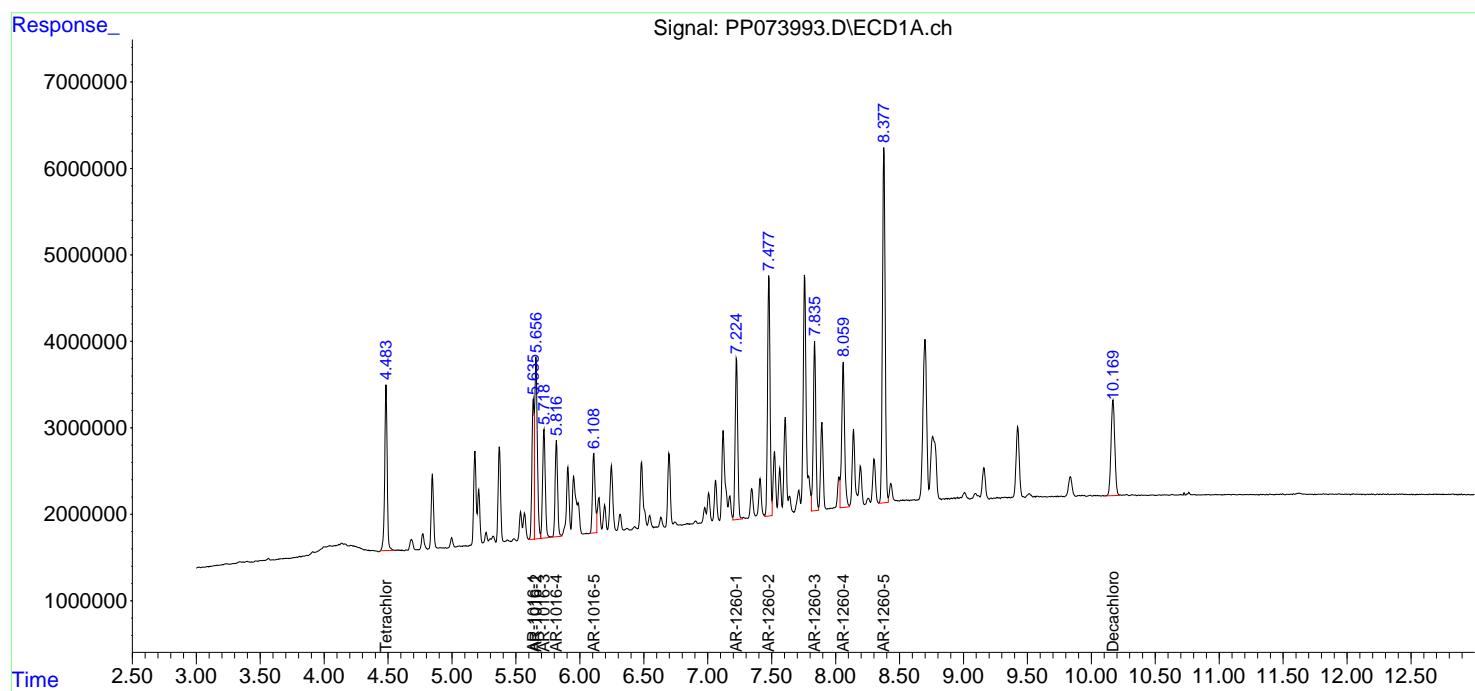

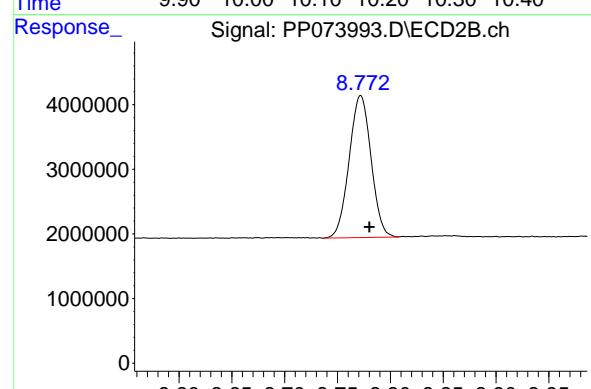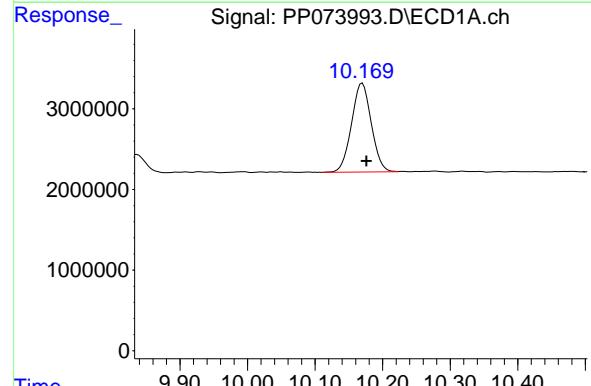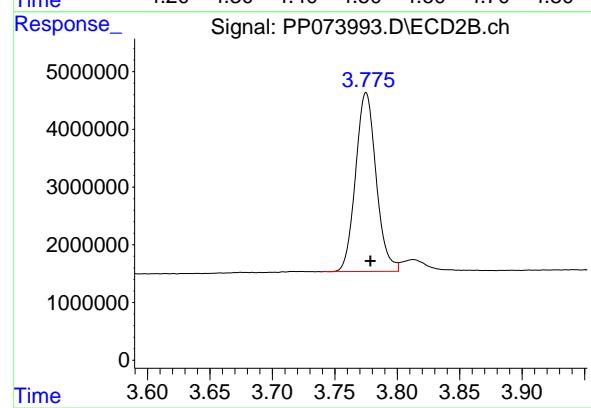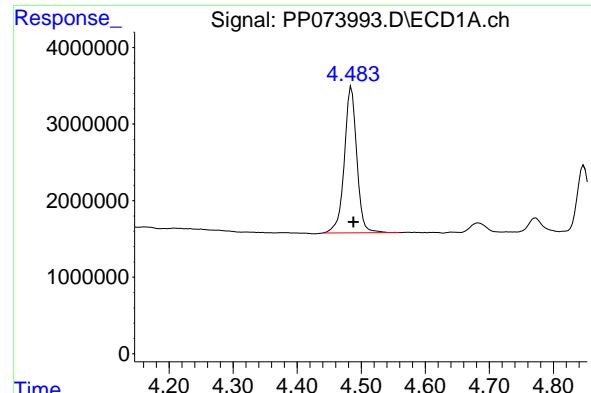

#1 Tetrachloro-m-xylene

R.T.: 4.485 min
 Delta R.T.: -0.003 min
 Response: 25710118
 Conc: 18.77 ng/ml

Instrument: ECD_P
 ClientSampleId: PB168927BS

#1 Tetrachloro-m-xylene


R.T.: 3.775 min
 Delta R.T.: -0.003 min
 Response: 35503610
 Conc: 19.27 ng/ml

#2 Decachlorobiphenyl

R.T.: 10.170 min
 Delta R.T.: -0.006 min
 Response: 22397635
 Conc: 20.53 ng/ml

#2 Decachlorobiphenyl

R.T.: 8.772 min
 Delta R.T.: -0.008 min
 Response: 31653782
 Conc: 23.92 ng/ml

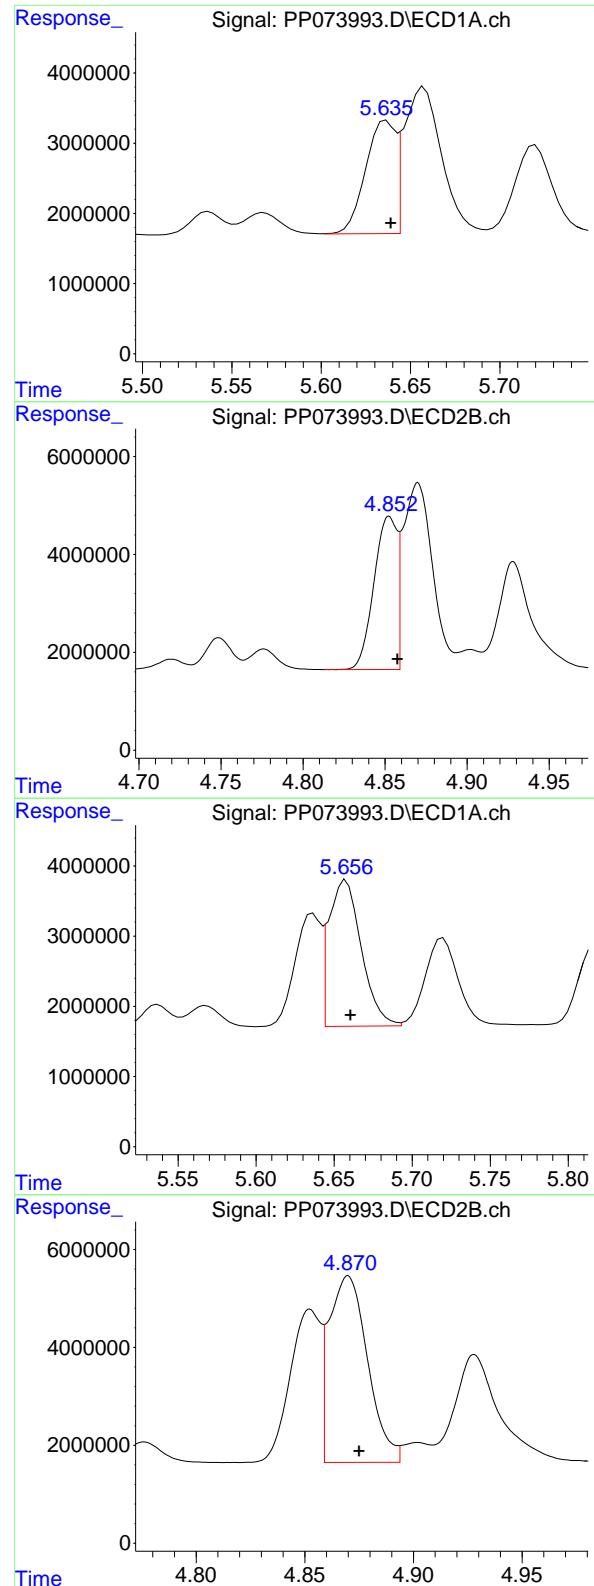

#3 AR-1016-1

R.T.: 5.637 min
 Delta R.T.: -0.002 min
 Response: 18648947
 Conc: 392.50 ng/ml

Instrument: ECD_P
 ClientSampleId: PB168927BS

#3 AR-1016-1


R.T.: 4.852 min
 Delta R.T.: -0.005 min
 Response: 30859437
 Conc: 452.65 ng/ml

#4 AR-1016-2

R.T.: 5.658 min
 Delta R.T.: -0.003 min
 Response: 30337806
 Conc: 426.00 ng/ml

#4 AR-1016-2

R.T.: 4.870 min
 Delta R.T.: -0.005 min
 Response: 46806903
 Conc: 459.41 ng/ml

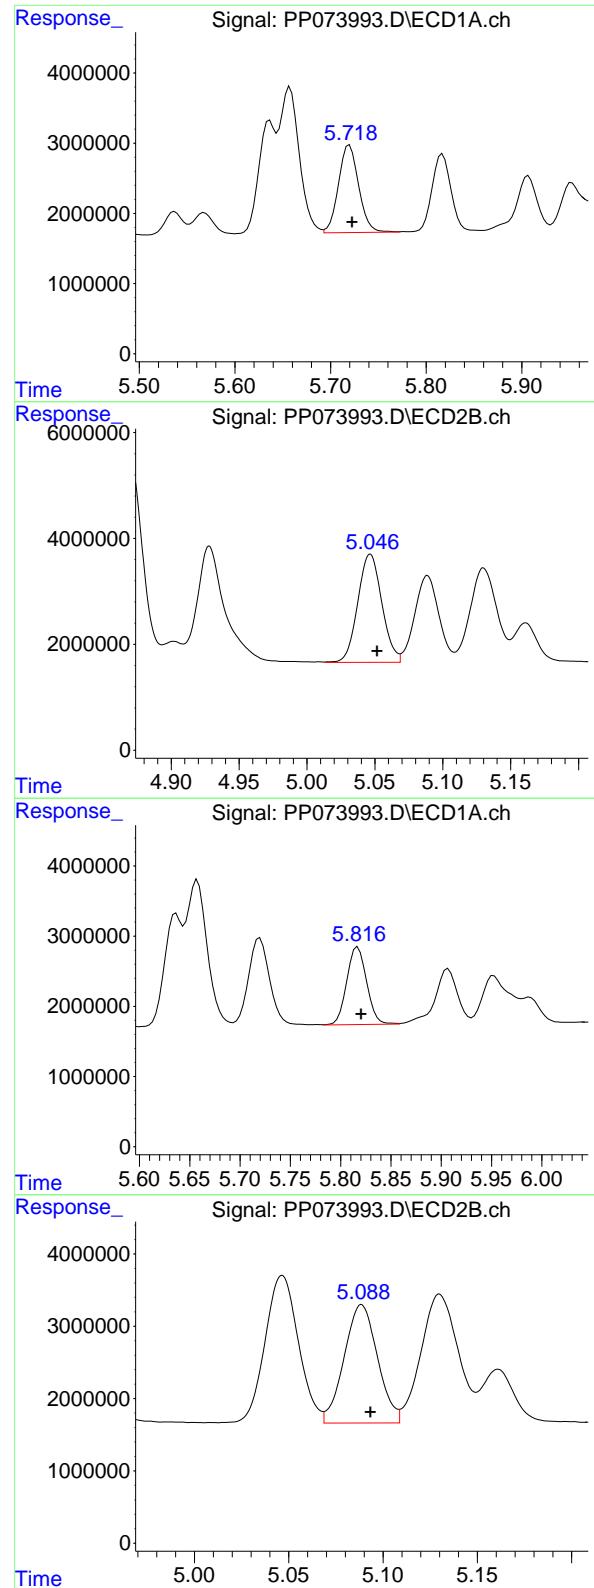

#5 AR-1016-3

R.T.: 5.720 min
 Delta R.T.: -0.003 min
 Response: 18341794
 Conc: 420.08 ng/ml

Instrument: ECD_P
 ClientSampleId: PB168927BS

#5 AR-1016-3





R.T.: 5.047 min
 Delta R.T.: -0.005 min
 Response: 25209696
 Conc: 465.93 ng/ml

#6 AR-1016-4

R.T.: 5.817 min
 Delta R.T.: -0.003 min
 Response: 15197443
 Conc: 422.79 ng/ml

#6 AR-1016-4

R.T.: 5.089 min
 Delta R.T.: -0.005 min
 Response: 20133996
 Conc: 458.83 ng/ml

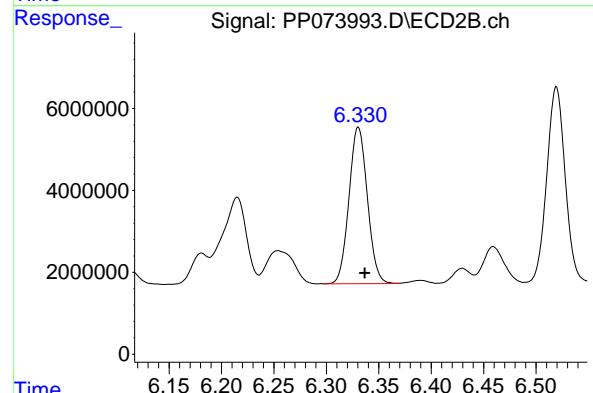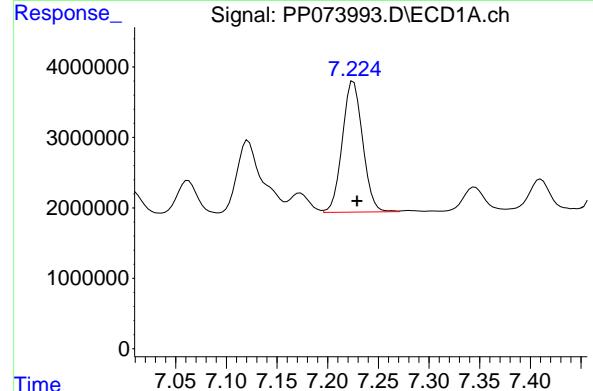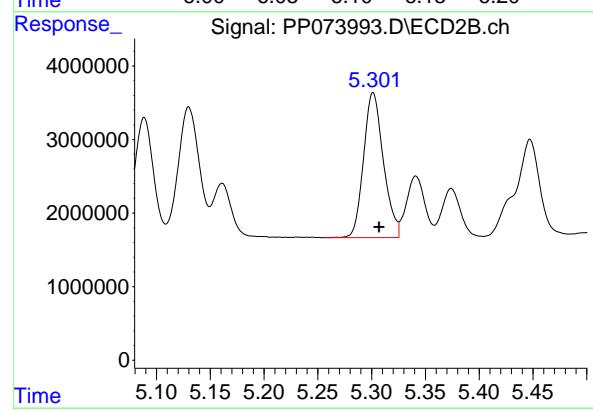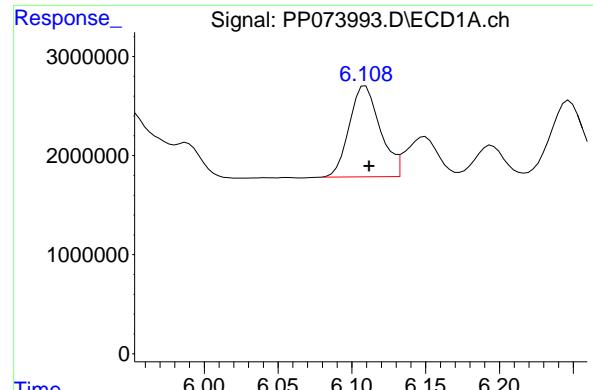

#7 AR-1016-5

R.T.: 6.109 min
 Delta R.T.: -0.003 min
 Response: 13328312
 Conc: 425.41 ng/ml

Instrument: ECD_P
 ClientSampleId: PB168927BS

#7 AR-1016-5


R.T.: 5.301 min
 Delta R.T.: -0.006 min
 Response: 25250923
 Conc: 462.62 ng/ml

#31 AR-1260-1

R.T.: 7.226 min
 Delta R.T.: -0.004 min
 Response: 25980515
 Conc: 440.64 ng/ml

#31 AR-1260-1

R.T.: 6.330 min
 Delta R.T.: -0.006 min
 Response: 46681069
 Conc: 478.48 ng/ml

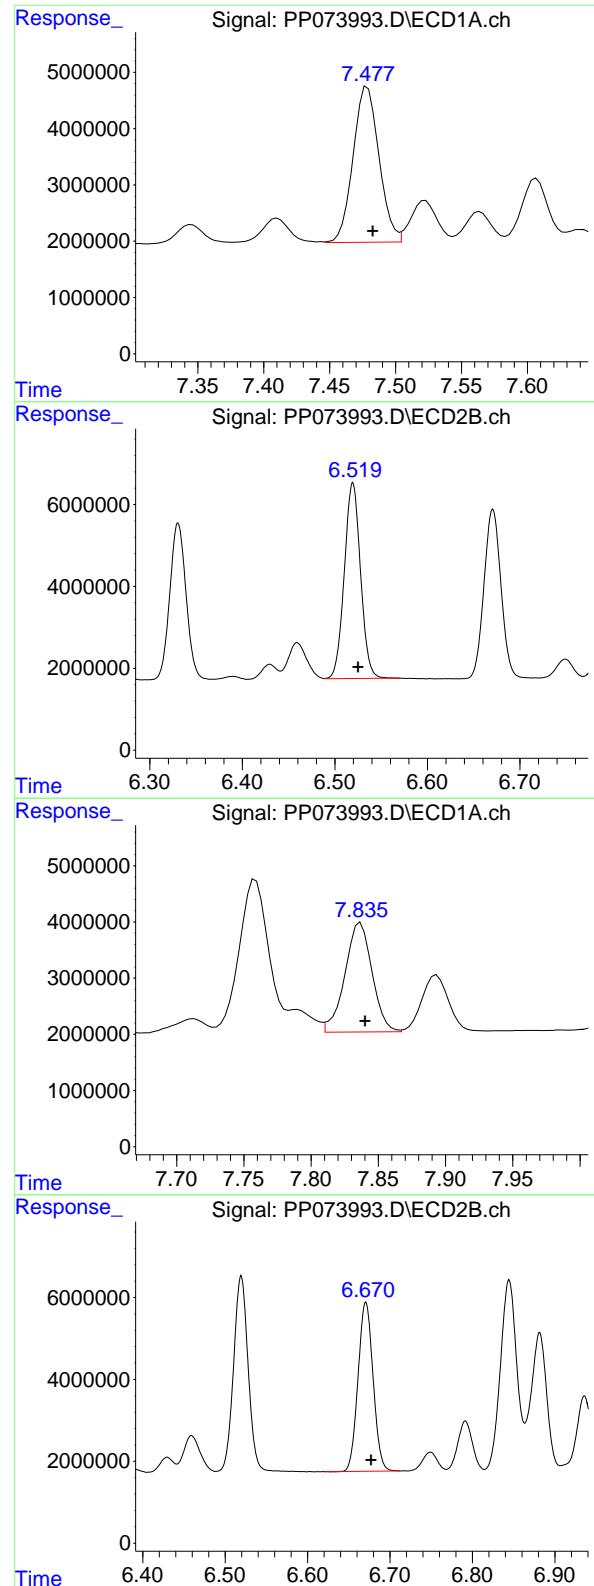

#32 AR-1260-2

R.T.: 7.479 min
 Delta R.T.: -0.004 min
 Response: 37795564
 Conc: 394.36 ng/ml

Instrument: ECD_P
 ClientSampleId: PB168927BS

#32 AR-1260-2


R.T.: 6.519 min
 Delta R.T.: -0.006 min
 Response: 58282520
 Conc: 474.47 ng/ml

#33 AR-1260-3

R.T.: 7.837 min
 Delta R.T.: -0.004 min
 Response: 27297740
 Conc: 373.58 ng/ml

#33 AR-1260-3

R.T.: 6.671 min
 Delta R.T.: -0.006 min
 Response: 52505882
 Conc: 479.66 ng/ml

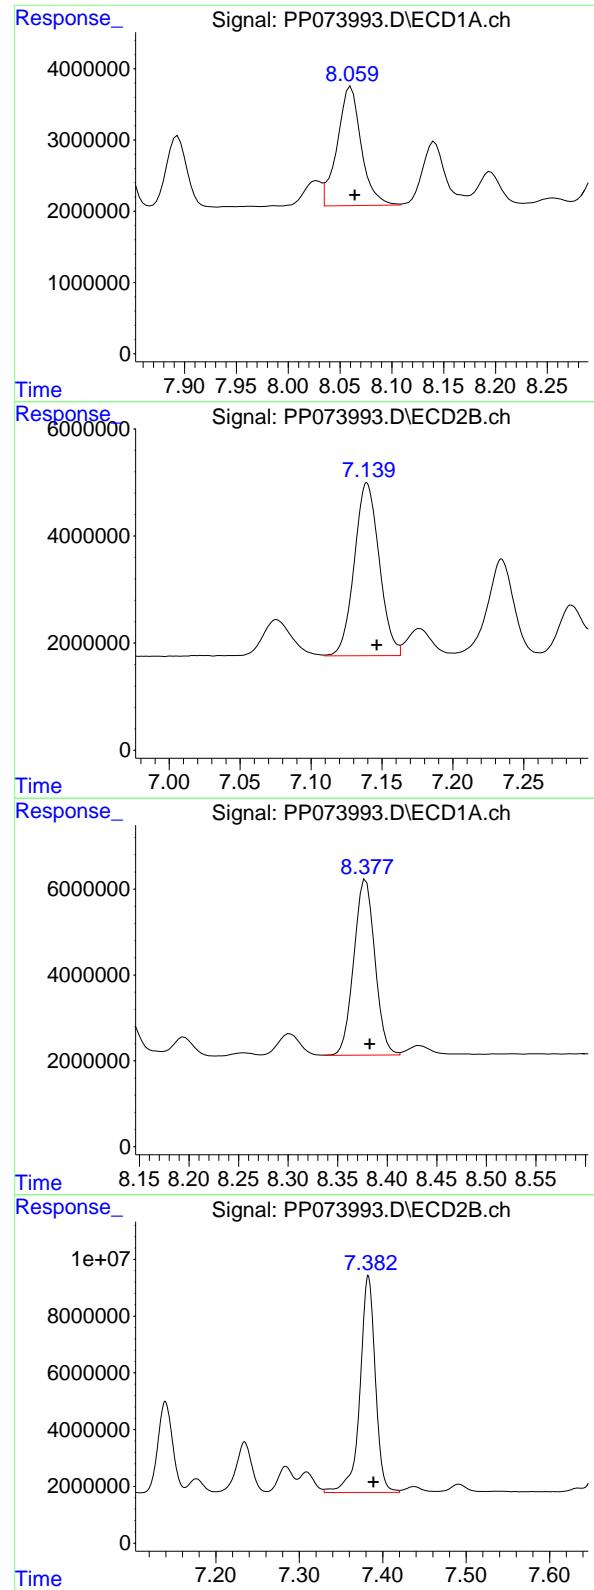

#34 AR-1260-4

R.T.: 8.060 min
 Delta R.T.: -0.004 min
 Response: 26969847
 Conc: 413.02 ng/ml

Instrument: ECD_P
 ClientSampleId: PB168927BS

#34 AR-1260-4

R.T.: 7.139 min
 Delta R.T.: -0.007 min
 Response: 39497845
 Conc: 441.77 ng/ml

#35 AR-1260-5

R.T.: 8.378 min
 Delta R.T.: -0.004 min
 Response: 60726734
 Conc: 402.56 ng/ml

#35 AR-1260-5

R.T.: 7.383 min
 Delta R.T.: -0.006 min
 Response: 97958387
 Conc: 435.88 ng/ml



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

Report of Analysis

Client:	Nobis Group			Date Collected:	07/17/25	
Project:	Raymark Superfund Site			Date Received:	07/17/25	
Client Sample ID:	RT2286MS			SDG No.:	Q2639	
Lab Sample ID:	Q2635-01MS			Matrix:	SOIL	
Analytical Method:	8082A			% Solid:	84.8	Decanted:
Sample Wt/Vol:	30.05	Units:	g	Final Vol:	10000	uL
Soil Aliquot Vol:	uL			Test:	PCB	
Extraction Type:				Injection Volume :		
GPC Factor :	1.0	PH :				
Prep Method :	SW3541B					

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PP073984.D	1	07/21/25 08:30	07/21/25 13:40	PB168927

CAS Number	Parameter	Conc.	Qualifier	MDL	LOD	LOQ / CRQL	Units(Dry Weight)
TARGETS							
12674-11-2	Aroclor-1016	177		4.70	9.80	20.0	ug/kg
11104-28-2	Aroclor-1221	15.3	U	4.70	15.3	20.0	ug/kg
11141-16-5	Aroclor-1232	9.80	U	4.40	9.80	20.0	ug/kg
53469-21-9	Aroclor-1242	9.80	U	4.70	9.80	20.0	ug/kg
12672-29-6	Aroclor-1248	15.3	U	7.00	15.3	20.0	ug/kg
11097-69-1	Aroclor-1254	9.80	U	3.80	9.80	20.0	ug/kg
37324-23-5	Aroclor-1262	15.3	U	5.90	15.3	20.0	ug/kg
11100-14-4	Aroclor-1268	9.80	U	4.20	9.80	20.0	ug/kg
11096-82-5	Aroclor-1260	214		3.80	9.80	20.0	ug/kg
SURROGATES							
877-09-8	Tetrachloro-m-xylene	17.9		44 - 130		89%	SPK: 20
2051-24-3	Decachlorobiphenyl	19.9		60 - 125		99%	SPK: 20

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP072125\
 Data File : PP073984.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jul 2025 13:40
 Operator : YP\AJ
 Sample : Q2635-01MS
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 RT2286MS

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/22/2025
 Supervised By :mohammad ahmed 07/23/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 22 01:50:37 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 08 08:35:32 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	4.480	3.773	22954565	32913477	16.761m	17.866
2) SA Decachlor...	10.168	8.770	19654459	26316757	18.014	19.889

Target Compounds

3) L1 AR-1016-1	5.633	4.849	18863800	29465448	397.019	432.205
4) L1 AR-1016-2	5.654	4.867	29837172	43500761	418.974	426.962
5) L1 AR-1016-3	5.716	5.043	18207530	24326097	417.001	449.598
6) L1 AR-1016-4	5.813	5.085	16224197	19663890	451.354	448.120
7) L1 AR-1016-5	6.107	5.298	17720270	24867794	565.593	455.600
31) L7 AR-1260-1	7.222	6.328	34694505	55075376	588.429	564.527
32) L7 AR-1260-2	7.476	6.517	49718794	66621540	518.769	542.355
33) L7 AR-1260-3	7.834	6.668	37706644	60304176	516.030	550.905
34) L7 AR-1260-4	8.058	7.137	36868595	47082456	564.604	526.600
35) L7 AR-1260-5	8.375	7.380	80346257	117.2E6	532.614	521.396

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP072125\
 Data File : PP073984.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jul 2025 13:40
 Operator : YP\AJ
 Sample : Q2635-01MS
 Misc :
 ALS Vial : 14 Sample Multiplier: 1



Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 22 01:50:37 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 08 08:35:32 2025
 Response via : Initial Calibration
 Integrator: ChemStation


Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Instrument :
 ECD_P
 ClientSampleId :
 RT2286MS

Manual Integrations APPROVED

Reviewed By :Yogesh Patel 07/22/2025
 Supervised By :mohammad ahmed 07/23/2025

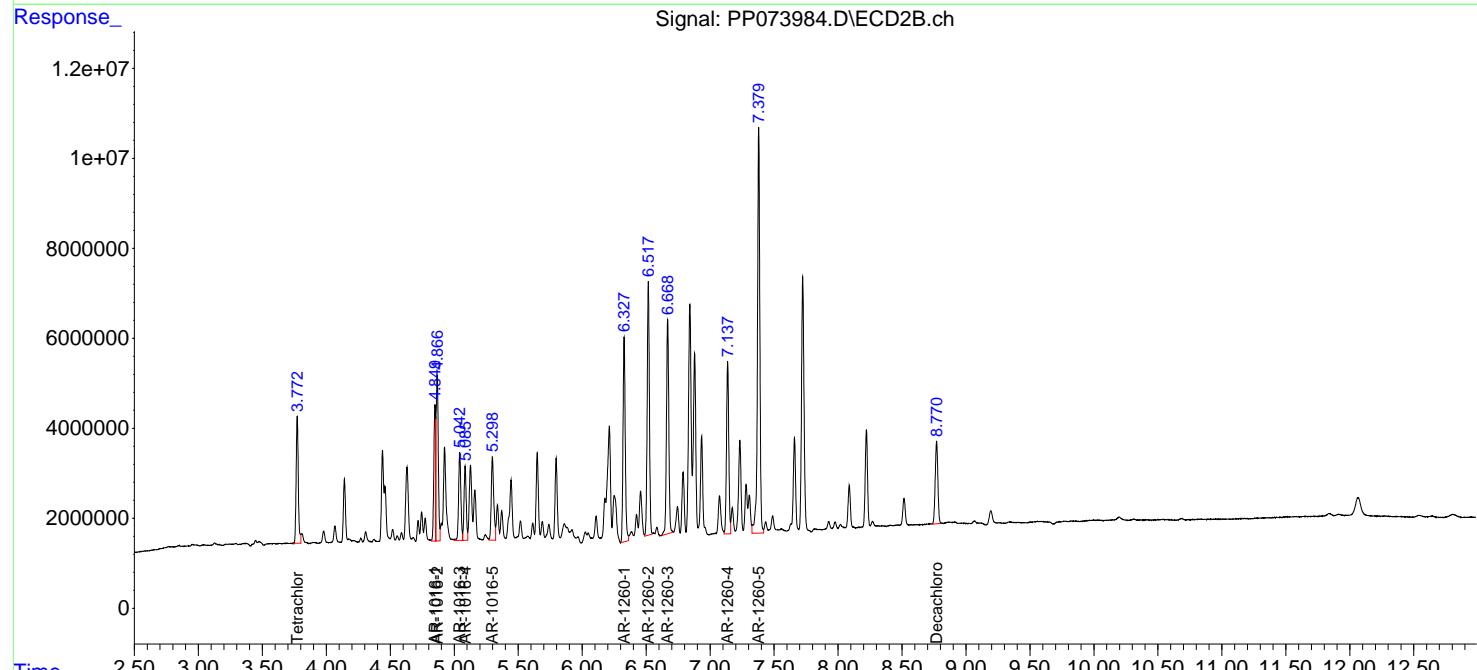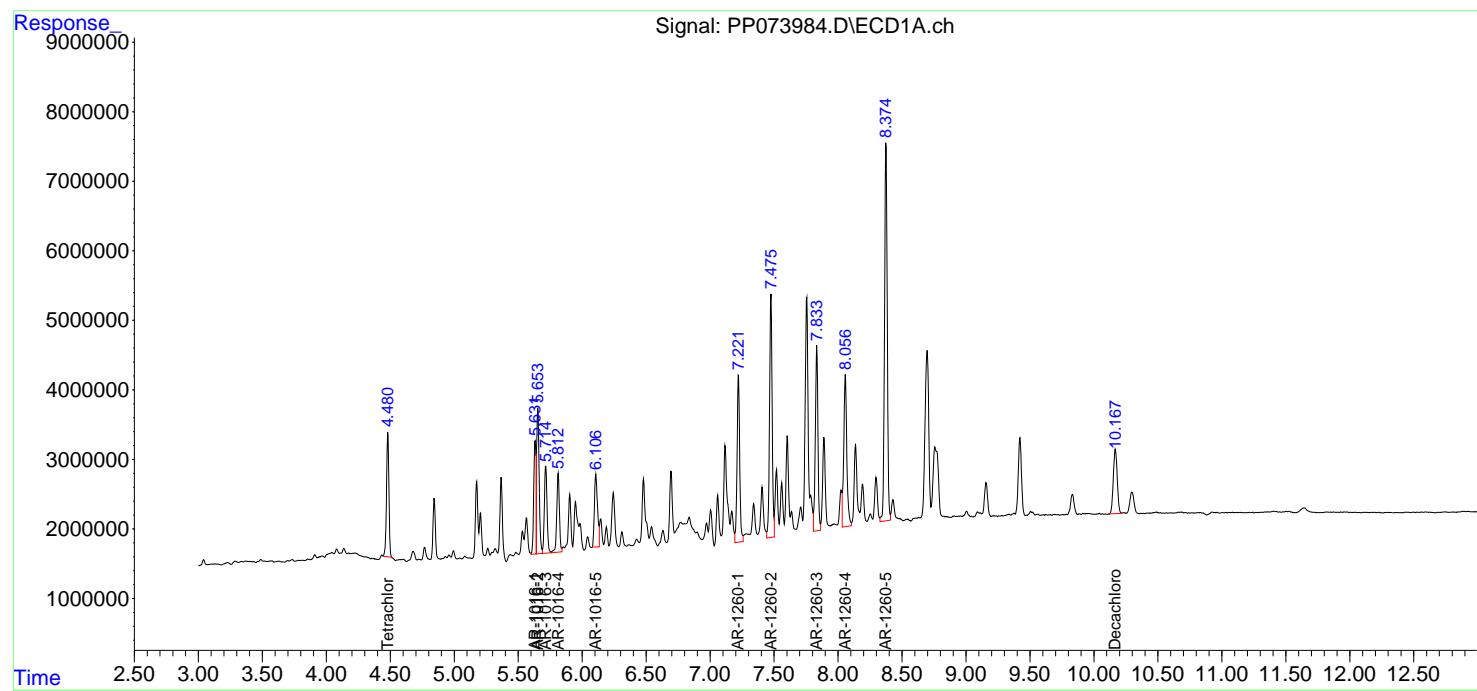

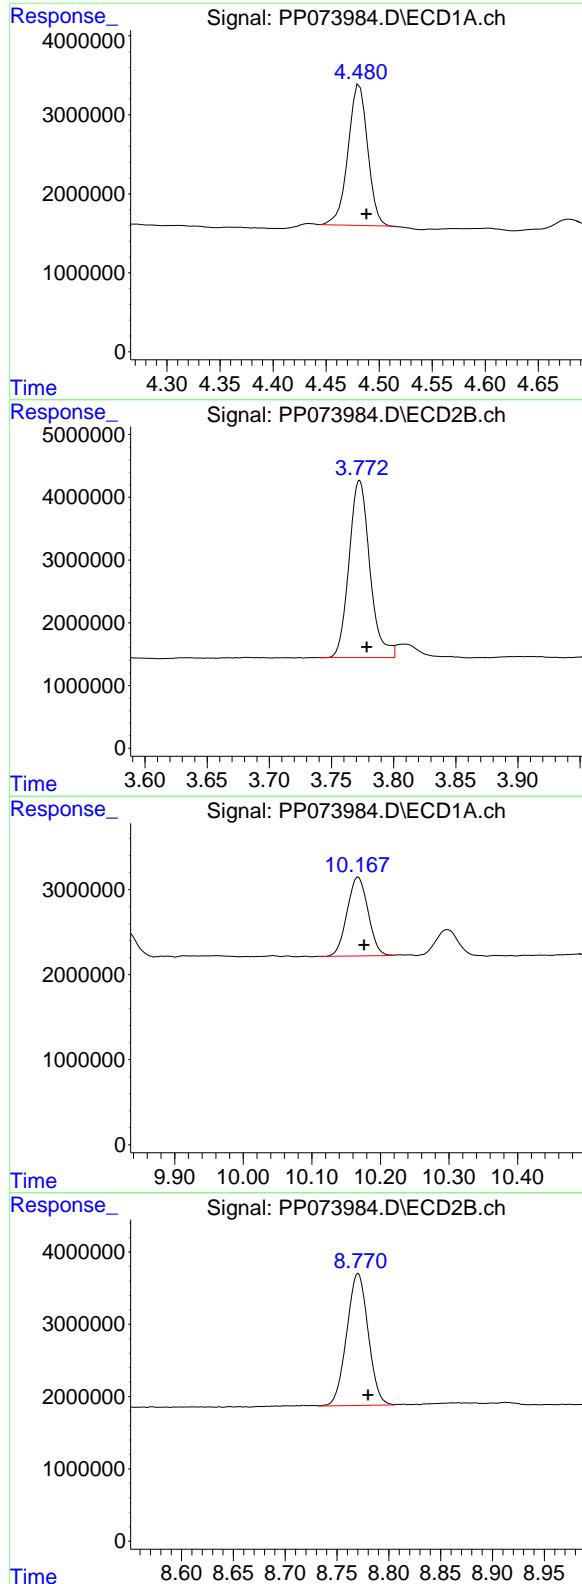

#1 Tetrachloro-m-xylene

R.T.: 4.480 min
Delta R.T.: -0.008 min
Response: 22954565
Conc: 16.76 ng/ml

Instrument: ECD_P
ClientSampleId: RT2286MS

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/22/2025
Supervised By :mohammad ahmed 07/23/2025

#1 Tetrachloro-m-xylene


R.T.: 3.773 min
Delta R.T.: -0.006 min
Response: 32913477
Conc: 17.87 ng/ml

#2 Decachlorobiphenyl

R.T.: 10.168 min
Delta R.T.: -0.008 min
Response: 19654459
Conc: 18.01 ng/ml

#2 Decachlorobiphenyl

R.T.: 8.770 min
Delta R.T.: -0.010 min
Response: 26316757
Conc: 19.89 ng/ml

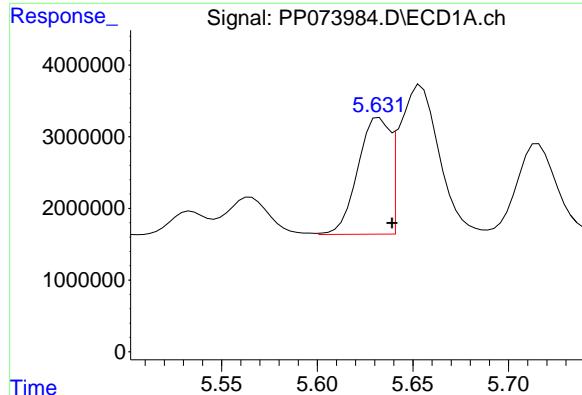


#3 AR-1016-1

R.T.: 5.633 min
Delta R.T.: -0.006 min
Response: 18863800
Conc: 397.02 ng/ml

Instrument :
ECD_P
ClientSampleId :
RT2286MS


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/22/2025
Supervised By :mohammad ahmed 07/23/2025

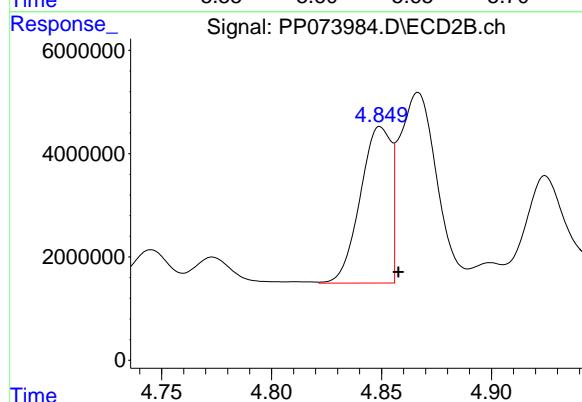


#3 AR-1016-1

R.T.: 4.849 min
Delta R.T.: -0.008 min
Response: 29465448
Conc: 432.20 ng/ml

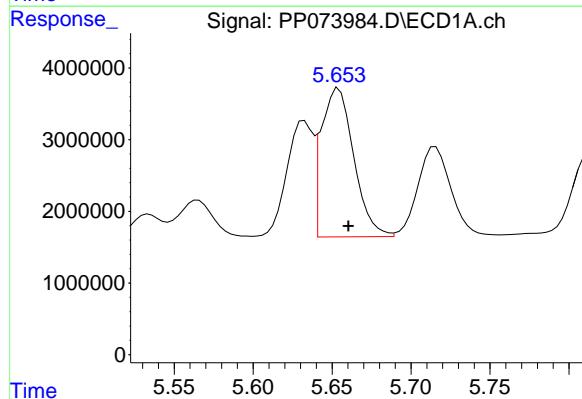


#4 AR-1016-2

R.T.: 5.654 min
Delta R.T.: -0.006 min
Response: 29837172
Conc: 418.97 ng/ml

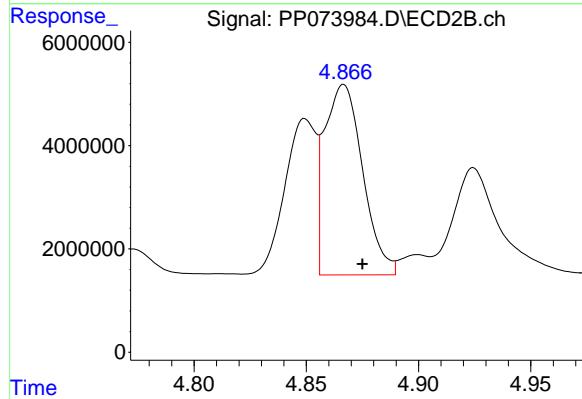

#4 AR-1016-2

R.T.: 4.867 min
Delta R.T.: -0.008 min
Response: 43500761
Conc: 426.96 ng/ml

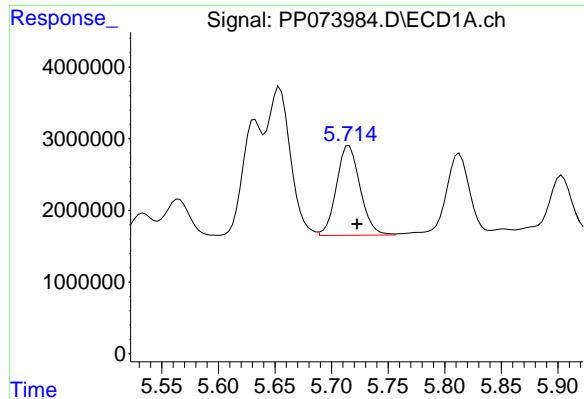


#5 AR-1016-3

R.T.: 5.716 min
Delta R.T.: -0.007 min
Response: 18207530
Conc: 417.00 ng/ml

Instrument:
ECD_P
ClientSampleId :
RT2286MS


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/22/2025
Supervised By :mohammad ahmed 07/23/2025

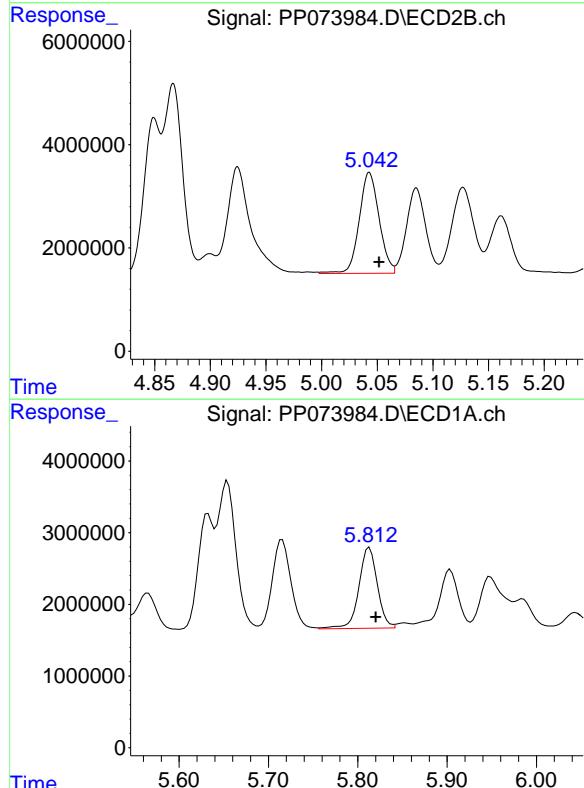

#5 AR-1016-3

R.T.: 5.043 min
Delta R.T.: -0.009 min
Response: 24326097
Conc: 449.60 ng/ml

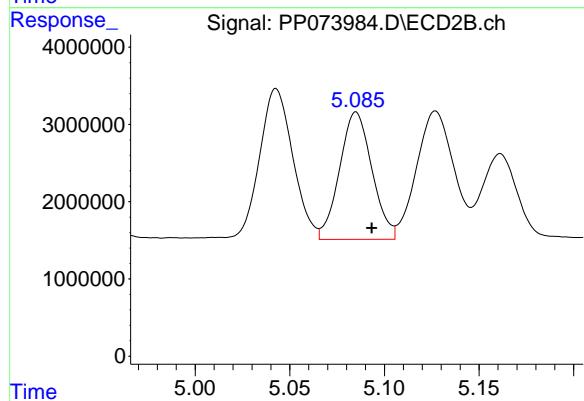


#6 AR-1016-4

R.T.: 5.813 min
Delta R.T.: -0.007 min
Response: 16224197
Conc: 451.35 ng/ml

#6 AR-1016-4

R.T.: 5.085 min
Delta R.T.: -0.008 min
Response: 19663890
Conc: 448.12 ng/ml

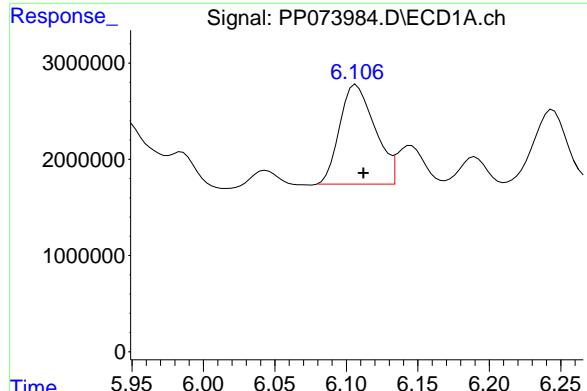


#7 AR-1016-5

R.T.: 6.107 min
Delta R.T.: -0.005 min
Response: 17720270
Conc: 565.59 ng/ml

Instrument: ECD_P
ClientSampleId: RT2286MS


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/22/2025
Supervised By :mohammad ahmed 07/23/2025

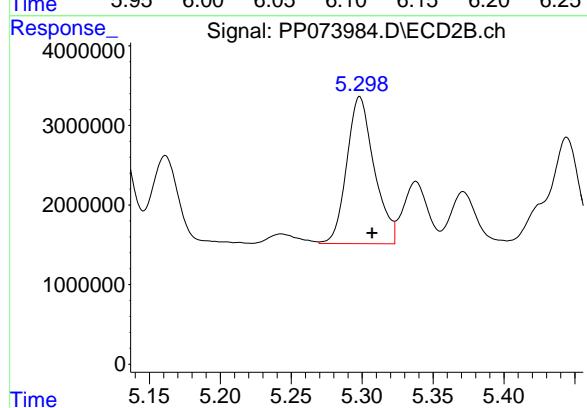


#7 AR-1016-5

R.T.: 5.298 min
Delta R.T.: -0.009 min
Response: 24867794
Conc: 455.60 ng/ml

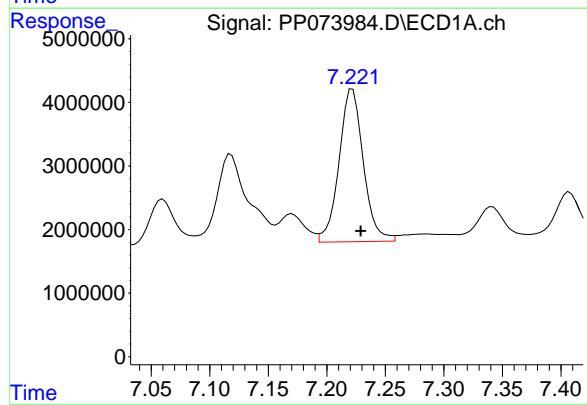


#31 AR-1260-1

R.T.: 7.222 min
Delta R.T.: -0.007 min
Response: 34694505
Conc: 588.43 ng/ml

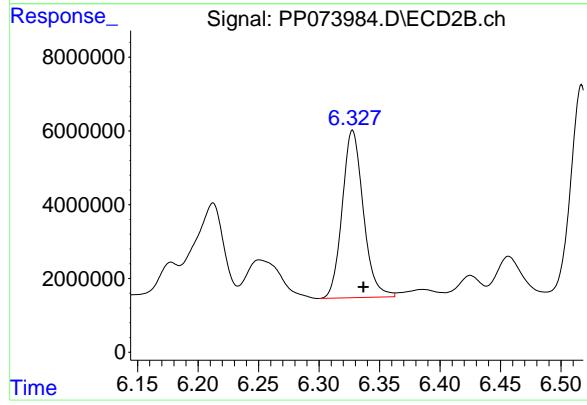

#31 AR-1260-1

R.T.: 6.328 min
Delta R.T.: -0.009 min
Response: 55075376
Conc: 564.53 ng/ml

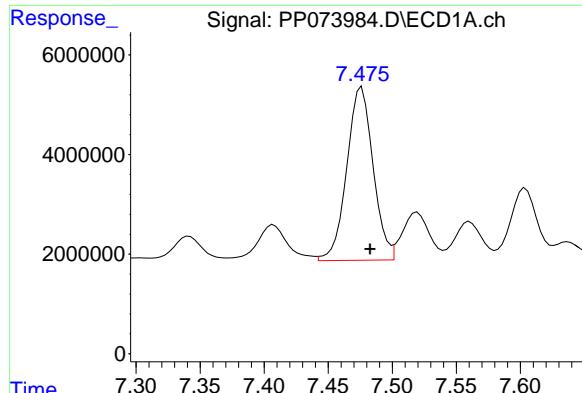


#32 AR-1260-2

R.T.: 7.476 min
Delta R.T.: -0.007 min
Response: 49718794
Conc: 518.77 ng/ml

Instrument: ECD_P
ClientSampleId: RT2286MS

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/22/2025
Supervised By :mohammad ahmed 07/23/2025

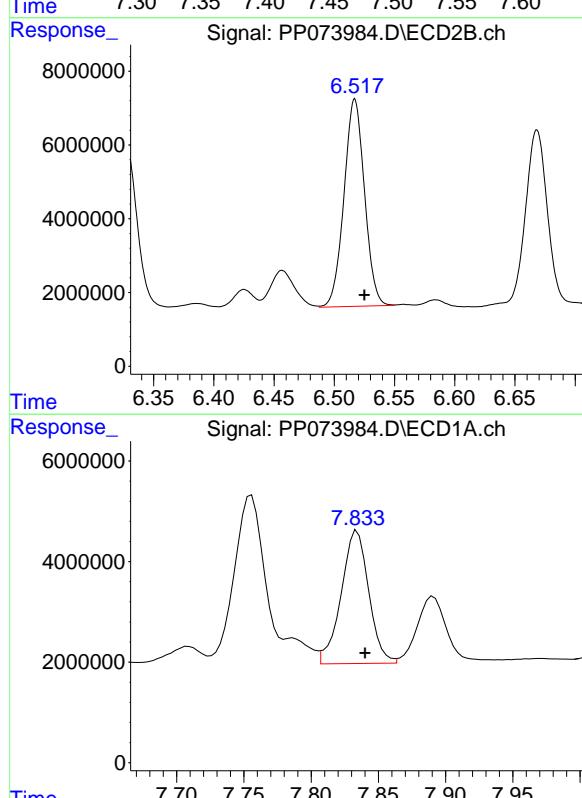


#33 AR-1260-3

R.T.: 7.834 min
Delta R.T.: -0.006 min
Response: 37706644
Conc: 516.03 ng/ml

#33 AR-1260-3

R.T.: 6.668 min
Delta R.T.: -0.009 min
Response: 60304176
Conc: 550.91 ng/ml

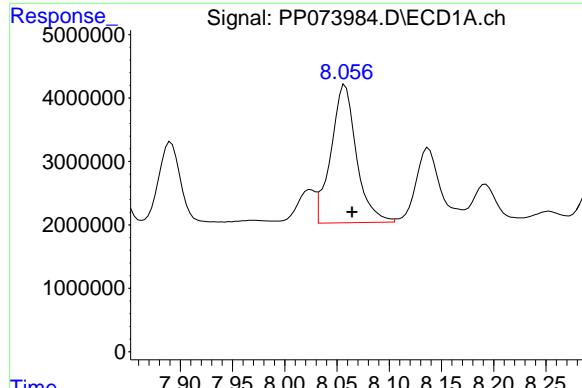


#34 AR-1260-4

R.T.: 8.058 min
Delta R.T.: -0.007 min
Response: 36868595
Conc: 564.60 ng/ml

Instrument: ECD_P
ClientSampleId: RT2286MS


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/22/2025
Supervised By :mohammad ahmed 07/23/2025

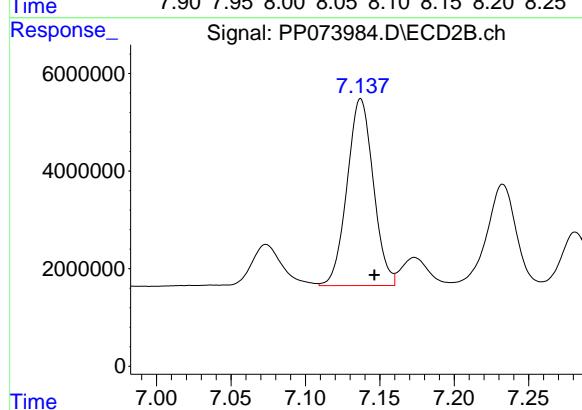


#34 AR-1260-4

R.T.: 7.137 min
Delta R.T.: -0.009 min
Response: 47082456
Conc: 526.60 ng/ml

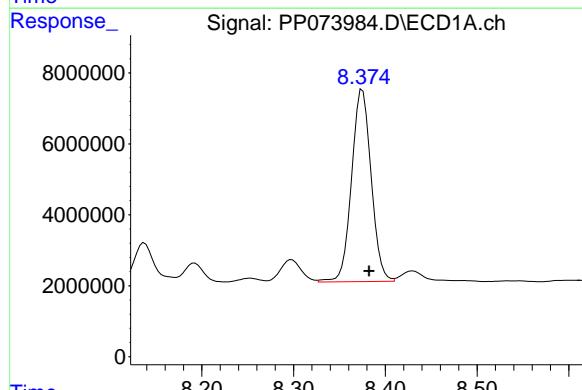

#35 AR-1260-5

R.T.: 8.375 min
Delta R.T.: -0.007 min
Response: 80346257
Conc: 532.61 ng/ml

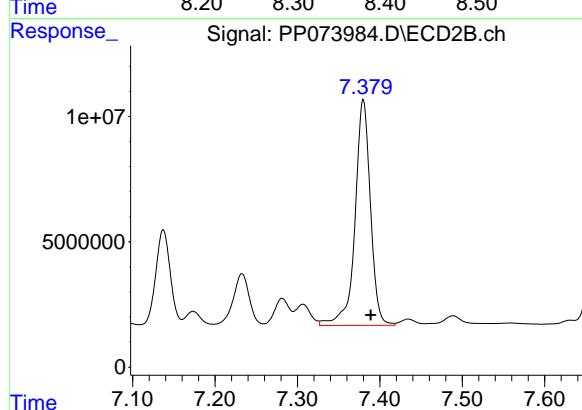

#35 AR-1260-5

R.T.: 7.380 min
Delta R.T.: -0.009 min
Response: 117176775
Conc: 521.40 ng/ml



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

Report of Analysis

Client:	Nobis Group			Date Collected:	07/17/25	
Project:	Raymark Superfund Site			Date Received:	07/17/25	
Client Sample ID:	RT2286MSD			SDG No.:	Q2639	
Lab Sample ID:	Q2635-01MSD			Matrix:	SOIL	
Analytical Method:	8082A			% Solid:	84.8	Decanted:
Sample Wt/Vol:	30.02	Units:	g	Final Vol:	10000	uL
Soil Aliquot Vol:	uL			Test:	PCB	
Extraction Type:				Injection Volume :		
GPC Factor :	1.0	PH :				
Prep Method :	SW3541B					

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PP073985.D	1	07/21/25 08:30	07/21/25 13:56	PB168927

CAS Number	Parameter	Conc.	Qualifier	MDL	LOD	LOQ / CRQL	Units(Dry Weight)
TARGETS							
12674-11-2	Aroclor-1016	177		4.70	9.80	20.0	ug/kg
11104-28-2	Aroclor-1221	15.3	U	4.70	15.3	20.0	ug/kg
11141-16-5	Aroclor-1232	9.80	U	4.40	9.80	20.0	ug/kg
53469-21-9	Aroclor-1242	9.80	U	4.70	9.80	20.0	ug/kg
12672-29-6	Aroclor-1248	15.3	U	7.00	15.3	20.0	ug/kg
11097-69-1	Aroclor-1254	9.80	U	3.80	9.80	20.0	ug/kg
37324-23-5	Aroclor-1262	15.3	U	5.90	15.3	20.0	ug/kg
11100-14-4	Aroclor-1268	9.80	U	4.20	9.80	20.0	ug/kg
11096-82-5	Aroclor-1260	211		3.80	9.80	20.0	ug/kg
SURROGATES							
877-09-8	Tetrachloro-m-xylene	17.9		44 - 130		89%	SPK: 20
2051-24-3	Decachlorobiphenyl	19.4		60 - 125		97%	SPK: 20

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP072125\
 Data File : PP073985.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jul 2025 13:56
 Operator : YP\AJ
 Sample : Q2635-01MSD
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
RT2286MSD

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/22/2025
 Supervised By :mohammad ahmed 07/23/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 22 01:51:16 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 08 08:35:32 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	4.485	3.774	23007780	32891692	16.800	17.854
2) SA Decachlor...	10.171	8.771	19437749	25634073	17.816	19.374

Target Compounds

3) L1 AR-1016-1	5.636	4.851	18736879	29541322	394.348	433.318
4) L1 AR-1016-2	5.657	4.869	30133135	43844893	423.130	430.340
5) L1 AR-1016-3	5.719	5.045	18269038	24208384	418.409	447.422
6) L1 AR-1016-4	5.816	5.087	16118675	19716668	448.419	449.323
7) L1 AR-1016-5	6.110	5.300	17783528	24543584	567.612	449.660
31) L7 AR-1260-1	7.224	6.330	31705759	54851085	537.739m	562.228
32) L7 AR-1260-2	7.478	6.518	47342830	65815583	493.978m	535.794
33) L7 AR-1260-3	7.837	6.670	37810191	59476912	517.447	543.348
34) L7 AR-1260-4	8.059	7.139	38655725	46277558	591.972m	517.597
35) L7 AR-1260-5	8.378	7.383	80997949	117.0E6	536.934	520.578

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP072125\
 Data File : PP073985.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jul 2025 13:56
 Operator : YP\AJ
 Sample : Q2635-01MSD
 Misc :
 ALS Vial : 15 Sample Multiplier: 1



Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 22 01:51:16 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 08 08:35:32 2025
 Response via : Initial Calibration
 Integrator: ChemStation


Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Instrument :
 ECD_P
 ClientSampleId :
 RT2286MSD

Manual Integrations APPROVED

Reviewed By :Yogesh Patel 07/22/2025
 Supervised By :mohammad ahmed 07/23/2025

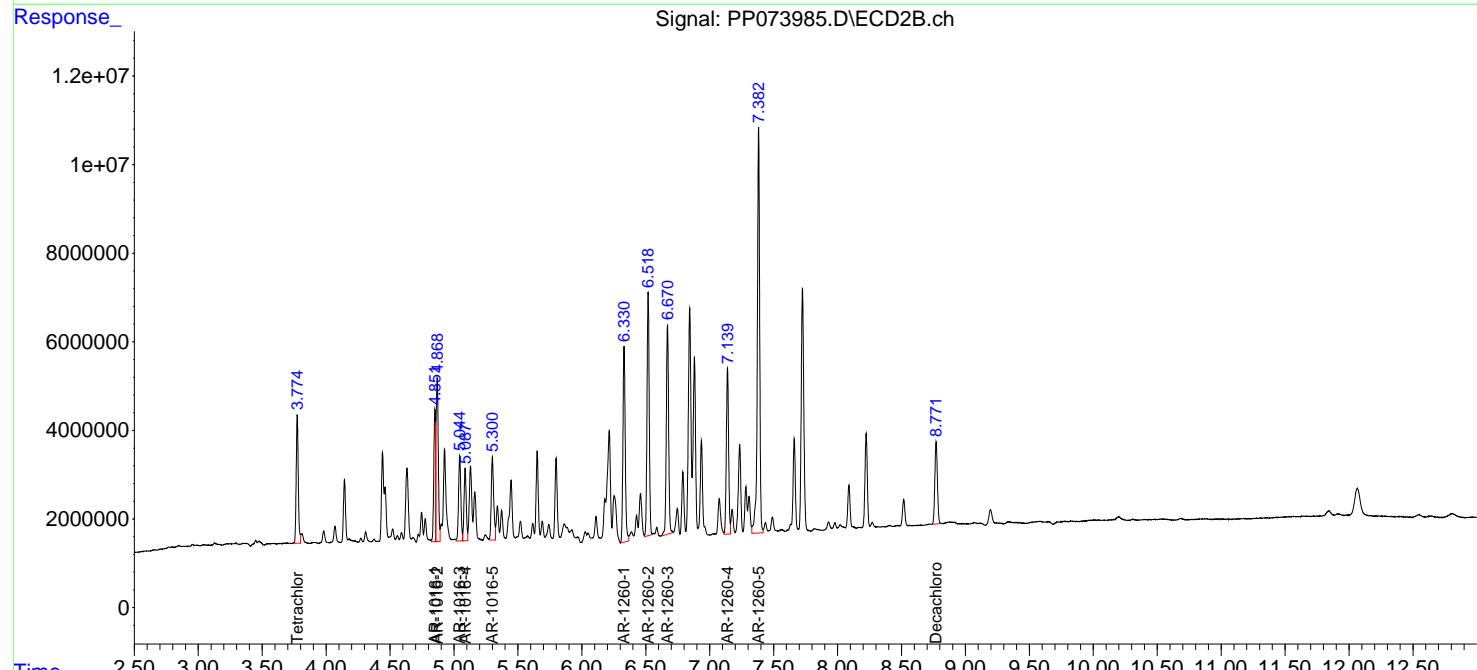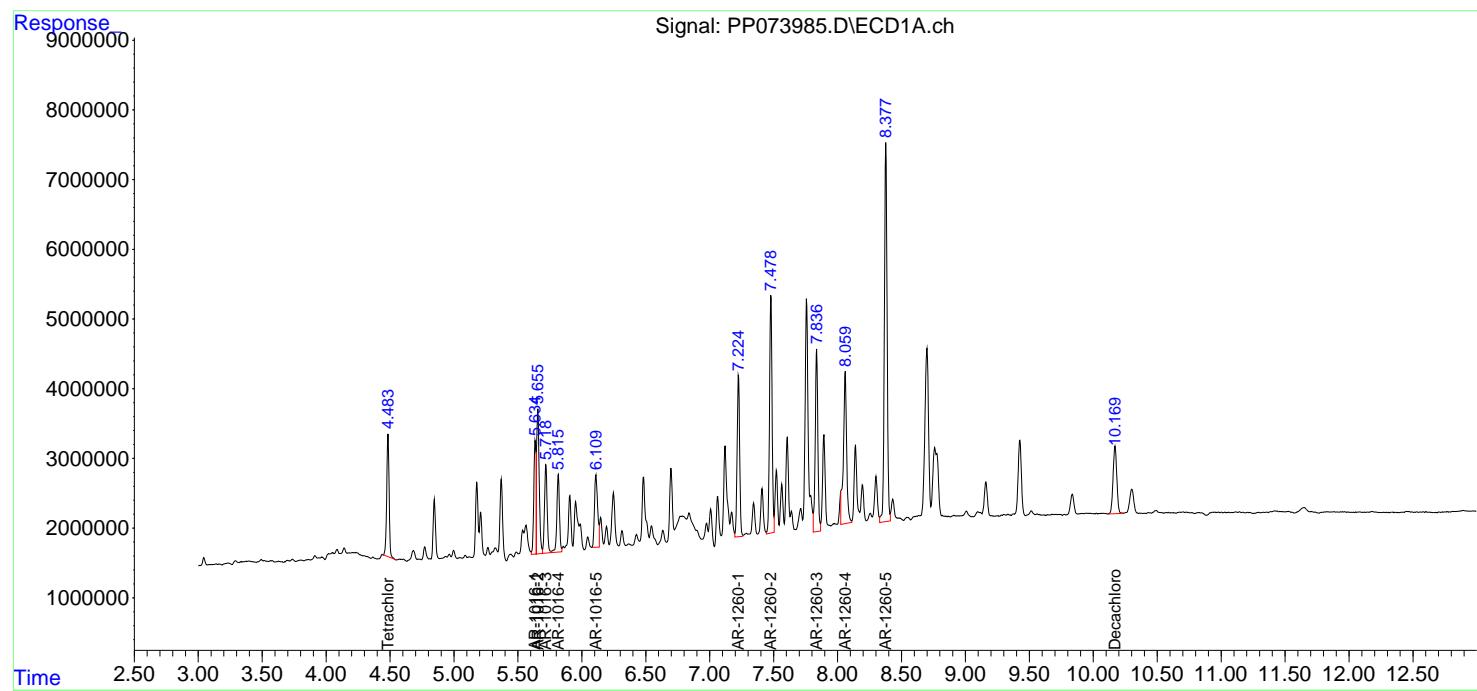

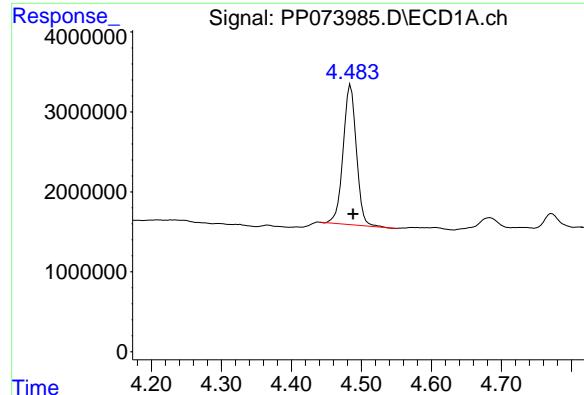


#1 Tetrachloro-m-xylene

R.T.: 4.485 min
Delta R.T.: -0.003 min
Response: 23007780
Conc: 16.80 ng/ml

Instrument:
ECD_P
ClientSampleId :
RT2286MSD


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/22/2025
Supervised By :mohammad ahmed 07/23/2025

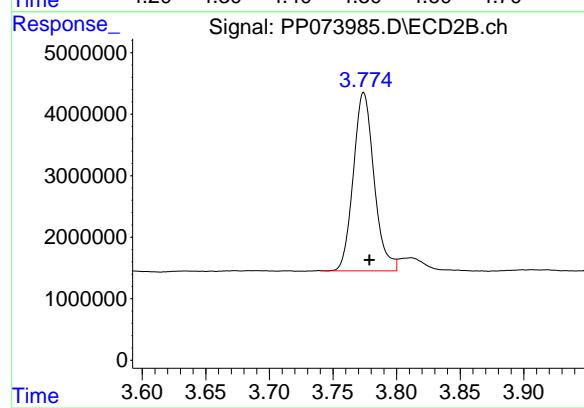


#1 Tetrachloro-m-xylene

R.T.: 3.774 min
Delta R.T.: -0.004 min
Response: 32891692
Conc: 17.85 ng/ml

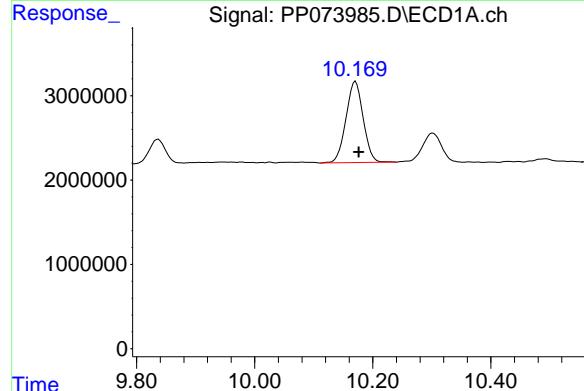


#2 Decachlorobiphenyl

R.T.: 10.171 min
Delta R.T.: -0.005 min
Response: 19437749
Conc: 17.82 ng/ml

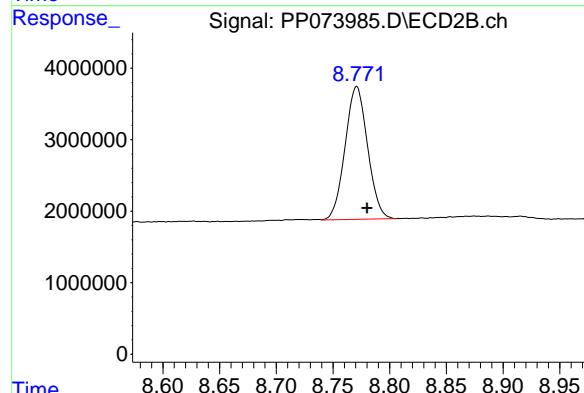

#2 Decachlorobiphenyl

R.T.: 8.771 min
Delta R.T.: -0.009 min
Response: 25634073
Conc: 19.37 ng/ml

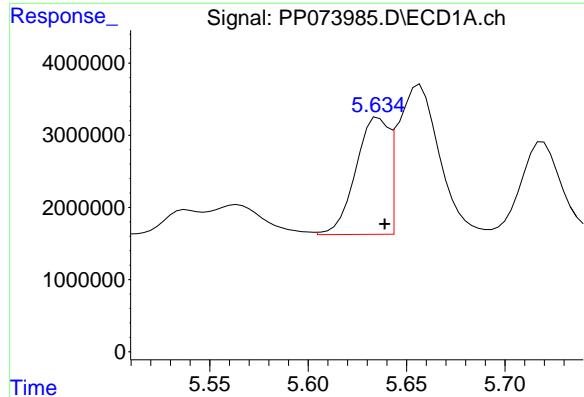


#3 AR-1016-1

R.T.: 5.636 min
Delta R.T.: -0.003 min
Response: 18736879
Conc: 394.35 ng/ml

Instrument:
ECD_P
ClientSampleId :
RT2286MSD


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/22/2025
Supervised By :mohammad ahmed 07/23/2025

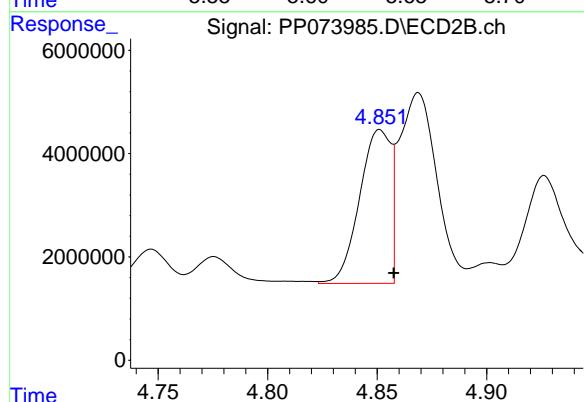


#3 AR-1016-1

R.T.: 4.851 min
Delta R.T.: -0.006 min
Response: 29541322
Conc: 433.32 ng/ml

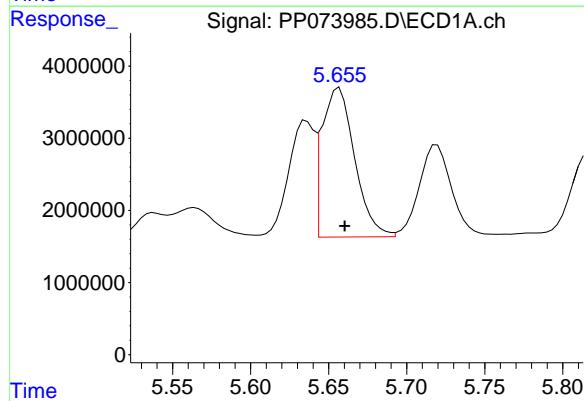


#4 AR-1016-2

R.T.: 5.657 min
Delta R.T.: -0.004 min
Response: 30133135
Conc: 423.13 ng/ml

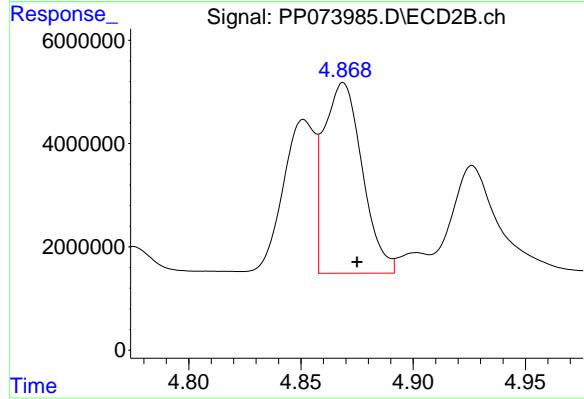

#4 AR-1016-2

R.T.: 4.869 min
Delta R.T.: -0.006 min
Response: 43844893
Conc: 430.34 ng/ml

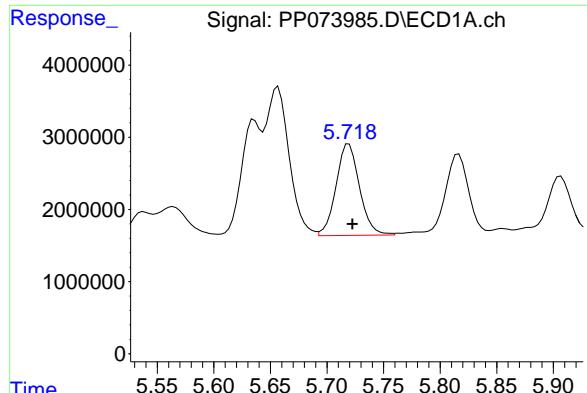


#5 AR-1016-3

R.T.: 5.719 min
Delta R.T.: -0.003 min
Response: 18269038
Conc: 418.41 ng/ml

Instrument: ECD_P
ClientSampleId: RT2286MSD


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/22/2025
Supervised By :mohammad ahmed 07/23/2025

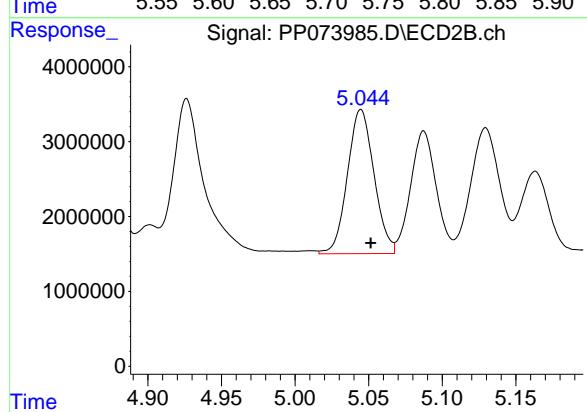


#5 AR-1016-3

R.T.: 5.045 min
Delta R.T.: -0.007 min
Response: 24208384
Conc: 447.42 ng/ml

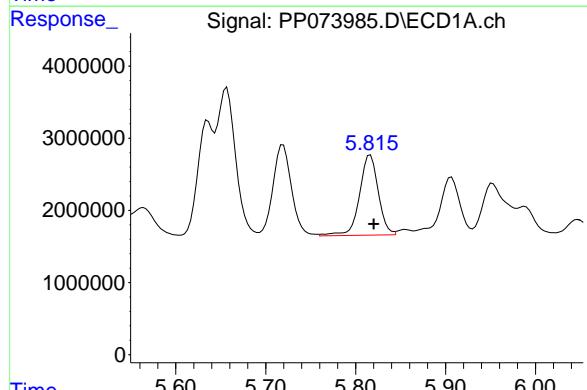


#6 AR-1016-4

R.T.: 5.816 min
Delta R.T.: -0.004 min
Response: 16118675
Conc: 448.42 ng/ml

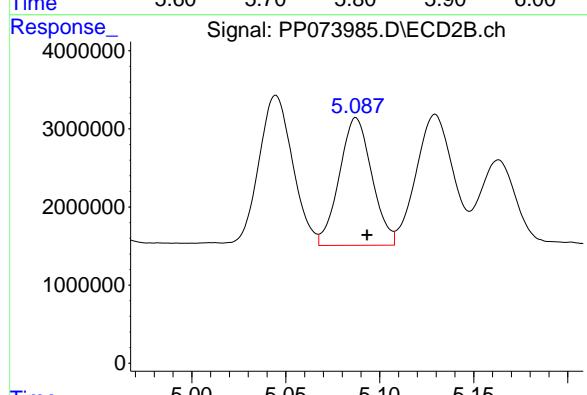

#6 AR-1016-4

R.T.: 5.087 min
Delta R.T.: -0.006 min
Response: 19716668
Conc: 449.32 ng/ml

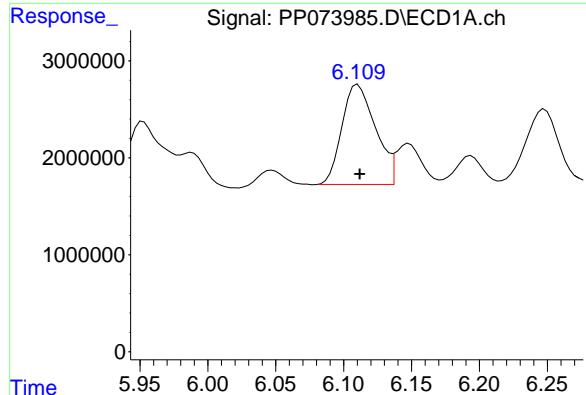


#7 AR-1016-5

R.T.: 6.110 min
Delta R.T.: -0.001 min
Response: 17783528
Conc: 567.61 ng/ml

Instrument: ECD_P
ClientSampleId: RT2286MSD


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/22/2025
Supervised By :mohammad ahmed 07/23/2025

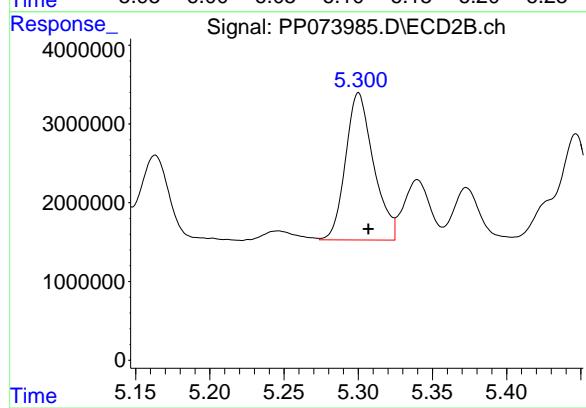


#7 AR-1016-5

R.T.: 5.300 min
Delta R.T.: -0.007 min
Response: 24543584
Conc: 449.66 ng/ml

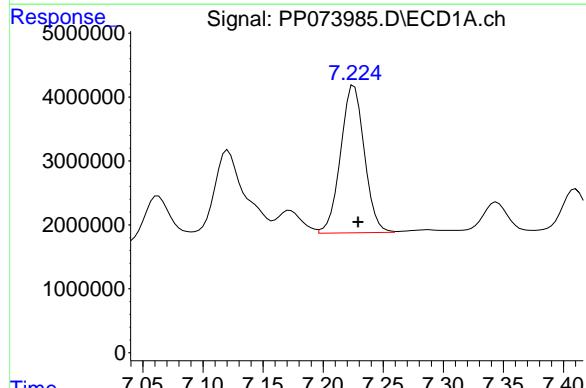


#31 AR-1260-1

R.T.: 7.224 min
Delta R.T.: -0.005 min
Response: 31705759
Conc: 537.74 ng/ml

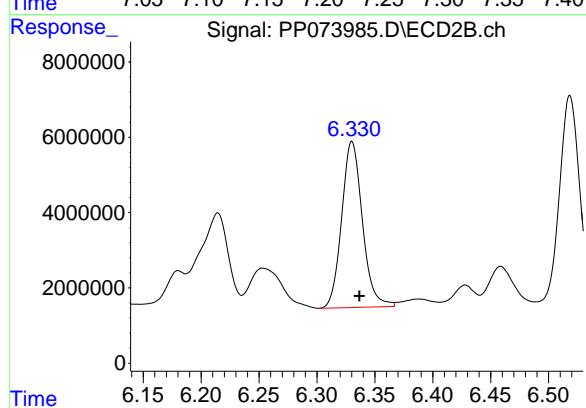

#31 AR-1260-1

R.T.: 6.330 min
Delta R.T.: -0.006 min
Response: 54851085
Conc: 562.23 ng/ml

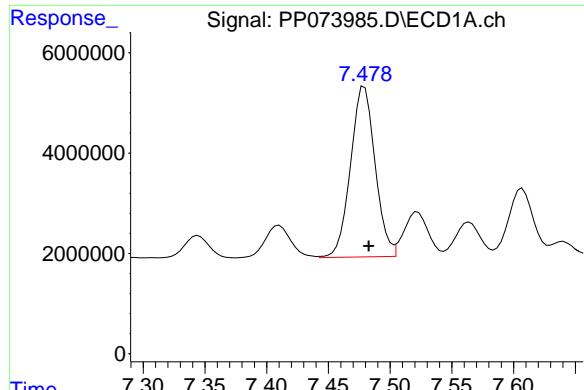


#32 AR-1260-2

R.T.: 7.478 min
Delta R.T.: -0.005 min
Response: 47342830
Conc: 493.98 ng/ml

Instrument: ECD_P
ClientSampleId: RT2286MSD

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/22/2025
Supervised By :mohammad ahmed 07/23/2025

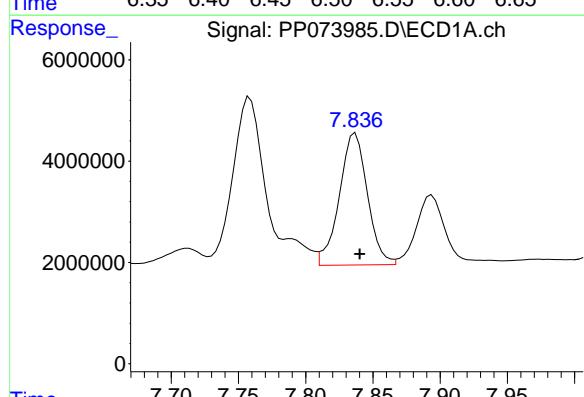


#33 AR-1260-3

R.T.: 7.837 min
Delta R.T.: -0.003 min
Response: 37810191
Conc: 517.45 ng/ml

#33 AR-1260-3

R.T.: 6.670 min
Delta R.T.: -0.007 min
Response: 59476912
Conc: 543.35 ng/ml

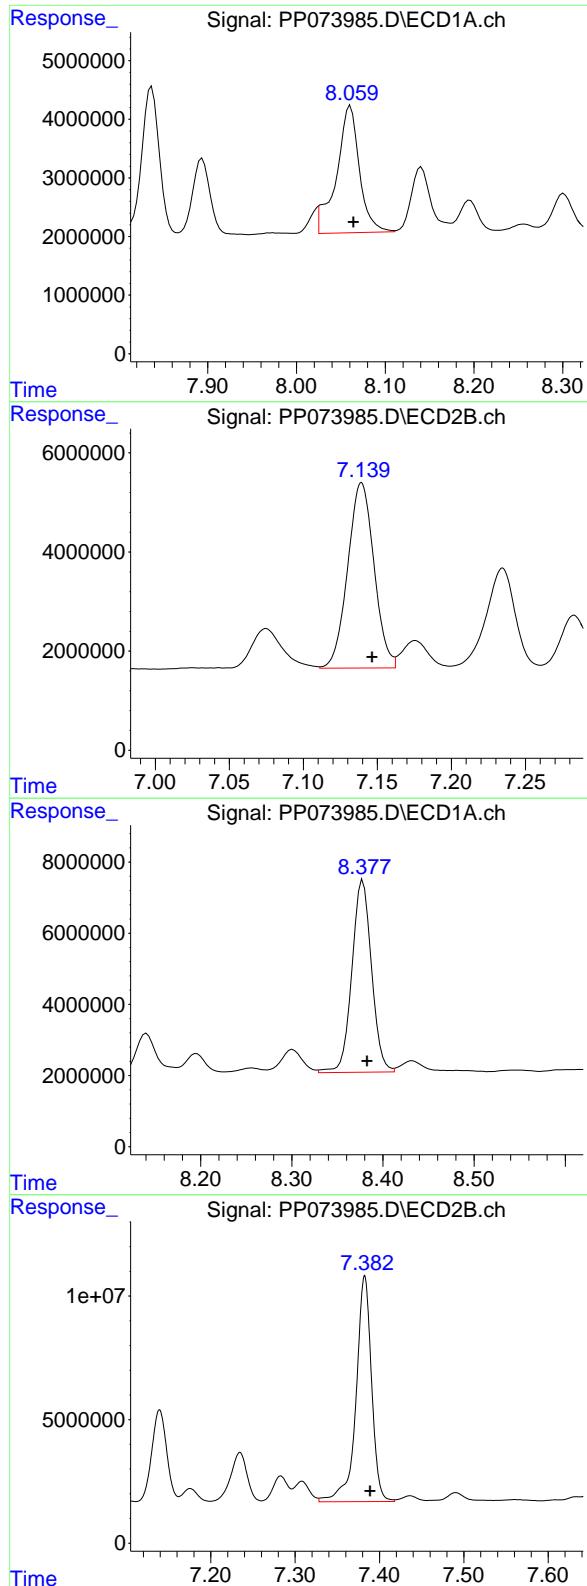

#34 AR-1260-4

R.T.: 8.059 min
 Delta R.T.: -0.005 min
 Response: 38655725
 Conc: 591.97 ng/ml

Instrument: ECD_P
 ClientSampleId: RT2286MSD

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/22/2025
 Supervised By :mohammad ahmed 07/23/2025

#34 AR-1260-4

R.T.: 7.139 min
 Delta R.T.: -0.007 min
 Response: 46277558
 Conc: 517.60 ng/ml

#35 AR-1260-5

R.T.: 8.378 min
 Delta R.T.: -0.005 min
 Response: 80997949
 Conc: 536.93 ng/ml

#35 AR-1260-5

R.T.: 7.383 min
 Delta R.T.: -0.006 min
 Response: 116992994
 Conc: 520.58 ng/ml

Manual Integration Report

Sequence:	po070825	Instrument	ECD_o
-----------	----------	------------	-------

Sample ID	File ID	Parameter	Review By	Review On	Supervised By	Supervised On	Reason
AR1660ICC1000	PO112088.D	AR-1016-3 #2	yogesh	7/9/2025 7:27:19 AM	mohammad	7/10/2025 2:03:44	Peak Integrated by Software
AR1660ICC1000	PO112088.D	AR-1260-3 #2	yogesh	7/9/2025 7:27:19 AM	mohammad	7/10/2025 2:03:44	Peak Integrated by Software
AR1660ICC1000	PO112088.D	Decachlorobiphenyl #2	yogesh	7/9/2025 7:27:19 AM	mohammad	7/10/2025 2:03:44	Peak Integrated by Software
AR1660ICC1000	PO112088.D	Tetrachloro-m-xylene	yogesh	7/9/2025 7:27:19 AM	mohammad	7/10/2025 2:03:44	Peak Integrated by Software
AR1660ICC1000	PO112088.D	Tetrachloro-m-xylene #2	yogesh	7/9/2025 7:27:19 AM	mohammad	7/10/2025 2:03:44	Peak Integrated by Software
AR1660ICC750	PO112089.D	AR-1016-3 #2	yogesh	7/9/2025 7:27:21 AM	mohammad	7/10/2025 2:03:44	Peak Integrated by Software
AR1660ICC750	PO112089.D	AR-1016-4 #2	yogesh	7/9/2025 7:27:21 AM	mohammad	7/10/2025 2:03:44	Peak Integrated by Software
AR1660ICC750	PO112089.D	AR-1016-5 #2	yogesh	7/9/2025 7:27:21 AM	mohammad	7/10/2025 2:03:44	Peak Integrated by Software
AR1660ICC750	PO112089.D	AR-1260-3 #2	yogesh	7/9/2025 7:27:21 AM	mohammad	7/10/2025 2:03:44	Peak Integrated by Software
AR1660ICC750	PO112089.D	Decachlorobiphenyl #2	yogesh	7/9/2025 7:27:21 AM	mohammad	7/10/2025 2:03:44	Peak Integrated by Software
AR1660ICC750	PO112089.D	Tetrachloro-m-xylene	yogesh	7/9/2025 7:27:21 AM	mohammad	7/10/2025 2:03:44	Peak Integrated by Software
AR1660ICC750	PO112089.D	Tetrachloro-m-xylene #2	yogesh	7/9/2025 7:27:21 AM	mohammad	7/10/2025 2:03:44	Peak Integrated by Software
AR1660ICC250	PO112091.D	AR-1260-1	yogesh	7/9/2025 7:27:23 AM	mohammad	7/10/2025 2:03:44	Peak Integrated by Software

1
2
3
4
5
6
7
8
9
10
11
12
13
14
15
16
17
18
19
20

Manual Integration Report

Sequence:	po070825	Instrument	ECD_o
-----------	----------	------------	-------

Sample ID	File ID	Parameter	Review By	Review On	Supervised By	Supervised On	Reason
AR1660ICC250	PO112091.D	AR-1260-2	yogesh	7/9/2025 7:27:23 AM	mohammad	7/10/2025 2:03:44	Peak Integrated by Software
AR1660ICC250	PO112091.D	AR-1260-3	yogesh	7/9/2025 7:27:23 AM	mohammad	7/10/2025 2:03:44	Peak Integrated by Software
AR1660ICC250	PO112091.D	AR-1260-3 #2	yogesh	7/9/2025 7:27:23 AM	mohammad	7/10/2025 2:03:44	Peak Integrated by Software
AR1660ICC250	PO112091.D	AR-1260-4	yogesh	7/9/2025 7:27:23 AM	mohammad	7/10/2025 2:03:44	Peak Integrated by Software
AR1660ICC250	PO112091.D	AR-1260-5	yogesh	7/9/2025 7:27:23 AM	mohammad	7/10/2025 2:03:44	Peak Integrated by Software
AR1660ICC250	PO112091.D	Decachlorobiphenyl #2	yogesh	7/9/2025 7:27:23 AM	mohammad	7/10/2025 2:03:44	Peak Integrated by Software
AR1660ICC250	PO112091.D	Tetrachloro-m-xylene #2	yogesh	7/9/2025 7:27:23 AM	mohammad	7/10/2025 2:03:44	Peak Integrated by Software
AR1660ICC050	PO112092.D	AR-1016-5	yogesh	7/9/2025 7:27:25 AM	mohammad	7/10/2025 2:03:44	Peak Integrated by Software
AR1660ICC050	PO112092.D	AR-1260-1	yogesh	7/9/2025 7:27:25 AM	mohammad	7/10/2025 2:03:44	Peak Integrated by Software
AR1660ICC050	PO112092.D	AR-1260-1 #2	yogesh	7/9/2025 7:27:25 AM	mohammad	7/10/2025 2:03:44	Peak Integrated by Software
AR1660ICC050	PO112092.D	AR-1260-2	yogesh	7/9/2025 7:27:25 AM	mohammad	7/10/2025 2:03:44	Peak Integrated by Software
AR1660ICC050	PO112092.D	AR-1260-2 #2	yogesh	7/9/2025 7:27:25 AM	mohammad	7/10/2025 2:03:44	Peak Integrated by Software
AR1660ICC050	PO112092.D	Decachlorobiphenyl #2	yogesh	7/9/2025 7:27:25 AM	mohammad	7/10/2025 2:03:44	Peak Integrated by Software

1
2
3
4
5
6
7
8
9
10
11
12
13
14
15
16
17
18
19
20

Manual Integration Report

Sequence:	po070825	Instrument	ECD_o
-----------	----------	------------	-------

Sample ID	File ID	Parameter	Review By	Review On	Supervised By	Supervised On	Reason
AR1242ICC050	PO112099.D	AR-1242-5	yogesh	7/9/2025 7:27:26 AM	mohammad	7/10/2025 2:03:44	Peak Integrated by Software
AR1242ICC050	PO112099.D	AR-1242-5 #2	yogesh	7/9/2025 7:27:26 AM	mohammad	7/10/2025 2:03:44	Peak Integrated by Software
AR1248ICC050	PO112104.D	AR-1248-4 #2	yogesh	7/9/2025 7:27:28 AM	mohammad	7/10/2025 2:03:44	Peak Integrated by Software
AR1248ICC050	PO112104.D	AR-1248-5 #2	yogesh	7/9/2025 7:27:28 AM	mohammad	7/10/2025 2:03:44	Peak Integrated by Software
AR1254ICC050	PO112109.D	AR-1254-1 #2	yogesh	7/9/2025 7:27:30 AM	mohammad	7/10/2025 2:03:44	Peak Integrated by Software
AR1254ICC050	PO112109.D	AR-1254-2 #2	yogesh	7/9/2025 7:27:30 AM	mohammad	7/10/2025 2:03:44	Peak Integrated by Software
AR1254ICC050	PO112109.D	AR-1254-4	yogesh	7/9/2025 7:27:30 AM	mohammad	7/10/2025 2:03:44	Peak Integrated by Software
AR1268ICC1000	PO112111.D	AR-1268-4	yogesh	7/9/2025 7:27:32 AM	mohammad	7/10/2025 2:03:44	Peak Integrated by Software
AR1268ICC050	PO112115.D	AR-1268-1	yogesh	7/9/2025 7:27:33 AM	mohammad	7/10/2025 2:03:44	Peak Integrated by Software
AR1268ICC050	PO112115.D	AR-1268-3	yogesh	7/9/2025 7:27:33 AM	mohammad	7/10/2025 2:03:44	Peak Integrated by Software
PO070825ICV500	PO112116.D	AR-1016-1 #2	yogesh	7/9/2025 7:27:35 AM	mohammad	7/10/2025 2:03:44	Peak Integrated by Software
PO070825ICV500	PO112116.D	AR-1016-2 #2	yogesh	7/9/2025 7:27:35 AM	mohammad	7/10/2025 2:03:44	Peak Integrated by Software
PO070825ICV500	PO112116.D	AR-1260-3 #2	yogesh	7/9/2025 7:27:35 AM	mohammad	7/10/2025 2:03:44	Peak Integrated by Software

1
2
3
4
5
6
7
8
9
10
11
12
13
14
15
16
17
18
19
20

Manual Integration Report

Sequence:	po070825	Instrument	ECD_o
-----------	----------	------------	-------

Sample ID	File ID	Parameter	Review By	Review On	Supervised By	Supervised On	Reason
PO070825ICV500	PO112116.D	AR-1260-4 #2	yogesh	7/9/2025 7:27:35 AM	mohammad	7/10/2025 2:03:44	Peak Integrated by Software

1
2
3
4
5
6
7
8
9
10
11
12
13
14
15
16
17
18
19
20

Manual Integration Report

Sequence:	po072125	Instrument	ECD_o
-----------	----------	------------	-------

Sample ID	File ID	Parameter	Review By	Review On	Supervised By	Supervised On	Reason
AR1660CCC500	PO112332.D	AR-1016-1 #2	yogesh	7/22/2025 10:13:35 AM	mohammad	7/23/2025 1:33:05	Peak Integrated by Software
AR1660CCC500	PO112332.D	AR-1016-2 #2	yogesh	7/22/2025 10:13:35 AM	mohammad	7/23/2025 1:33:05	Peak Integrated by Software
AR1660CCC500	PO112332.D	AR-1016-3 #2	yogesh	7/22/2025 10:13:35 AM	mohammad	7/23/2025 1:33:05	Peak Integrated by Software
AR1660CCC500	PO112332.D	AR-1016-4 #2	yogesh	7/22/2025 10:13:35 AM	mohammad	7/23/2025 1:33:05	Peak Integrated by Software
AR1660CCC500	PO112332.D	AR-1016-5 #2	yogesh	7/22/2025 10:13:35 AM	mohammad	7/23/2025 1:33:05	Peak Integrated by Software
AR1660CCC500	PO112332.D	AR-1260-3 #2	yogesh	7/22/2025 10:13:35 AM	mohammad	7/23/2025 1:33:05	Peak Integrated by Software
AR1660CCC500	PO112332.D	AR-1260-4 #2	yogesh	7/22/2025 10:13:35 AM	mohammad	7/23/2025 1:33:05	Peak Integrated by Software
AR1242CCC500	PO112333.D	AR-1242-1 #2	yogesh	7/22/2025 10:13:37 AM	mohammad	7/23/2025 1:33:05	Peak Integrated by Software
AR1242CCC500	PO112333.D	AR-1242-2 #2	yogesh	7/22/2025 10:13:37 AM	mohammad	7/23/2025 1:33:05	Peak Integrated by Software
AR1660CCC500	PO112346.D	AR-1016-1 #2	yogesh	7/22/2025 10:13:48 AM	mohammad	7/23/2025 1:33:05	Peak Integrated by Software
AR1660CCC500	PO112346.D	AR-1016-2 #2	yogesh	7/22/2025 10:13:48 AM	mohammad	7/23/2025 1:33:05	Peak Integrated by Software
AR1660CCC500	PO112346.D	AR-1016-3 #2	yogesh	7/22/2025 10:13:48 AM	mohammad	7/23/2025 1:33:05	Peak Integrated by Software
AR1660CCC500	PO112346.D	AR-1016-4 #2	yogesh	7/22/2025 10:13:48 AM	mohammad	7/23/2025 1:33:05	Peak Integrated by Software

1
2
3
4
5
6
7
8
9
10
11
12
13
14
15
16
17
18
19
20

Manual Integration Report

Sequence:	po072125	Instrument	ECD_o
-----------	----------	------------	-------

Sample ID	File ID	Parameter	Review By	Review On	Supervised By	Supervised On	Reason
AR1660CCC500	PO112346.D	AR-1016-5 #2	yogesh	7/22/2025 10:13:48 AM	mohammad	7/23/2025 1:33:05	Peak Integrated by Software
AR1660CCC500	PO112346.D	AR-1260-3 #2	yogesh	7/22/2025 10:13:48 AM	mohammad	7/23/2025 1:33:05	Peak Integrated by Software
AR1660CCC500	PO112346.D	AR-1260-4 #2	yogesh	7/22/2025 10:13:48 AM	mohammad	7/23/2025 1:33:05	Peak Integrated by Software
AR1242CCC500	PO112347.D	AR-1242-1 #2	yogesh	7/22/2025 10:13:50 AM	mohammad	7/23/2025 1:33:05	Peak Integrated by Software
AR1242CCC500	PO112347.D	AR-1242-5	yogesh	7/22/2025 10:13:50 AM	mohammad	7/23/2025 1:33:05	Peak Integrated by Software
AR1248CCC500	PO112348.D	AR-1248-1 #2	yogesh	7/22/2025 12:08:17 PM	mohammad	7/23/2025 1:33:05	Peak Integrated by Software
AR1660CCC500	PO112360.D	AR-1016-1 #2	yogesh	7/22/2025 10:14:17 AM	mohammad	7/23/2025 1:33:05	Peak Integrated by Software
AR1660CCC500	PO112360.D	AR-1016-2 #2	yogesh	7/22/2025 10:14:17 AM	mohammad	7/23/2025 1:33:05	Peak Integrated by Software
AR1660CCC500	PO112360.D	AR-1016-3 #2	yogesh	7/22/2025 10:14:17 AM	mohammad	7/23/2025 1:33:05	Peak Integrated by Software
AR1660CCC500	PO112360.D	AR-1016-4 #2	yogesh	7/22/2025 10:14:17 AM	mohammad	7/23/2025 1:33:05	Peak Integrated by Software
AR1660CCC500	PO112360.D	AR-1016-5 #2	yogesh	7/22/2025 10:14:17 AM	mohammad	7/23/2025 1:33:05	Peak Integrated by Software
AR1660CCC500	PO112360.D	AR-1260-3 #2	yogesh	7/22/2025 10:14:17 AM	mohammad	7/23/2025 1:33:05	Peak Integrated by Software
AR1660CCC500	PO112360.D	AR-1260-4 #2	yogesh	7/22/2025 10:14:17 AM	mohammad	7/23/2025 1:33:05	Peak Integrated by Software

1
2
3
4
5
6
7
8
9
10
11
12
13
14
15
16
17
18
19
20

Manual Integration Report

Sequence:	po072125	Instrument	ECD_o
-----------	----------	------------	-------

Sample ID	File ID	Parameter	Review By	Review On	Supervised By	Supervised On	Reason
AR1660CCC500	PO112360.D	Tetrachloro-m-xylene #2	yogesh	7/22/2025 10:14:17 AM	mohammad	7/23/2025 1:33:05	Peak Integrated by Software
AR1242CCC500	PO112361.D	AR-1242-1 #2	yogesh	7/22/2025 10:14:19 AM	mohammad	7/23/2025 1:33:05	Peak Integrated by Software

1
2
3
4
5
6
7
8
9
10
11
12
13
14
15
16
17
18
19
20

Manual Integration Report

Sequence:	po072225	Instrument	ECD_o
-----------	----------	------------	-------

Sample ID	File ID	Parameter	Review By	Review On	Supervised By	Supervised On	Reason
AR1660CCC500	PO112366.D	AR-1016-1 #2	yogesh	7/23/2025 8:14:01 AM	mohammad	7/24/2025 1:25:37	Peak Integrated by Software
AR1660CCC500	PO112366.D	AR-1016-2 #2	yogesh	7/23/2025 8:14:01 AM	mohammad	7/24/2025 1:25:37	Peak Integrated by Software
AR1660CCC500	PO112366.D	AR-1016-3 #2	yogesh	7/23/2025 8:14:01 AM	mohammad	7/24/2025 1:25:37	Peak Integrated by Software
AR1660CCC500	PO112366.D	AR-1016-4 #2	yogesh	7/23/2025 8:14:01 AM	mohammad	7/24/2025 1:25:37	Peak Integrated by Software
AR1660CCC500	PO112366.D	AR-1016-5 #2	yogesh	7/23/2025 8:14:01 AM	mohammad	7/24/2025 1:25:37	Peak Integrated by Software
AR1660CCC500	PO112366.D	AR-1260-3 #2	yogesh	7/23/2025 8:14:01 AM	mohammad	7/24/2025 1:25:37	Peak Integrated by Software
AR1660CCC500	PO112366.D	AR-1260-4 #2	yogesh	7/23/2025 8:14:01 AM	mohammad	7/24/2025 1:25:37	Peak Integrated by Software
AR1660CCC500	PO112366.D	Decachlorobiphenyl #2	yogesh	7/23/2025 8:14:01 AM	mohammad	7/24/2025 1:25:37	Peak Integrated by Software
AR1242CCC500	PO112367.D	AR-1242-1 #2	yogesh	7/23/2025 8:13:46 AM	mohammad	7/24/2025 1:25:37	Peak Integrated by Software
AR1248CCC500	PO112368.D	AR-1248-1 #2	yogesh	7/23/2025 8:13:48 AM	mohammad	7/24/2025 1:25:37	Peak Integrated by Software
AR1254CCC500	PO112369.D	AR-1254-1	yogesh	7/23/2025 8:13:49 AM	mohammad	7/24/2025 1:25:37	Peak Integrated by Software
Q2639-11	PO112373.D	Decachlorobiphenyl #2	yogesh	7/23/2025 11:47:24 AM	mohammad	7/24/2025 1:25:37	Peak Integrated by Software
AR1660CCC500	PO112381.D	AR-1016-1 #2	yogesh	7/23/2025 8:32:27 AM	mohammad	7/24/2025 1:25:37	Peak Integrated by Software

 1
2
3
4
5
6
7
8
9
10
11
12
13
14
15
16
17
18
19
20

Manual Integration Report

Sequence:	po072225	Instrument	ECD_o
-----------	----------	------------	-------

Sample ID	File ID	Parameter	Review By	Review On	Supervised By	Supervised On	Reason
AR1660CCC500	PO112381.D	AR-1016-2 #2	yogesh	7/23/2025 8:32:27 AM	mohammad	7/24/2025 1:25:37	Peak Integrated by Software
AR1660CCC500	PO112381.D	AR-1016-3 #2	yogesh	7/23/2025 8:32:27 AM	mohammad	7/24/2025 1:25:37	Peak Integrated by Software
AR1660CCC500	PO112381.D	AR-1016-4 #2	yogesh	7/23/2025 8:32:27 AM	mohammad	7/24/2025 1:25:37	Peak Integrated by Software
AR1660CCC500	PO112381.D	AR-1016-5 #2	yogesh	7/23/2025 8:32:27 AM	mohammad	7/24/2025 1:25:37	Peak Integrated by Software
AR1660CCC500	PO112381.D	AR-1260-3 #2	yogesh	7/23/2025 8:32:27 AM	mohammad	7/24/2025 1:25:37	Peak Integrated by Software
AR1660CCC500	PO112381.D	AR-1260-4 #2	yogesh	7/23/2025 8:32:27 AM	mohammad	7/24/2025 1:25:37	Peak Integrated by Software
AR1242CCC500	PO112382.D	AR-1242-1 #2	yogesh	7/23/2025 11:47:18 AM	mohammad	7/24/2025 1:25:37	Peak Integrated by Software
AR1242CCC500	PO112382.D	AR-1242-2 #2	yogesh	7/23/2025 11:47:18 AM	mohammad	7/24/2025 1:25:37	Peak Integrated by Software
AR1248CCC500	PO112383.D	AR-1248-1 #2	yogesh	7/23/2025 11:47:16 AM	mohammad	7/24/2025 1:25:37	Peak Integrated by Software
AR1254CCC500	PO112384.D	AR-1254-1	yogesh	7/23/2025 11:47:14 AM	mohammad	7/24/2025 1:25:37	Peak Integrated by Software
AR1254CCC500	PO112384.D	AR-1254-4	yogesh	7/23/2025 11:47:14 AM	mohammad	7/24/2025 1:25:37	Peak Integrated by Software
AR1660CCC500	PO112396.D	AR-1016-1 #2	yogesh	7/23/2025 8:32:38 AM	mohammad	7/24/2025 1:25:37	Peak Integrated by Software
AR1660CCC500	PO112396.D	AR-1016-2 #2	yogesh	7/23/2025 8:32:38 AM	mohammad	7/24/2025 1:25:37	Peak Integrated by Software

1
2
3
4
5
6
7
8
9
10
11
12
13
14
15
16
17
18
19
20

Manual Integration Report

Sequence:	po072225	Instrument	ECD_o
-----------	----------	------------	-------

Sample ID	File ID	Parameter	Review By	Review On	Supervised By	Supervised On	Reason
AR1660CCC500	PO112396.D	AR-1016-3 #2	yogesh	7/23/2025 8:32:38 AM	mohammad	7/24/2025 1:25:37	Peak Integrated by Software
AR1660CCC500	PO112396.D	AR-1016-4 #2	yogesh	7/23/2025 8:32:38 AM	mohammad	7/24/2025 1:25:37	Peak Integrated by Software
AR1660CCC500	PO112396.D	AR-1016-5 #2	yogesh	7/23/2025 8:32:38 AM	mohammad	7/24/2025 1:25:37	Peak Integrated by Software
AR1660CCC500	PO112396.D	AR-1260-3 #2	yogesh	7/23/2025 8:32:38 AM	mohammad	7/24/2025 1:25:37	Peak Integrated by Software
AR1660CCC500	PO112396.D	AR-1260-4 #2	yogesh	7/23/2025 8:32:38 AM	mohammad	7/24/2025 1:25:37	Peak Integrated by Software
AR1242CCC500	PO112397.D	AR-1242-1 #2	yogesh	7/23/2025 11:46:19 AM	mohammad	7/24/2025 1:25:37	Peak Integrated by Software
AR1242CCC500	PO112397.D	AR-1242-2 #2	yogesh	7/23/2025 11:46:19 AM	mohammad	7/24/2025 1:25:37	Peak Integrated by Software
AR1242CCC500	PO112397.D	AR-1242-5	yogesh	7/23/2025 11:46:19 AM	mohammad	7/24/2025 1:25:37	Peak Integrated by Software
AR1242CCC500	PO112397.D	Tetrachloro-m-xylene	yogesh	7/23/2025 11:46:19 AM	mohammad	7/24/2025 1:25:37	Peak Integrated by Software
AR1248CCC500	PO112398.D	AR-1248-1 #2	yogesh	7/23/2025 11:46:18 AM	mohammad	7/24/2025 1:25:37	Peak Integrated by Software
AR1254CCC500	PO112399.D	AR-1254-1	yogesh	7/23/2025 8:32:44 AM	mohammad	7/24/2025 1:25:37	Peak Integrated by Software
AR1254CCC500	PO112399.D	AR-1254-2	yogesh	7/23/2025 8:32:44 AM	mohammad	7/24/2025 1:25:37	Peak Integrated by Software
I.BLK	PO112400.D	Decachlorobiphenyl #2	yogesh	7/23/2025 8:32:46 AM	mohammad	7/24/2025 1:25:37	Peak Integrated by Software

 1
 2
 3
 4
 5
 6
 7
 8
 9
 10
 11
 12
 13
 14
 15
 16
 17
 18
 19
 20

Manual Integration Report

Sequence:	po072225	Instrument	ECD_o
-----------	----------	------------	-------

Sample ID	File ID	Parameter	Review By	Review On	Supervised By	Supervised On	Reason
AR1660CCC500	PO112410.D	AR-1016-1 #2	yogesh	7/23/2025 8:33:07 AM	mohammad	7/24/2025 1:25:37	Peak Integrated by Software
AR1660CCC500	PO112410.D	AR-1016-2 #2	yogesh	7/23/2025 8:33:07 AM	mohammad	7/24/2025 1:25:37	Peak Integrated by Software
AR1660CCC500	PO112410.D	AR-1016-3 #2	yogesh	7/23/2025 8:33:07 AM	mohammad	7/24/2025 1:25:37	Peak Integrated by Software
AR1660CCC500	PO112410.D	AR-1016-4 #2	yogesh	7/23/2025 8:33:07 AM	mohammad	7/24/2025 1:25:37	Peak Integrated by Software
AR1660CCC500	PO112410.D	AR-1016-5	yogesh	7/23/2025 8:33:07 AM	mohammad	7/24/2025 1:25:37	Peak Integrated by Software
AR1660CCC500	PO112410.D	AR-1016-5 #2	yogesh	7/23/2025 8:33:07 AM	mohammad	7/24/2025 1:25:37	Peak Integrated by Software
AR1660CCC500	PO112410.D	AR-1260-1 #2	yogesh	7/23/2025 8:33:07 AM	mohammad	7/24/2025 1:25:37	Peak Integrated by Software
AR1660CCC500	PO112410.D	AR-1260-2 #2	yogesh	7/23/2025 8:33:07 AM	mohammad	7/24/2025 1:25:37	Peak Integrated by Software
AR1660CCC500	PO112410.D	AR-1260-3 #2	yogesh	7/23/2025 8:33:07 AM	mohammad	7/24/2025 1:25:37	Peak Integrated by Software
AR1660CCC500	PO112410.D	AR-1260-4 #2	yogesh	7/23/2025 8:33:07 AM	mohammad	7/24/2025 1:25:37	Peak Integrated by Software
I.BLK	PO112411.D	Decachlorobiphenyl #2	yogesh	7/23/2025 8:33:10 AM	mohammad	7/24/2025 1:25:37	Peak Integrated by Software

1
2
3
4
5
6
7
8
9
10
11
12
13
14
15
16
17
18
19
20

Manual Integration Report

Sequence:	pp070825	Instrument	ECD_p
-----------	----------	------------	-------

Sample ID	File ID	Parameter	Review By	Review On	Supervised By	Supervised On	Reason
AR1660ICC250	PP073557.D	AR-1260-4 #2	yogesh	7/8/2025 8:51:16 AM	mohammad	7/9/2025 1:51:14	Peak Integrated by Software
AR1660ICC250	PP073557.D	AR-1260-5 #2	yogesh	7/8/2025 8:51:16 AM	mohammad	7/9/2025 1:51:14	Peak Integrated by Software
AR1660ICC050	PP073558.D	AR-1016-1	yogesh	7/8/2025 8:51:18 AM	mohammad	7/9/2025 1:51:14	Peak Integrated by Software
AR1660ICC050	PP073558.D	AR-1260-1 #2	yogesh	7/8/2025 8:51:18 AM	mohammad	7/9/2025 1:51:14	Peak Integrated by Software
AR1660ICC050	PP073558.D	AR-1260-4 #2	yogesh	7/8/2025 8:51:18 AM	mohammad	7/9/2025 1:51:14	Peak Integrated by Software
AR1660ICC050	PP073558.D	AR-1260-5 #2	yogesh	7/8/2025 8:51:18 AM	mohammad	7/9/2025 1:51:14	Peak Integrated by Software
AR1242ICC050	PP073565.D	AR-1242-1	yogesh	7/8/2025 8:51:20 AM	mohammad	7/9/2025 1:51:14	Peak Integrated by Software
AR1242ICC050	PP073565.D	AR-1242-2	yogesh	7/8/2025 8:51:20 AM	mohammad	7/9/2025 1:51:14	Peak Integrated by Software
AR1242ICC050	PP073565.D	AR-1242-3	yogesh	7/8/2025 8:51:20 AM	mohammad	7/9/2025 1:51:14	Peak Integrated by Software
AR1242ICC050	PP073565.D	AR-1242-5	yogesh	7/8/2025 8:51:20 AM	mohammad	7/9/2025 1:51:14	Peak Integrated by Software
AR1248ICC050	PP073570.D	AR-1248-1	yogesh	7/8/2025 8:51:21 AM	mohammad	7/9/2025 1:51:14	Peak Integrated by Software
AR1248ICC050	PP073570.D	AR-1248-4	yogesh	7/8/2025 8:51:21 AM	mohammad	7/9/2025 1:51:14	Peak Integrated by Software
AR1248ICC050	PP073570.D	AR-1248-5	yogesh	7/8/2025 8:51:21 AM	mohammad	7/9/2025 1:51:14	Peak Integrated by Software

1
2
3
4
5
6
7
8
9
10
11
12
13
14
15
16
17
18
19
20

Manual Integration Report

Sequence:	pp070825	Instrument	ECD_p
-----------	----------	------------	-------

Sample ID	File ID	Parameter	Review By	Review On	Supervised By	Supervised On	Reason
AR1254ICC050	PP073575.D	AR-1254-1	yogesh	7/8/2025 8:51:23 AM	mohammad	7/9/2025 1:51:14	Peak Integrated by Software
AR1254ICC050	PP073575.D	AR-1254-2	yogesh	7/8/2025 8:51:23 AM	mohammad	7/9/2025 1:51:14	Peak Integrated by Software
AR1254ICC050	PP073575.D	AR-1254-3	yogesh	7/8/2025 8:51:23 AM	mohammad	7/9/2025 1:51:14	Peak Integrated by Software
AR1254ICC050	PP073575.D	AR-1254-4	yogesh	7/8/2025 8:51:23 AM	mohammad	7/9/2025 1:51:14	Peak Integrated by Software
AR1268ICC250	PP073580.D	AR-1268-1 #2	yogesh	7/8/2025 8:51:24 AM	mohammad	7/9/2025 1:51:14	Peak Integrated by Software
AR1268ICC050	PP073581.D	AR-1268-5	yogesh	7/8/2025 8:51:26 AM	mohammad	7/9/2025 1:51:14	Peak Integrated by Software

1
2
3
4
5
6
7
8
9
10
11
12
13
14
15
16
17
18
19
20

Manual Integration Report

Sequence:	pp072125	Instrument	ECD_p
-----------	----------	------------	-------

Sample ID	File ID	Parameter	Review By	Review On	Supervised By	Supervised On	Reason
Q2635-01MS	PP073984.D	Tetrachloro-m-xylene	yogesh	7/22/2025 12:09:26 PM	mohammad	7/23/2025 1:32:53	Peak Integrated by Software
Q2635-01MSD	PP073985.D	AR-1254-1	yogesh	7/22/2025 8:25:03 AM	mohammad	7/23/2025 1:32:53	Peak Integrated by Software
Q2635-01MSD	PP073985.D	AR-1260-1	yogesh	7/22/2025 8:25:03 AM	mohammad	7/23/2025 1:32:53	Peak Integrated by Software
Q2635-01MSD	PP073985.D	AR-1260-2	yogesh	7/22/2025 8:25:03 AM	mohammad	7/23/2025 1:32:53	Peak Integrated by Software
Q2635-01MSD	PP073985.D	AR-1260-4	yogesh	7/22/2025 8:25:03 AM	mohammad	7/23/2025 1:32:53	Peak Integrated by Software
Q2639-01	PP074001.D	AR-1254-1	yogesh	7/22/2025 12:09:28 PM	mohammad	7/23/2025 1:32:53	Peak Integrated by Software
Q2639-01	PP074001.D	AR-1254-1 #2	yogesh	7/22/2025 12:09:28 PM	mohammad	7/23/2025 1:32:53	Peak Integrated by Software
Q2639-01	PP074001.D	AR-1254-2	yogesh	7/22/2025 12:09:28 PM	mohammad	7/23/2025 1:32:53	Peak Integrated by Software
Q2639-01	PP074001.D	AR-1254-2 #2	yogesh	7/22/2025 12:09:28 PM	mohammad	7/23/2025 1:32:53	Peak Integrated by Software
Q2639-01	PP074001.D	AR-1254-3	yogesh	7/22/2025 12:09:28 PM	mohammad	7/23/2025 1:32:53	Peak Integrated by Software
Q2639-01	PP074001.D	AR-1254-3 #2	yogesh	7/22/2025 12:09:28 PM	mohammad	7/23/2025 1:32:53	Peak Integrated by Software
Q2639-01	PP074001.D	AR-1254-4	yogesh	7/22/2025 12:09:28 PM	mohammad	7/23/2025 1:32:53	Peak Integrated by Software
Q2639-01	PP074001.D	AR-1254-4 #2	yogesh	7/22/2025 12:09:28 PM	mohammad	7/23/2025 1:32:53	Peak Integrated by Software

1
2
3
4
5
6
7
8
9
10
11
12
13
14
15
16
17
18
19
20

Manual Integration Report

Sequence:	pp072125	Instrument	ECD_p
-----------	----------	------------	-------

Sample ID	File ID	Parameter	Review By	Review On	Supervised By	Supervised On	Reason
AR1248CCC500	PP074004.D	AR-1248-3	yogesh	7/22/2025 12:09:29 PM	mohammad	7/23/2025 1:32:53	Peak Integrated by Software
AR1660CCC500	PP074017.D	AR-1260-2	yogesh	7/22/2025 8:25:17 AM	mohammad	7/23/2025 1:32:53	Peak Integrated by Software
AR1242CCC500	PP074018.D	Decachlorobiphenyl #2	yogesh	7/22/2025 12:09:32 PM	mohammad	7/23/2025 1:32:53	Peak Integrated by Software

1
2
3
4
5
6
7
8
9
10
11
12
13
14
15
16
17
18
19
20

Instrument ID: ECD_O

Daily Analysis Runlog For Sequence/QCBatch ID # PO070825

Review By	yogesh	Review On	7/8/2025 1:10:21 PM
Supervise By	mohammad	Supervise On	7/10/2025 2:03:44 AM
SubDirectory	PO070825	HP Acquire Method	HP Processing Method PO070825
STD. NAME	STD REF.#		
Tune/Reschk			
Initial Calibration Stds	PP24330,PP24331,PP24332,PP24333,PP24334,PP24335,PP24336,PP24337,PP24338,PP24339,PP24340,PP24341,PP24342,PP24343,PP24344 ,PP24345,PP24346,PP24347,PP24348,PP24349,PP24350,PP24351,PP24352,PP24353,PP24354,PP24355,PP24356,PP24357,PP24358,PP2435 9,PP24360,PP24361,PP24362,PP24363,PP24364,PP24365,PP24366,PP24367,PP24368,PP24369		
CCC			
Internal Standard/PEM			
ICV/I.BLK	PP24370,PP24371,PP24372,PP24373,PP24374,PP24375,PP24376,PP24377,PP24378,PP24379,PP24380,PP24381,PP24382,PP24384,PP24385,PP24386,PP2		
Surrogate Standard			
MS/MSD Standard			
LCS Standard			

Sr#	SampleId	Data File Name	Date-Time	Operator	Status
1	HEXANE	PO112086.D	08 Jul 2025 13:32	YP/AJ	Ok
2	I.BLK	PO112087.D	08 Jul 2025 13:49	YP/AJ	Ok
3	AR1660ICC1000	PO112088.D	08 Jul 2025 14:06	YP/AJ	Ok,M
4	AR1660ICC750	PO112089.D	08 Jul 2025 14:25	YP/AJ	Ok,M
5	AR1660ICC500	PO112090.D	08 Jul 2025 14:43	YP/AJ	Ok
6	AR1660ICC250	PO112091.D	08 Jul 2025 15:02	YP/AJ	Ok,M
7	AR1660ICC050	PO112092.D	08 Jul 2025 15:21	YP/AJ	Ok,M
8	AR1221ICC500	PO112093.D	08 Jul 2025 15:38	YP/AJ	Ok
9	AR1232ICC500	PO112094.D	08 Jul 2025 15:57	YP/AJ	Ok
10	AR1242ICC1000	PO112095.D	08 Jul 2025 16:15	YP/AJ	Ok
11	AR1242ICC750	PO112096.D	08 Jul 2025 16:34	YP/AJ	Ok
12	AR1242ICC500	PO112097.D	08 Jul 2025 16:52	YP/AJ	Ok
13	AR1242ICC250	PO112098.D	08 Jul 2025 17:11	YP/AJ	Ok
14	AR1242ICC050	PO112099.D	08 Jul 2025 17:29	YP/AJ	Ok,M
15	AR1248ICC1000	PO112100.D	08 Jul 2025 17:48	YP/AJ	Ok
16	AR1248ICC750	PO112101.D	08 Jul 2025 18:05	YP/AJ	Ok
17	AR1248ICC500	PO112102.D	08 Jul 2025 18:24	YP/AJ	Ok
18	AR1248ICC250	PO112103.D	08 Jul 2025 18:41	YP/AJ	Ok
19	AR1248ICC050	PO112104.D	08 Jul 2025 18:59	YP/AJ	Ok,M
20	AR1254ICC1000	PO112105.D	08 Jul 2025 19:18	YP/AJ	Ok
21	AR1254ICC750	PO112106.D	08 Jul 2025 19:35	YP/AJ	Ok

Instrument ID: ECD_O

Daily Analysis Runlog For Sequence/QCBatch ID # PO070825

Review By	yogesh	Review On	7/8/2025 1:10:21 PM
Supervise By	mohammad	Supervise On	7/10/2025 2:03:44 AM
SubDirectory	PO070825	HP Acquire Method	HP Processing Method PO070825
STD. NAME	STD REF.#		
Tune/Reschk			
Initial Calibration Stds	PP24330,PP24331,PP24332,PP24333,PP24334,PP24335,PP24336,PP24337,PP24338,PP24339,PP24340,PP24341,PP24342,PP24343,PP24344,PP24345,PP24346,PP24347,PP24348,PP24349,PP24350,PP24351,PP24352,PP24353,PP24354,PP24355,PP24356,PP24357,PP24358,PP24359,PP24360,PP24361,PP24362,PP24363,PP24364,PP24365,PP24366,PP24367,PP24368,PP24369		
CCC Internal Standard/PEM ICV/I.BLK Surrogate Standard MS/MSD Standard LCS Standard	PP24370,PP24371,PP24372,PP24373,PP24374,PP24375,PP24376,PP24377,PP24378,PP24379,PP24380,PP24381,PP24382,PP24384,PP24385,PP24386,PP24387		

22	AR1254ICC500	PO112107.D	08 Jul 2025 19:54	YP/AJ	Ok
23	AR1254ICC250	PO112108.D	08 Jul 2025 20:11	YP/AJ	Ok
24	AR1254ICC050	PO112109.D	08 Jul 2025 20:28	YP/AJ	Ok,M
25	AR1262ICC500	PO112110.D	08 Jul 2025 20:47	YP/AJ	Ok
26	AR1268ICC1000	PO112111.D	08 Jul 2025 21:04	YP/AJ	Ok,M
27	AR1268ICC750	PO112112.D	08 Jul 2025 21:22	YP/AJ	Ok
28	AR1268ICC500	PO112113.D	08 Jul 2025 21:39	YP/AJ	Ok
29	AR1268ICC250	PO112114.D	08 Jul 2025 21:57	YP/AJ	Ok
30	AR1268ICC050	PO112115.D	08 Jul 2025 22:16	YP/AJ	Ok,M
31	PO070825ICV500	PO112116.D	08 Jul 2025 22:34	YP/AJ	Ok,M
32	AR1242ICV500	PO112117.D	08 Jul 2025 23:11	YP/AJ	Ok
33	AR1248ICV500	PO112118.D	08 Jul 2025 23:47	YP/AJ	Ok
34	AR1254ICV500	PO112119.D	09 Jul 2025 00:24	YP/AJ	Ok
35	AR1268ICV500	PO112120.D	09 Jul 2025 01:01	YP/AJ	Ok

M : Manual Integration

Instrument ID: ECD_O

Daily Analysis Runlog For Sequence/QCBatch ID # PO072125

Review By	yogesh	Review On	7/21/2025 1:01:47 PM
Supervise By	mohammad	Supervise On	7/23/2025 1:33:05 AM
SubDirectory	PO072125	HP Acquire Method	HP Processing Method PO070825
STD. NAME	STD REF.#		
Tune/Reschk Initial Calibration Stds CCC Internal Standard/PEM ICV/I.BLK Surrogate Standard MS/MSD Standard LCS Standard	PP24330,PP24331,PP24332,PP24333,PP24334,PP24335,PP24336,PP24337,PP24338,PP24339,PP24340,PP24341,PP24342,PP24343,PP24344 ,PP24345,PP24346,PP24347,PP24348,PP24349,PP24350,PP24351,PP24352,PP24353,PP24354,PP24355,PP24356,PP24357,PP24358,PP2435 9,PP24360,PP24361,PP24362,PP24363,PP24364,PP24365,PP24366,PP24367,PP24368,PP24369 PP24332,PP24347,PP24352,PP24357 PP24370,PP24371,PP24372,PP24373,PP24374,PP24375,PP24376,PP24377,PP24378,PP24379,PP24380,PP24381,PP24382,PP24384,PP24385,PP24386,PP2		

Sr#	SampleId	Data File Name	Date-Time	Operator	Status
1	HEXANE	PO112331.D	21 Jul 2025 08:47	YP/AJ	Ok
2	AR1660CCC500	PO112332.D	21 Jul 2025 10:15	YP/AJ	Ok,M
3	AR1242CCC500	PO112333.D	21 Jul 2025 10:41	YP/AJ	Ok,M
4	AR1248CCC500	PO112334.D	21 Jul 2025 11:01	YP/AJ	Ok
5	AR1254CCC500	PO112335.D	21 Jul 2025 11:38	YP/AJ	Ok
6	I.BLK	PO112336.D	21 Jul 2025 12:34	YP/AJ	Ok
7	DDT ANALOG	PO112337.D	21 Jul 2025 12:53	YP/AJ	Ok
8	Q2639-03	PO112338.D	21 Jul 2025 13:11	YP/AJ	Ok
9	Q2639-05	PO112339.D	21 Jul 2025 13:30	YP/AJ	Ok
10	Q2639-07	PO112340.D	21 Jul 2025 13:47	YP/AJ	Ok
11	Q2639-09	PO112341.D	21 Jul 2025 14:06	YP/AJ	Not Ok
12	Q2639-11	PO112342.D	21 Jul 2025 14:24	YP/AJ	Not Ok
13	Q2639-13	PO112343.D	21 Jul 2025 14:41	YP/AJ	Not Ok
14	Q2641-01	PO112344.D	21 Jul 2025 14:59	YP/AJ	Ok,M
15	Q2645-02	PO112345.D	21 Jul 2025 15:16	YP/AJ	ReRun
16	AR1660CCC500	PO112346.D	21 Jul 2025 16:10	YP/AJ	Ok,M
17	AR1242CCC500	PO112347.D	21 Jul 2025 16:45	YP/AJ	Ok,M
18	AR1248CCC500	PO112348.D	21 Jul 2025 17:04	YP/AJ	Ok,M
19	AR1254CCC500	PO112349.D	21 Jul 2025 17:21	YP/AJ	Ok
20	I.BLK	PO112350.D	21 Jul 2025 17:38	YP/AJ	Ok
21	PB168943BL	PO112351.D	21 Jul 2025 19:42	YP/AJ	Ok

Instrument ID: ECD_O

Daily Analysis Runlog For Sequence/QCBatch ID # PO072125

Review By	yogesh	Review On	7/21/2025 1:01:47 PM		
Supervise By	mohammad	Supervise On	7/23/2025 1:33:05 AM		
SubDirectory	PO072125	HP Acquire Method		HP Processing Method	PO070825
STD. NAME	STD REF.#				
Tune/Reschk Initial Calibration Stds CCC Internal Standard/PEM ICV/I.BLK Surrogate Standard MS/MSD Standard LCS Standard	PP24330,PP24331,PP24332,PP24333,PP24334,PP24335,PP24336,PP24337,PP24338,PP24339,PP24340,PP24341,PP24342,PP24343,PP24344 ,PP24345,PP24346,PP24347,PP24348,PP24349,PP24350,PP24351,PP24352,PP24353,PP24354,PP24355,PP24356,PP24357,PP24358,PP2435 9,PP24360,PP24361,PP24362,PP24363,PP24364,PP24365,PP24366,PP24367,PP24368,PP24369 PP24332,PP24347,PP24352,PP24357 PP24370,PP24371,PP24372,PP24373,PP24374,PP24375,PP24376,PP24377,PP24378,PP24379,PP24380,PP24381,PP24382,PP24384,PP24385,PP24386,PP2				

22	PB168943BS	PO112352.D	21 Jul 2025 20:01	YP/AJ	Ok,M
23	Q2661-01	PO112353.D	21 Jul 2025 20:18	YP/AJ	Ok,M
24	Q2661-02	PO112354.D	21 Jul 2025 20:37	YP/AJ	Ok,M
25	Q2662-01	PO112355.D	21 Jul 2025 20:55	YP/AJ	Ok,M
26	Q2663-01	PO112356.D	21 Jul 2025 21:13	YP/AJ	Ok,M
27	Q2663-02	PO112357.D	21 Jul 2025 21:31	YP/AJ	Ok,M
28	Q2663-03	PO112358.D	21 Jul 2025 21:49	YP/AJ	Ok,M
29	Q2663-04	PO112359.D	21 Jul 2025 22:07	YP/AJ	Ok,M
30	AR1660CCC500	PO112360.D	21 Jul 2025 23:21	YP/AJ	Ok,M
31	AR1242CCC500	PO112361.D	22 Jul 2025 00:16	YP/AJ	Not Ok
32	AR1248CCC500	PO112362.D	22 Jul 2025 00:34	YP/AJ	Ok
33	AR1254CCC500	PO112363.D	22 Jul 2025 00:52	YP/AJ	Ok
34	I.BLK	PO112364.D	22 Jul 2025 01:10	YP/AJ	Ok

M : Manual Integration

Instrument ID: ECD_O

Daily Analysis Runlog For Sequence/QCBatch ID # PO072225

Review By	yogesh	Review On	7/22/2025 12:28:05 PM
Supervise By	mohammad	Supervise On	7/24/2025 1:25:37 AM
SubDirectory	PO072225	HP Acquire Method	HP Processing Method PO070825
STD. NAME	STD REF.#		
Tune/Reschk Initial Calibration Stds CCC Internal Standard/PEM ICV/I.BLK Surrogate Standard MS/MSD Standard LCS Standard	PP24330,PP24331,PP24332,PP24333,PP24334,PP24335,PP24336,PP24337,PP24338,PP24339,PP24340,PP24341,PP24342,PP24343,PP24344 ,PP24345,PP24346,PP24347,PP24348,PP24349,PP24350,PP24351,PP24352,PP24353,PP24354,PP24355,PP24356,PP24357,PP24358,PP2435 9,PP24360,PP24361,PP24362,PP24363,PP24364,PP24365,PP24366,PP24367,PP24368,PP24369 PP24332,PP24347,PP24352,PP24357 PP24370,PP24371,PP24372,PP24373,PP24374,PP24375,PP24376,PP24377,PP24378,PP24379,PP24380,PP24381,PP24382,PP24384,PP24385,PP24386,PP2		

Sr#	SampleId	Data File Name	Date-Time	Operator	Status
1	HEXANE	PO112365.D	22 Jul 2025 08:18	YP/AJ	Ok
2	AR1660CCC500	PO112366.D	22 Jul 2025 08:57	YP/AJ	Ok,M
3	AR1242CCC500	PO112367.D	22 Jul 2025 09:15	YP/AJ	Ok,M
4	AR1248CCC500	PO112368.D	22 Jul 2025 09:32	YP/AJ	Ok,M
5	AR1254CCC500	PO112369.D	22 Jul 2025 09:49	YP/AJ	Ok,M
6	I.BLK	PO112370.D	22 Jul 2025 10:08	YP/AJ	Ok
7	DDT ANALOG	PO112371.D	22 Jul 2025 10:26	YP/AJ	Ok
8	Q2639-09	PO112372.D	22 Jul 2025 11:08	YP/AJ	Ok
9	Q2639-11	PO112373.D	22 Jul 2025 11:26	YP/AJ	Ok,M
10	Q2639-13	PO112374.D	22 Jul 2025 11:44	YP/AJ	Ok
11	PB168946BL	PO112375.D	22 Jul 2025 13:35	YP/AJ	Ok
12	PB168946BS	PO112376.D	22 Jul 2025 13:53	YP/AJ	Ok,M
13	Q2645-02RX	PO112377.D	22 Jul 2025 14:12	YP/AJ	Confirms
14	Q2649-01	PO112378.D	22 Jul 2025 14:30	YP/AJ	Ok
15	Q2649-01MS	PO112379.D	22 Jul 2025 14:48	YP/AJ	Ok,M
16	Q2649-01MSD	PO112380.D	22 Jul 2025 15:07	YP/AJ	Ok,M
17	AR1660CCC500	PO112381.D	22 Jul 2025 16:21	YP/AJ	Ok,M
18	AR1242CCC500	PO112382.D	22 Jul 2025 16:39	YP/AJ	Ok,M
19	AR1248CCC500	PO112383.D	22 Jul 2025 16:56	YP/AJ	Ok,M
20	AR1254CCC500	PO112384.D	22 Jul 2025 17:14	YP/AJ	Ok,M
21	I.BLK	PO112385.D	22 Jul 2025 17:32	YP/AJ	Ok

Instrument ID: ECD_O

Daily Analysis Runlog For Sequence/QCBatch ID # PO072225

Review By	yogesh	Review On	7/22/2025 12:28:05 PM		
Supervise By	mohammad	Supervise On	7/24/2025 1:25:37 AM		
SubDirectory	PO072225	HP Acquire Method		HP Processing Method	PO070825
STD. NAME	STD REF.#				
Tune/Reschk Initial Calibration Stds CCC Internal Standard/PEM ICV/I.BLK Surrogate Standard MS/MSD Standard LCS Standard	PP24330,PP24331,PP24332,PP24333,PP24334,PP24335,PP24336,PP24337,PP24338,PP24339,PP24340,PP24341,PP24342,PP24343,PP24344 ,PP24345,PP24346,PP24347,PP24348,PP24349,PP24350,PP24351,PP24352,PP24353,PP24354,PP24355,PP24356,PP24357,PP24358,PP2435 9,PP24360,PP24361,PP24362,PP24363,PP24364,PP24365,PP24366,PP24367,PP24368,PP24369 PP24332,PP24347,PP24352,PP24357 PP24370,PP24371,PP24372,PP24373,PP24374,PP24375,PP24376,PP24377,PP24378,PP24379,PP24380,PP24381,PP24382,PP24384,PP24385,PP24386,PP2				

22	Q2670-01	PO112386.D	22 Jul 2025 17:49	YP/AJ	Ok,M
23	Q2670-02	PO112387.D	22 Jul 2025 18:08	YP/AJ	Ok,M
24	Q2670-03	PO112388.D	22 Jul 2025 18:25	YP/AJ	Ok,M
25	Q2670-04	PO112389.D	22 Jul 2025 18:44	YP/AJ	Ok,M
26	Q2670-05	PO112390.D	22 Jul 2025 19:02	YP/AJ	Ok,M
27	Q2670-06	PO112391.D	22 Jul 2025 19:20	YP/AJ	Ok,M
28	Q2670-07	PO112392.D	22 Jul 2025 19:39	YP/AJ	Ok,M
29	Q2670-08	PO112393.D	22 Jul 2025 19:57	YP/AJ	Ok,M
30	PB168958BL	PO112394.D	22 Jul 2025 20:34	YP/AJ	Ok,M
31	PB168958BS	PO112395.D	22 Jul 2025 20:52	YP/AJ	Ok,M
32	AR1660CCC500	PO112396.D	22 Jul 2025 22:05	YP/AJ	Ok,M
33	AR1242CCC500	PO112397.D	22 Jul 2025 23:00	YP/AJ	Ok,M
34	AR1248CCC500	PO112398.D	22 Jul 2025 23:18	YP/AJ	Ok,M
35	AR1254CCC500	PO112399.D	22 Jul 2025 23:37	YP/AJ	Ok,M
36	I.BLK	PO112400.D	22 Jul 2025 23:55	YP/AJ	Ok,M
37	PB168957BL	PO112401.D	23 Jul 2025 00:14	YP/AJ	Ok,M
38	PB168957BS	PO112402.D	23 Jul 2025 00:32	YP/AJ	Ok,M
39	PB168957BSD	PO112403.D	23 Jul 2025 00:50	YP/AJ	Ok,M
40	Q2640-01	PO112404.D	23 Jul 2025 01:09	YP/AJ	Ok,M
41	Q2646-01	PO112405.D	23 Jul 2025 01:27	YP/AJ	Ok,M
42	Q2655-03	PO112406.D	23 Jul 2025 01:46	YP/AJ	Ok,M
43	Q2655-04	PO112407.D	23 Jul 2025 02:04	YP/AJ	Ok
44	Q2657-01	PO112408.D	23 Jul 2025 02:22	YP/AJ	Ok,M

Instrument ID: ECD_O

Daily Analysis Runlog For Sequence/QCBatch ID # PO072225

Review By	yogesh	Review On	7/22/2025 12:28:05 PM
Supervise By	mohammad	Supervise On	7/24/2025 1:25:37 AM
SubDirectory	PO072225	HP Acquire Method	HP Processing Method PO070825
STD. NAME	STD REF.#		
Tune/Reschk			
Initial Calibration Stds	PP24330,PP24331,PP24332,PP24333,PP24334,PP24335,PP24336,PP24337,PP24338,PP24339,PP24340,PP24341,PP24342,PP24343,PP24344,PP24345,PP24346,PP24347,PP24348,PP24349,PP24350,PP24351,PP24352,PP24353,PP24354,PP24355,PP24356,PP24357,PP24358,PP24359,PP24360,PP24361,PP24362,PP24363,PP24364,PP24365,PP24366,PP24367,PP24368,PP24369		
CCC	PP24332,PP24347,PP24352,PP24357		
Internal Standard/PEM			
ICV/I.BLK	PP24370,PP24371,PP24372,PP24373,PP24374,PP24375,PP24376,PP24377,PP24378,PP24379,PP24380,PP24381,PP24382,PP24384,PP24385,PP24386,PP2		
Surrogate Standard			
MS/MSD Standard			
LCS Standard			

45	Q2660-05	PO112409.D	23 Jul 2025 02:41	YP/AJ	Ok,M
46	AR1660CCC500	PO112410.D	23 Jul 2025 04:12	YP/AJ	Ok,M
47	I.BLK	PO112411.D	23 Jul 2025 05:43	YP/AJ	Ok,M

M : Manual Integration

Instrument ID: ECD_P

Daily Analysis Runlog For Sequence/QCBatch ID # PP070825

Review By	yogesh	Review On	7/7/2025 4:17:13 PM
Supervise By	mohammad	Supervise On	7/9/2025 1:51:14 AM
SubDirectory	PP070825	HP Acquire Method	HP Processing Method PP070825
STD. NAME	STD REF.#		
Tune/Reschk Initial Calibration Stds CCC Internal Standard/PEM ICV/I.BLK Surrogate Standard MS/MSD Standard LCS Standard	PP24330,PP24331,PP24332,PP24333,PP24334,PP24335,PP24336,PP24337,PP24338,PP24339,PP24340,PP24341,PP24342,PP24343,PP24344 ,PP24345,PP24346,PP24347,PP24348,PP24349,PP24350,PP24351,PP24352,PP24353,PP24354,PP24355,PP24356,PP24357,PP24358,PP2435 9,PP24360,PP24361,PP24362,PP24363,PP24364,PP24365,PP24366,PP24367,PP24368,PP24369 PP24370,PP24371,PP24372,PP24373,PP24374,PP24375,PP24376,PP24377,PP24378,PP24379,PP24380,PP24381,PP24382,PP24384,PP24385,PP24386,PP2		

Sr#	SampleId	Data File Name	Date-Time	Operator	Status
1	HEXANE	PP073552.D	07 Jul 2025 20:13	YP\AJ	Ok
2	I.BLK	PP073553.D	07 Jul 2025 20:30	YP\AJ	Ok
3	AR1660ICC1000	PP073554.D	07 Jul 2025 21:03	YP\AJ	Ok
4	AR1660ICC750	PP073555.D	07 Jul 2025 21:19	YP\AJ	Ok
5	AR1660ICC500	PP073556.D	07 Jul 2025 21:35	YP\AJ	Ok
6	AR1660ICC250	PP073557.D	07 Jul 2025 21:52	YP\AJ	Ok,M
7	AR1660ICC050	PP073558.D	07 Jul 2025 22:08	YP\AJ	Ok,M
8	AR1221ICC500	PP073559.D	07 Jul 2025 22:24	YP\AJ	Ok
9	AR1232ICC500	PP073560.D	07 Jul 2025 22:41	YP\AJ	Ok
10	AR1242ICC1000	PP073561.D	07 Jul 2025 22:57	YP\AJ	Ok
11	AR1242ICC750	PP073562.D	07 Jul 2025 23:14	YP\AJ	Ok
12	AR1242ICC500	PP073563.D	07 Jul 2025 23:30	YP\AJ	Ok
13	AR1242ICC250	PP073564.D	07 Jul 2025 23:46	YP\AJ	Ok
14	AR1242ICC050	PP073565.D	08 Jul 2025 00:03	YP\AJ	Ok,M
15	AR1248ICC1000	PP073566.D	08 Jul 2025 00:19	YP\AJ	Ok
16	AR1248ICC750	PP073567.D	08 Jul 2025 00:35	YP\AJ	Ok
17	AR1248ICC500	PP073568.D	08 Jul 2025 00:52	YP\AJ	Ok
18	AR1248ICC250	PP073569.D	08 Jul 2025 01:08	YP\AJ	Ok
19	AR1248ICC050	PP073570.D	08 Jul 2025 01:25	YP\AJ	Ok,M
20	AR1254ICC1000	PP073571.D	08 Jul 2025 01:41	YP\AJ	Ok
21	AR1254ICC750	PP073572.D	08 Jul 2025 01:57	YP\AJ	Ok

Instrument ID: ECD_P

Daily Analysis Runlog For Sequence/QCBatch ID # PP070825

Review By	yogesh	Review On	7/7/2025 4:17:13 PM		
Supervise By	mohammad	Supervise On	7/9/2025 1:51:14 AM		
SubDirectory	PP070825	HP Acquire Method		HP Processing Method	PP070825
STD. NAME	STD REF.#				
Tune/Reschk					
Initial Calibration Stds	PP24330,PP24331,PP24332,PP24333,PP24334,PP24335,PP24336,PP24337,PP24338,PP24339,PP24340,PP24341,PP24342,PP24343,PP24344,PP24345,PP24346,PP24347,PP24348,PP24349,PP24350,PP24351,PP24352,PP24353,PP24354,PP24355,PP24356,PP24357,PP24358,PP24359,PP24360,PP24361,PP24362,PP24363,PP24364,PP24365,PP24366,PP24367,PP24368,PP24369				
CCC Internal Standard/PEM ICV/I.BLK Surrogate Standard MS/MSD Standard LCS Standard	PP24370,PP24371,PP24372,PP24373,PP24374,PP24375,PP24376,PP24377,PP24378,PP24379,PP24380,PP24381,PP24382,PP24384,PP24385,PP24386,PP24387				

22	AR1254ICC500	PP073573.D	08 Jul 2025 02:14	YP\AJ	Ok
23	AR1254ICC250	PP073574.D	08 Jul 2025 02:30	YP\AJ	Ok
24	AR1254ICC050	PP073575.D	08 Jul 2025 02:46	YP\AJ	Ok,M
25	AR1262ICC500	PP073576.D	08 Jul 2025 03:03	YP\AJ	Ok
26	AR1268ICC1000	PP073577.D	08 Jul 2025 03:19	YP\AJ	Ok
27	AR1268ICC750	PP073578.D	08 Jul 2025 03:35	YP\AJ	Ok
28	AR1268ICC500	PP073579.D	08 Jul 2025 03:52	YP\AJ	Ok
29	AR1268ICC250	PP073580.D	08 Jul 2025 04:08	YP\AJ	Ok,M
30	AR1268ICC050	PP073581.D	08 Jul 2025 04:24	YP\AJ	Ok,M
31	PP070825ICV500	PP073582.D	08 Jul 2025 04:41	YP\AJ	Ok
32	AR1242ICV500	PP073583.D	08 Jul 2025 05:30	YP\AJ	Ok
33	AR1248ICV500	PP073584.D	08 Jul 2025 05:46	YP\AJ	Ok
34	AR1254ICV500	PP073585.D	08 Jul 2025 06:19	YP\AJ	Ok
35	AR1268ICV500	PP073586.D	08 Jul 2025 06:52	YP\AJ	Ok
36	DDT ANALOGUE	PP073587.D	08 Jul 2025 07:24	YP\AJ	Ok

M : Manual Integration

Instrument ID: ECD_P

Daily Analysis Runlog For Sequence/QCBatch ID # PP072125

Review By	yogesh	Review On	7/21/2025 11:07:59 AM
Supervise By	mohammad	Supervise On	7/23/2025 1:32:53 AM
SubDirectory	PP072125	HP Acquire Method	HP Processing Method PP070825
STD. NAME	STD REF.#		
Tune/Reschk			
Initial Calibration Stds	PP24330,PP24331,PP24332,PP24333,PP24334,PP24335,PP24336,PP24337,PP24338,PP24339,PP24340,PP24341,PP24342,PP24343,PP24344,PP24345,PP24346,PP24347,PP24348,PP24349,PP24350,PP24351,PP24352,PP24353,PP24354,PP24355,PP24356,PP24357,PP24358,PP24359,PP24360,PP24361,PP24362,PP24363,PP24364,PP24365,PP24366,PP24367,PP24368,PP24369		
CCC	PP24332,PP24347,PP24352,PP24357		
Internal Standard/PEM			
ICV/I.BLK	PP24370,PP24371,PP24372,PP24373,PP24374,PP24375,PP24376,PP24377,PP24378,PP24379,PP24380,PP24381,PP24382,PP24384,PP24385,PP24386,PP2		
Surrogate Standard			
MS/MSD Standard			
LCS Standard			

Sr#	SampleId	Data File Name	Date-Time	Operator	Status
1	HEXANE	PP073971.D	21 Jul 2025 08:35	YP\AJ	Ok
2	AR1660CCC500	PP073972.D	21 Jul 2025 08:51	YP\AJ	Ok
3	AR1242CCC500	PP073973.D	21 Jul 2025 09:08	YP\AJ	Ok
4	AR1248CCC500	PP073974.D	21 Jul 2025 09:24	YP\AJ	Ok
5	AR1254CCC500	PP073975.D	21 Jul 2025 09:40	YP\AJ	Ok
6	I.BLK	PP073976.D	21 Jul 2025 09:56	YP\AJ	Ok
7	DDT ANALOG	PP073977.D	21 Jul 2025 10:13	YP\AJ	Ok
8	PB168911BS	PP073978.D	21 Jul 2025 10:46	YP\AJ	Ok
9	PB168911BSD	PP073979.D	21 Jul 2025 11:05	YP\AJ	Ok
10	Q2610-01DL	PP073980.D	21 Jul 2025 11:21	YP\AJ	Ok,M
11	Q2610-03DL	PP073981.D	21 Jul 2025 11:37	YP\AJ	Ok,M
12	Q2610-05DL	PP073982.D	21 Jul 2025 13:07	YP\AJ	Ok,M
13	Q2635-01	PP073983.D	21 Jul 2025 13:24	YP\AJ	Ok,M
14	Q2635-01MS	PP073984.D	21 Jul 2025 13:40	YP\AJ	Ok,M
15	Q2635-01MSD	PP073985.D	21 Jul 2025 13:56	YP\AJ	Ok,M
16	Q2634-01	PP073986.D	21 Jul 2025 14:13	YP\AJ	Ok,M
17	AR1660CCC500	PP073987.D	21 Jul 2025 15:18	YP\AJ	Ok
18	AR1242CCC500	PP073988.D	21 Jul 2025 15:34	YP\AJ	Ok
19	AR1248CCC500	PP073989.D	21 Jul 2025 15:50	YP\AJ	Ok
20	AR1254CCC500	PP073990.D	21 Jul 2025 16:07	YP\AJ	Ok
21	I.BLK	PP073991.D	21 Jul 2025 16:23	YP\AJ	Ok

Instrument ID: ECD_P

Daily Analysis Runlog For Sequence/QCBatch ID # PP072125

Review By	yogesh	Review On	7/21/2025 11:07:59 AM		
Supervise By	mohammad	Supervise On	7/23/2025 1:32:53 AM		
SubDirectory	PP072125	HP Acquire Method		HP Processing Method	PP070825
STD. NAME	STD REF.#				
Tune/Reschk Initial Calibration Stds	PP24330,PP24331,PP24332,PP24333,PP24334,PP24335,PP24336,PP24337,PP24338,PP24339,PP24340,PP24341,PP24342,PP24343,PP24344 ,PP24345,PP24346,PP24347,PP24348,PP24349,PP24350,PP24351,PP24352,PP24353,PP24354,PP24355,PP24356,PP24357,PP24358,PP2435 9,PP24360,PP24361,PP24362,PP24363,PP24364,PP24365,PP24366,PP24367,PP24368,PP24369				
CCC Internal Standard/PEM ICV/I.BLK Surrogate Standard MS/MSD Standard LCS Standard	PP24332,PP24347,PP24352,PP24357 PP24370,PP24371,PP24372,PP24373,PP24374,PP24375,PP24376,PP24377,PP24378,PP24379,PP24380,PP24381,PP24382,PP24384,PP24385,PP24386,PP2				

22	PB168927BL	PP073992.D	21 Jul 2025 16:39	YP\AJ	Ok
23	PB168927BS	PP073993.D	21 Jul 2025 16:56	YP\AJ	Ok
24	Q2638-01	PP073994.D	21 Jul 2025 17:12	YP\AJ	ReRun
25	Q2638-03	PP073995.D	21 Jul 2025 17:29	YP\AJ	ReRun
26	Q2638-05	PP073996.D	21 Jul 2025 17:45	YP\AJ	Ok
27	Q2638-07	PP073997.D	21 Jul 2025 18:01	YP\AJ	ReRun
28	Q2638-09	PP073998.D	21 Jul 2025 18:18	YP\AJ	Ok
29	Q2638-11	PP073999.D	21 Jul 2025 18:34	YP\AJ	Ok
30	Q2638-13	PP074000.D	21 Jul 2025 18:50	YP\AJ	Ok
31	Q2639-01	PP074001.D	21 Jul 2025 19:07	YP\AJ	Ok,M
32	AR1660CCC500	PP074002.D	21 Jul 2025 20:12	YP\AJ	Ok
33	AR1242CCC500	PP074003.D	21 Jul 2025 20:45	YP\AJ	Ok
34	AR1248CCC500	PP074004.D	21 Jul 2025 21:01	YP\AJ	Ok,M
35	AR1254CCC500	PP074005.D	21 Jul 2025 21:17	YP\AJ	Ok
36	I.BLK	PP074006.D	21 Jul 2025 21:34	YP\AJ	Ok
37	Q2663-05	PP074007.D	21 Jul 2025 21:50	YP\AJ	Ok
38	Q2663-06	PP074008.D	21 Jul 2025 22:06	YP\AJ	Ok
39	Q2663-07	PP074009.D	21 Jul 2025 22:23	YP\AJ	Ok,M
40	Q2663-08	PP074010.D	21 Jul 2025 22:39	YP\AJ	Ok
41	Q2663-09	PP074011.D	21 Jul 2025 22:55	YP\AJ	Ok,M
42	Q2663-10	PP074012.D	21 Jul 2025 23:11	YP\AJ	Ok
43	Q2663-11	PP074013.D	21 Jul 2025 23:28	YP\AJ	Ok,M
44	Q2663-12	PP074014.D	21 Jul 2025 23:44	YP\AJ	Ok,M

Instrument ID: ECD_P

Daily Analysis Runlog For Sequence/QCBatch ID # PP072125

Review By	yogesh	Review On	7/21/2025 11:07:59 AM
Supervise By	mohammad	Supervise On	7/23/2025 1:32:53 AM
SubDirectory	PP072125	HP Acquire Method	HP Processing Method PP070825
STD. NAME	STD REF.#		
Tune/Reschk Initial Calibration Stds CCC Internal Standard/PEM ICV/I.BLK Surrogate Standard MS/MSD Standard LCS Standard	PP24330,PP24331,PP24332,PP24333,PP24334,PP24335,PP24336,PP24337,PP24338,PP24339,PP24340,PP24341,PP24342,PP24343,PP24344 ,PP24345,PP24346,PP24347,PP24348,PP24349,PP24350,PP24351,PP24352,PP24353,PP24354,PP24355,PP24356,PP24357,PP24358,PP2435 9,PP24360,PP24361,PP24362,PP24363,PP24364,PP24365,PP24366,PP24367,PP24368,PP24369 PP24332,PP24347,PP24352,PP24357 PP24370,PP24371,PP24372,PP24373,PP24374,PP24375,PP24376,PP24377,PP24378,PP24379,PP24380,PP24381,PP24382,PP24384,PP24385,PP24386,PP2		

45	Q2663-13	PP074015.D	22 Jul 2025 00:00	YP\AJ	Not Ok
46	Q2663-14	PP074016.D	22 Jul 2025 00:17	YP\AJ	Ok,M
47	AR1660CCC500	PP074017.D	22 Jul 2025 01:38	YP\AJ	Ok,M
48	AR1242CCC500	PP074018.D	22 Jul 2025 01:55	YP\AJ	Ok,M
49	AR1248CCC500	PP074019.D	22 Jul 2025 02:11	YP\AJ	Ok
50	AR1254CCC500	PP074020.D	22 Jul 2025 02:27	YP\AJ	Ok
51	I.BLK	PP074021.D	22 Jul 2025 02:44	YP\AJ	Ok

M : Manual Integration

Instrument ID: ECD_O

Daily Analysis Runlog For Sequence/QCBatch ID # PO070825

Review By	yogesh	Review On	7/8/2025 1:10:21 PM
Supervise By	mohammad	Supervise On	7/10/2025 2:03:44 AM
SubDirectory	PO070825	HP Acquire Method	HP Processing Method PO070825
STD. NAME	STD REF.#		
Tune/Reschk Initial Calibration Stds CCC Internal Standard/PEM ICV/I.BLK Surrogate Standard MS/MSD Standard LCS Standard	PP24330,PP24331,PP24332,PP24333,PP24334,PP24335,PP24336,PP24337,PP24338,PP24339,PP24340,PP24341,PP24342,PP24343,PP24344,PP24345,PP24346,PP24347,PP24348,PP24349,PP24350,PP24351,PP24352,PP24353,PP24354,PP24355,PP24356,PP24357,PP24358,PP24359,PP24360,PP24361,PP24362,PP24363,PP24364,PP24365,PP24366,PP24367,PP24368,PP24369 PP24370,PP24371,PP24372,PP24373,PP24374,PP24375,PP24376,PP24377,PP24378,PP24379,PP24380,PP24381,PP24382,PP24384,PP24385,PP24386,PP24387		

Sr#	SampleId	ClientID	Data File Name	Date-Time	Comment	Operator	Status
1	HEXANE	HEXANE	PO112086.D	08 Jul 2025 13:32		YP/AJ	Ok
2	I.BLK	I.BLK	PO112087.D	08 Jul 2025 13:49		YP/AJ	Ok
3	AR1660ICC1000	AR1660ICC1000	PO112088.D	08 Jul 2025 14:06		YP/AJ	Ok,M
4	AR1660ICC750	AR1660ICC750	PO112089.D	08 Jul 2025 14:25		YP/AJ	Ok,M
5	AR1660ICC500	AR1660ICC500	PO112090.D	08 Jul 2025 14:43		YP/AJ	Ok
6	AR1660ICC250	AR1660ICC250	PO112091.D	08 Jul 2025 15:02		YP/AJ	Ok,M
7	AR1660ICC050	AR1660ICC050	PO112092.D	08 Jul 2025 15:21		YP/AJ	Ok,M
8	AR1221ICC500	AR1221ICC500	PO112093.D	08 Jul 2025 15:38		YP/AJ	Ok
9	AR1232ICC500	AR1232ICC500	PO112094.D	08 Jul 2025 15:57		YP/AJ	Ok
10	AR1242ICC1000	AR1242ICC1000	PO112095.D	08 Jul 2025 16:15		YP/AJ	Ok
11	AR1242ICC750	AR1242ICC750	PO112096.D	08 Jul 2025 16:34		YP/AJ	Ok
12	AR1242ICC500	AR1242ICC500	PO112097.D	08 Jul 2025 16:52		YP/AJ	Ok
13	AR1242ICC250	AR1242ICC250	PO112098.D	08 Jul 2025 17:11		YP/AJ	Ok
14	AR1242ICC050	AR1242ICC050	PO112099.D	08 Jul 2025 17:29		YP/AJ	Ok,M
15	AR1248ICC1000	AR1248ICC1000	PO112100.D	08 Jul 2025 17:48		YP/AJ	Ok
16	AR1248ICC750	AR1248ICC750	PO112101.D	08 Jul 2025 18:05		YP/AJ	Ok
17	AR1248ICC500	AR1248ICC500	PO112102.D	08 Jul 2025 18:24		YP/AJ	Ok
18	AR1248ICC250	AR1248ICC250	PO112103.D	08 Jul 2025 18:41		YP/AJ	Ok

Instrument ID: ECD_O

Daily Analysis Runlog For Sequence/QCBatch ID # PO070825

Review By	yogesh	Review On	7/8/2025 1:10:21 PM
Supervise By	mohammad	Supervise On	7/10/2025 2:03:44 AM
SubDirectory	PO070825	HP Acquire Method	HP Processing Method PO070825
STD. NAME	STD REF.#		
Tune/Reschk Initial Calibration Stds CCC Internal Standard/PEM ICV/I.BLK Surrogate Standard MS/MSD Standard LCS Standard	PP24330,PP24331,PP24332,PP24333,PP24334,PP24335,PP24336,PP24337,PP24338,PP24339,PP24340,PP24341,PP24342,PP24343,PP24344,PP24345,PP24346,PP24347,PP24348,PP24349,PP24350,PP24351,PP24352,PP24353,PP24354,PP24355,PP24356,PP24357,PP24358,PP24359,PP24360,PP24361,PP24362,PP24363,PP24364,PP24365,PP24366,PP24367,PP24368,PP24369 PP24370,PP24371,PP24372,PP24373,PP24374,PP24375,PP24376,PP24377,PP24378,PP24379,PP24380,PP24381,PP24382,PP24384,PP24385,PP24386,PP24387		

19	AR1248ICC050	AR1248ICC050	PO112104.D	08 Jul 2025 18:59		YP/AJ	Ok,M
20	AR1254ICC1000	AR1254ICC1000	PO112105.D	08 Jul 2025 19:18		YP/AJ	Ok
21	AR1254ICC750	AR1254ICC750	PO112106.D	08 Jul 2025 19:35		YP/AJ	Ok
22	AR1254ICC500	AR1254ICC500	PO112107.D	08 Jul 2025 19:54		YP/AJ	Ok
23	AR1254ICC250	AR1254ICC250	PO112108.D	08 Jul 2025 20:11		YP/AJ	Ok
24	AR1254ICC050	AR1254ICC050	PO112109.D	08 Jul 2025 20:28		YP/AJ	Ok,M
25	AR1262ICC500	AR1262ICC500	PO112110.D	08 Jul 2025 20:47		YP/AJ	Ok
26	AR1268ICC1000	AR1268ICC1000	PO112111.D	08 Jul 2025 21:04		YP/AJ	Ok,M
27	AR1268ICC750	AR1268ICC750	PO112112.D	08 Jul 2025 21:22		YP/AJ	Ok
28	AR1268ICC500	AR1268ICC500	PO112113.D	08 Jul 2025 21:39		YP/AJ	Ok
29	AR1268ICC250	AR1268ICC250	PO112114.D	08 Jul 2025 21:57		YP/AJ	Ok
30	AR1268ICC050	AR1268ICC050	PO112115.D	08 Jul 2025 22:16		YP/AJ	Ok,M
31	PO070825ICV500	ICVPO070825	PO112116.D	08 Jul 2025 22:34		YP/AJ	Ok,M
32	AR1242ICV500	ICVPO070825AR1242	PO112117.D	08 Jul 2025 23:11		YP/AJ	Ok
33	AR1248ICV500	ICVPO070825AR1248	PO112118.D	08 Jul 2025 23:47		YP/AJ	Ok
34	AR1254ICV500	ICVPO070825AR1254	PO112119.D	09 Jul 2025 00:24		YP/AJ	Ok
35	AR1268ICV500	ICVPO070825AR1268	PO112120.D	09 Jul 2025 01:01		YP/AJ	Ok

M : Manual Integration

Instrument ID: ECD_O

Daily Analysis Runlog For Sequence/QCBatch ID # PO072125

Review By	yogesh	Review On	7/21/2025 1:01:47 PM	
Supervise By	mohammad	Supervise On	7/23/2025 1:33:05 AM	
SubDirectory	PO072125	HP Acquire Method	HP Processing Method	PO070825
STD. NAME	STD REF.#			
Tune/Reschk Initial Calibration Stds	PP24330,PP24331,PP24332,PP24333,PP24334,PP24335,PP24336,PP24337,PP24338,PP24339,PP24340,PP24341,PP24342,PP24343,PP24344,PP24345,PP24346,PP24347,PP24348,PP24349,PP24350,PP24351,PP24352,PP24353,PP24354,PP24355,PP24356,PP24357,PP24358,PP24359,PP24360,PP24361,PP24362,PP24363,PP24364,PP24365,PP24366,PP24367,PP24368,PP24369			
CCC Internal Standard/PEM ICV/I.BLK Surrogate Standard MS/MSD Standard LCS Standard	PP24332,PP24347,PP24352,PP24357 PP24370,PP24371,PP24372,PP24373,PP24374,PP24375,PP24376,PP24377,PP24378,PP24379,PP24380,PP24381,PP24382,PP24384,PP24385,PP24386,PP24387			

Sr#	SampleId	ClientID	Data File Name	Date-Time	Comment	Operator	Status
1	HEXANE	HEXANE	PO112331.D	21 Jul 2025 08:47		YP/AJ	Ok
2	AR1660CCC500	AR1660CCC500	PO112332.D	21 Jul 2025 10:15		YP/AJ	Ok,M
3	AR1242CCC500	AR1242CCC500	PO112333.D	21 Jul 2025 10:41	TCMX high in first column	YP/AJ	Ok,M
4	AR1248CCC500	AR1248CCC500	PO112334.D	21 Jul 2025 11:01		YP/AJ	Ok
5	AR1254CCC500	AR1254CCC500	PO112335.D	21 Jul 2025 11:38		YP/AJ	Ok
6	I.BLK	I.BLK	PO112336.D	21 Jul 2025 12:34		YP/AJ	Ok
7	DDT ANALOG	DDT ANALOG	PO112337.D	21 Jul 2025 12:53		YP/AJ	Ok
8	Q2639-03	OU4-TS-39-071725	PO112338.D	21 Jul 2025 13:11		YP/AJ	Ok
9	Q2639-05	OU4-TS-40-071725	PO112339.D	21 Jul 2025 13:30		YP/AJ	Ok
10	Q2639-07	OU4-TS-41-071725	PO112340.D	21 Jul 2025 13:47		YP/AJ	Ok
11	Q2639-09	OU4-TS-42-071725	PO112341.D	21 Jul 2025 14:06	DCB Low in both column	YP/AJ	Not Ok
12	Q2639-11	OU4-TS-43-071725	PO112342.D	21 Jul 2025 14:24	DCB Low in both column	YP/AJ	Not Ok
13	Q2639-13	OU4-TS-44-071725	PO112343.D	21 Jul 2025 14:41	DCB Low in both column	YP/AJ	Not Ok
14	Q2641-01	P001-CONCRETE001-PO112344.D	PO112344.D	21 Jul 2025 14:59	AR1254+1260 Hit	YP/AJ	Ok,M
15	Q2645-02	RW5B-CARBON-20250	PO112345.D	21 Jul 2025 15:16	All Surrogate fail	YP/AJ	ReRun
16	AR1660CCC500	AR1660CCC500	PO112346.D	21 Jul 2025 16:10		YP/AJ	Ok,M
17	AR1242CCC500	AR1242CCC500	PO112347.D	21 Jul 2025 16:45		YP/AJ	Ok,M
18	AR1248CCC500	AR1248CCC500	PO112348.D	21 Jul 2025 17:04		YP/AJ	Ok,M

Instrument ID: ECD_O

Daily Analysis Runlog For Sequence/QCBatch ID # PO072125

Review By	yogesh	Review On	7/21/2025 1:01:47 PM
Supervise By	mohammad	Supervise On	7/23/2025 1:33:05 AM
SubDirectory	PO072125	HP Acquire Method	HP Processing Method PO070825
STD. NAME	STD REF.#		
Tune/Reschk Initial Calibration Stds CCC Internal Standard/PEM ICV/I.BLK Surrogate Standard MS/MSD Standard LCS Standard	PP24330,PP24331,PP24332,PP24333,PP24334,PP24335,PP24336,PP24337,PP24338,PP24339,PP24340,PP24341,PP24342,PP24343,PP24344,PP24345,PP24346,PP24347,PP24348,PP24349,PP24350,PP24351,PP24352,PP24353,PP24354,PP24355,PP24356,PP24357,PP24358,PP24359,PP24360,PP24361,PP24362,PP24363,PP24364,PP24365,PP24366,PP24367,PP24368,PP24369 PP24332,PP24347,PP24352,PP24357 PP24370,PP24371,PP24372,PP24373,PP24374,PP24375,PP24376,PP24377,PP24378,PP24379,PP24380,PP24381,PP24382,PP24384,PP24385,PP24386,PP24387		

19	AR1254CCC500	AR1254CCC500	PO112349.D	21 Jul 2025 17:21		YP/AJ	Ok
20	I.BLK	I.BLK	PO112350.D	21 Jul 2025 17:38		YP/AJ	Ok
21	PB168943BL	PB168943BL	PO112351.D	21 Jul 2025 19:42		YP/AJ	Ok
22	PB168943BS	PB168943BS	PO112352.D	21 Jul 2025 20:01		YP/AJ	Ok,M
23	Q2661-01	245F64-1-1	PO112353.D	21 Jul 2025 20:18		YP/AJ	Ok,M
24	Q2661-02	245F64-1-2	PO112354.D	21 Jul 2025 20:37		YP/AJ	Ok,M
25	Q2662-01	L10-A	PO112355.D	21 Jul 2025 20:55	AR1254 Hit	YP/AJ	Ok,M
26	Q2663-01	BC289086-1-1	PO112356.D	21 Jul 2025 21:13		YP/AJ	Ok,M
27	Q2663-02	BC289086-1-2	PO112357.D	21 Jul 2025 21:31		YP/AJ	Ok,M
28	Q2663-03	BC289086-2-1	PO112358.D	21 Jul 2025 21:49	AR1260 Hit	YP/AJ	Ok,M
29	Q2663-04	BC289086-2-2	PO112359.D	21 Jul 2025 22:07	AR1260 Hit	YP/AJ	Ok,M
30	AR1660CCC500	AR1660CCC500	PO112360.D	21 Jul 2025 23:21	DCB low in first column	YP/AJ	Ok,M
31	AR1242CCC500	AR1242CCC500	PO112361.D	22 Jul 2025 00:16	CCC fail on higher side	YP/AJ	Not Ok
32	AR1248CCC500	AR1248CCC500	PO112362.D	22 Jul 2025 00:34		YP/AJ	Ok
33	AR1254CCC500	AR1254CCC500	PO112363.D	22 Jul 2025 00:52	TCMX high in first column	YP/AJ	Ok
34	I.BLK	I.BLK	PO112364.D	22 Jul 2025 01:10		YP/AJ	Ok

M : Manual Integration

Instrument ID: ECD_O

Daily Analysis Runlog For Sequence/QCBatch ID # PO072225

Review By	yogesh	Review On	7/22/2025 12:28:05 PM
Supervise By	mohammad	Supervise On	7/24/2025 1:25:37 AM
SubDirectory	PO072225	HP Acquire Method	HP Processing Method PO070825
STD. NAME	STD REF.#		
Tune/Reschk Initial Calibration Stds	PP24330,PP24331,PP24332,PP24333,PP24334,PP24335,PP24336,PP24337,PP24338,PP24339,PP24340,PP24341,PP24342,PP24343,PP24344,PP24345,PP24346,PP24347,PP24348,PP24349,PP24350,PP24351,PP24352,PP24353,PP24354,PP24355,PP24356,PP24357,PP24358,PP24359,PP24360,PP24361,PP24362,PP24363,PP24364,PP24365,PP24366,PP24367,PP24368,PP24369		
CCC Internal Standard/PEM ICV/I.BLK Surrogate Standard MS/MSD Standard LCS Standard	PP24332,PP24347,PP24352,PP24357 PP24370,PP24371,PP24372,PP24373,PP24374,PP24375,PP24376,PP24377,PP24378,PP24379,PP24380,PP24381,PP24382,PP24384,PP24385,PP24386,PP24387		

Sr#	SampleId	ClientID	Data File Name	Date-Time	Comment	Operator	Status
1	HEXANE	HEXANE	PO112365.D	22 Jul 2025 08:18		YP/AJ	Ok
2	AR1660CCC500	AR1660CCC500	PO112366.D	22 Jul 2025 08:57		YP/AJ	Ok,M
3	AR1242CCC500	AR1242CCC500	PO112367.D	22 Jul 2025 09:15		YP/AJ	Ok,M
4	AR1248CCC500	AR1248CCC500	PO112368.D	22 Jul 2025 09:32		YP/AJ	Ok,M
5	AR1254CCC500	AR1254CCC500	PO112369.D	22 Jul 2025 09:49		YP/AJ	Ok,M
6	I.BLK	I.BLK	PO112370.D	22 Jul 2025 10:08		YP/AJ	Ok
7	DDT ANALOG	DDT ANALOG	PO112371.D	22 Jul 2025 10:26		YP/AJ	Ok
8	Q2639-09	OU4-TS-42-071725	PO112372.D	22 Jul 2025 11:08		YP/AJ	Ok
9	Q2639-11	OU4-TS-43-071725	PO112373.D	22 Jul 2025 11:26		YP/AJ	Ok,M
10	Q2639-13	OU4-TS-44-071725	PO112374.D	22 Jul 2025 11:44		YP/AJ	Ok
11	PB168946BL	PB168946BL	PO112375.D	22 Jul 2025 13:35		YP/AJ	Ok
12	PB168946BS	PB168946BS	PO112376.D	22 Jul 2025 13:53		YP/AJ	Ok,M
13	Q2645-02RX	RW5B-CARBON-20250	PO112377.D	22 Jul 2025 14:12	TCMX having F Flag in 2nd column, all surrogate fail	YP/AJ	Confirms
14	Q2649-01	WC-1	PO112378.D	22 Jul 2025 14:30		YP/AJ	Ok
15	Q2649-01MS	WC-1MS	PO112379.D	22 Jul 2025 14:48		YP/AJ	Ok,M
16	Q2649-01MSD	WC-1MSD	PO112380.D	22 Jul 2025 15:07	RPD Fail	YP/AJ	Ok,M
17	AR1660CCC500	AR1660CCC500	PO112381.D	22 Jul 2025 16:21		YP/AJ	Ok,M

Instrument ID: ECD_O

Daily Analysis Runlog For Sequence/QCBatch ID # PO072225

Review By	yogesh	Review On	7/22/2025 12:28:05 PM
Supervise By	mohammad	Supervise On	7/24/2025 1:25:37 AM
SubDirectory	PO072225	HP Acquire Method	HP Processing Method PO070825
STD. NAME	STD REF.#		
Tune/Reschk Initial Calibration Stds CCC Internal Standard/PEM ICV/I.BLK Surrogate Standard MS/MSD Standard LCS Standard	PP24330,PP24331,PP24332,PP24333,PP24334,PP24335,PP24336,PP24337,PP24338,PP24339,PP24340,PP24341,PP24342,PP24343,PP24344,PP24345,PP24346,PP24347,PP24348,PP24349,PP24350,PP24351,PP24352,PP24353,PP24354,PP24355,PP24356,PP24357,PP24358,PP24359,PP24360,PP24361,PP24362,PP24363,PP24364,PP24365,PP24366,PP24367,PP24368,PP24369 PP24332,PP24347,PP24352,PP24357 PP24370,PP24371,PP24372,PP24373,PP24374,PP24375,PP24376,PP24377,PP24378,PP24379,PP24380,PP24381,PP24382,PP24384,PP24385,PP24386,PP24387		

18	AR1242CCC500	AR1242CCC500	PO112382.D	22 Jul 2025 16:39		YP/AJ	Ok,M
19	AR1248CCC500	AR1248CCC500	PO112383.D	22 Jul 2025 16:56		YP/AJ	Ok,M
20	AR1254CCC500	AR1254CCC500	PO112384.D	22 Jul 2025 17:14		YP/AJ	Ok,M
21	I.BLK	I.BLK	PO112385.D	22 Jul 2025 17:32		YP/AJ	Ok
22	Q2670-01	RBR251375-1	PO112386.D	22 Jul 2025 17:49	AR1248 Hit	YP/AJ	Ok,M
23	Q2670-02	RBR251375-2	PO112387.D	22 Jul 2025 18:08	AR1248 Hit	YP/AJ	Ok,M
24	Q2670-03	72-11995-1	PO112388.D	22 Jul 2025 18:25	AR1248 Hit	YP/AJ	Ok,M
25	Q2670-04	72-11995-2	PO112389.D	22 Jul 2025 18:44	AR1248 Hit	YP/AJ	Ok,M
26	Q2670-05	72-12000-1	PO112390.D	22 Jul 2025 19:02	AR1248 Hit	YP/AJ	Ok,M
27	Q2670-06	72-12000-2	PO112391.D	22 Jul 2025 19:20	AR1248 Hit	YP/AJ	Ok,M
28	Q2670-07	72-11991-1	PO112392.D	22 Jul 2025 19:39	AR1248 Hit	YP/AJ	Ok,M
29	Q2670-08	72-11991-2	PO112393.D	22 Jul 2025 19:57	AR1248 Hit	YP/AJ	Ok,M
30	PB168958BL	PB168958BL	PO112394.D	22 Jul 2025 20:34		YP/AJ	Ok,M
31	PB168958BS	PB168958BS	PO112395.D	22 Jul 2025 20:52		YP/AJ	Ok,M
32	AR1660CCC500	AR1660CCC500	PO112396.D	22 Jul 2025 22:05		YP/AJ	Ok,M
33	AR1242CCC500	AR1242CCC500	PO112397.D	22 Jul 2025 23:00		YP/AJ	Ok,M
34	AR1248CCC500	AR1248CCC500	PO112398.D	22 Jul 2025 23:18		YP/AJ	Ok,M
35	AR1254CCC500	AR1254CCC500	PO112399.D	22 Jul 2025 23:37		YP/AJ	Ok,M
36	I.BLK	I.BLK	PO112400.D	22 Jul 2025 23:55		YP/AJ	Ok,M

Instrument ID: ECD_O

Daily Analysis Runlog For Sequence/QCBatch ID # PO072225

Review By	yogesh	Review On	7/22/2025 12:28:05 PM
Supervise By	mohammad	Supervise On	7/24/2025 1:25:37 AM
SubDirectory	PO072225	HP Acquire Method	HP Processing Method PO070825
STD. NAME	STD REF.#		
Tune/Reschk Initial Calibration Stds CCC Internal Standard/PEM ICV/I.BLK Surrogate Standard MS/MSD Standard LCS Standard	PP24330,PP24331,PP24332,PP24333,PP24334,PP24335,PP24336,PP24337,PP24338,PP24339,PP24340,PP24341,PP24342,PP24343,PP24344,PP24345,PP24346,PP24347,PP24348,PP24349,PP24350,PP24351,PP24352,PP24353,PP24354,PP24355,PP24356,PP24357,PP24358,PP24359,PP24360,PP24361,PP24362,PP24363,PP24364,PP24365,PP24366,PP24367,PP24368,PP24369 PP24332,PP24347,PP24352,PP24357 PP24370,PP24371,PP24372,PP24373,PP24374,PP24375,PP24376,PP24377,PP24378,PP24379,PP24380,PP24381,PP24382,PP24384,PP24385,PP24386,PP24387		

37	PB168957BL	PB168957BL	PO112401.D	23 Jul 2025 00:14		YP/AJ	Ok,M
38	PB168957BS	PB168957BS	PO112402.D	23 Jul 2025 00:32		YP/AJ	Ok,M
39	PB168957BSD	PB168957BSD	PO112403.D	23 Jul 2025 00:50		YP/AJ	Ok,M
40	Q2640-01	ELMORA-WATER	PO112404.D	23 Jul 2025 01:09		YP/AJ	Ok,M
41	Q2646-01	FRAC TANK	PO112405.D	23 Jul 2025 01:27		YP/AJ	Ok,M
42	Q2655-03	71125	PO112406.D	23 Jul 2025 01:46		YP/AJ	Ok,M
43	Q2655-04	71425	PO112407.D	23 Jul 2025 02:04		YP/AJ	Ok
44	Q2657-01	12825-A	PO112408.D	23 Jul 2025 02:22		YP/AJ	Ok,M
45	Q2660-05	MOO-25-0220	PO112409.D	23 Jul 2025 02:41		YP/AJ	Ok,M
46	AR1660CCC500	AR1660CCC500	PO112410.D	23 Jul 2025 04:12	DCB low in both column	YP/AJ	Ok,M
47	I.BLK	I.BLK	PO112411.D	23 Jul 2025 05:43		YP/AJ	Ok,M

M : Manual Integration

Instrument ID: ECD_P

Daily Analysis Runlog For Sequence/QCBatch ID # PP070825

Review By	yogesh	Review On	7/7/2025 4:17:13 PM
Supervise By	mohammad	Supervise On	7/9/2025 1:51:14 AM
SubDirectory	PP070825	HP Acquire Method	HP Processing Method PP070825
STD. NAME	STD REF.#		
Tune/Reschk Initial Calibration Stds CCC Internal Standard/PEM ICV/I.BLK Surrogate Standard MS/MSD Standard LCS Standard	PP24330,PP24331,PP24332,PP24333,PP24334,PP24335,PP24336,PP24337,PP24338,PP24339,PP24340,PP24341,PP24342,PP24343,PP24344,PP24345,PP24346,PP24347,PP24348,PP24349,PP24350,PP24351,PP24352,PP24353,PP24354,PP24355,PP24356,PP24357,PP24358,PP24359,PP24360,PP24361,PP24362,PP24363,PP24364,PP24365,PP24366,PP24367,PP24368,PP24369 PP24370,PP24371,PP24372,PP24373,PP24374,PP24375,PP24376,PP24377,PP24378,PP24379,PP24380,PP24381,PP24382,PP24384,PP24385,PP24386,PP24387		

Sr#	SampleId	ClientID	Data File Name	Date-Time	Comment	Operator	Status
1	HEXANE	HEXANE	PP073552.D	07 Jul 2025 20:13		YPAJ	Ok
2	I.BLK	I.BLK	PP073553.D	07 Jul 2025 20:30		YPAJ	Ok
3	AR1660ICC1000	AR1660ICC1000	PP073554.D	07 Jul 2025 21:03		YPAJ	Ok
4	AR1660ICC750	AR1660ICC750	PP073555.D	07 Jul 2025 21:19		YPAJ	Ok
5	AR1660ICC500	AR1660ICC500	PP073556.D	07 Jul 2025 21:35		YPAJ	Ok
6	AR1660ICC250	AR1660ICC250	PP073557.D	07 Jul 2025 21:52		YPAJ	Ok,M
7	AR1660ICC050	AR1660ICC050	PP073558.D	07 Jul 2025 22:08		YPAJ	Ok,M
8	AR1221ICC500	AR1221ICC500	PP073559.D	07 Jul 2025 22:24		YPAJ	Ok
9	AR1232ICC500	AR1232ICC500	PP073560.D	07 Jul 2025 22:41		YPAJ	Ok
10	AR1242ICC1000	AR1242ICC1000	PP073561.D	07 Jul 2025 22:57		YPAJ	Ok
11	AR1242ICC750	AR1242ICC750	PP073562.D	07 Jul 2025 23:14		YPAJ	Ok
12	AR1242ICC500	AR1242ICC500	PP073563.D	07 Jul 2025 23:30		YPAJ	Ok
13	AR1242ICC250	AR1242ICC250	PP073564.D	07 Jul 2025 23:46		YPAJ	Ok
14	AR1242ICC050	AR1242ICC050	PP073565.D	08 Jul 2025 00:03		YPAJ	Ok,M
15	AR1248ICC1000	AR1248ICC1000	PP073566.D	08 Jul 2025 00:19		YPAJ	Ok
16	AR1248ICC750	AR1248ICC750	PP073567.D	08 Jul 2025 00:35		YPAJ	Ok
17	AR1248ICC500	AR1248ICC500	PP073568.D	08 Jul 2025 00:52		YPAJ	Ok
18	AR1248ICC250	AR1248ICC250	PP073569.D	08 Jul 2025 01:08		YPAJ	Ok

Instrument ID: ECD_P

Daily Analysis Runlog For Sequence/QCBatch ID # PP070825

Review By	yogesh	Review On	7/7/2025 4:17:13 PM
Supervise By	mohammad	Supervise On	7/9/2025 1:51:14 AM
SubDirectory	PP070825	HP Acquire Method	HP Processing Method PP070825
STD. NAME	STD REF.#		
Tune/Reschk Initial Calibration Stds CCC Internal Standard/PEM ICV/I.BLK Surrogate Standard MS/MSD Standard LCS Standard	PP24330,PP24331,PP24332,PP24333,PP24334,PP24335,PP24336,PP24337,PP24338,PP24339,PP24340,PP24341,PP24342,PP24343,PP24344,PP24345,PP24346,PP24347,PP24348,PP24349,PP24350,PP24351,PP24352,PP24353,PP24354,PP24355,PP24356,PP24357,PP24358,PP24359,PP24360,PP24361,PP24362,PP24363,PP24364,PP24365,PP24366,PP24367,PP24368,PP24369 PP24370,PP24371,PP24372,PP24373,PP24374,PP24375,PP24376,PP24377,PP24378,PP24379,PP24380,PP24381,PP24382,PP24384,PP24385,PP24386,PP24387		

19	AR1248ICC050	AR1248ICC050	PP073570.D	08 Jul 2025 01:25		YPAJ	Ok,M
20	AR1254ICC1000	AR1254ICC1000	PP073571.D	08 Jul 2025 01:41		YPAJ	Ok
21	AR1254ICC750	AR1254ICC750	PP073572.D	08 Jul 2025 01:57		YPAJ	Ok
22	AR1254ICC500	AR1254ICC500	PP073573.D	08 Jul 2025 02:14		YPAJ	Ok
23	AR1254ICC250	AR1254ICC250	PP073574.D	08 Jul 2025 02:30		YPAJ	Ok
24	AR1254ICC050	AR1254ICC050	PP073575.D	08 Jul 2025 02:46		YPAJ	Ok,M
25	AR1262ICC500	AR1262ICC500	PP073576.D	08 Jul 2025 03:03		YPAJ	Ok
26	AR1268ICC1000	AR1268ICC1000	PP073577.D	08 Jul 2025 03:19		YPAJ	Ok
27	AR1268ICC750	AR1268ICC750	PP073578.D	08 Jul 2025 03:35		YPAJ	Ok
28	AR1268ICC500	AR1268ICC500	PP073579.D	08 Jul 2025 03:52		YPAJ	Ok
29	AR1268ICC250	AR1268ICC250	PP073580.D	08 Jul 2025 04:08		YPAJ	Ok,M
30	AR1268ICC050	AR1268ICC050	PP073581.D	08 Jul 2025 04:24		YPAJ	Ok,M
31	PP070825ICV500	ICVPP070825	PP073582.D	08 Jul 2025 04:41		YPAJ	Ok
32	AR1242ICV500	ICVPP070825AR1242	PP073583.D	08 Jul 2025 05:30		YPAJ	Ok
33	AR1248ICV500	ICVPP070825AR1248	PP073584.D	08 Jul 2025 05:46		YPAJ	Ok
34	AR1254ICV500	ICVPP070825AR1254	PP073585.D	08 Jul 2025 06:19		YPAJ	Ok
35	AR1268ICV500	ICVPP070825AR1268	PP073586.D	08 Jul 2025 06:52		YPAJ	Ok
36	DDT ANALOGUE	DDT ANALOGUE	PP073587.D	08 Jul 2025 07:24		YPAJ	Ok

M : Manual Integration

Instrument ID: ECD_P

Daily Analysis Runlog For Sequence/QCBatch ID # PP072125

Review By	yogesh	Review On	7/21/2025 11:07:59 AM
Supervise By	mohammad	Supervise On	7/23/2025 1:32:53 AM
SubDirectory	PP072125	HP Acquire Method	HP Processing Method PP070825
STD. NAME	STD REF.#		
Tune/Reschk Initial Calibration Stds	PP24330,PP24331,PP24332,PP24333,PP24334,PP24335,PP24336,PP24337,PP24338,PP24339,PP24340,PP24341,PP24342,PP24343,PP24344,PP24345,PP24346,PP24347,PP24348,PP24349,PP24350,PP24351,PP24352,PP24353,PP24354,PP24355,PP24356,PP24357,PP24358,PP24359,PP24360,PP24361,PP24362,PP24363,PP24364,PP24365,PP24366,PP24367,PP24368,PP24369		
CCC Internal Standard/PEM ICV/I.BLK Surrogate Standard MS/MSD Standard LCS Standard	PP24332,PP24347,PP24352,PP24357 PP24370,PP24371,PP24372,PP24373,PP24374,PP24375,PP24376,PP24377,PP24378,PP24379,PP24380,PP24381,PP24382,PP24384,PP24385,PP24386,PP24387		

Sr#	SampleID	ClientID	Data File Name	Date-Time	Comment	Operator	Status
1	HEXANE	HEXANE	PP073971.D	21 Jul 2025 08:35		YPAJ	Ok
2	AR1660CCC500	AR1660CCC500	PP073972.D	21 Jul 2025 08:51		YPAJ	Ok
3	AR1242CCC500	AR1242CCC500	PP073973.D	21 Jul 2025 09:08		YPAJ	Ok
4	AR1248CCC500	AR1248CCC500	PP073974.D	21 Jul 2025 09:24		YPAJ	Ok
5	AR1254CCC500	AR1254CCC500	PP073975.D	21 Jul 2025 09:40		YPAJ	Ok
6	I.BLK	I.BLK	PP073976.D	21 Jul 2025 09:56		YPAJ	Ok
7	DDT ANALOG	DDT ANALOG	PP073977.D	21 Jul 2025 10:13		YPAJ	Ok
8	PB168911BS	PB168911BS	PP073978.D	21 Jul 2025 10:46		YPAJ	Ok
9	PB168911BSD	PB168911BSD	PP073979.D	21 Jul 2025 11:05		YPAJ	Ok
10	Q2610-01DL	2010DL	PP073980.D	21 Jul 2025 11:21	AR1242 Hit	YPAJ	Ok,M
11	Q2610-03DL	2012DL	PP073981.D	21 Jul 2025 11:37	AR1248 Hit	YPAJ	Ok,M
12	Q2610-05DL	2014DL	PP073982.D	21 Jul 2025 13:07	AR1248 Hit	YPAJ	Ok,M
13	Q2635-01	RT2286	PP073983.D	21 Jul 2025 13:24	AR1254 Hit	YPAJ	Ok,M
14	Q2635-01MS	RT2286MS	PP073984.D	21 Jul 2025 13:40		YPAJ	Ok,M
15	Q2635-01MSD	RT2286MSD	PP073985.D	21 Jul 2025 13:56		YPAJ	Ok,M
16	Q2634-01	J2315	PP073986.D	21 Jul 2025 14:13		YPAJ	Ok,M
17	AR1660CCC500	AR1660CCC500	PP073987.D	21 Jul 2025 15:18	DCB HIGH in second column	YPAJ	Ok
18	AR1242CCC500	AR1242CCC500	PP073988.D	21 Jul 2025 15:34		YPAJ	Ok

Instrument ID: ECD_P

Daily Analysis Runlog For Sequence/QCBatch ID # PP072125

Review By	yogesh	Review On	7/21/2025 11:07:59 AM
Supervise By	mohammad	Supervise On	7/23/2025 1:32:53 AM
SubDirectory	PP072125	HP Acquire Method	HP Processing Method PP070825
STD. NAME	STD REF.#		
Tune/Reschk Initial Calibration Stds CCC Internal Standard/PEM ICV/I.BLK Surrogate Standard MS/MSD Standard LCS Standard	PP24330,PP24331,PP24332,PP24333,PP24334,PP24335,PP24336,PP24337,PP24338,PP24339,PP24340,PP24341,PP24342,PP24343,PP24344,PP24345,PP24346,PP24347,PP24348,PP24349,PP24350,PP24351,PP24352,PP24353,PP24354,PP24355,PP24356,PP24357,PP24358,PP24359,PP24360,PP24361,PP24362,PP24363,PP24364,PP24365,PP24366,PP24367,PP24368,PP24369 PP24332,PP24347,PP24352,PP24357 PP24370,PP24371,PP24372,PP24373,PP24374,PP24375,PP24376,PP24377,PP24378,PP24379,PP24380,PP24381,PP24382,PP24384,PP24385,PP24386,PP24387		

19	AR1248CCC500	AR1248CCC500	PP073989.D	21 Jul 2025 15:50		YPAJ	Ok
20	AR1254CCC500	AR1254CCC500	PP073990.D	21 Jul 2025 16:07		YPAJ	Ok
21	I.BLK	I.BLK	PP073991.D	21 Jul 2025 16:23		YPAJ	Ok
22	PB168927BL	PB168927BL	PP073992.D	21 Jul 2025 16:39		YPAJ	Ok
23	PB168927BS	PB168927BS	PP073993.D	21 Jul 2025 16:56		YPAJ	Ok
24	Q2638-01	OU4-TS-31-071725	PP073994.D	21 Jul 2025 17:12	DCB Low in both column	YPAJ	ReRun
25	Q2638-03	OU4-TS-32-071725	PP073995.D	21 Jul 2025 17:29	DCB Low in both column	YPAJ	ReRun
26	Q2638-05	OU4-TS-33-071725	PP073996.D	21 Jul 2025 17:45	DCB Low in 1st column	YPAJ	Ok
27	Q2638-07	OU4-TS-34-071725	PP073997.D	21 Jul 2025 18:01	DCB Low in both column	YPAJ	ReRun
28	Q2638-09	OU4-TS-35-071725	PP073998.D	21 Jul 2025 18:18		YPAJ	Ok
29	Q2638-11	OU4-TS-36-071725	PP073999.D	21 Jul 2025 18:34	DCB Low in 1st column	YPAJ	Ok
30	Q2638-13	OU4-TS-37-071725	PP074000.D	21 Jul 2025 18:50		YPAJ	Ok
31	Q2639-01	OU4-TS-38-071725	PP074001.D	21 Jul 2025 19:07	DCB Low in 1st column, AR1254 hit	YPAJ	Ok,M
32	AR1660CCC500	AR1660CCC500	PP074002.D	21 Jul 2025 20:12	AR1260-2 low in first column	YPAJ	Ok
33	AR1242CCC500	AR1242CCC500	PP074003.D	21 Jul 2025 20:45		YPAJ	Ok
34	AR1248CCC500	AR1248CCC500	PP074004.D	21 Jul 2025 21:01		YPAJ	Ok,M
35	AR1254CCC500	AR1254CCC500	PP074005.D	21 Jul 2025 21:17		YPAJ	Ok
36	I.BLK	I.BLK	PP074006.D	21 Jul 2025 21:34		YPAJ	Ok
37	Q2663-05	HEI379F-1-1	PP074007.D	21 Jul 2025 21:50		YPAJ	Ok

Instrument ID: ECD_P

Daily Analysis Runlog For Sequence/QCBatch ID # PP072125

Review By	yogesh	Review On	7/21/2025 11:07:59 AM
Supervise By	mohammad	Supervise On	7/23/2025 1:32:53 AM
SubDirectory	PP072125	HP Acquire Method	HP Processing Method PP070825
STD. NAME	STD REF.#		
Tune/Reschk Initial Calibration Stds CCC Internal Standard/PEM ICV/I.BLK Surrogate Standard MS/MSD Standard LCS Standard	PP24330,PP24331,PP24332,PP24333,PP24334,PP24335,PP24336,PP24337,PP24338,PP24339,PP24340,PP24341,PP24342,PP24343,PP24344,PP24345,PP24346,PP24347,PP24348,PP24349,PP24350,PP24351,PP24352,PP24353,PP24354,PP24355,PP24356,PP24357,PP24358,PP24359,PP24360,PP24361,PP24362,PP24363,PP24364,PP24365,PP24366,PP24367,PP24368,PP24369 PP24332,PP24347,PP24352,PP24357 PP24370,PP24371,PP24372,PP24373,PP24374,PP24375,PP24376,PP24377,PP24378,PP24379,PP24380,PP24381,PP24382,PP24384,PP24385,PP24386,PP24387		

38	Q2663-06	HEI379F-1-2	PP074008.D	21 Jul 2025 22:06		YPAJ	Ok
39	Q2663-07	BC274318-1-1	PP074009.D	21 Jul 2025 22:23		YPAJ	Ok,M
40	Q2663-08	BC274318-1-2	PP074010.D	21 Jul 2025 22:39	AR1260 hit	YPAJ	Ok
41	Q2663-09	BC247637-1-1	PP074011.D	21 Jul 2025 22:55		YPAJ	Ok,M
42	Q2663-10	BC247637-1-2	PP074012.D	21 Jul 2025 23:11		YPAJ	Ok
43	Q2663-11	BC122903-1-1	PP074013.D	21 Jul 2025 23:28		YPAJ	Ok,M
44	Q2663-12	BC122903-1-2	PP074014.D	21 Jul 2025 23:44		YPAJ	Ok,M
45	Q2663-13	HEH700H-1-1	PP074015.D	22 Jul 2025 00:00	Signal#2 not detected.	YPAJ	Not Ok
46	Q2663-14	HEH700H-1-2	PP074016.D	22 Jul 2025 00:17	AR1254 Hit	YPAJ	Ok,M
47	AR1660CCC500	AR1660CCC500	PP074017.D	22 Jul 2025 01:38		YPAJ	Ok,M
48	AR1242CCC500	AR1242CCC500	PP074018.D	22 Jul 2025 01:55		YPAJ	Ok,M
49	AR1248CCC500	AR1248CCC500	PP074019.D	22 Jul 2025 02:11		YPAJ	Ok
50	AR1254CCC500	AR1254CCC500	PP074020.D	22 Jul 2025 02:27		YPAJ	Ok
51	I.BLK	I.BLK	PP074021.D	22 Jul 2025 02:44		YPAJ	Ok

M : Manual Integration

PERCENT SOLID

Supervisor: Iwona
Analyst: jignesh
Date: 7/21/2025

OVENTEMP IN Celsius (°C): 107
Time IN: 17:15
In Date: 07/18/2025
Weight Check 1.0g: 1.00
Weight Check 10g: 10.00
OvenID: M OVEN#1

OVENTEMP OUT Celsius (°C): 104
Time OUT: 08:25
Out Date: 07/19/2025
Weight Check 1.0g: 1.00
Weight Check 10g: 10.00
BalanceID: M SC-4
Thermometer ID: % SOLID-OVEN

QC:LB136542

Lab ID	Client SampleID	Dish #	Dish Wt(g) (A)	Sample Wt(g)	Dish + Sample Wt(g) (B)	Dish+Dry Sample Wt(g) (C)	% Solid	Comments
Q2637-05	SVOC-GPC-BLANK	1	1.00	1.00	2.00	2.00	100.0	
Q2637-06	PEST-GPC-BLANK	2	1.00	1.00	2.00	2.00	100.0	
Q2637-07	PEST-GPC-BLANK-SPIKE	3	1.00	1.00	2.00	2.00	100.0	
Q2637-10	SVOC-GPC2-BLANK	4	1.00	1.00	2.00	2.00	100.0	
Q2637-11	PEST-GPC2-BLANK	5	1.00	1.00	2.00	2.00	100.0	
Q2637-12	PEST-GPC2-BLANK-SPIKE	6	1.00	1.00	2.00	2.00	100.0	
Q2638-01	OU4-TS-31-071725	7	1.15	10.44	11.59	8.29	68.4	
Q2638-03	OU4-TS-32-071725	8	1.14	10.41	11.55	7.92	65.1	
Q2638-05	OU4-TS-33-071725	9	1.12	10.69	11.81	8.04	64.7	
Q2638-07	OU4-TS-34-071725	10	1.18	10.81	11.99	8.58	68.5	
Q2638-09	OU4-TS-35-071725	11	1.18	10.24	11.42	9.62	82.4	
Q2638-11	OU4-TS-36-071725	12	1.16	10.22	11.38	9.53	81.9	
Q2638-13	OU4-TS-37-071725	13	1.14	10.27	11.41	9.48	81.2	
Q2639-01	OU4-TS-38-071725	14	1.16	10.58	11.74	9.69	80.6	
Q2639-03	OU4-TS-39-071725	15	1.12	10.64	11.76	9.74	81.0	
Q2639-05	OU4-TS-40-071725	16	1.16	10.23	11.39	9.42	80.7	
Q2639-07	OU4-TS-41-071725	17	1.18	10.20	11.38	9.54	82.0	
Q2639-09	OU4-TS-42-071725	18	1.19	10.34	11.53	7.42	60.3	
Q2639-11	OU4-TS-43-071725	19	1.19	10.67	11.86	7.38	58.0	
Q2639-13	OU4-TS-44-071725	20	1.12	10.87	11.99	8.18	64.9	
Q2641-01	P001-CONCRETE001-01	21	1.00	1.00	2.00	2.00	100.0	Concreate sample
Q2645-02	RW5B-CARBON-20250716	22	1.17	10.52	11.69	8.39	68.6	
Q2648-01	A3	23	1.00	1.00	2.00	2.00	100.0	WIPE SAMPLE
Q2648-02	A4	24	1.00	1.00	2.00	2.00	100.0	WIPE SAMPLE
Q2648-03	B2	25	1.00	1.00	2.00	2.00	100.0	WIPE SAMPLE
Q2648-04	B3	26	1.00	1.00	2.00	2.00	100.0	WIPE SAMPLE
Q2648-05	B4	27	1.00	1.00	2.00	2.00	100.0	WIPE SAMPLE
Q2651-01	MH 2-1	28	1.18	10.67	11.85	11.26	94.5	

PERCENT SOLID

Supervisor: Iwona
Analyst: jignesh
Date: 7/21/2025

OVENTEMP IN Celsius(°C): 107
Time IN: 17:15
In Date: 07/18/2025
Weight Check 1.0g: 1.00
Weight Check 10g: 10.00
OvenID: M OVEN#1

OVENTEMP OUT Celsius(°C): 104
Time OUT: 08:25
Out Date: 07/19/2025
Weight Check 1.0g: 1.00
Weight Check 10g: 10.00
BalanceID: M SC-4
Thermometer ID: % SOLID-OVEN

QC:LB136542

Lab ID	Client SampleID	Dish #	Dish Wt(g) (A)	Sample Wt(g)	Dish + Sample Wt(g) (B)	Dish+Dry Sample Wt(g) (C)	% Solid	Comments
Q2651-02	MH 6-5	29	1.15	10.40	11.55	10.9	93.8	
Q2651-03	MH 7-6	30	1.12	10.20	11.32	10.7	93.9	
Q2651-04	MH 8-7	31	1.13	10.44	11.57	11.01	94.6	
Q2651-05	MH 9-8	32	1.13	10.27	11.4	10.67	92.9	

$$\% \text{ Solid} = \frac{(C-A) * 100}{(B-A)}$$

WORKLIST(Hardcopy Internal Chain)

WorkList Name : %1-071825

WorkList ID : 190813

Department : Wet-Chemistry

W 136542

Date : 07-18-2025 07:56:12

Sample	Customer Sample	Matrix	Test	Preservative	Customer	Raw Sample Storage Location	Collect Date	Method
Q2637-05	SVOC-GPC-BLANK	Solid	Percent Solids	Cool 4 deg C	CHEM02	D31	07/11/2025	Chemtech -SO
Q2637-06	PEST-GPC-BLANK	Solid	Percent Solids	Cool 4 deg C	CHEM02	D31	07/11/2025	Chemtech -SO
Q2637-07	PEST-GPC-BLANK-SPIKE	Solid	Percent Solids	Cool 4 deg C	CHEM02	D31	07/11/2025	Chemtech -SO
Q2637-10	SVOC-GPC2-BLANK	Solid	Percent Solids	Cool 4 deg C	CHEM02	D31	07/11/2025	Chemtech -SO
Q2637-11	PEST-GPC2-BLANK	Solid	Percent Solids	Cool 4 deg C	CHEM02	D31	07/11/2025	Chemtech -SO
Q2637-12	PEST-GPC2-BLANK-SPIKE	Solid	Percent Solids	Cool 4 deg C	CHEM02	D31	07/11/2025	Chemtech -SO
Q2638-01	OU4-TS-31-071725	Solid	Percent Solids	Cool 4 deg C	CHEM02	D31	07/11/2025	Chemtech -SO
Q2638-03	OU4-TS-32-071725	Solid	Percent Solids	Cool 4 deg C	NOBI03	O21	07/17/2025	Chemtech -SO
Q2638-05	OU4-TS-33-071725	Solid	Percent Solids	Cool 4 deg C	NOBI03	O21	07/17/2025	Chemtech -SO
Q2638-07	OU4-TS-34-071725	Solid	Percent Solids	Cool 4 deg C	NOBI03	O21	07/17/2025	Chemtech -SO
Q2638-09	OU4-TS-35-071725	Solid	Percent Solids	Cool 4 deg C	NOBI03	O21	07/17/2025	Chemtech -SO
Q2638-11	OU4-TS-36-071725	Solid	Percent Solids	Cool 4 deg C	NOBI03	O21	07/17/2025	Chemtech -SO
Q2638-13	OU4-TS-37-071725	Solid	Percent Solids	Cool 4 deg C	NOBI03	O21	07/17/2025	Chemtech -SO
Q2639-01	OU4-TS-38-071725	Solid	Percent Solids	Cool 4 deg C	NOBI03	O21	07/17/2025	Chemtech -SO
Q2639-03	OU4-TS-39-071725	Solid	Percent Solids	Cool 4 deg C	NOBI03	O13	07/17/2025	Chemtech -SO
Q2639-05	OU4-TS-40-071725	Solid	Percent Solids	Cool 4 deg C	NOBI03	O13	07/17/2025	Chemtech -SO
Q2639-07	OU4-TS-41-071725	Solid	Percent Solids	Cool 4 deg C	NOBI03	O13	07/17/2025	Chemtech -SO
Q2639-09	OU4-TS-42-071725	Solid	Percent Solids	Cool 4 deg C	NOBI03	O13	07/17/2025	Chemtech -SO
Q2639-11	OU4-TS-43-071725	Solid	Percent Solids	Cool 4 deg C	NOBI03	O13	07/17/2025	Chemtech -SO
Q2639-13	OU4-TS-44-071725	Solid	Percent Solids	Cool 4 deg C	NOBI03	O13	07/17/2025	Chemtech -SO
Q2641-01	P001-CONCRETE001-01	Solid	Percent Solids	Cool 4 deg C	NOBI03	O13	07/17/2025	Chemtech -SO
					ROYF02	O22	07/16/2025	Chemtech -SO

Date/Time 07/18/25 15:30

Raw Sample Received by: SBW

Raw Sample Relinquished by: CPSM

Date/Time 07/18/25 15:35

Raw Sample Received by:

CPSM

Raw Sample Relinquished by:

712 of 1148

WORKLIST(Hardcopy Internal Chain)

VB 136542

WorkList Name : %1-071825

WorkList ID : 190813

Department : Wet-Chemistry

Date : 07-18-2025 07:56:12

Sample	Customer Sample	Matrix	Test	Preservative	Customer	Raw Sample Storage Location	Collect Date	Method
Q2645-02	RW5B-CARBON-20250716	Solid	Percent Solids	Cool 4 deg C	TETR06	O41	07/16/2025	Chemtech -SO
Q2648-01	A3	Solid	Percent Solids	Cool 4 deg C	PSEG03	D31	07/18/2025	Chemtech -SO
Q2648-02	A4	Solid	Percent Solids	Cool 4 deg C	PSEG03	D31	07/18/2025	Chemtech -SO
Q2648-03	B2	Solid	Percent Solids	Cool 4 deg C	PSEG03	D31	07/18/2025	Chemtech -SO
Q2648-04	B3	Solid	Percent Solids	Cool 4 deg C	PSEG03	D31	07/18/2025	Chemtech -SO
Q2648-05	B4	Solid	Percent Solids	Cool 4 deg C	PSEG03	D31	07/18/2025	Chemtech -SO
Q2651-01	MH 2-1	Solid	Percent Solids	Cool 4 deg C	PSEG03	D31	07/18/2025	Chemtech -SO
Q2651-02	MH 6-5	Solid	Percent Solids	Cool 4 deg C	EARTH03	O22	07/17/2025	Chemtech -SO
Q2651-03	MH 7-6	Solid	Percent Solids	Cool 4 deg C	EARTH03	O22	07/17/2025	Chemtech -SO
Q2651-04	MH 8-7	Solid	Percent Solids	Cool 4 deg C	EARTH03	O22	07/17/2025	Chemtech -SO
Q2651-05	MH 9-8	Solid	Percent Solids	Cool 4 deg C	EARTH03	O22	07/17/2025	Chemtech -SO

Date/Time 07/18/25 15:00

Raw Sample Received by: SP PCB
Raw Sample Relinquished by: CF SM

Q2639-PCB

Date/Time 07/18/25 14:35

Raw Sample Received by: CP SM
Raw Sample Relinquished by: SP PCB
Page 2 of 2

07/19 of 1148

SOP ID:	M3541-ASE Extraction-15		
Clean Up SOP #:	Acid Cleanup	Extraction Start Date :	07/21/2025
Matrix :	Solid	Extraction Start Time :	08:30
Weigh By:	EH	Extraction End Date :	07/21/2025
Balance check:	RJ	Extraction End Time :	11:45
Balance ID:	EX-SC-2	pH Meter ID:	N/A
pH Strip Lot#:	N/A	Hood ID:	3,7
Extraction Method:	<input type="checkbox"/> Separatory Funnel <input type="checkbox"/> Continous Liquid/Liquid		<input type="checkbox"/> Sonication <input type="checkbox"/> Waste Dilution <input checked="" type="checkbox"/> Soxhlet

Standard Name	MLS USED	Concentration ug/mL	STD REF. # FROM LOG
Spike Sol 1	1.0ML	5000 PPB	PP24650
Surrogate	1.0ML	200 PPB	PP24663
N/A	N/A	N/A	N/A
N/A	N/A	N/A	N/A
N/A	N/A	N/A	N/A

Chemical Used	ML/SAMPLE USED	Lot Number
Hexane/Acetone/1:1	N/A	EP2627
Baked Na2SO4	N/A	EP2625
Hexane	N/A	E3956
H2SO4 1:1	N/A	EP2610
Sand	N/A	E3951
N/A	N/A	N/A

Extraction Conformance/Non-Conformance Comments:

40ML Vial Lot # 03-40BTS723, Q2634-01 used Limited volume as sample is oil.

KD Bath ID: N/A Envap ID: NEVAP-02
 KD Bath Temperature: N/A Envap Temperature: 40 °C

Date / Time	Prepped Sample Relinquished By/Location	Received By/Location
7/21/25	R8 (Ext (alb))	Y-P-PESTIPLC3
11:50	Preparation Group	Analysis Group

Analytical Method: M3541-ASE Extraction-15

Concentration Date: 07/21/2025

Sample ID	Client Sample ID	Test	g/ mL	PH	Surr/Spike By:		Final Vol. (mL)	JarID	Comments	Prep Pos
					AddedBy	VerifiedBy				
PB168927BL	ABLK927	PCB	30.02	N/A	ritesh	Evelyn	10			U2-1
PB168927BS	ALCS927	PCB	30.01	N/A	ritesh	Evelyn	10			2
Q2634-01	J2315	PCB	1.03	N/A	ritesh	Evelyn	10		Oil	
Q2635-01	RT2286	PCB	30.06	N/A	ritesh	Evelyn	10	E		3
Q2635-01MS	RT2286MS	PCB	30.05	N/A	ritesh	Evelyn	10	E		4
Q2635-01MS D	RT2286MSD	PCB	30.02	N/A	ritesh	Evelyn	10	E		5
Q2638-01	OU4-TS-31-071725	PCB	30.04	N/A	ritesh	Evelyn	10	D		6
Q2638-03	OU4-TS-32-071725	PCB	30.08	N/A	ritesh	Evelyn	10	D		U3-1
Q2638-05	OU4-TS-33-071725	PCB	30.02	N/A	ritesh	Evelyn	10	D		2
Q2638-07	OU4-TS-34-071725	PCB	30.07	N/A	ritesh	Evelyn	10	D		3
Q2638-09	OU4-TS-35-071725	PCB	30.03	N/A	ritesh	Evelyn	10	D		4
Q2638-11	OU4-TS-36-071725	PCB	30.05	N/A	ritesh	Evelyn	10	D		5
Q2638-13	OU4-TS-37-071725	PCB	30.02	N/A	ritesh	Evelyn	10	D		6
Q2639-01	OU4-TS-38-071725	PCB	30.01	N/A	ritesh	Evelyn	10	D		U6-1
Q2639-03	OU4-TS-39-071725	PCB	30.04	N/A	ritesh	Evelyn	10	D		2
Q2639-05	OU4-TS-40-071725	PCB	30.06	N/A	ritesh	Evelyn	10	D		3
Q2639-07	OU4-TS-41-071725	PCB	30.09	N/A	ritesh	Evelyn	10	D		4
Q2639-09	OU4-TS-42-071725	PCB	30.05	N/A	ritesh	Evelyn	10	D		5
Q2639-11	OU4-TS-43-071725	PCB	30.06	N/A	ritesh	Evelyn	10	D		6
Q2639-13	OU4-TS-44-071725	PCB	30.02	N/A	ritesh	Evelyn	10	D		U1-1
Q2641-01	P001-CONCRETE001-01	PCB	30.06	N/A	ritesh	Evelyn	10		Concrete	2
Q2645-02	RW5B-CARBON-2025071 6	PCB	30.03	N/A	ritesh	Evelyn	10	B		3

RE
7/21

* Extracts relinquished on the same date as received.

66927
8/30

WORKLIST(Hardcopy Internal Chain)

WorkList Name : Q2635

WorkList ID : 190838

Department : Extraction

Date : 07-21-2025 08:25:02

Sample	Customer Sample	Matrix	Test	Preservative	Customer	Raw Sample Storage Location	Collect Date	Method
Q2634-01	J2315	Solid	PCB	Cool 4 deg C	PSEG03	D31	07/17/2025	8082A
Q2635-01	RT2286	Solid	PCB	Cool 4 deg C	PSEG03	D31	07/17/2025	8082A
Q2638-01	OU4-TS-31-071725	Solid	PCB	Cool 4 deg C	NOBI03	O21	07/17/2025	8082A
Q2638-03	OU4-TS-32-071725	Solid	PCB	Cool 4 deg C	NOBI03	O21	07/17/2025	8082A
Q2638-05	OU4-TS-33-071725	Solid	PCB	Cool 4 deg C	NOBI03	O21	07/17/2025	8082A
Q2638-07	OU4-TS-34-071725	Solid	PCB	Cool 4 deg C	NOBI03	O21	07/17/2025	8082A
Q2638-09	OU4-TS-35-071725	Solid	PCB	Cool 4 deg C	NOBI03	O21	07/17/2025	8082A
Q2638-11	OU4-TS-36-071725	Solid	PCB	Cool 4 deg C	NOBI03	O21	07/17/2025	8082A
Q2638-13	OU4-TS-37-071725	Solid	PCB	Cool 4 deg C	NOBI03	O21	07/17/2025	8082A
Q2639-01	OU4-TS-38-071725	Solid	PCB	Cool 4 deg C	NOBI03	O13	07/17/2025	8082A
Q2639-03	OU4-TS-39-071725	Solid	PCB	Cool 4 deg C	NOBI03	O13	07/17/2025	8082A
Q2639-05	OU4-TS-40-071725	Solid	PCB	Cool 4 deg C	NOBI03	O13	07/17/2025	8082A
Q2639-07	OU4-TS-41-071725	Solid	PCB	Cool 4 deg C	NOBI03	O13	07/17/2025	8082A
Q2639-09	OU4-TS-42-071725	Solid	PCB	Cool 4 deg C	NOBI03	O13	07/17/2025	8082A
Q2639-11	OU4-TS-43-071725	Solid	PCB	Cool 4 deg C	NOBI03	O13	07/17/2025	8082A
Q2639-13	OU4-TS-44-071725	Solid	PCB	Cool 4 deg C	NOBI03	O13	07/17/2025	8082A
Q2641-01	P001-CONCRETE001-01	Solid	PCB	Cool 4 deg C	ROYF02	O22	07/16/2025	8082A
Q2645-02	RW5B-CARBON-20250716	Solid	PCB	Cool 4 deg C	TETR06	O41	07/16/2025	8082A

Date/Time 07/21/25 8:25

Raw Sample Received by: RJ L (Ext-1ab)

Raw Sample Relinquished by: CJ S

Date/Time 07/21/25 8:55

Raw Sample Received by: CJ S

Raw Sample Relinquished by: RJ L (Ext-1ab)

Prep Standard - Chemical Standard Summary

Order ID : Q2639

Test : PCB

Prepbatch ID : PB168927,

Sequence ID/Qc Batch ID: po072125,PO072225,pp072125,

Standard ID :

EP2610,EP2625,EP2627,PP24329,PP24330,PP24331,PP24332,PP24333,PP24334,PP24335,PP24336,PP24337,PP24338,PP24339,PP24340,PP24341,PP24342,PP24343,PP24344,PP24345,PP24346,PP24347,PP24348,PP24349,PP24350,PP24351,PP24352,PP24353,PP24354,PP24355,PP24356,PP24357,PP24358,PP24359,PP24360,PP24361,PP24362,PP24363,PP24364,PP24365,PP24366,PP24367,PP24368,PP24369,PP24370,PP24371,PP24372,PP24373,PP24374,PP24375,PP24376,PP24377,PP24378,PP24379,PP24380,PP24381,PP24382,PP24384,PP24385,PP24386,PP24387,PP24650,PP24663,

Chemical ID :

E3551,E3804,E3877,E3940,E3944,E3949,E3950,E3951,E3956,M6157,P11522,P12699,P12702,P12931,P12936,P12949,P12950,P12957,P13356,P13373,P13381,P13589,P13591,P13697,P13702,P13786,P13830,P13878,P13883,W3112,W3177,

Extractions STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
314	1.1 H2SO4 SOLN	EP2610	05/07/2025	11/07/2025	RUPESHKUMA R SHAH	Extraction_SC ALE_2 (EX-SC-2)	None	Riteshkumar Patel 05/07/2025

FROM 1000.00000ml of M6157 + 1000.00000ml of W3112 = Final Quantity: 2000.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3923	Baked Sodium Sulfate	EP2625	07/15/2025	12/04/2025	RUPESHKUMA R SHAH	Extraction_SC ALE_2 (EX-SC-2)	None	Riteshkumar Patel 07/15/2025

FROM 4000.00000gram of E3551 = Final Quantity: 4000.000 gram

Extractions STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
230	1:1ACETONE/HEXANE	EP2627	07/15/2025	01/15/2026	RUPESHKUMA R SHAH	None	None	Riteshkumar Patel 07/15/2025

FROM 4000.00000ml of E3949 + 4000.00000ml of E3950 = Final Quantity: 8000.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
84	Pest/PCB Surrogate Stock 20 PPM	PP24329	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza 04/03/2025

FROM 1.00000ml of P13356 + 9.00000ml of W3177 = Final Quantity: 10.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
202	AR1660 1000/100 ppb working solution 1st source	PP24330	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza 04/03/2025

FROM 0.10000ml of P13697 + 99.40000ml of W3177 + 0.50000ml of PP24329 = Final Quantity: 100.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
203	AR1660 750 PPB STD	PP24331	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza 04/03/2025

FROM 0.25000ml of W3177 + 0.75000ml of PP24330 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
204	AR1660 500 PPB STD	PP24332	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza 04/03/2025

FROM 0.50000ml of W3177 + 0.50000ml of PP24330 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
205	AR1660 250 PPB STD	PP24333	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza 04/03/2025

FROM 0.75000ml of W3177 + 0.25000ml of PP24330 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
206	AR1660 50 PPB STD	PP24334	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza 04/03/2025

FROM 0.90000ml of W3177 + 0.10000ml of PP24332 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
213	AR1221 1000 PPB WORKING SOLUTION	PP24335	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza 04/03/2025

FROM 0.10000ml of P13702 + 99.40000ml of W3177 + 0.50000ml of PP24329 = Final Quantity: 100.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1079	AR1221 750 PPB STD	PP24336	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza 04/03/2025

FROM 0.25000ml of W3177 + 0.75000ml of PP24335 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
222	AR1221 500 PPB STD	PP24337	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza 04/03/2025

FROM 0.50000ml of W3177 + 0.50000ml of PP24335 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1080	AR1221 250 PPB STD	PP24338	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza 04/03/2025

FROM 0.75000ml of W3177 + 0.25000ml of PP24335 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1081	AR1221 50 PPB STD	PP24339	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza 04/03/2025

FROM 0.90000ml of W3177 + 0.10000ml of PP24337 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
214	AR1232 1000 PPB WORKING SOLUTION	PP24340	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza 04/03/2025

FROM 0.10000ml of P13878 + 99.40000ml of W3177 + 0.50000ml of PP24329 = Final Quantity: 100.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1063	AR1232 750 PPB STD	PP24341	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza 04/03/2025

FROM 0.25000ml of W3177 + 0.75000ml of PP24340 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
223	AR1232 500 PPB STD	PP24342	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza 04/03/2025

FROM 0.50000ml of W3177 + 0.50000ml of PP24340 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1064	AR1232 250 PPB STD	PP24343	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza 04/03/2025

FROM 0.75000ml of W3177 + 0.25000ml of PP24340 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1065	AR1232 50 PPB STD	PP24344	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza 04/03/2025

FROM 0.90000ml of W3177 + 0.10000ml of PP24342 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
215	AR1242 1000 PPB WORKING STD	PP24345	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza 04/03/2025

FROM 0.10000ml of P12931 + 99.40000ml of W3177 + 0.50000ml of PP24329 = Final Quantity: 100.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1067	AR1242 750 PPB STD	PP24346	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza 04/03/2025

FROM 0.75000ml of W3177 + 0.75000ml of PP24345 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
224	AR1242 500 PPB STD	PP24347	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza 04/03/2025

FROM 0.50000ml of W3177 + 0.50000ml of PP24345 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1068	AR1242 250 PPB STD	PP24348	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza 04/03/2025

FROM 0.75000ml of W3177 + 0.25000ml of PP24345 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1069	AR1242 50 PPB STD	PP24349	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza 04/03/2025

FROM 0.90000ml of W3177 + 0.10000ml of PP24347 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
216	AR1248 1000 PPB WORKING STD	PP24350	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza 04/03/2025

FROM 0.10000ml of P12936 + 99.40000ml of W3177 + 0.50000ml of PP24329 = Final Quantity: 100.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1075	AR1248 750 PPB STD	PP24351	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza 04/03/2025

FROM 0.25000ml of W3177 + 0.75000ml of PP24350 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
225	AR1248 500 PPB STD	PP24352	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza 04/03/2025

FROM 0.50000ml of W3177 + 0.50000ml of PP24350 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1076	AR1248 250 PPB STD	PP24353	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza 04/03/2025

FROM 0.75000ml of W3177 + 0.25000ml of PP24350 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1077	AR1248 50 PPB STD	PP24354	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza 04/03/2025

FROM 0.90000ml of W3177 + 0.10000ml of PP24352 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
217	AR1254 1000 PPB WORKING STD	PP24355	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza 04/03/2025

FROM 0.10000ml of P13830 + 99.40000ml of W3177 + 0.50000ml of PP24329 = Final Quantity: 100.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1071	AR1254 750 PPB STD	PP24356	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza 04/03/2025

FROM 0.25000ml of W3177 + 0.75000ml of PP24355 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
226	AR1254 500 PPB STD	PP24357	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza 04/03/2025

FROM 0.50000ml of W3177 + 0.50000ml of PP24355 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1072	AR1254 250 PPB STD	PP24358	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza 04/03/2025

FROM 0.75000ml of W3177 + 0.25000ml of PP24355 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1073	AR1254 50 PPB STD	PP24359	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza 04/03/2025

FROM 0.90000ml of W3177 + 0.10000ml of PP24357 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1529	AR1262 1000 PPB Working Solution	PP24360	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza 04/03/2025

FROM 0.10000ml of P13883 + 99.40000ml of W3177 + 0.50000ml of PP24329 = Final Quantity: 100.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3753	AR1262 750 PPB STD	PP24361	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza 04/03/2025

FROM 0.25000ml of W3177 + 0.75000ml of PP24360 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1530	AR1262 500 PPB STD	PP24362	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza 04/03/2025

FROM 0.50000ml of W3177 + 0.50000ml of PP24360 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3754	AR1262 250 PPB STD	PP24363	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza 04/03/2025

FROM 0.75000ml of W3177 + 0.25000ml of PP24360 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3755	AR1262 50 PPB STD	PP24364	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza 04/03/2025

FROM 0.90000ml of W3177 + 0.10000ml of PP24362 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1532	AR1268 1000 PPB Working Solution	PP24365	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza 04/03/2025

FROM 0.10000ml of P13381 + 99.40000ml of W3177 + 0.50000ml of PP24329 = Final Quantity: 100.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3820	AR1268 750 PPB STD	PP24366	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza 04/03/2025

FROM 0.25000ml of W3177 + 0.75000ml of PP24365 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1533	AR1268 500 PPB STD	PP24367	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza 04/03/2025

FROM 0.50000ml of W3177 + 0.50000ml of PP24365 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3821	AR1268 250 PPB STD	PP24368	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza 04/03/2025

FROM 0.75000ml of W3177 + 0.25000ml of PP24365 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3822	AR1268 50 PPB STD	PP24369	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza 04/03/2025

FROM 0.90000ml of W3177 + 0.10000ml of PP24367 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
404	AR1660 100 PPM Stock Solution 2nd Source	PP24370	03/18/2025	09/18/2025	Yogesh Patel	None	None	Abdul Mirza 04/03/2025

FROM 1.00000ml of P12949 + 9.00000ml of E3804 = Final Quantity: 10.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
405	AR1660 1000/100 PPB ICV STD	PP24371	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza 04/03/2025

FROM 98.50000ml of W3177 + 0.50000ml of PP24329 + 1.00000ml of PP24370 = Final Quantity: 100.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
406	AR1660 500 PPB ICV	PP24372	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza 04/03/2025

FROM 0.50000ml of W3177 + 0.50000ml of PP24371 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3789	AR1221 1000 PPB WORKING SOL.2ND SOURCE(AGILENT)	PP24373	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza 04/03/2025

FROM 1.00000ml of P13373 + 98.50000ml of W3177 + 0.50000ml of PP24329 = Final Quantity: 100.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1886	AR1221 500 PPB ICV	PP24374	03/18/2025	08/12/2025	Yogesh Patel	None	None	Abdul Mirza 04/03/2025

FROM 0.50000ml of E3877 + 0.50000ml of W3177 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1887	AR1232 1000 PPB Working Sol. 2nd Source	PP24375	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza 04/03/2025

FROM 1.00000ml of P12699 + 98.50000ml of W3177 + 0.50000ml of PP24329 = Final Quantity: 100.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1888	AR1232 500 PPB ICV	PP24376	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza 04/03/2025

FROM 0.50000ml of W3177 + 0.50000ml of PP24375 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1889	AR1242 1000 PPB Working Sol. 2nd Source	PP24377	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza 04/03/2025

FROM 1.00000ml of P13589 + 98.50000ml of W3177 + 0.50000ml of PP24329 = Final Quantity: 100.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1891	AR1242 500 PPB ICV	PP24378	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza 04/03/2025

FROM 0.50000ml of W3177 + 0.50000ml of PP24377 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1890	AR1248 1000 PPB Working Sol. 2nd Source	PP24379	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza 04/03/2025

FROM 1.00000ml of P13591 + 98.50000ml of W3177 + 0.50000ml of PP24329 = Final Quantity: 100.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1892	AR1248 500 PPB ICV	PP24380	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza 04/03/2025

FROM 0.50000ml of W3177 + 0.50000ml of PP24379 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1893	AR1254 1000 PPB Working Sol. 2nd Source	PP24381	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza 04/03/2025

FROM 1.00000ml of P12957 + 98.50000ml of W3177 + 0.50000ml of PP24329 = Final Quantity: 100.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1894	AR1254 500 PPB ICV	PP24382	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza 04/03/2025

FROM 0.50000ml of W3177 + 0.50000ml of PP24381 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3757	AR1262 1000 PPB Working Solution second source	PP24384	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza 04/03/2025

FROM 1.00000ml of P12702 + 98.50000ml of W3177 + 0.50000ml of PP24329 = Final Quantity: 100.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3758	AR1262 500 PPB STD ICV	PP24385	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza 04/03/2025

FROM 0.50000ml of W3177 + 0.50000ml of PP24384 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3817	AR1268 1000 ppb Working Soln. 2nd source	PP24386	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza 04/03/2025

FROM 1.00000ml of P11522 + 98.50000ml of W3177 + 0.50000ml of PP24329 = Final Quantity: 100.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3823	AR1268 500 PPB STD ICV	PP24387	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza 04/03/2025

FROM 0.50000ml of W3177 + 0.50000ml of PP24386 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3857	5000 PPB PCB SPIKE SOLUTION 2ND SOURCE	PP24650	06/16/2025	12/11/2025	Abdul Mirza	None	None	Yogesh Patel 07/21/2025

FROM 0.50000ml of P12950 + 99.50000ml of E3940 = Final Quantity: 100.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
465	200 PPB Pest/PCB Surrogate Spike	PP24663	06/24/2025	12/24/2025	Abdul Mirza	None	None	Yogesh Patel 07/21/2025

FROM 1.00000ml of P13786 + 999.00000ml of E3944 = Final Quantity: 1000.000 ml

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
PCI Scientific Supply, Inc.	PC19631-100 / SODIUM SULFATE, ANHYDROUS, PEST GRADE, 1	313201	12/04/2025	01/03/2024 / Rajesh	07/20/2023 / Rajesh	E3551
Seidler Chemical	9005-05 / Acetone Ultra (cs/4x4L)	24E0761004	11/05/2025	10/01/2024 / Rajesh	09/25/2024 / Rajesh	E3804
Seidler Chemical	BA-9262-03 / Hexane, Ultra-Resi (cs/4x4L)	243570	08/12/2025	02/12/2025 / Rajesh	02/12/2025 / Rajesh	E3877
Seidler Chemical	BA-9254-03 / Acetone, Ultra Resi (cs/4x4L)	24H1462005	12/11/2025	06/11/2025 / Rajesh	06/04/2025 / Rajesh	E3940
Seidler Chemical	BA-9254-03 / Acetone, Ultra Resi (cs/4x4L)	24H1462005	05/24/2027	06/20/2025 / RUPESH	05/14/2025 / RUPESH	E3944
Seidler Chemical	BA-9254-03 / Acetone, Ultra Resi (cs/4x4L)	24H2762008	04/18/2027	07/08/2025 / RITESHKUMAR	07/03/2025 / RUPESH	E3949

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9262-03 / Hexane, Ultra-Resi (cs/4x4L)	25C0362005	04/30/2026	07/08/2025 / RITESHKUMAR	07/03/2025 / RUPESH	E3950
Seidler Chemical	BA-3382-05 / Sand, Purified (cs/4x2.5kg)	25A2756718	12/31/2028	07/09/2025 / RUPESH	04/28/2020 / RUPESH	E3951
Seidler Chemical	BA-9262-03 / Hexane, Ultra-Resi (cs/4x4L)	25C0362005	04/30/2026	07/16/2025 / RUPESH	07/16/2025 / RUPESH	E3956
Seidler Chemical	BA-9673-33 / Sulfuric Acid, Instra-Analyzed (cs/6c2.5L)	24i1262013	11/07/2025	05/07/2025 / RUPESH	02/18/2025 / Mohan	M6157
Agilent Technologies	PP-382-1 / Aroclor 1268	0006587800	09/18/2025	03/18/2025 / yogesh	02/21/2022 / Ankita	P11522
Absolute Standards,Inc	91867 / Aroclor 1232 100 ug/mL	020823	09/18/2025	03/18/2025 / yogesh	08/07/2023 / Ankita	P12699

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	x9166 / Aroclor 1262 100 ug/mL	060523	09/18/2025	03/18/2025 / yogesh	08/07/2023 / Ankita	P12702
Restek	32009 / PCB Mix, Aroclor 1242, 1000ug/mL, Hexane, 1mL/ampul	a0203672	09/18/2025	03/18/2025 / yogesh	12/07/2023 / Ankita	P12931
Restek	32010 / PCB Mix, Aroclor 1248, 1000ug/mL, Hexane, 1mL/ampul	a0202803	09/18/2025	03/18/2025 / yogesh	12/07/2023 / Ankita	P12936
Absolute Standards, Inc.	20064 / Aroclor 1016/1260	022023	09/18/2025	03/18/2025 / yogesh	12/20/2023 / Yogesh	P12949
Absolute Standards, Inc.	20064 / Aroclor 1016/1260	022023	12/16/2025	06/16/2025 / Abdul	12/20/2023 / Yogesh	P12950
Absolute Standards, Inc.	/ Arochlor 1254	121823	04/03/2025	10/03/2024 / Ankita	12/20/2023 / Yogesh	P12957

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32000 / Pesticide Mix, CLP method, Pesticide Surrogate Mix, 200ug/mL, Acetone, 1mL	A0206810	09/18/2025	03/18/2025 / yogesh	04/22/2024 / Abdul	P13356
Agilent Technologies	PP-292-1 / Aroclor 1221	0006783205	09/18/2025	03/18/2025 / yogesh	05/02/2024 / Ankita	P13373
Restek	32410 / PCB Stock Solution, Aroclor 1268 Std, 1mL, Hexane	A0207475	09/18/2025	03/18/2025 / yogesh	05/03/2024 / Abdul	P13381
Agilent Technologies	PP-312-1 / Aroclor 1242	0006665550	09/18/2025	03/18/2025 / yogesh	10/14/2024 / Ankita	P13589
Agilent Technologies	PP-342-1 / Aroclor 1248	0006726317	09/18/2025	03/18/2025 / yogesh	10/14/2024 / Ankita	P13591
Restek	32039 / PCB Mix, Aroclor 1016/1260, 1000ug/mL, hexane, 1mL/ampul	A0210629	09/18/2025	03/18/2025 / yogesh	10/17/2024 / yogesh	P13697

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32007 / PCB Mix, Aroclor 1221, 1000ug/mL, Hexane, 1mL/ampul	A0215270	09/18/2025	03/18/2025 / yogesh	10/17/2024 / yogesh	P13702
Restek	32000 / Pesticide Mix, CLP method, Pesticide Surrogate Mix, 200ug/mL, Acetone, 1mL	A0214495	12/24/2025	06/24/2025 / Abdul	11/19/2024 / Ankita	P13786
Restek	32011 / PCB Mix, Aroclor 1254, 1000ug/mL, Hexane, 1mL/ampul	A0217391	09/18/2025	03/18/2025 / yogesh	12/09/2024 / Ankita	P13830
Restek	32008 / PCB Mix, Aroclor 1232, 1000ug/mL, Hexane, 1mL/ampul	A0219655	09/18/2025	03/18/2025 / yogesh	01/23/2025 / Ankita	P13878
Restek	32409 / PCB Stock Solution, Aroclor 1262 Std, 1mL, Hexane	A0220950	09/18/2025	03/18/2025 / yogesh	01/23/2025 / Ankita	P13883
Seidler Chemical	DIW / DI Water	Daily Lab-Certified	07/03/2029	07/03/2024 / Iwona	07/03/2024 / Iwona	W3112

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9262-03 / Hexane, Ultra-Resi (cs/4x4L)	24G1962003	08/22/2025	02/03/2025 / jignesh	01/31/2025 / jignesh	W3177

 1
 2
 3
 4
 5
 6
 7
 8
 9
 10
 11
 12
 13
 14
 15
 16
 17
 18
 19
 20



PRODUCTOS
QUÍMICOS
MONTERREY, S.A. DE C.V.

MIRADOR 201, COL. MIRADOR
MONTERREY, N.L. MEXICO
CP 64070
TEL +52 81 13 52 57 57
www.pqm.com.mx

CERTIFICATE OF ANALYSIS

PRODUCT :	SODIUM SULFATE CRYSTALS ANHYDROUS		
QUALITY :	ACS (CODE RMB3375)	FORMULA :	Na ₂ SO ₄
SPECIFICATION NUMBER :	6399	RELEASE DATE:	ABR/21/2023
LOT NUMBER :	313201		

TEST	SPECIFICATIONS	LOT VALUES
Assay (Na ₂ SO ₄)	Min. 99.0%	99.7 %
pH of a 5% solution at 25°C	5.2 - 9.2	6.1
Insoluble matter	Max. 0.01%	0.005 %
Loss on ignition	Max. 0.5%	0.1 %
Chloride (Cl)	Max. 0.001%	<0.001 %
Nitrogen compounds (as N)	Max. 5 ppm	<5 ppm
Phosphate (PO ₄)	Max. 0.001%	<0.001 %
Heavy metals (as Pb)	Max. 5 ppm	<5 ppm
Iron (Fe)	Max. 0.001%	<0.001 %
Calcium (Ca)	Max. 0.01%	0.002 %
Magnesium (Mg)	Max. 0.005%	0.001 %
Potassium (K)	Max. 0.008%	0.003 %
Extraction-concentration suitability	Passes test	Passes test
Appearance	Passes test	Passes test
Identification	Passes test	Passes test
Solubility and foreing matter	Passes test	Passes test
Retained on US Standard No. 10 sieve	Max. 1%	0.1 %
Retained on US Standard No. 60 sieve	Min. 94%	97.3 %
Through US Standard No. 60 sieve	Max. 5%	2.5 %
Through US Standard No. 100 sieve	Max. 10%	0.1 %

COMMENTS

QC: PhC Irma Belmares

If you need further details, please call our factory or contact our local distributor.

Recd. by R3 on 7/29/23 [E 3551]

RC-02-01, Ed. 3

Material No.: 9005-05
Batch No.: 24E0761004
Manufactured Date: 2024-05-02
Retest Date: 2029-05-01
Revision No.: 0

Certificate of Analysis

Test	Specification	Result
Assay ((CH ₃) ₂ CO) (by GC, corrected for water)	≥ 99.5 %	99.8 %
Color (APHA)	≤ 10	< 5
Residue after Evaporation	≤ 5 ppm	< 1 ppm
Titrable Acid (μeq/g)	≤ 0.3	0.1
Titrable Base (μeq/g)	≤ 0.5	0.1
Water (H ₂ O)	≤ 0.5 %	0.1 %
Solubility in H ₂ O	Passes Test	Passes Test
Chloride (Cl)	≤ 0.2 ppm	< 0.2 ppm
Phosphate (PO ₄)	≤ 0.05 ppm	< 0.05 ppm
Trace Impurities – Aluminum (Al)	≤ 50.0 ppb	< 5.0 ppb
Arsenic and Antimony (as As)	≤ 5.0 ppb	< 5.0 ppb
Trace Impurities – Barium (Ba)	≤ 20.0 ppb	< 1.0 ppb
Trace Impurities – Beryllium (Be)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Bismuth (Bi)	≤ 20.0 ppb	< 10.0 ppb
Trace Impurities – Boron (B)	≤ 10.0 ppb	< 5.0 ppb
Trace Impurities – Cadmium (Cd)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Calcium (Ca)	≤ 25.0 ppb	3.6 ppb
Trace Impurities – Chromium (Cr)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Cobalt (Co)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Copper (Cu)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Gallium (Ga)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Germanium (Ge)	≤ 10.0 ppb	< 10.0 ppb
Trace Impurities – Gold (Au)	≤ 20 ppb	< 5 ppb
Trace Impurities – Iron (Fe)	≤ 20.0 ppb	< 1.0 ppb
Trace Impurities – Lead (Pb)	≤ 10.0 ppb	< 10.0 ppb
Trace Impurities – Lithium (Li)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Magnesium (Mg)	≤ 20 ppb	< 1 ppb
Trace Impurities – Manganese (Mn)	≤ 10.0 ppb	< 1.0 ppb

Recd by RP on 9/25/24

E 3804

>>> Continued on page 2 >>>

Acetone
CMOS



Material No.: 9005-05
Batch No.: 24E0761004

Test	Specification	Result
Trace Impurities – Molybdenum (Mo)	≤ 10.0 ppb	< 5.0 ppb
Trace Impurities – Nickel (Ni)	≤ 10.0 ppb	< 5.0 ppb
Trace Impurities – Niobium (Nb)	≤ 50.0 ppb	< 1.0 ppb
Trace Impurities – Potassium (K)	≤ 10.0 ppb	< 10.0 ppb
Trace Impurities – Silicon (Si)	≤ 50 ppb	< 10 ppb
Trace Impurities – Silver (Ag)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Sodium (Na)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Strontium (Sr)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Tantalum (Ta)	≤ 50.0 ppb	< 5.0 ppb
Trace Impurities – Thallium (Tl)	≤ 10.0 ppb	< 5.0 ppb
Trace Impurities – Tin (Sn)	≤ 20.0 ppb	< 10.0 ppb
Trace Impurities – Titanium (Ti)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Vanadium (V)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Zinc (Zn)	≤ 20.0 ppb	7.9 ppb
Trace Impurities – Zirconium (Zr)	≤ 10.0 ppb	< 1.0 ppb
Particle Count – 0.5 µm and greater (Rion KS42AF)	≤ 100 par/ml	8 par/ml
Particle Count – 1.0 µm and greater (Rion KS42AF)	≤ 8 par/ml	2 par/ml

>>> Continued on page 3 >>>

Acetone CMOS



Material No.: 9005-05
Batch No.: 24E0761004

For Microelectronic Use

**Country of Origin: USA
Packaging Site: Paris Mfg Ctr & DC**

Michelle Bales
Michelle Bales
Sr. Manager, Quality Assurance



Certificate of Analysis

1 Reagent Lane
 Fair Lawn, NJ 07410
 201.796.7100 tel
 201.796.1329 fax

Thermo Fisher Scientific's Quality System has been found to conform to Quality Management System
 Standard ISO9001:2015 by SAI Global Certificate Number CERT – 0120633

This is to certify that units of the lot number below were tested and found to comply with the specifications of the grade listed. Certain data have been supplied by third parties. Thermo Fisher Scientific expressly disclaims all warranties, expressed or implied, including the implied warranties of merchantability and fitness for a particular purpose. Products are for research use or further manufacturing. Not for direct administration to humans or animals. It is the responsibility of the final formulator and end user to determine suitability based upon the intended use of the end product. Products are tested to meet the analytical requirements of the noted grade. The following information is the actual analytical results obtained.

Catalog Number	H303	Quality Test / Release Date	11/07/2024
Lot Number	243570		
Description	HEXANES - OPTIMA		
Country of Origin	United States	Suggested Retest Date	Nov/2029
Chemical Origin	Organic - non animal		
BSE/TSE Comment	No animal products are used as starting raw material ingredients, or used in processing, including lubricants, processing aids, or any other material that might migrate to the finished product.		

N/A

Result Name	Units	Specifications	Test Value
APPEARANCE		REPORT	Clear, colorless liquid
ASSAY (N-HEXANE)	%	>= 60	69
ASSAY (SUM C6 HYDROCARBONS)	%	>= 99.9	>99.9
COLOR	APHA	<= 5	<5
DENSITY AT 25 DEGREES C	GM/ML	Inclusive Between 0.653 - 0.673	0.669
EVAPORATION RESIDUE	ppm	<= 1	<1
FLUORESCENCE BACKGROUND	ppb	<= 1	<1
IDENTIFICATION	PASS/FAIL	= PASS TEST	PASS TEST
OPTICAL ABS AT 195 NM	ABS. UNITS	<= 1	0.74
OPTICAL ABS AT 210 NM	ABS. UNITS	<= 0.25	0.17
OPTICAL ABS AT 220 NM	ABS. UNITS	<= 0.07	0.05
OPTICAL ABS AT 254 NM	ABS. UNITS	<= 0.005	0.001
PESTICIDE RESIDUE ANALYSIS	NG/L	<= 10	<10
REFRACTIVE INDEX @ 25 DEG C		Inclusive Between 1.375 - 1.385	1.379
SUITABILITY FOR GC/MS		= PASS TEST	PASS TEST
SULFUR COMPOUNDS	%	<= 0.005	<0.005
THIOPHENE	PASS/FAIL	= PASS TEST	PASS TEST
WATER (H2O)	%	<= 0.01	<0.01
WATER-SOLUBLE TITRABLE ACID	MEQ/G	<= 0.0003	0.0001

Recd - by RP on 2/12/25

 [E3877]

Harout Sahagian - Quality Control Manager - Fair Lawn

Note: The data listed is valid for all package sizes of this lot of this product, expressed as an extension of this catalog number listed above.

If there are any questions with this certificate, please call at (800) 227-6701.

*Based on suggested storage condition.

Acetone

BAKER RESI-ANALYZED® Reagent
For Organic Residue Analysis



Material No.: 9254-03

Batch No.: 24H1462005

Manufactured Date: 2024-05-24

Expiration Date: 2027-05-24

Revision No.: 0

Certificate of Analysis

Test	Specification	Result
Assay ((CH ₃) ₂ CO) (by GC, corrected for water)	>= 99.4 %	99.8 %
Color (APHA)	<= 10	5
Residue after Evaporation	<= 1.0 ppm	0.2 ppm
Substances Reducing Permanganate	Passes Test	Passes Test
Titrable Acid (μeq/g)	<= 0.3	0.2
Titrable Base (μeq/g)	<= 0.6	<0.1
Water (H ₂ O)	<= 0.5 %	0.2 %
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	<= 5	<1
ECD Sensitive Impurities (as HeptachlorEpoxide) Single Peak (pg/mL)	<= 10	1

For Laboratory, Research, or Manufacturing Use

MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: United States

Packaging Site: Phillipsburg Mfg Ctr & DC

Recd by RP on 6/11/25

E3940

Jamie Croak
Director Quality Operations, Bioscience Production

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Acetone

BAKER RESI-ANALYZED® Reagent
For Organic Residue Analysis



Material No.: 9254-03

Batch No.: 24H1462005

Manufactured Date: 2024-05-24

Expiration Date: 2027-05-24

Revision No.: 0

Certificate of Analysis

Test	Specification	Result
Assay ((CH ₃) ₂ CO) (by GC, corrected for water)	>= 99.4 %	99.8 %
Color (APHA)	<= 10	5
Residue after Evaporation	<= 1.0 ppm	0.2 ppm
Substances Reducing Permanganate	Passes Test	Passes Test
Titrable Acid (μeq/g)	<= 0.3	0.2
Titrable Base (μeq/g)	<= 0.6	<0.1
Water (H ₂ O)	<= 0.5 %	0.2 %
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	<= 5	<1
ECD Sensitive Impurities (as HeptachlorEpoxide) Single Peak (pg/mL)	<= 10	1

For Laboratory, Research, or Manufacturing Use

MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: United States

Packaging Site: Phillipsburg Mfg Ctr & DC

E3944

A handwritten signature in black ink that reads "Jamie Croak".

Jamie Croak
Director Quality Operations, Bioscience Production

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Acetone

BAKER RESI-ANALYZED® Reagent
For Organic Residue Analysis



Material No.: 9254-03

Batch No.: 24H2762008

Manufactured Date: 2024-04-18

Expiration Date: 2027-04-18

Revision No.: 0

Certificate of Analysis

Test	Specification	Result
Assay ((CH ₃) ₂ CO) (by GC, corrected for water)	>= 99.4 %	100.0 %
Color (APHA)	<= 10	5
Residue after Evaporation	<= 1.0 ppm	0.0 ppm
Substances Reducing Permanganate	Passes Test	Passes Test
Titrable Acid (μeq/g)	<= 0.3	0.2
Titrable Base (μeq/g)	<= 0.6	<0.1
Water (H ₂ O)	<= 0.5 %	<0.1 %
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	<= 5	1
ECD Sensitive Impurities (as HeptachlorEpoxide) Single Peak (pg/mL)	<= 10	1

For Laboratory, Research, or Manufacturing Use

MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: United States

Packaging Site: Phillipsburg Mfg Ctr & DC

Reed on 7/2/25

E3949

A handwritten signature in black ink that reads "Jamie Croak".

Jamie Croak
Director Quality Operations, Bioscience Production

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

n-Hexane 95%
ULTRA RESI-ANALYZED
For Organic Residue Analysis



Material No.: 9262-03
Batch No.: 25C0362005
Manufactured Date: 2025-01-29
Expiration Date: 2026-04-30
Revision No.: 0

Certificate of Analysis

Test	Specification	Result
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	<= 5	1
ECD Sensitive Impurities (as HeptachlorEpoxide) Single Peak (pg/mL)	<= 10	6
ECD-Sensitive Impurities (as EthyleneDibromide) - Single Impurity Peak (ng/mL)	<= 5	5
Assay (Total Saturated C ₆ Isomers) (by GC, corrected for water)	>= 99.5 %	100.0 %
Assay (as n-Hexane) (by GC, corrected for water)	>= 95 %	100 %
Color (APHA)	<= 10	10
Residue after Evaporation	<= 1.0 ppm	0.1 ppm
Substances Darkened by H ₂ SO ₄	Passes Test	Passes Test
Water (by KF, coulometric)	<= 0.05 %	<0.01 %

For Laboratory, Research, or Manufacturing Use

MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: United States

Packaging Site: Phillipsburg Mfg Ctr & DC

3950

Read on 7/02/25

A handwritten signature in black ink that reads "Jamie Croak".

Jamie Croak
Director Quality Operations, Bioscience Production



Certificate of Analysis

Material	BDH9274-2.5KG
Material Description	BDH SAND STDD OTTAWA W+I 2.5KG
Grade	NOT APPLICABLE
Batch	25A2756718
Reassay Date	12/31/2028
CAS Number	14808-60-7
Molecular Formula	SiO ₂
Molecular Mass	60.09
Date of Manufacture	12/05/2024
Storage	Room Temperature

Characteristics	Specifications	Measured Values
Appearance	Beige granules.	Beige granules.
Moisture	<= 0.1 %	0.1 %
Particle Size 30-40 mesh	>= 80 %	99 %
CUSTOMER PART # BDH9274-2.5KG		

Received on 7/1/25.

E3951

Internal ID #: 793

Signature	Additional Information
We certify that this batch conforms to the specifications listed above. This document has been electronically produced and is valid without a signature. Leona Edwardson, Quality Control Sr. Manager - Solon VWR Chemicals, LLC. 28600 Fountain Parkway, Solon OH 44139 USA	Analysis may have been rounded to significant digits in specification limits Product meets analytical specifications of the grades listed.

n-Hexane 95%
ULTRA RESI-ANALYZED
For Organic Residue Analysis



Material No.: 9262-03
Batch No.: 25C0362005
Manufactured Date: 2025-01-29
Expiration Date: 2026-04-30
Revision No.: 0

Certificate of Analysis

Test	Specification	Result
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	<= 5	1
ECD Sensitive Impurities (as HeptachlorEpoxide) Single Peak (pg/mL)	<= 10	6
ECD-Sensitive Impurities (as EthyleneDibromide) – Single Impurity Peak (ng/mL)	<= 5	5
Assay (Total Saturated C ₆ Isomers) (by GC, corrected for water)	>= 99.5 %	100.0 %
Assay (as n-Hexane) (by GC, corrected for water)	>= 95 %	100 %
Color (APHA)	<= 10	10
Residue after Evaporation	<= 1.0 ppm	0.1 ppm
Substances Darkened by H ₂ SO ₄	Passes Test	Passes Test
Water (by KF, coulometric)	<= 0.05 %	<0.01 %

For Laboratory, Research, or Manufacturing Use

MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: United States

Packaging Site: Phillipsburg Mfg Ctr & DC

Received on 7/16/25

E3956

A handwritten signature in black ink that appears to read "Jamie Croak".

Jamie Croak
Director Quality Operations, Bioscience Production

Sulfuric Acid
BAKER INSTRA-ANALYZED® Reagent
For Trace Metal Analysis
Low Selenium



M6157
B

Material No.: 9673-33

Batch No.: 24I1262013

Manufactured Date: 2024-08-07

Retest Date: 2029-08-06

Revision No.: 0

Certificate of Analysis

Test	Specification	Result
ACS - Assay (H ₂ SO ₄)	95.0 – 98.0 %	96.2 %
Appearance	Passes Test	Passes Test
ACS - Color (APHA)	<= 10	5
ACS - Residue after Ignition	<= 3 ppm	<1 ppm
ACS - Substances Reducing Permanganate(as SO ₂)	<= 2 ppm	<2 ppm
Ammonium (NH ₄)	<= 1 ppm	<1 ppm
Chloride (Cl)	<= 0.1 ppm	<0.1 ppm
Nitrate (NO ₃)	<= 0.2 ppm	0.1 ppm
Phosphate (PO ₄)	<= 0.5 ppm	<0.1 ppm
Trace Impurities - Aluminum (Al)	<= 30.0 ppb	<5.0 ppb
Arsenic & Antimony (as As)	<= 4.0 ppb	<2.0 ppb
Trace Impurities - Boron (B)	<= 10.0 ppb	<5.0 ppb
Trace Impurities - Cadmium (Cd)	<= 2.0 ppb	<1.0 ppb
Trace Impurities - Chromium (Cr)	<= 6.0 ppb	<1.0 ppb
Trace Impurities - Cobalt (Co)	<= 0.5 ppb	<0.3 ppb
Trace Impurities - Copper (Cu)	<= 1.0 ppb	<1.0 ppb
Trace Impurities - Gold (Au)	<= 10.0 ppb	<5.0 ppb
Heavy Metals (as Pb)	<= 500.0 ppb	<100.0 ppb
Trace Impurities - Iron (Fe)	<= 50.0 ppb	<1.0 ppb
Trace Impurities - Lead (Pb)	<= 0.5 ppb	<0.5 ppb
Trace Impurities - Magnesium (Mg)	<= 7.0 ppb	<1.0 ppb
Trace Impurities - Manganese (Mn)	<= 1.0 ppb	<1.0 ppb
Trace Impurities - Mercury (Hg)	<= 0.5 ppb	<0.1 ppb
Trace Impurities - Nickel (Ni)	<= 2.0 ppb	<0.3 ppb
Trace Impurities - Potassium (K)	<= 500.0 ppb	<10.0 ppb
Trace Impurities - Selenium (Se)	<= 50.0 ppb	7.2 ppb
Trace Impurities - Silicon (Si)	<= 100.0 ppb	12.8 ppb
Trace Impurities - Silver (Ag)	<= 1.0 ppb	<1.0 ppb

Sulfuric Acid
BAKER INSTRA-ANALYZED® Reagent
For Trace Metal Analysis
Low Selenium



Material No.: 9673-33
Batch No.: 24I1262013

Test	Specification	Result
Trace Impurities – Sodium (Na)	<= 500.0 ppb	<5.0 ppb
Trace Impurities – Strontium (Sr)	<= 5.0 ppb	<1.0 ppb
Trace Impurities – Tin (Sn)	<= 5.0 ppb	1.1 ppb
Trace Impurities – Zinc (Zn)	<= 5.0 ppb	<1.0 ppb

For Laboratory, Research, or Manufacturing Use

Country of Origin: United States

Packaging Site: Phillipsburg Mfg Ctr & DC

A handwritten signature in black ink that reads "Jamie Croak".

Jamie Croak
Director Quality Operations, Bioscience Production



Certificate of Analysis

P11518
↓
P11522
02/21/22

Product Name: Aroclor 1268 Standard

Product Number: PP-382-1

Lot Issue Date: 09-Feb-2021

Lot Number: 0006587800

Expiration Date: 31-Mar-2029

Description:

This analytical reference material (RM) was manufactured and verified in accordance with an ISO 9001 registered quality system and analyte concentrations were verified by an ISO 17025 accredited laboratory. The concentration and uncertainty value at the 95% confidence level for each analyte, determined gravimetrically, is listed below.

Analyte	CAS#	Analyte Lot	Concentration ± Uncertainty
Aroclor 1268	011100-14-4	RM00937	100.0 ± 0.5 µg/mL

Matrix: isoctane (2,2,4-trimethylpentane)

Storage Conditions: Store at Room Temperature (15° to 30°C).

Traceability:

The balances used for these measurements are calibrated with weights traceable to NIST in compliance with ANSI/NCSL Z540.3, ISO 9001, ISO 17025, and ISO 17034. Calibrated Class A glassware is used for volumetric measurements. Thermometers are calibrated against a NIST traceable thermometer in accordance with NIST Special Publication 1088.

Homogeneity:

This RM was unitized according to an in-house procedure and is guaranteed to be homogeneous. There is no minimum sub-sample size required.

Intended Use:

This RM is intended for the preparation of working reference samples for use in routine laboratory analyses, calibration of instruments, validation of analytical methods, assessments of measurement methods, and continuing calibration verification.

Instructions for Use:

Sample aliquots for analysis should be withdrawn at 20°C to 25°C immediately after opening the container and should be processed without delay for the certified values to be valid within the stated uncertainties.

Hazards:

Refer to the Safety Data Sheet on www.agilent.com for information regarding this RM.

Expiration of Certification:

The certification of this RM is valid until the expiration date specified above, provided the RM is handled and stored in accordance with the instructions given in this certificate. This certification is nullified if the RM is damaged, contaminated, or otherwise modified.

Maintenance of Certification:

If substantive changes are noted that affect the certification before the expiration of this certificate, Agilent will notify the purchaser.

Sample lot approver:

Monica Bourgeois
QMS Representative



ISO 17034 Cert
No. AR-1936

RM was produced in accordance with TUV USA Inc registered ISO 9001 Quality Management System. Cert # 56 100 18560026

Page: 1 of 1

www.agilent.com/quality/
CSD-QA-015.1



ISO 17025 Cert
No. AT-1937



CERTIFIED WEIGHT REPORT

Part Number:	<u>91867</u>	Solvent#	10	
Lot Number:	<u>020823</u>	Acet	11	
Description:	WP 037 - Aroclor 1232		12	
Expiration Date:	PCB Technical Mixture		13	
Recommended Storage:	020833		14	
Nominal Concentration ($\mu\text{g/mL}$):	Ambient (20 °C)		15	
NIST Test ID#:	100	Balance Uncertainty	16	
Weight(s) shown below were combined and diluted to (mL):	6UTB	0.057	Flask Uncertainty	17
	100.0			

Compound	RM#	Lot Number	Nominal Conc ($\mu\text{g/mL}$)	Purity (%)	Uncertainty Purity	Target Weight (g)
1. Aroclor 1232	17	45-6A	100	100	0.5	0.01000

- The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
- All Standards, after opening ampule, should be stored with caps tight and under appropriate laboratory conditions.
- Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurements," Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).

Comments

GC3-M1 Analysis by Melissa Storier

Column ID SPB-608 30 meter X 0.53mm X 5 μm film thickness

Flow rates: Helium (carrier) = 5mL/min, Helium (make-up) = 25mL/min


Hydrogen (make-up) = 30mL/min, Air (make-up) = 350mL/min

Oven Profile: Temp 1 = 150°C (Time 1 = 4 min), Temp 2 = 290°C (Time 2 = 13.5 min)

Rate = 8°C/min, Total run time = 35 min

Injector temp. = 200°C, FID Temp. = 300°C. FID Signal = Edaq Channel 1

Standard injection = 1.5 μL , Range=3

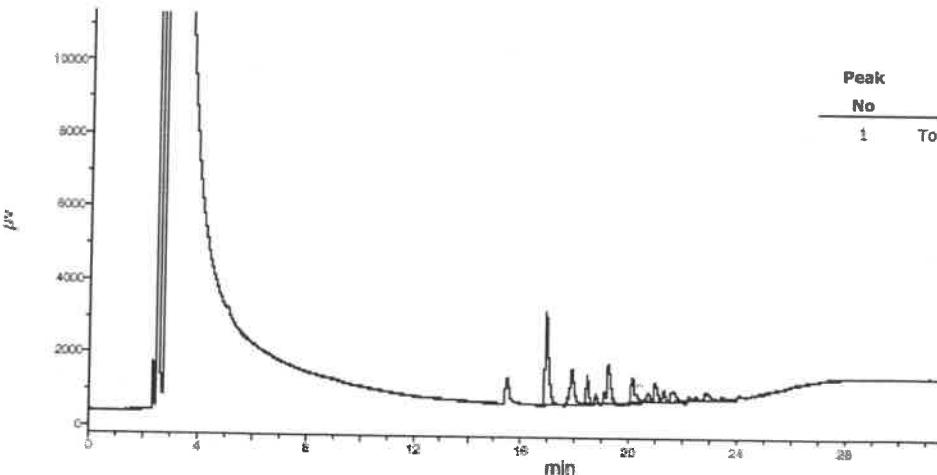



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 32009

Lot No.: A0203672

p12928

Description : Aroclor® 1242 Standard

Aroclor® 1242 Standard 1,000 µg/mL, Hexane, 1mL/ampul

↓
P 12932

Container Size : 2 mL

Pkg Amt: > 1 mL

AJ
T2 lot 123

Expiration Date : January 31, 2030

Storage: 25°C nominal

Handling: This product contains PCBs.

Ship: Ambient

C E R T I F I E D V A L U E S

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	Aroclor 1242	53469-21-9	01141	---%	1,004.7 µg/mL	+/- 55.7515

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Hexane

CAS # 110-54-3

Purity 99%

Quality Confirmation Test

Column:

30m x .25mm x .2um
Rtx-CLP II (cat.# 11323)

Carrier Gas:

helium-constant pressure 20 psi.

Temp. Program:

200°C to 300°C
@ 25°C/min. (hold 10 min.)

Inj. Temp:

250°C

Det. Temp:

300°C

Det. Type:


ECD

Split Vent:

10 ml/min.

Inj. Vol

0.2µl

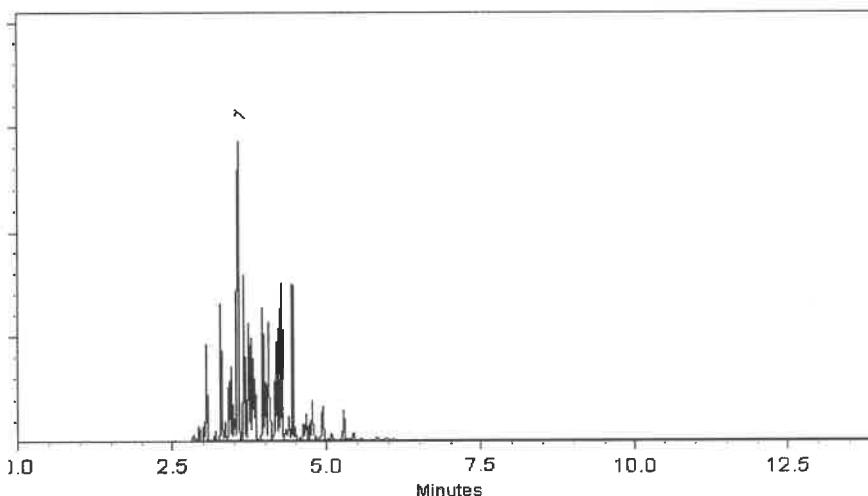

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Russ Bookhamer - Operations Technician I

Date Mixed: 26-Oct-2023 Balance Serial #: B442140311

Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 06-Nov-2023

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL



Certificate of Analysis *chromatographic plus*

FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 32010

Lot No.: A0202803

Description : Aroclor® 1248 Standard

Aroclor® 1248 Standard 1,000 μ g/mL, Hexane, 1mL/ampul

Container Size : 2 mL

Pkg Amt: > 1 mL

Expiration Date : January 31, 2030

Storage: 25°C nominal

Handling: This product contains PCBs.

Ship: Ambient

P12933
↓
P12937
AJ
12/07/23

C E R T I F I E D V A L U E S

Elation Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	Aroclor 1248	12672-29-6	13897600	---%	1,001.7 μ g/mL	+/- 55.5850

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Hexane

CAS # 110-54-3

Purity 99%

Quality Confirmation Test

Column:

30m x .25mm x .2um
Rtx-CLP II (cat.# 11323)

Carrier Gas:

helium-constant pressure 20 psi.

Temp. Program:

200°C to 300°C
@ 25°C/min. (hold 10 min.)

Inj. Temp:

250°C

Det. Temp:

300°C

Det. Type:


ECD

Split Vent:

10 ml/min.

Inj. Vol

0.2μl

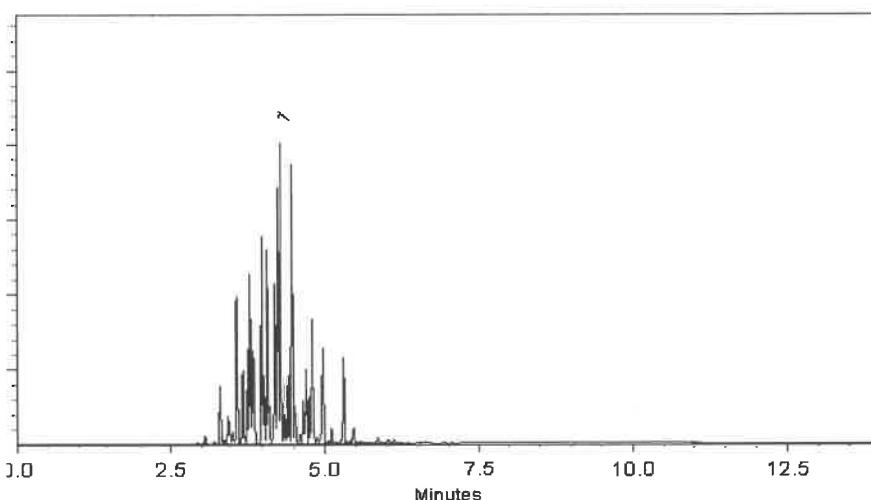

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.


Laith Clemente - Operations Technician |

Date Mixed: 03-Oct-2023 Balance Serial #: 1128360905


Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 09-Oct-2023

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397



CERTIFIED WEIGHT REPORT

Part Number: 20064
 Lot Number: 022023
 Description: CLP PCB'S - Aroclor Mix
 Aroclors 1016 & 1260
 Expiration Date: 022033
 Recommended Storage: Ambient (20 °C)
 Nominal Concentration ($\mu\text{g/mL}$): 1000
 NIST Test ID#: 6UTB
 5E-05 Balance Uncertainty
 Weight(s) shown below were combined and diluted to (mL): 200.0 0.010 Flask Uncertainty

<i>Benson Chan</i>	022023
Formulated By: <u>Benson Chan</u>	DATE
<i>Pedro L. Rentas</i>	022023
Reviewed By: <u>Pedro L. Rentas</u>	DATE


P129h6 7/19
↓ 12/19/23
P129SS

Compound	RM#	Lot Number	Nominal Conc ($\mu\text{g/mL}$)	Purity (%)	Uncertainty Purity	Target Weight(g)	Actual Weight(g)	Actual Conc ($\mu\text{g/mL}$)	Expanded Uncertainty (+/-) ($\mu\text{g/mL}$)	SDS Information		
										(Solvent Safety Info. On Attached pg.)	CAS#	OSHA PEL (TWA)
1. Aroclor 1016	15	020491JC	1000	100	0.2	0.20004	0.20060	1002.8	4.0	12674-11-2	N/A	N/A
2. Aroclor 1260	21	020491JC	1000	100	0.2	0.20004	0.20081	1003.9	4.0	11096-82-5	0.5mg/m3	oral-rat 1315mg/kg

- The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
- All Standards, after opening ampule, should be stored with caps tight and under appropriate laboratory conditions.
- Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).

Comments

GC3-M1 Analysis by Melissa Stenier
 Column ID SPB-608 30 meter X 0.53mm X5 μm film thickness
 Flow rates: Helium (carrier) = 5mL/min, Helium (make-up) = 25mL/min
 Hydrogen (make-up) = 30mL/min, Air (make-up) = 350mL/min
 Oven Profile: Temp 1 = 150°C (Time 1 = 4 min), Temp 2 = 290°C (Time 2 = 13.5 min)
 Rate = 8°C/min, Total run time = 35 min
 Injector temp. = 200°C, FID Temp. = 300°C. FID Signal = Edaq Channel 1
 Standard injection = 1.5 μL , Range=3

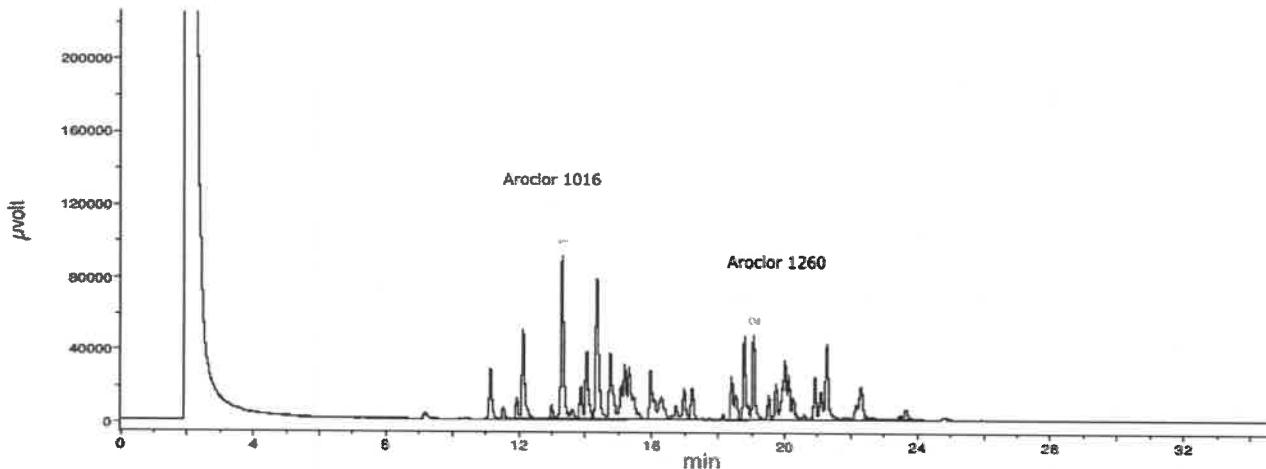



CERTIFIED WEIGHT REPORT

Part Number: 20064
 Lot Number: 022023
 Description: CLP PCB'S - Aroclor Mix
 Aroclors 1016 & 1260
 Expiration Date: 022033
 Recommended Storage: Ambient (20 °C)
 Nominal Concentration ($\mu\text{g/mL}$): 1000
 NIST Test ID#: 6UTB
 5E-05 Balance Uncertainty
 Weight(s) shown below were combined and diluted to (mL): 200.0 0.010 Flask Uncertainty

<i>Benson Chan</i>	022023
Formulated By: Benson Chan	DATE
<i>Pedro L. Rentas</i>	022023
Reviewed By: Pedro L. Rentas	DATE


P129h6 7/19
↓
12/19/23
P129SS

Compound	RM#	Lot Number	Nominal Conc ($\mu\text{g/mL}$)	Purity (%)	Uncertainty Purity	Target Weight(g)	Actual Weight(g)	Actual Conc ($\mu\text{g/mL}$)	Expanded Uncertainty (+/-) ($\mu\text{g/mL}$)	SDS Information		
										(Solvent Safety Info. On Attached pg.)	CAS#	OSHA PEL (TWA)
1. Aroclor 1016	15	020491JC	1000	100	0.2	0.20004	0.20060	1002.8	4.0	12674-11-2	N/A	N/A
2. Aroclor 1260	21	020491JC	1000	100	0.2	0.20004	0.20081	1003.9	4.0	11096-82-5	0.5mg/m3	oral-rat 1315mg/kg

- The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
- All Standards, after opening ampule, should be stored with caps tight and under appropriate laboratory conditions.
- Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).

Comments

GC3-M1 Analysis by Melissa Stenier
 Column ID SPB-608 30 meter X 0.53mm X5 μm film thickness
 Flow rates: Helium (carrier) = 5mL/min, Helium (make-up) = 25mL/min
 Hydrogen (make-up) = 30mL/min, Air (make-up) = 350mL/min
 Oven Profile: Temp 1 = 150°C (Time 1 = 4 min), Temp 2 = 290°C (Time 2 = 13.5 min)
 Rate = 8°C/min, Total run time = 35 min
 Injector temp. = 200°C, FID Temp. = 300°C. FID Signal = Edaq Channel 1
 Standard injection = 1.5 μL , Range=3

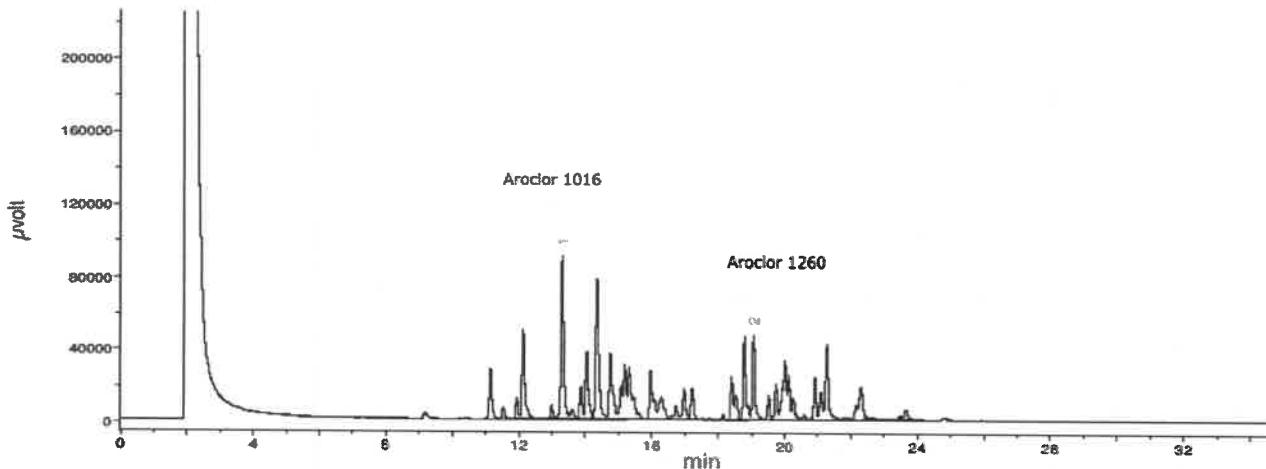



CERTIFIED WEIGHT REPORT

Part Number: 99139
Lot Number: 121823
Description: Aroclor 1254

Expiration Date: 121833
Recommended Storage: Ambient (20 °C)
Nominal Concentration ($\mu\text{g/mL}$): 100
NIST Test ID#: 6UTB

Volume(s) shown below were combined and diluted to (mL): 20.0

Note: Aroclor 1254 is a mix of isomers.

Compound	Part Number	Lot Number	Dilution Factor	Initial Vol. (mL)	Uncertainty Pipette (mL)	Initial Conc. ($\mu\text{g/mL}$)	Final Conc. ($\mu\text{g/mL}$)	Expanded Uncertainty (+/-) ($\mu\text{g/mL}$)	SDS Information (Solvent Safety Info. On Attached pg.)	CAS#	OSHA PEL (TWA)	LD50
1. Aroclor 1254	79100	121823	0.10	2.00	0.017	1003.3	100.1	1.8	11097-69-1 0.5mg/m3 (skin) oral-rat 1295mg/kg			

- The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
- All Standards, after opening ampule, should be stored with caps tight and under appropriate laboratory conditions.
- Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).

Comments

GC3-M1 Analysis by Melissa Stonier

Column ID SPB-600 30 meter X 0.53mm X5µm film thickness

Flow rates: Helium (carrier) = 5mL/min, Helium (make-up) = 25mL/min

Hydrogen (make-up) = 30mL/min, Air (make-up) = 350mL/min


Oven Profile: Temp 1 = 150°C (Time 1 = 4 min), Temp 2 = 260°C (Time 2 = 13.5 min)

Rate = 8°C/min. Total run time = 35 min

Injector temp. = 200°C, FID Temp. = 300°C. FID Signal = Edaq Channel 1

Standard injection = 1.5µL, Range=3

Peak No.	Name	FID RT (min.)
1	Total Aroclor 1254	18.12

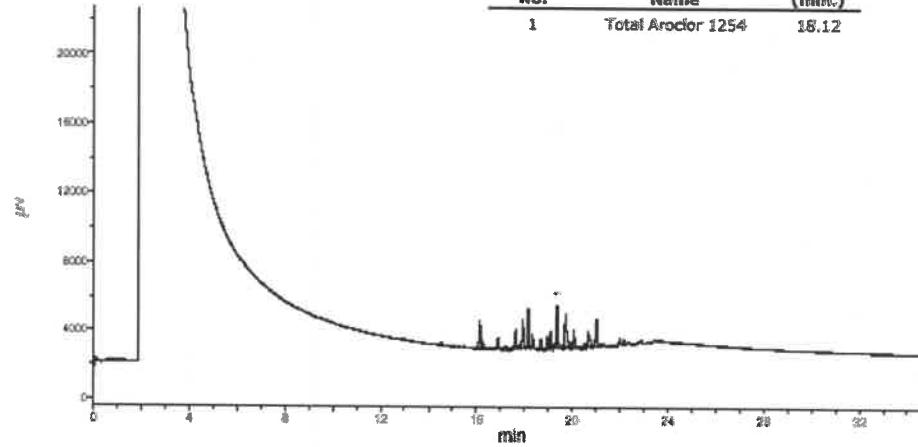



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL



Certificate of Analysis

chromatographic plus

FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No.: 32000

Lot No.: A0206810

Description: Pesticide Surrogate Mix

Pesticide Surrogate Mix 200 µg/mL, Acetone, 1mL/ampul

Container Size: 2 mL

Pkg Amt: > 1 mL

Expiration Date: April 30, 2030

Storage: 10°C or colder

Handling: Contains PCBs - sonicate prior to use.

Ship: Ambient

P13348
P13357
DAU
04/25/2024

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	2,4,5,6-Tetrachloro-m-xylene	877-09-8	RP220407	99%	200.3 µg/mL	+/- 11.1143
2	Decachlorobiphenyl (BZ# 209)	2051-24-3	30638	99%	200.6 µg/mL	+/- 11.1298

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Acetone

CAS # 67-64-1
Purity 99%

Tech Tips:

Decachlorobiphenyl has poor solubility in most organic solvents. The maximum concentration that can be prepared in acetone, hexane, or isoctane is 200µg/mL. Temperature will affect the solubility as well. Storing solutions at reduced temperatures will cause decachlorobiphenyl to precipitate.

Products containing decachlorobiphenyl must be sonicated for a minimum of 10 minutes prior to opening the ampul. Because each ultrasonic bath operates at a different energy level, 10 minutes is a guideline only. Longer sonication time will not affect product quality.

These precautions apply to working solutions prepared in your laboratory as well. The amount of compound that precipitates depends on concentration AND temperature. If you store your standards at a temperature lower than 4°C (even dilute solutions), allow extra sonication time.

Quality Confirmation Test

Column:30m x .25mm x .2um
Rtx-CLP II (cat.# 11323)**Carrier Gas:**

helium-constant pressure 20 psi.

Temp. Program:200°C to 300°C
@ 25°C/min. (hold 10 min.)**Inj. Temp:**

250°C

Det. Temp:

300°C

Det. Type:


ECD

Split Vent:

10 ml/min.

Inj. Vol


1µl

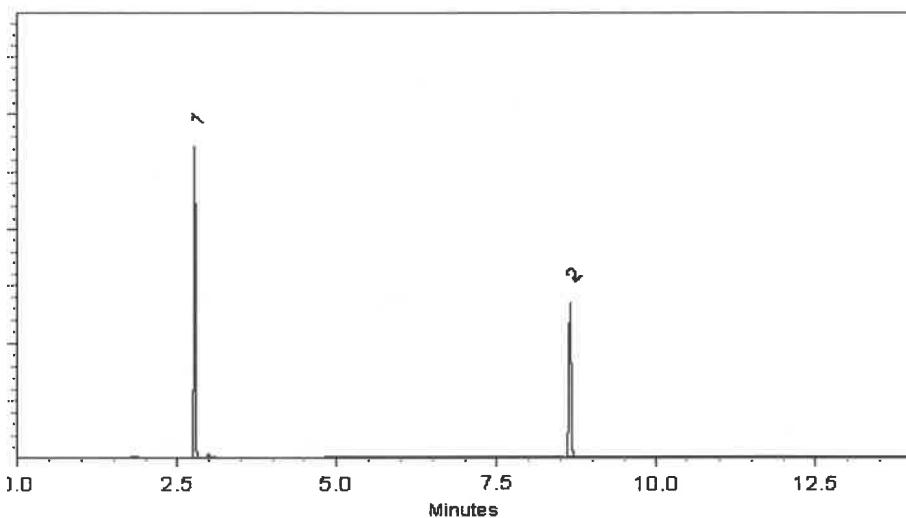

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.


Laith Clemente - Operations Technician I


Date Mixed: 22-Jan-2024 Balance Serial #: 1128360905


Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 24-Jan-2024

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

P 13348
↓
P 13357
S AUF
04/25/2025



Trusted Answers

ISO 17034

Reference Material Certificate

Product Information Sheet

Product Name:	Aroclor 1221 Standard	Lot Number:	0006783205
Product Number:	PP-292-1	Lot Issue Date:	20-Feb-2024
Storage Conditions:	Store at Room Temperature (15° to 30°C).	Expiration Date:	31-Mar-2032

Component Name	Concentration	Uncertainty	CAS#	Analyte Lot
Aroclor 1221	100.3 ± 0.5 µg/mL		011104-28-2	NT01017

Matrix: isoctane (2,2,4-trimethylpentane)

Description:

This document is prepared in accordance with ISO 17034 and Guide 31. This analytical reference material standard was manufactured and verified in accordance with an ISO 9001 registered quality system and analyte concentrations were verified by an ISO 17025 accredited laboratory. The concentration and uncertainty value at the 95% confidence level for each analyte, determined gravimetrically, is listed above.

Traceability:

The balances used for these measurements are calibrated with weights traceable to NIST in compliance with ANSI/NCSL Z540.3, ISO 9001, ISO 17025, and ISO 17034. Calibrated Class A glassware is used for volumetric measurements. Thermometers are calibrated against a NIST traceable thermometer in accordance with NIST Special Publication 1088.

Homogeneity:

This analytical reference standard was unitized according to an in-house procedure and is guaranteed to be homogeneous. There is no minimum sub-sample size required.

Instructions for Use:

Sample aliquots for analysis should be withdrawn at 20°C to 25°C immediately after opening the container and should be processed without delay for the certified values to be valid within the stated uncertainties.

Safety:

Refer to the Safety Data Sheet on www.agilent.com for information regarding this analytical reference material.

Intended Use:

This analytical reference standard is intended for the preparation of working reference samples for use in routine laboratory analyses, calibration of instruments, validation of analytical methods, assessments of measurement methods, and continuing calibration verification.

Expiration of Certification:

The certification of this analytical reference standard is valid until the expiration date specified above, provided the material is handled and stored in accordance with the instructions given in this certificate. This certification is nullified if the material is damaged, contaminated, or otherwise modified.

P133f2

↓

AJ
05106124

Page: 1 of 2

CSD-QA-015.2

ISO 17025
Cert No. AT-1937

250 Smith Street North Kingstown, Rhode Island 02852 www.agilent.com/quality

**Maintenance of Certification:**

If substantive changes are noted that affect the certification before the expiration of this certificate, Agilent will notify the purchaser.

Sample lot approver:

Monica Bourgeois
QMS Representative



ISO 17034
Cert No. AR-1936

RM was produced in accordance with the TUV/SUD registered ISO
9001:2015 Quality Management System. Cert# 951215321
Page: 2 of 2
www.agilent.com/quality/
CSD-QA-015.2

ISO 17025
Cert No. AT-1937

250 Smith Street North Kingstown, Rhode Island 02852 www.agilent.com/quality



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL



ILAC-MRA
ACCREDITED
ISO 17034 Accredited
Reference Material Producer
Certificate #3222.01



ILAC-MRA
ACCREDITED
ISO/IEC 17025 Accredited
Testing Laboratory
Certificate #3222.02

Certificate of Analysis *chromatographic plus*

FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No.: 32410

Lot No.: A0207475

Description: Aroclor® 1268 Standard

Aroclor® 1268 Standard 1,000 µg/mL, 1mL/ampul, Hexane

Container Size: 2 mL

Pkg Amt: > 1 mL

Expiration Date: May 31, 2030

Storage: 25°C nominal

Handling: This product contains PCBs.

Ship: Ambient

C E R T I F I E D V A L U E S

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	Aroclor 1268	11100-14-4	10947000	----%	1,000.0 µg/mL	+/- 55.4925

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Hexane
CAS # 110-54-3
Purity 99%

P 13386
P 13381
J. STANFORD
05/01/2024

Quality Confirmation Test

Column:

30m x .25mm x .2um
Rtx-CLP II (cat.# 11323)

Carrier Gas:

helium-constant pressure 20 psi.

Temp. Program:

200°C to 300°C
@ 25°C/min. (hold 10 min.)

Inj. Temp:

250°C

Det. Temp:

300°C

Det. Type:


ECD

Split Vent:

Split ratio 500:1

Inj. Vol

0.2µl

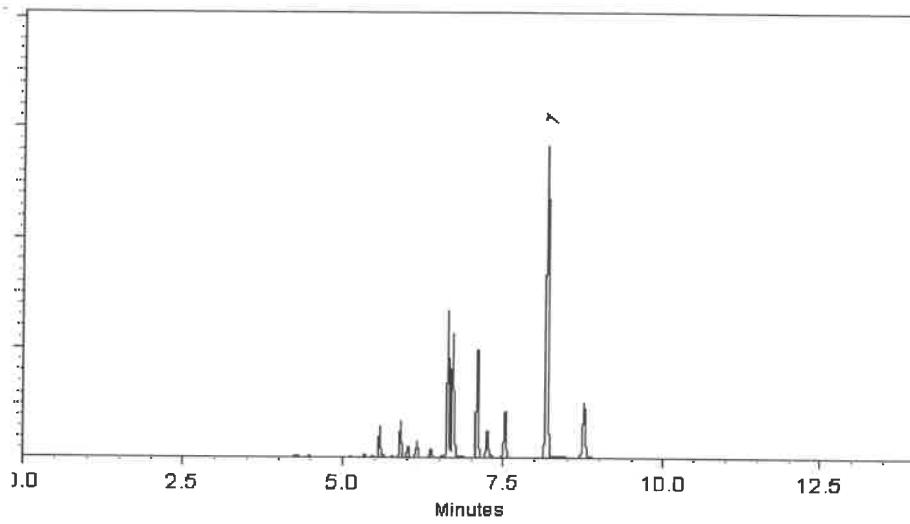

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

michael maye
Michael Maye - Operations Tech I


Date Mixed: 06-Feb-2024 Balance Serial #: B442140311

Dillan Murphy
Dillan Murphy - Operations Technician I

Date Passed: 09-Feb-2024

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

P13380
↓
P13381
②
Dated 05/6/2024



Reference Material Certificate

Product Name: Aroclor 1242 Standard **Lot Number:** 0006665550
Product Number: PP-312-1 **Lot Issue Date:** 08-Feb-2022
Storage Conditions: Store at Room Temperature (15° to 30°C). **Expiration Date:** 31-Jan-2027

Component Name	CERTIFIED VALUES			CAS#	Analyte Lot
	Concentration	Expanded Uncertainty			
Aroclor 1242	100.4	± 0.5 µg/mL		053469-21-9	NT01020

Matrix: isoctane (2,2,4-trimethylpentane)

Description:

This document is prepared in accordance with ISO 17034 and Guide 31. This analytical reference material standard was manufactured and verified in accordance with an ISO 9001 registered quality system and analyte concentrations were verified by an ISO 17025 accredited laboratory. The concentration and uncertainty value at the 95% confidence level for each analyte, determined gravimetrically, is listed above.

Traceability:

The balances used for these measurements are calibrated with weights traceable to NIST in compliance with ANSI/NCSL Z540.3, ISO 9001, ISO 17025, and ISO 17034. Calibrated Class A glassware is used for volumetric measurements. Thermometers are calibrated against a NIST traceable thermometer in accordance with NIST Special Publication 1088.

Homogeneity:

This analytical reference standard was unitized according to an in-house procedure and is guaranteed to be homogeneous. There is no minimum sub-sample size required.

Instructions for Use:

Sample aliquots for analysis should be withdrawn at 20°C to 25°C immediately after opening the container and should be processed without delay for the certified values to be valid within the stated uncertainties.

Safety:

Refer to the Safety Data Sheet on www.agilent.com for information regarding this analytical reference material.

Intended Use:


This analytical reference standard is intended for the preparation of working reference samples for use in routine laboratory analyses, calibration of instruments, validation of analytical methods, assessments of measurement methods, and continuing calibration verification.

Expiration of Certification:

The certification of this analytical reference standard is valid until the expiration date specified above, provided the material is handled and stored in accordance with the instructions given in this certificate. This certification is nullified if the material is damaged, contaminated, or otherwise modified.

p13589
↓
p13590

AJ
10/11/12/14

**Maintenance of Certification:**

If substantive changes are noted that affect the certification before the expiration of this certificate, Agilent will notify the purchaser.

Sample lot approver:

Monica Bourgeois
QMS Representative



ISO 17034 Cert
No. AR-1936

RM was produced in accordance with the TUV/SUD registered ISO 9001:2015
Quality Management System. Cert# 951215321

Page: 2 of 2

www.agilent.com/quality/

CSD-QA-015.1



ISO 17025
Cert No. AT-

Reference Material Certificate
Product Information Sheet

Product Name: Aroclor 1248 Standard

Lot Number: 0006726317

Product Number: PP-342-1

Lot Issue Date: 27-Jan-2023

Storage Conditions: Store at Room Temperature (15° to 30°C).

Expiration Date: 28-Feb-2031

Component Name	Concentration	Uncertainty	CAS#	Analyte Lot
Aroclor 1248	100.3	± 0.5 µg/mL	012672-29-6	NT01582

Matrix: isoctane (2,2,4-trimethylpentane)

Description:

This document is prepared in accordance with ISO 17034 and Guide 31. This analytical reference material (RM) standard was manufactured and verified in accordance with an ISO 9001 registered quality system and analyte concentrations were verified by an ISO 17025 accredited laboratory. The concentration and uncertainty value at the 95% confidence level for each analyte, determined gravimetrically, is listed above. Purity values are taken from approved vendor raw material certificates.

Traceability:

The balances used for these measurements are calibrated with weights traceable to NIST in compliance with ANSI/NCSL Z540.3, ISO 9001, ISO 17025, and ISO 17034. Calibrated Class A glassware is used for volumetric measurements. Thermometers are calibrated against a NIST traceable thermometer in accordance with NIST Special Publication 1088.

Homogeneity:

This analytical reference (RM) standard was unitized according to an in-house procedure and is guaranteed to be homogeneous. There is no minimum sub-sample size required.

Instructions for Use:

Sample aliquots for analysis should be withdrawn at 20°C to 25°C immediately after opening the container and should be processed without delay for the certified values to be valid within the stated uncertainties.

Safety:

Refer to the Safety Data Sheet on www.agilent.com for information regarding this analytical reference material.

Intended Use:

This analytical reference (RM) standard is intended for the preparation of working reference samples for use in routine laboratory analyses, calibration of instruments, validation of analytical methods, assessments of measurement methods, and continuing calibration verification.

Expiration of Certification:

The certification of this analytical reference standard (RM) is valid until the expiration date specified above, provided the material is handled and stored in accordance with the instructions given in this certificate. This certification is nullified if the material is damaged, contaminated, or otherwise modified.

P13591

↓


P13592

AJ
10/14/2024

**Maintenance of Certification:**

If substantive changes are noted that affect the certification before the expiration of this certificate, Agilent will notify the purchaser.

Sample lot approver:


Monica Bourgeois
QMS Representative



ISO 17034 Cert
No. AR-1936

RM was produced in accordance with the TUV/SUD registered ISO
9001:2015 Quality Management System. Cert# 951215321

Page: 2 of 2

www.agilent.com/quality/
CSD-QA-015.1

ISO 17025



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL



ISO 17034 Accredited
Reference Material Producer
Certificate #3222.01



ISO/IEC 17025 Accredited
Testing Laboratory
Certificate #3222.02

Certificate of Analysis *chromatographic plus*

FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 32039

Lot No.: A0210629

P13697
↓
P13701 } Y.P.
} 10/19/24

Description : Aroclor® 1016/1260 Mix

Aroclor® 1016/1260 Mix 1,000 µg/mL, Hexane, 1mL/ampul

Container Size : 2 mL

Pkg Amt: > 1 mL

Expiration Date : July 31, 2030

Storage: 25°C nominal

Handling: This product contains PCBs.

Ship: Ambient

C E R T I F I E D V A L U E S

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	Aroclor 1016	12674-11-2	07	----%	1,005.3 µg/mL	+/- 55.7809
2	Aroclor 1260	11096-82-5	1320657	----%	1,000.0 µg/mL	+/- 55.4850

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Hexane

CAS # 110-54-3

Purity 99%

Quality Confirmation Test

Column:

30m x .25mm x .2um
Rtx-CLP II (cat.# 11323)

Carrier Gas:

helium-constant pressure 20 psi.

Temp. Program:

200°C to 300°C
@ 25°C/min. (hold 10 min.)

Inj. Temp:

250°C

Det. Temp:

300°C

Det. Type:


ECD

Split Vent:

10 ml/min.

Inj. Vol


0.2µl

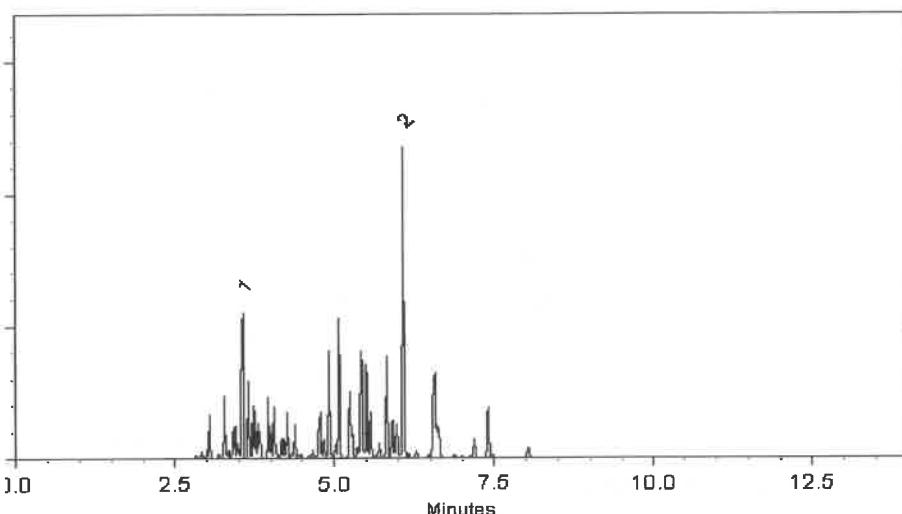

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.


Laith Clemente - Operations Technician I

Date Mixed: 22-Apr-2024 Balance Serial #: B442140311


Dillon Murphy - Operations Technician I

Date Passed: 24-Apr-2024

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/ μ ECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{\text{combined uncertainty}} = k \sqrt{u_{\text{gravimetric}}^2 + u_{\text{homogeneity}}^2 + u_{\text{storage stability}}^2 + u_{\text{shipping stability}}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL



Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No.: 32007

Lot No.: A0215270

Description: Aroclor® 1221 Standard

Aroclor® 1221 Standard 1,000 µg/mL, Hexane, 1mL/ampul

Container Size: 2 mL

Pkg Amt: > 1 mL

Expiration Date: November 30, 2030

Storage: 25°C nominal

Handling: This product contains PCBs.

Ship: Ambient

P13902 }
P13903 } Y.P.
10/17/24

C E R T I F I E D V A L U E S

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	Aroclor 1221	11104-28-2	14969200	----%	1,005.0 µg/mL	+/- 55.7700

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Hexane
CAS # 110-54-3
Purity 99%

Quality Confirmation Test

Column:

30m x .25mm x .2um
Rtx-CLP II (cat.# 11323)

Carrier Gas:

helium-constant pressure 20 psi.

Temp. Program:

200°C to 300°C
@ 25°C/min. (hold 10 min.)

Inj. Temp:

250°C

Det. Temp:

300°C

Det. Type:


ECD

Split Vent:

10 ml/min.

Inj. Vol

1µl

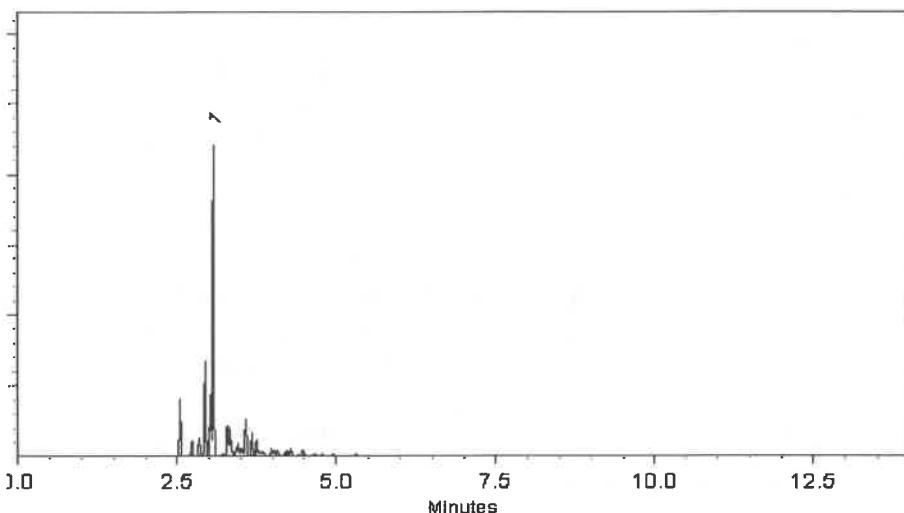

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

michael maye
Michael Maye - Operations Tech I

Date Mixed: 16-Aug-2024 Balance Serial #: 1128360905

Jennifer Pollino
Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 20-Aug-2024

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{\text{combined uncertainty}} = k \sqrt{u_{\text{gravimetric}}^2 + u_{\text{homogeneity}}^2 + u_{\text{storage stability}}^2 + u_{\text{shipping stability}}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL



Certificate of Analysis

chromatographic plus

FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 32000

Lot No.: A0214495

Description : Pesticide Surrogate Mix

Pesticide Surrogate Mix 200 µg/mL, Acetone, 1mL/ampul

Container Size : 2 mL

Pkg Amt: > 1 mL

Expiration Date : October 31, 2030

Storage: 10°C or colder

Handling: Contains PCBs - sonicate prior to use.

Ship: Ambient

p19785

J

AJ
11/19/24

p19789

11/19/24

C E R T I F I E D V A L U E S

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	2,4,5,6-Tetrachloro-m-xylene	877-09-8	RP220407	99%	200.2 µg/mL	+/- 11.1087
2	Decachlorobiphenyl (BZ# 209)	2051-24-3	30679	99%	201.4 µg/mL	+/- 11.1753

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Acetone

CAS # 67-64-1

Purity 99%

Tech Tips:

Decachlorobiphenyl has poor solubility in most organic solvents. The maximum concentration that can be prepared in acetone, hexane, or isoctane is 200µg/mL. Temperature will affect the solubility as well. Storing solutions at reduced temperatures will cause decachlorobiphenyl to precipitate.

Products containing decachlorobiphenyl must be sonicated for a minimum of 10 minutes prior to opening the ampul. Because each ultrasonic bath operates at a different energy level, 10 minutes is a guideline only. Longer sonication time will not affect product quality.

These precautions apply to working solutions prepared in your laboratory as well. The amount of compound that precipitates depends on concentration AND temperature. If you store your standards at a temperature lower than 4°C (even dilute solutions), allow extra sonication time.

Quality Confirmation Test

Column:

30m x .25mm x .2um
Rtx-CLP II (cat.# 11323)

Carrier Gas:

helium-constant pressure 20 psi.

Temp. Program:

200°C to 300°C
@ 25°C/min. (hold 10 min.)

Inj. Temp:

250°C

Det. Temp:

300°C

Det. Type:


ECD

Split Vent:

10 ml/min.

Inj. Vol

1µl

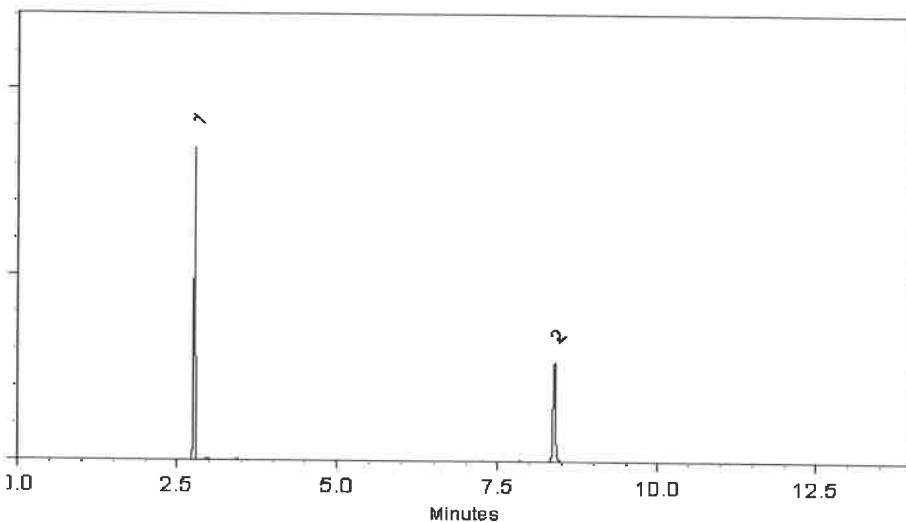

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Aaron Enyart
Aaron Enyart - Operations Tech I

Date Mixed: 29-Jul-2024 Balance Serial #: B345965662

Jennifer Pollino
Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 01-Aug-2024

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL



21
ISO 17034 Accredited
Reference Material Producer
Certificate #3222.01



22
ISO/IEC 17025 Accredited
Testing Laboratory
Certificate #3222.02

Certificate of Analysis *chromatographic plus*

FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 32011

Lot No.: A0217391

Description : Aroclor® 1254 Standard

Aroclor® 1254 Standard 1,000 µg/mL, Hexane, 1mL/ampul

Container Size : 2 mL

Pkg Amt: > 1 mL

Expiration Date : January 31, 2031

Storage: 25°C nominal

Handling: This product contains PCBs.

Ship: Ambient

C E R T I F I E D V A L U E S

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	Aroclor 1254	11097-69-1	124-191-B	----%	1,004.7 µg/mL	+/- 55.7515

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Hexane

CAS # 110-54-3

Purity 99%

P13830
↓
P13832 12/09/24 AJ

Quality Confirmation Test

Column:30m x .25mm x .2um
Rtx-CLP II (cat.# 11323)**Carrier Gas:**

helium-constant pressure 20 psi.

Temp. Program:200°C to 300°C
@ 25°C/min. (hold 10 min.)**Inj. Temp:**

250°C

Det. Temp:

300°C

Det. Type:


ECD

Split Vent:

300 ml/min.

Inj. Vol

1µl

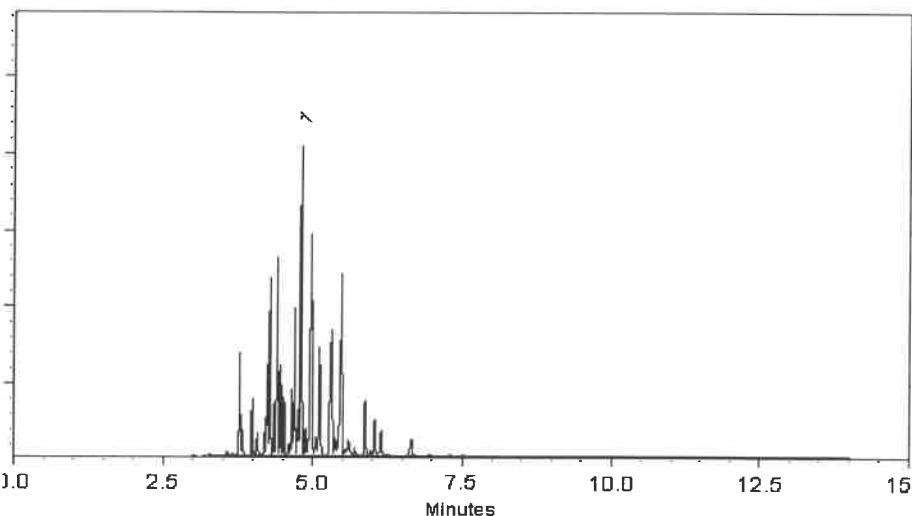

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

michael maye
Michael Maye - Operations Tech I

Date Mixed: 02-Oct-2024 Balance Serial #: C322230531

Jennifer Pollino
Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 07-Oct-2024

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 32008

Lot No.: A0219655

Description : Aroclor® 1232 Standard

Aroclor® 1232 Standard 1,000 µg/mL, Hexane, 1mL/ampul

Container Size : 2 mL

Pkg Amt: > 1 mL

Expiration Date : March 31, 2031

Storage: 25°C nominal

Handling: This product contains PCBs.

Ship: Ambient

C E R T I F I E D V A L U E S

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	Aroclor 1232	11141-16-5	15665-01	----%	1,007.0 µg/mL	+/- 55.8810

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Hexane

CAS # 110-54-3

Purity 99%

p13878
↓
p13860

AJ
01/28/25

Quality Confirmation Test

Column:30m x .25mm x .2um
Rtx-CLP II (cat.# 11323)**Carrier Gas:**

helium-constant pressure 20 psi.

Temp. Program:200°C to 300°C
@ 25°C/min. (hold 10 min.)**Inj. Temp:**

250°C

Det. Temp:

300°C

Det. Type:


ECD

Split Vent:

10 ml/min.

Inj. Vol

1μl

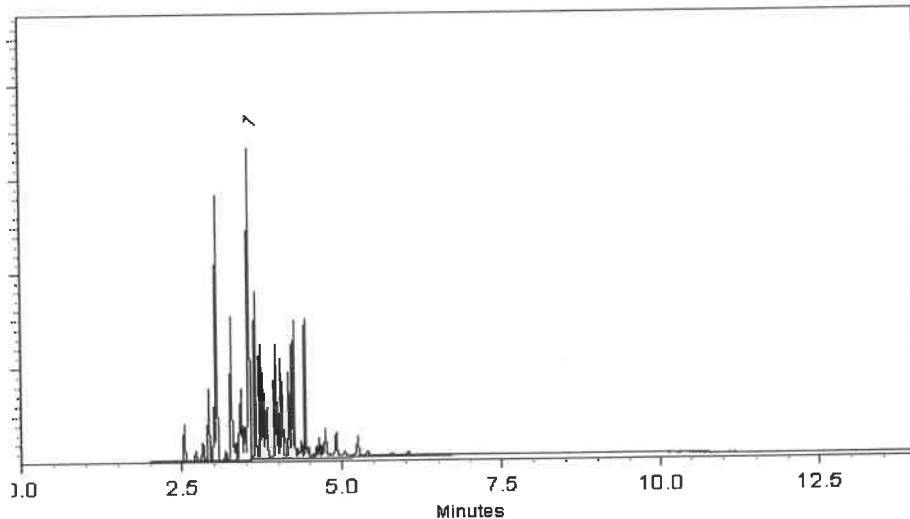

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

michael maye
Michael Maye - Operations Tech I

Date Mixed: 02-Dec-2024 Balance Serial #: C322230531

Brittany Federinko
Brittany Federinko - Operations Tech I

Date Passed: 05-Dec-2024

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



ILAC-MRA
ACCREDITED
ISO 17034 Accredited
Reference Material Producer
Certificate #3222.01



ILAC-MRA
ACCREDITED
ISO/IEC 17025 Accredited
Testing Laboratory
Certificate #3222.02

FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No.: 32409

Lot No.: A0220950

Description : Aroclor® 1262 Standard

Aroclor® 1262 Standard 1,000 µg/mL, 1mL/ampul, Hexane

Container Size : 2 mL

Pkg Amt: > 1 mL

Expiration Date : April 30, 2031

Storage: 25°C nominal

Handling: This product contains PCBs.

Ship: Ambient

C E R T I F I E D V A L U E S

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	Aroclor 1262	37324-23-5	10849100	----%	1,002.0 µg/mL	+/- 55.6035

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Hexane

CAS # 110-54-3

Purity 99%

P13882

↓

AJ
01/28/25

P13883

Quality Confirmation Test

Column:

30m x .25mm x .2um

Rtx-CLP II (cat.# 11323)

Carrier Gas:

helium-constant pressure 20 psi.

Temp. Program:

200°C to 300°C

@ 25°C/min. (hold 10 min.)

Inj. Temp:

250°C

Det. Temp:

300°C

Det. Type:


ECD

Split Vent:

300 ml/min.

Inj. Vol

0.2µl

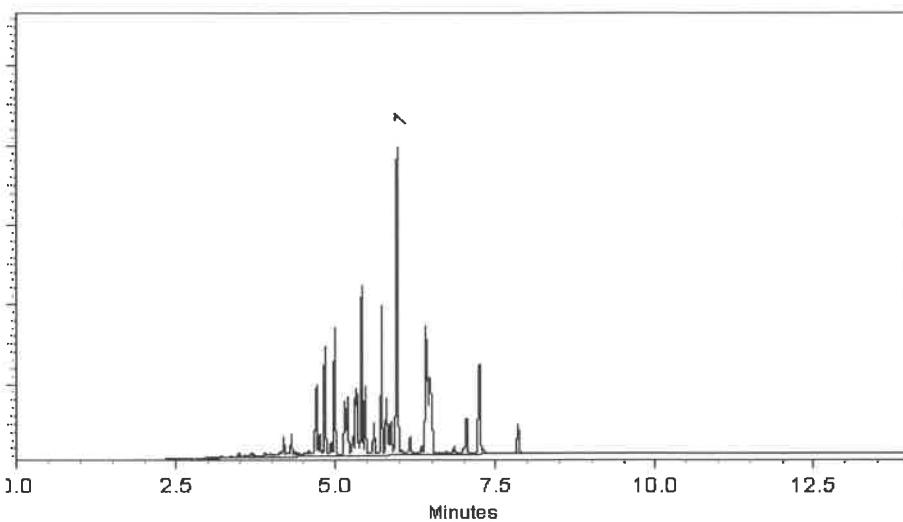

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.


Tom Suckar - Mix Technician

Date Mixed: 09-Jan-2025 Balance Serial #: C322230531


Brittany Federinko - Operations Tech I

Date Passed: 14-Jan-2025

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

n-Hexane 95%
ULTRA RESI-ANALYZED
For Organic Residue Analysis



Material No.: 9262-03
Batch No.: 24G1962003
Manufactured Date: 2024-05-23
Expiration Date: 2025-08-22
Revision No.: 0

W314X
W314X
CPLTE. 02/03/2023
SP

Certificate of Analysis

Test	Specification	Result
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	≤ 5	3
ECD Sensitive Impurities (as Heptachlor Epoxide) Single Peak (pg/mL)	≤ 10	1
ECD-Sensitive Impurities (as Ethylene Dibromide) - Single Impurity Peak (ng/mL)	≤ 5	1
Assay (Total Saturated C ₆ Isomers) (by GC, corrected for water)	≥ 99.5 %	99.7 %
Assay (as n-Hexane) (by GC, corrected for water)	≥ 95 %	98 %
Color (APHA)	≤ 10	5
Residue after Evaporation	≤ 1.0 ppm	0.1 ppm
Substances Darkened by H ₂ SO ₄	Passes Test	Passes Test
Water (by KF, coulometric)	≤ 0.05 %	< 0.01 %

For Laboratory, Research, or Manufacturing Use
MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: USA
Packaging Site: Phillipsburg Mfg Ctr & DC

A handwritten signature in black ink, appearing to read 'Jamie Croak'.

Jamie Croak

Director Quality Operations, Biosciences

802 of 1148n



SHIPPING DOCUMENTS

1
2
3
4
5
6
7
8
9
10
11
12
13
14
15
16
17
18
19
20

Chemtech

Phone: (908) 789-8900
Fax: (908) 789-8922

284 Sheffield Street, Mountainside, NJ 07092

Company Name: Nobis Group

Address: 55 Technology Dr Suite 101, Lowell, MA 01851

Phone: 978-703-6014

Project Name: Raymark

Project Location: Stratford, CT

Project Number: 95700

Project Manager: Adam Roy

Con-Test Quote Name/Number:

Invoice Recipient:

Sampled By: A. Brittingham

CHAIN OF CUSTODY RECORD

39 Spruce Street
East Longmeadow, MA 01028

		Requested Turnaround Time		Dissolved Metals Samples		ANALYSIS REQUESTED										Preservation Code													
5-Day	<input type="checkbox"/>	10-Day	<input checked="" type="checkbox"/>	<input type="radio"/>	Field Filtered	M/O	I	I	I	I	I	I	I	I	I		I	Total Number Of:											
PFAS 10-Day (std)	<input type="checkbox"/>	Due Date:		<input type="radio"/>	Lab to Filter												VIALS _____												
		Rush Approval Required		Orthophosphate Samples													GLASS _____												
		1-Day	<input type="checkbox"/>	3-Day	<input type="checkbox"/>	<input type="radio"/>	Field Filtered										PLASTIC _____												
		2-Day	<input type="checkbox"/>	4-Day	<input type="checkbox"/>	<input type="radio"/>	Lab to Filter										BACTERIA _____												
		Date Delivery																		ENCORE _____									
		Format:	PDF <input checked="" type="checkbox"/>	EXCEL <input checked="" type="checkbox"/>	PCB ONLY																								
		Other:	SOXHLET <input checked="" type="checkbox"/>																Glassware in the fridge? Y / N										
		CLP Like Data Pkg Required:	<input type="checkbox"/>	No	NON SOXHLET <input type="checkbox"/>															Glassware in freezer? Y / N									
		Email To:	aroy@nobis-group.com																Prepackaged Cooler? Y / N										
		Fax To #:																	*Contest is not responsible for missing samples from prepacked coolers										
Con-Test Work Order#	Client Sample ID / Description	Beginning Date/Time	Ending Date/Time	COMP/GRAB	¹ Matrix Code	Conc Code	VIALS	GLASS	PLASTIC	BACTERIA	ENCORE	RCP VOCs	% Solids	PAHs	Herbicides	Pesticides	PCBs	Metals ICP + Hg - 6010	Cyanide	SPLP RCP Metals - 6020									
OU4-TS-38-071725	7/17/25	11:40	G	SO			3	2				X	X	X	X	X	X	X	X										
OU4-TS-39-071725	7/17/25	11:50	G	SO			3	2				X	X	X	X	X	X	X	X										
OU4-TS-40-071725	7/17/25	12:00	G	SO			3	2				X	X	X	X	X	X	X	X										
OU4-TS-41-071725	7/17/25	12:10	G	SO			3	2				X	X	X	X	X	X	X	X										
OU4-TS-42-071725	7/17/25	12:20	G	SO			3	2				X	X	X	X	X	X	X	X										
OU4-TS-43-071725	7/17/25	12:30	G	SO			3	2				X	X	X	X	X	X	X	X										
OU4-TS-44-071725	7/17/25	12:40	G	SO			3	2				X	X	X	X	X	X	X	X										
Relinquished by: (signature)	Date/Time: 7/17/25 1500	Client Comments:																											
Received by: (signature)	Date/Time: 7/17/25 0955																												
Relinquished by: (signature)	Date/Time:	Detection Limit Requirements				Special Requirements										Please use the following codes to indicate possible sample concentration within the Conc Code column above: H - High; M - Medium; L - Low; C - Clean; U - Unknown													
Received by: (signature)	Date/Time:	MA	<input type="checkbox"/>	MA MCP Required																									
Relinquished by: (signature)	Date/Time:	CT	<input checked="" type="checkbox"/>	CT RCP Required																									
Received by: (signature)	Date/Time:	Other:	<input type="checkbox"/>	MA State DW Required																									
Relinquished by: (signature)	Date/Time:	Project Entity																		NELAC and AIHA-LAP, LLC Accredited									
Received by: (signature)	Date/Time:																			Government <input type="checkbox"/>	Municipality <input type="checkbox"/>	MWRA <input type="checkbox"/>	WRTA <input type="checkbox"/>	Other <input type="checkbox"/>	Chromatogram <input type="checkbox"/>				
Received by: (signature)	Date/Time:																			Federal <input type="checkbox"/>	21 J <input type="checkbox"/>	School <input type="checkbox"/>		AIHA-LAP, LLC <input type="checkbox"/>					
Lab Comments:	Disclaimer: Con-Test Labs is not responsible for any omitted information on the Chain of Custody. The Chain of Custody is a legal document that must be complete and accurate and is used to determine what analyses the laboratory will perform. Any missing information is not the laboratory's responsibility. Con-Test values your partnership on each project and will try to assist with missing information, but will not be held accountable.																												

Laboratory Certification

Certified By	License No.
CAS EPA CLP Contract	68HERH20D0011
Connecticut	PH-0830
DOD ELAP (ANAB)	L2219
Maine	2024021
Maryland	296
New Hampshire	255424 Rev 1
New Jersey	20012
New York	11376
Pennsylvania	68-00548
Soil Permit	525-24-234-08441
Texas	T104704488

1
2
3
4
5
6
7
8
9
10
11
12
13
14
15
16
17
18
19
20

LOGIN REPORT/SAMPLE TRANSFER

Order ID :	Q2639	NOBI03	Order Date :	7/18/2025 10:22:00 AM	Project Mgr :	
Client Name :	Nobis Group		Project Name :	Raymark Superfund Site		
Client Contact :	Adam Roy		Receive DateTime :	7/18/2025 9:55:00 AM		
Invoice Name :	Nobis Group		Purchase Order :			
Invoice Contact :	Adam Roy		Hard Copy Date :			
			Date Signoff :			

LAB ID	CLIENT ID	MATRIX	SAMPLE DATE	SAMPLE TIME	TEST	TEST GROUP	METHOD	FAX DATE	DUE DATES
Q2639-01	OU4-TS-38-071725	Solid	07/17/2025	11:40	VOCMS Group3		8260D	10 Bus. Days	
Q2639-03	OU4-TS-39-071725	Solid	07/17/2025	11:50	VOCMS Group3		8260D	10 Bus. Days	
Q2639-05	OU4-TS-40-071725	Solid	07/17/2025	12:00	VOCMS Group3		8260D	10 Bus. Days	
Q2639-07	OU4-TS-41-071725	Solid	07/17/2025	12:10	VOCMS Group3		8260D	10 Bus. Days	
Q2639-09	OU4-TS-42-071725	Solid	07/17/2025	12:20	VOCMS Group3		8260D	10 Bus. Days	
Q2639-11	OU4-TS-43-071725	Solid	07/17/2025	12:30	VOCMS Group3		8260D	10 Bus. Days	
Q2639-13	OU4-TS-44-071725	Solid	07/17/2025	12:40	VOCMS Group3		8260D	10 Bus. Days	

LOGIN REPORT/SAMPLE TRANSFER

Order ID :	Q2639	NOBI03	Order Date :	7/18/2025 10:22:00 AM	Project Mgr :
Client Name :	Nobis Group		Project Name :	Raymark Superfund Site	
Client Contact :	Adam Roy		Receive DateTime :	7/18/2025 9:55:00 AM	Report Type :
Invoice Name :	Nobis Group		Purchase Order :		EDD Type :
Invoice Contact :	Adam Roy				Hard Copy Date :
					Date Signoff :

LAB ID	CLIENT ID	MATRIX	SAMPLE DATE	SAMPLE TIME	TEST	TEST GROUP	METHOD	FAX DATE	DUE DATES

Relinquished By : 
 Date / Time : 7/18/25 1100

Received By : 
 Date / Time : 07/18/25 11:00 EJ#6
FZL
 Storage Area : VOA Refrigerator Room

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0070825\
 Data File : P0112088.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jul 2025 14:06
 Operator : YP/AJ
 Sample : AR1660ICC1000
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1660ICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 08 15:11:12 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 08 15:05:13 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	3.671	3.666	1065.4E6	678.6E6	100.030	99.492
2) SA Decachlor...	8.702	8.650	709.2E6	145.2E6	99.363	82.863

Target Compounds

3) L1 AR-1016-1	4.759	4.743	360.7E6	224.7E6	1002.967	1009.911
4) L1 AR-1016-2	4.777	4.761	524.8E6	333.7E6	997.596	990.816
5) L1 AR-1016-3	4.834	4.937	332.8E6	170.0E6	996.764	978.505
6) L1 AR-1016-4	4.954	4.980	267.1E6	133.5E6	996.410	973.937
7) L1 AR-1016-5	5.211	5.191	281.3E6	173.0E6	1001.444	970.770
31) L7 AR-1260-1	6.249	6.220	515.3E6	274.0E6	991.090	981.321
32) L7 AR-1260-2	6.438	6.409	755.5E6	339.5E6	994.979	991.780
33) L7 AR-1260-3	6.805	6.560	672.8E6	271.1E6	982.211	938.011
34) L7 AR-1260-4	7.065	7.031	428.5E6	190.3E6	967.221	967.353
35) L7 AR-1260-5	7.308	7.272	1355.3E6	439.4E6	1014.259	981.589



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0070825\
 Data File : P0112088.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jul 2025 14:06
 Operator : YP/AJ
 Sample : AR1660ICC1000
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1660ICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 08 15:11:12 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 08 15:05:13 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

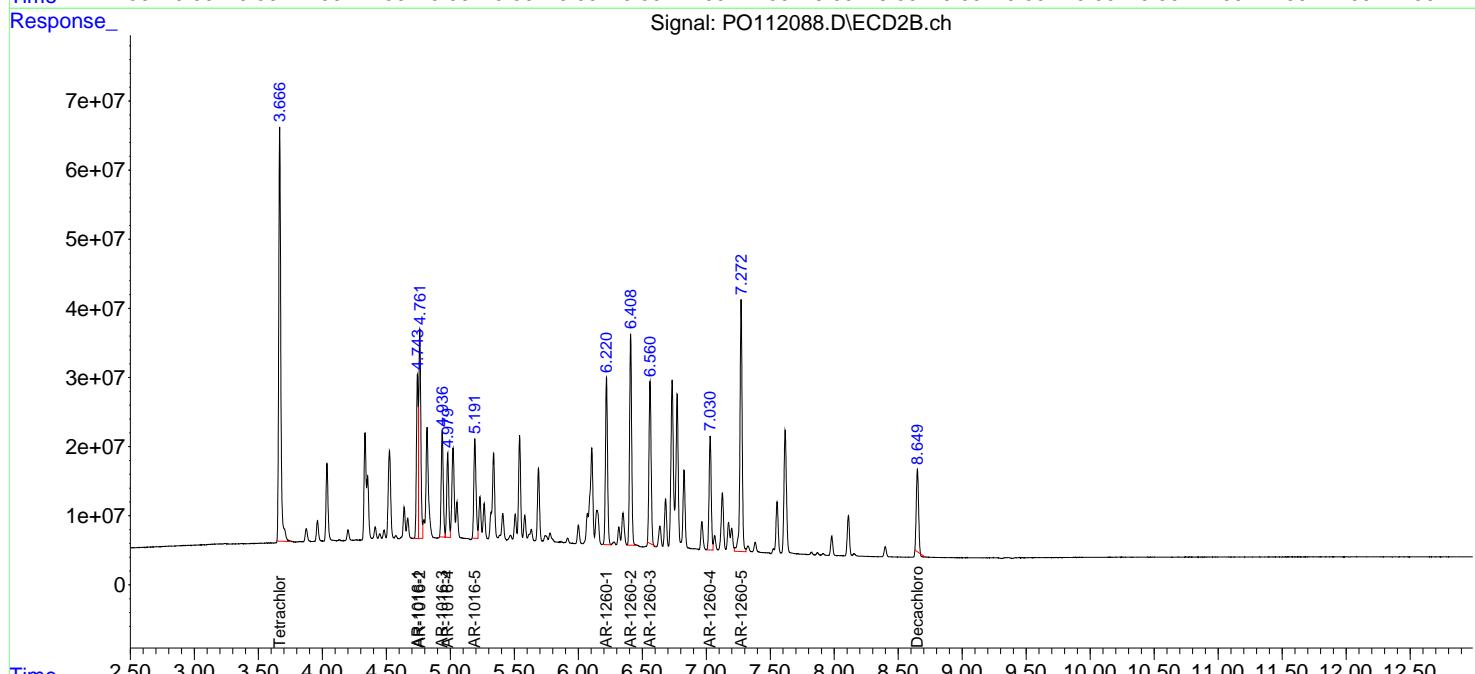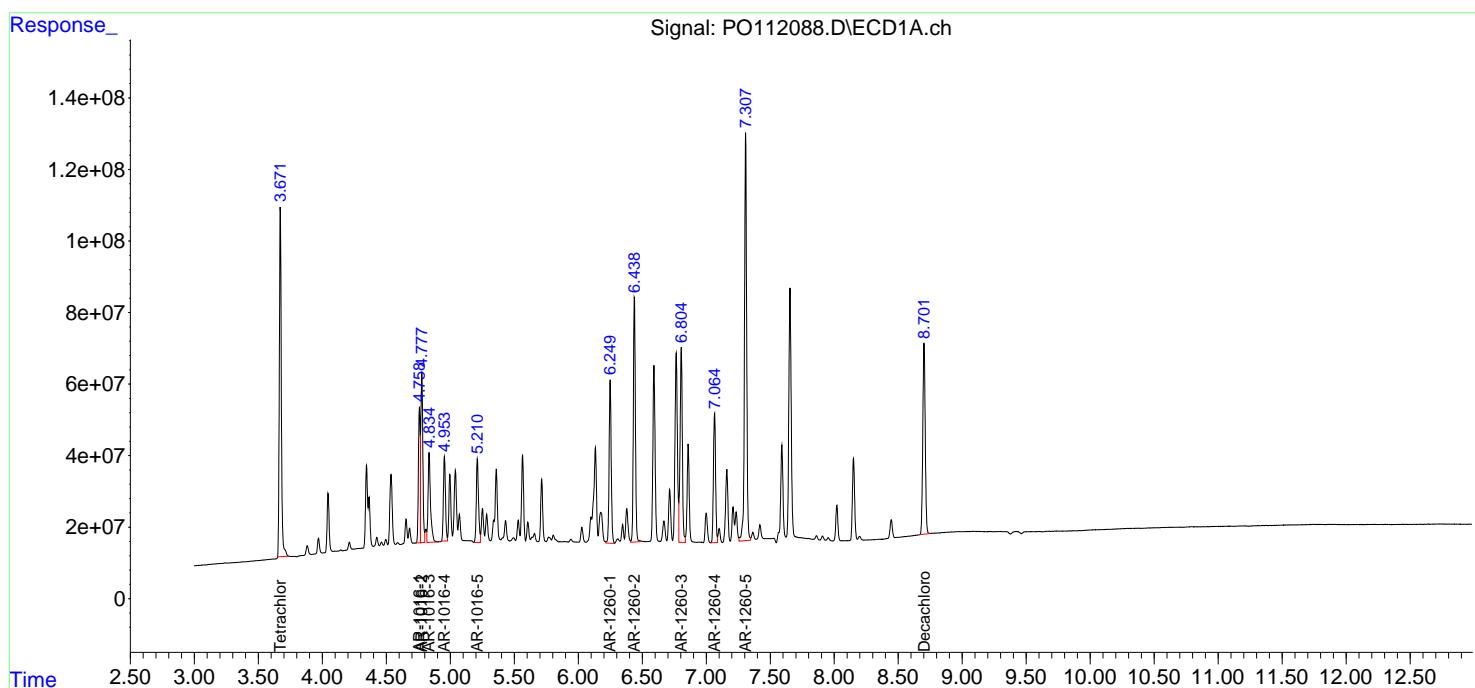

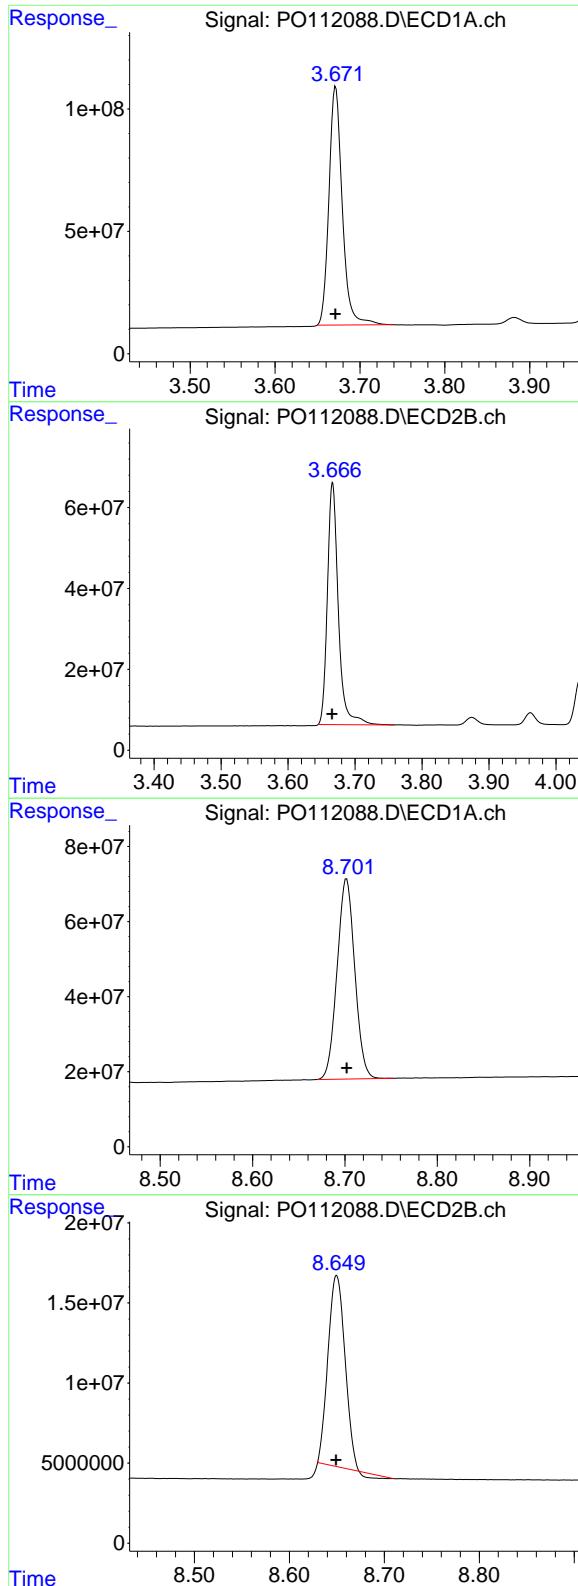

#1 Tetrachloro-m-xylene

R.T.: 3.671 min
 Delta R.T.: 0.000 min
 Response: 1065391349
 Conc: 100.03 ng/ml

Instrument:

ECD_O

ClientSampleId :
 AR1660ICC1000

#1 Tetrachloro-m-xylene


R.T.: 3.666 min
 Delta R.T.: 0.000 min
 Response: 678623932
 Conc: 99.49 ng/ml

#2 Decachlorobiphenyl

R.T.: 8.702 min
 Delta R.T.: 0.000 min
 Response: 709169575
 Conc: 99.36 ng/ml

#2 Decachlorobiphenyl

R.T.: 8.650 min
 Delta R.T.: 0.000 min
 Response: 145220382
 Conc: 82.86 ng/ml

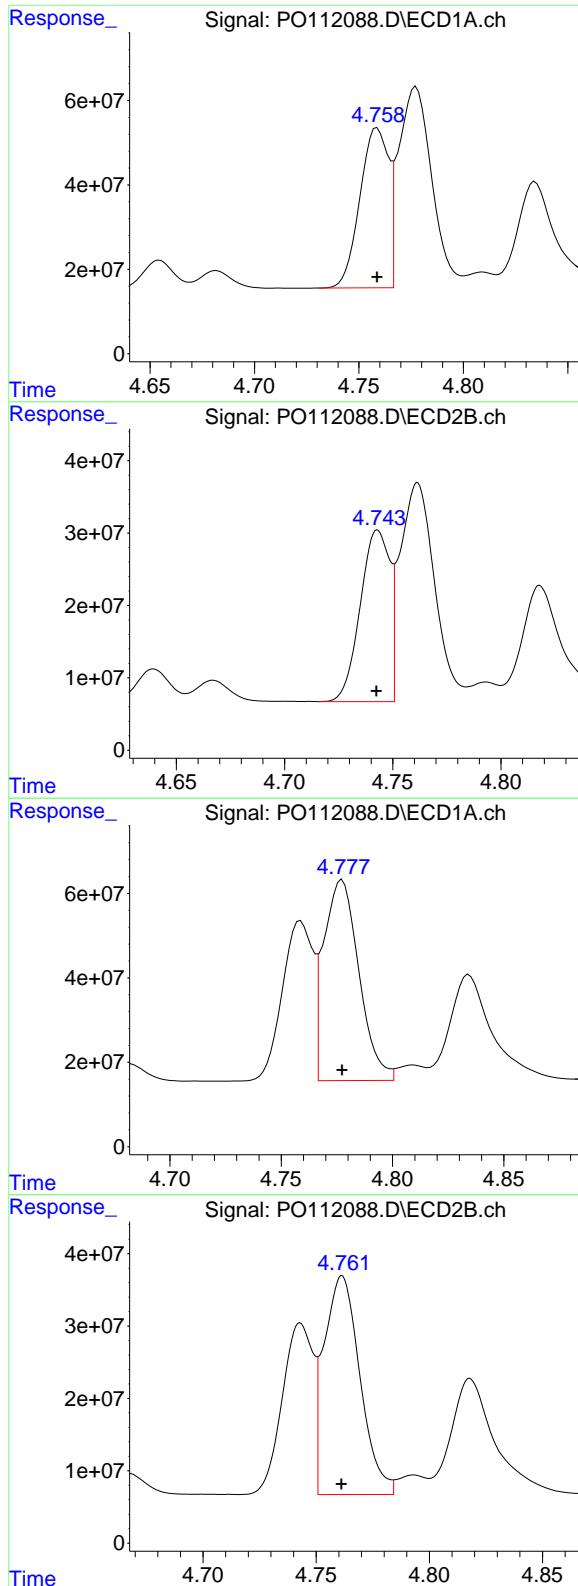

#3 AR-1016-1

R.T.: 4.759 min
 Delta R.T.: 0.000 min
 Response: 360742355
 Conc: 1002.97 ng/ml

Instrument: ECD_O
 ClientSampleId: AR1660ICC1000

#3 AR-1016-1


R.T.: 4.743 min
 Delta R.T.: 0.000 min
 Response: 224689947
 Conc: 1009.91 ng/ml

#4 AR-1016-2

R.T.: 4.777 min
 Delta R.T.: 0.000 min
 Response: 524757576
 Conc: 997.60 ng/ml

#4 AR-1016-2

R.T.: 4.761 min
 Delta R.T.: 0.000 min
 Response: 333676696
 Conc: 990.82 ng/ml

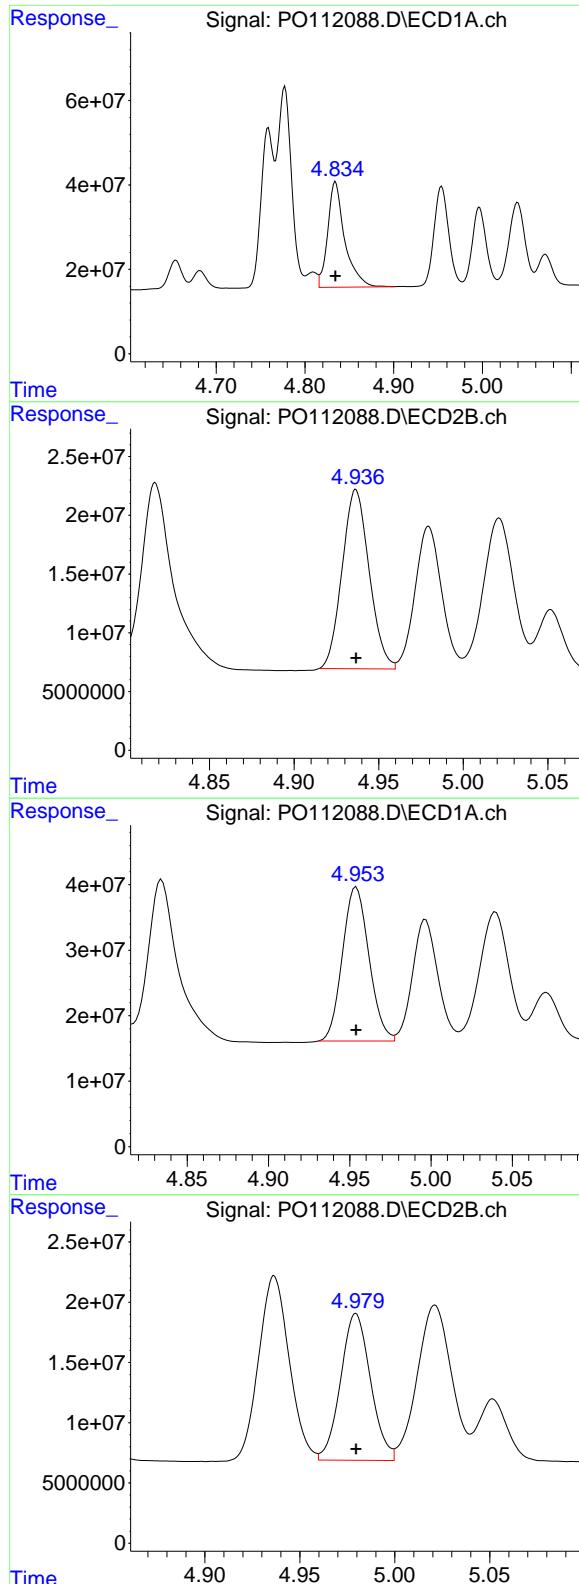

#5 AR-1016-3

R.T.: 4.834 min
 Delta R.T.: 0.000 min
 Response: 332829086
 Conc: 996.76 ng/ml

Instrument: ECD_O
 ClientSampleId : AR1660ICC1000

#5 AR-1016-3


R.T.: 4.937 min
 Delta R.T.: 0.000 min
 Response: 170039672
 Conc: 978.50 ng/ml

#6 AR-1016-4

R.T.: 4.954 min
 Delta R.T.: 0.000 min
 Response: 267114546
 Conc: 996.41 ng/ml

#6 AR-1016-4

R.T.: 4.980 min
 Delta R.T.: 0.000 min
 Response: 133548654
 Conc: 973.94 ng/ml

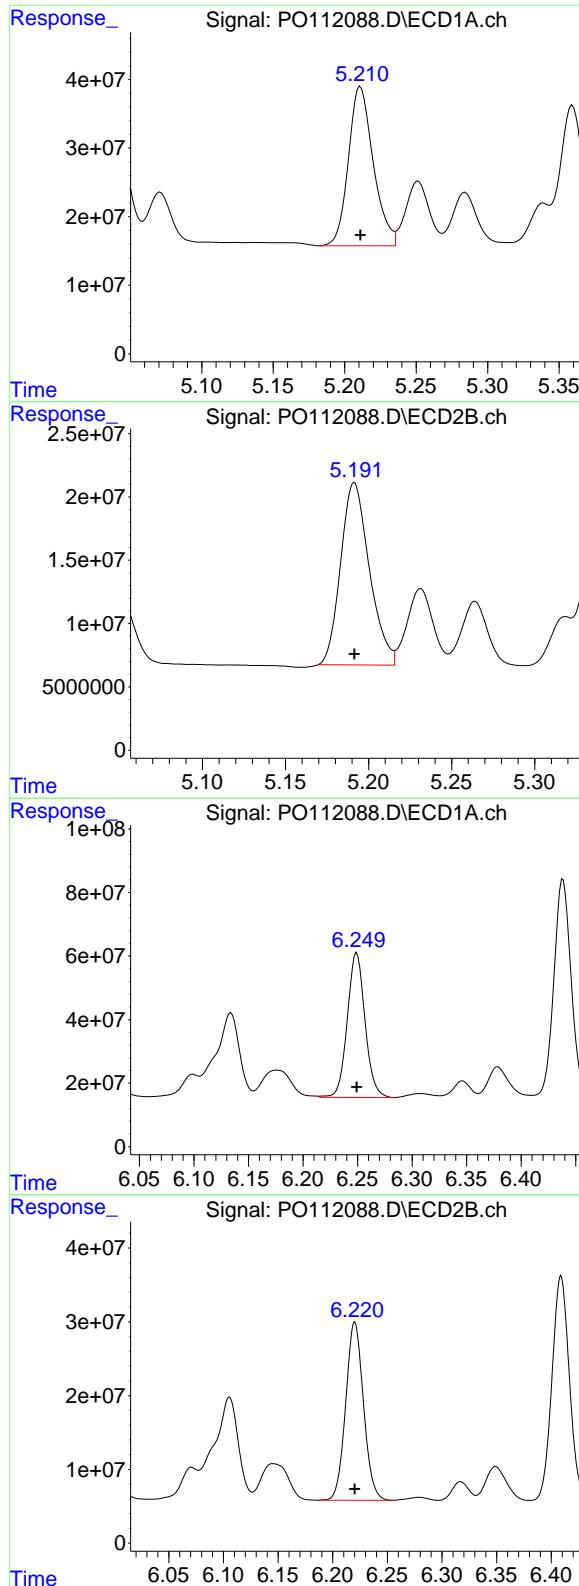

#7 AR-1016-5

R.T.: 5.211 min
 Delta R.T.: 0.000 min
Instrument:
 Response: 281257689 ECD_O
 Conc: 1001.44 ng/ml
ClientSampleId :
 AR1660ICC1000

#7 AR-1016-5


R.T.: 5.191 min
 Delta R.T.: 0.000 min
 Response: 172958737
 Conc: 970.77 ng/ml

#31 AR-1260-1

R.T.: 6.249 min
 Delta R.T.: 0.000 min
 Response: 515263930
 Conc: 991.09 ng/ml

#31 AR-1260-1

R.T.: 6.220 min
 Delta R.T.: 0.000 min
 Response: 273966572
 Conc: 981.32 ng/ml

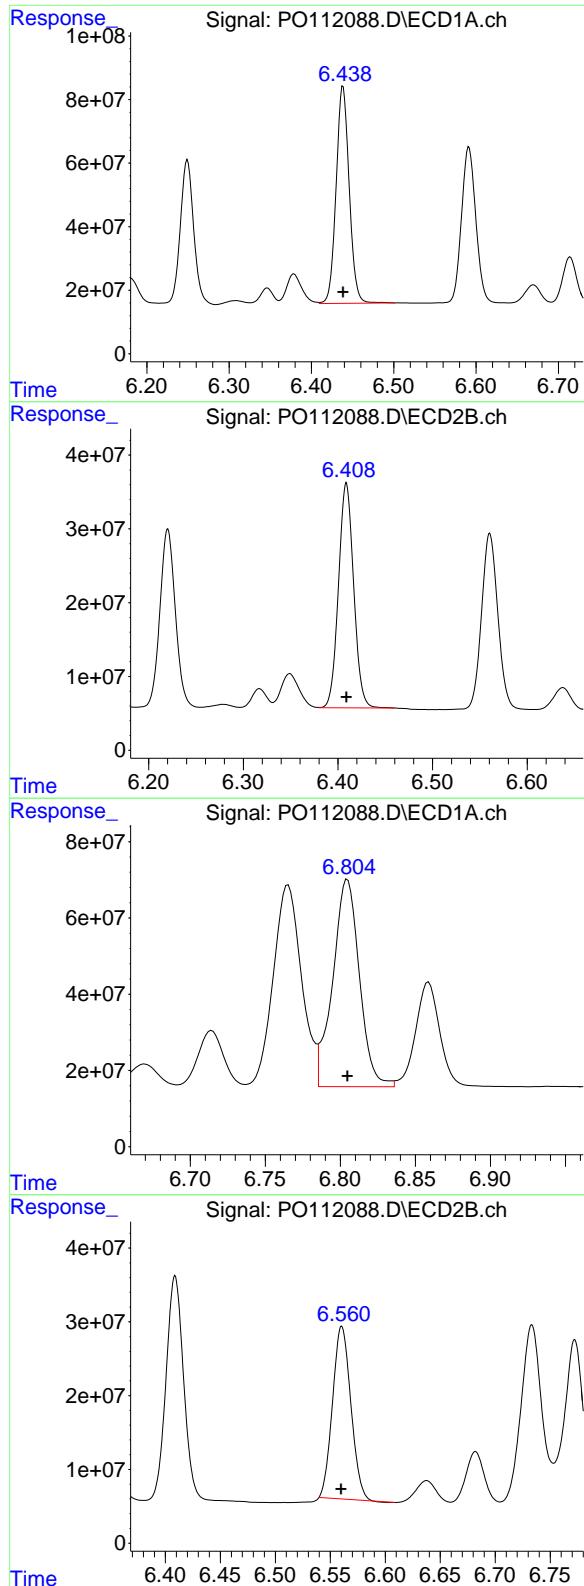

#32 AR-1260-2

R.T.: 6.438 min
 Delta R.T.: 0.000 min
 Response: 755458656
 Conc: 994.98 ng/ml

Instrument: ECD_O
ClientSampleId: AR1660ICC1000

#32 AR-1260-2


R.T.: 6.409 min
 Delta R.T.: 0.000 min
 Response: 339471861
 Conc: 991.78 ng/ml

#33 AR-1260-3

R.T.: 6.805 min
 Delta R.T.: 0.000 min
 Response: 672764264
 Conc: 982.21 ng/ml

#33 AR-1260-3

R.T.: 6.560 min
 Delta R.T.: 0.000 min
 Response: 271095387
 Conc: 938.01 ng/ml

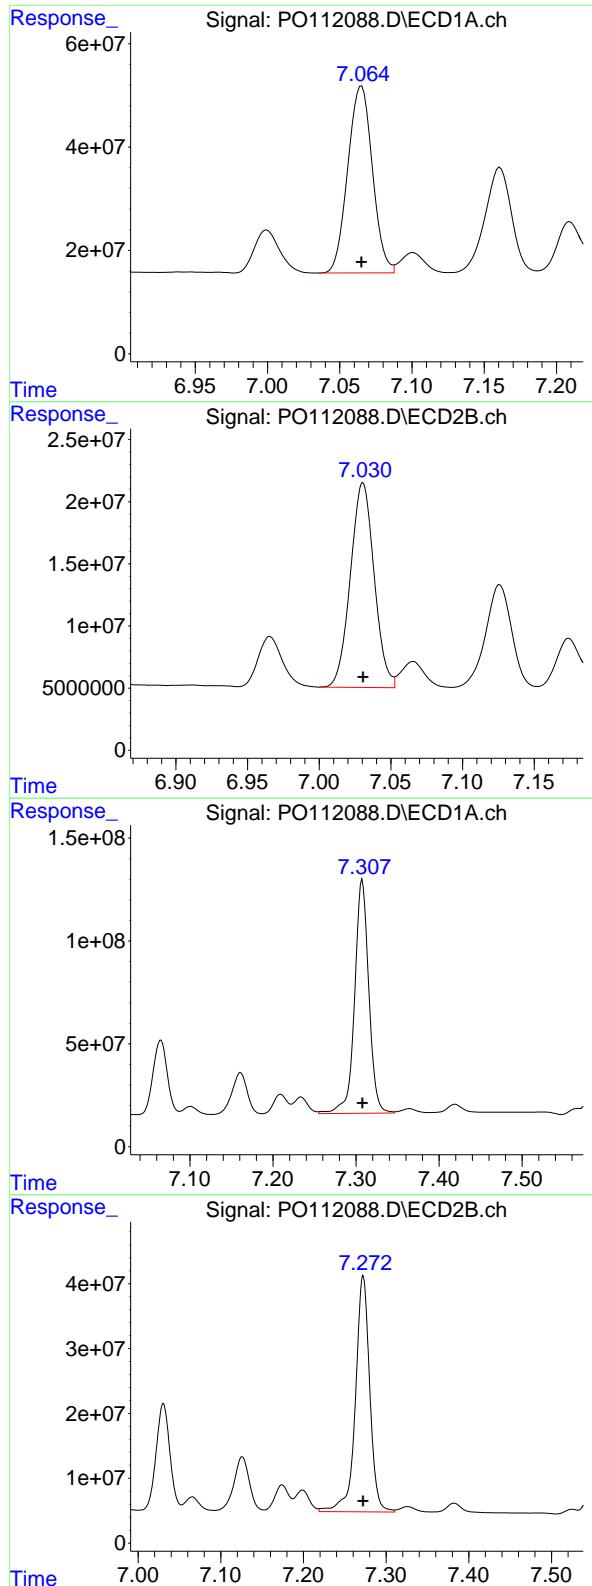

#34 AR-1260-4

R.T.: 7.065 min
Delta R.T.: 0.000 min **Instrument:**
Response: 428461498 ECD_O
Conc: 967.22 ng/ml **ClientSampleId:**
AR1660ICC1000

#34 AR-1260-4

R.T.: 7.031 min
Delta R.T.: 0.000 min
Response: 190320237
Conc: 967.35 ng/ml

#35 AR-1260-5

R.T.: 7.308 min
Delta R.T.: 0.000 min
Response: 1355306152
Conc: 1014.26 ng/ml

#35 AR-1260-5

R.T.: 7.272 min
Delta R.T.: 0.000 min
Response: 439428363
Conc: 981.59 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0070825\
 Data File : P0112089.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jul 2025 14:25
 Operator : YP/AJ
 Sample : AR1660ICC750
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1660ICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 08 15:14:45 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 08 15:05:13 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	3.673	3.666	782.4E6	495.9E6	73.811	73.003
2) SA Decachlor...	8.704	8.650	536.0E6	117.1E6	75.070	66.913

Target Compounds

3) L1 AR-1016-1	4.761	4.743	265.1E6	165.9E6	741.241	736.514
4) L1 AR-1016-2	4.780	4.762	385.3E6	249.7E6	738.229	743.699
5) L1 AR-1016-3	4.837	4.937	243.8E6	126.3E6	736.557	729.877
6) L1 AR-1016-4	4.956	4.979	197.7E6	99974022	741.523	735.926
7) L1 AR-1016-5	5.213	5.192	204.1E6	129.1E6	734.329	732.695
31) L7 AR-1260-1	6.252	6.221	385.5E6	206.7E6	744.352	743.536
32) L7 AR-1260-2	6.441	6.409	563.9E6	254.9E6	745.065	746.483
33) L7 AR-1260-3	6.808	6.561	509.8E6	203.6E6	746.212	709.489
34) L7 AR-1260-4	7.067	7.031	332.1E6	145.8E6	749.812	743.946
35) L7 AR-1260-5	7.309	7.273	1000.2E6	336.4E6	749.018	750.945



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0070825\
 Data File : P0112089.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jul 2025 14:25
 Operator : YP/AJ
 Sample : AR1660ICC750
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1660ICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 08 15:14:45 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 08 15:05:13 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

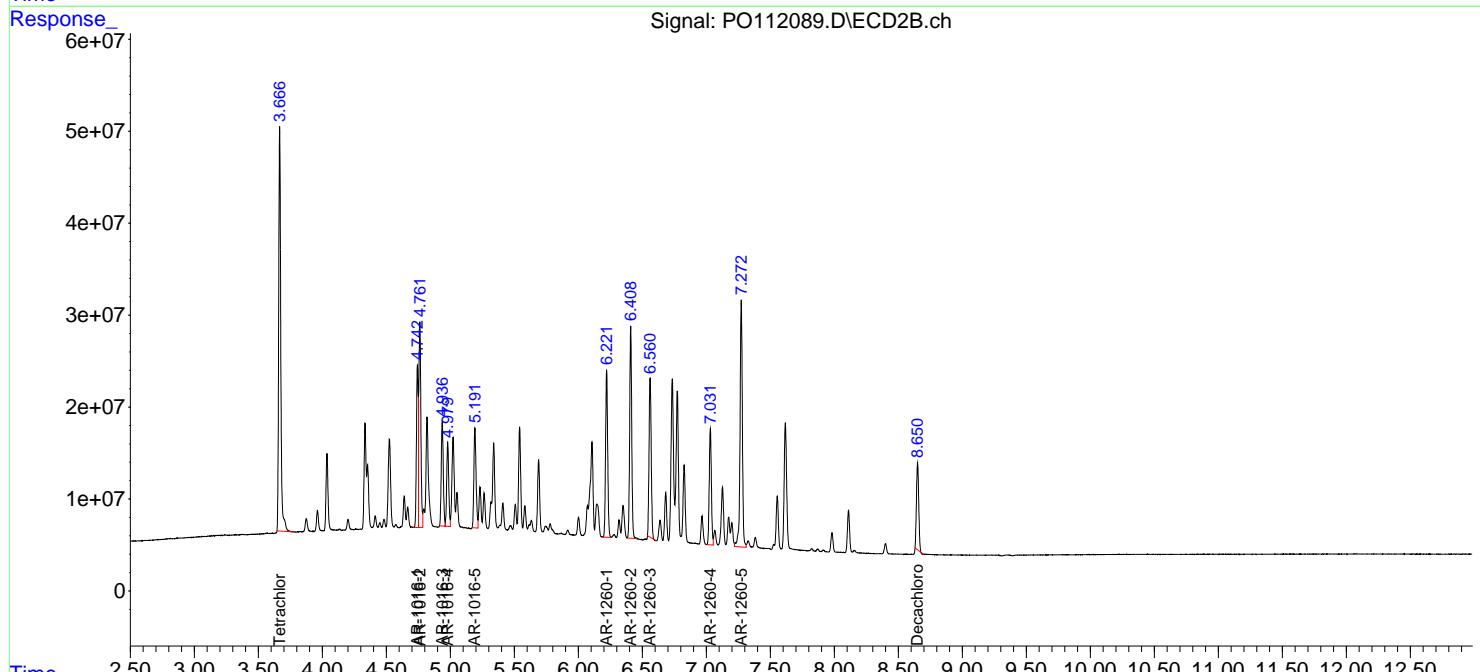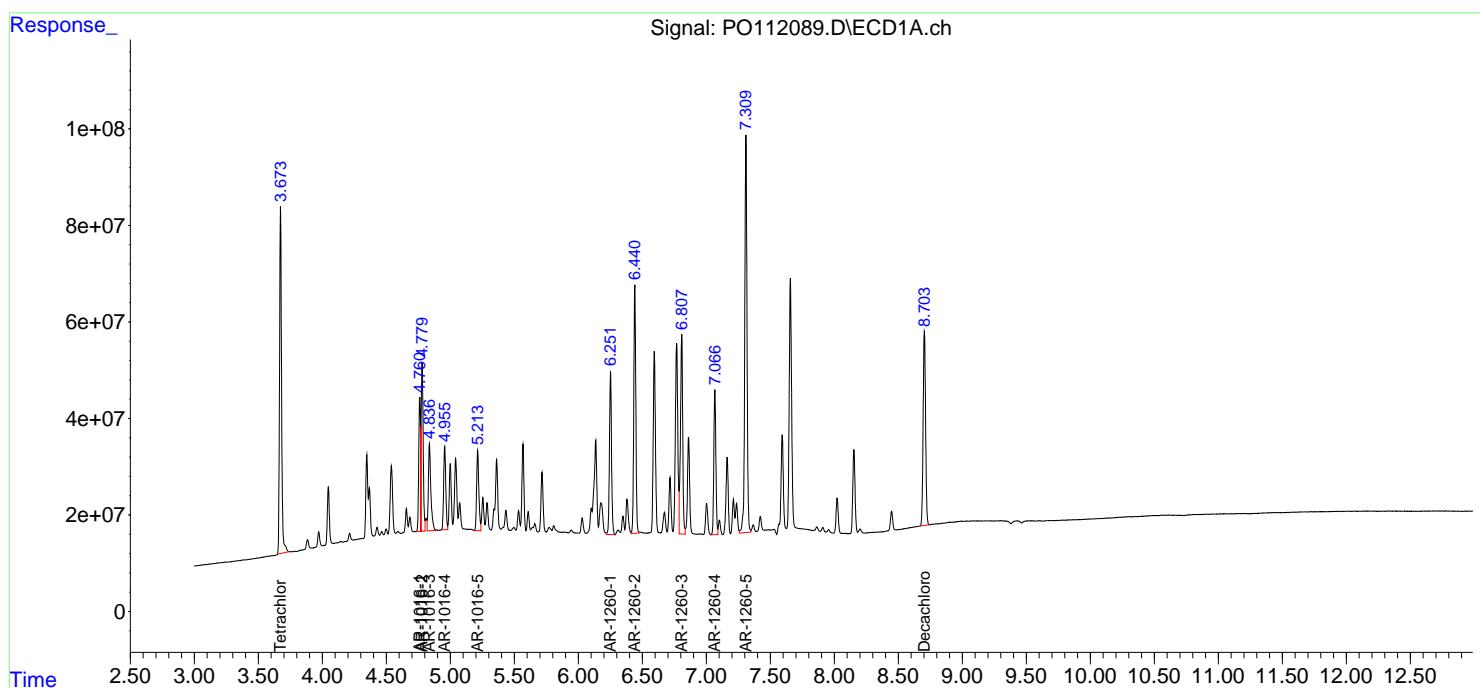

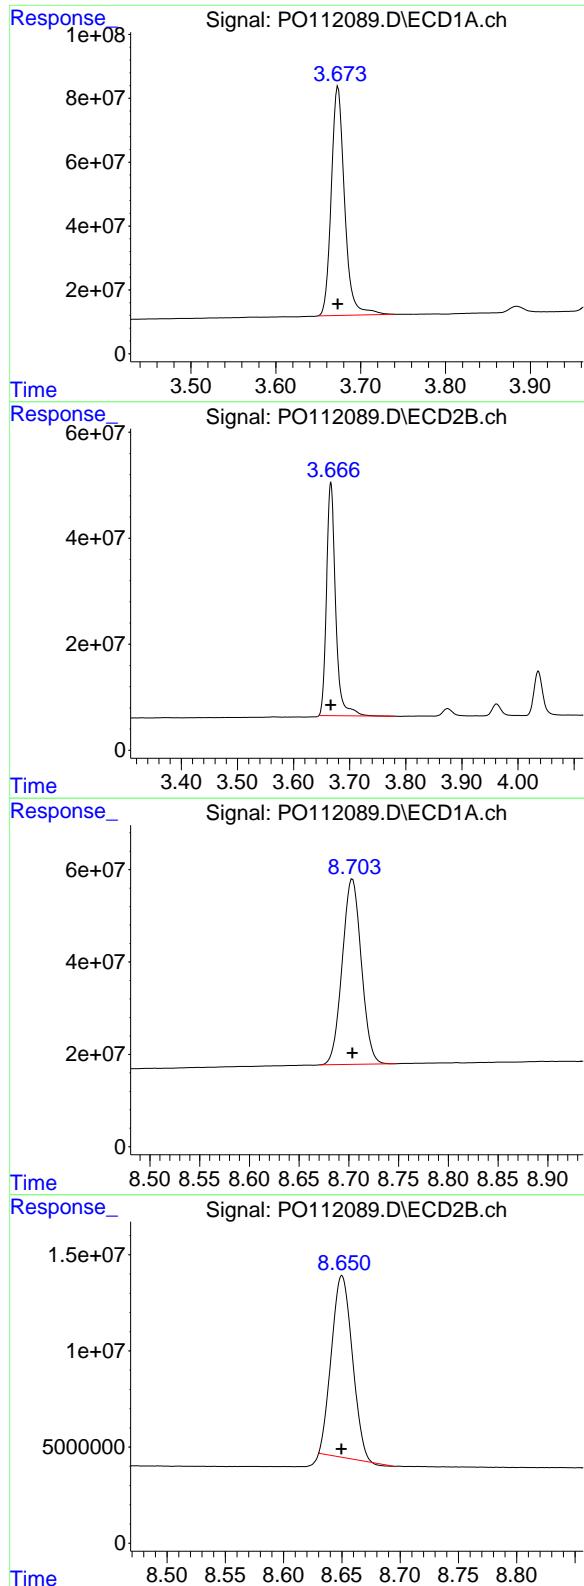

#1 Tetrachloro-m-xylene

R.T.: 3.673 min
Delta R.T.: 0.000 min
Response: 782438196
Conc: 73.81 ng/ml

Instrument: ECD_O
ClientSampleId: AR1660ICC750

#1 Tetrachloro-m-xylene


R.T.: 3.666 min
Delta R.T.: 0.000 min
Response: 495928068
Conc: 73.00 ng/ml

#2 Decachlorobiphenyl

R.T.: 8.704 min
Delta R.T.: 0.000 min
Response: 536034291
Conc: 75.07 ng/ml

#2 Decachlorobiphenyl

R.T.: 8.650 min
Delta R.T.: 0.000 min
Response: 117060156
Conc: 66.91 ng/ml

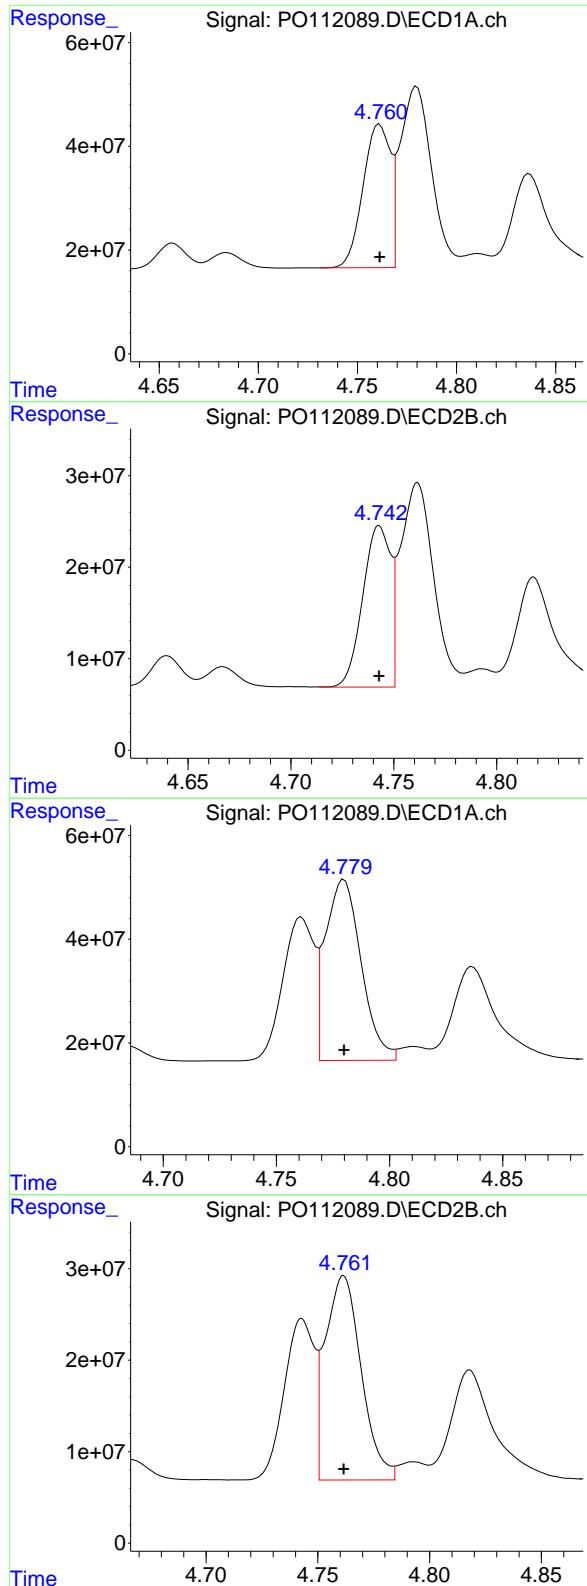

#3 AR-1016-1

R.T.: 4.761 min
 Delta R.T.: 0.000 min
 Response: 265058313
 Conc: 741.24 ng/ml

Instrument: ECD_O
 ClientSampleId: AR1660ICC750

#3 AR-1016-1


R.T.: 4.743 min
 Delta R.T.: 0.000 min
 Response: 165898192
 Conc: 736.51 ng/ml

#4 AR-1016-2

R.T.: 4.780 min
 Delta R.T.: 0.000 min
 Response: 385300934
 Conc: 738.23 ng/ml

#4 AR-1016-2

R.T.: 4.762 min
 Delta R.T.: 0.000 min
 Response: 249723612
 Conc: 743.70 ng/ml

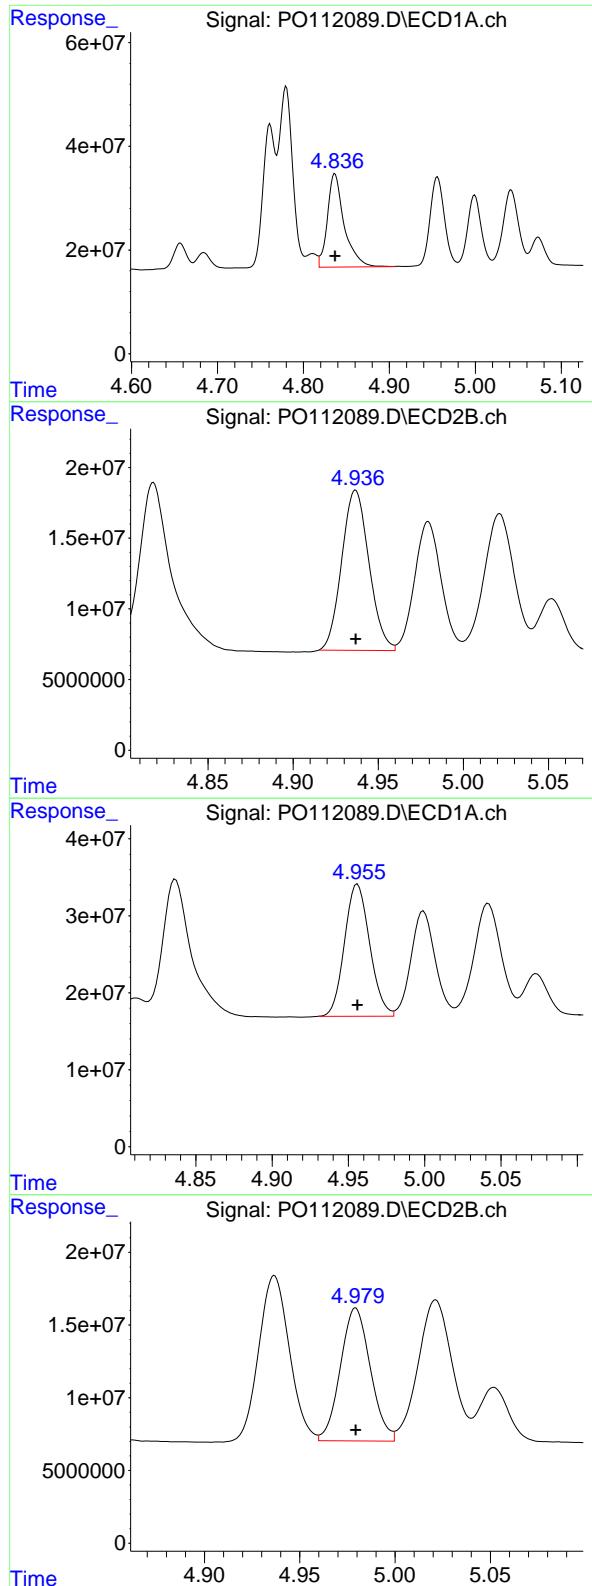

#5 AR-1016-3

R.T.: 4.837 min
 Delta R.T.: 0.000 min
 Response: 243759059
 Conc: 736.56 ng/ml

Instrument: ECD_O
 ClientSampleId: AR1660ICC750

#5 AR-1016-3


R.T.: 4.937 min
 Delta R.T.: 0.000 min
 Response: 126300756
 Conc: 729.88 ng/ml

#6 AR-1016-4

R.T.: 4.956 min
 Delta R.T.: 0.000 min
 Response: 197668080
 Conc: 741.52 ng/ml

#6 AR-1016-4

R.T.: 4.979 min
 Delta R.T.: 0.000 min
 Response: 99974022
 Conc: 735.93 ng/ml

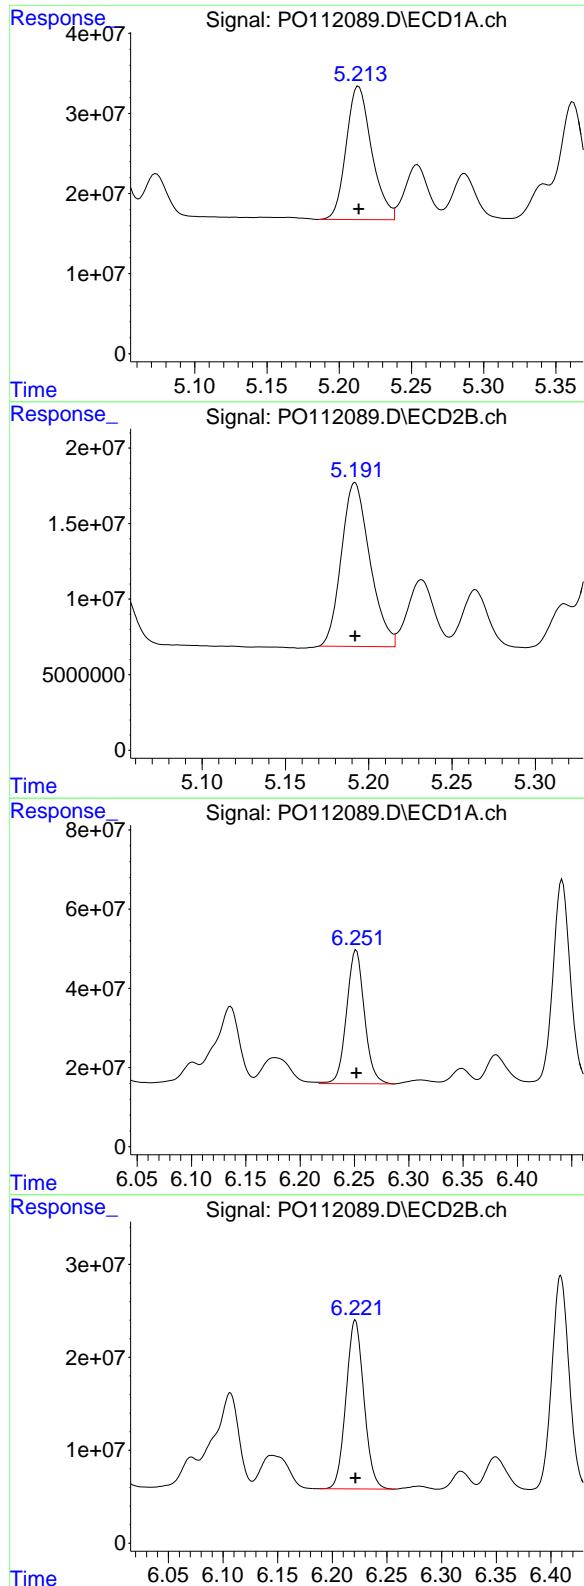

#7 AR-1016-5

R.T.: 5.213 min
 Delta R.T.: 0.000 min
 Response: 204105527
 Conc: 734.33 ng/ml

Instrument: ECD_O
 ClientSampleId: AR1660ICC750

#7 AR-1016-5


R.T.: 5.192 min
 Delta R.T.: 0.000 min
 Response: 129052813
 Conc: 732.69 ng/ml

#31 AR-1260-1

R.T.: 6.252 min
 Delta R.T.: 0.000 min
 Response: 385533844
 Conc: 744.35 ng/ml

#31 AR-1260-1

R.T.: 6.221 min
 Delta R.T.: 0.000 min
 Response: 206690683
 Conc: 743.54 ng/ml

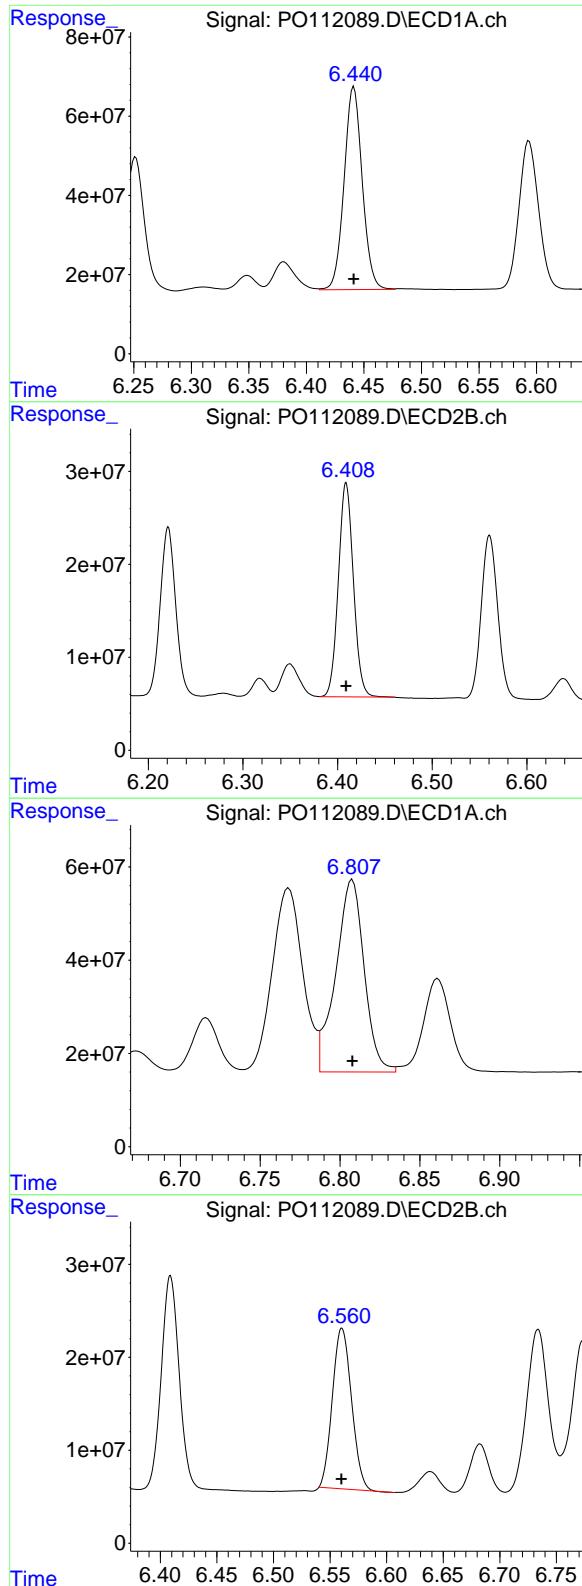

#32 AR-1260-2

R.T.: 6.441 min
 Delta R.T.: 0.000 min
 Response: 563851179
 Conc: 745.06 ng/ml

Instrument: ECD_O
 ClientSampleId: AR1660ICC750

#32 AR-1260-2


R.T.: 6.409 min
 Delta R.T.: 0.000 min
 Response: 254912389
 Conc: 746.48 ng/ml

#33 AR-1260-3

R.T.: 6.808 min
 Delta R.T.: 0.000 min
 Response: 509828933
 Conc: 746.21 ng/ml

#33 AR-1260-3

R.T.: 6.561 min
 Delta R.T.: 0.000 min
 Response: 203595451
 Conc: 709.49 ng/ml

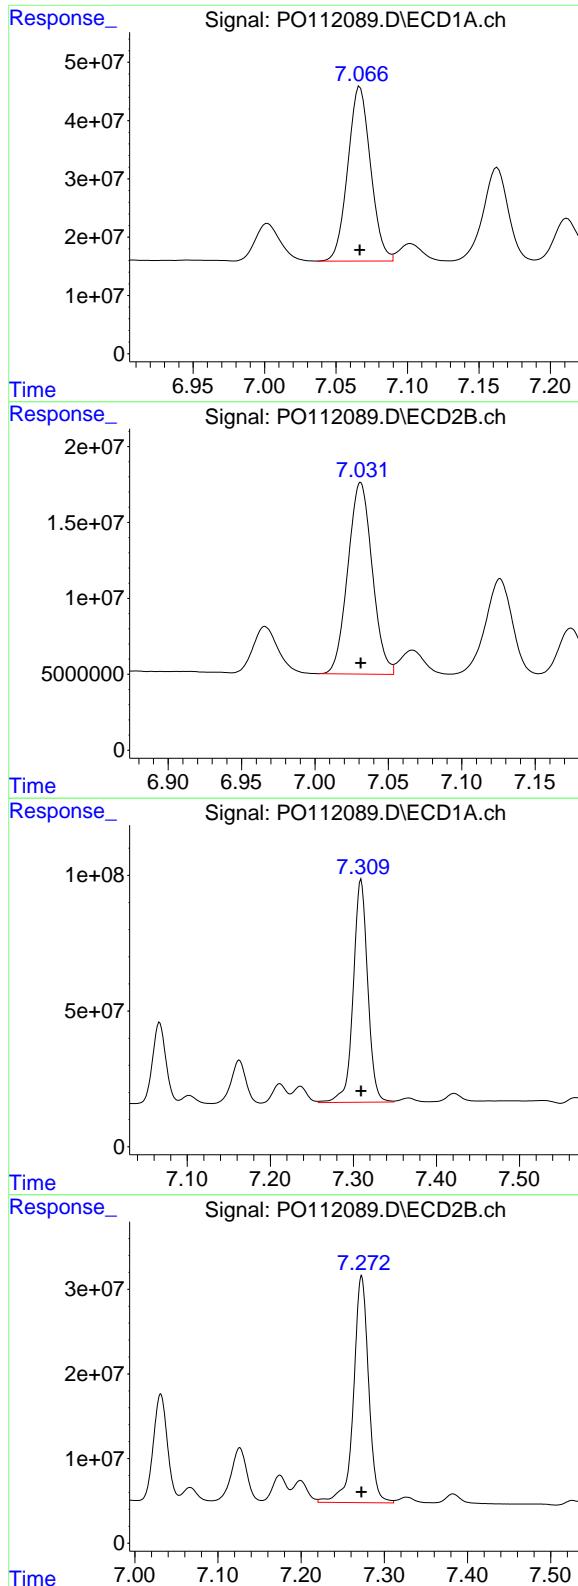

#34 AR-1260-4

R.T.: 7.067 min
 Delta R.T.: 0.000 min
 Response: 332111911
 Conc: 749.81 ng/ml

Instrument: ECD_O
 ClientSampleId: AR1660ICC750

#34 AR-1260-4

R.T.: 7.031 min
 Delta R.T.: 0.000 min
 Response: 145778050
 Conc: 743.95 ng/ml

#35 AR-1260-5

R.T.: 7.309 min
 Delta R.T.: 0.000 min
 Response: 1000222126
 Conc: 749.02 ng/ml

#35 AR-1260-5

R.T.: 7.273 min
 Delta R.T.: 0.000 min
 Response: 336387510
 Conc: 750.94 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0070825\
 Data File : P0112091.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jul 2025 15:02
 Operator : YP/AJ
 Sample : AR1660ICC250
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1660ICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 08 15:21:22 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 08 15:05:13 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	3.674	3.667	254.6E6	165.8E6	24.239	24.516
2) SA Decachlor...	8.704	8.650	182.1E6	41869017	25.379	23.534

Target Compounds

3) L1 AR-1016-1	4.762	4.743	87952907	58858758	246.959	258.385
4) L1 AR-1016-2	4.780	4.762	131.2E6	86217779	251.058	255.039
5) L1 AR-1016-3	4.838	4.937	85456999	43830930	256.116	251.057
6) L1 AR-1016-4	4.957	4.979	66370456	35386243	249.234	257.115
7) L1 AR-1016-5	5.214	5.192	71497345	44870816	255.385	251.028
31) L7 AR-1260-1	6.252	6.221	161.0E6	79739924	310.782	276.656
32) L7 AR-1260-2	6.442	6.409	220.9E6	91585006	293.482	263.404
33) L7 AR-1260-3	6.807	6.561	178.6E6	71570152	263.201	247.541
34) L7 AR-1260-4	7.067	7.031	134.0E6	54771859	297.846	271.502
35) L7 AR-1260-5	7.310	7.272	335.4E6	120.8E6	250.863	264.490



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0070825\
 Data File : P0112091.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jul 2025 15:02
 Operator : YP/AJ
 Sample : AR1660ICC250
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1660ICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 08 15:21:22 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 08 15:05:13 2025
 Response via : Initial Calibration
 Integrator: ChemStation


Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

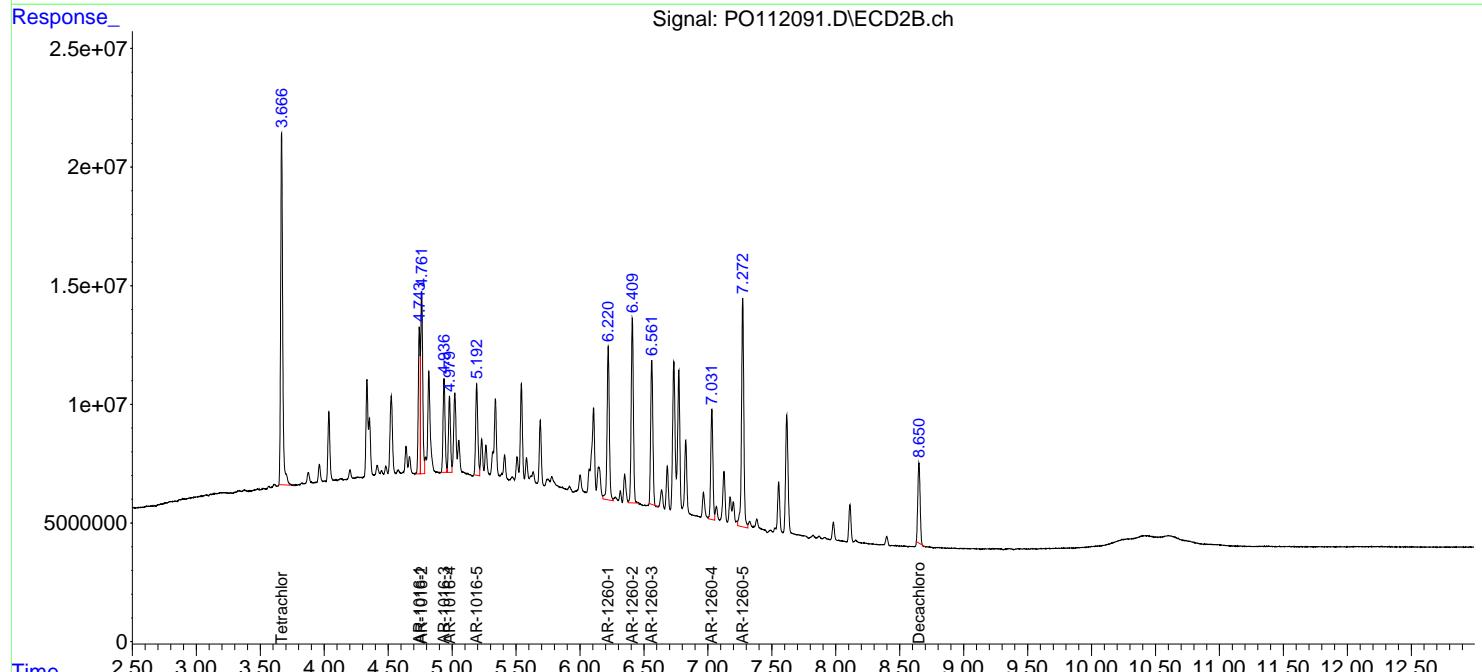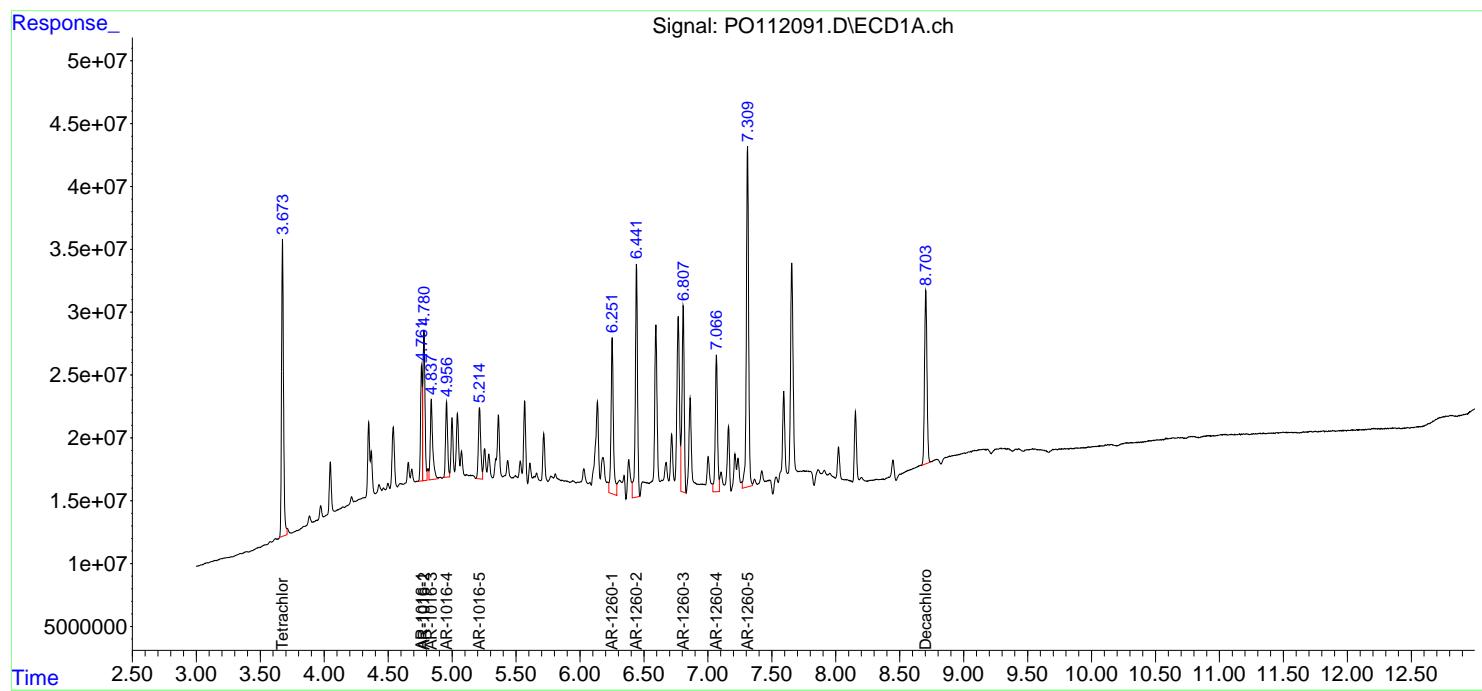

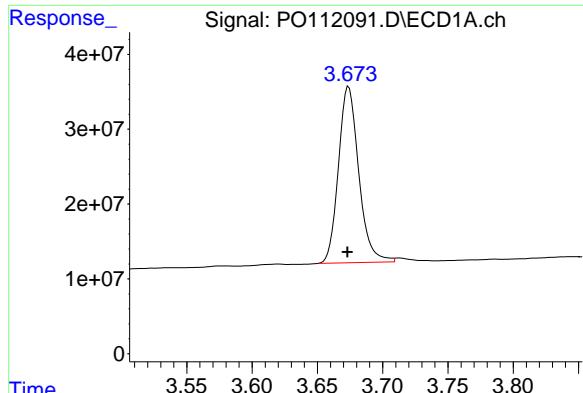


#1 Tetrachloro-m-xylene
R.T.: 3.674 min
Delta R.T.: 0.000 min
Response: 254587950
Conc: 24.24 ng/ml


Instrument: ECD_O
ClientSampleId: AR1660ICC250

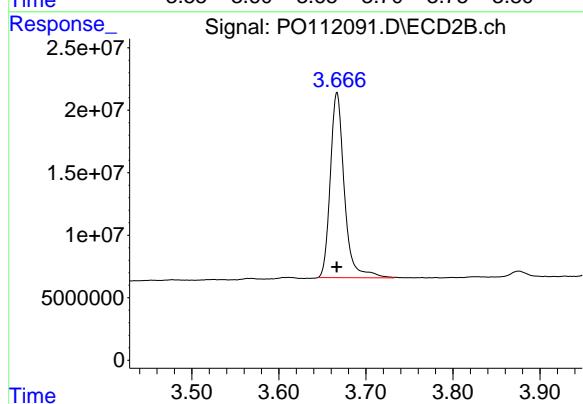


#1 Tetrachloro-m-xylene
R.T.: 3.667 min
Delta R.T.: 0.000 min
Response: 165806941
Conc: 24.52 ng/ml

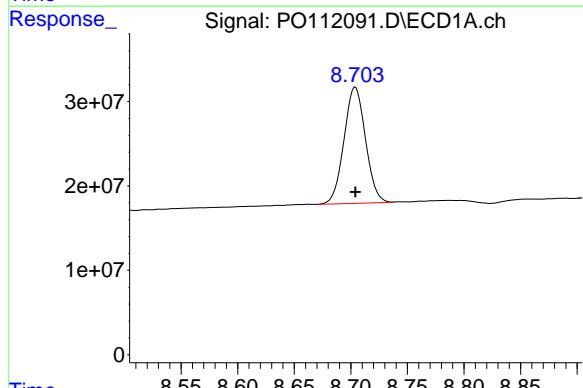

#2 Decachlorobiphenyl
R.T.: 8.704 min
Delta R.T.: 0.000 min
Response: 182135512
Conc: 25.38 ng/ml

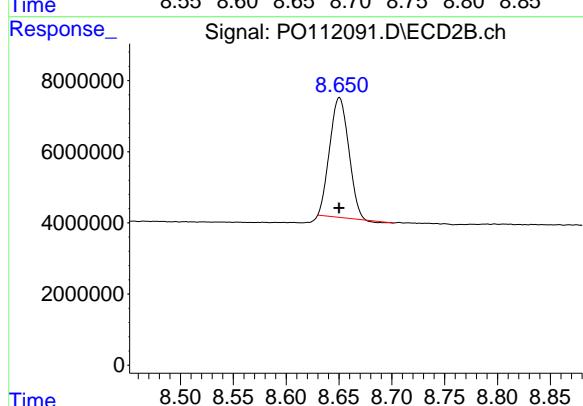

#2 Decachlorobiphenyl
R.T.: 8.650 min
Delta R.T.: 0.000 min
Response: 41869017
Conc: 23.53 ng/ml

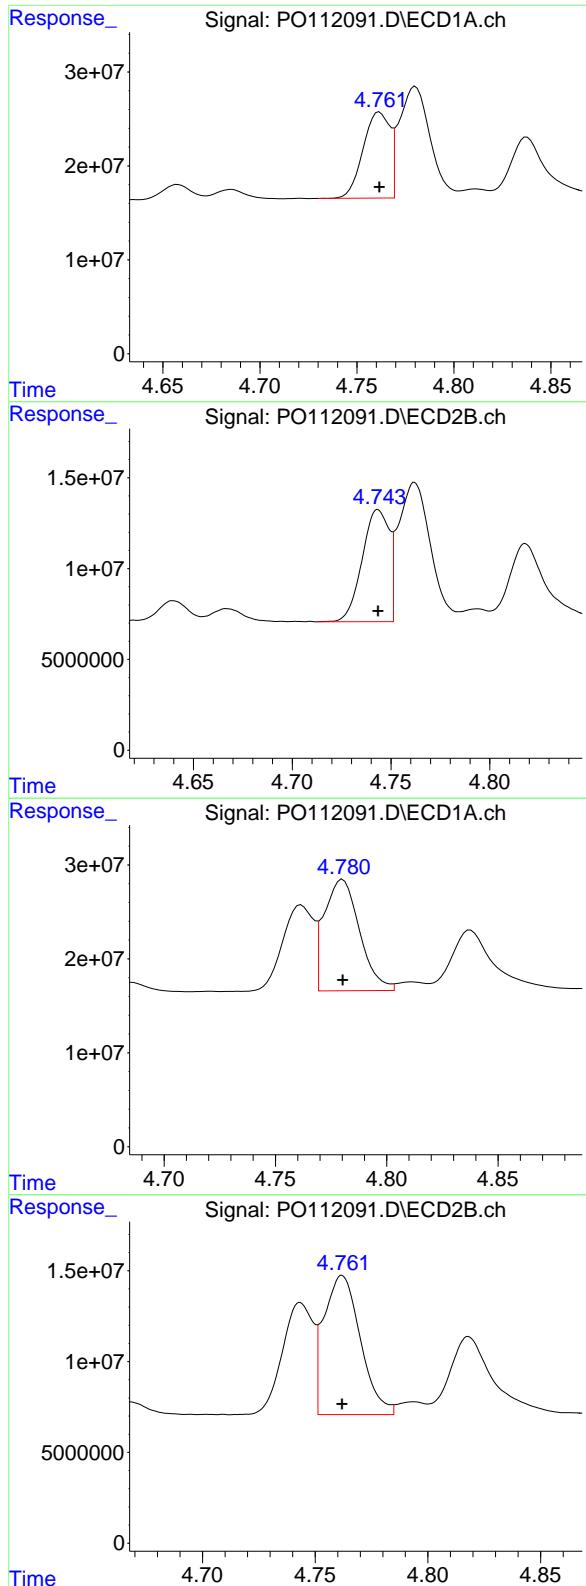

#3 AR-1016-1

R.T.: 4.762 min
 Delta R.T.: 0.000 min
 Response: 87952907
 Conc: 246.96 ng/ml

Instrument: ECD_O
 ClientSampleId: AR1660ICC250

#3 AR-1016-1


R.T.: 4.743 min
 Delta R.T.: 0.000 min
 Response: 58858758
 Conc: 258.39 ng/ml

#4 AR-1016-2

R.T.: 4.780 min
 Delta R.T.: 0.000 min
 Response: 131218582
 Conc: 251.06 ng/ml

#4 AR-1016-2

R.T.: 4.762 min
 Delta R.T.: 0.000 min
 Response: 86217779
 Conc: 255.04 ng/ml

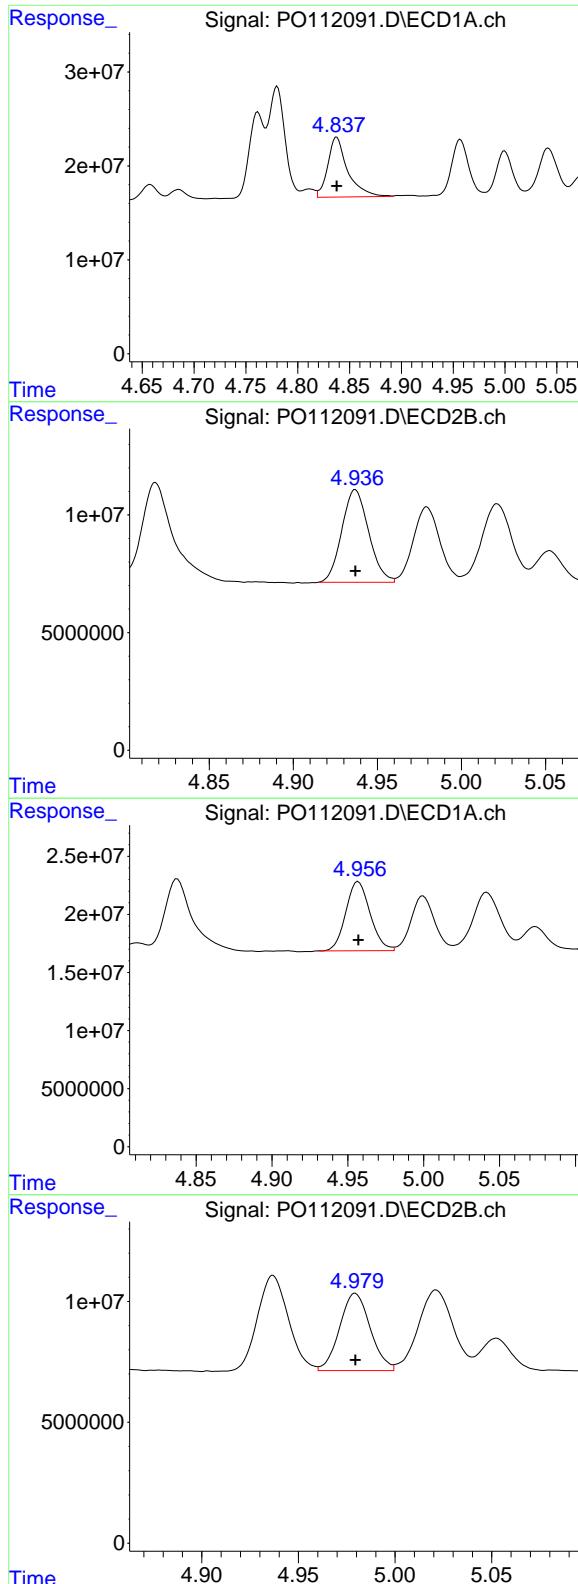

#5 AR-1016-3

R.T.: 4.838 min
Delta R.T.: 0.000 min
Response: 85456999
Conc: 256.12 ng/ml

Instrument: ECD_O
ClientSampleId: AR1660ICC250

#5 AR-1016-3


R.T.: 4.937 min
Delta R.T.: 0.000 min
Response: 43830930
Conc: 251.06 ng/ml

#6 AR-1016-4

R.T.: 4.957 min
Delta R.T.: 0.000 min
Response: 66370456
Conc: 249.23 ng/ml

#6 AR-1016-4

R.T.: 4.979 min
Delta R.T.: 0.000 min
Response: 35386243
Conc: 257.11 ng/ml

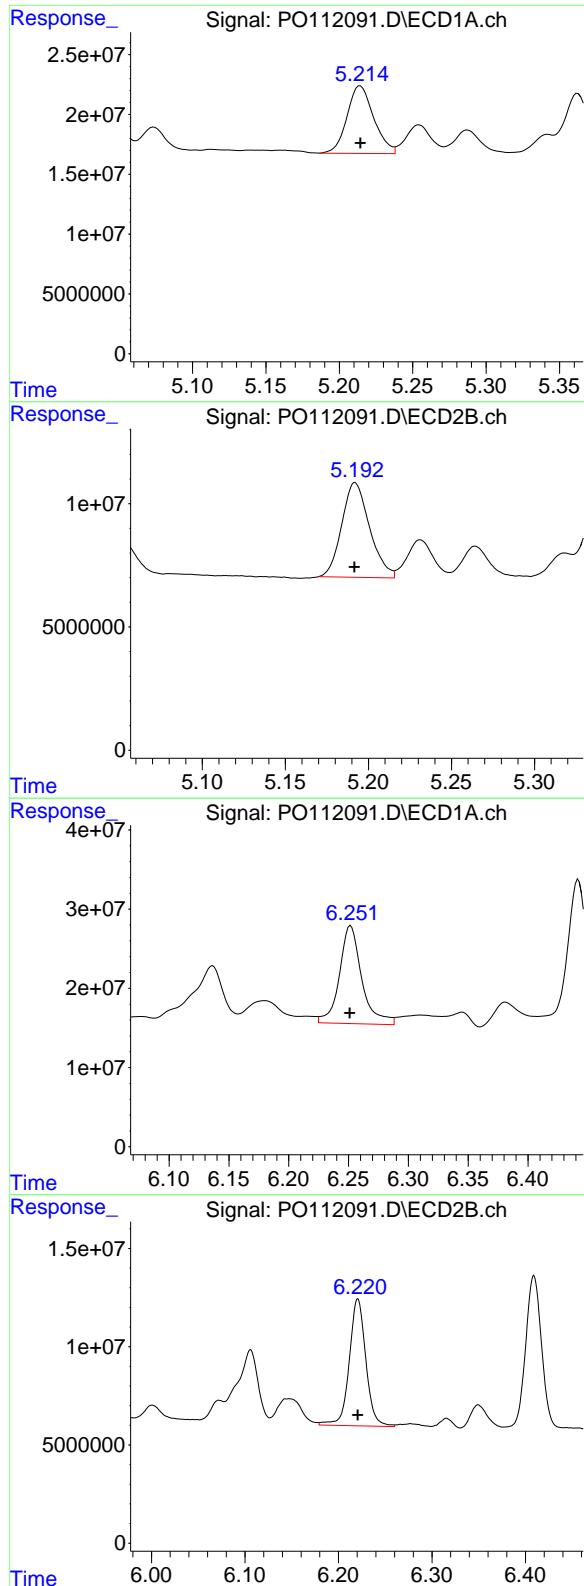

#7 AR-1016-5

R.T.: 5.214 min
 Delta R.T.: 0.000 min
 Response: 71497345
 Conc: 255.39 ng/ml

Instrument: ECD_O
 ClientSampleId: AR1660ICC250

#7 AR-1016-5


R.T.: 5.192 min
 Delta R.T.: 0.000 min
 Response: 44870816
 Conc: 251.03 ng/ml

#31 AR-1260-1

R.T.: 6.252 min
 Delta R.T.: 0.000 min
 Response: 160998170
 Conc: 310.78 ng/ml

#31 AR-1260-1

R.T.: 6.221 min
 Delta R.T.: 0.000 min
 Response: 79739924
 Conc: 276.66 ng/ml

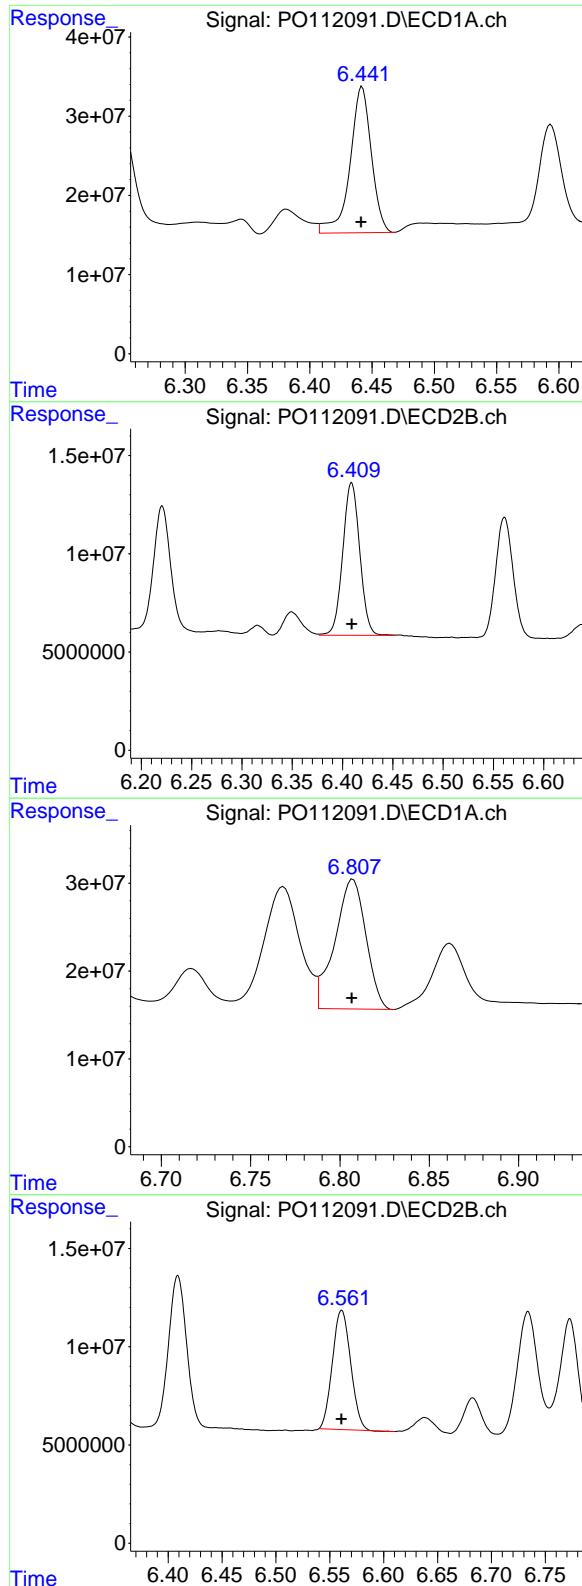

#32 AR-1260-2

R.T.: 6.442 min
 Delta R.T.: 0.000 min
 Response: 220921013
 Conc: 293.48 ng/ml

Instrument: ECD_O
 ClientSampleId: AR1660ICC250

#32 AR-1260-2


R.T.: 6.409 min
 Delta R.T.: 0.000 min
 Response: 91585006
 Conc: 263.40 ng/ml

#33 AR-1260-3

R.T.: 6.807 min
 Delta R.T.: 0.000 min
 Response: 178596185
 Conc: 263.20 ng/ml

#33 AR-1260-3

R.T.: 6.561 min
 Delta R.T.: 0.000 min
 Response: 71570152
 Conc: 247.54 ng/ml

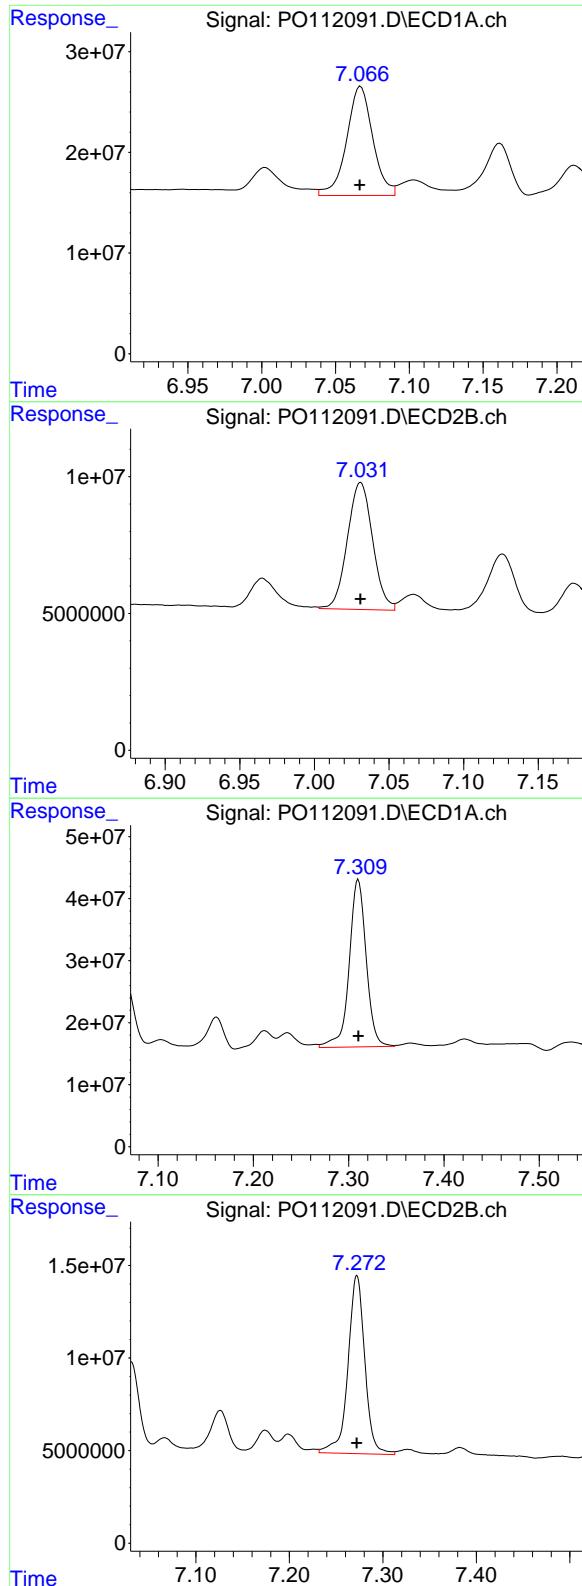

#34 AR-1260-4

R.T.: 7.067 min
 Delta R.T.: 0.000 min
 Response: 133993035
 Conc: 297.85 ng/ml

Instrument: ECD_O
 ClientSampleId: AR1660ICC250

#34 AR-1260-4

R.T.: 7.031 min
 Delta R.T.: 0.000 min
 Response: 54771859
 Conc: 271.50 ng/ml

#35 AR-1260-5

R.T.: 7.310 min
 Delta R.T.: 0.000 min
 Response: 335383544
 Conc: 250.86 ng/ml

#35 AR-1260-5

R.T.: 7.272 min
 Delta R.T.: 0.000 min
 Response: 120812819
 Conc: 264.49 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0070825\
 Data File : P0112092.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jul 2025 15:21
 Operator : YP/AJ
 Sample : AR1660ICC050
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1660ICC050

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 08 15:36:17 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 08 15:36:04 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	3.673	3.666	37442397	24163066	3.784	3.793
2) SA Decachlor...	8.703	8.650	27391770	6408552	4.006	3.715

Target Compounds

3) L1 AR-1016-1	4.761	4.743	13802015	10149679	40.580	45.548
4) L1 AR-1016-2	4.780	4.761	19790298	14662938	39.796	44.555
5) L1 AR-1016-3	4.836	4.936	14195524	7549659	43.852	44.445
6) L1 AR-1016-4	4.956	4.979	10940244	6781238	42.602	49.416
7) L1 AR-1016-5	5.212	5.191	14240179	7528374	51.694	43.655
31) L7 AR-1260-1	6.251	6.220	59957659	21359833	120.174	76.207 #
32) L7 AR-1260-2	6.441	6.408	51044679	20093020	69.700	58.992
33) L7 AR-1260-3	6.806	6.559	29007819	11088040	44.254	40.234
34) L7 AR-1260-4	7.066	7.030	19317003	9814007	44.382	48.912
35) L7 AR-1260-5	7.309	7.272	50382935	20576692	39.906	45.958



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0070825\
 Data File : P0112092.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jul 2025 15:21
 Operator : YP/AJ
 Sample : AR1660ICC050
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1660ICC050

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 08 15:36:17 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 08 15:36:04 2025
 Response via : Initial Calibration
 Integrator: ChemStation


Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

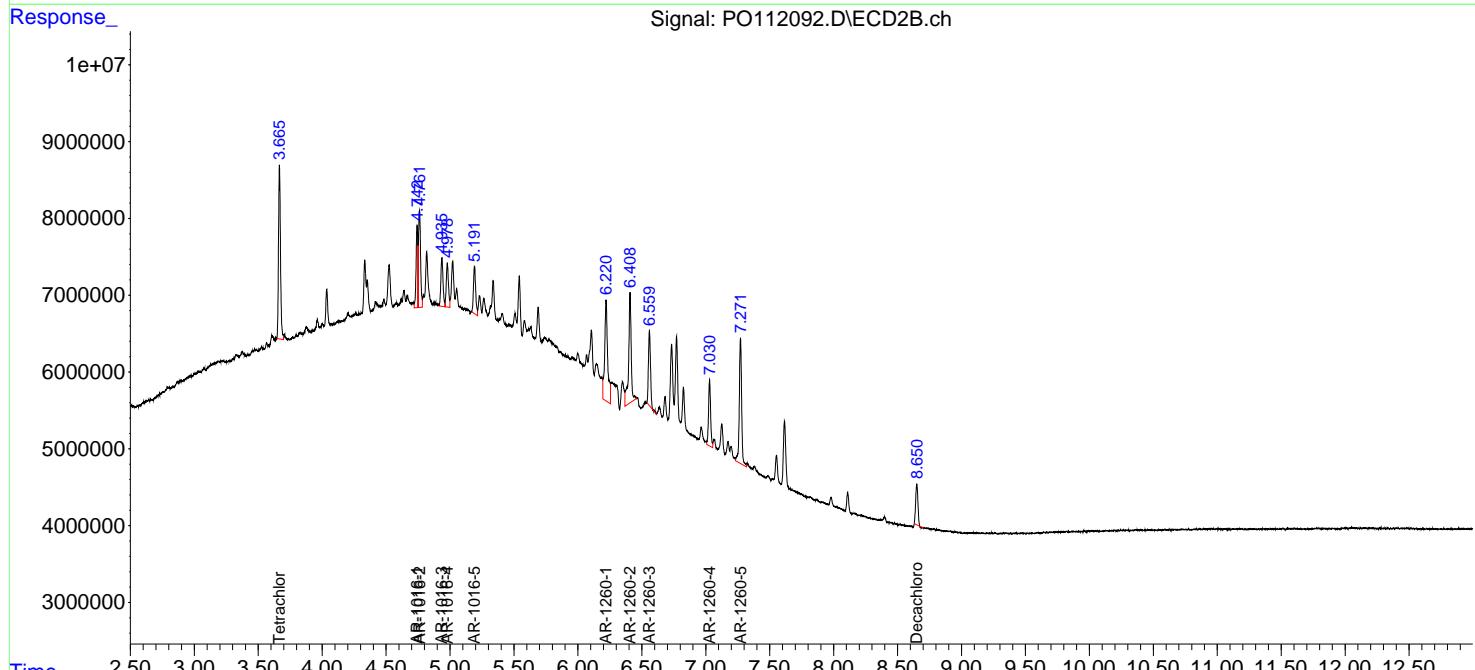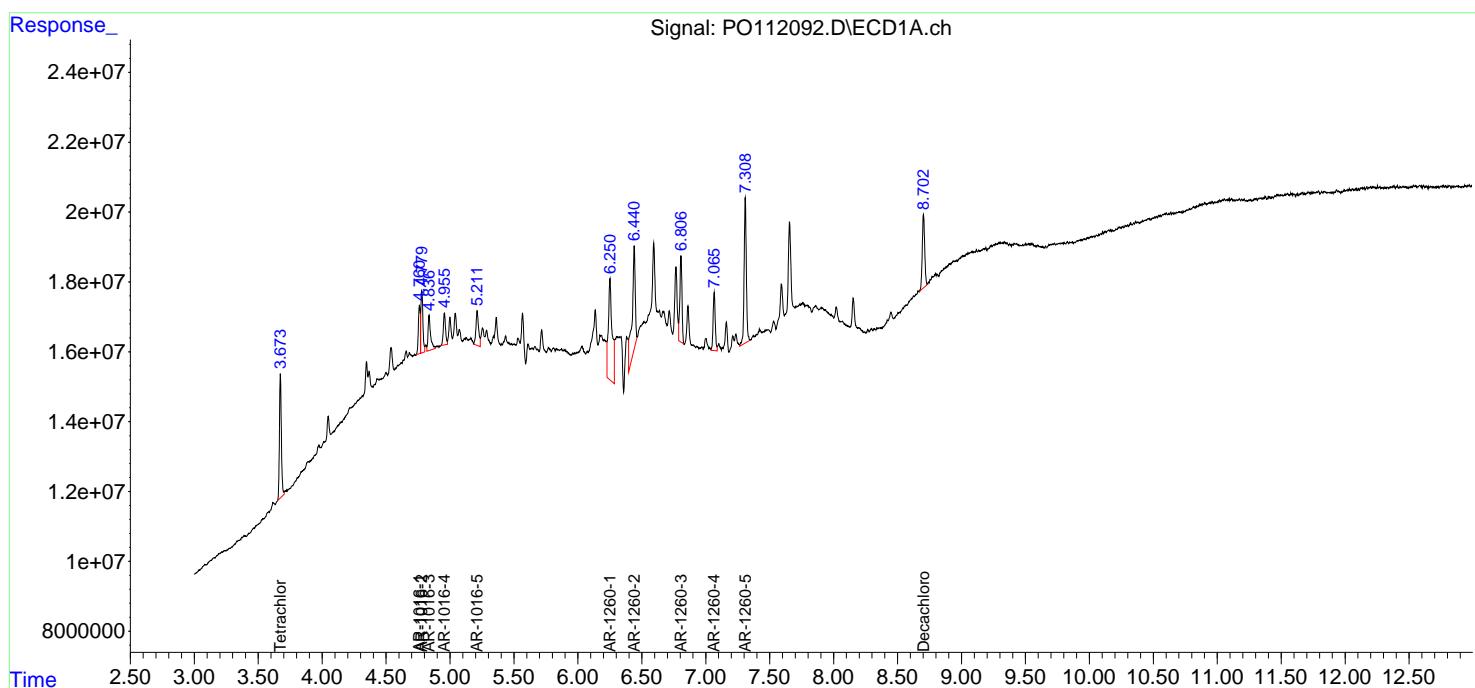

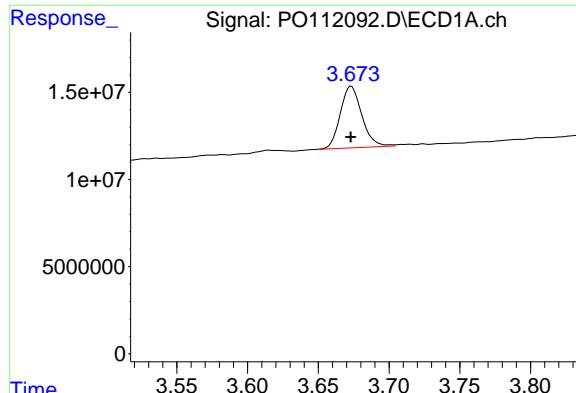


#1 Tetrachloro-m-xylene
R.T.: 3.673 min
Delta R.T.: 0.000 min
Response: 37442397
Conc: 3.78 ng/ml


Instrument: ECD_O
ClientSampleId: AR1660ICC050

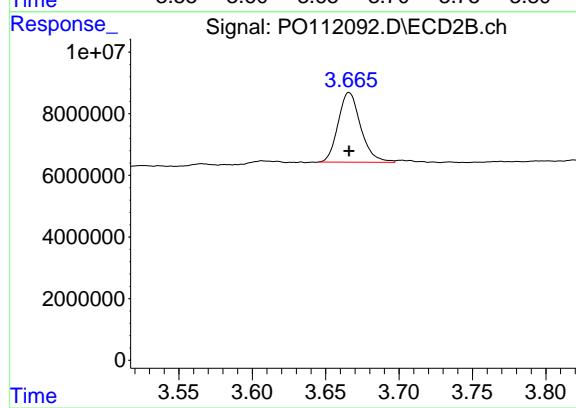


#1 Tetrachloro-m-xylene
R.T.: 3.666 min
Delta R.T.: 0.000 min
Response: 24163066
Conc: 3.79 ng/ml

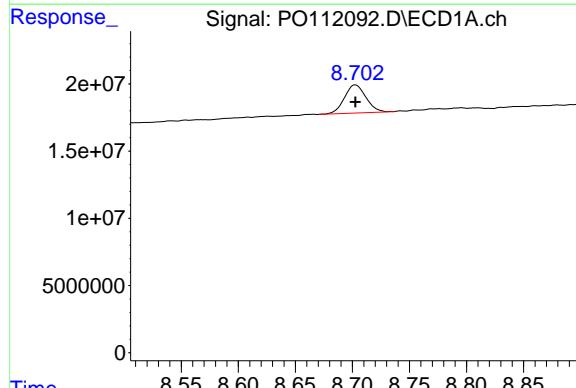

#2 Decachlorobiphenyl
R.T.: 8.703 min
Delta R.T.: 0.000 min
Response: 27391770
Conc: 4.01 ng/ml

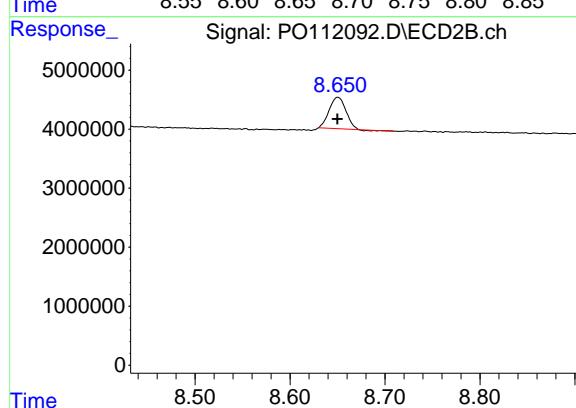

#2 Decachlorobiphenyl
R.T.: 8.650 min
Delta R.T.: 0.000 min
Response: 6408552
Conc: 3.72 ng/ml

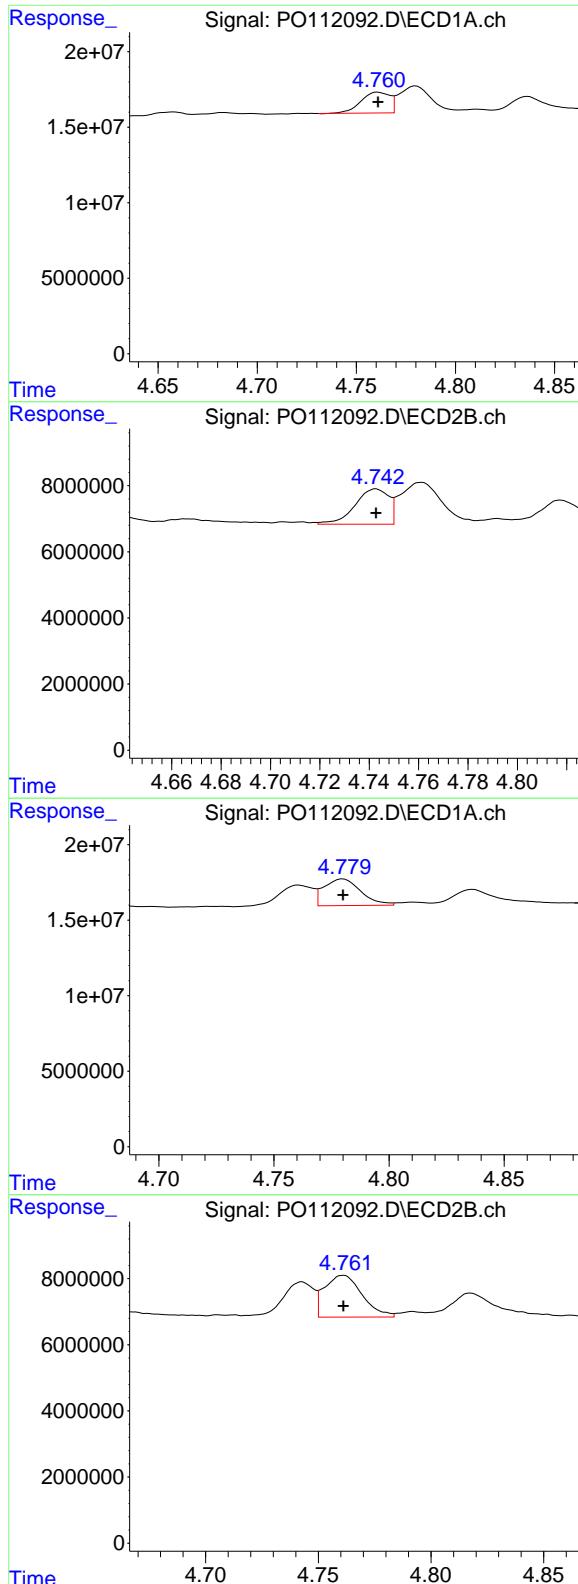

#3 AR-1016-1

R.T.: 4.761 min
 Delta R.T.: 0.000 min
 Response: 13802015
 Conc: 40.58 ng/ml

Instrument: ECD_O
 ClientSampleId: AR1660ICC050

#3 AR-1016-1


R.T.: 4.743 min
 Delta R.T.: 0.000 min
 Response: 10149679
 Conc: 45.55 ng/ml

#4 AR-1016-2

R.T.: 4.780 min
 Delta R.T.: 0.000 min
 Response: 19790298
 Conc: 39.80 ng/ml

#4 AR-1016-2

R.T.: 4.761 min
 Delta R.T.: 0.000 min
 Response: 14662938
 Conc: 44.55 ng/ml

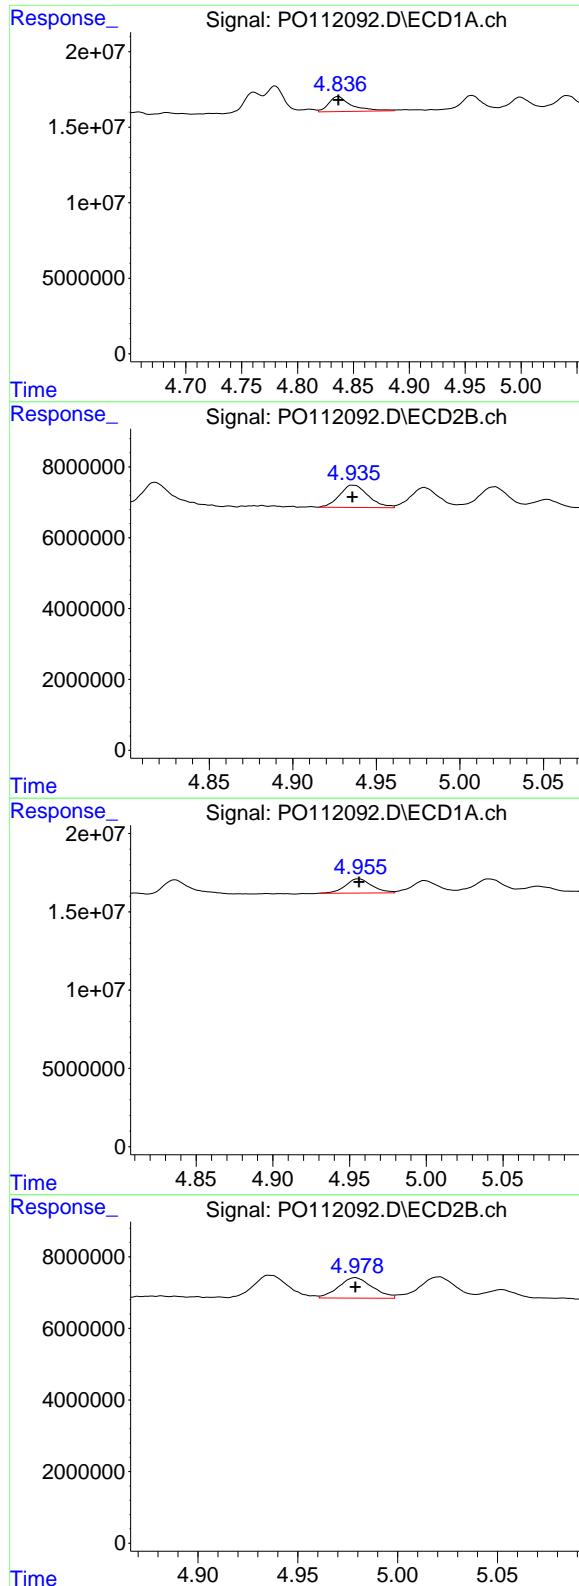

#5 AR-1016-3

R.T.: 4.836 min
 Delta R.T.: 0.000 min **Instrument:**
 Response: 14195524 ECD_O
 Conc: 43.85 ng/ml **ClientSampleId:**
 AR1660ICC050

#5 AR-1016-3


R.T.: 4.936 min
 Delta R.T.: 0.000 min
 Response: 7549659
 Conc: 44.44 ng/ml

#6 AR-1016-4

R.T.: 4.956 min
 Delta R.T.: 0.000 min
 Response: 10940244
 Conc: 42.60 ng/ml

#6 AR-1016-4

R.T.: 4.979 min
 Delta R.T.: 0.000 min
 Response: 6781238
 Conc: 49.42 ng/ml

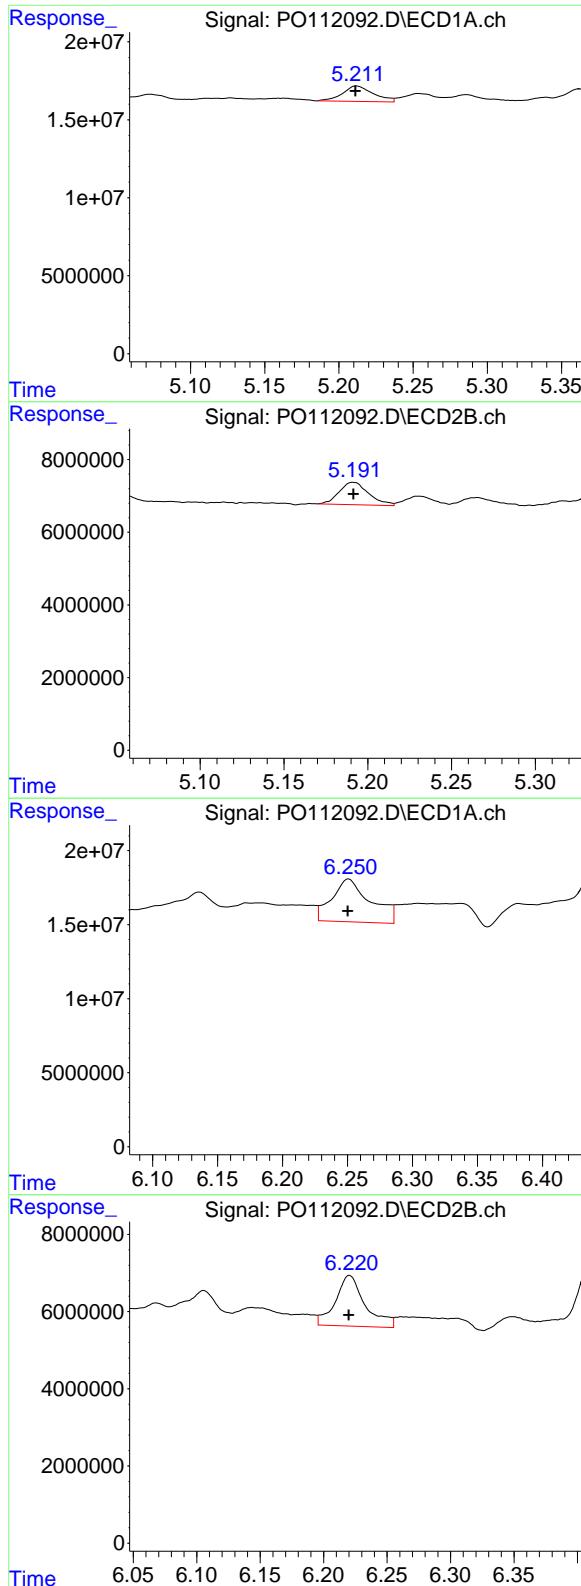

#7 AR-1016-5

R.T.: 5.212 min
 Delta R.T.: 0.000 min **Instrument:**
 Response: 14240179 ECD_O
 Conc: 51.69 ng/ml **ClientSampleId:**
 AR1660ICC050

#7 AR-1016-5


R.T.: 5.191 min
 Delta R.T.: 0.000 min
 Response: 7528374
 Conc: 43.66 ng/ml

#31 AR-1260-1

R.T.: 6.251 min
 Delta R.T.: 0.000 min
 Response: 59957659
 Conc: 120.17 ng/ml

#31 AR-1260-1

R.T.: 6.220 min
 Delta R.T.: 0.000 min
 Response: 21359833
 Conc: 76.21 ng/ml

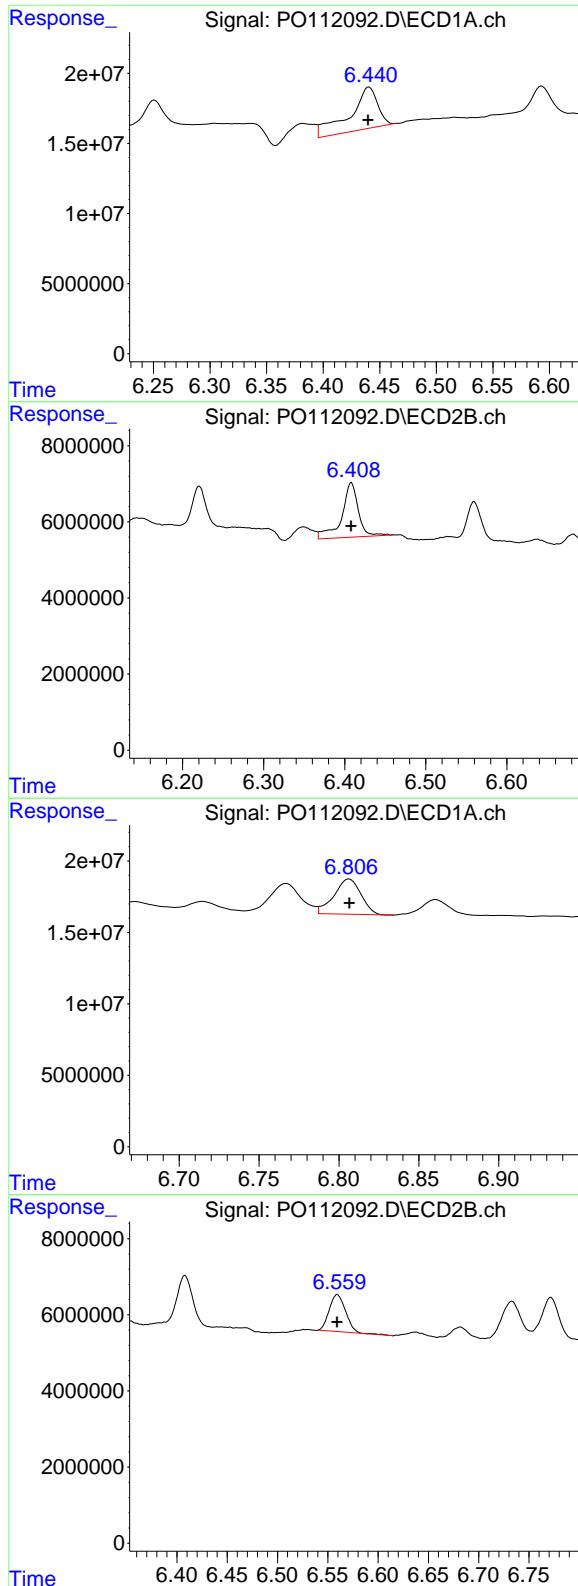

#32 AR-1260-2

R.T.: 6.441 min
 Delta R.T.: 0.000 min
 Response: 51044679
 Conc: 69.70 ng/ml

Instrument: ECD_O
 ClientSampleId: AR1660ICC050

#32 AR-1260-2


R.T.: 6.408 min
 Delta R.T.: 0.000 min
 Response: 20093020
 Conc: 58.99 ng/ml

#33 AR-1260-3

R.T.: 6.806 min
 Delta R.T.: 0.000 min
 Response: 29007819
 Conc: 44.25 ng/ml

#33 AR-1260-3

R.T.: 6.559 min
 Delta R.T.: 0.000 min
 Response: 11088040
 Conc: 40.23 ng/ml

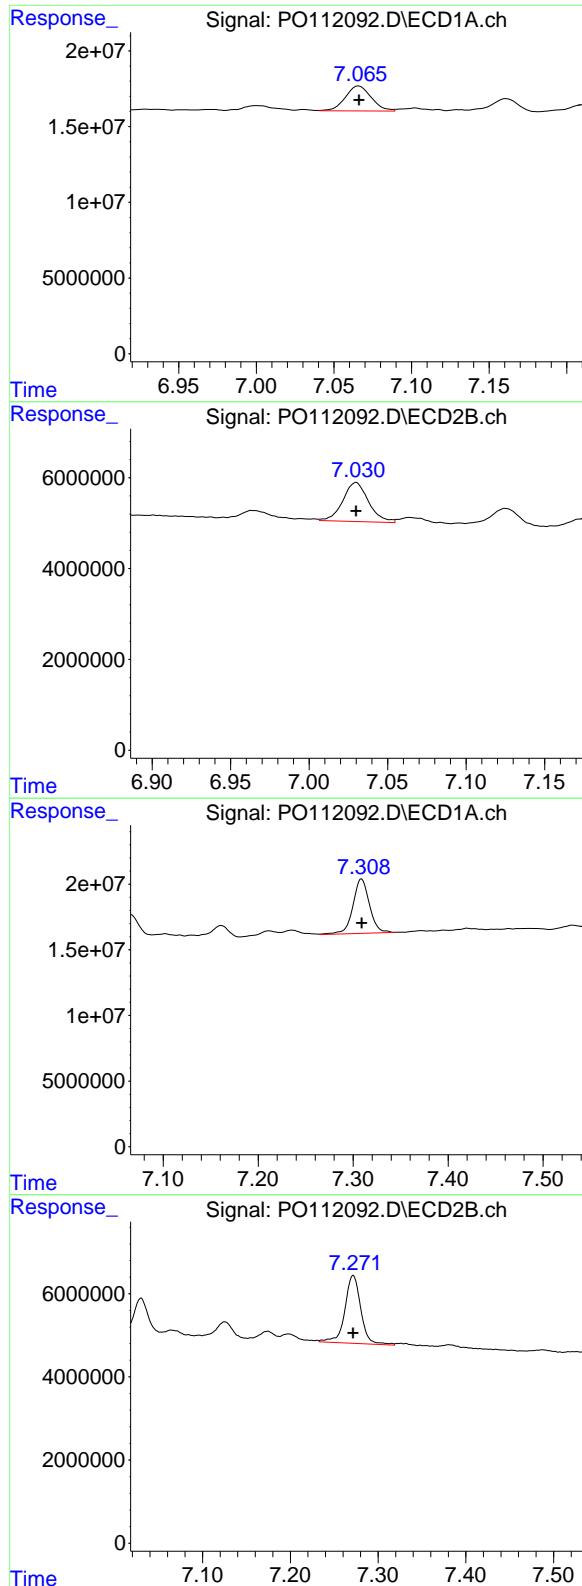

#34 AR-1260-4

R.T.: 7.066 min
 Delta R.T.: 0.000 min **Instrument:**
 Response: 19317003 ECD_O
 Conc: 44.38 ng/ml **ClientSampleId:**
 AR1660ICC050

#34 AR-1260-4

R.T.: 7.030 min
 Delta R.T.: 0.000 min
 Response: 9814007
 Conc: 48.91 ng/ml

#35 AR-1260-5

R.T.: 7.309 min
 Delta R.T.: 0.000 min
 Response: 50382935
 Conc: 39.91 ng/ml

#35 AR-1260-5

R.T.: 7.272 min
 Delta R.T.: 0.000 min
 Response: 20576692
 Conc: 45.96 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0070825\
 Data File : P0112099.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jul 2025 17:29
 Operator : YP/AJ
 Sample : AR1242ICC050
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1242ICC050

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 09 02:31:15 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 09 02:27:13 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	3.673	3.666	42912716	27696407	4.072	4.115
2) SA Decachlor...	8.704	8.650	28291682	7899910	3.950	4.390

Target Compounds

16) L4 AR-1242-1	4.761	4.743	12609363	9619088	41.672	49.038
17) L4 AR-1242-2	4.780	4.761	17776215	13881256	39.541	48.067
18) L4 AR-1242-3	4.837	4.937	12004480	6736786	41.773	44.908
19) L4 AR-1242-4	4.957	5.021	10638220	7029005	45.904	48.940
20) L4 AR-1242-5	5.609	5.541	17753976	13107939	79.074	70.069



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0070825\
 Data File : P0112099.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jul 2025 17:29
 Operator : YP/AJ
 Sample : AR1242ICC050
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1242ICC050

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 09 02:31:15 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 09 02:27:13 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

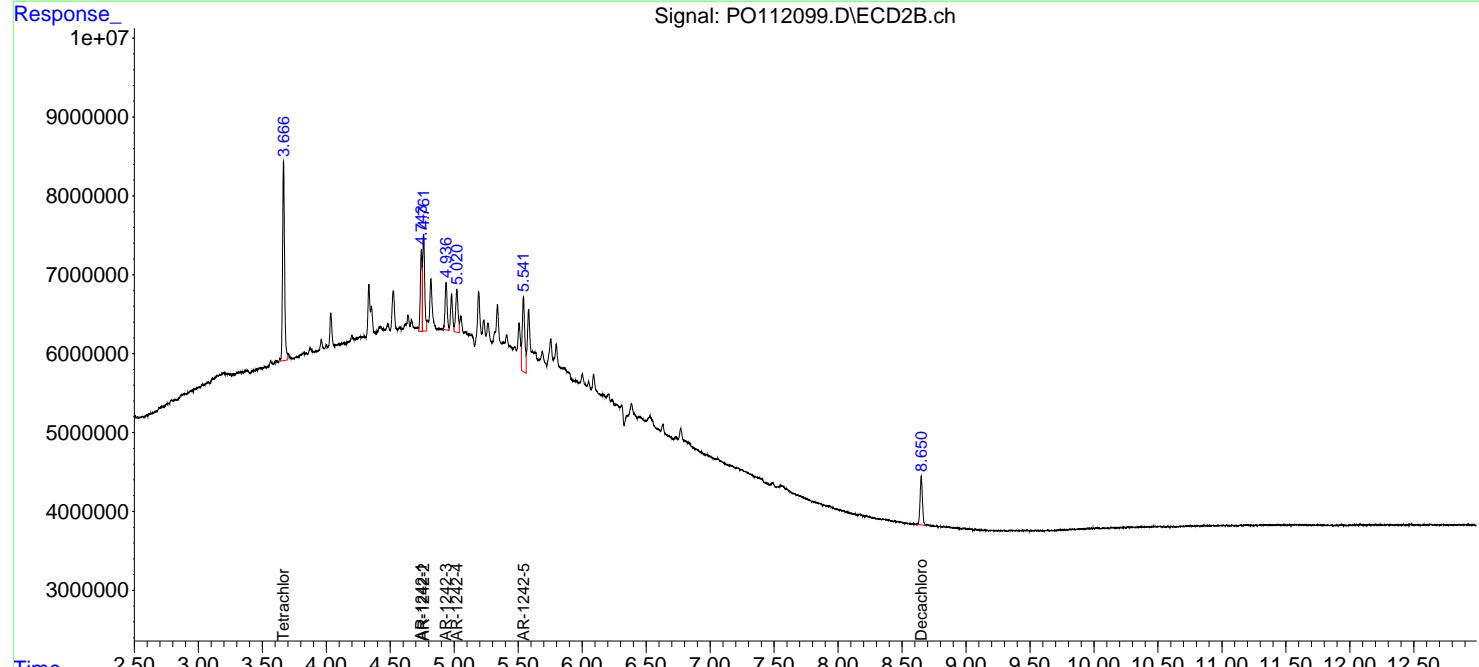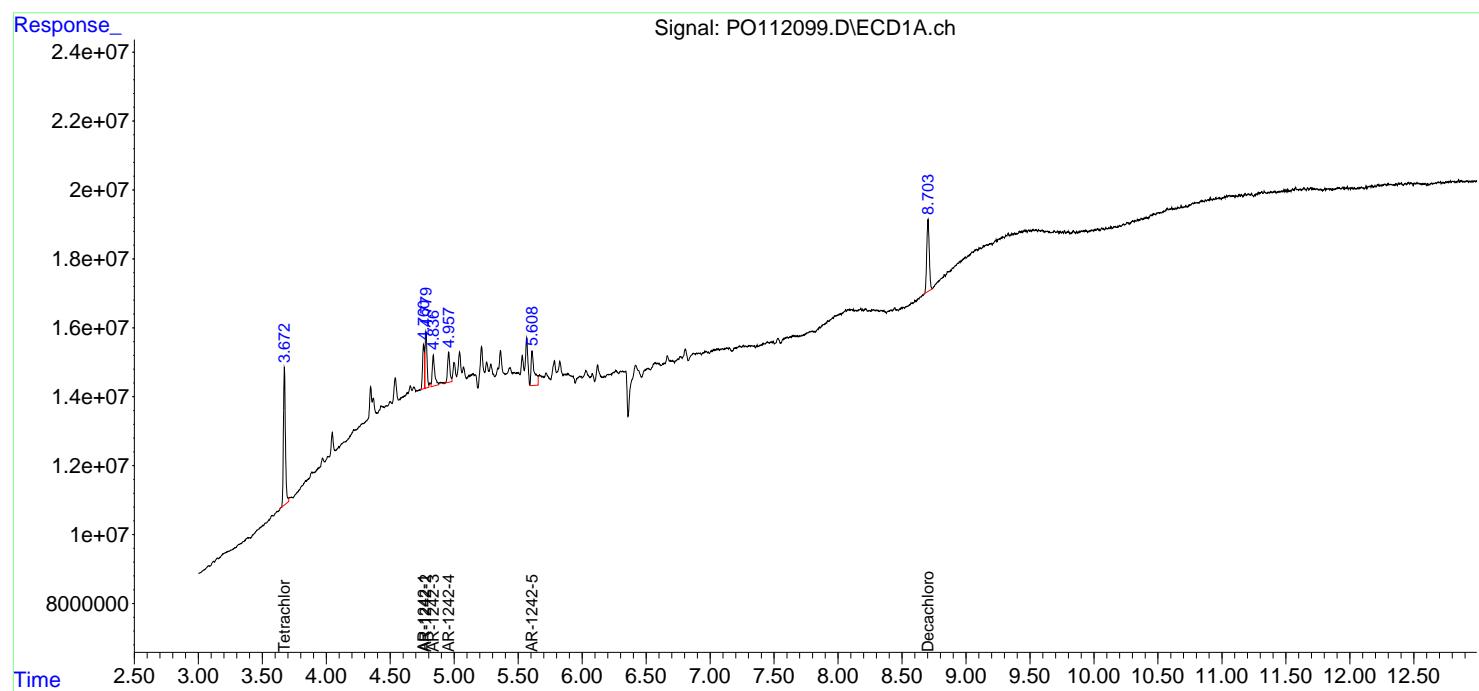




#1 Tetrachloro-m-xylene


R.T.: 3.673 min
Delta R.T.: 0.000 min
Response: 42912716
Conc: 4.07 ng/ml

Instrument: ECD_O
ClientSampleId: AR1242ICC050

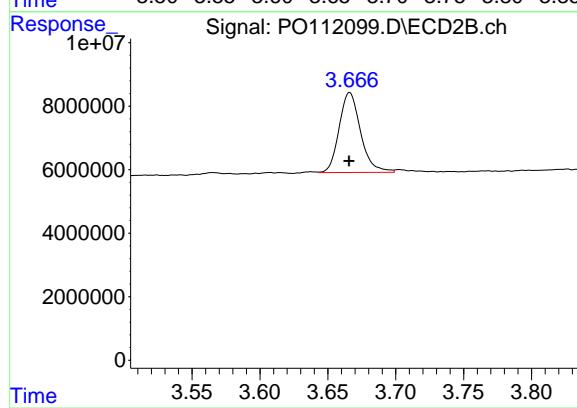


#1 Tetrachloro-m-xylene

R.T.: 3.666 min
Delta R.T.: 0.000 min
Response: 27696407
Conc: 4.11 ng/ml

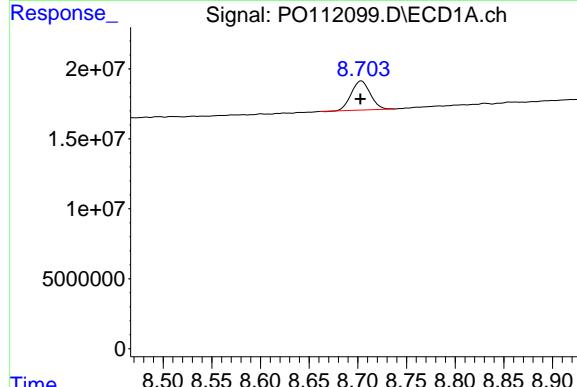


#2 Decachlorobiphenyl

R.T.: 8.704 min
Delta R.T.: 0.000 min
Response: 28291682
Conc: 3.95 ng/ml

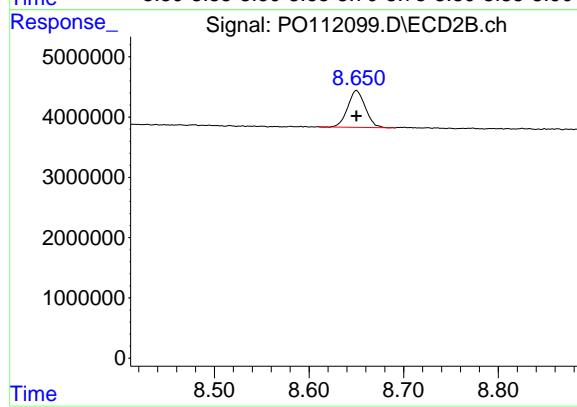

#2 Decachlorobiphenyl

R.T.: 8.650 min
Delta R.T.: 0.000 min
Response: 7899910
Conc: 4.39 ng/ml

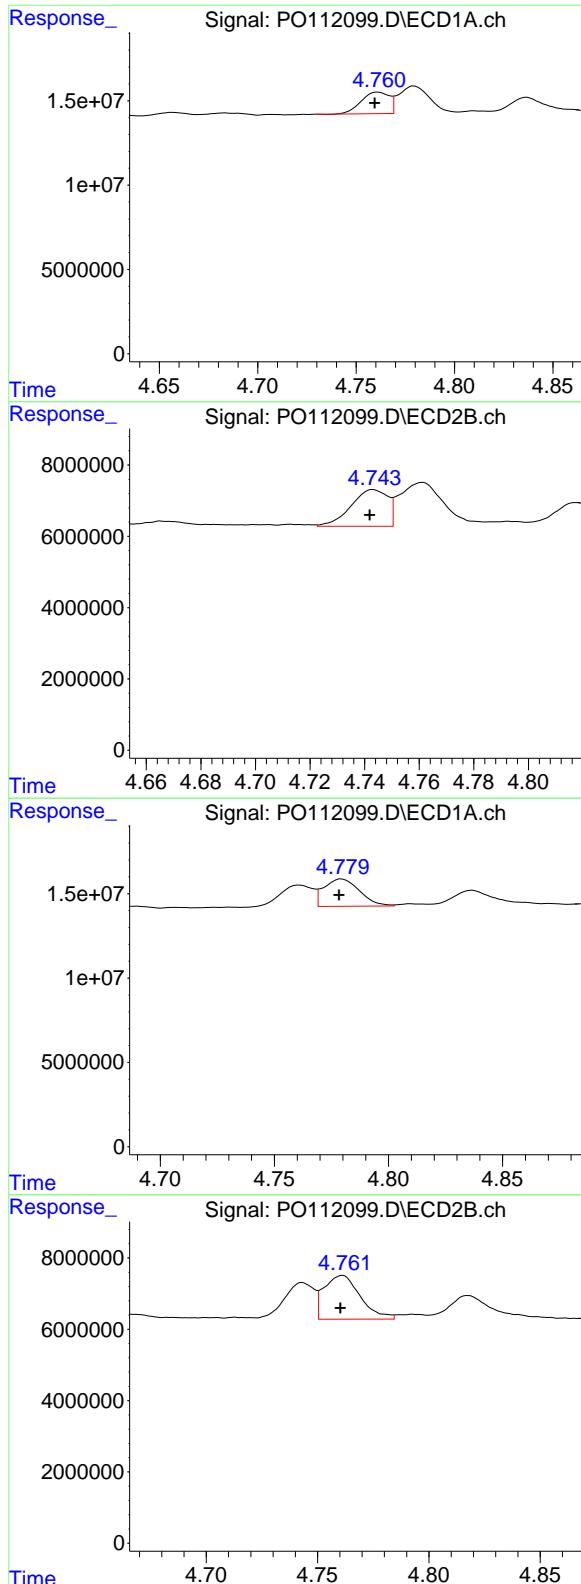

#16 AR-1242-1

R.T.: 4.761 min
 Delta R.T.: 0.002 min
 Response: 12609363
 Conc: 41.67 ng/ml

Instrument: ECD_O
 ClientSampleId: AR1242ICC050

#16 AR-1242-1


R.T.: 4.743 min
 Delta R.T.: 0.001 min
 Response: 9619088
 Conc: 49.04 ng/ml

#17 AR-1242-2

R.T.: 4.780 min
 Delta R.T.: 0.001 min
 Response: 17776215
 Conc: 39.54 ng/ml

#17 AR-1242-2


R.T.: 4.761 min
 Delta R.T.: 0.001 min
 Response: 13881256
 Conc: 48.07 ng/ml

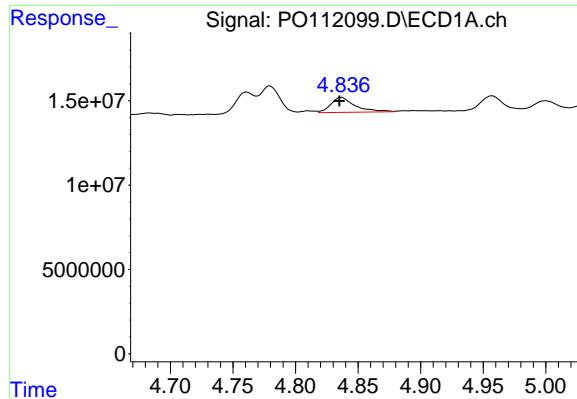

#18 AR-1242-3


R.T.: 4.837 min
Delta R.T.: 0.002 min
Response: 12004480
Conc: 41.77 ng/ml

Instrument: ECD_O
ClientSampleId: AR1242ICC050

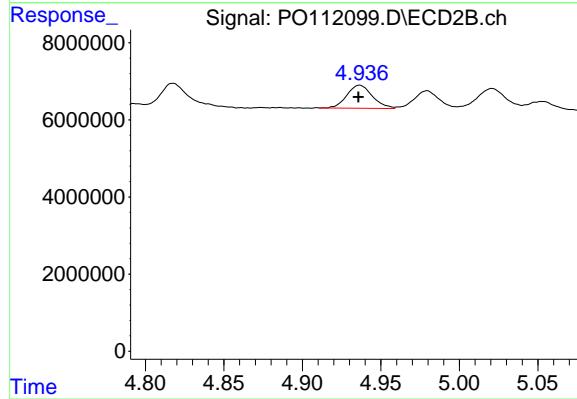


#18 AR-1242-3

R.T.: 4.937 min
Delta R.T.: 0.000 min
Response: 6736786
Conc: 44.91 ng/ml

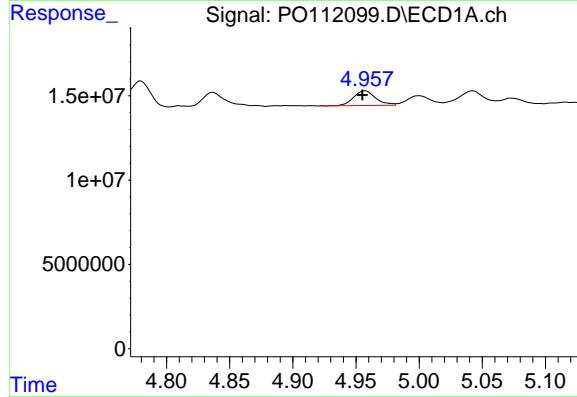


#19 AR-1242-4

R.T.: 4.957 min
Delta R.T.: 0.002 min
Response: 10638220
Conc: 45.90 ng/ml

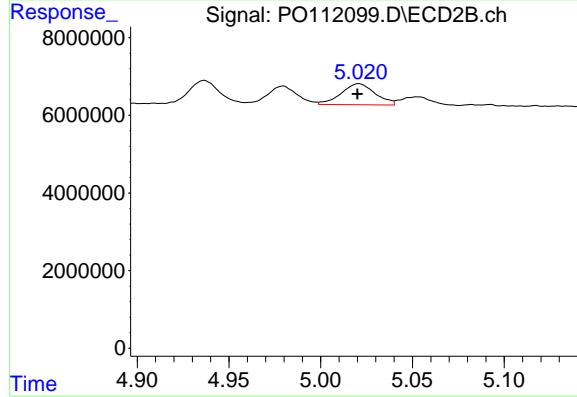

#19 AR-1242-4

R.T.: 5.021 min
Delta R.T.: 0.000 min
Response: 7029005
Conc: 48.94 ng/ml

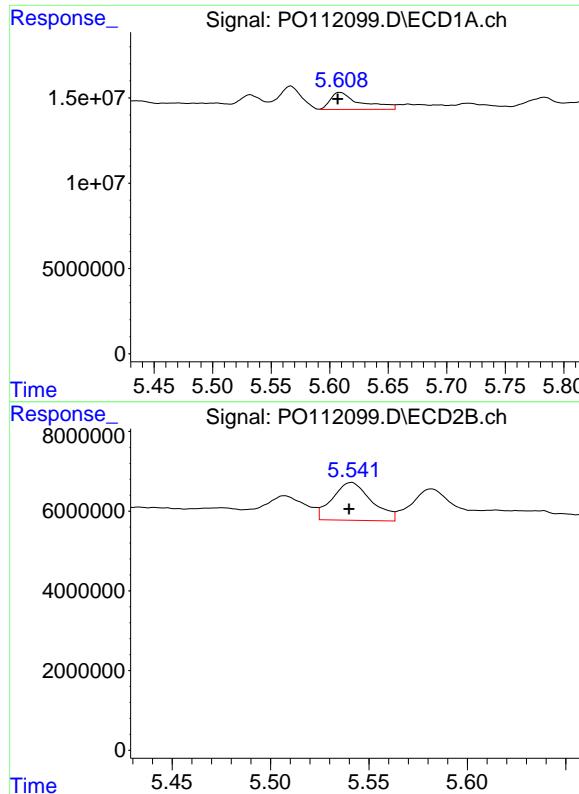

#20 AR-1242-5

R.T.: 5.609 min
Delta R.T.: 0.002 min
Response: 17753976
Conc: 79.07 ng/ml

Instrument: ECD_O
ClientSampleId: AR1242ICC050

#20 AR-1242-5

R.T.: 5.541 min
Delta R.T.: 0.001 min
Response: 13107939
Conc: 70.07 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0070825\
 Data File : P0112104.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jul 2025 18:59
 Operator : YP/AJ
 Sample : AR1248ICC050
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1248ICC050

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 09 02:45:42 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 09 02:41:59 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	3.673	3.666	43320523	27979420	4.113	4.205
2) SA Decachlor...	8.703	8.650	29248819	7966074	4.030	4.341

Target Compounds

21) L5 AR-1248-1	4.761	4.742	9816500	7672405	43.126	51.273
22) L5 AR-1248-2	4.999	4.979	13335961	9853335	43.403	48.509
23) L5 AR-1248-3	5.213	5.020	19880304	9961976	50.597	46.817
24) L5 AR-1248-4	5.567	5.191	27262638	13537632	47.367	53.399
25) L5 AR-1248-5	5.608	5.582	17126268	14613633	43.835	58.225 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0070825\
 Data File : P0112104.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jul 2025 18:59
 Operator : YP/AJ
 Sample : AR1248ICC050
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1248ICC050

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 09 02:45:42 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 09 02:41:59 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

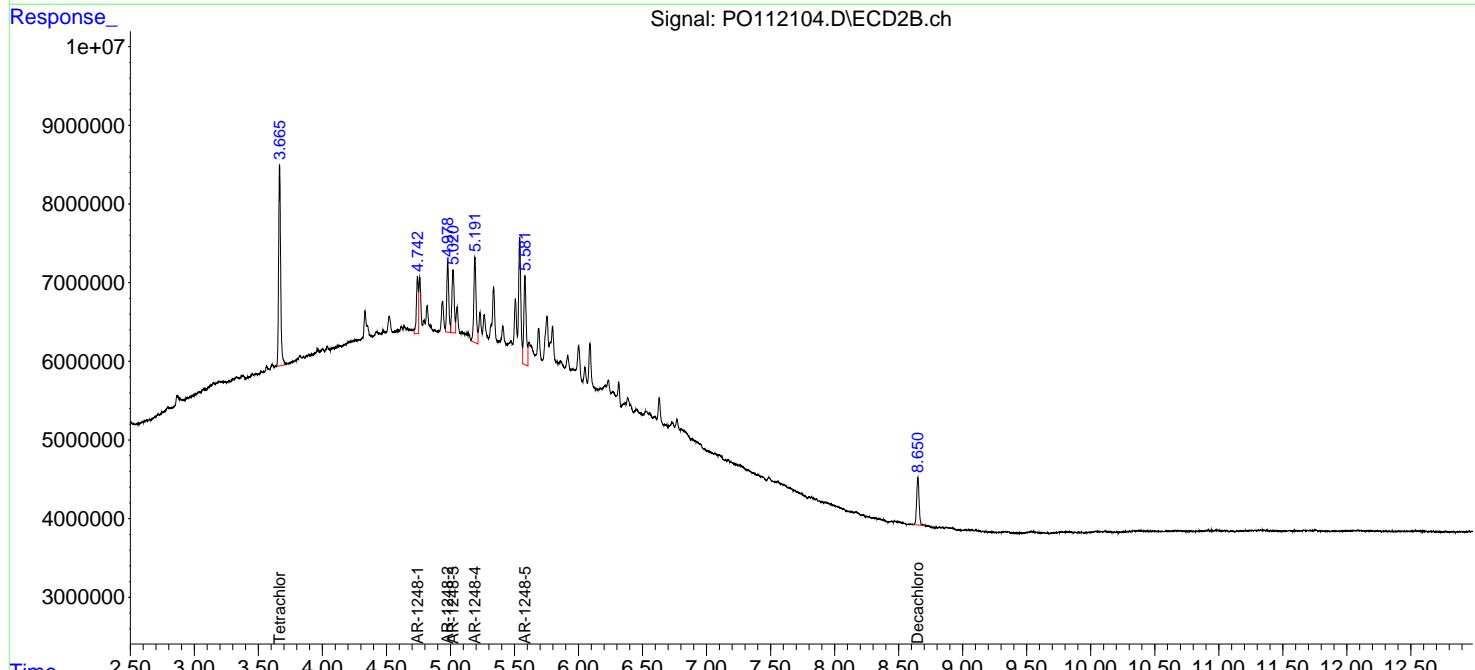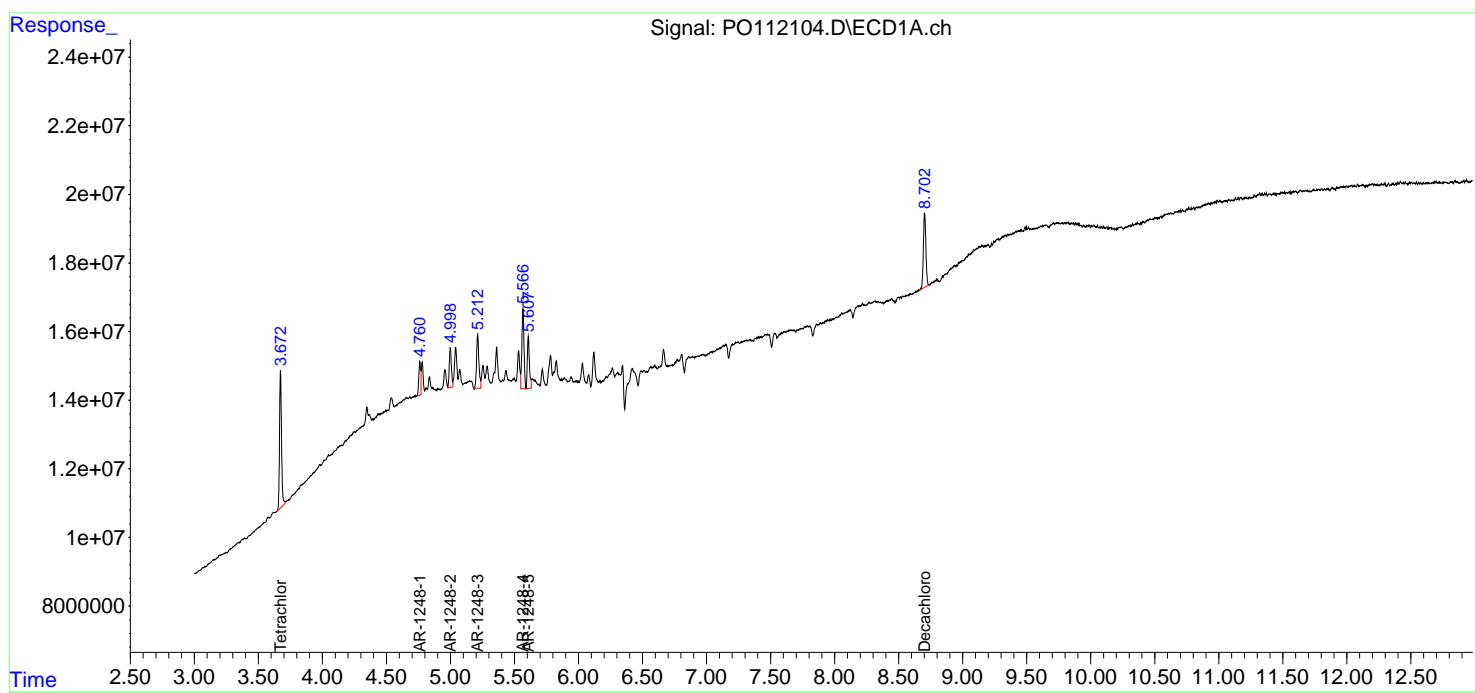

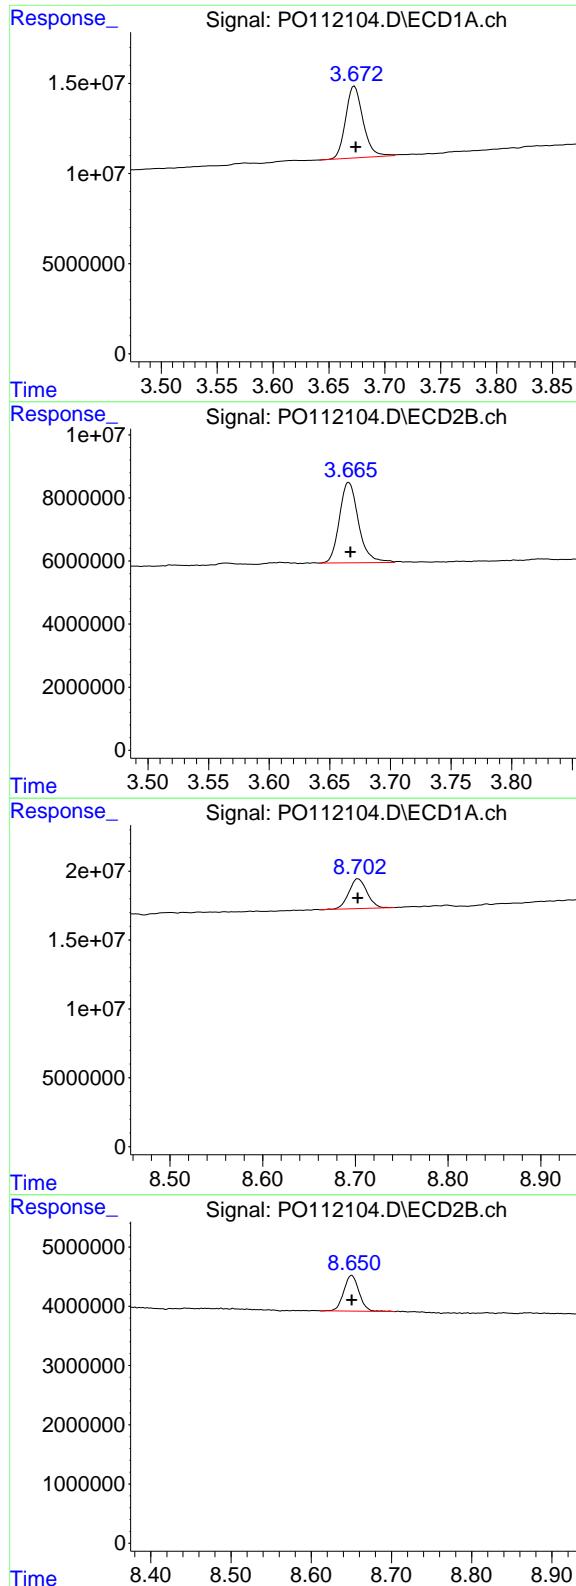

#1 Tetrachloro-m-xylene

R.T.: 3.673 min
 Delta R.T.: -0.001 min
 Response: 43320523
 Conc: 4.11 ng/ml

Instrument:

ECD_O

ClientSampleId :

AR1248ICC050

#1 Tetrachloro-m-xylene


R.T.: 3.666 min
 Delta R.T.: -0.001 min
 Response: 27979420
 Conc: 4.21 ng/ml

#2 Decachlorobiphenyl

R.T.: 8.703 min
 Delta R.T.: 0.000 min
 Response: 29248819
 Conc: 4.03 ng/ml

#2 Decachlorobiphenyl

R.T.: 8.650 min
 Delta R.T.: 0.000 min
 Response: 7966074
 Conc: 4.34 ng/ml

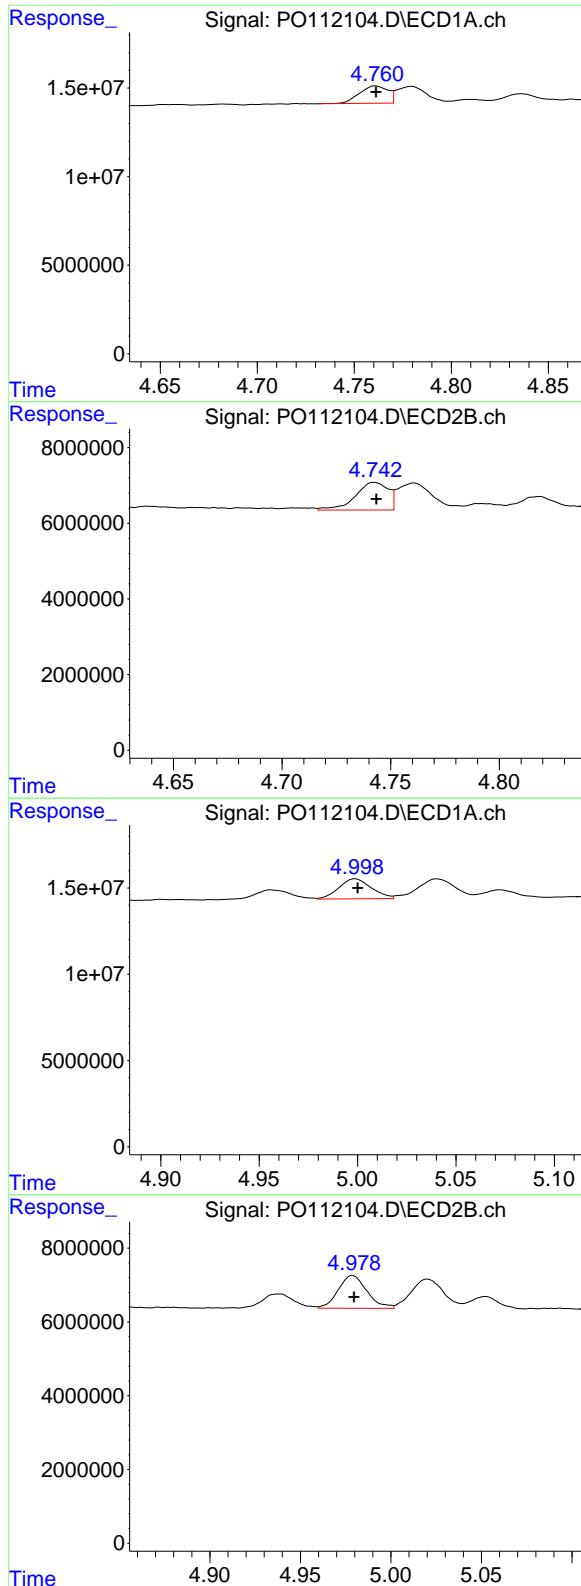

#21 AR-1248-1

R.T.: 4.761 min
 Delta R.T.: 0.000 min
 Response: 9816500
 Conc: 43.13 ng/ml

Instrument: ECD_O
 ClientSampleId: AR1248ICC050

#21 AR-1248-1


R.T.: 4.742 min
 Delta R.T.: -0.001 min
 Response: 7672405
 Conc: 51.27 ng/ml

#22 AR-1248-2

R.T.: 4.999 min
 Delta R.T.: -0.001 min
 Response: 13335961
 Conc: 43.40 ng/ml

#22 AR-1248-2

R.T.: 4.979 min
 Delta R.T.: 0.000 min
 Response: 9853335
 Conc: 48.51 ng/ml

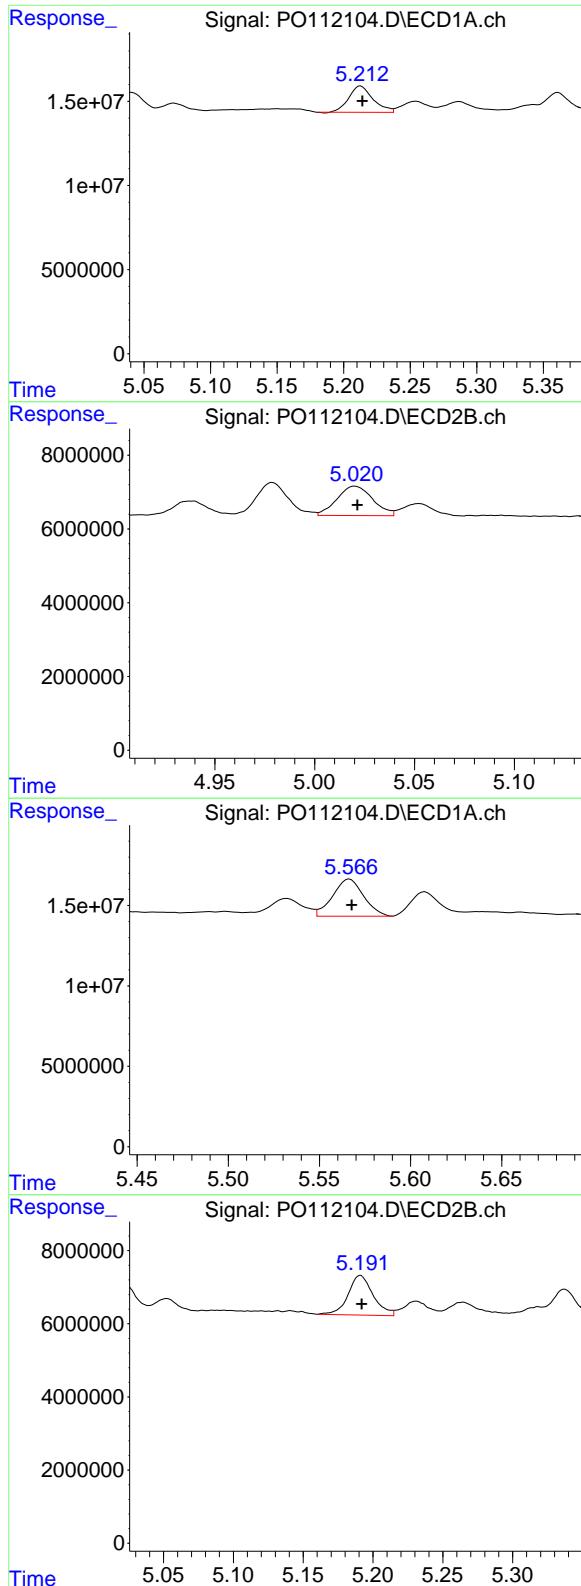

#23 AR-1248-3

R.T.: 5.213 min
 Delta R.T.: -0.001 min
 Response: 19880304
 Conc: 50.60 ng/ml

Instrument: ECD_O
 ClientSampleId: AR1248ICC050

#23 AR-1248-3


R.T.: 5.020 min
 Delta R.T.: -0.001 min
 Response: 9961976
 Conc: 46.82 ng/ml

#24 AR-1248-4

R.T.: 5.567 min
 Delta R.T.: -0.001 min
 Response: 27262638
 Conc: 47.37 ng/ml

#24 AR-1248-4

R.T.: 5.191 min
 Delta R.T.: -0.001 min
 Response: 13537632
 Conc: 53.40 ng/ml

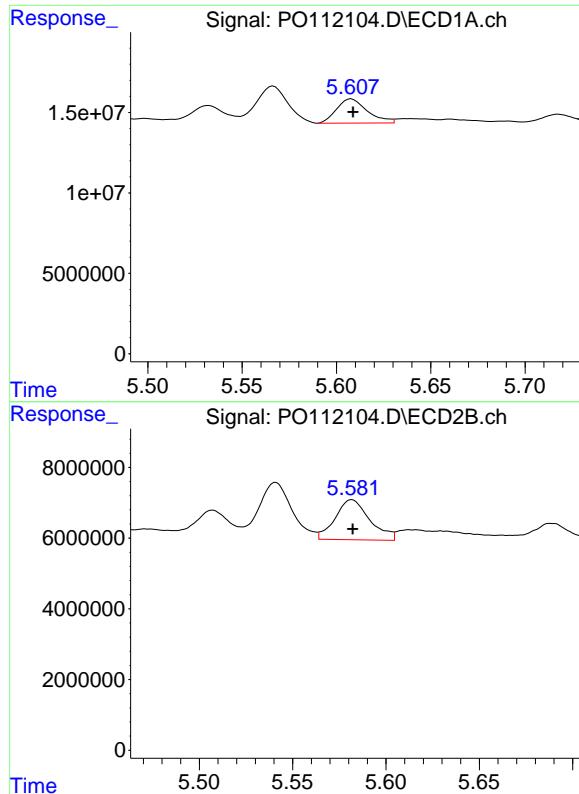

#25 AR-1248-5

R.T.: 5.608 min
Delta R.T.: -0.001 min
Response: 17126268
Conc: 43.84 ng/ml

Instrument: ECD_O
ClientSampleId: AR1248ICC050

#25 AR-1248-5

R.T.: 5.582 min
Delta R.T.: 0.000 min
Response: 14613633
Conc: 58.22 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0070825\
 Data File : P0112109.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jul 2025 20:28
 Operator : YP/AJ
 Sample : AR1254ICC050
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1254ICC050

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 09 03:13:58 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 09 03:10:24 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	3.672	3.666	45533046	29689581	4.236	4.372
2) SA Decachlor...	8.701	8.650	32557073	8527820	4.327	4.604

Target Compounds

26) L6 AR-1254-1	5.565	5.541	30856160	21377359	50.127	56.761
27) L6 AR-1254-2	5.714	5.688	25962033	19942992	48.227	61.182 #
28) L6 AR-1254-3	6.118	6.089	40531096	25609316	47.989	54.406
29) L6 AR-1254-4	6.346	6.316	23345099	12905837	44.210	48.800
30) L6 AR-1254-5	6.765	6.733	35718880	18096474	45.127	50.826



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0070825\
 Data File : P0112109.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jul 2025 20:28
 Operator : YP/AJ
 Sample : AR1254ICC050
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1254ICC050

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 09 03:13:58 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 09 03:10:24 2025
 Response via : Initial Calibration
 Integrator: ChemStation


Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

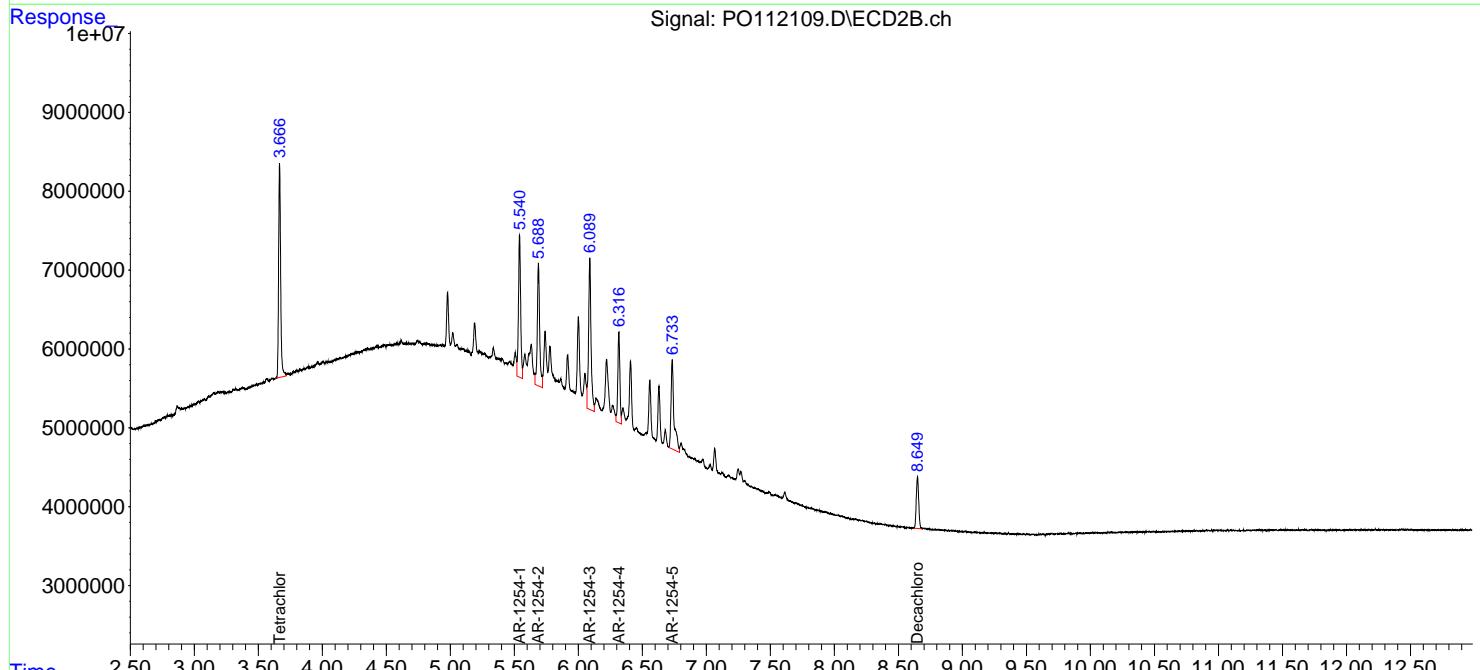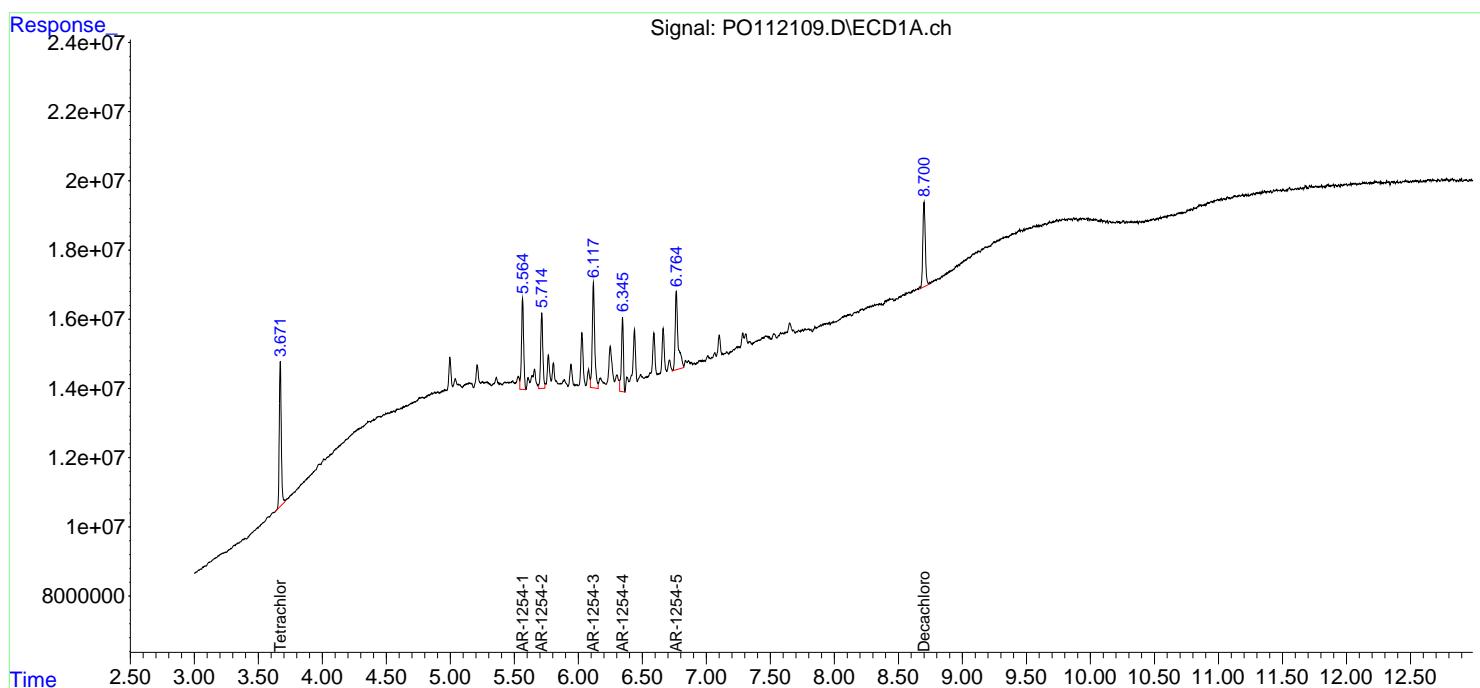

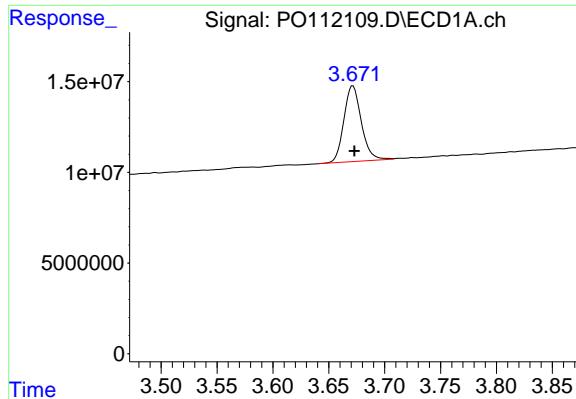


#1 Tetrachloro-m-xylene
R.T.: 3.672 min
Delta R.T.: -0.001 min
Response: 45533046
Conc: 4.24 ng/ml


Instrument: ECD_O
ClientSampleId: AR1254ICC050

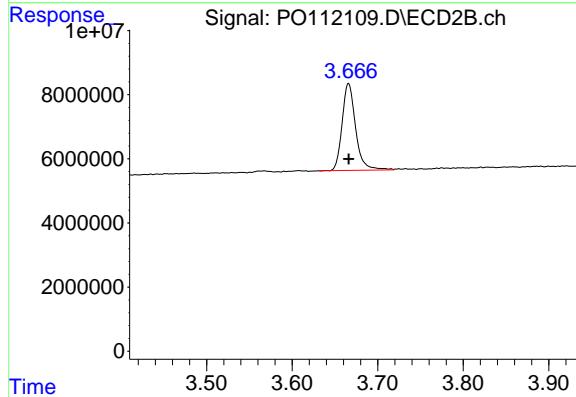


#1 Tetrachloro-m-xylene
R.T.: 3.666 min
Delta R.T.: 0.000 min
Response: 29689581
Conc: 4.37 ng/ml

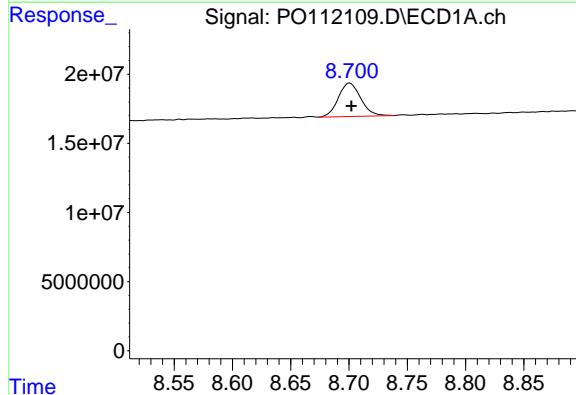

#2 Decachlorobiphenyl
R.T.: 8.701 min
Delta R.T.: -0.001 min
Response: 32557073
Conc: 4.33 ng/ml

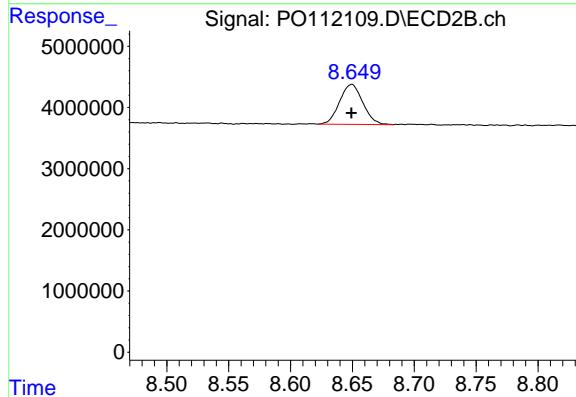

#2 Decachlorobiphenyl
R.T.: 8.650 min
Delta R.T.: 0.000 min
Response: 8527820
Conc: 4.60 ng/ml

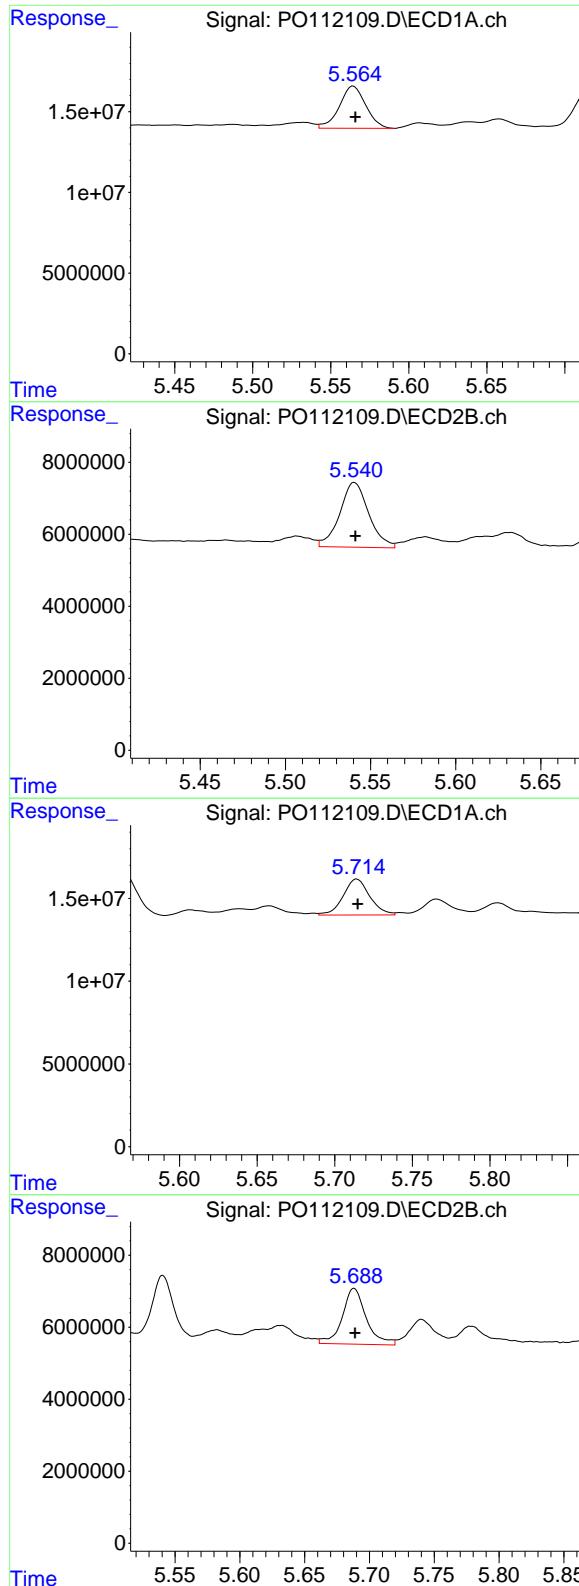

#26 AR-1254-1

R.T.: 5.565 min
 Delta R.T.: -0.001 min
 Response: 30856160
 Conc: 50.13 ng/ml

Instrument: ECD_O
ClientSampleId: AR1254ICC050

#26 AR-1254-1


R.T.: 5.541 min
 Delta R.T.: 0.000 min
 Response: 21377359
 Conc: 56.76 ng/ml

#27 AR-1254-2

R.T.: 5.714 min
 Delta R.T.: 0.000 min
 Response: 25962033
 Conc: 48.23 ng/ml

#27 AR-1254-2

R.T.: 5.688 min
 Delta R.T.: 0.000 min
 Response: 19942992
 Conc: 61.18 ng/ml

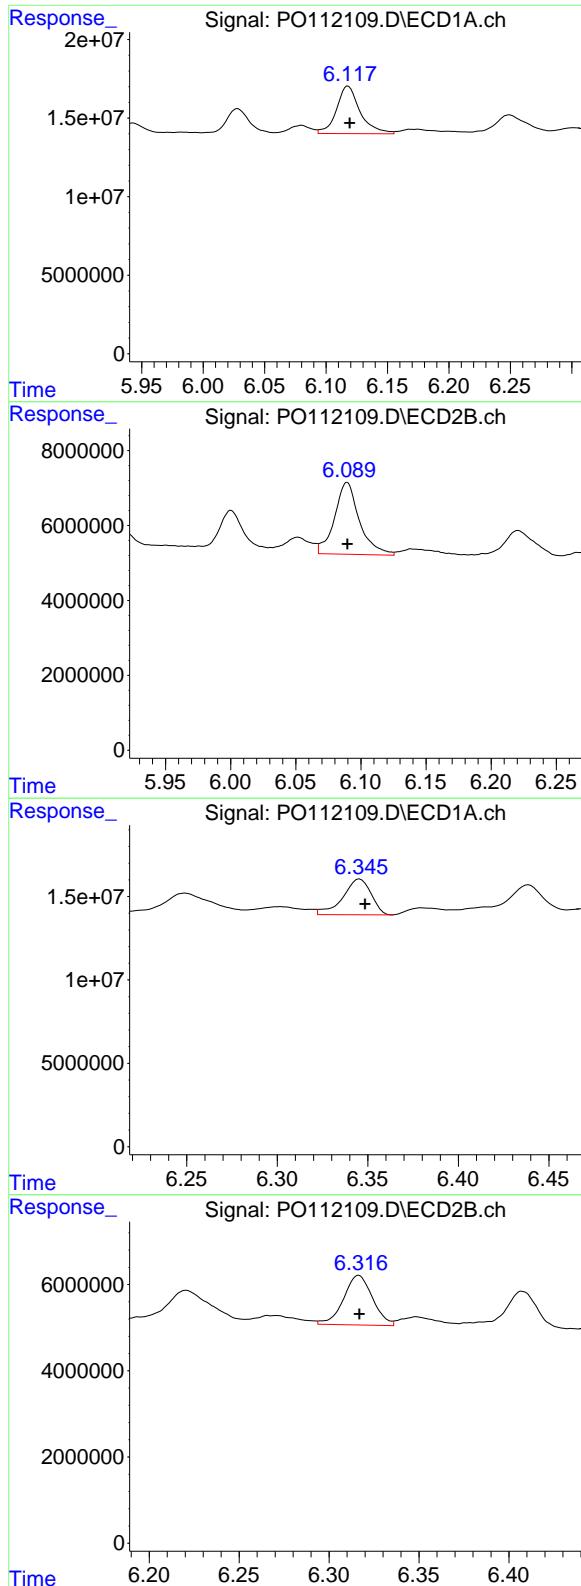

#28 AR-1254-3

R.T.: 6.118 min
 Delta R.T.: -0.001 min
 Response: 40531096
 Conc: 47.99 ng/ml

Instrument: ECD_O
 ClientSampleId: AR1254ICC050

#28 AR-1254-3


R.T.: 6.089 min
 Delta R.T.: 0.000 min
 Response: 25609316
 Conc: 54.41 ng/ml

#29 AR-1254-4

R.T.: 6.346 min
 Delta R.T.: -0.003 min
 Response: 23345099
 Conc: 44.21 ng/ml

#29 AR-1254-4

R.T.: 6.316 min
 Delta R.T.: 0.000 min
 Response: 12905837
 Conc: 48.80 ng/ml

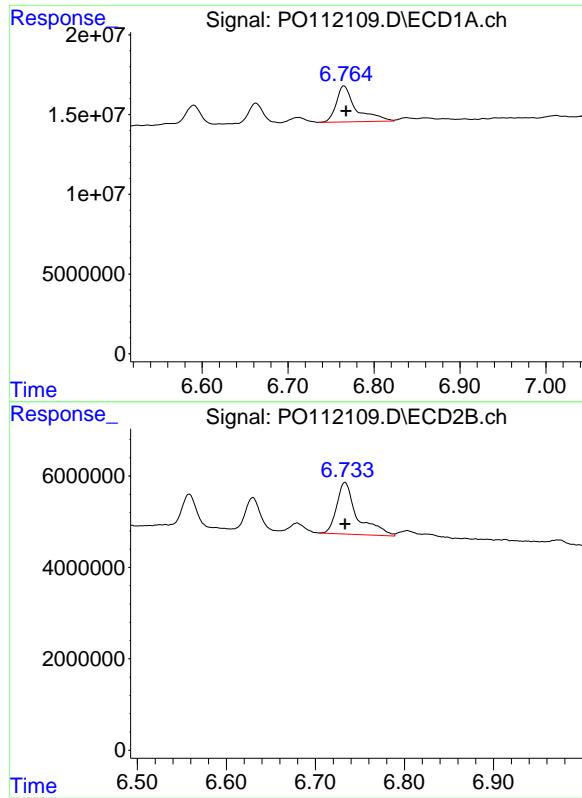

#30 AR-1254-5

R.T.: 6.765 min
Delta R.T.: -0.002 min
Response: 35718880
Conc: 45.13 ng/ml

Instrument: ECD_O
ClientSampleId: AR1254ICC050

#30 AR-1254-5

R.T.: 6.733 min
Delta R.T.: 0.000 min
Response: 18096474
Conc: 50.83 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0070825\
 Data File : P0112111.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jul 2025 21:04
 Operator : YP/AJ
 Sample : AR1268ICC1000
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1268ICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 09 03:41:55 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 09 03:33:24 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	3.672	3.667	1082.8E6	673.3E6	101.066	99.562
2) SA Decachlor...	8.702	8.650	1378.0E6	313.9E6	99.628	96.478

Target Compounds

41) L9 AR-1268-1	7.590	7.554	1933.7E6	486.6E6	1000.189	974.104
42) L9 AR-1268-2	7.656	7.619	1621.3E6	414.1E6	997.801	973.991
43) L9 AR-1268-3	7.862	7.823	1337.7E6	309.6E6	989.536	960.409
44) L9 AR-1268-4	8.151	8.111	513.2E6	111.4E6	998.446	963.536
45) L9 AR-1268-5	8.445	8.399	3474.7E6	736.5E6	1008.979	983.566



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0070825\
 Data File : P0112111.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jul 2025 21:04
 Operator : YP/AJ
 Sample : AR1268ICC1000
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1268ICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 09 03:41:55 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 09 03:33:24 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

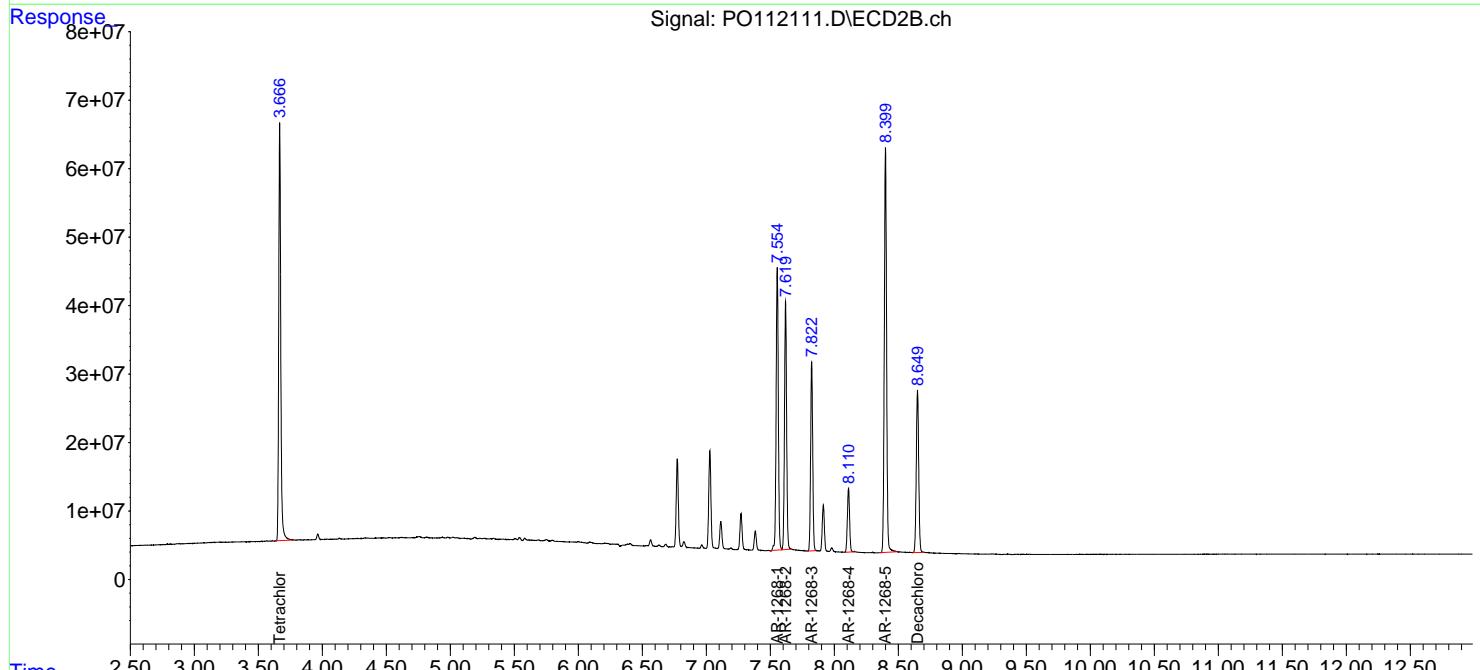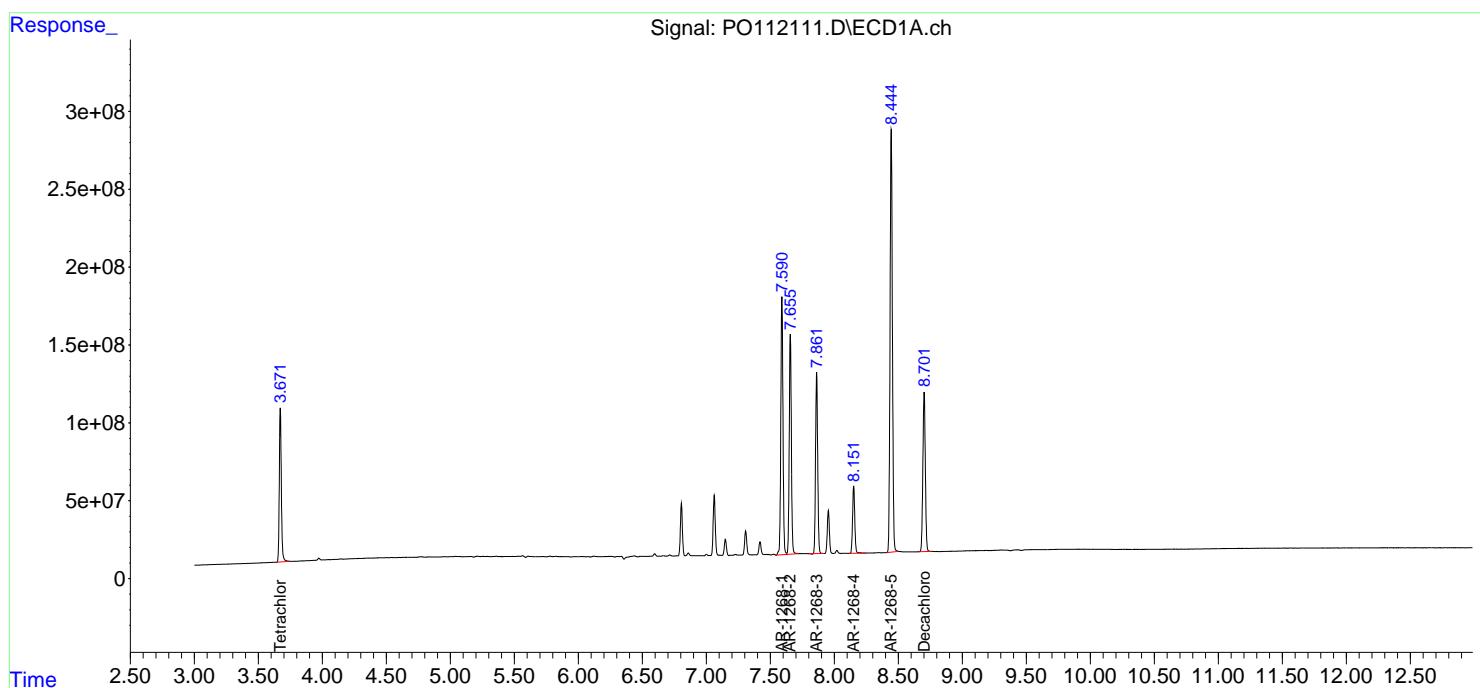

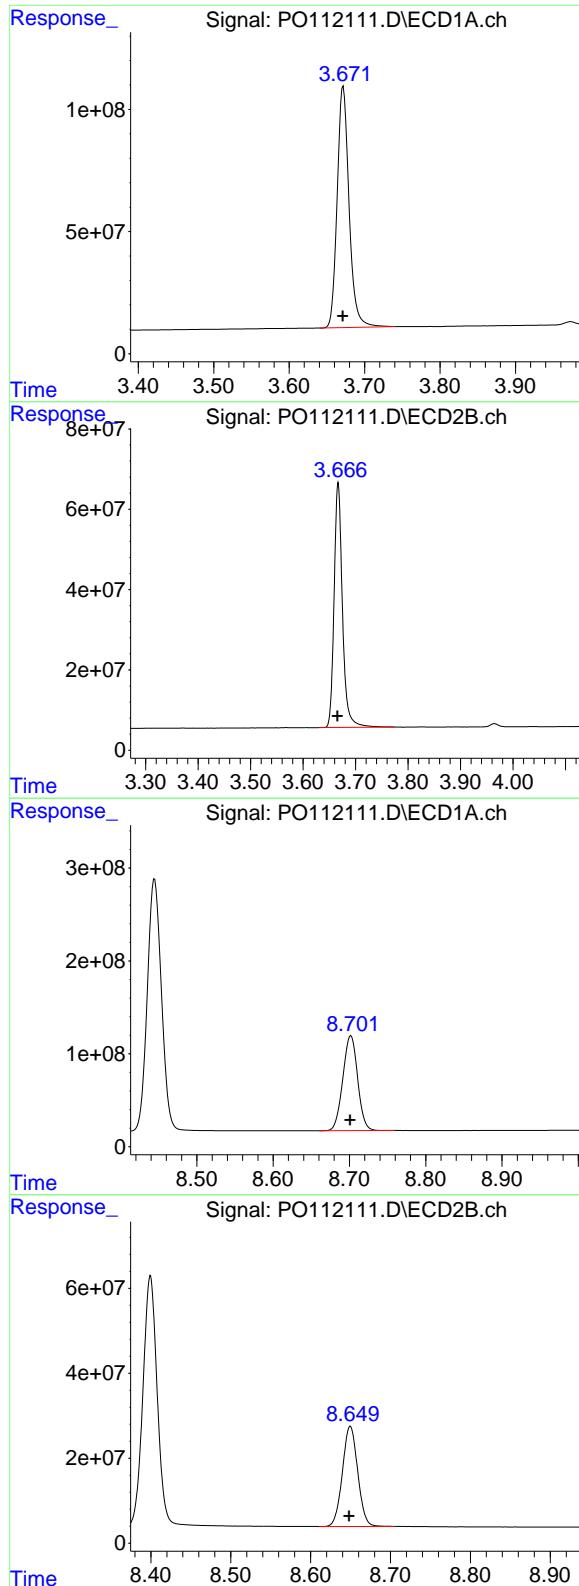

#1 Tetrachloro-m-xylene

R.T.: 3.672 min
Delta R.T.: 0.000 min
Response: 1082841647
Conc: 101.07 ng/ml

Instrument:

ECD_O

ClientSampleId :

AR1268ICC1000

#1 Tetrachloro-m-xylene


R.T.: 3.667 min
Delta R.T.: 0.001 min
Response: 673253587
Conc: 99.56 ng/ml

#2 Decachlorobiphenyl

R.T.: 8.702 min
Delta R.T.: 0.000 min
Response: 1377978961
Conc: 99.63 ng/ml

#2 Decachlorobiphenyl

R.T.: 8.650 min
Delta R.T.: 0.002 min
Response: 313919147
Conc: 96.48 ng/ml

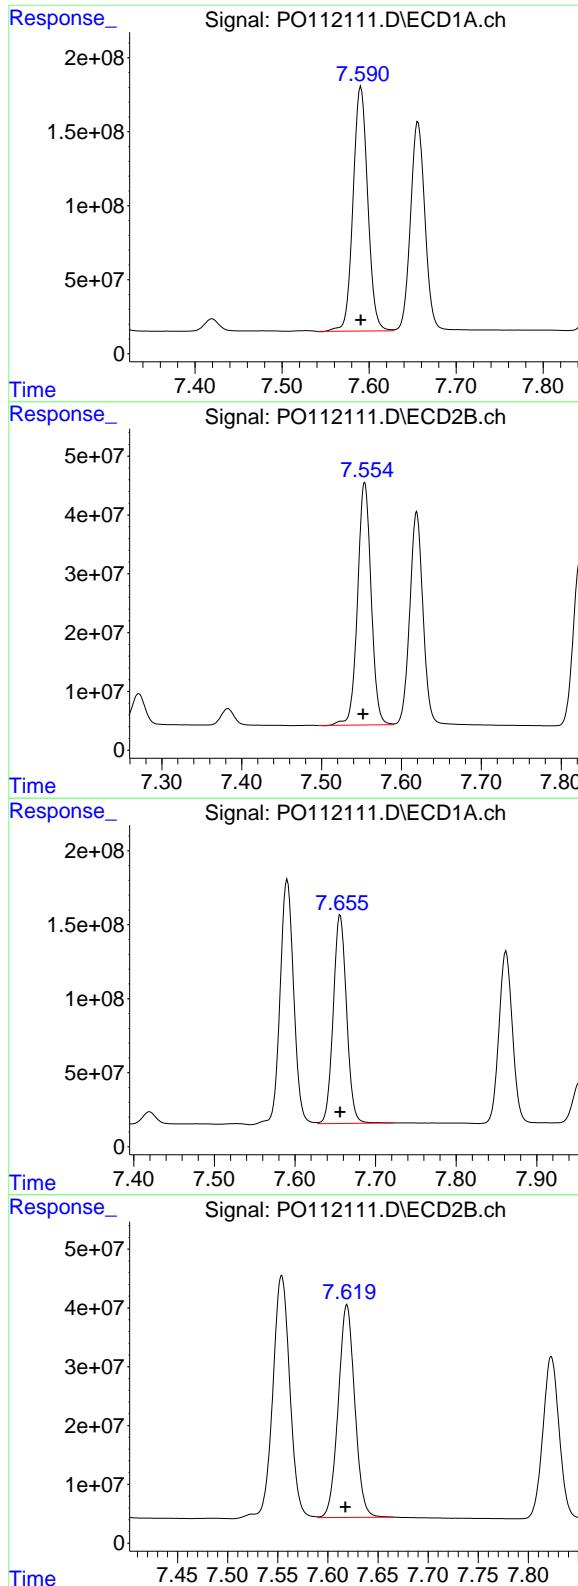

#41 AR-1268-1

R.T.: 7.590 min
Delta R.T.: 0.000 min **Instrument:**
Response: 1933697823 ECD_O
Conc: 1000.19 ng/ml **ClientSampleId:**
AR1268ICC1000

#41 AR-1268-1


R.T.: 7.554 min
Delta R.T.: 0.002 min
Response: 486556055
Conc: 974.10 ng/ml

#42 AR-1268-2

R.T.: 7.656 min
Delta R.T.: 0.000 min
Response: 1621310763
Conc: 997.80 ng/ml

#42 AR-1268-2

R.T.: 7.619 min
Delta R.T.: 0.002 min
Response: 414074889
Conc: 973.99 ng/ml

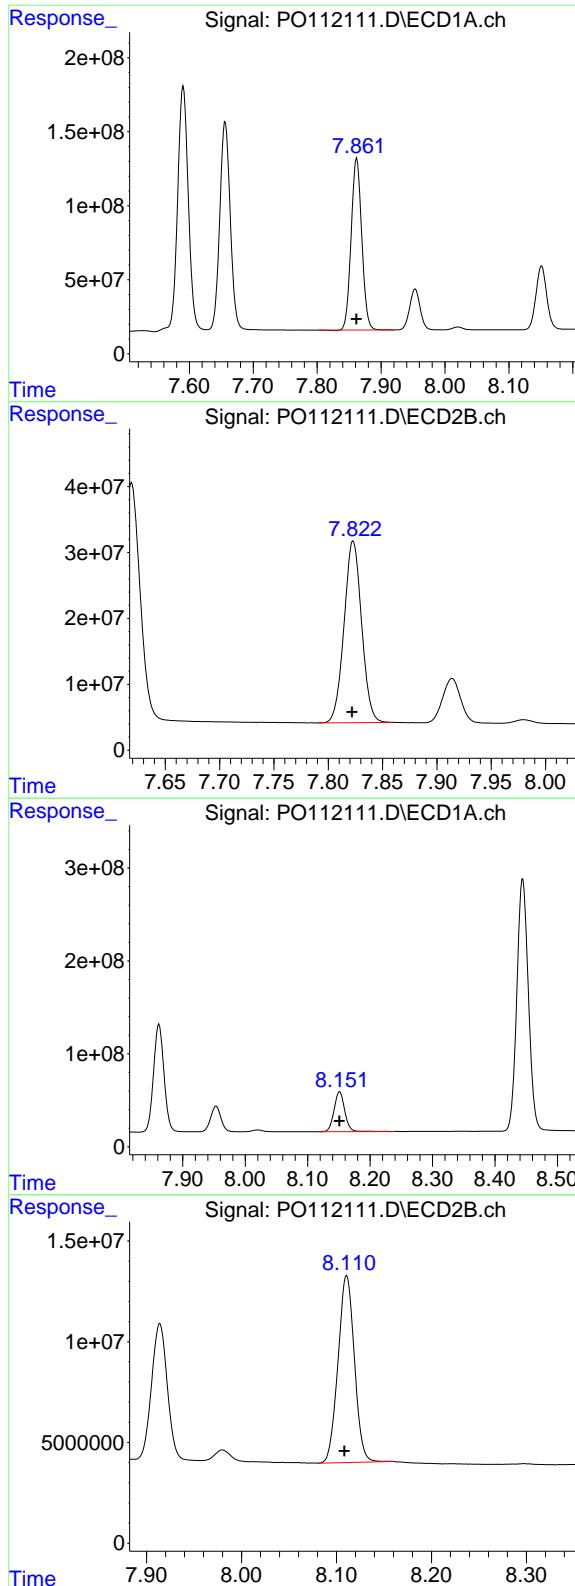

#43 AR-1268-3

R.T.: 7.862 min
 Delta R.T.: 0.000 min
Instrument:
 Response: 1337748865 ECD_O
 Conc: 989.54 ng/ml
ClientSampleId :
 AR1268ICC1000

#43 AR-1268-3


R.T.: 7.823 min
 Delta R.T.: 0.001 min
 Response: 309607188
 Conc: 960.41 ng/ml

#44 AR-1268-4

R.T.: 8.151 min
 Delta R.T.: 0.000 min
 Response: 513241738
 Conc: 998.45 ng/ml

#44 AR-1268-4

R.T.: 8.111 min
 Delta R.T.: 0.002 min
 Response: 111375490
 Conc: 963.54 ng/ml

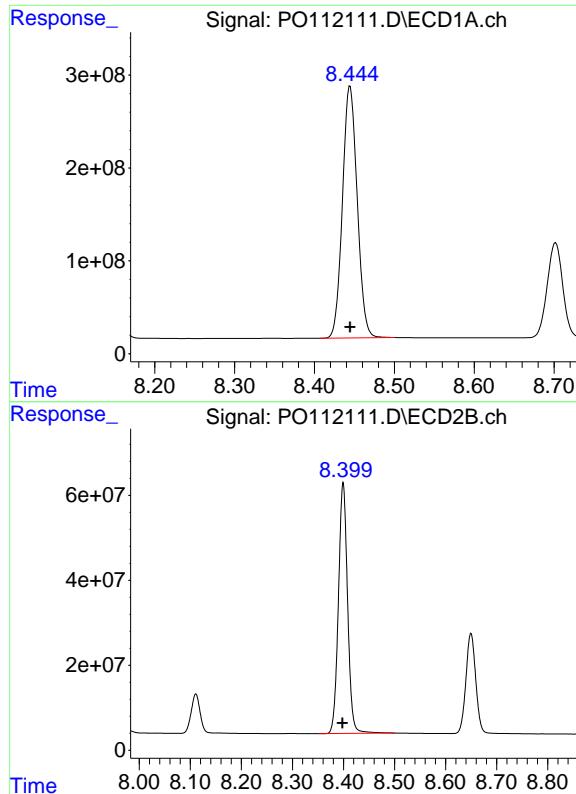

#45 AR-1268-5

R.T.: 8.445 min
Delta R.T.: 0.000 min
Response: 3474681887
Conc: 1008.98 ng/ml

Instrument: ECD_O
ClientSampleId: AR1268ICC1000

#45 AR-1268-5

R.T.: 8.399 min
Delta R.T.: 0.002 min
Response: 736492551
Conc: 983.57 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0070825\
 Data File : P0112115.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jul 2025 22:16
 Operator : YP/AJ
 Sample : AR1268ICC050
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1268ICC050

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 09 03:42:35 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 09 03:33:24 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	3.674	3.666	38867548	25586379	3.628	3.784
2) SA Decachlor...	8.703	8.649	53087700	13607316	3.838	4.182

Target Compounds

41) L9 AR-1268-1	7.592	7.553	74576160	23025590	38.574	46.098
42) L9 AR-1268-2	7.658	7.618	64617530	19259498	39.767	45.302
43) L9 AR-1268-3	7.863	7.822	50498893	14843274	37.354	46.044
44) L9 AR-1268-4	8.154	8.109	18826938	4939808	36.625	42.735
45) L9 AR-1268-5	8.447	8.398	127.8E6	32095228	37.097	42.862



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0070825\
 Data File : P0112115.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jul 2025 22:16
 Operator : YP/AJ
 Sample : AR1268ICC050
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1268ICC050

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 09 03:42:35 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 09 03:33:24 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

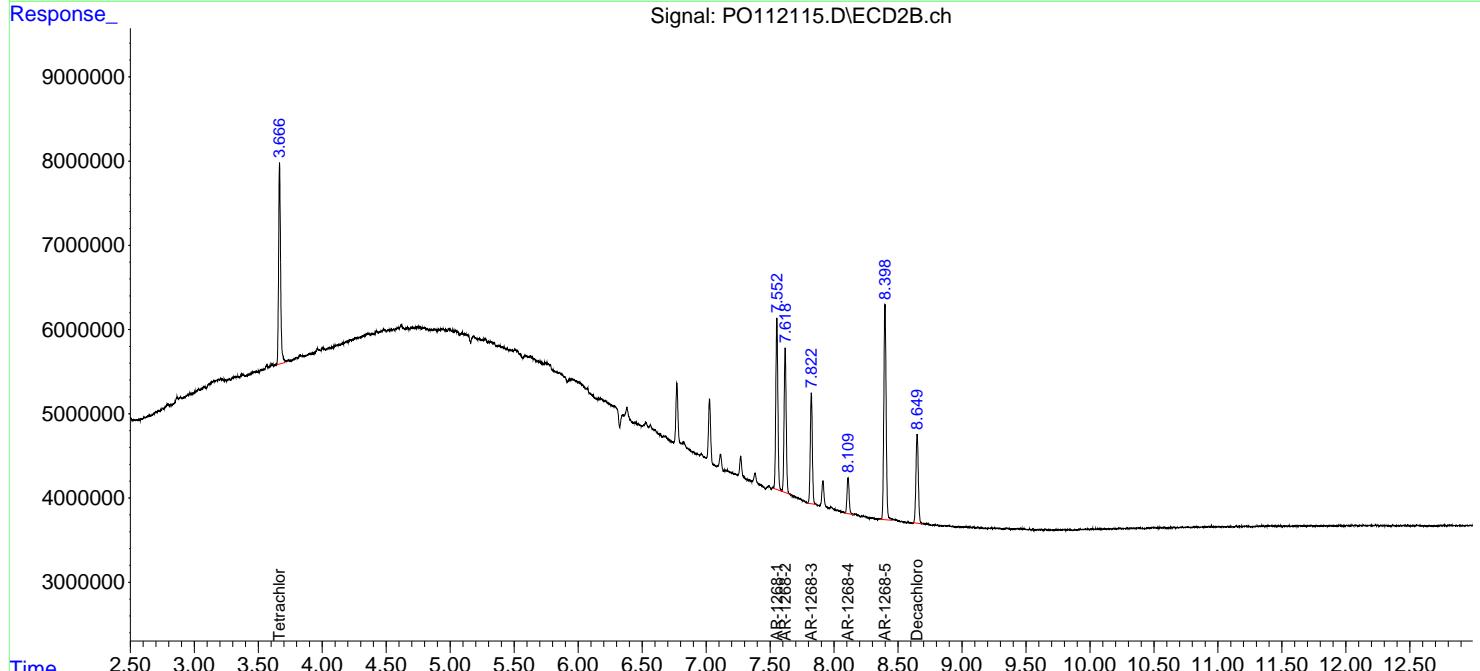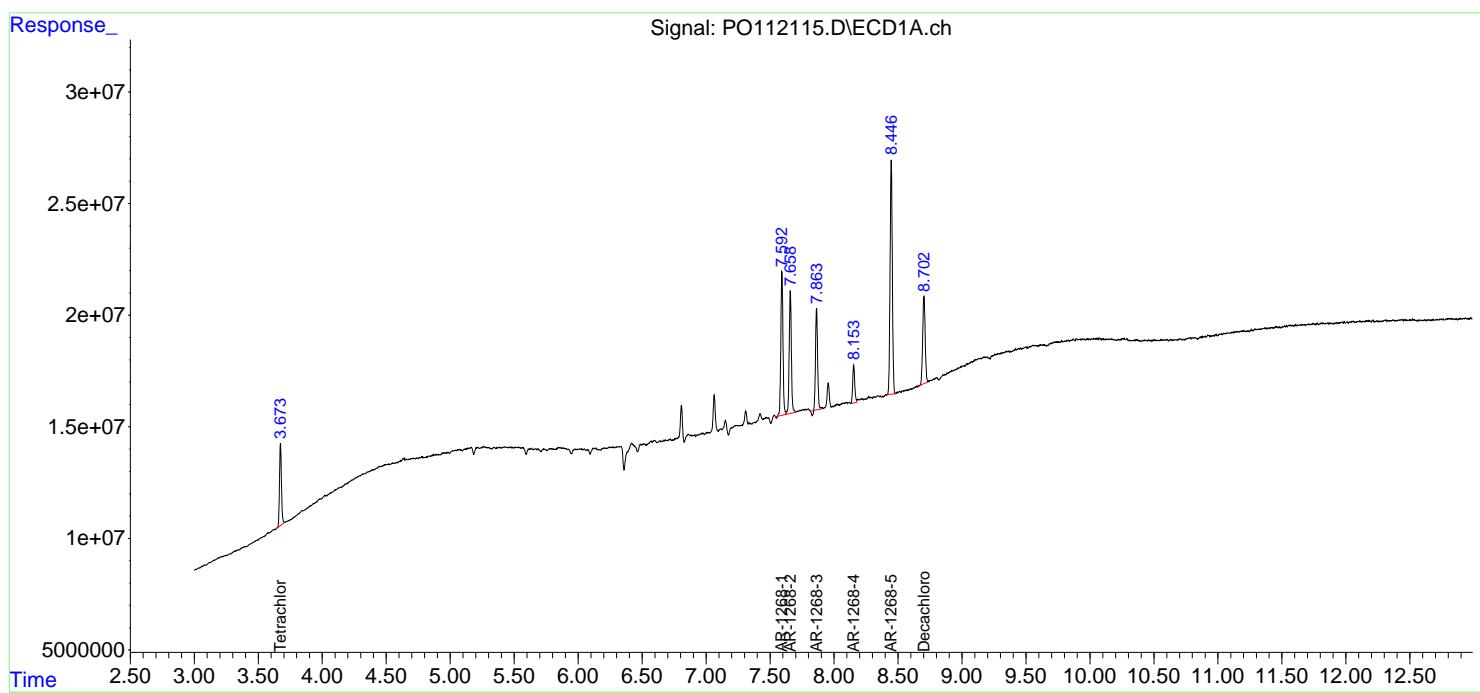


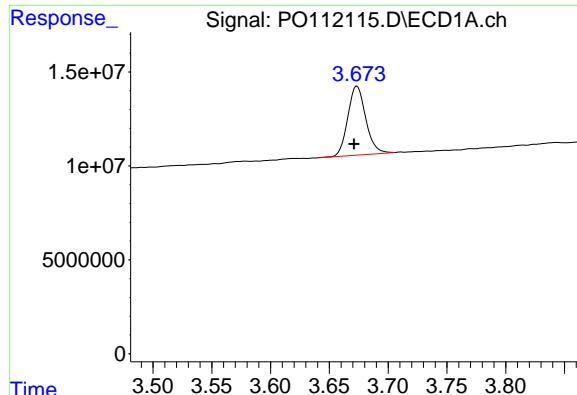

#1 Tetrachloro-m-xylene


R.T.: 3.674 min
Delta R.T.: 0.003 min
Response: 38867548
Conc: 3.63 ng/ml

Instrument: ECD_O
ClientSampleId: AR1268ICC050

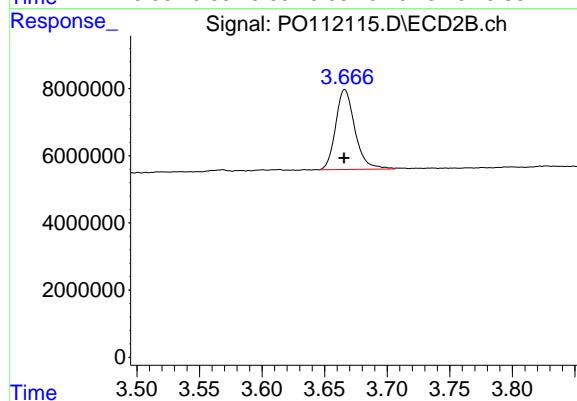


#1 Tetrachloro-m-xylene

R.T.: 3.666 min
Delta R.T.: 0.000 min
Response: 25586379
Conc: 3.78 ng/ml

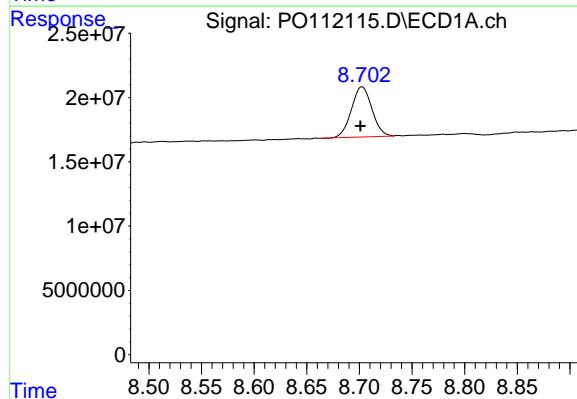


#2 Decachlorobiphenyl

R.T.: 8.703 min
Delta R.T.: 0.002 min
Response: 53087700
Conc: 3.84 ng/ml

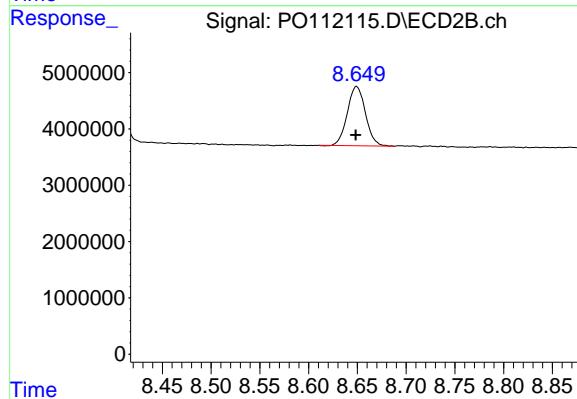

#2 Decachlorobiphenyl

R.T.: 8.649 min
Delta R.T.: 0.001 min
Response: 13607316
Conc: 4.18 ng/ml

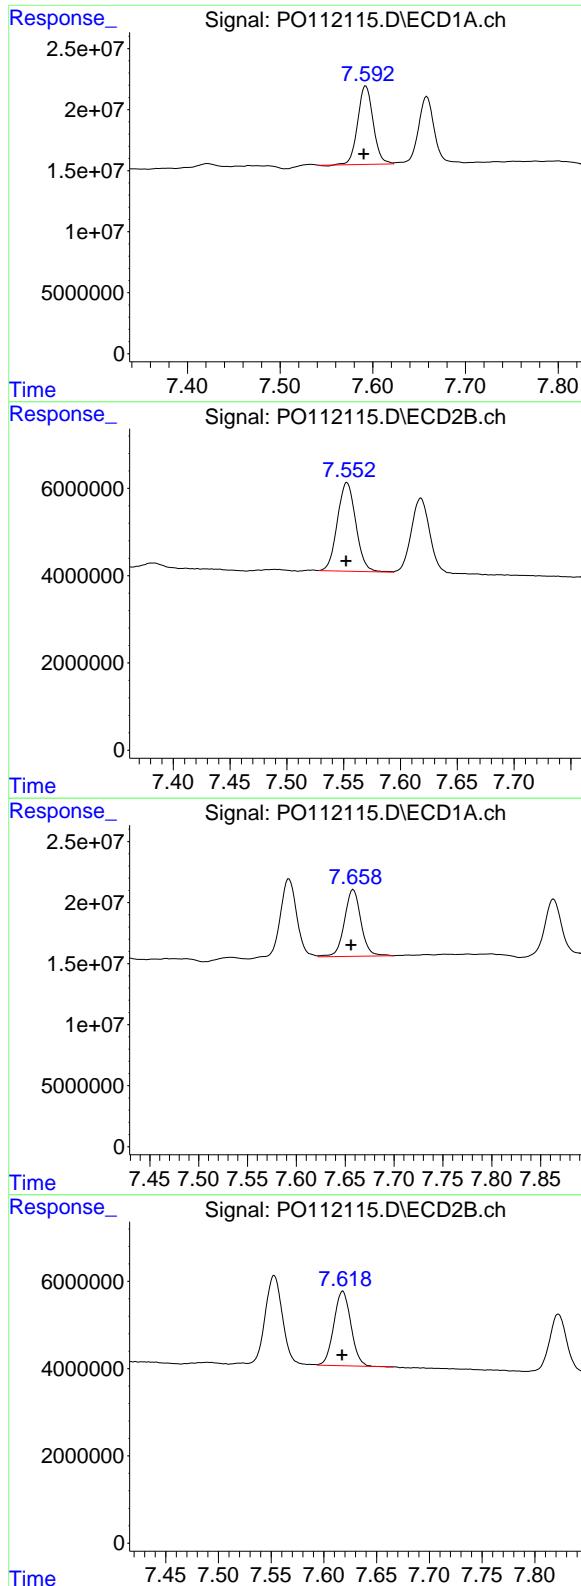

#41 AR-1268-1

R.T.: 7.592 min
 Delta R.T.: 0.002 min
 Response: 74576160
 Conc: 38.57 ng/ml

Instrument: ECD_O
 ClientSampleId: AR1268ICC050

#41 AR-1268-1


R.T.: 7.553 min
 Delta R.T.: 0.000 min
 Response: 23025590
 Conc: 46.10 ng/ml

#42 AR-1268-2

R.T.: 7.658 min
 Delta R.T.: 0.002 min
 Response: 64617530
 Conc: 39.77 ng/ml

#42 AR-1268-2

R.T.: 7.618 min
 Delta R.T.: 0.000 min
 Response: 19259498
 Conc: 45.30 ng/ml

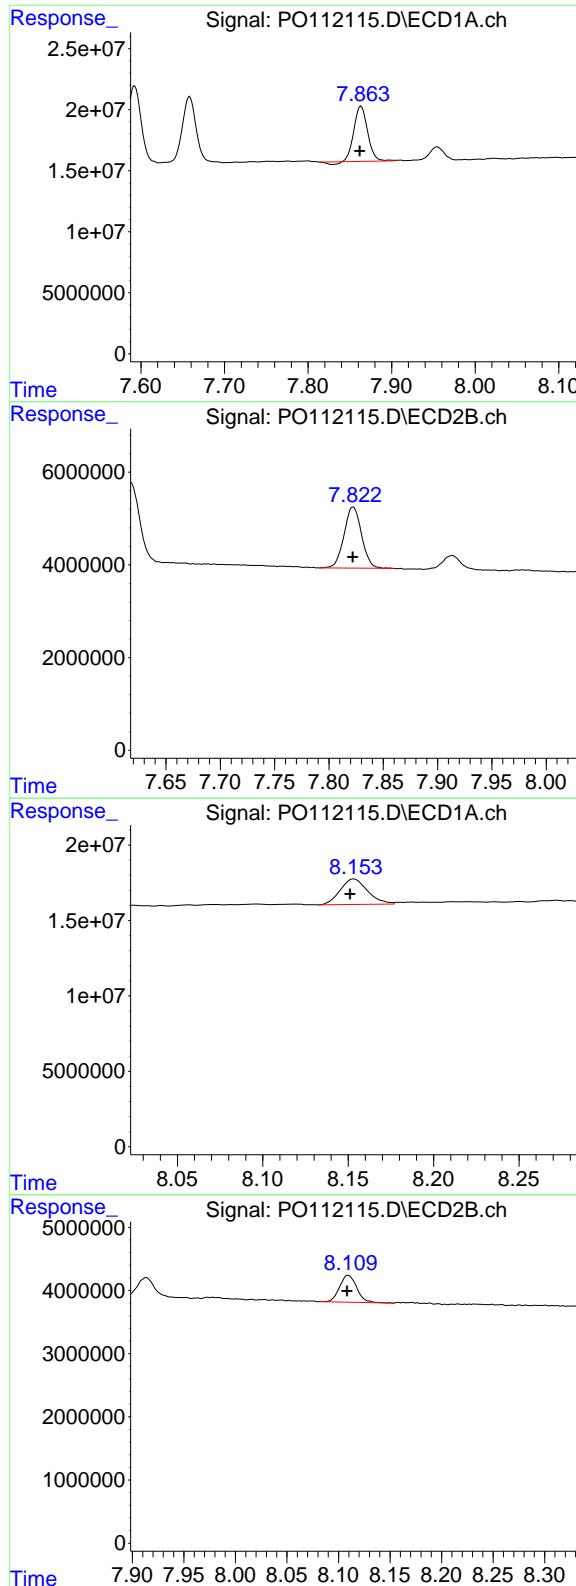

#43 AR-1268-3

R.T.: 7.863 min
Delta R.T.: 0.002 min **Instrument:**
Response: 50498893 ECD_O
Conc: 37.35 ng/ml **ClientSampleId:**
AR1268ICC050

#43 AR-1268-3


R.T.: 7.822 min
Delta R.T.: 0.000 min
Response: 14843274
Conc: 46.04 ng/ml

#44 AR-1268-4

R.T.: 8.154 min
Delta R.T.: 0.002 min
Response: 18826938
Conc: 36.63 ng/ml

#44 AR-1268-4

R.T.: 8.109 min
Delta R.T.: 0.000 min
Response: 4939808
Conc: 42.74 ng/ml

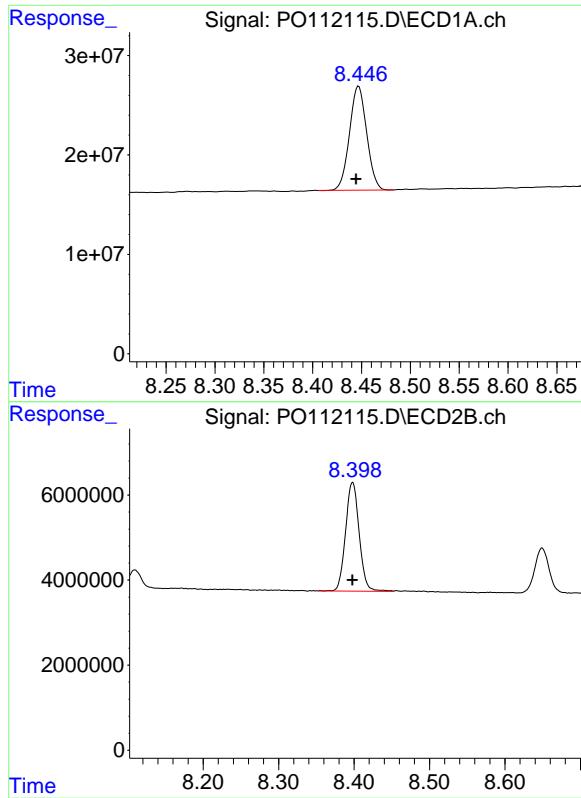

#45 AR-1268-5

R.T.: 8.447 min
Delta R.T.: 0.002 min
Response: 127752115
Conc: 37.10 ng/ml

Instrument: ECD_O
ClientSampleId: AR1268ICC050

#45 AR-1268-5

R.T.: 8.398 min
Delta R.T.: 0.000 min
Response: 32095228
Conc: 42.86 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0070825\
 Data File : P0112116.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jul 2025 22:34
 Operator : YP/AJ
 Sample : P0070825ICV500
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
ICVPO070825

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 09 04:04:41 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 09 04:02:23 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	3.672	3.666	521.7E6	329.9E6	52.728	51.784
2) SA Decachlor...	8.702	8.649	362.0E6	87909411	52.944	51.007

Target Compounds

3) L1 AR-1016-1	4.760	4.761	175.3E6	164.0E6	515.284	736.075 #
4) L1 AR-1016-2	4.779	4.792	259.8E6	11895525	522.388	36.146 #
5) L1 AR-1016-3	4.836	4.936	165.0E6	85046592	509.600	500.666
6) L1 AR-1016-4	4.956	4.979	132.8E6	68299058	517.300	497.707
7) L1 AR-1016-5	5.213	5.190	137.8E6	89116759	503.683	516.768
8) L2 AR-1221-1	3.883	3.873	15947935	11246969	136.758	136.666
9) L2 AR-1221-2	3.971	3.961	21794231	16662019	276.434	280.725
10) L2 AR-1221-3	4.046	4.036	87428058	61302785	324.310	324.737
11) L3 AR-1232-1	4.046	4.036	87428058	61302785	407.272	408.415
12) L3 AR-1232-2	4.539	4.761	132.6E6	164.0E6	1166.980	1071.444
13) L3 AR-1232-3	4.779	4.936	259.8E6	85046592	1134.364	1126.355
14) L3 AR-1232-4	4.956	5.020	132.8E6	81017586	1162.259	1227.759
15) L3 AR-1232-5	4.998	5.190	102.3E6	89116759	1393.978	1200.065
16) L4 AR-1242-1	4.760	4.742	175.3E6	109.9E6	605.102	566.708
17) L4 AR-1242-2	4.779	4.761	259.8E6	164.0E6	609.926	578.865
18) L4 AR-1242-3	4.836	4.936	165.0E6	85046592	602.752	583.801
19) L4 AR-1242-4	4.956	5.020	132.8E6	81017586	589.577	571.187
20) L4 AR-1242-5	5.607	5.540	29284624	86955161	138.350	478.475 #
21) L5 AR-1248-1	4.760	4.742	175.3E6	109.9E6	772.411	711.683
22) L5 AR-1248-2	4.998	4.979	102.3E6	68299058	331.852	331.923
23) L5 AR-1248-3	5.213	5.020	137.8E6	81017586	338.404	377.180
24) L5 AR-1248-4	5.566	5.190	135.0E6	89116759	233.845	344.444 #
25) L5 AR-1248-5	5.607	5.581	29284624	22496977	75.030	89.791
26) L6 AR-1254-1	5.566	5.540	135.0E6	86955161	219.411	228.128
27) L6 AR-1254-2	5.715	5.688	90019733	62065631	168.046	187.051
28) L6 AR-1254-3	6.135	6.105	227.7E6	108.7E6	271.151	225.457
29) L6 AR-1254-4	6.347	6.316	25832693	12233696	53.704	46.927
30) L6 AR-1254-5	6.767	6.732	353.7E6	156.0E6	456.992	437.848
31) L7 AR-1260-1	6.250	6.220	257.1E6	138.6E6	512.929	493.882
32) L7 AR-1260-2	6.440	6.408	380.3E6	165.9E6	515.168	487.864
33) L7 AR-1260-3	6.806	6.559	331.7E6	128.1E6	506.110	464.787
34) L7 AR-1260-4	7.065	7.065	235.9E6	12589968	541.983	62.747 #
35) L7 AR-1260-5	7.308	7.271	694.1E6	218.4E6	549.787	487.907
36) L8 AR-1262-1	6.806	6.771	331.7E6	137.5E6	324.704	337.557
37) L8 AR-1262-2	7.308	7.271	694.1E6	218.4E6	423.410	426.203
38) L8 AR-1262-3	7.592	7.552	161.8E6	44636216	252.033	248.636
39) L8 AR-1262-4	7.655	7.616	445.6E6	119.2E6	415.901	409.608
40) L8 AR-1262-5	8.153	8.109	146.1E6	33885824	325.982	320.332
41) L9 AR-1268-1	7.592	7.552	161.8E6	44636216	88.056	90.825

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0070825\
 Data File : P0112116.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jul 2025 22:34
 Operator : YP/AJ
 Sample : P0070825ICV500
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
ICVPO070825

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 09 04:04:41 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 09 04:02:23 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9 AR-1268-2	7.655	7.616	445.6E6	119.2E6	286.087	285.635
43) L9 AR-1268-3	7.863	7.821	2769823	2396044	2.131	7.573 #
44) L9 AR-1268-4	8.153	8.109	146.1E6	33885824	304.087	303.876
45) L9 AR-1268-5	8.446	8.398	35455171	8565740	10.863	11.790



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0070825\
 Data File : P0112116.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jul 2025 22:34
 Operator : YP/AJ
 Sample : P0070825ICV500
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 ICPPO070825

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 09 04:04:41 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 09 04:02:23 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

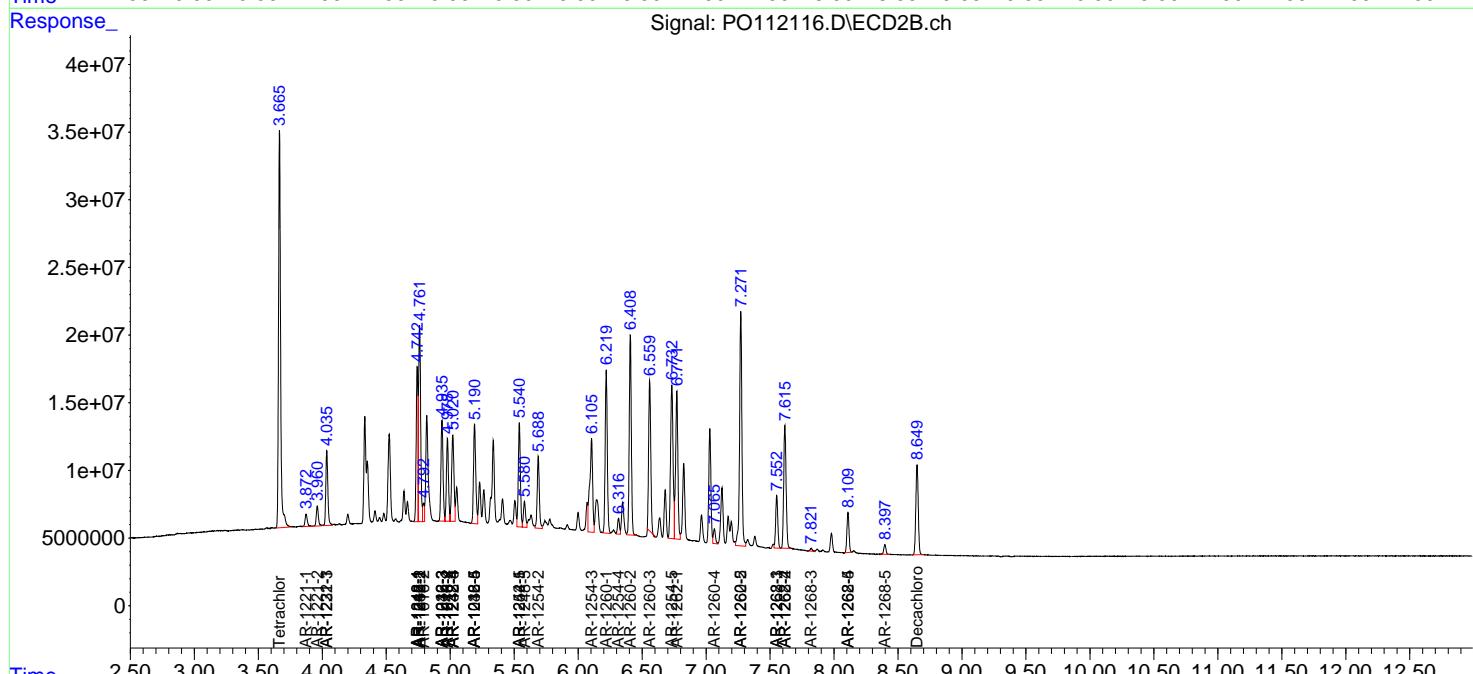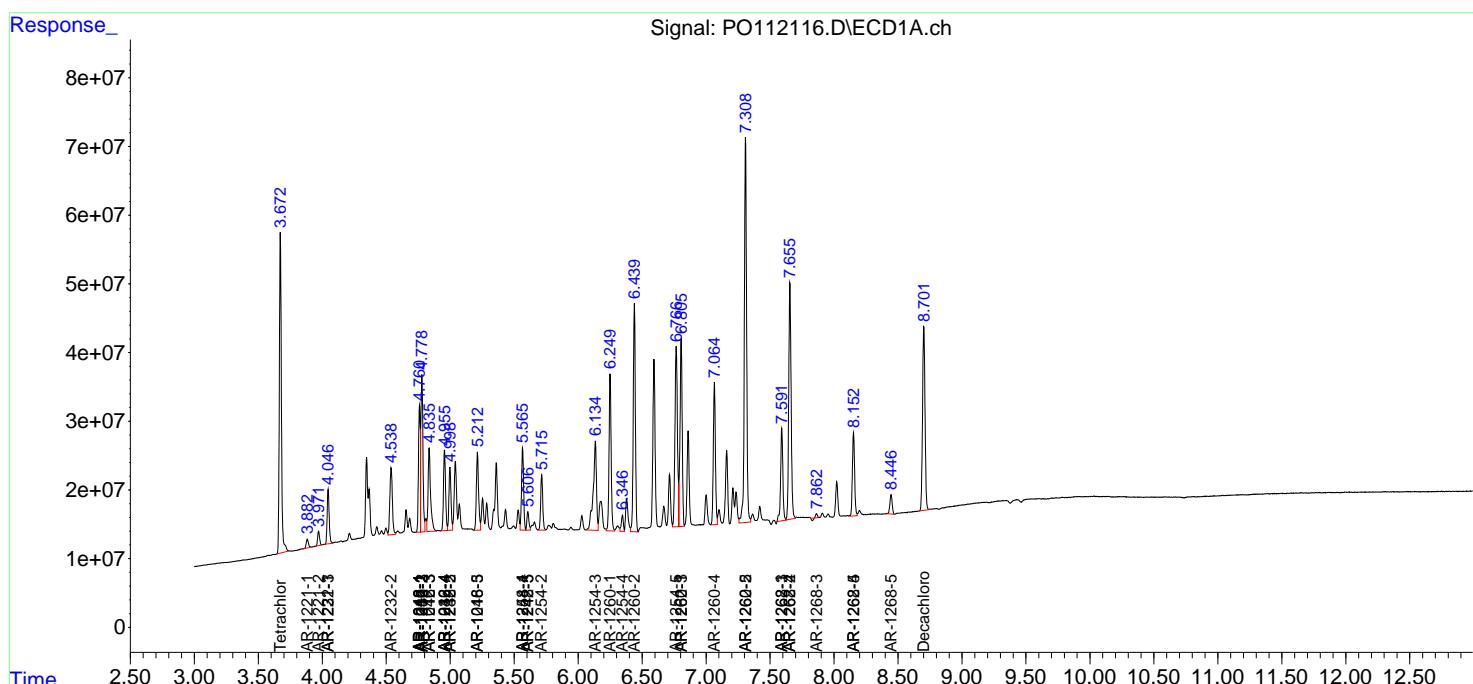

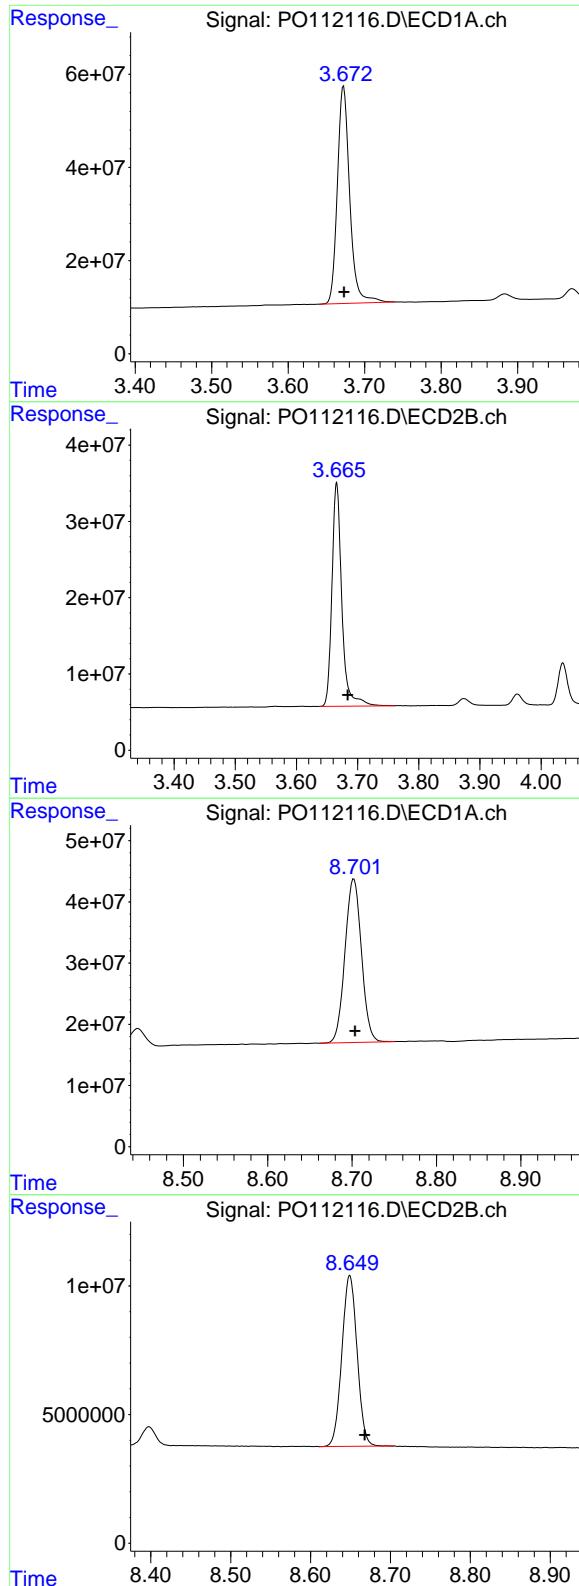

#1 Tetrachloro-m-xylene

R.T.: 3.672 min
Delta R.T.: 0.000 min
Response: 521724349
Conc: 52.73 ng/ml

Instrument:

ECD_O

ClientSampleId :

ICVPO070825

#1 Tetrachloro-m-xylene


R.T.: 3.666 min
Delta R.T.: -0.018 min
Response: 329918340
Conc: 51.78 ng/ml

#2 Decachlorobiphenyl

R.T.: 8.702 min
Delta R.T.: -0.001 min
Response: 361977757
Conc: 52.94 ng/ml

#2 Decachlorobiphenyl

R.T.: 8.649 min
Delta R.T.: -0.019 min
Response: 87909411
Conc: 51.01 ng/ml

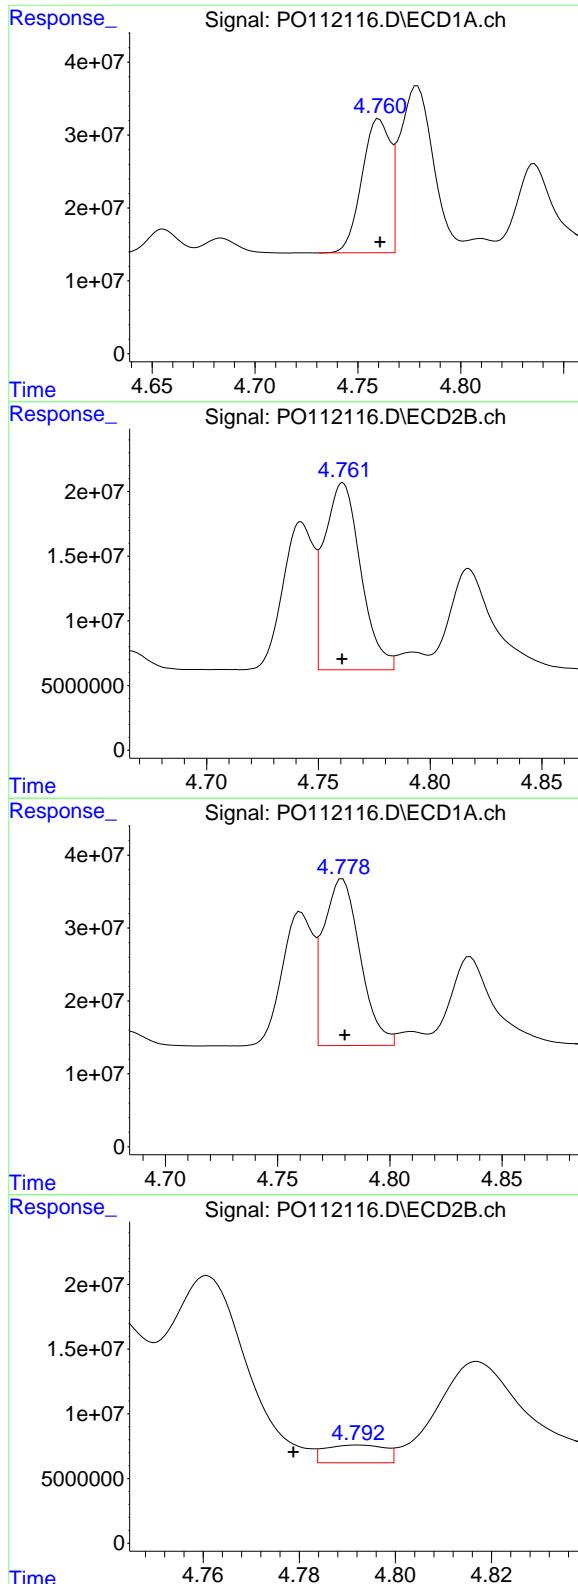

#3 AR-1016-1

R.T.: 4.760 min
 Delta R.T.: 0.000 min
 Response: 175259674
 Conc: 515.28 ng/ml

Instrument: ECD_O
 ClientSampleId: ICVPO070825

#3 AR-1016-1


R.T.: 4.761 min
 Delta R.T.: 0.000 min
 Response: 164022813
 Conc: 736.07 ng/ml

#4 AR-1016-2

R.T.: 4.779 min
 Delta R.T.: -0.001 min
 Response: 259779428
 Conc: 522.39 ng/ml

#4 AR-1016-2


R.T.: 4.792 min
 Delta R.T.: 0.013 min
 Response: 11895525
 Conc: 36.15 ng/ml

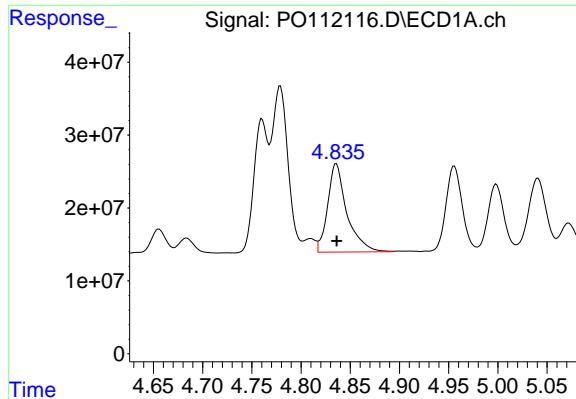

#5 AR-1016-3


R.T.: 4.836 min
 Delta R.T.: 0.000 min
 Response: 164964568
 Conc: 509.60 ng/ml

Instrument: ECD_O
 ClientSampleId: ICVPO070825

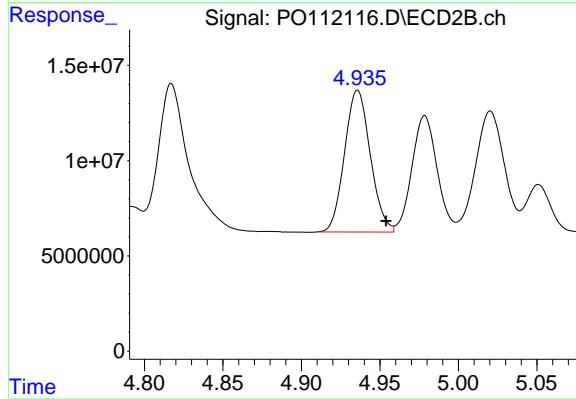


#5 AR-1016-3

R.T.: 4.936 min
 Delta R.T.: -0.018 min
 Response: 85046592
 Conc: 500.67 ng/ml

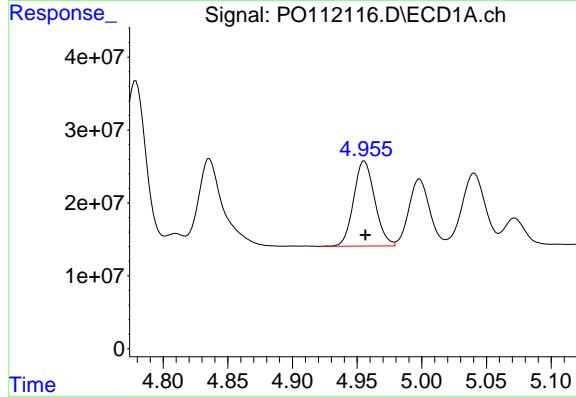


#6 AR-1016-4

R.T.: 4.956 min
 Delta R.T.: 0.000 min
 Response: 132842340
 Conc: 517.30 ng/ml

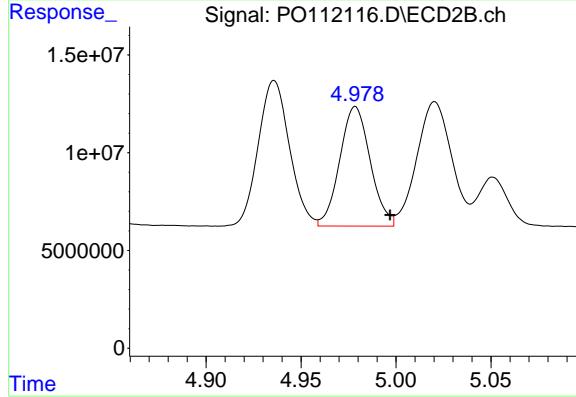


#6 AR-1016-4

R.T.: 4.979 min
 Delta R.T.: -0.018 min
 Response: 68299058
 Conc: 497.71 ng/ml

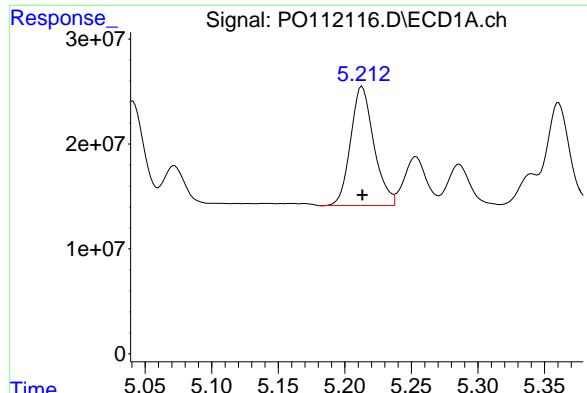


#7 AR-1016-5

R.T.: 5.213 min
 Delta R.T.: 0.000 min **Instrument:**
 Response: 137838808 ECD_O
 Conc: 503.68 ng/ml **ClientSampleId:**
 ICPPO070825

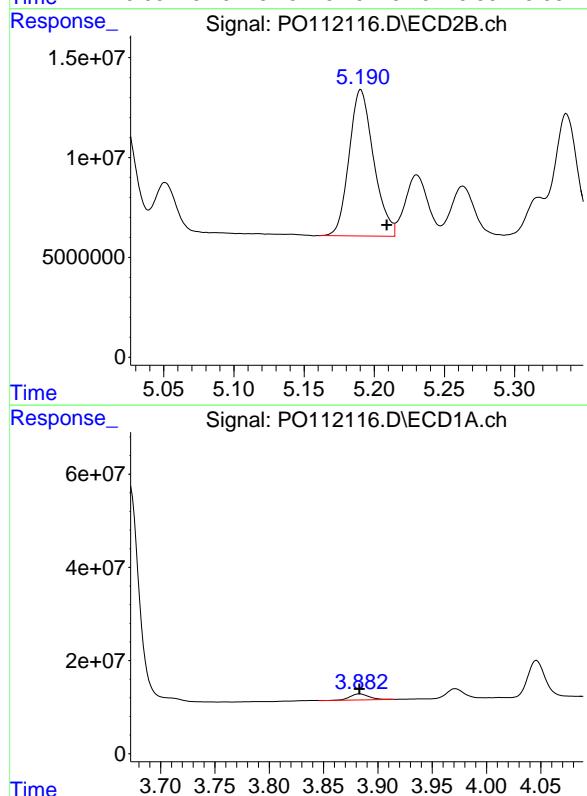


#8 AR-1221-1

R.T.: 3.883 min
 Delta R.T.: 0.000 min
 Response: 15947935
 Conc: 136.76 ng/ml

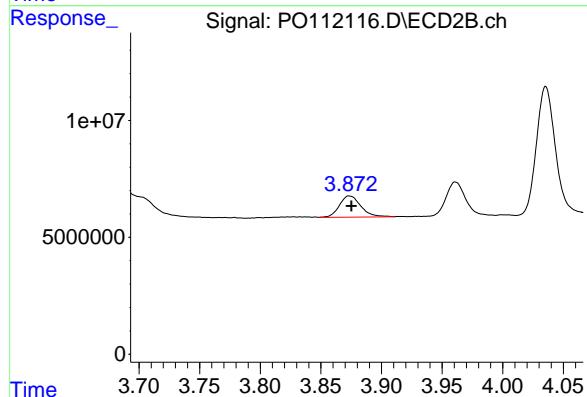

#8 AR-1221-1

R.T.: 3.873 min
 Delta R.T.: -0.002 min
 Response: 11246969
 Conc: 136.67 ng/ml

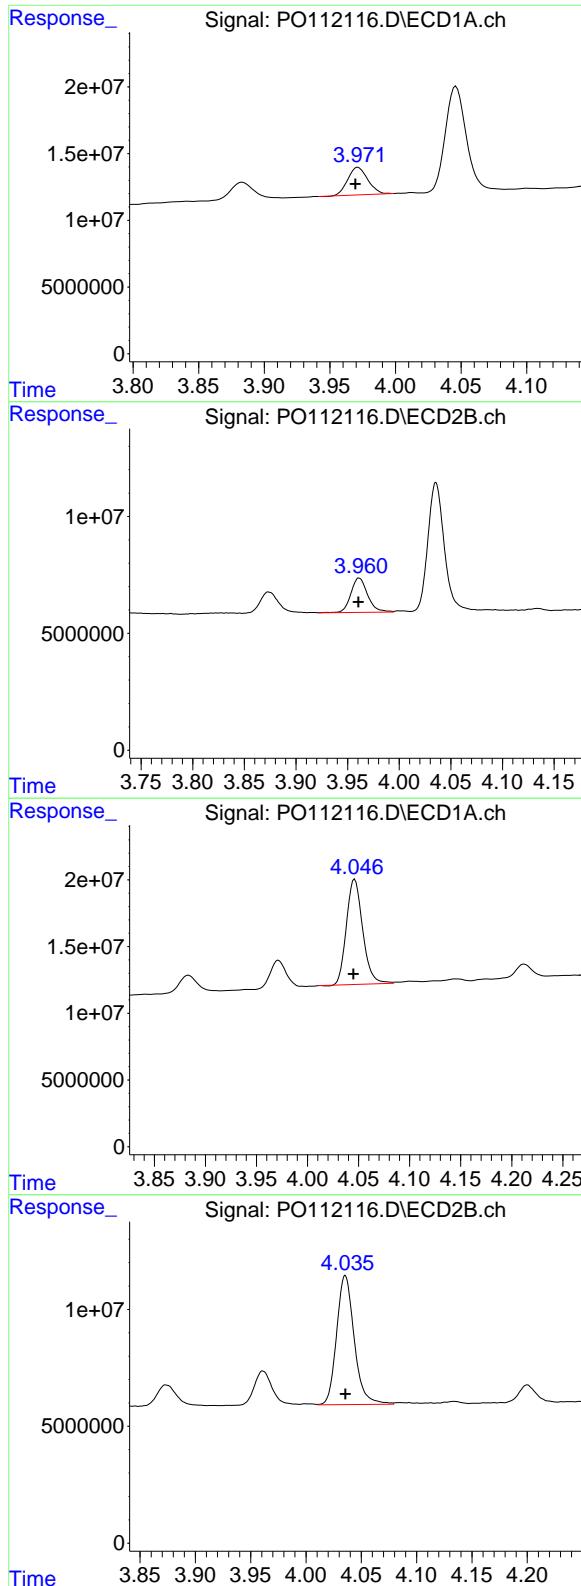

#9 AR-1221-2

R.T.: 3.971 min
 Delta R.T.: 0.002 min
 Response: 21794231
 Conc: 276.43 ng/ml

Instrument: ECD_O
 ClientSampleId: ICPVPO070825

#9 AR-1221-2


R.T.: 3.961 min
 Delta R.T.: 0.000 min
 Response: 16662019
 Conc: 280.72 ng/ml

#10 AR-1221-3

R.T.: 4.046 min
 Delta R.T.: 0.001 min
 Response: 87428058
 Conc: 324.31 ng/ml

#10 AR-1221-3

R.T.: 4.036 min
 Delta R.T.: 0.000 min
 Response: 61302785
 Conc: 324.74 ng/ml

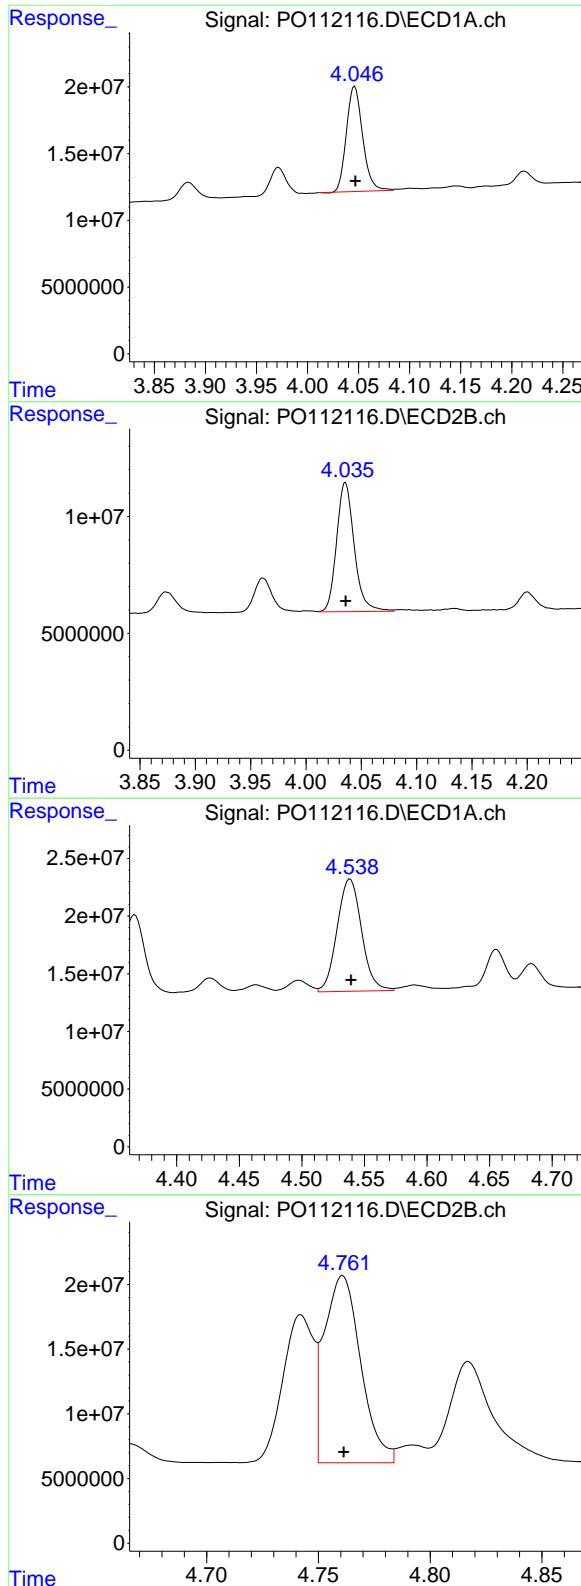

#11 AR-1232-1

R.T.: 4.046 min
 Delta R.T.: 0.000 min
 Response: 87428058
 Conc: 407.27 ng/ml

Instrument: ECD_O
 ClientSampleId: ICVPO070825

#11 AR-1232-1


R.T.: 4.036 min
 Delta R.T.: 0.000 min
 Response: 61302785
 Conc: 408.41 ng/ml

#12 AR-1232-2

R.T.: 4.539 min
 Delta R.T.: 0.000 min
 Response: 132612101
 Conc: 1166.98 ng/ml

#12 AR-1232-2

R.T.: 4.761 min
 Delta R.T.: 0.000 min
 Response: 164022813
 Conc: 1071.44 ng/ml

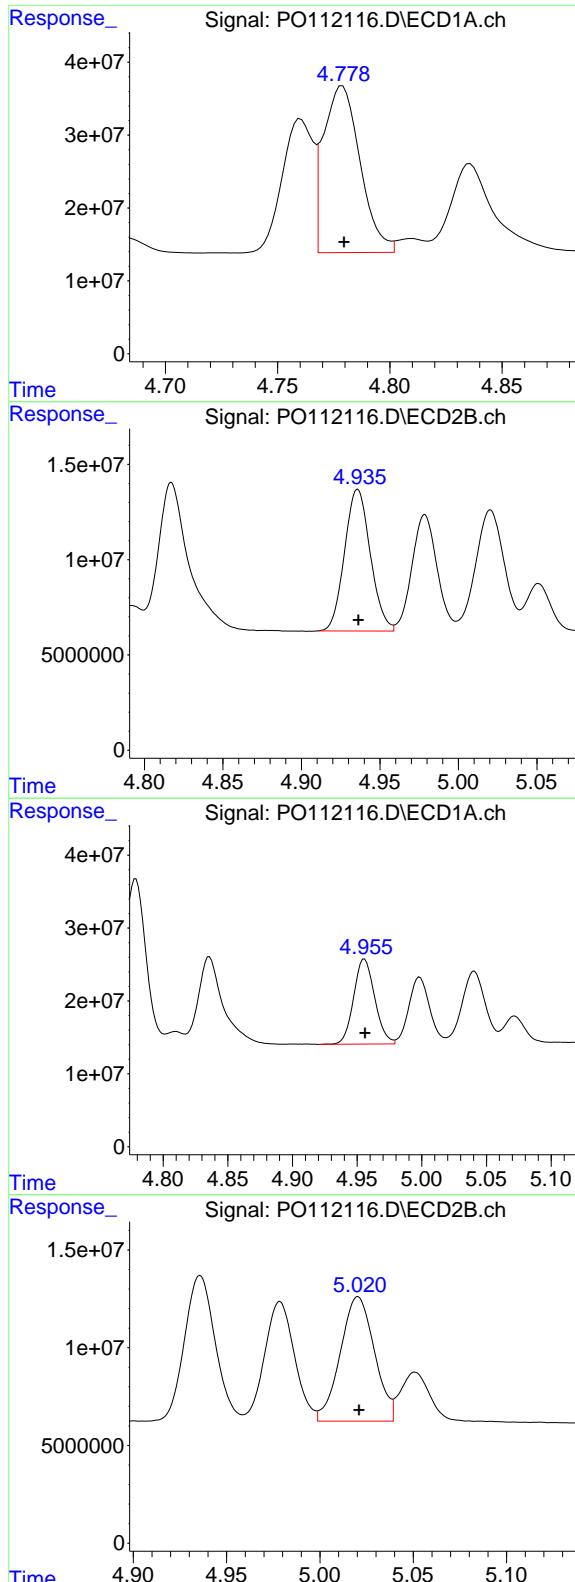

#13 AR-1232-3

R.T.: 4.779 min
 Delta R.T.: 0.000 min
 Response: 259779428
 Conc: 1134.36 ng/ml

Instrument: ECD_O
ClientSampleId: ICVPO070825

#13 AR-1232-3


R.T.: 4.936 min
 Delta R.T.: 0.000 min
 Response: 85046592
 Conc: 1126.35 ng/ml

#14 AR-1232-4

R.T.: 4.956 min
 Delta R.T.: 0.000 min
 Response: 132842340
 Conc: 1162.26 ng/ml

#14 AR-1232-4


R.T.: 5.020 min
 Delta R.T.: 0.000 min
 Response: 81017586
 Conc: 1227.76 ng/ml

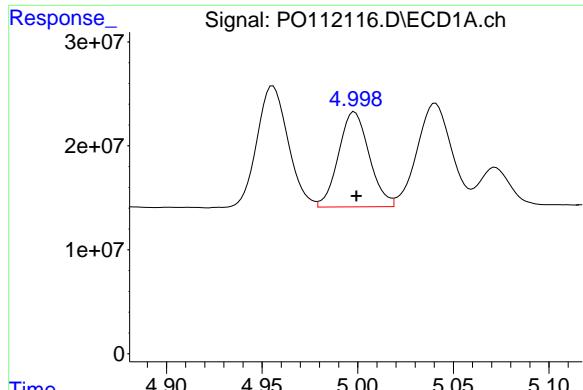

#15 AR-1232-5


R.T.: 4.998 min
 Delta R.T.: -0.001 min
 Response: 102318301
 Conc: 1393.98 ng/ml

Instrument: ECD_O
 ClientSampleId: ICVPO070825

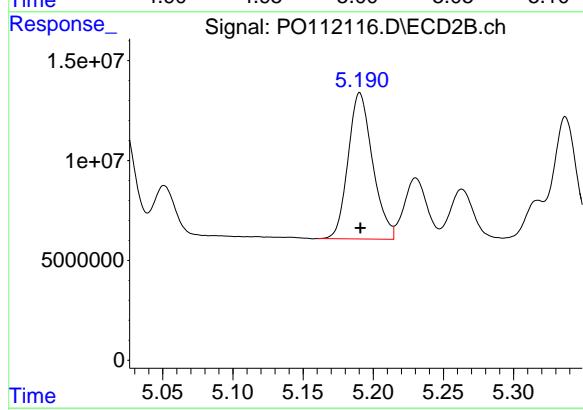


#15 AR-1232-5

R.T.: 5.190 min
 Delta R.T.: 0.000 min
 Response: 89116759
 Conc: 1200.07 ng/ml

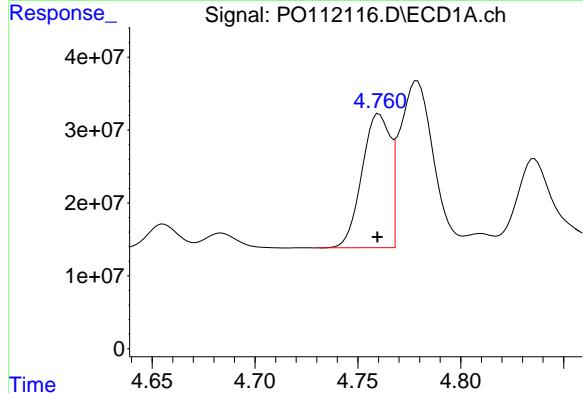


#16 AR-1242-1

R.T.: 4.760 min
 Delta R.T.: 0.000 min
 Response: 175259674
 Conc: 605.10 ng/ml

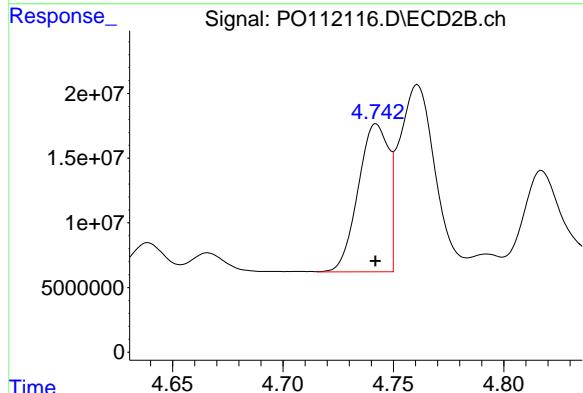

#16 AR-1242-1

R.T.: 4.742 min
 Delta R.T.: 0.000 min
 Response: 109861140
 Conc: 566.71 ng/ml

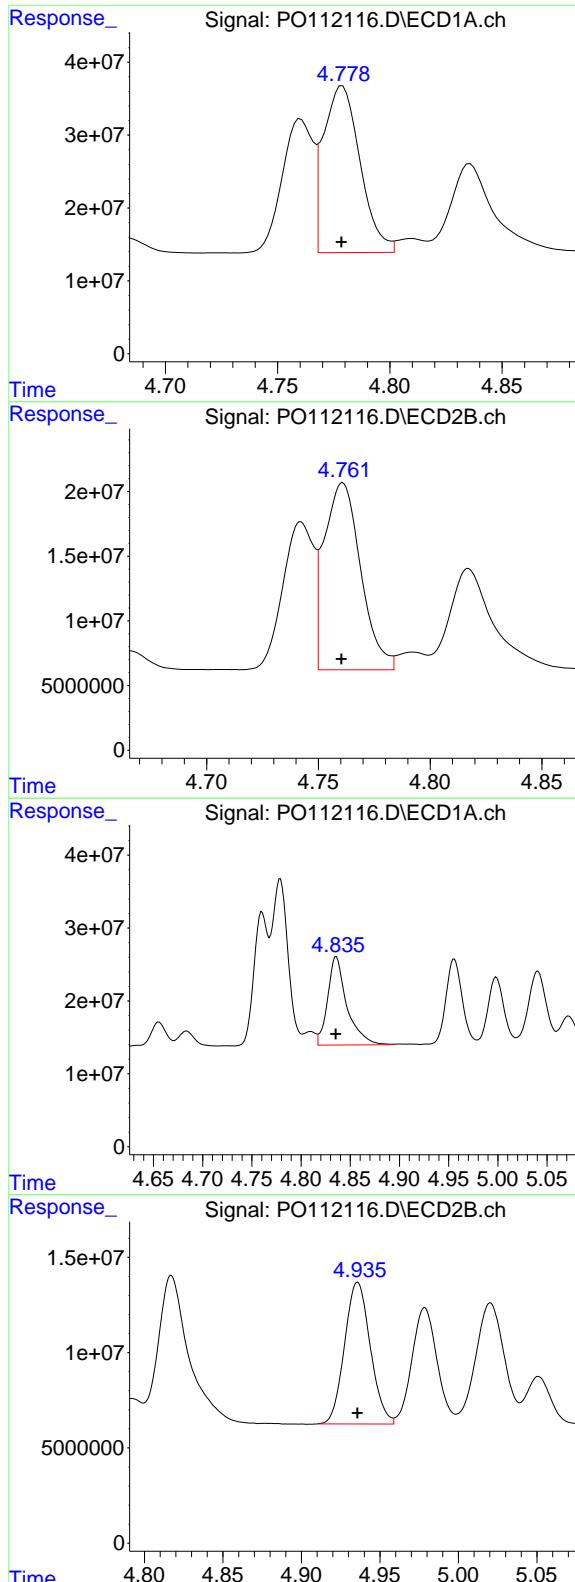

#17 AR-1242-2

R.T.: 4.779 min
 Delta R.T.: 0.000 min
Instrument:
 Response: 259779428 ECD_O
 Conc: 609.93 ng/ml ClientSampleId :
 ICVPO070825

#17 AR-1242-2


R.T.: 4.761 min
 Delta R.T.: 0.000 min
 Response: 164022813
 Conc: 578.87 ng/ml

#18 AR-1242-3

R.T.: 4.836 min
 Delta R.T.: 0.000 min
 Response: 164964568
 Conc: 602.75 ng/ml

#18 AR-1242-3

R.T.: 4.936 min
 Delta R.T.: 0.000 min
 Response: 85046592
 Conc: 583.80 ng/ml

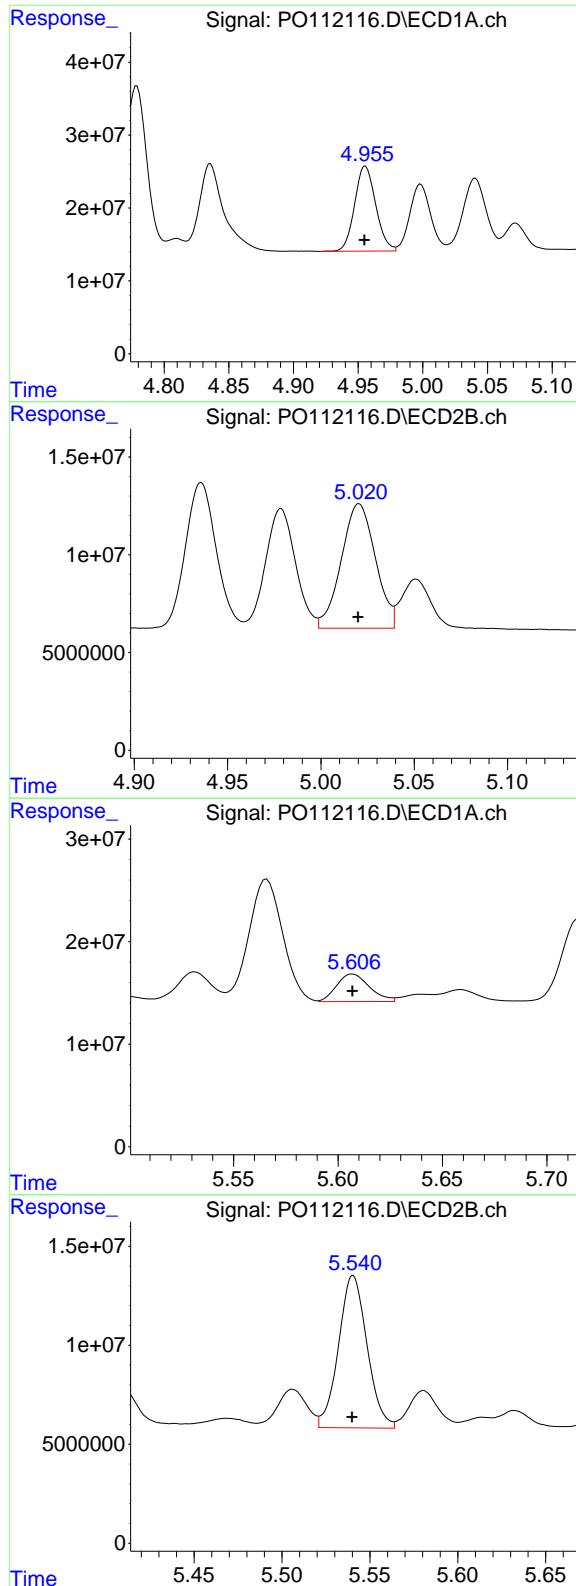

#19 AR-1242-4

R.T.: 4.956 min
 Delta R.T.: 0.000 min
 Response: 132842340
 Conc: 589.58 ng/ml

Instrument: ECD_O
 ClientSampleId: ICVPO070825

#19 AR-1242-4


R.T.: 5.020 min
 Delta R.T.: 0.000 min
 Response: 81017586
 Conc: 571.19 ng/ml

#20 AR-1242-5

R.T.: 5.607 min
 Delta R.T.: 0.000 min
 Response: 29284624
 Conc: 138.35 ng/ml

#20 AR-1242-5


R.T.: 5.540 min
 Delta R.T.: 0.000 min
 Response: 86955161
 Conc: 478.47 ng/ml

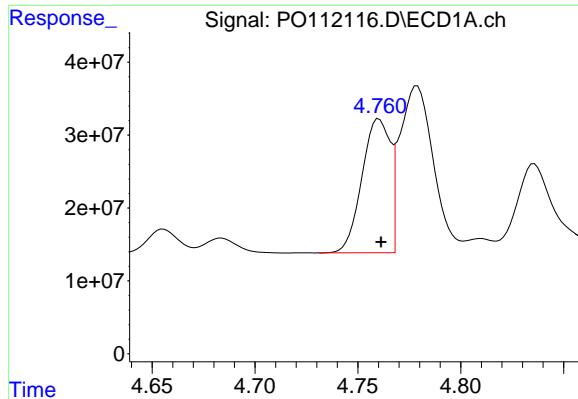

#21 AR-1248-1


R.T.: 4.760 min
 Delta R.T.: 0.000 min
 Response: 175259674
 Conc: 772.41 ng/ml

Instrument: ECD_O
 ClientSampleId: ICVPO070825

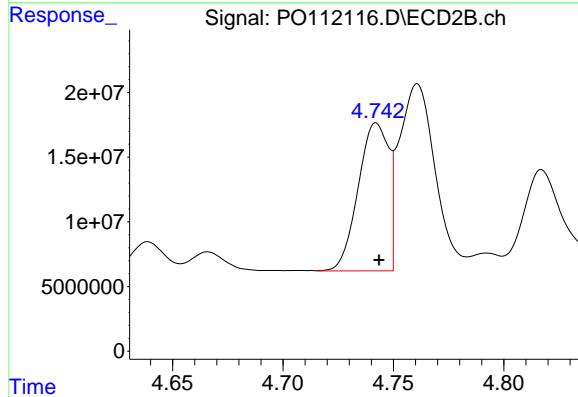


#21 AR-1248-1

R.T.: 4.742 min
 Delta R.T.: -0.001 min
 Response: 109861140
 Conc: 711.68 ng/ml

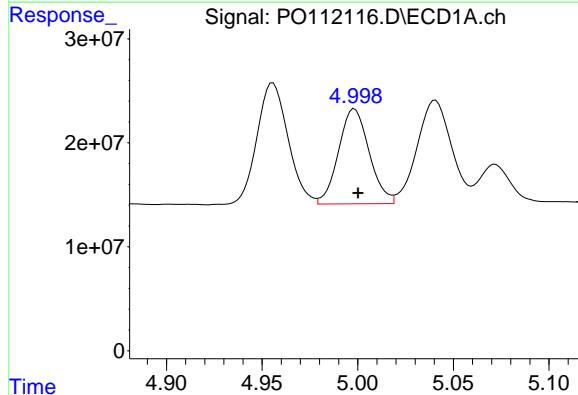


#22 AR-1248-2

R.T.: 4.998 min
 Delta R.T.: -0.002 min
 Response: 102318301
 Conc: 331.85 ng/ml

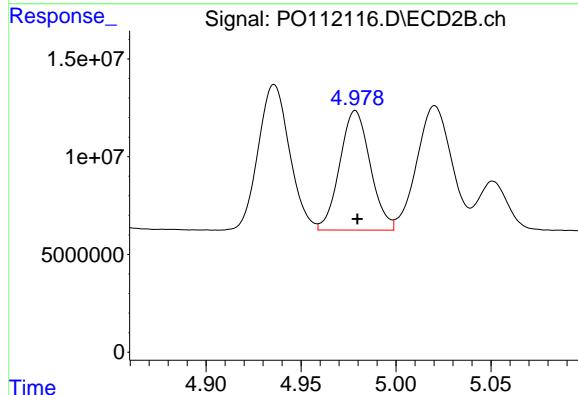

#22 AR-1248-2

R.T.: 4.979 min
 Delta R.T.: -0.001 min
 Response: 68299058
 Conc: 331.92 ng/ml

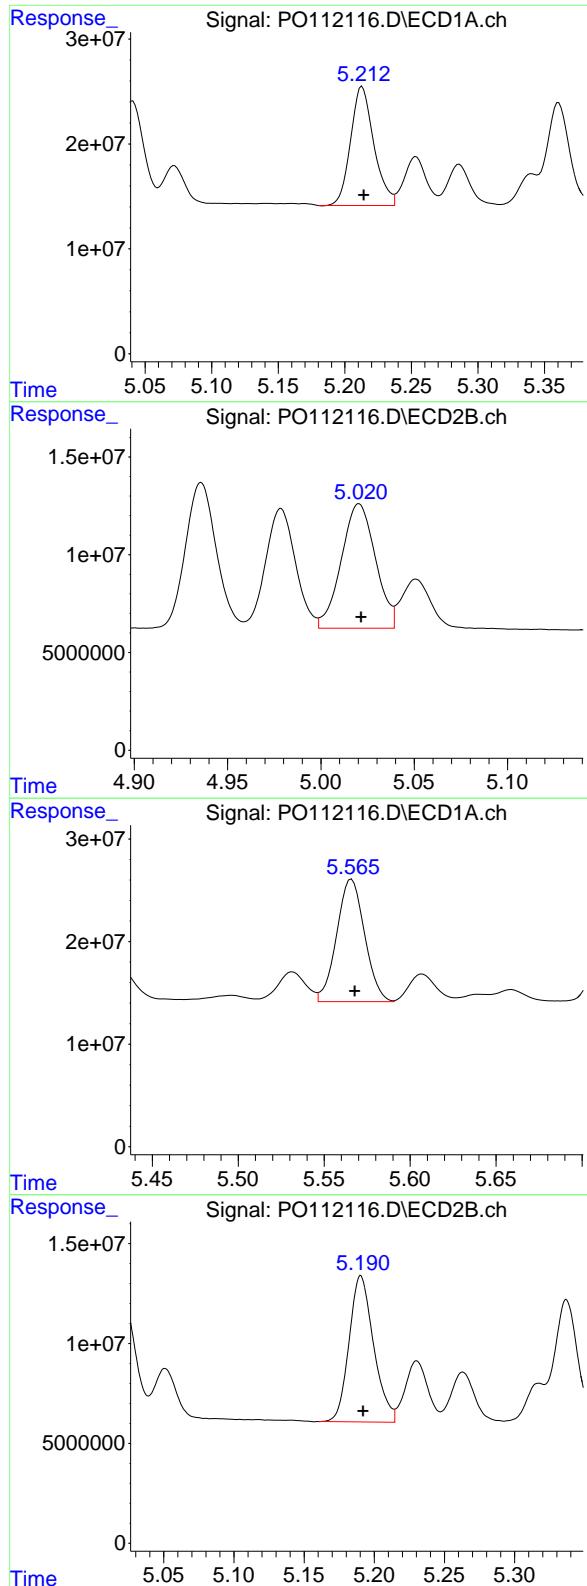

#23 AR-1248-3

R.T.: 5.213 min
 Delta R.T.: -0.001 min
 Response: 137838808
 Conc: 338.40 ng/ml

Instrument: ECD_O
 ClientSampleId: ICVPO070825

#23 AR-1248-3


R.T.: 5.020 min
 Delta R.T.: -0.001 min
 Response: 81017586
 Conc: 377.18 ng/ml

#24 AR-1248-4

R.T.: 5.566 min
 Delta R.T.: -0.002 min
 Response: 134962836
 Conc: 233.84 ng/ml

#24 AR-1248-4

R.T.: 5.190 min
 Delta R.T.: -0.002 min
 Response: 89116759
 Conc: 344.44 ng/ml

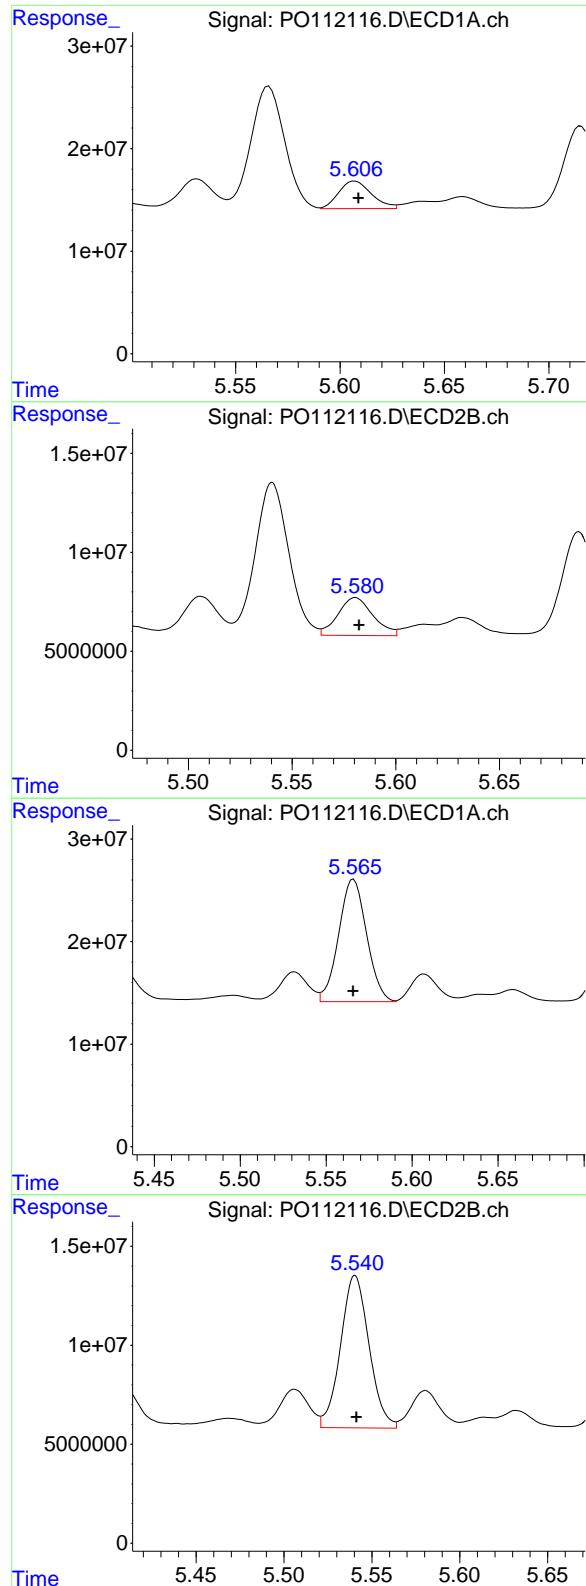

#25 AR-1248-5

R.T.: 5.607 min
 Delta R.T.: -0.002 min
 Response: 29284624
 Conc: 75.03 ng/ml

Instrument: ECD_O
 ClientSampleId: ICVPO070825

#25 AR-1248-5


R.T.: 5.581 min
 Delta R.T.: -0.002 min
 Response: 22496977
 Conc: 89.79 ng/ml

#26 AR-1254-1

R.T.: 5.566 min
 Delta R.T.: 0.000 min
 Response: 134962836
 Conc: 219.41 ng/ml

#26 AR-1254-1

R.T.: 5.540 min
 Delta R.T.: 0.000 min
 Response: 86955161
 Conc: 228.13 ng/ml

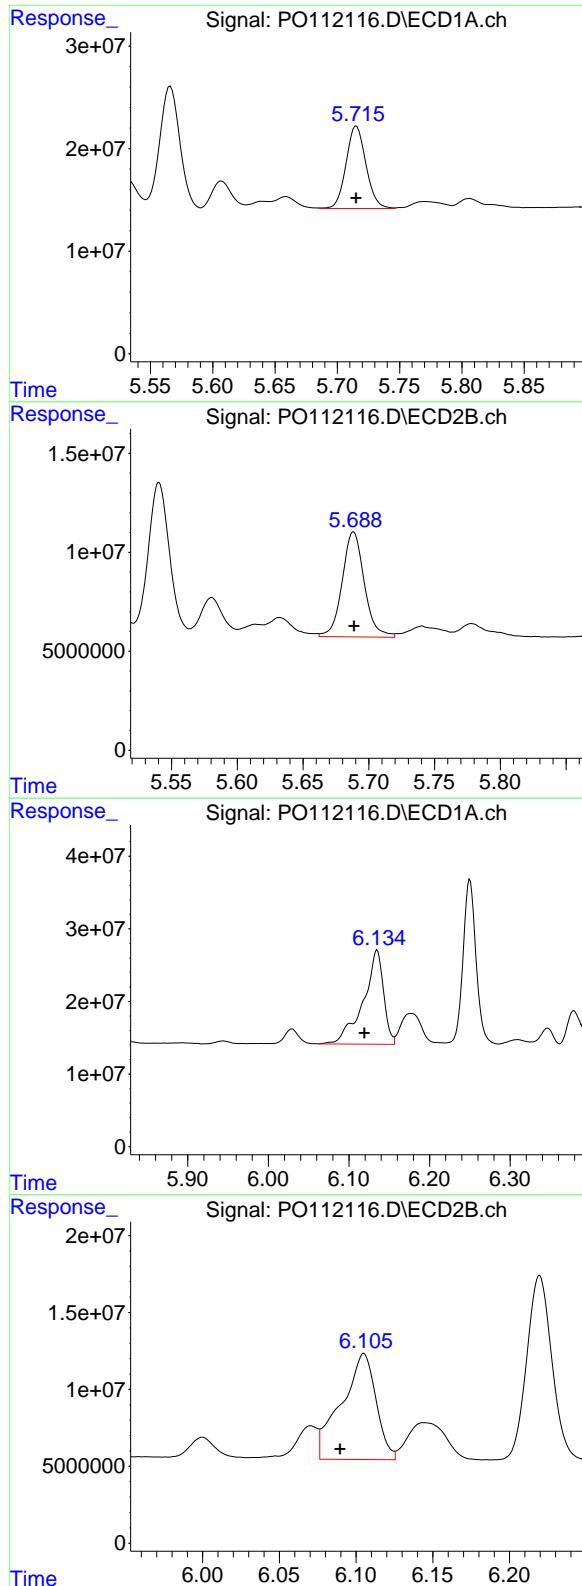

#27 AR-1254-2

R.T.: 5.715 min
 Delta R.T.: 0.000 min
 Response: 90019733
 Conc: 168.05 ng/ml

Instrument: ECD_O
 ClientSampleId: ICVPO070825

#27 AR-1254-2


R.T.: 5.688 min
 Delta R.T.: 0.000 min
 Response: 62065631
 Conc: 187.05 ng/ml

#28 AR-1254-3

R.T.: 6.135 min
 Delta R.T.: 0.016 min
 Response: 227652491
 Conc: 271.15 ng/ml

#28 AR-1254-3

R.T.: 6.105 min
 Delta R.T.: 0.015 min
 Response: 108679730
 Conc: 225.46 ng/ml

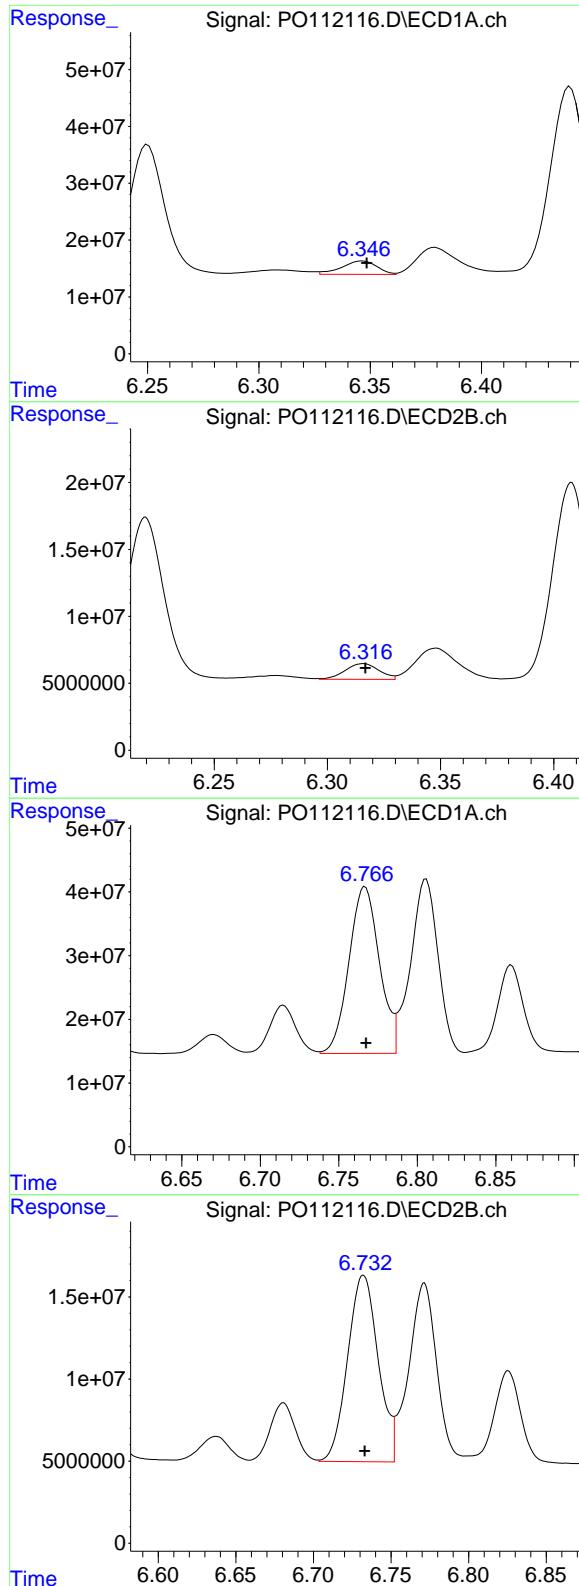

#29 AR-1254-4

R.T.: 6.347 min
 Delta R.T.: -0.002 min
 Response: 25832693
 Conc: 53.70 ng/ml

Instrument: ECD_O
ClientSampleId: ICVPO070825

#29 AR-1254-4


R.T.: 6.316 min
 Delta R.T.: 0.000 min
 Response: 12233696
 Conc: 46.93 ng/ml

#30 AR-1254-5

R.T.: 6.767 min
 Delta R.T.: 0.000 min
 Response: 353687794
 Conc: 456.99 ng/ml

#30 AR-1254-5

R.T.: 6.732 min
 Delta R.T.: 0.000 min
 Response: 156029824
 Conc: 437.85 ng/ml

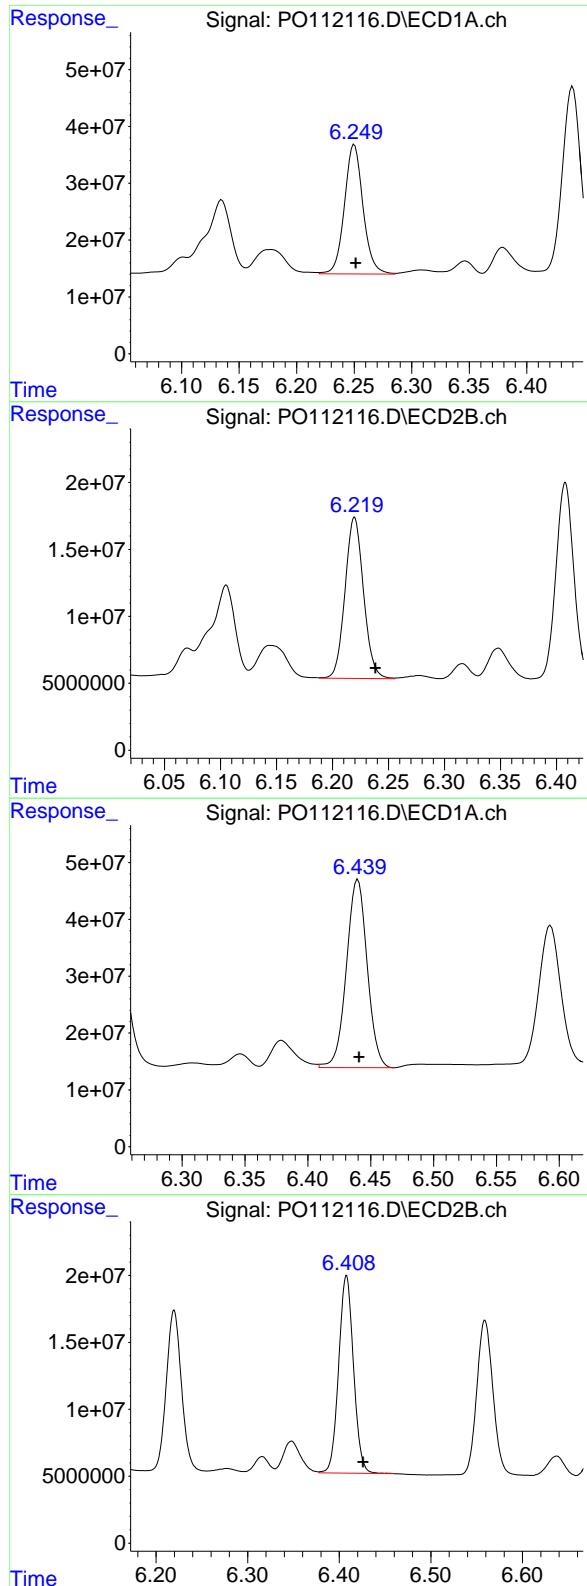

#31 AR-1260-1

R.T.: 6.250 min
 Delta R.T.: -0.001 min
 Response: 257100150
 Conc: 512.93 ng/ml

Instrument: ECD_O
 ClientSampleId: ICVPO070825

#31 AR-1260-1


R.T.: 6.220 min
 Delta R.T.: -0.019 min
 Response: 138564703
 Conc: 493.88 ng/ml

#32 AR-1260-2

R.T.: 6.440 min
 Delta R.T.: -0.001 min
 Response: 380263019
 Conc: 515.17 ng/ml

#32 AR-1260-2

R.T.: 6.408 min
 Delta R.T.: -0.018 min
 Response: 165872316
 Conc: 487.86 ng/ml

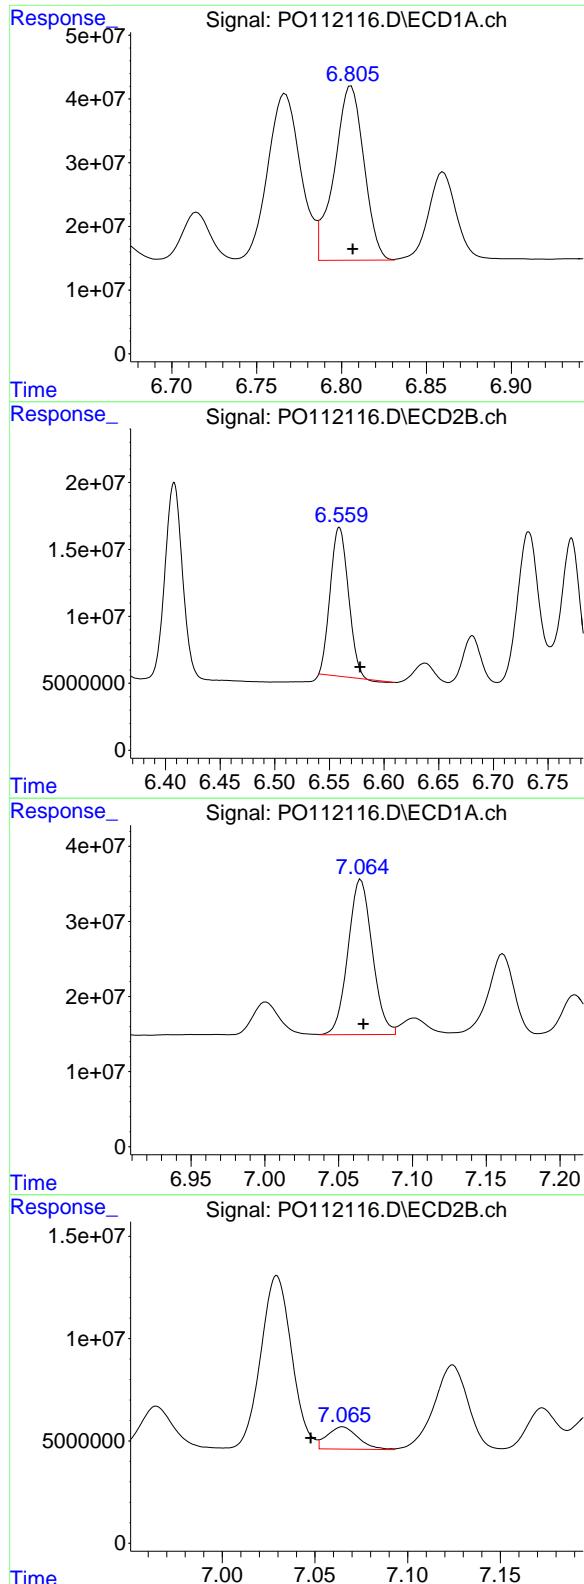

#33 AR-1260-3

R.T.: 6.806 min
 Delta R.T.: -0.001 min
 Response: 331746197
 Conc: 506.11 ng/ml

Instrument: ECD_O
 ClientSampleId: ICVPO070825

#33 AR-1260-3


R.T.: 6.559 min
 Delta R.T.: -0.019 min
 Response: 128088840
 Conc: 464.79 ng/ml

#34 AR-1260-4

R.T.: 7.065 min
 Delta R.T.: -0.002 min
 Response: 235897061
 Conc: 541.98 ng/ml

#34 AR-1260-4

R.T.: 7.065 min
 Delta R.T.: 0.017 min
 Response: 12589968
 Conc: 62.75 ng/ml

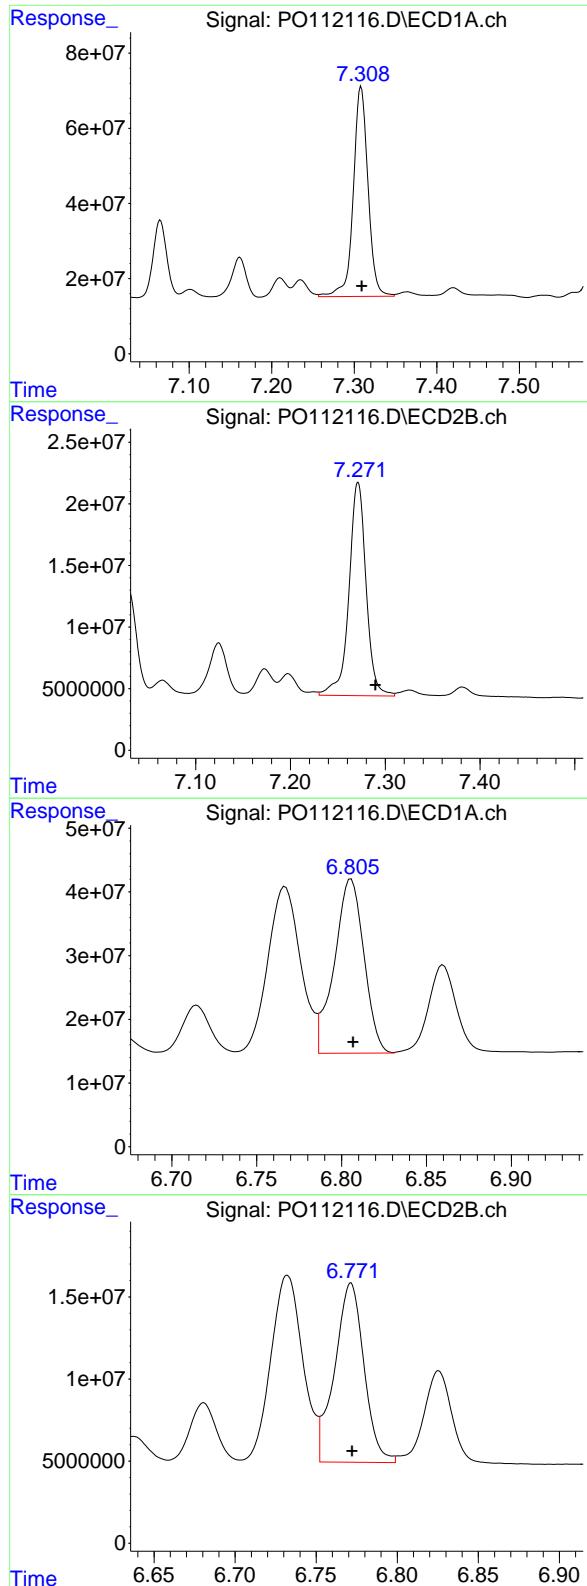

#35 AR-1260-5

R.T.: 7.308 min
 Delta R.T.: 0.000 min
 Response: 694127135
 Conc: 549.79 ng/ml

Instrument: ECD_O
 ClientSampleId: ICVPO070825

#35 AR-1260-5


R.T.: 7.271 min
 Delta R.T.: -0.018 min
 Response: 218449847
 Conc: 487.91 ng/ml

#36 AR-1262-1

R.T.: 6.806 min
 Delta R.T.: -0.001 min
 Response: 331746197
 Conc: 324.70 ng/ml

#36 AR-1262-1

R.T.: 6.771 min
 Delta R.T.: 0.000 min
 Response: 137493855
 Conc: 337.56 ng/ml

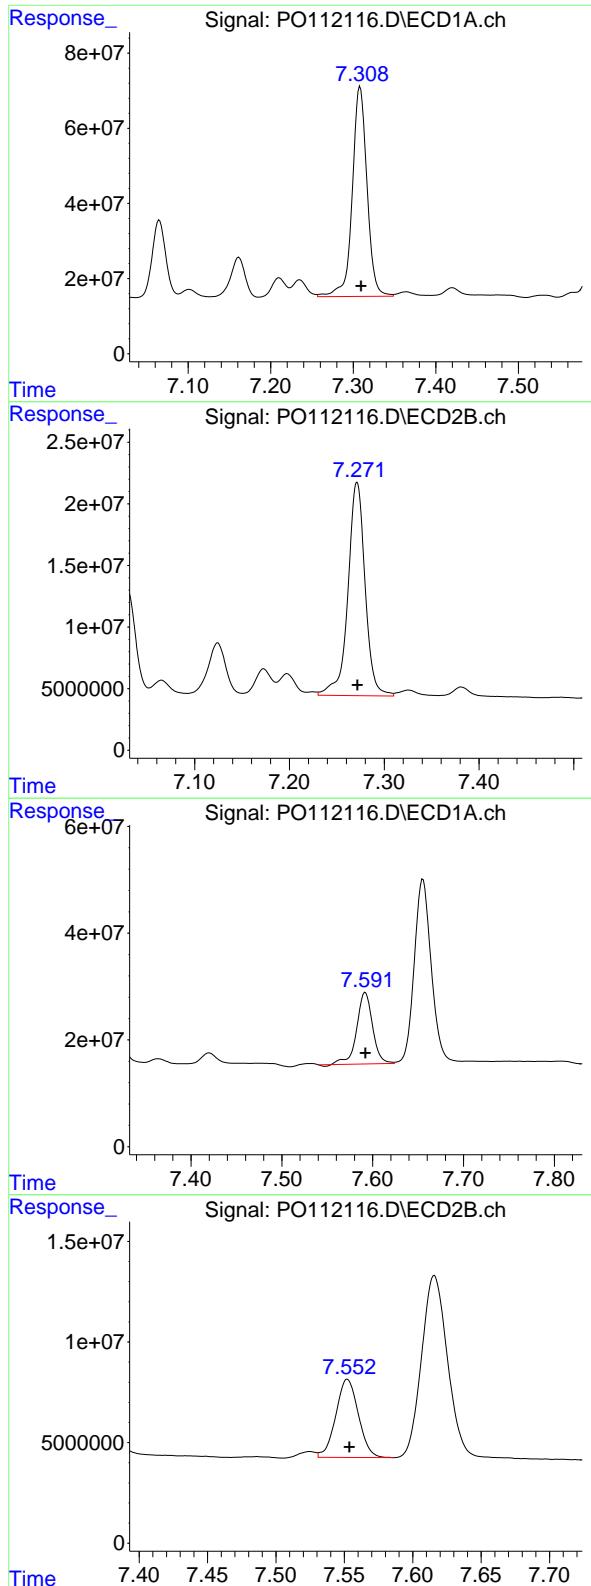

#37 AR-1262-2

R.T.: 7.308 min
Delta R.T.: -0.001 min **Instrument:**
Response: 694127135 ECD_O
Conc: 423.41 ng/ml **ClientSampleId:**
ICVPO070825

#37 AR-1262-2


R.T.: 7.271 min
Delta R.T.: 0.000 min
Response: 218449847
Conc: 426.20 ng/ml

#38 AR-1262-3

R.T.: 7.592 min
Delta R.T.: 0.000 min
Response: 161799024
Conc: 252.03 ng/ml

#38 AR-1262-3

R.T.: 7.552 min
Delta R.T.: -0.002 min
Response: 44636216
Conc: 248.64 ng/ml

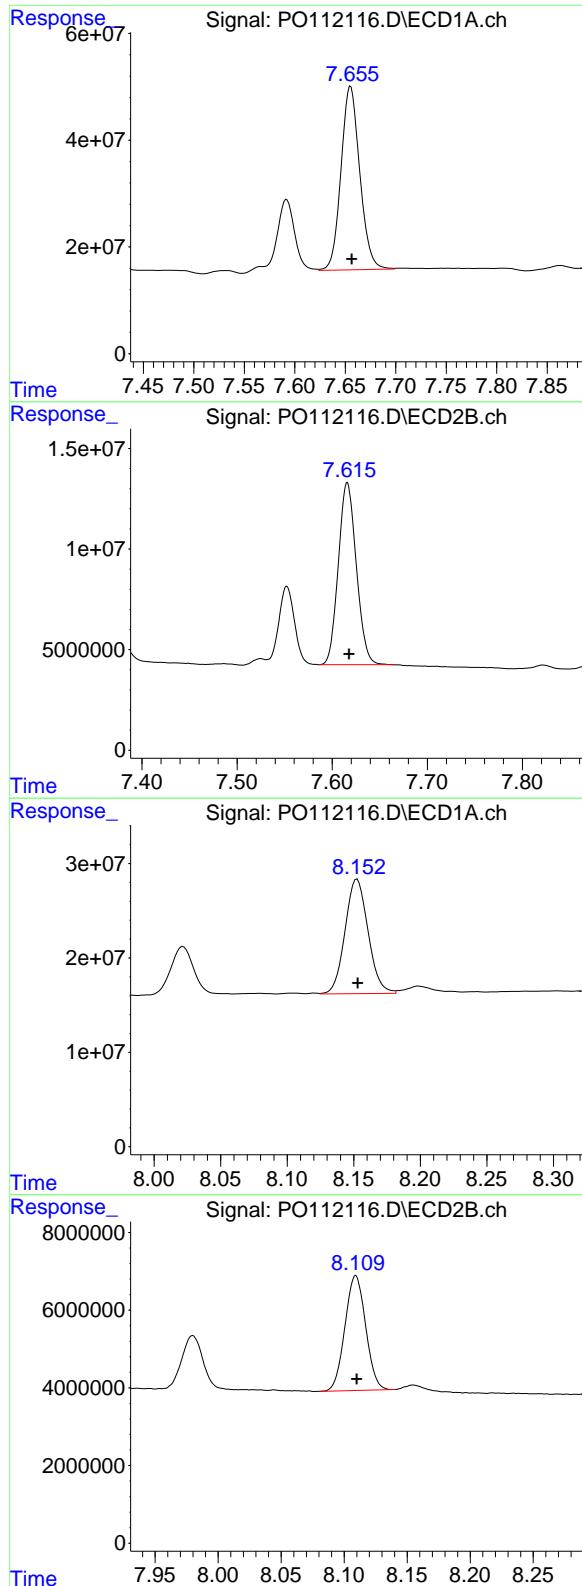

#39 AR-1262-4

R.T.: 7.655 min
 Delta R.T.: -0.001 min
 Response: 445610398
 Conc: 415.90 ng/ml

Instrument: ECD_O
 ClientSampleId: ICVPO070825

#39 AR-1262-4


R.T.: 7.616 min
 Delta R.T.: -0.002 min
 Response: 119162908
 Conc: 409.61 ng/ml

#40 AR-1262-5

R.T.: 8.153 min
 Delta R.T.: 0.000 min
 Response: 146085704
 Conc: 325.98 ng/ml

#40 AR-1262-5

R.T.: 8.109 min
 Delta R.T.: 0.000 min
 Response: 33885824
 Conc: 320.33 ng/ml

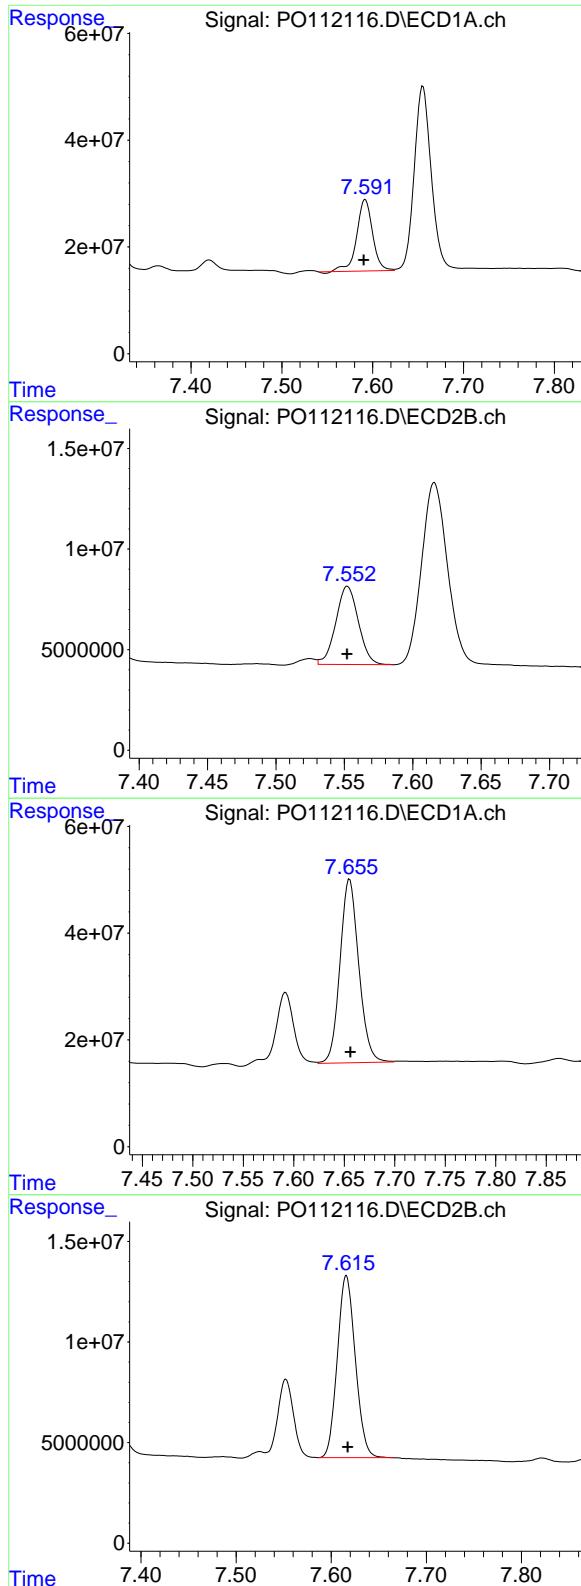

#41 AR-1268-1

R.T.: 7.592 min
 Delta R.T.: 0.002 min
 Response: 161799024
 Conc: 88.06 ng/ml

Instrument: ECD_O
 ClientSampleId: ICVPO070825

#41 AR-1268-1


R.T.: 7.552 min
 Delta R.T.: 0.000 min
 Response: 44636216
 Conc: 90.82 ng/ml

#42 AR-1268-2

R.T.: 7.655 min
 Delta R.T.: 0.000 min
 Response: 445610398
 Conc: 286.09 ng/ml

#42 AR-1268-2

R.T.: 7.616 min
 Delta R.T.: -0.002 min
 Response: 119162908
 Conc: 285.63 ng/ml

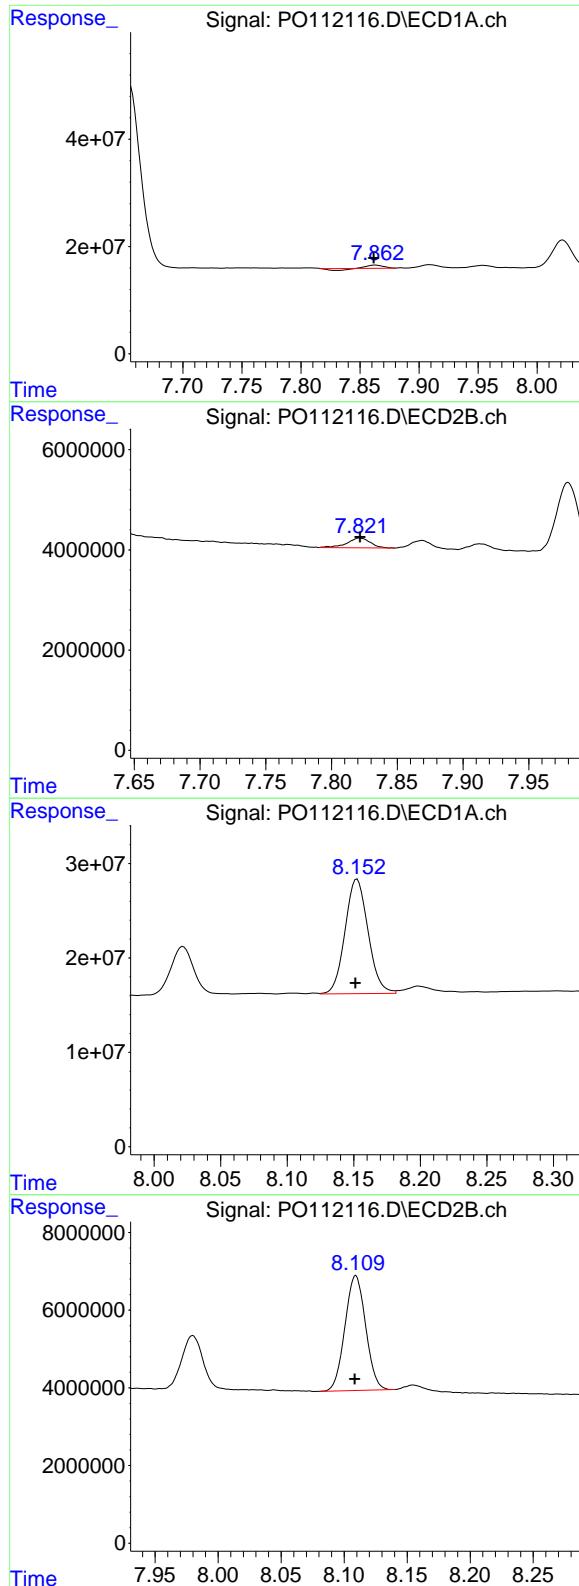

#43 AR-1268-3

R.T.: 7.863 min
 Delta R.T.: 0.001 min **Instrument:**
 Response: 2769823 ECD_O
 Conc: 2.13 ng/ml **ClientSampleId:**
 ICVPO070825

#43 AR-1268-3


R.T.: 7.821 min
 Delta R.T.: 0.000 min
 Response: 2396044
 Conc: 7.57 ng/ml

#44 AR-1268-4

R.T.: 8.153 min
 Delta R.T.: 0.001 min
 Response: 146085704
 Conc: 304.09 ng/ml

#44 AR-1268-4

R.T.: 8.109 min
 Delta R.T.: 0.000 min
 Response: 33885824
 Conc: 303.88 ng/ml

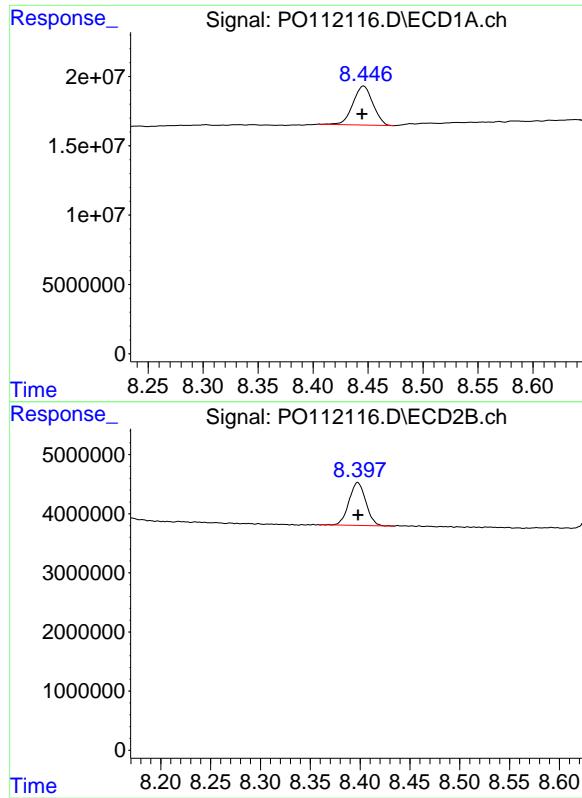

#45 AR-1268-5

R.T.: 8.446 min
Delta R.T.: 0.002 min
Response: 35455171
Conc: 10.86 ng/ml

Instrument: ECD_O
ClientSampleId: ICVPO070825

#45 AR-1268-5

R.T.: 8.398 min
Delta R.T.: 0.000 min
Response: 8565740
Conc: 11.79 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0072125\
 Data File : P0112332.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jul 2025 10:15
 Operator : YP/AJ
 Sample : AR1660CCC500
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1660CCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 22 01:44:41 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Jul 21 10:54:00 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	3.670	3.663	592.8E6	349.3E6	59.914	54.828
2) SA Decachlor...	8.699	8.645	322.9E6	76065272	47.232	44.135

Target Compounds

3) L1 AR-1016-1	4.757	4.739	189.6E6	110.1E6	557.415	494.291
4) L1 AR-1016-2	4.776	4.757	277.9E6	150.6E6	558.822	457.715
5) L1 AR-1016-3	4.833	4.975	174.9E6	70204245	540.411	413.290
6) L1 AR-1016-4	4.953	5.017	143.2E6	83633519	557.827	609.452
7) L1 AR-1016-5	5.210	5.187	146.7E6	90853568	536.029	526.839
8) L2 AR-1221-1	3.881	3.871	18912211	12291205	162.178	149.355
9) L2 AR-1221-2	3.969	3.958	25420609	17491866	322.431	294.706
10) L2 AR-1221-3	4.044	4.032	98680542	65225339	366.051	345.516
11) L3 AR-1232-1	4.044	4.032	98680542	65225339	459.690	434.548
12) L3 AR-1232-2	4.536	4.757	141.5E6	150.6E6	1245.600	983.978
13) L3 AR-1232-3	4.776	4.932	277.9E6	86189982	1213.480	1141.498
14) L3 AR-1232-4	4.953	5.017	143.2E6	83633519	1253.314	1267.401
15) L3 AR-1232-5	4.996	5.187	111.4E6	90853568	1518.361	1223.454
16) L4 AR-1242-1	4.757	4.739	189.6E6	110.1E6	654.577	568.172
17) L4 AR-1242-2	4.776	4.757	277.9E6	150.6E6	652.465	531.610
18) L4 AR-1242-3	4.833	4.932	174.9E6	86189982	639.196	591.650
19) L4 AR-1242-4	4.953	5.017	143.2E6	83633519	635.766	589.630
20) L4 AR-1242-5	5.605	5.537	37881289	89535680	178.963	492.674 #
21) L5 AR-1248-1	4.757	4.739	189.6E6	110.1E6	835.566	713.521
22) L5 AR-1248-2	4.996	4.975	111.4E6	70204245	361.463	341.182
23) L5 AR-1248-3	5.210	5.017	146.7E6	83633519	360.137	389.358
24) L5 AR-1248-4	5.563	5.187	151.4E6	90853568	262.377	351.156 #
25) L5 AR-1248-5	5.605	5.578	37881289	24255105	97.056	96.808
26) L6 AR-1254-1	5.563	5.537	151.4E6	89535680	246.183	234.898
27) L6 AR-1254-2	5.713	5.685	107.1E6	64931210	199.889	195.687
28) L6 AR-1254-3	6.132	6.101	205.6E6	110.7E6	244.922	229.567
29) L6 AR-1254-4	6.346	6.313	28736958	14502528	59.742	55.630
30) L6 AR-1254-5	6.765	6.730	335.2E6	149.2E6	433.135	418.744
31) L7 AR-1260-1	6.247	6.216	256.8E6	138.7E6	512.292	494.432
32) L7 AR-1260-2	6.437	6.404	371.6E6	169.6E6	503.427	498.705
33) L7 AR-1260-3	6.804	6.556	324.3E6	111.0E6	494.727	402.957
34) L7 AR-1260-4	7.063	7.026	219.4E6	91190737	504.087	454.488
35) L7 AR-1260-5	7.307	7.268	619.0E6	195.5E6	490.290	436.745
36) L8 AR-1262-1	6.804	6.768	324.3E6	136.0E6	317.401	333.968
37) L8 AR-1262-2	7.307	7.268	619.0E6	195.5E6	377.589	381.512
38) L8 AR-1262-3	7.589	7.549	147.2E6	40414023	229.279	225.118
39) L8 AR-1262-4	7.653	7.613	396.1E6	105.8E6	369.713	363.837
40) L8 AR-1262-5	8.150	8.106	133.3E6	30285816	297.528	286.300
41) L9 AR-1268-1	7.589	7.549	147.2E6	40414023	80.106	82.233

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0072125\
 Data File : P0112332.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jul 2025 10:15
 Operator : YP/AJ
 Sample : AR1660CCC500
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1660CCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 22 01:44:41 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Jul 21 10:54:00 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9 AR-1268-2	7.653	7.613	396.1E6	105.8E6	254.316	253.717
43) L9 AR-1268-3	7.860	7.819	6757622	1705565	5.199	5.391
44) L9 AR-1268-4	8.150	8.106	133.3E6	30285816	277.544	271.592
45) L9 AR-1268-5	8.443	8.394	31026023	7575024	9.506	10.426



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0072125\
 Data File : P0112332.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jul 2025 10:15
 Operator : YP/AJ
 Sample : AR1660CCC500
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1660CCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 22 01:44:41 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Jul 21 10:54:00 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

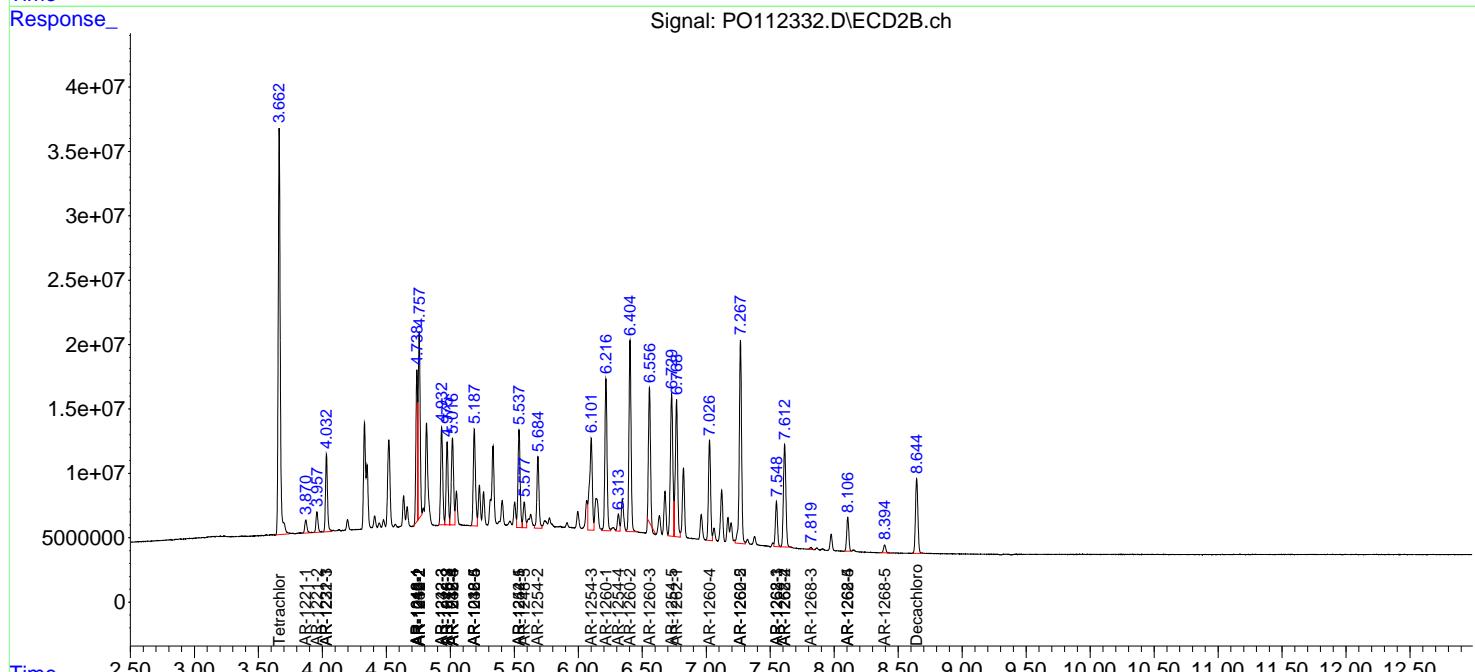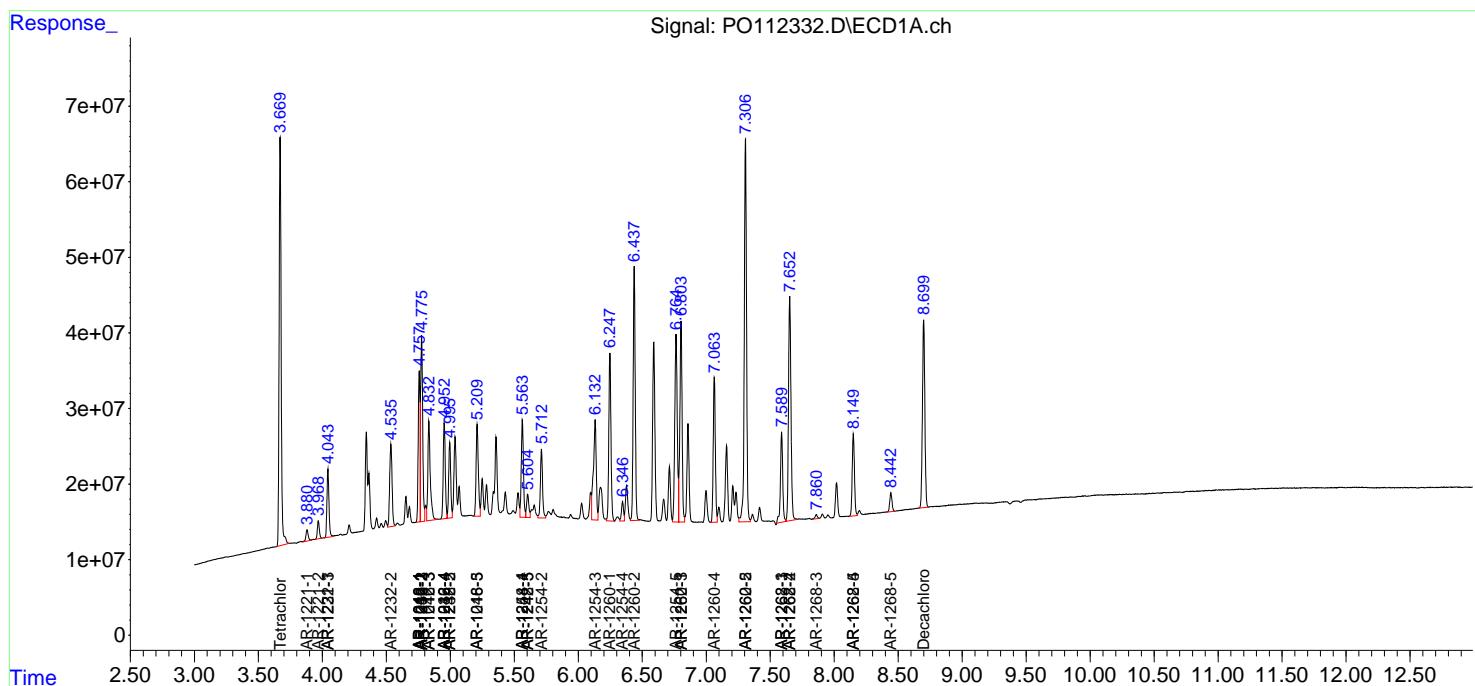


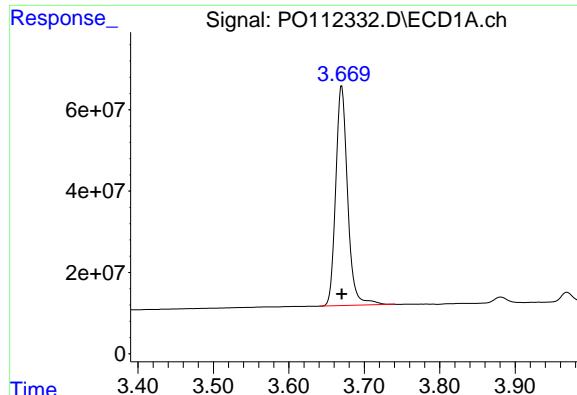

#1 Tetrachloro-m-xylene


R.T.: 3.670 min
 Delta R.T.: 0.000 min
 Response: 592831825
 Conc: 59.91 ng/ml

Instrument: ECD_O
ClientSampleId: AR1660CCC500

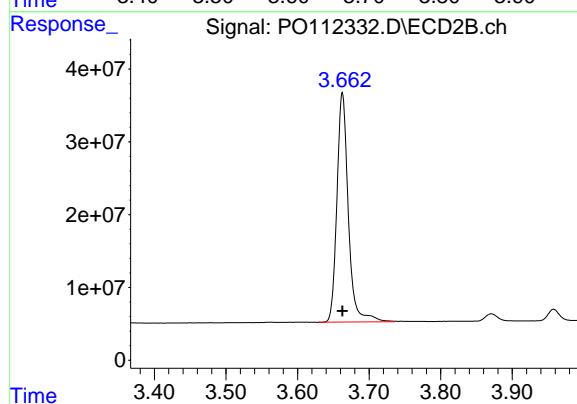


#1 Tetrachloro-m-xylene

R.T.: 3.663 min
 Delta R.T.: 0.000 min
 Response: 349312435
 Conc: 54.83 ng/ml

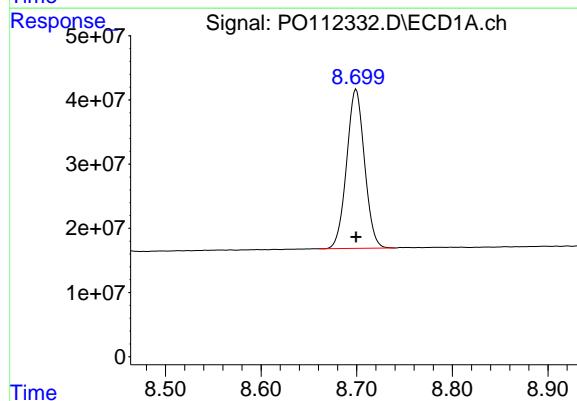


#2 Decachlorobiphenyl

R.T.: 8.699 min
 Delta R.T.: 0.000 min
 Response: 322926705
 Conc: 47.23 ng/ml

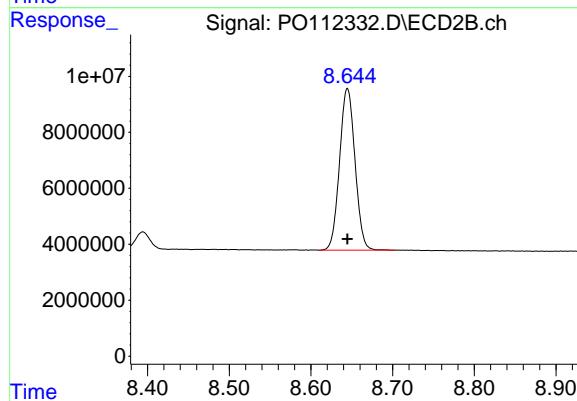

#2 Decachlorobiphenyl

R.T.: 8.645 min
 Delta R.T.: 0.000 min
 Response: 76065272
 Conc: 44.14 ng/ml

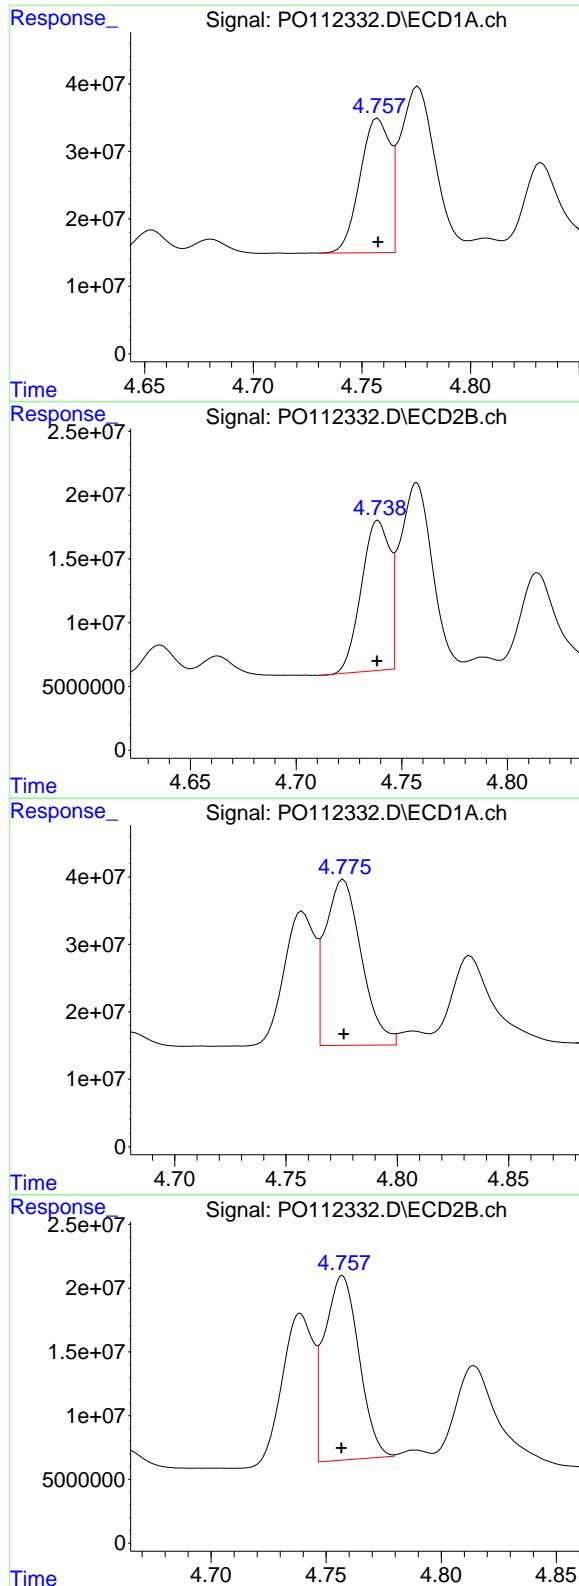

#3 AR-1016-1

R.T.: 4.757 min
 Delta R.T.: 0.000 min
 Response: 189589630
 Conc: 557.42 ng/ml

Instrument: ECD_O
 ClientSampleId: AR1660CCC500

#3 AR-1016-1


R.T.: 4.739 min
 Delta R.T.: 0.000 min
 Response: 110144934
 Conc: 494.29 ng/ml

#4 AR-1016-2

R.T.: 4.776 min
 Delta R.T.: 0.000 min
 Response: 277897665
 Conc: 558.82 ng/ml


#4 AR-1016-2

R.T.: 4.757 min
 Delta R.T.: 0.000 min
 Response: 150632998
 Conc: 457.72 ng/ml

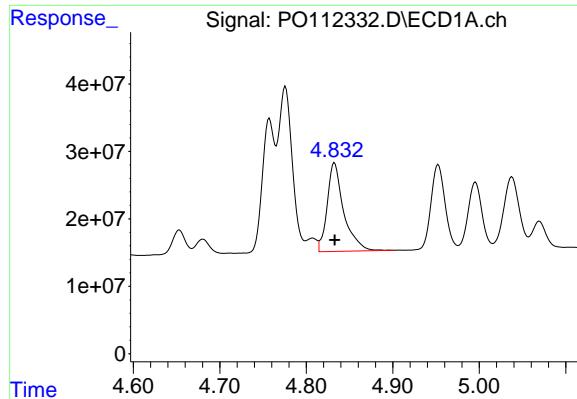


#5 AR-1016-3

R.T.: 4.833 min
 Delta R.T.: 0.000 min
Instrument:
 Response: 174938598 ECD_O
 Conc: 540.41 ng/ml
ClientSampleId:
 AR1660CCC500

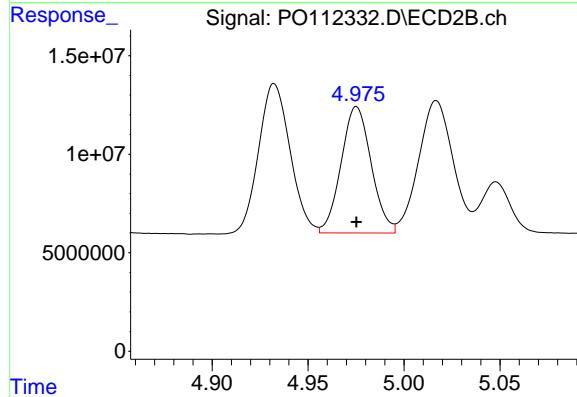


#5 AR-1016-3

R.T.: 4.975 min
 Delta R.T.: 0.000 min
 Response: 70204245
 Conc: 413.29 ng/ml

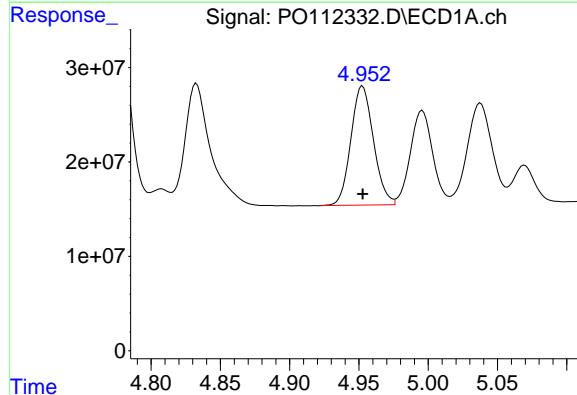


#6 AR-1016-4

R.T.: 4.953 min
 Delta R.T.: 0.000 min
 Response: 143249651
 Conc: 557.83 ng/ml

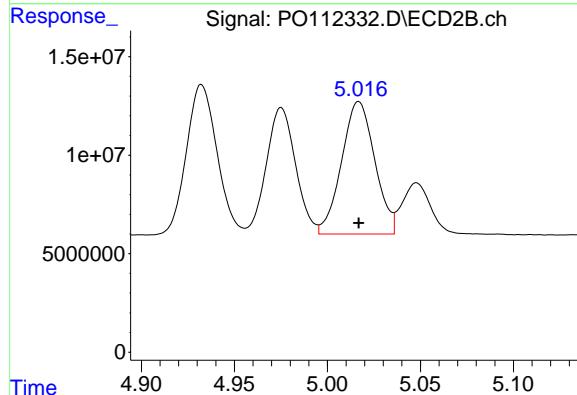

#6 AR-1016-4

R.T.: 5.017 min
 Delta R.T.: 0.000 min
 Response: 83633519
 Conc: 609.45 ng/ml

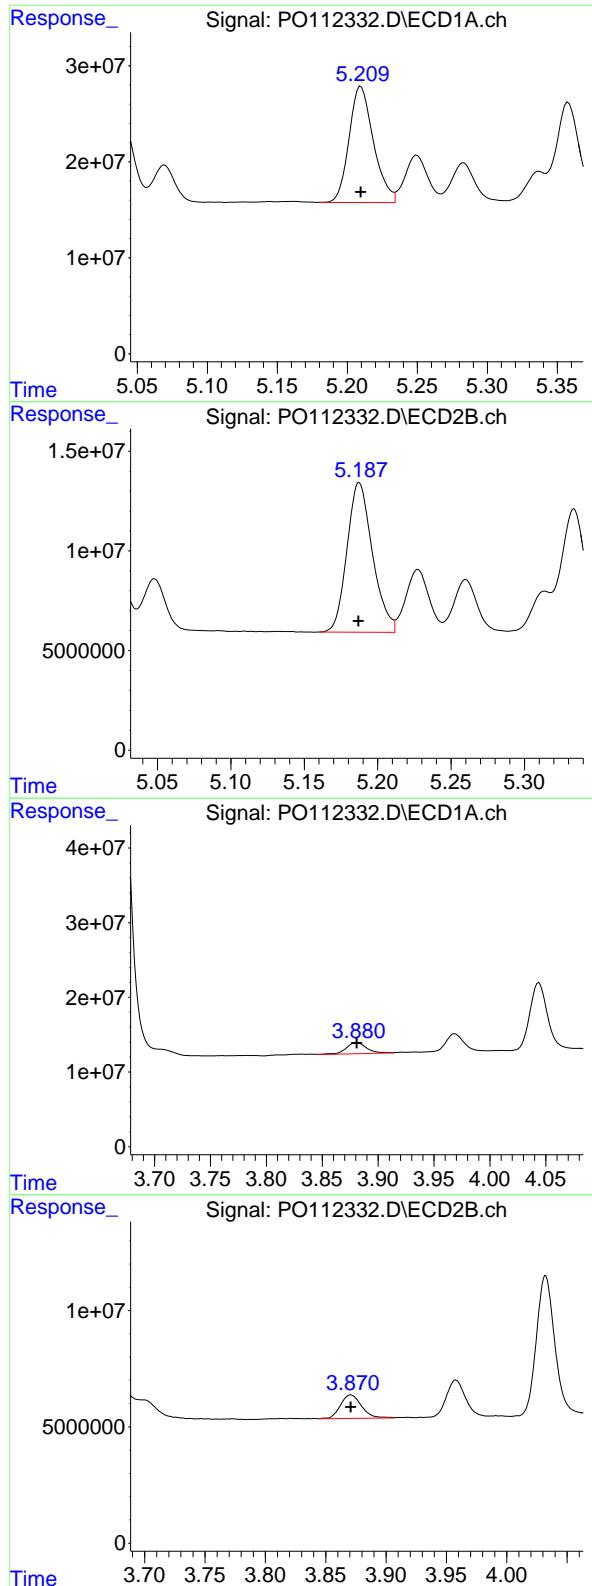

#7 AR-1016-5

R.T.: 5.210 min
 Delta R.T.: 0.000 min
 Response: 146690723
 Conc: 536.03 ng/ml

Instrument: ECD_O
 ClientSampleId: AR1660CCC500

#7 AR-1016-5


R.T.: 5.187 min
 Delta R.T.: 0.000 min
 Response: 90853568
 Conc: 526.84 ng/ml

#8 AR-1221-1

R.T.: 3.881 min
 Delta R.T.: 0.000 min
 Response: 18912211
 Conc: 162.18 ng/ml

#8 AR-1221-1


R.T.: 3.871 min
 Delta R.T.: 0.000 min
 Response: 12291205
 Conc: 149.36 ng/ml

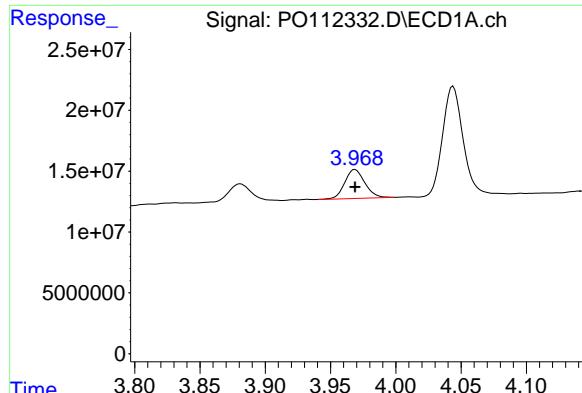

#9 AR-1221-2


R.T.: 3.969 min
Delta R.T.: 0.000 min
Response: 25420609
Conc: 322.43 ng/ml

Instrument: ECD_O
ClientSampleId: AR1660CCC500

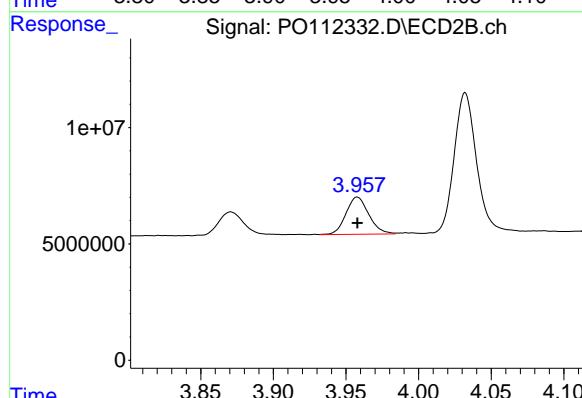


#9 AR-1221-2

R.T.: 3.958 min
Delta R.T.: 0.000 min
Response: 17491866
Conc: 294.71 ng/ml

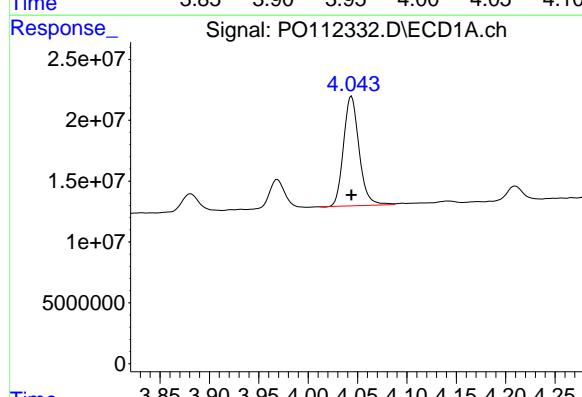


#10 AR-1221-3

R.T.: 4.044 min
Delta R.T.: 0.000 min
Response: 98680542
Conc: 366.05 ng/ml

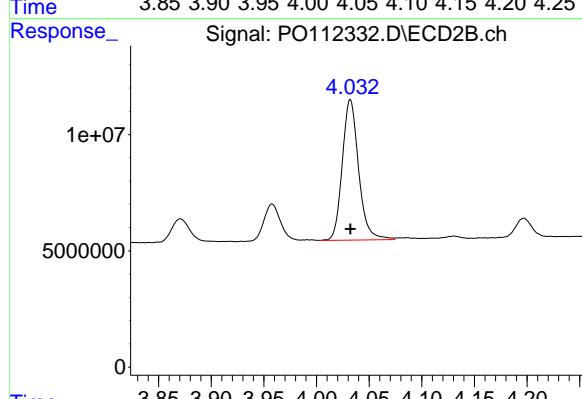

#10 AR-1221-3

R.T.: 4.032 min
Delta R.T.: 0.000 min
Response: 65225339
Conc: 345.52 ng/ml

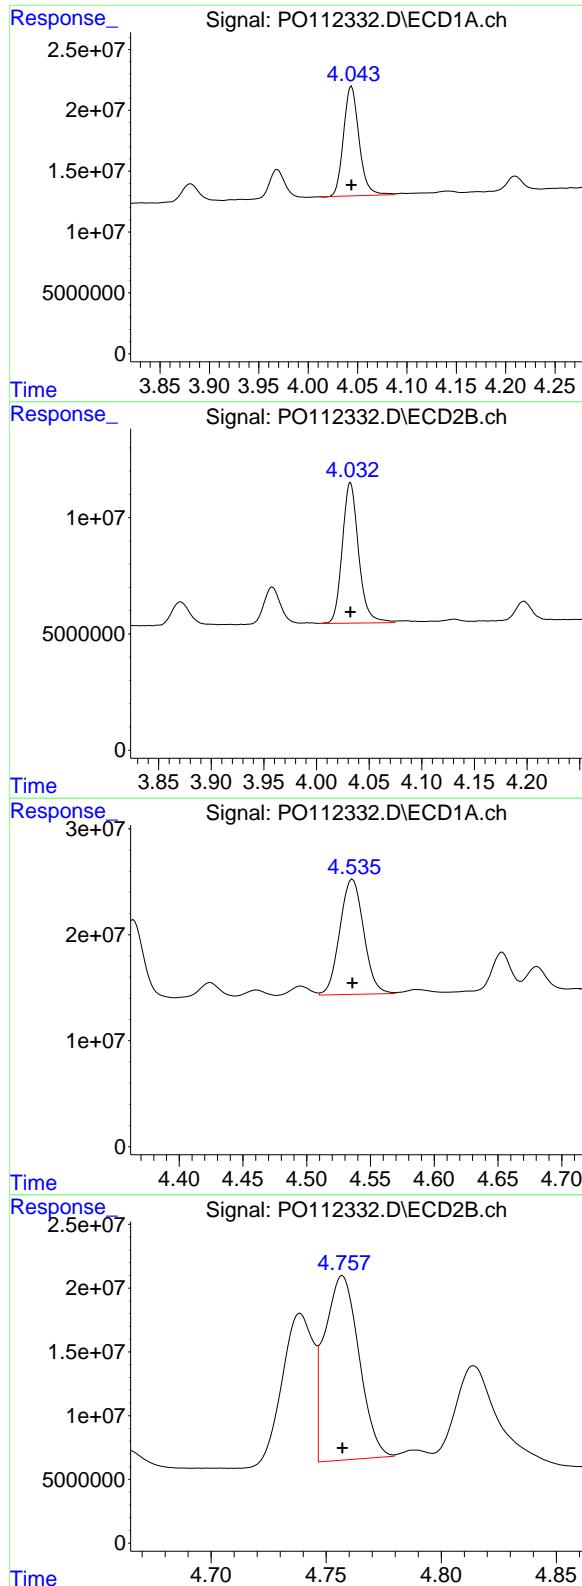

#11 AR-1232-1

R.T.: 4.044 min
 Delta R.T.: 0.000 min
 Response: 98680542
 Conc: 459.69 ng/ml

Instrument: ECD_O
 ClientSampleId: AR1660CCC500

#11 AR-1232-1


R.T.: 4.032 min
 Delta R.T.: 0.000 min
 Response: 65225339
 Conc: 434.55 ng/ml

#12 AR-1232-2

R.T.: 4.536 min
 Delta R.T.: 0.000 min
 Response: 141546178
 Conc: 1245.60 ng/ml


#12 AR-1232-2

R.T.: 4.757 min
 Delta R.T.: 0.000 min
 Response: 150632998
 Conc: 983.98 ng/ml

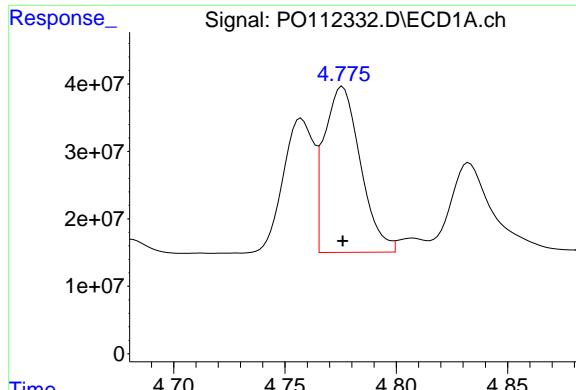


#13 AR-1232-3

R.T.: 4.776 min
 Delta R.T.: 0.000 min **Instrument:**
 Response: 277897665 ECD_O
 Conc: 1213.48 ng/ml **ClientSampleId :**
 AR1660CCC500

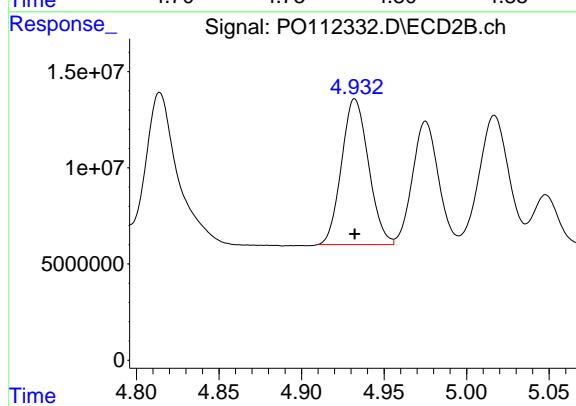


#13 AR-1232-3

R.T.: 4.932 min
 Delta R.T.: 0.000 min
 Response: 86189982
 Conc: 1141.50 ng/ml

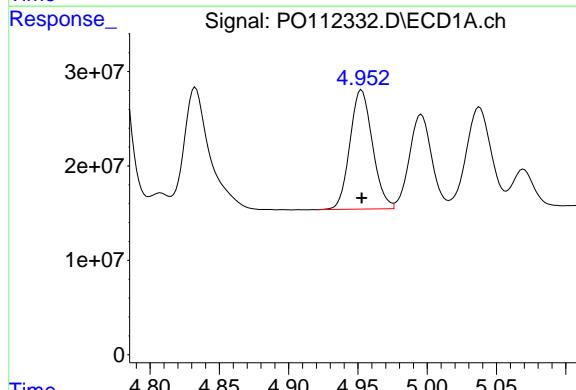


#14 AR-1232-4

R.T.: 4.953 min
 Delta R.T.: 0.000 min
 Response: 143249651
 Conc: 1253.31 ng/ml

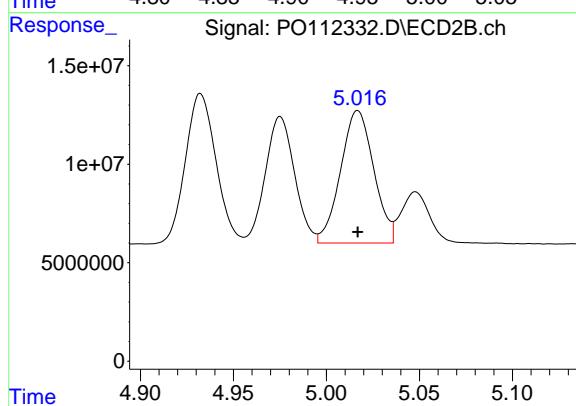


#14 AR-1232-4

R.T.: 5.017 min
 Delta R.T.: 0.000 min
 Response: 83633519
 Conc: 1267.40 ng/ml

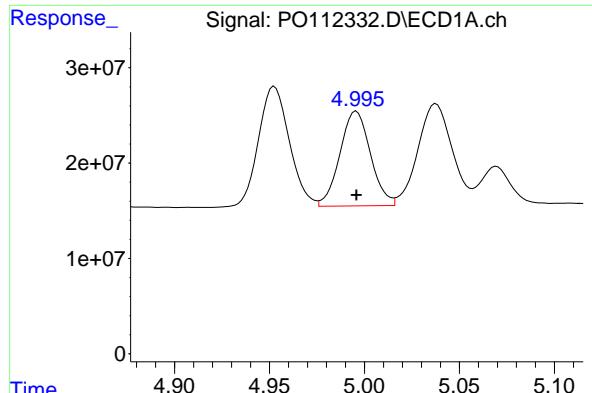


#15 AR-1232-5

R.T.: 4.996 min
 Delta R.T.: 0.000 min
 Response: 111448082
 Conc: 1518.36 ng/ml
Instrument: ECD_O
ClientSampleId: AR1660CCC500

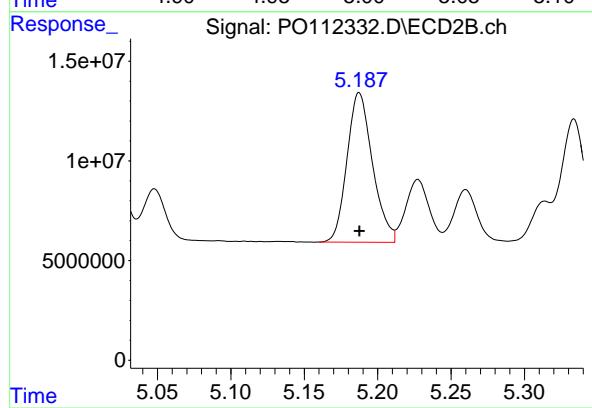


#15 AR-1232-5

R.T.: 5.187 min
 Delta R.T.: 0.000 min
 Response: 90853568
 Conc: 1223.45 ng/ml

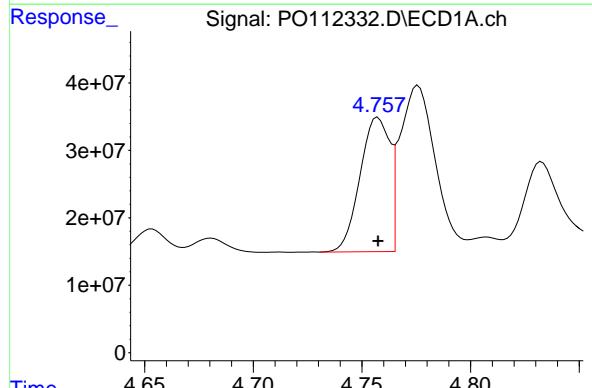


#16 AR-1242-1

R.T.: 4.757 min
 Delta R.T.: 0.000 min
 Response: 189589630
 Conc: 654.58 ng/ml

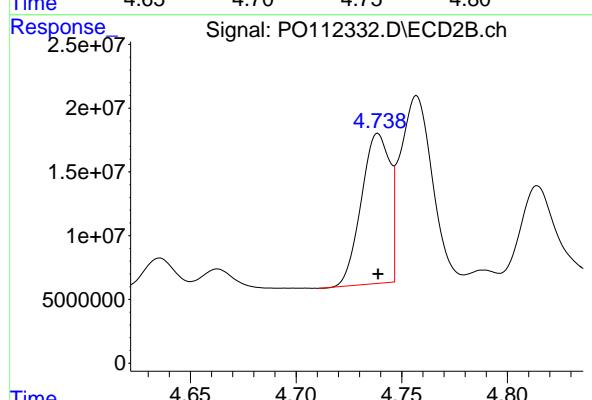

#16 AR-1242-1

R.T.: 4.739 min
 Delta R.T.: 0.000 min
 Response: 110144934
 Conc: 568.17 ng/ml

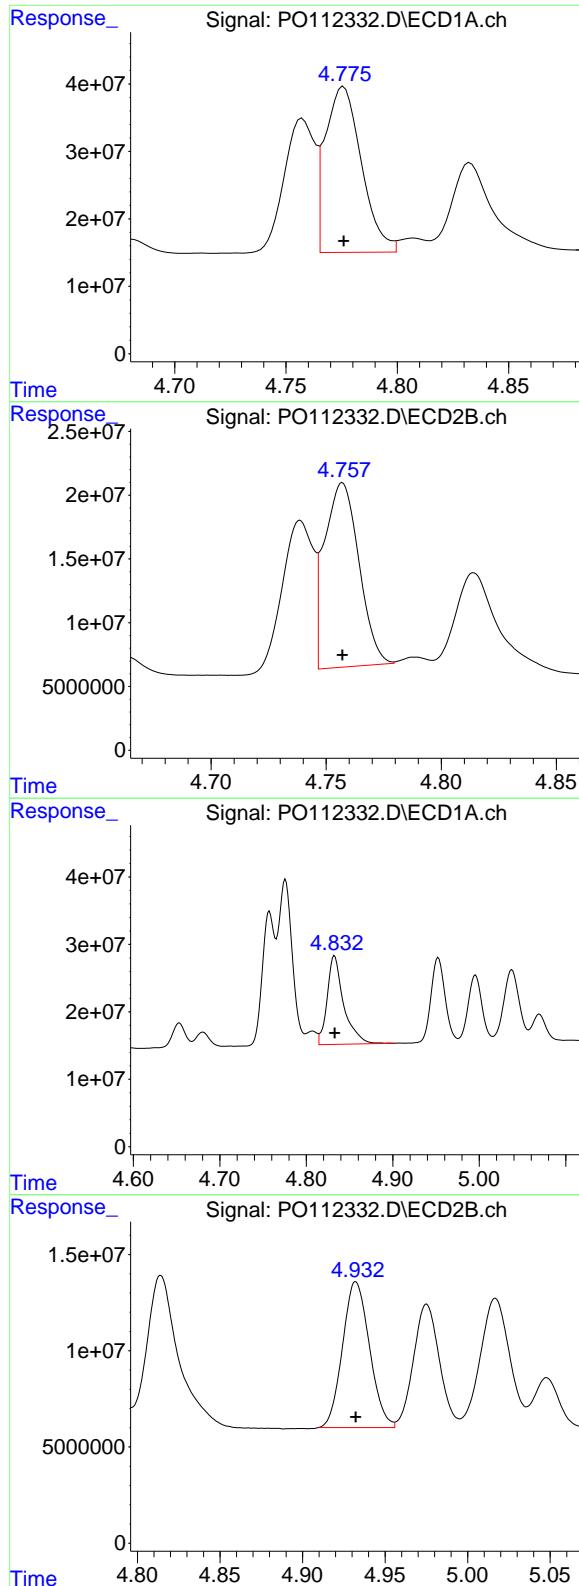

#17 AR-1242-2

R.T.: 4.776 min
 Delta R.T.: 0.000 min
 Response: 277897665
 Conc: 652.47 ng/ml

Instrument: ECD_O
 ClientSampleId: AR1660CCC500

#17 AR-1242-2


R.T.: 4.757 min
 Delta R.T.: 0.000 min
 Response: 150632998
 Conc: 531.61 ng/ml

#18 AR-1242-3

R.T.: 4.833 min
 Delta R.T.: 0.000 min
 Response: 174938598
 Conc: 639.20 ng/ml

#18 AR-1242-3

R.T.: 4.932 min
 Delta R.T.: 0.000 min
 Response: 86189982
 Conc: 591.65 ng/ml

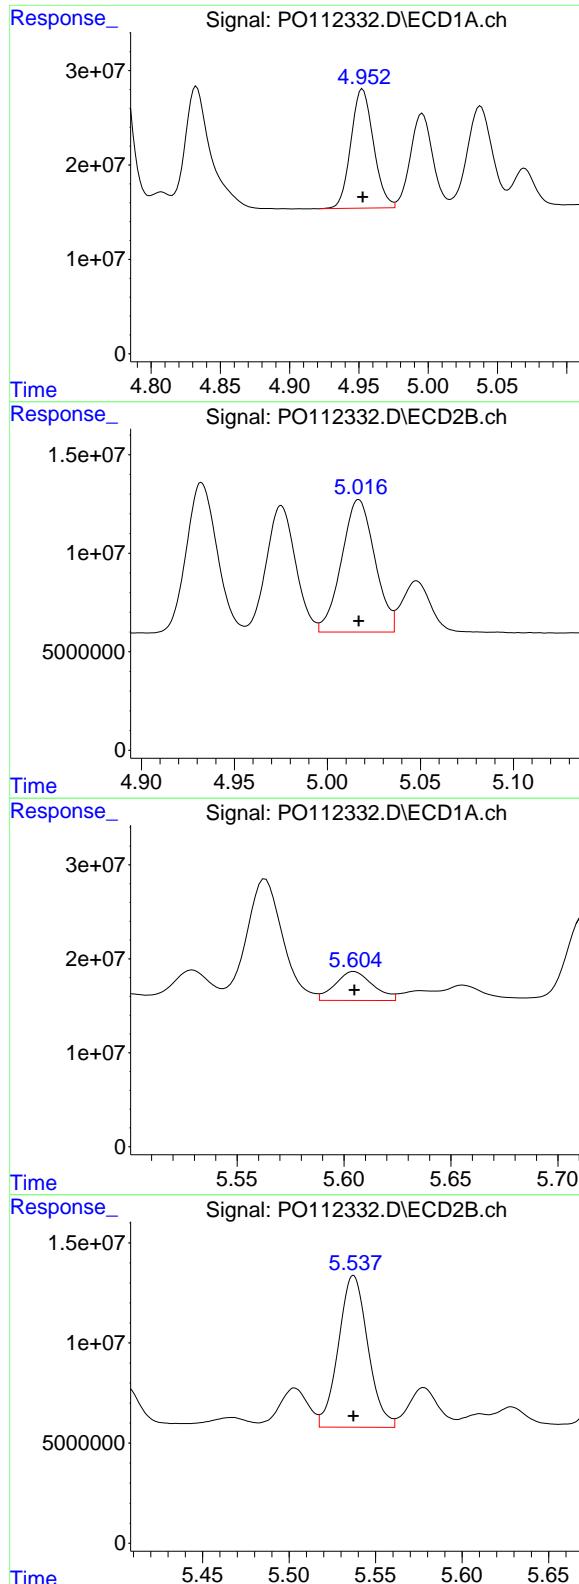

#19 AR-1242-4

R.T.: 4.953 min
 Delta R.T.: 0.000 min
 Response: 143249651
 Conc: 635.77 ng/ml

Instrument: ECD_O
 ClientSampleId: AR1660CCC500

#19 AR-1242-4


R.T.: 5.017 min
 Delta R.T.: 0.000 min
 Response: 83633519
 Conc: 589.63 ng/ml

#20 AR-1242-5

R.T.: 5.605 min
 Delta R.T.: 0.000 min
 Response: 37881289
 Conc: 178.96 ng/ml

#20 AR-1242-5

R.T.: 5.537 min
 Delta R.T.: 0.000 min
 Response: 89535680
 Conc: 492.67 ng/ml

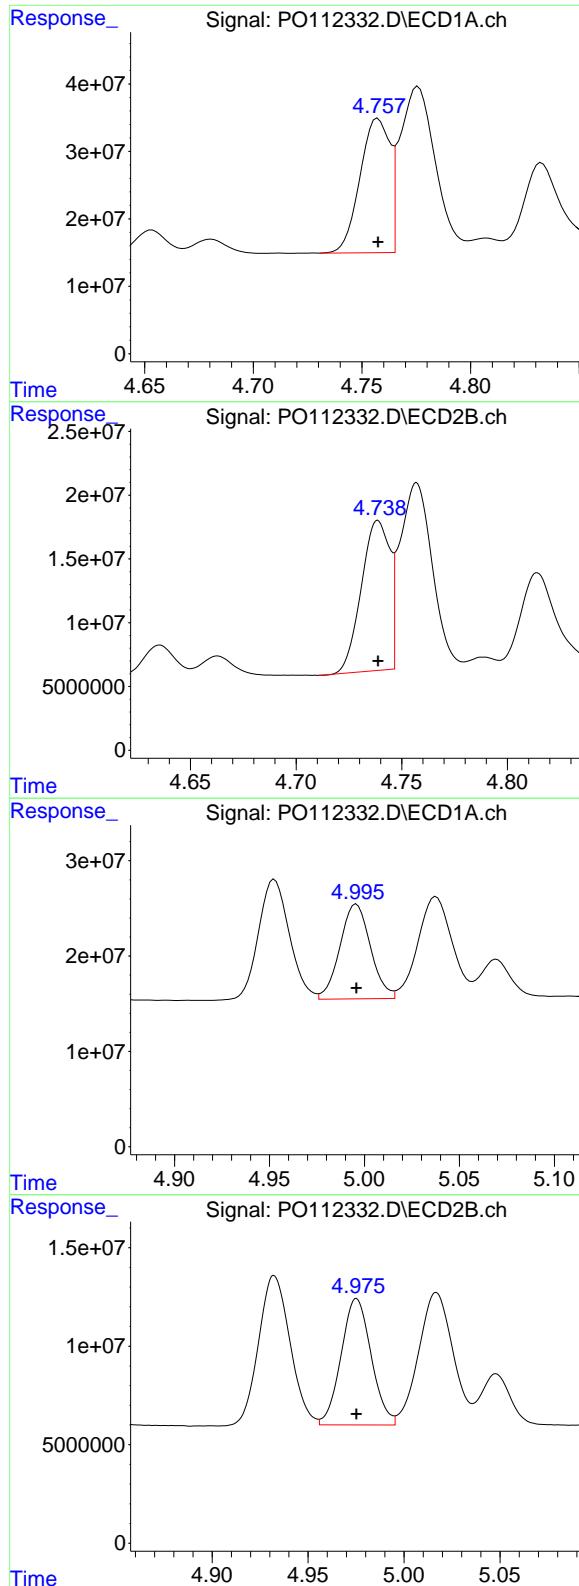

#21 AR-1248-1

R.T.: 4.757 min
 Delta R.T.: 0.000 min
 Response: 189589630
 Conc: 835.57 ng/ml

Instrument: ECD_O
 ClientSampleId: AR1660CCC500

#21 AR-1248-1


R.T.: 4.739 min
 Delta R.T.: 0.000 min
 Response: 110144934
 Conc: 713.52 ng/ml

#22 AR-1248-2

R.T.: 4.996 min
 Delta R.T.: 0.000 min
 Response: 111448082
 Conc: 361.46 ng/ml

#22 AR-1248-2

R.T.: 4.975 min
 Delta R.T.: 0.000 min
 Response: 70204245
 Conc: 341.18 ng/ml

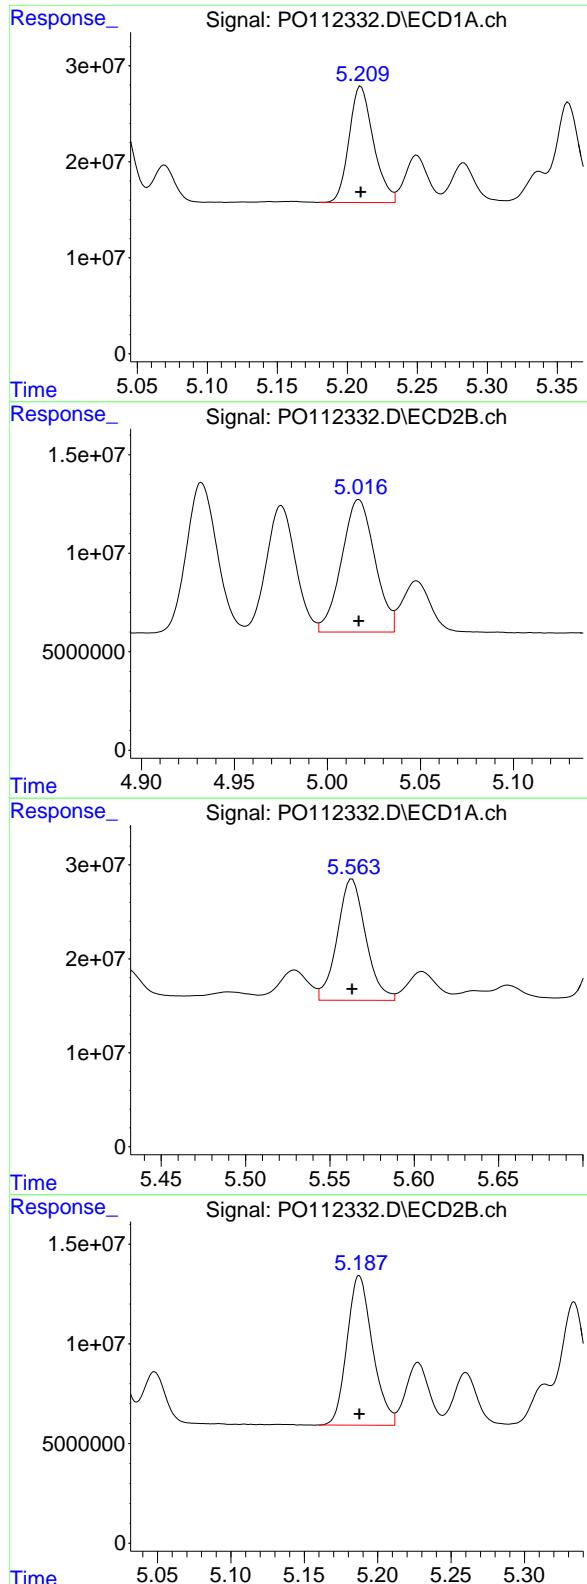

#23 AR-1248-3

R.T.: 5.210 min
 Delta R.T.: 0.000 min
 Response: 146690723
 Conc: 360.14 ng/ml

Instrument: ECD_O
ClientSampleId: AR1660CCC500

#23 AR-1248-3


R.T.: 5.017 min
 Delta R.T.: 0.000 min
 Response: 83633519
 Conc: 389.36 ng/ml

#24 AR-1248-4

R.T.: 5.563 min
 Delta R.T.: 0.000 min
 Response: 151430506
 Conc: 262.38 ng/ml

#24 AR-1248-4

R.T.: 5.187 min
 Delta R.T.: 0.000 min
 Response: 90853568
 Conc: 351.16 ng/ml

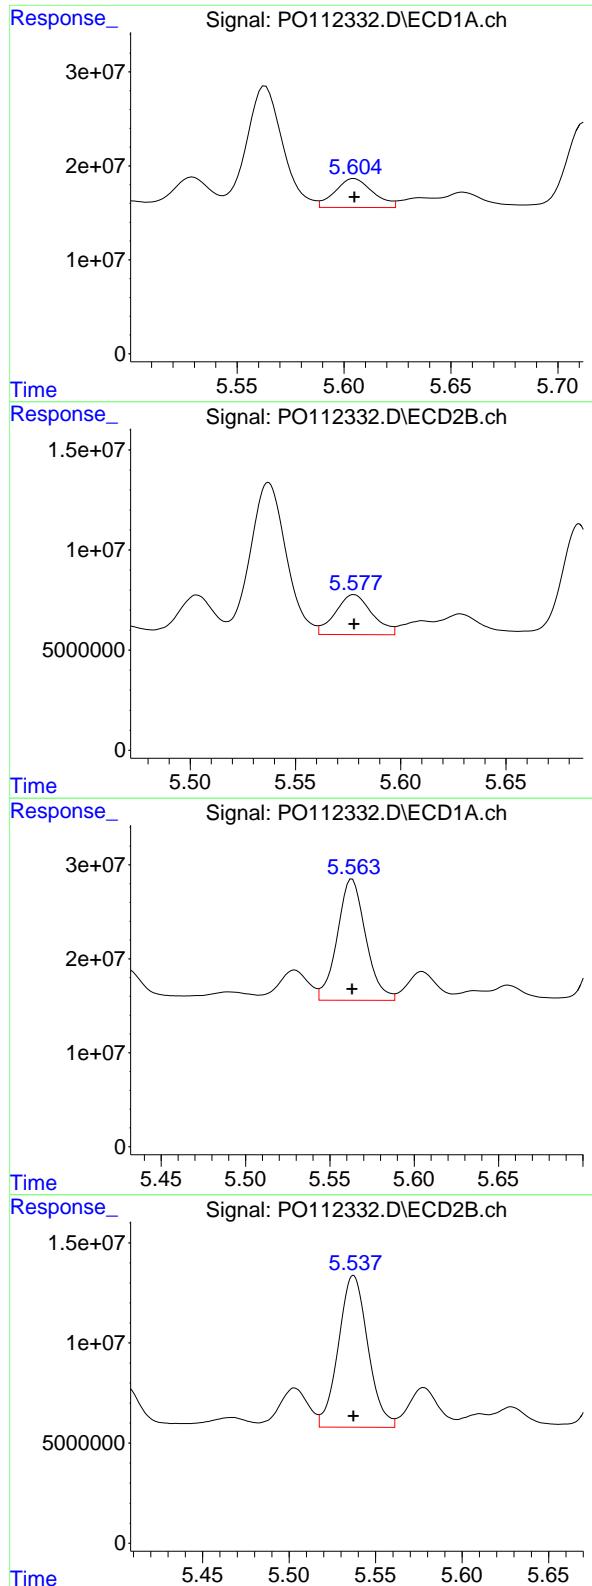

#25 AR-1248-5

R.T.: 5.605 min
 Delta R.T.: 0.000 min
 Response: 37881289
 Conc: 97.06 ng/ml

Instrument: ECD_O
 ClientSampleId: AR1660CCC500

#25 AR-1248-5


R.T.: 5.578 min
 Delta R.T.: 0.000 min
 Response: 24255105
 Conc: 96.81 ng/ml

#26 AR-1254-1

R.T.: 5.563 min
 Delta R.T.: 0.000 min
 Response: 151430506
 Conc: 246.18 ng/ml

#26 AR-1254-1

R.T.: 5.537 min
 Delta R.T.: 0.000 min
 Response: 89535680
 Conc: 234.90 ng/ml

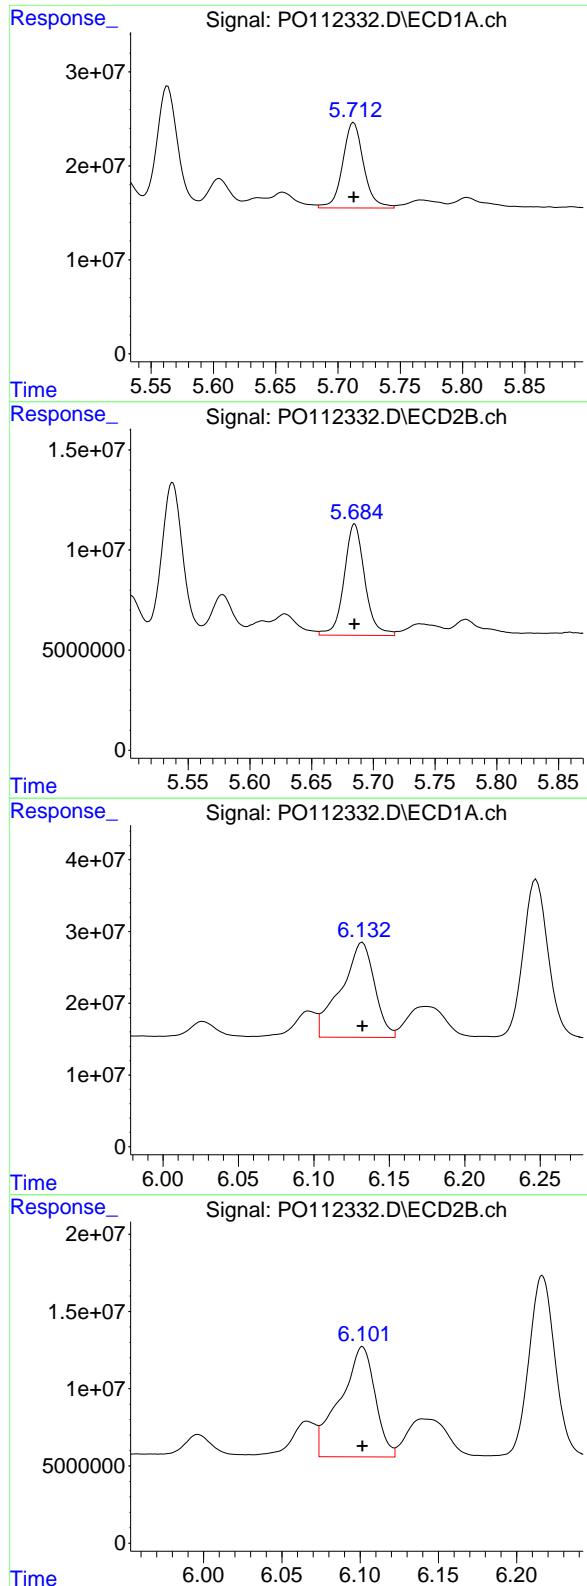

#27 AR-1254-2

R.T.: 5.713 min
 Delta R.T.: 0.000 min
 Response: 107077635
 Conc: 199.89 ng/ml

Instrument: ECD_O
 ClientSampleId: AR1660CCC500

#27 AR-1254-2


R.T.: 5.685 min
 Delta R.T.: 0.000 min
 Response: 64931210
 Conc: 195.69 ng/ml

#28 AR-1254-3

R.T.: 6.132 min
 Delta R.T.: 0.000 min
 Response: 205631323
 Conc: 244.92 ng/ml

#28 AR-1254-3

R.T.: 6.101 min
 Delta R.T.: 0.000 min
 Response: 110661125
 Conc: 229.57 ng/ml

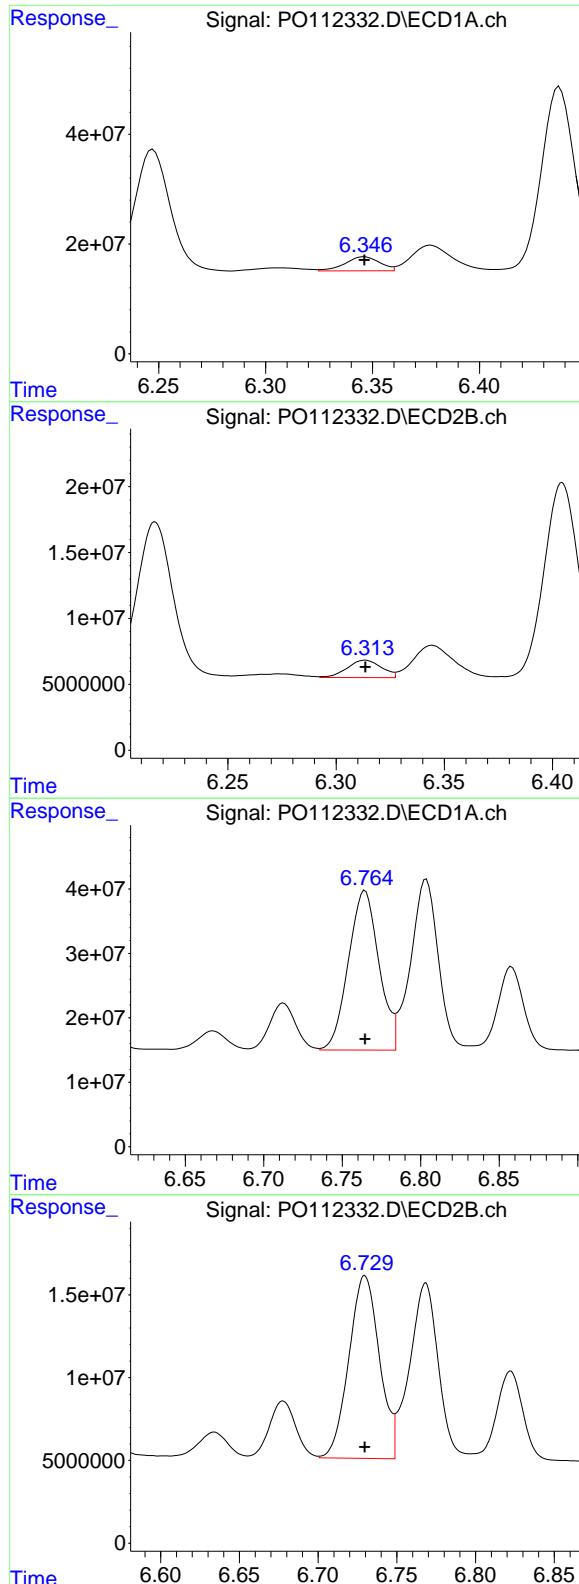

#29 AR-1254-4

R.T.: 6.346 min
 Delta R.T.: 0.000 min
 Response: 28736958
 Conc: 59.74 ng/ml

Instrument: ECD_O
ClientSampleId: AR1660CCC500

#29 AR-1254-4


R.T.: 6.313 min
 Delta R.T.: 0.000 min
 Response: 14502528
 Conc: 55.63 ng/ml

#30 AR-1254-5

R.T.: 6.765 min
 Delta R.T.: 0.000 min
 Response: 335223572
 Conc: 433.13 ng/ml

#30 AR-1254-5

R.T.: 6.730 min
 Delta R.T.: 0.000 min
 Response: 149222076
 Conc: 418.74 ng/ml

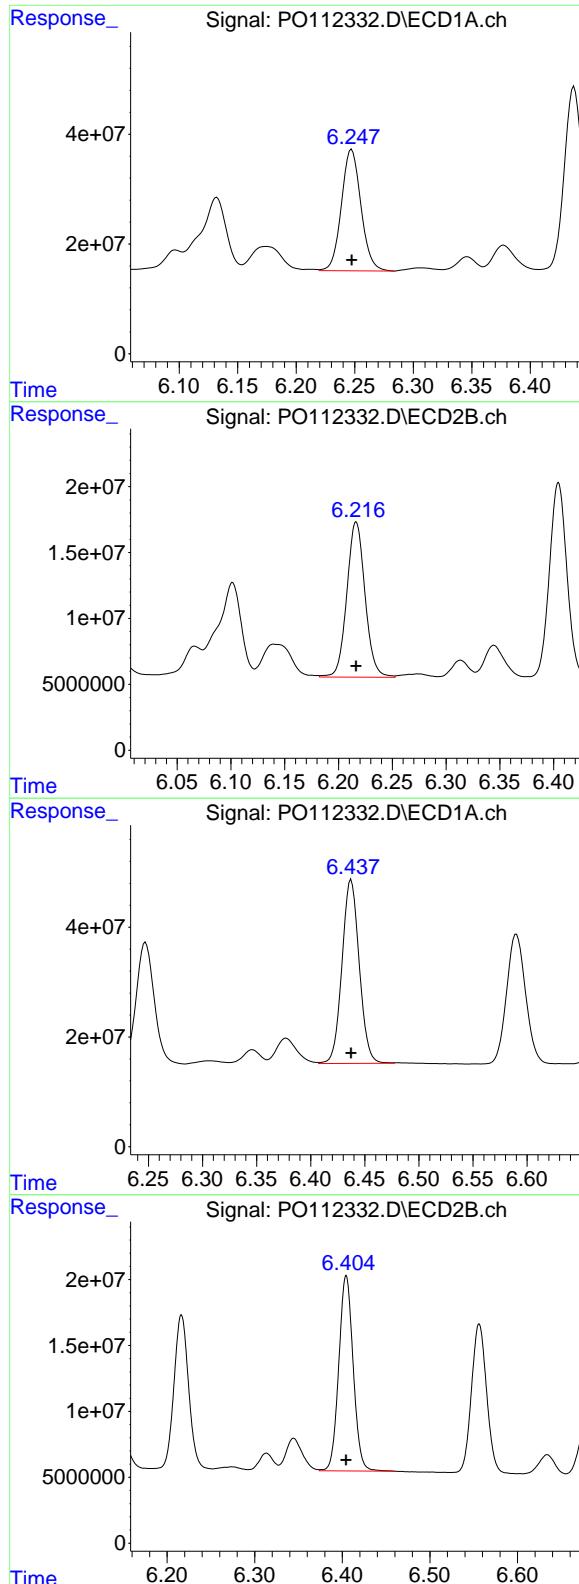

#31 AR-1260-1

R.T.: 6.247 min
 Delta R.T.: 0.000 min
 Response: 256780650
 Conc: 512.29 ng/ml

Instrument: ECD_O
ClientSampleId: AR1660CCC500

#31 AR-1260-1


R.T.: 6.216 min
 Delta R.T.: 0.000 min
 Response: 138718933
 Conc: 494.43 ng/ml

#32 AR-1260-2

R.T.: 6.437 min
 Delta R.T.: 0.000 min
 Response: 371597084
 Conc: 503.43 ng/ml

#32 AR-1260-2


R.T.: 6.404 min
 Delta R.T.: 0.000 min
 Response: 169558040
 Conc: 498.70 ng/ml



#33 AR-1260-3


R.T.: 6.804 min
 Delta R.T.: 0.000 min
 Response: 324284745
 Conc: 494.73 ng/ml

Instrument: ECD_O
 ClientSampleId: AR1660CCC500

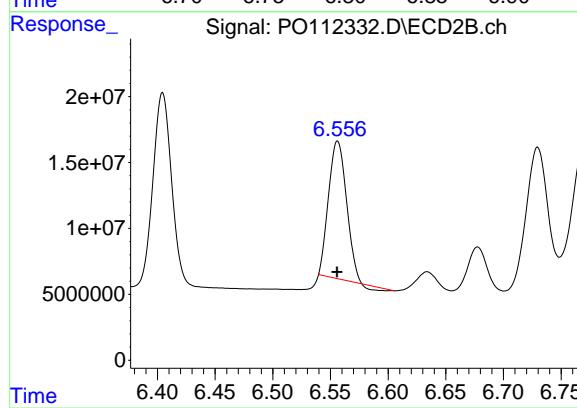


#33 AR-1260-3

R.T.: 6.556 min
 Delta R.T.: 0.000 min
 Response: 111049471
 Conc: 402.96 ng/ml




#34 AR-1260-4

R.T.: 7.063 min
 Delta R.T.: 0.000 min
 Response: 219402703
 Conc: 504.09 ng/ml

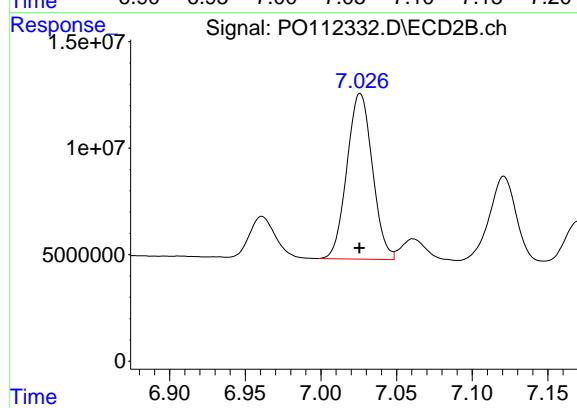

#34 AR-1260-4

R.T.: 7.026 min
 Delta R.T.: 0.000 min
 Response: 91190737
 Conc: 454.49 ng/ml

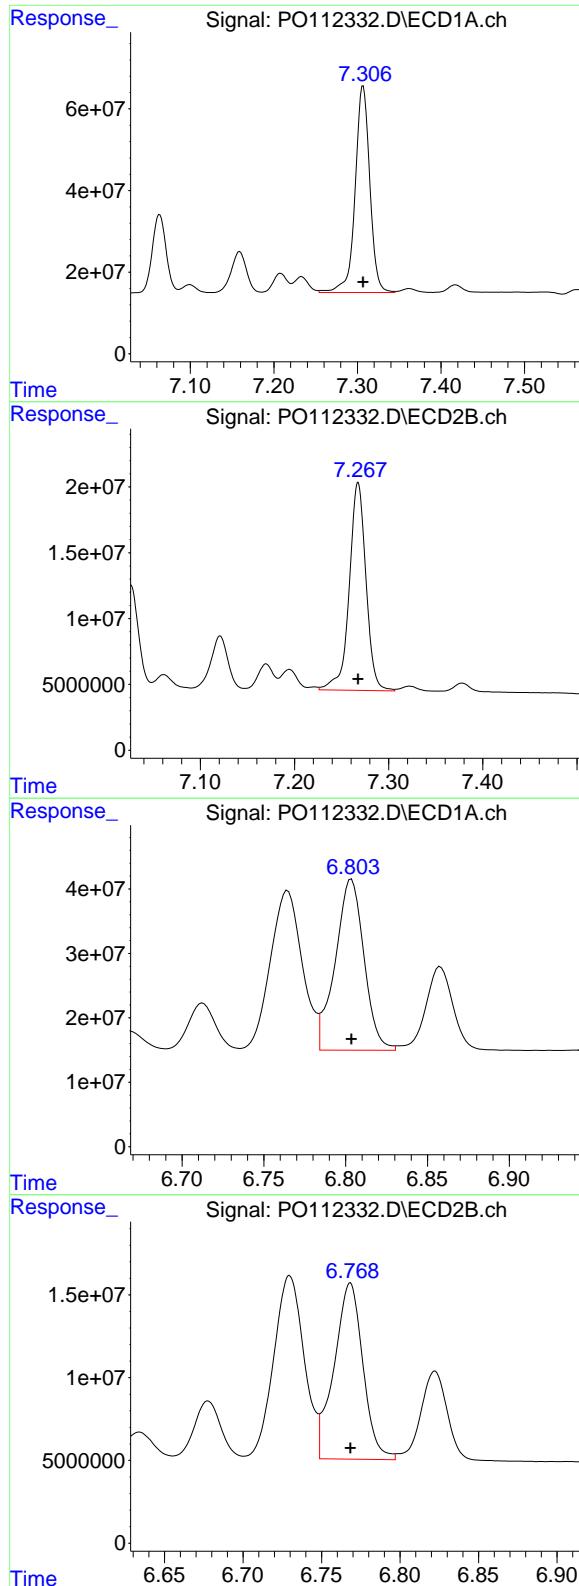

#35 AR-1260-5

R.T.: 7.307 min
Delta R.T.: 0.000 min **Instrument:**
Response: 619009807 ECD_O
Conc: 490.29 ng/ml **ClientSampleId:**
AR1660CCC500

#35 AR-1260-5


R.T.: 7.268 min
Delta R.T.: 0.000 min
Response: 195543329
Conc: 436.75 ng/ml

#36 AR-1262-1

R.T.: 6.804 min
Delta R.T.: 0.000 min
Response: 324284745
Conc: 317.40 ng/ml


#36 AR-1262-1

R.T.: 6.768 min
Delta R.T.: 0.000 min
Response: 136031986
Conc: 333.97 ng/ml




#37 AR-1262-2

R.T.: 7.307 min
 Delta R.T.: 0.000 min **Instrument:**
 Response: 619009807 ECD_O
 Conc: 377.59 ng/ml **ClientSampleId:**
 AR1660CCC500

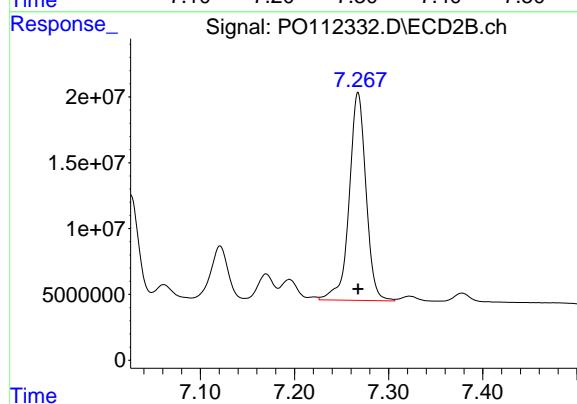


#37 AR-1262-2

R.T.: 7.268 min
 Delta R.T.: 0.000 min
 Response: 195543329
 Conc: 381.51 ng/ml

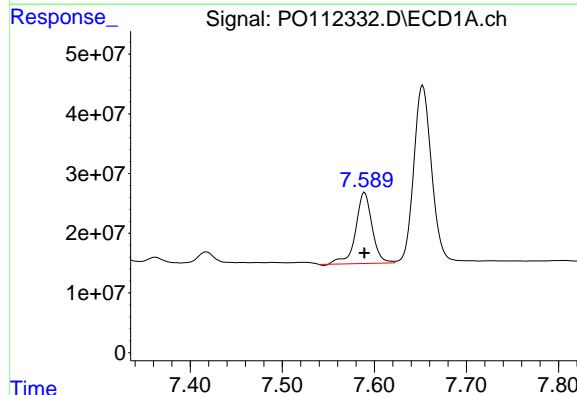


#38 AR-1262-3

R.T.: 7.589 min
 Delta R.T.: 0.000 min
 Response: 147191344
 Conc: 229.28 ng/ml

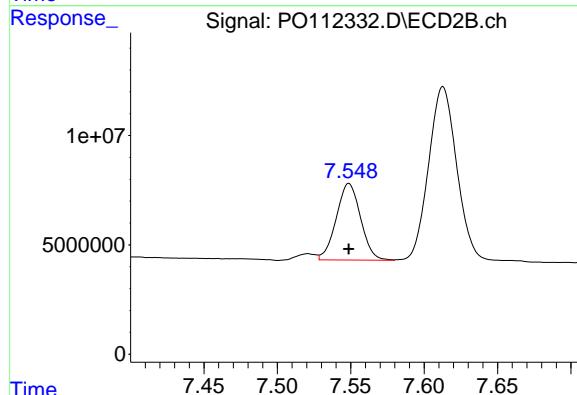

#38 AR-1262-3

R.T.: 7.549 min
 Delta R.T.: 0.000 min
 Response: 40414023
 Conc: 225.12 ng/ml

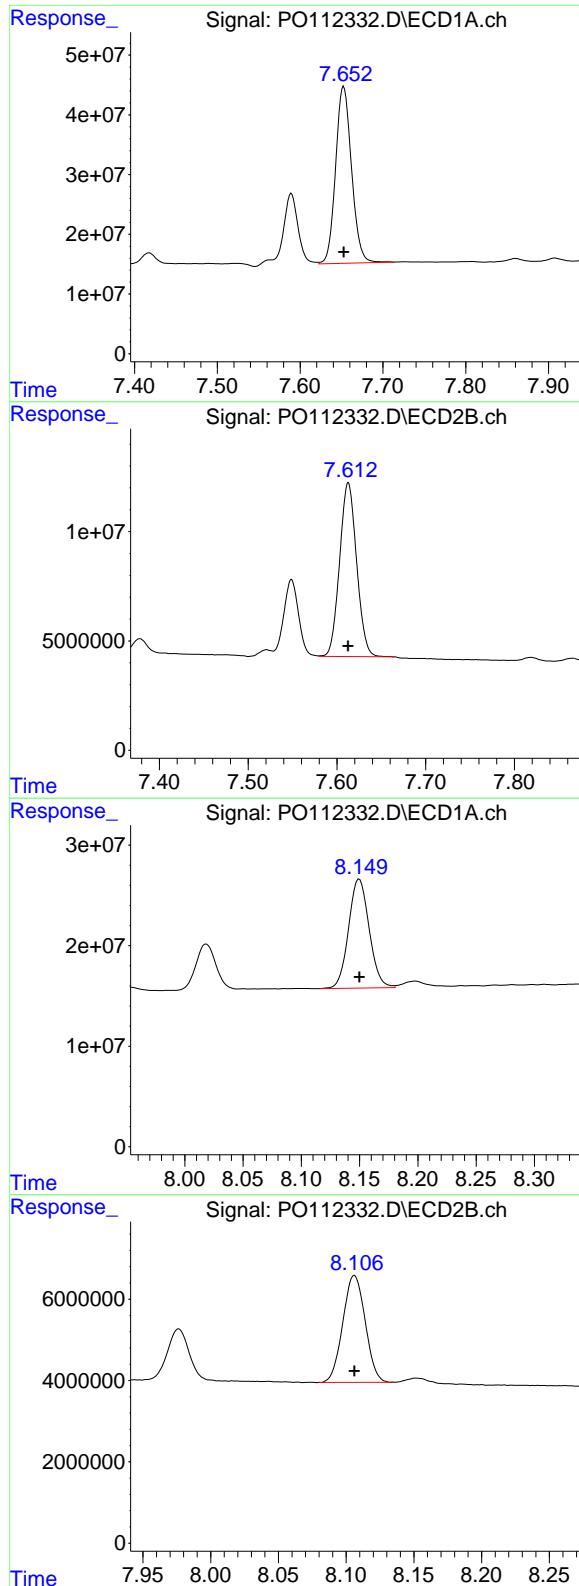

#39 AR-1262-4

R.T.: 7.653 min
Delta R.T.: 0.000 min
Response: 396123736
Conc: 369.71 ng/ml

Instrument: ECD_O
ClientSampleId: AR1660CCC500

#39 AR-1262-4


R.T.: 7.613 min
Delta R.T.: 0.000 min
Response: 105847263
Conc: 363.84 ng/ml

#40 AR-1262-5

R.T.: 8.150 min
Delta R.T.: 0.000 min
Response: 133334327
Conc: 297.53 ng/ml


#40 AR-1262-5

R.T.: 8.106 min
Delta R.T.: 0.000 min
Response: 30285816
Conc: 286.30 ng/ml

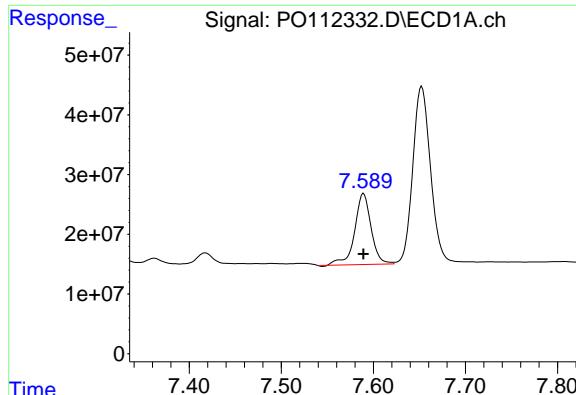


#41 AR-1268-1

R.T.: 7.589 min
 Delta R.T.: 0.000 min **Instrument:**
 Response: 147191344 ECD_O
 Conc: 80.11 ng/ml **ClientSampleId:**
 AR1660CCC500

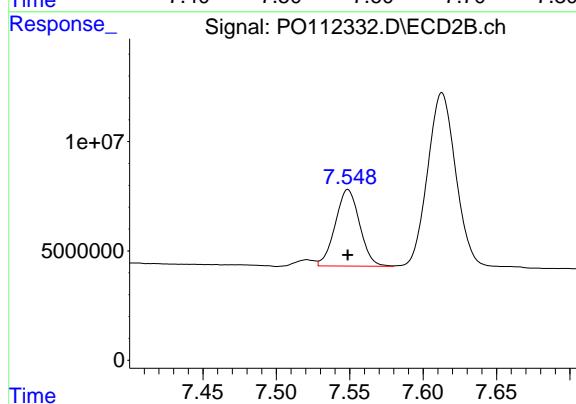


#41 AR-1268-1

R.T.: 7.549 min
 Delta R.T.: 0.000 min
 Response: 40414023
 Conc: 82.23 ng/ml

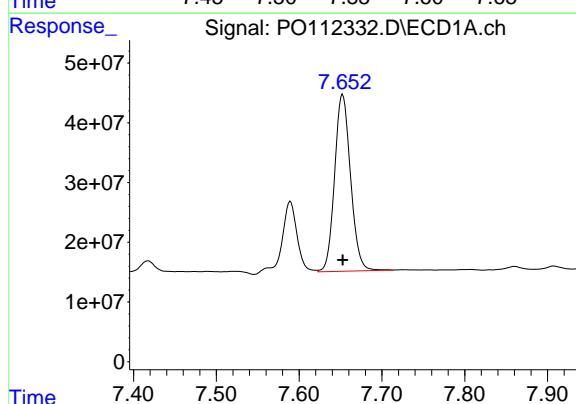


#42 AR-1268-2

R.T.: 7.653 min
 Delta R.T.: 0.000 min
 Response: 396123736
 Conc: 254.32 ng/ml

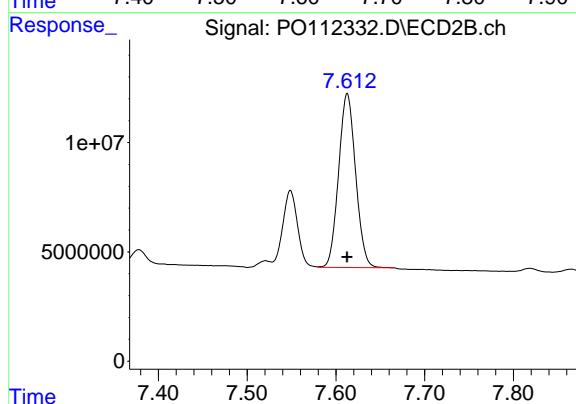

#42 AR-1268-2

R.T.: 7.613 min
 Delta R.T.: 0.000 min
 Response: 105847263
 Conc: 253.72 ng/ml

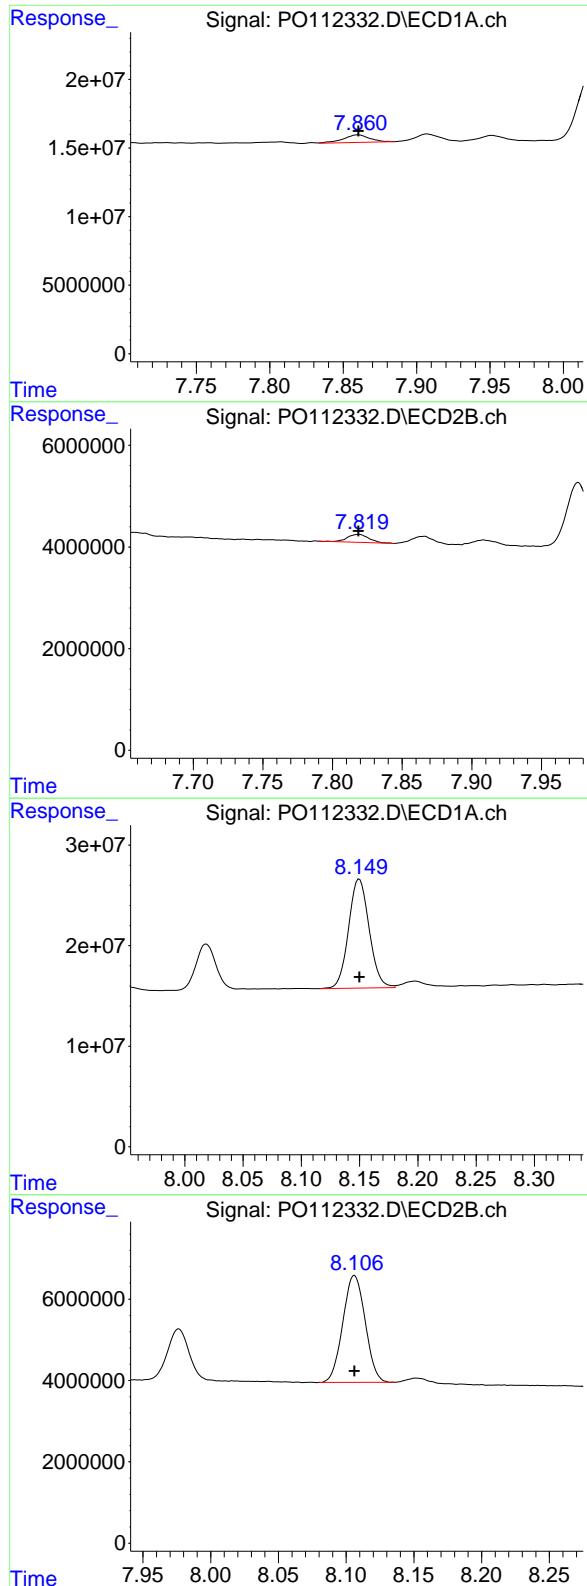

#43 AR-1268-3

R.T.: 7.860 min
 Delta R.T.: 0.000 min
 Response: 6757622
 Conc: 5.20 ng/ml

Instrument: ECD_O
ClientSampleId: AR1660CCC500

#43 AR-1268-3


R.T.: 7.819 min
 Delta R.T.: 0.000 min
 Response: 1705565
 Conc: 5.39 ng/ml

#44 AR-1268-4

R.T.: 8.150 min
 Delta R.T.: 0.000 min
 Response: 133334327
 Conc: 277.54 ng/ml

#44 AR-1268-4

R.T.: 8.106 min
 Delta R.T.: 0.000 min
 Response: 30285816
 Conc: 271.59 ng/ml

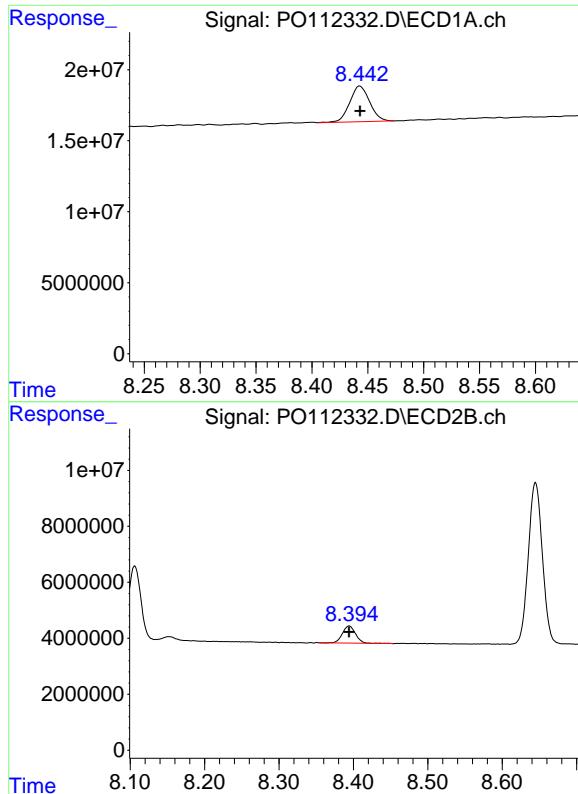

#45 AR-1268-5

R.T.: 8.443 min
Delta R.T.: 0.000 min
Response: 31026023
Conc: 9.51 ng/ml

Instrument: ECD_O
ClientSampleId: AR1660CCC500

#45 AR-1268-5

R.T.: 8.394 min
Delta R.T.: 0.000 min
Response: 7575024
Conc: 10.43 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0072125\
 Data File : P0112346.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jul 2025 16:10
 Operator : YP/AJ
 Sample : AR1660CCC500
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1660CCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 22 01:51:22 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Jul 21 10:54:00 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	3.669	3.663	530.3E6	312.7E6	53.594	49.077
2) SA Decachlor...	8.697	8.645	306.0E6	74451617	44.762	43.199

Target Compounds

3) L1 AR-1016-1	4.755	4.739	167.7E6	97218771	493.201	436.283
4) L1 AR-1016-2	4.774	4.757	250.9E6	135.3E6	504.494	411.128
5) L1 AR-1016-3	4.831	4.975	157.2E6	61302098	485.598	360.883 #
6) L1 AR-1016-4	4.950	5.017	127.0E6	74044940	494.505	539.578
7) L1 AR-1016-5	5.208	5.187	141.5E6	82476996	517.122	478.265
8) L2 AR-1221-1	3.879	3.871	15722840	10860941	134.828	131.976
9) L2 AR-1221-2	3.967	3.958	23372962	15634060	296.459	263.406
10) L2 AR-1221-3	4.042	4.032	89050131	57995386	330.327	307.217
11) L3 AR-1232-1	4.042	4.032	89050131	57995386	414.828	386.380
12) L3 AR-1232-2	4.533	4.757	128.4E6	135.3E6	1129.844	883.826
13) L3 AR-1232-3	4.774	4.932	250.9E6	76865187	1095.506	1018.001
14) L3 AR-1232-4	4.950	5.017	127.0E6	74044940	1111.045	1122.094
15) L3 AR-1232-5	4.994	5.187	95361665	82476996	1299.201	1110.653
16) L4 AR-1242-1	4.755	4.739	167.7E6	97218771	579.170	501.494
17) L4 AR-1242-2	4.774	4.757	250.9E6	135.3E6	589.033	477.501
18) L4 AR-1242-3	4.831	4.932	157.2E6	76865187	574.363	527.640
19) L4 AR-1242-4	4.950	5.017	127.0E6	74044940	563.597	522.029
20) L4 AR-1242-5	5.603	5.537	36994145	81589337	174.772	448.949 #
21) L5 AR-1248-1	4.755	4.739	167.7E6	97218771	739.309	629.785
22) L5 AR-1248-2	4.994	4.975	95361665	61302098	309.289	297.919
23) L5 AR-1248-3	5.208	5.017	141.5E6	74044940	347.433	344.718
24) L5 AR-1248-4	5.561	5.187	136.9E6	82476996	237.149	318.780 #
25) L5 AR-1248-5	5.603	5.577	36994145	23078382	94.783	92.111
26) L6 AR-1254-1	5.561	5.537	136.9E6	81589337	222.512	214.051
27) L6 AR-1254-2	5.710	5.684	99169571	59758329	185.126	180.097
28) L6 AR-1254-3	6.129	6.101	179.6E6	101.2E6	213.949	210.041
29) L6 AR-1254-4	6.344	6.312	23749159	13372256	49.373	51.295
30) L6 AR-1254-5	6.761	6.729	300.0E6	140.3E6	387.663	393.801
31) L7 AR-1260-1	6.245	6.215	226.0E6	125.6E6	450.876	447.762
32) L7 AR-1260-2	6.435	6.404	335.1E6	159.1E6	453.990	468.063
33) L7 AR-1260-3	6.801	6.556	294.4E6	95203208	449.209	345.457
34) L7 AR-1260-4	7.061	7.025	198.1E6	89511018	455.117	446.116
35) L7 AR-1260-5	7.304	7.268	561.8E6	205.5E6	444.971	459.066
36) L8 AR-1262-1	6.801	6.768	294.4E6	130.4E6	288.198	320.095
37) L8 AR-1262-2	7.304	7.268	561.8E6	205.5E6	342.688	401.010
38) L8 AR-1262-3	7.587	7.548	142.8E6	45395147	222.427	252.864
39) L8 AR-1262-4	7.650	7.612	364.2E6	112.7E6	339.960	387.420
40) L8 AR-1262-5	8.147	8.106	125.0E6	31357784	278.982	296.434
41) L9 AR-1268-1	7.587	7.548	142.8E6	45395147	77.712	92.369

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0072125\
 Data File : P0112346.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jul 2025 16:10
 Operator : YP/AJ
 Sample : AR1660CCC500
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1660CCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 22 01:51:22 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Jul 21 10:54:00 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9 AR-1268-2	7.650	7.612	364.2E6	112.7E6	233.849	270.163
43) L9 AR-1268-3	7.858	7.817	6022964	1789840	4.634	5.657
44) L9 AR-1268-4	8.147	8.106	125.0E6	31357784	260.244	281.205
45) L9 AR-1268-5	8.442	8.394	29486963	7543187	9.035	10.383



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0072125\
 Data File : P0112346.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jul 2025 16:10
 Operator : YP/AJ
 Sample : AR1660CCC500
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1660CCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 22 01:51:22 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Jul 21 10:54:00 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

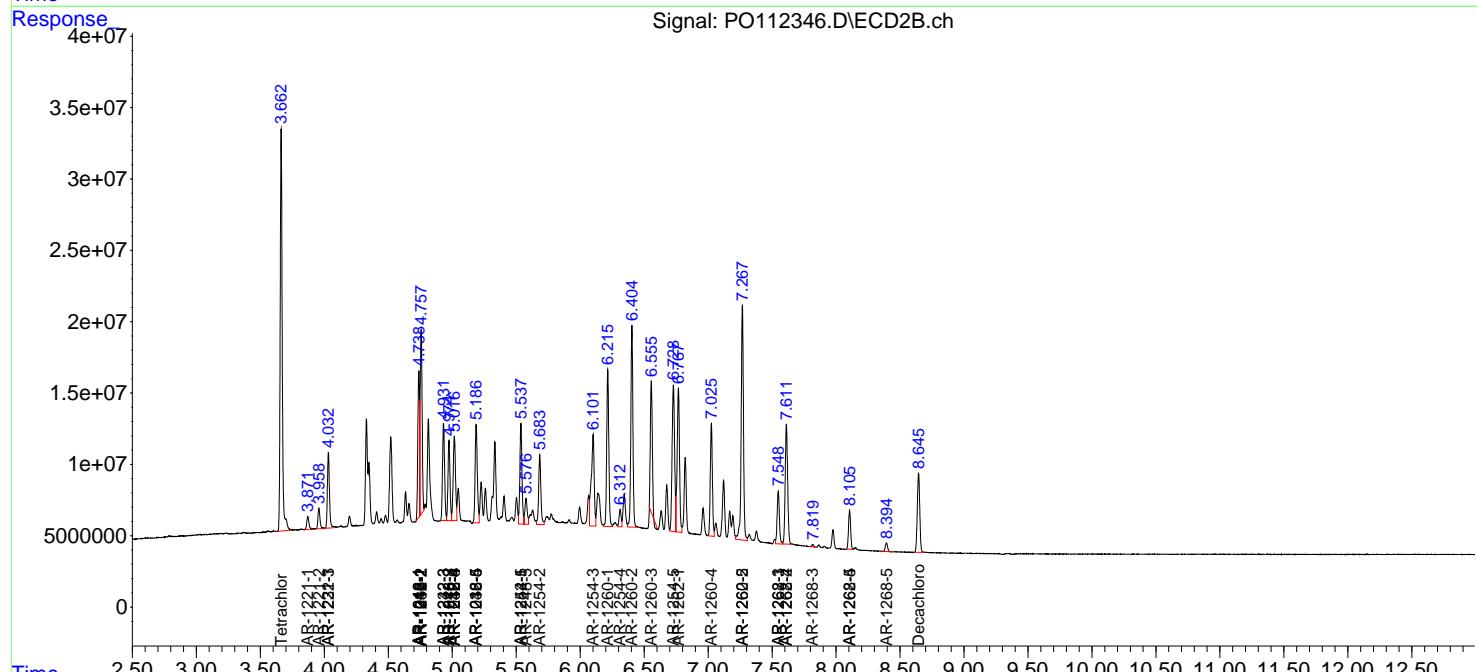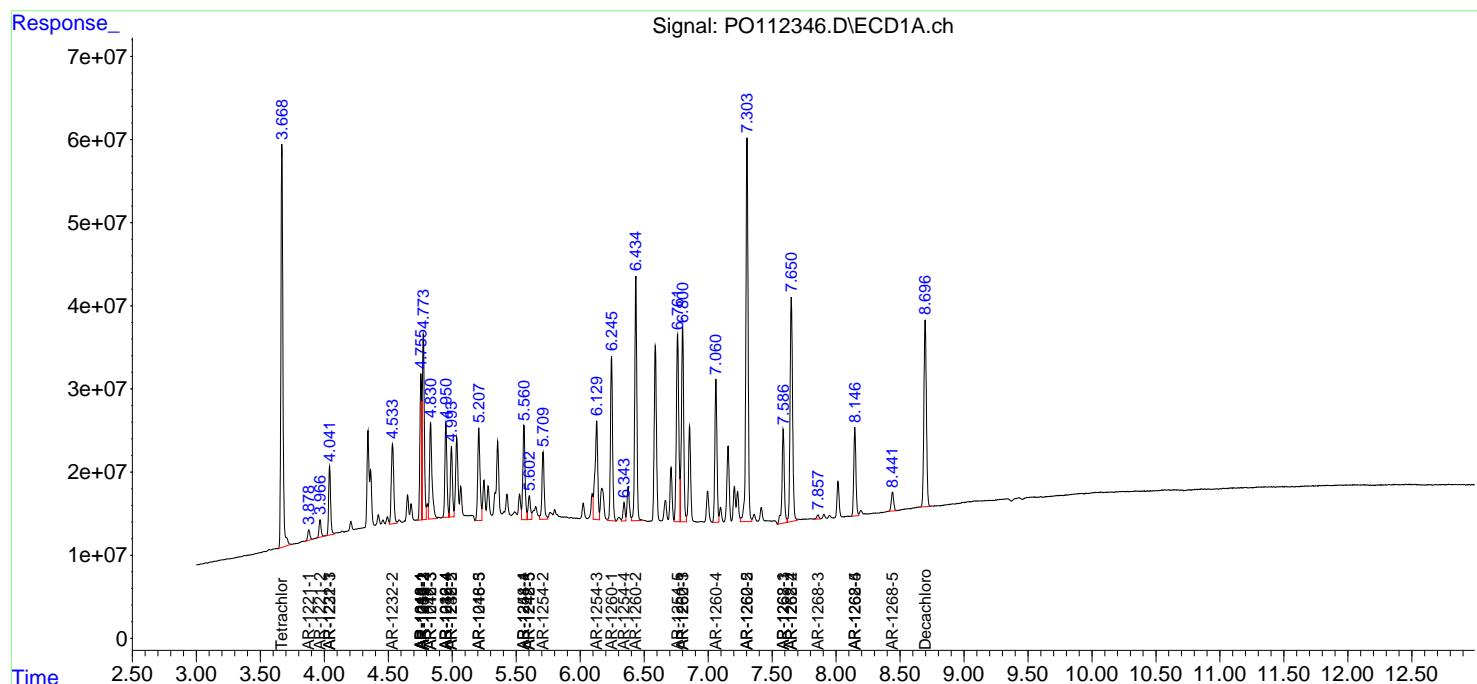

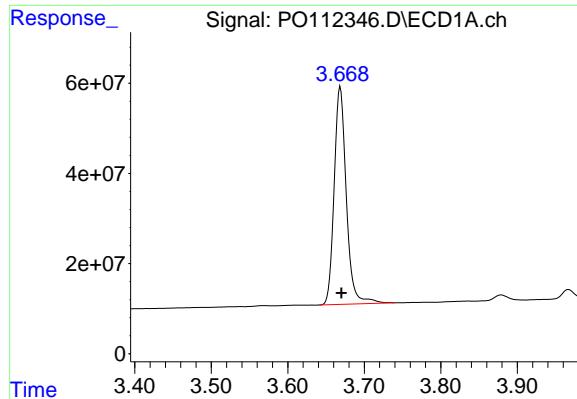


#1 Tetrachloro-m-xylene

R.T.: 3.669 min
Delta R.T.: -0.001 min
Response: 530299098
Conc: 53.59 ng/ml

Instrument:


ECD_O

ClientSampleId :
AR1660CCC500

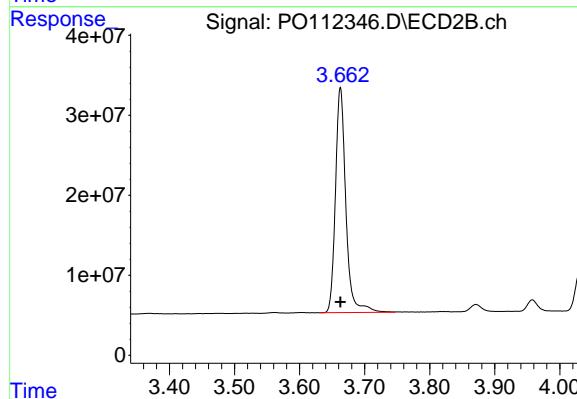


#1 Tetrachloro-m-xylene

R.T.: 3.663 min
Delta R.T.: 0.000 min
Response: 312671778
Conc: 49.08 ng/ml

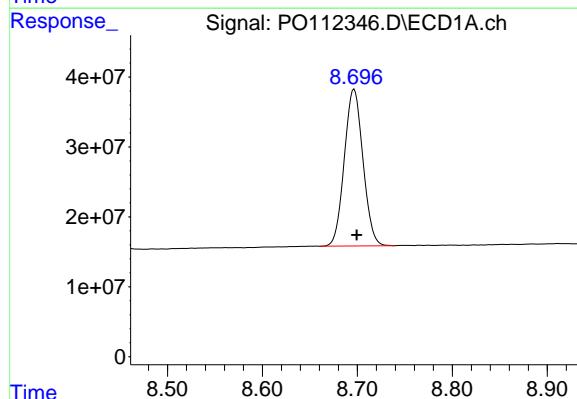


#2 Decachlorobiphenyl

R.T.: 8.697 min
Delta R.T.: -0.003 min
Response: 306036817
Conc: 44.76 ng/ml

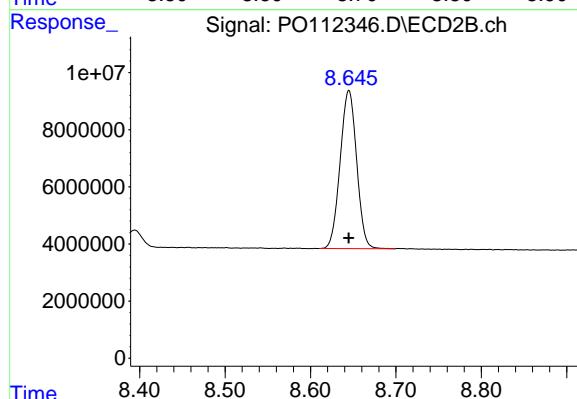

#2 Decachlorobiphenyl

R.T.: 8.645 min
Delta R.T.: 0.000 min
Response: 74451617
Conc: 43.20 ng/ml

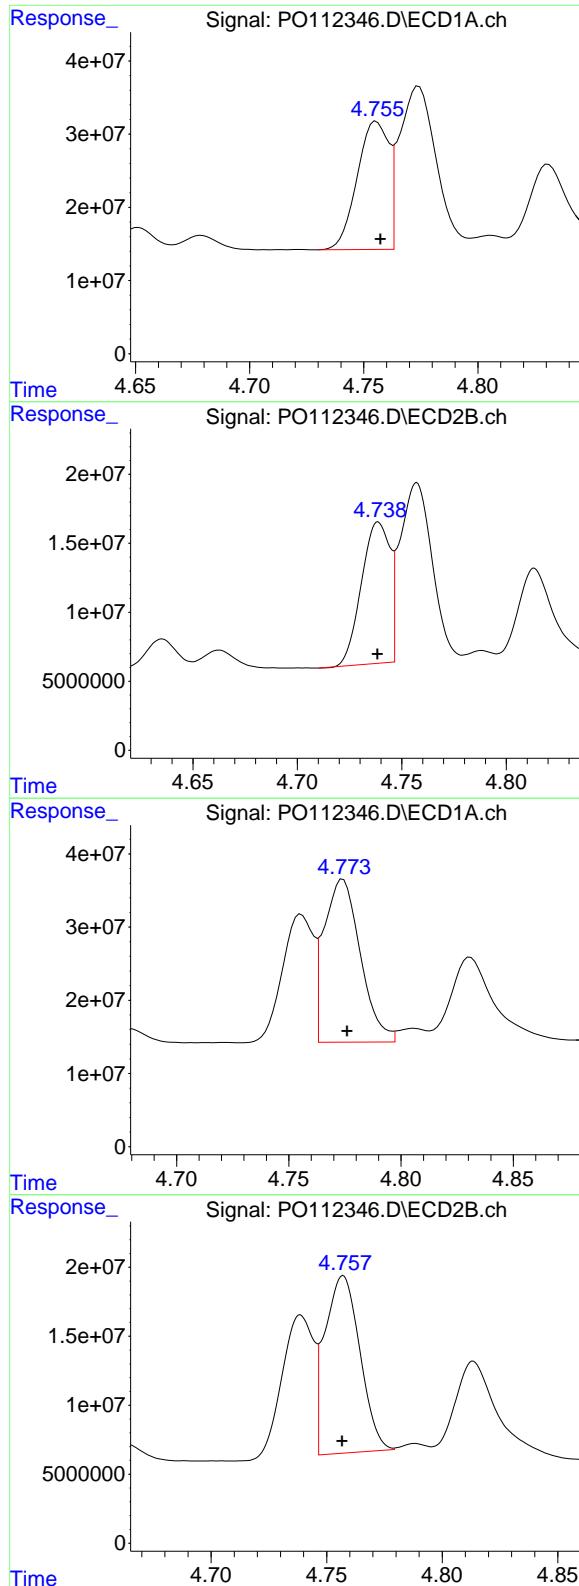

#3 AR-1016-1

R.T.: 4.755 min
 Delta R.T.: -0.002 min
 Response: 167749009
 Conc: 493.20 ng/ml

Instrument: ECD_O
 ClientSampleId: AR1660CCC500

#3 AR-1016-1


R.T.: 4.739 min
 Delta R.T.: 0.000 min
 Response: 97218771
 Conc: 436.28 ng/ml

#4 AR-1016-2

R.T.: 4.774 min
 Delta R.T.: -0.002 min
 Response: 250880622
 Conc: 504.49 ng/ml

#4 AR-1016-2

R.T.: 4.757 min
 Delta R.T.: 0.000 min
 Response: 135301146
 Conc: 411.13 ng/ml

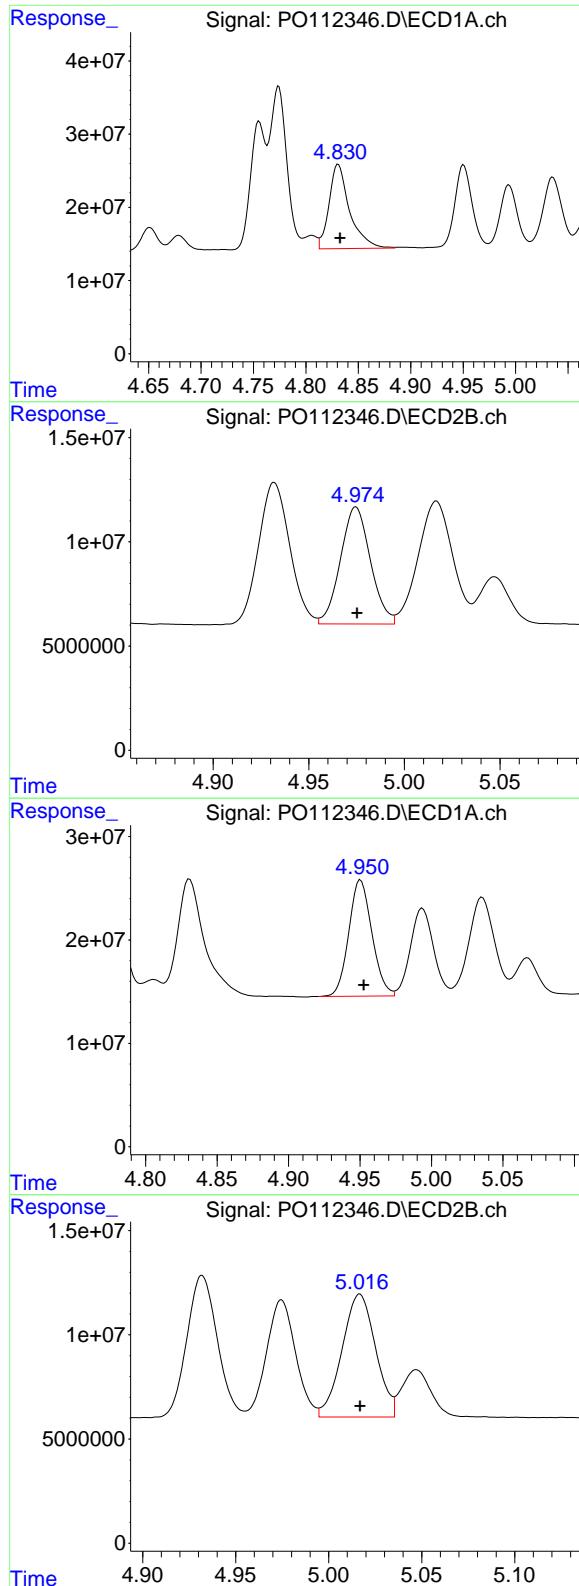

#5 AR-1016-3

R.T.: 4.831 min
 Delta R.T.: -0.002 min
 Response: 157194927
 Conc: 485.60 ng/ml

Instrument: ECD_O
 ClientSampleId: AR1660CCC500

#5 AR-1016-3


R.T.: 4.975 min
 Delta R.T.: 0.000 min
 Response: 61302098
 Conc: 360.88 ng/ml

#6 AR-1016-4

R.T.: 4.950 min
 Delta R.T.: -0.002 min
 Response: 126988725
 Conc: 494.51 ng/ml

#6 AR-1016-4

R.T.: 5.017 min
 Delta R.T.: 0.000 min
 Response: 74044940
 Conc: 539.58 ng/ml

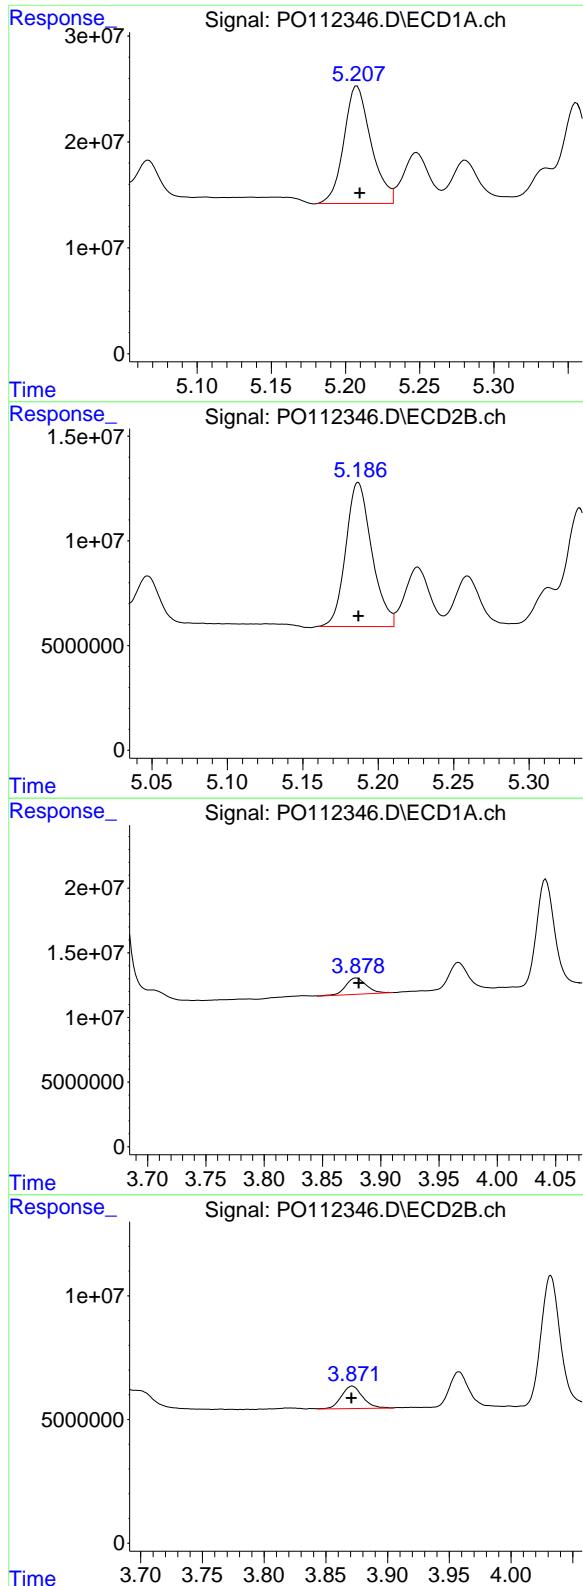

#7 AR-1016-5

R.T.: 5.208 min
 Delta R.T.: -0.002 min
 Response: 141516499
 Conc: 517.12 ng/ml

Instrument: ECD_O
 ClientSampleId: AR1660CCC500

#7 AR-1016-5


R.T.: 5.187 min
 Delta R.T.: 0.000 min
 Response: 82476996
 Conc: 478.27 ng/ml

#8 AR-1221-1

R.T.: 3.879 min
 Delta R.T.: -0.002 min
 Response: 15722840
 Conc: 134.83 ng/ml

#8 AR-1221-1


R.T.: 3.871 min
 Delta R.T.: 0.000 min
 Response: 10860941
 Conc: 131.98 ng/ml

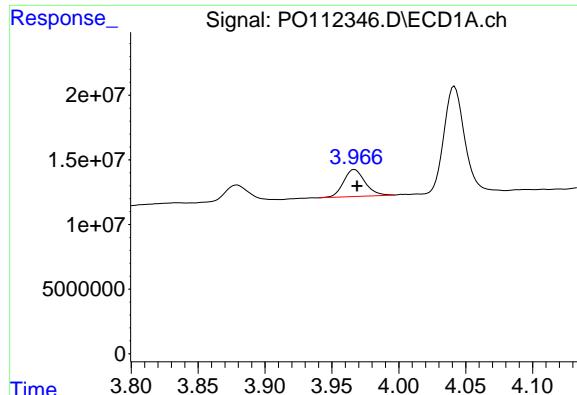

#9 AR-1221-2


R.T.: 3.967 min
Delta R.T.: -0.002 min
Response: 23372962
Conc: 296.46 ng/ml

Instrument: ECD_O
ClientSampleId: AR1660CCC500

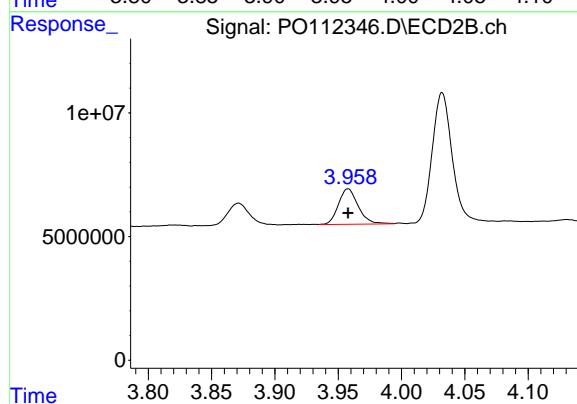


#9 AR-1221-2

R.T.: 3.958 min
Delta R.T.: 0.000 min
Response: 15634060
Conc: 263.41 ng/ml

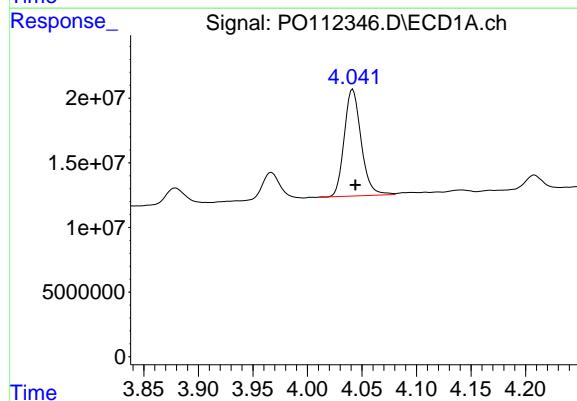


#10 AR-1221-3

R.T.: 4.042 min
Delta R.T.: -0.002 min
Response: 89050131
Conc: 330.33 ng/ml

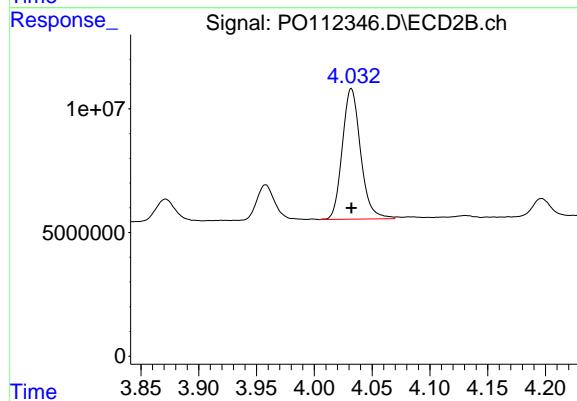

#10 AR-1221-3

R.T.: 4.032 min
Delta R.T.: 0.000 min
Response: 57995386
Conc: 307.22 ng/ml

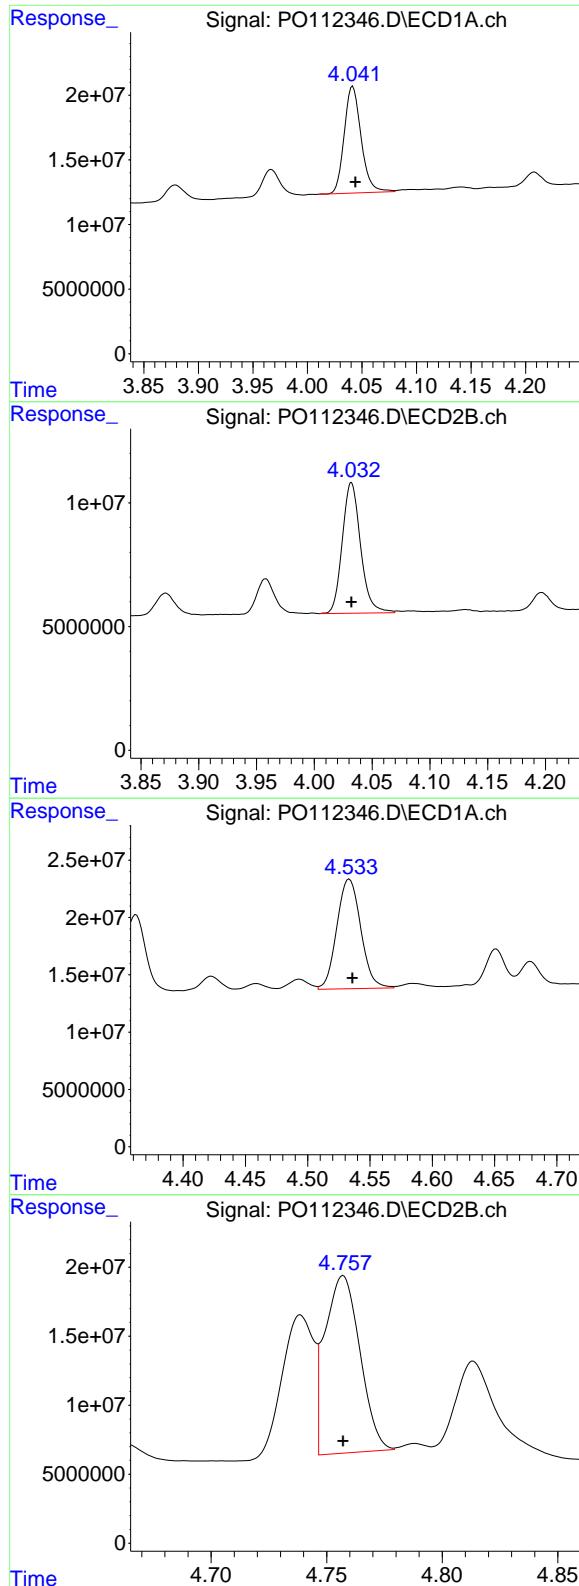

#11 AR-1232-1

R.T.: 4.042 min
 Delta R.T.: -0.002 min
 Response: 89050131
 Conc: 414.83 ng/ml

Instrument: ECD_O
 ClientSampleId: AR1660CCC500

#11 AR-1232-1


R.T.: 4.032 min
 Delta R.T.: 0.000 min
 Response: 57995386
 Conc: 386.38 ng/ml

#12 AR-1232-2

R.T.: 4.533 min
 Delta R.T.: -0.002 min
 Response: 128392006
 Conc: 1129.84 ng/ml


#12 AR-1232-2

R.T.: 4.757 min
 Delta R.T.: 0.000 min
 Response: 135301146
 Conc: 883.83 ng/ml

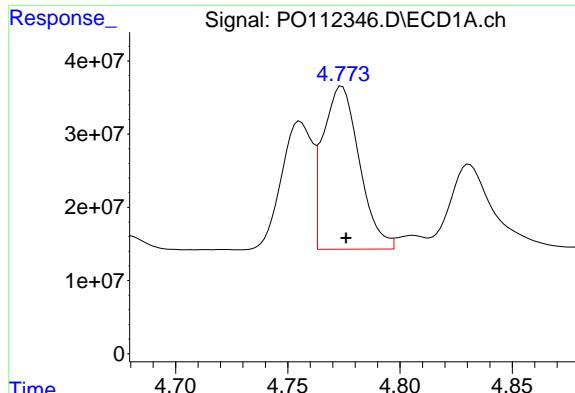


#13 AR-1232-3

R.T.: 4.774 min
 Delta R.T.: -0.002 min
 Response: 250880622
 Conc: 1095.51 ng/ml
Instrument:
 ECD_O
ClientSampleId :
 AR1660CCC500

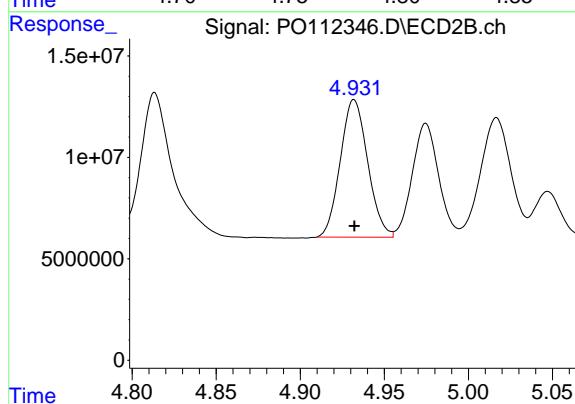


#13 AR-1232-3

R.T.: 4.932 min
 Delta R.T.: 0.000 min
 Response: 76865187
 Conc: 1018.00 ng/ml

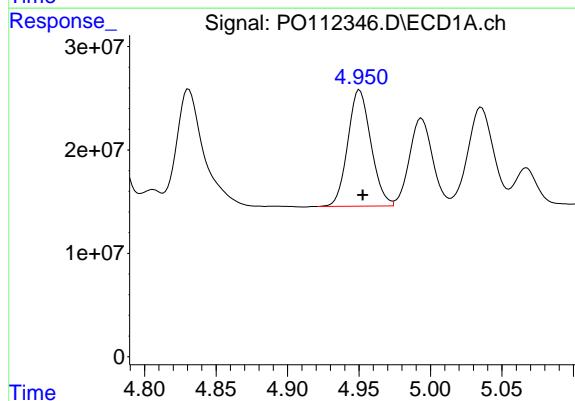


#14 AR-1232-4

R.T.: 4.950 min
 Delta R.T.: -0.002 min
 Response: 126988725
 Conc: 1111.04 ng/ml

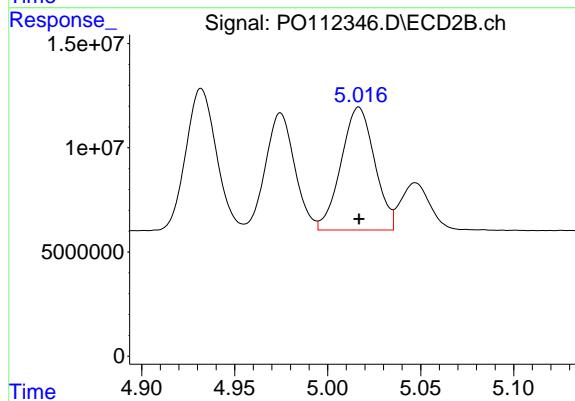


#14 AR-1232-4

R.T.: 5.017 min
 Delta R.T.: 0.000 min
 Response: 74044940
 Conc: 1122.09 ng/ml

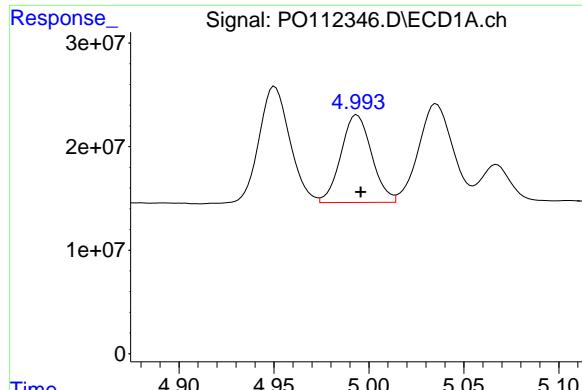


#15 AR-1232-5

R.T.: 4.994 min
 Delta R.T.: -0.002 min
 Response: 95361665
 Conc: 1299.20 ng/ml
Instrument: ECD_O
ClientSampleId : AR1660CCC500

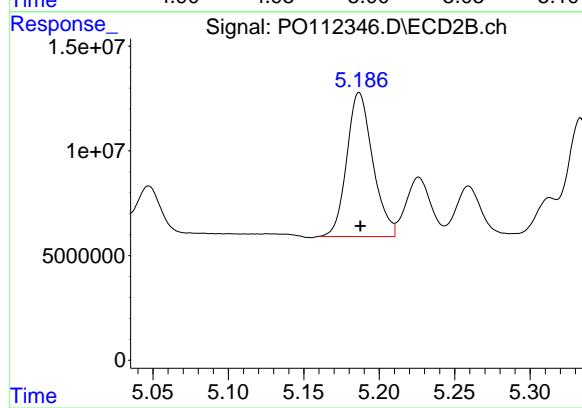


#15 AR-1232-5

R.T.: 5.187 min
 Delta R.T.: 0.000 min
 Response: 82476996
 Conc: 1110.65 ng/ml

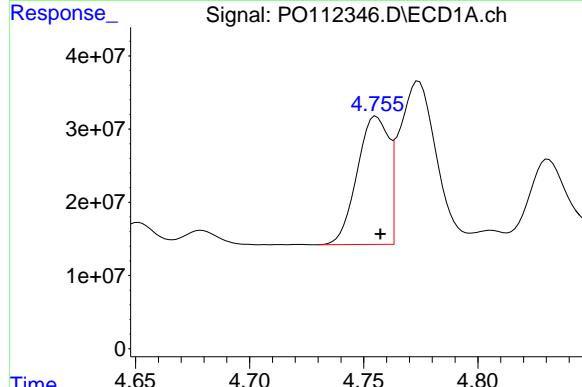


#16 AR-1242-1

R.T.: 4.755 min
 Delta R.T.: -0.002 min
 Response: 167749009
 Conc: 579.17 ng/ml

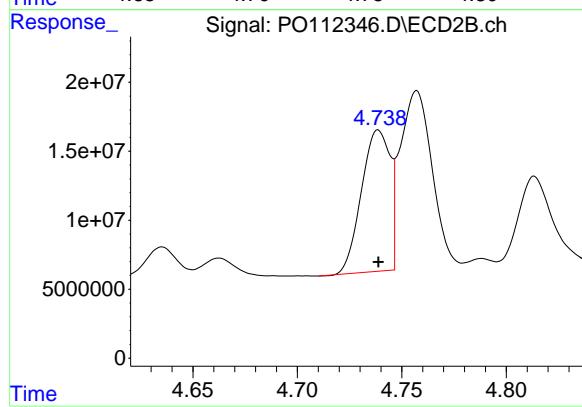

#16 AR-1242-1


R.T.: 4.739 min
 Delta R.T.: 0.000 min
 Response: 97218771
 Conc: 501.49 ng/ml



#17 AR-1242-2


R.T.: 4.774 min
 Delta R.T.: -0.002 min
 Response: 250880622
 Conc: 589.03 ng/ml

Instrument: ECD_O
 ClientSampleId: AR1660CCC500

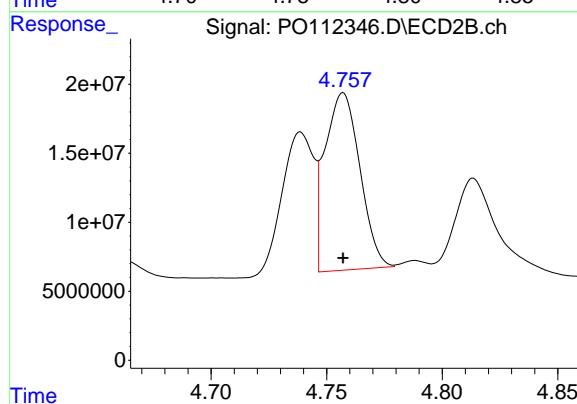


#17 AR-1242-2

R.T.: 4.757 min
 Delta R.T.: 0.000 min
 Response: 135301146
 Conc: 477.50 ng/ml

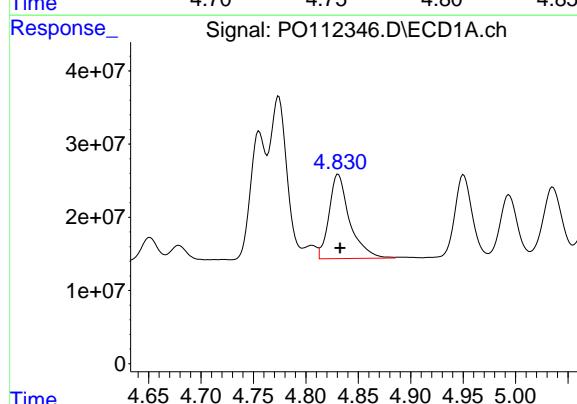


#18 AR-1242-3

R.T.: 4.831 min
 Delta R.T.: -0.002 min
 Response: 157194927
 Conc: 574.36 ng/ml

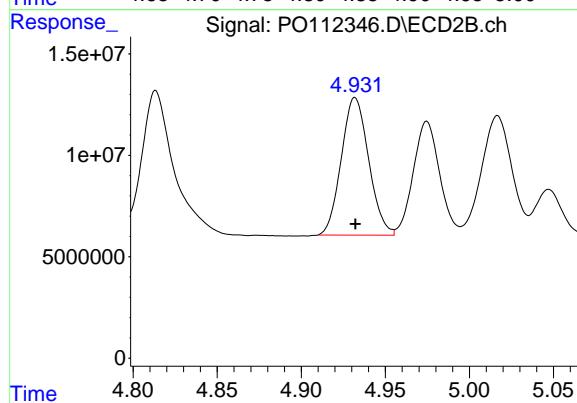

#18 AR-1242-3

R.T.: 4.932 min
 Delta R.T.: 0.000 min
 Response: 76865187
 Conc: 527.64 ng/ml

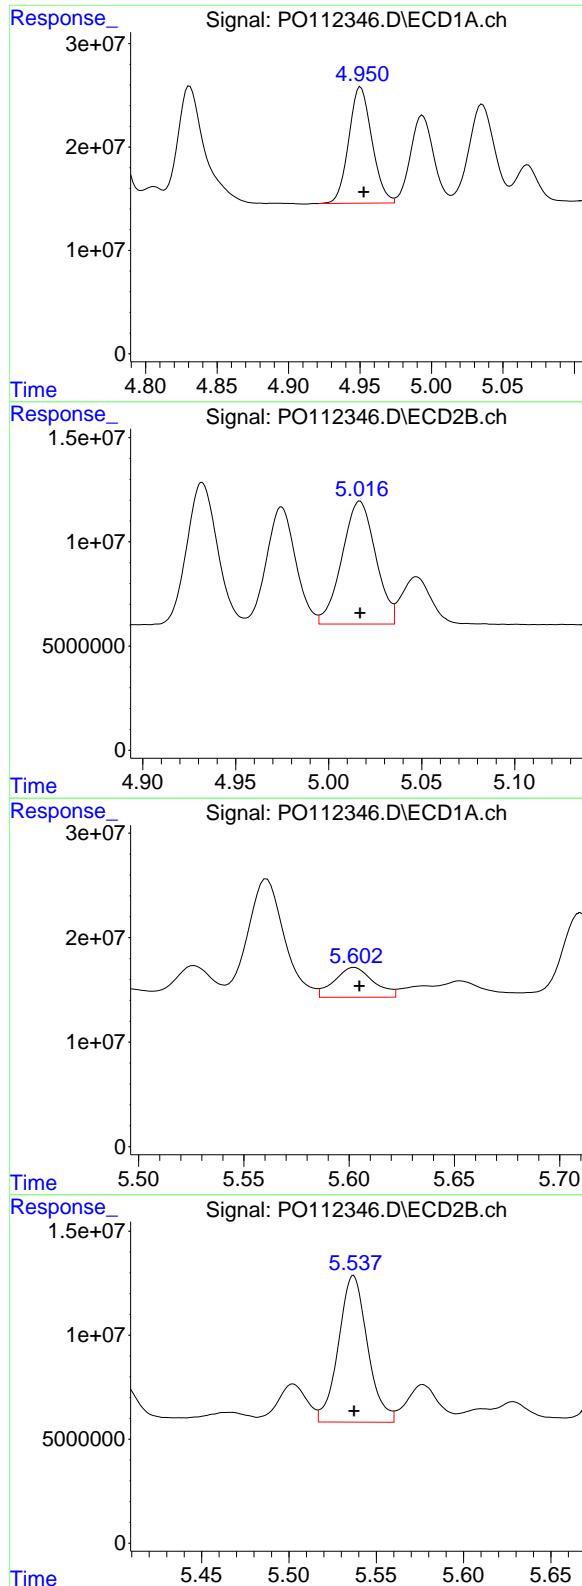

#19 AR-1242-4

R.T.: 4.950 min
 Delta R.T.: -0.002 min
 Response: 126988725
 Conc: 563.60 ng/ml

Instrument: ECD_O
 ClientSampleId: AR1660CCC500

#19 AR-1242-4


R.T.: 5.017 min
 Delta R.T.: 0.000 min
 Response: 74044940
 Conc: 522.03 ng/ml

#20 AR-1242-5

R.T.: 5.603 min
 Delta R.T.: -0.002 min
 Response: 36994145
 Conc: 174.77 ng/ml

#20 AR-1242-5


R.T.: 5.537 min
 Delta R.T.: 0.000 min
 Response: 81589337
 Conc: 448.95 ng/ml

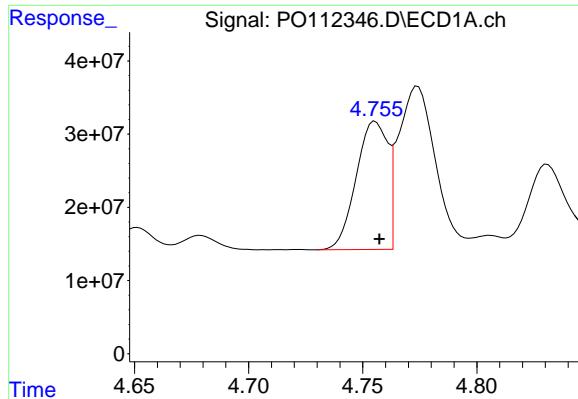

#21 AR-1248-1


R.T.: 4.755 min
 Delta R.T.: -0.002 min
 Response: 167749009
 Conc: 739.31 ng/ml

Instrument: ECD_O
 ClientSampleId: AR1660CCC500

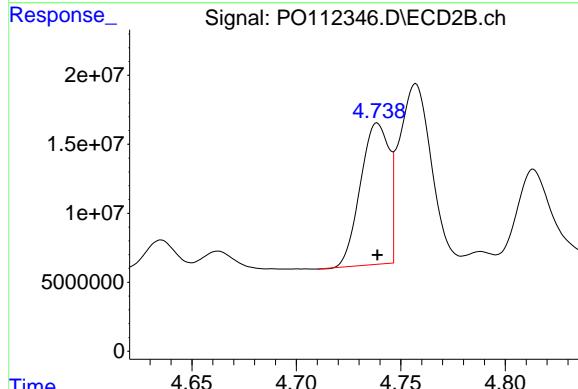


#21 AR-1248-1

R.T.: 4.739 min
 Delta R.T.: 0.000 min
 Response: 97218771
 Conc: 629.79 ng/ml

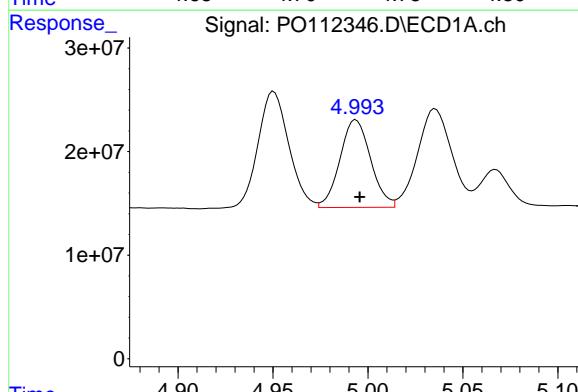


#22 AR-1248-2

R.T.: 4.994 min
 Delta R.T.: -0.002 min
 Response: 95361665
 Conc: 309.29 ng/ml

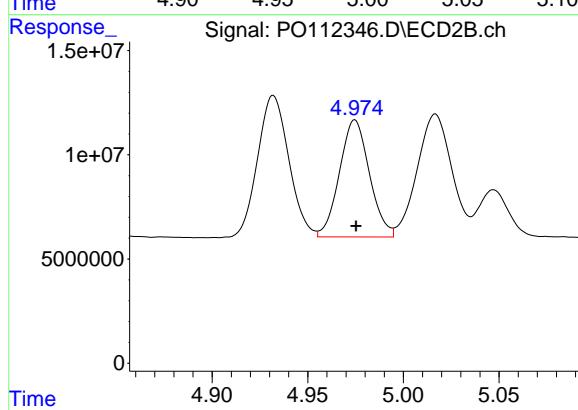

#22 AR-1248-2

R.T.: 4.975 min
 Delta R.T.: 0.000 min
 Response: 61302098
 Conc: 297.92 ng/ml

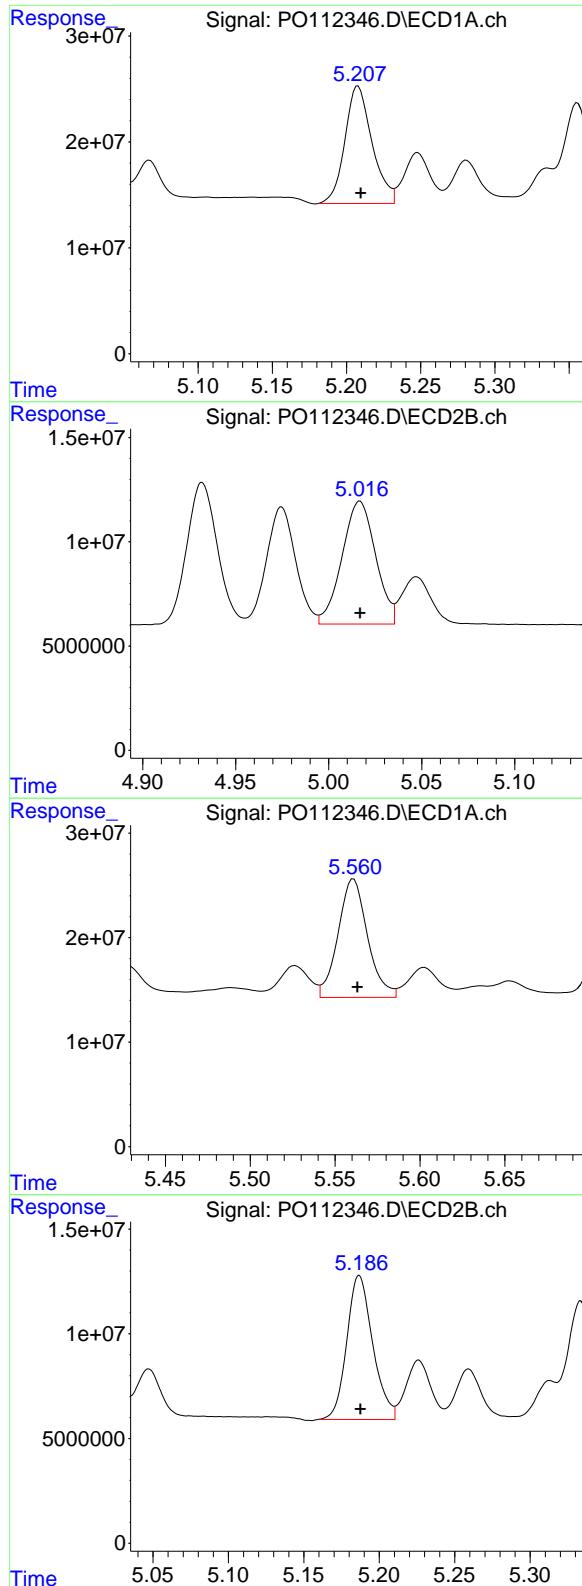

#23 AR-1248-3

R.T.: 5.208 min
 Delta R.T.: -0.002 min
 Response: 141516499
 Conc: 347.43 ng/ml

Instrument: ECD_O
 ClientSampleId: AR1660CCC500

#23 AR-1248-3


R.T.: 5.017 min
 Delta R.T.: 0.000 min
 Response: 74044940
 Conc: 344.72 ng/ml

#24 AR-1248-4

R.T.: 5.561 min
 Delta R.T.: -0.002 min
 Response: 136870190
 Conc: 237.15 ng/ml

#24 AR-1248-4

R.T.: 5.187 min
 Delta R.T.: 0.000 min
 Response: 82476996
 Conc: 318.78 ng/ml

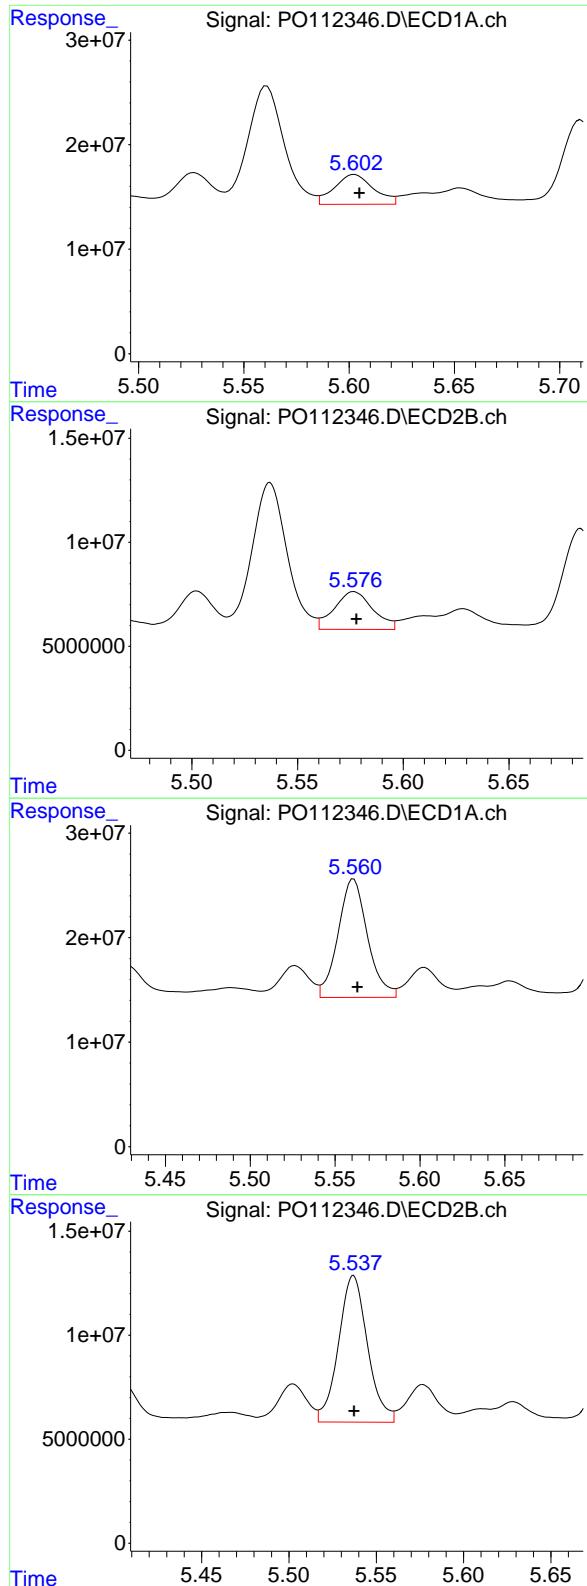

#25 AR-1248-5

R.T.: 5.603 min
 Delta R.T.: -0.002 min
 Response: 36994145
 Conc: 94.78 ng/ml

Instrument: ECD_O
ClientSampleId: AR1660CCC500

#25 AR-1248-5


R.T.: 5.577 min
 Delta R.T.: -0.001 min
 Response: 23078382
 Conc: 92.11 ng/ml

#26 AR-1254-1

R.T.: 5.561 min
 Delta R.T.: -0.002 min
 Response: 136870190
 Conc: 222.51 ng/ml

#26 AR-1254-1


R.T.: 5.537 min
 Delta R.T.: 0.000 min
 Response: 81589337
 Conc: 214.05 ng/ml

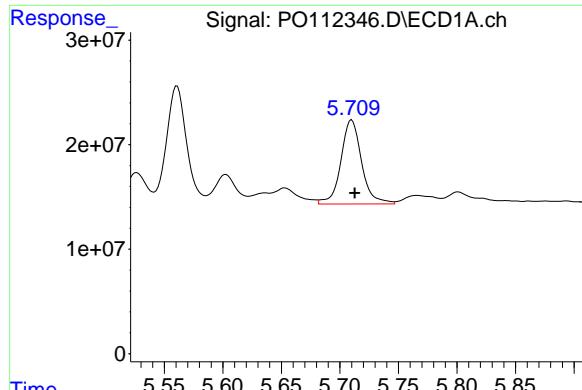

#27 AR-1254-2


R.T.: 5.710 min
Delta R.T.: -0.003 min
Response: 99169571
Conc: 185.13 ng/ml

Instrument: ECD_O
ClientSampleId: AR1660CCC500

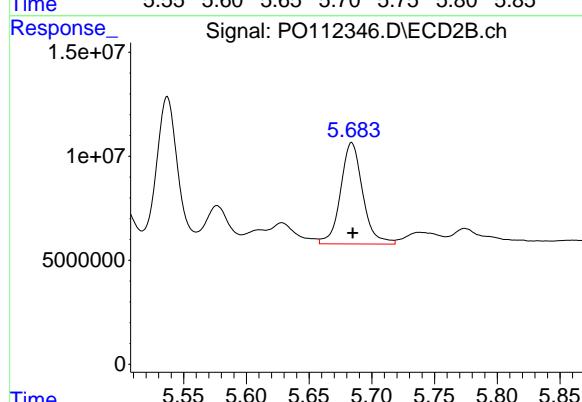


#27 AR-1254-2

R.T.: 5.684 min
Delta R.T.: 0.000 min
Response: 59758329
Conc: 180.10 ng/ml

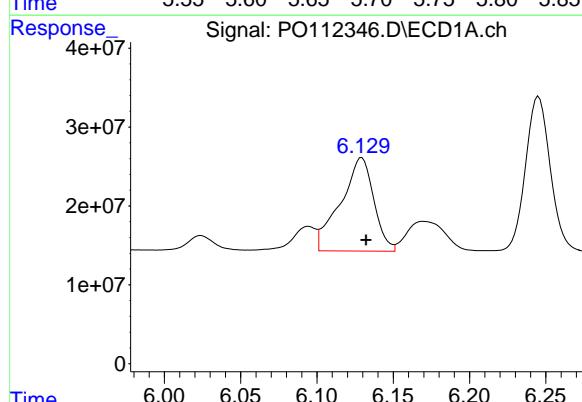


#28 AR-1254-3

R.T.: 6.129 min
Delta R.T.: -0.003 min
Response: 179626589
Conc: 213.95 ng/ml

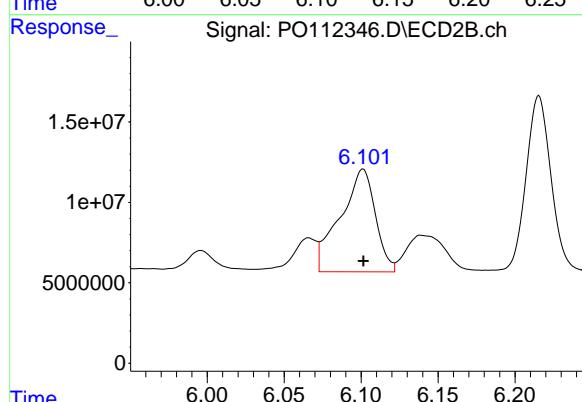

#28 AR-1254-3

R.T.: 6.101 min
Delta R.T.: 0.000 min
Response: 101248832
Conc: 210.04 ng/ml

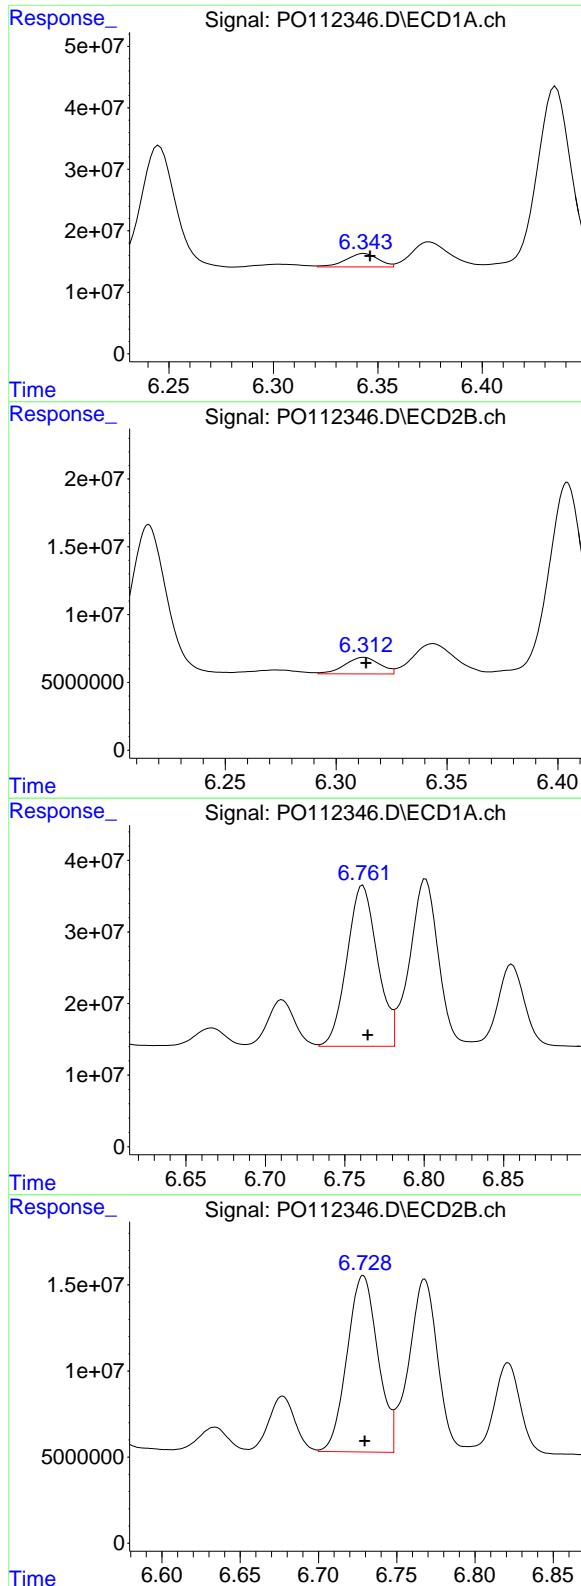

#29 AR-1254-4

R.T.: 6.344 min
 Delta R.T.: -0.003 min
 Response: 23749159
 Conc: 49.37 ng/ml

Instrument: ECD_O
 ClientSampleId: AR1660CCC500

#29 AR-1254-4


R.T.: 6.312 min
 Delta R.T.: 0.000 min
 Response: 13372256
 Conc: 51.29 ng/ml

#30 AR-1254-5

R.T.: 6.761 min
 Delta R.T.: -0.003 min
 Response: 300030747
 Conc: 387.66 ng/ml

#30 AR-1254-5


R.T.: 6.729 min
 Delta R.T.: -0.001 min
 Response: 140333264
 Conc: 393.80 ng/ml

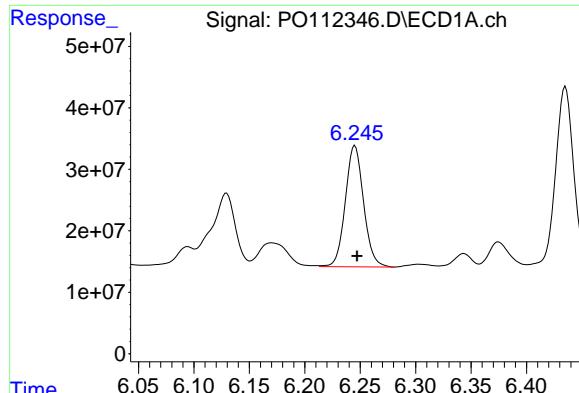

#31 AR-1260-1


R.T.: 6.245 min
 Delta R.T.: -0.002 min
 Response: 225996595
 Conc: 450.88 ng/ml

Instrument: ECD_O
 ClientSampleId: AR1660CCC500

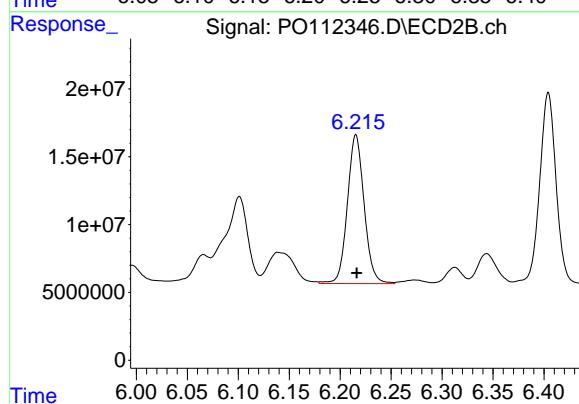


#31 AR-1260-1

R.T.: 6.215 min
 Delta R.T.: 0.000 min
 Response: 125625189
 Conc: 447.76 ng/ml

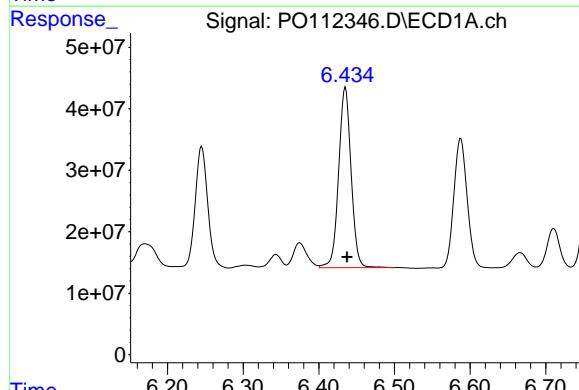


#32 AR-1260-2

R.T.: 6.435 min
 Delta R.T.: -0.002 min
 Response: 335105953
 Conc: 453.99 ng/ml

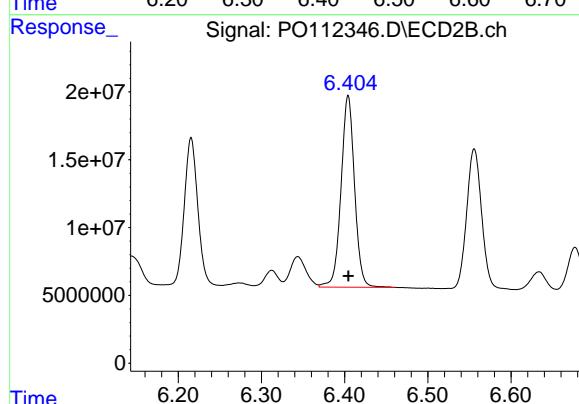


#32 AR-1260-2

R.T.: 6.404 min
 Delta R.T.: 0.000 min
 Response: 159139752
 Conc: 468.06 ng/ml




#33 AR-1260-3

R.T.: 6.801 min
 Delta R.T.: -0.003 min
Instrument:
 Response: 294448405 ECD_O
 Conc: 449.21 ng/ml ClientSampleId :
 AR1660CCC500

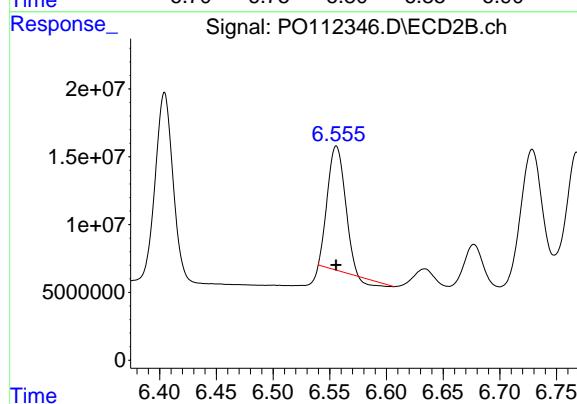


#33 AR-1260-3

R.T.: 6.556 min
 Delta R.T.: 0.000 min
 Response: 95203208
 Conc: 345.46 ng/ml

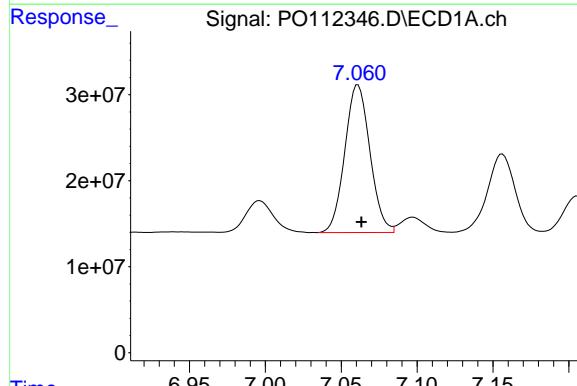


#34 AR-1260-4

R.T.: 7.061 min
 Delta R.T.: -0.002 min
 Response: 198088517
 Conc: 455.12 ng/ml

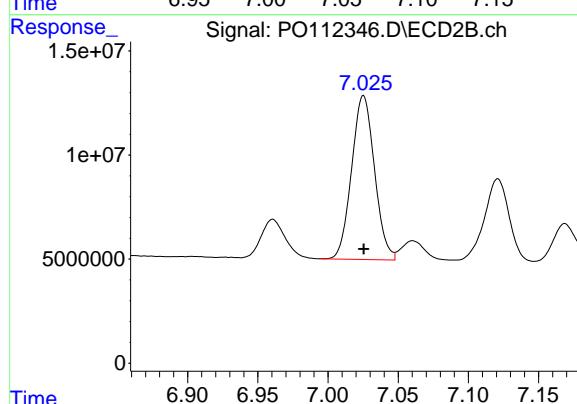

#34 AR-1260-4

R.T.: 7.025 min
 Delta R.T.: 0.000 min
 Response: 89511018
 Conc: 446.12 ng/ml

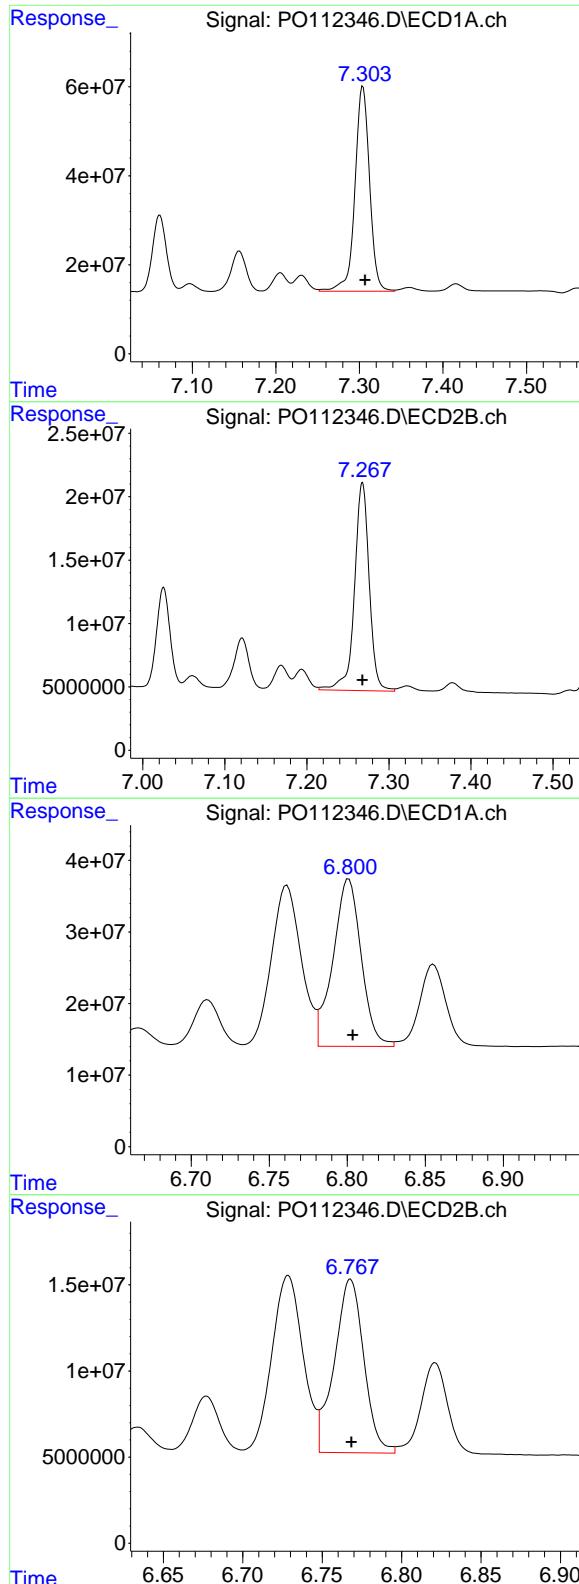

#35 AR-1260-5

R.T.: 7.304 min
 Delta R.T.: -0.003 min
 Response: 561793030
 Conc: 444.97 ng/ml

Instrument: ECD_O
 ClientSampleId: AR1660CCC500

#35 AR-1260-5


R.T.: 7.268 min
 Delta R.T.: 0.000 min
 Response: 205537159
 Conc: 459.07 ng/ml

#36 AR-1262-1

R.T.: 6.801 min
 Delta R.T.: -0.003 min
 Response: 294448405
 Conc: 288.20 ng/ml

#36 AR-1262-1

R.T.: 6.768 min
 Delta R.T.: 0.000 min
 Response: 130381288
 Conc: 320.09 ng/ml

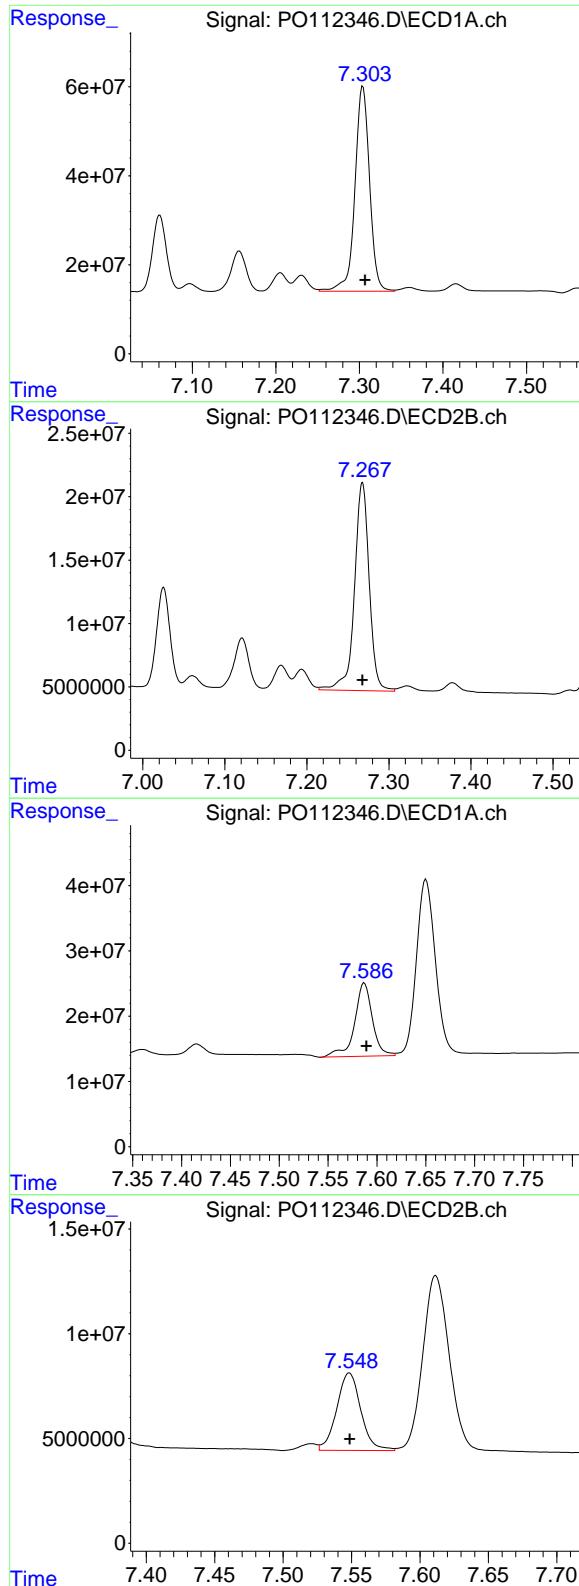

#37 AR-1262-2

R.T.: 7.304 min
 Delta R.T.: -0.003 min
 Response: 561793030
 Conc: 342.69 ng/ml

Instrument: ECD_O
 ClientSampleId: AR1660CCC500

#37 AR-1262-2


R.T.: 7.268 min
 Delta R.T.: 0.000 min
 Response: 205537159
 Conc: 401.01 ng/ml

#38 AR-1262-3

R.T.: 7.587 min
 Delta R.T.: -0.002 min
 Response: 142792840
 Conc: 222.43 ng/ml

#38 AR-1262-3

R.T.: 7.548 min
 Delta R.T.: 0.000 min
 Response: 45395147
 Conc: 252.86 ng/ml

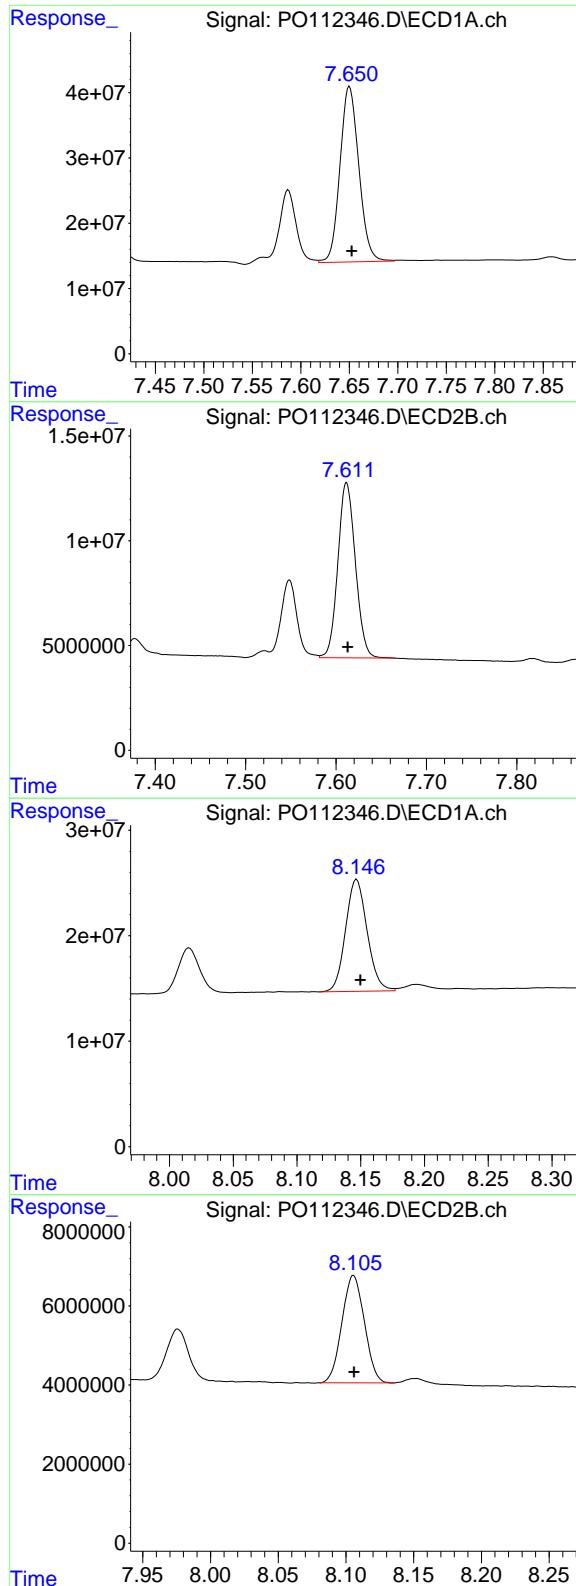

#39 AR-1262-4

R.T.: 7.650 min
 Delta R.T.: -0.002 min
 Response: 364244563
 Conc: 339.96 ng/ml

Instrument: ECD_O
ClientSampleId: AR1660CCC500

#39 AR-1262-4


R.T.: 7.612 min
 Delta R.T.: -0.001 min
 Response: 112708159
 Conc: 387.42 ng/ml

#40 AR-1262-5

R.T.: 8.147 min
 Delta R.T.: -0.003 min
 Response: 125023184
 Conc: 278.98 ng/ml

#40 AR-1262-5

R.T.: 8.106 min
 Delta R.T.: 0.000 min
 Response: 31357784
 Conc: 296.43 ng/ml

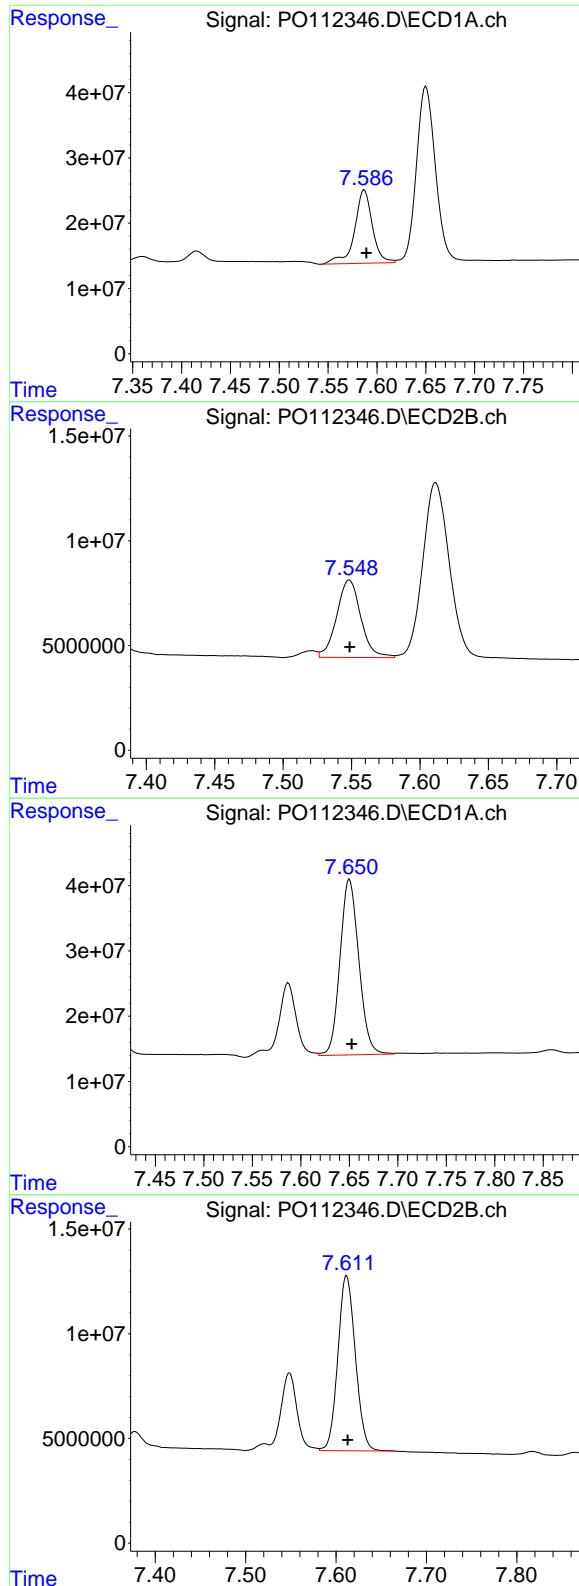

#41 AR-1268-1

R.T.: 7.587 min
 Delta R.T.: -0.002 min
 Response: 142792840
 Conc: 77.71 ng/ml

Instrument: ECD_O
ClientSampleId: AR1660CCC500

#41 AR-1268-1


R.T.: 7.548 min
 Delta R.T.: 0.000 min
 Response: 45395147
 Conc: 92.37 ng/ml

#42 AR-1268-2

R.T.: 7.650 min
 Delta R.T.: -0.002 min
 Response: 364244563
 Conc: 233.85 ng/ml

#42 AR-1268-2

R.T.: 7.612 min
 Delta R.T.: -0.001 min
 Response: 112708159
 Conc: 270.16 ng/ml

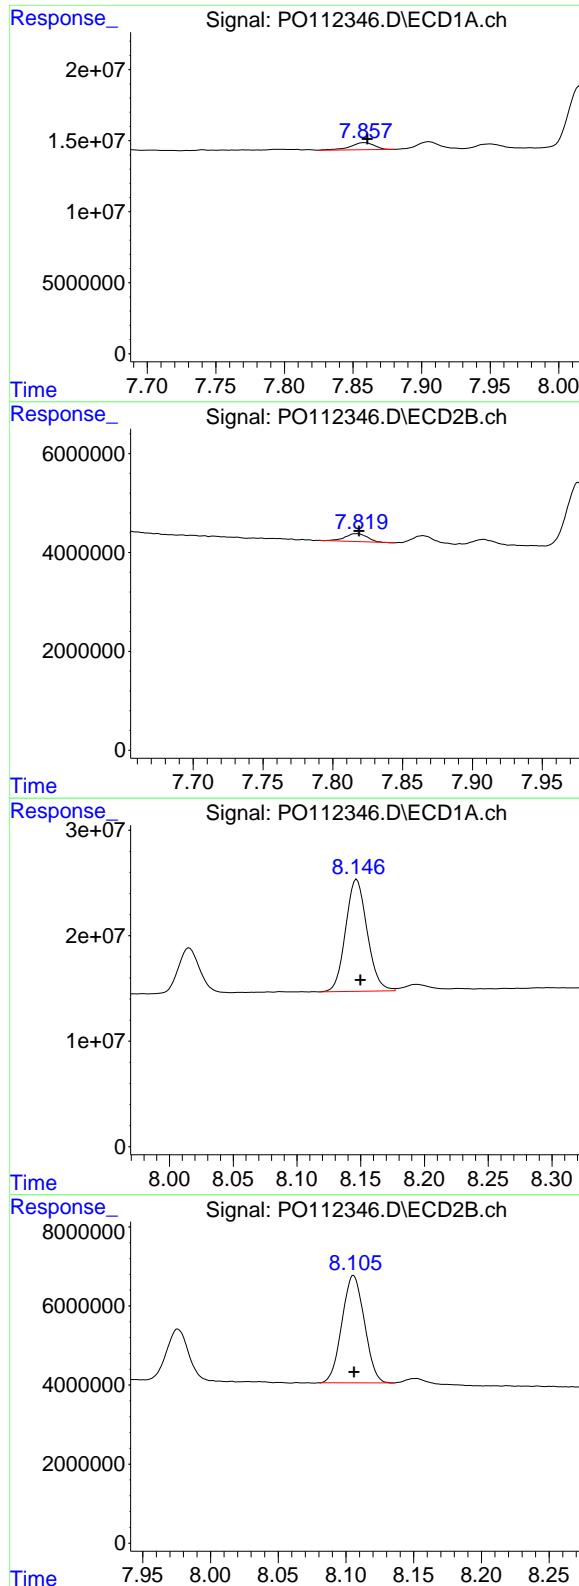

#43 AR-1268-3

R.T.: 7.858 min
 Delta R.T.: -0.002 min
 Response: 6022964
 Conc: 4.63 ng/ml

Instrument: ECD_O
ClientSampleId: AR1660CCC500

#43 AR-1268-3


R.T.: 7.817 min
 Delta R.T.: -0.002 min
 Response: 1789840
 Conc: 5.66 ng/ml

#44 AR-1268-4

R.T.: 8.147 min
 Delta R.T.: -0.003 min
 Response: 125023184
 Conc: 260.24 ng/ml

#44 AR-1268-4


R.T.: 8.106 min
 Delta R.T.: 0.000 min
 Response: 31357784
 Conc: 281.21 ng/ml

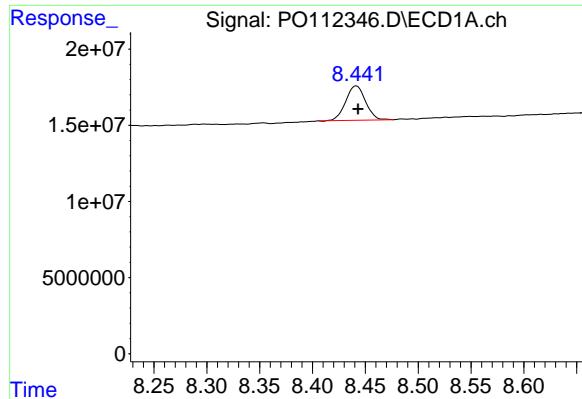

#45 AR-1268-5

R.T.: 8.442 min
Delta R.T.: -0.002 min
Response: 29486963
Conc: 9.03 ng/ml

Instrument: ECD_O
ClientSampleId: AR1660CCC500

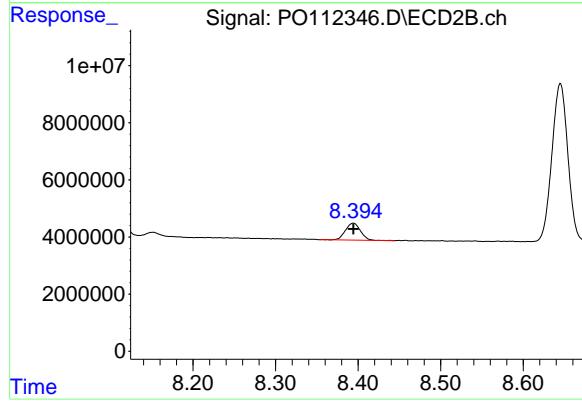

#45 AR-1268-5

R.T.: 8.394 min
Delta R.T.: 0.000 min
Response: 7543187
Conc: 10.38 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0072225\
 Data File : P0112366.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Jul 2025 08:57
 Operator : YP/AJ
 Sample : AR1660CCC500
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1660CCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 22 10:29:49 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 22 09:14:26 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	3.672	3.662	565.9E6	325.3E6	57.195	51.055
2) SA Decachlor...	8.700	8.691	341.7E6	64731	49.977	0.038 #

Target Compounds

3) L1 AR-1016-1	4.759	4.756	176.5E6	139.4E6	518.970	625.719
4) L1 AR-1016-2	4.778	4.787	264.8E6	2293532	532.518	6.969 #
5) L1 AR-1016-3	4.835	4.973	166.5E6	62926663	514.472	370.447 #
6) L1 AR-1016-4	4.954	5.015	134.2E6	75969252	522.411	553.601
7) L1 AR-1016-5	5.211	5.225	140.0E6	31986403	511.454	185.482 #
8) L2 AR-1221-1	3.883	3.869	17862403	11214221	153.176	136.269
9) L2 AR-1221-2	3.971	3.957	24509341	16486507	310.872	277.768
10) L2 AR-1221-3	4.045	4.031	94275348	60498897	349.710	320.479
11) L3 AR-1232-1	4.045	4.031	94275348	60498897	439.169	403.059
12) L3 AR-1232-2	4.538	4.756	137.6E6	139.4E6	1210.725	910.807
13) L3 AR-1232-3	4.778	4.931	264.8E6	77402062	1156.361	1025.111
14) L3 AR-1232-4	4.954	5.015	134.2E6	75969252	1173.744	1151.255
15) L3 AR-1232-5	4.997	5.185	104.6E6	83417066	1424.451	1123.312
16) L4 AR-1242-1	4.759	4.737	176.5E6	98386664	609.431	507.518
17) L4 AR-1242-2	4.778	4.756	264.8E6	139.4E6	621.754	492.079
18) L4 AR-1242-3	4.835	4.931	166.5E6	77402062	608.515	531.326
19) L4 AR-1242-4	4.954	5.015	134.2E6	75969252	595.403	535.596
20) L4 AR-1242-5	5.606	5.535	36092211	84564389	170.511	465.319 #
21) L5 AR-1248-1	4.759	4.737	176.5E6	98386664	777.937	637.351
22) L5 AR-1248-2	4.997	4.973	104.6E6	62926663	339.106	305.814
23) L5 AR-1248-3	5.211	5.015	140.0E6	75969252	343.625	353.677
24) L5 AR-1248-4	5.565	5.185	144.2E6	83417066	249.820	322.414 #
25) L5 AR-1248-5	5.606	5.575	36092211	22841188	92.472	91.164
26) L6 AR-1254-1	5.565	5.535	144.2E6	84564389	234.400	221.856
27) L6 AR-1254-2	5.714	5.683	100.1E6	60270259	186.903	181.640
28) L6 AR-1254-3	6.134	6.100	198.2E6	109.0E6	236.105	226.131
29) L6 AR-1254-4	6.347	6.312	28382091	15522172	59.004	59.542
30) L6 AR-1254-5	6.765	6.727	332.9E6	156.0E6	430.103	437.799
31) L7 AR-1260-1	6.249	6.214	247.5E6	135.5E6	493.782	482.798
32) L7 AR-1260-2	6.439	6.403	365.4E6	175.0E6	495.002	514.627
33) L7 AR-1260-3	6.805	6.555	327.9E6	91053432	500.210	330.399 #
34) L7 AR-1260-4	7.064	7.060	219.2E6	12369917	503.511	61.651 #
35) L7 AR-1260-5	7.307	7.267	613.9E6	232.7E6	486.246	519.751
36) L8 AR-1262-1	6.805	6.767	327.9E6	147.1E6	320.919	361.097
37) L8 AR-1262-2	7.307	7.267	613.9E6	232.7E6	374.475	454.020
38) L8 AR-1262-3	7.591	7.548	145.7E6	49200657	226.955	274.062
39) L8 AR-1262-4	7.654	7.612	412.9E6	127.8E6	385.331	439.466
40) L8 AR-1262-5	8.151	8.105	139.2E6	35416682	310.521	334.803
41) L9 AR-1268-1	7.591	7.548	145.7E6	49200657	79.294	100.112 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0072225\
 Data File : P0112366.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Jul 2025 08:57
 Operator : YP/AJ
 Sample : AR1660CCC500
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1660CCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 22 10:29:49 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 22 09:14:26 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9 AR-1268-2	7.654	7.612	412.9E6	127.8E6	265.059	306.456
43) L9 AR-1268-3	7.861	7.816	6667277	2004613	5.130	6.336
44) L9 AR-1268-4	8.151	8.105	139.2E6	35416682	289.664	317.604
45) L9 AR-1268-5	8.444	8.392	32257747	8529469	9.884	11.740



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0072225\
 Data File : P0112366.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Jul 2025 08:57
 Operator : YP/AJ
 Sample : AR1660CCC500
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1660CCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 22 10:29:49 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 22 09:14:26 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

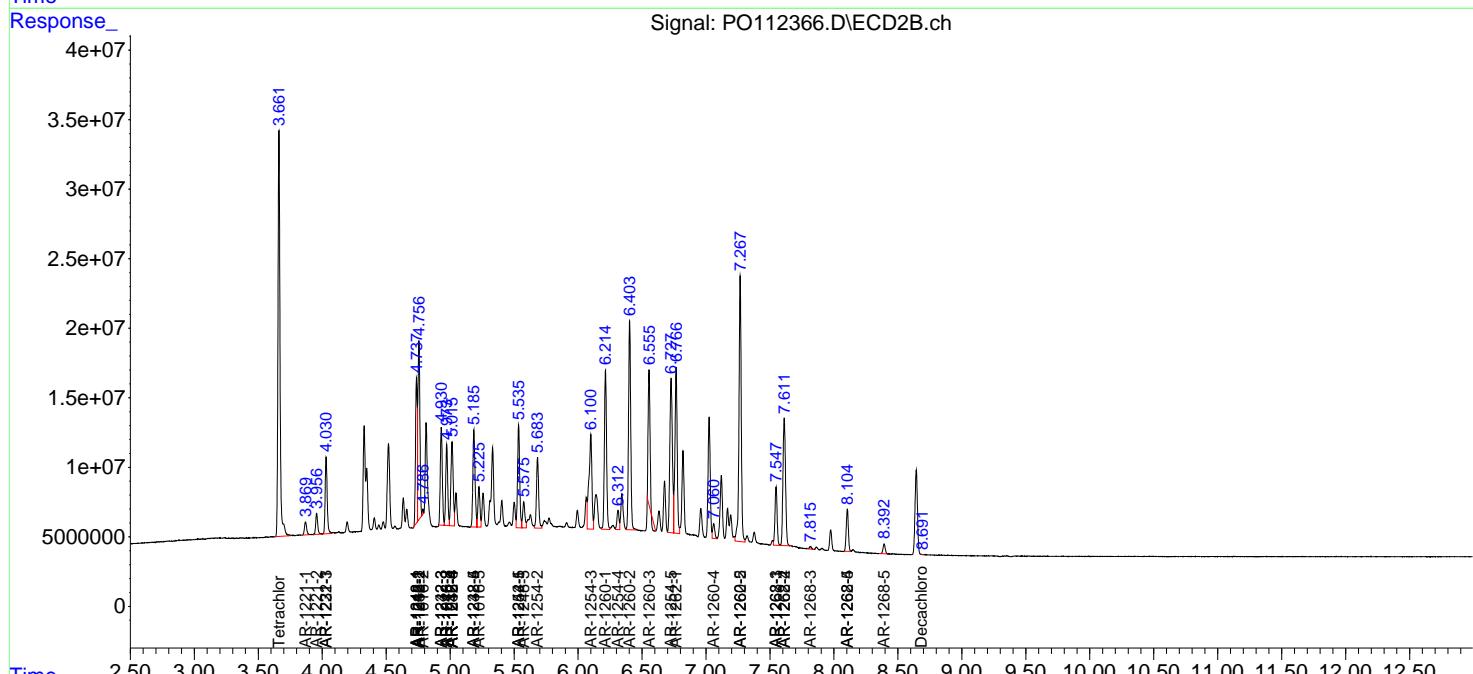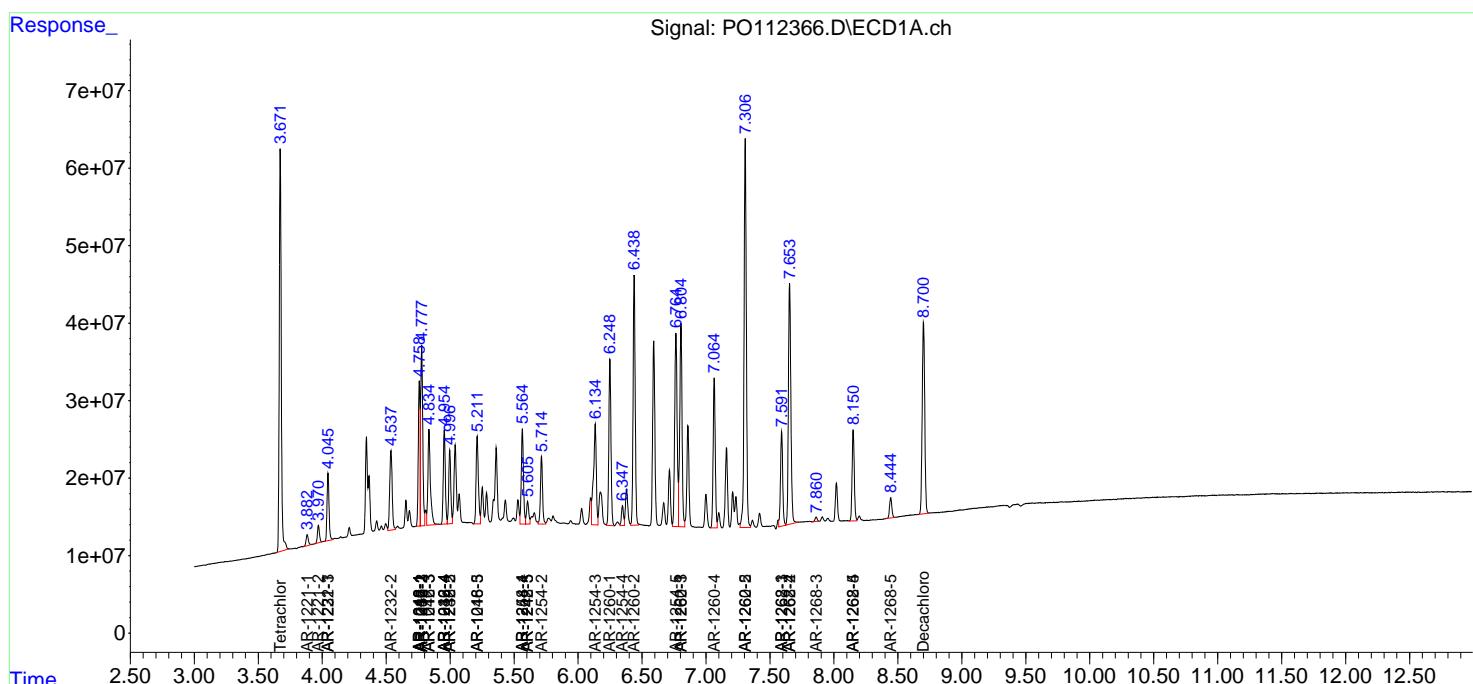

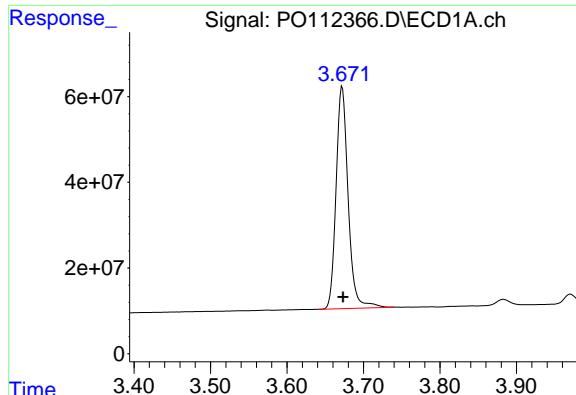

#1 Tetrachloro-m-xylene


R.T.: 3.672 min
Delta R.T.: 0.000 min
Response: 565932233
Conc: 57.20 ng/ml

Instrument:

ECD_O


ClientSampleId :

AR1660CCC500

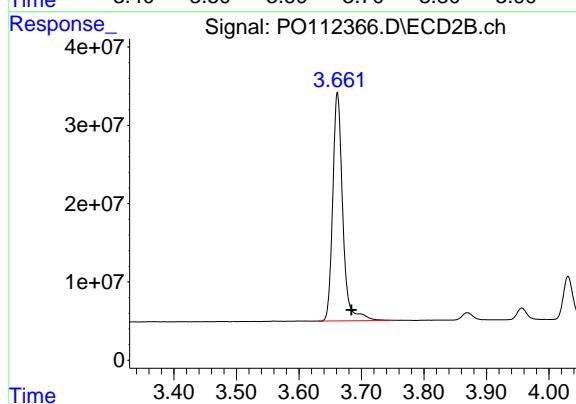


#1 Tetrachloro-m-xylene

R.T.: 3.662 min
Delta R.T.: -0.022 min
Response: 325275039
Conc: 51.06 ng/ml

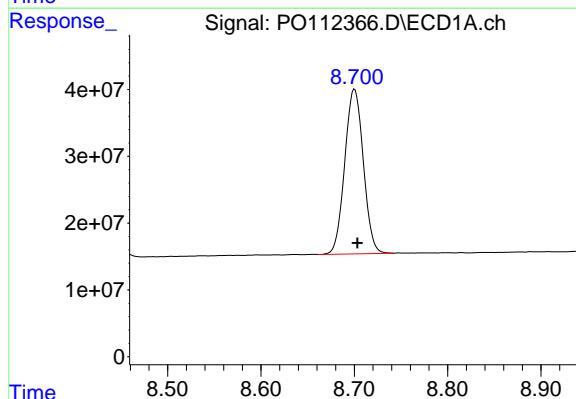


#2 Decachlorobiphenyl

R.T.: 8.700 min
Delta R.T.: -0.003 min
Response: 341696880
Conc: 49.98 ng/ml

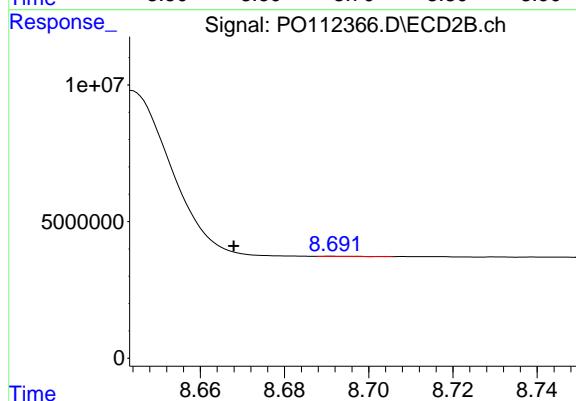

#2 Decachlorobiphenyl

R.T.: 8.691 min
Delta R.T.: 0.023 min
Response: 64731
Conc: 0.04 ng/ml

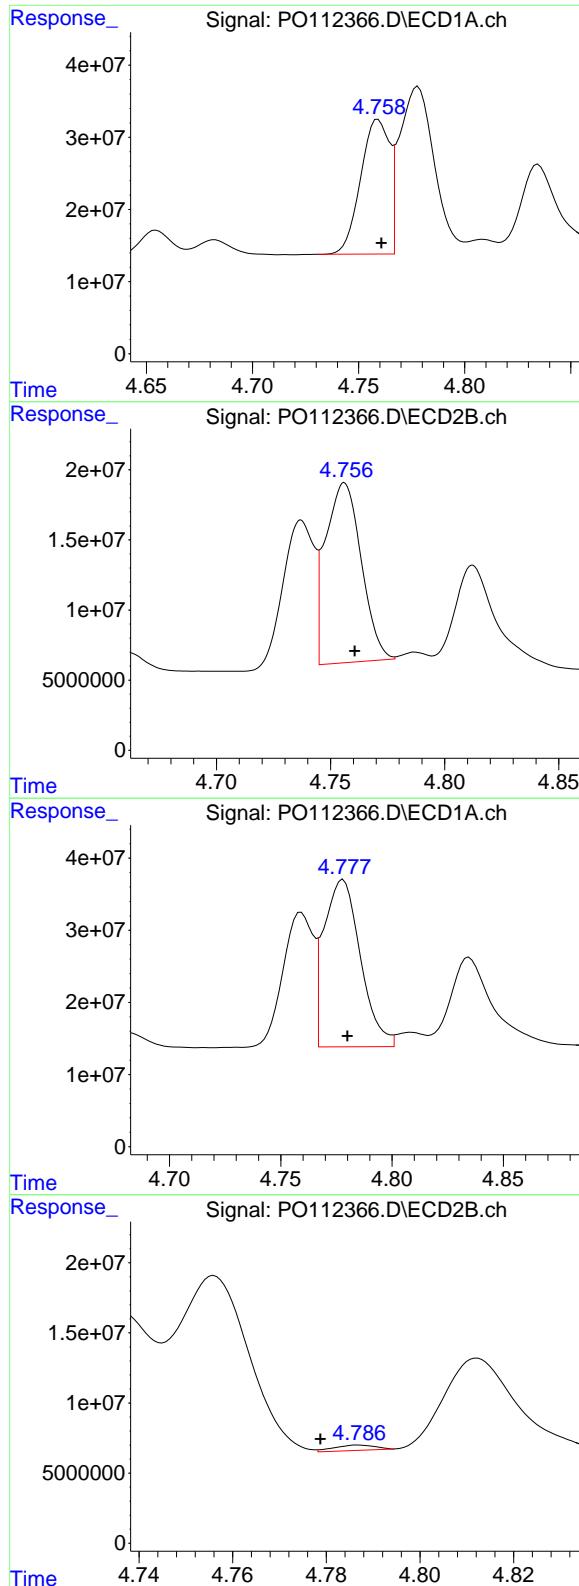

#3 AR-1016-1

R.T.: 4.759 min
 Delta R.T.: -0.002 min
 Response: 176513620
 Conc: 518.97 ng/ml

Instrument: ECD_O
 ClientSampleId: AR1660CCC500

#3 AR-1016-1


R.T.: 4.756 min
 Delta R.T.: -0.005 min
 Response: 139431612
 Conc: 625.72 ng/ml

#4 AR-1016-2

R.T.: 4.778 min
 Delta R.T.: -0.002 min
 Response: 264817007
 Conc: 532.52 ng/ml

#4 AR-1016-2

R.T.: 4.787 min
 Delta R.T.: 0.008 min
 Response: 2293532
 Conc: 6.97 ng/ml

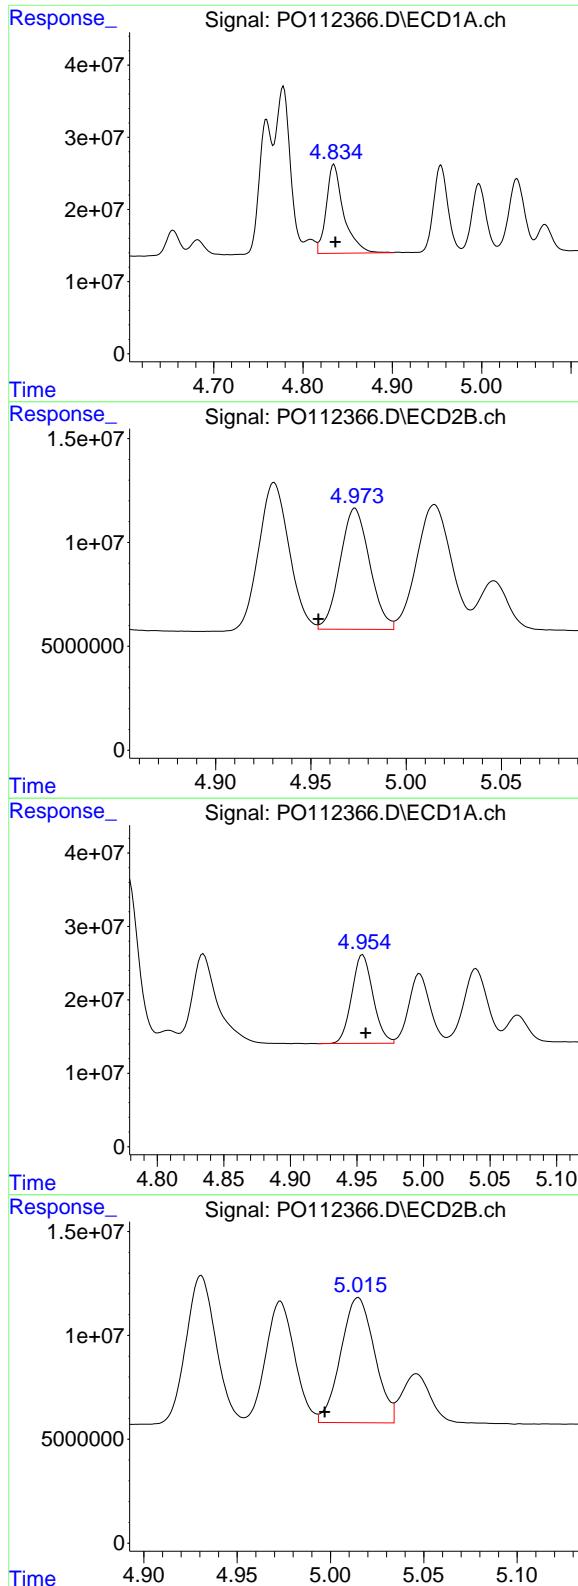

#5 AR-1016-3

R.T.: 4.835 min
 Delta R.T.: -0.002 min
 Response: 166541661
 Conc: 514.47 ng/ml

Instrument: ECD_O
 ClientSampleId: AR1660CCC500

#5 AR-1016-3


R.T.: 4.973 min
 Delta R.T.: 0.019 min
 Response: 62926663
 Conc: 370.45 ng/ml

#6 AR-1016-4

R.T.: 4.954 min
 Delta R.T.: -0.002 min
 Response: 134155056
 Conc: 522.41 ng/ml

#6 AR-1016-4

R.T.: 5.015 min
 Delta R.T.: 0.018 min
 Response: 75969252
 Conc: 553.60 ng/ml

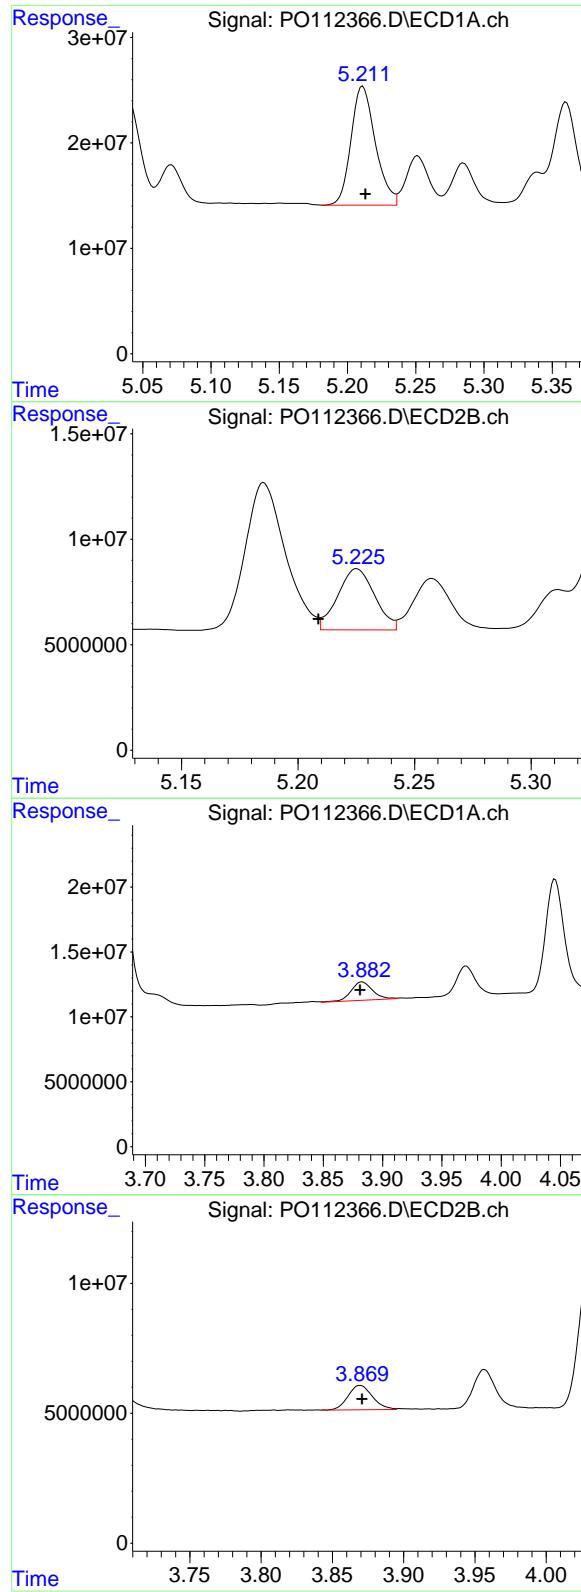

#7 AR-1016-5

R.T.: 5.211 min
Delta R.T.: -0.002 min
Response: 139965370
Conc: 511.45 ng/ml

#7 AR-1016-5


R.T.: 5.225 min
Delta R.T.: 0.016 min
Response: 31986403
Conc: 185.48 ng/ml

#8 AR-1221-1

R.T.: 3.883 min
Delta R.T.: 0.002 min
Response: 17862403
Conc: 153.18 ng/ml

#8 AR-1221-1

R.T.: 3.869 min
Delta R.T.: -0.001 min
Response: 11214221
Conc: 136.27 ng/ml

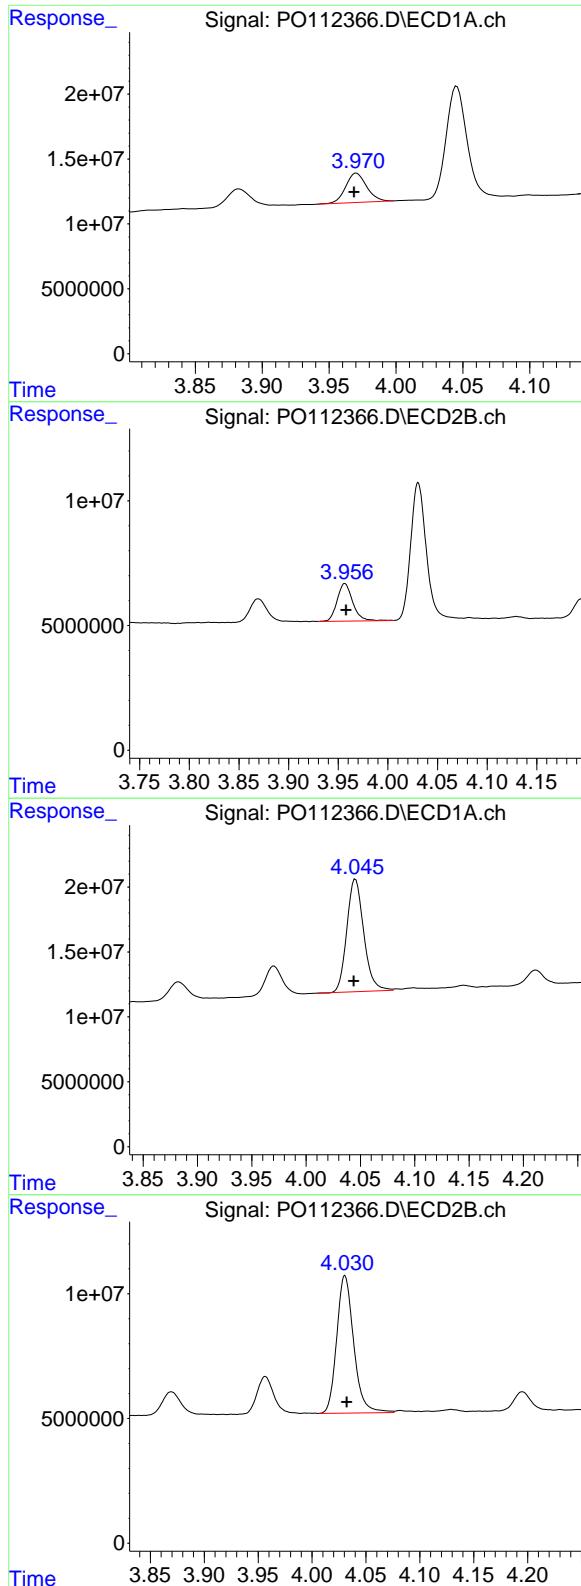

#9 AR-1221-2

R.T.: 3.971 min
 Delta R.T.: 0.002 min
 Response: 24509341
 Conc: 310.87 ng/ml

Instrument: ECD_O
 ClientSampleId: AR1660CCC500

#9 AR-1221-2


R.T.: 3.957 min
 Delta R.T.: -0.001 min
 Response: 16486507
 Conc: 277.77 ng/ml

#10 AR-1221-3

R.T.: 4.045 min
 Delta R.T.: 0.002 min
 Response: 94275348
 Conc: 349.71 ng/ml

#10 AR-1221-3

R.T.: 4.031 min
 Delta R.T.: -0.002 min
 Response: 60498897
 Conc: 320.48 ng/ml

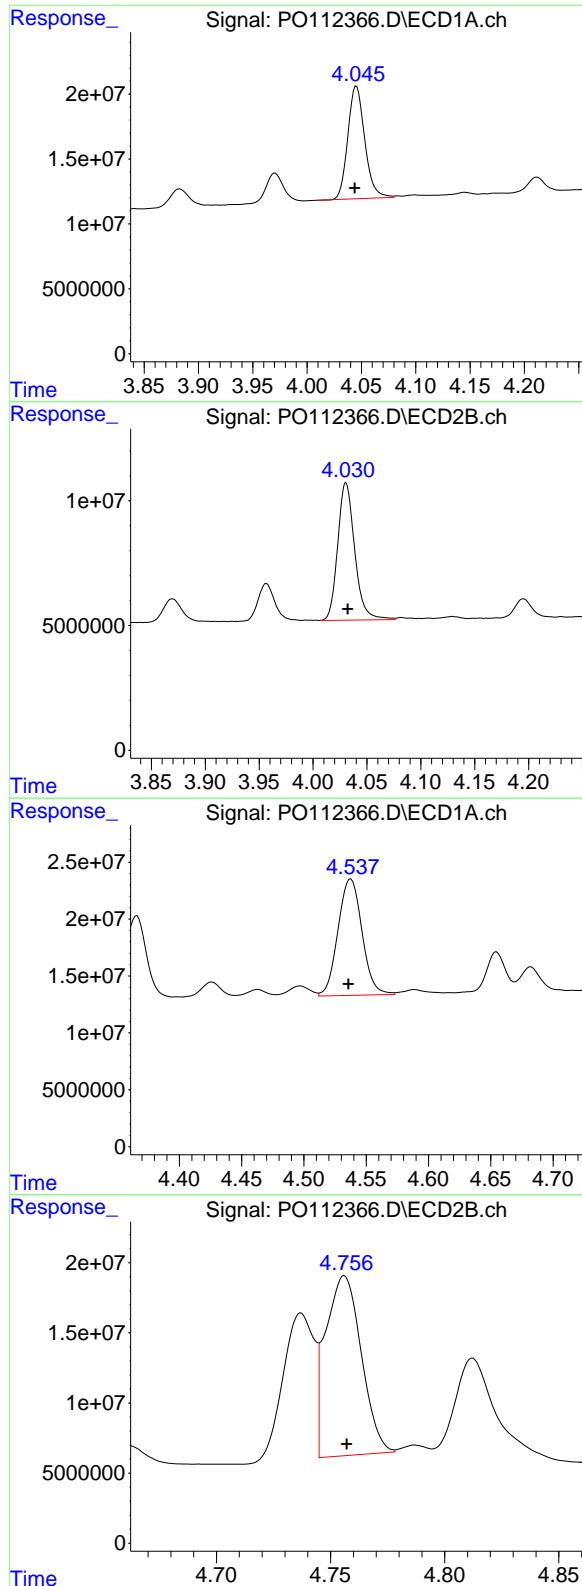

#11 AR-1232-1

R.T.: 4.045 min
 Delta R.T.: 0.002 min
 Response: 94275348
 Conc: 439.17 ng/ml

Instrument: ECD_O
 ClientSampleId: AR1660CCC500

#11 AR-1232-1


R.T.: 4.031 min
 Delta R.T.: -0.002 min
 Response: 60498897
 Conc: 403.06 ng/ml

#12 AR-1232-2

R.T.: 4.538 min
 Delta R.T.: 0.002 min
 Response: 137583153
 Conc: 1210.73 ng/ml


#12 AR-1232-2

R.T.: 4.756 min
 Delta R.T.: 0.000 min
 Response: 139431612
 Conc: 910.81 ng/ml

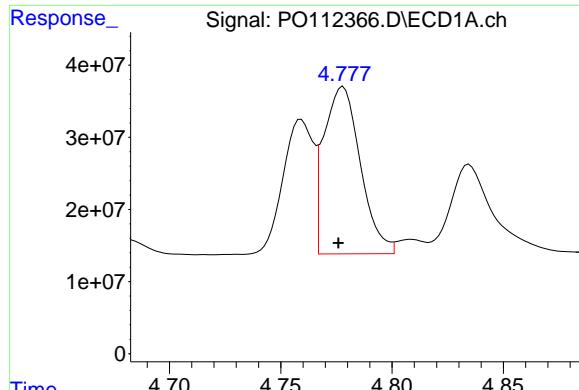


#13 AR-1232-3

R.T.: 4.778 min
 Delta R.T.: 0.002 min
 Response: 264817007
 Conc: 1156.36 ng/ml
Instrument: ECD_O
ClientSampleId : AR1660CCC500

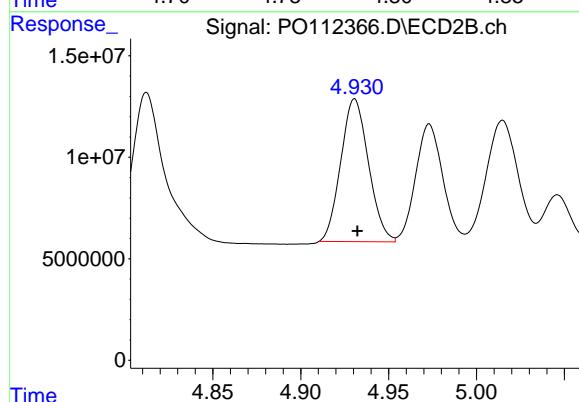


#13 AR-1232-3

R.T.: 4.931 min
 Delta R.T.: -0.002 min
 Response: 77402062
 Conc: 1025.11 ng/ml

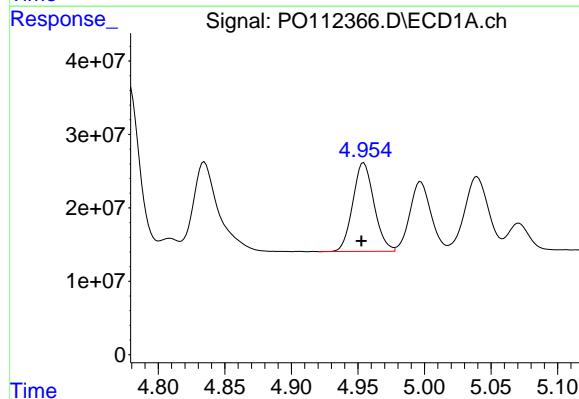


#14 AR-1232-4

R.T.: 4.954 min
 Delta R.T.: 0.002 min
 Response: 134155056
 Conc: 1173.74 ng/ml

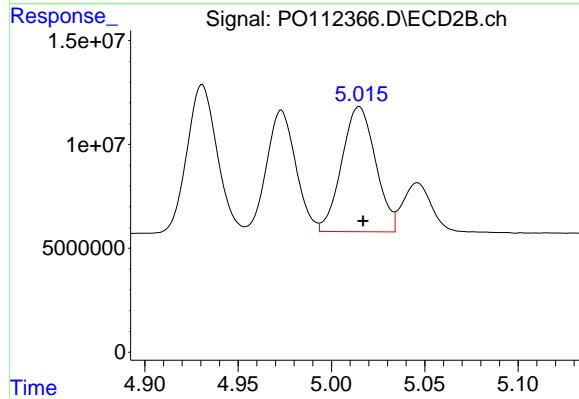

#14 AR-1232-4

R.T.: 5.015 min
 Delta R.T.: -0.002 min
 Response: 75969252
 Conc: 1151.26 ng/ml

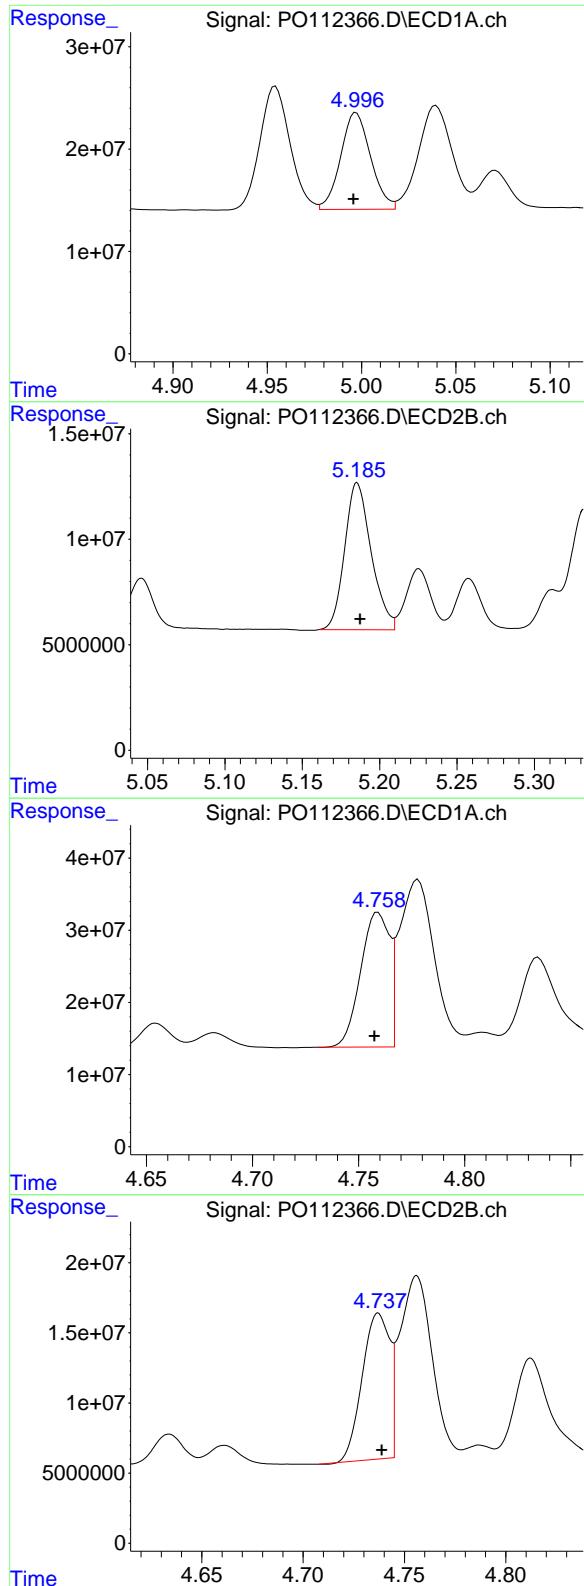

#15 AR-1232-5

R.T.: 4.997 min
 Delta R.T.: 0.001 min
 Response: 104555045
 Conc: 1424.45 ng/ml
Instrument: ECD_O
ClientSampleId: AR1660CCC500

#15 AR-1232-5


R.T.: 5.185 min
 Delta R.T.: -0.002 min
 Response: 83417066
 Conc: 1123.31 ng/ml

#16 AR-1242-1

R.T.: 4.759 min
 Delta R.T.: 0.002 min
 Response: 176513620
 Conc: 609.43 ng/ml

#16 AR-1242-1

R.T.: 4.737 min
 Delta R.T.: -0.002 min
 Response: 98386664
 Conc: 507.52 ng/ml

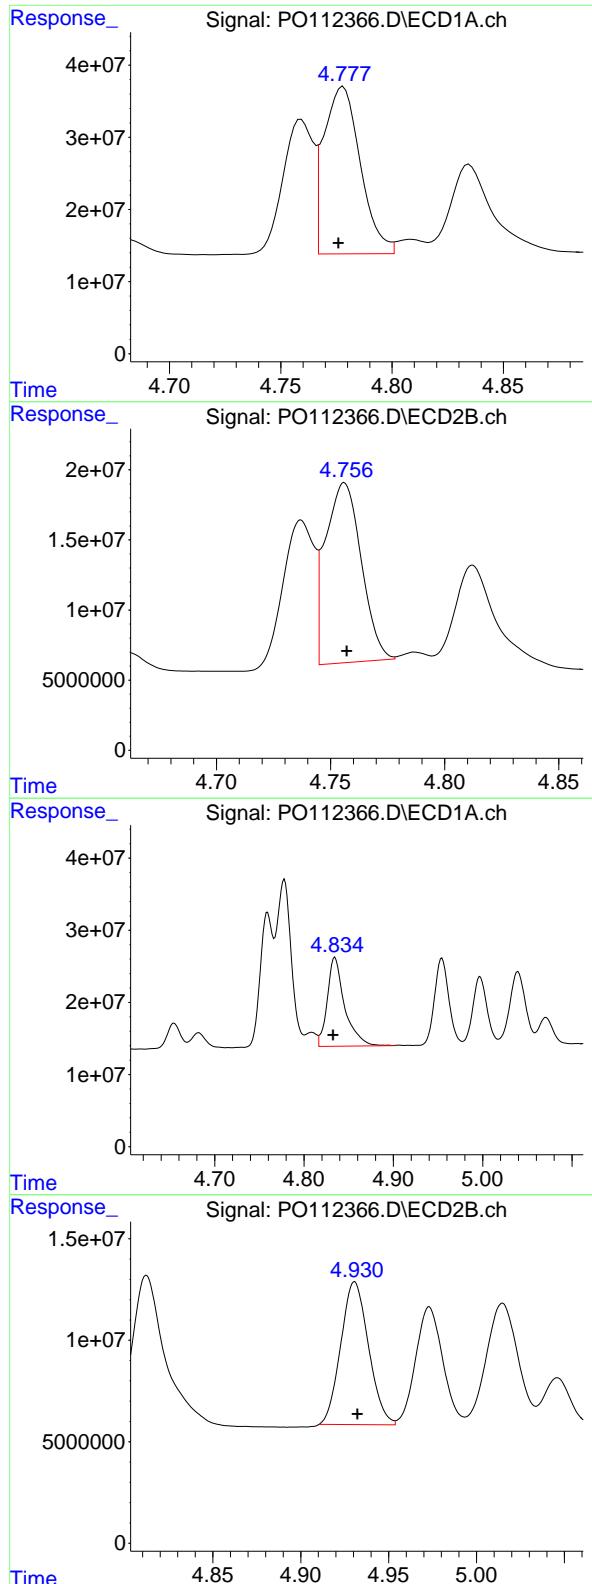

#17 AR-1242-2

R.T.: 4.778 min
 Delta R.T.: 0.002 min
 Response: 264817007
 Conc: 621.75 ng/ml

Instrument: ECD_O
 ClientSampleId: AR1660CCC500

#17 AR-1242-2


R.T.: 4.756 min
 Delta R.T.: 0.000 min
 Response: 139431612
 Conc: 492.08 ng/ml

#18 AR-1242-3

R.T.: 4.835 min
 Delta R.T.: 0.002 min
 Response: 166541661
 Conc: 608.51 ng/ml

#18 AR-1242-3

R.T.: 4.931 min
 Delta R.T.: -0.002 min
 Response: 77402062
 Conc: 531.33 ng/ml

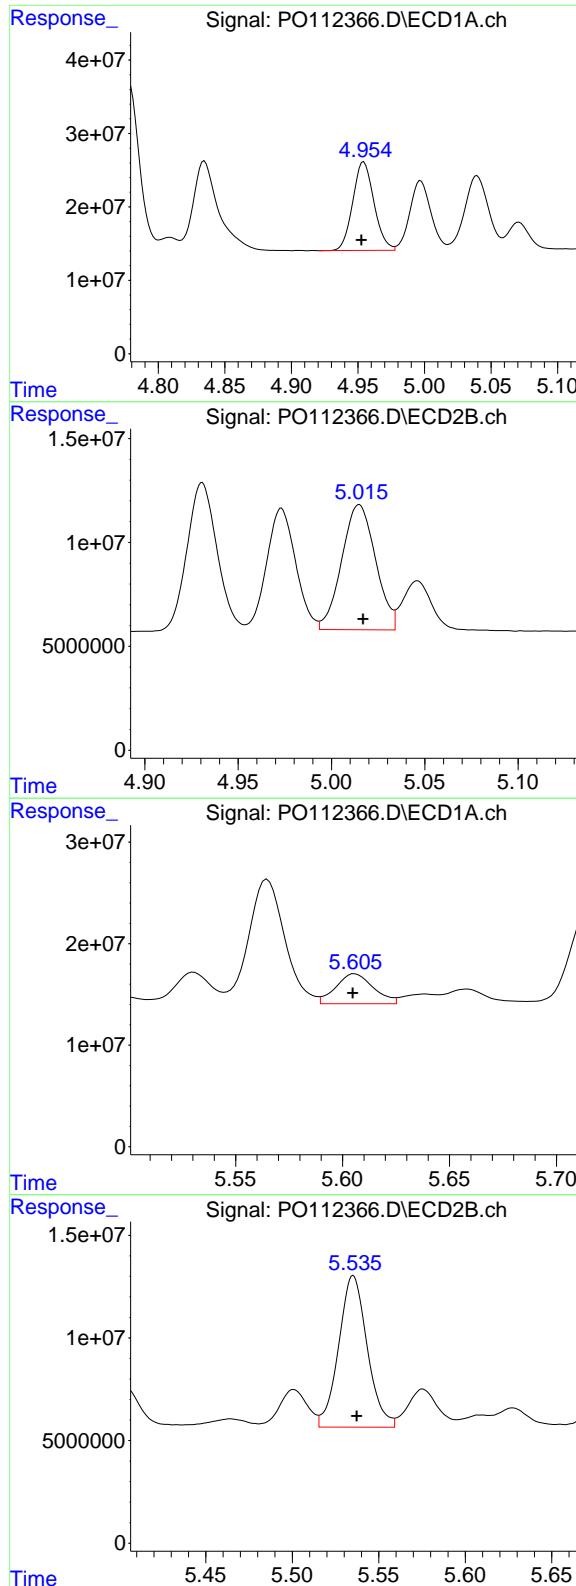

#19 AR-1242-4

R.T.: 4.954 min
 Delta R.T.: 0.002 min
 Response: 134155056
 Conc: 595.40 ng/ml

Instrument: ECD_O
 ClientSampleId: AR1660CCC500

#19 AR-1242-4


R.T.: 5.015 min
 Delta R.T.: -0.002 min
 Response: 75969252
 Conc: 535.60 ng/ml

#20 AR-1242-5

R.T.: 5.606 min
 Delta R.T.: 0.000 min
 Response: 36092211
 Conc: 170.51 ng/ml

#20 AR-1242-5


R.T.: 5.535 min
 Delta R.T.: -0.002 min
 Response: 84564389
 Conc: 465.32 ng/ml

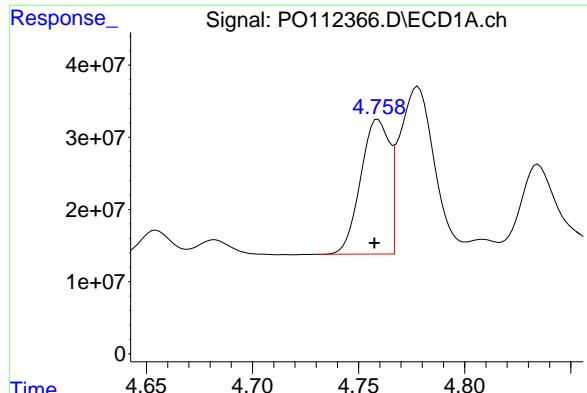

#21 AR-1248-1


R.T.: 4.759 min
 Delta R.T.: 0.002 min
 Response: 176513620
 Conc: 777.94 ng/ml

Instrument: ECD_O
 ClientSampleId: AR1660CCC500

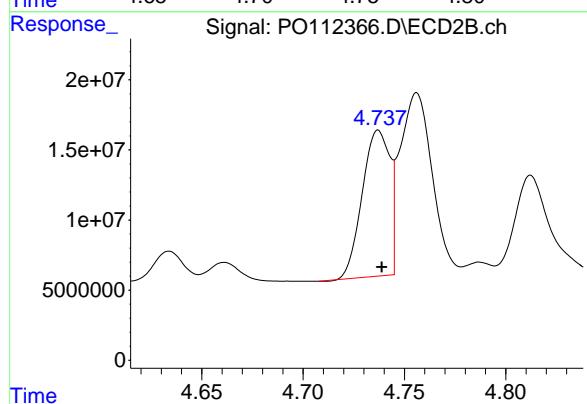


#21 AR-1248-1

R.T.: 4.737 min
 Delta R.T.: -0.002 min
 Response: 98386664
 Conc: 637.35 ng/ml

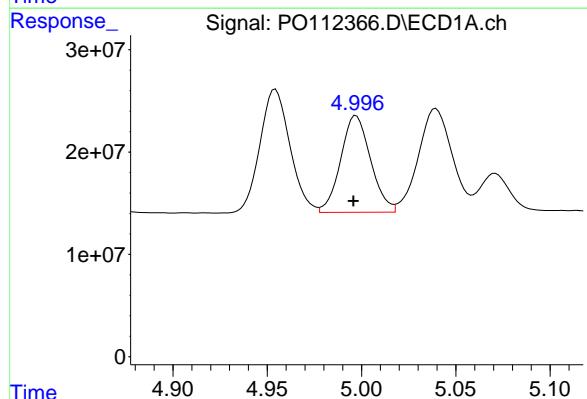


#22 AR-1248-2

R.T.: 4.997 min
 Delta R.T.: 0.001 min
 Response: 104555045
 Conc: 339.11 ng/ml

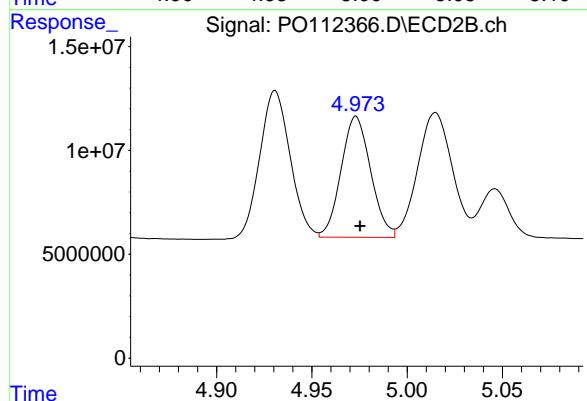

#22 AR-1248-2

R.T.: 4.973 min
 Delta R.T.: -0.002 min
 Response: 62926663
 Conc: 305.81 ng/ml

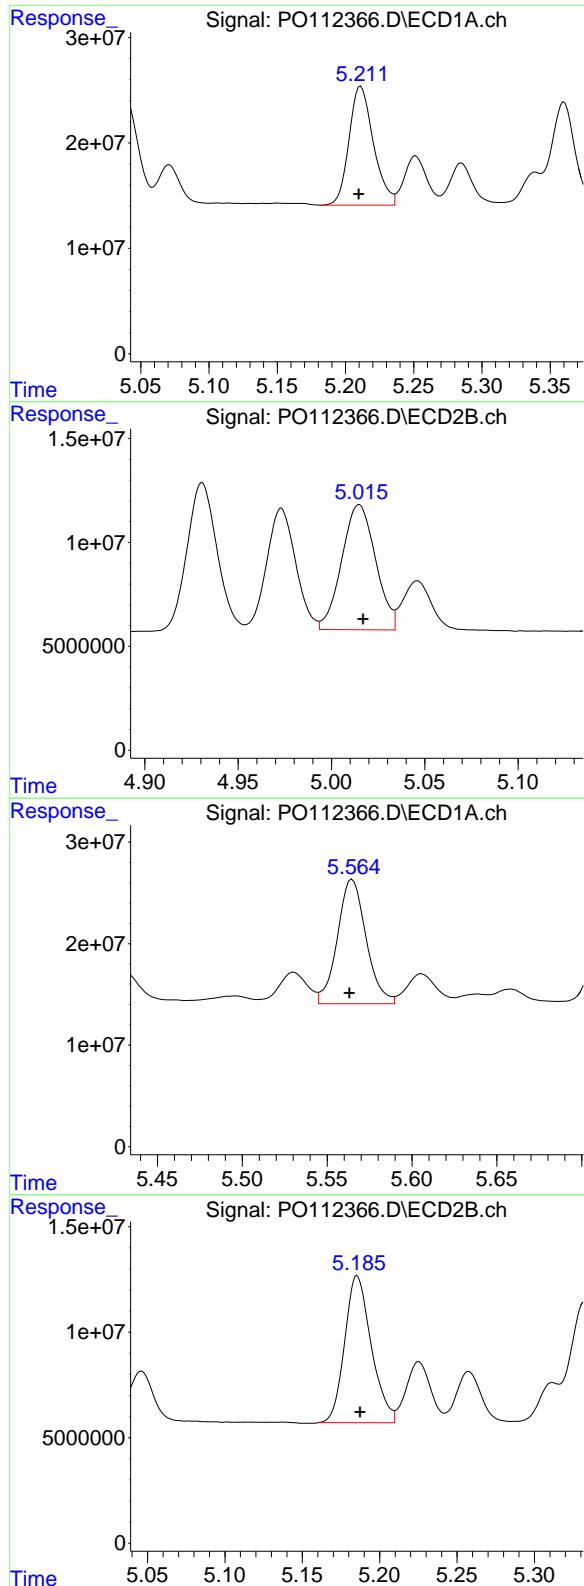

#23 AR-1248-3

R.T.: 5.211 min
 Delta R.T.: 0.002 min
 Response: 139965370
 Conc: 343.63 ng/ml

Instrument: ECD_O
 ClientSampleId: AR1660CCC500

#23 AR-1248-3


R.T.: 5.015 min
 Delta R.T.: -0.002 min
 Response: 75969252
 Conc: 353.68 ng/ml

#24 AR-1248-4

R.T.: 5.565 min
 Delta R.T.: 0.002 min
 Response: 144182766
 Conc: 249.82 ng/ml

#24 AR-1248-4

R.T.: 5.185 min
 Delta R.T.: -0.002 min
 Response: 83417066
 Conc: 322.41 ng/ml

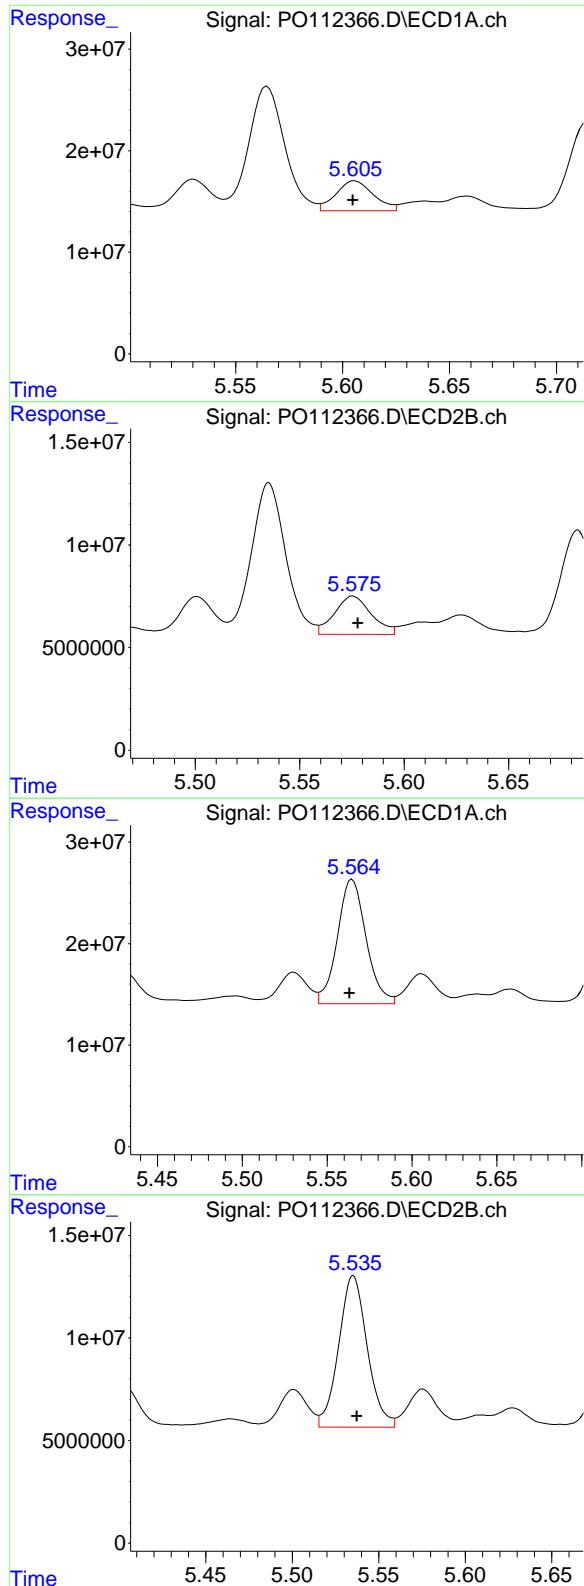

#25 AR-1248-5

R.T.: 5.606 min
 Delta R.T.: 0.000 min
 Response: 36092211
 Conc: 92.47 ng/ml

Instrument: ECD_O
 ClientSampleId: AR1660CCC500

#25 AR-1248-5


R.T.: 5.575 min
 Delta R.T.: -0.002 min
 Response: 22841188
 Conc: 91.16 ng/ml

#26 AR-1254-1

R.T.: 5.565 min
 Delta R.T.: 0.002 min
 Response: 144182766
 Conc: 234.40 ng/ml

#26 AR-1254-1

R.T.: 5.535 min
 Delta R.T.: -0.002 min
 Response: 84564389
 Conc: 221.86 ng/ml

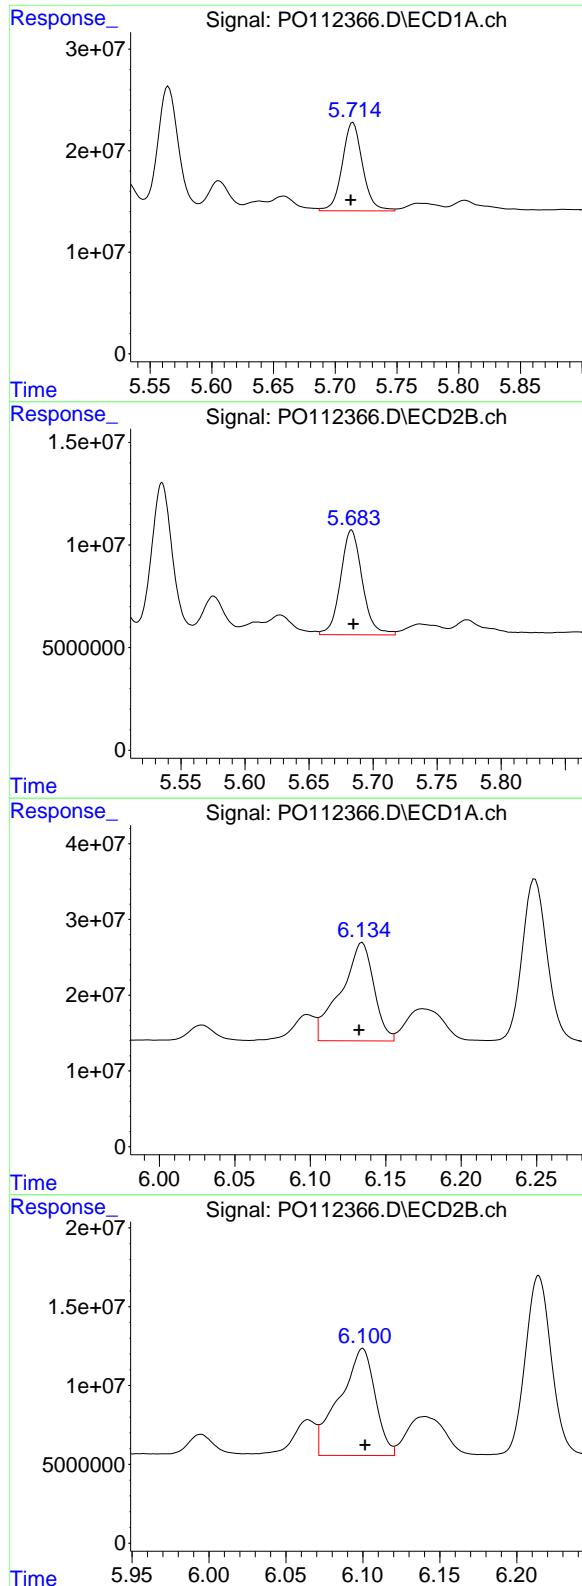

#27 AR-1254-2

R.T.: 5.714 min
 Delta R.T.: 0.002 min
 Response: 100121117
 Conc: 186.90 ng/ml

Instrument: ECD_O
 ClientSampleId: AR1660CCC500

#27 AR-1254-2


R.T.: 5.683 min
 Delta R.T.: -0.002 min
 Response: 60270259
 Conc: 181.64 ng/ml

#28 AR-1254-3

R.T.: 6.134 min
 Delta R.T.: 0.002 min
 Response: 198228185
 Conc: 236.10 ng/ml

#28 AR-1254-3


R.T.: 6.100 min
 Delta R.T.: -0.002 min
 Response: 109004944
 Conc: 226.13 ng/ml

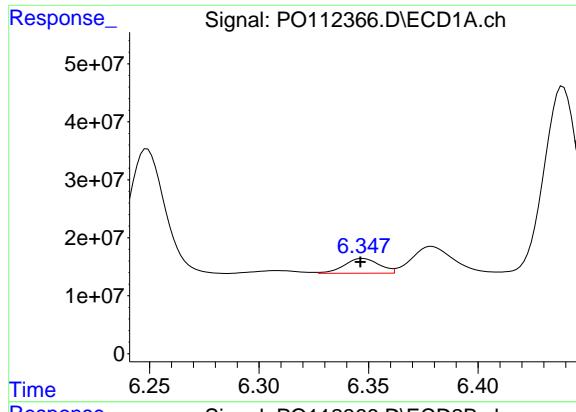

#29 AR-1254-4


R.T.: 6.347 min
 Delta R.T.: 0.001 min
 Response: 28382091
 Conc: 59.00 ng/ml

Instrument: ECD_O
 ClientSampleId: AR1660CCC500

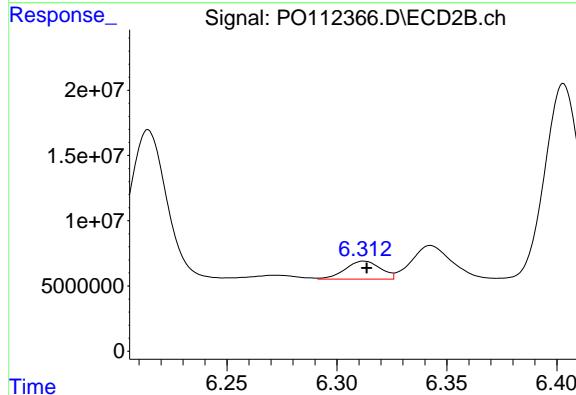


#29 AR-1254-4

R.T.: 6.312 min
 Delta R.T.: -0.001 min
 Response: 15522172
 Conc: 59.54 ng/ml

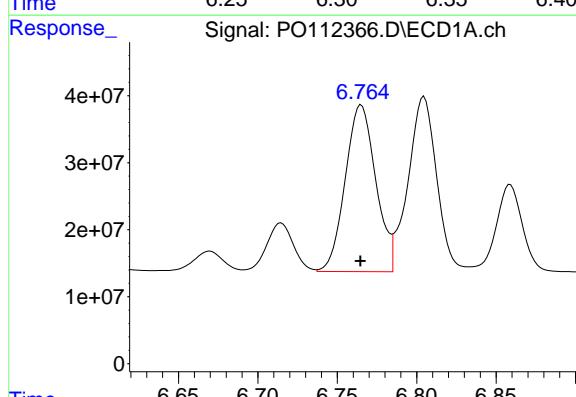


#30 AR-1254-5

R.T.: 6.765 min
 Delta R.T.: 0.000 min
 Response: 332877182
 Conc: 430.10 ng/ml

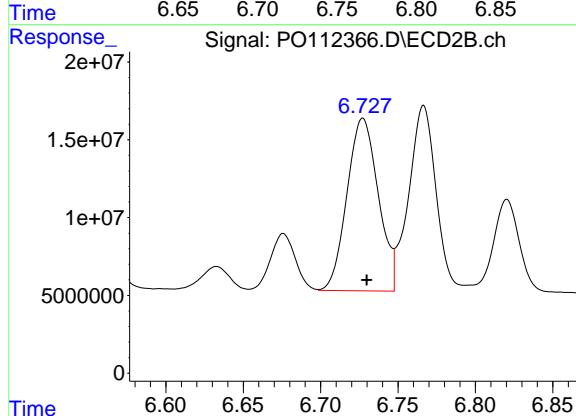

#30 AR-1254-5


R.T.: 6.727 min
 Delta R.T.: -0.002 min
 Response: 156012311
 Conc: 437.80 ng/ml

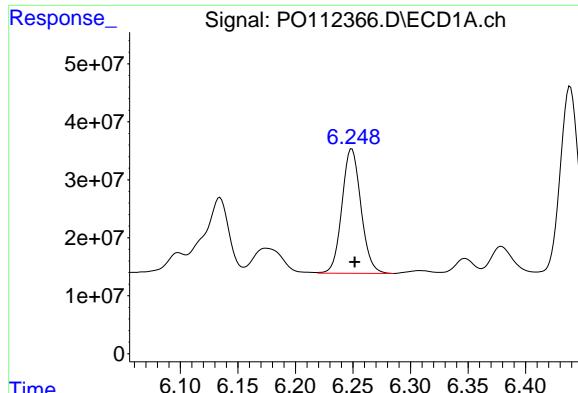

#31 AR-1260-1


R.T.: 6.249 min
 Delta R.T.: -0.003 min
 Response: 247502934
 Conc: 493.78 ng/ml

Instrument: ECD_O
 ClientSampleId: AR1660CCC500

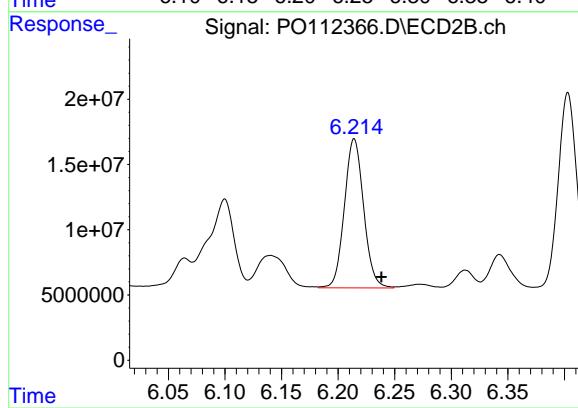


#31 AR-1260-1

R.T.: 6.214 min
 Delta R.T.: -0.024 min
 Response: 135454857
 Conc: 482.80 ng/ml

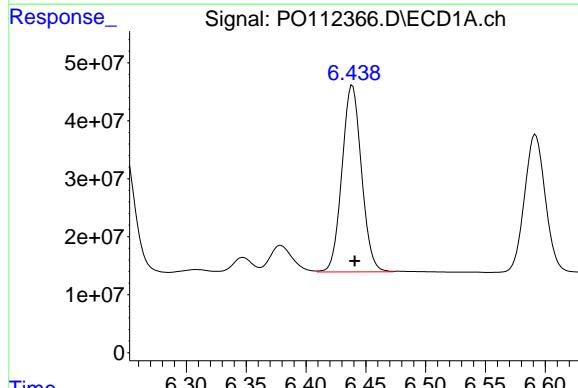


#32 AR-1260-2

R.T.: 6.439 min
 Delta R.T.: -0.002 min
 Response: 365378129
 Conc: 495.00 ng/ml

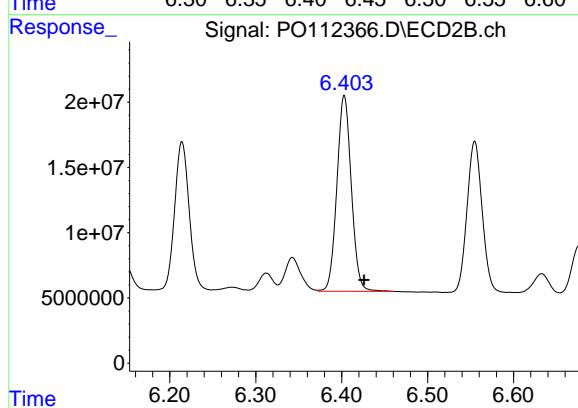

#32 AR-1260-2


R.T.: 6.403 min
 Delta R.T.: -0.023 min
 Response: 174971478
 Conc: 514.63 ng/ml

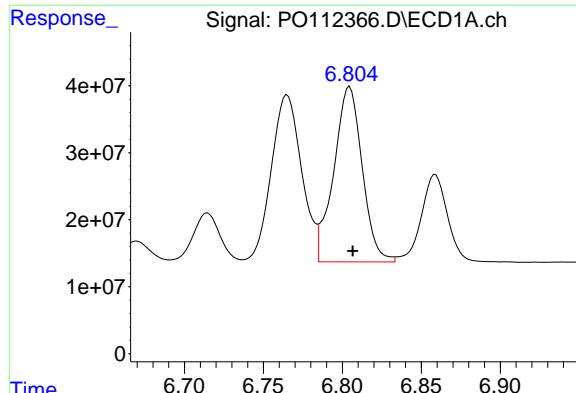

#33 AR-1260-3


R.T.: 6.805 min
 Delta R.T.: -0.002 min
 Response: 327878936
 Conc: 500.21 ng/ml

Instrument: ECD_O
 ClientSampleId: AR1660CCC500

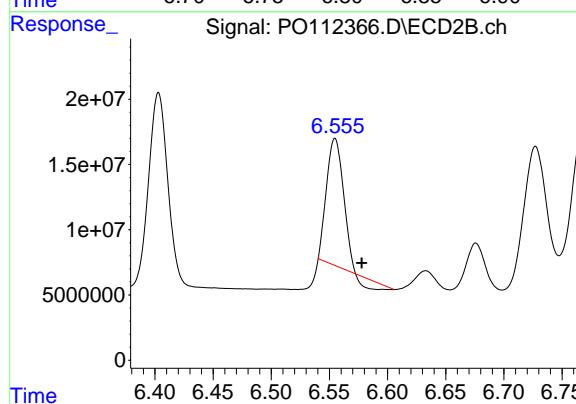


#33 AR-1260-3

R.T.: 6.555 min
 Delta R.T.: -0.023 min
 Response: 91053432
 Conc: 330.40 ng/ml

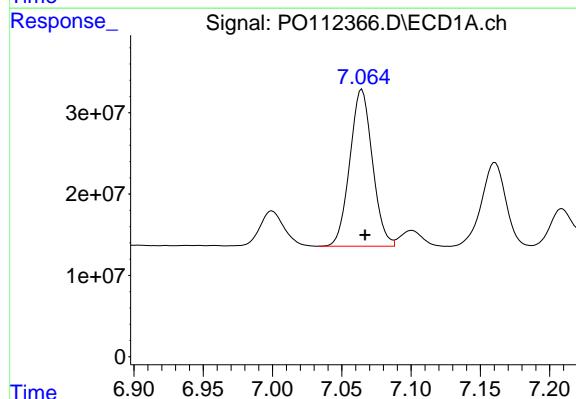


#34 AR-1260-4

R.T.: 7.064 min
 Delta R.T.: -0.002 min
 Response: 219151907
 Conc: 503.51 ng/ml

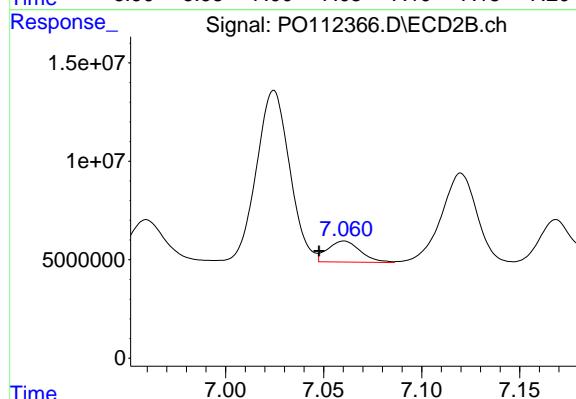

#34 AR-1260-4


R.T.: 7.060 min
 Delta R.T.: 0.013 min
 Response: 12369917
 Conc: 61.65 ng/ml



#35 AR-1260-5


R.T.: 7.307 min
 Delta R.T.: -0.002 min
 Response: 613903993
 Conc: 486.25 ng/ml

Instrument: ECD_O
 ClientSampleId: AR1660CCC500

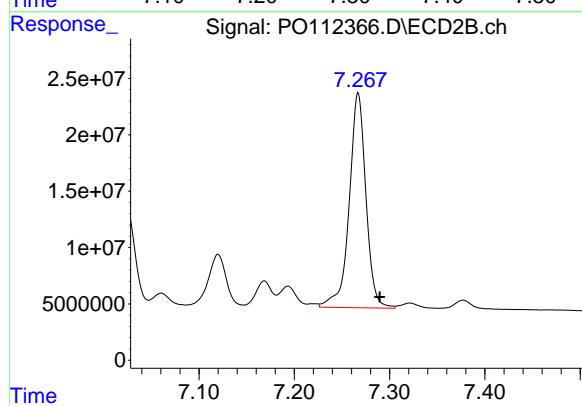


#35 AR-1260-5

R.T.: 7.267 min
 Delta R.T.: -0.022 min
 Response: 232707276
 Conc: 519.75 ng/ml

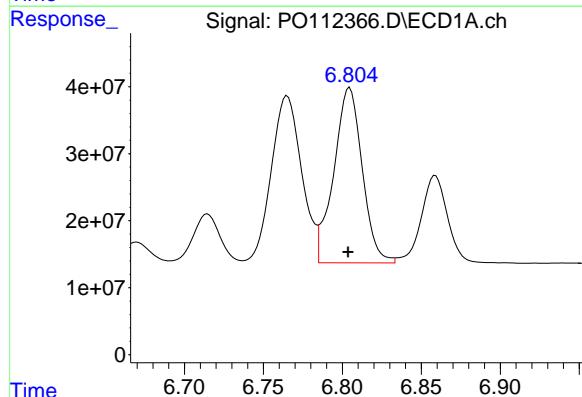


#36 AR-1262-1

R.T.: 6.805 min
 Delta R.T.: 0.001 min
 Response: 327878936
 Conc: 320.92 ng/ml

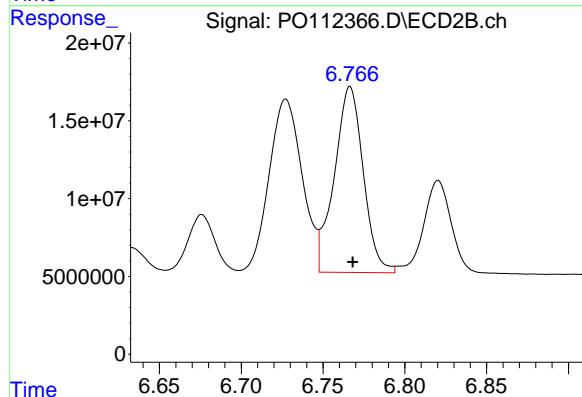

#36 AR-1262-1

R.T.: 6.767 min
 Delta R.T.: -0.002 min
 Response: 147082291
 Conc: 361.10 ng/ml

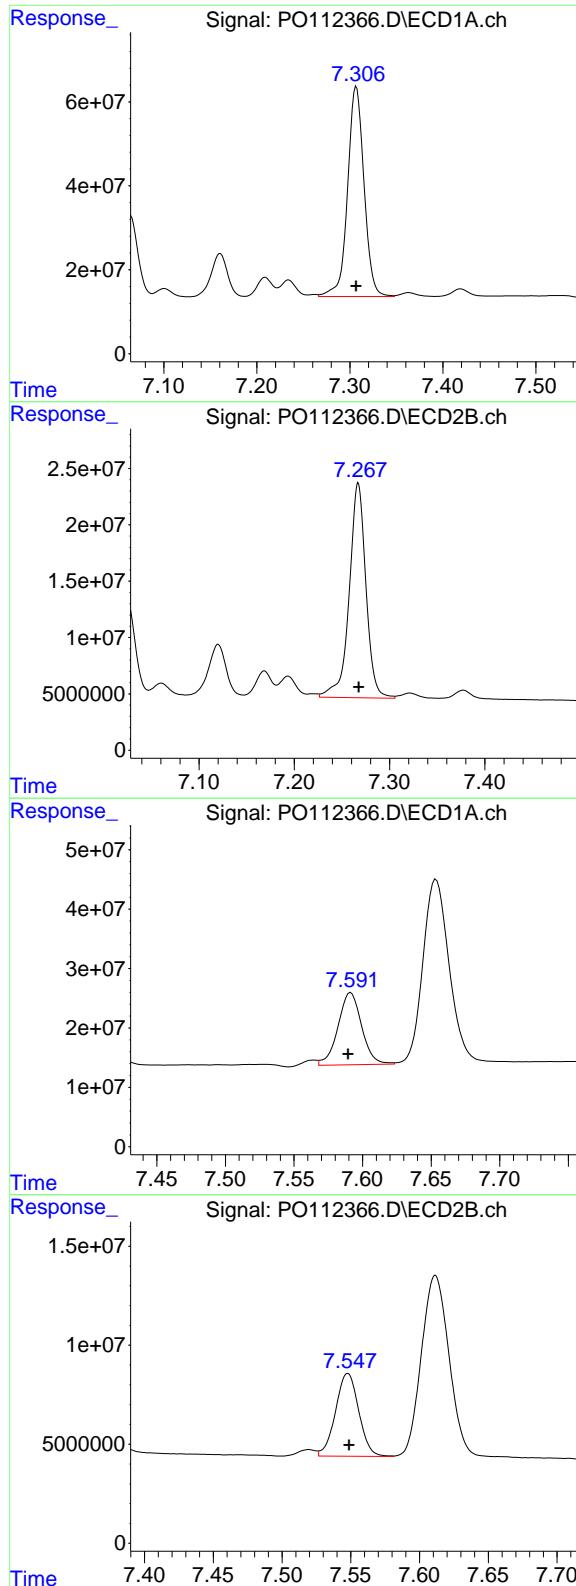

#37 AR-1262-2

R.T.: 7.307 min
 Delta R.T.: 0.000 min
 Response: 613903993
 Conc: 374.47 ng/ml

Instrument: ECD_O
 ClientSampleId: AR1660CCC500

#37 AR-1262-2


R.T.: 7.267 min
 Delta R.T.: 0.000 min
 Response: 232707276
 Conc: 454.02 ng/ml

#38 AR-1262-3

R.T.: 7.591 min
 Delta R.T.: 0.002 min
 Response: 145699653
 Conc: 226.96 ng/ml

#38 AR-1262-3

R.T.: 7.548 min
 Delta R.T.: 0.000 min
 Response: 49200657
 Conc: 274.06 ng/ml

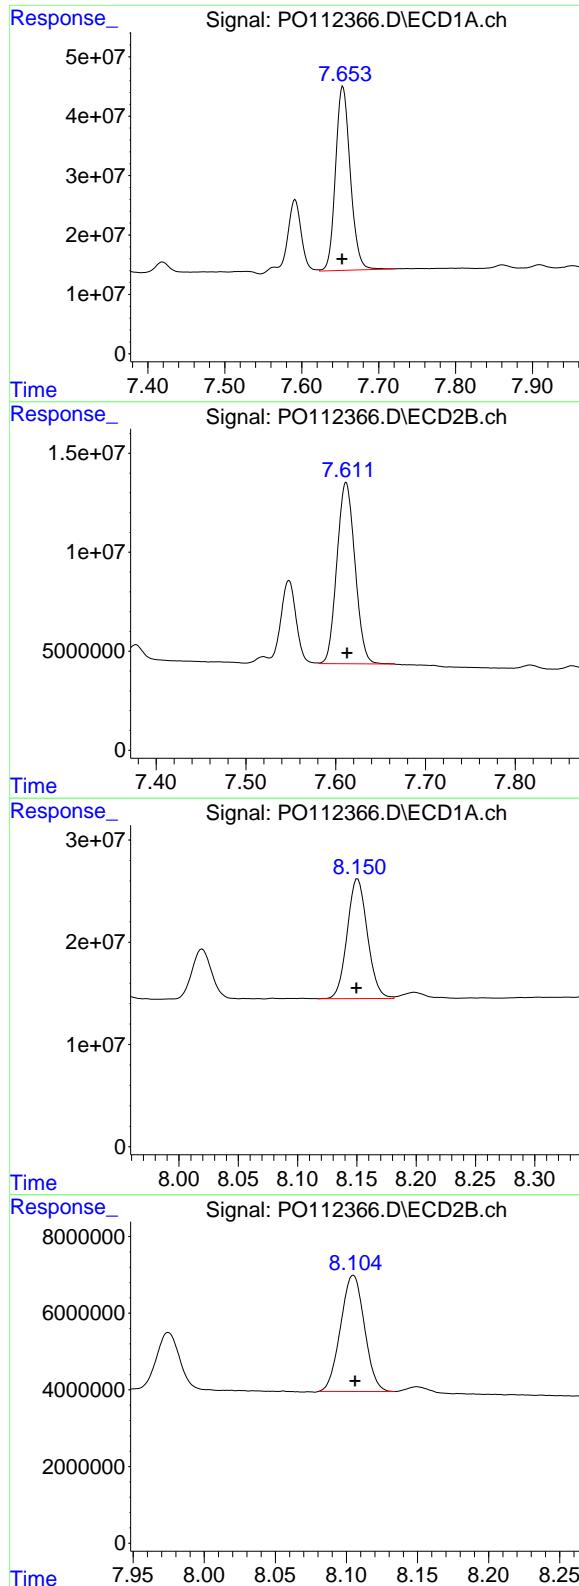

#39 AR-1262-4

R.T.: 7.654 min
 Delta R.T.: 0.001 min
 Response: 412857283
 Conc: 385.33 ng/ml

Instrument: ECD_O
ClientSampleId: AR1660CCC500

#39 AR-1262-4


R.T.: 7.612 min
 Delta R.T.: -0.001 min
 Response: 127849232
 Conc: 439.47 ng/ml

#40 AR-1262-5

R.T.: 8.151 min
 Delta R.T.: 0.000 min
 Response: 139157075
 Conc: 310.52 ng/ml

#40 AR-1262-5

R.T.: 8.105 min
 Delta R.T.: -0.001 min
 Response: 35416682
 Conc: 334.80 ng/ml

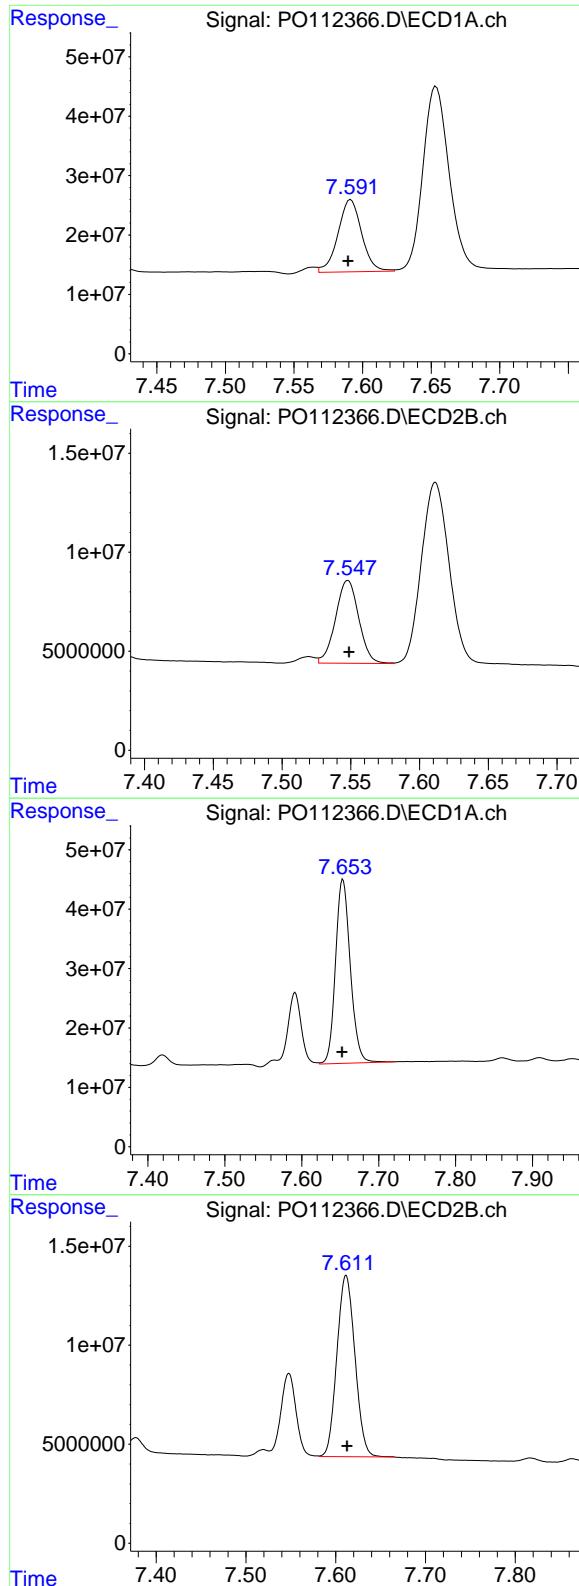

#41 AR-1268-1

R.T.: 7.591 min
 Delta R.T.: 0.002 min
 Response: 145699653
 Conc: 79.29 ng/ml

Instrument: ECD_O
 ClientSampleId: AR1660CCC500

#41 AR-1268-1


R.T.: 7.548 min
 Delta R.T.: 0.000 min
 Response: 49200657
 Conc: 100.11 ng/ml

#42 AR-1268-2

R.T.: 7.654 min
 Delta R.T.: 0.001 min
 Response: 412857283
 Conc: 265.06 ng/ml

#42 AR-1268-2

R.T.: 7.612 min
 Delta R.T.: -0.001 min
 Response: 127849232
 Conc: 306.46 ng/ml

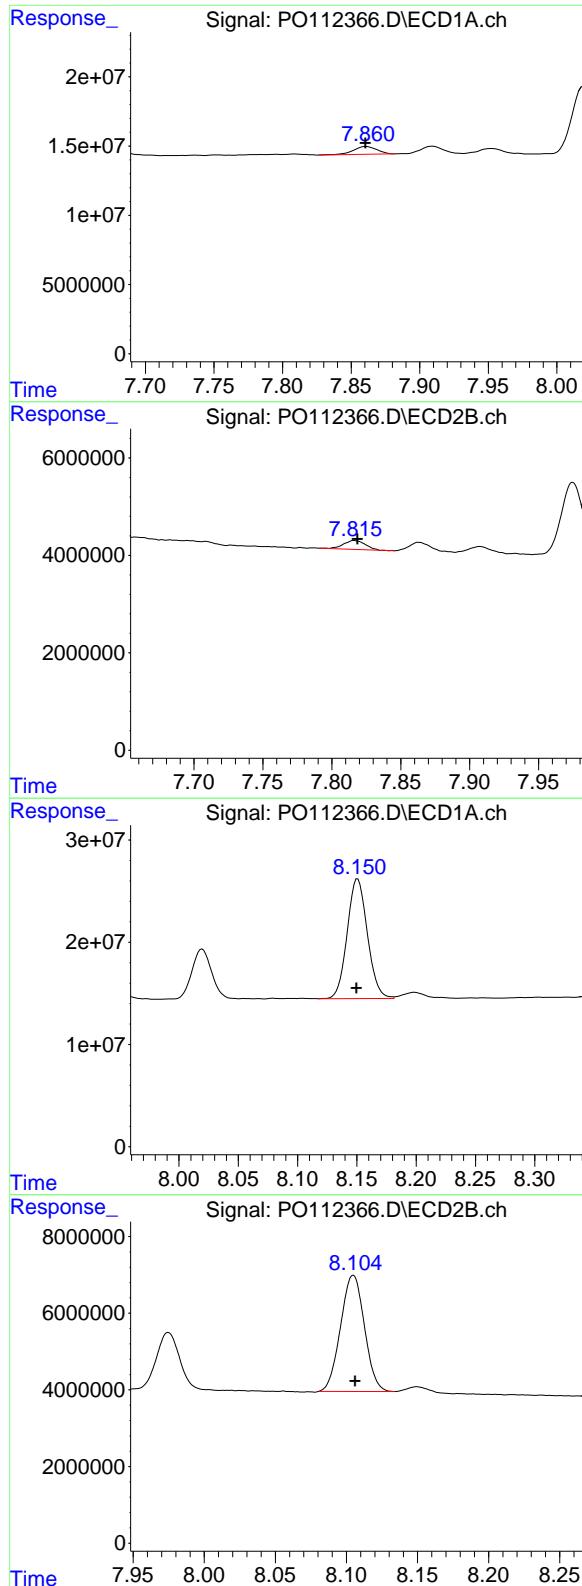

#43 AR-1268-3

R.T.: 7.861 min
 Delta R.T.: 0.000 min **Instrument:**
 Response: 6667277 ECD_O
 Conc: 5.13 ng/ml **ClientSampleId:**
 AR1660CCC500

#43 AR-1268-3


R.T.: 7.816 min
 Delta R.T.: -0.002 min
 Response: 2004613
 Conc: 6.34 ng/ml

#44 AR-1268-4

R.T.: 8.151 min
 Delta R.T.: 0.000 min
 Response: 139157075
 Conc: 289.66 ng/ml

#44 AR-1268-4

R.T.: 8.105 min
 Delta R.T.: -0.001 min
 Response: 35416682
 Conc: 317.60 ng/ml

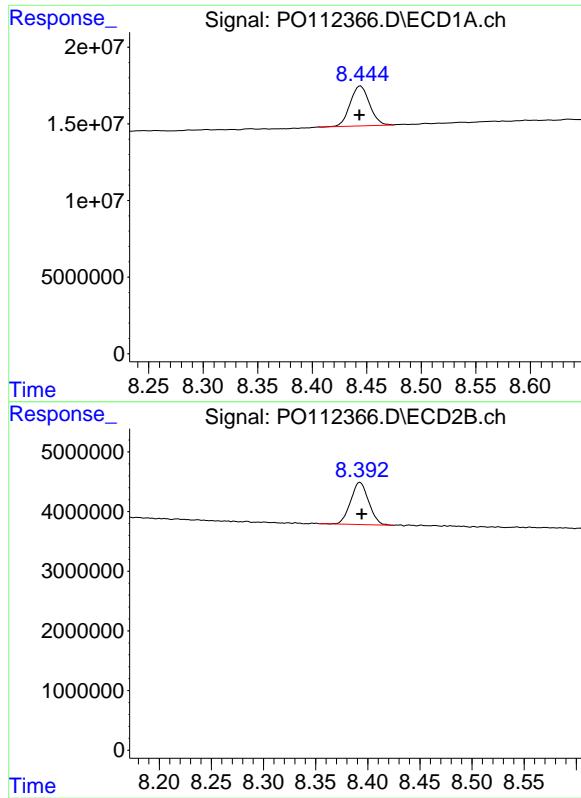

#45 AR-1268-5

R.T.: 8.444 min
Delta R.T.: 0.001 min
Response: 32257747
Conc: 9.88 ng/ml

Instrument: ECD_O
ClientSampleId: AR1660CCC500

#45 AR-1268-5

R.T.: 8.392 min
Delta R.T.: -0.002 min
Response: 8529469
Conc: 11.74 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0072225\
 Data File : P0112373.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Jul 2025 11:26
 Operator : YP/AJ
 Sample : Q2639-11RE
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
OU4-TS-43-071725

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 23 01:48:03 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 22 09:14:26 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	3.668	3.662	158.9E6	93373800	16.056	14.656
2) SA Decachlor...	8.695	8.681	112.4E6	20636	16.441	0.012 #

Target Compounds

5) L1 AR-1016-3	4.832	4.935	9836742	2009509	30.387	11.830 #
7) L1 AR-1016-5	5.196	5.212	13300023	546515	48.600	3.169 #
8) L2 AR-1221-1	3.872	3.860	6415151	2298237	55.012	27.927 #
9) L2 AR-1221-2	3.971	3.963	9158748	9563958	116.168	161.135 #
10) L2 AR-1221-3	4.044	4.030	2932076	6951984	10.876	36.827 #
11) L3 AR-1232-1	4.044	4.030	2932076	6951984	13.659	46.316 #
12) L3 AR-1232-2	4.530	4.766	11325187	1682474	99.661	10.990 #
13) L3 AR-1232-3	4.785	4.935	-2917415	2009509	N.D.	26.614 #
14) L3 AR-1232-4	4.956	5.015	-735652	435339	N.D.	6.597 #
15) L3 AR-1232-5	4.998	5.196	2764611	796399	37.665	10.724 #
18) L4 AR-1242-3	4.832	4.935	9836742	2009509	35.942	13.794 #
20) L4 AR-1242-5	5.600	5.543	16376015	11939197	77.365	65.696
22) L5 AR-1248-2	4.998	4.975	2764611	1451854	8.967	7.056
23) L5 AR-1248-3	5.196	5.015	13300023	435339	32.653	2.027 #
24) L5 AR-1248-4	5.569	5.196	22176832	796399	38.425	3.078 #
25) L5 AR-1248-5	5.600	5.571	16376015	9354361	41.957	37.335
26) L6 AR-1254-1	5.569	5.543	22176832	11939197	36.053	31.323
27) L6 AR-1254-2	5.710	5.683	15605025	8781774	29.131	26.466
28) L6 AR-1254-3	6.134	6.096	8022042	6503916	9.555	13.492 #
29) L6 AR-1254-4	6.332	6.298	12064042	2984702	25.080	11.449 #
30) L6 AR-1254-5	6.761	6.725	8164834	3373459	10.550	9.467
31) L7 AR-1260-1	6.250	6.252	36774403	2989170	73.367	10.654 #
32) L7 AR-1260-2	6.434	6.441	43025789	3264350	58.290	9.601 #
33) L7 AR-1260-3	6.799	6.583	3908110	586698	5.962	2.129 #
34) L7 AR-1260-4	7.065	7.055	1069848	844445	2.458	4.209 #
35) L7 AR-1260-5	7.302	7.292	7752788	644749	6.141	1.440 #
36) L8 AR-1262-1	6.799	6.779	3908110	19892	3.825	0.049 #
37) L8 AR-1262-2	7.302	7.265	7752788	2150057	4.729	4.195
38) L8 AR-1262-3	7.601	7.558	18790082	6190981	29.269	34.486
39) L8 AR-1262-4	7.648	7.609	7593807	1482669	7.088	5.096 #
40) L8 AR-1262-5	8.152	8.096	1483311	148000	3.310	1.399 #
41) L9 AR-1268-1	7.601	7.558	18790082	6190981	10.226	12.597
42) L9 AR-1268-2	7.648	7.609	7593807	1482669	4.875	3.554 #
44) L9 AR-1268-4	8.152	8.096	1483311	148000	3.088	1.327 #
45) L9 AR-1268-5	8.443	8.391	2022144	319590	0.620	0.440 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0072225\
 Data File : P0112373.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Jul 2025 11:26
 Operator : YP/AJ
 Sample : Q2639-11RE
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 OU4-TS-43-071725

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 23 01:48:03 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 22 09:14:26 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

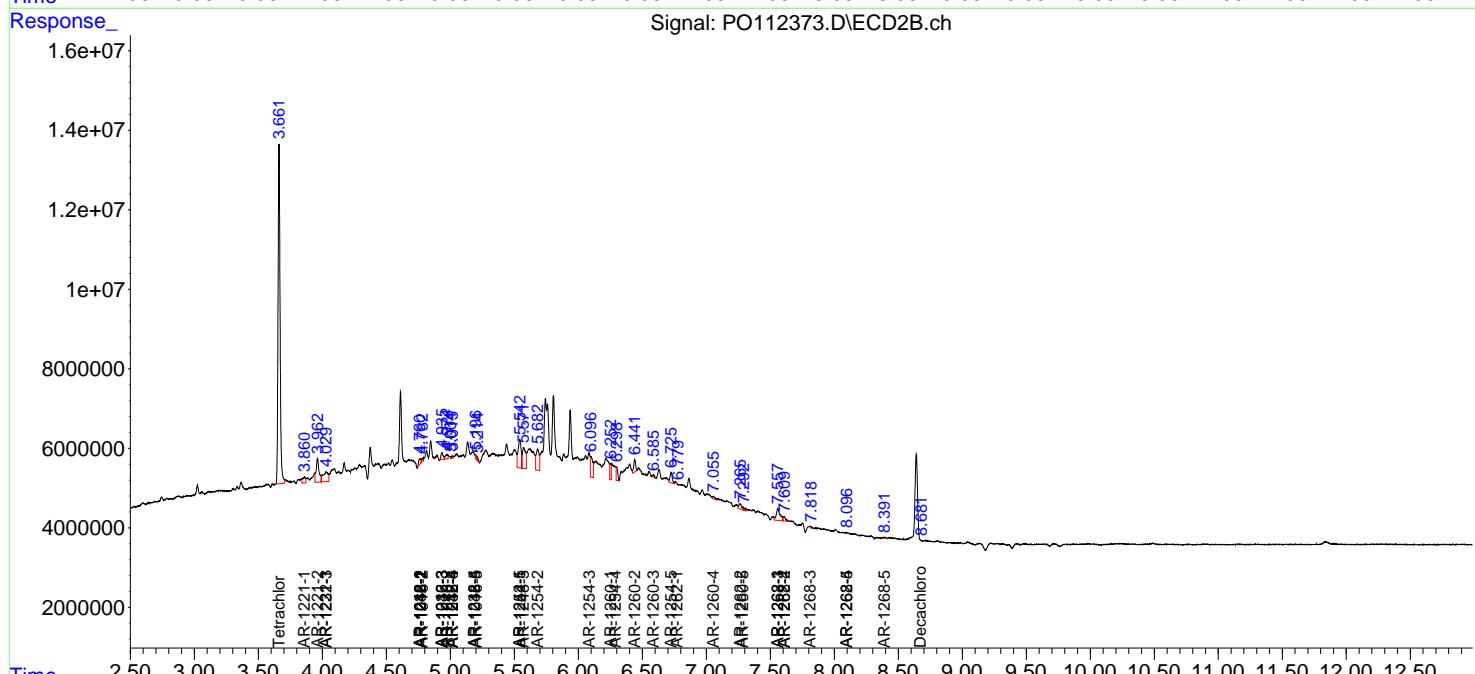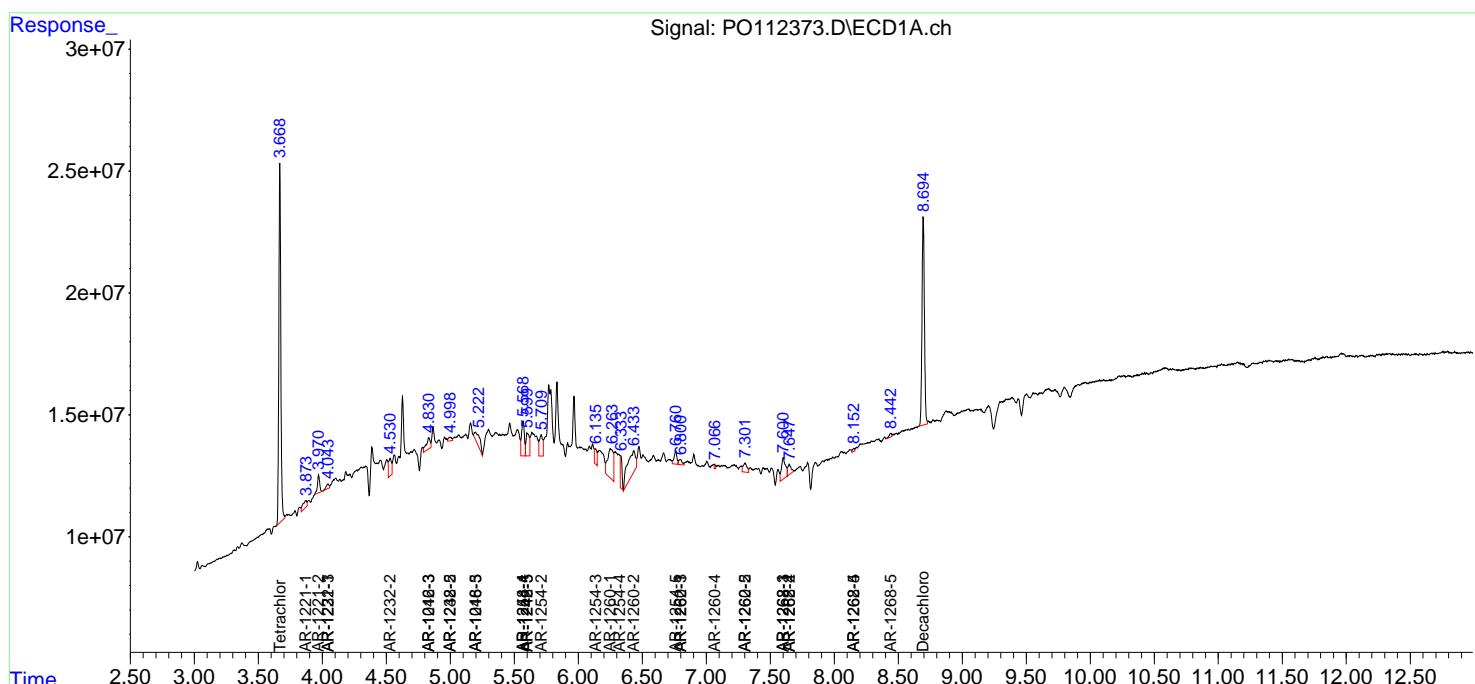


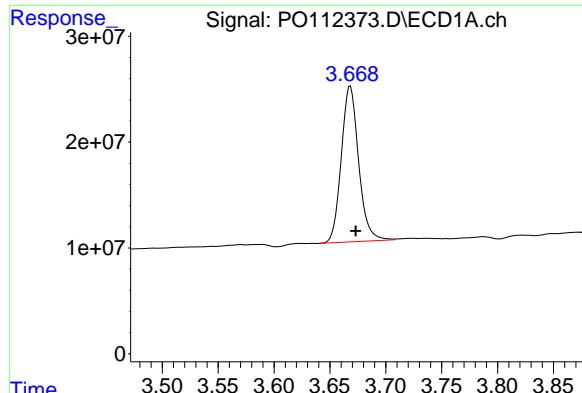

#1 Tetrachloro-m-xylene


R.T.: 3.668 min
Delta R.T.: -0.005 min
Response: 158871223
Conc: 16.06 ng/ml

Instrument: ECD_O
ClientSampleId: OU4-TS-43-071725

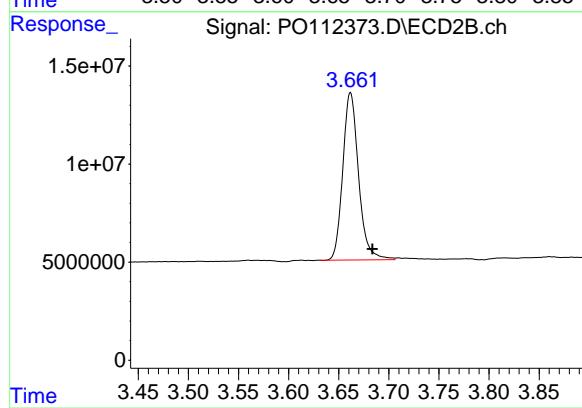


#1 Tetrachloro-m-xylene

R.T.: 3.662 min
Delta R.T.: -0.022 min
Response: 93373800
Conc: 14.66 ng/ml

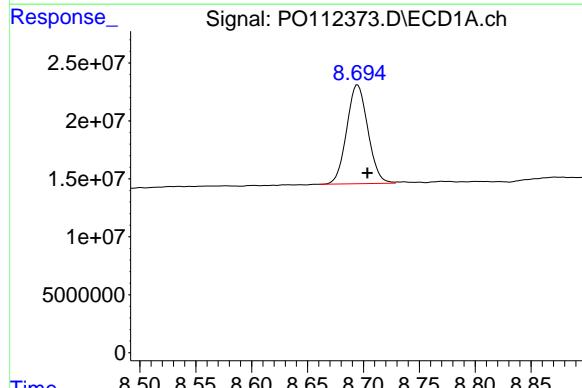


#2 Decachlorobiphenyl

R.T.: 8.695 min
Delta R.T.: -0.009 min
Response: 112410188
Conc: 16.44 ng/ml

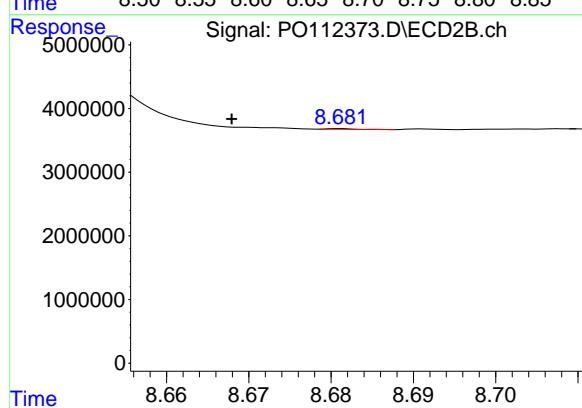

#2 Decachlorobiphenyl

R.T.: 8.681 min
Delta R.T.: 0.013 min
Response: 20636
Conc: 0.01 ng/ml

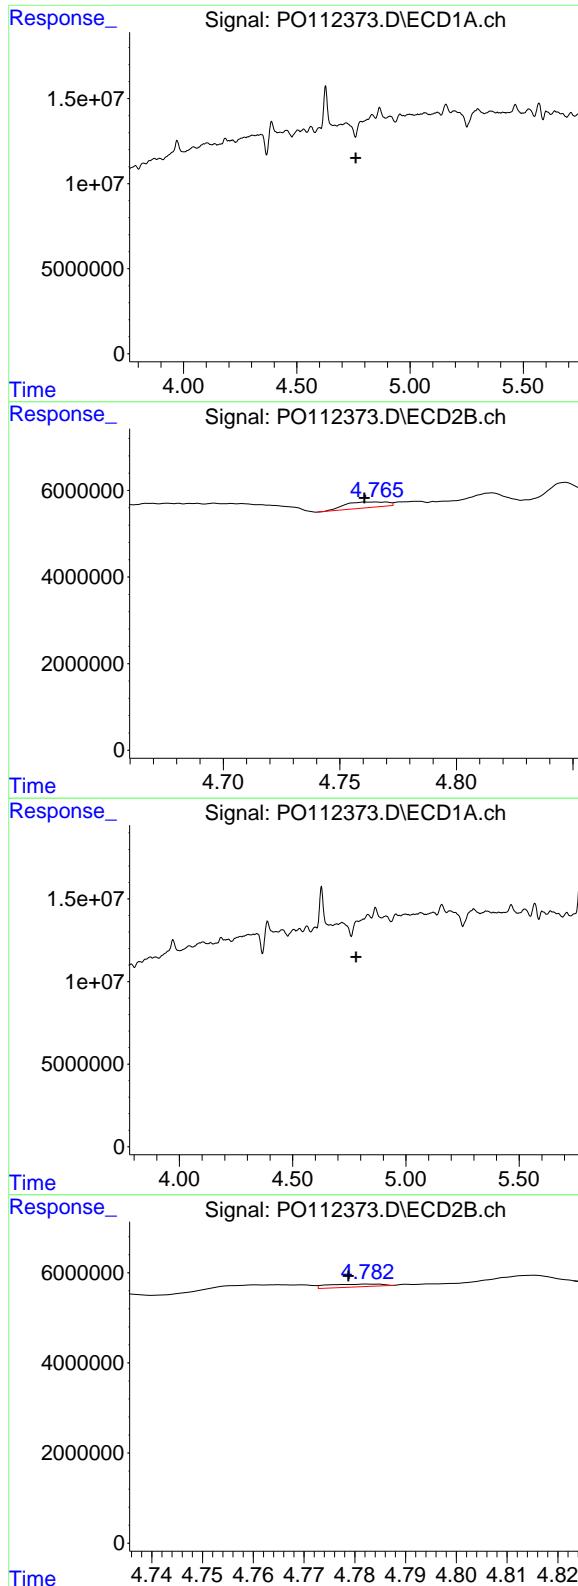

#3 AR-1016-1

R.T.: 4.785 min
 Delta R.T.: 0.024 min
 Response: -2917415
 Conc: N.D.

Instrument: ECD_O
ClientSampleId: OU4-TS-43-071725

#3 AR-1016-1


R.T.: 4.766 min
 Delta R.T.: 0.005 min
 Response: 1682474
 Conc: 7.55 ng/ml

#4 AR-1016-2

R.T.: 4.785 min
 Delta R.T.: 0.005 min
 Response: -2917415
 Conc: N.D.

#4 AR-1016-2


R.T.: 4.783 min
 Delta R.T.: 0.004 min
 Response: 462649
 Conc: 1.41 ng/ml

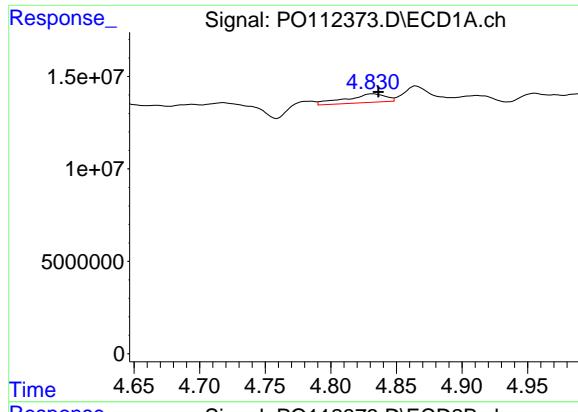

#5 AR-1016-3


R.T.: 4.832 min
Delta R.T.: -0.004 min
Response: 9836742
Conc: 30.39 ng/ml

Instrument: ECD_O
ClientSampleId: OU4-TS-43-071725

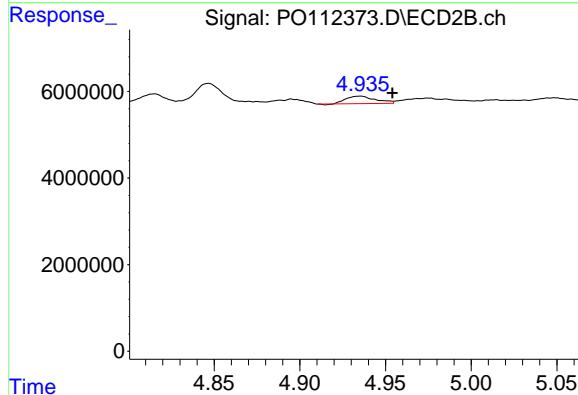


#5 AR-1016-3

R.T.: 4.935 min
Delta R.T.: -0.019 min
Response: 2009509
Conc: 11.83 ng/ml

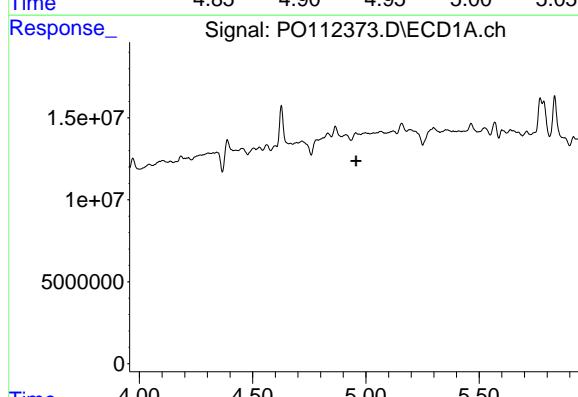


#6 AR-1016-4

R.T.: 4.956 min
Delta R.T.: 0.000 min
Response: -735652
Conc: N.D.

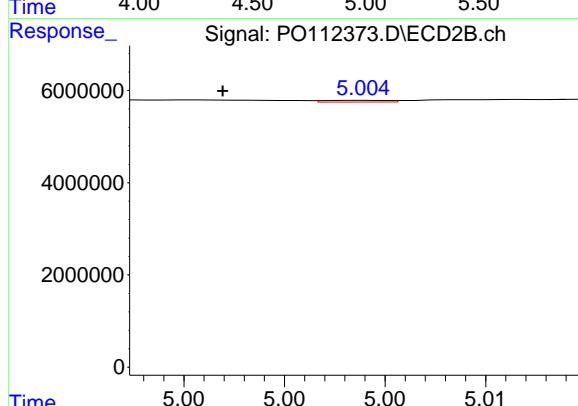

#6 AR-1016-4

R.T.: 5.004 min
Delta R.T.: 0.007 min
Response: 80051
Conc: 0.58 ng/ml

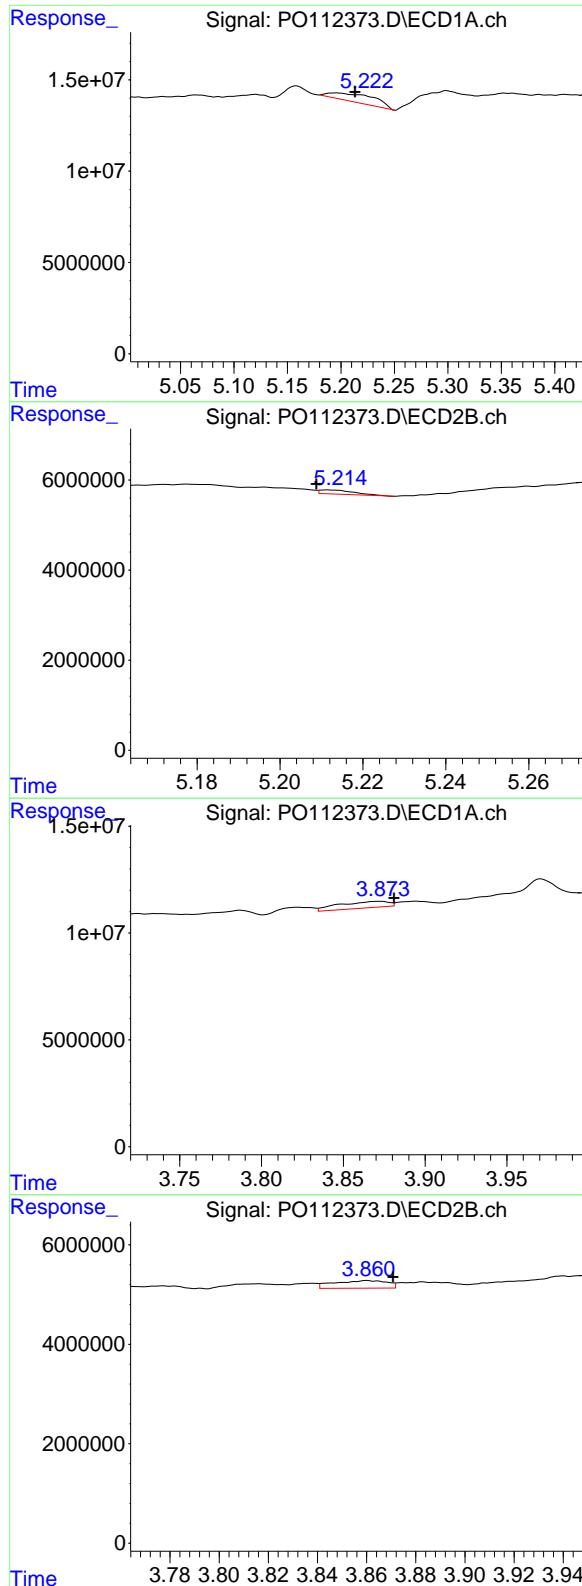

#7 AR-1016-5

R.T.: 5.196 min
 Delta R.T.: -0.017 min
 Response: 13300023
 Conc: 48.60 ng/ml

Instrument: ECD_O
 ClientSampleId : OU4-TS-43-071725

#7 AR-1016-5


R.T.: 5.212 min
 Delta R.T.: 0.003 min
 Response: 546515
 Conc: 3.17 ng/ml

#8 AR-1221-1

R.T.: 3.872 min
 Delta R.T.: -0.009 min
 Response: 6415151
 Conc: 55.01 ng/ml

#8 AR-1221-1

R.T.: 3.860 min
 Delta R.T.: -0.011 min
 Response: 2298237
 Conc: 27.93 ng/ml

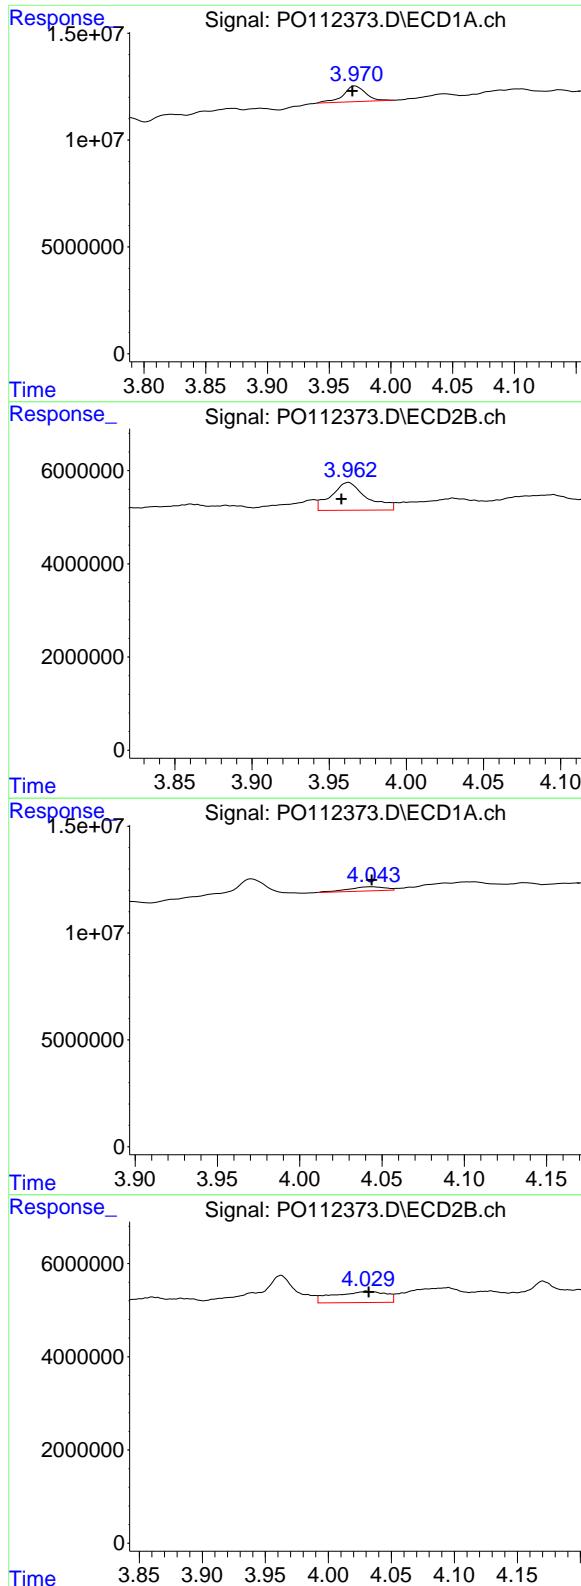

#9 AR-1221-2

R.T.: 3.971 min
 Delta R.T.: 0.002 min
 Response: 9158748
 Conc: 116.17 ng/ml

Instrument: ECD_O
 ClientSampleId: OU4-TS-43-071725

#9 AR-1221-2


R.T.: 3.963 min
 Delta R.T.: 0.005 min
 Response: 9563958
 Conc: 161.14 ng/ml

#10 AR-1221-3

R.T.: 4.044 min
 Delta R.T.: 0.000 min
 Response: 2932076
 Conc: 10.88 ng/ml

#10 AR-1221-3

R.T.: 4.030 min
 Delta R.T.: -0.002 min
 Response: 6951984
 Conc: 36.83 ng/ml

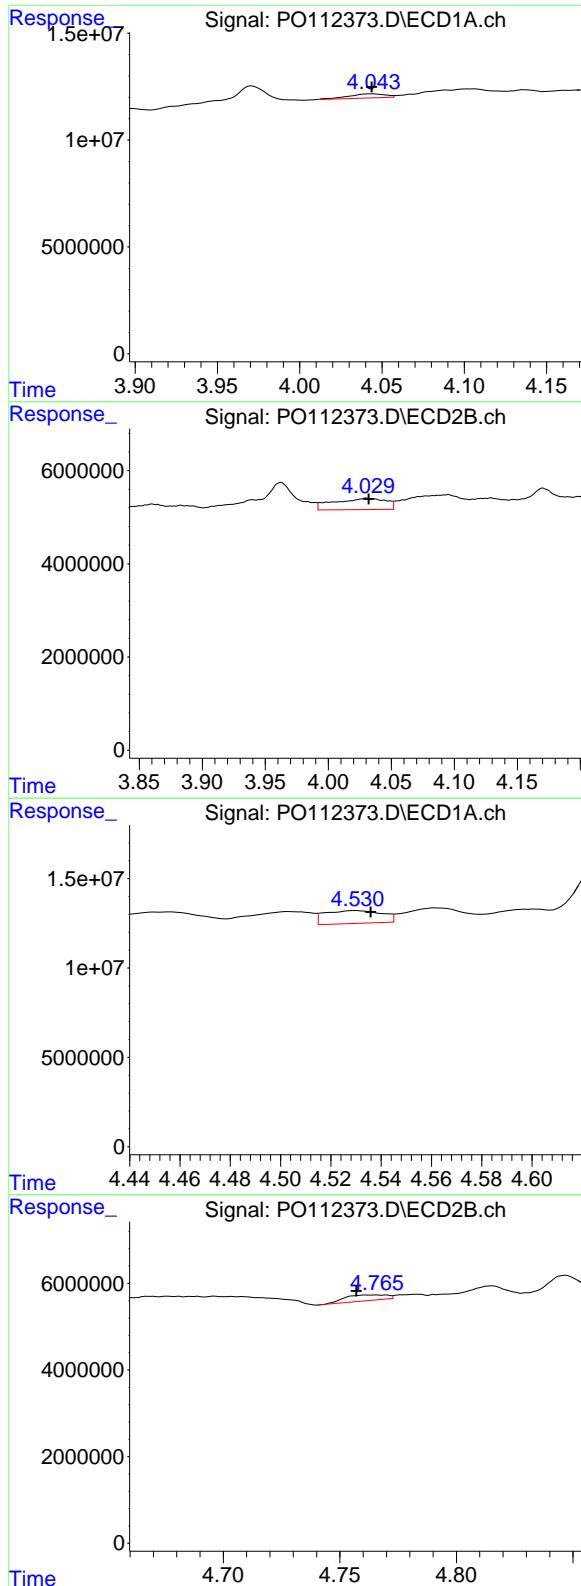

#11 AR-1232-1

R.T.: 4.044 min
 Delta R.T.: 0.000 min
 Response: 2932076
 Conc: 13.66 ng/ml

Instrument: ECD_O
 ClientSampleId: OU4-TS-43-071725

#11 AR-1232-1


R.T.: 4.030 min
 Delta R.T.: -0.002 min
 Response: 6951984
 Conc: 46.32 ng/ml

#12 AR-1232-2

R.T.: 4.530 min
 Delta R.T.: -0.006 min
 Response: 11325187
 Conc: 99.66 ng/ml

#12 AR-1232-2

R.T.: 4.766 min
 Delta R.T.: 0.008 min
 Response: 1682474
 Conc: 10.99 ng/ml

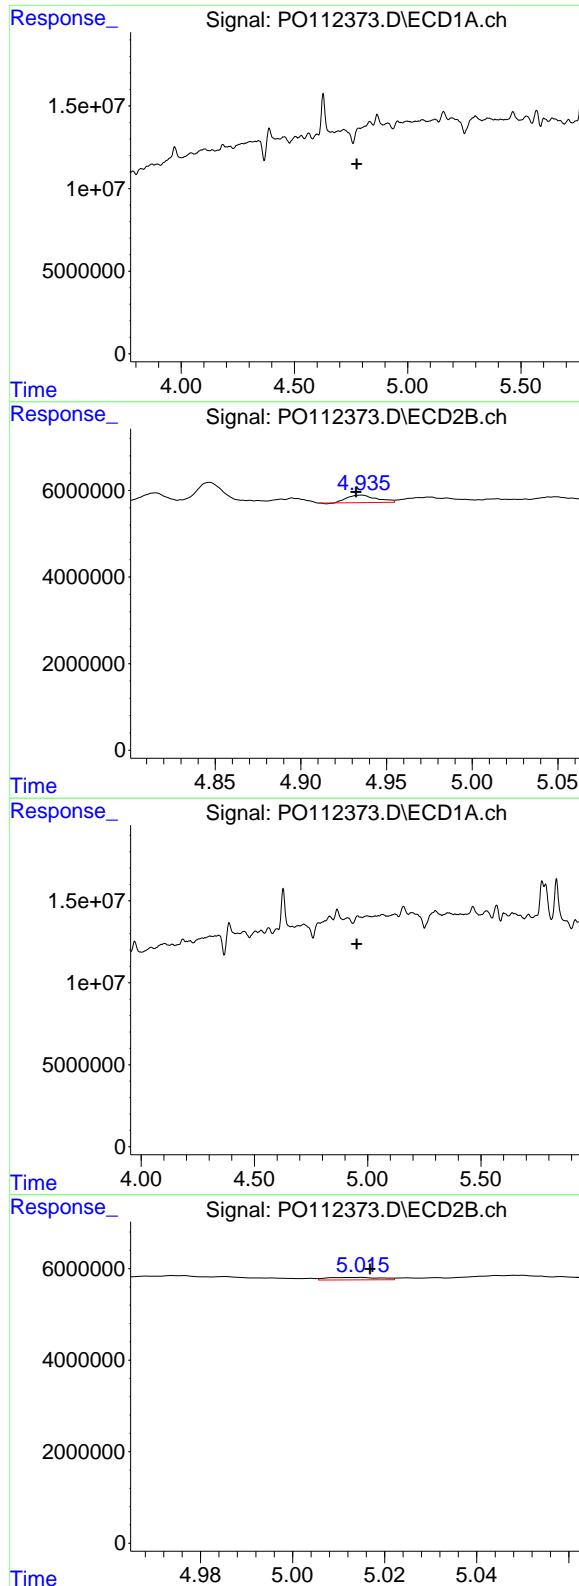

#13 AR-1232-3

R.T.: 4.785 min
 Delta R.T.: 0.009 min
 Response: -2917415
 Conc: N.D.

Instrument: ECD_O
ClientSampleId: OU4-TS-43-071725

#13 AR-1232-3


R.T.: 4.935 min
 Delta R.T.: 0.003 min
 Response: 2009509
 Conc: 26.61 ng/ml

#14 AR-1232-4

R.T.: 4.956 min
 Delta R.T.: 0.003 min
 Response: -735652
 Conc: N.D.

#14 AR-1232-4

R.T.: 5.015 min
 Delta R.T.: -0.002 min
 Response: 435339
 Conc: 6.60 ng/ml

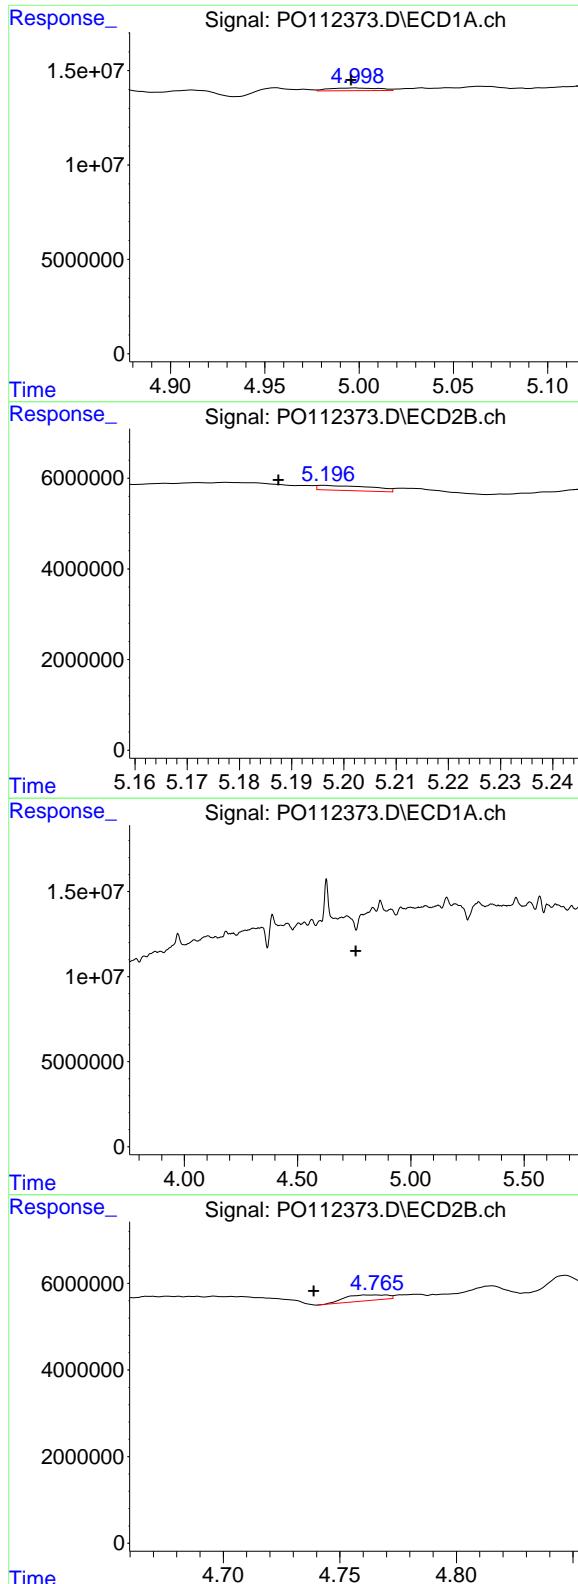

#15 AR-1232-5

R.T.: 4.998 min
 Delta R.T.: 0.002 min
 Response: 2764611
 Conc: 37.66 ng/ml

Instrument: ECD_O
 ClientSampleId: OU4-TS-43-071725

#15 AR-1232-5


R.T.: 5.196 min
 Delta R.T.: 0.009 min
 Response: 796399
 Conc: 10.72 ng/ml

#16 AR-1242-1

R.T.: 4.785 min
 Delta R.T.: 0.027 min
 Response: -2917415
 Conc: N.D.

#16 AR-1242-1

R.T.: 4.766 min
 Delta R.T.: 0.027 min
 Response: 1682474
 Conc: 8.68 ng/ml

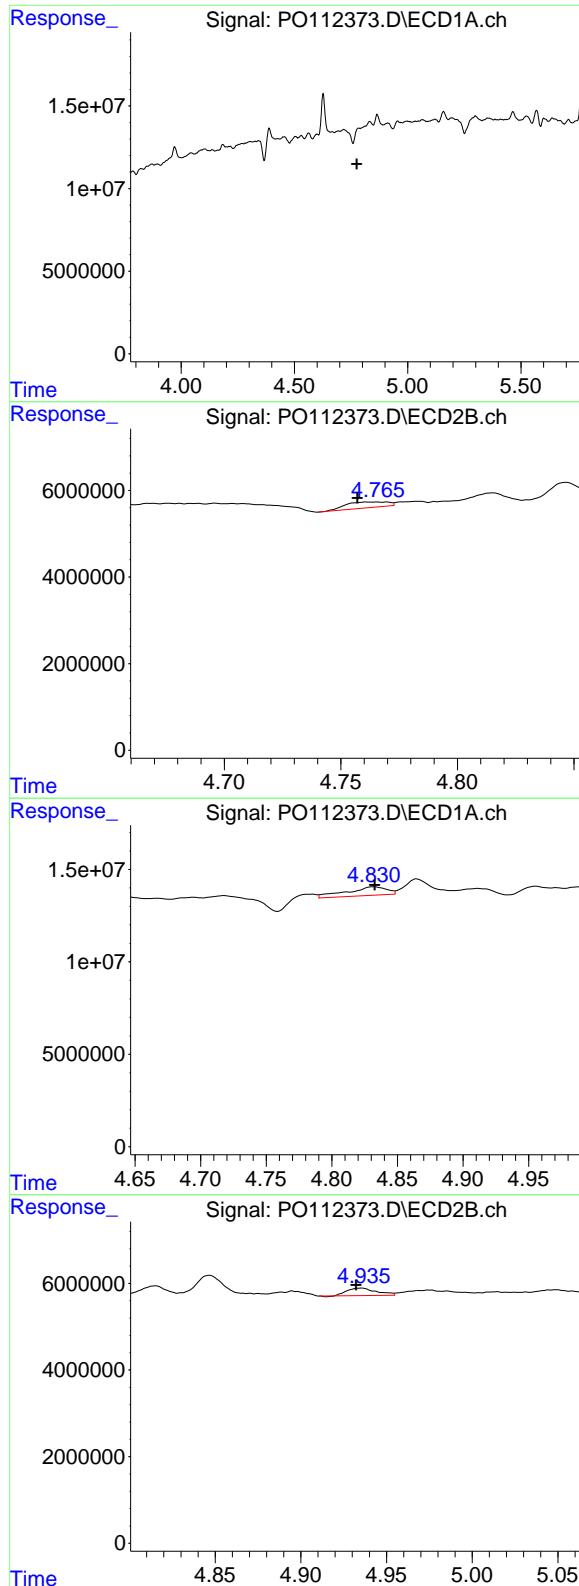

#17 AR-1242-2

R.T.: 4.785 min
 Delta R.T.: 0.009 min
 Response: -2917415
 Conc: N.D.

Instrument: ECD_O
ClientSampleId: OU4-TS-43-071725

#17 AR-1242-2





R.T.: 4.766 min
 Delta R.T.: 0.008 min
 Response: 1682474
 Conc: 5.94 ng/ml

#18 AR-1242-3

R.T.: 4.832 min
 Delta R.T.: 0.000 min
 Response: 9836742
 Conc: 35.94 ng/ml

#18 AR-1242-3

R.T.: 4.935 min
 Delta R.T.: 0.003 min
 Response: 2009509
 Conc: 13.79 ng/ml

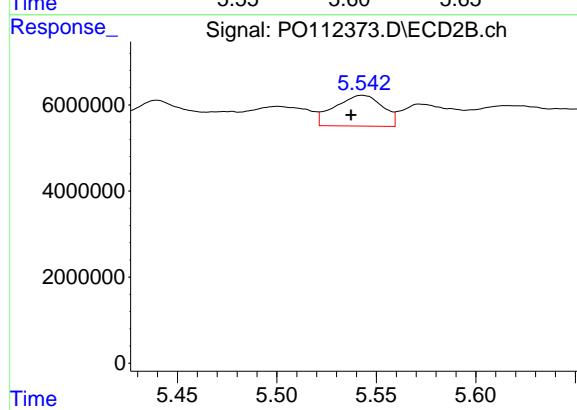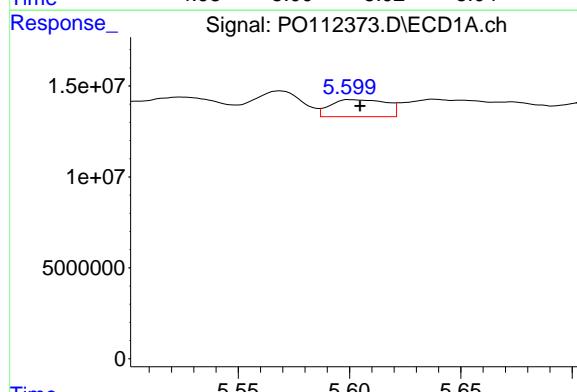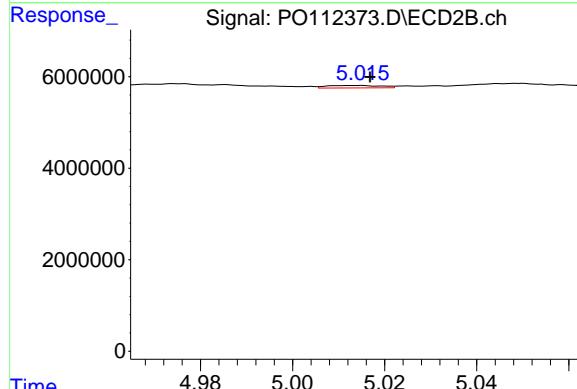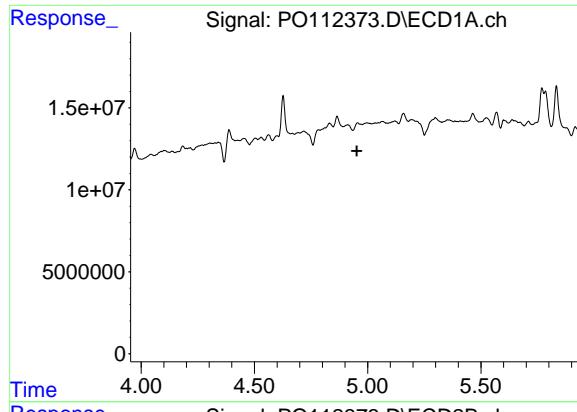

#19 AR-1242-4

R.T.: 4.956 min
 Delta R.T.: 0.003 min
 Response: -735652
 Conc: N.D.

Instrument: ECD_O
ClientSampleId : OU4-TS-43-071725

#19 AR-1242-4


R.T.: 5.015 min
 Delta R.T.: -0.002 min
 Response: 435339
 Conc: 3.07 ng/ml

#20 AR-1242-5

R.T.: 5.600 min
 Delta R.T.: -0.005 min
 Response: 16376015
 Conc: 77.37 ng/ml

#20 AR-1242-5

R.T.: 5.543 min
 Delta R.T.: 0.006 min
 Response: 11939197
 Conc: 65.70 ng/ml

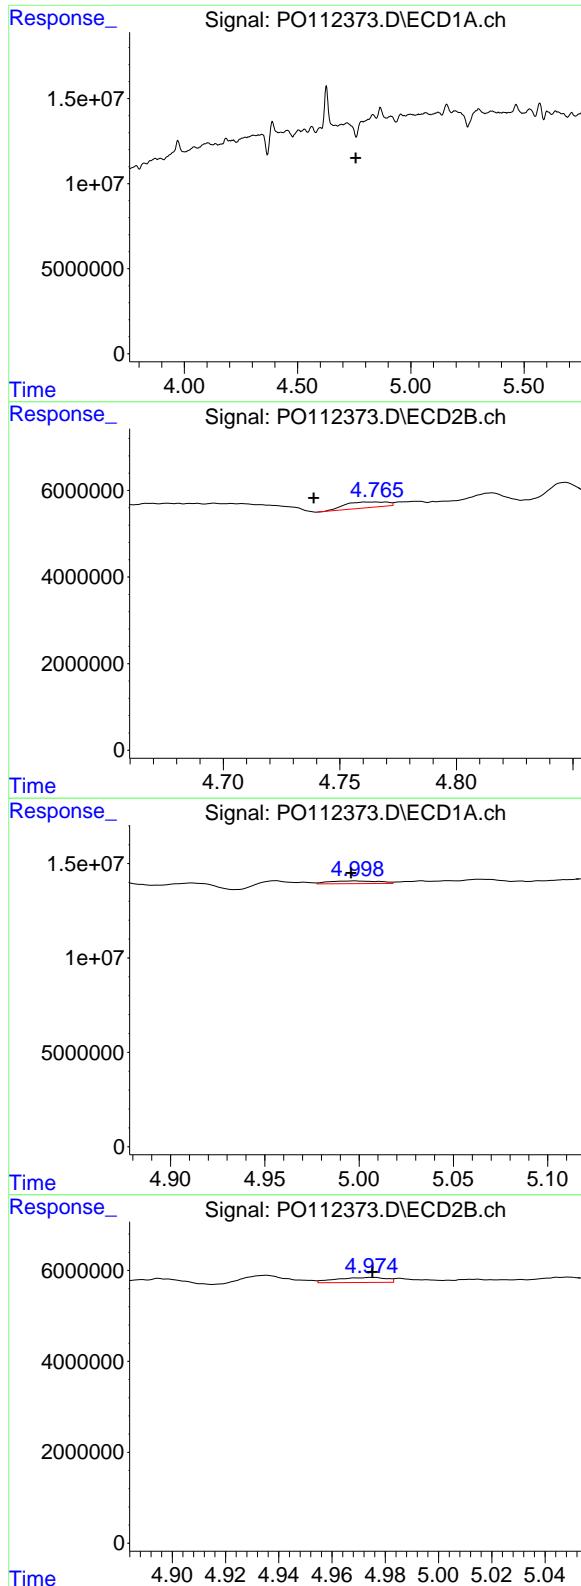

#21 AR-1248-1

R.T.: 4.785 min
 Delta R.T.: 0.027 min
 Response: -2917415
 Conc: N.D.

Instrument: ECD_O
ClientSampleId: OU4-TS-43-071725

#21 AR-1248-1


R.T.: 4.766 min
 Delta R.T.: 0.027 min
 Response: 1682474
 Conc: 10.90 ng/ml

#22 AR-1248-2

R.T.: 4.998 min
 Delta R.T.: 0.002 min
 Response: 2764611
 Conc: 8.97 ng/ml

#22 AR-1248-2

R.T.: 4.975 min
 Delta R.T.: 0.000 min
 Response: 1451854
 Conc: 7.06 ng/ml

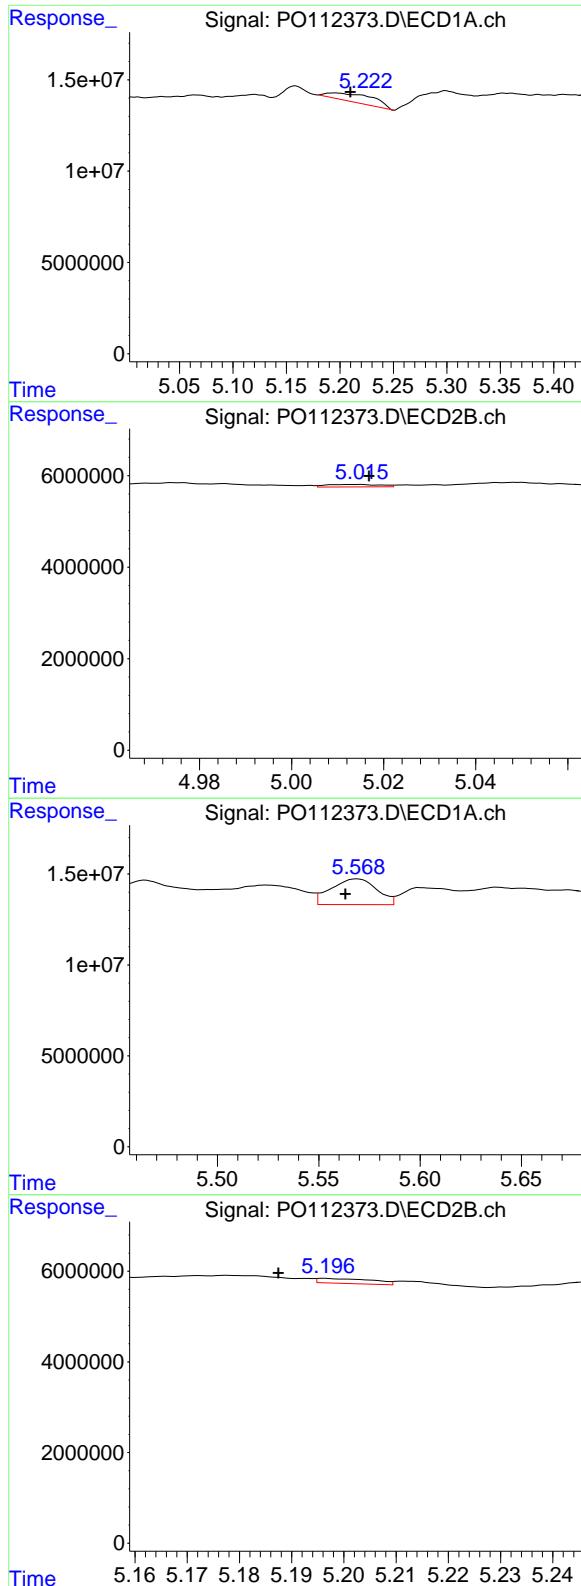

#23 AR-1248-3

R.T.: 5.196 min
 Delta R.T.: -0.014 min
 Response: 13300023
 Conc: 32.65 ng/ml

Instrument: ECD_O
 ClientSampleId: OU4-TS-43-071725

#23 AR-1248-3


R.T.: 5.015 min
 Delta R.T.: -0.002 min
 Response: 435339
 Conc: 2.03 ng/ml

#24 AR-1248-4

R.T.: 5.569 min
 Delta R.T.: 0.006 min
 Response: 22176832
 Conc: 38.42 ng/ml

#24 AR-1248-4

R.T.: 5.196 min
 Delta R.T.: 0.009 min
 Response: 796399
 Conc: 3.08 ng/ml

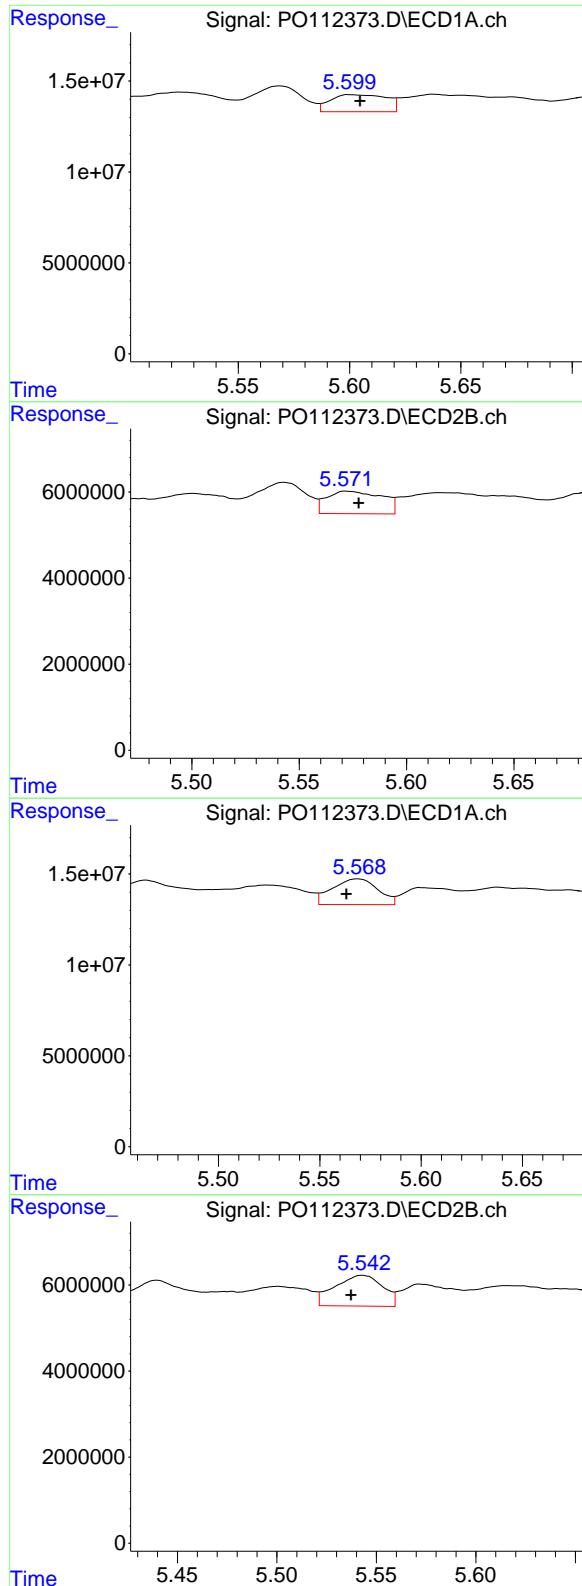

#25 AR-1248-5

R.T.: 5.600 min
 Delta R.T.: -0.005 min
 Response: 16376015
 Conc: 41.96 ng/ml

Instrument: ECD_O
 ClientSampleId : OU4-TS-43-071725

#25 AR-1248-5


R.T.: 5.571 min
 Delta R.T.: -0.006 min
 Response: 9354361
 Conc: 37.34 ng/ml

#26 AR-1254-1

R.T.: 5.569 min
 Delta R.T.: 0.006 min
 Response: 22176832
 Conc: 36.05 ng/ml

#26 AR-1254-1

R.T.: 5.543 min
 Delta R.T.: 0.006 min
 Response: 11939197
 Conc: 31.32 ng/ml

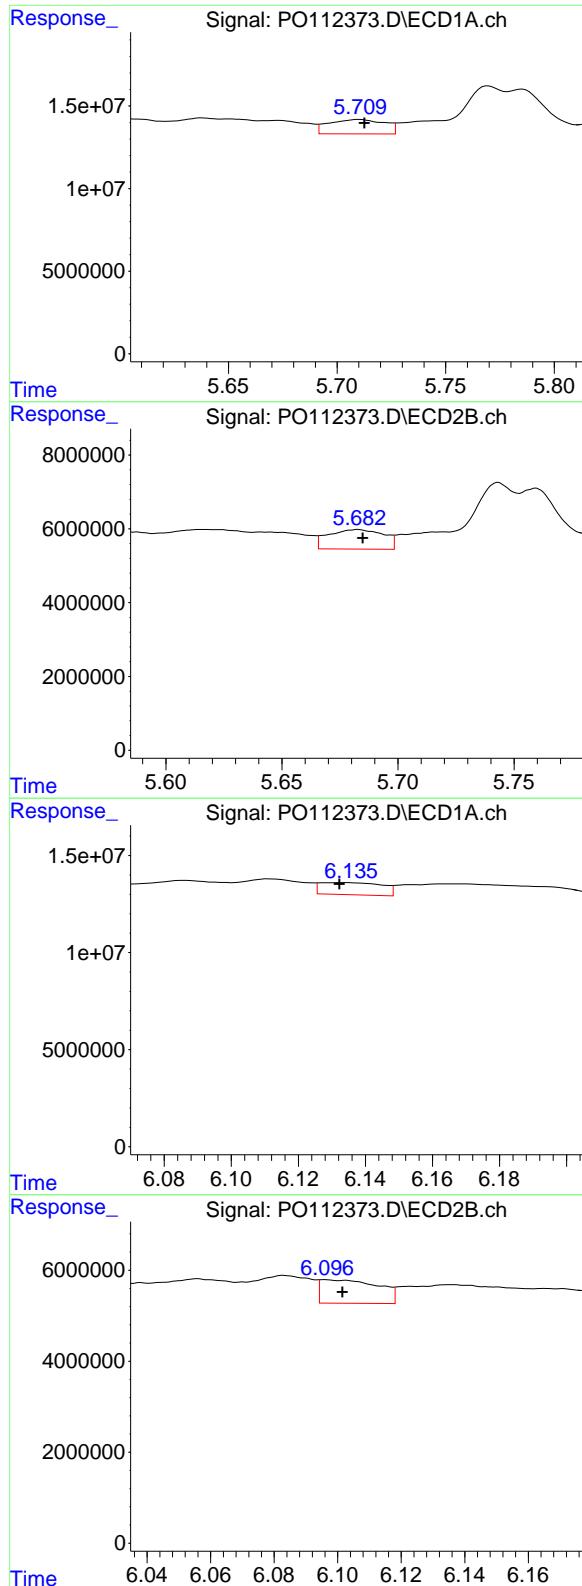

#27 AR-1254-2

R.T.: 5.710 min
 Delta R.T.: -0.002 min
 Response: 15605025
 Conc: 29.13 ng/ml

Instrument: ECD_O
 ClientSampleId: OU4-TS-43-071725

#27 AR-1254-2


R.T.: 5.683 min
 Delta R.T.: -0.002 min
 Response: 8781774
 Conc: 26.47 ng/ml

#28 AR-1254-3

R.T.: 6.134 min
 Delta R.T.: 0.002 min
 Response: 8022042
 Conc: 9.55 ng/ml

#28 AR-1254-3

R.T.: 6.096 min
 Delta R.T.: -0.005 min
 Response: 6503916
 Conc: 13.49 ng/ml

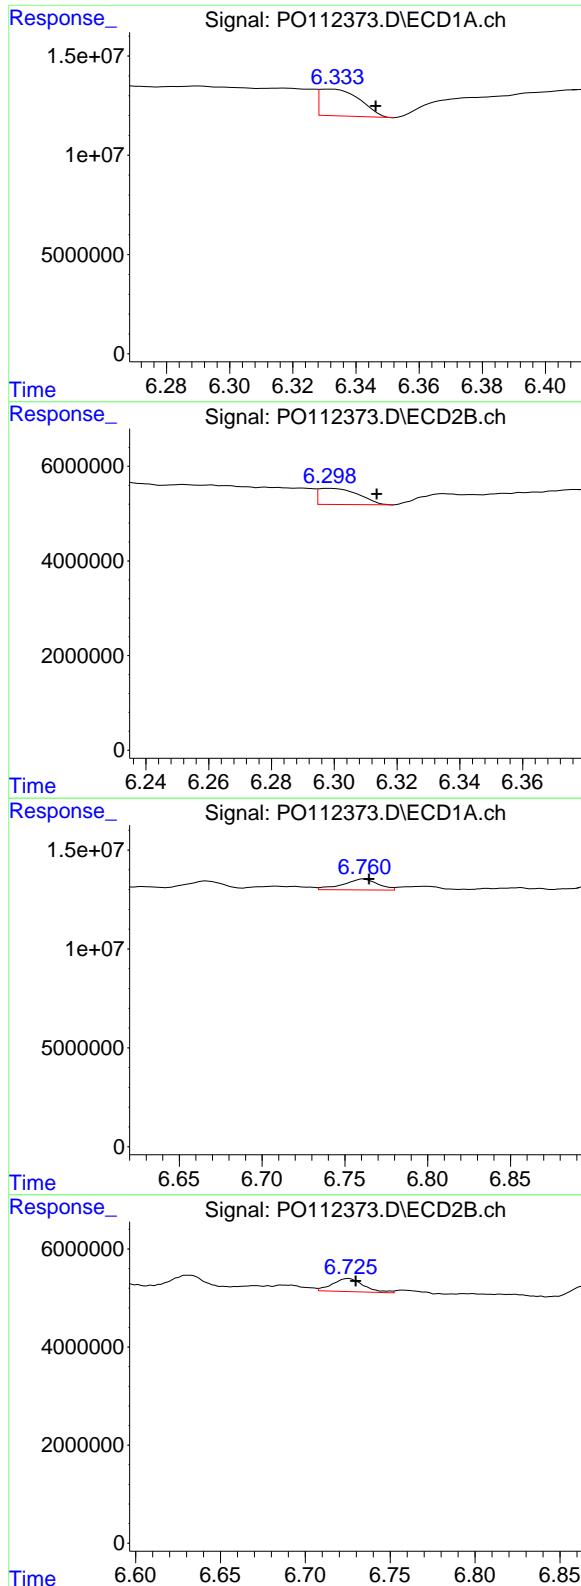

#29 AR-1254-4

R.T.: 6.332 min
 Delta R.T.: -0.014 min
 Response: 12064042
 Conc: 25.08 ng/ml

Instrument: ECD_O
ClientSampleId: OU4-TS-43-071725

#29 AR-1254-4


R.T.: 6.298 min
 Delta R.T.: -0.015 min
 Response: 2984702
 Conc: 11.45 ng/ml

#30 AR-1254-5

R.T.: 6.761 min
 Delta R.T.: -0.003 min
 Response: 8164834
 Conc: 10.55 ng/ml

#30 AR-1254-5

R.T.: 6.725 min
 Delta R.T.: -0.004 min
 Response: 3373459
 Conc: 9.47 ng/ml

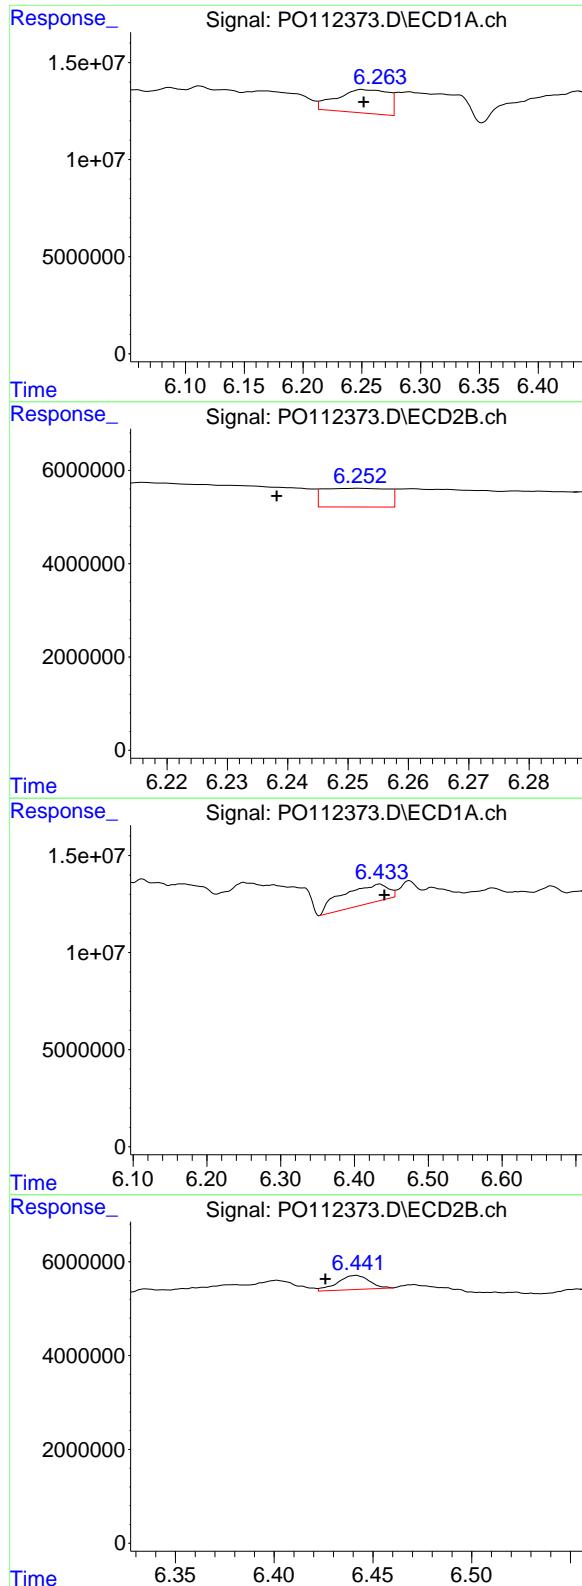

#31 AR-1260-1

R.T.: 6.250 min
 Delta R.T.: -0.002 min
 Response: 36774403
 Conc: 73.37 ng/ml

Instrument: ECD_O
 ClientSampleId : OU4-TS-43-071725

#31 AR-1260-1


R.T.: 6.252 min
 Delta R.T.: 0.014 min
 Response: 2989170
 Conc: 10.65 ng/ml

#32 AR-1260-2

R.T.: 6.434 min
 Delta R.T.: -0.007 min
 Response: 43025789
 Conc: 58.29 ng/ml

#32 AR-1260-2

R.T.: 6.441 min
 Delta R.T.: 0.015 min
 Response: 3264350
 Conc: 9.60 ng/ml

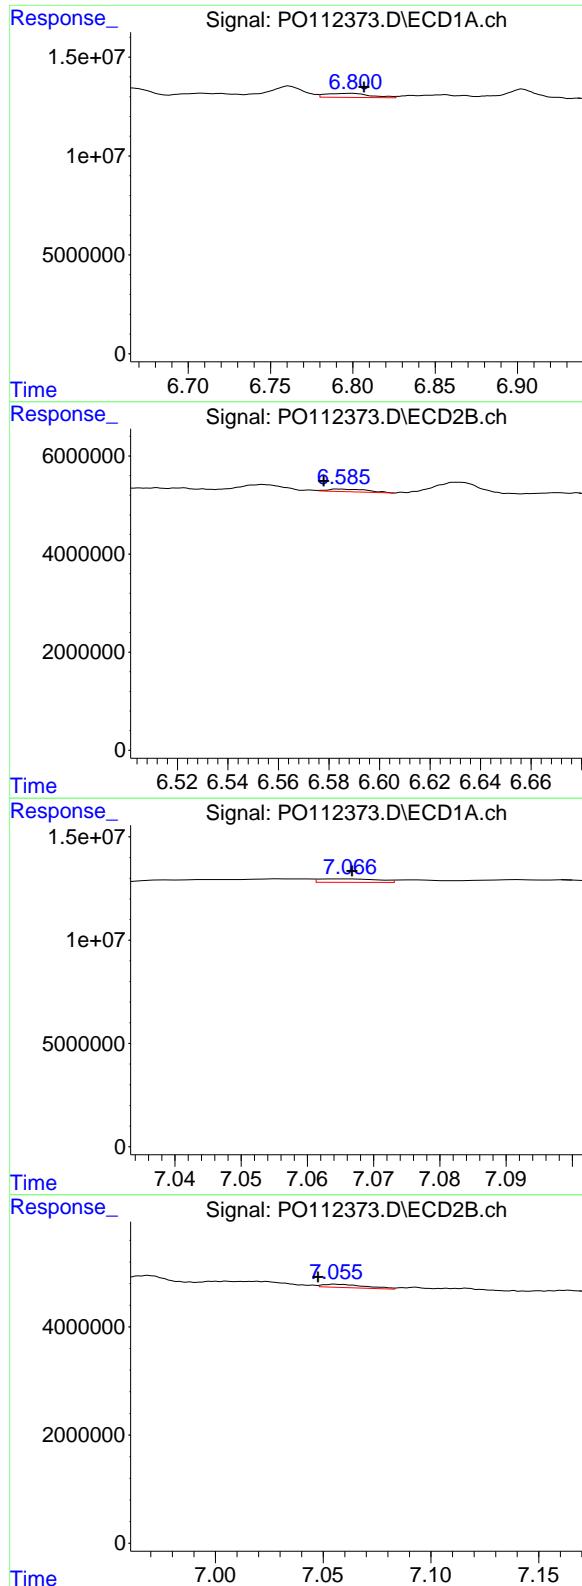

#33 AR-1260-3

R.T.: 6.799 min
 Delta R.T.: -0.008 min
 Response: 3908110
 Conc: 5.96 ng/ml

Instrument: ECD_O
 ClientSampleId : OU4-TS-43-071725

#33 AR-1260-3


R.T.: 6.583 min
 Delta R.T.: 0.005 min
 Response: 586698
 Conc: 2.13 ng/ml

#34 AR-1260-4

R.T.: 7.065 min
 Delta R.T.: -0.001 min
 Response: 1069848
 Conc: 2.46 ng/ml

#34 AR-1260-4

R.T.: 7.055 min
 Delta R.T.: 0.007 min
 Response: 844445
 Conc: 4.21 ng/ml

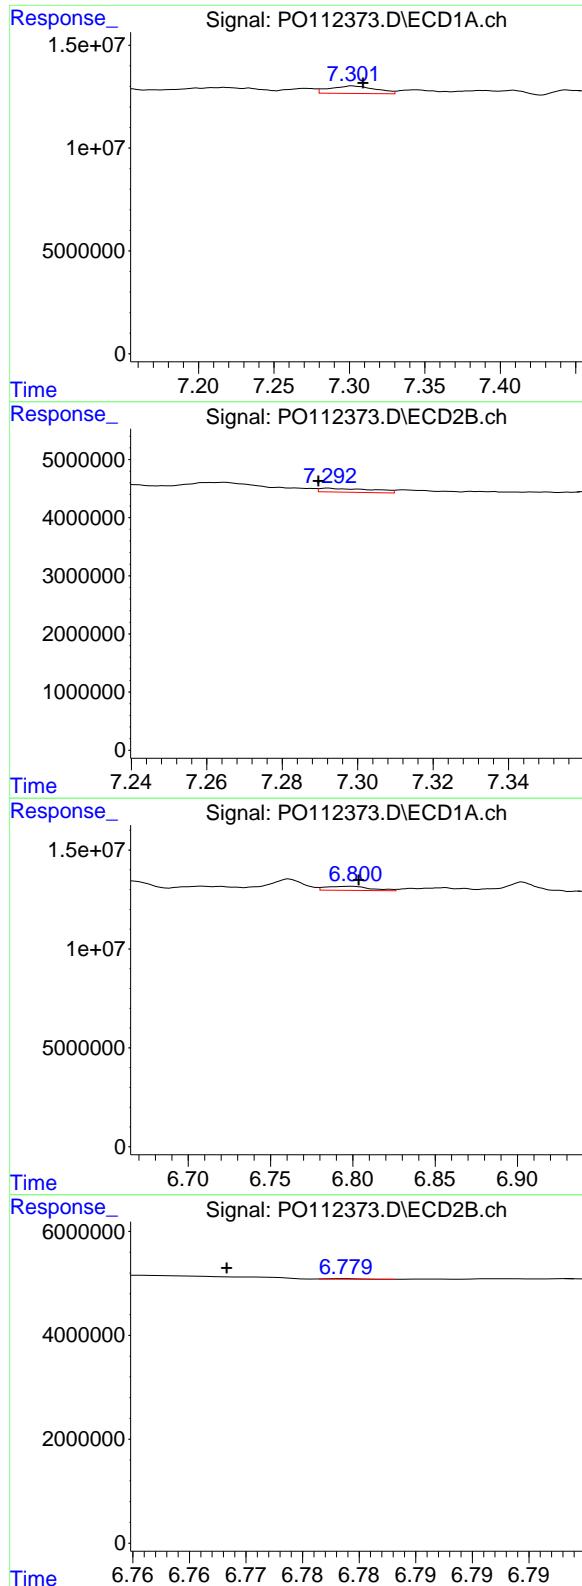

#35 AR-1260-5

R.T.: 7.302 min
 Delta R.T.: -0.007 min
 Response: 7752788
 Conc: 6.14 ng/ml

Instrument: ECD_O
 ClientSampleId: OU4-TS-43-071725

#35 AR-1260-5


R.T.: 7.292 min
 Delta R.T.: 0.003 min
 Response: 644749
 Conc: 1.44 ng/ml

#36 AR-1262-1

R.T.: 6.799 min
 Delta R.T.: -0.005 min
 Response: 3908110
 Conc: 3.83 ng/ml

#36 AR-1262-1

R.T.: 6.779 min
 Delta R.T.: 0.011 min
 Response: 19892
 Conc: 0.05 ng/ml

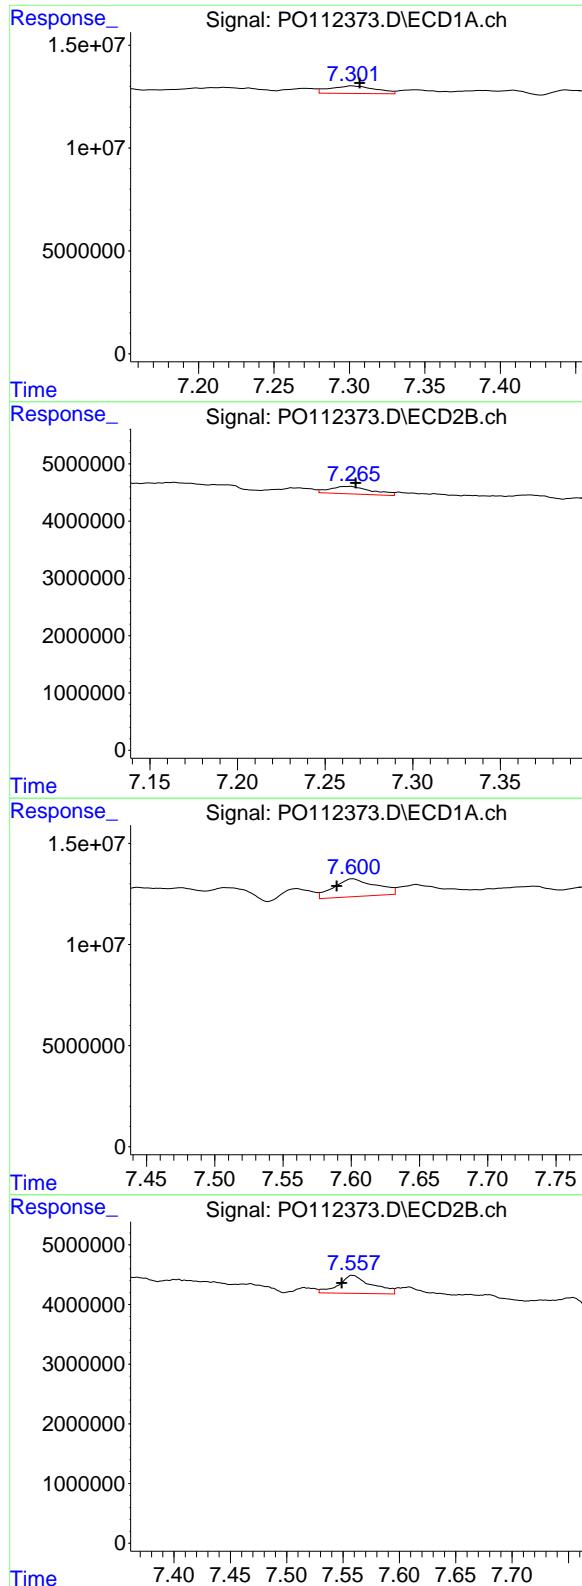

#37 AR-1262-2

R.T.: 7.302 min
 Delta R.T.: -0.005 min
 Response: 7752788
 Conc: 4.73 ng/ml

Instrument: ECD_O
 ClientSampleId: OU4-TS-43-071725

#37 AR-1262-2


R.T.: 7.265 min
 Delta R.T.: -0.003 min
 Response: 2150057
 Conc: 4.19 ng/ml

#38 AR-1262-3

R.T.: 7.601 min
 Delta R.T.: 0.012 min
 Response: 18790082
 Conc: 29.27 ng/ml

#38 AR-1262-3

R.T.: 7.558 min
 Delta R.T.: 0.009 min
 Response: 6190981
 Conc: 34.49 ng/ml

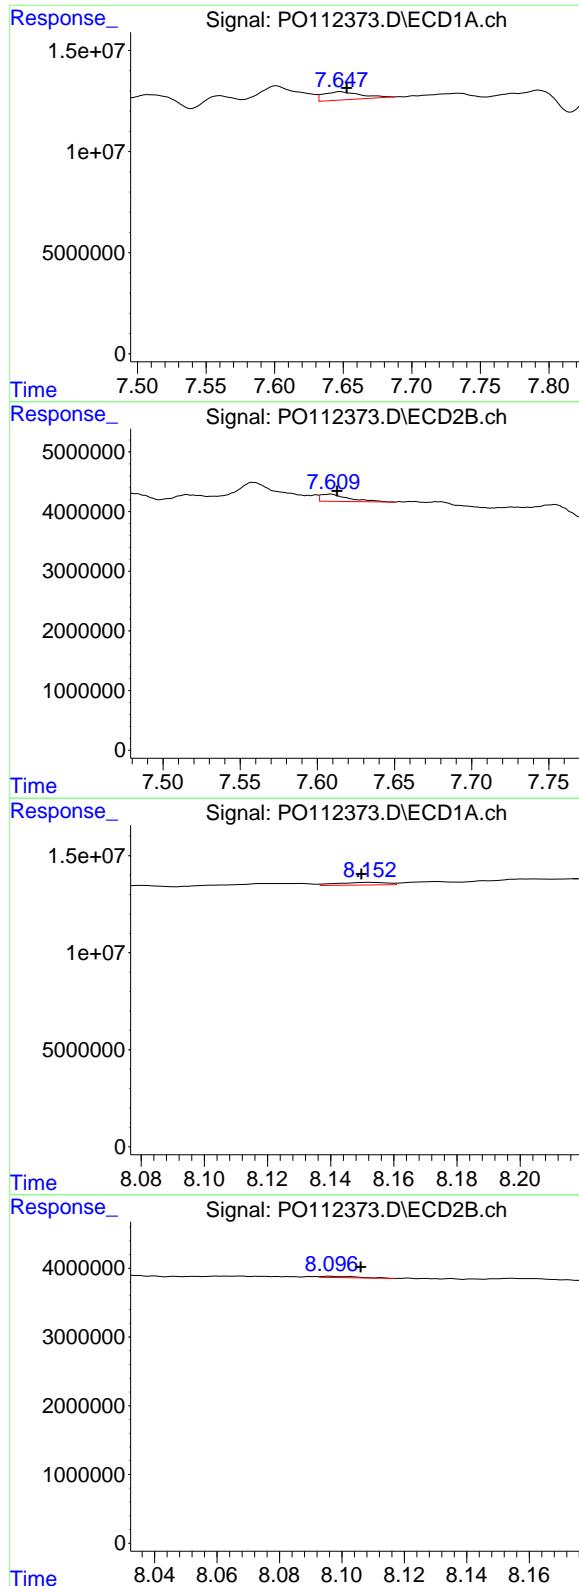

#39 AR-1262-4

R.T.: 7.648 min
 Delta R.T.: -0.005 min
 Response: 7593807
 Conc: 7.09 ng/ml

Instrument: ECD_O
 ClientSampleId: OU4-TS-43-071725

#39 AR-1262-4


R.T.: 7.609 min
 Delta R.T.: -0.004 min
 Response: 1482669
 Conc: 5.10 ng/ml

#40 AR-1262-5

R.T.: 8.152 min
 Delta R.T.: 0.003 min
 Response: 1483311
 Conc: 3.31 ng/ml

#40 AR-1262-5

R.T.: 8.096 min
 Delta R.T.: -0.010 min
 Response: 148000
 Conc: 1.40 ng/ml

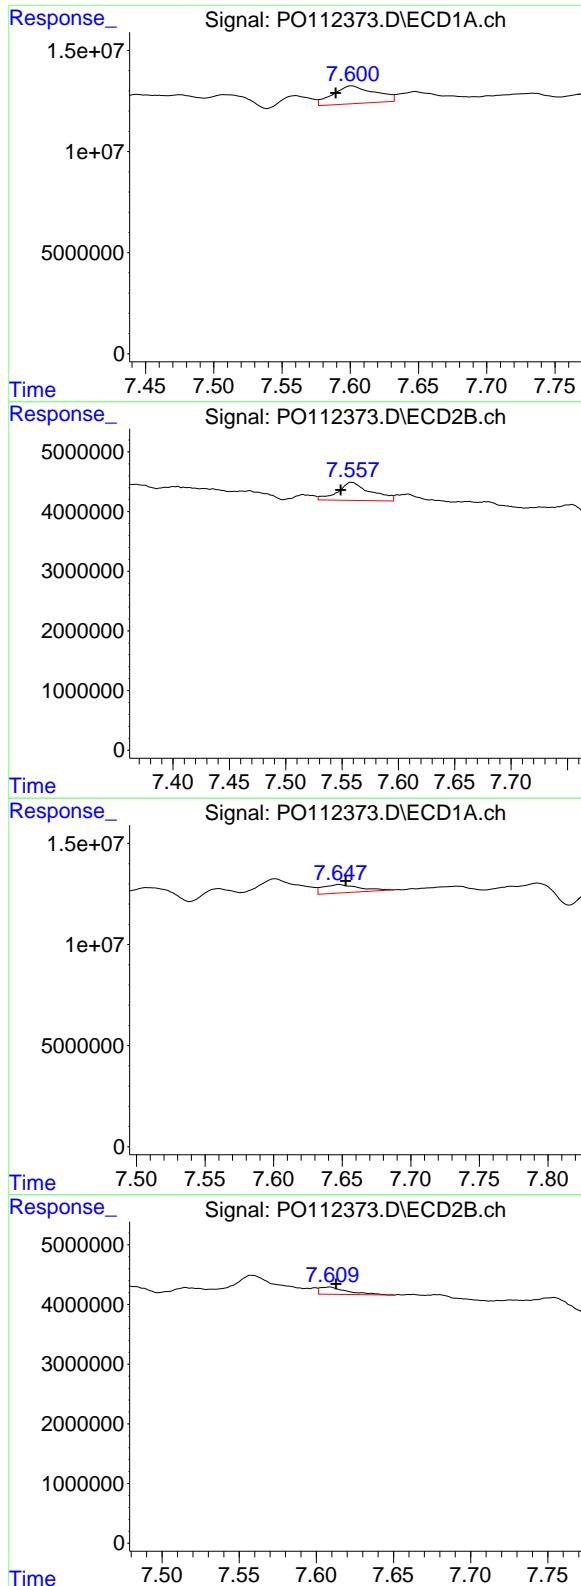

#41 AR-1268-1

R.T.: 7.601 min
 Delta R.T.: 0.012 min
 Response: 18790082
 Conc: 10.23 ng/ml

Instrument: ECD_O
ClientSampleId: OU4-TS-43-071725

#41 AR-1268-1


R.T.: 7.558 min
 Delta R.T.: 0.009 min
 Response: 6190981
 Conc: 12.60 ng/ml

#42 AR-1268-2

R.T.: 7.648 min
 Delta R.T.: -0.005 min
 Response: 7593807
 Conc: 4.88 ng/ml

#42 AR-1268-2

R.T.: 7.609 min
 Delta R.T.: -0.004 min
 Response: 1482669
 Conc: 3.55 ng/ml

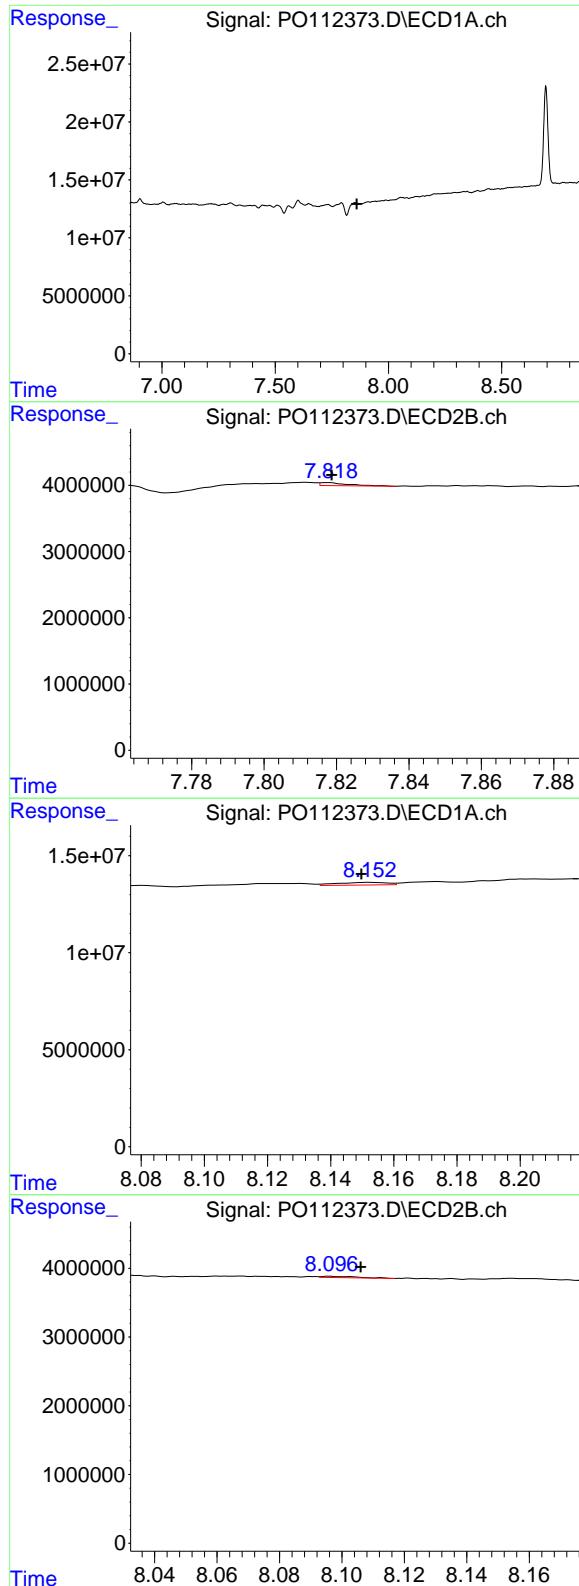

#43 AR-1268-3

R.T.: 7.852 min
 Delta R.T.: -0.008 min
 Response: -6079304
 Conc: N.D.

Instrument: ECD_O
ClientSampleId : OU4-TS-43-071725

#43 AR-1268-3


R.T.: 7.818 min
 Delta R.T.: 0.000 min
 Response: 247954
 Conc: 0.78 ng/ml

#44 AR-1268-4

R.T.: 8.152 min
 Delta R.T.: 0.003 min
 Response: 1483311
 Conc: 3.09 ng/ml

#44 AR-1268-4

R.T.: 8.096 min
 Delta R.T.: -0.010 min
 Response: 148000
 Conc: 1.33 ng/ml

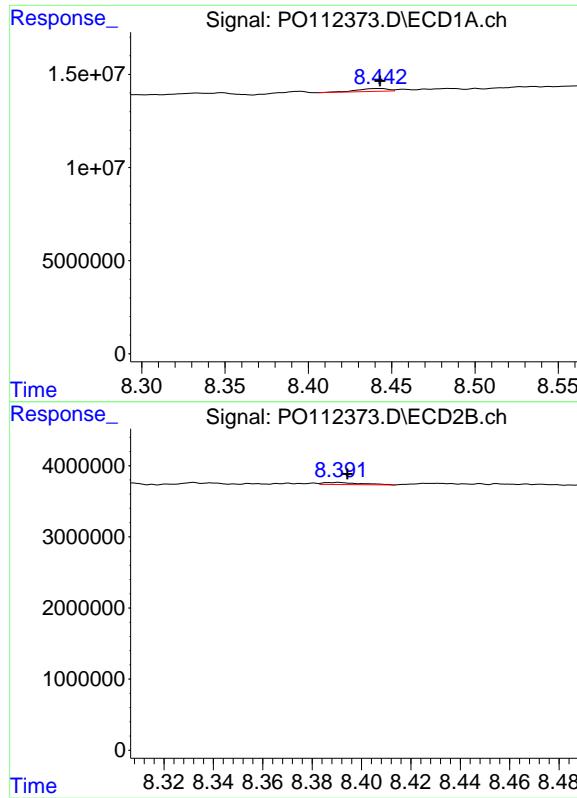

#45 AR-1268-5

R.T.: 8.443 min
Delta R.T.: 0.000 min
Response: 2022144
Conc: 0.62 ng/ml

Instrument: ECD_O
ClientSampleId: OU4-TS-43-071725

#45 AR-1268-5

R.T.: 8.391 min
Delta R.T.: -0.003 min
Response: 319590
Conc: 0.44 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0072225\
 Data File : P0112381.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Jul 2025 16:21
 Operator : YP/AJ
 Sample : AR1660CCC500
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1660CCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 23 01:52:11 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 22 09:14:26 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	3.670	3.662	578.5E6	338.2E6	58.470	53.081
2) SA Decachlor...	8.695	8.642	338.8E6	80859360	49.551	46.917

Target Compounds

3) L1 AR-1016-1	4.756	4.756	180.9E6	145.2E6	531.757	651.446
4) L1 AR-1016-2	4.775	4.788	267.5E6	2118165	537.929	6.436 #
5) L1 AR-1016-3	4.832	4.974	167.8E6	65031858	518.228	382.840 #
6) L1 AR-1016-4	4.951	5.016	135.3E6	78356304	526.679	570.996
7) L1 AR-1016-5	5.209	5.226	150.3E6	34466083	549.172	199.861 #
8) L2 AR-1221-1	3.880	3.871	18239399	11668776	156.408	141.792
9) L2 AR-1221-2	3.968	3.957	24438120	17263867	309.969	290.865
10) L2 AR-1221-3	4.043	4.031	96368419	62424512	357.474	330.679
11) L3 AR-1232-1	4.043	4.031	96368419	62424512	448.919	415.888
12) L3 AR-1232-2	4.535	4.756	138.2E6	145.2E6	1215.807	948.256
13) L3 AR-1232-3	4.775	4.931	267.5E6	81132873	1168.111	1074.522
14) L3 AR-1232-4	4.951	5.016	135.3E6	78356304	1183.332	1187.429
15) L3 AR-1232-5	4.994	5.186	102.4E6	87512117	1394.546	1178.457
16) L4 AR-1242-1	4.756	4.738	180.9E6	102.3E6	624.447	527.854
17) L4 AR-1242-2	4.775	4.756	267.5E6	145.2E6	628.071	512.311
18) L4 AR-1242-3	4.832	4.931	167.8E6	81132873	612.958	556.936
19) L4 AR-1242-4	4.951	5.016	135.3E6	78356304	600.267	552.425
20) L4 AR-1242-5	5.604	5.536	39800546	86773714	188.030	477.476 #
21) L5 AR-1248-1	4.756	4.738	180.9E6	102.3E6	797.104	662.889
22) L5 AR-1248-2	4.994	4.974	102.4E6	65031858	331.987	316.045
23) L5 AR-1248-3	5.209	5.016	150.3E6	78356304	368.967	364.790
24) L5 AR-1248-4	5.562	5.186	147.0E6	87512117	254.644	338.241 #
25) L5 AR-1248-5	5.604	5.576	39800546	25069754	101.973	100.059
26) L6 AR-1254-1	5.562	5.536	147.0E6	86773714	238.927	227.652
27) L6 AR-1254-2	5.711	5.684	105.7E6	62838205	197.308	189.379
28) L6 AR-1254-3	6.131	6.100	194.9E6	108.0E6	232.105	224.084
29) L6 AR-1254-4	6.344	6.312	28936254	15324206	60.156	58.782
30) L6 AR-1254-5	6.762	6.727	319.7E6	146.2E6	413.050	410.365
31) L7 AR-1260-1	6.246	6.215	244.7E6	135.1E6	488.228	481.696
32) L7 AR-1260-2	6.436	6.404	360.4E6	169.8E6	488.264	499.283
33) L7 AR-1260-3	6.801	6.554	313.3E6	87394780	477.962	317.123 #
34) L7 AR-1260-4	7.061	7.059	219.4E6	11069571	504.145	55.170 #
35) L7 AR-1260-5	7.304	7.266	633.5E6	205.6E6	501.754	459.271
36) L8 AR-1262-1	6.801	6.766	313.3E6	135.3E6	306.646	332.127
37) L8 AR-1262-2	7.304	7.266	633.5E6	205.6E6	386.418	401.189
38) L8 AR-1262-3	7.586	7.547	150.8E6	44908619	234.902	250.154
39) L8 AR-1262-4	7.649	7.611	404.9E6	112.6E6	377.891	387.117
40) L8 AR-1262-5	8.147	8.104	133.4E6	31930474	297.619	301.847
41) L9 AR-1268-1	7.586	7.547	150.8E6	44908619	82.071	91.379

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0072225\
 Data File : P0112381.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Jul 2025 16:21
 Operator : YP/AJ
 Sample : AR1660CCC500
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1660CCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 23 01:52:11 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 22 09:14:26 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9 AR-1268-2	7.649	7.611	404.9E6	112.6E6	259.941	269.951
43) L9 AR-1268-3	7.858	7.815	5775100	1744375	4.443	5.513
44) L9 AR-1268-4	8.147	8.104	133.4E6	31930474	277.629	286.341
45) L9 AR-1268-5	8.441	8.391	31825405	7796084	9.751	10.731



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0072225\
 Data File : P0112381.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Jul 2025 16:21
 Operator : YP/AJ
 Sample : AR1660CCC500
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1660CCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 23 01:52:11 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 22 09:14:26 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

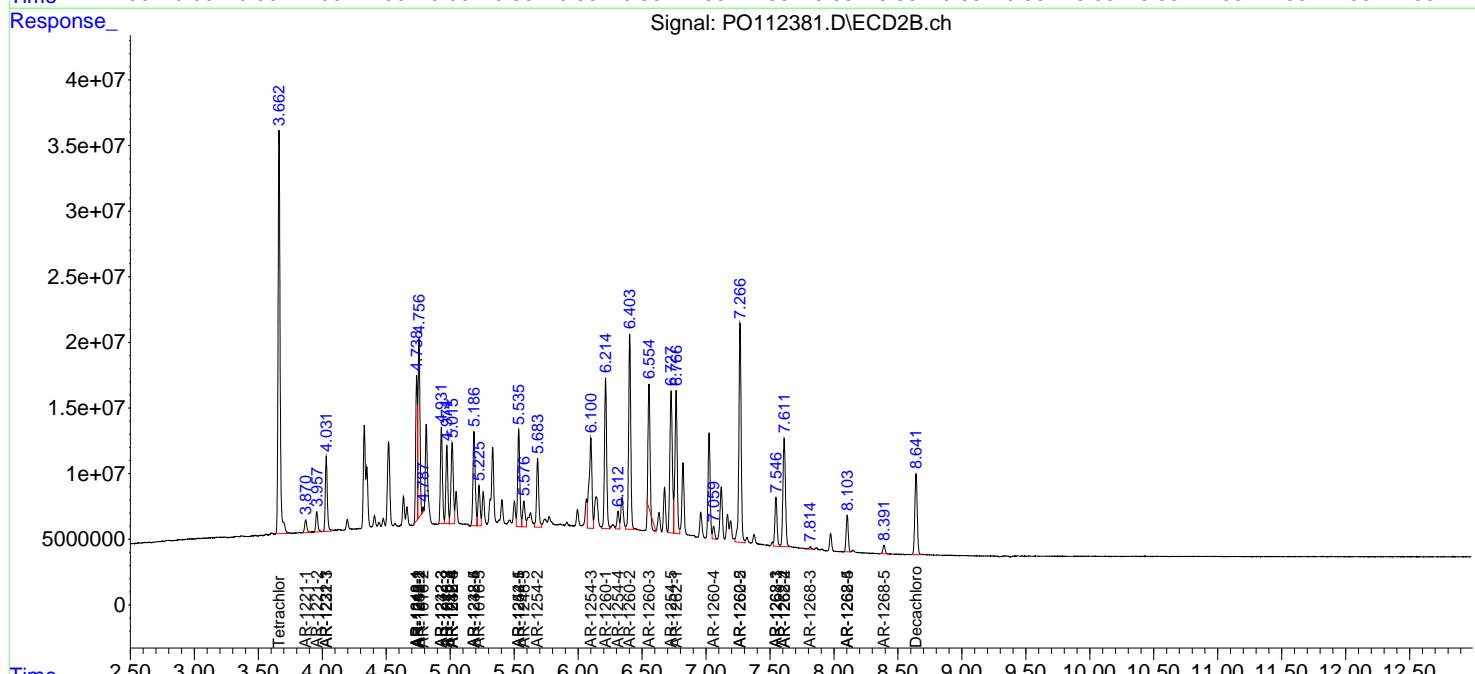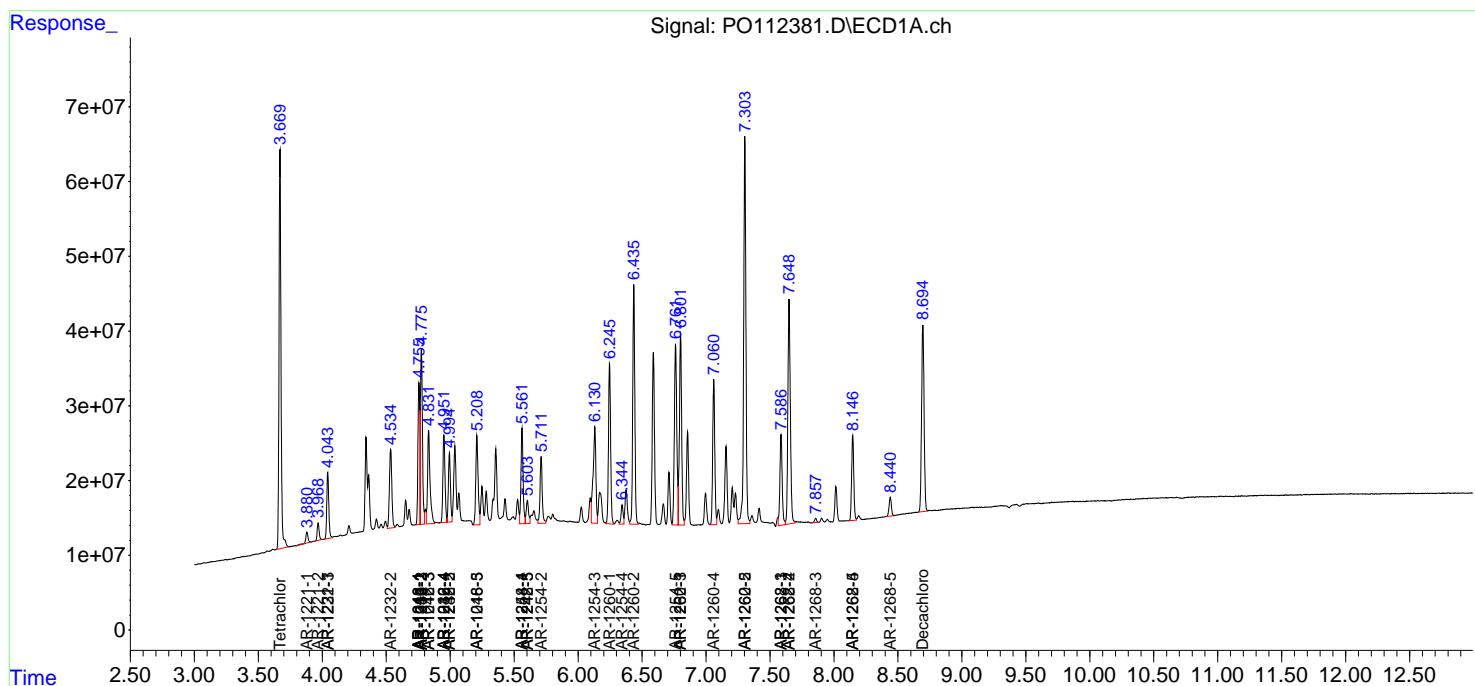

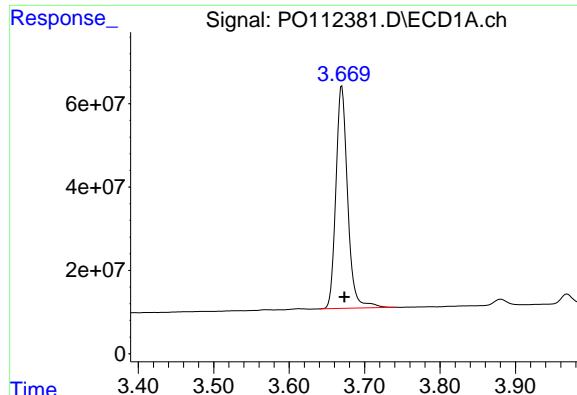

#1 Tetrachloro-m-xylene


R.T.: 3.670 min
Delta R.T.: -0.003 min
Response: 578547123
Conc: 58.47 ng/ml

Instrument:

ECD_O


ClientSampleId :

AR1660CCC500

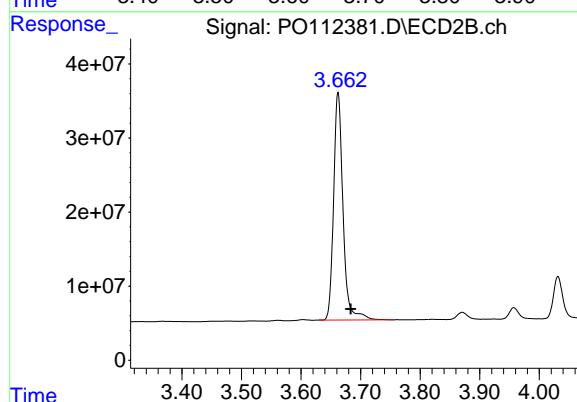


#1 Tetrachloro-m-xylene

R.T.: 3.662 min
Delta R.T.: -0.021 min
Response: 338183063
Conc: 53.08 ng/ml

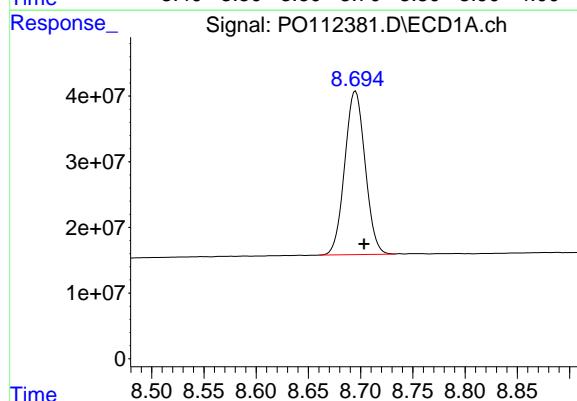


#2 Decachlorobiphenyl

R.T.: 8.695 min
Delta R.T.: -0.008 min
Response: 338782695
Conc: 49.55 ng/ml

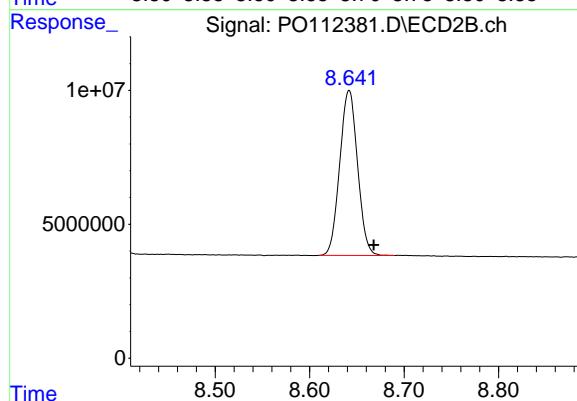

#2 Decachlorobiphenyl

R.T.: 8.642 min
Delta R.T.: -0.026 min
Response: 80859360
Conc: 46.92 ng/ml

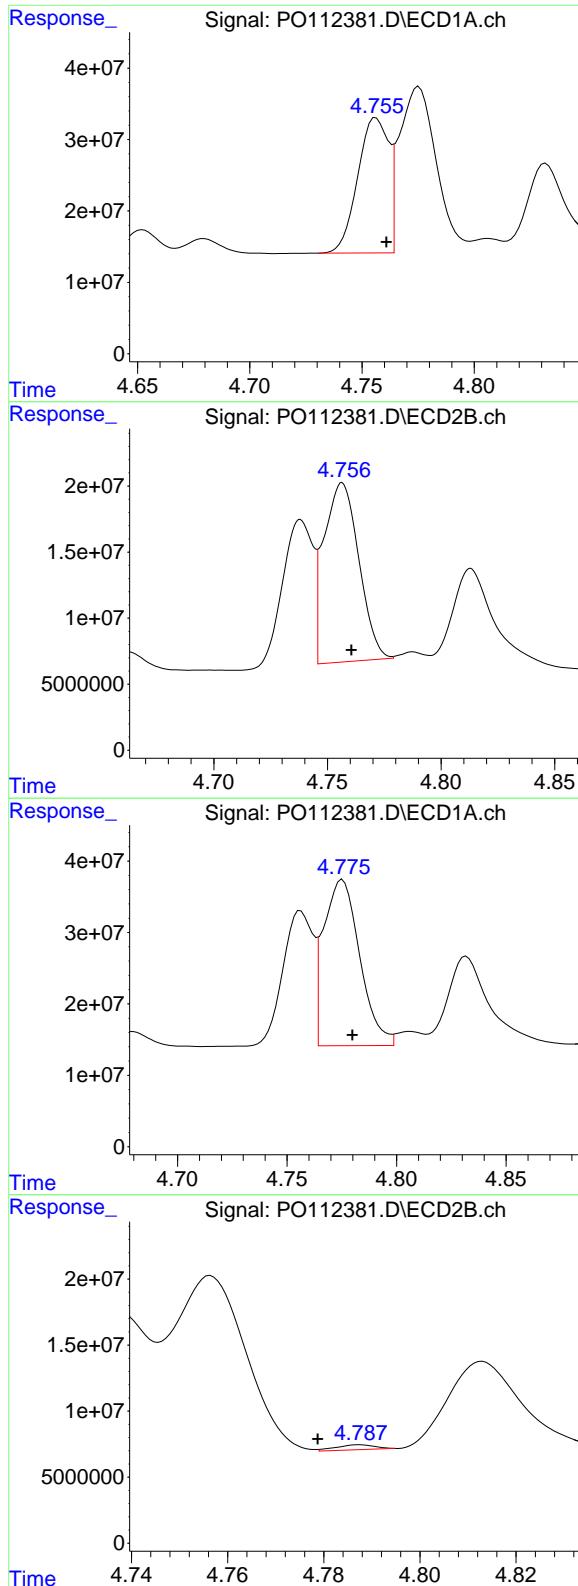

#3 AR-1016-1

R.T.: 4.756 min
 Delta R.T.: -0.005 min
 Response: 180862710
 Conc: 531.76 ng/ml

Instrument: ECD_O
 ClientSampleId: AR1660CCC500

#3 AR-1016-1


R.T.: 4.756 min
 Delta R.T.: -0.004 min
 Response: 145164528
 Conc: 651.45 ng/ml

#4 AR-1016-2

R.T.: 4.775 min
 Delta R.T.: -0.005 min
 Response: 267507791
 Conc: 537.93 ng/ml

#4 AR-1016-2

R.T.: 4.788 min
 Delta R.T.: 0.009 min
 Response: 2118165
 Conc: 6.44 ng/ml

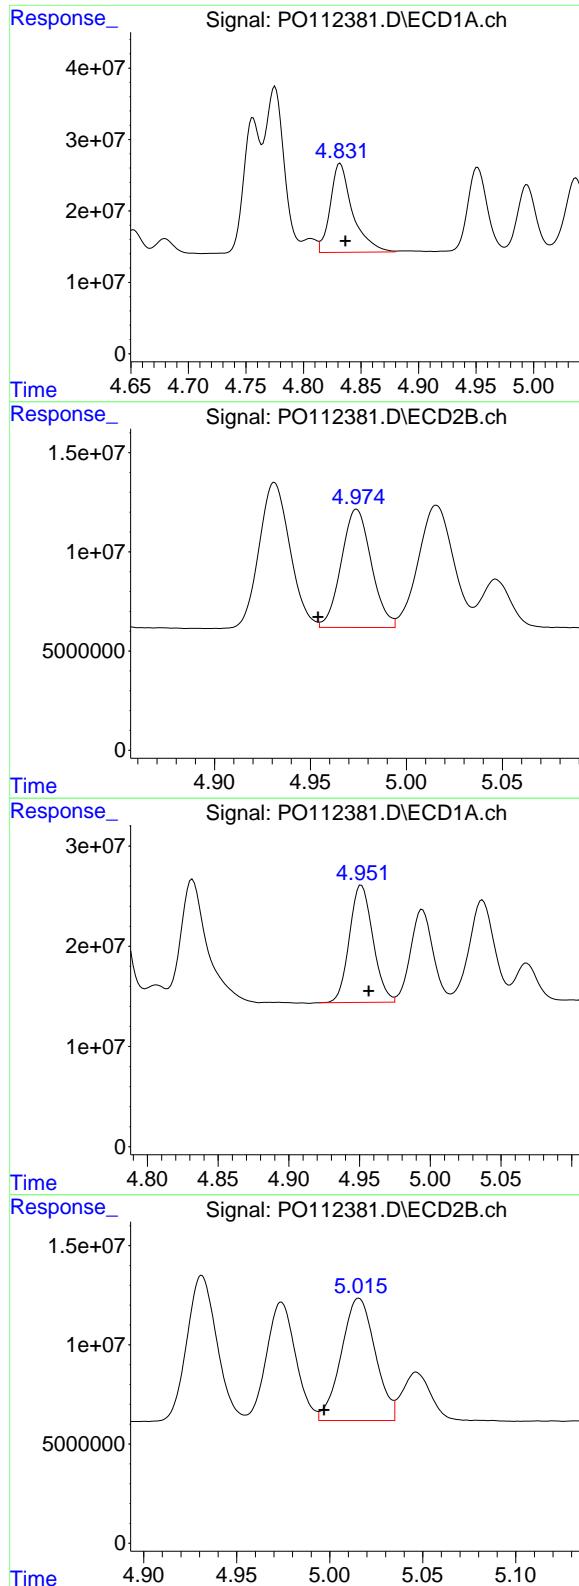

#5 AR-1016-3

R.T.: 4.832 min
 Delta R.T.: -0.004 min
 Response: 167757685
 Conc: 518.23 ng/ml

Instrument: ECD_O
 ClientSampleId: AR1660CCC500

#5 AR-1016-3


R.T.: 4.974 min
 Delta R.T.: 0.020 min
 Response: 65031858
 Conc: 382.84 ng/ml

#6 AR-1016-4

R.T.: 4.951 min
 Delta R.T.: -0.005 min
 Response: 135250965
 Conc: 526.68 ng/ml

#6 AR-1016-4

R.T.: 5.016 min
 Delta R.T.: 0.019 min
 Response: 78356304
 Conc: 571.00 ng/ml

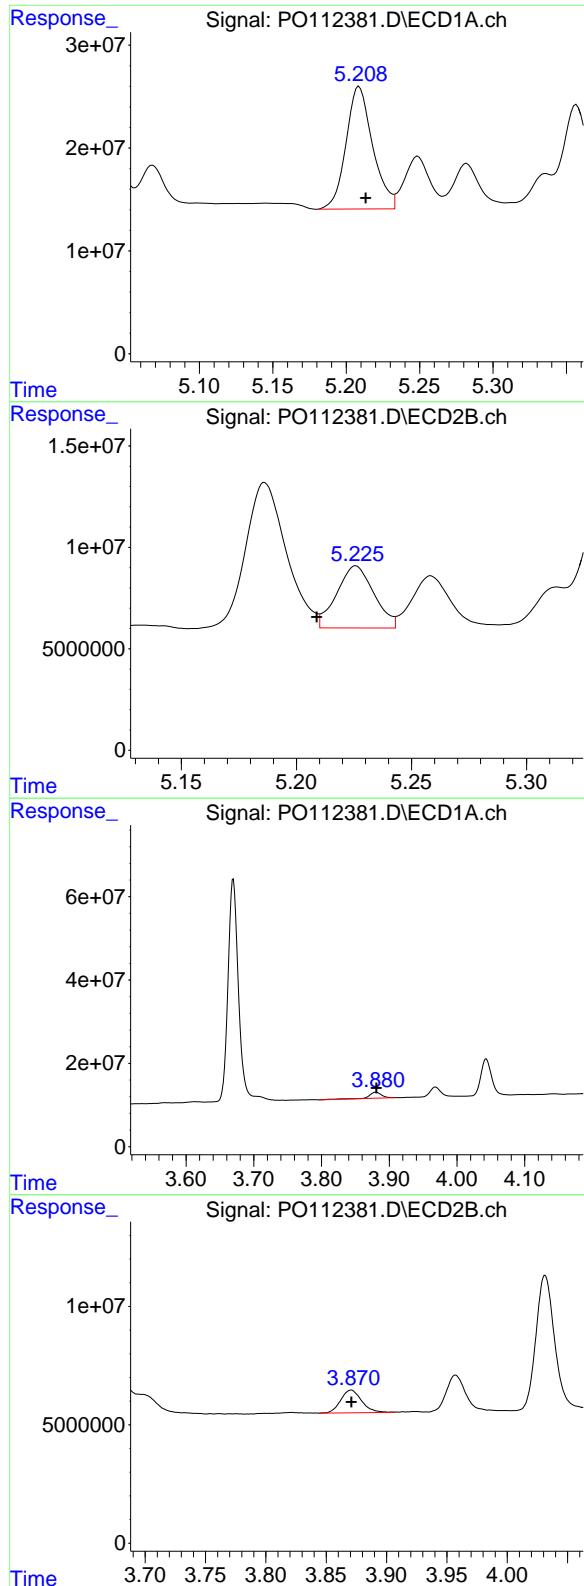

#7 AR-1016-5

R.T.: 5.209 min
 Delta R.T.: -0.004 min
 Response: 150287384
 Conc: 549.17 ng/ml

Instrument: ECD_O
 ClientSampleId: AR1660CCC500

#7 AR-1016-5


R.T.: 5.226 min
 Delta R.T.: 0.017 min
 Response: 34466083
 Conc: 199.86 ng/ml

#8 AR-1221-1

R.T.: 3.880 min
 Delta R.T.: 0.000 min
 Response: 18239399
 Conc: 156.41 ng/ml

#8 AR-1221-1

R.T.: 3.871 min
 Delta R.T.: 0.000 min
 Response: 11668776
 Conc: 141.79 ng/ml

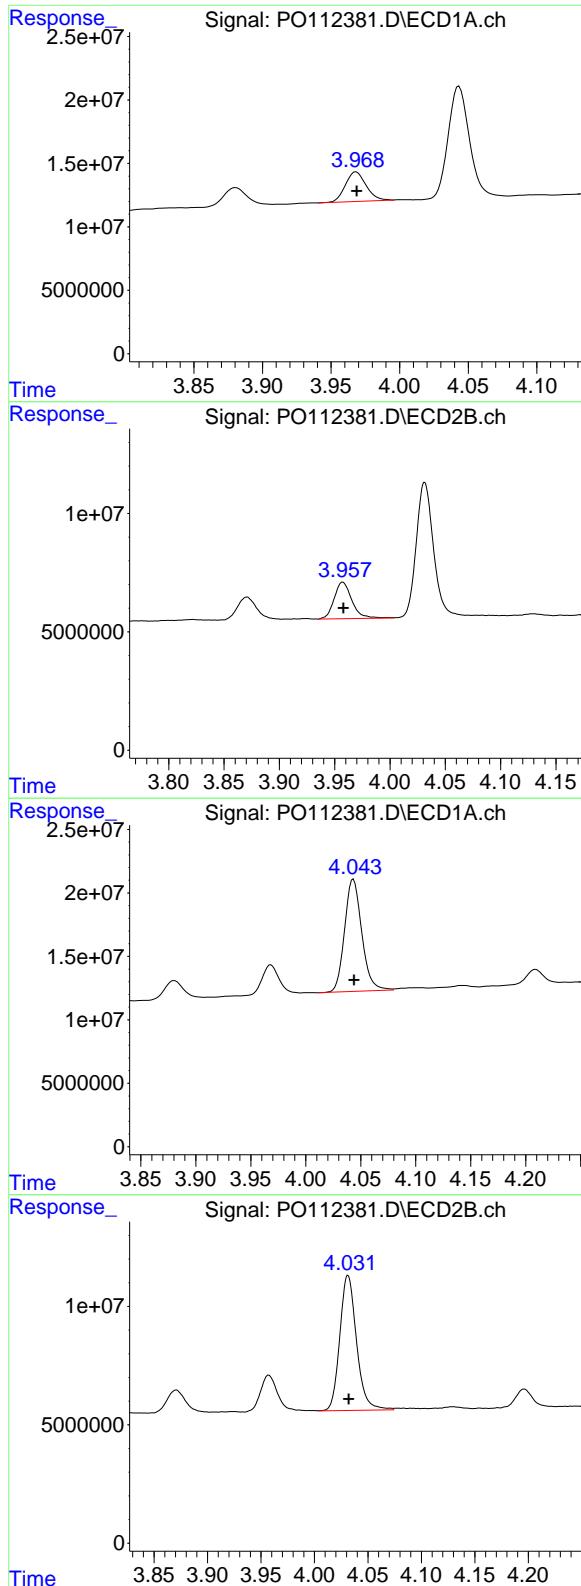

#9 AR-1221-2

R.T.: 3.968 min
 Delta R.T.: 0.000 min
 Response: 24438120
 Conc: 309.97 ng/ml

Instrument: ECD_O
ClientSampleId: AR1660CCC500

#9 AR-1221-2


R.T.: 3.957 min
 Delta R.T.: 0.000 min
 Response: 17263867
 Conc: 290.86 ng/ml

#10 AR-1221-3

R.T.: 4.043 min
 Delta R.T.: 0.000 min
 Response: 96368419
 Conc: 357.47 ng/ml

#10 AR-1221-3

R.T.: 4.031 min
 Delta R.T.: 0.000 min
 Response: 62424512
 Conc: 330.68 ng/ml

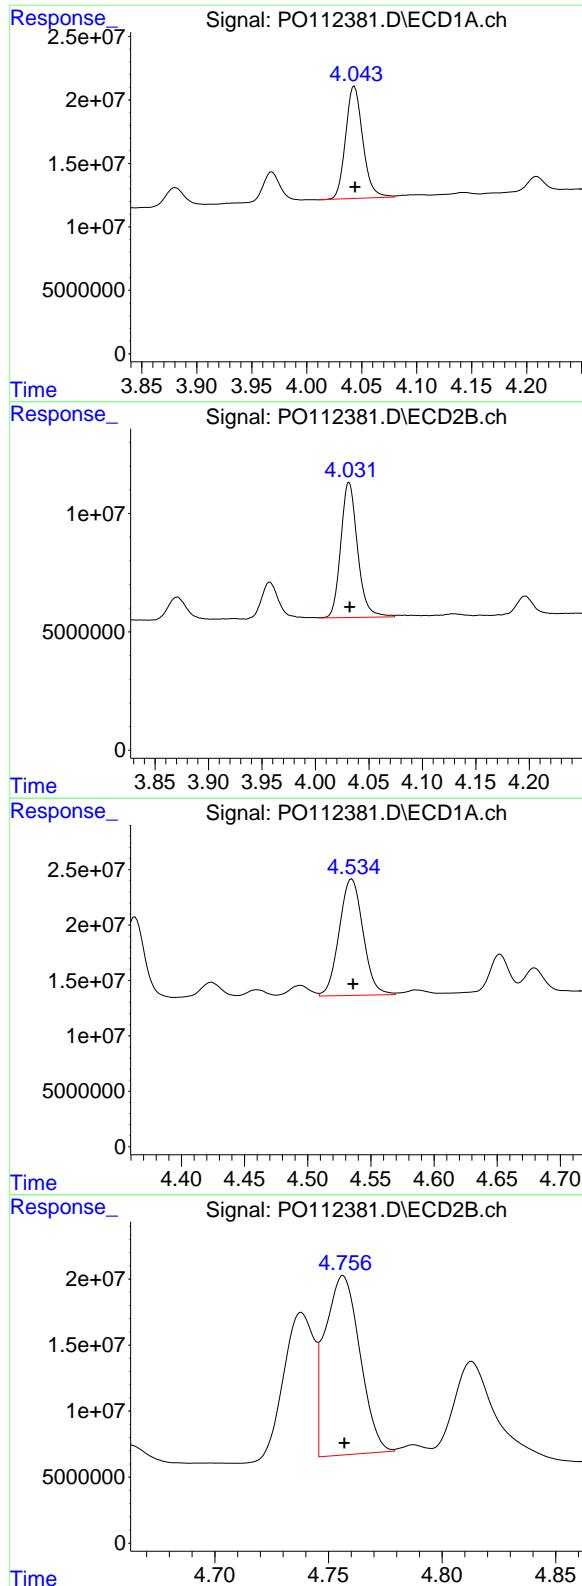

#11 AR-1232-1

R.T.: 4.043 min
 Delta R.T.: 0.000 min
 Response: 96368419
 Conc: 448.92 ng/ml

Instrument: ECD_O
ClientSampleId: AR1660CCC500

#11 AR-1232-1


R.T.: 4.031 min
 Delta R.T.: 0.000 min
 Response: 62424512
 Conc: 415.89 ng/ml

#12 AR-1232-2

R.T.: 4.535 min
 Delta R.T.: 0.000 min
 Response: 138160661
 Conc: 1215.81 ng/ml

#12 AR-1232-2

R.T.: 4.756 min
 Delta R.T.: 0.000 min
 Response: 145164528
 Conc: 948.26 ng/ml

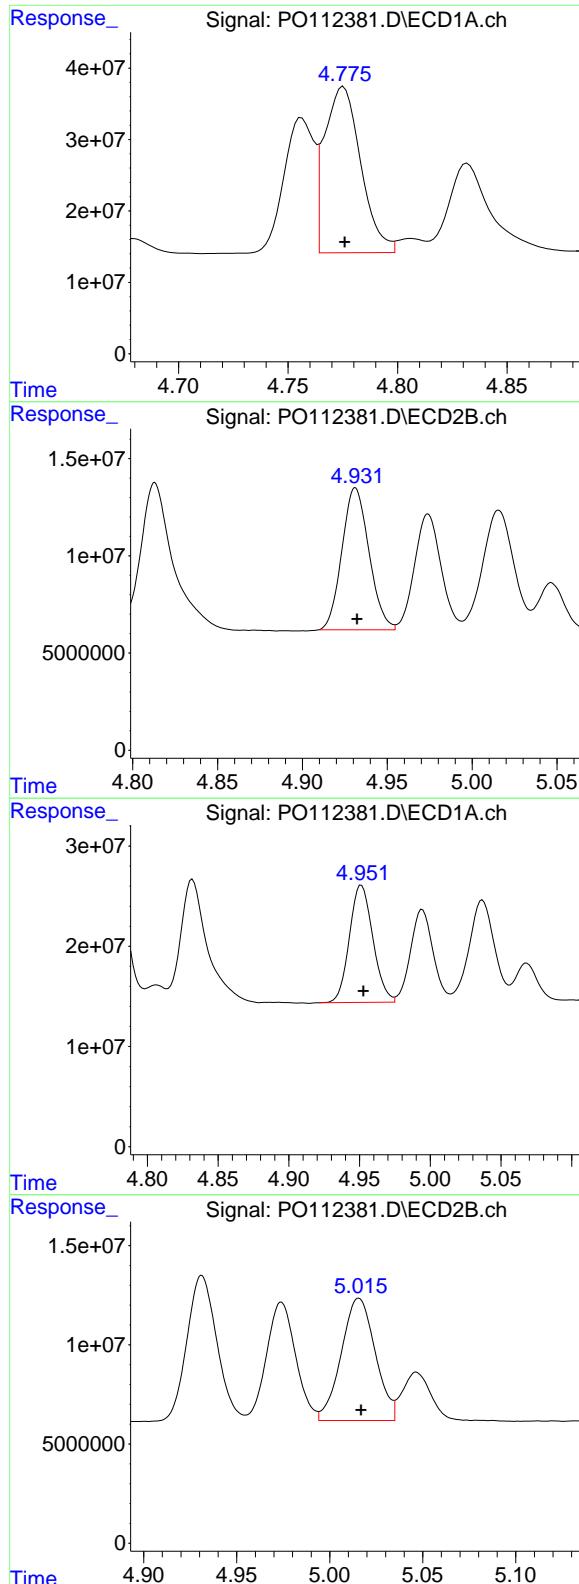

#13 AR-1232-3

R.T.: 4.775 min
 Delta R.T.: 0.000 min
 Response: 267507791
 Conc: 1168.11 ng/ml

Instrument: ECD_O
 ClientSampleId: AR1660CCC500

#13 AR-1232-3


R.T.: 4.931 min
 Delta R.T.: 0.000 min
 Response: 81132873
 Conc: 1074.52 ng/ml

#14 AR-1232-4

R.T.: 4.951 min
 Delta R.T.: -0.001 min
 Response: 135250965
 Conc: 1183.33 ng/ml

#14 AR-1232-4

R.T.: 5.016 min
 Delta R.T.: -0.001 min
 Response: 78356304
 Conc: 1187.43 ng/ml

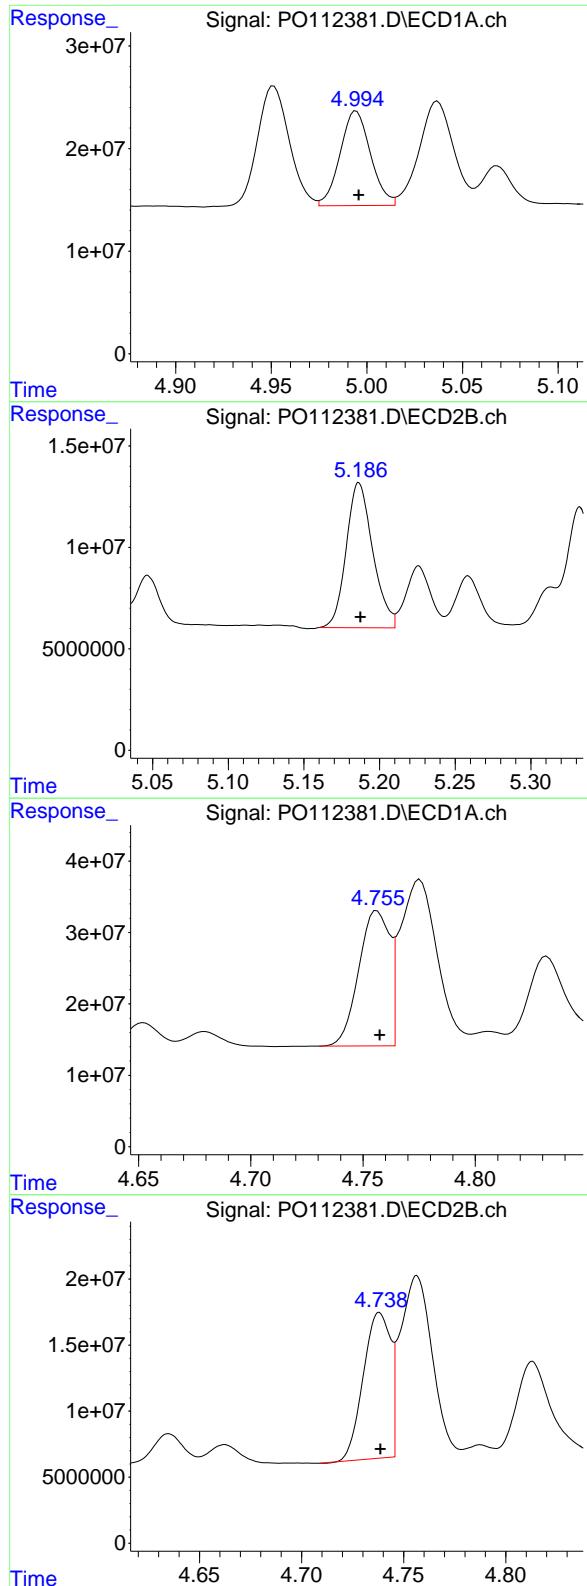

#15 AR-1232-5

R.T.: 4.994 min
 Delta R.T.: -0.001 min
 Response: 102360025
 Conc: 1394.55 ng/ml

Instrument: ECD_O
 ClientSampleId: AR1660CCC500

#15 AR-1232-5


R.T.: 5.186 min
 Delta R.T.: -0.001 min
 Response: 87512117
 Conc: 1178.46 ng/ml

#16 AR-1242-1

R.T.: 4.756 min
 Delta R.T.: -0.001 min
 Response: 180862710
 Conc: 624.45 ng/ml

#16 AR-1242-1

R.T.: 4.738 min
 Delta R.T.: 0.000 min
 Response: 102328989
 Conc: 527.85 ng/ml

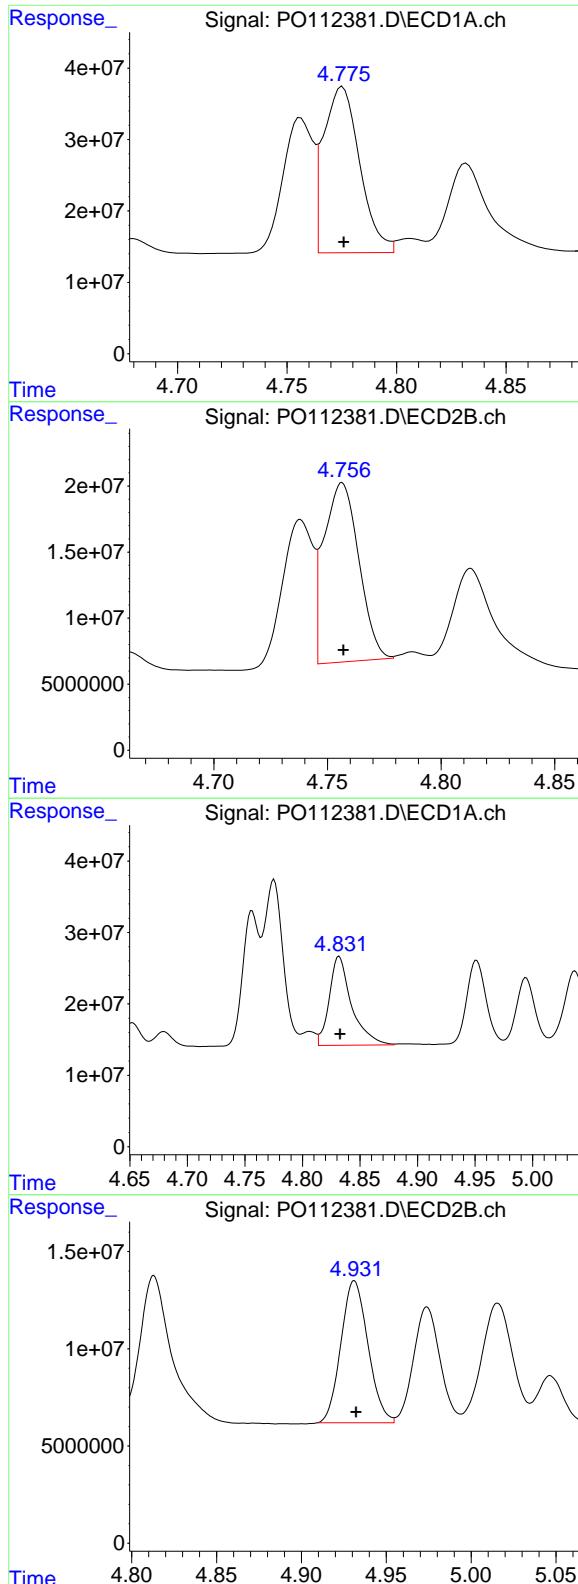

#17 AR-1242-2

R.T.: 4.775 min
 Delta R.T.: 0.000 min
Instrument:
 Response: 267507791 ECD_O
 Conc: 628.07 ng/ml
ClientSampleId :
 AR1660CCC500

#17 AR-1242-2


R.T.: 4.756 min
 Delta R.T.: 0.000 min
 Response: 145164528
 Conc: 512.31 ng/ml

#18 AR-1242-3

R.T.: 4.832 min
 Delta R.T.: 0.000 min
 Response: 167757685
 Conc: 612.96 ng/ml

#18 AR-1242-3


R.T.: 4.931 min
 Delta R.T.: 0.000 min
 Response: 81132873
 Conc: 556.94 ng/ml

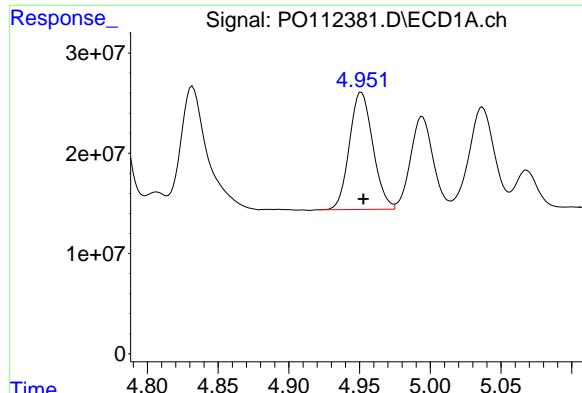

#19 AR-1242-4


R.T.: 4.951 min
 Delta R.T.: -0.001 min
 Response: 135250965
 Conc: 600.27 ng/ml

Instrument: ECD_O
 ClientSampleId: AR1660CCC500

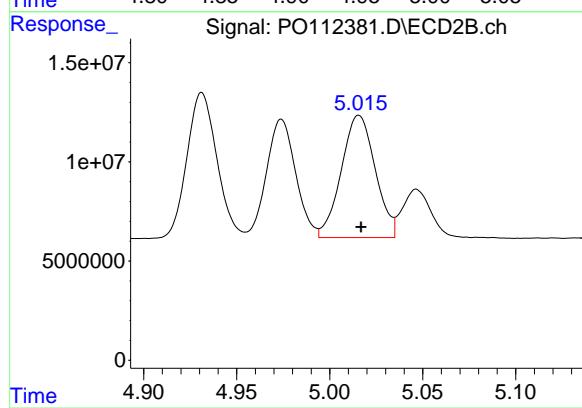


#19 AR-1242-4

R.T.: 5.016 min
 Delta R.T.: -0.001 min
 Response: 78356304
 Conc: 552.42 ng/ml

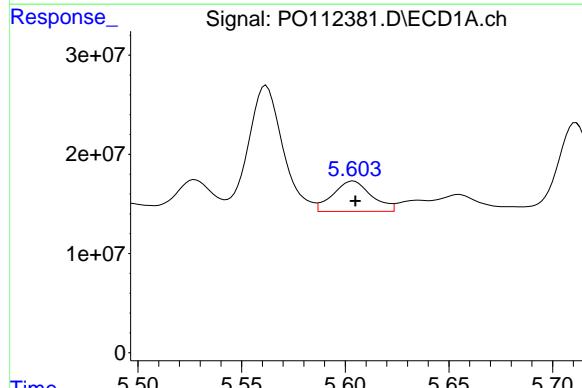


#20 AR-1242-5

R.T.: 5.604 min
 Delta R.T.: 0.000 min
 Response: 39800546
 Conc: 188.03 ng/ml

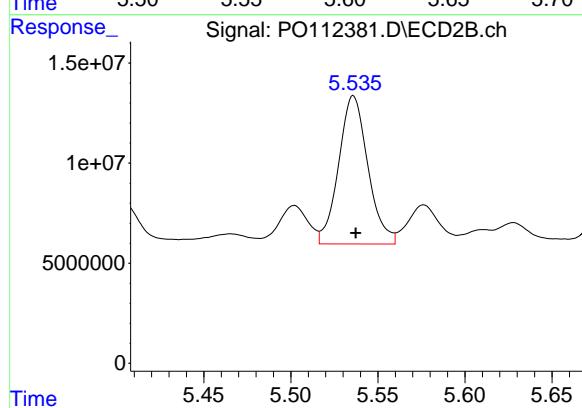

#20 AR-1242-5


R.T.: 5.536 min
 Delta R.T.: -0.001 min
 Response: 86773714
 Conc: 477.48 ng/ml

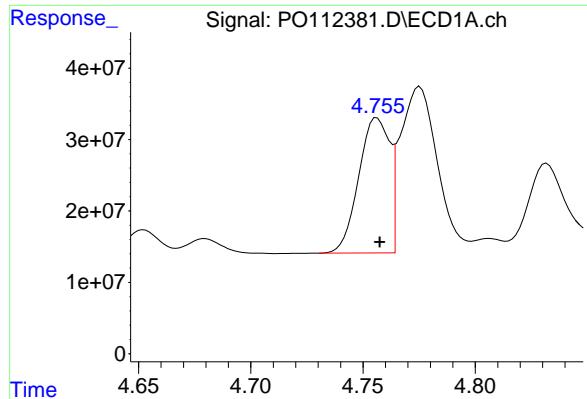

#21 AR-1248-1


R.T.: 4.756 min
 Delta R.T.: -0.001 min
 Response: 180862710
 Conc: 797.10 ng/ml

Instrument: ECD_O
 ClientSampleId: AR1660CCC500

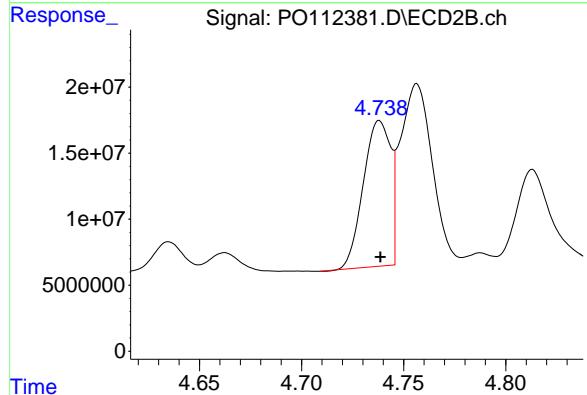


#21 AR-1248-1

R.T.: 4.738 min
 Delta R.T.: 0.000 min
 Response: 102328989
 Conc: 662.89 ng/ml

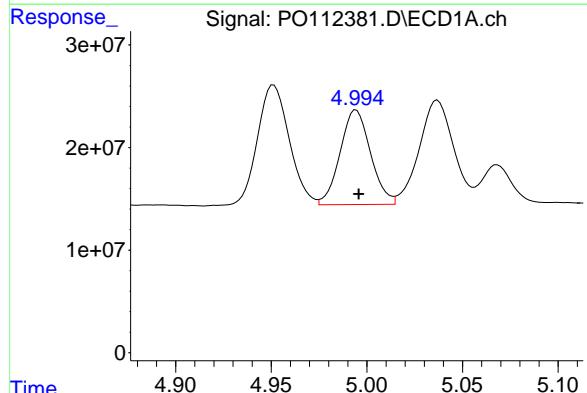


#22 AR-1248-2

R.T.: 4.994 min
 Delta R.T.: -0.001 min
 Response: 102360025
 Conc: 331.99 ng/ml

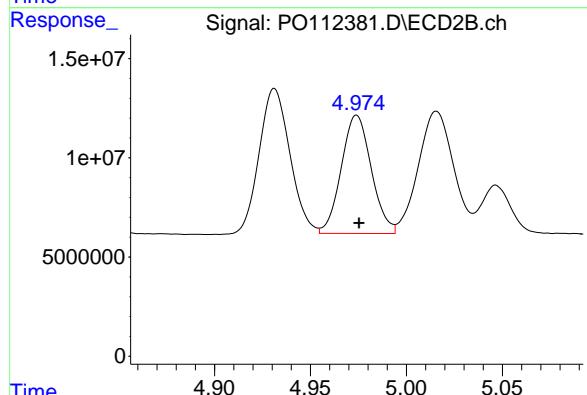

#22 AR-1248-2

R.T.: 4.974 min
 Delta R.T.: -0.001 min
 Response: 65031858
 Conc: 316.05 ng/ml

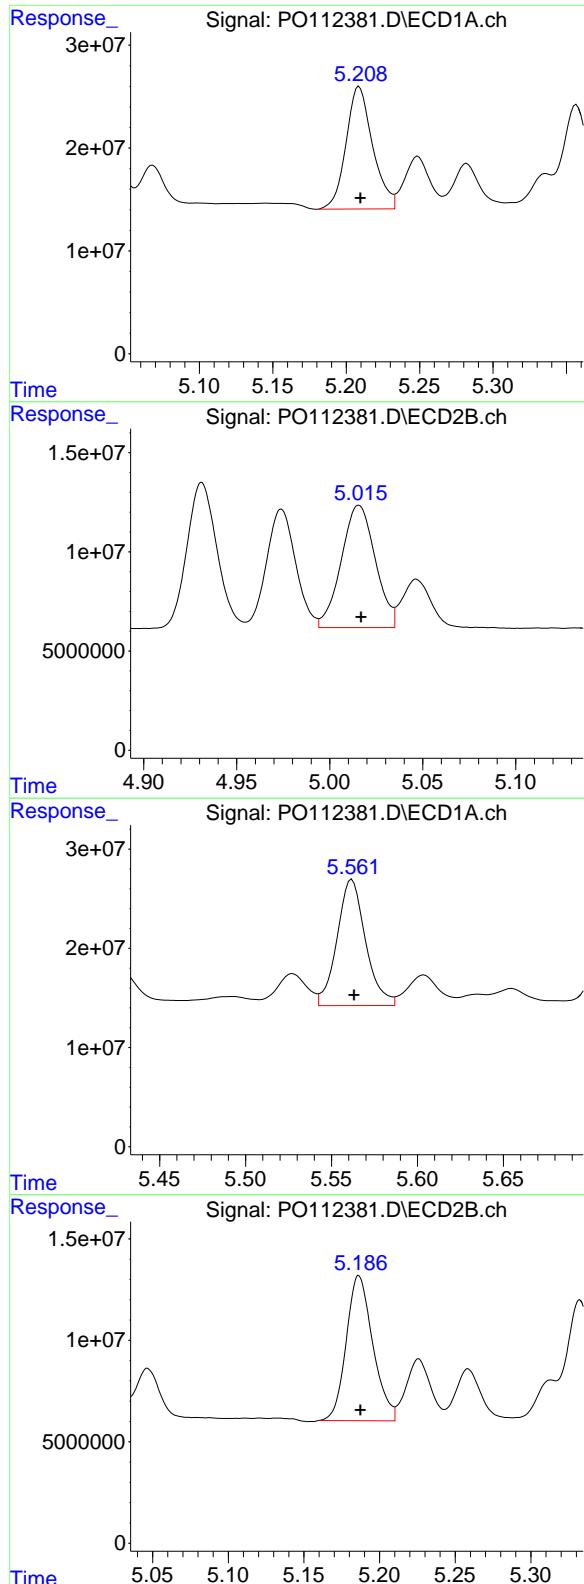

#23 AR-1248-3

R.T.: 5.209 min
 Delta R.T.: 0.000 min
 Response: 150287384
 Conc: 368.97 ng/ml

Instrument: ECD_O
 ClientSampleId: AR1660CCC500

#23 AR-1248-3


R.T.: 5.016 min
 Delta R.T.: -0.001 min
 Response: 78356304
 Conc: 364.79 ng/ml

#24 AR-1248-4

R.T.: 5.562 min
 Delta R.T.: -0.001 min
 Response: 146966864
 Conc: 254.64 ng/ml

#24 AR-1248-4

R.T.: 5.186 min
 Delta R.T.: -0.001 min
 Response: 87512117
 Conc: 338.24 ng/ml

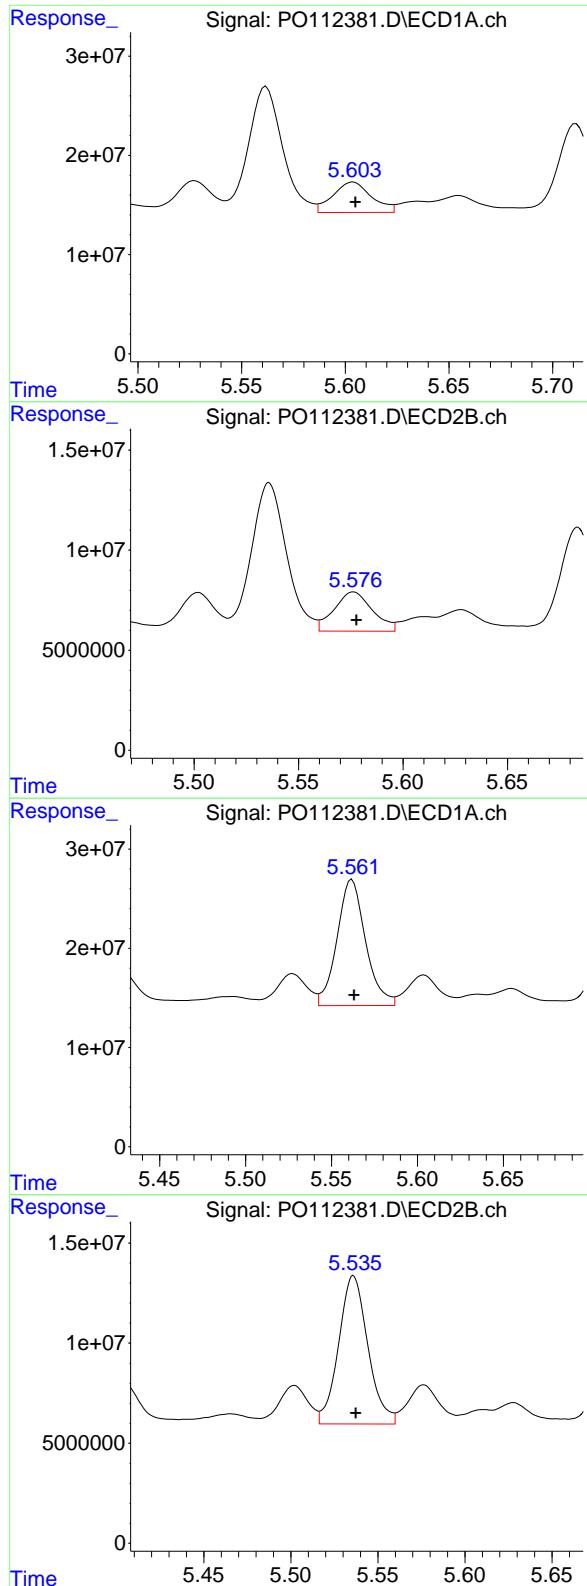

#25 AR-1248-5

R.T.: 5.604 min
 Delta R.T.: 0.000 min
 Response: 39800546
 Conc: 101.97 ng/ml

Instrument: ECD_O
 ClientSampleId: AR1660CCC500

#25 AR-1248-5


R.T.: 5.576 min
 Delta R.T.: -0.001 min
 Response: 25069754
 Conc: 100.06 ng/ml

#26 AR-1254-1

R.T.: 5.562 min
 Delta R.T.: -0.001 min
 Response: 146966864
 Conc: 238.93 ng/ml

#26 AR-1254-1

R.T.: 5.536 min
 Delta R.T.: -0.001 min
 Response: 86773714
 Conc: 227.65 ng/ml

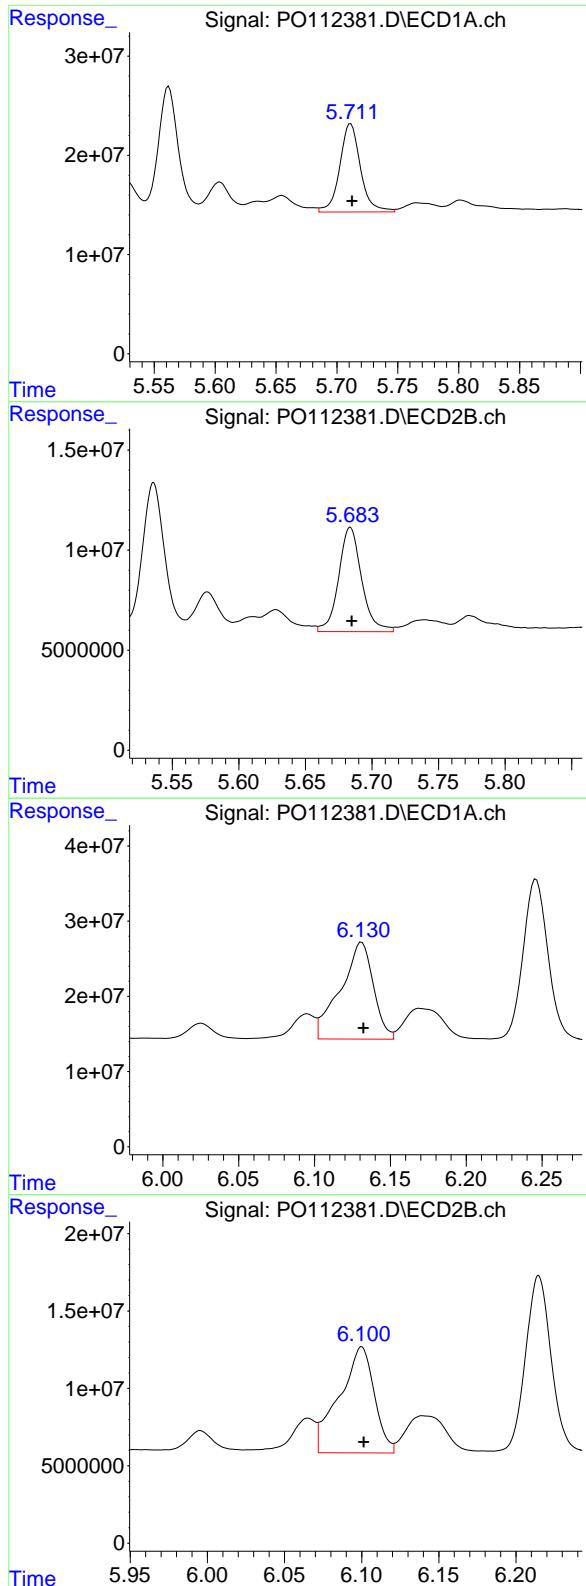

#27 AR-1254-2

R.T.: 5.711 min
 Delta R.T.: -0.001 min
 Response: 105695298
 Conc: 197.31 ng/ml

Instrument: ECD_O
 ClientSampleId: AR1660CCC500

#27 AR-1254-2


R.T.: 5.684 min
 Delta R.T.: -0.001 min
 Response: 62838205
 Conc: 189.38 ng/ml

#28 AR-1254-3

R.T.: 6.131 min
 Delta R.T.: -0.001 min
 Response: 194870048
 Conc: 232.10 ng/ml

#28 AR-1254-3

R.T.: 6.100 min
 Delta R.T.: -0.002 min
 Response: 108017982
 Conc: 224.08 ng/ml

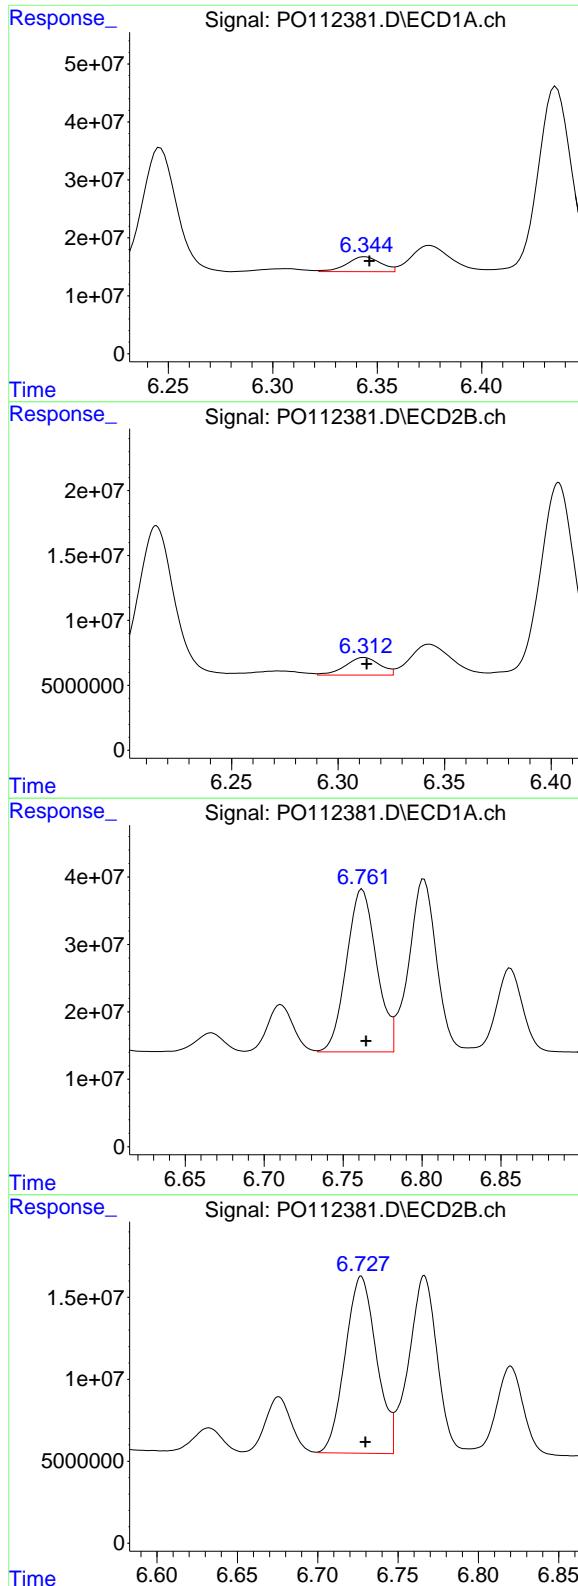

#29 AR-1254-4

R.T.: 6.344 min
 Delta R.T.: -0.002 min
 Response: 28936254
 Conc: 60.16 ng/ml

Instrument: ECD_O
 ClientSampleId: AR1660CCC500

#29 AR-1254-4


R.T.: 6.312 min
 Delta R.T.: -0.001 min
 Response: 15324206
 Conc: 58.78 ng/ml

#30 AR-1254-5

R.T.: 6.762 min
 Delta R.T.: -0.002 min
 Response: 319678834
 Conc: 413.05 ng/ml

#30 AR-1254-5

R.T.: 6.727 min
 Delta R.T.: -0.003 min
 Response: 146236236
 Conc: 410.37 ng/ml

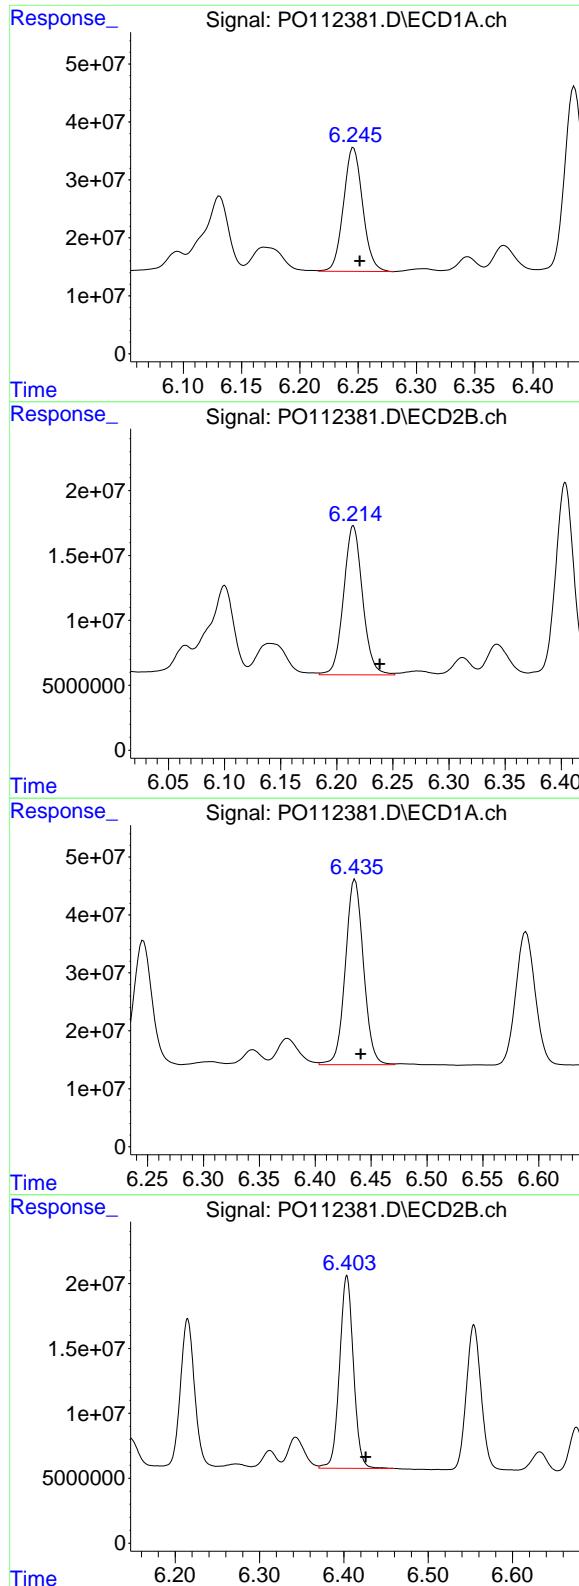

#31 AR-1260-1

R.T.: 6.246 min
 Delta R.T.: -0.005 min
 Response: 244719104
 Conc: 488.23 ng/ml

Instrument: ECD_O
ClientSampleId: AR1660CCC500

#31 AR-1260-1


R.T.: 6.215 min
 Delta R.T.: -0.023 min
 Response: 135145555
 Conc: 481.70 ng/ml

#32 AR-1260-2

R.T.: 6.436 min
 Delta R.T.: -0.005 min
 Response: 360404699
 Conc: 488.26 ng/ml

#32 AR-1260-2

R.T.: 6.404 min
 Delta R.T.: -0.022 min
 Response: 169754475
 Conc: 499.28 ng/ml

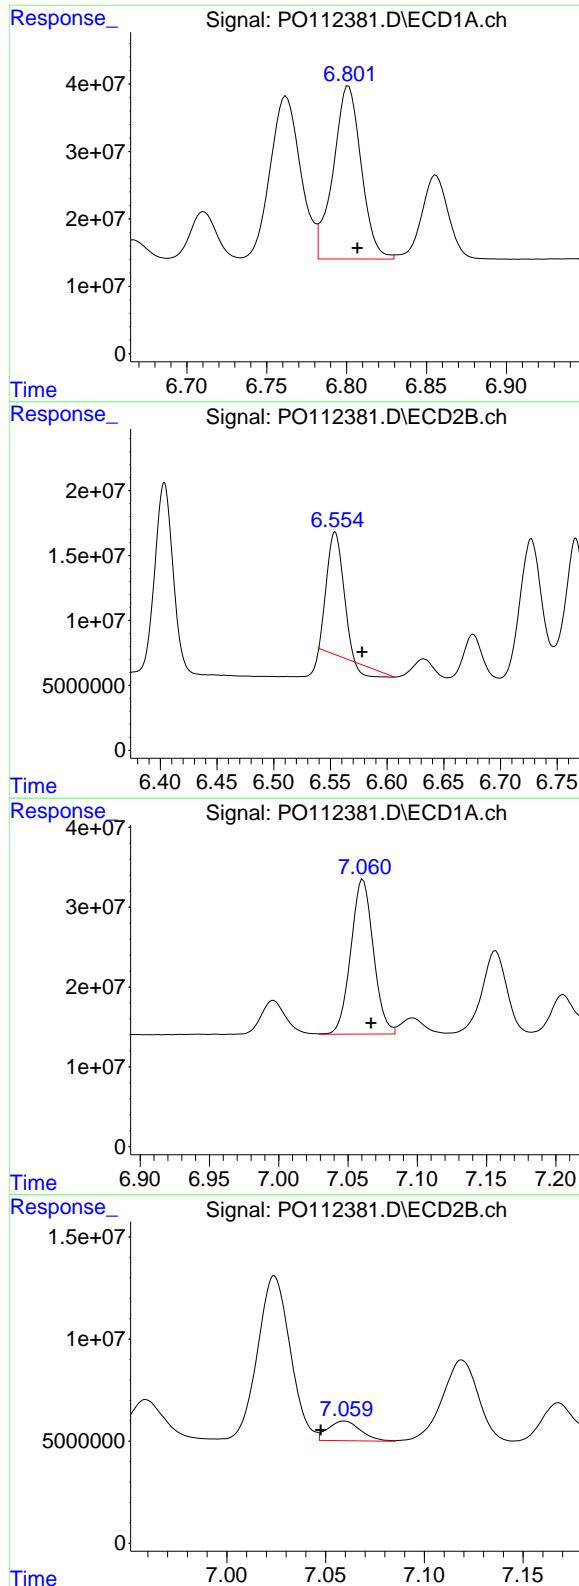

#33 AR-1260-3

R.T.: 6.801 min
 Delta R.T.: -0.005 min
 Response: 313295711
 Conc: 477.96 ng/ml

Instrument: ECD_O
 ClientSampleId: AR1660CCC500

#33 AR-1260-3


R.T.: 6.554 min
 Delta R.T.: -0.024 min
 Response: 87394780
 Conc: 317.12 ng/ml

#34 AR-1260-4

R.T.: 7.061 min
 Delta R.T.: -0.006 min
 Response: 219427950
 Conc: 504.14 ng/ml

#34 AR-1260-4


R.T.: 7.059 min
 Delta R.T.: 0.012 min
 Response: 11069571
 Conc: 55.17 ng/ml



#35 AR-1260-5


R.T.: 7.304 min
 Delta R.T.: -0.005 min
 Response: 633483438
 Conc: 501.75 ng/ml

Instrument: ECD_O
 ClientSampleId: AR1660CCC500

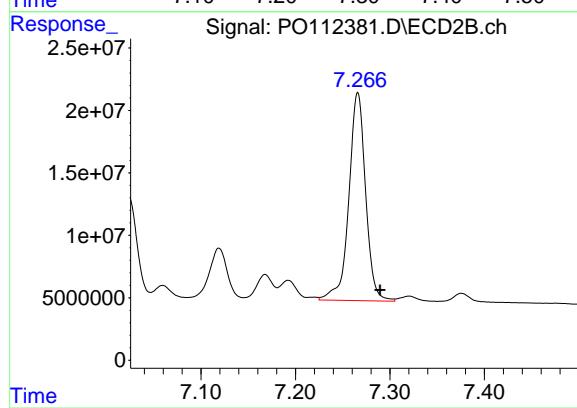


#35 AR-1260-5

R.T.: 7.266 min
 Delta R.T.: -0.024 min
 Response: 205628634
 Conc: 459.27 ng/ml

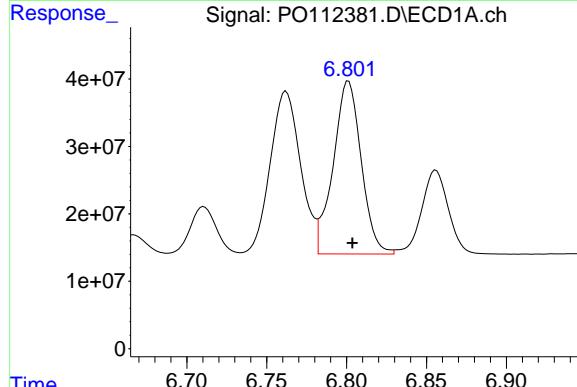


#36 AR-1262-1

R.T.: 6.801 min
 Delta R.T.: -0.002 min
 Response: 313295711
 Conc: 306.65 ng/ml

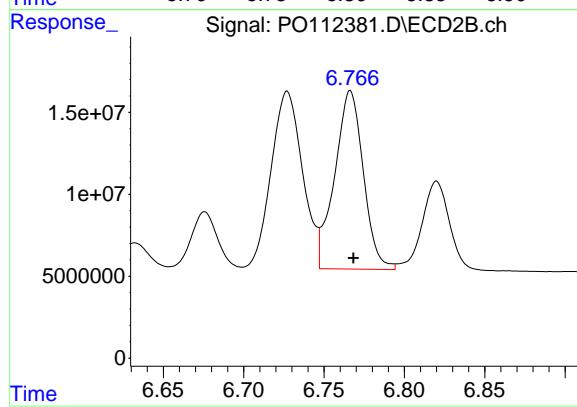

#36 AR-1262-1

R.T.: 6.766 min
 Delta R.T.: -0.002 min
 Response: 135282397
 Conc: 332.13 ng/ml

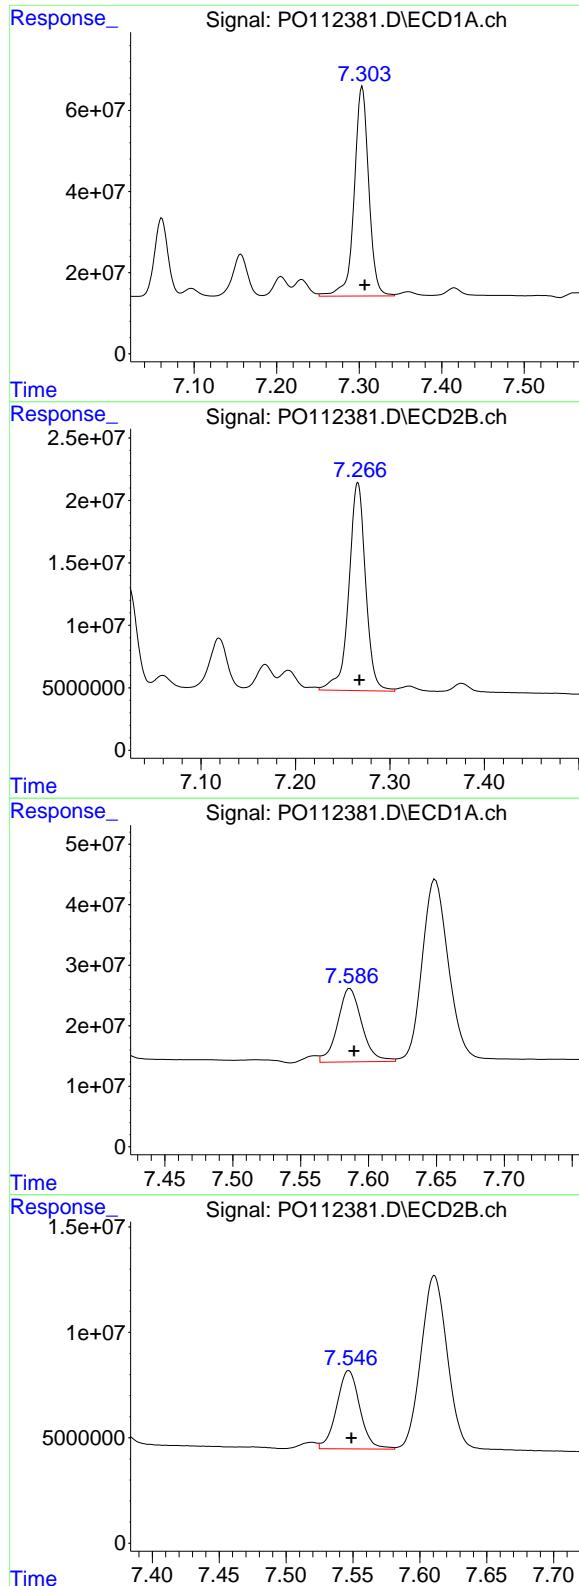

#37 AR-1262-2

R.T.: 7.304 min
 Delta R.T.: -0.003 min
 Response: 633483438
 Conc: 386.42 ng/ml

Instrument: ECD_O
 ClientSampleId: AR1660CCC500

#37 AR-1262-2


R.T.: 7.266 min
 Delta R.T.: -0.002 min
 Response: 205628634
 Conc: 401.19 ng/ml

#38 AR-1262-3

R.T.: 7.586 min
 Delta R.T.: -0.003 min
 Response: 150801416
 Conc: 234.90 ng/ml

#38 AR-1262-3

R.T.: 7.547 min
 Delta R.T.: -0.002 min
 Response: 44908619
 Conc: 250.15 ng/ml

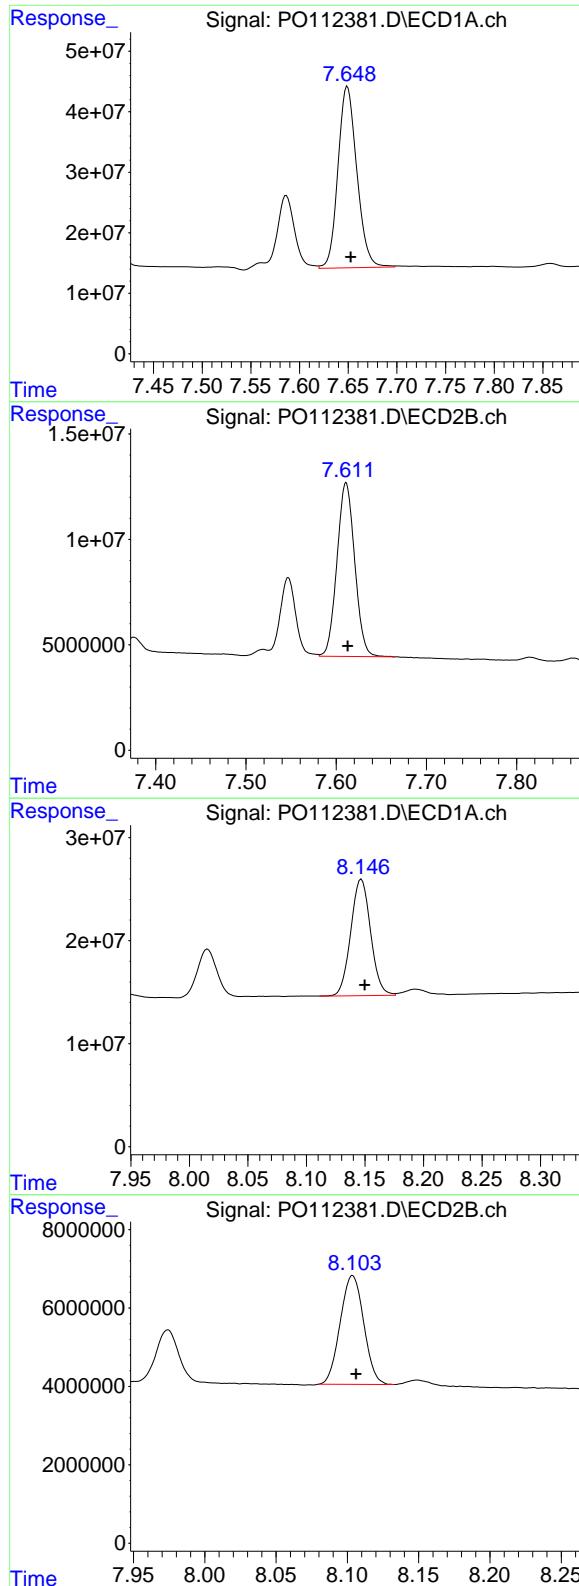

#39 AR-1262-4

R.T.: 7.649 min
 Delta R.T.: -0.003 min
 Response: 404885637
 Conc: 377.89 ng/ml

Instrument: ECD_O
ClientSampleId: AR1660CCC500

#39 AR-1262-4


R.T.: 7.611 min
 Delta R.T.: -0.002 min
 Response: 112620008
 Conc: 387.12 ng/ml

#40 AR-1262-5

R.T.: 8.147 min
 Delta R.T.: -0.003 min
 Response: 133375109
 Conc: 297.62 ng/ml

#40 AR-1262-5

R.T.: 8.104 min
 Delta R.T.: -0.002 min
 Response: 31930474
 Conc: 301.85 ng/ml

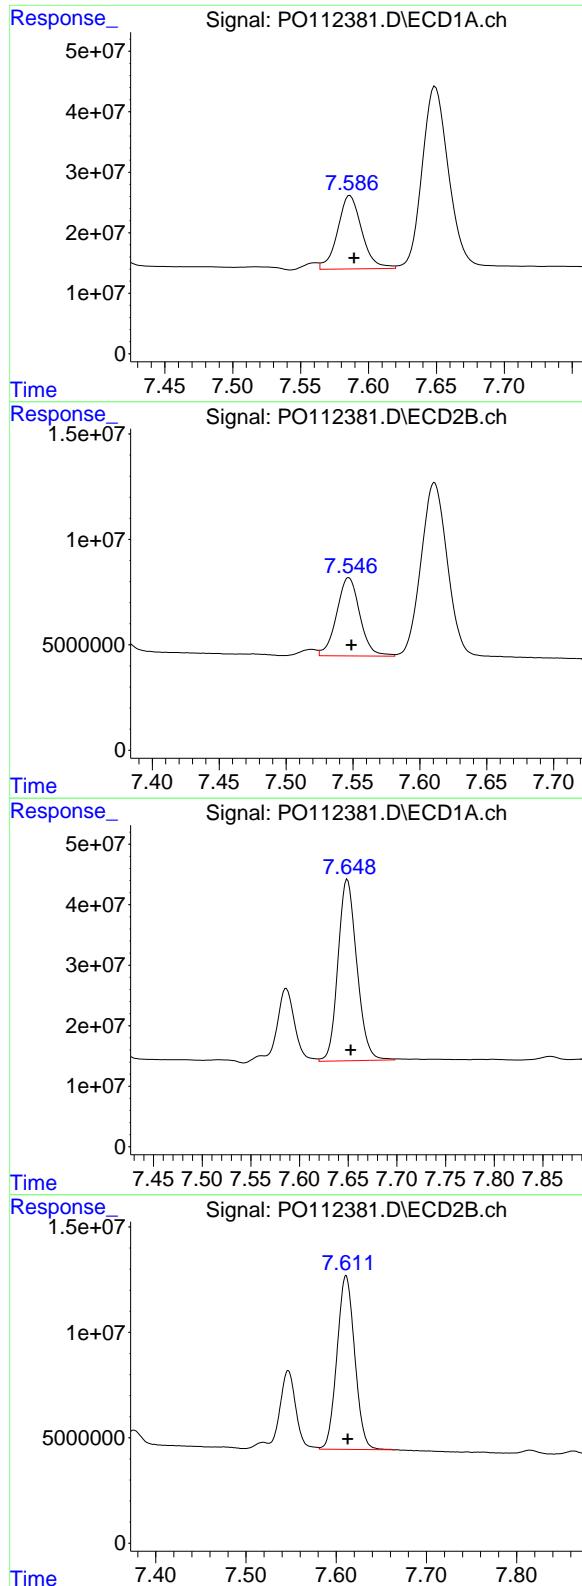

#41 AR-1268-1

R.T.: 7.586 min
 Delta R.T.: -0.003 min
 Response: 150801416
 Conc: 82.07 ng/ml

Instrument: ECD_O
ClientSampleId: AR1660CCC500

#41 AR-1268-1


R.T.: 7.547 min
 Delta R.T.: -0.002 min
 Response: 44908619
 Conc: 91.38 ng/ml

#42 AR-1268-2

R.T.: 7.649 min
 Delta R.T.: -0.003 min
 Response: 404885637
 Conc: 259.94 ng/ml

#42 AR-1268-2

R.T.: 7.611 min
 Delta R.T.: -0.002 min
 Response: 112620008
 Conc: 269.95 ng/ml

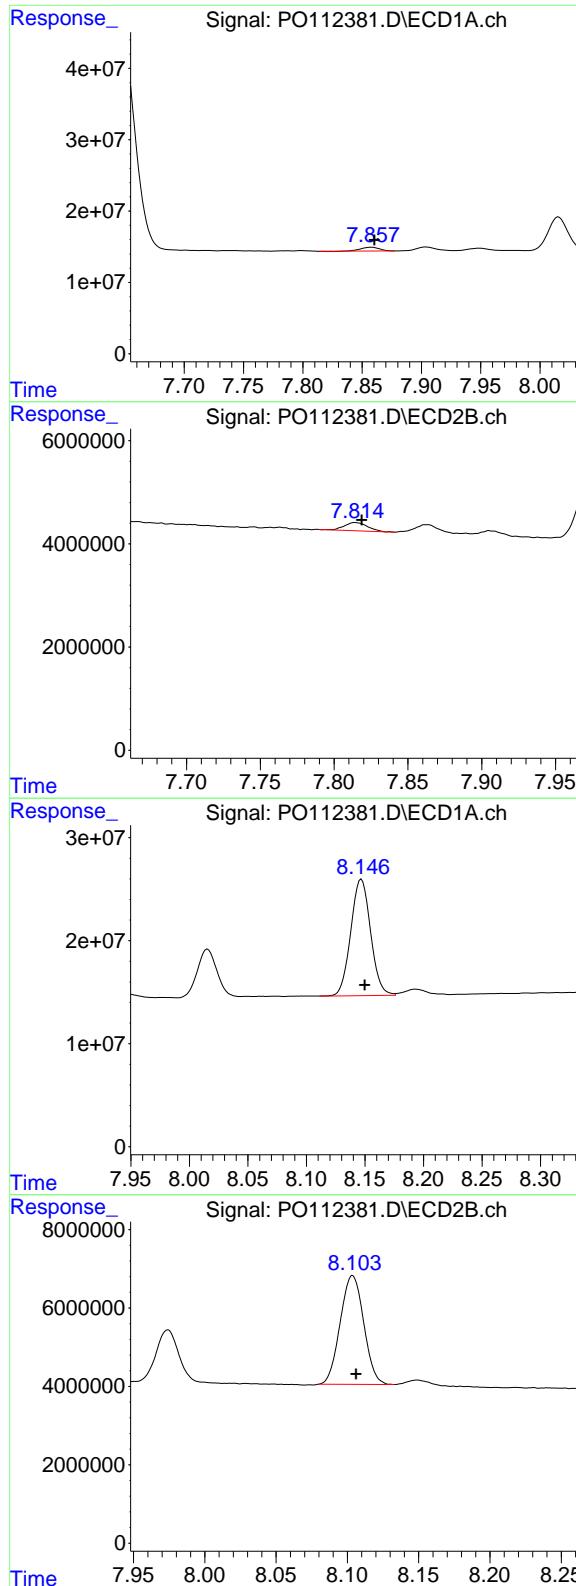

#43 AR-1268-3

R.T.: 7.858 min
 Delta R.T.: -0.003 min
 Response: 5775100
 Conc: 4.44 ng/ml

Instrument: ECD_O
 ClientSampleId: AR1660CCC500

#43 AR-1268-3


R.T.: 7.815 min
 Delta R.T.: -0.004 min
 Response: 1744375
 Conc: 5.51 ng/ml

#44 AR-1268-4

R.T.: 8.147 min
 Delta R.T.: -0.003 min
 Response: 133375109
 Conc: 277.63 ng/ml

#44 AR-1268-4


R.T.: 8.104 min
 Delta R.T.: -0.002 min
 Response: 31930474
 Conc: 286.34 ng/ml

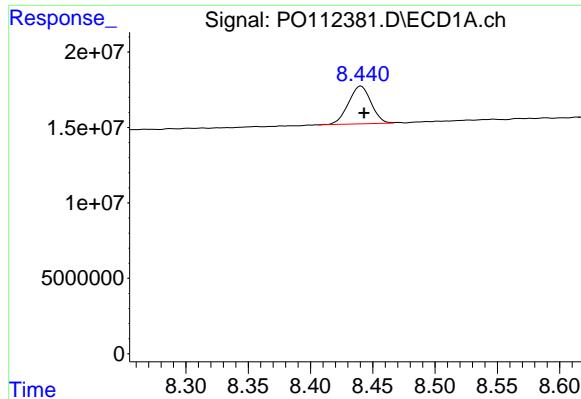

#45 AR-1268-5

R.T.: 8.441 min
Delta R.T.: -0.003 min
Response: 31825405
Conc: 9.75 ng/ml

Instrument: ECD_O
ClientSampleId: AR1660CCC500

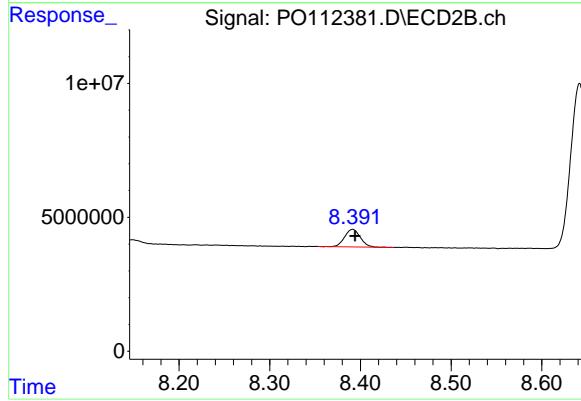

#45 AR-1268-5

R.T.: 8.391 min
Delta R.T.: -0.003 min
Response: 7796084
Conc: 10.73 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP070825\
 Data File : PP073557.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Jul 2025 21:52
 Operator : YP\AJ
 Sample : AR1660ICC250
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
AR1660ICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 08 01:40:26 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 08 01:37:59 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	4.489	3.780	36726195	48601054	25.988	25.943
2) SA Decachlor...	10.180	8.781	29096309	36663112	25.387	27.681

Target Compounds

3) L1 AR-1016-1	5.640	4.858	12627919	18293907	267.888	266.983
4) L1 AR-1016-2	5.662	4.876	19179159	27468197	266.197	267.749
5) L1 AR-1016-3	5.723	5.053	11597460	14482667	262.608	264.046
6) L1 AR-1016-4	5.821	5.095	9615182	11760046	262.767	267.901
7) L1 AR-1016-5	6.113	5.308	8568508	14818058	261.344	266.223
31) L7 AR-1260-1	7.231	6.339	15831007	26051826	265.337	261.903
32) L7 AR-1260-2	7.484	6.527	24493361	32462748	270.963	261.789
33) L7 AR-1260-3	7.843	6.679	19201014	29417085	257.072	261.967
34) L7 AR-1260-4	8.066	7.148	17258868	25990153	258.636	281.433
35) L7 AR-1260-5	8.385	7.391	40210084	64242310	259.594	276.638



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP070825\
 Data File : PP073557.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Jul 2025 21:52
 Operator : YP\AJ
 Sample : AR1660ICC250
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
AR1660ICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 08 01:40:26 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 08 01:37:59 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ m Signal #2 Info : 30M x 0.32mm x 0.25 μ m

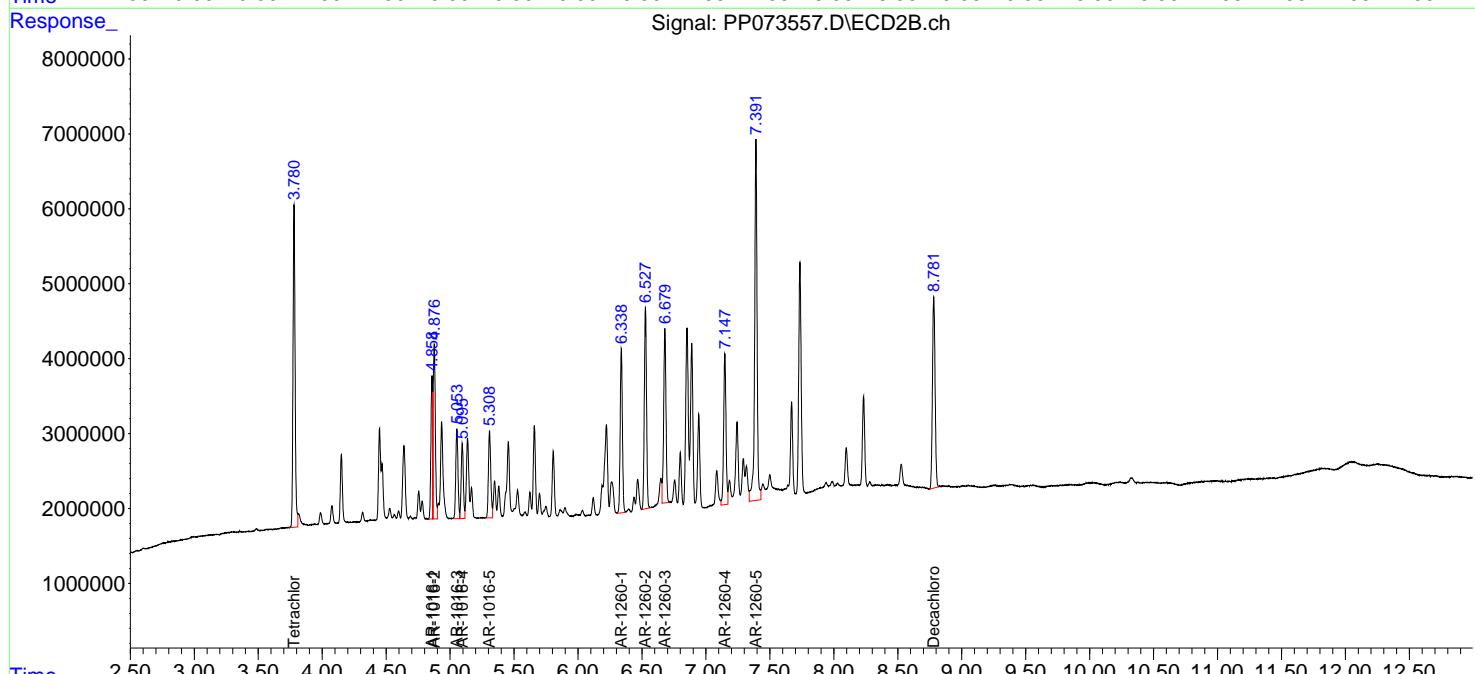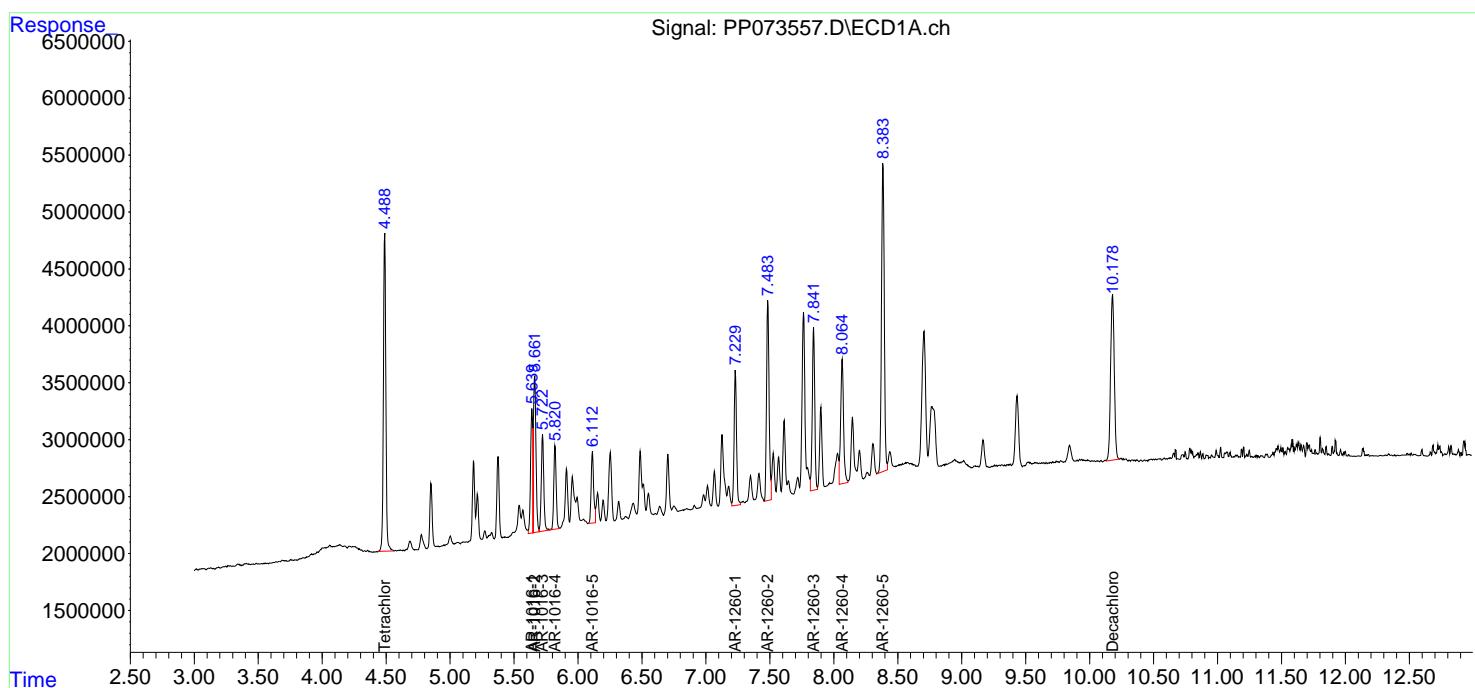

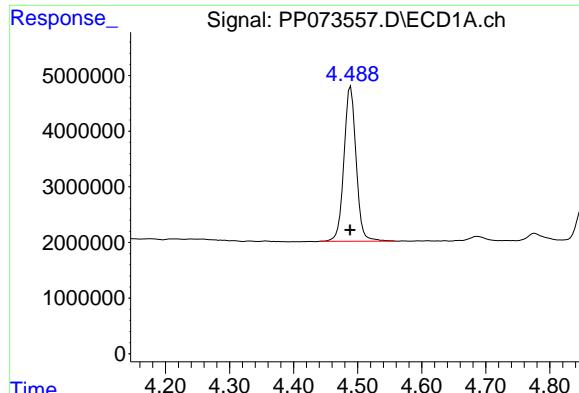


#1 Tetrachloro-m-xylene

R.T.: 4.489 min
Delta R.T.: 0.001 min
Response: 36726195
Conc: 25.99 ng/ml

Instrument:

ECD_P

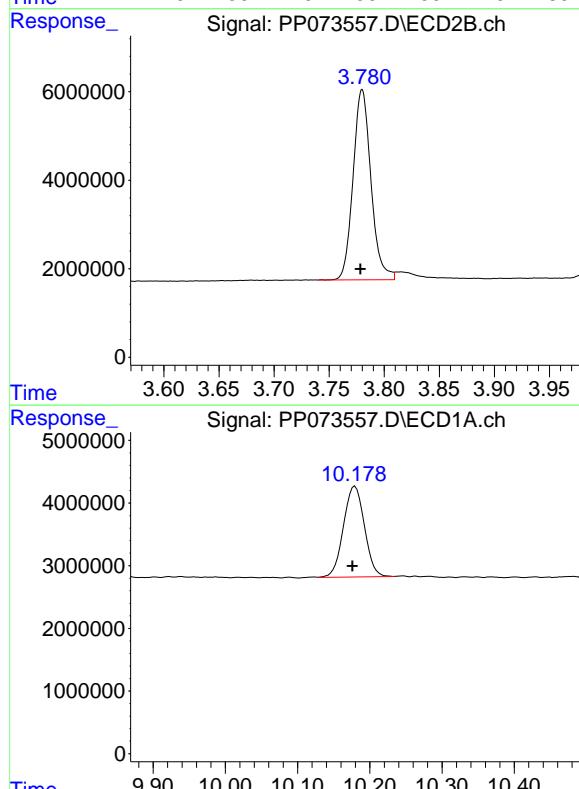ClientSampleId :
AR1660ICC250

#1 Tetrachloro-m-xylene


R.T.: 3.780 min
Delta R.T.: 0.002 min
Response: 48601054
Conc: 25.94 ng/ml

#2 Decachlorobiphenyl

R.T.: 10.180 min
Delta R.T.: 0.003 min
Response: 29096309
Conc: 25.39 ng/ml

#2 Decachlorobiphenyl


R.T.: 8.781 min
Delta R.T.: 0.001 min
Response: 36663112
Conc: 27.68 ng/ml

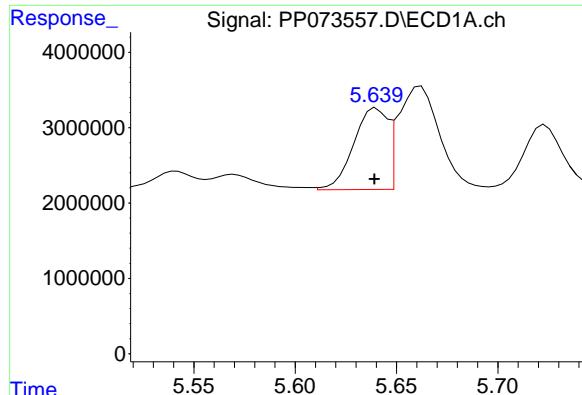

#3 AR-1016-1

R.T.: 5.640 min
 Delta R.T.: 0.001 min
 Response: 12627919
 Conc: 267.89 ng/ml

Instrument: ECD_P
 ClientSampleId: AR1660ICC250

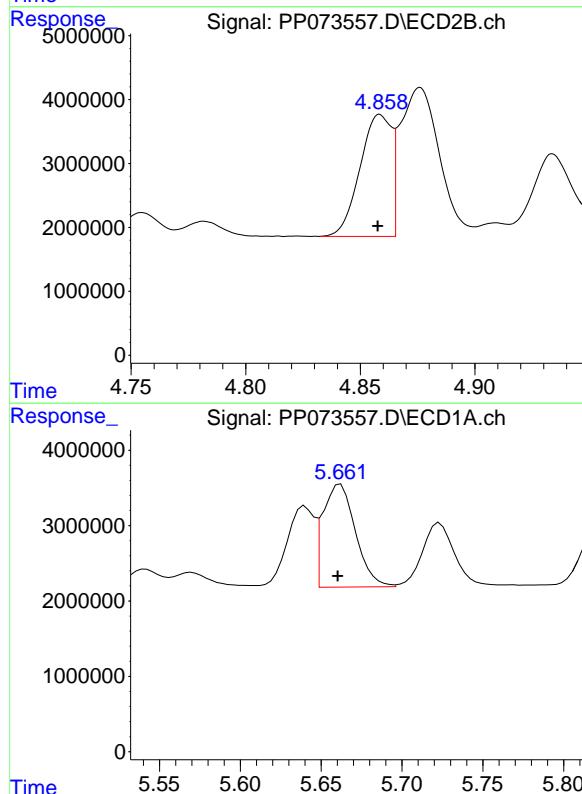


#4 AR-1016-2

R.T.: 5.662 min
 Delta R.T.: 0.002 min
 Response: 19179159
 Conc: 266.20 ng/ml

#4 AR-1016-2


R.T.: 4.876 min
 Delta R.T.: 0.001 min
 Response: 27468197
 Conc: 267.75 ng/ml

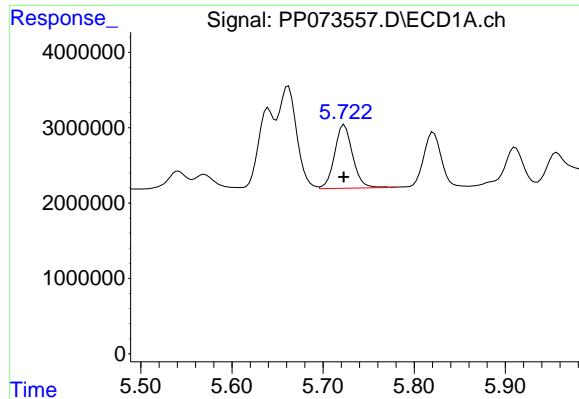

#5 AR-1016-3

R.T.: 5.723 min
Delta R.T.: 0.000 min
Response: 11597460
Conc: 262.61 ng/ml

Instrument: ECD_P
ClientSampleId: AR1660ICC250

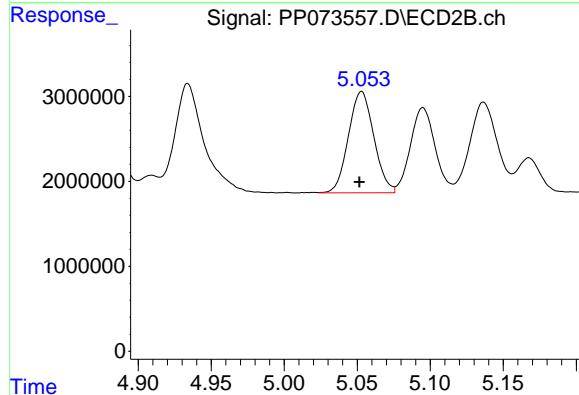


#6 AR-1016-4

R.T.: 5.821 min
Delta R.T.: 0.000 min
Response: 9615182
Conc: 262.77 ng/ml

#6 AR-1016-4

R.T.: 5.095 min
Delta R.T.: 0.002 min
Response: 11760046
Conc: 267.90 ng/ml

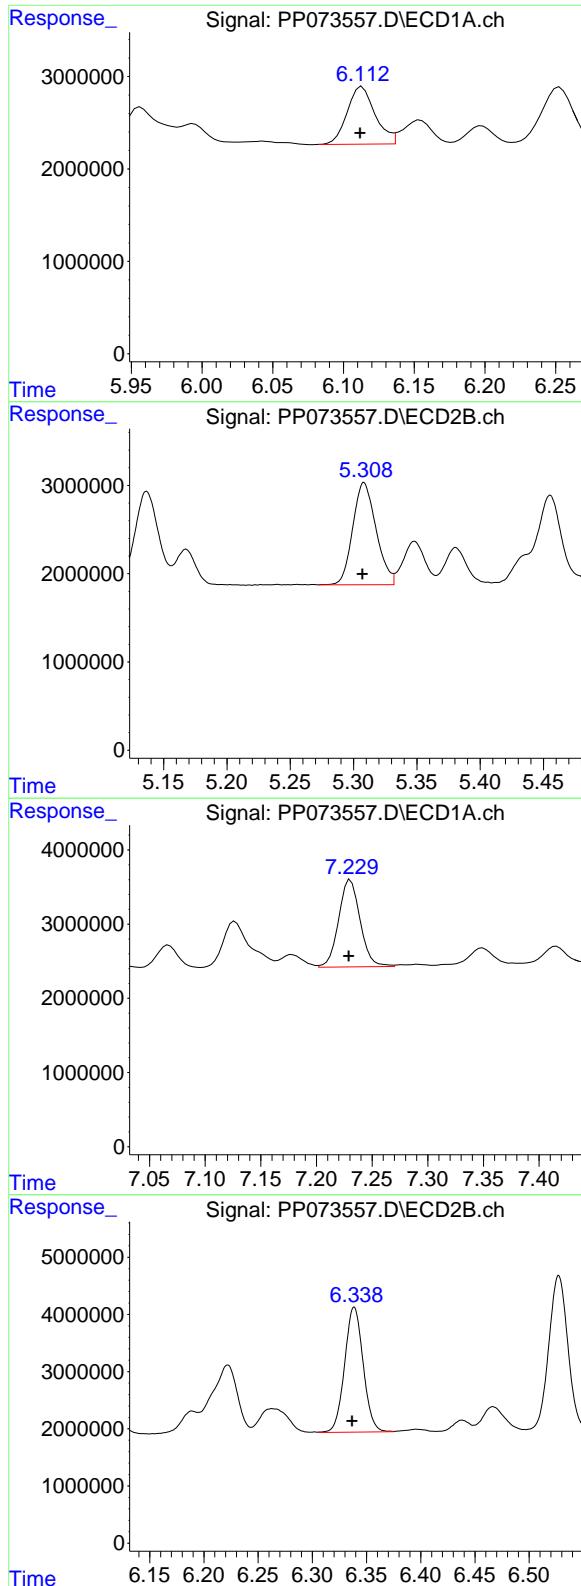

#7 AR-1016-5

R.T.: 6.113 min
 Delta R.T.: 0.001 min
 Response: 8568508
 Conc: 261.34 ng/ml

Instrument: ECD_P
 ClientSampleId: AR1660ICC250

#7 AR-1016-5


R.T.: 5.308 min
 Delta R.T.: 0.001 min
 Response: 14818058
 Conc: 266.22 ng/ml

#31 AR-1260-1

R.T.: 7.231 min
 Delta R.T.: 0.002 min
 Response: 15831007
 Conc: 265.34 ng/ml

#31 AR-1260-1


R.T.: 6.339 min
 Delta R.T.: 0.002 min
 Response: 26051826
 Conc: 261.90 ng/ml

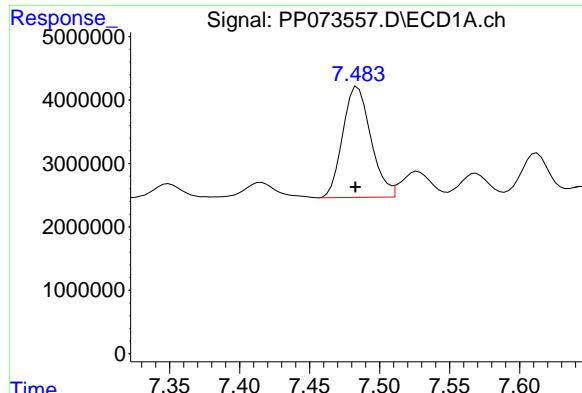

#32 AR-1260-2


R.T.: 7.484 min
Delta R.T.: 0.002 min
Response: 24493361
Conc: 270.96 ng/ml

Instrument: ECD_P
ClientSampleId: AR1660ICC250

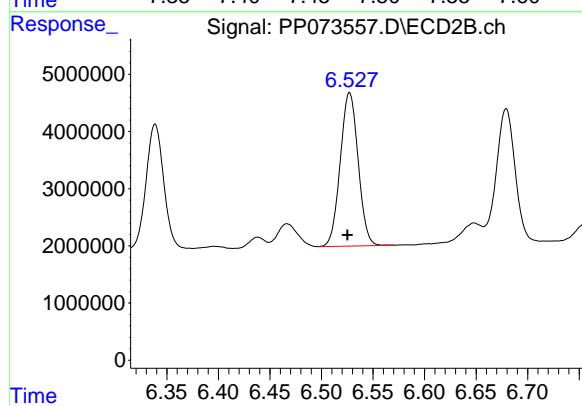


#32 AR-1260-2

R.T.: 6.527 min
Delta R.T.: 0.002 min
Response: 32462748
Conc: 261.79 ng/ml

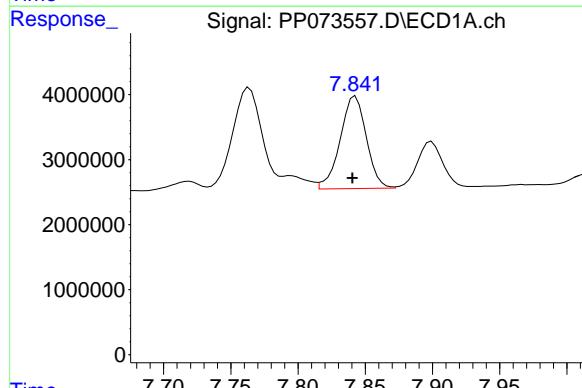


#33 AR-1260-3

R.T.: 7.843 min
Delta R.T.: 0.002 min
Response: 19201014
Conc: 257.07 ng/ml

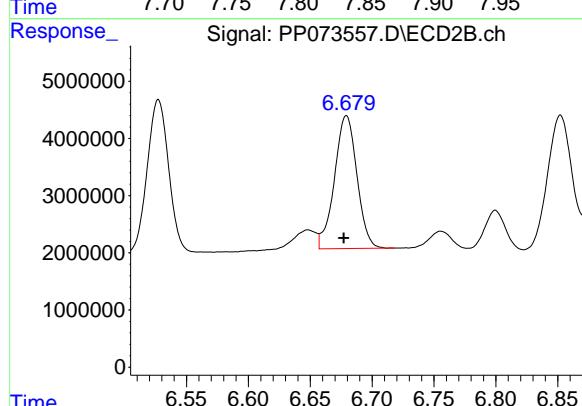

#33 AR-1260-3


R.T.: 6.679 min
Delta R.T.: 0.002 min
Response: 29417085
Conc: 261.97 ng/ml

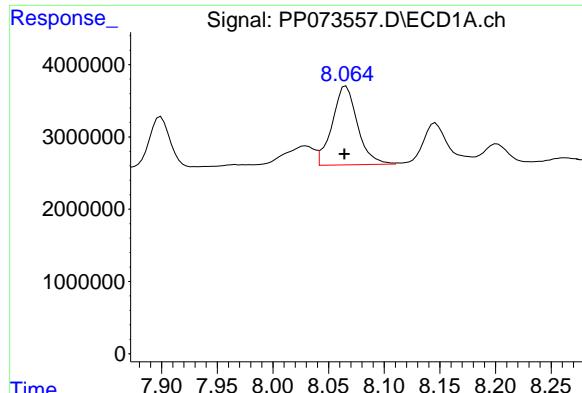

#34 AR-1260-4


R.T.: 8.066 min
 Delta R.T.: 0.001 min
 Response: 17258868
 Conc: 258.64 ng/ml

Instrument: ECD_P
 ClientSampleId: AR1660ICC250

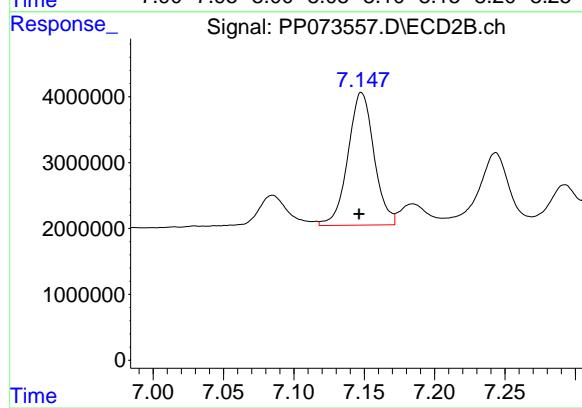


#34 AR-1260-4

R.T.: 7.148 min
 Delta R.T.: 0.002 min
 Response: 25990153
 Conc: 281.43 ng/ml

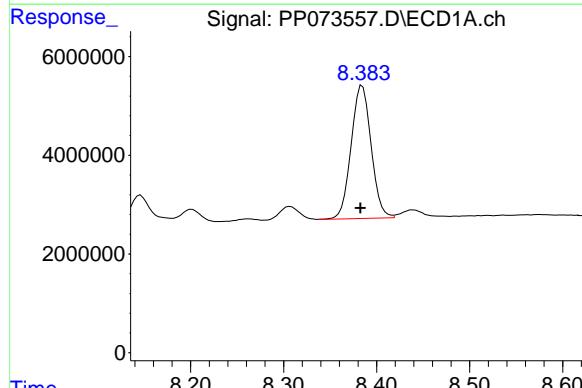

#35 AR-1260-5

R.T.: 8.385 min
 Delta R.T.: 0.002 min
 Response: 40210084
 Conc: 259.59 ng/ml

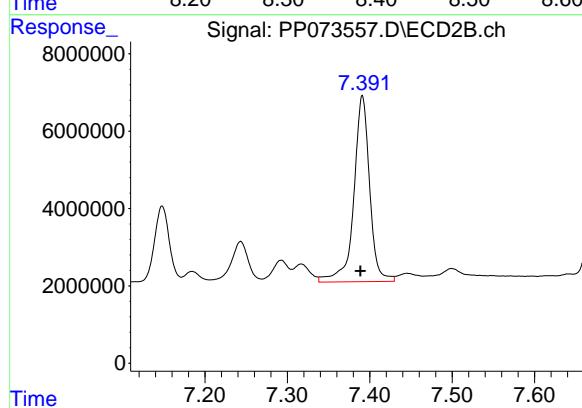

#35 AR-1260-5

R.T.: 7.391 min
 Delta R.T.: 0.002 min
 Response: 64242310
 Conc: 276.64 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP070825\
 Data File : PP073558.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Jul 2025 22:08
 Operator : YP\AJ
 Sample : AR1660ICC050
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
AR1660ICC050

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 08 01:40:50 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 08 01:37:59 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	4.485	3.779	6400868	8634125	4.529	4.609
2) SA Decachlor...	10.173	8.780	4780120	5986472	4.171	4.520

Target Compounds

3) L1 AR-1016-1	5.637	4.857	2553683	3433572	54.174	50.110
4) L1 AR-1016-2	5.658	4.875	3532445	5058097	49.029	49.304
5) L1 AR-1016-3	5.719	5.052	2287754	2711653	51.803	49.438
6) L1 AR-1016-4	5.817	5.094	1779663	2333668	48.635	53.162
7) L1 AR-1016-5	6.109	5.307	1335478	2709671	40.733	48.682
31) L7 AR-1260-1	7.226	6.337	2914675	5720547	48.852	57.510
32) L7 AR-1260-2	7.482	6.525	6085083	6438631	67.317	51.923
33) L7 AR-1260-3	7.838	6.677	3450365	5301254	46.195	47.209
34) L7 AR-1260-4	8.061	7.146	3038521	5704265	45.534	61.768 #
35) L7 AR-1260-5	8.379	7.388	6955237	12058667	44.903	51.927



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP070825\
 Data File : PP073558.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Jul 2025 22:08
 Operator : YP\AJ
 Sample : AR1660ICC050
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
AR1660ICC050

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 08 01:40:50 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 08 01:37:59 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

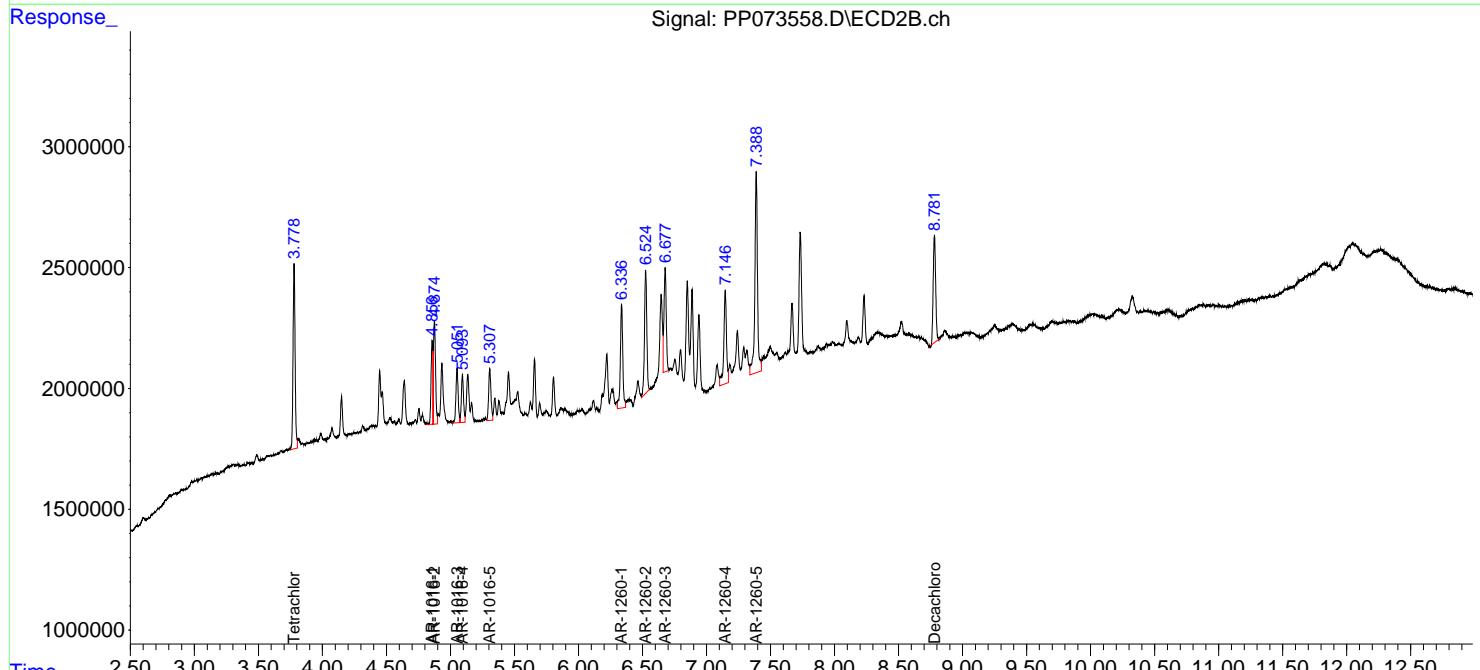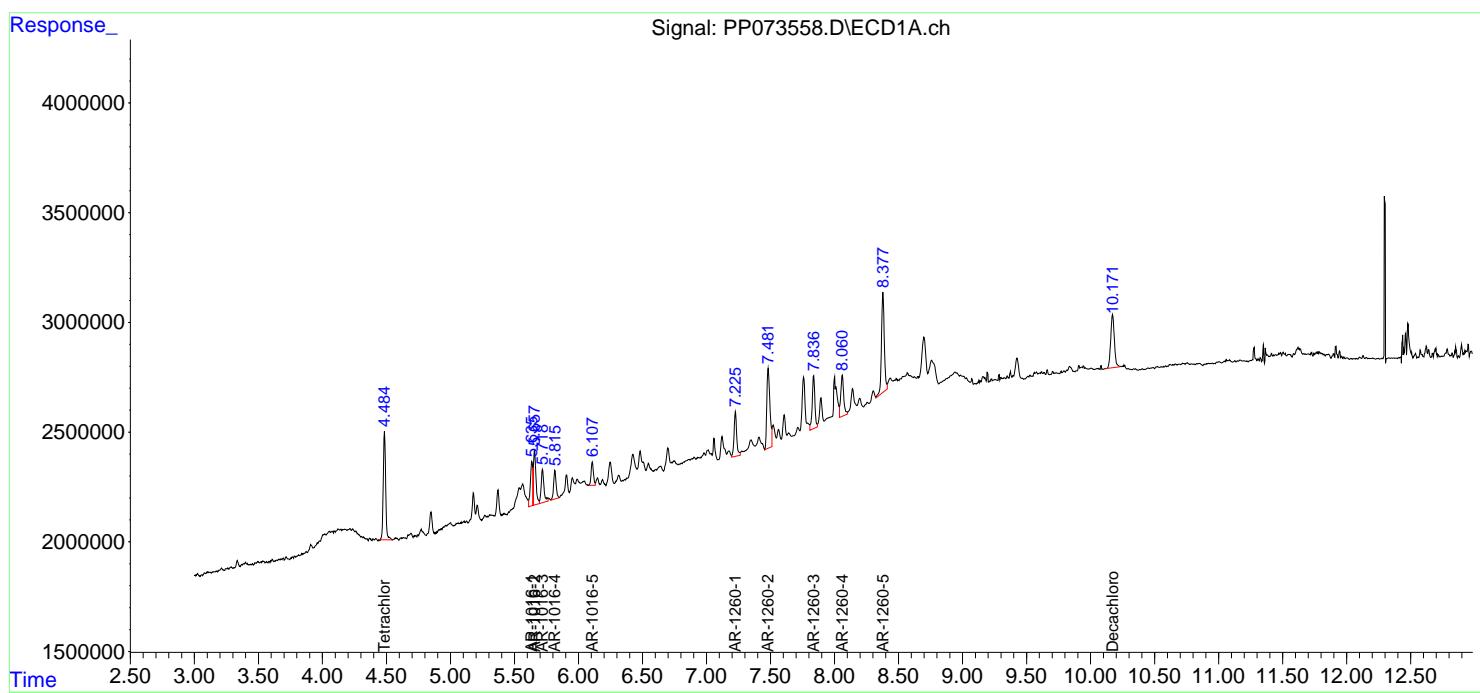

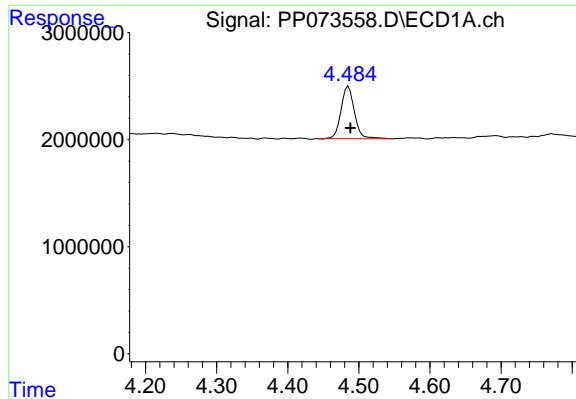

#1 Tetrachloro-m-xylene


R.T.: 4.485 min
Delta R.T.: -0.003 min
Response: 6400868
Conc: 4.53 ng/ml

Instrument:

ECD_P


ClientSampleId :

AR1660ICC050

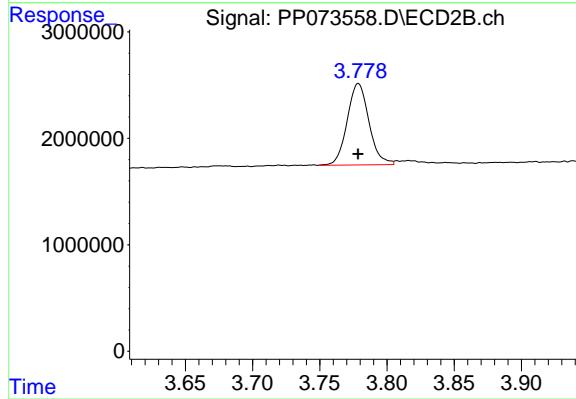


#1 Tetrachloro-m-xylene

R.T.: 3.779 min
Delta R.T.: 0.000 min
Response: 8634125
Conc: 4.61 ng/ml

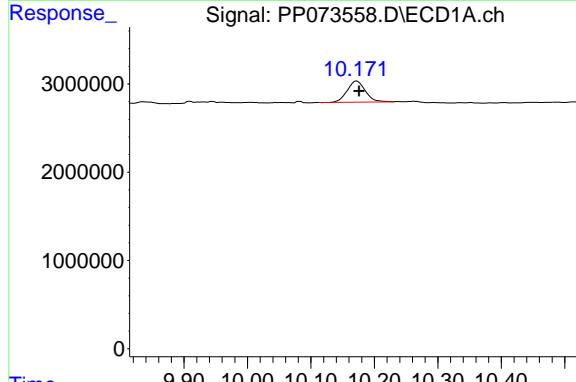


#2 Decachlorobiphenyl

R.T.: 10.173 min
Delta R.T.: -0.004 min
Response: 4780120
Conc: 4.17 ng/ml

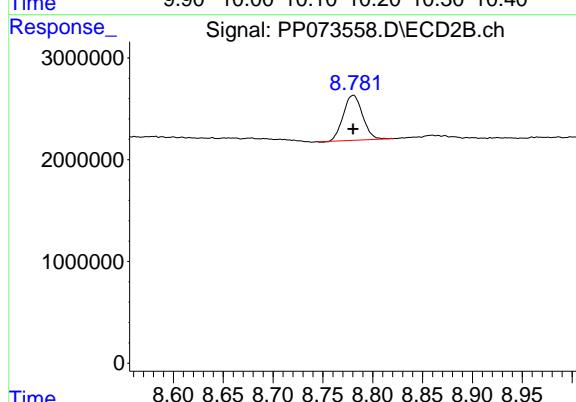

#2 Decachlorobiphenyl


R.T.: 8.780 min
Delta R.T.: 0.000 min
Response: 5986472
Conc: 4.52 ng/ml

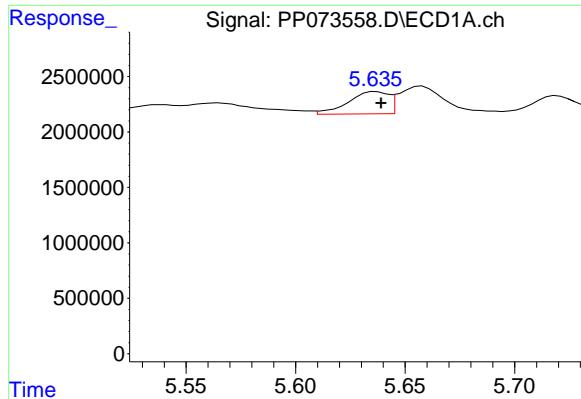

#3 AR-1016-1


R.T.: 5.637 min
Delta R.T.: -0.002 min
Response: 2553683
Conc: 54.17 ng/ml

Instrument: ECD_P
ClientSampleId: AR1660ICC050

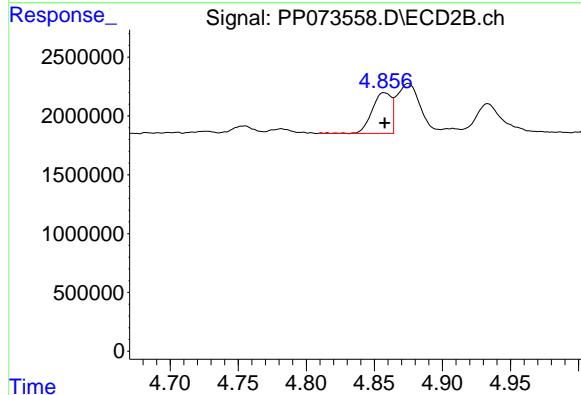


#3 AR-1016-1

R.T.: 4.857 min
Delta R.T.: 0.000 min
Response: 3433572
Conc: 50.11 ng/ml

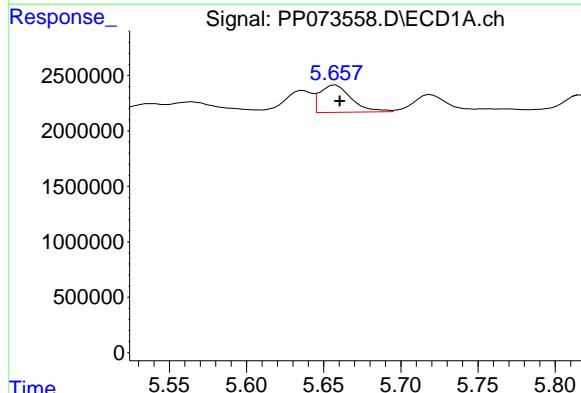


#4 AR-1016-2

R.T.: 5.658 min
Delta R.T.: -0.003 min
Response: 3532445
Conc: 49.03 ng/ml

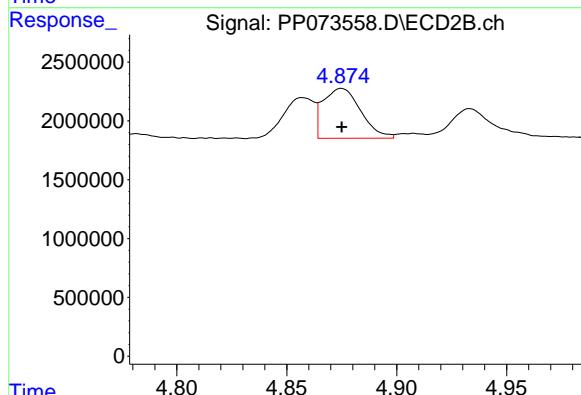

#4 AR-1016-2


R.T.: 4.875 min
Delta R.T.: 0.000 min
Response: 5058097
Conc: 49.30 ng/ml

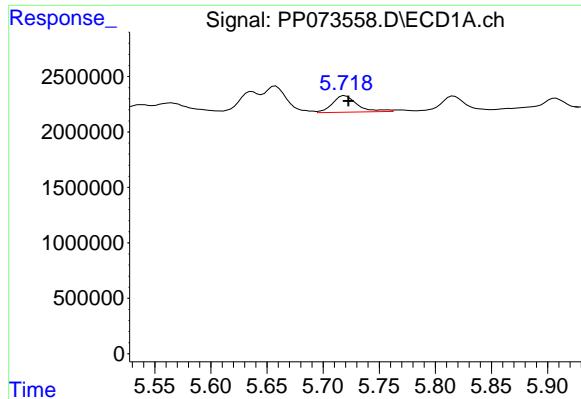

#5 AR-1016-3


R.T.: 5.719 min
Delta R.T.: -0.003 min
Response: 2287754
Conc: 51.80 ng/ml

Instrument: ECD_P
ClientSampleId: AR1660ICC050

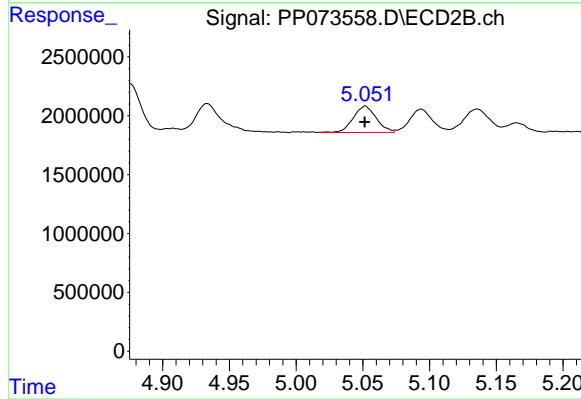


#5 AR-1016-3

R.T.: 5.052 min
Delta R.T.: 0.000 min
Response: 2711653
Conc: 49.44 ng/ml

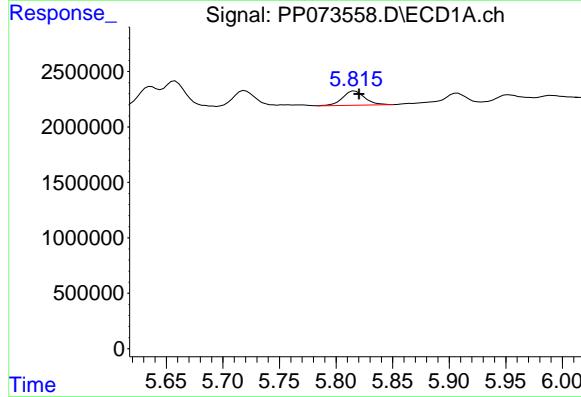


#6 AR-1016-4

R.T.: 5.817 min
Delta R.T.: -0.004 min
Response: 1779663
Conc: 48.64 ng/ml

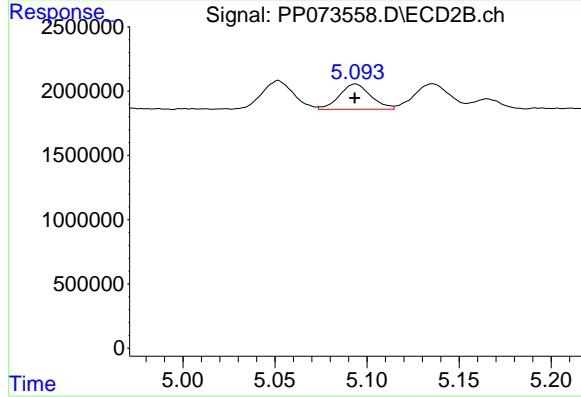

#6 AR-1016-4

R.T.: 5.094 min
Delta R.T.: 0.000 min
Response: 2333668
Conc: 53.16 ng/ml

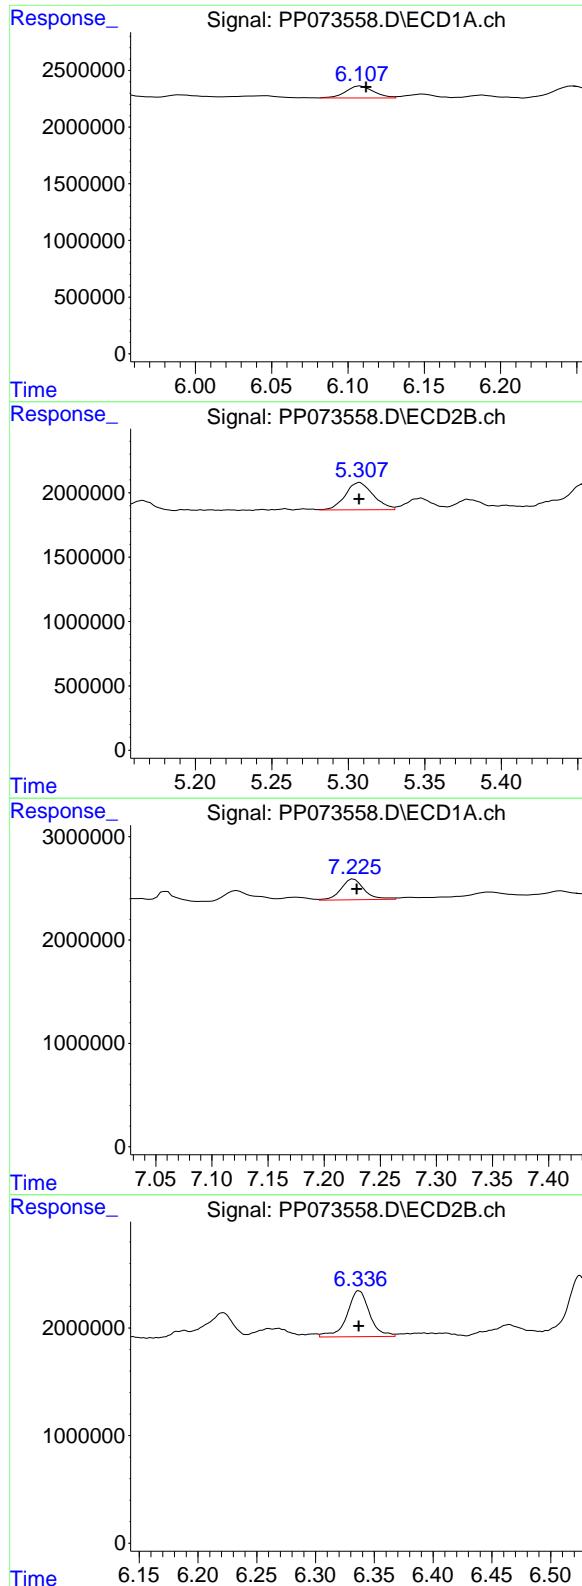

#7 AR-1016-5

R.T.: 6.109 min
 Delta R.T.: -0.003 min
 Response: 1335478
 Conc: 40.73 ng/ml

Instrument: ECD_P
 ClientSampleId: AR1660ICC050

#7 AR-1016-5


R.T.: 5.307 min
 Delta R.T.: 0.000 min
 Response: 2709671
 Conc: 48.68 ng/ml

#31 AR-1260-1

R.T.: 7.226 min
 Delta R.T.: -0.003 min
 Response: 2914675
 Conc: 48.85 ng/ml

#31 AR-1260-1

R.T.: 6.337 min
 Delta R.T.: 0.000 min
 Response: 5720547
 Conc: 57.51 ng/ml

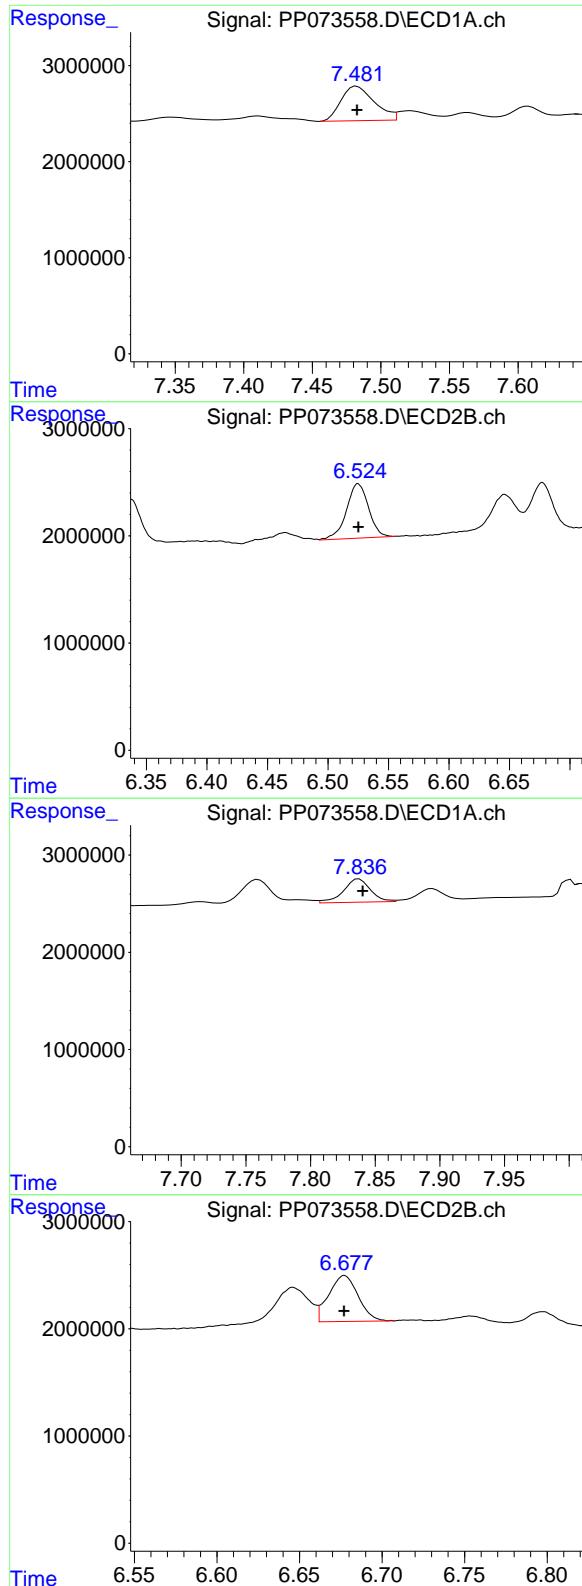

#32 AR-1260-2

R.T.: 7.482 min
 Delta R.T.: 0.000 min
 Response: 6085083
 Conc: 67.32 ng/ml

Instrument: ECD_P
 ClientSampleId: AR1660ICC050

#32 AR-1260-2


R.T.: 6.525 min
 Delta R.T.: 0.000 min
 Response: 6438631
 Conc: 51.92 ng/ml

#33 AR-1260-3

R.T.: 7.838 min
 Delta R.T.: -0.003 min
 Response: 3450365
 Conc: 46.20 ng/ml

#33 AR-1260-3


R.T.: 6.677 min
 Delta R.T.: 0.000 min
 Response: 5301254
 Conc: 47.21 ng/ml

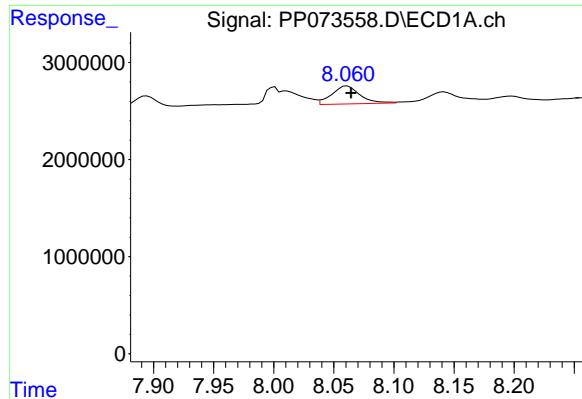

#34 AR-1260-4


R.T.: 8.061 min
Delta R.T.: -0.003 min
Response: 3038521
Conc: 45.53 ng/ml

Instrument: ECD_P
ClientSampleId: AR1660ICC050

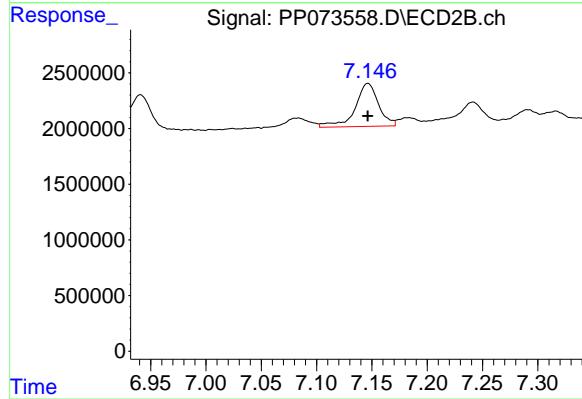


#34 AR-1260-4

R.T.: 7.146 min
Delta R.T.: 0.000 min
Response: 5704265
Conc: 61.77 ng/ml

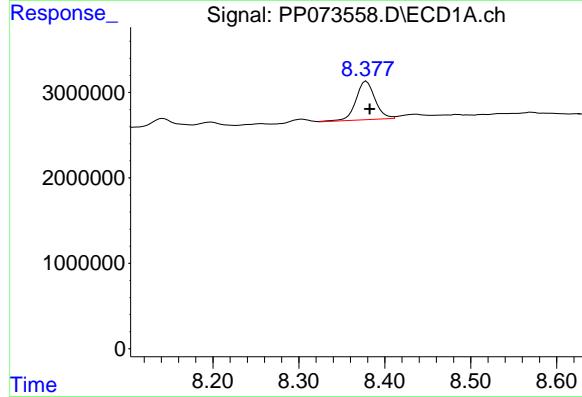

#35 AR-1260-5

R.T.: 8.379 min
Delta R.T.: -0.004 min
Response: 6955237
Conc: 44.90 ng/ml

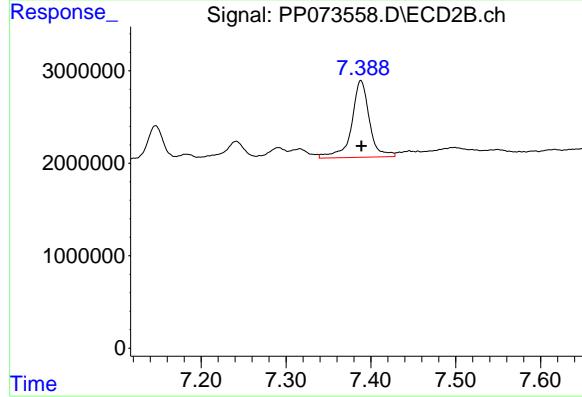

#35 AR-1260-5

R.T.: 7.388 min
Delta R.T.: 0.000 min
Response: 12058667
Conc: 51.93 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP070825\
 Data File : PP073565.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jul 2025 00:03
 Operator : YP\AJ
 Sample : AR1242ICC050
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
AR1242ICC050

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 08 02:05:27 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 08 02:03:06 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	4.487	3.779	6312847	8330986	4.423	4.400
2) SA Decachlor...	10.173	8.780	4963140	5974096	4.336	4.415

Target Compounds

16) L4 AR-1242-1	5.637	4.857	2418928	2804106	59.340	46.472
17) L4 AR-1242-2	5.658	4.875	3555771	4375880	56.321	49.207
18) L4 AR-1242-3	5.721	5.052	2548756	2296207	66.954	48.260 #
19) L4 AR-1242-4	5.818	5.136	1851147	2337623	58.325	51.812
20) L4 AR-1242-5	6.547	5.657	2626667	2688857	78.753	47.117 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP070825\
 Data File : PP073565.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jul 2025 00:03
 Operator : YP\AJ
 Sample : AR1242ICC050
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
AR1242ICC050

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 08 02:05:27 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 08 02:03:06 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

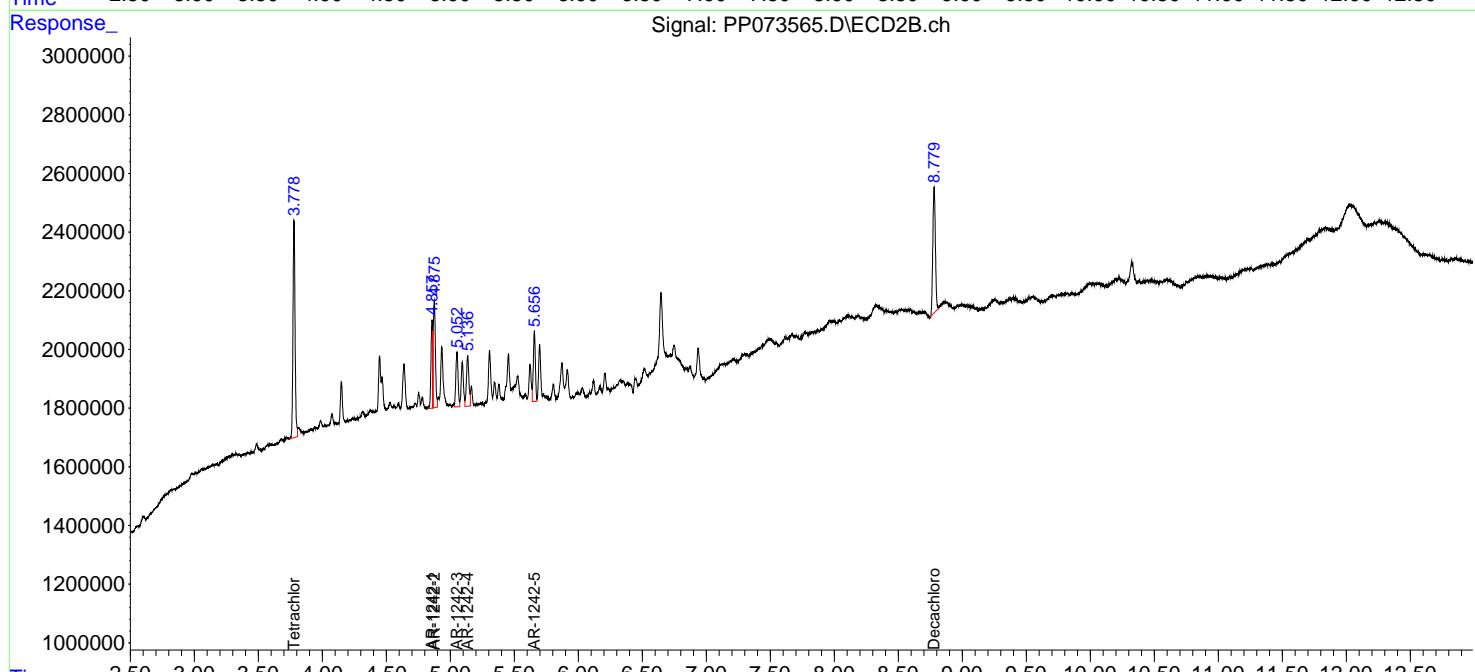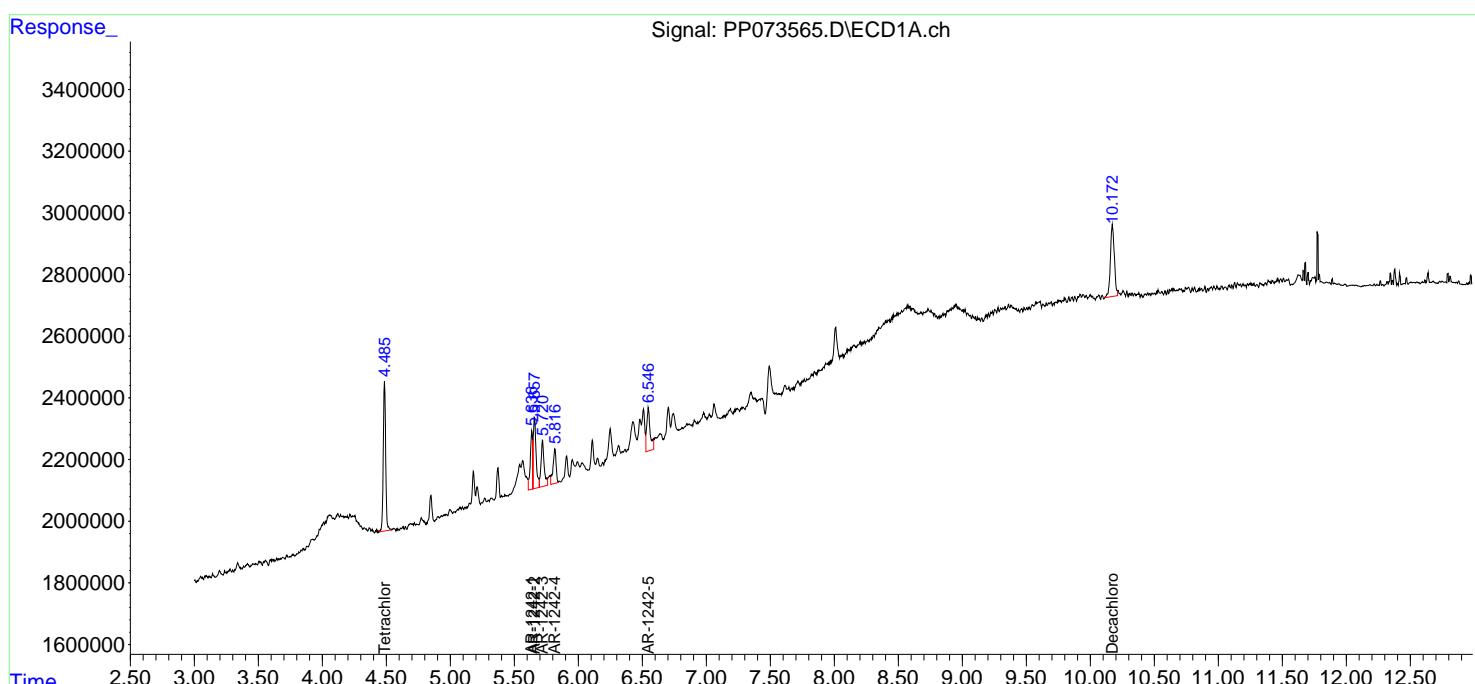


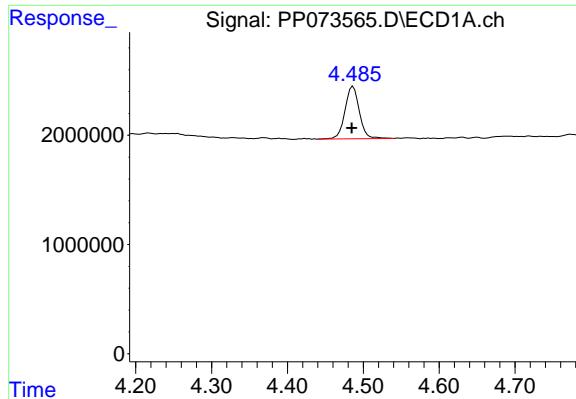

#1 Tetrachloro-m-xylene


R.T.: 4.487 min
Delta R.T.: 0.002 min
Response: 6312847
Conc: 4.42 ng/ml

Instrument: ECD_P
ClientSampleId: AR1242ICC050

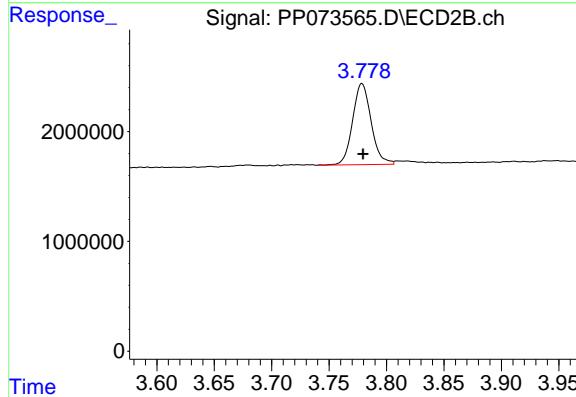


#1 Tetrachloro-m-xylene

R.T.: 3.779 min
Delta R.T.: 0.000 min
Response: 8330986
Conc: 4.40 ng/ml

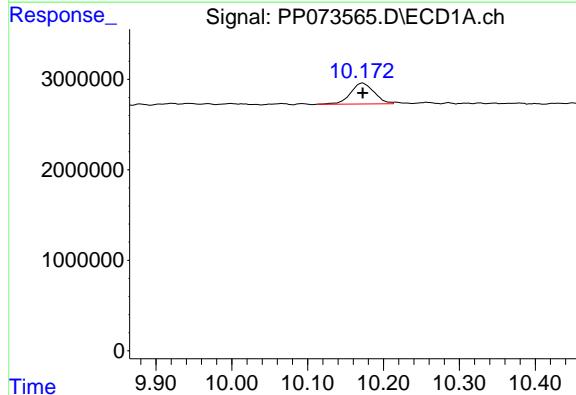


#2 Decachlorobiphenyl

R.T.: 10.173 min
Delta R.T.: 0.000 min
Response: 4963140
Conc: 4.34 ng/ml

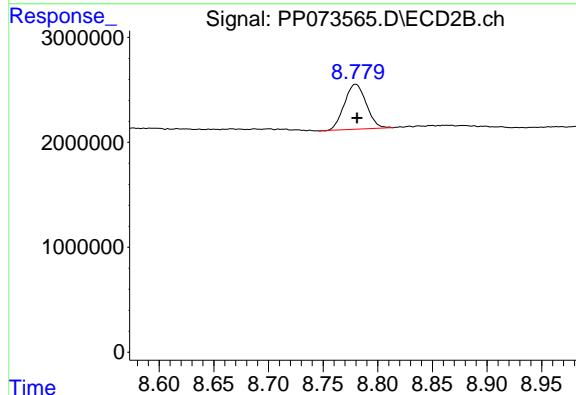

#2 Decachlorobiphenyl

R.T.: 8.780 min
Delta R.T.: -0.001 min
Response: 5974096
Conc: 4.42 ng/ml

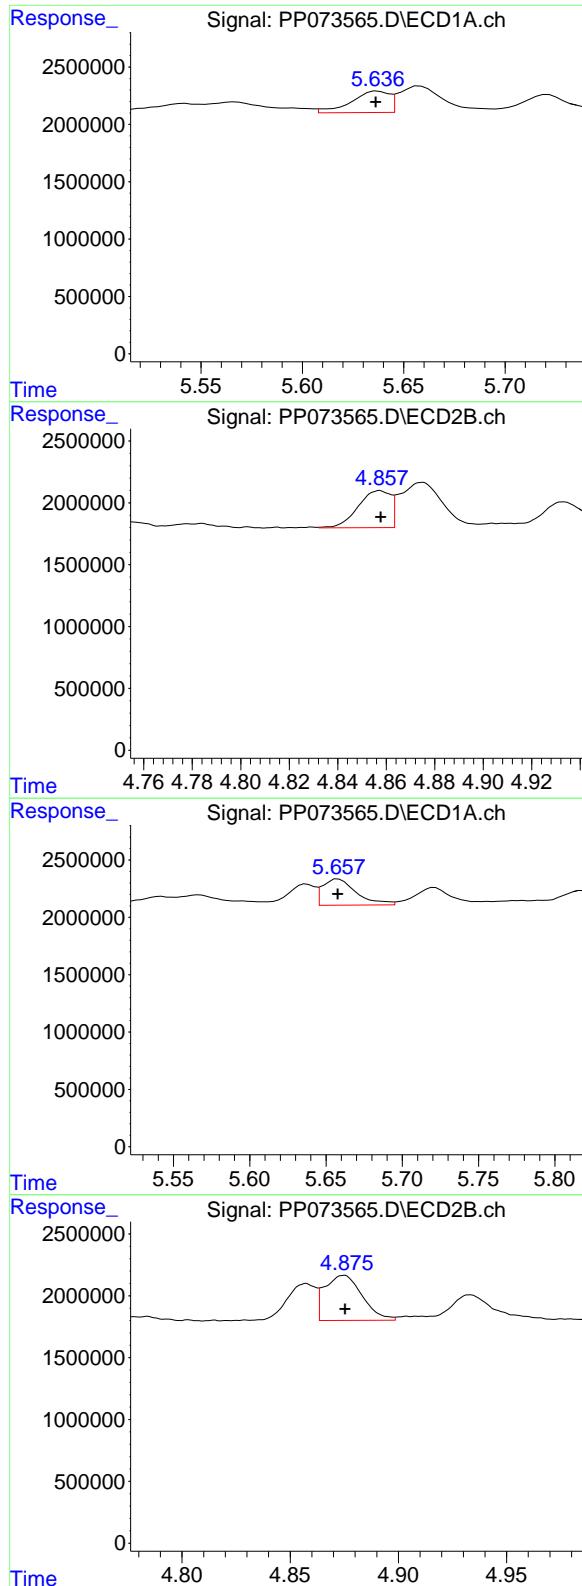

#16 AR-1242-1

R.T.: 5.637 min
 Delta R.T.: 0.001 min **Instrument:**
 Response: 2418928 ECD_P
 Conc: 59.34 ng/ml **ClientSampleId:**
 AR1242ICC050

#16 AR-1242-1


R.T.: 4.857 min
 Delta R.T.: 0.000 min
 Response: 2804106
 Conc: 46.47 ng/ml

#17 AR-1242-2

R.T.: 5.658 min
 Delta R.T.: 0.000 min
 Response: 3555771
 Conc: 56.32 ng/ml

#17 AR-1242-2

R.T.: 4.875 min
 Delta R.T.: 0.000 min
 Response: 4375880
 Conc: 49.21 ng/ml

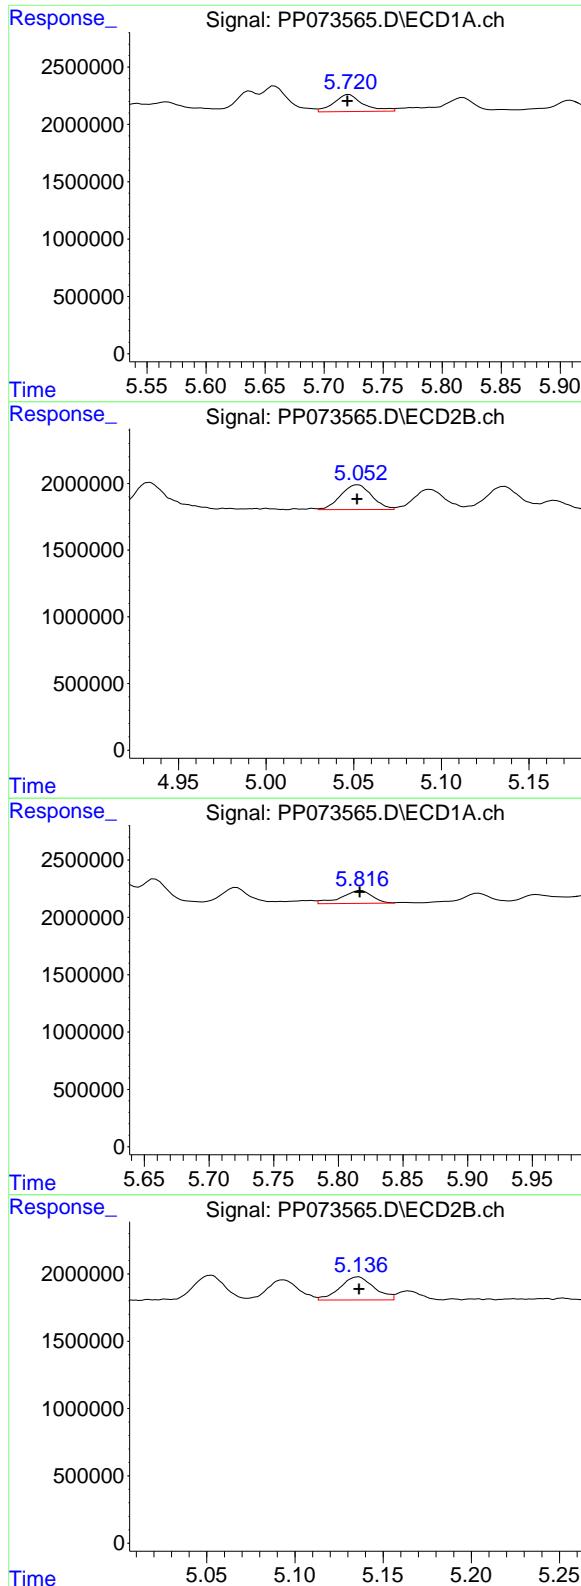

#18 AR-1242-3

R.T.: 5.721 min
 Delta R.T.: 0.002 min
 Response: 2548756
 Conc: 66.95 ng/ml

Instrument: ECD_P
 ClientSampleId: AR1242ICC050

#18 AR-1242-3


R.T.: 5.052 min
 Delta R.T.: 0.000 min
 Response: 2296207
 Conc: 48.26 ng/ml

#19 AR-1242-4

R.T.: 5.818 min
 Delta R.T.: 0.001 min
 Response: 1851147
 Conc: 58.32 ng/ml

#19 AR-1242-4

R.T.: 5.136 min
 Delta R.T.: 0.000 min
 Response: 2337623
 Conc: 51.81 ng/ml

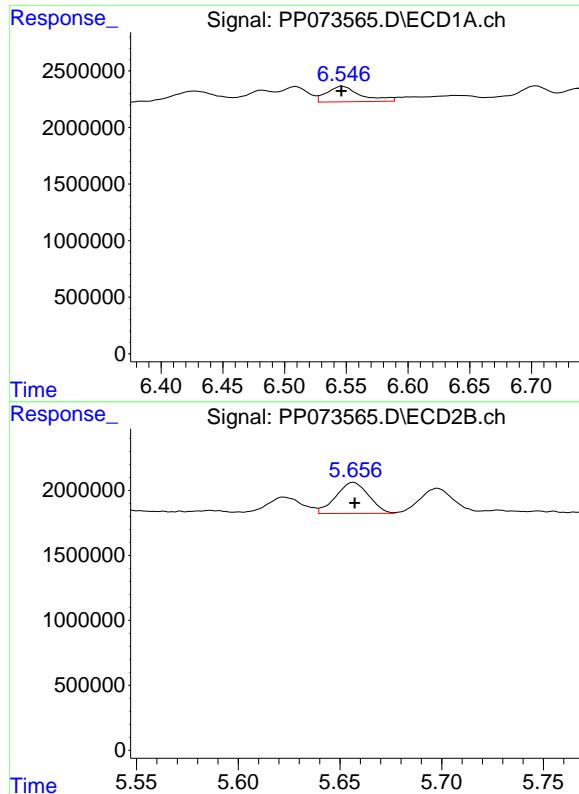

#20 AR-1242-5

R.T.: 6.547 min
Delta R.T.: 0.001 min
Response: 2626667
Conc: 78.75 ng/ml

Instrument: ECD_P
ClientSampleId: AR1242ICC050

#20 AR-1242-5

R.T.: 5.657 min
Delta R.T.: 0.000 min
Response: 2688857
Conc: 47.12 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP070825\
 Data File : PP073570.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jul 2025 01:25
 Operator : YP\AJ
 Sample : AR1248ICC050
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
AR1248ICC050

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 08 02:22:43 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 08 02:20:17 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	4.485	3.779	6203851	8373290	4.383	4.383
2) SA Decachlor...	10.173	8.780	4448332	5794229	3.885	4.259

Target Compounds

21) L5 AR-1248-1	5.635	4.857	1669049	2193065	53.053	48.535
22) L5 AR-1248-2	5.906	5.093	1882218	3238127	46.434	52.322
23) L5 AR-1248-3	6.108	5.135	1881440	3334641	40.834	51.774 #
24) L5 AR-1248-4	6.508	5.307	2994458	3957834	52.399	52.555
25) L5 AR-1248-5	6.546	5.698	3079701	3594939	55.232	47.040



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP070825\
 Data File : PP073570.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jul 2025 01:25
 Operator : YP\AJ
 Sample : AR1248ICC050
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
AR1248ICC050

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 08 02:22:43 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 08 02:20:17 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ m Signal #2 Info : 30M x 0.32mm x 0.25 μ m

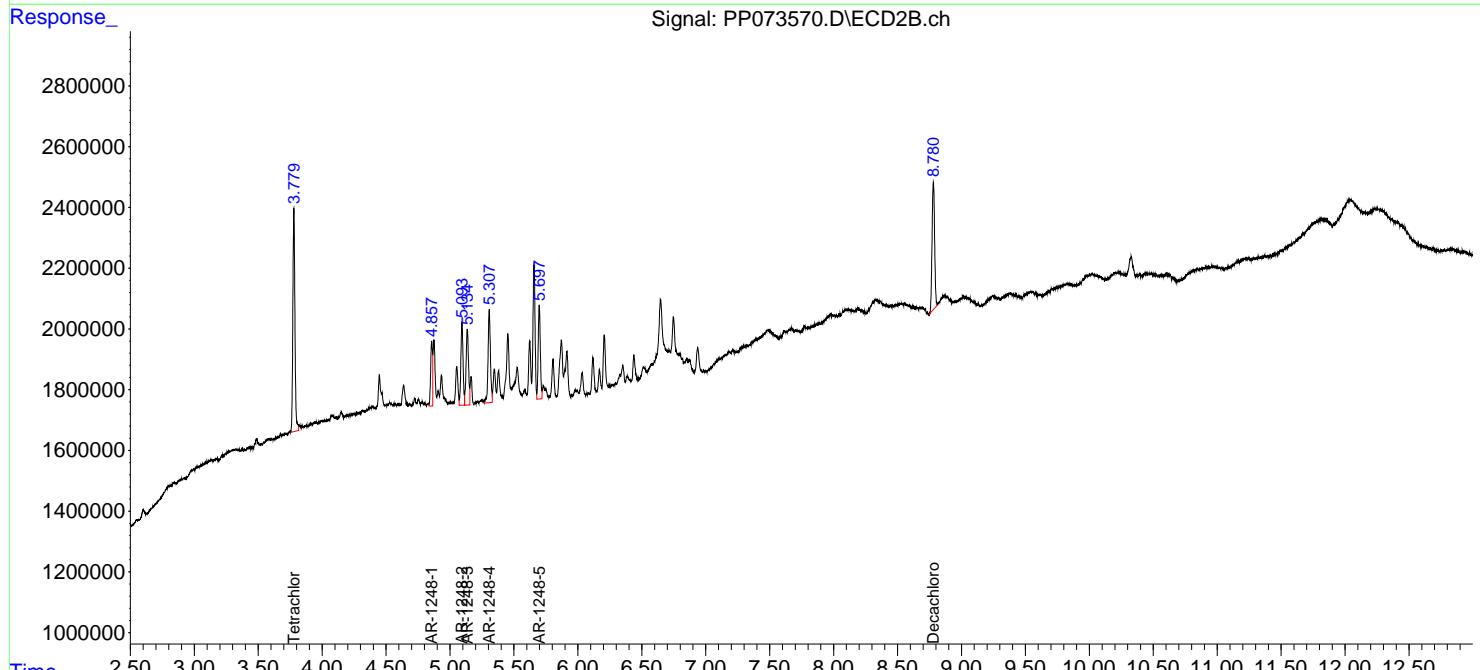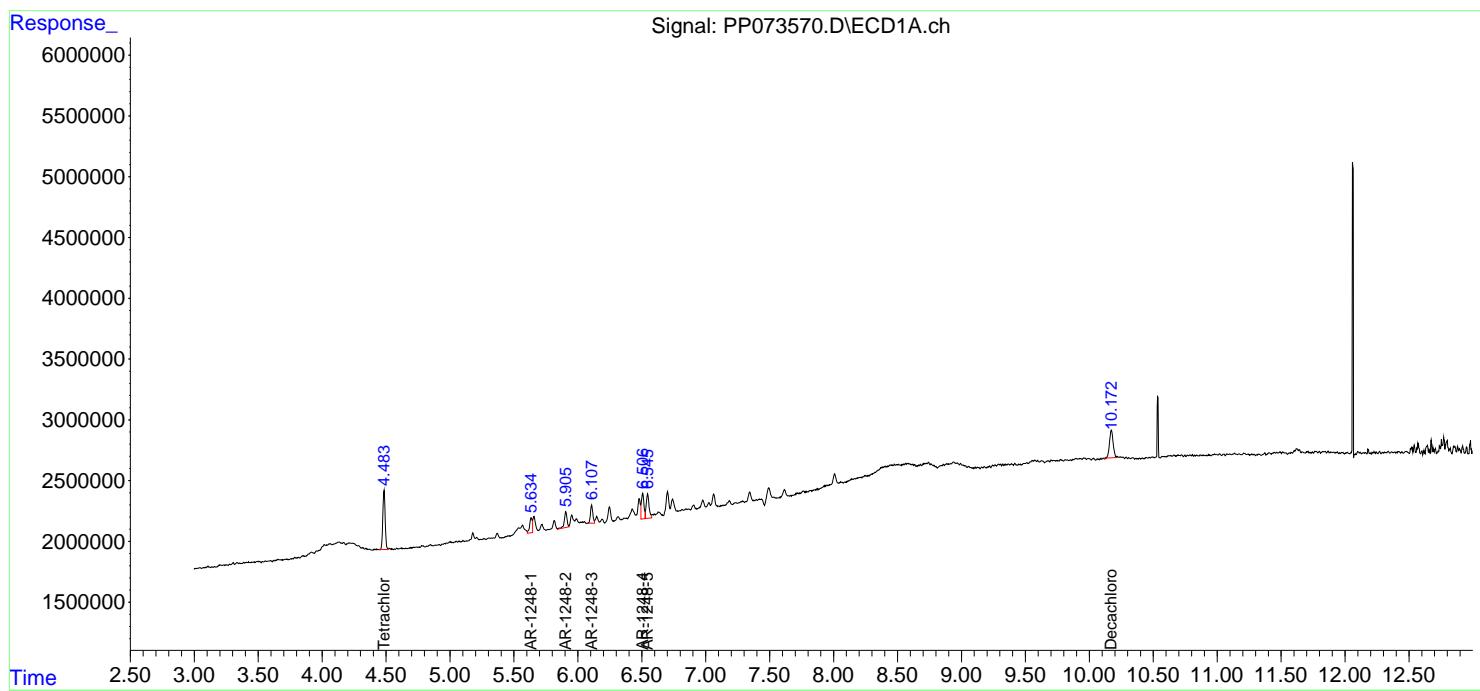

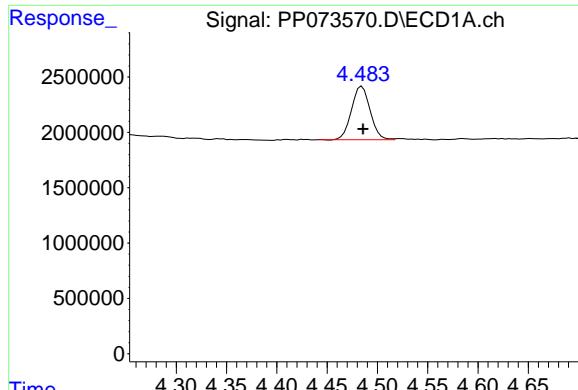

#1 Tetrachloro-m-xylene


R.T.: 4.485 min
Delta R.T.: -0.001 min
Response: 6203851
Conc: 4.38 ng/ml

Instrument:

ECD_P


ClientSampleId :

AR1248ICC050

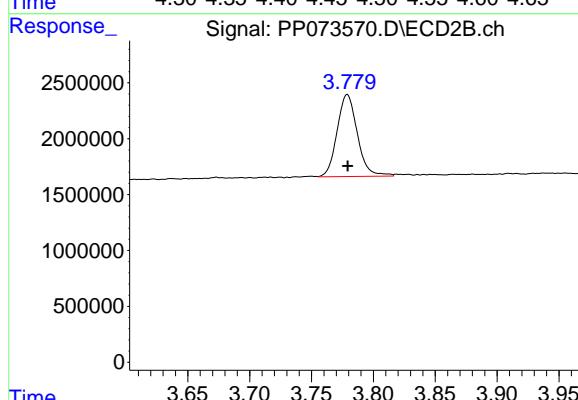


#1 Tetrachloro-m-xylene

R.T.: 3.779 min
Delta R.T.: 0.000 min
Response: 8373290
Conc: 4.38 ng/ml

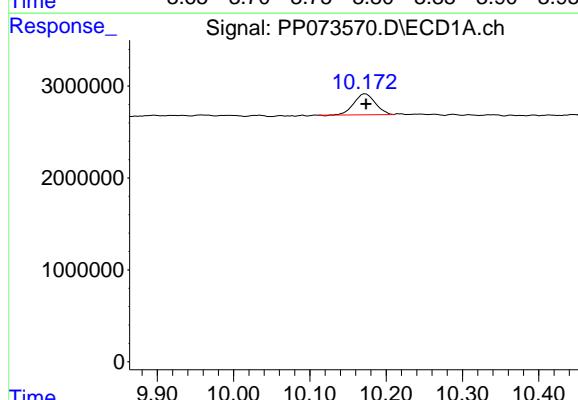


#2 Decachlorobiphenyl

R.T.: 10.173 min
Delta R.T.: 0.000 min
Response: 4448332
Conc: 3.88 ng/ml

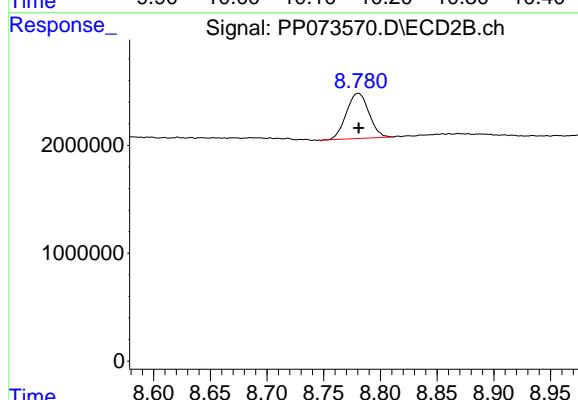

#2 Decachlorobiphenyl

R.T.: 8.780 min
Delta R.T.: 0.000 min
Response: 5794229
Conc: 4.26 ng/ml

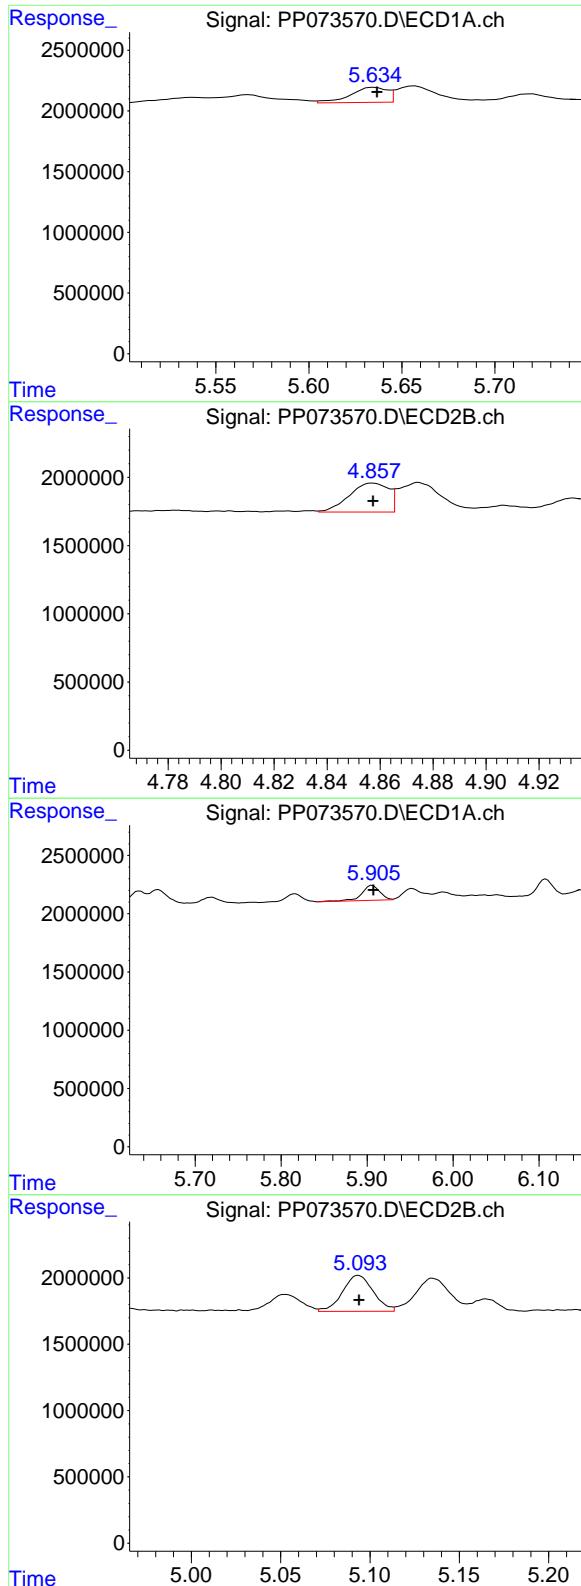

#21 AR-1248-1

R.T.: 5.635 min
 Delta R.T.: -0.001 min
 Response: 1669049
 Conc: 53.05 ng/ml

Instrument: ECD_P
 ClientSampleId: AR1248ICC050

#21 AR-1248-1


R.T.: 4.857 min
 Delta R.T.: 0.000 min
 Response: 2193065
 Conc: 48.53 ng/ml

#22 AR-1248-2

R.T.: 5.906 min
 Delta R.T.: -0.001 min
 Response: 1882218
 Conc: 46.43 ng/ml

#22 AR-1248-2

R.T.: 5.093 min
 Delta R.T.: 0.000 min
 Response: 3238127
 Conc: 52.32 ng/ml

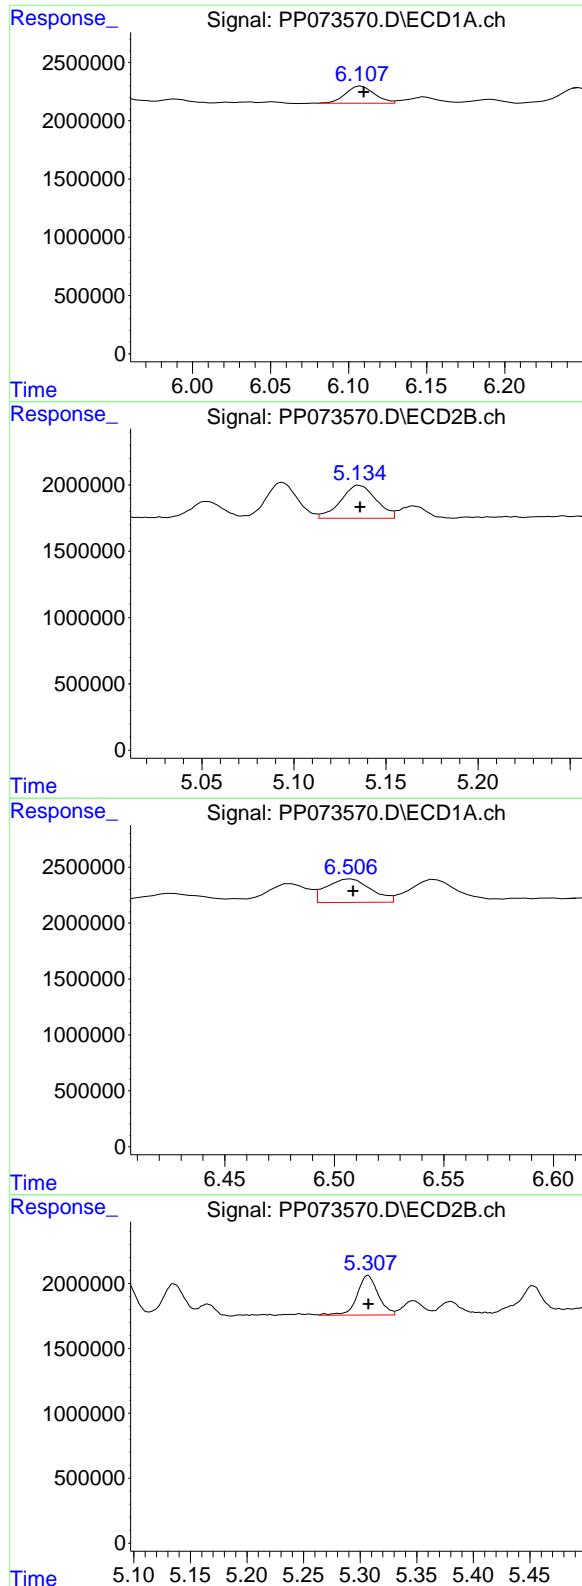

#23 AR-1248-3

R.T.: 6.108 min
 Delta R.T.: -0.001 min
 Response: 1881440
 Conc: 40.83 ng/ml

Instrument: ECD_P
 ClientSampleId: AR1248ICC050

#23 AR-1248-3


R.T.: 5.135 min
 Delta R.T.: 0.000 min
 Response: 3334641
 Conc: 51.77 ng/ml

#24 AR-1248-4

R.T.: 6.508 min
 Delta R.T.: 0.000 min
 Response: 2994458
 Conc: 52.40 ng/ml

#24 AR-1248-4

R.T.: 5.307 min
 Delta R.T.: 0.000 min
 Response: 3957834
 Conc: 52.56 ng/ml

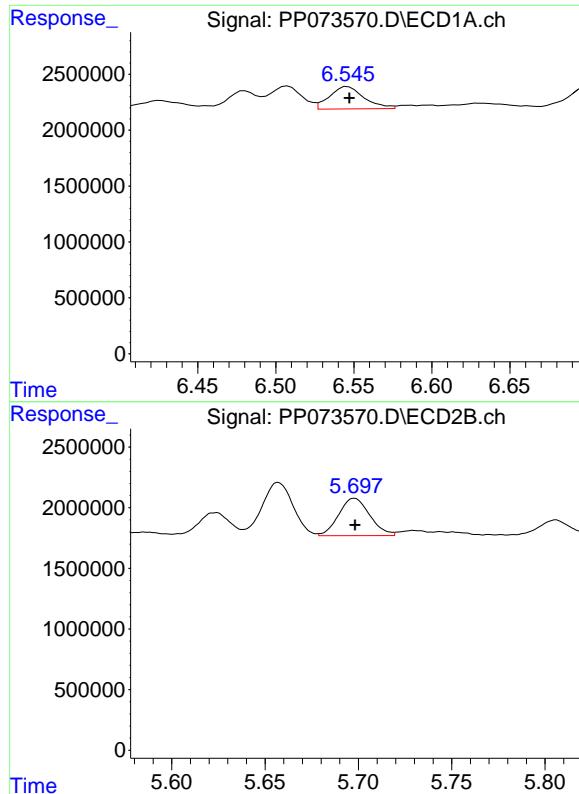

#25 AR-1248-5

R.T.: 6.546 min
Delta R.T.: -0.001 min
Response: 3079701
Conc: 55.23 ng/ml

Instrument: ECD_P
ClientSampleId: AR1248ICC050

#25 AR-1248-5

R.T.: 5.698 min
Delta R.T.: 0.000 min
Response: 3594939
Conc: 47.04 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP070825\
 Data File : PP073575.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jul 2025 02:46
 Operator : YP\AJ
 Sample : AR1254ICC050
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
AR1254ICC050

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 08 03:42:13 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 08 02:41:54 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	4.488	3.779	6938090	9721913	4.952	5.138
2) SA Decachlor...	10.178	8.780	5667149	6887289	4.948	5.019

Target Compounds

26) L6 AR-1254-1	6.486	5.657	3346488	6452648	60.615	57.447
27) L6 AR-1254-2	6.703	5.806	4971490	5754555	60.232	59.894
28) L6 AR-1254-3	7.065	6.207	5174325	8163980	58.472	53.675
29) L6 AR-1254-4	7.349	6.436	5012264	4857854	62.974	51.487
30) L6 AR-1254-5	7.764	6.851	3548489	7039930	47.554	53.848



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP070825\
 Data File : PP073575.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jul 2025 02:46
 Operator : YP\AJ
 Sample : AR1254ICC050
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
AR1254ICC050

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 08 03:42:13 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 08 02:41:54 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

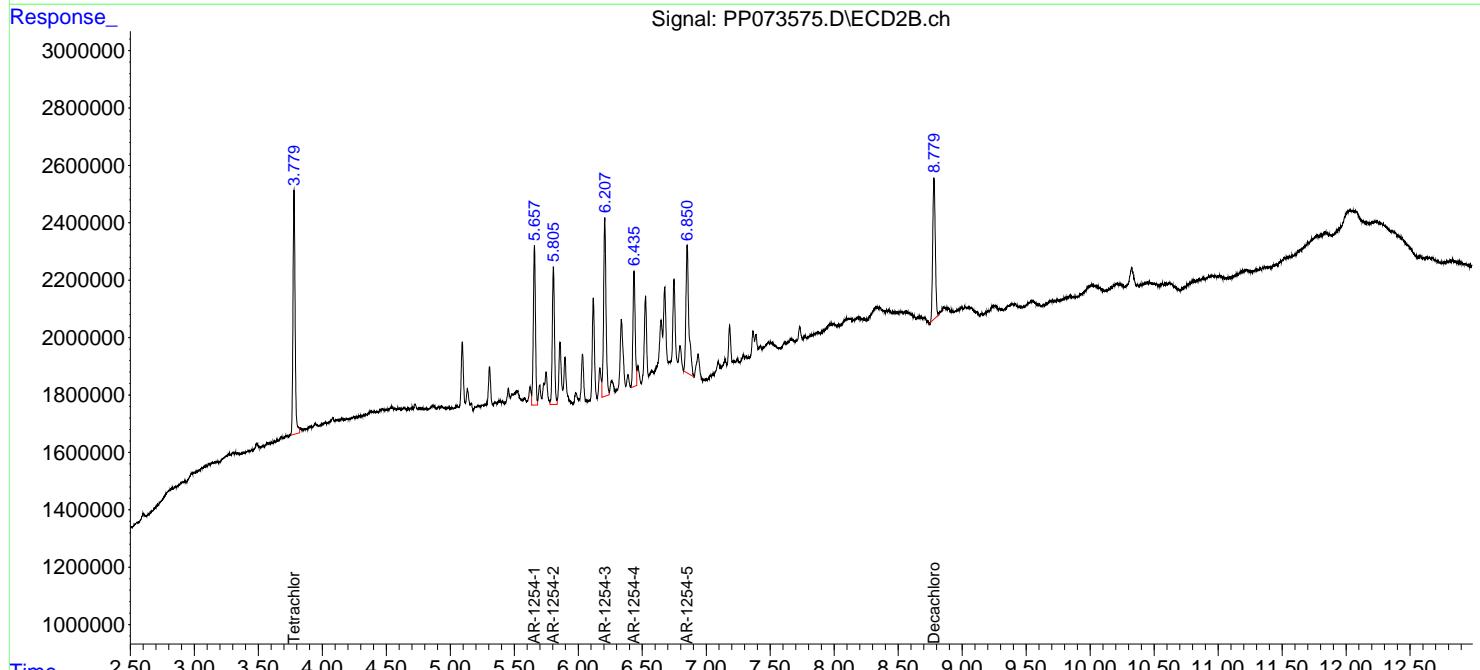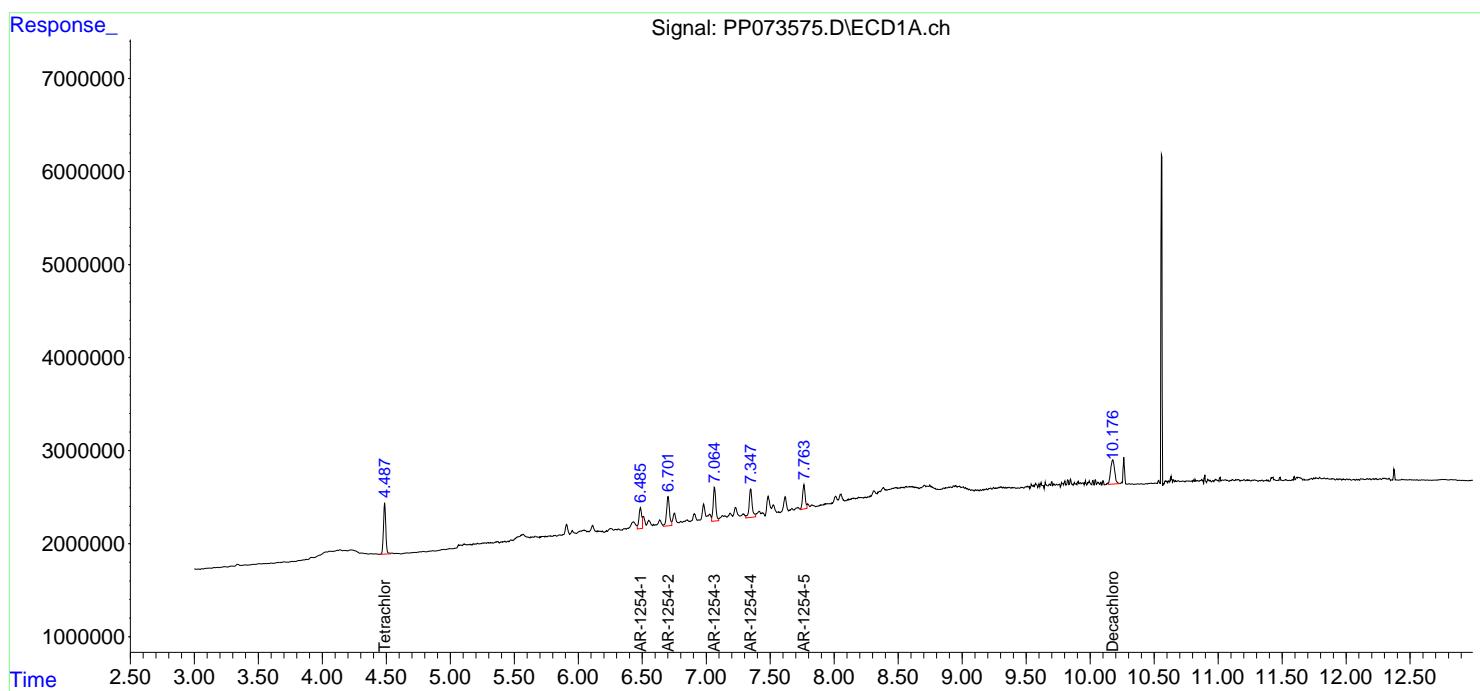


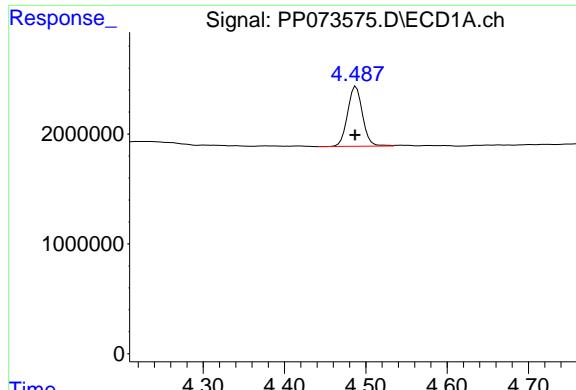

#1 Tetrachloro-m-xylene


R.T.: 4.488 min
Delta R.T.: 0.001 min
Response: 6938090
Conc: 4.95 ng/ml

Instrument: ECD_P
ClientSampleId: AR1254ICC050

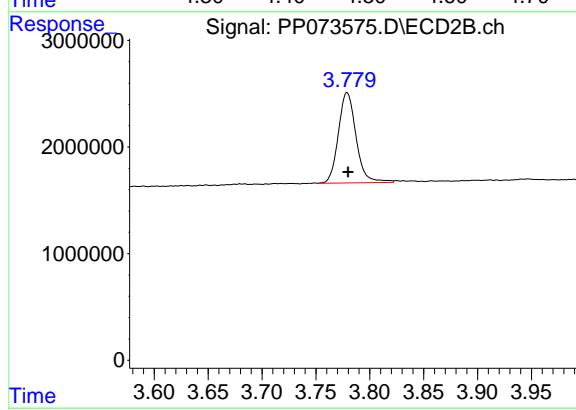


#1 Tetrachloro-m-xylene

R.T.: 3.779 min
Delta R.T.: 0.000 min
Response: 9721913
Conc: 5.14 ng/ml

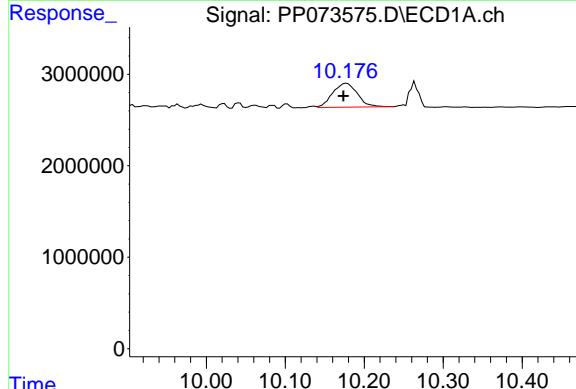


#2 Decachlorobiphenyl

R.T.: 10.178 min
Delta R.T.: 0.004 min
Response: 5667149
Conc: 4.95 ng/ml

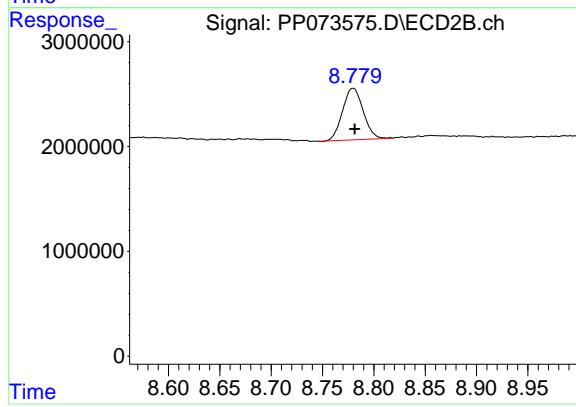

#2 Decachlorobiphenyl

R.T.: 8.780 min
Delta R.T.: -0.002 min
Response: 6887289
Conc: 5.02 ng/ml

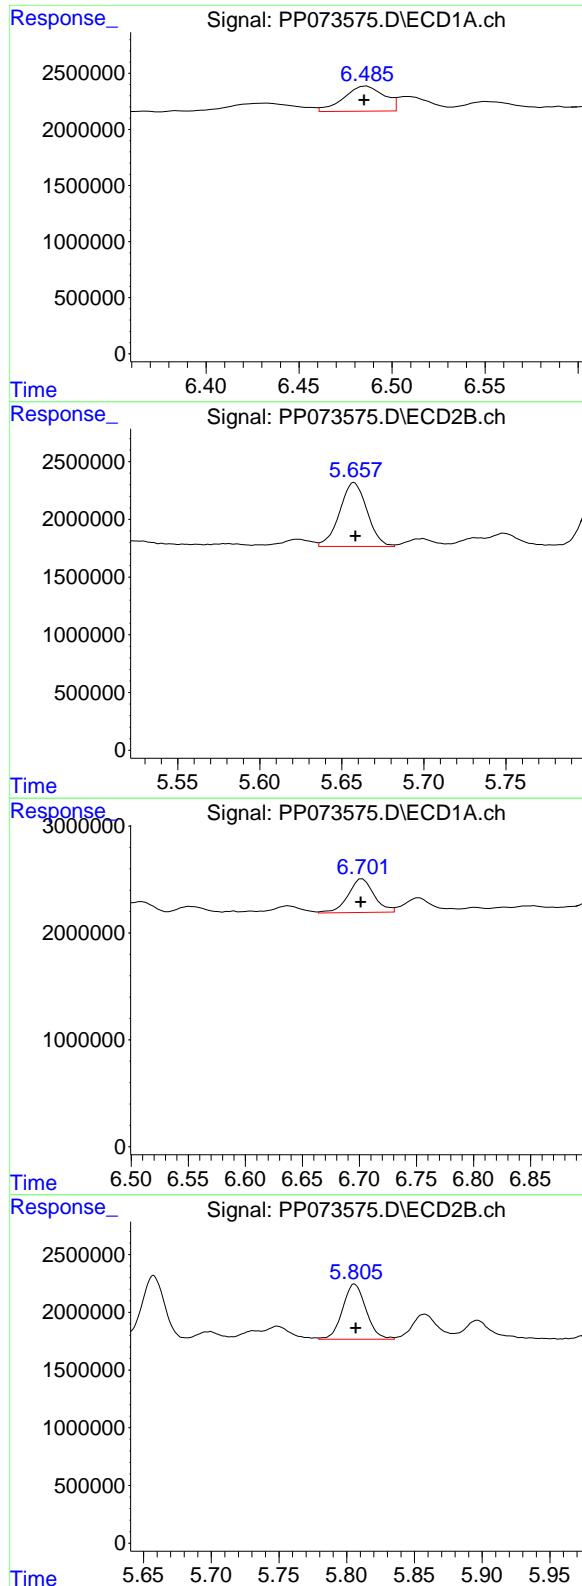

#26 AR-1254-1

R.T.: 6.486 min
 Delta R.T.: 0.002 min
 Response: 3346488
 Conc: 60.61 ng/ml

Instrument: ECD_P
 ClientSampleId: AR1254ICC050

#26 AR-1254-1


R.T.: 5.657 min
 Delta R.T.: 0.000 min
 Response: 6452648
 Conc: 57.45 ng/ml

#27 AR-1254-2

R.T.: 6.703 min
 Delta R.T.: 0.002 min
 Response: 4971490
 Conc: 60.23 ng/ml

#27 AR-1254-2


R.T.: 5.806 min
 Delta R.T.: 0.000 min
 Response: 5754555
 Conc: 59.89 ng/ml

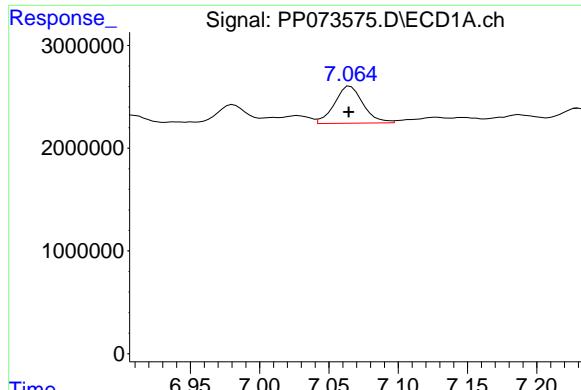

#28 AR-1254-3


R.T.: 7.065 min
Delta R.T.: 0.000 min
Response: 5174325
Conc: 58.47 ng/ml

Instrument: ECD_P
ClientSampleId: AR1254ICC050

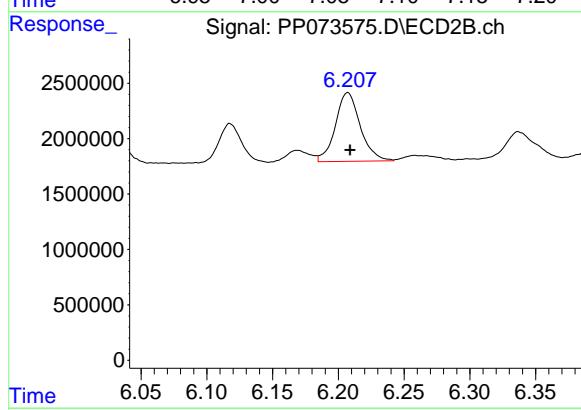


#28 AR-1254-3

R.T.: 6.207 min
Delta R.T.: -0.002 min
Response: 8163980
Conc: 53.68 ng/ml

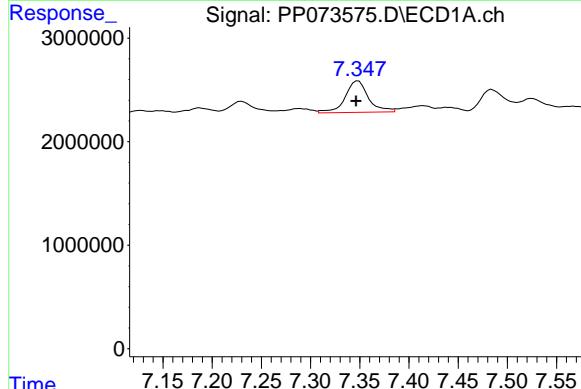


#29 AR-1254-4

R.T.: 7.349 min
Delta R.T.: 0.002 min
Response: 5012264
Conc: 62.97 ng/ml

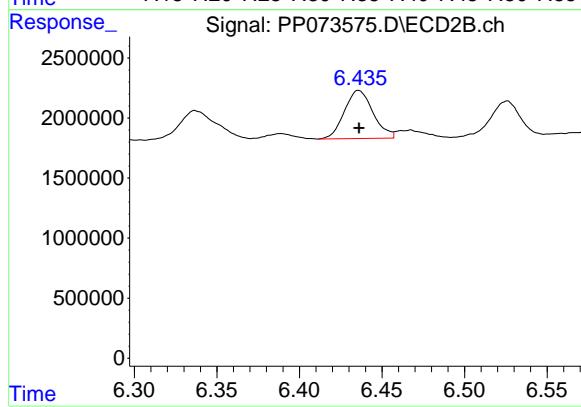

#29 AR-1254-4

R.T.: 6.436 min
Delta R.T.: 0.000 min
Response: 4857854
Conc: 51.49 ng/ml

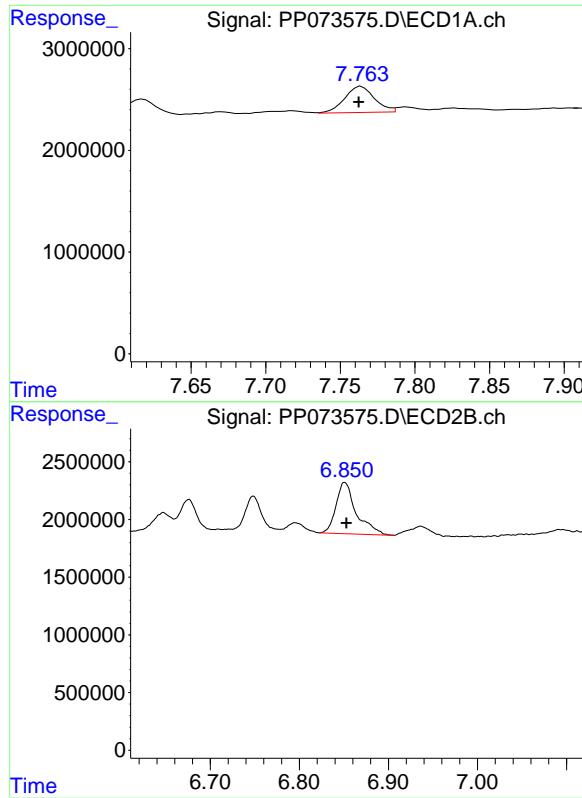

#30 AR-1254-5

R.T.: 7.764 min
Delta R.T.: 0.002 min
Response: 3548489
Conc: 47.55 ng/ml

Instrument: ECD_P
ClientSampleId: AR1254ICC050

#30 AR-1254-5

R.T.: 6.851 min
Delta R.T.: -0.002 min
Response: 7039930
Conc: 53.85 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP070825\
 Data File : PP073580.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jul 2025 04:08
 Operator : YP\AJ
 Sample : AR1268ICC250
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
AR1268ICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 08 04:41:57 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 08 04:40:39 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	4.485	3.779	37383725	50542988	26.404	26.083
2) SA Decachlor...	10.171	8.781	54731552	67087696	26.607	26.464

Target Compounds

41) L9 AR-1268-1	8.690	7.668	59422367	81364216	260.528	264.345
42) L9 AR-1268-2	8.783	7.735	50730840	70740492	261.191	264.376
43) L9 AR-1268-3	9.010	7.936	43805027	60554343	262.765	266.395
44) L9 AR-1268-4	9.428	8.231	18771767	24970476	269.872	262.245
45) L9 AR-1268-5	9.839	8.525	124.3E6	162.7E6	256.278	261.384



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP070825\
 Data File : PP073580.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jul 2025 04:08
 Operator : YP\AJ
 Sample : AR1268ICC250
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
AR1268ICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 08 04:41:57 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 08 04:40:39 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

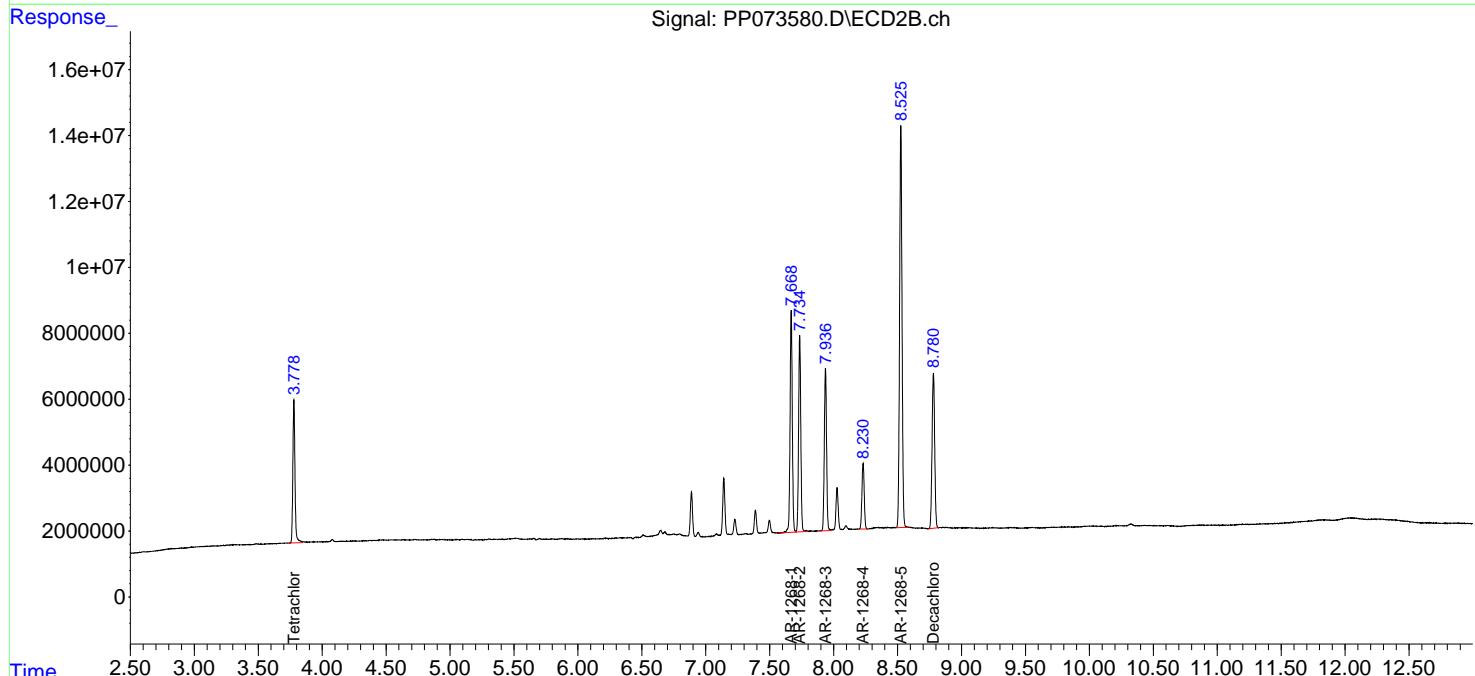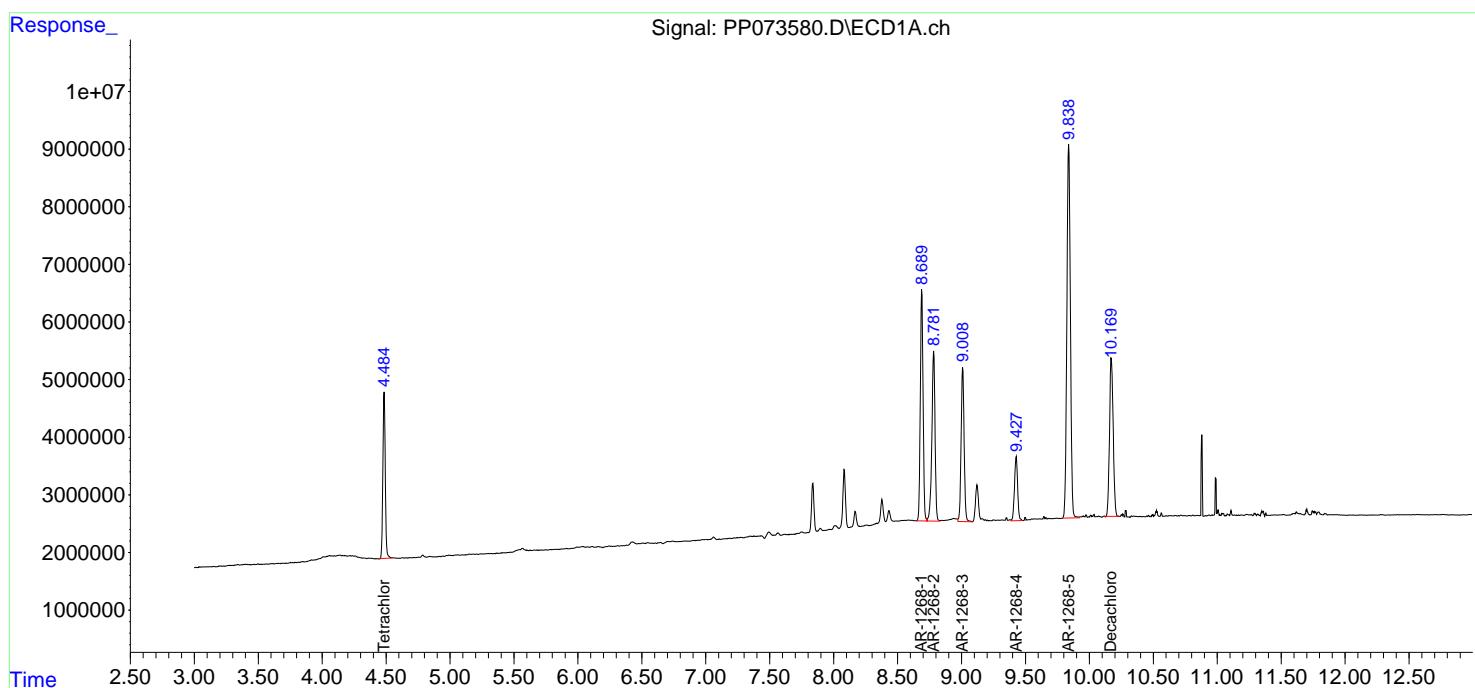

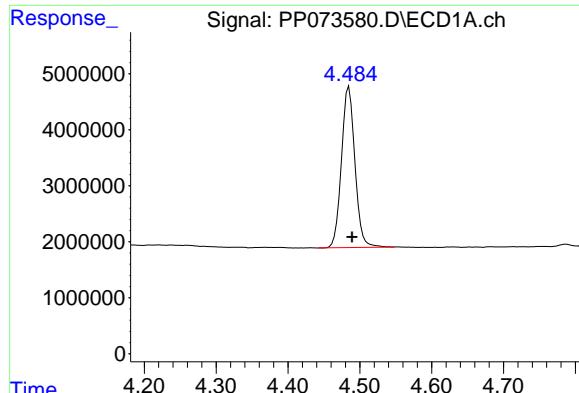

#1 Tetrachloro-m-xylene


R.T.: 4.485 min
Delta R.T.: -0.004 min
Response: 37383725
Conc: 26.40 ng/ml

Instrument:

ECD_P


ClientSampleId :

AR1268ICC250

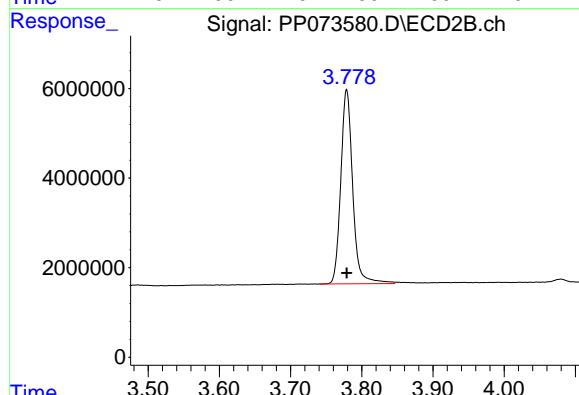


#1 Tetrachloro-m-xylene

R.T.: 3.779 min
Delta R.T.: 0.000 min
Response: 50542988
Conc: 26.08 ng/ml

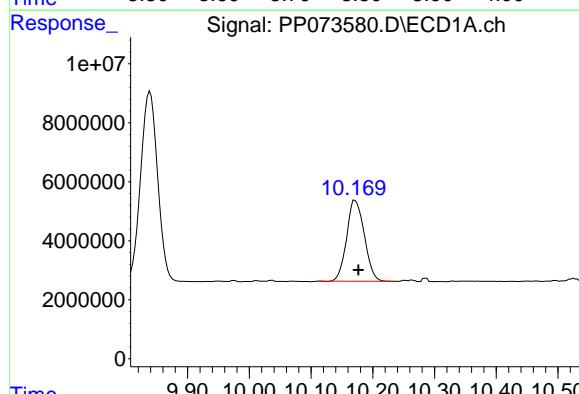


#2 Decachlorobiphenyl

R.T.: 10.171 min
Delta R.T.: -0.005 min
Response: 54731552
Conc: 26.61 ng/ml

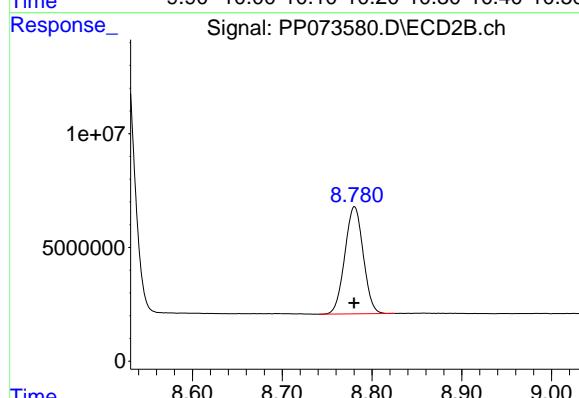

#2 Decachlorobiphenyl


R.T.: 8.781 min
Delta R.T.: 0.000 min
Response: 67087696
Conc: 26.46 ng/ml

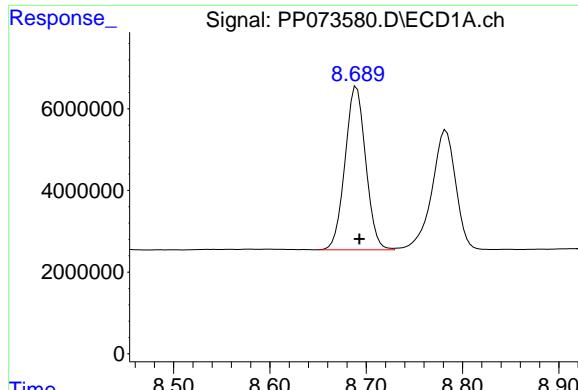

#41 AR-1268-1


R.T.: 8.690 min
Delta R.T.: -0.003 min
Response: 59422367
Conc: 260.53 ng/ml

Instrument: ECD_P
ClientSampleId: AR1268ICC250

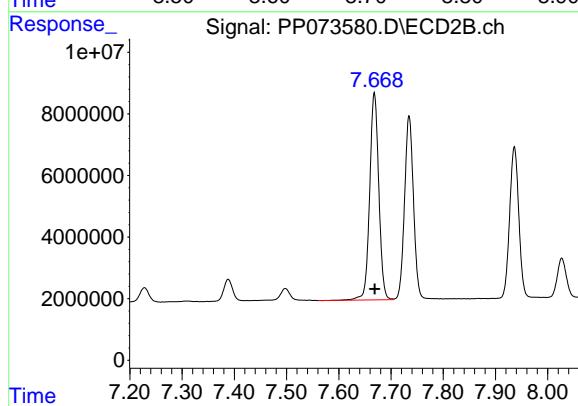


#41 AR-1268-1

R.T.: 7.668 min
Delta R.T.: 0.000 min
Response: 81364216
Conc: 264.35 ng/ml

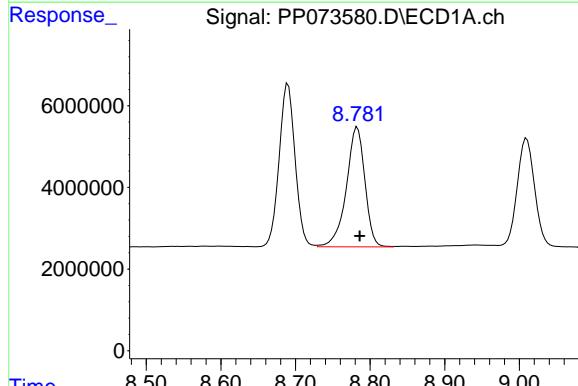


#42 AR-1268-2

R.T.: 8.783 min
Delta R.T.: -0.003 min
Response: 50730840
Conc: 261.19 ng/ml

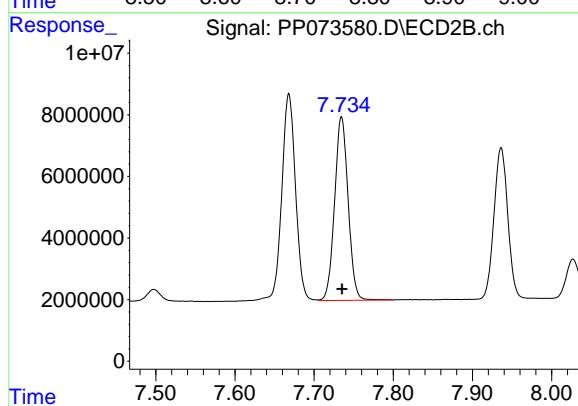

#42 AR-1268-2


R.T.: 7.735 min
Delta R.T.: 0.000 min
Response: 70740492
Conc: 264.38 ng/ml

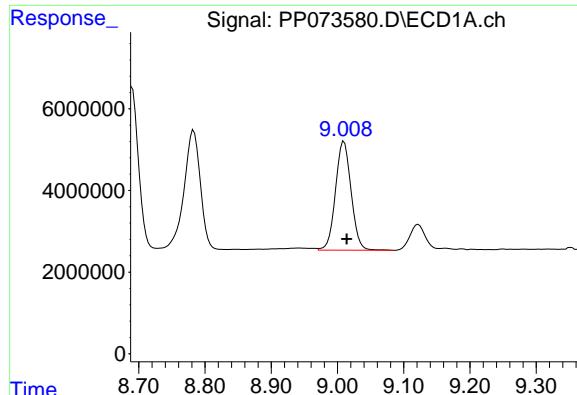

#43 AR-1268-3


R.T.: 9.010 min
 Delta R.T.: -0.004 min
 Response: 43805027
 Conc: 262.76 ng/ml

Instrument: ECD_P
 ClientSampleId: AR1268ICC250

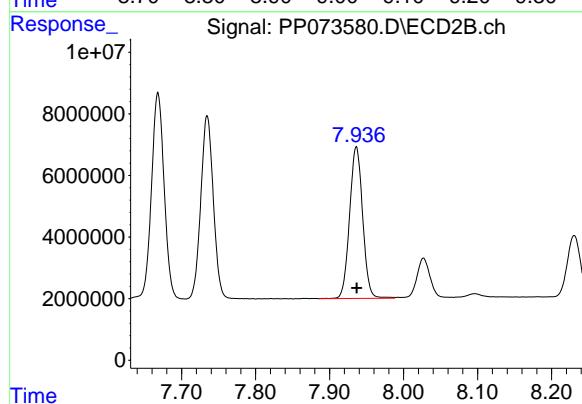


#43 AR-1268-3

R.T.: 7.936 min
 Delta R.T.: 0.000 min
 Response: 60554343
 Conc: 266.40 ng/ml

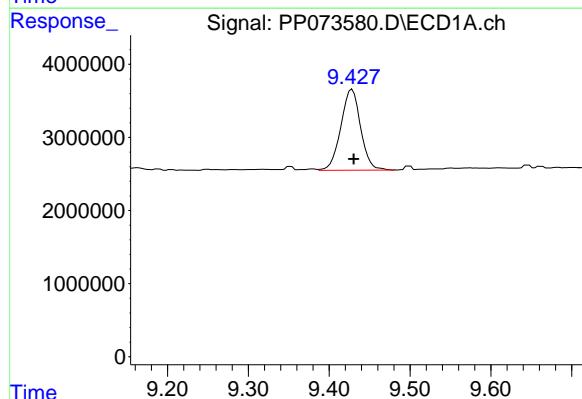


#44 AR-1268-4

R.T.: 9.428 min
 Delta R.T.: -0.002 min
 Response: 18771767
 Conc: 269.87 ng/ml

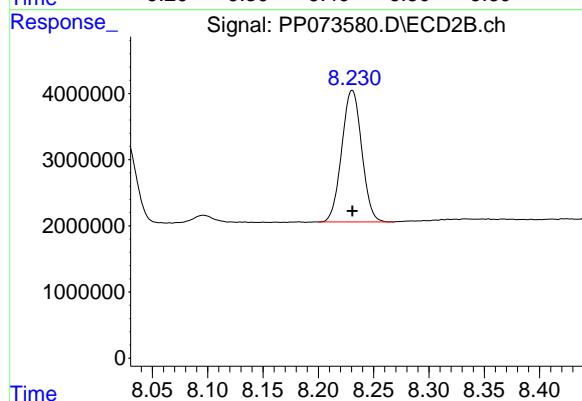

#44 AR-1268-4

R.T.: 8.231 min
 Delta R.T.: 0.000 min
 Response: 24970476
 Conc: 262.24 ng/ml

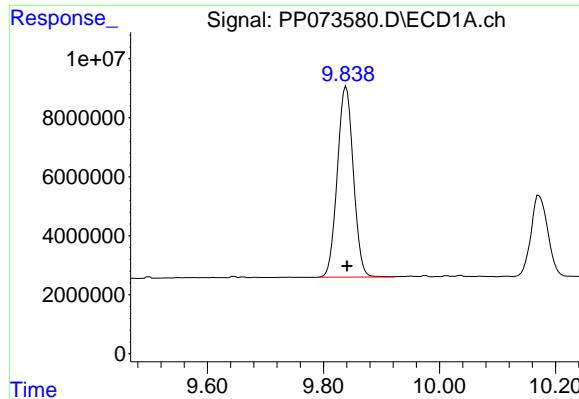

#45 AR-1268-5


R.T.: 9.839 min
Delta R.T.: -0.002 min
Response: 124334254
Conc: 256.28 ng/ml

Instrument:

ECD_P

ClientSampleId:

AR1268ICC250

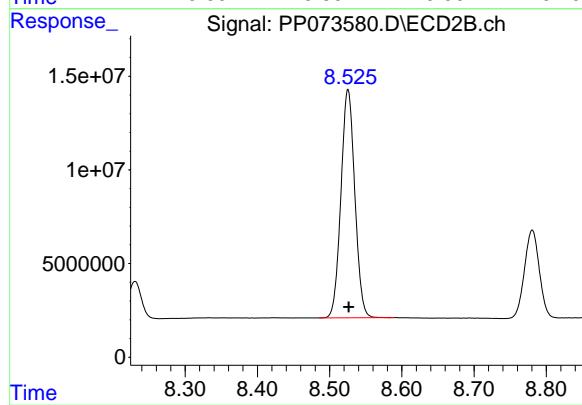

#45 AR-1268-5

R.T.: 8.525 min
Delta R.T.: -0.001 min
Response: 162694547
Conc: 261.38 ng/ml

1
2
3
4
5
6
7
8
9
10
11
12
13
14
15
16
17
18
19
20

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP070825\
 Data File : PP073581.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jul 2025 04:24
 Operator : YP\AJ
 Sample : AR1268ICC050
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
AR1268ICC050

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 08 04:52:34 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 08 04:46:40 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	4.489	3.778	6570480	8954068	4.649	4.604
2) SA Decachlor...	10.178	8.780	8974224	11778445	4.354	4.632

Target Compounds

41) L9 AR-1268-1	8.694	7.668	10231981	15365679	44.903	49.987
42) L9 AR-1268-2	8.787	7.735	8726381	12801300	44.866	47.748
43) L9 AR-1268-3	9.015	7.936	8012537	11044482	48.006	48.707
44) L9 AR-1268-4	9.433	8.231	3216586	4250036	45.402	44.756
45) L9 AR-1268-5	9.841	8.526	6017980	28831591	12.454	46.018 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP070825\
 Data File : PP073581.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jul 2025 04:24
 Operator : YP\AJ
 Sample : AR1268ICC050
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
AR1268ICC050

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 08 04:52:34 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 08 04:46:40 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

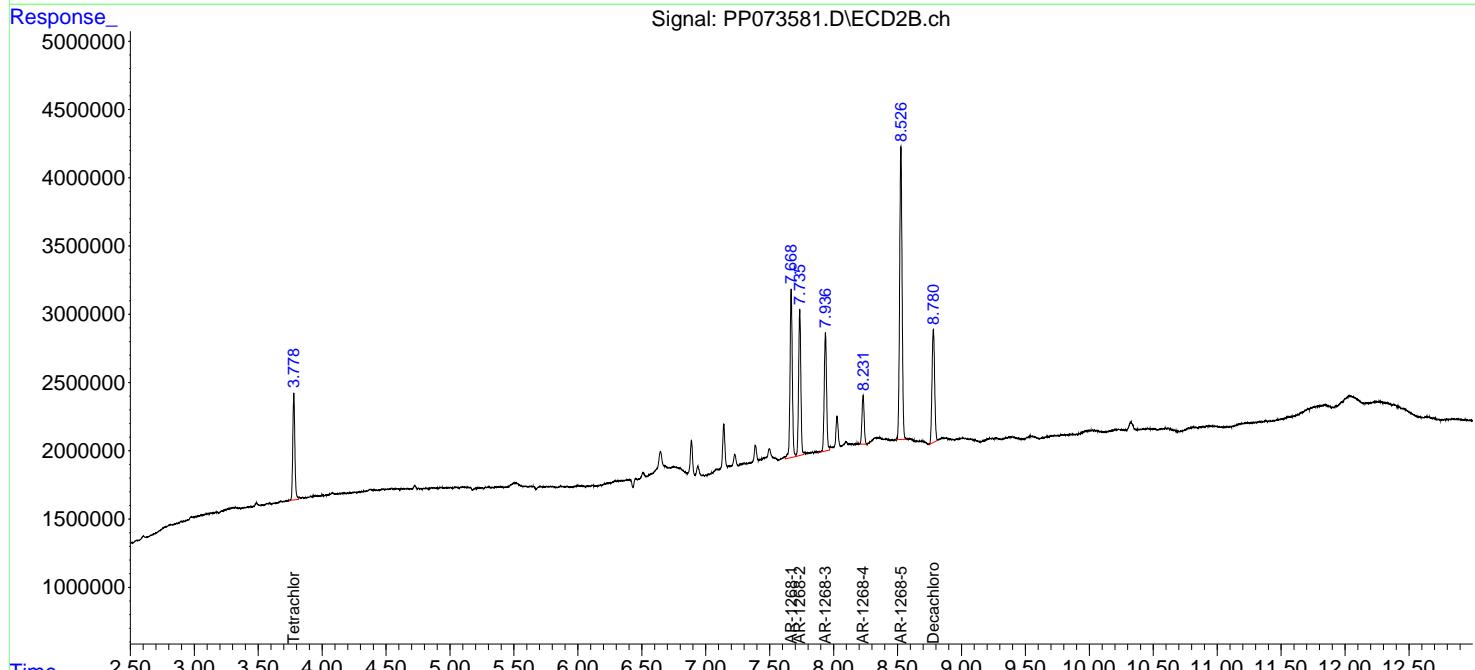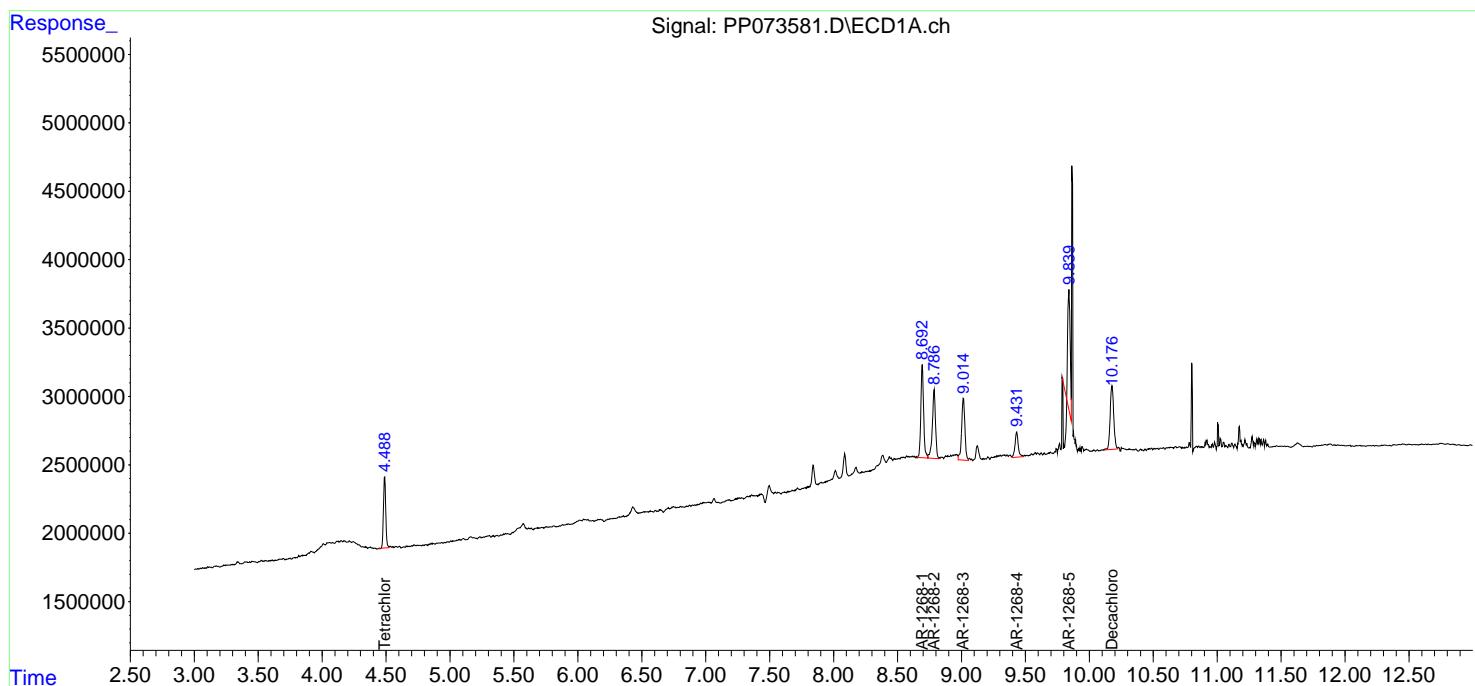



#1 Tetrachloro-m-xylene


R.T.: 4.489 min
Delta R.T.: 0.000 min
Response: 6570480
Conc: 4.65 ng/ml

Instrument:

ECD_P


ClientSampleId :

AR1268ICC050

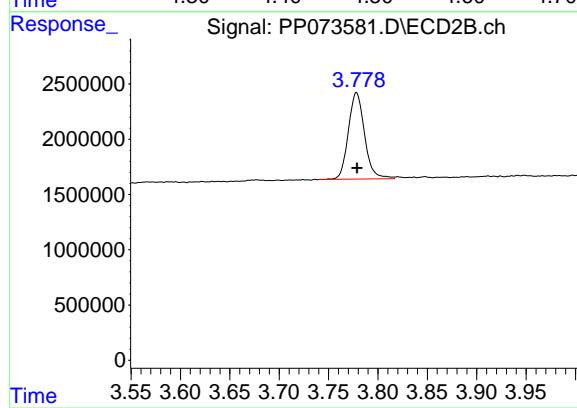


#1 Tetrachloro-m-xylene

R.T.: 3.778 min
Delta R.T.: 0.000 min
Response: 8954068
Conc: 4.60 ng/ml




#2 Decachlorobiphenyl

R.T.: 10.178 min
Delta R.T.: 0.001 min
Response: 8974224
Conc: 4.35 ng/ml

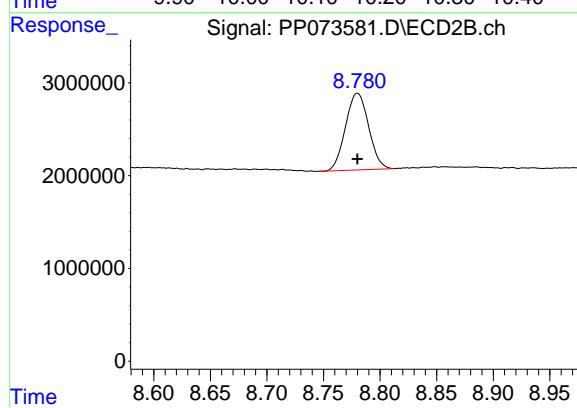

#2 Decachlorobiphenyl


R.T.: 8.780 min
Delta R.T.: 0.000 min
Response: 11778445
Conc: 4.63 ng/ml

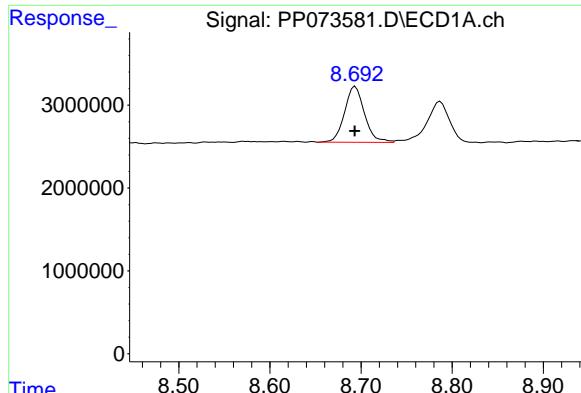

#41 AR-1268-1


R.T.: 8.694 min
Delta R.T.: 0.000 min
Response: 10231981
Conc: 44.90 ng/ml

Instrument: ECD_P
ClientSampleId: AR1268ICC050

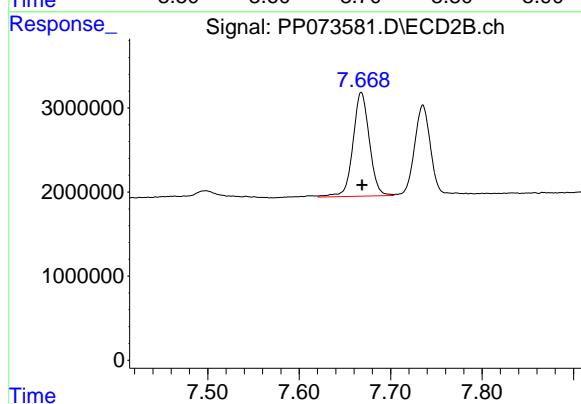


#41 AR-1268-1

R.T.: 7.668 min
Delta R.T.: 0.000 min
Response: 15365679
Conc: 49.99 ng/ml




#42 AR-1268-2

R.T.: 8.787 min
Delta R.T.: 0.000 min
Response: 8726381
Conc: 44.87 ng/ml

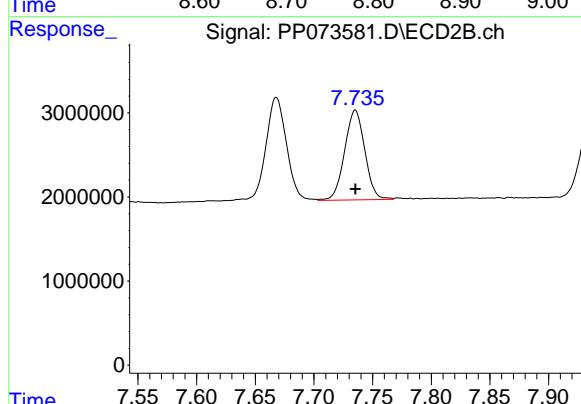

#42 AR-1268-2

R.T.: 7.735 min
Delta R.T.: 0.000 min
Response: 12801300
Conc: 47.75 ng/ml

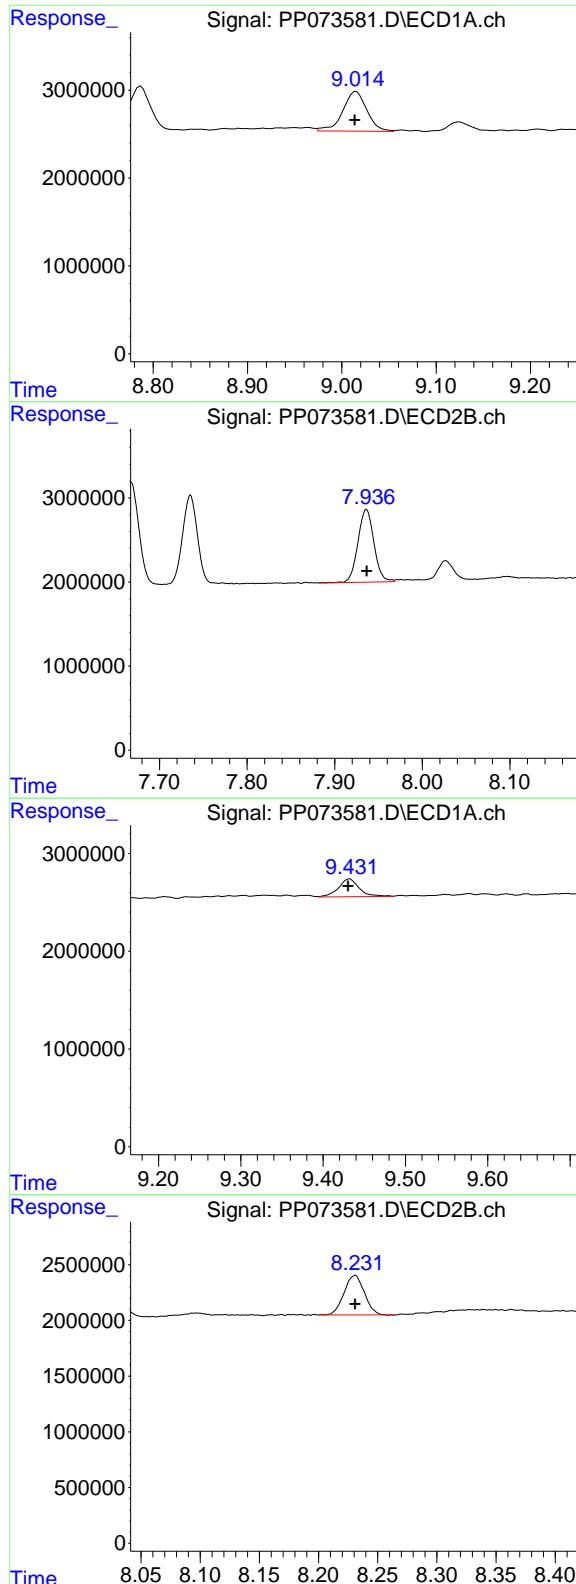

#43 AR-1268-3

R.T.: 9.015 min
 Delta R.T.: 0.002 min
 Response: 8012537
 Conc: 48.01 ng/ml

Instrument: ECD_P
 ClientSampleId: AR1268ICC050

#43 AR-1268-3


R.T.: 7.936 min
 Delta R.T.: 0.000 min
 Response: 11044482
 Conc: 48.71 ng/ml

#44 AR-1268-4

R.T.: 9.433 min
 Delta R.T.: 0.003 min
 Response: 3216586
 Conc: 45.40 ng/ml

#44 AR-1268-4


R.T.: 8.231 min
 Delta R.T.: 0.000 min
 Response: 4250036
 Conc: 44.76 ng/ml

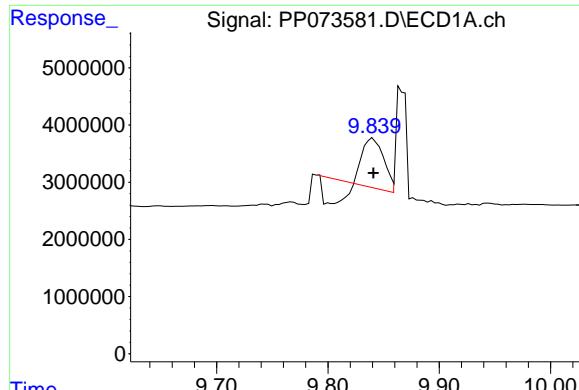

#45 AR-1268-5

R.T.: 9.841 min
Delta R.T.: 0.000 min
Response: 6017980
Conc: 12.45 ng/ml

Instrument: ECD_P
ClientSampleId: AR1268ICC050

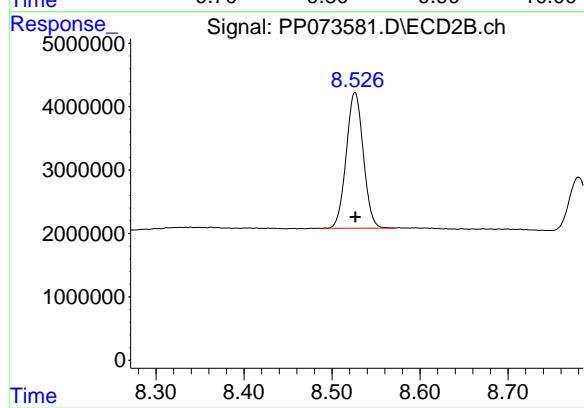

#45 AR-1268-5

R.T.: 8.526 min
Delta R.T.: 0.000 min
Response: 28831591
Conc: 46.02 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP072125\
 Data File : PP073984.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jul 2025 13:40
 Operator : YP\AJ
 Sample : Q2635-01MS
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
RT2286MS

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 22 01:50:37 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 08 08:35:32 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	4.481	3.773	23650205	32913477	17.269	17.866
2) SA Decachlor...	10.168	8.770	19654459	26316757	18.014	19.889

Target Compounds

3) L1 AR-1016-1	5.633	4.849	18863800	29465448	397.019	432.205
4) L1 AR-1016-2	5.654	4.867	29837172	43500761	418.974	426.962
5) L1 AR-1016-3	5.716	5.043	18207530	24326097	417.001	449.598
6) L1 AR-1016-4	5.813	5.085	16224197	19663890	451.354	448.120
7) L1 AR-1016-5	6.107	5.298	17720270	24867794	565.593	455.600
8) L2 AR-1221-1	4.680	3.980	2047139	3518450	114.580	130.096
9) L2 AR-1221-2	4.769	4.068	2580436	4761204	191.080	233.847
10) L2 AR-1221-3	4.844	4.142	11299312	16319425	271.587	265.578
11) L3 AR-1232-1	4.844	4.142	11299312	16319425	346.066	350.094
12) L3 AR-1232-2	5.368	4.867	17207807	43500761	1058.637	912.735
13) L3 AR-1232-3	5.654	5.043	29837172	24326097	904.336	971.915
14) L3 AR-1232-4	5.813	5.127	16224197	22558031	986.564	1041.639
15) L3 AR-1232-5	5.904	5.298	11990321	24867794	1134.334	1102.127
16) L4 AR-1242-1	5.633	4.849	18863800	29465448	493.969	510.094
17) L4 AR-1242-2	5.654	4.867	29837172	43500761	498.266	503.165
18) L4 AR-1242-3	5.716	5.043	18207530	24326097	497.189	529.442
19) L4 AR-1242-4	5.813	5.127	16224197	22558031	504.860	509.633
20) L4 AR-1242-5	6.543	5.649	5443873	24531218	166.292	444.065 #
21) L5 AR-1248-1	5.633	4.849	18863800	29465448	611.062	656.321
22) L5 AR-1248-2	5.904	5.085	11990321	19663890	300.334	319.548
23) L5 AR-1248-3	6.107	5.127	17720270	22558031	399.019	352.114
24) L5 AR-1248-4	6.480	5.298	18595954	24867794	337.614	329.910
25) L5 AR-1248-5	6.543	5.689	5443873	6016352	101.205	80.658
26) L6 AR-1254-1	6.480	5.649	18595954	24531218	347.007	211.421 #
27) L6 AR-1254-2	6.695	5.796	17350776	23885552	208.320	237.375
28) L6 AR-1254-3	7.060	6.212	10719877	44314410	121.359	286.924 #
29) L6 AR-1254-4	7.341	6.425	8914494	6462960	113.319	68.348 #
30) L6 AR-1254-5	7.756	6.842	53170622	71346544	721.644	534.652 #
31) L7 AR-1260-1	7.222	6.328	34694505	55075376	588.429	564.527
32) L7 AR-1260-2	7.476	6.517	49718794	66621540	518.769	542.355
33) L7 AR-1260-3	7.834	6.668	37706644	60304176	516.030	550.905
34) L7 AR-1260-4	8.058	7.137	36868595	47082456	564.604	526.600
35) L7 AR-1260-5	8.375	7.380	80346257	117.2E6	532.614	521.396
36) L8 AR-1262-1	8.058	6.879	36868595	52862605	423.644	357.925
37) L8 AR-1262-2	8.375	7.137	80346257	47082456	405.733	368.324
38) L8 AR-1262-3	8.697	7.659	47764045	26973034	379.909	236.566 #
39) L8 AR-1262-4	8.758	7.724	28415445	77752202	304.682	422.454 #
40) L8 AR-1262-5	9.422	8.222	19854543	25455071	313.216	301.473
41) L9 AR-1268-1	8.697	7.659	47764045	26973034	213.974	87.752 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP072125\
 Data File : PP073984.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jul 2025 13:40
 Operator : YP\AJ
 Sample : Q2635-01MS
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
RT2286MS

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 22 01:50:37 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 08 08:35:32 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9 AR-1268-2	8.758	7.724	28415445	77752202	149.158	292.645 #
43) L9 AR-1268-3	9.006	7.927	1539585	2942539	9.298	13.044 #
44) L9 AR-1268-4	9.422	8.222	19854543	25455071	285.497	273.805
45) L9 AR-1268-5	9.833	8.516	5638616	8000594	12.232	12.976



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP072125\
 Data File : PP073984.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jul 2025 13:40
 Operator : YP\AJ
 Sample : Q2635-01MS
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 RT2286MS

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 22 01:50:37 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 08 08:35:32 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

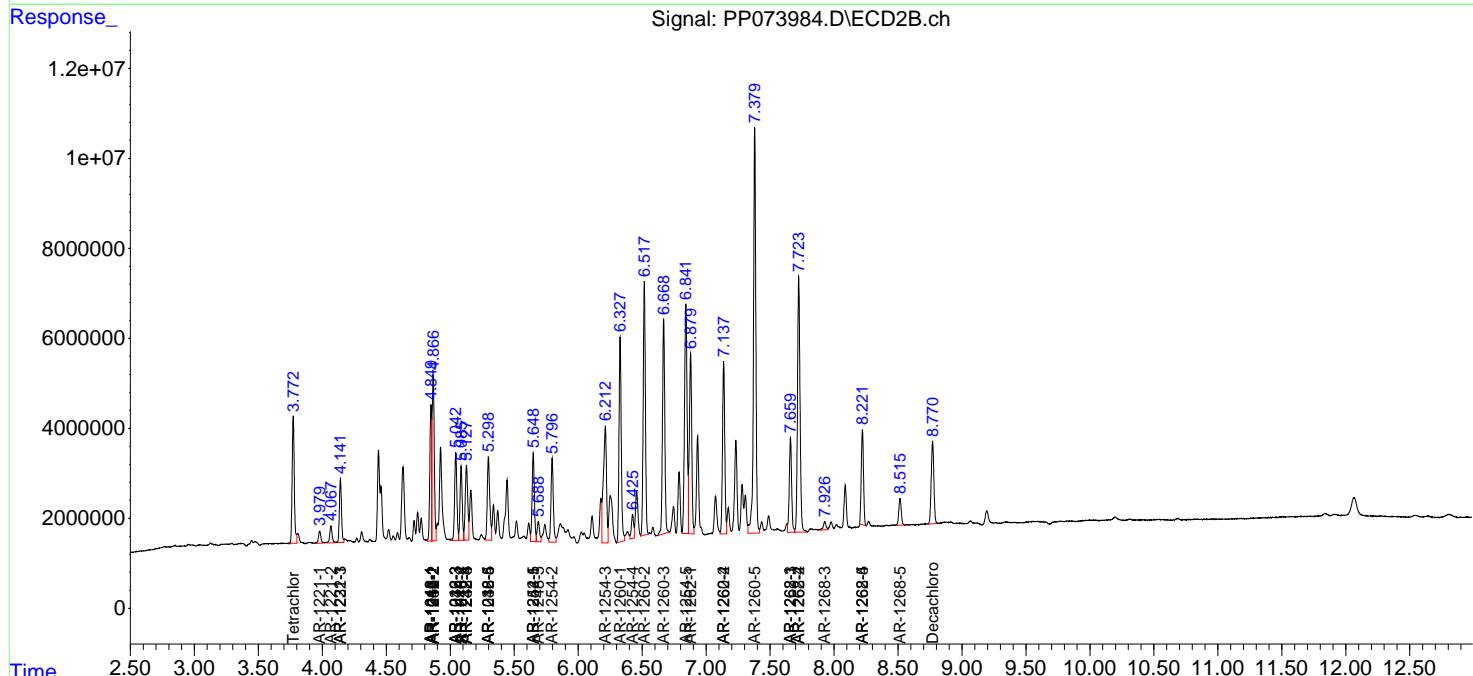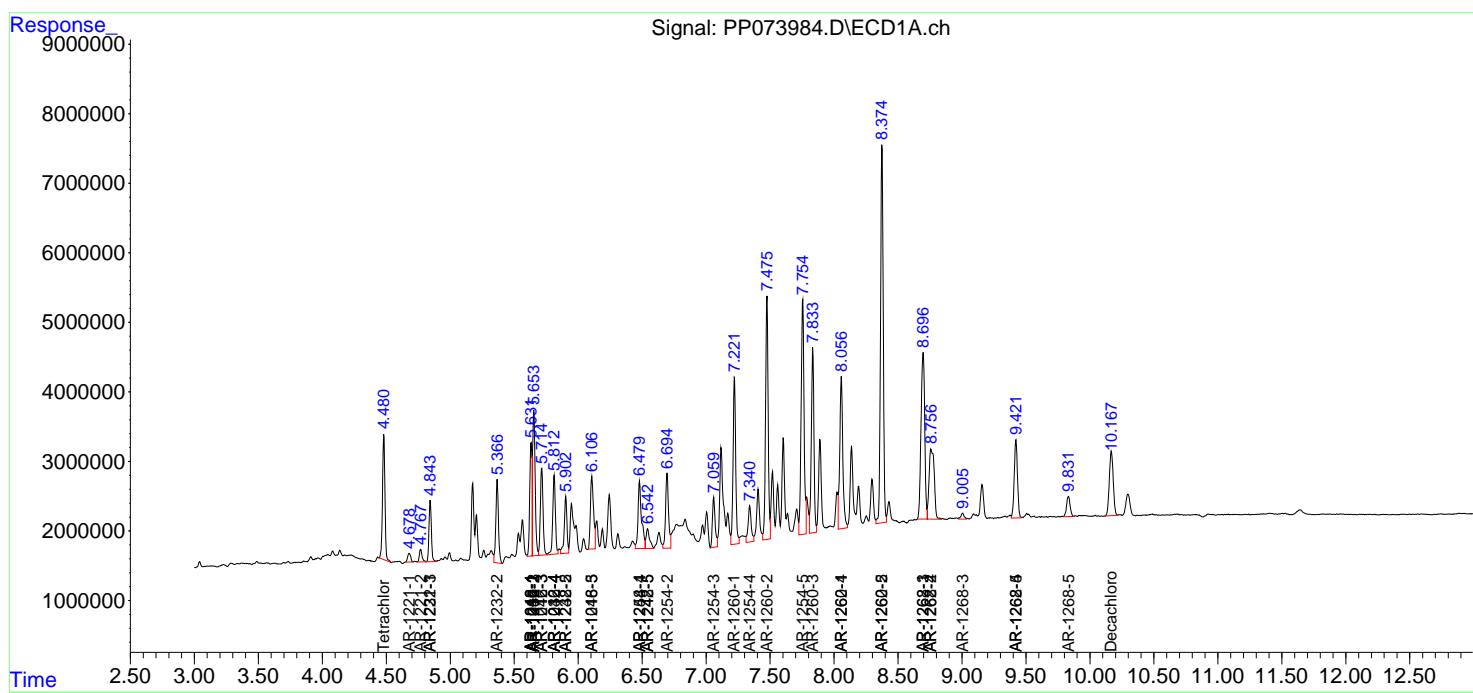

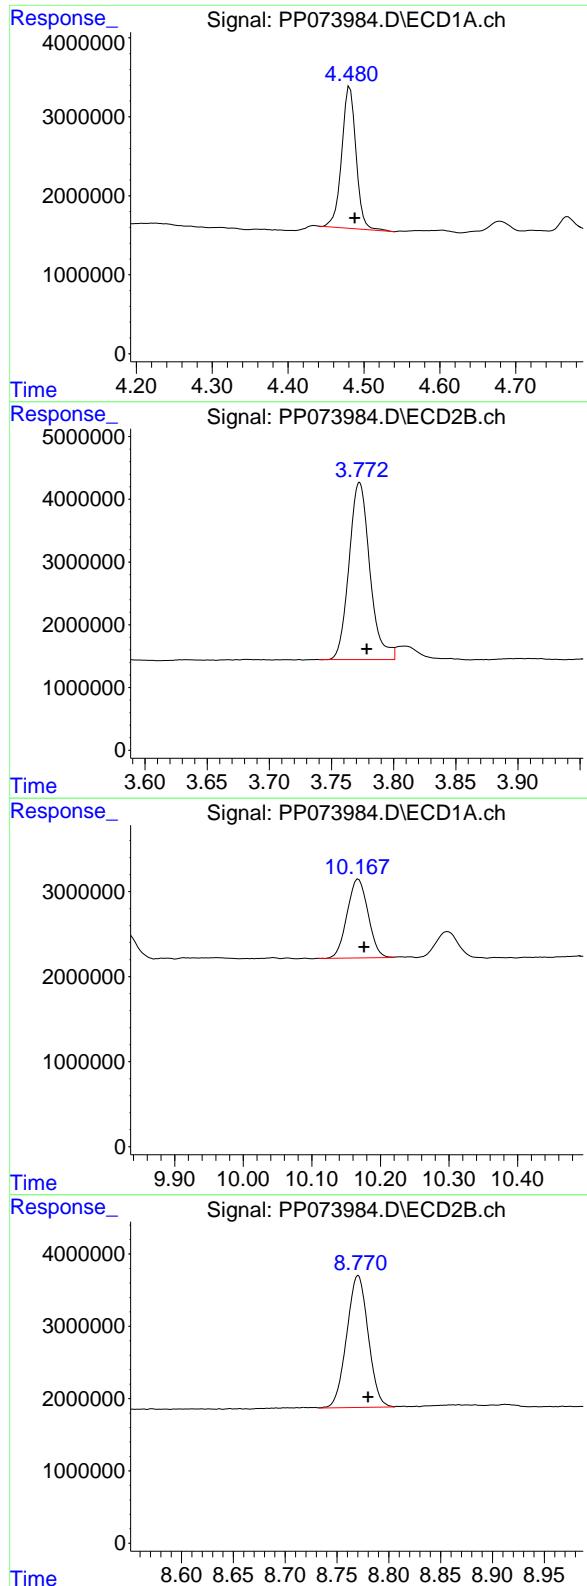

#1 Tetrachloro-m-xylene

R.T.: 4.481 min
 Delta R.T.: -0.007 min
 Response: 23650205
 Conc: 17.27 ng/ml

Instrument:

ECD_P

ClientSampleId :
 RT2286MS

#1 Tetrachloro-m-xylene


R.T.: 3.773 min
 Delta R.T.: -0.006 min
 Response: 32913477
 Conc: 17.87 ng/ml

#2 Decachlorobiphenyl

R.T.: 10.168 min
 Delta R.T.: -0.008 min
 Response: 19654459
 Conc: 18.01 ng/ml

#2 Decachlorobiphenyl


R.T.: 8.770 min
 Delta R.T.: -0.010 min
 Response: 26316757
 Conc: 19.89 ng/ml

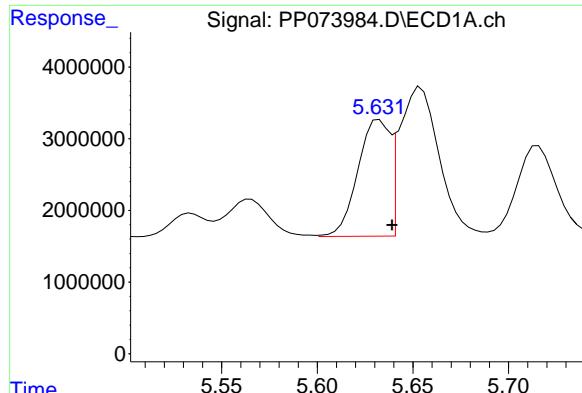

#3 AR-1016-1


R.T.: 5.633 min
 Delta R.T.: -0.006 min
 Response: 18863800
 Conc: 397.02 ng/ml

Instrument: ECD_P
 ClientSampleId: RT2286MS

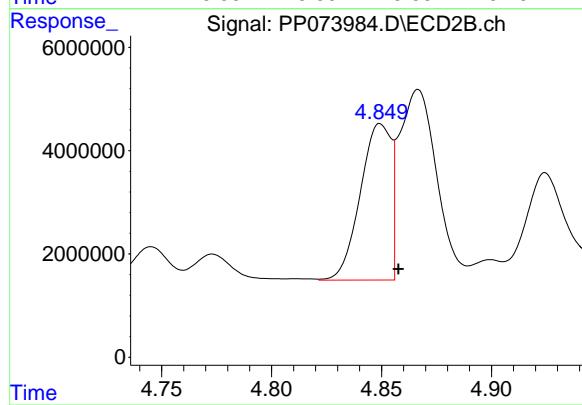


#3 AR-1016-1

R.T.: 4.849 min
 Delta R.T.: -0.008 min
 Response: 29465448
 Conc: 432.20 ng/ml

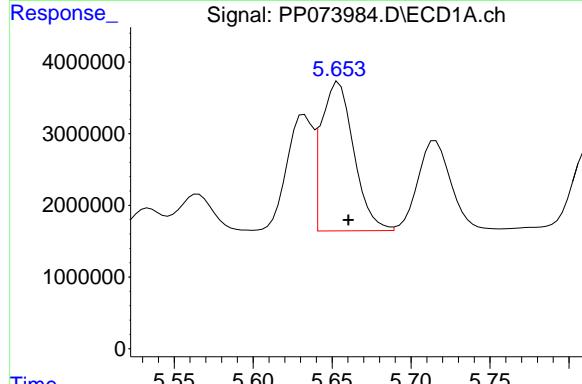


#4 AR-1016-2

R.T.: 5.654 min
 Delta R.T.: -0.006 min
 Response: 29837172
 Conc: 418.97 ng/ml

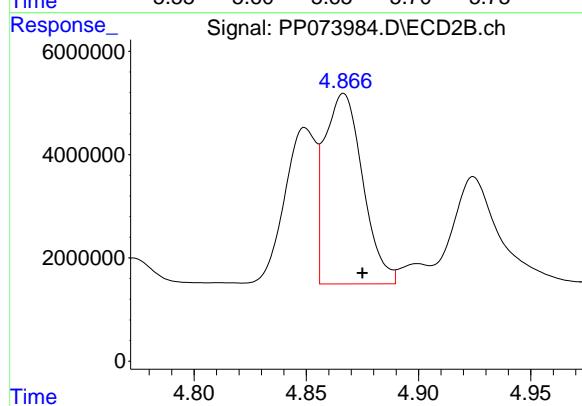

#4 AR-1016-2


R.T.: 4.867 min
 Delta R.T.: -0.008 min
 Response: 43500761
 Conc: 426.96 ng/ml

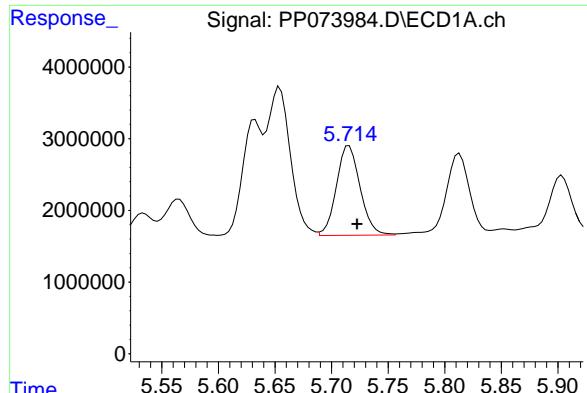

#5 AR-1016-3


R.T.: 5.716 min
 Delta R.T.: -0.007 min
 Response: 18207530
 Conc: 417.00 ng/ml

Instrument: ECD_P
 ClientSampleId: RT2286MS

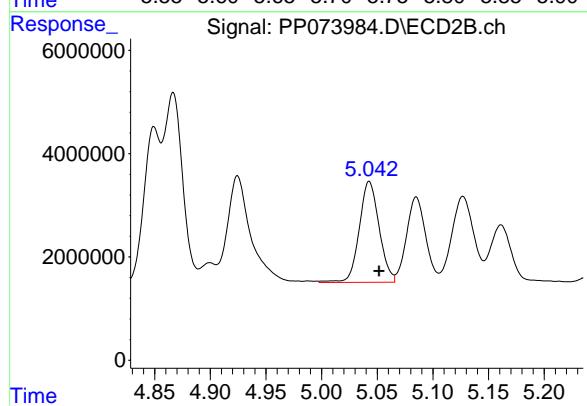


#5 AR-1016-3

R.T.: 5.043 min
 Delta R.T.: -0.009 min
 Response: 24326097
 Conc: 449.60 ng/ml

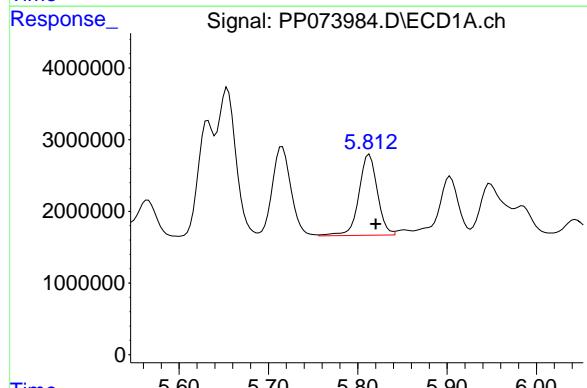


#6 AR-1016-4

R.T.: 5.813 min
 Delta R.T.: -0.007 min
 Response: 16224197
 Conc: 451.35 ng/ml

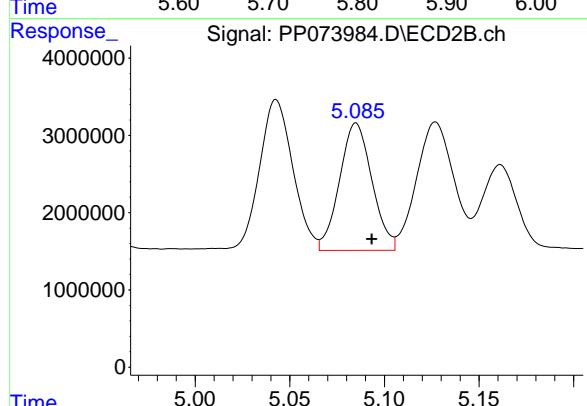

#6 AR-1016-4

R.T.: 5.085 min
 Delta R.T.: -0.008 min
 Response: 19663890
 Conc: 448.12 ng/ml

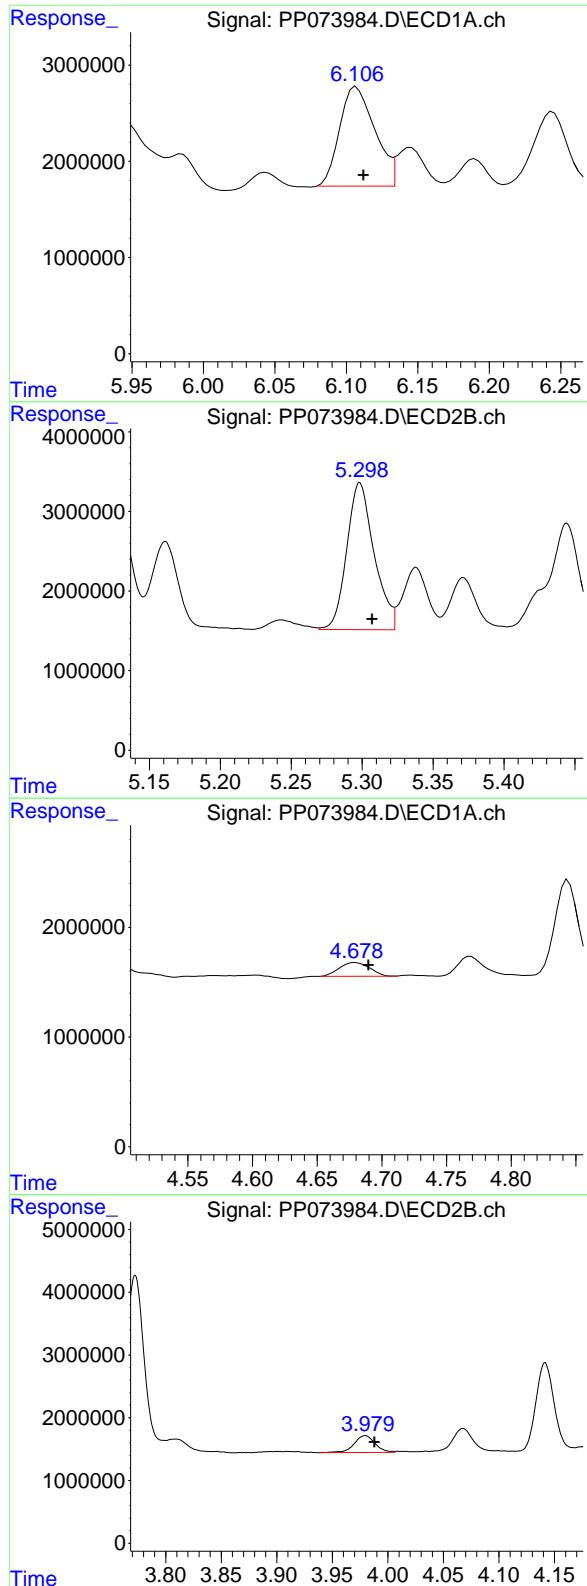

#7 AR-1016-5

R.T.: 6.107 min
 Delta R.T.: -0.005 min
 Response: 17720270
 Conc: 565.59 ng/ml

Instrument: ECD_P
 ClientSampleId: RT2286MS

#7 AR-1016-5


R.T.: 5.298 min
 Delta R.T.: -0.009 min
 Response: 24867794
 Conc: 455.60 ng/ml

#8 AR-1221-1

R.T.: 4.680 min
 Delta R.T.: -0.010 min
 Response: 2047139
 Conc: 114.58 ng/ml

#8 AR-1221-1


R.T.: 3.980 min
 Delta R.T.: -0.008 min
 Response: 3518450
 Conc: 130.10 ng/ml

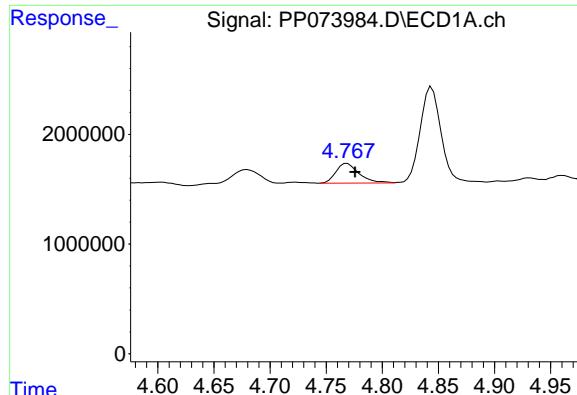

#9 AR-1221-2


R.T.: 4.769 min
Delta R.T.: -0.007 min
Response: 2580436
Conc: 191.08 ng/ml

Instrument: ECD_P
ClientSampleId: RT2286MS

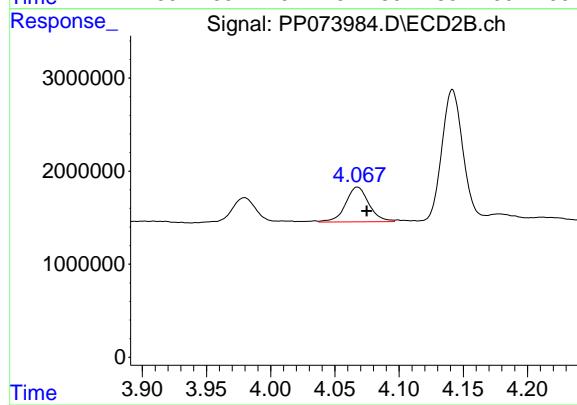


#9 AR-1221-2

R.T.: 4.068 min
Delta R.T.: -0.007 min
Response: 4761204
Conc: 233.85 ng/ml




#10 AR-1221-3

R.T.: 4.844 min
Delta R.T.: -0.007 min
Response: 11299312
Conc: 271.59 ng/ml

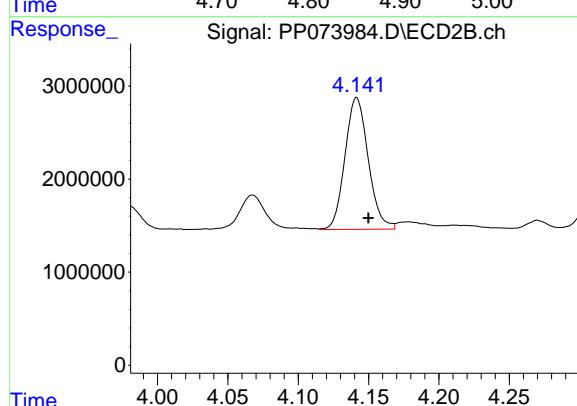

#10 AR-1221-3

R.T.: 4.142 min
Delta R.T.: -0.008 min
Response: 16319425
Conc: 265.58 ng/ml

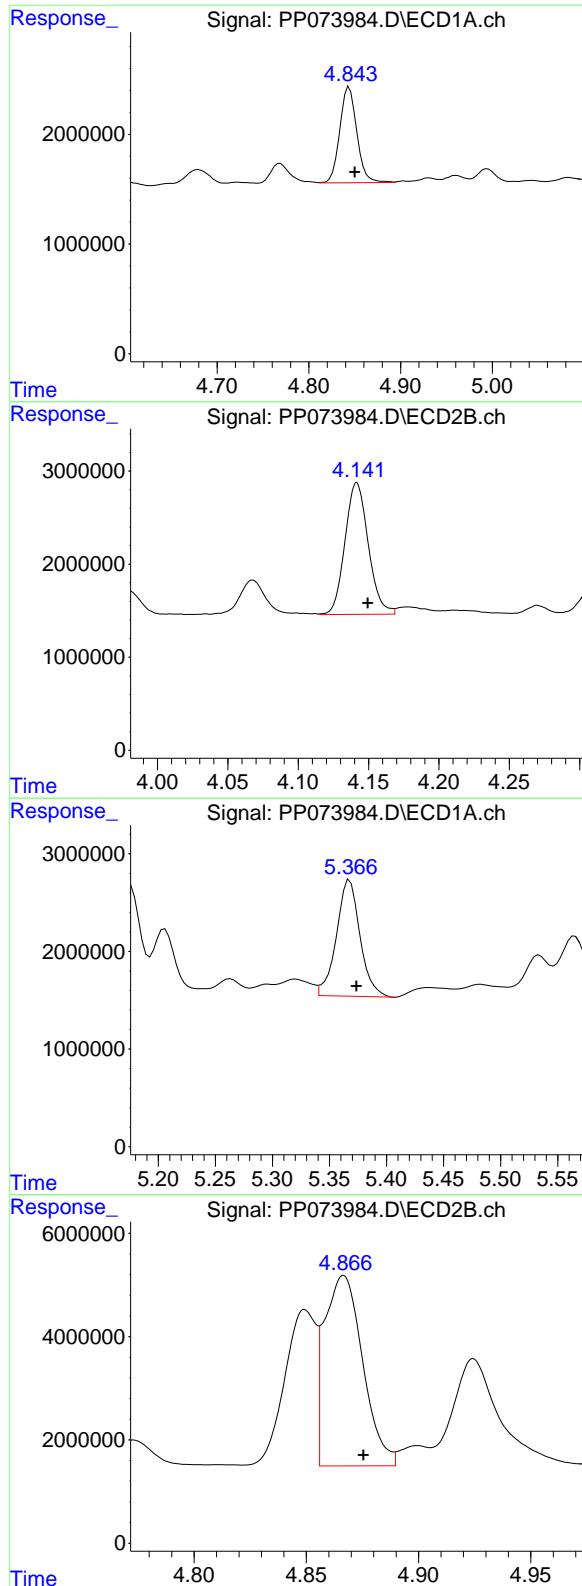

#11 AR-1232-1

R.T.: 4.844 min
 Delta R.T.: -0.006 min
 Response: 11299312
 Conc: 346.07 ng/ml

Instrument: ECD_P
 ClientSampleId: RT2286MS

#11 AR-1232-1


R.T.: 4.142 min
 Delta R.T.: -0.008 min
 Response: 16319425
 Conc: 350.09 ng/ml

#12 AR-1232-2

R.T.: 5.368 min
 Delta R.T.: -0.006 min
 Response: 17207807
 Conc: 1058.64 ng/ml

#12 AR-1232-2


R.T.: 4.867 min
 Delta R.T.: -0.009 min
 Response: 43500761
 Conc: 912.73 ng/ml

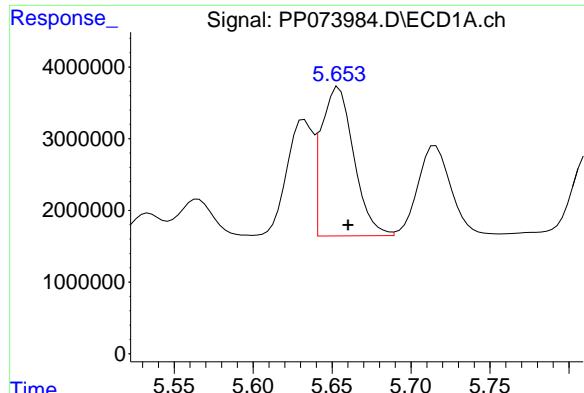

#13 AR-1232-3


R.T.: 5.654 min
 Delta R.T.: -0.006 min
 Response: 29837172
 Conc: 904.34 ng/ml

Instrument: ECD_P
 ClientSampleId: RT2286MS

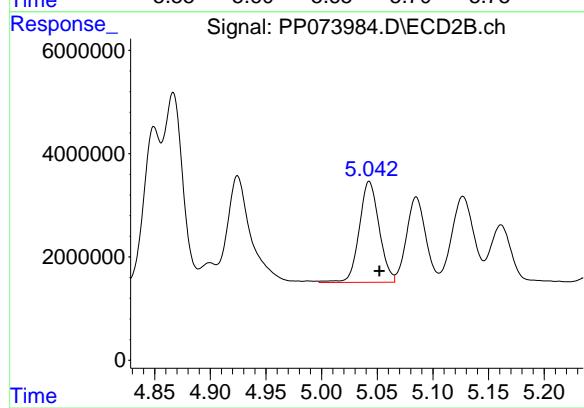


#13 AR-1232-3

R.T.: 5.043 min
 Delta R.T.: -0.009 min
 Response: 24326097
 Conc: 971.92 ng/ml

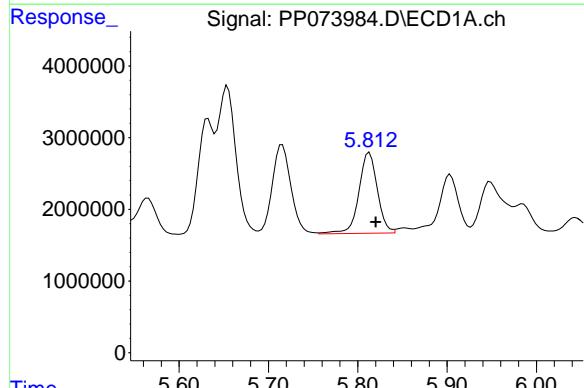


#14 AR-1232-4

R.T.: 5.813 min
 Delta R.T.: -0.007 min
 Response: 16224197
 Conc: 986.56 ng/ml

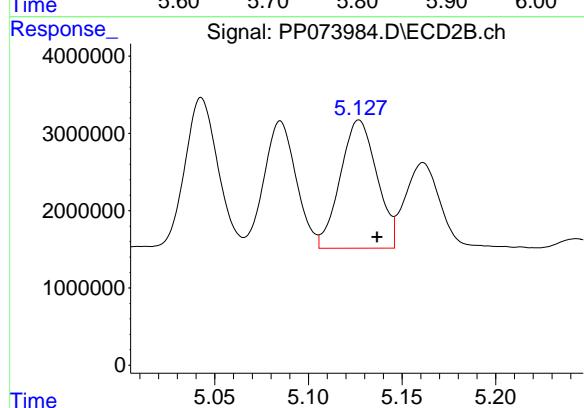

#14 AR-1232-4

R.T.: 5.127 min
 Delta R.T.: -0.010 min
 Response: 22558031
 Conc: 1041.64 ng/ml

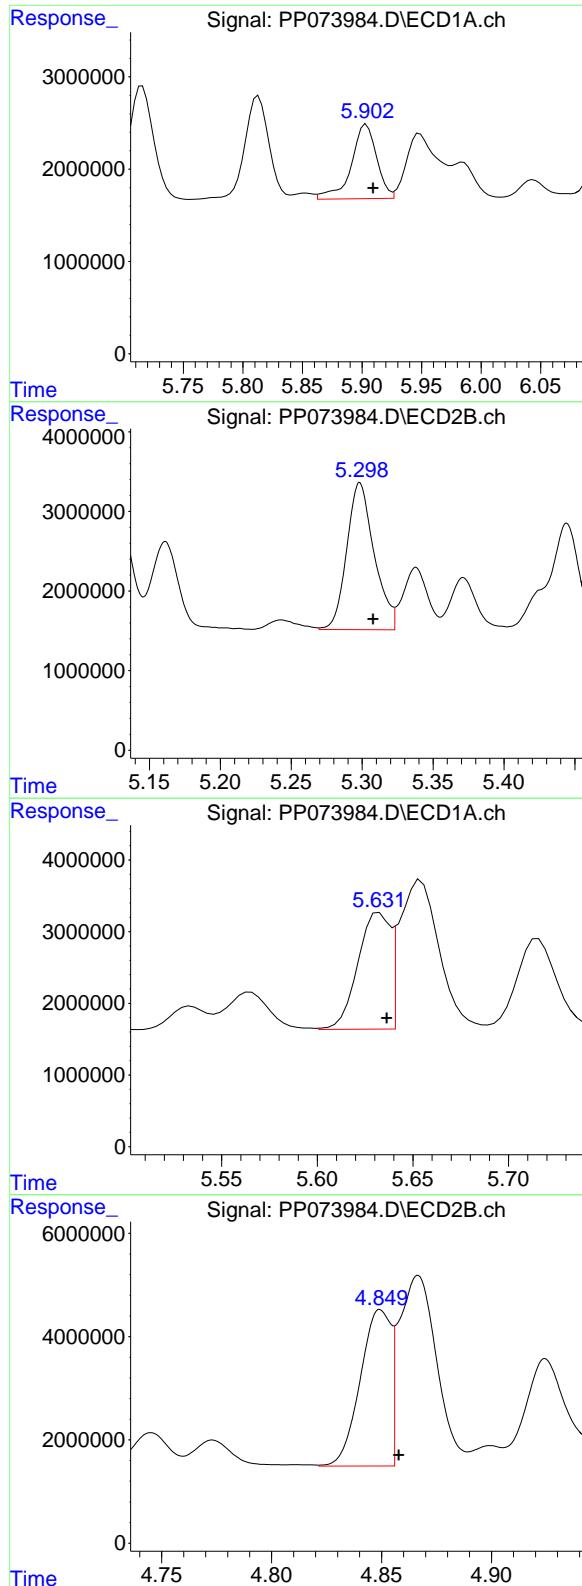

#15 AR-1232-5

R.T.: 5.904 min
 Delta R.T.: -0.006 min
 Response: 11990321
 Conc: 1134.33 ng/ml

Instrument: ECD_P
 ClientSampleId: RT2286MS

#15 AR-1232-5


R.T.: 5.298 min
 Delta R.T.: -0.009 min
 Response: 24867794
 Conc: 1102.13 ng/ml

#16 AR-1242-1

R.T.: 5.633 min
 Delta R.T.: -0.004 min
 Response: 18863800
 Conc: 493.97 ng/ml

#16 AR-1242-1

R.T.: 4.849 min
 Delta R.T.: -0.008 min
 Response: 29465448
 Conc: 510.09 ng/ml

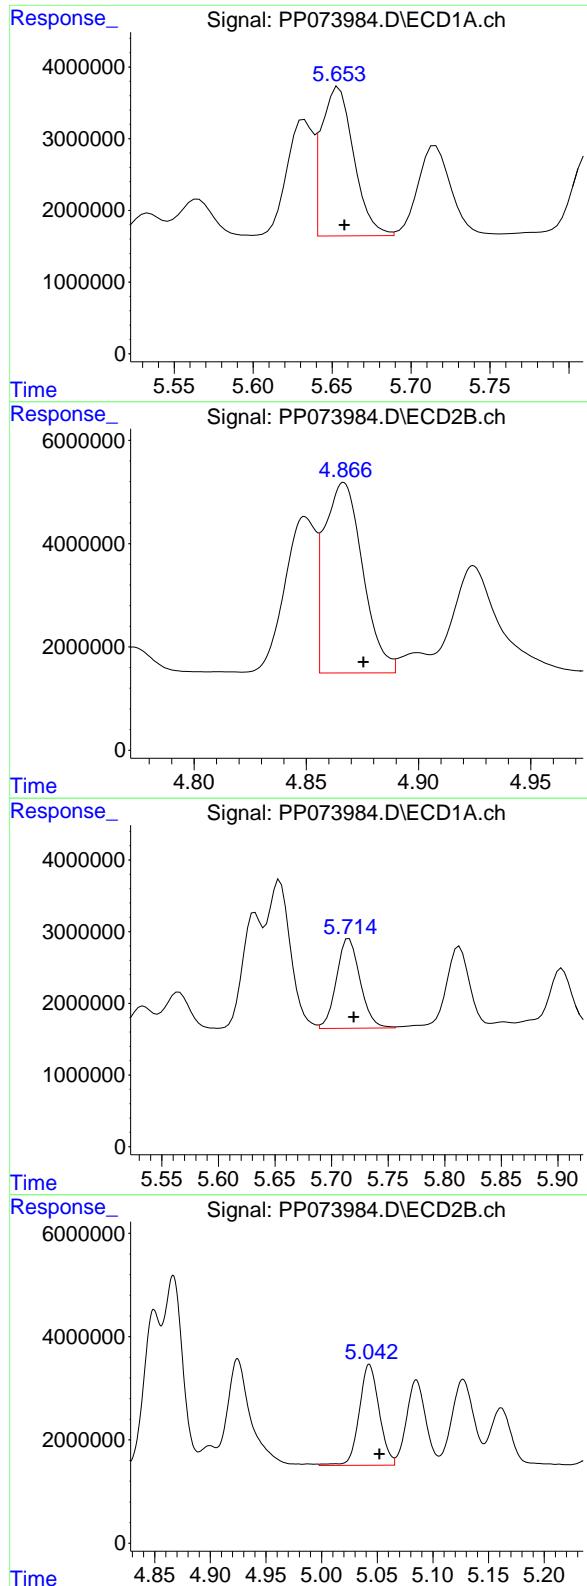

#17 AR-1242-2

R.T.: 5.654 min
 Delta R.T.: -0.003 min
 Response: 29837172
 Conc: 498.27 ng/ml

Instrument: ECD_P
 ClientSampleId: RT2286MS

#17 AR-1242-2


R.T.: 4.867 min
 Delta R.T.: -0.009 min
 Response: 43500761
 Conc: 503.17 ng/ml

#18 AR-1242-3

R.T.: 5.716 min
 Delta R.T.: -0.004 min
 Response: 18207530
 Conc: 497.19 ng/ml

#18 AR-1242-3


R.T.: 5.043 min
 Delta R.T.: -0.009 min
 Response: 24326097
 Conc: 529.44 ng/ml

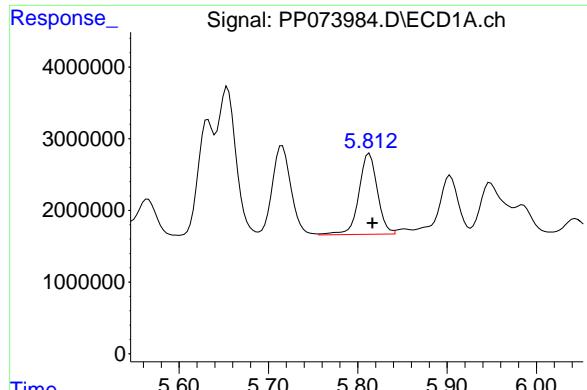

#19 AR-1242-4


R.T.: 5.813 min
 Delta R.T.: -0.004 min
 Response: 16224197
 Conc: 504.86 ng/ml

Instrument: ECD_P
 ClientSampleId: RT2286MS

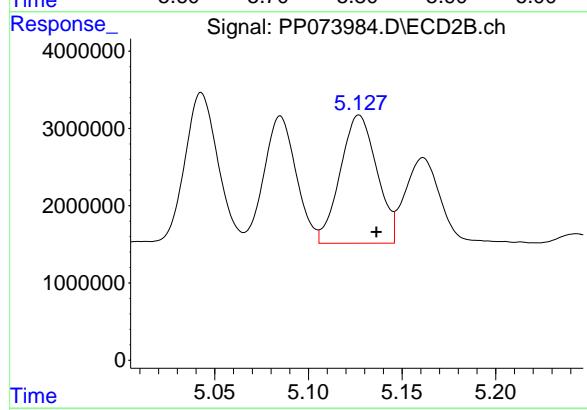


#19 AR-1242-4

R.T.: 5.127 min
 Delta R.T.: -0.009 min
 Response: 22558031
 Conc: 509.63 ng/ml

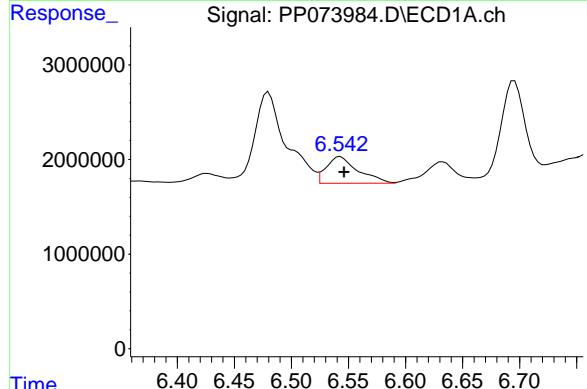


#20 AR-1242-5

R.T.: 6.543 min
 Delta R.T.: -0.003 min
 Response: 5443873
 Conc: 166.29 ng/ml

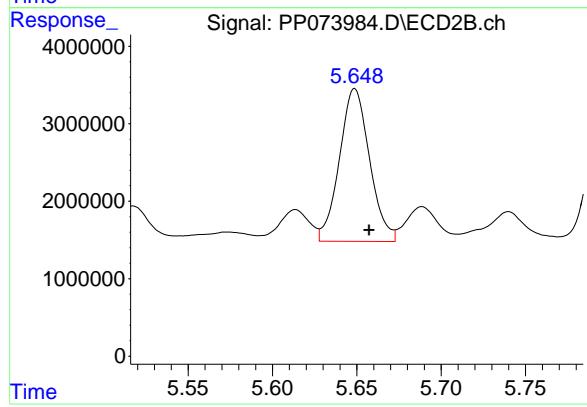

#20 AR-1242-5


R.T.: 5.649 min
 Delta R.T.: -0.008 min
 Response: 24531218
 Conc: 444.06 ng/ml

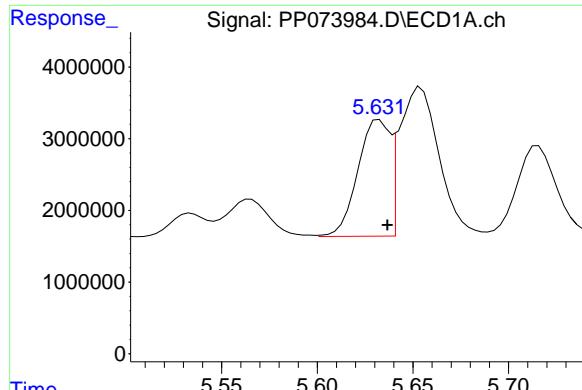

#21 AR-1248-1


R.T.: 5.633 min
 Delta R.T.: -0.004 min
 Response: 18863800
 Conc: 611.06 ng/ml

Instrument: ECD_P
 ClientSampleId: RT2286MS

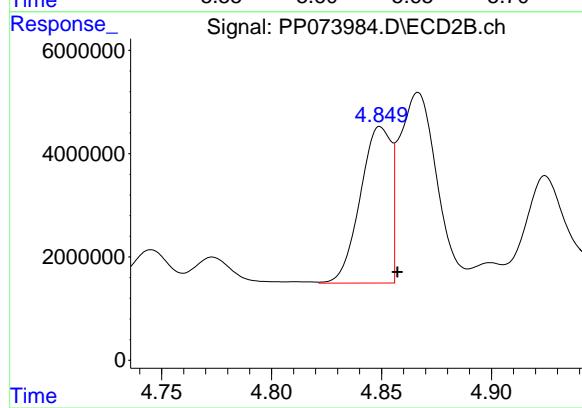


#21 AR-1248-1

R.T.: 4.849 min
 Delta R.T.: -0.008 min
 Response: 29465448
 Conc: 656.32 ng/ml

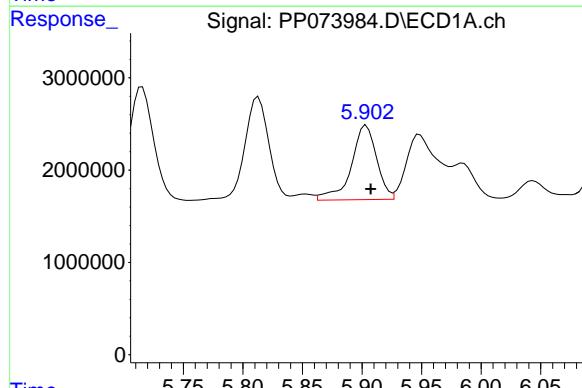


#22 AR-1248-2

R.T.: 5.904 min
 Delta R.T.: -0.004 min
 Response: 11990321
 Conc: 300.33 ng/ml

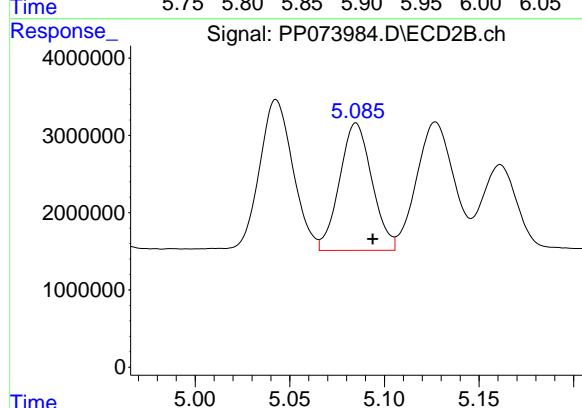

#22 AR-1248-2


R.T.: 5.085 min
 Delta R.T.: -0.009 min
 Response: 19663890
 Conc: 319.55 ng/ml

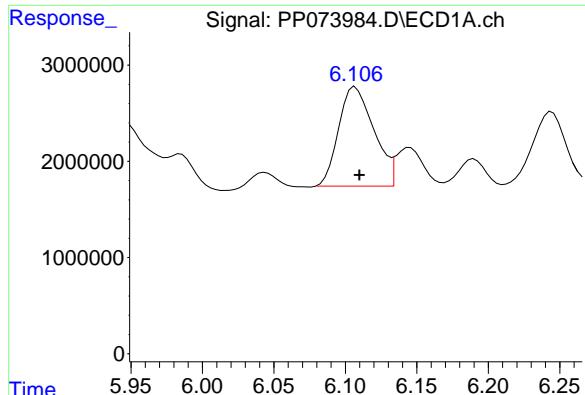

#23 AR-1248-3


R.T.: 6.107 min
 Delta R.T.: -0.003 min
 Response: 17720270
 Conc: 399.02 ng/ml

Instrument: ECD_P
 ClientSampleId: RT2286MS

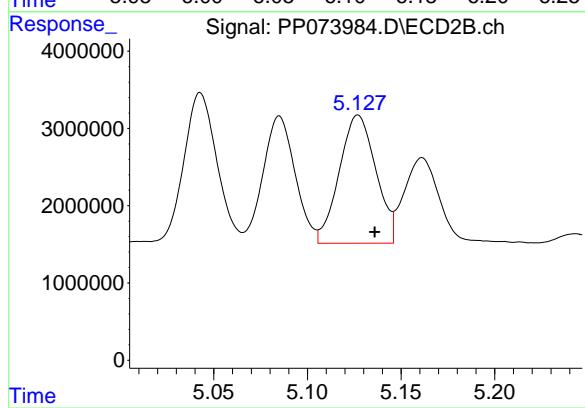


#23 AR-1248-3

R.T.: 5.127 min
 Delta R.T.: -0.009 min
 Response: 22558031
 Conc: 352.11 ng/ml

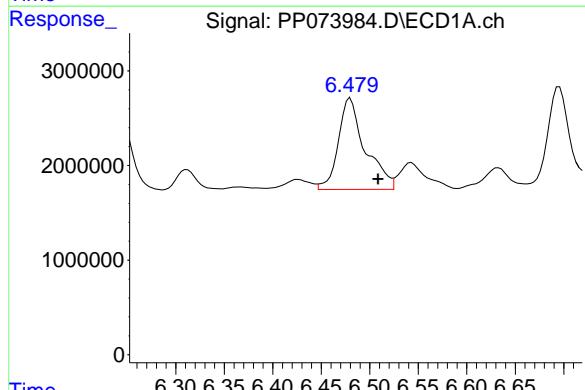


#24 AR-1248-4

R.T.: 6.480 min
 Delta R.T.: -0.029 min
 Response: 18595954
 Conc: 337.61 ng/ml

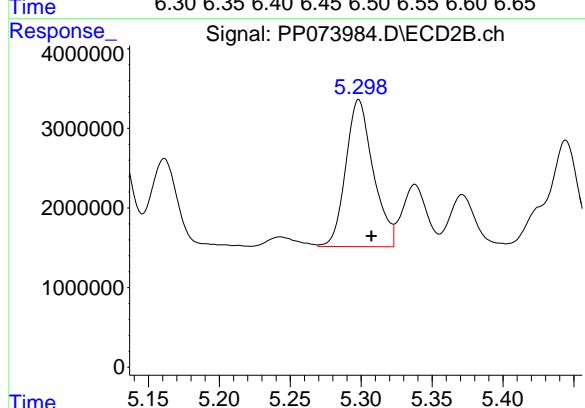

#24 AR-1248-4


R.T.: 5.298 min
 Delta R.T.: -0.009 min
 Response: 24867794
 Conc: 329.91 ng/ml

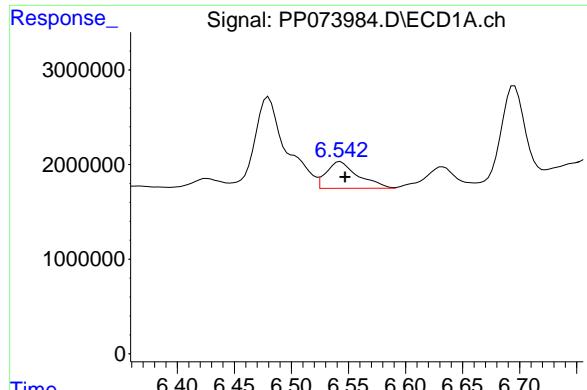

#25 AR-1248-5


R.T.: 6.543 min
 Delta R.T.: -0.004 min
 Response: 5443873
 Conc: 101.20 ng/ml

Instrument: ECD_P
 ClientSampleId: RT2286MS

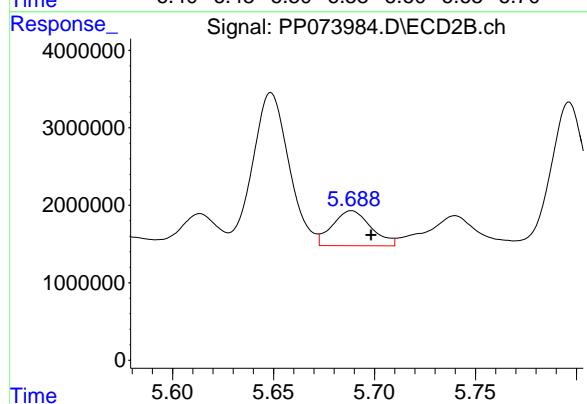


#25 AR-1248-5

R.T.: 5.689 min
 Delta R.T.: -0.010 min
 Response: 6016352
 Conc: 80.66 ng/ml

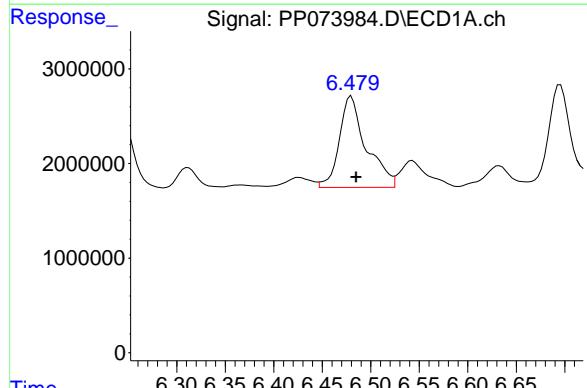


#26 AR-1254-1

R.T.: 6.480 min
 Delta R.T.: -0.005 min
 Response: 18595954
 Conc: 347.01 ng/ml

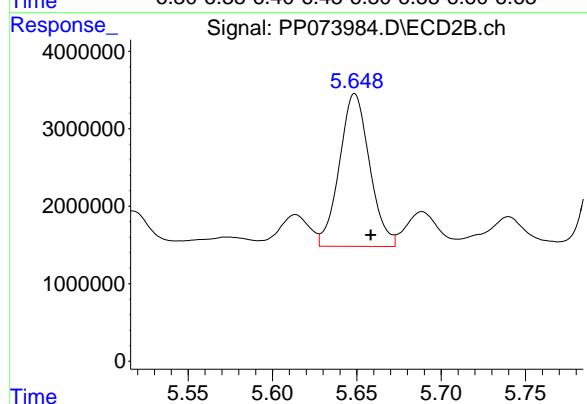

#26 AR-1254-1


R.T.: 5.649 min
 Delta R.T.: -0.009 min
 Response: 24531218
 Conc: 211.42 ng/ml

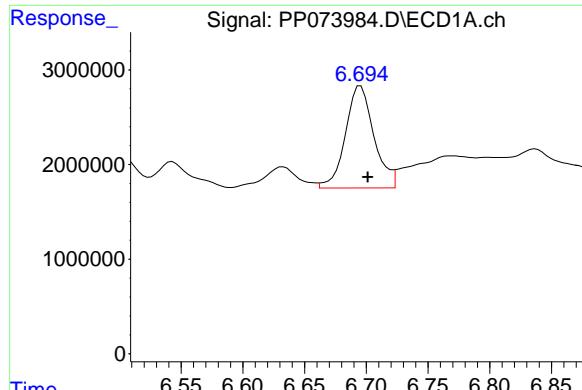

#27 AR-1254-2


R.T.: 6.695 min
 Delta R.T.: -0.006 min
 Response: 17350776
 Conc: 208.32 ng/ml

Instrument: ECD_P
 ClientSampleId: RT2286MS

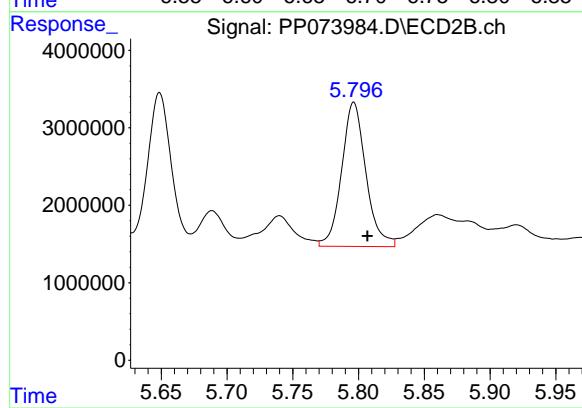


#27 AR-1254-2

R.T.: 5.796 min
 Delta R.T.: -0.010 min
 Response: 23885552
 Conc: 237.38 ng/ml

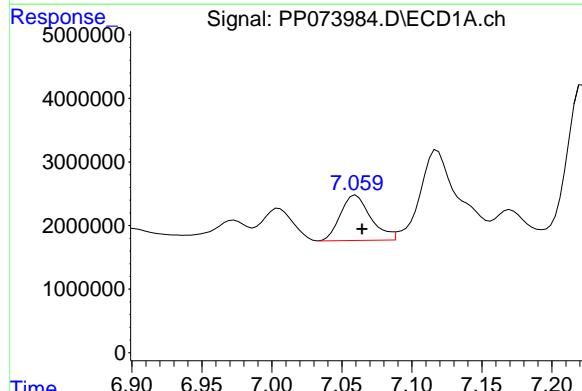


#28 AR-1254-3

R.T.: 7.060 min
 Delta R.T.: -0.004 min
 Response: 10719877
 Conc: 121.36 ng/ml

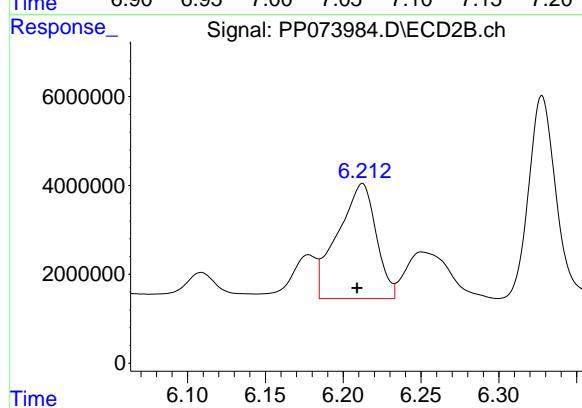

#28 AR-1254-3


R.T.: 6.212 min
 Delta R.T.: 0.003 min
 Response: 44314410
 Conc: 286.92 ng/ml

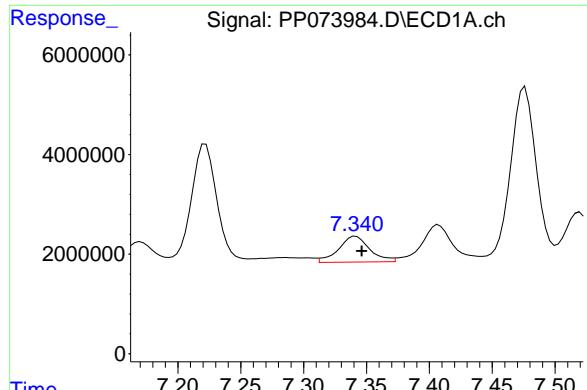

#29 AR-1254-4


R.T.: 7.341 min
 Delta R.T.: -0.005 min
 Response: 8914494
 Conc: 113.32 ng/ml

Instrument: ECD_P
 ClientSampleId: RT2286MS

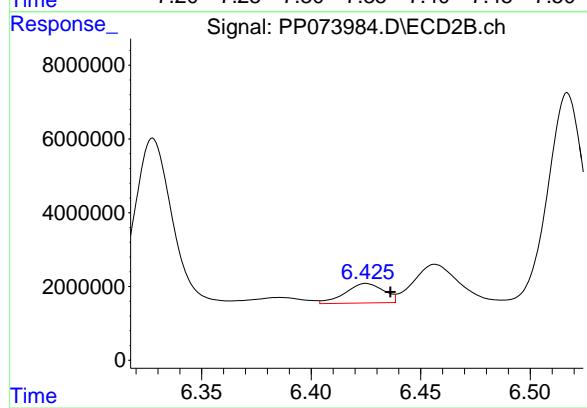


#29 AR-1254-4

R.T.: 6.425 min
 Delta R.T.: -0.011 min
 Response: 6462960
 Conc: 68.35 ng/ml

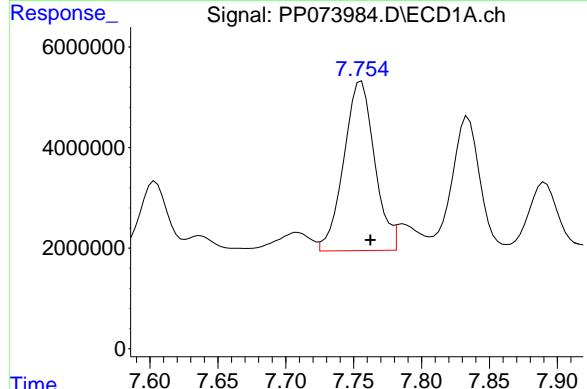


#30 AR-1254-5

R.T.: 7.756 min
 Delta R.T.: -0.007 min
 Response: 53170622
 Conc: 721.64 ng/ml

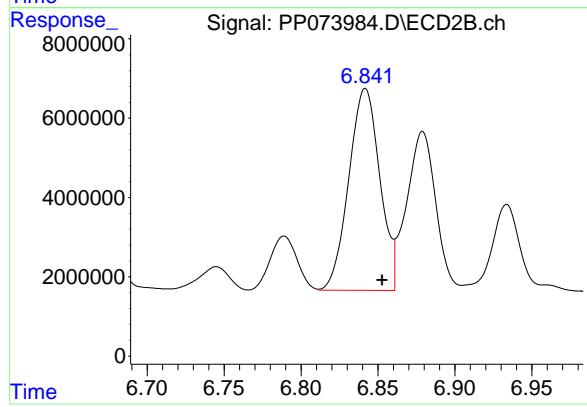

#30 AR-1254-5

R.T.: 6.842 min
 Delta R.T.: -0.011 min
 Response: 71346544
 Conc: 534.65 ng/ml

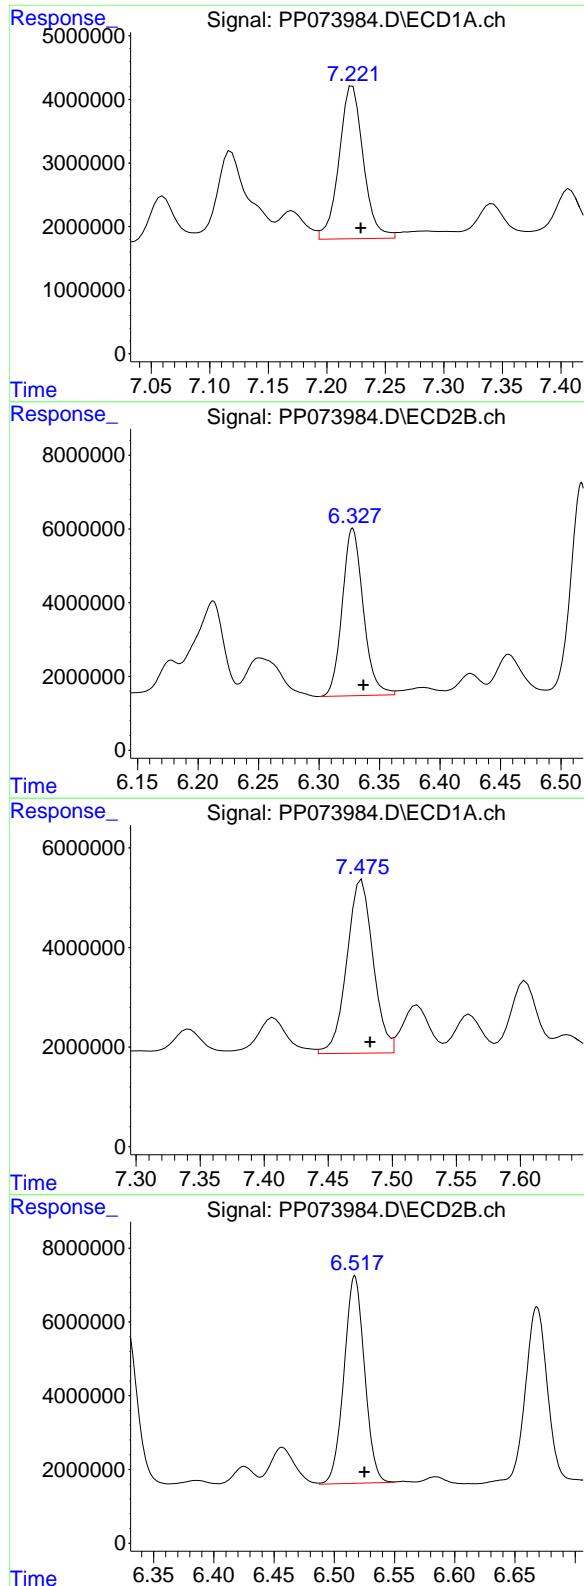

#31 AR-1260-1

R.T.: 7.222 min
 Delta R.T.: -0.007 min
 Response: 34694505
 Conc: 588.43 ng/ml

Instrument: ECD_P
 ClientSampleId: RT2286MS

#31 AR-1260-1


R.T.: 6.328 min
 Delta R.T.: -0.009 min
 Response: 55075376
 Conc: 564.53 ng/ml

#32 AR-1260-2

R.T.: 7.476 min
 Delta R.T.: -0.007 min
 Response: 49718794
 Conc: 518.77 ng/ml

#32 AR-1260-2

R.T.: 6.517 min
 Delta R.T.: -0.008 min
 Response: 66621540
 Conc: 542.35 ng/ml

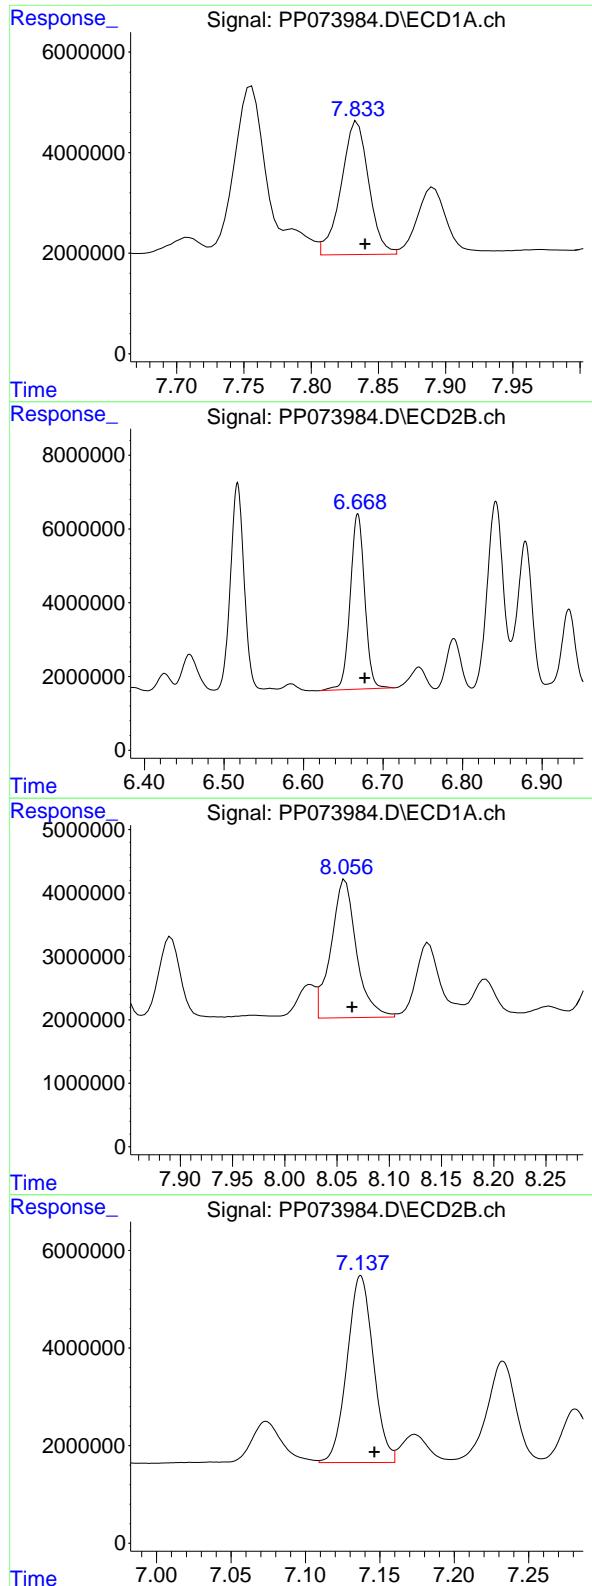

#33 AR-1260-3

R.T.: 7.834 min
 Delta R.T.: -0.006 min
 Response: 37706644
 Conc: 516.03 ng/ml

Instrument: ECD_P
 ClientSampleId: RT2286MS

#33 AR-1260-3


R.T.: 6.668 min
 Delta R.T.: -0.009 min
 Response: 60304176
 Conc: 550.91 ng/ml

#34 AR-1260-4

R.T.: 8.058 min
 Delta R.T.: -0.007 min
 Response: 36868595
 Conc: 564.60 ng/ml

#34 AR-1260-4

R.T.: 7.137 min
 Delta R.T.: -0.009 min
 Response: 47082456
 Conc: 526.60 ng/ml

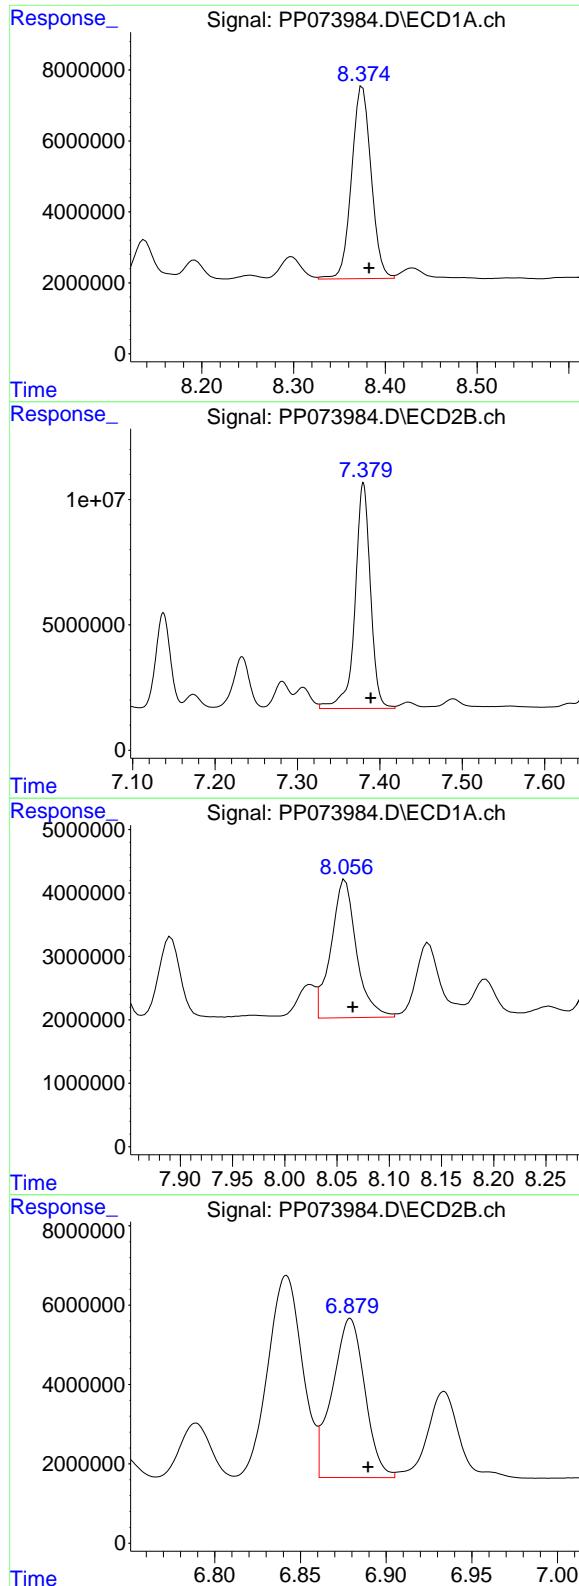

#35 AR-1260-5

R.T.: 8.375 min
 Delta R.T.: -0.007 min
 Response: 80346257
 Conc: 532.61 ng/ml

Instrument: ECD_P
 ClientSampleId: RT2286MS

#35 AR-1260-5


R.T.: 7.380 min
 Delta R.T.: -0.009 min
 Response: 117176775
 Conc: 521.40 ng/ml

#36 AR-1262-1

R.T.: 8.058 min
 Delta R.T.: -0.007 min
 Response: 36868595
 Conc: 423.64 ng/ml

#36 AR-1262-1


R.T.: 6.879 min
 Delta R.T.: -0.010 min
 Response: 52862605
 Conc: 357.93 ng/ml



#37 AR-1262-2


R.T.: 8.375 min
Delta R.T.: -0.008 min
Response: 80346257
Conc: 405.73 ng/ml

Instrument: ECD_P
ClientSampleId: RT2286MS

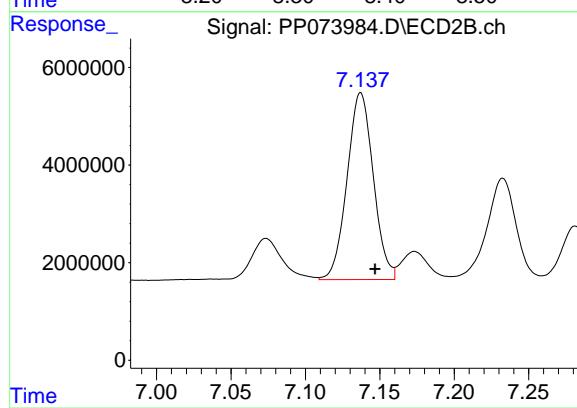


#37 AR-1262-2

R.T.: 7.137 min
Delta R.T.: -0.010 min
Response: 47082456
Conc: 368.32 ng/ml

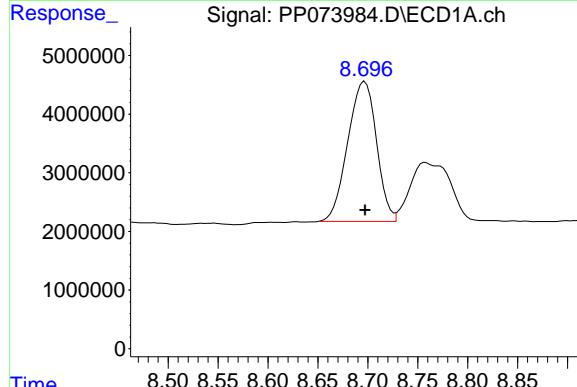


#38 AR-1262-3

R.T.: 8.697 min
Delta R.T.: 0.000 min
Response: 47764045
Conc: 379.91 ng/ml

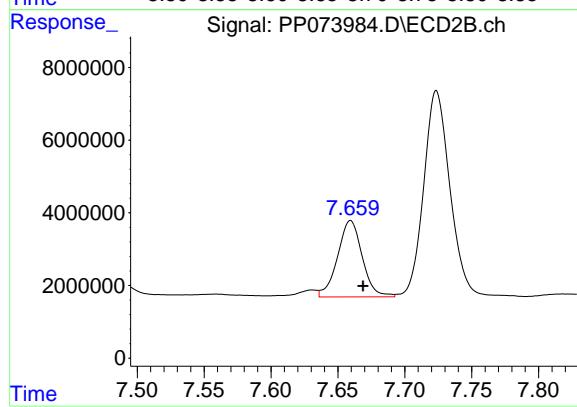

#38 AR-1262-3

R.T.: 7.659 min
Delta R.T.: -0.009 min
Response: 26973034
Conc: 236.57 ng/ml

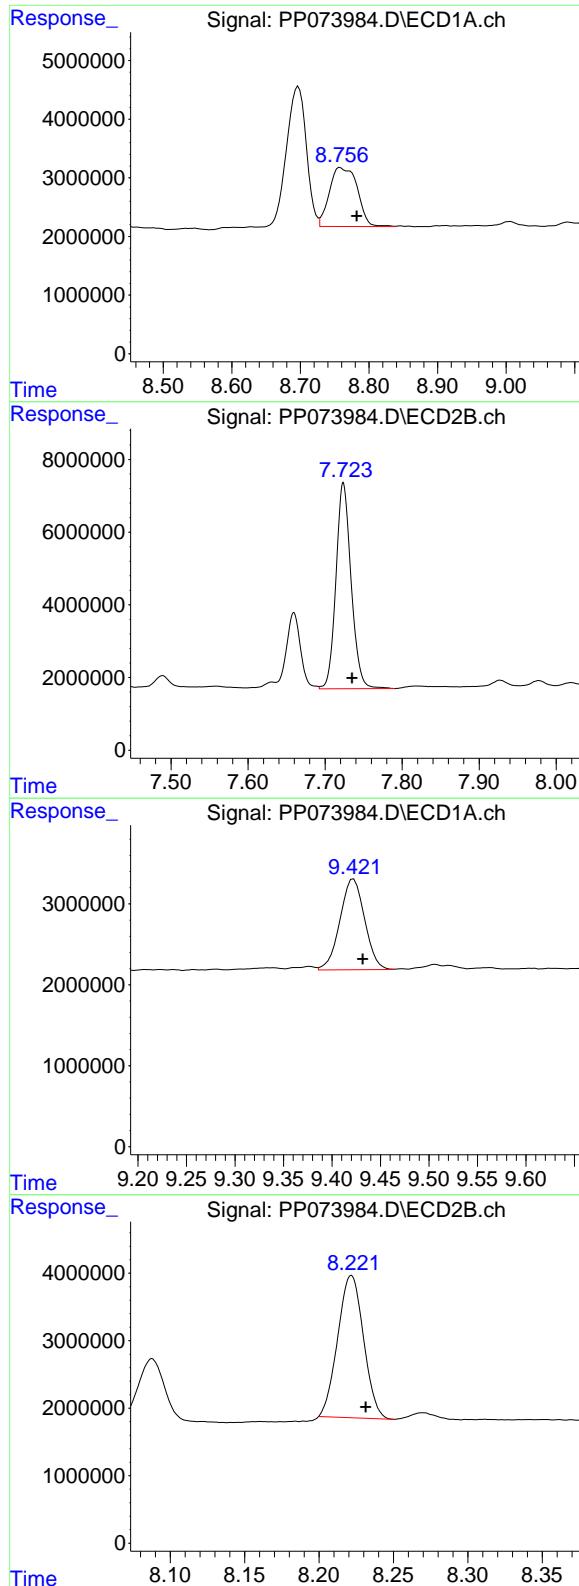

#39 AR-1262-4

R.T.: 8.758 min
 Delta R.T.: -0.024 min
 Response: 28415445
 Conc: 304.68 ng/ml

Instrument: ECD_P
 ClientSampleId: RT2286MS

#39 AR-1262-4


R.T.: 7.724 min
 Delta R.T.: -0.011 min
 Response: 77752202
 Conc: 422.45 ng/ml

#40 AR-1262-5

R.T.: 9.422 min
 Delta R.T.: -0.009 min
 Response: 19854543
 Conc: 313.22 ng/ml

#40 AR-1262-5

R.T.: 8.222 min
 Delta R.T.: -0.010 min
 Response: 25455071
 Conc: 301.47 ng/ml

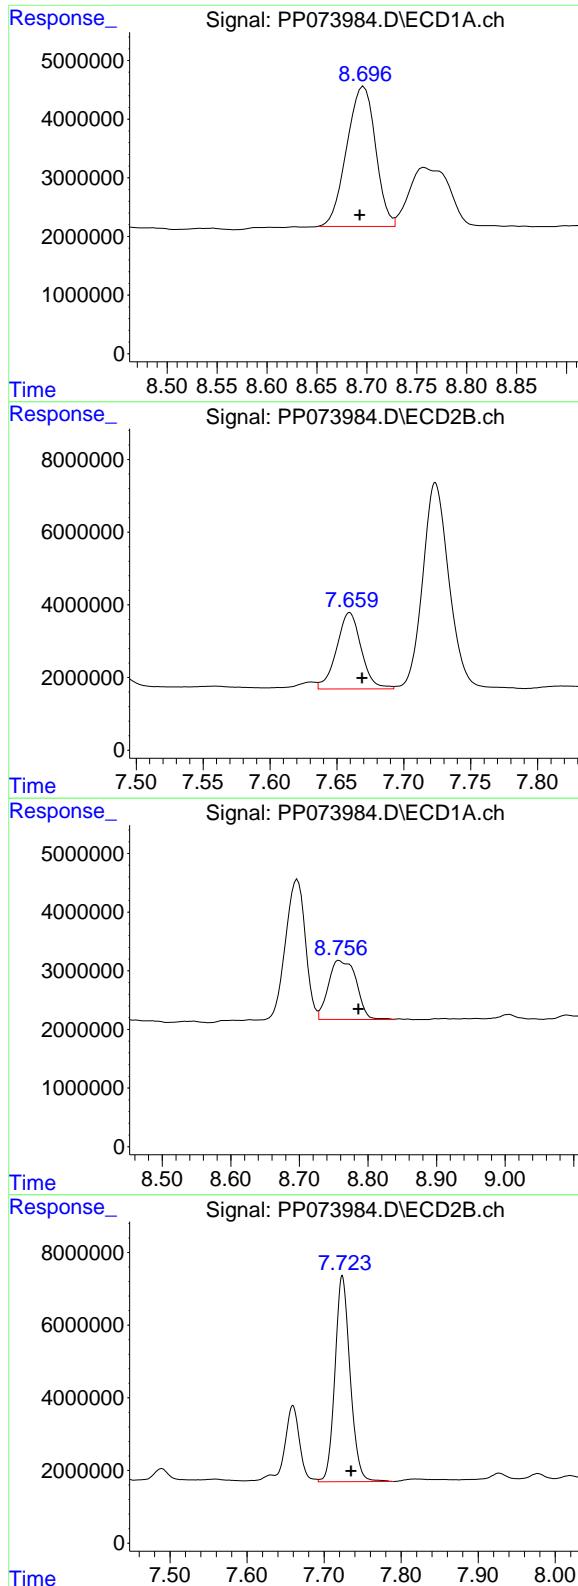

#41 AR-1268-1

R.T.: 8.697 min
 Delta R.T.: 0.004 min
 Response: 47764045
 Conc: 213.97 ng/ml

Instrument: ECD_P
 ClientSampleId: RT2286MS

#41 AR-1268-1


R.T.: 7.659 min
 Delta R.T.: -0.009 min
 Response: 26973034
 Conc: 87.75 ng/ml

#42 AR-1268-2

R.T.: 8.758 min
 Delta R.T.: -0.028 min
 Response: 28415445
 Conc: 149.16 ng/ml

#42 AR-1268-2


R.T.: 7.724 min
 Delta R.T.: -0.012 min
 Response: 77752202
 Conc: 292.64 ng/ml

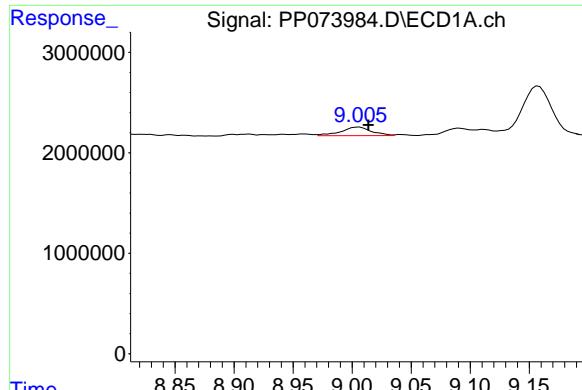

#43 AR-1268-3


R.T.: 9.006 min
Delta R.T.: -0.008 min
Response: 1539585
Conc: 9.30 ng/ml

Instrument: ECD_P
ClientSampleId: RT2286MS

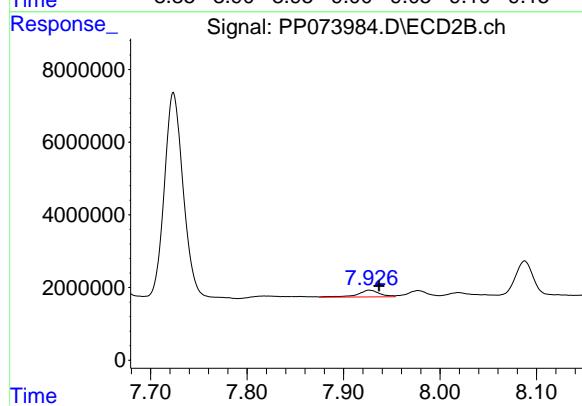


#43 AR-1268-3

R.T.: 7.927 min
Delta R.T.: -0.010 min
Response: 2942539
Conc: 13.04 ng/ml

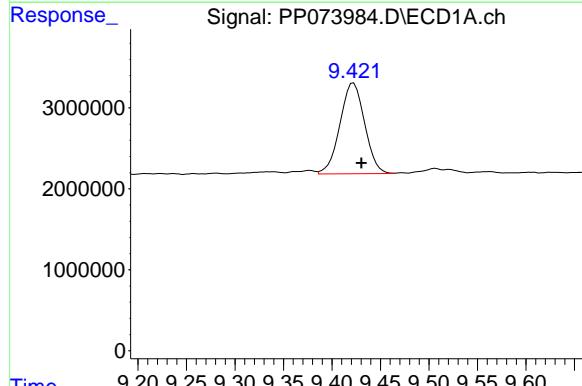


#44 AR-1268-4

R.T.: 9.422 min
Delta R.T.: -0.008 min
Response: 19854543
Conc: 285.50 ng/ml

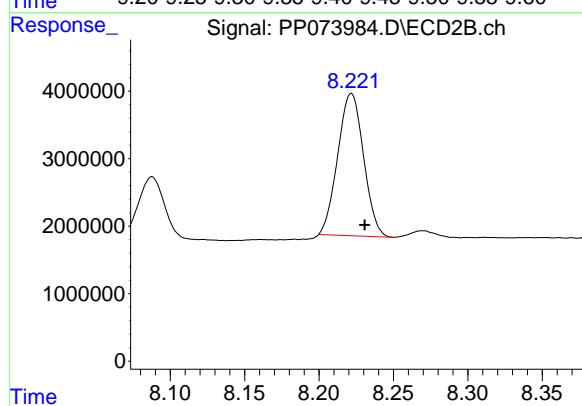

#44 AR-1268-4

R.T.: 8.222 min
Delta R.T.: -0.009 min
Response: 25455071
Conc: 273.81 ng/ml

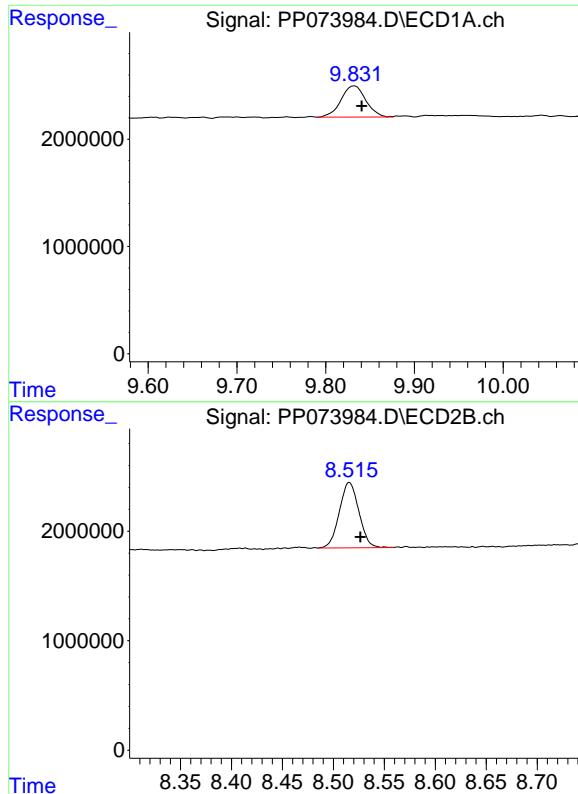

#45 AR-1268-5

R.T.: 9.833 min
Delta R.T.: -0.008 min
Response: 5638616
Conc: 12.23 ng/ml

Instrument: ECD_P
ClientSampleId: RT2286MS

#45 AR-1268-5

R.T.: 8.516 min
Delta R.T.: -0.011 min
Response: 8000594
Conc: 12.98 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP072125\
 Data File : PP073985.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jul 2025 13:56
 Operator : YP\AJ
 Sample : Q2635-01MSD
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
RT2286MSD

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 22 01:51:16 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 08 08:35:32 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	4.485	3.774	23007780	32891692	16.800	17.854
2) SA Decachlor...	10.171	8.771	19437749	25634073	17.816	19.374

Target Compounds

3) L1 AR-1016-1	5.636	4.851	18736879	29541322	394.348	433.318
4) L1 AR-1016-2	5.657	4.869	30133135	43844893	423.130	430.340
5) L1 AR-1016-3	5.719	5.045	18269038	24208384	418.409	447.422
6) L1 AR-1016-4	5.816	5.087	16118675	19716668	448.419	449.323
7) L1 AR-1016-5	6.110	5.300	17783528	24543584	567.612	449.660
8) L2 AR-1221-1	4.684	3.982	2316741	3672400	129.670	135.789
9) L2 AR-1221-2	4.772	4.069	2571348	4922940	190.407	241.791 #
10) L2 AR-1221-3	4.847	4.144	11286630	16409637	271.282	267.046
11) L3 AR-1232-1	4.847	4.144	11286630	16409637	345.678	352.030
12) L3 AR-1232-2	5.371	4.869	17167747	43844893	1056.173	919.955
13) L3 AR-1232-3	5.657	5.045	30133135	24208384	913.306	967.212
14) L3 AR-1232-4	5.816	5.129	16118675	22709464	980.147	1048.631
15) L3 AR-1232-5	5.907	5.300	11991357	24543584	1134.432	1087.759
16) L4 AR-1242-1	5.636	4.851	18736879	29541322	490.646	511.407
17) L4 AR-1242-2	5.657	4.869	30133135	43844893	503.208	507.146
18) L4 AR-1242-3	5.719	5.045	18269038	24208384	498.869	526.880
19) L4 AR-1242-4	5.816	5.129	16118675	22709464	501.577	513.054
20) L4 AR-1242-5	6.546	5.651	6319352	24658094	193.035	446.361 #
21) L5 AR-1248-1	5.636	4.851	18736879	29541322	606.950	658.011
22) L5 AR-1248-2	5.907	5.087	11991357	19716668	300.359	320.406
23) L5 AR-1248-3	6.110	5.129	17783528	22709464	400.443	354.478
24) L5 AR-1248-4	6.483	5.300	19277292	24543584	349.984	325.609
25) L5 AR-1248-5	6.546	5.690	6319352	5986328	117.481	80.255 #
26) L6 AR-1254-1	6.483	5.651	19277292	24658094	359.721	212.515 #
27) L6 AR-1254-2	6.698	5.799	18157197	23975260	218.003	238.267
28) L6 AR-1254-3	7.063	6.214	10928576	44083931	123.722	285.432 #
29) L6 AR-1254-4	7.344	6.428	10348921	6367228	131.553	67.336 #
30) L6 AR-1254-5	7.759	6.844	53191433	71090554	721.927	532.734 #
31) L7 AR-1260-1	7.226	6.330	35309050	54851085	598.852	562.228
32) L7 AR-1260-2	7.479	6.518	49841976	65815583	520.055	535.794
33) L7 AR-1260-3	7.837	6.670	37810191	59476912	517.447	543.348
34) L7 AR-1260-4	8.061	7.139	45575779	46277558	697.946	517.597 #
35) L7 AR-1260-5	8.378	7.383	80997949	117.0E6	536.934	520.578
36) L8 AR-1262-1	8.061	6.881	45575779	52214863	523.695	353.540 #
37) L8 AR-1262-2	8.378	7.139	80997949	46277558	409.024	362.027
38) L8 AR-1262-3	8.700	7.661	47490444	26041835	377.733	228.399 #
39) L8 AR-1262-4	8.777	7.726	10905481	76651297	116.933	416.472 #
40) L8 AR-1262-5	9.426	8.224	19633340	25848025	309.726	306.127
41) L9 AR-1268-1	8.700	7.661	47490444	26041835	212.748	84.723 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP072125\
 Data File : PP073985.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jul 2025 13:56
 Operator : YP\AJ
 Sample : Q2635-01MSD
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
RT2286MSD

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 22 01:51:16 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 08 08:35:32 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9 AR-1268-2	8.777	7.726	10905481	76651297	57.245	288.501 #
43) L9 AR-1268-3	9.009	7.930	1635702	2877785	9.879	12.757 #
44) L9 AR-1268-4	9.426	8.224	19633340	25848025	282.316	278.032
45) L9 AR-1268-5	9.836	8.517	5572340	7686741	12.089	12.467



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP072125\
 Data File : PP073985.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jul 2025 13:56
 Operator : YP\AJ
 Sample : Q2635-01MSD
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
RT2286MSD

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 22 01:51:16 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 08 08:35:32 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ m Signal #2 Info : 30M x 0.32mm x 0.25 μ m

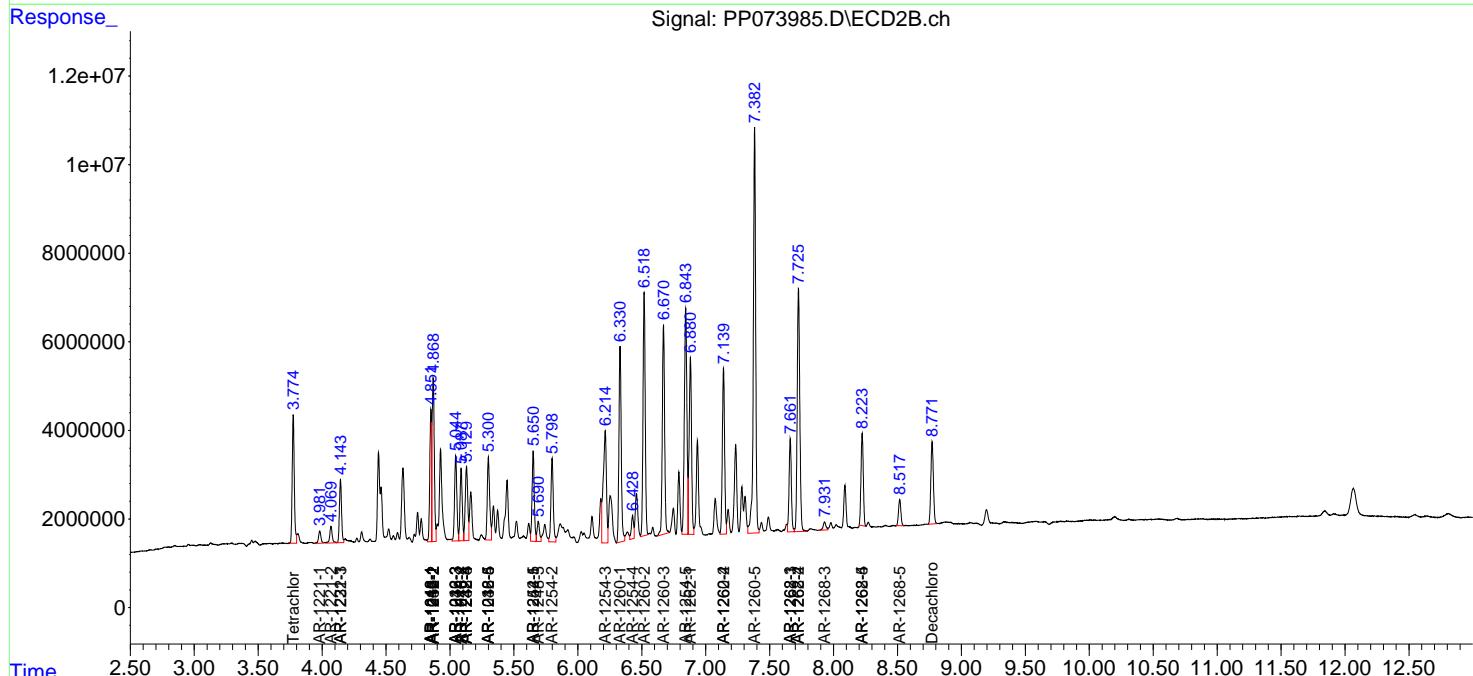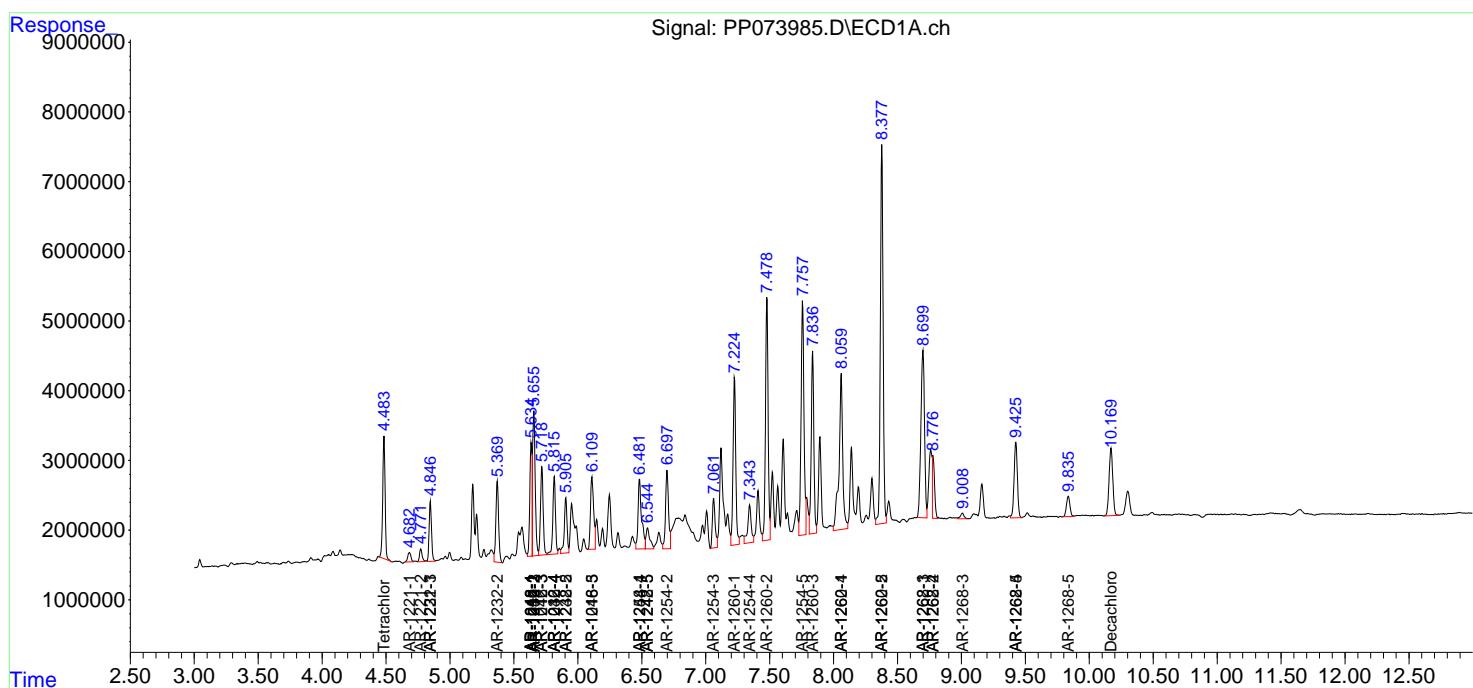

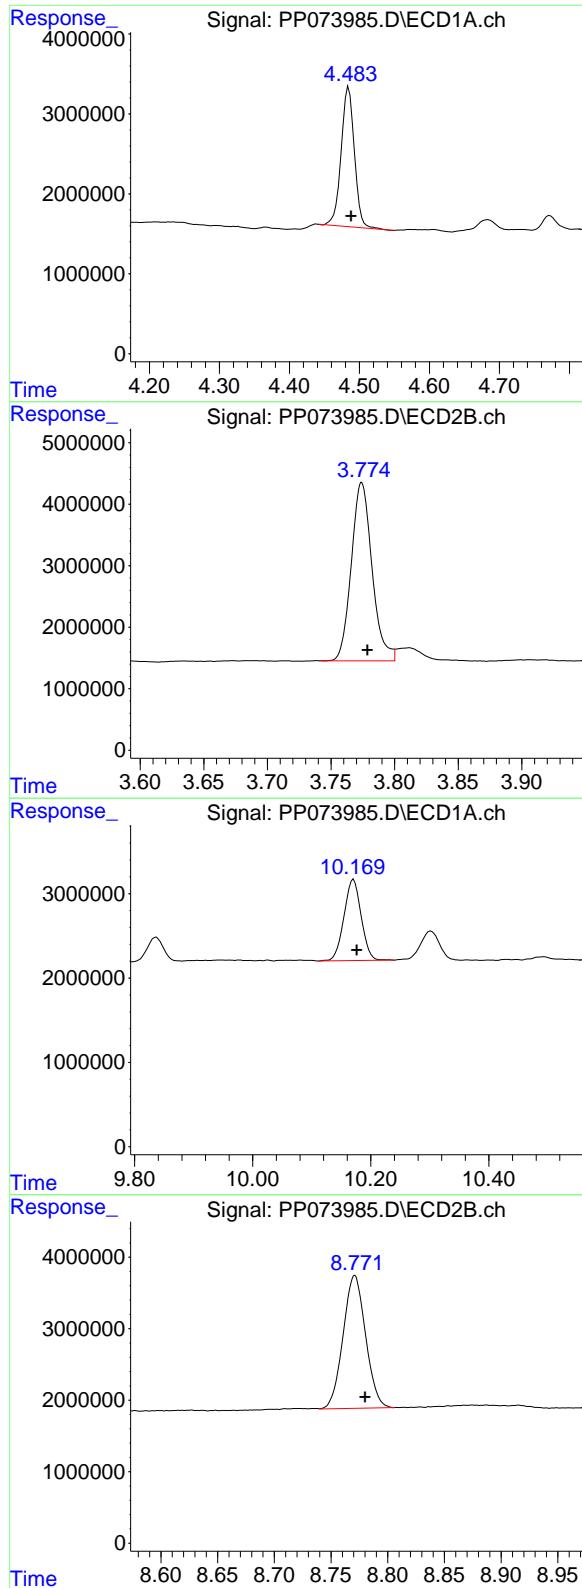

#1 Tetrachloro-m-xylene

R.T.: 4.485 min
 Delta R.T.: -0.003 min
 Response: 23007780
 Conc: 16.80 ng/ml

Instrument: ECD_P
 ClientSampleId: RT2286MSD

#1 Tetrachloro-m-xylene


R.T.: 3.774 min
 Delta R.T.: -0.004 min
 Response: 32891692
 Conc: 17.85 ng/ml

#2 Decachlorobiphenyl

R.T.: 10.171 min
 Delta R.T.: -0.005 min
 Response: 19437749
 Conc: 17.82 ng/ml

#2 Decachlorobiphenyl

R.T.: 8.771 min
 Delta R.T.: -0.009 min
 Response: 25634073
 Conc: 19.37 ng/ml

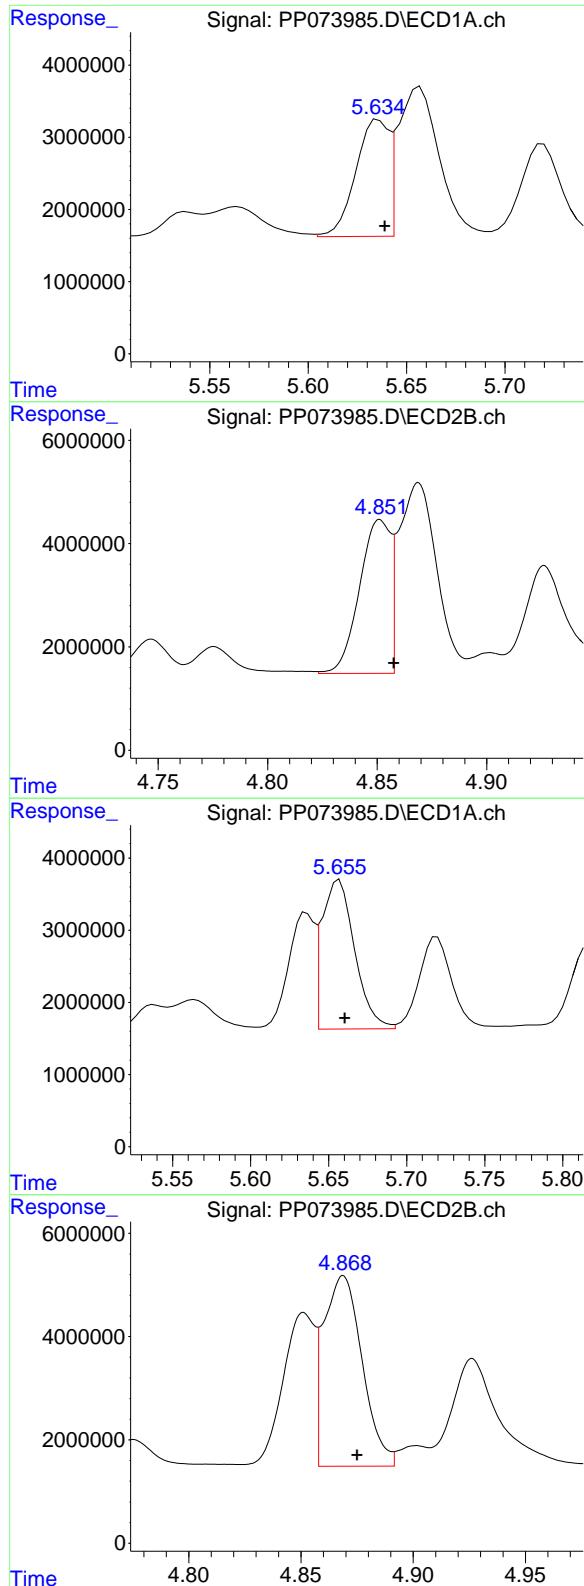

#3 AR-1016-1

R.T.: 5.636 min
 Delta R.T.: -0.003 min
 Response: 18736879
 Conc: 394.35 ng/ml

Instrument: ECD_P
 ClientSampleId: RT2286MSD

#3 AR-1016-1


R.T.: 4.851 min
 Delta R.T.: -0.006 min
 Response: 29541322
 Conc: 433.32 ng/ml

#4 AR-1016-2

R.T.: 5.657 min
 Delta R.T.: -0.004 min
 Response: 30133135
 Conc: 423.13 ng/ml

#4 AR-1016-2


R.T.: 4.869 min
 Delta R.T.: -0.006 min
 Response: 43844893
 Conc: 430.34 ng/ml

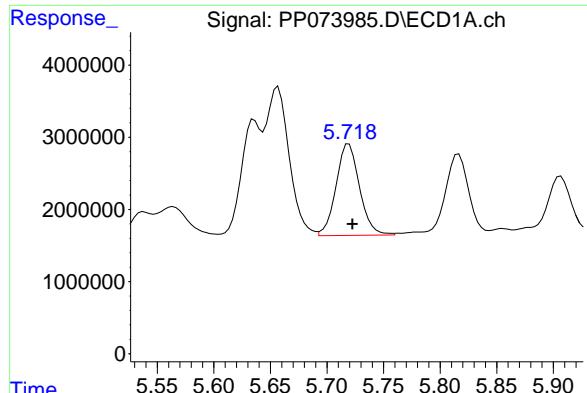

#5 AR-1016-3


R.T.: 5.719 min
 Delta R.T.: -0.003 min
 Response: 18269038
 Conc: 418.41 ng/ml

Instrument: ECD_P
 ClientSampleId: RT2286MSD

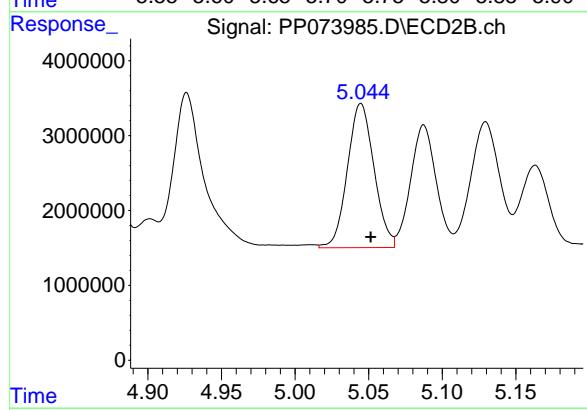


#5 AR-1016-3

R.T.: 5.045 min
 Delta R.T.: -0.007 min
 Response: 24208384
 Conc: 447.42 ng/ml

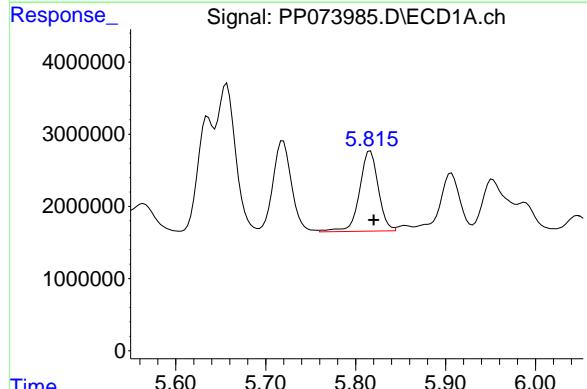


#6 AR-1016-4

R.T.: 5.816 min
 Delta R.T.: -0.004 min
 Response: 16118675
 Conc: 448.42 ng/ml

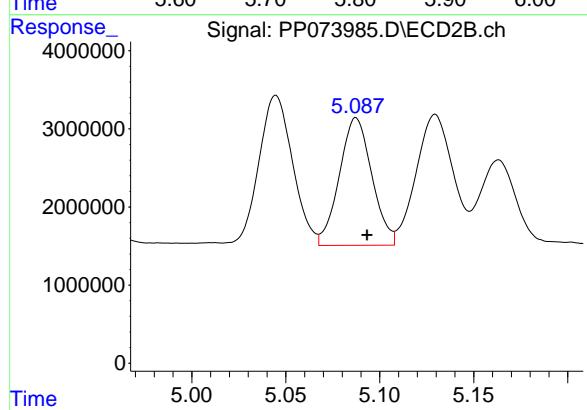

#6 AR-1016-4


R.T.: 5.087 min
 Delta R.T.: -0.006 min
 Response: 19716668
 Conc: 449.32 ng/ml

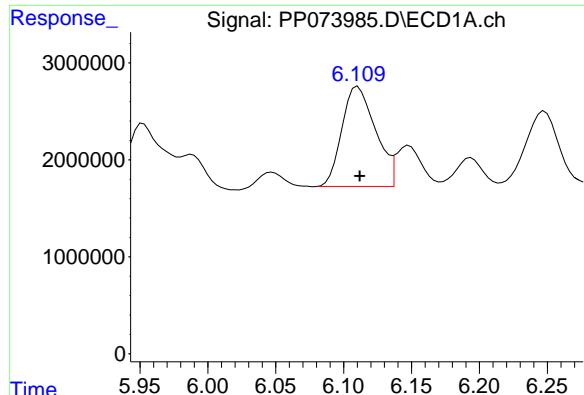

#7 AR-1016-5


R.T.: 6.110 min
 Delta R.T.: -0.001 min
 Response: 17783528
 Conc: 567.61 ng/ml

Instrument: ECD_P
 ClientSampleId: RT2286MSD

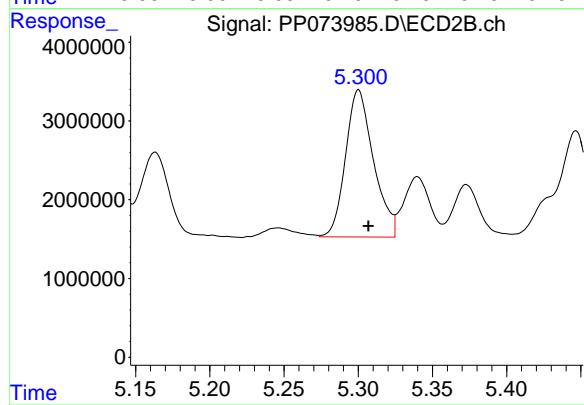


#7 AR-1016-5

R.T.: 5.300 min
 Delta R.T.: -0.007 min
 Response: 24543584
 Conc: 449.66 ng/ml

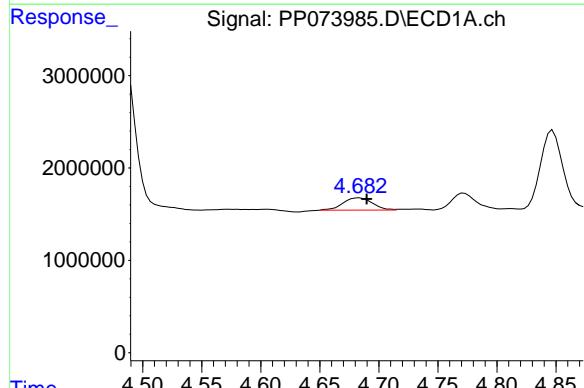


#8 AR-1221-1

R.T.: 4.684 min
 Delta R.T.: -0.006 min
 Response: 2316741
 Conc: 129.67 ng/ml

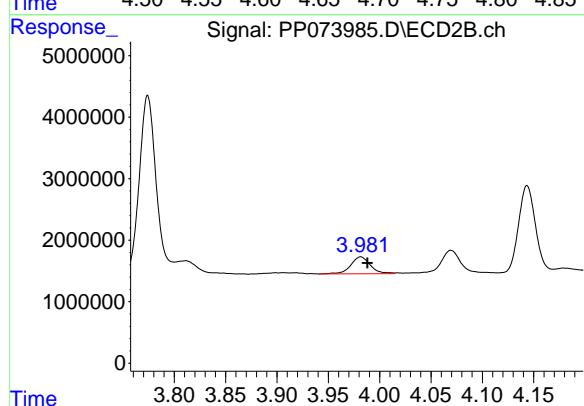

#8 AR-1221-1

R.T.: 3.982 min
 Delta R.T.: -0.006 min
 Response: 3672400
 Conc: 135.79 ng/ml

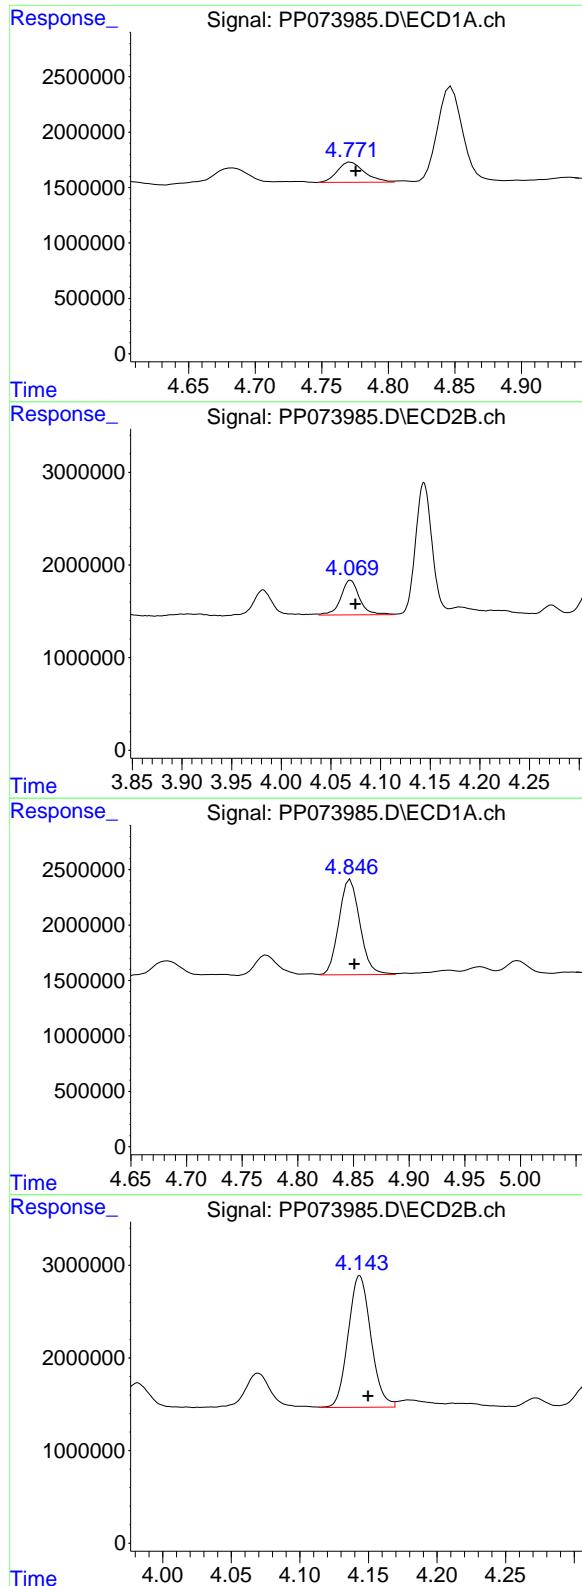

#9 AR-1221-2

R.T.: 4.772 min
 Delta R.T.: -0.003 min
 Response: 2571348
 Conc: 190.41 ng/ml

Instrument: ECD_P
 ClientSampleId: RT2286MSD

#9 AR-1221-2


R.T.: 4.069 min
 Delta R.T.: -0.005 min
 Response: 4922940
 Conc: 241.79 ng/ml

#10 AR-1221-3

R.T.: 4.847 min
 Delta R.T.: -0.004 min
 Response: 11286630
 Conc: 271.28 ng/ml

#10 AR-1221-3


R.T.: 4.144 min
 Delta R.T.: -0.006 min
 Response: 16409637
 Conc: 267.05 ng/ml

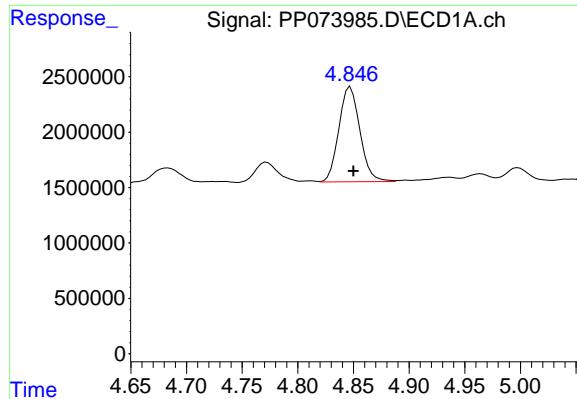

#11 AR-1232-1


R.T.: 4.847 min
 Delta R.T.: -0.003 min
 Response: 11286630
 Conc: 345.68 ng/ml

Instrument: ECD_P
 ClientSampleId: RT2286MSD

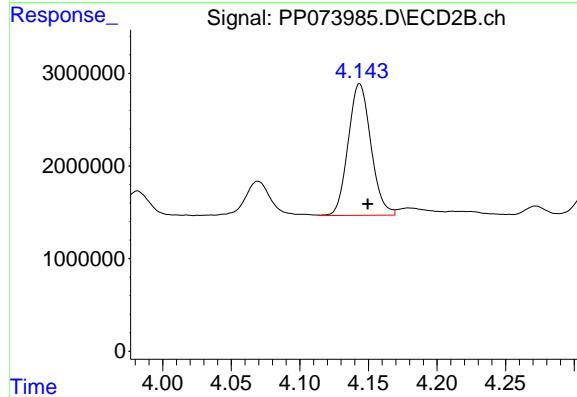


#11 AR-1232-1

R.T.: 4.144 min
 Delta R.T.: -0.006 min
 Response: 16409637
 Conc: 352.03 ng/ml

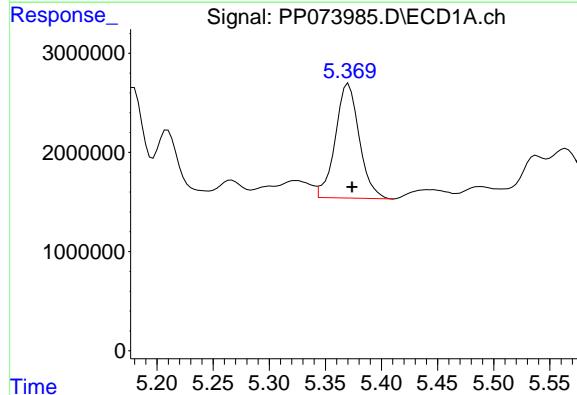


#12 AR-1232-2

R.T.: 5.371 min
 Delta R.T.: -0.003 min
 Response: 17167747
 Conc: 1056.17 ng/ml

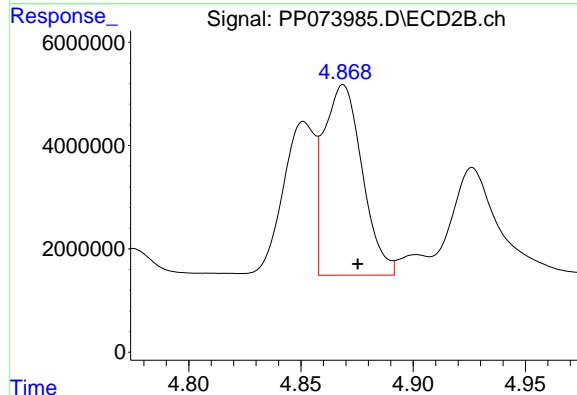

#12 AR-1232-2


R.T.: 4.869 min
 Delta R.T.: -0.007 min
 Response: 43844893
 Conc: 919.96 ng/ml

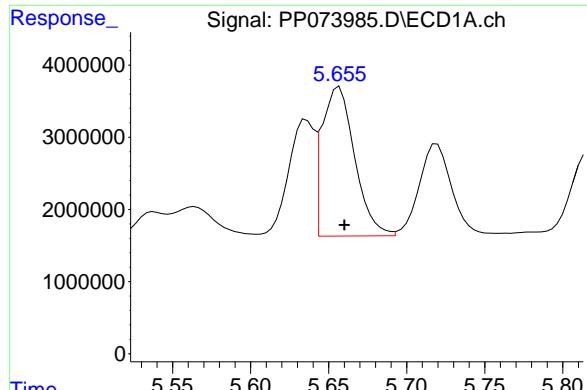

#13 AR-1232-3


R.T.: 5.657 min
 Delta R.T.: -0.003 min
 Response: 30133135
 Conc: 913.31 ng/ml

Instrument: ECD_P
 ClientSampleId: RT2286MSD

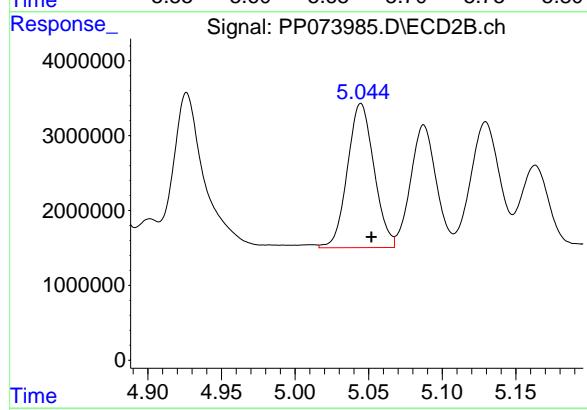


#13 AR-1232-3

R.T.: 5.045 min
 Delta R.T.: -0.007 min
 Response: 24208384
 Conc: 967.21 ng/ml

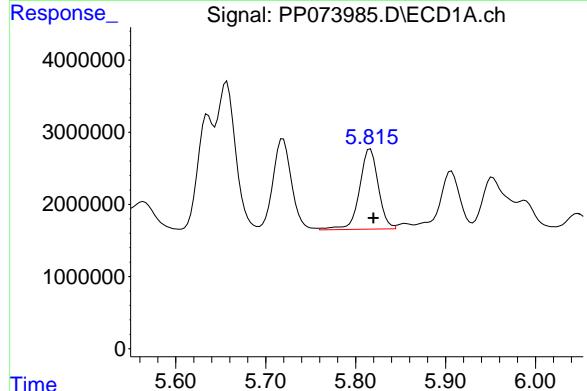


#14 AR-1232-4

R.T.: 5.816 min
 Delta R.T.: -0.004 min
 Response: 16118675
 Conc: 980.15 ng/ml

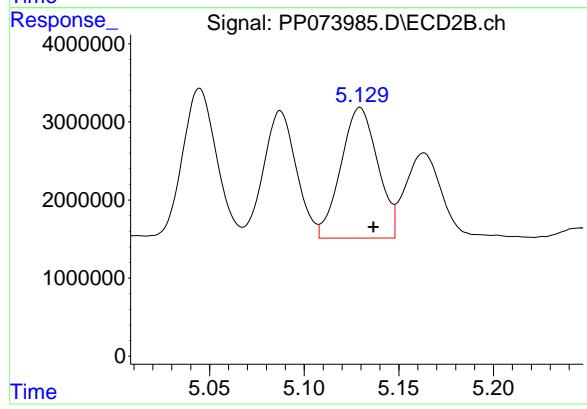

#14 AR-1232-4

R.T.: 5.129 min
 Delta R.T.: -0.007 min
 Response: 22709464
 Conc: 1048.63 ng/ml

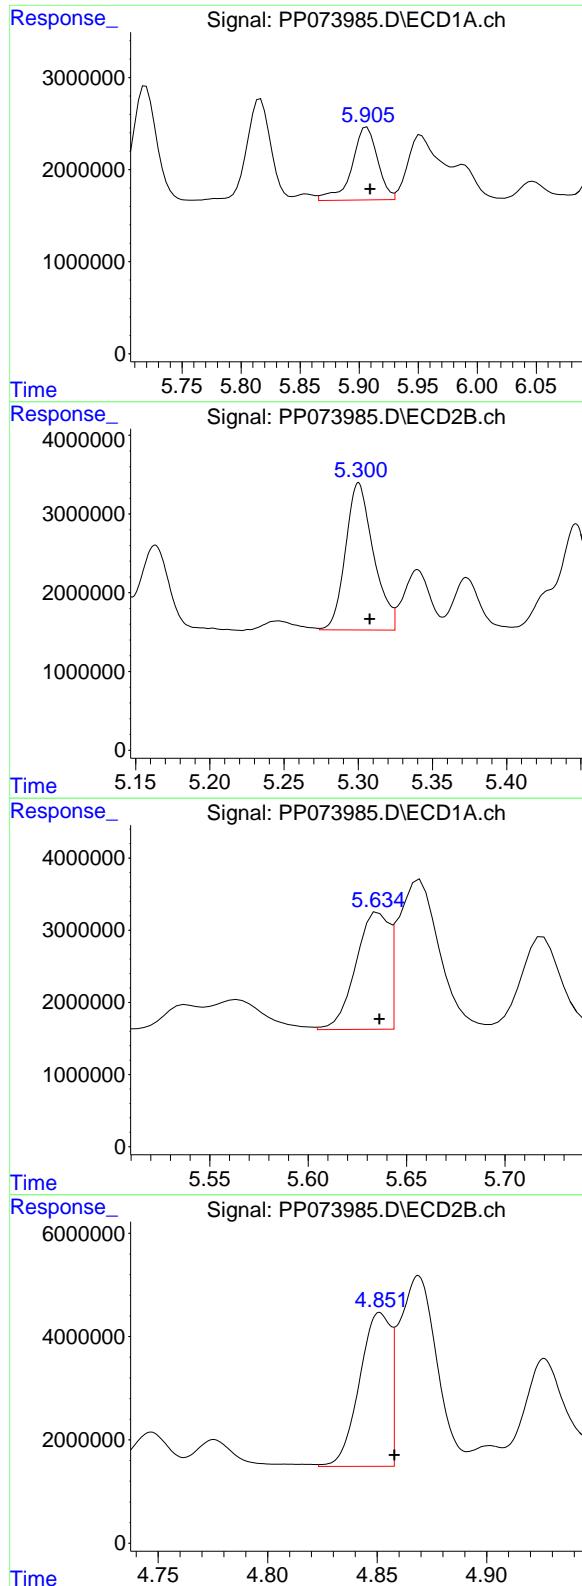

#15 AR-1232-5

R.T.: 5.907 min
 Delta R.T.: -0.003 min
 Response: 11991357
 Conc: 1134.43 ng/ml

Instrument: ECD_P
 ClientSampleId: RT2286MSD

#15 AR-1232-5


R.T.: 5.300 min
 Delta R.T.: -0.008 min
 Response: 24543584
 Conc: 1087.76 ng/ml

#16 AR-1242-1

R.T.: 5.636 min
 Delta R.T.: 0.000 min
 Response: 18736879
 Conc: 490.65 ng/ml

#16 AR-1242-1

R.T.: 4.851 min
 Delta R.T.: -0.007 min
 Response: 29541322
 Conc: 511.41 ng/ml

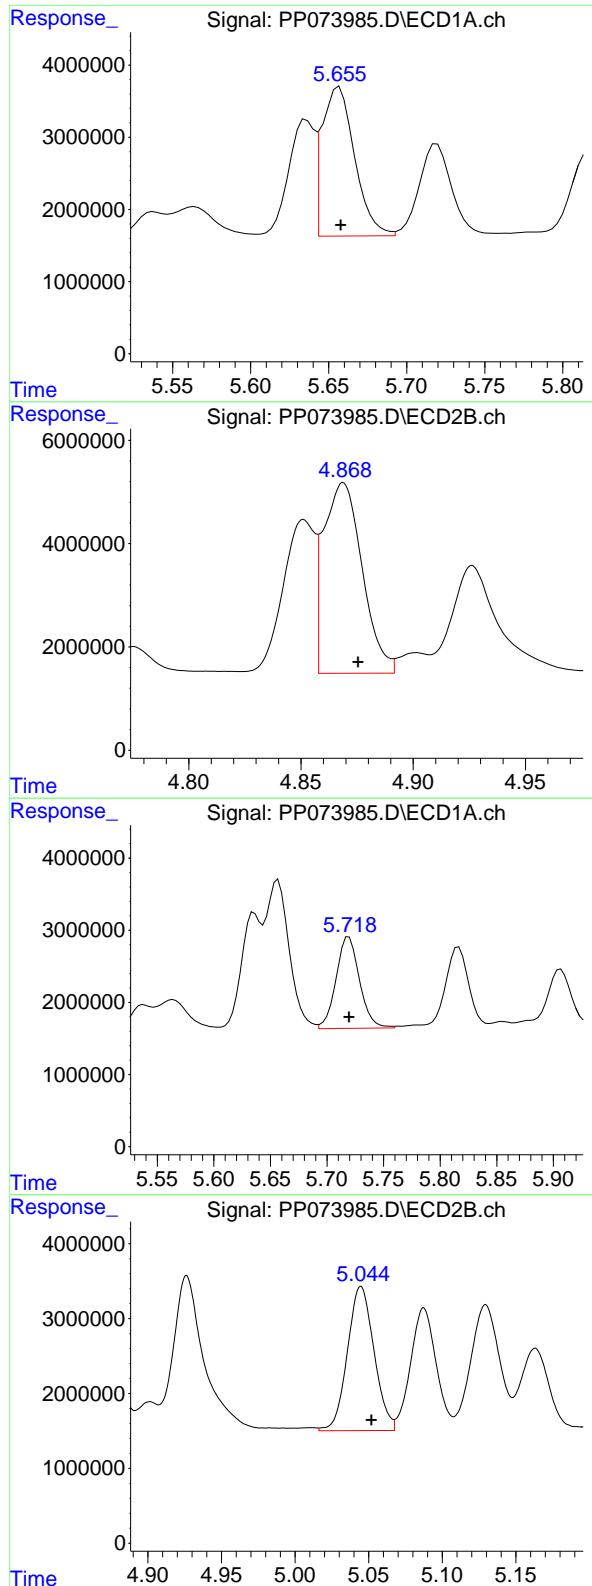

#17 AR-1242-2

R.T.: 5.657 min
 Delta R.T.: 0.000 min
 Response: 30133135
 Conc: 503.21 ng/ml

Instrument: ECD_P
 ClientSampleId: RT2286MSD

#17 AR-1242-2


R.T.: 4.869 min
 Delta R.T.: -0.007 min
 Response: 43844893
 Conc: 507.15 ng/ml

#18 AR-1242-3

R.T.: 5.719 min
 Delta R.T.: 0.000 min
 Response: 18269038
 Conc: 498.87 ng/ml


#18 AR-1242-3

R.T.: 5.045 min
 Delta R.T.: -0.007 min
 Response: 24208384
 Conc: 526.88 ng/ml

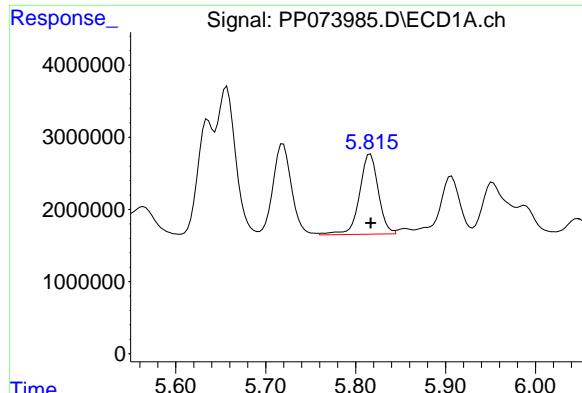


#19 AR-1242-4

R.T.: 5.816 min
 Delta R.T.: 0.000 min **Instrument:**
 Response: 16118675 ECD_P
 Conc: 501.58 ng/ml **ClientSampleId:**
 RT2286MSD

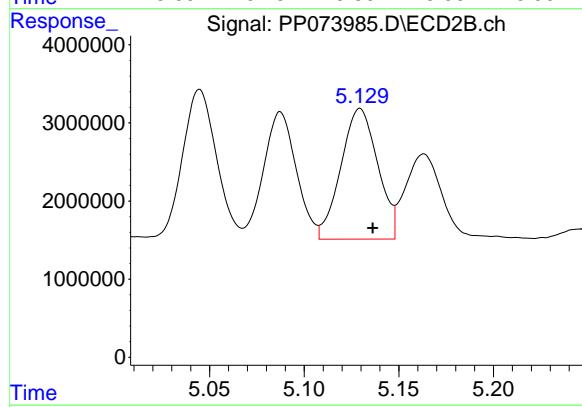


#19 AR-1242-4

R.T.: 5.129 min
 Delta R.T.: -0.007 min
 Response: 22709464
 Conc: 513.05 ng/ml

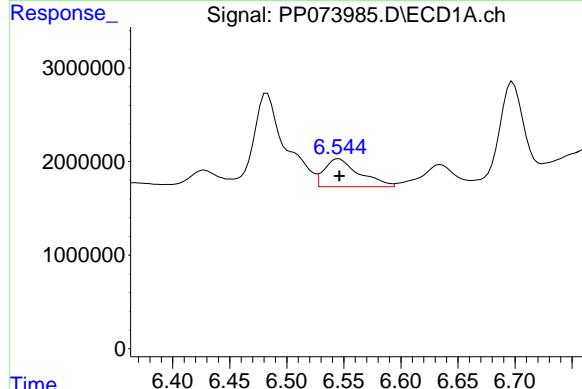


#20 AR-1242-5

R.T.: 6.546 min
 Delta R.T.: 0.000 min
 Response: 6319352
 Conc: 193.03 ng/ml

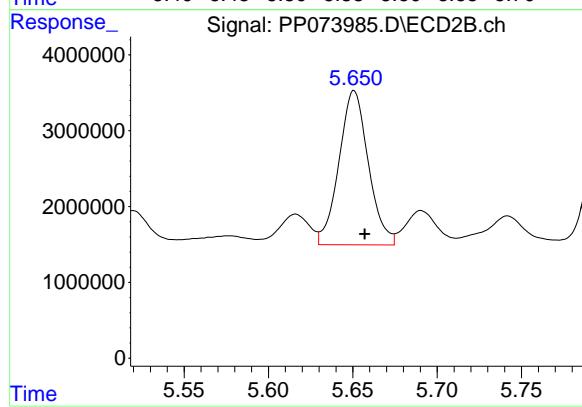

#20 AR-1242-5

R.T.: 5.651 min
 Delta R.T.: -0.006 min
 Response: 24658094
 Conc: 446.36 ng/ml

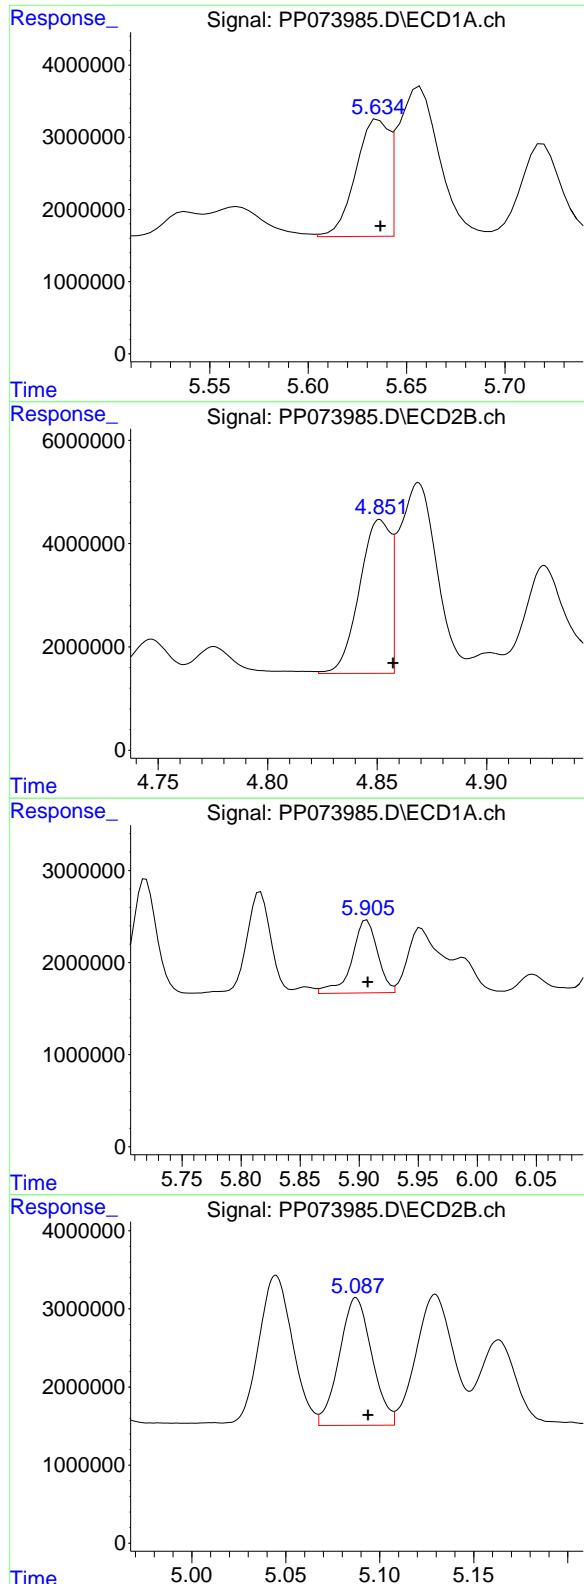

#21 AR-1248-1

R.T.: 5.636 min
 Delta R.T.: 0.000 min
 Response: 18736879
 Conc: 606.95 ng/ml

Instrument: ECD_P
 ClientSampleId: RT2286MSD

#21 AR-1248-1


R.T.: 4.851 min
 Delta R.T.: -0.006 min
 Response: 29541322
 Conc: 658.01 ng/ml

#22 AR-1248-2

R.T.: 5.907 min
 Delta R.T.: 0.000 min
 Response: 11991357
 Conc: 300.36 ng/ml

#22 AR-1248-2

R.T.: 5.087 min
 Delta R.T.: -0.006 min
 Response: 19716668
 Conc: 320.41 ng/ml

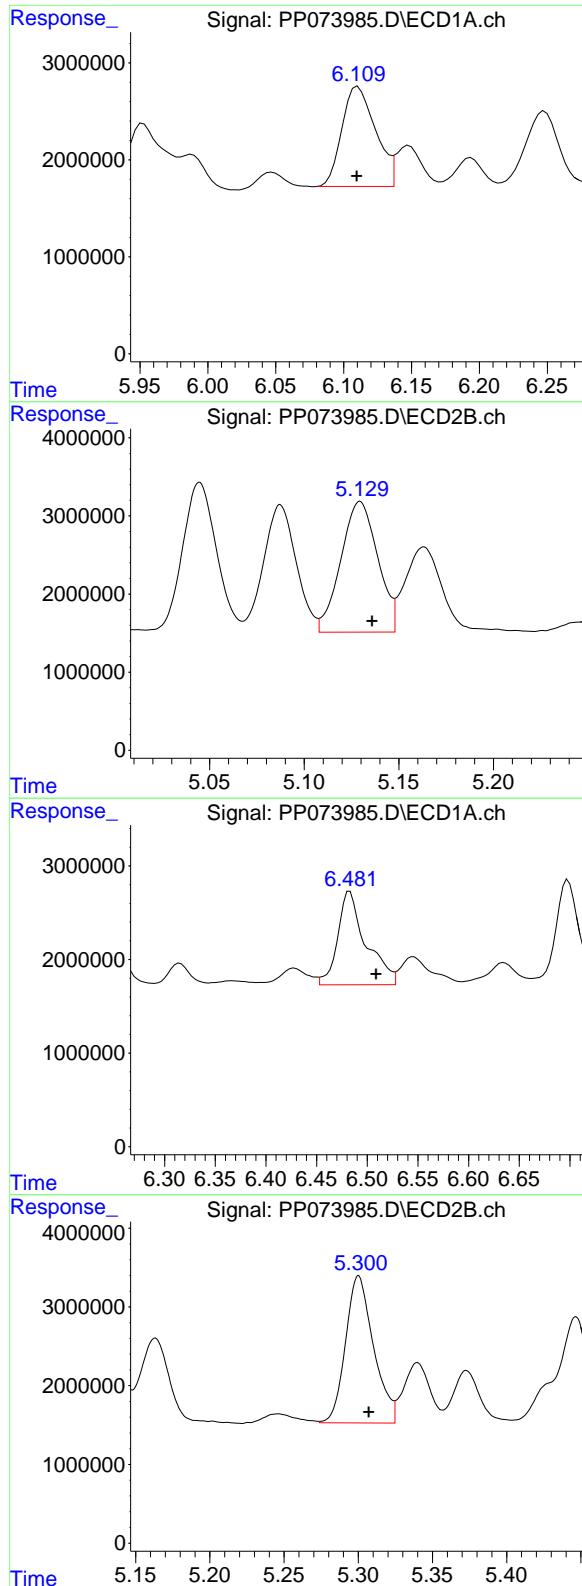

#23 AR-1248-3

R.T.: 6.110 min
 Delta R.T.: 0.000 min
 Response: 17783528
 Conc: 400.44 ng/ml

Instrument: ECD_P
 ClientSampleId: RT2286MSD

#23 AR-1248-3


R.T.: 5.129 min
 Delta R.T.: -0.006 min
 Response: 22709464
 Conc: 354.48 ng/ml

#24 AR-1248-4

R.T.: 6.483 min
 Delta R.T.: -0.026 min
 Response: 19277292
 Conc: 349.98 ng/ml

#24 AR-1248-4


R.T.: 5.300 min
 Delta R.T.: -0.007 min
 Response: 24543584
 Conc: 325.61 ng/ml

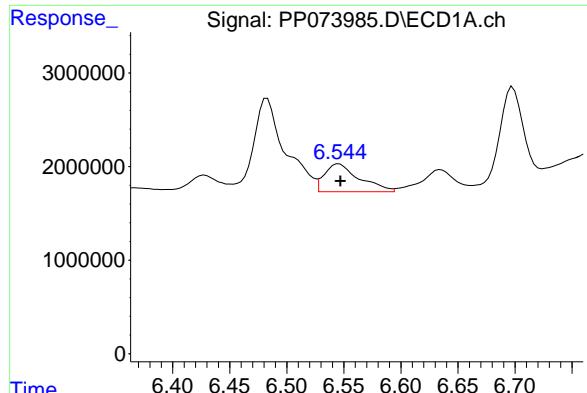

#25 AR-1248-5


R.T.: 6.546 min
Delta R.T.: -0.001 min
Response: 6319352
Conc: 117.48 ng/ml

Instrument: ECD_P
ClientSampleId: RT2286MSD

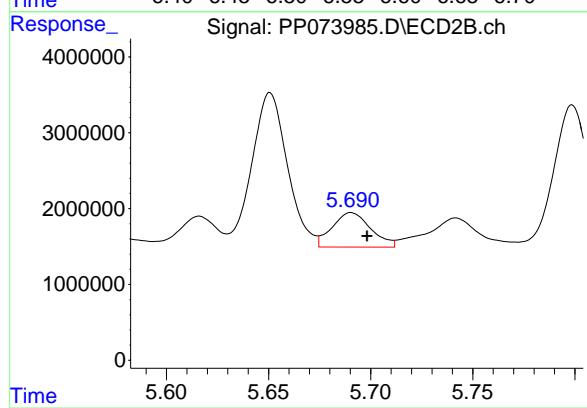


#25 AR-1248-5

R.T.: 5.690 min
Delta R.T.: -0.008 min
Response: 5986328
Conc: 80.26 ng/ml

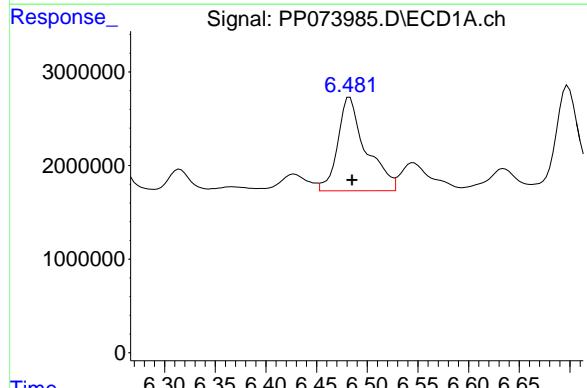


#26 AR-1254-1

R.T.: 6.483 min
Delta R.T.: -0.002 min
Response: 19277292
Conc: 359.72 ng/ml

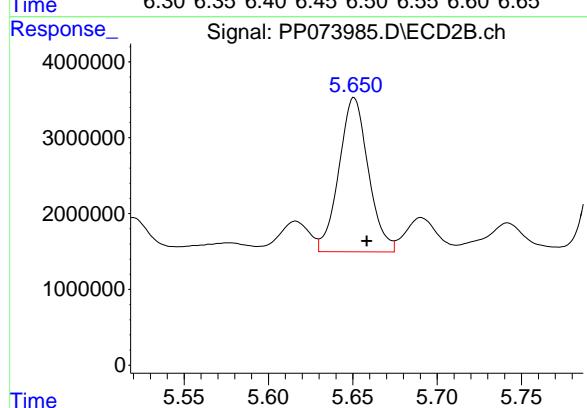

#26 AR-1254-1


R.T.: 5.651 min
Delta R.T.: -0.007 min
Response: 24658094
Conc: 212.51 ng/ml

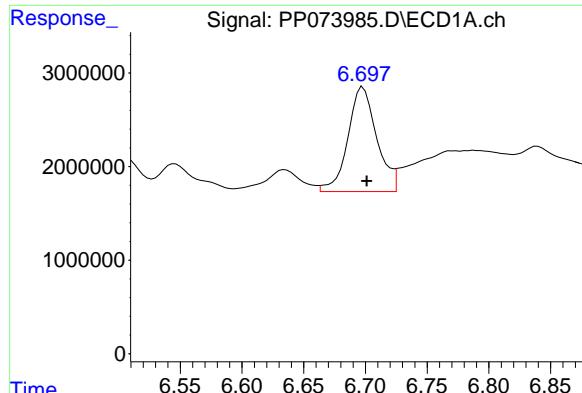

#27 AR-1254-2

R.T.: 6.698 min
 Delta R.T.: -0.003 min
 Response: 18157197
 Conc: 218.00 ng/ml

Instrument: ECD_P
 ClientSampleId: RT2286MSD

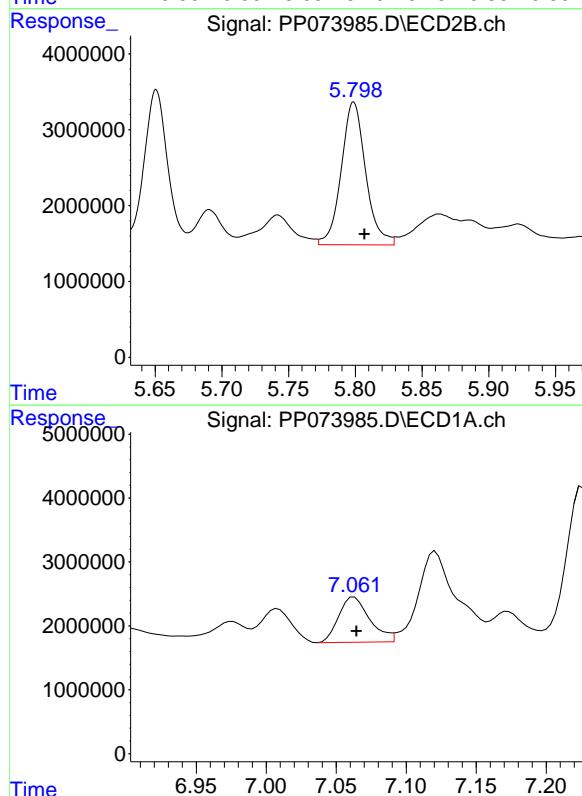


#28 AR-1254-3

R.T.: 7.063 min
 Delta R.T.: -0.002 min
 Response: 10928576
 Conc: 123.72 ng/ml

#28 AR-1254-3


R.T.: 6.214 min
 Delta R.T.: 0.006 min
 Response: 44083931
 Conc: 285.43 ng/ml

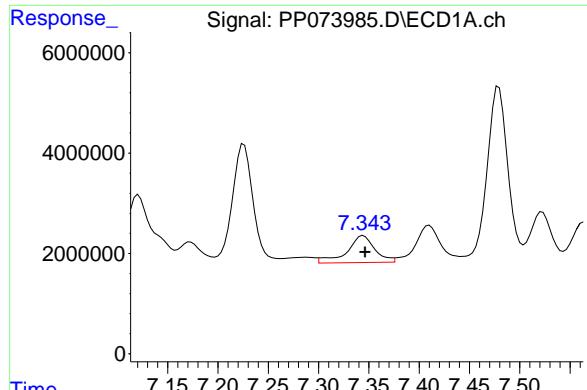

#29 AR-1254-4


R.T.: 7.344 min
 Delta R.T.: -0.002 min
 Response: 10348921
 Conc: 131.55 ng/ml

Instrument: ECD_P
 ClientSampleId: RT2286MSD

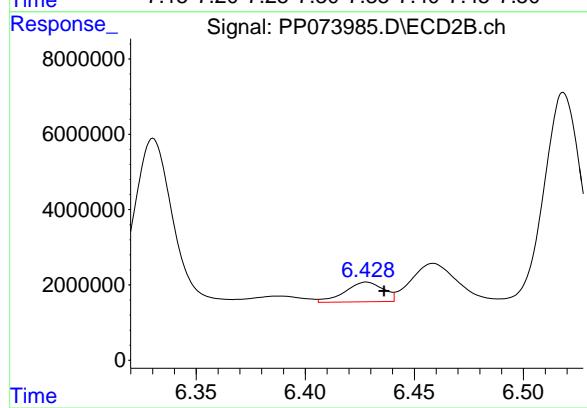


#29 AR-1254-4

R.T.: 6.428 min
 Delta R.T.: -0.008 min
 Response: 6367228
 Conc: 67.34 ng/ml

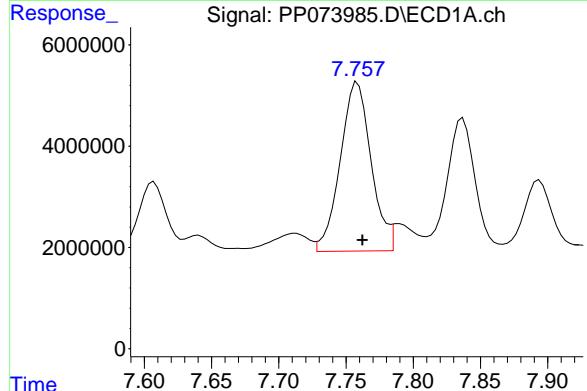


#30 AR-1254-5

R.T.: 7.759 min
 Delta R.T.: -0.004 min
 Response: 53191433
 Conc: 721.93 ng/ml

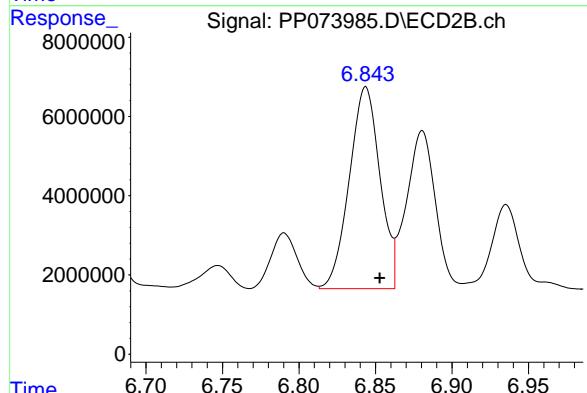

#30 AR-1254-5

R.T.: 6.844 min
 Delta R.T.: -0.009 min
 Response: 71090554
 Conc: 532.73 ng/ml

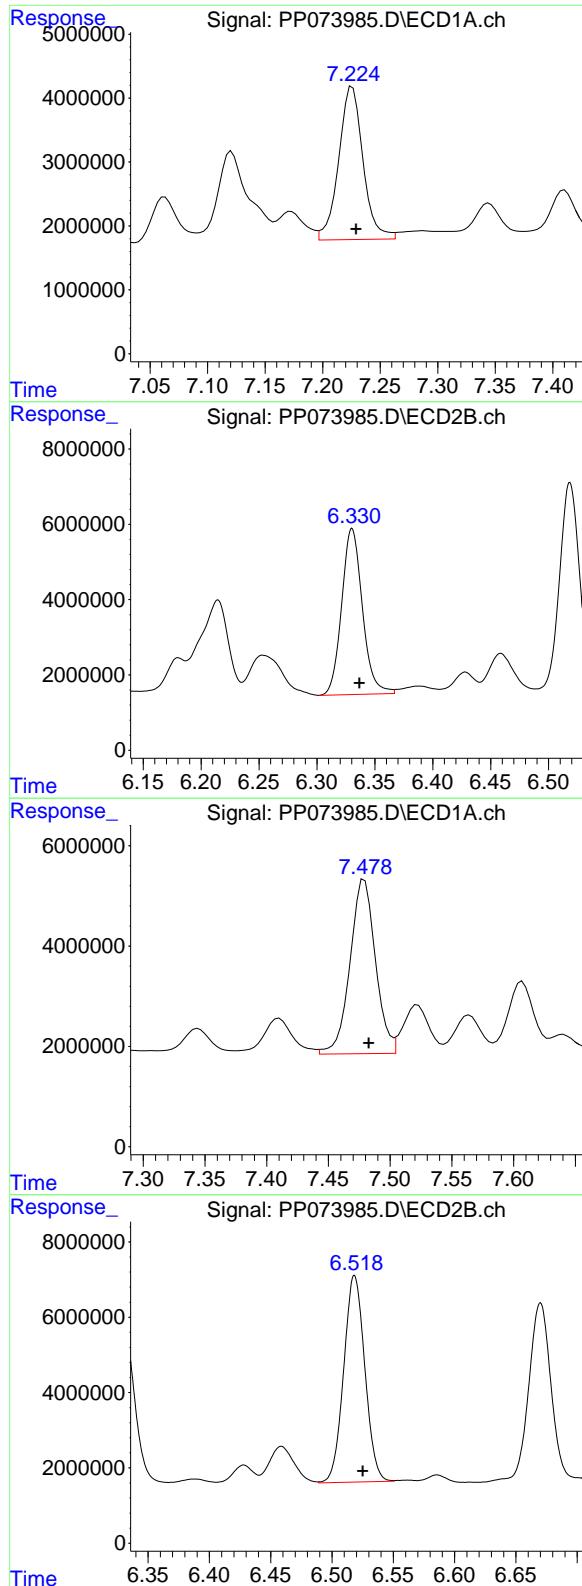

#31 AR-1260-1

R.T.: 7.226 min
 Delta R.T.: -0.003 min
 Response: 35309050
 Conc: 598.85 ng/ml

Instrument: ECD_P
 ClientSampleId: RT2286MSD

#31 AR-1260-1


R.T.: 6.330 min
 Delta R.T.: -0.006 min
 Response: 54851085
 Conc: 562.23 ng/ml

#32 AR-1260-2

R.T.: 7.479 min
 Delta R.T.: -0.004 min
 Response: 49841976
 Conc: 520.05 ng/ml

#32 AR-1260-2

R.T.: 6.518 min
 Delta R.T.: -0.007 min
 Response: 65815583
 Conc: 535.79 ng/ml

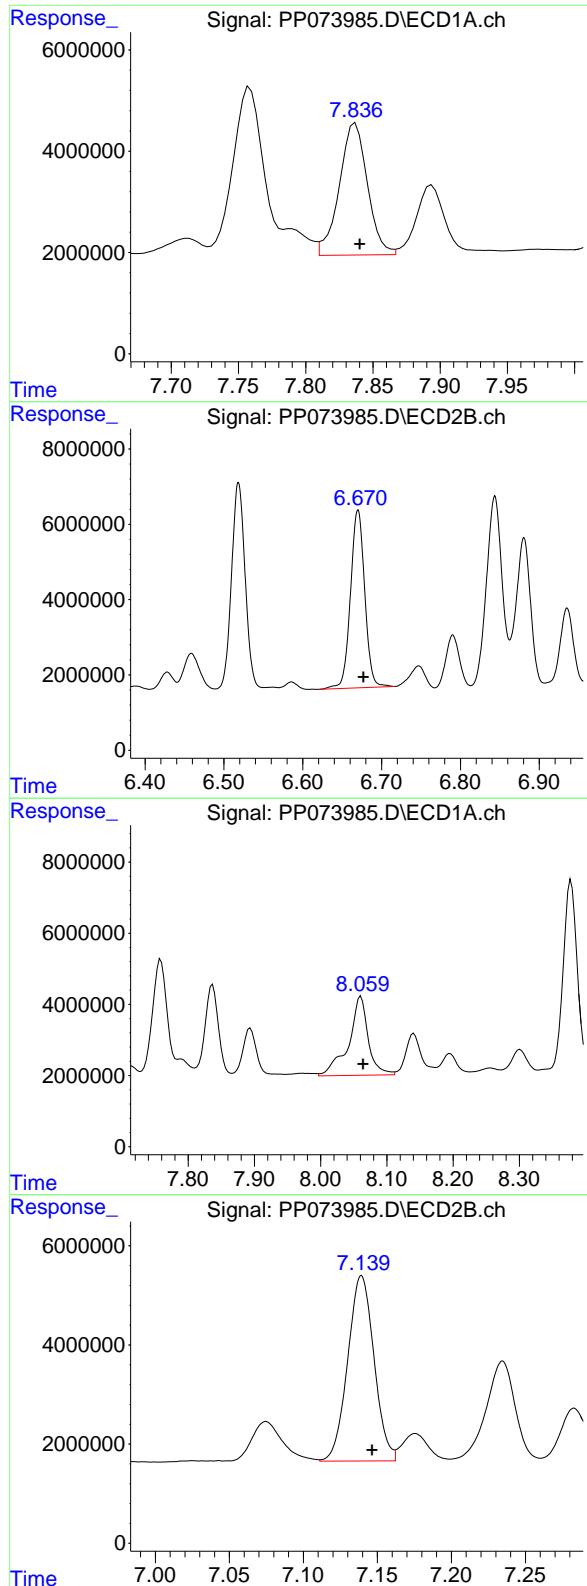

#33 AR-1260-3

R.T.: 7.837 min
 Delta R.T.: -0.003 min
 Response: 37810191
 Conc: 517.45 ng/ml

Instrument: ECD_P
 ClientSampleId: RT2286MSD

#33 AR-1260-3


R.T.: 6.670 min
 Delta R.T.: -0.007 min
 Response: 59476912
 Conc: 543.35 ng/ml

#34 AR-1260-4

R.T.: 8.061 min
 Delta R.T.: -0.004 min
 Response: 45575779
 Conc: 697.95 ng/ml

#34 AR-1260-4

R.T.: 7.139 min
 Delta R.T.: -0.007 min
 Response: 46277558
 Conc: 517.60 ng/ml

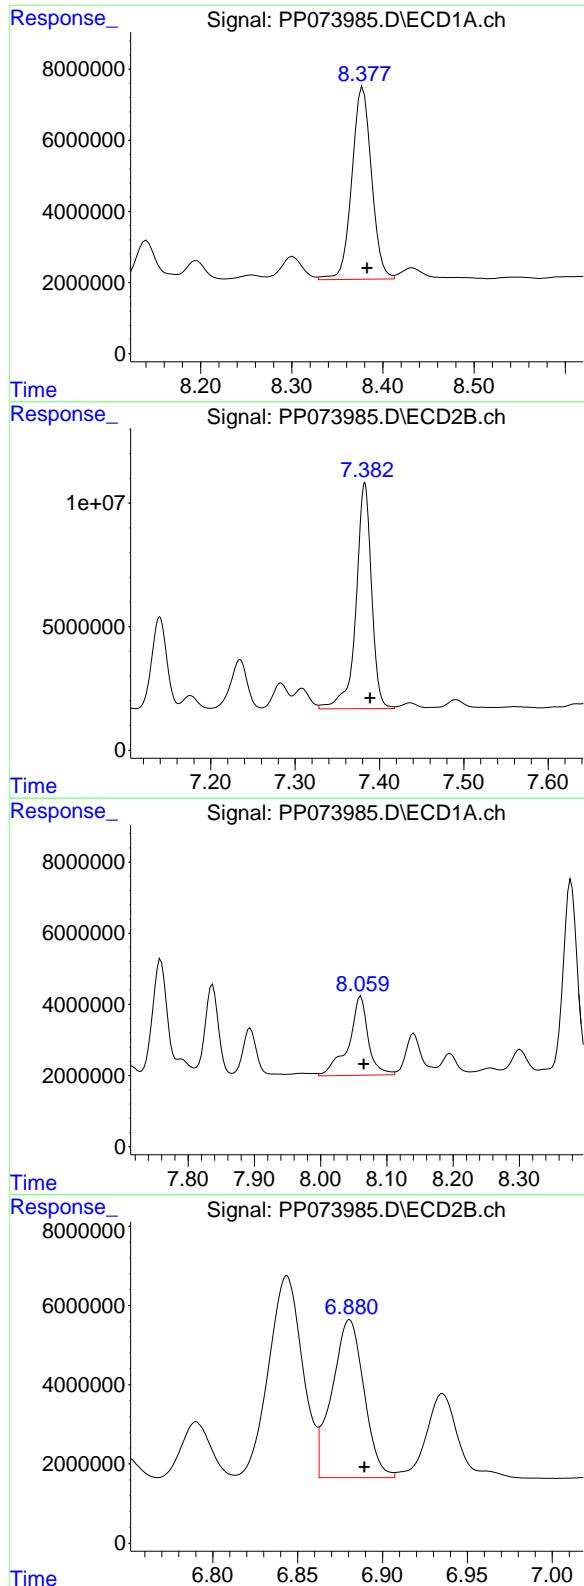

#35 AR-1260-5

R.T.: 8.378 min
 Delta R.T.: -0.005 min
 Response: 80997949
 Conc: 536.93 ng/ml

Instrument: ECD_P
 ClientSampleId: RT2286MSD

#35 AR-1260-5


R.T.: 7.383 min
 Delta R.T.: -0.006 min
 Response: 116992994
 Conc: 520.58 ng/ml

#36 AR-1262-1

R.T.: 8.061 min
 Delta R.T.: -0.004 min
 Response: 45575779
 Conc: 523.70 ng/ml

#36 AR-1262-1


R.T.: 6.881 min
 Delta R.T.: -0.009 min
 Response: 52214863
 Conc: 353.54 ng/ml



#37 AR-1262-2


R.T.: 8.378 min
 Delta R.T.: -0.005 min
 Response: 80997949
 Conc: 409.02 ng/ml

Instrument: ECD_P
 ClientSampleId: RT2286MSD

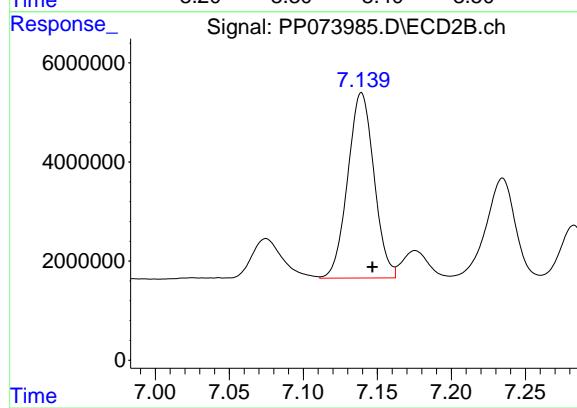


#37 AR-1262-2

R.T.: 7.139 min
 Delta R.T.: -0.007 min
 Response: 46277558
 Conc: 362.03 ng/ml




#38 AR-1262-3

R.T.: 8.700 min
 Delta R.T.: 0.003 min
 Response: 47490444
 Conc: 377.73 ng/ml

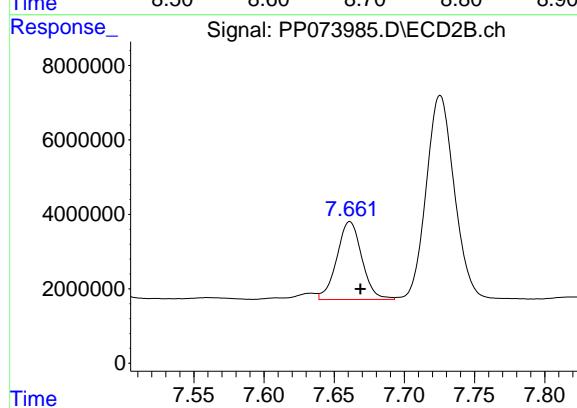

#38 AR-1262-3


R.T.: 7.661 min
 Delta R.T.: -0.008 min
 Response: 26041835
 Conc: 228.40 ng/ml

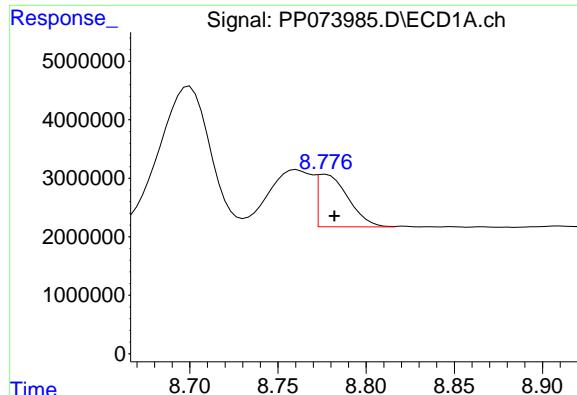

#39 AR-1262-4


R.T.: 8.777 min
 Delta R.T.: -0.005 min
 Response: 10905481
 Conc: 116.93 ng/ml

Instrument: ECD_P
 ClientSampleId: RT2286MSD

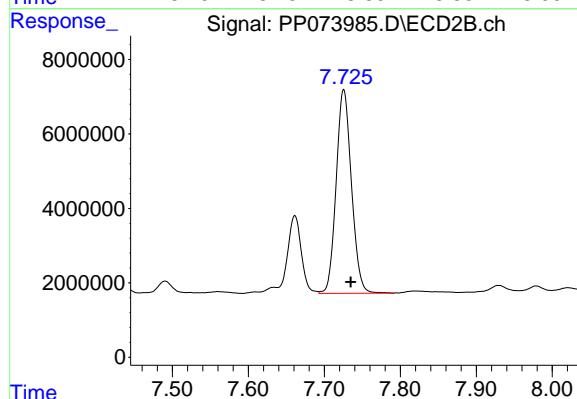


#39 AR-1262-4

R.T.: 7.726 min
 Delta R.T.: -0.009 min
 Response: 76651297
 Conc: 416.47 ng/ml

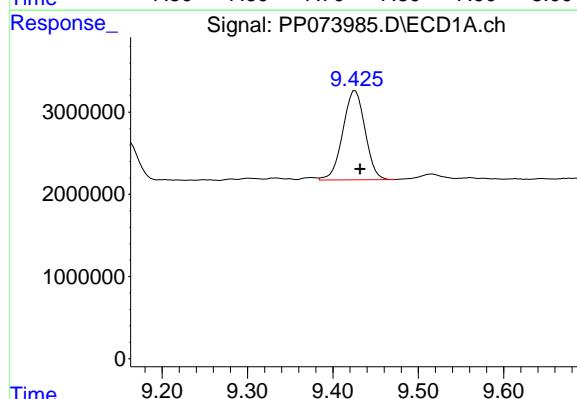


#40 AR-1262-5

R.T.: 9.426 min
 Delta R.T.: -0.005 min
 Response: 19633340
 Conc: 309.73 ng/ml

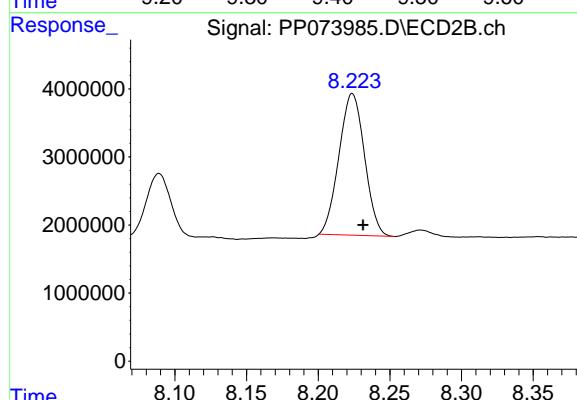

#40 AR-1262-5

R.T.: 8.224 min
 Delta R.T.: -0.008 min
 Response: 25848025
 Conc: 306.13 ng/ml

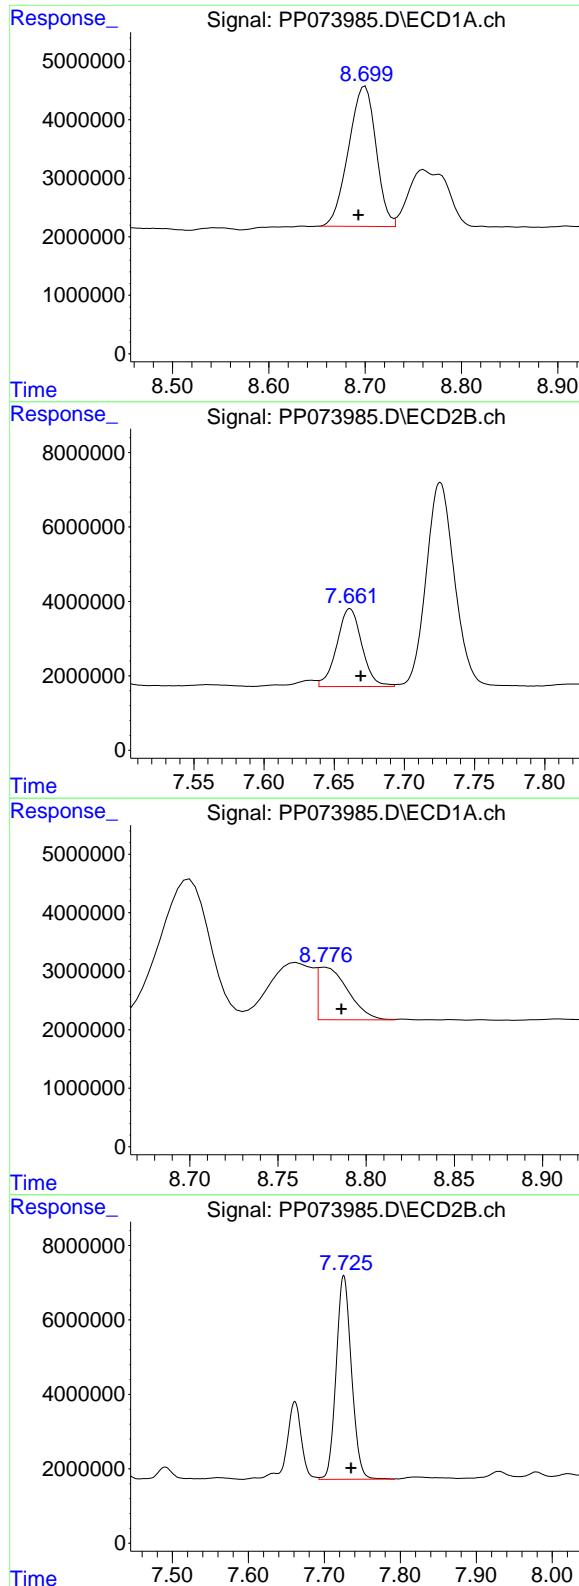

#41 AR-1268-1

R.T.: 8.700 min
 Delta R.T.: 0.007 min
 Response: 47490444
 Conc: 212.75 ng/ml

Instrument: ECD_P
 ClientSampleId: RT2286MSD

#41 AR-1268-1


R.T.: 7.661 min
 Delta R.T.: -0.008 min
 Response: 26041835
 Conc: 84.72 ng/ml

#42 AR-1268-2

R.T.: 8.777 min
 Delta R.T.: -0.009 min
 Response: 10905481
 Conc: 57.25 ng/ml

#42 AR-1268-2


R.T.: 7.726 min
 Delta R.T.: -0.010 min
 Response: 76651297
 Conc: 288.50 ng/ml

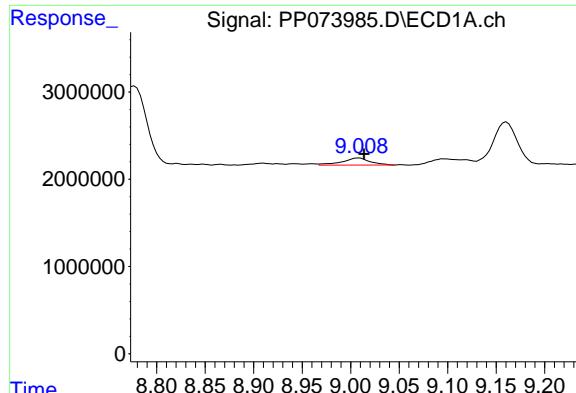

#43 AR-1268-3


R.T.: 9.009 min
Delta R.T.: -0.005 min
Response: 1635702
Conc: 9.88 ng/ml

Instrument: ECD_P
ClientSampleId: RT2286MSD

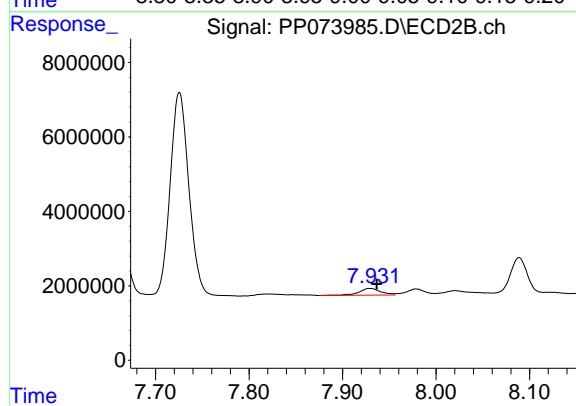


#43 AR-1268-3

R.T.: 7.930 min
Delta R.T.: -0.007 min
Response: 2877785
Conc: 12.76 ng/ml

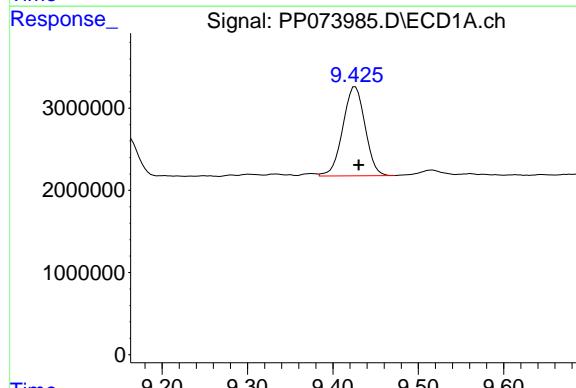


#44 AR-1268-4

R.T.: 9.426 min
Delta R.T.: -0.004 min
Response: 19633340
Conc: 282.32 ng/ml

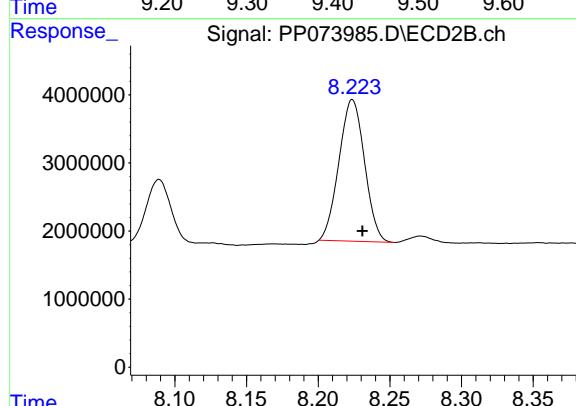

#44 AR-1268-4

R.T.: 8.224 min
Delta R.T.: -0.007 min
Response: 25848025
Conc: 278.03 ng/ml

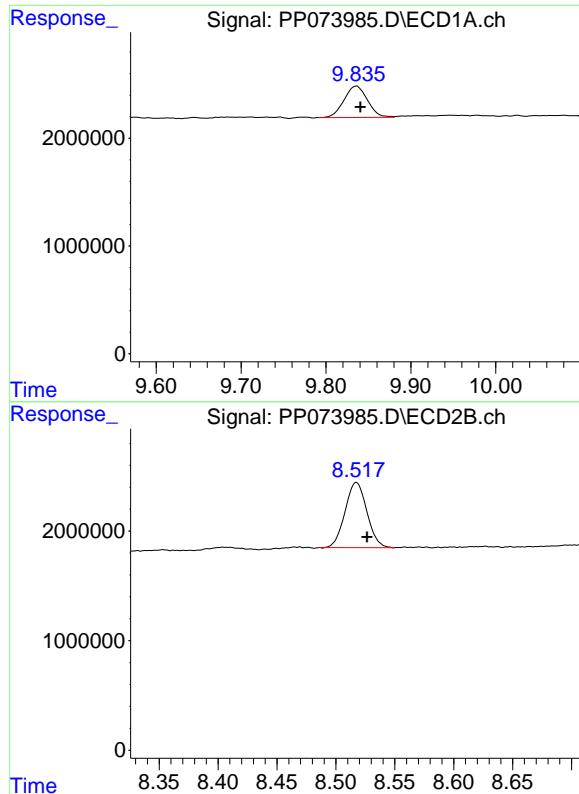

#45 AR-1268-5

R.T.: 9.836 min
Delta R.T.: -0.004 min
Response: 5572340
Conc: 12.09 ng/ml

Instrument: ECD_P
ClientSampleId: RT2286MSD

#45 AR-1268-5

R.T.: 8.517 min
Delta R.T.: -0.009 min
Response: 7686741
Conc: 12.47 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP072125\
 Data File : PP074001.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jul 2025 19:07
 Operator : YP\AJ
 Sample : Q2639-01
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
OU4-TS-38-071725

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 22 02:15:21 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 08 08:35:32 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	4.482	3.773	20953277	30094893	15.300	16.336
2) SA Decachlor...	10.165	8.770	12316627	16836055	11.289	12.724

Target Compounds

3) L1 AR-1016-1	5.657	4.855	880393	562669	18.529	8.253 #
4) L1 AR-1016-2	5.657	4.867	880393	315522	12.362	3.097 #
5) L1 AR-1016-3	5.731	5.048	188431	779812	4.316	14.413 #
6) L1 AR-1016-4	5.796	5.086	1186711	2306867	33.014	52.571 #
7) L1 AR-1016-5	6.108	5.298	264863	1381588	8.454	25.312 #
8) L2 AR-1221-1	4.685	3.987	302982	51842	16.958	1.917 #
9) L2 AR-1221-2	4.782	4.075	328332	1204131	24.313	59.141 #
10) L2 AR-1221-3	4.864	4.143	2512130	3000814	60.381	48.835
11) L3 AR-1232-1	4.864	4.143	2512130	3000814	76.940	64.375
12) L3 AR-1232-2	5.351	4.867	2789095	315522	171.587	6.620 #
13) L3 AR-1232-3	5.657	5.048	880393	779812	26.684	31.156
14) L3 AR-1232-4	5.796	5.130	1186711	828082	72.162	38.237 #
15) L3 AR-1232-5	5.906	5.298	639242	1381588	60.475	61.231
16) L4 AR-1242-1	5.657	4.855	880393	562669	23.054	9.741 #
17) L4 AR-1242-2	5.657	4.867	880393	315522	14.702	3.650 #
18) L4 AR-1242-3	5.731	5.048	188431	779812	5.145	16.972 #
19) L4 AR-1242-4	5.796	5.130	1186711	828082	36.928	18.708 #
20) L4 AR-1242-5	6.547	5.651	2626686	5699832	80.236	103.178 #
21) L5 AR-1248-1	5.657	4.855	880393	562669	28.519	12.533 #
22) L5 AR-1248-2	5.906	5.086	639242	2306867	16.012	37.488 #
23) L5 AR-1248-3	6.108	5.130	264863	828082	5.964	12.926 #
24) L5 AR-1248-4	6.504	5.298	1403645	1381588	25.484	18.329 #
25) L5 AR-1248-5	6.547	5.691	2626686	2191923	48.832	29.386 #
26) L6 AR-1254-1	6.480	5.651	2283377	5699832	42.609	49.124
27) L6 AR-1254-2	6.701	5.799	4334234	3836337	52.039	38.126 #
28) L6 AR-1254-3	7.067	6.214	7845977	15063536	88.824	97.532
29) L6 AR-1254-4	7.341	6.428	1959487	1886359	24.909	19.949
30) L6 AR-1254-5	7.776	6.840	11486495	20407242	155.897	152.926
31) L7 AR-1260-1	7.221	6.330	2823933	4466526	47.895	45.782
32) L7 AR-1260-2	7.465	6.519	10469388	2773734	109.238	22.581 #
33) L7 AR-1260-3	7.836	6.669	907435	2209772	12.419	20.187 #
34) L7 AR-1260-4	8.049	7.137	3898789	1387004	59.706	15.513 #
35) L7 AR-1260-5	8.375	7.380	2514577	3370940	16.669	15.000
36) L8 AR-1262-1	8.049	6.877	3898789	847997	44.800	5.742 #
37) L8 AR-1262-2	8.375	7.137	2514577	1387004	12.698	10.850
38) L8 AR-1262-3	8.687	7.659	710351	2301706	5.650	20.187 #
39) L8 AR-1262-4	8.777	7.725	489718	2093441	5.251	11.374 #
40) L8 AR-1262-5	9.422	8.221	891155	433627	14.058	5.136 #
41) L9 AR-1268-1	8.687	7.659	710351	2301706	3.182	7.488 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP072125\
 Data File : PP074001.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jul 2025 19:07
 Operator : YP\AJ
 Sample : Q2639-01
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
OU4-TS-38-071725

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 22 02:15:21 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 08 08:35:32 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9 AR-1268-2	8.777	7.725	489718	2093441	2.571	7.879 #
43) L9 AR-1268-3	8.969f	7.920	324985	2205194	1.963	9.776 #
44) L9 AR-1268-4	9.422	8.221	891155	433627	12.814	4.664 #
45) L9 AR-1268-5	9.844	8.513	187351	406224	0.406	0.659 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP072125\
 Data File : PP074001.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jul 2025 19:07
 Operator : YP\AJ
 Sample : Q2639-01
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
OU4-TS-38-071725

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 22 02:15:21 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 08 08:35:32 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

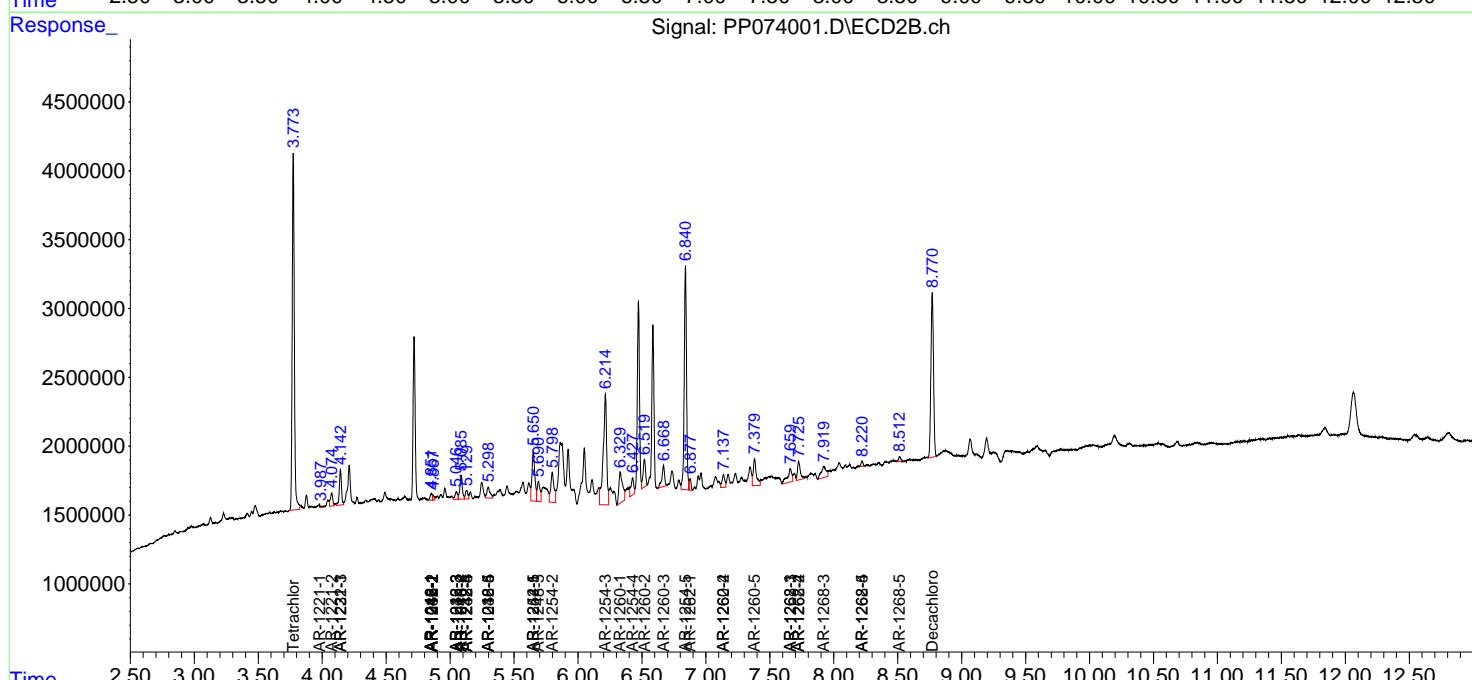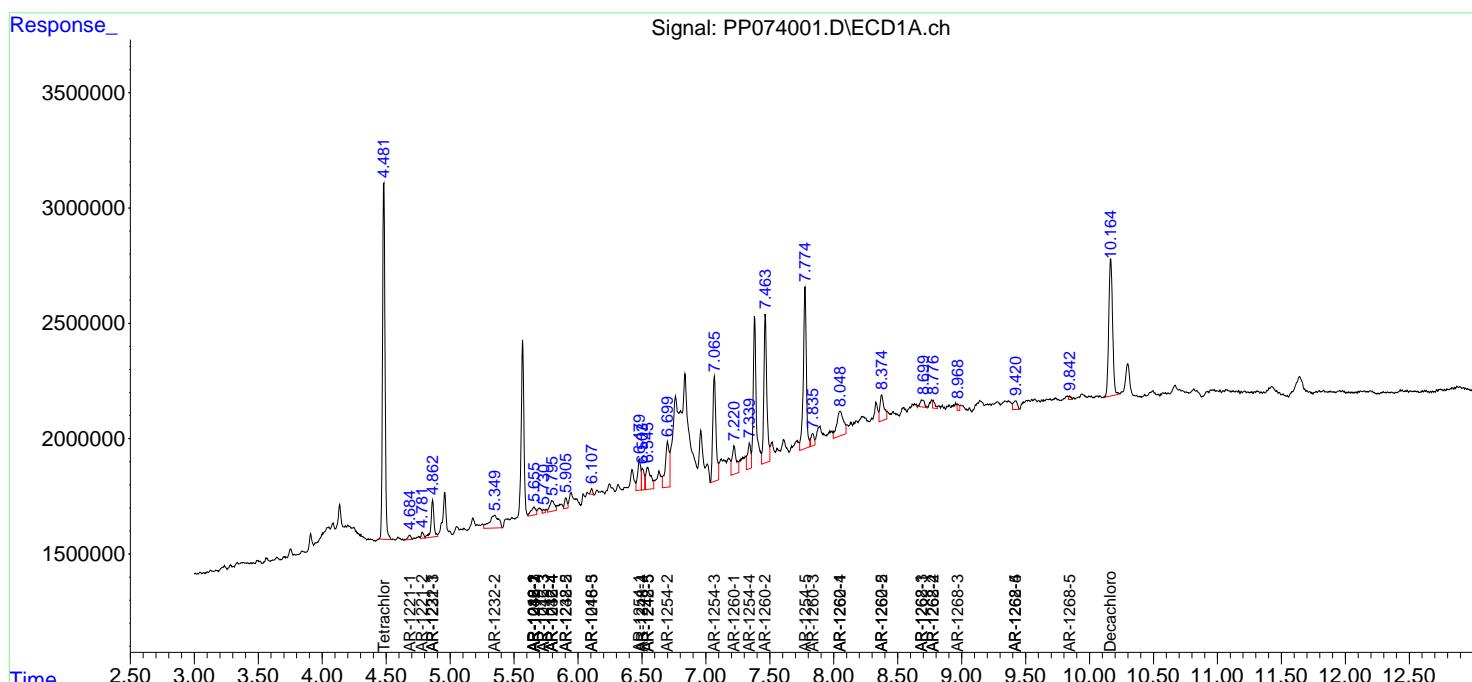

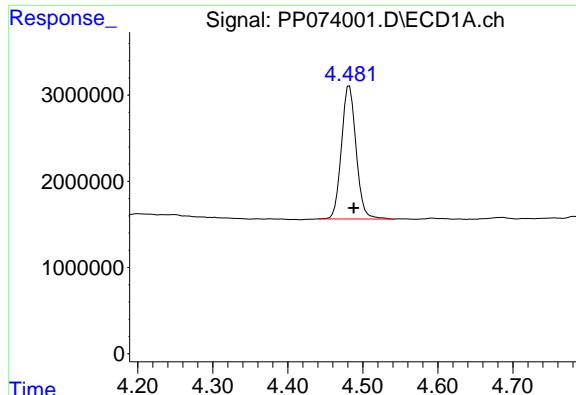

#1 Tetrachloro-m-xylene


R.T.: 4.482 min
Delta R.T.: -0.006 min
Response: 20953277
Conc: 15.30 ng/ml

Instrument:

ECD_P


ClientSampleId :

OU4-TS-38-071725

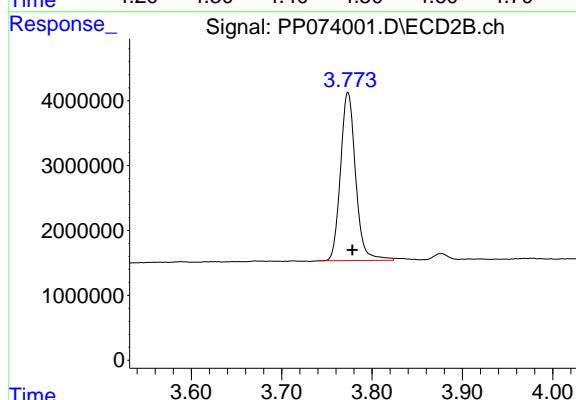


#1 Tetrachloro-m-xylene

R.T.: 3.773 min
Delta R.T.: -0.005 min
Response: 30094893
Conc: 16.34 ng/ml

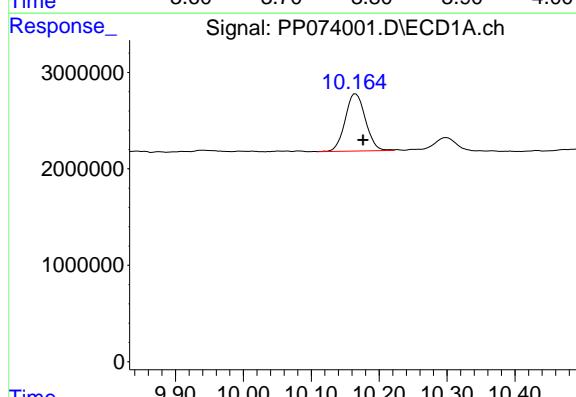


#2 Decachlorobiphenyl

R.T.: 10.165 min
Delta R.T.: -0.011 min
Response: 12316627
Conc: 11.29 ng/ml

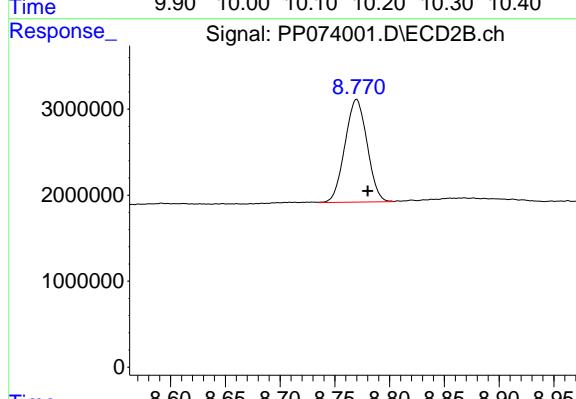

#2 Decachlorobiphenyl

R.T.: 8.770 min
Delta R.T.: -0.010 min
Response: 16836055
Conc: 12.72 ng/ml

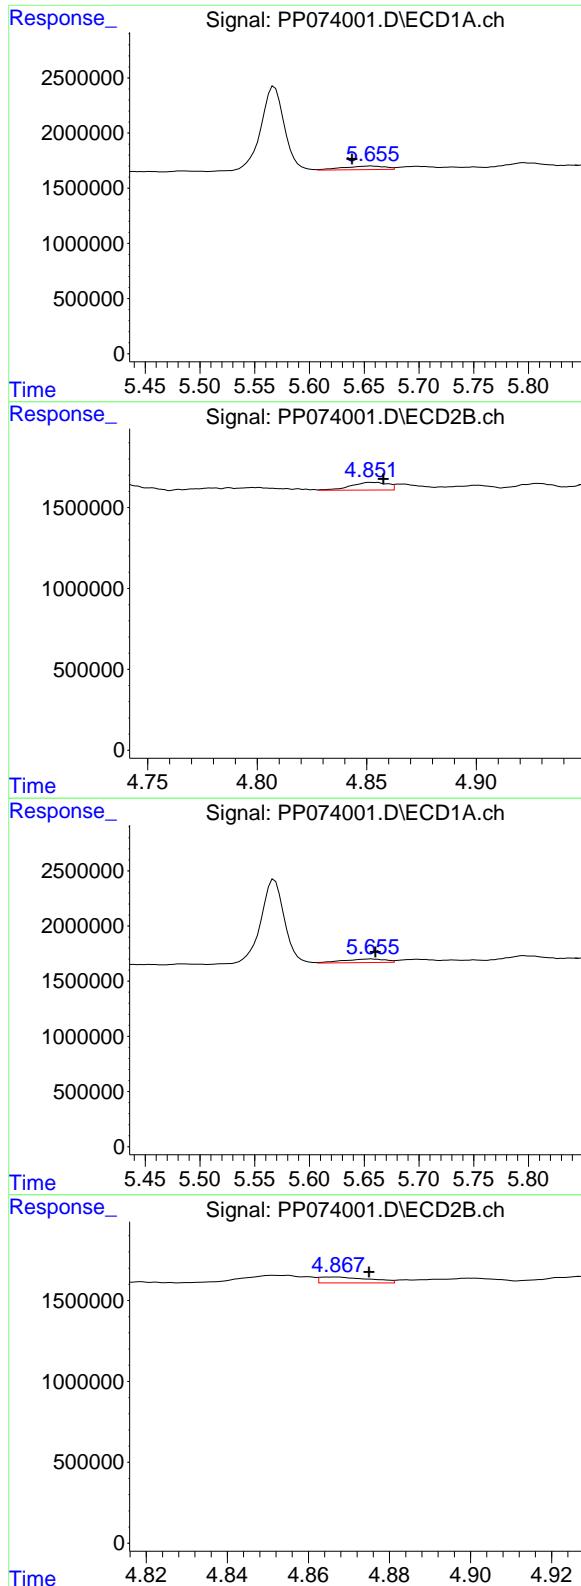

#3 AR-1016-1

R.T.: 5.657 min
 Delta R.T.: 0.018 min Instrument:
 Response: 880393 ECD_P
 Conc: 18.53 ng/ml ClientSampleId :
 OU4-TS-38-071725

#3 AR-1016-1


R.T.: 4.855 min
 Delta R.T.: -0.003 min
 Response: 562669
 Conc: 8.25 ng/ml

#4 AR-1016-2

R.T.: 5.657 min
 Delta R.T.: -0.004 min
 Response: 880393
 Conc: 12.36 ng/ml

#4 AR-1016-2

R.T.: 4.867 min
 Delta R.T.: -0.008 min
 Response: 315522
 Conc: 3.10 ng/ml

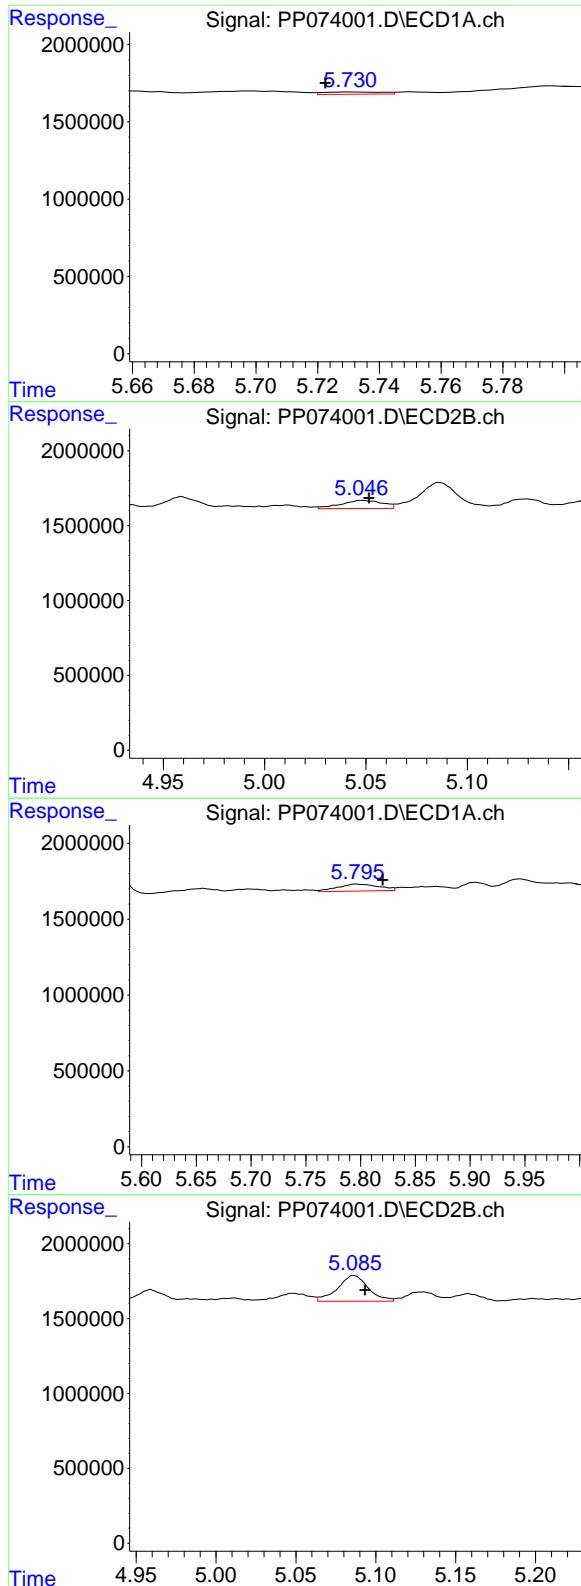

#5 AR-1016-3

R.T.: 5.731 min
 Delta R.T.: 0.009 min
 Response: 188431
 Conc: 4.32 ng/ml

Instrument: ECD_P
 ClientSampleId: OU4-TS-38-071725

#5 AR-1016-3


R.T.: 5.048 min
 Delta R.T.: -0.004 min
 Response: 779812
 Conc: 14.41 ng/ml

#6 AR-1016-4

R.T.: 5.796 min
 Delta R.T.: -0.024 min
 Response: 1186711
 Conc: 33.01 ng/ml

#6 AR-1016-4

R.T.: 5.086 min
 Delta R.T.: -0.007 min
 Response: 2306867
 Conc: 52.57 ng/ml

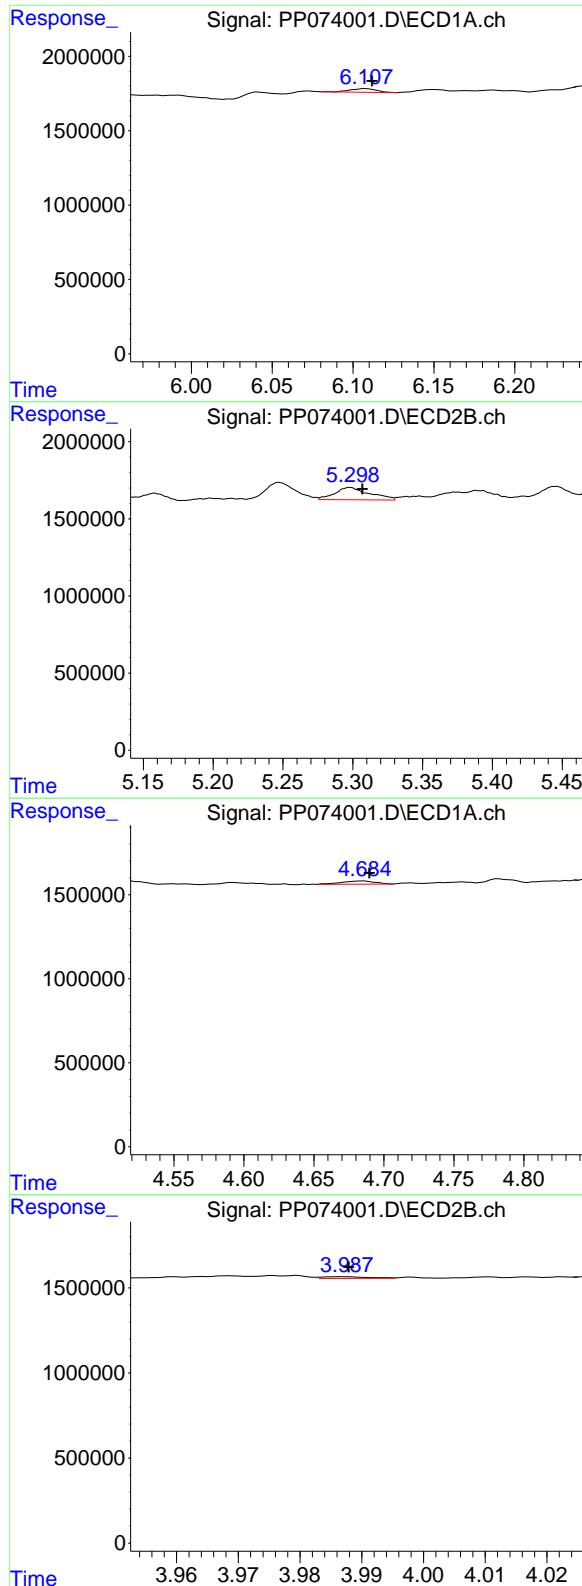

#7 AR-1016-5

R.T.: 6.108 min
 Delta R.T.: -0.004 min
 Response: 264863
 Conc: 8.45 ng/ml

Instrument: ECD_P
 ClientSampleId: OU4-TS-38-071725

#7 AR-1016-5


R.T.: 5.298 min
 Delta R.T.: -0.009 min
 Response: 1381588
 Conc: 25.31 ng/ml

#8 AR-1221-1

R.T.: 4.685 min
 Delta R.T.: -0.004 min
 Response: 302982
 Conc: 16.96 ng/ml

#8 AR-1221-1

R.T.: 3.987 min
 Delta R.T.: 0.000 min
 Response: 51842
 Conc: 1.92 ng/ml

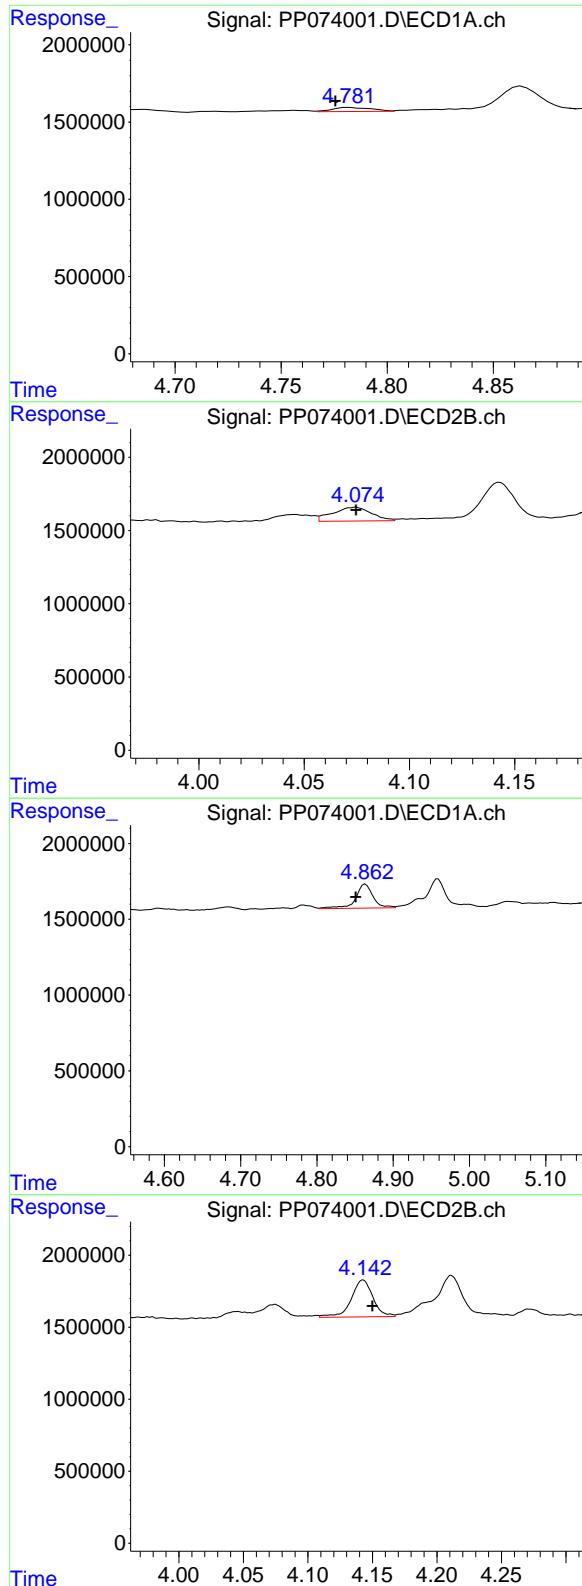

#9 AR-1221-2

R.T.: 4.782 min
 Delta R.T.: 0.007 min **Instrument:**
 Response: 328332 ECD_P
 Conc: 24.31 ng/ml **ClientSampleId:**
 OU4-TS-38-071725

#9 AR-1221-2


R.T.: 4.075 min
 Delta R.T.: 0.000 min
 Response: 1204131
 Conc: 59.14 ng/ml

#10 AR-1221-3

R.T.: 4.864 min
 Delta R.T.: 0.013 min
 Response: 2512130
 Conc: 60.38 ng/ml

#10 AR-1221-3


R.T.: 4.143 min
 Delta R.T.: -0.007 min
 Response: 3000814
 Conc: 48.83 ng/ml

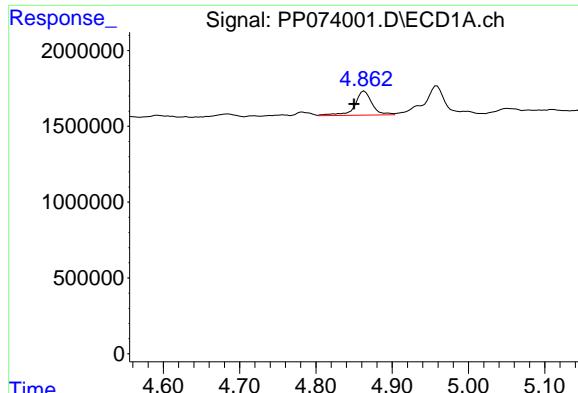

#11 AR-1232-1


R.T.: 4.864 min
Delta R.T.: 0.013 min
Response: 2512130
Conc: 76.94 ng/ml

Instrument: ECD_P
ClientSampleId: OU4-TS-38-071725

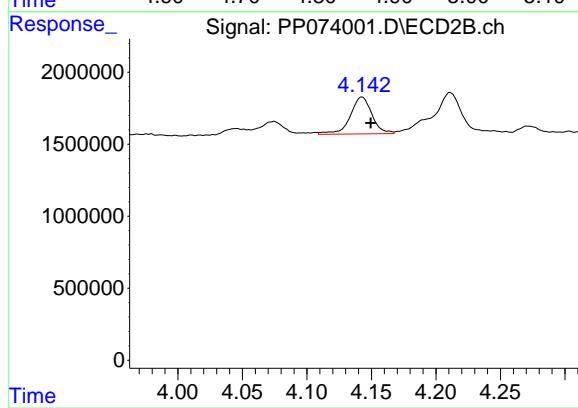


#11 AR-1232-1

R.T.: 4.143 min
Delta R.T.: -0.007 min
Response: 3000814
Conc: 64.38 ng/ml

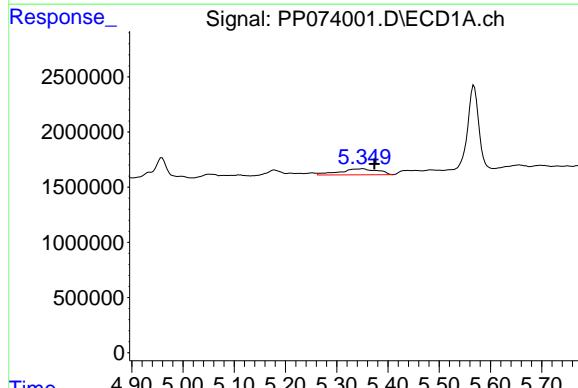


#12 AR-1232-2

R.T.: 5.351 min
Delta R.T.: -0.023 min
Response: 2789095
Conc: 171.59 ng/ml

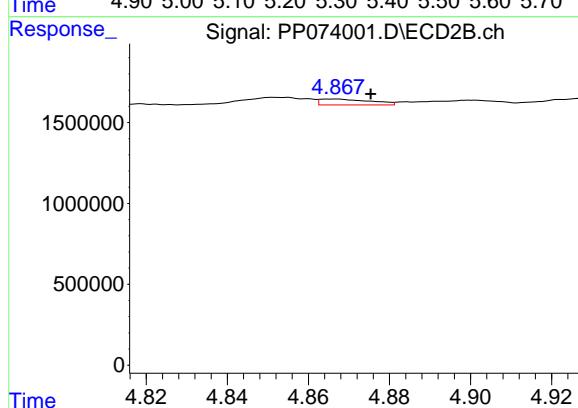

#12 AR-1232-2

R.T.: 4.867 min
Delta R.T.: -0.008 min
Response: 315522
Conc: 6.62 ng/ml

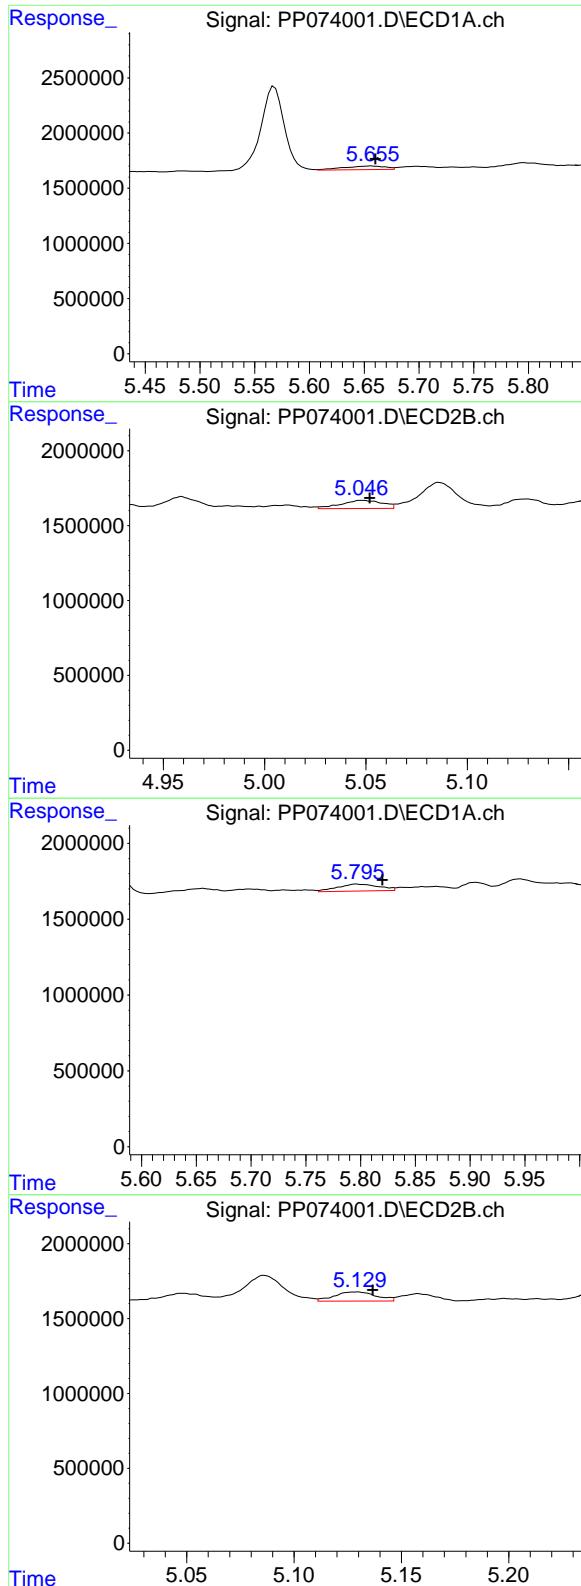

#13 AR-1232-3

R.T.: 5.657 min
 Delta R.T.: -0.003 min
 Response: 880393
 Conc: 26.68 ng/ml

Instrument: ECD_P
 ClientSampleId: OU4-TS-38-071725

#13 AR-1232-3


R.T.: 5.048 min
 Delta R.T.: -0.004 min
 Response: 779812
 Conc: 31.16 ng/ml

#14 AR-1232-4

R.T.: 5.796 min
 Delta R.T.: -0.024 min
 Response: 1186711
 Conc: 72.16 ng/ml

#14 AR-1232-4

R.T.: 5.130 min
 Delta R.T.: -0.007 min
 Response: 828082
 Conc: 38.24 ng/ml

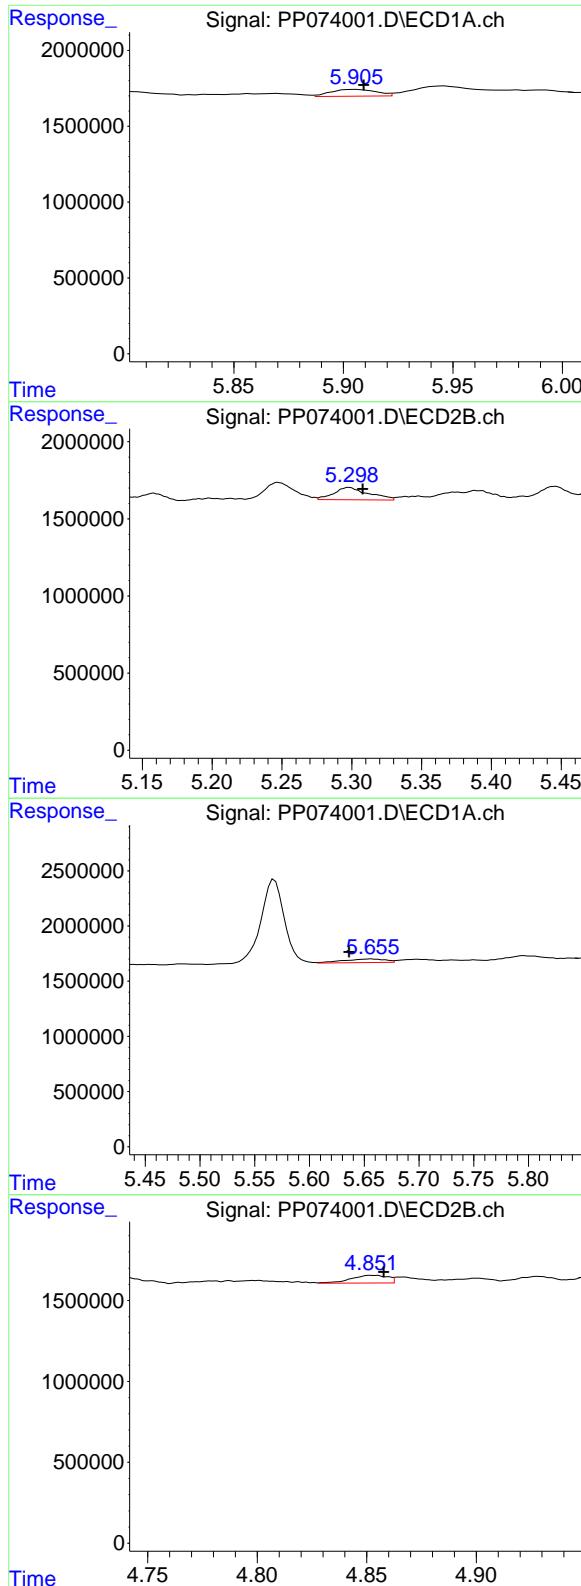

#15 AR-1232-5

R.T.: 5.906 min
 Delta R.T.: -0.003 min
 Response: 639242
 Conc: 60.47 ng/ml

Instrument: ECD_P
 ClientSampleId : OU4-TS-38-071725

#15 AR-1232-5


R.T.: 5.298 min
 Delta R.T.: -0.010 min
 Response: 1381588
 Conc: 61.23 ng/ml

#16 AR-1242-1

R.T.: 5.657 min
 Delta R.T.: 0.021 min
 Response: 880393
 Conc: 23.05 ng/ml

#16 AR-1242-1

R.T.: 4.855 min
 Delta R.T.: -0.003 min
 Response: 562669
 Conc: 9.74 ng/ml

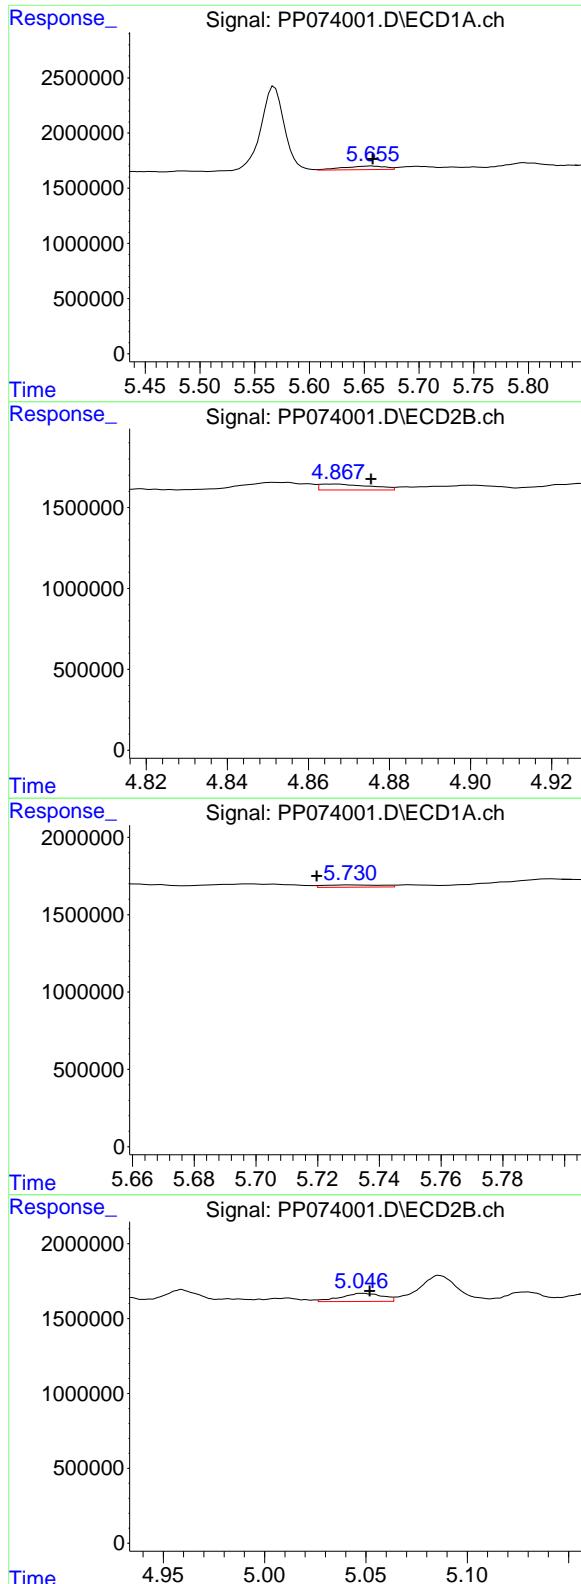

#17 AR-1242-2

R.T.: 5.657 min
 Delta R.T.: 0.000 min **Instrument:**
 Response: 880393 ECD_P
 Conc: 14.70 ng/ml **ClientSampleId:**
 OU4-TS-38-071725

#17 AR-1242-2


R.T.: 4.867 min
 Delta R.T.: -0.009 min
 Response: 315522
 Conc: 3.65 ng/ml

#18 AR-1242-3

R.T.: 5.731 min
 Delta R.T.: 0.011 min
 Response: 188431
 Conc: 5.15 ng/ml

#18 AR-1242-3

R.T.: 5.048 min
 Delta R.T.: -0.004 min
 Response: 779812
 Conc: 16.97 ng/ml

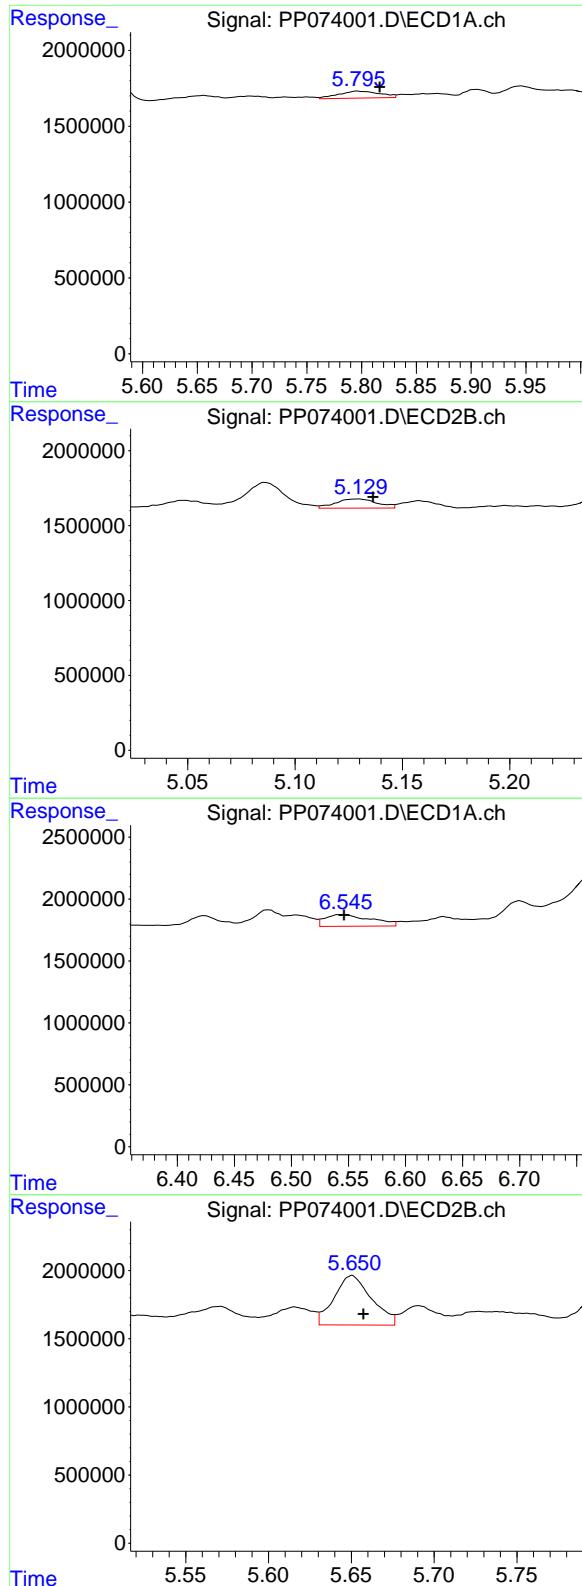

#19 AR-1242-4

R.T.: 5.796 min
 Delta R.T.: -0.020 min Instrument:
 Response: 1186711 ECD_P
 Conc: 36.93 ng/ml ClientSampleId :
 OU4-TS-38-071725

#19 AR-1242-4


R.T.: 5.130 min
 Delta R.T.: -0.007 min
 Response: 828082
 Conc: 18.71 ng/ml

#20 AR-1242-5

R.T.: 6.547 min
 Delta R.T.: 0.000 min
 Response: 2626686
 Conc: 80.24 ng/ml

#20 AR-1242-5

R.T.: 5.651 min
 Delta R.T.: -0.007 min
 Response: 5699832
 Conc: 103.18 ng/ml

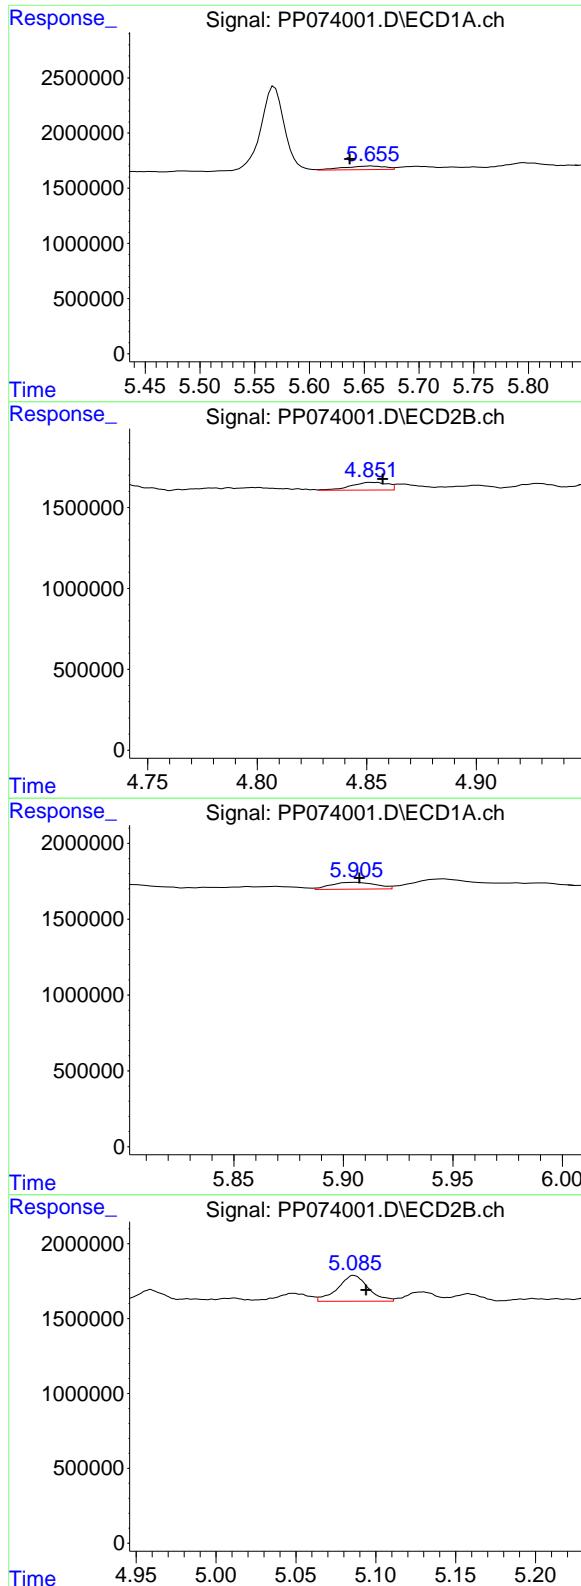

#21 AR-1248-1

R.T.: 5.657 min
 Delta R.T.: 0.020 min
 Response: 880393
 Conc: 28.52 ng/ml

Instrument: ECD_P
 ClientSampleId: OU4-TS-38-071725

#21 AR-1248-1


R.T.: 4.855 min
 Delta R.T.: -0.003 min
 Response: 562669
 Conc: 12.53 ng/ml

#22 AR-1248-2

R.T.: 5.906 min
 Delta R.T.: -0.001 min
 Response: 639242
 Conc: 16.01 ng/ml

#22 AR-1248-2


R.T.: 5.086 min
 Delta R.T.: -0.008 min
 Response: 2306867
 Conc: 37.49 ng/ml

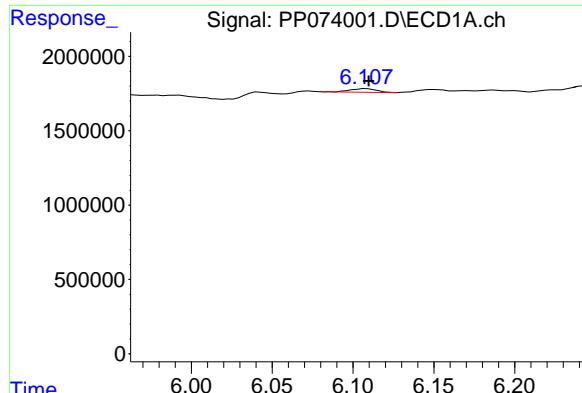

#23 AR-1248-3


R.T.: 6.108 min
Delta R.T.: -0.001 min
Response: 264863
Conc: 5.96 ng/ml

Instrument: ECD_P
ClientSampleId: OU4-TS-38-071725

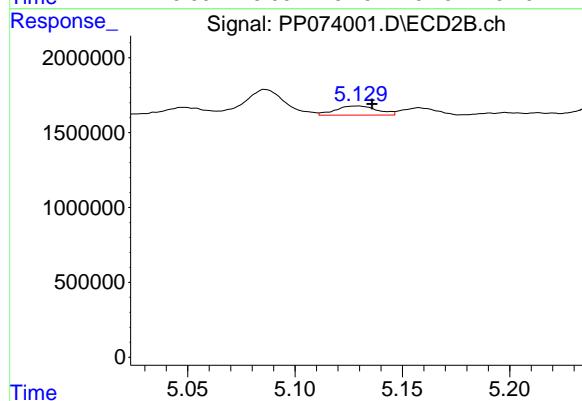


#23 AR-1248-3

R.T.: 5.130 min
Delta R.T.: -0.006 min
Response: 828082
Conc: 12.93 ng/ml

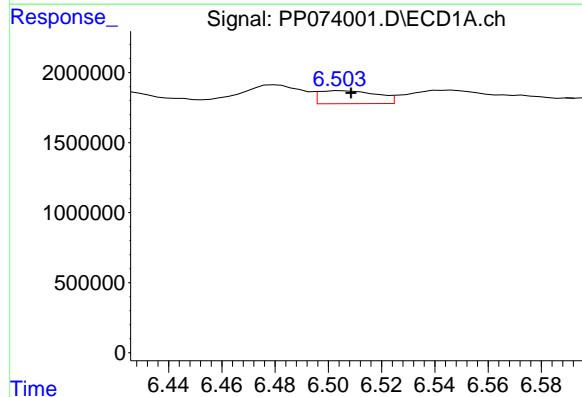


#24 AR-1248-4

R.T.: 6.504 min
Delta R.T.: -0.004 min
Response: 1403645
Conc: 25.48 ng/ml

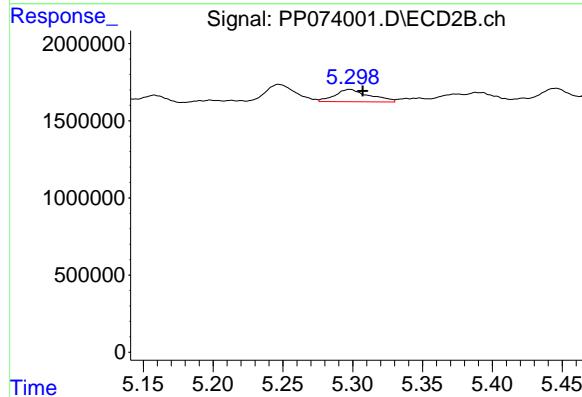

#24 AR-1248-4

R.T.: 5.298 min
Delta R.T.: -0.009 min
Response: 1381588
Conc: 18.33 ng/ml

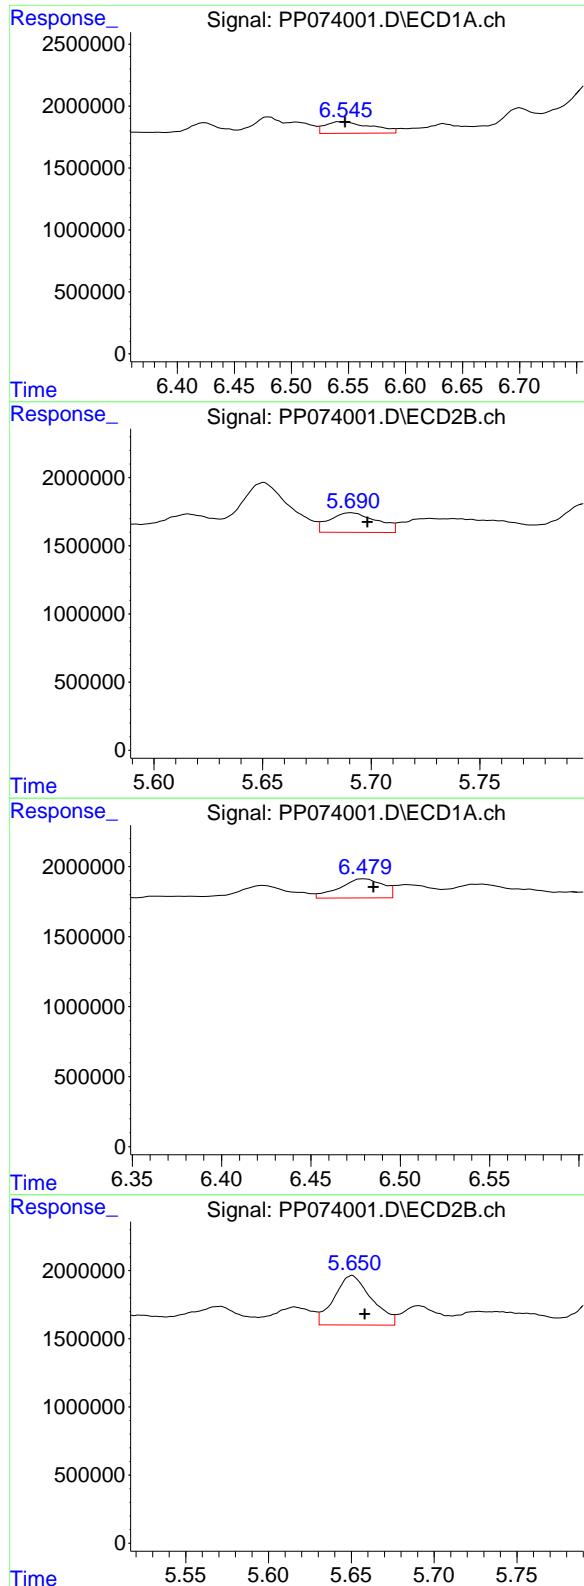

#25 AR-1248-5

R.T.: 6.547 min
 Delta R.T.: 0.000 min
 Response: 2626686
 Conc: 48.83 ng/ml

Instrument: ECD_P
 ClientSampleId: OU4-TS-38-071725

#25 AR-1248-5


R.T.: 5.691 min
 Delta R.T.: -0.008 min
 Response: 2191923
 Conc: 29.39 ng/ml

#26 AR-1254-1

R.T.: 6.480 min
 Delta R.T.: -0.005 min
 Response: 2283377
 Conc: 42.61 ng/ml

#26 AR-1254-1

R.T.: 5.651 min
 Delta R.T.: -0.008 min
 Response: 5699832
 Conc: 49.12 ng/ml

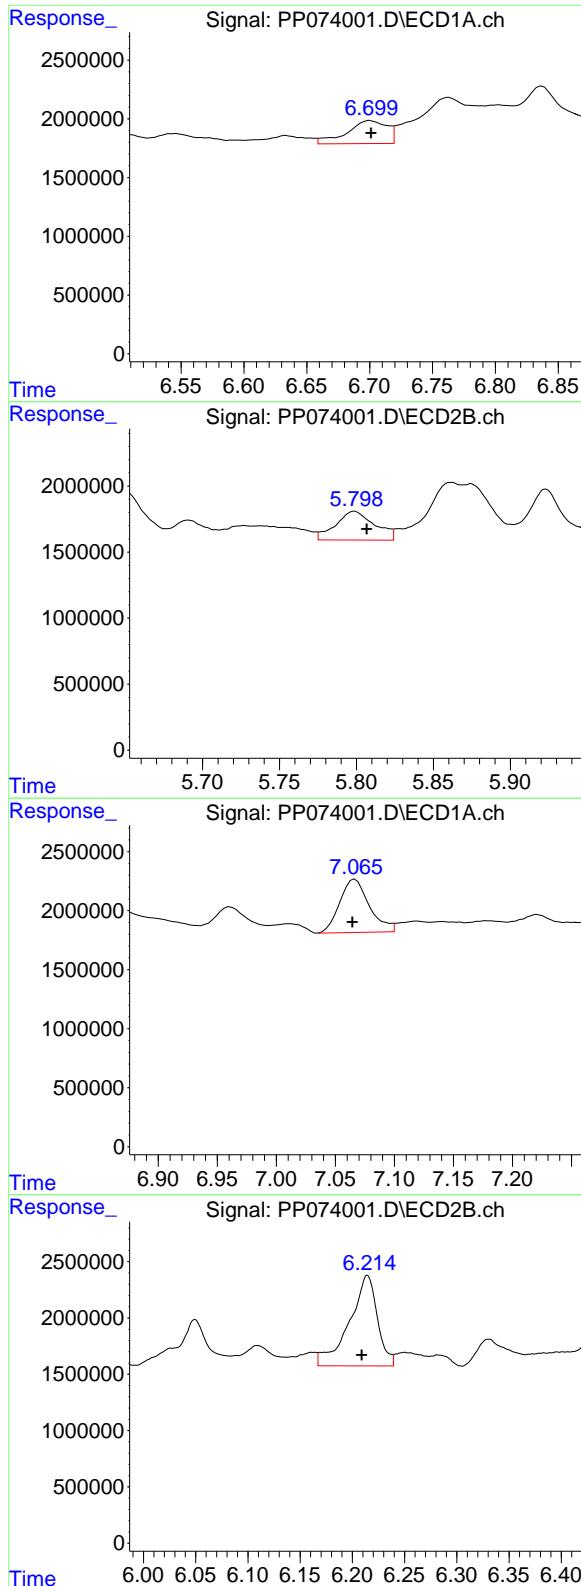

#27 AR-1254-2

R.T.: 6.701 min
 Delta R.T.: 0.000 min **Instrument:**
 Response: 4334234 ECD_P
 Conc: 52.04 ng/ml **ClientSampleId:**
 OU4-TS-38-071725

#27 AR-1254-2


R.T.: 5.799 min
 Delta R.T.: -0.008 min
 Response: 3836337
 Conc: 38.13 ng/ml

#28 AR-1254-3

R.T.: 7.067 min
 Delta R.T.: 0.002 min
 Response: 7845977
 Conc: 88.82 ng/ml

#28 AR-1254-3

R.T.: 6.214 min
 Delta R.T.: 0.005 min
 Response: 15063536
 Conc: 97.53 ng/ml

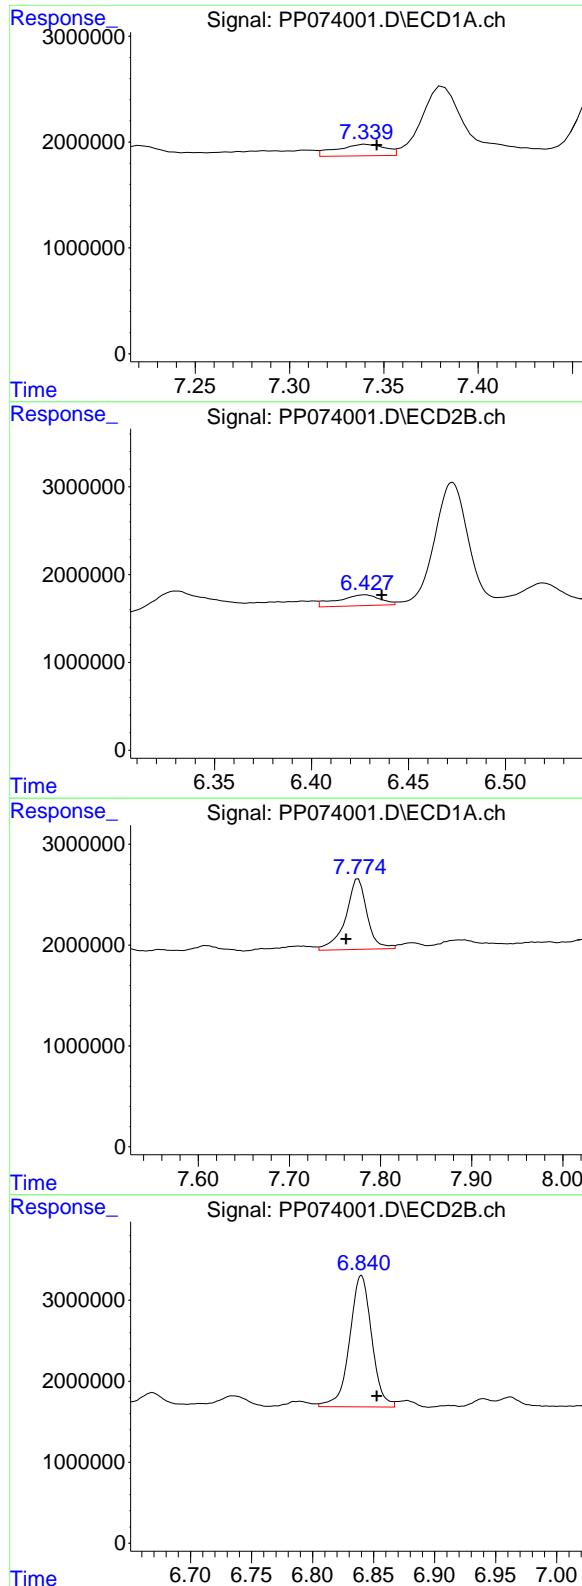

#29 AR-1254-4

R.T.: 7.341 min
 Delta R.T.: -0.005 min
 Response: 1959487
 Conc: 24.91 ng/ml

Instrument: ECD_P
 ClientSampleId: OU4-TS-38-071725

#29 AR-1254-4


R.T.: 6.428 min
 Delta R.T.: -0.009 min
 Response: 1886359
 Conc: 19.95 ng/ml

#30 AR-1254-5

R.T.: 7.776 min
 Delta R.T.: 0.013 min
 Response: 11486495
 Conc: 155.90 ng/ml

#30 AR-1254-5

R.T.: 6.840 min
 Delta R.T.: -0.013 min
 Response: 20407242
 Conc: 152.93 ng/ml

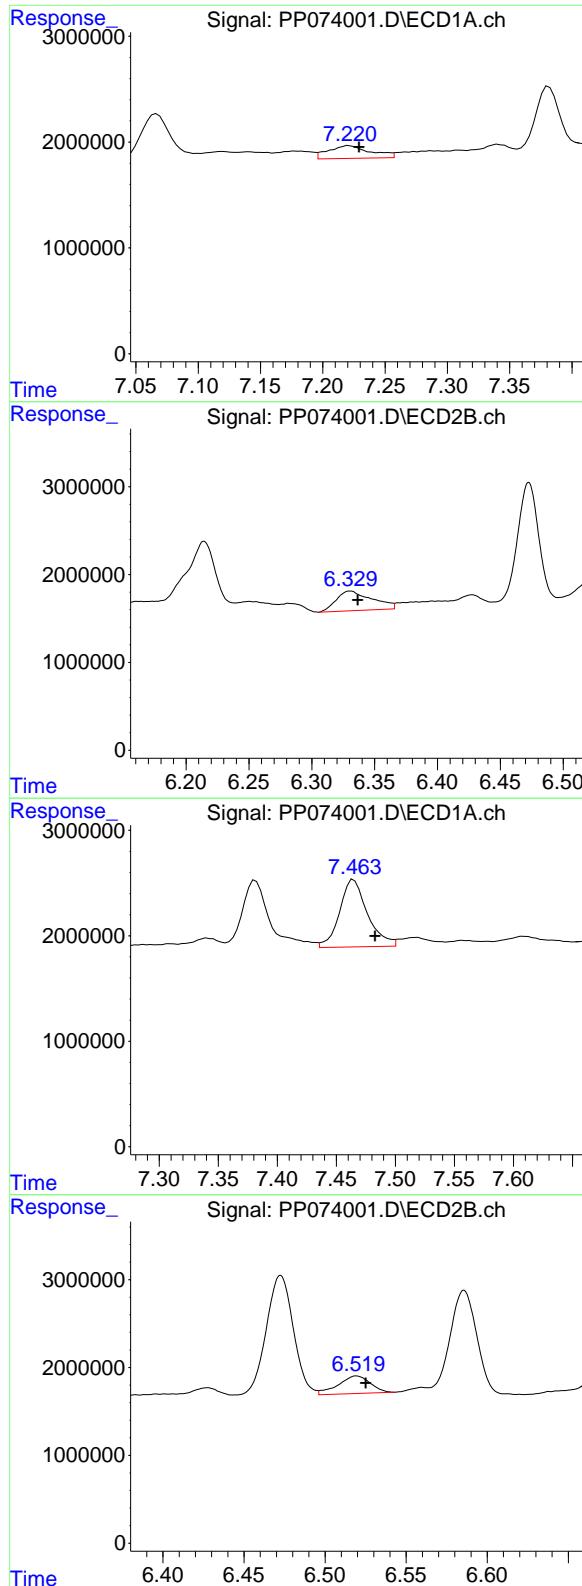

#31 AR-1260-1

R.T.: 7.221 min
 Delta R.T.: -0.008 min
 Response: 2823933
 Conc: 47.89 ng/ml

Instrument: ECD_P
 ClientSampleId: OU4-TS-38-071725

#31 AR-1260-1


R.T.: 6.330 min
 Delta R.T.: -0.006 min
 Response: 4466526
 Conc: 45.78 ng/ml

#32 AR-1260-2

R.T.: 7.465 min
 Delta R.T.: -0.018 min
 Response: 10469388
 Conc: 109.24 ng/ml

#32 AR-1260-2


R.T.: 6.519 min
 Delta R.T.: -0.006 min
 Response: 2773734
 Conc: 22.58 ng/ml

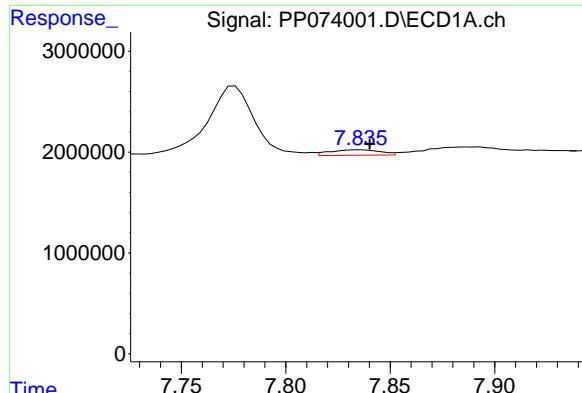

#33 AR-1260-3


R.T.: 7.836 min
Delta R.T.: -0.004 min
Response: 907435
Conc: 12.42 ng/ml

Instrument: ECD_P
ClientSampleId: OU4-TS-38-071725

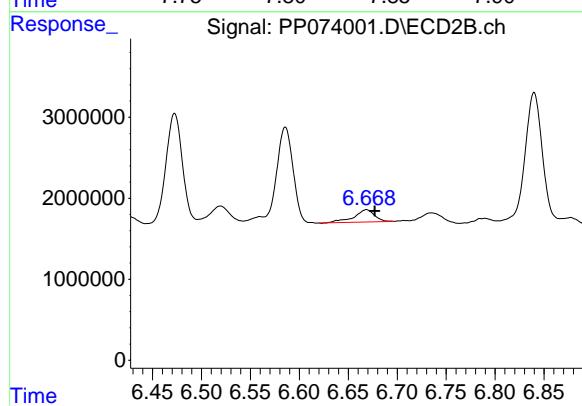


#33 AR-1260-3

R.T.: 6.669 min
Delta R.T.: -0.008 min
Response: 2209772
Conc: 20.19 ng/ml

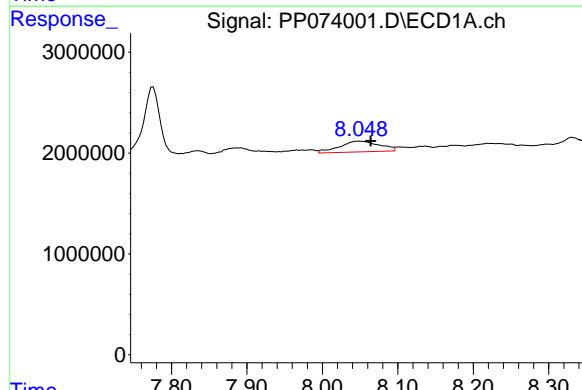


#34 AR-1260-4

R.T.: 8.049 min
Delta R.T.: -0.015 min
Response: 3898789
Conc: 59.71 ng/ml

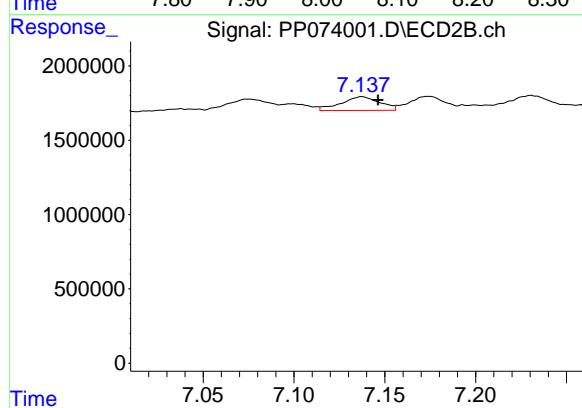

#34 AR-1260-4


R.T.: 7.137 min
Delta R.T.: -0.009 min
Response: 1387004
Conc: 15.51 ng/ml

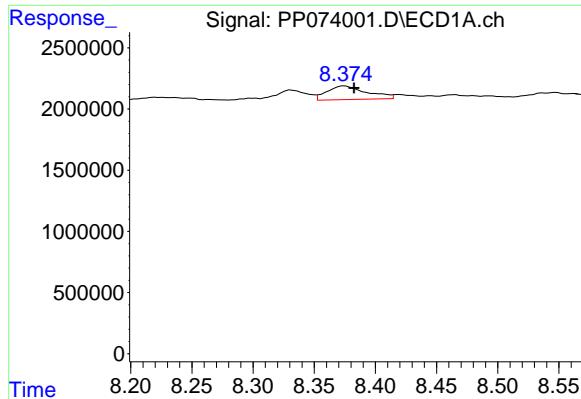

#35 AR-1260-5


R.T.: 8.375 min
 Delta R.T.: -0.008 min
 Response: 2514577
 Conc: 16.67 ng/ml

Instrument: ECD_P
 ClientSampleId: OU4-TS-38-071725

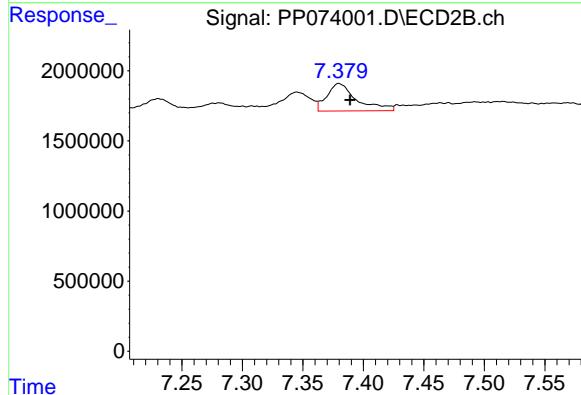


#35 AR-1260-5

R.T.: 7.380 min
 Delta R.T.: -0.009 min
 Response: 3370940
 Conc: 15.00 ng/ml

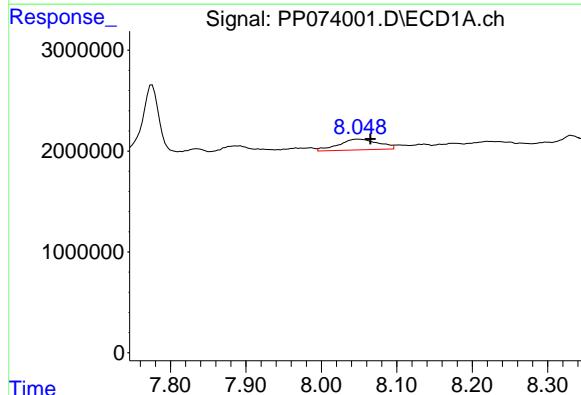


#36 AR-1262-1

R.T.: 8.049 min
 Delta R.T.: -0.016 min
 Response: 3898789
 Conc: 44.80 ng/ml

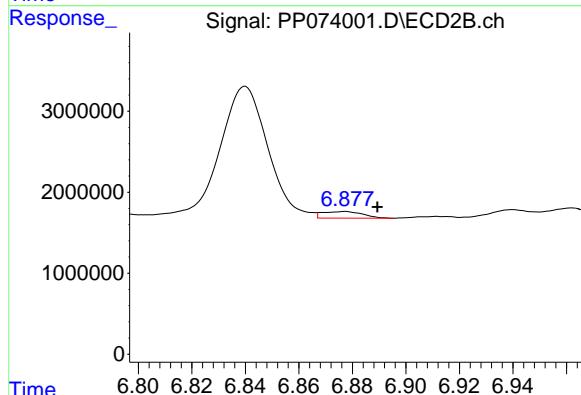

#36 AR-1262-1

R.T.: 6.877 min
 Delta R.T.: -0.012 min
 Response: 847997
 Conc: 5.74 ng/ml

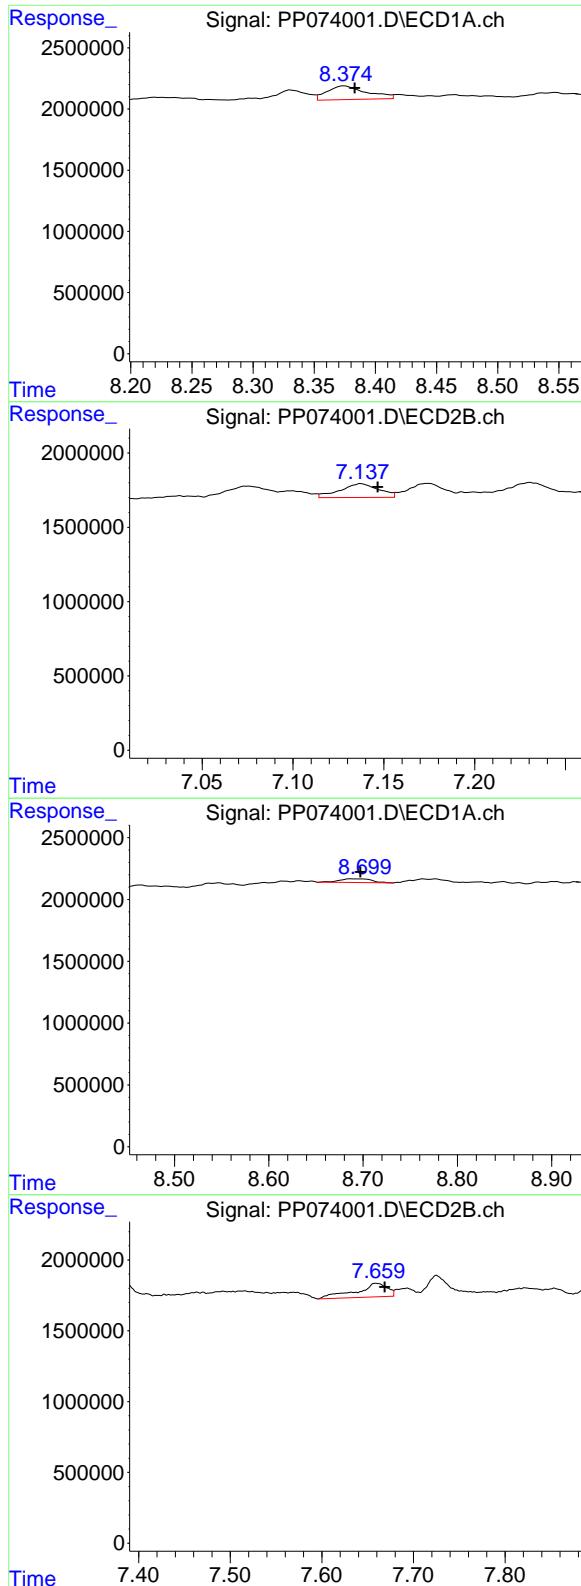

#37 AR-1262-2

R.T.: 8.375 min
 Delta R.T.: -0.008 min
 Response: 2514577
 Conc: 12.70 ng/ml

Instrument: ECD_P
 ClientSampleId: OU4-TS-38-071725

#37 AR-1262-2


R.T.: 7.137 min
 Delta R.T.: -0.009 min
 Response: 1387004
 Conc: 10.85 ng/ml

#38 AR-1262-3

R.T.: 8.687 min
 Delta R.T.: -0.010 min
 Response: 710351
 Conc: 5.65 ng/ml

#38 AR-1262-3

R.T.: 7.659 min
 Delta R.T.: -0.010 min
 Response: 2301706
 Conc: 20.19 ng/ml

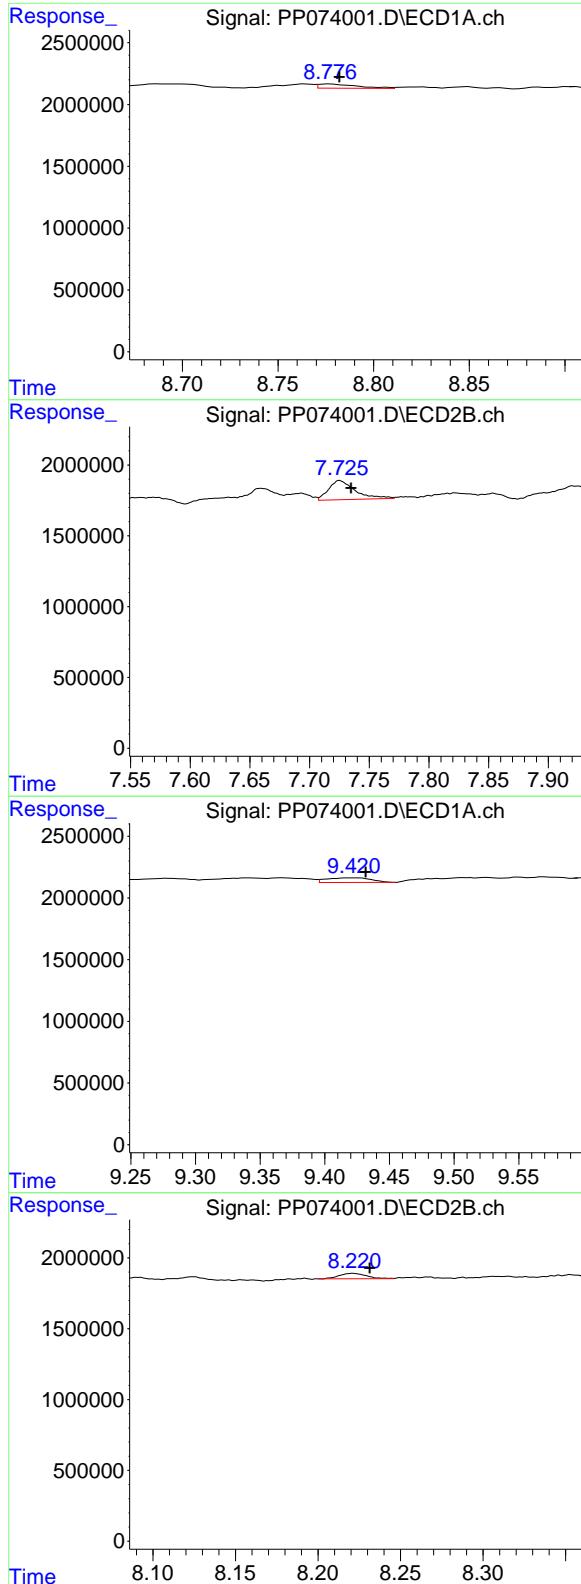

#39 AR-1262-4

R.T.: 8.777 min
 Delta R.T.: -0.005 min
 Response: 489718
 Conc: 5.25 ng/ml

Instrument: ECD_P
 ClientSampleId: OU4-TS-38-071725

#39 AR-1262-4


R.T.: 7.725 min
 Delta R.T.: -0.010 min
 Response: 2093441
 Conc: 11.37 ng/ml

#40 AR-1262-5

R.T.: 9.422 min
 Delta R.T.: -0.009 min
 Response: 891155
 Conc: 14.06 ng/ml

#40 AR-1262-5

R.T.: 8.221 min
 Delta R.T.: -0.010 min
 Response: 433627
 Conc: 5.14 ng/ml

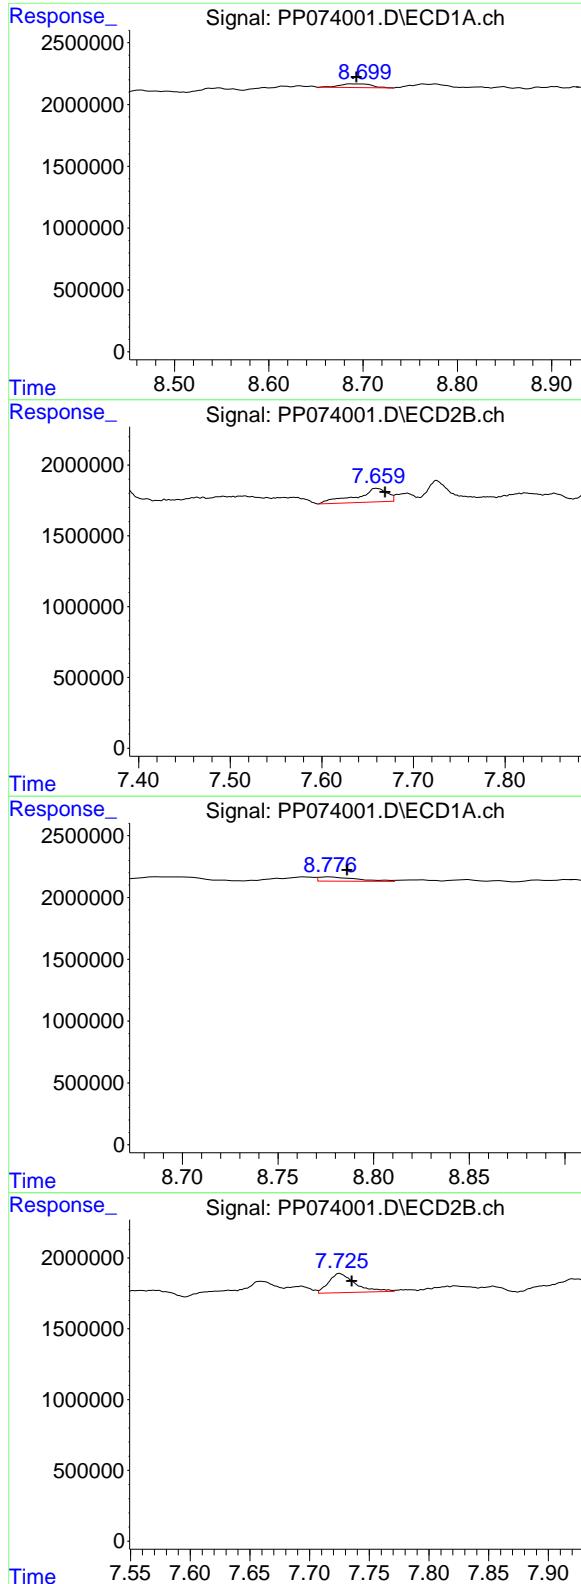

#41 AR-1268-1

R.T.: 8.687 min
 Delta R.T.: -0.006 min Instrument:
 Response: 710351 ECD_P
 Conc: 3.18 ng/ml ClientSampleId :
 OU4-TS-38-071725

#41 AR-1268-1


R.T.: 7.659 min
 Delta R.T.: -0.010 min
 Response: 2301706
 Conc: 7.49 ng/ml

#42 AR-1268-2

R.T.: 8.777 min
 Delta R.T.: -0.009 min
 Response: 489718
 Conc: 2.57 ng/ml

#42 AR-1268-2


R.T.: 7.725 min
 Delta R.T.: -0.010 min
 Response: 2093441
 Conc: 7.88 ng/ml



#43 AR-1268-3


R.T.: 8.969 min
Delta R.T.: -0.045 min
Response: 324985
Conc: 1.96 ng/ml

Instrument: ECD_P
ClientSampleId: OU4-TS-38-071725

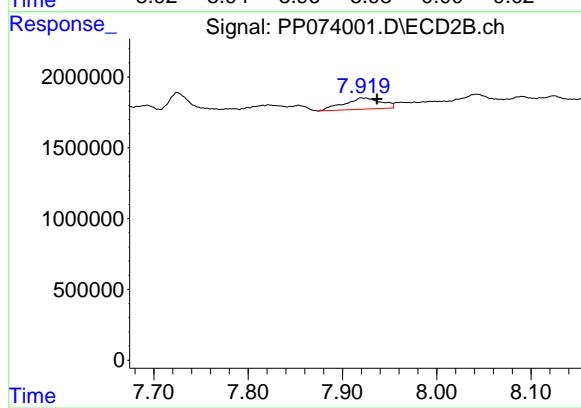


#43 AR-1268-3

R.T.: 7.920 min
Delta R.T.: -0.016 min
Response: 2205194
Conc: 9.78 ng/ml

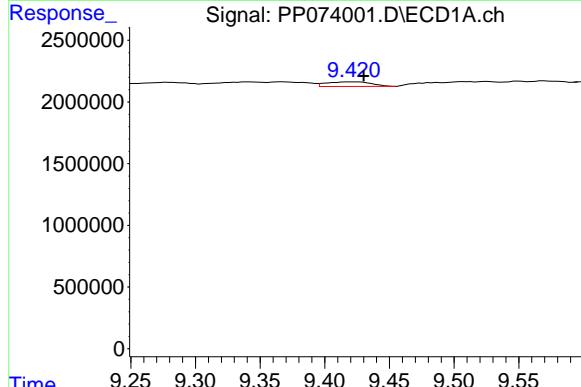


#44 AR-1268-4

R.T.: 9.422 min
Delta R.T.: -0.008 min
Response: 891155
Conc: 12.81 ng/ml

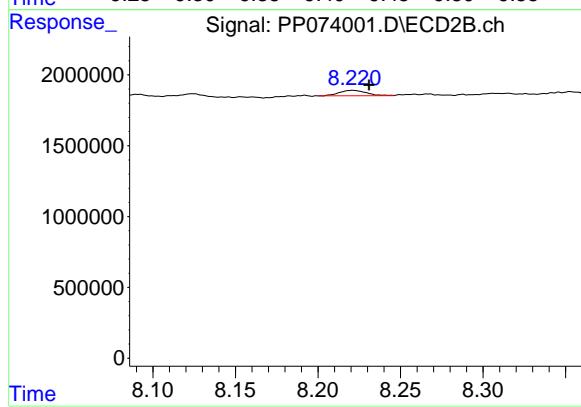

#44 AR-1268-4

R.T.: 8.221 min
Delta R.T.: -0.010 min
Response: 433627
Conc: 4.66 ng/ml

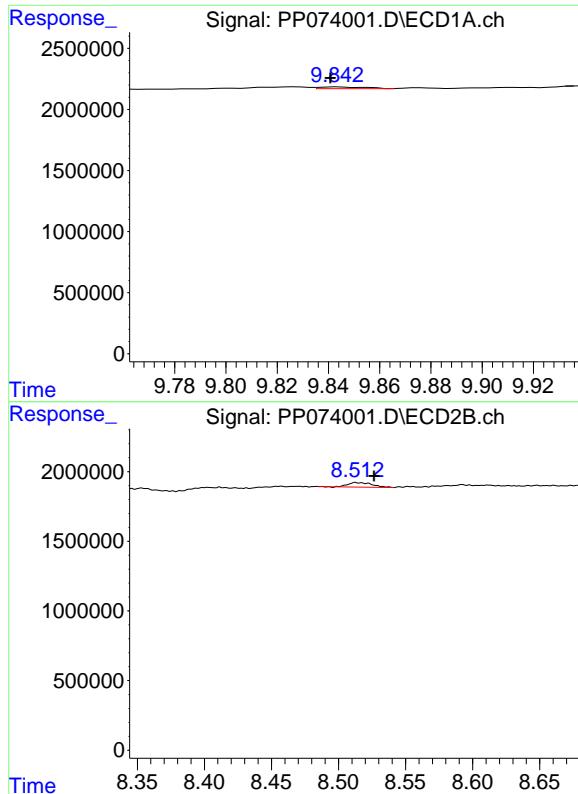

#45 AR-1268-5

R.T.: 9.844 min
Delta R.T.: 0.003 min
Response: 187351
Conc: 0.41 ng/ml

Instrument: ECD_P
ClientSampleId: OU4-TS-38-071725

1
2
3
4
5
6
7
8
9
10
11
12
13
14
15
16
17
18
19
20