

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD072125\
 Data File : PD089539.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jul 2025 12:35
 Operator : AR\AJ
 Sample : RESCHK
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 RESCHK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 22 04:42:17 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD072125.M
 Quant Title : GC Extractables
 QLast Update : Tue Jul 22 04:39:29 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.548	2.879	51809968	366.9E6	17.981	18.750
28)	SA Decachlor...	9.071	8.070	78129847	453.3E6	19.023	18.452
Target Compounds							
9)	A Endosulfan I	6.073	5.244	38431902	224.6E6	8.645	9.458
10)	B gamma-Chl...	5.944	5.123	42237481	267.0E6	8.909	9.982
12)	B 4,4'-DDE	6.194	5.373	77258612	510.3E6	17.993	19.434
13)	MA Dieldrin	6.345	5.510	83847363	504.8E6	17.762	19.103
19)	B Endosulfa...	7.148	6.480	70006243	429.5E6	18.549	19.348
20)	A Methoxychlor	7.492	6.752	174.7E6	1003.1E6	87.156	82.274
21)	B Endrin ke...	7.629	6.990	73683552	472.0E6	18.310	19.274



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD072125\
Data File : PD089539.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Jul 2025 12:35
Operator : AR\AJ
Sample : RESCHK
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESCHK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 22 04:42:17 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD072125.M
Quant Title : GC Extractables
QLast Update : Tue Jul 22 04:39:29 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

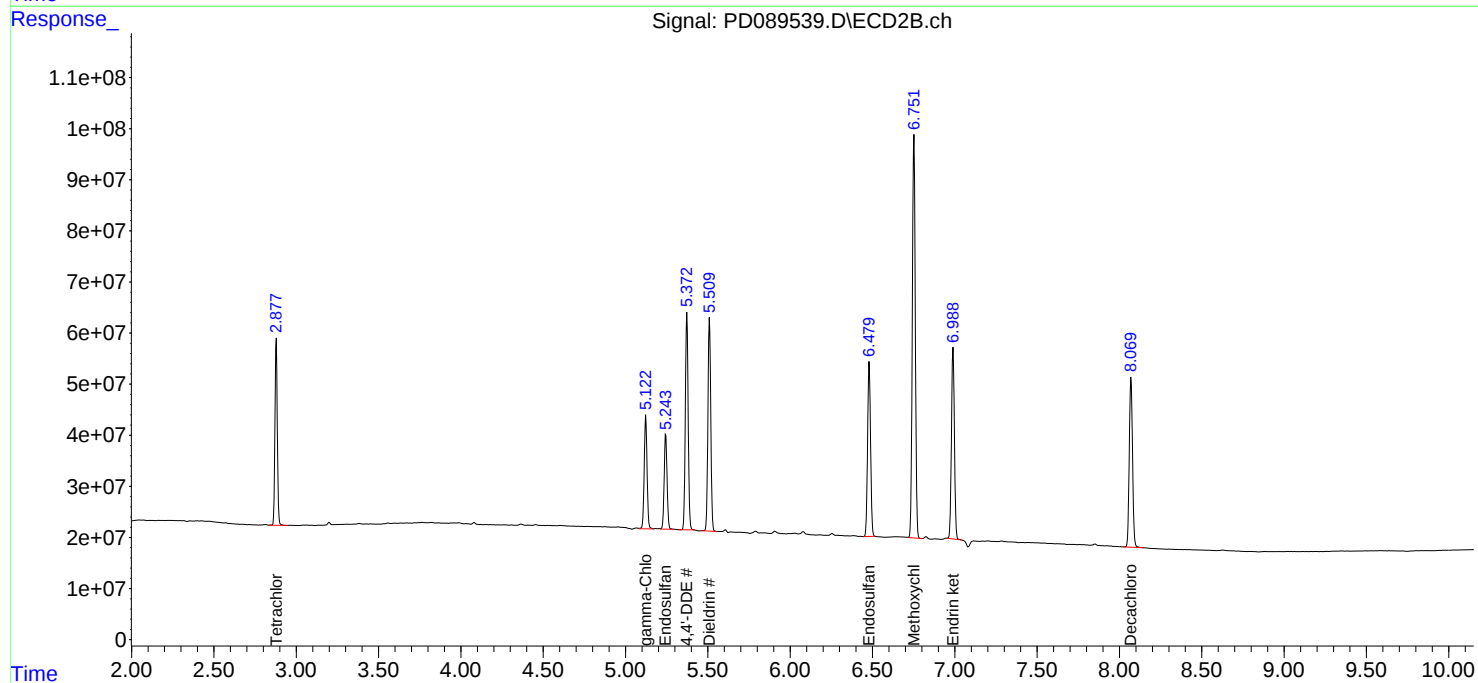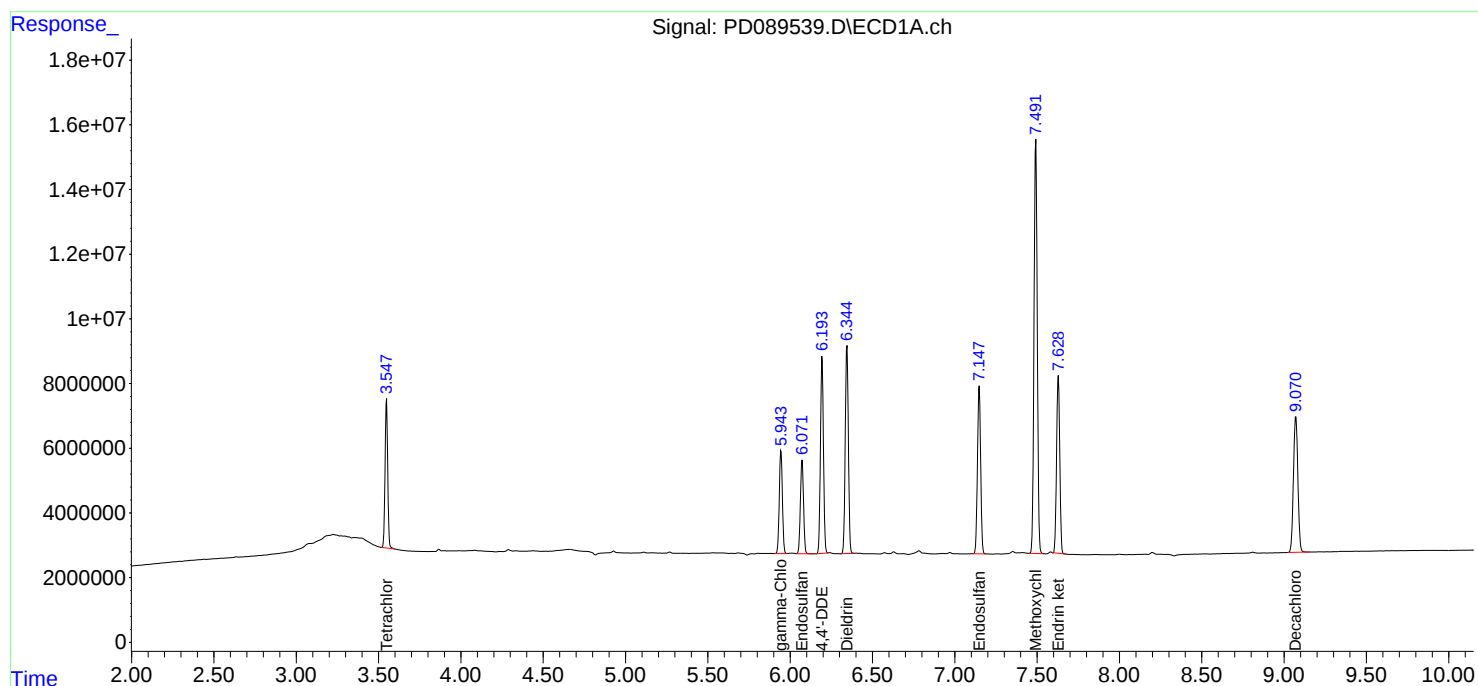


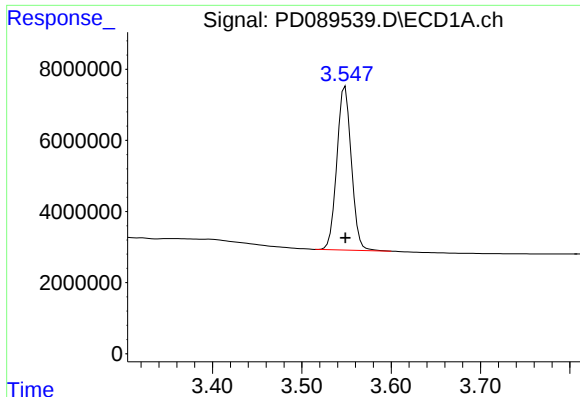

#1 Tetrachloro-m-xylene


R.T.: 3.548 min
Delta R.T.: 0.000 min
Response: 51809968
Conc: 17.98 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

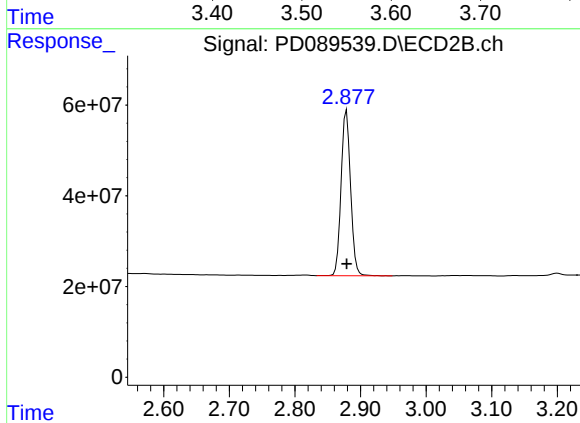


#1 Tetrachloro-m-xylene

R.T.: 2.879 min
Delta R.T.: 0.000 min
Response: 366859486
Conc: 18.75 ng/ml

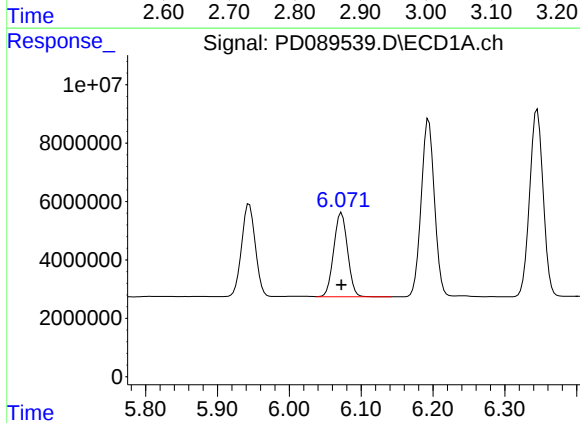


#9 Endosulfan I

R.T.: 6.073 min
Delta R.T.: 0.000 min
Response: 38431902
Conc: 8.64 ng/ml

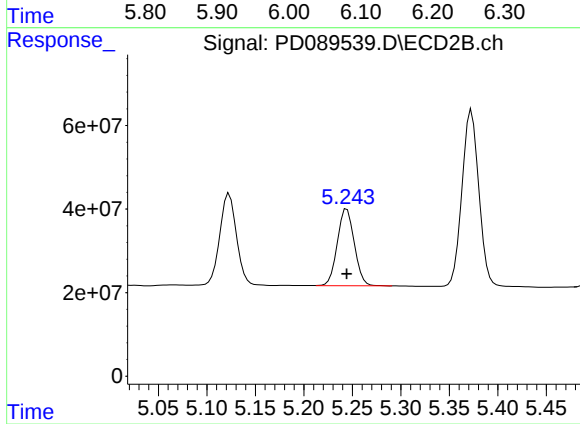

#9 Endosulfan I


R.T.: 5.244 min
Delta R.T.: 0.000 min
Response: 224597727
Conc: 9.46 ng/ml

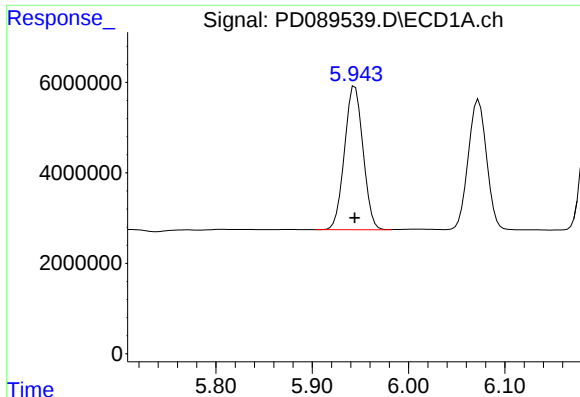

#10 gamma-Chlordane


R.T.: 5.944 min
Delta R.T.: 0.000 min
Response: 42237481
Conc: 8.91 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

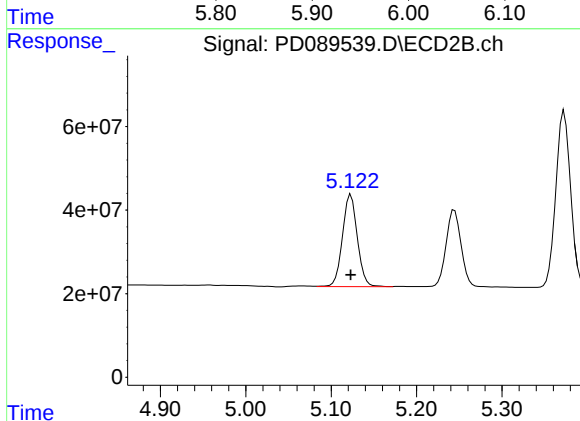


#10 gamma-Chlordane

R.T.: 5.123 min
Delta R.T.: 0.000 min
Response: 267039042
Conc: 9.98 ng/ml

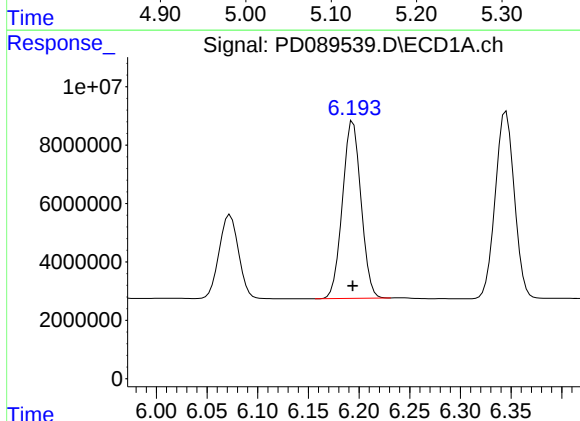


#12 4,4'-DDE

R.T.: 6.194 min
Delta R.T.: 0.000 min
Response: 77258612
Conc: 17.99 ng/ml

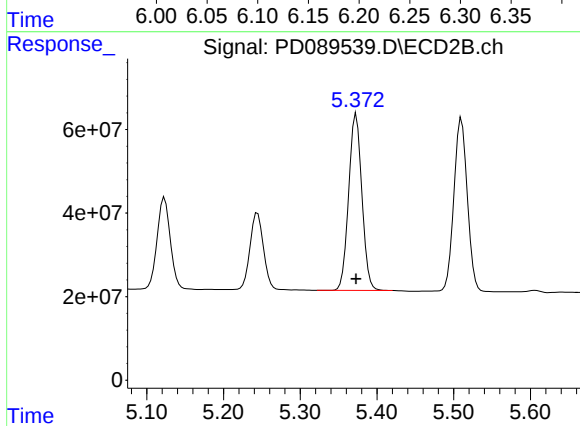

#12 4,4'-DDE


R.T.: 5.373 min
Delta R.T.: 0.000 min
Response: 510254291
Conc: 19.43 ng/ml

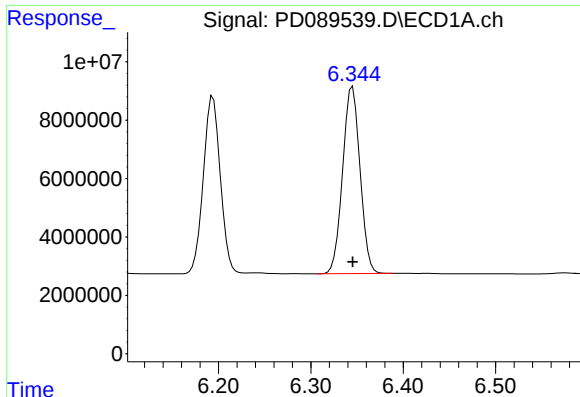

#13 Dieldrin


R.T.: 6.345 min
Delta R.T.: 0.000 min
Response: 83847363
Conc: 17.76 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

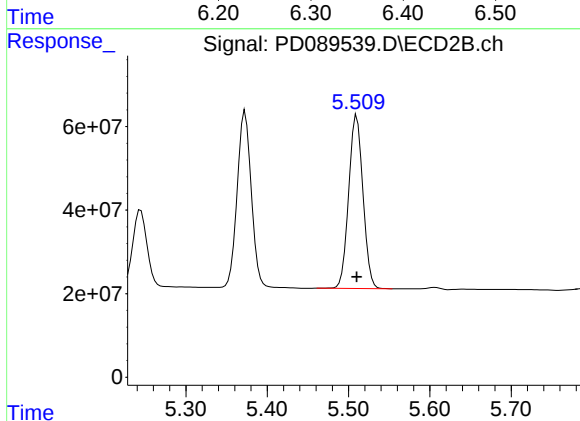


#13 Dieldrin

R.T.: 5.510 min
Delta R.T.: 0.000 min
Response: 504825335
Conc: 19.10 ng/ml

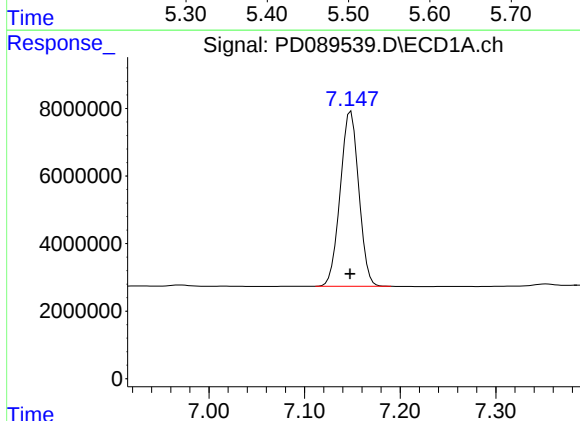


#19 Endosulfan Sulfate

R.T.: 7.148 min
Delta R.T.: 0.000 min
Response: 70006243
Conc: 18.55 ng/ml

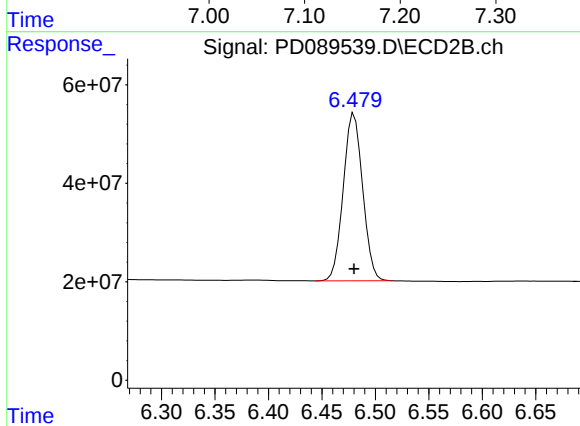

#19 Endosulfan Sulfate


R.T.: 6.480 min
Delta R.T.: 0.000 min
Response: 429487748
Conc: 19.35 ng/ml

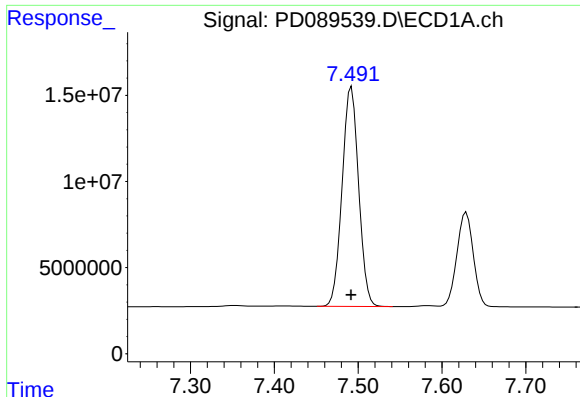

#20 Methoxychlor


R.T.: 7.492 min
Delta R.T.: 0.000 min
Response: 174739023
Conc: 87.16 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

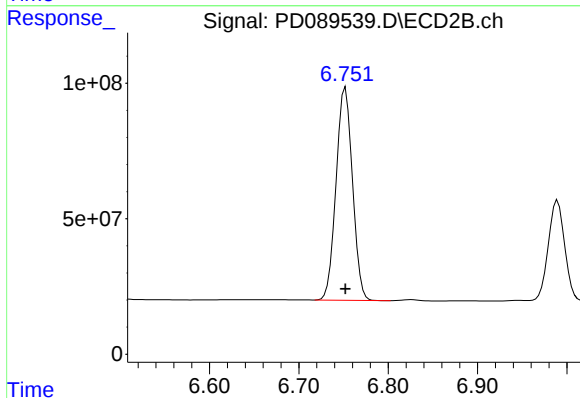


#20 Methoxychlor

R.T.: 6.752 min
Delta R.T.: 0.000 min
Response: 1003076887
Conc: 82.27 ng/ml

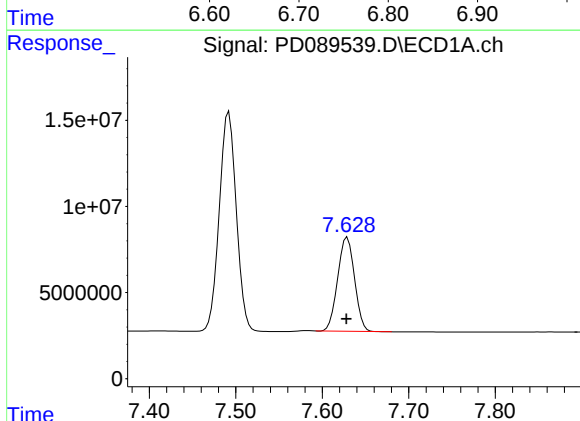


#21 Endrin ketone

R.T.: 7.629 min
Delta R.T.: 0.000 min
Response: 73683552
Conc: 18.31 ng/ml

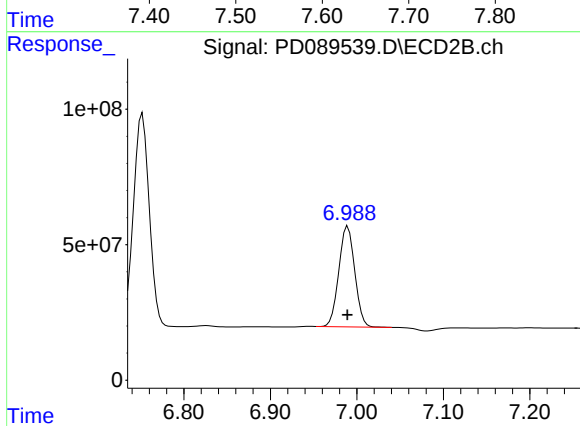

#21 Endrin ketone


R.T.: 6.990 min
Delta R.T.: 0.000 min
Response: 471998069
Conc: 19.27 ng/ml

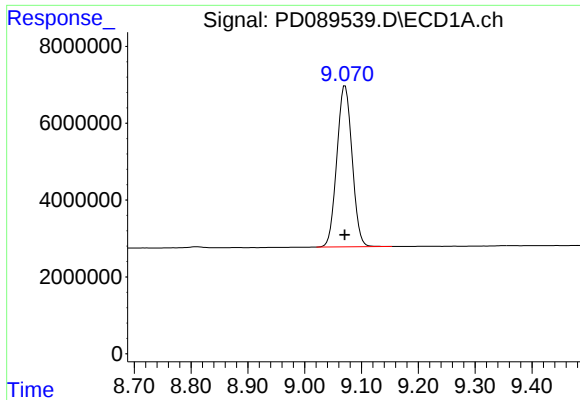

#28 Decachlorobiphenyl

R.T.: 9.071 min
Delta R.T.: 0.000 min
Response: 78129847
Conc: 19.02 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

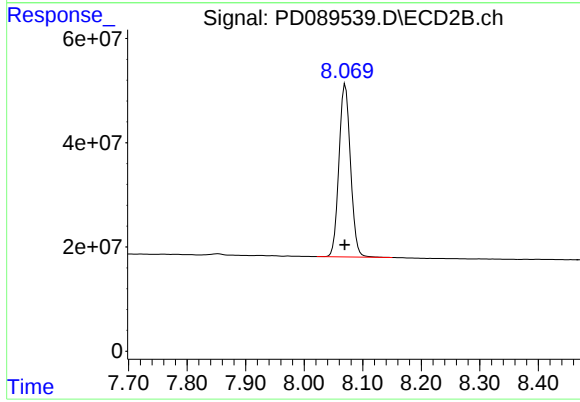

#28 Decachlorobiphenyl

R.T.: 8.070 min
Delta R.T.: 0.000 min
Response: 453328331
Conc: 18.45 ng/ml