

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD072125\
 Data File : PD089547.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jul 2025 14:25
 Operator : AR\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 22 04:16:43 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD072125.M
 Quant Title : GC Extractables
 QLast Update : Tue Jul 22 04:15:29 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.549	2.879	137.0E6	1147.5E6	50.000	50.000
28)	SA Decachlor...	9.071	8.070	191.4E6	1159.2E6	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.713	3.904	95759549	451.9E6	500.000	500.000
24)	Chlordane-2	5.239	4.485	96700402	471.2E6	500.000	500.000
25)	Chlordane-3	5.944	5.123	384.7E6	1387.3E6	500.000	500.000
26)	Chlordane-4	6.029	5.188	464.4E6	1166.3E6	500.000	500.000
27)	Chlordane-5	6.869	6.088	81273058	568.6E6	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD072125\
Data File : PD089547.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Jul 2025 14:25
Operator : AR\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 22 04:16:43 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD072125.M
Quant Title : GC Extractables
QLast Update : Tue Jul 22 04:15:29 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

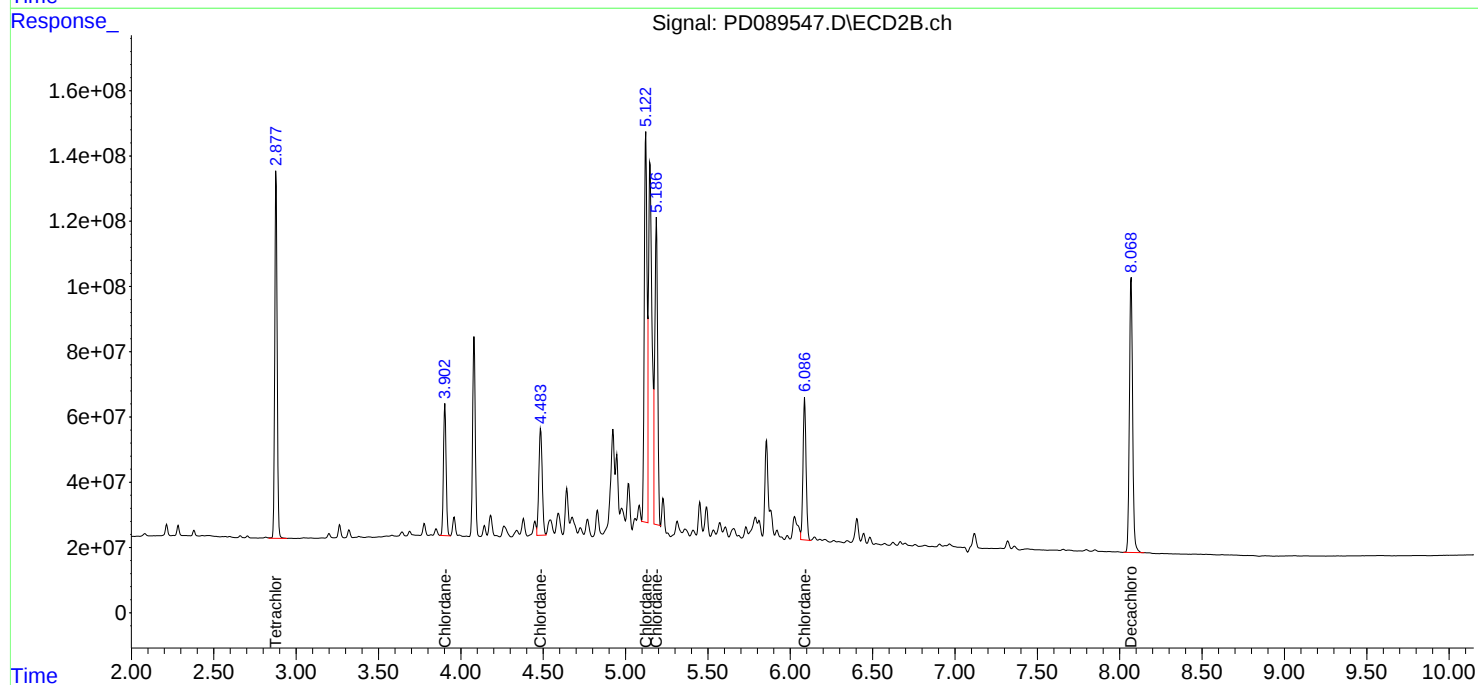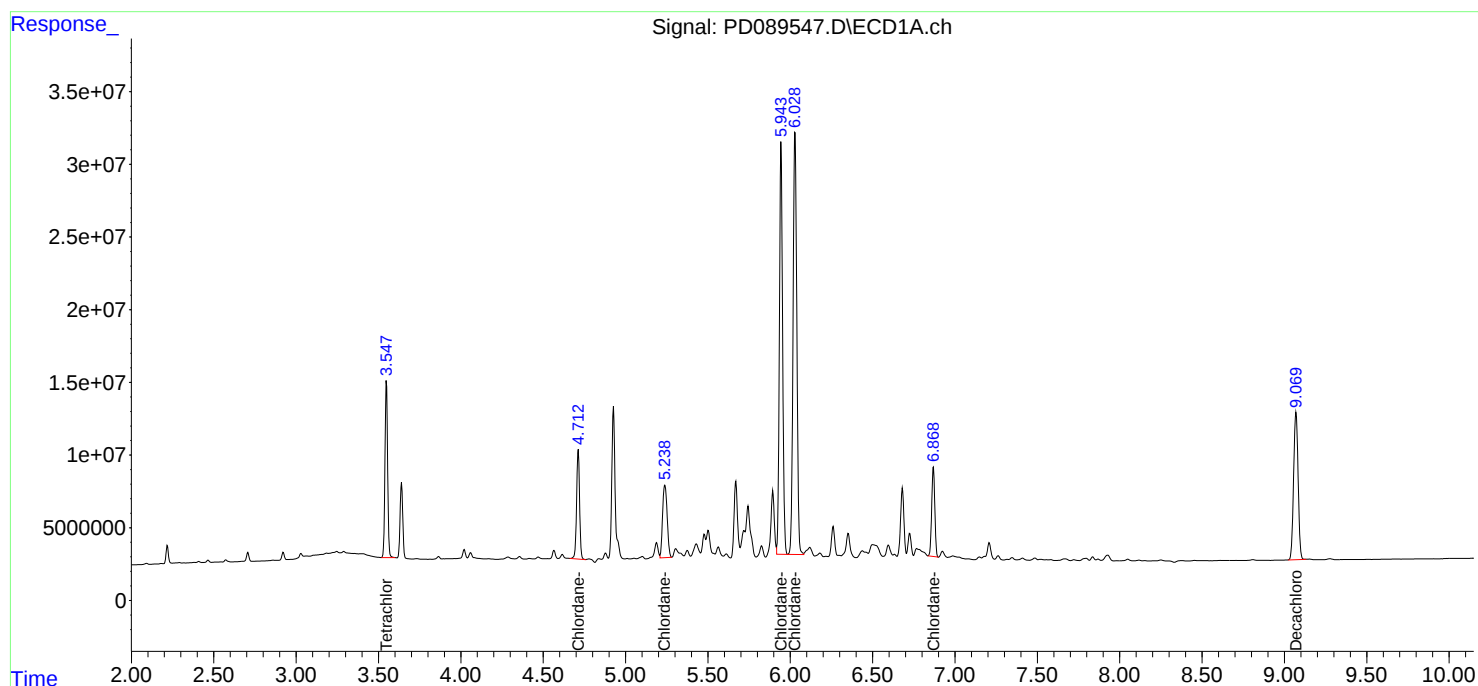


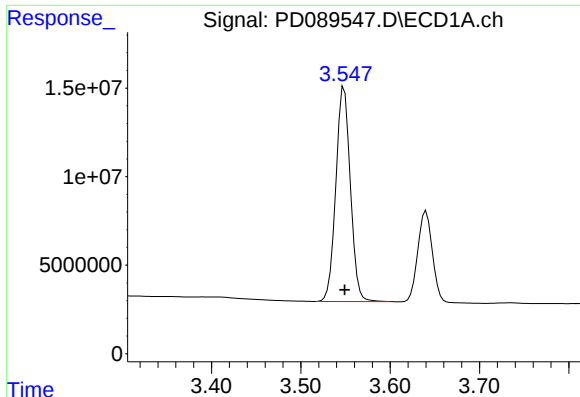

#1 Tetrachloro-m-xylene


R.T.: 3.549 min
Delta R.T.: 0.000 min
Response: 136988831
Conc: 50.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

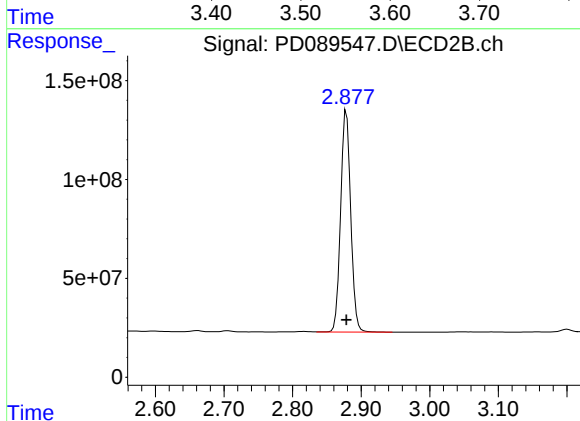


#1 Tetrachloro-m-xylene

R.T.: 2.879 min
Delta R.T.: 0.000 min
Response: 1147510938
Conc: 50.00 ng/ml

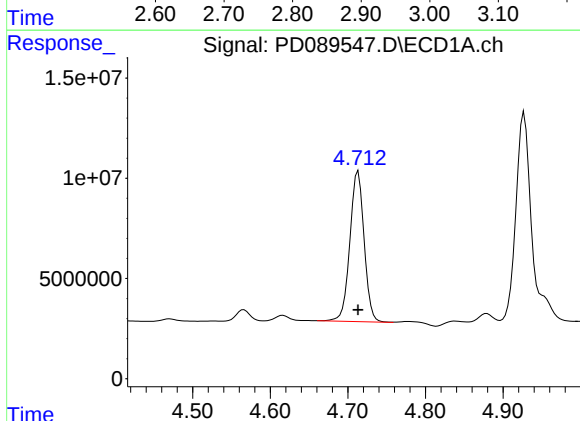


#23 Chlordane-1

R.T.: 4.713 min
Delta R.T.: 0.000 min
Response: 95759549
Conc: 500.00 ng/ml

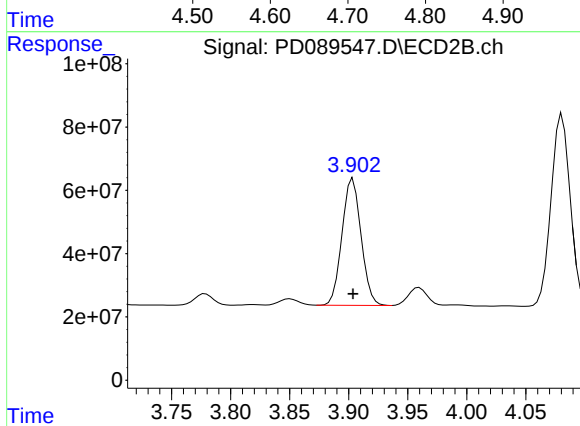

#23 Chlordane-1


R.T.: 3.904 min
Delta R.T.: 0.000 min
Response: 451936761
Conc: 500.00 ng/ml

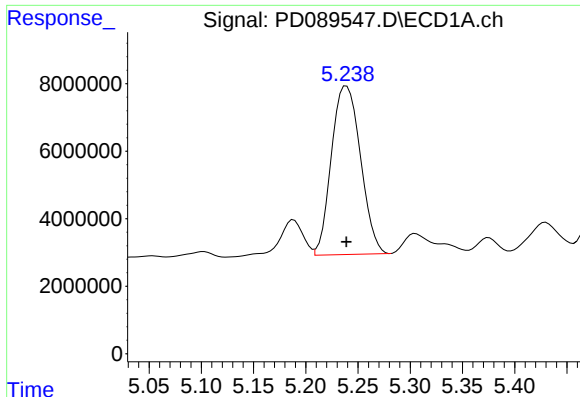

#24 Chlordane-2


R.T.: 5.239 min
Delta R.T.: 0.000 min
Response: 96700402
Conc: 500.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

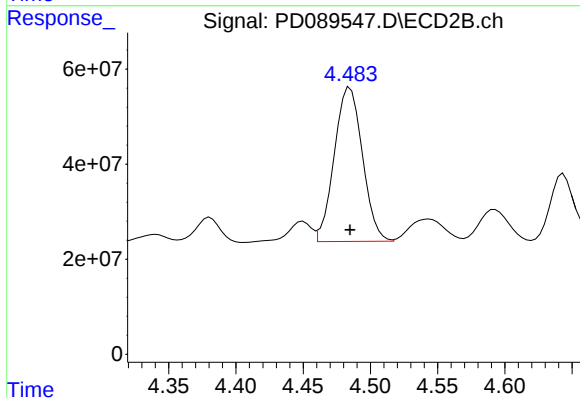


#24 Chlordane-2

R.T.: 4.485 min
Delta R.T.: 0.000 min
Response: 471219127
Conc: 500.00 ng/ml

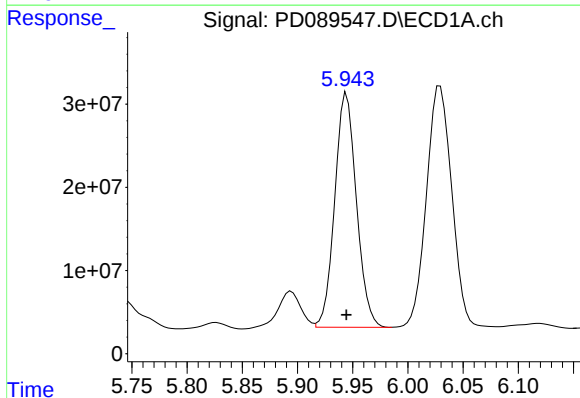


#25 Chlordane-3

R.T.: 5.944 min
Delta R.T.: 0.000 min
Response: 384734362
Conc: 500.00 ng/ml

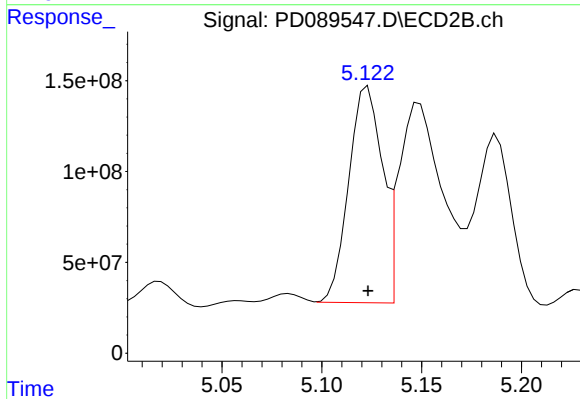

#25 Chlordane-3


R.T.: 5.123 min
Delta R.T.: 0.000 min
Response: 1387289900
Conc: 500.00 ng/ml

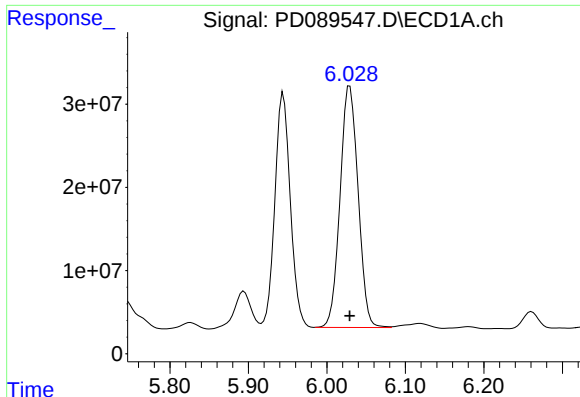

#26 Chlordane-4


R.T.: 6.029 min
Delta R.T.: 0.000 min
Response: 464421533
Conc: 500.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

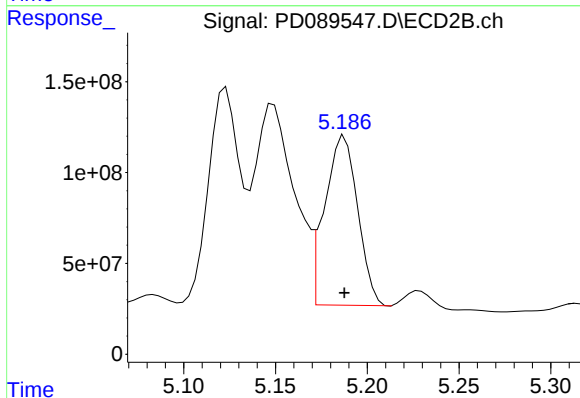


#26 Chlordane-4

R.T.: 5.188 min
Delta R.T.: 0.000 min
Response: 1166286432
Conc: 500.00 ng/ml

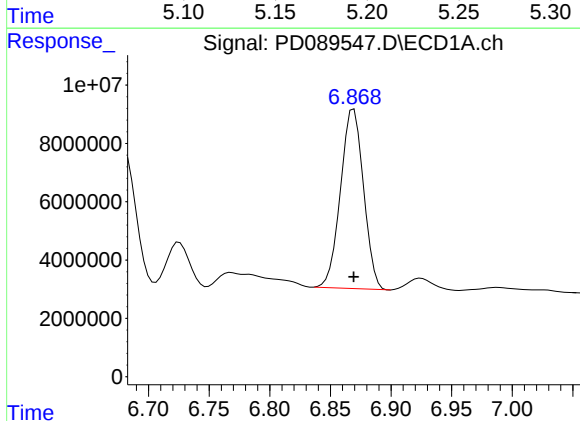


#27 Chlordane-5

R.T.: 6.869 min
Delta R.T.: 0.000 min
Response: 81273058
Conc: 500.00 ng/ml

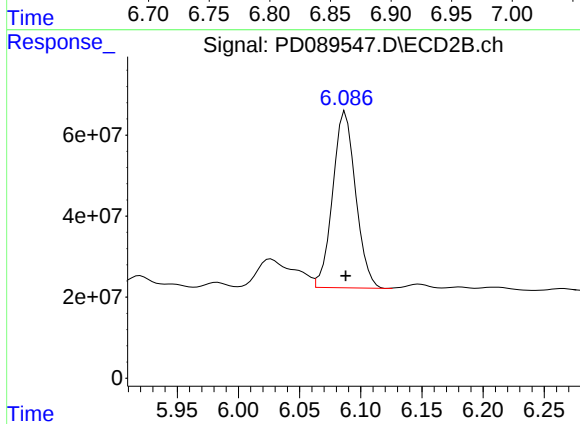

#27 Chlordane-5


R.T.: 6.088 min
Delta R.T.: 0.000 min
Response: 568647475
Conc: 500.00 ng/ml

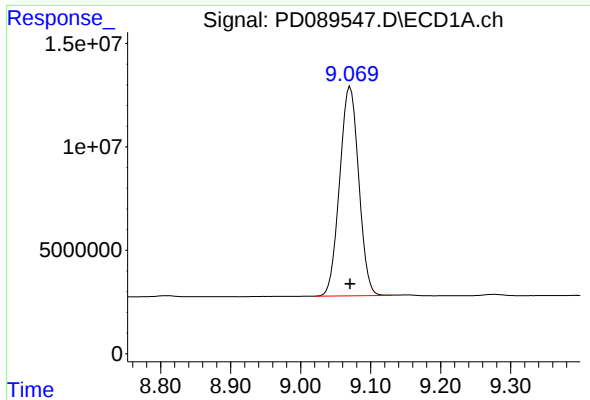

#28 Decachlorobiphenyl

R.T.: 9.071 min
Delta R.T.: 0.000 min
Response: 191372995
Conc: 50.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

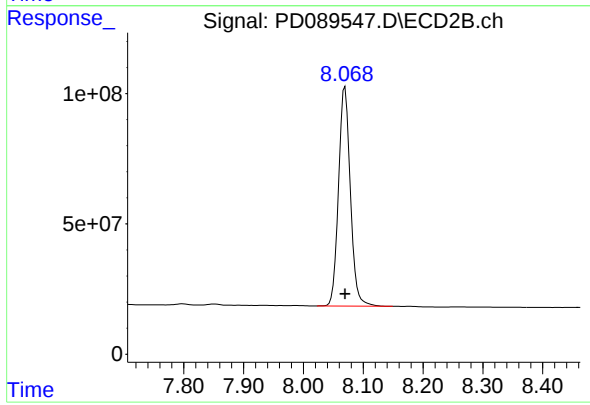

#28 Decachlorobiphenyl

R.T.: 8.070 min
Delta R.T.: 0.000 min
Response: 1159232979
Conc: 50.00 ng/ml