


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072325\
Data File : BF143209.D
Acq On : 23 Jul 2025 13:34
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF071725.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Jul 17 15:14:05 2025

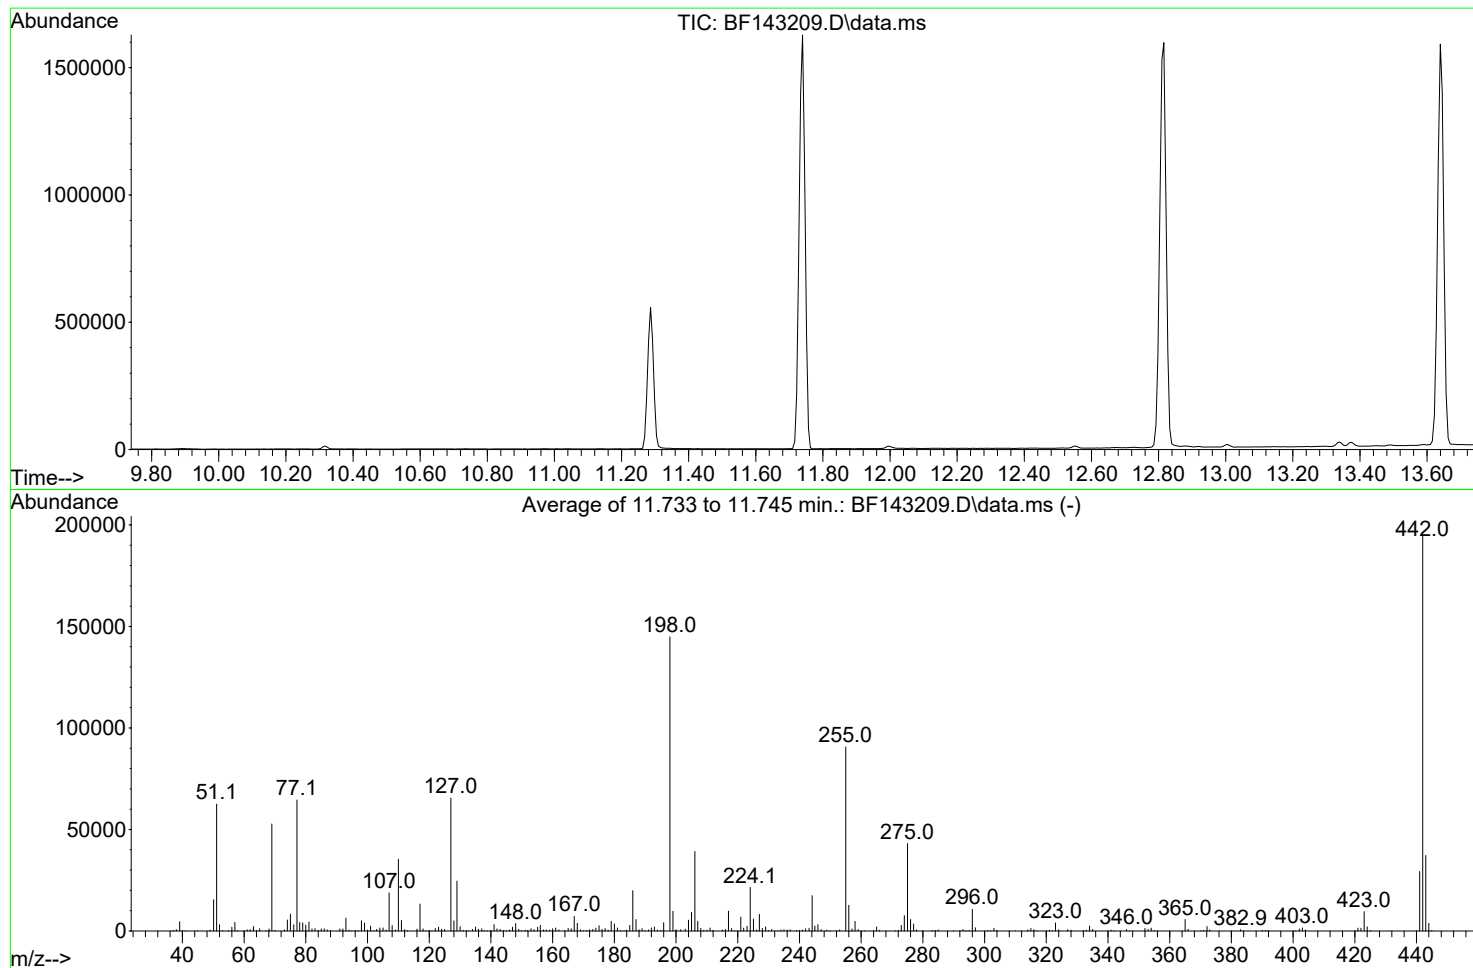

AutoFind: Scans 1622, 1623, 1624; Background Corrected with Scan 1615

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	1.9	1017	PASS
69	69	100	100	100.0	52688	PASS
70	69	0.00	2	0.6	323	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	144864	PASS
199	198	5	9	6.7	9687	PASS
365	198	1	100	3.9	5697	PASS
441	443	0.01	150	78.8	29299	PASS
442	442	100	100	100.0	194453	PASS
443	442	15	24	19.1	37184	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
7/23/2025	BNA_F	<u>BF143209.D</u>
Compound Name	Response	Retention Time
DDT	391883	13.639
DDD	8780	13.339
DDE	2192	13.004
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
10972	402855	2.72

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072325\
Data File : BF143209.D
Acq On : 23 Jul 2025 13:34
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jul 23 15:17:33 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF071725.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 17 15:14:05 2025
Response via : Initial Calibration

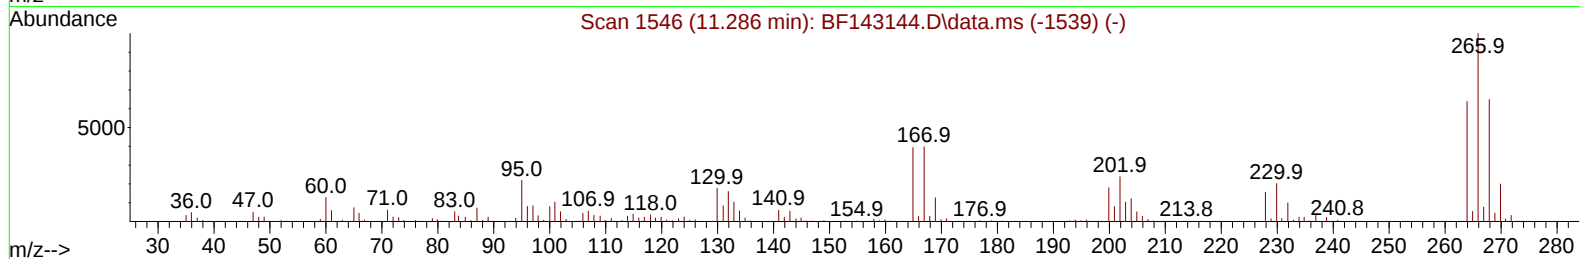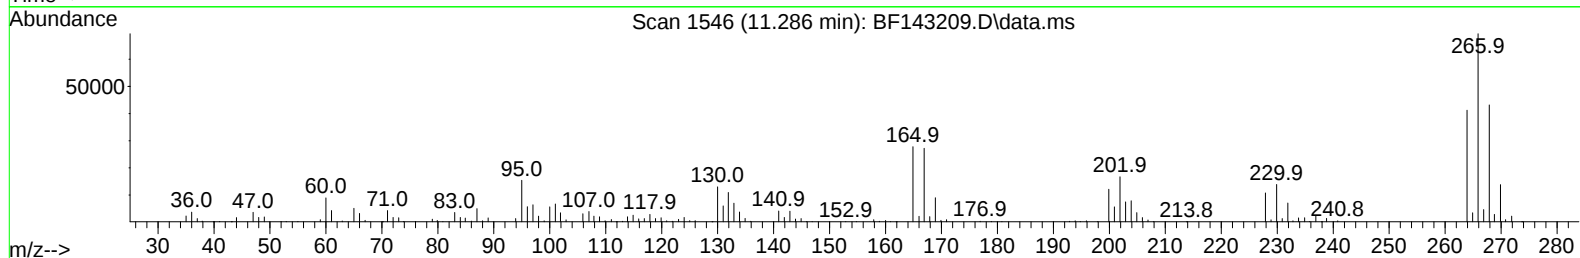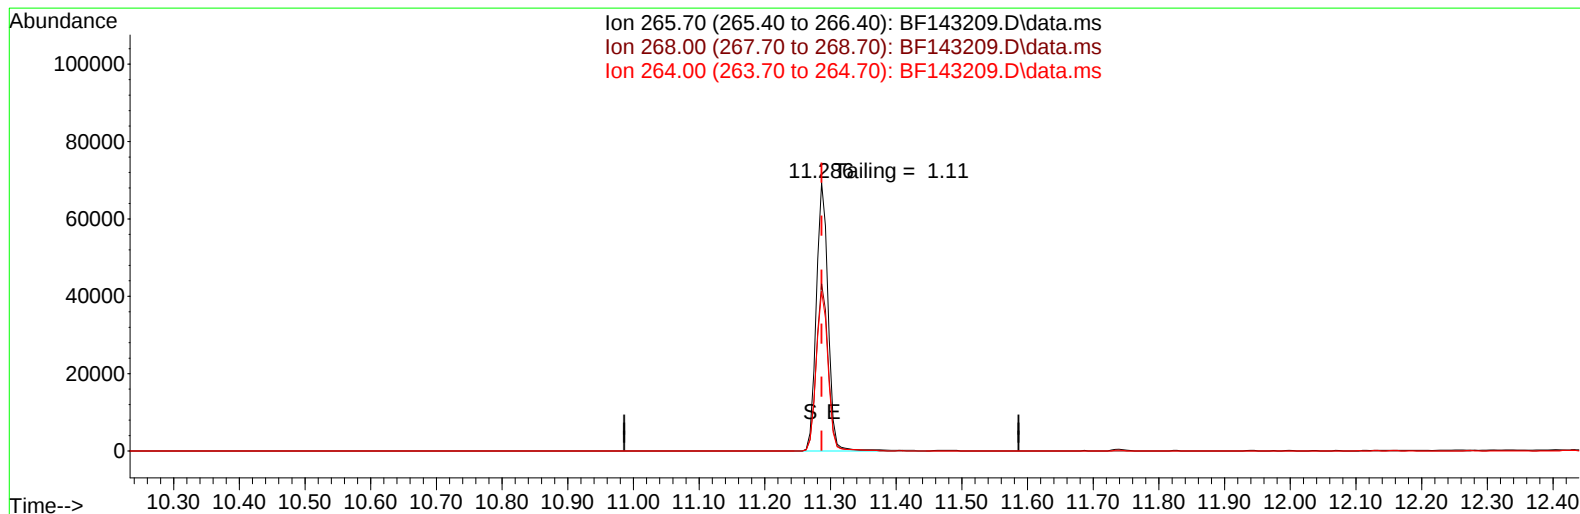

TIC: BF143209.D\data.ms

(70) Pentachlorophenol (C)

11.286min (+ 0.000) 14501.34 ng




response 87636

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.90	62.26
264.00	63.80	59.46
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072325\
Data File : BF143209.D
Acq On : 23 Jul 2025 13:34
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jul 23 15:17:33 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF071725.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 17 15:14:05 2025
Response via : Initial Calibration

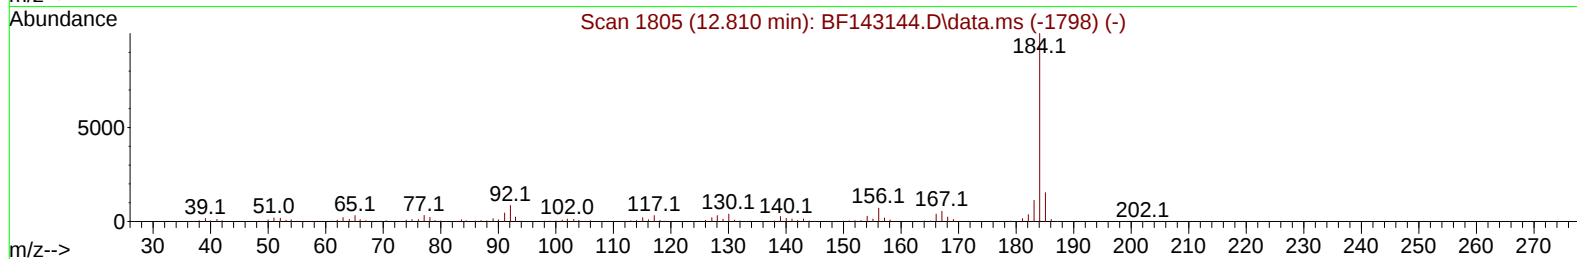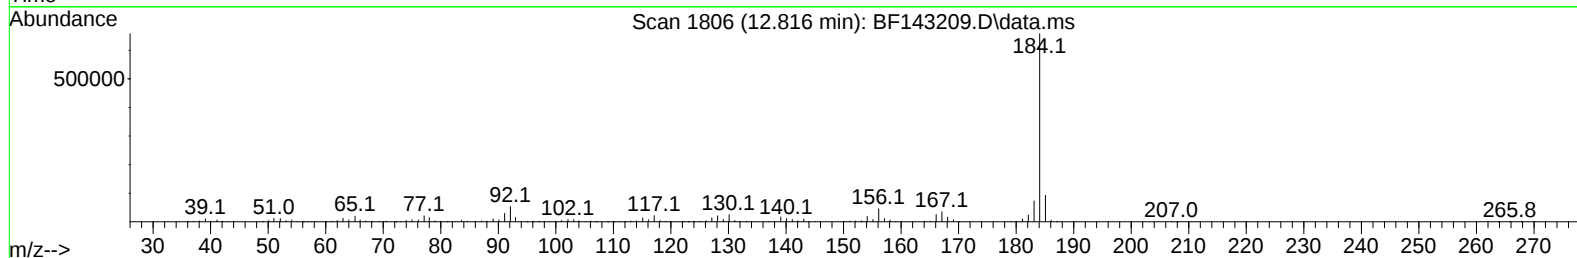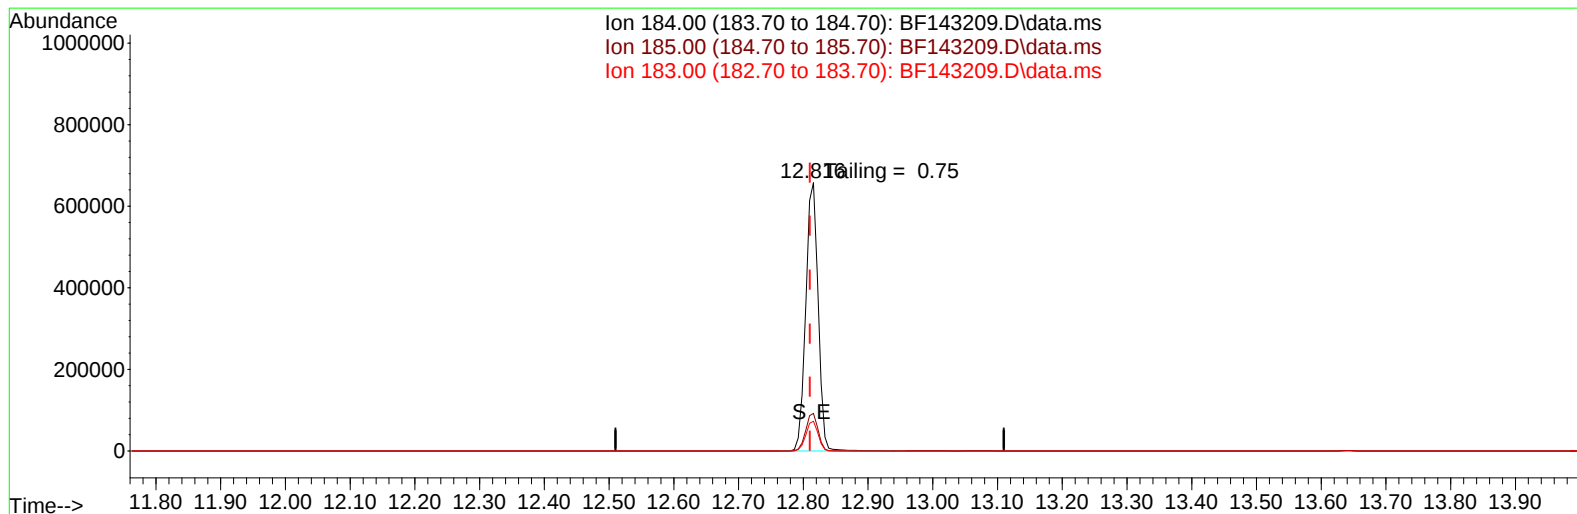

TIC: BF143209.D\data.ms

(77) Benzidine

12.816min (+ 0.006) 0.00 ng

response 876486

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.30	14.03
183.00	11.20	11.13
0.00	0.00	0.00