


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072225\
Data File : BP025206.D
Acq On : 22 Jul 2025 09:04
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP072125.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Jul 22 02:55:21 2025

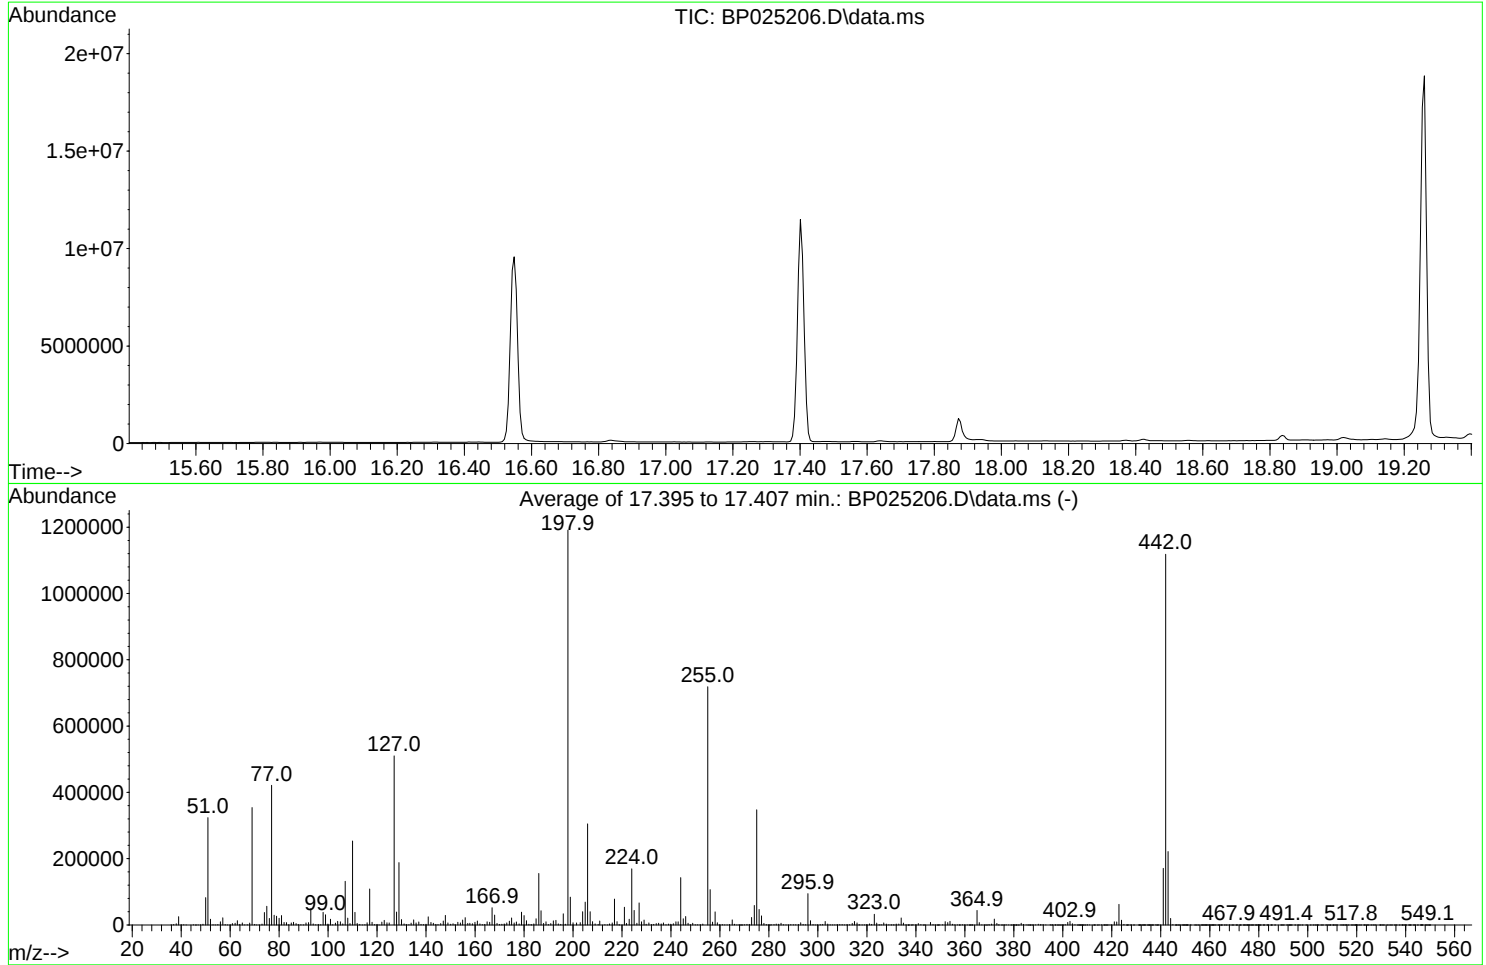




AutoFind: Scans 2458, 2459, 2460; Background Corrected with Scan 2451

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
68	69	0.00	2	1.6	5773	PASS
69	69	100	100	100.0	354212	PASS
70	69	0.00	2	0.5	1756	PASS
197	198	0.00	2	0.2	2051	PASS
198	198	100	100	100.0	1191197	PASS
199	198	5	9	7.0	83600	PASS
365	198	1	100	3.7	43541	PASS
441	443	0.01	150	77.1	170565	PASS
442	442	100	100	100.0	1118240	PASS
443	442	15	24	19.8	221205	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072225\
Data File : BP025206.D
Acq On : 22 Jul 2025 09:04
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Jul 22 11:04:29 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP072125.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 22 02:55:21 2025
Response via : Initial Calibration

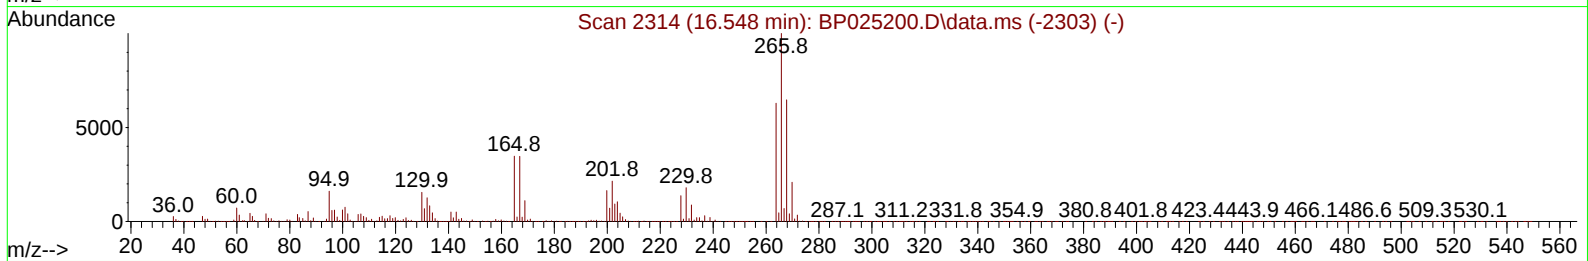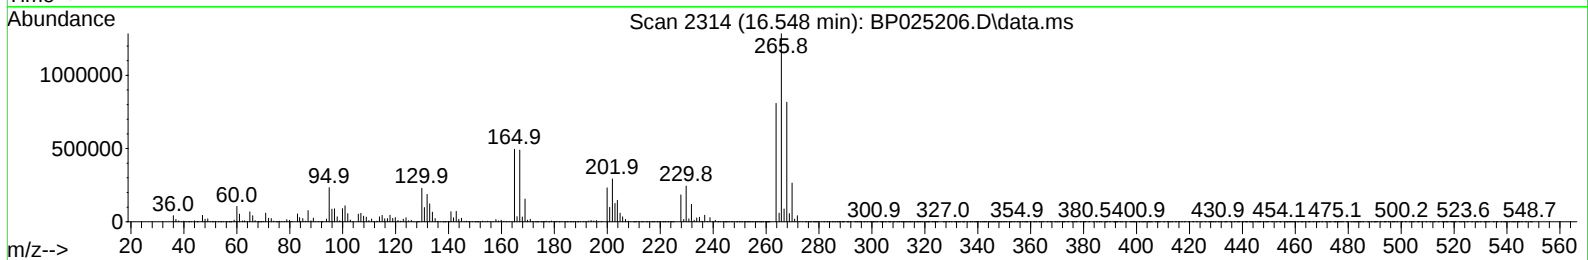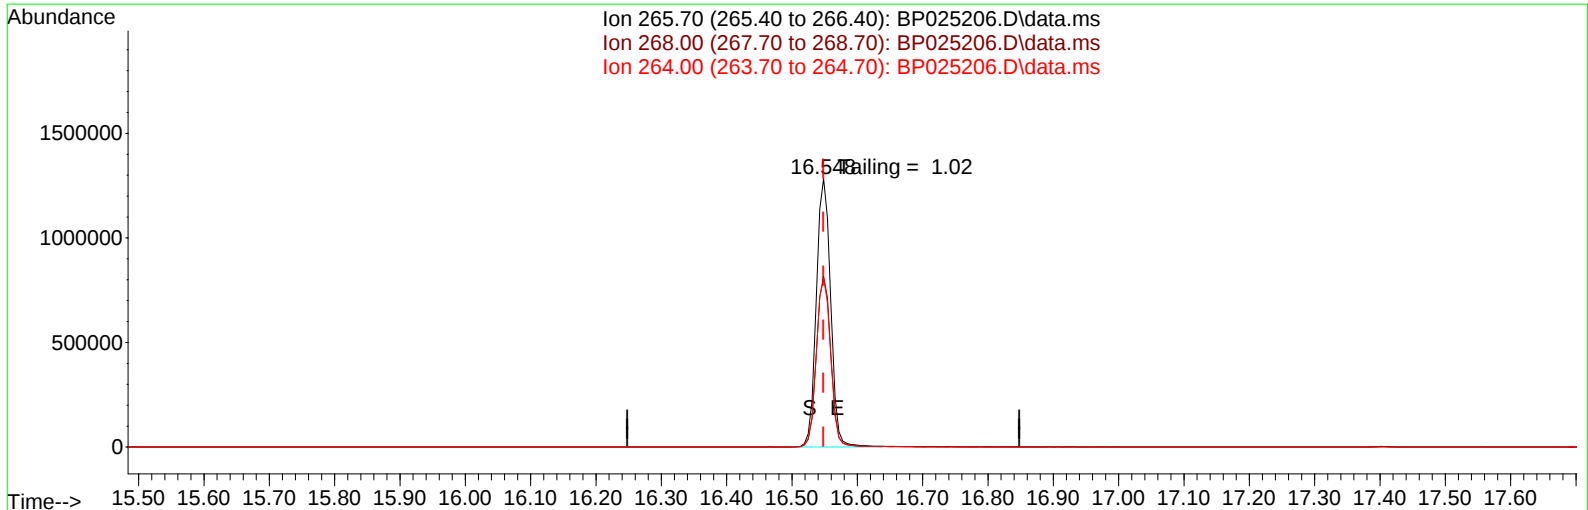

TIC: BP025206.D\data.ms

(70) Pentachlorophenol (C)

16.548min (+ 0.000) 665481.51 ng




response 1963129

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.70	63.58
264.00	62.90	63.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072225\
Data File : BP025206.D
Acq On : 22 Jul 2025 09:04
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Jul 22 11:04:29 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP072125.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 22 02:55:21 2025
Response via : Initial Calibration

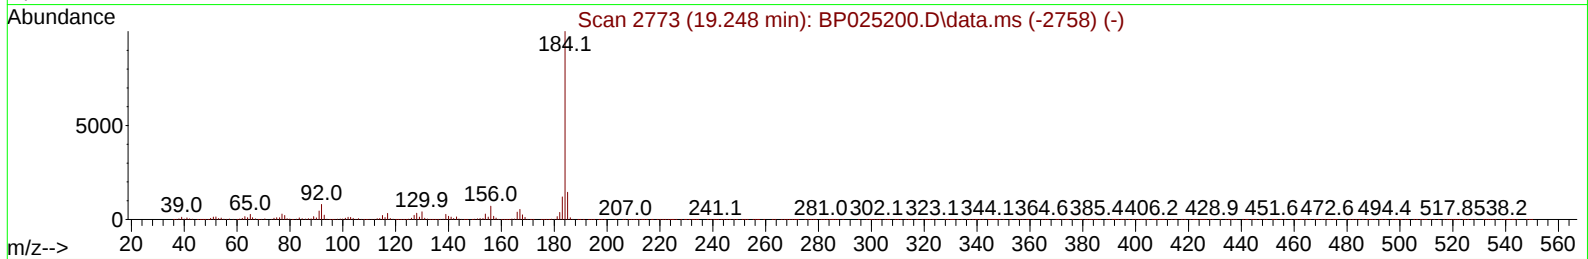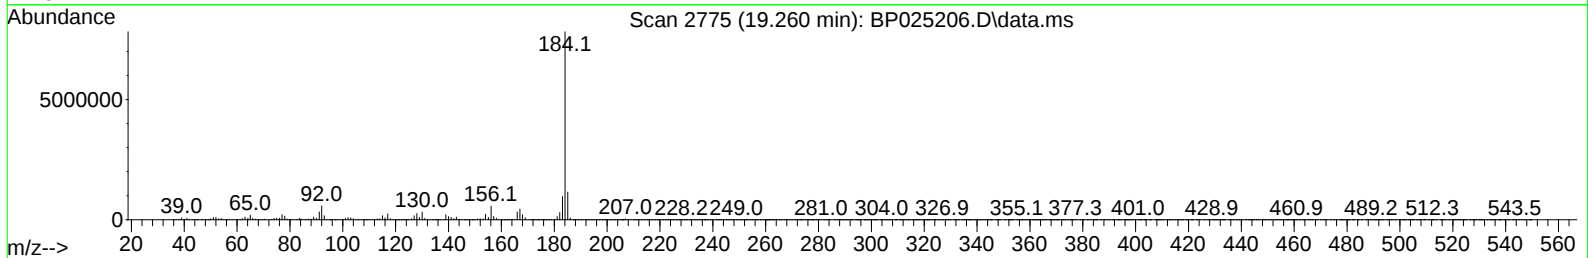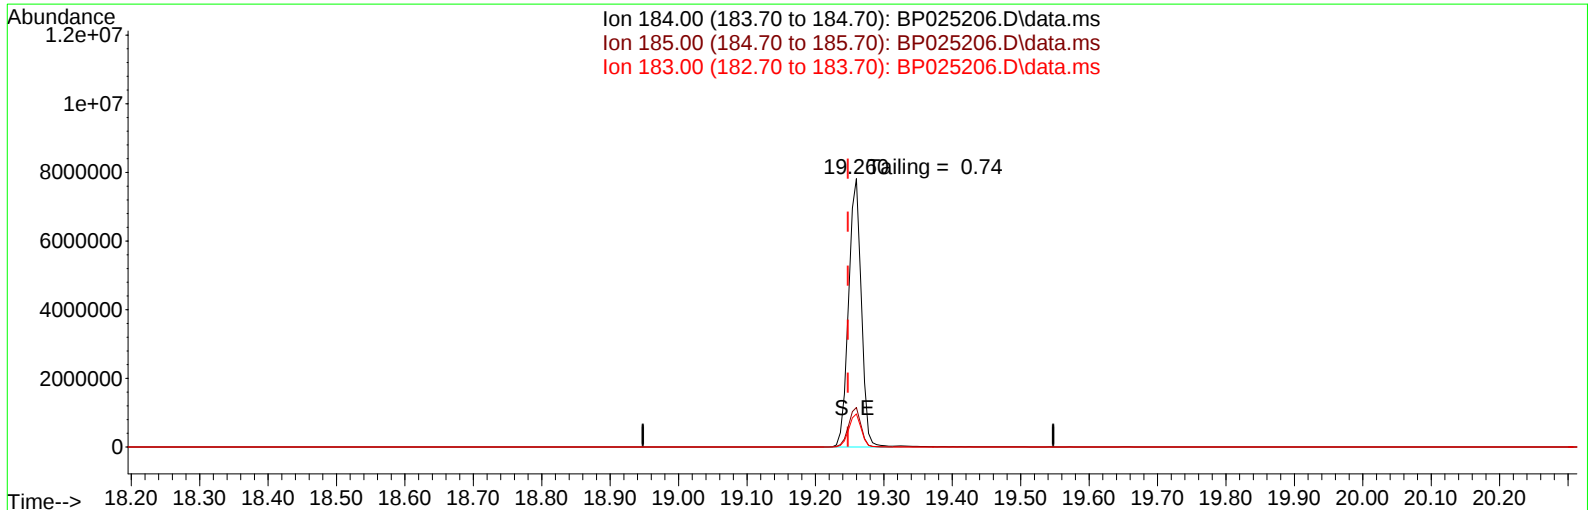

TIC: BP025206.D\data.ms

(77) Benzidine

19.260min (+ 0.012) 1969.03 ng

response 10060052

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.73
183.00	12.00	12.36
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
7/22/2025	BNA_P	<u>BP025206.D</u>
Compound Name	Response	Retention Time
DDT	4798982	20.572
DDD	87623	20.107
DDE	7575	19.578
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
95198	4894180	1.95

Instrument :
BNA_P
ClientSampleId :
DFTPP