
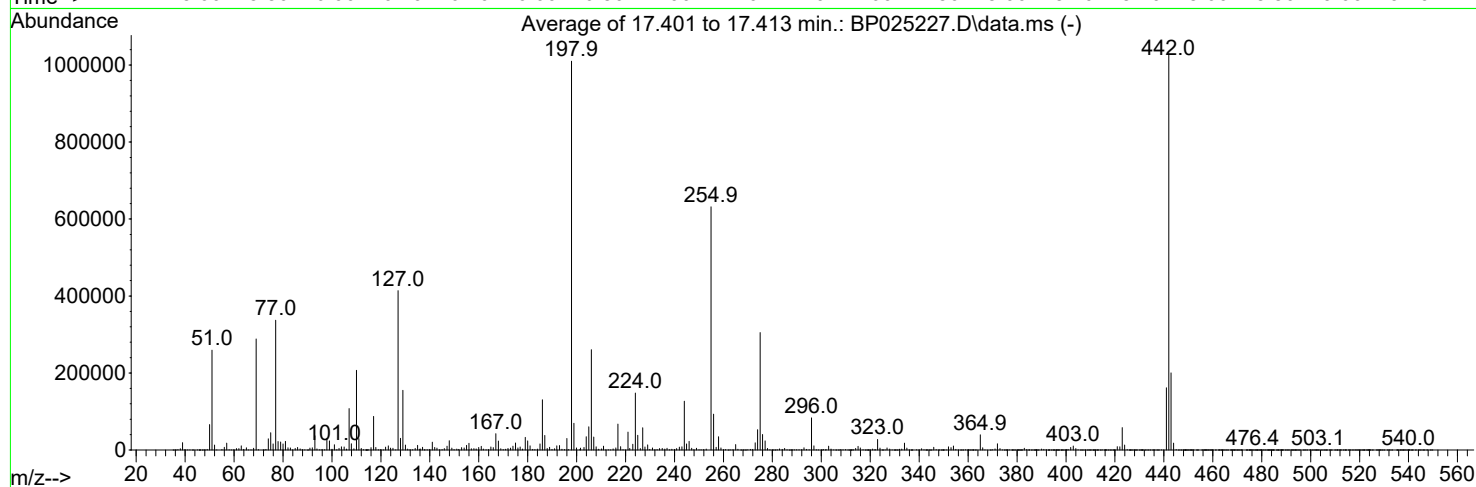


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072325\
Data File : BP025227.D
Acq On : 23 Jul 2025 16:54
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP072125.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Jul 22 02:55:21 2025

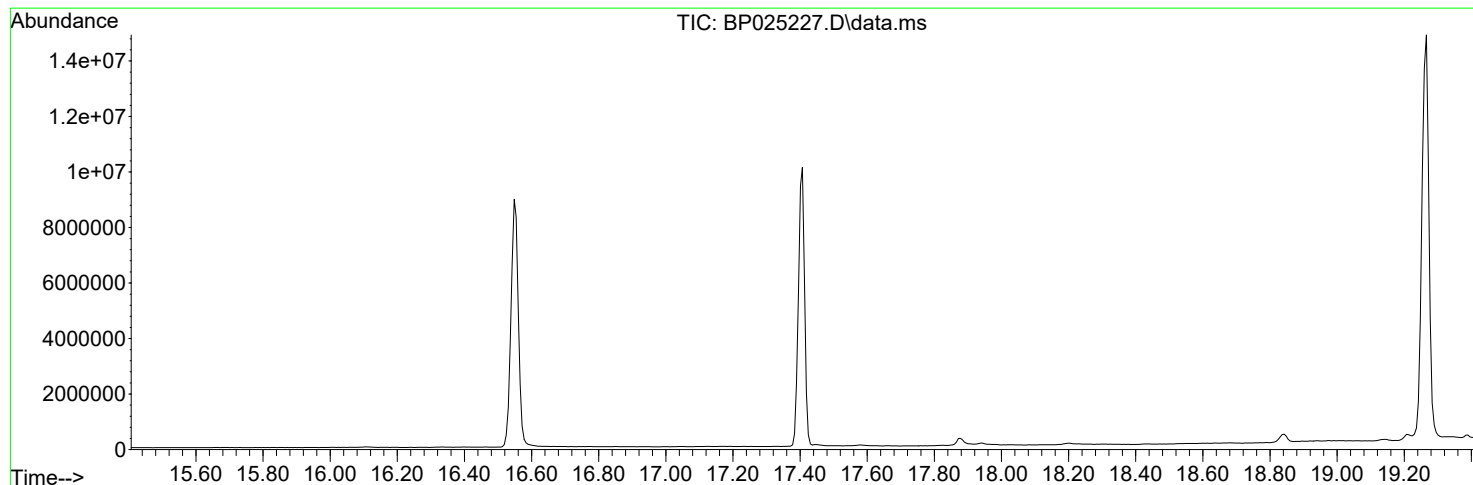

AutoFind: Scans 2459, 2460, 2461; Background Corrected with Scan 2450

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	1.6	4506	PASS
69	69	100	100	100.0	288431	PASS
70	69	0.00	2	0.5	1388	PASS
197	198	0.00	2	0.1	1198	PASS
198	198	100	100	100.0	1009879	PASS
199	198	5	9	6.9	69387	PASS
365	198	1	100	3.9	39603	PASS
441	443	0.01	150	80.8	161870	PASS
442	442	100	100	100.0	1025700	PASS
443	442	15	24	19.5	200403	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
7/23/2025	BNA_P	<u>BP025227.D</u>
Compound Name	Response	Retention Time
DDT	2433989	20.572
DDD	1509314	20.101
DDE	4496	19.577
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
1513810	3947799	38.35

Instrument :
BNA_P
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072325\
Data File : BP025227.D
Acq On : 23 Jul 2025 16:54
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Jul 23 17:14:32 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP072125.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 22 02:55:21 2025
Response via : Initial Calibration

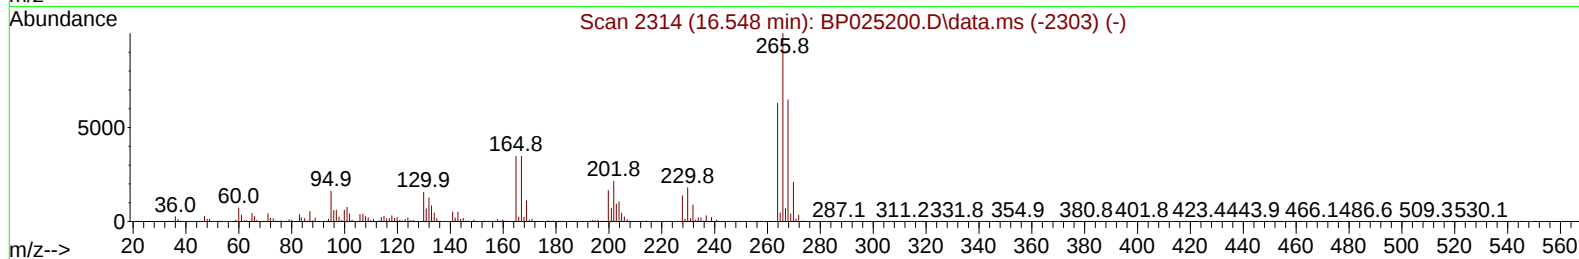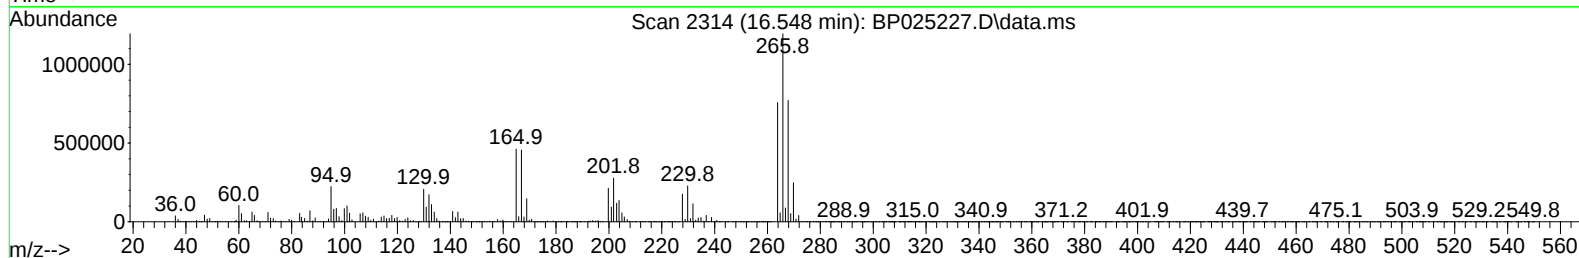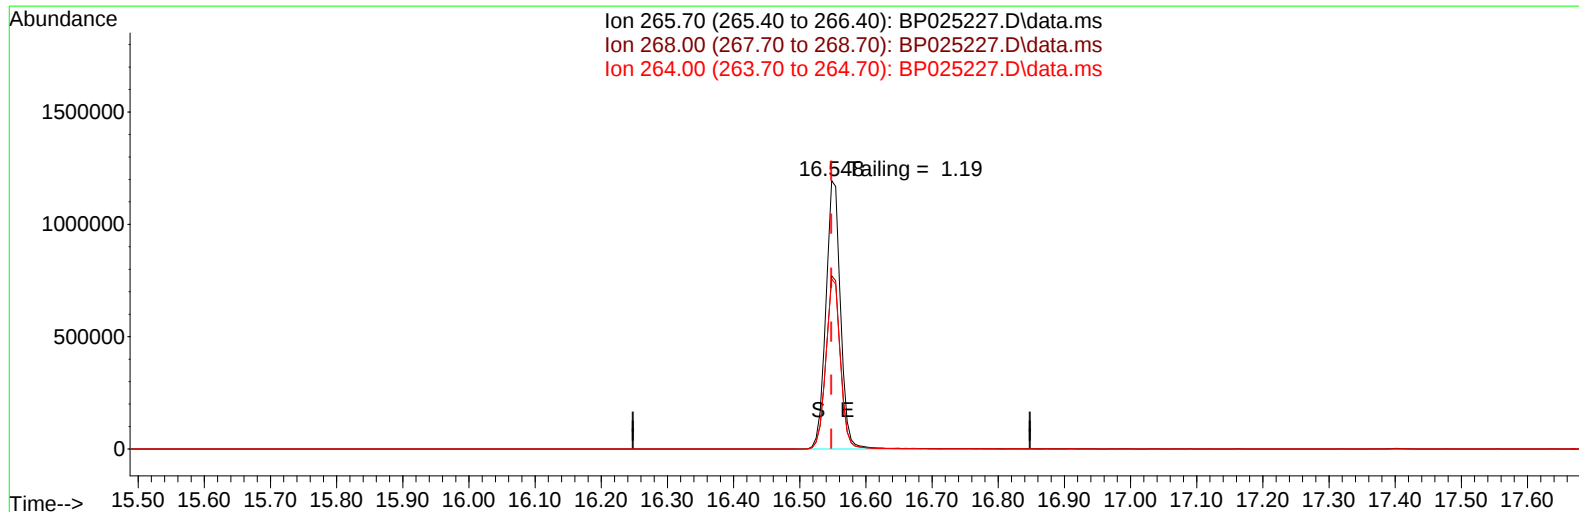

TIC: BP025227.D\data.ms

(70) Pentachlorophenol (C)

16.548min (+ 0.000) 694149.25 ng m




response 1844890

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.70	64.51
264.00	62.90	63.41
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072325\
Data File : BP025227.D
Acq On : 23 Jul 2025 16:54
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Jul 23 17:14:32 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP072125.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 22 02:55:21 2025
Response via : Initial Calibration

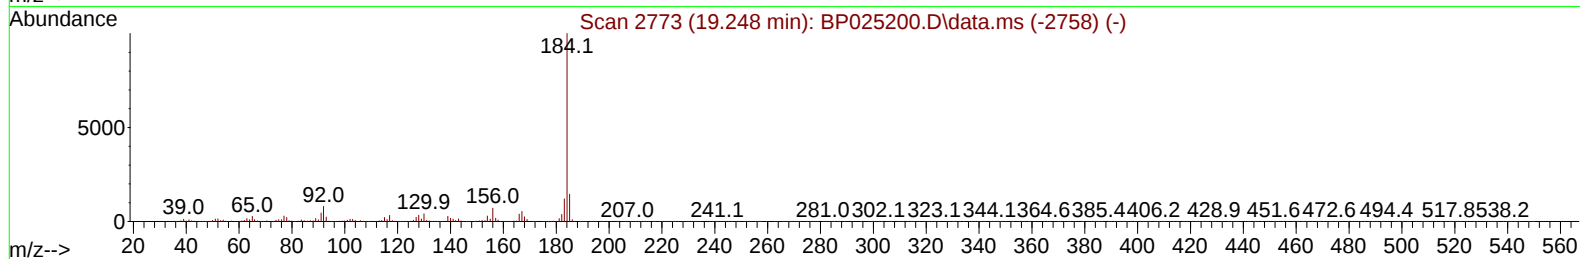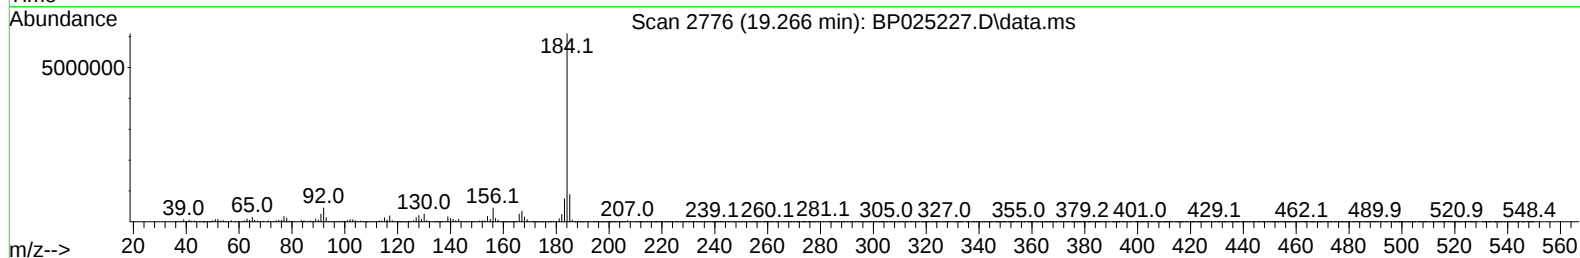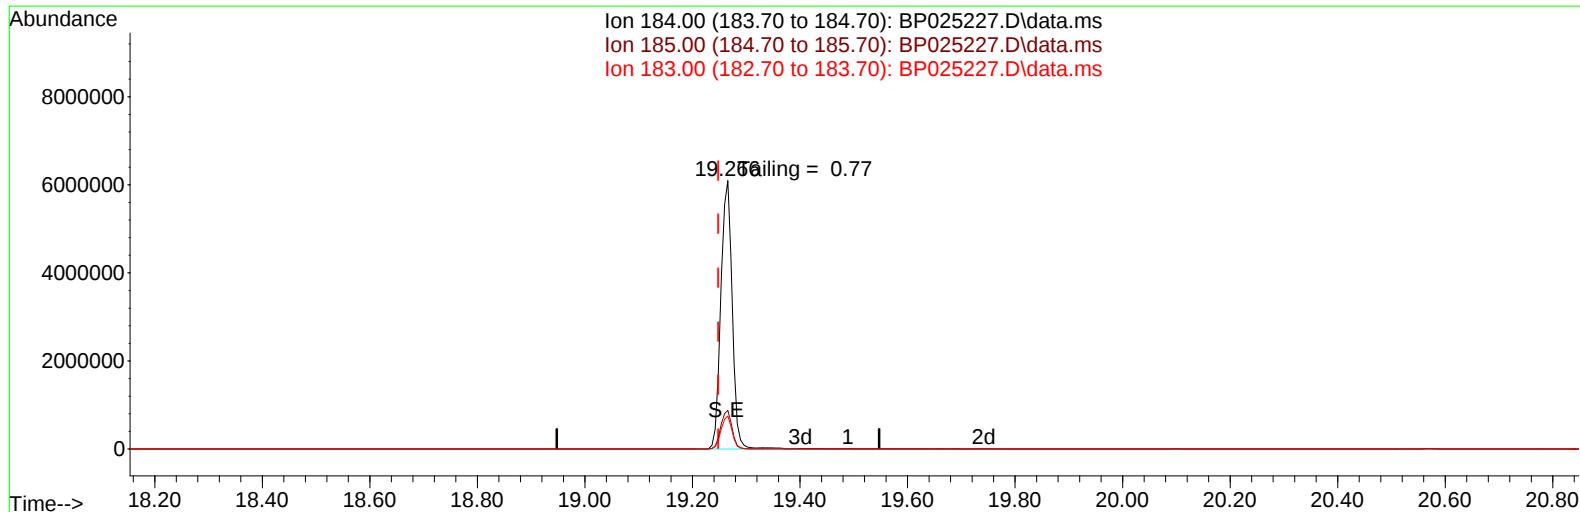

TIC: BP025227.D\data.ms

(77) Benzidine

19.266min (+ 0.018) 273382.31 ng m

response 9089196

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.46
183.00	12.00	12.30
0.00	0.00	0.00