

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072225\
Data File : BF143178.D
Acq On : 22 Jul 2025 09:15
Operator : RC/JU
Sample : PB168929BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB168929BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF071725.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF143178.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.216	507	514	526	rBV	264026	445994	9.53%	1.493%
2	5.604	573	580	585	rBV	2657887	3835507	82.00%	12.836%
3	6.581	739	746	752	rBV	2550099	3862431	82.57%	12.926%
4	6.963	805	811	816	rBV	712481	872004	18.64%	2.918%
5	7.516	898	905	911	rBV	1831742	2646160	56.57%	8.856%
6	8.240	1022	1028	1034	rBV	857445	1151835	24.62%	3.855%
7	9.316	1204	1211	1217	rBV	3322918	4677534	100.00%	15.654%
8	9.998	1321	1327	1332	rBV	1030254	1270956	27.17%	4.253%
9	10.786	1455	1461	1466	rBV	2223765	2898347	61.96%	9.700%
10	11.486	1574	1580	1585	rBV	1078380	1345689	28.77%	4.503%
11	13.069	1843	1849	1855	rBV	3304967	4583932	98.00%	15.341%
12	14.122	2023	2028	2036	rBV	687637	871593	18.63%	2.917%
13	15.627	2278	2284	2297	rBV	474095	771062	16.48%	2.580%
14	17.533	2598	2608	2632	rVB	126407	647987	13.85%	2.169%




Sum of corrected areas: 29881031

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072225\
Data File : BF143178.D
Acq On : 22 Jul 2025 09:15
Operator : RC/JU
Sample : PB168929BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB168929BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF071725.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

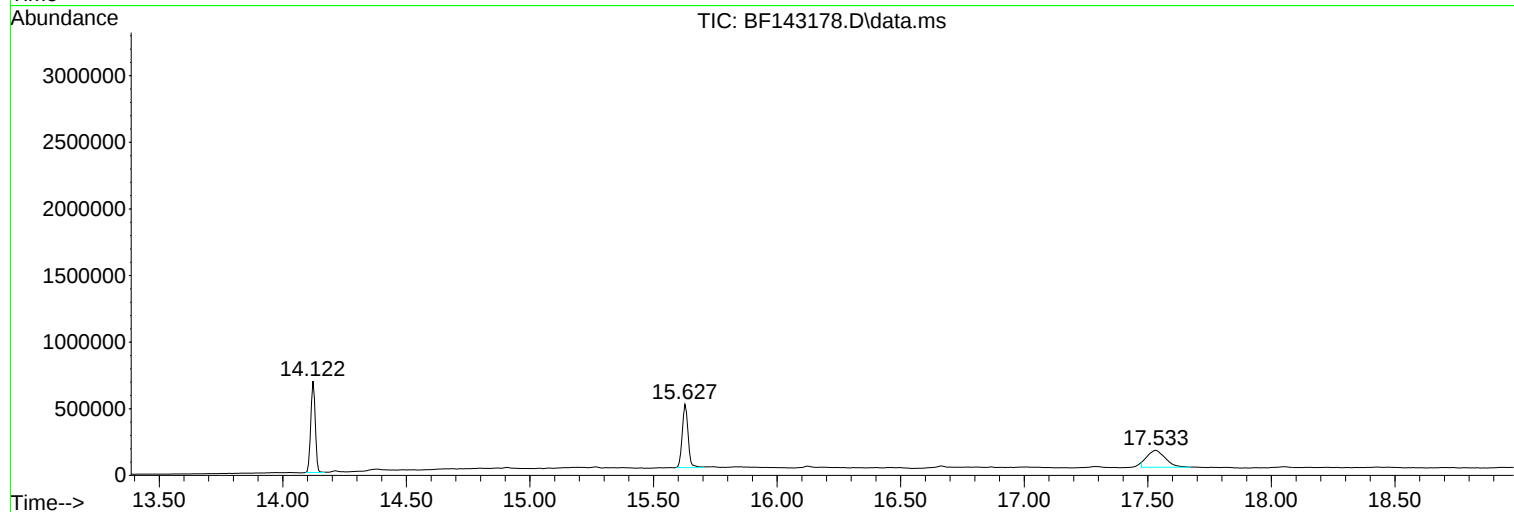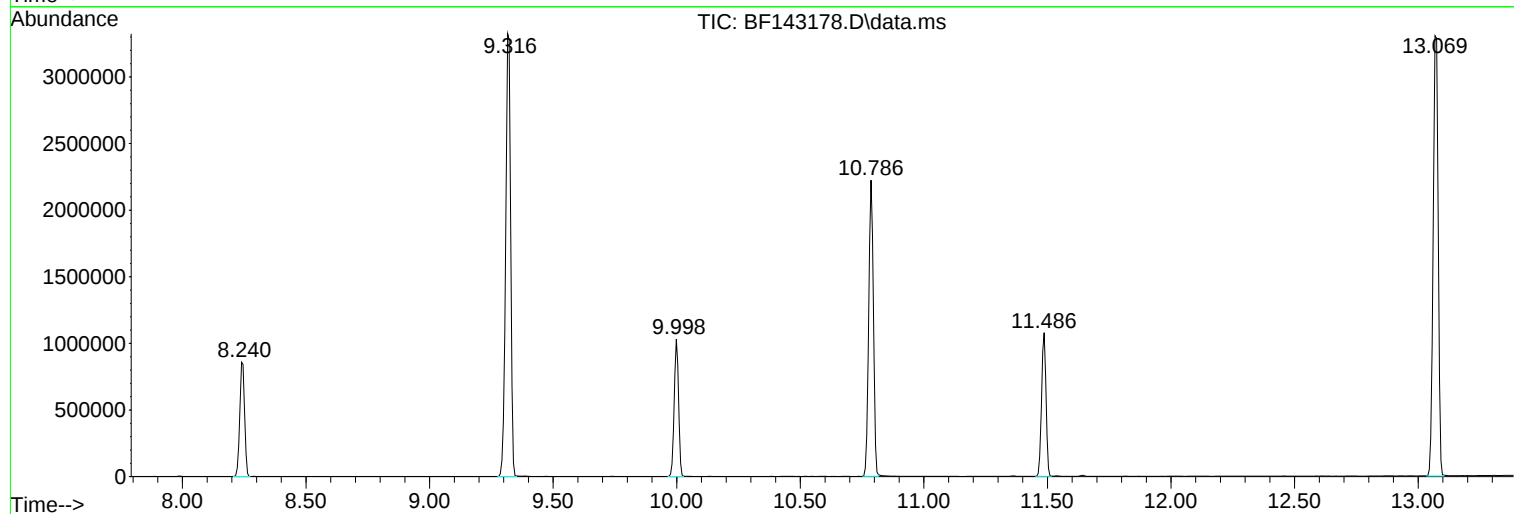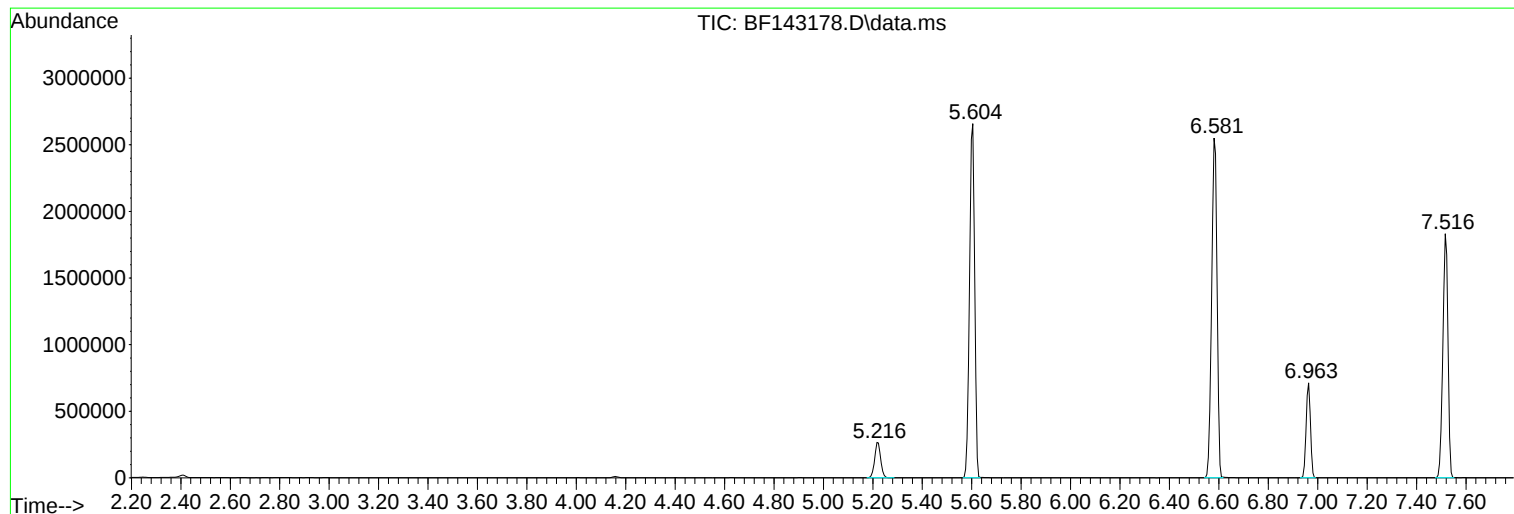

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072225\
Data File : BF143178.D
Acq On : 22 Jul 2025 09:15
Operator : RC/JU
Sample : PB168929BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB168929BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF071725.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072225\
Data File : BF143178.D
Acq On : 22 Jul 2025 09:15
Operator : RC/JU
Sample : PB168929BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB168929BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF071725.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------