

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072325\
 Data File : BP025222.D
 Acq On : 23 Jul 2025 13:28
 Operator : CG/JU
 Sample : Q2639-01
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 OU4-TS-38-071725

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP072125.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP025222.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.655	287	292	300	rVB	352649	486948	3.10%	0.380%
2	5.102	362	368	381	rBV	4207658	5829832	37.17%	4.547%
3	6.637	623	629	644	rVB	4000562	6350698	40.49%	4.953%
4	7.437	758	765	773	rBV	1842796	2726423	17.38%	2.126%
5	8.560	948	956	968	rBV	2516794	4173668	26.61%	3.255%
6	10.178	1223	1231	1237	rBV	2454727	4053727	25.85%	3.162%
7	12.672	1648	1655	1670	rVB	6523894	10727744	68.40%	8.367%
8	13.525	1791	1800	1807	rBV3	81251	224346	1.43%	0.175%
9	13.795	1840	1846	1855	rVB	218758	435494	2.78%	0.340%
10	14.078	1887	1894	1902	rBV	3568124	6054395	38.60%	4.722%
11	14.984	2043	2048	2056	rVB	83403	167784	1.07%	0.131%
12	15.172	2072	2080	2083	rBV	79957	164152	1.05%	0.128%
13	15.484	2127	2133	2142	rVB	851769	1287326	8.21%	1.004%
14	15.613	2148	2155	2163	rBV	6318785	9211122	58.73%	7.184%
15	16.895	2368	2373	2377	rBV2	5353529	7138691	45.52%	5.568%
16	16.931	2377	2379	2385	rVB	489934	546108	3.48%	0.426%
17	17.042	2388	2398	2403	rVB2	246710	626486	3.99%	0.489%
18	17.825	2523	2531	2534	rBV3	187076	465753	2.97%	0.363%
19	17.884	2534	2541	2548	rBV2	3396238	5496224	35.04%	4.287%
20	17.995	2556	2560	2564	rBV2	321771	537330	3.43%	0.419%
21	18.172	2587	2590	2599	rBV8	166352	316512	2.02%	0.247%
22	18.307	2610	2613	2615	rBV	125867	164397	1.05%	0.128%
23	18.713	2680	2682	2687	rBV5	162291	286233	1.83%	0.223%
24	18.772	2690	2692	2698	rVB2	356284	532056	3.39%	0.415%
25	18.919	2714	2717	2719	rBV3	192937	256949	1.64%	0.200%
26	18.948	2720	2722	2731	rVB2	284941	456270	2.91%	0.356%
27	19.042	2734	2738	2742	rBV	1728644	2326528	14.83%	1.815%
28	19.142	2752	2755	2761	rBV7	237566	493583	3.15%	0.385%
29	19.225	2765	2769	2774	rVB	868919	1257093	8.02%	0.980%
30	19.425	2796	2803	2807	rBV	1676827	2297712	14.65%	1.792%
31	19.660	2838	2843	2854	rVB	10604588	15683562	100.00%	12.232%
32	20.266	2944	2946	2950	rVB	451135	504143	3.21%	0.393%
33	20.966	3062	3065	3069	rVB2	684652	847770	5.41%	0.661%
34	21.066	3078	3082	3089	rVB2	1515910	2250328	14.35%	1.755%
35	21.342	3122	3129	3133	rBV3	5962286	10722049	68.36%	8.363%
36	21.377	3133	3135	3142	rVB	1831842	2617353	16.69%	2.041%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072325\
Data File : BP025222.D
Acq On : 23 Jul 2025 13:28
Operator : CG/JU
Sample : Q2639-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
OU4-TS-38-071725

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP072125.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	22.254	3280	3284	3292	rVB3	1268652	2365680	15.08%	1.845%
38	23.748	3533	3538	3545	rBV	2332506	4849255	30.92%	3.782%
39	24.483	3655	3663	3670	rVB	3293977	8298285	52.91%	6.472%
40	25.842	3887	3894	3903	rVB	1634932	4985341	31.79%	3.888%




Sum of corrected areas: 128215350

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072325\
Data File : BP025222.D
Acq On : 23 Jul 2025 13:28
Operator : CG/JU
Sample : Q2639-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
OU4-TS-38-071725

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP072125.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

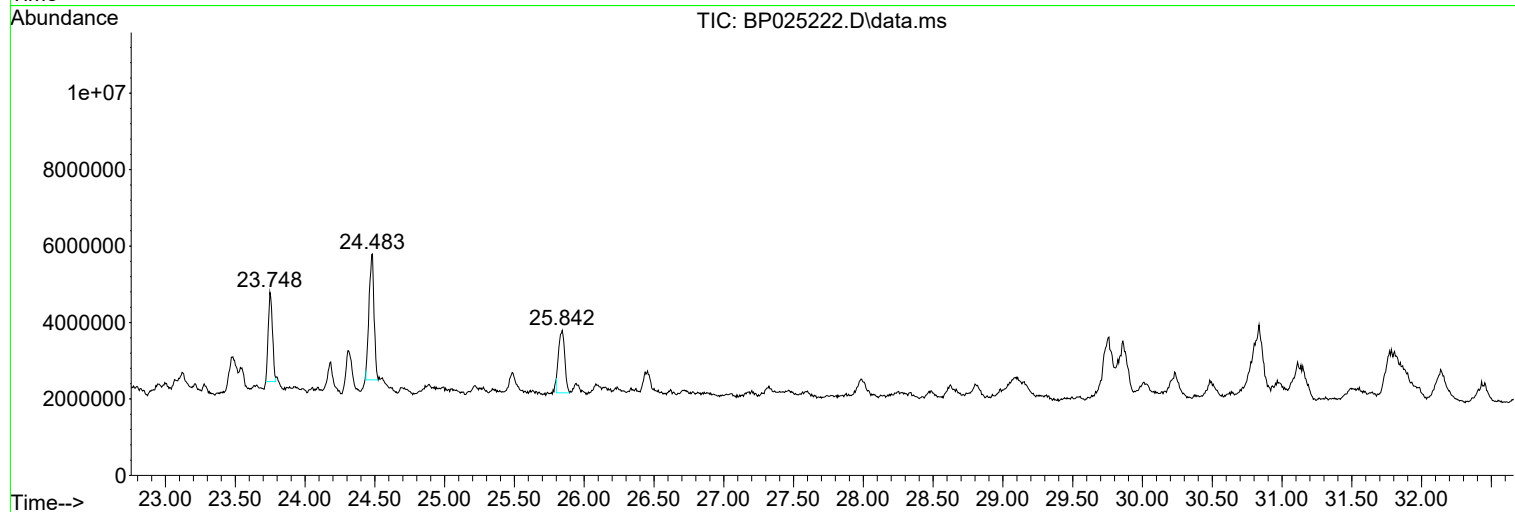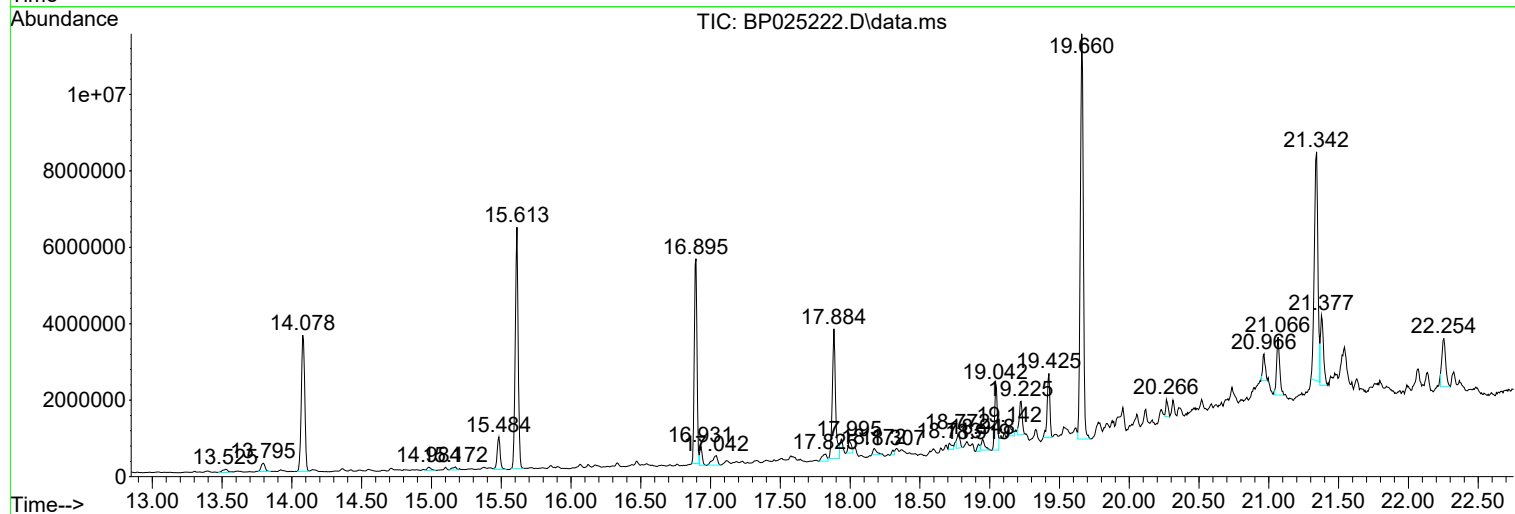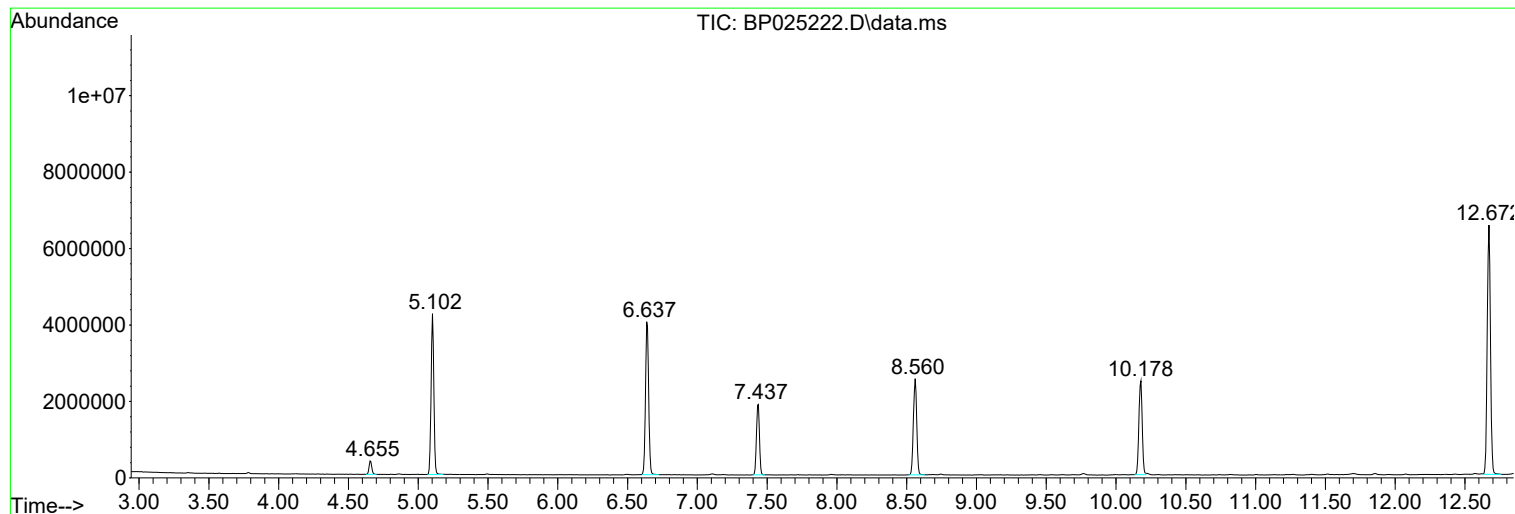

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072325\
Data File : BP025222.D
Acq On : 23 Jul 2025 13:28
Operator : CG/JU
Sample : Q2639-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
OU4-TS-38-071725

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP072125.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072325\
Data File : BP025222.D
Acq On : 23 Jul 2025 13:28
Operator : CG/JU
Sample : Q2639-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
OU4-TS-38-071725

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP072125.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------