

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072325\
 Data File : BP025223.D
 Acq On : 23 Jul 2025 14:09
 Operator : CG/JU
 Sample : Q2639-13
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 OU4-TS-44-071725

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP072125.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP025223.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.660	288	293	299	rBV	576626	743237	4.67%	0.512%
2	5.107	362	369	383	rBV	6078699	8541946	53.66%	5.889%
3	6.637	622	629	642	rBV	5491773	8579709	53.89%	5.915%
4	7.437	758	765	774	rVB	2191264	3422610	21.50%	2.359%
5	8.560	949	956	964	rBV	3829845	6020125	37.82%	4.150%
6	10.178	1223	1231	1241	rBV	2522316	4518495	28.38%	3.115%
7	10.319	1246	1255	1265	rVB	428696	745856	4.69%	0.514%
8	12.684	1650	1657	1664	rBV	9007549	12273906	77.10%	8.461%
9	14.083	1888	1895	1905	rBV	3838770	5289978	33.23%	3.647%
10	15.483	2127	2133	2143	rVB	470400	753266	4.73%	0.519%
11	15.613	2148	2155	2163	rBV	6471482	9196921	57.77%	6.340%
12	16.054	2222	2230	2236	rBV	135294	268279	1.69%	0.185%
13	16.113	2236	2240	2246	rBV2	128864	193935	1.22%	0.134%
14	16.330	2273	2277	2283	rVB2	132830	171087	1.07%	0.118%
15	16.842	2360	2364	2367	rBV	269225	371317	2.33%	0.256%
16	16.895	2367	2373	2379	rVB2	3207978	6009518	37.75%	4.143%
17	17.001	2386	2391	2394	rBV2	160129	243172	1.53%	0.168%
18	17.042	2394	2398	2403	rVB	233145	334956	2.10%	0.231%
19	17.583	2486	2490	2492	rBV	117625	173210	1.09%	0.119%
20	17.789	2522	2525	2527	rVV	155557	167314	1.05%	0.115%
21	17.819	2527	2530	2535	rVB2	197195	226884	1.43%	0.156%
22	17.877	2535	2540	2547	rBV	3493609	4603542	28.92%	3.174%
23	18.160	2584	2588	2591	rBV	593610	695835	4.37%	0.480%
24	18.189	2591	2593	2602	rVB5	195331	361109	2.27%	0.249%
25	18.948	2718	2722	2732	rVB	544898	765553	4.81%	0.528%
26	19.042	2734	2738	2743	rBV	255419	545870	3.43%	0.376%
27	19.101	2744	2748	2750	rBV4	238016	399725	2.51%	0.276%
28	19.230	2767	2770	2778	rVB	1087609	1467236	9.22%	1.011%
29	19.666	2838	2844	2851	rBV	13018055	15919709	100.00%	10.974%
30	20.348	2957	2960	2963	rBV	551214	702556	4.41%	0.484%
31	20.513	2985	2988	2993	rBV	804714	1077788	6.77%	0.743%
32	20.954	3058	3063	3072	rBV7	1295951	3274954	20.57%	2.258%
33	21.060	3077	3081	3091	rVB2	1580120	2537581	15.94%	1.749%
34	21.324	3121	3126	3132	rBV	5229299	8694945	54.62%	5.994%
35	21.448	3141	3147	3153	rVB4	1347057	2721194	17.09%	1.876%
36	21.512	3155	3158	3172	rVB4	1604408	4695854	29.50%	3.237%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072325\
Data File : BP025223.D
Acq On : 23 Jul 2025 14:09
Operator : CG/JU
Sample : Q2639-13
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
OU4-TS-44-071725

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP072125.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	22.236	3276	3281	3290	rVB2	1567462	2994626	18.81%	2.064%
38	23.754	3533	3539	3552	rVB	2940061	7187728	45.15%	4.955%
39	24.465	3653	3660	3670	rBV	3676557	9424327	59.20%	6.497%
40	25.853	3888	3896	3906	rVB2	3009890	8745419	54.93%	6.029%


Sum of corrected areas: 145061272

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072325\
Data File : BP025223.D
Acq On : 23 Jul 2025 14:09
Operator : CG/JU
Sample : Q2639-13
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
OU4-TS-44-071725

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP072125.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

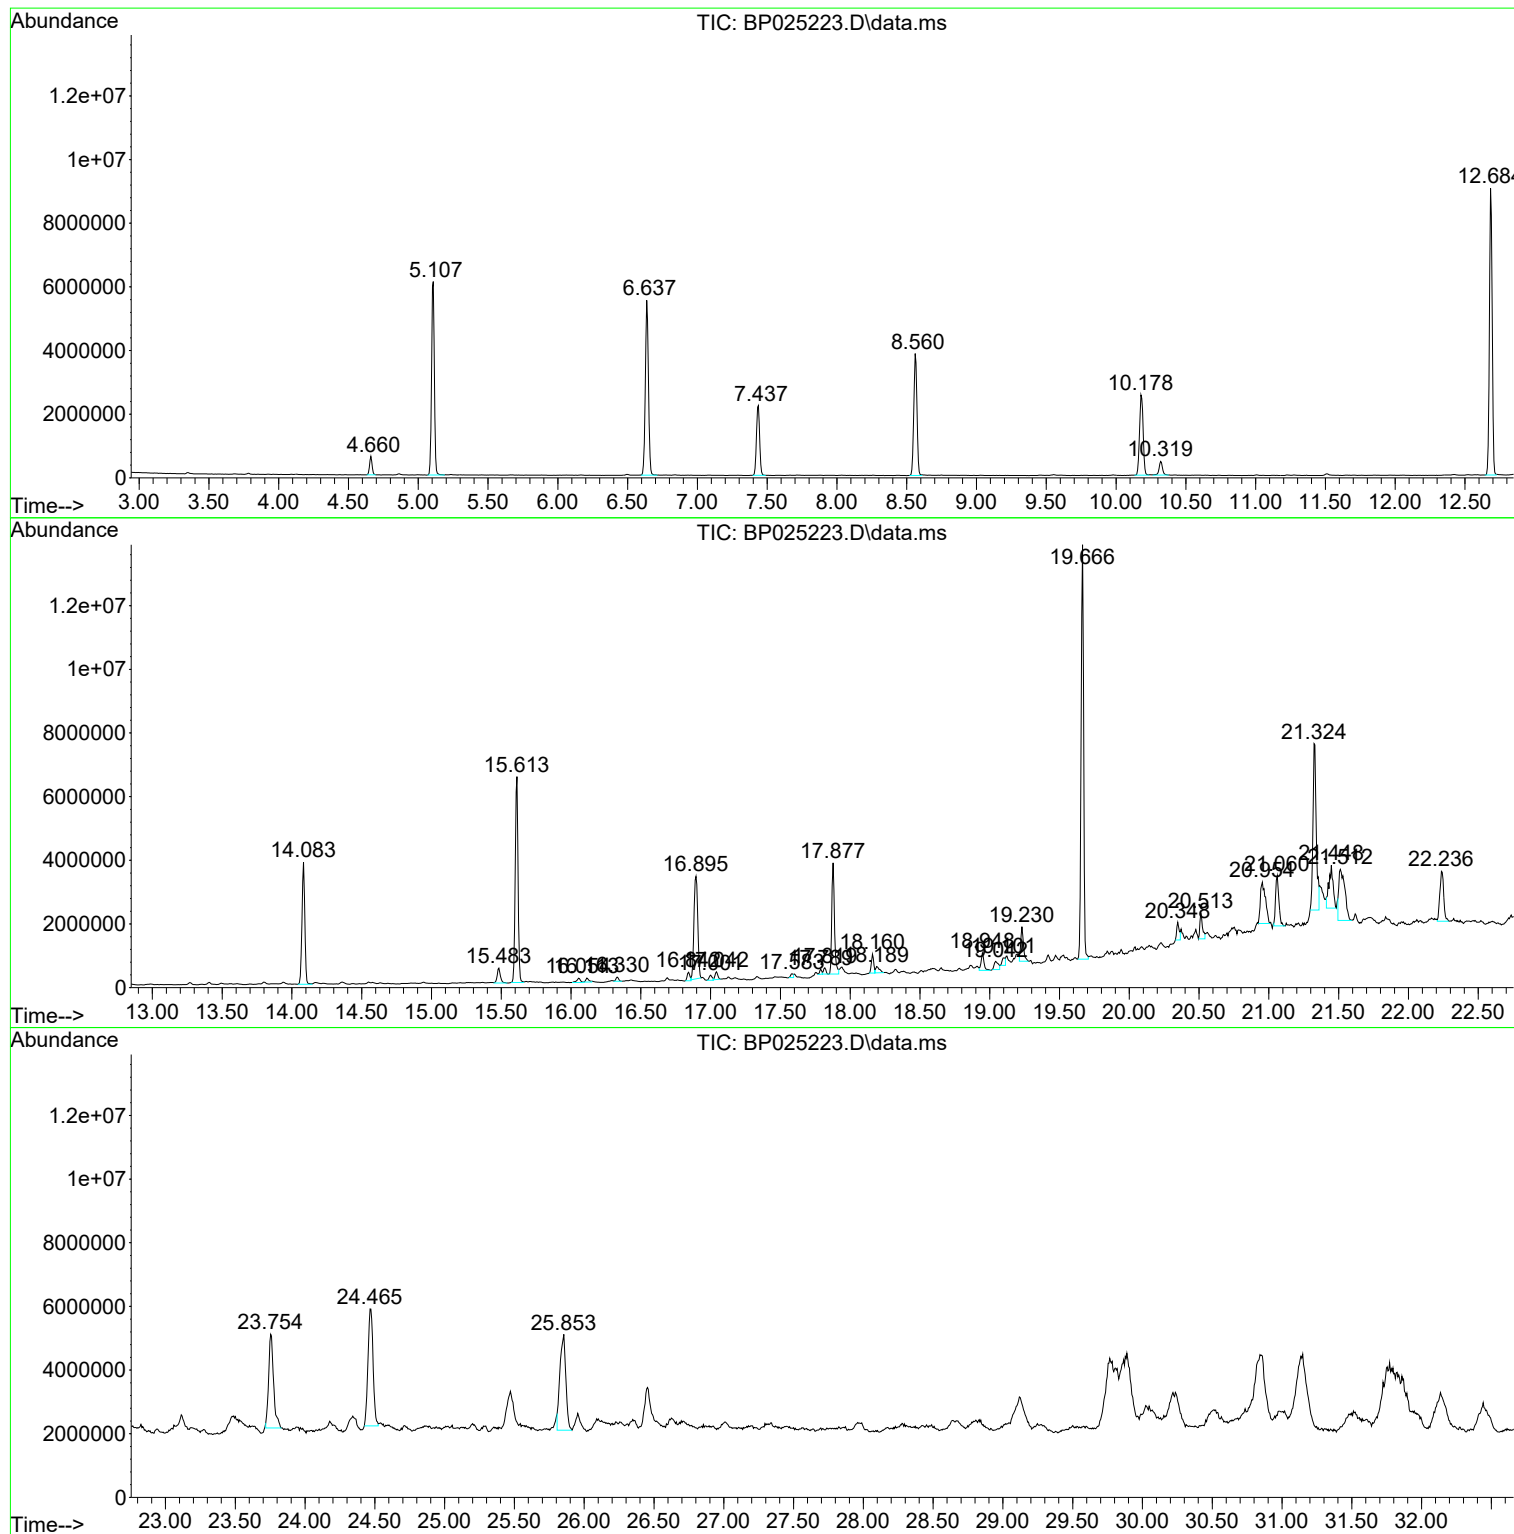

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072325\
Data File : BP025223.D
Acq On : 23 Jul 2025 14:09
Operator : CG/JU
Sample : Q2639-13
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
OU4-TS-44-071725

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP072125.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072325\
Data File : BP025223.D
Acq On : 23 Jul 2025 14:09
Operator : CG/JU
Sample : Q2639-13
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
OU4-TS-44-071725

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP072125.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------