
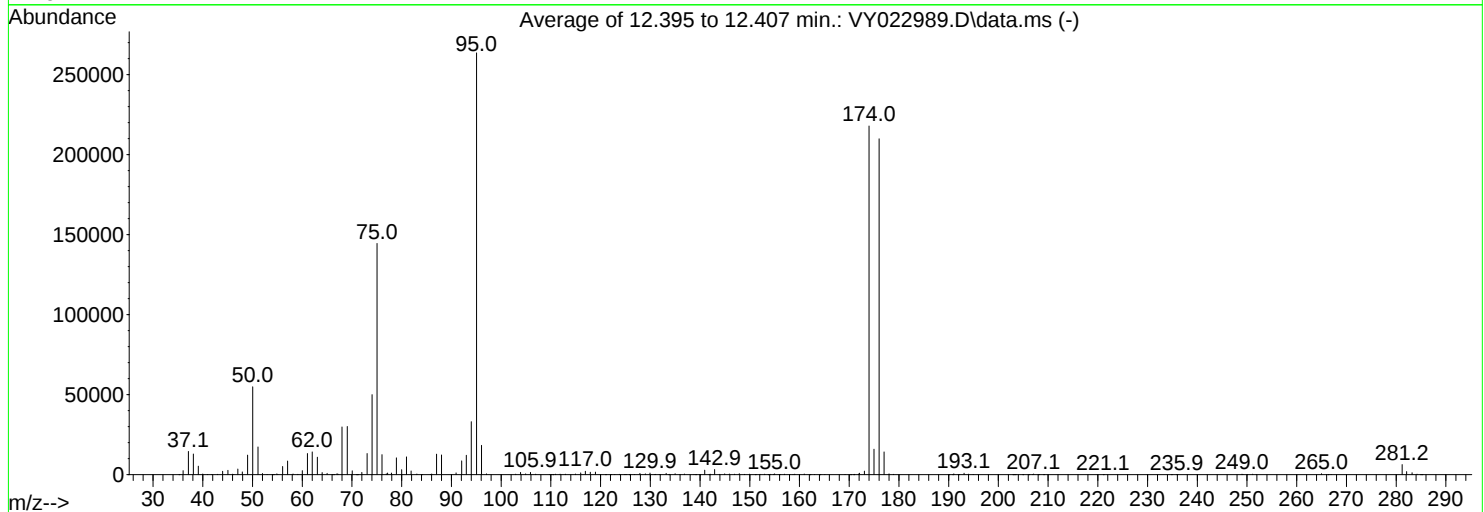


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY071825\
Data File : VY022989.D
Acq On : 18 Jul 2025 09:38
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y071825S.M
Title : SW846 8260
Last Update : Sat Jul 19 01:50:49 2025

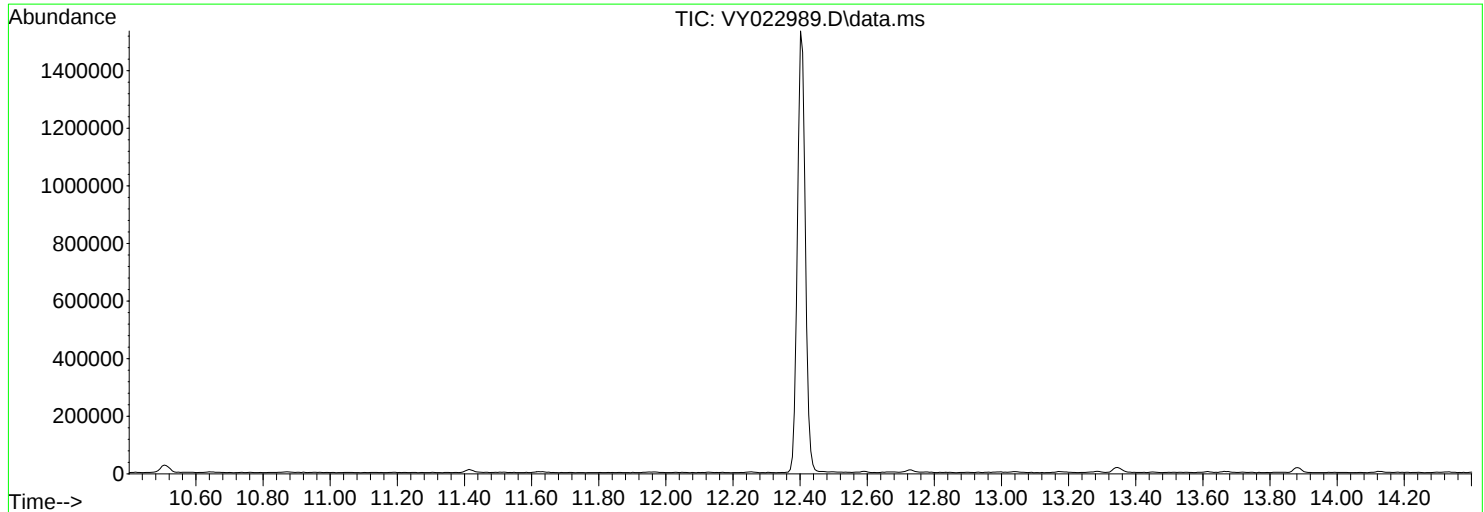

AutoFind: Scans 1751, 1752, 1753; Background Corrected with Scan 1742

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	20.8	54925	PASS
75	95	30	60	54.8	144493	PASS
95	95	100	100	100.0	263616	PASS
96	95	5	9	7.0	18352	PASS
173	174	0.00	2	1.0	2222	PASS
174	95	50	100	82.7	217899	PASS
175	174	5	9	7.3	15902	PASS
176	174	95	101	96.3	209877	PASS
177	176	5	9	6.8	14187	PASS