
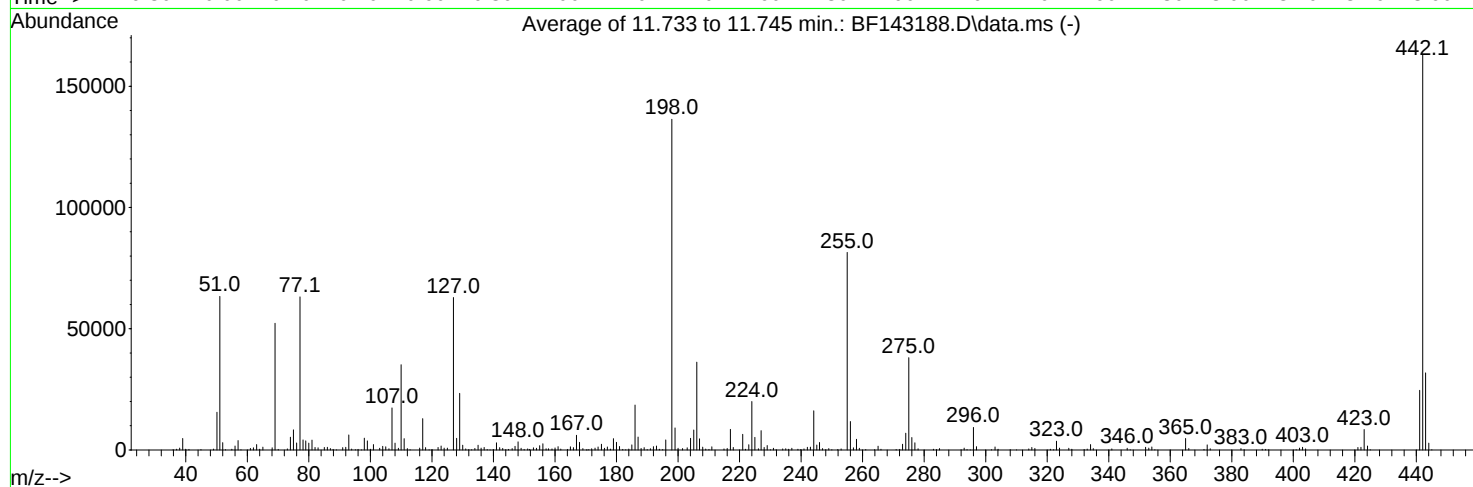


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072225\
 Data File : BF143188.D
 Acq On : 22 Jul 2025 14:54
 Operator : RC/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270E-Tune.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Mar 23 16:55:25 2022

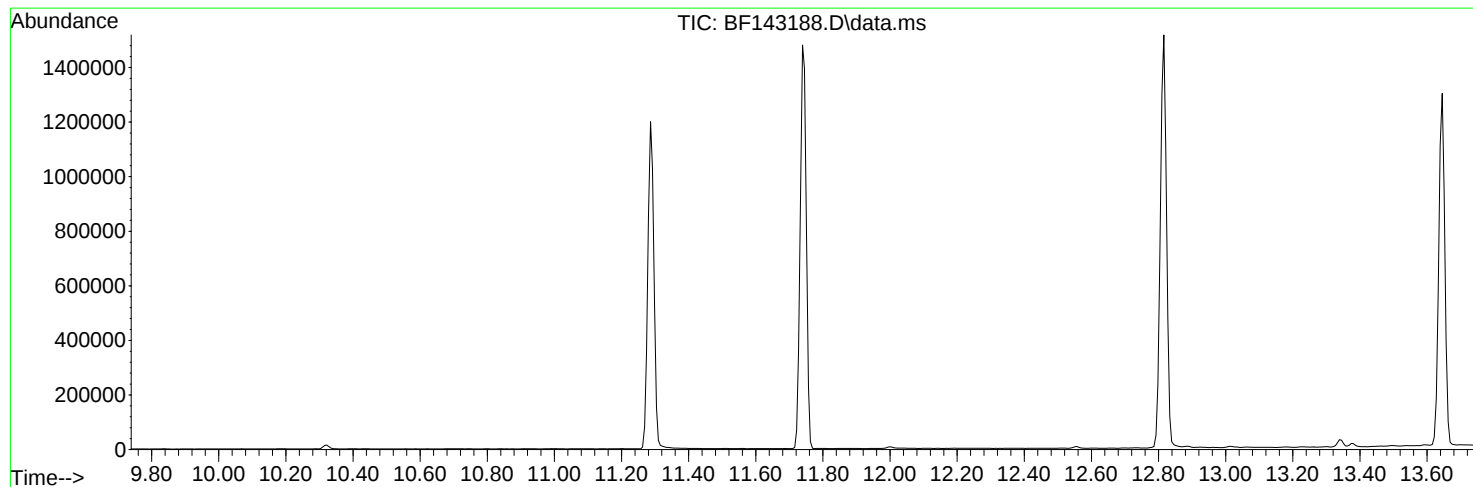




AutoFind: Scans 1622, 1623, 1624; Background Corrected with Scan 1616

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
68	69	0.00	2	1.8	941	PASS
69	69	100	100	100.0	52240	PASS
70	69	0.00	2	0.5	245	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	136379	PASS
199	198	5	9	6.7	9132	PASS
365	198	1	100	3.5	4754	PASS
441	443	0.01	150	77.4	24601	PASS
442	442	100	100	100.0	162824	PASS
443	442	15	24	19.5	31792	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072225\
Data File : BF143188.D
Acq On : 22 Jul 2025 14:54
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jul 22 15:28:42 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF071725.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 17 15:14:05 2025
Response via : Initial Calibration

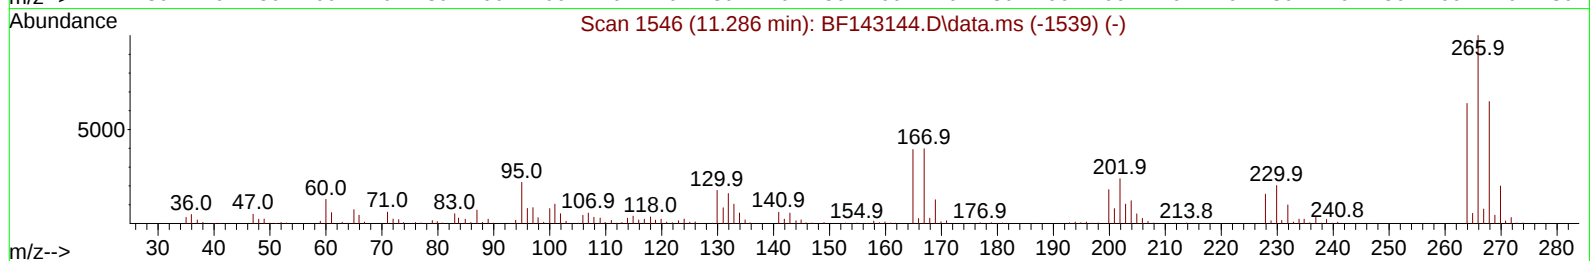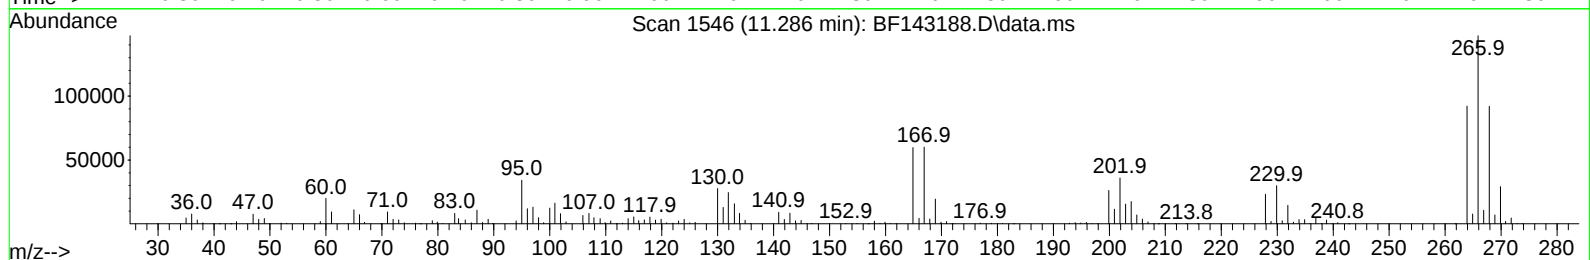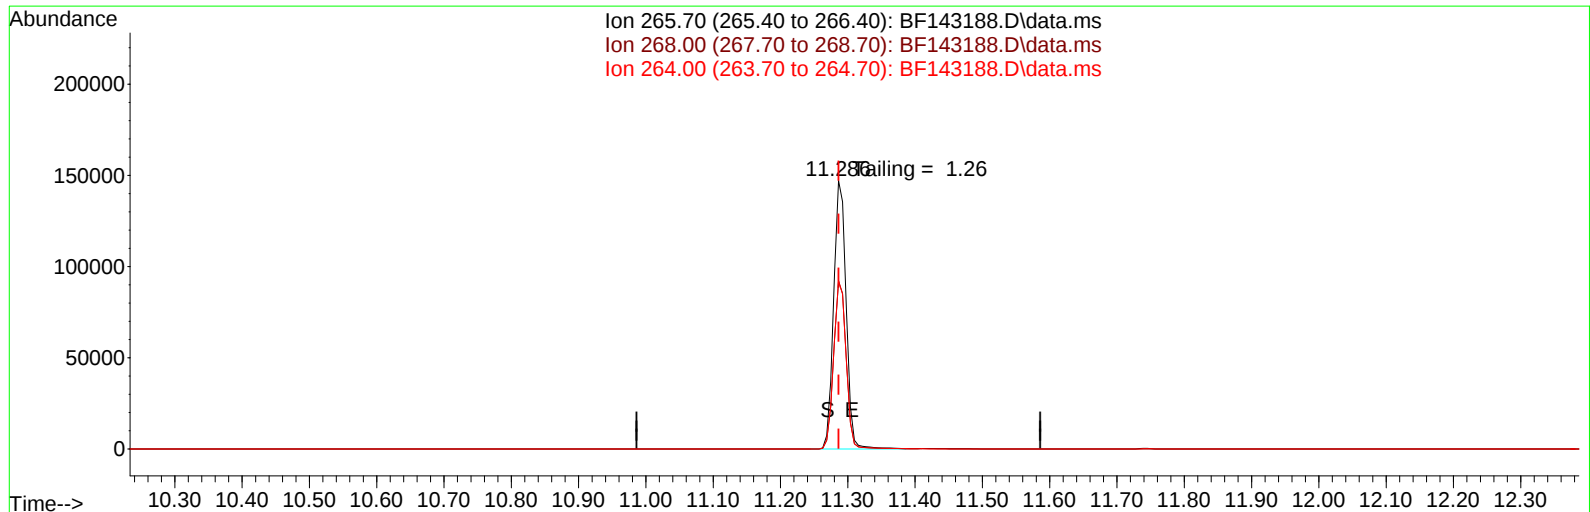

TIC: BF143188.D\data.ms

(70) Pentachlorophenol (C)

11.286min (+ 0.000) 29592.15 ng




response 189456

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.90	62.53
264.00	63.80	62.63
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072225\
Data File : BF143188.D
Acq On : 22 Jul 2025 14:54
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jul 22 15:28:42 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF071725.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 17 15:14:05 2025
Response via : Initial Calibration

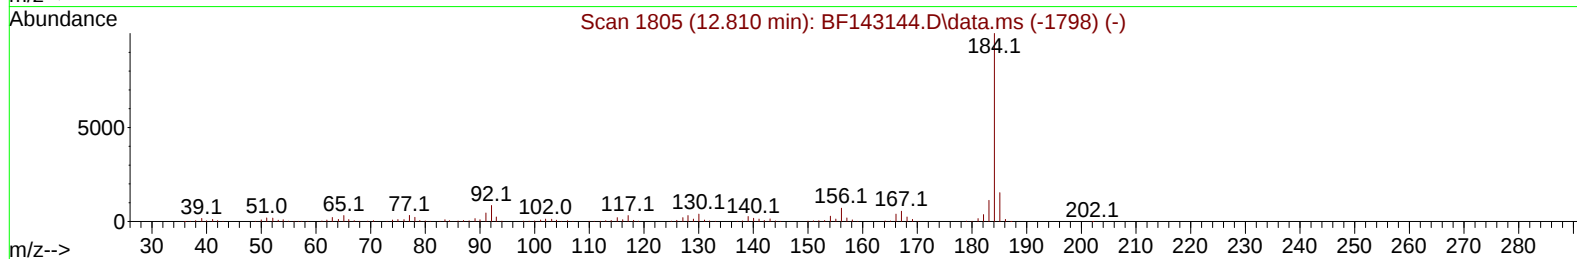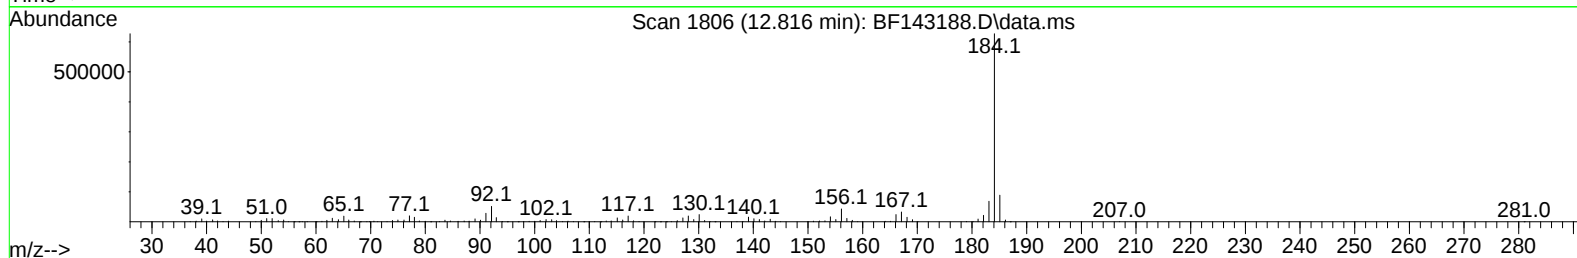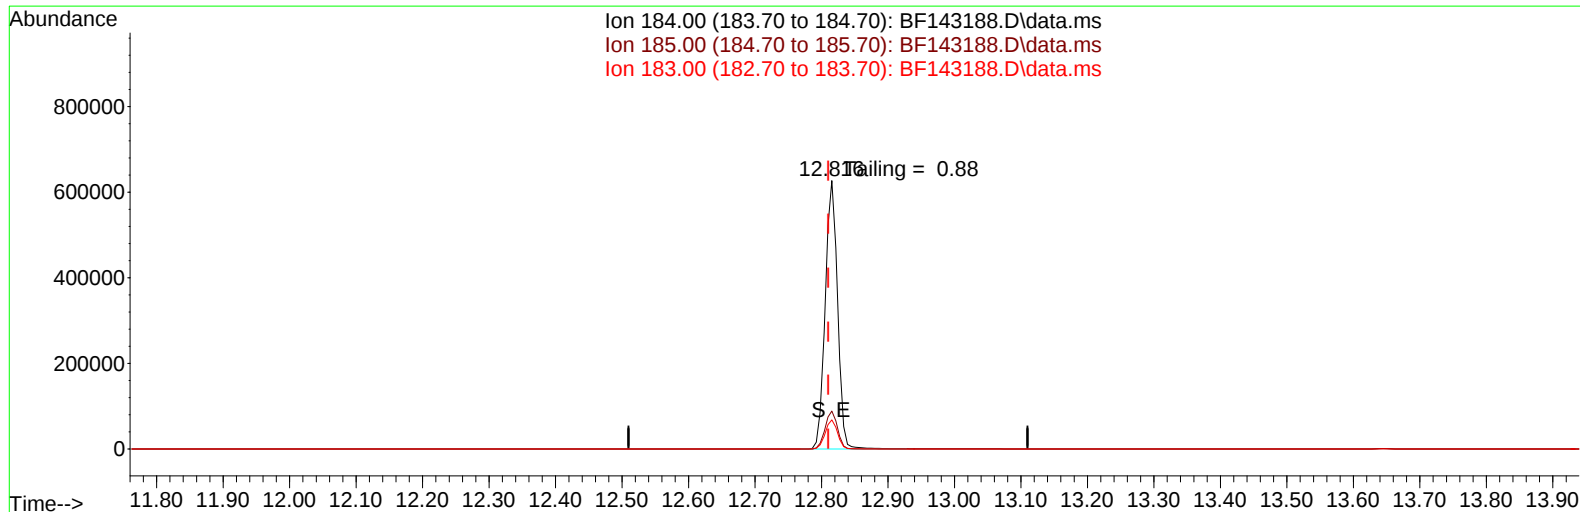

TIC: BF143188.D\data.ms

(77) Benzidine

12.816min (+ 0.006) 0.00 ng

response 811788

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.30	14.15
183.00	11.20	10.89
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
7/22/2025	BNA_F	<u>BF143188.D</u>
Compound Name	Response	Retention Time
DDT	317873	13.645
DDD	10239	13.339
DDE	1665	13.01
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
11904	329777	3.61

Instrument :
BNA_F
ClientSampleId :
DFTPP