


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072325\
Data File : BP025218.D
Acq On : 23 Jul 2025 10:41
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP072125.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Jul 22 02:55:21 2025

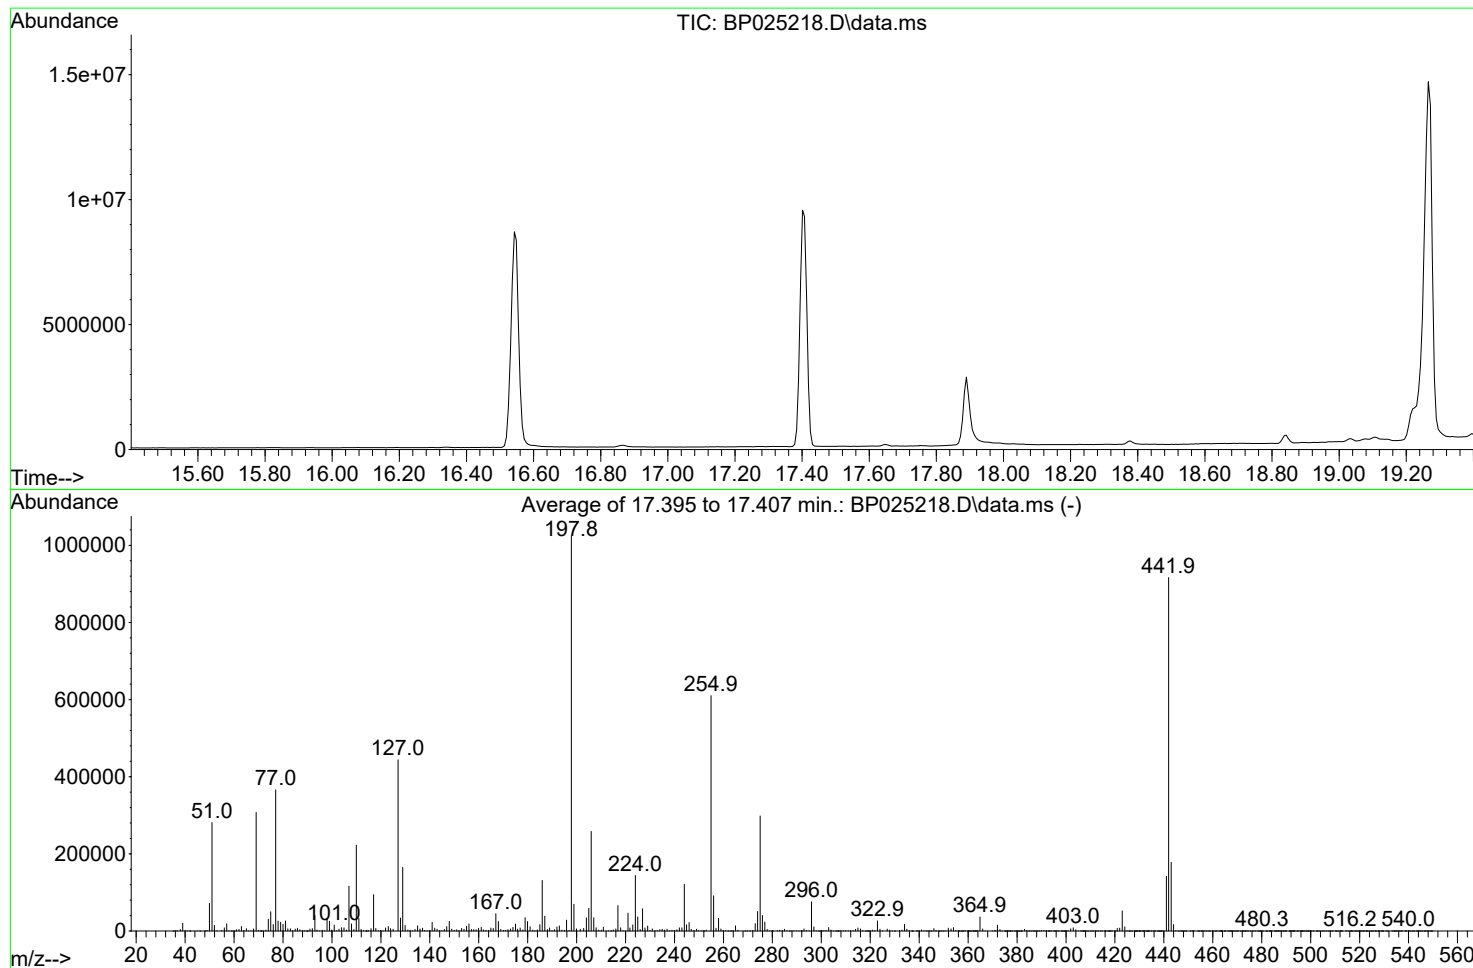

AutoFind: Scans 2458, 2459, 2460; Background Corrected with Scan 2448

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	1.7	5333	PASS
69	69	100	100	100.0	307298	PASS
70	69	0.00	2	0.5	1489	PASS
197	198	0.00	2	0.2	1879	PASS
198	198	100	100	100.0	1023695	PASS
199	198	5	9	6.8	69278	PASS
365	198	1	100	3.6	36590	PASS
441	443	0.01	150	79.6	141723	PASS
442	442	100	100	100.0	916262	PASS
443	442	15	24	19.4	178125	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
7/23/2025	BNA_P	<u>BP025218.D</u>
Compound Name	Response	Retention Time
DDT	4585613	20.578
DDD	91482	20.16
DDE	4697	19.578
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
96179	4681792	2.05

Instrument :
BNA_P
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072325\
Data File : BP025218.D
Acq On : 23 Jul 2025 10:41
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Jul 23 12:04:22 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP072125.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 22 02:55:21 2025
Response via : Initial Calibration

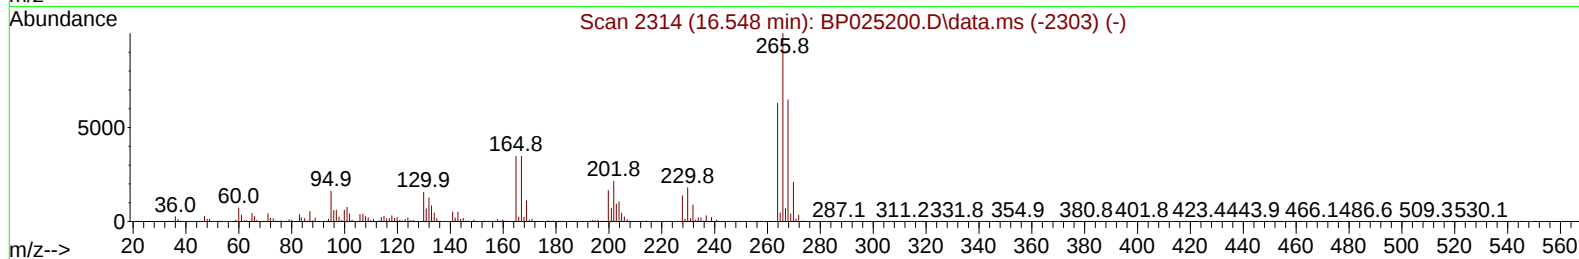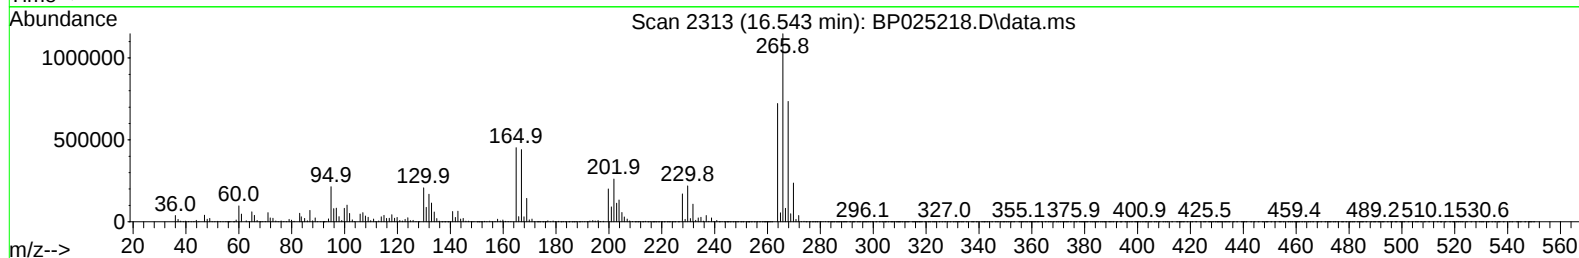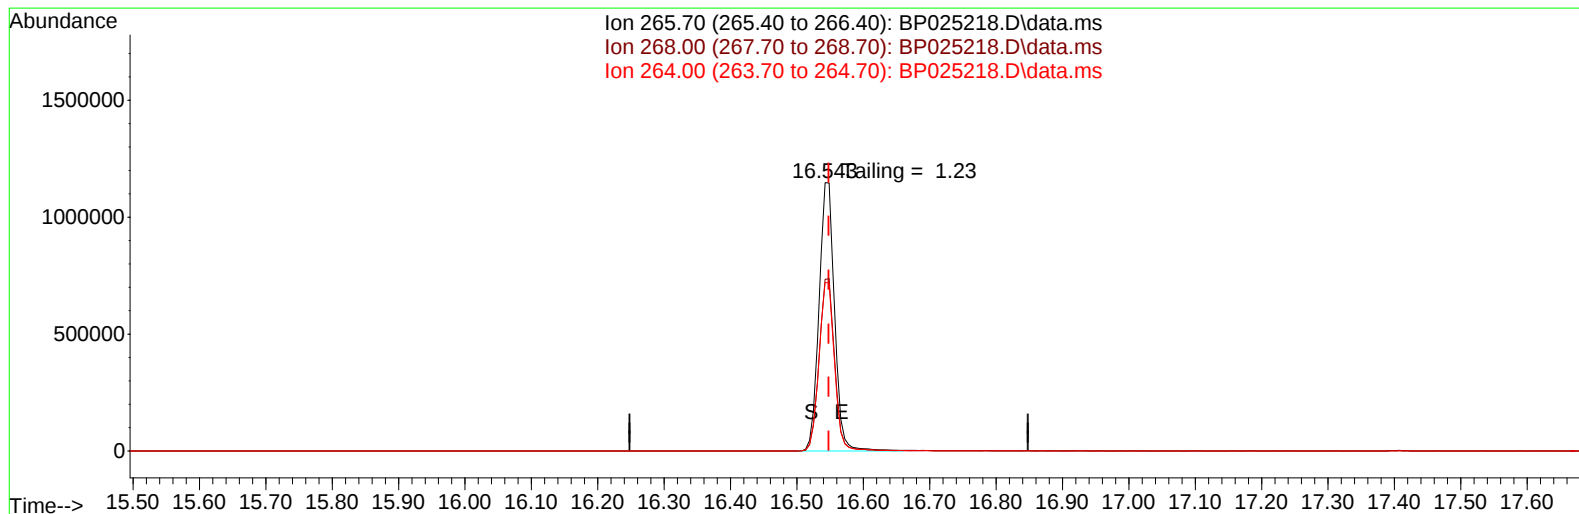

TIC: BP025218.D\data.ms

(70) Pentachlorophenol (C)

16.543min (-0.005) 1096666.83 ng




response 1870776

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.70	63.99
264.00	62.90	62.86
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072325\
Data File : BP025218.D
Acq On : 23 Jul 2025 10:41
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Jul 23 12:04:22 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP072125.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 22 02:55:21 2025
Response via : Initial Calibration

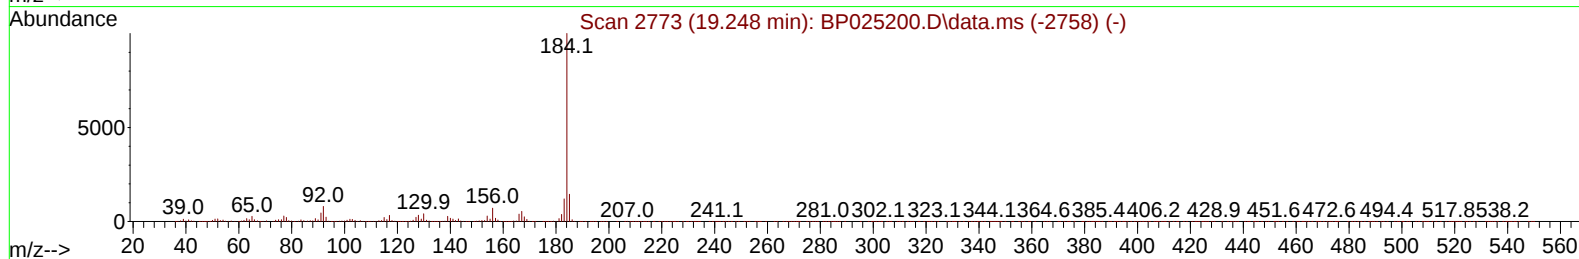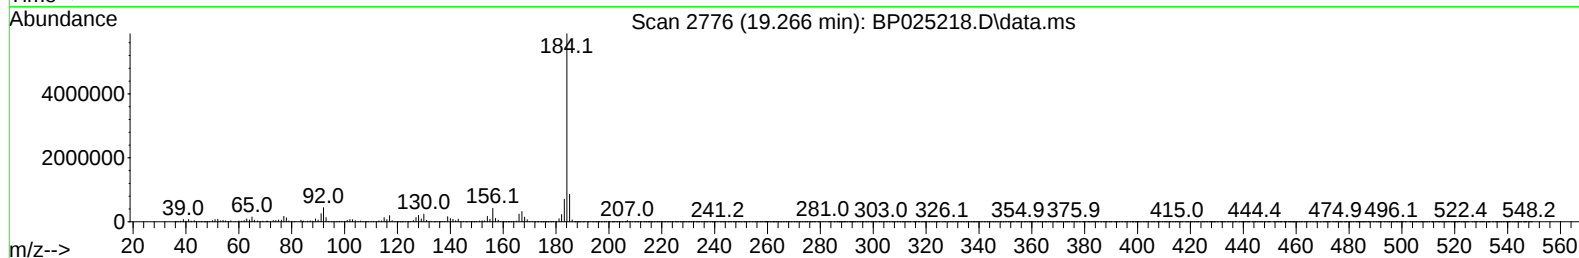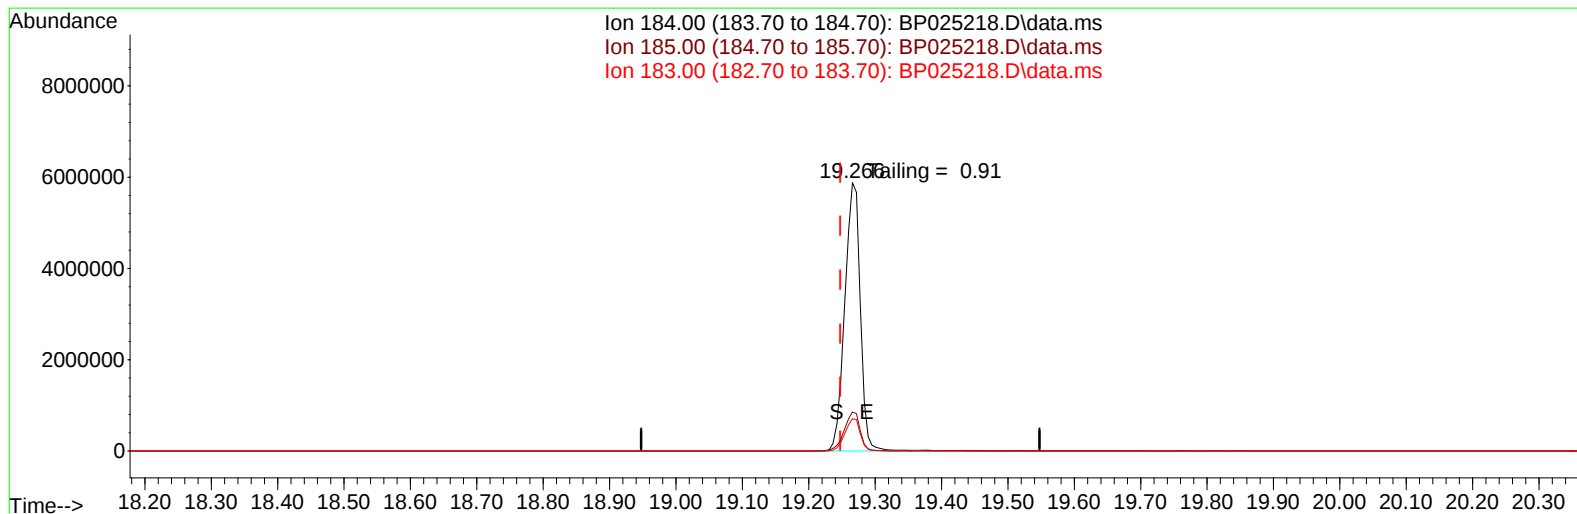

TIC: BP025218.D\data.ms

(77) Benzidine

19.266min (+ 0.018) 624111.67 ng

response 9553310

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.58
183.00	12.00	12.04
0.00	0.00	0.00