


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071525\
Data File : BN037497.D
Acq On : 15 Jul 2025 10:57
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN071525.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Jul 16 01:39:21 2025

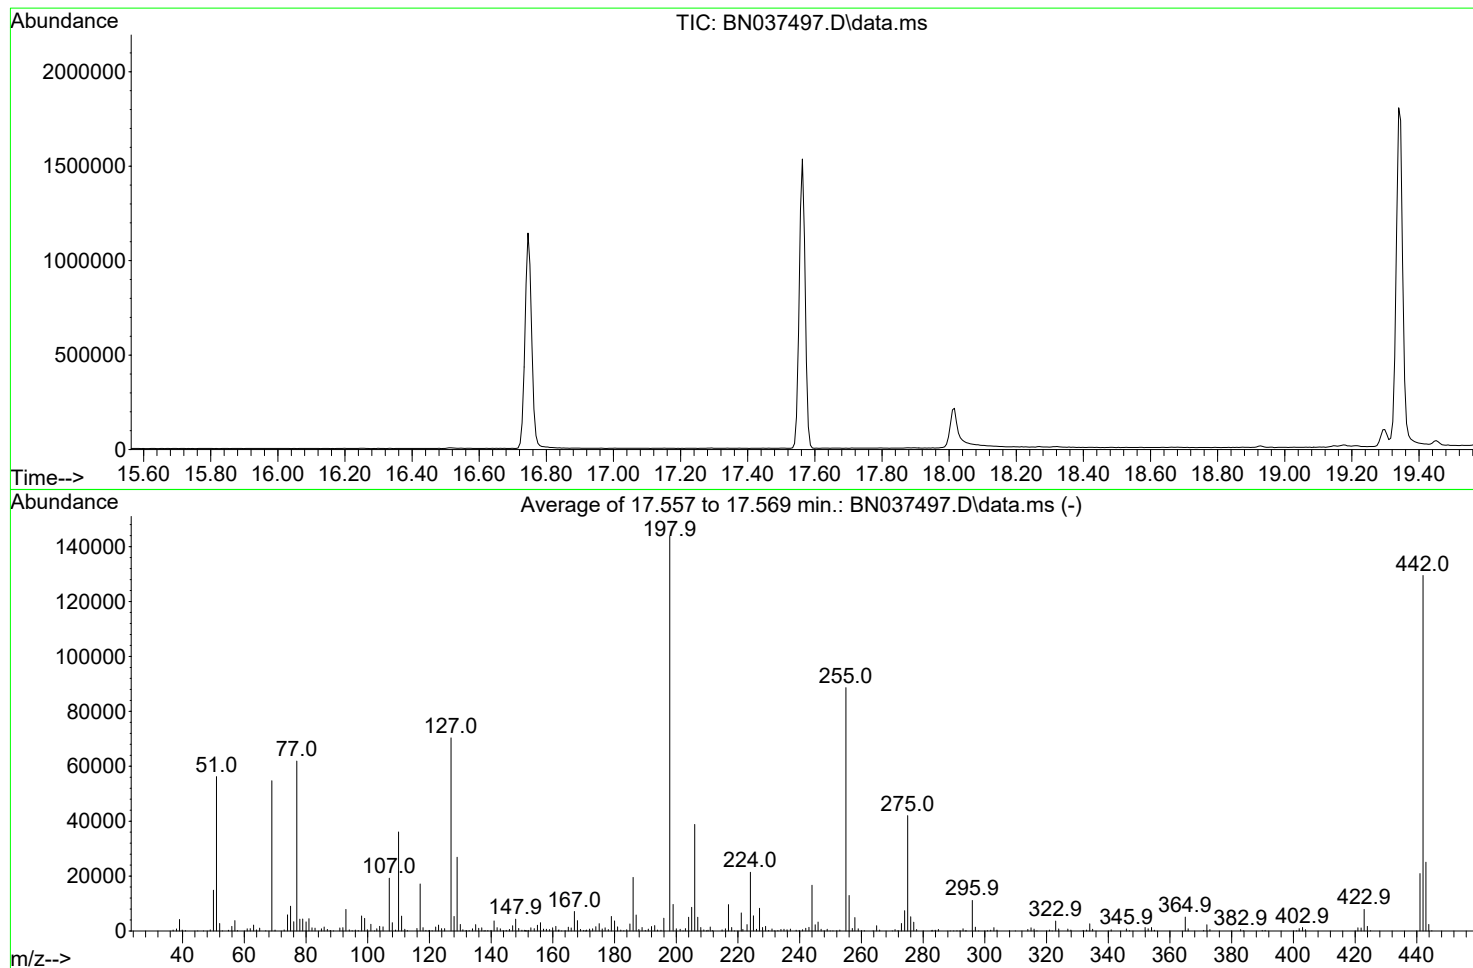

AutoFind: Scans 2460, 2461, 2462; Background Corrected with Scan 2453

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
68	69	0.00	2	0.0	0	PASS
69	69	100	100	100.0	54709	PASS
70	69	0.00	2	0.6	344	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	143808	PASS
199	198	5	9	6.7	9669	PASS
365	198	1	100	3.5	5100	PASS
441	443	0.01	150	83.6	20941	PASS
442	442	100	100	100.0	129491	PASS
443	442	15	24	19.4	25064	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
7/15/2025	BNA_N	<u>BN037497.D</u>
Compound Name	Response	Retention Time
DDT	478094	20.592
DDD	7051	20.145
DDE	60	19.639
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7111	485205	1.47

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071525\
Data File : BN037497.D
Acq On : 15 Jul 2025 10:57
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jul 15 18:10:23 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 10 02:20:59 2025
Response via : Initial Calibration

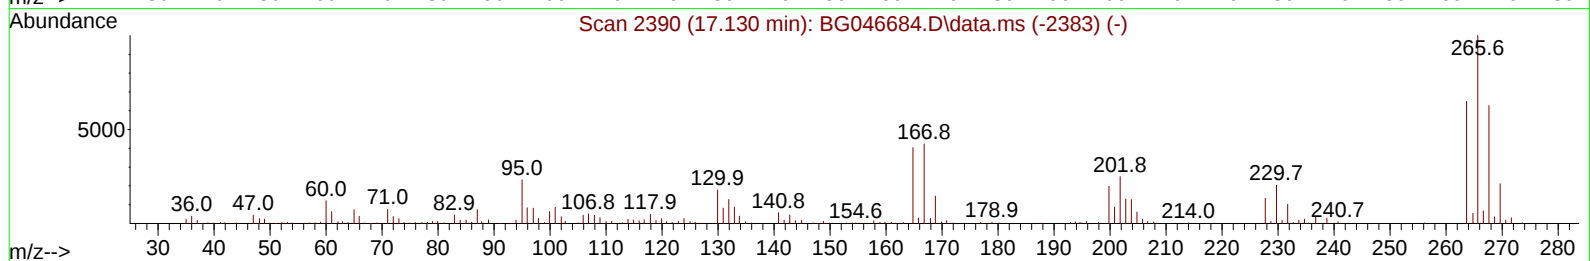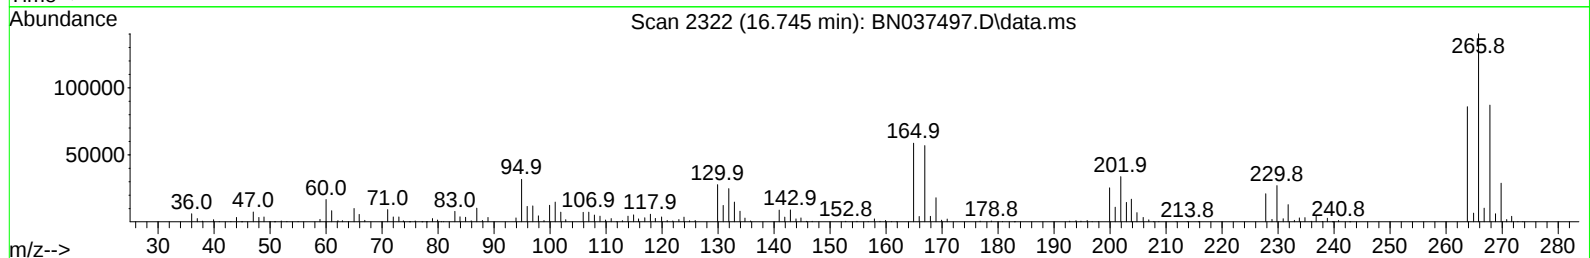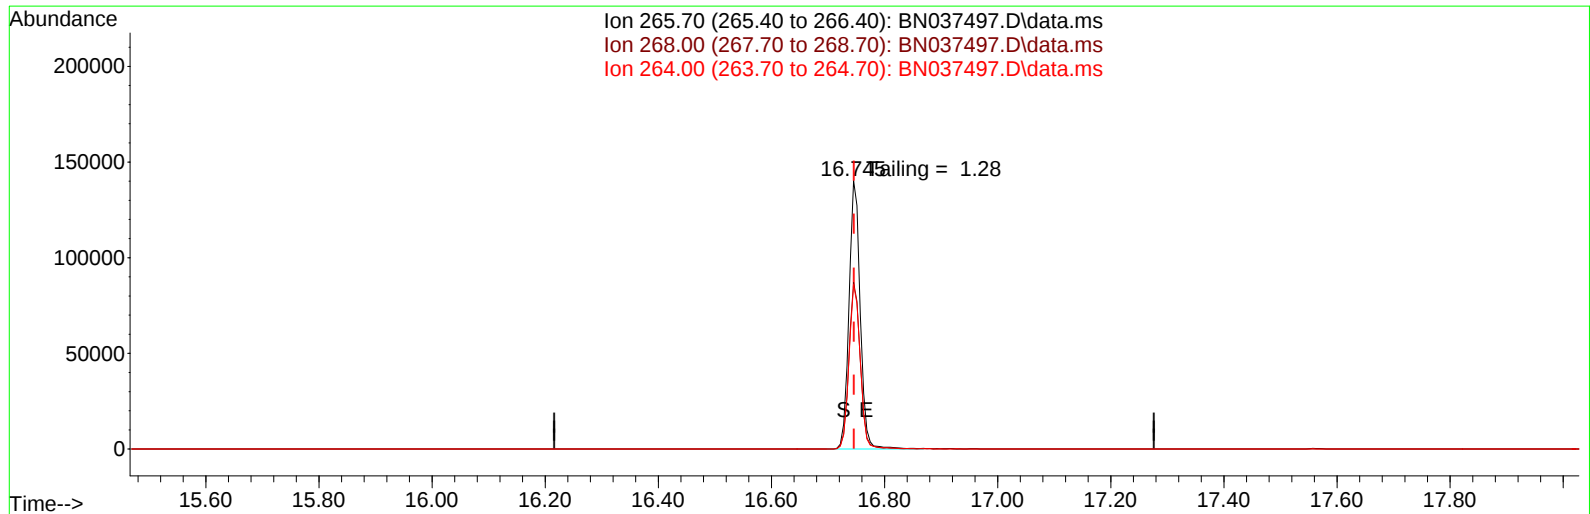

TIC: BN037497.D\data.ms

(70) Pentachlorophenol (C)

16.745min (-0.001) 31259.96 ng




response 194539

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.06
264.00	61.60	61.25
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071525\
Data File : BN037497.D
Acq On : 15 Jul 2025 10:57
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jul 15 18:10:23 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 10 02:20:59 2025
Response via : Initial Calibration

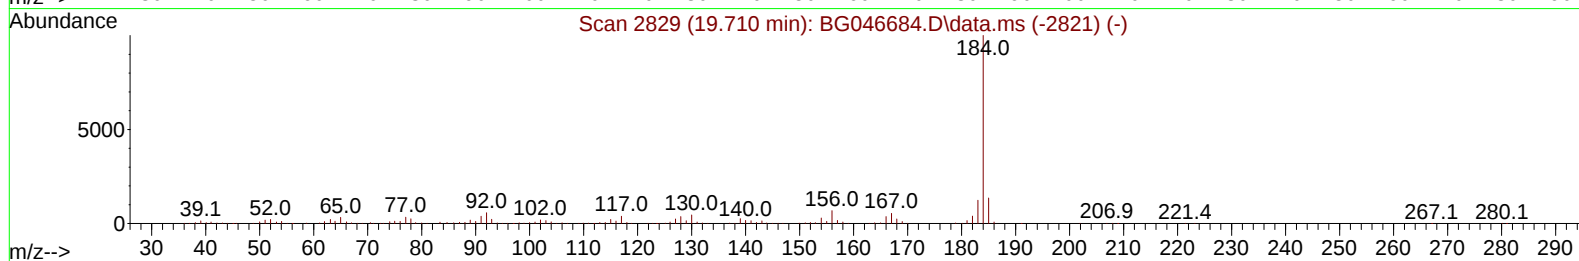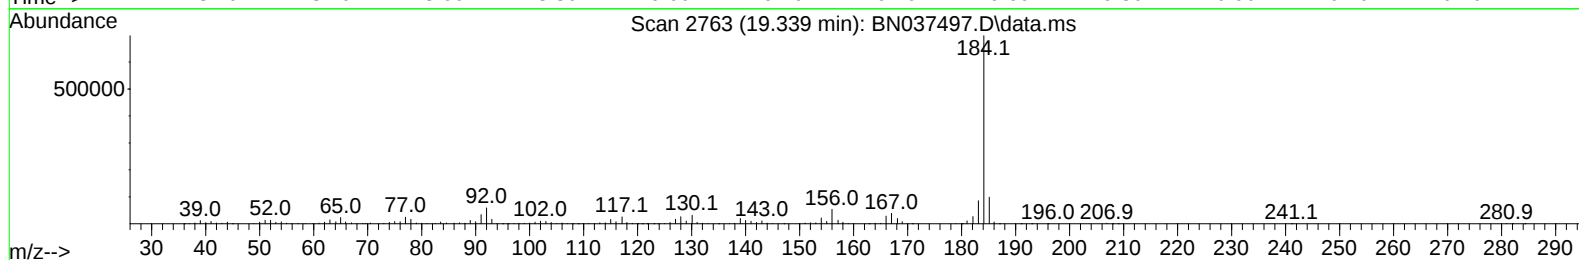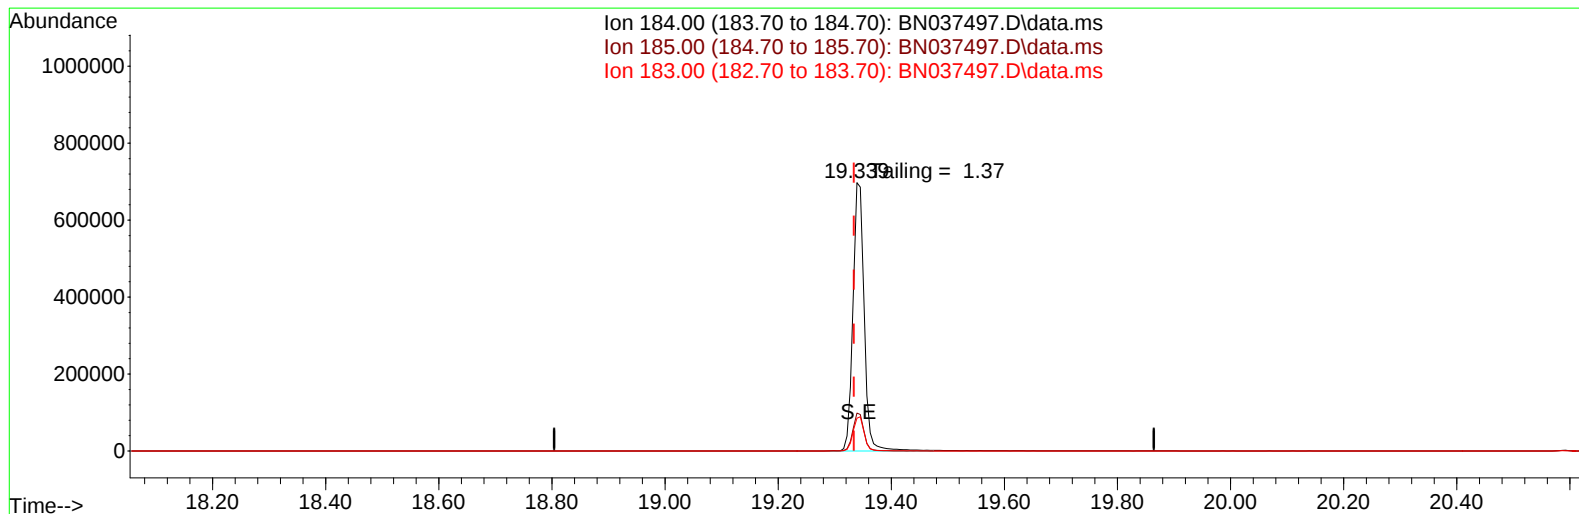

TIC: BN037497.D\data.ms

(77) Benzidine

19.339min (+ 0.005) 0.00 ng

response 963155

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.14
183.00	13.20	12.27
0.00	0.00	0.00