
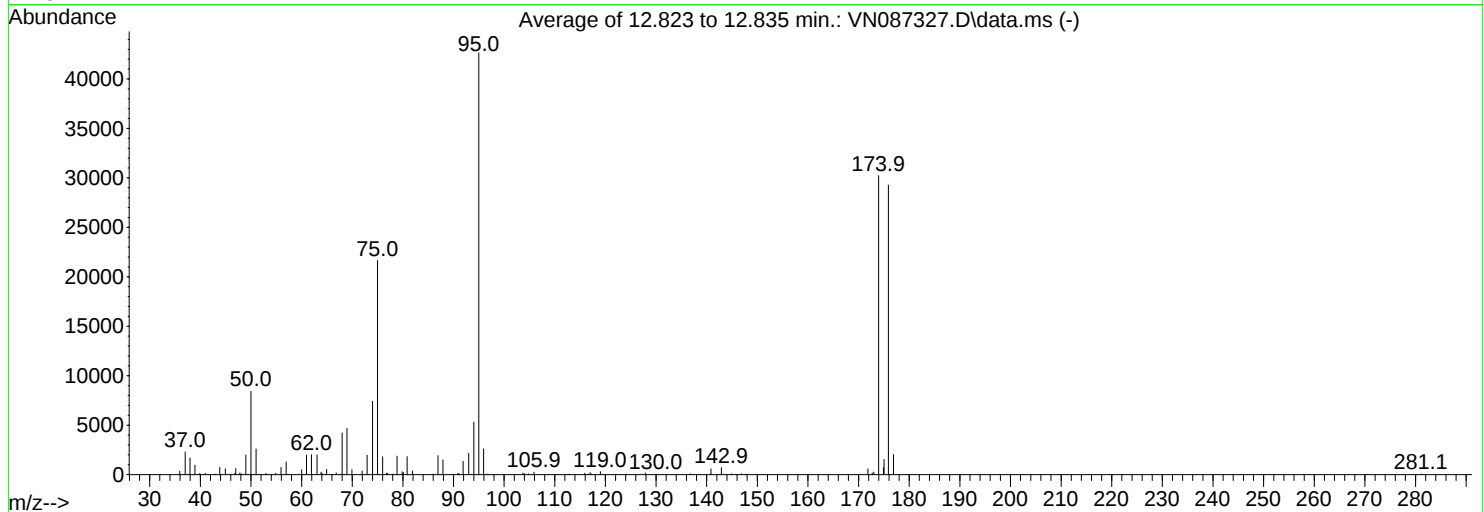


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN071625\
Data File : VN087327.D
Acq On : 16 Jul 2025 16:10
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N071625W.M
Title : SW846 8260
Last Update : Thu Jul 17 02:56:13 2025

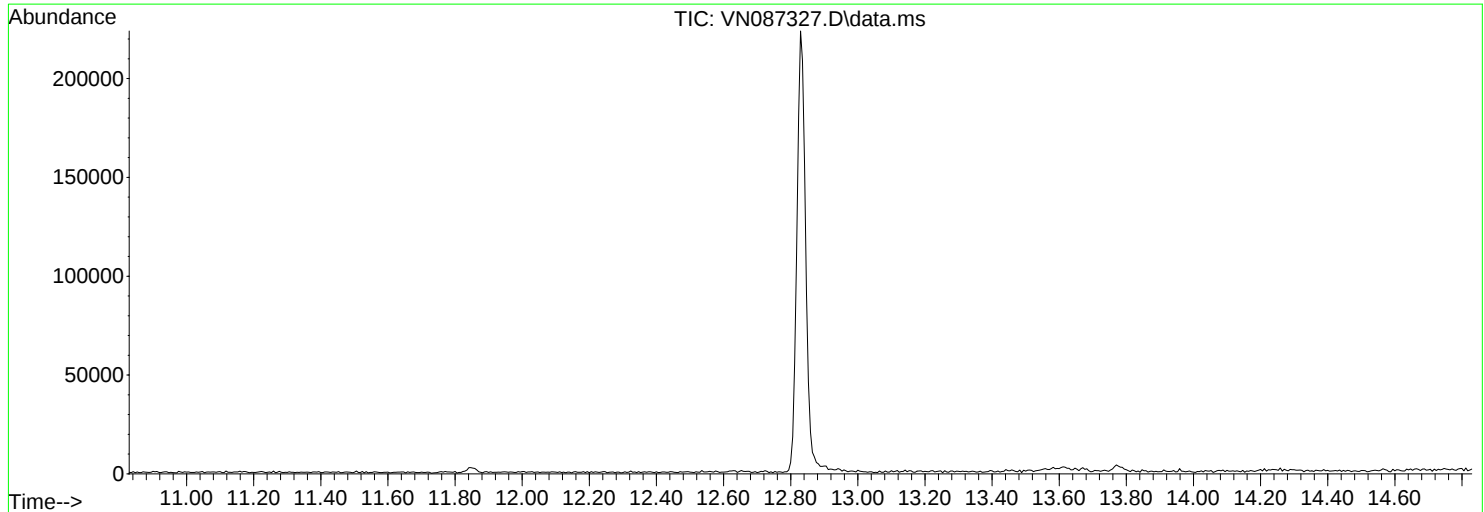

AutoFind: Scans 1848, 1849, 1850; Background Corrected with Scan 1839

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.8	8426	PASS
75	95	30	60	50.8	21643	PASS
95	95	100	100	100.0	42640	PASS
96	95	5	9	6.1	2612	PASS
173	174	0.00	2	0.8	255	PASS
174	95	50	100	70.9	30229	PASS
175	174	5	9	5.1	1538	PASS
176	174	95	101	96.9	29285	PASS
177	176	5	9	7.0	2046	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.95	354	47.80	181	61.95	2016	74.00	742
37.00	2290	48.10	60	63.05	2010	75.00	2164
37.95	1679	49.00	1995	63.85	261	76.00	181
38.95	954	50.00	8426	64.10	115	76.75	14
39.90	107	51.00	2608	64.95	542	77.00	122
40.95	135	52.95	119	66.85	179	78.10	60
42.90	65	54.90	138	68.00	4227	78.85	1870
43.85	725	55.95	722	68.95	4698	79.85	287
44.95	593	56.95	1299	69.95	494	80.10	209
46.80	115	60.00	486	71.95	381	80.85	1827
47.00	608	60.95	1996	72.95	1978	81.90	375

Average of 12.823 to 12.835 min.: VN087327.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
86.00	53	103.70	156	127.90	178	173.95	30229
86.95	1927	104.00	90	130.00	72	174.90	709
87.90	1486	104.80	81	136.80	89	175.05	1538
90.85	118	105.90	261	140.85	580	175.90	29285
91.10	107	112.80	55	142.90	707	176.90	2046
91.90	1340	115.90	151	144.90	80	281.10	60
93.00	2153	116.60	61	146.90	74		
94.00	5304	117.00	209	147.70	57		
95.00	42640	117.20	66	171.85	576		
95.95	2612	119.00	301	172.70	163		
96.80	56	124.10	52	173.00	255		

Instrument :

MSVOA_N

ClientSampleId :

BFB