


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN072125\
Data File : VN087367.D
Acq On : 21 Jul 2025 10:05
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N071625W.M
Title : SW846 8260
Last Update : Thu Jul 17 02:56:13 2025

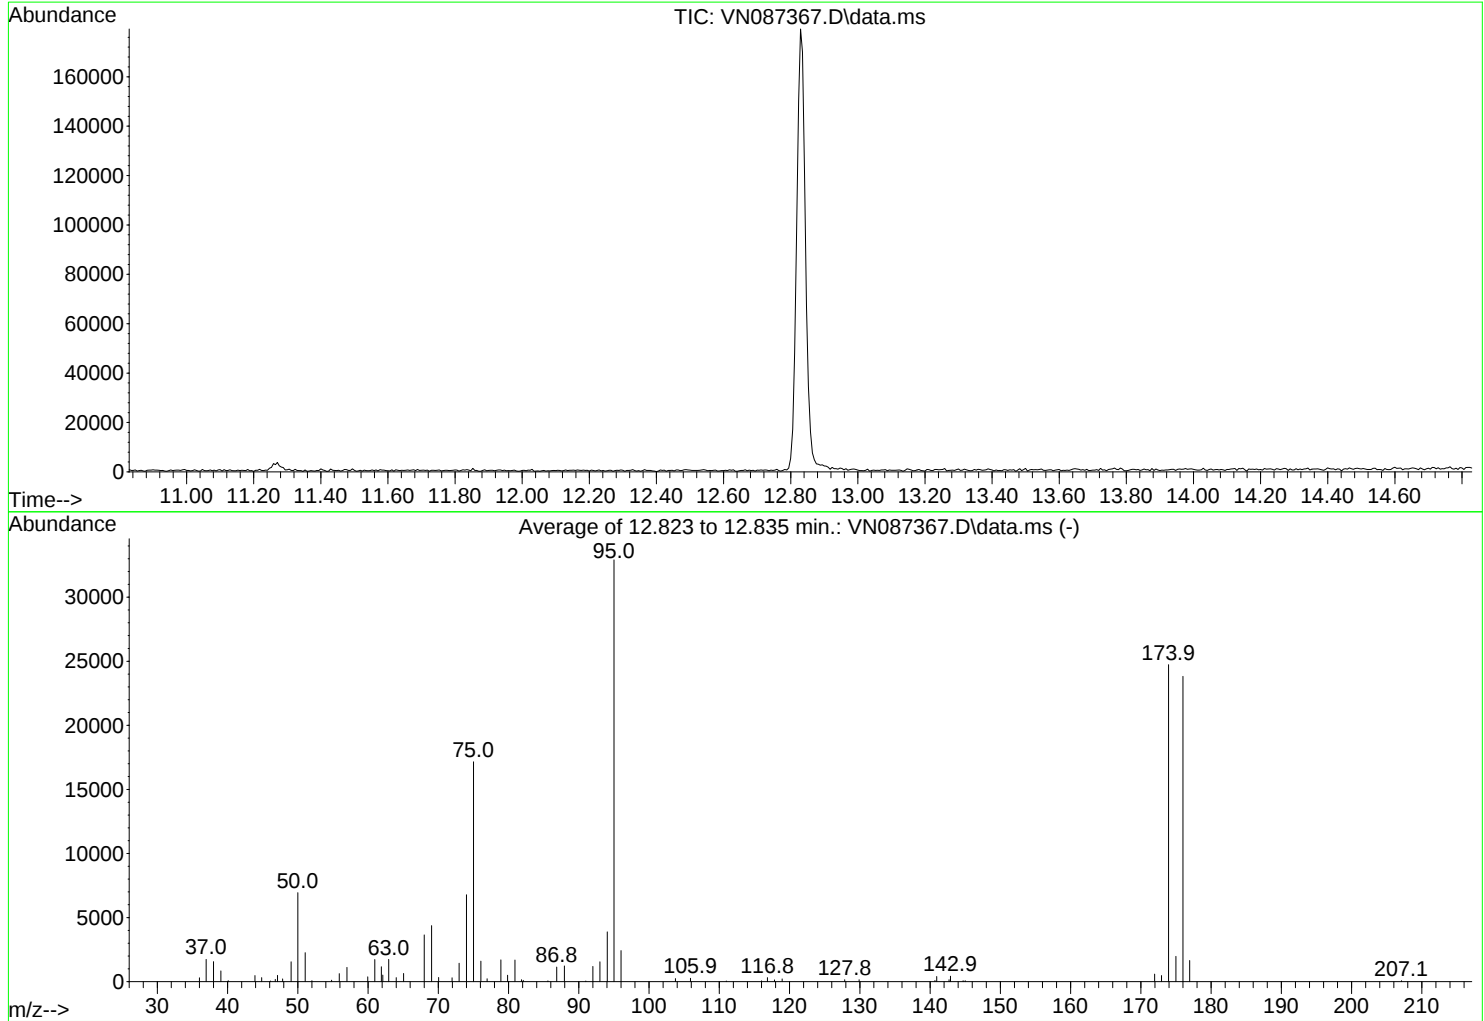

AutoFind: Scans 1848, 1849, 1850; Background Corrected with Scan 1840

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.1	6948	PASS
75	95	30	60	52.1	17152	PASS
95	95	100	100	100.0	32912	PASS
96	95	5	9	7.4	2423	PASS
173	174	0.00	2	1.9	479	PASS
174	95	50	100	75.2	24736	PASS
175	174	5	9	8.0	1975	PASS
176	174	95	101	96.3	23816	PASS
177	176	5	9	6.9	1646	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	302	49.05	1549	62.95	1731	76.95	221
36.95	1740	50.00	6948	64.00	319	78.90	169
38.00	1561	51.05	2254	65.05	643	79.85	49
39.05	842	52.00	74	68.00	3653	80.90	169
40.10	77	54.80	114	69.05	4374	81.85	153
43.90	471	55.90	630	70.05	327	82.10	106
44.85	308	57.00	1107	71.95	303	85.60	68
46.10	51	59.95	371	72.95	1431	86.85	1142
46.80	171	60.95	1721	74.00	6775	87.95	1224
47.10	492	61.90	1159	75.00	17152	91.00	50
47.85	218	62.10	519	76.05	1599	92.00	1189

Average of 12.823 to 12.835 min.: VN087367.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
93.00	1549	127.85	157	175.00	1975		
94.05	3882	129.90	156	176.00	23816		
95.00	32912	140.70	89	176.95	1646		
96.00	2423	140.95	397	207.10	79		
103.75	235	142.70	154				
105.90	265	142.90	426				
111.00	53	144.70	81				
116.00	67	145.00	76				
116.85	315	171.95	587				
117.85	138	172.95	479				
118.95	211	173.95	24736				

Instrument :

MSVOA_N

ClientSampleId :

BFB