

Prep Standard - Chemical Standard Summary

Order ID : Q2651

Test : EPH_NF

Prepbatch ID : PB168930,

Sequence ID/Qc Batch ID: FE072125AL,FE072225AL,

Standard ID :

EP2625,EP2626,PP24170,PP24174,PP24175,PP24176,PP24177,PP24178,PP24179,PP24652,PP24673,PP24728,

Chemical ID :

E3551,E3940,E3947,E3949,E3951,E3954,E3956,P12363,P12981,P12983,P13279,P13609,P13610,P13611,P13612,P13650,P13671,P13682,P13683,P13684,P13686,P14000,P14001,P14002,P14003,P14004,P14022,P14023,P14024,P14025,P14026,P14046,P14047,P14048,P14049,W3177,

Extractions STANDARD PREPARATION LOG

| <u>Recipe ID</u> | <u>NAME</u> | <u>NO.</u> | <u>Prep Date</u> | <u>Expiration Date</u> | <u>Prepared By</u> | <u>ScaleID</u> | <u>PipetteID</u> | <u>Supervised By</u> |
|------------------|----------------------|------------------------|------------------|------------------------|--------------------|-------------------------------------|------------------|-------------------------------------|
| 3923 | Baked Sodium Sulfate | EP2625 | 07/15/2025 | 12/04/2025 | RUPESHKUMAR SHAH | Extraction_SC ALE_2 (EX-SC-2) | None | Riteshkumar Patel 07/15/2025 |

FROM 4000.00000gram of E3551 = Final Quantity: 4000.000 gram

| <u>Recipe ID</u> | <u>NAME</u> | <u>NO.</u> | <u>Prep Date</u> | <u>Expiration Date</u> | <u>Prepared By</u> | <u>ScaleID</u> | <u>PipetteID</u> | <u>Supervised By</u> |
|------------------|--------------------------------|------------------------|------------------|------------------------|--------------------|----------------|------------------|-------------------------------------|
| 2017 | 1:1 ACETONE/METHYLENE CHLORIDE | EP2626 | 07/15/2025 | 01/15/2026 | RUPESHKUMAR SHAH | None | None | Riteshkumar Patel 07/15/2025 |

FROM 8000.00000ml of E3949 + 8000.00000ml of E3954 = Final Quantity: 16000.000 ml



| <u>Recipe ID</u> | <u>NAME</u> | <u>NO.</u> | <u>Prep Date</u> | <u>Expiration Date</u> | <u>Prepared By</u> | <u>ScaleID</u> | <u>PipetteID</u> | <u>Supervised By</u> |
|--|---|-------------------------|------------------|------------------------|--------------------|----------------|------------------|------------------------------|
| 781 | 100 PPM Aliphatic HC Working STD (Restek) | PP24170 | 02/03/2025 | 08/03/2025 | Yogesh Patel | None | None | Ankita Jodhani 02/03/2025 |
| <u>FROM</u> 0.25000ml of P12981 + 0.25000ml of P13671 + 1.25000ml of P12363 + 23.25000ml of W3177 = Final Quantity: 25.000 ml | | | | | | | | |

| <u>Recipe ID</u> | <u>NAME</u> | <u>NO.</u> | <u>Prep Date</u> | <u>Expiration Date</u> | <u>Prepared By</u> | <u>ScaleID</u> | <u>PipetteID</u> | <u>Supervised By</u> |
|------------------|---|-------------------------|------------------|------------------------|--------------------|----------------|------------------|----------------------------------|
| 2900 | 100 PPM Aliphatic HC STD (Absolute) | PP24174 | 02/03/2025 | 08/03/2025 | Yogesh Patel | None | None | Ankita Jodhani 02/03/2025 |
| <u>FROM</u> | 0.25000ml of P12983 + 0.25000ml of P13650 + 2.50000ml of P13279 + 22.00000ml of W3177 = Final Quantity: 25.000 ml | | | | | | | |

Pest/Pcb STANDARD PREPARATION LOG

| <u>Recipe ID</u> | <u>NAME</u> | <u>NO.</u> | <u>Prep Date</u> | <u>Expiration Date</u> | <u>Prepared By</u> | <u>ScaleID</u> | <u>PipetteID</u> | <u>Supervised By</u> |
|------------------|-------------------------|-------------------------|------------------|------------------------|--------------------|----------------|------------------|----------------------|
| 783 | 50 PPM Aliphatic HC STD | PP24175 | 02/03/2025 | 08/03/2025 | Yogesh Patel | None | None | Ankita Jodhani |
| 02/03/2025 | | | | | | | | |

FROM 0.50000ml of W3177 + 0.50000ml of PP24170 = Final Quantity: 1.000 ml

| <u>Recipe ID</u> | <u>NAME</u> | <u>NO.</u> | <u>Prep Date</u> | <u>Expiration Date</u> | <u>Prepared By</u> | <u>ScaleID</u> | <u>PipetteID</u> | <u>Supervised By</u> |
|------------------|-------------------------|-------------------------|------------------|------------------------|--------------------|----------------|------------------|----------------------|
| 784 | 20 PPM Aliphatic HC STD | PP24176 | 02/03/2025 | 08/03/2025 | Yogesh Patel | None | None | Ankita Jodhani |
| 02/03/2025 | | | | | | | | |

FROM 0.80000ml of W3177 + 0.20000ml of PP24170 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

| <u>Recipe ID</u> | <u>NAME</u> | <u>NO.</u> | <u>Prep Date</u> | <u>Expiration Date</u> | <u>Prepared By</u> | <u>ScaleID</u> | <u>PipetteID</u> | <u>Supervised By</u> |
|------------------|-------------------------|-------------------------|------------------|------------------------|--------------------|----------------|------------------|----------------------|
| 785 | 10 PPM Aliphatic HC STD | PP24177 | 02/03/2025 | 08/03/2025 | Yogesh Patel | None | None | Ankita Jodhani |
| | | | | | | | | 02/03/2025 |

FROM 0.90000ml of W3177 + 0.10000ml of PP24170 = Final Quantity: 1.000 ml

| <u>Recipe ID</u> | <u>NAME</u> | <u>NO.</u> | <u>Prep Date</u> | <u>Expiration Date</u> | <u>Prepared By</u> | <u>ScaleID</u> | <u>PipetteID</u> | <u>Supervised By</u> |
|------------------|------------------------|-------------------------|------------------|------------------------|--------------------|----------------|------------------|----------------------|
| 786 | 5 PPM Aliphatic HC STD | PP24178 | 02/03/2025 | 08/03/2025 | Yogesh Patel | None | None | Ankita Jodhani |
| | | | | | | | | 02/03/2025 |

FROM 0.90000ml of W3177 + 0.10000ml of PP24175 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

| <u>Recipe ID</u> | <u>NAME</u> | <u>NO.</u> | <u>Prep Date</u> | <u>Expiration Date</u> | <u>Prepared By</u> | <u>ScaleID</u> | <u>PipetteID</u> | <u>Supervised By</u> |
|------------------|--|-------------------------|------------------|------------------------|--------------------|----------------|------------------|----------------------|
| 2901 | 20 PPM Aliphatic HC STD ICV (Absolute) | PP24179 | 02/03/2025 | 08/03/2025 | Yogesh Patel | None | None | Ankita Jodhani |
| | | | | | | | | 02/03/2025 |

FROM 0.80000ml of W3177 + 0.20000ml of PP24174 = Final Quantity: 1.000 ml

| <u>Recipe ID</u> | <u>NAME</u> | <u>NO.</u> | <u>Prep Date</u> | <u>Expiration Date</u> | <u>Prepared By</u> | <u>ScaleID</u> | <u>PipetteID</u> | <u>Supervised By</u> |
|------------------|-------------------------------|-------------------------|------------------|------------------------|--------------------|----------------|------------------|----------------------|
| 1339 | 100 PPM NJEPH Surrogate Spike | PP24652 | 06/17/2025 | 12/11/2025 | Abdul Mirza | None | None | Yogesh Patel |
| | | | | | | | | 07/24/2025 |

FROM 1.25000ml of P13609 + 1.25000ml of P13610 + 1.25000ml of P13611 + 1.25000ml of P13612 + 1.25000ml of P13682 + 1.25000ml of P13683 + 1.25000ml of P13684 + 1.25000ml of P13686 + 490.00000ml of E3940 = Final Quantity: 500.000 ml



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

CHEMICAL RECEIPT LOG BOOK

| Supplier | ItemCode / ItemName | Lot # | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|-----------------------------|--|--------|-----------------|-------------------------|-----------------------------|----------------|
| PCI Scientific Supply, Inc. | PC19631-100 / SODIUM SULFATE, ANHYDROUS, PEST GRADE, 1 | 313201 | 12/04/2025 | 01/03/2024 / Rajesh | 07/20/2023 / Rajesh | E3551 |

| Supplier | ItemCode / ItemName | Lot # | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|------------------|--|------------|-----------------|-------------------------|-----------------------------|----------------|
| Seidler Chemical | BA-9254-03 / Acetone, Ultra Resi (cs/4x4L) | 24H1462005 | 12/11/2025 | 06/11/2025 / Rajesh | 06/04/2025 / Rajesh | E3940 |

| Supplier | ItemCode / ItemName | Lot # | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|------------------|---|--------|-----------------|-------------------------|-----------------------------|----------------|
| Seidler Chemical | BA-9262-03 / Hexane, Ultra-Resi (cs/4x4L) | 243570 | 11/07/2029 | 06/26/2025 / RUPESH | 06/19/2025 / RUPESH | E3947 |

| Supplier | ItemCode / ItemName | Lot # | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|------------------|--|------------|-----------------|--------------------------|-----------------------------|----------------|
| Seidler Chemical | BA-9254-03 / Acetone, Ultra Resi (cs/4x4L) | 24H2762008 | 04/18/2027 | 07/08/2025 / RITESHKUMAR | 07/03/2025 / RUPESH | E3949 |

| Supplier | ItemCode / ItemName | Lot # | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|------------------|--|------------|-----------------|-------------------------|-----------------------------|----------------|
| Seidler Chemical | BA-3382-05 / Sand, Purified (cs/4x2.5kg) | 25A2756718 | 12/31/2028 | 07/09/2025 / RUPESH | 04/28/2020 / RUPESH | E3951 |

| Supplier | ItemCode / ItemName | Lot # | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|------------------|---|------------|-----------------|-------------------------|-----------------------------|----------------|
| Seidler Chemical | BA-9644-A4 / Methylene Chloride,U-Resi, Cycle-Tainer (215L) | 25B1862001 | 03/19/2026 | 07/14/2025 / RUPESH | 06/11/2025 / RUPESH | E3954 |

CHEMICAL RECEIPT LOG BOOK

| Supplier | ItemCode / ItemName | Lot # | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|------------------|---|------------|-----------------|-------------------------|-----------------------------|----------------|
| Seidler Chemical | BA-9262-03 / Hexane, Ultra-Resi (cs/4x4L) | 25C0362005 | 04/30/2026 | 07/16/2025 / RUPESH | 07/16/2025 / RUPESH | E3956 |

| Supplier | ItemCode / ItemName | Lot # | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|----------|--|----------|-----------------|-------------------------|-----------------------------|----------------|
| Restek | 30540 / Custom NJEPH Aliphatics Calibration Standard | A0190424 | 08/03/2025 | 02/03/2025 / yogesh | 03/16/2023 / Yogesh | P12363 |

| Supplier | ItemCode / ItemName | Lot # | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|----------|-------------------------------------|----------|-----------------|-------------------------|-----------------------------|----------------|
| Restek | 31098 / 1-Chlorooctadecane Standard | A0204989 | 08/03/2025 | 02/03/2025 / yogesh | 12/20/2023 / Yogesh | P12981 |

| Supplier | ItemCode / ItemName | Lot # | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|----------|-------------------------------------|----------|-----------------|-------------------------|-----------------------------|----------------|
| Restek | 31098 / 1-Chlorooctadecane Standard | A0204989 | 08/03/2025 | 02/03/2025 / yogesh | 12/20/2023 / Yogesh | P12983 |

| Supplier | ItemCode / ItemName | Lot # | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|--------------------------|---|--------|-----------------|-------------------------|-----------------------------|----------------|
| Absolute Standards, Inc. | 95899 / NJ EPH Aliphatic n-Hydrocarbons-Revised, 1000 PPM | 040524 | 08/03/2025 | 02/03/2025 / yogesh | 04/11/2024 / yogesh | P13279 |

| Supplier | ItemCode / ItemName | Lot # | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|----------|-------------------------------------|----------|-----------------|-------------------------|-----------------------------|----------------|
| Restek | 31098 / 1-Chlorooctadecane Standard | A0213283 | 12/17/2025 | 06/17/2025 / Abdul | 10/16/2024 / yogesh | P13609 |

CHEMICAL RECEIPT LOG BOOK

| Supplier | ItemCode / ItemName | Lot # | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|----------|---|----------|-----------------|-------------------------|-----------------------------|----------------|
| Restek | 31098 / 1-Chlorooctadecane Standard | A0213283 | 12/17/2025 | 06/17/2025 / Abdul | 10/16/2024 / yogesh | P13610 |

| Supplier | ItemCode / ItemName | Lot # | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|----------|---|----------|-----------------|-------------------------|-----------------------------|----------------|
| Restek | 31098 / 1-Chlorooctadecane Standard | A0213283 | 12/17/2025 | 06/17/2025 / Abdul | 10/16/2024 / yogesh | P13611 |

| Supplier | ItemCode / ItemName | Lot # | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|----------|---|----------|-----------------|-------------------------|-----------------------------|----------------|
| Restek | 31098 / 1-Chlorooctadecane Standard | A0213283 | 12/17/2025 | 06/17/2025 / Abdul | 10/16/2024 / yogesh | P13612 |

| Supplier | ItemCode / ItemName | Lot # | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|----------|---------------------------------|----------|-----------------|-------------------------|-----------------------------|----------------|
| Restek | 31097 / o-Terphenyl Standard | A0216631 | 08/03/2025 | 02/03/2025 / yogesh | 10/16/2024 / yogesh | P13650 |

| Supplier | ItemCode / ItemName | Lot # | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|----------|---------------------------------|----------|-----------------|-------------------------|-----------------------------|----------------|
| Restek | 31097 / o-Terphenyl Standard | A0216631 | 08/03/2025 | 02/03/2025 / yogesh | 10/16/2024 / yogesh | P13671 |

| Supplier | ItemCode / ItemName | Lot # | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|----------|---------------------------------|----------|-----------------|-------------------------|-----------------------------|----------------|
| Restek | 31097 / o-Terphenyl Standard | A0216631 | 12/17/2025 | 06/17/2025 / Abdul | 10/16/2024 / yogesh | P13682 |

CHEMICAL RECEIPT LOG BOOK

| Supplier | ItemCode / ItemName | Lot # | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|----------|------------------------------|----------|-----------------|-------------------------|-----------------------------|----------------|
| Restek | 31097 / o-Terphenyl Standard | A0216631 | 12/17/2025 | 06/17/2025 / Abdul | 10/16/2024 / yogesh | P13683 |

| Supplier | ItemCode / ItemName | Lot # | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|----------|------------------------------|----------|-----------------|-------------------------|-----------------------------|----------------|
| Restek | 31097 / o-Terphenyl Standard | A0216631 | 12/17/2025 | 06/17/2025 / Abdul | 10/16/2024 / yogesh | P13684 |

| Supplier | ItemCode / ItemName | Lot # | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|----------|------------------------------|----------|-----------------|-------------------------|-----------------------------|----------------|
| Restek | 31097 / o-Terphenyl Standard | A0216631 | 12/17/2025 | 06/17/2025 / Abdul | 10/16/2024 / yogesh | P13686 |

| Supplier | ItemCode / ItemName | Lot # | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|----------|---|----------|-----------------|-------------------------|-----------------------------|----------------|
| Restek | 30543 / Custom NJEPH Aromatics Matrix Spike Mix | A0225381 | 01/14/2026 | 07/14/2025 / Abdul | 05/20/2025 / Rahul | P14000 |

| Supplier | ItemCode / ItemName | Lot # | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|----------|---|----------|-----------------|-------------------------|-----------------------------|----------------|
| Restek | 30543 / Custom NJEPH Aromatics Matrix Spike Mix | A0225381 | 01/14/2026 | 07/14/2025 / Abdul | 05/20/2025 / Rahul | P14001 |

| Supplier | ItemCode / ItemName | Lot # | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|----------|---|----------|-----------------|-------------------------|-----------------------------|----------------|
| Restek | 30543 / Custom NJEPH Aromatics Matrix Spike Mix | A0225381 | 01/14/2026 | 07/14/2025 / Abdul | 05/20/2025 / Rahul | P14002 |

CHEMICAL RECEIPT LOG BOOK

| Supplier | ItemCode / ItemName | Lot # | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|----------|---|----------|-----------------|-------------------------|-----------------------------|----------------|
| Restek | 30543 / Custom NJEPH Aromatics Matrix Spike Mix | A0225381 | 01/14/2026 | 07/14/2025 / Abdul | 05/20/2025 / Rahul | P14003 |

| Supplier | ItemCode / ItemName | Lot # | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|----------|---|----------|-----------------|-------------------------|-----------------------------|----------------|
| Restek | 30543 / Custom NJEPH Aromatics Matrix Spike Mix | A0225381 | 01/14/2026 | 07/14/2025 / Abdul | 05/20/2025 / Rahul | P14004 |

| Supplier | ItemCode / ItemName | Lot # | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|----------|--|----------|-----------------|-------------------------|-----------------------------|----------------|
| Restek | 30542 / Custom NJEPH Aliphatics Matrix Spike Mix | A0220449 | 01/14/2026 | 07/14/2025 / Abdul | 05/20/2025 / Rahul | P14022 |

| Supplier | ItemCode / ItemName | Lot # | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|----------|--|----------|-----------------|-------------------------|-----------------------------|----------------|
| Restek | 30542 / Custom NJEPH Aliphatics Matrix Spike Mix | A0220449 | 01/14/2026 | 07/14/2025 / Abdul | 05/20/2025 / Rahul | P14023 |

| Supplier | ItemCode / ItemName | Lot # | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|----------|--|----------|-----------------|-------------------------|-----------------------------|----------------|
| Restek | 30542 / Custom NJEPH Aliphatics Matrix Spike Mix | A0220449 | 01/14/2026 | 07/14/2025 / Abdul | 05/20/2025 / Rahul | P14024 |

| Supplier | ItemCode / ItemName | Lot # | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|----------|--|----------|-----------------|-------------------------|-----------------------------|----------------|
| Restek | 30542 / Custom NJEPH Aliphatics Matrix Spike Mix | A0220449 | 01/14/2026 | 07/14/2025 / Abdul | 05/20/2025 / Rahul | P14025 |

CHEMICAL RECEIPT LOG BOOK

| Supplier | ItemCode / ItemName | Lot # | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|----------|--|----------|-----------------|-------------------------|-----------------------------|----------------|
| Restek | 30542 / Custom NJEPH Aliphatics Matrix Spike Mix | A0220449 | 01/14/2026 | 07/14/2025 / Abdul | 05/20/2025 / Rahul | P14026 |

| Supplier | ItemCode / ItemName | Lot # | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|----------|--|----------|-----------------|-------------------------|-----------------------------|----------------|
| Restek | 31480 / MA Fractionation Surrogate Spike Mix | A0224278 | 12/30/2025 | 06/30/2025 / Abdul | 06/09/2025 / anahy | P14046 |

| Supplier | ItemCode / ItemName | Lot # | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|----------|--|----------|-----------------|-------------------------|-----------------------------|----------------|
| Restek | 31480 / MA Fractionation Surrogate Spike Mix | A0224278 | 03/31/2031 | 06/30/2025 / Abdul | 06/09/2025 / anahy | P14047 |

| Supplier | ItemCode / ItemName | Lot # | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|----------|--|----------|-----------------|-------------------------|-----------------------------|----------------|
| Restek | 31480 / MA Fractionation Surrogate Spike Mix | A0224278 | 12/30/2025 | 06/30/2025 / Abdul | 06/09/2025 / anahy | P14048 |

| Supplier | ItemCode / ItemName | Lot # | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|----------|--|----------|-----------------|-------------------------|-----------------------------|----------------|
| Restek | 31480 / MA Fractionation Surrogate Spike Mix | A0224278 | 12/30/2025 | 06/30/2025 / Abdul | 06/09/2025 / anahy | P14049 |

| Supplier | ItemCode / ItemName | Lot # | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|------------------|---|------------|-----------------|-------------------------|-----------------------------|----------------|
| Seidler Chemical | BA-9262-03 / Hexane, Ultra-Resi (cs/4x4L) | 24G1962003 | 08/22/2025 | 02/03/2025 / jignesh | 01/31/2025 / jignesh | W3177 |



**PRODUCTOS
QUÍMICOS
MONTERREY, S.A. DE C.V.**

MIRADOR 201, COL. MIRADOR
MONTERREY, N.L. MEXICO
CP 64070
TEL +52 81 13 52 57 57
www.pqm.com.mx

CERTIFICATE OF ANALYSIS

| | | | |
|------------------------|-----------------------------------|---------------|---------------------------------|
| PRODUCT : | SODIUM SULFATE CRYSTALS ANHYDROUS | | |
| QUALITY : | ACS (CODE RMB3375) | FORMULA : | Na ₂ SO ₄ |
| SPECIFICATION NUMBER : | 6399 | RELEASE DATE: | ABR/21/2023 |
| LOT NUMBER : | 313201 | | |

| TEST | SPECIFICATIONS | LOT VALUES |
|--|----------------|-------------|
| Assay (Na ₂ SO ₄) | Min. 99.0% | 99.7 % |
| pH of a 5% solution at 25°C | 5.2 - 9.2 | 6.1 |
| Insoluble matter | Max. 0.01% | 0.005 % |
| Loss on ignition | Max. 0.5% | 0.1 % |
| Chloride (Cl) | Max. 0.001% | <0.001 % |
| Nitrogen compounds (as N) | Max. 5 ppm | <5 ppm |
| Phosphate (PO ₄) | Max. 0.001% | <0.001 % |
| Heavy metals (as Pb) | Max. 5 ppm | <5 ppm |
| Iron (Fe) | Max. 0.001% | <0.001 % |
| Calcium (Ca) | Max. 0.01% | 0.002 % |
| Magnesium (Mg) | Max. 0.005% | 0.001 % |
| Potassium (K) | Max. 0.008% | 0.003 % |
| Extraction-concentration suitability | Passes test | Passes test |
| Appearance | Passes test | Passes test |
| Identification | Passes test | Passes test |
| Solubility and foreign matter | Passes test | Passes test |
| Retained on US Standard No. 10 sieve | Max. 1% | 0.1 % |
| Retained on US Standard No. 60 sieve | Min. 94% | 97.3 % |
| Through US Standard No. 60 sieve | Max. 5% | 2.5 % |
| Through US Standard No. 100 sieve | Max. 10% | 0.1 % |

COMMENTS

QC: PhC Irma Belmares

If you need further details, please call our factory or contact our local distributor.

Recd. by R3 on 7/24/23 E 3551

RC-02-01, Ed. 3

Acetone

BAKER RESI-ANALYZED® Reagent

For Organic Residue Analysis

avantor™



Material No.: 9254-03

Batch No.: 24H1462005

Manufactured Date: 2024-05-24

Expiration Date: 2027-05-24

Revision No.: 0

Certificate of Analysis

| Test | Specification | Result |
|---|---------------|-------------|
| Assay ((CH ₃) ₂ CO) (by GC, corrected for water) | >= 99.4 % | 99.8 % |
| Color (APHA) | <= 10 | 5 |
| Residue after Evaporation | <= 1.0 ppm | 0.2 ppm |
| Substances Reducing Permanganate | Passes Test | Passes Test |
| Titration Acid (µeq/g) | <= 0.3 | 0.2 |
| Titration Base (µeq/g) | <= 0.6 | <0.1 |
| Water (H ₂ O) | <= 0.5 % | 0.2 % |
| FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL) | <= 5 | <1 |
| ECD Sensitive Impurities (as Heptachlor Epoxide) Single Peak (pg/mL) | <= 10 | 1 |

For Laboratory, Research, or Manufacturing Use

MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: United States

Packaging Site: Phillipsburg Mfg Ctr & DC

Rec'd by RP on 6/11/25

E3940

Jamie Croak

Director Quality Operations, Bioscience Production

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Avantor Performance Materials LLC

Certificate of Analysis

1 Reagent Lane
 Fair Lawn, NJ 07410
 201.796.7100 tel
 201.796.1329 fax

Thermo Fisher Scientific's Quality System has been found to conform to Quality Management System
 Standard ISO9001:2015 by SAI Global Certificate Number CERT - 0120633

This is to certify that units of the lot number below were tested and found to comply with the specifications of the grade listed. Certain data have been supplied by third parties. Thermo Fisher Scientific expressly disclaims all warranties, expressed or implied, including the implied warranties of merchantability and fitness for a particular purpose. Products are for research use or further manufacturing. Not for direct administration to humans or animals. It is the responsibility of the final formulator and end user to determine suitability based upon the intended use of the end product. Products are tested to meet the analytical requirements of the noted grade. The following information is the actual analytical results obtained.

| | | | |
|-------------------|---|-----------------------------|------------|
| Catalog Number | H303 | Quality Test / Release Date | 11/07/2024 |
| Lot Number | 243570 | | |
| Description | HEXANES - OPTIMA | | |
| Country of Origin | United States | Suggested Retest Date | Nov/2029 |
| Chemical Origin | Organic - non animal | | |
| BSE/TSE Comment | No animal products are used as starting raw material ingredients, or used in processing, including lubricants, processing aids, or any other material that might migrate to the finished product. | | |

N/A

| Result Name | Units | Specifications | Test Value |
|-----------------------------|------------|---------------------------------|-------------------------|
| APPEARANCE | | REPORT | Clear, colorless liquid |
| ASSAY (N-HEXANE) | % | >= 60 | 69 |
| ASSAY (SUM C6 HYDROCARBONS) | % | >= 99.9 | >99.9 |
| COLOR | APHA | <= 5 | <5 |
| DENSITY AT 25 DEGREES C | GM/ML | Inclusive Between 0.653 - 0.673 | 0.669 |
| EVAPORATION RESIDUE | ppm | <= 1 | <1 |
| FLUORESCENCE BACKGROUND | ppb | <= 1 | <1 |
| IDENTIFICATION | PASS/FAIL | = PASS TEST | PASS TEST |
| OPTICAL ABS AT 195 NM | ABS. UNITS | <= 1 | 0.74 |
| OPTICAL ABS AT 210 NM | ABS. UNITS | <= 0.25 | 0.17 |
| OPTICAL ABS AT 220 NM | ABS. UNITS | <= 0.07 | 0.05 |
| OPTICAL ABS AT 254 NM | ABS. UNITS | <= 0.005 | 0.001 |
| PESTICIDE RESIDUE ANALYSIS | NG/L | <= 10 | <10 |
| REFRACTIVE INDEX @ 25 DEG C | | Inclusive Between 1.375 - 1.385 | 1.379 |
| SUITABILITY FOR GC/MS | | = PASS TEST | PASS TEST |
| SULFUR COMPOUNDS | % | <= 0.005 | <0.005 |
| THIOPHENE | PASS/FAIL | = PASS TEST | PASS TEST |
| WATER (H2O) | % | <= 0.01 | <0.01 |
| WATER-SOLUBLE TITRABLE ACID | MEQ/G | <= 0.0003 | 0.0001 |

Recd on 6/19/25

E3947

Harout Sahagian

Harout Sahagian - Quality Control Manager - Fair Lawn

Note: The data listed is valid for all package sizes of this lot of this product, expressed as an extension of this catalog number listed above.
 If there are any questions with this certificate, please call at (800) 227-6701.

*Based on suggested storage condition.

Acetone

BAKER RESI-ANALYZED® Reagent
For Organic Residue Analysis

Avantor™



Material No.: 9254-03

Batch No.: 24H2762008

Manufactured Date: 2024-04-18

Expiration Date: 2027-04-18

Revision No.: 0

Certificate of Analysis

| Test | Specification | Result |
|---|---------------|-------------|
| Assay ((CH ₃) ₂ CO) (by GC, corrected for water) | >= 99.4 % | 100.0 % |
| Color (APHA) | <= 10 | 5 |
| Residue after Evaporation | <= 1.0 ppm | 0.0 ppm |
| Substances Reducing Permanganate | Passes Test | Passes Test |
| Titration Acid (µeq/g) | <= 0.3 | 0.2 |
| Titration Base (µeq/g) | <= 0.6 | <0.1 |
| Water (H ₂ O) | <= 0.5 % | <0.1 % |
| FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL) | <= 5 | 1 |
| ECD Sensitive Impurities (as Heptachlor Epoxide) Single Peak (pg/mL) | <= 10 | 1 |

For Laboratory, Research, or Manufacturing Use

MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: United States

Packaging Site: Phillipsburg Mfg Ctr & DC

Reed on 7/2/25

E3949

Jamie Croak
Director Quality Operations, Bioscience Production

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Avantor Performance Materials LLC



| | |
|----------------------|--------------------------------|
| Material | BDH9274-2.5KG |
| Material Description | BDH SAND STDD OTTAWA W+I 2.5KG |
| Grade | NOT APPLICABLE |
| Batch | 25A2756718 |
| Reassay Date | 12/31/2028 |
| CAS Number | 14808-60-7 |
| Molecular Formula | SiO ₂ |
| Molecular Mass | 60.09 |
| Date of Manufacture | 12/05/2024 |
| Storage | Room Temperature |

| Characteristics | Specifications | Measured Values |
|-------------------------------|-----------------|-----------------|
| Appearance | Beige granules. | Beige granules. |
| Moisture | <= 0.1 % | 0.1 % |
| Particle Size 30-40 mesh | >= 80 % | 99 % |
| CUSTOMER PART # BDH9274-2.5KG | | |

Received on 1/12/25.

E3951

Internal ID #: 793

| Signature | Additional Information |
|---|--|
| <p>We certify that this batch conforms to the specifications listed above.</p> <p>This document has been electronically produced and is valid without a signature.</p> <p>Leona Edwardson, Quality Control Sr. Manager - Solon VWR Chemicals, LLC. 28600 Fountain Parkway, Solon OH 44139 USA</p> | <p>Analysis may have been rounded to significant digits in specification limits</p> <p>Product meets analytical specifications of the grades listed.</p> |

Methylene Chloride
ULTRA RESI-ANALYZED
For Organic Residue Analysis
(dichloromethane)



Material No.: 9266-A4
Batch No.: 25B1862001
Manufactured Date: 2024-12-18
Expiration Date: 2026-03-19
Revision No.: 0

Certificate of Analysis

| Test | Specification | Result |
|--|----------------|---------|
| FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL) | ≤ 5 | <1 |
| ECD Sensitive Impurities (as HeptachlorEpoxide) Single Peak (pg/mL) | ≤ 10 | 2 |
| Assay (CH ₂ Cl ₂) (by GC, exclusive of preservative, corrected for water) | $\geq 99.8 \%$ | 99.9 % |
| Color (APHA) | ≤ 10 | 5 |
| Residue after Evaporation | ≤ 1.0 ppm | 0.3 ppm |
| Titration Acid (μ eq/g) | ≤ 0.3 | <0.1 |
| Chloride (Cl) | ≤ 10 ppm | <5 ppm |
| Water (by KF, coulometric) | $\leq 0.02 \%$ | <0.01 % |

For Laboratory, Research, or Manufacturing Use
MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: United States
Packaging Site: Phillipsburg Mfg Ctr & DC

RS
7/14/25

E3954

Jamie Croak
Director Quality Operations, Bioscience Production

n-Hexane 95%
ULTRA RESI-ANALYZED
For Organic Residue Analysis

 **avantors**[™]



Material No.: 9262-03

Batch No.: 25C0362005

Manufactured Date: 2025-01-29

Expiration Date: 2026-04-30

Revision No.: 0

Certificate of Analysis

| Test | Specification | Result |
|--|----------------|-------------|
| FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL) | ≤ 5 | 1 |
| ECD Sensitive Impurities (as HeptachlorEpoxide) Single Peak (pg/mL) | ≤ 10 | 6 |
| ECD-Sensitive Impurities (as EthyleneDibromide) - Single Impurity Peak (ng/mL) | ≤ 5 | 5 |
| Assay (Total Saturated C ₆ Isomers) (by GC, corrected for water) | $\geq 99.5 \%$ | 100.0 % |
| Assay (as n-Hexane) (by GC, corrected for water) | $\geq 95 \%$ | 100 % |
| Color (APHA) | ≤ 10 | 10 |
| Residue after Evaporation | ≤ 1.0 ppm | 0.1 ppm |
| Substances Darkened by H ₂ SO ₄ | Passes Test | Passes Test |
| Water (by KF, coulometric) | $\leq 0.05 \%$ | $< 0.01 \%$ |

For Laboratory, Research, or Manufacturing Use

MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: United States

Packaging Site: Phillipsburg Mfg Ctr & DC

Received on 7/16/25

E3956



Jamie Croak
Director Quality Operations, Bioscience Production



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: (800)356-1688
Fax: (814)353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 30540 **Lot No.:** A0190424

Description : NJEPH Aliphatics Calibration Standard

Aliphatics Calibration Standard 2000µg/mL, Hexane/Carbon Disulfide (80:20), 1mL/ampul

Container Size : 2 mL **Pkg Amt:** > 1 mL

Expiration Date : November 30, 2029 **Storage:** 25°C nominal

Handling: Sonicate prior to use. **Ship:** Ambient

P12361
↓
P12370 } Y.P.
031/6/23

CERTIFIED VALUES

| Elution Order | Compound | Grav. Conc. (weight/volume) | Expanded Uncertainty (95% C.L.; K=2) | |
|---------------|---|-----------------------------|---|--|
| 1 | n-Nonane (C9) CAS # 111-84-2 Purity 99% (Lot SHBN5361) | 2,014.0 µg/mL | +/- 11.8193 +/- 50.0027 +/- 59.9491 | µg/mL Gravimetric Unstressed Stressed |
| 2 | n-Decane (C10) CAS # 124-18-5 Purity 99% (Lot SHBN8619) | 2,014.7 µg/mL | +/- 11.8232 +/- 50.0193 +/- 59.9689 | µg/mL Gravimetric Unstressed Stressed |
| 3 | Naphthalene CAS # 91-20-3 Purity 99% (Lot MKCH0219) | 2,015.3 µg/mL | +/- 11.8271 +/- 50.0358 +/- 59.9888 | µg/mL Gravimetric Unstressed Stressed |
| 4 | n-Dodecane (C12) CAS # 112-40-3 Purity 99% (Lot SHBN7174) | 2,008.0 µg/mL | +/- 11.7841 +/- 49.8538 +/- 59.7705 | µg/mL Gravimetric Unstressed Stressed |
| 5 | 2-Methylnaphthalene CAS # 91-57-6 Purity 96% (Lot STBK0259) | 2,007.0 µg/mL | +/- 11.7784 +/- 49.8299 +/- 59.7419 | µg/mL Gravimetric Unstressed Stressed |
| 6 | n-Tetradecane (C14) CAS # 629-59-4 Purity 99% (Lot STBK2282) | 2,016.7 µg/mL | +/- 11.8349 +/- 50.0689 +/- 60.0284 | µg/mL Gravimetric Unstressed Stressed |
| 7 | n-Hexadecane (C16) CAS # 544-76-3 Purity 98% (Lot SHBM4146) | 2,014.9 µg/mL | +/- 11.8244 +/- 50.0246 +/- 59.9753 | µg/mL Gravimetric Unstressed Stressed |

| | | | | | | | |
|---|--|------------------|---------------|-----|---------|-------|-------------|
| 8 | n-Octadecane (C18) CAS # 593-45-3 Purity 97% | (Lot VZKOJ) | 2,004.7 µg/mL | +/- | 11.7645 | µg/mL | Gravimetric |
| | | | | +/- | 49.7710 | µg/mL | Unstressed |
| | | | | +/- | 59.6712 | µg/mL | Stressed |
| 9 | n-Eicosane (C20) CAS # 112-95-8 Purity 99% | (Lot MKCF7888) | 2,018.0 µg/mL | +/- | 11.8428 | µg/mL | Gravimetric |
| | | | | +/- | 50.1020 | µg/mL | Unstressed |
| | | | | +/- | 60.0681 | µg/mL | Stressed |
| 10 | n-Heneicosane (C21) CAS # 629-94-7 Purity 99% | (Lot MKCL3226) | 2,000.7 µg/mL | +/- | 11.7410 | µg/mL | Gravimetric |
| | | | | +/- | 49.6717 | µg/mL | Unstressed |
| | | | | +/- | 59.5522 | µg/mL | Stressed |
| 11 | n-Docosane (C22) CAS # 629-97-0 Purity 99% | (Lot MKCL8918) | 2,005.3 µg/mL | +/- | 11.7684 | µg/mL | Gravimetric |
| | | | | +/- | 49.7876 | µg/mL | Unstressed |
| | | | | +/- | 59.6911 | µg/mL | Stressed |
| 12 | n-Tetracosane (C24) CAS # 646-31-1 Purity 99% | (Lot MKCN2863) | 2,018.0 µg/mL | +/- | 11.8428 | µg/mL | Gravimetric |
| | | | | +/- | 50.1020 | µg/mL | Unstressed |
| | | | | +/- | 60.0681 | µg/mL | Stressed |
| 13 | n-Hexacosane (C26) CAS # 630-01-3 Purity 99% | (Lot MKCD4540) | 2,014.0 µg/mL | +/- | 11.8193 | µg/mL | Gravimetric |
| | | | | +/- | 50.0027 | µg/mL | Unstressed |
| | | | | +/- | 59.9491 | µg/mL | Stressed |
| 14 | n-Octacosane (C28) CAS # 630-02-4 Purity 99% | (Lot BCCG0084) | 2,002.0 µg/mL | +/- | 11.7489 | µg/mL | Gravimetric |
| | | | | +/- | 49.7048 | µg/mL | Unstressed |
| | | | | +/- | 59.5919 | µg/mL | Stressed |
| 15 | n-Triacontane (C30) CAS # 638-68-6 Purity 97% | (Lot MKCQ9436) | 2,011.1 µg/mL | +/- | 11.8025 | µg/mL | Gravimetric |
| | | | | +/- | 49.9316 | µg/mL | Unstressed |
| | | | | +/- | 59.8637 | µg/mL | Stressed |
| 16 | n-Dotriacontane (C32) CAS # 544-85-4 Purity 99% | (Lot BCBW0661) | 2,012.0 µg/mL | +/- | 11.8075 | µg/mL | Gravimetric |
| | | | | +/- | 49.9531 | µg/mL | Unstressed |
| | | | | +/- | 59.8895 | µg/mL | Stressed |
| 17 | n-Tetratriacontane (C34) CAS # 14167-59-0 Purity 99% | (Lot OML4N) | 2,006.7 µg/mL | +/- | 11.7762 | µg/mL | Gravimetric |
| | | | | +/- | 49.8207 | µg/mL | Unstressed |
| | | | | +/- | 59.7308 | µg/mL | Stressed |
| 18 | n-Hexatriacontane (C36) CAS # 630-06-8 Purity 99% | (Lot Z27H018) | 2,017.3 µg/mL | +/- | 11.8388 | µg/mL | Gravimetric |
| | | | | +/- | 50.0855 | µg/mL | Unstressed |
| | | | | +/- | 60.0483 | µg/mL | Stressed |
| 19 | n-Octatriacontane (C38) CAS # 7194-85-6 Purity 96% | (Lot 0000145137) | 2,017.3 µg/mL | +/- | 11.8385 | µg/mL | Gravimetric |
| | | | | +/- | 50.0842 | µg/mL | Unstressed |
| | | | | +/- | 60.0467 | µg/mL | Stressed |
| 20 | n-Tetracontane (C40) CAS # 4181-95-7 Purity 99% | (Lot BSBME) | 2,008.7 µg/mL | +/- | 11.7880 | µg/mL | Gravimetric |
| | | | | +/- | 49.8703 | µg/mL | Unstressed |
| | | | | +/- | 59.7903 | µg/mL | Stressed |
| Solvent: Hexane/Carbon disulfide (80:20) | | | | | | | |
| | CAS # 110-54-3/75-15-0 | | | | | | |
| | Purity 99% | | | | | | |

Column:
30m x 0.25mm x 0.25µm
Pxx-5 (cat.#10223)


Carrier Gas:
hydrogen-constant pressure 10 psi.

Temp. Program:
40°C (hold 2 min.) to 330°C
@ 10°C/min. (hold 10 min.)

Inj. Temp:
250°C

Det. Temp:
330°C

Det. Type:
FID

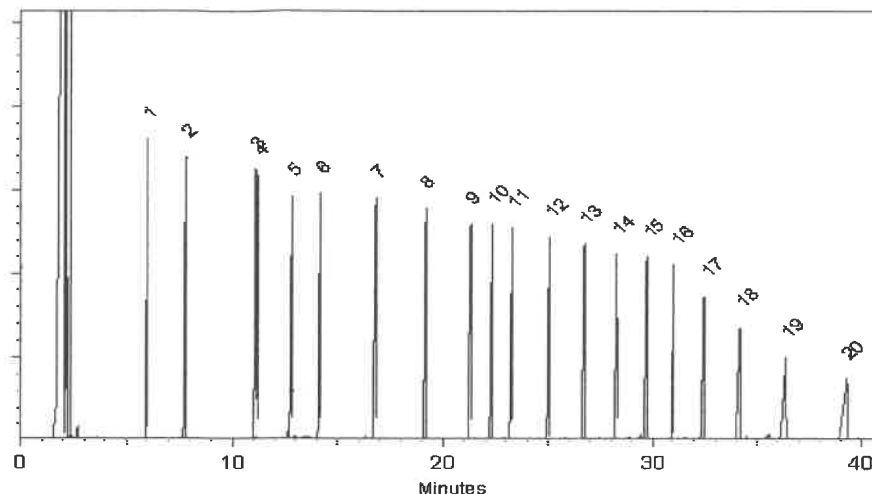

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.


Morgan Craighead - Mix Technician

Date Mixed: 10-Oct-2022 Balance: 1128360905


Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 20-Oct-2022

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified combined stressed uncertainty value (includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ stressed} = k \sqrt{U_{gravimetric}^2 + U_{homogeneity}^2 + U_{storage\ stability}^2 + U_{shipping\ stability}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- It is important to note that the shipping stability uncertainty was obtained under temperature extremes for specific time intervals; therefore, the certified combined stressed uncertainty value should only be applied to the product if it was stored at non-standard temperature conditions up to and including 7 days. Contact Restek Technical Service at www.restek.com/Contact-Us for use recommendations if your shipment was in-transit for more than 7 days at non-standard temperature conditions.
- Apply the certified combined unstressed uncertainty value if the product was received under standard shipping conditions. Apply the certified combined stressed uncertainty value if the product was received under non-standard conditions as specified below.

| Label Conditions | Standard Conditions | Non-Standard Conditions |
|---|---------------------|-------------------------|
| 25°C Nominal (Room Temperature) | < 60°C | ≥ 60°C up to 7 days |
| 10°C or colder (Refrigerate) | < 40°C | ≥ 40°C up to 7 days |
| 0°C or colder (Freezer) -20°C or colder (Deep Freezer) | < 25°C | ≥ 25°C up to 7 days |

- Separate (not combined) uncertainty values for gravimetric uncertainty are also displayed on the certificate, if needed, separate homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty values are available by contacting Restek Technical Service at www.restek.com/Contact-Us.
- The packaged amount is the minimum sample size for which uncertainty is valid. The ampules are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampules. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No.: 31098 **Lot No.:** A0204989

Description: 1-Chlorooctadecane Standard

1-Chlorooctadecane Standard 10,000µg/mL, Methylene Chloride, 1mL/ampul

Container Size: 2 mL **Pkg Amt:** > 1 mL

Expiration Date: January 31, 2031 **Storage:** 10°C or colder

Ship: Ambient

P12960
↓
P12991 } Y.P.
12/21/2023

CERTIFIED VALUES

| Elution Order | Compound | CAS # | Lot # | Purity | Grav. Conc. (weight/volume) | Expanded Uncertainty * (95% C.L.; K=2) |
|---------------|--------------------|-----------|----------|--------|-----------------------------|--|
| 1 | 1-Chlorooctadecane | 3386-33-2 | 14738400 | 99% | 10,097.3 µg/mL | +/- 567.2675 |

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Methylene chloride
CAS # 75-09-2
Purity 99%

Quality Confirmation Test

Column:

30m x 0.25mm x 0.25µm
Rtx-5 (cat.#10223)

Carrier Gas:

hydrogen-constant pressure 10 psi.

Temp. Program:

75°C (hold 1 min.) to 330°C
@ 20°C/min. (hold 10 min.)

Inj. Temp:

250°C

Det. Temp:

330°C

Det. Type:


FID

Split Vent:

10 ml/min.

Inj. Vol

1µl

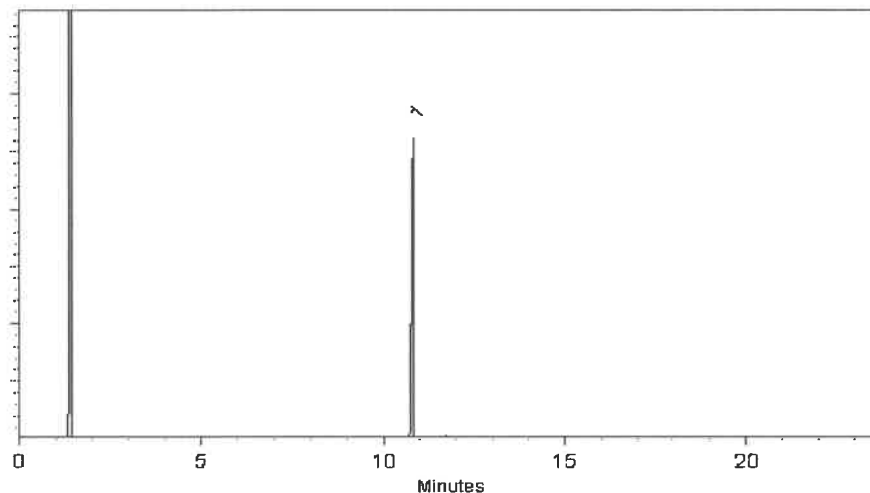

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Peter Robbins - Operations Technician I

Date Mixed: 02-Dec-2023

Balance Serial # B345965662

Christie Mills - Operations Lead Tech - ARM QC

Date Passed: 08-Dec-2023

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No.: 31098 **Lot No.:** A0204989
Description: 1-Chlorooctadecane Standard
1-Chlorooctadecane Standard 10,000µg/mL, Methylene Chloride, 1mL/ampul
Container Size: 2 mL **Pkg Amt:** > 1 mL
Expiration Date: January 31, 2031 **Storage:** 10°C or colder
Ship: Ambient

P12960
↓
P12991 } Y.P.
12/21/2023

CERTIFIED VALUES

| Elution Order | Compound | CAS # | Lot # | Purity | Grav. Conc. (weight/volume) | Expanded Uncertainty * (95% C.L.; K=2) |
|---------------|--------------------|-----------|----------|--------|-----------------------------|--|
| 1 | 1-Chlorooctadecane | 3386-33-2 | 14738400 | 99% | 10,097.3 µg/mL | +/- 567.2675 |

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Methylene chloride
CAS # 75-09-2
Purity 99%

Quality Confirmation Test

Column:

30m x 0.25mm x 0.25µm
Rtx-5 (cat.#10223)

Carrier Gas:

hydrogen-constant pressure 10 psi.

Temp. Program:

75°C (hold 1 min.) to 330°C
@ 20°C/min. (hold 10 min.)

Inj. Temp:

250°C

Det. Temp:

330°C

Det. Type:


FID

Split Vent:

10 ml/min.

Inj. Vol

1µl

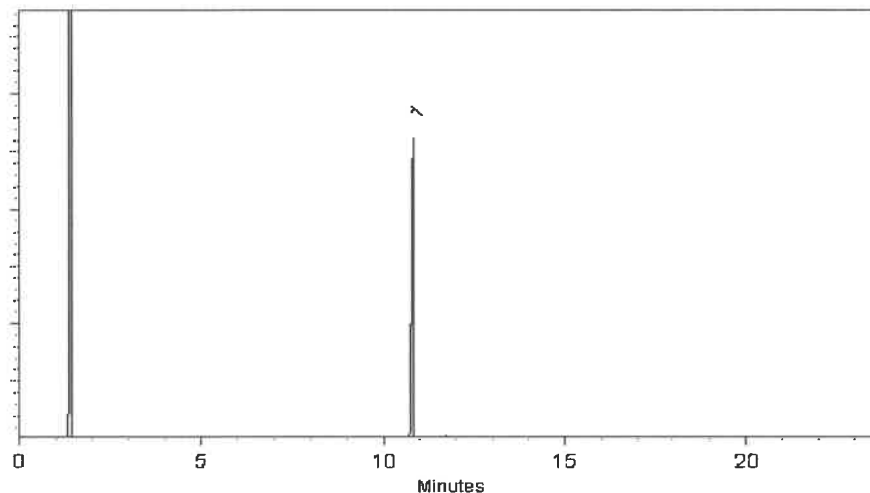

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Peter Robbins - Operations Technician I

Date Mixed: 02-Dec-2023

Balance Serial # B345965662

Christie Mills - Operations Lead Tech - ARM QC

Date Passed: 08-Dec-2023

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.


- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



CERTIFIED WEIGHT REPORT

Part Number: 95999

Lot Number: 040524

Description: NJ EPH Aliphatic n-Hydrocarbons - Revised
20 components

Expiration Date: 040534

Recommended Storage: Ambient (20 °C)

Nominal Concentration (µg/mL): 1000

NIST Test ID#: 6UTB

Weight(s) shown below were combined and diluted to (mL):

CAUTION: Sonicate Before Use

Solvent(s):
Cyclohexane

Lot#
28930

P13278
2
P13287
Y.P.
04/11/24

5E-05 Balance Uncertainty
0.001 Flask Uncertainty

| | | | |
|----------------|-----------------|--------|------|
| Formulated By: | Anthony Mahoney | 040524 | DATE |
| Reviewed By: | Pedro L. Rentas | 040524 | DATE |

| Compound | | Part Number | (RM#) | Lot Number | DIL Factor | Initial Vol. (mL) | Initial Conc (µg/mL) | Nominal Conc (µg/mL) | Purity (%) | Purity Uncertainty | Pipette | Target Weight(g) | Actual Weight(g) | Actual Conc (µg/mL) | Expanded Uncertainty (+/-) (µg/mL) | SDS Information | |
|----------|---------------------|-------------|-----------|------------|------------|-------------------|----------------------|----------------------|------------|--------------------|---------|------------------|------------------|---------------------|------------------------------------|--|---|
| | | | | | | | | | | | | | | | | (Solvent Safety Info. On Attached pg.) | |
| | | | | | | | | | | | | | | | | OSHA PEL (TWA) | |
| | | | | | | | | | | | | | | | | CAS# | |
| 1. | 2-Methylnaphthalene | (0214) | MKBF3783V | NA | NA | NA | NA | 1000 | 97 | 0.2 | NA | 0.02579 | 0.02594 | 1005.7 | 5.7 | 91-57-6 | N/A |
| 2. | Naphthalene | (0222) | MKB28680V | NA | NA | NA | NA | 1000 | 100 | 0.2 | NA | 0.02502 | 0.02511 | 1003.7 | 5.7 | 91-20-3 | 10 ppm (50mg/m ³ 8H) orl-rat 1630mg/kg |
| 3. | n-Nonane | 95708 | 120222 | 1.00 | 25.00 | 1000.7 | 1000.7 | 1000 | NA | NA | 0.013 | NA | NA | 1000.0 | 4.2 | 111-84-2 | 200 ppm (1050mg/m ³ 8H) orl-rat 490mg/kg |
| 4. | n-Decane | 95708 | 120222 | 1.00 | 25.00 | 1000.9 | 1000.9 | 1000 | NA | NA | 0.013 | NA | NA | 1000.2 | 4.2 | 124-18-5 | ivn-mus 218mg/kg |
| 5. | n-Dodecane | 95708 | 120222 | 1.00 | 25.00 | 1000.7 | 1000.7 | 1000 | NA | NA | 0.013 | NA | NA | 1000.0 | 4.2 | 112-40-3 | N/A |
| 6. | n-Tetradecane | 95708 | 120222 | 1.00 | 25.00 | 1002.1 | 1002.1 | 1000 | NA | NA | 0.013 | NA | NA | 1001.3 | 4.2 | 629-59-4 | ivn-mus 3494mg/kg |
| 7. | n-Hexadecane | 95708 | 120222 | 1.00 | 25.00 | 1000.5 | 1000.5 | 1000 | NA | NA | 0.013 | NA | NA | 999.7 | 4.2 | 544-76-3 | N/A |
| 8. | n-Octadecane | 95708 | 120222 | 1.00 | 25.00 | 1001.0 | 1001.0 | 1000 | NA | NA | 0.013 | NA | NA | 1000.3 | 4.1 | 583-45-3 | N/A |
| 9. | n-Eicosane | 95708 | 120222 | 1.00 | 25.00 | 1001.0 | 1001.0 | 1000 | NA | NA | 0.013 | NA | NA | 1000.3 | 4.2 | 112-95-8 | N/A |
| 10. | n-Henicosane | 95708 | 120222 | 1.00 | 25.00 | 1002.4 | 1002.4 | 1000 | NA | NA | 0.013 | NA | NA | 1001.6 | 4.2 | 629-94-7 | N/A |
| 11. | n-Docosane | 95708 | 120222 | 1.00 | 25.00 | 1001.9 | 1001.9 | 1000 | NA | NA | 0.013 | NA | NA | 1001.2 | 4.2 | 629-97-0 | N/A |
| 12. | n-Triacosane | 95708 | 120222 | 1.00 | 25.00 | 1000.8 | 1000.8 | 1000 | NA | NA | 0.013 | NA | NA | 1000.1 | 4.2 | 646-31-1 | N/A |
| 13. | n-Hexacosane | 95708 | 120222 | 1.00 | 25.00 | 1001.2 | 1001.2 | 1000 | NA | NA | 0.013 | NA | NA | 1000.4 | 4.2 | 630-01-3 | N/A |
| 14. | n-Octacosane | 95708 | 120222 | 1.00 | 25.00 | 1000.5 | 1000.5 | 1000 | NA | NA | 0.013 | NA | NA | 999.8 | 4.2 | 630-02-4 | N/A |
| 15. | n-Triacontane | 95708 | 120222 | 1.00 | 25.00 | 1000.5 | 1000.5 | 1000 | NA | NA | 0.013 | NA | NA | 999.8 | 4.2 | 638-68-6 | N/A |
| 16. | n-Dotriacontane | 95708 | 120222 | 1.00 | 25.00 | 1000.5 | 1000.5 | 1000 | NA | NA | 0.013 | NA | NA | 999.8 | 4.3 | 544-85-4 | ivn-mus 100mg/kg |
| 17. | n-Tetraacontane | 95708 | 120222 | 1.00 | 25.00 | 1000.4 | 1000.4 | 1000 | NA | NA | 0.013 | NA | NA | 999.7 | 4.2 | 14167-59-0 | N/A |
| 18. | n-Hexatriacontane | 95708 | 120222 | 1.00 | 25.00 | 1001.5 | 1001.5 | 1000 | NA | NA | 0.013 | NA | NA | 1000.8 | 4.2 | 630-06-8 | N/A |
| 19. | n-Octatriacontane | 95708 | 120222 | 1.00 | 25.00 | 1000.3 | 1000.3 | 1000 | NA | NA | 0.013 | NA | NA | 999.6 | 4.3 | 7184-86-6 | N/A |
| 20. | n-Tetracontane | 95708 | 120222 | 1.00 | 25.00 | 1000.6 | 1000.6 | 1000 | NA | NA | 0.013 | NA | NA | 999.9 | 4.3 | 4181-95-7 | N/A |

* The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
* Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
* Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
* All Standards, after opening ampule, should be stored with caps tight and under appropriate laboratory conditions.
* Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 31098 **Lot No.:** A0213283

Description : 1-Chlorooctadecane Standard

1-Chlorooctadecane Standard 10,000µg/mL, Methylene Chloride, 1mL/ampul

Container Size : 2 mL **Pkg Amt:** > 1 mL

Expiration Date : July 31, 2031 **Storage:** 10°C or colder

Ship: Ambient

P13595
↓
P13624 } Y.P.
10/16/24

CERTIFIED VALUES

| Elution Order | Compound | CAS # | Lot # | Purity | Grav. Conc. (weight/volume) | Expanded Uncertainty * (95% C.L.; K=2) |
|---------------|--------------------|-----------|----------|--------|-----------------------------|--|
| 1 | 1-Chlorooctadecane | 3386-33-2 | 15018900 | 99% | 10,058.0 µg/mL | +/- 565.0578 |

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Methylene chloride
CAS # 75-09-2
Purity 99%

Quality Confirmation Test

Column:

30m x 0.25mm x 0.25µm
Rtx-S (cat.#10223)

Carrier Gas:

hydrogen-constant pressure 10 psi.

Temp. Program:

75°C (hold 1 min.) to 330°C
@ 20°C/min. (hold 10 min.)

Inj. Temp:

250°C

Det. Temp:

330°C

Det. Type:


FID

Split Vent:

10 ml/min.

Inj. Vol

1µl

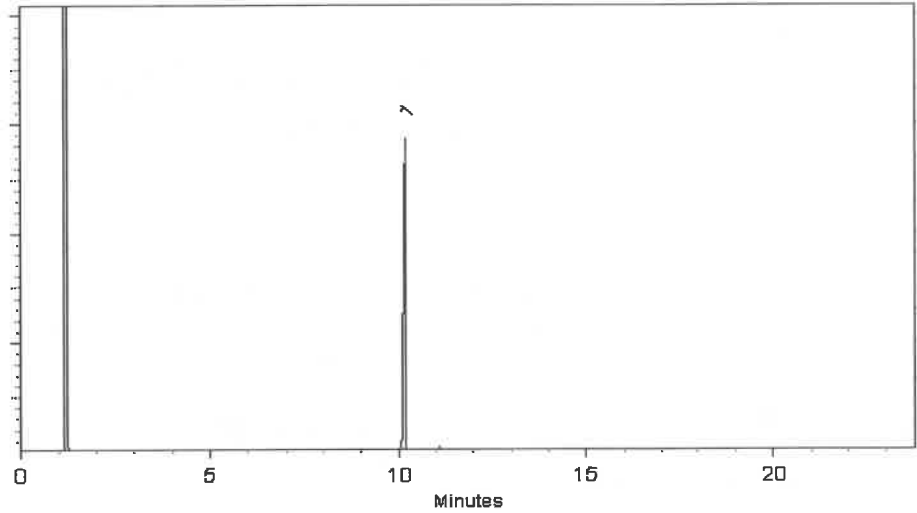

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Stacey Wanner - Operations Technician I

Date Mixed: 28-Jun-2024

Balance Serial # B345965662

Dillan Murphy - Operations Technician I

Date Passed: 01-Jul-2024

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 31098 **Lot No.:** A0213283

Description : 1-Chlorooctadecane Standard

1-Chlorooctadecane Standard 10,000µg/mL, Methylene Chloride, 1mL/ampul

Container Size : 2 mL **Pkg Amt:** > 1 mL

Expiration Date : July 31, 2031 **Storage:** 10°C or colder

Ship: Ambient

P13595
↓
P13624 } Y.P.
10/16/24

CERTIFIED VALUES

| Elution Order | Compound | CAS # | Lot # | Purity | Grav. Conc. (weight/volume) | Expanded Uncertainty * (95% C.L.; K=2) |
|---------------|--------------------|-----------|----------|--------|-----------------------------|--|
| 1 | 1-Chlorooctadecane | 3386-33-2 | 15018900 | 99% | 10,058.0 µg/mL | +/- 565.0578 |

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Methylene chloride
CAS # 75-09-2
Purity 99%

Quality Confirmation Test

Column:

30m x 0.25mm x 0.25µm
Rtx-S (cat.#10223)

Carrier Gas:

hydrogen-constant pressure 10 psi.

Temp. Program:

75°C (hold 1 min.) to 330°C
@ 20°C/min. (hold 10 min.)

Inj. Temp:

250°C

Det. Temp:

330°C

Det. Type:


FID

Split Vent:

10 ml/min.

Inj. Vol

1µl

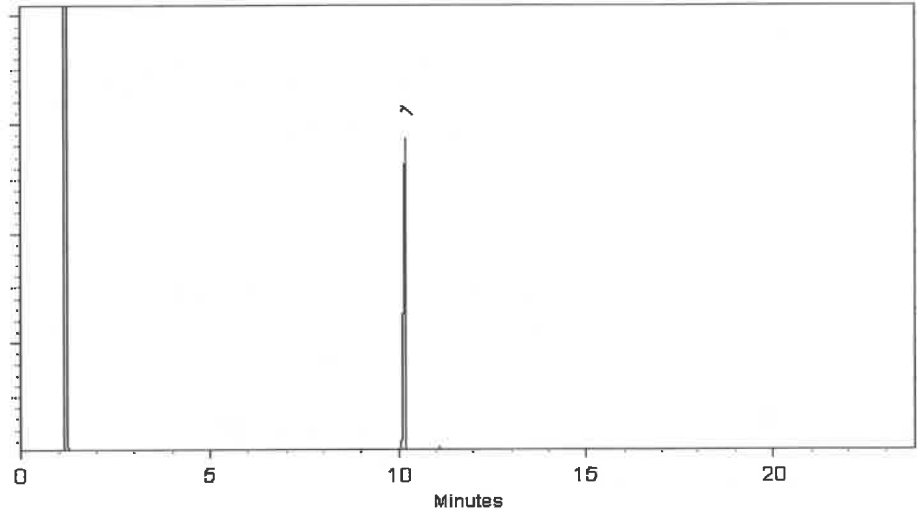

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Stacey Wanner - Operations Technician I

Date Mixed: 28-Jun-2024

Balance Serial # B345965662

Dillan Murphy - Operations Technician I

Date Passed: 01-Jul-2024

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 31098 **Lot No.:** A0213283

Description : 1-Chlorooctadecane Standard

1-Chlorooctadecane Standard 10,000µg/mL, Methylene Chloride, 1mL/ampul

Container Size : 2 mL **Pkg Amt:** > 1 mL

Expiration Date : July 31, 2031 **Storage:** 10°C or colder

Ship: Ambient

P13595
↓
P13624 } Y.P.
10/16/24

CERTIFIED VALUES

| Elution Order | Compound | CAS # | Lot # | Purity | Grav. Conc. (weight/volume) | Expanded Uncertainty * (95% C.L.; K=2) |
|---------------|--------------------|-----------|----------|--------|-----------------------------|--|
| 1 | 1-Chlorooctadecane | 3386-33-2 | 15018900 | 99% | 10,058.0 µg/mL | +/- 565.0578 |

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Methylene chloride
CAS # 75-09-2
Purity 99%

Quality Confirmation Test

Column:

30m x 0.25mm x 0.25µm
Rtx-S (cat.#10223)

Carrier Gas:

hydrogen-constant pressure 10 psi.

Temp. Program:

75°C (hold 1 min.) to 330°C
@ 20°C/min. (hold 10 min.)

Inj. Temp:

250°C

Det. Temp:

330°C

Det. Type:


FID

Split Vent:

10 ml/min.

Inj. Vol

1µl

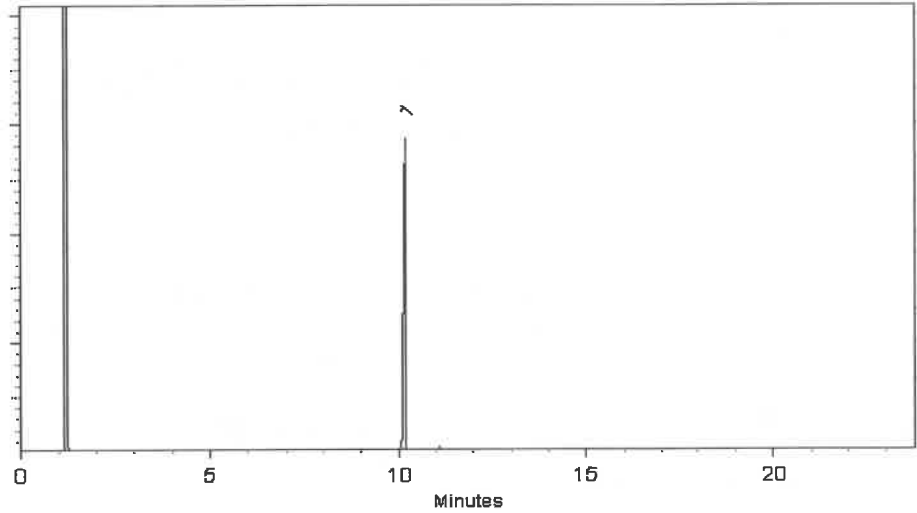

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Stacey Wanner - Operations Technician I

Date Mixed: 28-Jun-2024

Balance Serial # B345965662

Dillan Murphy - Operations Technician I

Date Passed: 01-Jul-2024

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 31098 **Lot No.:** A0213283

Description : 1-Chlorooctadecane Standard

1-Chlorooctadecane Standard 10,000µg/mL, Methylene Chloride, 1mL/ampul

Container Size : 2 mL **Pkg Amt:** > 1 mL

Expiration Date : July 31, 2031 **Storage:** 10°C or colder

Ship: Ambient

P13595
↓
P13624 } Y.P.
10/16/24

CERTIFIED VALUES

| Elution Order | Compound | CAS # | Lot # | Purity | Grav. Conc. (weight/volume) | Expanded Uncertainty * (95% C.L.; K=2) |
|---------------|--------------------|-----------|----------|--------|-----------------------------|--|
| 1 | 1-Chlorooctadecane | 3386-33-2 | 15018900 | 99% | 10,058.0 µg/mL | +/- 565.0578 |

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Methylene chloride
CAS # 75-09-2
Purity 99%

Quality Confirmation Test

Column:

30m x 0.25mm x 0.25µm
Rtx-S (cat.#10223)

Carrier Gas:

hydrogen-constant pressure 10 psi.

Temp. Program:

75°C (hold 1 min.) to 330°C
@ 20°C/min. (hold 10 min.)

Inj. Temp:

250°C

Det. Temp:

330°C

Det. Type:


FID

Split Vent:

10 ml/min.

Inj. Vol

1µl

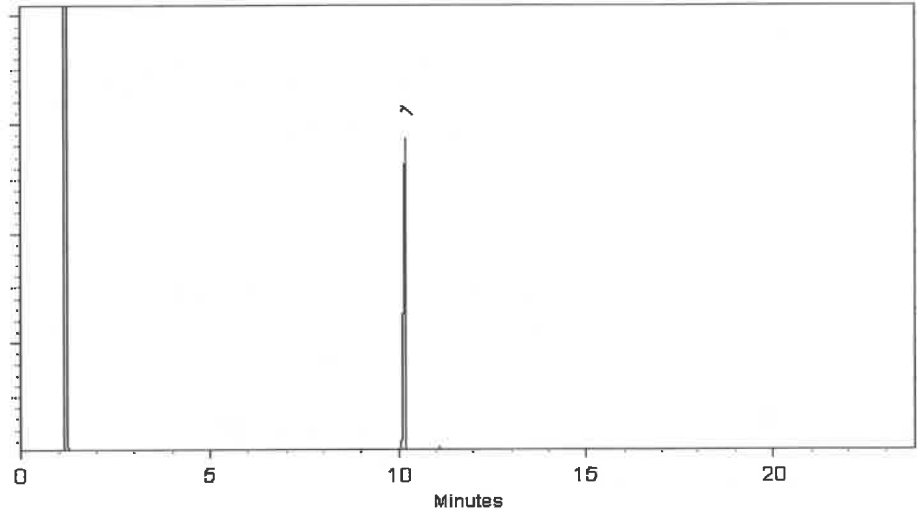

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Stacey Wanner - Operations Technician I

Date Mixed: 28-Jun-2024

Balance Serial # B345965662

Dillan Murphy - Operations Technician I

Date Passed: 01-Jul-2024

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 31097 **Lot No.:** A0216631
Description : o-Terphenyl Standard
o-Terphenyl Standard 10,000 µg/mL, Methylene Chloride, 1mL/ampul
Container Size : 2 mL **Pkg Amt:** > 1 mL
Expiration Date : April 30, 2028 **Storage:** 10°C or colder
Handling: Sonicate prior to use. **Ship:** Ambient

P13645 } Y.P.
↓
P13694 } 10/16/24

CERTIFIED VALUES

| Elution Order | Compound | CAS # | Lot # | Purity | Grav. Conc. (weight/volume) | Expanded Uncertainty * (95% C.L.; K=2) |
|---------------|-------------|---------|-------|--------|-----------------------------|--|
| 1 | o-Terphenyl | 84-15-1 | GKSSA | 99% | 10,065.0 µg/mL | +/- 453.3336 |

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Methylene chloride
CAS # 75-09-2
Purity 99%

Quality Confirmation Test

Column:

30m x 0.25mm x 0.25µm
Rtx-5 (cat.#10223)

Carrier Gas:

hydrogen-constant pressure 10 psi.

Temp. Program:

75°C (hold 1 min.) to 330°C
@ 20°C/min. (hold 10 min.)

Inj. Temp:

250°C

Det. Temp:

330°C

Det. Type:


FID

Split Vent:

10 ml/min.

Inj. Vol

1µl

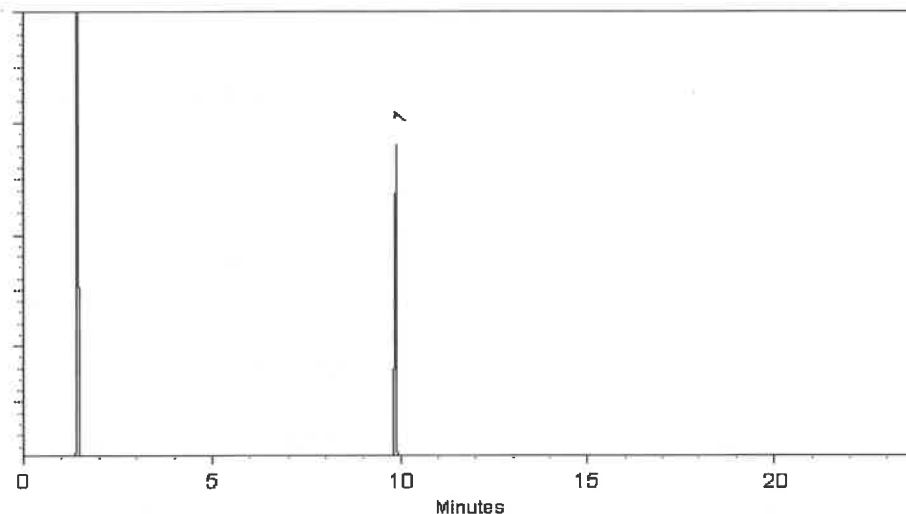

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Ven Kelley - Operations Tech I

Date Mixed: 17-Sep-2024

Balance Serial # 1128353505

Dillan Murphy - Operations Technician I

Date Passed: 23-Sep-2024

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/ μ ECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 31097 **Lot No.:** A0216631
Description : o-Terphenyl Standard
o-Terphenyl Standard 10,000 µg/mL, Methylene Chloride, 1mL/ampul
Container Size : 2 mL **Pkg Amt:** > 1 mL
Expiration Date : April 30, 2028 **Storage:** 10°C or colder
Handling: Sonicate prior to use. **Ship:** Ambient

P13645 } Y.P.
↓
P13694 } 10/16/24

CERTIFIED VALUES

| Elution Order | Compound | CAS # | Lot # | Purity | Grav. Conc. (weight/volume) | Expanded Uncertainty * (95% C.L.; K=2) |
|---------------|-------------|---------|-------|--------|-----------------------------|--|
| 1 | o-Terphenyl | 84-15-1 | GKSSA | 99% | 10,065.0 µg/mL | +/- 453.3336 |

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Methylene chloride
CAS # 75-09-2
Purity 99%

Quality Confirmation Test

Column:

30m x 0.25mm x 0.25µm
Rtx-5 (cat.#10223)

Carrier Gas:

hydrogen-constant pressure 10 psi.

Temp. Program:

75°C (hold 1 min.) to 330°C
@ 20°C/min. (hold 10 min.)

Inj. Temp:

250°C

Det. Temp:

330°C

Det. Type:

FID

Split Vent:

10 ml/min.

Inj. Vol

1µl



This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Ven Kelley - Operations Tech I

Date Mixed: 17-Sep-2024

Balance Serial # 1128353505

Dillan Murphy - Operations Technician I

Date Passed: 23-Sep-2024

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 31097 **Lot No.:** A0216631
Description : o-Terphenyl Standard
o-Terphenyl Standard 10,000 µg/mL, Methylene Chloride, 1mL/ampul
Container Size : 2 mL **Pkg Amt:** > 1 mL
Expiration Date : April 30, 2028 **Storage:** 10°C or colder
Handling: Sonicate prior to use. **Ship:** Ambient

P13645 } Y.P.
↓
P13694 } 10/16/24

CERTIFIED VALUES

| Elution Order | Compound | CAS # | Lot # | Purity | Grav. Conc. (weight/volume) | Expanded Uncertainty * (95% C.L.; K=2) |
|---------------|-------------|---------|-------|--------|-----------------------------|--|
| 1 | o-Terphenyl | 84-15-1 | GKSSA | 99% | 10,065.0 µg/mL | +/- 453.3336 |

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Methylene chloride
CAS # 75-09-2
Purity 99%

Quality Confirmation Test

Column:

30m x 0.25mm x 0.25µm
Rtx-5 (cat.#10223)

Carrier Gas:

hydrogen-constant pressure 10 psi.

Temp. Program:

75°C (hold 1 min.) to 330°C
@ 20°C/min. (hold 10 min.)

Inj. Temp:

250°C

Det. Temp:

330°C

Det. Type:

FID

Split Vent:

10 ml/min.

Inj. Vol

1µl



This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Ven Kelley - Operations Tech I

Date Mixed: 17-Sep-2024

Balance Serial # 1128353505

Dillan Murphy - Operations Technician I

Date Passed: 23-Sep-2024

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 31097 **Lot No.:** A0216631
Description : o-Terphenyl Standard
o-Terphenyl Standard 10,000 µg/mL, Methylene Chloride, 1mL/ampul
Container Size : 2 mL **Pkg Amt:** > 1 mL
Expiration Date : April 30, 2028 **Storage:** 10°C or colder
Handling: Sonicate prior to use. **Ship:** Ambient

P13645 } Y.P.
↓
P13694 } 10/16/24

CERTIFIED VALUES

| Elution Order | Compound | CAS # | Lot # | Purity | Grav. Conc. (weight/volume) | Expanded Uncertainty * (95% C.L.; K=2) |
|---------------|-------------|---------|-------|--------|-----------------------------|--|
| 1 | o-Terphenyl | 84-15-1 | GKSSA | 99% | 10,065.0 µg/mL | +/- 453.3336 |

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Methylene chloride
CAS # 75-09-2
Purity 99%

Quality Confirmation Test

Column:

30m x 0.25mm x 0.25µm
Rtx-5 (cat.#10223)

Carrier Gas:

hydrogen-constant pressure 10 psi.

Temp. Program:

75°C (hold 1 min.) to 330°C
@ 20°C/min. (hold 10 min.)

Inj. Temp:

250°C

Det. Temp:

330°C

Det. Type:

FID

Split Vent:

10 ml/min.

Inj. Vol

1µl



This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Ven Kelley - Operations Tech I

Date Mixed: 17-Sep-2024

Balance Serial # 1128353505

Dillan Murphy - Operations Technician I

Date Passed: 23-Sep-2024

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/ μ ECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 31097 **Lot No.:** A0216631
Description : o-Terphenyl Standard
o-Terphenyl Standard 10,000 µg/mL, Methylene Chloride, 1mL/ampul
Container Size : 2 mL **Pkg Amt:** > 1 mL
Expiration Date : April 30, 2028 **Storage:** 10°C or colder
Handling: Sonicate prior to use. **Ship:** Ambient

P13645 } Y.P.
↓
P13694 } 10/16/24

CERTIFIED VALUES

| Elution Order | Compound | CAS # | Lot # | Purity | Grav. Conc. (weight/volume) | Expanded Uncertainty * (95% C.L.; K=2) |
|---------------|-------------|---------|-------|--------|-----------------------------|--|
| 1 | o-Terphenyl | 84-15-1 | GKSSA | 99% | 10,065.0 µg/mL | +/- 453.3336 |

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Methylene chloride
CAS # 75-09-2
Purity 99%

Quality Confirmation Test

Column:

30m x 0.25mm x 0.25µm
Rtx-5 (cat.#10223)

Carrier Gas:

hydrogen-constant pressure 10 psi.

Temp. Program:

75°C (hold 1 min.) to 330°C
@ 20°C/min. (hold 10 min.)

Inj. Temp:

250°C

Det. Temp:

330°C

Det. Type:

FID

Split Vent:

10 ml/min.

Inj. Vol

1µl



This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Ven Kelley - Operations Tech I

Date Mixed: 17-Sep-2024

Balance Serial # 1128353505

Dillan Murphy - Operations Technician I

Date Passed: 23-Sep-2024

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/ μ ECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 31097 **Lot No.:** A0216631
Description : o-Terphenyl Standard
o-Terphenyl Standard 10,000 µg/mL, Methylene Chloride, 1mL/ampul
Container Size : 2 mL **Pkg Amt:** > 1 mL
Expiration Date : April 30, 2028 **Storage:** 10°C or colder
Handling: Sonicate prior to use. **Ship:** Ambient

P13645 } Y.P.
↓
P13694 } 10/16/24

CERTIFIED VALUES

| Elution Order | Compound | CAS # | Lot # | Purity | Grav. Conc. (weight/volume) | Expanded Uncertainty * (95% C.L.; K=2) |
|---------------|-------------|---------|-------|--------|-----------------------------|--|
| 1 | o-Terphenyl | 84-15-1 | GKSSA | 99% | 10,065.0 µg/mL | +/- 453.3336 |

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Methylene chloride
CAS # 75-09-2
Purity 99%

Quality Confirmation Test

Column:

30m x 0.25mm x 0.25µm
Rtx-5 (cat.#10223)

Carrier Gas:

hydrogen-constant pressure 10 psi.

Temp. Program:

75°C (hold 1 min.) to 330°C
@ 20°C/min. (hold 10 min.)

Inj. Temp:

250°C

Det. Temp:

330°C

Det. Type:

FID

Split Vent:

10 ml/min.

Inj. Vol

1µl



This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Ven Kelley - Operations Tech I

Date Mixed: 17-Sep-2024

Balance Serial # 1128353505

Dillan Murphy - Operations Technician I

Date Passed: 23-Sep-2024

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 30543 **Lot No.:** A0225381

Description : NJEPH Aromatics Matrix Spike Mix

NJEPH Aromatics Matrix Spike Mix 200µg/mL, Acetone/Toluene (50:50), 5mL/ampul

Container Size : 5 mL **Pkg Amt:** > 5 mL

Expiration Date : April 30, 2031 **Storage:** 10°C or colder

Handling: Sonication required. Mix is photosensitive. **Ship:** Ambient

P13998
↓
P14017

} RC/
5/21/25

CERTIFIED VALUES

| Elution Order | Compound | CAS # | Lot # | Purity | Grav. Conc. (weight/volume) | Expanded Uncertainty * (95% C.L.; K=2) |
|---------------|------------------------|----------|--------------|--------|-----------------------------|--|
| 1 | 1,2,3-Trimethylbenzene | 526-73-8 | 8776.10-39 | 98% | 200.3 µg/mL | +/- 9.0255 |
| 2 | Naphthalene | 91-20-3 | STBL1057 | 99% | 200.4 µg/mL | +/- 9.0294 |
| 3 | 2-Methylnaphthalene | 91-57-6 | STBL3028 | 99% | 200.4 µg/mL | +/- 9.0294 |
| 4 | Acenaphthylene | 208-96-8 | 214935V16F | 97% | 200.2 µg/mL | +/- 9.0208 |
| 5 | Acenaphthene | 83-32-9 | MKCV8166 | 99% | 200.0 µg/mL | +/- 9.0114 |
| 6 | Fluorene | 86-73-7 | 10246250 | 98% | 200.3 µg/mL | +/- 9.0255 |
| 7 | Phenanthrene | 85-01-8 | MKCV8193 | 99% | 200.8 µg/mL | +/- 9.0474 |
| 8 | Anthracene | 120-12-7 | 101492T18R | 99% | 200.4 µg/mL | +/- 9.0294 |
| 9 | Fluoranthene | 206-44-0 | A0458721 | 99% | 200.4 µg/mL | +/- 9.0294 |
| 10 | Pyrene | 129-00-0 | BCCK2592 | 99% | 200.8 µg/mL | +/- 9.0474 |
| 11 | Benz(a)anthracene | 56-55-3 | I70012022BAA | 99% | 200.4 µg/mL | +/- 9.0294 |
| 12 | Chrysene | 218-01-9 | RP250121RSR | 99% | 200.0 µg/mL | +/- 9.0114 |
| 13 | Benzo(b)fluoranthene | 205-99-2 | 022013B | 99% | 200.4 µg/mL | +/- 9.0294 |
| 14 | Benzo(k)fluoranthene | 207-08-9 | 012022K | 99% | 200.4 µg/mL | +/- 9.0294 |
| 15 | Benzo(a)pyrene | 50-32-8 | NQLXA | 98% | 200.7 µg/mL | +/- 9.0431 |
| 16 | Indeno(1,2,3-cd)pyrene | 193-39-5 | 12-JKL-118-9 | 97% | 200.6 µg/mL | +/- 9.0383 |


| | | | | | | |
|----|-----------------------|----------|---------------|-----|-------------|------------|
| 17 | Dibenz(a,h)anthracene | 53-70-3 | 712061504-1-1 | 99% | 200.4 µg/mL | +/- 9.0294 |
| 18 | Benzo(g,h,i)perylene | 191-24-2 | RP250219RSR | 99% | 200.0 µg/mL | +/- 9.0114 |

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Acetone/Toluene (50:50)
CAS # 67-64-1/108-88-3
Purity 99%

Quality Confirmation Test

Column:
30m x 0.25mm x 0.25µm
Rtx-5 (cat.#10223)
Carrier Gas:
hydrogen-constant pressure 10 psi.
Temp. Program:
100°C (hold 1 min.) to 330°C
@ 4°C/min. (hold 5 min.)
Inj. Temp:
250°C
Det. Temp:
330°C
Det. Type:
FID
Split Vent:
20 ml/min.
Inj. Vol
1µl

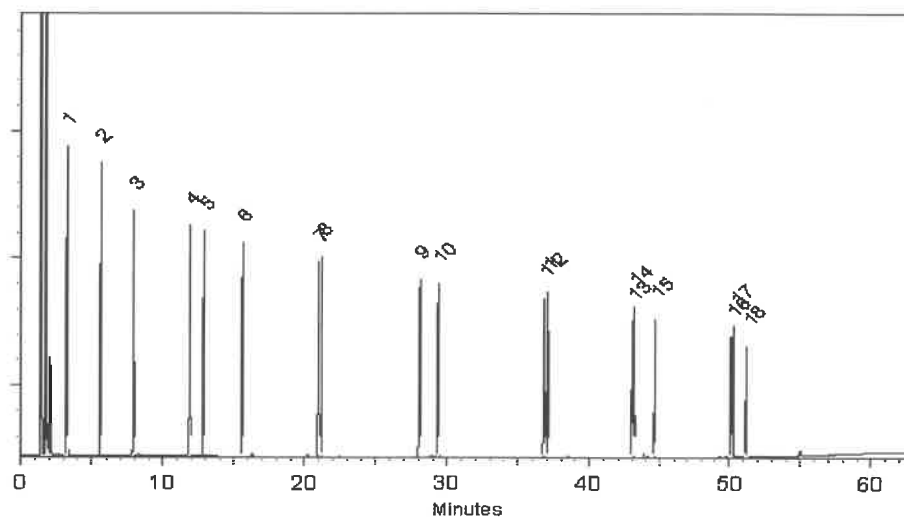

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Richard Zimmerman
Richard Zimmerman - Operations Tech I

Date Mixed: 06-May-2025 **Balance Serial #** 1128353505

Brittany Federinko
Brittany Federinko - Operations Tech II

Date Passed: 09-May-2025

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 30543 **Lot No.:** A0225381

Description : NJEPH Aromatics Matrix Spike Mix

NJEPH Aromatics Matrix Spike Mix 200µg/mL, Acetone/Toluene (50:50), 5mL/ampul

Container Size : 5 mL **Pkg Amt:** > 5 mL

Expiration Date : April 30, 2031 **Storage:** 10°C or colder

Handling: Sonication required. Mix is photosensitive. **Ship:** Ambient

P13998
↓
P14017

} Rc/
5/21/25

CERTIFIED VALUES

| Elution Order | Compound | CAS # | Lot # | Purity | Grav. Conc. (weight/volume) | Expanded Uncertainty * (95% C.L.; K=2) |
|---------------|------------------------|----------|--------------|--------|-----------------------------|--|
| 1 | 1,2,3-Trimethylbenzene | 526-73-8 | 8776.10-39 | 98% | 200.3 µg/mL | +/- 9.0255 |
| 2 | Naphthalene | 91-20-3 | STBL1057 | 99% | 200.4 µg/mL | +/- 9.0294 |
| 3 | 2-Methylnaphthalene | 91-57-6 | STBL3028 | 99% | 200.4 µg/mL | +/- 9.0294 |
| 4 | Acenaphthylene | 208-96-8 | 214935V16F | 97% | 200.2 µg/mL | +/- 9.0208 |
| 5 | Acenaphthene | 83-32-9 | MKCV8166 | 99% | 200.0 µg/mL | +/- 9.0114 |
| 6 | Fluorene | 86-73-7 | 10246250 | 98% | 200.3 µg/mL | +/- 9.0255 |
| 7 | Phenanthrene | 85-01-8 | MKCV8193 | 99% | 200.8 µg/mL | +/- 9.0474 |
| 8 | Anthracene | 120-12-7 | 101492T18R | 99% | 200.4 µg/mL | +/- 9.0294 |
| 9 | Fluoranthene | 206-44-0 | A0458721 | 99% | 200.4 µg/mL | +/- 9.0294 |
| 10 | Pyrene | 129-00-0 | BCCK2592 | 99% | 200.8 µg/mL | +/- 9.0474 |
| 11 | Benz(a)anthracene | 56-55-3 | I70012022BAA | 99% | 200.4 µg/mL | +/- 9.0294 |
| 12 | Chrysene | 218-01-9 | RP250121RSR | 99% | 200.0 µg/mL | +/- 9.0114 |
| 13 | Benzo(b)fluoranthene | 205-99-2 | 022013B | 99% | 200.4 µg/mL | +/- 9.0294 |
| 14 | Benzo(k)fluoranthene | 207-08-9 | 012022K | 99% | 200.4 µg/mL | +/- 9.0294 |
| 15 | Benzo(a)pyrene | 50-32-8 | NQLXA | 98% | 200.7 µg/mL | +/- 9.0431 |
| 16 | Indeno(1,2,3-cd)pyrene | 193-39-5 | 12-JKL-118-9 | 97% | 200.6 µg/mL | +/- 9.0383 |

| | | | | | | |
|----|-----------------------|----------|---------------|-----|-------------|------------|
| 17 | Dibenz(a,h)anthracene | 53-70-3 | 712061504-1-1 | 99% | 200.4 µg/mL | +/- 9.0294 |
| 18 | Benzo(g,h,i)perylene | 191-24-2 | RP250219RSR | 99% | 200.0 µg/mL | +/- 9.0114 |

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Acetone/Toluene (50:50)
CAS # 67-64-1/108-88-3
Purity 99%

Quality Confirmation Test

Column:
30m x 0.25mm x 0.25µm
Rtx-5 (cat.#10223)

Carrier Gas:
hydrogen-constant pressure 10 psi.

Temp. Program:
100°C (hold 1 min.) to 330°C
@ 4°C/min. (hold 5 min.)


Inj. Temp:
250°C

Det. Temp:
330°C

Det. Type:
FID

Split Vent:
20 ml/min.

Inj. Vol
1µl

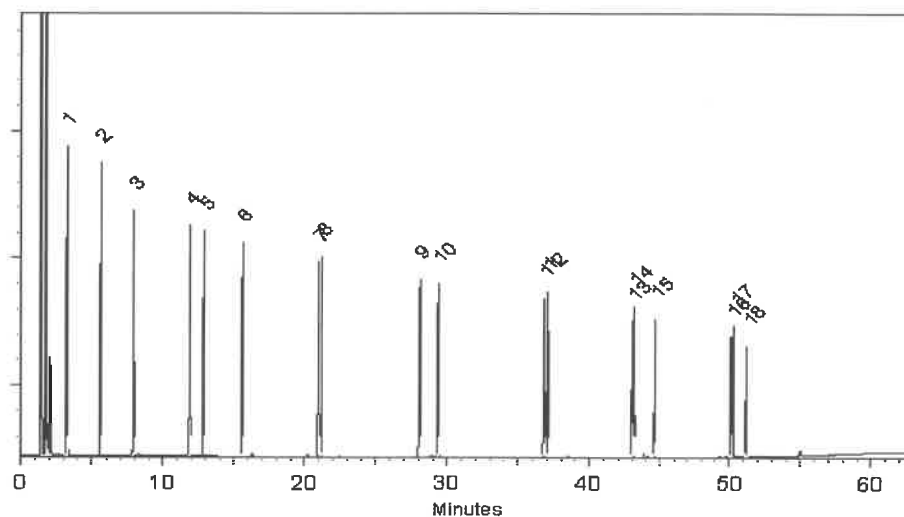

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.


Richard Zimmerman - Operations Tech I

Date Mixed: 06-May-2025 **Balance Serial #** 1128353505


Brittany Federinko - Operations Tech II

Date Passed: 09-May-2025

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 30543 **Lot No.:** A0225381

Description : NJEPH Aromatics Matrix Spike Mix

NJEPH Aromatics Matrix Spike Mix 200µg/mL, Acetone/Toluene (50:50), 5mL/ampul

Container Size : 5 mL **Pkg Amt:** > 5 mL

Expiration Date : April 30, 2031 **Storage:** 10°C or colder

Handling: Sonication required. Mix is photosensitive. **Ship:** Ambient

P13998
↓
P14017

} Rc/
5/21/25

CERTIFIED VALUES

| Elution Order | Compound | CAS # | Lot # | Purity | Grav. Conc. (weight/volume) | Expanded Uncertainty * (95% C.L.; K=2) |
|---------------|------------------------|----------|--------------|--------|-----------------------------|--|
| 1 | 1,2,3-Trimethylbenzene | 526-73-8 | 8776.10-39 | 98% | 200.3 µg/mL | +/- 9.0255 |
| 2 | Naphthalene | 91-20-3 | STBL1057 | 99% | 200.4 µg/mL | +/- 9.0294 |
| 3 | 2-Methylnaphthalene | 91-57-6 | STBL3028 | 99% | 200.4 µg/mL | +/- 9.0294 |
| 4 | Acenaphthylene | 208-96-8 | 214935V16F | 97% | 200.2 µg/mL | +/- 9.0208 |
| 5 | Acenaphthene | 83-32-9 | MKCV8166 | 99% | 200.0 µg/mL | +/- 9.0114 |
| 6 | Fluorene | 86-73-7 | 10246250 | 98% | 200.3 µg/mL | +/- 9.0255 |
| 7 | Phenanthrene | 85-01-8 | MKCV8193 | 99% | 200.8 µg/mL | +/- 9.0474 |
| 8 | Anthracene | 120-12-7 | 101492T18R | 99% | 200.4 µg/mL | +/- 9.0294 |
| 9 | Fluoranthene | 206-44-0 | A0458721 | 99% | 200.4 µg/mL | +/- 9.0294 |
| 10 | Pyrene | 129-00-0 | BCCK2592 | 99% | 200.8 µg/mL | +/- 9.0474 |
| 11 | Benz(a)anthracene | 56-55-3 | I70012022BAA | 99% | 200.4 µg/mL | +/- 9.0294 |
| 12 | Chrysene | 218-01-9 | RP250121RSR | 99% | 200.0 µg/mL | +/- 9.0114 |
| 13 | Benzo(b)fluoranthene | 205-99-2 | 022013B | 99% | 200.4 µg/mL | +/- 9.0294 |
| 14 | Benzo(k)fluoranthene | 207-08-9 | 012022K | 99% | 200.4 µg/mL | +/- 9.0294 |
| 15 | Benzo(a)pyrene | 50-32-8 | NQLXA | 98% | 200.7 µg/mL | +/- 9.0431 |
| 16 | Indeno(1,2,3-cd)pyrene | 193-39-5 | 12-JKL-118-9 | 97% | 200.6 µg/mL | +/- 9.0383 |


| | | | | | | |
|----|-----------------------|----------|---------------|-----|-------------|------------|
| 17 | Dibenz(a,h)anthracene | 53-70-3 | 712061504-1-1 | 99% | 200.4 µg/mL | +/- 9.0294 |
| 18 | Benzo(g,h,i)perylene | 191-24-2 | RP250219RSR | 99% | 200.0 µg/mL | +/- 9.0114 |

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Acetone/Toluene (50:50)
CAS # 67-64-1/108-88-3
Purity 99%

Quality Confirmation Test

Column:
30m x 0.25mm x 0.25µm
Rtx-5 (cat.#10223)
Carrier Gas:
hydrogen-constant pressure 10 psi.
Temp. Program:
100°C (hold 1 min.) to 330°C
@ 4°C/min. (hold 5 min.)
Inj. Temp:
250°C
Det. Temp:
330°C
Det. Type:
FID
Split Vent:
20 ml/min.
Inj. Vol
1µl

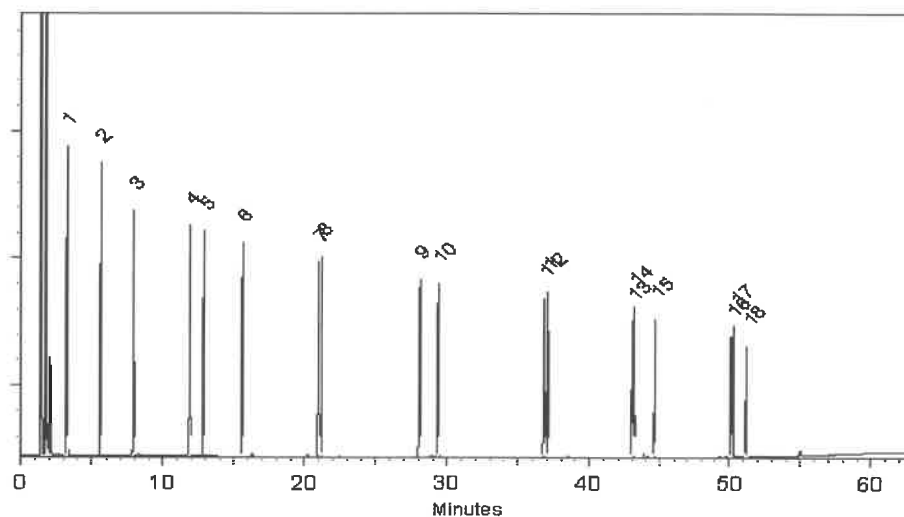

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Richard Zimmerman
Richard Zimmerman - Operations Tech I

Date Mixed: 06-May-2025 **Balance Serial #** 1128353505

Brittany Federinko
Brittany Federinko - Operations Tech II

Date Passed: 09-May-2025

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 30543 **Lot No.:** A0225381

Description : NJEPH Aromatics Matrix Spike Mix

NJEPH Aromatics Matrix Spike Mix 200µg/mL, Acetone/Toluene (50:50), 5mL/ampul

Container Size : 5 mL **Pkg Amt:** > 5 mL

Expiration Date : April 30, 2031 **Storage:** 10°C or colder

Handling: Sonication required. Mix is photosensitive. **Ship:** Ambient

P13998
↓
P14017

} RC/
5/21/25

CERTIFIED VALUES

| Elution Order | Compound | CAS # | Lot # | Purity | Grav. Conc. (weight/volume) | Expanded Uncertainty * (95% C.L.; K=2) |
|---------------|------------------------|----------|--------------|--------|-----------------------------|--|
| 1 | 1,2,3-Trimethylbenzene | 526-73-8 | 8776.10-39 | 98% | 200.3 µg/mL | +/- 9.0255 |
| 2 | Naphthalene | 91-20-3 | STBL1057 | 99% | 200.4 µg/mL | +/- 9.0294 |
| 3 | 2-Methylnaphthalene | 91-57-6 | STBL3028 | 99% | 200.4 µg/mL | +/- 9.0294 |
| 4 | Acenaphthylene | 208-96-8 | 214935V16F | 97% | 200.2 µg/mL | +/- 9.0208 |
| 5 | Acenaphthene | 83-32-9 | MKCV8166 | 99% | 200.0 µg/mL | +/- 9.0114 |
| 6 | Fluorene | 86-73-7 | 10246250 | 98% | 200.3 µg/mL | +/- 9.0255 |
| 7 | Phenanthrene | 85-01-8 | MKCV8193 | 99% | 200.8 µg/mL | +/- 9.0474 |
| 8 | Anthracene | 120-12-7 | 101492T18R | 99% | 200.4 µg/mL | +/- 9.0294 |
| 9 | Fluoranthene | 206-44-0 | A0458721 | 99% | 200.4 µg/mL | +/- 9.0294 |
| 10 | Pyrene | 129-00-0 | BCCK2592 | 99% | 200.8 µg/mL | +/- 9.0474 |
| 11 | Benz(a)anthracene | 56-55-3 | I70012022BAA | 99% | 200.4 µg/mL | +/- 9.0294 |
| 12 | Chrysene | 218-01-9 | RP250121RSR | 99% | 200.0 µg/mL | +/- 9.0114 |
| 13 | Benzo(b)fluoranthene | 205-99-2 | 022013B | 99% | 200.4 µg/mL | +/- 9.0294 |
| 14 | Benzo(k)fluoranthene | 207-08-9 | 012022K | 99% | 200.4 µg/mL | +/- 9.0294 |
| 15 | Benzo(a)pyrene | 50-32-8 | NQLXA | 98% | 200.7 µg/mL | +/- 9.0431 |
| 16 | Indeno(1,2,3-cd)pyrene | 193-39-5 | 12-JKL-118-9 | 97% | 200.6 µg/mL | +/- 9.0383 |


| | | | | | | |
|----|-----------------------|----------|---------------|-----|-------------|------------|
| 17 | Dibenz(a,h)anthracene | 53-70-3 | 712061504-1-1 | 99% | 200.4 µg/mL | +/- 9.0294 |
| 18 | Benzo(g,h,i)perylene | 191-24-2 | RP250219RSR | 99% | 200.0 µg/mL | +/- 9.0114 |

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Acetone/Toluene (50:50)
CAS # 67-64-1/108-88-3
Purity 99%

Quality Confirmation Test

Column:
30m x 0.25mm x 0.25µm
Rtx-5 (cat.#10223)
Carrier Gas:
hydrogen-constant pressure 10 psi.
Temp. Program:
100°C (hold 1 min.) to 330°C
@ 4°C/min. (hold 5 min.)
Inj. Temp:
250°C
Det. Temp:
330°C
Det. Type:
FID
Split Vent:
20 ml/min.
Inj. Vol
1µl

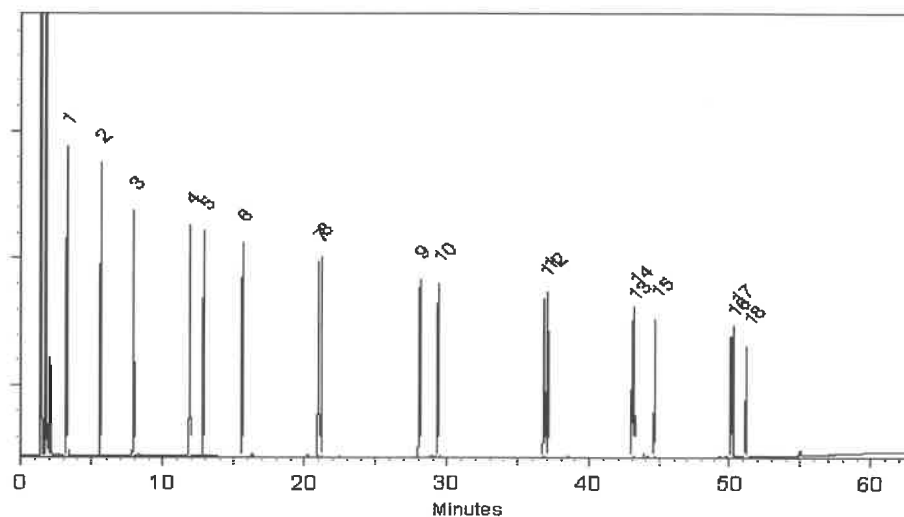

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.


Richard Zimmerman - Operations Tech I

Date Mixed: 06-May-2025 **Balance Serial #** 1128353505


Brittany Federinko - Operations Tech II

Date Passed: 09-May-2025

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 30543 **Lot No.:** A0225381

Description : NJEPH Aromatics Matrix Spike Mix

NJEPH Aromatics Matrix Spike Mix 200µg/mL, Acetone/Toluene (50:50), 5mL/ampul

Container Size : 5 mL **Pkg Amt:** > 5 mL

Expiration Date : April 30, 2031 **Storage:** 10°C or colder

Handling: Sonication required. Mix is photosensitive. **Ship:** Ambient

P13998
↓
P14017

} RC/
5/21/25

CERTIFIED VALUES

| Elution Order | Compound | CAS # | Lot # | Purity | Grav. Conc. (weight/volume) | Expanded Uncertainty * (95% C.L.; K=2) |
|---------------|------------------------|----------|--------------|--------|-----------------------------|--|
| 1 | 1,2,3-Trimethylbenzene | 526-73-8 | 8776.10-39 | 98% | 200.3 µg/mL | +/- 9.0255 |
| 2 | Naphthalene | 91-20-3 | STBL1057 | 99% | 200.4 µg/mL | +/- 9.0294 |
| 3 | 2-Methylnaphthalene | 91-57-6 | STBL3028 | 99% | 200.4 µg/mL | +/- 9.0294 |
| 4 | Acenaphthylene | 208-96-8 | 214935V16F | 97% | 200.2 µg/mL | +/- 9.0208 |
| 5 | Acenaphthene | 83-32-9 | MKCV8166 | 99% | 200.0 µg/mL | +/- 9.0114 |
| 6 | Fluorene | 86-73-7 | 10246250 | 98% | 200.3 µg/mL | +/- 9.0255 |
| 7 | Phenanthrene | 85-01-8 | MKCV8193 | 99% | 200.8 µg/mL | +/- 9.0474 |
| 8 | Anthracene | 120-12-7 | 101492T18R | 99% | 200.4 µg/mL | +/- 9.0294 |
| 9 | Fluoranthene | 206-44-0 | A0458721 | 99% | 200.4 µg/mL | +/- 9.0294 |
| 10 | Pyrene | 129-00-0 | BCCK2592 | 99% | 200.8 µg/mL | +/- 9.0474 |
| 11 | Benz(a)anthracene | 56-55-3 | I70012022BAA | 99% | 200.4 µg/mL | +/- 9.0294 |
| 12 | Chrysene | 218-01-9 | RP250121RSR | 99% | 200.0 µg/mL | +/- 9.0114 |
| 13 | Benzo(b)fluoranthene | 205-99-2 | 022013B | 99% | 200.4 µg/mL | +/- 9.0294 |
| 14 | Benzo(k)fluoranthene | 207-08-9 | 012022K | 99% | 200.4 µg/mL | +/- 9.0294 |
| 15 | Benzo(a)pyrene | 50-32-8 | NQLXA | 98% | 200.7 µg/mL | +/- 9.0431 |
| 16 | Indeno(1,2,3-cd)pyrene | 193-39-5 | 12-JKL-118-9 | 97% | 200.6 µg/mL | +/- 9.0383 |

| | | | | | | |
|----|-----------------------|----------|---------------|-----|-------------|------------|
| 17 | Dibenz(a,h)anthracene | 53-70-3 | 712061504-1-1 | 99% | 200.4 µg/mL | +/- 9.0294 |
| 18 | Benzo(g,h,i)perylene | 191-24-2 | RP250219RSR | 99% | 200.0 µg/mL | +/- 9.0114 |

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Acetone/Toluene (50:50)
CAS # 67-64-1/108-88-3
Purity 99%

Quality Confirmation Test

Column:
30m x 0.25mm x 0.25µm
Rtx-5 (cat.#10223)

Carrier Gas:
hydrogen-constant pressure 10 psi.

Temp. Program:
100°C (hold 1 min.) to 330°C
@ 4°C/min. (hold 5 min.)


Inj. Temp:
250°C

Det. Temp:
330°C

Det. Type:
FID

Split Vent:
20 ml/min.

Inj. Vol
1µl

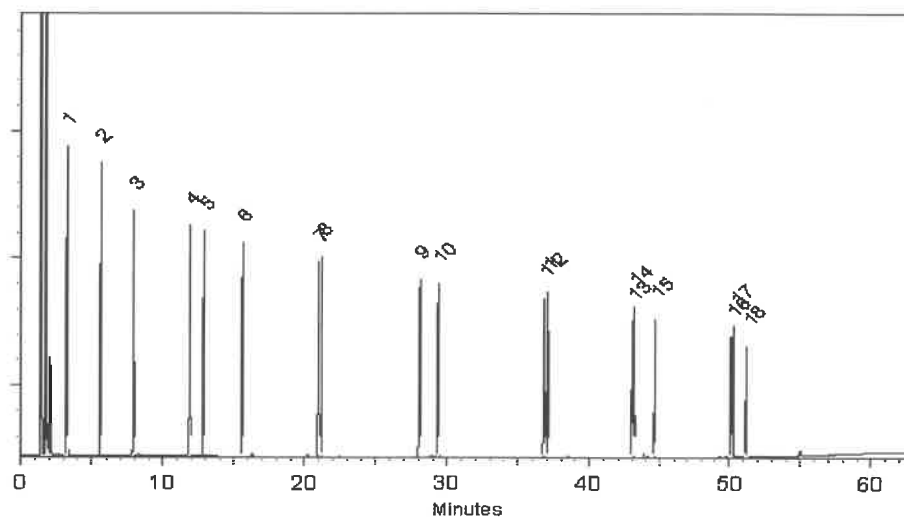

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.


Richard Zimmerman - Operations Tech I

Date Mixed: 06-May-2025 **Balance Serial #** 1128353505


Brittany Federinko - Operations Tech II

Date Passed: 09-May-2025

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 30542 **Lot No.:** A0220449

Description : NJEPH Aliphatics Matrix Spike Mix
NJEPH Aliphatics Matrix Spike Mix 200 µg/mL, n-Pentane, 5mL/ampul

Container Size : 5 mL **Pkg Amt:** > 5 mL

Expiration Date : January 31, 2032 **Storage:** 10°C or colder

Handling: Sonicate prior to use. **Ship:** Ambient

P14018 } RC/
↓
P14027 } 5/21/25.

CERTIFIED VALUES

| Elution Order | Compound | CAS # | Lot # | Purity | Grav. Conc. (weight/volume) | Expanded Uncertainty * (95% C.L.; K=2) |
|---------------|--------------------------|------------|------------|--------|-----------------------------|--|
| 1 | n-Nonane (C9) | 111-84-2 | SHBP9752 | 99% | 201.3 µg/mL | +/- 5.2012 |
| 2 | n-Decane (C10) | 124-18-5 | SHBQ1342 | 99% | 201.7 µg/mL | +/- 5.2098 |
| 3 | n-Dodecane (C12) | 112-40-3 | SHBP7054 | 99% | 201.3 µg/mL | +/- 5.2012 |
| 4 | n-Tetradecane (C14) | 629-59-4 | STBL0465 | 99% | 200.7 µg/mL | +/- 5.1839 |
| 5 | n-Hexadecane (C16) | 544-76-3 | SHBR0669 | 99% | 200.3 µg/mL | +/- 5.1753 |
| 6 | n-Octadecane (C18) | 593-45-3 | UE5NG | 99% | 200.7 µg/mL | +/- 5.1839 |
| 7 | n-Eicosane (C20) | 112-95-8 | MKCN8767 | 97% | 200.1 µg/mL | +/- 5.1704 |
| 8 | n-Heneicosane (C21) | 629-94-7 | MKCP1960 | 99% | 200.7 µg/mL | +/- 5.1839 |
| 9 | n-Docosane (C22) | 629-97-0 | MKCQ3882 | 99% | 200.3 µg/mL | +/- 5.1753 |
| 10 | n-Tetracosane (C24) | 646-31-1 | UH5GN | 99% | 201.3 µg/mL | +/- 5.2012 |
| 11 | n-Hexacosane (C26) | 630-01-3 | MKCQ4814 | 99% | 201.0 µg/mL | +/- 5.1926 |
| 12 | n-Octacosane (C28) | 630-02-4 | BCCJ4566 | 99% | 200.3 µg/mL | +/- 5.1753 |
| 13 | n-Triacontane (C30) | 638-68-6 | MKCV7007 | 98% | 201.2 µg/mL | +/- 5.1984 |
| 14 | n-Dotriacontane (C32) | 544-85-4 | BCBW0661 | 99% | 201.7 µg/mL | +/- 5.2098 |
| 15 | n-Tetratriacontane (C34) | 14167-59-0 | 6JNHB | 99% | 201.3 µg/mL | +/- 5.2012 |
| 16 | n-Hexatriacontane (C36) | 630-06-8 | Z27H018 | 99% | 201.7 µg/mL | +/- 5.2098 |
| 17 | n-Octatriacontane (C38) | 7194-85-6 | 0000207852 | 96% | 201.6 µg/mL | +/- 5.2081 |

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: n-Pentane
CAS # 109-66-0
Purity 99%

Quality Confirmation Test

Column:
30m x 0.25mm x 0.25µm
Rtx-5 (cat.#10223)
Carrier Gas:
hydrogen-constant pressure 10 psi.

Temp. Program:
40°C (hold 2 min.) to 330°C
@ 10°C/min. (hold 10 min.)


Inj. Temp:
250°C

Det. Temp:
330°C

Det. Type:
FID

Split Vent:
2 ml/min.

Inj. Vol
1µl

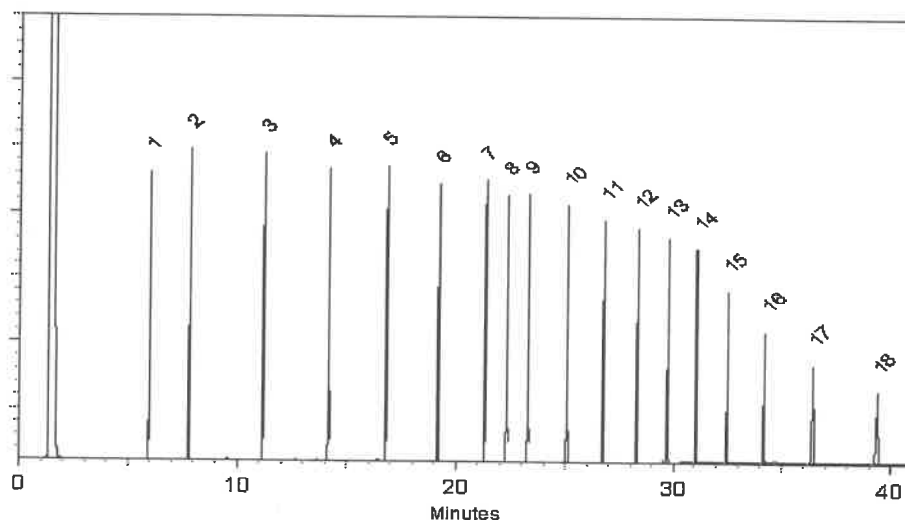

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Brandon Reish
Brandon Reish - Operations Technician III

Date Mixed: 23-Dec-2024

Balance Serial # C322230531

Dylan Murphy
Dylan Murphy - Operations Technician I

Date Passed: 27-Dec-2024

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 30542 **Lot No.:** A0220449

Description : NJEPH Aliphatics Matrix Spike Mix
NJEPH Aliphatics Matrix Spike Mix 200 µg/mL, n-Pentane, 5mL/ampul

Container Size : 5 mL **Pkg Amt:** > 5 mL

Expiration Date : January 31, 2032 **Storage:** 10°C or colder

Handling: Sonicate prior to use. **Ship:** Ambient

P14018 } RC/
↓
P14027 } 5/21/25.

CERTIFIED VALUES

| Elution Order | Compound | CAS # | Lot # | Purity | Grav. Conc. (weight/volume) | Expanded Uncertainty * (95% C.L.; K=2) |
|---------------|--------------------------|------------|------------|--------|-----------------------------|--|
| 1 | n-Nonane (C9) | 111-84-2 | SHBP9752 | 99% | 201.3 µg/mL | +/- 5.2012 |
| 2 | n-Decane (C10) | 124-18-5 | SHBQ1342 | 99% | 201.7 µg/mL | +/- 5.2098 |
| 3 | n-Dodecane (C12) | 112-40-3 | SHBP7054 | 99% | 201.3 µg/mL | +/- 5.2012 |
| 4 | n-Tetradecane (C14) | 629-59-4 | STBL0465 | 99% | 200.7 µg/mL | +/- 5.1839 |
| 5 | n-Hexadecane (C16) | 544-76-3 | SHBR0669 | 99% | 200.3 µg/mL | +/- 5.1753 |
| 6 | n-Octadecane (C18) | 593-45-3 | UE5NG | 99% | 200.7 µg/mL | +/- 5.1839 |
| 7 | n-Eicosane (C20) | 112-95-8 | MKCN8767 | 97% | 200.1 µg/mL | +/- 5.1704 |
| 8 | n-Heneicosane (C21) | 629-94-7 | MKCP1960 | 99% | 200.7 µg/mL | +/- 5.1839 |
| 9 | n-Docosane (C22) | 629-97-0 | MKCQ3882 | 99% | 200.3 µg/mL | +/- 5.1753 |
| 10 | n-Tetracosane (C24) | 646-31-1 | UH5GN | 99% | 201.3 µg/mL | +/- 5.2012 |
| 11 | n-Hexacosane (C26) | 630-01-3 | MKCQ4814 | 99% | 201.0 µg/mL | +/- 5.1926 |
| 12 | n-Octacosane (C28) | 630-02-4 | BCCJ4566 | 99% | 200.3 µg/mL | +/- 5.1753 |
| 13 | n-Triacontane (C30) | 638-68-6 | MKCV7007 | 98% | 201.2 µg/mL | +/- 5.1984 |
| 14 | n-Dotriacontane (C32) | 544-85-4 | BCBW0661 | 99% | 201.7 µg/mL | +/- 5.2098 |
| 15 | n-Tetratriacontane (C34) | 14167-59-0 | 6JNHB | 99% | 201.3 µg/mL | +/- 5.2012 |
| 16 | n-Hexatriacontane (C36) | 630-06-8 | Z27H018 | 99% | 201.7 µg/mL | +/- 5.2098 |
| 17 | n-Octatriacontane (C38) | 7194-85-6 | 0000207852 | 96% | 201.6 µg/mL | +/- 5.2081 |

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: n-Pentane
CAS # 109-66-0
Purity 99%

Quality Confirmation Test

Column:

30m x 0.25mm x 0.25µm
Rtx-5 (cat.#10223)

Carrier Gas:

hydrogen-constant pressure 10 psi.

Temp. Program:

40°C (hold 2 min.) to 330°C
@ 10°C/min. (hold 10 min.)

Inj. Temp:

250°C

Det. Temp:

330°C

Det. Type:


FID

Split Vent:

2 ml/min.

Inj. Vol

1µl

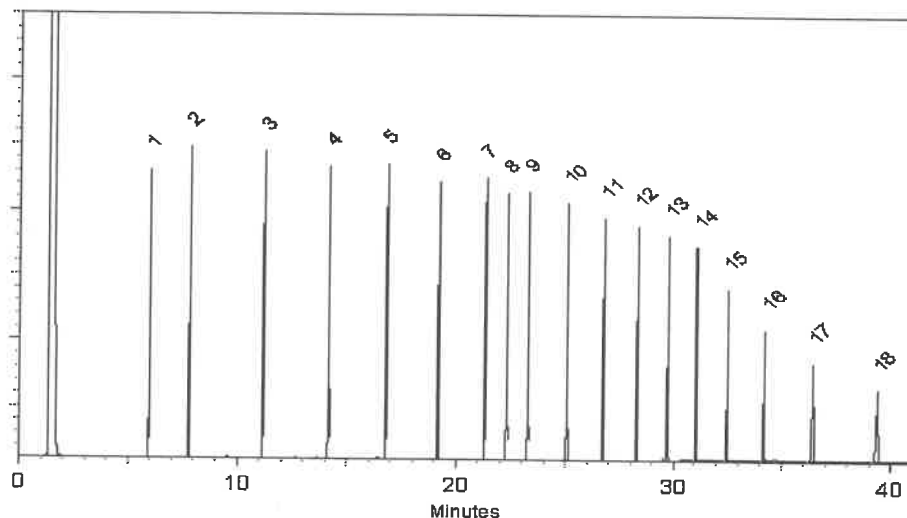

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Brandon Reish
Brandon Reish - Operations Technician III

Date Mixed: 23-Dec-2024

Balance Serial # C322230531

Dylan Murphy
Dylan Murphy - Operations Technician I

Date Passed: 27-Dec-2024

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 30542 **Lot No.:** A0220449

Description : NJEPH Aliphatics Matrix Spike Mix
NJEPH Aliphatics Matrix Spike Mix 200 µg/mL, n-Pentane, 5mL/ampul

Container Size : 5 mL **Pkg Amt:** > 5 mL

Expiration Date : January 31, 2032 **Storage:** 10°C or colder

Handling: Sonicate prior to use. **Ship:** Ambient

P14018 } RC/
↓
P14027 } 5/21/25.

CERTIFIED VALUES

| Elution Order | Compound | CAS # | Lot # | Purity | Grav. Conc. (weight/volume) | Expanded Uncertainty * (95% C.L.; K=2) |
|---------------|--------------------------|------------|------------|--------|-----------------------------|--|
| 1 | n-Nonane (C9) | 111-84-2 | SHBP9752 | 99% | 201.3 µg/mL | +/- 5.2012 |
| 2 | n-Decane (C10) | 124-18-5 | SHBQ1342 | 99% | 201.7 µg/mL | +/- 5.2098 |
| 3 | n-Dodecane (C12) | 112-40-3 | SHBP7054 | 99% | 201.3 µg/mL | +/- 5.2012 |
| 4 | n-Tetradecane (C14) | 629-59-4 | STBL0465 | 99% | 200.7 µg/mL | +/- 5.1839 |
| 5 | n-Hexadecane (C16) | 544-76-3 | SHBR0669 | 99% | 200.3 µg/mL | +/- 5.1753 |
| 6 | n-Octadecane (C18) | 593-45-3 | UE5NG | 99% | 200.7 µg/mL | +/- 5.1839 |
| 7 | n-Eicosane (C20) | 112-95-8 | MKCN8767 | 97% | 200.1 µg/mL | +/- 5.1704 |
| 8 | n-Heneicosane (C21) | 629-94-7 | MKCP1960 | 99% | 200.7 µg/mL | +/- 5.1839 |
| 9 | n-Docosane (C22) | 629-97-0 | MKCQ3882 | 99% | 200.3 µg/mL | +/- 5.1753 |
| 10 | n-Tetracosane (C24) | 646-31-1 | UH5GN | 99% | 201.3 µg/mL | +/- 5.2012 |
| 11 | n-Hexacosane (C26) | 630-01-3 | MKCQ4814 | 99% | 201.0 µg/mL | +/- 5.1926 |
| 12 | n-Octacosane (C28) | 630-02-4 | BCCJ4566 | 99% | 200.3 µg/mL | +/- 5.1753 |
| 13 | n-Triacontane (C30) | 638-68-6 | MKCV7007 | 98% | 201.2 µg/mL | +/- 5.1984 |
| 14 | n-Dotriacontane (C32) | 544-85-4 | BCBW0661 | 99% | 201.7 µg/mL | +/- 5.2098 |
| 15 | n-Tetratriacontane (C34) | 14167-59-0 | 6JNHB | 99% | 201.3 µg/mL | +/- 5.2012 |
| 16 | n-Hexatriacontane (C36) | 630-06-8 | Z27H018 | 99% | 201.7 µg/mL | +/- 5.2098 |
| 17 | n-Octatriacontane (C38) | 7194-85-6 | 0000207852 | 96% | 201.6 µg/mL | +/- 5.2081 |

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: n-Pentane
CAS # 109-66-0
Purity 99%

Quality Confirmation Test

Column:

30m x 0.25mm x 0.25µm
Rtx-5 (cat.#10223)

Carrier Gas:

hydrogen-constant pressure 10 psi.

Temp. Program:

40°C (hold 2 min.) to 330°C
@ 10°C/min. (hold 10 min.)

Inj. Temp:

250°C

Det. Temp:

330°C

Det. Type:


FID

Split Vent:

2 ml/min.

Inj. Vol

1µl

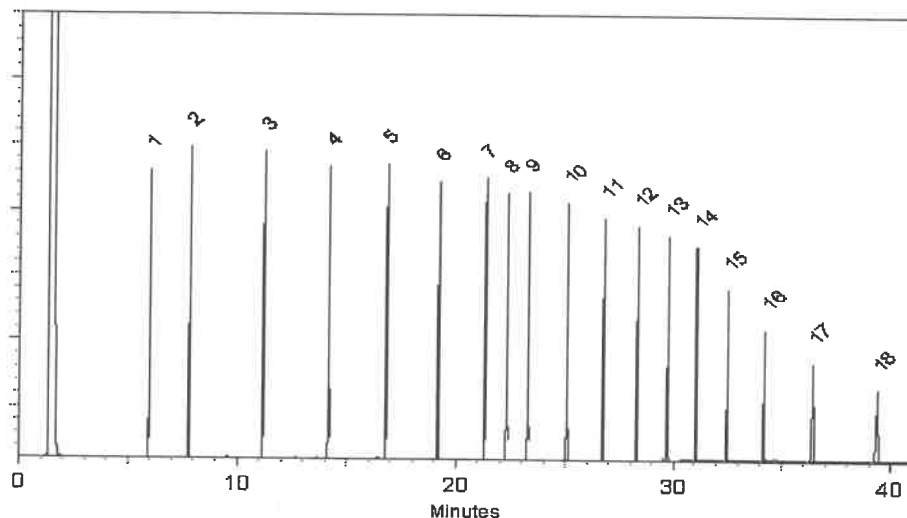

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Brandon Reish
Brandon Reish - Operations Technician III

Date Mixed: 23-Dec-2024

Balance Serial # C322230531

Dylan Murphy
Dylan Murphy - Operations Technician I

Date Passed: 27-Dec-2024

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 30542 **Lot No.:** A0220449

Description : NJEPH Aliphatics Matrix Spike Mix
NJEPH Aliphatics Matrix Spike Mix 200 µg/mL, n-Pentane, 5mL/ampul

Container Size : 5 mL **Pkg Amt:** > 5 mL

Expiration Date : January 31, 2032 **Storage:** 10°C or colder

Handling: Sonicate prior to use. **Ship:** Ambient

P14018 } RC/
↓
P14027 } 5/21/25.

CERTIFIED VALUES

| Elution Order | Compound | CAS # | Lot # | Purity | Grav. Conc. (weight/volume) | Expanded Uncertainty * (95% C.L.; K=2) |
|---------------|--------------------------|------------|------------|--------|-----------------------------|--|
| 1 | n-Nonane (C9) | 111-84-2 | SHBP9752 | 99% | 201.3 µg/mL | +/- 5.2012 |
| 2 | n-Decane (C10) | 124-18-5 | SHBQ1342 | 99% | 201.7 µg/mL | +/- 5.2098 |
| 3 | n-Dodecane (C12) | 112-40-3 | SHBP7054 | 99% | 201.3 µg/mL | +/- 5.2012 |
| 4 | n-Tetradecane (C14) | 629-59-4 | STBL0465 | 99% | 200.7 µg/mL | +/- 5.1839 |
| 5 | n-Hexadecane (C16) | 544-76-3 | SHBR0669 | 99% | 200.3 µg/mL | +/- 5.1753 |
| 6 | n-Octadecane (C18) | 593-45-3 | UE5NG | 99% | 200.7 µg/mL | +/- 5.1839 |
| 7 | n-Eicosane (C20) | 112-95-8 | MKCN8767 | 97% | 200.1 µg/mL | +/- 5.1704 |
| 8 | n-Heneicosane (C21) | 629-94-7 | MKCP1960 | 99% | 200.7 µg/mL | +/- 5.1839 |
| 9 | n-Docosane (C22) | 629-97-0 | MKCQ3882 | 99% | 200.3 µg/mL | +/- 5.1753 |
| 10 | n-Tetracosane (C24) | 646-31-1 | UH5GN | 99% | 201.3 µg/mL | +/- 5.2012 |
| 11 | n-Hexacosane (C26) | 630-01-3 | MKCQ4814 | 99% | 201.0 µg/mL | +/- 5.1926 |
| 12 | n-Octacosane (C28) | 630-02-4 | BCCJ4566 | 99% | 200.3 µg/mL | +/- 5.1753 |
| 13 | n-Triacontane (C30) | 638-68-6 | MKCV7007 | 98% | 201.2 µg/mL | +/- 5.1984 |
| 14 | n-Dotriacontane (C32) | 544-85-4 | BCBW0661 | 99% | 201.7 µg/mL | +/- 5.2098 |
| 15 | n-Tetratriacontane (C34) | 14167-59-0 | 6JNHB | 99% | 201.3 µg/mL | +/- 5.2012 |
| 16 | n-Hexatriacontane (C36) | 630-06-8 | Z27H018 | 99% | 201.7 µg/mL | +/- 5.2098 |
| 17 | n-Octatriacontane (C38) | 7194-85-6 | 0000207852 | 96% | 201.6 µg/mL | +/- 5.2081 |

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: n-Pentane
CAS # 109-66-0
Purity 99%

Quality Confirmation Test

Column:

30m x 0.25mm x 0.25µm
Rtx-5 (cat.#10223)

Carrier Gas:

hydrogen-constant pressure 10 psi.

Temp. Program:

40°C (hold 2 min.) to 330°C
@ 10°C/min. (hold 10 min.)

Inj. Temp:

250°C

Det. Temp:

330°C

Det. Type:


FID

Split Vent:

2 ml/min.

Inj. Vol

1µl

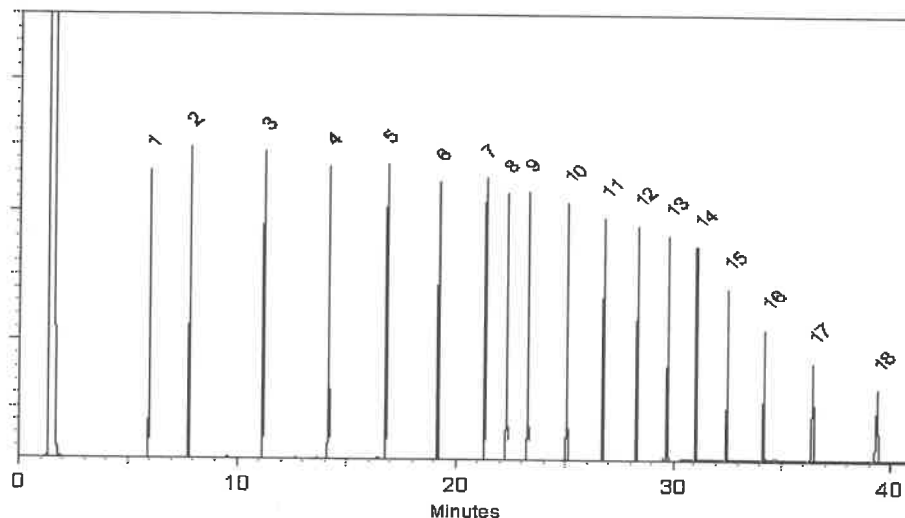

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Brandon Reish
Brandon Reish - Operations Technician III

Date Mixed: 23-Dec-2024

Balance Serial # C322230531

Dylan Murphy
Dylan Murphy - Operations Technician I

Date Passed: 27-Dec-2024

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 30542 **Lot No.:** A0220449

Description : NJEPH Aliphatics Matrix Spike Mix
NJEPH Aliphatics Matrix Spike Mix 200 µg/mL, n-Pentane, 5mL/ampul

Container Size : 5 mL **Pkg Amt:** > 5 mL

Expiration Date : January 31, 2032 **Storage:** 10°C or colder

Handling: Sonicate prior to use. **Ship:** Ambient

P14018 } RC/
↓
P14027 } 5/21/25.

CERTIFIED VALUES

| Elution Order | Compound | CAS # | Lot # | Purity | Grav. Conc. (weight/volume) | Expanded Uncertainty * (95% C.L.; K=2) |
|---------------|--------------------------|------------|------------|--------|-----------------------------|--|
| 1 | n-Nonane (C9) | 111-84-2 | SHBP9752 | 99% | 201.3 µg/mL | +/- 5.2012 |
| 2 | n-Decane (C10) | 124-18-5 | SHBQ1342 | 99% | 201.7 µg/mL | +/- 5.2098 |
| 3 | n-Dodecane (C12) | 112-40-3 | SHBP7054 | 99% | 201.3 µg/mL | +/- 5.2012 |
| 4 | n-Tetradecane (C14) | 629-59-4 | STBL0465 | 99% | 200.7 µg/mL | +/- 5.1839 |
| 5 | n-Hexadecane (C16) | 544-76-3 | SHBR0669 | 99% | 200.3 µg/mL | +/- 5.1753 |
| 6 | n-Octadecane (C18) | 593-45-3 | UE5NG | 99% | 200.7 µg/mL | +/- 5.1839 |
| 7 | n-Eicosane (C20) | 112-95-8 | MKCN8767 | 97% | 200.1 µg/mL | +/- 5.1704 |
| 8 | n-Heneicosane (C21) | 629-94-7 | MKCP1960 | 99% | 200.7 µg/mL | +/- 5.1839 |
| 9 | n-Docosane (C22) | 629-97-0 | MKCQ3882 | 99% | 200.3 µg/mL | +/- 5.1753 |
| 10 | n-Tetracosane (C24) | 646-31-1 | UH5GN | 99% | 201.3 µg/mL | +/- 5.2012 |
| 11 | n-Hexacosane (C26) | 630-01-3 | MKCQ4814 | 99% | 201.0 µg/mL | +/- 5.1926 |
| 12 | n-Octacosane (C28) | 630-02-4 | BCCJ4566 | 99% | 200.3 µg/mL | +/- 5.1753 |
| 13 | n-Triacontane (C30) | 638-68-6 | MKCV7007 | 98% | 201.2 µg/mL | +/- 5.1984 |
| 14 | n-Dotriacontane (C32) | 544-85-4 | BCBW0661 | 99% | 201.7 µg/mL | +/- 5.2098 |
| 15 | n-Tetratriacontane (C34) | 14167-59-0 | 6JNHB | 99% | 201.3 µg/mL | +/- 5.2012 |
| 16 | n-Hexatriacontane (C36) | 630-06-8 | Z27H018 | 99% | 201.7 µg/mL | +/- 5.2098 |
| 17 | n-Octatriacontane (C38) | 7194-85-6 | 0000207852 | 96% | 201.6 µg/mL | +/- 5.2081 |

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: n-Pentane
CAS # 109-66-0
Purity 99%

Quality Confirmation Test

Column:

30m x 0.25mm x 0.25µm
Rtx-5 (cat.#10223)

Carrier Gas:

hydrogen-constant pressure 10 psi.

Temp. Program:

40°C (hold 2 min.) to 330°C
@ 10°C/min. (hold 10 min.)

Inj. Temp:

250°C

Det. Temp:

330°C

Det. Type:


FID

Split Vent:

2 ml/min.

Inj. Vol

1µl

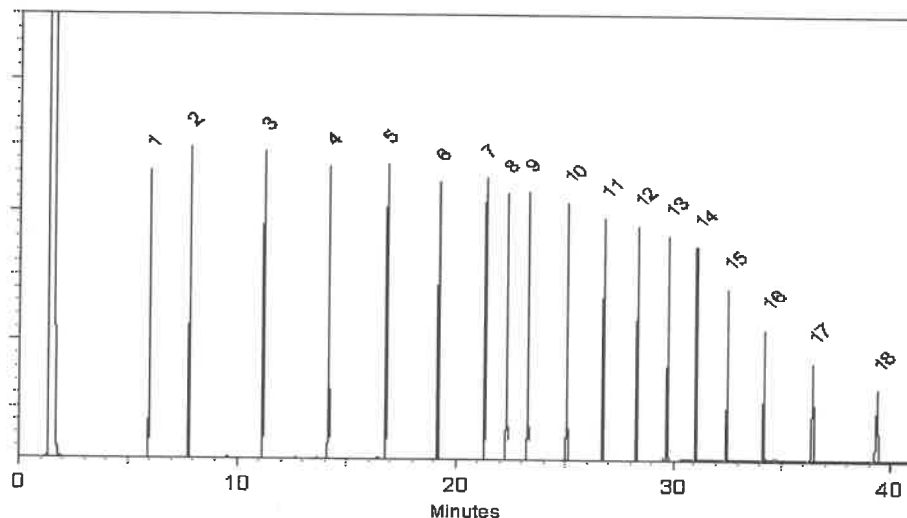

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Brandon Reish
Brandon Reish - Operations Technician III

Date Mixed: 23-Dec-2024

Balance Serial # C322230531

Dylan Murphy
Dylan Murphy - Operations Technician I

Date Passed: 27-Dec-2024

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 31480 **Lot No.:** A0224278

Description : MA Fractionation Surrogate Spike Mix
MA Fractionation Surrogate Spike Mix 4000µg/mL, Hexane, 1mL/ampul

Container Size : 2 mL **Pkg Amt:** > 1 mL

Expiration Date : March 31, 2031 **Storage:** 10°C or colder

Handling: Sonication required. Mix is photosensitive. **Ship:** Ambient

P14043 } AC
↓
P14058 } 6/10/25

CERTIFIED VALUES

| Elution Order | Compound | CAS # | Lot # | Purity | Grav. Conc. (weight/volume) | Expanded Uncertainty * (95% C.L.; K=2) |
|---------------|--------------------|----------|-----------|--------|-----------------------------|--|
| 1 | 2-Fluorobiphenyl | 321-60-8 | 00021384 | 99% | 4,018.5 µg/mL | +/- 181.0240 |
| 2 | 2-Bromonaphthalene | 580-13-2 | STBC5362V | 99% | 4,019.5 µg/mL | +/- 181.0691 |

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Hexane
CAS # 110-54-3
Purity 99%



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 31480 **Lot No.:** A0224278

Description : MA Fractionation Surrogate Spike Mix
MA Fractionation Surrogate Spike Mix 4000µg/mL, Hexane, 1mL/ampul

Container Size : 2 mL **Pkg Amt:** > 1 mL

Expiration Date : March 31, 2031 **Storage:** 10°C or colder

Handling: Sonication required. Mix is photosensitive. **Ship:** Ambient

P14043 } AC
↓
P14058 } 6/10/25

CERTIFIED VALUES

| Elution Order | Compound | CAS # | Lot # | Purity | Grav. Conc. (weight/volume) | Expanded Uncertainty * (95% C.L.; K=2) |
|---------------|--------------------|----------|-----------|--------|-----------------------------|--|
| 1 | 2-Fluorobiphenyl | 321-60-8 | 00021384 | 99% | 4,018.5 µg/mL | +/- 181.0240 |
| 2 | 2-Bromonaphthalene | 580-13-2 | STBC5362V | 99% | 4,019.5 µg/mL | +/- 181.0691 |

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Hexane
CAS # 110-54-3
Purity 99%



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 31480 **Lot No.:** A0224278

Description : MA Fractionation Surrogate Spike Mix
MA Fractionation Surrogate Spike Mix 4000µg/mL, Hexane, 1mL/ampul

Container Size : 2 mL **Pkg Amt:** > 1 mL

Expiration Date : March 31, 2031 **Storage:** 10°C or colder

Handling: Sonication required. Mix is photosensitive. **Ship:** Ambient

P14043 } AC
↓
P14058 } 6/10/25

CERTIFIED VALUES

| Elution Order | Compound | CAS # | Lot # | Purity | Grav. Conc. (weight/volume) | Expanded Uncertainty * (95% C.L.; K=2) |
|---------------|--------------------|----------|-----------|--------|-----------------------------|--|
| 1 | 2-Fluorobiphenyl | 321-60-8 | 00021384 | 99% | 4,018.5 µg/mL | +/- 181.0240 |
| 2 | 2-Bromonaphthalene | 580-13-2 | STBC5362V | 99% | 4,019.5 µg/mL | +/- 181.0691 |

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Hexane
CAS # 110-54-3
Purity 99%



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 31480 **Lot No.:** A0224278

Description : MA Fractionation Surrogate Spike Mix
MA Fractionation Surrogate Spike Mix 4000µg/mL, Hexane, 1mL/ampul

Container Size : 2 mL **Pkg Amt:** > 1 mL

Expiration Date : March 31, 2031 **Storage:** 10°C or colder

Handling: Sonication required. Mix is photosensitive. **Ship:** Ambient

P14043 } AC
↓
P14058 } 6/10/25

CERTIFIED VALUES

| Elution Order | Compound | CAS # | Lot # | Purity | Grav. Conc. (weight/volume) | Expanded Uncertainty * (95% C.L.; K=2) |
|---------------|--------------------|----------|-----------|--------|-----------------------------|--|
| 1 | 2-Fluorobiphenyl | 321-60-8 | 00021384 | 99% | 4,018.5 µg/mL | +/- 181.0240 |
| 2 | 2-Bromonaphthalene | 580-13-2 | STBC5362V | 99% | 4,019.5 µg/mL | +/- 181.0691 |

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Hexane
CAS # 110-54-3
Purity 99%

n-Hexane 95%
ULTRA RESI-ANALYZED
For Organic Residue Analysis

avantor™



Material No.: 9262-03
Batch No.: 24G1962003
Manufactured Date: 2024-05-23
Expiration Date: 2025-08-22
Revision No.: 0

Certificate of Analysis

| Test | Specification | Result |
|---|----------------|-------------|
| FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL) | ≤ 5 | 3 |
| ECD Sensitive Impurities (as Heptachlor Epoxide) Single Peak (pg/mL) | ≤ 10 | 1 |
| ECD-Sensitive Impurities (as Ethylene Dibromide) - Single Impurity Peak (ng/mL) | ≤ 5 | 1 |
| Assay (Total Saturated C ₆ Isomers) (by GC, corrected for water) | $\geq 99.5 \%$ | 99.7 % |
| Assay (as n-Hexane) (by GC, corrected for water) | $\geq 95 \%$ | 98 % |
| Color (APHA) | ≤ 10 | 5 |
| Residue after Evaporation | ≤ 1.0 ppm | 0.1 ppm |
| Substances Darkened by H ₂ SO ₄ | Passes Test | Passes Test |
| Water (by KF, coulometric) | $\leq 0.05 \%$ | < 0.01 % |

For Laboratory, Research, or Manufacturing Use
MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: USA
Packaging Site: Phillipsburg Mfg Ctr & DC

Jamie Croak
Director Quality Operations, Bioscience Production