
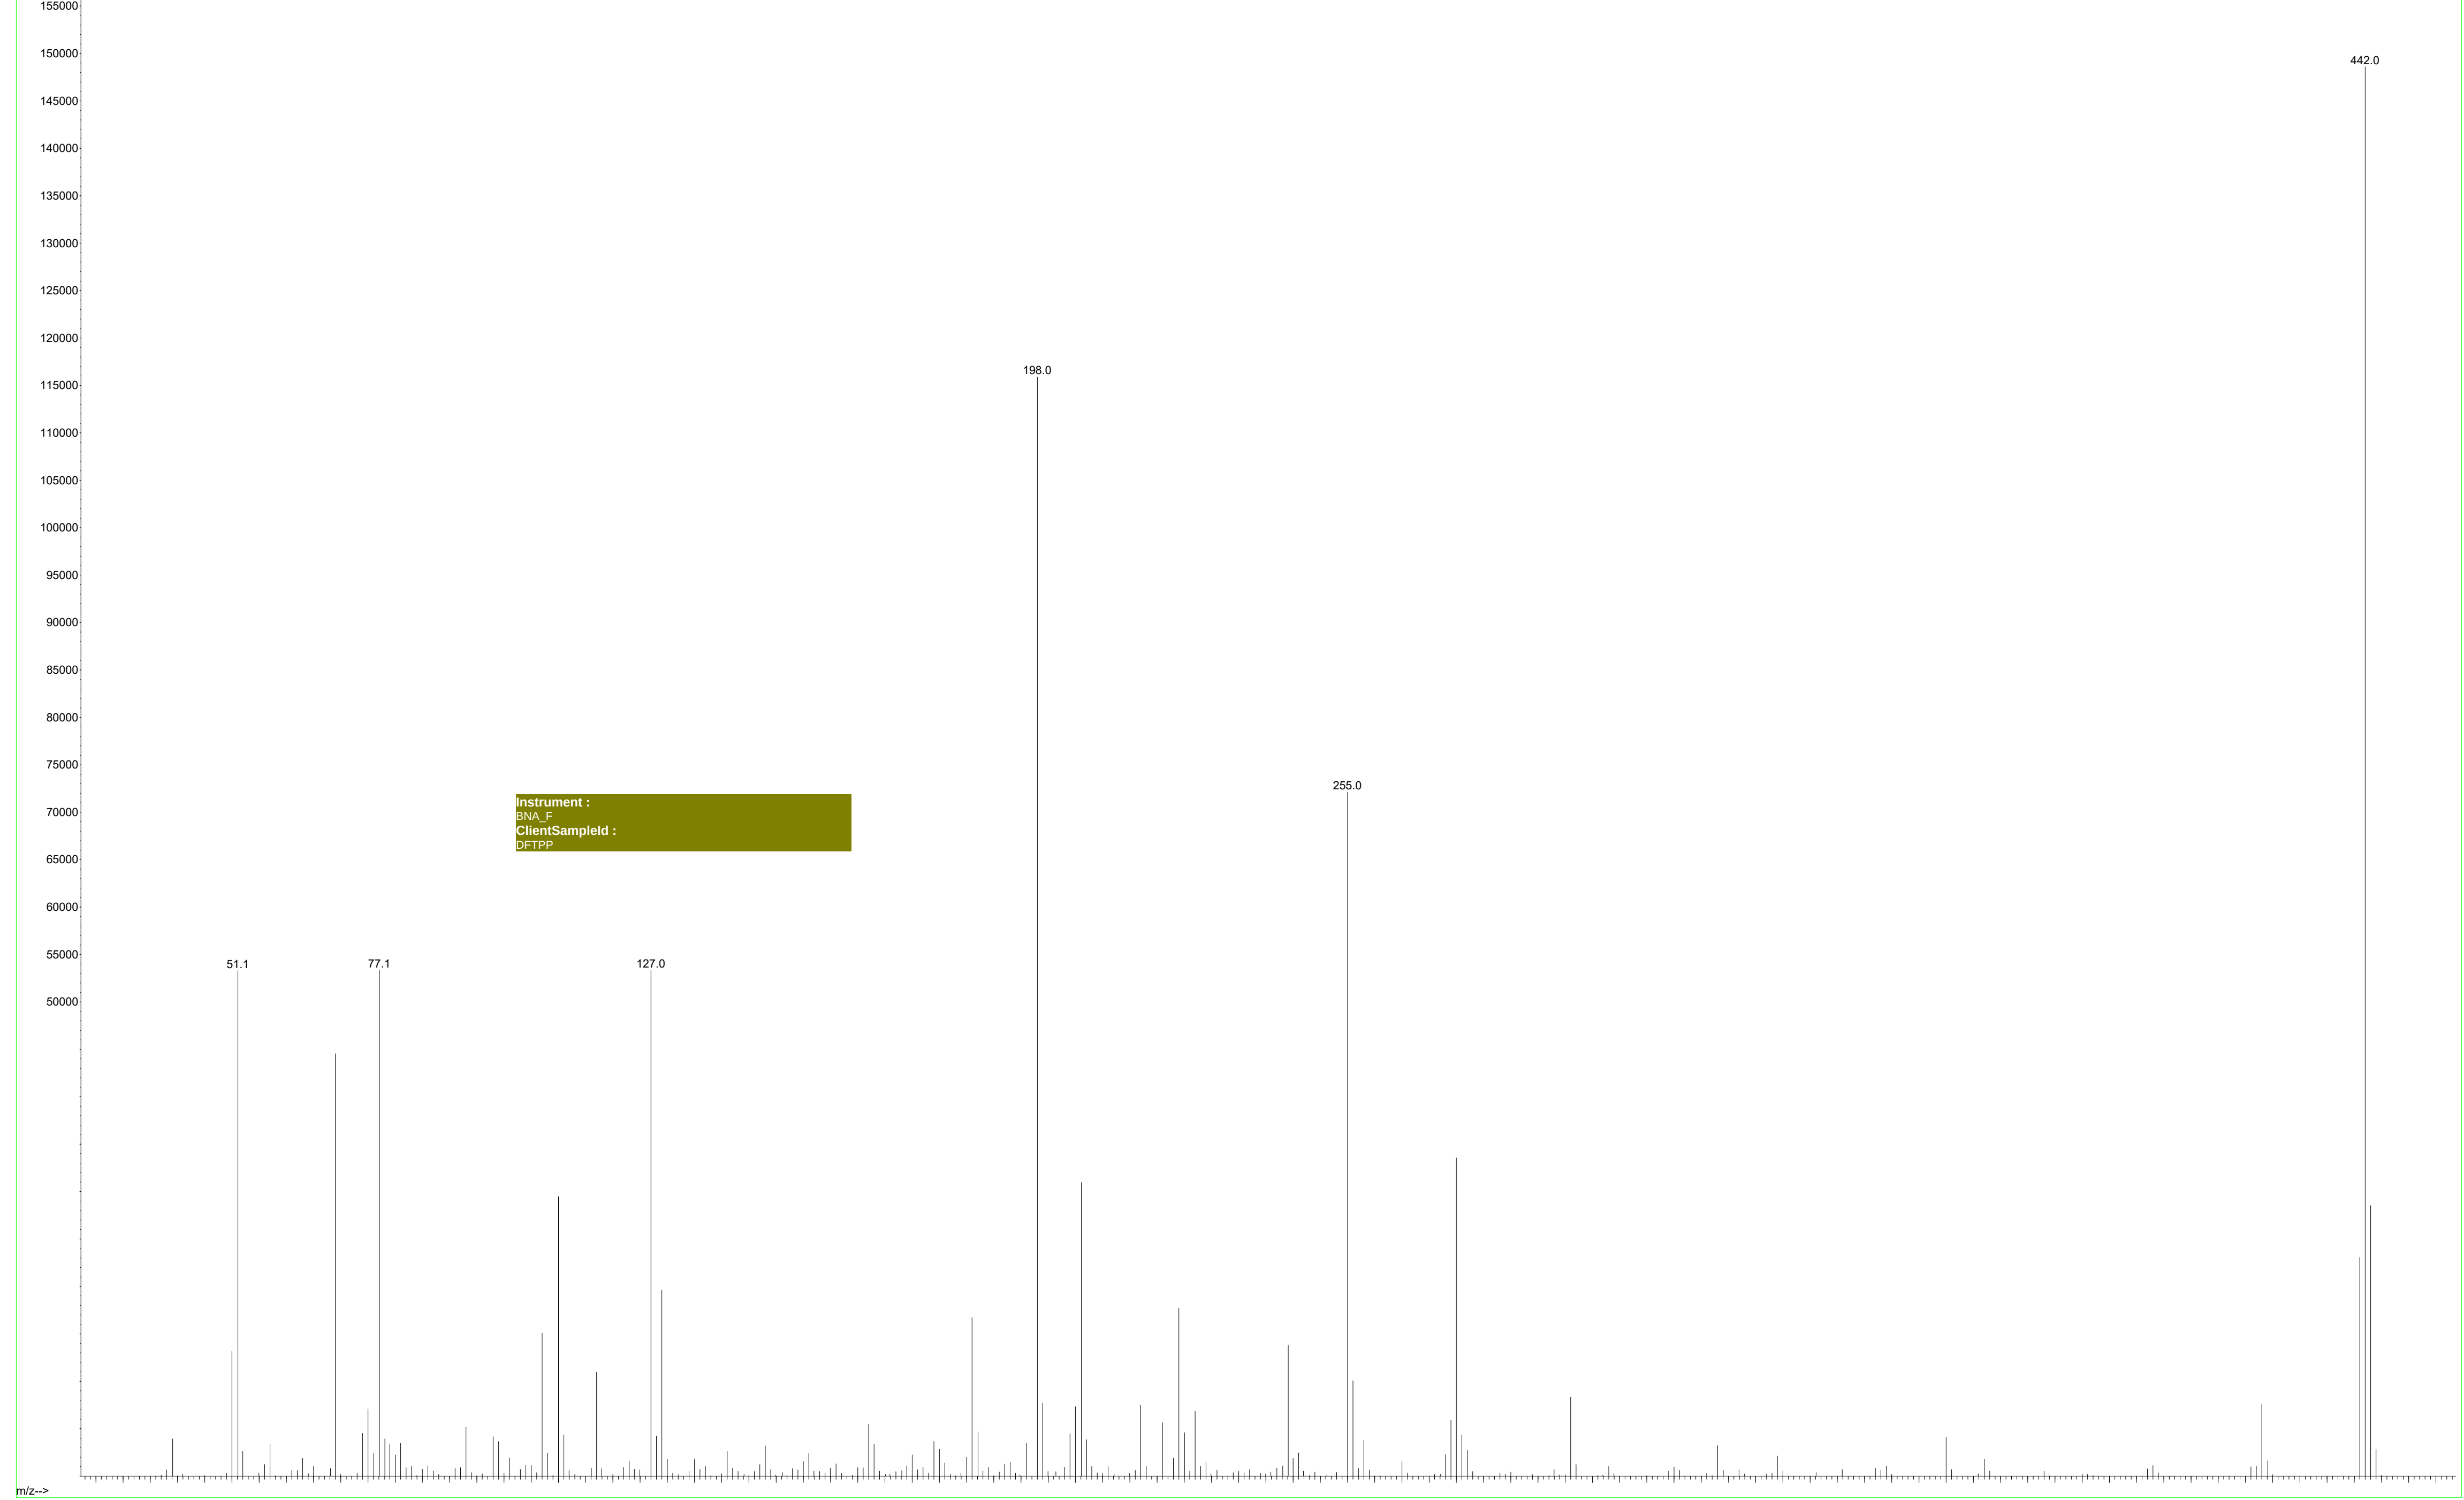


DFTPP
 Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072125\
 Data File : BF143167.D
 Acq On : 21 Jul 2025 12:27
 Operator : RC/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1
 Integration File: rteint.p
 Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF071725.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jul 17 15:14:05 2025

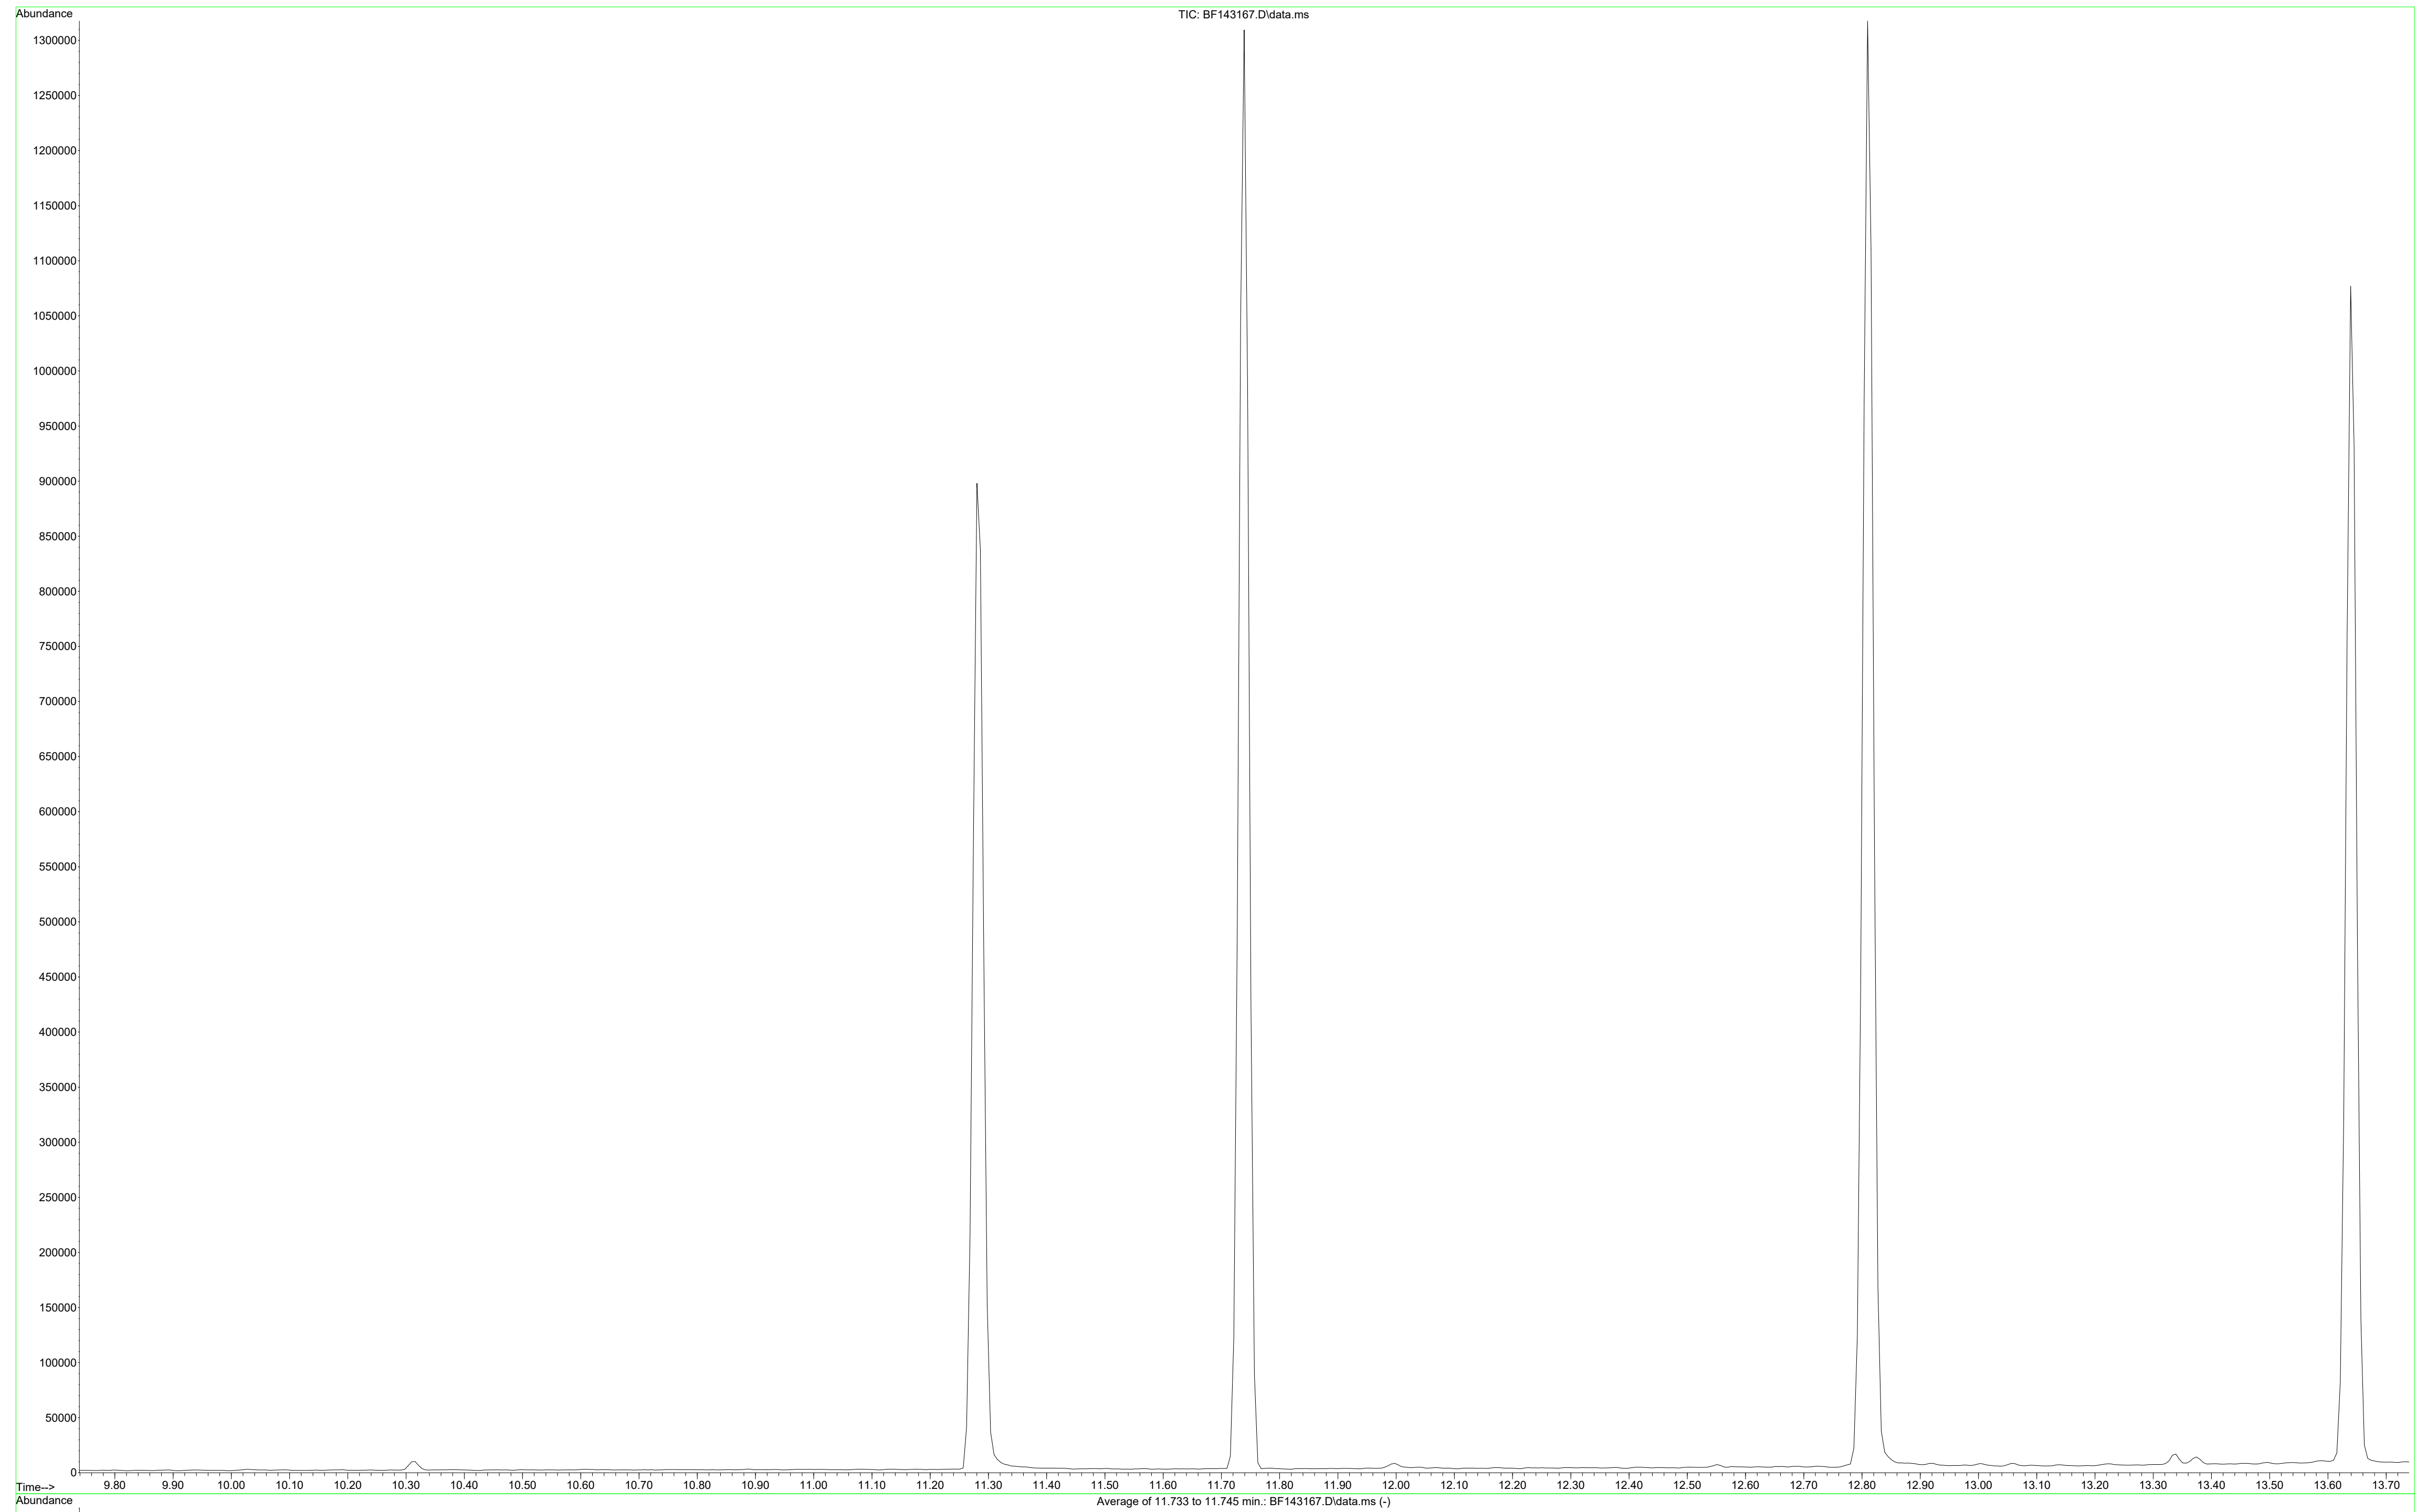

AutoFind: Scans 1622, 1623, 1624; Background Corrected with Scan 1616

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
68	69	0.00	2	1.8	806	PASS
69	69	100	100	100.0	44549	PASS
70	69	0.00	2	0.5	234	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	115907	PASS
199	198	5	9	6.6	7700	PASS
365	198	1	100	3.6	4118	PASS
441	443	0.01	150	80.8	23064	PASS
442	442	100	100	100.0	148600	PASS
443	442	15	24	19.2	28531	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
7/21/2025	BNA_F	BF143167.D
Compound Name	Response	Retention Time
DDT	249364	13.639
DDD	5341	13.339
DDE	652	13.004
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5993	255357	2.35

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072125\
Data File : BF143167.D
Acq On : 21 Jul 2025 12:27
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jul 21 13:16:27 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF071725.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 17 15:14:05 2025
Response via : Initial Calibration

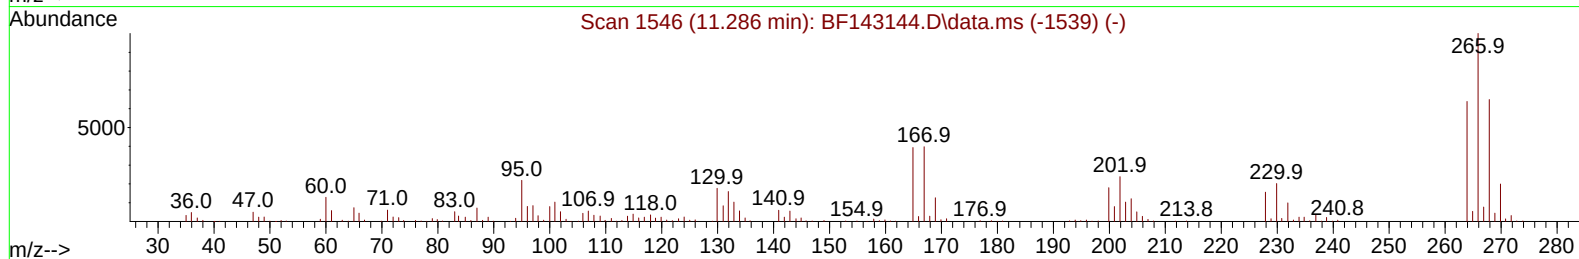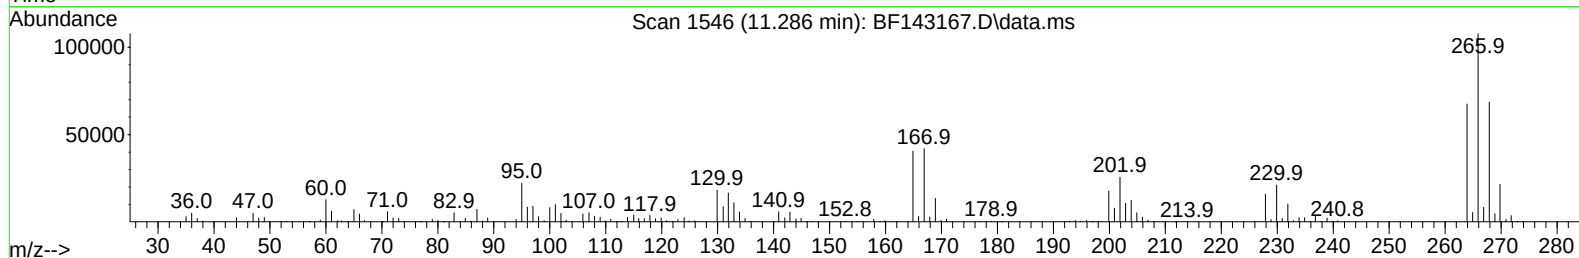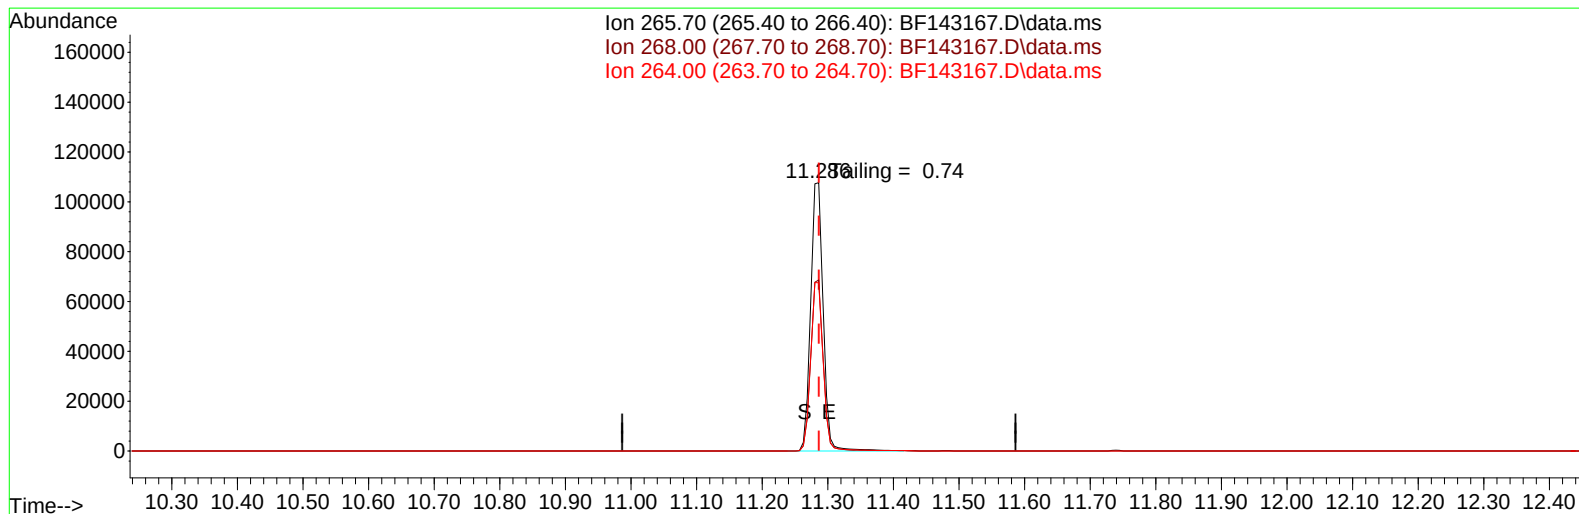

TIC: BF143167.D\data.ms

(70) Pentachlorophenol (C)

11.286min (-0.000) 25703.29 ng




response 143471

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.90	63.71
264.00	63.80	62.66
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072125\
Data File : BF143167.D
Acq On : 21 Jul 2025 12:27
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jul 21 13:16:27 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF071725.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 17 15:14:05 2025
Response via : Initial Calibration

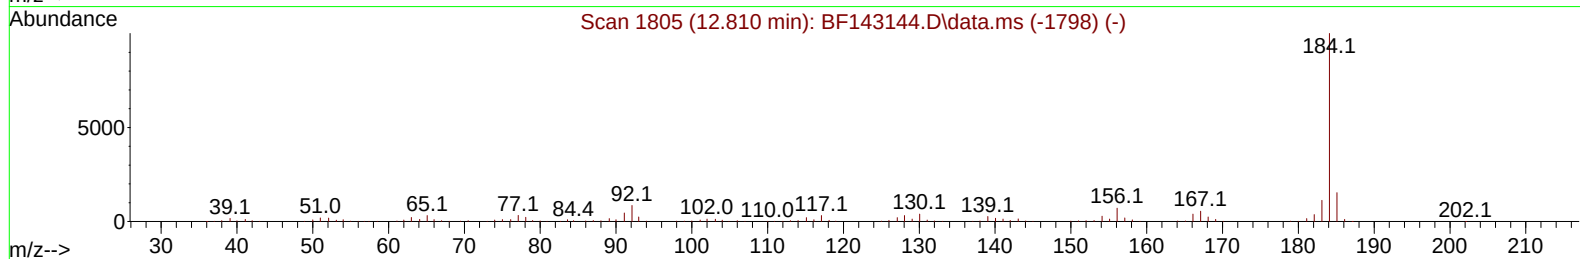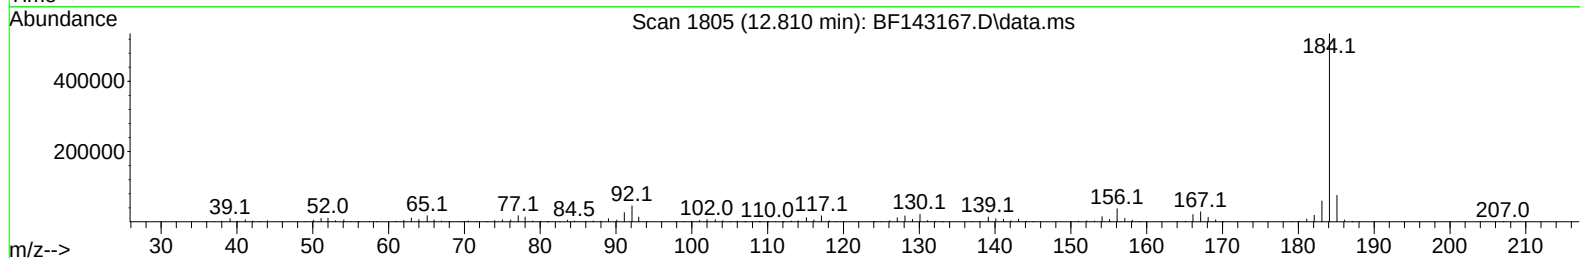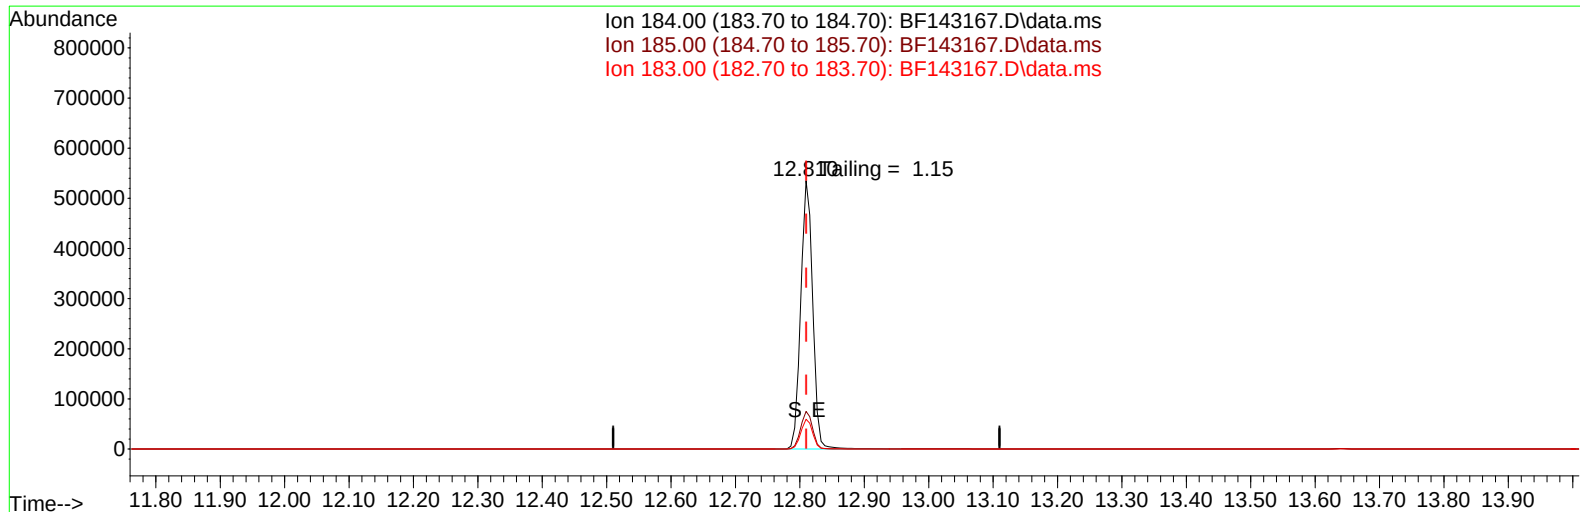

TIC: BF143167.D\data.ms

(77) Benzidine

12.810min (-0.000) 0.00 ng

response 694622

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.30	14.06
183.00	11.20	11.08
0.00	0.00	0.00