
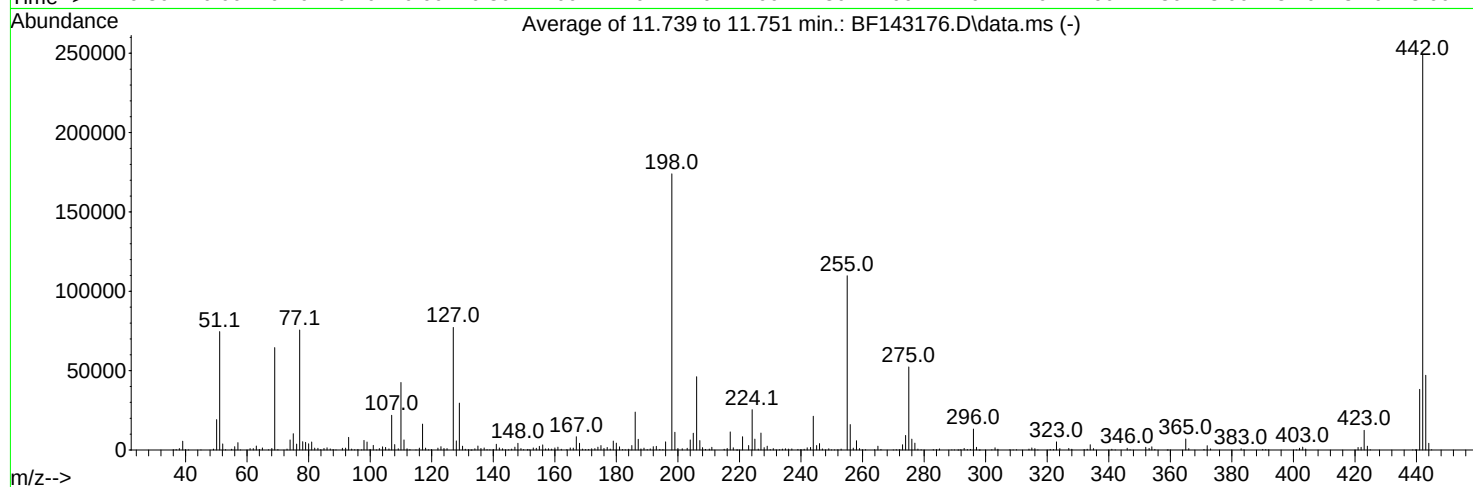


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072225\
 Data File : BF143176.D
 Acq On : 22 Jul 2025 07:48
 Operator : RC/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270E-Tune.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Mar 23 16:55:25 2022

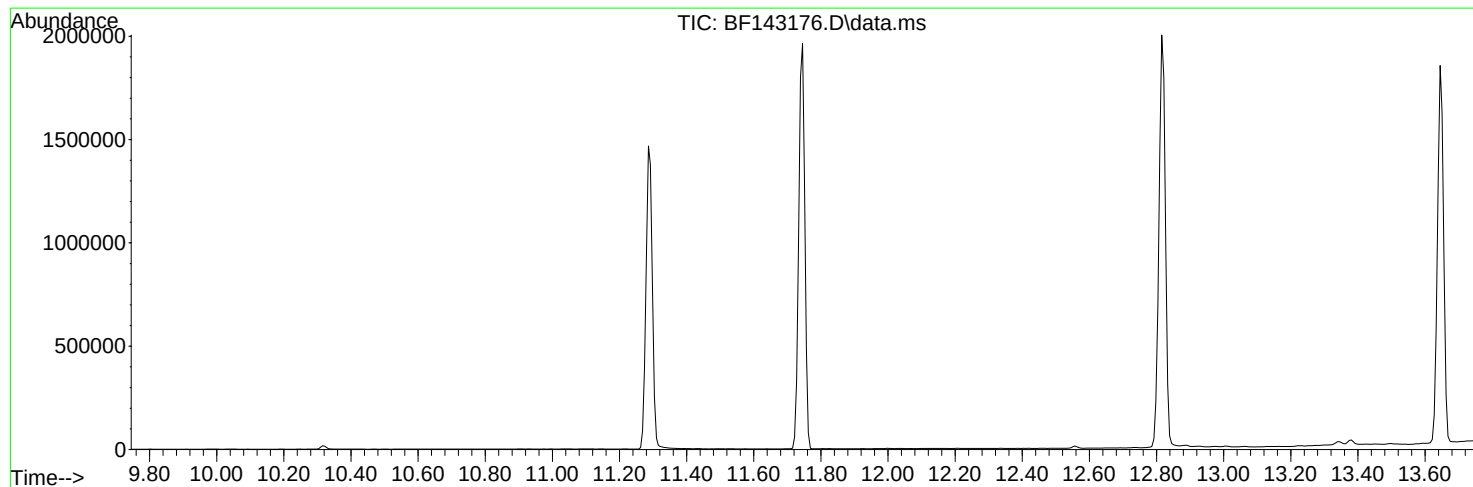




AutoFind: Scans 1623, 1624, 1625; Background Corrected with Scan 1616

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
68	69	0.00	2	1.6	1012	PASS
69	69	100	100	100.0	64563	PASS
70	69	0.00	2	0.5	329	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	174029	PASS
199	198	5	9	6.4	11198	PASS
365	198	1	100	4.0	6980	PASS
441	443	0.01	150	81.1	38184	PASS
442	442	100	100	100.0	248789	PASS
443	442	15	24	18.9	47107	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072225\
Data File : BF143176.D
Acq On : 22 Jul 2025 07:48
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jul 22 11:11:41 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF071725.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 17 15:14:05 2025
Response via : Initial Calibration

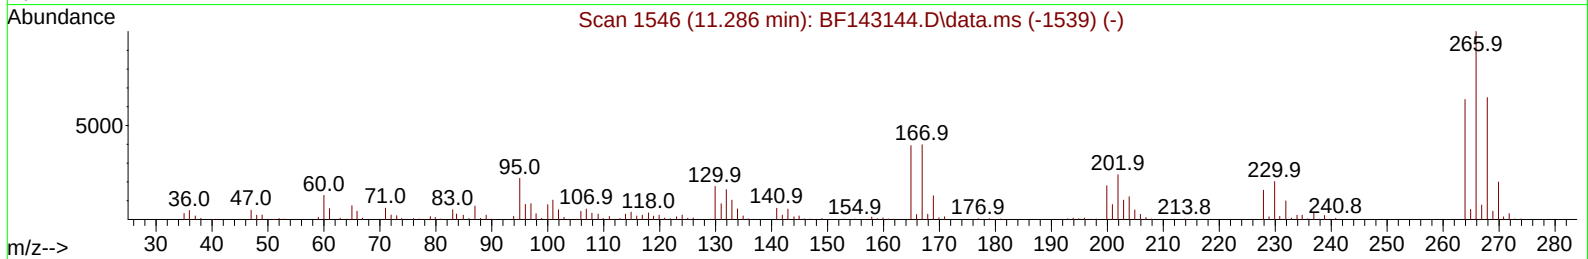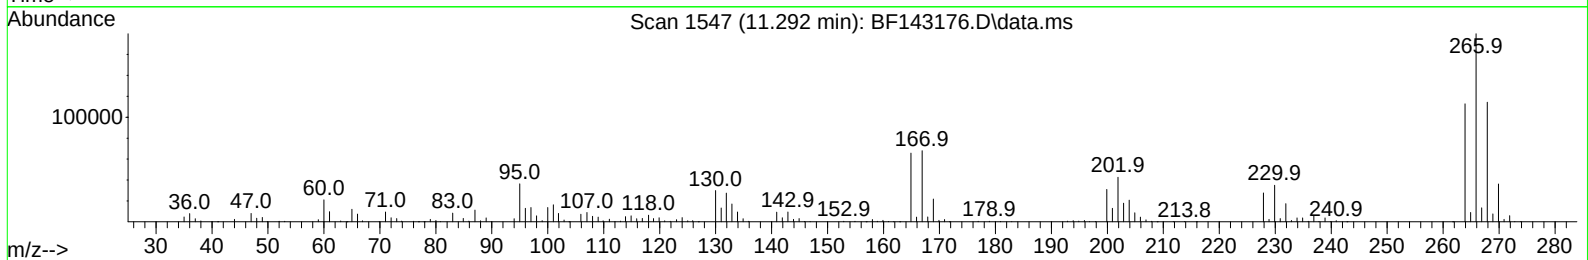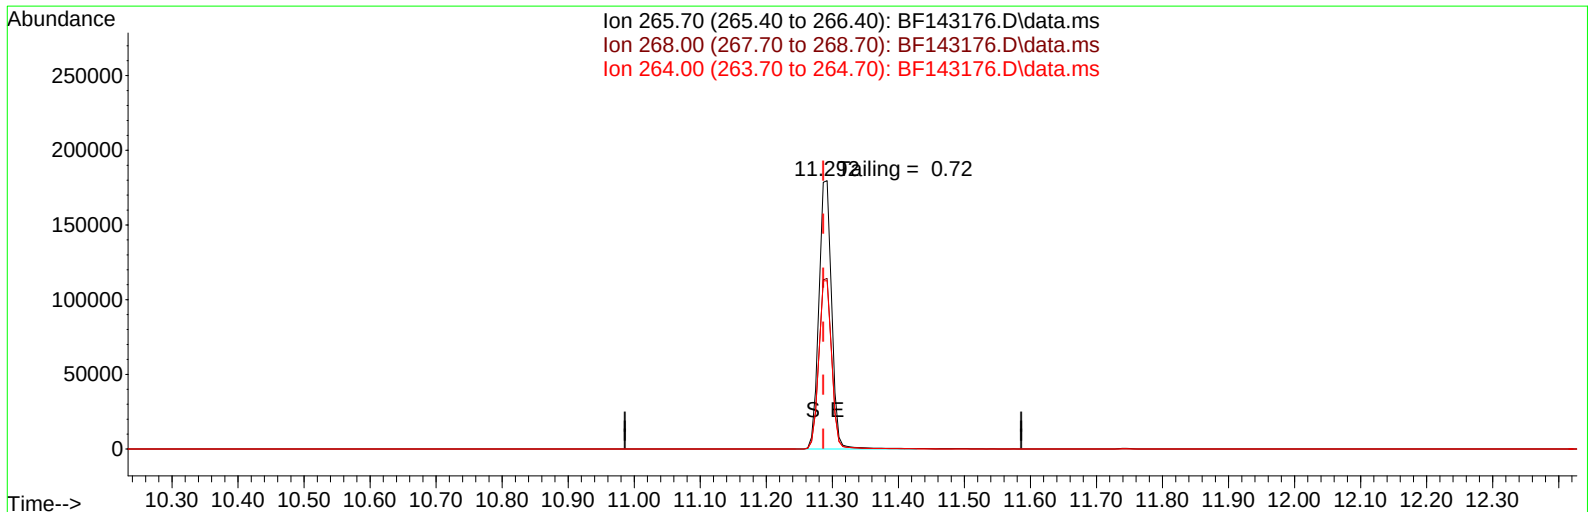

TIC: BF143176.D\data.ms

(70) Pentachlorophenol (C)

11.292min (+ 0.006) 32381.96 ng




response 241949

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.90	63.58
264.00	63.80	62.74
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072225\
Data File : BF143176.D
Acq On : 22 Jul 2025 07:48
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jul 22 11:11:41 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF071725.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 17 15:14:05 2025
Response via : Initial Calibration

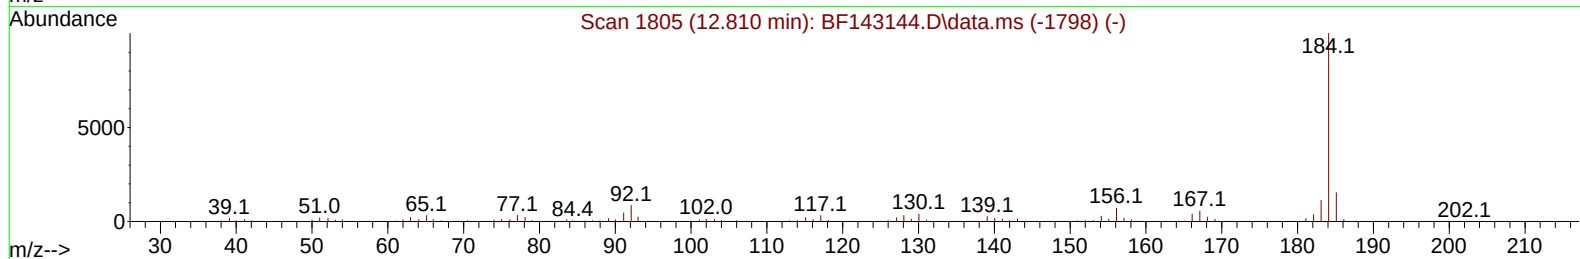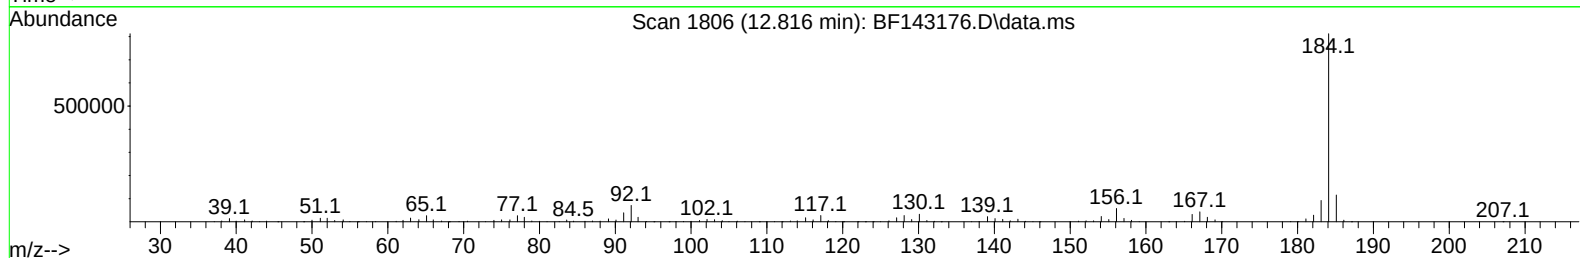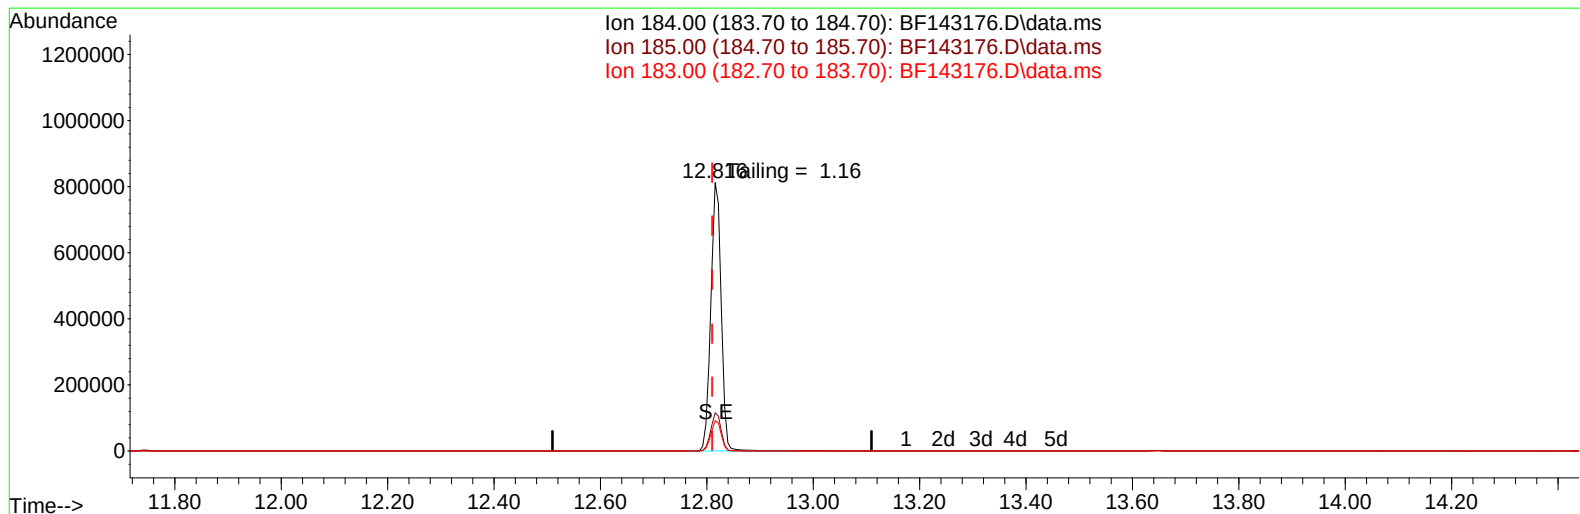

TIC: BF143176.D\data.ms

(77) Benzidine

12.816min (+ 0.006) 514868.65 ng m

response 1110844

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.30	14.24
183.00	11.20	11.33
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
7/22/2025	BNA_F	<u>BF143176.D</u>
Compound Name	Response	Retention Time
DDT	445109	13.645
DDD	8683	13.38
DDE	869	13.01
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
9552	454661	2.10

Instrument :
BNA_F
ClientSampleId :
DFTPP