

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY072225\
 Data File : VY023043.D
 Acq On : 22 Jul 2025 14:01
 Operator : SY/MD
 Sample : Q2651-01
 Misc : 5.18g/5.0mL/MSVOA_Y/SOIL/B
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 MH 2-1

Quant Time: Jul 23 02:04:12 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y071825S.M
 Quant Title : SW846 8260
 QLast Update : Sat Jul 19 01:50:49 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.713	168	283867	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.616	114	534269	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.414	117	538212	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.346	152	226724	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.061	65	163005	56.724	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	113.440%
35) Dibromofluoromethane	7.634	113	173941	51.324	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	102.640%
50) Toluene-d8	10.103	98	663191	49.346	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	=	98.700%
62) 4-Bromofluorobenzene	12.402	95	231301	54.673	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	=	109.340%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY072225\
Data File : VY023043.D
Acq On : 22 Jul 2025 14:01
Operator : SY/MD
Sample : Q2651-01
Misc : 5.18g/5.0mL/MSVOA_Y/SOIL/B
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
MH 2-1

Quant Time: Jul 23 02:04:12 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y071825S.M
Quant Title : SW846 8260
QLast Update : Sat Jul 19 01:50:49 2025
Response via : Initial Calibration




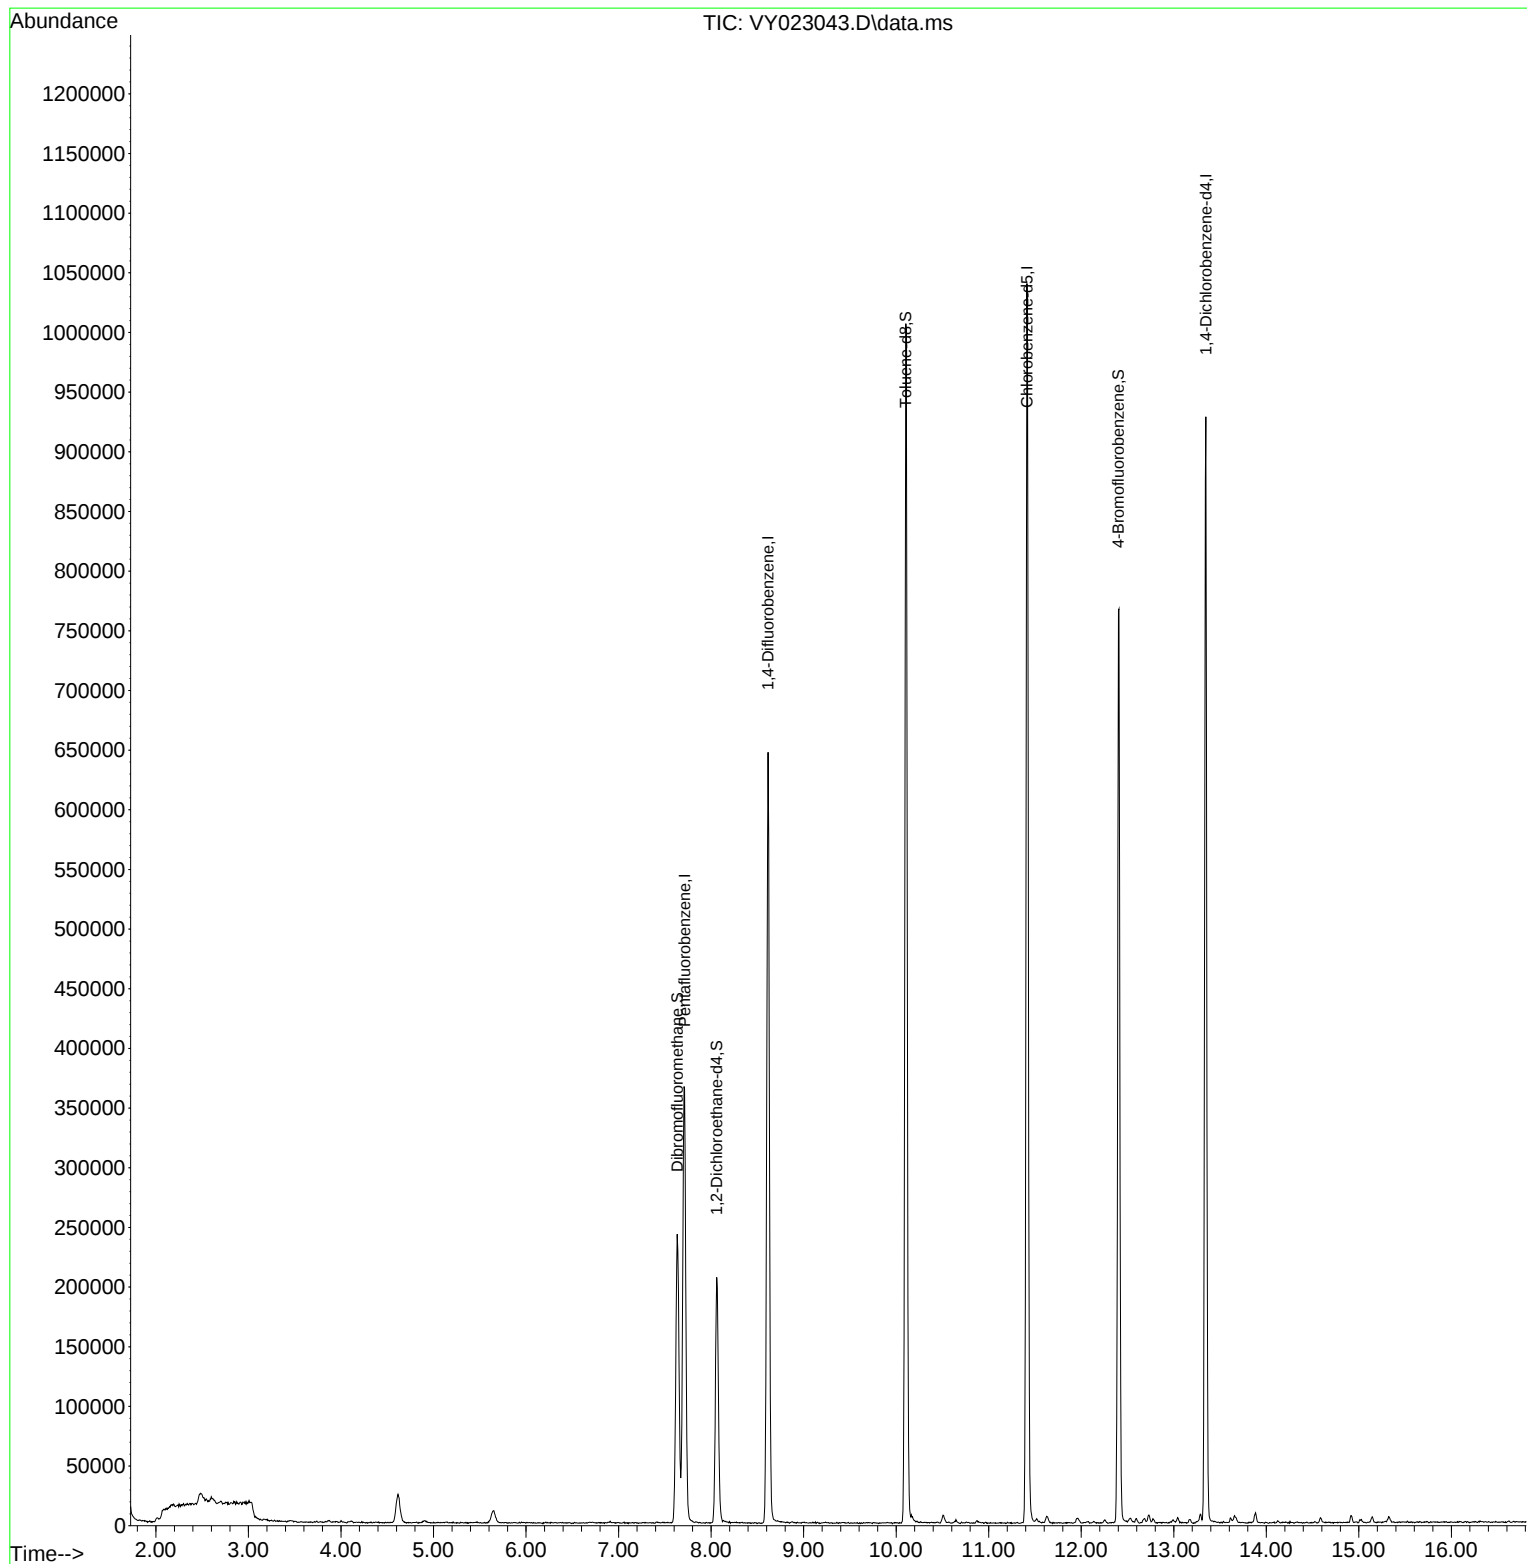


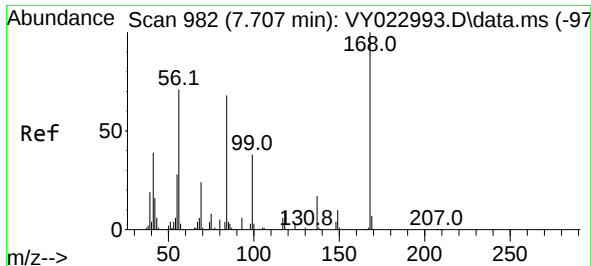

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.713 min Scan# 982
Delta R.T. 0.006 min
Lab File: VY023043.D
Acq: 22 Jul 2025 14:01




Instrument :
MSVOA_Y
ClientSampleId :
MH 2-1


Tgt Ion:168 Resp: 283867
Ion Ratio Lower Upper
168 100
99 53.5 44.4 66.6

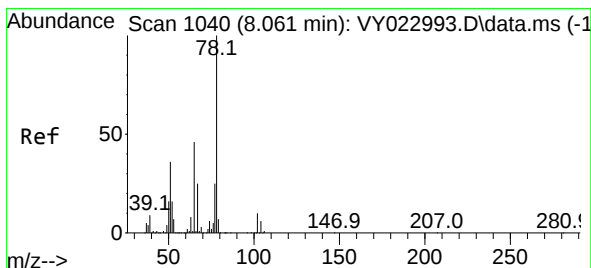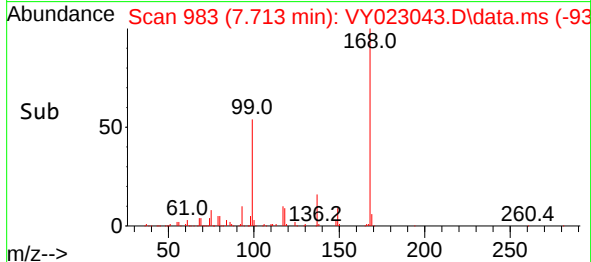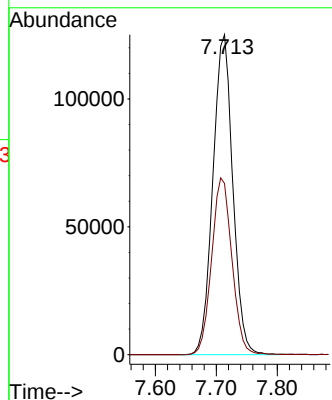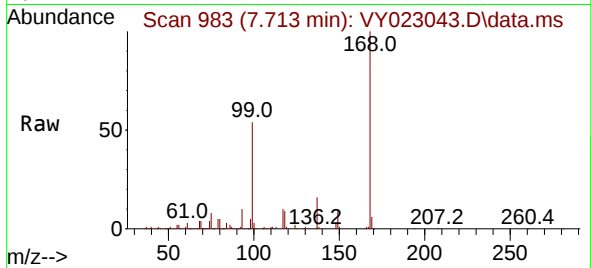

#33
1,2-Dichloroethane-d4
Concen: 56.724 ug/l
RT: 8.061 min Scan# 1040
Delta R.T. 0.000 min
Lab File: VY023043.D
Acq: 22 Jul 2025 14:01

Tgt Ion: 65 Resp: 163005
Ion Ratio Lower Upper
65 100
67 52.9 0.0 107.4


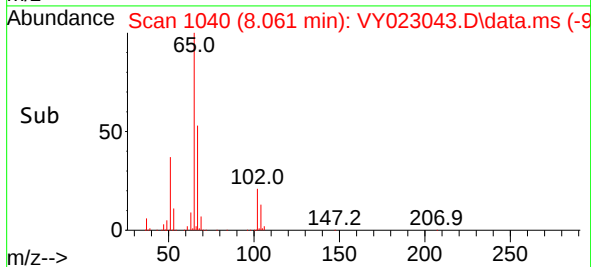
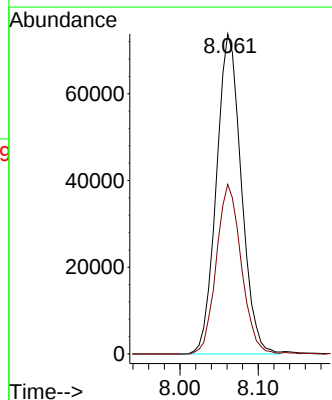
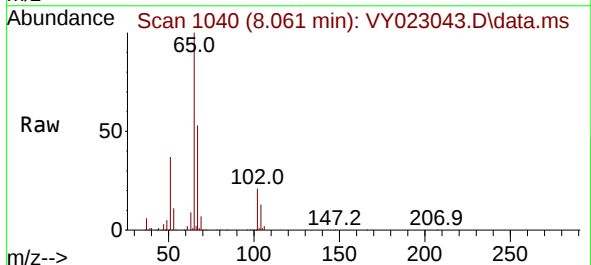


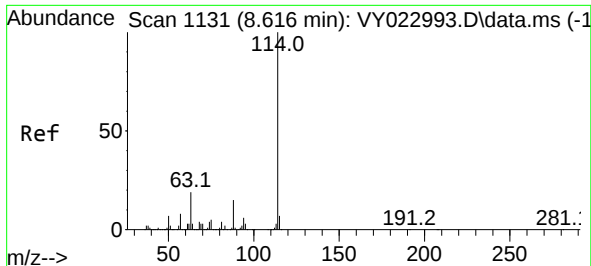

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.616 min Scan# 1131
Delta R.T. 0.000 min
Lab File: VY023043.D
Acq: 22 Jul 2025 14:01




Instrument :
MSVOA_Y
ClientSampleId :
MH 2-1


Tgt Ion:114 Resp: 534269
Ion Ratio Lower Upper
114 100
63 21.1 0.0 38.8
88 16.4 0.0 30.2

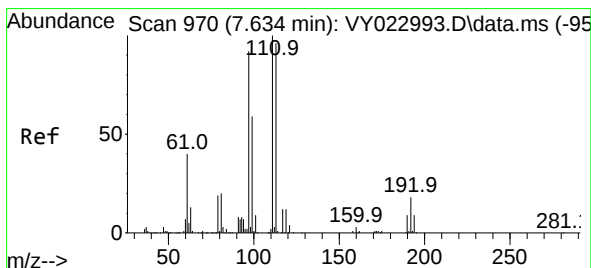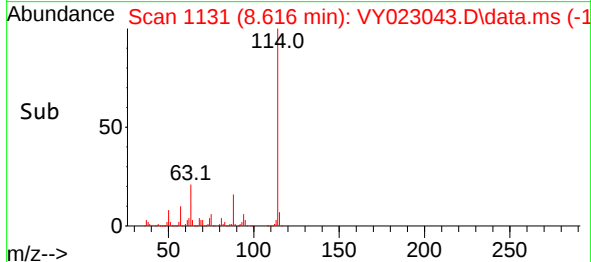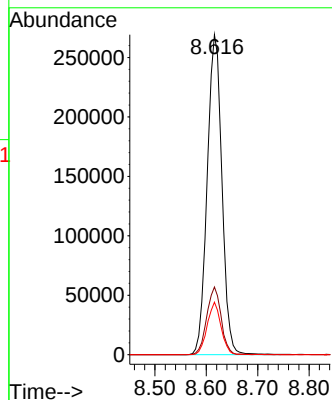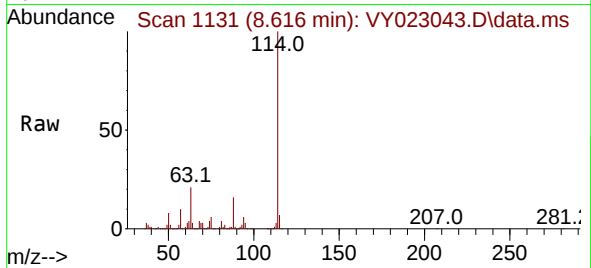

#35
Dibromofluoromethane
Concen: 51.324 ug/l
RT: 7.634 min Scan# 970
Delta R.T. 0.000 min
Lab File: VY023043.D
Acq: 22 Jul 2025 14:01

Tgt Ion:113 Resp: 173941
Ion Ratio Lower Upper
113 100
111 102.9 83.2 124.8
192 18.4 15.3 22.9


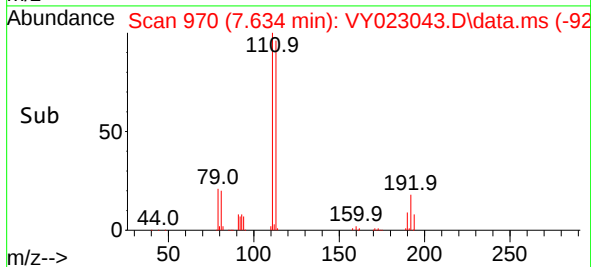
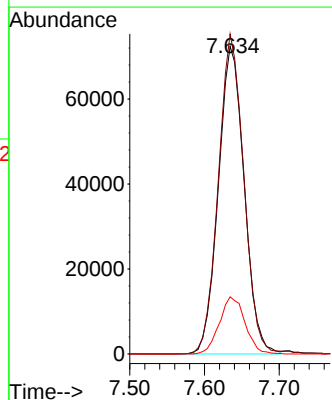
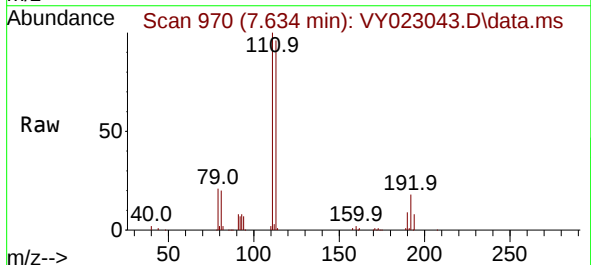


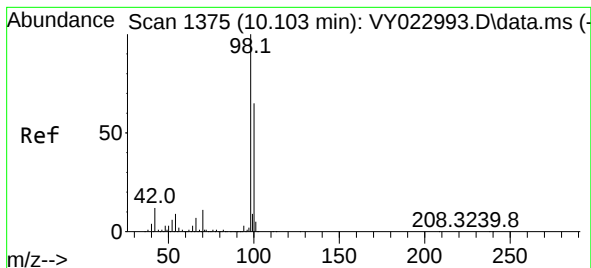

#50
Toluene-d8
Concen: 49.346 ug/l
RT: 10.103 min Scan# 1375
Delta R.T. 0.000 min
Lab File: VY023043.D
Acq: 22 Jul 2025 14:01




Instrument :
MSVOA_Y
ClientSampleId :
MH 2-1


Tgt Ion: 98 Resp: 663191
Ion Ratio Lower Upper
98 100
100 65.0 52.2 78.2

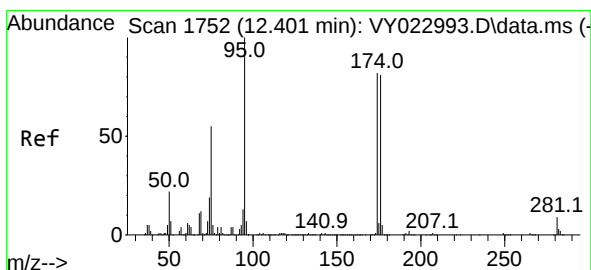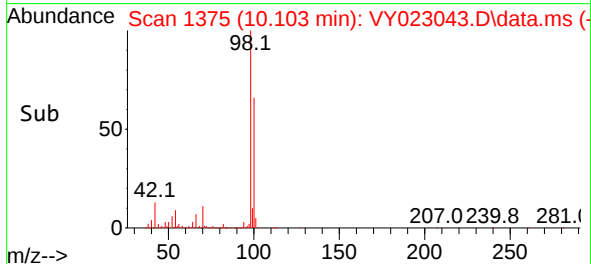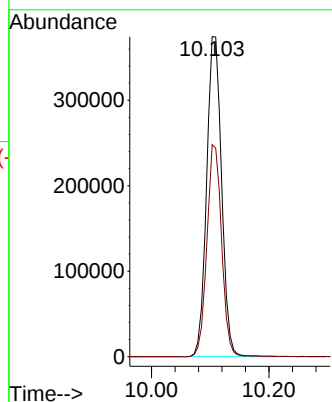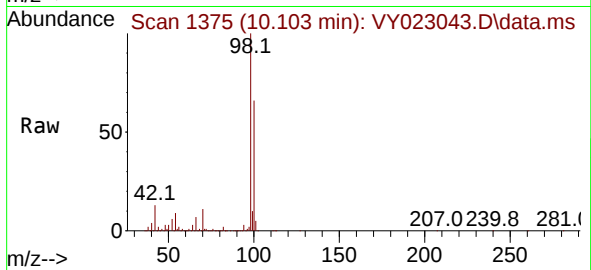

#62
4-Bromofluorobenzene
Concen: 54.673 ug/l
RT: 12.402 min Scan# 1752
Delta R.T. 0.000 min
Lab File: VY023043.D
Acq: 22 Jul 2025 14:01

Tgt Ion: 95 Resp: 231301
Ion Ratio Lower Upper
95 100
174 84.5 0.0 170.8
176 81.1 0.0 163.6


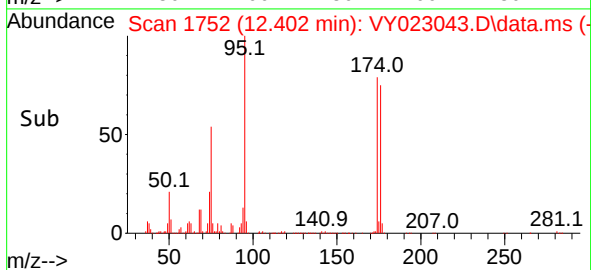
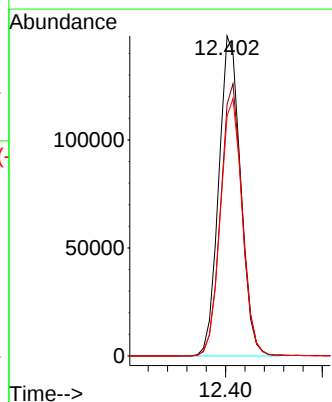
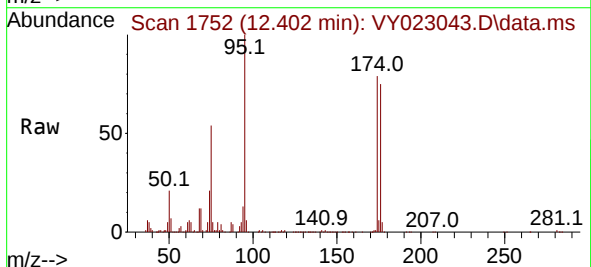


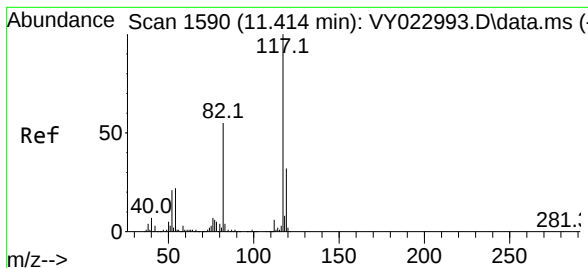

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.414 min Scan# 117
Delta R.T. 0.000 min
Lab File: VY023043.D
Acq: 22 Jul 2025 14:01

Instrument :
MSVOA_Y
ClientSampleId :
MH 2-1

Tgt Ion:117 Resp: 538212
Ion Ratio Lower Upper
117 100
82 57.6 44.3 66.5
119 32.0 25.8 38.8

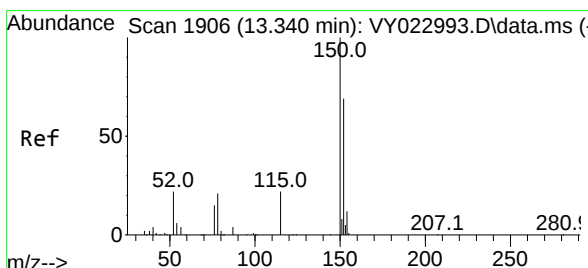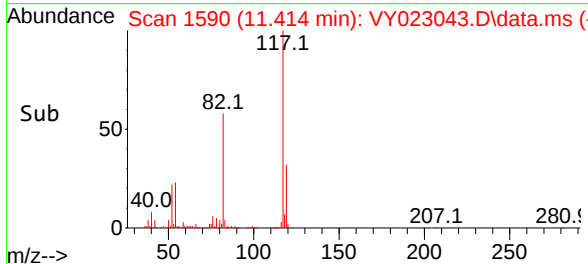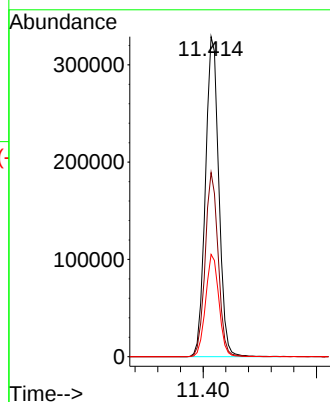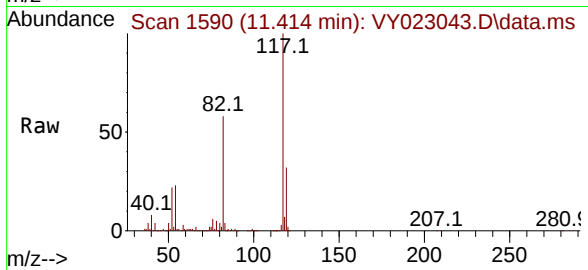

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.346 min Scan# 1907
Delta R.T. 0.006 min
Lab File: VY023043.D
Acq: 22 Jul 2025 14:01

Tgt Ion:152 Resp: 226724
Ion Ratio Lower Upper
152 100
115 58.0 29.4 88.2
150 157.1 0.0 350.0

