
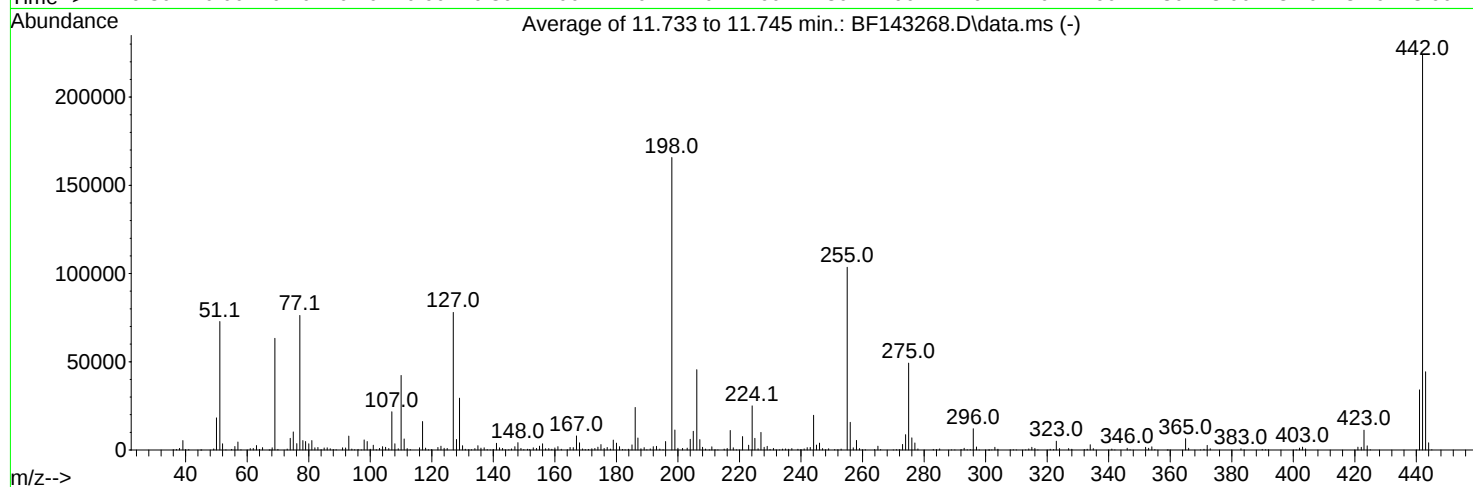


Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF073025\  
Data File : BF143268.D  
Acq On : 30 Jul 2025 14:53  
Operator : RC/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF071725.M  
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
Last Update : Thu Jul 17 15:14:05 2025

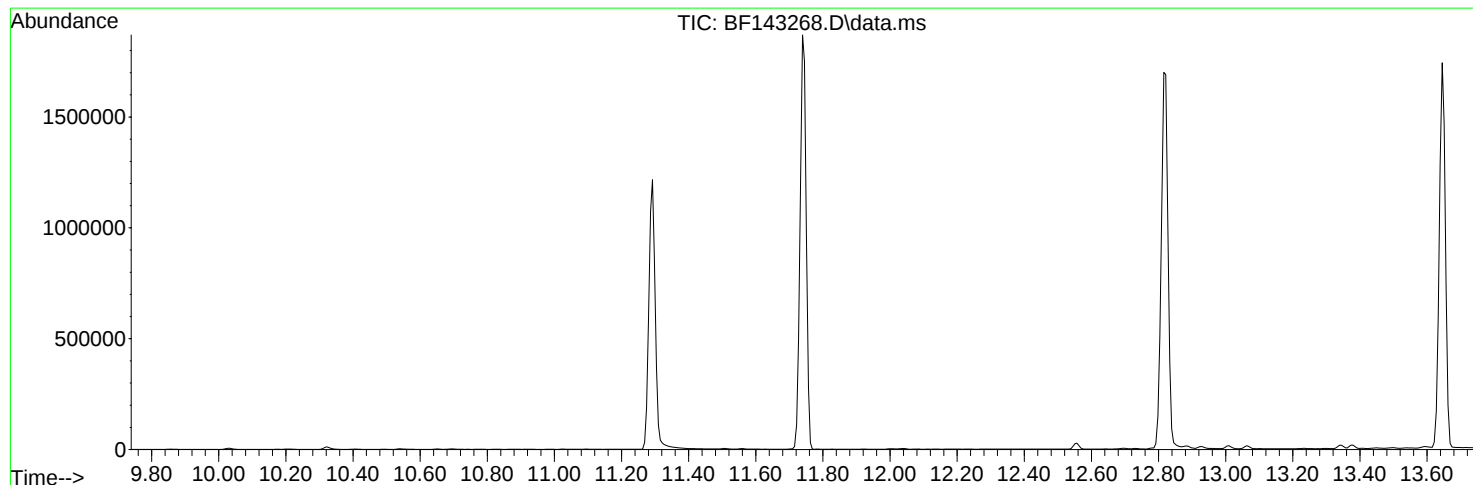




AutoFind: Scans 1622, 1623, 1624; Background Corrected with Scan 1616

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 68             | 69              | 0.00            | 2               | 2.0          | 1248       | PASS                |
| 69             | 69              | 100             | 100             | 100.0        | 63325      | PASS                |
| 70             | 69              | 0.00            | 2               | 0.6          | 350        | PASS                |
| 197            | 198             | 0.00            | 2               | 0.0          | 0          | PASS                |
| 198            | 198             | 100             | 100             | 100.0        | 165715     | PASS                |
| 199            | 198             | 5               | 9               | 6.8          | 11319      | PASS                |
| 365            | 198             | 1               | 100             | 3.9          | 6438       | PASS                |
| 441            | 443             | 0.01            | 150             | 76.8         | 34077      | PASS                |
| 442            | 442             | 100             | 100             | 100.0        | 223747     | PASS                |
| 443            | 442             | 15              | 24              | 19.8         | 44365      | PASS                |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF073025\  
Data File : BF143268.D  
Acq On : 30 Jul 2025 14:53  
Operator : RC/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP

Quant Time: Jul 30 15:27:43 2025  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF071725.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Jul 17 15:14:05 2025  
Response via : Initial Calibration

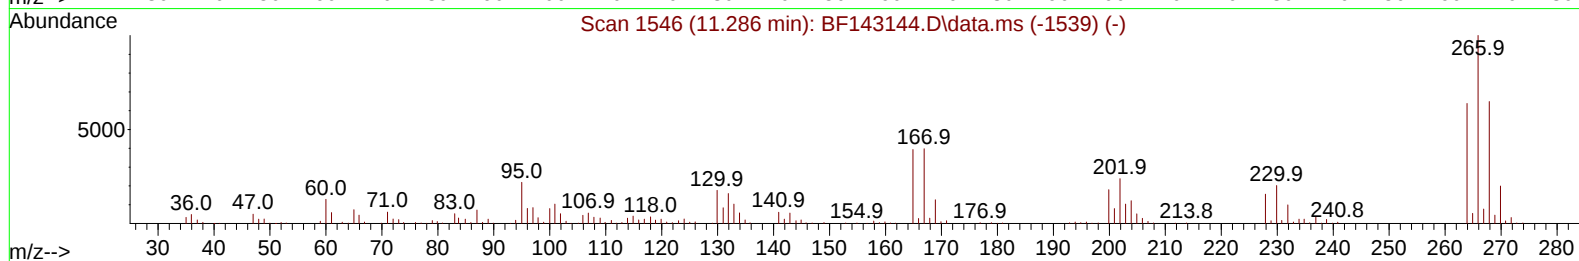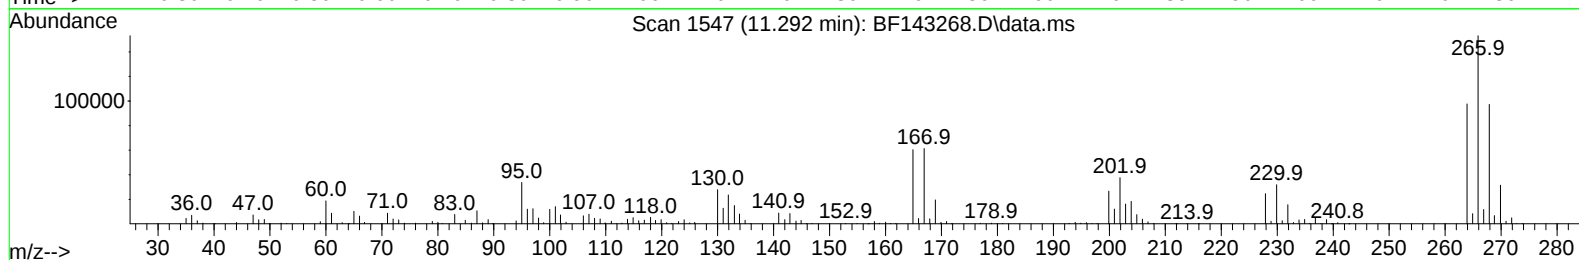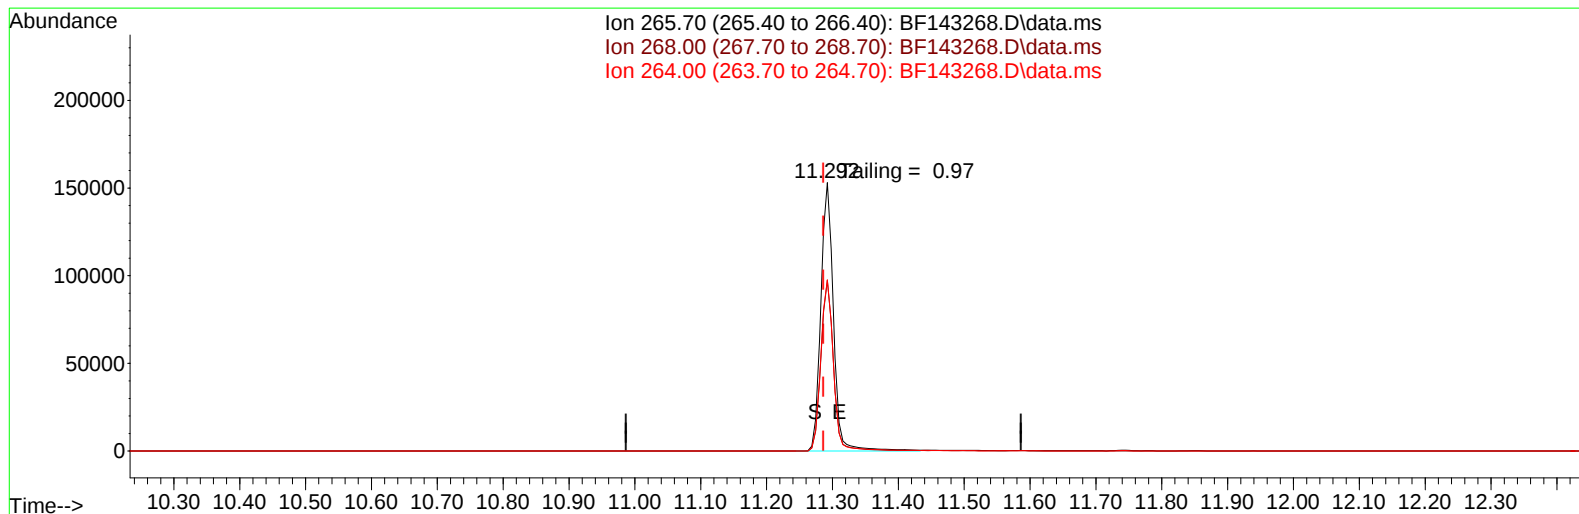

TIC: BF143268.D\data.ms

**(70) Pentachlorophenol (C)**

**11.292min (+ 0.006) 27370.33 ng**




**response 204704**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 64.90  | 63.57  |
| 264.00 | 63.80  | 63.80  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF073025\  
Data File : BF143268.D  
Acq On : 30 Jul 2025 14:53  
Operator : RC/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP

Quant Time: Jul 30 15:27:43 2025  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF071725.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Jul 17 15:14:05 2025  
Response via : Initial Calibration

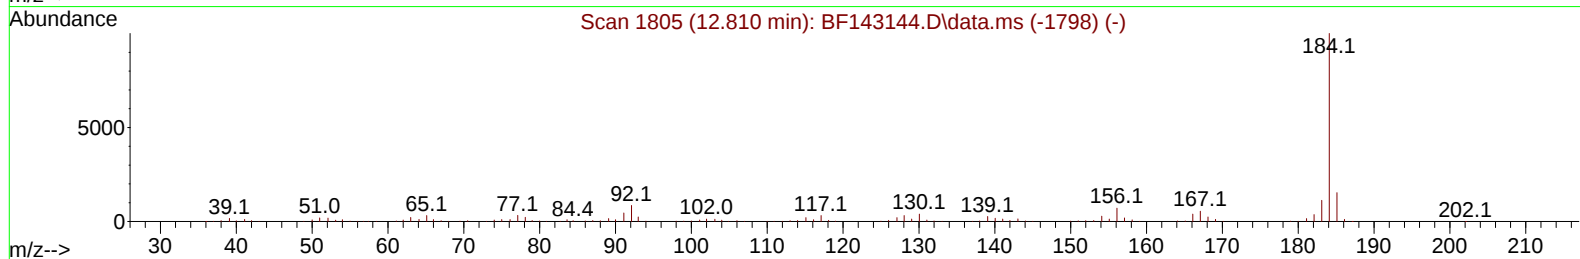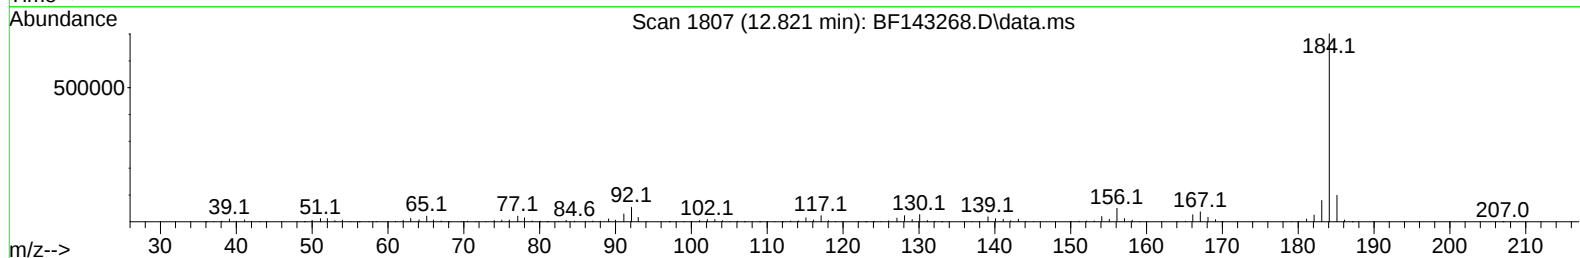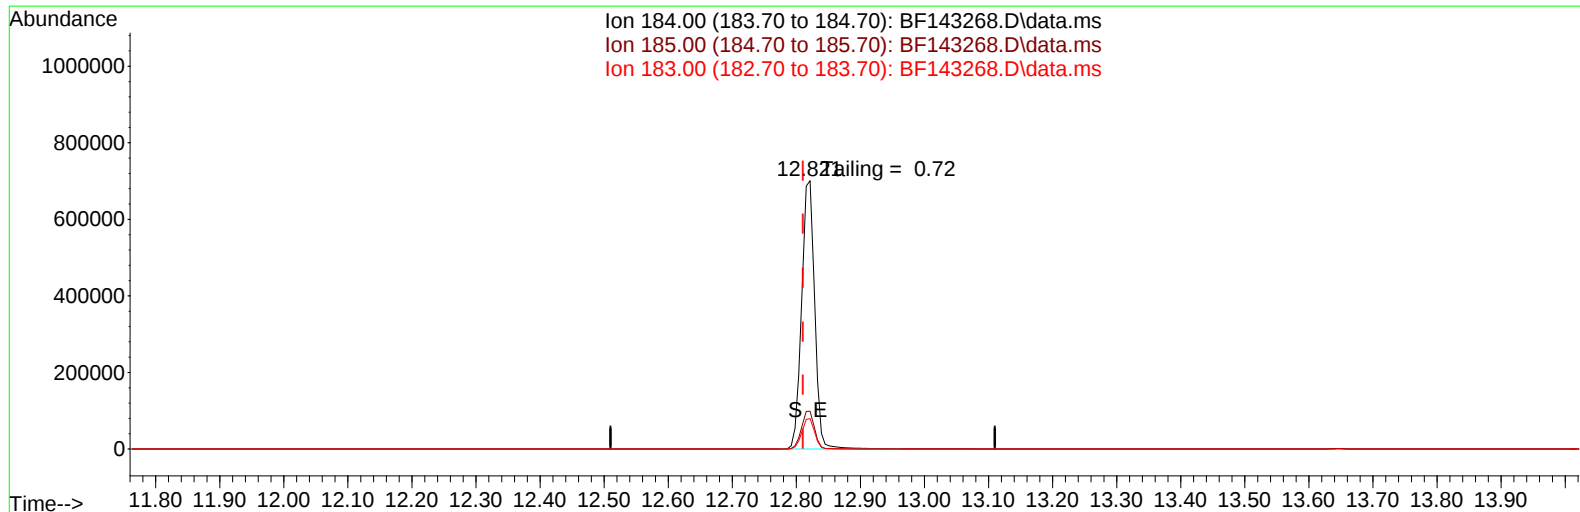

TIC: BF143268.D\data.ms

(77) Benzidine

12.821min (+ 0.011) 0.00 ng

response 999340

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 15.30  | 14.07  |
| 183.00 | 11.20  | 11.34  |
| 0.00   | 0.00   | 0.00   |

# DDT Breakdown

| Date          | Instrument Name  | DFTPP Data File    |
|---------------|------------------|--------------------|
| 7/30/2025     | BNA_F            | <u>BF143268.D</u>  |
|               |                  |                    |
|               |                  |                    |
| Compound Name | Response         | Retention Time     |
|               |                  |                    |
| DDT           | 437079           | 13.645             |
| DDD           | 9446             | 13.345             |
| DDE           | 3560             | 13.01              |
|               |                  |                    |
|               |                  |                    |
| SUM(DDD+DDE)  | SUM(DDT+DDD+DDE) | % Breakdown Of DDT |
|               |                  |                    |
| 13006         | 450085           | 2.89               |
|               |                  |                    |

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP