


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072325\
Data File : BM050487.D
Acq On : 23 Jul 2025 12:35
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM070925.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Jul 17 16:20:15 2025

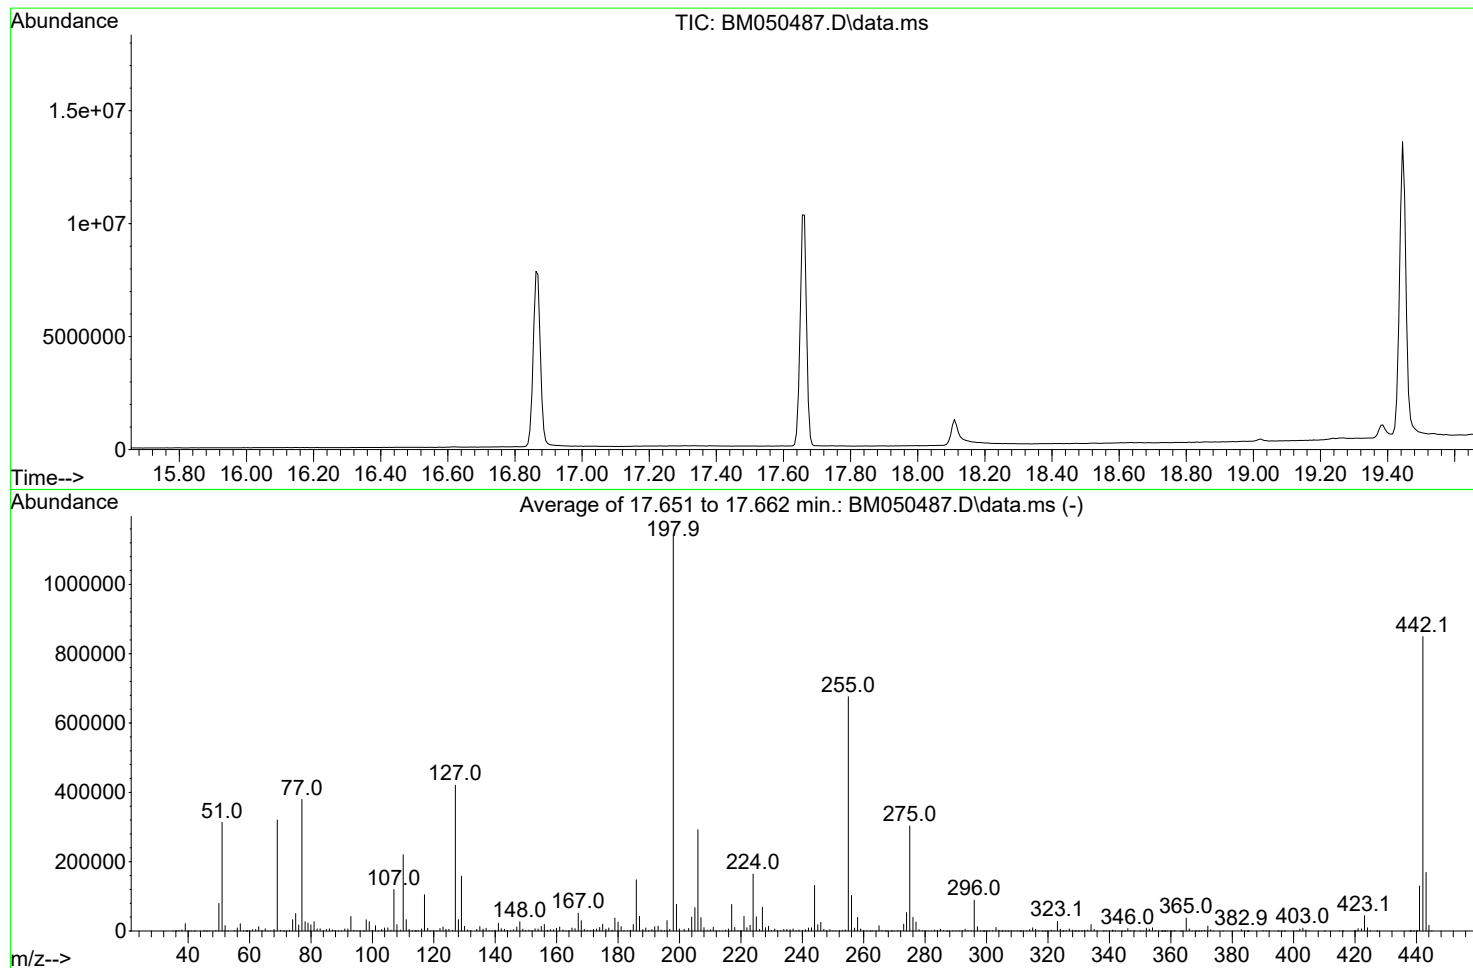

AutoFind: Scans 2493, 2494, 2495; Background Corrected with Scan 2485

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	1.5	4738	PASS
69	69	100	100	100.0	320226	PASS
70	69	0.00	2	0.6	1841	PASS
197	198	0.00	2	0.4	4668	PASS
198	198	100	100	100.0	1139221	PASS
199	198	5	9	6.8	77010	PASS
365	198	1	100	3.3	37427	PASS
441	443	0.01	150	76.9	129965	PASS
442	442	100	100	100.0	849365	PASS
443	442	15	24	19.9	168944	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
7/23/2025	BNA_M	<u>BM050487.D</u>
Compound Name	Response	Retention Time
DDT	4070715	20.68
DDD	75522	20.245
DDE	8099	19.739
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
83621	4154336	2.01

Instrument :
BNA_M
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072325\
Data File : BM050487.D
Acq On : 23 Jul 2025 12:35
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Jul 23 14:45:33 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM070925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 17 16:20:15 2025
Response via : Initial Calibration

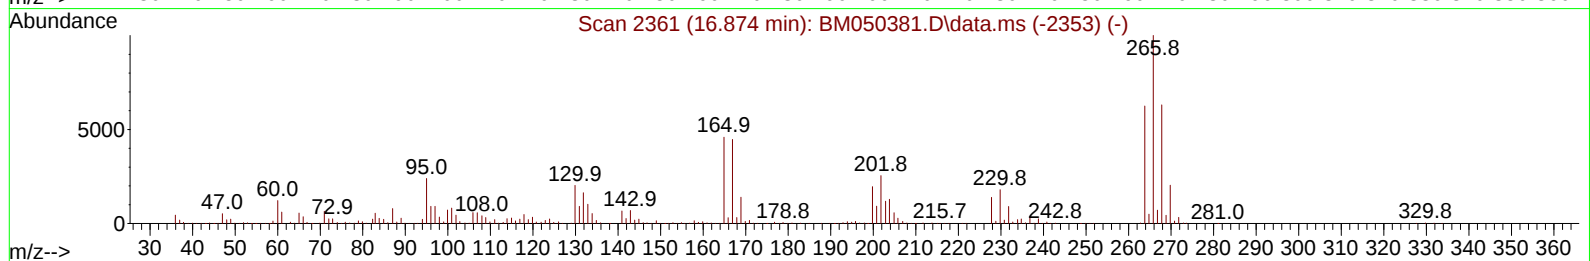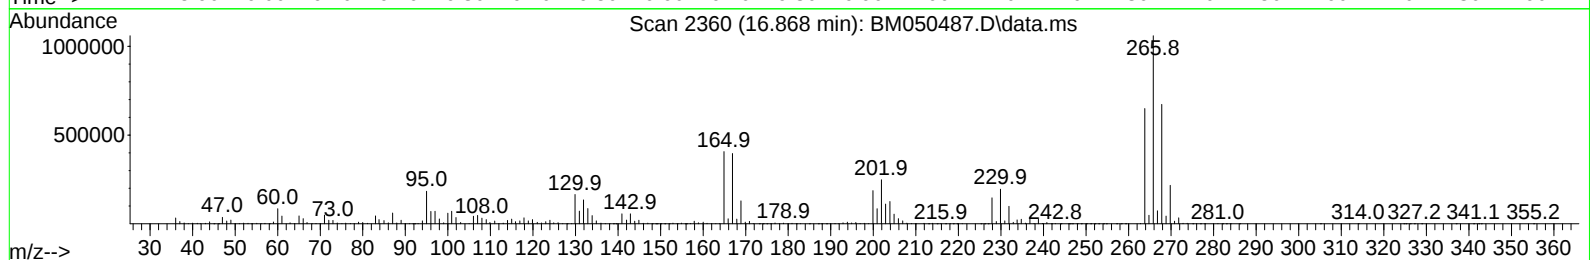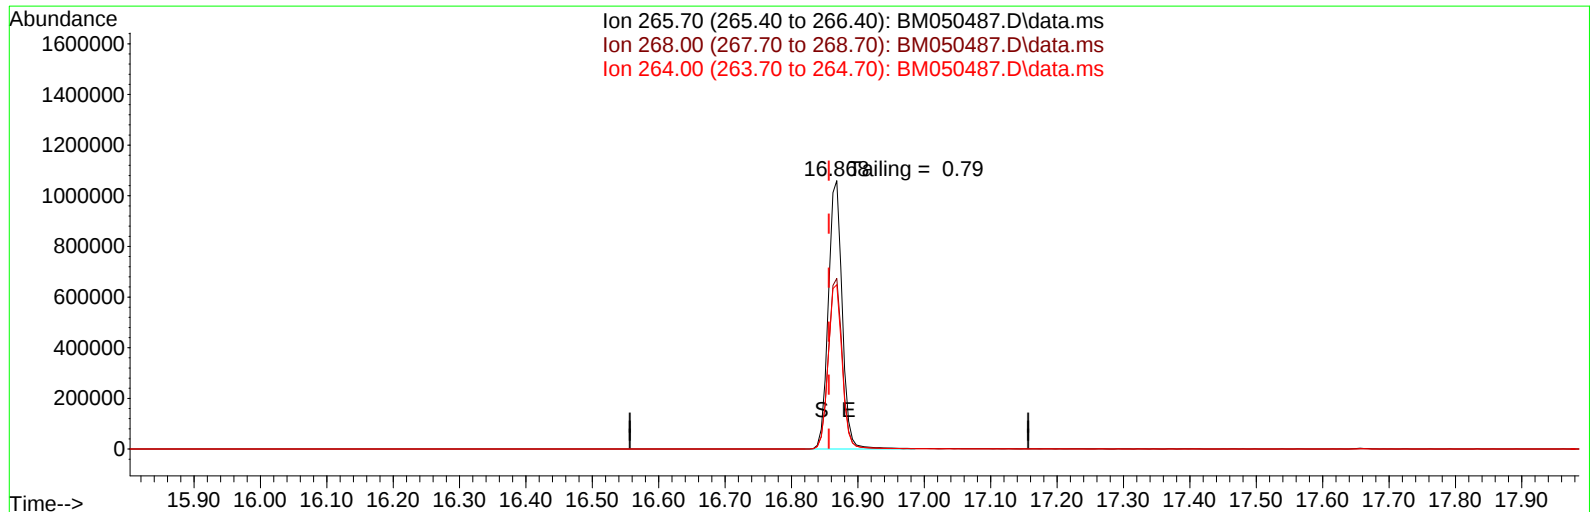

TIC: BM050487.D\data.ms

(70) Pentachlorophenol (C)

16.868min (+ 0.012) 319491.94 ng




response 1542491

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	63.54
264.00	62.40	61.26
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072325\
Data File : BM050487.D
Acq On : 23 Jul 2025 12:35
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Jul 23 14:45:33 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM070925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 17 16:20:15 2025
Response via : Initial Calibration

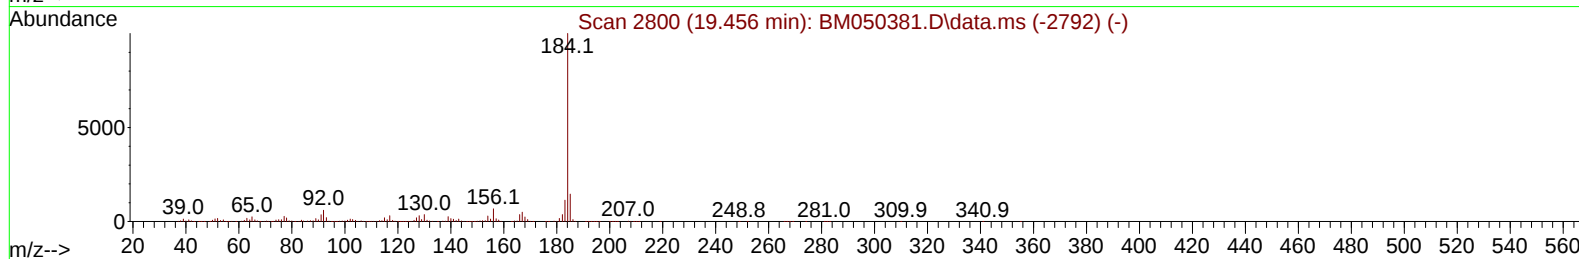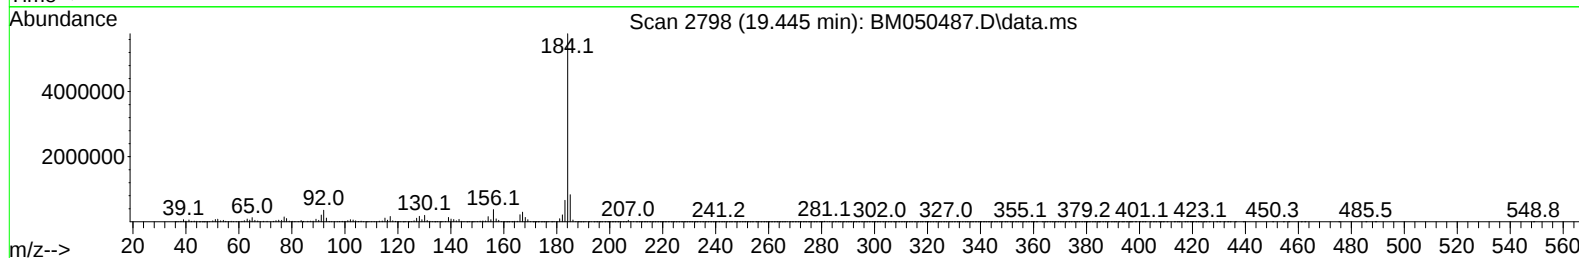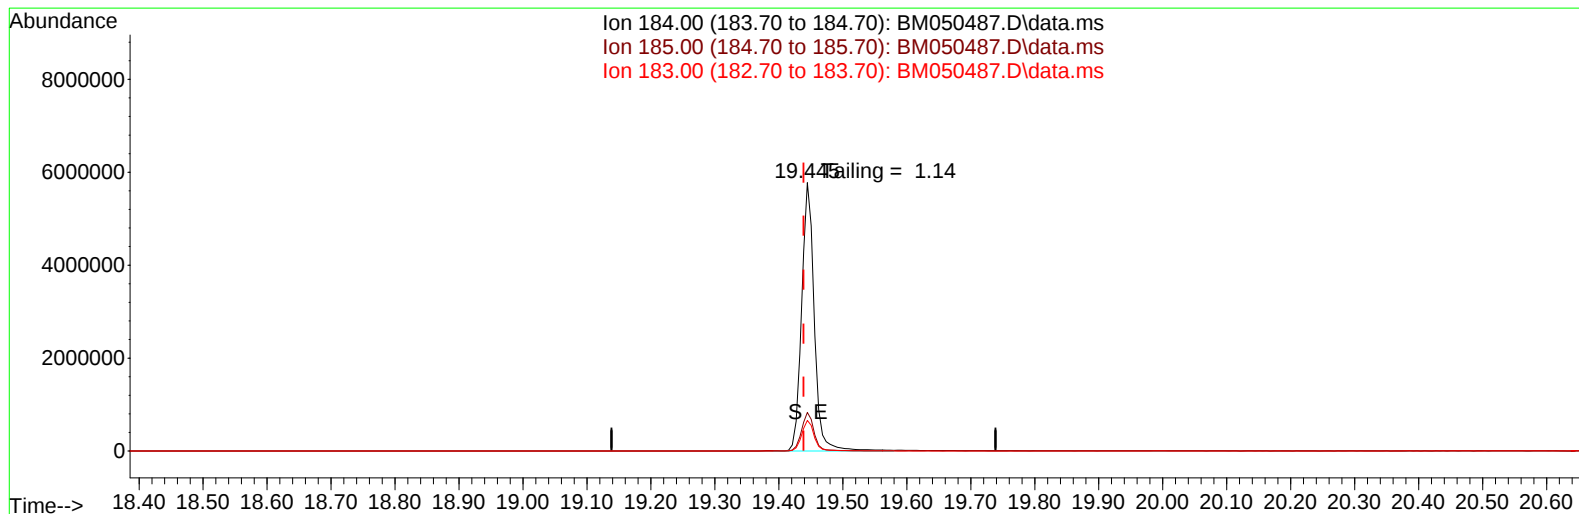

TIC: BM050487.D\data.ms

(77) Benzidine

19.445min (+ 0.006) 2965.50 ng

response 7990741

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.37
183.00	11.30	11.39
0.00	0.00	0.00